



US010674928B2

(12) **United States Patent**
Anderson et al.

(10) **Patent No.:** **US 10,674,928 B2**
(45) **Date of Patent:** **Jun. 9, 2020**

(54) **LEADLESS PACING SYSTEM INCLUDING SENSING EXTENSION**

(71) Applicant: **Medtronic, Inc.**, Minneapolis, MN (US)

(72) Inventors: **Thomas A Anderson**, New Hope, MN (US); **Todd J Sheldon**, North Oaks, MN (US); **Matthew D Bonner**, Plymouth, MN (US); **Noelle C Neafus**, Minneapolis, MN (US)

(73) Assignee: **Medtronic, Inc.**, Minneapolis, MN (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 908 days.

(21) Appl. No.: **14/694,910**

(22) Filed: **Apr. 23, 2015**

(65) **Prior Publication Data**

US 2016/0015322 A1 Jan. 21, 2016

Related U.S. Application Data

(60) Provisional application No. 62/025,690, filed on Jul. 17, 2014.

(51) **Int. Cl.**

A61N 1/362 (2006.01)
A61B 5/042 (2006.01)
A61B 5/00 (2006.01)
A61N 1/368 (2006.01)
A61N 1/372 (2006.01)
A61N 1/375 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 5/0422** (2013.01); **A61B 5/0452** (2013.01); **A61B 5/686** (2013.01); **A61N 1/362** (2013.01); **A61N 1/368** (2013.01); **A61N 1/3756** (2013.01); **A61N 1/37205** (2013.01); **A61N 1/056** (2013.01)

(58) **Field of Classification Search**

CPC ... **A61N 1/368**; **A61N 1/37205**; **A61N 1/3756**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,486,506 A 12/1969 Auphan
3,659,615 A 5/1972 Enger
(Continued)

FOREIGN PATENT DOCUMENTS

CN 101185789 A 5/2008
CN 101284160 A 10/2008
(Continued)

OTHER PUBLICATIONS


US 8,116,861 B2, 02/2012, Root et al. (withdrawn)
(Continued)

Primary Examiner — George R Evanisko

(57) **ABSTRACT**

A leadless pacing system includes a leadless pacing device and a sensing extension extending from a housing of the leadless pacing device. The sensing extension includes one or more electrodes with which the leadless pacing device may sense electrical cardiac activity. The one or more electrodes of the sensing extension may be carried by a self-supporting body that is configured to passively position the one or more electrodes proximate or within a chamber of the heart other than the chamber in which the LPD is implanted.

21 Claims, 8 Drawing Sheets

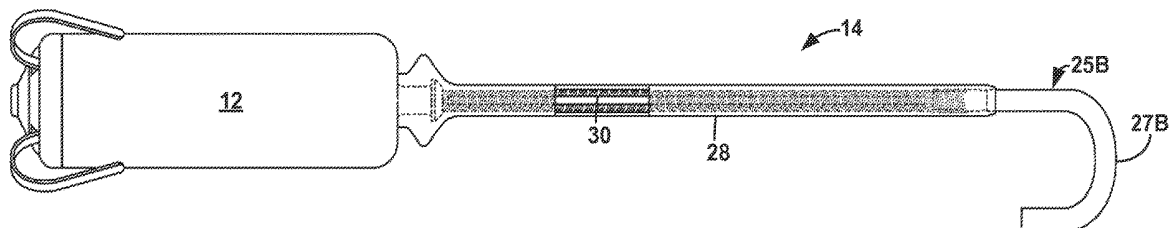

(51)	Int. Cl.							
	<i>A61B 5/0452</i>	(2006.01)						
	<i>A61N 1/05</i>	(2006.01)						
(56)	References Cited							
	U.S. PATENT DOCUMENTS							
	3,693,625	A	9/1972	Auphan	7,214,189	B2	5/2007	Zdeblick
	3,835,864	A	9/1974	Razor et al.	7,236,821	B2	6/2007	Cates et al.
	3,943,936	A	3/1976	Razor et al.	7,236,829	B1	6/2007	Farazi et al.
	4,157,720	A	6/1979	Greatbatch	7,260,436	B2	8/2007	Kilgore et al.
	RE30,366	E	8/1980	Razor et al.	7,283,874	B2	10/2007	Penner
	4,256,115	A	3/1981	Bilitch	7,286,883	B2	10/2007	Schulman et al.
	4,333,469	A	6/1982	Jeffcoat et al.	7,292,890	B2	11/2007	Whitehurst et al.
	5,170,784	A	12/1992	Ramon et al.	7,294,108	B1	11/2007	Bornzin et al.
	5,193,540	A	3/1993	Schulman et al.	7,295,879	B2	11/2007	Denker et al.
	5,193,539	A	6/1993	Schulman et al.	7,310,556	B2	12/2007	Bulkes
	5,243,977	A	9/1993	Trabucco et al.	7,330,756	B2	2/2008	Marnfeldt
	5,312,439	A	5/1994	Loeb	7,343,204	B2	3/2008	Schulman et al.
	5,324,316	A	6/1994	Schulman et al.	7,351,921	B1	4/2008	Haller et al.
	5,404,877	A	4/1995	Nolan et al.	7,363,082	B2	4/2008	Ransbury et al.
	5,405,367	A	4/1995	Schulman et al.	7,428,438	B2	9/2008	Parramon et al.
	5,411,535	A	5/1995	Fujii et al.	7,437,193	B2	10/2008	Parramon et al.
	5,441,527	A	8/1995	Erickson et al.	7,444,180	B2	10/2008	Kuzma et al.
	5,674,259	A	10/1997	Gray	7,450,998	B2	11/2008	Zilberman et al.
	5,792,208	A	8/1998	Gray	7,493,172	B2	2/2009	Whitehurst et al.
	5,814,089	A	9/1998	Stokes et al.	7,513,257	B2	4/2009	Schulman et al.
	5,843,132	A	12/1998	Ilvento	7,519,421	B2	4/2009	Denker et al.
	5,895,414	A	4/1999	Sanchez-Zambrano	7,519,424	B2	4/2009	Dennis et al.
	5,954,757	A	9/1999	Gray	7,529,589	B2	5/2009	Williams et al.
	5,970,986	A	10/1999	Bolz et al.	7,532,932	B2	5/2009	Denker et al.
	5,987,352	A	11/1999	Klein et al.	7,532,933	B2	5/2009	Hastings et al.
	6,044,300	A	3/2000	Gray	7,535,296	B2	5/2009	Bulkes et al.
	6,051,017	A	4/2000	Loeb et al.	7,555,345	B2	6/2009	Wahlstrand et al.
	6,141,588	A	10/2000	Cox et al.	7,558,631	B2	7/2009	Cowan et al.
	6,144,879	A	11/2000	Gray et al.	7,565,195	B1	7/2009	Kroll et al.
	6,175,764	B1	1/2001	Loeb et al.	7,587,241	B2	9/2009	Parramon et al.
	6,181,965	B1	1/2001	Loeb et al.	7,606,621	B2	10/2009	Brisken et al.
	6,185,452	B1	2/2001	Schulman et al.	7,610,092	B2	10/2009	Cowan et al.
	6,185,455	B1	2/2001	Loeb et al.	7,616,990	B2	11/2009	Chavan et al.
	6,208,894	B1	3/2001	Schulman et al.	7,616,992	B2	11/2009	Dennis et al.
	6,214,032	B1	4/2001	Loeb et al.	7,617,007	B2	11/2009	Williams et al.
	6,240,316	B1	5/2001	Richmond et al.	7,627,371	B2	12/2009	Wang et al.
	6,315,721	B2	11/2001	Schulman et al.	7,627,376	B2	12/2009	Dennis et al.
	6,415,184	B1	7/2002	Ishikawa et al.	7,627,383	B2	12/2009	Haller et al.
	6,445,953	B1	9/2002	Bulkes et al.	7,630,767	B1	12/2009	Poore et al.
	6,592,518	B2	7/2003	Denker et al.	7,634,313	B1	12/2009	Kroll et al.
	6,628,989	B1	9/2003	Penner et al.	7,637,867	B2	12/2009	Zdeblick
	6,654,638	B1	11/2003	Sweeny	7,640,060	B2	12/2009	Zdeblick
	6,733,485	B1	5/2004	Whitehurst et al.	7,640,061	B2	12/2009	He et al.
	6,735,474	B1	5/2004	Loeb et al.	7,640,601	B2	1/2010	Lee
	6,735,475	B1	5/2004	Whitehurst et al.	7,647,109	B2	1/2010	Hastings et al.
	6,738,672	B2	5/2004	Schulman et al.	7,650,186	B2	1/2010	Hastings et al.
	6,764,446	B2	7/2004	Wolinsky et al.	7,706,892	B2	4/2010	Colvin et al.
	6,788,975	B1	9/2004	Whitehurst et al.	7,713,194	B2	5/2010	Zdeblick
	6,804,561	B2	10/2004	Stover	7,734,343	B2	6/2010	Ransbury et al.
	6,871,099	B1	3/2005	Whitehurst et al.	7,747,335	B2	6/2010	Williams
	6,907,285	B2	6/2005	Denker et al.	7,751,881	B2	7/2010	Cowan et al.
	6,917,833	B2	7/2005	Denker et al.	7,766,216	B2	8/2010	Daulton
	6,941,171	B2	9/2005	Mann et al.	7,771,838	B1	8/2010	He et al.
	6,947,782	B2	9/2005	Schulman et al.	7,781,683	B2	8/2010	Haller et al.
	7,003,350	B2	2/2006	Denker et al.	7,809,438	B2	10/2010	Echt et al.
	7,006,864	B2	2/2006	Echt et al.	7,822,480	B2	10/2010	Park et al.
	7,024,248	B2	4/2006	Penner et al.	7,826,903	B2	11/2010	Denker et al.
	7,050,849	B2	5/2006	Echt et al.	7,840,282	B2	11/2010	Williams et al.
	7,054,692	B1	5/2006	Whitehurst et al.	7,848,815	B2	12/2010	Brisken et al.
	7,082,336	B2	7/2006	Ransbury et al.	7,848,823	B2	12/2010	Drasler et al.
	7,103,408	B2	9/2006	Haller et al.	7,860,564	B2	12/2010	Root et al.
	7,114,502	B2	10/2006	Schulman et al.	7,860,570	B2	12/2010	Whitehurst et al.
	7,120,992	B2	10/2006	He et al.	7,890,173	B2	2/2011	Brisken et al.
	7,132,173	B2	11/2006	Daulton	7,894,907	B2	2/2011	Cowan et al.
	7,167,751	B1	1/2007	Whitehurst et al.	7,899,541	B2	3/2011	Cowan et al.
	7,177,698	B2	2/2007	Klosterman et al.	7,899,542	B2	3/2011	Cowan et al.
	7,184,830	B2	2/2007	Echt et al.	7,899,554	B2	3/2011	Williams et al.
	7,198,603	B2	4/2007	Penner et al.	7,904,167	B2	3/2011	Klosterman et al.
	7,200,437	B1	4/2007	Nabutovsky et al.	7,930,031	B2	4/2011	Penner
	7,203,548	B2	4/2007	Whitehurst et al.	7,937,148	B2	5/2011	Jacobson
					7,945,333	B2	5/2011	Jacobson
					7,954,533	B2	6/2011	Nonaka et al.
					7,957,805	B2	6/2011	He
					7,979,126	B2	7/2011	Payne et al.
					7,991,467	B2	8/2011	Markowitz et al.
					7,996,097	B2	8/2011	DiBernardo et al.
					8,010,209	B2	8/2011	Jacobson
					8,019,419	B1	9/2011	Panescu et al.
					8,032,219	B2	10/2011	Neumann et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,032,220	B2	10/2011	Kuzma	2006/0173497	A1	8/2006	Mech et al.
8,032,227	B2	10/2011	Parramon et al.	2006/0241705	A1	10/2006	Neumann et al.
8,078,279	B2	12/2011	Dennis et al.	2006/0241732	A1	10/2006	Denker et al.
8,078,283	B2	12/2011	Cowan et al.	2007/0027508	A1	2/2007	Cowan et al.
8,116,883	B2	2/2012	Williams et al.	2007/0060961	A1	3/2007	Echt et al.
8,126,561	B2	2/2012	Chavan et al.	2007/0073353	A1	3/2007	Rooney et al.
8,127,424	B2	3/2012	Haller et al.	2007/0075905	A1	4/2007	Denker et al.
8,165,696	B2	4/2012	McClure et al.	2007/0078490	A1	4/2007	Cowan et al.
8,185,212	B2	5/2012	Carbunaru et al.	2007/0088396	A1	4/2007	Jacobson
8,204,595	B2	6/2012	Pianca et al.	2007/0088397	A1	4/2007	Jacobson
8,224,449	B2	7/2012	Carbunaru et al.	2007/0106332	A1	5/2007	Denker et al.
8,239,045	B2	8/2012	Ransbury et al.	2007/0106357	A1	5/2007	Denker et al.
8,240,780	B1	8/2012	Klimes	2007/0118187	A1	5/2007	Denker et al.
8,295,939	B2	10/2012	Jacobson	2007/0129773	A1	6/2007	Bulkes
8,301,242	B2	10/2012	Root et al.	2007/0135883	A1	6/2007	Drasler et al.
8,301,262	B2	10/2012	Mi et al.	2007/0150037	A1	6/2007	Hastings et al.
8,311,627	B2	11/2012	Root et al.	2007/0156204	A1	7/2007	Denker et al.
8,315,701	B2	11/2012	Cowan et al.	2007/0179550	A1	8/2007	Dennis et al.
8,321,036	B2	11/2012	Brockway et al.	2007/0179552	A1	8/2007	Dennis et al.
8,332,036	B2	12/2012	Hastings et al.	2007/0179581	A1	8/2007	Dennis et al.
8,340,780	B2	12/2012	Hastings et al.	2007/0185538	A1	8/2007	Denker et al.
8,352,025	B2	1/2013	Jacobson	2007/0210862	A1	9/2007	Denker et al.
8,352,028	B2	1/2013	Wenger	2007/0219590	A1	9/2007	Hastings et al.
8,359,098	B2	1/2013	Lund et al.	2007/0276444	A1	11/2007	Gelbart et al.
8,364,267	B2	1/2013	Schleicher et al.	2007/0288076	A1	12/2007	Bulkes et al.
8,364,276	B2	1/2013	Willis	2007/0288077	A1	12/2007	Bulkes et al.
8,364,278	B2	1/2013	Pianca et al.	2007/0293904	A1	12/2007	Gelbart et al.
8,364,280	B2	1/2013	Marnfeldt et al.	2007/0293908	A1	12/2007	Cowan et al.
8,368,051	B2	2/2013	Ting et al.	2007/0293912	A1	12/2007	Cowan et al.
8,374,696	B2	2/2013	Sanchez et al.	2007/0293913	A1	12/2007	Cowan et al.
8,386,051	B2	2/2013	Rys	2008/0033497	A1	2/2008	Bulkes et al.
8,457,742	B2	6/2013	Jacobson	2008/0039094	A1	2/2008	Jeong et al.
8,478,408	B2	7/2013	Hastings et al.	2008/0039904	A1	2/2008	Bulkes et al.
8,478,431	B2	7/2013	Griswold et al.	2008/0051854	A1	2/2008	Bulkes et al.
8,489,205	B2	7/2013	Stotts et al.	2008/0058886	A1	3/2008	Williams
8,494,637	B2	7/2013	Cowan et al.	2008/0077184	A1	3/2008	Denker et al.
8,494,642	B2	7/2013	Cowan et al.	2008/0077188	A1	3/2008	Denker et al.
8,494,644	B2	7/2013	Cowan et al.	2008/0097529	A1	4/2008	Parramon et al.
8,504,156	B2	8/2013	Bonner et al.	2008/0109054	A1	5/2008	Hastings et al.
8,527,068	B2	9/2013	Ostroff	2008/0119911	A1	5/2008	Rosero
8,532,790	B2	9/2013	Griswold	2008/0132961	A1	6/2008	Jaax et al.
8,541,131	B2	9/2013	Lund et al.	2008/0140154	A1	6/2008	Loeb et al.
8,543,190	B2	9/2013	Wasson et al.	2008/0288039	A1	11/2008	Reddy
8,543,204	B2	9/2013	Demmer et al.	2008/0294208	A1	11/2008	Willis et al.
8,543,205	B2	9/2013	Ostroff	2008/0294210	A1	11/2008	Rosero
8,543,216	B2	9/2013	Carbunaru et al.	2008/0319502	A1	12/2008	Sunagawa et al.
8,548,605	B2	10/2013	Ollivier	2009/0024180	A1	1/2009	Kisker et al.
8,560,892	B2	10/2013	Nicholes	2009/0048583	A1	2/2009	Williams et al.
8,565,897	B2	10/2013	Regnier et al.	2009/0082827	A1	3/2009	Kveen et al.
8,588,926	B2	11/2013	Moore et al.	2009/0082828	A1	3/2009	Ostroff
8,615,310	B2	12/2013	Khairkahan et al.	2009/0171408	A1	7/2009	Solem
8,626,294	B2	1/2014	Sheldon et al.	2009/0192570	A1	7/2009	Jaax et al.
8,634,912	B2	1/2014	Bornzin et al.	2009/0198293	A1	8/2009	Cauller et al.
8,634,919	B1	1/2014	Hou et al.	2009/0198295	A1	8/2009	Dennis et al.
8,639,335	B2	1/2014	Peichel et al.	2009/0198308	A1	8/2009	Gross et al.
8,644,922	B2	2/2014	Root et al.	2009/0326601	A1	12/2009	Brisken et al.
8,660,660	B2	2/2014	Dai et al.	2010/0094367	A1	4/2010	Sen
8,670,842	B1	3/2014	Bornzin et al.	2010/0137936	A1	6/2010	Dennis et al.
8,700,181	B2	4/2014	Bornzin et al.	2010/0161002	A1	6/2010	Aghassian et al.
2003/0114905	A1	6/2003	Kuzma	2010/0179628	A1	7/2010	Towe et al.
2004/0015204	A1	1/2004	Whitehurst et al.	2010/0249883	A1	9/2010	Zdeblick
2004/0073267	A1	4/2004	Holzer	2010/0249885	A1	9/2010	Colvin et al.
2004/0093039	A1	5/2004	Schumert	2010/0286744	A1	11/2010	Echt et al.
2004/0122477	A1	6/2004	Whitehurst et al.	2010/0304209	A1	12/2010	Lund et al.
2004/0133242	A1	7/2004	Chapman et al.	2010/0305627	A1	12/2010	Anderson
2004/0147973	A1	7/2004	Hauser	2010/0305628	A1	12/2010	Lund et al.
2004/0162590	A1	8/2004	Whitehurst et al.	2010/0305629	A1	12/2010	Lund et al.
2004/0172089	A1	9/2004	Whitehurst et al.	2010/0312320	A1	12/2010	Faltys et al.
2005/0055061	A1	3/2005	Holzer	2011/0054555	A1	3/2011	Williams et al.
2005/0070962	A1	3/2005	Echt et al.	2011/0060392	A1	3/2011	Zdeblick et al.
2005/0256549	A1	11/2005	Holzer	2011/0071585	A1	3/2011	Ransbury et al.
2005/0288717	A1	12/2005	Sunagawa	2011/0071586	A1	3/2011	Jacobson
2006/0074449	A1	4/2006	Denker et al.	2011/0077708	A1	3/2011	Ostroff
2006/0135999	A1	6/2006	Bodner et al.	2011/0077721	A1	3/2011	Whitehurst et al.
2006/0136005	A1	6/2006	Brisken et al.	2011/0137378	A1	6/2011	Klosterman et al.
				2011/0160801	A1	6/2011	Markowitz et al.
				2011/0208260	A1	8/2011	Jacobson
				2011/0245782	A1	10/2011	Berthiaume et al.
				2011/0270339	A1	11/2011	Murray, III et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0270340 A1 11/2011 Pellegrini et al.
 2011/0282423 A1 11/2011 Jacobson
 2011/0313490 A1 12/2011 Parramon et al.
 2012/0059431 A1 3/2012 Williams et al.
 2012/0081201 A1 4/2012 Norgaard et al.
 2012/0095521 A1 4/2012 Hintz
 2012/0095539 A1 4/2012 Khairkahan et al.
 2012/0109149 A1 5/2012 Bonner et al.
 2012/0109236 A1 5/2012 Jacobson et al.
 2012/0116489 A1 5/2012 Khairkahan et al.
 2012/0143271 A1 6/2012 Root et al.
 2012/0158090 A1 6/2012 Chavan et al.
 2012/0158111 A1 6/2012 Khairkahan et al.
 2012/0165827 A1 6/2012 Khairkahan et al.
 2012/0172690 A1 7/2012 Anderson et al.
 2012/0172891 A1 7/2012 Lee
 2012/0172892 A1 7/2012 Grubac et al.
 2012/0179219 A1 7/2012 Kisker et al.
 2012/0197352 A1 8/2012 Carbanaru et al.
 2012/0197373 A1 8/2012 Khairkahan et al.
 2012/0232371 A1 9/2012 Mech et al.
 2012/0290021 A1 11/2012 Saurkar et al.
 2012/0290025 A1 11/2012 Keimel
 2012/0316622 A1 12/2012 Whitehurst et al.
 2012/0323099 A1 12/2012 Mothilal et al.
 2013/0023975 A1 1/2013 Locsin
 2013/0030483 A1 1/2013 Demmer et al.
 2013/0035748 A1 2/2013 Bonner et al.
 2013/0053921 A1* 2/2013 Bonner A61N 1/3756
 607/36
 2013/0066169 A1 3/2013 Rys et al.
 2013/0073004 A1 3/2013 Root et al.
 2013/0079798 A1 3/2013 Tran et al.
 2013/0079861 A1 3/2013 Reinert et al.
 2013/0103047 A1 4/2013 Steingisser et al.
 2013/0103109 A1 4/2013 Jacobson
 2013/0110127 A1 5/2013 Bornzin et al.
 2013/0110219 A1 5/2013 Bornzin et al.
 2013/0116529 A1 5/2013 Min et al.
 2013/0116738 A1 5/2013 Samade et al.
 2013/0116740 A1* 5/2013 Bornzin A61N 1/3756
 607/9
 2013/0116741 A1* 5/2013 Bornzin A61N 1/3756
 607/9
 2013/0123872 A1 5/2013 Bornzin et al.
 2013/0123875 A1 5/2013 Varady et al.
 2013/0131159 A1 5/2013 Ko et al.
 2013/0131693 A1 5/2013 Berthiaume et al.
 2013/0138006 A1 5/2013 Bornzin et al.
 2013/0150695 A1 6/2013 Biela et al.
 2013/0184790 A1 7/2013 Schleicher et al.
 2013/0226259 A1 8/2013 Penner et al.
 2013/0231710 A1 9/2013 Jacobson
 2013/0234692 A1 9/2013 Liang et al.
 2013/0235663 A1 9/2013 Walsh et al.
 2013/0235672 A1 9/2013 Walsh et al.
 2013/0238044 A1 9/2013 Penner
 2013/0238056 A1 9/2013 Poore et al.
 2013/0238072 A1 9/2013 Deterre et al.
 2013/0238073 A1 9/2013 Makdissi et al.
 2013/0238840 A1 9/2013 Walsh et al.
 2013/0253309 A1 9/2013 Allan et al.
 2013/0253344 A1 9/2013 Griswold et al.
 2013/0253345 A1 9/2013 Griswold et al.
 2013/0253346 A1 9/2013 Griswold et al.
 2013/0253347 A1 9/2013 Griswold et al.
 2013/0261497 A1 10/2013 Pertijis et al.
 2013/0268042 A1 10/2013 Hastings et al.
 2013/0274828 A1 10/2013 Willis

2013/0274847 A1 10/2013 Ostroff
 2013/0280270 A1 10/2013 Sunday et al.
 2013/0282070 A1 10/2013 Cowan et al.
 2013/0282073 A1 10/2013 Cowan et al.
 2013/0302665 A1 11/2013 Zhao et al.
 2013/0303872 A1 11/2013 Taff et al.
 2013/0323099 A1 12/2013 Li et al.
 2013/0324825 A1 12/2013 Ostroff et al.
 2013/0325081 A1* 12/2013 Karst A61N 1/36592
 607/25
 2013/0345770 A1* 12/2013 Dianaty A61N 1/368
 607/36
 2014/0012342 A1 1/2014 Penner et al.
 2014/0012344 A1 1/2014 Hastings et al.
 2014/0018876 A1 1/2014 Ostroff
 2014/0018877 A1 1/2014 Demmer et al.
 2014/0026016 A1 1/2014 Nicholes
 2014/0031836 A1 1/2014 Ollivier
 2014/0031837 A1 1/2014 Perryman et al.
 2014/0039570 A1 2/2014 Carroll et al.
 2014/0039578 A1 2/2014 Whitehurst et al.
 2014/0039588 A1 2/2014 Ok et al.
 2014/0039591 A1 2/2014 Drasler et al.
 2014/0046395 A1 2/2014 Regnier et al.
 2014/0058240 A1 2/2014 Mothilal et al.
 2014/0072872 A1 3/2014 Hodgkinson et al.
 2014/0100627 A1 4/2014 Min
 2014/0107723 A1 4/2014 Hou et al.
 2014/0172034 A1* 6/2014 Bornzin A61N 1/375
 607/17

FOREIGN PATENT DOCUMENTS

EP 1541191 A1 6/2005
 EP 2662113 A3 1/2014
 TW I251986 B 3/2006
 TW I252007 B 3/2006
 WO 2006099425 A1 9/2006
 WO 2009006531 A1 1/2009
 WO 2009052480 A2 4/2009
 WO 2012154599 A2 11/2012
 WO 2013080038 A2 6/2013
 WO 2012150000 11/2013
 WO 20130184787 A1 12/2013
 WO 2014046662 3/2014

OTHER PUBLICATIONS

Response to Office Action dated Feb. 26, 2016, from U.S. Appl. No. 14/694,952, filed May 20, 2016, 10 pp.
 Final Office Action from U.S. Appl. No. 14/694,952, dated Sep. 14, 2016, 20 pp.
 Response to Final Office Action dated Sep. 14, 2016, from U.S. Appl. No. 14/694,952, filed Nov. 14, 2016, 8 pp.
 U.S. Appl. No. 14/694,952, office action dated Feb. 26, 2016, 46 pages.
 (PCT/US2015/040934) PCT Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, dated Sep. 30, 2015, 11 pages.
 Pre-Appeal Brief Request for Review from U.S. Appl. No. 14/694,952, filed Dec. 21, 2016, 6 pp.
 Advisory Action from U.S. Appl. No. 14/694,952, dated Dec. 21, 2016, 4 pp.
 Examiners Answer to Appeal Brief from U.S. Appl. No. 14/694,952, dated Jul. 28, 2017, 11 pp.
 Reply Brief in response to the Examiner's Answer dated Jul. 28, 2017, from U.S. Appl. No. 14/694,952, filed Sep. 28, 2017, 14 pp.
 Decision on Appeal from U.S. Appl. No. 14/694,952, dated Dec. 19, 2018, 9 pp.

* cited by examiner

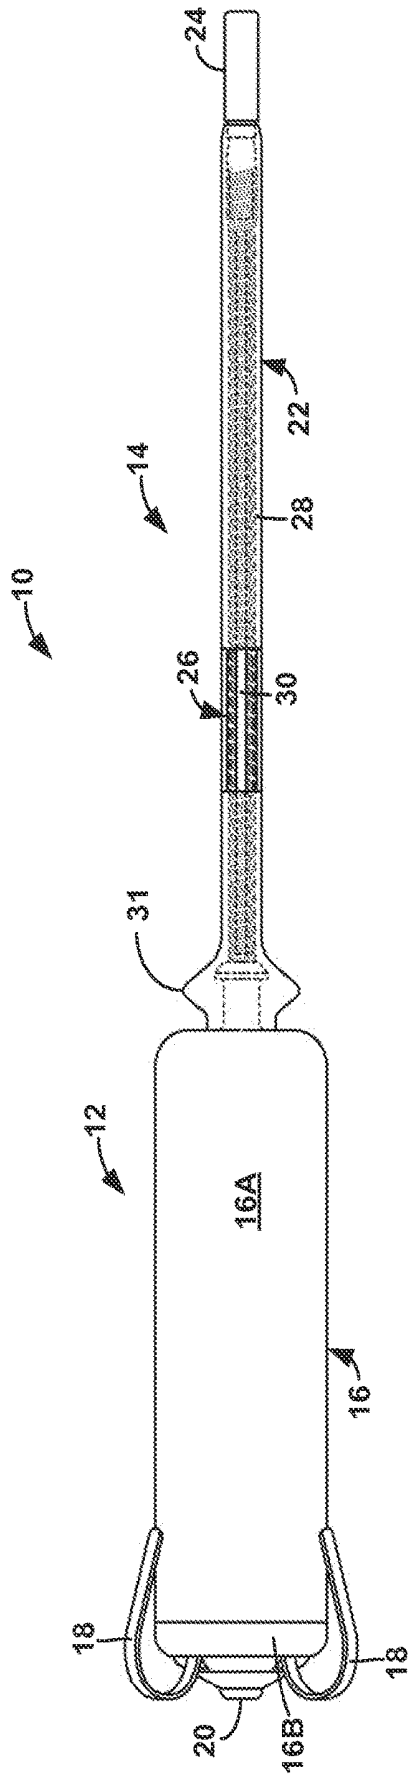


FIG. 1

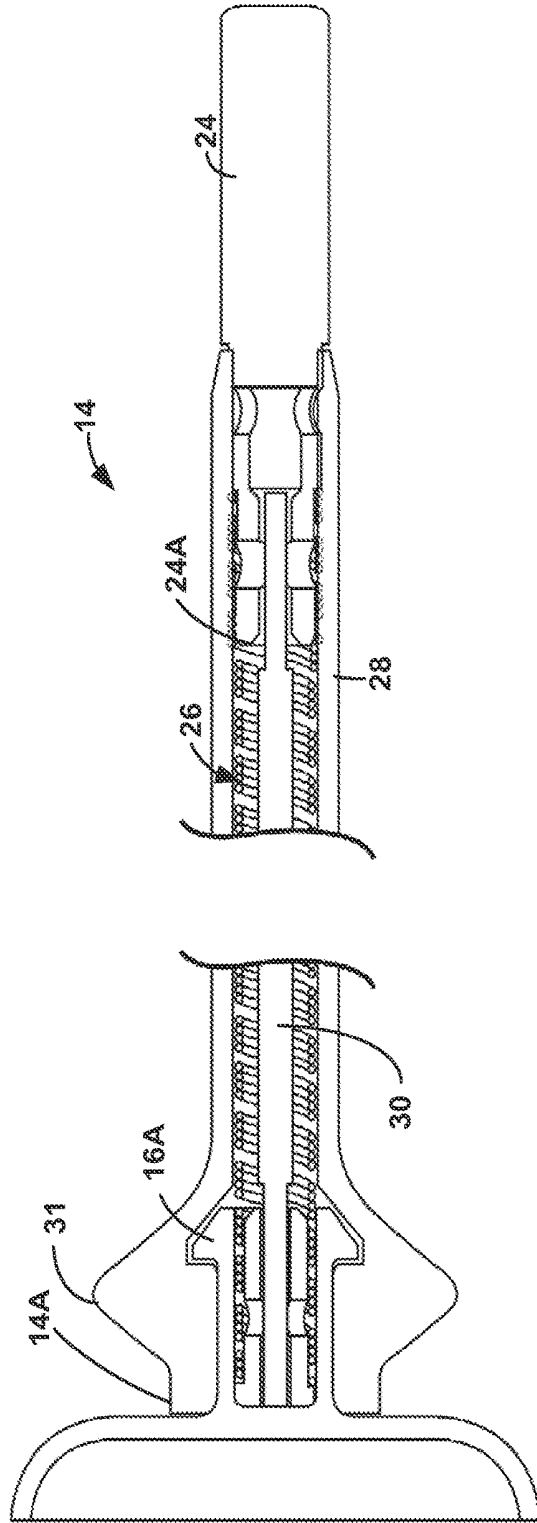


FIG. 2

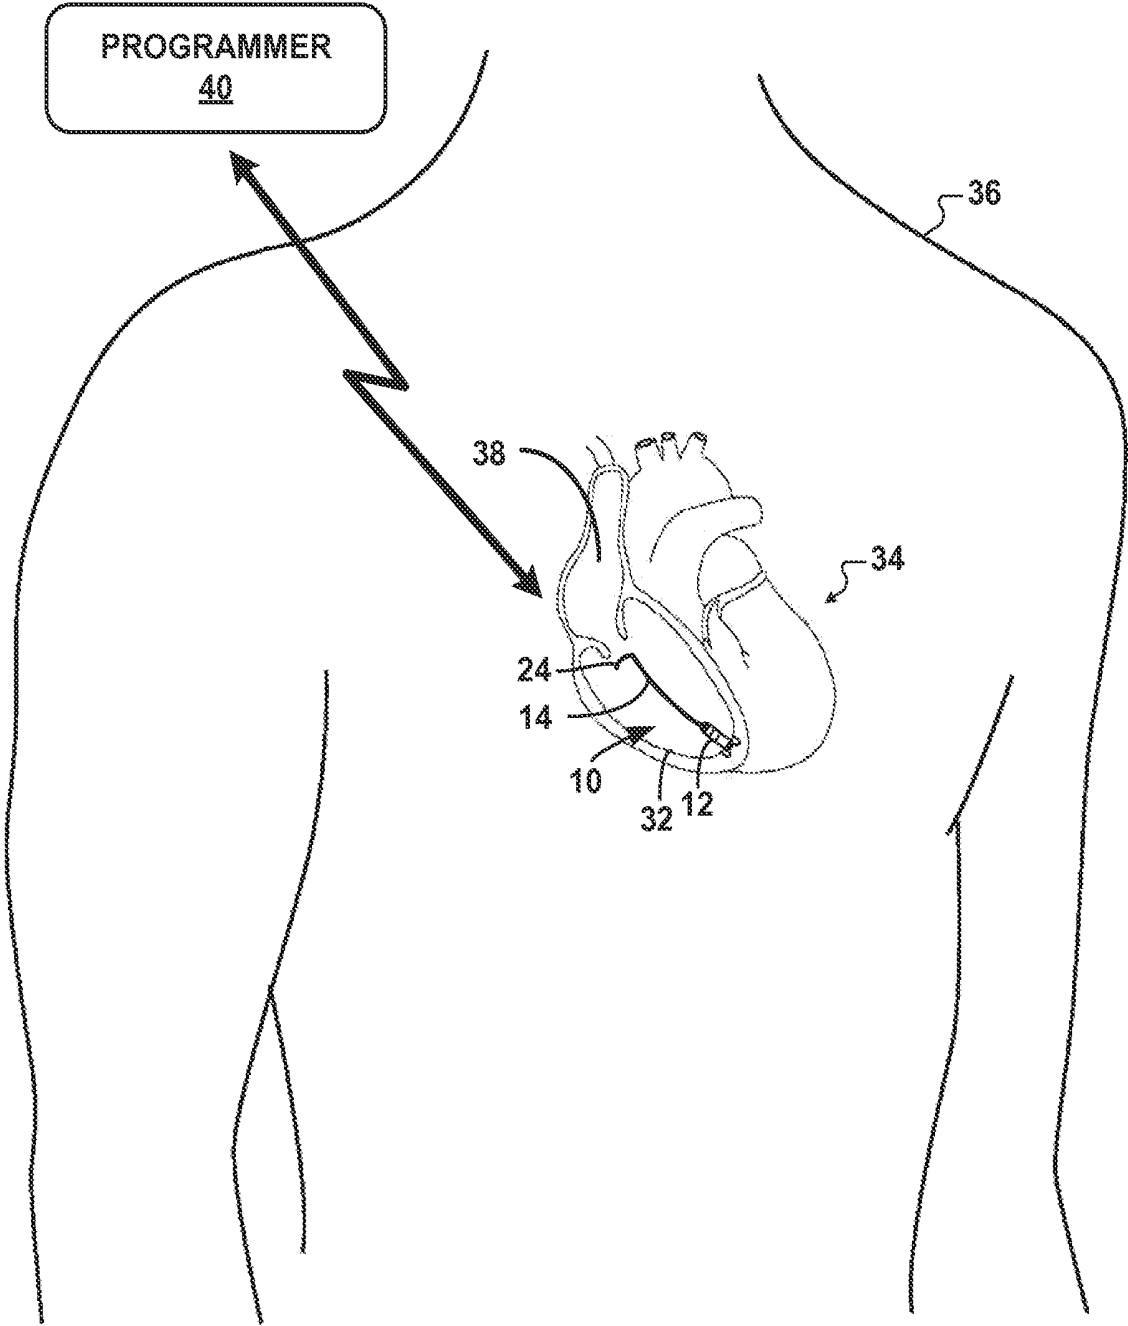


FIG. 3

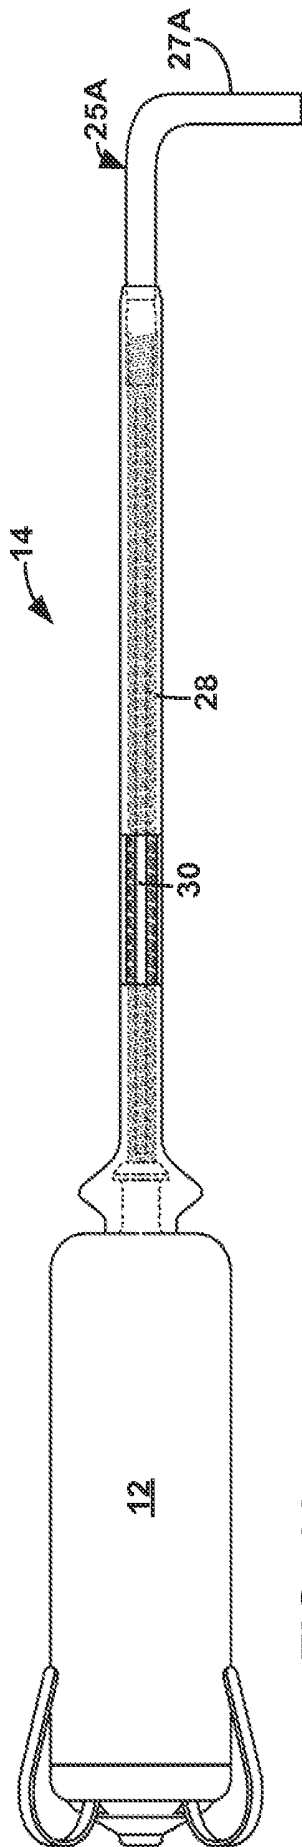


FIG. 4A

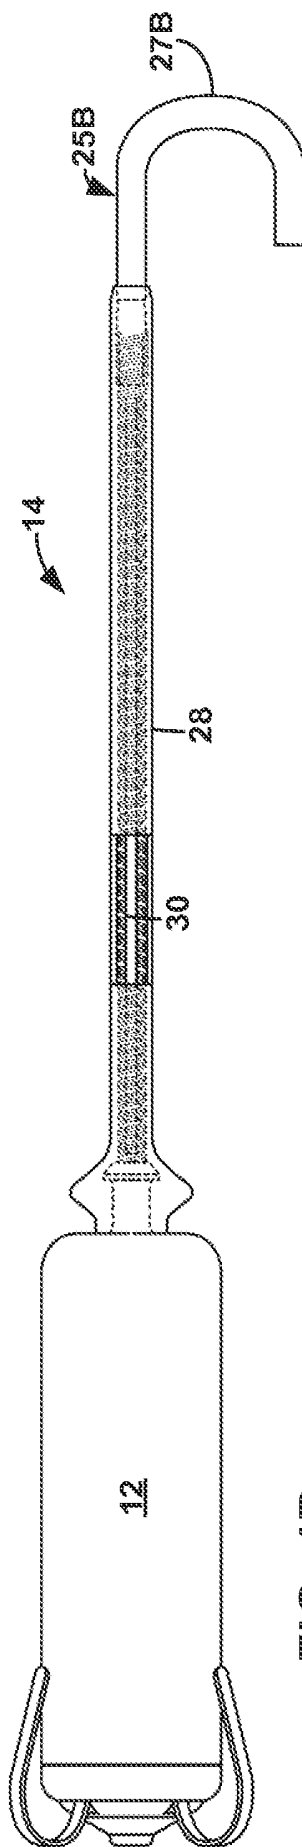


FIG. 4B

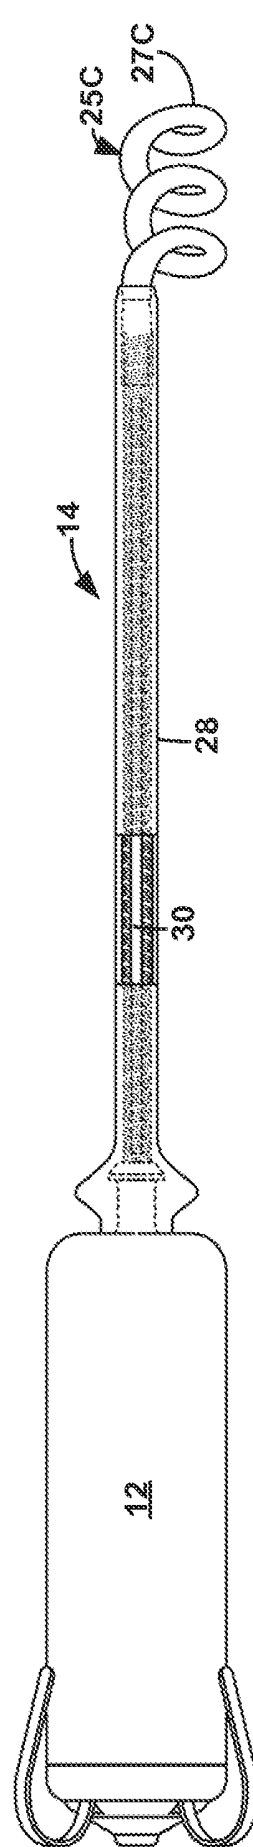


FIG. 4C

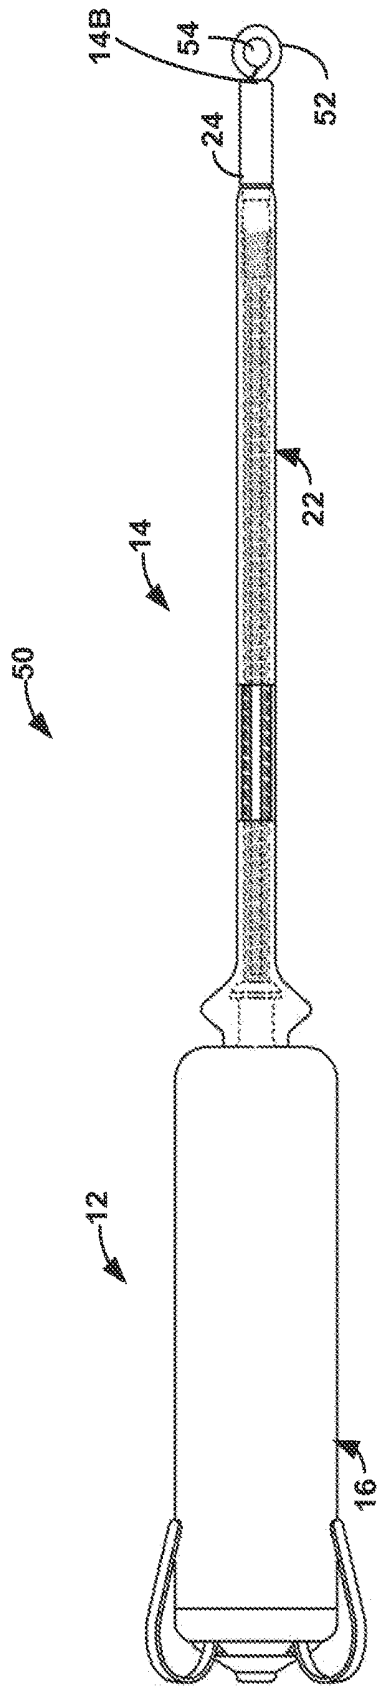


FIG. 5

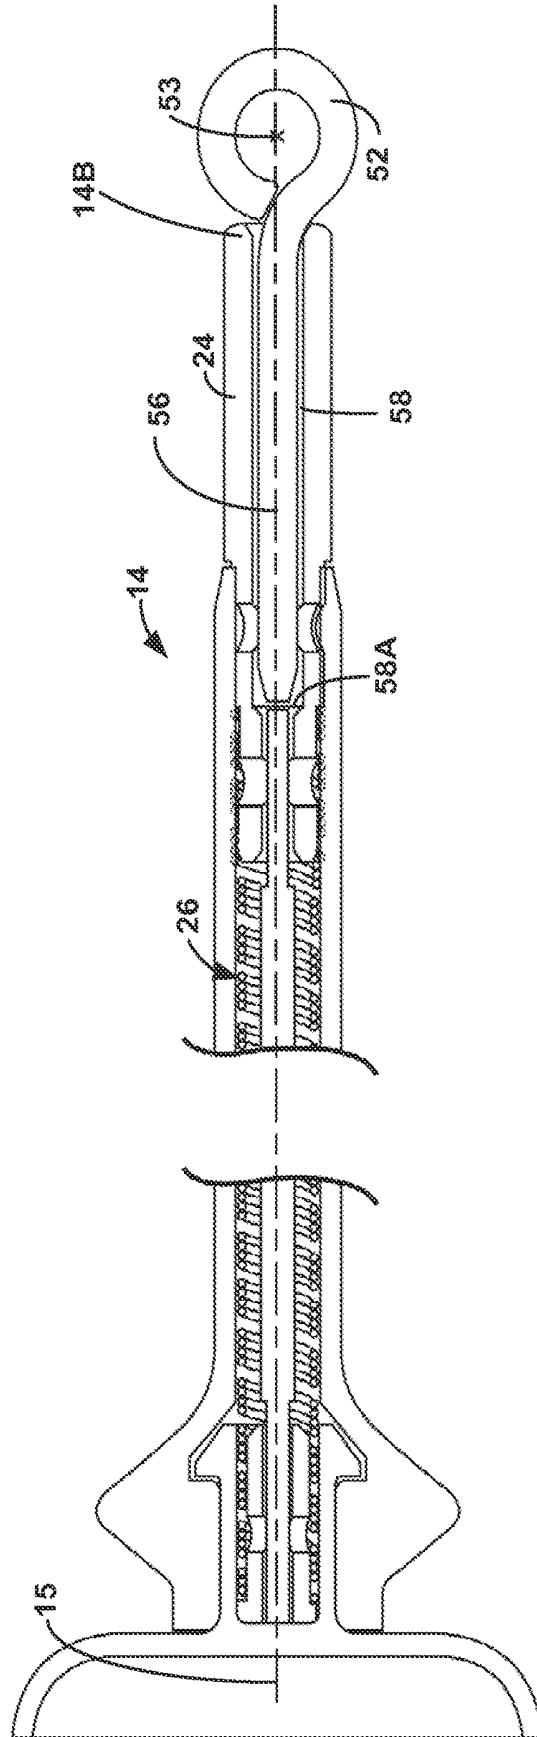


FIG. 6

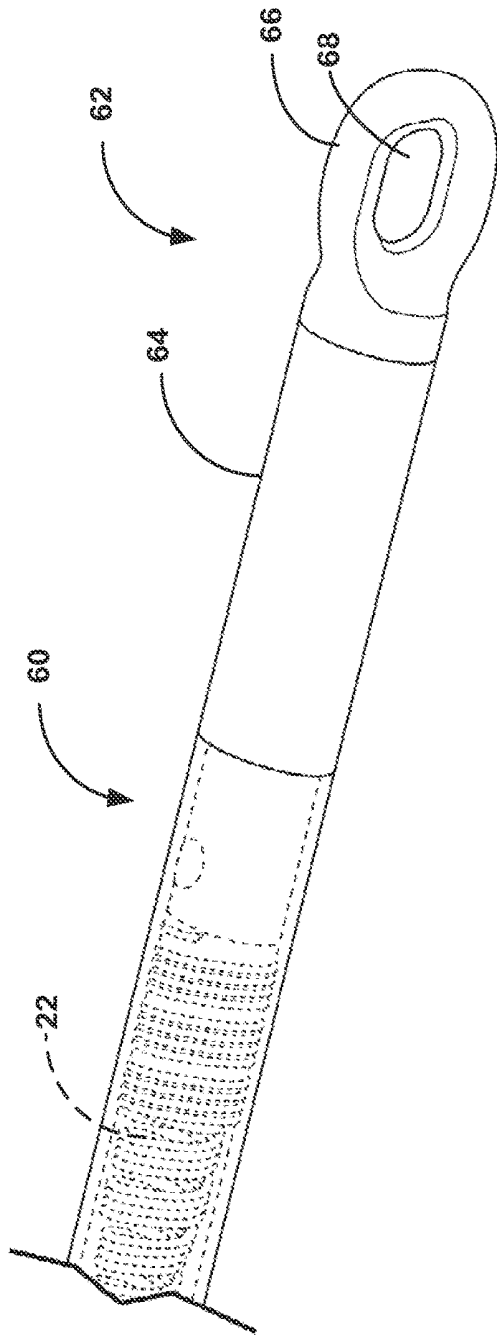


FIG. 7

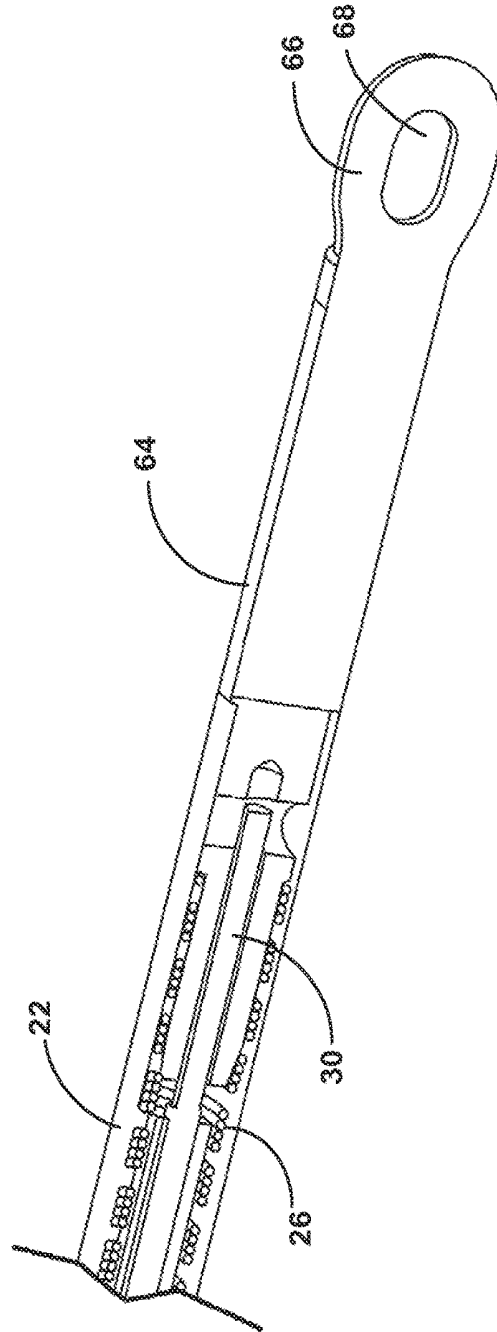


FIG. 8

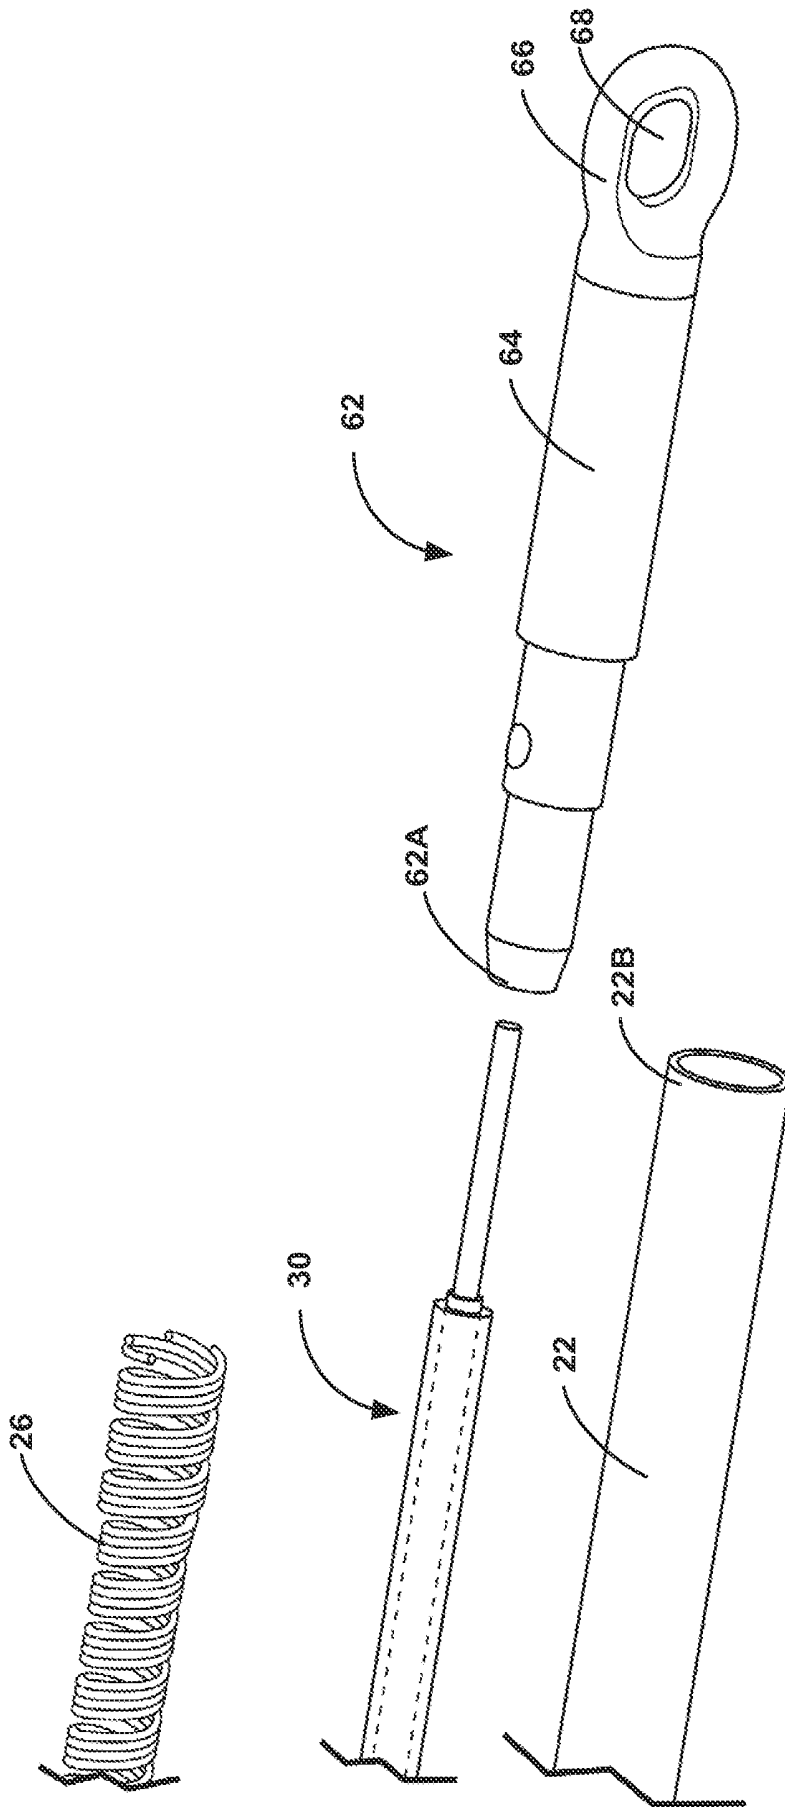


FIG. 9

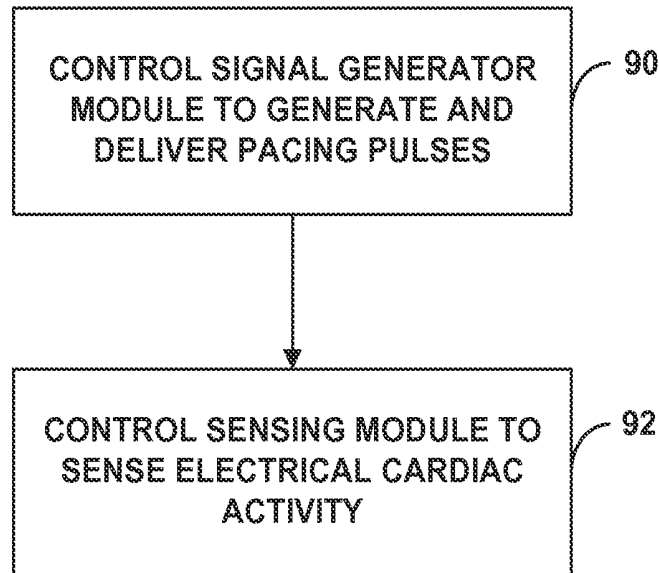


FIG. 11

LEADLESS PACING SYSTEM INCLUDING SENSING EXTENSION

This application claims the benefit of U.S. Provisional Application Ser. No. 62/025,690 by Sheldon et al., filed Jul. 17, 2014, and entitled "LEADLESS PACING SYSTEM INCLUDING SENSING EXTENSION," which is incorporated herein by reference in its entirety.

TECHNICAL FIELD

The disclosure relates to cardiac pacing, and more particularly, to cardiac pacing using a leadless pacing device.

BACKGROUND

An implantable pacemaker may deliver pacing pulses to a patient's heart and monitor conditions of the patient's heart. In some examples, the implantable pacemaker comprises a pulse generator and one or more electrical leads. The pulse generator may, for example, be implanted in a small pocket in the patient's chest. The electrical leads may be coupled to the pulse generator, which may contain circuitry that generates pacing pulses and/or senses cardiac electrical activity. The electrical leads may extend from the pulse generator to a target site (e.g., an atrium and/or a ventricle) such that electrodes at the proximal ends of the electrical leads are positioned at a target site. The pulse generator may provide electrical stimulation to the target site and/or monitor cardiac electrical activity at the target site via the electrodes.

A leadless pacing device has also been proposed for sensing electrical activity and/or delivering therapeutic electrical signals to the heart. The leadless pacing device may include one or more electrodes on its outer housing to deliver therapeutic electrical signals and/or sense intrinsic depolarizations of the heart. The leadless pacing device may be positioned within or outside of the heart and, in some examples, may be anchored to a wall of the heart via a fixation mechanism.

SUMMARY

The disclosure describes a leadless pacing system that includes a leadless pacing device (hereinafter, "LPD") and a sensing extension extending from a housing of the LPD, where the sensing extension includes one or more electrodes with which the LPD may sense electrical cardiac activity. The sensing extension is electrically coupled to a sensing module of the LPD via a conductive portion of the housing of the LPD. The one or more electrodes of the sensing extension may be carried by a self-supporting body that is configured to passively position the one or more electrodes proximate or within a chamber of the heart other than the chamber in which the LPD is implanted. In some examples, a proximal portion of the sensing extension is configured to reduce interference with the mechanical movement of the heart.

The sensing extension facilitates sensing, by the LPD, of electrical activity of a chamber of the heart other than the one in which the LPD is implanted. The LPD is configured to be implanted within a chamber of the heart of the patient and the sensing extension is configured to extend away from the LPD to position an electrode proximate or within another chamber of the heart, e.g., to sense electrical activity of the other chamber. In some examples, the sensing extension includes a feature configured to facilitate control of the

sensing extension during implantation of the sensing extension in the patient. The feature may be, for example, an eyelet at a proximal end of the sensing extension, the eyelet being configured to receive a tether that may be used to control the positioning of the proximal end of the sensing extension during implantation of the leadless pacing system in a patient. The tether may also be used to confirm the LPD is fixed to the target tissue site, e.g., to perform a tug test.

In one aspect, the disclosure is directed to a system comprising a leadless pacing device comprising a stimulation module configured to generate pacing pulses, a sensing module, a processing module, a housing comprising a conductive portion, wherein the housing is configured to be implanted within a chamber of a heart of a patient and encloses the stimulation module, the sensing module, and the processing module, and a first electrode electrically coupled to the sensing module and the stimulation module. The system further comprises a sensing extension extending from the housing and comprising a self-supporting body extending from the housing and comprising a curved proximal portion, and a second electrode carried by the self-supporting body and electrically connected to the sensing module and the stimulation module via the conductive portion of the housing. The processing module is configured to control the sensing module to sense electrical cardiac activity via the second electrode.

In another aspect, the disclosure is directed to a method comprising controlling, by a processor, a stimulation module of a leadless pacing device to deliver a pacing pulse to a patient, the leadless pacing device comprising the stimulation module, a sensing module, the processor, a housing comprising a conductive portion, wherein the housing is configured to be implanted within a chamber of a heart of a patient and encloses the stimulation module, the sensing module, and the processor, and a first electrode electrically coupled to the sensing module and the stimulation module. The method further comprises controlling, by the processor, the sensing module of the leadless pacing device to sense electrical cardiac activity via the first electrode and a second electrode of a sensing extension that extends from the housing, the sensing extension further comprising a self-supporting body extending from the housing and comprising a curved proximal portion, and the second electrode carried by the self-supporting body and electrically connected to the sensing module and the stimulation module via the conductive portion of the housing.

In another aspect, the disclosure is directed to a system comprising a leadless pacing device comprising a stimulation module configured to generate pacing pulses, a sensing module, a processing module, a housing comprising a conductive portion, wherein the housing is configured to be implanted within a chamber of a heart of a patient and encloses the stimulation module, the sensing module, and the processing module, and wherein the conductive portion is electrically connected to the sensing module, and a first electrode electrically coupled to the sensing module and the stimulation module. The system further comprises a sensing extension extending from the housing and comprising a self-supporting body mechanically connected to the housing and comprising a conductor electrically connected to the conductive portion of the housing, a second electrode carried by the self-supporting body and electrically connected to the conductor, and an eyelet at a proximal end of the sensing extension.

In another aspect, the disclosure is directed to a system comprising a leadless pacing device comprising a stimulation module configured to generate pacing pulses, a sensing

module, a processing module, a housing configured to be implanted within a chamber of a heart of a patient, wherein the housing encloses the stimulation module, the sensing module, and the processing module, and a first electrode electrically coupled to the sensing module and the stimulation module. The system further comprises an extension extending from the housing and comprising a body mechanically connected to the housing and comprising a conductor electrically connected to at least one of the sensing module or the stimulation module, a second electrode carried by the body and electrically connected to the conductor, and an eyelet at a proximal end of the extension.

In another aspect, the disclosure is directed to a method comprising controlling, by a processor, a stimulation module of a leadless pacing device to deliver a pacing pulse to a patient, the leadless pacing device comprising the stimulation module, a sensing module, the processor, a housing configured to be implanted within a chamber of a heart of a patient, wherein the housing encloses the stimulation module, the sensing module, and the processing module, and a first electrode electrically coupled to the sensing module and the stimulation module. The method further comprises controlling, by the processor, the sensing module of the leadless pacing device to sense electrical cardiac activity via the first electrode and a second electrode of a sensing extension that extends from the housing, the sensing extension further comprising a body mechanically connected to the housing and comprising a conductor electrically connected to the sensing module, a second electrode carried by the body and electrically connected to the conductor, and an eyelet at a proximal end of the extension.

In another aspect, the disclosure is directed to a computer-readable storage medium comprising computer-readable instructions for execution by a processor. The instructions cause a programmable processor to perform any whole or part of the techniques described herein. The instructions may be, for example, software instructions, such as those used to define a software or computer program. The computer-readable medium may be a computer-readable storage medium such as a storage device (e.g., a disk drive, or an optical drive), memory (e.g., a Flash memory, read only memory (ROM), or random access memory (RAM)) or any other type of volatile or non-volatile memory that stores instructions (e.g., in the form of a computer program or other executable) to cause a programmable processor to perform the techniques described herein. In some examples, the computer-readable medium is an article of manufacture and is non-transitory.

The details of one or more examples are set forth in the accompanying drawings and the description below. Other features, objects, and advantages will be apparent from the description and drawings, and from the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates an example leadless pacing system that comprises a leadless pacing device and a sensing extension.

FIG. 2 is a schematic cross-sectional view of the sensing extension of FIG. 1.

FIG. 3 is a conceptual illustration of the leadless pacing system of FIG. 1 implanted in a patient.

FIGS. 4A-4C illustrate example shapes of a proximal end of a sensing extension.

FIG. 5 illustrates another example leadless pacing system that comprises a leadless pacing device and a sensing extension.

FIG. 6 is a schematic cross-sectional view of the sensing extension of FIG. 5.

FIG. 7 is a perspective view of another example sensing extension.

FIG. 8 is a cross-sectional perspective view of the sensing extension of FIG. 7.

FIG. 9 is an exploded perspective view of the sensing extension of FIG. 7.

FIG. 10 is a functional block diagram of an example leadless pacing system.

FIG. 11 is a flow diagram of an example technique for delivering therapy and sensing electrical cardiac activity with the leadless pacing system of FIG. 1.

DETAILED DESCRIPTION

A leadless pacing system includes an LPD and a sensing extension that is coupled to the LPD and configured to facilitate sensing of electrical activity of a chamber of the heart other than the one in which the LPD is implanted. The sensing extension includes one or more electrodes and a self-supporting body that extends away from an outer housing of the LPD. In contrast to leadless pacing systems, the leadless pacing systems described herein do not include leads that pass out of the heart. Rather, both the LPD and sensing extension are configured to be entirely implanted in a heart of a patient. In some examples, the sensing extension is sized to be entirely implanted within the same chamber of the heart as the LPD. In other examples, the LPD is configured to be implanted in a first chamber of the heart, and the sensing extension is sized to extend into another chamber.

The LPD is configured to be implanted within a first chamber (e.g., a ventricle) of a heart of a patient, and the sensing extension is configured to position one or more electrodes proximate or within a second chamber of the heart, e.g., to sense electrical activity of the second chamber. The sensing extension has a length sufficient to locate one or more electrodes of the sensing extension closer to the second chamber than any electrodes of the LPD. For example, the sensing extension may have a length selected to position the one or more electrodes of the sensing extension adjacent the right atrium or in the right atrium when the LPD is implanted in or near the apex of the right ventricle. The one or more electrodes of the sensing extension may be used to sense intrinsic ventricular electrical activity, as well as detect atrial electrical activity.

In some examples described herein, the self-supporting body is configured to passively (i.e., without any active fixation elements, such as tines or a fixation helix) position an electrode extension at a location away from the LPD, e.g., at a location proximate the second chamber of the heart. The self-supporting body may be flexible enough to reduce irritation to the tissue of the heart when the body contacts the tissue, but have sufficient rigidity to permit the sensing extension to extend away from the LPD housing and towards the second chamber, even in the presence of blood in the first chamber of the heart. The stiffness of the self-supporting body is selected to help prevent the body from collapsing in on itself and/or towards the LPD, e.g., in the presence of blood flow. In addition, the stiffness of the self-supporting body may be selected so that the body is configured to support its own weight, e.g., in the presence of gravity.

The sensing extension also includes a proximal portion that is configured to help reduce interference with the mechanical movement of the heart. For example, in

examples in which the LPD is configured to be implanted within a ventricle of the heart and the sensing extension is configured to extend towards an atrium, the proximal portion of the sensing extension may be shaped and sized to reduce interference with the opening and closing of an atrioventricular valve (e.g., the tricuspid valve or the mitral valve). In addition, the proximal end of the sensing extension is configured to be atraumatic (e.g., blunt) in order to reduce irritation to the heart tissue if the proximal end comes into contact with the heart tissue. As an example of a configuration of a proximal portion that may help reduce interference with the mechanical movement of the heart, the proximal portion may be curved with one or more bends. For example, the proximal portion may define an L-shaped curve, a C-shaped curve, a pigtail, or any other suitable curve.

In some examples, a sensing extension also includes a feature configured to facilitate control of the sensing extension during implantation of the sensing extension in the heart. In these examples, the sensing extension may or may not have a self-supporting body. In some examples, the feature includes an eyelet at a proximal end of the sensing extension. A tether may be fed through the eyelet prior to introducing the LPD and the sensing extension in a heart of a patient. During the implantation process, a clinician may pull back on the tether to help control the position of the proximal end of the sensing extension, to confirm that the LPD is adequately fixed to the target tissue site (e.g., a “tug test” that confirms the LPD does not move in response to a pull on the tether). After implantation, the tether may be removed from the eyelet.

FIG. 1 is a conceptual illustration of an example leadless pacing system 10 that includes LPD 12 and sensing extension 14. LPD 12 is configured to be implanted within a chamber of a heart of a patient, e.g., to monitor electrical activity of the heart and/or provide electrical therapy to the heart. In the example shown in FIG. 1, LPD 12 includes outer housing 16, a plurality of fixation tines 18, and electrode 20. Sensing extension 14 includes self-supporting body 22, electrode 24, and conductor 26.

Outer housing 16 has a size and form factor that allows LPD 12 to be entirely implanted within a chamber of a heart of a patient. In some examples, outer housing 16 may have a cylindrical (e.g., pill-shaped) form factor. LPD 12 may include a fixation mechanism configured to fix LPD 12 to cardiac tissue. For example, in the example shown in FIG. 1, LPD 12 includes fixation tines 18 extending from housing 16 and configured to engage with cardiac tissue to substantially fix a position of housing 16 within the chamber of the heart. Fixation tines 18 are configured to anchor housing 16 to the cardiac tissue such that LPD 12 moves along with the cardiac tissue during cardiac contractions. Fixation tines 18 may be fabricated from any suitable material, such as a shape memory material (e.g., Nitinol). Although LPD 12 includes a plurality of fixation tines 18 that are configured to anchor LPD 12 to cardiac tissue in a chamber of a heart, in other examples, LPD 12 may be fixed to cardiac tissue using other types of fixation mechanisms, such as, but not limited to, barbs, coils, and the like.

Housing 16 houses electronic components of LPD 12, e.g., a sensing module for sensing cardiac electrical activity via electrodes 20, 24, and an electrical stimulation module for delivering electrical stimulation therapy via electrodes 20, 24. Electronic components may include any discrete and/or integrated electronic circuit components that implement analog and/or digital circuits capable of producing the functions attributed to LPD 12 described herein. In some

examples, housing 16 may also house components for sensing other physiological parameters, such as acceleration, pressure, sound, and/or impedance.

Additionally, housing 16 may also house a memory that includes instructions that, when executed by one or more processors housed within housing 16, cause LPD 12 to perform various functions attributed to LPD 12 herein. In some examples, housing 16 may house a communication module that enables LPD 12 to communicate with other electronic devices, such as a medical device programmer. In some examples, housing 16 may house an antenna for wireless communication. Housing 16 may also house a power source, such as a battery. Housing 16 can be hermetically or near-hermetically sealed in order to help prevent fluid ingress into housing 16.

LPD 12 is configured to sense electrical activity of the heart and deliver electrical stimulation to the heart via electrodes 20, 24. LPD 12 comprises electrode 20 and sensing extension 14 comprises electrode 24. For example, electrode 20 may be mechanically connected to housing 16. As another example, electrode 20 may be defined by an outer portion of housing 16 that is electrically conductive. Fixation tines 18 may be configured to anchor LPD 12 to cardiac tissue such that electrode 20 maintains contact with the cardiac tissue.

Sensing extension 14 is configured to position electrode 24 proximate to or outside the chamber in which LPD 12 is implanted. For example, sensing extension 14 may be configured to position electrode 24 within a chamber other than the one in which LPD 12 resides. In this way, sensing extension 24 may extend the sensing capabilities of system 10. In the example shown in FIG. 1, electrode 24 is carried by self-supporting body 22 of sensing extension 14, and is located at a proximal end of body 22. In other examples, however, electrode 24 may have another position relative to body 22, such mid-way between housing 16 and the proximal end of body 22, or otherwise away from the proximal end of body 22. Electrode 24 may have any suitable configuration. For example, electrode 24 may have a ring-shaped configuration, or a partial-ring configuration. Electrode 24 may be formed from any suitable material, such as a titanium nitride coated metal.

In other examples, system 10 may include more than two electrodes. For example, LPD 12 and/or sensing extension 14 may have more than one electrode. As an example, one or more additional electrodes having the same polarity as electrode 24 may be carried by sensing extension 14. The one or more additional electrodes may be electrically connected to the same or a different electrical conductor than sensing extension 14. The additional electrodes of sensing extension 14 may increase the probability that an electrode of system 10 is positioned to sense electrical activity of a chamber of the heart other than the one in which LPD 12 is implanted.

In the example shown in FIG. 1, electrode 24 is electrically connected to at least some electronics of LPD 12 (e.g., a sensing module and a stimulation module) via electrical conductor 26 of sensing extension 14 and electrically conductive portion 16A of housing 16. Electrical conductor 26 is electrically connected to and extends between conductive portion 16A of housing 16 and electrode 24. Conductive portion 16A is electrically isolated from electrode 20, but is electrically connected to electrode 24, such that conductive portion 16A and electrode 24 have the same polarity and are electrically common. For example, electrode 20 may be carried by second portion 16B of housing 16, which is electrically isolated from conductive portion 16A. Conduc-

tive portion 16A of housing 16 is electrically connected to at least some electronics of LPD 12 (e.g., a sensing module, an electrical stimulation module, or both), such that conductive portion 16A defines part of an electrically conductive pathway from electrode 24 to the electronics. In some examples, conductive portion 16A may define at least a part of a power source case of LPD 12. The power source case may house a power source (e.g., a battery) of LPD 12.

In some examples, conductive portion 16A is substantially completely electrically insulated (e.g., completely electrically insulated or nearly completely electrically insulated). Substantially completely electrically insulating conductive portion 16A may help a sensing module of LPD 12 sense electrical cardiac activity with electrode 24 of sensing extension 14. For example, in examples in which LPD 12 and sensing extension are implanted in a right ventricle, as shown and described with respect to FIG. 3, substantially completely electrically insulating conductive portion 16A may help electrode 24 pick-up a stronger far field P-wave. In other examples, however, at least a part of conductive portion 16A may be exposed to define one or more electrodes, which have the same polarity as electrode 24.

As shown in FIG. 2, which is a schematic cross-sectional view of sensing extension 14 and a part of that conductive portion 16A of housing 16, in some examples, conductor 26 may be coiled around conductive portion 16A to establish an electrical connection between conductor 26 and conductive portion 16A. In other examples, however, an electrical connection between conductor 26 and conductive portion 16A may be established using another configuration. For example, conductor 26 may not be coiled within sensing extension 14 and may be crimped or otherwise placed in contact with conductive portion 16A near distal end 14A of sensing extension 14.

FIG. 2 also illustrates an example electrical connection between electrode 24 and conductor 26. In particular, FIG. 2 illustrates an example in which a proximal portion of conductor 26 is welded to a distal portion of electrode 24, the distal portion including distal end 24A. In other examples, electrode 24 and conductor 26 may be electrically connected using another configuration. As shown in FIG. 2, electrode 24 may be substantially closed at a proximal end in some examples, which may help prevent fluids from entering an inner portion (e.g., where conductor 26 is positioned) of sensing extension 14.

In the example shown in FIGS. 1 and 2, self-supporting body 22 of sensing extension 14 extends between housing 16 and electrode 24. Self-supporting body 22 has a stiffness that permits body 22 to substantially maintain (e.g., completely maintain or nearly maintain) its position relative to LPD 12, or at least the position of electrode 24 relative to LPD 12, even in the presence of gravity and in the presence of blood flow in the heart. For example, self-supporting body 22 may have a bending stiffness of about $0.8 \text{ e}^{-6} \text{ N}\cdot\text{m}^2$ to about $4.8 \text{ e}^{-6} \text{ N}\cdot\text{m}^2$ (about 0.8×10^{-6} to about $4.8 \times 10^{-6} \text{ N}\cdot\text{m}^2$), such as about 1.6 Newtons-square meter ($\text{N}\cdot\text{m}^2$). In other examples, self-supporting bodies having other bending stiffness values may also be used.

Self-supporting body 22 is configured to passively position electrode 24 at a location away from LPD 12, e.g., proximate or within a chamber of the heart other than the one in which LPD 12 is implanted. For example, self-supporting body 22 may have sufficient rigidity (e.g., stiffness) to permit sensing extension 14 to extend away from housing 16, even as the sensing extension moves within blood in the chamber of the heart. In addition, self-support-

ing body 22 may be flexible enough to minimize irritation to the tissue of the heart, should body 22 contact the tissue.

In some examples, a bending stiffness of self-supporting body is substantially the same throughout the length of self-supporting body 22 (e.g., the same or nearly from a distal end to a proximal end of body 22). In other examples, self-supporting body 22 may have a variable stiffness along its length. For example, self-supporting body may decrease in stiffness from a distal end (closest to housing 16 LPD 12) to a proximal end, such that a distal portion of body 22 closest to housing 16 may have a higher stiffness than a proximal portion of body 22 closest to electrode 24 and including the proximal end. For example, the distal portion may be configured to have the highest stiffness and the proximal portion may be configured to have the lowest stiffness. A lower stiffness at the proximal portion of body 22 may help further minimize irritation to the tissue of the heart, should the proximal end of body 22 contact tissue, while the stiffer distal portion may permit body 22 to position electrode 24 at a location away from LPD 12.

In the example shown in FIGS. 1 and 2, electrical conductor 26 is covered by an electrically conductive material, such as a polymer (e.g., polyurethane) or silicone. For example, conductor 26 may be housed within a polyurethane or silicone sleeve 28, as shown in FIGS. 1 and 2. In some cases, coiled conductor 26 may not provide sufficient stiffness to sensing extension 14 to enable self-supporting body 22 to substantially maintain its position relative to LPD 12 in the presence of blood flow in the heart. Thus, in some examples, sensing extension 14 may also include a stiffness member 30, which has a higher stiffness than coiled conductor 26 (when coiled). In the example shown in FIGS. 1 and 2, self-supporting body 22 of sensing extension 14 is defined by conductor 26, sleeve 28, and stiffness member 30.

Stiffness member 30 has a stiffness that helps prevent self-supporting body 22 from collapsing in on itself and/or towards LPD 12, e.g., in the presence of blood flow. For example, in examples in which conductor 26 is coiled and is enclosed in a polyurethane or silicone sleeve, stiffness member 30 may have a stiffness that results in self-supporting body 22 having a stiffness of about $0.8 \text{ e}^{-6} \text{ N}\cdot\text{m}^2$ to about $4.8 \text{ e}^{-6} \text{ N}\cdot\text{m}^2$ (about 0.8×10^{-6} to about $4.8 \times 10^{-6} \text{ N}\cdot\text{m}^2$). The stiffness, however, for stiffness member 30 that may be suitable for providing the desired stiffness characteristics to self-supporting body 22 may depend on various factors, such as length of self-supporting body 22 and the diameter (or other cross-sectional dimensions in examples in which self-supporting body 22 has a non-circular cross-sectional shape when the cross-section is taken substantially perpendicular to a longitudinal axis) of self-supporting body 22. Stiffness member 30 may be more stiff as the length of self-supporting body 22 increases, and as the diameter of self-supporting body increases. A bigger diameter may cause the blood flow to push self-supporting body 22 around more within the heart. As with self-supporting body 22, in some examples, stiffness member 30 may also have a variable stiffness along its length or may have substantially the same stiffness along its length.

Stiffness member 30 may be formed from any suitable material non-metallic or metallic material, such as a nickel-cobalt-chromium-molybdenum alloy (e.g., MP35N, such as a 7x7 MP35N cable).

In addition, stiffness member 30 may limit the amount sensing extension 14 stretches in response to a pulling force applied to the proximal end of sensing extension 14 (the end furthest from LPD 12) during a tug test performed to confirm that LPD 12 is secured to a target tissue site, e.g., that tines

18 are securely engaged with tissue of the heart of the patient. In some examples, such as examples in which conductor 26 is coiled, conductor 26 may stretch (e.g., elongate) in response to the pulling force. However, stiffness member 30 may be configured to stretch less than conductor 26 in some examples, and, as a result, when a clinician applies a pulling force to the proximal end of sensing extension 14 (the end furthest from LPD 12) during a tug test to confirm that LPD 12 is secured to a target tissue site, stiffness member 30 may limit the amount sensing extension 14 stretches in response to the pulling relative to examples in which sensing extension 14 does not include stiffness member 30.

As shown in FIGS. 1 and 2, in some examples, stiffness member 30 extends through a center of coiled conductor 26 (e.g., conductor 26 may be coiled around member 30) and is coaxial with a longitudinal axis of sensing extension 14. In other examples however, stiffness member 30 may have another position within sensing extension 14.

In other examples, such as examples in which conductor 26 is not coiled, sensing extension 14 may not include stiffness member 30. For example, the material of sleeve 28, in combination with the conductor 26, may provide body 22 with sufficient stiffness to permit body 22 to maintain its position relative to LPD 12, even in the presence of gravity and in the presence of blood flow in the heart.

In some examples, in addition to, or instead of, electrically connecting electrode 24 to electronics of LPD 12 via electrical conductor 26, stiffening member 30 may be electrically conductive and may electrically connect electrode 24 to electronics of LPD 12. For example, a proximal portion of stiffening member 30 may be welded or otherwise electrically connected to a distal portion of electrode 24. Thus, in some examples, sensing extension 14 does not include electrical conductor 26 and stiffening member 30 may both electrically connect electrode 24 to electronics of LPD 12 and increases the stiffness of sensing extension 14, e.g., to help prevent self-supporting body 22 from collapsing in on itself and/or towards LPD 12. Stiffness member 30 may have a higher stiffness than, for example, sleeve 28. In examples in which both electrical conductor 26 and stiffening member 30 electrically connect electrode 24 to electronics of LPD 12, sensing extension 14 may provide redundant electrical pathways for electrically connecting electrode 24 to electronics of LPD 12.

In the example shown in FIGS. 1 and 2, system 10 includes retrieval member 31, which is positioned at or near the distal end of sensing extension 14, which is mechanically connected to outer housing 16 of LPD 12. Retrieval member 31 can be, for example, a bump, protrusion, or any other suitable feature that can be used to grasp system 10, e.g., when removing or implanting system 10 in a patient. For example, retrieval member 31 can be a bump configured to be grabbed by a snare. In some examples, retrieval member 31 is incorporated in a molded part used for insulating sensing extension 14, or may be formed integrally with outer housing 16. In other examples, retrieval member 31 can be separate from and attached to sensing extension 14, outer housing 16, or both.

As discussed above, sensing extension 14 is configured to position electrode 24 proximate to or within a chamber of a heart other than the one in which LPD 12 is implanted. FIG. 3 illustrates system 10 implanted in right ventricle 32 of heart 34 of patient 36. In the example shown in FIG. 3, sensing extension 14 is configured to extend away from LPD 12 and towards right atrium 38 when LPD 12 is implanted in an apex of right ventricle 32. In some examples, sensing

extension 14 may have a length that permits sensing extension 14 to remain in right ventricle 32 with LPD 12, as shown in FIG. 3. For example, sensing extension 14 may have a length of about 40 millimeters (mm) to about 150 mm, such as about 60 millimeters (as measured from the distal end connected to LPD 12 and a proximal end of electrode 24). A single chamber system 10 may provide the advantages of sensing electrical activity of two chambers (e.g., right ventricle 32 and right atrium 38 in the example shown in FIG. 3) without the burden of placing extension 14 in right atrium 38.

In examples in which extension 14 remains in the same chamber as LPD 12, a proximal portion of sensing extension 14 may be configured to help reduce interference with the mechanical movement of the heart, such as, in the example shown in FIG. 3, movement of the tricuspid valve. For example, electrode 24 at the proximal end of extension 14 may define an L-shaped curve, a C-shaped curve, a pigtail, or any other suitable curve, as shown with respect to electrodes 25A, 25B, and 25C in FIGS. 4A, 4B, and 4C, respectively. The L-shaped curve is also shown in FIG. 3.

The L-shaped curve, the C-shaped curve, and the pigtail shaped curve shown in FIGS. 4A, 4B, and 4C may define curved or relatively flat surfaces (e.g., surfaces 27A-27C) against which the tricuspid valve (or other valve in the case of other implantation sites for LPD 12) may still substantially close, which may help prevent blood from back flowing into another chamber of heart 34, e.g., right atrium 38. In some examples, the shape of proximal portion of sensing extension 14 may be selected based on the implant location for system 10. Different shapes may help reduce interference with different valves and different implantation sites for LPD 12 and sensing extension 14.

In other examples, a portion of sensing extension 14 in addition to, or other than, electrode 24 may define the shapes shown in FIGS. 4A-4C. For example, sleeve 28 and stiffness member 30 may be configured to define the proximal portion shapes shown in FIGS. 4A-4C and electrode 24 may be positioned on an outer surface of sleeve 28.

In other examples, sensing extension 14 may have a length that enables at least electrode 24 to extend into right atrium 38 when LPD 12 is implanted in an apex of right ventricle 32. In examples in which sensing extension 14 extends into right atrium 38, sensing extension 14 may be relatively small and flexible enough to permit the tricuspid valve to sufficiently close around the sensing extension 14 to prevent backflow into right atrium 38 from right ventricle 32. For example, sensing extension 14 may be about 4 French (i.e., about 1.33 millimeters in diameter).

LPD 12 may sense electrical activity of right atrium 38 or right ventricle 32 with electrodes 20, 24. As shown in FIG. 3 sensing extension 14 is passive and extends away from LPD 12, which enables electrode 24 to be positioned relatively close to right atrium 38. The distance between electrode 24 and right atrium 38 may be less than the distance between electrode 20 of LPD 12 and right atrium 38. As a result, electrode 24 may be positioned to pick up higher amplitude P-waves than electrode 20. In this way, sensing extension 14 may facilitate atrial sensing when LPD 12 is implanted in right ventricle 32.

Rather than being affixed to cardiac tissue such that electrode 24 is in direct contact with heart 34, a proximal portion of sensing extension 14 is passive, such that sensing extension 14 may move within right ventricle 32. However, due at least in part to the self-supporting configuration of body 22 (FIGS. 1 and 2), sensing extension 14 is configured to continue to extend away from LPD 12 and towards right

atrium 38, even in the presence of blood flow from right atrium 38 to right ventricle 32. Providing self-supporting member 22 of sensing extension 14 with some flexibility may enable sensing extension 14 to minimize interference with blood flow in right ventricle 32 (or another chamber if LPD 12 is implanted in another chamber).

Also shown in FIG. 3 is medical device programmer 40, which is configured to program LPD 12 and retrieve data from LPD 12. Programmer 40 may be a handheld computing device, desktop computing device, a networked computing device, etc. Programmer 40 may include a computer-readable storage medium having instructions that cause a processor of programmer 40 to provide the functions attributed to programmer 40 in the present disclosure. LPD 12 may wirelessly communicate with programmer 40. For example, LPD 12 may transfer data to programmer 40 and may receive data from programmer 40. Programmer 40 may also wirelessly program and/or wirelessly charge LPD 12.

Data retrieved from LPD 12 using programmer 40 may include cardiac EGMs stored by LPD 12 that indicate electrical activity of heart 34 and marker channel data that indicates the occurrence and timing of sensing, diagnosis, and therapy events associated with LPD 12. Data transferred to LPD 12 using programmer 40 may include, for example, operational programs for LPD 12 that causes LPD 12 to operate as described herein.

Leadless pacing system 10 may be implanted in right ventricle 32, or another chamber of heart 34, using any suitable technique. In some cases, sensing extension 14 may include a feature that helps control a position of proximal end of sensing extension 14 during implantation of system 10 in patient 36. The feature may also be used to facilitate relatively easy capture of a proximal end of sensing extension 14 by a retrieval device, e.g., during explanation of system 10 from patient 36. FIGS. 5 and 6 illustrate an example of such a feature.

FIGS. 5 and 6 illustrate an example leadless pacing system 50, which is similar to system 10 of FIG. 1, but further includes eyelet 52 at a proximal end of sensing extension 14. In other examples of the system 50, however, the sensing extension may be any suitable extension, e.g., may not include a self-supporting body, as described above with respect to FIGS. 1 and 2, may include one or more additional electrodes, which may be used for sensing or electrical stimulation, or any combination thereof.

Eyelet 52 defines an opening 54 configured to receive, e.g., a tether or another tool used during implantation, during explanation, or both implantation and explanation. A tether may, for example, a suture thread or another material that is relatively thin and flexible, compared to sensing extension 14. The tether may be looped through opening 54 prior to inserting system 10 in right ventricle 32, and, after sensing extension 14 is implanted in heart 34 (FIG. 3), a clinician may pull back on the tether in order to pull back on proximal end 14B of sensing extension 14, to move proximal end 14B of sensing extension 14, or to otherwise control the position of proximal end 14B. In addition, eyelet 52 may be configured to facilitate capture of system 10 by a retrieval device, e.g. during explanation of system 10 from the patient or to move LPD 12 to another location after tines 18 have fixed to a particular location.

Although shown to have a circular cross-section in FIGS. 5 and 6, eyelet 52 may have any suitable cross-sectional shape configured to receive a tether or other tool. In addition, although shown in FIGS. 5 and 6 to define an opening that has a center axis 53 that is transverse and substantially orthogonal (e.g., orthogonal or nearly orthogonal) to longi-

tudinal axis 15 of sensing extension 14, in other examples, center axis 53 may have another orientation relative to longitudinal axis 15. For example, the opening defined by eyelet 52 may be oriented such that center axis 53 is substantially parallel (e.g., parallel or nearly parallel) or oriented at an angle less than 90 degrees relative to longitudinal axis 15. Thus, in some examples, the opening defined by eyelet 52 may be oriented such that center axis 53 is 90 degrees or less relative to longitudinal axis 15.

In addition, in some examples, center axis 53 may not be aligned with longitudinal axis 53, but, rather, eyelet 52 may extend away from a side surface of extension 14. In FIGS. 5 and 6, center axis 53 is aligned with longitudinal axis 53. However, if, for example, sensing extension 14 defines a curved proximal portion (e.g., as shown in FIGS. 4A-4C), center axis 53 may not be aligned with longitudinal axis 53.

Eyelet 52 may be mechanically connected to sensing extension 14 using any suitable technique. In the example shown in FIGS. 5 and 6, eyelet 52 includes base portion 56 that is received in cavity 58 defined by electrode 24. Electrode 24 and base portion 56 may be attached using any suitable technique, such as by crimping electrode 24 around base portion 56, via an adhesive, welding, or another suitable technique. The attachment between sensing extension 14 and eyelet 52 is strong enough to maintain the mechanical connection between eyelet 52 and sensing extension 14, even in the presence of forces (e.g., from a tether or other retrieval tool) pulling the eyelet 52 in a direction away from sensing extension 14. Likewise, the attachment between LPD 12 and sensing extension 14 is strong enough to maintain the mechanical connection between LPD 12 and sensing extension 14, even in the presence of forces pulling the sensing extension 14 and LPD 12 away from each other.

In some examples, end 58A of cavity 58 may be closed (i.e., cavity 58 may be a blind hole), which may help prevent environmental contaminants from being introduced into the portion of sensing extension 14 including conductor 26.

Eyelet 52 may be formed from any suitable material. In some examples, eyelet 52 is formed from an electrically nonconductive material. In other examples, eyelet 52 is formed from an electrically conductive material. In some examples in which eyelet 52 is formed from an electrically conductive material, eyelet is configured to function as an extension of electrode 24. Thus, LPD 12 may sense electrical cardiac signals and deliver electrical stimulation with the aid of eyelet 52. Eyelet 52 may be electrically connected to electrode 24 by virtue of being in contact with electrode 24. In other examples in which eyelet 52 is formed from an electrically conductive material, the conductivity of eyelet 52 may be relatively low when compared to the conductivity of electrode 24 for eyelet 52 to function as an extension of electrode 24. For example, eyelet 52 may be formed from stainless steel. In addition, eyelet 52 is configured to not be in contact with cardiac tissue when system 10 is implanted in a patient, e.g., sensing extension is configured to position eyelet not in contact with cardiac tissue, such that eyelet 52 may not function as a stimulation electrode.

Base portion 56 of eyelet 52 is shown in FIGS. 5 and 6 as being coaxial with a longitudinal axis of sensing extension 14, in some examples, base portion 56 may have another arrangement relative to the longitudinal axis of sensing extension 14. For example, in examples in which a proximal portion of extension 14 defines a curve (e.g., as shown in FIGS. 4A-4C), when eyelet 52 is positioned at a proximal end of sensing extension 14, base portion 56 may curve with the proximal portion. As another example, base portion 56 may be curvilinear or otherwise nonlinear (e.g., may define

a 90 degree angle) and attached to sensing extension 14 such that base portion 56 extends away from electrode 24. Other configurations of eyelet 52 may also be used.

Eyelet 52 provides a feature for controlling a positioning of extension 52, as well as a feature that facilitates retrieval of system 50 from an implant site. These features may be useful with other type of extensions that are connected to electronics of LPD 12 (e.g., a stimulation module, a sensing module, or both). Thus, in some examples, system 50 may include an extension having a configuration different than sensing extension 14, the extension including eyelet 52 at a proximal end. For example, in FIGS. 5 and 6, rather than being connected to sensing extension 14 including electrode 24 electrically connected to conductive portion 16A of housing 16 of LPD 12, LPD 12 may be mechanically connected to an extension that includes multiple electrodes electrically connected to conductive portion 16A of housing 16, and the extension may extend away from housing 16 of LPD 12 and include eyelet 52 at a proximal end (similar to the position shown in FIG. 5).

As another example, LPD 12 may be mechanically connected to an extension that includes one or more electrodes that are not electrically connected to conductive portion 16A of housing 16, but, rather, connected to electronics (e.g., a sensing module and a stimulation module) of LPD 12 using another conductive path, such as a conductive feedthrough that extends through housing 16; in this example, eyelet 52 may be positioned at a proximal end of the extension, which may also extend away from housing 16. As yet another example, LPD 12 may be mechanically connected to an extension that is not self-supporting and/or includes one or more fixation elements. In these examples, eyelet 52 may be positioned at a proximal end of the extension. Other configurations of extensions including eyelet 52 are also contemplated.

In other examples of system 50, sense electrode 24 and eyelet 52 may be integrated into a common, integral component. FIGS. 7-9 illustrate an example of such a sensing extension. FIG. 7 is a perspective view of example sensing extension 60, which may be similar to sensing extension 14 of FIGS. 5 and 6, but includes sense electrode 62 defining electrode portion 64 and eyelet portion 66 instead of sense electrode 24 and eyelet 52. FIG. 8 is a cross-sectional perspective view of sensing extension 60 and illustrates self-supporting body 22, electrical conductor 26, stiffness member 30, and sense electrode 62. FIG. 9 is an exploded perspective view of sensing extension 60.

As shown in FIGS. 7-9, electrode portion 64 and eyelet portion 66 are continuous and are portions of a common body of sense electrode 62, rather than being separate components that are attached together. In contrast, sense electrode 24 and eyelet 52 shown in FIGS. 5 and 6 are separate components. Eyelet portion 66 is configured similarly to eyelet 52 and defines an opening 68 configured to receive, e.g., a tether or another tool used during implantation, during explanation, or both implantation and explanation.

Electrode 62 including integral electrode portion 64 and eyelet portion 66 may minimize the number of openings through which a fluid may enter an inner portion (e.g., where conductor 26 is positioned) of sensing extension 60.

Electrode 62 may be formed using any suitable technique. In some examples, electrode 62 may be produced with a cold-heading operation that defines a metal or other suitable electrically conductive material into the shape of electrode 62. In some examples, after forming the shape of electrode 62, eyelet portion 66 may be polished. All or only a part of

electrode 62 may be electrically conductive. For example, in some examples, both electrode portion 64 and eyelet portion 66 are electrically conductive, though they may have different impedances, while in other examples, eyelet portion 66 is not electrically conductive and electrode portion 64 is electrically conductive. In some examples, to form electrode 62 including eyelet portion 66 that is not electrically conductive, eyelet portion 66 may be masked during the coating of electrode portion 62 with an electrically conductive material, such as titanium nitride (TiN).

As with electrode 24, sense electrode 62 may be electrically connected to electrical conductor 26, stiffness member 30, or both stiffness member 30 and electrical conductor 26 using any suitable technique, such as the ones described above with respect to electrode 24. For example, a proximal portion of conductor 26 or stiffness member 30 may be welded or crimped to a distal portion of electrode 62.

Electrode 62 may define a distal portion 62A that is configured to be received in self-supporting body 22. In addition, in some examples, as shown in FIG. 9, distal portion 62A may define an opening configured to receive stiffness member 30, such that stiffness member 30 and electrode 60 are partially co-extensive, e.g., overlap in a longitudinal direction. In other examples, however, stiffness member 30 and electrode 60 may not be co-extensive. Electrode 60 may, for example, provide sufficient stiffness to the proximal end of sensing extension 60 without stiffness member 30.

Electrode 62 may be mechanically connected to self-supporting body 22 using any suitable technique, such as by a friction fit achieved when distal portion 62A of electrode 62 is received in proximal end 22B of self-supporting body 22, by ultrasonic welding, by an adhesive, or any other suitable technique or combinations of techniques. The mechanical connection may define a relatively fluid tight seal between electrode 62 and self-supporting body 22 to help prevent the ingress of fluids into self-supporting body 22.

In each of the examples described herein, stiffness member 30 may comprise one or more elements. For example, in the example shown in FIG. 9, stiffness member 30 includes three members that are substantially co-axial. Using two or more elements to form stiffness member 30 may provide design freedom for achieving the desired stiffness of stiffness member 30 than, for example, one element.

FIG. 10 is a functional block diagram of an example LPD 12. LPD 12 includes a processing module 70, memory 72, stimulation module 74, electrical sensing module 76, communication module 78, sensor 80, and power source 82. Power source 82 may include a battery, e.g., a rechargeable or non-rechargeable battery.

Modules included in LPD 12 represent functionality that may be included in LPD 12 of the present disclosure. Modules of the present disclosure may include any discrete and/or integrated electronic circuit components that implement analog and/or digital circuits capable of producing the functions attributed to the modules herein. For example, the modules may include analog circuits, e.g., amplification circuits, filtering circuits, and/or other signal conditioning circuits. The modules may also include digital circuits, e.g., combinational or sequential logic circuits, memory devices, and the like. The functions attributed to the modules herein may be embodied as one or more processors, hardware, firmware, software, or any combination thereof. Depiction of different features as modules is intended to highlight different functional aspects, and does not necessarily imply that such modules must be realized by separate hardware or

software components. Rather, functionality associated with one or more modules may be performed by separate hardware or software components, or integrated within common or separate hardware or software components.

Processing module 70 may include any one or more of a microprocessor, a controller, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field-programmable gate array (FPGA), or equivalent discrete or integrated logic circuitry. In some examples, processing module 70 may include multiple components, such as any combination of one or more microprocessors, one or more controllers, one or more DSPs, one or more ASICs, or one or more FPGAs, as well as other discrete or integrated logic circuitry.

Processing module 70 may communicate with memory 72. Memory 72 may include computer-readable instructions that, when executed by processing module 70, cause processing module 70 to perform the various functions attributed to processing module 70 herein. Memory 72 may include any volatile, non-volatile, magnetic, or electrical media, such as a random access memory (RAM), read-only memory (ROM), non-volatile RAM (NVRAM), electrically-erasable programmable ROM (EEPROM), Flash memory, or any other memory device. Furthermore, memory 72 may include instructions that, when executed by one or more processors, cause the modules to perform various functions attributed to the modules herein. For example, memory 72 may include pacing instructions and values. The pacing instructions and values may be updated by programmer 40 (FIG. 3).

Stimulation module 74 and electrical sensing module 76 are electrically coupled to electrodes 20, 24. Processing module 70 is configured to control stimulation module 74 to generate and deliver electrical stimulation to heart 34 (e.g., right ventricle 32 in the example shown in FIG. 3) via electrodes 20, 24. Electrical stimulation may include, for example, pacing pulses, or any other suitable electrical stimulation. Processing module 70 may control stimulation module 74 to deliver electrical stimulation therapy via electrodes 20, 24 according to one or more therapy programs including pacing instructions that define a ventricular pacing rate, which may be stored in memory 72.

In addition, processing module 70 is configured to control electrical sensing module 76 monitor signals from electrodes 20, 24 in order to monitor electrical activity of heart 34. Electrical sensing module 76 may include circuits that acquire electrical signals. Electrical signals acquired by electrical sensing module 76 may include intrinsic cardiac electrical activity, such as intrinsic atrial depolarization and/or intrinsic ventricular depolarization. Electrical sensing module 76 may filter, amplify, and digitize the acquired electrical signals to generate raw digital data. Processing module 70 may receive the digitized data generated by electrical sensing module 76. In some examples, processing module 70 may perform various digital signal processing operations on the raw data, such as digital filtering.

Processing module 70 may sense cardiac events based on the data received from electrical sensing module 76. For example, processing module 70 may sense atrial electrical activity based on the data received from electrical sensing module 76. For example, in examples in which LPD 12 and sensing extension 14 are implanted in right ventricle 32, processing module 70 may detect far field P-waves indicative of atrial activation events based on the data received from electrical sensing module 76. In some examples, processing module 70 may also sense ventricular electrical activity based on the data received from electrical sensing

module 76. For example, processing module 70 may detect R-waves indicative of ventricular activation events based on the data received from electrical sensing module 76. In examples in which processor 70 uses both electrodes 20 and 24 for both R-wave and P-wave sensing, processor 70 may detect the R-waves and P-waves from the same sensed signal, and the sensing vector can be between electrodes 20, 24.

In some examples, in addition to electrical sensing module 76, LPD 12 includes sensor 80, which may comprise at least one of a variety of different sensors. For example, sensor 80 may comprise at least one of a pressure sensor and an accelerometer. Sensor 80 may generate signals that indicate at least one of parameter of patient 12, such as, but not limited to, at least one of: an activity level of patient 36, a hemodynamic pressure, and heart sounds.

Communication module 78 may include any suitable hardware (e.g., an antenna), firmware, software, or any combination thereof for communicating with another device, such as programmer 40 (FIG. 3) or a patient monitor. Under the control of processing module 70, communication module 78 may receive downlink telemetry from and send uplink telemetry to other devices, such as programmer 40 or a patient monitor, with the aid of an antenna included in communication module 78.

FIG. 11 is a flow diagram of an example technique performed by leadless pacing system 10. While FIG. 11 is described as primarily being performed by processing module 70 of LPD 12, in other examples, another processor (e.g., a processor of programmer 40), alone or with the aid of processing module 70, may perform any part of the technique shown in FIG. 11. In addition, while the technique is described with reference to an example in which LPD 12 is implanted in right ventricle 32 (FIG. 3), the technique shown in FIG. 11 may also be used with other examples.

In accordance with the example shown in FIG. 11, processing module 70 controls stimulation module 74 to generate and deliver pacing pulses to right ventricle 32 via electrodes 20, 24 (90). For example, electrode 20 may be selected as a source electrode and electrode 24 may be selected as the sink electrode. Processing module 70 also controls electrical sensing module 76 (FIG. 10) to sense electrical cardiac activity with electrodes 20, 24 (92). The electrical cardiac activity can be, for example, any combination of the following: intrinsic ventricular depolarization, intrinsic atrial depolarization, other ventricular activation events (e.g., paced events), or other atrial activation events (e.g., paced events). Processing module 70 may receive sensed electrical cardiac signals from sensing module 76 and detect atrial depolarization by at least detecting a far field P-wave. In some examples, processing module 70 controls electrical sensing module 76 (FIG. 10) to sense electrical cardiac activity with electrodes 20, 24 during a refractory period of heart 34.

The techniques described in this disclosure, including those attributed to image IMD 16, programmer 24, or various constituent components, may be implemented, at least in part, in hardware, software, firmware or any combination thereof. For example, various aspects of the techniques may be implemented within one or more processors, including one or more microprocessors, DSPs, ASICs, FPGAs, or any other equivalent integrated or discrete logic circuitry, as well as any combinations of such components, embodied in programmers, such as physician or patient programmers, stimulators, image processing devices or other devices. The term "processor" or "processing circuitry" may generally refer to any of the foregoing logic

circuitry, alone or in combination with other logic circuitry, or any other equivalent circuitry.

Such hardware, software, firmware may be implemented within the same device or within separate devices to support the various operations and functions described in this disclosure. In addition, any of the described units, modules or components may be implemented together or separately as discrete but interoperable logic devices. Depiction of different features as modules or units is intended to highlight different functional aspects and does not necessarily imply that such modules or units must be realized by separate hardware or software components. Rather, functionality associated with one or more modules or units may be performed by separate hardware or software components, or integrated within common or separate hardware or software components.

When implemented in software, the functionality ascribed to the systems, devices and techniques described in this disclosure may be embodied as instructions on a computer-readable medium such as RAM, ROM, NVRAM, EEPROM, FLASH memory, magnetic data storage media, optical data storage media, or the like. The instructions may be executed to support one or more aspects of the functionality described in this disclosure.

Various examples have been described. These and other examples are within the scope of the following claims.

What is claimed is:

1. A system comprising:

a leadless pacing device comprising:

a stimulation module configured to generate pacing pulses;

a sensing module;

a processing module;

a housing comprising a conductive portion, wherein the housing is configured to be implanted within a chamber of a heart of a patient and encloses the stimulation module, the sensing module, and the processing module; and

a first electrode electrically coupled to the sensing module and the stimulation module; and

a sensing extension extending from the housing, a proximal-most portion of the sensing extension being curved, the sensing extension comprising:

a self-supporting body extending from the housing; and

a second electrode carried by the self-supporting body at the proximal-most portion of the sensing extension that is curved, wherein the second electrode is electrically connected to the sensing module and the stimulation module via the conductive portion of the housing,

wherein the processing module is configured to control the sensing module to sense electrical cardiac activity via the second electrode.

2. The system of claim 1, further comprising an eyelet at a proximal end of the sensing extension.

3. The system of claim 2, wherein the second electrode defines a blind hole configured to receive the eyelet.

4. The system of claim 1, wherein the sensing extension further comprises an electrical conductor electrically connecting the second electrode to the conductive portion of the housing.

5. The system of claim 1, wherein the self-supporting body has a stiffness of about 1.6×10^{-6} Newtons-square meter.

6. The system of claim 1, wherein the self-supporting body has a stiffness of about 0.8×10^{-6} Newtons-square meter ($\text{N}\cdot\text{m}^2$) to about 4.8×10^{-6} $\text{N}\cdot\text{m}^2$.

7. The system of claim 6, wherein the self-supporting body further comprises:

a stiffness member;

an electrically insulative sleeve; and

a coiled conductor within the electrically insulative sheath, the coiled conductor being electrically connected to the second electrode and coiled around the stiffness member.

8. The system of claim 1, wherein a stiffness of the self-supporting body is substantially the same along a length of the self-supporting body.

9. The system of claim 1, wherein a stiffness of the self-supporting body varies along a length of the self-supporting body.

10. The system of claim 1, wherein the sensing extension is configured to remain in the chamber of the heart when the leadless pacing device is implanted in the chamber of the heart.

11. The system of claim 10, wherein the chamber comprises a right ventricle, and wherein the sensing extension is configured to extend from the leadless pacing device towards the right atrium when the leadless pacing device is implanted in an apex of the right ventricle.

12. The system of claim 1, wherein the sensing extension is configured such that the second electrode is located outside a chamber of the heart in which the leadless pacing device resides when the leadless pacing device is implanted in the chamber of the heart.

13. The system of claim 12, wherein the sensing extension is configured such that the second electrode is located in the right atrium of the heart when the leadless pacing device resides in the right ventricle.

14. The system of claim 1, wherein the conductive portion comprises a first conductive portion, the housing further comprising a second conductive portion electrically isolated from the first conductive portion, wherein the first electrode is defined by the second conductive portion.

15. The system of claim 1, wherein the leadless pacing device further comprises a battery and the housing comprises a battery case, and wherein the battery case includes the conductive portion.

16. The system of claim 1, wherein the conductive portion of the housing is substantially completely electrically insulated.

17. The system of claim 1, further comprising an electrically insulative layer over the conductive portion of the housing, wherein the electrically insulative layer exposes a section of the conductive portion of the housing, the section defining a third electrode electrically common with the second electrode.

18. The system of claim 1, wherein the self-supporting body is devoid of any fixation elements.

19. The system of claim 1, wherein the proximal-most portion of the sensing extension defines one of a C-shape, an L-shape, or a pigtail shape.

20. A method comprising:

controlling, by a processor, a stimulation module of a leadless pacing device to deliver a pacing pulse to a patient, the leadless pacing device comprising:

the stimulation module;

a sensing module;

the processor;

a housing comprising a conductive portion, wherein the housing is configured to be implanted within a chamber of a heart of a patient and encloses the stimulation module, the sensing module, and the processor; and

a first electrode electrically coupled to the sensing module and the stimulation module; and
controlling, by the processor, the sensing module of the leadless pacing device to sense electrical cardiac activity via the first electrode and a second electrode of a sensing extension that extends from the housing, a proximal-most portion of the sensing extension being curved, the sensing extension further comprising:
a self-supporting body extending from the housing; and the second electrode carried by the self-supporting body at the proximal-most portion of the sensing extension that is curved, wherein the second electrode is electrically connected to the sensing module and the stimulation module via the conductive portion of the housing.

21. The method of claim **20**, further comprising detecting, by the processor, atrial activity based on the sensed electrical cardiac activity, the atrial activity comprising a far-field P-wave.

* * * * *

专利名称(译)	无铅起搏系统，包括感应扩展		
公开(公告)号	US10674928	公开(公告)日	2020-06-09
申请号	US14/694910	申请日	2015-04-23
[标]申请(专利权)人(译)	美敦力公司		
申请(专利权)人(译)	美敦力公司，INC.		
当前申请(专利权)人(译)	美敦力公司，INC.		
[标]发明人	ANDERSON THOMAS A SHELDON TODD J BONNER MATTHEW D NEAFUS NOELLE C		
发明人	ANDERSON, THOMAS A SHELDON, TODD J BONNER, MATTHEW D NEAFUS, NOELLE C		
IPC分类号	A61N1/362 A61N1/368 A61B5/00 A61B5/042 A61N1/372 A61B5/0452 A61N1/375 A61N1/05		
CPC分类号	A61B5/0422 A61B5/0452 A61N1/362 A61B5/686 A61N1/37205 A61N1/3756 A61N1/368 A61N1/056		
优先权	62/025690 2014-07-17 US		
其他公开文献	US20160015322A1		
外部链接	Espacenet		

摘要(译)

无铅起搏系统包括无铅起搏装置和从无铅起搏装置的壳体延伸的感测延伸部。感测延伸部包括一个或多个电极，无铅起搏设备可利用该电极感测心脏的电活动。感测延伸部的一个或多个电极可以由自支撑体承载，该自支撑体被配置为将一个或多个电极被动地定位在除了LPD所植入的腔室之外的腔室附近或心脏内。

