



US010231670B2

(12) **United States Patent**
Blank et al.

(10) **Patent No.:** **US 10,231,670 B2**
(45) **Date of Patent:** **Mar. 19, 2019**

(54) **PROXIMITY SENSOR IN PULSE OXIMETER**

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(72) Inventors: **Thomas B. Blank**, Laguna Beach, CA (US); **Gregory A. Olsen**, Lake Forest, CA (US); **Cristiano Dalvi**, Lake Forest, CA (US); **Hung T. Vo**, Fountain Valley, CA (US)

(73) Assignee: **MASIMO CORPORATION**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 422 days.

(21) Appl. No.: **14/743,479**

(22) Filed: **Jun. 18, 2015**

(65) **Prior Publication Data**

US 2015/0366507 A1 Dec. 24, 2015

Related U.S. Application Data

(60) Provisional application No. 62/014,611, filed on Jun. 19, 2014.

(51) **Int. Cl.**

A61B 5/00 (2006.01)

A61B 5/1455 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/6844** (2013.01); **A61B 5/14552** (2013.01); **A61B 5/684** (2013.01); **A61B 5/6826** (2013.01); **A61B 2562/0257** (2013.01)

(58) **Field of Classification Search**

CPC . **A61B 5/6826**; **A61B 5/6844**; **A61B 5/14552**; **A61B 2562/0257**

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,960,128 A	10/1990	Gordon et al.
4,964,408 A	10/1990	Hink et al.
5,041,187 A	8/1991	Hink et al.
5,069,213 A	12/1991	Polczynski
5,163,438 A	11/1992	Gordon et al.
5,319,355 A	6/1994	Russek
5,337,744 A	8/1994	Branigan
5,341,805 A	8/1994	Stavridi et al.
D353,195 S	12/1994	Savage et al.
D353,196 S	12/1994	Savage et al.
5,377,676 A	1/1995	Vari et al.
D359,546 S	6/1995	Savage et al.
5,431,170 A	7/1995	Mathews
D361,840 S	8/1995	Savage et al.
D362,063 S	9/1995	Savage et al.
5,452,717 A	9/1995	Branigan et al.

(Continued)

Primary Examiner — Thaddeus B Cox


(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP

(57)

ABSTRACT

Systems and methods are disclosed for proximity sensing in physiological sensors, and more specifically to using one or more proximity sensors located on or within a physiological sensor to determine the positioning of the physiological sensor on a patient measurement site. Accurate placement of a physiological sensor on the patient measurement site is a key factor in obtaining reliable measurement of physiological parameters of the patient. Proper alignment between a measurement site and a sensor optical assembly provides more accurate physiological measurement data. This alignment can be determined based on data from a proximity sensor or sensors placed on or within the physiological sensor.

18 Claims, 11 Drawing Sheets

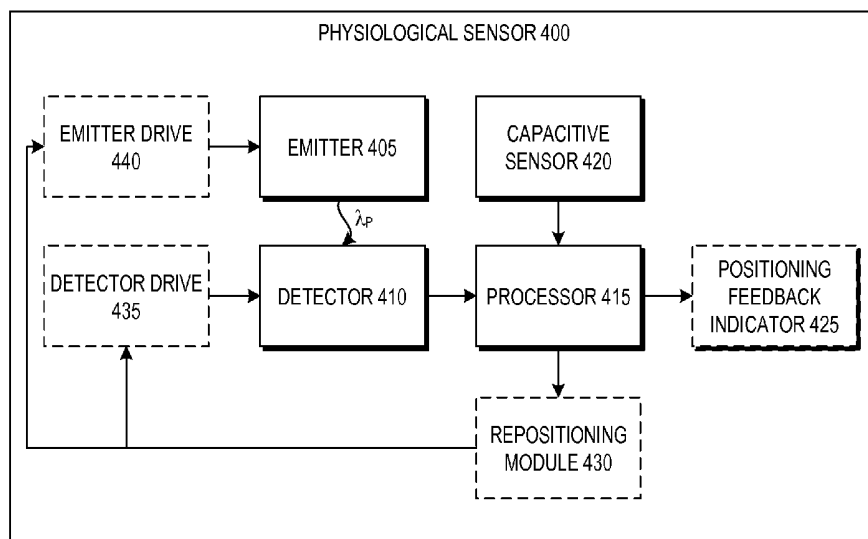

(56)

References Cited

U.S. PATENT DOCUMENTS

D363,120 S	10/1995	Savage et al.	6,360,114 B1	3/2002	Diab et al.
5,456,252 A	10/1995	Vari et al.	6,368,283 B1	4/2002	Xu et al.
5,479,934 A	1/1996	Imran	6,371,921 B1	4/2002	Caro et al.
5,482,036 A	1/1996	Diab et al.	6,377,829 B1	4/2002	Al-Ali
5,490,505 A	2/1996	Diab et al.	6,388,240 B2	5/2002	Schulz et al.
5,494,043 A	2/1996	O'Sullivan et al.	6,397,091 B2	5/2002	Diab et al.
5,533,511 A	7/1996	Kaspari et al.	6,430,437 B1	8/2002	Marro
5,534,851 A	7/1996	Russek	6,430,525 B1	8/2002	Weber et al.
5,561,275 A	10/1996	Savage et al.	6,463,311 B1	10/2002	Diab
5,562,002 A	10/1996	Lalin	6,470,199 B1	10/2002	Kopotic et al.
5,590,649 A	1/1997	Caro et al.	6,501,975 B2	12/2002	Diab et al.
5,602,924 A	2/1997	Durand et al.	6,505,059 B1	1/2003	Kollias et al.
5,632,272 A	5/1997	Diab et al.	6,515,273 B2	2/2003	Al-Ali
5,638,818 A	6/1997	Diab et al.	6,519,487 B1	2/2003	Parker
5,638,816 A	7/1997	Kiani-Azarbayjany et al.	6,525,386 B1	2/2003	Mills et al.
5,645,440 A	7/1997	Tobler et al.	6,526,300 B1	2/2003	Kiani et al.
5,685,299 A	11/1997	Diab et al.	6,541,756 B2	4/2003	Schulz et al.
D393,830 S	4/1998	Tobler et al.	6,542,764 B1	4/2003	Al-Ali et al.
5,743,262 A	4/1998	Lepper, Jr. et al.	6,580,086 B1	6/2003	Schulz et al.
5,758,644 A	6/1998	Diab et al.	6,584,336 B1	6/2003	Ali et al.
5,760,910 A	6/1998	Lepper, Jr. et al.	6,595,316 B2	7/2003	Cybulski et al.
5,769,785 A	6/1998	Diab et al.	6,597,932 B2	7/2003	Tian et al.
5,782,757 A	7/1998	Diab et al.	6,597,933 B2	7/2003	Kiani et al.
5,785,659 A	7/1998	Caro et al.	6,606,511 B1	8/2003	Ali et al.
5,791,347 A	8/1998	Flaherty et al.	6,632,181 B2	10/2003	Flaherty et al.
5,810,734 A	9/1998	Caro et al.	6,639,668 B1	10/2003	Trepagnier
5,823,950 A	10/1998	Diab et al.	6,640,116 B2	10/2003	Diab
5,830,131 A	11/1998	Caro et al.	6,643,530 B2	11/2003	Diab et al.
5,833,618 A	11/1998	Caro et al.	6,650,917 B2	11/2003	Diab et al.
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	6,654,624 B2	11/2003	Diab et al.
5,890,929 A	4/1999	Mills et al.	6,658,276 B2	12/2003	Kiani et al.
5,904,654 A	5/1999	Wohltmann et al.	6,661,161 B1	12/2003	Lanzo et al.
5,919,134 A	7/1999	Diab	6,671,528 B2 *	12/2003	Steuer A61B 5/14535 600/322
5,934,925 A	8/1999	Tobler et al.	6,671,531 B2	12/2003	Al-Ali et al.
5,940,182 A	8/1999	Lepper, Jr. et al.	6,678,543 B2	1/2004	Diab et al.
5,987,343 A	11/1999	Kinast	6,684,090 B2	1/2004	Ali et al.
5,995,855 A	11/1999	Kiani et al.	6,684,091 B2	1/2004	Parker
5,997,343 A	12/1999	Mills et al.	6,697,656 B1	2/2004	Al-Ali
6,002,952 A	12/1999	Diab et al.	6,697,657 B1	2/2004	Shehada et al.
6,011,986 A	1/2000	Diab et al.	6,697,658 B2	2/2004	Al-Ali
6,027,452 A	2/2000	Flaherty et al.	RE38,476 E	3/2004	Diab et al.
6,036,642 A	3/2000	Diab et al.	6,699,194 B1	3/2004	Diab et al.
6,045,509 A	4/2000	Caro et al.	6,714,804 B2	3/2004	Al-Ali et al.
6,067,462 A	5/2000	Diab et al.	RE38,492 E	4/2004	Diab et al.
6,081,735 A	6/2000	Diab et al.	6,721,582 B2	4/2004	Trepagnier et al.
6,088,607 A	7/2000	Diab et al.	6,721,585 B1	4/2004	Parker
6,110,522 A	8/2000	Lepper, Jr. et al.	6,725,075 B2	4/2004	Al-Ali
6,124,597 A	9/2000	Shehada	6,728,560 B2	4/2004	Kollias et al.
6,128,521 A	10/2000	Marro et al.	6,735,459 B2	5/2004	Parker
6,129,675 A	10/2000	Jay	6,745,060 B2	6/2004	Diab et al.
6,144,868 A	11/2000	Parker	6,760,607 B2	7/2004	Al-Ali
6,151,516 A	11/2000	Kiani-Azarbayjany et al.	6,770,028 B1	8/2004	Ali et al.
6,152,754 A	11/2000	Gerhardt et al.	6,771,994 B2	8/2004	Kiani et al.
6,157,850 A	12/2000	Diab et al.	6,792,300 B1	9/2004	Diab et al.
6,165,005 A	12/2000	Mills et al.	6,813,511 B2	11/2004	Diab et al.
6,184,521 B1	2/2001	Coffin, IV et al.	6,816,741 B2	11/2004	Diab
6,206,830 B1	3/2001	Diab et al.	6,822,564 B2	11/2004	Al-Ali
6,229,856 B1	5/2001	Diab et al.	6,826,419 B2	11/2004	Diab et al.
6,232,609 B1	5/2001	Snyder et al.	6,830,711 B2	12/2004	Mills et al.
6,236,872 B1	5/2001	Diab et al.	6,850,787 B2	2/2005	Weber et al.
6,241,683 B1	6/2001	Macklem et al.	6,850,788 B2	2/2005	Al-Ali
6,253,097 B1	6/2001	Aronow et al.	6,852,083 B2	2/2005	Caro et al.
6,256,523 B1	7/2001	Diab et al.	6,861,639 B2	3/2005	Al-Ali
6,263,222 B1	7/2001	Diab et al.	6,898,452 B2	5/2005	Al-Ali et al.
6,278,522 B1	8/2001	Lepper, Jr. et al.	6,920,345 B2	7/2005	Al-Ali et al.
6,280,213 B1	8/2001	Tobler et al.	6,931,268 B1	8/2005	Kiani-Azarbayjany et al.
6,285,896 B1	9/2001	Tobler et al.	6,934,570 B2	8/2005	Kiani et al.
6,301,493 B1	10/2001	Marro et al.	6,939,305 B2	9/2005	Flaherty et al.
6,308,089 B1	10/2001	von der Ruhr et al.	6,943,348 B1	9/2005	Coffin, IV
6,317,627 B1	11/2001	Ennen et al.	6,950,687 B2	9/2005	Al-Ali
6,321,100 B1	11/2001	Parker	6,961,598 B2	11/2005	Diab
6,325,761 B1	12/2001	Jay	6,970,792 B1	11/2005	Diab
6,334,065 B1	12/2001	Al-Ali et al.	6,979,812 B2	12/2005	Al-Ali
6,343,224 B1	1/2002	Parker	6,985,764 B2	1/2006	Mason et al.
6,349,228 B1	2/2002	Kiani et al.	6,993,371 B2	1/2006	Kiani et al.
			6,996,427 B2	2/2006	Ali et al.
			6,999,904 B2	2/2006	Weber et al.
			7,003,338 B2	2/2006	Weber et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,003,339 B2	2/2006	Diab et al.	7,530,955 B2	5/2009	Diab et al.
7,015,451 B2	3/2006	Dalke et al.	7,563,110 B2	7/2009	Al-Ali et al.
7,024,233 B2	4/2006	Ali et al.	7,596,398 B2	9/2009	Al-Ali et al.
7,027,849 B2	4/2006	Al-Ali	7,618,375 B2	11/2009	Flaherty
7,030,749 B2	4/2006	Al-Ali	D606,659 S	12/2009	Kiani et al.
7,039,449 B2	5/2006	Al-Ali	7,647,083 B2	1/2010	Al-Ali et al.
7,041,060 B2	5/2006	Flaherty et al.	D609,193 S	2/2010	Al-Ali et al.
7,044,918 B2	5/2006	Diab	D614,305 S	4/2010	Al-Ali et al.
7,048,687 B1	5/2006	Reuss et al.	RE41,317 E	5/2010	Parker
7,067,893 B2	6/2006	Mills et al.	7,729,733 B2	6/2010	Al-Ali et al.
7,096,052 B2	8/2006	Mason et al.	7,734,320 B2	6/2010	Al-Ali
7,096,054 B2	8/2006	Abdul-Hafiz et al.	7,761,127 B2	7/2010	Al-Ali et al.
7,132,641 B2	11/2006	Schulz et al.	7,761,128 B2	7/2010	Al-Ali et al.
7,142,901 B2	11/2006	Kiani et al.	7,764,982 B2	7/2010	Dalke et al.
7,149,561 B2	12/2006	Diab	D621,516 S	8/2010	Kiani et al.
7,186,966 B2	3/2007	Al-Ali	7,791,155 B2	9/2010	Diab
7,190,261 B2	3/2007	Al-Ali	7,801,581 B2	9/2010	Diab
7,215,984 B2	5/2007	Diab	7,822,452 B2	10/2010	Schurman et al.
7,215,986 B2	5/2007	Diab	RE41,912 E	11/2010	Parker
7,221,971 B2	5/2007	Diab	7,844,313 B2	11/2010	Kiani et al.
7,225,006 B2	5/2007	Al-Ali et al.	7,844,314 B2	11/2010	Al-Ali
7,225,007 B2	5/2007	Al-Ali	7,844,315 B2	11/2010	Al-Ali
RE39,672 E	6/2007	Shehada et al.	7,865,222 B2	1/2011	Weber et al.
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	7,873,497 B2	1/2011	Weber et al.
7,245,953 B1	7/2007	Parker	7,880,606 B2	2/2011	Al-Ali
7,254,429 B2	8/2007	Schurman et al.	7,880,626 B2	2/2011	Al-Ali et al.
7,254,431 B2	8/2007	Al-Ali	7,891,355 B2	2/2011	Al-Ali et al.
7,254,433 B2	8/2007	Diab et al.	7,894,868 B2	2/2011	Al-Ali et al.
7,254,434 B2	8/2007	Schulz et al.	7,899,507 B2	3/2011	Al-Ali et al.
7,272,425 B2	9/2007	Al-Ali	7,899,518 B2	3/2011	Trepagnier et al.
7,274,955 B2	9/2007	Kiani et al.	7,904,132 B2	3/2011	Weber et al.
D554,263 S	10/2007	Al-Ali	7,909,772 B2	3/2011	Popov et al.
7,280,858 B2	10/2007	Al-Ali et al.	7,910,875 B2	3/2011	Al-Ali
7,289,835 B2	10/2007	Mansfield et al.	7,919,713 B2	4/2011	Al-Ali et al.
7,292,883 B2	11/2007	De Felice et al.	7,937,128 B2	5/2011	Al-Ali
7,295,866 B2	11/2007	Al-Ali	7,937,129 B2	5/2011	Mason et al.
7,328,053 B1	2/2008	Diab et al.	7,937,130 B2	5/2011	Diab et al.
7,332,784 B2	2/2008	Mills et al.	7,941,199 B2	5/2011	Kiani
7,340,287 B2	3/2008	Mason et al.	7,951,086 B2	5/2011	Flaherty et al.
7,341,559 B2	3/2008	Schulz et al.	7,957,780 B2	6/2011	Lamego et al.
7,343,186 B2	3/2008	Lamego et al.	7,962,188 B2	6/2011	Kiani et al.
D566,282 S	4/2008	Al-Ali et al.	7,962,190 B1	6/2011	Diab et al.
7,355,512 B1	4/2008	Al-Ali	7,976,472 B2	7/2011	Kiani
7,356,365 B2	4/2008	Schurman	7,988,637 B2	8/2011	Diab
7,371,981 B2	5/2008	Abdul-Hafiz	7,990,382 B2	8/2011	Kiani
7,373,193 B2	5/2008	Al-Ali et al.	7,991,446 B2	8/2011	Al-Ali et al.
7,373,194 B2	5/2008	Weber et al.	8,000,761 B2	8/2011	Al-Ali
7,376,453 B1	5/2008	Diab et al.	8,008,088 B2	8/2011	Bellott et al.
7,377,794 B2	5/2008	Al Ali et al.	RE42,753 E	9/2011	Kiani-Azarbayjany et al.
7,377,899 B2	5/2008	Weber et al.	8,019,400 B2	9/2011	Diab et al.
7,383,070 B2	6/2008	Diab et al.	8,028,701 B2	10/2011	Al-Ali et al.
7,415,297 B2	8/2008	Al-Ali et al.	8,029,765 B2	10/2011	Bellott et al.
7,428,432 B2	9/2008	Ali et al.	8,036,727 B2	10/2011	Schurman et al.
7,438,683 B2	10/2008	Al-Ali et al.	8,036,728 B2	10/2011	Diab et al.
7,440,787 B2	10/2008	Diab	8,046,040 B2	10/2011	Ali et al.
7,454,240 B2	11/2008	Diab et al.	8,046,041 B2	10/2011	Diab et al.
7,467,002 B2	12/2008	Weber et al.	8,046,042 B2	10/2011	Diab et al.
7,469,157 B2	12/2008	Diab et al.	8,048,040 B2	11/2011	Kiani
7,471,969 B2	12/2008	Diab et al.	8,050,728 B2	11/2011	Al-Ali et al.
7,471,971 B2	12/2008	Diab et al.	RE43,169 E	2/2012	Parker
7,483,729 B2	1/2009	Al-Ali et al.	8,118,620 B2	2/2012	Al-Ali et al.
7,483,730 B2	1/2009	Diab et al.	8,126,528 B2	2/2012	Diab et al.
7,489,958 B2	2/2009	Diab et al.	8,128,572 B2	3/2012	Diab et al.
7,496,391 B2	2/2009	Diab et al.	8,130,105 B2	3/2012	Al-Ali et al.
7,496,393 B2	2/2009	Diab et al.	8,145,287 B2	3/2012	Diab et al.
D587,657 S	3/2009	Al-Ali et al.	8,150,487 B2	4/2012	Diab et al.
7,499,741 B2	3/2009	Diab et al.	8,175,672 B2	5/2012	Parker
7,499,835 B2	3/2009	Weber et al.	8,180,420 B2	5/2012	Diab et al.
7,500,950 B2	3/2009	Al-Ali et al.	8,182,443 B1	5/2012	Kiani
7,509,154 B2	3/2009	Diab et al.	8,185,180 B2	5/2012	Diab et al.
7,509,494 B2	3/2009	Al-Ali	8,190,223 B2	5/2012	Al-Ali et al.
7,510,849 B2	3/2009	Schurman et al.	8,190,227 B2	5/2012	Diab et al.
7,526,328 B2	4/2009	Diab et al.	8,203,438 B2	6/2012	Kiani et al.
7,530,942 B1	5/2009	Diab	8,203,704 B2	6/2012	Merritt et al.
7,530,949 B2	5/2009	Al Ali et al.	8,204,566 B2	6/2012	Schurman et al.
			8,219,172 B2	7/2012	Schurman et al.
			8,224,411 B2	7/2012	Al-Ali et al.
			8,228,181 B2	7/2012	Al-Ali
			8,229,533 B2	7/2012	Diab et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,233,955	B2	7/2012	Al-Ali et al.	8,666,468	B1	3/2014	Al-Ali
8,244,325	B2	8/2012	Al-Ali et al.	8,667,967	B2	3/2014	Al-Ali et al.
8,255,026	B1	8/2012	Al-Ali	8,670,811	B2	3/2014	O'Reilly
8,255,027	B2	8/2012	Al-Ali et al.	8,670,814	B2	3/2014	Diab et al.
8,255,028	B2	8/2012	Al-Ali et al.	8,676,286	B2	3/2014	Weber et al.
8,260,577	B2	9/2012	Weber et al.	8,682,407	B2	3/2014	Al-Ali
8,265,723	B1	9/2012	McHale et al.	RE44,823	E	4/2014	Parker
8,274,360	B2	9/2012	Sampath et al.	RE44,875	E	4/2014	Kiani et al.
8,280,473	B2	10/2012	Al-Ali	8,690,799	B2	4/2014	Telfort et al.
8,301,217	B2	10/2012	Al-Ali et al.	8,700,112	B2	4/2014	Kiani
8,306,596	B2	11/2012	Schurman et al.	8,702,627	B2	4/2014	Telfort et al.
8,310,336	B2	11/2012	Muhsin et al.	8,706,179	B2	4/2014	Parker
8,315,683	B2	11/2012	Al-Ali et al.	8,712,494	B1	4/2014	MacNeish, III et al.
RE43,860	E	12/2012	Parker	8,715,206	B2	5/2014	Telfort et al.
8,337,403	B2	12/2012	Al-Ali et al.	8,718,735	B2	5/2014	Lamego et al.
8,346,330	B2	1/2013	Lamego	8,718,737	B2	5/2014	Diab et al.
8,353,842	B2	1/2013	Al-Ali et al.	8,718,738	B2	5/2014	Blank et al.
8,355,766	B2	1/2013	MacNeish, III et al.	8,720,249	B2	5/2014	Al-Ali
8,359,080	B2	1/2013	Diab et al.	8,721,541	B2	5/2014	Al-Ali et al.
8,364,223	B2	1/2013	Al-Ali et al.	8,721,542	B2	5/2014	Al-Ali et al.
8,364,226	B2	1/2013	Diab et al.	8,723,677	B1	5/2014	Kiani
8,374,665	B2	2/2013	Lamego	8,740,792	B1	6/2014	Kiani et al.
8,385,995	B2	2/2013	Al-Ali et al.	8,754,776	B2	6/2014	Poeze et al.
8,385,996	B2	2/2013	Smith et al.	8,755,535	B2	6/2014	Telfort et al.
8,388,353	B2	3/2013	Kiani et al.	8,755,856	B2	6/2014	Diab et al.
8,399,822	B2	3/2013	Al-Ali	8,755,872	B1	6/2014	Marinow
8,401,602	B2	3/2013	Kiani	8,761,850	B2	6/2014	Lamego
8,405,608	B2	3/2013	Al-Ali et al.	8,764,671	B2	7/2014	Kiani
8,414,499	B2	4/2013	Al-Ali et al.	8,768,423	B2	7/2014	Shakespeare et al.
8,418,524	B2	4/2013	Al-Ali	8,771,204	B2	7/2014	Telfort et al.
8,423,106	B2	4/2013	Lamego et al.	8,777,634	B2	7/2014	Kiani et al.
8,428,967	B2	4/2013	Olsen et al.	8,781,543	B2	7/2014	Diab et al.
8,430,817	B1	4/2013	Al-Ali et al.	8,781,544	B2	7/2014	Al-Ali et al.
8,437,825	B2	5/2013	Dalvi et al.	8,781,549	B2	7/2014	Al-Ali et al.
8,455,290	B2	6/2013	Siskavich	8,788,003	B2	7/2014	Schurman et al.
8,457,703	B2	6/2013	Al-Ali	8,790,268	B2	7/2014	Al-Ali
8,457,707	B2	6/2013	Kiani	8,801,613	B2	8/2014	Al-Ali et al.
8,463,349	B2	6/2013	Diab et al.	8,821,397	B2	9/2014	Al-Ali et al.
8,466,286	B2	6/2013	Bellot et al.	8,821,415	B2	9/2014	Al-Ali et al.
8,471,713	B2	6/2013	Poeze et al.	8,830,449	B1	9/2014	Lamego et al.
8,473,020	B2	6/2013	Kiani et al.	8,831,700	B2	9/2014	Schurman et al.
8,483,787	B2	7/2013	Al-Ali et al.	8,840,549	B2	9/2014	Al-Ali et al.
8,489,364	B2	7/2013	Weber et al.	8,847,740	B2	9/2014	Kiani et al.
8,498,684	B2	7/2013	Weber et al.	8,849,365	B2	9/2014	Smith et al.
8,504,128	B2	8/2013	Blank et al.	8,852,094	B2	10/2014	Al-Ali et al.
8,509,867	B2	8/2013	Workman et al.	8,852,994	B2	10/2014	Wojtczuk et al.
8,515,509	B2	8/2013	Bruinsma et al.	8,868,147	B2	10/2014	Stippick et al.
8,523,781	B2	9/2013	Al-Ali	8,868,150	B2	10/2014	Al-Ali et al.
8,529,301	B2	9/2013	Al-Ali et al.	8,870,792	B2	10/2014	Al-Ali et al.
8,532,727	B2	9/2013	Ali et al.	8,886,271	B2	11/2014	Kiani et al.
8,532,728	B2	9/2013	Diab et al.	8,888,539	B2	11/2014	Al-Ali et al.
D692,145	S	10/2013	Al-Ali et al.	8,888,708	B2	11/2014	Diab et al.
8,547,209	B2	10/2013	Kiani et al.	8,892,180	B2	11/2014	Weber et al.
8,548,548	B2	10/2013	Al-Ali	8,897,847	B2	11/2014	Al-Ali
8,548,549	B2	10/2013	Schurman et al.	8,909,310	B2	12/2014	Lamego et al.
8,548,550	B2	10/2013	Al-Ali et al.	8,911,377	B2	12/2014	Al-Ali
8,560,032	B2	10/2013	Al-Ali et al.	8,912,909	B2	12/2014	Al-Ali et al.
8,560,034	B1	10/2013	Diab et al.	8,920,317	B2	12/2014	Al-Ali et al.
8,570,167	B2	10/2013	Al-Ali	8,921,699	B2	12/2014	Al-Ali et al.
8,570,503	B2	10/2013	Vo et al.	8,922,382	B2	12/2014	Al-Ali et al.
8,571,617	B2	10/2013	Reichgott et al.	8,929,964	B2	1/2015	Al-Ali et al.
8,571,618	B1	10/2013	Lamego et al.	8,942,777	B2	1/2015	Diab et al.
8,571,619	B2	10/2013	Al-Ali et al.	8,948,834	B2	2/2015	Diab et al.
8,577,431	B2	11/2013	Lamego et al.	8,948,835	B2	2/2015	Diab
8,581,732	B2	11/2013	Al-Ali et al.	8,965,471	B2	2/2015	Lamego
8,584,345	B2	11/2013	Al-Ali et al.	8,983,564	B2	3/2015	Al-Ali
8,588,880	B2	11/2013	Abdul-Hafiz et al.	8,989,831	B2	3/2015	Al-Ali et al.
8,600,467	B2	12/2013	Al-Ali et al.	8,996,085	B2	3/2015	Kiani et al.
8,606,342	B2	12/2013	Diab	8,998,809	B2	4/2015	Kiani
8,626,255	B2	1/2014	Al-Ali et al.	9,028,429	B2	5/2015	Telfort et al.
8,630,691	B2	1/2014	Lamego et al.	9,037,207	B2	5/2015	Al-Ali et al.
8,634,889	B2	1/2014	Al-Ali et al.	9,060,721	B2	6/2015	Reichgott et al.
8,641,631	B2	2/2014	Sierra et al.	9,066,666	B2	6/2015	Kiani
8,652,060	B2	2/2014	Al-Ali	9,066,680	B1	6/2015	Al-Ali et al.
8,663,107	B2	3/2014	Kiani	9,072,474	B2	7/2015	Al-Ali et al.
				9,078,560	B2	7/2015	Schurman et al.
				9,084,569	B2	7/2015	Weber et al.
				9,095,316	B2	8/2015	Welch et al.
				9,106,038	B2	8/2015	Telfort et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,107,625 B2	8/2015	Telfort et al.	9,622,693 B2	4/2017	Diab
9,107,626 B2	8/2015	Al-Ali et al.	D788,312 S	5/2017	Al-Ali et al.
9,113,831 B2	8/2015	Al-Ali	9,636,055 B2	5/2017	Al-Ali et al.
9,113,832 B2	8/2015	Al-Ali	9,636,056 B2	5/2017	Al-Ali
9,119,595 B2	9/2015	Lamego	9,649,054 B2	5/2017	Lamego et al.
9,131,881 B2	9/2015	Diab et al.	9,662,052 B2	5/2017	Al-Ali et al.
9,131,882 B2	9/2015	Al-Ali et al.	9,668,679 B2	6/2017	Schurman et al.
9,131,883 B2	9/2015	Al-Ali	9,668,680 B2	6/2017	Bruinsma et al.
9,131,917 B2	9/2015	Telfort et al.	9,668,703 B2	6/2017	Al-Ali
9,138,180 B1	9/2015	Coverston et al.	9,675,286 B2	6/2017	Diab
9,138,182 B2	9/2015	Al-Ali et al.	9,687,160 B2	6/2017	Kiani
9,138,192 B2	9/2015	Weber et al.	9,693,719 B2	7/2017	Al-Ali et al.
9,142,117 B2	9/2015	Muhsin et al.	9,693,737 B2	7/2017	Al-Ali
9,153,112 B1	10/2015	Kiani et al.	9,697,928 B2	7/2017	Al-Ali et al.
9,153,121 B2	10/2015	Kiani et al.	9,717,425 B2	8/2017	Kiani et al.
9,161,696 B2	10/2015	Al-Ali et al.	9,717,458 B2	8/2017	Lamego et al.
9,161,713 B2	10/2015	Al-Ali et al.	9,724,016 B1	8/2017	Al-Ali et al.
9,167,995 B2	10/2015	Lamego et al.	9,724,024 B2	8/2017	Al-Ali
9,176,141 B2	11/2015	Al-Ali et al.	9,724,025 B1	8/2017	Kiani et al.
9,186,102 B2	11/2015	Bruinsma et al.	9,730,640 B2	8/2017	Diab et al.
9,192,312 B2	11/2015	Al-Ali	9,743,887 B2	8/2017	Al-Ali et al.
9,192,329 B2	11/2015	Al-Ali	9,749,232 B2	8/2017	Sampath et al.
9,192,351 B1	11/2015	Telfort et al.	9,750,442 B2	9/2017	Olsen
9,195,385 B2	11/2015	Al-Ali et al.	9,750,443 B2	9/2017	Smith et al.
9,211,072 B2	12/2015	Kiani	9,750,461 B1	9/2017	Telfort
9,211,095 B1	12/2015	Al-Ali	9,775,545 B2	10/2017	Al-Ali et al.
9,218,454 B2	12/2015	Kiani et al.	9,775,546 B2	10/2017	Diab et al.
9,226,696 B2	1/2016	Kiani	9,775,570 B2	10/2017	Al-Ali
9,241,662 B2	1/2016	Al-Ali et al.	9,778,079 B1	10/2017	Al-Ali et al.
9,245,668 B1	1/2016	Vo et al.	9,782,077 B2	10/2017	Lamego et al.
9,259,185 B2	2/2016	Abdul-Hafiz et al.	9,782,110 B2	10/2017	Kiani
9,267,572 B2	2/2016	Barker et al.	9,787,568 B2	10/2017	Lamego et al.
9,277,880 B2	3/2016	Poeze et al.	9,788,735 B2	10/2017	Al-Ali
9,289,167 B2	3/2016	Diab et al.	9,788,768 B2	10/2017	Al-Ali et al.
9,295,421 B2	3/2016	Kiani et al.	9,795,300 B2	10/2017	Al-Ali
9,307,928 B1	4/2016	Al-Ali et al.	9,795,310 B2	10/2017	Al-Ali
9,323,894 B2	4/2016	Kiani	9,795,358 B2	10/2017	Telfort et al.
D755,392 S	5/2016	Hwang et al.	9,795,739 B2	10/2017	Al-Ali et al.
9,326,712 B1	5/2016	Kiani	9,801,556 B2	10/2017	Kiani
9,333,316 B2	5/2016	Kiani	9,801,588 B2	10/2017	Weber et al.
9,339,220 B2	5/2016	Lamego et al.	9,808,188 B1	11/2017	Perea et al.
9,341,565 B2	5/2016	Lamego et al.	9,814,418 B2	11/2017	Weber et al.
9,351,673 B2	5/2016	Diab et al.	9,820,691 B2	11/2017	Kiani
9,351,675 B2	5/2016	Al-Ali et al.	9,833,152 B2	12/2017	Kiani et al.
9,364,181 B2	6/2016	Kiani et al.	9,833,180 B2	12/2017	Shakespeare et al.
9,368,671 B2	6/2016	Wojtczuk et al.	9,839,379 B2	12/2017	Al-Ali et al.
9,370,325 B2	6/2016	Al-Ali et al.	9,839,381 B1	12/2017	Weber et al.
9,370,326 B2	6/2016	McHale et al.	9,847,002 B2	12/2017	Kiani et al.
9,370,335 B2	6/2016	Al-Ali et al.	9,847,749 B2	12/2017	Kiani et al.
9,375,185 B2	6/2016	Ali et al.	9,848,800 B1	12/2017	Lee et al.
9,386,953 B2	7/2016	Al-Ali	9,848,806 B2	12/2017	Al-Ali et al.
9,386,961 B2	7/2016	Al-Ali et al.	9,848,807 B2	12/2017	Lamego
9,392,945 B2	7/2016	Al-Ali et al.	9,861,298 B2	1/2018	Eckerbom et al.
9,397,448 B2	7/2016	Al-Ali et al.	9,861,304 B2	1/2018	Al-Ali et al.
9,408,542 B1	8/2016	Kinast et al.	9,861,305 B1	1/2018	Weber et al.
9,436,645 B2	9/2016	Al-Ali et al.	9,867,578 B2	1/2018	Al-Ali et al.
9,445,759 B1	9/2016	Lamego et al.	9,872,623 B2	1/2018	Al-Ali
9,466,919 B2	10/2016	Kiani et al.	9,876,320 B2	1/2018	Coverston et al.
9,474,474 B2	10/2016	Lamego et al.	9,877,650 B2	1/2018	Muhsin et al.
9,480,422 B2	11/2016	Al-Ali	9,877,686 B2	1/2018	Al-Ali et al.
9,480,435 B2	11/2016	Olsen	9,891,079 B2	2/2018	Dalvi
9,492,110 B2	11/2016	Al-Ali et al.	9,895,107 B2	2/2018	Al-Ali et al.
9,510,779 B2	12/2016	Poeze et al.	2005/0007125 A1	1/2005	Heger
9,517,024 B2	12/2016	Kiani et al.	2006/0161054 A1	7/2006	Reuss et al.
9,532,722 B2	1/2017	Lamego et al.	2007/0282478 A1	12/2007	Al-Ali et al.
9,538,949 B2	1/2017	Al-Ali et al.	2008/0033275 A1	2/2008	Blank et al.
9,538,980 B2	1/2017	Telfort et al.	2008/0319299 A1	12/2008	Stippick et al.
9,549,696 B2	1/2017	Lamego et al.	2009/0247984 A1	10/2009	Lamego et al.
9,554,737 B2	1/2017	Schurman et al.	2009/0275813 A1	11/2009	Davis
9,560,996 B2	2/2017	Kiani	2009/0275844 A1	11/2009	Al-Ali
9,560,998 B2	2/2017	Al-Ali et al.	2010/0004518 A1	1/2010	Vo et al.
9,566,019 B2	2/2017	Al-Ali et al.	2010/0030040 A1	2/2010	Poeze et al.
9,579,039 B2	2/2017	Jansen et al.	2011/0082711 A1	4/2011	Poeze et al.
9,591,975 B2	3/2017	Dalvi et al.	2011/0105854 A1	5/2011	Kiani et al.
9,622,692 B2	4/2017	Lamego et al.	2011/0125060 A1	5/2011	Telfort et al.
			2011/0208015 A1	8/2011	Welch et al.
			2011/0230733 A1	9/2011	Al-Ali
			2012/0165629 A1	6/2012	Merritt et al.
			2012/0209082 A1	8/2012	Al-Ali

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0209084 A1	8/2012	Olsen et al.	2015/0257689 A1	9/2015	Al-Ali et al.
2012/0283524 A1	11/2012	Kiani et al.	2015/0272514 A1	10/2015	Kiani et al.
2012/0319816 A1	12/2012	Al-Ali	2015/0351697 A1	12/2015	Weber et al.
2013/0023775 A1	1/2013	Lamego et al.	2015/0359429 A1	12/2015	Al-Ali et al.
2013/0041591 A1	2/2013	Lamego	2016/0029932 A1	2/2016	Al-Ali
2013/0060147 A1	3/2013	Welch et al.	2016/0058347 A1	3/2016	Reichgott et al.
2013/0096405 A1	4/2013	Garfio	2016/0066824 A1	3/2016	Al-Ali et al.
2013/0096936 A1	4/2013	Sampath et al.	2016/0081552 A1	3/2016	Wojtczuk et al.
2013/0243021 A1	9/2013	Siskavich	2016/0095543 A1	4/2016	Telfort et al.
2013/0253334 A1	9/2013	Al-Ali et al.	2016/0095548 A1	4/2016	Al-Ali et al.
2013/0296672 A1	11/2013	O'Neil et al.	2016/0103598 A1	4/2016	Al-Ali et al.
2013/0296713 A1	11/2013	Al-Ali et al.	2016/0143548 A1	5/2016	Al-Ali
2013/0324808 A1	12/2013	Al-Ali et al.	2016/0166182 A1	6/2016	Al-Ali et al.
2013/0331660 A1	12/2013	Al-Ali et al.	2016/0166183 A1	6/2016	Poeze et al.
2014/0012100 A1	1/2014	Al-Ali et al.	2016/0192869 A1	7/2016	Kiani et al.
2014/0051953 A1	2/2014	Lamego et al.	2016/0196388 A1	7/2016	Lamego
2014/0081175 A1	3/2014	Telfort	2016/0197436 A1	7/2016	Barker et al.
2014/0120564 A1	5/2014	Workman et al.	2016/0213281 A1	7/2016	Eckerbom et al.
2014/0121482 A1	5/2014	Merritt et al.	2016/0228043 A1	8/2016	O'Neil et al.
2014/0127137 A1	5/2014	Bellott et al.	2016/0233632 A1	8/2016	Scruggs et al.
2014/0135588 A1	5/2014	Al-Ali et al.	2016/0234944 A1	8/2016	Schmidt et al.
2014/0135602 A1 *	5/2014	Lemke A61B 5/6829 600/324	2016/0270735 A1	9/2016	Diab et al.
2014/0163344 A1	6/2014	Al-Ali	2016/0283665 A1	9/2016	Sampath et al.
2014/0163402 A1	6/2014	Lamego et al.	2016/0287090 A1	10/2016	Al-Ali et al.
2014/0166076 A1	6/2014	Kiani et al.	2016/0287786 A1	10/2016	Kiani
2014/0171763 A1	6/2014	Diab	2016/0296169 A1	10/2016	McHale et al.
2014/0180038 A1	6/2014	Kiani	2016/0310052 A1	10/2016	Al-Ali et al.
2014/0180154 A1	6/2014	Sierra et al.	2016/0314260 A1	10/2016	Kiani
2014/0180160 A1	6/2014	Brown et al.	2016/0324486 A1	11/2016	Al-Ali et al.
2014/0187973 A1	7/2014	Brown et al.	2016/0324488 A1	11/2016	Olsen
2014/0213864 A1	7/2014	Abdul-Hafiz et al.	2016/0327984 A1	11/2016	Al-Ali et al.
2014/0266790 A1	9/2014	Al-Ali et al.	2016/0328528 A1	11/2016	Al-Ali et al.
2014/0275808 A1	9/2014	Poeze et al.	2016/0331332 A1	11/2016	Al-Ali
2014/0275835 A1	9/2014	Lamego et al.	2016/0367173 A1	12/2016	Dalvi et al.
2014/0275871 A1	9/2014	Lamego et al.	2017/0000394 A1	1/2017	Al-Ali et al.
2014/0275872 A1	9/2014	Merritt et al.	2017/0007134 A1	1/2017	Al-Ali et al.
2014/0276115 A1	9/2014	Dalvi et al.	2017/0007198 A1	1/2017	Al-Ali et al.
2014/0288400 A1	9/2014	Diab et al.	2017/0014083 A1	1/2017	Diab et al.
2014/0316217 A1	10/2014	Purdon et al.	2017/0014084 A1	1/2017	Al-Ali et al.
2014/0316218 A1	10/2014	Purdon et al.	2017/0027456 A1	2/2017	Kinast et al.
2014/0316228 A1	10/2014	Blank et al.	2017/0042488 A1	2/2017	Muhsin
2014/0323825 A1	10/2014	Al-Ali et al.	2017/0055851 A1	3/2017	Al-Ali
2014/0323897 A1	10/2014	Brown et al.	2017/0055882 A1	3/2017	Al-Ali et al.
2014/0323898 A1	10/2014	Purdon et al.	2017/0055887 A1	3/2017	Al-Ali
2014/0330092 A1	11/2014	Al-Ali et al.	2017/0055896 A1	3/2017	Al-Ali et al.
2014/0330098 A1	11/2014	Merritt et al.	2017/0079594 A1	3/2017	Telfort et al.
2014/0357966 A1	12/2014	Al-Ali et al.	2017/0086723 A1	3/2017	Al-Ali et al.
2015/0005600 A1	1/2015	Blank et al.	2017/0143281 A1	5/2017	Olsen
2015/0011907 A1	1/2015	Purdon et al.	2017/0147774 A1	5/2017	Kiani
2015/0012231 A1	1/2015	Poeze et al.	2017/0156620 A1	6/2017	Al-Ali et al.
2015/0032029 A1	1/2015	Al-Ali et al.	2017/0173632 A1	6/2017	Al-Ali
2015/0038859 A1	2/2015	Dalvi et al.	2017/0187146 A1	6/2017	Kiani et al.
2015/0080754 A1	3/2015	Purdon et al.	2017/0188919 A1	7/2017	Al-Ali et al.
2015/0087936 A1	3/2015	Al-Ali et al.	2017/0196464 A1	7/2017	Jansen et al.
2015/0094546 A1	4/2015	Al-Ali	2017/0196470 A1	7/2017	Lamego et al.
2015/0097701 A1	4/2015	Al-Ali et al.	2017/0202490 A1	7/2017	Al-Ali et al.
2015/0099950 A1	4/2015	Al-Ali et al.	2017/0224262 A1	8/2017	Al-Ali
2015/0099955 A1	4/2015	Al-Ali et al.	2017/0228516 A1	8/2017	Sampath et al.
2015/0101844 A1	4/2015	Al-Ali et al.	2017/0245790 A1	8/2017	Al-Ali et al.
2015/0106121 A1	4/2015	Muhsin et al.	2017/0251974 A1	9/2017	Shreim et al.
2015/0112151 A1	4/2015	Muhsin et al.	2017/0251975 A1	9/2017	Shreim et al.
2015/0116076 A1	4/2015	Al-Ali et al.	2017/0258403 A1	9/2017	Abdul-Hafiz et al.
2015/0126830 A1	5/2015	Schurman et al.	2017/0311891 A1	11/2017	Kiani et al.
2015/0165312 A1	6/2015	Kiani	2017/0325728 A1	11/2017	Al-Ali et al.
2015/0196249 A1	7/2015	Brown et al.	2017/0332976 A1	11/2017	Al-Ali et al.
2015/0216459 A1	8/2015	Al-Ali et al.	2017/0340293 A1	11/2017	Al-Ali et al.
2015/0238722 A1	8/2015	Al-Ali	2017/0360310 A1	12/2017	Kiani et al.
2015/0245773 A1	9/2015	Lamego et al.	2017/0367632 A1	12/2017	Al-Ali et al.
2015/0245794 A1	9/2015	Al-Ali	2018/0008146 A1	1/2018	Al-Ali et al.
			2018/0014752 A1	1/2018	Al-Ali et al.
			2018/0028124 A1	2/2018	Al-Ali et al.

* cited by examiner

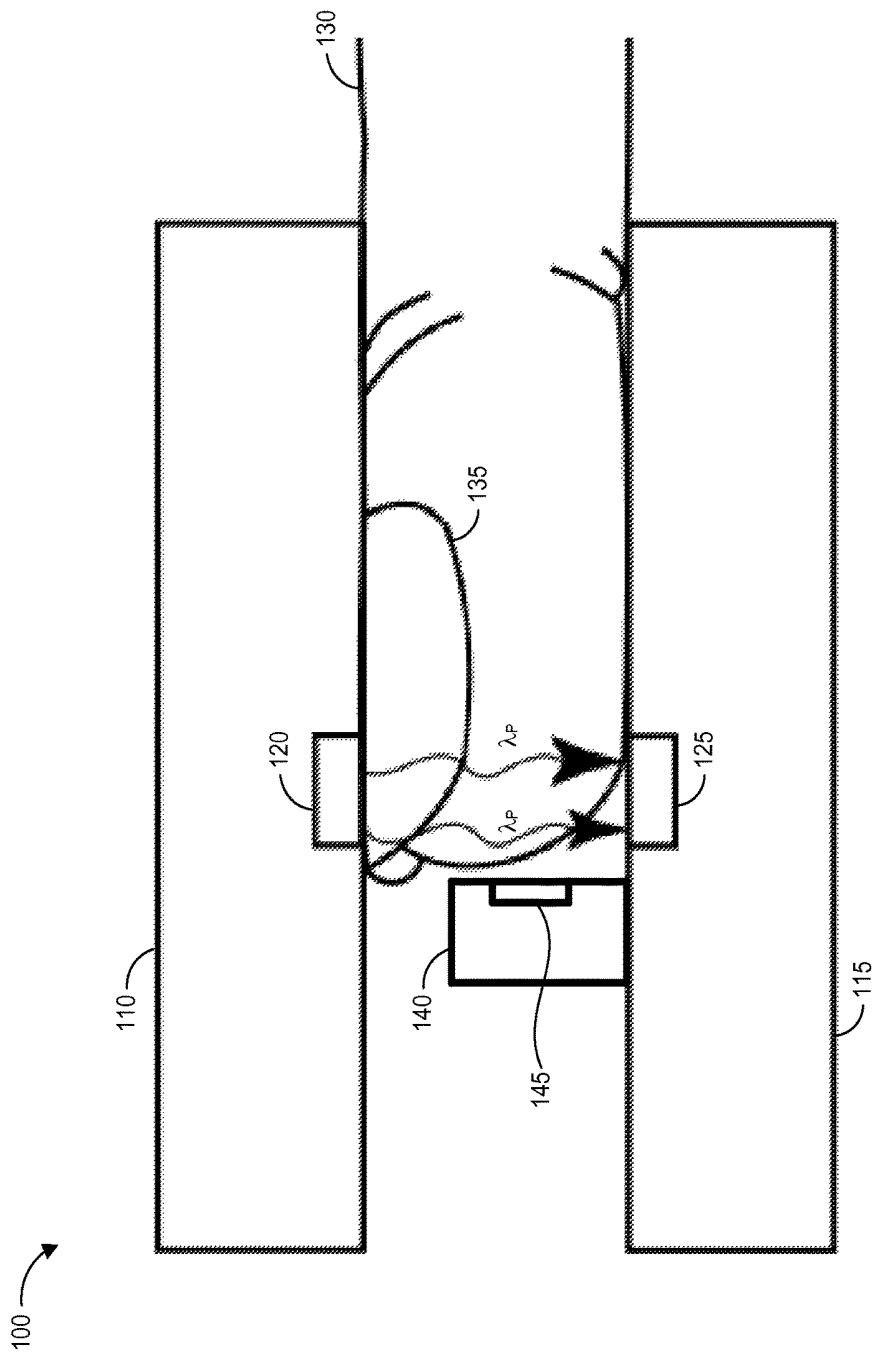


FIG. 1A

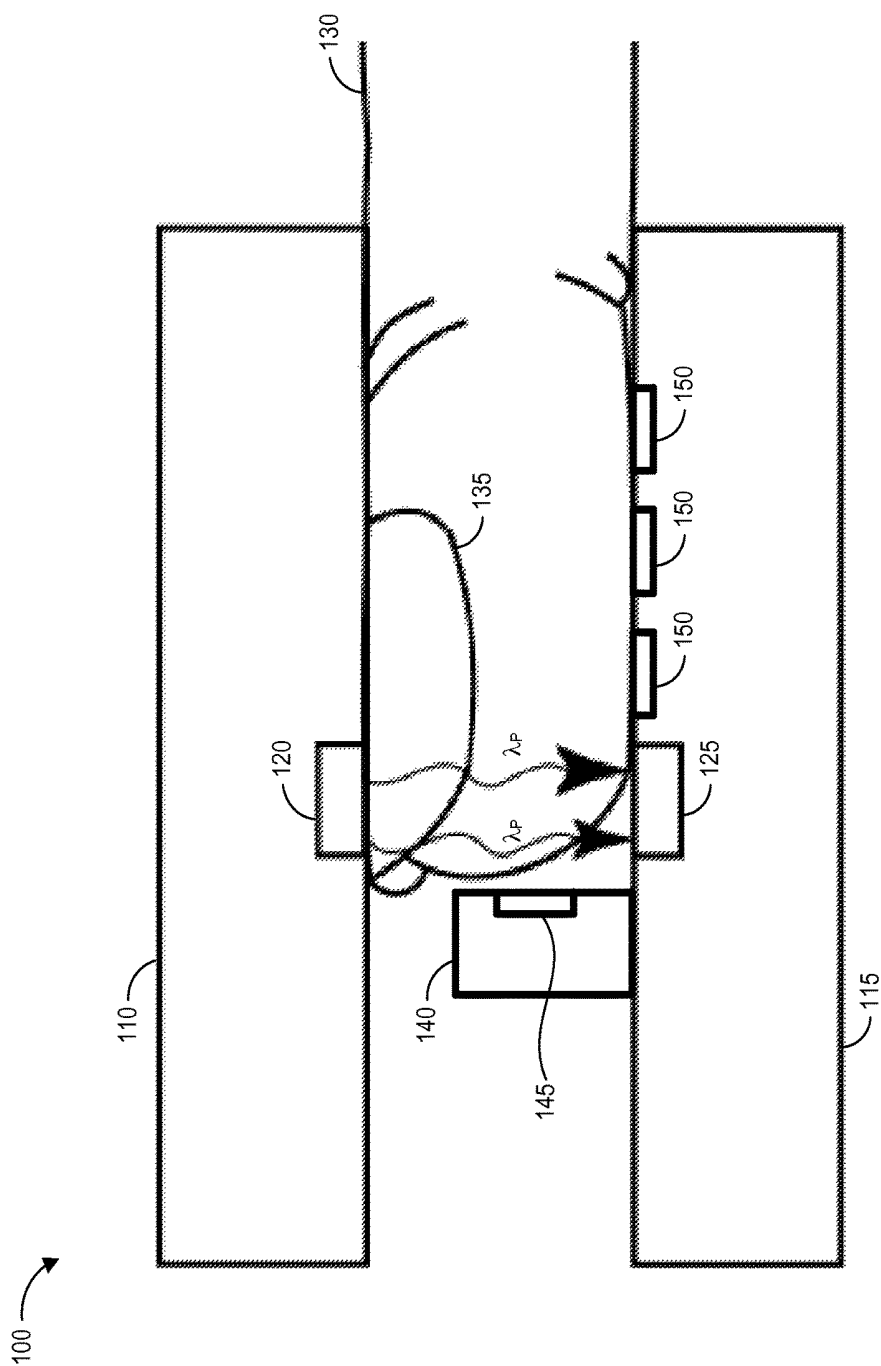


FIG. 1B

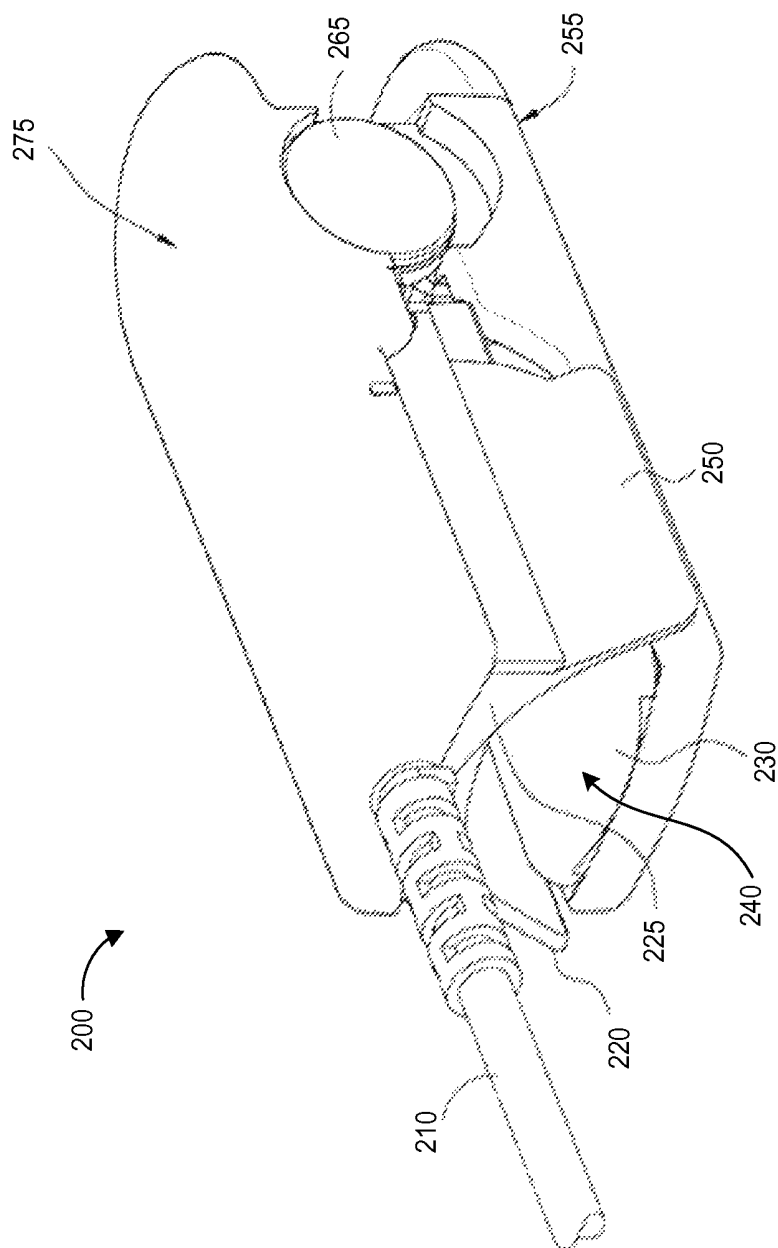


FIG. 2A

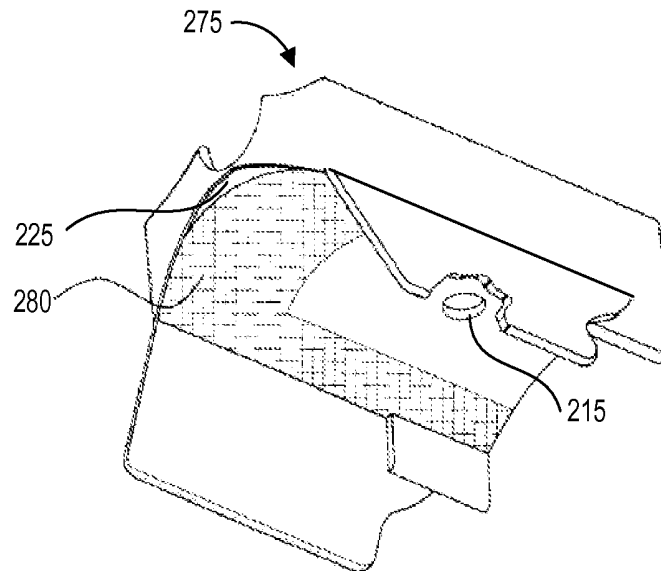


FIG. 2B

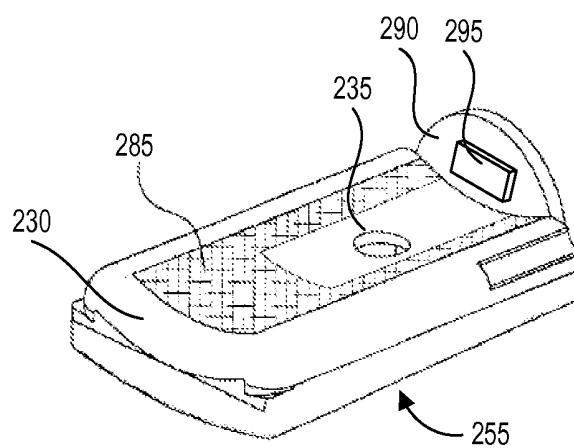


FIG. 2C

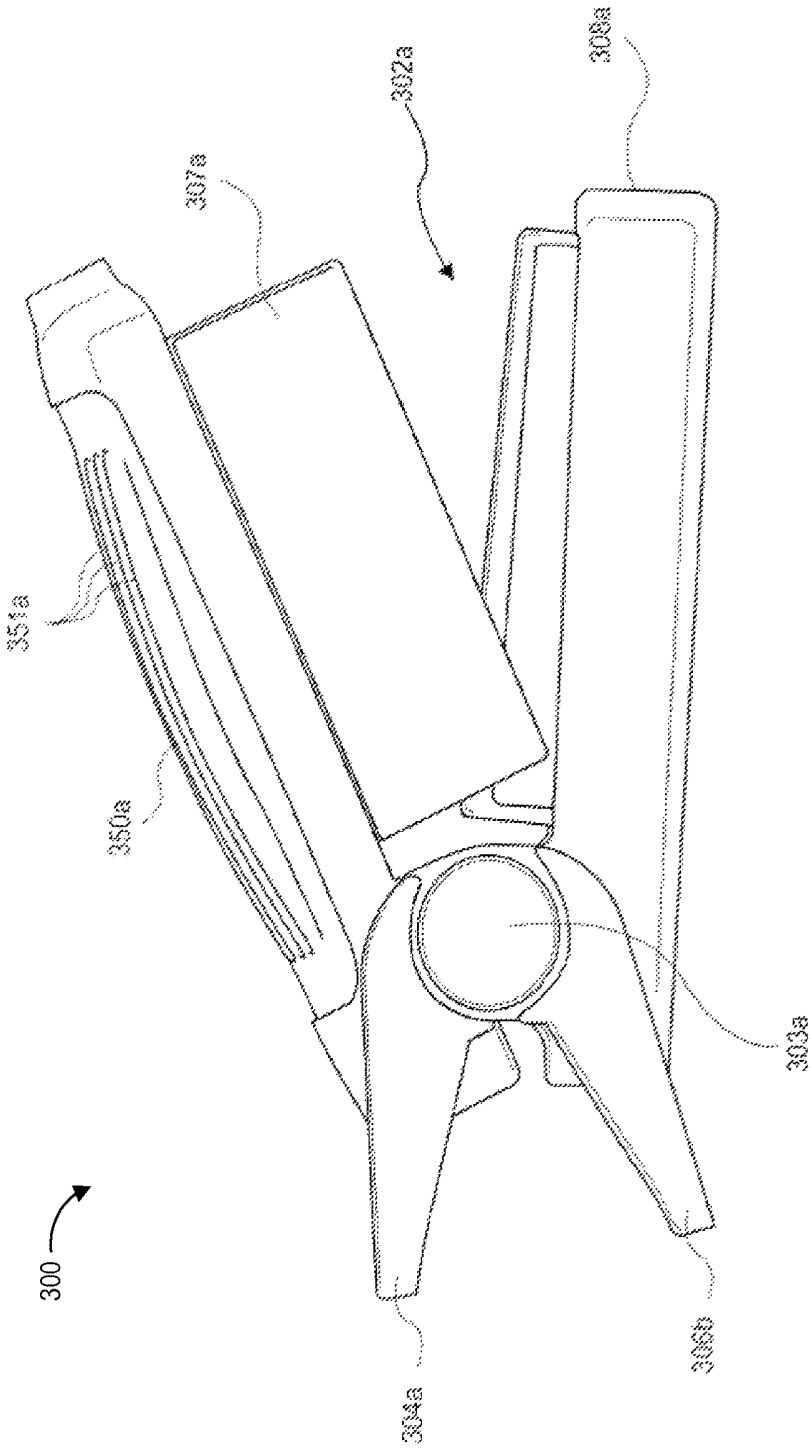
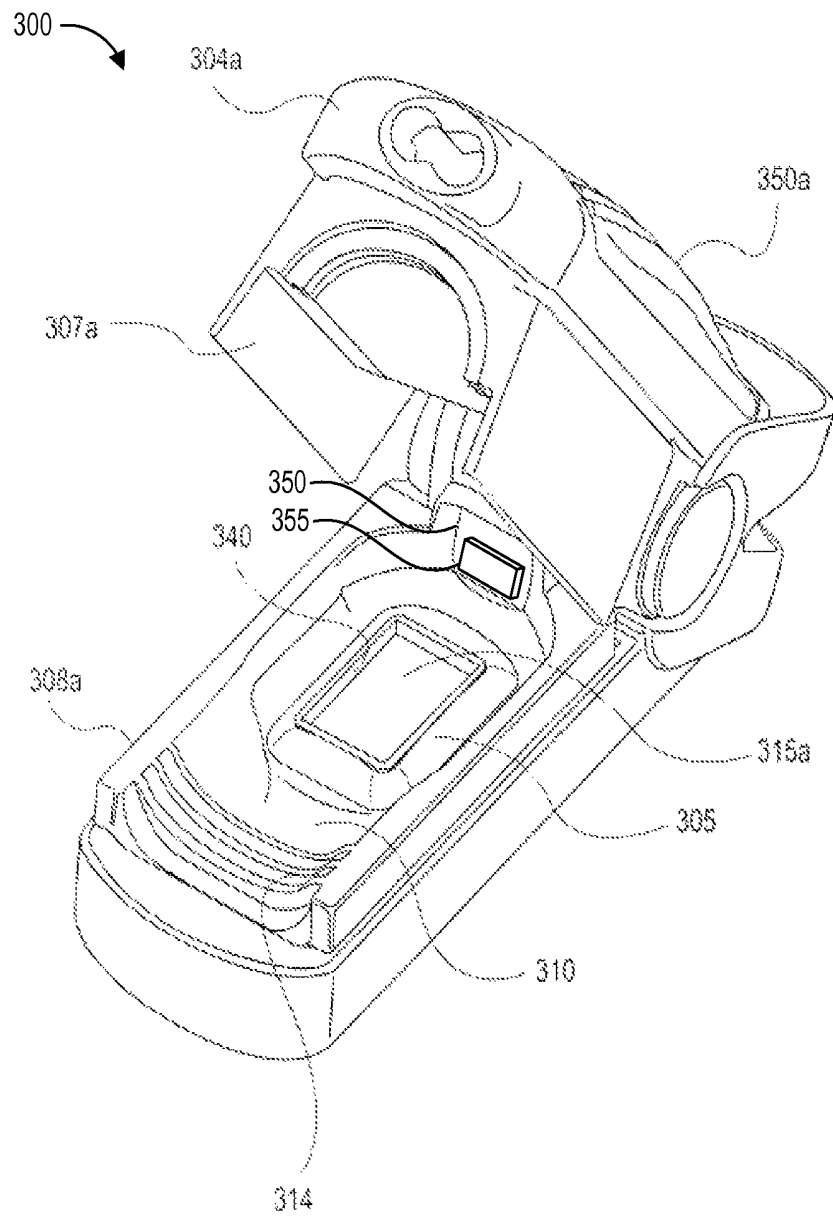


FIG. 3A

**FIG. 3B**

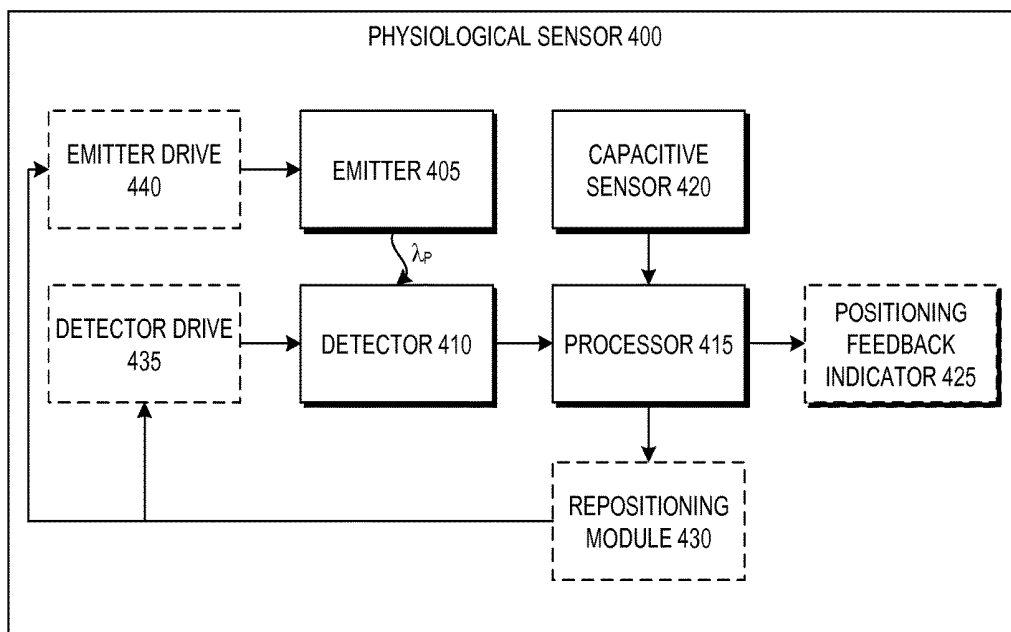


FIG. 4

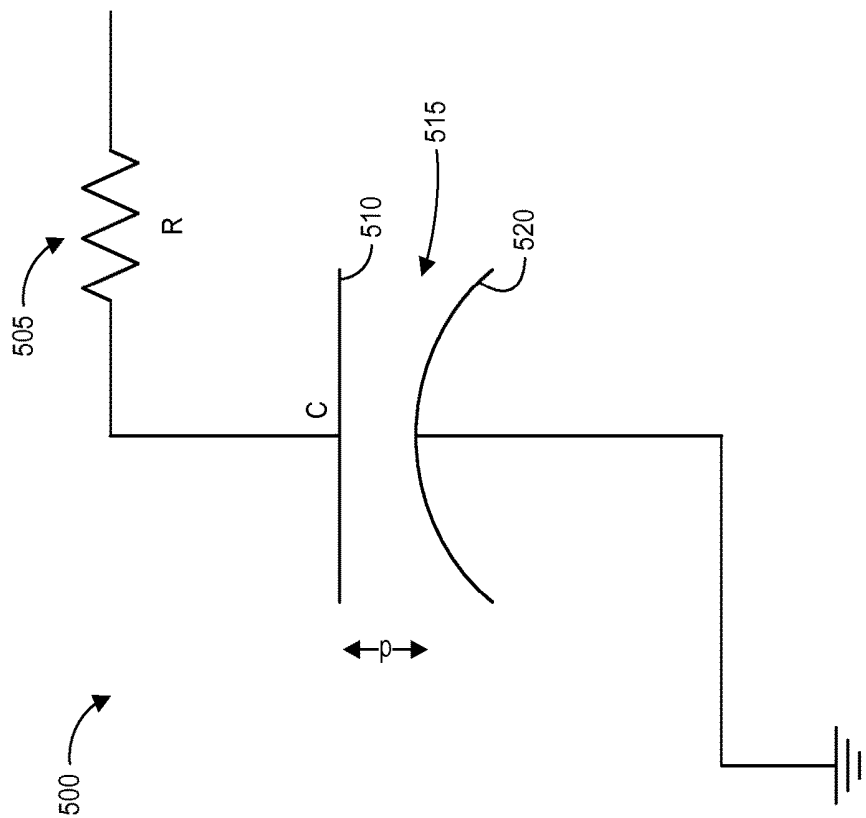
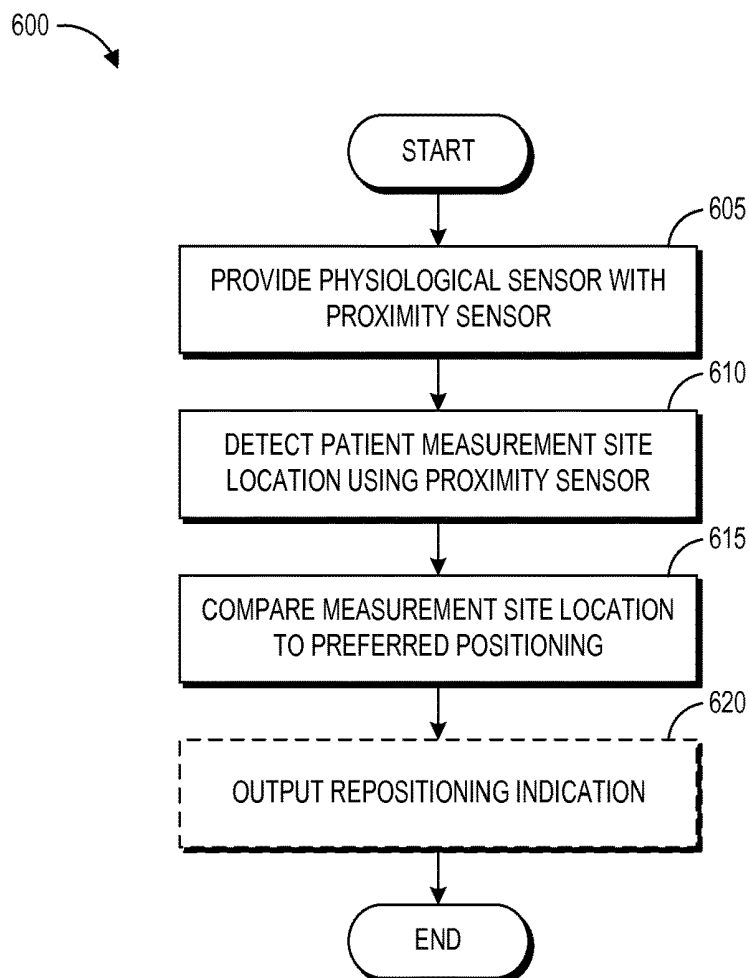
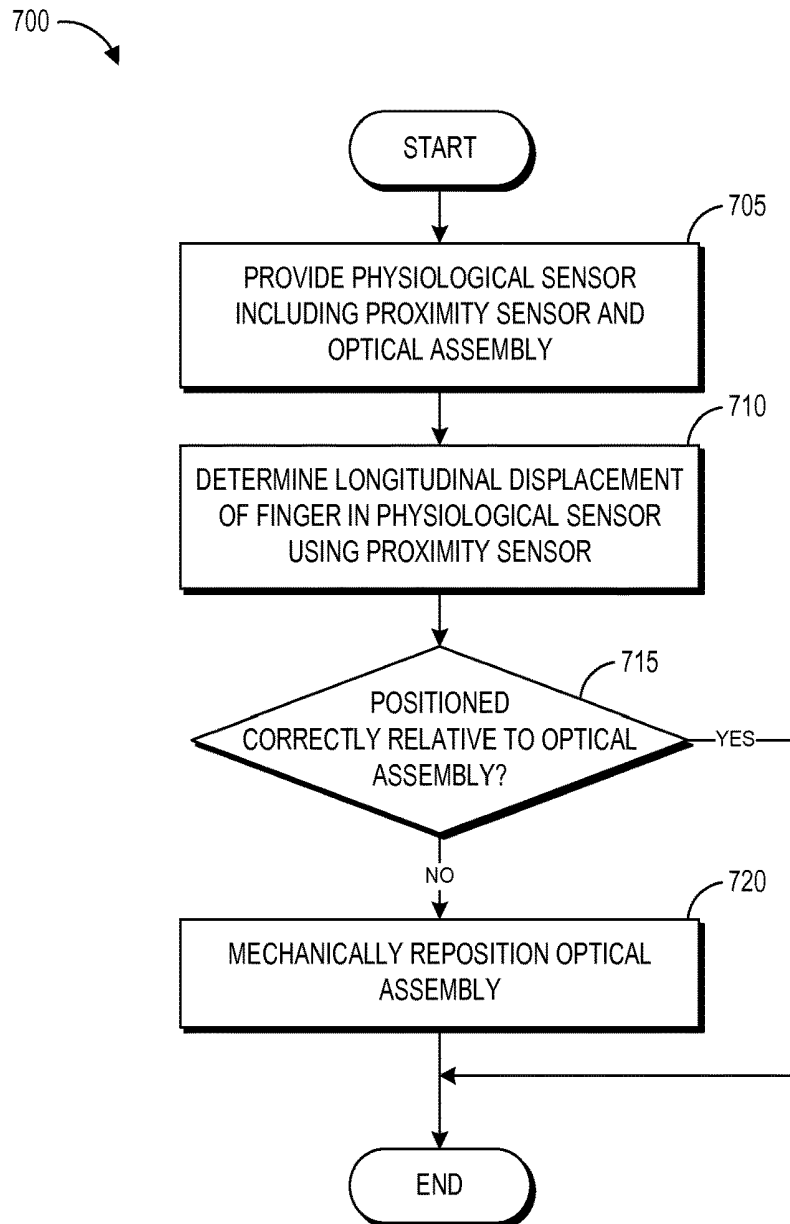
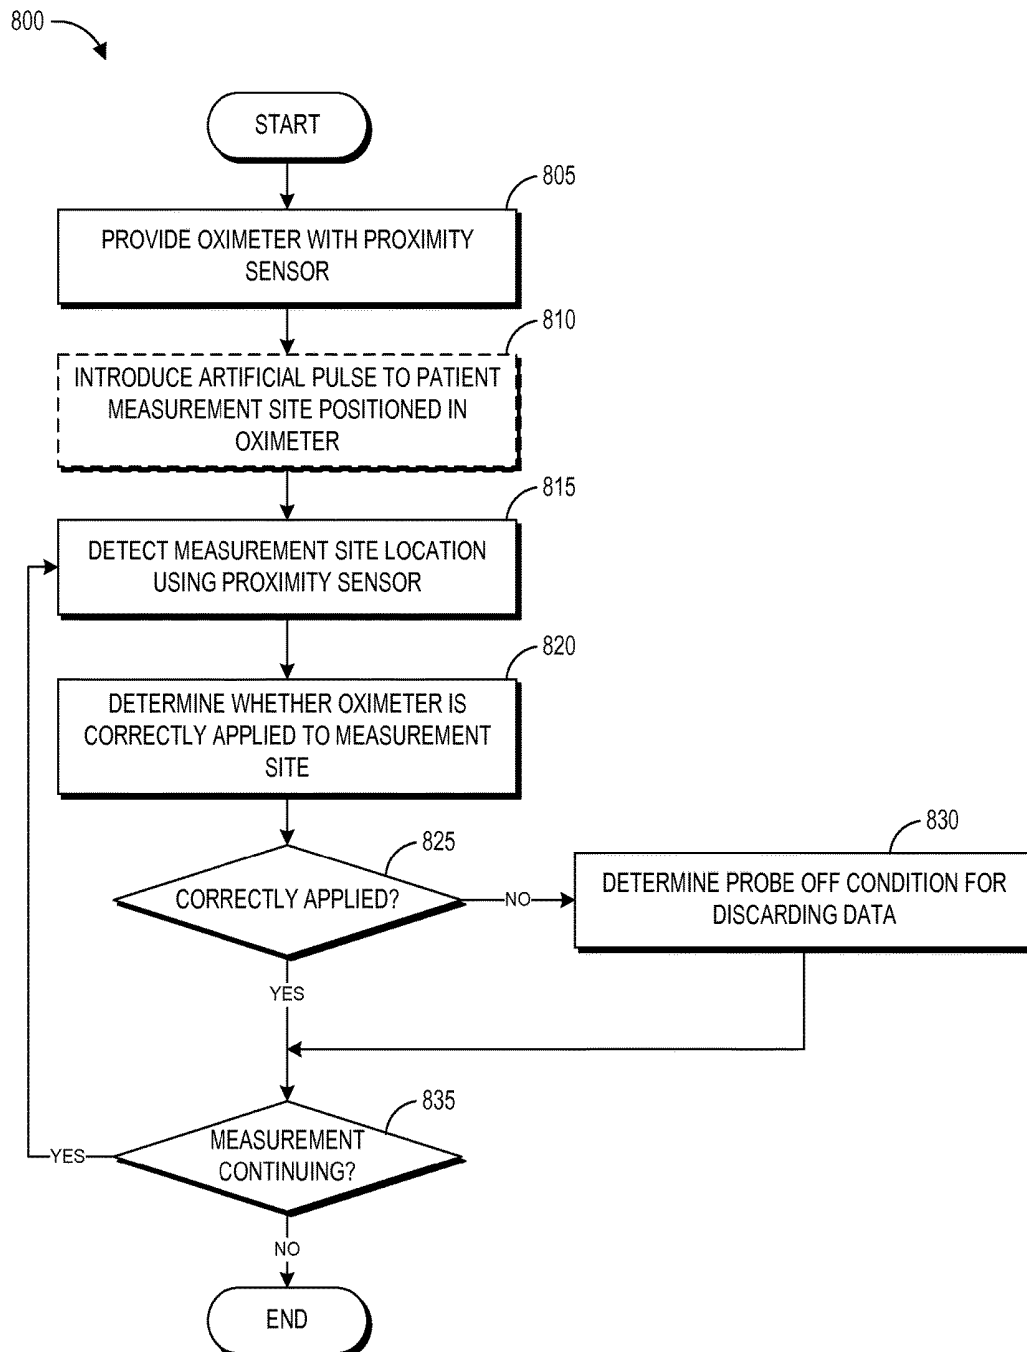


FIG. 5

SENSOR APPLICATION POSITIONING DETECTION**FIG. 6**

OPTICAL ASSEMBLY REPOSITIONING**FIG. 7**

PROBE OFF DETERMINATION BASED ON PROXIMITY SENSING**FIG. 8**

PROXIMITY SENSOR IN PULSE OXIMETER**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application claims the benefit of U.S. Provisional Application Ser. No. 62/014,611, filed Jun. 19, 2014, titled "PROXIMITY SENSOR IN PULSE OXIMETER," the entirety of which is hereby incorporated by reference.

TECHNICAL FIELD

The systems and methods disclosed herein are directed to patient monitoring, and, more particularly, to pulse oximeter patient monitors capable of capacitive proximity detection.

BACKGROUND

The standard of care in caregiver environments includes patient monitoring through spectroscopic analysis using, for example, a pulse oximeter. Devices capable of spectroscopic analysis generally include a light source(s) transmitting optical radiation into or reflecting off a measurement site, such as, body tissue carrying pulsing blood. After attenuation by tissue and fluids of the measurement site, a photo-detection device(s) detects the attenuated light and outputs a detector signal(s) responsive to the detected attenuated light. A signal processing device(s) process the detector(s) signal(s) and outputs a measurement indicative of a blood constituent of interest, such as glucose, oxygen, methemoglobin, total hemoglobin, other physiological parameters, or other data or combinations of data useful in determining a state or trend of wellness of a patient.

In noninvasive devices and methods, a sensor is often adapted to position a finger proximate the light source and light detector. For example, noninvasive finger clip sensors often include a clothespin-shaped housing that includes a contoured bed conforming generally to the shape of a finger.

Accurate determination of physiological measurements is often dependent upon proper application of the optical sensor to the measurement site. Clip-type pulse oximeter sensors typically include a physical stop near the hinge of the housing to indicate desired placement of a user's finger or other measurement site within the sensor. However, the physical stop does not ensure that the patient's finger is positioned far enough into the sensor. In addition, even if a sensor is initially placed correctly, movement, either of the patient or of the sensor during artificial pulsing, can longitudinally displace the patient's finger within the sensor. This can result in the light source and detector of the oximeter being positioned around a portion of the finger that provides inaccurate physiological measurements.

SUMMARY

The foregoing and other problems are addressed, in some embodiments, by providing an oximeter with proximity sensing technology that can be used to determine whether the oximeter is correctly applied to a patient measurement site. For example, one or more capacitive sensor electrodes can provide an indication to a processor of the oximeter regarding whether the sensor is correctly positioned by sensing proximity to the skin of the measurement site. Capacitive sensor electrodes can provide data representing a distance or relative distance between the electrodes and skin of the measurement site. Due to the inverse relationship between capacitance and distance, the sensitivity to the

distance between the measurement site and the capacitive sensor electrodes increases as the distance between the measurement site and the capacitive sensor electrodes decreases. Accordingly, in one embodiment, a plurality of capacitive sensor electrodes can be positioned at various locations within the oximeter housing to provide proximity accurate feedback when the measurement site is located at a number of different positions relative to the oximeter. Though discussed primarily herein in the context of capacitive sensor electrodes, proximity feedback in pulse oximeters can be provided in other examples by optical, mechanical, or electrical sensors interfacing with skin of a measurement site, or a combination of one or more of capacitive, optical, mechanical, and electrical sensors.

In some embodiments, capacitive sensor electrodes can be used to determine the longitudinal displacement of a patient's finger within a clip-type pulse oximeter sensor housing. Using the determined displacement, the oximeter can determine whether to provide an indication to the patient or physician to reposition the oximeter. The oximeter can additionally or alternatively use the determined displacement to determine whether to mechanically reposition the optical assembly of the oximeter relative to the patient's finger. In oximeters implementing artificial pulsing, the capacitive sensor electrodes can periodically or continuously monitor the longitudinal displacement of the patient's finger within the sensor housing to determine a probe off condition. These examples illustrate some of the many benefits of an oximeter sensor having proximity sensing technology for determining positioning of the sensor relative to a measurement site.

For purposes of summarizing the disclosure, certain aspects, advantages and novel features of the inventions have been described herein. It is to be understood that not necessarily all such advantages can be achieved in accordance with any particular embodiment of the inventions disclosed herein. Thus, the inventions disclosed herein can be embodied or carried out in a manner that achieves or optimizes one advantage or group of advantages as taught herein without necessarily achieving other advantages as can be taught or suggested herein.

BRIEF DESCRIPTION OF THE DRAWINGS

Throughout the drawings, reference numbers can be re-used to indicate correspondence between referenced elements. The drawings are provided to illustrate embodiments of the inventions described herein and not to limit the scope thereof.

FIG. 1A illustrates a high-level diagram of an embodiment of a physiological sensor having proximity sensing capabilities positioned around a patient measurement site.

FIG. 1B illustrates another embodiment of the physiological sensor of FIG. 1A.

FIG. 2A illustrates a perspective view of an embodiment of a physiological sensor having proximity sensing capabilities.

FIGS. 2B and 2C illustrate an exploded view of two components of the physiological sensor of FIG. 2A when disassembled.

FIG. 3A illustrates a perspective view of another embodiment of a physiological sensor having proximity sensing capabilities.

FIG. 3B illustrates a perspective view of the physiological sensor of FIG. 3A in an open position.

FIG. 4 illustrates a high-level schematic block diagram of an embodiment of a physiological sensor having proximity sensing capabilities.

FIG. 5 illustrates a schematic diagram of an embodiment of a circuit for measuring proximity of a measurement site to a sensor.

FIG. 6 illustrates an example process for determining positioning during sensor application.

FIG. 7 illustrates an example process for repositioning an applied sensor based on proximity sensing.

FIG. 8 illustrates an example process for determining a probe off condition based on proximity sensing.

DETAILED DESCRIPTION

I. Introduction

Implementations described herein relate generally to proximity sensing in physiological sensors, and more specifically to using one or more proximity sensors located on or within a physiological sensor to determine the positioning of the physiological sensor on a patient measurement site. Accurate placement of a physiological sensor on the patient measurement site is a key factor in obtaining reliable measurement of physiological parameters of the patient. For example, in clip-type pulse oximeter sensors, longitudinal positioning of the patient's finger within the sensor housing determines which portion of the patient's finger is aligned with an optical assembly used to generate physiological measurement data for determining one or more physiological parameters. Proper alignment with the optical assembly covers a detector of the optical assembly with the patient's fingertip and reduces introduction of ambient light to the detector, and accordingly provides more accurate physiological measurement data. This alignment can be determined based on data from a proximity sensor or sensors placed on or within the physiological sensor. Suitable proximity sensors include one or more capacitive sensors, optical scanning sensors, electrical sensors, or mechanical contact sensors.

The proximity data generated by the proximity sensors on or within a pulse oximeter can enable provision of more accurate physiological measurement data. For example, the proximity sensors described herein can be used to provide an indication to the oximeter to generate feedback for a patient or physician to reposition an improperly aligned oximeter sensor. In another example, the proximity sensors can be used to provide alignment information for mechanically repositioning the optical assembly with respect to the oximeter housing and patient finger. As a further example, the proximity sensors can be used to determine a probe off condition indicating that physiological measurement data obtained during persistence of the probe off condition should be discarded due to improper alignment. In additional examples, the proximity sensors can be used to associate distance data with measurement data output by the sensor, e.g. for assigning a confidence value to the measurement data.

II. Overview of Example Proximity Sensing Physiological Monitoring Systems

FIGS. 1A and 1B illustrate embodiments of a high-level diagram of an embodiment of a physiological sensor having proximity sensing capabilities positioned around a patient measurement site. The sensor 100 can include a first housing component 110 including an emitter 120 and a second housing component 115 including a detector 125. The sensor 100 can also include a physical stop 140 to guide the positioning of a patient finger 130 or other measurement site

within the sensor 100. One or more proximity sensors 145 can be positioned on or within the sensor 100.

The emitter 120 can be configured to emit light having multiple primary wavelengths λ_p into the tissue of the patient finger 130 or other measurement site. The emitter 120 can be comprised of one or more devices such as semi-conductive light emitting diodes (LEDs), although it will be appreciated that other light generating devices may be used. The light emitter 120 may be chosen to emit light at a single known discrete wavelength, at multiple discrete wavelengths, or across a portion of the spectrum (such as that emitted by a "white light" LED), depending on the needs of the particular application. In one embodiment, the emitter 120 consists of two or more diodes emitting light energy in the infrared and red regions of the electromagnetic spectrum, and a parallel resistor (or resistors) used for security. The construction and operation of such light source drive circuitry is described in U.S. Pat. No. 5,758,644 incorporated herein by reference.

The detector 125 can be any suitable light energy detector responsive to light energy from the emitter, for example a semi-conductive photodetector. The emitter 120 and detector 125 can be aligned such that the detector 125 detects the emitted light after attenuation by the tissue of the patient finger 130.

The physical stop 140 can provide tactile feedback to a clinician or patient positioning the finger 130 within the sensor in order to achieve proper positioning. Proper positioning of the patient finger 130 or other tissue site relative to the detector 125 enables accurate physiological measurements to be made. In particular, the emitter 120 is placed so as to illuminate a blood-perfused tissue site 135, such as a nail bed, and the detector 125 is positioned so that only light transmitted by the emitter 120 and attenuated by pulsatile blood flowing within the tissue site 135 is received by the detector 125.

Physical stop 140 can prevent the tissue site 135 from being positioned beyond the emitter 120 and detector 125, that is, too far into the sensor 100. However, the physical stop 140 does not ensure that the tissue site 135 will be placed far enough within the sensor 100 for adequate transmission of light from the emitter 120 through the tissue site 135 to the detector 125 to enable clinically accurate physiological measurements. Accordingly, the sensor 100 can be provided with one or more proximity sensors 145 positioned within the sensor housing. The proximity sensor(s) 145 can be used to determine whether the tissue site 135 is positioned properly relative to the emitter 120 and detector 125.

Proximity sensor 145 can be a capacitive sensor, in some embodiments, that uses capacitance of the human body as an input to determine a distance between the patient's finger 130 and the proximity sensor 145. In another embodiment, proximity sensor 145 can be an optical scanning sensor, for example a camera or a near-infrared proximity sensor that uses light to determine how close or far the patient's finger 130 is from the proximity sensor 145. In still further embodiments, proximity sensor 145 can be a mechanical contact sensor that determines whether physical contact is made between the patient's finger 130 and the proximity sensor 145 mounted on the physical stop 140. Other sensors suitable for determining contact or distance between patient finger 130 and sensor 145 can be used in other embodiments.

As illustrated by FIG. 1A, the physical stop 140 can include a proximity sensor 145. The proximity sensor 145 of FIG. 1A can be used to determine the distance (or whether there is contact) between the location of the proximity

sensor 145 on the physical stop 140 and the end of the patient's finger 130 nearest the stop 140. The proximity sensor 145 can be positioned on the physical stop 140 so as to sense or contact a portion of the patient fingertip below the nail, in particular for embodiments in which a capacitive proximity sensor is implemented. As illustrated by FIG. 1B, an additional array of proximity sensors 145 can be positioned longitudinally along the finger bed of the second housing component 115. The array 150 of proximity sensors can provide additional feedback regarding the longitudinal positioning of the patient finger 130 within the sensor 100.

As illustrated in FIGS. 2A and 2B, an embodiment of a sensor 200 can include a two-piece housing and an electrical supply and signal cable 210. The housing consists of a first (upper) housing element 275 and a second (lower) housing element 255, which can be rotatably attached to one another via a pivot element 265. A light emitter can be disposed within the upper housing element 275, while a detector can be disposed within the lower housing element 255. The housing is adapted to receive the distal end of a finger as shown in the block diagrams of FIGS. 1A and 1B, with the "upper" housing element 275 engaging the upper surface of the finger, and the "lower" housing element engaging the lower surface of the finger. It will be recognized, however, that the sensor 200 may be used in any orientation, such as with the first housing element 275 being located below the second housing element 255. Furthermore, the light emitter may alternatively be placed in the lower housing element 255, and the detector in the upper housing element 275 if desired, subject to modification of other probe components as described further below. It is also noted that while the following discussion describes a series of exemplary embodiments based on measuring the optical characteristics of a finger, the sensor 200 may be adapted for use with any number of other body parts, such as earlobes or loose skin, with equal success. Additional details of an embodiment of the sensor are disclosed in U.S. Pat. No. 6,580,086 entitled "Shield Optical Probe and Method," filed on Oct. 19, 1999 and assigned to Masimo Corporation, the entirety of which is hereby incorporated by reference.

The first and second housing elements 275, 255 can be generally rectangular in form with a pivot element 265 disposed near a common end of each of the elongate housing elements 275, 255. The two housing elements 275, 255 can be biased around the rotational axis of the pivot element by a biasing element, for example a hinge spring. The upper housing element 275 can be accordingly biased against the lower housing element 255 for secure placement on a patient finger or other measurement site. The user can grasp the sensor 200 between his or her fingers and separate the probe housing elements 275, 255 by applying force counter to the spring biasing force. In this fashion, the user simply grasps the sensor 200, opens it by applying a light force with the grasping fingers, and inserts the distal end of the patient's finger into the end 240 of the sensor 200. Once the finger is inserted into the sensor 200, the disproportionate compression of the finger (due to interaction of the angled housing elements 275, 255 and the substantially cylindrical finger) and the aforementioned bias spring separating force act to lower housing elements 275, 255 substantially parallel to each other, allowing more of the surface area of the upper and lower support surface elements 225, 230 to contact the finger, and for more even pressure distribution thereon. This assists with accurate positioning of the finger with respect to the emitter and detector for clinically accurate physiological measurement readings using the sensor 200.

As shown in more detail in FIGS. 2B and 2C, the housing elements 275, 255 can include first (upper) and second (lower) support surface elements 225, 230, respectively, which provide support and alignment for the tissue material, such as the finger, when the sensor 200 is clamped thereon. The upper support surface element 225 can be fashioned from a substantially pliable polymer such as silicone rubber, so as to permit some deformation of the element 225 when in contact with the fairly rigid upper portion 280 of the patient's finger. The upper support surface element 225 further includes an optical energy shield 250 which protrudes from the upper support surface element 225. The shield 250 can be sized and shaped so as to conform substantially to the outer circumference of the patient's finger, providing at least a partial seal against ambient light incident on the probe exterior and otherwise exposed portions of the finger. In this fashion, patients having fingers of different circumferences can be accommodated with the same sensor 200 due to use of shield 250. The lower surface element 230 can be fashioned from a substantially solid and rigid (i.e., higher durometer) polymer. This harder, solid polymer can be used for the lower surface element 230 since the lower portion of the finger is generally more fleshy and deformable, thereby allowing the skin and tissue material thereof to deform and contour to the shape of the inner region 285 of the lower surface element. The inner regions 280, 285 can be contoured to assist in mitigating the effects of patient movement during operation of the sensor 200. Accordingly, the construction of the sensor 200 provides some alignment between the patient finger and the sensor 200 for proper positioning relative to the emitter and detector.

The upper surface element 225 includes an aperture 215 for transmission of light therethrough after emission by the emitter in the upper housing element 275. The lower surface element 230 includes an aperture 235 aligned with the detector for transmission of light therethrough after passing through the measurement site. The apertures 215, 235 allow for light energy to be transmitted between the light emitter and tissue material of the measurement site, and similarly between the tissue material and detector. The first aperture 215 is also axially located with the second aperture 235 in the vertical dimension, such that when the probe 100 is in the closed configuration with the patient's finger disposed between the upper and lower surface support elements 225, 230, light emitted by the light source through the first aperture 215 is transmitted through the finger and the second aperture 235 and received by the detector. Hence, the light source, first aperture 215, second aperture 235, and detector are substantially axial in this configuration.

The lower support element 230 is further provided with a physical stop 290 disposed near the pivot element of the sensor 200. The physical stop 290 is oriented vertically with respect to the lower support element 230 so as to stop the distal end of the patient's finger from being inserted into the probe past a certain point, thereby facilitating proper alignment of the finger within the sensor 200, especially with respect to the source and detector apertures 215, 235. While the present embodiment uses a semi-circular tab as the physical stop 290, it will be recognized that other configurations and locations of the physical stop 290 may be used. For example, the tab could be bifurcated with a portion being located on the upper support surface element 230, and a portion on the lower support surface element 225. Alternatively, the positioning element could be in the form of a tapered collar which receives, aligns, and restrains only the distal portion of the patient's finger. Many such alternative

embodiments of the positioning element are possible, and considered to be within the scope of the present invention.

A proximity sensor **295** is positioned on the physical stop **290** that can be used to determine whether the patient finger or other measurement site is positioned properly within the sensor **200**. As discussed above, proximity sensor **295** can be a capacitive sensor, an optical scanning sensor, or a mechanical contact sensor, or a combination of two or more of these sensors in some embodiments. Proximity sensor **295** provides feedback regarding distance or contact between the patient finger and the proximity sensor **295** located on physical stop **290**, and accordingly can be used to determine whether the patient finger is aligned with the emitter and detector of the sensor **200**. This feedback can be used to provide a repositioning indication to the user of the sensor **200**, to mechanically reposition the optical components of the sensor **200**, or for data filtering, as described in more detail below. Accordingly, the feedback from the proximity sensor **295** can enable more accurate physiological measurements using the sensor **200**.

FIGS. 3A and 3B illustrate another embodiment of a sensor **300**. The sensor **300** shown can include all of the features of the sensors **100** and **200** described above.

Referring to FIG. 3A, the sensor **300** in the depicted embodiment is a clothespin-shaped clip sensor that includes an enclosure **302a** for receiving a patient's finger. The enclosure **302a** is formed by an upper housing or emitter shell **304a**, which is pivotably connected with a lower housing or detector shell **306a**. The emitter shell **304a** can be biased with the detector shell **306a** to close together around a pivot point **303a** and thereby sandwich finger tissue between the emitter and detector shells **304a**, **306a**.

In an embodiment, the pivot point **303a** advantageously includes a pivot capable of adjusting the relationship between the emitter and detector housings **304a**, **306a** to effectively level the sections when applied to a tissue site. In another embodiment, the sensor **300** includes some or all features of the finger clip described in U.S. Pat. No. 8,437, 825, entitled "Contoured Protrusion for Improving Spectroscopic Measurement of Blood Constituents," filed on Jul. 2, 2009 and assigned to Cercacor Laboratories, the entirety of which is hereby incorporated by reference. For example, the sensor **300** can include a spring that causes finger clip forces to be distributed along the finger.

The emitter housing **304a** can position and house various emitter components of the sensor **301a**. It can be constructed of reflective material (e.g., white silicone or plastic) and/or can be metallic or include metalized plastic (e.g., including carbon and aluminum) to possibly serve as a heat sink including one or more fins **351a**. The emitter housing **304a** can also include absorbing opaque material, such as, for example, black or grey colored material, at various areas, such as on one or more flaps **307a**, to reduce ambient light entering the sensor **301a**. The emitter housing **304a** can also include optical shield **307a** to block ambient light from entering the sensor **300**.

The detector housing **306a** can position and house one or more detector portions of the sensor **301a**. The detector housing **306a** can be constructed of reflective material, such as white silicone or plastic. As noted, such materials can increase the usable signal at a detector by forcing light back into the tissue and measurement site (see FIG. 1). The detector housing **306a** can also include absorbing opaque material at various areas, such as lower area **308a**, to reduce ambient light entering the sensor **301a**.

Referring to FIG. 3B, an example of finger bed **310** is shown in the sensor **301b**. The finger bed **310** includes a

generally curved surface shaped generally to receive tissue, such as a human digit. The finger bed **310** includes one or more ridges or channels **314**. Each of the ridges **314** has a generally convex shape that can facilitate increasing traction or gripping of the patient's finger to the finger bed. Advantageously, the ridges **314** can improve the accuracy of spectroscopic analysis in certain embodiments by reducing noise that can result from a measurement site moving or shaking loose inside of the sensor **301a**. The ridges **314** can be made from reflective or opaque materials in some embodiments to further increase signal to noise ration (SNR). In other implementations, other surface shapes can be used, such as, for example, generally flat, concave, or convex finger beds **310**.

Finger bed **310** can also include an embodiment of a tissue thickness adjuster or protrusion **305**. The protrusion **305** includes a measurement site contact area **370** that can contact body tissue of a measurement site. The protrusion **305** can be removed from or integrated with the finger bed **310**. Interchangeable, different shaped protrusions **305** can also be provided, which can correspond to different finger shapes, characteristics, opacity, sizes, or the like. In some embodiments, protrusion **305** can include one or more proximity sensors to determine positioning of a patient finger over the protrusion **305**.

The detector housing **306a** can also include a physical stop **350** to prevent a patient's finger from being longitudinally placed too far into the sensor for proper alignment with the emitter and detector. Proper positioning of the patient finger or other tissue site relative to the detector enables accurate physiological measurements to be made. The physical stop **350** can include one or more proximity sensors **355** for determining distance or contact between the end of the patient's finger and the proximity sensor **355** to provide feedback regarding alignment of the patient's finger with the emitter and detector. As described above, the proximity sensor **355** can be a capacitive sensor, optical scanning sensor, or mechanical contact sensor. Data from proximity sensor **355** can be used to determine whether the patient finger is aligned with the emitter and detector of the sensor **300**. This feedback can be used to provide a repositioning indication to the user of the sensor **300**, to mechanically reposition the optical components of the sensor **200**, or for data filtering, as described in more detail below. Accordingly, the feedback from the proximity sensor **295** can enable more accurate physiological measurements using the sensor **200**.

In a vascular bed the arterial vasculature is coupled mechanically to the venous vasculature through the tissues. Although this coupling is small, the optical arterial pulse, e.g. photo-plethysmograph, has invariably a small venous component. This component is not fixed across subjects but its average is indirectly calibrated for in the saturation calibration curve. Its effect on the arterial pulse is proportional to the coupling size as well as the difference between the arterial and venous saturations at the site. Its effects may be explained by the reduction in the optical effect of venous coupling as the delta saturation between the arterial and the venous is reduced due to the increase in availability of plasma oxygen. Under this condition, the venous blood will look, optically, a lot like the arterial blood. Hence, the size of the Red photo-plethysmograph signal will shrink with respect to the IR indicating a shrinking ΔSat , i.e. higher venous saturation. In 1995, Masimo Corporation (Masimo) introduced a new technique for calculation the venous

oxygen saturation (SpvO₂) by introducing an artificial pulse into the digit (see, e.g., U.S. Pat. No. 5,638,816, incorporated herein by reference).

The sensor **300** depicted in FIGS. 3A and 3B can be capable of introducing an artificial pulse into the measurement site. The sensor **300** can induce an artificial pulse at a frequency distinguishable from the frequency of a human arterial pulse. As a result, information related to both the arterial pulse as well as the artificial pulse is recoverable from the body. The redundant nature of both pieces of information provide additional information useful in determining physiological parameters.

Introducing an artificial excitation can cause perturbations in the blood flow similar to the effects of a heart beat. These artificial excitations can be used as an alternative to the natural pulse rate or in addition to the natural pulse rate. Artificial excitations have the added benefit that the excitations introduced are introduced at known frequencies. Thus, it is not necessary to first determine the pulse rate of an individual.

However, the movement required to generate the artificial pulse can cause movement of the sensor relative to the patient, introducing the variable of distance into denoising equations for the resultant sensor data. For example, the artificial pulse can dislodge the sensor **300** from the patient measurement site or misalign the measurement site with the emitter and detector of the sensor **300**. Accordingly, sensor data from active pulse sensors typically is filtered to determine probe off and probe on conditions, where probe on conditions indicate reliable sensor data and probe off conditions include their ordinary broad meaning known to one of skill in the art, including designating improper application of an optical probe to a measurement site, for example due to movement of the sensor relative to the patient caused by artificial pulsing.

Data from the proximity sensor **355** within the sensor **300** can be used instead of or in addition to more complex data processing methods to determine a probe off condition due to improper alignment of the measurement site and the sensor. For example, if data from the proximity sensor **355** indicates that the measurement site is not properly aligned with the sensor **300**, then the sensor **300** can determine a probe off condition for the duration of such data from the proximity sensor **355**. Accordingly, data from proximity sensor **355** can provide a computationally simple and accurate means for determining the probe off condition.

In some embodiments, instead of or in addition to using proximity data to determine a probe off condition, data from the proximity sensor **355** can be used to generate a confidence value indicating potential accuracy of measurement data, e.g., plethysmographic data output by a pulse oximeter. For example, during operation a sensor can supply associated proximity data and plethysmographic data to a patient monitor without utilizing probe-off detection or probe repositioning. The patient monitor can then determine a confidence value for each portion of the plethysmographic data based on the associated proximity data, for example a measured distance between a fingertip and a capacitive proximity sensor measured at substantially the same time as when the plethysmographic data was captured. Using the confidence values for the plethysmographic data (e.g., to discard certain portions of the plethysmographic data or to assign different weights to different portions of the plethysmographic data), the patient monitor can estimate pulse rates, respiration rates, and the like for the patient.

FIG. 4 illustrates a high-level schematic block diagram of an embodiment of a physiological sensor **400** having prox-

imity sensing capabilities. The physiological sensor **400** includes an emitter **405**, detector **410**, processor **415**, and capacitive sensor **420**. In other embodiments the capacitive sensor **420** can be replaced or supplemented by the other types of proximity sensors discussed herein. Various embodiments of the sensor **400** can also include one or more of a set of optional components such as positioning feedback indicator **425**, repositioning module **430**, emitter drive **440**, or detector drive **435**. Though not illustrated, the sensor **400** can also include memory, a display, connection ports, user interface elements, alarms, and other components.

The emitter **405** can be capable of emitting light at one or a plurality of wavelengths λ_p for noninvasive measurement of constituents of blood flowing within the tissue of a patient measurement site. The emitter **405** and detector **410** can be aligned so that some or all of the light λ_p is incident on detector **410** after passage through the measurement site and attenuation by the constituents of the blood.

Intensity signals representing the light λ_p incident on detector **410** can be sent to processor **415**. Processor **415** can analyze the intensity signals and determine one or more physiological parameter values. For example, processor **415** can calculate a ratio of detected red and infrared intensities, and an arterial oxygen saturation value is empirically determined based on that ratio. Processor **415** can also perform noise filtering on the raw intensity signal data, and can determine probe off and probe on conditions for purposes of excluding unreliable data from use in calculating physiological parameters. Data from the capacitive sensor **420** can provide feedback regarding the distance of a patient measurement from the capacitive sensor, which can be compared to a threshold to determine whether the sensor and finger are improperly aligned. The determination of improper alignment can be used by the processor **415** in one embodiment to determine a probe off condition.

In some embodiments, the processor **415** can generate a repositioning signal based at least partly on the determination of improper alignment from capacitive sensor data. This signal can be sent, in one embodiment, to positioning feedback indicator **425**. Positioning feedback indicator **425** can provide visual, audible, or tactile feedback to a user of sensor **400** to indicate whether the sensor should be repositioned. For example, sensor **400** may emit a beep or audible alarm when the sensor **400** is improperly positioned. Sensor **400** may also include one or more visual indications, for example LED lights, that can be used to provide positioning feedback to the user. For instance, a green light may be illuminated to indicate to the user that the sensor **400** is properly positioned. A red light may be illuminated to indicate to the user that sensor **400** is improperly positioned. As another example, sensor **400** may output text or voice commands indicating how far the user must adjust the sensor **400** in order to achieve proper alignment based on the proximity sensor data. Positioning feedback indicator **425** can provide an initial positioning indication when the user first applies the sensor in one embodiment. In some embodiments, positioning feedback indicator **425** can periodically or continuously output positioning feedback to the user, for example for active pulse sensors introducing an artificial pulse during measurement.

The repositioning signal can be sent, in another embodiment, to repositioning module **430**. Repositioning module **430** can use the repositioning signal to generate instructions for mechanical repositioning of the emitter **405** and detector **410**, for example using emitter drive **440** and detector drive **435**. In some embodiments, emitter drive **440** and detector drive **435** could be implemented together as a single optical

assembly drive. Emitter drive **440** and detector drive **435** can be used to reposition the emitter **405** and detector **410**, respectively, according to the data provided by the capacitive sensor **420** in order to align the emitter **405** and detector **410** with the measurement site.

As discussed above with respect to the sensors of FIGS. 1A-3B, the capacitive sensor **420** can be placed within the body of the sensor **400** to gauge longitudinal displacement of a patient's finger relative to the sensor **400** and, more specifically, the optical assembly including the emitter **405** and detector **410**. In some embodiments, multiple capacitive sensors can be positioned along a longitudinal axis of the sensor **400** for additional data as the patient's finger moves within the sensor housing.

III. Overview of Example Capacitive Proximity Sensor

FIG. 5 illustrates a schematic diagram of an embodiment of a circuit **500** that can be used to determine proximity of a patient measurement site to a physiological sensor. The circuit includes a capacitor **515** and a resistor **505**. Here the capacitance, C , can be calculated according to Equation (1), below:

$$C \propto \frac{A}{d} \quad (1)$$

where the capacitance, C , is proportional to the area, A , of the capacitor divided by the distance, d , between the capacitor plates. The capacitor **515** has two plates **510**, **520**. The first capacitive plate **510** is integrated or connected to the physiological sensor, for example a physical stop near the hinge of the housing of clip-type pulse oximeter, or in an array along the longitudinal axis of the surface of a finger bed of clip-type pulse oximeter. The second capacitor plate **520** is the skin surface of the patient measurement site, with the assumption that the patient is a capacitor. A typical adult has a capacitance of about 120 pF, however capacitance of different people will vary. Accordingly, the distance, d , between the capacitor plates **510**, **520** represents the distance between the location of the capacitive sensor within the physiological sensor and the surface of the patient measurement site. In order to obtain the value of the distance, d , from Equation (1), the values of both the capacitance, C , and the area, A , must be known. The area can be predetermined based on the dimensions of the first capacitive plate **510**.

The capacitance can be determined from the value of the resistance, R , of the resistor **505** and the value of a time constant, τ , of the circuit **500**. The time constant of the circuit **500** can be calculated according to Equation (2), below:

$$\tau = RC \quad (2)$$

where the time constant, τ , is equal to the resistance, R , times the capacitance, C . Hence, the distance, d , between the capacitor plates **510**, **520** can be calculated through the combination of Equations (1) and (2) through the measurement of the circuit time constant. Accordingly, as a distance between a patient measurement site, such as a digit of a hand, and the capacitor plate **510** decreases, the time constant τ increases and the capacitance C increases.

In one embodiment, the time constant τ can be determined from the time required to trip a set voltage level, such as about 2.2 volts, given a power supply of known power, such as about 3.3 volts. Although not illustrated, a processor or microprocessor can be in communication with the circuit **500** to measure the time constant. The determined time constant τ can be used to calculate the capacitance, C , using

Equation (2). The capacitance C can then be used to calculate the distance or relative distance through Equation (1). Accordingly, as a distance between a patient measurement site, such as a digit of a hand, and the capacitor plate **510** decreases, the time constant τ increases and the capacitance C increases.

The value of the distance d can be used to provide a repositioning indication to the patient or physician, to mechanically reposition the optical assembly of an oximeter sensor, or to determine a probe off condition for removing potentially unreliable data from a physiological measurement data set. In some embodiments, a number of circuits **500** can be provided within an oximeter for precise determination of longitudinal displacement of a patient finger within the oximeter housing. Accordingly, at least one of the repositioning indication, optical assembly repositioning, or probe off can be based on a number of distance values corresponding to each of the circuits. Although an example capacitive circuit **500** is depicted, this is for purposes of illustration and in other embodiments other capacitive circuit arrangements can be used. For example, other suitable circuits can include amplifiers, additional resistors, and other elements, for instance to amplify the signal to noise and to minimize changes to capacitance based on environmental changes.

IV. Overview of Example Proximity-Sensing Physiological Monitoring Processes

FIG. 6 illustrates an example process **600** for determining positioning during sensor application. The process **600** can be implemented on any physiological sensor including proximity sensing capabilities, for example the physiological sensors illustrated in FIGS. 1A-FIG. 4.

At block **605**, a physiological sensor is provided with at least one proximity sensor. For example, one proximity sensor or an array of proximity sensors can be provided including capacitive, optical, electrical, or mechanical proximity sensors, or a combination thereof. The proximity sensor can be configured to determine distance or contact between a measurement site and itself, and can be positioned within the sensor so as to provide feedback regarding alignment of the measurement site and optical components of the sensor.

At block **610**, the patient measurement site location is detected using the proximity sensor. For example, using a capacitive proximity sensor, a distance between a capacitive plate in the sensor and the capacitive skin of the patient can be determined. An optical scanning proximity sensor can also determine a distance between the sensor and a patient measurement site. In another example, using a mechanical contact proximity sensor, it can be determined whether the patient measurement site has contacted the mechanical contact proximity sensor, such as by depressing a button.

At block **615**, the measurement site location can be compared to preferred positioning. The preferred positioning can include a range of placements relative to the optical components of the sensor that are likely to produce clinically accurate physiological measurements. To illustrate, if a capacitive proximity sensor is used on a physical stop in a pulse oximeter finger clip sensor such as is depicted in FIG. 2A, 2B, 3A, or 3B, a distance of approximately 4 mm-10 mm between the capacitive proximity sensor and the patient fingertip can correspond to proper positioning of an adult finger with respect to an LED emitter and detector. In one embodiment, a distance of approximately 6 mm between the capacitive sensor and the fingertip can indicate preferred positioning of the finger within the sensor. Other ranges can

be used to indicate preferred placement in other sensor configurations, for other finger sizes, or for other measurement sites.

At block **620**, the sensor can optionally cause the sensor to output a repositioning indication. For instance, in one embodiment of a pulse oximeter finger clip sensor such as is depicted in FIG. 2A, 2B, 3A, or 3B having a capacitive sensor on a physical stop, if the capacitive proximity sensor data indicates that the patient fingertip is closer than approximately 4 mm to the capacitive sensor or farther than approximately 10 mm from the capacitive sensor, the sensor may output a repositioning indication. In some embodiments, the sensor may output a first positioning indication when the sensor is correctly positioned and may output a second positioning indication when the sensor is incorrectly positioned. The second positioning indication may be a visual, auditory, or tactile signal alerting the user that the sensor is incorrectly positioned, and in one example may include specific instructions regarding how to reposition the sensor for proper placement.

Process **600** can be implemented when a user first applies a sensor to a measurement site to indicate proper positioning. In some embodiments, blocks **610-620** may be repeated one or more times during measurement to gauge whether the sensor positioning continues to be proper or whether the sensor should be repositioned. Repetition of this measurement site location detection and comparison portion of process **600** can be beneficial, in one example, in active pulse oximeters that introduce an artificial pulse to a measurement site and therefore possibly introduce movement of the sensor relative to the measurement site. Repetition of blocks **610-620** can also be beneficial, in another example, in patient monitoring situations in which the patient can move during the time in which the sensor is worn and therefore may dislodge the sensor.

FIG. 7 illustrates an example process **700** for repositioning an applied sensor based on proximity sensing. The process **700** can be implemented by the components of any physiological sensor including proximity sensing capabilities, for example the physiological sensors illustrated in FIGS. 1A-FIG. 4.

At block **705**, a physiological sensor is provided with at least one proximity sensor. For example, one proximity sensor or an array of proximity sensors can be provided including capacitive, optical, electrical, or mechanical proximity sensors, or a combination thereof. The proximity sensor can be configured to determine distance or contact between a measurement site and itself, and can be positioned within the sensor so as to provide feedback regarding alignment of the measurement site and optical components of the sensor. The physiological sensor also includes an optical assembly, for instance an aligned emitter and detector as discussed above with respect to FIGS. 1A-FIG. 4, for generating intensity signals from which to determine physiological signals.

At block **710**, the sensor determines longitudinal displacement of a patient finger in the physiological sensor using the proximity sensor. Many pulse oximeters are contoured to naturally center a patient finger within the sensor, and therefore the proximity sensing discussed herein focuses primarily on determining longitudinal displacement. However, in other sensor embodiments displacement of the measurement site along a vertical or horizontal axis of the sensor may alternatively or additionally be determined. For example, using a capacitive proximity sensor, a distance between a capacitive plate in the sensor and the capacitive skin of the patient can be determined. An optical scanning

proximity sensor can also determine a distance between the sensor and a patient measurement site. In another example, using a mechanical contact proximity sensor, it can be determined whether the patient measurement site has contacted the mechanical contact proximity sensor, such as by depressing a button.

At block **715**, the sensor determines whether the patient measurement site is correctly positioned relative to the optical assembly based on the proximity sensor data. As discussed above, for capacitive proximity sensors the distance between the capacitive proximity sensor and the skin of the measurement site can be compared to a threshold or to a range of acceptable positions to determine whether the measurement site is correctly positioned. For a mechanical contact sensor producing a binary contact or no contact output, the correct positioning determination may be made based on the binary output.

If the measurement site is positioned correctly relative to the optical assembly, then the process **700** ends. If the measurement site is not positioned correctly relative to the optical assembly, then the process **700** transitions to block **720** in which the sensor mechanically repositions the optical assembly to achieve proper alignment with the measurement site. For example, capacitive sensing data can be used to determine a distance to mechanically move the optical assembly along the longitudinal axis of the sensor.

FIG. 8 illustrates an example process **800** for determining a probe off condition based on proximity sensing. The process **800** can be implemented by the components of any physiological sensor including proximity sensing capabilities, for example the physiological sensors illustrated in FIGS. 1A-FIG. 4. Some embodiments of process **800** can be implemented on an active pulse sensor capable of introducing an artificial pulse into a measurement site.

At block **805**, a physiological sensor is provided with at least one proximity sensor. For example, one proximity sensor or an array of proximity sensors can be provided including capacitive, optical, electrical, or mechanical proximity sensors, or a combination thereof. The proximity sensor can be configured to determine distance or contact between a measurement site and itself, and can be positioned within the sensor so as to provide feedback regarding alignment of the measurement site and optical components of the sensor.

At block **810**, the sensor optionally introduces an artificial pulse to the patient measurement site, such as a finger positioned within a pulse oximeter. As discussed above, the artificial pulse can assist in obtaining more reliable measurement data, however it can also cause movement of the sensor relative to the measurement site, thereby affecting proper positioning of the sensor on the measurement site.

At block **815**, the patient measurement site location is detected using the proximity sensor. As discussed above, in some embodiments of a finger clip pulse oximeter the sensor may be placed on a physical stop, and may be oriented to determine longitudinal displacement of the patient finger within the sensor relative to the optical assembly. In one example, using a capacitive proximity sensor, a distance between a capacitive plate in the sensor and the capacitive skin of the patient can be determined. An optical scanning proximity sensor can also determine a distance between the sensor and a patient measurement site. In another example, using a mechanical contact proximity sensor, it can be determined whether the patient measurement site has contacted the mechanical contact proximity sensor, such as by depressing a button.

At block **820**, the measurement site location can be compared to preferred positioning data to determine whether the oximeter is correctly applied to the measurement site. Preferred positioning data can be stored in memory of the oximeter, for example a read-only memory (ROM). The preferred positioning can include a range of placements relative to the optical components of the sensor that are likely to produce clinically accurate physiological measurements. In one embodiment, if a capacitive proximity sensor is used on a physical stop in a pulse oximeter finger clip sensor such as is depicted in FIG. 2A, 2B, 3A, or 3B, a distance of approximately 4 mm-10 mm between the capacitive proximity sensor and the patient fingertip can correspond to proper positioning of an adult finger with respect to an LED emitter and detector. As an example, a distance of approximately 6 mm between the capacitive sensor and the fingertip can indicate preferred positioning of the finger within the sensor. As discussed above, other ranges can be used to indicate preferred placement in other sensor configurations, for other finger sizes, or for other measurement sites.

At block **825**, the sensor determines based on the comparison of block **810** whether the oximeter is correctly applied to the measurement site. If the sensor is not correctly applied, then the process **800** transitions to block **830** in which the sensor, for example a processor of the sensor or a processor of another device connected to and receiving data from the sensor, determines a probe off condition for discarding the data taken while the sensor was not correctly applied. In some embodiments, a default may be to determine a probe on condition for including data, and data may only be discarded when a probe off condition is determined for a time or range of times during which sensor data was gathered at improper positioning.

After determining the probe off condition at block **830**, or if the sensor is determined at block **825** to be correctly applied, the process **800** transitions to block **835** to determine whether measurement is continuing. If measurement continues, then the process **800** loops back to block **815** to determine the measurement site location and to repeat blocks **820** and **825**. Once measurement has concluded, for instance when the sensor is powered off or if the sensor detects that the patient measurement site is no longer at least partially within the sensor housing, then the process **800** ends.

V. Terminology

Although many of the examples discussed herein are in the context of pulse oximetry, this is for illustrative purposes only. The sensors, signal conditioning techniques, and proximity sensing applications discussed herein can be adapted for other physiological sensors monitoring other physiological parameters or multiple physiological parameters.

Many other variations than those described herein will be apparent from this disclosure. For example, depending on the embodiment, certain acts, events, or functions of any of the algorithms described herein can be performed in a different sequence, can be added, merged, or left out all together (e.g., not all described acts or events are necessary for the practice of the algorithms). Moreover, in certain embodiments, acts or events can be performed concurrently, e.g., through multi-threaded processing, interrupt processing, or multiple processors or processor cores or on other parallel architectures, rather than sequentially. In addition, different tasks or processes can be performed by different machines and/or computing systems that can function together.

The various illustrative logical blocks, modules, and algorithm steps described in connection with the embodiments disclosed herein can be implemented as electronic hardware, computer software, or combinations of both. To clearly illustrate this interchangeability of hardware and software, various illustrative components, blocks, modules, and steps have been described above generally in terms of their functionality. Whether such functionality is implemented as hardware or software depends upon the particular application and design constraints imposed on the overall system. The described functionality can be implemented in varying ways for each particular application, but such implementation decisions should not be interpreted as causing a departure from the scope of the disclosure.

The various illustrative logical blocks and modules described in connection with the embodiments disclosed herein can be implemented or performed by a machine, such as a general purpose processor, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field programmable gate array (FPGA) or other programmable logic device, discrete gate or transistor logic, discrete hardware components, or any combination thereof designed to perform the functions described herein. A general purpose processor can be a microprocessor, but in the alternative, the processor can be a controller, microcontroller, or state machine, combinations of the same, or the like. A processor can also be implemented as a combination of computing devices, e.g., a combination of a DSP and a microprocessor, a plurality of microprocessors, one or more microprocessors in conjunction with a DSP core, or any other such configuration. Although described herein primarily with respect to digital technology, a processor can also include primarily analog components. For example, any of the signal processing algorithms described herein can be implemented in analog circuitry. A computing environment can include any type of computer system, including, but not limited to, a computer system based on a microprocessor, a mainframe computer, a digital signal processor, a portable computing device, a personal organizer, a device controller, and a computational engine within an appliance, to name a few.

The steps of a method, process, or algorithm described in connection with the embodiments disclosed herein can be embodied directly in hardware, in a software module executed by a processor, or in a combination of the two. A software module can reside in RAM memory, flash memory, ROM memory, EPROM memory, EEPROM memory, registers, hard disk, a removable disk, a CD-ROM, or any other form of non-transitory computer-readable storage medium, media, or physical computer storage known in the art. An exemplary storage medium can be coupled to the processor such that the processor can read information from, and write information to, the storage medium. In the alternative, the storage medium can be integral to the processor. The processor and the storage medium can reside in an ASIC. The ASIC can reside in a user terminal. In the alternative, the processor and the storage medium can reside as discrete components in a user terminal.

Conditional language used herein, such as, among others, "can," "might," "may," "e.g.," and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodiments necessarily include logic for deciding, with or without

author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment. The terms “comprising,” “including,” “having,” and the like are synonymous and are used inclusively, in an open-ended fashion, and do not exclude additional elements, features, acts, operations, and so forth. Also, the term “or” is used in its inclusive sense (and not in its exclusive sense) so that when used, for example, to connect a list of elements, the term “or” means one, some, or all of the elements in the list.

Disjunctive language such as the phrase “at least one of X, Y, or Z,” unless specifically stated otherwise, is otherwise understood with the context as used in general to present that an item, term, etc., may be either X, Y, or Z, or any combination thereof (e.g., X, Y, and/or Z). Thus, such disjunctive language is not generally intended to, and should not, imply that certain embodiments require at least one of X, at least one of Y, or at least one of Z to each be present.

Unless otherwise explicitly stated, articles such as “a” or “an” should generally be interpreted to include one or more described items. Accordingly, phrases such as “a device configured to” are intended to include one or more recited devices. Such one or more recited devices can also be collectively configured to carry out the stated recitations. For example, “a processor configured to carry out recitations A, B and C” can include a first processor configured to carry out recitation A working in conjunction with a second processor configured to carry out recitations B and C.

While the above detailed description has shown, described, and pointed out novel features as applied to various embodiments, it will be understood that various omissions, substitutions, and changes in the form and details of the devices or algorithms illustrated can be made without departing from the spirit of the disclosure. As will be recognized, certain embodiments of the inventions described herein can be embodied within a form that does not provide all of the features and benefits set forth herein, as some features can be used or practiced separately from others. It should be emphasized that many variations and modifications may be made to the above-described embodiments, the elements of which are to be understood as being among other acceptable examples. All such modifications and variations are intended to be included herein within the scope of this disclosure and protected by the following claims.

What is claimed is:

1. A physiological monitoring system comprising:

an optical assembly including an emitter configured to at least emit light at one or more wavelengths when in use and a detector aligned with the emitter to detect at least a portion of the light, the detector configured to at least generate intensity signals representing detected light when in use;

a sensor housing configured to at least accept a measurement site of a patient, the sensor housing comprising: a first housing component including the emitter, a second housing component including the detector, and

a proximity sensor positioned on one or both of the first housing component and the second housing component; and

a processor configured to at least:

receive data from the proximity sensor representing positioning of the measurement site relative to the proximity sensor,

based at least partly on the data from the proximity sensor, determine that a distance between the proximity sensor and the measurement site does not

correspond to correct positioning of the measurement site relative to the emitter and the detector, and based at least partly on the distance, generate instructions for at least one drive to reposition one or both of the emitter and detector to align with the measurement site.

2. The system of claim 1, wherein the proximity sensor comprises a capacitor.

3. The system of claim 2, wherein the proximity sensor is configured to generate capacitive sensor data representing a distance between the measurement site and the proximity sensor.

4. The system of claim 3, wherein the processor is configured to determine the positioning of the measurement site relative to the emitter and the detector based at least partly on the distance between the measurement site and the proximity sensor.

5. The system of claim 1, the second housing component comprising a physical stop positioned to contact the measurement site when inserted into the sensor housing and configured to assist in positioning the measurement site relative to the detector.

6. The system of claim 5, wherein the proximity sensor is located along a surface of the physical stop.

7. The system of claim 1, the second housing component comprising a finger bed including a generally curved surface shaped generally to receive the measurement site, the finger bed including an aperture over the detector.

8. The system of claim 7, further comprising a plurality of proximity sensors positioned in an array along a longitudinal axis of the finger bed.

9. The system of claim 1, wherein the proximity sensor comprises one or more of an optical, mechanical, or electrical sensor configured to interface with skin of a measurement site.

10. The system of claim 1, wherein the processor is further configured to:

determine improper alignment of the measurement site and detector based at least partly on the distance; and generate a repositioning signal indicating that the measurement site should be repositioned within the sensor housing.

11. The system of claim 10, wherein the processor is configured to generate the instructions for the at least one drive based at least partly on the repositioning signal.

12. The system of claim 1, further comprising the at least one drive, wherein the at least one drive is configured for mechanically repositioning the one or both of the emitter and the detector along a longitudinal axis of the sensor housing based at least partly on the instructions.

13. The system of claim 1, wherein the processor is configured to compare the positioning of the measurement site relative to the emitter and the detector to a preferred positioning.

14. The system of claim 13, wherein the processor is configured to determine improper alignment based at least partly on comparing the positioning of the measurement site relative to the optical assembly to the preferred positioning.

15. The system of claim 14, wherein the processor is configured to determine a probe off condition based on the improper alignment, and to discard any data obtained from the detector during persistence of the probe off condition.

16. The system of claim 1, wherein the processor is configured to determine one or more physiological parameter values based on the positioning of the measurement site relative to the emitter and the detector and on the intensity signals received from the detector.

19

17. The system of claim **16**, wherein the processor is configured to generate a confidence value for each portion of the intensity signals received from the detector based on corresponding data received from the proximity sensor.

18. The system of claim **17**, wherein, to determine the one 5 or more physiological parameter values, the processor is configured to discard or assign a weight to each portion of the intensity signals received from the detector based on the associated confidence value.

* * * * *

10

20

专利名称(译)	脉搏血氧仪中的接近传感器		
公开(公告)号	US10231670	公开(公告)日	2019-03-19
申请号	US14/743479	申请日	2015-06-18
[标]申请(专利权)人(译)	CERCACOR LAB		
申请(专利权)人(译)	CERCACOR LABORATORIES , INC.		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	BLANK THOMAS B OLSEN GREGORY A DALVI CRISTIANO		
发明人	BLANK, THOMAS B. OLSEN, GREGORY A. DALVI, CRISTIANO VO, HUNG T.		
IPC分类号	A61B5/00 A61B5/1455		
CPC分类号	A61B5/6844 A61B5/14552 A61B5/6826 A61B5/684 A61B2562/0257		
代理机构(译)	KNOBBE , MARTENS , 奥尔森 & BEAR LLP		
优先权	62/014611 2014-06-19 US		
其他公开文献	US20150366507A1		
外部链接	Espacenet		

摘要(译)

公开了用于生理传感器中的接近感测的系统和方法，并且更具体地，公开了使用位于生理传感器上或内的一个或多个接近传感器来确定生理传感器在患者测量部位上的定位。在患者测量部位上准确放置生理传感器是获得患者生理参数的可靠测量的关键因素。测量位置和传感器光学组件之间的适当对准提供了更准确的生理测量数据。可以基于来自接近传感器或放置在生理传感器上或内的传感器的数据来确定该对准。

