



US010398334B2

(12) **United States Patent**
Felix et al.

(10) **Patent No.:** **US 10,398,334 B2**
(45) **Date of Patent:** **Sep. 3, 2019**

(54) **SELF-AUTHENTICATING
ELECTROCARDIOGRAPHY MONITORING
CIRCUIT**

(71) Applicant: **Bardy Diagnostics, Inc.**, Charlotte, NC
(US)

(72) Inventors: **Jason Felix**, Vashon Island, WA (US);
Gust H. Bardy, Carnation, WA (US);
Jon Mikalsen Bishay, Seattle, WA
(US)

(73) Assignee: **Bardy Diagnostics, Inc.**, Seattle, WA
(US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 64 days.

(21) Appl. No.: **15/602,007**

(22) Filed: **May 22, 2017**

(65) **Prior Publication Data**

US 2017/0251948 A1 Sep. 7, 2017

Related U.S. Application Data

(63) Continuation of application No. 14/082,066, filed on
Nov. 15, 2013, now Pat. No. 9,655,538, which is a
(Continued)

(51) **Int. Cl.**
A61B 5/0408 (2006.01)
A61B 5/0432 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/04087** (2013.01); **A61B 5/0006**
(2013.01); **A61B 5/0022** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC . A61B 5/0408; A61B 5/0432-5/04325; A61B
5/6832-5/6833; A61B 2560/0408;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,215,136 A 11/1965 Holter et al.
3,569,852 A 3/1971 Berkovits
(Continued)

FOREIGN PATENT DOCUMENTS

DE 19955211 5/2001
EP 1859833 11/2007
(Continued)

OTHER PUBLICATIONS

15 of the Hottest Wearable Gadgets, URL <<http://thehottestgadgets.com/2008/09/the-15-hottest-wearable-gadgets-001253>> (Web page
cached on Sep. 27, 2008).

(Continued)

Primary Examiner — Lee S Cohen

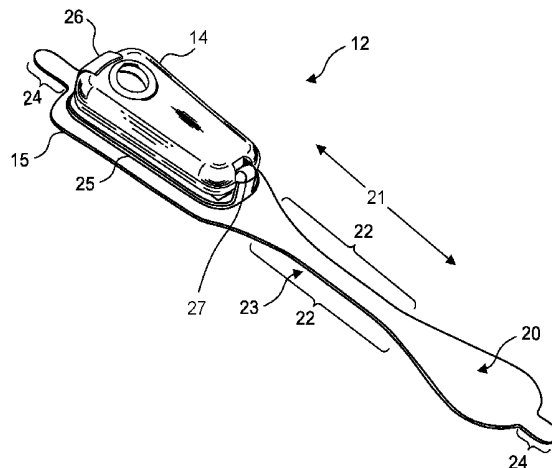
Assistant Examiner — Erin M Cardinal

(74) *Attorney, Agent, or Firm* — Krista A. Wittman

(57) **ABSTRACT**

Physiological monitoring can be provided through a wear-
able monitor that includes two components, a flexible
extended wear electrode patch and a removable reusable
monitor recorder. The wearable monitor sits centrally (in the
midline) on the patient's chest along the sternum oriented
top-to-bottom. The placement of the wearable monitor in a
location at the sternal midline (or immediately to either side
of the sternum) benefits extended wear by removing the
requirement that ECG electrodes be continually placed in
the same spots on the skin throughout the monitoring period.
Instead, the patient can place an electrode patch anywhere
within the general region of the sternum. Ensuring that the
quality level of ECG recording remains constant over an
extended period of time is provided through self-authenti-
cation of electrode patches. The monitor recorder imple-
ments a challenge response scheme upon being connected to
an electrode patch. Failing self-authentication, the monitor
recorder signals an error condition.

20 Claims, 8 Drawing Sheets



Related U.S. Application Data

- continuation-in-part of application No. 14/080,717, filed on Nov. 14, 2013, now Pat. No. 9,545,204, and a continuation-in-part of application No. 14/080,725, filed on Nov. 14, 2013, now Pat. No. 9,730,593.
- (60) Provisional application No. 61/882,403, filed on Sep. 25, 2013.
- (51) **Int. Cl.**
A61B 5/0402 (2006.01)
A61B 5/00 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61B 5/0402* (2013.01); *A61B 5/04085* (2013.01); *A61B 5/04325* (2013.01); *A61B 5/6823* (2013.01); *A61B 2562/08* (2013.01)
- (58) **Field of Classification Search**
 CPC *A61B 2560/0412*; *A61B 2560/0443*; *A61B 2560/045*; *A61B 2560/0456*; *A61B 2560/0475*; *A61B 2560/04085*; *A61B 2562/0209*; *A61B 2562/08*; *A61B 2562/227*; *A61B 2560/028*
 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

- | | | | | | |
|-------------|---------|------------------|----------------|---------|---------------------------------------|
| 3,699,948 A | 10/1972 | Ota et al. | D377,983 S | 2/1997 | Sabri et al. |
| 3,718,772 A | 2/1973 | Sanctuary | 5,601,089 A | 2/1997 | Bledsoe et al. |
| 3,893,453 A | 7/1975 | Goldberg | 5,623,935 A | 4/1997 | Faisandier |
| 4,123,785 A | 10/1978 | Cherry et al. | 5,682,901 A | 11/1997 | Kamen |
| 4,151,513 A | 4/1979 | Menken et al. | 5,697,955 A | 12/1997 | Stolte |
| 4,328,814 A | 5/1982 | Arkans | 5,724,967 A | 3/1998 | Venkatachalam |
| 4,441,500 A | 4/1984 | Sessions et al. | 5,749,902 A | 5/1998 | Olson et al. |
| 4,532,934 A | 8/1985 | Kelen | 5,788,633 A | 8/1998 | Mahoney |
| 4,546,342 A | 10/1985 | Weaver et al. | 5,817,151 A | 10/1998 | Olson et al. |
| 4,550,502 A | 11/1985 | Grayzel | 5,819,741 A | 10/1998 | Karlsson et al. |
| 4,580,572 A | 4/1986 | Granek et al. | 5,850,920 A | 12/1998 | Gilman et al. |
| 4,635,646 A | 1/1987 | Gilles et al. | D407,159 S | 3/1999 | Roberg |
| 4,653,022 A | 3/1987 | Koro | 5,876,351 A | 3/1999 | Rohde |
| 4,716,903 A | 1/1988 | Hansen | 5,906,583 A | 5/1999 | Rogel |
| 4,809,705 A | 3/1989 | Ascher | 5,951,598 A | 9/1999 | Bishay et al. |
| 4,915,656 A | 4/1990 | Alferness | 5,957,857 A | 9/1999 | Hartley |
| 5,007,429 A | 4/1991 | Treatch et al. | 5,984,102 A | 11/1999 | Tay |
| 5,025,794 A | 6/1991 | Albert et al. | 6,032,064 A | 2/2000 | Devlin et al. |
| 5,107,480 A | 4/1992 | Naus | 6,038,469 A | 3/2000 | Karlsson et al. |
| 5,168,876 A | 12/1992 | Quedens et al. | 6,101,413 A | 8/2000 | Olson et al. |
| 5,215,098 A | 6/1993 | Steinhaus | 6,115,638 A | 9/2000 | Groenke |
| 5,231,990 A | 8/1993 | Gauglitz | 6,117,077 A | 9/2000 | Del Mar et al. |
| D341,423 S | 11/1993 | Bible | 6,134,479 A | 10/2000 | Brewer et al. |
| 5,263,481 A | 11/1993 | Axelgaard | 6,148,233 A | 11/2000 | Owen et al. |
| 5,265,579 A | 11/1993 | Ferrari | 6,149,602 A | 11/2000 | Arcelus |
| 5,333,615 A | 8/1994 | Craelius et al. | 6,149,781 A | 11/2000 | Forand |
| 5,341,806 A | 8/1994 | Gadsby et al. | 6,188,407 B1 | 2/2001 | Smith et al. |
| 5,348,008 A | 9/1994 | Bornn et al. | D443,063 S | 5/2001 | Pisani et al. |
| 5,355,891 A | 10/1994 | Wateridge et al. | 6,245,025 B1 | 6/2001 | Torok et al. |
| 5,365,934 A | 11/1994 | Leon et al. | 6,246,330 B1 | 6/2001 | Nielsen |
| 5,365,935 A | 11/1994 | Righter et al. | 6,249,696 B1 | 6/2001 | Olson et al. |
| 5,392,784 A | 2/1995 | Gudaitis | D445,507 S | 7/2001 | Pisani et al. |
| D357,069 S | 4/1995 | Plahn et al. | 6,269,267 B1 | 7/2001 | Bardy et al. |
| 5,402,780 A | 4/1995 | Faasse, Jr. | 6,272,385 B1 | 8/2001 | Bishay et al. |
| 5,402,884 A | 4/1995 | Gilman et al. | 6,298,255 B1 * | 10/2001 | Cordero A61B 5/04085
600/372 |
| 5,450,845 A | 9/1995 | Axelgaard | 6,301,502 B1 | 10/2001 | Owen et al. |
| 5,451,876 A | 9/1995 | Sendford et al. | 6,304,773 B1 | 10/2001 | Taylor et al. |
| 5,458,141 A | 10/1995 | Neil | 6,304,780 B1 | 10/2001 | Owen et al. |
| 5,473,537 A | 12/1995 | Glazer et al. | 6,304,783 B1 | 10/2001 | Lyster et al. |
| 5,483,969 A | 1/1996 | Testerman et al. | 6,374,138 B1 | 4/2002 | Owen et al. |
| 5,511,553 A | 4/1996 | Segalowitz | 6,381,482 B1 | 4/2002 | Jayaraman et al. |
| 5,540,733 A | 7/1996 | Testerman et al. | 6,416,471 B1 | 7/2002 | Kumar et al. |
| 5,546,952 A | 8/1996 | Erickson | 6,418,342 B1 | 7/2002 | Owen et al. |
| 5,549,655 A | 8/1996 | Erickson | 6,424,860 B1 | 7/2002 | Karlsson et al. |
| 5,579,919 A | 12/1996 | Gilman et al. | 6,427,083 B1 | 7/2002 | Owen et al. |
| 5,582,181 A | 12/1996 | Ruess | 6,427,085 B1 | 7/2002 | Boon et al. |
| | | | 6,454,708 B1 | 9/2002 | Ferguson et al. |
| | | | 6,456,872 B1 | 9/2002 | Faisandier |
| | | | 6,463,320 B1 | 10/2002 | Xue et al. |
| | | | 6,546,285 B1 | 4/2003 | Owen et al. |
| | | | 6,605,046 B1 | 8/2003 | Del Mar |
| | | | 6,607,485 B2 | 8/2003 | Bardy |
| | | | 6,611,705 B2 | 8/2003 | Hopman et al. |
| | | | 6,671,545 B2 | 12/2003 | Fincke |
| | | | 6,671,547 B2 | 12/2003 | Lyster et al. |
| | | | 6,694,186 B2 | 2/2004 | Bardy |
| | | | 6,704,595 B2 | 3/2004 | Bardy |
| | | | 6,705,991 B2 | 3/2004 | Bardy |
| | | | 6,719,701 B2 | 4/2004 | Lade |
| | | | 6,754,523 B2 | 6/2004 | Toole |
| | | | 6,782,293 B2 | 8/2004 | Dupelle et al. |
| | | | 6,856,832 B1 | 2/2005 | Matsumura et al. |
| | | | 6,860,897 B2 | 3/2005 | Bardy |
| | | | 6,866,629 B2 | 3/2005 | Bardy |
| | | | 6,887,201 B2 | 5/2005 | Bardy |
| | | | 6,893,397 B2 | 5/2005 | Bardy |
| | | | 6,904,312 B2 | 6/2005 | Bardy |
| | | | 6,908,431 B2 | 6/2005 | Bardy |
| | | | 6,913,577 B2 | 7/2005 | Bardy |
| | | | 6,944,498 B2 | 9/2005 | Owen et al. |
| | | | 6,960,167 B2 | 11/2005 | Bardy |
| | | | 6,970,731 B1 | 11/2005 | Jayaraman et al. |
| | | | 6,978,169 B1 | 12/2005 | Guerra |
| | | | 6,993,377 B2 | 1/2006 | Flick et al. |
| | | | 7,020,508 B2 | 3/2006 | Stivoric et al. |
| | | | 7,027,864 B2 | 4/2006 | Snyder et al. |
| | | | 7,065,401 B2 | 6/2006 | Worden |
| | | | 7,085,601 B1 | 8/2006 | Bardy et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

7,104,955 B2	9/2006	Bardy	9,204,813 B2	12/2015	Kaib et al.
7,134,996 B2	11/2006	Bardy	9,241,649 B2	1/2016	Kumar et al.
7,137,389 B2	11/2006	Berthon-Jones	9,259,154 B2	2/2016	Miller et al.
7,147,600 B2	12/2006	Bardy	9,277,864 B2	3/2016	Yang et al.
7,215,991 B2	5/2007	Besson et al.	9,339,202 B2	5/2016	Brockway et al.
7,248,916 B2	7/2007	Bardy	9,414,786 B1	8/2016	Brockway et al.
7,257,438 B2	8/2007	Kinast	9,439,566 B2	9/2016	Arne et al.
7,277,752 B2	10/2007	Matos	9,603,542 B2	3/2017	Veen et al.
7,294,108 B1	11/2007	Bomzin et al.	9,655,538 B2 *	5/2017	Felix A61B 5/04087
D558,882 S	1/2008	Brady	9,700,222 B2	7/2017	Quinlan et al.
7,328,061 B2	2/2008	Rowlandson et al.	9,770,182 B2	9/2017	Bly et al.
7,412,395 B2	8/2008	Rowlandson et al.	10,034,614 B2	7/2018	Edic et al.
7,429,938 B1	9/2008	Corndorf	10,045,708 B2	8/2018	Dusan
7,552,031 B2	6/2009	Vock et al.	10,049,182 B2	8/2018	Cheffles et al.
D606,656 S	12/2009	Kobayashi et al.	2002/0013538 A1	1/2002	Teller
7,706,870 B2	4/2010	Shieh et al.	2002/0013717 A1	1/2002	Ando et al.
7,756,721 B1	7/2010	Falchuk et al.	2002/0016798 A1	2/2002	Sakai et al.
7,787,943 B2	8/2010	McDonough	2002/0103422 A1	8/2002	Harder et al.
7,874,993 B2	1/2011	Bardy	2002/0109621 A1	8/2002	Khair et al.
7,881,785 B2	2/2011	Nassif et al.	2002/0120310 A1	8/2002	Linden et al.
D639,437 S	6/2011	Bishay et al.	2002/0128686 A1	9/2002	Minogue et al.
7,959,574 B2	6/2011	Bardy	2002/0184055 A1	12/2002	Naghavi et al.
8,108,035 B1	1/2012	Bharmi	2002/0193668 A1	12/2002	Munneke
8,116,841 B2	2/2012	Bly et al.	2003/0004547 A1	1/2003	Owen et al.
8,135,459 B2	3/2012	Bardy et al.	2003/0073916 A1	4/2003	Yonce
8,150,502 B2	4/2012	Kumar et al.	2003/0083559 A1	5/2003	Thompson
8,160,682 B2	4/2012	Kumar et al.	2003/0097078 A1	5/2003	Maeda
8,172,761 B1	5/2012	Rulkov et al.	2003/0139785 A1	7/2003	Riff et al.
8,180,425 B2	5/2012	Selvitelli et al.	2003/0176802 A1	9/2003	Galen et al.
8,200,320 B2	6/2012	Kovacs	2003/0211797 A1	11/2003	Hill et al.
8,231,539 B2	7/2012	Bardy	2004/0008123 A1	1/2004	Carrender
8,231,540 B2	7/2012	Bardy	2004/0019288 A1	1/2004	Kinast
8,239,012 B2	8/2012	Felix et al.	2004/0034284 A1	2/2004	Aversano et al.
8,249,686 B2	8/2012	Libbus et al.	2004/0049132 A1	3/2004	Barron et al.
8,260,414 B2	9/2012	Nassif et al.	2004/0073127 A1	4/2004	Istvan et al.
8,266,008 B1	9/2012	Siegal et al.	2004/0087836 A1	5/2004	Green et al.
8,277,378 B2	10/2012	Bardy	2004/0088019 A1	5/2004	Rueter et al.
8,285,356 B2	10/2012	Bly et al.	2004/0093192 A1	5/2004	Hasson et al.
8,285,370 B2	10/2012	Felix et al.	2004/0148194 A1	7/2004	Wellons et al.
8,308,650 B2	11/2012	Bardy	2004/0163034 A1	8/2004	Colbath et al.
8,366,629 B2	2/2013	Bardy	2004/0167416 A1	8/2004	Lee
8,374,688 B2	2/2013	Libbus et al.	2004/0207530 A1	10/2004	Nielsen
8,412,317 B2	4/2013	Mazar	2004/0210165 A1	10/2004	Marmaropoulos et al.
8,460,189 B2	6/2013	Libbus et al.	2004/0236202 A1	11/2004	Burton
8,473,047 B2	6/2013	Chakravarthy et al.	2004/0243435 A1	12/2004	Williams
8,478,418 B2	7/2013	Fahey	2004/0256453 A1	12/2004	Lammle
8,538,503 B2	9/2013	Kumar et al.	2004/0260188 A1	12/2004	Syed et al.
8,554,311 B2	10/2013	Warner et al.	2004/0260192 A1	12/2004	Yamamoto
8,560,046 B2	10/2013	Kumar et al.	2005/0010139 A1	1/2005	Aminian et al.
8,591,430 B2	11/2013	Amurthur et al.	2005/0096717 A1	5/2005	Bishay et al.
8,594,763 B1	11/2013	Bibian et al.	2005/0108055 A1	5/2005	Ott et al.
8,600,486 B2	12/2013	Kaib et al.	2005/0151640 A1	7/2005	Hastings
8,613,708 B2	12/2013	Bishay et al.	2005/0154267 A1	7/2005	Bardy
8,613,709 B2	12/2013	Bishay et al.	2005/0182308 A1	8/2005	Bardy
8,620,418 B1	12/2013	Kuppuraj et al.	2005/0182309 A1	8/2005	Bardy
8,626,277 B2	1/2014	Felix et al.	2005/0215918 A1	9/2005	Frantz et al.
8,628,020 B2	1/2014	Beck	2005/0222513 A1	10/2005	Hadley et al.
8,668,653 B2	3/2014	Nagata et al.	2005/0228243 A1	10/2005	Bardy
8,684,925 B2	4/2014	Manicka et al.	2005/0245839 A1	11/2005	Stivoric et al.
8,688,190 B2	4/2014	Libbus et al.	2005/0275416 A1	12/2005	Hervieux et al.
8,718,752 B2	5/2014	Libbus et al.	2006/0025696 A1	2/2006	Kurzweil et al.
8,744,561 B2	6/2014	Fahey	2006/0025824 A1	2/2006	Freeman et al.
8,774,932 B2	7/2014	Fahey	2006/0030767 A1	2/2006	Lang et al.
8,790,257 B2	7/2014	Libbus et al.	2006/0030904 A1	2/2006	Quiles
8,790,259 B2	7/2014	Katra et al.	2006/0041201 A1	2/2006	Behbehani et al.
8,795,174 B2	8/2014	Manicka et al.	2006/0084883 A1	4/2006	Linker
8,798,729 B2	8/2014	Kaib et al.	2006/0122469 A1	6/2006	Martel
8,798,734 B2	8/2014	Kuppuraj et al.	2006/0124193 A1	6/2006	Orr et al.
8,818,478 B2	8/2014	Scheffler et al.	2006/0224072 A1	10/2006	Shennib
8,818,481 B2	8/2014	Bly et al.	2006/0229522 A1 *	10/2006	Barr A61B 5/0006 600/509
8,823,490 B2	9/2014	Libbus et al.	2006/0235320 A1	10/2006	Tan et al.
8,938,287 B2	1/2015	Felix et al.	2006/0253006 A1	11/2006	Bardy
8,965,492 B2	2/2015	Baker et al.	2006/0264730 A1 *	11/2006	Stivoric A61B 5/0205 600/390
9,066,664 B2	6/2015	Karjalainen	2006/0264767 A1	11/2006	Shennib
9,155,484 B2	10/2015	Baker et al.	2007/0003115 A1	1/2007	Patton et al.
			2007/0038057 A1	2/2007	Nam et al.
			2007/0050209 A1	3/2007	Yered

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0078324 A1	4/2007	Wijisiriwardana	2010/0007413 A1	1/2010	Herleikson
2007/0078354 A1	4/2007	Holland	2010/0022897 A1	1/2010	Parker et al.
2007/0088406 A1	4/2007	Bennett et al.	2010/0056881 A1	3/2010	Libbus et al.
2007/0089800 A1	4/2007	Sharma	2010/0081913 A1	4/2010	Cross et al.
2007/0093719 A1	4/2007	Nichols, Jr. et al.	2010/0174229 A1	7/2010	Hsu et al.
2007/0100248 A1	5/2007	Van Dam et al.	2010/0177100 A1	7/2010	Carnes et al.
2007/0100667 A1	5/2007	Bardy	2010/0185063 A1	7/2010	Bardy
2007/0123801 A1	5/2007	Goldberger et al.	2010/0185076 A1	7/2010	Jeong et al.
2007/0131595 A1	6/2007	Jansson et al.	2010/0191154 A1	7/2010	Berger et al.
2007/0136091 A1	6/2007	McTaggart	2010/0191310 A1	7/2010	Bly
2007/0179357 A1	8/2007	Bardy	2010/0223020 A1	9/2010	Goetz
2007/0185390 A1	8/2007	Perkins et al.	2010/0234715 A1	9/2010	Shin et al.
2007/0203415 A1	8/2007	Bardy	2010/0234716 A1	9/2010	Engel
2007/0203423 A1	8/2007	Bardy	2010/0280366 A1	11/2010	Ame et al.
2007/0208232 A1	9/2007	Kovacs	2010/0312188 A1	12/2010	Robertson et al.
2007/0208233 A1	9/2007	Kovacs	2010/0324384 A1	12/2010	Moon et al.
2007/0208266 A1	9/2007	Hadley	2011/0021937 A1*	1/2011	Hugh A61B 5/0006 600/523
2007/0225611 A1	9/2007	Kumar et al.	2011/0054286 A1	3/2011	Crosby et al.
2007/0244405 A1	10/2007	Xue et al.	2011/0060215 A1	3/2011	Tupin et al.
2007/0249946 A1	10/2007	Kumar et al.	2011/0066041 A1	3/2011	Pandia et al.
2007/0255153 A1	11/2007	Kumar et al.	2011/0077497 A1	3/2011	Oster et al.
2007/0265510 A1	11/2007	Bardy	2011/0105861 A1	5/2011	Derchak et al.
2007/0276270 A1	11/2007	Tran	2011/0144470 A1	6/2011	Mazar et al.
2007/0276275 A1	11/2007	Proctor et al.	2011/0160548 A1	6/2011	Forster et al.
2007/0293738 A1	12/2007	Bardy	2011/0224564 A1	9/2011	Moon et al.
2007/0293739 A1	12/2007	Bardy	2011/0237922 A1	9/2011	Parker, III et al.
2007/0293740 A1	12/2007	Bardy	2011/0237924 A1	9/2011	McGusty et al.
2007/0293741 A1	12/2007	Bardy	2011/0245699 A1	10/2011	Snell et al.
2007/0293772 A1	12/2007	Bardy	2011/0245711 A1	10/2011	Katra et al.
2007/0299325 A1	12/2007	Farrell et al.	2011/0288605 A1	11/2011	Kaib et al.
2007/0299617 A1	12/2007	Willis	2012/0003933 A1	1/2012	Baker et al.
2008/0027339 A1	1/2008	Nagai et al.	2012/0029306 A1	2/2012	Paquet et al.
2008/0051668 A1	2/2008	Bardy	2012/0029315 A1	2/2012	Raptis et al.
2008/0058661 A1	3/2008	Bardy	2012/0029316 A1	2/2012	Raptis
2008/0088467 A1*	4/2008	Al-Ali A61B 5/14551 340/679	2012/0035432 A1	2/2012	Katra et al.
2008/0091097 A1	4/2008	Linti et al.	2012/0078127 A1	3/2012	McDonald et al.
2008/0108890 A1	5/2008	Teng	2012/0088998 A1	4/2012	Bardy et al.
2008/0114232 A1	5/2008	Gazit	2012/0088999 A1	4/2012	Bishay et al.
2008/0139953 A1*	6/2008	Baker A61B 5/0006 600/509	2012/0089000 A1	4/2012	Bishay et al.
2008/0143080 A1	6/2008	Burr	2012/0089001 A1	4/2012	Bishay et al.
2008/0177168 A1	7/2008	Callahan et al.	2012/0089037 A1	4/2012	Bishay et al.
2008/0194927 A1	8/2008	KenKnight et al.	2012/0089412 A1	4/2012	Bardy et al.
2008/0208009 A1	8/2008	Shklarski	2012/0089417 A1	4/2012	Bardy et al.
2008/0208014 A1	8/2008	KenKnight et al.	2012/0095352 A1	4/2012	Tran
2008/0284599 A1	11/2008	Zdeblick et al.	2012/0101358 A1	4/2012	Boettcher et al.
2008/0288026 A1*	11/2008	Cross A61B 5/0408 607/60	2012/0101396 A1*	4/2012	Solosko A61B 5/0006 600/509
2008/0294024 A1	11/2008	Cosentino et al.	2012/0165645 A1	6/2012	Russel et al.
2008/0306359 A1	12/2008	Zdeblick et al.	2012/0306662 A1	6/2012	Vosch et al.
2008/0312522 A1	12/2008	Rowlandson	2012/0172695 A1	7/2012	Ko et al.
2009/0012412 A1	1/2009	Wesel	2012/0238910 A1	9/2012	Nordstrom
2009/0012979 A1	1/2009	Bateni et al.	2012/0253847 A1	10/2012	Dell'Anno et al.
2009/0054952 A1	2/2009	Glukhovskiy et al.	2012/0302906 A1	11/2012	Felix et al.
2009/0062897 A1	3/2009	Axelgaard	2012/0323132 A1	12/2012	Warner et al.
2009/0069867 A1	3/2009	KenKnight et al.	2012/0330126 A1	12/2012	Hoppe et al.
2009/0073991 A1	3/2009	Landrum et al.	2013/0041272 A1	2/2013	Guillen Arredondo et al.
2009/0076336 A1	3/2009	Mazar et al.	2013/0077263 A1	3/2013	Oleson et al.
2009/0076341 A1	3/2009	James et al.	2013/0079611 A1	3/2013	Besko
2009/0076342 A1	3/2009	Amurthur et al.	2013/0085347 A1	4/2013	Manicka et al.
2009/0076343 A1	3/2009	James et al.	2013/0085403 A1	4/2013	Gunderson et al.
2009/0076346 A1	3/2009	James et al.	2013/0096395 A1	4/2013	Katra et al.
2009/0076349 A1	3/2009	Libbus et al.	2013/0116533 A1	5/2013	Lian et al.
2009/0076397 A1	3/2009	Libbus et al.	2013/0123651 A1	5/2013	Bardy
2009/0076401 A1	3/2009	Mazar et al.	2013/0158361 A1	6/2013	Bardy
2009/0076559 A1	3/2009	Libbus et al.	2013/0197380 A1	8/2013	Oral et al.
2009/0088652 A1	4/2009	Tremblay	2013/0225963 A1	8/2013	Kodandaramaiah et al.
2009/0112116 A1	4/2009	Lee et al.	2013/0225966 A1	8/2013	Macia Barber et al.
2009/0131759 A1	5/2009	Sims et al.	2013/0231947 A1	9/2013	Shusterman
2009/0156908 A1	6/2009	Belalcazar et al.	2013/0243105 A1	9/2013	Lei et al.
2009/0216132 A1	8/2009	Orbach	2013/0274584 A1	10/2013	Finlay et al.
2009/0270708 A1	10/2009	Shen et al.	2013/0275158 A1	10/2013	Fahey
2009/0270747 A1	10/2009	Van Dam et al.	2013/0324809 A1	12/2013	Lisogurski et al.
2009/0292194 A1	11/2009	Libbus et al.	2013/0324855 A1	12/2013	Lisogurski et al.
			2013/0324856 A1	12/2013	Lisogurski et al.
			2013/0325081 A1	12/2013	Karst et al.
			2013/0325359 A1	12/2013	Jarverud et al.
			2013/0331665 A1	12/2013	Libbus et al.
			2013/0338448 A1	12/2013	Libbus et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0338472	A1	12/2013	Macia Barber et al.
2014/0012154	A1	1/2014	Mazar et al.
2014/0056452	A1	2/2014	Moss et al.
2014/0088399	A1	3/2014	Lian et al.
2014/0140359	A1	5/2014	Kalevo et al.
2014/0180027	A1	6/2014	Buller
2014/0189928	A1	7/2014	Oleson et al.
2014/0206977	A1	7/2014	Bahney et al.
2014/0215246	A1	7/2014	Lee et al.
2014/0249852	A1	9/2014	Proud
2014/0296651	A1	10/2014	Stone
2014/0343390	A1	11/2014	Berzowska et al.
2014/0358193	A1	12/2014	Lyons et al.
2014/0364756	A1	12/2014	Brockway et al.
2015/0048836	A1	2/2015	Guthrie et al.
2015/0065842	A1	3/2015	Lee et al.
2015/0250422	A1	9/2015	Bay
2015/0257670	A1	9/2015	Ortega et al.
2015/0305676	A1	11/2015	Shoshani
2015/0359489	A1	12/2015	Baudenbacher et al.
2016/0135746	A1	5/2016	Kumar et al.
2016/0217691	A1	7/2016	Kadobayashi et al.
2019/0021671	A1	1/2019	Kumar et al.

FOREIGN PATENT DOCUMENTS

EP	2438851	4/2012
EP	2438852	4/2012
EP	2465415	6/2012
EP	2589333	5/2013
JP	H06319711	11/1994
JP	H11188015	7/1999
JP	2004129788	4/2004
JP	2007082938	4/2007
JP	2009219554	10/2009
WO	199852463	11/1998
WO	0078213	12/2000
WO	2003032192	4/2003
WO	2006009767	1/2006
WO	2006014806	2/2006
WO	2007066270	6/2007
WO	2007092543	8/2007
WO	2008010216	1/2008
WO	2008057884	5/2008
WO	2008092098	7/2008
WO	2009036306	3/2009
WO	2009036313	3/2009
WO	2009036327	3/2009
WO	2009112976	9/2009
WO	2009112978	9/2009
WO	2009112979	9/2009
WO	2009142975	11/2009
WO	2010066507	6/2010
WO	2010105045	9/2010
WO	2011047207	4/2011
WO	2012140559	10/2012
WO	2012146957	11/2012

OTHER PUBLICATIONS

Alivecor's Heart Monitor for iPhone Receives FDA Clearance, URL <<http://www.businesswire.com/news/home/20121203005545/en/AliveCor%E2%80%99s-Heart-Monitor-iPhone-Receives-FDA-Clearance#.U7rtq7FVTyF>> (Dec. 3, 2012).

Bharadwaj et al., Techniques for Accurate ECG signal processing, EE Times, URL <www.eetimes.com/document.asp?doc_id=1278571> (Feb. 14, 2011).

Chen et al., "Monitoring Body Temperature of Newborn Infants At Neonatal Intensive Care Units Using Wearable Sensors," BodyNets 2010, Corfu Island, Greece. (Sep. 10, 2010).

Epstein, Andrew E. et al.; ACC/AHA/HRS 2008 Guidelines for Device-Based Therapy of Cardiac Rhythm Abnormalities. J. Am. Coll. Cardiol. 2008; 51; e1-e62, 66 Pgs.

Fitbit automatically tracks your fitness and sleep, URL <<http://www.fitbit.com/>> (Web page cached on Sep. 10, 2008).

Smith, Kevin, "Jawbone Up VS. Fitbit Flex: Which Is the Best Fitness Band?" URL <<http://www.businessinsider.com/fitbit-flex-vs-jawbone-up-2013-5?op=1>> (Jun. 1, 2013).

Kligfield, Paul et al., Recommendations for the Standardization and Interpretation of the Electrocardiogram: Part I. J. Am. Coll. Cardiol; 2007; 49; 1109-27, 75 Pgs.

Lauren Gravit, "When Your Diet Needs a Band-Aid," Technology Review, MIT. (May 1, 2009).

Lieberman, Jonathan, "How Telemedicine Is Aiding Prompt ECG Diagnosis in Primary Care," British Journal of Community Nursing, vol. 13, No. 3, Mar. 1, 2008 (Mar. 1, 2008), pp. 123-126, XP009155082, ISSN: 1462-4753.

McManus et al., "A Novel Application for the Detection of an Irregular Pulse using an iPhone 4S in Patients with Atrial Fibrillation," vol. 10(3), pp. 315-319 (Mar. 2013).

Nike+ Fuel Band, URL <http://www.nike.com/us/en_us/c/nikeplus-fuelband> (Web page cached on Jan. 11, 2013).

P. Libby et al., "Braunwald's Heart Disease—A Textbook of Cardiovascular Medicine," Chs. 11, pp. 125-148 and 12, pp. 149-193 (8th ed. 2008), American Heart Association.

Initial hands-on with Polar Loop activity tracker, URL <<http://www.dcrainmaker.com/2013/09/polar-loop-firstlook.html>> (Sep. 17, 2013).

Sittig et al., "A Computer-Based Outpatient Clinical Referral System," International Journal of Medical Informatics, Shannon, IR, vol. 55, No. 2, Aug. 1, 1999, pp. 149-158, XO004262434, ISSN: 1386-5056(99)00027-1.

Sleepview, URL <<http://www.clevemed.com/sleepview/overview.shtml>> (Web pages cached on Feb. 23, 2010, Dec. 29, 2012 and Sep. 4, 2013).

Actigraphy/ Circadian Rhythm SOMNOWatch, URL <<http://www.somnomedics.eu/news-events/publications/somnowatchtm.html>> (Web cached on Jan. 23, 2010).

Zio Event Card, URL <<http://www.irhythmtech.com/zio-solution/zio-event/>> (Web page cached on Mar. 11, 2013).

Zio Patch System, URL <<http://www.irhythmtech.com/zio-solution/zio-system/index.html>> (Web page cached on Sep. 8, 2013).

Saadi et al. "Heart Rhythm Analysis Using ECG Recorded With a Novel Sternum Based Patch Technology—A Pilot Study." Cardio technix 2013—Proceedings of the International Congress on Cardiovascular Technologies, Sep. 20, 2013.

Anonymous. "Omegawave Launches Consumer App 2.0 in U.S. Endurance Sportswire—Endurance Sportswire." Jul. 11, 2013. URL: <http://endurancesportswire.com/omegawave-launches-consumer-app-2-0-in-u-s/>.

Chan et al. "Wireless Patch Sensor for Remote Monitoring of Heart Rate, Respiration, Activity, and Falls." pp. 6115-6118. 2013 35th Annual International Conference of the IEEE Engineering in Medical and Biology Society. Jul. 1, 2013.

Daoud et al. "Fall Detection Using Shimmer Technology and Multiresolution Analysis." Aug. 2, 2013. URL: <https://decibel.ni.com/content/docs/Doc-26652>.

Libbus. "Adherent Cardiac Monitor With Wireless Fall Detection for Patients With Unexplained Syncope." Abstracts of the First AMA-IEEE Medical Technology Conference on Individualized Healthcare. May 22, 2010.

Duttweiler et al., "Probability Estimation in Arithmetic and Adaptive-Huffman Entropy Coders," IEEE Transactions on Image Processing, vol. 4, No. 3, Mar. 1, 1995, pp. 237-246.

Gupta et al., "An ECG Compression Technique for Telecardiology Application," India Conference (INDICON), 2011 Annual IEEE, Dec. 16, 2011, pp. 1-4.

Nave et al., "ECG Compression Using Long-Term Prediction," IEEE Transactions on Biomedical Engineering, IEEE Service Center, NY, USA, vol. 40, No. 9, Sep. 1, 1993, pp. 877-885.

Skretting et al., "Improved Huffman Coding Using Recursive Splitting," NORSIG, Jan. 1, 1999.

A Voss et al., "Linear and Nonlinear Methods for Analyses of Cardiovascular Variability in Bipolar Disorders," Bipolar Disorders, vol. 8, No. 5p1, Oct. 1, 2006, pp. 441-452, XP55273826, DK ISSN: 1398-5647, DOI: 10.1111/1399-5618.2006.00364.x.

(56)

References Cited

OTHER PUBLICATIONS

“Varicrad-Kardi Software User’s Manual Rev. 1.1”, Jul. 8, 2009 (Jul. 8, 2009), XP002757888, retrieved from the Internet: URL:<http://www.ehrlich.tv/KARDiVAR-Software.pdf> [retrieved on May 20, 2016].

BIOPAC Systems, Inc. #AS148—Automated ECG Analysis , Mar. 24, 2006.

<https://web.archive.org/web/20130831204020/http://www.biopac.com/research.asp?CatID=37&Main=Software> (Aug. 2013).

ADINSTRUMENTS:ECG Analysis Module for LabChart & PowerLab, 2008.

G. G. Ivanov, “HRV Analysis Under the Usage of Different Electrocardiography Systems,” Apr. 15, 2008 (Apr. 15, 2008), XP55511209, Retrieved from the Internet: URL:[http://www.drkucera.eu/upload_doc/hrv_analysis_\(methodical_recommendations\).pdf](http://www.drkucera.eu/upload_doc/hrv_analysis_(methodical_recommendations).pdf) [retrieved on Oct. 1, 2018].

* cited by examiner

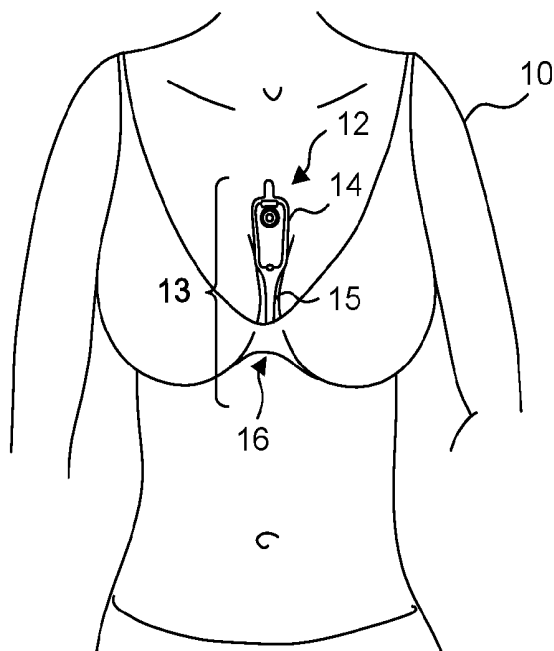
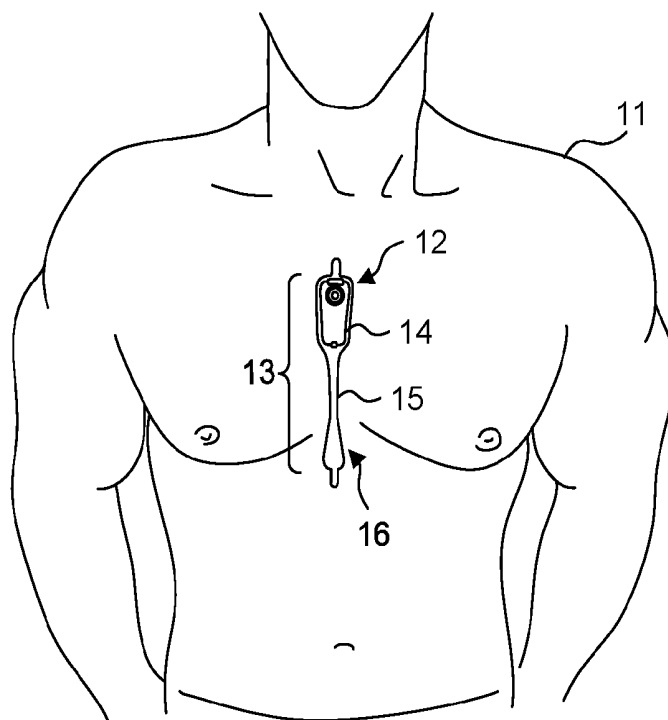
Fig. 1.**Fig. 2.**

Fig. 3.

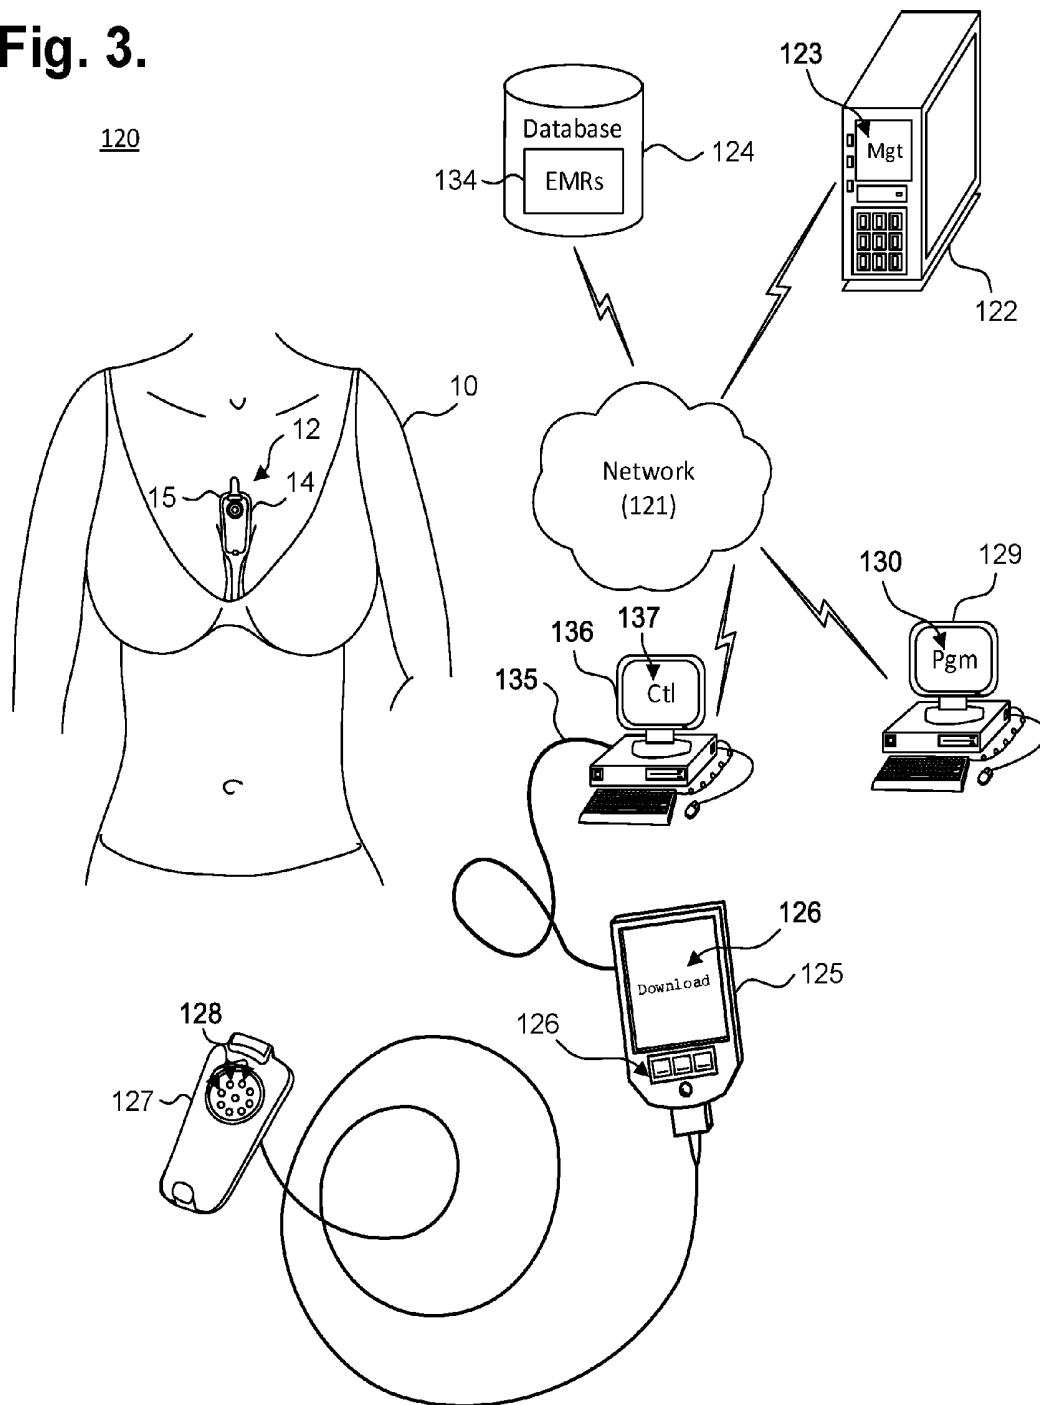


Fig. 4.

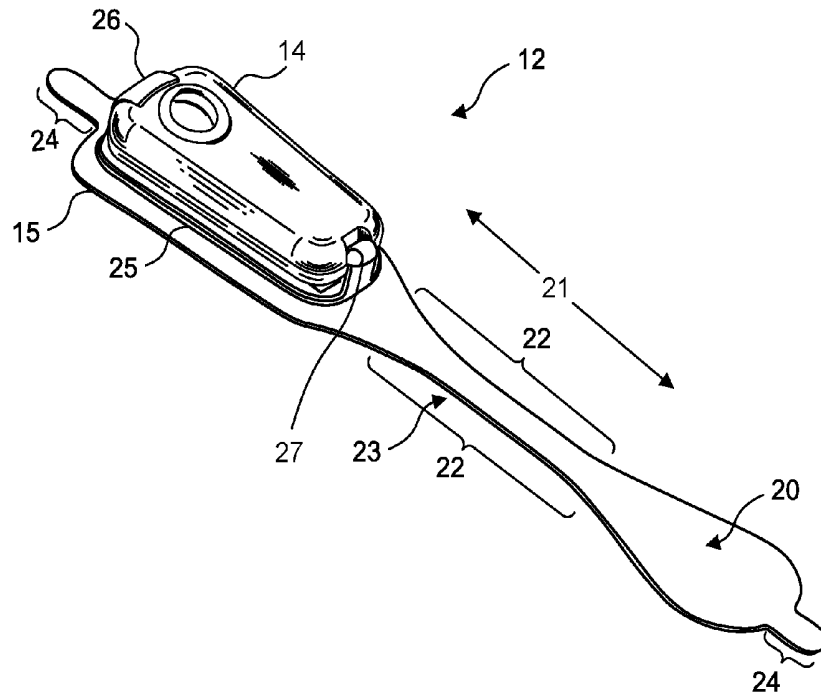


Fig. 5.

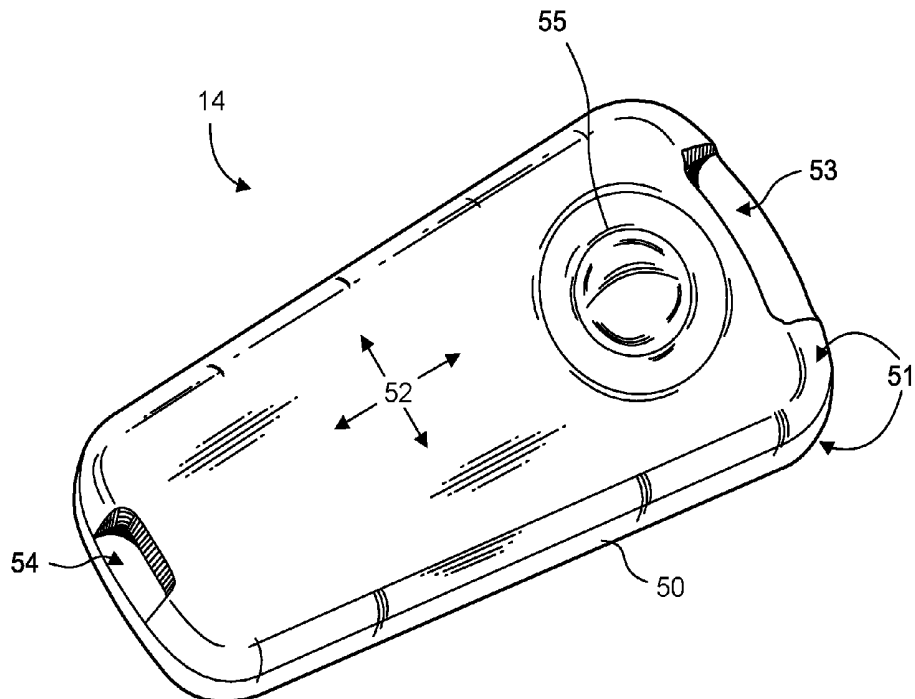


Fig. 6.

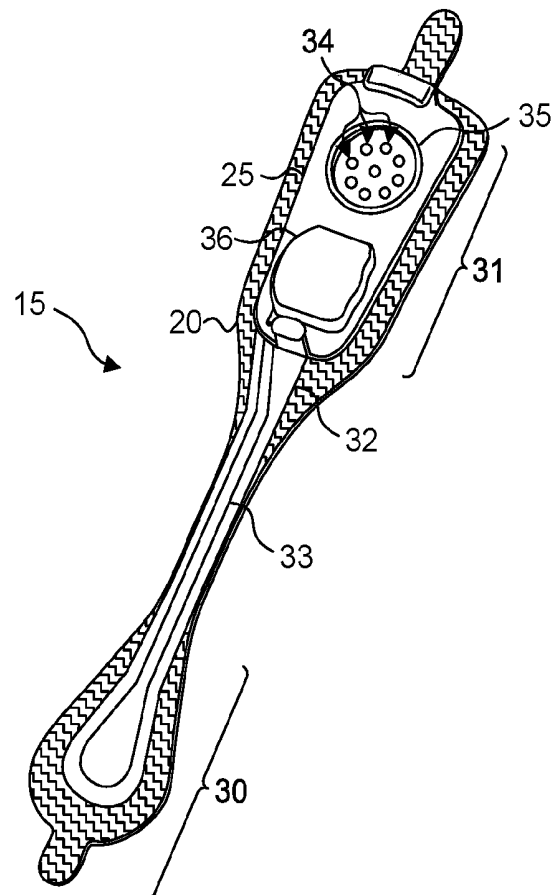


Fig. 7.

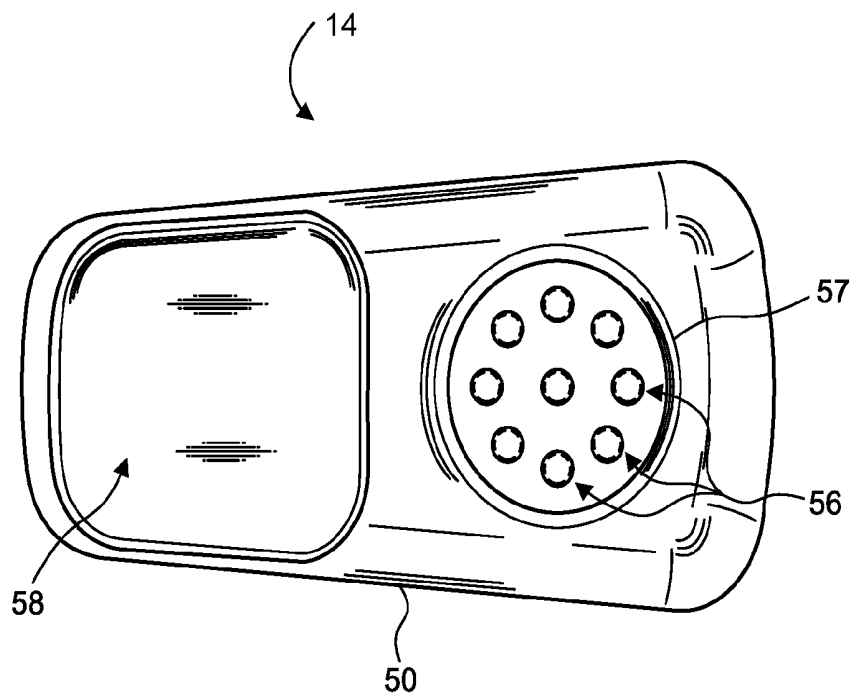


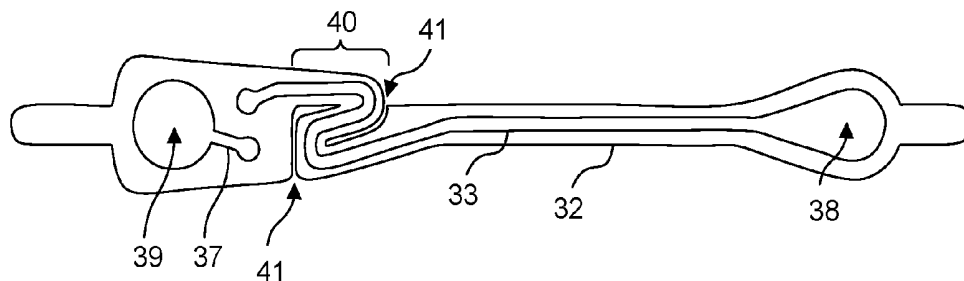
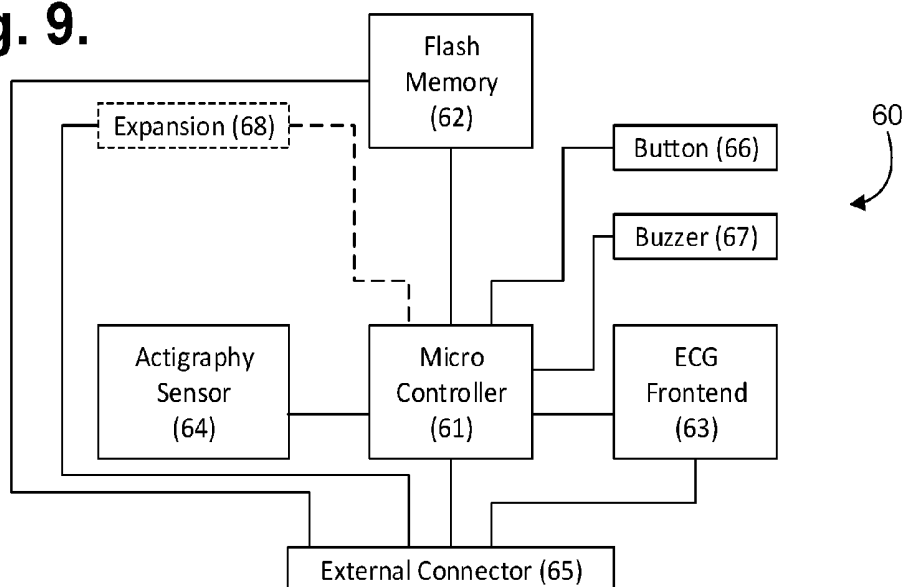
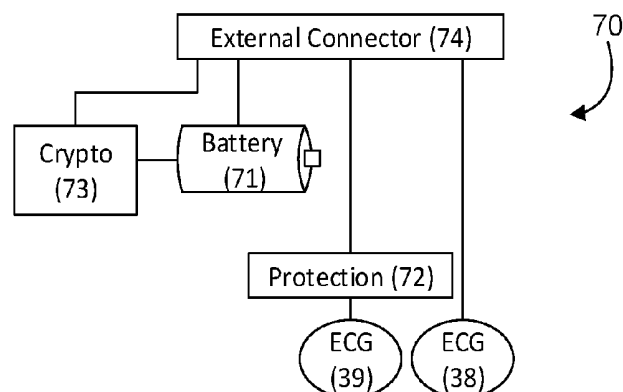
Fig. 8.**Fig. 9.****Fig. 10.**

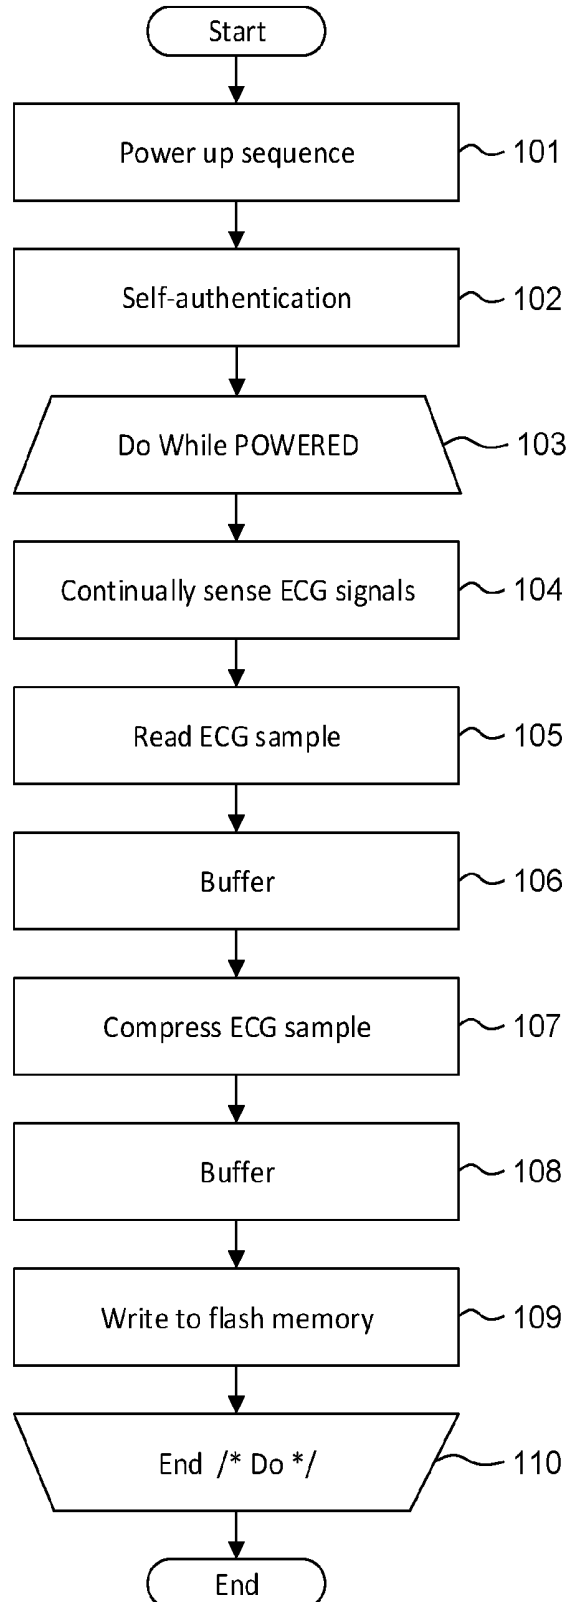
Fig. 11.100

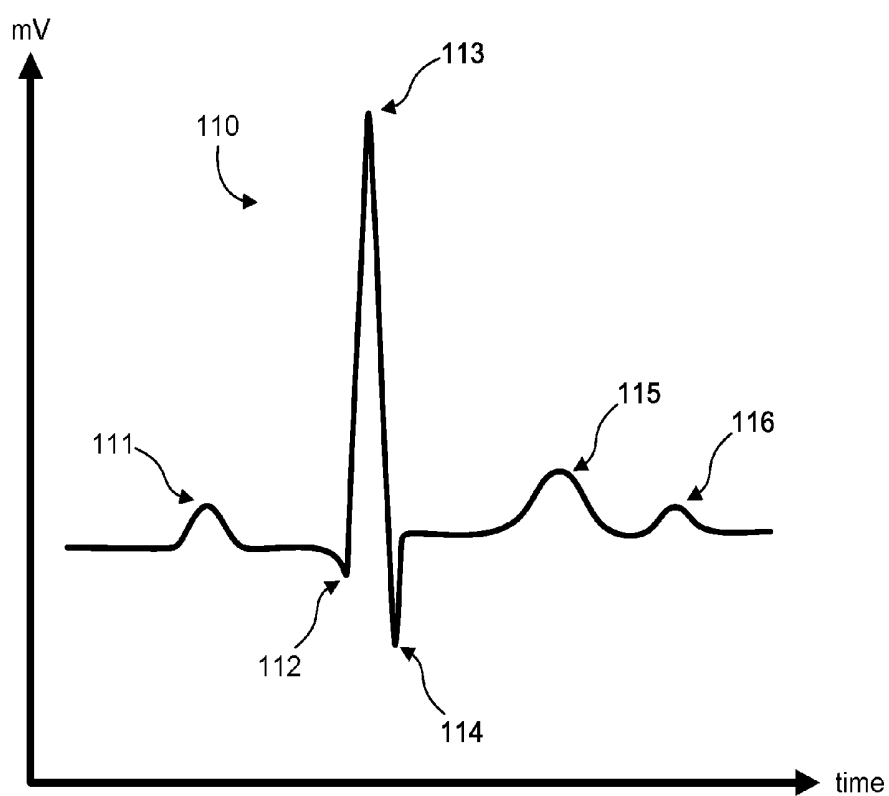
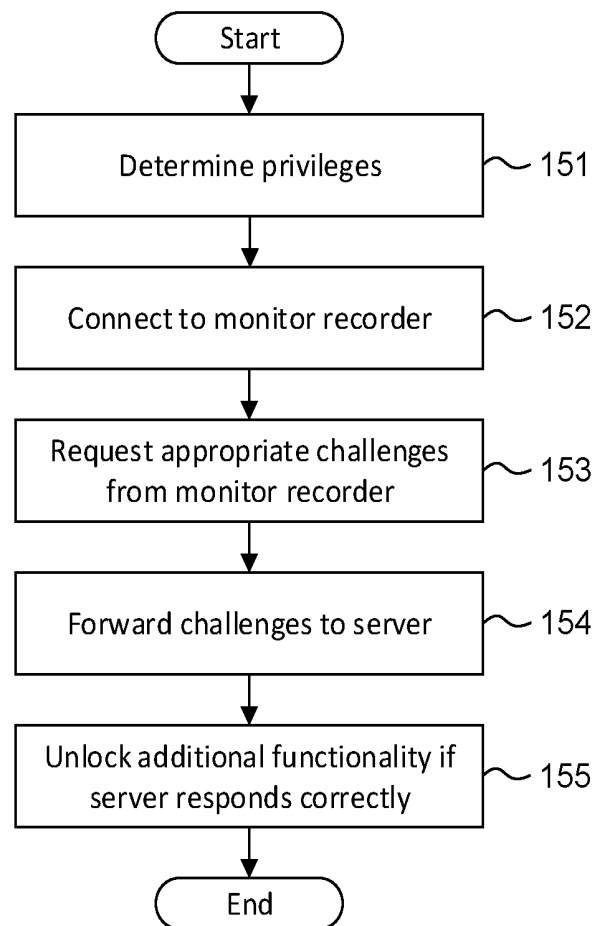
Fig. 12.

Fig. 13.150

1

SELF-AUTHENTICATING ELECTROCARDIOGRAPHY MONITORING CIRCUIT

CROSS-REFERENCE TO RELATED APPLICATION

This non-provisional patent application is a continuation of U.S. Pat. No. 9,655,538, issued May 23, 2017, which is a continuation-in-part of U.S. Pat. No. 9,545,204, issued Jan. 17, 2017, and is a continuation-in-part of U.S. Pat. No. 9,730,593, issued Aug. 15, 2017, and further claims priority under 35 U.S.C. § 119(e) to U.S. Provisional Patent application, Ser. No. 61/882,403, filed Sep. 25, 2013, the disclosures of which are incorporated by reference.

FIELD

This application relates in general to electrocardiographic monitoring and, in particular, to a self-authenticating electrocardiography monitoring circuit.

BACKGROUND

The heart emits electrical signals as a by-product of the propagation of the action potentials that trigger depolarization of heart fibers. An electrocardiogram (ECG) measures and records such electrical potentials to visually depict the electrical activity of the heart over time. Conventionally, a standardized set format 12-lead configuration is used by an ECG machine to record cardiac electrical signals from well-established traditional chest locations. Electrodes at the end of each lead are placed on the skin over the anterior thoracic region of the patient's body to the lower right and to the lower left of the sternum, on the left anterior chest, and on the limbs. Sensed cardiac electrical activity is represented by PQRSTU waveforms that can be interpreted post-ECG recordation to derive heart rate and physiology. The P-wave represents atrial electrical activity. The QRS components represent ventricular electrical activity.

An ECG is a tool used by physicians to diagnose heart problems and other potential health concerns. An ECG is a snapshot of heart function, typically recorded over 12 seconds, that can help diagnose rate and regularity of heartbeats, effect of drugs or cardiac devices, including pacemakers and implantable cardioverter-defibrillators (ICDs), and whether a patient has heart disease. ECGs are used in-clinic during appointments, and, as a result, are limited to recording only those heart-related aspects present at the time of recording. Sporadic conditions that may not show up during a spot ECG recording require other means to diagnose them. These disorders include fainting or syncope; rhythm disorders, such as tachyarrhythmias and bradyarrhythmias; apneic episodes; and other cardiac and related disorders. Thus, an ECG only provides a partial picture and can be insufficient for complete patient diagnosis of many cardiac disorders.

Diagnostic efficacy can be improved, when appropriate, through the use of long-term extended ECG monitoring. Recording sufficient ECG and related physiology over an extended period is challenging, and often essential to enabling a physician to identify events of potential concern. A 30-day observation period is considered the "gold standard" of ECG monitoring, yet achieving a 30-day observation day period has proven unworkable because such ECG monitoring systems are arduous to employ, cumbersome to the patient, and excessively costly. Ambulatory monitoring

2

in-clinic is implausible and impracticable. Nevertheless, if a patient's ECG could be recorded in an ambulatory setting, thereby allowing the patient to engage in activities of daily living, the chances of acquiring meaningful information and capturing an abnormal event while the patient is engaged in normal activities becomes more likely to be achieved.

For instance, the long-term wear of ECG electrodes is complicated by skin irritation and the inability ECG electrodes to maintain continual skin contact after a day or two. Moreover, time, dirt, moisture, and other environmental contaminants, as well as perspiration, skin oil, and dead skin cells from the patient's body, can get between an ECG electrode, the non-conductive adhesive used to adhere the ECG electrode, and the skin's surface. All of these factors adversely affect electrode adhesion and the quality of cardiac signal recordings. Furthermore, the physical movements of the patient and their clothing impart various compressional, tensile, and torsional forces on the contact point of an ECG electrode, especially over long recording times, and an inflexibly fastened ECG electrode will be prone to becoming dislodged. Notwithstanding the cause of electrode dislodgment, depending upon the type of ECG monitor employed, precise re-placement of a dislodged ECG electrode maybe essential to ensuring signal capture at the same fidelity. Moreover, dislodgment may occur unbeknownst to the patient, making the ECG recordings worthless. Further, some patients may have skin that is susceptible to itching or irritation, and the wearing of ECG electrodes can aggravate such skin conditions. Thus, a patient may want or need to periodically remove or replace ECG electrodes during a long-term ECG monitoring period, whether to replace a dislodged electrode, reestablish better adhesion, alleviate itching or irritation, allow for cleansing of the skin, allow for showering and exercise, or for other purpose. Such replacement or slight alteration in electrode location actually facilitates the goal of recording the ECG signal for long periods of time; however, ensuring that the level of quality of ECG recording and patient service remains constant over an extended period of time is dependent upon the monitoring equipment being up to a known standard. Use of third party consumables, such as ECG electrodes, could undermine expectations of ECG recording fidelity and adversely skew monitoring results.

Conventionally, Holter monitors are widely used for long-term extended ECG monitoring. Typically, they are used for only 24-48 hours. A typical Holter monitor is a wearable and portable version of an ECG that include cables for each electrode placed on the skin and a separate battery-powered ECG recorder. The cable and electrode combination (or leads) are placed in the anterior thoracic region in a manner similar to what is done with an in-clinic standard ECG machine. The duration of a Holter monitoring recording depends on the sensing and storage capabilities of the monitor, as well as battery life. A "looping" Holter monitor (or event) can operate for a longer period of time by overwriting older ECG tracings, thence "recycling" storage in favor of extended operation, yet at the risk of losing event data. Although capable of extended ECG monitoring, Holter monitors are cumbersome, expensive and typically only available by medical prescription, which limits their usability. Further, the skill required to properly place the electrodes on the patient's chest hinders or precludes a patient from replacing or removing the precordial leads and usually involves moving the patient from the physician office to a specialized center within the hospital or clinic.

The ZIO XT Patch and ZIO Event Card devices, manufactured by iRhythm Tech., Inc., San Francisco, Calif., are

wearable stick-on monitoring devices that are typically worn on the upper left pectoral region to respectively provide continuous and looping ECG recording. The location is used to simulate surgically implanted monitors. Both of these devices are prescription-only and for single patient use. The ZIO XT Patch device is limited to a 14-day monitoring period, while the electrodes only of the ZIO Event Card device can be worn for up to 30 days. The ZIO XT Patch device combines both electronic recordation components, including battery, and physical electrodes into a unitary assembly that adheres to the patient's skin. The ZIO XT Patch device uses adhesive sufficiently strong to support the weight of both the monitor and the electrodes over an extended period of time and to resist disadherence from the patient's body, albeit at the cost of disallowing removal or relocation during the monitoring period. Moreover, throughout monitoring, the battery is continually depleted and battery capacity can potentially limit overall monitoring duration. The ZIO Event Card device is a form of downsized Holter monitor with a recorder component that must be removed temporarily during baths or other activities that could damage the non-waterproof electronics. Both devices represent compromises between length of wear and quality of ECG monitoring, especially with respect to ease of long term use, female-friendly fit, and quality of atrial (P-wave) signals. Moreover, both devices rely on the same set of ECG electrodes for the duration of the monitoring period; signal capture can suffer as the ECG electrodes disadhere from the patient's body over time.

Therefore, a need remains for an extended wear continuously recording ECG monitor practicably capable of being worn for a long period of time in both men and women and capable of recording atrial signals reliably with quality assurance implemented as part of disposable component replenishment.

A further need remains for a device capable of recording signals ideal for arrhythmia discrimination, especially a device designed for atrial activity recording.

SUMMARY

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. The wearable monitor sits centrally (in the midline) on the patient's chest along the sternum oriented top-to-bottom. The placement of the wearable monitor in a location at the sternal midline (or immediately to either side of the sternum), with its unique narrow "hourglass"-like shape, benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch anywhere within the general region of the sternum, the area most likely to record high quality atrial signals or P-waves. In addition, ensuring that the level of quality of ECG recording and patient service remains constant over an extended period of time is provided through self-authentication of electrode patches (and other accessories). The monitor recorder implements a challenge response scheme upon being connected to an electrode patch (or other accessory). Failing self-authentication, the monitor recorder signals an error condition. In addition, electrode patches (and other accessories) can be limited to operating for only a certain period of time, or with pre-defined operational parameters or privileges. In a further embodiment, a patient

can purchase additional time, pre-defined operational parameters or privileges through a server-based subscription service.

One embodiment provides an extended wear electrocardiography and physiological sensor monitor recorder. A sealed housing is adapted to be removably secured into the non-conductive receptacle on a disposable extended wear electrode patch. Electronic circuitry is included within the sealed housing. An externally-powered micro-controller is operable to execute under micro programmable control only upon authentication of the disposable extended wear electrode patch during power up of the electronic circuitry. An electrocardiographic front end circuit is electrically interfaced to the micro-controller and is operable to sense electrocardiographic signals through electrocardiographic electrodes provided on the disposable extended wear electrode patch. Externally-powered flash memory is electrically interfaced with the micro-controller and is operable to store samples of the electrocardiographic signals.

A further embodiment provides an extended wear electrocardiography and physiological sensor monitor with self-authenticating electrocardiography monitoring circuit. An electrode patch includes an elongated strip of stretchable material and a pair of electrocardiographic electrodes conductively exposed on a contact surface of each end of the elongated strip. A non-conductive receptacle is adhered to an outward-facing surface of the elongated strip and has a plurality of electrical pads. A circuit is affixed on each end of the elongated strip and includes a pair of circuit traces electrically coupled to the pair of the electrocardiographic electrodes and a pair of the electrical pads. An electrocardiography monitor includes a sealed housing adapted to be removably secured into the non-conductive receptacle on the electrode patch. Electronic circuitry is included within the sealed housing and includes an electrocardiographic front end circuit operable to sense electrocardiographic signals through the electrocardiographic electrodes provided on the electrode patch and flash memory to record the electrocardiographic signals. A micro-controller periodically writes data into a memory of the electrode patch during continuous recording of the electrocardiographic signals via the front end circuit and determines an expiration of the electrode patch based on an amount of the data stored in the memory of the electrode patch.

The monitoring patch is especially suited to the female anatomy. The narrow longitudinal midsection can fit nicely within the intermammary cleft of the breasts without inducing discomfort, whereas conventional patch electrodes are wide and, if adhered between the breasts, would cause chafing, irritation, frustration, and annoyance, leading to low patient compliance.

The foregoing aspects enhance ECG monitoring performance and quality, facilitating long-term ECG recording, critical to accurate arrhythmia diagnosis.

In addition, the foregoing aspects enhance comfort in women (and certain men), but not irritation of the breasts, by placing the monitoring patch in the best location possible for optimizing the recording of cardiac signals from the atrium, another feature critical to proper arrhythmia diagnosis.

Finally, the foregoing aspects as relevant to monitoring are equally applicable to recording other physiological measures, such as temperature, respiratory rate, blood sugar, oxygen saturation, and blood pressure, as well as other measures of body chemistry and physiology.

Still other embodiments will become readily apparent to those skilled in the art from the following detailed description, wherein are described embodiments by way of illus-

trating the best mode contemplated. As will be realized, other and different embodiments are possible and the embodiments' several details are capable of modifications in various obvious respects, all without departing from their spirit and the scope. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor respectively fitted to the sternal region of a female patient and a male patient.

FIG. 3 is a functional block diagram showing a system for providing a self-authenticating electrocardiography monitoring circuit in accordance with one embodiment.

FIG. 4 is a perspective view showing an extended wear electrode patch with a monitor recorder in accordance with one embodiment inserted.

FIG. 5 is a perspective view showing the monitor recorder of FIG. 4.

FIG. 6 is a perspective view showing the extended wear electrode patch of FIG. 4 without a monitor recorder inserted.

FIG. 7 is a bottom plan view of the monitor recorder of FIG. 4.

FIG. 8 is a top view showing the flexible circuit of the extended wear electrode patch of FIG. 4 when mounted above the flexible backing.

FIG. 9 is a functional block diagram showing the component architecture of the circuitry of the monitor recorder of FIG. 4.

FIG. 10 is a functional block diagram showing the circuitry of the extended wear electrode patch of FIG. 4.

FIG. 11 is a flow diagram showing a monitor recorder-implemented method for monitoring ECG data for use in the monitor recorder of FIG. 4.

FIG. 12 is a graph showing, by way of example, a typical ECG waveform.

FIG. 13 is a flow diagram showing a method for providing a self-authenticating electrocardiography monitoring circuit in accordance with one embodiment.

DETAILED DESCRIPTION

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor 12, including a monitor recorder 14 in accordance with one embodiment, respectively fitted to the sternal region of a female patient 10 and a male patient 11. The wearable monitor 12 sits centrally (in the midline) on the patient's chest along the sternum 13 oriented top-to-bottom with the monitor recorder 14 preferably situated towards the patient's head. In a further embodiment, the orientation of the wearable monitor 12 can be corrected post-monitoring, as further described infra. The electrode patch 15 is shaped to fit comfortably and conformal to the contours of the patient's chest approximately centered on the sternal midline 16 (or immediately to either side of the sternum 13). The distal end of the electrode patch 15 extends towards the Xiphoid process and, depending upon the patient's build, may straddle the region over the Xiphoid process. The proximal end of the electrode patch

15, located under the monitor recorder 14, is below the manubrium and, depending upon patient's build, may straddle the region over the manubrium.

The placement of the wearable monitor 12 in a location at the sternal midline 16 (or immediately to either side of the sternum 13) significantly improves the ability of the wearable monitor 12 to cutaneously sense cardiac electric signals, particularly the P-wave (or atrial activity) and, to a lesser extent, the QRS interval signals in the ECG waveforms that indicate ventricular activity, while simultaneously facilitating comfortable long-term wear for many weeks. The sternum 13 overlies the right atrium of the heart and the placement of the wearable monitor 12 in the region of the sternal midline 13 puts the ECG electrodes of the electrode patch 15 in a location better adapted to sensing and recording P-wave signals than other placement locations, say, the upper left pectoral region or lateral thoracic region or the limb leads. In addition, placing the lower or inferior pole (ECG electrode) of the electrode patch 15 over (or near) the Xiphoid process facilitates sensing of ventricular activity and provides superior recordation of the QRS interval.

The monitor recorder 14 of the extended wear electrocardiography and physiological sensor monitor 12 senses and records the patient's ECG data into an onboard memory. Over time, disposable electrode patches 15 will require replacement and ensuring that the level of quality of ECG recording and patient service remains constant over an extended period of time is dependent upon the monitoring equipment, particularly the replacement electrode patches 15, being up to a known standard. FIG. 3 is a functional block diagram showing a system 120 for providing a self-authenticating electrocardiography monitoring circuit in accordance with one embodiment. Self-authentication allows quality and safety expectations to be maintained. The monitor recorder 14 is a reusable component that can be fitted during patient monitoring into a non-conductive receptacle provided on the electrode patch 15, as further described infra with reference to FIG. 4, and later removed for offloading of stored ECG data or to receive revised programming. The monitor recorder 14 executes an authentication protocol as part of a power up sequence, as further described infra with reference to FIG. 11. Following completion of ECG monitoring, the monitor recorder 14 can be connected to a download station 125, which could be a programmer or other device that permits the retrieval of stored ECG monitoring data, execution of diagnostics on or programming of the monitor recorder 14, or performance of other functions. The monitor recorder 14 has a set of electrical contacts (not shown) that enable the monitor recorder 14 to physically interface to a set of terminals 128 on a paired receptacle 127 of the download station 125. In turn, the download station 125 executes a communications or offload program 126 ("Offload") or similar program that interacts with the monitor recorder 14 via the physical interface to retrieve the stored ECG monitoring data. The download station 125 could be a server, personal computer, tablet or handheld computer, smart mobile device, or purpose-built programmer designed specific to the task of interfacing with a monitor recorder 14. Still other forms of download station 125 are possible.

Upon retrieving stored ECG monitoring data from a monitor recorder 14, middleware first operates on the retrieved data to adjust the ECG waveform, as necessary, and to convert the retrieved data into a format suitable for use by third party post-monitoring analysis software. The formatted data can then be retrieved from the download station 125 over a hard link 135 using a control program 137

("Ctl") or analogous application executing on a personal computer **136** or other connectable computing device, via a communications link (not shown), whether wired or wireless, or by physical transfer of storage media (not shown). The personal computer **136** or other connectable device may also execute middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program, as further described infra with reference to FIG. **13**. Note that formatted data stored on the personal computer **136** would have to be maintained and safeguarded in the same manner as electronic medical records (EMRs) **134** in the secure database **124**, as further discussed infra. In a further embodiment, the download station **125** is able to directly interface with other devices over a computer communications network **121**, which could be some combination of a local area network and a wide area network, including the Internet, over a wired or wireless connection.

A client-server model could be used to employ a server **122** to remotely interface with the download station **125** over the network **121** and retrieve the formatted data or other information. The server **122** executes a patient management program **123** ("Mgt") or similar application that stores the retrieved formatted data and other information in a secure database **124** cataloged in that patient's EMRs **134**. In addition, the patient management program **123** could manage a subscription service that authorizes a monitor recorder **14** to operate for a set period of time or under pre-defined operational parameters and privileges, such as described in infra with reference to FIG. **13**.

The patient management program **123**, or other trusted application, also maintains and safeguards the secure database **124** to limit access to patient EMRs **134** to only authorized parties for appropriate medical or other uses, such as mandated by state or federal law, such as under the Health Insurance Portability and Accountability Act (HIPAA) or per the European Union's Data Protection Directive. For example, a physician may seek to review and evaluate his patient's ECG monitoring data, as securely stored in the secure database **124**. The physician would execute an application program **130** ("Pgm"), such as a post-monitoring ECG analysis program, on a personal computer **129** or other connectable computing device, and, through the application **130**, coordinate access to his patient's EMRs **134** with the patient management program **123**. Other schemes and safeguards to protect and maintain the integrity of patient EMRs **134** are possible.

During use, the electrode patch **15** is first adhered to the skin along the sternal midline **16** (or immediately to either side of the sternum **13**). A monitor recorder **14** is then snapped into place on the electrode patch **15** to initiate ECG monitoring. FIG. **4** is a perspective view showing an extended wear electrode patch **15** with a monitor recorder **14** in accordance with one embodiment inserted. The body of the electrode patch **15** is preferably constructed using a flexible backing **20** formed as an elongated strip **21** of wrap knit or similar stretchable material with a narrow longitudinal mid-section **23** evenly tapering inward from both sides. A pair of cut-outs **22** between the distal and proximal ends of the electrode patch **15** create a narrow longitudinal midsection **23** or "isthmus" and defines an elongated "hourglass"-like shape, when viewed from above.

The electrode patch **15** incorporates features that significantly improve wearability, performance, and patient comfort throughout an extended monitoring period. During wear, the electrode patch **15** is susceptible to pushing, pulling, and torquing movements, including compressional

and torsional forces when the patient bends forward, and tensile and torsional forces when the patient leans backwards. To counter these stress forces, the electrode patch **15** incorporates strain and crimp reliefs, such as described in commonly-assigned U.S. Pat. No. 9,545,204, issued Jan. 17, 2017, the disclosure of which is incorporated by reference. In addition, the cut-outs **22** and longitudinal midsection **23** help minimize interference with and discomfort to breast tissue, particularly in women (and gynecomastic men). The cut-outs **22** and longitudinal midsection **23** further allow better conformity of the electrode patch **15** to sternal bowing and to the narrow isthmus of flat skin that can occur along the bottom of the intermammary cleft between the breasts, especially in buxom women. The cut-outs **22** and longitudinal midsection **23** help the electrode patch **15** fit nicely between a pair of female breasts in the intermammary cleft. Still other shapes, cut-outs and conformities to the electrode patch **15** are possible.

The monitor recorder **14** removably and reusably snaps into an electrically non-conductive receptacle **25** during use. The monitor recorder **14** contains electronic circuitry for recording and storing the patient's electrocardiography as sensed via a pair of ECG electrodes provided on the electrode patch **15**, such as described in commonly-assigned U.S. Pat. No. 9,730,593, issued Aug. 15, 2017, the disclosure of which is incorporated by reference. The non-conductive receptacle **25** is provided on the top surface of the flexible backing **20** with a retention catch **26** and tension clip **27** molded into the non-conductive receptacle **25** to conformably receive and securely hold the monitor recorder **14** in place.

The monitor recorder **14** includes a sealed housing that snaps into place in the non-conductive receptacle **25**. FIG. **5** is a perspective view showing the monitor recorder **14** of FIG. **4**. The sealed housing **50** of the monitor recorder **14** intentionally has a rounded isosceles trapezoidal-like shape **52**, when viewed from above, such as described in commonly-assigned U.S. Design Patent No. D717955, issued Nov. 18, 2014, the disclosure of which is incorporated by reference. The edges **51** along the top and bottom surfaces are rounded for patient comfort. The sealed housing **50** is approximately 47 mm long, 23 mm wide at the widest point, and 7 mm high, excluding a patient-operable tactile-feedback button **55**. The sealed housing **50** can be molded out of polycarbonate, ABS, or an alloy of those two materials. The button **55** is waterproof and the button's top outer surface is molded silicon rubber or similar soft pliable material. A retention detent **53** and tension detent **54** are molded along the edges of the top surface of the housing **50** to respectively engage the retention catch **26** and the tension clip **27** molded into non-conductive receptacle **25**. Other shapes, features, and conformities of the sealed housing **50** are possible.

The electrode patch **15** is intended to be disposable. The monitor recorder **14**, however, is reusable and can be transferred to successive electrode patches **15** to ensure continuity of monitoring. The placement of the wearable monitor **12** in a location at the sternal midline **16** (or immediately to either side of the sternum **13**) benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch **15** anywhere within the general region of the sternum **13**.

As a result, at any point during ECG monitoring, the patient's skin is able to recover from the wearing of an electrode patch **15**, which increases patient comfort and satisfaction, while the monitor recorder **14** ensures ECG

monitoring continuity with minimal effort. A monitor recorder 14 is merely unsnapped from a worn out electrode patch 15, the worn out electrode patch 15 is removed from the skin, a new electrode patch 15 is adhered to the skin, possibly in a new spot immediately adjacent to the earlier location, and the same monitor recorder 14 is snapped into the new electrode patch 15 to reinitiate and continue the ECG monitoring.

During use, the electrode patch 15 is first adhered to the skin in the sternal region. FIG. 6 is a perspective view showing the extended wear electrode patch 15 of FIG. 4 without a monitor recorder 14 inserted. A flexible circuit 32 is adhered to each end of the flexible backing 20. A distal circuit trace 33 and a proximal circuit trace (not shown) electrically couple ECG electrodes (not shown) to a pair of electrical pads 34. The electrical pads 34 are provided within a moisture-resistant seal 35 formed on the bottom surface of the non-conductive receptacle 25. When the monitor recorder 14 is securely received into the non-conductive receptacle 25, that is, snapped into place, the electrical pads 34 interface to electrical contacts (not shown) protruding from the bottom surface of the monitor recorder 14, and the moisture-resistant seal 35 enables the monitor recorder 14 to be worn at all times, even during bathing or other activities that could expose the monitor recorder 14 to moisture.

In addition, a battery compartment 36 is formed on the bottom surface of the non-conductive receptacle 25, and a pair of battery leads (not shown) electrically interface the battery to another pair of the electrical pads 34. The battery contained within the battery compartment 35 can be replaceable, rechargeable or disposable.

The monitor recorder 14 draws power externally from the battery provided in the non-conductive receptacle 25, thereby uniquely obviating the need for the monitor recorder 14 to carry a dedicated power source. FIG. 7 is a bottom plan view of the monitor recorder 14 of FIG. 4. A cavity 58 is formed on the bottom surface of the sealed housing 50 to accommodate the upward projection of the battery compartment 36 from the bottom surface of the non-conductive receptacle 25, when the monitor recorder 14 is secured in place on the non-conductive receptacle 25. A set of electrical contacts 56 protrude from the bottom surface of the sealed housing 50 and are arranged in alignment with the electrical pads 34 provided on the bottom surface of the non-conductive receptacle 25 to establish electrical connections between the electrode patch 15 and the monitor recorder 14. In addition, a seal coupling 57 circumferentially surrounds the set of electrical contacts 56 and securely mates with the moisture-resistant seal 35 formed on the bottom surface of the non-conductive receptacle 25.

The placement of the flexible backing 20 on the sternal midline 16 (or immediately to either side of the sternum 13) also helps to minimize the side-to-side movement of the wearable monitor 12 in the left- and right-handed directions during wear. To counter the dislodgment of the flexible backing 20 due to compressional and torsional forces, a layer of non-irritating adhesive, such as hydrocolloid, is provided at least partially on the underside, or contact surface of the flexible backing 20, but only on the distal end 30 and the proximal end 31. As a result, the underside, or contact surface of the longitudinal midsection 23 does not have an adhesive layer and remains free to move relative to the skin. Thus, the longitudinal midsection 23 forms a crimp relief that respectively facilitates compression and twisting of the flexible backing 20 in response to compressional and torsional forces. Other forms of flexible backing crimp reliefs are possible.

Unlike the flexible backing 20, the flexible circuit 32 is only able to bend and cannot stretch in a planar direction. The flexible circuit 32 can be provided either above or below the flexible backing 20. FIG. 8 is a top view showing the flexible circuit 32 of the extended wear electrode patch 15 of FIG. 4 when mounted above the flexible backing 20. A distal ECG electrode 38 and proximal ECG electrode 39 are respectively coupled to the distal and proximal ends of the flexible circuit 32. A strain relief 40 is defined in the flexible circuit 32 at a location that is partially underneath the battery compartment 36 when the flexible circuit 32 is affixed to the flexible backing 20. The strain relief 40 is laterally extendable to counter dislodgment of the ECG electrodes 38, 39 due to tensile and torsional forces. A pair of strain relief cutouts 41 partially extend transversely from each opposite side of the flexible circuit 32 and continue longitudinally towards each other to define in 'S'-shaped pattern, when viewed from above. The strain relief respectively facilitates longitudinal extension and twisting of the flexible circuit 32 in response to tensile and torsional forces. Other forms of circuit board strain relief are possible.

ECG monitoring and other functions performed by the monitor recorder 14 are provided through a micro controlled architecture. FIG. 9 is a functional block diagram showing the component architecture of the circuitry 60 of the monitor recorder 14 of FIG. 4. The circuitry 60 is externally powered through a battery provided in the non-conductive receptacle 25 (shown in FIG. 6). Both power and raw ECG signals, which originate in the pair of ECG electrodes 38, 39 (shown in FIG. 8) on the distal and proximal ends of the electrode patch 15, are received through an external connector 65 that mates with a corresponding physical connector on the electrode patch 15. The external connector 65 includes the set of electrical contacts 56 that protrude from the bottom surface of the sealed housing 50 and which physically and electrically interface with the set of pads 34 provided on the bottom surface of the non-conductive receptacle 25. The external connector includes electrical contacts 56 for data download, microcontroller communications, power, analog inputs, and a peripheral expansion port. The arrangement of the pins on the electrical connector 65 of the monitor recorder 14 and the device into which the monitor recorder 14 is attached, whether an electrode patch 15 or download station (not shown), follow the same electrical pin assignment convention to facilitate interoperability. The external connector 65 also serves as a physical interface to a download station that permits the retrieval of stored ECG monitoring data, communication with the monitor recorder 14, and performance of other functions.

Operation of the circuitry 60 of the monitor recorder 14 is managed by a microcontroller 61. The micro-controller 61 includes a program memory unit containing internal flash memory that is readable and writeable. The internal flash memory can also be programmed externally. The micro-controller 61 draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. The microcontroller 61 connects to the ECG front end circuit 63 that measures raw cutaneous electrical signals and generates an analog ECG signal representative of the electrical activity of the patient's heart over time.

The circuitry 60 of the monitor recorder 14 also includes a flash memory 62, which the micro-controller 61 uses for storing ECG monitoring data and other physiology and information. The flash memory 62 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. Data is stored in a serial flash memory circuit, which supports read, erase and pro-

gram operations over a communications bus. The flash memory 62 enables the microcontroller 61 to store digitized ECG data. The communications bus further enables the flash memory 62 to be directly accessed externally over the external connector 65 when the monitor recorder 14 is

The circuitry 60 of the monitor recorder 14 further includes an actigraphy sensor 64 implemented as a 3-axis accelerometer. The accelerometer may be configured to generate interrupt signals to the microcontroller 61 by independent initial wake up and free fall events, as well as by device position. In addition, the actigraphy provided by the accelerometer can be used during post-monitoring analysis to correct the orientation of the monitor recorder 14 if, for instance, the monitor recorder 14 has been inadvertently installed upside down, that is, with the monitor recorder 14 oriented on the electrode patch 15 towards the patient's feet, as well as for other event occurrence analyses, such as described in commonly-assigned, U.S. Pat. No. 9,737,224, issued Aug. 22, 2017, the disclosure of which is incorporated by reference.

The microcontroller 61 includes an expansion port that also utilizes the communications bus. External devices, separately drawing power externally from the battery provided on the electrode patch 15 or other source, can interface to the microcontroller 61 over the expansion port in half duplex mode. For instance, an external physiology sensor can be provided as part of the circuitry 60 of the monitor recorder 14, or can be provided on the electrode patch 15 with communication with the microcontroller 61 provided over one of the electrical contacts 56. The physiology sensor can include a SpO₂ sensor, blood pressure sensor, temperature sensor, respiratory rate sensor, glucose sensor, airflow sensor, volumetric pressure sensing, or other types of sensor or telemetric input sources. For instance, the integration of an airflow sensor is described in commonly-assigned U.S. Pat. No. 9,364,155, issued Jun. 14, 2016, the disclosure of which is incorporated by reference. In a further embodiment, a wireless interface for interfacing with other wearable (or implantable) physiology monitors, as well as data offload and programming, can be provided as part of the circuitry 60 of the monitor recorder 14, or can be provided on the electrode patch 15 with communication with the microcontroller 61 provided over one of the electrical contacts 56, such as described in commonly-assigned U.S. Pat. No. 9,433,367, issued Sep. 6, 2016 the disclosure of which is incorporated by reference.

Finally, the circuitry 60 of the monitor recorder 14 includes patient-interfaceable components, including a tactile feedback button 66, which a patient can press to mark events or to perform other functions, and a buzzer 67, such as a speaker, magnetic resonator or piezoelectric buzzer. The buzzer 67 can be used by the microcontroller 61 to output feedback to a patient such as to confirm power up and initiation of ECG monitoring. Still other components as part of the circuitry 60 of the monitor recorder 14 are possible.

While the monitor recorder 14 operates under micro control, most of the electrical components of the electrode patch 15 operate passively. FIG. 10 is a functional block diagram showing the circuitry 70 of the extended wear electrode patch 15 of FIG. 4. The circuitry 70 of the electrode patch 15 is electrically coupled with the circuitry 60 of the monitor recorder 14 through an external connector 74. The external connector 74 is terminated through the set of pads 34 provided on the bottom of the non-conductive receptacle 25, which electrically mate to corresponding electrical contacts 56 protruding from the bottom surface of

the sealed housing 50 to electrically interface the monitor recorder 14 to the electrode patch 15.

The circuitry 70 of the electrode patch 15 performs three primary functions. First, a battery 71 is provided in a battery compartment formed on the bottom surface of the non-conductive receptacle 25. The battery 71 is electrically interfaced to the circuitry 60 of the monitor recorder 14 as a source of external power. The unique provisioning of the battery 71 on the electrode patch 15 provides several advantages. First, the locating of the battery 71 physically on the electrode patch 15 lowers the center of gravity of the overall wearable monitor 12 and thereby helps to minimize shear forces and the effects of movements of the patient and clothing. Moreover, the housing 50 of the monitor recorder 14 is sealed against moisture and providing power externally avoids having to either periodically open the housing 50 for the battery replacement, which also creates the potential for moisture intrusion and human error, or to recharge the battery, which can potentially take the monitor recorder 14 off line for hours at a time. In addition, the electrode patch 15 is intended to be disposable, while the monitor recorder 14 is a reusable component. Each time that the electrode patch 15 is replaced, a fresh battery is provided for the use of the monitor recorder 14, which enhances ECG monitoring performance quality and duration of use. Finally, the architecture of the monitor recorder 14 is open, in that other physiology sensors or components can be added by virtue of the expansion port of the microcontroller 61. Requiring those additional sensors or components to draw power from a source external to the monitor recorder 14 keeps power considerations independent of the monitor recorder 14. Thus, a battery of higher capacity could be introduced when needed to support the additional sensors or components without effecting the monitor recorders circuitry 60.

Second, the pair of ECG electrodes 38, 39 respectively provided on the distal and proximal ends of the flexible circuit 32 are electrically coupled to the set of pads 34 provided on the bottom of the non-conductive receptacle 25 by way of their respective circuit traces 33, 37. The signal ECG electrode 39 includes a protection circuit 72, which is an inline resistor that protects the patient from excessive leakage current.

Last, in a further embodiment, the circuitry 70 of the electrode patch 15 includes a cryptographic circuit 73 to authenticate an electrode patch 15 for use with a monitor recorder 14. The cryptographic circuit 73 includes a device capable of secure authentication and validation. The cryptographic device 73 ensures that only genuine, non-expired, safe, and authenticated electrode patches 15 are permitted to provide monitoring data to a monitor recorder 14.

The monitor recorder 14 continuously monitors the patient's heart rate and physiology. FIG. 11 is a flow diagram showing a monitor recorder-implemented method 100 for monitoring ECG data for use in the monitor recorder 14 of FIG. 4. Initially, upon being connected to the set of pads 34 provided with the non-conductive receptacle 25 when the monitor recorder 14 is snapped into place, the microcontroller 61 executes a power up sequence (step 101) and performs self-authentication of the electrode patch 15 (step 102). During the power up sequence, the voltage of the battery 71 is checked, the state of the flash memory 62 is confirmed, both in terms of operability check and available capacity, and microcontroller operation is diagnostically confirmed.

Self-authentication is performed between the microcontroller 61 and the electrode patch 15 each time that the monitor recorder 14 is inserted into an electrode patch 15 (or

other accessory) to ensure patient safety. An authenticated patch will conform to product quality standards, as well as applicable federal regulatory quality requirements and international standards, such as ISO 13485, IEC 60601-2-47 and IEC 60601-1. Quality assurance, through self-authentication, is crucial, as electrode patches **15** and other accessories may be authorized, but may not necessarily be manufactured, by the entity ultimately responsible for quality standards compliance. Self-authentication mitigates the risk of incorrect device output due to non-compliant accessories.

In one embodiment, the micro-controller **61** contains a private key or a precomputed digest, of which the electrode patch **15** (or other accessory) will have a copy. To authenticate an electrode patch **15** (or other accessory), the micro-controller **61** will challenge the electrode patch **15** (or other accessory) using a code hashed with the private key or precomputed digest. If the electrode patch **15** (or other accessory) responds correctly, the micro-controller **61** will continue with normal program execution. Otherwise, the monitor recorder **14** will signal an error condition, such as chirping the buzzer **67** to notify the patient. Failing self-authentication, other actions could also be taken.

In a further embodiment, an electrode patch **15** (or other accessory) can be set to operate for only a certain period of time. Upon authentication, the monitor recorder **14** will run with that electrode patch **15** (or other accessory) until the electrode patch **15** (or other accessory) is depleted. If the electrode patch **15** (or other accessory) is detected to be expired during self-authentication, the monitor recorder **14** will fail to operate or signal an error condition. To cause an electrode patch **15** (or other accessory) to expire after a certain amount of time has elapsed, the micro-controller **61** periodically writes into the read-only memory (ROM) of the cryptographic circuit **73**. After the data in the ROM written by the micro-controller **61** has reached a certain fullness, the micro-controller **61** will turn off to ensure that an expired electrode patch **15** (or other accessory) does not create an unsafe condition, such as an incorrect output. Still other forms of authentication and device expiration are possible.

Following satisfactory completion of the power up sequence, an iterative processing loop (steps **103-110**) is continually executed by the microcontroller **61**. During each iteration (step **103**) of the processing loop, the ECG frontend **63** (shown in FIG. 9) continually senses the cutaneous ECG electrical signals (step **104**) via the ECG electrodes **38, 29** and is optimized to maintain the integrity of the P-wave. A sample of the ECG signal is read (step **105**) by the micro-controller **61** by sampling the analog ECG signal output front end **63**. FIG. 12 is a graph showing, by way of example, a typical ECG waveform **110**. The x-axis represents time in approximate units of tenths of a second. The y-axis represents cutaneous electrical signal strength in approximate units of millivolts. The P-wave **111** has a smooth, normally upward, that is, positive, waveform that indicates atrial depolarization. The QRS complex usually begins with the downward deflection of a Q wave **112**, followed by a larger upward deflection of an R-wave **113**, and terminated with a downward waveform of the S wave **114**, collectively representative of ventricular depolarization. The T wave **115** is normally a modest upward waveform, representative of ventricular depolarization, while the U wave **116**, often not directly observable, indicates the recovery period of the Purkinje conduction fibers.

Sampling of the R-to-R interval enables heart rate information derivation. For instance, the R-to-R interval represents the ventricular rate and rhythm, while the P-to-P interval represents the atrial rate and rhythm. Importantly,

the PR interval is indicative of atrioventricular (AV) conduction time and abnormalities in the PR interval can reveal underlying heart disorders, thus representing another reason why the P-wave quality achievable by the extended wear ambulatory electrocardiography and physiological sensor monitor described herein is medically unique and important. The long-term observation of these ECG indicia, as provided through extended wear of the wearable monitor **12**, provides valuable insights to the patient's cardiac function and overall well-being.

Each sampled ECG signal, in quantized and digitized form, is temporarily staged in buffer (step **106**), pending compression preparatory to storage in the flash memory **62** (step **107**). Following compression, the compressed ECG digitized sample is again buffered (step **108**), then written to the flash memory **62** (step **109**) using the communications bus. Processing continues (step **110**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

The patient management program **123** could manage a subscription service that authorizes a monitor recorder **14** to operate for a set period of time or under pre-defined operational parameters and privileges. FIG. 13 is a flow diagram showing a method **150** for providing a self-authenticating electrocardiography monitoring circuit in accordance with one embodiment. The method **150** can be implemented in software and execution of the software can be performed on a download station **125**, which could be a programmer or other device, or a computer system, including a server **122** or personal computer **129**, such as further described supra with reference to FIG. 3, as a series of process or method modules or steps.

For convenience, the method **150** will be described in the context of being performed by a personal computer **136** or other connectable computing device (shown in FIG. 3) as middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program. Execution of the method **150** by a computer system would be analogous mutatis mutandis.

Initially, the download station **125** is connected to the monitor recorder **14** (step **151**), such as by physically interfacing to a set of terminals **128** on a paired receptacle **127** or by wireless connection, if available. The data stored on the monitor recorder **14**, including ECG and physiological monitoring data, other recorded data, and other information are retrieved (step **152**) over a hard link **135** using a control program **137** ("Ctl") or analogous application executing on a personal computer **136** or other connectable computing device.

The data retrieved from the monitor recorder **14** is in a proprietary storage format and each datum of recorded ECG monitoring data, as well as any other physiological data or other information, must be converted, so that the data can be used by a third-party post-monitoring analysis program. Each datum of ECG monitoring data is converted by the middleware (steps **153-159**) in an iterative processing loop. During each iteration (step **153**), the ECG datum is read (step **154**) and, if necessary, the gain of the ECG signal is adjusted (step **155**) to compensate, for instance, for relocation or replacement of the electrode patch **15** during the monitoring period.

In addition, depending upon the configuration of the wearable monitor **12**, other physiological data (or other information), including patient events, such as a fall, peak activity level, detection of patient activity levels and states,

15

sedentary detection and so on, may be recorded along with the ECG monitoring data. For instance, actigraphy data may have been sampled by the actigraphy sensor 64 based on a sensed event occurrence, such as a sudden change in orientation due to the patient taking a fall. In response, the monitor recorder 14 will embed the actigraphy data samples into the stream of data, including ECG monitoring data that is recorded to the flash memory 62 by the micro-controller 61. Post-monitoring, the actigraphy data is temporally matched to the ECG data to provide the proper physiological context to the sensed event occurrence. As a result, the three-axis actigraphy signal is turned into an actionable event occurrence that is provided, through conversion by the middleware, to third party post-monitoring analysis programs, along with the ECG recordings contemporaneous to the event occurrence. Other types of processing of the other physiological data (or other information) are possible.

Thus, during execution of the middleware, any other physiological data (or other information) that has been embedded into the recorded ECG monitoring data is read (step 156) and time-correlated to the time frame of the ECG signals that occurred at the time that the other physiological data (or other information) was noted (step 157). Finally, the ECG datum, signal gain adjusted, if appropriate, and other physiological data, if applicable and as time-correlated, are stored in a format suitable to the backend software (step 158) used in post-monitoring analysis.

While the invention has been particularly shown and described as referenced to the embodiments thereof, those skilled in the art will understand that the foregoing and other changes in form and detail may be made therein without departing from the spirit and scope.

What is claimed is:

1. An extended wear electrocardiography and physiological sensor monitor recorder with self-authenticating electrocardiography monitoring circuit, comprising:

a sealed housing adapted to be removably secured into a non-conductive receptacle on an electrode patch; and electronic circuitry comprised within the sealed housing, comprising:

an electrocardiographic front end circuit operable to sense electrocardiographic signals through electrocardiographic electrodes provided on the electrode patch;

flash memory to record the electrocardiographic signals; and

a micro-controller to periodically write data into a memory of the electrode patch on which the sealed housing is removably secured via the non-conductive receptacle during continuous recording of the electrocardiographic signals via the electrocardiographic front end circuit, to determine an expiration of the electrode patch based on an amount of the data stored in the memory of the electrode patch, and to turn off the micro-controller upon the expiration of the electrode patch.

2. An electrocardiography and physiological sensor monitor recorder according to claim 1, wherein the recorded electrocardiographic signals are retrieved via a download station.

3. An electrocardiography and physiological sensor monitor recorder according to claim 2, further comprising:

a set of electrical contacts formed on a surface of the sealed housing; and

a set of terminals on a paired receptacle of the download station and configured to interface with the set of electrical contacts on the sealed housing.

16

4. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

middleware operable to convert the sensed or recorded electrocardiographic signals into a different format as formatted electrocardiography data.

5. An electrocardiography and physiological sensor monitor recorder according to claim 4, wherein the formatted electrocardiography data is retrieved via a server remotely interfaced with a download station.

6. An electrocardiography and physiological sensor monitor recorder according to claim 4, wherein a gain of at least a portion of the formatted electrocardiography data is adjusted to compensate for relocation or replacement of the sealed housing on a wearer.

7. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

one or more sensors configured to record physiological data in response to a sensed event; and

the electronic circuitry configured to embed the physiological data into a stream of the sensed or recorded electrocardiographic signals.

8. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

one or more sensors within the sealed housing or the electrode patch, and configured to record physiological data in response to a sensed event, wherein the physiological data is matched to the sensed or recorded electrocardiographic signals.

9. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

a feedback button formed on a surface of the sealed housing and configured to mark events identified by a wearer.

10. An electrocardiography and physiological sensor monitor recorder according to claim 1, further comprising:

located within the sealed housing, a buzzer comprising a speaker, magnetic resonator or piezoelectric buzzer and configured to output feedback to a wearer.

11. An extended wear electrocardiography and physiological sensor monitor with self-authenticating electrocardiography monitoring circuit, comprising:

an electrode patch, comprising:

an elongated strip of stretchable material;

a pair of electrocardiographic electrodes, each electrocardiographic electrode conductively exposed on a contact surface of a respective end of the elongated strip;

a non-conductive receptacle adhered to an outward-facing surface of the elongated strip and comprising a plurality of electrical pads; and

a circuit affixed on each end of the elongated strip and comprising a pair of circuit traces electrically coupled to the pair of the electrocardiographic electrodes and a pair of the electrical pads; and

an electrocardiography monitor having a sealed housing adapted to be removably secured into the non-conductive receptacle on the electrode patch and electronic circuitry comprised within the sealed housing, comprising:

an electrocardiographic front end circuit operable to sense electrocardiographic signals through the electrocardiographic electrodes provided on the electrode patch;

flash memory to record the electrocardiographic signals; and

an externally-powered micro-controller to periodically write data into a memory of the electrode patch on

17

which the electrocardiography monitor is removably secured via the non-conductive receptacle during continuous recording of the electrocardiographic signals via the front end circuit, to determine an expiration of the electrode patch based on an amount of the data stored in the memory of the electrode patch, and to turn off the micro-controller upon the expiration of the electrode patch.

12. An electrocardiography and physiological sensor monitor according to claim 11, wherein the recorded electrocardiographic signals are retrieved via a download station.

13. An electrocardiography and physiological sensor monitor according to claim 12, further comprising:

- a set of electrical contacts formed on a surface of the sealed housing; and
- a set of terminals on a paired receptacle of the download station and configured to interface with the set of electrical contacts on the sealed housing.

14. An electrocardiography and physiological sensor monitor according to claim 11, further comprising:

- middleware operable to convert the sensed or recorded electrocardiographic signals into a different format as formatted electrocardiography data.

15. An electrocardiography and physiological sensor monitor according to claim 14, wherein the formatted electrocardiography data is retrieved via a server remotely interfaced with a download station.

16. An electrocardiography and physiological sensor monitor according to claim 14, wherein a gain of at least a

18

portion of the formatted electrocardiography data is adjusted to compensate for relocation or replacement of the sealed housing on a wearer.

17. An electrocardiography and physiological sensor monitor according to claim 11, further comprising:

- one or more sensors configured to record physiological data in response to a sensed event; and
- the electronic circuitry configured to embed the physiological data into a stream of the sensed or recorded electrocardiographic signals.

18. An electrocardiography and physiological sensor monitor according to claim 11, further comprising:

- one or more sensors within the sealed housing or the electrode patch, and configured to record physiological data in response to a sensed event, wherein the physiological data is matched to the sensed or recorded electrocardiographic signals.

19. An electrocardiography and physiological sensor monitor according to claim 11, further comprising:

- a feedback button formed on a surface of the sealed housing and configured to mark events identified by a wearer.

20. An electrocardiography and physiological sensor monitor according to claim 11, further comprising:

- located within the sealed housing, a buzzer comprising a speaker, magnetic resonator or piezoelectric buzzer and configured to output feedback to a wearer.

* * * * *

专利名称(译)	自我认证心电图监测电路		
公开(公告)号	US10398334	公开(公告)日	2019-09-03
申请号	US15/602007	申请日	2017-05-22
[标]申请(专利权)人(译)	BARDY诊断		
申请(专利权)人(译)	BARDY诊断, INC.		
当前申请(专利权)人(译)	BARDY诊断, INC.		
[标]发明人	FELIX JASON BARDY GUST H BISHAY JON MIKALSON		
发明人	FELIX, JASON BARDY, GUST H. BISHAY, JON MIKALSON		
IPC分类号	A61B5/0402 A61B5/0432 A61B5/0408 A61B5/00		
CPC分类号	A61B5/6823 A61B5/0006 A61B5/0022 A61B5/0402 A61B5/04085 A61B5/04087 A61B5/04325 A61B2562/08		
优先权	61/882403 2013-09-25 US		
其他公开文献	US20170251948A1		
外部链接	Espacenet		

摘要(译)

可以通过可穿戴式监视器提供生理监测，该监视器包括两个组件，一个灵活的扩展耐磨电极贴片和一个可拆卸的可重复使用的监视器记录器。可穿戴式监视器位于患者胸部的中央（中线），沿着胸骨从上到下。将可穿戴式监视器放置在胸骨中线（或紧邻胸骨的任一侧）的位置，通过消除在整个监测期间将ECG电极连续放置在皮肤上的相同斑点中的要求，有利于延长佩戴。相反，患者可以将电极贴片放置在胸骨的一般区域内的任何位置。通过电极贴片的自我认证，确保ECG记录的质量水平在延长的时间段内保持恒定。监视器记录器在连接到电极贴片时实施挑战响应方案。如果验证失败，监视录像机会发出错误信号。

