



US 20170231597A1

(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2017/0231597 A1**
Howard (43) **Pub. Date: Aug. 17, 2017**(54) **NETWORKED ELECTRONIC
STETHOSCOPE**(71) Applicant: **Newton Howard**, Providence, RI (US)(72) Inventor: **Newton Howard**, Providence, RI (US)(21) Appl. No.: **15/431,221**(22) Filed: **Feb. 13, 2017****Related U.S. Application Data**

(60) Provisional application No. 62/294,421, filed on Feb. 12, 2016.

Publication Classification(51) **Int. Cl.**
A61B 7/04 (2006.01)
A61B 5/0408 (2006.01)
A61B 5/00 (2006.01)(52) **U.S. Cl.**
CPC *A61B 7/04* (2013.01); *A61B 5/0022*
(2013.01); *A61B 5/04085* (2013.01)(57) **ABSTRACT**

Embodiments of the present systems and methods may provide improved electronic stethoscopes that provide diversified diagnosis functionality. For example, embodiments may provide the capability to diagnose a wide range of pathologies by using the device's wireless network capacity to link it to wearable sensors of different kinds, maintaining the traditional use of the stethoscope while enabling it to sense a whole new set of physiological signals. For example, in an embodiment, a system may comprise a networked electronic stethoscope and a sensor adapted to be attached to the networked electronic stethoscope, the sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of a patient, a processor adapted to digitize and process the obtained signal to form data, and a wireless network adapter adapted to transmit the data to the networked electronic stethoscope.

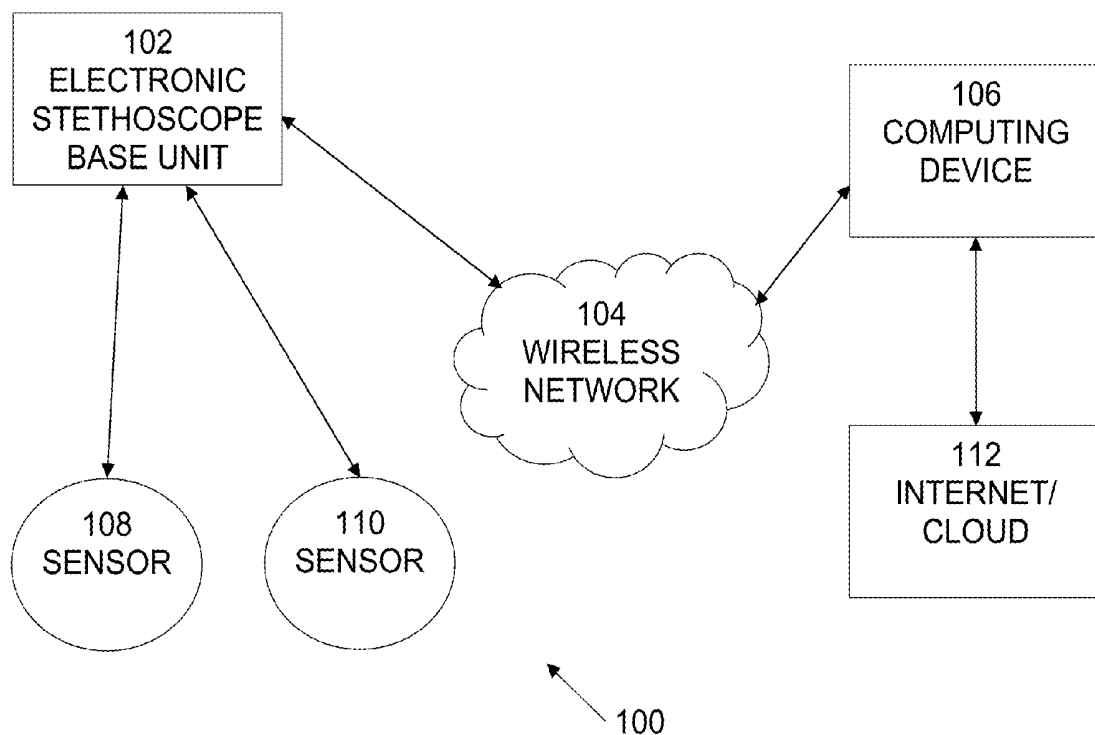


Fig. 1

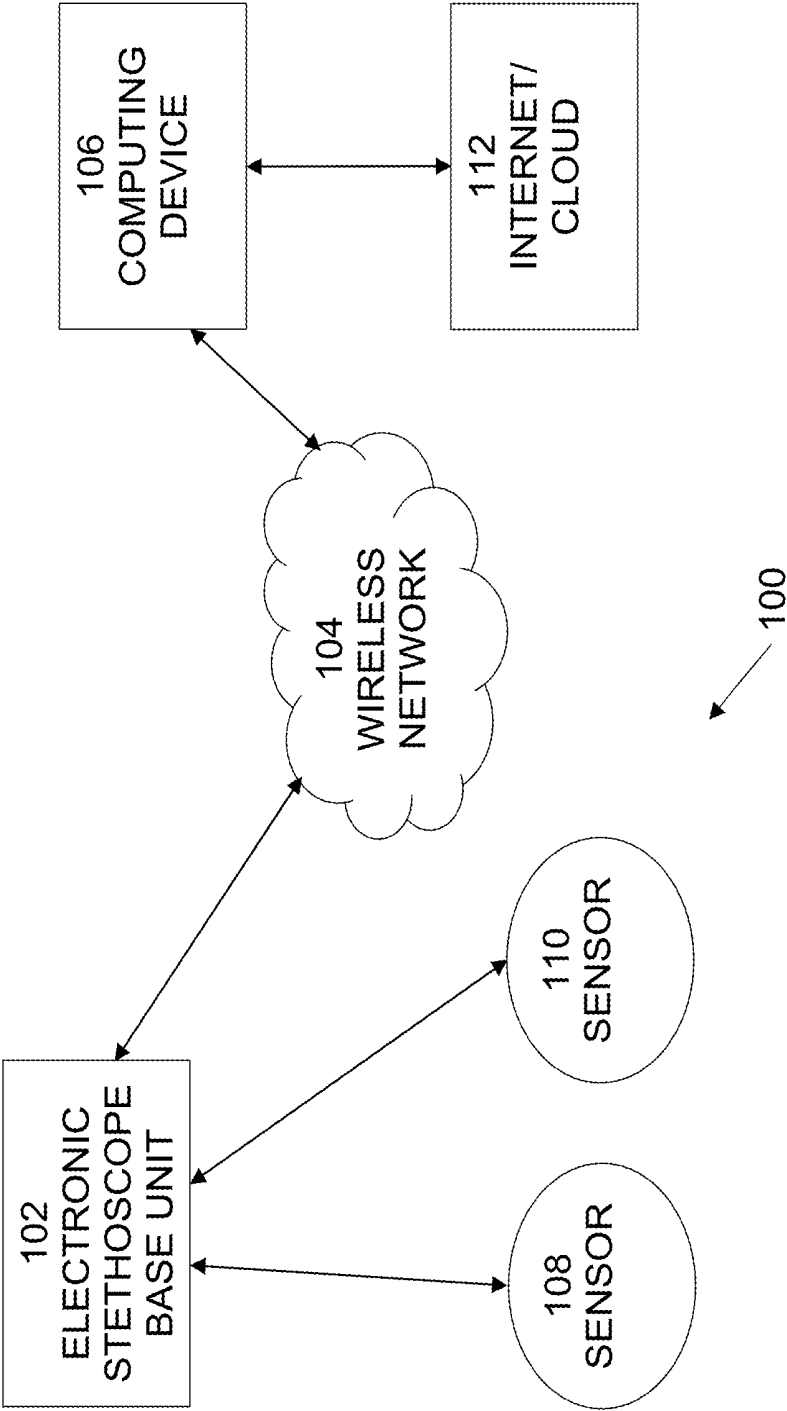


Fig. 2

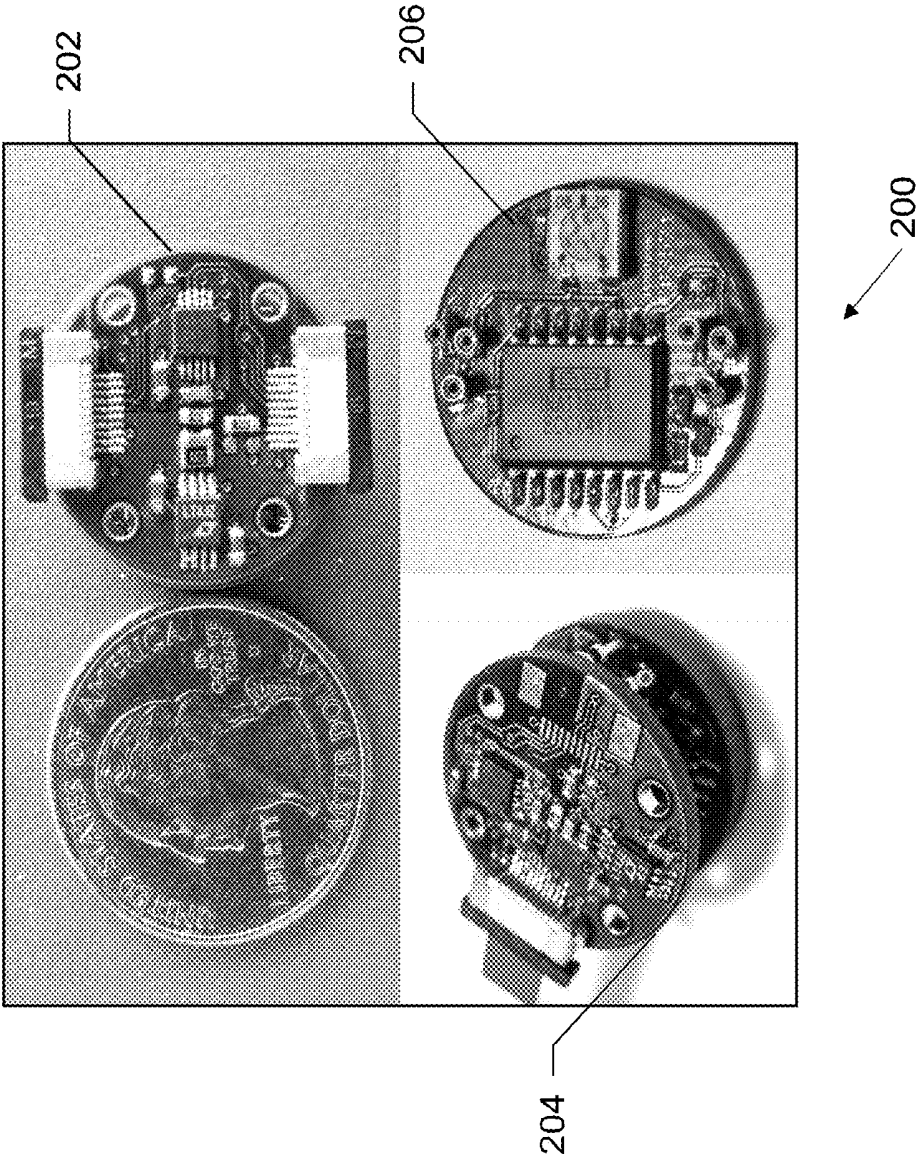


Fig. 3

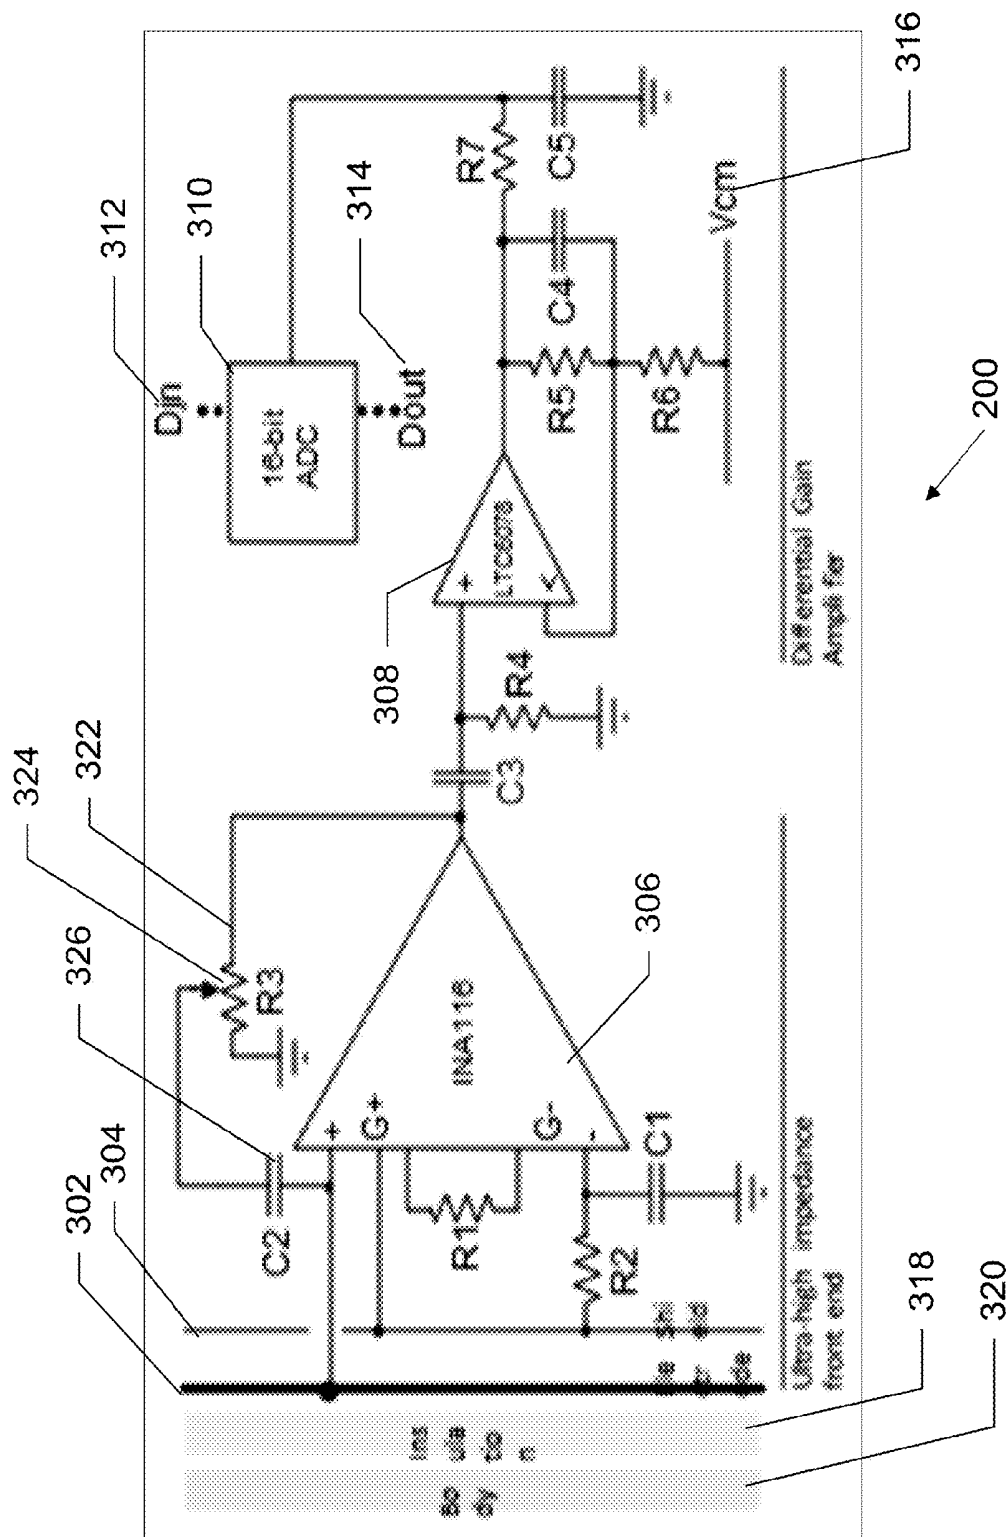


Fig. 4

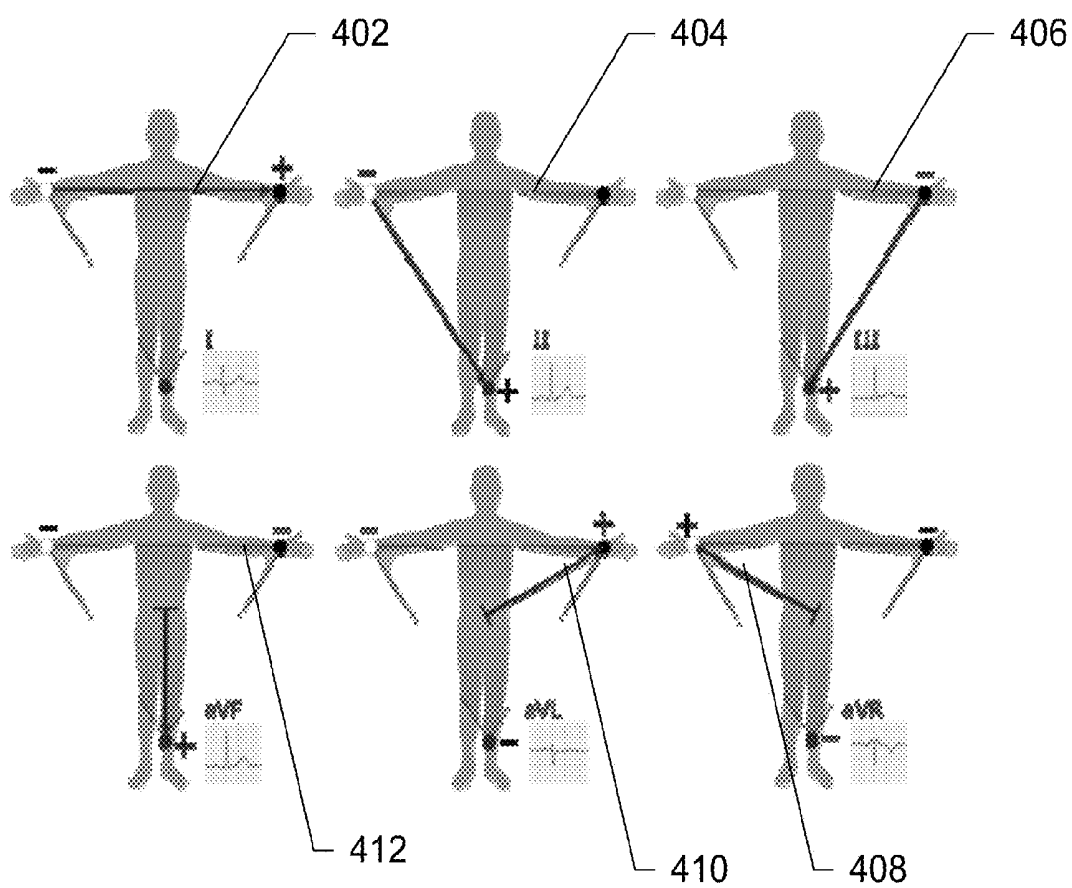


Fig. 5

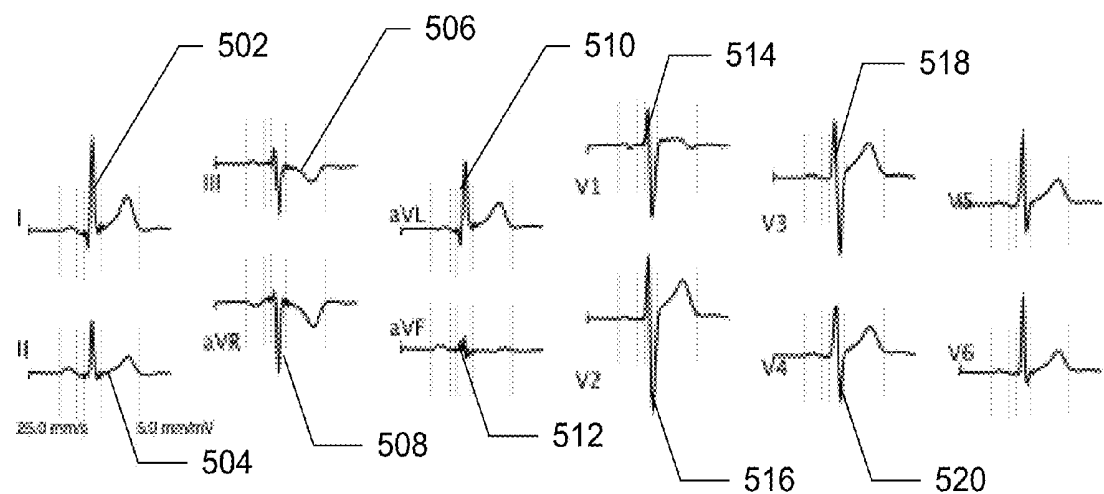


Fig. 6

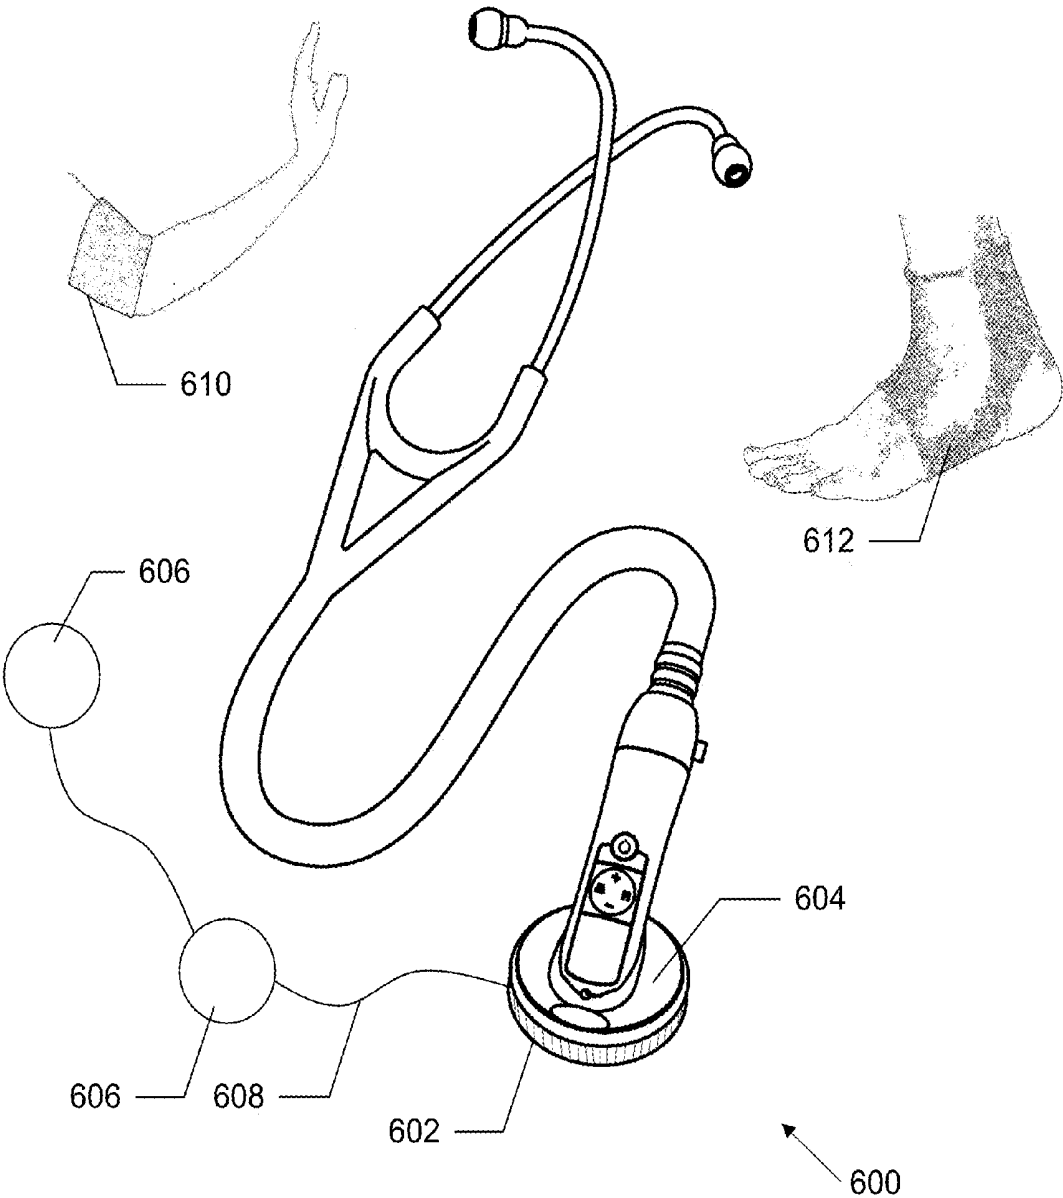


Fig. 7

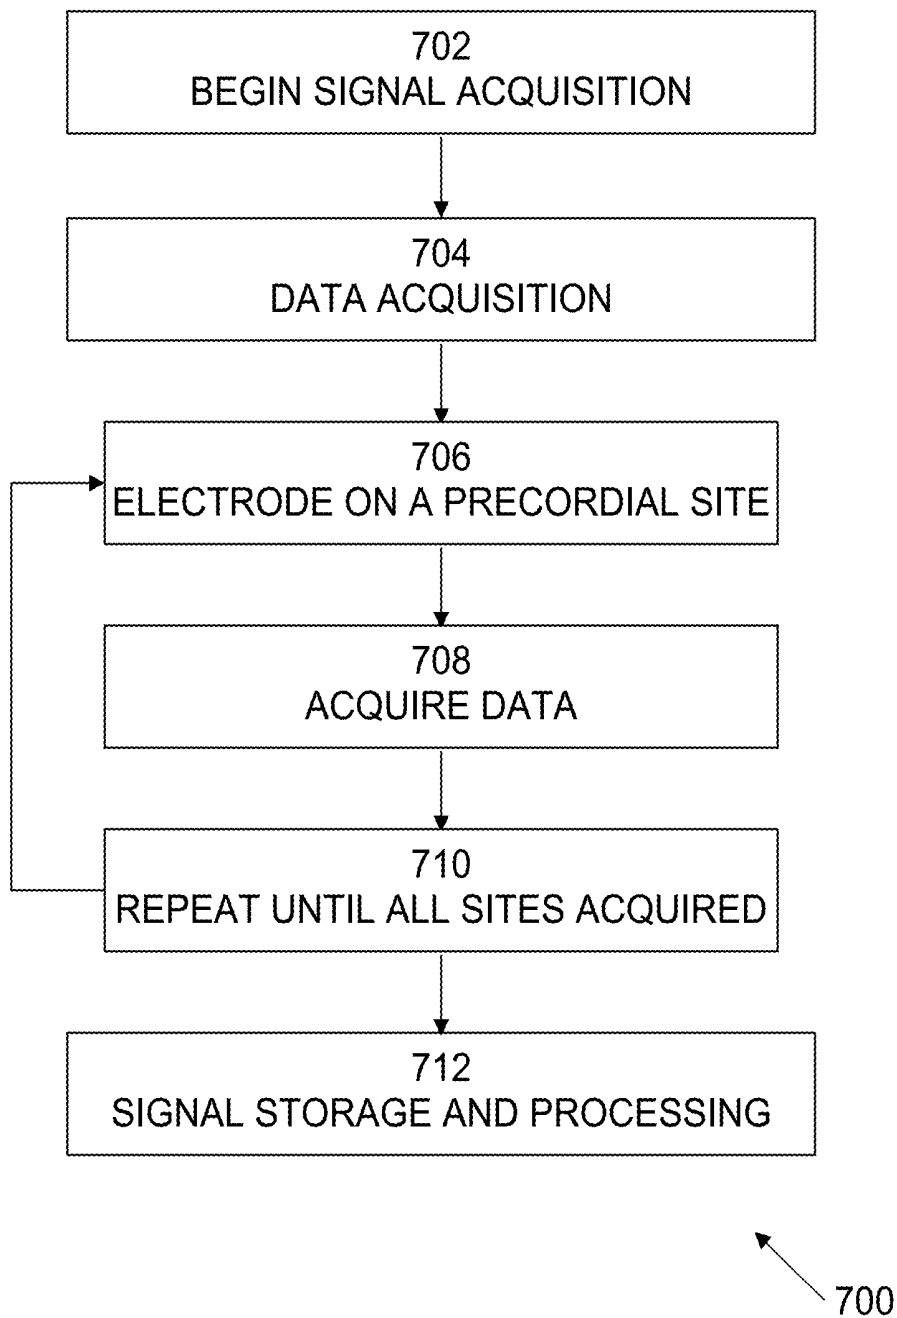


Fig. 8


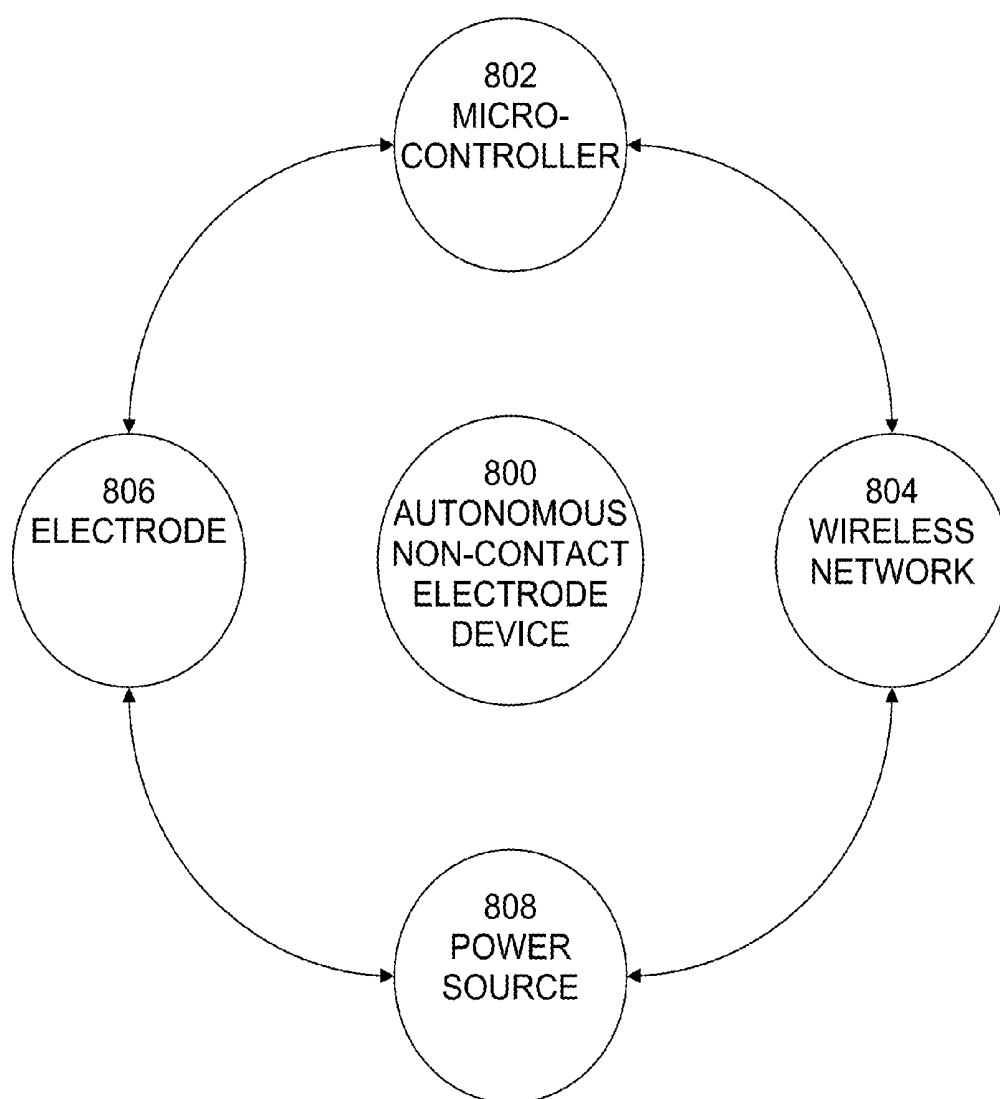


Fig. 9

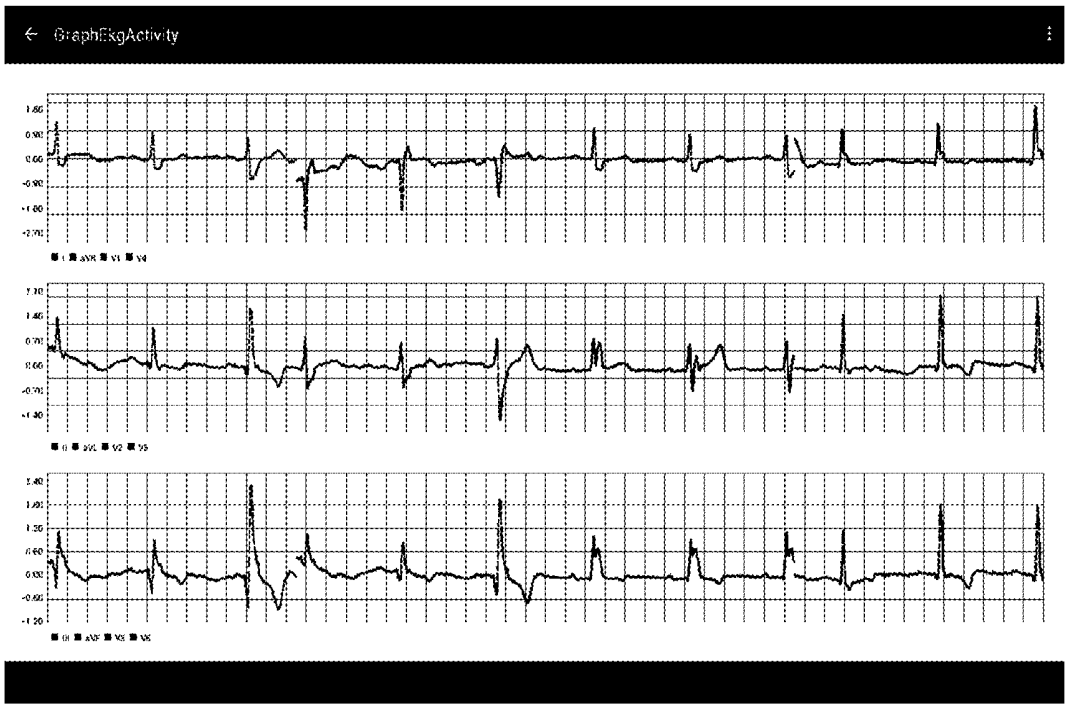

900

Fig 10

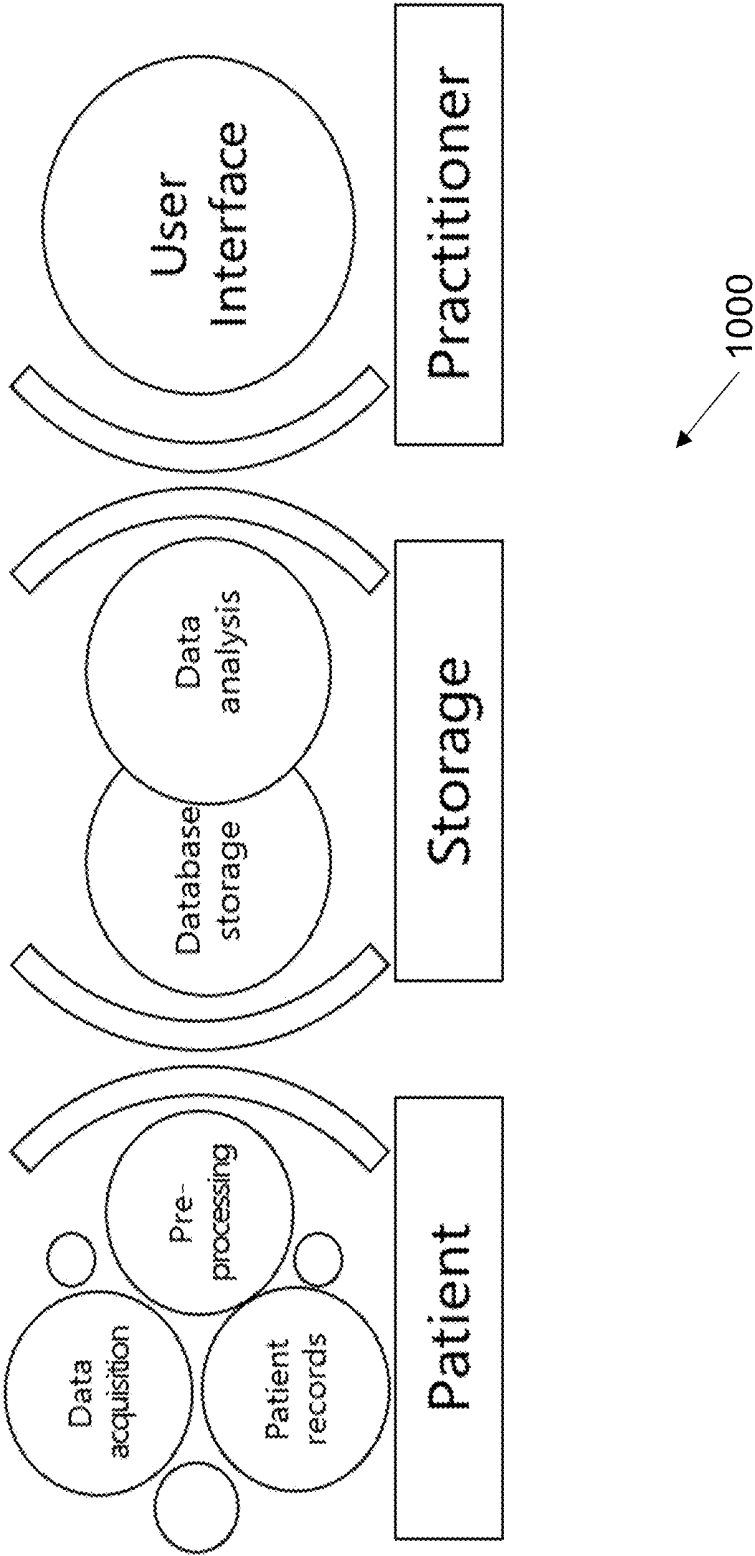


Fig. 11


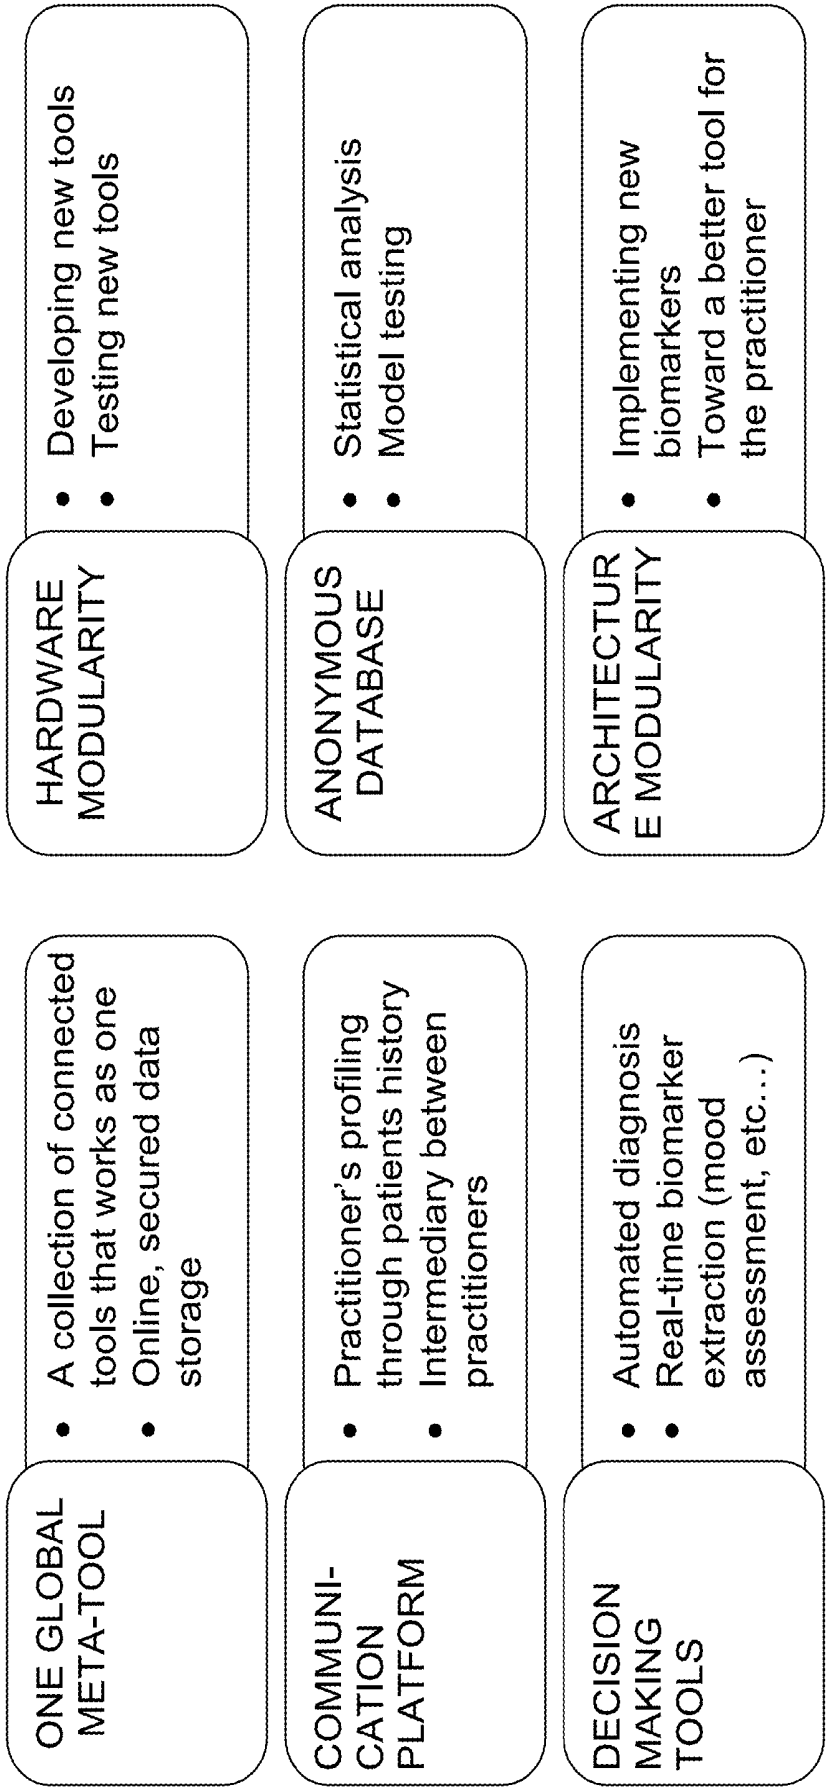


Fig. 12

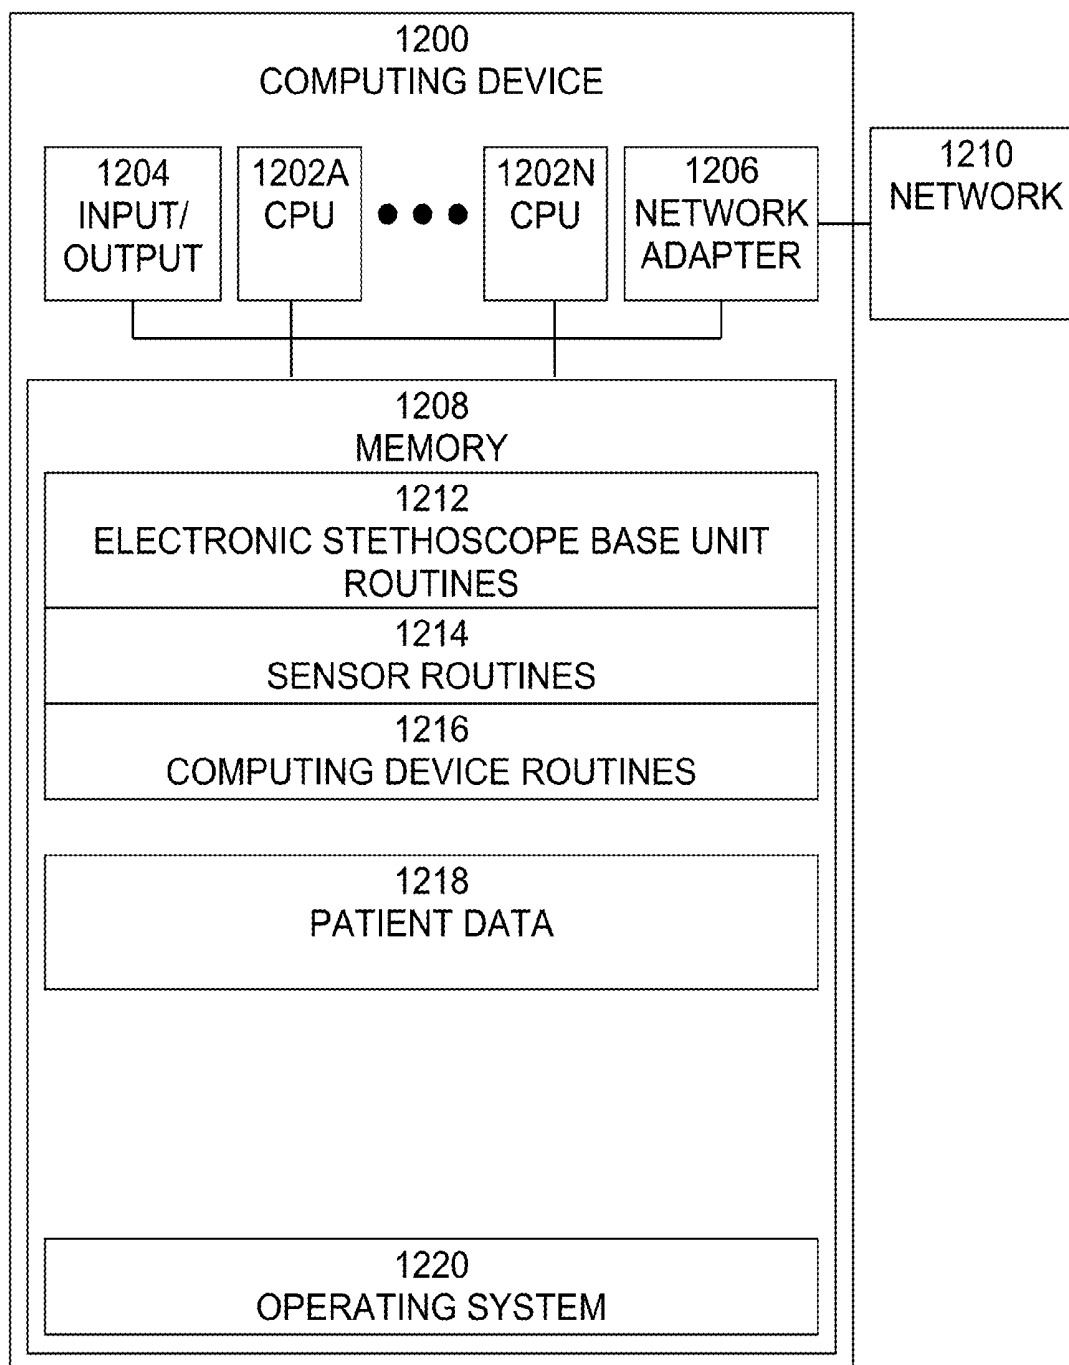

NETWORKED ELECTRONIC STETHOSCOPE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Provisional Application No. 62/294,421, filed Feb. 12, 2016, the contents of which are incorporated herein in their entirety.

BACKGROUND

[0002] The present invention relates to techniques for expanding the functionality of a traditional stethoscope, enabling it to digitally measure and store several physiological signals and transform the common stethoscope into a diversified diagnostic tool which would be useful across a wide spectrum of medical fields.

[0003] Conventional mechanical acoustic stethoscopes may be used to listen to the internal sounds of a body and have been in common use by physicians for many years. More recently, electronic stethoscopes have provided improved functionality over mechanical stethoscopes. A typical electronic stethoscope may include a built-in microphone, connected to a micro controller and a network interface, such as a Bluetooth chip, enabling it to record sounds during patient examination and digitally store the recording in a linked computer through wireless network, such as Bluetooth, communication. Such a stethoscope may possess a built-in controller with a digital screen that can be used to trigger several actions and can be expanded by developers with the help of dedicated APIs.

[0004] However, the conventional electronic stethoscopes still provide relatively limited information, and do not provide diversified diagnosis functionality. Typically, the use of the conventional stethoscope in medicine, while not insignificant, has been limited to pulmonary applications and has not been adapted to diagnose a wider range of pathologies.

[0005] Accordingly, a need arises for improved electronic stethoscopes that provide diversified diagnosis functionality.

SUMMARY

[0006] Embodiments of the present systems and methods may provide improved electronic stethoscopes that provide diversified diagnosis functionality. For example, embodiments may provide the capability to diagnose a wide range of pathologies by using the device's wireless network capacity to link it to wearable sensors of different kinds, maintaining the traditional use of the stethoscope while enabling it to sense a whole new set of physiological signals

[0007] For example, in an embodiment, a system may comprise a networked electronic stethoscope and a sensor adapted to be attached to the networked electronic stethoscope, the sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of a patient, a processor adapted to digitize and process the obtained signal to form data, and a wireless network adapter adapted to transmit the data to the networked electronic stethoscope.

[0008] In an embodiment, the electrode may be a non-contact electrode adapted to obtain a signal representing a physiological parameter of the patient without direct contact with the patient. The system may further comprise at least one additional sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of the

patient. The at least one additional sensor may be communicatively connected to the sensor adapted to be attached to the networked electronic stethoscope. The at least one additional sensor may be communicatively connected to the sensor adapted to be attached to the networked electronic stethoscope via at least one wire. The at least one additional sensor may be communicatively connected to the sensor adapted to be attached to the networked electronic stethoscope via a wireless communication network. The sensor may be adapted to be attached to a membrane support circle the networked electronic stethoscope. The system may further comprise at least one additional sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of the patient. The processor may be adapted to generate a representation of the physiological parameter of the patient based on at least the signal representing the physiological parameter of a patient obtained from the sensor adapted to be attached to the networked electronic stethoscope and the signal representing the physiological parameter of a patient obtained from the at least one additional sensor. The processor may be adapted to generate a plurality of representations of the physiological parameter of the patient based on at least a plurality of signals representing the physiological parameter of a patient obtained from the sensor adapted to be attached to the networked electronic stethoscope, placed at each of a plurality of locations on the patient, and the signal representing a physiological parameter of a patient obtained from the at least one additional sensor. The signal representing the physiological parameter of the patient may be an electrocardiogram (EKG) signal.

[0009] For example, in an embodiment, a method may comprise placing at a location on a patient at least one sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of the patient, repeatedly placing at a different location on the patient a sensor attached to a networked electronic stethoscope, the networked electronic stethoscope comprising an electrode adapted to obtain a signal representing a physiological parameter of a patient, a processor adapted to digitize and process the obtained signal to form data, and a wireless network adapter adapted to transmit the data to the networked electronic stethoscope, and for each different location on the patient at which the sensor is placed, obtaining the signal representing the physiological parameter of the patient.

[0010] In an embodiment, the electrodes may be non-contact electrodes adapted to obtain a signal representing a physiological parameter of the patient without direct contact with the patient. The at least one sensor may be communicatively connected to the sensor attached to the networked electronic stethoscope. The at least one sensor may be communicatively connected to the sensor attached to the networked electronic stethoscope via at least one wire. The at least one sensor is communicatively connected to the sensor attached to the networked electronic stethoscope via a wireless communication network. The signal representing the physiological parameter of the patient is an electrocardiogram (EKG) signal.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] The details of the present invention, both as to its structure and operation, can best be understood by referring to the accompanying drawings, in which like reference numbers and designations refer to like elements.

[0012] FIG. 1 is an exemplary block diagram of a communication network, in which embodiments of the present systems and methods may be implemented.

[0013] FIG. 2 is an exemplary diagram of exemplary embodiment of a sensor, such as a non-contact electrode device.

[0014] FIG. 3 is an exemplary schematic diagram of an embodiment of a wireless non-contact electrode sensor.

[0015] FIG. 4 is an exemplary diagram of voltage differences making up the Limb Leads and Augmented Limb Leads.

[0016] FIG. 5 is an exemplary diagram of an embodiment of signals detected on each of the leads.

[0017] FIG. 6 is an exemplary diagram of an embodiment of a networked electronic stethoscope.

[0018] FIG. 7 is an exemplary flow diagram of an embodiment of a process for acquiring physiological data from a patient.

[0019] FIG. 8 is an exemplary diagram of an embodiment of a wireless sensor electrode device.

[0020] FIG. 9 is an exemplary diagram of an embodiment of an electro-cardiogram (EKG) display.

[0021] FIG. 10 is an exemplary diagram of an embodiment of a communication platform.

[0022] FIG. 11 is an exemplary diagram of advantages provided by an embodiment of a communication platform.

[0023] FIG. 12 is an exemplary diagram of an embodiment of a computing device, in which processes involved in the embodiments described herein may be implemented.

DETAILED DESCRIPTION

[0024] Embodiments of the present systems and methods may provide improved electronic stethoscopes that provide diversified diagnosis functionality. For example, embodiments may provide the capability to diagnose a wide range of pathologies by using the device's wireless network capacity to link it to wearable sensors of different kinds, maintaining the traditional use of the stethoscope while enabling it to sense a whole new set of physiological signals

[0025] An exemplary block diagram of a communication network 100, in which embodiments of the present systems and methods may be implemented, is shown in FIG. 1. Network 100 may include electronic stethoscope/base unit 102, wireless network 104, computing device 106, and sensors 108, 110, and computing device 106 may be connected to the Internet and/or cloud facilities 112. Electronic stethoscope/base unit 102 may include functionality of a conventional stethoscope, but also may provide the capability to record signals from sensors 108, 110 and digitally store the recordings in a linked computing device 106 through wireless network 104. Such a system may provide the capability for a patient can get their recordings, and submit them to other practitioners for second opinion without need of any redundant examination. Further, doctors can analyze the recordings later in a non-clinical setting, can replay the recordings, and can even apply different layers of filtration and signal processing algorithms on the recording. Further, patient data may be uploaded to the cloud 112 to be applied against volumes of prior patient data for research purposes or even automated diagnostic assistance.

[0026] Wireless network 104 may include any type of wireless communication network that may be used to communicate information. Computing device 106 may be any type or number of computers or data processing systems,

including, but not limited to personal computers, servers, special purpose data processors, etc. Sensors 108, 110 may include any type of sensor that may be used to obtain information about physical parameters of signals of a living organism. Examples of such sensors may include, but are not limited to, acoustic sensors, pressure sensors, optical sensors, temperature sensors, electrical sensors, etc. Sensors 108, 110 may be communicatively connected to electronic stethoscope/base unit 102. Such communicative connections may use wired or wireless connections. In addition, sensors 108, 110 may be physically or electrically connected to electronic stethoscope/base unit 102, or sensors 108, 110 may be physically or electrically remote from, or isolated from, electronic stethoscope/base unit 102.

[0027] For example, electronic stethoscope/base unit 102 may include wireless network, such as Bluetooth, capability, which may be used to link electronic stethoscope/base unit 102 with sensors 108, 110 of different kinds, such as wearable sensors. For example, electronic stethoscope/base unit 102 may provide EKG acquisition functionality. This may be done without overcomplicating data acquisition and minimally disrupting existing clinical processes. Important elements within an EKG machine are its electrode sets. Accordingly, wireless electrodes in combination with a wireless network stethoscope, may provide advantageous functionality.

[0028] Sensors 108, 110 may include a set of capacitive electrodes manufactured on a printed circuit board that is able to operate through fabric or other insulation. An exemplary embodiment of a sensor, such as a non-contact electrode device 200 is shown in FIG. 2. The upper PCB 202 may include a differential amplifier and ADC along with two serial daisy chain connectors. A side view of the electrode 204 shows the upper PCB 202 and lower PCB 206 joined together. The lower PCB 206 may include an ultra-high input impedance amplifier front-end. The bottom of this PCB may be a solid, insulated copper fill, which may function as a capacitive electrode.

[0029] In an exemplary embodiment, an electrode device 200 may provide 46 dB of gain over a 0.7-100 Hz bandwidth with a noise level of 3.8 μ V RMS for high quality brain and cardiac recordings. Signals may be digitized directly in the device 200 and are may be transmitted over a wired or wireless connection. For example, a wired connection may include a digital serial daisy chain connecting all of the electrodes, which would minimize the number of wires required on the body. Referring briefly to FIG. 1, a small wireless base unit 102 may transmit EEG/EKG telemetry to a computing device 106 for storage and processing.

[0030] The system may include a set of non-contact biopotential sensors 200 which may be connected along a single common wire. An exemplary schematic diagram of a wireless non-contact electrode sensor 200 is shown in FIG. 3. The sensors 200 may either be in direct contact with the skin or embedded within fabric and clothing. Sensors 200 may include an electrode 302 to detect the desired signal, a single adhesive or dry contact sensor (not shown) that may be placed anywhere convenient is used to establish the ground reference for the system. As shown in FIG. 3, a sensor 200 may include an ultra-high input impedance front-end amplifier 306, such as an INA116, a differential amplifier 308, such as an LTC6078, and an analog-to-digital converter (ADC) 310, such as a 16-bit ADC. The voltages at nodes Din 312, Dout 312, and Vcm 312 may be carried along the daisy

chain. Each electrode may be constructed from two PCBs, each, for example, the size of a US quarter, stacked upon one another. The upper PCB contains a low noise differential amplifier and a 16-bit ADC. Rather than outputting a single analog signal, the electrode may output a digitized value, which can be carried in a serial daisy chain to drastically reduce the number of wires needed. A miniature ribbon cable may carry the power supply, digital control as well as analog common mode reference from electrode-to-electrode.

[0031] The lower PCB contains the INA116, configured as an ultra-high input impedance amplifier. The bottom surface of the PCB is a solid copper fill, insulated by a solder mask, which functions as the electrode. This surface forms a coupling capacitor with the body. An active shield formed in a solid inner plane protects the electrode from external noise pick-up. To minimize the shield capacitance, an extra thick PCB is used for the electrode. The full schematic of the two PCBs of the non-contact electrode is shown in FIG. 2, above.

[0032] Designing an ultra-high input impedance amplifier with low noise levels is the main challenge in implementing non-contact electrodes. A simplified, generic model for a capacitive sensor that is directly applicable to the circuit used in this design is shown in FIG. 3. The sensor may include electrode **302** to detect the desired signal, an electrical shield **304**, and insulation **318** to prevent direct electrical contact with the body **320** of the subject being monitored. Signal sources from the body (EEG/EKG) may be thought of as a voltage source, V_s , connected to the input of an amplifier via a small coupling capacitance, C_s . All real amplifiers will also have some finite resistance, R_b , and input capacitance. A small amount of positive feedback **322** may be applied through C_2 **324**, as adjusted using R_3 **326**, to neutralize the effect of the input capacitance for better channel matching and common-mode rejection ratio (CMRR).

[0033] Important noise sources may include the input-referred voltage noise of the amplifier, V_{na} , the input current noise, I_{na} and the additional current noise, I_{nb} , due to the leakage and conductance of the biasing element. The current noise contribution may be either $4kTR$ thermal noise for a resistive device or $2qI$ shot noise for a PN junction. Bootstrapping may be used to electronically boost the effective impedance of the biasing element, but the noise contribution may depend only on the physical resistance or leakage current, illustrating the challenge in finding suitable components for a non-contact sensor. The total input referred noise of a capacitive amplifier may be written as,

$$v_n^2 = v_{na}^2 \left(1 + \frac{C_m + C_n}{C_s} \right)^2 + \frac{i_{na}^2 + i_{nb}^2}{\omega^2 C_s^2}.$$

[0034] This equation shows the effect of the parasitic input capacitances and leakage currents on the noise performance of the amplifier and the difficulty in designing a non-contact electrode. Any excess input capacitance may directly multiply the effect of the amplifier's input voltage noise as $C_m + C_n > C_s$. Furthermore, since biopotential signals are at low frequencies (0.1-100 Hz), even small amounts of current noise may become integrated into large amounts of input

voltage noise. This necessitates an amplifier with very low input and guard capacitance, as well as almost zero leakage currents.

[0035] The INA116, originally by Burr-Brown, now produced by Texas Instruments, is an example of an amplifier that is well known for ultra-high input impedance applications by virtue of its extremely low current noise (0.1 fA/Hz). However, any other comparable amplifier may be used for this application. Any circuit introduced to bias the inputs may significantly degrade the noise performance of the amplifier. An extremely difficult to obtain resistor (greater than 1 TΩ) would be required to match the current noise specification of the INA116. The INA116 may reliably charge a floating input to a point inside the allowable input range shortly after power-up, purely through leakage currents, removing the need for any external bias network. To remove drift and DC offsets, a low-passed version of the input signal was taken from the non-inverting input's guard and connected to the inverting input. This effectively performs AC coupling without degrading the input impedance and centers the output to mid-rail for maximum signal swing. The overall gain of the first stage INA116 may be written as

$$A_v = \left(1 + \frac{50k\Omega}{R_1} \right) \times \frac{sR_2C_1}{1 + sR_2C_1}.$$

[0036] For this exemplary application the cut-off frequency may be set at 0.7 Hz and the amplifier may be configured with a gain of 2.02. This relatively low gain value was dictated by the limited voltage headroom of the INA116, which was operated with only a 5V power supply, not the datasheet recommended 10V.

[0037] Electrocardiography (EKG or ECG) is the process of recording the electrical activity of the heart over a period of time using electrodes placed on a patient's body. These electrodes detect the tiny electrical changes on the skin that arise from the heart muscle depolarizing during each heart-beat.

[0038] In a conventional 12 lead EKG, ten electrodes are placed on the patient's limbs and on the surface of the chest. The overall magnitude of the heart's electrical potential is then measured from twelve different angles ("leads") and is recorded over a period of time (usually 10 seconds). In this way, the overall magnitude and direction of the heart's electrical depolarization is captured at each moment throughout the cardiac cycle. The graph of voltage versus time produced by this non-invasive medical procedure is referred to as an electrocardiogram.

[0039] In an embodiment, an electronic stethoscope may be enabled with this 12 lead EKG diagnostic capability, which may provide the most precise output existing in clinical use. An EKG acquisition comes from a set of electrodes applied to a patient's body, or with non-contact electrodes, on some fabric or clothing. The locations of the electrodes on a patient are as follows:

Electrode Name Electrode Placement

- [0040]** RA On the right arm, avoiding thick muscle.
- [0041]** LA In the same location where RA was placed, but on the left arm.
- [0042]** RL On the right leg, lateral calf muscle.

[0043] LL In the same location where RL was placed, but on the left leg.

[0044] V₁ In the fourth intercostal space (between ribs 4 and 5) just to the right of the sternum (breastbone).

[0045] V₂ In the fourth intercostal space (between ribs 4 and 5) just to the left of the sternum.

[0046] V₃ Between leads V₂ and V₄.

[0047] V₄ In the fifth intercostal space (between ribs 5 and 6) in the mid-clavicular line.

[0048] V₅ Horizontally even with V₄, in the left anterior axillary line.

[0049] V₆ Horizontally even with V₄ and V₅ in the midaxillary line.

[0050] The signals obtained from each of these electrodes may then be combined in 12 different ways to build the EKG's 12 leads. These 12 leads are divided between the Limb Leads, Augmented Limb Leads, and Precordial Leads. First is the definition of the Wilson's central terminal, which is commonly used in the definition of many of the leads.

$$V_w = 1/3(RA+LA+LL)$$

[0051] The voltage differences making up the Limb Leads and Augmented Limb Leads are shown in FIG. 4. Leads I, II and III are called the Limb Leads. The electrodes that form these signals are located on the limbs—one on each arm and one on the left leg.

[0052] Lead I 402 is the voltage between the (positive) left arm (LA) electrode and right arm (RA) electrode:

$$I=LA-RA$$

[0053] Lead II 404 is the voltage between the (positive) left leg (LL) electrode and the right arm (RA) electrode:

$$II=LL-RA$$

[0054] Lead III 406 is the voltage between the (positive) left leg (LL) electrode and the left arm (LA) electrode:

$$III=LL-LA$$

[0055] Leads aVR, aVL, and aVF are the Augmented Limb Leads. They are derived from the same three electrodes as leads I, II, and III, but they use Wilson's central terminal as their negative pole.

[0056] Lead augmented Vector Right (aVR) 408 has the positive electrode on the right arm. The negative pole is a combination of the left arm electrode and the left leg electrode:

$$aVR=RA-1/2(LA+LL)=3/2(RA-V_w)$$

[0057] Lead augmented Vector Left (aVL) 410 has the positive electrode on the left arm. The negative pole is a combination of the right arm electrode and the left leg electrode:

$$aVL=LA-1/2(RA+LL)=3/2(LA-V_w)$$

[0058] Lead augmented Vector Foot (aVF) 412 has the positive electrode on the left leg. The negative pole is a combination of the right arm electrode and the left arm electrode:

$$aVF=LL-1/2(RA+LA)=3/2(LL-V_w)$$

[0059] Together with leads I, II, and III, Augmented Limb Leads aVR, aVL, and aVF form the basis of the hexaxial reference system, which is used to calculate the heart's electrical axis in the frontal plane.

[0060] The precordial leads lie in the transverse (horizontal) plane, perpendicular to the other six leads. The six

precordial electrodes act as the positive poles for the six corresponding precordial leads: (V1, V2, V3, V4, V5 and V6). Exemplary signals detected on each of the leads are shown in FIG. 5. For example, a lead I signal 502, a lead II signal 504, a lead III signal 506, a lead aVR signal 508, a lead aVL signal 510, a lead aVF signal 512, a lead V1 signal 514, a lead V2 signal 516, a lead V3 signal 518, a lead V4 signal 520, a lead V5 signal 522, and a lead V6 signal 524 are shown.

[0061] Wilson's central terminal is used as the negative pole.

[0062] In an embodiment, a networked electronic stethoscope may include two main functionalities. The first functionality may include enhanced stethoscope acquisition capabilities, and the second functionality may include linking the electronic stethoscope to a network of wireless sensors.

[0063] An example of an embodiment of a networked electronic stethoscope 600 is shown in FIG. 6. In this example, a networked electronic stethoscope may include a device 602 with a built-in electrode, a dedicated wireless network, such as Bluetooth, communication device 604, and a power supply 606. The device may be attached to a membrane support circle 604 of the electronic stethoscope 600. The device may be removable to allow a practitioner perform standard stethoscope assessment.

[0064] Equipped with this electrode setup, the stethoscope would enable the practitioner to easily measure cardiac related electrical signals from anywhere on the patient's body. The device may provide the capability to acquire physiological data related to all of the precordial leads. Indeed, these leads being located on the patient's torso, measuring them with a stethoscope-like device makes complete sense, as both the practitioner and the patient are used to such an examination type.

[0065] However, as corresponding data from limb leads must be acquired, additional electrodes 606 for limb lead signal acquisition may be needed.

[0066] In an embodiment a wire 608 may connect every sensor to a ground location as well as a wireless transmitter and an alimentation. However, this embodiment may cause discomfort to both the patient and the practitioner during the acquisition process.

[0067] In an embodiment, the electrodes 606 may be implemented as a tissue fabric armband and/or anklet with built-in wireless (for example, Bluetooth) electrodes, driven by the stethoscope's controller. The electrode sensor technology may perform without any substantial lack of signal quality even when separated from the skin by layers of fabric. This would simplify the process of putting the electrodes on the patient. In addition, the discomfort caused by the electrodes/wire system would be reduced, allowing the patient to improved mobility.

[0068] In an embodiment, the system may include two or more armband electrodes 610 and two or more anklet electrodes 612, driven by the stethoscope wireless network controller, that would stream continuously data from each of the limb leads and augmented limb leads to a computing device, such as a personal computer or smartphone, precordial leads signal acquisition is being performed with the stethoscope's built in electrode.

[0069] With the combination of both the armband/anklet sensors and the electrode-enabled stethoscope, embodiments are capable of acquiring digitized 12 lead EKG data.

An exemplary process **700** for acquiring such data is shown in FIG. 7. In the example shown in FIG. 7, data may be acquired continuously for the limb leads and augmented limb leads, while data may be acquired for only one or more precordial leads at a time. This may lead to a lack of synchronicity among the recorded precordial lead signals.

[0070] Process **700** begins with **702** the signal acquisition is begun utilizing the networked electronic stethoscope and the network thereof, such as a wireless network, such as Bluetooth. At **704**, data acquisition is performed using the limb leads and augmented limb leads by attaching the armlet and ankle on the patient's limbs and beginning continuous data acquisition using those leads. At **706**, a precordial lead electrode, for example, the electrode attached to the networked electronic stethoscope, is placed at a precordial site. At **708**, data is acquired from the precordial site, as well as from the limb leads and augmented limb leads. Data may be acquired for a specific period, such as ten seconds. At **710**, the process loops back to **706**, where the precordial lead electrode, such as the electrode attached to the networked electronic stethoscope, is placed at another precordial site and the data acquisition is repeated for that precordial site. **706** and **708** may be repeated until data has been acquired for all precordial sites. At **712**, the acquired data is stored and processed.

[0071] In this example, the physiological signals needed for a 12 lead EKG acquisition are acquired and processed. The results may be displayed on a computing device, such as a personal computer, smartphone, tablet, etc., and may be stored online for cloud-based applications, such as those described below.

[0072] An exemplary embodiment of a wireless sensor electrode device **800** is shown in FIG. 8. Device **800** may include a micro-controller **802**, a wireless network adapter **804**, an electrode **806**, and a power source **808**. In this embodiment, each electrode device **800** may be autonomous. Each electrode device **800** may be attached to a tissue fabric armlet or ankle with built-in sensors, for placement on a patient. Micro-controller **802** may be, for example, a single-chip micro-controller, or an embedded processor in an FPGA or ASIC device. Wireless network adapter **804** may implement a standard wireless network protocol, such as Bluetooth, or it may implement a proprietary or custom wireless network protocol, or any other wireless network or communication protocol, and may be implemented as a separate device from the micro-controller device, or may be implemented in the same device, such as an FPGA or ASIC device, as the micro-controller device. Power source **808** may typically include a rechargeable or non-rechargeable battery and may further include power conditioning circuitry and battery charging circuitry. Such circuitry may be implemented as a separate device from the micro-controller and/or wireless network device, or may be implemented in the same device, such as an FPGA or ASIC device, as the micro-controller device and/or wireless network device.

[0073] Although conventional EKG systems typically utilize a wired ground electrode to provide a point of potential difference for signal measurement, embodiments may not require such a wired ground electrode. For example, as it is used to define potentials within an electrical circuit, EKG electrodes already measure potentials, which include the data needed to assess the patient physiological signals. Accordingly, in an embodiment, the desired EKG signals may be synthesized without any actual ground connection,

using mathematical processing to build the EKG from the signals that are obtained from the electrodes. In an embodiment, as the signal from the electrodes is immediately digitized within the built-in electronic circuit, a ground connection may be stimulating by utilizing a digitized, transmitted equivalent of a ground signal. Such a signal may be used to directly rebuild EKG signals.

[0074] In an embodiment, the device may acquire four signals, from two armlets and two anklets, all driven by wireless network of the stethoscope. The device may then record and stream the data directly to the practitioner's smartphone, tablet or computer. As an example, three sensors, such as the left armlet, right armlet, and left ankle, may be used as sensors for data acquisition, whereas the remaining sensor, such as the right ankle, may be used as the artificial ground connection. Once all of those sensors are attached, the global acquisition process may be performed by a practitioner.

[0075] In an embodiment, the electrodes may be incorporated in armlets/anklets in a similar way, but utilizing a wire to connect each of them. Only one of the electrodes, such as the right leg ankle, may include the wireless network adapter and power unit, as well as a traditional ground reference. This embodiment may require the electrode of the stethoscope to be linked to the wire, which may limit the freedom of movement of both the practitioner and patient. In such an embodiment, the wire may be designed to provide improved comfort for each user.

[0076] In an embodiment, the storage of digitized biometric data may be provided on a number of devices, such as a smartphone, tablet or laptop, in addition to storage (and analysis) in the cloud or local server. This pooling of synchronous, multimodal data may create an opportunity for medical professionals to collaborate with one another and leverage Big Data computing, opening the door to additional innovative applications.

[0077] For example, in an embodiment, preliminary data processing capabilities may be provided on the devices and back-end analytic technology may be provided in the cloud or local server.

[0078] For example, in an embodiment, a software application for a computing device, such as a smartphone, tablet, computer, etc., may provide the capability for wireless stethoscope interfacing, collecting signals from a set of sensors, preliminary data processing, analyzing, and uploading on to the cloud or local server based platform. This application may provide a practitioner's window into the digitized physiological profile of his patient. An example of an EKG display **900** provided by such an application is shown in FIG. 9.

[0079] It is to be noted that the application is applicable not only to EKG display interfacing, but is also applicable to a variety of sensor devices capable of assessing diverse physiological signals from the patient. As such, the application may provide the capability to easily integrate new parts as new sensors are created. The application may provide an interface that is familiar and easy to use for the practitioner. The application may provide the capability to display many of the classical tools previously used by the practitioner. The application may provide the capability to perform advanced data processing both locally and in collaboration with the cloud platform or local server. The application may be responsive and efficient with computation time, whether it is for graph displaying, data crunching

or dialog with the cloud platform or local server. The application may provide a first step to digitally assisted medicine and may connect to a massive, state of the art backend data analytics platform in the cloud.

[0080] In an embodiment, a communication platform may provide the capability for various practitioners around the world to share and contribute to medical knowledge. An example of such a communication platform **1000** is shown in FIG. 10. Every practitioner has acquired through years of personal practice a specific, personal insight regarding medicine and diagnosis. As this experience makes a better doctor, it also engenders specialization and so one practitioner might lack efficiency when facing a patient that quite doesn't fit their mental map of diseases and diagnosis. Even though that specific doctor might be at a loss in a specific case, another with a different set of experience might be right in their comfort zone, and completely able to diagnose quickly, surely and securely. Such a communication platform may provide the capability to map a practitioner to a specific condition, with pooled former patient, treatment and outcome data. The communication platform may provide the capability to quantify patient data sufficiently to enable comparisons to be made. Indeed, with precise physiological data extracted from every patient, patterns may be found in both clinical data and clinicians themselves. Through ongoing analysis a doctors profiles may be defined from their past experiences, diagnoses and outcomes, thus allowing connection of two practitioners when needed.

[0081] In an embodiment, a number of processes may be performed by communication platform **1000**, shown in FIG. 10. For example, communication platform **1000** may perform patient oriented processes, such as a practitioner performing a number of different examinations, all of which can be captured and uploaded by several means, such as text, binary item for simpler criteria, pictures or data obtained from hardware dedicated to acquire digitized physiological signals (such as our device). When the practitioner has enough information from the digitized data presented on the device, combined with his past experience to diagnose the patient. The practitioner may choose to get a second opinion from another doctor connected to the database. The platform chooses the best fit for the case the practitioner is dealing with. If both doctors accept the platform's proposal, the patient's data is shared to the second practitioner, who can share his insight to the first doctor.

[0082] Such a communications platform may provide several advantages and functions, as shown in FIG. 11. First, it would give practitioners a tool with which they can transparently share their insights with the world, making every member doctor a member of a massive community-based diagnosis meta organism. In an embodiment, that machine learning could be applied to analyze these interactions to allow this "meta organism" to learn with each new patient treated. In the short term, expert assistance will allow practitioners to offer better diagnoses and over the longer term will capture these lessons learned to empower practitioners to learn from each other's experience. Secondly, although Big Data medical applications and decision support systems are generally intimidating to medical staff, this application is relatively non-invasive, meaning that all data and diagnosis-related decision remains in the hands of a human being that has demonstrated their ability in making such decisions. The transparent, non-invasive method of data collection and sharing presented by embodiments of

this system is likely the best way to introduce the medical world to this Big Data revolution that is transforming so many other industries. Finally, this application is, from an algorithmic point of view, relatively easy to implement:

[0083] Each practitioner uses the hardware solution which uploads the patient's data online.

[0084] Using machine learning, clustering algorithms may classify patients by their similarities between their respective physiological signals.

[0085] Practitioners may be classified from the types of patients they are most used to treating may be developed.

[0086] Practitioners with similar cases may get in touch with each other. For example, one practitioner might be specialized in one particular disease. While a naive approach may put every doctor confronted to such a disease in touch with said specialist (which would be overwhelming), a more sophisticated approach may utilize a network of information transmission and passive feedback to provide improved functionality.

[0087] Embodiments may provide practitioners a first glimpse of what Big Data assisted medicine could be, allowing them to get used to the implementation of data science tools in the diagnosis process.

[0088] Embodiments may provide is a massive tool allowing the implementation of automated diagnosis of several diseases from biomarker detection. Given the large amount of data collected by the system, the cloud platform has the potential to become one of the most massive sets of physiological signal data tied to case studies, treatments, outcomes and other medical related items. Indeed, each time a patient gets an examination, their data may be uploaded and (with patient consent) may contribute to the enrichment of the overall platform (in an anonymized, HIPAA-compliant way). This data may be accessible by any member of the community of practitioners contributing to the platform. As a consequence, each doctor may help to create a massive (as well as highly diverse) dataset that can provide one with information regarding a whole set of different diseases.

[0089] Such a dataset, in combination with powerful, specialized tools, such as the latest data analysis techniques, may provide any medical researcher with a significant insight. Over the longer term, such a system in combination with expert learning systems may allow the implementation of automated diagnosis algorithms.

[0090] An exemplary block diagram of a computing device **1200**, in which processes involved in the embodiments described herein may be implemented, such as those processes performed by an electronic stethoscope base unit **102**, a sensor **108**, **110**, or a computing device **106**, as shown in FIG. 1, is shown in FIG. 12. Computing device **1200** is typically a programmed general-purpose computer system, such as an embedded processor, system on a chip, personal computer, workstation, server system, and minicomputer or mainframe computer. Likewise, computing device **1200** may be implemented in a wrist-worn, or other personal or mobile device, and may include sensor circuitry as well as display circuitry to display object identification information. Computing device **1200** may include one or more processors (CPUs) **1202A-1202N**, input/output circuitry **1204**, network adapter **1206**, and memory **1208**. CPUs **1202A-1202N** execute program instructions in order to carry out the functions of the present invention. Typically, CPUs **1202A-1202N** are one or more microprocessors, such as an INTEL PENTIUM® processor. FIG. 12 illustrates an embodiment

in which computing device **1200** is implemented as a single multi-processor computer system, in which multiple processors **1202A-1202N** share system resources, such as memory **1208**, input/output circuitry **1204**, and network adapter **1206**. However, the present invention also contemplates embodiments in which computing device **1200** is implemented as a plurality of networked computer systems, which may be single-processor computer systems, multi-processor computer systems, or a mix thereof.

[0091] Input/output circuitry **1204** provides the capability to input data to, or output data from, computing device **1200**. For example, input/output circuitry may include input devices, such as keyboards, mice, touchpads, trackballs, scanners, analog to digital converters, etc., output devices, such as video adapters, monitors, printers, etc., and input/output devices, such as, modems, etc. Network adapter **1206** interfaces device **1200** with a network **1210**. Network **1210** may be any public or proprietary LAN or WAN, including, but not limited to the Internet.

[0092] Memory **1208** stores program instructions that are executed by, and data that are used and processed by, CPU **1202** to perform the functions of computing device **1200**. Memory **1208** may include, for example, electronic memory devices, such as random-access memory (RAM), read-only memory (ROM), programmable read-only memory (PROM), electrically erasable programmable read-only memory (EEPROM), flash memory, etc., and electro-mechanical memory, such as magnetic disk drives, tape drives, optical disk drives, etc., which may use an integrated drive electronics (IDE) interface, or a variation or enhancement thereof, such as enhanced IDE (EIDE) or ultra-direct memory access (UDMA), or a small computer system interface (SCSI) based interface, or a variation or enhancement thereof, such as fast-SCSI, wide-SCSI, fast and wide-SCSI, etc., or Serial Advanced Technology Attachment (SATA), or a variation or enhancement thereof, or a fiber channel-arbitrated loop (FC-AL) interface.

[0093] The contents of memory **1208** may vary depending upon the function that computing device **1200** is programmed to perform. In the example shown in FIG. **12**, exemplary memory contents are shown representing routines and data for embodiments of the processes described above, such as those processes performed by an electronic stethoscope base unit **102**, a sensor **108**, **110**, or a computing device **106** of FIG. **1**. However, one of skill in the art would recognize that these routines, along with the memory contents related to those routines, may not be included on one system or device, but rather may be distributed among a plurality of systems or devices, based on well-known engineering considerations. The present invention contemplates any and all such arrangements.

[0094] In the example shown in FIG. **12**, memory **1208** may include electronic stethoscope base unit routines **1212**, sensor routines **1214**, computing device routines **1216**, patient data **1218**, and operating system **1220**. For example, electronic stethoscope base unit routines **1212** may include routines that operate electronic stethoscope base unit **102** and interact with a sensor **108**, **110**, or a computing device. Sensor routines **1214** may include routines to capture data with sensors **108**, **110** and interact with electronic stethoscope base unit **102**. Computing device routines **1216** may include routines to interact with electronic stethoscope base

unit **102** and to analyze patient data **1218** received therefrom. Operating system **1220** provides overall system functionality.

[0095] As shown in FIG. **12**, the present invention contemplates implementation on a system or systems that provide multi-processor, multi-tasking, multi-process, and/or multi-thread computing, as well as implementation on systems that provide only single processor, single thread computing. Multi-processor computing involves performing computing using more than one processor. Multi-tasking computing involves performing computing using more than one operating system task. A task is an operating system concept that refers to the combination of a program being executed and bookkeeping information used by the operating system. Whenever a program is executed, the operating system creates a new task for it. The task is like an envelope for the program in that it identifies the program with a task number and attaches other bookkeeping information to it. Many operating systems, including Linux, UNIX®, OS/2®, and Windows®, are capable of running many tasks at the same time and are called multitasking operating systems. Multi-tasking is the ability of an operating system to execute more than one executable at the same time. Each executable is running in its own address space, meaning that the executables have no way to share any of their memory. This has advantages, because it is impossible for any program to damage the execution of any of the other programs running on the system. However, the programs have no way to exchange any information except through the operating system (or by reading files stored on the file system). Multi-process computing is similar to multi-tasking computing, as the terms task and process are often used interchangeably, although some operating systems make a distinction between the two.

[0096] The present invention may be a system, a method, and/or a computer program product at any possible technical detail level of integration. The computer program product may include a computer readable storage medium (or media) having computer readable program instructions thereon for causing a processor to carry out aspects of the present invention. The computer readable storage medium can be a tangible device that can retain and store instructions for use by an instruction execution device.

[0097] The computer readable storage medium may be, for example, but is not limited to, an electronic storage device, a magnetic storage device, an optical storage device, an electromagnetic storage device, a semiconductor storage device, or any suitable combination of the foregoing. A non-exhaustive list of more specific examples of the computer readable storage medium includes the following: a portable computer diskette, a hard disk, a random access memory (RAM), a read-only memory (ROM), an erasable programmable read-only memory (EPROM or Flash memory), a static random access memory (SRAM), a portable compact disc read-only memory (CD-ROM), a digital versatile disk (DVD), a memory stick, a floppy disk, a mechanically encoded device such as punch-cards or raised structures in a groove having instructions recorded thereon, and any suitable combination of the foregoing. A computer readable storage medium, as used herein, is not to be construed as being transitory signals per se, such as radio waves or other freely propagating electromagnetic waves, electromagnetic waves propagating through a waveguide or

other transmission media (e.g., light pulses passing through a fiber-optic cable), or electrical signals transmitted through a wire.

[0098] Computer readable program instructions described herein can be downloaded to respective computing/processing devices from a computer readable storage medium or to an external computer or external storage device via a network, for example, the Internet, a local area network, a wide area network and/or a wireless network. The network may comprise copper transmission cables, optical transmission fibers, wireless transmission, routers, firewalls, switches, gateway computers, and/or edge servers. A network adapter card or network interface in each computing/processing device receives computer readable program instructions from the network and forwards the computer readable program instructions for storage in a computer readable storage medium within the respective computing/processing device.

[0099] Computer readable program instructions for carrying out operations of the present invention may be assembler instructions, instruction-set-architecture (ISA) instructions, machine instructions, machine dependent instructions, microcode, firmware instructions, state-setting data, configuration data for integrated circuitry, or either source code or object code written in any combination of one or more programming languages, including an object oriented programming language such as Smalltalk, C++, or the like, and procedural programming languages, such as the “C” programming language or similar programming languages. The computer readable program instructions may execute entirely on the user's computer, partly on the user's computer, as a stand-alone software package, partly on the user's computer and partly on a remote computer or entirely on the remote computer or server. In the latter scenario, the remote computer may be connected to the user's computer through any type of network, including a local area network (LAN) or a wide area network (WAN), or the connection may be made to an external computer (for example, through the Internet using an Internet Service Provider). In some embodiments, electronic circuitry including, for example, programmable logic circuitry, field-programmable gate arrays (FPGA), or programmable logic arrays (PLA) may execute the computer readable program instructions by utilizing state information of the computer readable program instructions to personalize the electronic circuitry, in order to perform aspects of the present invention.

[0100] Aspects of the present invention are described herein with reference to flowchart illustrations and/or block diagrams of methods, apparatus (systems), and computer program products according to embodiments of the invention. It will be understood that each block of the flowchart illustrations and/or block diagrams, and combinations of blocks in the flowchart illustrations and/or block diagrams, can be implemented by computer readable program instructions.

[0101] These computer readable program instructions may be provided to a processor of a general purpose computer, special purpose computer, or other programmable data processing apparatus to produce a machine, such that the instructions, which execute via the processor of the computer or other programmable data processing apparatus, create means for implementing the functions/acts specified in the flowchart and/or block diagram block or blocks. These computer readable program instructions may also be stored

in a computer readable storage medium that can direct a computer, a programmable data processing apparatus, and/or other devices to function in a particular manner, such that the computer readable storage medium having instructions stored therein comprises an article of manufacture including instructions which implement aspects of the function/act specified in the flowchart and/or block diagram block or blocks.

[0102] The computer readable program instructions may also be loaded onto a computer, other programmable data processing apparatus, or other device to cause a series of operational steps to be performed on the computer, other programmable apparatus or other device to produce a computer implemented process, such that the instructions which execute on the computer, other programmable apparatus, or other device implement the functions/acts specified in the flowchart and/or block diagram block or blocks.

[0103] The flowchart and block diagrams in the Figures illustrate the architecture, functionality, and operation of possible implementations of systems, methods, and computer program products according to various embodiments of the present invention. In this regard, each block in the flowchart or block diagrams may represent a module, segment, or portion of instructions, which comprises one or more executable instructions for implementing the specified logical function(s). In some alternative implementations, the functions noted in the blocks may occur out of the order noted in the Figures. For example, two blocks shown in succession may, in fact, be executed substantially concurrently, or the blocks may sometimes be executed in the reverse order, depending upon the functionality involved. It will also be noted that each block of the block diagrams and/or flowchart illustration, and combinations of blocks in the block diagrams and/or flowchart illustration, can be implemented by special purpose hardware-based systems that perform the specified functions or acts or carry out combinations of special purpose hardware and computer instructions.

[0104] Although specific embodiments of the present invention have been described, it will be understood by those of skill in the art that there are other embodiments that are equivalent to the described embodiments. Accordingly, it is to be understood that the invention is not to be limited by the specific illustrated embodiments, but only by the scope of the appended claims.

What is claimed is:

1. A system comprising:
 - a networked electronic stethoscope; and
 - a sensor adapted to be attached to the networked electronic stethoscope, the sensor comprising:
 - an electrode adapted to obtain a signal representing a physiological parameter of a patient,
 - a processor adapted to digitize and process the obtained signal to form data, and
 - a wireless network adapter adapted to transmit the data to the networked electronic stethoscope.
2. The system of claim 1, wherein the electrode is a non-contact electrode adapted to obtain a signal representing a physiological parameter of the patient without direct contact with the patient.
3. The system of claim 2, further comprising:
 - at least one additional sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of the patient.

4. The system of claim 3, wherein the at least one additional sensor is communicatively connected to the sensor adapted to be attached to the networked electronic stethoscope.

5. The system of claim 4, wherein the at least one additional sensor is communicatively connected to the sensor adapted to be attached to the networked electronic stethoscope via at least one wire.

6. The system of claim 4, wherein the at least one additional sensor is communicatively connected to the sensor adapted to be attached to the networked electronic stethoscope via a wireless communication network.

7. The system of claim 1, wherein the sensor is adapted to be attached to a membrane support circle the networked electronic stethoscope.

8. The system of claim 7, further comprising:

at least one additional sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of the patient.

9. The system of claim 8, wherein the processor is adapted to generate a representation of the physiological parameter of the patient based on at least the signal representing the physiological parameter of a patient obtained from the sensor adapted to be attached to the networked electronic stethoscope and the signal representing the physiological parameter of a patient obtained from the at least one additional sensor.

10. The system of claim 8, wherein the processor is adapted to generate a plurality of representations of the physiological parameter of the patient based on at least a plurality of signals representing the physiological parameter of a patient obtained from the sensor adapted to be attached to the networked electronic stethoscope, placed at each of a plurality of locations on the patient, and the signal representing a physiological parameter of a patient obtained from the at least one additional sensor.

11. The system of claim 2, wherein the signal representing the physiological parameter of the patient is an electrocardiogram (EKG) signal.

12. A method comprising:

placing at a location on a patient at least one sensor comprising an electrode adapted to obtain a signal representing a physiological parameter of the patient; repeatedly placing at a different location on the patient a sensor attached to a networked electronic stethoscope, the networked electronic stethoscope comprising an electrode adapted to obtain a signal representing a physiological parameter of a patient, a processor adapted to digitize and process the obtained signal to form data, and a wireless network adapter adapted to transmit the data to the networked electronic stethoscope; and

for each different location on the patient at which the sensor is placed, obtaining the signal representing the physiological parameter of the patient.

13. The system of claim 12, wherein the electrodes are non-contact electrodes adapted to obtain a signal representing a physiological parameter of the patient without direct contact with the patient.

14. The system of claim 13, wherein the at least one sensor is communicatively connected to the sensor attached to the networked electronic stethoscope.

15. The system of claim 14, wherein the at least one sensor is communicatively connected to the sensor attached to the networked electronic stethoscope via at least one wire.

16. The system of claim 14, wherein the at least one sensor is communicatively connected to the sensor attached to the networked electronic stethoscope via a wireless communication network.

17. The system of claim 12, wherein the signal representing the physiological parameter of the patient is an electrocardiogram (EKG) signal.

* * * * *

专利名称(译)	网络电子听诊器		
公开(公告)号	US20170231597A1	公开(公告)日	2017-08-17
申请号	US15/431221	申请日	2017-02-13
[标]申请(专利权)人(译)	霍华德NEWTON		
申请(专利权)人(译)	霍华德，牛顿		
当前申请(专利权)人(译)	霍华德，牛顿		
[标]发明人	HOWARD NEWTON		
发明人	HOWARD, NEWTON		
IPC分类号	A61B7/04 A61B5/0408 A61B5/00		
CPC分类号	A61B7/04 A61B5/04085 A61B5/0022 A61B5/0024 A61B5/0404 A61B5/0408 G16H40/67		
优先权	62/294421 2016-02-12 US		
外部链接	Espacenet USPTO		

摘要(译)

本系统和方法的实施例可以提供改进的电子听诊器，其提供多样化的诊断功能。例如，实施例可以通过使用设备的无线网络容量将其链接到不同类型的可穿戴传感器来提供诊断各种病症的能力，保持听诊器的传统使用同时使其能够感测全新的生理学集合。信号。例如，在一个实施例中，系统可以包括联网的电子听诊器和适于连接到联网的电子听诊器的传感器，该传感器包括适于获得表示患者的生理参数的信号的电极，适于数字化和处理获得的信号以形成数据，以及适于将数据发送到联网的电子听诊器的无线网络适配器。

