



US010034637B2

(12) **United States Patent**
Harlev et al.

(10) **Patent No.:** **US 10,034,637 B2**
(45) **Date of Patent:** ***Jul. 31, 2018**

(54) **CARDIAC MAPPING CATHETER**

(71) Applicant: **Rhythmia Medical, Inc.**, Burlington,
MA (US)

(72) Inventors: **Doron Harlev**, Brookline, MA (US);
Justin Callaway, Goffstown, NH (US)

(73) Assignee: **Boston Scientific Scimed, Inc.**, Maple
Grove, MN (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 1003 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **14/277,122**

(22) Filed: **May 14, 2014**

(65) **Prior Publication Data**

US 2014/0275921 A1 Sep. 18, 2014

Related U.S. Application Data

(63) Continuation of application No. 13/868,151, filed on
Apr. 23, 2013, now Pat. No. 8,755,861, which is a
continuation of application No. 13/289,367, filed on
Nov. 4, 2011, now Pat. No. 8,447,377, which is a
(Continued)

(51) **Int. Cl.**

A61B 5/0402 (2006.01)
A61B 5/00 (2006.01)
A61B 5/042 (2006.01)
A61M 25/00 (2006.01)
A61M 25/01 (2006.01)
A61B 18/00 (2006.01)
A61B 18/14 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/6852** (2013.01); **A61B 5/042**
(2013.01); **A61B 5/0422** (2013.01); **A61B**
5/6859 (2013.01); **A61M 25/0015** (2013.01);

A61M 25/0147 (2013.01); **A61B 18/1492**
(2013.01); **A61B 2018/00214** (2013.01); **A61B**
2018/00351 (2013.01); **A61B 2018/00839**
(2013.01); **A61B 2018/00898** (2013.01); **A61M**
2025/0161 (2013.01); **Y10T 29/49117**
(2015.01)

(58) **Field of Classification Search**

CPC **A61B 5/0422**; **A61B 5/042**; **A61B 5/6852**;
A61B 5/6859; **A61B 18/1492**; **A61B**
2018/00214; **A61B 2018/00839**; **A61B**
2018/00351

USPC **600/372**, **373**, **374**, **381**, **509**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,649,924 A 3/1987 Taccardi
4,674,518 A 6/1987 Salo
4,840,182 A 6/1989 Carlson
(Continued)

FOREIGN PATENT DOCUMENTS

CA 2719329 A1 10/2009
EP 0779059 B1 6/1997
(Continued)

OTHER PUBLICATIONS

Written Opinion of International Searching Authority issued in
PCT/US2009/061277, dated Apr. 8, 2010, 10 pages.
(Continued)

Primary Examiner — Lee S Cohen


Assistant Examiner — Erin M Cardinal

(74) Attorney, Agent, or Firm — Faegre Baker Daniels
LLP

(57) **ABSTRACT**

A multi electrode catheter for non contact mapping of the
heart having independent articulation and deployment fea-
tures.

16 Claims, 15 Drawing Sheets

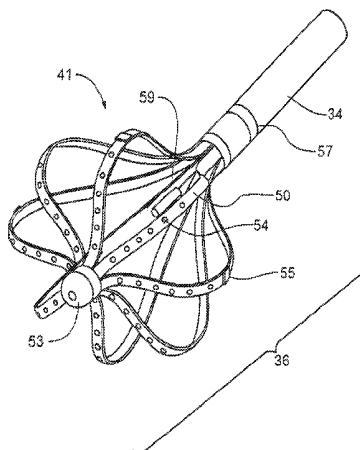

Related U.S. Application Data

continuation of application No. 12/005,975, filed on
Dec. 28, 2007, now Pat. No. 8,103,327.

(56)

References Cited

U.S. PATENT DOCUMENTS

4,890,623 A	1/1990	Cook et al.	6,314,310 B1	11/2001	Ben-Haim et al.
4,920,490 A	4/1990	Isaacson	6,317,619 B1	11/2001	Boernert et al.
4,940,064 A	7/1990	Desai et al.	6,318,375 B1	11/2001	Plicchi et al.
5,156,151 A	10/1992	Imran	6,360,123 B1	3/2002	Kimchi et al.
5,228,442 A	7/1993	Imran	6,368,285 B1	4/2002	Osadchy et al.
5,255,679 A	10/1993	Imran	6,400,981 B1	6/2002	Govari
5,279,299 A	1/1994	Imran	6,516,807 B1	2/2003	Panescu et al.
5,284,142 A	2/1994	Goble et al.	6,547,082 B1	4/2003	Babini
5,297,549 A	3/1994	Beatty et al.	6,556,695 B1	4/2003	Packer et al.
5,300,068 A	4/1994	Rosar et al.	6,574,492 B1	6/2003	Ben-Haim et al.
5,309,910 A	5/1994	Edwards et al.	6,574,498 B1	6/2003	Gilboa
5,311,866 A	5/1994	Kagan et al.	6,593,884 B1	7/2003	Gilboa et al.
5,313,943 A	5/1994	Houser et al.	6,600,948 B2	7/2003	Ben-Haim et al.
5,341,807 A	8/1994	Nardella	6,603,996 B1	8/2003	Beatty et al.
5,345,936 A	9/1994	Pomeranz et al.	6,631,290 B1	10/2003	Guck et al.
5,381,333 A	1/1995	Isaacson et al.	6,640,119 B1	10/2003	Budd et al.
5,415,166 A	5/1995	Imran	6,650,927 B1	11/2003	Keidar
5,425,364 A	6/1995	Imran	6,826,421 B1	1/2004	Beatty et al.
5,456,254 A	10/1995	Pietroski et al.	6,690,963 B2	2/2004	Ben-Haim et al.
5,469,858 A	11/1995	Osborne	6,701,176 B1	3/2004	Halperin et al.
5,417,982 A	12/1995	Modi	6,728,562 B1	4/2004	Budd et al.
5,480,422 A	1/1996	Ben-Haim	6,773,402 B2	8/2004	Govari et al.
5,490,859 A	2/1996	Mische et al.	6,807,439 B2	10/2004	Edwards et al.
5,499,981 A	3/1996	Kordis	6,837,886 B2	1/2005	Collins et al.
5,500,011 A	3/1996	Desai	6,839,588 B1	1/2005	Rudy
5,553,611 A	9/1996	Budd et al.	6,847,839 B2	1/2005	Ciaccio et al.
5,568,809 A	10/1996	Ben-Haim	6,872,428 B2	3/2005	Yang et al.
5,577,502 A	11/1996	Darrow et al.	6,892,090 B2	5/2005	Verard et al.
5,588,429 A	12/1996	Isaacson et al.	6,892,091 B1	5/2005	Ben-Haim et al.
5,634,469 A	6/1997	Bruder et al.	6,893,588 B2	5/2005	Lawson et al.
5,647,870 A	7/1997	Kordis et al.	6,939,309 B1	9/2005	Beatty et al.
5,662,108 A	9/1997	Budd et al.	6,957,101 B2	10/2005	Porath et al.
5,681,280 A	10/1997	Rusk et al.	6,978,168 B2	12/2005	Beatty et al.
5,681,308 A	10/1997	Edwards	6,990,370 B1	1/2006	Beatty et al.
5,687,737 A	11/1997	Branham et al.	7,016,719 B2	3/2006	Rudy et al.
5,697,377 A	12/1997	Wittkampf	7,043,292 B2	5/2006	Tarjan et al.
5,699,796 A	12/1997	Littman et al.	7,198,635 B2	4/2007	Danek et al.
5,702,438 A	12/1997	Avitall	7,263,397 B2	8/2007	Hauck et al.
5,704,365 A	1/1998	Albrecht et al.	7,505,810 B2	3/2009	Harlev et al.
5,722,402 A	3/1998	Swanson et al.	7,515,954 B2	4/2009	Harlev et al.
5,782,239 A	7/1998	Webster et al.	7,615,049 B2	11/2009	West et al.
5,840,025 A	11/1998	Ben-Haim	7,729,752 B2	6/2010	Harlev et al.
5,840,031 A	11/1998	Crowley	8,103,327 B2	1/2012	Harlev et al.
5,846,198 A	12/1998	Killmann	8,137,343 B2	3/2012	Harlev et al.
5,848,972 A	12/1998	Triedman et al.	8,224,416 B2	7/2012	de la Rama et al.
5,871,443 A	2/1999	Edwards et al.	8,364,235 B2	1/2013	Kordis et al.
5,893,847 A	4/1999	Kordis	8,447,377 B2	5/2013	Harlev et al.
5,896,847 A	4/1999	Usuki	8,463,368 B2	6/2013	Harlev et al.
5,911,739 A	6/1999	Kordis et al.	8,538,509 B2	9/2013	Harlev et al.
5,921,982 A	7/1999	Lesh et al.	8,725,240 B2	5/2014	Harlev et al.
5,928,228 A	7/1999	Kordis et al.	9,014,793 B2	4/2015	Harlev et al.
5,928,239 A	7/1999	Mirza	2002/0151807 A1	10/2002	Goldin
5,954,665 A	9/1999	Ben-Haim	2002/0177766 A1	11/2002	Mogul
5,971,933 A	10/1999	Gopakumaran et al.	2003/0018251 A1	1/2003	Solomon
5,983,126 A	11/1999	Wittkampf	2003/0065271 A1	4/2003	Khoury
5,986,126 A	11/1999	Bunel et al.	2003/0076277 A1	4/2003	Muramatsu et al.
6,014,581 A	1/2000	Wayne et al.	2003/0078509 A1	4/2003	Panescu
6,050,267 A	4/2000	Nardella et al.	2003/0216630 A1	11/2003	Jersey-Willuhn et al.
6,064,905 A	5/2000	Webster	2004/0077942 A1	4/2004	Hall et al.
6,095,150 A	8/2000	Panescu et al.	2004/0097806 A1	5/2004	Hunter et al.
6,163,716 A	12/2000	Edwards et al.	2004/0243015 A1	12/2004	Smith et al.
6,167,296 A	12/2000	Shahidi	2004/0254437 A1	12/2004	Hauck et al.
6,226,542 B1	5/2001	Reisfeld	2005/0033136 A1	2/2005	Govari et al.
6,236,886 B1	5/2001	Cherepenin et al.	2005/0033137 A1	2/2005	Oral et al.
6,240,307 B1	5/2001	Beatty et al.	2005/0038337 A1	2/2005	Edwards
6,246,898 B1	6/2001	Vesely et al.	2005/0054918 A1	3/2005	Sra
6,254,536 B1	7/2001	DeVito	2005/0107834 A1	5/2005	Freeman et al.
6,278,894 B1	8/2001	Salo et al.	2005/0154282 A1	7/2005	Li et al.
6,298,257 B1	10/2001	Hall et al.	2005/0288599 A1	12/2005	MacAdam et al.
6,308,093 B1	10/2001	Armoundas et al.	2006/0085049 A1	4/2006	Cory et al.
			2006/0116575 A1	6/2006	Willis
			2006/0122526 A1	6/2006	Berenfeld et al.
			2006/0173251 A1	8/2006	Govari et al.
			2006/0178587 A1	8/2006	Khoury
			2006/0241401 A1	10/2006	Govari et al.
			2007/0016007 A1	1/2007	Govari et al.
			2007/0038078 A1	2/2007	Osadchy
			2007/0049821 A1	3/2007	Willis
			2007/0083194 A1	4/2007	Kunis et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0112342	A1	5/2007	Pearson et al.
2007/0197929	A1	8/2007	Porath et al.
2007/0265539	A1	11/2007	Hastings et al.
2007/0270703	A1	11/2007	He et al.
2007/0287902	A1	12/2007	Fuimaono et al.
2007/0299351	A1	12/2007	Harlev et al.
2007/0299352	A1	12/2007	Harlev et al.
2007/0299353	A1	12/2007	Harlev et al.
2008/0140152	A1	6/2008	Imran et al.
2008/0190438	A1	8/2008	Harlev et al.
2008/0221566	A1	9/2008	Krishnan
2008/0234588	A1	9/2008	Feldman et al.
2008/0249424	A1	10/2008	Harlev et al.
2009/0171274	A1	7/2009	Harlev et al.
2009/0177072	A1	7/2009	Harlev et al.
2009/0253976	A1	10/2009	Harlev et al.
2009/0299355	A1	12/2009	Bencini et al.
2010/0286551	A1	11/2010	Harlev et al.
2012/0078077	A1	3/2012	Harlev et al.
2012/0277567	A1	11/2012	Harlev et al.
2013/0172715	A1	7/2013	Just et al.
2013/0345538	A1	12/2013	Harlev et al.
2014/0018880	A1	1/2014	Zarins et al.
2014/0200442	A1	7/2014	Harlev et al.
2015/0223726	A1	8/2015	Harlev
2015/0342491	A1	12/2015	Marecki et al.
2015/0351652	A1	12/2015	Marecki et al.
2015/0374252	A1	12/2015	de la Rama et al.

FOREIGN PATENT DOCUMENTS

EP	1484026	A1	12/2004
EP	2265172	A2	12/2010
EP	2269505	B1	5/2012
JP	H08511438	A	12/1996
JP	H11504541	A	4/1999
JP	2000504242	A	4/2000
JP	2002078694	A	3/2002
WO	1995/013111		5/1995
WO	1996/034652		11/1996
WO	WO199725917	A1	7/1997
WO	2002/043789		6/2002
WO	2005/114720		12/2005
WO	2006/036408		4/2006
WO	2008097767	A2	8/2008
WO	2009085108	A1	7/2009
WO	2009123819	A2	10/2009
WO	2014110579	A1	7/2014
WO	2015187386	A1	12/2015
WO	2015187430	A2	12/2015

OTHER PUBLICATIONS

Adams et al., "Seeded Region Growing", IEEE Transactions on Pattern Analysis and Machine Intelligence, 16(6):641-647, 1994.

Arthur, "Clinical Use of Intracardiac Impedance: Current Applications and Future Perspectives", PACE, vol. 24:500-506, Apr. 2001.

Authorized officer Carl H. Layno, International Search Report and the Written Opinion in PCT/US07/70854 dated Sep. 12, 2008, 15 pages.

Authorized officer Lee W. Young, International Search Report and the Written Opinion in PCT/US08/52385 dated Aug. 8, 2003, 11 pages.

Authorized officer, Blaine R. Copenheaver, International Search Report and the Written Opinion in PCT/US2009/061277 dated Apr. 8, 2010, 13 pages.

Baan, Jan et al., "Continuous Measurement of Left Ventricular Volume in Animals and Humans by Conductance Catheter", Circulation, 07(5):812-823, 1984.

Badics, "Real-Time Reconstruction of Endocardial Potential Maps in Non-Contact Cardiac Mapping", International Journal for computation and Mathematics in Electrical Engineering (COMPEL), vol. 28, No. 4, 2009.

Ben-Haim et al., "Nonfluoroscopic, in Vivo Navigation and Mapping Technique", Nature Medicine, 2(12):1393-1395, 1996.

Besi et al., "A Method for Registration of 3-D Shapes", IEEE Transaction on Pattern Analysis and Machine Intelligence, 14(2):239-256, 1992.

Blomstrom-Lundqvist et al., "ACC/AHA/ESC Guidelines for the Management of Patients with Supraventricular Arrhythmias-Executive Summary", Journal of the American College of Cardiology, 42(8):1493-1531, 2003.

Breithardt et al., "AHA Medical/Scientific Statement—Special Report: Standards for Analysis of Ventricular Late Potentials Using High-Resolution or Signal/Averaged Electrocardiography", Circulation, 83(4):1481-1488, 1991.

Brooks et al., "Electrical Imaging of the Heart", IEEE Signal Processing Magazine, pp. 24-42, 1997.

Caspi et al., "Stem Cell Research: Regenerating the Heart Using Human Embryonic Stem Cells—from Cell to Bedside", IMAJ 8:208-214, 2006.

Cheney et al., "Electrical Impedance Tomography," SIAM Review 41, pp. 85-101, 1999.

Communication pursuant to Article 94(3) EPC in European Application No. 07798369, dated Nov. 17, 2011, 5 pages.

De Groot et al., "Three-Dimensional Catheter Positioning During Radiofrequency Ablation in Patients: First Application of a Real-Time Position Management System", Journal of Cardiovascular Electrophysiology, 11:1183-1192, 2000.

Donahue et al., "Focal Modification of Electrical Conduction in the Heart by Viral Gene Transfer", Nature Medicine, 6 (12):1395-1398, 2000.

Dong et al., "Integrated Electroanatomic Mapping With Three-Dimensional Computed Tomographic Images for Real-Time Guided Ablations", Circulation 113:186-194, 2006.

Durrer et al., "Total Excitation of the Isolated Human Heart", Circulation, XL1:899-912, 1970.

Ector, Joris et al., "Cardiac Three-Dimensional Magnetic Resonance Imaging and Fluoroscopy Merging", Circulation, 112:3769-3776, 2005.

Extended European Search Report issued in EP Application No. 09727423.7, dated May 15, 2012, 5 pages.

Friedman, "Catheter Cryoablation of Cardiac Arrhythmias", Current Opinion in Cardiology, 20:48-54, 2005.

Friedman, "Novel Mapping Techniques for Cardiac Electrophysiology", Heart, 37:575-582, 2002.

Geddes et al., "Criteria for the Selection of Materials for Implanted Electrodes," Annals of Biomedical Engineering 31:879-890, 2003.

Gepstein et al., "A Novel Method for Nonfluoroscopic Catheter-Based Electroanatomical Mapping of the Heart", Circulation 95:1611-1622, 1997.

Haug, E. J. et al.: Design Sensitivity Analysis of Structural Systems, Mathematics in Science and Engineering, vol. 177 (1986).

Huang, Yi-Chih et al., "Development of a Third Generation Intraventricular Impedance Imaging (Iii) System Evaluation of Hardware Design", Engineering in Medicine and Biology Society, Proceedings of the 19th Annual Internal Conference of the IEEE/EMBS, 6:2442-2444 Oct. 30-Nov. 2, 1997

International Preliminary Report on Patentability issued in PCT/US2008/052385, dated Aug. 8, 2008, 6 pages.

International Preliminary Report on Patentability issued in PCT/US2009/036099, dated Oct. 14, 2010, 20 pages.

International Search Report and Written Opinion issued in PCT/US2009/036099, dated Apr. 28, 2009, 21 pages.

International Search Report and Written Opinion issued in PCT/US2014/060137, dated Dec. 10, 2014, 11 pages.

Jain et al., "Cell Therapy Attenuates Deleterious Ventricular Remodeling and Improves Cardiac Performance after Myocardial Infarction", Circulation, 103:1920-1927, 2001.

Jalife, "Rotors and Spiral Waves in Atrial Fibrillation", Journal of Cardiovascular Electrophysiology, 14:776-780, 2003.

Jane et al., Alignment Methods for Averaging of High-Resolution Cardiac Signals: A Comparative Study of Performance, IEEE Transaction on Biomedical Engineering, 38(6):571-579, 1991.

Jia et al., "Electrophysiologic Endocardial Mapping from a Noncontact Nonexpandable Catheter: A Validation Study of a

(56)

References Cited

OTHER PUBLICATIONS

- Geometry-Based Concept". *Journal of Cardiovascular Electrophysiology*, 11:1238-1251, 2000.
- Kikuchi et al., "Targeted Modification of Atrial Electrophysiology by Homogeneous Transmural Atrial Gene Transfer", *Circulation*, 111:264-270, 2005.
- Kistler et al., "Validation of Three-Dimensional Cardiac Image Integration: Use of Integrated CT Image into Electroanatomic Mapping System to Perform Catheter Ablation of Atrial Fibrillation", *Journal of Cardiovascular Electrophysiology*, 17:341-348, 2006.
- Kuklik et al., The reconstruction, from a set of points, and analysis of the interior surface of the heart chamber, *Physiological Measurement* 25, pp. 617-627, 2004.
- Kun, Stevan et al., "Conductance Volumetric Model of an Eccentrically Positioned Catheter within a Three-Compartment Ellipsoidal Ventricle", *U, IEEE Transactions on Jun.* 1993, 40(6): 589-592.
- L. Piegl, W. Tiller: *The NURBS Book*, 2nd Edition, Springer (1997).
- Laciar et al., "Improved Alignment Method for Noisy High-Resolution ECG and Holter Records Using Multiscale Cross-Correlation", *IEEE Transactions on Biomedical Engineering*, 50(3):344-353, 2003.
- Liu et al., "Endocardial Potential Mapping from a Noncontact Nonexpandable Catheter: A Feasibility Study", *Annals of Biomedical Engineering*, 26:994-1009, 1998.
- Lorensen et al., "Marching Cubes: A High Resolution 3D Surface Construction Algorithm", *Computer Graphics* 21 (4):163-169, Jul. 1987.
- Makela et al., "A Review of Cardiac Image Registration Methods", *IEEE Transaction on Medical Imaging*, 21(9):1011-1021, 2002.
- Malladi, R. et al., "A Geometric Approach to Segmentation and Analysis of 3D Medical Images", *Mathematical Methods in Biomedical Image Analysis, Proceedings of the Workshop on Jun.* 21-22, 1996, pp. 244-252.
- Mangan, Alan et al., "Partitioning 3D Surface Meshes Using Watershed Segmentation", *IEEE Transactions on Visualization and Computer Graphics*, 5(4):308-321, 1999.
- International Search Report and Written Opinion issued in PCT/US2015/032004, dated Sep. 4, 2015, 8 pages.
- European Search Report issued in EP Application No. 12815179.2, dated Apr. 28, 2015, 6 pages.
- International Preliminary Examination Report issued in PCT/US2008/013553, completed Jan. 22, 2009, 6 pages.
- International Search Report and Written Opinion issued in PCT/US208/13553, dated Feb. 5, 2009, 6 pages.
- International Preliminary Report on Patentability issued in PCT/US2015/032004, dated Dec. 6, 2016, 7 pages.
- International Preliminary Report on Patentability issued in PCT/US2015/032753, dated Dec. 6, 2016, 10 pages.
- Meininger et al., "Initial Experience with a Novel Focused Ultrasound Ablation System for Ring Ablation Outside the Pulmonary Vein", *Journal of Interventional Cardiac Electrophysiology*, 8:141-148, 2003.
- Merrill, Daniel R. et al., "Electrical stimulation of excitable tissue: design of efficacious and safe protocols", *Journal of Neuroscience Methods*, 141:171-198, 2005.
- Miller, "Editor's Forum—Application of Registration for Ablation: A Marriage of Technologies", *Journal of Interventional Cardiac Electrophysiology*, 11:87-89, 2004.
- Nademanee et al., "A New Approach for Catheter Ablation of Atrial Fibrillation: Mapping of the Electrophysiologic Substrate", *Journal of the American College of Cardiology*, 43(11):2044-2053, 2004.
- Non-Final Office Action in U.S. Appl. No. 11/451,908, dated Sep. 4, 2008, 12 pages.
- Non-Final Office Action issued in U.S. Appl. No. 11/451,898 dated Sep. 25, 2008, 13 pages.
- Noseworthy et al., "The impact of Respiration on Left Atrial and Pulmonary Venous Anatomy: Implications for Image-Guided Intervention", *Heart Rhythm*, 2:1173-1178, 2005.
- Pappone et al., "Robotic Magnetic Navigation for Atrial Fibrillation Ablation", *Journal of the American College of Cardiology*, 47(7): 1390-1400, 2006.
- Paragios, "A Level Set Approach for Shape-Driven Segmentation and Tracking of the Left Ventricle", *IEEE Transactions on Medical Imaging*, 22(6):773-776, 2003.
- Persson et al., "A Simple Mesh Generator in MATLAB", *SIAM Review*, 46(2):329-345, 2004.
- Persson, "Mesh Generation for Implicit Geometrics", *Massachusetts Institute of Technology—Thesis*, Feb. 5, 2006.
- Pham, Dzung, et al., "Current Methods in Medical Image Segmentation", *Annu. Rev. Biomed. Eng.*, 02:315-337, 2000.
- Rao et al., "Novel Noncontact Catheter System for Endocardial Electrical and Anatomical Imaging", *Annals of Biomedical Engineering*, 32(4):573-584, 2004.
- Reddy et al., "Use of a Diode Laser Balloon Ablation Catheter to Generate Circumferential Pulmonary Venous Lesions in an Open-Thoracotomy Caprine Model", *PACE*, 27:52-57, 2004.
- Reddy et al., "Integration of Cardiac Magnetic Resonance Imaging with Three-Dimensional Electroanatomic Mapping to Guide Left Ventricular Catheter Manipulation—Feasibility in a Porcine Model of Healed Myocardial Infarction" *Journal of the American College of Cardiology*, 44(11):2202-2213, 2004.
- Sanders et al., "Spectral Analysis Identifies Sites of High-Frequency Activity Maintaining Atrial Fibrillation in Humans", *Circulation*, 112:789-797, 2005.
- Sethian, "Level Set Methods and Fast Marching Methods: Evolving Interfaces in Computational Geometry, Fluid Mechanics, Computer Vision, and Materials Science", *Department of Mathematics—University of California, Berkeley, Cambridge University Press*, 1999.
- Simon et al., "Electroanatomic Mapping of the Right Arm With a Right Atrial Basket Catheter and Three-Dimensional Intracardiac Echocardiography", *PACE*, 27: 318-326, 2004.
- Smits et al., "Catheter-Based Intramyocardial Injection of Autologous Skeletal Myoblasts as a Primary Treatment of Ischemic Heart Failure", *Journal of the American College of Cardiology*, 42(12):2063-2069, 2003.
- Solomon et al., "Real-Time Cardiac Catheter Navigation on Three-Dimensional CT Images", *Journal of Interventional Cardiac Electrophysiology*, 8:27-36, 2003.
- Sra et al., "Registration of Three-Dimensional Left Atrial Computed Tomographic Images With Projection Images Obtained Using Fluoroscopy", *Circulation*, 112:3763-3768, 2005.
- Sra, Jasbir et al., "Registration of 3D Computed Tomographic Images With Interventional Systems: Implications for Catheter Ablation of Atrial Fibrillation", *J Intery Card Electrophysiol*, 16:141-148, 2006.
- Stevenson, "Radiofrequency Catheter Ablation of Ventricular Tachycardia After Myocardial Infarction", *Circulation*, 98:308-314, 1998.
- Taccardi et al., "A New Intracavitary Probe for Detecting the Site of the Origin of Ectopic Ventricular Beats During One Cardiac Cycle", *Circulation*, 75(1):272-281, 1987.
- Thal et al., "Novel Applications in Catheter Ablation", *Journal of Interventional Cardiac Electrophysiology*, 13:17-21, 2005.
- Thiagalingam et al., "Noncontact Mapping of the Left Ventricle: Insights from Validation With Transmural Contact Mapping", *PACE*, 27:570-578, 2004.
- Voth, "The Inverse Problem of Electrocardiography: Industrial Solutions and Simulations", *BEM and NFSI Conference Proceedings*, Minneapolis, MN, May 12-15, 2005, pp. 191-194.
- Wittkamp et al., "LocaLisa: New Technique for Real-Time 3-Dimensional Localization of Regular Intracardiac Electrodes", *Circulation*, 99:1312-1317, 1999.
- Yezzi, Anthony et al., "A Geometric Snake Model for Segmentation", *IEEE Transactions on Medical Imaging*, 16(2) Apr. 1997.
- International Preliminary Report on Patentability issued in PCT/US2014/060137, dated Apr. 28, 2016, 9 pages.
- Authorized officer Yoshiko Kuwahara, International Preliminary Report on Patentability in PCT/US2008/013553 dated Jul. 8, 2010, 7 pages.

(56)

References Cited

OTHER PUBLICATIONS

Authorized officer Patricia Jameson, Supplementary Partial European Search Report in Application No. 08867908.9, dated Sep. 6, 2011, 12 pages.

International Search Report and Written Opinion issued in PCT/US2015/032753, dated Mar. 9, 2016, 17 pages.

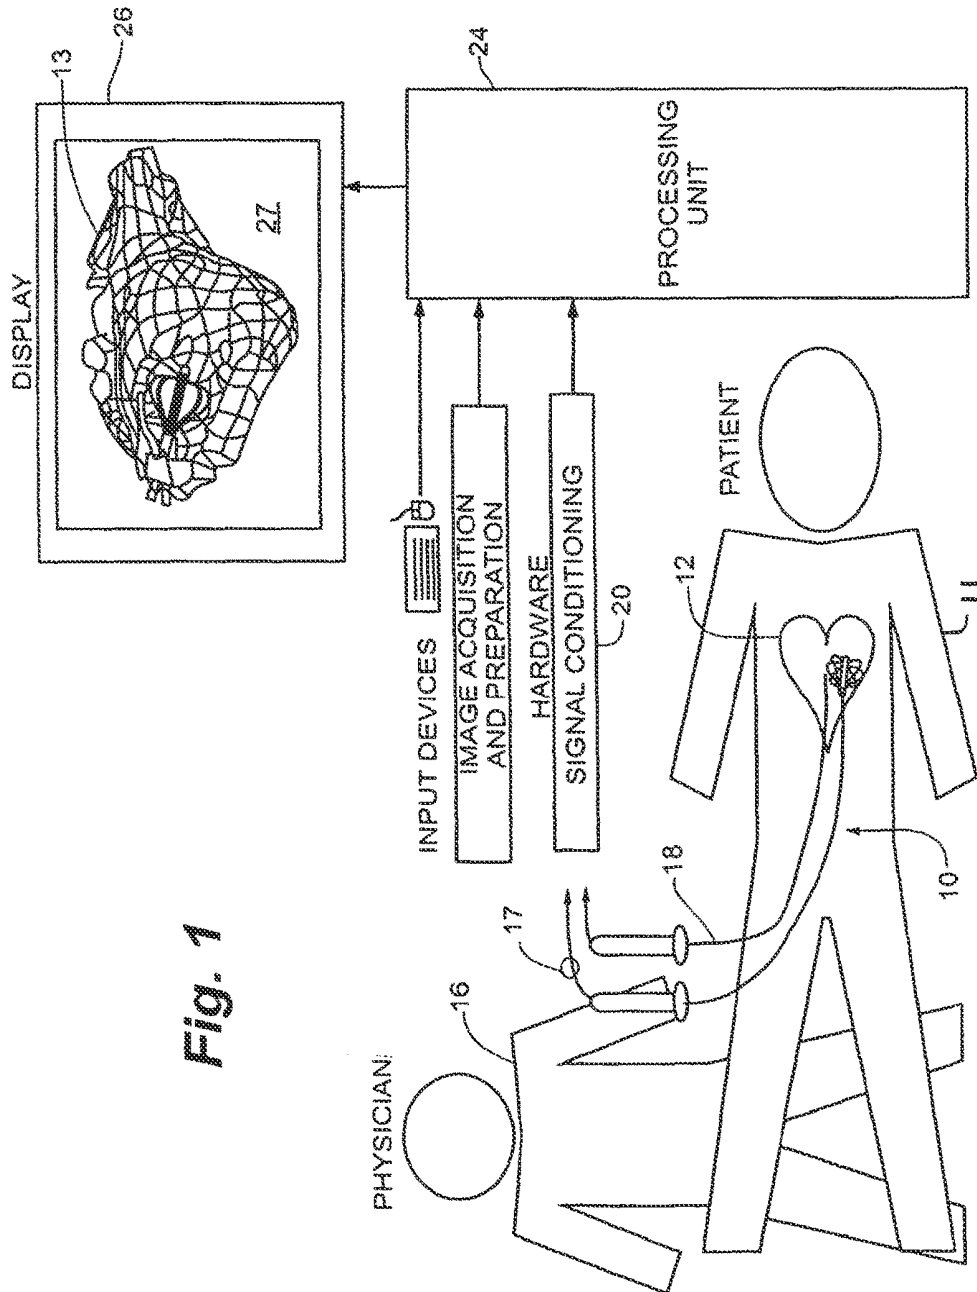


Fig. 2A

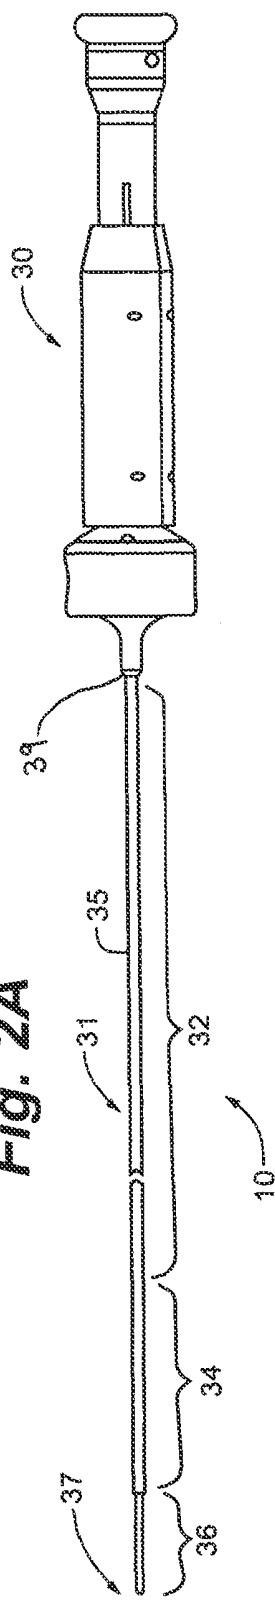


Fig. 2B

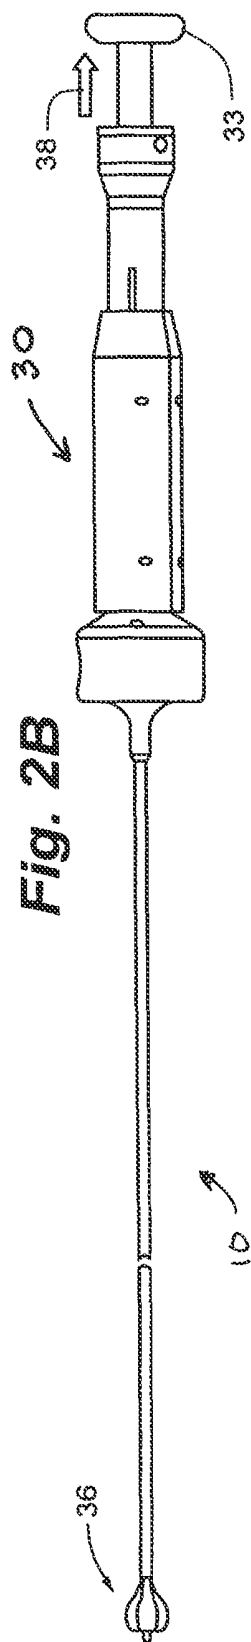


Fig. 2C

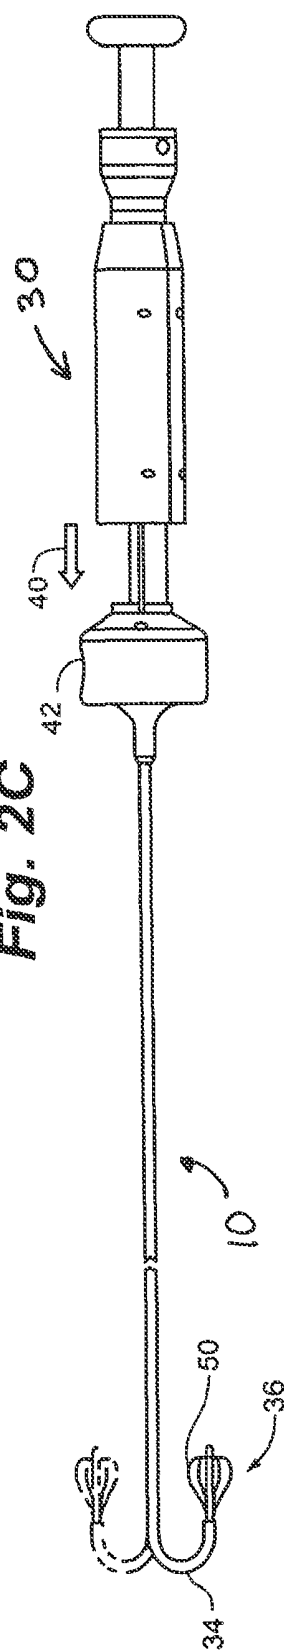


Fig. 3B

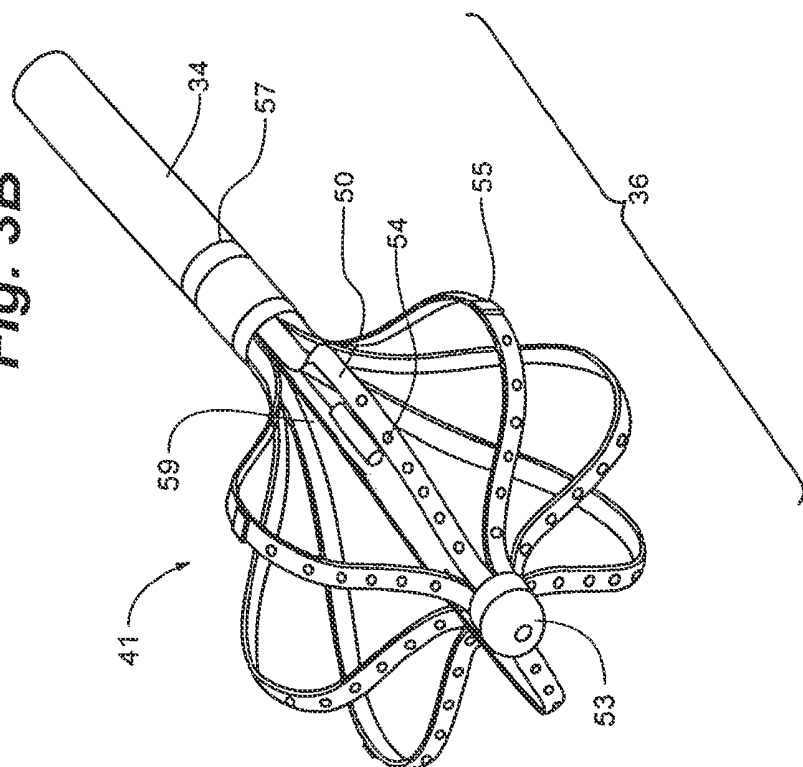
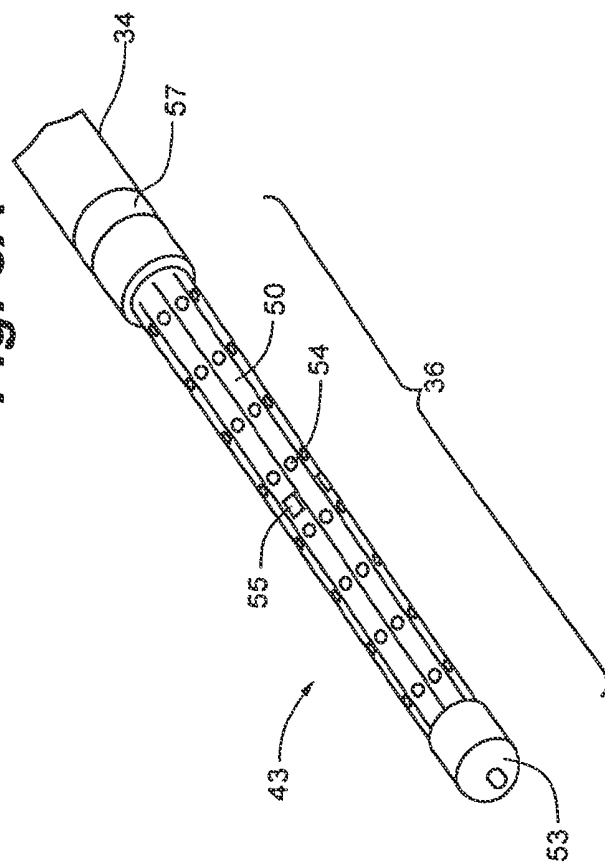


Fig. 3A



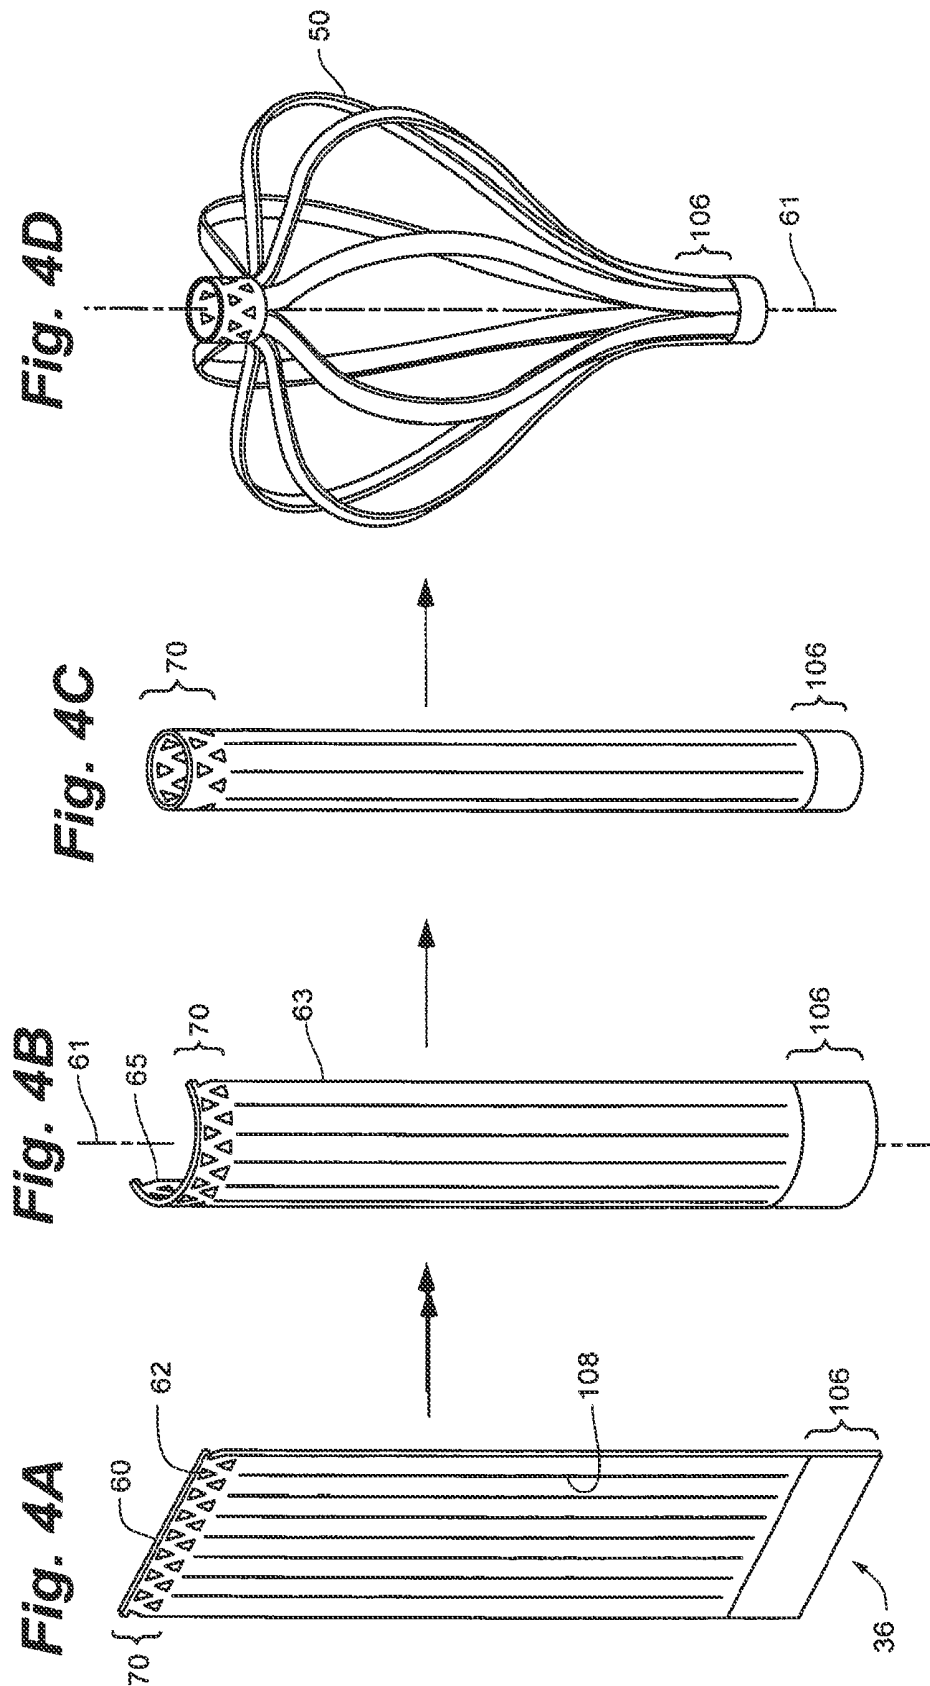


Fig. 5B

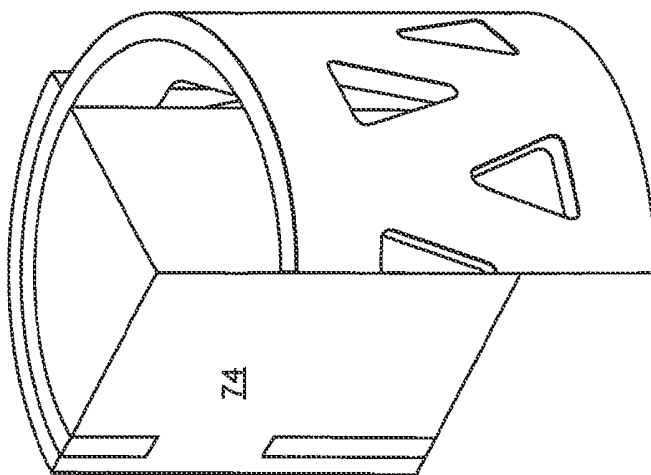
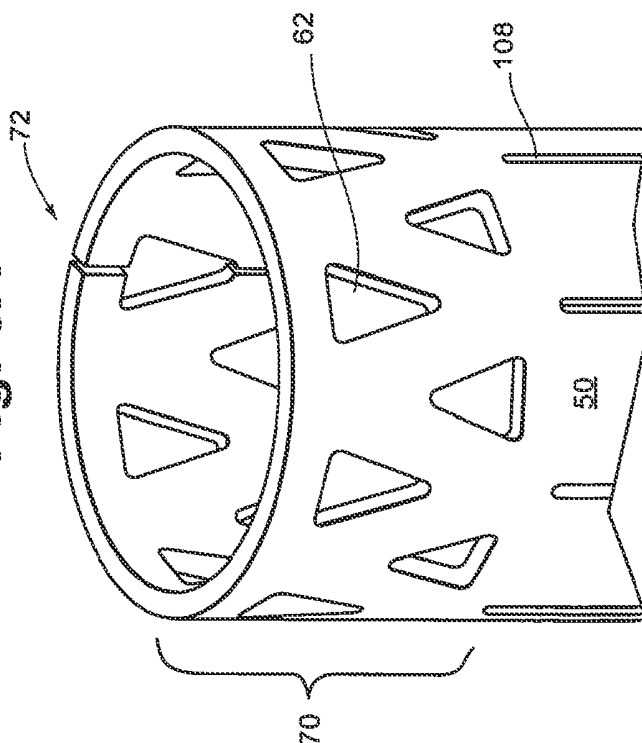


Fig. 5A



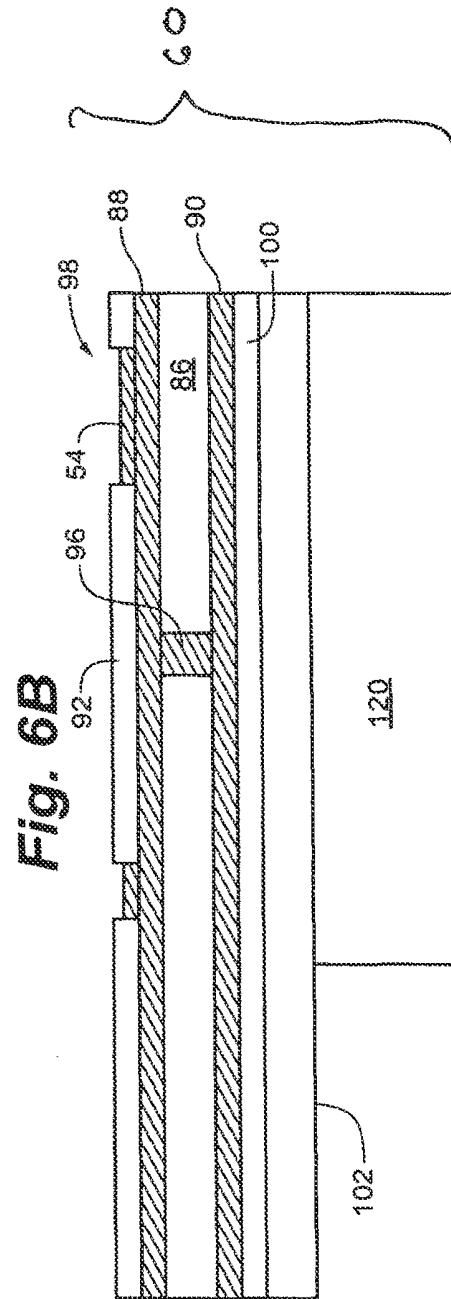
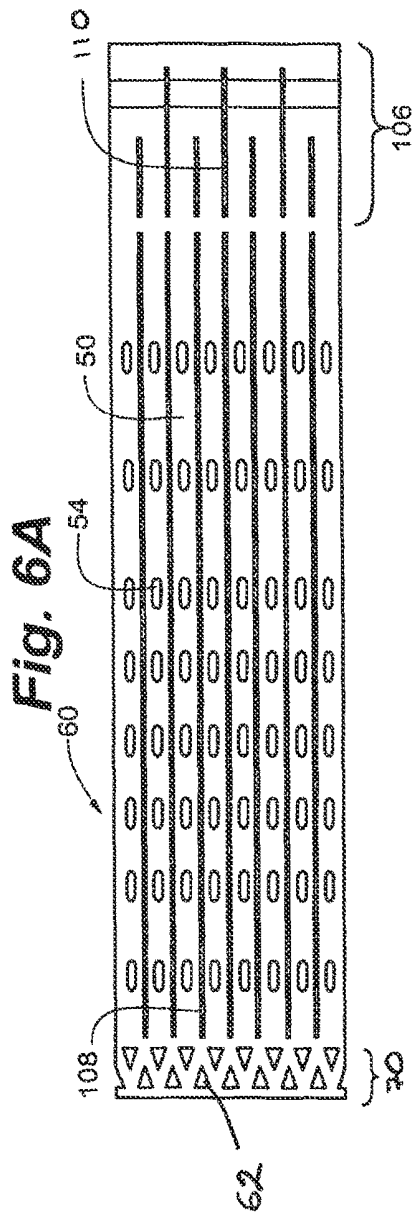


Fig. 7

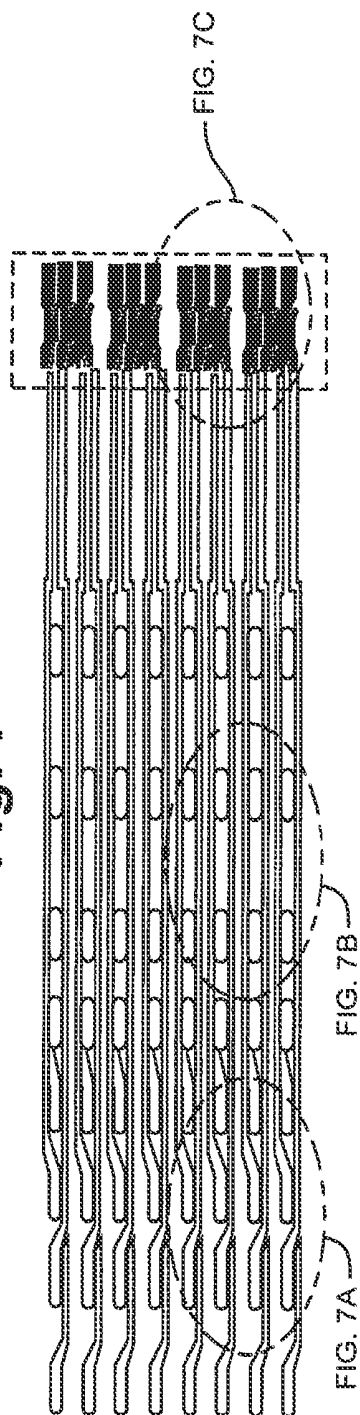


Fig. 7C

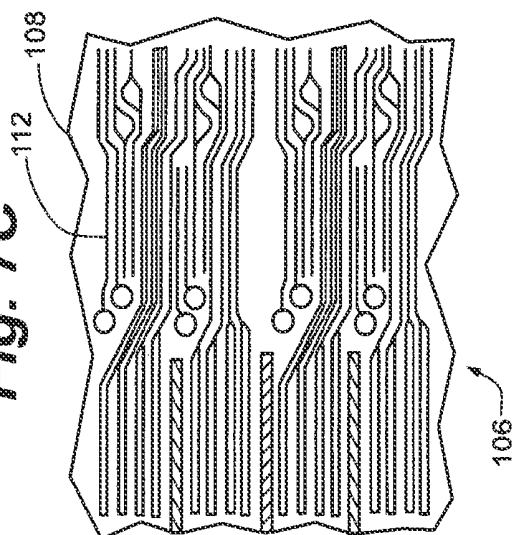


Fig. 7B

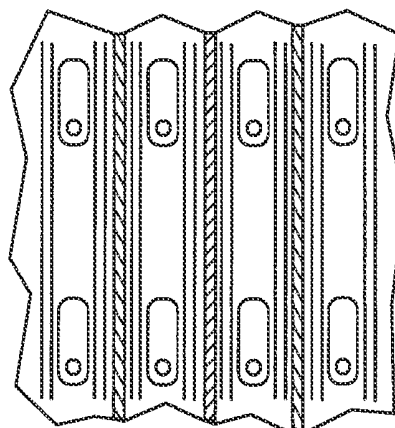
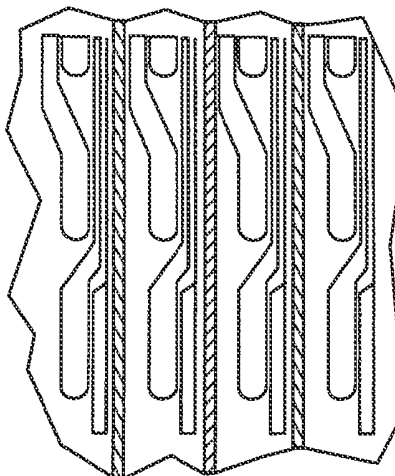


Fig. 7A



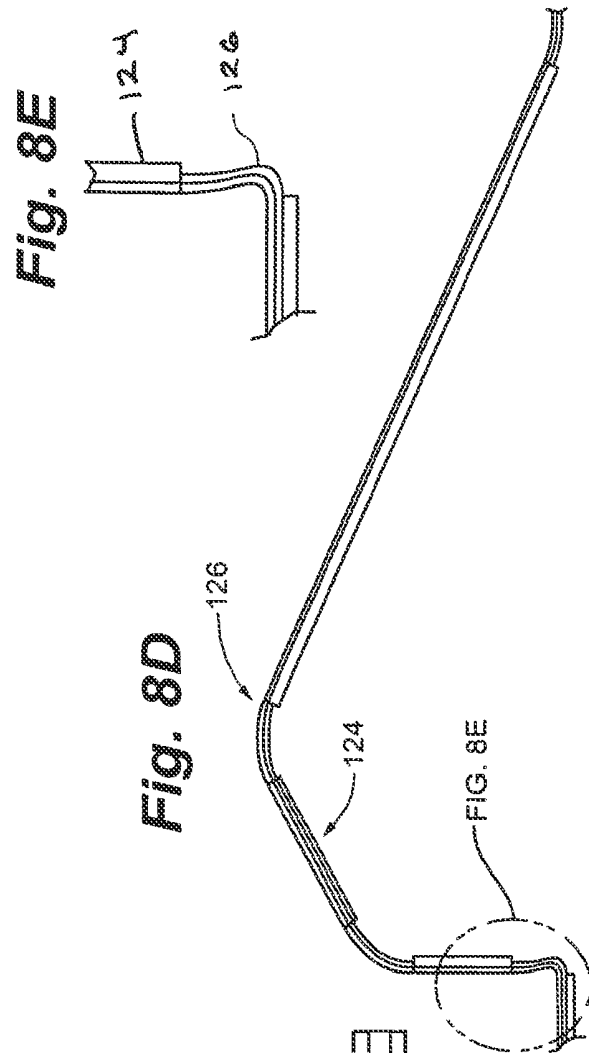
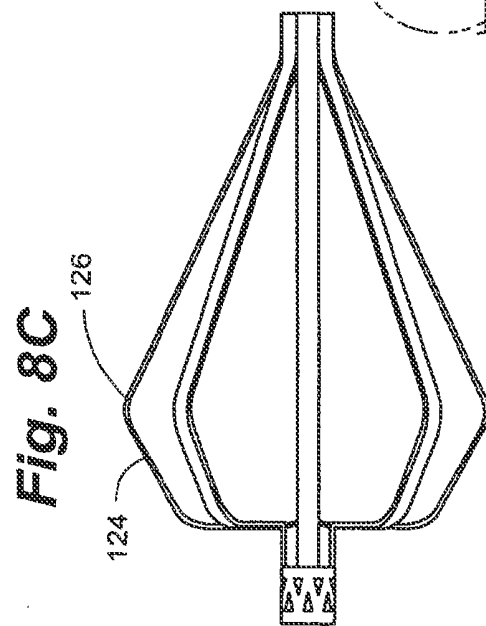
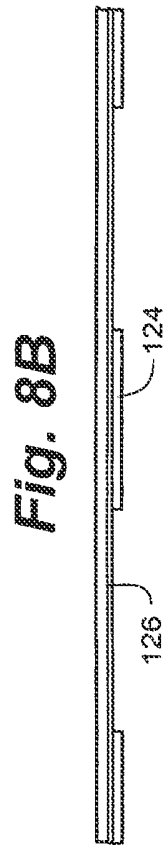
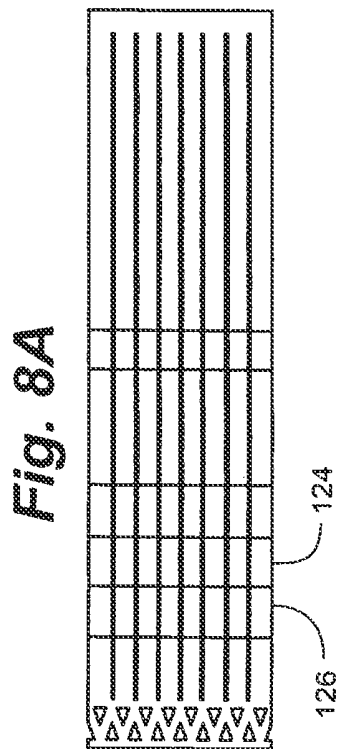


Fig. 9A

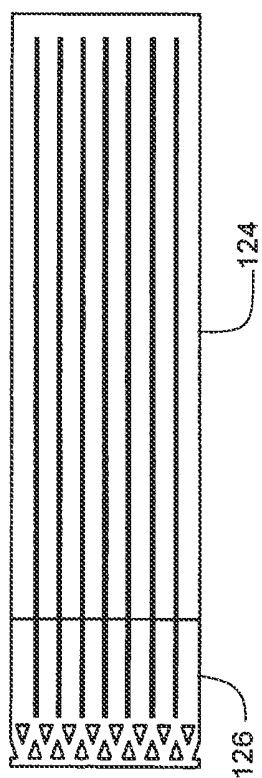


Fig. 9B

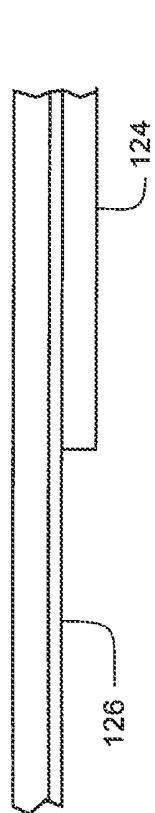


Fig. 9C

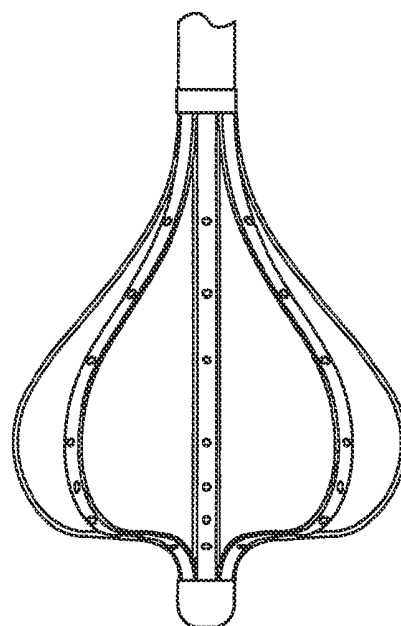


Fig. 9D

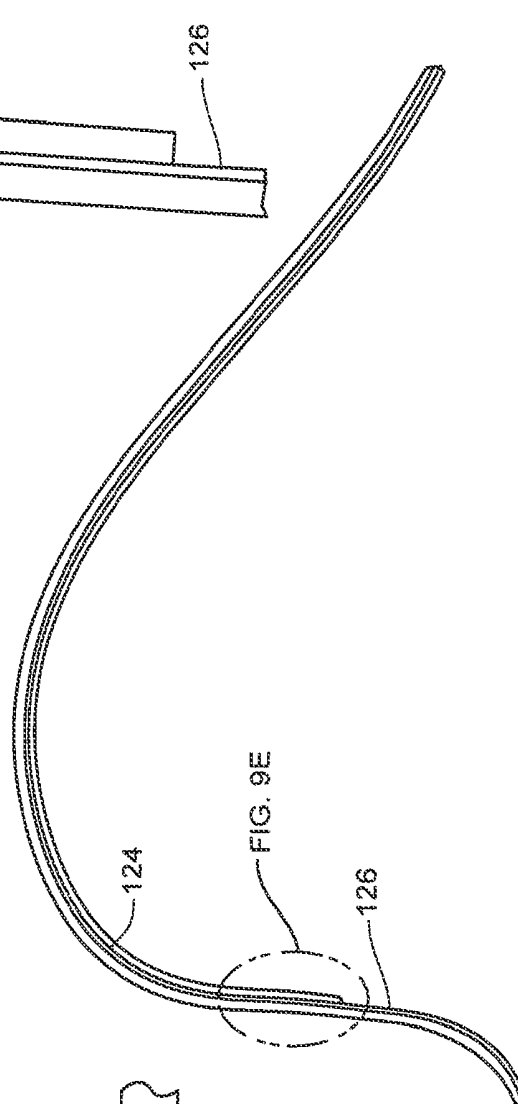
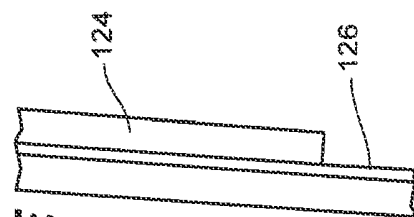
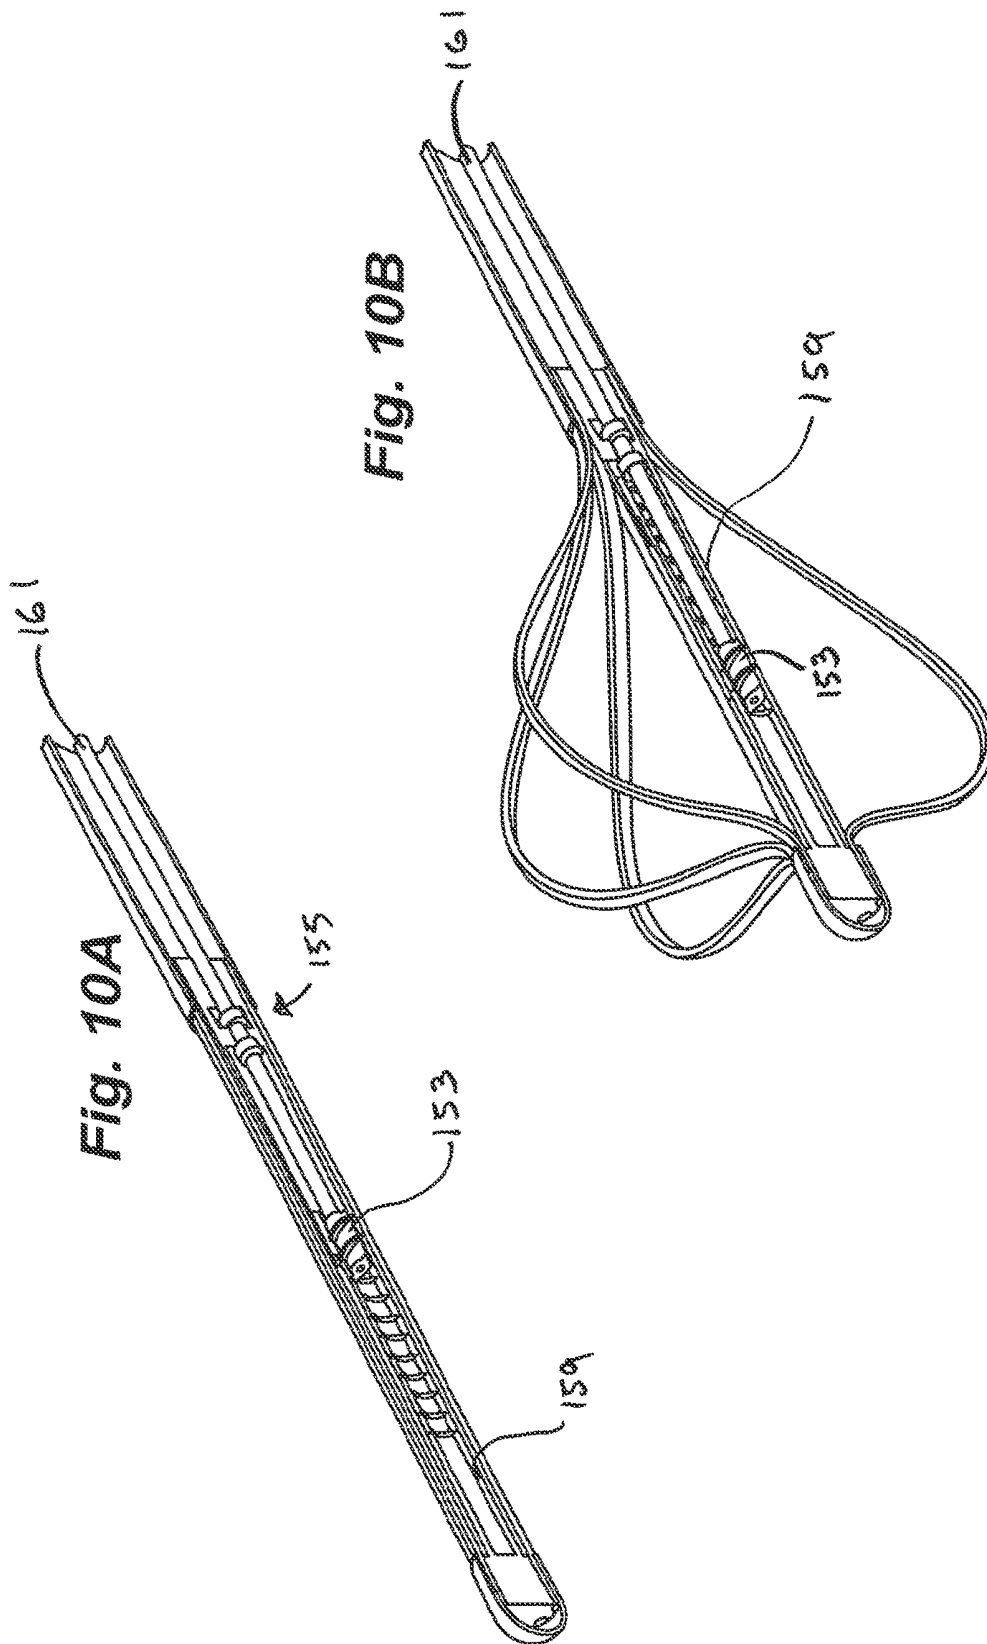


Fig. 9E





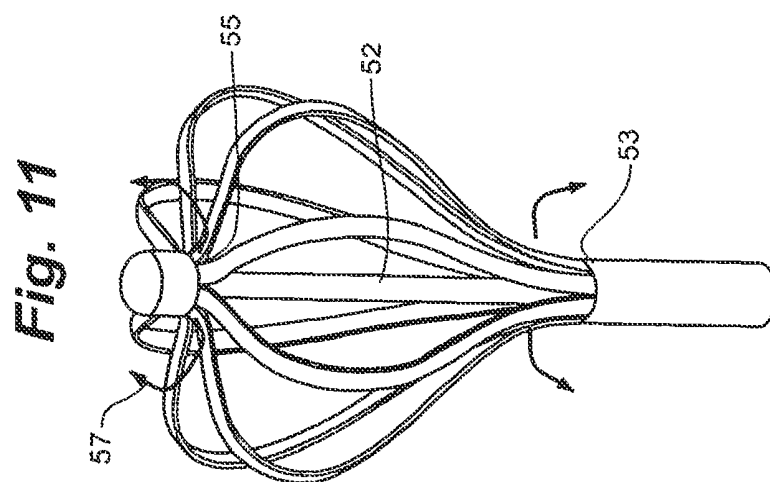
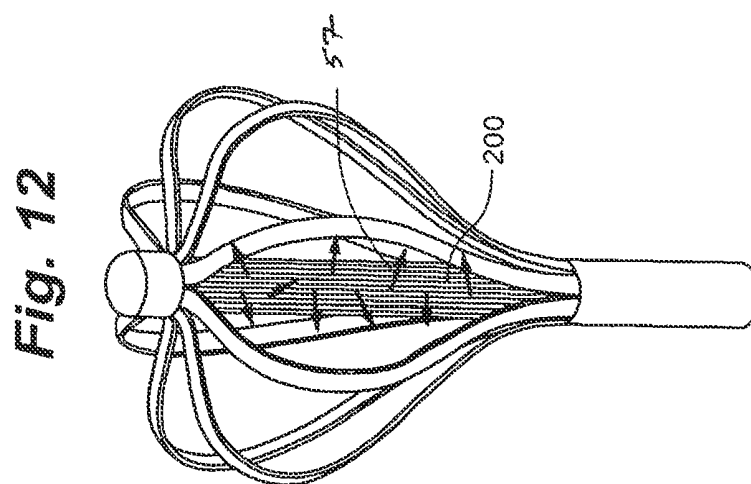
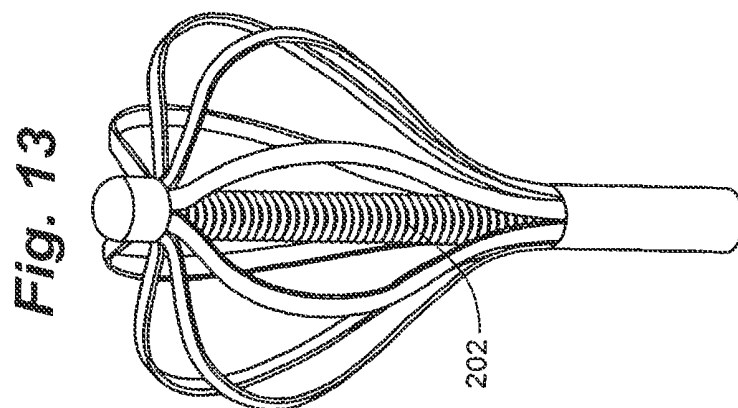


Fig. 14

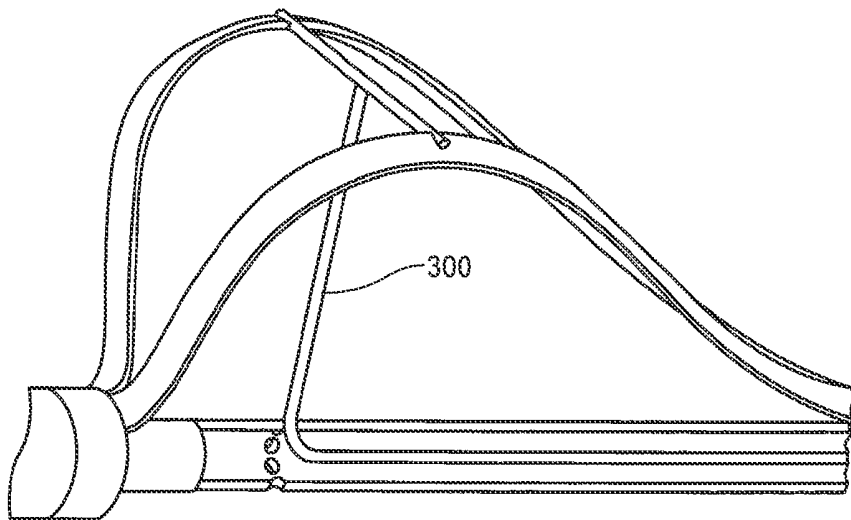


Fig. 15

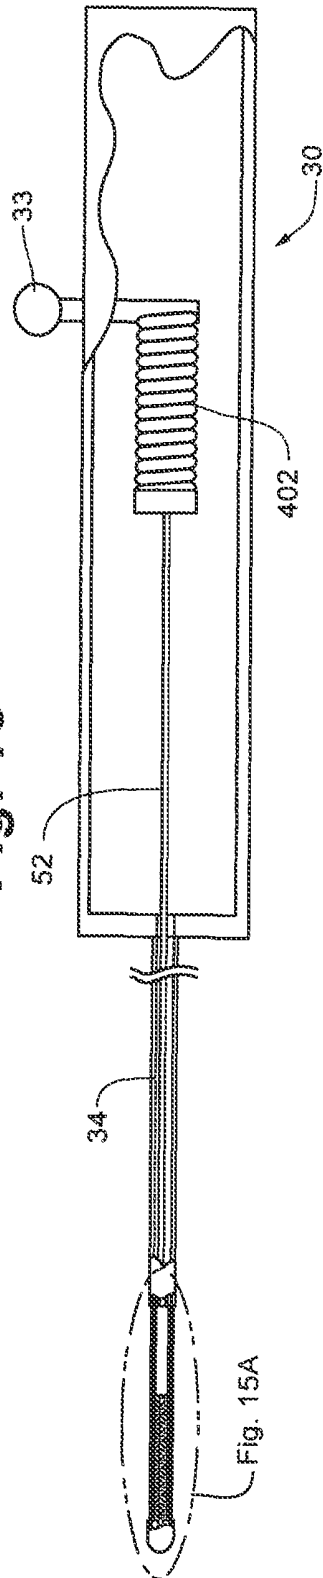
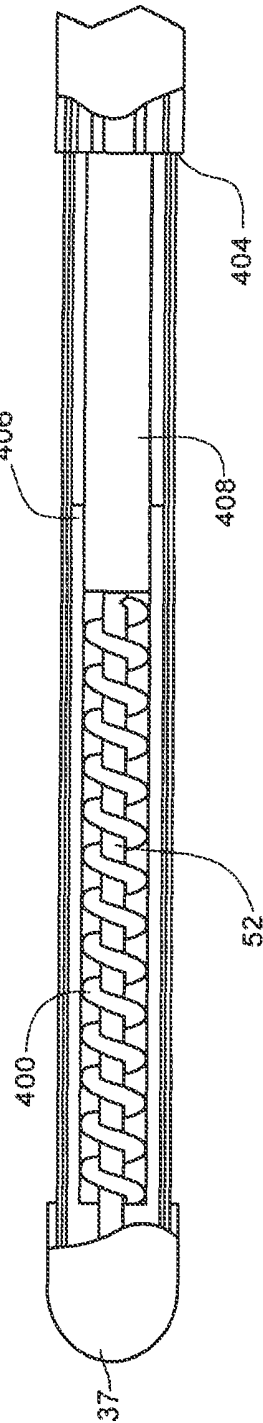


Fig. 15A






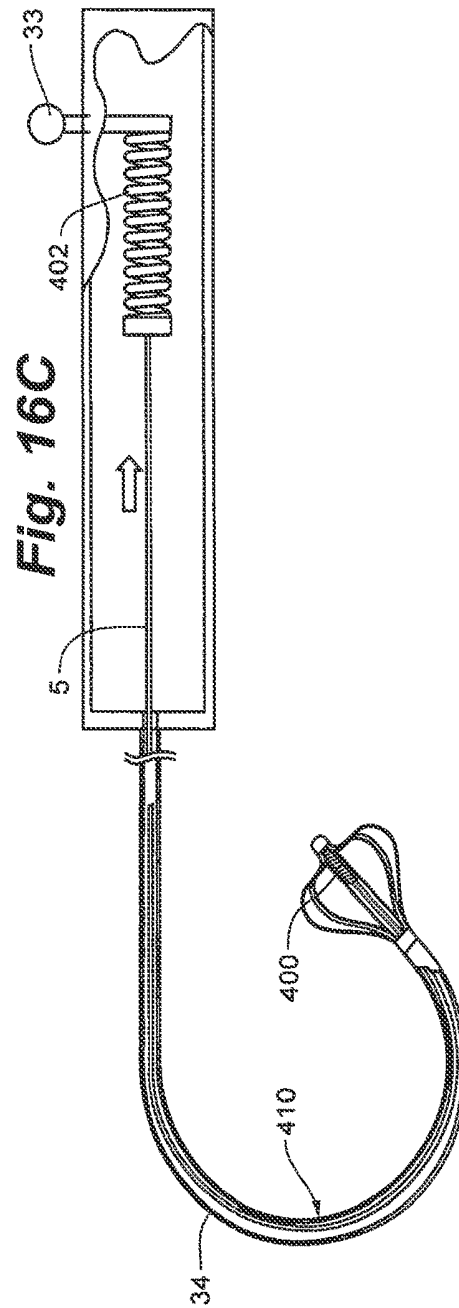


Fig. 17

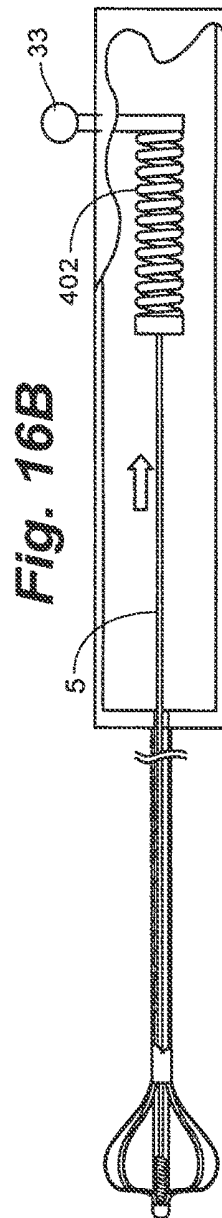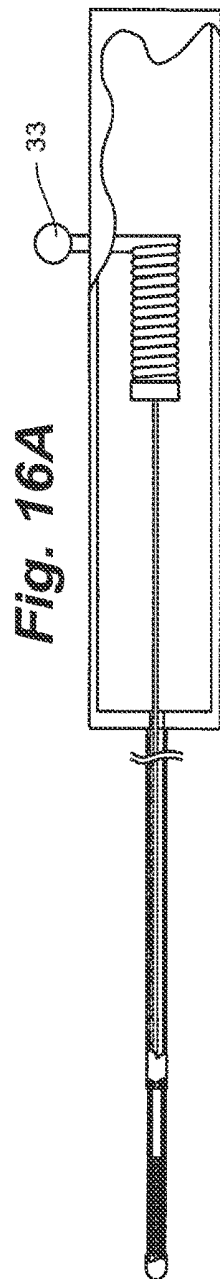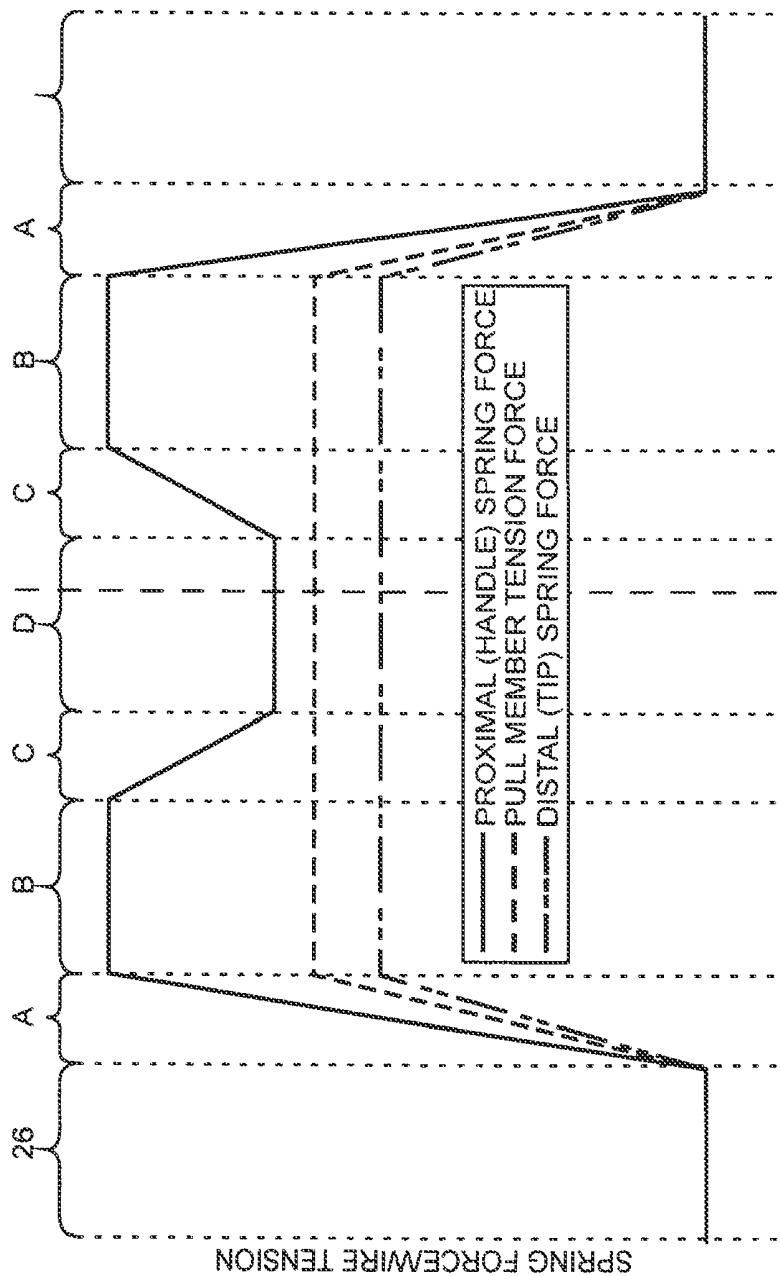

CARDIAC MAPPING CATHETER**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a continuation application and claims priority under 35 U.S.C. § 120 to U.S. patent application Ser. No. 13/868,151, filed on Apr. 23, 2013, now U.S. Pat. No. 8,755,861, which is a continuation of U.S. patent application Ser. No. 13/289,367, filed on Nov. 4, 2011, now U.S. Pat. No. 8,447,377, which is a continuation of U.S. patent application Ser. No. 12/005,975, filed on Dec. 28, 2007, now U.S. Pat. No. 8,103,327, the entire contents of which are hereby incorporated by reference.

FIELD OF THE INVENTION

The present invention relates generally to a catheter for use inside the human heart during medical procedures. The catheter can be used for “non-contact” mapping of the electrical activity of the heart, for locating and reporting the position of other procedure catheters within the heart, and for other purposes. The catheter includes an electrode array that can be deployed and retracted independently from catheter articulation.

BACKGROUND OF THE INVENTION

Cardiac arrhythmias are a leading cause of stroke, heart disease, and sudden death. The physiological mechanism of arrhythmia involves an abnormality in the electrical conduction of the heart. There are a number of treatment options for patients with arrhythmia that include medication, implantable devices, and catheter ablation of cardiac tissue.

Traditionally, the arrhythmia is studied and diagnosed by “electrically mapping” the heart with catheters inserted through the vasculature into a heart chamber. Traditionally, the electrical activity of the heart is acquired directly by “in-contact” mapping of the interior wall surface of a heart chamber. In this technique electrodes are placed in intimate contact with the heart wall and the voltage at that location is recorded and plotted against time for display to the physician. The in-contact catheters may be large and essentially fill the entire heart chamber, or they may be smaller and moved around in the heart chamber to sequentially map various areas of the heart. Mechanically, the in-contact mapping catheters are “soft” so that they can conform to the heart chamber. Softness is required so the electrodes come into intimate contact with the heart wall while accommodating wall motion of the beating heart.

For example, multiple electrode in-contact mapping catheters are known from U.S. Pat. No. 5,628,313 to Webster that shows a so-called “basket” catheter. In use, this very flexible and conformal catheter is deployed in the heart and presses individual electrodes against the chamber wall for full chamber contact mapping of a beating heart. Smaller multiple electrode catheters are known as well. For example, the U.S. Pat. No. 5,279,299 to Imran illustrates techniques for creating smaller catheter arrays that are used to selectively contact map portions of the cardiac chamber. This catheter is flexible and electrodes remain in contact with the wall even when the catheter shaft is displaced slightly. In each of these examples, the limbs of the catheter are very flexible and gently contact the chamber wall while the wall of the heart is moving.

“Non-contact mapping,” also known in the art, is an alternative to in-contact mapping where a catheter array

positioned within a chamber is used to collect global electrical information. This global information is then used to compute a solution to the so-called “inverse problem”. The inverse problem of electrophysiology is the calculation of wall electrical potentials from the measured field voltages associated with the wall potentials as measured within the blood pool remote from the chamber wall. The mathematical “solution” displayed to the physician is the computed wall surface voltages that can be used to detect problems in electrical conduction in the heart wall.

Although in-contact and non-contact catheters are used for the same patient indications, they have very different mechanical and electrical requirements. Chief among the requirements of a non-contact catheter is stability of the electrode array. The geometry and locations of the electrodes are assumed for the inverse solution calculation and need to be known with great precision. Small error in electrode position can render large discrepancies in computed mathematical solution. In addition, controlled movement of the electrode array within the chamber of interest is necessary in order to improve the accuracy of the non-contact map. Deployment of the electrode array into a repeatable precisely known shape, while supporting controlled movement of the catheter, pose particularly complex and novel requirements on the catheter design.

Once the anatomic origin of problems in electrical conduction are identified, the physician may proceed to ablate the offending tissue, thus treating the arrhythmia. Catheter ablation procedures have evolved in recent years to become an established treatment for patients with a variety of supraventricular and ventricular arrhythmias. The typical catheter ablation procedure involves mapping of the heart tissue in order to identify the site of origin of the arrhythmia, followed by a targeted ablation of the site with an RF catheter. The procedure takes place in an electrophysiology laboratory and takes several hours most of which is spent mapping the electrical conduction in the heart.

Although in-contact and non-contact mapping methods are known in the art and various deflectable, displaceable and deployable catheters are known as well, there is a continuing need to improve the accuracy, stability and maneuverability of such devices so that they can be more widely used, especially as an adjunct to cardiac ablation procedures.

SUMMARY OF THE INVENTION

The present invention is an intravascular catheter that may be deployed within a heart chamber placing multiple electrodes in a known spatial configuration. The catheter may be used to map electro-anatomical characteristics of the heart and/or to locate and position other catheters within the heart. Adoption of the inventive construction of the present catheter provides a device that is smaller, less expensive to manufacture, maneuverable, and stable in its deployed configuration. Electrode stability makes the device much more accurate and therefore, of more value to the physician. The design and construction also make the device smaller in cross section than existing designs and therefore, more easily used by a physician and better tolerated by the patient. As set forth in detail hereafter, the distal array of the catheter is fabricated as a flexible printed circuit. The deployment and articulation functions of the catheter are very independent of each other.

Two separate embodiments of the deployment mechanisms are disclosed. In contrast to prior art devices both of these mechanisms permit the deployment function to operate

wholly independently from the articulation or deflection feature of the catheter. The independence of the deployment feature and the articulation feature together with innovative structural features and materials create a noncontact mapping catheter that is easily placed and used with a very stable electrode geometry.

BRIEF DESCRIPTION OF THE DRAWINGS

An illustrative embodiment of the invention is shown in the several views of the figures. The use of identical reference numerals throughout the several figures and views indicate the same element of the device, wherein;

FIG. 1 is a schematic diagram showing the catheter in the context of the system;

FIG. 2A is a schematic diagram showing the catheter;

FIG. 2B is a schematic diagram showing the catheter;

FIG. 2C is a schematic diagram showing the catheter;

FIG. 3A is a schematic diagram showing the distal portion of the catheter;

FIG. 3B is a schematic diagram showing the distal portion of the catheter;

FIG. 4A shows a step in the construction of the distal portion;

FIG. 4B shows a step in the construction of the distal portion;

FIG. 4C shows a step in the construction of the distal portion;

FIG. 4D shows a step in the construction of the distal portion;

FIG. 5A shows a step in the manufacture of the distal portion;

FIG. 5B shows a step in the manufacture of the distal portion;

FIG. 6A shows the flexible printed circuit in plan view;

FIG. 6B shows the flexible printed circuit in cross-section;

FIG. 7 shows a metallization layer of the flexible printed circuit;

FIG. 7A shows a portion of the metallization layer of the flexible printed circuit of FIG. 7;

FIG. 7B shows a portion of the metallization layer of the flexible printed circuit of FIG. 7;

FIG. 7C shows a portion of the metallization layer of the flexible printed circuit of FIG. 7;

FIG. 8A shows the spline assembly formed from a flexible printed circuit in plan view;

FIG. 8B shows the spline assembly formed from a flexible printed circuit in cross-section view;

FIG. 8C shows a distal array segment in projection view;

FIG. 8D shows a spline in cross section;

FIG. 8E depicts a portion of a spline of FIG. 8D;

FIG. 9A shows the spline assembly formed from a flexible printed circuit in plan view;

FIG. 9B shows the spline assembly formed from a flexible printed circuit in cross-section view;

FIG. 9C shows a distal array segment in projection view;

FIG. 9D shows a spline in cross section;

FIG. 9E depicts a portion of the spline shown in FIG. 9D;

FIG. 10A shows a first embodiment of the deployment actuator;

FIG. 10B shows a first embodiment of the deployment actuator;

FIG. 11 shows a distal array segment in projection view;

FIG. 12 shows a distal array segment in projection view;

FIG. 13 shows a distal array segment in projection view

FIG. 14 shows a partial section of a distal segment with an additional feature;

FIG. 15 shows simplified schematic of second embodiment of the deployment actuator showing complimentary distal and proximal springs;

FIG. 15A shows a portion of the actuator of FIG. 15;

FIG. 16A is a simplified schematic of the catheter;

FIG. 16B is a simplified schematic of the catheter;

FIG. 16C is a simplified schematic of the catheter; and,

FIG. 17 is a plot of force against displacement of several structures in the catheter.

DESCRIPTION OF THE INVENTION

FIG. 1 depicts the context of the invention. The figure shows a highly schematic view of the overall system that includes the physician, patient, catheters, and related electrophysiology equipment located within an operating room. The physician 16 introduces the catheter 10 into the vasculature of the patient 11 at the patient's leg and advances it along a blood vessel ultimately, entering the patient's heart 12. Other catheters that may be used in the procedure are represented by companion catheter 18. Each catheter is coupled to signal conditioning hardware 20 with appropriate catheter cabling typified by catheter cable 17. The signal, conditioning hardware 20 performs various interface functions applicable to the mapping, tracking, and registration procedures that are performed in conjunction with the workstation class computer-processing unit 24. If the companion catheter 18 is an ablation catheter, then conditioning hardware also forms an interface to an RF ablation unit (not illustrated). Three patent applications all published Dec. 27, 2007 are incorporated by reference herein to further explain the use of the catheter for non-contact mapping as follows: 20070299353; 20070299352 and 20070299351.

In use, the physician looks at a computer display 26. Present on the display is a substantial amount of information. A large window presents an image of the heart chamber 13 along with an image of the catheter 10. The physician will manipulate and control the catheter 10 based in part on the images and other data presented on the display 26. The image 27 seen in FIG. 1 is schematic and depicts the distal array of the catheter 10 deployed, occupying a small portion of the heart chamber 13 volume. The representation of the heart chamber 13 may use color, wire frame, or other techniques to depict the structure of the heart chamber 13 and to simultaneously portray electrical activity of the patient's heart. It is regarded as useful to display chamber geometry, catheter location, and electrical activity in an integrated fashion on the display 26. In use, the physician will observe the display 26 and interact with the workstation processing unit 24 and the catheters 10 and 18, to direct the therapy as a medical procedure.

FIG. 2 A through FIG. 2 C depicts array deployment and catheter articulation along with the associated positions of the handle controls. FIG. 2A shows the catheter 10 in isolation. The catheter 10 has an elongate body 31 with a distal end 37 and a proximal end 39. The elongate body 31 includes a tubular sheath 35. The proximal end 39 connects to an assembly that includes a handle segment 30. The physician may manipulate the handle segment 30 to selectively deflect, deploy, and rotate the catheter to perform the medical procedure. The handle segment 30 is coupled to an elongate intermediate section or segment 32. The intermediate section is coupled to a deflection segment 34, which in turn is coupled to a distal array segment 36, located at the distal tip or end 37. Not shown is the catheter cable 17 used

to connect the electrodes on the distal array segment 36 to the-Signal conditioning hardware 20. In FIG. 2A the catheter 10 is in the undeflected and undeployed state where the distal array segment 36 is collapsed and the deflection segment 34 is straight. In this configuration, the catheter is introduced into the body using the familiar Seldinger technique.

FIG. 2B shows the catheter 10 with the handle segment 30 manipulated to deploy the distal array segment 36 into the open or deployed state. In one embodiment, the pommel 33 of the handle assembly 30 is moved retrograde with respect to the handle assembly as indicated by motion arrow 38 to deploy the distal electrode array segment 36. In this embodiment, the pommel 33 will lock into position to deploy the array 36. To set the lock, the pommel 33 will have to be pulled enough to overcome a modest spring force to reach a detent position. When deployed, the distal array segment 36 opens to place electrodes into the operating position. In alternative embodiments the deployment control may be turned or rotated to deploy the electrode array.

FIG. 2C shows activation of the deflection segment 34. Antegrade motion of the handle ferrule 42 of the handle segment 30 depicted by motion arrow 40 deflects or articulates the deflection segment 34. Note that the catheter 10 responds to this motion and the deflection segment 34 forms an arc confined to a single plane. In the figure, the articulation or deflection motion lies in the plane of the page. The deflection operation causes the distal array segment 36 to be pointed up to 180° from the initial direction shown in panel 2A. The phantom dotted position seen in the figure shows that this articulation may be symmetrically “bi-directional.” It should also be understood that the articulation may also be asymmetrically bi-directional such that the arc shape is different in each direction. In one embodiment, best depicted in FIG. 15, articulation or deflection of the segment 34 moves a pull wire from the center axis of the catheter and it moves off to the side within the catheter body. This displacement of the pull wire reduces tension in the pull wire and leads to the deflection.

Thus it is shown that the catheter 10 has an elongate body 31 having a distal end 37, and a proximal end 39, and an elongate central axis. A proximal handle segment 30 having an articulation control 42 and a deployment control 33 are attached to the proximal end 39. There is an intermediate segment 32 connected to the handle and a deflectable segment 34 connected to the intermediate segment 32. The deflectable segment 34 will articulate in a plane through an angle in response to the articulation control. Also a distal array segment 36 is connected to the deflectable segment 34. This distal array segment 36 includes a deployable distal electrode array that can move from a first retracted position depicted in FIG. 2A to a second deployed position depicted in FIG. 2B. The deployment mechanism coupled to said deployment control couples the motion of the deployment control to operate the distal electrode array segment which causes the distal array segment to deploy into said second deployed position, independently of the operation of said articulation control.

The physician can rotate the handle segment 30 and operate ferrule 42 to position and “aim” the distal array segment 36 toward any part of the cardiac anatomy within the heart chamber. When deployed, the various splines typified by spline 50 carry various electrodes into specific highly stable and reproducible spatial locations.

FIG. 3A and FIG. 3B depict the distal array segment 36 in the deployed and undeployed states and serve to illustrate the location of the electrodes. FIG. 3A shows the distal array

segment 36 in isolation and in the retracted or undeployed 43 state or condition. The drawing shows a uniform and symmetrical distribution of the electrode sites as typified by electrode 54 along the length of a typical spline 50. It may be useful to place more of the sensing electrodes near the most distal end or tip 37 of the distal array segment 36. An asymmetrical electrode distribution may be advantageous for non-contact mapping functions. In addition to multiple sensing electrodes, current injecting locator electrodes, typified by locator electrode 55, may be placed at a location along the spline 50. In general it is preferred to position locator electrodes so that they are far apart in the deployed state. Current sourcing or sinking for the locator electrodes may also take place from ring electrodes 57 and tip electrode 53. Tip electrode 53 may also be provided for cardiac stimulation, ablation or as a locator electrode.

In summary, the splines 50 of the distal electrode array segment 36 may carry various sets of independent electrodes 54. Typically sixty-four sensing electrodes will be distributed over and along the various splines 50. Several locator electrodes may be positioned diametrically opposed to each other as illustrated by example, on the meridian of the deployed shape. Optionally other electrodes may occupy space in the distal electrode array. In use, sets of the electrodes are used at various times or concurrently during the medical procedure.

FIG. 3B shows the distal array segment 36 in the deployed state 41. Together FIGS. 3A and 3B show the motion of the several splines that make up the distal electrode array 36 as they move from the undeployed state 43 to the deployed state 41. While in the undeployed state 43, the splines lie together along side each other in a roughly tubular shape seen in FIG. 3A. The splines typified by spline 50 deflect and blossom moving outwardly in a radial direction as the array is deployed to the deployed state 41 as seen in FIG. 3B. This spline motion may be driven by a pull wire (FIG. 15 element 52) in a pull wire embodiment. Alternatively the spline motion may be driven by a rotating screw 153 that moves the screw driven pull member 159 seen within the array in FIGS. 10A and 10B. A rotatable member is used as a torque transmitting device from the handle to the screw member in the distal section. The rotatable member needs to be able to transfer torque while in a curved environment. The rotatable member can be implemented in the form of a torque transmitting wire, coil, braid reinforced plastic tube or laser cut hypotube. The term rotatable member is intended to describe all of these alternative constructions. This

In the pull wire embodiment, the pull wire 52 is pulled back into the catheter body of the deflectable segment 34 and the splines deform into a shape reminiscent of a bulb of garlic. The pommel control 33 and the proximal spring 402 are connected to the pull wire 52 and motion of the pommel control 33 moves the splines to the deployed state.

The individual splines may carry several types of electrodes. The array of sensing electrodes typified by spline electrode 54 are used for non-contact mapping and may also be used for assisting in the detection and location of companion catheters in the heart chamber. These non-contact electrodes are in the blood pool and they must receive and detect very small voltages to perform the mapping operation. Locator electrode 55 is typical of such a spline electrode used for location purposes (also shown in FIG. 3A). Typically locator electrodes will lie on the greatest meridian of the deployed array 41 so that once deployed they are quite far from each other as seen in FIG. 3B. However not every spline need carry a locator electrode.

Each electrode on a spline is electrically connected to the cabling in the handle. It is preferred that the signal from each individual electrode be independently available to the hardware interface 20. This may be achieved by passing a conductor for each electrode through the connection cable 17. As an alternative, the electrical connections may be multiplexed in the catheter device 10 to minimize conductors.

It is important that the high-density electrode array be deployed into a known, reproducible, and relatively stiff shape. The number of electrodes, their distribution and deployment shape, and stability in shape determine the limits of system performance. As electrode number and deployment volume increase, the performance is improved. However it is both difficult and important to balance complexity, cost, and performance with usability and patient benefit. An increase in electrode number and deployment size increases catheter 10 complexity and maneuverability of the catheter 10 is compromised. Experimental work suggests that a typical catheter 10 should have sixty-four sensing electrodes and deploy to a three dimensional somewhat spherical shape with a diameter of 18 mm. In order to know electrode locations for analysis by the processing unit 24, the deployment shape must be tightly controlled. Therefore, several critical design features must be tightly controlled. The location of the electrodes 54 within the array must be accurately placed. These electrodes 54 should also be placed in a manner that facilitates their use in close proximity to the endocardial surface when the array is deployed. This requirement may necessitate a non-uniform distribution of the electrodes 54 as certain regions of the deployed array are more likely to be positioned closely to the endocardium.

The deployed shape of the electrode array must be repeatable through multiple deployment cycles. For example, electrode locations need to be known to within 1 mm between multiple deployments. The array should be capable of deploying to a known shape and subsequently dosing to a low profile (e.g. 8 French) for retraction. This shape change may be binary or continuous, but in either situation, the shape must be repeatable and have a known geometry at the time of data collection. The repeatable shape requirement is applicable to the electrode array shape in both the circumferential and radial directions and represent a significant design challenges. The inventive combination of fabrication technology, structural design and material choices cooperate together to achieve the design goal.

Also seen in FIG. 3B is a locator sensor 59. There are several commercially available 3-D location systems available for use in medical devices. In general location of the locator sensor 59 in space is reported by a base station located near the patient. This technology is widely used in robotic surgery and need not be described in detail. Typically the locator sensor 59 would take the place of locator electrode 55.

FIG. 4A through FIG. 9D depict the formation of the array structure from a flexible printed circuit.

FIG. 4A shows a step in a preferred construction methodology for the distal array segment 36. The distal array segment 36 is manufactured in part from a flexible printed circuit 60 ("FPC"). This construction methodology has the advantage of repeatable high accuracy and low manufacturing cost. To construct the FPC 60, the material is initially fabricated in a planar form seen in FIG. 4A. In the planar condition, a series of apertures 62 are cut through the FPC 60 at one end typified by hole 62. Together the series of apertures 62 form a bonding band 70. At the opposite more

proximal end of the FPC 60 there is formed a termination band 106. The planar FPC 60 is also slit to free the individual splines. Conventional laser processing is well suited to this fabrication step.

FIG. 4B shows a process where the planar FPC 60 is wound around a major axis 61 bringing first edge 63 toward second edge 65.

FIG. 4C shows the two edges juxtaposed with both ends fixed. Together the bonding band 70 and the termination band or section 106 complete a cylindrical form. In general the distal bonding band 70 is fixed by encapsulation and the termination band is fixed by anchoring or bonding it to the deflection segment of the catheter.

FIG. 4D shows that with both ends fixed, the splines typified by spline 50 may be moved radially with respect to the axis 61.

FIG. 5A shows that the ring of apertures 62 that together from a bonding band 70. In the figure, the edges of the gap are seen in close proximity at reference numeral 72;

FIG. 5B shows the use of the bonding band 70. Note that the edges may be held together with a melted polymer or adhesive or other plastic or thermoplastic material that is applied to the interior and exterior of the tubular structure. This thermoplastic formed-in-place plug 74 encapsulates the inside and outside of the FPC 60 providing an unusually robust and durable structure that permits reliable deployment of the splines.

FIG. 6A shows the FPC 60 in plan view. This view reveals the several slits typified by slot or slit 108 which taken together form the individual splines such as spline 50. These slits 108 extend from the distal bonding section or band 70 to the termination section 106. Holes 62 appear in the bonding band 70 and additional slits 110 are formed within the termination section 106 to facilitate attachment to the deflectable section of the catheter.

The splines typified by spline 50 of the FPC 60 serve to position the electrodes typified by electrode 54 along the length of the FPC 60. The splines 50 also carry interconnecting metal traces (not shown) that serve to electrically connect the electrodes to pads in the termination section 106. The splines 50 are separated from each other using slits 108. The slits are thin gaps that are cut in the FPC using one of many cutting techniques that may include laser cutting, die cutting or chemical etching. The slits 108 of the exemplary FPC are cut using a laser so as, to position slit location precisely.

The distribution of the electrodes 54 may be tightly controlled in the design of the FPC 60. For example, in FIG. 6A we note that electrodes are distributed more densely in the distal tip area. It should be appreciated that any desirable electrode distribution may be accomplished using this method.

FIG. 6B shows the FPC 60 in cross-section. The various layers are not to scale. Some layers described are very thin while other thick, not all layers are depicted in the figure for clarity. In particular, very thin layers are not shown explicitly in the drawings. The FPC is constructed using a relatively thick core insulating layer 86. The core layer 86 of the exemplary circuit is constructed of a 50 um layer of polyimide. Alternative materials and thickness core layers may be used to obtain the desired mechanical and process characteristics. The core insulating layer 86 is coated with a top metallization layer 88 and a bottom metallization layer 90. Each of the exemplary metallization layers is deposited by first sputtering a thin layer (~0.1 um) of titanium over the core insulating layer 86. The titanium layer serves as an interface layer to adhere additional metallization to the core

insulating layer **86**. The metallization layers **88** and **90** can be added by further sputtering and/or plating of additional metal over the titanium layers. The exemplary metallization layers **88** and **90** are sputtered with a gold layer over the titanium layer and then further plated with gold until the total thickness of the metal layers measures 2 μm . It should be noted that other conductors such as copper may also be used. It is also necessary to provide electrical connection between metal layers **88** and **90** for the purpose of connecting circuit features that reside on each layer. A connection can be formed by constructing a via **96** between the two metallization layers. A via can be formed by creating a hole through both metallization layers **88** and **90** and the core insulating layer **86**. Electrical connection is then made by plating the walls of the hole between the two metallization layers forming a metal connection **96** between the metallization layers **88** and **90**. The FPC is further constructed by providing a top covercoat **92** over the top metallization layer **90**. The top covercoat **92** serves to insulate portions of the top metal layer **88** from external contact. The top covercoat has openings **98** placed in regions where it is desired to have the top metal layer exposed to external contact. For example a mapping electrode **54** may have the covercoat above it exposed and be sputtered or plated onto the top metal layer **88** as seen in FIG. 6B.

In the exemplary construction of FIG. 6B, the covercoat **92** of the FPC is formed by a 25 μm layer of liquid photoimageable polyimide. The photoimageable polyimide covercoat is exposed and developed to precisely locate geometric features on the exterior surface to create blood contacting electrodes, using similar registration and optical techniques used to fabricate other features on the FPC.

A bottom cover coat **100** is applied to the bottom metal layer **90** in order to insulate the bottom metal layer **90** from external contact. It may be necessary in some applications to enable the bottom covercoat **100** to have openings similar to the openings **98** of the top covercoat **92**. Such applications may require external contact to the bottom metal layer **90**. One important application for the mapping electrodes **54** is to sense low voltage biological signals. The biological signals of interest are generally in the tens of microvolts to several millivolt range in amplitude and are time varying in the frequency range of 0.05 Hz to several kHz. The detailed design of the Flexible Printed Circuit (FPC) layers and electrodes in particular impact the noise level of the measurement system. Reducing the impedance of the electrochemical interface between the electrode and blood reduces overall system noise.

Although a wide range of materials may be used to reduce impedance, our preferred electrode materials are selected from a small group which have demonstrated to us that they are especially well suited for this design. We prefer to select electrode materials for blood contact from the group of gold, stainless steel, platinum, platinum-iridium, titanium nitride, platinum black or iridium' oxide (in order of highest to lowest impedance). Electrode materials are applied using an electroplating or sputtering process.

At present our preferred FPC **60** and electrode construction includes an FPC with a polyimide core layer with gold metal layers. The blood contacting electrodes are gold coated with iridium oxide.

In addition to material properties, electrode area has a profound impact on impedance and in the design the electrode area may be increased to a width limited by the dimension of the spline and further limited by the presence of other metal features including traces.

It is also possible to increase the surface area of electrodes through surface finishing. Roughening of the electrode surface can be accomplished through anyone of several mechanical or chemical surface treatments.

FIG. 6B also shows that a stiffener layer **102** may be applied over the bottom covercoat **100** as seen in FIG. 6B. The stiffener layer **102** may have various thickness and material compositions in order to achieve the desired rigidity of the FPC in order to control the deployed shape. The exemplary FPC of the invention is comprised of a 50 μm thick polyimide stiffener **102** over the bottom covercoat **100**. It should be appreciated that other materials such as PEEK or Nitinol may be used as a stiffener. The stiffener **102** is adhered to the bottom covercoat using a polyimide adhesive layer. Other adhesives, and in particular, pressure sensitive adhesives may also be used for this purpose. Additional stiffener layers may be applied over stiffener layer **102**. Stiffener layer **120** serves to increase the stiffness of the circuit in selected areas.

The termination section **106** also serves to provide a region where the FPC may be bonded to the outer catheter shaft during installation.

FIG. 7 shows a metallization layer in plan view. The dark areas in FIG. 7 are the metallization traces created by the processes described in connection with FIG. 6A, but the core layer and other layers are not shown for clarity. Subpanels seen in the figure are enlargements of the metallization trace pattern to show various features. For example, the termination section **106** of the FPC of FIG. 6A is shown as traces **108** in this figure. The traces are metallic layers that serve to create a region where the FPC can be connected to wire or cabling that serve to electrically connect the FPC to circuitry or connectors in the proximal section of the catheter. The wire or cabling may be attached to the FPC at a series of termination lines as designated by reference numeral **112**.

It should be appreciated that a number of metallization layers ranging from 1 to 16 may be used. The addition of layers is helpful in carrying additional signals given a width constraint such as the spline width.

FIG. 8A shows how to increase the stiffness of the exemplary FPC of FIG. 6 forming areas of high stiffness **124** and areas of lower stiffness **126**.

FIG. 8B shows how to control the deployed shape of the array by controlling the stiffness of the exemplary FPC forming areas of high stiffness **124** and areas of lower stiffness **126**.

FIG. 8C shows a representative shape where stiff zones **124** or areas interspersed with less stiff areas **126** can create a complex array shape upon deployment. In the figure, there is more stress in the thin areas **126** which bend more readily than in the stiffer regions **124**.

FIG. 8D shows thicker regions with additional stiffener layers forming stiff zones **124** while less stiff material yields a less thick more flexible area **126**. The use of alternating stiffness areas helps to control the distribution of stress as well as determine deployed shape. In this embodiment the spline shape is segmented into relatively rigid "straight" sections **124** followed by "hinged" areas **126**. The detail drawing of FIG. 8E shows the high stiffness area **124** next to a lower stiffness area **126**.

FIG. 9A shows how to increase the stiffness of the exemplary FPC of FIG. 6 forming areas of high stiffness **124** and areas of lower stiffness **126** that are spaced along the spline.

FIG. 9B shows that a stiffener layer **102** may be applied over the bottom covercoat **100** as described in connection with FIG. 8B.

FIG. 9C shows a representative shape where stiff zones 124 or areas combined with less stiff areas 126 can create a complex array shape upon deployment. In the figure there is more stress in the thin areas that bend more readily than in the stiffer regions 124. Together the added material allows for a smoothly varying distribution of stress along the spline.

FIG. 9D shows thicker regions with additional stiffener layers forming stiff zones 124 while less stiffener material yields a less thick more flexible area 126. The use of alternating stiffness areas helps to control the distribution of stress as well as determine deployed shape yielding a continuously curved spline having a smoothly varying distribution of stress along the spline. The detail drawing in FIG. 9E shows a stiff area 124 next to a less stiff area 126.

Thus it is shown that distal deployable electrode array segment is formed from a multiple layer flexible printed circuit slit to form splines and rolled about said longitudinal central axis to form said distal electrode array. The slits may be wider or narrower along the length of the spline and this non-uniform shape characteristic results in control of the shape of the electrode array in the deployed position. It should also be appreciated that the stiffer elements along the splines also create a non-uniform shape characteristic that results in control of the final shape of the electrode array in the deployed position or state.

To provide the physician with visual feedback of the array state (deployed or undeployed), the array needs to be visible on fluoroscopy. This may be accomplished in several ways. The circuit may be made from and enhanced with an additional layer made from materials that are, in themselves, radiopaque such as gold, platinum, and/or tungsten, including others. Alternatively, a radiopaque substrate can be added to the array to enhance visualization upon deployment. This substrate can be in the form of marker bands, coiled wire, or radiopaque ink. In particular, the radiopaque ink may contain suspended tungsten that has radiopaque properties. This type of ink could be applied through a printing process on the undeployed electrode assembly while in the FPC configuration.

FIG. 11, FIG. 12, and FIG. 13 show differing strategies to reduce blood clotting on the array. It is conventional practice to administer anticoagulants to a patient undergoing these procedures. However is very useful to eliminate blood clotting on the catheter itself. FIG. 11, FIG. 12, and FIG. 13 show several techniques that may be adopted to achieve this goal. Continuous or episodic injection of saline or heparinized saline are contemplated with the embodiments of FIG. 11 and FIG. 12. It should be noted that various coating such as hydrophilic coatings, heparinized coatings, and parylene may also be applied to catheter surface alone or in combination with the techniques presented in the figures in order to reduce clot.

FIG. 11 shows a distal segment having a fluid supply lumen associated with the pull wire feature 52. Fluid 57 introduced into a hub at the proximal end of the catheter emerges from aperture 53 and aperture 55 to flood the array and prevent blood clots from adhering to the splines.

FIG. 12 shows a porous membrane associated with the pull wire feature location in the distal array segment to allow fluid introduced into the catheter under pressure to emerge from the porous sheath 200 and flood the array to prevent blood clots from adhering to the splines.

FIG. 13 shows a collapsible corrugated section 202 preventing blood from entering the catheter opening in the distal array structures

FIG. 14 shows a strategy for constraining the deployment providing tight control over the final shape of the deployed

array. For example tether 300 may emerge from the central shaft in FIG. 14 to restrain the motion of the splines or limbs.

As described previously, it is of great importance for the catheter to support controlled articulation while keeping the deployed shape known. FIG. 15 and FIG. 10 describe two different embodiments that meet this requirement. The mechanism in FIG. 15 relies on a spring to accomplish independence of the two mechanisms, while the mechanism of FIG. 10 relies on threads in distal array segment 36 to accomplish the same goals.

FIG. 15 is a simplified schematic diagram of the catheter that serves to describe the interaction between the articulation and deflection aspects of the catheter. The figure serves to explain the operation of one embodiment of the array deployment construction. In brief, the array is pulled open with a pull wire. The array is biased by a spring 400 to return to the undeployed state. The pull wire 52 extends from the handle 30 where it is anchored to a proximal spring. 402 to the distal tip 37 where it is anchored in the distal tip. The proximal spring 402 is in turn connected to the pommel or deployment control 33. As the deployment control 33 is retracted the pull wire pulls the distal tip 37 toward the handle 30. The tip motion is guided by tube 406 sliding over a bushing 408. This motion can continue until the tube bottoms out on surface 404. This mechanical stop determines the amount of shortening of the distal segment. As a consequence this stop also serves to limit the deployed state of the deployable array. In this figure the splines are not shown for clarity (for comparison see FIG. 16B). This motion also compresses the distal spring 400. If tension of the pull wire is eased then the distal spring 400 restores the array to the undeployed state.

The pull wire 5 and the proximal compensator spring 402 have a nominal length that gets longer or increases as the deployment control moves into the locked 30 position. The increase in length comes from the tension supplied to the spring that increases spring length. This process is seen clearly comparing FIG. 16A to FIG. 16B.

FIG. 16C corresponds to deflection or articulation of the catheter deflectable segment 34. The deflection control causes the catheter to deflect in the plane of the figure and this displaces the pull wire 52 within the elongate catheter body 32. As the pull wire moves from a concentric to an offset position within the body 34 the relative length of the pull wire compared to the length of the shaft changes. This is seen most clearly at reference numeral 410.

The proximal spring 402 compensates for and takes up this motion by contracting slightly while still providing enough tension in the pull wire to keep the distal array fully deployed.

FIG. 17 shows the interplay of tension in the pull wire and displacement of catheter components. As the control 33 is activated and moved toward the deployed condition, tension rises in the wire as seen at panel A. When the array is fully deployed the mechanical stop engages the proximal spring and force preferably remains constant as the control reaches the deployed state depicted in panel B. In this state, the catheter is in the state depicted in FIG. 16B. During deflection, as seen in FIG. 16C, the relative motion of the pull wire and its housing causes the spring tension to falloff in the proximal spring as seen in panel C to D, while the distal array remains against its stop. In this fashion, the distal spring and its mechanical stop cooperate with the proximal spring force to stabilize the array deployment during catheter deflection. FIG. 10A and FIG. 10B show an alternative embodiment for deploying the array of the catheter. In this embodiment a screw 153 is positioned in the distal segment

13

of the catheter. This screw **153** is rotated by a rotatable member or shaft **161** driven by a knob located in the handle which is not illustrated in the figures. The rotatable member **161** is keyed to the distal array segment **36** with the construction in section **155**. The construction provides the counter-force against which distal array segment **26** is deployed and retracted. This construction also isolates the screw **153** and prevents it from being influenced by tension in the rotatable member **161**. A complimentary nut forms a pull member **159** is free to slide over the stationary screw. The pull member **159** has an end anchored in the distal tip of the array and the traction supplied by the screw **153** causes the pull member **159** to move retrograde deploying the splines **50** of the array as seen in FIG. **10B**. This construction renders the deployment function independent of the articulation function of the catheter since the deployment function is unaffected by the tension on rotatable member **161**. In addition, this embodiment permits the array to deploy to known continuous intermediate states or positions between the fully retracted and fully deployed states. These continuous intermediate positions are useful in mapping operations where it is desirable to introduce the catheter into structures smaller than its fully deployed diameter while maintaining accurate knowledge of electrode locations. Electrode locations are determined from the amount of deployment which can be derived from the number of rotations employed by the rotatable member during deployment.

What is claimed is:

1. A catheter comprising:

an elongate catheter body having a distal end and a proximal end;

a proximal handle segment having deployment control, said proximal handle segment connected to said proximal end;

a distal array segment including a deployable electrode array, said distal array segment connected to said distal end;

a plurality of electrodes coupled to said distal array segment, the plurality of electrodes configured to be arranged in known spatial configurations including at least a retracted configuration and a deployed configuration; and

at least one set of current injecting locator electrodes situated on the greatest meridian of said deployable electrode array in said deployed configuration.

2. A catheter comprising:

an elongate catheter body having a distal end and a proximal end;

a proximal handle segment having an articulation control and a deployment control, said proximal handle segment connected to said proximal end;

an intermediate segment connected to said proximal handle segment;

a deflectable segment connected to said intermediate segment, said deflectable segment adapted to articulate in a plane through an angle in response to said articulation control;

a distal array segment connected to said deflectable segment, said distal array segment including a deployable electrode array configured to transition between a retracted position and at least one known deployed position that places multiple electrodes in known spatial configurations in response to said deployment control;

14

a plurality of locator electrodes situated on the greatest meridian of said deployable electrode array in said known deployed position; and

a deployment mechanism coupled to said deployment control for coupling motion of said deployment control to said deployable electrode array to cause the deployable electrode array to transition independently of the operation of said articulation control.

3. The catheter according to claim **2**, wherein said deployment mechanism comprises:

a pull wire anchored in the distal array segment and anchored to a spring in said proximal handle segment; said spring coupled to said deployment control, whereby actuation of said deployment control stretches said spring and increases a pull wire tension to a deployment tension value sufficient to cause said deployable electrode array to move to said at least one known deployed position; and

said articulation control reducing said pull wire tension while operating-to articulate said deflectable segment but not reducing said pull wire tension below said deployment tension value, thereby rendering deployment independent of articulation.

4. The catheter of claim **3**, further comprising:

a distal spring located in said distal array segment coupled to said deflectable segment biased to force said deployable electrode array into the retracted position when the pull wire tension drops below a deployment tension value as the pull wire tension is relaxed with said deployment control.

5. A catheter according to claim **2** wherein said deployment mechanism comprises:

an elongate rotatable member coupled to said deployment control; a first threaded member anchored in said distal array segment;

a second threaded member coupled to said elongate rotatable member;

said first and second threaded members adapted for engagement by rotation of said rotatable member;

wherein the relative position of said second threaded member and said first threaded member determines a deployment position of said deployable electrode array; whereby changes in rotatable member tension do not alter the relative position of said first and second members thereby rendering deployment independent of articulation.

6. The catheter of claim **2**, further comprising:

a tracking sensor that is part of said distal array segment.

7. The catheter of claim **2**, further comprising:

a set of current injecting tracking electrodes located in said distal array segment.

8. The catheter according to claim **2**, further including:

an articulation mechanism coupled to said articulation control for coupling motion of said articulation control to said deflectable segment to cause the deflectable segment to symmetrically and bi-directionally articulate in said plane through said angle.

9. The catheter according to claim **2**, further including:

an articulation mechanism coupled to said articulation control for coupling motion of said articulation control to said deflectable segment to cause the deflectable segment to asymmetrically and bi-directionally articulate in said plane through said angle.

10. The catheter of claim **2**, wherein the deployable electrode array has at least a first region having a first stiffness and a second region having a second stiffness.

15

11. A catheter comprising:
 an elongate catheter body having a distal end and a proximal end;
 a proximal handle segment having an articulation control and a deployment control, said proximal handle segment connected to said proximal end;
 an intermediate segment connected to said proximal handle segment;
 a deflectable segment connected to said intermediate segment, said deflectable segment adapted to articulate in a plane through an angle in response to said articulation control; and
 a distal array segment connected to said deflectable segment, said distal array segment including a deployable electrode array that can move from a retracted position to at least one known deployed position, said deployable electrode array formed from a flexible printed circuit slit to form splines and rolled about a major axis to form a tubular shape, at least one of the splines including a first segment having a first stiffness and a second segment having a second stiffness,
 wherein said deployable electrode array has a plurality of bonding apertures at an end of the deployable electrode array and thermoplastic material is positioned on an

16

exterior and an interior of said tubular shape and extends through the plurality of bonding apertures to retain said tubular shape.
 12. The catheter according to claim 11, wherein:
 each spline in said deployable electrode array has a non-uniform shape characteristic resulting in control of the shape of the deployable electrode array in the known deployed position.
 13. The catheter according to claim 11, wherein:
 said deployable electrode array has a uniform and symmetrical distribution of electrodes in the array.
 14. The catheter according to claim 11, wherein:
 said deployable electrode array is formed from said flexible printed circuit with electrode material selected from a group consisting of: gold, stainless steel, platinum, platinum-iridium, titanium nitride, platinum black and iridium-oxide.
 15. The catheter of claim 11, further comprising:
 a fluid delivery lumen to flood the distal array segment with a fluid injected into the catheter.
 16. The catheter of claim 11, further comprising:
 a radio-opaque pattern applied to the distal array segment such that the pattern changes during deployment to provide a discernable radiographic image to confirm deployment.

* * * * *

专利名称(译)	心脏标测导管		
公开(公告)号	US10034637	公开(公告)日	2018-07-31
申请号	US14/277122	申请日	2014-05-14
[标]申请(专利权)人(译)	里斯米亚医疗公司		
申请(专利权)人(译)	RHYTHMIA MEDICAL , INC.		
当前申请(专利权)人(译)	BOSTON SCIENTIFIC SCIMED , INC.		
[标]发明人	HARLEV DORON CALLAWAY JUSTIN		
发明人	HARLEV, DORON CALLAWAY, JUSTIN		
IPC分类号	A61B5/0402 A61M25/00 A61B5/042 A61B5/00 A61M25/01 A61B18/00 A61B18/14		
CPC分类号	A61B5/6852 A61B5/042 A61B5/0422 A61B5/6859 A61M25/0015 A61M25/0147 Y10T29/49117 A61B2018/00214 A61B2018/00351 A61B2018/00839 A61B2018/00898 A61M2025/0161 A61B18/1492 A61B5/6858 A61B34/20 A61B2034/2053		
代理机构(译)	FAEGRE BAKER丹尼尔斯律师事务所		
优先权	13/289367 2013-05-21 US		
其他公开文献	US20140275921A1		
外部链接	Espacenet		

摘要(译)

一种用于心脏的非接触式绘图的多电极导管，具有独立的关节和展开特征。

