



US010194846B2

(12) **United States Patent**
Fennell

(10) **Patent No.:** **US 10,194,846 B2**
(45) **Date of Patent:** ***Feb. 5, 2019**

(54) **METHOD AND APPARATUS FOR PROVIDING DYNAMIC MULTI-STAGE SIGNAL AMPLIFICATION IN A MEDICAL DEVICE**

(71) Applicant: **Abbott Diabetes Care Inc.**, Alameda, CA (US)

(72) Inventor: **Martin J. Fennell**, Concord, CA (US)

(73) Assignee: **Abbott Diabetes Care Inc.**, Alameda, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **15/686,156**

(22) Filed: **Aug. 25, 2017**

(65) **Prior Publication Data**

US 2017/0354356 A1 Dec. 14, 2017

Related U.S. Application Data

(63) Continuation of application No. 15/209,741, filed on Jul. 13, 2016, now Pat. No. 9,743,866, which is a continuation of application No. 14/596,759, filed on Jan. 14, 2015, now Pat. No. 9,402,584, which is a continuation of application No. 14/188,659, filed on (Continued)

(51) **Int. Cl.**

A61B 5/145 (2006.01)
A61B 5/00 (2006.01)
A61B 5/1486 (2006.01)
A61M 5/172 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/14532** (2013.01); **A61B 5/002** (2013.01); **A61B 5/0004** (2013.01); **A61B 5/14546** (2013.01); **A61B 5/14865** (2013.01); **A61B 5/7225** (2013.01); **A61B 5/7246** (2013.01); **A61B 5/7475** (2013.01); **A61M 5/1723** (2013.01); **A61B 2560/0209** (2013.01); (Continued)

(58) **Field of Classification Search**

CPC **A61B 5/14532**; **A61B 5/14546**; **A61B 5/14865**; **A61B 5/7475**; **A61B 5/002**; **A61B 5/0004**; **A61B 5/7225**; **A61B 5/7246**; **A61M 5/1723**
USPC 340/511
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,260,656 A 7/1966 Ross, Jr.
3,581,062 A 5/1971 Aston
(Continued)

FOREIGN PATENT DOCUMENTS

EP 0098592 1/1984
EP 0127958 12/1984
(Continued)

OTHER PUBLICATIONS

Armour, J. C., et al., "Application of Chronic Intravascular Blood Glucose Sensor in Dogs", *Diabetes*, vol. 39, 1990, pp. 1519-1526.
(Continued)


Primary Examiner — John A Tweel, Jr.

(74) *Attorney, Agent, or Firm* — Jackson & Co., LLP

(57) **ABSTRACT**

Methods and apparatus for providing multi-stage signal amplification in a medical telemetry system are provided.

20 Claims, 4 Drawing Sheets

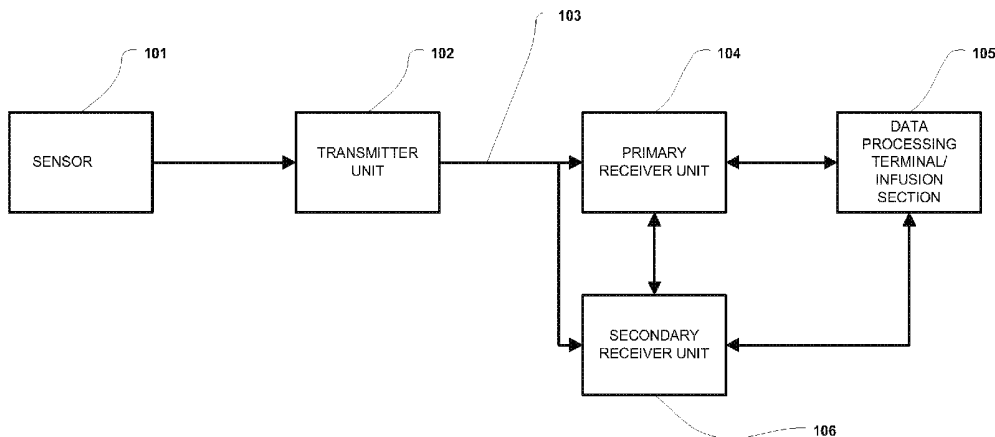

Related U.S. Application Data

- Feb. 24, 2014, now Pat. No. 8,937,540, which is a continuation of application No. 13/867,948, filed on Apr. 22, 2013, now Pat. No. 8,698,615, which is a continuation of application No. 13/437,894, filed on Apr. 2, 2012, now Pat. No. 8,427,298, which is a continuation of application No. 13/114,029, filed on May 23, 2011, now Pat. No. 8,149,103, which is a continuation of application No. 12/849,004, filed on Aug. 2, 2010, now Pat. No. 7,948,369, which is a continuation of application No. 12/102,836, filed on Apr. 14, 2008, now Pat. No. 7,768,387.
- (60) Provisional application No. 60/911,866, filed on Apr. 14, 2007.
- (52) **U.S. Cl.**
CPC . *A61B 2560/0252* (2013.01); *A61B 2560/045* (2013.01)

(56) References Cited

U.S. PATENT DOCUMENTS

3,926,760 A	12/1975	Allen et al.	5,264,105 A	11/1993	Gregg et al.
3,949,388 A	4/1976	Fuller	5,279,294 A	1/1994	Anderson et al.
4,031,449 A	6/1977	Trombly	5,285,792 A	2/1994	Sjoquist et al.
4,036,749 A	7/1977	Anderson	5,293,877 A	3/1994	O'Hara et al.
4,055,175 A	10/1977	Clemens et al.	5,299,571 A	4/1994	Mastrototaro
4,129,128 A	12/1978	McFarlane	5,320,725 A	6/1994	Gregg et al.
4,245,634 A	1/1981	Albisser et al.	5,322,063 A	6/1994	Allen et al.
4,327,725 A	5/1982	Cortese et al.	5,340,722 A	8/1994	Wolfbeis et al.
4,344,438 A	8/1982	Schultz	5,342,789 A	8/1994	Chick et al.
4,349,728 A	9/1982	Phillips et al.	5,356,786 A	10/1994	Heller et al.
4,425,920 A	1/1984	Bourland et al.	5,360,404 A	11/1994	Novacek et al.
4,445,090 A	4/1984	Melocik et al.	5,371,787 A	12/1994	Hamilton
4,464,170 A	8/1984	Clemens et al.	5,372,427 A	12/1994	Padovani et al.
4,478,976 A	10/1984	Goertz et al.	5,379,238 A	1/1995	Stark
4,494,950 A	1/1985	Fischell	5,390,671 A	2/1995	Lord et al.
4,509,531 A	4/1985	Ward	5,391,250 A	2/1995	Cheney, II et al.
4,527,240 A	7/1985	Kvitash	5,408,999 A	4/1995	Singh et al.
4,538,616 A	9/1985	Rogoff	5,411,647 A	5/1995	Johnson et al.
4,583,035 A	4/1986	Sloan	5,425,868 A	6/1995	Pedersen
4,619,793 A	10/1986	Lee	5,429,602 A	7/1995	Hauser
4,671,288 A	6/1987	Gough	5,431,160 A	7/1995	Wilkins
4,703,756 A	11/1987	Gough et al.	5,431,921 A	7/1995	Thombre
4,731,726 A	3/1988	Allen, III	5,438,271 A	8/1995	White et al.
4,749,985 A	6/1988	Corsberg	5,438,983 A	8/1995	Falcone
4,757,022 A	7/1988	Shults et al.	5,462,051 A	10/1995	Oka et al.
4,777,953 A	10/1988	Ash et al.	5,462,645 A	10/1995	Albery et al.
4,779,618 A	10/1988	Mund et al.	5,497,772 A	3/1996	Schulman et al.
4,847,785 A	7/1989	Stephens	5,507,288 A	4/1996	Bocker et al.
4,854,322 A	8/1989	Ash et al.	5,509,410 A	4/1996	Hill et al.
4,890,620 A	1/1990	Gough	5,514,718 A	5/1996	Lewis et al.
4,925,268 A	5/1990	Iyer et al.	5,531,878 A	7/1996	Vadgama et al.
4,953,552 A	9/1990	DeMarzo	5,558,638 A	9/1996	Evers et al.
4,986,271 A	1/1991	Wilkins	5,568,806 A	10/1996	Cheney, II et al.
4,995,402 A	2/1991	Smith et al.	5,569,186 A	10/1996	Lord et al.
5,000,180 A	3/1991	Kuypers et al.	5,582,184 A	12/1996	Erickson et al.
5,002,054 A	3/1991	Ash et al.	5,586,553 A	12/1996	Halili et al.
5,019,974 A	5/1991	Beckers	5,593,852 A	1/1997	Heller et al.
5,050,612 A	9/1991	Matsumura	5,609,575 A	3/1997	Larson et al.
5,055,171 A	10/1991	Peck	5,628,310 A	5/1997	Rao et al.
5,061,941 A	10/1991	Lizzi et al.	5,628,324 A	5/1997	Sarbach
5,068,536 A	11/1991	Rosenthal	5,653,239 A	8/1997	Pompei et al.
5,082,550 A	1/1992	Rishpon et al.	5,665,222 A	9/1997	Heller et al.
5,106,365 A	4/1992	Hernandez	5,711,001 A	1/1998	Bussan et al.
5,112,455 A	5/1992	Cozzette et al.	5,711,861 A	1/1998	Ward et al.
5,122,925 A	6/1992	Inpyun	5,726,646 A	3/1998	Bane et al.
5,135,004 A	8/1992	Adams et al.	5,729,225 A	3/1998	Ledzius
5,165,407 A	11/1992	Wilson et al.	5,733,313 A	3/1998	Barreras, Sr. et al.
5,246,867 A	9/1993	Lakowicz et al.	5,769,873 A	6/1998	Zadeh
5,262,035 A	11/1993	Gregg et al.	5,772,586 A	6/1998	Heinonen et al.
5,262,305 A	11/1993	Heller et al.	5,791,344 A	8/1998	Schulman et al.
5,264,104 A	11/1993	Gregg et al.	5,830,129 A	11/1998	Baer et al.
			5,830,132 A	11/1998	Robinson
			5,856,758 A	1/1999	Joffe et al.
			5,899,855 A	5/1999	Brown
			5,919,141 A	7/1999	Money et al.
			5,925,021 A	7/1999	Castellano et al.
			5,935,224 A	8/1999	Svancarek et al.
			5,942,979 A	8/1999	Luppino
			5,957,854 A	9/1999	Besson et al.
			5,964,993 A	10/1999	Blubaugh, Jr. et al.
			5,965,380 A	10/1999	Heller et al.
			5,971,922 A	10/1999	Arita et al.
			5,995,860 A	11/1999	Sun et al.
			6,001,067 A	12/1999	Shults et al.
			6,024,699 A	2/2000	Surwit et al.
			6,028,413 A	2/2000	Brockmann
			6,049,727 A	4/2000	Crothall
			6,055,316 A	4/2000	Perlman et al.
			6,066,448 A	5/2000	Wohlstadter et al.
			6,083,710 A	7/2000	Heller et al.
			6,084,523 A	7/2000	Gelnovatch et al.
			6,088,608 A	7/2000	Schulman et al.
			6,091,976 A	7/2000	Pfeiffer et al.
			6,093,172 A	7/2000	Funderburk et al.
			6,096,364 A	8/2000	Bok et al.
			6,103,033 A	8/2000	Say et al.
			6,117,290 A	9/2000	Say et al.
			6,119,028 A	9/2000	Schulman et al.
			6,120,676 A	9/2000	Heller et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,121,009	A	9/2000	Heller et al.	6,692,446	B2	2/2004	Hoek
6,121,611	A	9/2000	Lindsay et al.	6,694,191	B2	2/2004	Starkweather et al.
6,122,351	A	9/2000	Schlueter, Jr. et al.	6,695,860	B1	2/2004	Ward et al.
6,134,461	A	10/2000	Say et al.	6,698,269	B2	3/2004	Baber et al.
6,151,517	A	11/2000	Honigs et al.	6,702,857	B2	3/2004	Brauker et al.
6,162,611	A	12/2000	Heller et al.	6,730,025	B1	5/2004	Platt
6,175,752	B1	1/2001	Say et al.	6,733,446	B2	5/2004	Lebel et al.
6,200,265	B1	3/2001	Walsh et al.	6,740,075	B2	5/2004	Lebel et al.
6,212,416	B1	4/2001	Ward et al.	6,741,877	B1	5/2004	Shults et al.
6,218,809	B1	4/2001	Downs et al.	6,746,582	B2	6/2004	Heller et al.
6,219,574	B1	4/2001	Cormier et al.	6,758,810	B2	7/2004	Lebel et al.
6,233,471	B1	5/2001	Berner et al.	6,770,030	B1	8/2004	Schaupp et al.
6,248,067	B1	6/2001	Causey, III et al.	6,790,178	B1	9/2004	Mault et al.
6,270,455	B1	8/2001	Brown	6,809,653	B1	10/2004	Mann et al.
6,275,717	B1	8/2001	Gross et al.	6,810,290	B2	10/2004	Lebel et al.
6,284,478	B1	9/2001	Heller et al.	6,811,533	B2	11/2004	Lebel et al.
6,293,925	B1	9/2001	Safabash et al.	6,811,534	B2	11/2004	Bowman, IV et al.
6,295,506	B1	9/2001	Heinonen et al.	6,813,519	B2	11/2004	Lebel et al.
6,299,347	B1	10/2001	Pompei	6,862,465	B2	3/2005	Shults et al.
6,306,104	B1	10/2001	Cunningham et al.	6,873,268	B2	3/2005	Lebel et al.
6,309,884	B1	10/2001	Cooper et al.	6,881,551	B2	4/2005	Heller et al.
6,314,317	B1	11/2001	Willis	6,892,085	B2	5/2005	Mclvor et al.
6,329,161	B1	12/2001	Heller et al.	6,893,396	B2	5/2005	Schulze et al.
6,359,270	B1	3/2002	Bridson	6,895,263	B2	5/2005	Shin et al.
6,359,594	B1	3/2002	Junod	6,895,265	B2	5/2005	Silver
6,360,888	B1	3/2002	Mclvor et al.	6,926,670	B2	8/2005	Rich et al.
6,366,794	B1	4/2002	Moussy et al.	6,931,327	B2	8/2005	Goode, Jr. et al.
6,377,828	B1	4/2002	Chaiken et al.	6,932,894	B2	8/2005	Mao et al.
6,379,301	B1	4/2002	Worthington et al.	6,936,006	B2	8/2005	Sabra
6,385,473	B1	5/2002	Haines et al.	6,950,708	B2	9/2005	Bowman, IV et al.
6,424,847	B1	7/2002	Mastrototaro et al.	6,958,705	B2	10/2005	Lebel et al.
6,427,088	B1	7/2002	Bowman, IV et al.	6,968,294	B2	11/2005	Gutta et al.
6,440,068	B1	8/2002	Brown et al.	6,971,274	B2	12/2005	Olin
6,471,689	B1	10/2002	Joseph et al.	6,974,437	B2	12/2005	Lebel et al.
6,478,736	B1	11/2002	Mault	6,983,176	B2	1/2006	Gardner et al.
6,480,744	B2	11/2002	Ferek-Petric	6,987,474	B2	1/2006	Freeman et al.
6,484,046	B1	11/2002	Say et al.	6,990,317	B2	1/2006	Arnold
6,493,069	B1	12/2002	Nagashimada et al.	6,990,366	B2	1/2006	Say et al.
6,514,718	B2	2/2003	Heller et al.	6,997,907	B2	2/2006	Safabash et al.
6,533,733	B1	3/2003	Ericson et al.	6,998,247	B2	2/2006	Monfre et al.
6,544,212	B2	4/2003	Galley et al.	7,003,336	B2	2/2006	Holker et al.
6,546,268	B1	4/2003	Ishikawa et al.	7,003,340	B2	2/2006	Say et al.
6,551,494	B1	4/2003	Heller et al.	7,003,341	B2	2/2006	Say et al.
6,558,321	B1	5/2003	Burd et al.	7,022,072	B2	4/2006	Fox et al.
6,558,351	B1	5/2003	Steil et al.	7,024,245	B2	4/2006	Lebel et al.
6,560,471	B1	5/2003	Heller et al.	7,027,621	B1	4/2006	Prokoski
6,561,978	B1	5/2003	Conn et al.	7,027,931	B1	4/2006	Jones et al.
6,562,001	B2	5/2003	Lebel et al.	7,029,444	B2	4/2006	Shin et al.
6,564,105	B2	5/2003	Starkweather et al.	7,041,068	B2	5/2006	Freeman et al.
6,565,509	B1	5/2003	Say et al.	7,052,483	B2	5/2006	Wojcik
6,571,128	B2	5/2003	Lebel et al.	7,056,302	B2	6/2006	Douglas
6,572,545	B2	6/2003	Knobbe et al.	7,068,227	B2	6/2006	Ying
6,576,101	B1	6/2003	Heller et al.	7,074,307	B2	7/2006	Simpson et al.
6,577,899	B2	6/2003	Lebel et al.	7,081,195	B2	7/2006	Simpson et al.
6,579,690	B1	6/2003	Bonnecaze et al.	7,098,803	B2	8/2006	Mann et al.
6,580,364	B1	6/2003	Munch et al.	7,108,778	B2	9/2006	Simpson et al.
6,585,644	B2	7/2003	Lebel et al.	7,110,803	B2	9/2006	Shults et al.
6,591,125	B1	7/2003	Buse et al.	7,113,821	B1	9/2006	Sun et al.
6,595,919	B2	7/2003	Berner et al.	7,134,999	B2	11/2006	Brauker et al.
6,599,243	B2	7/2003	Woltermann et al.	7,136,689	B2	11/2006	Shults et al.
6,605,200	B1	8/2003	Mao et al.	7,167,818	B2	1/2007	Brown
6,605,201	B1	8/2003	Mao et al.	7,171,274	B2	1/2007	Starkweather et al.
6,607,509	B2	8/2003	Bobroff et al.	7,174,199	B2	2/2007	Berner et al.
6,610,012	B2	8/2003	Mault	7,181,505	B2	2/2007	Haller et al.
6,633,772	B2	10/2003	Ford et al.	7,190,988	B2	3/2007	Say et al.
6,635,014	B2	10/2003	Starkweather et al.	7,192,450	B2	3/2007	Brauker et al.
6,645,368	B1	11/2003	Beaty et al.	7,198,606	B2	4/2007	Boecker et al.
6,648,821	B2	11/2003	Lebel et al.	7,222,054	B2	5/2007	Geva
6,654,625	B1	11/2003	Say et al.	7,226,978	B2	6/2007	Tapsak et al.
6,656,114	B1	12/2003	Poulson et al.	7,258,665	B2	8/2007	Kohls et al.
6,658,396	B1	12/2003	Tang et al.	7,267,665	B2	9/2007	Steil et al.
6,659,948	B2	12/2003	Lebel et al.	7,276,029	B2	10/2007	Goode, Jr. et al.
6,668,196	B1	12/2003	Villegas et al.	7,286,894	B1	10/2007	Grant et al.
6,687,546	B2	2/2004	Lebel et al.	7,299,082	B2	11/2007	Feldman et al.
6,689,056	B1	2/2004	Kilcoyne et al.	7,310,544	B2	12/2007	Brister et al.
				7,335,294	B2	2/2008	Heller et al.
				7,354,420	B2	4/2008	Steil et al.
				7,364,592	B2	4/2008	Carr-Brendel et al.
				7,366,556	B2	4/2008	Brister et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,379,765 B2	5/2008	Petisce et al.	2003/0032874 A1	2/2003	Rhodes et al.
7,402,153 B2	7/2008	Steil et al.	2003/0035371 A1	2/2003	Reed et al.
7,424,318 B2	9/2008	Brister et al.	2003/0042137 A1	3/2003	Mao et al.
7,460,898 B2	12/2008	Brister et al.	2003/0060689 A1	3/2003	Kohls et al.
7,467,003 B2	12/2008	Brister et al.	2003/0060692 A1	3/2003	Ruchti et al.
7,471,972 B2	12/2008	Rhodes et al.	2003/0060753 A1	3/2003	Starkweather et al.
7,494,465 B2	2/2009	Brister et al.	2003/0065308 A1	4/2003	Lebel et al.
7,497,827 B2	3/2009	Brister et al.	2003/0100821 A1	5/2003	Heller et al.
7,506,046 B2	3/2009	Rhodes	2003/0119457 A1	6/2003	Standke
7,519,408 B2	4/2009	Rasdal et al.	2003/0125612 A1	7/2003	Fox et al.
7,547,281 B2	6/2009	Hayes et al.	2003/0130616 A1	7/2003	Steil et al.
7,569,030 B2	8/2009	Lebel et al.	2003/0134347 A1	7/2003	Heller et al.
7,583,990 B2	9/2009	Goode, Jr. et al.	2003/0144581 A1	7/2003	Conn et al.
7,591,801 B2	9/2009	Brauker et al.	2003/0168338 A1	9/2003	Gao et al.
7,599,726 B2	10/2009	Goode, Jr. et al.	2003/0175992 A1	9/2003	Toranto et al.
7,613,491 B2	11/2009	Boock et al.	2003/0176933 A1	9/2003	Lebel et al.
7,615,007 B2	11/2009	Shults et al.	2003/0179705 A1	9/2003	Kojima
7,618,369 B2	11/2009	Hayter et al.	2003/0187338 A1	10/2003	Say et al.
7,632,228 B2	12/2009	Brauker et al.	2003/0199790 A1	10/2003	Boecker et al.
7,653,425 B2	1/2010	Hayter et al.	2003/0208113 A1	11/2003	Mault et al.
7,699,775 B2	4/2010	Desai et al.	2003/0212317 A1	11/2003	Kovatchev et al.
7,766,829 B2	8/2010	Sloan et al.	2003/0212379 A1	11/2003	Bylund et al.
7,768,387 B2	8/2010	Fennell et al.	2003/0216630 A1	11/2003	Jersey-Willuhn et al.
7,775,444 B2	8/2010	DeRocco et al.	2003/0217966 A1	11/2003	Tapsak et al.
7,804,197 B2	9/2010	Iisaka et al.	2004/0010207 A1	1/2004	Flaherty et al.
7,811,231 B2	10/2010	Jin et al.	2004/0011671 A1	1/2004	Shults et al.
7,826,382 B2	11/2010	Sicurello et al.	2004/0030581 A1	2/2004	Levin et al.
7,833,151 B2	11/2010	Khait et al.	2004/0034289 A1	2/2004	Teller et al.
7,889,069 B2	2/2011	Fifolt et al.	2004/0039255 A1	2/2004	Simonsen et al.
7,948,369 B2	5/2011	Fennell et al.	2004/0039298 A1	2/2004	Abreu et al.
7,978,063 B2	7/2011	Baldus et al.	2004/0040840 A1	3/2004	Mao et al.
8,000,918 B2	8/2011	Fjield et al.	2004/0045879 A1	3/2004	Shults et al.
8,010,174 B2	8/2011	Goode et al.	2004/0063435 A1	4/2004	Sakamoto et al.
8,010,256 B2	8/2011	Oowada	2004/0064068 A1	4/2004	DeNuzzio et al.
8,123,686 B2	2/2012	Fennell et al.	2004/0106858 A1	6/2004	Say et al.
8,149,103 B2	4/2012	Fennell et al.	2004/0106859 A1	6/2004	Say et al.
8,233,456 B1	7/2012	Kopikare et al.	2004/0116786 A1	6/2004	Iijima et al.
8,260,393 B2	9/2012	Kamath et al.	2004/0122353 A1	6/2004	Shahmirian et al.
8,282,549 B2	10/2012	Brauker et al.	2004/0128161 A1	7/2004	Mazar et al.
8,417,312 B2	4/2013	Kamath et al.	2004/0133164 A1	7/2004	Funderburk et al.
8,427,298 B2	4/2013	Fennell et al.	2004/0133390 A1	7/2004	Osorio et al.
8,478,389 B1	7/2013	Brockway et al.	2004/0136361 A1	7/2004	Holloway et al.
8,560,037 B2	10/2013	Goode, Jr. et al.	2004/0136377 A1	7/2004	Miyazaki et al.
8,622,903 B2	1/2014	Jin et al.	2004/0138588 A1	7/2004	Saikley et al.
8,638,411 B2	1/2014	Park et al.	2004/0146909 A1	7/2004	Duong et al.
8,698,615 B2	4/2014	Fennell et al.	2004/0147872 A1	7/2004	Thompson
8,849,459 B2	9/2014	Ramey et al.	2004/0152622 A1	8/2004	Keith et al.
8,914,090 B2	12/2014	Jain et al.	2004/0167801 A1	8/2004	Say et al.
8,937,540 B2	1/2015	Fennell	2004/0171921 A1	9/2004	Say et al.
9,402,584 B2	8/2016	Fennell	2004/0176672 A1	9/2004	Silver et al.
9,743,866 B2*	8/2017	Fennell A61B 5/14532	2004/0186362 A1	9/2004	Brauker et al.
9,801,545 B2	10/2017	Fennell et al.	2004/0186365 A1	9/2004	Jin et al.
2001/0011795 A1	8/2001	Ohtsuka et al.	2004/0193020 A1	9/2004	Chiba et al.
2002/0019022 A1	2/2002	Dunn et al.	2004/0193025 A1	9/2004	Steil et al.
2002/0023852 A1	2/2002	McIvor et al.	2004/0193090 A1	9/2004	Lebel et al.
2002/0026111 A1	2/2002	Ackerman	2004/0197846 A1	10/2004	Hockersmith et al.
2002/0042090 A1	4/2002	Heller et al.	2004/0199056 A1	10/2004	Husemann et al.
2002/0045808 A1	4/2002	Ford et al.	2004/0199059 A1	10/2004	Brauker et al.
2002/0046300 A1	4/2002	Hanko et al.	2004/0204055 A1	10/2004	Nousiainen
2002/0065454 A1	5/2002	Lebel et al.	2004/0204687 A1	10/2004	Mogensen et al.
2002/0085719 A1	7/2002	Crosbie	2004/0204868 A1	10/2004	Maynard et al.
2002/0099854 A1	7/2002	Jorgensen	2004/0206916 A1	10/2004	Colvin, Jr. et al.
2002/0103499 A1	8/2002	Perez et al.	2004/0212536 A1	10/2004	Mori et al.
2002/0106709 A1	8/2002	Potts et al.	2004/0225199 A1	11/2004	Evanyk et al.
2002/0109621 A1	8/2002	Khair et al.	2004/0225338 A1	11/2004	Lebel et al.
2002/0117639 A1	8/2002	Paolini et al.	2004/0236200 A1	11/2004	Say et al.
2002/0128594 A1	9/2002	Das et al.	2004/0254433 A1	12/2004	Bandis et al.
2002/0161288 A1	10/2002	Shin et al.	2004/0260478 A1	12/2004	Schwamm
2002/0169635 A1	11/2002	Shillingburg	2004/0267300 A1	12/2004	Mace
2002/0173830 A1	11/2002	Starkweather et al.	2005/0001024 A1	1/2005	Kusaka et al.
2002/0185130 A1	12/2002	Wright et al.	2005/0004439 A1	1/2005	Shin et al.
2002/0188748 A1	12/2002	Blackwell et al.	2005/0004494 A1	1/2005	Perez et al.
2003/0004403 A1	1/2003	Drinan et al.	2005/0010269 A1	1/2005	Lebel et al.
2003/0009203 A1	1/2003	Lebel et al.	2005/0017864 A1	1/2005	Tsoukalis
2003/0023317 A1	1/2003	Brauker et al.	2005/0027177 A1	2/2005	Shin et al.
			2005/0031689 A1	2/2005	Shults et al.
			2005/0038332 A1	2/2005	Saidara et al.
			2005/0043598 A1	2/2005	Goode, Jr. et al.
			2005/0049179 A1	3/2005	Davidson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2005/0059372	A1	3/2005	Arayashiki et al.	2006/0247508	A1	11/2006	Fennell
2005/0070777	A1	3/2005	Cho et al.	2006/0253296	A1	11/2006	Liisberg et al.
2005/0090607	A1	4/2005	Tapsak et al.	2006/0264785	A1	11/2006	Dring et al.
2005/0096511	A1	5/2005	Fox et al.	2006/0264888	A1	11/2006	Moberg et al.
2005/0096512	A1	5/2005	Fox et al.	2006/0270922	A1	11/2006	Brauker et al.
2005/0096516	A1	5/2005	Soykan et al.	2006/0272652	A1	12/2006	Stocker et al.
2005/0112169	A1	5/2005	Brauker et al.	2006/0276714	A1	12/2006	Holt et al.
2005/0113648	A1	5/2005	Yang et al.	2006/0293607	A1	12/2006	Alt et al.
2005/0116683	A1	6/2005	Cheng et al.	2007/0007133	A1	1/2007	Mang et al.
2005/0121322	A1	6/2005	Say et al.	2007/0016381	A1	1/2007	Kamath et al.
2005/0131346	A1	6/2005	Douglas	2007/0017983	A1	1/2007	Frank et al.
2005/0137530	A1	6/2005	Campbell et al.	2007/0026440	A1	2/2007	Broderick et al.
2005/0143635	A1	6/2005	Kamath et al.	2007/0027381	A1	2/2007	Stafford
2005/0176136	A1	8/2005	Burd et al.	2007/0027507	A1	2/2007	Burdett et al.
2005/0177398	A1	8/2005	Watanabe et al.	2007/0032706	A1	2/2007	Kamath et al.
2005/0182306	A1	8/2005	Sloan	2007/0033074	A1	2/2007	Nitzan et al.
2005/0182358	A1	8/2005	Veit et al.	2007/0038044	A1	2/2007	Dobbles et al.
2005/0187720	A1	8/2005	Goode, Jr. et al.	2007/0053341	A1	3/2007	Lizzi
2005/0192494	A1	9/2005	Ginsberg	2007/0060814	A1	3/2007	Stafford
2005/0192557	A1	9/2005	Brauker et al.	2007/0060869	A1	3/2007	Tolle et al.
2005/0195930	A1	9/2005	Spital et al.	2007/0066873	A1	3/2007	Kamath et al.
2005/0199494	A1	9/2005	Say et al.	2007/0066877	A1	3/2007	Arnold et al.
2005/0203360	A1	9/2005	Brauker et al.	2007/0071681	A1	3/2007	Gadkar et al.
2005/0221504	A1	10/2005	Petruno et al.	2007/0073129	A1	3/2007	Shah et al.
2005/0236361	A1	10/2005	Ufer et al.	2007/0078320	A1	4/2007	Stafford
2005/0239154	A1	10/2005	Feldman et al.	2007/0078321	A1	4/2007	Mazza et al.
2005/0241957	A1	11/2005	Mao et al.	2007/0078322	A1	4/2007	Stafford
2005/0242479	A1	11/2005	Petisce et al.	2007/0078323	A1	4/2007	Reggiardo et al.
2005/0245795	A1	11/2005	Goode, Jr. et al.	2007/0093786	A1	4/2007	Goldsmith et al.
2005/0245799	A1	11/2005	Brauker et al.	2007/0100222	A1	5/2007	Mastrototaro et al.
2005/0245839	A1	11/2005	Stivoric et al.	2007/0106133	A1	5/2007	Satchwell et al.
2005/0245904	A1	11/2005	Estes et al.	2007/0106135	A1	5/2007	Sloan et al.
2005/0259514	A1	11/2005	Iseli et al.	2007/0118030	A1	5/2007	Bruce et al.
2005/0277912	A1	12/2005	John	2007/0124002	A1	5/2007	Estes et al.
2005/0287620	A1	12/2005	Heller et al.	2007/0135697	A1	6/2007	Reggiardo
2006/0001538	A1	1/2006	Kraft et al.	2007/0149875	A1	6/2007	Ouyang et al.
2006/0004270	A1	1/2006	Bedard et al.	2007/0153705	A1	7/2007	Rosar et al.
2006/0015020	A1	1/2006	Neale et al.	2007/0156094	A1	7/2007	Safabash et al.
2006/0015024	A1	1/2006	Brister et al.	2007/0163880	A1	7/2007	Woo et al.
2006/0016700	A1	1/2006	Brister et al.	2007/0168224	A1	7/2007	Letzt et al.
2006/0019327	A1	1/2006	Brister et al.	2007/0170893	A1	7/2007	Kao et al.
2006/0020186	A1	1/2006	Brister et al.	2007/0173706	A1	7/2007	Neinast et al.
2006/0020187	A1	1/2006	Brister et al.	2007/0173712	A1	7/2007	Shah et al.
2006/0020188	A1	1/2006	Kamath et al.	2007/0173761	A1	7/2007	Kanderian et al.
2006/0020189	A1	1/2006	Brister et al.	2007/0179349	A1	8/2007	Hoyme et al.
2006/0020190	A1	1/2006	Kamath et al.	2007/0179352	A1	8/2007	Randlov et al.
2006/0020191	A1	1/2006	Brister et al.	2007/0191701	A1	8/2007	Feldman et al.
2006/0020192	A1	1/2006	Brister et al.	2007/0191702	A1	8/2007	Yodfat et al.
2006/0020300	A1	1/2006	Nghiem et al.	2007/0203407	A1	8/2007	Hoss et al.
2006/0029177	A1	2/2006	Cranford, Jr. et al.	2007/0203966	A1	8/2007	Brauker et al.
2006/0031094	A1	2/2006	Cohen et al.	2007/0208245	A1	9/2007	Brauker et al.
2006/0036139	A1	2/2006	Brister et al.	2007/0219496	A1	9/2007	Kamen et al.
2006/0036140	A1	2/2006	Brister et al.	2007/0222609	A1	9/2007	Duron et al.
2006/0036141	A1	2/2006	Kamath et al.	2007/0235331	A1	10/2007	Simpson et al.
2006/0036142	A1	2/2006	Brister et al.	2007/0249922	A1	10/2007	Peyser et al.
2006/0036143	A1	2/2006	Brister et al.	2007/0255321	A1	11/2007	Gerber et al.
2006/0036144	A1	2/2006	Brister et al.	2007/0255348	A1	11/2007	Holtzclaw
2006/0036145	A1	2/2006	Brister et al.	2007/0271285	A1	11/2007	Eichorn et al.
2006/0058588	A1	3/2006	Zdeblick	2008/0009692	A1	1/2008	Stafford
2006/0154642	A1	7/2006	Scannell	2008/0012701	A1	1/2008	Kass et al.
2006/0155180	A1	7/2006	Brister et al.	2008/0017522	A1	1/2008	Heller et al.
2006/0166629	A1	7/2006	Reggiardo	2008/0021666	A1	1/2008	Goode, Jr. et al.
2006/0173260	A1	8/2006	Gaoni et al.	2008/0021972	A1	1/2008	Huelskamp et al.
2006/0173406	A1	8/2006	Hayes et al.	2008/0027586	A1	1/2008	Hern et al.
2006/0173444	A1	8/2006	Choy et al.	2008/0029391	A1	2/2008	Mao et al.
2006/0183984	A1	8/2006	Dobbles et al.	2008/0033254	A1	2/2008	Kamath et al.
2006/0183985	A1	8/2006	Brister et al.	2008/0039702	A1	2/2008	Hayter et al.
2006/0189863	A1	8/2006	Peyser et al.	2008/0045824	A1	2/2008	Tapsak et al.
2006/0193375	A1	8/2006	Lee et al.	2008/0057484	A1	3/2008	Miyata et al.
2006/0198426	A1	9/2006	Partyka	2008/0058625	A1	3/2008	McGarraugh et al.
2006/0222566	A1	10/2006	Brauker et al.	2008/0058626	A1	3/2008	Miyata et al.
2006/0224109	A1	10/2006	Steil et al.	2008/0058678	A1	3/2008	Miyata et al.
2006/0229512	A1	10/2006	Petisce et al.	2008/0060955	A1	3/2008	Goodnow
				2008/0062055	A1	3/2008	Cunningham et al.
				2008/0064937	A1	3/2008	McGarraugh et al.
				2008/0067627	A1	3/2008	Boeck et al.
				2008/0071156	A1	3/2008	Brister et al.
				2008/0071157	A1	3/2008	McGarraugh et al.
				2008/0071158	A1	3/2008	McGarraugh et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0081977	A1	4/2008	Hayter et al.	2009/0033482	A1	2/2009	Hayter et al.
2008/0083617	A1	4/2008	Simpson et al.	2009/0036747	A1	2/2009	Hayter et al.
2008/0086042	A1	4/2008	Brister et al.	2009/0036758	A1	2/2009	Brauker et al.
2008/0086044	A1	4/2008	Brister et al.	2009/0036760	A1	2/2009	Hayter
2008/0086273	A1	4/2008	Shults et al.	2009/0036763	A1	2/2009	Brauker et al.
2008/0092638	A1	4/2008	Brenneman et al.	2009/0040022	A1	2/2009	Finkenzeller
2008/0097289	A1	4/2008	Steil et al.	2009/0043181	A1	2/2009	Brauker et al.
2008/0108942	A1	5/2008	Brister et al.	2009/0043182	A1	2/2009	Brauker et al.
2008/0154513	A1	6/2008	Kovatchev et al.	2009/0043525	A1	2/2009	Brauker et al.
2008/0161666	A1	7/2008	Feldman et al.	2009/0043541	A1	2/2009	Brauker et al.
2008/0167543	A1	7/2008	Say et al.	2009/0043542	A1	2/2009	Brauker et al.
2008/0172205	A1	7/2008	Breton et al.	2009/0045055	A1	2/2009	Rhodes et al.
2008/0179187	A1	7/2008	Ouyang et al.	2009/0048503	A1	2/2009	Dalal et al.
2008/0183060	A1	7/2008	Steil et al.	2009/0054747	A1	2/2009	Fennell
2008/0183061	A1	7/2008	Goode et al.	2009/0055149	A1	2/2009	Hayter et al.
2008/0183399	A1	7/2008	Goode et al.	2009/0062633	A1	3/2009	Brauker et al.
2008/0188731	A1	8/2008	Brister et al.	2009/0062635	A1	3/2009	Brauker et al.
2008/0188796	A1	8/2008	Steil et al.	2009/0062767	A1	3/2009	VanAntwerp et al.
2008/0189051	A1	8/2008	Goode et al.	2009/0063187	A1	3/2009	Johnson et al.
2008/0194934	A1	8/2008	Ray et al.	2009/0063402	A1	3/2009	Hayter
2008/0194935	A1	8/2008	Brister et al.	2009/0076356	A1	3/2009	Simpson et al.
2008/0194936	A1	8/2008	Goode et al.	2009/0076359	A1	3/2009	Peyser et al.
2008/0194937	A1	8/2008	Goode et al.	2009/0076360	A1	3/2009	Brister et al.
2008/0194938	A1	8/2008	Brister et al.	2009/0076361	A1	3/2009	Kamath et al.
2008/0195232	A1	8/2008	Carr-Brendel et al.	2009/0085873	A1	4/2009	Betts et al.
2008/0195967	A1	8/2008	Goode et al.	2009/0093687	A1	4/2009	Telfort et al.
2008/0197024	A1	8/2008	Simpson et al.	2009/0094680	A1	4/2009	Gupta et al.
2008/0200788	A1	8/2008	Brister et al.	2009/0099436	A1	4/2009	Brister et al.
2008/0200789	A1	8/2008	Brister et al.	2009/0105570	A1	4/2009	Sloan et al.
2008/0200791	A1	8/2008	Simpson et al.	2009/0105571	A1	4/2009	Fennell et al.
2008/0208025	A1	8/2008	Shults et al.	2009/0105636	A1	4/2009	Hayter et al.
2008/0208113	A1	8/2008	Damiano et al.	2009/0124877	A1	5/2009	Goode et al.
2008/0212600	A1	9/2008	Yoo	2009/0124878	A1	5/2009	Goode et al.
2008/0214900	A1	9/2008	Fennell et al.	2009/0124879	A1	5/2009	Brister et al.
2008/0214915	A1	9/2008	Brister et al.	2009/0124964	A1	5/2009	Leach et al.
2008/0214918	A1	9/2008	Brister et al.	2009/0131768	A1	5/2009	Simpson et al.
2008/0228051	A1	9/2008	Shults et al.	2009/0131769	A1	5/2009	Leach et al.
2008/0228054	A1	9/2008	Shults et al.	2009/0131776	A1	5/2009	Simpson et al.
2008/0234943	A1	9/2008	Ray et al.	2009/0131777	A1	5/2009	Simpson et al.
2008/0242961	A1	10/2008	Brister et al.	2009/0137886	A1	5/2009	Shariati et al.
2008/0254544	A1	10/2008	Modzelewski et al.	2009/0137887	A1	5/2009	Shariati et al.
2008/0255434	A1	10/2008	Hayter et al.	2009/0143659	A1	6/2009	Li et al.
2008/0255437	A1	10/2008	Hayter	2009/0143660	A1	6/2009	Brister et al.
2008/0255808	A1	10/2008	Hayter	2009/0146826	A1	6/2009	Gofman et al.
2008/0256048	A1	10/2008	Hayter	2009/0156919	A1	6/2009	Brister et al.
2008/0262469	A1	10/2008	Brister et al.	2009/0156924	A1	6/2009	Shariati et al.
2008/0267823	A1	10/2008	Wang et al.	2009/0163790	A1	6/2009	Brister et al.
2008/0275313	A1	11/2008	Brister et al.	2009/0163791	A1	6/2009	Brister et al.
2008/0287761	A1	11/2008	Hayter	2009/0164190	A1	6/2009	Hayter
2008/0287762	A1	11/2008	Hayter	2009/0164239	A1	6/2009	Hayter et al.
2008/0287763	A1	11/2008	Hayter	2009/0164251	A1	6/2009	Hayter
2008/0287764	A1	11/2008	Rasdal et al.	2009/0178459	A1	7/2009	Li et al.
2008/0287765	A1	11/2008	Rasdal et al.	2009/0182217	A1	7/2009	Li et al.
2008/0287766	A1	11/2008	Rasdal et al.	2009/0192366	A1	7/2009	Mensingher et al.
2008/0288180	A1	11/2008	Hayter	2009/0192380	A1	7/2009	Shariati et al.
2008/0288204	A1	11/2008	Hayter et al.	2009/0192722	A1	7/2009	Shariati et al.
2008/0294024	A1	11/2008	Cosentino et al.	2009/0192724	A1	7/2009	Brauker et al.
2008/0296155	A1	12/2008	Shults et al.	2009/0192745	A1	7/2009	Kamath et al.
2008/0301436	A1	12/2008	Yao et al.	2009/0192751	A1	7/2009	Kamath et al.
2008/0306368	A1	12/2008	Goode et al.	2009/0198118	A1	8/2009	Hayter et al.
2008/0306434	A1	12/2008	Dobbles et al.	2009/0203981	A1	8/2009	Brauker et al.
2008/0306435	A1	12/2008	Kamath et al.	2009/0204340	A1	8/2009	Feldman et al.
2008/0306444	A1	12/2008	Brister et al.	2009/0204341	A1	8/2009	Brauker et al.
2008/0312841	A1	12/2008	Hayter	2009/0216103	A1	8/2009	Brister et al.
2008/0312842	A1	12/2008	Hayter	2009/0237216	A1	9/2009	Twitchell, Jr.
2008/0312844	A1	12/2008	Hayter et al.	2009/0240120	A1	9/2009	Mensingher et al.
2008/0312845	A1	12/2008	Hayter et al.	2009/0240128	A1	9/2009	Mensingher et al.
2008/0319295	A1	12/2008	Bernstein et al.	2009/0240193	A1	9/2009	Mensingher et al.
2008/0319296	A1	12/2008	Bernstein et al.	2009/0242399	A1	10/2009	Kamath et al.
2008/0320587	A1	12/2008	Vauclair et al.	2009/0242425	A1	10/2009	Kamath et al.
2009/0005665	A1	1/2009	Hayter et al.	2009/0247855	A1	10/2009	Boock et al.
2009/0006034	A1	1/2009	Hayter et al.	2009/0247856	A1	10/2009	Boock et al.
2009/0012379	A1	1/2009	Goode et al.	2009/0287073	A1	11/2009	Boock et al.
2009/0018424	A1	1/2009	Kamath et al.	2009/0287074	A1	11/2009	Shults et al.
2009/0030294	A1	1/2009	Petisce et al.	2009/0296742	A1	12/2009	Sicurello et al.
				2009/0299155	A1	12/2009	Yang et al.
				2009/0299156	A1	12/2009	Simpson et al.
				2009/0299162	A1	12/2009	Brauker et al.
				2009/0299276	A1	12/2009	Brauker et al.

(56)

References Cited

OTHER PUBLICATIONS

U.S. PATENT DOCUMENTS

2010/0010329	A1	1/2010	Taub et al.
2010/0025238	A1	2/2010	Gottlieb et al.
2010/0057040	A1	3/2010	Hayter
2010/0057041	A1	3/2010	Hayter
2010/0057042	A1	3/2010	Hayter
2010/0057044	A1	3/2010	Hayter
2010/0057057	A1	3/2010	Hayter et al.
2010/0105999	A1	4/2010	Dixon et al.
2010/0110931	A1	5/2010	Shim et al.
2010/0119881	A1	5/2010	Patel et al.
2010/0152554	A1	6/2010	Steine et al.
2010/0160759	A1	6/2010	Celentano et al.
2010/0168538	A1	7/2010	Keenan et al.
2010/0168545	A1	7/2010	Kamath et al.
2010/0174266	A1	7/2010	Estes
2010/0185071	A1	7/2010	Simpson et al.
2010/0185175	A1	7/2010	Kamen et al.
2010/0191085	A1	7/2010	Budiman
2010/0198142	A1	8/2010	Sloan et al.
2010/0213080	A1	8/2010	Celentano et al.
2010/0235439	A1	9/2010	Goodnow et al.
2010/0267161	A1	10/2010	Wu et al.
2010/0313105	A1	12/2010	Nekoomaram et al.
2010/0324403	A1	12/2010	Brister et al.
2010/0331646	A1	12/2010	Hoss et al.
2010/0332142	A1	12/2010	Shadforth et al.
2011/0031986	A1	2/2011	Bhat et al.
2011/0074349	A1	3/2011	Ghovanloo
2011/0125040	A1	5/2011	Crawford et al.
2011/0148905	A1	6/2011	Simmons et al.
2011/0184268	A1	7/2011	Taub
2011/0191059	A1	8/2011	Farrell et al.
2011/0230741	A1	9/2011	Liang et al.
2011/0257895	A1	10/2011	Brauker et al.
2011/0270112	A1	11/2011	Manera et al.
2011/0287528	A1	11/2011	Fern et al.
2012/0108931	A1	5/2012	Taub et al.
2012/0148054	A1	6/2012	Rank et al.
2012/0190989	A1	7/2012	Kaiser et al.
2012/0215092	A1	8/2012	Harris, III et al.
2013/0035575	A1	2/2013	Mayou et al.
2013/0235166	A1	9/2013	Jones et al.
2015/0335245	A1	11/2015	Fennell et al.

FOREIGN PATENT DOCUMENTS

EP	0320109	6/1989
EP	0353328	2/1990
EP	0390390	10/1990
EP	0396788	11/1990
EP	0286118	1/1995
EP	1048264	11/2000
WO	WO-1996/025089	8/1996
WO	WO-1996/035370	11/1996
WO	WO-1998/035053	8/1998
WO	WO-1999/056613	11/1999
WO	WO-2000/049940	8/2000
WO	WO-2000/059370	10/2000
WO	WO-2000/060350	10/2000
WO	WO-2000/078992	12/2000
WO	WO-2001/052935	7/2001
WO	WO-2001/054753	8/2001
WO	WO-2002/016905	2/2002
WO	WO-2002/058537	8/2002
WO	WO-2003/076893	9/2003
WO	WO-2003/082091	10/2003
WO	WO-2003/085372	10/2003
WO	WO-2004/061420	7/2004
WO	WO-2005/010756	2/2005
WO	WO-2005/041766	5/2005
WO	WO-2005/089103	9/2005
WO	WO-2005/117269	12/2005
WO	WO-2006/024671	3/2006

Bennion, N., et al., "Alternate Site Glucose Testing: A Crossover Design", *Diabetes Technology & Therapeutics*, vol. 4, No. 1, 2002, pp. 25-33.

Blank, T. B., et al., "Clinical Results From a Non-Invasive Blood Glucose Monitor", *Optical Diagnostics and Sensing of Biological Fluids and Glucose and Cholesterol Monitoring II, Proceedings of SPIE*, vol. 4624, 2002, pp. 1-10.

Brooks, S. L., et al., "Development of an On-Line Glucose Sensor for Fermentation Monitoring", *Biosensors*, vol. 3, 1987/1988, pp. 45-56.

Cass, A. E., et al., "Ferrocene-Medicated Enzyme Electrode for Amperometric Determination of Glucose" *Analytical Chemistry*, vol. 56, No. 4, 1984, 667-671.

Csoregi, E., et al., "Design and Optimization of a Selective Subcutaneously Implantable Glucose Electrode Based on 'Wired' Glucose Oxidase", *Analytical Chemistry*, vol. 67, No. 7, 1995, pp. 1240-1244.

Feldman, B., et al., "A Continuous Glucose Sensor Based on Wired Enzyme™ Technology—Results from a 3-Day Trial in Patients with Type 1 Diabetes", *Diabetes Technology & Therapeutics*, vol. 5, No. 5, 2003, pp. 769-779.

Feldman, B., et al., "Correlation of Glucose Concentrations in Interstitial Fluid and Venous Blood During Periods of Rapid Glucose Change", Abbott Diabetes Care, Inc. *Freestyle Navigator Continuous Glucose Monitor Pamphlet*, 2004.

Isermann, R., "Supervision, Fault-Detection and Fault-Diagnosis Methods—An Introduction", *Control Engineering Practice*, vol. 5, No. 5, 1997, pp. 639-652.

Isermann, R., et al., "Trends in the Application of Model-Based Fault Detection and Diagnosis of Technical Processes", *Control Engineering Practice*, vol. 5, No. 5, 1997, pp. 709-719.

Johnson, P. C., "Peripheral Circulation", *John Wiley & Sons*, 1978, pp. 198.

Jungheim, K., et al., "How Rapid Does Glucose Concentration Change in Daily Life of Patients with Type 1 Diabetes?", 2002, pp. 250.

Jungheim, K., et al., "Risky Delay of Hypoglycemia Detection by Glucose Monitoring at the Arm", *Diabetes Care*, vol. 24, No. 7, 2001, pp. 1303-1304.

Kaplan, S. M., "Wiley Electrical and Electronics Engineering Dictionary", *IEEE Press*, 2004, pp. 141, 142, 548, 549.

Lortz, J., et al., "What is Bluetooth? We Explain the Newest Short-Range Connectivity Technology", *Smart Computing Learning Series, Wireless Computing*, vol. 8, Issue 5, 2002, pp. 72-74.

Malin, S. F., et al., "Noninvasive Prediction of Glucose by Near-Infrared Diffuse Reflectance Spectroscopy", *Clinical Chemistry*, vol. 45, No. 9, 1999, pp. 1651-1658.

McGarraugh, G., et al., "Glucose Measurements Using Blood Extracted from the Forearm and the Finger", *TheraSense, Inc.*, 2001, 16 Pages.

McGarraugh, G., et al., "Physiological Influences on Off-Finger Glucose Testing", *Diabetes Technology & Therapeutics*, vol. 3, No. 3, 2001, pp. 367-376.

McKean, B. D., et al., "A Telemetry-Instrumentation System for Chronically Implanted Glucose and Oxygen Sensors", *IEEE Transactions on Biomedical Engineering*, vol. 35, No. 7, 1988, pp. 526-532.

Pickup, J., et al., "Implantable Glucose Sensors: Choosing the Appropriate Sensing Strategy", *Biosensors*, vol. 3, 1987/1988, pp. 335-346.

Pickup, J., et al., "In Vivo Molecular Sensing in Diabetes Mellitus: An Implantable Glucose Sensor with Direct Electron Transfer", *Diabetologia*, vol. 32, 1989, pp. 213-217.

Pishko, M. V., et al., "Amperometric Glucose Microelectrodes Prepared Through Immobilization of Glucose Oxidase in Redox Hydrogels", *Analytical Chemistry*, vol. 63, No. 20, 1991, pp. 2268-2272.

Quinn, C. P., et al., "Kinetics of Glucose Delivery to Subcutaneous Tissue in Rats Measured with 0.3-mm Amperometric Microsensors", *The American Physiological Society*, 1995, E155-E161.


(56)

References Cited

OTHER PUBLICATIONS

- Roe, J. N., et al., "Bloodless Glucose Measurements", *Critical Review in Therapeutic Drug Carrier Systems*, vol. 15, Issue 3, 1998, pp. 199-241.
- Sakakida, M., et al., "Development of Ferrocene-Mediated Needle-Type Glucose Sensor as a Measure of True Subcutaneous Tissue Glucose Concentrations", *Artificial Organs Today*, vol. 2, No. 2, 1992, pp. 145-158.
- Sakakida, M., et al., "Ferrocene-Mediated Needle-Type Glucose Sensor Covered with Newly Designed Biocompatible Membrane", *Sensors and Actuators B*, vol. 13-14, 1993, pp. 319-322.
- Salehi, C., et al., "A Telemetry-Instrumentation System for Long-Term Implantable Glucose and Oxygen Sensors", *Analytical Letters*, vol. 29, No. 13, 1996, pp. 2289-2308.
- Schmidtke, D. W., et al., "Measurement and Modeling of the Transient Difference Between Blood and Subcutaneous Glucose Concentrations in the Rat After Injection of Insulin", *Proceedings of the National Academy of Sciences*, vol. 95, 1998, pp. 294-299.
- Shaw, G. W., et al., "In Vitro Testing of a Simply Constructed, Highly Stable Glucose Sensor Suitable for Implantation in Diabetic Patients", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 401-406.
- Shichiri, M., et al., "Glycaemic Control in Pancreatectomized Dogs with a Wearable Artificial Endocrine Pancreas", *Diabetologia*, vol. 24, 1983, pp. 179-184.
- Shichiri, M., et al., "In Vivo Characteristics of Needle-Type Glucose Sensor—Measurements of Subcutaneous Glucose Concentrations in Human Volunteers", *Hormone and Metabolic Research Supplement Series*, vol. 20, 1988, pp. 17-20.
- Shichiri, M., et al., "Membrane Design for Extending the Long-Life of an Implantable Glucose Sensor" *Diabetes Nutrition and Metabolism*, vol. 2, 1989, pp. 309-313.
- Shichiri, M., et al., "Needle-type Glucose Sensor for Wearable Artificial Endocrine Pancreas", *Implantable Sensors for Closed-Loop Prosthetic Systems*, Chapter 15, 1985, pp. 197-210.
- Shichiri, M., et al., "Telemetry Glucose Monitoring Device With Needle-Type Glucose Sensor: A Useful Tool for Blood Glucose Monitoring in Diabetic Individuals", *Diabetes Care*, vol. 9, No. 3, 1986, pp. 298-301.
- Shichiri, M., et al., "Wearable Artificial Endocrine Pancreas With Needle-Type Glucose Sensor", *The Lancet*, 1982, pp. 1129-1131.
- Shults, M. C., et al., "A Telemetry-Instrumentation System for Monitoring Multiple Subcutaneously Implanted Glucose Sensors", *IEEE Transactions on Biomedical Engineering*, vol. 41, No. 10, 1994, pp. 937-942.
- Sternberg, R., et al., "Study and Development of Multilayer Needle-Type Enzyme-Based Glucose Microsensors", *Biosensors*, vol. 4, 1988, pp. 27-40.
- Thompson, M., et al., "In Vivo Probes: Problems and Perspectives", *Clinical Biochemistry*, vol. 19, 1986, pp. 255-261.
- Turner, A., et al., "Diabetes Mellitus: Biosensors for Research and Management", *Biosensors*, vol. 1, 1985, pp. 85-115.
- Updike, S. J., et al., "Principles of Long-Term Fully Implanted Sensors with Emphasis on Radiotelemetric Monitoring of Blood Glucose from Inside a Subcutaneous Foreign Body Capsule (FBC)", *Biosensors in the Body: Continuous in vivo Monitoring, Chapter 4*, 1997, pp. 117-137.
- Velho, G., et al., "Strategies for Calibrating a Subcutaneous Glucose Sensor", *Biomedica Biochimica Acta*, vol. 48, 1989, pp. 957-964.
- Wilson, G. S., et al., "Progress Toward the Development of an Implantable Sensor for Glucose", *Clinical Chemistry*, vol. 38, No. 9, 1992, pp. 1613-1617.
- Canadian Patent Application No. 2,683,721, Examiner's Report dated Mar. 17, 2015.
- European Patent Application No. 08745799.0, Extended European Search Report dated Oct. 16, 2012.
- PCT Application No. PCT/US2008/060273, International Preliminary Report on Patentability and Written Opinion of the International Searching Authority dated Oct. 29, 2009.
- PCT Application No. PCT/US2008/060273, International Search Report and Written Opinion of the International Searching Authority dated Oct. 1, 2008.
- U.S. Appl. No. 12/102,836, Notice of Allowance dated Jun. 18, 2010.
- U.S. Appl. No. 12/102,836, Office Action dated Mar. 11, 2010.
- U.S. Appl. No. 12/894,004, Notice of Allowance dated Apr. 7, 2011.
- U.S. Appl. No. 12/894,004, Office Action dated Dec. 30, 2010.
- U.S. Appl. No. 12/894,004, Office Action dated Jan. 21, 2011.
- U.S. Appl. No. 13/114,029, Notice of Allowance dated Jan. 18, 2012.
- U.S. Appl. No. 13/114,029, Office Action dated Nov. 2, 2011.
- U.S. Appl. No. 13/437,894, Notice of Allowance dated Jan. 15, 2013.
- U.S. Appl. No. 13/437,894, Office Action dated Oct. 17, 2012.
- U.S. Appl. No. 13/867,948, Notice of Allowance dated Feb. 4, 2014.
- U.S. Appl. No. 13/867,948, Office Action dated Dec. 16, 2013.
- U.S. Appl. No. 13/867,948, Office Action dated Jul. 10, 2013.
- U.S. Appl. No. 14/188,659, Notice of Allowance dated Nov. 26, 2014.
- U.S. Appl. No. 14/188,659, Office Action dated Sep. 17, 2014.
- U.S. Appl. No. 14/596,759, Notice of Allowance dated Apr. 20, 2016.
- U.S. Appl. No. 14/596,759, Office Action dated Jan. 25, 2016.
- U.S. Appl. No. 15/209,741, Office Action dated May 4, 2017.
- U.S. Appl. No. 15/209,741, Notice of Allowance dated May 11, 2017.

* cited by examiner

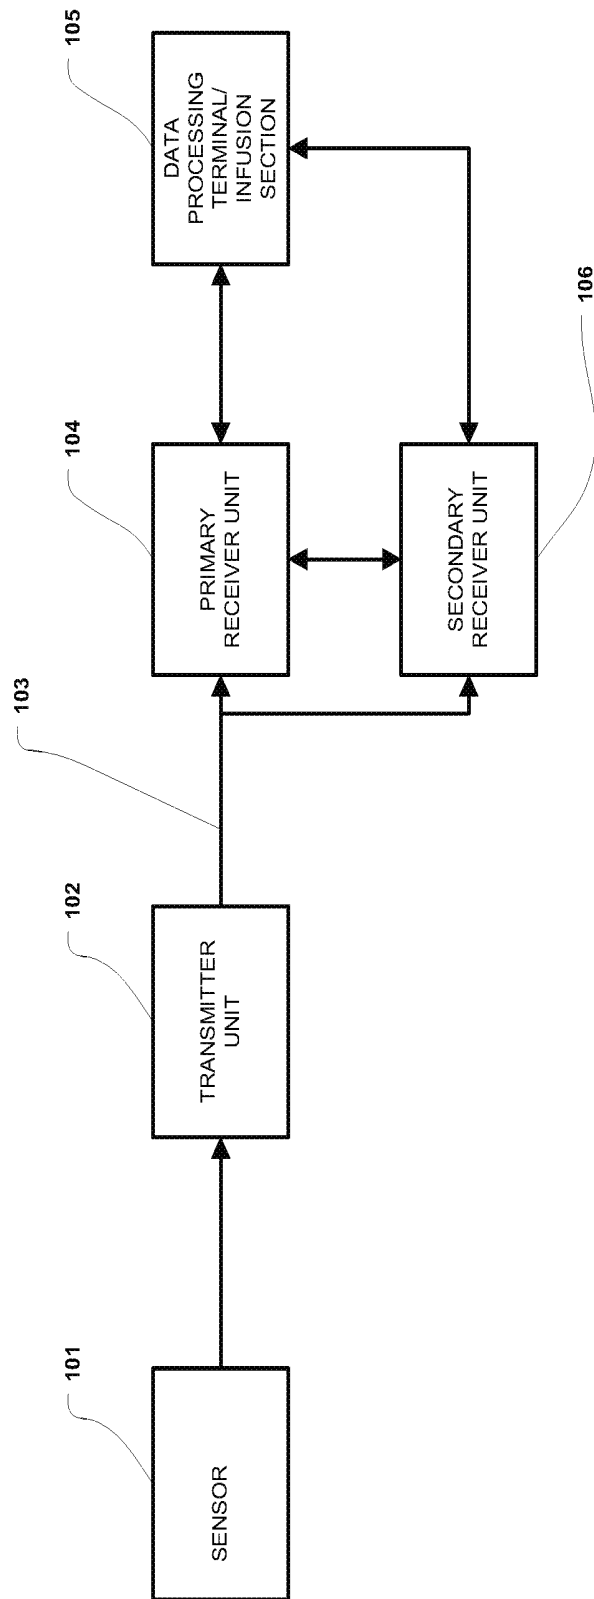

100

FIGURE 1

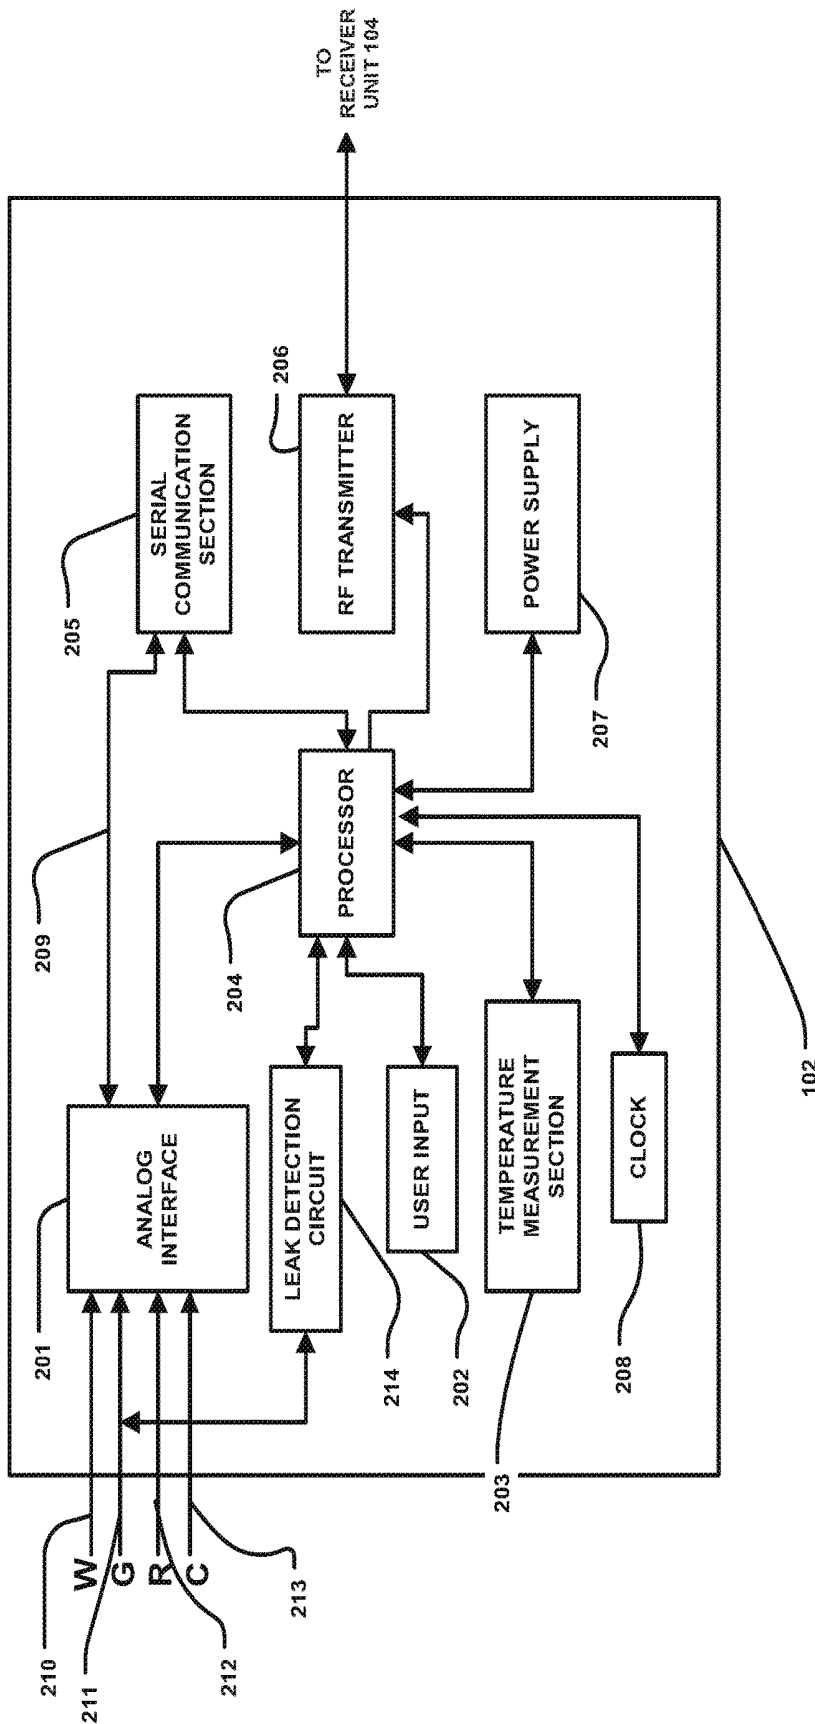


FIGURE 2

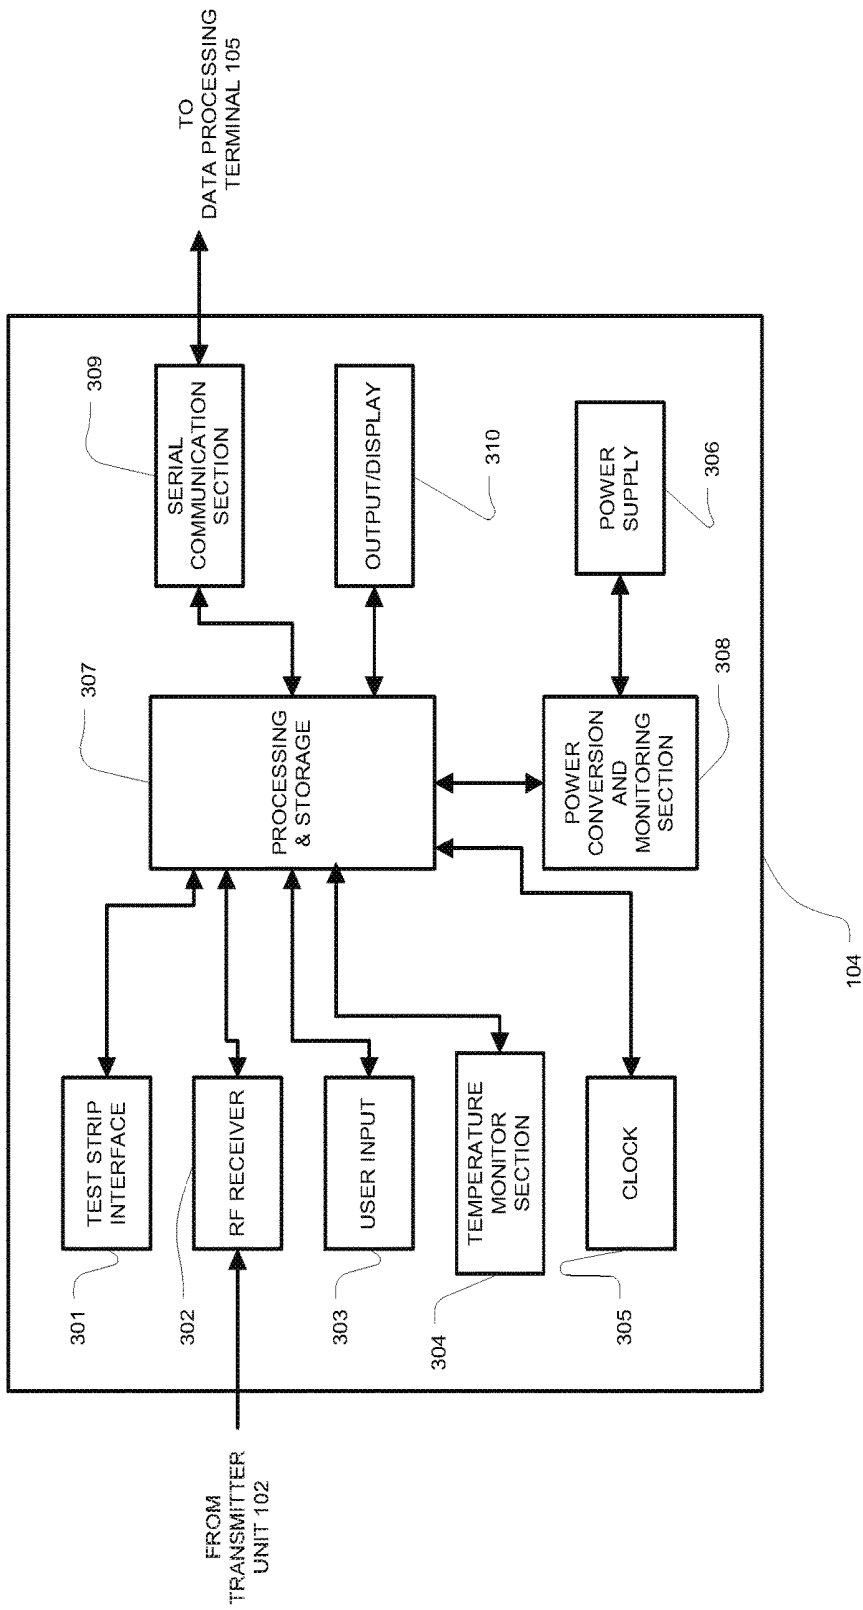


FIGURE 3

**METHOD AND APPARATUS FOR
PROVIDING DYNAMIC MULTI-STAGE
SIGNAL AMPLIFICATION IN A MEDICAL
DEVICE**

RELATED APPLICATIONS

The present application is a continuation of U.S. patent application Ser. No. 15/209,741 filed Jul. 13, 2016, now U.S. Pat. No. 9,743,866, which is a continuation of U.S. patent application Ser. No. 14/596,759 filed Jan. 14, 2015, now U.S. Pat. No. 9,402,584, which is a continuation of U.S. patent application Ser. No. 14/188,659 filed Feb. 24, 2014, now U.S. Pat. No. 8,937,540, which is a continuation of U.S. patent application Ser. No. 13/867,948 filed Apr. 22, 2013, now U.S. Pat. No. 8,698,615, which is a continuation of U.S. patent application Ser. No. 13/437,894 filed Apr. 2, 2012, now U.S. Pat. No. 8,427,298, which is a continuation of U.S. patent application Ser. No. 13/114,029 filed May 23, 2011, now U.S. Pat. No. 8,149,103, which is a continuation of U.S. patent application Ser. No. 12/849,004 filed Aug. 2, 2010, now U.S. Pat. No. 7,948,369, which is a continuation of U.S. patent application Ser. No. 12/102,836 filed Apr. 14, 2008, now U.S. Pat. No. 7,768,387, which claims priority under § 35 U.S.C. 119(e) to U.S. Provisional Application No. 60/911,866 filed Apr. 14, 2007, entitled "Method and Apparatus for Providing Dynamic Multi-Stage Signal Amplification in a Medical Device", the disclosures of each of which are incorporated herein by reference for all purposes.

BACKGROUND

Analyte (e.g., glucose) monitoring systems including continuous and discrete monitoring systems generally include a small, lightweight battery powered and microprocessor controlled system which is configured to detect signals proportional to the corresponding measured glucose levels using an electrometer, and RF signals to transmit the collected data. One aspect of certain analyte monitoring systems include a transcutaneous or subcutaneous analyte sensor configuration which is, for example, partially mounted on the skin of a subject whose analyte level is to be monitored. The sensor cell may use a two or three-electrode (work, reference and counter electrodes) configuration driven by a controlled potential (potentiostat) analog circuit connected through a contact system.

The analyte sensor may be configured so that a portion thereof is placed under the skin of the patient so as to detect the analyte levels of the patient, and another portion of segment of the analyte sensor that is in communication with the transmitter unit. The transmitter unit is configured to transmit the analyte levels detected by the sensor over a wireless communication link such as an RF (radio frequency) communication link to a receiver/monitor unit. The receiver/monitor unit performs data analysis, among others on the received analyte levels to generate information pertaining to the monitored analyte levels. To provide flexibility in analyte sensor manufacturing and/or design, among others, tolerance of a larger range of the analyte sensor sensitivities for processing by the transmitter unit is desirable.

In view of the foregoing, it would be desirable to have a method and apparatus for providing a dynamic multi-stage amplification of signals for use in medical telemetry systems such as, for example, analyte monitoring systems.

SUMMARY OF THE INVENTION

In one embodiment, an apparatus including a first amplifier having at least one input terminal and an output terminal,

the at least one input terminal coupled to a signal source, the output terminal configured to provide a first output signal, a second amplifier having at least one input terminal and an output terminal, the at least one input terminal coupled to the output terminal of the first amplifier, the output terminal of the second amplifier configured to provide a second output signal, a processor operatively coupled to receive the first output signal and the second output signal, where the first output signal is a predetermined ratio of the second output signal, and further, where the first output signal and the second output signal are associated with a monitored analyte level of a user is disclosed.

These and other objects, features and advantages of the present invention will become more fully apparent from the following detailed description of the embodiments, the appended claims and the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a block diagram of a data monitoring and management system for practicing one or more embodiments of the present invention;

FIG. 2 is a block diagram of the transmitter unit of the data monitoring and management system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIG. 3 is a block diagram of the receiver/monitor unit of the data monitoring and management system shown in FIG. 1 in accordance with one embodiment of the present invention; and

FIG. 4 is a schematic of the dynamic multi-stage signal amplification in the transmitter unit of the data monitoring and management system shown in FIG. 1 in accordance with one embodiment of the present invention.

DETAILED DESCRIPTION

As described in further detail below, in accordance with the various embodiments of the present invention, there is provided a method and apparatus for providing dynamic multi-stage signal amplification for use in a medical telemetry system. In particular, within the scope of the present invention, there are provided method and apparatus for a multi-stage signal amplifier configuration in the analog interface of the data transmitter unit in the data processing and management system.

FIG. 1 illustrates a data monitoring and management system such as, for example, analyte (e.g., glucose) monitoring system **100** in accordance with one embodiment of the present invention. The subject invention is further described primarily with respect to a glucose monitoring system for convenience and such description is in no way intended to limit the scope of the invention. It is to be understood that the analyte monitoring system may be configured to monitor a variety of analytes, e.g., lactate, and the like.

Analytes that may be monitored include, for example, acetyl choline, amylase, bilirubin, cholesterol, chorionic gonadotropin, creatine kinase (e.g., CK-MB), creatine, DNA, fructosamine, glucose, glutamine, growth hormones, hormones, ketones, lactate, peroxide, prostate-specific antigen, prothrombin, RNA, thyroid stimulating hormone, and troponin. The concentration of drugs, such as, for example, antibiotics (e.g., gentamicin, vancomycin, and the like), digitoxin, digoxin, drugs of abuse, theophylline, and warfarin, may also be monitored.

The analyte monitoring system **100** includes a sensor **101**, a transmitter unit **102** coupled to the sensor **101**, and a

primary receiver unit **104** which is configured to communicate with the transmitter unit **102** via a communication link **103**. The primary receiver unit **104** may be further configured to transmit data to a data processing terminal **105** for evaluating the data received by the primary receiver unit **104**. Moreover, the data processing terminal in one embodiment may be configured to receive data directly from the transmitter unit **102** via a communication link which may optionally be configured for bi-directional communication.

Also shown in FIG. **1** is a secondary receiver unit **106** which is operatively coupled to the communication link and configured to receive data transmitted from the transmitter unit **102**. Moreover, as shown in the Figure, the secondary receiver unit **106** is configured to communicate with the primary receiver unit **104** as well as the data processing terminal **105**. Indeed, the secondary receiver unit **106** may be configured for bi-directional wireless communication with each of the primary receiver unit **104** and the data processing terminal **105**. As discussed in further detail below, in one embodiment of the present invention, the secondary receiver unit **106** may be configured to include a limited number of functions and features as compared with the primary receiver unit **104**. As such, the secondary receiver unit **106** may be configured substantially in a smaller compact housing or embodied in a device such as a wrist watch, for example. Alternatively, the secondary receiver unit **106** may be configured with the same or substantially similar functionality as the primary receiver unit **104**, and may be configured to be used in conjunction with a docking cradle unit for placement by bedside, for night time monitoring, and/or bi-directional communication device.

Only one sensor **101**, transmitter unit **102**, communication link **103**, and data processing terminal **105** are shown in the embodiment of the analyte monitoring system **100** illustrated in FIG. **1**. However, it will be appreciated by one of ordinary skill in the art that the analyte monitoring system **100** may include one or more sensor **101**, transmitter unit **102**, communication link **103**, and data processing terminal **105**. Moreover, within the scope of the present invention, the analyte monitoring system **100** may be a continuous monitoring system, or semi-continuous, or a discrete monitoring system. In a multi-component environment, each device is configured to be uniquely identified by each of the other devices in the system so that communication conflict is readily resolved between the various components within the analyte monitoring system **100**.

In one embodiment of the present invention, the sensor **101** is physically positioned in or on the body of a user whose analyte level is being monitored. The sensor **101** may be configured to continuously sample the analyte level of the user and convert the sampled analyte level into a corresponding data signal for transmission by the transmitter unit **102**. In one embodiment, the transmitter unit **102** is coupled to the sensor **101** so that both devices are positioned on the user's body, with at least a portion of the analyte sensor **101** positioned transcutaneously under the skin layer of the user. The transmitter unit **102** performs data processing such as filtering and encoding on data signals, each of which corresponds to a sampled analyte level of the user, for transmission to the primary receiver unit **104** via the communication link **103**.

In one embodiment, the analyte monitoring system **100** is configured as a one-way RF communication path from the transmitter unit **102** to the primary receiver unit **104**. In such embodiment, the transmitter unit **102** transmits the sampled data signals received from the sensor **101** without acknowl-

edgement from the primary receiver unit **104** that the transmitted sampled data signals have been received. For example, the transmitter unit **102** may be configured to transmit the encoded sampled data signals at a fixed rate (e.g., at one minute intervals) after the completion of the initial power on procedure. Likewise, the primary receiver unit **104** may be configured to detect such transmitted encoded sampled data signals at predetermined time intervals. Alternatively, the analyte monitoring system **100** may be configured with a bi-directional RF (or otherwise) communication between the transmitter unit **102** and the primary receiver unit **104**.

Additionally, in one aspect, the primary receiver unit **104** may include two sections. The first section is an analog interface section that is configured to communicate with the transmitter unit **102** via the communication link **103**. In one embodiment, the analog interface section may include an RF receiver and an antenna for receiving and amplifying the data signals from the transmitter unit **102**, which are thereafter, demodulated with a local oscillator and filtered through a band-pass filter. The second section of the primary receiver unit **104** is a data processing section which is configured to process the data signals received from the transmitter unit **102** such as by performing data decoding, error detection and correction, data clock generation, and data bit recovery.

In operation, upon completing the power-on procedure, the primary receiver unit **104** is configured to detect the presence of the transmitter unit **102** within its range based on, for example, the strength of the detected data signals received from the transmitter unit **102** or a predetermined transmitter identification information. Upon successful synchronization with the corresponding transmitter unit **102**, the primary receiver unit **104** is configured to begin receiving from the transmitter unit **102** data signals corresponding to the user's detected analyte level. More specifically, the primary receiver unit **104** in one embodiment is configured to perform synchronized time hopping with the corresponding synchronized transmitter unit **102** via the communication link **103** to obtain the user's detected analyte level.

Referring again to FIG. **1**, the data processing terminal **105** may include a personal computer, a portable computer such as a laptop or a handheld device (e.g., personal digital assistants (PDAs)), and the like, each of which may be configured for data communication with the receiver via a wired or a wireless connection. Additionally, the data processing terminal **105** may further be connected to a data network (not shown) for storing, retrieving and updating data corresponding to the detected analyte level of the user.

Within the scope of the present invention, the data processing terminal **105** may include an infusion device such as an insulin infusion pump or the like, which may be configured to administer insulin to patients, and which may be configured to communicate with the receiver unit **104** for receiving, among others, the measured analyte level. Alternatively, the receiver unit **104** may be configured to integrate an infusion device therein so that the receiver unit **104** is configured to administer insulin therapy to patients, for example, for administering and modifying basal profiles, as well as for determining appropriate boluses for administration based on, among others, the detected analyte levels received from the transmitter unit **102**.

Additionally, the transmitter unit **102**, the primary receiver unit **104** and the data processing terminal **105** may each be configured for bi-directional wireless communication such that each of the transmitter unit **102**, the primary receiver unit **104** and the data processing terminal **105** may

be configured to communicate (that is, transmit data to and receive data from) with each other via the wireless communication link. More specifically, the data processing terminal **105** may in one embodiment be configured to receive data directly from the transmitter unit **102** via the communication link, where the communication link, as described above, may be configured for bi-directional communication.

In this embodiment, the data processing terminal **105** which may include an insulin pump, may be configured to receive the analyte signals from the transmitter unit **102**, and thus, incorporate the functions of the receiver unit **104** including data processing for managing the patient's insulin therapy and analyte monitoring. In one embodiment, the communication link **103** may include one or more of an RF communication protocol, an infrared communication protocol, a Bluetooth® enabled communication protocol, an 802.11x wireless communication protocol, or an equivalent wireless communication protocol which would allow secure, wireless communication of several units (for example, per HIPAA requirements) while avoiding potential data collision and interference.

FIG. 2 is a block diagram of the transmitter of the data monitoring and detection system shown in FIG. 1 in accordance with one embodiment of the present invention. Referring to the Figure, the transmitter unit **102** in one embodiment includes an analog interface **201** configured to communicate with the sensor **101** (FIG. 1), a user input **202**, and a temperature detection section **203**, each of which is operatively coupled to a transmitter processor **204** such as a central processing unit (CPU). As can be seen from FIG. 2, there are provided four contacts, three of which are electrodes—work electrode (W) **210**, guard contact (G) **211**, reference electrode (R) **212**, and counter electrode (C) **213**, each operatively coupled to the analog interface **201** of the transmitter unit **102** for connection to the sensor **101** (FIG. 1). In one embodiment, each of the work electrode (W) **210**, guard contact (G) **211**, reference electrode (R) **212**, and counter electrode (C) **213** may be made using a conductive material that is either printed or etched, for example, such as carbon which may be printed, or metal foil (e.g., gold) which may be etched. Moreover, in a further aspect, the electrode layers may be disposed in a stacked configuration where, each of the working electrode **210**, the reference electrode **212** and the counter electrode **213** may be disposed on a substrate layer with one or more dielectric layers disposed therebetween such that at least a portion of each of the electrodes are positioned on top of one another in a stacked or layered configuration.

Further shown in FIG. 2 are a transmitter serial communication section **205** and an RF transmitter **206**, each of which is also operatively coupled to the transmitter processor **204**. Moreover, a power supply **207** such as a battery is also provided in the transmitter unit **102** to provide the necessary power for the transmitter unit **102**. Additionally, as can be seen from the Figure, clock **208** is provided to, among others, supply real time information to the transmitter processor **204**.

In one embodiment, a unidirectional input path is established from the sensor **101** (FIG. 1) and/or manufacturing and testing equipment to the analog interface **201** of the transmitter unit **102**, while a unidirectional output is established from the output of the RF transmitter **206** of the transmitter unit **102** for transmission to the primary receiver unit **104**. In this manner, a data path is shown in FIG. 2 between the aforementioned unidirectional input and output via a dedicated link **209** from the analog interface **201** to serial communication section **205**, thereafter to the proces-

sor **204**, and then to the RF transmitter **206**. As such, in one embodiment, via the data path described above, the transmitter unit **102** is configured to transmit to the primary receiver unit **104** (FIG. 1), via the communication link **103** (FIG. 1), processed and encoded data signals received from the sensor **101** (FIG. 1). Additionally, the unidirectional communication data path between the analog interface **201** and the RF transmitter **206** discussed above allows for the configuration of the transmitter unit **102** for operation upon completion of the manufacturing process as well as for direct communication for diagnostic and testing purposes.

As discussed above, the transmitter processor **204** is configured to transmit control signals to the various sections of the transmitter unit **102** during the operation of the transmitter unit **102**. In one embodiment, the transmitter processor **204** also includes a memory (not shown) for storing data such as the identification information for the transmitter unit **102**, as well as the data signals received from the sensor **101**. The stored information may be retrieved and processed for transmission to the primary receiver unit **104** under the control of the transmitter processor **204**. Furthermore, the power supply **207** may include a commercially available battery.

The transmitter unit **102** is also configured such that the power supply section **207** is capable of providing power to the transmitter for a minimum of about three months of continuous operation after having been stored for about eighteen months in a low-power (non-operating) mode. In one embodiment, this may be achieved by the transmitter processor **204** operating in low power modes in the non-operating state, for example, drawing no more than approximately 1 μ A of current. Indeed, in one embodiment, the final step during the manufacturing process of the transmitter unit **102** may place the transmitter unit **102** in the lower power, non-operating state (i.e., post-manufacture sleep mode). In this manner, the shelf life of the transmitter unit **102** may be significantly improved. Moreover, as shown in FIG. 2, while the power supply unit **207** is shown as coupled to the processor **204**, and as such, the processor **204** is configured to provide control of the power supply unit **207**, it should be noted that within the scope of the present invention, the power supply unit **207** is configured to provide the necessary power to each of the components of the transmitter unit **102** shown in FIG. 2.

Referring back to FIG. 2, the power supply section **207** of the transmitter unit **102** in one embodiment may include a rechargeable battery unit that may be recharged by a separate power supply recharging unit (for example, provided in the receiver unit **104**) so that the transmitter unit **102** may be powered for a longer period of usage time. Moreover, in one embodiment, the transmitter unit **102** may be configured without a battery in the power supply section **207**, in which case the transmitter unit **102** may be configured to receive power from an external power supply source (for example, a battery) as discussed in further detail below.

Referring yet again to FIG. 2, the temperature detection section **203** of the transmitter unit **102** is configured to monitor the temperature of the skin near the sensor insertion site. The temperature reading is used to adjust the analyte readings obtained from the analog interface **201**. The RF transmitter **206** of the transmitter unit **102** may be configured for operation in the frequency band of 315 MHz to 322 MHz, for example, in the United States. Further, in one embodiment, the RF transmitter **206** is configured to modulate the carrier frequency by performing Frequency Shift Keying and Manchester encoding. In one embodiment, the

data transmission rate is 19,200 symbols per second, with a minimum transmission range for communication with the primary receiver unit 104.

Referring yet again to FIG. 2, also shown is a leak detection circuit 214 coupled to the guard contact (G) 211 and the processor 204 in the transmitter unit 102 of the data monitoring and management system 100. The leak detection circuit 214 in accordance with one embodiment of the present invention may be configured to detect leakage current in the sensor 101 to determine whether the measured sensor data are corrupt or whether the measured data from the sensor 101 is accurate.

Additional detailed description of the continuous analyte monitoring system, its various components including the functional descriptions of the transmitter are provided in U.S. Pat. No. 6,175,752 issued Jan. 16, 2001 entitled "Analyte Monitoring Device and Methods of Use", and in U.S. patent application Ser. No. 10/745,878 filed Dec. 26, 2003, now U.S. Pat. No. 7,811,231, entitled "Continuous Glucose Monitoring System and Methods of Use", each assigned to the Assignee of the present application, the disclosure of each of which are incorporated herein by reference for all purposes.

FIG. 3 is a block diagram of the receiver/monitor unit of the data monitoring and management system shown in FIG. 1 in accordance with one embodiment of the present invention. Referring to FIG. 3, the primary receiver unit 104 includes a blood glucose test strip interface 301, an RF receiver 302, an input 303, a temperature detection section 304, and a clock 305, each of which is operatively coupled to a receiver processor 307. As can be further seen from the Figure, the primary receiver unit 104 also includes a power supply 306 operatively coupled to a power conversion and monitoring section 308. Further, the power conversion and monitoring section 308 is also coupled to the receiver processor 307. Moreover, also shown are a receiver serial communication section 309, and an output 310, each operatively coupled to the receiver processor 307.

In one embodiment, the test strip interface 301 includes a glucose level testing portion to receive a manual insertion of a glucose test strip, and thereby determine and display the glucose level of the test strip on the output 310 of the primary receiver unit 104. This manual testing of glucose can be used to calibrate sensor 101. The RF receiver 302 is configured to communicate, via the communication link 103 (FIG. 1) with the RF transmitter 206 of the transmitter unit 102, to receive encoded data signals from the transmitter unit 102 for, among others, signal mixing, demodulation, and other data processing. The input 303 of the primary receiver unit 104 is configured to allow the user to enter information into the primary receiver unit 104 as needed. In one aspect, the input 303 may include one or more keys of a keypad, a touch-sensitive screen, or a voice-activated input command unit. The temperature detection section 304 is configured to provide temperature information of the primary receiver unit 104 to the receiver processor 307, while the clock 305 provides, among others, real time information to the receiver processor 307.

Each of the various components of the primary receiver unit 104 shown in FIG. 3 is powered by the power supply 306 which, in one embodiment, includes a battery. Furthermore, the power conversion and monitoring section 308 is configured to monitor the power usage by the various components in the primary receiver unit 104 for effective power management and to alert the user, for example, in the event of power usage which renders the primary receiver unit 104 in sub-optimal operating conditions. An example of

such sub-optimal operating condition may include, for example, operating the vibration output mode (as discussed below) for a period of time thus substantially draining the power supply 306 while the processor 307 (thus, the primary receiver unit 104) is turned on. Moreover, the power conversion and monitoring section 308 may additionally be configured to include a reverse polarity protection circuit such as a field effect transistor (FET) configured as a battery activated switch.

The serial communication section 309 in the primary receiver unit 104 is configured to provide a bi-directional communication path from the testing and/or manufacturing equipment for, among others, initialization, testing, and configuration of the primary receiver unit 104. Serial communication section 309 can also be used to upload data to a computer, such as time-stamped blood glucose data. The communication link with an external device (not shown) can be made, for example, by cable, infrared (IR) or RF link. The output 310 of the primary receiver unit 104 is configured to provide, among others, a graphical user interface (GUI) such as a liquid crystal display (LCD) for displaying information. Additionally, the output 310 may also include an integrated speaker for outputting audible signals as well as to provide vibration output as commonly found in handheld electronic devices, such as mobile telephones presently available. In a further embodiment, the primary receiver unit 104 also includes an electro-luminescent lamp configured to provide backlighting to the output 310 for output visual display in dark ambient surroundings.

Referring back to FIG. 3, the primary receiver unit 104 in one embodiment may also include a storage section such as a programmable, non-volatile memory device as part of the processor 307, or provided separately in the primary receiver unit 104, operatively coupled to the processor 307. The processor 307 is further configured to perform Manchester decoding as well as error detection and correction upon the encoded data signals received from the transmitter unit 102 via the communication link 103.

In a further embodiment, the one or more of the transmitter unit 102, the primary receiver unit 104, secondary receiver unit 106, or the data processing terminal/infusion section 105 may be configured to receive the blood glucose value wirelessly over a communication link from, for example, a glucose meter. In still a further embodiment, the user or patient manipulating or using the analyte monitoring system 100 (FIG. 1) may manually input the blood glucose value using, for example, a user interface (for example, a keyboard, keypad, and the like) incorporated in the one or more of the transmitter unit 102, the primary receiver unit 104, secondary receiver unit 106, or the data processing terminal/infusion section 105.

FIG. 4 is a schematic of the dynamic multi-stage signal amplification in the transmitter unit of the data monitoring and management system shown in FIG. 1 in accordance with one embodiment of the present invention. Referring to FIG. 4, there is provided in one embodiment a transimpedance amplifier 420 whose output terminal 423 is coupled to a first input terminal 411 of the analog to digital converter (ADC) 410 in the analog interface 201 (FIG. 2) of the transmitter unit 102. Further shown in FIG. 4, the monitored analyte sensor signal from the sensor 101 is provided to an inverting input terminal 421 of the transimpedance amplifier 420. The sensor signal in FIG. 4 is shown as a signal source 440. Also shown in FIG. 4 is resistor 460. Furthermore, a noninverting input terminal 422 of the transimpedance amplifier 420 is provided with a reference voltage signal from a reference signal source Vref 450. In one embodiment, the reference

voltage signal may be approximately 1.012 volts. However, based upon the component tolerance, and design configuration, other suitable reference voltage signals may be used.

In one aspect, based on the input analyte sensor signal from the signal source **440** and the reference signal **Vref 450**, the transimpedance amplifier **420** may be in one embodiment configured to convert the received current signal representing the monitored or detected analyte level, and to convert the current signal to a corresponding voltage signal which is provided to the output terminal **423** of the transimpedance amplifier **420**. Further, as shown in FIG. 4 the monitored analyte voltage signal from the output terminal **423** of the transimpedance amplifier **420** is provided to the first input terminal **411** (Channel 1) of the ADC **410**.

Referring again to FIG. 4, a second amplifier **430** is provided in one embodiment whose noninverting input terminal **431** is coupled to the output terminal **423** of the transimpedance amplifier **420** to receive the output voltage signal corresponding to the monitored analyte level, while an inverting input terminal **432** of the second amplifier **430** is coupled in one embodiment to the reference signal **Vref** source **450**. Moreover, output terminal **433** of the second amplifier is coupled in one embodiment to a second input terminal **412** (Channel 2) of the ADC **410**. In operation, the second amplifier **430** may be configured to step up the output signal of the transimpedance amplifier **410** by a predetermined factor (for example, a factor of 2), and to provide the stepped up signal to the analog to digital converter (ADC) **410**.

Referring back to FIG. 4, the analog to digital converter (ADC) **410** of the analog interface **201** (FIG. 2) of the transmitter unit **102** (FIG. 1) in one embodiment may be configured to detect signals at both the first and second input terminals or channels **411**, **412**, and based on one or more predetermined process or routine, the voltage signal at one of the first or the second input terminals or channels **411**, **412** is used by the ADC **410** for further processing as corresponding to the monitored analyte level from the sensor **101** (FIG. 1). That is, in one embodiment, depending upon the signal resolution corresponding to the analyte level monitored, the ADC **410** may be configured to select one of the output signals from the transimpedance amplifier **420** or the second amplifier **430** for further processing.

For example, when the signal received at the second input terminal **412** of the ADC **410** exceeds a predetermined threshold value, the input signal at the first input terminal **411** may be used. More specifically, in one embodiment, the ADC **410** may be configured to process the signals at the second input terminal **412** (Channel 2) since it has a higher resolution compared to the signal at the first input terminal **411** received from the transimpedance amplifier **420**. When the signal received at the second input terminal **412** exceeds a predetermined threshold level (for example, based on the tolerance level of the analog to digital converter (ADC) **410**), the voltage signal received at the first input terminal **411** from the transimpedance amplifier **420** may be used to convert to a corresponding digital signal representing the monitored analyte level detected by the sensor **101** (FIG. 1).

Referring back to FIG. 4, in one embodiment, the analog to digital converter (ADC) **410** may include a 12 bit A/D converter configured to support up to approximately 4,096 bits or ADC counts. In this case, in one embodiment, when the signal at the second input terminal **412** of the ADC **410** approaches approximately 4,000 bits or ADC counts, for example, the processor **204** (FIG. 2) of the transmitter unit **102** may be configured to switch from the second input terminal **412** to the first input terminal **411**, to use the output

signal from the transimpedance amplifier **420**. In this manner, in one embodiment, the processor **204** of the transmitter unit **102** may be configured to monitor the signal levels at the two input terminals **411**, **412** of the ADC **410**, and when the signal level or ADC count associated with the output signal from the second amplifier **430** provided at the second input terminal **412** of the ADC **410** exceeds the predetermined threshold (for example, 4,000 bits or ADC count), the processor **204** may be configured to switch over to the output signal of the transimpedance amplifier **410** provided on the first input terminal **411** of the ADC **410** for further processing.

In the manner described above, the dynamic multi-stage amplifier configuration in one embodiment may be configured to support variations in the analyte sensor sensitivities due to, for example, manufacturing variations, among others, while maintaining an acceptable or desirable sensor signal resolution. For example, in one embodiment, high sensitivity sensors may be configured for use with the full scale or range (for example, up to approximately 150 nA corresponding to the supported approximately 500 mg/dL glucose level) associated with the transimpedance amplifier **420** output signal provided to the first input terminal **411** (Channel 1) of the analog to digital converter (ADC) **410**, while low sensitivity sensors may be associated with the second amplifier **430** output signal (for example, full scale current signal level of approximately 75 nA corresponding to the supported approximately 500 mg/dL glucose level) provided to the second input terminal **412** (Channel 2) of the analog to digital converter (ADC) **410**.

For example, as discussed above, in one embodiment, the processor **204** of the transmitter unit **102** may be configured to monitor the signals at the two input terminals **411**, **412** of the ADC **410**, and determine, that if the received signal level does not have sufficient resolution to convert to the desired resolution of the digital signal (for example, 12 bits for the ADC **410**) corresponding to the monitored analyte level associated with the sensor **101**, the processor **204** may be configured to dynamically toggle or switch from using the voltage signal received from one of the two input terminals **411**, **412**, to using the voltage signal from the other one of the two input terminals **411**, **412** to provide a dynamic range of tolerance level for the sensor sensitivities.

Accordingly, an apparatus in one embodiment includes a first amplifier having at least one input terminal and an output terminal, the at least one input terminal coupled to a signal source, the output terminal configured to provide a first output signal, a second amplifier having at least one input terminal and an output terminal, the at least one input terminal coupled to the output terminal of the first amplifier, the output terminal of the second amplifier configured to provide a second output signal, a processor operatively coupled to receive the first output signal and the second output signal, where the first output signal is a predetermined ratio of the second output signal, and further, where the first output signal and the second output signal are associated with a monitored analyte level of a user.

In one aspect, the first amplifier may include a transimpedance amplifier.

The monitored analyte level may include glucose level.

Also, the at least one input terminal of the first amplifier may include an inverting input terminal, and, also may include a reference signal source coupled to a noninverting input terminal of the first amplifier.

In a further aspect, the second amplifier may include a gain of approximately two.

In still another aspect, the first output signal may be associated with a signal level from the signal source.

The apparatus may also include an analog to digital converter coupled to the output terminals of the first and second amplifiers, where the analog to digital (A/D) converter may include a 12 bit A/D converter.

The apparatus in another embodiment may include a processor operatively coupled to the A/D converter for processing the one or more signals received at the one or more first amplifier output terminal and the second amplifier output terminal.

Moreover, the processor may be configured to compare the one or more signals received at the one or more first amplifier output terminal and the second amplifier output terminal to a predetermined threshold value, which, in one embodiment may include approximately 4,000 bits (or analog to digital converter (ADC) counts).

Still further, the processor may be configured to process a signal associated with one of the one or more signals received at the one or more first amplifier output terminal and the second amplifier output terminal when another signal associated with the other one of the one or more signals received at the one or more first amplifier output terminal and the second amplifier output terminal exceeds the predetermined threshold value.

A method in accordance with another embodiment includes receiving a first signal having a first signal resolution and associated with a monitored analyte level of a user, receiving a second signal having a second signal resolution and associated with the monitored analyte level of the user, comparing the received first signal to a predetermined threshold level, and processing one of the received first or second signals based on the comparing step.

When the received first signal does not exceed the predetermined threshold level, further including processing the first signal. On the other hand, when the received first signal exceeds the predetermined threshold level, further including processing the second signal.

A data processing device in accordance with still another embodiment includes a multi stage amplifier unit configured to receive a signal and to generate a plurality of amplifier unit output signals each corresponding to a monitored analyte level of a patient, an analog to digital (A/D) conversion unit operatively coupled to the multi-stage amplifier unit configured to digitally convert the plurality of amplifier unit output signals, and a processor unit operatively coupled to the A/D conversion unit, the processor unit configured to process one of the plurality of digitally converted amplifier unit output signals.

The device in another aspect may include a data communication unit operatively coupled to the processor unit, and configured to transmit the digitally converted and processed amplifier unit output signal.

The data communication unit may include an RF transmitter for wireless data transmission to a remote device such as, for example, a data receiver unit, data processing terminal, an infusion device or the like configured for RF communication.

Various other modifications and alterations in the structure and method of operation of this invention will be apparent to those skilled in the art without departing from the scope and spirit of the invention. Although the invention has been described in connection with specific preferred embodiments, it should be understood that the invention as claimed should not be unduly limited to such specific embodiments. It is intended that the following claims define

the scope of the present invention and that structures and methods within the scope of these claims and their equivalents be covered thereby.

What is claimed is:

1. A method of processing signals from an analyte sensor, comprising:

coupling a first amplifier to a second amplifier and a signal source;

determining that a first signal at an output terminal of the second amplifier exceeds a converter tolerance value; and

processing a second signal at the output terminal of the second amplifier when the first signal at the output terminal of the second amplifier exceeds the converter tolerance value.

2. The method of claim 1, wherein the first amplifier comprises a transimpedance amplifier.

3. The method of claim 2, wherein the transimpedance amplifier is coupled to an analog to digital converter, and wherein the converter tolerance value corresponds to a tolerance level of the analog to digital converter.

4. The method of claim 1, wherein the first amplifier has a higher resolution than the second amplifier.

5. The method of claim 1, wherein the first signal and the second signal are from an in vivo analyte sensor.

6. The method of claim 5, wherein the in vivo analyte sensor comprises a plurality of electrodes including a working electrode comprising an analyte-responsive enzyme bonded to a polymer disposed on the working electrode.

7. The method of claim 6, wherein the analyte-responsive enzyme is chemically bonded to the polymer.

8. The method of claim 6, wherein the working electrode further comprises a mediator.

9. The method of claim 5, wherein the in vivo analyte sensor comprises a plurality of electrodes including a working electrode comprising a mediator bonded to a polymer disposed on the working electrode.

10. The method of claim 9, wherein the mediator is chemically bonded to the polymer.

11. An apparatus, comprising:

a first amplifier operatively coupled to a signal source; a second amplifier operatively coupled to the first amplifier, the second amplifier comprising an output terminal; and

a processing unit operatively coupled to one or more of the first amplifier and the second amplifier, the processing unit configured to:

determine that a first signal at the output terminal of the second amplifier exceeds a converter tolerance value; and

process a second signal at the output terminal of the second amplifier when the first signal at the output terminal of the second amplifier exceeds the converter tolerance value.

12. The apparatus of claim 11, wherein the first amplifier comprises a transimpedance amplifier.

13. The apparatus of claim 12, wherein the transimpedance amplifier is coupled to an analog to digital converter, and wherein the converter tolerance value corresponds to a tolerance level of the analog to digital converter.

14. The apparatus of claim 11, wherein the first amplifier has a higher resolution than the second amplifier.

15. The apparatus of claim 11, wherein the first signal and the second signal are sensor signals from an in vivo analyte sensor.

16. The apparatus of claim 15, wherein the in vivo analyte sensor comprises a plurality of electrodes including a work-

ing electrode comprising an analyte-responsive enzyme bonded to a polymer disposed on the working electrode.

17. The apparatus of claim 16, wherein the analyte-responsive enzyme is chemically bonded to the polymer.

18. The apparatus of claim 16, wherein the working 5 electrode further comprises a mediator.

19. The apparatus of claim 15, wherein the in vivo analyte sensor comprises a plurality of electrodes including a working electrode comprising a mediator bonded to a polymer disposed on the working electrode. 10

20. The apparatus of claim 19, wherein the mediator is chemically bonded to the polymer.

* * * * *

专利名称(译)	用于在医疗设备中提供动态多级信号放大的方法和装置		
公开(公告)号	US10194846	公开(公告)日	2019-02-05
申请号	US15/686156	申请日	2017-08-25
[标]申请(专利权)人(译)	雅培糖尿病护理公司		
申请(专利权)人(译)	雅培糖尿病INC.		
当前申请(专利权)人(译)	雅培糖尿病INC.		
[标]发明人	FENNELL MARTIN J		
发明人	FENNELL, MARTIN J.		
IPC分类号	A61B5/145 A61B5/00 A61M5/172 A61B5/1486		
CPC分类号	A61B5/14532 A61B5/002 A61B5/0004 A61B5/14546 A61B5/14865 A61B5/7246 A61B5/7475 A61M5/1723 A61B5/7225 A61B2560/045 A61B2560/0209 A61B2560/0252		
优先权	60/911866 2007-04-14 US		
其他公开文献	US20170354356A1		
外部链接	Espacenet		

摘要(译)

提供了用于在医疗遥测系统中提供多级信号放大的方法和装置。

