



US009962091B2

(12) **United States Patent**
Jin et al.

(10) **Patent No.:** **US 9,962,091 B2**
(45) **Date of Patent:** **May 8, 2018**

(54) **CONTINUOUS GLUCOSE MONITORING
SYSTEM AND METHODS OF USE**

(56) **References Cited**

U.S. PATENT DOCUMENTS

(71) Applicant: **Abbott Diabetes Care Inc.**, Alameda,
CA (US)

3,260,656 A 7/1966 Ross, Jr.
3,304,413 A 2/1967 Lehmann et al.
(Continued)

(72) Inventors: **Robert Y. Jin**, Irvine, CA (US); **Mark
Kent Sloan**, Redwood City, CA (US)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Abbott Diabetes Care Inc.**, Alameda,
CA (US)

DE 2903216 8/1979
DE 227029 9/1985
(Continued)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 529 days.

OTHER PUBLICATIONS

(21) Appl. No.: **14/148,034**

(22) Filed: **Jan. 6, 2014**

(65) **Prior Publication Data**

US 2014/0121477 A1 May 1, 2014

Abruna, H. D., et al., "Rectifying Interfaces Using Two-Layer Films
of Electrochemically Polymerized Vinylpyridine and
Vinylbipyridine Complexes of Ruthenium and Iron on Electrodes",
Journal of the American Chemical Society, vol. 103, No. 1, 1981,
pp. 1-5.

(Continued)

Primary Examiner — David C Eastwood

Assistant Examiner — Shirley Jian

(74) *Attorney, Agent, or Firm* — Jackson & Co., LLP

Related U.S. Application Data

(63) Continuation of application No. 13/481,256, filed on
May 25, 2012, now Pat. No. 8,622,903, which is a
(Continued)

(51) **Int. Cl.**
A61B 5/00 (2006.01)
A61B 5/01 (2006.01)
A61B 5/145 (2006.01)


(52) **U.S. Cl.**
CPC **A61B 5/01** (2013.01); **A61B 5/0002**
(2013.01); **A61B 5/14532** (2013.01); **A61B**
2562/08 (2013.01)

(58) **Field of Classification Search**
USPC 709/203-204, 218
See application file for complete search history.

(57) **ABSTRACT**

A continuous glucose monitoring system including a sensor
configured to detect one or more glucose levels, a transmitter
operatively coupled to the sensor, the transmitter configured
to receive the detected one or more glucose levels, the
transmitter further configured to transmit signals corre-
sponding to the detected one or more glucose levels, and a
receiver operatively coupled to the transmitter configured to
receive transmitted signals corresponding to the detected
one or more glucose levels, and methods thereof, are dis-
closed. In one aspect, the transmitter may be configured to
transmit a current data point and at least one previous data
point, the current data point and the at least one previous
data point corresponding to the detected one or more glucose
levels.

20 Claims, 6 Drawing Sheets

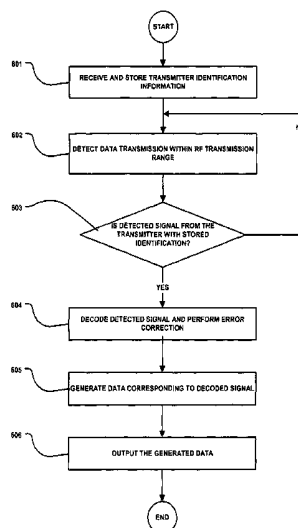

Related U.S. Application Data

continuation of application No. 12/902,138, filed on Oct. 11, 2010, now Pat. No. 8,187,183, which is a continuation of application No. 10/745,878, filed on Dec. 26, 2003, now Pat. No. 7,811,231.

- (60) Provisional application No. 60/437,374, filed on Dec. 31, 2002.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,651,318 A	3/1972	Czekajewski	4,461,691 A	7/1984	Frank
3,653,841 A	4/1972	Klein	4,464,170 A	8/1984	Clemens et al.
3,698,386 A	10/1972	Fried	4,467,811 A	8/1984	Clark, Jr.
3,719,564 A	3/1973	Lilly, Jr. et al.	4,469,110 A	9/1984	Slama
3,768,014 A	10/1973	Smith et al.	4,475,901 A	10/1984	Kraegen et al.
3,776,832 A	12/1973	Oswin et al.	4,477,314 A	10/1984	Richter et al.
3,785,939 A	1/1974	Hsu	4,478,976 A	10/1984	Goertz et al.
3,912,614 A	10/1975	Spracklen et al.	4,483,924 A	11/1984	Tsuji et al.
3,919,051 A	11/1975	Koch et al.	4,484,987 A	11/1984	Gough
3,926,760 A	12/1975	Allen et al.	4,494,950 A	1/1985	Fischell
3,972,320 A	8/1976	Kalman	4,512,348 A	4/1985	Uchigaki et al.
3,979,274 A	9/1976	Newman	RE31,916 E	6/1985	Oswin et al.
4,008,717 A	2/1977	Kowarski	4,522,690 A	6/1985	Venkatsetty
4,016,866 A	4/1977	Lawton	4,524,114 A	6/1985	Samuels et al.
4,031,449 A	6/1977	Trombly	4,526,661 A	7/1985	Steckhan et al.
4,036,749 A	7/1977	Anderson	4,527,240 A	7/1985	Kvitash
4,055,175 A	10/1977	Clemens et al.	4,534,356 A	8/1985	Papadakis
4,059,406 A	11/1977	Fleet	4,538,616 A	9/1985	Rogoff
4,076,596 A	2/1978	Connery et al.	4,543,955 A	10/1985	Schroepfel
4,098,574 A	7/1978	Dappen	4,545,382 A	10/1985	Higgins et al.
4,100,048 A	7/1978	Pompei et al.	4,552,840 A	11/1985	Riffer
4,129,128 A	12/1978	McFarlane	4,560,534 A	12/1985	Kung et al.
4,151,845 A	5/1979	Clemens	4,569,589 A	2/1986	Neufeld
4,154,231 A	5/1979	Russell	4,571,292 A	2/1986	Liu et al.
4,168,205 A	9/1979	Danniger et al.	4,573,994 A	3/1986	Fischell et al.
4,172,770 A	10/1979	Semersky et al.	4,581,336 A	4/1986	Malloy et al.
4,178,916 A	12/1979	McNamara	4,583,035 A	4/1986	Sloan
4,206,755 A	6/1980	Klein	4,595,011 A	6/1986	Phillips
4,224,125 A	9/1980	Nakamura et al.	4,595,479 A	6/1986	Kimura et al.
4,240,438 A	12/1980	Updike et al.	4,619,754 A	10/1986	Niki et al.
4,240,889 A	12/1980	Yoda et al.	4,619,793 A	10/1986	Lee
4,245,634 A	1/1981	Albisser et al.	4,627,445 A	12/1986	Garcia et al.
4,247,297 A	1/1981	Berti et al.	4,627,908 A	12/1986	Miller
4,271,449 A	6/1981	Grogan	4,633,878 A	1/1987	Bombardien
4,276,888 A	7/1981	Smith et al.	4,633,881 A	1/1987	Moore et al.
4,318,784 A	3/1982	Higgins et al.	4,637,403 A	1/1987	Garcia et al.
4,327,725 A	5/1982	Cortese et al.	RE32,361 E	2/1987	Duggan
4,331,869 A	5/1982	Rollo	4,648,408 A	3/1987	Hutcheson et al.
4,340,458 A	7/1982	Lerner et al.	4,650,547 A	3/1987	Gough
4,344,438 A	8/1982	Schultz	4,653,513 A	3/1987	Dombrowski
4,352,960 A	10/1982	Dormer et al.	4,654,197 A	3/1987	Lilja et al.
4,356,074 A	10/1982	Johnson	4,655,880 A	4/1987	Liu
4,365,637 A	12/1982	Johnson	4,655,885 A	4/1987	Hill et al.
4,366,033 A	12/1982	Richter et al.	4,658,463 A	4/1987	Sugita et al.
4,375,399 A	3/1983	Havas et al.	4,671,288 A	6/1987	Gough
4,384,586 A	5/1983	Christiansen	4,674,652 A	6/1987	Aten et al.
4,390,621 A	6/1983	Bauer	4,679,562 A	7/1987	Luksha
4,392,933 A	7/1983	Nakamura et al.	4,680,268 A	7/1987	Clark, Jr.
4,401,122 A	8/1983	Clark, Jr.	4,682,602 A	7/1987	Prohaska
4,404,066 A	9/1983	Johnson	4,684,537 A	8/1987	Graetzel et al.
4,407,959 A	10/1983	Tsuji et al.	4,685,463 A	8/1987	Williams
4,417,588 A	11/1983	Houghton et al.	4,686,624 A	8/1987	Blum et al.
4,418,148 A	11/1983	Oberhardt	4,703,324 A	10/1987	White
4,420,564 A	12/1983	Tsuji et al.	4,703,756 A	11/1987	Gough et al.
4,425,920 A	1/1984	Bourland et al.	4,714,462 A	12/1987	DiDomenico
4,427,004 A	1/1984	Miller et al.	4,718,893 A	1/1988	Dorman
4,427,770 A	1/1984	Chen et al.	4,721,601 A	1/1988	Wrighton et al.
4,431,004 A	2/1984	Bessman et al.	4,721,677 A	1/1988	Clark, Jr.
4,436,094 A	3/1984	Cerami	4,726,378 A	2/1988	Kaplan
4,440,175 A	4/1984	Wilkins	4,726,716 A	2/1988	McGuire
4,444,892 A	4/1984	Malmros	4,731,726 A	3/1988	Allen, III
4,445,090 A	4/1984	Melocik et al.	4,749,985 A	6/1988	Corsberg
4,450,842 A	5/1984	Zick et al.	4,750,496 A	6/1988	Reinhardt
4,458,686 A	7/1984	Clark, Jr.	4,757,022 A	7/1988	Shults et al.
			4,758,323 A	7/1988	Davis et al.
			4,759,371 A	7/1988	Franetzki
			4,759,828 A	7/1988	Young et al.
			4,764,416 A	8/1988	Ueyama et al.
			4,776,944 A	10/1988	Janata et al.
			4,777,953 A	10/1988	Ash et al.
			4,779,618 A	10/1988	Mund et al.
			4,781,798 A	11/1988	Gough
			4,784,736 A	11/1988	Lonsdale et al.
			4,795,707 A	1/1989	Niiyama et al.
			4,796,634 A	1/1989	Huntsman et al.
			4,803,625 A	2/1989	Fu et al.
			4,805,624 A	2/1989	Yao et al.
			4,813,424 A	3/1989	Wilkins
			4,815,469 A	3/1989	Cohen et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

4,820,399	A	4/1989	Senda et al.	5,049,487	A	9/1991	Phillips et al.
4,822,337	A	4/1989	Newhouse et al.	5,050,612	A	9/1991	Matsumura
4,830,959	A	5/1989	McNeil et al.	5,051,688	A	9/1991	Murase et al.
4,832,797	A	5/1989	Vadgama et al.	5,055,171	A	10/1991	Peck
4,835,372	A	5/1989	Gombrich et al.	5,058,592	A	10/1991	Whisler
RE32,947	E	6/1989	Dormer et al.	5,061,941	A	10/1991	Lizzi et al.
4,837,049	A	6/1989	Byers et al.	5,063,081	A	11/1991	Cozzette et al.
4,840,893	A	6/1989	Hill et al.	5,068,536	A	11/1991	Rosenthal
RE32,974	E	7/1989	Porat et al.	5,070,535	A	12/1991	Hochmair et al.
4,844,076	A	7/1989	Lesho et al.	5,073,500	A	12/1991	Saito et al.
4,845,035	A	7/1989	Fanta et al.	5,077,476	A	12/1991	Rosenthal
4,847,785	A	7/1989	Stephens	5,078,854	A	1/1992	Burgess et al.
4,848,351	A	7/1989	Finch	5,082,550	A	1/1992	Rishpon et al.
4,854,322	A	8/1989	Ash et al.	5,082,786	A	1/1992	Nakamoto
4,856,340	A	8/1989	Garrison	5,084,828	A	1/1992	Kaufman et al.
4,857,713	A	8/1989	Brown	5,089,112	A	2/1992	Skotheim et al.
4,858,617	A	8/1989	Sanders	5,094,951	A	3/1992	Rosenberg
4,870,561	A	9/1989	Love et al.	5,095,904	A	3/1992	Seligman et al.
4,871,351	A	10/1989	Feingold	5,096,560	A	3/1992	Takai et al.
4,871,440	A	10/1989	Nagata et al.	5,096,836	A	3/1992	Macho et al.
4,874,499	A	10/1989	Smith et al.	5,101,814	A	4/1992	Palti
4,874,500	A	10/1989	Madou et al.	5,106,365	A	4/1992	Hernandez
4,890,620	A	1/1990	Gough	5,108,564	A	4/1992	Szuminsky et al.
4,890,621	A	1/1990	Hakky	5,109,850	A	5/1992	Blanco et al.
4,894,137	A	1/1990	Takizawa et al.	5,111,539	A	5/1992	Hiruta et al.
4,897,162	A	1/1990	Lewandowski et al.	5,111,818	A	5/1992	Suzuji et al.
4,897,173	A	1/1990	Nankai et al.	5,112,455	A	5/1992	Cozzette et al.
4,899,839	A	2/1990	Dessertine et al.	5,114,678	A	5/1992	Crawford et al.
4,909,908	A	3/1990	Ross et al.	5,120,420	A	6/1992	Nankai et al.
4,911,794	A	3/1990	Parce et al.	5,120,421	A	6/1992	Glass et al.
4,917,800	A	4/1990	Lonsdale et al.	5,122,925	A	6/1992	Inpyn
4,919,141	A	4/1990	Zier et al.	5,124,661	A	6/1992	Zellin et al.
4,919,767	A	4/1990	Vadgama et al.	5,126,034	A	6/1992	Carter et al.
4,920,969	A	5/1990	Suzuki	5,126,247	A	6/1992	Palmer et al.
4,920,977	A	5/1990	Haynes	5,130,009	A	7/1992	Marsoner et al.
4,923,586	A	5/1990	Katayama et al.	5,133,856	A	7/1992	Yamaguchi et al.
4,925,268	A	5/1990	Iyer et al.	5,134,391	A	7/1992	Okada
4,927,516	A	5/1990	Yamaguchi et al.	5,135,003	A	8/1992	Souma
4,931,795	A	6/1990	Gord	5,135,004	A	8/1992	Adams et al.
4,934,369	A	6/1990	Maxwell	5,139,023	A	8/1992	Stanley et al.
4,935,105	A	6/1990	Churchouse	5,140,393	A	8/1992	Hijikihigawa et al.
4,935,345	A	6/1990	Guibeaue et al.	5,141,868	A	8/1992	Shanks et al.
4,936,956	A	6/1990	Wrighton	5,161,532	A	11/1992	Joseph
4,938,860	A	7/1990	Wogoman	5,165,407	A	11/1992	Wilson et al.
4,942,127	A	7/1990	Wada et al.	5,168,046	A	12/1992	Hamamoto et al.
4,944,299	A	7/1990	Silvian	5,174,291	A	12/1992	Schoonen et al.
4,945,045	A	7/1990	Forrest et al.	5,176,644	A	1/1993	Srisathapat et al.
4,950,378	A	8/1990	Nagara	5,176,662	A	1/1993	Bartholomew et al.
4,953,552	A	9/1990	DeMarzo	5,182,707	A	1/1993	Cooper et al.
4,954,129	A	9/1990	Giuliani et al.	5,184,359	A	2/1993	Tsukamura et al.
4,957,115	A	9/1990	Selker	5,185,256	A	2/1993	Nankai et al.
4,958,632	A	9/1990	Duggan	5,190,041	A	3/1993	Palti
4,968,400	A	11/1990	Shimomura et al.	5,192,415	A	3/1993	Yoshioka et al.
4,969,468	A	11/1990	Byers et al.	5,192,416	A	3/1993	Wang et al.
4,970,145	A	11/1990	Bennetto et al.	5,193,539	A	3/1993	Schulman et al.
4,974,929	A	12/1990	Curry	5,193,540	A	3/1993	Schulman et al.
4,979,509	A	12/1990	Hakky	5,197,322	A	3/1993	Indravudh
4,986,271	A	1/1991	Wilkins	5,198,367	A	3/1993	Aizawa et al.
4,990,845	A	2/1991	Gord	5,200,051	A	4/1993	Cozzette et al.
4,991,582	A	2/1991	Byers et al.	5,202,261	A	4/1993	Musho et al.
4,994,068	A	2/1991	Hufnagie	5,205,920	A	4/1993	Oyama et al.
4,994,167	A	2/1991	Shults et al.	5,206,145	A	4/1993	Cattell
4,995,402	A	2/1991	Smith et al.	5,208,154	A	5/1993	Weaver et al.
5,000,180	A	3/1991	Kuypers et al.	5,209,229	A	5/1993	Gilli
5,001,054	A	3/1991	Wagner	5,215,887	A	6/1993	Saito
5,002,054	A	3/1991	Ash et al.	5,216,597	A	6/1993	Beckers
5,007,427	A	4/1991	Suzuki et al.	5,217,442	A	6/1993	Davis
5,016,172	A	5/1991	Dessertine	5,217,595	A	6/1993	Smith et al.
5,016,201	A	5/1991	Bryan et al.	5,227,042	A	7/1993	Zawodzinski et al.
5,019,974	A	5/1991	Beckers	5,229,282	A	7/1993	Yoshioka et al.
5,034,192	A	7/1991	Wrighton et al.	5,236,143	A	8/1993	Dragon
5,035,860	A	7/1991	Kleingeld et al.	5,237,993	A	8/1993	Skrabal
5,036,860	A	8/1991	Leigh et al.	5,245,314	A	9/1993	Kah et al.
5,036,861	A	8/1991	Sembrowich et al.	5,246,867	A	9/1993	Lakowicz et al.
5,037,527	A	8/1991	Hayashi et al.	5,250,439	A	10/1993	Musho et al.
				5,251,126	A	10/1993	Kahn et al.
				5,257,971	A	11/1993	Lord et al.
				5,257,980	A	11/1993	Van Antwerp et al.
				5,261,401	A	11/1993	Baker et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,262,035	A	11/1993	Gregg et al.	5,410,471	A	4/1995	Alyfuku et al.
5,262,305	A	11/1993	Heller et al.	5,410,474	A	4/1995	Fox
5,264,103	A	11/1993	Yoshioka et al.	5,411,647	A	5/1995	Johnson et al.
5,264,104	A	11/1993	Gregg et al.	5,413,690	A	5/1995	Kost et al.
5,264,105	A	11/1993	Gregg et al.	5,422,246	A	6/1995	Koopal et al.
5,264,106	A	11/1993	McAleer et al.	5,425,868	A	6/1995	Pedersen
5,265,888	A	11/1993	Yamamoto et al.	5,429,602	A	7/1995	Hauser
5,266,179	A	11/1993	Nankai et al.	5,431,160	A	7/1995	Wilkins
5,269,212	A	12/1993	Peters et al.	5,431,691	A	7/1995	Snell et al.
5,271,815	A	12/1993	Wong	5,431,921	A	7/1995	Thombre
5,272,060	A	12/1993	Hamamoto et al.	5,433,710	A	7/1995	Van Antwerp et al.
5,275,159	A	1/1994	Griebel	5,437,973	A	8/1995	Vadgama et al.
5,278,079	A	1/1994	Gubinski et al.	5,437,999	A	8/1995	Dieboid et al.
5,279,294	A	1/1994	Anderson	5,438,271	A	8/1995	White et al.
5,282,950	A	2/1994	Dietze et al.	5,438,983	A	8/1995	Falcone
5,284,156	A	2/1994	Schramm et al.	5,445,611	A	8/1995	Eppstein et al.
5,285,792	A	2/1994	Sjoquist et al.	5,445,920	A	8/1995	Saito
5,286,362	A	2/1994	Hoenes et al.	5,456,692	A	10/1995	Smith, Jr. et al.
5,286,364	A	2/1994	Yacynych et al.	5,456,940	A	10/1995	Funderburk
5,288,387	A	2/1994	Ito et al.	5,458,140	A	10/1995	Eppstein et al.
5,288,636	A	2/1994	Pollmann et al.	5,460,618	A	10/1995	Harreld
5,289,497	A	2/1994	Jackobson et al.	5,462,064	A	10/1995	D'Angelo et al.
5,291,887	A	3/1994	Stanley et al.	5,462,525	A	10/1995	Srisathapat et al.
5,293,546	A	3/1994	Tadros et al.	5,462,645	A	10/1995	Albery et al.
5,293,877	A	3/1994	O'Hara et al.	5,466,218	A	11/1995	Srisathapat et al.
5,299,571	A	4/1994	Mastrototaro	5,467,778	A	11/1995	Catt et al.
5,304,468	A	4/1994	Phillips et al.	5,469,846	A	11/1995	Khan
5,307,263	A	4/1994	Brown	5,472,317	A	12/1995	Field et al.
5,309,919	A	5/1994	Snell et al.	5,476,460	A	12/1995	Montalvo
5,310,885	A	5/1994	Maier et al.	5,477,855	A	12/1995	Schindler et al.
5,320,098	A	6/1994	Davidson	5,482,473	A	1/1996	Lord et al.
5,320,725	A	6/1994	Gregg et al.	5,484,404	A	1/1996	Schulman et al.
5,322,063	A	6/1994	Allen et al.	5,487,751	A	1/1996	Radons et al.
5,324,303	A	6/1994	Strong et al.	5,491,474	A	2/1996	Suni et al.
5,324,316	A	6/1994	Schulman et al.	5,494,562	A	2/1996	Maley et al.
5,326,449	A	7/1994	Cunningham	5,496,453	A	3/1996	Uenoyama et al.
5,333,615	A	8/1994	Craelius et al.	5,497,772	A	3/1996	Schulman et al.
5,337,258	A	8/1994	Dennis	5,499,243	A	3/1996	Hall
5,337,747	A	8/1994	Neftei	5,501,956	A	3/1996	Wada et al.
5,340,722	A	8/1994	Wolfbeis et al.	5,505,709	A	4/1996	Funderburk
5,342,408	A	8/1994	deCoriolis et al.	5,505,713	A	4/1996	Van Antwerp et al.
5,342,789	A	8/1994	Chick et al.	5,507,288	A	4/1996	Bocker et al.
5,352,348	A	10/1994	Young et al.	5,508,171	A	4/1996	Walling et al.
5,356,348	A	10/1994	Bellio et al.	5,509,410	A	4/1996	Hill et al.
5,356,786	A	10/1994	Heller et al.	5,514,103	A	5/1996	Srisathapat et al.
5,358,135	A	10/1994	Robbins et al.	5,514,253	A	5/1996	Davis et al.
5,358,514	A	10/1994	Schulman et al.	5,514,718	A	5/1996	Lewis et al.
5,360,404	A	11/1994	Novacek et al.	5,518,006	A	5/1996	Mawhirt et al.
5,364,797	A	11/1994	Olson et al.	5,520,787	A	5/1996	Hanagan et al.
5,366,609	A	11/1994	White et al.	5,522,865	A	6/1996	Schulman et al.
5,368,028	A	11/1994	Palti	5,525,511	A	6/1996	D'Costa
5,370,622	A	12/1994	Livingston et al.	5,526,120	A	6/1996	Jina et al.
5,371,687	A	12/1994	Holmes, II et al.	5,527,307	A	6/1996	Srisathapat et al.
5,371,734	A	12/1994	Fischer	5,529,676	A	6/1996	Maley et al.
5,371,787	A	12/1994	Hamilton	5,531,878	A	7/1996	Vadgama et al.
5,372,133	A	12/1994	Hogen Esch	5,532,686	A	7/1996	Urbas et al.
5,372,427	A	12/1994	Padovani et al.	5,538,511	A	7/1996	Van Antwerp et al.
5,376,070	A	12/1994	Purvis et al.	5,544,196	A	8/1996	Tiedmann, Jr. et al.
5,376,251	A	12/1994	Kaneko et al.	5,545,152	A	8/1996	Funderburk et al.
5,377,258	A	12/1994	Bro	5,545,191	A	8/1996	Mann et al.
5,378,628	A	1/1995	Gratzel et al.	5,549,113	A	8/1996	Halleck et al.
5,379,238	A	1/1995	Stark	5,549,115	A	8/1996	Morgan et al.
5,379,764	A	1/1995	Barnes et al.	5,552,027	A	9/1996	Birkle et al.
5,380,422	A	1/1995	Negishis et al.	5,554,166	A	9/1996	Lange et al.
5,382,346	A	1/1995	Uenoyama et al.	5,556,524	A	9/1996	Albers
5,387,327	A	2/1995	Khan	5,558,638	A	9/1996	Evers et al.
5,390,671	A	2/1995	Lord et al.	5,560,357	A	10/1996	Faupei et al.
5,391,250	A	2/1995	Cheney, II et al.	5,562,713	A	10/1996	Silvian
5,393,903	A	2/1995	Gratzel et al.	5,565,085	A	10/1996	Ikeda et al.
5,395,504	A	3/1995	Saurer et al.	5,567,302	A	10/1996	Song et al.
5,399,823	A	3/1995	McCusker	5,568,806	A	10/1996	Cheney, II et al.
5,400,782	A	3/1995	Beaubiah	5,569,186	A	10/1996	Lord et al.
5,400,794	A	3/1995	Gorman	5,569,212	A	10/1996	Brown
5,408,999	A	4/1995	Singh et al.	5,573,647	A	11/1996	Maley et al.
5,410,326	A	4/1995	Goldstein	5,575,895	A	11/1996	Ikeda et al.
				5,580,527	A	12/1996	Bell et al.
				5,580,794	A	12/1996	Allen
				5,581,206	A	12/1996	Chevallier et al.
				5,582,184	A	12/1996	Erickson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,582,697 A	12/1996	Ikeda et al.	5,741,211 A	4/1998	Renirie et al.
5,582,698 A	12/1996	Flaherty et al.	5,741,688 A	4/1998	Oxenboll et al.
5,584,813 A	12/1996	Livingston et al.	5,746,217 A	5/1998	Erickson et al.
5,586,553 A	12/1996	Halli et al.	5,750,926 A	5/1998	Schulman et al.
5,589,326 A	12/1996	Deng et al.	5,758,290 A	5/1998	Nealon et al.
5,593,852 A	1/1997	Heller et al.	5,769,873 A	6/1998	Zadeh
5,594,906 A	1/1997	Holmes, II et al.	5,770,028 A	6/1998	Maley et al.
5,596,150 A	1/1997	Arndt et al.	5,771,001 A	6/1998	Cobb
5,596,994 A	1/1997	Bro	5,771,890 A	6/1998	Tamada
5,600,301 A	2/1997	Robinson, III	5,772,586 A	6/1998	Heinonen et al.
5,601,435 A	2/1997	Quy	5,777,060 A	7/1998	Van Antwerp
5,601,694 A	2/1997	Maley et al.	5,779,665 A	7/1998	Mastrototaro et al.
5,605,152 A	2/1997	Slate et al.	5,781,024 A	7/1998	Blomberg et al.
5,609,575 A	3/1997	Larson et al.	5,782,814 A	7/1998	Brown et al.
5,611,900 A	3/1997	Worden et al.	5,785,681 A	7/1998	Indravudh
5,615,135 A	3/1997	Waclawsky et al.	5,786,439 A	7/1998	Van Antwerp et al.
5,615,671 A	4/1997	Schoonen et al.	5,786,584 A	7/1998	Button et al.
5,616,222 A	4/1997	Maley et al.	5,788,678 A	8/1998	Van Antwerp
5,617,851 A	4/1997	Lipkovker	5,791,344 A	8/1998	Schulman et al.
5,623,925 A	4/1997	Swenson et al.	5,792,117 A	8/1998	Brown
5,623,933 A	4/1997	Amano et al.	5,793,292 A	8/1998	Ivey
5,628,309 A	5/1997	Brown	5,800,420 A	9/1998	Gross et al.
5,628,310 A	5/1997	Rao et al.	5,804,048 A	9/1998	Wong et al.
5,628,324 A	5/1997	Sarbach	5,806,517 A	9/1998	Gerhardt et al.
5,628,890 A	5/1997	Carter et al.	5,807,315 A	9/1998	Van Antwerp et al.
5,629,981 A	5/1997	Nerlikar	5,807,375 A	9/1998	Gross et al.
5,634,468 A	6/1997	Platt et al.	5,814,599 A	9/1998	Mitragotri et al.
5,637,095 A	6/1997	Nason et al.	5,820,551 A	10/1998	Hill et al.
5,640,764 A	6/1997	Strojniak	5,820,570 A	10/1998	Erickson et al.
5,640,954 A	6/1997	Pfeiffer et al.	5,820,622 A	10/1998	Gross et al.
5,643,212 A	7/1997	Coutre et al.	5,822,715 A	10/1998	Worthington et al.
5,647,853 A	7/1997	Feldmann et al.	5,825,488 A	10/1998	Kohl et al.
5,650,062 A	7/1997	Ikeda et al.	5,827,179 A	10/1998	Lichter et al.
5,651,767 A	7/1997	Schulman et al.	5,827,183 A	10/1998	Kurnik et al.
5,651,869 A	7/1997	Yoshioka et al.	5,827,184 A	10/1998	Netherly et al.
5,653,239 A	8/1997	Pompei et al.	5,828,943 A	10/1998	Brown
5,659,454 A	8/1997	Vermesse	5,830,064 A	11/1998	Bradish et al.
5,660,163 A	8/1997	Schulman et al.	5,830,132 A	11/1998	Robinson
5,665,065 A	9/1997	Colman et al.	5,830,341 A	11/1998	Gilmartin
5,665,222 A	9/1997	Heller et al.	5,832,448 A	11/1998	Brown
5,667,983 A	9/1997	Abel et al.	5,834,224 A	11/1998	Ruger et al.
5,670,031 A	9/1997	Hintsche et al.	5,835,508 A	11/1998	Kushita
5,678,571 A	10/1997	Brown	5,837,454 A	11/1998	Cozzette et al.
5,679,690 A	10/1997	Andre et al.	5,837,546 A	11/1998	Allen et al.
5,680,858 A	10/1997	Hansen et al.	5,840,020 A	11/1998	Heinonen et al.
5,682,233 A	10/1997	Brinda	5,842,983 A	12/1998	Abel et al.
5,686,717 A	11/1997	Knowles et al.	5,843,140 A	12/1998	Strojniak
5,687,717 A	11/1997	Halpern et al.	5,846,702 A	12/1998	Deng et al.
5,690,893 A	11/1997	Ozawa et al.	5,846,744 A	12/1998	Athey et al.
5,693,577 A	12/1997	Krenik et al.	5,851,197 A	12/1998	Marano et al.
5,695,623 A	12/1997	Michel et al.	5,854,078 A	12/1998	Asher et al.
5,695,949 A	12/1997	Galen et al.	5,854,189 A	12/1998	Kruse et al.
5,701,894 A	12/1997	Cherry et al.	5,856,758 A	1/1999	Joffe et al.
5,704,922 A	1/1998	Brown	5,857,967 A	1/1999	Frid et al.
5,707,502 A	1/1998	McCaffrey et al.	5,857,983 A	1/1999	Douglas et al.
5,708,247 A	1/1998	McAleer et al.	5,860,917 A	1/1999	Comanor et al.
5,710,630 A	1/1998	Essenpreis et al.	5,862,803 A	1/1999	Besson et al.
5,711,001 A	1/1998	Bussan et al.	5,872,713 A	2/1999	Douglas et al.
5,711,297 A	1/1998	Iliff et al.	5,876,484 A	3/1999	Raskin et al.
5,711,861 A	1/1998	Ward et al.	5,879,163 A	3/1999	Brown et al.
5,711,862 A	1/1998	Sakoda et al.	5,879,311 A	3/1999	Duchon et al.
5,711,868 A	1/1998	Maley et al.	5,880,829 A	3/1999	Kauhaniemi et al.
5,718,234 A	2/1998	Warden et al.	5,882,494 A	3/1999	Van Antwerp
5,720,733 A	2/1998	Brown	5,885,211 A	3/1999	Eppstein et al.
5,720,862 A	2/1998	Hamamoto et al.	5,887,133 A	3/1999	Brown et al.
5,721,783 A	2/1998	Anderson	5,891,049 A	4/1999	Cyrus et al.
5,722,397 A	3/1998	Eppstein	5,897,493 A	4/1999	Brown
5,724,030 A	3/1998	Urbas et al.	5,898,025 A	4/1999	Burg et al.
5,727,548 A	3/1998	Hill et al.	5,899,855 A	5/1999	Brown
5,729,225 A	3/1998	Ledzius	5,913,310 A	6/1999	Brown
5,730,124 A	3/1998	Yamauchi	5,917,346 A	6/1999	Gord
5,730,654 A	3/1998	Brown	5,918,603 A	7/1999	Brown
5,733,313 A	3/1998	Barreras, Sr. et al.	5,919,141 A	7/1999	Money et al.
5,735,273 A	4/1998	Kurnik et al.	5,923,679 A	7/1999	Itoh et al.
5,735,285 A	4/1998	Albert et al.	5,925,021 A	7/1999	Castellano et al.
			5,931,791 A	8/1999	Saltzstein et al.
			5,933,136 A	8/1999	Brown
			5,935,224 A	8/1999	Svancarek et al.
			5,939,609 A	8/1999	Knapp et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,940,801 A	8/1999	Brown	6,093,167 A	7/2000	Houben et al.
5,942,979 A	8/1999	Luppino	6,093,172 A	7/2000	Funderburk et al.
5,945,345 A	8/1999	Blatt et al.	6,096,364 A	8/2000	Bok et al.
5,947,921 A	9/1999	Johnson et al.	6,097,480 A	8/2000	Kaplan
5,948,512 A	9/1999	Kubota et al.	6,097,831 A	8/2000	Wieck et al.
5,949,790 A	9/1999	Pehkonen et al.	6,099,484 A	8/2000	Douglas et al.
5,950,632 A	9/1999	Reber et al.	6,101,478 A	8/2000	Brown
5,951,300 A	9/1999	Brown	6,103,033 A	8/2000	Say et al.
5,951,485 A	9/1999	Cyrus et al.	6,106,780 A	8/2000	Douglas et al.
5,951,492 A	9/1999	Douglas et al.	6,110,148 A	8/2000	Brown et al.
5,951,521 A	9/1999	Mastrototaro et al.	6,110,152 A	8/2000	Kovelman
5,951,836 A	9/1999	McAleer et al.	6,113,578 A	9/2000	Brown
5,954,643 A	9/1999	Van Antwerp	6,119,028 A	9/2000	Schulman et al.
5,954,685 A	9/1999	Tierny	6,120,676 A	9/2000	Heller et al.
5,954,700 A	9/1999	Kovelman	6,121,009 A	9/2000	Heller et al.
5,956,501 A	9/1999	Brown	6,121,611 A	9/2000	Lindsay et al.
5,957,854 A	9/1999	Besson et al.	6,122,351 A	9/2000	Schlueter, Jr. et al.
5,957,890 A	9/1999	Mann et al.	6,125,978 A	10/2000	Ando et al.
5,957,958 A	9/1999	Schulman et al.	6,130,623 A	10/2000	MacLellan et al.
5,960,403 A	9/1999	Brown	6,134,461 A	10/2000	Say et al.
5,961,451 A	10/1999	Reber et al.	6,134,504 A	10/2000	Douglas et al.
5,964,993 A	10/1999	Blubaugh, Jr. et al.	6,139,718 A	10/2000	Kurnik et al.
5,965,380 A	10/1999	Heller et al.	6,141,573 A	10/2000	Kurnik et al.
5,968,839 A	10/1999	Blatt et al.	6,142,939 A	11/2000	Eppstein et al.
5,971,922 A	10/1999	Arita et al.	6,143,164 A	11/2000	Heller et al.
5,971,941 A	10/1999	Simons et al.	6,144,837 A	11/2000	Quy
5,974,124 A	10/1999	Schlueter, Jr. et al.	6,144,869 A	11/2000	Berner et al.
5,977,476 A	11/1999	Guha et al.	6,144,922 A	11/2000	Douglas et al.
5,981,294 A	11/1999	Blatt et al.	6,148,094 A	11/2000	Kinsella
5,989,409 A	11/1999	Kurnik et al.	6,150,128 A	11/2000	Uretsky
5,994,476 A	11/1999	Shin et al.	6,151,517 A	11/2000	Honigs et al.
5,995,860 A	11/1999	Sun et al.	6,151,586 A	11/2000	Brown
5,997,476 A	12/1999	Brown	6,153,062 A	11/2000	Saito et al.
5,999,848 A	12/1999	Gord et al.	6,153,069 A	11/2000	Pottgen et al.
5,999,849 A	12/1999	Gord et al.	6,159,147 A	12/2000	Lichter et al.
6,001,067 A	12/1999	Shults et al.	6,161,095 A	12/2000	Brown
6,002,954 A	12/1999	Van Antwerp et al.	6,162,611 A	12/2000	Heller et al.
6,002,961 A	12/1999	Mitragotri et al.	6,162,639 A	12/2000	Douglas
6,004,441 A	12/1999	Fujiwara et al.	6,167,362 A	12/2000	Brown et al.
6,011,984 A	1/2000	Van Antwerp et al.	6,168,563 B1	1/2001	Brown
6,014,577 A	1/2000	Henning et al.	6,170,318 B1	1/2001	Lewis
6,018,678 A	1/2000	Mitragotri et al.	6,175,752 B1	1/2001	Say et al.
6,023,629 A	2/2000	Tamada	6,180,416 B1	1/2001	Kurnik et al.
6,024,699 A	2/2000	Surwit et al.	6,186,145 B1	2/2001	Brown
6,026,320 A	2/2000	Carlson et al.	6,192,891 B1	2/2001	Gravel et al.
6,027,459 A	2/2000	Shain et al.	6,193,873 B1	2/2001	Ohara et al.
6,027,692 A	2/2000	Galen et al.	6,196,970 B1	3/2001	Brown
6,028,413 A	2/2000	Brockmann	6,198,957 B1	3/2001	Green
6,032,059 A	2/2000	Henning et al.	6,201,979 B1	3/2001	Kurnik et al.
6,032,199 A	2/2000	Lim et al.	6,201,980 B1	3/2001	Darrow et al.
6,033,866 A	3/2000	Guo et al.	6,203,495 B1	3/2001	Bardy et al.
6,035,237 A	3/2000	Schulman et al.	6,206,841 B1	3/2001	Cunningham et al.
6,040,194 A	3/2000	Chick et al.	6,206,856 B1	3/2001	Mahurkar
6,041,253 A	3/2000	Kost et al.	6,208,894 B1	3/2001	Schulman et al.
6,043,437 A	3/2000	Schulman et al.	6,210,272 B1	4/2001	Brown
6,049,727 A	4/2000	Crothall	6,210,976 B1	4/2001	Sabbadini
6,052,565 A	4/2000	Ishikura et al.	6,212,416 B1	4/2001	Ward et al.
6,055,316 A	4/2000	Perlman et al.	6,218,809 B1	4/2001	Downs et al.
6,056,718 A	5/2000	Funderburk et al.	6,219,565 B1	4/2001	Cupp et al.
6,063,459 A	5/2000	Velte	6,219,574 B1	4/2001	Cormier et al.
6,066,243 A	5/2000	Anderson et al.	6,224,745 B1	5/2001	Baltruschat
6,067,474 A	5/2000	Schulman et al.	6,232,130 B1	5/2001	Wolf
6,068,615 A	5/2000	Brown et al.	6,232,370 B1	5/2001	Kubota et al.
6,071,249 A	6/2000	Cunningham et al.	6,233,471 B1	5/2001	Berner et al.
6,071,251 A	6/2000	Cunningham et al.	6,233,539 B1	5/2001	Brown
6,071,294 A	6/2000	Simons et al.	6,239,161 B1	5/2001	Tang et al.
6,071,391 A	6/2000	Gotoh et al.	6,239,925 B1	5/2001	Ardrey et al.
6,073,031 A	6/2000	Helstab et al.	6,241,862 B1	6/2001	McAleer et al.
6,081,736 A	6/2000	Colvin et al.	6,246,330 B1	6/2001	Nielsen
6,083,710 A	7/2000	Heller et al.	6,246,992 B1	6/2001	Brown
6,088,608 A	7/2000	Schulman et al.	6,248,065 B1	6/2001	Brown
6,091,975 A	7/2000	Daddona et al.	6,248,067 B1	6/2001	Causey, III et al.
6,091,976 A	7/2000	Pfeiffer et al.	6,248,093 B1	6/2001	Moberg
6,091,987 A	7/2000	Thompson	6,251,260 B1	6/2001	Heller et al.
6,093,156 A	7/2000	Cunningham et al.	6,252,032 B1	6/2001	Van Antwerp et al.
			6,253,804 B1	7/2001	Safabash
			6,254,586 B1	7/2001	Mann et al.
			6,256,643 B1	7/2001	Cork et al.
			6,259,587 B1	7/2001	Sheldon et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,259,937	B1	7/2001	Schulman et al.	6,443,942	B2	9/2002	Van Antwerp et al.
6,260,022	B1	7/2001	Brown	6,449,255	B1	9/2002	Waclawsky et al.
6,266,645	B1	7/2001	Simpson	6,454,710	B1	9/2002	Ballerstadt et al.
6,267,724	B1	7/2001	Taylor	6,462,162	B2	10/2002	Van Antwerp et al.
6,268,161	B1	7/2001	Han et al.	6,464,848	B1	10/2002	Matsumoto
6,270,445	B1	8/2001	Dean, Jr. et al.	6,466,810	B1	10/2002	Ward et al.
6,270,455	B1	8/2001	Brown	6,468,222	B1	10/2002	Mault et al.
6,272,364	B1	8/2001	Kurnik	6,472,122	B1	10/2002	Schulman et al.
6,275,717	B1	8/2001	Gross et al.	6,475,750	B1	11/2002	Han et al.
6,280,416	B1	8/2001	Van Antwerp et al.	6,477,395	B2	11/2002	Schulman et al.
6,280,587	B1	8/2001	Matsumoto	6,478,736	B1	11/2002	Mault
6,281,006	B1	8/2001	Heller et al.	6,480,730	B2	11/2002	Darrow et al.
6,282,179	B1	8/2001	Sherman	6,480,744	B2	11/2002	Ferek-Petric
6,283,943	B1	9/2001	Dy et al.	6,482,156	B2	11/2002	Iliff
6,284,126	B1	9/2001	Kurnik et al.	6,482,158	B2	11/2002	Mault
6,284,478	B1	9/2001	Heller et al.	6,482,604	B2	11/2002	Kwon
6,291,200	B1	9/2001	LeJeune et al.	6,484,045	B1	11/2002	Holker et al.
6,293,925	B1	9/2001	Safabash et al.	6,484,046	B1	11/2002	Say et al.
6,294,281	B1	9/2001	Heller	6,485,138	B1	11/2002	Kubota et al.
6,294,997	B1	9/2001	Paratore et al.	6,493,069	B1	12/2002	Nagashimada et al.
6,295,463	B1	9/2001	Stenzler	6,494,830	B1	12/2002	Wessel
6,295,506	B1	9/2001	Heinonen et al.	6,496,728	B2	12/2002	Li et al.
6,298,254	B2	10/2001	Tamada	6,496,729	B2	12/2002	Thompson
6,299,347	B1	10/2001	Pompei	6,497,655	B1	12/2002	Linberg et al.
6,299,578	B1	10/2001	Kurnik et al.	6,505,059	B1	1/2003	Kollias et al.
6,299,757	B1	10/2001	Feldman et al.	6,505,121	B1	1/2003	Russel
6,301,499	B1	10/2001	Carlson et al.	6,512,939	B1	1/2003	Colvin et al.
6,304,766	B1	10/2001	Colvin, Jr. et al.	6,513,532	B2	2/2003	Mault et al.
6,307,867	B1	10/2001	Roobol et al.	6,514,718	B2	2/2003	Heller et al.
6,309,351	B1	10/2001	Kurnik et al.	6,515,593	B1	2/2003	Stark et al.
6,309,884	B1	10/2001	Cooper et al.	6,520,326	B2	2/2003	McIvor et al.
6,313,749	B1	11/2001	Horne et al.	6,529,755	B2	3/2003	Kurnik et al.
6,314,317	B1	11/2001	Willis	6,529,772	B2	3/2003	Carlson et al.
6,315,721	B2	11/2001	Schulman et al.	6,530,915	B1	3/2003	Eppstein et al.
6,319,540	B1	11/2001	Van Antwerp et al.	6,534,322	B1	3/2003	Sabbadini
6,326,160	B1	12/2001	Dunn et al.	6,534,323	B1	3/2003	Sabbadini
6,329,161	B1	12/2001	Heller et al.	6,535,753	B1	3/2003	Raskas
6,329,929	B1	12/2001	Weijand et al.	6,537,243	B1	3/2003	Henning et al.
6,330,426	B2	12/2001	Brown et al.	6,540,675	B2	4/2003	Aceti et al.
6,330,464	B1	12/2001	Colvin, Jr. et al.	6,541,266	B2	4/2003	Modzelweskei et al.
6,331,518	B2	12/2001	Hemm et al.	6,544,212	B2	4/2003	Galley et al.
6,334,778	B1	1/2002	Brown	6,546,269	B1	4/2003	Kurnik
6,336,900	B1	1/2002	Alleckson et al.	6,549,796	B2	4/2003	Sohrab
6,338,790	B1	1/2002	Feldman et al.	6,551,276	B1	4/2003	Mann et al.
6,340,421	B1	1/2002	Vachon et al.	6,551,494	B1	4/2003	Heller et al.
6,341,232	B1	1/2002	Conn et al.	6,553,244	B2	4/2003	Lesho et al.
6,356,776	B1	3/2002	Berner et al.	6,554,798	B1	4/2003	Mann et al.
6,359,270	B1	3/2002	Bridson	6,558,320	B1	5/2003	Causey, III et al.
6,359,594	B1	3/2002	Junod	6,558,321	B1	5/2003	Burd et al.
6,360,888	B1	3/2002	McIvor et al.	6,558,351	B1	5/2003	Steil et al.
6,366,793	B1	4/2002	Bell et al.	6,560,471	B1	5/2003	Heller et al.
6,366,794	B1	4/2002	Moussy et al.	6,561,975	B1	5/2003	Pool et al.
6,368,141	B1	4/2002	Van Antwerp et al.	6,561,978	B1	5/2003	Conn et al.
6,368,274	B1	4/2002	Van Antwerp et al.	6,562,001	B2	5/2003	Lebel et al.
6,370,410	B2	4/2002	Kurnik et al.	6,564,105	B2	5/2003	Starkweather et al.
6,377,828	B1	4/2002	Chaiken et al.	6,564,807	B1	5/2003	Schulman et al.
6,379,301	B1	4/2002	Worthington et al.	6,565,509	B1	5/2003	Say et al.
6,383,767	B1	5/2002	Polak	6,571,128	B2	5/2003	Lebel et al.
6,385,473	B1	5/2002	Haines et al.	6,571,200	B1	5/2003	Mault
6,387,048	B1	5/2002	Schulman et al.	6,574,510	B2	6/2003	Von Arx et al.
6,391,643	B1	5/2002	Chen et al.	6,576,101	B1	6/2003	Heller et al.
6,393,318	B1	5/2002	Conn et al.	6,576,117	B1	6/2003	Iketaki et al.
6,398,562	B1	6/2002	Butler et al.	6,577,899	B2	6/2003	Lebel et al.
6,400,974	B1	6/2002	Lesho	6,579,231	B1	6/2003	Phipps
6,405,066	B1	6/2002	Essenpreis et al.	6,579,498	B1	6/2003	Eglise
6,413,393	B1	7/2002	Van Antwerp et al.	6,579,690	B1	6/2003	Bonnecaze et al.
6,418,332	B1	7/2002	Mastrototaro et al.	6,580,364	B1	6/2003	Munch et al.
6,424,847	B1	7/2002	Mastrototaro et al.	6,584,335	B1	6/2003	Haar et al.
6,427,088	B1	7/2002	Bowman, IV et al.	6,585,644	B2	7/2003	Lebel et al.
6,434,409	B1	8/2002	Pfeiffer et al.	6,587,705	B1	7/2003	Kim et al.
6,438,414	B1	8/2002	Conn et al.	6,591,125	B1	7/2003	Buse et al.
6,440,068	B1	8/2002	Brown et al.	6,591,126	B2	7/2003	Roeper et al.
6,441,747	B1	8/2002	Khair et al.	6,594,514	B2	7/2003	Berner et al.
6,442,637	B1	8/2002	Hawkins et al.	6,595,919	B2	7/2003	Berner et al.
6,442,672	B1	8/2002	Ganapathy	6,595,929	B2	7/2003	Stivoric et al.
				6,599,243	B2	7/2003	Woltermann et al.
				6,602,469	B1	8/2003	Maus et al.
				6,602,678	B2	8/2003	Kwon et al.
				6,602,909	B1	8/2003	Jarowski

(56)

References Cited

U.S. PATENT DOCUMENTS

6,605,200 B1	8/2003	Mao et al.	6,780,156 B2	8/2004	Haueter et al.
6,605,201 B1	8/2003	Mao et al.	6,780,297 B2	8/2004	Matsumoto et al.
6,607,509 B2	8/2003	Bobroff et al.	6,780,871 B2	8/2004	Glick et al.
6,608,562 B1	8/2003	Kimura et al.	6,784,274 B2	8/2004	Van Antwerp et al.
6,610,012 B2	8/2003	Mault	6,790,178 B1	9/2004	Mault et al.
6,611,206 B2	8/2003	Eshelman et al.	6,794,195 B2	9/2004	Colvin, Jr.
6,612,306 B1	9/2003	Mault	6,800,451 B2	10/2004	Daniloff et al.
6,615,078 B1	9/2003	Burson et al.	6,804,544 B2	10/2004	Van Antwerp et al.
6,616,613 B1	9/2003	Goodman	6,804,558 B2	10/2004	Haller et al.
6,618,603 B2	9/2003	Varalli et al.	6,809,507 B2	10/2004	Morgan et al.
6,620,106 B2	9/2003	Mault	6,809,653 B1	10/2004	Mann et al.
6,627,058 B1	9/2003	Chan	6,810,290 B2	10/2004	Lebel et al.
6,627,154 B1	9/2003	Goodman et al.	6,810,309 B2	10/2004	Sadler et al.
6,629,934 B2	10/2003	Mault et al.	6,811,533 B2	11/2004	Lebel et al.
6,633,772 B2	10/2003	Ford et al.	6,811,534 B2	11/2004	Bowman, IV et al.
6,635,014 B2	10/2003	Starkweather et al.	6,811,659 B2	11/2004	Vachon
6,641,533 B2	11/2003	Causey, III et al.	6,812,031 B1	11/2004	Carlsson
6,642,015 B2	11/2003	Vachon et al.	6,813,519 B2	11/2004	Lebel et al.
6,645,142 B2	11/2003	Braig et al.	6,816,742 B2	11/2004	Kim et al.
6,645,368 B1	11/2003	Beaty et al.	6,835,553 B2	12/2004	Han et al.
6,648,821 B2	11/2003	Lebel et al.	RE38,681 E	1/2005	Kurnik et al.
6,653,091 B1	11/2003	Dunn et al.	6,840,912 B2	1/2005	Kloepfer et al.
6,654,625 B1	11/2003	Say et al.	6,844,023 B2	1/2005	Schulman et al.
6,656,114 B1	12/2003	Poulson et al.	6,849,237 B2	2/2005	Housefield et al.
6,658,396 B1	12/2003	Tang et al.	6,850,790 B2	2/2005	Berner et al.
6,659,948 B2	12/2003	Lebel et al.	6,852,104 B2	2/2005	Blomquist
6,668,196 B1	12/2003	Villegas et al.	6,852,500 B1	2/2005	Hoss et al.
6,671,554 B2	12/2003	Gibson et al.	6,852,694 B2	2/2005	Van Antwerp et al.
6,673,625 B2	1/2004	Satcher, Jr. et al.	6,853,854 B1	2/2005	Proniewicz et al.
6,682,938 B1	1/2004	Satcher, Jr. et al.	6,856,928 B2	2/2005	Harmon
6,683,040 B2	1/2004	Bragulla et al.	6,858,403 B2	2/2005	Han et al.
6,687,522 B2	2/2004	Tamada	6,862,465 B2	3/2005	Shults et al.
6,687,546 B2	2/2004	Lebel et al.	6,862,466 B2	3/2005	Ackerman
6,689,056 B1	2/2004	Kilcoyne et al.	6,872,200 B2	3/2005	Mann et al.
6,690,276 B1	2/2004	Marino	6,873,268 B2	3/2005	Lebel et al.
6,692,446 B2	2/2004	Hoek	6,878,112 B2	4/2005	Linberg et al.
6,693,069 B2	2/2004	Korber et al.	6,881,551 B2	4/2005	Heller et al.
6,694,158 B2	2/2004	Polak	6,882,940 B2	4/2005	Potts et al.
6,694,191 B2	2/2004	Starkweather et al.	6,885,883 B2	4/2005	Parris et al.
6,695,860 B1	2/2004	Ward et al.	6,889,331 B2	5/2005	Soerensen et al.
6,698,269 B2	3/2004	Baber et al.	6,892,085 B2	5/2005	McIvor et al.
6,701,270 B1	3/2004	Miller et al.	6,893,396 B2	5/2005	Schulze et al.
6,702,857 B2	3/2004	Brauker et al.	6,895,263 B2	5/2005	Shin et al.
6,704,587 B1	3/2004	Kumar et al.	6,895,265 B2	5/2005	Silver
6,708,057 B2	3/2004	Marganroth	6,899,683 B2	5/2005	Mault et al.
6,711,423 B2	3/2004	Colvin, Jr.	6,899,684 B2	5/2005	Mault et al.
6,723,046 B2	4/2004	Lichtenstein et al.	6,902,207 B2	6/2005	Lickliter
6,728,560 B2	4/2004	Kollias et al.	6,902,905 B2	6/2005	Burson et al.
6,730,025 B1	5/2004	Platt	6,904,301 B2	6/2005	Raskas
6,731,976 B2	5/2004	Penn et al.	6,907,127 B1	6/2005	Kravitz et al.
6,733,446 B2	5/2004	Lebel et al.	6,915,147 B2	7/2005	Lebel et al.
6,734,162 B2	5/2004	Van Antwerp et al.	6,918,874 B1 *	7/2005	Hatch A61B 5/00 600/309
6,735,183 B2	5/2004	O'Toole et al.	6,922,578 B2	7/2005	Eppstein et al.
6,735,479 B2	5/2004	Fabian et al.	RE38,775 E	8/2005	Kurnik et al.
6,736,777 B2	5/2004	Kim et al.	6,923,764 B2	8/2005	Aceti et al.
6,736,797 B1	5/2004	Larsen et al.	6,923,936 B2	8/2005	Swanson et al.
6,737,401 B2	5/2004	Kim et al.	6,926,670 B2 *	8/2005	Rich A61B 5/0031 600/459
6,738,654 B2	5/2004	Sohrab	6,927,246 B2	8/2005	Noronha et al.
6,740,075 B2	5/2004	Lebel et al.	6,931,327 B2	8/2005	Goode, Jr. et al.
6,741,163 B1	5/2004	Roberts	6,936,006 B2	8/2005	Sabra
6,741,876 B1	5/2004	Scecina et al.	6,936,029 B2	8/2005	Mann et al.
6,741,877 B1	5/2004	Shults et al.	6,937,222 B2	8/2005	Numao
6,743,635 B2	6/2004	Neel et al.	6,940,403 B2	9/2005	Kail, IV
6,746,582 B2	6/2004	Heller et al.	6,940,590 B2	9/2005	Colvin, Jr. et al.
6,748,445 B1	6/2004	Darcey et al.	6,941,163 B2	9/2005	Ford et al.
6,749,587 B2	6/2004	Flaherty	6,950,708 B2	9/2005	Bowman, IV et al.
6,750,311 B1	6/2004	Van Antwerp et al.	6,952,603 B2	10/2005	Gerber et al.
6,758,810 B2	7/2004	Lebel et al.	6,954,673 B2	10/2005	Von Arx et al.
6,766,183 B2	7/2004	Walsh et al.	6,955,650 B2	10/2005	Mault et al.
6,766,201 B2	7/2004	Von Arx et al.	6,957,102 B2	10/2005	Silver et al.
6,768,425 B2	7/2004	Flaherty et al.	6,957,107 B2	10/2005	Rogers et al.
6,770,030 B1	8/2004	Schaupp et al.	6,958,705 B2	10/2005	Lebel et al.
6,770,729 B2	8/2004	Van Antwerp et al.	6,968,294 B2	11/2005	Gutta et al.
6,771,995 B2	8/2004	Kurnik et al.	6,968,375 B1	11/2005	Brown
6,773,563 B2	8/2004	Matsumoto	6,971,274 B2	12/2005	Olin
			6,974,437 B2	12/2005	Lebel et al.
			6,978,182 B2	12/2005	Mazar et al.

(56)	References Cited		7,222,054 B2 *	5/2007	Geva	A61B 5/1112 340/539.12
	U.S. PATENT DOCUMENTS		7,226,442 B2	6/2007	Sheppard et al.	
			7,226,978 B2	6/2007	Tapsak et al.	
6,979,326 B2	12/2005	Mann et al.	7,228,162 B2	6/2007	Ward et al.	
6,983,176 B2	1/2006	Gardner et al.	7,228,163 B2	6/2007	Ackerman	
6,985,870 B2	1/2006	Martucci et al.	7,228,182 B2	6/2007	Healy et al.	
6,987,474 B2	1/2006	Freeman et al.	7,233,817 B2	6/2007	Yen	
6,990,317 B2 *	1/2006	Arnold	7,237,712 B2	7/2007	DeRocco et al.	
		G08C 17/02 370/345	7,241,266 B2	7/2007	Zhou et al.	
6,990,366 B2	1/2006	Say et al.	7,258,665 B2 *	8/2007	Kohls	A61B 5/0002 128/920
6,991,096 B2	1/2006	Gottlieb et al.				
6,997,907 B2	2/2006	Safabash et al.	7,261,691 B1	8/2007	Asomani	
6,997,920 B2	2/2006	Mann et al.	7,267,665 B2	9/2007	Steil et al.	
6,998,247 B2	2/2006	Monfre et al.	7,276,029 B2	10/2007	Goode, Jr. et al.	
6,999,810 B2	2/2006	Berner et al.	7,286,894 B1	10/2007	Grant et al.	
7,003,336 B2	2/2006	Holker et al.	7,291,107 B2	11/2007	Hellwig et al.	
7,003,340 B2	2/2006	Say et al.	7,295,867 B2	11/2007	Berner et al.	
7,003,341 B2	2/2006	Say et al.	7,297,112 B2	11/2007	Zhou et al.	
7,004,901 B2	2/2006	Fish	7,310,544 B2	12/2007	Brister et al.	
7,005,857 B2	2/2006	Stiene et al.	7,318,816 B2	1/2008	Bobroff et al.	
7,009,511 B2	3/2006	Mazar et al.	7,324,850 B2	1/2008	Persen et al.	
7,011,630 B2	3/2006	Desai et al.	7,335,294 B2	2/2008	Heller et al.	
7,018,366 B2	3/2006	Easter	7,347,819 B2	3/2008	Lebel et al.	
7,018,568 B2	3/2006	Tierney	7,354,420 B2	4/2008	Steil et al.	
7,020,508 B2	3/2006	Stivoric et al.	7,364,592 B2	4/2008	Carr-Brendel et al.	
7,022,072 B2	4/2006	Fox et al.	7,366,556 B2	4/2008	Brister et al.	
7,024,236 B2	4/2006	Ford et al.	7,379,765 B2	5/2008	Petisce et al.	
7,024,245 B2	4/2006	Lebel et al.	7,384,397 B2	6/2008	Zhang et al.	
7,025,743 B2	4/2006	Mann et al.	7,387,010 B2	6/2008	Sunshine et al.	
7,027,621 B1	4/2006	Prokoski	7,398,183 B2	7/2008	Holland et al.	
7,027,931 B1	4/2006	Jones et al.	7,402,153 B2	7/2008	Steil et al.	
7,029,444 B2	4/2006	Shin et al.	7,404,796 B2	7/2008	Ginsberg	
7,039,810 B1	5/2006	Nichols	7,408,132 B2	8/2008	Wambsganss et al.	
7,041,068 B2	5/2006	Freeman et al.	7,418,285 B2	8/2008	Ghesquiere et al.	
7,041,468 B2	5/2006	Drucker et al.	7,419,573 B2	9/2008	Gundel	
7,043,305 B2	5/2006	KenKnight et al.	7,424,318 B2	9/2008	Brister et al.	
7,049,277 B2	5/2006	Bagulla et al.	7,460,898 B2	12/2008	Brister et al.	
7,052,251 B2	5/2006	Nason et al.	7,467,003 B2	12/2008	Brister et al.	
7,052,472 B1	5/2006	Miller et al.	7,471,972 B2	12/2008	Rhodes et al.	
7,052,483 B2	5/2006	Wojcik	7,492,254 B2	2/2009	Bandy et al.	
7,056,302 B2	6/2006	Douglas	7,494,465 B2	2/2009	Brister et al.	
7,058,453 B2	6/2006	Nelson et al.	7,497,827 B2	3/2009	Brister et al.	
7,060,030 B2	6/2006	Von Arx et al.	7,506,046 B2	3/2009	Rhodes	
7,060,031 B2	6/2006	Webb et al.	7,519,408 B2	4/2009	Rasdal et al.	
7,068,227 B2	6/2006	Ying	7,547,281 B2	6/2009	Hayes et al.	
7,074,307 B2	7/2006	Simpson et al.	7,565,197 B2	7/2009	Haubrich et al.	
7,081,195 B2	7/2006	Simpson et al.	7,569,030 B2	8/2009	Lebel et al.	
7,089,780 B2	8/2006	Sunshine et al.	7,574,266 B2	8/2009	Dudding et al.	
7,098,803 B2	8/2006	Mann et al.	7,583,990 B2	9/2009	Goode, Jr. et al.	
7,108,778 B2	9/2006	Simpson et al.	7,591,801 B2	9/2009	Brauker et al.	
7,109,878 B2	9/2006	Mann et al.	7,599,726 B2	10/2009	Goode, Jr. et al.	
7,110,803 B2	9/2006	Shults et al.	7,602,310 B2	10/2009	Mann et al.	
7,113,821 B1	9/2006	Sun et al.	7,604,178 B2	10/2009	Stewart	
7,114,502 B2	10/2006	Schulman et al.	7,613,491 B2	11/2009	Boock et al.	
7,124,027 B1	10/2006	Ernst et al.	7,615,007 B2	11/2009	Shults et al.	
7,125,382 B2	10/2006	Zhou et al.	7,618,369 B2	11/2009	Hayter et al.	
7,133,710 B2	11/2006	Acosta et al.	7,632,228 B2	12/2009	Brauker et al.	
7,134,999 B2	11/2006	Brauker et al.	7,637,868 B2	12/2009	Saint et al.	
7,136,689 B2	11/2006	Shults et al.	7,640,048 B2	12/2009	Dobbles et al.	
7,137,964 B2	11/2006	Flaherty	7,651,596 B2	1/2010	Petisce et al.	
7,150,975 B2	12/2006	Tamada et al.	7,653,425 B2	1/2010	Hayter et al.	
7,154,398 B2	12/2006	Chen et al.	7,654,956 B2	2/2010	Brister et al.	
7,155,112 B2	12/2006	Uno et al.	7,657,297 B2	2/2010	Simpson et al.	
7,155,290 B2	12/2006	Von Arx et al.	7,659,823 B1	2/2010	Killian et al.	
7,163,511 B2	1/2007	Conn et al.	7,668,596 B2	2/2010	Von Arx et al.	
7,167,818 B2	1/2007	Brown	7,699,775 B2	4/2010	Desai et al.	
7,171,274 B2	1/2007	Starkweather et al.	7,701,052 B2	4/2010	Borland et al.	
7,174,199 B2	2/2007	Berner et al.	7,711,402 B2	5/2010	Shults et al.	
7,181,505 B2	2/2007	Haller et al.	7,713,574 B2	5/2010	Brister et al.	
7,183,068 B2	2/2007	Burson et al.	7,715,893 B2	5/2010	Kamath et al.	
7,183,102 B2	2/2007	Monfre et al.	7,741,734 B2	6/2010	Joannopoulos et al.	
7,187,528 B2	3/2007	Talbot et al.	7,766,829 B2	8/2010	Sloan et al.	
7,189,341 B2	3/2007	Li et al.	7,767,149 B2	8/2010	Maus et al.	
7,190,988 B2	3/2007	Say et al.	7,768,387 B2	8/2010	Fennell et al.	
7,192,450 B2	3/2007	Brauker et al.	7,775,444 B2	8/2010	DeRocco et al.	
7,198,606 B2	4/2007	Boecker et al.	7,779,332 B2	8/2010	Karr et al.	
7,218,890 B1	5/2007	Iseli et al.	7,782,192 B2	8/2010	Jeckelmann et al.	
7,221,977 B1	5/2007	Weaver et al.	7,791,467 B2	9/2010	Mazar et al.	

(56)	References Cited		8,622,903 B2 *	1/2014	Jin	A61B 5/0002 600/301
	U.S. PATENT DOCUMENTS		8,638,411 B2	1/2014	Park et al.	
			8,849,459 B2	9/2014	Ramey et al.	
7,804,197 B2	9/2010	Iisaka et al.	8,914,090 B2	12/2014	Jain et al.	
7,811,231 B2	10/2010	Jin et al.	9,402,584 B2	8/2016	Fennell	
7,813,809 B2	10/2010	Strother et al.	2001/0011224 A1	8/2001	Brown	
7,826,382 B2	11/2010	Sicurello et al.	2001/0011795 A1	8/2001	Ohtsuka et al.	
7,831,310 B2	11/2010	Lebel et al.	2001/0016310 A1	8/2001	Brown et al.	
7,833,151 B2	11/2010	Khait et al.	2001/0016682 A1	8/2001	Berner et al.	
7,860,574 B2	12/2010	Von Arx et al.	2001/0016683 A1	8/2001	Darrow et al.	
7,882,611 B2	2/2011	Shah et al.	2001/0020124 A1	9/2001	Tamada	
7,889,069 B2	2/2011	Fifolt et al.	2001/0029340 A1	10/2001	Mault et al.	
7,899,545 B2	3/2011	John	2001/0032278 A1	10/2001	Brown et al.	
7,905,833 B2	3/2011	Brister et al.	2001/0037060 A1	11/2001	Thompson et al.	
7,912,674 B2	3/2011	Killoren Clark et al.	2001/0037069 A1	11/2001	Carlson et al.	
7,914,460 B2	3/2011	Melker et al.	2001/0037366 A1	11/2001	Webb et al.	
7,916,013 B2	3/2011	Stevenson	2001/0039504 A1	11/2001	Linberg et al.	
7,920,906 B2	4/2011	Goode et al.	2001/0041830 A1	11/2001	Varalli et al.	
7,948,369 B2	5/2011	Fennell et al.	2001/0041831 A1	11/2001	Starkweather et al.	
7,955,258 B2	6/2011	Goscha et al.	2001/0044581 A1	11/2001	Mault	
7,970,448 B2	6/2011	Shults et al.	2001/0044588 A1	11/2001	Mault	
7,974,672 B2	7/2011	Shults et al.	2001/0047125 A1	11/2001	Quy	
7,978,063 B2	7/2011	Baldus et al.	2001/0047127 A1	11/2001	New et al.	
7,999,674 B2	8/2011	Kamen	2001/0049096 A1	12/2001	Brown	
8,000,918 B2	8/2011	Fjield et al.	2001/0049470 A1	12/2001	Mault et al.	
8,010,256 B2	8/2011	Oowada	2001/0051768 A1	12/2001	Schulman et al.	
8,029,735 B2	10/2011	Schell	2002/0002326 A1	1/2002	Causey, III et al.	
8,072,310 B1	12/2011	Everhart	2002/0002328 A1	1/2002	Tamada	
8,090,445 B2	1/2012	Ginggen	2002/0004640 A1	1/2002	Conn et al.	
8,093,991 B2	1/2012	Stevenson et al.	2002/0010414 A1	1/2002	Coston et al.	
8,094,009 B2	1/2012	Allen et al.	2002/0013522 A1	1/2002	Lav et al.	
8,098,159 B2	1/2012	Batra et al.	2002/0013538 A1	1/2002	Teller	
8,098,160 B2	1/2012	Howarth et al.	2002/0016530 A1	2/2002	Brown	
8,098,161 B2	1/2012	Lavedas	2002/0016719 A1	2/2002	Nemeth et al.	
8,098,201 B2	1/2012	Choi et al.	2002/0018013 A1	2/2002	Nakao et al.	
8,098,208 B2	1/2012	Ficker et al.	2002/0019022 A1	2/2002	Dunn et al.	
8,102,021 B2	1/2012	Degani	2002/0019584 A1	2/2002	Schulze et al.	
8,102,154 B2	1/2012	Bishop et al.	2002/0019586 A1	2/2002	Teller et al.	
8,102,263 B2	1/2012	Yeo et al.	2002/0019748 A1	2/2002	Brown	
8,102,789 B2	1/2012	Rosar et al.	2002/0026111 A1	2/2002	Ackerman	
8,103,241 B2	1/2012	Young et al.	2002/0026937 A1	3/2002	Mault	
8,103,325 B2	1/2012	Swedlow et al.	2002/0027164 A1	3/2002	Mault et al.	
8,106,780 B2	1/2012	Goodnow et al.	2002/0028995 A1	3/2002	Mault	
8,111,042 B2	2/2012	Bennett	2002/0040208 A1	4/2002	Flaherty et al.	
8,115,488 B2	2/2012	McDowell	2002/0042090 A1	4/2002	Heller et al.	
8,116,681 B2	2/2012	Baarman	2002/0042561 A1	4/2002	Schulman et al.	
8,116,683 B2	2/2012	Baarman	2002/0046300 A1	4/2002	Hanko et al.	
8,117,481 B2	2/2012	Anselmi et al.	2002/0047867 A1	4/2002	Mault et al.	
8,120,493 B2	2/2012	Burr	2002/0049482 A1	4/2002	Fabian et al.	
8,123,686 B2	2/2012	Fennell et al.	2002/0053637 A1	5/2002	Conn et al.	
8,124,452 B2	2/2012	Sheats	2002/0062069 A1	5/2002	Mault	
8,130,093 B2	3/2012	Mazar et al.	2002/0063060 A1	5/2002	Gascoyne et al.	
8,131,351 B2	3/2012	Kalgren et al.	2002/0065454 A1	5/2002	Lebel et al.	
8,131,365 B2	3/2012	Zhang et al.	2002/0068858 A1	6/2002	Braig et al.	
8,131,565 B2	3/2012	Dicks et al.	2002/0072784 A1	6/2002	Sheppard et al.	
8,132,037 B2	3/2012	Fehr et al.	2002/0072858 A1	6/2002	Cheng	
8,135,352 B2	3/2012	Langsweirdt et al.	2002/0074162 A1	6/2002	Su et al.	
8,136,735 B2	3/2012	Arai et al.	2002/0077765 A1	6/2002	Mault	
8,138,925 B2	3/2012	Downie et al.	2002/0077766 A1	6/2002	Mault	
8,140,160 B2	3/2012	Pless et al.	2002/0081559 A1	6/2002	Brown et al.	
8,140,168 B2	3/2012	Olson et al.	2002/0083461 A1	6/2002	Hutcheson et al.	
8,140,294 B2	3/2012	Ramey et al.	2002/0085719 A1	7/2002	Crosbie	
8,140,299 B2	3/2012	Siess	2002/0087056 A1	7/2002	Aceti et al.	
8,150,321 B2	4/2012	Winter et al.	2002/0091312 A1	7/2002	Berner et al.	
8,150,516 B2	4/2012	Vine et al.	2002/0091796 A1	7/2002	Higginson et al.	
8,160,669 B2	4/2012	Brauker et al.	2002/0093969 A1	7/2002	Lin et al.	
8,179,266 B2	5/2012	Hermle	2002/0099854 A1 *	7/2002	Jorgensen	H04L 1/20 709/249
8,192,394 B2	6/2012	Estes et al.	2002/0103425 A1	8/2002	Mault	
8,233,456 B1	7/2012	Kopikare et al.	2002/0103499 A1	8/2002	Perez et al.	
8,260,393 B2	9/2012	Kamath et al.	2002/0106709 A1	8/2002	Potts et al.	
8,282,549 B2	10/2012	Brauker et al.	2002/0107433 A1	8/2002	Mault	
8,346,337 B2	1/2013	Heller et al.	2002/0107476 A1	8/2002	Mann et al.	
8,417,312 B2	4/2013	Kamath et al.	2002/0109600 A1	8/2002	Mault et al.	
8,427,298 B2	4/2013	Fennell et al.	2002/0109621 A1	8/2002	Khair et al.	
8,461,985 B2	6/2013	Fennell et al.	2002/0117639 A1	8/2002	Paolini et al.	
8,478,389 B1	7/2013	Brockway et al.	2002/0118528 A1	8/2002	Su et al.	
8,560,037 B2	10/2013	Goode, Jr. et al.	2002/0119711 A1	8/2002	Van Antwerp et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

2002/0124017	A1	9/2002	Mault		2003/0195403	A1	10/2003	Berner et al.
2002/0126036	A1	9/2002	Flaherty et al.		2003/0195462	A1	10/2003	Mann et al.
2002/0128594	A1	9/2002	Das et al.		2003/0199790	A1	10/2003	Boecker et al.
2002/0130042	A1	9/2002	Moerman et al.		2003/0199791	A1	10/2003	Boecker et al.
2002/0133378	A1	9/2002	Mault et al.		2003/0199903	A1	10/2003	Boecker et al.
2002/0147135	A1	10/2002	Schnell		2003/0203498	A1	10/2003	Neel et al.
2002/0161286	A1	10/2002	Gerber et al.		2003/0204290	A1	10/2003	Sadler et al.
2002/0161288	A1	10/2002	Shin et al.		2003/0208110	A1	11/2003	Mault et al.
2002/0169394	A1	11/2002	Eppstein et al.		2003/0208113	A1	11/2003	Mault et al.
2002/0169635	A1	11/2002	Shillingburg		2003/0208114	A1	11/2003	Ackerman
2002/0173830	A1 *	11/2002	Starkweather	A61N 1/37211 607/60	2003/0208133	A1	11/2003	Mault
					2003/0208409	A1	11/2003	Mault
					2003/0212346	A1	11/2003	Yuzhakov et al.
					2003/0212379	A1	11/2003	Bylund et al.
					2003/0212579	A1	11/2003	Brown et al.
					2003/0216630	A1	11/2003	Jersey-Willuhn et al.
					2003/0217966	A1	11/2003	Tapsak et al.
2002/0177764	A1	11/2002	Sohrab		2003/0224729	A1	12/2003	Arnold
2002/0185130	A1	12/2002	Wright et al.		2003/0226695	A1	12/2003	Mault
2002/0193679	A1	12/2002	Malave et al.		2003/0229514	A2	12/2003	Brown
2002/0198513	A1	12/2002	Lebel et al.		2003/0232370	A1	12/2003	Trifiro
2003/0004403	A1	1/2003	Drinan et al.		2003/0235817	A1	12/2003	Bartkowiak et al.
2003/0009203	A1	1/2003	Lebel et al.		2004/0010207	A1	1/2004	Flaherty et al.
2003/0023182	A1	1/2003	Mault et al.		2004/0011671	A1	1/2004	Shults et al.
2003/0023317	A1	1/2003	Brauker et al.		2004/0017300	A1	1/2004	Kotzin et al.
2003/0028089	A1	2/2003	Galley et al.		2004/0018486	A1	1/2004	Dunn et al.
2003/0028120	A1	2/2003	Mault et al.		2004/0030226	A1	2/2004	Quy
2003/0032077	A1	2/2003	Itoh et al.		2004/0030531	A1	2/2004	Miller et al.
2003/0032867	A1	2/2003	Crothall et al.		2004/0030581	A1	2/2004	Levin et al.
2003/0032868	A1	2/2003	Graskov et al.		2004/0034289	A1	2/2004	Teller et al.
2003/0032874	A1	2/2003	Rhodes et al.		2004/0039255	A1	2/2004	Simonsen et al.
2003/0035371	A1 *	2/2003	Reed	H04L 47/12 370/230	2004/0039256	A1	2/2004	Kawatahara et al.
					2004/0040840	A1	3/2004	Mao et al.
2003/0040683	A1	2/2003	Rule et al.		2004/0045879	A1	3/2004	Shults et al.
2003/0042137	A1	3/2003	Mao et al.		2004/0054263	A1	3/2004	Moerman et al.
2003/0050537	A1	3/2003	Wessel		2004/0059201	A1	3/2004	Ginsberg
2003/0050546	A1	3/2003	Desai et al.		2004/0063435	A1	4/2004	Sakamoto et al.
2003/0060689	A1 *	3/2003	Kohls	A61B 5/0002 600/300	2004/0064068	A1	4/2004	DeNuzzio et al.
					2004/0069164	A1	4/2004	Nakamura et al.
2003/0060692	A1	3/2003	Ruchti et al.		2004/0072357	A1	4/2004	Stiene et al.
2003/0060753	A1	3/2003	Starkweather et al.		2004/0073095	A1	4/2004	Causey, III et al.
2003/0065257	A1	4/2003	Mault et al.		2004/0096959	A1	5/2004	Stiene et al.
2003/0065273	A1	4/2003	Mault et al.		2004/0100376	A1	5/2004	Lye et al.
2003/0065274	A1	4/2003	Mault et al.		2004/0105411	A1	6/2004	Boatwright et al.
2003/0065275	A1	4/2003	Mault et al.		2004/0106858	A1	6/2004	Say et al.
2003/0065308	A1	4/2003	Lebel et al.		2004/0106859	A1	6/2004	Say et al.
2003/0076792	A1	4/2003	Theimer		2004/0108226	A1	6/2004	Polychronakos et al.
2003/0081370	A1	5/2003	Haskell et al.		2004/0116786	A1	6/2004	Iijima et al.
2003/0100040	A1	5/2003	Bonnecaze et al.		2004/0122353	A1	6/2004	Shahmirian et al.
2003/0100821	A1	5/2003	Heller et al.		2004/0122489	A1	6/2004	Mazar et al.
2003/0105407	A1	6/2003	Pearce et al.		2004/0122530	A1	6/2004	Hansen et al.
2003/0108976	A1	6/2003	Braig et al.		2004/0128161	A1	7/2004	Mazar et al.
2003/0114897	A1	6/2003	Von Arx et al.		2004/0133164	A1	7/2004	Funderburk et al.
2003/0119457	A1	6/2003	Standke		2004/0133390	A1	7/2004	Osorio et al.
2003/0122021	A1	7/2003	McConnell et al.		2004/0136361	A1	7/2004	Holloway et al.
2003/0122660	A1 *	7/2003	Kachouh	B60C 23/0408 340/442	2004/0136377	A1	7/2004	Miyazaki et al.
					2004/0138588	A1	7/2004	Saikley et al.
2003/0130616	A1	7/2003	Steil et al.		2004/0146909	A1	7/2004	Duong et al.
2003/0134347	A1	7/2003	Heller et al.		2004/0147872	A1	7/2004	Thompson
2003/0135100	A1	7/2003	Kim et al.		2004/0152961	A1	8/2004	Carlson et al.
2003/0135333	A1	7/2003	Aceti et al.		2004/0153585	A1	8/2004	Kawatahara et al.
2003/0144579	A1	7/2003	Buss		2004/0162473	A1	8/2004	Sohrab
2003/0144581	A1	7/2003	Conn et al.		2004/0164961	A1	8/2004	Bal et al.
2003/0146841	A1	8/2003	Koenig		2004/0167383	A1	8/2004	Kim et al.
2003/0153820	A1	8/2003	Berner et al.		2004/0167464	A1	8/2004	Ireland et al.
2003/0153821	A1	8/2003	Berner et al.		2004/0167801	A1	8/2004	Say et al.
2003/0158472	A1	8/2003	Sohrab		2004/0171921	A1	9/2004	Say et al.
2003/0158707	A1	8/2003	Doi		2004/0172284	A1	9/2004	Sullivan et al.
2003/0168338	A1	9/2003	Gao et al.		2004/0176672	A1	9/2004	Silver et al.
2003/0175806	A1	9/2003	Rule et al.		2004/0176913	A1	9/2004	Kawatahara et al.
2003/0175992	A1	9/2003	Toranto et al.		2004/0186362	A1	9/2004	Brauker et al.
2003/0176183	A1	9/2003	Drucker et al.		2004/0186365	A1	9/2004	Jin et al.
2003/0176933	A1	9/2003	Lebel et al.		2004/0193020	A1	9/2004	Chiba et al.
2003/0179705	A1	9/2003	Kojima		2004/0193025	A1	9/2004	Steil et al.
2003/0181851	A1	9/2003	Mann et al.		2004/0193090	A1	9/2004	Lebel et al.
2003/0181852	A1	9/2003	Mann et al.		2004/0197846	A1	10/2004	Hockersmith et al.
2003/0187338	A1	10/2003	Say et al.		2004/0199056	A1	10/2004	Husemann et al.
2003/0187525	A1	10/2003	Mann et al.		2004/0199059	A1	10/2004	Brauker et al.
2003/0191376	A1	10/2003	Samuels et al.		2004/0202576	A1	10/2004	Aceti et al.
2003/0191431	A1	10/2003	Mann et al.					

(56)

References Cited

U.S. PATENT DOCUMENTS

2004/0204055	A1	10/2004	Nousiainen	2005/0171513	A1	8/2005	Mann et al.
2004/0204868	A1	10/2004	Maynard et al.	2005/0173245	A1	8/2005	Feldman et al.
2004/0206916	A1	10/2004	Colvin, Jr. et al.	2005/0176136	A1	8/2005	Burd et al.
2004/0208780	A1	10/2004	Faries, Jr. et al.	2005/0177036	A1	8/2005	Shults et al.
2004/0212536	A1	10/2004	Mori et al.	2005/0177398	A1	8/2005	Watanabe et al.
2004/0219664	A1	11/2004	Heller et al.	2005/0181012	A1	8/2005	Saint et al.
2004/0221057	A1	11/2004	Darcey et al.	2005/0182306	A1	8/2005	Sloan et al.
2004/0225199	A1	11/2004	Evanyk et al.	2005/0182358	A1	8/2005	Veit et al.
2004/0225338	A1	11/2004	Lebel et al.	2005/0182451	A1	8/2005	Griffin et al.
2004/0235446	A1	11/2004	Flaherty et al.	2005/0187720	A1	8/2005	Goode, Jr. et al.
2004/0236200	A1	11/2004	Say et al.	2005/0192494	A1	9/2005	Ginsberg
2004/0248204	A1	12/2004	Moerman	2005/0192557	A1	9/2005	Brauker et al.
2004/0249250	A1	12/2004	McGee et al.	2005/0195930	A1	9/2005	Spital et al.
2004/0249253	A1	12/2004	Racchini et al.	2005/0199494	A1	9/2005	Say et al.
2004/0249254	A1	12/2004	Racchini et al.	2005/0203360	A1	9/2005	Brauker et al.
2004/0249999	A1	12/2004	Connolly et al.	2005/0203707	A1	9/2005	Tsutsui et al.
2004/0253736	A1	12/2004	Stout et al.	2005/0204134	A1	9/2005	Von Arx et al.
2004/0254429	A1	12/2004	Yang	2005/0214892	A1	9/2005	Kovatchev et al.
2004/0254433	A1	12/2004	Bandis et al.	2005/0215871	A1	9/2005	Feldman et al.
2004/0254434	A1	12/2004	Goodnow et al.	2005/0215872	A1	9/2005	Berner et al.
2004/0260363	A1	12/2004	Von Arx et al.	2005/0221504	A1	10/2005	Petrino et al.
2004/0260478	A1	12/2004	Schwamm	2005/0236361	A1	10/2005	Ufer et al.
2004/0263354	A1	12/2004	Mann et al.	2005/0239154	A1	10/2005	Feldman et al.
2004/0267300	A1	12/2004	Mace	2005/0239156	A1	10/2005	Drucker et al.
2005/0001024	A1	1/2005	Kusaka et al.	2005/0241957	A1	11/2005	Mao et al.
2005/0003470	A1	1/2005	Nelson et al.	2005/0245795	A1	11/2005	Goode, Jr. et al.
2005/0004494	A1	1/2005	Perez et al.	2005/0245799	A1	11/2005	Brauker et al.
2005/0010087	A1	1/2005	Banet et al.	2005/0245839	A1	11/2005	Stivoric et al.
2005/0010269	A1	1/2005	Lebel et al.	2005/0245904	A1	11/2005	Estes et al.
2005/0016276	A1	1/2005	Guan et al.	2005/0251033	A1	11/2005	Scarantino et al.
2005/0017864	A1	1/2005	Tsoukalis	2005/0251083	A1	11/2005	Carr-Brendel et al.
2005/0027177	A1	2/2005	Shin et al.	2005/0259514	A1	11/2005	Iseli et al.
2005/0027179	A1	2/2005	Berner et al.	2005/0261660	A1	11/2005	Choi
2005/0027180	A1	2/2005	Goode, Jr. et al.	2005/0267780	A1	12/2005	Ray et al.
2005/0027181	A1	2/2005	Goode, Jr. et al.	2005/0271546	A1	12/2005	Gerber et al.
2005/0027462	A1	2/2005	Goode, Jr. et al.	2005/0271547	A1	12/2005	Gerber et al.
2005/0027463	A1	2/2005	Goode, Jr. et al.	2005/0272640	A1	12/2005	Doyle, III et al.
2005/0031689	A1	2/2005	Shults et al.	2005/0272985	A1	12/2005	Kotulla et al.
2005/0033132	A1	2/2005	Shults et al.	2005/0277164	A1	12/2005	Drucker et al.
2005/0038680	A1	2/2005	McMahon	2005/0277912	A1	12/2005	John
2005/0043598	A1	2/2005	Goode, Jr. et al.	2005/0287620	A1	12/2005	Heller et al.
2005/0043894	A1	2/2005	Fernandez	2006/0001538	A1	1/2006	Kraft et al.
2005/0049179	A1	3/2005	Davidson et al.	2006/0001550	A1	1/2006	Mann et al.
2005/0049473	A1	3/2005	Desai et al.	2006/0001551	A1	1/2006	Kraft et al.
2005/0051427	A1	3/2005	Brauker et al.	2006/0003398	A1	1/2006	Heller et al.
2005/0051440	A1	3/2005	Simpson et al.	2006/0004270	A1	1/2006	Bedard et al.
2005/0054909	A1	3/2005	Petisce et al.	2006/0004271	A1	1/2006	Peyser et al.
2005/0056552	A1	3/2005	Simpson et al.	2006/0007017	A1	1/2006	Mann et al.
2005/0059372	A1	3/2005	Arayashiki et al.	2006/0015020	A1	1/2006	Neale et al.
2005/0065464	A1	3/2005	Talbot et al.	2006/0015024	A1	1/2006	Brister et al.
2005/0070777	A1	3/2005	Cho et al.	2006/0016700	A1	1/2006	Brister et al.
2005/0090607	A1	4/2005	Tapsak et al.	2006/0019327	A1	1/2006	Brister et al.
2005/0096511	A1	5/2005	Fox et al.	2006/0020186	A1	1/2006	Brister et al.
2005/0096512	A1	5/2005	Fox et al.	2006/0020187	A1	1/2006	Brister et al.
2005/0096516	A1	5/2005	Soykan et al.	2006/0020188	A1	1/2006	Kamath et al.
2005/0112169	A1	5/2005	Brauker et al.	2006/0020189	A1	1/2006	Brister et al.
2005/0112544	A1	5/2005	Xu et al.	2006/0020190	A1	1/2006	Kamath et al.
2005/0113648	A1	5/2005	Yang et al.	2006/0020191	A1	1/2006	Brister et al.
2005/0113657	A1	5/2005	Alarcon et al.	2006/0020192	A1	1/2006	Brister et al.
2005/0113658	A1	5/2005	Jacobson et al.	2006/0025663	A1	2/2006	Talbot et al.
2005/0113886	A1	5/2005	Fischell et al.	2006/0029177	A1	2/2006	Cranford, Jr. et al.
2005/0114068	A1	5/2005	Chey et al.	2006/0031094	A1	2/2006	Cohen et al.
2005/0116683	A1	6/2005	Cheng et al.	2006/0036139	A1	2/2006	Brister et al.
2005/0118726	A1	6/2005	Schultz et al.	2006/0036140	A1	2/2006	Brister et al.
2005/0121322	A1	6/2005	Say et al.	2006/0036141	A1	2/2006	Kamath et al.
2005/0124873	A1	6/2005	Shults et al.	2006/0036142	A1	2/2006	Brister et al.
2005/0131346	A1	6/2005	Douglas	2006/0036143	A1	2/2006	Brister et al.
2005/0137471	A1	6/2005	Haar et al.	2006/0036144	A1	2/2006	Brister et al.
2005/0143635	A1	6/2005	Kamath et al.	2006/0036145	A1	2/2006	Brister et al.
2005/0143636	A1	6/2005	Zhang et al.	2006/0036187	A1	2/2006	Vos et al.
2005/0143675	A1	6/2005	Neel et al.	2006/0040402	A1	2/2006	Brauker et al.
2005/0148003	A1	7/2005	Kieth et al.	2006/0052679	A1	3/2006	Kotulla et al.
2005/0154271	A1	7/2005	Rasdal et al.	2006/0058588	A1	3/2006	Zdeblick
2005/0161346	A1	7/2005	Simpson et al.	2006/0058602	A1	3/2006	Kwiatkowski et al.
2005/0171503	A1	8/2005	Van Den Berghe et al.	2006/0063218	A1	3/2006	Bartkowiak et al.
				2006/0068208	A1	3/2006	Tapsak et al.
				2006/0074564	A1	4/2006	Bartowiak et al.
				2006/0086624	A1	4/2006	Tapsak et al.
				2006/0129733	A1	6/2006	Solbelman

(56)

References Cited

U.S. PATENT DOCUMENTS

2006/0142651 A1	6/2006	Brister et al.	2007/0153705 A1	7/2007	Rosar et al.
2006/0154642 A1	7/2006	Scannell	2007/0156033 A1	7/2007	Causey, III et al.
2006/0155180 A1	7/2006	Brister et al.	2007/0156094 A1	7/2007	Safabash et al.
2006/0166629 A1	7/2006	Reggiardo	2007/0161879 A1	7/2007	Say et al.
2006/0173260 A1	8/2006	Gaoni et al.	2007/0161880 A1	7/2007	Say et al.
2006/0173406 A1	8/2006	Hayes et al.	2007/0163880 A1	7/2007	Woo et al.
2006/0173444 A1	8/2006	Choy et al.	2007/0168224 A1	7/2007	Letzt et al.
2006/0183984 A1	8/2006	Dobbles et al.	2007/0173706 A1	7/2007	Neinast et al.
2006/0183985 A1	8/2006	Brister et al.	2007/0173712 A1	7/2007	Shah et al.
2006/0189856 A1	8/2006	Petisce et al.	2007/0173761 A1	7/2007	Kanderian et al.
2006/0189863 A1	8/2006	Peyser et al.	2007/0179349 A1	8/2007	Hoyme et al.
2006/0193375 A1	8/2006	Lee et al.	2007/0179352 A1	8/2007	Randlov et al.
2006/0195029 A1	8/2006	Shults et al.	2007/0179370 A1	8/2007	Say et al.
2006/0198426 A1	9/2006	Partyka	2007/0179372 A1	8/2007	Say et al.
2006/0198864 A1	9/2006	Shults et al.	2007/0191699 A1	8/2007	Say et al.
2006/0200019 A1	9/2006	Petisce et al.	2007/0191700 A1	8/2007	Say et al.
2006/0200020 A1	9/2006	Brister et al.	2007/0191702 A1	8/2007	Yodfat et al.
2006/0200022 A1	9/2006	Brauker et al.	2007/0197889 A1	8/2007	Brister et al.
2006/0200112 A1	9/2006	Paul	2007/0203408 A1	8/2007	Say et al.
2006/0202805 A1	9/2006	Schulman et al.	2007/0203410 A1	8/2007	Say et al.
2006/0202859 A1	9/2006	Mastrototaro et al.	2007/0203411 A1	8/2007	Say et al.
2006/0211921 A1	9/2006	Brauker et al.	2007/0203966 A1	8/2007	Brauker et al.
2006/0222566 A1	10/2006	Brauker et al.	2007/0208244 A1	9/2007	Brauker et al.
2006/0224108 A1	10/2006	Brauker et al.	2007/0208245 A1	9/2007	Brauker et al.
2006/0224141 A1	10/2006	Rush et al.	2007/0208246 A1	9/2007	Brauker et al.
2006/0226985 A1	10/2006	Goodnow et al.	2007/0208247 A1	9/2007	Say et al.
2006/0229512 A1	10/2006	Petisce et al.	2007/0213610 A1	9/2007	Say et al.
2006/0235285 A1	10/2006	Brister et al.	2007/0213611 A1	9/2007	Simpson et al.
2006/0247710 A1	11/2006	Goetz et al.	2007/0215491 A1	9/2007	Heller et al.
2006/0247985 A1	11/2006	Liamos et al.	2007/0218097 A1	9/2007	Heller et al.
2006/0253296 A1	11/2006	Liisberg et al.	2007/0219496 A1	9/2007	Kamen et al.
2006/0258918 A1	11/2006	Burd et al.	2007/0222609 A1	9/2007	Duron et al.
2006/0258929 A1	11/2006	Goode, Jr. et al.	2007/0232877 A1	10/2007	He
2006/0263763 A1	11/2006	Simpson et al.	2007/0232880 A1	10/2007	Siddiqui et al.
2006/0264785 A1	11/2006	Dring et al.	2007/0235331 A1	10/2007	Simpson et al.
2006/0264888 A1	11/2006	Moberg et al.	2007/0244380 A1	10/2007	Say et al.
2006/0270922 A1	11/2006	Brauker et al.	2007/0244383 A1	10/2007	Talbot et al.
2006/0270923 A1	11/2006	Brauker et al.	2007/0249919 A1	10/2007	Say et al.
2006/0272652 A1	12/2006	Stocker et al.	2007/0249920 A1	10/2007	Say et al.
2006/0276714 A1	12/2006	Holt et al.	2007/0249922 A1	10/2007	Peyser et al.
2006/0287691 A1	12/2006	Drew	2007/0253021 A1	11/2007	Mehta et al.
2006/0290496 A1	12/2006	Peeters et al.	2007/0255321 A1	11/2007	Gelber et al.
2006/0293607 A1	12/2006	Alt et al.	2007/0255348 A1	11/2007	Holtzclaw
2007/0007133 A1	1/2007	Mang et al.	2007/0255531 A1	11/2007	Drew
2007/0016381 A1	1/2007	Kamath et al.	2007/0258395 A1	11/2007	Jollota et al.
2007/0017983 A1	1/2007	Frank et al.	2007/0271285 A1	11/2007	Eichorn et al.
2007/0026440 A1	2/2007	Broderick et al.	2007/0282299 A1	12/2007	Hellwig
2007/0027381 A1	2/2007	Stafford	2007/0285238 A1	12/2007	Batra
2007/0027384 A1	2/2007	Brister et al.	2007/0299617 A1	12/2007	Willis
2007/0027385 A1	2/2007	Brister et al.	2008/0009304 A1	1/2008	Fry
2007/0027507 A1	2/2007	Burdett et al.	2008/0018433 A1	1/2008	Pitt-Pladdy
2007/0032706 A1	2/2007	Kamath et al.	2008/0021436 A1	1/2008	Wolpert et al.
2007/0032717 A1	2/2007	Brister et al.	2008/0021666 A1	1/2008	Goode, Jr. et al.
2007/0032718 A1	2/2007	Shults et al.	2008/0027586 A1	1/2008	Hern et al.
2007/0033074 A1	2/2007	Nitzan et al.	2008/0030369 A1	2/2008	Mann et al.
2007/0045902 A1	3/2007	Brauker et al.	2008/0033254 A1	2/2008	Kamath et al.
2007/0053341 A1	3/2007	Lizzi	2008/0033271 A1	2/2008	Say et al.
2007/0055799 A1	3/2007	Koehler et al.	2008/0045824 A1	2/2008	Tapsak et al.
2007/0060814 A1	3/2007	Stafford	2008/0055070 A1	3/2008	Bange et al.
2007/0060869 A1	3/2007	Tolle et al.	2008/0057484 A1	3/2008	Miyata et al.
2007/0066873 A1	3/2007	Kamath et al.	2008/0058626 A1	3/2008	Miyata et al.
2007/0066877 A1	3/2007	Arnold et al.	2008/0058678 A1	3/2008	Miyata et al.
2007/0071681 A1	3/2007	Gadkar et al.	2008/0058773 A1	3/2008	John
2007/0073129 A1	3/2007	Shah et al.	2008/0060955 A1	3/2008	Goodnow
2007/0078320 A1	4/2007	Stafford	2008/0061961 A1	3/2008	John
2007/0078321 A1	4/2007	Mazza et al.	2008/0062055 A1	3/2008	Cunningham et al.
2007/0090511 A1	4/2007	Borland et al.	2008/0064943 A1	3/2008	Talbot et al.
2007/0093704 A1	4/2007	Brister et al.	2008/0067627 A1	3/2008	Boeck et al.
2007/0100222 A1	5/2007	Mastrototaro et al.	2008/0071156 A1	3/2008	Brister et al.
2007/0106133 A1	5/2007	Satchwell et al.	2008/0071328 A1	3/2008	Haubrich et al.
2007/0106135 A1	5/2007	Sloan et al.	2008/0076997 A1	3/2008	Peyser et al.
2007/0124002 A1	5/2007	Estes et al.	2008/0083617 A1	4/2008	Simpson et al.
2007/0149873 A1	6/2007	Say et al.	2008/0086039 A1	4/2008	Heller et al.
2007/0149874 A1	6/2007	Say et al.	2008/0086040 A1	4/2008	Heller et al.
2007/0151869 A1	7/2007	Heller et al.	2008/0086041 A1	4/2008	Heller et al.
			2008/0086042 A1	4/2008	Brister et al.
			2008/0086043 A1	4/2008	Heller et al.
			2008/0086044 A1	4/2008	Brister et al.
			2008/0086273 A1	4/2008	Shults et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0091094	A1	4/2008	Heller et al.	2009/0043182	A1	2/2009	Brauker et al.
2008/0091095	A1	4/2008	Heller et al.	2009/0043525	A1	2/2009	Brauker et al.
2008/0091096	A1	4/2008	Say et al.	2009/0043541	A1	2/2009	Brauker et al.
2008/0092638	A1	4/2008	Brenneman et al.	2009/0043542	A1	2/2009	Brauker et al.
2008/0097289	A1	4/2008	Steil et al.	2009/0045055	A1	2/2009	Rhodes et al.
2008/0108942	A1	5/2008	Brister et al.	2009/0048503	A1	2/2009	Dalal et al.
2008/0119705	A1	5/2008	Patel et al.	2009/0054747	A1	2/2009	Fennell
2008/0139910	A1	6/2008	Mastrototaro et al.	2009/0055149	A1	2/2009	Hayter et al.
2008/0154513	A1	6/2008	Kovatchev et al.	2009/0062633	A1	3/2009	Brauker et al.
2008/0167543	A1	7/2008	Say et al.	2009/0062634	A1	3/2009	Say et al.
2008/0167572	A1	7/2008	Stivoric et al.	2009/0062635	A1	3/2009	Brauker et al.
2008/0172205	A1	7/2008	Breton et al.	2009/0062767	A1	3/2009	VanAntwerp et al.
2008/0179187	A1	7/2008	Ouyang et al.	2009/0063402	A1	3/2009	Hayter
2008/0183060	A1	7/2008	Steil et al.	2009/0069655	A1	3/2009	Say et al.
2008/0183061	A1	7/2008	Goode, Jr. et al.	2009/0069656	A1	3/2009	Say et al.
2008/0183399	A1	7/2008	Goode, Jr. et al.	2009/0069657	A1	3/2009	Say et al.
2008/0188731	A1	8/2008	Brister et al.	2009/0069658	A1	3/2009	Say et al.
2008/0188796	A1	8/2008	Steil et al.	2009/0076356	A1	3/2009	Simpson et al.
2008/0189051	A1	8/2008	Goode, Jr. et al.	2009/0076359	A1	3/2009	Peyser et al.
2008/0194934	A1	8/2008	Ray et al.	2009/0076360	A1	3/2009	Brister et al.
2008/0194935	A1	8/2008	Brister et al.	2009/0076361	A1	3/2009	Kamath et al.
2008/0194936	A1	8/2008	Goode, Jr. et al.	2009/0085768	A1	4/2009	Patel et al.
2008/0194937	A1	8/2008	Goode, Jr. et al.	2009/0085873	A1	4/2009	Betts et al.
2008/0194938	A1	8/2008	Brister et al.	2009/0089999	A1	4/2009	Say et al.
2008/0195232	A1	8/2008	Carr-Brendel et al.	2009/0093687	A1	4/2009	Telfort et al.
2008/0195967	A1	8/2008	Goode, Jr. et al.	2009/0093696	A1	4/2009	Say et al.
2008/0197024	A1	8/2008	Simpson et al.	2009/0094680	A1	4/2009	Gupta et al.
2008/0200788	A1	8/2008	Brister et al.	2009/0099432	A1	4/2009	Say et al.
2008/0200789	A1	8/2008	Brister et al.	2009/0099435	A1	4/2009	Say et al.
2008/0200791	A1	8/2008	Simpson et al.	2009/0099436	A1	4/2009	Brister et al.
2008/0208025	A1	8/2008	Shults et al.	2009/0105554	A1	4/2009	Stahmann et al.
2008/0208113	A1	8/2008	Damiano et al.	2009/0105560	A1	4/2009	Solomon
2008/0212600	A1	9/2008	Yoo	2009/0112478	A1	4/2009	Mueller, Jr. et al.
2008/0214914	A1	9/2008	Say et al.	2009/0124877	A1	5/2009	Goode, Jr. et al.
2008/0214915	A1	9/2008	Brister et al.	2009/0124878	A1	5/2009	Goode, Jr. et al.
2008/0214918	A1	9/2008	Brister et al.	2009/0124879	A1	5/2009	Brister et al.
2008/0228051	A1	9/2008	Shults et al.	2009/0124964	A1	5/2009	Leach et al.
2008/0228054	A1	9/2008	Shults et al.	2009/0131768	A1	5/2009	Simpson et al.
2008/0234943	A1	9/2008	Ray et al.	2009/0131769	A1	5/2009	Leach et al.
2008/0235469	A1	9/2008	Drew	2009/0131776	A1	5/2009	Simpson et al.
2008/0242961	A1	10/2008	Brister et al.	2009/0131777	A1	5/2009	Simpson et al.
2008/0254544	A1	10/2008	Modzelewski et al.	2009/0137886	A1	5/2009	Shariati et al.
2008/0255438	A1	10/2008	Saidara et al.	2009/0137887	A1	5/2009	Shariati et al.
2008/0262329	A1	10/2008	Say et al.	2009/0143659	A1	6/2009	Li et al.
2008/0262469	A1	10/2008	Brister et al.	2009/0143660	A1	6/2009	Brister et al.
2008/0267823	A1	10/2008	Wang et al.	2009/0146826	A1	6/2009	Gofman et al.
2008/0269672	A1	10/2008	Say et al.	2009/0149717	A1	6/2009	Brauer et al.
2008/0275313	A1	11/2008	Brister et al.	2009/0150186	A1	6/2009	Cohen et al.
2008/0287764	A1	11/2008	Rasdal et al.	2009/0156919	A1	6/2009	Brister et al.
2008/0287765	A1	11/2008	Rasdal et al.	2009/0156924	A1	6/2009	Shariati et al.
2008/0287766	A1	11/2008	Rasdal et al.	2009/0163781	A1	6/2009	Say et al.
2008/0294024	A1	11/2008	Cosentino et al.	2009/0163788	A1	6/2009	Say et al.
2008/0296155	A1	12/2008	Shults et al.	2009/0163789	A1	6/2009	Say et al.
2008/0300572	A1	12/2008	Rankers et al.	2009/0163790	A1	6/2009	Brister et al.
2008/0300919	A1	12/2008	Charlton et al.	2009/0163791	A1	6/2009	Brister et al.
2008/0300920	A1	12/2008	Brown et al.	2009/0171179	A1	7/2009	Say et al.
2008/0301158	A1	12/2008	Brown et al.	2009/0173628	A1	7/2009	Say et al.
2008/0301436	A1	12/2008	Yao et al.	2009/0177054	A1	7/2009	Say et al.
2008/0301665	A1	12/2008	Charlton et al.	2009/0177055	A1	7/2009	Say et al.
2008/0306368	A1	12/2008	Goode, Jr. et al.	2009/0177056	A1	7/2009	Say et al.
2008/0306434	A1	12/2008	Dobbles et al.	2009/0177057	A1	7/2009	Say et al.
2008/0306435	A1	12/2008	Kamath et al.	2009/0177058	A1	7/2009	Say et al.
2008/0306444	A1	12/2008	Brister et al.	2009/0177059	A1	7/2009	Say et al.
2008/0312518	A1	12/2008	Jina et al.	2009/0177060	A1	7/2009	Say et al.
2008/0319292	A1	12/2008	Say et al.	2009/0177061	A1	7/2009	Say et al.
2008/0320587	A1	12/2008	Vauclair et al.	2009/0177062	A1	7/2009	Say et al.
2009/0005666	A1	1/2009	Shin et al.	2009/0177063	A1	7/2009	Say et al.
2009/0006133	A1	1/2009	Weinert et al.	2009/0177064	A1	7/2009	Say et al.
2009/0012379	A1	1/2009	Goode, Jr. et al.	2009/0177065	A1	7/2009	Say et al.
2009/0018424	A1	1/2009	Kamath et al.	2009/0177066	A1	7/2009	Say et al.
2009/0030294	A1	1/2009	Petisce et al.	2009/0178459	A1	7/2009	Li et al.
2009/0036758	A1	2/2009	Brauker et al.	2009/0182212	A1	7/2009	Say et al.
2009/0036763	A1	2/2009	Brauker et al.	2009/0182213	A1	7/2009	Say et al.
2009/0040022	A1	2/2009	Finkenzeller	2009/0182214	A1	7/2009	Say et al.
2009/0043181	A1	2/2009	Brauker et al.	2009/0182215	A1	7/2009	Say et al.
				2009/0182217	A1	7/2009	Li et al.
				2009/0187088	A1	7/2009	Say et al.
				2009/0187089	A1	7/2009	Say et al.
				2009/0187090	A1	7/2009	Say et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2009/0187091 A1 7/2009 Say et al.
 2009/0187092 A1 7/2009 Say et al.
 2009/0187093 A1 7/2009 Say et al.
 2009/0187094 A1 7/2009 Say et al.
 2009/0187095 A1 7/2009 Say et al.
 2009/0189738 A1 7/2009 Hermle
 2009/0192366 A1 7/2009 Mensinger et al.
 2009/0192368 A1 7/2009 Say et al.
 2009/0192369 A1 7/2009 Say et al.
 2009/0192370 A1 7/2009 Say et al.
 2009/0192371 A1 7/2009 Say et al.
 2009/0192372 A1 7/2009 Say et al.
 2009/0192373 A1 7/2009 Say et al.
 2009/0192374 A1 7/2009 Say et al.
 2009/0192375 A1 7/2009 Say et al.
 2009/0192376 A1 7/2009 Say et al.
 2009/0192377 A1 7/2009 Say et al.
 2009/0192378 A1 7/2009 Say et al.
 2009/0192379 A1 7/2009 Say et al.
 2009/0192380 A1 7/2009 Shariati et al.
 2009/0192722 A1 7/2009 Shariati et al.
 2009/0192724 A1 7/2009 Brauker et al.
 2009/0192745 A1 7/2009 Kamath et al.
 2009/0192751 A1 7/2009 Kamath et al.
 2009/0198115 A1 8/2009 Say et al.
 2009/0198116 A1 8/2009 Say et al.
 2009/0198175 A1 8/2009 Say et al.
 2009/0203978 A1 8/2009 Say et al.
 2009/0203981 A1 8/2009 Brauker et al.
 2009/0204341 A1 8/2009 Brauker et al.
 2009/0209838 A1 8/2009 Say et al.
 2009/0216101 A1 8/2009 Say et al.
 2009/0216103 A1 8/2009 Brister et al.
 2009/0227940 A1 9/2009 Say et al.
 2009/0227941 A1 9/2009 Say et al.
 2009/0228214 A1 9/2009 Say et al.
 2009/0234200 A1 9/2009 Husheer
 2009/0237216 A1 9/2009 Twitchell, Jr.
 2009/0240120 A1 9/2009 Mensinger et al.
 2009/0240128 A1 9/2009 Mensinger et al.
 2009/0240193 A1 9/2009 Mensinger et al.
 2009/0242399 A1 10/2009 Kamath et al.
 2009/0242425 A1 10/2009 Kamath et al.
 2009/0247855 A1 10/2009 Boock et al.
 2009/0247856 A1 10/2009 Boock et al.
 2009/0247931 A1 10/2009 Damgaard-Sorensen
 2009/0253973 A1 10/2009 Bashan et al.
 2009/0267765 A1 10/2009 Greene et al.
 2009/0287073 A1 11/2009 Boock et al.
 2009/0287074 A1 11/2009 Shults et al.
 2009/0289796 A1 11/2009 Blumberg
 2009/0298182 A1 12/2009 Schulat et al.
 2009/0299155 A1 12/2009 Yang et al.
 2009/0299156 A1 12/2009 Simpson et al.
 2009/0299162 A1 12/2009 Brauker et al.
 2009/0299276 A1 12/2009 Brauker et al.
 2010/0010324 A1 1/2010 Brauker et al.
 2010/0010329 A1 1/2010 Taub et al.
 2010/0010331 A1 1/2010 Brauker et al.
 2010/0010332 A1 1/2010 Brauker et al.
 2010/0016687 A1 1/2010 Brauker et al.
 2010/0016698 A1 1/2010 Rasdal et al.
 2010/0022855 A1 1/2010 Brauker et al.
 2010/0025238 A1 2/2010 Gottlieb et al.
 2010/0030038 A1 2/2010 Brauker et al.
 2010/0030053 A1 2/2010 Goode, Jr. et al.
 2010/0030484 A1 2/2010 Brauker et al.
 2010/0030485 A1 2/2010 Brauker et al.
 2010/0036215 A1 2/2010 Goode, Jr. et al.
 2010/0036216 A1 2/2010 Goode, Jr. et al.
 2010/0036222 A1 2/2010 Goode, Jr. et al.
 2010/0036223 A1 2/2010 Goode, Jr. et al.
 2010/0036225 A1 2/2010 Goode, Jr. et al.
 2010/0041971 A1 2/2010 Goode, Jr. et al.
 2010/0045465 A1 2/2010 Brauker et al.

2010/0049024 A1 2/2010 Saint et al.
 2010/0063373 A1 3/2010 Kamath et al.
 2010/0076283 A1 3/2010 Simpson et al.
 2010/0081908 A1 4/2010 Dobbles et al.
 2010/0081910 A1 4/2010 Brister et al.
 2010/0087724 A1 4/2010 Brauker et al.
 2010/0096259 A1 4/2010 Zhang et al.
 2010/0099970 A1 4/2010 Shults et al.
 2010/0099971 A1 4/2010 Shults et al.
 2010/0110931 A1 5/2010 Shim et al.
 2010/0119693 A1 5/2010 Tapsak et al.
 2010/0119881 A1 5/2010 Patel et al.
 2010/0121169 A1 5/2010 Petisce et al.
 2010/0160759 A1 6/2010 Celentano et al.
 2010/0168538 A1 7/2010 Keenan et al.
 2010/0174266 A1 7/2010 Estes
 2010/0185175 A1 7/2010 Kamen et al.
 2010/0190435 A1 7/2010 Cook et al.
 2010/0213080 A1 8/2010 Celentano et al.
 2010/0235439 A1 9/2010 Goodnow et al.
 2010/0267161 A1 10/2010 Wu et al.
 2010/0312176 A1 12/2010 Lauer et al.
 2010/0313105 A1 12/2010 Nekoomaram et al.
 2010/0332142 A1 12/2010 Shadforth et al.
 2011/0004276 A1 1/2011 Blair et al.
 2011/0031986 A1 2/2011 Bhat et al.
 2011/0074349 A1 3/2011 Ghovanloo
 2011/0125040 A1 5/2011 Crawford et al.
 2011/0148905 A1 6/2011 Simmons et al.
 2011/0152637 A1 6/2011 Kateraas et al.
 2011/0184268 A1 * 7/2011 Taub A61B 5/14532
 600/365
 2011/0191059 A1 8/2011 Farrell et al.
 2011/0230741 A1 9/2011 Liang et al.
 2011/0257895 A1 10/2011 Brauker et al.
 2011/0270112 A1 11/2011 Manera et al.
 2011/0287528 A1 11/2011 Fern et al.
 2012/0108931 A1 * 5/2012 Taub A61B 5/14532
 600/347
 2012/0148054 A1 6/2012 Rank et al.
 2012/0190989 A1 7/2012 Kaiser et al.
 2012/0215092 A1 * 8/2012 Harris, III H04B 7/0602
 600/410
 2013/0035575 A1 2/2013 Mayou et al.
 2013/0235166 A1 9/2013 Jones et al.

FOREIGN PATENT DOCUMENTS

DE 3934299 10/1990
 DE 4234553 1/1995
 DE 4401400 7/1995
 EP 0010375 4/1980
 EP 0026995 4/1981
 EP 0048090 3/1982
 EP 0078636 5/1983
 EP 0080304 6/1983
 EP 0096228 12/1983
 EP 0096288 12/1983
 EP 0098592 1/1984
 EP 0125139 11/1984
 EP 0127958 12/1984
 EP 0136362 4/1985
 EP 0170375 2/1986
 EP 0177743 4/1986
 EP 0184909 6/1986
 EP 0206218 12/1986
 EP 0230472 8/1987
 EP 0241309 10/1987
 EP 0245073 11/1987
 EP 0255291 2/1988
 EP 0278647 8/1988
 EP 0320109 6/1989
 EP 0353328 2/1990
 EP 0359831 3/1990
 EP 0368209 5/1990
 EP 0368290 5/1990
 EP 0390390 10/1990
 EP 0396788 11/1990
 EP 0400918 12/1990

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	0453283	10/1991	WO	WO-1990/005300	5/1990
EP	0470290	2/1992	WO	WO-1990/005910	5/1990
EP	0504835	9/1992	WO	WO-1991/001680	2/1991
EP	0286118	1/1995	WO	WO-1991/004704	4/1991
EP	0653718	5/1995	WO	WO-1991/015993	10/1991
EP	0800082	10/1997	WO	WO-1992/013271	8/1992
EP	0880936	12/1998	WO	WO-1994/020602	9/1994
EP	0970655	1/2000	WO	WO-1994/027140	11/1994
EP	1034734	9/2000	WO	WO-1995/006240	3/1995
EP	1048264	11/2000	WO	WO-1996/007908	3/1996
EP	1445893	8/2004	WO	WO-1996/014026	5/1996
GB	1394171	5/1975	WO	WO-1996/025089	8/1996
GB	1579690	11/1980	WO	WO-1996/030431	10/1996
GB	1599241	9/1981	WO	WO-1996/035370	11/1996
GB	2073891	10/1981	WO	WO-1997/019344	5/1997
GB	2154003	8/1985	WO	WO-1997/020207	6/1997
GB	2194892	3/1988	WO	WO-1997/041421	11/1997
GB	2204408	11/1988	WO	WO-1997/042882	11/1997
GB	2225637	6/1990	WO	WO-1997/042883	11/1997
GB	2254436	10/1992	WO	WO-1997/042886	11/1997
JP	54-041191	4/1979	WO	WO-1997/042888	11/1997
JP	55-010581	1/1980	WO	WO-1997/043962	11/1997
JP	55-010583	1/1980	WO	WO-1997/046868	12/1997
JP	55-010584	1/1980	WO	WO-1998/009167	3/1998
JP	55-012406	1/1980	WO	WO-1998/024358	6/1998
JP	56-163447	12/1981	WO	WO-1998/052045	11/1998
JP	57-070448	4/1982	WO	WO-1998/052293	11/1998
JP	60-173457	9/1985	WO	WO-1998/056293	12/1998
JP	60-173458	9/1985	WO	WO-1999/005966	2/1999
JP	60-173459	9/1985	WO	WO-1999/013574	3/1999
JP	60-210243	10/1985	WO	WO-1999/032883	7/1999
JP	61-090050	5/1986	WO	WO-1999/048419	9/1999
JP	62-085855	4/1987	WO	WO-1999/058051	11/1999
JP	62-114747	5/1987	WO	WO-1999/058973	11/1999
JP	63-058149	3/1988	WO	WO-2000/018294	4/2000
JP	63-128252	5/1988	WO	WO-2000/019887	4/2000
JP	63-139246	6/1988	WO	WO-2000/020626	4/2000
JP	63-294799	12/1988	WO	WO-2000/032098	6/2000
JP	63-317757	12/1988	WO	WO-2000/049940	8/2000
JP	63-317758	12/1988	WO	WO-2000/059370	10/2000
JP	1-114746	5/1989	WO	WO-2000/059373	10/2000
JP	1-114747	5/1989	WO	WO-2000/062665	10/2000
JP	1-124060	5/1989	WO	WO-2000/074753	12/2000
JP	1-134244	5/1989	WO	WO-2000/078210	12/2000
JP	1-156658	6/1989	WO	WO-2000/078992	12/2000
JP	2-062958	3/1990	WO	WO-2001/012158	2/2001
JP	2-120655	5/1990	WO	WO-2001/033216	5/2001
JP	2-287145	11/1990	WO	WO-2001/052727	7/2001
JP	2-310457	12/1990	WO	WO-2001/052935	7/2001
JP	3-026956	2/1991	WO	WO-2001/054753	8/2001
JP	3-028752	2/1991	WO	WO-2001/057238	8/2001
JP	3-202764	9/1991	WO	WO-2001/057239	8/2001
JP	5-072171	3/1993	WO	WO-2001/058348	8/2001
JP	5-196595	8/1993	WO	WO-2001/067009	9/2001
JP	6-190050	7/1994	WO	WO-2001/068901	9/2001
JP	7-055757	3/1995	WO	WO-2001/069222	9/2001
JP	7-072585	3/1995	WO	WO-2001/088524	11/2001
JP	8-154903	6/1996	WO	WO-2001/088534	11/2001
JP	8-285814	11/1996	WO	WO-2002/016905	2/2002
JP	8-285815	11/1996	WO	WO-2002/017210	2/2002
JP	9-021778	1/1997	WO	WO-2002/058537	8/2002
JP	9-101280	4/1997	WO	WO-2002/078512	10/2002
JP	9-285459	11/1997	WO	WO-2003/072269	9/2003
JP	10-170471	6/1998	WO	WO-2003/076893	9/2003
JP	2000-000231	1/2000	WO	WO-2003/082091	10/2003
JP	2000-116628	4/2000	WO	WO-2004/061420	7/2004
SU	1281988	1/1987	WO	WO-2005/010756	2/2005
WO	WO-1985/005119	11/1985	WO	WO-2005/089103	9/2005
WO	WO-1986/000513	1/1986	WO	WO-2006/119084	11/2006
WO	WO-1987/000513	1/1987	WO	WO-2007/002189	1/2007
WO	WO-1987/006040	10/1987	WO	WO-2007/016399	2/2007
WO	WO-1989/002246	3/1989	WO	WO-2007/027381	3/2007
WO	WO-1989/005119	6/1989	WO	WO-2007/027788	3/2007
WO	WO-1989/008713	9/1989	WO	WO-2007/051139	5/2007
WO	WO-1990/000367	1/1990	WO	WO-2007/053832	5/2007
			WO	WO-2007/056638	5/2007

OTHER PUBLICATIONS

(56)

References Cited

OTHER PUBLICATIONS

- Albery, W. J., et al., "Amperometric Enzyme Electrodes Part II: Conducting Salts as Electrode Materials for the Oxidation of Glucose Oxidase", *Journal of ElectroAnalytical Chemistry*, vol. 194, 1985, pp. 223-235.
- Albery, W. J., et al., "Amperometric Enzyme Electrodes", *Philosophical Transactions of The Royal Society of London*, vol. 316, 1987, pp. 107-119.
- Alcock, S. J., et al., "Continuous Analyte Monitoring to Aid Clinical Practice", *IEEE Engineering in Medicine and Biology Magazine*, 1994, pp. 319-325.
- Anderson, L. B., et al., "Thin-Layer Electrochemistry: Steady-State Methods of Studying Rate Processes", *Journal of ElectroAnalytical Chemistry*, vol. 10, 1965, pp. 295-305.
- Armour, J. C., et al., "Application of Chronic Intravascular Blood Glucose Sensor in Dogs", *Diabetes*, vol. 39, 1990, pp. 1519-1526.
- Bartlett, P. N., et al., "Covalent Binding of Electron Relays to Glucose Oxidase", *Journal of the Chemical Society, Chemical Communications*, 1987, pp. 1603-1604.
- Bartlett, P. N., et al., "Modification of Glucose Oxidase by Tetrathiafulvalene", *Journal of the Chemical Society, Chemical Communications*, 1990, pp. 1135-1136.
- Bartlett, P. N., et al., "Strategies for the Development of Amperometric Enzyme Electrodes", *Biosensors*, vol. 3, 1987/88, pp. 359-379.
- Bennion, N., et al., "Alternate Site Glucose Testing: A Crossover Design", *Diabetes Technology & Therapeutics*, vol. 4, No. 1, 2002, pp. 25-33.
- Bindra, D. S., et al., "Design and in Vitro Studies of a Needle-Type Glucose Sensor for Subcutaneous Monitoring", *Analytical Chemistry*, vol. 63, No. 17, 1991, pp. 1692-1696.
- Blank, T. B., et al., "Clinical Results From a Non-Invasive Blood Glucose Monitor", *Optical Diagnostics and Sensing of Biological Fluids and Glucose and Cholesterol Monitoring II, Proceedings of SPIE*, vol. 4624, 2002, pp. 1-10.
- Bobbioni-Harsch, E., et al., "Lifespan of Subcutaneous Glucose Sensors and Their Performances During Dynamic Glycaemia Changes in Rats", *Journal of Biomedical Engineering*, vol. 15, 1993, pp. 457-463.
- Boedeker Plastics, Inc., "Polyethylene Specifications", Web Page of Boedeker.com, 2007, pp. 1-3.
- Brandt, J., et al., "Covalent Attachment of Proteins to Polysaccharide Carriers by Means of Benzoquinone", *Biochimica et Biophysica Acta*, vol. 386, 1975, pp. 196-202.
- Brooks, S. L., et al., "Development of an On-Line Glucose Sensor for Fermentation Monitoring", *Biosensors*, vol. 3, 1987/88, pp. 45-56.
- Brownlee, M., et al., "A Glucose-Controlled Insulin-Delivery System: Semisynthetic Insulin Bound to Lectin", *Science*, vol. 206, 1979, 1190-1191.
- Cass, A. E., et al., "Ferricinium Ion As an Electron Acceptor for Oxido-Reductases", *Journal of ElectroAnalytical Chemistry*, vol. 190, 1985, pp. 117-127.
- Cass, A. E., et al., "Ferrocene-Medicated Enzyme Electrode for Amperometric Determination of Glucose", *Analytical Chemistry*, vol. 56, No. 4, 1984, 667-671.
- Castner, J. F., et al., "Mass Transport and Reaction Kinetic Parameters Determined Electrochemically for Immobilized Glucose Oxidase", *Biochemistry*, vol. 23 No. 10, 1984, 2203-2210.
- Claremont, D. J., et al., "Biosensors for Continuous In Vivo Glucose Monitoring", *Proceedings of the Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 10, 1988.
- Clark Jr., L. C., et al., "Differential Anodic Enzyme Polarography for the Measurement of Glucose", *Oxygen Transport to Tissue: Instrumentation, Methods, and Physiology*, 1973, pp. 127-133.
- Clark Jr., L. C., et al., "Electrode Systems for Continuous Monitoring in Cardiovascular Surgery", *Annals New York Academy of Sciences*, 1962, pp. 29-45.
- Clark Jr., L. C., et al., "Long-term Stability of Electroenzymatic Glucose Sensors Implanted in Mice", *American Society of Artificial Internal Organs Transactions*, vol. XXXIV, 1988, pp. 259-265.
- Clarke, W. L., et al., "Evaluating Clinical Accuracy of Systems for Self-Monitoring of Blood Glucose", *Diabetes Care*, vol. 10, No. 5, 1987, pp. 622-628.
- Csoregi, E., et al., "Design and Optimization of a Selective Subcutaneously Implantable Glucose Electrode Based on 'Wired' Glucose Oxidase", *Analytical Chemistry*, vol. 67, No. 7, 1995, pp. 1240-1244.
- Csoregi, E., et al., "Design, Characterization, and One-Point in Vivo Calibration of a Subcutaneously Implanted Glucose Electrode", *Analytical Chemistry*, vol. 66 No. 19, 1994, pp. 3131-3138.
- Csoregi, E., et al., "On-Line Glucose Monitoring by Using Microdialysis Sampling and Amperometric Detection Based on 'Wired' Glucose Oxidase in Carbon Paste", *Mikrochimica Acta*, vol. 121, 1995, pp. 31-40.
- Dai, W. S., et al., "Hydrogel Membranes with Mesh Size Asymmetry Based on the Gradient Crosslinking of Poly(vinyl alcohol)", *Journal of Membrane Science*, vol. 156, 1999, pp. 67-79.
- Davis, G., "Electrochemical Techniques for the Development of Amperometric Biosensors", *Biosensors*, vol. 1, 1985, pp. 161-178.
- Degani, Y., et al., "Direct Electrical Communication Between Chemically Modified Enzymes and Metal Electrodes. 1. Electron Transfer from Glucose Oxidase to Metal Electrodes via Electron Relays, Bound Covalently to the Enzyme", *The Journal of Physical Chemistry*, vol. 91, No. 6, 1987, pp. 1285-1289.
- Degani, Y., et al., "Direct Electrical Communication Between Chemically Modified Enzymes and Metal Electrodes. 2. Methods for Bonding Electron-Transfer Relays to Glucose Oxidase and D-Amino-Acid Oxidase", *Journal of the American Chemical Society*, vol. 110, No. 8, 1988, pp. 2615-2620.
- Degani, Y., et al., "Electrical Communication Between Redox Centers of Glucose Oxidase and Electrodes via Electrostatically and Covalently Bound Redox Polymers", *Journal of the American Chemical Society*, vol. 111, 1989, pp. 2357-2358.
- Denisevich, P., et al., "Unidirectional Current Flow and Charge State Trapping at Redox Polymer Interfaces on Bilayer Electrodes: Principles, Experimental Demonstration, and Theory", *Journal of the American Chemical Society*, vol. 103, 1981, pp. 4727-4737.
- Dicks, J. M., et al., "Ferrocene Modified Polypyrrole with Immobilised Glucose Oxidase and its Application in Amperometric Glucose Microbiosensors", *Annales de Biologie Clinique*, vol. 47, 1989, pp. 607-619.
- Ellis, C. D., et al., "Selectivity and Directed Charge Transfer through an Electroactive Metallopolymer Film", *Journal of the American Chemical Society*, vol. 103, No. 25, 1981, pp. 7480-7483.
- Engstrom, R. C., "Electrochemical Pretreatment of Glassy Carbon Electrodes", *Analytical Chemistry*, vol. 54, No. 13, 1982, pp. 2310-2314.
- Engstrom, R. C., et al., "Characterization of Electrochemically Pretreated Glassy Carbon Electrodes", *Analytical Chemistry*, vol. 56, No. 2, 1984, pp. 136-141.
- Feldman, B., et al., "A Continuous Glucose Sensor Based on Wired Enzyme™ Technology—Results from a 3-Day Trial in Patients with Type 1 Diabetes", *Diabetes Technology & Therapeutics*, vol. 5, No. 5, 2003, pp. 769-779.
- Feldman, B., et al., "Correlation of Glucose Concentrations in Interstitial Fluid and Venous Blood During Periods of Rapid Glucose Change", *Abbott Diabetes Care, Inc. Freestyle Navigator Continuous Glucose Monitor Pamphlet*, 2004.
- Feldman, B., et al., "Electron Transfer Kinetics at Redox Polymer/Solution Interfaces Using Microelectrodes and Twin Electrode Thin Layer Cells", *Journal of ElectroAnalytical Chemistry*, vol. 194, 1985, pp. 63-81.
- Fischer, H., et al., "Intramolecular Electron Transfer Medicated by 4,4'-Bipyridine and Related Bridging Groups", *Journal of the American Chemical Society*, vol. 98, No. 18, 1976, pp. 5512-5517.
- Flentge, F., et al., "An Enzyme-Reactor for Electrochemical Monitoring of Choline and Acetylcholine: Applications in High-Performance Liquid Chromatography, Brain Tissue, Microdialysis and Cerebrospinal Fluid", *Analytical Biochemistry*, vol. 204, 1992, pp. 305-310.

(56)

References Cited

OTHER PUBLICATIONS

- Foulds, N. C., et al., "Enzyme Entrapment in Electrically Conducting Polymers: Immobilisation of Glucose Oxidase in Polypyrrole and its Application in Amperometric Glucose Sensors", *Journal of the Chemical Society, Faraday Transactions 1*, vol. 82, 1986, pp. 1259-1264.
- Foulds, N. C., et al., "Immobilization of Glucose Oxidase in Ferrocene-Modified Pyrrole Polymers", *Analytical Chemistry*, vol. 60, No. 22, 1988, pp. 2473-2478.
- Frew, J. E., et al., "Electron-Transfer Biosensors", *Philosophical Transactions of The Royal Society of London*, vol. 316, 1987, pp. 95-106.
- Godsland, I. F., et al., "Maximizing the Success Rate of Minimal Model Insulin Sensitivity Measurement in Humans: The Importance of Basal Glucose Levels," *Clinical Science*, vol. 101, 2001, pp. 1-9.
- Gorton, L., et al., "Selective Detection in Flow Analysis Based on the Combination of Immobilized Enzymes and Chemically Modified Electrodes", *Analytica Chimica Acta*, vol. 250, 1991, pp. 203-248.
- Graham, N. B., "Poly(ethylene oxide) and Related Hydrogels," *Hydrogels in Medicine and Pharmacy*, vol. II: Polymers, Chapter 4, 1987, pp. 95-113.
- Gregg, B. A., et al., "Cross-Linked Redox Gels Containing Glucose Oxidase for Amperometric Biosensor Applications", *Analytical Chemistry*, vol. 62, No. 3, 1990, pp. 258-263.
- Gregg, B. A., et al., "Redox Polymer Films Containing Enzymes. I. A Redox-Conducting Epoxy Cement: Synthesis, Characterization, and Electrocatalytic Oxidation of Hydroquinone", *Journal of Physical Chemistry*, vol. 95, No. 15, 1991, 5970-5975.
- Hale, P. D., et al., "A New Class of Amperometric Biosensor Incorporating a Polymeric Electron-Transfer Mediator", *Journal of the American Chemical Society*, vol. 111, No. 9, 1989, pp. 3482-3484.
- Hamilton, "Hamilton Needle Gauge Index", www.hamiltoncompany.com.
- Harrison, D. J., et al., "Characterization of Perfluorosulfonic Acid Polymer Coated Enzyme Electrodes and a Miniatureized Integrated Potentiostat for Glucose Analysis in Whole Blood", *Analytical Chemistry*, vol. 60, No. 19, 1988, pp. 2002-2007.
- Hawkrigde, F. M., et al., "Indirect Coulometric Titration of Biological Electron Transport Components", *Analytical Chemistry*, vol. 45, No. 7, 1973, pp. 1021-1027.
- Heller, A., "Electrical Connection Enzyme Redox Centers to Electrodes", *Journal of Physical Chemistry*, vol. 96, No. 9, 1990, pp. 3579-3587.
- Heller, A., "Electrical Wiring of Redox Enzymes", *Accounts of Chemical Research* vol. 23, No. 5, 1990, 128-134.
- Heller, A., et al., "Amperometric Biosensors Based on Three-Dimensional Hydrogel-Forming Epoxy Networks", *Sensors and Actuators B*, vol. 13-14, 1993, pp. 180-183.
- Ianniello, R. M., et al., "Differential Pulse Voltammetric Study of Direct Electron Transfer in Glucose Oxidase Chemically Modified Graphite Electrodes", *Analytical Chemistry*, vol. 54, No. 7, 1982, pp. 1098-1101.
- Ianniello, R. M., et al., "Immobilized Enzyme Chemically Modified Electrode as an Amperometric Sensor", *Analytical Chemistry*, vol. 53, No. 13, 1981, pp. 2090-2095.
- Ikeda, T., et al., "Glucose Oxidase-Immobilized Benzoquinone-Carbon Paste Electrode as a Glucose Sensor", *Agricultural and Biological Chemistry*, vol. 49, No. 2, 1985, pp. 541-543.
- Ikeda, T., et al., "Kinetics of Outer-Sphere Electron Transfers Between Metal Complexes in Solutions and Polymeric Films on Modified Electrodes", *Journal of the American Chemical Society*, vol. 103, No. 25, 1981, pp. 7422-7425.
- Johnson, J. M., et al., "Potential-Dependent Enzymatic Activity in an Enzyme Thin-Layer Cell", *Analytical Chemistry*, vol. 54, No. 8, 1982, pp. 1377-1383.
- Johnson, K. W., "Reproducible Electrodeposition of Biomolecules for the Fabrication of Miniature Electroenzymatic Biosensors", *Sensors and Actuators B*, vol. 5, 1991, pp. 85-89.
- Johnson, K. W., et al., "In vivo Evaluation of an Electroenzymatic Glucose Sensor Implanted in Subcutaneous Tissue", *Biosensors & Bioelectronics*, vol. 7, 1992, pp. 709-714.
- Johnson, P. C., "Peripheral Circulation", *John Wiley & Sons*, 1978, pp. 198.
- Jonsson, G., et al., "An Amperometric Glucose Sensor Made by Modification of a Graphite Electrode Surface With Immobilized Glucose Oxidase and Adsorbed Mediator", *Biosensors*, vol. 1, 1985, pp. 355-368.
- Josowicz, M., et al., "Electrochemical Pretreatment of Thin Film Platinum Electrodes", *Journal of the Electrochemical Society*, vol. 135 No. 1, 1988, pp. 112-115.
- Jungheim, K., et al., "How Rapid Does Glucose Concentration Change in Daily Life of Patients with Type 1 Diabetes?", *Second Annual Diabetes Technology Meeting*, 2002, pp. A61-A62.
- Jungheim, K., et al., "Risky Delay of Hypoglycemia Detection by Glucose Monitoring at the Arm", *Diabetes Care*, vol. 24, No. 7, 2001, pp. 1303-1304.
- Kaplan, S. M., "Wiley Electrical and Electronics Engineering Dictionary", *IEEE Press*, 2004, pp. 141, 142, 548, 549.
- Katakis, I., et al., "Electrostatic Control of the Electron Transfer Enabling Binding of Recombinant Glucose Oxidase and Redox Polyelectrolytes", *Journal of the American Chemical Society*, vol. 116, No. 8, 1994, pp. 3617-3618.
- Katakis, I., et al., "L- α -Glycerophosphate and L-Lactate Electrodes Based on the Electrochemical 'Wiring' of Oxidases", *Analytical Chemistry*, vol. 64, No. 9, 1992, pp. 1008-1013.
- Kemp, G. J., "Theoretical Aspects of One-Point Calibration: Causes and Effects of Some Potential Errors, and Their Dependence on Concentration," *Clinical Chemistry*, vol. 30, No. 7, 1984, pp. 1163-1167.
- Kenausis, G., et al., "'Wiring' of Glucose Oxidase and Lactate Oxidase Within a Hydrogel Made with Poly(vinyl pyridine) complexed with [Os(4,4'-dimethoxy-2,2'-bipyridine)₂Cl]⁺²", *Journal of the Chemical Society, Faraday Transactions*, vol. 92, No. 20, 1996, pp. 4131-4136.
- Kerner, W., et al., "The Function of a Hydrogen Peroxide-Detecting Electroenzymatic Glucose Electrode is Markedly Impaired in Human Subcutaneous Tissue and Plasma," *Biosensors & Bioelectronics*, vol. 8, 1993, pp. 473-482.
- Korf, J., et al., "Monitoring of Glucose and Lactate Using Microdialysis: Applications in Neonates and Rat Brain," *Developmental Neuroscience*, vol. 15, 1993, pp. 240-246.
- Koudelka, M., et al., "In-Vivo Behaviour of Hypodermically Implanted Microfabricated Glucose Sensors", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 31-36.
- Kruger, D., et al., "Psychological Motivation and Patient Education: A Role for Continuous Glucose Monitoring", *Diabetes Technology & Therapeutics*, vol. 2, Sup. 1, 2000, pp. S93-S97.
- Kulys, J., et al., "Mediatorless Peroxidase Electrode and Preparation of Bienzyme Sensors", *Bioelectrochemistry and Bioenergetics*, vol. 24, 1990, pp. 305-311.
- Lager, W., et al., "Implantable Electrocatalytic Glucose Sensor", *Hormone Metabolic Research*, vol. 26, 1994, pp. 526-530.
- Laurell, T., "A Continuous Glucose Monitoring System Based on Microdialysis", *Journal of Medical Engineering & Technology*, vol. 16, No. 5, 1992, pp. 187-193.
- Lindner, E., et al., "Flexible (Kapton-Based) Microsensor Arrays of High Stability for Cardiovascular Applications", *Journal of the Chemical Society, Faraday Transactions*, vol. 89, No. 2, 1993, pp. 361-367.
- Lortz, J., et al., "What is Bluetooth? We Explain the Newest Short-Range Connectivity Technology", *Smart Computing Learning Series, Wireless Computing*, vol. 8, Issue 5, 2002, pp. 72-74.
- Maidan, R., et al., "Elimination of Electrooxidizable Interferant-Produced Currents in Amperometric Biosensors", *Analytical Chemistry*, vol. 64, No. 23, 1992, pp. 2889-2896.
- Malin, S. F., et al., "Noninvasive Prediction of Glucose by Near-Infrared Diffuse Reflectance Spectroscopy", *Clinical Chemistry*, vol. 45, No. 9, 1999, pp. 1651-1658.
- Marko-Varga, G., et al., "Enzyme-Based Biosensor as a Selective Detection Unit in Column Liquid Chromatography", *Journal of Chromatography A*, vol. 660, 1994, pp. 153-167.

(56)

References Cited

OTHER PUBLICATIONS

- Mastrototaro, J. J., et al., "An Electroenzymatic Glucose Sensor Fabricated on a Flexible Substrate", *Sensors and Actuators B*, vol. 5, 1991, pp. 139-144.
- Mauras, N., et al., "Lack of Accuracy of Continuous Glucose Sensors in Healthy, Nondiabetic Children: Results of the Diabetes Research in Children Network (DirecNet) Accuracy Study," *Journal of Pediatrics*, 2004, pp. 770-775.
- McGarraugh, G., et al., "Glucose Measurements Using Blood Extracted from the Forearm and the Finger", *TheraSense, Inc.*, 2000, 16 pp. 1-16.
- McGarraugh, G., et al., "Physiological Influences on Off-Finger Glucose Testing", *Diabetes Technology & Therapeutics*, vol. 3, No. 3, 2001, pp. 367-376.
- McKean, B. D., et al., "A Telemetry-Instrumentation System for Chronically Implanted Glucose and Oxygen Sensors", *IEEE Transactions on Biomedical Engineering*, vol. 35, No. 7, 1988, pp. 526-532.
- McNeil, C. J., et al., "Thermostable Reduced Nicotinamide Adenine Dinucleotide Oxidase: Application to Amperometric Enzyme Assay", *Analytical Chemistry*, vol. 61, No. 1, 1989, pp. 25-29.
- Miyawaki, O., et al., "Electrochemical and Glucose Oxidase Coenzyme Activity of Flavin Adenine Dinucleotide Covalently Attached to Glassy Carbon at the Adenine Amino Group", *Biochimica et Biophysica Acta*, vol. 838, 1985, pp. 60-68.
- Moatti-Sirat, D., et al., "Evaluating In Vitro and In Vivo the Interference of Ascorbate and Acetaminophen on Glucose Detection by a Needle-Type Glucose Sensor", *Biosensors & Bioelectronics*, vol. 7, 1992, pp. 345-352.
- Moatti-Sirat, D., et al., "Reduction of Acetaminophen Interference in Glucose Sensors by a Composite Nafion Membrane: Demonstration in Rats and Man", *Diabetologia*, vol. 37, 1994, pp. 610-616.
- Moatti-Sirat, D., et al., "Towards Continuous Glucose Monitoring: In Vivo Evaluation of a Miniaturized Glucose Sensor Implanted for Several Days in Rat Subcutaneous Tissue", *Diabetologia*, vol. 35, 1992, pp. 224-330.
- Nagy, G., et al., "A New Type of Enzyme Electrode: The Ascorbic Acid Eliminator Electrode", *Life Sciences*, vol. 31, No. 23, 1982, pp. 2611-2616.
- Nakamura, S., et al., "Effect of Periodate Oxidation on the Structure and Properties of Glucose Oxidase", *Biochimica et Biophysica Acta*, vol. 445, 1976, pp. 294-308.
- Narasimham, K., et al., "p-Benzoquinone Activation of Metal Oxide Electrodes for Attachment of Enzymes", *Enzyme and Microbial Technology*, vol. 7, 1985, pp. 283-286.
- Ohara, T. J., "Osmium Bipyridyl Redox Polymers Used in Enzyme Electrodes", *Platinum Metals Review*, vol. 39, No. 2, 1995, pp. 54-62.
- Ohara, T. J., et al., "'Wired' Enzyme Electrodes for Amperometric Determination of Glucose or Lactate in the Presence of Interfering Substances", *Analytical Chemistry*, vol. 66, No. 15, 1994, pp. 2451-2457.
- Ohara, T. J., et al., "Glucose Electrodes Based on Cross-Linked [Os(bpy)₂Cl]²⁺ Complexed Poly(1-Vinylimidazole) Films", *Analytical Chemistry*, vol. 65, No. 23, 1993, pp. 3512-3517.
- Olivier, C. N., et al., "In Vivo Measurement of Carbon Dioxide Tension with a Miniature Electrodes", *Pflugers Archiv: European Journal of Physiology*, vol. 373, 1978, pp. 269-272.
- Paddock, R. M., et al., "Electrocatalytic Reduction of Hydrogen Peroxide via Direct Electron Transfer From Pyrolytic Graphite Electrodes to Irreversibly Adsorbed Cytochrome C Peroxidase", *Journal of ElectroAnalytical Chemistry*, vol. 260, 1989, pp. 487-494.
- Palleschi, G., et al., "A Study of Interferences in Glucose Measurements in Blood by Hydrogen Peroxide Based Glucose Probes", *Analytical Biochemistry*, vol. 159, 1986, pp. 114-121.
- Pankratov, I., et al., "Sol-Gel Derived Renewable-Surface Biosensors", *Journal of ElectroAnalytical Chemistry*, vol. 393, 1995, pp. 35-41.
- Pathak, C., et al., "Rapid Photopolymerization of Immunoprotective Gels in Contact with Cells and Tissue", *Journal of the American Chemical Society*, vol. 114, No. 21, 1992, pp. 8311-8312.
- Pickup, J., "Developing Glucose Sensors for In Vivo Use", *Tibtech*, vol. 11, 1993, pp. 285-291.
- Pickup, J., et al., "Implantable Glucose Sensors: Choosing the Appropriate Sensing Strategy", *Biosensors*, vol. 3, 1987/88, pp. 335-346.
- Pickup, J., et al., "In Vivo Molecular Sensing in Diabetes Mellitus: An Implantable Glucose Sensor with Direct Electron Transfer", *Diabetologia*, vol. 32, 1989, pp. 213-217.
- Pickup, J., et al., "Potentially-Implantable, Amperometric Glucose Sensors with Mediated Electron Transfer: Improving the Operating Stability", *Biosensors*, vol. 4, 1989, pp. 109-119.
- Pishko, M. V., et al., "Amperometric Glucose Microelectrodes Prepared Through Immobilization of Glucose Oxidase in Redox Hydrogels", *Analytical Chemistry*, vol. 63, No. 20, 1991, pp. 2268-2272.
- Poitout, V., et al., "A Glucose Monitoring System for on Line Estimation in Man of Blood Glucose Concentration Using a Miniaturized Glucose Sensor Implanted in the Subcutaneous Tissue and a Wearable Control Unit", *Diabetologia*, vol. 36, 1993, pp. 658-663.
- Poitout, V., et al., "Calibration in Dogs of a Subcutaneous Miniaturized Glucose Sensor Using a Glucose Meter for Blood Glucose Determination", *Biosensors & Bioelectronics*, vol. 7, 1992, pp. 587-592.
- Poitout, V., et al., "In Vitro and In Vivo Evaluation in Dogs of a Miniaturized Glucose Sensor", *ASAIO Transactions*, vol. 37, No. 3, 1991, pp. M298-M300.
- Pollak, A., et al., "Enzyme Immobilization by Condensation Copolymerization into Cross-Linked Polyacrylamide Gels", *Journal of the American Chemical Society*, vol. 102, No. 20, 1980, pp. 6324-6336.
- Quinn, C. P., et al., "Kinetics of Glucose Delivery to Subcutaneous Tissue in Rats Measured with 0.3-mm Amperometric Microsensors", *The American Physiological Society*, 1995, E155-E161.
- Reach, G., et al., "Can Continuous Glucose Monitoring Be Used for the Treatment of Diabetes?", *Analytical Chemistry*, vol. 64, No. 6, 1992, pp. 381-386.
- Rebrin, K., et al., "Automated Feedback Control of Subcutaneous Glucose Concentration in Diabetic Dogs", *Diabetologia*, vol. 32, 1989, pp. 573-576.
- Reusch, W., "Other Topics: Organometallic Chemistry: Organometallic Compounds: Main Group Organometallic Compounds," *Virtual Textbook of Organic Chemistry*, 1999, Rev. 2007, 25 pages.
- Roe, J. N., et al., "Bloodless Glucose Measurements", *Critical Review in Therapeutic Drug Carrier Systems*, vol. 15, Issue 3, 1998, pp. 199-241.
- Sacks (ED), "Guidelines and Recommendations for Laboratory Analysis in the Diagnosis and Management of Diabetes Mellitus," *The National Academy of Clinical Biochemistry Presents Laboratory Medicine Practice Guidelines*, vol. 13, 2002, pp. 8-11, 21-23, 52-56, 63.
- Sakakida, M., et al., "Development of Ferrocene-Mediated Needle-Type Glucose Sensor as a Measure of True Subcutaneous Tissue Glucose Concentrations", *Artificial Organs Today*, vol. 2, No. 2, 1992, pp. 145-158.
- Sakakida, M., et al., "Ferrocene-Mediated Needle-Type Glucose Sensor Covered with Newly Designed Biocompatible Membrane", *Sensors and Actuators B*, vol. 13-14, 1993, pp. 319-322.
- Salehi, C., et al., "A Telemetry-Instrumentation System for Long-Term Implantable Glucose and Oxygen Sensors", *Analytical Letters*, vol. 29, No. 13, 1996, pp. 2289-2308.
- Samuels, G. J., et al., "An Electrode-Supported Oxidation Catalyst Based on Ruthenium (IV). pH 'Encapsulation' in a Polymer Film", *Journal of the American Chemical Society*, vol. 103, No. 2, 1981, pp. 307-312.
- Sasso, S. V., et al., "Electropolymerized 1,2-Diaminobenzene as a Means to Prevent Interferences and Fouling and to Stabilize Immobilized Enzyme in Electrochemical Biosensors", *Analytical Chemistry*, vol. 62, No. 11, 1990, pp. 1111-1117.

(56)

References Cited

OTHER PUBLICATIONS

- Scheller, F. W., et al., "Second Generation Biosensors," *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 245-253.
- Scheller, F., et al., "Enzyme Electrodes and Their Application", *Philosophical Transactions of The Royal Society of London B*, vol. 316, 1987, pp. 85-94.
- Schmehl, R. H., et al., "The Effect of Redox Site Concentration on the Rate of Mediated Oxidation of Solution Substrates by a Redox Copolymer Film", *Journal of ElectroAnalytical Chemistry*, vol. 152, 1983, pp. 97-109.
- Schmidt, F. J., et al., "Calibration of a Wearable Glucose Sensor", *The International Journal of Artificial Organs*, vol. 15, No. 1, 1992, pp. 55-61.
- Schmidtke, D. W., et al., "Measurement and Modeling of the Transient Difference Between Blood and Subcutaneous Glucose Concentrations in the Rat After Injection of Insulin", *Proceedings of the National Academy of Sciences*, vol. 95, 1998, pp. 294-299.
- Shaw, G. W., et al., "In Vitro Testing of a Simply Constructed, Highly Stable Glucose Sensor Suitable for Implantation in Diabetic Patients", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 401-406.
- Shichiri, M., et al., "Glycaemic Control in Pancreatectomized Dogs with a Wearable Artificial Endocrine Pancreas", *Diabetologia*, vol. 24, 1983, pp. 179-184.
- Shichiri, M., et al., "In Vivo Characteristics of Needle-Type Glucose Sensor—Measurements of Subcutaneous Glucose Concentrations in Human Volunteers", *Hormone and Metabolic Research Supplement Series*, vol. 20, 1988, pp. 17-20.
- Shichiri, M., et al., "Membrane Design for Extending the Long-Life of an Implantable Glucose Sensor", *Diabetes Nutrition and Metabolism*, vol. 2, 1989, pp. 309-313.
- Shichiri, M., et al., "Needle-type Glucose Sensor for Wearable Artificial Endocrine Pancreas", *Implantable Sensors for Closed-Loop Prosthetic Systems*, Chapter 15, 1985, pp. 197-210.
- Shichiri, M., et al., "Telemetry Glucose Monitoring Device With Needle-Type Glucose Sensor: A Useful Tool for Blood Glucose Monitoring in Diabetic Individuals", *Diabetes Care*, vol. 9, No. 3, 1986, pp. 298-301.
- Shichiri, M., et al., "Wearable Artificial Endocrine Pancreas With Needle-Type Glucose Sensor", *The Lancet*, 1982, pp. 1129-1131.
- Shults, M. C., et al., "A Telemetry-Instrumentation System for Monitoring Multiple Subcutaneously Implanted Glucose Sensors", *IEEE Transactions on Biomedical Engineering*, vol. 41, No. 10, 1994, pp. 937-942.
- Sittampalam, G., et al., "Surface-Modified Electrochemical Detector for Liquid Chromatography", *Analytical Chemistry*, vol. 55, No. 9, 1983, pp. 1608-1610.
- Skoog, D. A., et al., "Evaluation of Analytical Data," *Fundamentals of Analytical Chemistry*, 1966, pp. 55.
- Soegijoko, S., et al., "External Artificial Pancreas: A New Control Unit Using Microprocessor", *Hormone and Metabolic Research Supplement Series*, vol. 12, 1982, pp. 165-169.
- Sprules, S. D., et al., "Evaluation of a New Disposable Screen-Printed Sensor Strip for the Measurement of NADH and Its Modification to Produce a Lactate Biosensor Employing Microliter Volumes", *Electroanalysis*, vol. 8, No. 6, 1996, pp. 539-543.
- Sternberg, F., et al., "Calibration Problems of Subcutaneous Glucosensors when Applied 'In-Situ' in Man", *Hormone and Metabolic Research*, vol. 26, 1994, pp. 523-526.
- Sternberg, R., et al., "Covalent Enzyme Coupling on Cellulose Acetate Membranes for Glucose Sensor Development", *Analytical Chemistry*, vol. 60, No. 24, 1988, pp. 2781-2786.
- Sternberg, R., et al., "Study and Development of Multilayer Needle-Type Enzyme-Based Glucose Microsensors", *Biosensors*, vol. 4, 1988, pp. 27-40.
- Suekane, M., "Immobilization of Glucose Isomerase", *Zeitschrift für Allgemeine Mikrobiologie*, vol. 22, No. 8, 1982, pp. 565-576.
- Tajima, S., et al., "Simultaneous Determination of Glucose and 1,5-Anhydroglucitol", *Chemical Abstracts*, vol. 111, No. 25, 1989, pp. 394.
- Takamura, A., et al., Drug release from Poly(vinyl alcohol) Gel Prepared by Freeze-Thaw Procedure, *Journal of Controlled Release*, vol. 20, 1992, pp. 21-27.
- Tarasevich, M. R., "Bioelectrocatalysis", *Comprehensive Treatise of Electrochemistry*, vol. 10, 1985, pp. 231-295.
- Tatsuma, T., et al., "Enzyme Monolayer- and Bilayer-Modified Tin Oxide Electrodes for the Determination of Hydrogen Peroxide and Glucose", *Analytical Chemistry*, vol. 61, No. 21, 1989, pp. 2352-2355.
- Taylor, C., et al., "'Wiring' of Glucose Oxidase Within a Hydrogel Made with Polyvinyl Imidazole Complexed with [(Os-4,4'-dimethoxy-2,2'-bipyridine)Cl]^{+/2+}", *Journal of ElectroAnalytical Chemistry*, vol. 396, 1995, pp. 511-515.
- Thompson, M., et al., "In Vivo Probes: Problems and Perspectives", *Clinical Biochemistry*, vol. 19, 1986, pp. 255-261.
- Trojanowicz, M., et al., "Enzyme Entrapped Polypyrrole Modified Electrode for Flow-Injection Determination of Glucose", *Biosensors & Bioelectronics*, vol. 5, 1990, pp. 149-156.
- Tsalikian, E., et al., "Accuracy of the GlucoWatch G2® Biographer and the Continuous Glucose Monitoring System During Hypoglycemia: Experience of the Diabetes Research in Children Network", *Diabetes Care*, vol. 27, No. 3, 2004, pp. 722-726.
- Turner, A., et al., "Diabetes Mellitus: Biosensors for Research and Management", *Biosensors*, vol. 1, 1985, pp. 85-115.
- Turner, R. F., et al., "A Biocompatible Enzyme Electrode for Continuous in vivo Glucose Monitoring in Whole Blood", *Sensors and Actuators B*, vol. 1, 1990, pp. 561-564.
- Tuzhi, P., et al., "Constant Potential Pretreatment of Carbon Fiber Electrodes for In Vivo Electrochemistry", *Analytical Letters*, vol. 24, No. 6, 1991, pp. 935-945.
- Umana, M., "Protein-Modified Electrochemically Active Biomaterial Surface", *U.S. Army Research Office, Analytical and Chemical Sciences Research Triangle Institute*, 1988, pp. 1-9.
- Updike, S. J., et al., "Principles of Long-Term Fully Implanted Sensors with Emphasis on Radiotelemetric Monitoring of Blood Glucose from Inside a Subcutaneous Foreign Body Capsule (FBC)", *Biosensors in the Body: Continuous in vivo Monitoring*, Chapter 4, 1997, pp. 117-137.
- Urban, G., et al., "Miniaturized Thin-Film Biosensors Using Covalently Immobilized Glucose Oxidase", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 555-562.
- Velho, G., et al., "In Vitro and In Vivo Stability of Electrode Potentials in Needle-Type Glucose Sensors", *Diabetes*, vol. 38, No. 2, 1989, pp. 164-171.
- Velho, G., et al., "Strategies for Calibrating a Subcutaneous Glucose Sensor", *Biomedica Biochimica Acta*, vol. 48, 1989, pp. 957-964.
- Von Woedtke, T., et al., "In Situ Calibration of Implanted Electrochemical Glucose Sensors", *Biomedica Biochimica Acta*, vol. 48, 1989, pp. 943-952.
- Vreeke, M. S., et al., "Hydrogen Peroxide Electrodes Based on Electrical Connection of Redox Centers of Various Peroxidases to Electrodes through a Three-Dimensional Electron-Relaying Polymer Network", *Diagnostic Biosensors Polymers*, Chapter 15, 1993, pp. 180-193.
- Vreeke, M., et al., "Hydrogen Peroxide and β -Nicotinamide Adenine Dinucleotide Sensing Amperometric Electrodes Based on Electrical Connection of Horseradish Peroxidase Redox Centers to Electrodes through a Three-Dimensional Electron Relaying Polymer Network", *Analytical Chemistry*, vol. 64, No. 24, 1992, pp. 3084-3090.
- Wagner, J. G., et al., "Continuous Amperometric Monitoring of Glucose in a Brittle Diabetic Chimpanzee with a Miniature Subcutaneous Electrode", *Proceedings of the National Academy of Sciences USA*, 1998, pp. 6379-6382.
- Wang, D. L., et al., "Miniaturized Flexible Amperometric Lactate Probe", *Analytical Chemistry*, vol. 65, No. 8, 1993, pp. 1069-1073.
- Wang, J., et al., "Activation of Glassy Carbon Electrodes by Alternating Current Electrochemical Treatment", *Analytica Chimica Acta*, vol. 167, 1985, pp. 325-334.
- Wang, J., et al., "Amperometric Biosensing of Organic Peroxides with Peroxidase-Modified Electrodes", *Analytica Chimica Acta*, vol. 254, 1991, pp. 81-88.


(56)

References Cited

OTHER PUBLICATIONS

- Wang, J., et al., "Highly Selective Membrane-Free, Mediator-Free Glucose Biosensor", *Analytical Chemistry*, vol. 66, No. 21, 1994, pp. 3600-3606.
- Wang, J., et al., "Screen-Printable Sol-Gel Enzyme-Containing Carbon Inks", *Analytical Chemistry*, vol. 68, No. 15, 1996, pp. 2705-2708.
- Wang, J., et al., "Sol-Gel-Derived Metal-Dispersed Carbon Composite Amperometric Biosensors", *Electroanalysis*, vol. 9, No. 1, 1997, pp. 52-55.
- Williams, D. L., et al., "Electrochemical-Enzymatic Analysis of Blood Glucose and Lactate", *Analytical Chemistry*, vol. 42, No. 1, 1970, pp. 118-121.
- Wilson, G. S., et al., "Progress Toward the Development of an Implantable Sensor for Glucose", *Clinical Chemistry*, vol. 38, No. 9, 1992, pp. 1613-1617.
- Wood, W. D., et al., "Hermetic Sealing with Epoxy", *Mechanical Engineering*, 1990, pp. 46-48.
- Yabuki, S., et al., "Electro-Conductive Enzyme Membrane", *Journal of the Chemical Society, Chemical Communications*, 1989, pp. 945-946.
- Yang, C., et al., "A Comparison of Physical Properties and Fuel Cell Performance of Nation and Zirconium Phosphate/Nafion Composite Membranes," *Journal of Membrane Science*, vol. 237, 2004, pp. 145-161.
- Yang, L., et al., "Determination of Oxidase Enzyme Substrates Using Cross-Flow Thin-Layer Amperometry", *Electroanalysis*, vol. 8, No. 8-9, 1996, pp. 716-721.
- Yao, T., "A Chemically-Modified Enzyme Membrane Electrode as an Amperometric Glucose Sensor", *Analytica Chimica Acta*, vol. 148, 1983, pp. 27-33.
- Ye, L., et al., "High Current Density 'Wired' Quinoprotein Glucose Dehydrogenase Electrode", *Analytical Chemistry*, vol. 65, No. 3, 1993, pp. 238-241.
- Yildiz, A., et al., "Evaluation of an Improved Thin-Layer Electrode", *Analytical Chemistry*, vol. 40, No. 7, 1968, pp. 1018-1024.
- Zamzow, K., et al., "New Wearable Continuous Blood Glucose Monitor (BGM) and Artificial Pancreas (AP)", *Diabetes*, vol. 39, 1990, pp. 5A-20A.
- Zhang, Y., et al., "Application of Cell Culture Toxicity Tests to the Development of Implantable Biosensors", *Biosensors & Bioelectronics*, vol. 6, 1991, pp. 653-661.
- Zhang, Y., et al., "Elimination of the Acetaminophen Interference in an Implantable Glucose Sensor", *Analytical Chemistry*, vol. 66, No. 7, 1994, pp. 1183-1188.
- European Patent Application No. 03808614.6, Decision to Refuse the Application dated Apr. 8, 2014.
- European Patent Application No. 03808614.6, Examination Report dated Dec. 30, 2011.
- European Patent Application No. 03808614.6, Summons to Attend Oral Proceedings dated Nov. 12, 2013.
- European Patent Application No. 03808614.6, Supplementary European Search Report with International Filing Date of Dec. 26, 2003.
- PCT Application No. PCT/US2003/041640, International Preliminary Examination Report dated Jul. 11, 2005.
- PCT Application No. PCT/US2003/041640, International Search Report dated Dec. 28, 2004.
- U.S. Appl. No. 10/745,878, Notice of Allowance dated Jul. 26, 2010.
- U.S. Appl. No. 10/745,878, Office Action dated Feb. 10, 2006.
- U.S. Appl. No. 10/745,878, Office Action dated Feb. 24, 2005.
- U.S. Appl. No. 10/745,878, Office Action dated Feb. 5, 2010.
- U.S. Appl. No. 10/745,878, Office Action dated May 30, 2008.
- U.S. Appl. No. 10/745,878, Office Action dated Sep. 15, 2009.
- U.S. Appl. No. 10/745,878, Office Action dated Sep. 21, 2007.
- U.S. Appl. No. 12/902,138, Notice of Allowance, dated Feb. 23, 2012.
- U.S. Appl. No. 12/902,138, Office Action dated Jan. 27, 2012.
- U.S. Appl. No. 12/902,138, Office Action dated Jun. 7, 2011.
- U.S. Appl. No. 13/481,256, Notice of Allowance dated Oct. 28, 2013.
- U.S. Appl. No. 13/481,256, Office Action dated Aug. 22, 2012.
- U.S. Appl. No. 13/481,256, Office Action dated Jul. 30, 2013.
- U.S. Patent Reexamination Application No. 90/007,903, Request for Reexamination of U.S. Pat. No. 6,565,509 filed Jan. 25, 2006.
- U.S. Patent Reexamination Application No. 90/007,910, Request for Reexamination of U.S. Pat. No. 6,175,752 filed Feb. 1, 2006.
- U.S. Patent Reexamination Application No. 90/007,913, Request for Reexamination of U.S. Pat. No. 6,284,478 filed Feb. 1, 2006.
- U.S. Patent Reexamination Application No. 90/007,914, Request for Reexamination of U.S. Pat. No. 6,329,161 filed Feb. 1, 2006.
- U.S. Patent Reexamination Application No. 90/008,172, Request for Reexamination of U.S. Pat. No. 6,990,366 filed Aug. 16, 2006.
- U.S. Patent Reexamination Application No. 90/008,173, Request for Reexamination of U.S. Pat. No. 6,134,461 filed Aug. 16, 2006.
- U.S. Patent Reexamination Application No. 90/008,457, Request for Reexamination of U.S. Pat. No. 6,990,366 filed Jan. 23, 2007.
- U.S. Patent Reexamination Application No. 90/008,665, Request for Reexamination of U.S. Pat. No. 6,284,478 filed May 25, 2007.
- U.S. Patent Reexamination Application No. 90/008,713, Request for Reexamination of U.S. Pat. No. 6,329,161 filed Jul. 25, 2007.
- Lo, B., et al., "Key Technical Challenges and Current Implementations of Body Sensor Networks", *Body Sensor Networks*, 2005, pp. 1-5.
- Rodriguez, N., et al., "Flexible Communication and Control Protocol for Injectable Neuromuscular Interfaces", *IEEE Transactions on Biomedical Circuits and Systems*, vol. 1, No. 1, 2007, pp. 19-27.
- Canadian Patent Application No. 2,556,331, Examiners Report dated Jan. 6, 2012.
- European Patent Application No. 05723142.5, Official Letter mailed Aug. 6, 2010.
- European Patent Application No. 05723142.5, Official Letter mailed Jan. 22, 2013.
- European Patent Application No. 05723142.5, Official Letter mailed Sep. 4, 2009.
- European Patent Application No. 05723142.5, Supplementary European Search Report dated May 6, 2008.
- PCT Application No. PCT/US2005/004892, International Search Report and Written Opinion of the International Searching Authority dated Dec. 11, 2006.
- PCT Application No. PCT/US2005/004892, Preliminary Report on Patentability and Written Opinion of the International Searching Authority dated Dec. 28, 2006.
- U.S. Appl. No. 11/060,365, Advisory Action dated Dec. 5, 2011.
- U.S. Appl. No. 11/060,365, Advisory Action dated Sep. 3, 2009.
- U.S. Appl. No. 11/060,365, Notice of Allowance dated Dec. 26, 2013.
- U.S. Appl. No. 11/060,365, Office Action dated Dec. 27, 2010.
- U.S. Appl. No. 11/060,365, Office Action dated Jul. 23, 2009.
- U.S. Appl. No. 11/060,365, Office Action dated Nov. 13, 2008.
- U.S. Appl. No. 11/060,365, Office Action dated Sep. 13, 2011.
- U.S. Appl. No. 11/060,365, Office Action dated Sep. 29, 2009.
- U.S. Appl. No. 14/325,253, Office Action dated May 1, 2017.
- U.S. Appl. No. 14/325,253, Office Action dated Oct. 6, 2016.
- U.S. Appl. No. 14/325,253, Office Action dated Aug. 30, 2017.

* cited by examiner

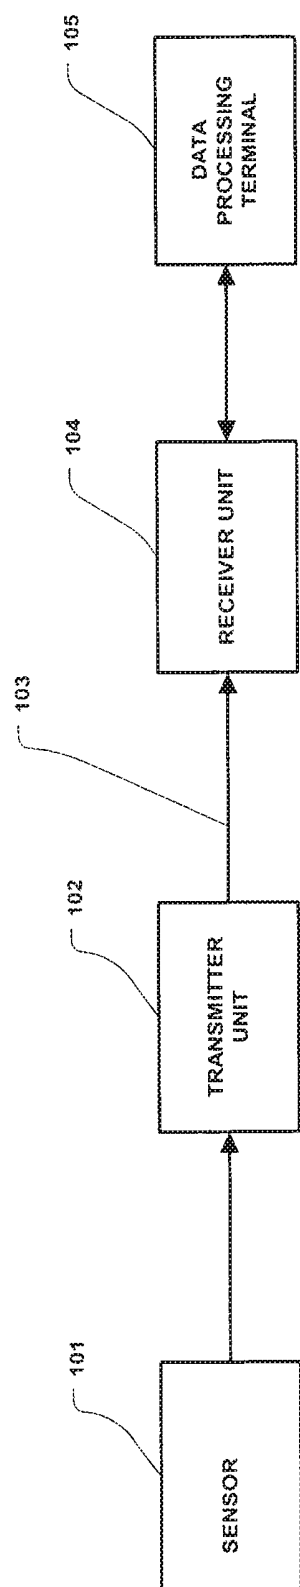

100

FIGURE 1

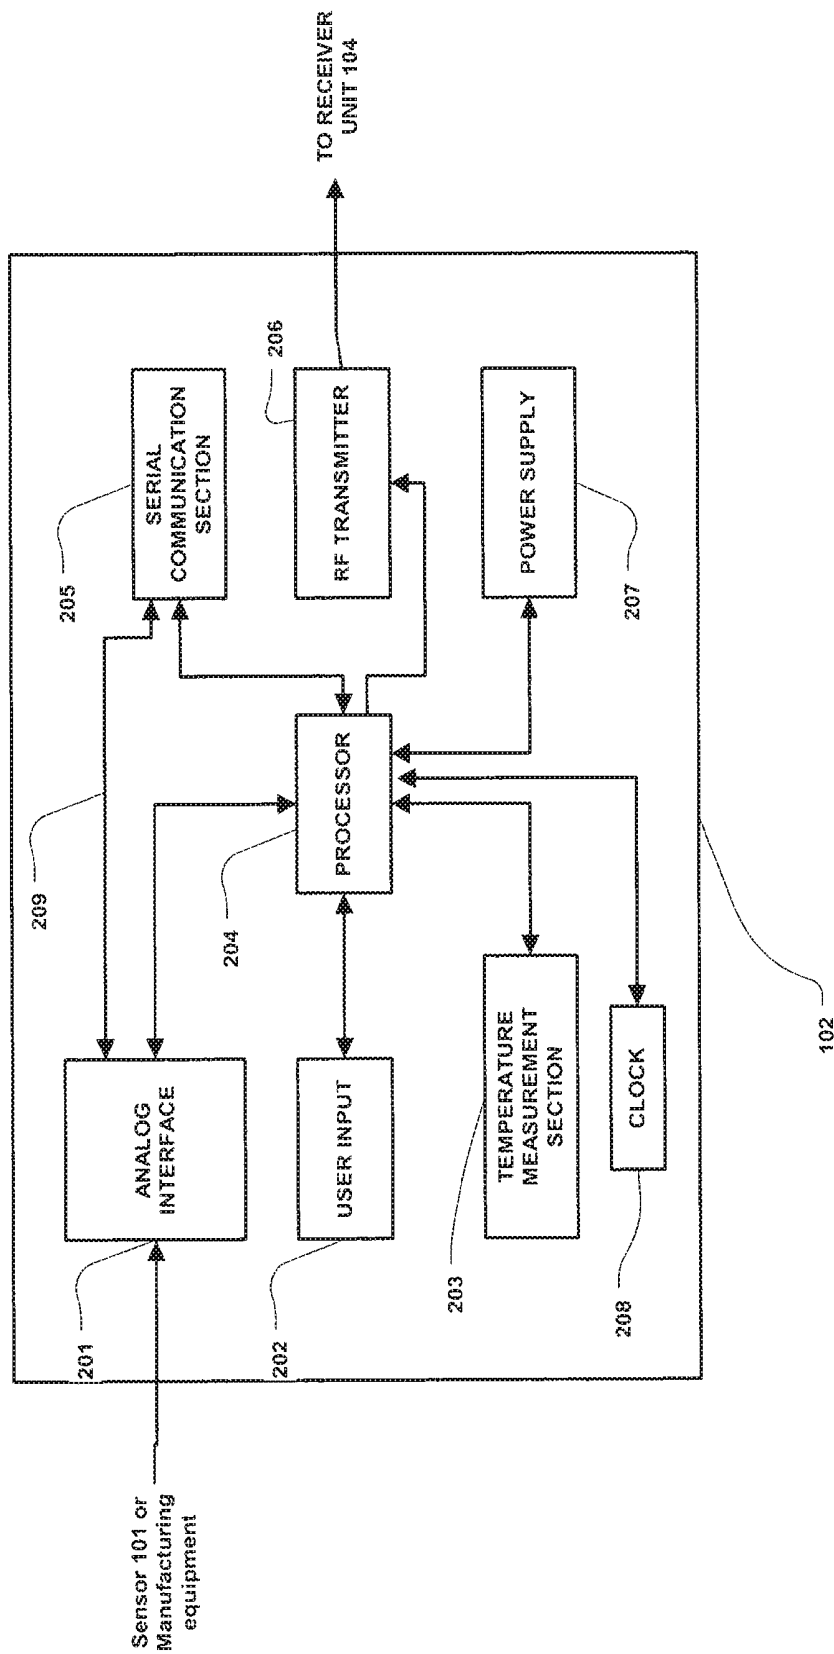


FIGURE 2

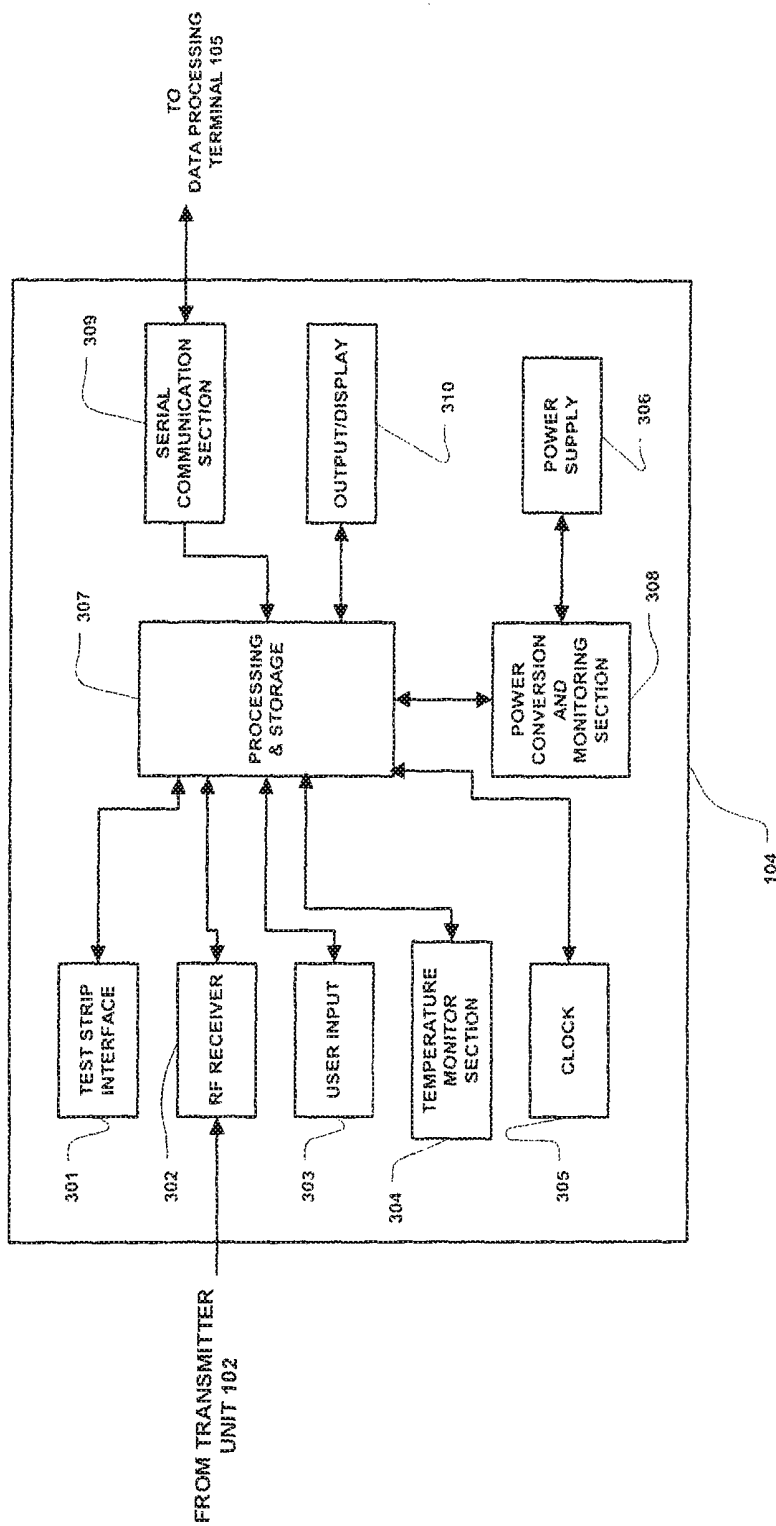


FIGURE 3

Byte		High Nibble	Low Nibble
0	TX ID (lsbyte)		
1	Tx Time		
2	Tx Status	Tx Status n1	Tx Status n0
3		Sensor n0	Tx Status n2
4		Sensor n2	Sensor n1
5		Tx Status-1 n1	Tx Status-1 n0
6		Sensor-1 n0	Tx Status-1 n2
7		Sensor-1 n2	Sensor-1 n1
8		Tx Status-2 n1	Tx Status-2 n0
9		Sensor-2 n0	Tx Status-2 n2
10		Sensor-2 n2	Sensor-2 n1
11		CV-1, Tx Status-1	CV, Tx Status
12		Tx Pending, Tx Batt	CV-2, Tx Status-2

FIGURE 4

1	Packed Data	13 bytes
2	Tx ID, middle sb	1 byte
3	Tx ID, msb	1 byte
4	Zero Pad	232 bytes
5	Parity Symbols	8 bytes
	Total	255 bytes

FIGURE 5A

1	Packed data	13 bytes
2	Parity Symbols	8 bytes
	Total	21 bytes

FIGURE 5B

1		0x00 0x00 0x12 0x34	4 bytes
1	Depadded Data Block Contents		21 bytes

FIGURE 5C

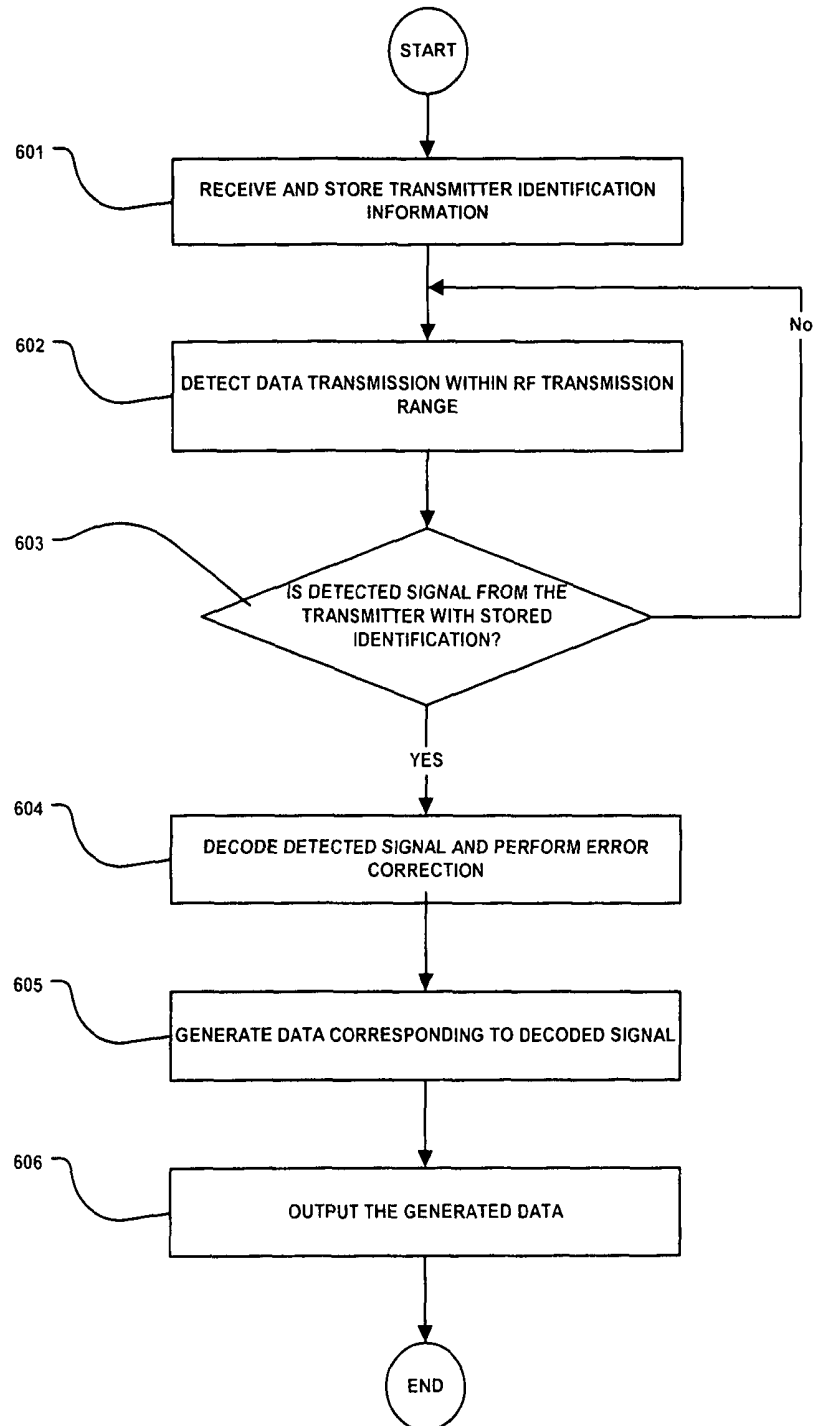


FIGURE 6

CONTINUOUS GLUCOSE MONITORING SYSTEM AND METHODS OF USE

RELATED APPLICATIONS

The present application is a continuation of U.S. patent application Ser. No. 13/481,256 filed May 25, 2012, now U.S. Pat. No. 8,622,903, which is a continuation of U.S. patent application Ser. No. 12/902,138 filed Oct. 11, 2010, now U.S. Pat. No. 8,187,183, which is a continuation of U.S. patent application Ser. No. 10/745,878 filed Dec. 26, 2003, now U.S. Pat. No. 7,811,231, which claims the benefit of U.S. Provisional Application No. 60/437,374 filed Dec. 31, 2002, entitled "Continuous Glucose Monitoring System and Methods of Use", the disclosures of each of which are incorporated herein by reference for all purposes.

BACKGROUND

The present invention relates to continuous glucose monitoring systems. More specifically, the present invention relates to an in-vivo continuous glucose monitoring system which detects glucose levels continuously and transfers the detected glucose level information at predetermined time intervals to data processing devices for monitoring, diagnosis and analysis.

SUMMARY

A continuous glucose monitoring system in accordance with one embodiment of the present invention includes a sensor configured to detect one or more glucose levels, a transmitter operatively coupled to the sensor, the transmitter configured to receive the detected one or more glucose levels, the transmitter further configured to transmit signals corresponding to the detected one or more glucose levels, a receiver operatively coupled to the transmitter configured to receive transmitted signals corresponding to the detected one or more glucose levels, where the transmitter is configured to transmit a current data point and at least one previous data point, the current data point and the at least one previous data point corresponding to the detected one or more glucose levels.

The receiver may be operatively coupled to the transmitter via an RF communication link, and further, configured to decode the encoded signals received from the transmitter.

In one embodiment, the transmitter may be configured to periodically transmit a detected and processed glucose level from the sensor to the receiver via the RF data communication link. In one embodiment, the transmitter may be configured to sample four times every second to obtain 240 data points for each minute, and to transmit at a rate of one data point (e.g., an average value of the 240 sampled data points for the minute) per minute to the receiver.

The transmitter may be alternately configured to transmit three data points per minute to the receiver, the first data point representing the current sampled data, and the remaining two transmitted data points representing the immediately past two data points previously sent to the receiver. In this manner, in the case where the receiver does not successfully receive the sampled data from the transmitter, at the subsequent data transmission, the immediately prior transmitted data is received by the receiver. Thus, even with a faulty connection between the transmitter and the receiver, or a failed RF data link, the present approach ensures that missed

data points may be ascertained from the subsequent data point transmissions without retransmission of the missed data points to the receiver.

The transmitter may be configured to encode the detected one or more glucose levels received from the sensor to generate encoded signals, and to transmit the encoded signals to the receiver. In one embodiment, the transmitter may be configured to transmit the encoded signals to the receiver at a transmission rate of one data point per minute. Further, the transmitter may be configured to transmit the current data point and the at least one previous data points in a single transmission per minute to the receiver. In one aspect, the current data point may correspond to a current glucose level, and where the at least one previous data point may include at least two previous data points corresponding respectively to at least two consecutive glucose levels, the one of the at least two consecutive glucose levels immediately preceding the current glucose level.

In a further embodiment, the receiver may include an output unit for outputting the received transmitted signals corresponding to one or more glucose levels. The output unit may include a display unit for displaying data corresponding to the one or more glucose levels, where the display unit may include one of a LCD display, a cathode ray tube display, and a plasma display.

The displayed data may include one or more of an alphanumeric representation corresponding to the one or more glucose levels, a graphical representation of the one or more glucose levels, and a three-dimensional representation of the one or more glucose levels. Moreover, the display unit may be configured to display the data corresponding to the one or more glucose levels substantially in real time.

Further, the output unit may include a speaker for outputting an audio signal corresponding to the one or more glucose levels.

In yet a further embodiment, the receiver may be configured to store an identification information corresponding to the transmitter.

The receiver may be further configured to perform a time hopping procedure for synchronizing with the transmitter. Alternatively, the receiver may be configured to synchronize with the transmitter based on the signal strength detected from the transmitter, where the detected signal strength exceeds a preset threshold level.

The transmitter in one embodiment may be encased in a substantially water-tight housing to ensure continuous operation even in the situation where the transmitter is in contact with water.

Furthermore, the transmitter may be configured with a disable switch which allows the user to temporarily disable the transmission of data to the receiver when the user is required to disable electronic devices, for example, when aboard an airplane. In another embodiment, the transmitter may be configured to operate in an additional third state (such as under Class B radiated emissions standard) in addition to the operational state and the disable state discussed above, so as to allow limited operation while aboard an airplane yet still complying with the Federal Aviation Administration (FAA) regulations. Additionally, the disable switch may also be configured to switch the transmitter between various operating modes such as fully functional transmission mode, post-manufacture sleep mode, and so on. In this manner, the power supply for the transmitter is optimized for prolonged usage by effectively managing the power usage.

Furthermore, the transmitter may be configured to transmit the data to the receiver in predetermined data packets,

encoded, in one embodiment, using Reed Solomon encoding, and transmitted via the RF communication link. Additionally, in a further aspect of the present invention, the RF communication link between the transmitter and the receiver of the continuous glucose monitoring system may be implemented using a low cost, off the shelf remote keyless entry (RKE) chip set.

The receiver in an additional embodiment may be configured to perform, among others, data decoding, error detection and correction (using, for example, forward error correction) on the encoded data packets received from the transmitter to minimize transmission errors such as transmitter stabilization errors and preamble bit errors resulting from noise. The receiver is further configured to perform a synchronized time hopping procedure with the transmitter to identify and synchronize with the corresponding transmitter for data transmission.

Additionally, the receiver may include a graphical user interface (GUI) for displaying the data received from the transmitter for the user. The GUI may include a liquid crystal display (LCD) with backlighting feature to enable visual display in dark surroundings. The receiver may also include an output unit for generating and outputting audible signal alerts for the user, or placing the receiver in a vibration mode for alerting the user by vibrating the receiver.

More specifically, in a further aspect, the receiver may be configured to, among others, display the received glucose levels on a display section of the receiver either real time or in response to user request, and provide visual (and/or auditory) notification to the user of the detected glucose levels being monitored. To this end, the receiver is configured to identify the corresponding transmitter from which it is to receive data via the RF data link, by initially storing the identification information of the transmitter, and performing a time hopping procedure to isolate the data transmission from the transmitter corresponding to the stored identification information and thus to synchronize with the transmitter. Alternatively, the receiver may be configured to identify the corresponding transmitter based on the signal strength detected from the transmitter, determined to exceed a preset threshold level.

A method in accordance with one embodiment of the present invention includes the steps of receiving an identification information corresponding to a transmitter, detecting data within a predetermined RF transmission range, determining whether the detected data is transmitted from the transmitter, decoding the detected data, and generating an output signal corresponding to the decoded data.

In one embodiment, the step of determining whether the detected data transmission is transmitted from the transmitter may be based on the received identification information. In another embodiment, the step of determining whether the detected data transmission is transmitted from the transmitter may be based on the signal strength and duration of the detected data within the predetermined RF transmission range.

In a further embodiment, the step of decoding may also include the step of performing error correction on the decoded data. Moreover, the step of decoding may include the step of performing Reed-Solomon decoding on the detected data.

In the manner described, the present invention provides a continuous glucose monitoring system that is simple to use and substantially compact so as to minimize any interference with the user's daily activities. Furthermore, the continuous glucose monitoring system may be configured to be substantially water-resistant so that the user may freely bathe,

swim, or enjoy other water related activities while using the monitoring system. Moreover, the components comprising the monitoring system including the transmitter and the receiver are configured to operate in various modes to enable power savings, and thus enhancing post-manufacture shelf life.

INCORPORATION BY REFERENCE

Applicants herein incorporate by reference application Ser. No. 09/753,746 filed on Jan. 2, 2001, and issued on May 6, 2003 as U.S. Pat. No. 6,560,471, entitled "Analyte Monitoring Device and Methods of Use" assigned to the Assignee of the present application for all purposes.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a continuous glucose monitoring system in accordance with one embodiment of the present invention;

FIG. 2 is a block diagram of the transmitter of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIG. 3 is a block diagram of the receiver of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIG. 4 illustrates a data packet of the transmitter of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention;

FIGS. 5A, 5B and 5C illustrate a data packet table for Reed-Solomon encoding in the transmitter, a depadded data table, and a link prefix table, respectively, in accordance with one embodiment of the continuous glucose monitoring system of FIG. 1; and

FIG. 6 is a flowchart illustrating the time hopping procedure for the receiver of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention.

DETAILED DESCRIPTION

FIG. 1 illustrates a continuous glucose monitoring system 100 in accordance with one embodiment of the present invention. In such embodiment, the continuous glucose monitoring system 100 includes a sensor 101, a transmitter 102 coupled to the sensor 101, and a receiver 104 which is configured to communicate with the transmitter 102 via a communication link 103. The receiver 104 may be further configured to transmit data to a data processing terminal 105 for evaluating the data received by the receiver 104. Only one sensor 101, transmitter 102, communication link 103, receiver 104, and data processing terminal 105 are shown in the embodiment of the continuous glucose monitoring system 100 illustrated in FIG. 1. However, it will be appreciated by one of ordinary skill in the art that the continuous glucose monitoring system 100 may include one or more sensor 101, transmitter 102, communication link 103, receiver 104, and data processing terminal 105, where each receiver 104 is uniquely synchronized with a respective transmitter 102.

In one embodiment of the present invention, the sensor 101 is physically positioned on the body of a user whose glucose is being monitored. The term user as used herein is intended to include humans, animals, as well as any other who might benefit from the use of the glucose monitoring system 100. The sensor 101 is configured to continuously sample the glucose level of the user and convert the sampled glucose level into a corresponding data signal for transmis-

sion by the transmitter **102**. In one embodiment, the transmitter **102** is mounted on the sensor **101** so that both devices are positioned on the user's body. The transmitter **102** performs data processing such as filtering and encoding on data signals, each of which corresponds to a sampled glucose level of the user, for transmission to the receiver **104** via the communication link **103**.

In one embodiment, the continuous glucose monitoring system **100** is configured as a one-way RF communication path from the transmitter **102** to the receiver **104**. In such embodiment, the transmitter **102** transmits the sampled data signals received from the sensor **101** without acknowledgement from the receiver **104** that the transmitted sampled data signals have been received. For example, the transmitter **102** may be configured to transmit the encoded sampled data signals at a fixed rate (e.g., at one minute intervals) after the completion of the initial power on procedure. Likewise, the receiver **104** may be configured to detect such transmitted encoded sampled data signals at predetermined time intervals.

As discussed in further detail below, in one embodiment of the present invention the receiver **104** includes two sections. The first section is an analog interface section that is configured to communicate with the transmitter **102** via the communication link **103**. In one embodiment, the analog interface section may include an RF receiver and an antenna for receiving and amplifying the data signals from the transmitter **102**, which are thereafter, demodulated with a local oscillator and filtered through a band-pass filter. The second section of the receiver **104** is a data processing section which is configured to process the data signals received from the transmitter **102** such as by performing data decoding, error detection and correction, data clock generation, and data bit recovery.

In operation, upon completing the power-on procedure, the receiver **104** is configured to detect the presence of the transmitter **102** within its range based on the strength of the detected data signals received from the transmitter **102**. For example, in one embodiment, the receiver **104** is configured to detect signals whose strength exceeds a predetermined level to identify the transmitter **102** from which the receiver **104** is to receive data. Alternatively, the receiver **104** in a further embodiment may be configured to respond to signal transmission for a predetermined transmitter identification information of a particular transmitter **102** such that, rather than detecting the signal strength of a transmitter **102** to identify the transmitter, the receiver **104** may be configured to detect transmitted signal of a predetermined transmitter **102** based on the transmitted transmitter identification information corresponding to the pre-assigned transmitter identification information for the particular receiver **104**.

In one embodiment, the identification information of the transmitters **102** includes a 16-bit ID number. In an alternate embodiment, the ID number may be a predetermined length including a 24-bit ID number or a 32-bit ID number. Further, any other length ID number may also be used. Thus, in the presence of multiple transmitters **102**, the receiver **104** will only recognize the transmitter **102** which corresponds to the stored identification information. Data signals transmitted from the other transmitters within the range of the receiver **104** are considered invalid signals.

Referring again to FIG. 1, where the receiver **104** determines the corresponding transmitter **102** based on the signal strength of the transmitter **102**, when the receiver **104** is initially powered-on, the receiver **104** is configured to continuously sample the signal strength of the data signals received from the transmitters within its range. If the signal

strength of the data signals meets or exceeds the signal strength threshold level and the transmission duration threshold level, the receiver **104** returns a positive indication for the transmitter **102** transmitting the data signals. That is, in one embodiment, the receiver **104** is configured to positively identify the transmitter **102** after one data signal transmission. Thereafter, the receiver **104** is configured to detect positive indications for three consecutive data signal transmissions for a predetermined time period. At such point, after three consecutive transmissions, the transmitter **102** is fully synchronized with the receiver **104**.

Upon identifying the appropriate transmitter **102**, the receiver **104** begins a decoding procedure to decode the received data signals. In one embodiment, a sampling clock signal may be obtained from the preamble portion of the received data signals. The decoded data signals, which include fixed length data fields, are then sampled with the sampling clock signal. In one embodiment of the present invention, based on the received data signals and the time interval between each of the three data signal transmissions, the receiver **104** determines the wait time period for receiving the next transmission from the identified and synchronized transmitter **102**. Upon successful synchronization, the receiver **104** begins receiving from the transmitter **102** data signals corresponding to the user's detected glucose level. As described in further detail below, the receiver **104** in one embodiment is configured to perform synchronized time hopping with the corresponding synchronized transmitter **102** via the communication link **103** to obtain the user's detected glucose level.

Referring yet again to FIG. 1, the data processing terminal **105** may include a personal computer, a portable computer such as a laptop or a handheld device (e.g., personal digital assistants (PDAs)), and the like, each of which is configured for data communication with the receiver via a wired or a wireless connection. Additionally, the data processing terminal **105** may further be connected to a data network (not shown) for storing, retrieving and updating data corresponding to the detected glucose level of the user.

FIG. 2 is a block diagram of the transmitter **102** of the continuous glucose monitoring system **100** in accordance with one embodiment of the present invention. The transmitter **102** includes an analog interface **201** configured to communicate with the sensor **101** (FIG. 1), a user input **202**, and a temperature detection section **203**, each of which is operatively coupled to a transmitter processor **204** such as a central processing unit (CPU). Further shown in FIG. 2 are a transmitter serial communication section **205** and an RF transmitter **206**, each of which is also operatively coupled to the transmitter processor **204**. Moreover, a power supply **207** is also provided in the transmitter **102** to provide the necessary power for the transmitter **102**. Additionally, as can be seen from the Figure, clock **208** is provided to, among others, supply real time information to the transmitter processor **204**.

In one embodiment, a unidirectional input path is established from the sensor **101** (FIG. 1) and/or manufacturing and testing equipment to the analog interface **201**, while a unidirectional output is established from the output of the RF transmitter **206**. In this manner, a data path is shown in FIG. 2 between the aforementioned unidirectional input and output via a dedicated link **209** from the analog interface **201** to serial communication section **205**, thereafter to the processor **204**, and then to the RF transmitter **206**. As such, in one embodiment, through the data path described above, the transmitter **102** is configured to transmit to the receiver **104** (FIG. 1), via the communication link **103** (FIG. 1), pro-

cessed and encoded data signals received from the sensor **101** (FIG. 1). Additionally, the unidirectional communication data path between the analog interface **201** and the RF transmitter **206** discussed above allows for the configuration of the transmitter **102** for operation upon completion of the manufacturing process as well as for direct communication for diagnostic and testing purposes.

Referring back to FIG. 2, the user input **202** includes a disable device that allows the operation of the transmitter **102** to be temporarily disabled, such as, by the user wearing the transmitter **102**. In an alternate embodiment, the disable device of the user input **202** may be configured to initiate the power-up procedure of the transmitter **102**.

As discussed above, the transmitter processor **204** is configured to transmit control signals to the various sections of the transmitter **102** during the operation of the transmitter **102**. In one embodiment, the transmitter processor **204** also includes a memory (not shown) for storing data such as the identification information for the transmitter **102**, as well as the data signals received from the sensor **101**. The stored information may be retrieved and processed for transmission to the receiver **104** under the control of the transmitter processor **204**. Furthermore, the power supply **207** may include a commercially available battery pack.

The physical configuration of the transmitter **102** is designed to be substantially water resistant, so that it may be immersed in non-saline water for a brief period of time without degradation in performance. Furthermore, in one embodiment, the transmitter **102** is designed so that it is substantially compact and light-weight, not weighing more than a predetermined weight such as, for example, approximately 18 grams. Furthermore, the dimensions of the transmitter **102** in one embodiment includes 52 mm in length, 30 mm in width and 12 mm in thickness. Such small size and weight enable the user to easily carry the transmitter **102**.

The transmitter **102** is also configured such that the power supply section **207** is capable of providing power to the transmitter for a minimum of three months of continuous operation after having been stored for 18 months in a low-power (non-operating) mode. In one embodiment, this may be achieved by the transmitter processor **204** operating in low power modes in the non-operating state, for example, drawing no more than approximately 1 μ A. Indeed, in one embodiment, the final step during the manufacturing process of the transmitter **102** places the transmitter **102** in the lower power, non-operating state (i.e., post-manufacture sleep mode). In this manner, the shelf life of the transmitter **102** may be significantly improved.

Referring again to FIG. 2, the analog interface **201** of the transmitter **102** in one embodiment includes a sensor interface (not shown) configured to physically couple to the various sensor electrodes (such as, for example, working electrode, reference electrode, counter electrode, (not shown)) of the sensor **101** (FIG. 1) of the monitoring system **100**. The analog interface section **201** further includes a potentiostat circuit (not shown) which is configured to generate the Poise voltage determined from the current signals received from the sensor electrodes. In particular, the Poise voltage is determined by setting the voltage difference between the working electrode and the reference electrode (i.e., the offset voltage between the working electrode and the reference electrode of the sensor **101**). Further, the potentiostat circuit also includes a transimpedance amplifier for converting the current signal on the working electrode into a corresponding voltage signal proportional to the current. The signal from the potentiostat circuit is then low pass filtered with a predetermined cut-off frequency to

provide anti-aliasing, and thereafter, passed through a gain stage to provide sufficient gain to allow accurate signal resolution detected from the sensor **101** for analog-to-digital conversion and encoding for transmission to the receiver **104**.

Referring yet again to FIG. 2, the temperature detection section **203** of the transmitter **102** is configured to monitor the temperature of the skin near the sensor insertion site. The temperature reading is used to adjust the glucose readings obtained from the analog interface **201**. As discussed above, the input section **202** of the transmitter **102** includes the disable device which allows the user to temporarily disable the transmitter **102** such as for, example, to comply with the FAA regulations when aboard an aircraft. Moreover, in a further embodiment, the disable device may be further configured to interrupt the transmitter processor **204** of the transmitter **102** while in the low power, non-operating mode to initiate operation thereof.

The RF transmitter **206** of the transmitter **102** may be configured for operation in the frequency band of 315 MHz to 322 MHz, for example, in the United States. Further, in one embodiment, the RF transmitter **206** is configured to modulate the carrier frequency by performing Frequency Shift Keying and Manchester encoding. In one embodiment, the data transmission rate is 19,200 symbols per second, with a minimum transmission range for communication with the receiver **104**.

FIG. 3 is a block diagram of the receiver **104** of the continuous glucose monitoring system **100** in accordance with one embodiment of the present invention. Referring to FIG. 3, the receiver **104** includes a blood glucose test strip interface **301**, an RF receiver **302**, an input **303**, a temperature detection section **304**, and a clock **305**, each of which is operatively coupled to a receiver processor **307**. As can be further seen from the Figure, the receiver **104** also includes a power supply **306** operatively coupled to a power conversion and monitoring section **308**. Further, the power conversion and monitoring section **308** is also coupled to the receiver processor **307**. Moreover, also shown are a receiver serial communication section **309**, and an output **310**, each operatively coupled to the receiver processor **307**.

In one embodiment, the test strip interface **301** includes a glucose level testing portion to receive a manual insertion of a glucose testing strip, and thereby determine and display the glucose level of the testing strip on the output **310** of the receiver **104**. This manual testing of glucose can be used to calibrate sensor **101**. The RF receiver **302** is configured to communicate, via the communication link **103** (FIG. 1) with the RF transmitter **206** of the transmitter **102**, to receive encoded data signals from the transmitter **102** for, among others, signal mixing, demodulation, and other data processing. The input **303** of the receiver **104** is configured to allow the user to enter information into the receiver **104** as needed. In one aspect, the input **303** may include one or more keys of a keypad, a touch-sensitive screen, or a voice-activated input command unit. The temperature detection section **304** is configured to provide temperature information of the receiver **104** to the receiver processor **307**, while the clock **305** provides, among others, real time information to the receiver processor **307**.

Each of the various components of the receiver **104** shown in FIG. 3 are powered by the power supply **306** which, in one embodiment, includes a battery. Furthermore, the power conversion and monitoring section **308** is configured to monitor the power usage by the various components in the receiver **104** for effective power management and to alert the user, for example, in the event of power usage

which renders the receiver **104** in sub-optimal operating conditions. An example of such sub-optimal operating condition may include, for example, operating the vibration output mode (as discussed below) for a period of time thus substantially draining the power supply **306** while the processor **307** (thus, the receiver **104**) is turned on. Moreover, the power conversion and monitoring section **308** may additionally be configured to include a reverse polarity protection circuit such as a field effect transistor (FET) configured as a battery activated switch.

The serial communication section **309** in the receiver **104** is configured to provide a bi-directional communication path from the testing and/or manufacturing equipment for, among others, initialization, testing, and configuration of the receiver **104**. Serial communication section **309** can also be used to upload data to a computer, such as time-stamped blood glucose data. The communication link with an external device (not shown) can be made, for example, by cable, infrared (IR) or RF link. The output **310** of the receiver **104** is configured to provide, among others, a graphical user interface (GUI) such as a liquid crystal display (LCD) for displaying information. Additionally, the output **310** may also include an integrated speaker for outputting audible signals as well as to provide vibration output as commonly found in handheld electronic devices, such as mobile telephones presently available. In a further embodiment, the receiver **104** also includes an electro-luminescent lamp configured to provide backlighting to the output **310** for output visual display in dark ambient surroundings.

Referring back to FIG. 3, the receiver **104** in one embodiment may also include a storage section such as a programmable, non-volatile memory device as part of the processor **307**, or provided separately in the receiver **104**, operatively coupled to the processor **307**. The processor **307** is further configured to perform Manchester decoding as well as error detection and correction upon the encoded data signals received from the transmitter **102** via the communication link **103**.

In conjunction with FIGS. 4, 5A, 5B and 5C, a description is provided of a data packet from the transmitter **102** to the receiver **104** via the communication link **103**.

FIG. 4 illustrates a data pack from the transmitter **102** (FIG. 1) in accordance with one embodiment of the present invention. Referring to FIG. 4, each data packet from the transmitter **102** includes 13 bytes as shown in the Figure. For example, the first byte (zero byte) includes the transmitter **102** identification information ("Tx ID"), while the third byte (byte two) provides transmitter status information, where a high nibble (byte) indicates an operating mode status, while a low nibble indicates a non-operating mode. In this manner, the signals received from the sensor **101** are packed into 13-byte data packs, for transmission to the receiver **104**.

FIGS. 5A, 5B and 5C illustrate a data packet table for Reed-Solomon encoding in the transmitter, a depadded data table, and a link prefix table, respectively, in accordance with one embodiment of the continuous glucose monitoring system of FIG. 1. Referring to FIG. 5A, it can be seen that the Reed Solomon encoded data block contents include 13 bytes of packed data (FIG. 4), one byte of the middle significant bit of the transmitter identification information (Tx ID), one byte of the most significant bit of the transmitter identification information, 232 bytes of zero pads, 8 bytes of parity symbols, to comprise a total of 255 bytes. In one embodiment, the Reed Solomon encode procedure at the transmitter **102** uses 8 bit symbols for a 255 symbol block to generate 8 parity symbols. Thereafter, the transmitter **102**

is configured to remove the 232 bytes of zero pads, resulting in the 21 bytes of depadded data block including the 13 bytes of packed data as well as the 8 bytes of the parity symbols as shown in FIG. 5B.

Thereafter, a link prefix is added to the depadded data block to complete the data packet for transmission to the receiver **104**. The link prefix allows the receiver **104** to synchronize with the transmitter **102** as described in further detail below. More specifically, as shown in FIG. 5C, the transmitter **102** is configured to add 4 bytes of link prefix (0x00, 0x00, 0x12, and 0x34) to the 21 bytes of depadded data block to result in 25 bytes of data packet. Once powered up and enabled in operational mode, the transmitter **102** is configured to transmit the 25 byte data packet once every minute. More specifically, the transmitter **102** is configured to Manchester encode the data at 2 bits per data bit (0=10; 1=01), and transmit the Manchester bits at 19,200 symbols per second. The transmitter **102** is configured to transmit the data packets with the most significant bit of byte zero first.

FIG. 6 is a flowchart illustrating the time hopping procedure for the receiver of the continuous glucose monitoring system shown in FIG. 1 in accordance with one embodiment of the present invention.

Referring to FIG. 6, upon completing the power up procedure as discussed above, the receiver **104** listens for the presence of a transmitter within the RF communication link range. At step **601**, when the transmitter **102** is detected within the RF communication link range, the receiver **104** is configured to receive and store the identification information corresponding to the detected transmitter **102**. Thereafter, at step **602**, the receiver **104** is configured to detect (or sample) data transmission within its RF communication range. In one aspect, the receiver **104** is configured to identify a positive data transmission upon ascertaining that the data transmission is above a predetermined strength level for a given period of time (for example, receiving three separate data signals above the predetermined strength level from the transmitter **102** at one minute intervals over a period of five minutes).

At step **603**, the receiver **104** is configured to determine whether the detected signals within the RF communication range is transmitted from the transmitter **102** having the transmitter identification information stored in the receiver **104**. If it is determined at step **603** that the detected data transmission at step **602** does not originate from the transmitter with the stored transmitter identification information, then the procedure returns to step **602** and waits for the detection of the next data transmission.

On the other hand, if at step **603** it is determined that the detected data transmission is from the transmitter **102** corresponding to the stored transmitter identification information, then at step **604**, the receiver proceeds with decoding the received data and performing error correction thereon. In one embodiment, the receiver is configured to perform Reed-Solomon decoding, where the transmitted data received by the receiver is encoded with Reed-Solomon encoding. Furthermore, the receiver is configured to perform forward error correction to minimize data error due to, for example, external noise, transmission noise and so on.

Referring back to FIG. 6, after decoding and error correcting the received data, the receiver **104** at step **605** generates output data corresponding to the decoded error corrected data received from the transmitter **102**, and thereafter, at step **606**, the receiver **104** outputs the generated output data for the user as a real time display of the output data, or alternatively, in response to the user operation requesting the display of the output data. Additionally,

before displaying the output data for the user, other pre-processing procedures may be performed on the output data to for example, smooth out the output signals. In one aspect, the generated output data may include a visual graphical output displayed on the graphical user interface of the receiver. Alternatively, the output data may be numerically displayed representing the corresponding glucose level.

Referring now to FIGS. 4 and 6, the time hopping procedure of one embodiment is described. More specifically, since more than one transmitter 102 may be within the receiving range of a particular receiver 104, and each transmitting data every minute on the same frequency, transmitter units 102 are configured to transmit data packets at different times to avoid co-location collisions (that is, where one or more receivers 104 cannot discern the data signals transmitted by their respective associated transmitter units 102 because they are transmitting at the same time).

In one aspect, transmitter 102 is configured to transmit once every minute randomly in a window of time of plus or minus 5 seconds (i.e., it time hops.) To conserve power, receiver 104 does not listen for its associated transmitter 102 during the entire 10 second receive window, but only at the predetermined time it knows the data packet will be coming from the corresponding transmitter 102. In one embodiment, the 10 second window is divided into 400 different time segments of 25 milliseconds each. Before each RF transmission from the transmitter 102 takes place, both the transmitter 102 and the receiver 104 is configured to recognize in which one of the 400 time segments the data transmission will occur (or in which to start, if the transmission time exceeds 25 milliseconds). Accordingly, receiver 104 only listens for a RF transmission in a single 25 millisecond time segment each minute, which varies from minute to minute within the 10 second time window.

Moreover, each transmitter 102 is configured to maintain a "master time" clock that the associated receiver unit 104 may reference to each minute (based on the time of transmission and known offset for that minute). A counter also on the transmitter 102 may be configured to keep track of a value "Tx Time" that increments by 1 each minute, from 0 to 255 and then repeats. This Tx Time value is transmitted in the data packet each minute, shown as Byte 1 in FIG. 4. Using the Tx Time value and the transmitter's unique identification information (TX ID, shown as Byte 0 in FIG. 4), both the transmitter 102 and the receiver 104 can calculate which of the 400 time segments will be used for the subsequent transmission. In one embodiment, the function that is used to calculate the offset from the master clock 1-minute tick is a pseudo-random number generator that uses both the Tx Time and the TX ID as seed numbers. Accordingly, the transmission time varies pseudo-randomly within the 10 second window for 256 minutes, and then repeats the same time hopping sequence again for that particular transmitter 102.

In the manner described above, in accordance with one embodiment of the present invention, co-location collisions may be avoided with the above-described time hopping procedure. That is, in the event that two transmitters interfere with one another during a particular transmission, they are not likely to fall within the same time segment in the following minute. As previously described, three glucose data points are transmitted each minute (one current and two redundant/historical), so collisions or other interference must occur for 3 consecutive data transmissions for data to be lost. In one aspect, when a transmission is missed, the receiver 104 may be configured to successively widen its listening window until normal transmissions from the

respective transmitter 102 resume. Under this approach, the transmitter listens for up to 70 seconds when first synchronizing with a transmitter 102 so it is assured of receiving a transmission from transmitter 102 under normal conditions.

Various other modifications and alterations in the structure and method of operation of this invention will be apparent to those skilled in the art without departing from the scope and spirit of the invention. Although the invention has been described in connection with specific preferred embodiments, it should be understood that the invention as claimed should not be unduly limited to such specific embodiments. It is intended that the following claims define the scope of the present invention and that structures and methods within the scope of these claims and their equivalents be covered thereby.

What is claimed is:

1. An analyte monitoring system, comprising:

a sensor configured to generate signals corresponding to a monitored analyte level in interstitial fluid; and sensor electronics operatively coupled to the sensor, the sensor electronics comprising (i) a processor configured to process the generated signals to form data packets associated with the generated signals from the sensor, and (ii) a temperature sensor configured to monitor temperature associated with the sensor, wherein the monitored temperature is used to adjust the processed generated signals;

wherein the sensor electronics include programming to provide data communications to a receiving device by at least communicating one or more data packets with each data communication during a period of time corresponding to a predetermined listening window, the data packets including at least a current data point that corresponds to an analyte level of a current time period, a time value information that corresponds to a point in time when the one or more data packets are communicated from the sensor electronics to the receiving device, and data identifying the sensor electronics;

wherein the receiving device is configured to use the time value information and the data identifying the sensor electronics to identify the predetermined listening window;

wherein the sensor electronics further include programming to communicate the one or more data packets by data communications to the receiving device at a time outside the predetermined listening window in response to a user request provided from the receiving device; and

wherein the sensor electronics further include programming to, in response to the current data point not being successfully received by the receiving device, transmit at least one subsequent data communication including a subsequent data packet during a subsequent widened time period greater than the predetermined listening window, the subsequent data packet including at least a subsequent data point that corresponds to an analyte level at that subsequent time period.

2. The system of claim 1, wherein the subsequent data packet at least includes two consecutive data points that correspond to the monitored analyte levels of two consecutive previous time periods with respect to the subsequent data point, one of the two consecutive previous time periods immediately preceding the subsequent widened time period.

3. The system of claim 2, wherein the two consecutive data points of the subsequent data packet includes the current data point, and wherein the one of the two consecu-

13

tive previous time periods immediately preceding the subsequent widened time period is the current time period.

4. The system of claim 1, wherein the subsequent data communication is transmitted to the receiving device so that the receiving device may receive and ascertain the current data point.

5. The system of claim 1, wherein the receiving device comprises a receiver unit configured for receiving the data packets over a paired communication link from the sensor electronics.

6. The system of claim 5, wherein the sensor is configured to generate the signals corresponding to the monitored analyte level while operating in an operational mode, wherein the sensor is further configured to operate in a non-operational mode wherein the analyte level is not monitored and the signals corresponding to the monitored analyte level are not generated; wherein the processor of the sensor electronics is configured to determine whether the sensor is operating in the operational mode or the non-operational mode, and is further configured to form the data packets associated with the generated signals from the sensor when the sensor is operating in the operational mode, and is further configured to form the data packets associated with the generated signals from the sensor to include an indicator that the sensor is operating in the operational mode; and wherein the receiver unit is configured to determine that the sensor is operating in the operational mode in response to receiving the data packets associated with the generated signals from the sensor, based on the indicator.

7. The system of claim 5, wherein the sensor electronics is configured to encode the data packets to generate encoded data packets, the sensor electronics further configured to communicate the encoded data packets to the receiver unit.

8. The system of claim 5, wherein the receiver unit is configured to decode encoded signals received from the sensor electronics.

9. The system of claim 5, wherein the receiver unit is configured to receive the one or more data packets, and includes an output unit for outputting data related to the received one or more data packets, wherein the data is related to one or more glucose levels.

10. The system of claim 1, wherein the data packets includes data points corresponding to the monitored analyte level over a predetermined time period.

11. The system of claim 1, wherein the sensor electronics is configured to store a count; wherein the sensor electronics is further configured to increment the count each minute; and wherein the time value information corresponds to the stored count at the point in time when the one or more data packets are communicated.

12. The system of claim 1, wherein the receiving device is further configured to determine a wait time period for the predetermined listening window based at least on time intervals between at least three previous communications from the sensor electronics to the receiving device.

13. An apparatus, comprising:

one or more processors; and

a memory operatively coupled to the one or more processors, the memory for storing instructions which, when executed by the one or more processors, causes the one or more processors to:

process signals received and generated from an analyte sensor to form data packets associated with the gener-

14

ated signals from the analyte sensor, the signals corresponding to a monitored analyte level in interstitial fluid;

provide data communications to a receiving device by at least communicating one or more data packets with each data communication during a period of time corresponding to a predetermined listening window, the data packets including at least a current data point that corresponds to an analyte level of a current time period, a time value information that corresponds to a point in time when the one or more data packets are communicated from the apparatus to the receiving device, and data identifying the apparatus, wherein the receiving device is configured to use the time value information and the data identifying the apparatus to identify the predetermined listening window;

provide data communications to the receiving device by at least communicating the one or more data packets by data communications to the receiving device at a time outside the predetermined listening window in response to a user request provided from the receiving device; and

in response to the current data point not being successfully received by the receiving device, transmit at least one subsequent data communication including a subsequent data packet during a subsequent widened time period greater than the predetermined window, the subsequent data packet including at least a subsequent data point that corresponds to an analyte level at that subsequent time period.

14. The apparatus of claim 13, wherein the subsequent data packet at least includes two consecutive data points that correspond to the monitored analyte levels of two consecutive previous time periods with respect to the subsequent data point, one of the two consecutive previous time periods immediately preceding the subsequent widened time period.

15. The apparatus of claim 14, wherein the two consecutive data points of the subsequent data packet includes the current data point, and wherein the one of the two consecutive previous time periods immediately preceding the subsequent widened time period is the current time period.

16. The apparatus of claim 13, wherein the subsequent data communication is transmitted to the receiving device so that the receiving device may receive and ascertain the current data point.

17. The apparatus of claim 13, wherein the one or more processors is configured to encode the data packets to generate encoded data packets for the data communication.

18. The apparatus of claim 13, wherein the data packets includes data points corresponding to monitored analyte level over a predetermined time period.

19. The apparatus of claim 13, further including a temperature sensor operatively coupled to the one or more processors and configured to monitor temperature associated with the analyte sensor, wherein the monitored temperature is used to adjust the processed generated signals.

20. The apparatus of claim 19, wherein the temperature sensor detects temperature level of an insertion site of the analyte sensor to obtain a temperature reading, wherein the one or more processors uses the temperature reading to adjust the processed generated signals.

* * * * *

专利名称(译)	连续血糖监测系统和使用方法		
公开(公告)号	US9962091	公开(公告)日	2018-05-08
申请号	US14/148034	申请日	2014-01-06
[标]申请(专利权)人(译)	雅培糖尿病护理公司		
申请(专利权)人(译)	雅培糖尿病INC.		
当前申请(专利权)人(译)	雅培糖尿病INC.		
[标]发明人	JIN ROBERT Y SLOAN MARK KENT		
发明人	JIN, ROBERT Y. SLOAN, MARK KENT		
IPC分类号	A61B5/00 A61B5/01 A61B5/145		
CPC分类号	A61B5/01 A61B5/14532 A61B5/0002 A61B2562/08		
其他公开文献	US20140121477A1		
外部链接	USPTO		

摘要(译)

一种连续葡萄糖监测系统，包括配置成检测一个或多个葡萄糖水平的传感器，可操作地耦合到所述传感器的发射器，所述发射器配置成接收检测到的一个或多个葡萄糖水平，所述发射器还配置为发射与检测到的一个或多个葡萄糖水平，以及可操作地耦合到发射器的接收器及其方法被公开，所述接收器被配置为接收对应于检测到的一个或多个葡萄糖水平的发射信号。在一个方面，发射器可以被配置为发送当前数据点和至少一个先前数据点，当前数据点和与检测到的一个或多个葡萄糖水平相对应的至少一个先前数据点。

