



US010251286B2

(12) **United States Patent**
Rickert et al.

(10) **Patent No.: US 10,251,286 B2**
(45) **Date of Patent: Apr. 2, 2019**

(54) **MEDICAL IMPLANT AS WELL AS METHOD
FOR THE PRODUCTION THEREOF**

2560/0219; A61B 2562/0247; A61B
2562/0271; A61B 2562/029; H05K
5/0247; H05K 5/0004; H05K 5/0239;
H05K 5/02; H04Q 9/14; B23K 1/20;
B23K 1/0008

(71) Applicant: **CorTec GmbH**, Freiburg (DE)

(72) Inventors: **Jörn Rickert**, Freiburg (DE); **Fabian
Kohler**, Freiburg (DE); **Martin
Schüttler**, Freiburg (DE)

See application file for complete search history.

(73) Assignee: **CorTec GmbH**, Freiburg (DE)

(56) **References Cited**

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 881 days.

5,556,421 A 9/1996 Prutchi et al.
8,332,037 B2 * 12/2012 Imran A61N 1/375
607/36

(Continued)

(21) Appl. No.: **14/629,454**

FOREIGN PATENT DOCUMENTS

(22) Filed: **Feb. 23, 2015**

(65) **Prior Publication Data**

US 2015/0173215 A1 Jun. 18, 2015

CN 1907514 A 2/2007
CN 101935208 A 1/2011

(Continued)

Related U.S. Application Data

(63) Continuation of application No.
PCT/EP2013/067526, filed on Aug. 23, 2013.

Chinese Search Report issued for corresponding Chinese Patent
Application No. 201380043713X dated Jun. 12, 2016 with an
English translation.

(51) **Int. Cl.**
H05K 5/02 (2006.01)
H05K 5/00 (2006.01)

(Continued)

(Continued)

(52) **U.S. Cl.**
CPC **H05K 5/02** (2013.01); **A61B 5/0031**
(2013.01); **A61B 5/686** (2013.01); **B23K**
1/0008 (2013.01); **B23K 1/20** (2013.01);
H04Q 9/14 (2013.01); **H05K 5/0004**
(2013.01); **H05K 5/0239** (2013.01); **H05K**
5/0247 (2013.01); **A61B 2560/0219** (2013.01);
A61B 2562/029 (2013.01); **A61B 2562/0247**
(2013.01); **A61B 2562/0271** (2013.01)

Primary Examiner — Christine H Matthews

Assistant Examiner — Joshua D Lannu


(74) *Attorney, Agent, or Firm* — Myers Wolin, LLC

(57) **ABSTRACT**

Disclosed are a housing for a medical implant, a medical
implant for a human or animal organism, a method for
manufacturing a medical implant, and a system comprising
a medical implant and a transceiver unit that can be coupled
to the medical implant.

(58) **Field of Classification Search**
CPC A61B 5/686; A61B 5/0031; A61B

11 Claims, 6 Drawing Sheets

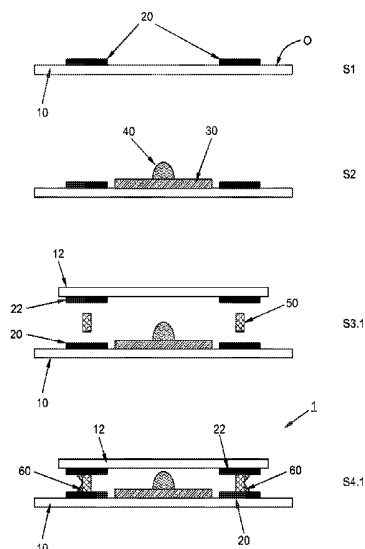

(51) **Int. Cl.**
B23K 1/20 (2006.01)
H04Q 9/14 (2006.01)
A61B 5/00 (2006.01)
B23K 1/00 (2006.01)

EP	1184351	A1	3/2002
JP	2010246856	A	11/2010
JP	2011500143	A	1/2011
JP	2011516198	A	5/2011
WO	2009048580	A1	4/2009
WO	2009125903	A1	10/2009
WO	2012126003	A1	9/2012

(56) **References Cited**

U.S. PATENT DOCUMENTS

2006/0212096	A1 *	9/2006	Stevenson		A61N 1/37211	607/60
2006/0217792	A1	9/2006	Hussein et al.			
2007/0167867	A1 *	7/2007	Wolf		A61B 5/0017	600/561
2009/0204141	A1 *	8/2009	Dlugos, Jr.		A61F 5/0059	606/191
2010/0114205	A1	5/2010	Donofrio et al.			
2010/0114225	A1 *	5/2010	Imran		A61N 1/375	607/9
2010/0262208	A1	10/2010	Parker			

FOREIGN PATENT DOCUMENTS

CN	101939043	A	1/2011
CN	102027757	A	4/2011
DE	103 23 627	A1	12/2004
DE	10 2011 009 867	A1	8/2012

OTHER PUBLICATIONS

German Search Report issued for corresponding German Patent Application No. 10 2012 107 835.1 dated May 2, 2013 with an English translation.


Mi et al., "The Research and Development of Transparent Ceramics", vol. 26, No. 4, Bulletin of the Chinese Ceramic Society, pp. 1, 766-769 and 820, Aug. 2007 with an English translation.

International Preliminary Report on Patentability with the Written Opinion issued for corresponding International Patent Application No. PCT/EP2013/067526 dated Feb. 24, 2015 with an English abstract and an English translation.

International Search Report dated Jan. 15, 2014 in corresponding International Application No. PCT/EP2013/067526.

Notice of Reasons for Rejection issued for corresponding Japanese Patent Application No. 2015-527929 dated Jul. 3, 2017 with an English Translation.

* cited by examiner

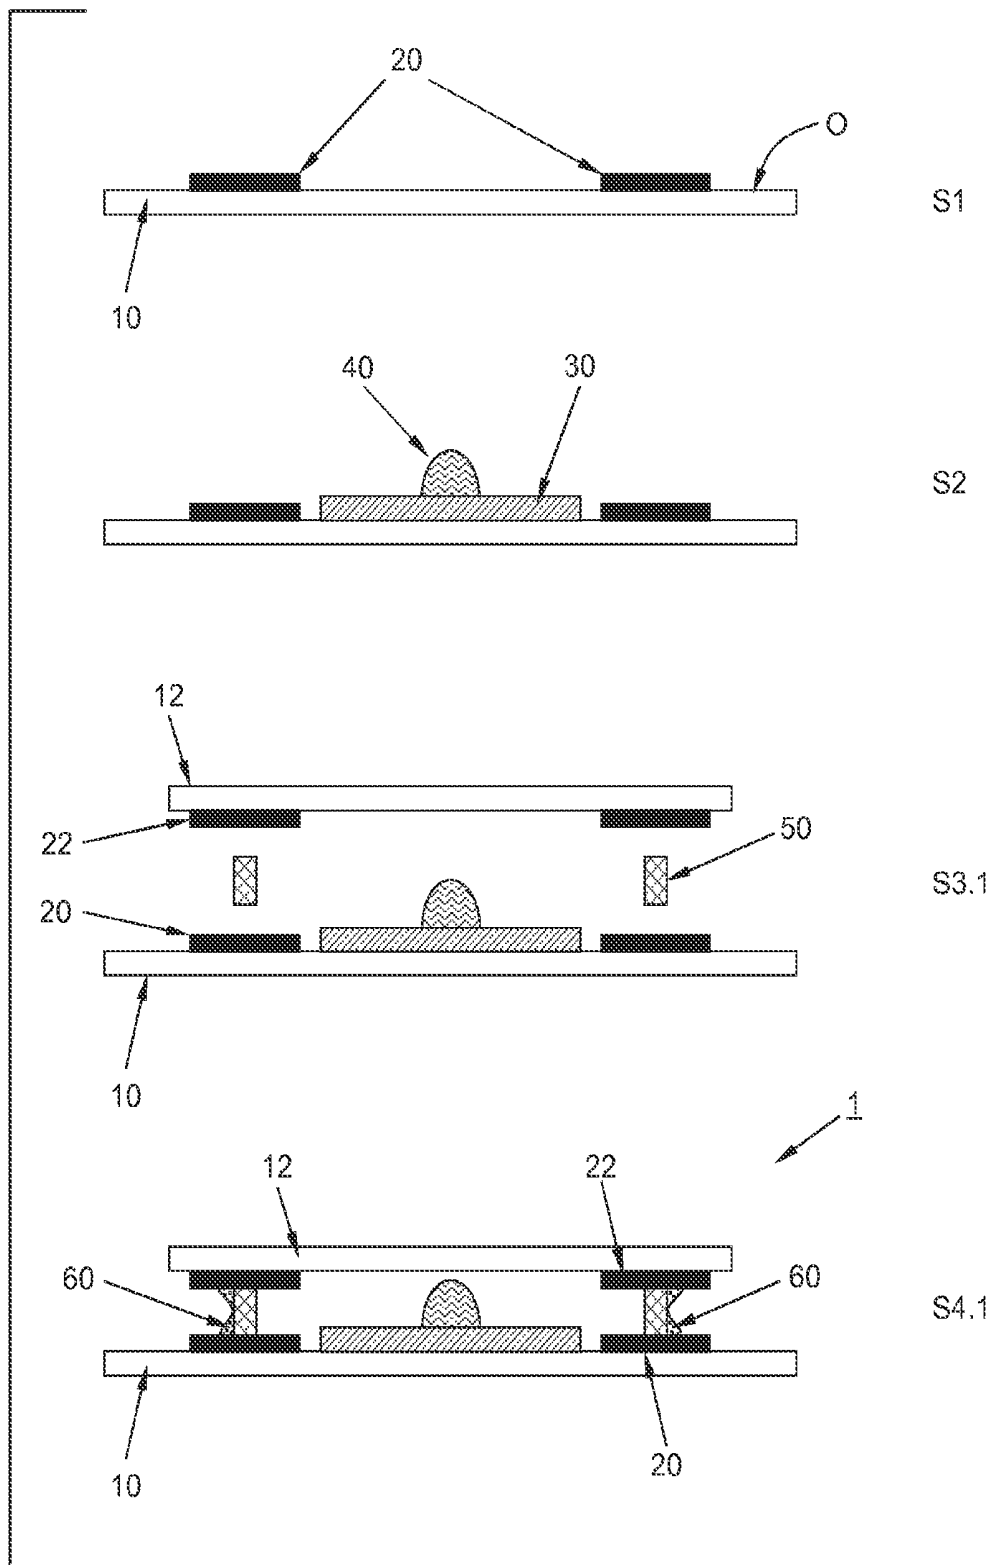*FIG. 1*

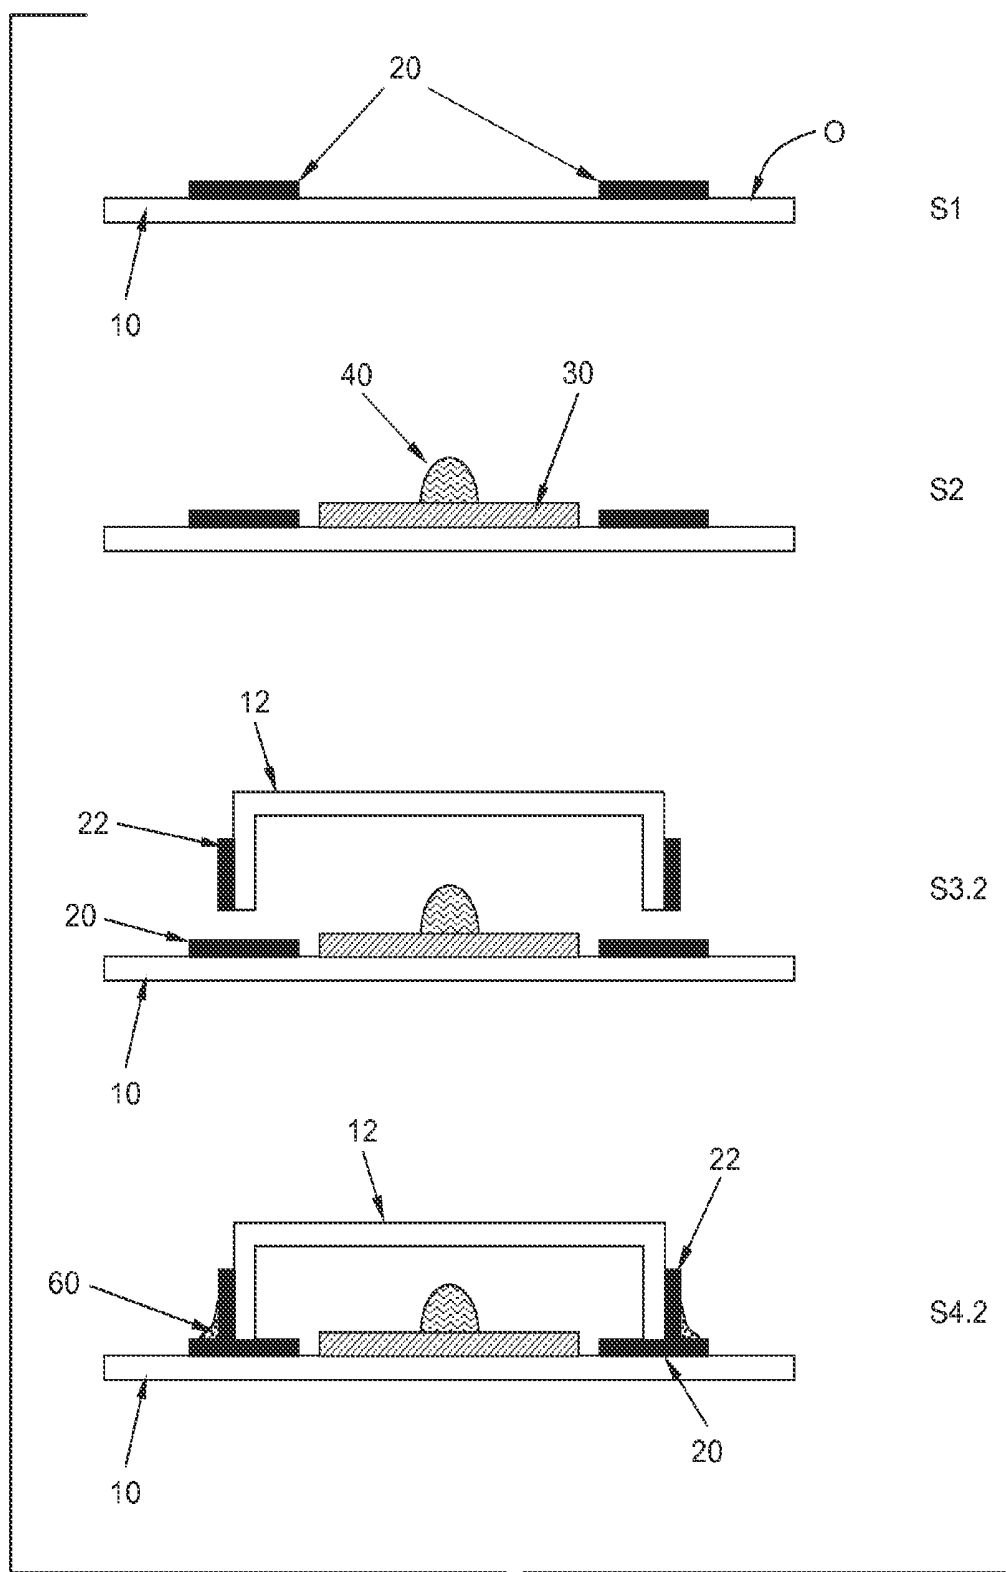
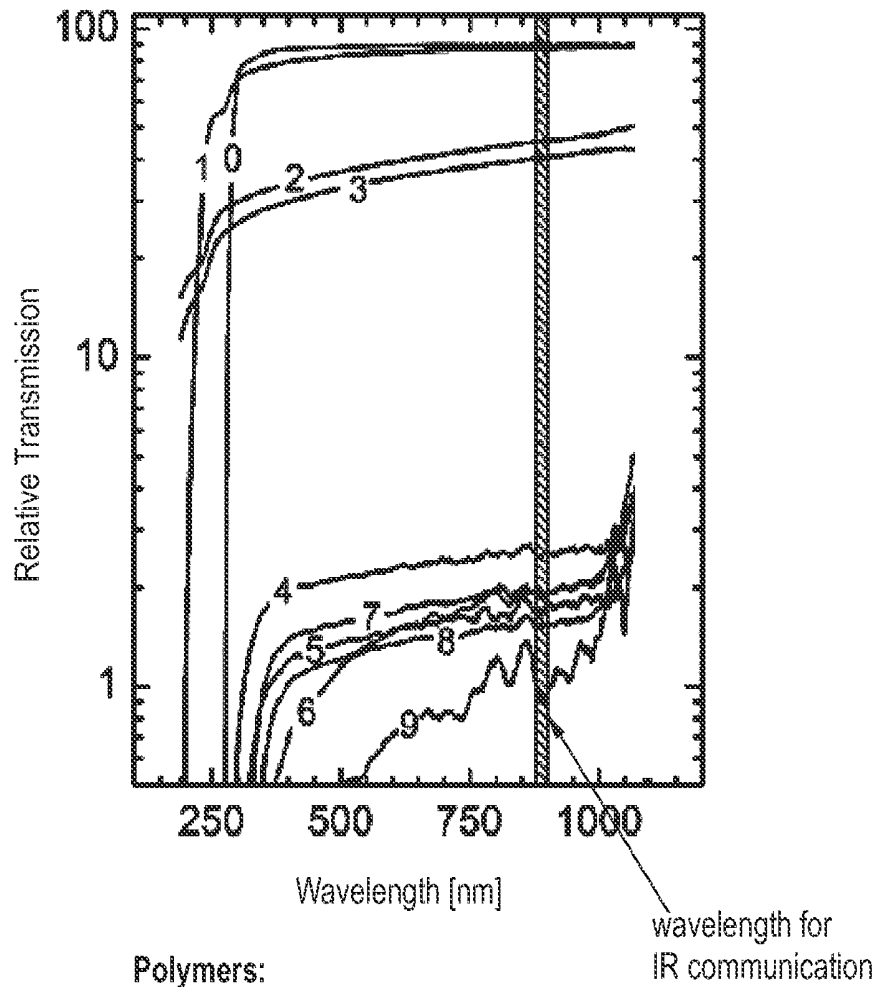


FIG. 2

**Polymers:**

- (0) Parylene C, 15 μm : 89.5 %
- (1) PDMS (MED-1000), 300 μm : 87.5 %

Ceramics:

- (2) Sapphire, 430 μm : 45.5 %
- (3) Sapphire, 330 μm : 40.5 %
- (4) HTCC 44000, 175 μm : 2.45 %
- (5) HTCC 44000, 290 μm : 1.67 %
- (6) Rubalit 710, 635 μm : 1.9 %
- (7) Rubalit 708S, 380 μm : 1.9 %
- (8) Rubalit 708S, 635 μm : 1.5 %
- (9) Aluminum, 2mm: 0.95 %

FIG. 3

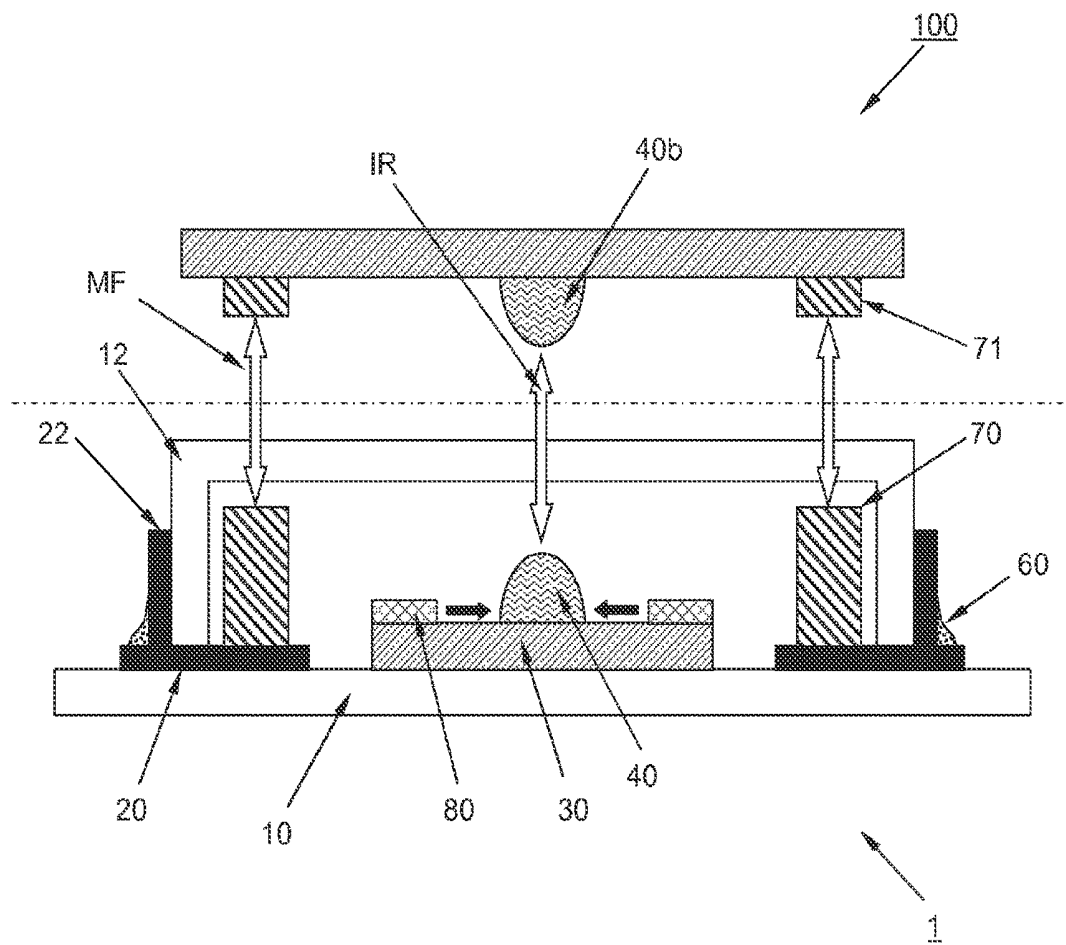
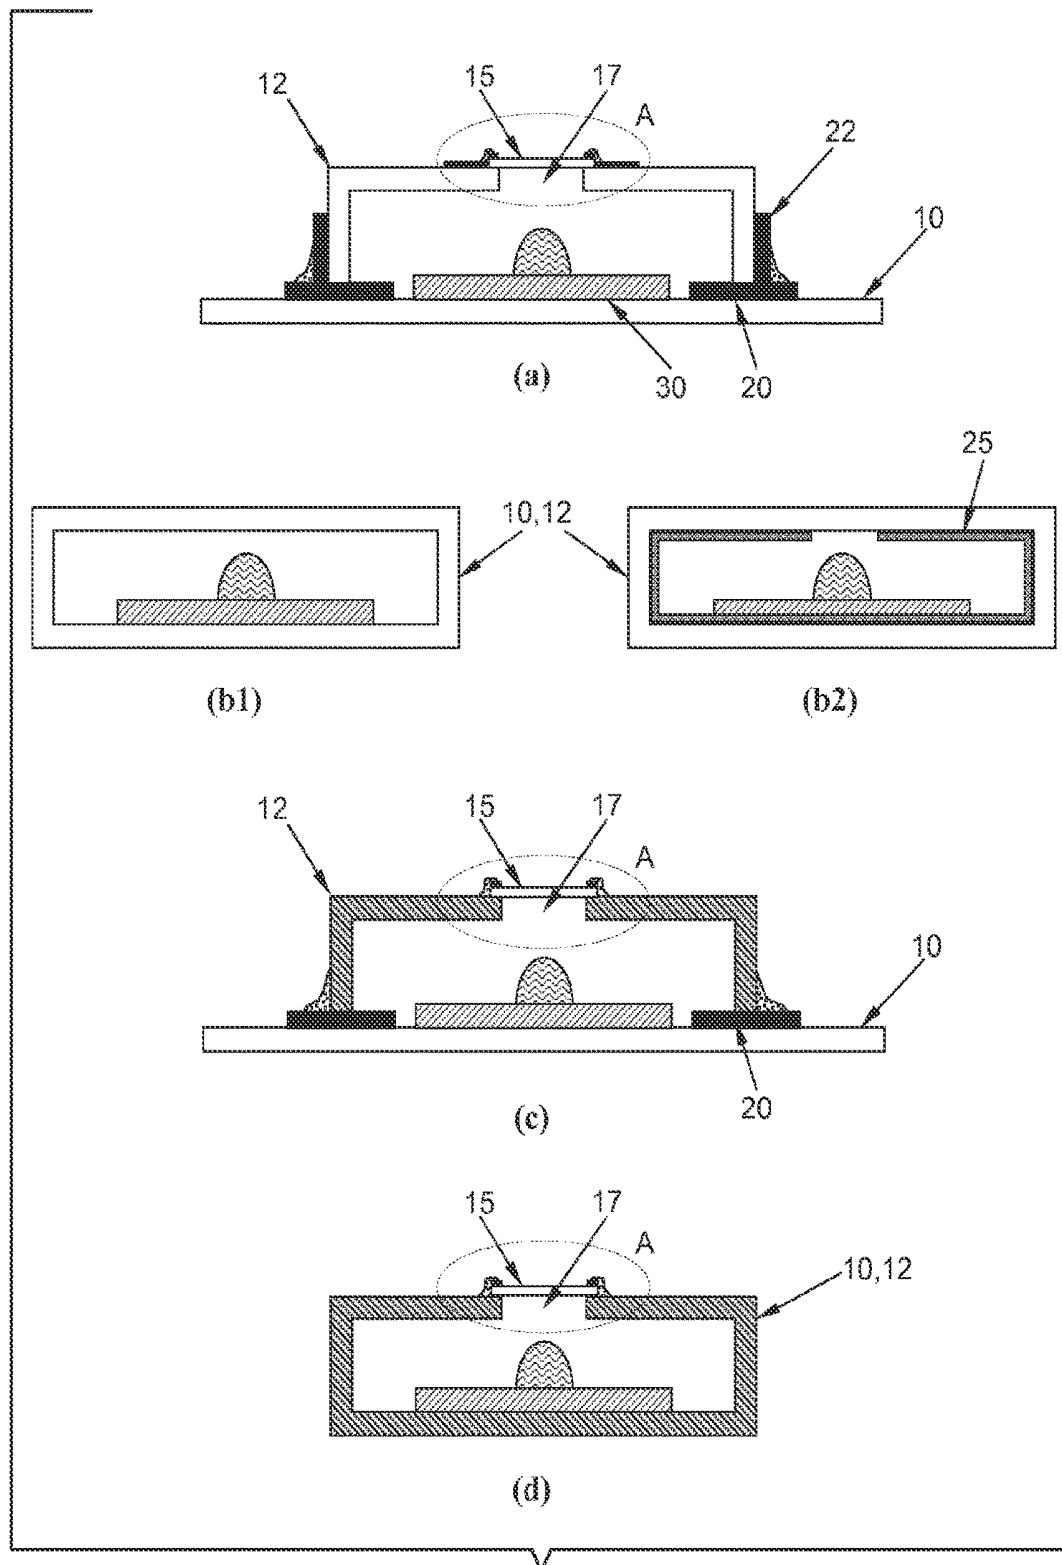


FIG. 4

**FIG. 5**

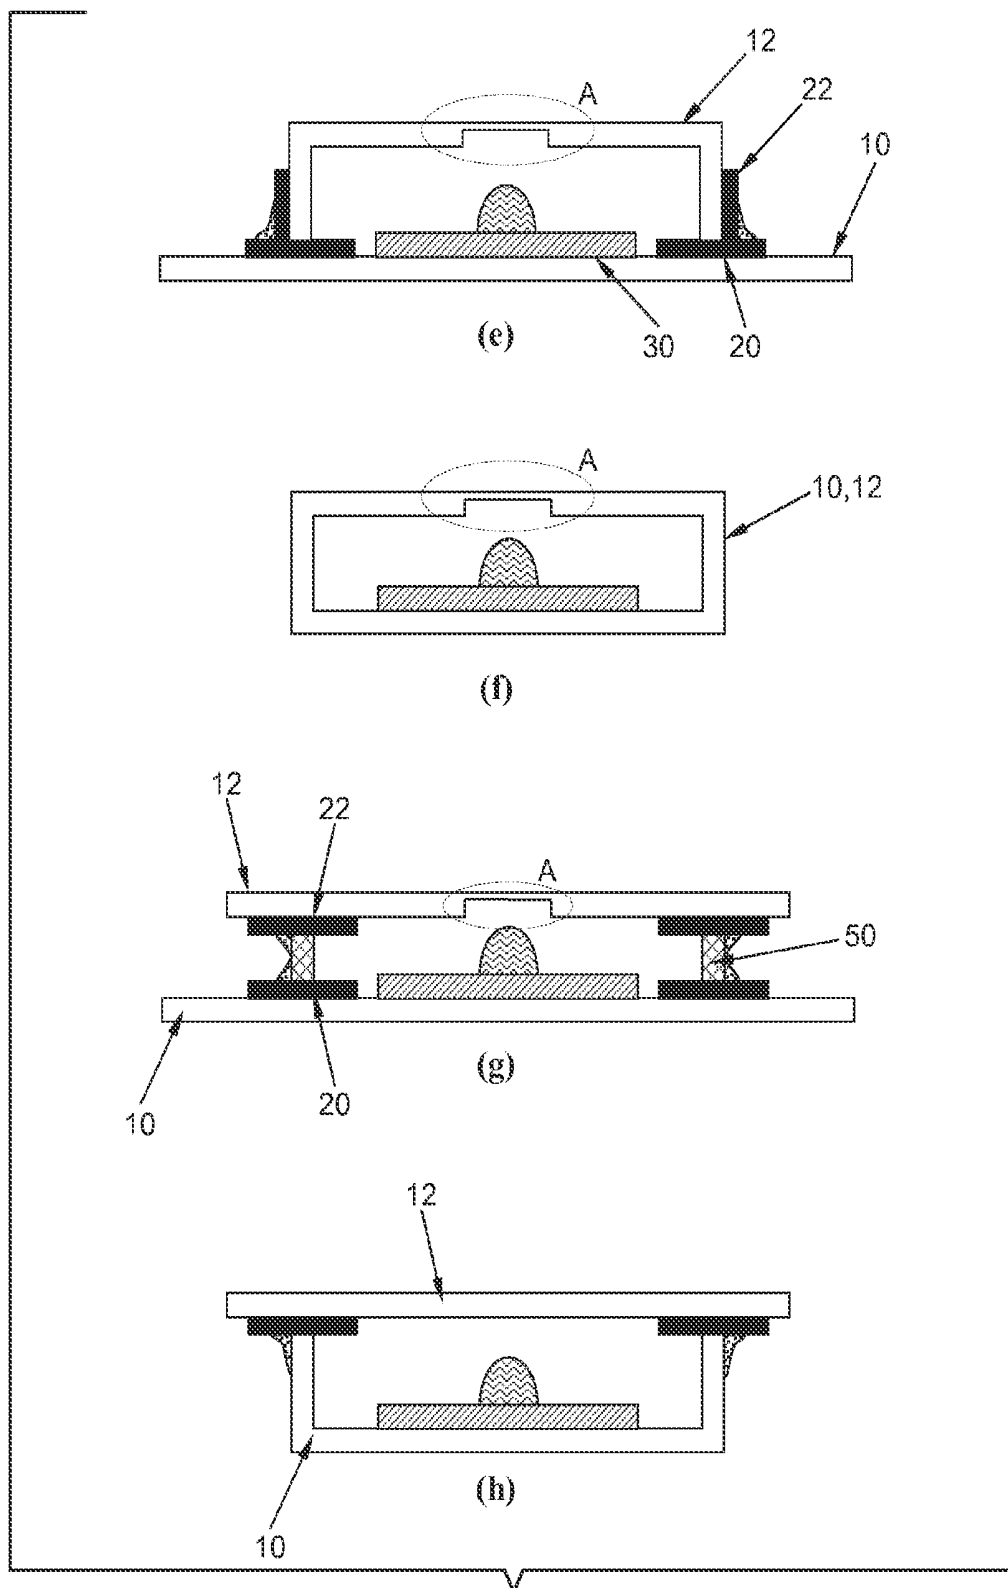


FIG. 6

MEDICAL IMPLANT AS WELL AS METHOD FOR THE PRODUCTION THEREOF

CROSS REFERENCE TO RELATED APPLICATIONS

This application is a continuation of international Application No. PCT/EP2013/067526, filed Aug. 23, 2013, which claims priority to German Application No. 10 2012 107 835.1, filed Aug. 24, 2012, the contents of each are incorporated by reference herein.

FIELD OF THE INVENTION

The invention relates to a medical implant for a human or animal organism, a housing for a medical implant, a method for the production of a medical implant, as well as a system which comprises the medical implant according to the invention, and a transceiver unit which can be coupled to the medical implant.

BACKGROUND OF THE INVENTION AND PRIOR ART

It is known to arrange medical implants, in particular, active medical implants tier a human or animal organism in a housing which then is implanted into the human or animal body. The implant housings, thereby, are mostly made from metal shells. Further, it is known to configure the implants such that a communication between the implant and an external transceiver unit is enabled. The communication, hereby, is carried out via radio or inductance.

During communication via inductance, however, the transmission bandwidth is restricted by the carrier frequency. In case the carrier frequency is selected to be high for a high bandwidth, i.e., high data traffic, then it will be attenuated by the materials of the housing and/or by the biological tissue. The thus resulting loss has to be compensated for in that the transmission power is increased accordingly, the latter being detrimental in case the implant is powered by a battery. An increased transmission power may also be detrimental to the biological tissue surrounding the implant if, for example, due to the increased transmission power, the tissue immediately surrounding the implant is heated directly or indirectly by the inherent electrical losses of the electronic circuits.

Further, with respect to the implant housings known from prior art it is disadvantageous that moisture, for example, body fluid enters into the housing which may impair the implant electronics within the housing. It is known to design implants or implant housings such that a leak through which moisture may enter has to be correspondingly small. The expected durability of the implant is estimated during production by measuring the leak. This, however, is disadvantageous in case the implant has to be designed such that it does not have to be replaced during the lifetime of the patient, and has to operate reliably, if needed, over many decades. However, in case moisture enters into the implant housing, functional disorders or even failure of the implant may occur, thus, being detrimental to the patient's health.

Therefore, it is an object of the invention to provide solutions for a medical implant which at least partially overcomes the disadvantages known from prior art, and which enables a high bandwidth of communication between the implant and an external transceiver unit with a high durability of the implant at the same time.

SUMMARY

This object is solved according to the invention by a medical implant for a human or animal organism, a housing for a medical implant, a method for the production of a medical implant, as well as a system which comprises a medical implant, and a transceiver unit which can be coupled to the medical implant, according to the independent claims. Preferred embodiments and further developments of the invention are specified in the respective dependent claims.

Accordingly, a housing for a medical implant is provided wherein a housing wall of the housing is configured to be at least partially transparent, in particular, transparent to infrared light. It is advantageous if the housing wall or at least parts thereof which is/are transparent to light or transparent to infrared light is/are transparent to light having a wavelength of approximately between 700 nm and 1000 nm, preferably between 850 nm and 900 nm. Light of these wavelengths is absorbed at least by the body tissue and, therefore, is suited very well tier data transmission.

The information is transmitted in a manner known per se in that the infrared light source is switched on and off in short sequences which is registered by the respective infrared receiver. As protocol, the IrDA may be provided.

Communication is enabled through the light or infrared transparent housing wall between the implant and an external transceiver unit in bidirectional manner by means of infrared radiation. Thereby, a more energy-efficient and interference-free transmission at higher data rates is enabled. Because an infrared transmission unit is integrated into the housing of the medical implant, or may be arranged in the housing and the data transmission results from the light or infrared transparent area of the housing wall, the housing may be designed in a more air-tight or moisture-tight manner because apertures in the housing wall for cables for the communication with the external transceiver unit may be omitted.

The housing, in particular, the area of the housing which is configured to be transparent to light, may comprise ceramics, in particular, aluminum oxide or zirconium oxide in amorphous, crystalline and/or partially crystalline form, a high temperature multi-layer ceramic with an aluminum oxide proportion, or a glass or glass ceramic.

The area of the housing or housing wall which is configured to be transparent to light, may be formed by a cover which covers the opening in the housing wall. In an advantageous embodiment of the invention, the cover may comprise one of the materials mentioned above.

Moreover, a medical implant for a human or animal organism is provided which has a housing with a housing wall which has at least one area configured to be transparent to light, in particular, transparent to infrared light, and comprises an infrared transmission means and/or infrared receiver means arranged in the interior of the housing.

Because the housing wall is configured to be transparent to light or infrared light, a communication may be performed between the implant and an external transceiver unit through a housing wall. The bandwidth of the communication connection, thereby, can be increased substantially. A further advantage is that the handling and the production of a medical implant can be substantially simplified by integration of all components into a housing. Moreover, additional apertures in the housing for the connection of an external communication unit are omitted allowing a more compact system design and increasing the reliability because, for example, mechanical weak points at the housing do not

occur. Further, due to the data rates which are realizable by the infrared technology, the application range of the implant is substantially increased, and allows the use of more complex and electronic systems for more complex applications.

It has been found to be advantageous if the area which is configured to be transparent to light comprises ceramics, in particular, aluminum oxide or zirconium oxide in amorphous, crystalline, and/or partially crystalline form, a high temperature multi-layer ceramic having an aluminum oxide proportion, or a glass or a glass ceramics.

It has been found that these materials have sufficient high transparency for infrared rays at different thicknesses between about 150 μm and 2 μm .

In an embodiment of the invention, the area being configured to be transparent to light may be formed by a cover which covers an opening in the housing wall. Thereby, the transparent area of the housing can be created in a particularly simple manner which has different materials than the rest of the housing.

It has been found to be advantageous if at least one sensor, in particular, a moisture sensor, and/or a temperature sensor, and/or a pressure sensor, is arranged in the interior of the housing which is coupled operatively to the infrared transmission means and/or infrared receiver means.

Thereby, the possibility is provided in an advantageous manner to acquire parameters of the surroundings of the electronic circuit which are relevant for the reliable operation, for example, moisture, pressure, or temperature of the housing or of the interior of the housing and to communicate the latter via the infrared interface to the outside.

It is advantageous if at least one magnet, in particular, a permanent magnet is arranged within the interior of the housing which may cooperate with magnets of an external transceiver unit arranged outside of the housing. Thereby, a simple alignment of the external transceiver unit with respect to the medical implant may result.

Advantageously, the energy supply of the implant results from magnetic induction wherein an alternating magnetic field required for wireless transmission of energy is provided outside of the body. The alternating magnetic field is not used for the transmission of data such that the alternating magnetic field does not have to be modulated for the purpose of data transfer, and thereby, the use of induction coils with very high quality is enabled on the transmission side and on the receiver side (implant). Thereby, a very efficient coupling to the sender or to the sender-sided induction coil is enabled.

In a preferred embodiment of the implant, the induction coil may be formed by an electrical conductor wrapped around the implant housing. Hereby, it is advantageous if the implant housing is made from ceramics. By means of the coil, the alternating magnetic field is transformed to voltage in the implant.

By the combination of inductive energy supply of the implant with a (bidirectional) IR data transmission, an energy-saving implementation of the implant is possible because the implant, for example, is only activated upon applying the alternating magnetic field to the implant. Moreover, the implant and, in particular, the data transmission are substantially more insensitive to electromagnetic interferences. Further, an internal energy supply, for example, an accumulator, may be provided within the implant which, if needed, can be charged with the transmitted energy inductively. A further advantage is the separation of (bidirectional) data transmission and energy supply.

It has been found to be of further advantage if a desiccant, for example, getter materials, is provided in the housing interior. Thereby, the moisture within the interior of the housing can be reduced, thus, contributing to the protection of the electronic components arranged within the interior of the housing. The desiccant may be applied to the inner wall of the housing.

In an embodiment of the invention, the area of the housing being configured to be transparent to light may have a lower thickness than the rest of the housing. Thereby, a stable housing may be provided which only has a lower thickness in the area which is configured to be transparent to light for the infrared communication.

Further, it has been found to be advantageous if an electrical shielding, for example, a metal foil, is arranged at the inner wall of the housing wherein the electrical shielding is configured such that it is transparent to light or infrared light at predetermined locations.

Further, it may be advantageous to coat the housing with materials which are transparent to light or infrared light. In an embodiment of the invention, the plastics coating can be provided for mechanical protection and for increase of the biocompatibility of the implant which comprises an area configured to be transparent to light or infrared light. Also, the wrapped induction coil may be coated by the plastics coating. Hereby, a multi-layered plastics coating can be provided. In a further embodiment of the invention the exterior side of the housing may be coated with materials which are favorable for biological processes, for example, tissue repair.

Further, a method for the production of a medical implant, in particular, an implant according to the invention, is provided wherein

- a. a first substantially frame-shaped metal layer or metallic layer is applied onto a top side of a base substrate,
- b. an infrared transmission means and/or infrared receiver means is/are arranged on the top side of the base substrate and within the first frame-shaped metallic layer,
- c. a cover substrate is arranged on the top side of the base substrate which covers the area within the first frame-shaped metallic layer and which has at least one area configured to be transparent to light, in particular, transparent to infrared light wherein a second frame-shaped metallic layer corresponding to the first frame-shaped metallic layer is provided at the cover substrate, and
- d. the first frame-shaped metallic layer is connected to the second frame-shaped metallic layer non-releasably such that the base substrate, the cover substrate, and the frame-shaped metallic layers together form a substantially hermetically sealed housing of the implant.

Hermetically sealed means that the housing is air-tight, and/or water-tight, or moisture-tight to a large extent or completely such that no malfunctions of the implant due to moisture will occur during the intended operating period which may be several years or decades.

Because the infrared transmission means and/or infrared receiver means is/are arranged in the interior of the housing, the production of an implant may be facilitated substantially because apertures in the housing wall for data communication can be omitted such that during the production of an implant no measures have to be taken in order to close such apertures in an air-tight or water-tight manner.

Between the first frame-shaped metallic layer and the second frame-shaped metallic layer, a circumferential frame,

preferably a metal frame, may be arranged wherein the circumferential frame is connected to the two metallic layers non-releasably.

The area configured to be transparent to light can be formed by a cover by means of which an opening in the cover substrate can be closed.

In an embodiment of the invention, the cover substrate may be configured such that the transparent area has a lower thickness than the remaining area of the cover substrate.

It is advantageous if for the transparent area, ceramics, in particular, aluminum oxide or zirconium oxide in amorphous, crystalline and/or partially crystalline form, high temperature multi-layer ceramics with an aluminum oxide proportion, or a glass or glass ceramics is/are used.

At least one sensor, in particular, a moisture sensor, and/or a temperature sensor, and/or the pressure sensor may be arranged within the interior of the housing which is/are coupled operatively to the infrared transmission means and/or infrared receiver means.

Alternatively or additionally, a magnet may be arranged within the interior of the housing, in particular, a permanent magnet which may cooperate with a magnet of an external transceiver unit which can be arranged outside of the housing.

Alternatively or additionally, the housing may be wrapped by an induction coil which is provided as inductive receiver coil for an inductive energy transmission. Preferably, an induction coil having a very high quality is provided for this. It is advantageous if the induction coil is only used for the energy transmission but not for a wireless data transmission.

Further, additionally or alternatively, a desiccant may be arranged within the interior of the housing.

Further, a system is provided by the invention comprising a medical implant for a human or animal organism, in particular, an implant according to the invention, and a transceiver unit wherein the transceiver unit cooperates with an infrared transmission means and/or infrared receiver means of the implant. The transceiver unit may comprise an infrared transmission means and/or an infrared receiver means. The infrared transmission means and/or infrared receiver means of the implant and the infrared transmission means and/or infrared receiver means of the transceiver unit may be coupled operatively through an area of the housing of the implant configured to be transparent to light, in particular, transparent to infrared light.

BRIEF DESCRIPTION OF THE DRAWINGS

Further details and features of the invention as well as concrete embodiments of the invention can be derived from the following description in connection with the drawing in which

FIG. 1 shows the steps of the production method of a medical implant according to a first embodiment;

FIG. 2 shows the steps of the production method of an implant according to the invention according to a second embodiment;

FIG. 3 shows a diagram from which the relative transmission of infrared radiation with respect to the wavelength of the infrared rays and the materials used can be derived;

FIG. 4 shows a schematic assembly of a medical implant according to the invention;

FIG. 5 shows five different design variants of a medical implant according to the invention; and

FIG. 6 shows four further design variants of a medical implant according to the present invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

According to the present invention, the communication between a medical implant and a transceiver unit which may be arranged exterior to the body is effected on the basis of light or infrared light wherein the communication can be carried out in a bidirectional manner. In order to enable this, at least a part of the implant housing is configured to be transparent to light or infrared light.

The communication of implants with the outside world, for example, with a transceiver unit arranged outside of the body, is necessary, on the one hand, to check the functionality and the condition of the implant. For this, no high bandwidths or information transmission rates are required.

On the other hand, the communication or transmission of physiological data is necessary for various diagnostic and therapeutic applications. Such data are, for example, blood pressure, temperature, hormone or other messenger material concentrations, or the electrical activity of nerves or muscles. The data transmission on the basis of light or infrared light, hereby, has found to be particularly advantageous because these data can be transmitted with high-performance, i.e., with a high information content, in an energy-saving and secure manner, i.e., with low error/loss rates such that these data are usable for clinical purposes.

Vice versa, also the communication of the outer world, for example, of a transceiver unit arranged outside of the body, with the implant is possible. Thereby, for example, the implant may be switched on or off, or new functional modes can be notified to the implant. For this, no high bandwidths or information transmission rates are necessary.

According to the invention, it is also possible to perform a lasting up to a continuous communication in order to react flexible and fast during therapeutic applications. For example, thereby the supply of substances can be controlled fast and independent of a condition, micro-pumps can be controlled according to the demand, or an electric stimulation of nerves and muscles can be realized fast and according to the demand. For example, the neural stimulation with respect to Parkinson patients according to the demand, or the reactive stimulation with respect to epilepsy patients is possible in case an imminent seizure is measured.

Contrary to a reaction mode determined in the interior of the implant, control from the outside brings along two substantial advantages. A first advantage is that a physician or the patient himself may adapt the activity of the implant at any time. For example, the patient may adapt the effect of the implant by direct control of the exterior transmission unit immediately. A second advantage is that the activity of the implant may be controlled by means of information from the exterior. For example, the activity of an optical prosthesis can be controlled automatically up and down by means of the intensity of light (inside/outside, day/night).

FIG. 1 and FIG. 2 show the essential method steps of two methods for the production of the medical implant according to the invention. The first two method steps S1, S2 in the production method according to the first variant (FIG. 1) are identical to the two first method steps S1, S2 of the production method according to a second variant according to the invention (FIG. 2).

In a first step S1, a metallic layer or a metallization layer is applied onto the top side O of the base substrate 10 which basically forms a first frame-shaped metallic layer 20. The

first frame-shaped metallic layer **20** serves as solder base for further elements of the housing of the medical implant.

In the subsequent production step **S2**, all electronic components are arranged on the top side **O** of the base substrate **10** and within the first frame-shaped metallic layer **20** and are fixed to the base substrate **10**. The electronic components, here, comprise the circuit board **30** and an infrared transmission means and/or infrared receiver means **40** arranged on the circuit board **30** wherein the infrared transceiver unit, here, comprises an infrared diode. Further electronic components, for example, sensors, for example, temperature sensors, moisture sensors, or pressure sensors, may be arranged on the circuit board **30**, as will be further explained with reference to FIG. **4**.

In a third step **S3.1** of the production method according to the first variant shown in FIG. **1**, a cover substrate **12** is arranged on the top side **O** of the base substrate **10**. The cover substrate **12** covers the area within the first frame-shaped metallic layer **20**. At the cover substrate **12** or at the lower side of the cover substrate **12**, a second frame-shaped metallic layer **22** is provided which corresponds to the first frame-shaped metallic layer **20** of the base substrate **10**. Between the first frame-shaped metallic layer **20** and the second frame-shaped metallic layer **22** additionally a circumferential frame **50** is arranged which basically forms the sidewall of the implant housing. The circumferential frame **50** may be made from a metal.

In a further step **S4.1** of the first variant of the production method, the circumferential frame **50** is placed onto the first circumferential metallic layer **20**. Subsequently, the cover substrate **12** is placed onto the second circumferential layer **22** such that the second circumferential layer **22** rests on the circumferential frame **50**. Subsequently, the circumferential frame **50** is connected to the two metallic layers **20**, **22** in a non-releasable manner, resulting, for example, from soldering the two metallic layers **20**, **22** to the circumferential frame **50**. In FIG. **1**, the soldering tin **60** is applied in the area between the two circumferential layers **20**, **22**.

Thereby, a closed housing system is formed which is substantially air- and moisture-tight, and in the interior of which all electronic components, in particular, the infrared receiver or transmission units are arranged.

The cover substrate **12** is at least partially configured to be transparent to light or infrared light in order to allow for a communication by means of infrared radiation through the housing using an external transceiver unit. Possible embodiments of an area of a housing wall which is transparent to light or infrared light will be explained in further detail with respect to FIG. **5** and FIG. **6**.

FIG. **2** shows a second variant of the production method according to the invention wherein the production steps **S1** and **S2** are identical to the production method shown in FIG. **1**.

In a third step **S3.2** of the second variant of the production method shown in FIG. **2**, a cover substrate **12** which here is configured as a half-shell is arranged at the top side of the base substrate **12** such that the rim of the half-shell rests on the circumferential metallic layer **20** of the base substrate **10**. The circumferential metallic layer **22** is provided at the external sidewall of the half shell **12** which extends up to the rim of the half shell and thereby comes into contact with the circumferential metallic layer **20** during placing the half shell on the base substrate **12**.

In of fourth step **S4.2** of the second production variant, the first frame-shaped metallic layer **20** is connected to the second frame-shaped metallic layer **22** non-releasably, for example, by means of a solder method. The soldering tin **60**

can be seen in FIG. **2**. The cover substrate **12** or the half shell is configured to be transparent to light or infrared light in an area as will be further described with reference to FIG. **5** and FIG. **6**.

In order to configure the cover substrate to be transparent to light or infrared light, different materials may be used for the area of the cover substrate which is transparent to light or infrared light. For example, different ceramics may be used with different thicknesses as substrate material for the cover substrate. Examples of such ceramics are, for example, aluminum oxide Al_2O_3 in amorphous form (Rubalit), in crystalline form (sapphire), or in semi-crystalline form. Alternatively, also glass and glass ceramics can be used. Further, also zirconium oxide ZrO_2 or high temperature multi-layer ceramics (HTCC) with a varying proportion of aluminum oxide Al_2O_3 can be used for the production of the areas which are transparent to light or infrared light.

By adapting the thickness or strength of the substrate material in the area which is transparent to light or infrared light, the infrared transmission, i.e., the transparency for infrared radiation, can be varied.

With respect to the production methods shown with respect to FIG. **1** and FIG. **2**, also a production step not shown here may be provided according to which the housing is wrapped by an electrical conductor which forms an induction coil for inductive energy transmission.

FIG. **3** shows the relative transmission of infrared light through various materials depending on the wavelength of the infrared light and on the material used wherein the specifications of the relative transmission with respect to the single materials are referred to a wavelength of the infrared radiation between 850 nm and 900 nm.

In the diagram shown in FIG. **3**, the relative transmission for Rubalit, sapphire, and a high temperature multi-layer ceramic (HTCC) is shown for respectively different thicknesses. Further, in the diagram of FIG. **3**, also the relative transmission for aluminum with a thickness of 2 mm, for Parylene C with a thickness of 15 μm , and for polydimethylsiloxane PDMS (MED-1000) with a thickness of 300 μm is plotted.

As can be seen from FIG. **3**, the infrared transparency can be increased in that the respective material is made thinner. Further, the materials are the more transparent to infrared radiation the more crystalline the material is, as is also visible in FIG. **3**.

For air- or moisture-tight encapsulation of the housing, materials which can be soldered, for example, copper, or copper foil are suitable. Also possible are hermetic housings from titanium or stainless steel wherein in these housings, an area transparent to light or infrared light has to be provided (for example, sapphire, ruby, diamond, or a similar solid crystal or gemstone which is transparent to light or infrared light, or similar ceramics which are transparent to light or infrared light) has to be provided, as shown, for example, with reference to FIG. **5**.

As soldering tin for non-releasable connection of the cover to the bottom of the housing, all conventional alloys can be used wherein however, lead-free materials are preferable.

Further, it may be necessary to cast the housing in a medical elastomer or to coat the housing with a medical elastomer. For this, conventional medical silicones may be used, for example, polydimethylsiloxane. Alternatively or additionally, the housing can be coated or encapsulated for this by a polymer, for example, Parylene C.

The infrared transmission properties are influenced by the polydimethylsiloxane as well as by Parylene C only insignificantly, as can be seen from FIG. 3.

FIG. 4 shows a system according to the invention which comprises a medical implant **1** and an external transceiver unit **100**. The communication between the implant **1** and the external transceiver unit **100** is effected on the basis of infrared radiation. The cover substrate **12** of the implant **1** is configured to be at least partially transparent to light or infrared light for this such that an infrared data transmission IR between the implant **1** and the external transceiver unit **100** is possible.

The implant **1** shown in FIG. 4 has been produced according to the production method shown in FIG. 2. Prior to closing the housing in steps S3.2 or S4.2, magnets **70** have been arranged in the interior of the housing which are configured as permanent magnets. The external transceiver unit **100** which comprises an infrared transmitter and/or infrared receiver **40b** also has magnets or permanent magnets **71** which correspond to the magnets **70** of the implant **1**. Thereby, an alignment of the external transceiver unit **100** with respect to the implanted implant **1** can be supported. Also shown in FIG. 4 is the magnetic field MF formed between the respective magnets.

Further, prior to closing the housing, a number of sensors **80** can be arranged in the interior of the housing in steps S3.2 or S4.2. For example, a moisture sensor, a temperature sensor and/or a pressure sensor may be provided. The sensors are coupled to the infrared transceiver means **40** of the implant **1** such that the sensor values of the sensors can be transmitted by means of IR communication to the external transceiver unit **100**.

The magnet **70** and the sensors **80** may also be arranged in the interior of the housing in the steps S3.1 and S4.1 according to the production method shown in FIG. 1.

The moisture in the interior of the implant housing can be checked in regular intervals by means of a moisture sensor which preferably has a very low drift. In case the sensor value of the moisture sensor exceeds a critical value, this can be indicated to the user such that a replacement of the implant due to safety reasons is suggested to the user. Thereby, it is possible to leave the implant in the body of the patient as long as possible. The merely prophylactic replacement of an implant, thus, can be prevented.

For the extension of time in which the moisture within the implant housing is very low and thereby allows for a reliable operation of the electronic components arranged within the housing interior, desiccants can be introduced into the housing which bind the water entering into the interior of the housing up to a certain amount chemically or physically such that they cannot contribute to an increase of the air moisture within the interior of the housing. For this, so called getter materials can be provided. The desiccant or the getter material may be applied onto the housing wall wherein the infrared transmission is effected through the substrate material and the desiccant or the getter material.

The temperature sensor may be provided in order to further increase the reliability of the electronics within the housing. The temperature sensor may, for example, be used in order to prevent a thermal overload of the implant or a not intended heating of the tissue surrounding the implant. In case the temperature exceeds a predetermined value, counter measures can be initiated by the implant. For example, the functioning of the implant can be reduced to a minimum function. The measured temperature values can be transmitted also by means of IR communication to the external transceiver unit **100**. Upon frequent exceeding of certain

temperature values, a replacement of the implant may be proposed to the patient or to the user.

FIG. 5 shows five variants of a medical implant for a human or animal organism according to the invention.

With respect to the variants in (a), (c), and (d), the cover substrate **12** has an opening **17** which is closed by a cover **15** wherein the cover **15** is configured to be transparent to light or infrared light. As materials for the cover **15**, the materials mentioned above can be used. The cover substrate **12** does not have to be configured to be transparent to light or infrared light in these embodiments.

The cover **115** is soldered onto the cover substrate **12** wherein a metallic layer is applied onto the cover substrate **12** and in the rim-sided region of the cover **15** depending on the material used for the cover substrate **12** in order to allow a soldering of the cover substrate **12** to the cover **15**. In the variant (a), corresponding metallic layers are applied to the cover substrate **12** as well as to the cover **15**. With respect to the variant (c), corresponding metallic layers are only applied on the cover **15** because according to this variant, the cover substrate is configured metallically. Also, according to the variant (d), a corresponding metallic layer is also only provided on the cover **15**.

With respect to the variant (d), the cover substrate **12** as well as the base substrate **10** is metallic.

According to variant (b1), the housing is made as one piece wherein the entire housing **10, 12** comprises a material transparent to light or infrared light.

The variant (b2) differs from the variant according to (b1) in that an electrical shielding is applied to the inner walls of the housing, for example, a metal foil wherein the shielding comprises an area which is transparent to light or infrared light. The area of the shielding **25** which is transparent to light or infrared light may be realized by a recess in the metal foil.

The metallic shielding shown in the variant (b2) may be provided for all variants shown in FIG. 5 and FIG. 6.

FIG. 6 shows four further variants of a medical implant according to the invention.

With respect to the variants (e), (f), and (g), the cover substrate **12** is made thinner in the area in which the cover substrate is to be configured transparent to light or infrared light than in the remaining area of the cover substrate. The thickness or strength of the area of the cover substrate which is transparent to light or infrared light may be selected depending on the selected substrate material, as shown with respect to the diagram in FIG. 3.

With respect to the variant (h), the electronic components or the infrared transceiver means **40** of the implant are not arranged on the base substrate **10** but rather on the interior bottom of a cover substrate **12** which is half-shell shaped. In this case, the base substrate **10** has to be configured to be transparent to light or infrared light at the corresponding locations, as shown with reference to the variants (a) to (g) of FIG. 5 and FIG. 6.

REFERENCE NUMERALS

- 1** medical implant
- 10** substrate (base substrate) as part of the housing
- 12** substrate (cover substrate) as part of the housing
- 15** cover for an opening in the housing wall
- 17** opening in the housing wall (aperture)
- 20** first frame-shaped metallic layer on the base substrate
- 22** second frame-shaped metallic layer on the cover substrate
- 25** electric current shielding, for example, metal foil

11

30 circuit board (electronic circuit board)
 40 infrared transmission means and/or infrared receiver means of the implant
 40*b* infrared transmission means and/or infrared receiver means of the external transceiver unit
 50 circumferential frame, preferably metal frame, as part of the housing
 60 non-releasable connection between the first and second frame-shaped metallic layers or between the frame-shaped metallic layers and the metal frame, preferably, soldering tin
 70 magnet or permanent magnet in the implant
 71 magnet or permanent magnet at the external infrared transceiver unit
 80 sensor, for example, moisture sensor and/or temperature sensor and/or pressure sensor
 100 external R transceiver unit
 A portion of the housing wall in which the area being transparent to light is located
 HTCC high temperature multi-layer ceramics (High Temperature Cofired Ceramics)
 IR infrared data transmission
 MF magnetic field
 O top side of the base substrate
 S1 first step of the production method
 S2 second step of the production method
 S3.1 third step of the production method according to a first variant
 S3.2 third step of the production method according to a second variant
 S4.1 fourth step of the production method according to a first variant
 S4.2 fourth step of the production method according to a second variant
 What is claimed is:

1. A method for the production of a medical implant for a human or animal organism comprising: a housing with a housing wall which comprises an area configured to be transparent to light, and an infrared transmission means or infrared receiving means arranged in an interior of the housing, wherein the area configured to be transparent to light has a lower thickness than a remaining area of the housing, the method comprising:
 - applying a first metallic circumferential frame layer on a top side of a base substrate;
 - arranging the infrared transmission means or infrared receiver means on the top side of the base substrate and within the first metallic circumferential frame layer;
 - arranging a cover substrate on the top side of the base substrate which covers an area within the first metallic circumferential frame layer and which has the area configured to be transparent to light;
 - providing a second metallic circumferential frame layer corresponding to the first metallic circumferential frame layer at the cover substrate;
 - connecting the first metallic circumferential frame layer to the second metallic circumferential frame layer non-releasably such that the base substrate, the cover substrate, and the metallic circumferential frame layers together form the housing, wherein said housing is a substantially hermetically closed housing of the implant; and
 - arranging a circumferential frame between the first metallic circumferential frame layer and the second metallic circumferential frame layer, and the frame is connected to the two metallic circumferential frame layers non-releasably.

12

2. The method of claim 1 wherein the area of the medical implant configured to be transparent to light comprises aluminum oxide Al_2O_3 in amorphous, or partially crystalline form, or zirconium oxide ZrO_2 in amorphous or partially crystalline form, or high temperature multi-layer ceramics having an aluminum oxide proportion.
3. The method of claim 1, wherein the area of the medical implant configured to be transparent to light is formed by a cover which closes an opening in the housing wall.
4. The method of claim 1, wherein at least one sensor or a temperature sensor is arranged in the interior of the housing of the medical implant which is coupled operatively to the infrared transmission means or infrared receiver means.
5. The method of claim 1, wherein at least one magnet is arranged within the interior of the housing of the medical implant which can cooperate with a magnet of an external transceiver unit which can be arranged outside of the housing.
6. The method of claim 1, wherein the medical implant has an induction coil which can be coupled inductively to an inductive transmission unit which can be arranged outside of the human or animal organism in order to transmit energy from the inductive transmission unit to the implant.
7. The method of claim 6, wherein the induction coil comprises an electrical conductor which can be wrapped around the housing of the implant.
8. The method of claim 1, wherein a desiccant is provided in the interior of the housing.
9. The method of claim 1, wherein the area transparent to light comprises:
 - aluminum oxide Al_2O_3 in amorphous, or partially crystalline form, or zirconium oxide ZrO_2 in amorphous, or partially crystalline form, or high temperature multi-layer ceramics, HTCC, with an aluminum oxide proportion.
10. A method for the production of a medical implant for a human or animal organism comprising: a housing with a housing wall which comprises an area configured to be transparent to light, and an infrared transmission means or infrared receiving means arranged in an interior of the housing, wherein the area configured to be transparent to light has a lower thickness than a remaining area of the housing, the method comprising:
 - applying a first metallic circumferential frame layer on a top side of a base substrate,
 - arranging an infrared transmission means or infrared receiver means on the top side of the base substrate and within the first metallic circumferential frame layer,
 - arranging a cover substrate on the top side of the base substrate which covers an area within the first metallic circumferential frame layer and which has the area configured to be transparent to light,
 - providing a second metallic circumferential frame layer corresponding to the first metallic circumferential frame layer at the cover substrate, and
 - connecting the first metallic circumferential frame layer to the second metallic circumferential frame layer non-releasably such that the base substrate, the cover substrate, and the metallic circumferential frame layers together form the housing, said housing being a substantially hermetically closed housing of the implant, wherein the area configured to be transparent to light is formed by a cover by means of which an opening in the cover substrate is closed.

11. A method for the production of a medical implant for a human or animal organism comprising: a housing with a housing wall which comprises an area configured to be transparent to light, and an infrared transmission means or infrared receiving means arranged in an interior of the housing, wherein the area configured to be transparent to light has a lower thickness than a remaining area of the housing, the method comprising

- applying a first metallic circumferential frame layer on a top side of a base substrate, 10
- arranging an infrared transmission means or infrared receiver means on the top side of the base substrate and within the first metallic circumferential frame layer,
- arranging a cover substrate on the top side of the base substrate which covers an area within the metallic circumferential frame layer and which has the area configured to be transparent to light, 15
- providing a second metallic circumferential frame layer corresponding to the first metallic circumferential frame layer at the cover substrate, and 20
- connecting the first metallic circumferential frame layer to the second metallic circumferential frame layer non-releasably such that the base substrate, the cover substrate, and the metallic circumferential frame layers together form the housing, wherein said housing is a substantially hermetically closed housing of the implant, 25

wherein the cover substrate is configured such that the area transparent to light has a lower thickness than a remaining area of the cover substrate. 30

* * * * *

专利名称(译)	医疗植入物及其制造方法		
公开(公告)号	US10251286	公开(公告)日	2019-04-02
申请号	US14/629454	申请日	2015-02-23
[标]申请(专利权)人(译)	科塔克公司		
申请(专利权)人(译)	CORTEC GMBH ALBERT - 路德维希安大学弗莱堡		
当前申请(专利权)人(译)	CORTEC GMBH		
[标]发明人	RICKERT JORN KOHLEFABIAN SCHUTTLER MARTIN		
发明人	RICKERT, JORN KOHLEFABIAN SCHUTTLER, MARTIN		
IPC分类号	H05K5/02 B23K1/20 H04Q9/14 A61B5/00 B23K1/00 H05K5/00		
CPC分类号	H05K5/02 A61B5/0031 A61B5/686 B23K1/0008 B23K1/20 H04Q9/14 H05K5/0239 H05K5/0247 H05K5/0004 A61B2562/0271 A61B2560/0219 A61B2562/029 A61B2562/0247		
代理机构(译)	MYERS沃林有限责任公司		
其他公开文献	US20150173215A1		
外部链接	Espacenet		

摘要(译)

公开了一种用于医疗植入物的壳体，用于人体或动物有机体的医疗植入物，用于制造医疗植入物的方法，以及包括医疗植入物和可以连接到医疗植入物的收发器单元的系统。

