



US009918618B2

(12) **United States Patent**
Molnar

(10) **Patent No.:** **US 9,918,618 B2**
(45) **Date of Patent:** ***Mar. 20, 2018**

(54) **MEDICAL DEVICES AND METHODS OF PLACEMENT**

(71) Applicant: **WM & DG, INC.**, Deerfield, IL (US)

(72) Inventor: **Robert W. Molnar**, Long Grove, IL (US)

(73) Assignee: **WM & DG, Inc.**, Deerfield, IL (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/455,470**

(22) Filed: **Aug. 8, 2014**

(65) **Prior Publication Data**

US 2016/0038008 A1 Feb. 11, 2016

(51) **Int. Cl.**

A61B 1/00 (2006.01)

A61B 1/07 (2006.01)

A61B 7/02 (2006.01)

A61B 1/233 (2006.01)

A61B 1/24 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 1/00154** (2013.01); **A61B 1/0014** (2013.01); **A61B 1/00016** (2013.01); **A61B 1/00135** (2013.01); **A61B 1/00137** (2013.01); **A61B 1/00142** (2013.01); **A61B 1/05** (2013.01); **A61B 1/07** (2013.01); **A61B 1/233** (2013.01); **A61B 1/24** (2013.01); **A61B 1/2673** (2013.01); **A61B 1/303** (2013.01); **A61B 7/023** (2013.01); **A61M 16/0463** (2013.01); **A61M 16/0465** (2013.01); **A61M 16/0488** (2013.01); **A61M 16/0666** (2013.01); **A61B 1/00078** (2013.01); **A61B 1/015** (2013.01); **A61B 1/018** (2013.01); **A61B 5/0008** (2013.01); **A61B 5/01** (2013.01)

(58) **Field of Classification Search**

CPC **A61B 1/00009**; **A61B 1/00016**; **A61B 1/00114**; **A61B 1/00154**; **A61B 1/015**

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,231,365 A 11/1980 Scarberry
4,360,008 A 11/1982 Corazzelli, Jr.
(Continued)

FOREIGN PATENT DOCUMENTS

EP 0 665 029 A2 8/1995
KR 2012-0095385 8/2012
(Continued)

OTHER PUBLICATIONS

Bledsoe, "The Disappearing Endotracheal Tube", Clinical Professor of Emergency Medicine, University of Nevada School of Medicine.

"Incubation Threatened by New Devices and Lack of Paramedic Practice", Patient Care, Jems.com; <http://www.jems.com/article/patient-care/incubation-threatened-new-devi>.

"Incubation Threatened by New Devices and Lack of Paramedic Practice", Patient Care; <http://www.jems.com/article/patient-care/intubation-threatened-new-devi>.

(Continued)


Primary Examiner — Baisakhi Roy

(74) *Attorney, Agent, or Firm* — Greer, Burns & Crain, Ltd.

(57) **ABSTRACT**

The present invention provides improved medical devices equipped with a visualization device for intubation, ventilation, drug delivery, feeding and continuous remote monitoring of a patient. The present invention also provides methods for rapid and accurate placement of a medical device in a patient and continuous real time monitoring, including a remote monitoring, of the patient after the placement.

22 Claims, 30 Drawing Sheets

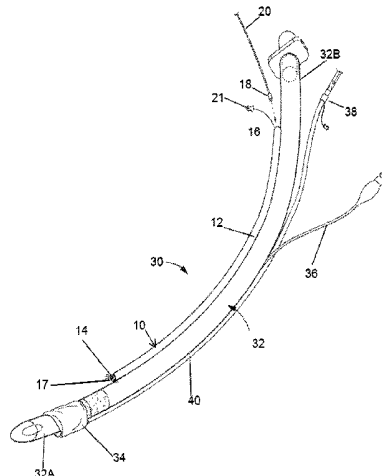

Page 2

(51)	Int. Cl.			7,896,007	B2	3/2011	Brain		
	A61B 1/267	(2006.01)		7,921,847	B2	4/2011	Totz		
	A61B 1/303	(2006.01)		7,942,813	B2	5/2011	Mackin		
	A61M 16/04	(2006.01)		7,976,458	B2	7/2011	Stefanchik et al.		
	A61M 16/06	(2006.01)		8,016,760	B2	9/2011	Chalana et al.		
	A61B 1/05	(2006.01)		8,038,629	B2	10/2011	Solanki et al.		
	A61B 1/015	(2006.01)		8,202,215	B2	6/2012	Xiao et al.		
	A61B 1/018	(2006.01)		8,215,307	B2	7/2012	Nasir		
	A61B 5/01	(2006.01)		8,297,275	B2	10/2012	Ogilvie et al.		
	A61B 5/00	(2006.01)		8,308,644	B2	11/2012	McMorrow et al.		
			8,371,303	B2	2/2013	Schaner et al.			
			8,529,442	B2 *	9/2013	Pacey		A61B 1/00142	
(56)	References Cited			8,928,746	B1 *	1/2015	Stevrin		G02B 23/2461
	U.S. PATENT DOCUMENTS								348/68
				9,211,060	B2	12/2015	Waldron et al.		
				9,415,179	B2 *	8/2016	Molnar		A61B 7/003
	4,577,638	A	3/1986	Graham	9,427,142	B2	8/2016	Terliuc	
	4,584,998	A	4/1986	McGrail	9,579,012	B2	2/2017	Vazales et al.	
	4,607,643	A	8/1986	Bell et al.	2003/0220542	A1	11/2003	Belson et al.	
	5,052,386	A	10/1991	Fischer, Jr.	2005/0182297	A1	8/2005	Gravenstein et al.	
	5,193,692	A	3/1993	Farley et al.	2006/0111633	A1	5/2006	McMorrow et al.	
	5,241,956	A	9/1993	Brain	2006/0149129	A1	7/2006	Watts et al.	
5,353,787	A	10/1994	Price	2006/0162730	A1	7/2006	Glassenberg et al.		
5,400,771	A	3/1995	Pirak et al.	2006/0180155	A1	8/2006	Glassenberg et al.		
5,499,625	A	3/1996	Frass et al.	2006/0276694	A1	12/2006	Acha Gandarias		
5,511,916	A	4/1996	Farley et al.	2007/0137651	A1	6/2007	Glassenberg et al.		
5,513,627	A	5/1996	Flam	2007/0156068	A1	7/2007	Dubey		
5,515,844	A *	5/1996	Christopher		A61M 16/10	2007/0180887	A1	8/2007	Frenken
					128/200.26	2007/0203393	A1	8/2007	Stefanchik
5,551,947	A	9/1996	Kaali			2007/0239197	A1	10/2007	Dubey
5,632,271	A	5/1997	Brain			2007/0255185	A1	11/2007	Dubey
5,682,880	A	11/1997	Brain			2008/0029100	A1	2/2008	Glassenberg et al.
5,733,242	A *	3/1998	Rayburn		A61B 1/0052	2008/0114268	A1	5/2008	Dubey
					600/120	2008/0146879	A1 *	6/2008	Pacey
									A61B 1/05
5,740,791	A	4/1998	Aves						600/188
5,819,733	A	10/1998	Bertram			2008/0188774	A1	8/2008	Dubey
5,879,306	A *	3/1999	Fontenot		A61B 5/0086	2008/0276932	A1	11/2008	Bassoul
					600/473	2009/0194114	A1	8/2009	Chen et al.
5,888,195	A	3/1999	Schneider			2009/0227835	A1	9/2009	Terliuc
6,142,144	A	11/2000	Pacey			2010/0051024	A1 *	3/2010	Abrons
6,189,533	B1	2/2001	Simon et al.						A61M 16/0488
6,196,225	B1	3/2001	Allgeyer						128/200.26
6,349,720	B1	2/2002	Clark			2010/0113916	A1	5/2010	Kumar
6,386,199	B1	5/2002	Alfery			2010/0249639	A1	9/2010	Bhatt
6,439,232	B1	8/2002	Brain			2010/0261967	A1	10/2010	Pacey et al.
6,440,061	B1	8/2002	Wenner et al.			2010/0312069	A1 *	12/2010	Sutherland
6,443,156	B1	9/2002	Niklason et al.						A61B 17/0218
6,527,704	B1	3/2003	Chang et al.			2011/0030694	A1	2/2011	Schaner et al.
6,543,447	B2 *	4/2003	Pacey		A61B 1/05	2011/0178372	A1	7/2011	Pacey et al.
					128/200.26	2011/0201882	A1	8/2011	Schwartz et al.
6,626,169	B2	9/2003	Gaitini			2011/0315147	A1	12/2011	Wood et al.
6,631,720	B1	10/2003	Brain			2012/0059223	A1 *	3/2012	McGrath
6,634,354	B2	10/2003	Christopher						A61B 1/267
6,655,377	B2 *	12/2003	Pacey		A61B 1/2676	2012/0259173	A1 *	10/2012	Waldron
					128/200.26				A61B 1/00073
									600/109
6,860,264	B2	3/2005	Christopher			2012/0260921	A1	10/2012	Sangwan
6,860,270	B2	3/2005	Sniadach			2012/0302833	A1	11/2012	Hayman et al.
6,918,391	B1	7/2005	Moore			2013/0006051	A1	1/2013	Stace et al.
7,052,456	B2	5/2006	Simon			2013/0030249	A1	1/2013	Vazales et al.
7,128,509	B2	10/2006	Farley et al.			2013/0197303	A1 *	8/2013	Chun
7,156,091	B2	1/2007	Koyama et al.						A61M 16/06
7,237,993	B2	7/2007	Farley et al.						600/103
7,331,925	B2	2/2008	McMorrow et al.			2013/0253368	A1	9/2013	Are et al.
7,421,877	B2	9/2008	Frenken			2013/0324798	A1	12/2013	Molnar et al.
7,450,746	B2	11/2008	Yang et al.			2014/0018626	A1	1/2014	Lee
7,520,857	B2	4/2009	Chalana et al.			2014/0166020	A1	6/2014	Chang
7,527,601	B2	5/2009	Dubey et al.			2014/0194694	A1	7/2014	Chen
7,611,466	B2	11/2009	Chalana et al.			2014/0357951	A1 *	12/2014	Muller
7,654,970	B2	2/2010	Dubey						G02B 23/2415
7,713,189	B2	5/2010	Hanke			2016/0038014	A1	2/2016	Molnar
7,713,216	B2	5/2010	Dubey et al.						600/111
7,727,150	B2	6/2010	Chalana et al.						
7,744,534	B2	6/2010	Chalana et al.						
7,749,165	B2	7/2010	McMorrow et al.			WO	94/05200	3/1994	
7,749,176	B2	7/2010	Dubey			WO	03/084719	A2	10/2003
7,811,239	B2	10/2010	Dubey et al.			WO	WO 2008/123934	A1	10/2008
7,819,806	B2	10/2010	Yang et al.			WO	2009025843	A1	2/2009
7,854,324	B2	12/2010	Farley et al.			WO	2010/120950		10/2010
				</					

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	2012/080293 A2	6/2012
WO	2013/017535 A2	2/2013
WO	WO2015013172 A2	1/2015

OTHER PUBLICATIONS

“Continuous Airway Control”; Vivasight.

Genzwuerker, MD. et al. “Laryngeal tube: a review of current literature” AJA-Online.com 2011:vol. 12.

Kidali MD, “Capnography in emergency medicine—911” <http://www.capnography.com/outside/922.htm>.

VivaSight, Airway management for lung isolation, ETVIEW.

ETView Medical, Ltd., Announces Exclusive Patent License Agreement—Feb. 22, 2012. ETVIEW.

ETVIEW, http://www.etview.com/index_old.php.

VivaSight-SL, ETVIEW.

How to Use a Jem Endotracheal Tube Changer.

ETView Medical, Ltd., Announces Exclusive Patent License Agreement—Feb. 2, 2012, http://worldnetdaily.com.uk/markets/news/read/20671060/etview_medical, Jul. 5, 2012.

ETView Medical, Ltd., Announces the Appointment of David Amar, MD to Its Scientific Advisory Board, 2012; <http://finance.yahoo.com/news/etview-medical-ltd-announces-appointment-104300770.html>, Jun. 4, 2012, 3 pages.

* cited by examiner

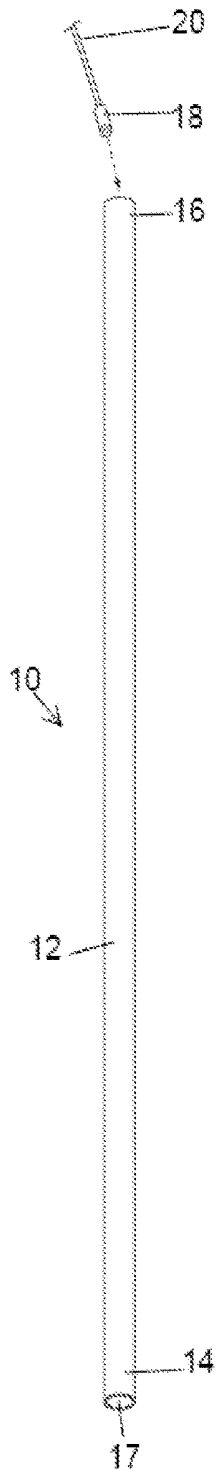


FIG. 1A

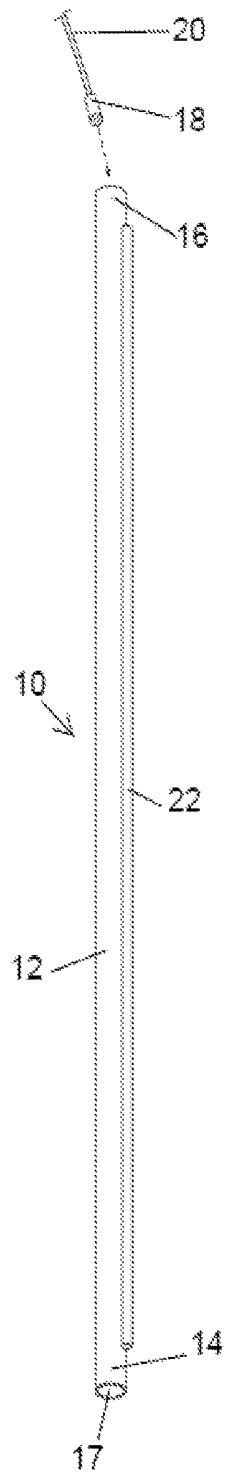


FIG. 1B

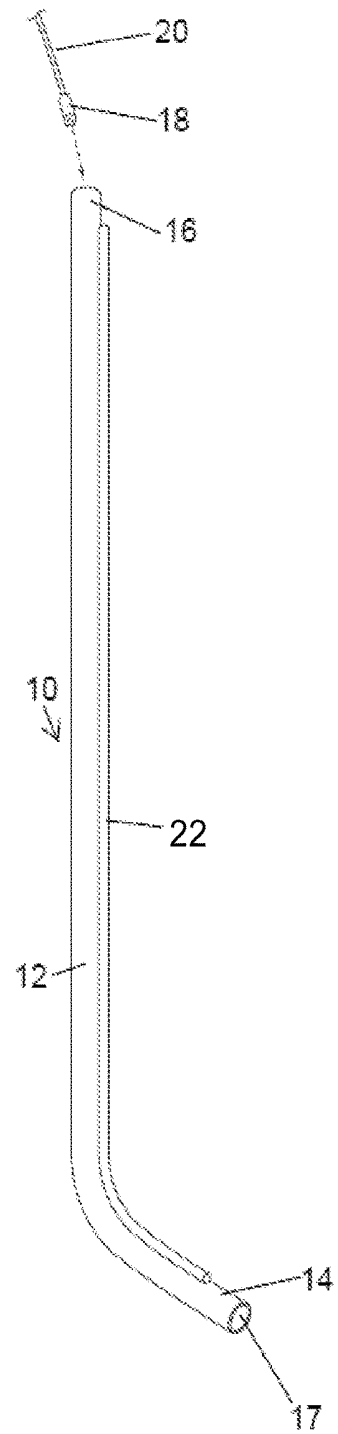


FIG. 1C

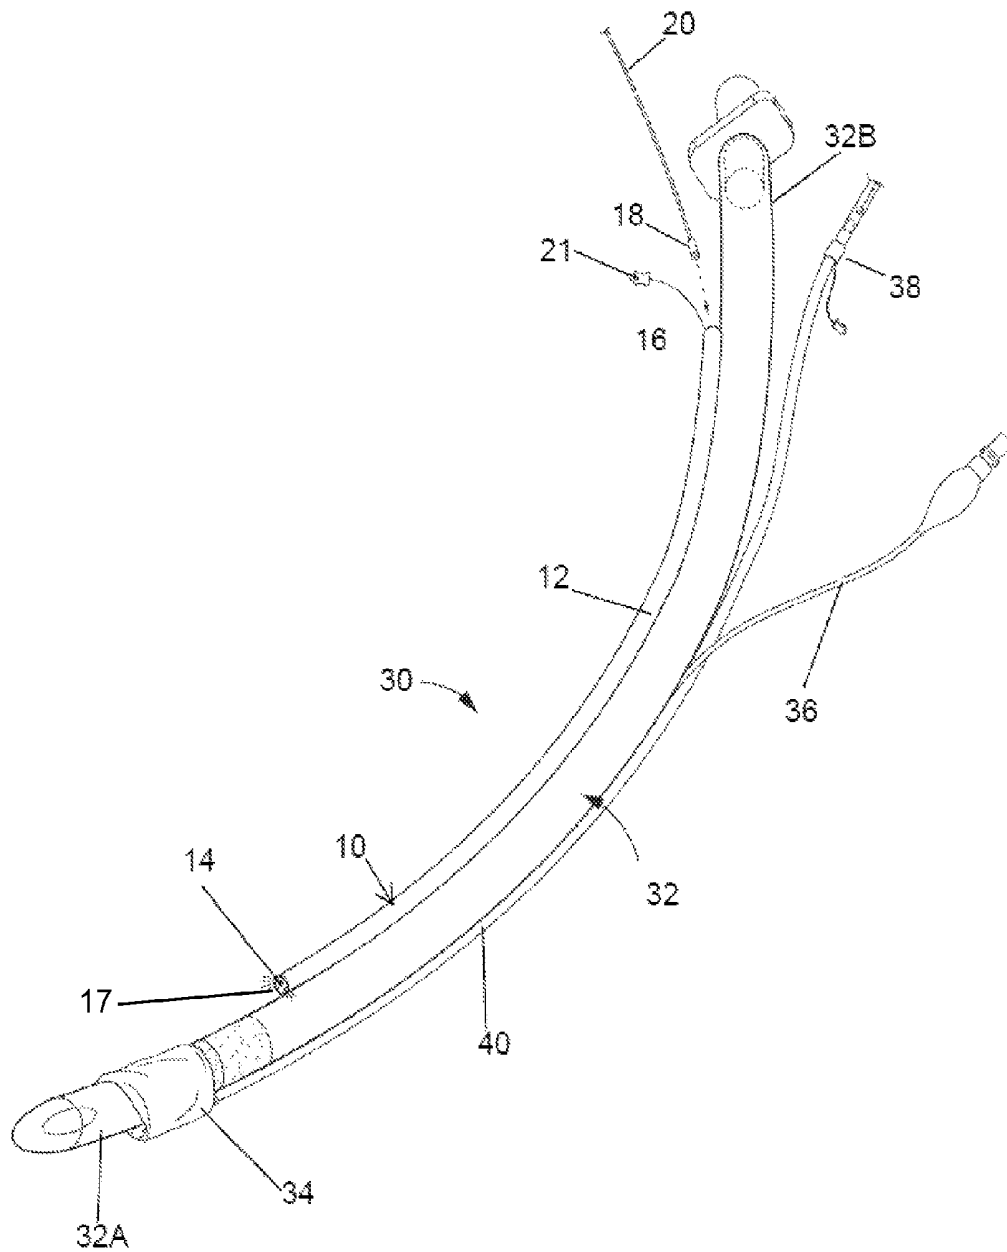


FIG. 2

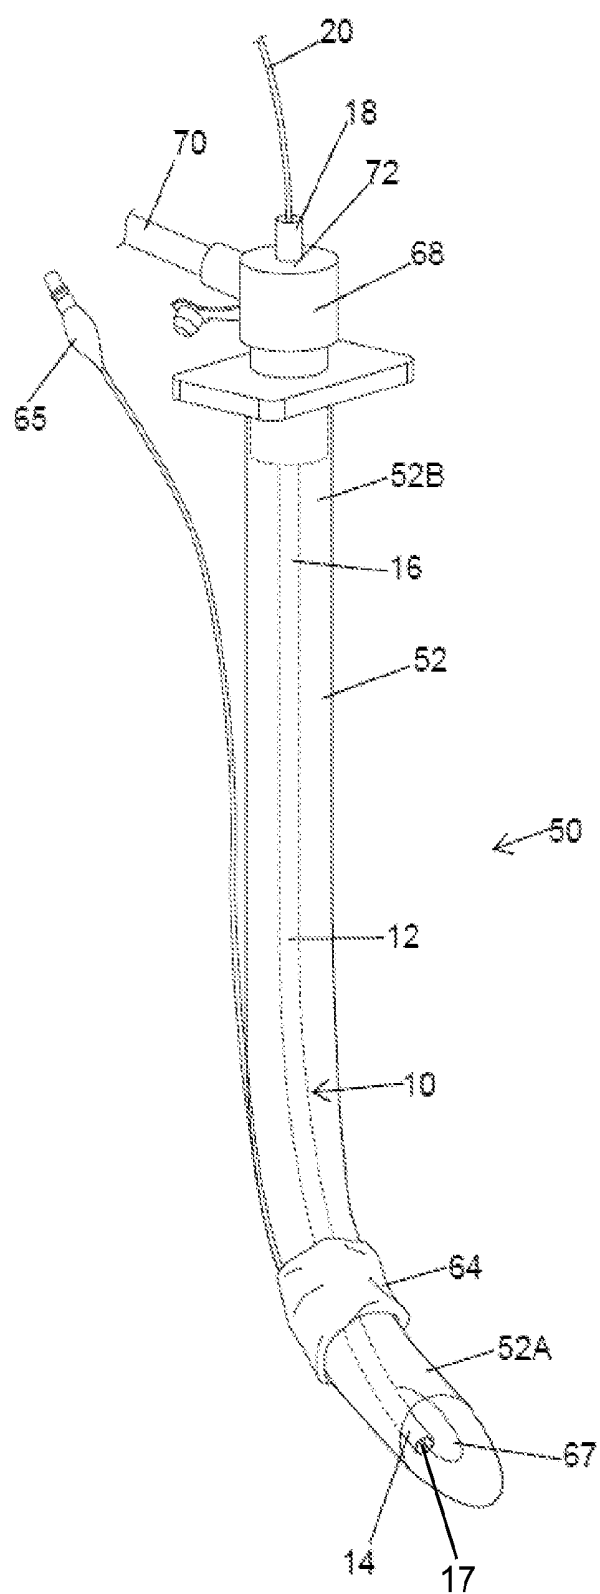


FIG. 3

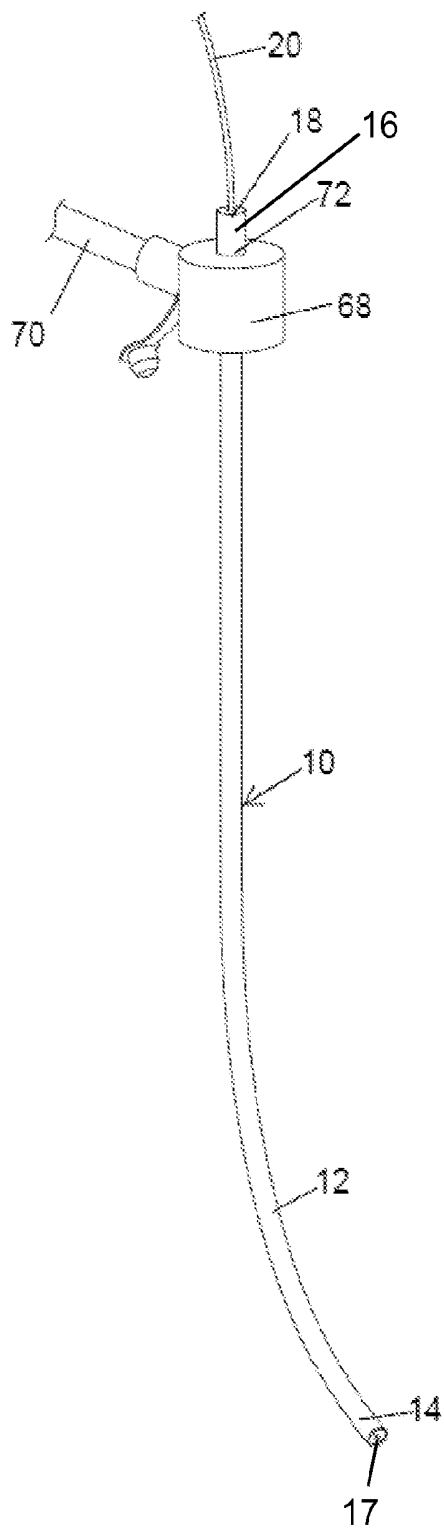


FIG. 4A

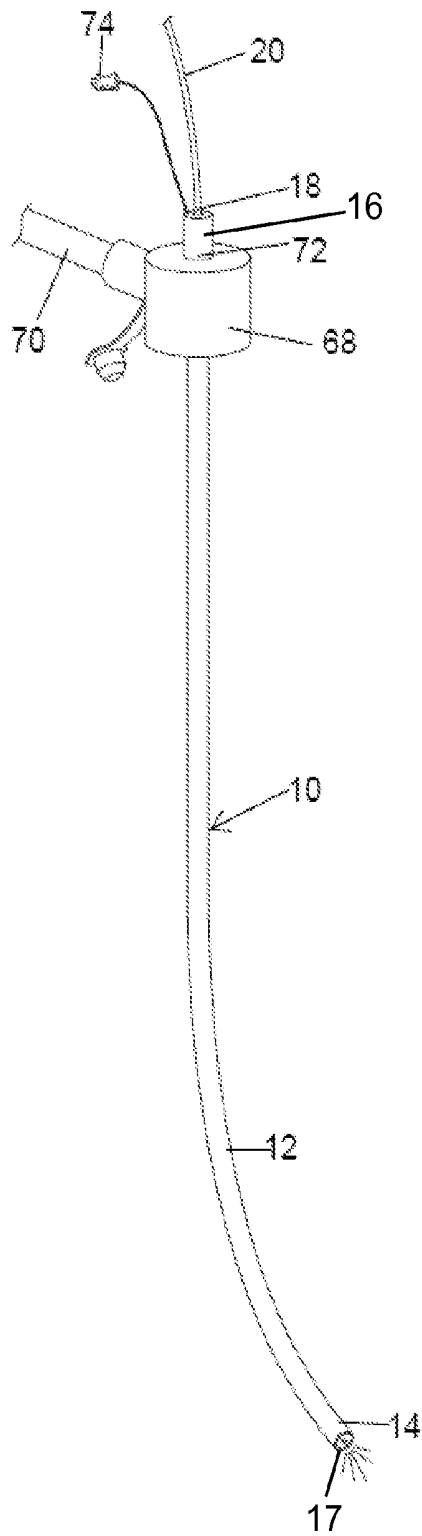


FIG. 4B

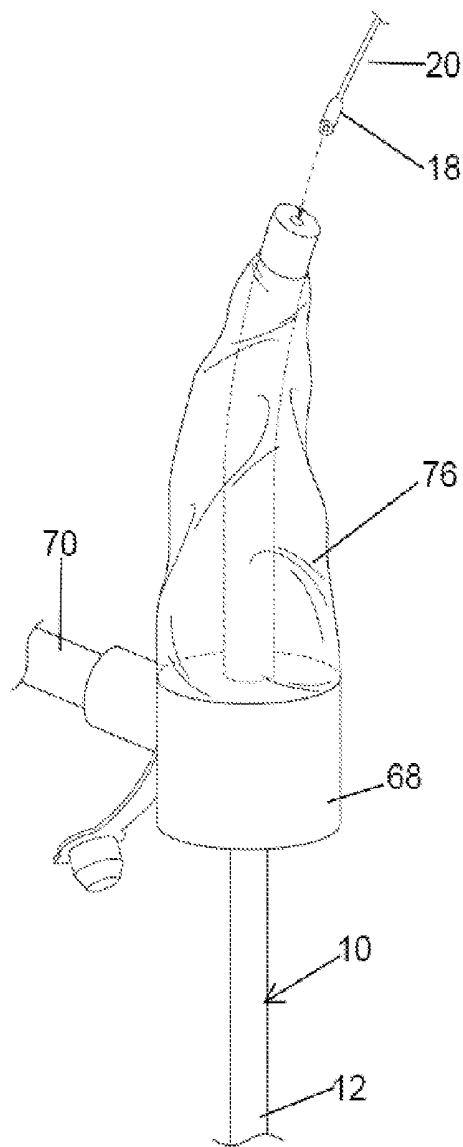


FIG. 5A

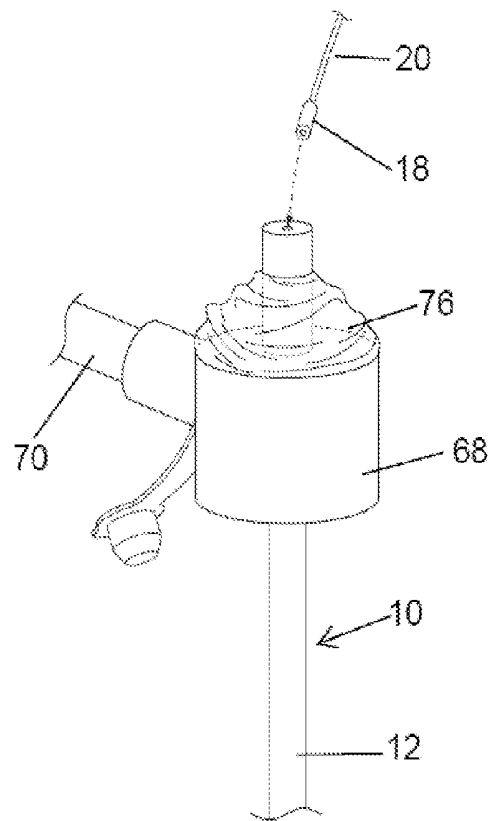


FIG. 5B

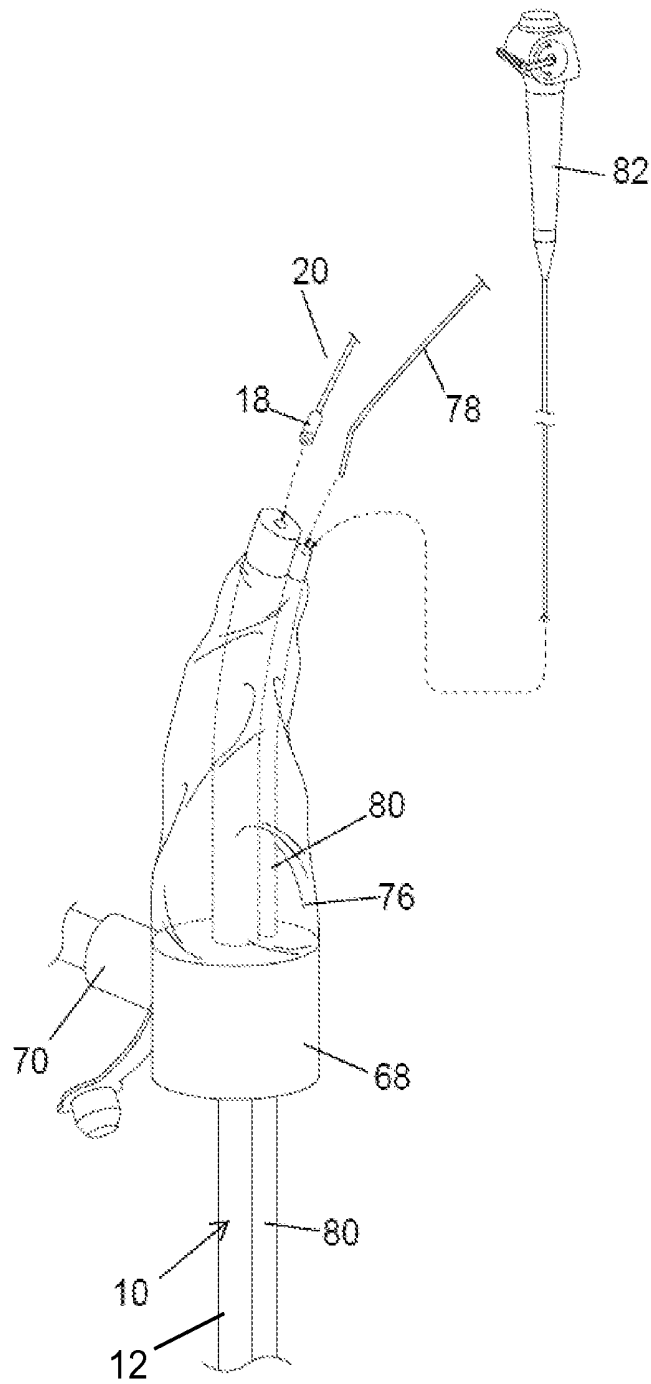
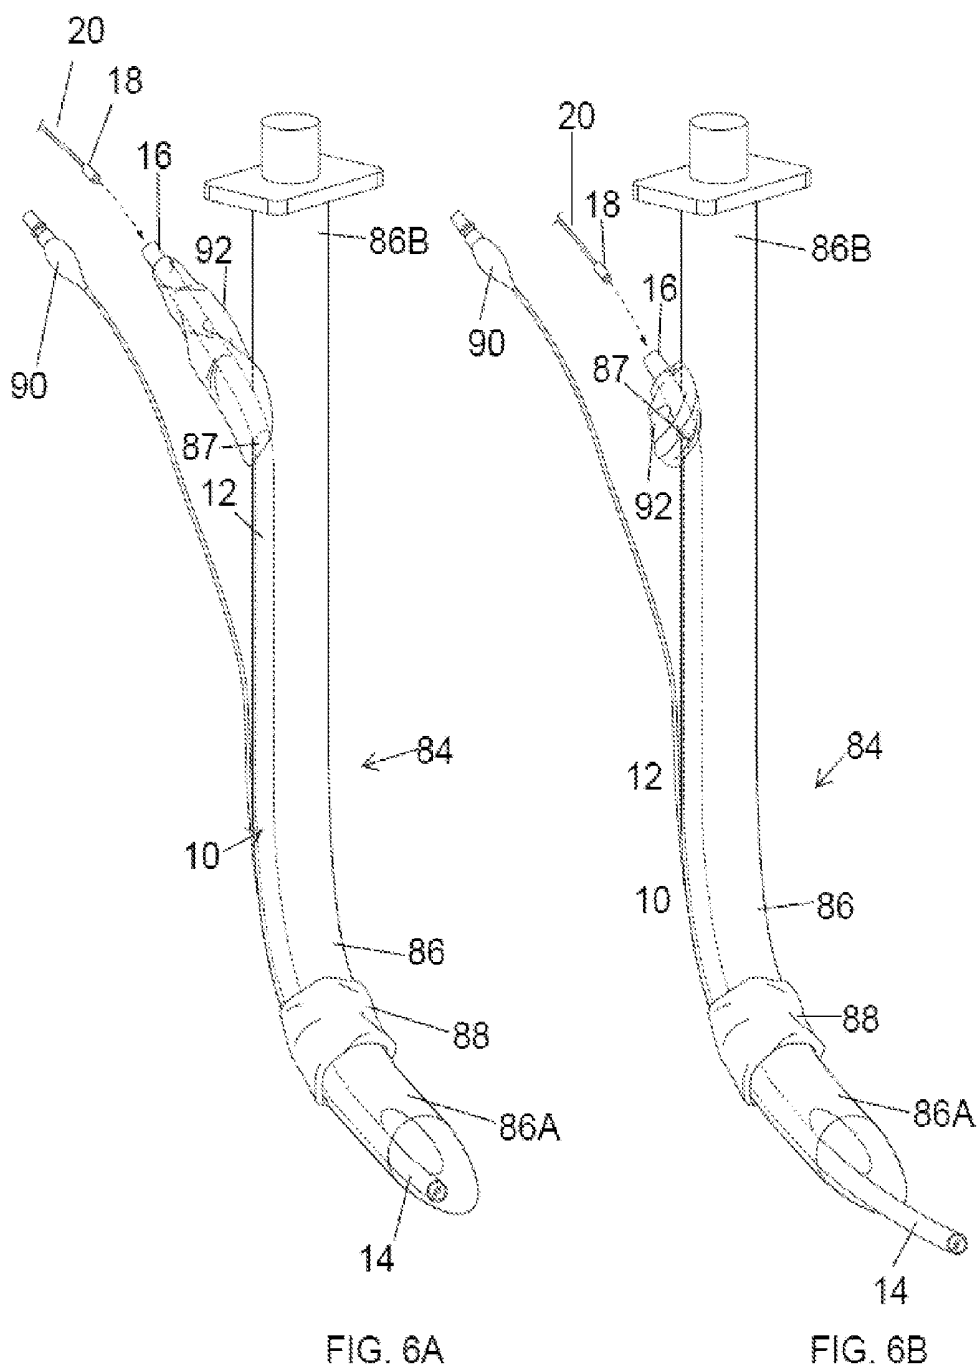


FIG. 5C



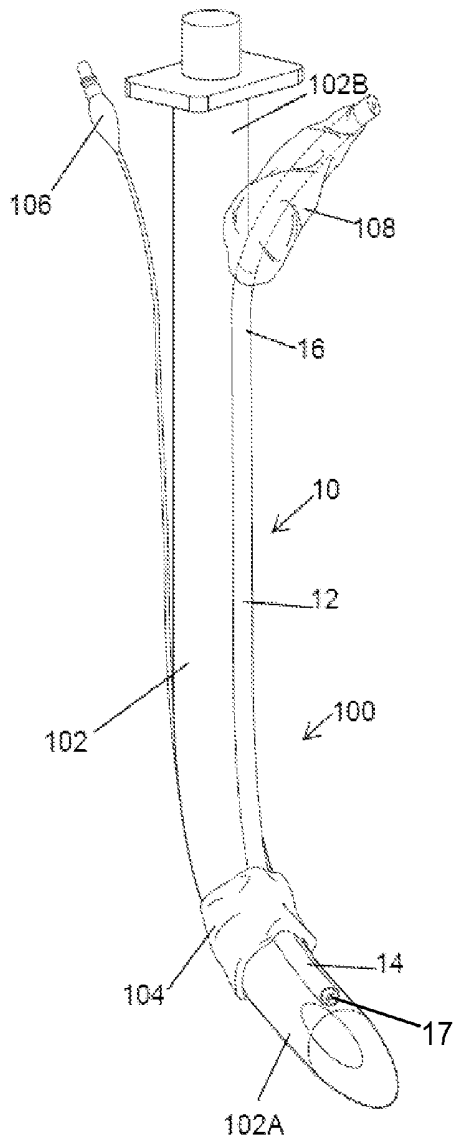


FIG. 7A

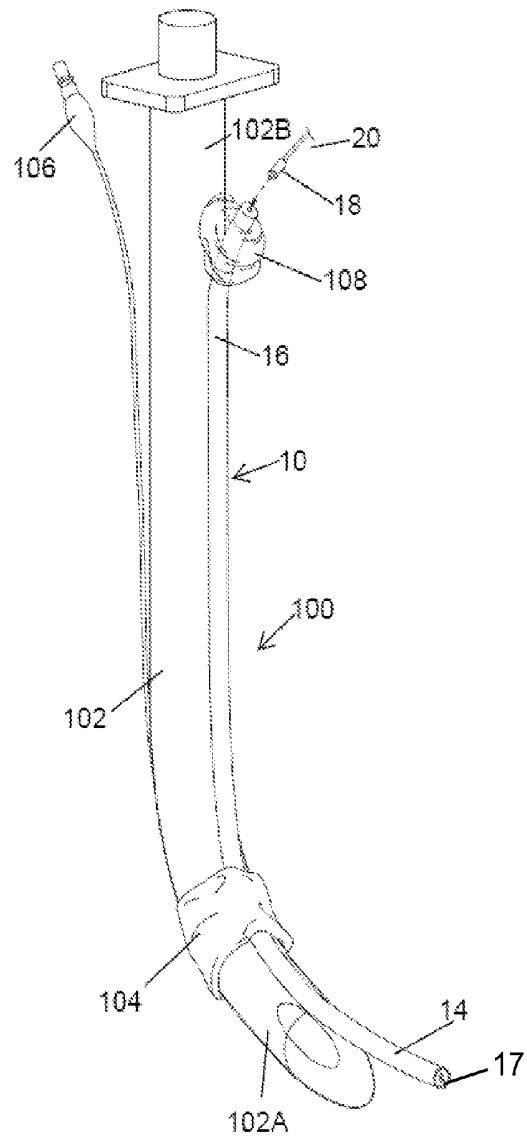


FIG. 7B

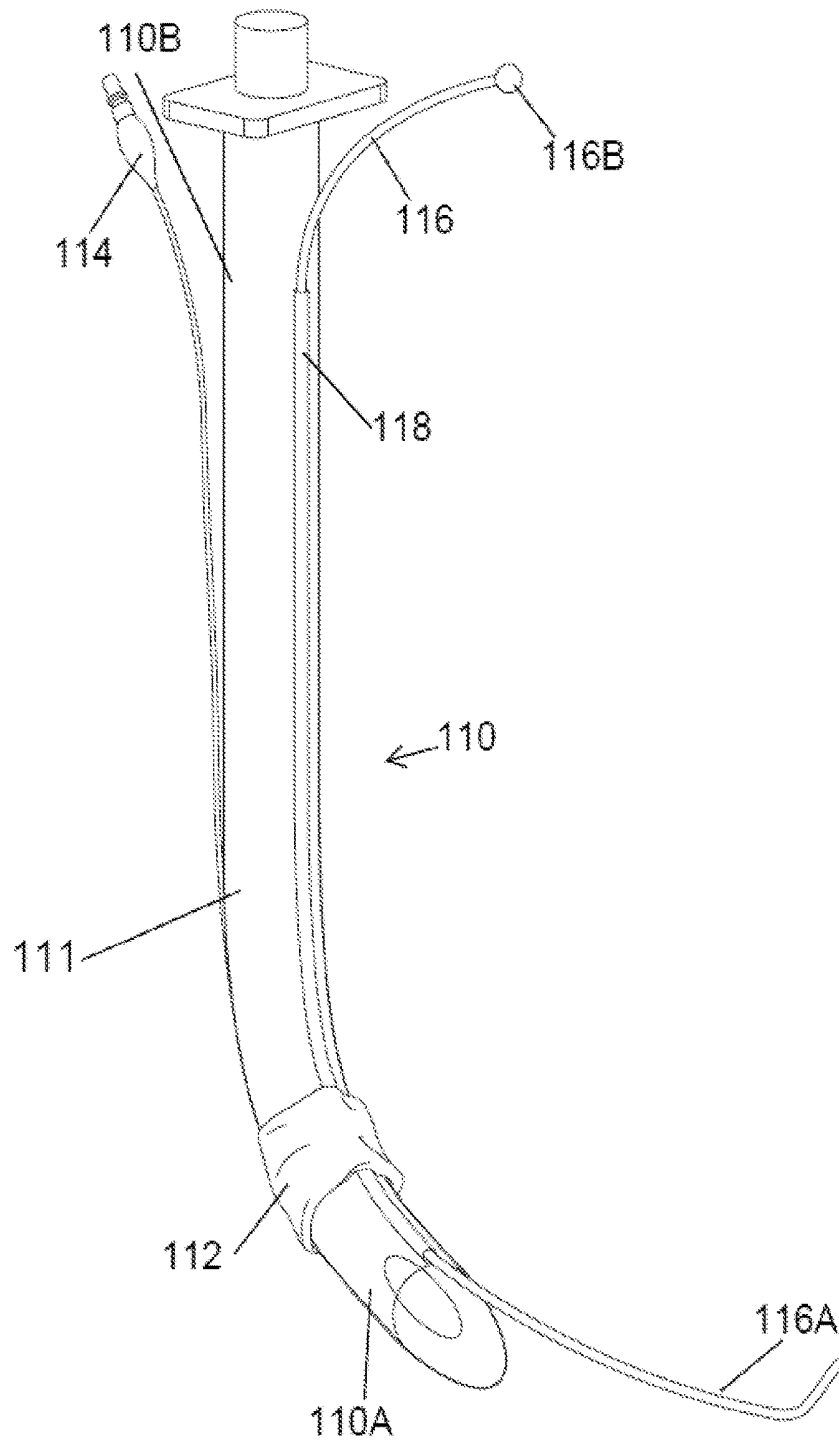
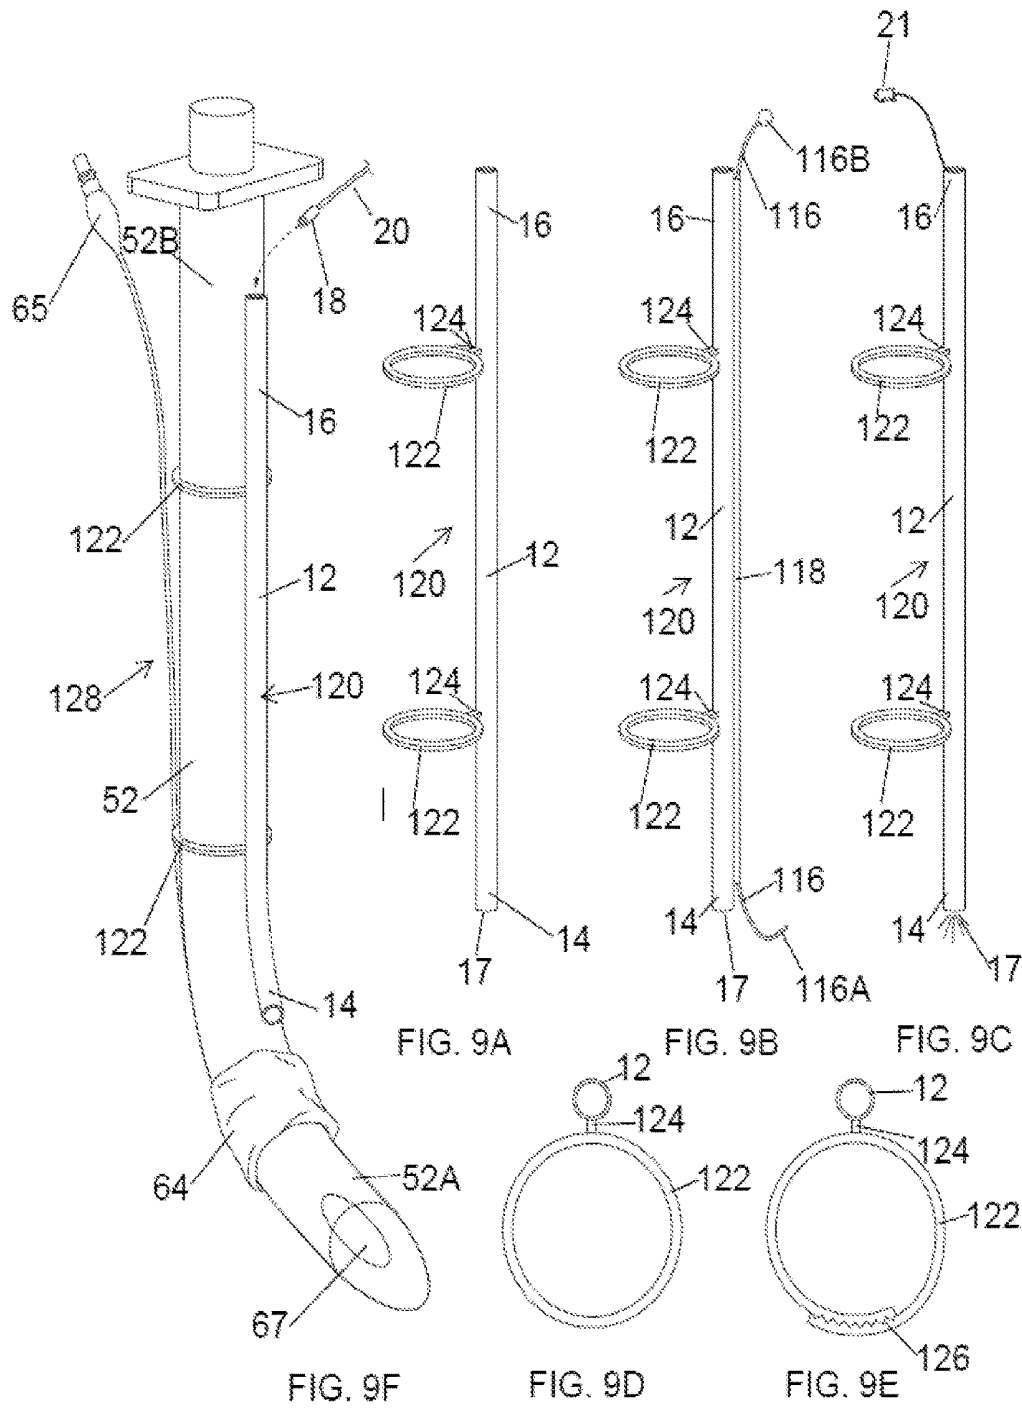


FIG. 8



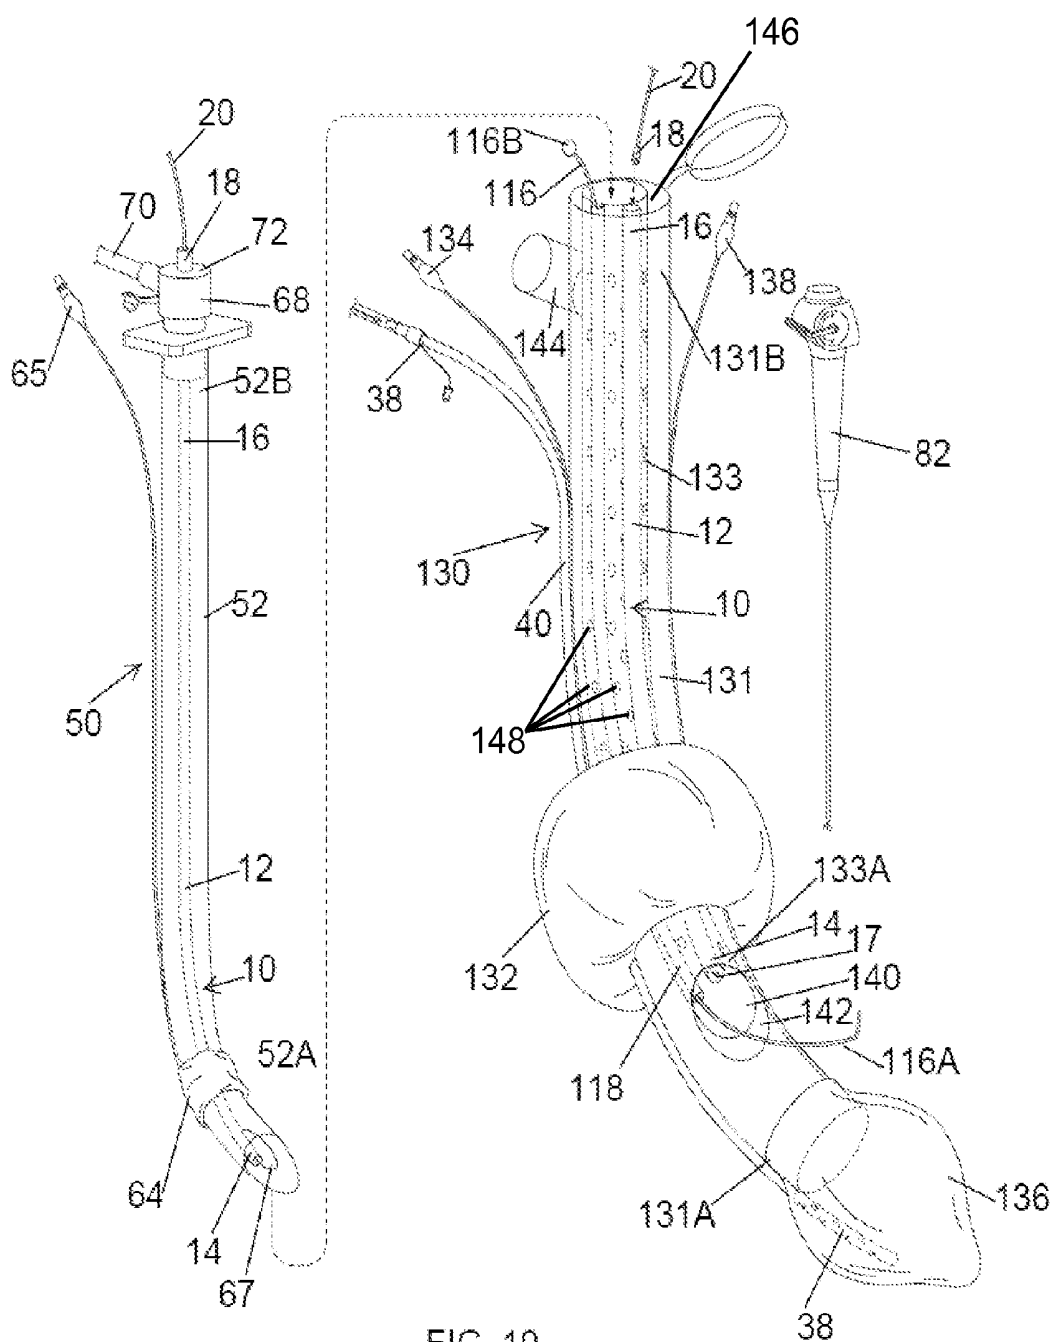


FIG. 10

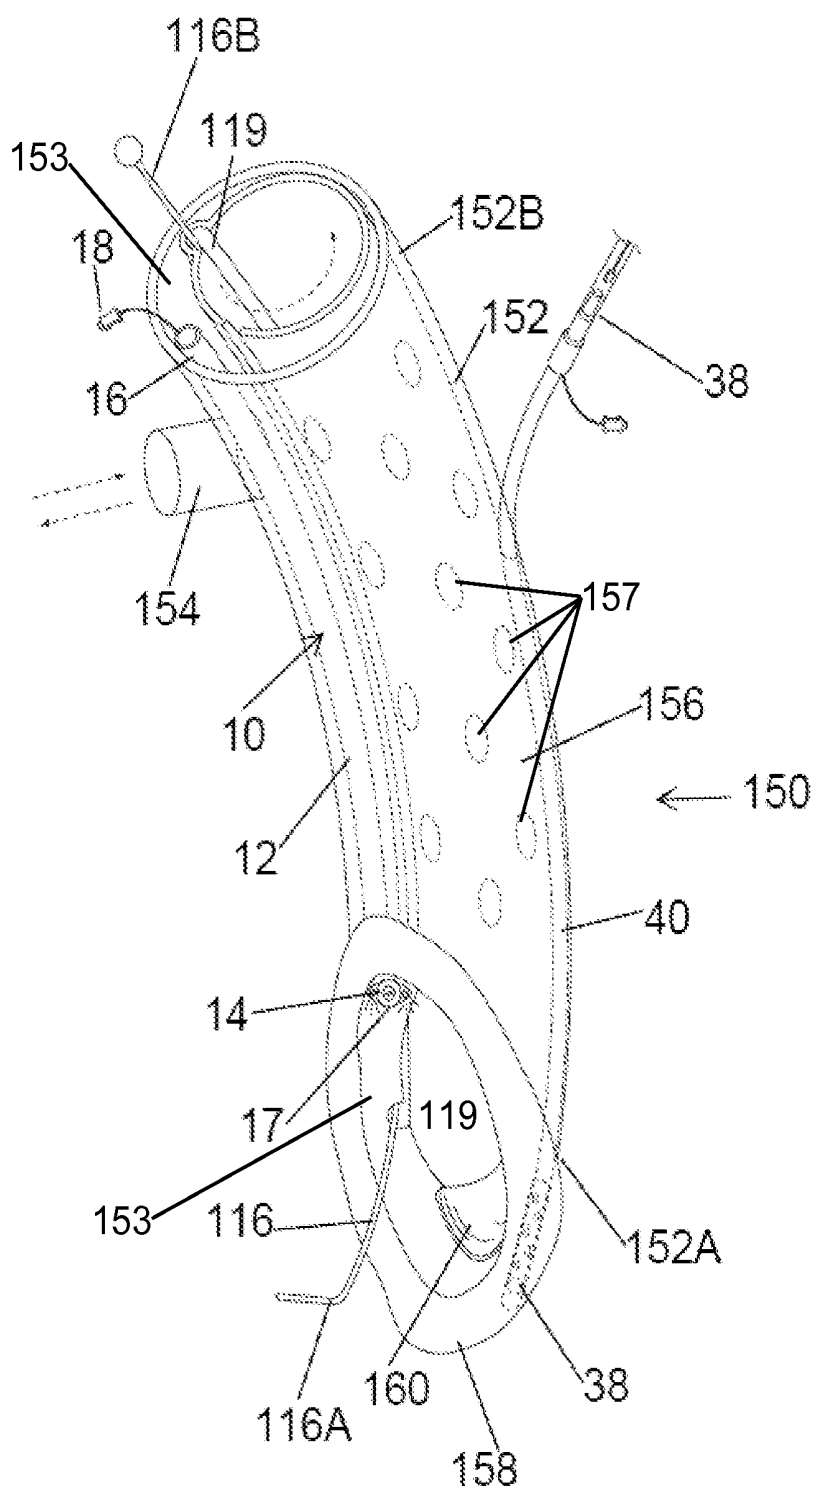


FIG. 11A

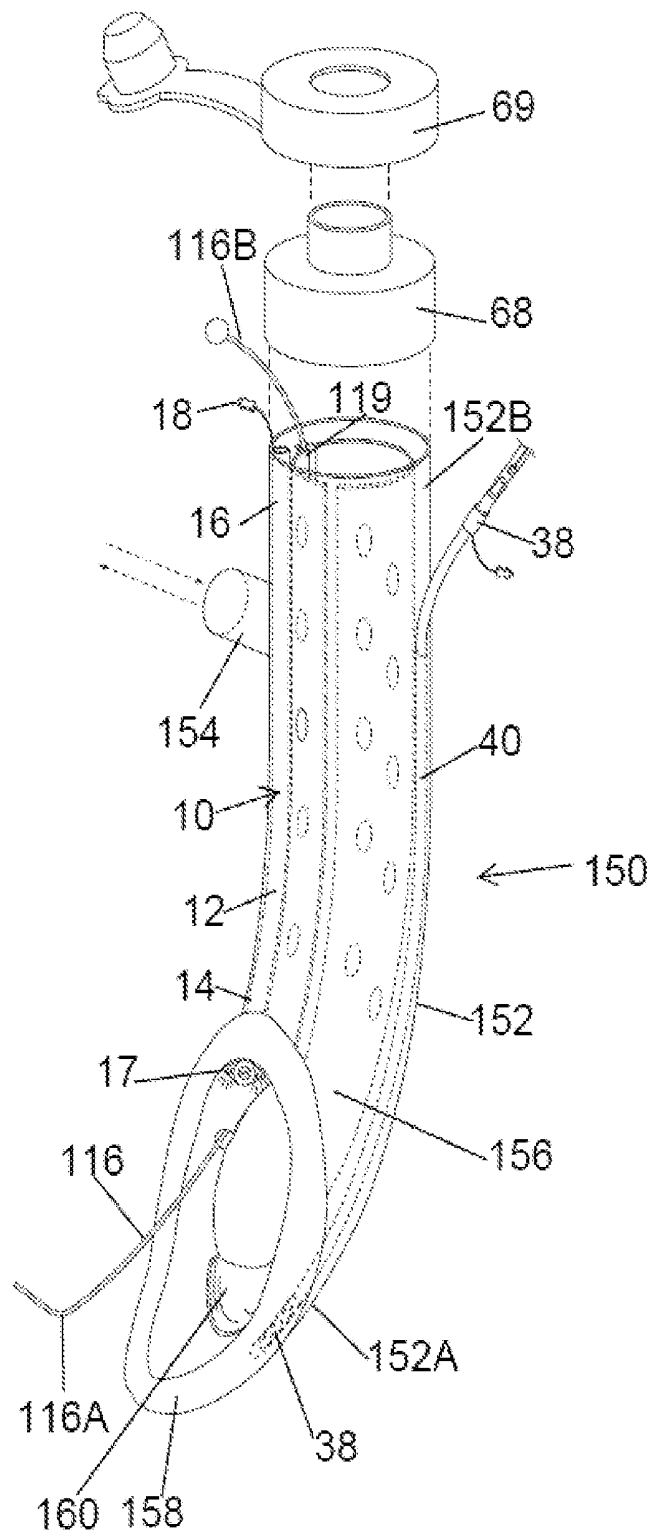
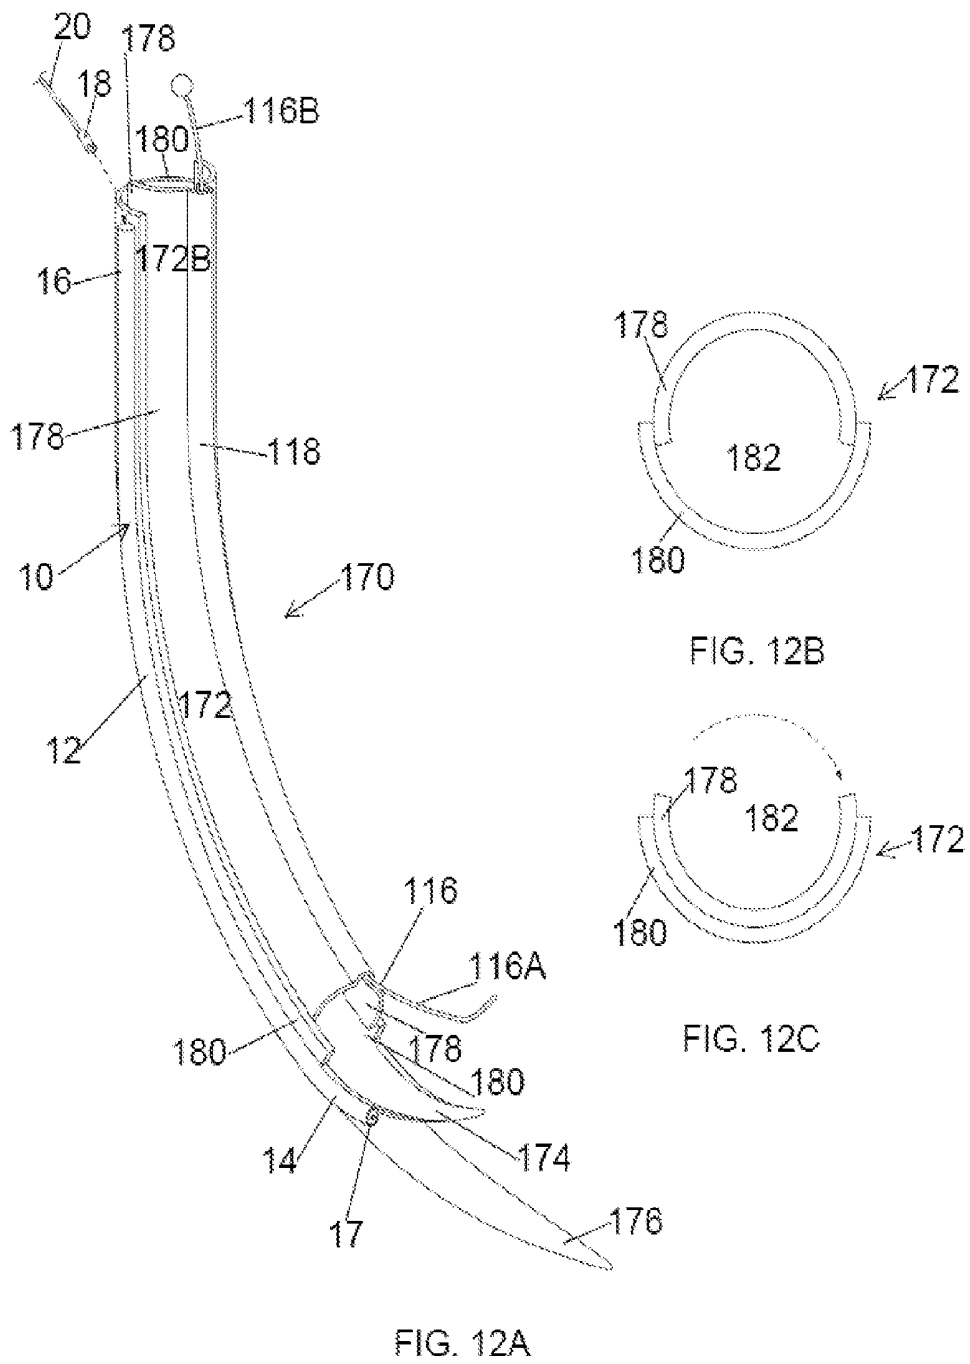


FIG. 11B



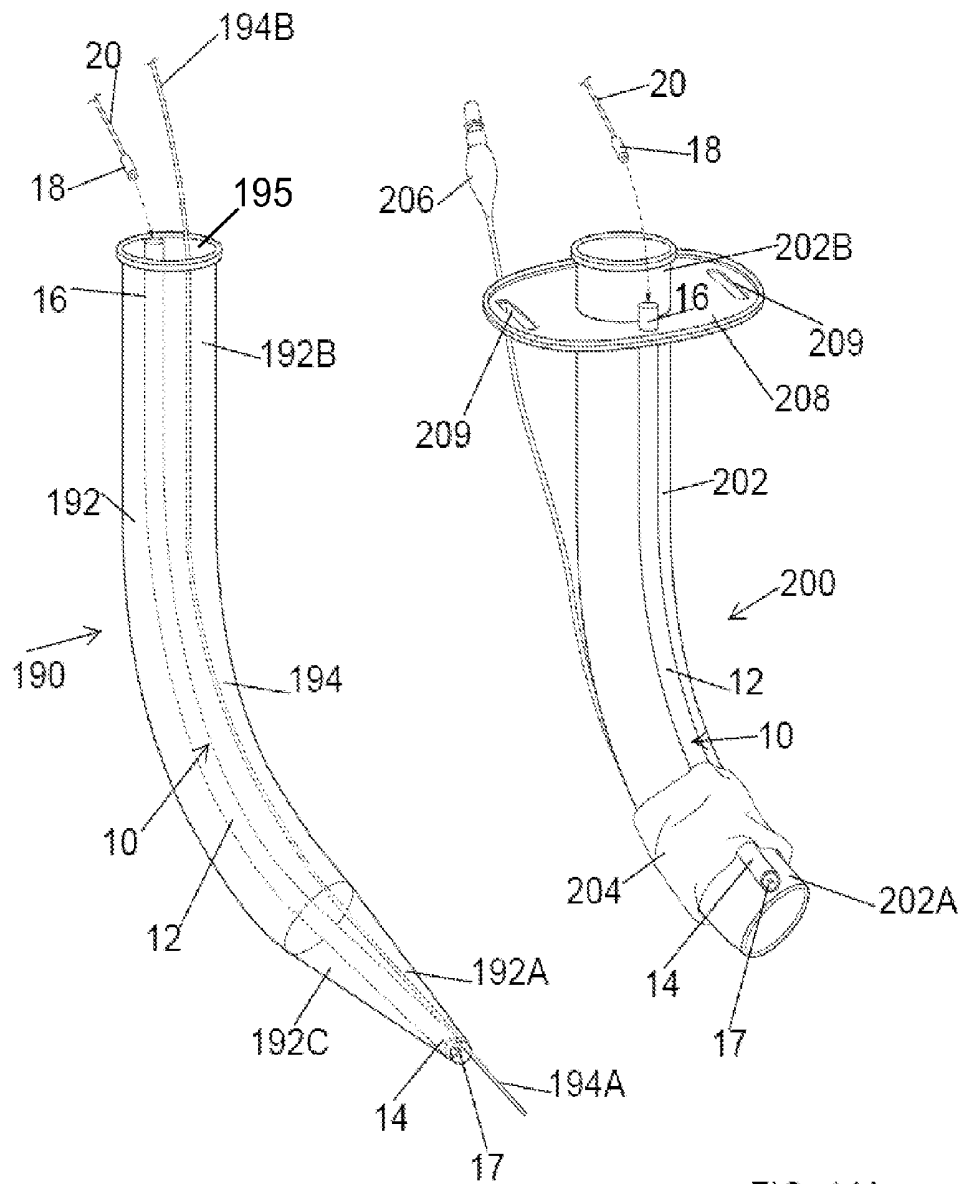


FIG. 13

FIG. 14A

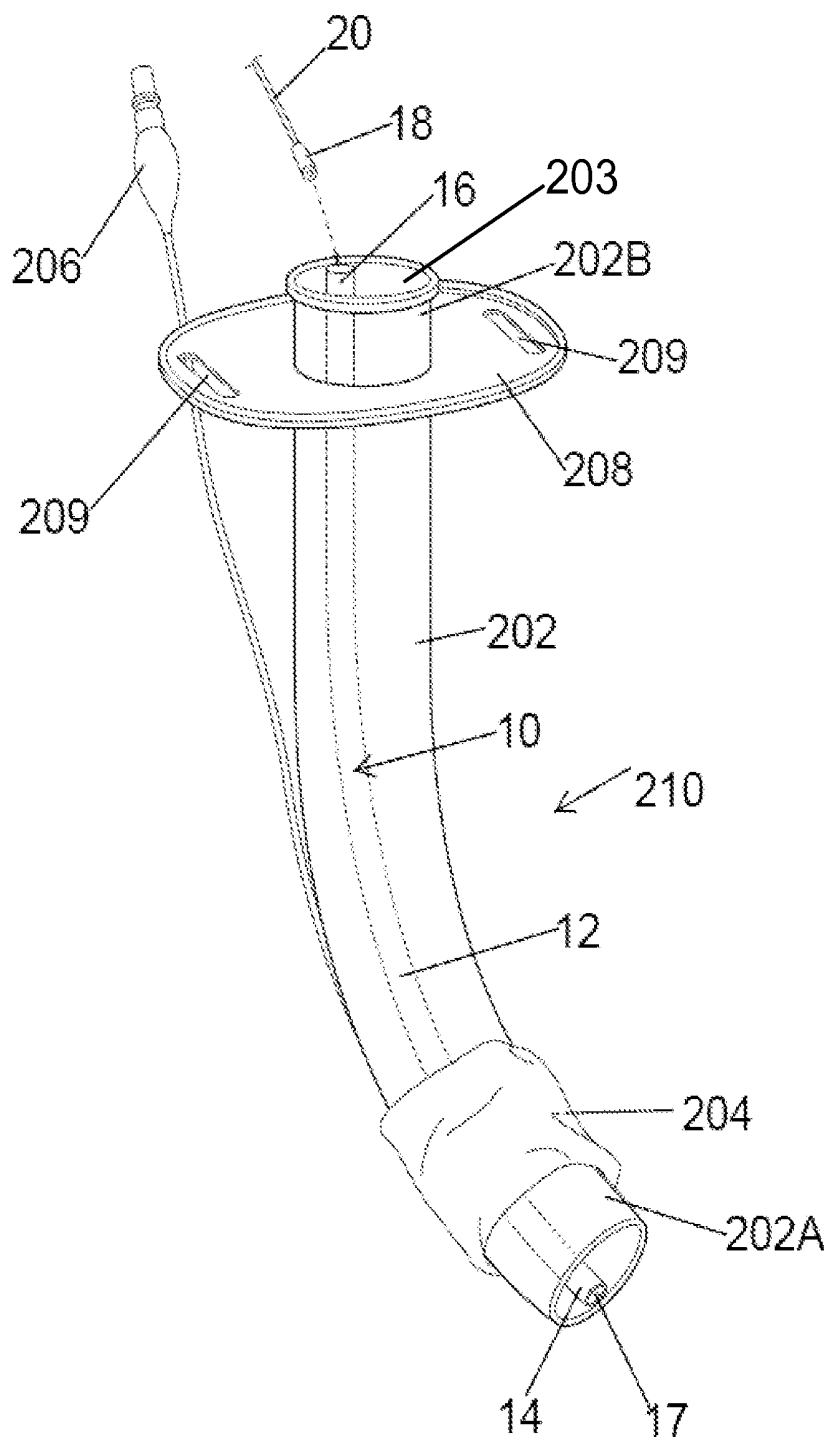


FIG. 14B

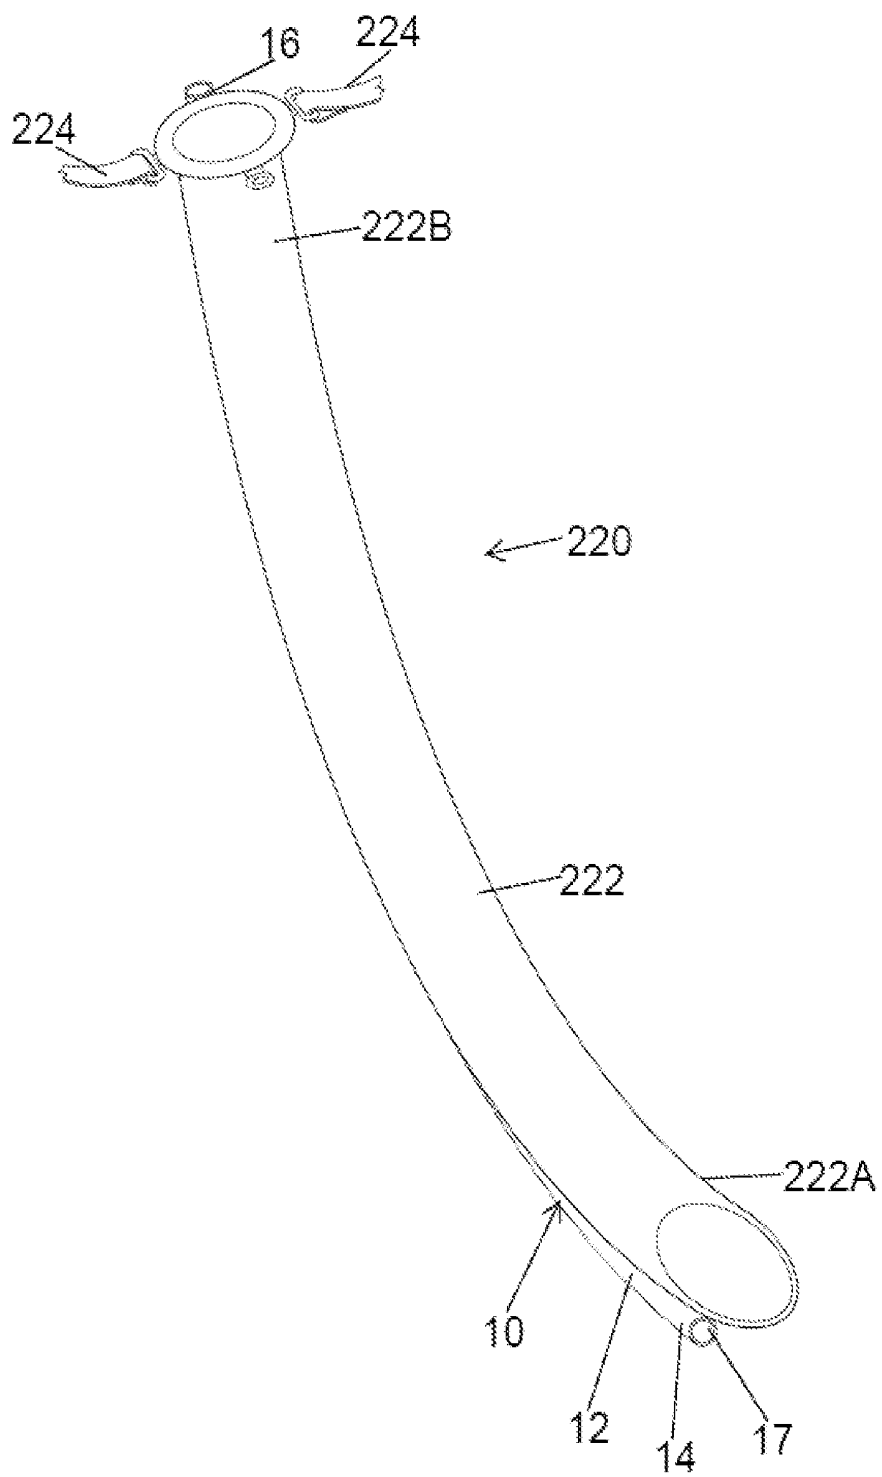


FIG. 15

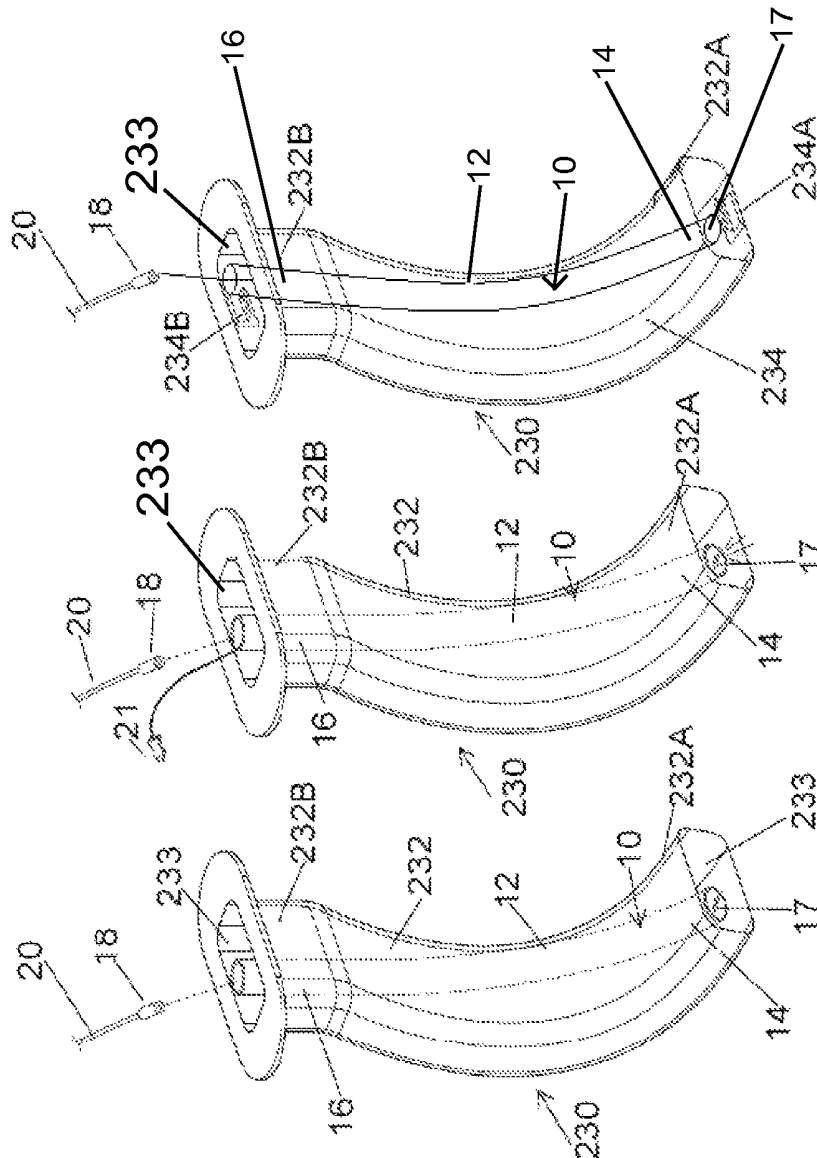


FIG. 16A

FIG. 16B

FIG. 16C

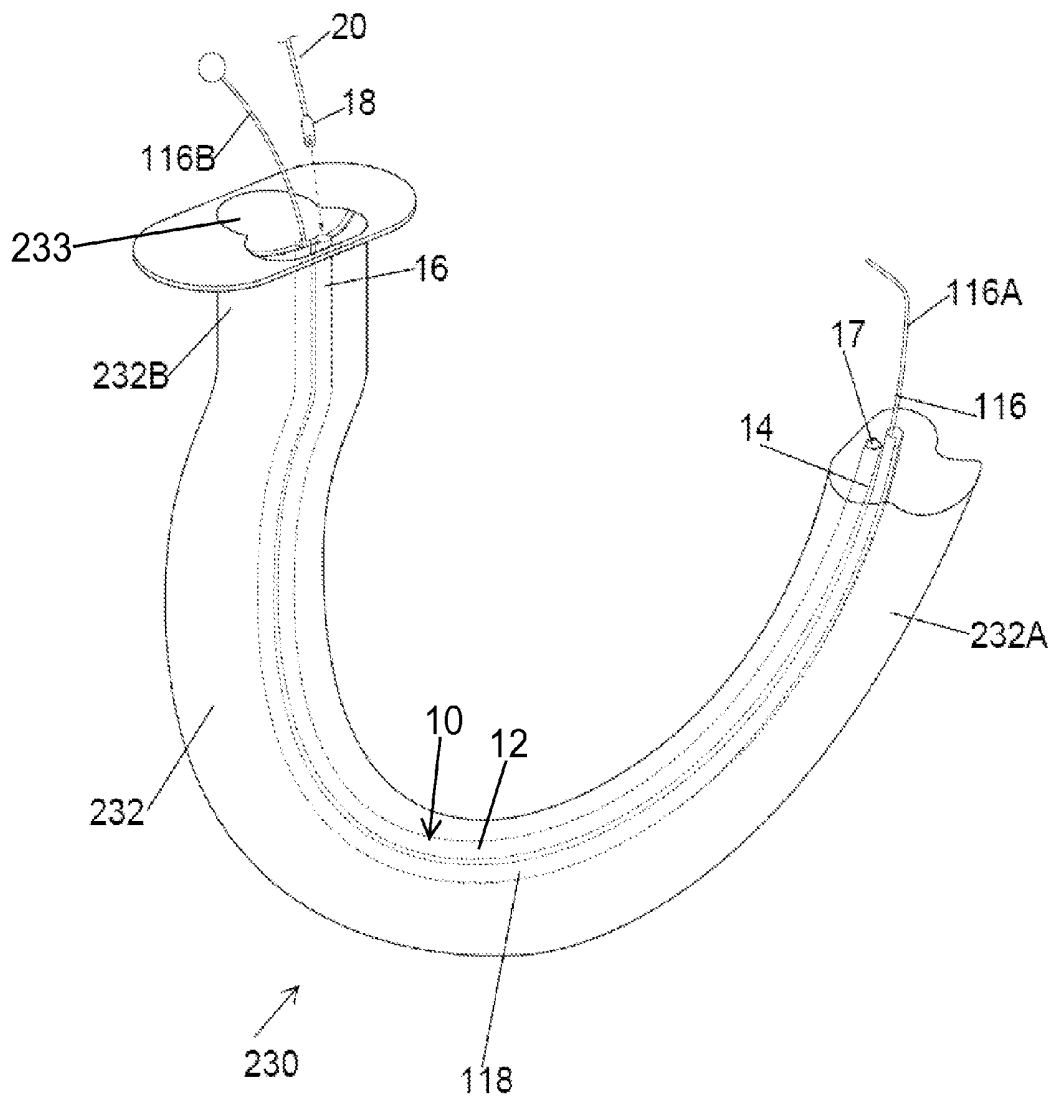


FIG. 16D

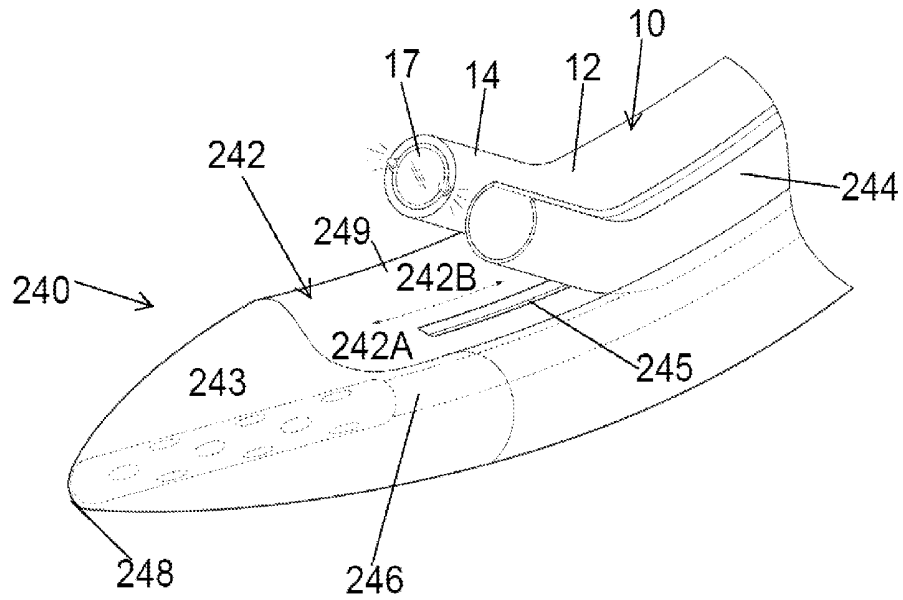
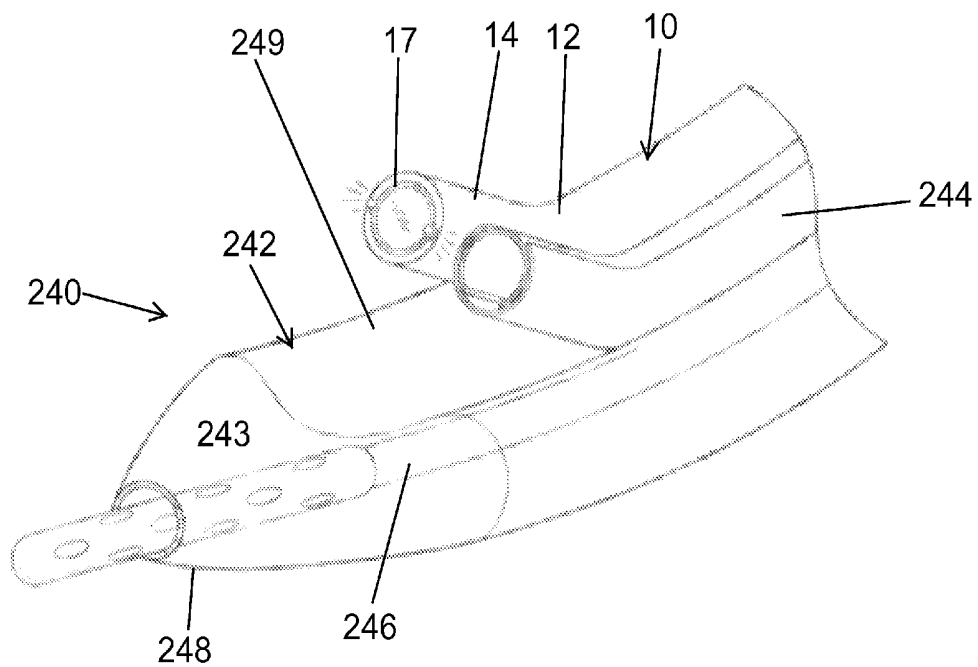


FIG. 17A



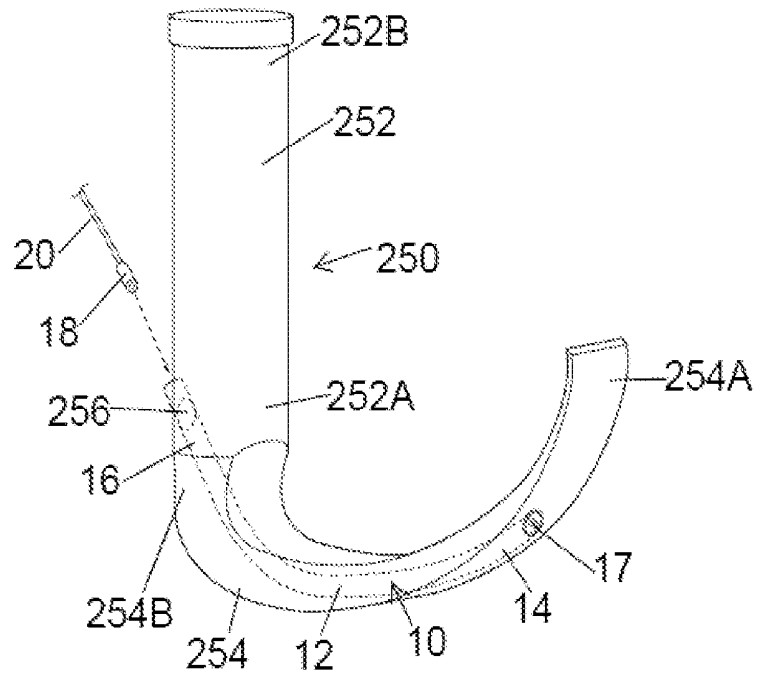


FIG. 18A

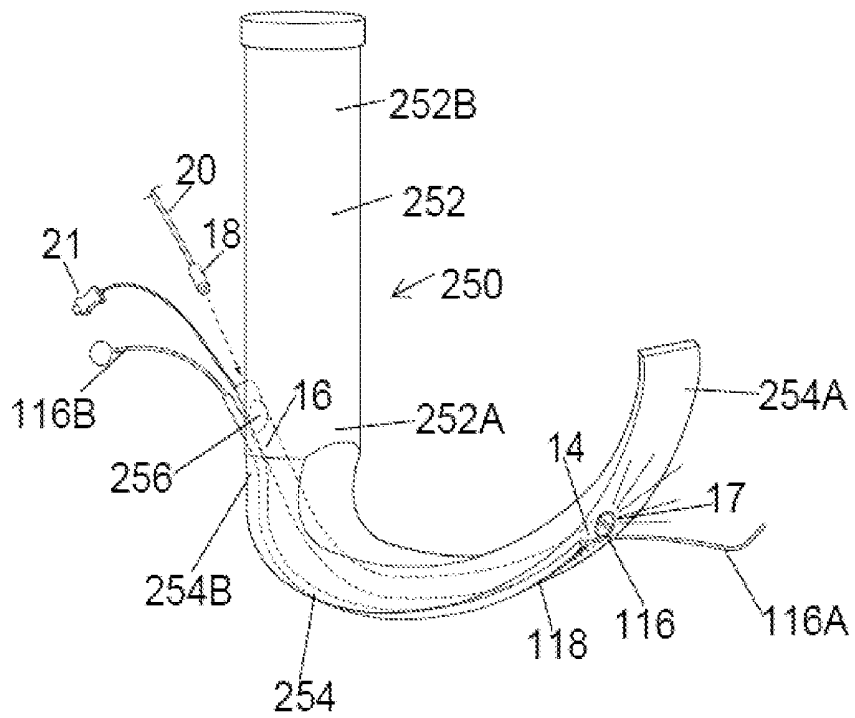


FIG. 18B

FIG. 19

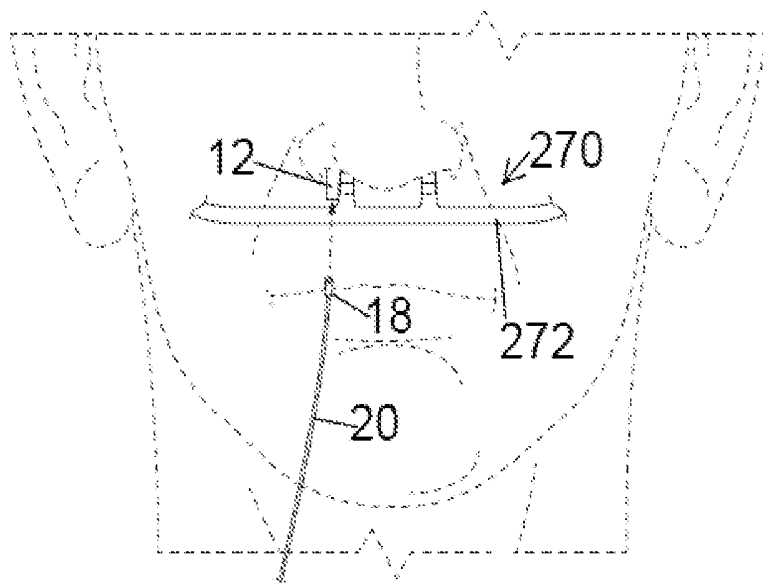


FIG. 20A

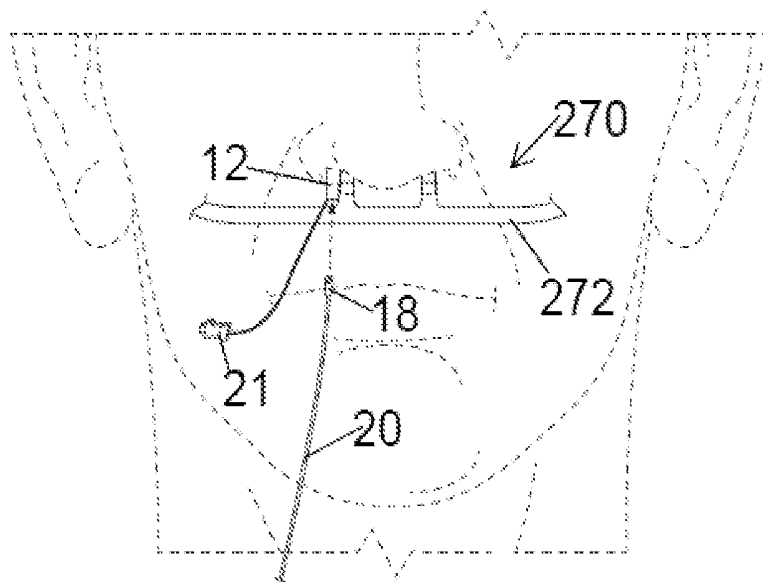


FIG. 20B

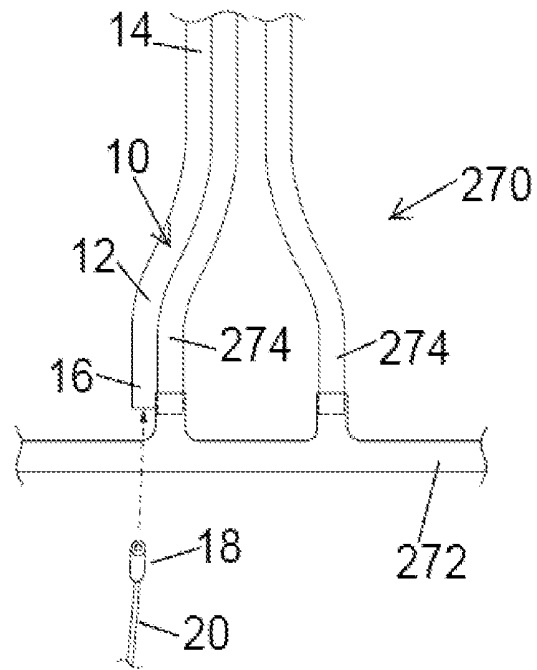


FIG. 20C

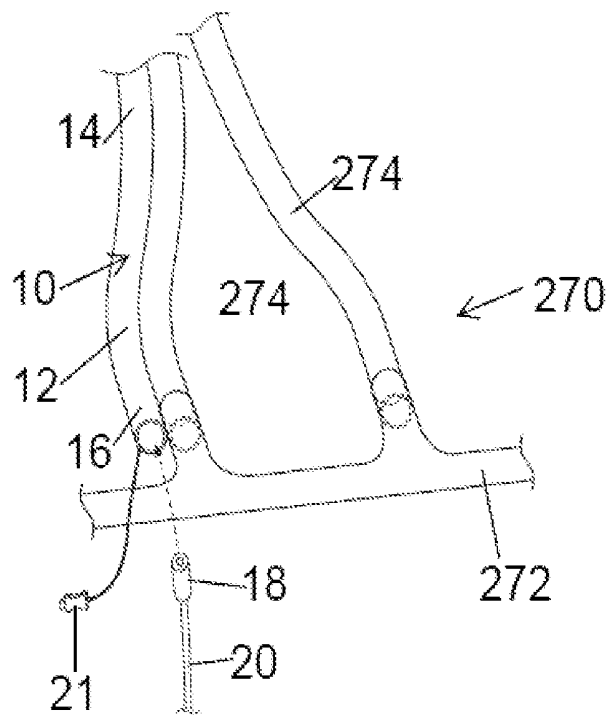


FIG. 20D

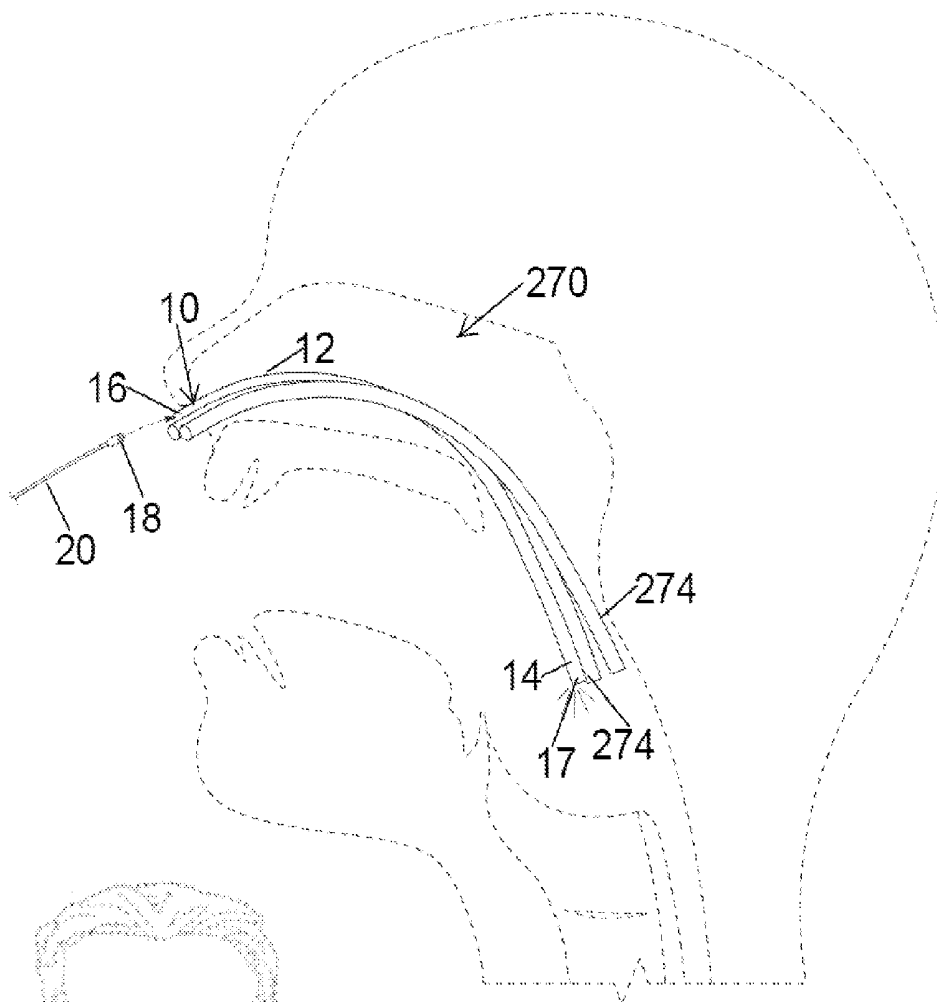


FIG. 20E

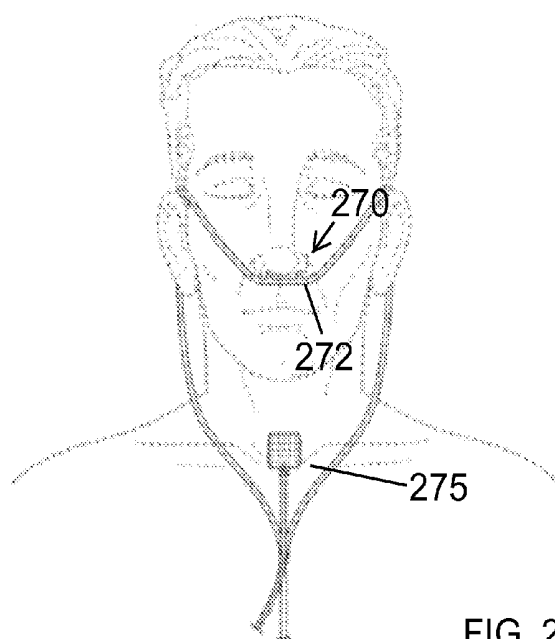


FIG. 20F

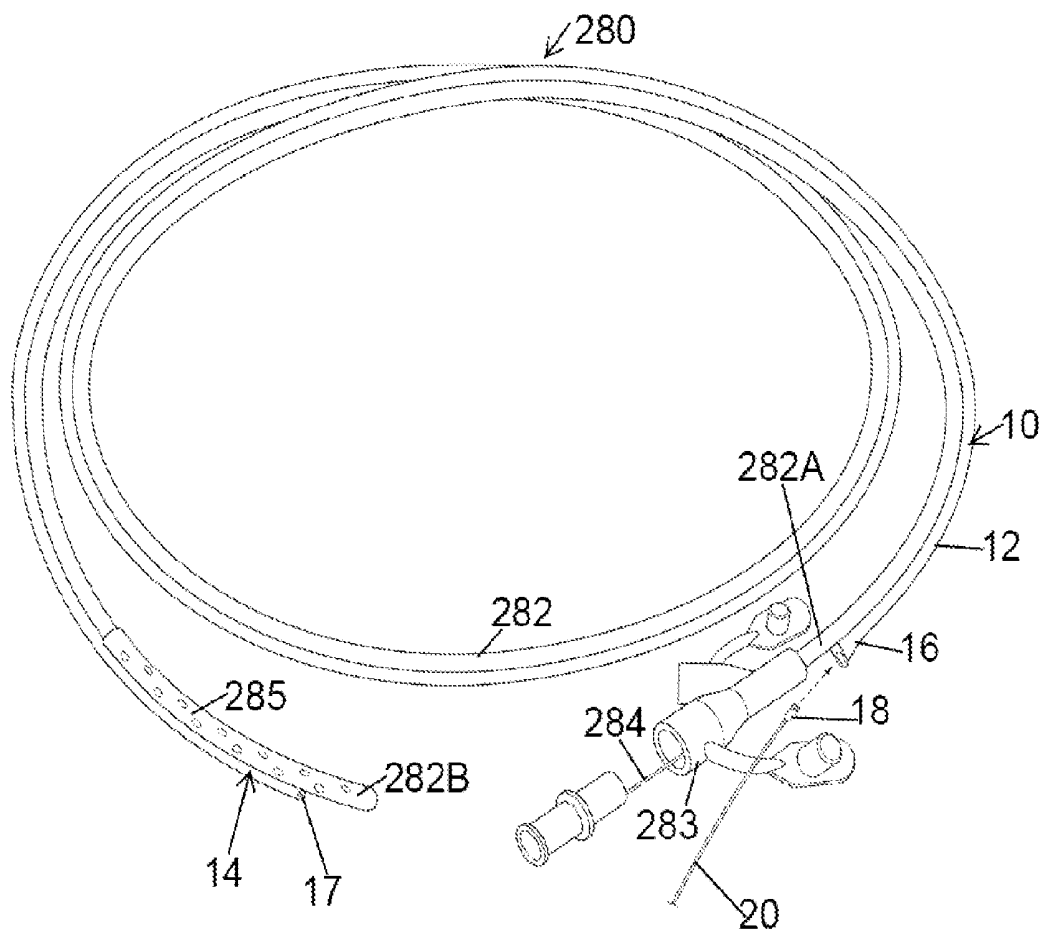


FIG. 21

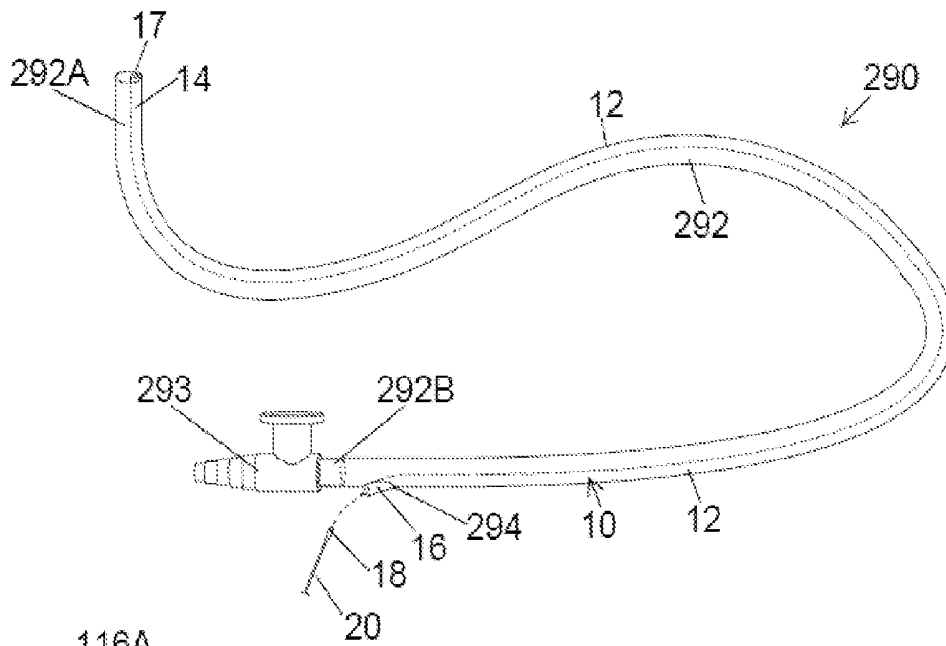


FIG. 22A

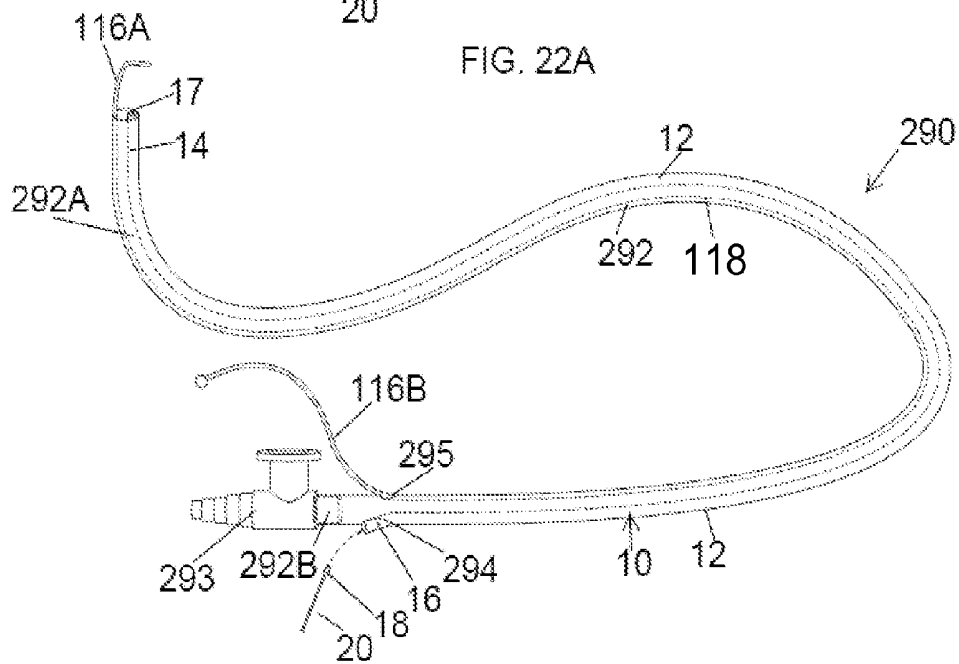


FIG. 22B

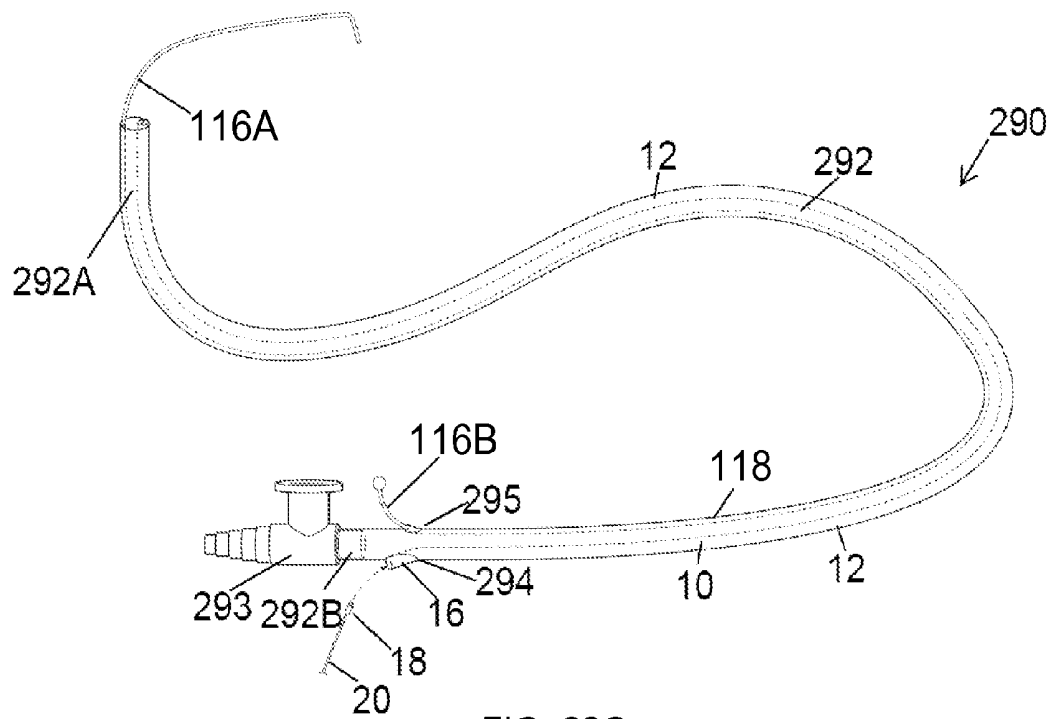


FIG. 22C

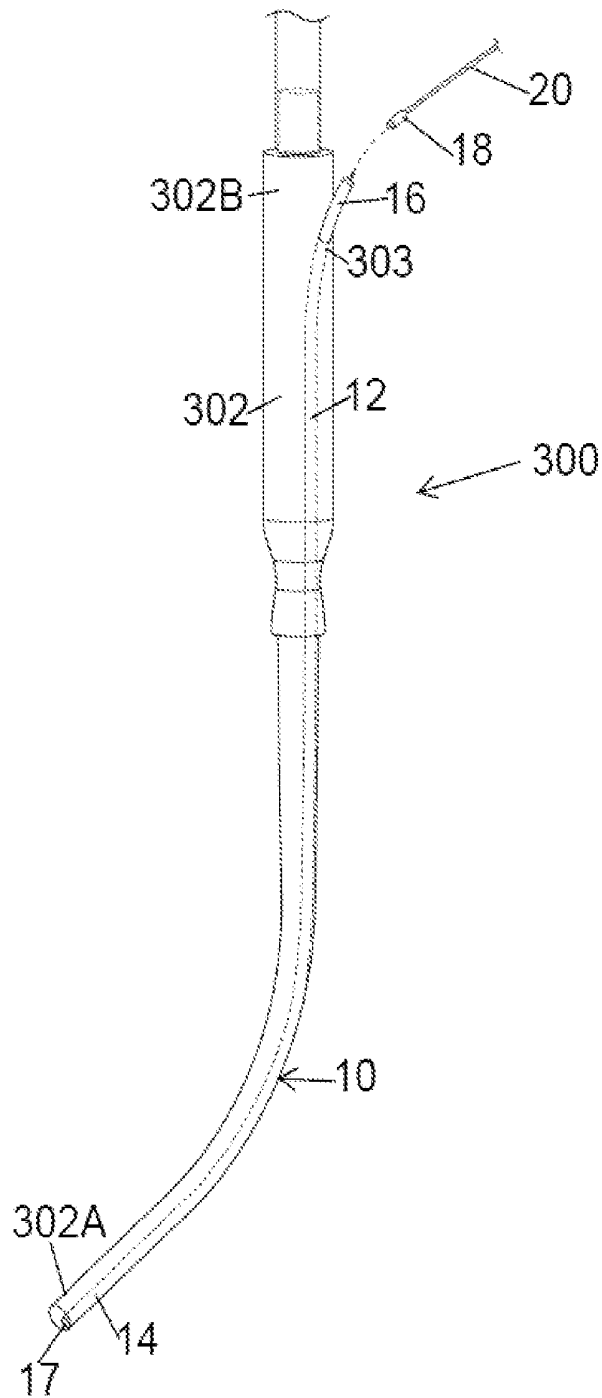


FIG. 23

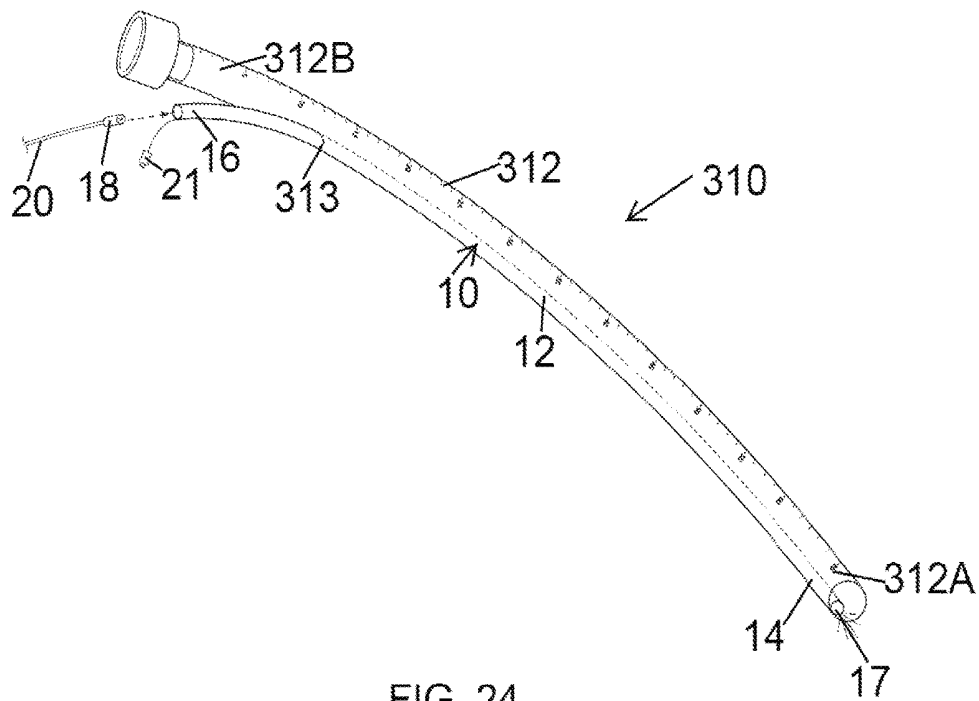


FIG. 24

MEDICAL DEVICES AND METHODS OF PLACEMENT

FIELD OF THE INVENTION

The invention provides various medical devices, each with a camera placed in a camera tube, which allows for one camera to provide continuous visualization for each device during and after placement in a patient. A sound device, such as a microphone, is incorporated in many devices and provides continuous monitoring of breath and heart sounds in a patient. The camera and microphone do not contact the patient's tissues and thus, do not require sterilization. The continuous visualization and sound monitoring of the patient are in real time and enable remote monitoring as well. Methods for rapid and accurate placement of a medical device in a patient are provided as well.

BACKGROUND

Various devices are available to stabilize a patient and facilitate his breathing, feeding and medication delivery. Such devices are used in patients during surgical procedures, after certain traumas including spinal cord injuries, and in patients suffering from certain medical conditions including advanced Alzheimer disease. These devices include endotracheal tubes, airway devices, feeding tubes, oral airways, nasal cannulas and the like.

Because human anatomy varies significantly from a patient to a patient, properly placing a medical device in a patient's trachea requires a significant skill and is a task laced with inherent risk. The task becomes even more complicated because the insertion procedure may have to be performed immediately at an accident site, on pediatric patients, in a nursing home, on a battlefield or at a natural disaster site where many patients have to be attended at the same time.

The process of placing a breathing tube in a patient is called intubation. Devices such as laryngoscopes, videolaryngoscopes, fiberoptic scopes, as well as other proprietary videoscopes have been developed. These devices provide accuracy for initial placement, but do not provide continuous visualization or mobility of the image after a medical device has been placed in a patient. Newer devices, such as Vivasight SL or DL endotracheal tubes, provide continuous visualization, but are costly because they depend on a single use of disposable cameras and they are not transferrable from one medical device to another. The Totaltrack VLM supraglottic airway has a proprietary reusable camera for only its one device, and it cannot be transferred to other medical devices.

Thus, there remains the need for improved devices which can be easily monitored remotely by a qualified personal during placement and after placement for an adverse reaction. After a medical device has been placed in a patient, the need remains to monitor in real time the patient's possible adverse reactions such as for example, aspiration, airway secretion, apnea, etc.

SUMMARY OF THE INVENTION

At least some of these needs are addressed by present medical devices which are equipped with a portable universal visualization device in which a camera is contained within a separate camera tube and which transmits information that can be accessed and monitored remotely and simultaneously from several patients in real time.

One embodiment provides a medical visualization device which comprises a camera tube with a distal end and a proximal end. The distal end is sealed with a transparent material and a proximal end has an opening. A camera with a wire is placed inside of the camera tube. The camera can be placed inside of the camera tube and it can be retracted from the camera tube on demand. The camera can be reused in various devices without sterilization. The camera can transmit images to a remote location wirelessly. In some embodiments, the camera tube comprises a fiber optic material. The visualization device can be equipped with at least one of the following: a light source, a stylet, a bougie and a sound- and temperature-monitoring device which can transmit the information to a remote location wirelessly. The visualization device can transmit images, sounds and other data to any number of remotely located monitoring devices and/or data storage devices. Such devices include, but are not limited to, a wireless portable device, smart phone, tablet, watch, cell phone, hand-held wireless device, computer, remote data server, radio, television, walkie-talkie and the like.

A further embodiment provides a method of continuous monitoring of a patient's at least one internal organ, the method comprising placing in the patient the visualization device with the camera in the sealed camera tube, causing the camera to transmit images of the internal organ in real time through the transparent material at the distal end of the camera tube, and analyzing the transmitted images. In some embodiments, the images are transmitted wirelessly to at least one remote location.

Various internal organs can be monitored by this method, including nasopharynx, pharynx, hypopharynx, supraglottic structures, airway, trachea, vocal cords, stomach, and vagina.

In some embodiments, the length of the camera tube in the visualization device is adjustable and it can be adjusted to the length of at least one of the following devices: an endotracheal tube, a supraglottic airway, airway device, oral airway, dilator, tracheostomy device, intubating oral airway, esophageal stethoscope, nasal cannula, feeding tube, suction tube and endotracheal changing tube.

Further embodiments provide a method for placing a medical device in a patient in which the medical device is equipped with the visualization device and a bougie. The medical device is inserted in the patient and the placement of the device is guided with the bougie under continuous visualization.

A kit for monitoring a patient's internal organ in real time is also provided. The kit comprises a camera tube with the adjustable length and with at least one ring attached externally to the camera tube, wherein the camera tube has a distal end and a proximal end and wherein the distal end of the camera tube is sealed with a transparent material; and a reusable camera which can be placed and removed from the camera tube and which can transmit images wirelessly to at least one remote location. This real time information obtained with the visualization device can be transferred or stored to multiple distant monitoring sites.

Also provided is a medical device comprising a visualization device sealed to, attached to or otherwise combined with at least one of the following second devices: an endotracheal tube, a supraglottic airway device, a ventilator adaptive cap, a dilator, a tracheostomy device, a nasal trumpet, a an oral airway, an esophageal stethoscope, a laryngoscope, a speculum, a nasal cannula, a feeding tube, a suction tube, a suction catheter, and an endotracheal changing tube; and wherein the visualization device com-

prises a camera tube with a distal end and proximal end, the distal end being sealed with a transparent material and a camera being placed inside of the camera tube through an opening at the proximal end. These medical devices can be further equipped with at least one of the following a bougie, a flexible stylet and a sound- and temperature-monitoring device. In some embodiments, the visualization device is sealed, attached or otherwise connected externally to the second device. In other embodiments, the visualization device can be placed inside of the second device. Various endotracheal tubes equipped with the visualization device are contemplated as well, including an endotracheal tube which comprises a sleeve through which the visualization device can be inserted, an endotracheal tube into which the visualization device is placed internally through a ventilator adaptive cap and an endotracheal tube to which the visualization device is attached externally.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A, 1B and 1C depict a side view of an embodiment for a visualization device as shown in FIG. 1A which can be further equipped with a stylet as shown in FIGS. 1B and 1C.

FIG. 2 depicts a side view of an embodiment for an endotracheal device equipped with a visualization device.

FIG. 3 depicts a side view of an alternative embodiment for an endotracheal device equipped with a visualization device.

FIGS. 4A and 4B depict two embodiments showing a visualization device attached to a built-in ventilator adaptive cap. FIG. 4A is an embodiment without a light source and FIG. 4B is an embodiment with a light source.

FIGS. 5A, 5B and 5C depict side views of further embodiments of a visualization device attached to a built-in ventilator adaptive cap and delivered through a sliding sleeve (FIGS. 5A and 5B), with further embodiment in FIG. 5C which includes a bougie or a flexible stylet as shown in the insert.

FIGS. 6A and 6B depict side views of an embodiment for an endotracheal device equipped with a visualization device delivered through a sliding sleeve.

FIGS. 7A and 7B depict side views of an alternative embodiment for an endotracheal device equipped with a visualization device and delivered through a sliding sleeve.

FIG. 8 is a side view of an embodiment for an endotracheal device equipped with a bougie.

FIGS. 9A, 9B and 9C are a side view of a visualization device equipped with rings. FIG. 9A is a side view of a visualization device equipped with two rings. FIG. 9B is a side view of the visualization device as shown in FIG. 9A, but equipped further with a bougie. FIG. 9C is a side view of the visualization device as shown in FIG. 9A, but equipped further with a light source. FIG. 9D is a cross-sectional view through the visualization device of FIG. 9A showing a ring connected to the camera tube. FIG. 9E is a cross-sectional view through the visualization device of FIG. 9A showing an adjustable sliding ring with a clasp connected to the camera tube. FIG. 9F is a side view of an endotracheal tube to which the visualization device of FIG. 9A is connected with two sliding rings.

FIG. 10 is a side view of a supraglottic airway device equipped with a visualization device. An endotracheal device of FIG. 3 is shown as an insert on the left and a flexible guided stylet is shown as an insert on the right.

FIGS. 11A and 11B depict a side view of an alternative airway device with a visualization device. FIG. 11A is a side

view of the airway device and FIG. 11B is the device as shown in FIG. 11A, but with a ventilator adaptive cap.

FIGS. 12A, 12B and 12C depict an oral airway intubating device with a visualization device. FIG. 12A is a side view of the oral airway device, while FIGS. 12B and 12C are cross-sections through the airway device in its full cylinder form (FIG. 12B) and in its half-cylinder form in which one half-cylinder is retracted into the other half-cylinder (FIG. 12C).

FIG. 13 depicts a side view of a dilator with a visualization device.

FIGS. 14A and 14B depict a side view of a tracheostomy device with a visualization device. FIG. 14A depicts an embodiment in which the visualization device is attached externally to a tracheostomy tube, while FIG. 14B depicts an embodiment in which the visualization device is attached inside of the tracheostomy tube.

FIG. 15 depicts a side view of a nasal trumpet with a visualization device.

FIGS. 16A-16C depict a side view of an oral airway equipped with a visualization device and FIG. 16D depicts an intubating oral airway also equipped with a visualization device. FIG. 16A shows a visualization device being positioned inside of the oral airway. FIG. 16B is the same as FIG. 16A, but includes a light source for the visualization device. FIG. 16C is the same as FIG. 16A, but includes a whistle. FIG. 16D is an intubating oral airway with a main lumen into which an endotracheal tube can be placed.

FIGS. 17A and 17B depict a side view for an esophageal stethoscope equipped with a visualization device and working tube and bougie tube.

FIGS. 18A-18B depict a side view for a one-piece laryngoscope with a visualization device. FIG. 18A shows a laryngoscope with a visualization device, and FIG. 18B is the same, except it is further equipped with a bougie and the visualization device is equipped with a light source.

FIG. 19 depicts a side view of a speculum with a visualization device.

FIG. 20A-F depict a nasal cannula with a visualization device. FIG. 20A depict positioning of the cannula on a patient's head and FIG. 20B is the same as in FIG. 20A, except the visualization device is equipped with a light source. FIG. 20C is a side view of the cannula of FIG. 20A, and FIG. 20D is a side view of the cannula of FIG. 20B. FIG. 20E is a cross-sectional view of a patient's head with the cannula of FIG. 20A inserted. FIG. 20F is a further embodiment in which a nasal cannula with a visualization device as shown in FIG. 20A is further combined with an external stethoscope.

FIG. 21 is a feeding tube equipped with a visualization device.

FIG. 22A, 22B, 22C depict various embodiments of a suction tube equipped with a visualization device. FIG. 22A depicts a visualization device positioned inside of the suction tube. FIG. 22B the same as in 22A, but equipped further with a bougie, and FIG. 22C is the same as FIG. 22B, but showing the bougie protruding from the distal end of the suction tube.

FIG. 23 depicts a suction catheter equipped with a visualization device.

FIG. 24 depicts an endotracheal changing tube equipped with a visualization device.

DETAILED DESCRIPTION

The present invention provides improved medical devices equipped with a visualization device for intubation, venti-

lation, feeding and monitoring of a patient. The present invention also provides methods for rapid and accurate placement of a medical device in a patient and remote continuous real-time monitoring of the patient after the placement.

These medical devices are equipped with a visualization device in which a camera is placed in a separate sealed camera tube. As the camera does not come in contact with a patient, there is no need to sterilize the camera and the same camera can be reused in many applications. Thus, the same camera can be switched between different medical devices which monitor internal organs such as medical devices that are placed in patient's airway, larynx, gastrointestinal tract, chest or vaginal cavity.

One embodiment provides a visualization device as shown in FIG. 1A and its further embodiments as shown in FIGS. 1B and 1C. A visualization device, generally 10, in FIG. 1A comprises a camera tube 12 with a distal end 14 and a proximal end 16. The camera tube 12 can be a plastic tubing. In some embodiments, the camera tube 12 may comprise a fiber-optic material. The camera tube 12 is sealed at the distal end 14 with a transparent material 17. The diameter of camera tube 12 is designed in such a way that a camera 18 with wire 20 can be inserted inside of the camera tube 12 through an opening at the proximal end 16 and moved down the camera tube 12 toward the distal end 14, so that the camera 18 transmits continuously images obtained through the transparent material 17. The length of the camera tube 12 can vary and it can be adjusted dependent on the length of a medical device with which the visualization device is to be used. For example, the length of the camera tube 12 may be longer when the visualization device 10 is used with a feeding tube in comparison to the length of the camera tube 12 when the visualization device 10 is used with an endotracheal tube. In some embodiments, the visualization device obtains images and transmits wirelessly, broadcasts or records this information to at least one device positioned at a remote location.

Because the camera tube 12 is sealed at the distal end 14 with the transparent material 17, the camera 18 does not come in contact with patient's tissues or fluids and therefore, the camera 18 does not have to be sterilized or to be disposable, and it can be reused in further applications. However, the camera 18 can be disposable in some applications. The camera 18 can be loaded with a chip and equipped to obtain and transmit digital images in real time. The camera 18 is further connected by an electric wire 20 to an image receiving and processing device (not shown) such as a computer equipped with a monitor or a computer network. The camera 18 may also be in communication wirelessly with an image-receiving device located at any location, including multiple locations and remote locations. Because the length and diameter of the camera tube 12 can be adjusted based on patient's needs, the visualization device 10 is suitable for a broad variety of patients, including pediatric patients and adult patients with abnormal anatomy or trauma.

As the visualization device 10 is bendable and flexible, the visualization device 10 is easy to insert in a patient and remove from the patient. The camera 18 may have its own light source. As the visualization device 10 transmits images from a patient in real time, it can be used for guiding a medical device for proper placement. Thus, some embodiments are concerned with methods for rapid and accurate placement of a medical device inside of a patient, including a method for guided and rapid placement into patient's

airway, larynx, gastrointestinal tract, chest or vaginal cavity under continuous visualization.

As shown in embodiment of FIG. 1B, the visualization device 10 can be further equipped with a stylet 22 which can be sealed onto or otherwise attached to the camera tube 12 externally on at least one side of the camera tube 12 along the proximal-to-distal (16-14) axis of the camera tube 12. The stylet 22 can be made of metal wire or some other sturdy material with the purpose to keep the otherwise flexible visualization device 10 in a particular shape. In some embodiments, the stylet 22 can be of the same length as the camera tube 12. In other embodiments, the stylet 22 is shorter than the camera tube 12 such that at least a portion of the camera tube 12 on either the proximal end 16 or distal end 14, or on the both ends 16 and 14 is not in contact with the stylet 22. As shown in FIG. 1C, the stylet 22 can be bent into various shapes and it retains the shape into which it has been bent, which permits for visualization device 10, which is otherwise flexible, to retain a particular shape.

In alternative embodiments, the visualization device 10 can be equipped with a bougie which can be attached to the camera tube 12 externally on at least one side of the camera lumen 12 along the proximal-distal (16-14) axis of the visualization device 10.

The bougie can be made of various materials, including plastic material which is bendable. As the bougie is bendable, but keeps a shape into which it is bent, the bougie is suitable for guiding the visualization device 10 inside of a patient. In some embodiments, the bougie can be of the same length as the camera tube 12. In other embodiments, the bougie can be made shorter or longer than the camera tube 12 such that only a portion of the camera tube 12 is in contact with the bougie. In some embodiments, the bougie protrudes on at least the distal end 14.

The visualization device 10 can be further equipped with a portable light source (not shown) which can be either built-in the camera 18 or it can be built-in the camera tube 12. In alternative, a light source can remain outside the camera tube 12 on the proximal end 16, but still be placed such that the light source sheds light inside of the camera tube 12.

In embodiments of FIGS. 1A-1C, the camera tube 12 can be disposable, while the camera 18 is reusable without the need of sterilization. However, the camera 18 can be also disposable in at least some embodiments.

During placement in a patient, a visualization device 10 either alone or in combination with another medical device is positioned such that it is inserted with its distal end 14 in the patient under continuous visualization with the camera 18.

Any of the visualization devices 10 described above can be attached, sealed or otherwise connected to a disposable or non-disposable medical device either externally or internally and as described in more detail below. Various medical devices for pediatric and adult patients can be built such that the camera device tube 12 is sealed or attached to the medical device during manufacturing.

In other embodiments, the visualization device 10 can be sold as a kit which can be attached by a medical practitioner to a pre-made medical device for pediatric and adult patients, based on a particular patient's individual needs. The length of the camera tube 12 can vary such that the camera tube 12 is of the same or similar length with a medical device to which the visualization device 10 is sealed, attached or otherwise connected to.

Having the ability to verify placement for a medical device in real time from near and far allows several experts

to assist and verify placement. This is accomplished by equipping the medical device with the visualization device 10. In some embodiments, a method is provided in which the visualization device 10 is used for placing a medical device in a patient in ambulances, on battlefields, in nursing homes or hospitals. The visualization device 10 provides the ability to monitor in real time a patient. Because the visualization device 10 may interact with a plethora of devices disposable and otherwise, the use of the device 10 on various medical devices provides for a method in which a medical practitioner can customize a proper device for each patient or situation. Having the same camera equipment that can interact with various medical devices provides economy of scale such that even the smallest of organizations can have all the proper vigilance and technology.

At least in some embodiments the visualization device 10 can be used in assembly with at least one medical device as described in more detail below. A method in which the visualization device 10 is used on an airway device allows continuous visualization of any of the following in a patient in real time: nasopharynx, pharynx/hypo pharynx, supraglottic structures, airway, internal organ anatomy, vocal cords during normal and abnormal ventilation. This method also allows detection of abnormal anatomy and abnormal vocal cord movements.

Referring to FIG. 2, this embodiment provides an endotracheal device, generally 30. The endotracheal device 30 comprises an endotracheal tube 32 with a distal end 32A and a proximal end 32B. The visualization device 10 is sealed or otherwise attached externally on at least one side of the endotracheal tube 32, along the proximal-distal (32B-32A) axis of the endotracheal tube 32. The visualization device 10 comprises essentially of all elements as shown in FIG. 1A, with the camera 18 inserted inside of the camera tube 12 through an opening at the proximal end 16 of the camera tube 12, all the way down to the distal end 14 and the opening of the distal end 14 being sealed with the transparent material 17. Because the camera 18 is positioned inside of the sealed camera tube 12, the camera 18 does not come into contact with a patient and the camera 18 does not need to be sterilized and can be reused in multiple applications. Thus, the camera 12 does not have to be disposable or to be sterilized before further applications. However, the camera 18 can be disposable in at least some applications.

As the camera 18 is contained inside of the separate camera tube 12 which is positioned externally on the endotracheal tube 32, a diameter of the camera tube 12 is not limited by a diameter of the endotracheal tube 32. Thus, the diameter of the camera tube 12 can be larger or smaller than the diameter of the endotracheal tube 32.

Thus, the visualization device 10 can be used on endotracheal devices for pediatric patients and patients with abnormal anatomy. In some embodiments, the visualization device 10 has a diameter larger than that of the endotracheal tube 32.

The camera 18 is connected by electric wire 20 to an external device such as a computer and monitor (not shown). At least in some embodiments, the visualization device 10 is further equipped with a light source 21. The light source 21 can be kept outside of the camera tube 12, but in proximity with the proximal end 16 of the visualization tube 12 so that the light source 21 sheds light inside of the camera tube 12. In alternative embodiments, the light source 21 can be built-in the camera tube 12 or in further embodiments, the light source 21 can be built-in the camera 18.

At least in some applications, the camera 18 is a digital camera equipped with a chip and it collects and transmits

images continuously. The camera 18 can be connected wirelessly or hard-wired with a computer network (not shown) which collects and analyzes images obtained by the camera 18. This arrangement permits for remote, continuous and real time monitoring of the endotracheal device 30 during placement and after-placement in a patient. Thus, an accurate and rapid placement of the endotracheal device 30 can be achieved. Further and because the visualization device 10 continues to acquire images after the endotracheal device 30 is placed inside of a patient, the patient can be monitored in real time for adverse reactions such as bleeding, airway obstruction, shifting or malfunctioning, etc. of the endotracheal device 30 and other reactions. The endotracheal device 30 may continue to transmit images and information for as long as it remains in a patient.

In some embodiments, the endotracheal tube 32 is further fitted with a cuff 34 at its distal end 32A. In other embodiments, the endotracheal tube 32 is not fitted with the cuff 34. The cuff 34 can be inflated with a device 36 after the endotracheal device 30 is placed in a patient and its proper positioning inside of the patient is verified by images obtained with the visualization device 10.

The endotracheal device 30 can be further equipped with a sound-monitoring device 38 which is sealed onto or otherwise attached externally on one side of the endotracheal tube 32 along the proximal-distal axis (32B-32A) of the endotracheal tube 32. The sound-monitoring device 38 can be a microphone placed inside of a plastic tube 40. It monitors heart beats and breathing tones and can be connected by wire or wirelessly to a remote device which collects and monitors patient's vital signals. In the embodiment of FIG. 2, the visualization device 10 is placed proximally to the cuff 34 and externally to the endotracheal tube 32. It will be understood that the endotracheal device 30 can be built with any endotracheal tube 32, including single-lumen and double-lumen tubes. The endotracheal device 30 can be used for either pediatric or adult patients. The endotracheal device 30 can be made in various sizes.

In another embodiment and as shown in FIG. 3, an endotracheal device, generally 50, comprises an endotracheal tube 52 with a distal end 52A and a proximal end 52B, and a visualization device 10 placed inside of the endotracheal tube 52 through an opening in the proximal end 52B. In this embodiment, the visualization device 10 is attached to a built-in ventilator adaptable cap 68 which connects the endotracheal device 50 to a ventilator (not shown) through an outlet 70. The built-in ventilator adaptable cap 68 comprises an opening 72 through the cap 68. The visualization device 10 is passed through the opening 72 and is placed inside of the endotracheal tube 52. The built-in ventilator adaptable cap 68 is then connected with the endotracheal tube 52 at the proximal end 52B of the endotracheal tube 52.

The visualization device 10 is the same as the visualization device 10 of FIG. 1A and it comprises a camera tube 12 with a sealed distal end 14 and an open proximal end 16. A camera 18 is placed inside of the camera tube 12 through the proximal end 16 of the camera tube 12. The camera 18 is connected by electrical wire 20 to an image-monitoring device (not shown). In some embodiments, the camera 18 is connected wireless to an image-monitoring device (not shown). The camera 18 collects images continuously and in real time through a transparent material 17 with which the distal end 14 of the camera tube 12 is sealed. The images can be transmitted to a remote location.

The endotracheal tube 52 can be optionally equipped with a cuff 64 at the distal end 52A such that the cuff 64 wraps around the endotracheal tube 52 and the cuff 64 can be

inflated with a device **65**, once the endotracheal device **50** is properly placed inside of a patient's airway. As can be seen from FIG. **3**, the distal end **14** of the visualization device **10** extends distally from the distal end **52A** of the endotracheal tube **52** and below the cuff **64** such that even when the cuff **64** is inflated with a device **65** after placement in a patient, the visualization device **10** can still record images inside of a patient's body and below the cuff **64**. Further, the endotracheal device **50** may have an elliptical opening **67** at the distal end **52A** and the visualization device **10** can be positioned inside of the endotracheal tube **52** such that the distal end **14** of the visualization device **10** aligns with or is in close proximity with the elliptical opening **67** of the endotracheal tube **52**.

Referring to FIGS. **4A** and **4B**, further embodiments provide a visualization device **10** assembled with a built-in ventilator adaptable cap **68** which connects to a ventilator (not shown) by an outlet **70**. The visualization device **10** is inserted through an opening **72** in the built-in ventilator adaptable cap **68** as shown in FIGS. **4A** and **4B**. As shown in FIG. **4B**, the visualization device **10** can be further equipped with a light source **74** which can be a part of the camera tube **12** or it can be built in the camera **18**, or it can remain outside the built-in ventilator adaptable cap **68**. The visualization device **10** is assembled with the built-in ventilator adaptable cap **68** as shown in FIGS. **4A** and **4B** and can be then used in an endotracheal tube as described in connection with FIG. **3** or in a supraglottic device or with a laryngeal mask or with any other medical device to which a built-in ventilator adaptable cap **68** can be attached. As shown in FIGS. **4A** and **4B**, the camera tube **12** has a distal end **14** and a proximal end **16**. The camera **18** is placed inside of the tube **12** through an opening in the proximal end **16** and moved all the way down to the distal end **14** which is sealed with a transparent material **17**. The camera **18** collects images through the transparent material **17** and transmits the images in real time to a monitoring device which can be located remotely.

Further embodiments for a built-in ventilator adaptable cap **68** equipped with a visualization device **10** are shown in FIGS. **5A**, **5B** and **5C**. As can be appreciated from FIG. **5A**, the visualization device **10** comprises the camera **18** inside of the camera tube **12**. The visualization device **10** is inserted through the ventilator adaptable cap **68**. As shown in the embodiment of FIG. **5A**, a plastic clear sleeve **76** can be attached over the adaptable cap **68** such that the sleeve **76** can slide up and down as shown in FIGS. **5A** and **5B** in the proximal-distal direction, which allows the visualization device **10** to remain sterile during insertion and removal. As the visualization device **10** is inserted and removed through the sleeve **76**, the visualization device **10** remains sterile and free of contamination. The sleeve **76** is long enough to maintain the whole visualization device **10** outside the ventilation cap and remain sterile. A further embodiment is shown in FIG. **5C** in which the visualization device **10** is inserted through the sleeve **76** as shown in FIGS. **5A** and **5B**, except a bougie **78** is added through a bougie tube **80**.

The bougie **78** can be replaced with a flexible guided stylet **82** as shown in the insert to FIG. **5C** which rotates and guides a stylet inside of a patient, which is protected from patient's tissues. If the tube **80** is used with a stylet, then the tube **80** has to be sealed at the distal end. Additional tubes can be attached and placed through the sleeve **76**. Such tubes include, but are not limited to a suction tube and a tool tube which can be used for delivering biopsy forceps and other tools. The assembly of the built-in ventilator adaptable cap **68** and visualization device **10** with the sleeve **76** can be

used with any medical device to which a built-in ventilator adaptable cap can be attached, including an endotracheal tube as described in connection with FIG. **3**, a supraglottic device or with a laryngeal mask airway. If an embodiment with a bougie or stylet is used as described in connection with FIG. **5C**, the bougie **78** can protrude distally or slide independently from a medical device and guide the medical device movement inside of a patient during placement under visualization with the visualization device **10**.

Further embodiments for an endotracheal device equipped with a visualization device, generally **84**, are shown in FIGS. **6A** and **6B**. As can be appreciated from FIG. **6A**, the visualization device **10** which comprises the camera **18** inside of the camera tube **12** can be inserted inside of an endotracheal tube **86** through an opening **87** on one side of the endotracheal tube **86**. As shown in the embodiment of FIG. **6A**, a plastic sleeve **92** can be attached over the opening **87** such that the sleeve **92** can slide up and down as shown in FIGS. **6A** and **6B**, which facilitates keeping the visualization device **10** sterile while it is moved in or out of the endotracheal tube **86**. As the visualization device **10** is inserted and removed from the endotracheal tube **86** through the sleeve **92**, the visualization device **10** remains sterile and free of contamination. The visualization device **10** can be removed entirely from the endotracheal tube **86** through the sleeve **92** and remain sterile. The endotracheal tube **86** may be equipped with a cuff **88** positioned near the distal end **86A**. The visualization device **10** can move inside the endotracheal tube **86** along the proximal-distal (**86B-86A**) axis such that the visualization device **10** is distal to the cuff **88** or the visualization device **10** can protrude outside the endotracheal tube **86** distally as shown in FIG. **6B**. This permits for obtaining images from a patient with the visualization device **10** after the cuff **88** is inflated with a device **90** and obtaining the images from the area in a patient's body which is distal to the cuff **88**. This distal to the cuff **88** area is available for monitoring after the cuff **88** is inflated because of the visualization device **10** in which the camera **18** collects images through the transparent material **17** at the distal end **14**.

In this embodiment, the visualization device can slide up and down inside of an endotracheal tube, which permits advancement and retraction of the camera tube **12** while maintaining sterility of an endotracheal tube into which the visualization device **10** can be inserted as described above. The camera **18** can be easily advanced inside of the camera tube **12** and provide inspection of the endotracheal tube through its length as well as distal to the tip of the endotracheal tube.

Further embodiments for an endotracheal device, generally **100**, equipped with a visualization device **10** are shown in FIGS. **7A** and **7B**. Additional tubes can be attached to the tube **10** or be placed adjacent to the tube **10**. Such tubes include, but are not limited to a suction tube, a tube for delivering instruments such as forceps, a bougie or flexible stylet. As can be appreciated from FIG. **7A**, the visualization device **10** comprises the camera **18** inside of the camera tube **12** positioned externally on the endotracheal tube **102** and along the proximal-distal (**102B-102A**) axis. As shown in the embodiment of FIG. **7A**, a plastic sleeve **108** can be attached to the endotracheal tube **102** such that the sleeve **108** can slide up and down outside the endotracheal tube **102** as shown in FIGS. **7A** and **7B**, which facilitates the movement of the visualization device **10** along the proximal-distal (**102B-102A**) axis of the endotracheal tube **102**. As the visualization device **10** is inserted and removed through the sleeve **108**, the visualization device **10** remains sterile and

free of contamination. The endotracheal tube **102** may be equipped with a cuff **104** wrapped around the endotracheal tube **102** near its distal end **102A**. The visualization device **10** moves outside the endotracheal tube **102** along the proximal-distal axis **102B-102A** such that the visualization device **10** can be proximal to the cuff **104**. This also permits for obtaining images from a patient with the visualization device **10** after the cuff **88** is inflated with a device **106**. The camera tube **12** can slide proximal or distal of the cuff **104**. Thus, at least in some embodiments, the camera tube **12** would be into a sealed tunnel.

FIG. **8** depicts a further embodiment of an endotracheal device, generally **110**. The device **110** can be equipped with the visualization device **10** and the sound tube **40** described in connection with FIG. **2** (not shown). The endotracheal device is further equipped with a bougie **116** which can slide up and down along the proximal-distal (**116B-116A**) axis inside of a tube **118** which is attached externally to the endotracheal tube **111**. The endotracheal tube **111** is equipped with a cuff **112** located in proximity to a distal end **110A** of the tube. The cuff **112** can be inflated with a device **114** after the endotracheal device **110** is placed inside of a patient. The visualization device **10** can be sealed or attached to the endotracheal tube **111** either outside or inside as described above in connection with embodiments provided by FIGS. **2**, **3**, **4A**, **4B**, **5A**, **5B**, **6A**, **6B**, **7A** and **7B**. The bougie **116** guides the movement of the endotracheal device **111** during placement in a patient under visualization with the visualization device **10** and permits guided sliding down the medical device over the bougie **116** inside of the patient's airway.

Further embodiments of a visualization device, generally **120**, are shown in FIGS. **9A-9C**. As shown in FIG. **9A**, the camera tube **12** can be equipped with at least one, and preferably two external rings **122** which are sealed or otherwise connected by means **124** to the camera tube **12**. In some embodiments, one ring **122** is positioned at about $\frac{1}{3}$ of the camera tube length from the proximal end **16** and the other ring is positioned at about $\frac{2}{3}$ of the camera tube length from the proximal end. While in the embodiment of FIG. **9A**, the camera tube **12** is equipped with two rings **122**, other embodiments include those in which more than 2 rings are used or only one ring is used. The positioning of the rings along the proximal-distal (**16-14**) axis of the camera tube **12** can also vary. Other modalities include a clasp or a plastic band to hold the camera tube **12**.

As in all other embodiments, the camera tube **12** has a distal end **14** sealed with a transparent material **17** and a proximal end **16** with an opening through which a camera **18** is inserted into the camera tube **12**. As shown in FIG. **9B**, the visualization device **120** can be further equipped with a tube **118** sealed or otherwise attached externally along the proximal-distal (**16-14**) axis of the camera tube **12**. A bougie **116** is placed inside of the tube **118** such that a distal end **116A** of the bougie **116** protrudes distally over the camera tube **12**, while its proximal end **116B** extends outside the visualization device **120** proximally and can be used by a medical provider to rotate the distal end **116A** and in this way guide the movement of the visualization device **120** along with a medical device to which it is attached.

As shown in FIG. **9C**, the visualization device **120** can be further equipped with a light source **21** which can be either built in the camera tube **12**, built in the camera **18** or it can be kept outside the visualization device **120** and outside the patient's body. The visualization device **120** is attached to a medical device with the rings **122**, and this permits for

customized positioning of the visualization device **120** as it can slide up and down along a proximal-distal axis of a medical device.

As shown in a cross-sectional view in FIG. **9D**, the ring **122** can be of any diameter in order to fit on a medical device of choice. As shown further in FIG. **9E**, at least in some embodiments the ring **122** may have a clasp **126** such that the diameter of the ring **122** can be adjusted according to a diameter of a medical device to which the visualization device **120** is attached with the rings **122**.

An embodiment as shown in FIG. **9F** provides an assembly, generally **128**, in which the visualization device **120** is attached with the rings **122** to an endotracheal tube **52**. The rings **122** can slide up and down along the proximal-distal (**52B-52A**) axis of the endotracheal tube **52**, and in this way the position of the visualization device **120** can be adjusted with respect to the endotracheal tube **52**. Further, the rings **122** can rotate around the endotracheal tube **52**, which permits altering the positioning of the camera device **120** if images are needed from a different area inside of a patient.

Because the rings **122** can be adjustable, the visualization device **120** can be used with an endotracheal tube of any size, including those for pediatric patients. Further, the visualization device **120** with at least two rings connected externally to the camera tube **12** can be provided as a kit, and a medical practitioner can assemble the visualization device with any conventional endotracheal tube or any other conventional medical device for which visualization and monitoring are needed at the time of treatment.

Further embodiments provide an intubation method in which an endotracheal tube, including any of the endotracheal tubes described above and equipped with the visualization device as described above, is placed in patient's airway and positioned under the patient's vocal cords under constant visualization by the visualization device **10**.

Referring to FIG. **10**, it depicts a side view of a supraglottic airway device, generally **130**. Any standard endotracheal tube known in the art and an endotracheal device of FIG. **3** is shown in the insert on the left of FIG. **10** can be used in combination with the supraglottic airway device **130**.

The supraglottic airway device **130** comprises a supraglottic tubal body **131** with a distal end **131A** and a proximal end **131B** and a lumen **146**. The supraglottic airway device **130** includes a designated intubation tube **133** which is inserted into the lumen **146** and into which an endotracheal device **50** can be placed as shown in FIG. **10**. The distal end **133A** of the intubation tube **133** ends with an elliptical opening **140** which is located distally from a cuff **132** which can be inflated with a device **134**. The intubation tube **133** has a plurality of holes **148** distributed throughout its body to allow ventilation from outlet **144** through tubal body **131**.

While a standard endotracheal device, including an endotracheal device **50**, may be equipped with a visualization device, the supraglottic airway device **130** comprises its own visualization device **10** which is placed in the lumen **146**. The visualization device **10** comprises a camera tube **12** with a distal end **14** and a proximal end **16**. The distal end **14** is sealed with a transparent material **17**. The camera tube **12** is sealed or otherwise attached externally to the intubation tube **133** along the proximal-distal (**131B-131A**) axis. The supraglottic device **130** can be further equipped with a bougie **116** which is located inside of the tube **118**. The tube **118** is placed inside of the lumen **146** and such that the distal end **116A** of the bougie **116** protrudes from the tube **118** and outside the supraglottic tubal body **131** through an elliptical opening **142** which is located on the supraglottic tubal body

131 slightly proximally from the distal end 131A. The elliptic opening 142 of the supraglottic tubal body 131 overlaps partially with the elliptic opening 140 of the intubation tube 133. The bougie tube has its own opening through 140.

At the distal end 131A, the tubal body 131 is capped with a balloon 136 which can be inflated with a device 138. In some embodiments, the bougie 116 can be replaced with a flexible guided stylet 82 shown on the right of FIG. 10.

In addition to the visualization device 10, the supraglottic device 130 can be also equipped with a sound- and temperature-monitoring device 38 which is located inside a tube 40 which is sealed or otherwise attached externally to the tubal body 131 along the proximal-distal (131B-131A) axis. The sound device 38 can monitor patient's heart beat and breathing after the supraglottic device 130 is placed inside of the patient. On its proximal end 131B, the tubal body 131 may be connected to a ventilator (not shown) though an outlet 144. Because the supraglottic device 130 can ventilate in a closed circuit through the tubal body 131, an endotracheal tube 50 can be placed inside of the intubation tube 133 without the need to stop ventilation and therefore, the supraglottic device 130 provides continuous ventilation, continuous visualization in real time through the visualization device 10 and continuous sound and temperature monitoring by the sound monitoring device 38 with a temperature probe. This real time information can be transferred or stored to multiple distant monitoring sites.

Other advantages for the supraglottic airway device include the ability to intubate, extubate and to easily reintubate if needed under continuous ventilation and the ability to continuously visualize vocal cords and supraglottic structures. The device 130 is suitable for applications in children and adults. Further, the device 130 is equipped with the cuff 132 for blocking the pharynx and the balloon 136 which blocks the esophagus after the device 130 is placed in a patient. Furthermore, an endotracheal tube can be placed just proximal to the vocal cords in the tubal body 133. This permits ventilation through 144 and tubal body 131 uninterrupted.

Referring to FIGS. 11A and 11B, an alternative embodiment for an airway device, generally 150, is provided. This device can be used in pediatric and adult patients as it is adoptable to different sizes. It provides continuous visualization of supraglottic structures and it can be advanced, retracted, or rotated, side to side to provide direct visualization of vocal cords. As can be appreciated from FIGS. 11A and 11B, the airway device 150 comprises a tubal body 152 with a distal end 152A and a proximal end 152B and a lumen 153. The tubal body 152 may be connected to a ventilator through an outlet 154. A visualization device 10 is sealed or otherwise attached inside of the tubal body 152 along the proximal-distal (152B-152A) axis on at least one side. The visualization device 10 comprises a camera tube 12 with a distal end 14 and a proximal end 16. The camera tube 12 is sealed at the distal end 14 with a transparent material 17. The proximal end 16 of the camera tube 12 remains open and a camera 18 is inserted in the camera tube 12 through the proximal end 16. The camera 18 does not come in contact with a patient's body and it does not have to be sterilized, it does not have to be disposable, although it may be disposable in at least some applications. The visualization device 10 can be further equipped with a light source which can be built in the camera tube 12 or be a part of the camera 18. In alternative, a light source may be left

outside the camera tube 12, but still shed enough light inside of the camera tube 12 for the camera 18 to obtain images inside of a patient's body.

An intubation tube 156 is placed inside of the lumen 153 of the tubal body 152 along the proximal-distal (152B-152A) axis. The intubation tube 156 shares a lumen 119 with a bougie 116 which is inserted inside the lumen 119 along the proximal-distal (152B-152A) axis such that a distal end 116A of the bougie 116 may protrude outside the tubal body 152 at the distal end 152A and proximal end 116B may protrude outside the tubal body 152 and the proximal end 152B can be used by a medical practitioner to guide the movement of the airway device 150 with the bougie 116 during placement in a patient, including advancing the bougie 116 through patient's vocal cords under direct visualization by camera 18. The intubation tube 156 has a plurality of holes 157 distributed along the intubation tube 156.

At least in some embodiments, the airway device 150 is further equipped with a sound- and temperature-monitoring device 38 which can be inserted in a tube 40 which is sealed or otherwise attached inside of the tubal body 152 along the proximal-distal (152B-152A) axis such as the distal end of the sound-monitoring device 38 is positioned at or near the distal end 152A of the tubal body 152, which is also equipped with a cuff 158 along the perimeter of the tubal body 152 at the distal end 152A. The intubation tube 156 is designed such that at least in some embodiments the intubation tube 156 has a ramp 160 at the distal end 152A of the airway device 150. A standard endotracheal tube, including those described in various embodiments above, can be placed inside of the lumen 119 in the intubation tube 156 for positioning in a patient.

As shown in FIG. 11B, a ventilator adaptable cap 68 and a lid 69 are attached to the tubal body 152 at the proximal end 152B. The endotracheal tube is inserted into the device 150 through the cap 68. Using the cap 68 with the lid 69 on the airway device 150 is preferred when ventilation is accomplished through an outlet 154.

Yet another embodiment for an oral airway device, generally 170, is provided as shown in FIGS. 12A, 12B and 12C. As can be appreciated from FIG. 12A, the airway device 170 comprises a tubal body 172 with a distal end 172A and a proximal end 172B. The tubal body 172 ends with two ramps 174 and 176 at the distal end 172B. As can be appreciated from a side view in FIG. 12A and cross-sectional views of the tubal body 172 in FIGS. 12B and 12C, the tubal body 172 is made of two half-cylinders 178 and 180. The half-cylinder 178 is slightly smaller in diameter than the half-cylinder 180. The tubal body 172 can be present in one of the two forms: as a full cylinder shown in FIG. 12B or as a half-cylinder as shown in FIG. 12C. The half-cylinder 178 and the half-cylinder 180 are connected by means such that the half-cylinder 178 can rotate and retract into the half-cylinder 180. The half-cylinder form of FIG. 12C is achieved by the half-cylinder 178 rotating at about 180 degrees and aligning with the half-cylinder 180 such that the half-cylinder 178 is located inside of the half-cylinder 180 as shown in FIG. 12C.

A visualization device, generally 10, is sealed or otherwise attached externally to the half-cylinder 180 along the proximal-distal (172B-172A) axis. The visualization device 10 comprises of a camera tube 12 with a distal end 14 and a proximal end 16. The distal end 14 is sealed with a transparent material 17. A camera 18 is placed through an opening at the proximal end 16 into the camera tube 12 and is moved inside the camera tube 12 to the distal end 14.

15

Similarly to all other embodiments, the camera **18** does not come in contact with a patient's body, and it does not have to be disposable, does not have to be sterilized and it can be reused in multiple devices. The camera **18** is connected with wire **20** to at least one monitoring device and it transmits images in real time. The camera **18** can be connected wirelessly to at least one monitoring device which can be positioned at some remote location. A light source can be added as described in connection with the visualization device in other applications.

The half-cylinder **180** ends in two ramps **174** and **176** at the distal end **172A**. The ramp **174** is smaller in size than the ramp **176** and the two ramps are superimposed over each other such as the smaller ramp **174** is proximal to a lumen **182** created by half-cylinders **178** and **180** when they are in the full-cylinder form as shown in FIG. **12B**, while the ramp **176** is distal to the lumen **182**. The ramps **174** and **176** are flexible and absorb the shock from sliding and releasing an endotracheal tube which can be delivered into a patient by the oral airway device **170**. The ramps also facilitate the removal of the oral airway device **170** after the endotracheal tube is placed inside of the patient.

As shown in FIG. **12A**, the oral airway intubating device **170** can be further equipped with a bougie **160** which can be inserted into a tube **118** along the proximal-distal (**172B-172A**) axis such that a distal end **116A** of the bougie **116** protrudes distally from the oral airway device **170** and a proximal end **116B** protrudes outside the oral airway device proximally and can be used to manipulate the distal end **116A** of the bougie **116** such that it guides the movement of the airway device **170** during placement in a patient. The bougie tube **118** is located on the smaller half-cylinder **178** and it shares the lumen **182** with the tubal body **172**.

A further embodiment provides a dilator with a visualization device, generally **190** in FIG. **13**. As can be appreciated from FIG. **13**, the dilator **190** comprises a tubal body **192** with a proximal end **192B** and a distal end **192A**. A certain distal portion of the tubal body **192** is tapered into a conical shape **192C** such that the opening at the distal end **192A** of the tubal body **192** is significantly smaller in diameter in comparison to an opening at the proximal end **192B**. A visualization device **10** is positioned inside of a lumen **195** of the tubal body **192** and along the proximal-distal (**192B-192A**) axis. The visualization device **10** may be sealed or otherwise attached inside of the tubal body **192**. The visualization device **10** is essentially the same device as shown in FIG. **1A**, and it comprises a camera tube **12** with a proximal end **16** and a distal end **14**. The distal end **14** of the camera tube **12** is in close proximity with the distal end **192A** of the tubal body **192**. A camera **18** which can be either disposable or reusable is placed inside of the camera tube **12** through an opening at the proximal end **16** and all the way down to the distal end **14** of the camera tube **12**, which is sealed with a transparent material **17**. Just like other embodiments, the visualization device **10** can be equipped with a light source located outside of the dilator **194** or built in the camera tube **12**. In some embodiments, the light source can be built in the camera **18**.

As shown in FIG. **13**, the camera **18** is connected by electrical wire **20** to a monitoring device (not shown). In some embodiments, the camera **18** can be in communication with a monitoring device wirelessly. A guide wire at the proximal end **194A** is positioned inside of the lumen **195** of the tubal body **192**. A proximate end **194B** of the guide wire **194** protrudes outside of the tubal body **192** at the proximal end **192B**. The visualization device **10** verifies appropriate placement of the dilator device **190** and allows mobility of

16

continuous visualization as dilation proceeds. The dilator device **190** is especially well suited for use with the Seldinger technique.

Further embodiments provide various tracheostomy tubes equipped with a visualization device. FIG. **14A** depicts a side view of an embodiment for a tracheostomy device, generally **200**. The device **200** comprises a tubal body **202** with a distal end **202A** and a proximal end **202B**. An inflatable cuff **204** is wrapped around the tubal body **200** in some proximity to the distal end **202A**, but never at the very distal end **202A**. The cuff **204** can be inflated with a device **206** after proper placement of the device **200** in a patient. At the proximal end **202B**, the tubal body **202** protrudes through a plastic plate **208** such that some portion of the tubal body **202** is proximal to the plastic plate and will remain outside of a patient's neck after the device **202** is positioned in the patient. The plastic plate **208** may be oval in shape with the tubal body **202** protruding from the plate in the middle of the oval plastic plate **208**. The plastic plate **208** may have two openings **209**, one on each side of the plate such that the device **200** can be secured around patient's neck with some bandage by tying the device **200** through the openings **209** around patient's neck.

In the embodiment of FIG. **14A**, the visualization device **10** is sealed or otherwise attached to the tubal body **202** externally. The visualization device **10** comprises a camera tube **12** which is sealed or otherwise attached externally along the proximal-distal (**202B-202A**) axis to the tubal body **202**. The camera tube **12** is placed under the cuff **204** such that the cuff **204** wraps over the camera tube **12** and a distal end **14** of the camera tube **12** is distal to the cuff **204**. The distal end **14** is sealed with a transparent material **17**. A proximal end **16** of the camera tube **12** protrudes through the plastic plate **208** and remains outside of patient's neck. A camera **18** can be placed inside of the camera tube **12** through an opening in the proximal end **16**. The camera **18** is not disposable, does not need to be sterilized and can be easily removed from the camera tube **12**. The camera **18** is connected by electrical wire **20** to a monitoring device. In further embodiments, the camera **18** can be in communication with a monitoring device wirelessly. A light source can be added to the visualization device **10** as was described in other embodiments above.

FIG. **14B** depicts another embodiment for a tracheostomy device, generally **210**. In this embodiment, the device **210** comprises of the same tubal body **202**, cuff **204**, plate **208** and other components as was discussed in connection with the device **200**. However, unlike the device **200**, a visualization device **10** is placed inside of a lumen **203** of the tubal body **202**. The visualization device **10** comprises a camera tube **12** with a distal end **14** and a proximal end **16**. The camera tube **12** may be sealed or otherwise attached internally to the tubal body **202** along the proximal-distal (**202B-202A**) axis such as the distal end **14** of the camera tube **12** is in close proximity with the distal end **202A** of the tubal body **202**. The distal end **14** is sealed with a transparent material **17**. A camera **18** is placed inside of the camera tube **12** through an opening at the proximal end **16** which remains outside of the patient's neck after the device **210** is placed in the patient. The camera **18** is connected by electrical wire **20** to a monitoring device. In other embodiments, the camera **18** communicates with a monitoring device wirelessly. In some embodiments, the visualization device **10** comprises a light source.

A further embodiment provides a nasal trumpet with a visualization device, generally **220** in FIG. **15**. The trumpet **220** comprises a tubal body **222** with a proximal end **222B**

17

and a distal end 222A. Two fasteners 224 are attached at the proximal end 222B of the tubal body 222. After placing the trumpet 220 in a patient, the proximal portion of the tubal body 222 with the fasteners 224 remains outside of the patient, and the fasteners 224 can be used to secure the trumpet 220 around the patient's head.

A visualization device 10 is sealed or otherwise attached to the tubal body 222 externally along the proximal-distal (222B-222A) axis. The visualization device 10 comprises a camera tube 12 with a proximal end 16 and a distal end 14. The distal end is in near proximity with the distal end 222A of the tubal body 222. The distal end 14 is sealed with a transparent material 17. A camera 18 is placed inside of the camera tube 12 through an opening at the proximal end 16. The camera 18 is moved all the way to the distal end 14 and collects images in real time inside of a patient's body during placement of the device 220 as well as after the device 220 has been properly placed and secured. As in other embodiments, the camera 18 does not come in contact with patient's body, does not have to be sterilized and can be reused in multiple devices or in different patients. The camera 18 communicates with a monitoring device (not shown) either with electrical wire 20 or wirelessly, or both.

Further embodiments provide various oral airways as shown in FIGS. 16A, 16B, 16C, and 16D. Referring to FIG. 16A, an oral airway with a visualization device, generally 230, comprises a tubal body 232 with a lumen 233. The tubal body is slightly curved in a hook-like shape along the proximal-distal (232B-232A) axis. A visualization device 10 is placed inside of the lumen 233 of the tubal body 232. The visualization device 10 comprises a camera tube 12 and a camera 18. The camera tube 12 may be sealed or otherwise attached internally to the tubal body 232 inside of the lumen 233 and along the proximal-distal (232B-232A) axis. The camera tube 12 has a proximal end 16 and a distal end 14. The distal end 14 is in close proximity with the distal end 232A of the tubal body 232. The distal end 14 is sealed with a transparent material 17.

The camera tube 12 has an opening at the proximal end 16 through which the camera 18 is inserted into the camera tube 12 all the way to the distal end 14. The camera 18 communicates with a monitoring device either wirelessly or by electrical wire 20. The embodiment shown in FIG. 16B is the same as in FIG. 16A, except a light source 21 is added to the visualization device 10. The light source 21 may remain outside of the camera tube 12 or it may be built in the camera tube 12 or it may be a part of the camera 18.

The embodiment shown in FIG. 16C is the same as that of the FIG. 16A, except two whistles 234A and 234B are added inside of the lumen 233 of the tubal body 232. The whistle 234B is located at the proximal end of the tubal body 232 and it produces a sound when a patient breathes in. The whistle 234A is located at the distal end of the tubal body 232 and it produces a sound when the patient breathes out.

Further embodiments include an oral airway as shown in FIGS. 16A-16C, but further equipped with a sound and temperature monitoring device which is also placed inside of the lumen 233 and transmits information to a monitoring device which can be positioned at a remote location.

The embodiment of FIG. 16D is an intubating airway device with a visualization device, generally 230. The intubating airway device 230 comprises a tubal body 232 with a lumen 233 in which an endotracheal tube can be placed. A visualization device 10 comprises a camera tube 12 with a distal end 14 and a proximal end 16. The distal end 14 is sealed with a transparent material 17. A camera 18 is placed inside of the camera tube 12 through an opening at the

18

proximal end 16. The camera tube 12 is placed inside the lumen 233 of the tubal body 232.

A bougie 116 is added inside of the tubal body 232 such that the bougie 116 is inserted in a tube 118 which shares the lumen with the lumen 233 along the proximal-distal (232B-232A) axis. A portion 116A of the bougie 116 protrudes outside the distal end 232A of the tubal body 232. A portion 116B of the bougie 116 protrudes outside the tubal body 232 from the proximal end 232B and over vocal cords. An endotracheal tube can be positioned inside the lumen 233 and the bougie 116 is used under constant visualization from the camera 10 to guide the placement of the endotracheal tube through patient's vocal cords. The distal end 14 of the camera tube 12 is in proximity with the distal portion 116A of the bougie 116 and therefore, the guided placement takes place under constant visualization.

Further embodiments provide an esophageal stethoscope with a visualization device. Referring to FIG. 17A, it depicts an esophageal stethoscope with a visualization device, generally 240. It comprises a body 242 with a lumen 243 into which a sound-monitoring device 246 is placed. The body 242 may have a cylinder-like shape tapered at the distal end, and with the distal end the body 242 protruding with a tongue-like tip 248. At least a portion of the body 242 surface is slightly curved toward the lumen 243 and creates a surface 249. The visualization device, generally 10, comprises a camera tube 12 with a distal end 14 which is sealed with a transparent material 17, and a camera 18 which is placed inside of the camera tube 12 through an opening at the proximal end of the camera tube 12. The camera tube is positioned externally on surface 249 along the distal-proximal axis of the body 242. The camera tube 12 is connected with the surface 249 by a sliding means 245 such that the camera tube 12 can slide along the 242A-242B axis on the surface 249.

The camera 18 is placed inside of the camera tube 12 and because the camera tube 12 is sealed at the distal end 14, the camera 18 does not come in contact with a patient and the camera 18 does not need to be sterilized and it can be reused in other applications. The camera 18 is connected by electric wire 20 or wirelessly to a monitoring device. The camera 18 is not disposable and can be reused in other applications.

The stethoscope 240 is further equipped with a bougie tube 244 which is also located on the surface 249 and is connected to the surface 249 with a sliding means 245 such that the bougie tube 244 can slide along the 242A-242B axis. FIG. 17B provides an alternative embodiment for the stethoscope 240, in which the sound and temperature monitoring device 246 can protrude through an opening at the 248 tip.

A further embodiment provides a one-piece video-laryngoscope with a visualization device, generally 250, as shown in FIGS. 18A and 18B. The video-laryngoscope 250 comprises a tubal body 252 which has a proximal end 252B and a distal end 252A. The tubal body 252 extends with a scoop-like portion 254 at the distal end 252A. The scoop-like portion 254 curves horizontally such that the distal end 254A of the scoop-like portion 254 is nearly parallel to the proximal end 254B of the scoop-like portion. The tubal body 252 has an opening 256 near its distal end 252A. A visualization device 10 which comprises a camera 18 placed inside of a camera tube 12 is placed through the opening 256 such that the distal end 14 of the camera tube 12 may be in proximity with the proximal end 254A of the scoop-like portion 254. The device can be easily inserted to an upper esophagus and visualize vocal cords.

However, the position of the distal end 14 can be adjusted as needed by sliding the camera tube 12 through the opening

256. The distal end 14 is sealed with a transparent material 17 such that the camera 18 does not come in contact with a patient's body and therefore, the camera 18 does not need to be sterilized and it can be reused in multiple applications. The camera 18 is inserted into the camera tube 12 through an opening at the proximal end 16. The camera 18 is connected to at least one monitoring device either by electrical wire 20 or wirelessly.

The embodiment of FIG. 18B is the same as that of FIG. 18A, except a light source 21 is added to the visualization device 10 as described in connection with the light source 21 in other medical devices above. A bougie 116 in a tube 118 is also added through the opening 256, and the distal end 116A of the bougie 116 can be manipulated at the proximal end 116B such that the placement of the device 250 is guided under continuous visualization with the camera 18.

A further embodiment includes a vaginal speculum with visualization device, generally 260 as shown in FIG. 19. Any speculum 261, including disposable, generally known and used for a pelvic exam can be equipped with a visualization device, generally 10, which comprises a camera 18 placed inside of a camera tube 12. The camera tube 12 can be attached to the speculum 261 or to some other instrument. The camera 18 is placed in the camera tube 12 through an opening at a proximal end 16 and is moved all the way toward the distal end 14 which is sealed with a transparent material 17. The camera 18 connected to at least one monitoring device by electric wire 20 or the camera 18 can be connected wirelessly.

Further embodiments relate to various tubing equipped with a visualization device shown in FIG. 1A and as described in more detail below.

FIGS. 20A-20F refer to various embodiments for a nasal cannula with a visualization device, generally 270. FIG. 20A shows the positioning of a nasal cannula 272 on patient's head with a visualization device 10 added to one of the two nostril tubes. The nasal cannula 272 can be any nasal cannula known in the art and used by medical practitioners. The visualization device 10 is as described in connection with FIG. 1A and comprises a camera 18 inserted inside of a camera tube 12. The camera tube 12 is sealed or otherwise attached externally along at least one nostril tube 274 of the nasal cannula 272 as shown in more detail in FIG. 20C. This nasal cannula with the visualization device 10 provides continuous visualization of vocal cords, upper esophagus. The cannula can be used to determine whether vocal cords are moving correctly, if there is any abnormal anatomy and the color of the patient's tissues.

As shown in FIG. 20E, the nasal cannula with the visualization device can be properly positioned through patient's nostrils as the positioning is guided and constantly visualized with the camera device 10. The distal end 14 of the camera tube 12 aligns with the distal end of at least one nostril tube 274. As shown in FIG. 20F, the nasal cannula with the visualization device can be further equipped with an external stethoscope 275, which can be placed on patient's chest externally and monitors breathing and heart-beat sounds.

FIGS. 20B and 20D show the same embodiment as in FIGS. 20A and 20C, except the visualization device 10 is equipped with a light source 21 as was described in connection with the light source 21 in other embodiments.

A further embodiment includes a feeding tube with a visualization device, generally 280, as shown in FIG. 21. A visualization device, generally 10, is sealed or otherwise attached externally along the proximal-distal (282A-282B) axis of a feeding tube 282. The visualization device 10 is

essentially the same as described in connection with FIG. 1A and other embodiments above. It comprises a camera tube 12 with a proximal end 16 and a distal end 14. A camera 18 with wire 20 is inserted into the camera tube 12 through an opening at the proximal end 16 and is slid all the way to the distal end 14 which is sealed with a transparent material 17. The camera 18 does not come in contact with a patient's body and can be reused in multiple devices. Any feeding tubes known in the art can be used in this embodiment, including a feeding tube with a stylet 284 as shown in FIG. 21. The feeding tube 282 can be equipped with an adaptor 283 at the proximal end 282A. The feeding tube 282 may further comprise a plurality of holes 285 at the distal end 282B for food distribution.

Further embodiments provide various suction tubes equipped with a visualization device, generally 290, as shown in FIGS. 22A, 22B and 22C. Any suction tube including but not limited to the nasal gastric tubes known in the art can be used and in general a suction tube 292 with an adaptor 293 at a proximal end 292B is suitable, as shown in FIG. 22A. A visualization device, generally 10, comprises a camera tube 12 and a camera 18 with wire 20. The camera 18 is inserted into the camera tube 12 through an opening at a proximal end 16 and is slid all the way to the distal end 14 of the camera tube 12. The distal end 14 is sealed with a transparent material 17. The camera 18 can transmit information to a remote location.

The camera tube 12 is placed inside of the suction tube 292 through an opening 294 at the proximal end 292B of the suction tube 292. The camera tube 12 is then aligned with the length of the suction tube 292 such that the distal end 14 of the camera tube 12 is in close proximity with the distal end 292A of the suction tube 292.

FIGS. 22B and 22C is a further embodiment of a suction tube with a visualization device, generally 290 as shown in FIG. 22A, but it is further equipped with a bougie 116 placed inside of a tube 118 which is placed inside of the suction tube 292 through an opening 295. A distal end 116A of the bougie 116 can protrude outside the distal end 292A of the suction tube 292 and can be manipulated by a medical practitioner with a proximal end 116B which protrudes outside a patient such as the placement of the suction tube 292 is guided under constant visualization with the camera 18 through the distal end 14 of the camera tube 12. The bougie 116 under constant visualization from the camera 12 permits rapid and accurate placement of the device 290 in a patient. The bougie 116 can be used to guide the placement of the device 290 and moving it left or right in the trachea.

Referring to FIG. 23, this embodiment provides a suction catheter with a visualization device, generally 300. The suction catheter 302 is not flexible and can be any suction catheter known in the art. A visualization device, generally 10, is positioned inside the suction catheter 302 through an opening 303 which is in near proximity with a proximal end 302B of the suction catheter 302. The visualization device 10 comprises a camera 18 with wire 20 which is placed inside of a camera tube 12 through an opening at a proximal end 16 of the camera tube 12 and then the camera 18 is slid to the distal end 14 which is sealed with a transparent material 17. The distal end 14 of the camera tube 12 is aligned with the distal end 302A of the suction catheter 302, while the proximal end 16 of the camera tube 12 protrudes outside the patient's body such as the camera 18 can be pulled out from the camera tube 12 as needed. In other embodiments, the suction tube is placed externally and this combination can work with suction caps.

Referring to FIG. 24, this embodiment provides an endotracheal changing tube with a visualization device, generally 310. An endotracheal changing tube can be any endotracheal changing tube as known in the art. A visualization device, generally 10, comprises a camera 18 with wire 20 which is placed inside of a camera tube 12 through an opening at a proximal end 16 of the camera tube 12 and slid all the way to a distal end 14 of the camera tube 12. The distal end 14 is sealed with a transparent material 17. The visualization device 10 is placed inside of the endotracheal changing tube 312 through an opening 313 in the changing tube 312 such as the camera tube 12 is aligned with the changing tube 312 along the proximal-distal (312B-312A) axis, and the distal end 14 of the camera tube 12 is in close proximity with the distal end 312A of the changing tube 312. In other embodiments, the camera tube 12 can be placed outside of the endotracheal changing tube or it can be fitted externally onto an endotracheal changing tube known in the art.

While certain medical devices are described above, a person of skill would appreciate that this invention also includes embodiments with various obvious modifications as would be easily apparent to a person of skill.

What is claimed is:

1. A medical device for intubating a patient, the medical device comprising a medical visualization device, the medical visualization device comprising:

a camera tube, the camera tube comprising a distal end and a proximal end, wherein the distal end is sealed with a transparent material and a proximal end has an opening; and

a camera with a wire placed inside of the camera tube, wherein the camera can be placed inside of the camera tube and it can be retracted from the camera tube on demand while the camera tube remains inserted in the patient, and wherein the camera can be reused in various devices without sterilization and wherein the camera can transmit images to a remote location wirelessly;

wherein the camera tube of the medical visualization device is sealed to, attached to or otherwise combined with at least one of the following second devices: an endotracheal tube, a supraglottic airway device, a ventilator adaptive cap, a dilator, a tracheostomy device, a nasal trumpet, an oral airway, an esophageal stethoscope, a stylet, a bougie, a speculum, a nasal cannula, a feeding tube, a suction tube, a suction catheter, and an endotracheal changing tube.

2. The medical visualization device of claim 1, wherein the camera tube comprises a fiber optic material.

3. The medical visualization device of claim 1, wherein the device can transmit information wirelessly and wherein the device is further equipped with at least one of the following: a light source, a stylet, a sound and temperature monitoring device, suction tube, bougie tube, stylet tube and a tool tube.

4. The medical visualization device of claim 1, wherein the camera is a digital camera.

5. The medical visualization device of claim 1, wherein the visualization device is in communication with at least one monitoring device wirelessly.

6. A method of continuous monitoring of a patient's at least one internal organ, the method comprising placing in the patient the visualization device of claim 1, transmitting images of the internal organ in real time with the camera through the transparent material at the distal end of the camera tube, and analyzing the transmitted images.

7. The method of claim 6, wherein the images, sound, data, information about temperature are transmitted wirelessly, broadcast or recorded to at least one device positioned at a remote location.

8. The method of claim 6, wherein the internal organ is selected from at least one of the following: nasopharynx, pharynx, hypo pharynx, supraglottic structures, subglottic airway, vocal cords, thorax, stomach and vagina.

9. The visualization device of claim 1, wherein the length of the camera tube can be adjusted to the length of at least one of the following second devices by sliding: an endotracheal tube, a supraglottic airway, airway device, oral airway, dilator, tracheostomy device, intubating oral airway, esophageal stethoscope, nasal cannula, feeding tube, stylet, bougie, suction tube and endotracheal changing tube and wherein the camera tube can slide along the distal/proximal axis of the device.

10. A method for placing a medical device in a patient, the method comprising equipping the medical device with the visualization device of claim 1 and a bougie and guiding the placement of the device with the bougie under continuous visualization with the visualization device of claim 1.

11. The medical device of claim 1 which further comprises at least one of the following a bougie and a sound- and temperature-monitoring device.

12. The medical device of claim 1 wherein the camera is retractable from the device and reusable in other devices.

13. The medical device of claim 1, wherein the camera tube of the visualization device is sealed, attached or otherwise connected externally to the second device.

14. The medical device of claim 1, wherein the visualization device is equipped with a light source.

15. The medical device of claim 1, wherein the second device is an endotracheal tube selected from the group consisting of: an endotracheal tube which comprises a sleeve through which the visualization device can be inserted, an endotracheal tube into which the visualization device is placed internally through a ventilator adaptive cap and an endotracheal tube to which the visualization device is attached.

16. The medical device of claim 1, wherein the second device is the supraglottic airway device or airway device.

17. The medical device of claim 1, wherein the visualization device is combined with the ventilator adaptive cap by being inserted through the cap.

18. The medical device of claim 1, wherein the second device is an endotracheal tube and wherein the visualization device is placed inside of the endotracheal tube through an opening on one side of the endotracheal tube, and wherein a plastic sleeve being attached over the opening such that the sleeve can slide up and down and facilitates keeping the visualization device sterile while it is moved in and out of the endotracheal tube.

19. The medical device of claim 1, wherein the second device is an endotracheal tube, and wherein the visualization device being positioned externally on the endotracheal tube along the proximal-distal axis of the endotracheal tube, and wherein a plastic sleeve being attached to the endotracheal tube such that the sleeve can slide up and down outside the endotracheal tube and facilitates the movement of the visualization device along the proximal-distal axis of the endotracheal tube.

20. The medical device of claim 19, wherein the endotracheal tube is equipped with a cuff wrapped around the endotracheal tube near its distal end; and wherein the visualization device can slide outside the endotracheal tube

along the proximal-distal axis such that the visualization device can be proximal or distal to the cuff.

21. The medical device of claim 1, wherein the visualization device is equipped with at least one ring, the visualization device is positioned externally on the second device along the proximal-distal axis of the second device, and the visualization device is connected to the second device with the at least one ring, and wherein the visualization device can slide along the proximal-distal axis of the second device.

22. The medical device of claim 1, wherein the second device is an oral airway which comprises a tubal body with a lumen, the tubal body is slightly curved in a hook-like shape and the visualization device is placed inside of the lumen and the visualization device can slide inside of the lumen along the proximal-distal axis of the oral airway.

* * * * *

专利名称(译)	医疗器械和放置方法		
公开(公告)号	US9918618	公开(公告)日	2018-03-20
申请号	US14/455470	申请日	2014-08-08
[标]申请(专利权)人(译)	伍恩迪吉股份有限公司		
申请(专利权)人(译)	WM & DG , INC.		
当前申请(专利权)人(译)	WM & DG , INC.		
[标]发明人	MOLNAR ROBERT W		
发明人	MOLNAR, ROBERT W.		
IPC分类号	A61B1/00 A61B1/24 A61B1/267 A61B1/303 A61M16/04 A61B1/233 A61B7/02 A61B1/07 A61M16/06 A61B1/05 A61B1/015 A61B1/018 A61B5/01 A61B5/00		
CPC分类号	A61B1/00154 A61B1/00016 A61B1/00135 A61B1/00137 A61B1/00142 A61B1/05 A61B1/07 A61B1/233 A61B1/24 A61B1/2673 A61B1/303 A61B7/023 A61M16/0463 A61M16/0465 A61M16/0488 A61M16/0666 A61B1/0014 A61B5/01 A61B1/00078 A61B1/015 A61B1/018 A61B5/0008		
其他公开文献	US20160038008A1		
外部链接	Espacenet USPTO		

摘要(译)

本发明提供了配备有用于插管，通气，药物输送，喂食和对患者的连续远程监测的可视化装置的改进的医疗装置。本发明还提供了用于将医疗装置快速且准确地放置在患者体内以及在放置之后连续实时监测患者的远程监测的方法。

