



US 20180184944A1

(19) **United States**

(12) **Patent Application Publication**
Bodewes et al.

(10) **Pub. No.: US 2018/0184944 A1**

(43) **Pub. Date: Jul. 5, 2018**

(54) **IMPLANTABLE KNEE SENSOR AND METHODS OF USE**

A61B 5/00 (2006.01)

A61B 5/1459 (2006.01)

(71) Applicant: **Biomet Manufacturing, LLC**, Warsaw, IN (US)

(52) **U.S. Cl.**

CPC *A61B 5/076* (2013.01); *A61B 5/01* (2013.01); *A61B 5/14539* (2013.01); *A61B 5/14551* (2013.01); *A61B 2560/0219* (2013.01); *A61B 5/0031* (2013.01); *A61B 5/6878* (2013.01); *A61B 5/1459* (2013.01); *A61B 5/14532* (2013.01)

(72) Inventors: **Hilbrandus H. Bodewes**, Delfgauw (NL); **Mohammed Imran Khan**, Berkshire (GB); **Daniel László-Deli**, Dordrecht (NL); **Max Hoeboer**, Dordrecht (NL); **Lisa Abdel Alim-van den Berg**, Dordrecht (NL); **Siemon Van Opstal**, Dordrecht (NL); **Bonita Koperdraat**, Dordrecht (NL); **Bart Krijgsman**, Dordrecht (NL); **Jurrit Heerink**, Dordrecht (NL)

(57) **ABSTRACT**

An implantable sensor configured to be inserted in an intramedullary canal can include a primary insert, a secondary insert, and an antenna. The primary insert can include a distal end, a proximal end opposite the distal end, and a central bore that can extend from an opening in the distal end towards the proximal end. A secondary insert can be receivable within the central bore through the opening. The secondary insert can include a body and a sensor module. The body can be removably engageable with an inside surface of the central bore. The sensor module can be disposable within the body and can be configured to produce a sensor signal as a function of a first sensed parameter indicative of infection. The antenna can be disposed in the central bore. The antenna can be configured to transmit a wireless signal as a function of the sensor signal.

(21) Appl. No.: **15/399,131**

(22) Filed: **Jan. 5, 2017**

Publication Classification


(51) **Int. Cl.**

A61B 5/07 (2006.01)

A61B 5/01 (2006.01)

A61B 5/145 (2006.01)

A61B 5/1455 (2006.01)

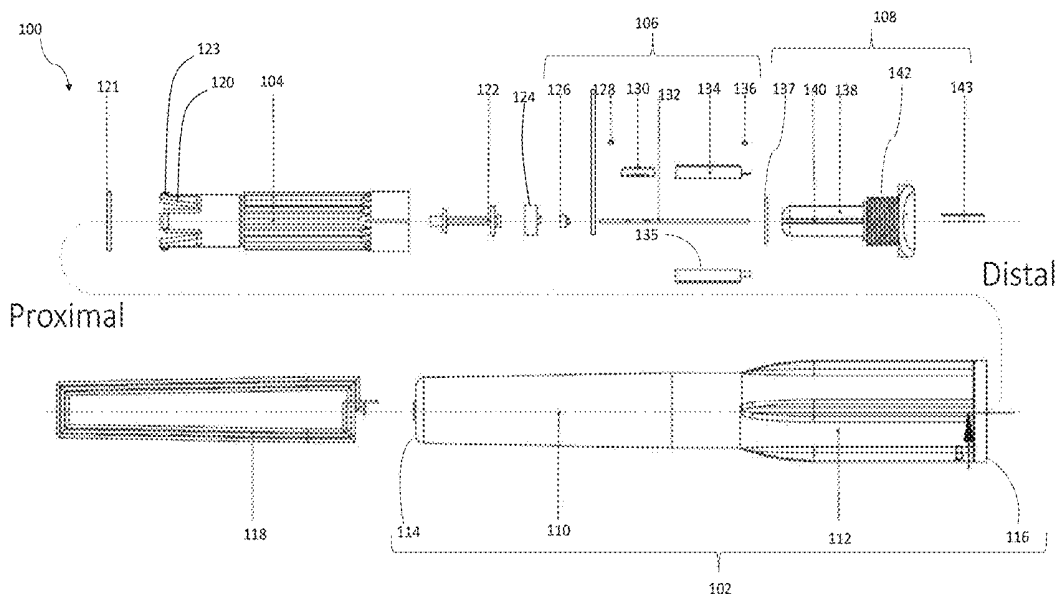

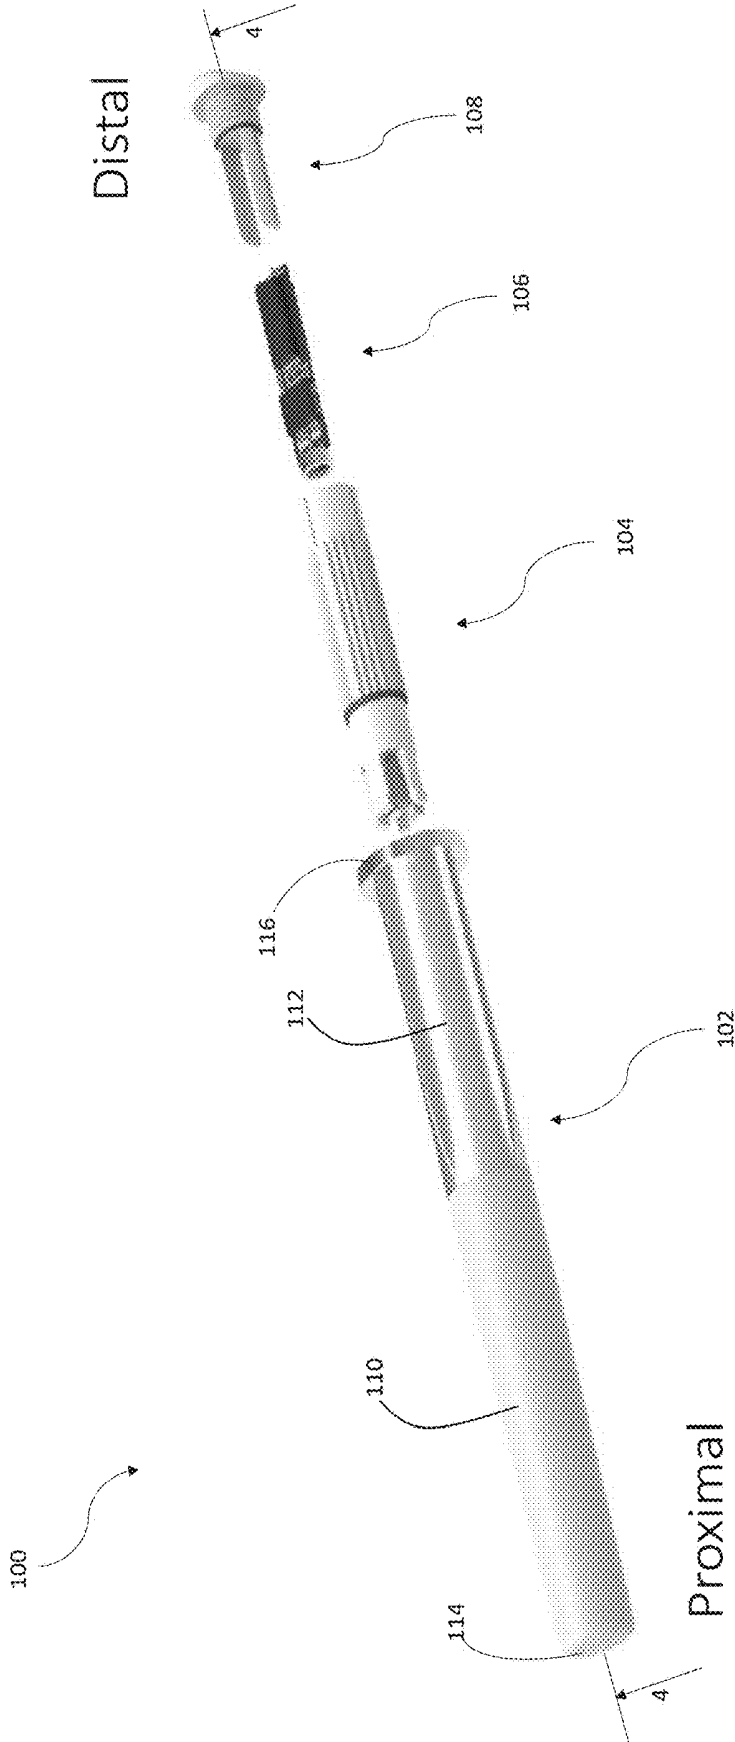
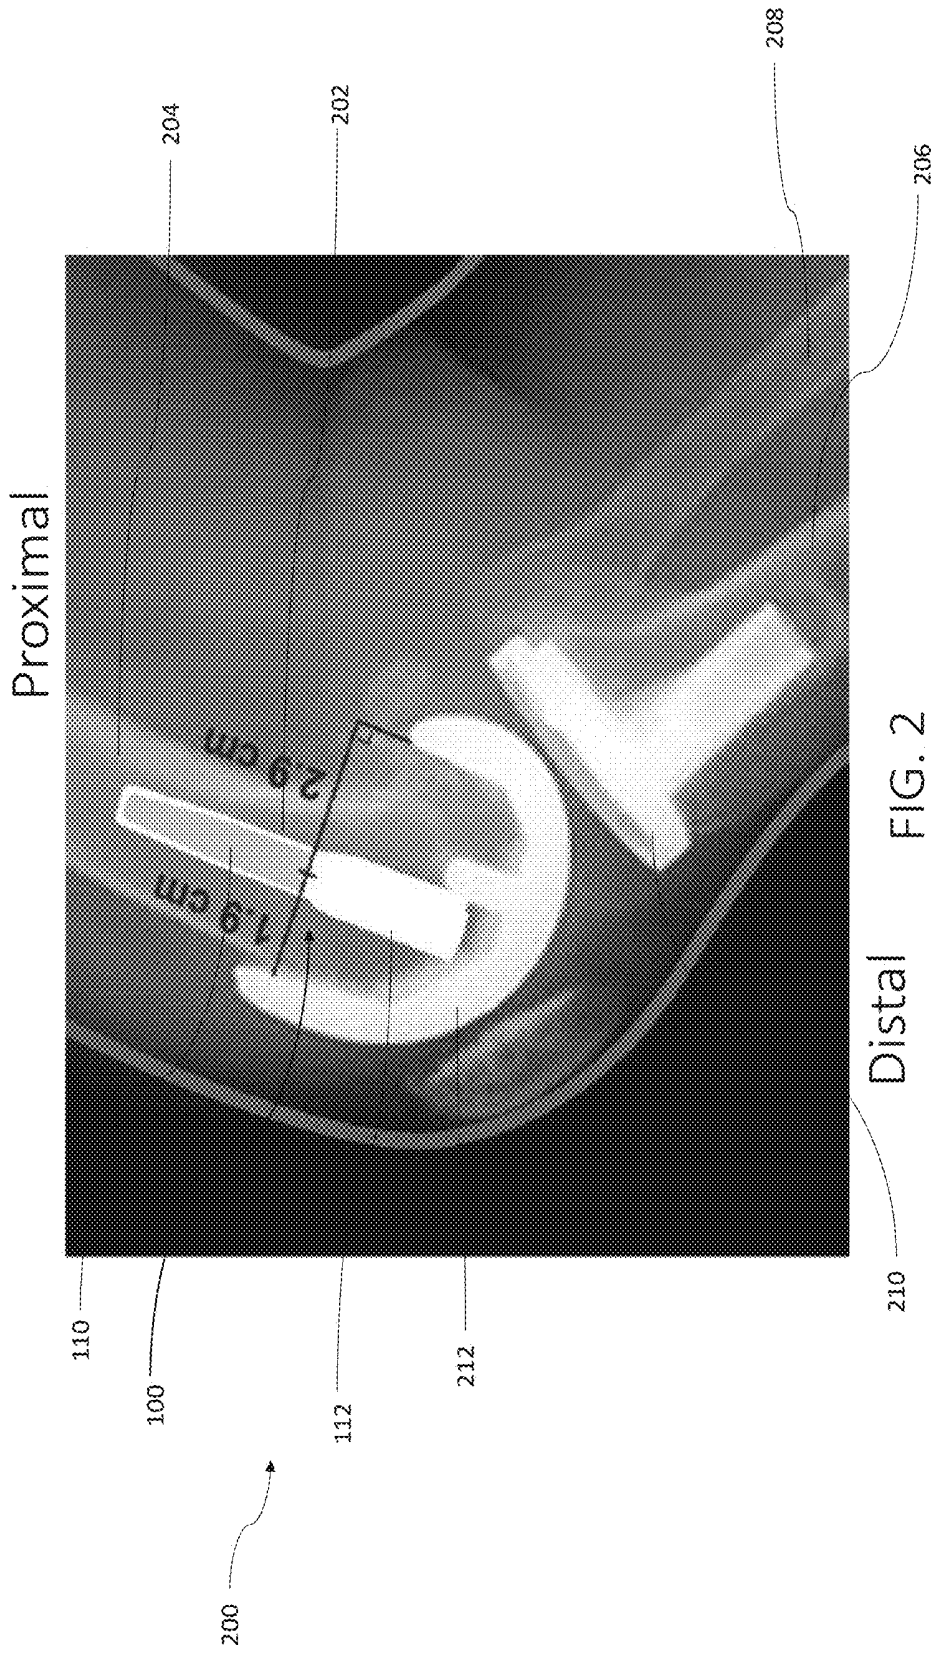


FIG. 1



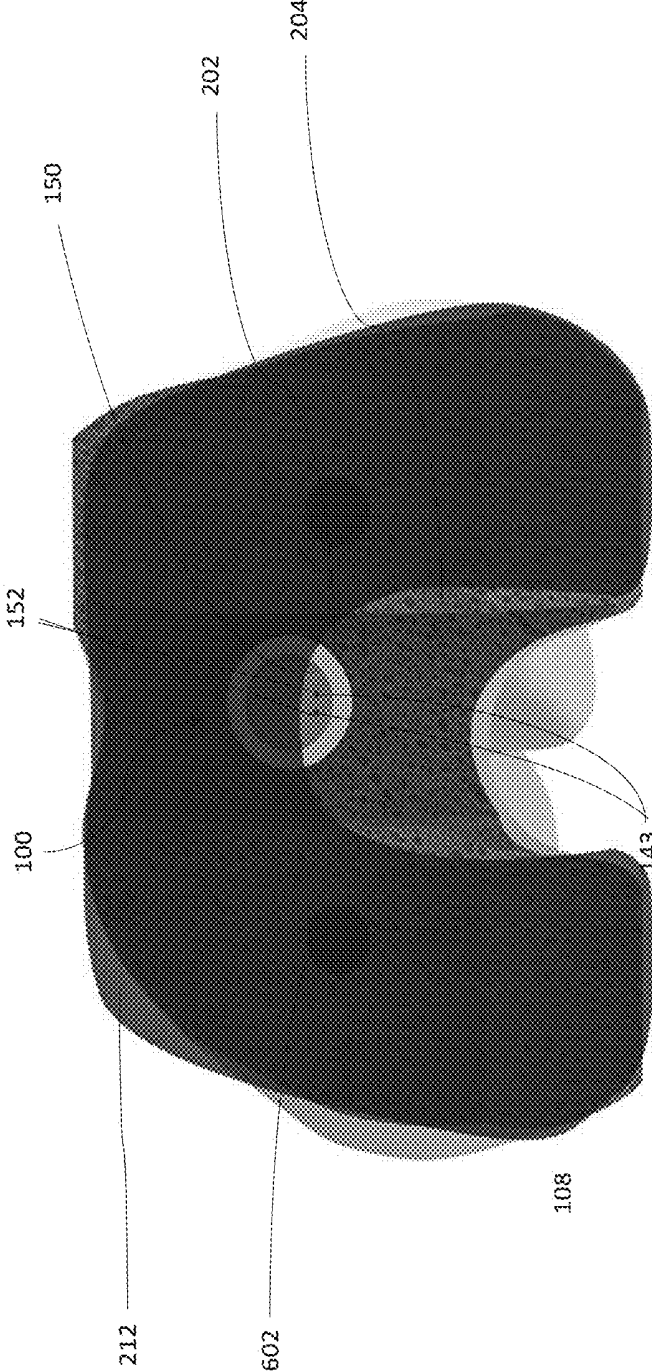


FIG. 6

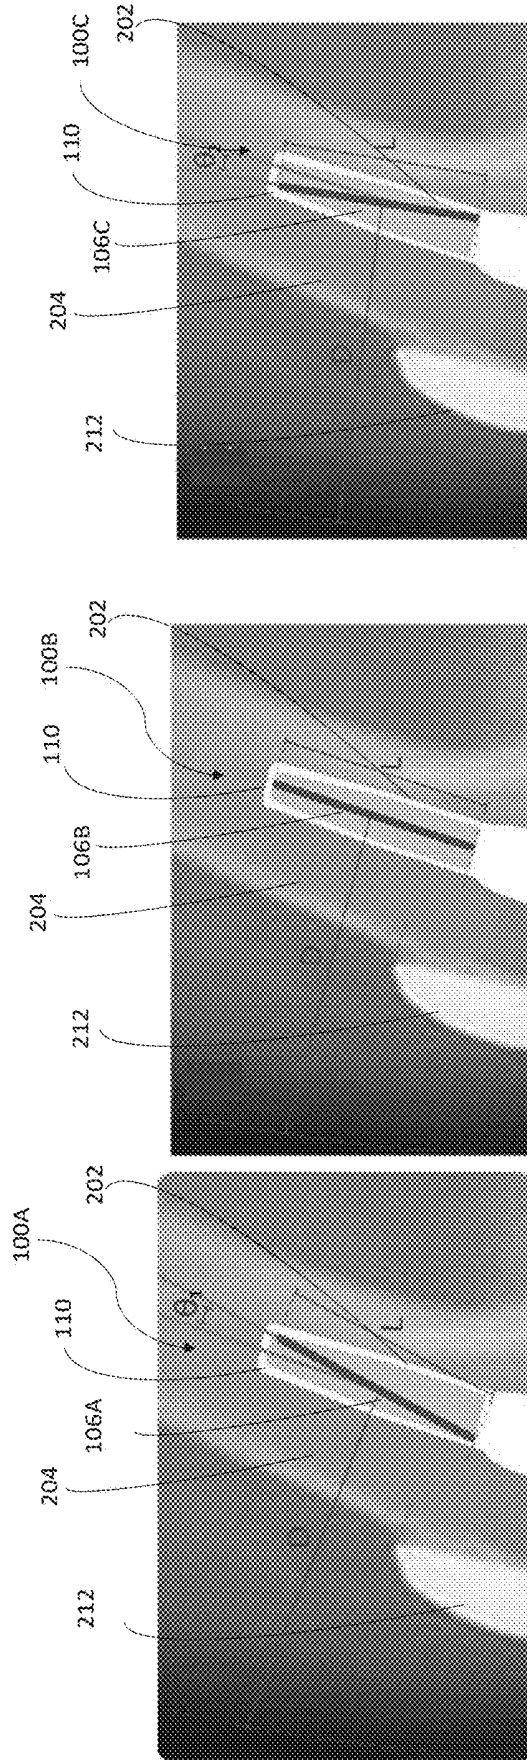


FIG. 7C

FIG. 7B

FIG. 7A

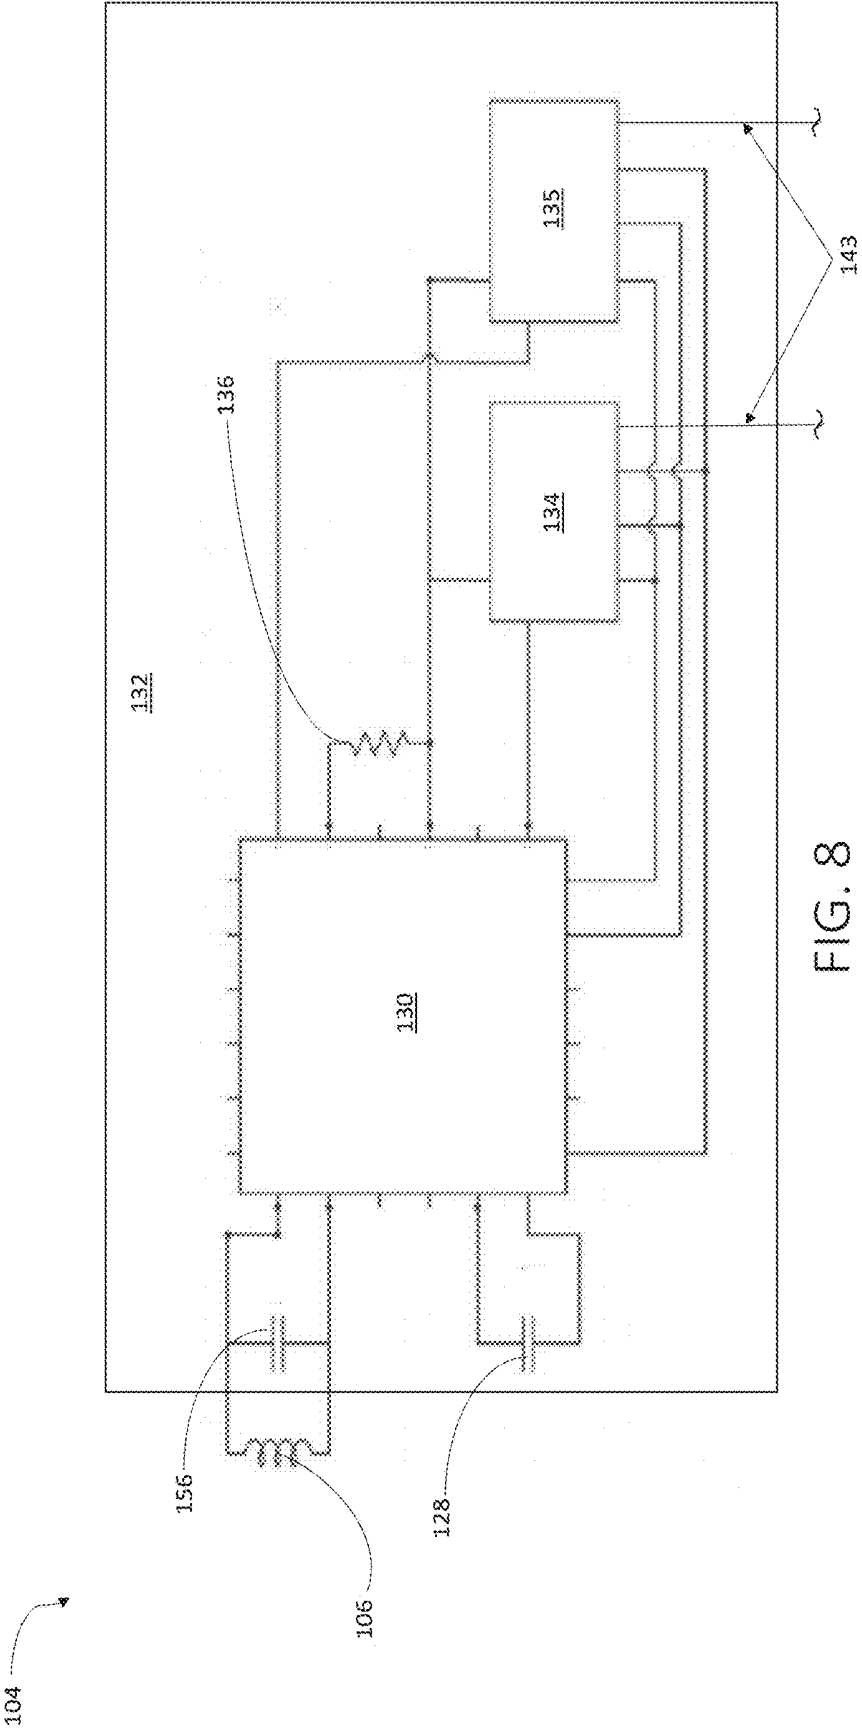


FIG. 8

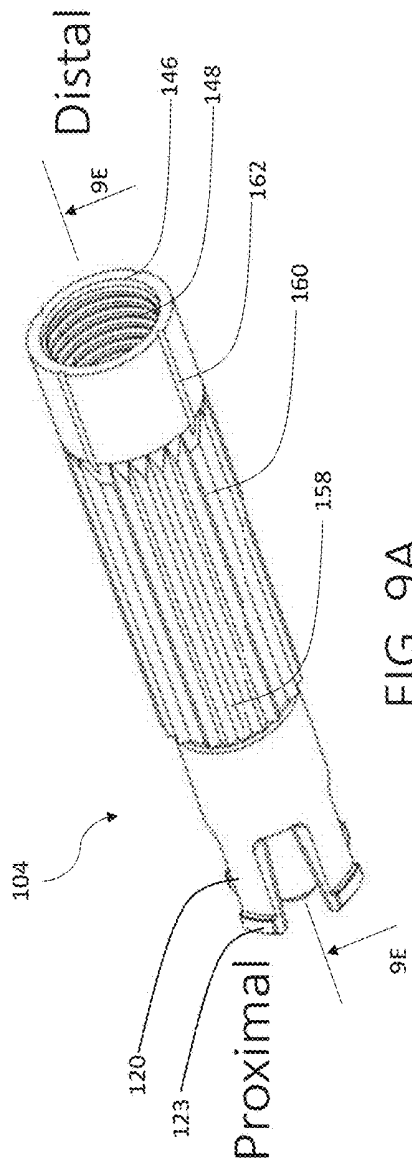


FIG. 9A

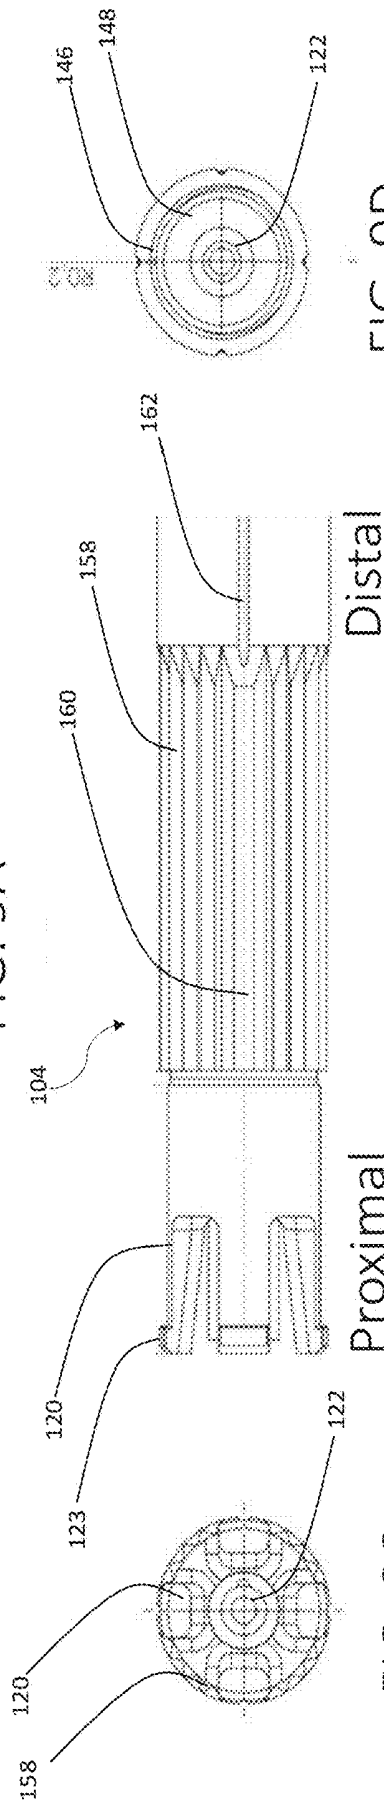


FIG. 9B

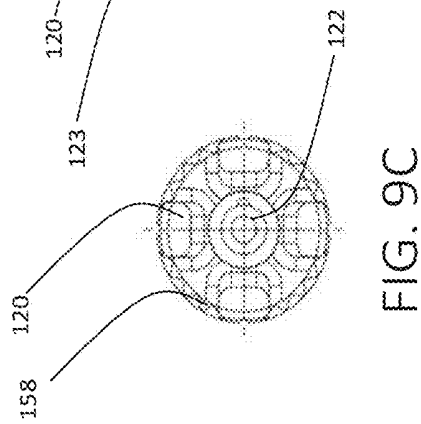


FIG. 9C

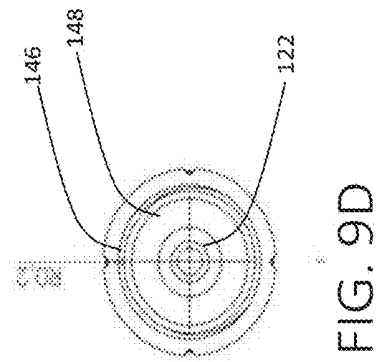


FIG. 9D

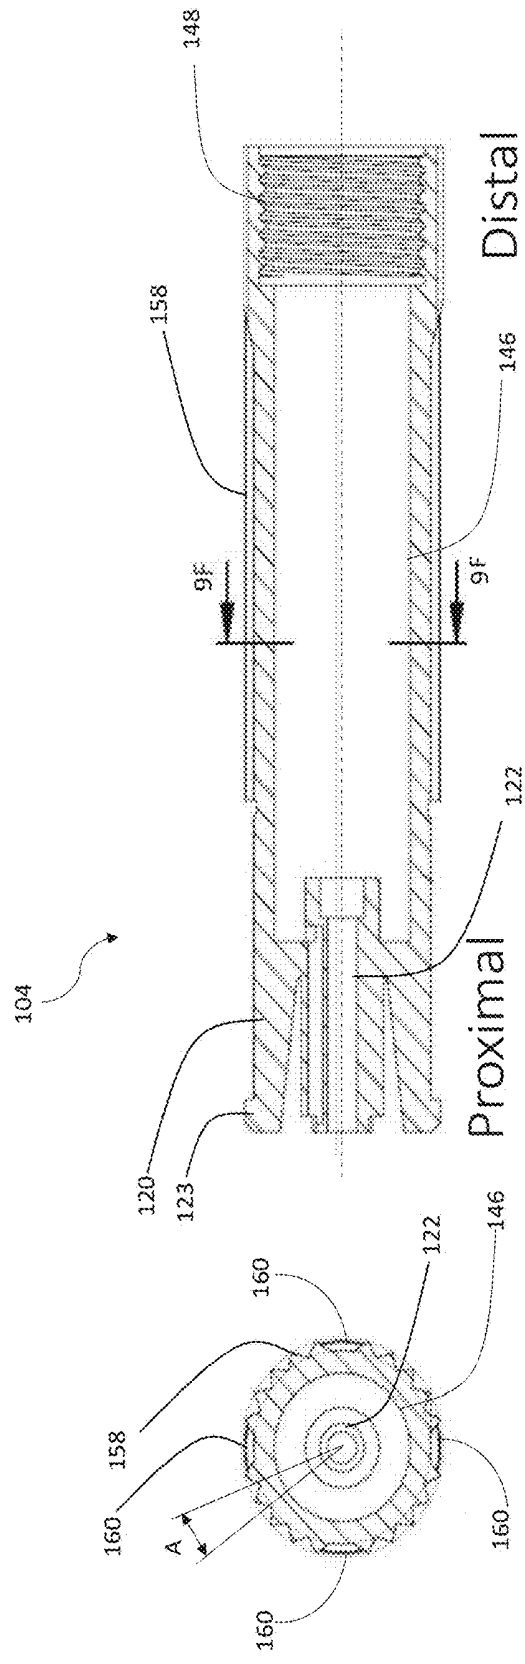


FIG. 9E

FIG. 9F

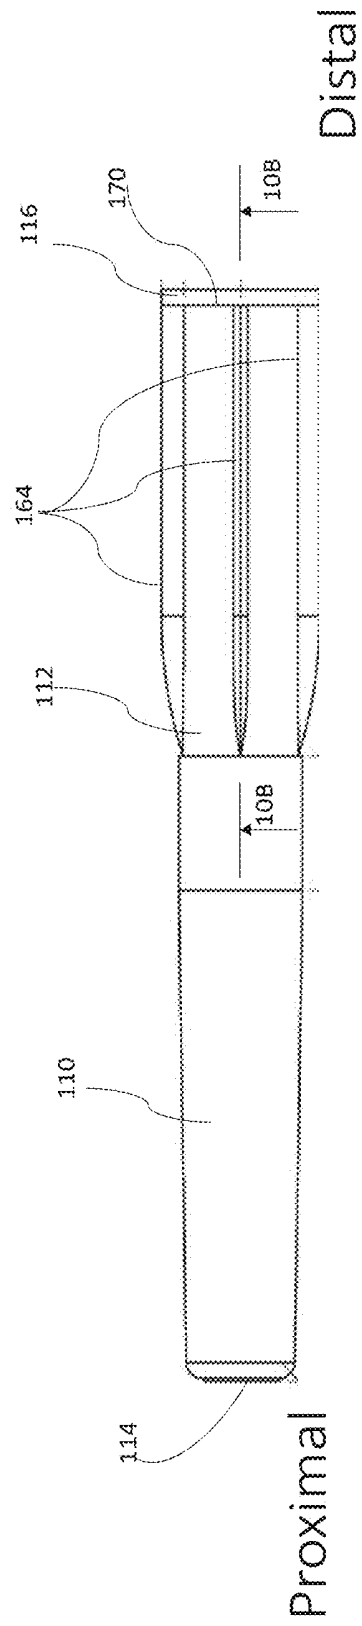


FIG. 10A

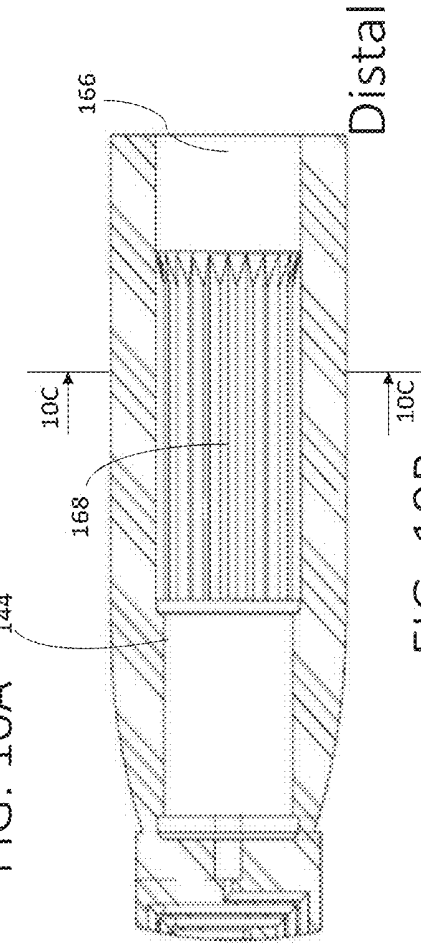


FIG. 10B

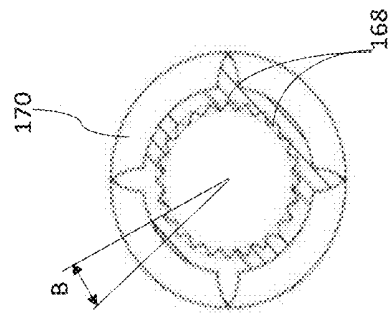


FIG. 10C

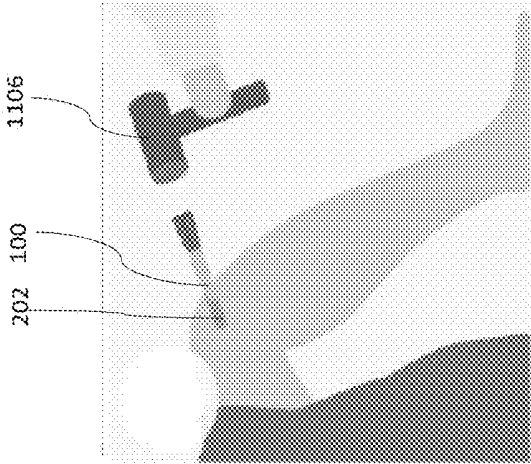


FIG. 11C

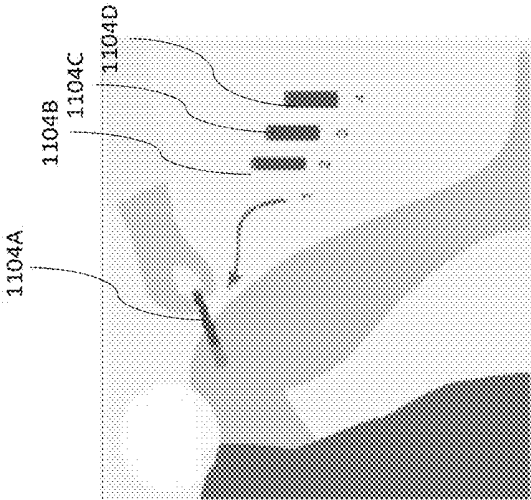


FIG. 11B

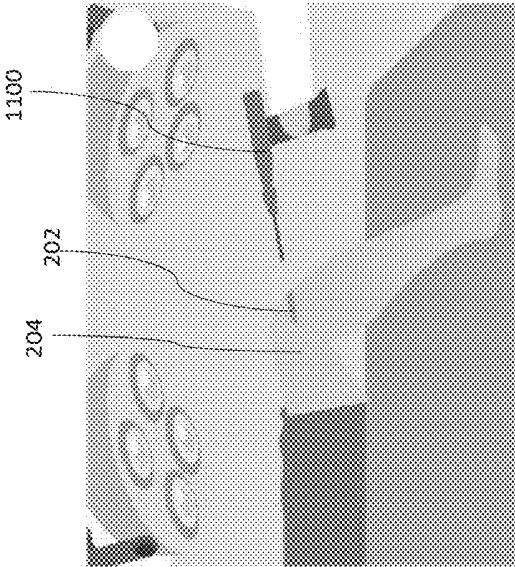


FIG. 11A

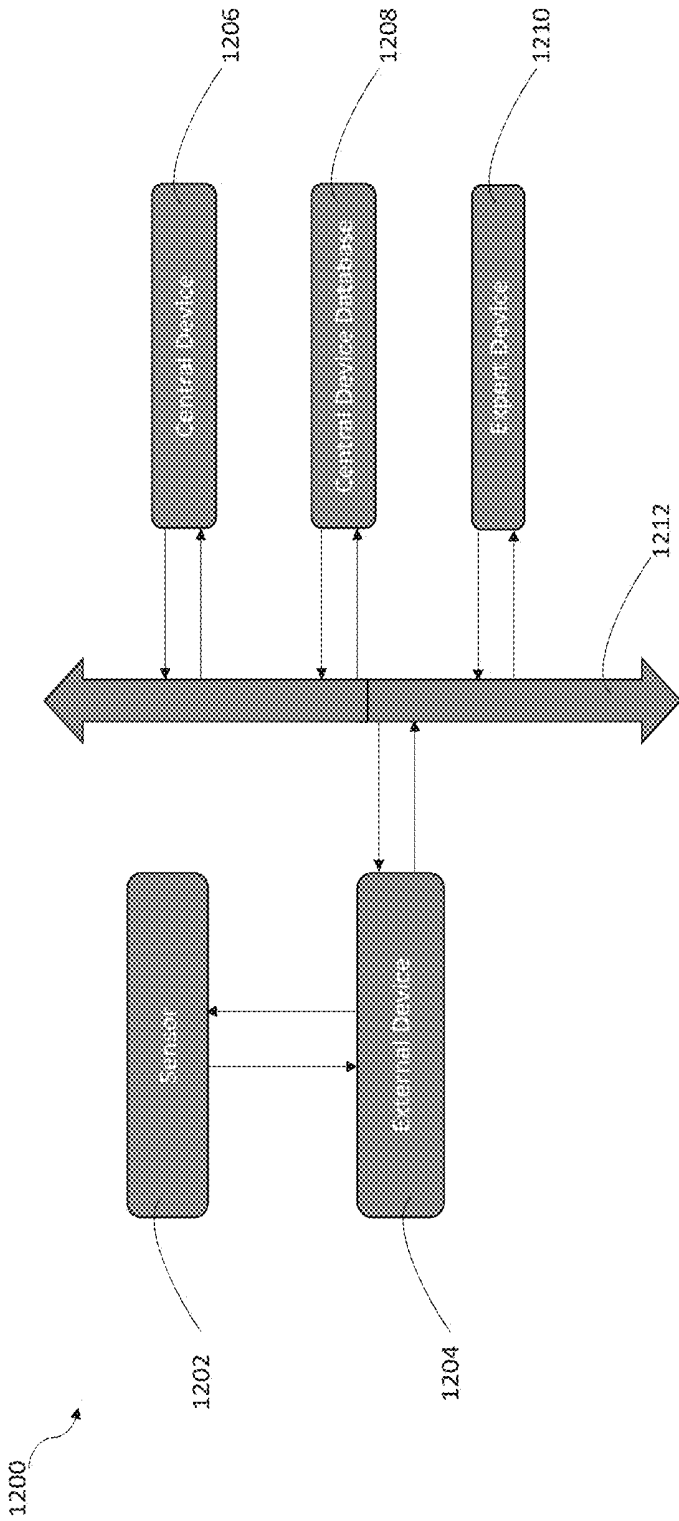


FIG. 12

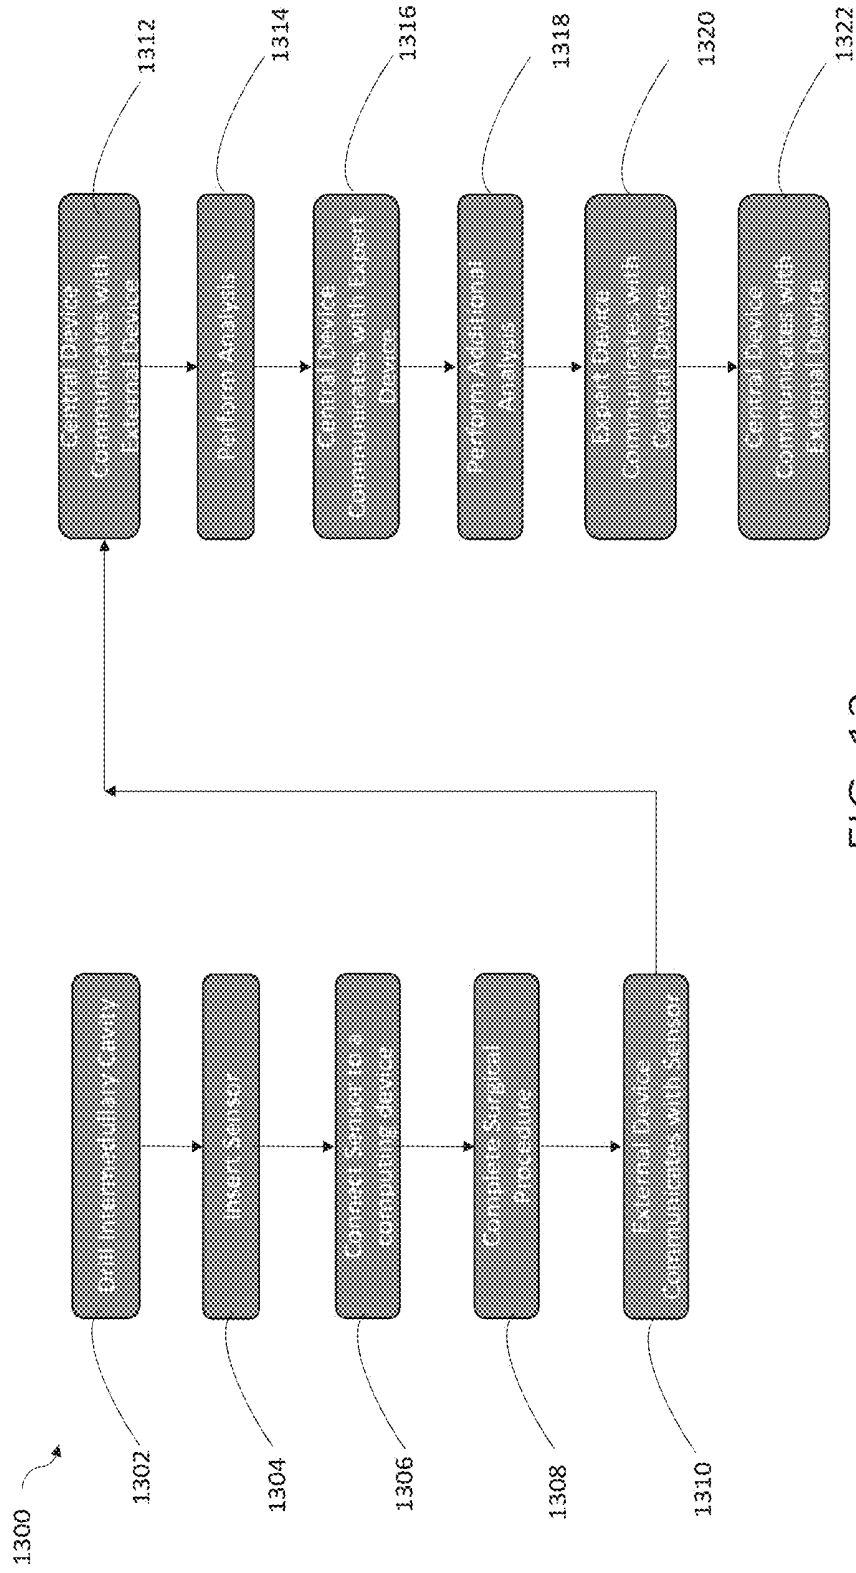


FIG. 13

IMPLANTABLE KNEE SENSOR AND METHODS OF USE

BACKGROUND

[0001] Orthopedic procedures and prostheses are commonly utilized to repair and/or replace damaged bone and tissue in the human body. For example, a knee arthroplasty can be used to restore natural knee function by repairing damaged or diseased articular surfaces of the femur and/or tibia. An incision is made into the knee joint to expose the bones comprising the joint. Cut guides are used to guide the removal of the articular surfaces that are to be replaced. Prostheses are used to replicate the articular surfaces. Knee prostheses can include a femoral component implanted on the distal end of the femur, which articulates with a tibial bearing component and a tibial component implanted on the proximal end of a tibia to replicate the function of a healthy natural knee. Various types of arthroplasties are known including a total knee arthroplasty, where all of the articulating compartments of the joint are repaired with prosthetic components. During orthopedic procedures, such as knee replacement or similar joint reconstruction surgeries, various prostheses can be used in the various procedures, including implant prostheses including sensors.

OVERVIEW

[0002] Assemblies, configurations, and methods of use for an implantable sensor module can be useful for early detection of infection. In an example, the implantable sensor provides a convenient, compact, and self-contained module that can be inserted into an already required cavity for various knee reconstruction surgeries. The implantable sensor module can be a passive sensor that is wirelessly activated and powered, such as through NFC, and wirelessly communicates with an external computing device to provide sensed information regarding the environment surrounding a prosthetic implant. The external computing device and other devices connected thereto can perform complex calculations, render graphical interfaces, and store data information related to data provided by the implantable sensor, providing significant means for detection of an infection.

[0003] The present inventors have recognized, among other things, the current surgical techniques, and surgeries in general, for joint reconstruction and other similar procedures can result in an infection around the installed prosthetic. These problems, and others, are addressed by the present invention through the ability to install a sensor module into the joint of a patient. An installed sensor that can communicate with an external device the existing conditions within a body of a patient in and around a prosthesis can offer a benefit of early detection of infection. Early detection of infection can reduce further required procedures, such as revisions, saving cost and providing improved quality of life. Additional benefits arising from the present subject matter will be obvious to one of ordinary skill in the art when reading the remainder of the detailed description.

[0004] The following, non-limiting examples, detail certain aspects of the present subject matter to solve the challenges and provide the benefits discussed herein, among others.

[0005] Example 1 is an implantable sensor configured to be inserted in an intramedullary canal, the implantable sensor comprising: a primary insert including a distal end, a

proximal end opposite the distal end, and a central bore extending from an opening in the distal end towards the proximal end; a secondary insert receivable within the central bore through the opening, the secondary insert comprising: a body removably engageable with an inside surface of the central bore; and a sensor module disposable within the body and configured to produce a sensor signal as a function of a first sensed parameter indicative of infection; and an antenna disposed in the central bore, the antenna configured to: transmit a wireless signal as a function of the sensor signal.

[0006] In Example 2, the subject matter of Example 1 optionally includes wherein the sensor comprises one of a temperature sensor, a pH sensor, an oxygen sensor, a carbon dioxide sensor, and a glucose sensor.

[0007] In Example 3, the subject matter of any one or more of Examples 1-2 optionally include wherein the antenna is configured to receive power from an external source and distribute the power to the sensor.

[0008] In Example 4, the subject matter of any one or more of Examples 1-3 optionally include wherein the secondary insert further comprises: a cap releasably securable to the secondary insert.

[0009] In Example 5, the subject matter of Example 4 optionally includes wherein the cap and sensor module are releasable from the secondary insert while the secondary insert is inserted in the intramedullary canal.

[0010] In Example 6, the subject matter of any one or more of Examples 4-5 optionally include wherein the cap further comprises: a plurality of legs projecting proximally from a proximal surface of the cap and configured to retain the sensor capsule.

[0011] In Example 7, the subject matter of any one or more of Examples 1-6 optionally include wherein the secondary insert further comprises: a second sensor configured to produce a second sensor signal as a function of a second sensed parameter indicative of infection.

[0012] In Example 8, the subject matter of Example 7 optionally includes wherein the secondary insert further comprises: a third sensor configured to produce a third sensor signal as a function of a third sensed parameter indicative of infection.

[0013] In Example 9, the subject matter of any one or more of Examples 1-8 optionally include wherein the secondary insert further comprises: an optical fiber connected to the sensor and extending through a periphery of the secondary insert to expose the optical fiber to a joint cavity adjacent to the intramedullary canal to send an optical signal to the sensor as a function of sensed optical conditions of the joint cavity.

[0014] In Example 10, the subject matter of Example 9 optionally includes a cap releasably securable to the secondary insert, the cap comprising: a passage exposing the sensor module to the joint cavity, the passage receivable of the optical fiber.

[0015] In Example 11, the subject matter of any one or more of Examples 1-10 optionally include wherein the central bore further comprises a plurality of grooves extending axially along a surface of the central bore, and wherein the secondary insert further comprises a plurality of ribs projecting radially outward from an outer surface of the secondary insert and extending axially along the outer

surface, the plurality of ribs mateable with the plurality of grooves to prevent rotation of the secondary insert relative to the primary insert.

[0016] Example 12 is a system for monitoring a joint cavity, the system comprising: an implantable sensor comprising: a femoral insert implantable in a femoral intramedullary canal adjacent to the joint cavity, the femoral insert comprising: a proximal end and a distal end; and a central bore extending from the distal end through the distal portion and terminating prior to the proximal end; a sensor insertable into the central bore through the distal end, the sensor configured to produce a sensor signal as a function of a sensed condition of the joint cavity; and an antenna disposed in the central bore, the antenna configured to: transmit a wireless signal as a function of the sensor signal; and receive power and distribute the power to the sensor.

[0017] In Example 13, the subject matter of Example 12 optionally includes a central device in communication with the external computing device, the central device configured to analyze data received from the external computing device and return analysis to the external computing device.

[0018] In Example 14, the subject matter of Example 13 optionally includes an expert device in communication with at least one of the external computing device and the central device, the expert device configured to: analyze data received from at least one of the external computing device the central device; and analyze analysis received from the central device.

[0019] In Example 15, the subject matter of any one or more of Examples 12-14 optionally include wherein the secondary insert further comprises: a communication chip connected to the antenna and the sensor, the communication chip configured to process the sensor signal and distribute power from the antenna to the sensor.

[0020] In Example 16, the subject matter of Example 15 optionally includes wherein the communication chip comprises a near field communication chip.

[0021] Example 17 is an intramedullary implant configured to be inserted in a femoral intramedullary canal, the intramedullary implant comprising: a housing insertable into a femoral intramedullary canal, the housing comprising: a proximal portion including a proximal end; a distal portion including a distal end; and a bore extending from the distal end towards the proximal end; a secondary insert receivable in the bore, the secondary insert engageable with an internal surface of the bore, and including a sensor configured to produce a sensor signal as function of a first sensed parameter of a joint cavity adjacent the intramedullary canal, the first sensed parameter indicative of infection; and an antenna coil disposed in the proximal portion, the antenna configured to transmit a wireless signal as a function of the sensor signal.

[0022] In Example 18, the subject matter of Example 17 optionally includes wherein the secondary insert comprises a snap fit connection securable to the central bore.

[0023] In Example 19, the subject matter of Example 18 optionally includes wherein the snap fit connection comprises a plurality of straight arms, each arm of the plurality of arms including a projection extending radially from a proximal termination of each arm.

[0024] In Example 20, the subject matter of any one or more of Examples 17-19 optionally include wherein the antenna coil is positionable within the proximal portion to change a coil angle relative to the sensor module.

[0025] In Example 21, the subject matter of any one or more of Examples 1-11 optionally include wherein primary insert is comprised of PEEK.

[0026] This overview is intended to provide an overview of subject matter of the present patent application. It is not intended to provide an exclusive or exhaustive explanation of the invention. The detailed description is included to provide further information about the present patent application.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] In the drawings, which are not necessarily drawn to scale, like numerals may describe similar components in different views. Like numerals having different letter suffixes may represent different instances of similar components. The drawings illustrate generally, by way of example, but not by way of limitation, various embodiments discussed in the present document.

[0028] FIG. 1 illustrates a three dimensional exploded view of an implantable sensor, in accordance with at least one example of this disclosure.

[0029] FIG. 2 illustrates an adapted, illustrative X-ray image of an implantable sensor installed in a femoral intramedullary canal, in accordance with at least one example of this disclosure.

[0030] FIG. 3 illustrates an exploded view of an implantable sensor, in accordance with at least one example of this disclosure.

[0031] FIG. 4 illustrates cross-sectional view of an implantable sensor across indicators 4-4 of FIG. 1, in accordance with at least one example of this disclosure.

[0032] FIG. 5A illustrates a side view of a cap for an implantable sensor, in accordance with at least one example of this disclosure.

[0033] FIG. 5B illustrates an isometric view of a cap for an implantable sensor from a distal perspective, in accordance with at least one example of this disclosure.

[0034] FIG. 6 illustrates an implantable sensor installed in a femoral intramedullary canal, in accordance with at least one example of this disclosure.

[0035] FIGS. 7A-7C illustrate an electromagnetic image of an implantable sensor installed in a femoral intramedullary canal with an antenna at multiple angles, in accordance with at least one example of this disclosure.

[0036] FIG. 8 illustrates a schematic of electrical components of an implantable sensor, in accordance with at least one example of this disclosure.

[0037] FIG. 9A illustrates an isometric view of a secondary insert of an implantable sensor, in accordance with at least one example of this disclosure.

[0038] FIG. 9B illustrates a plan view of a secondary insert of an implantable sensor, in accordance with at least one example of this disclosure.

[0039] FIG. 9C illustrates an end view of a secondary insert of an implantable sensor from a proximal perspective, in accordance with at least one example of this disclosure.

[0040] FIG. 9D illustrates an end view of a secondary insert of an implantable sensor from a distal perspective, in accordance with at least one example of this disclosure.

[0041] FIG. 9E illustrates a cross-section view of an implantable sensor across indicators 9E-9E of FIG. 9A, in accordance with at least one example of this disclosure.

[0042] FIG. 9F illustrates a cross-section view of an implantable sensor across indicators 9F-9F of FIG. 9E, in accordance with at least one example of this disclosure.

[0043] FIG. 10A illustrates a plan view of an implantable sensor, in accordance with at least one example of this disclosure.

[0044] FIG. 10B illustrates a cross-section view of an implantable sensor across indicators 10B-10B of FIG. 10A, in accordance with at least one example of this disclosure.

[0045] FIG. 10C illustrates a cross-section view of an implantable sensor across indicators 10C-10C of FIG. 10B, in accordance with at least one example of this disclosure.

[0046] FIG. 11A illustrates a step of a surgical procedure, in accordance with at least one example of this disclosure.

[0047] FIG. 11B illustrates a step of a surgical procedure, in accordance with at least one example of this disclosure.

[0048] FIG. 11C illustrates a step of a surgical procedure, in accordance with at least one example of this disclosure.

[0049] FIG. 12 illustrates a schematic components of a sensor system, in accordance with at least one example of this disclosure.

[0050] FIG. 13 illustrates a method of using a sensor system, in accordance with at least one example of this disclosure.

DETAILED DESCRIPTION

[0051] Detailed structure, configurations, and methods of use for an implantable knee sensor are generally disclosed herein. In one example, an implantable sensor includes a primary insert, secondary insert, an antenna, and a sensor. For example, during total knee arthroplasty (TKA), a surgeon can install an implantable sensor in an intramedullary femoral cavity including a sensor that can be configured to detect conditions indicative of infection. The antenna can then broadcast a signal containing data produced as a function of the sensed conditions.

[0052] FIG. 1 illustrates a three dimensional exploded view of implantable sensor 100, in accordance with at least one example of this disclosure. Implantable sensor 100 can include primary insert 102 and secondary insert 104. Secondary insert 104 can include sensor module 106, and cap 108. Primary insert can include proximal portion 110, distal portion 112, proximal end 114, and distal end 116.

[0053] Primary insert 102, or femoral fixation unit (FFU), can be an elongate member, such as a tubular member, having a generally tapered cylindrical shape, including a flange at distal end 116. Distal portion 112 can be press fit into proximal portion 110, such that distal portion 112 has a pin or insertion portion that is similar in size to, or slightly larger than, a bore within the proximal portion 110. For example, the pin portion and the bore can be about 5 millimeters to 15 millimeters in some examples, and about 8 millimeters to 10 millimeters in some examples, with an interference of -0.5 to 0.5 millimeters in some examples.

[0054] Primary insert 102 can be comprised of a suitable metal, polymer, and the like, for insertion into a bone of a human body, such as steel, cobalt, titanium, polyether ether ketone (PEEK). In one example, primary insert 102 can be comprised of PEEK and coated with titanium and/or a hydroxyapatite coating. Secondary insert 104 and cap 108 can be comprised of similar materials. This can provide the benefit of reducing signal attenuation of signal while accepting coatings enabling fixation.

[0055] Secondary insert 104 can be a generally tubular body having a snap connection at a proximal end and an opening at a distal end. Secondary insert 104 can be inserted and secured within distal portion 112 of primary insert 110.

[0056] Sensor module 106 can include one or more sensors, a communication chip, and a processor, as discussed further below. Sensor module 106 can be coupled to cap 108 and inserted into secondary insert 104. Sensor module 106 can be electrically connected to an antenna enclosed within proximal portion 110 of primary insert 102. Cap 108 can include a threaded portion configured to releasably secure to a threaded portion of distal portion 112, securing sensor module 106 within secondary insert, and axially securing secondary insert 104 within distal portion 112. Cap 108 can be removed during, for example, follow-up procedures such as to revise or replace components of implantable sensor 100. However, cap 108 can be securable to distal portion 112 such that cap 108 will not become separated from sensor module 106 under normal conditions of use while implanted. In some other examples, cap 108 can engage sensor module 106 so that cap 108 is not removable from sensor module 106, which can protect sensor module 106, helping to prevent exposure of electronic components to bodily fluids.

[0057] FIG. 2 illustrates an adapted, illustrative X-ray image of implantable sensor 100 installed in femoral intramedullary canal 202 of femur 204, in accordance with at least one example of this disclosure. FIG. 2 also shows proximal portion 110 and distal portion 112 of implantable sensor 100. Also shown in FIG. 1 are tibia 206, fibula 208, tibial implant 210, and femoral implant 212.

[0058] The components of FIG. 2 can be consistent with those of a total knee arthroplasty or knee revision procedure, where orthopedic procedures and prostheses can be utilized to repair and/or replace damaged bone and tissue in a human body. In some examples, such as the example of FIG. 2, prostheses can be used to replicate articular knee surfaces. Knee prostheses can include tibial implant 210 inserted into through a resected proximal surface of tibia 206 and into fibula 206. Femoral implant 212 can be implanted on and secured to a distal end of femur 204. Femoral implant 212 can articulate with a tibial bearing component on the proximal end of tibial implant 210 implanted to replicate the function of a healthy natural knee.

[0059] During some types of arthroplasties, a bore can be drilled into the distal end of femur 204. The bore can be sized to receive surgical tools, such as cutting guides. The bore can also be used to secure femoral implant 212 to femur 203 using a fastener, such as a screw. This process can create or expand intramedullary canal 202. After installation of femoral implant 212 onto femur 204 in the prior art, intramedullary canal 202 can be filled, can receive a fastener, or can be left empty for use in future procedures. The present disclosure offers the benefit of making use of a cavity already required by some arthroplasty procedures, by providing implantable sensor 100, which can be configured for installation within intramedullary canal 202.

[0060] Implantable sensor 100 can be sized to secure to intramedullary canal 202 in a press fit configuration. For example, implantable sensor 100 can have an outside diameter that is similar to or slightly larger than an inside diameter of intramedullary canal 202. Additionally, implantable sensor 100 can have a length (in an axial direction of implantable sensor 100) such that implantable sensor 100

does not interfere with femoral implant 212, and such that cap 108 (of FIG. 1) is exposed (as discussed below). Implantable sensor 100 can be additionally secured to femur 204 using an adhesive, such as polymethylmethacrylate (PMMA).

[0061] In some examples, implantable sensor 100 can be secured within intramedullary canal 202 disposed through femoral implant 212, but not connected or secured thereto. This can enable removal of implantable sensor 100 without removing femoral implant 212. In some examples, implantable sensor 100 can be mechanically interconnected (upon implantation) with the femoral implant. In some examples, implantable sensor 100 can be secured to femoral implant 212 using a peg, pin, screw, and the like, to help prevent axial motion of implantable sensor relative to intramedullary canal 202.

[0062] FIG. 3 illustrates an exploded view of implantable sensor 100, in accordance with at least one example of this disclosure. FIG. 4 illustrates a cross-sectional view of implantable sensor 100 across indicators 4-4 of FIG. 1, in accordance with at least one example of this disclosure. FIGS. 3 and 4 are discussed concurrently.

[0063] Implantable sensor 100 can include primary insert 102 and secondary insert 104. Secondary insert 104 can include sensor module 106, cap 108, and antenna coil 118. Primary insert can include proximal portion 110, distal portion 112, proximal end 114, and distal end 116. Secondary insert can include snap fits 120, outer ring 121, coil connector 122, projections 123, and outer connector 124. Sensor module 106 can include inner connector 126, capacitor 128, communication chip 130, printed circuit board (PCB) 132, first sensor 134, second sensor 135, and third sensor 136. Cap 108 can include inner ring 137, arms 138, PCB slots 140, threaded portion 142, and optical fibers 143 (FIG. 3). Primary insert 102 can also include central bore 144 (FIG. 4). Secondary insert 104 can also include secondary insert bore 146 (FIG. 4) and internal threaded portion 148 (FIG. 4).

[0064] Antenna coil 118 can be a coil type antenna in some examples, configured to be disposed in proximal portion 110 and connected to coil connector 122. Coil connector can connect to outer connector 124, thus electrically connecting sensor module 106 to antenna coil 118. Coil connector 122, outer connector 124, and inner connector 126 can be comprised of biocompatible materials that are conductive, such as titanium, steel, silver, and the like. Because secondary insert 104 can be placed in primary insert at several positions (as described below), and antenna coil 118 can be placed within proximal portion 110 at varying angles (also described below), coil connector 122 can be configured to connect antenna coil 118 to sensor module 106 at a variety of angles.

[0065] Central bore 144 can be a bore beginning at distal end 116 and extending through distal portion 112 and proximal portion 110, terminating in proximal portion 110 prior to proximal end 114. In some examples, central bore 144 can have a diameter in proximal portion 110 that is larger than a second diameter in distal portion 112.

[0066] Secondary insert 104 can be disposed within central bore 144 within distal portion 112 of primary insert 102, such that secondary insert extends from distal end 116 through distal portion 112, terminating at proximal portion 110. Outer ring 121 can be disposed around an outer surface of secondary insert 104 to form a seal in central bore 144.

In some examples, outer ring 121 of secondary insert 104 can be a seal such as an o-ring or other type of annular seal.

[0067] Snap fits 120 of secondary insert 104, can be disposed at the proximal termination of secondary insert 104. Snap fits 120 can each include projections 123, which can extend radially from a proximal termination of snap fits 120. Projections 123 can be sized to have a larger diameter than that of central bore 144, so that when secondary insert 104 is inserted into central bore 144, central bore 144 can force projections 123 radially inward, allowing secondary insert 104 to be moved through central bore 144 axially towards proximal end 114. As secondary insert 104 moves further into central bore 144, projections 123 can expand when projections 123 reach a section of central bore 144 having a larger diameter, such as an undercut or counter bore. After expanding, projections 123 can engage the undercut or other surface of central bore 144 after projections 123 and snap fits 120 expand to their original diameter.

[0068] In some examples, the engagement of snap fits 120 with a portion of central bore 144 can prevent secondary insert from moving axially towards distal end 116. In some examples, projections 123 can be sized to be as small as possible, to minimize a wall thickness of primary insert 102. In some examples, snap fits 120 can include a quantity of snap fits 120 designed to reduce stress in snap fits 120 during installation (compression and expansion of snap fits 120) of secondary insert 104 in central bore 144. In some examples, a quantity of snap fits 120 can be 1, 2, 3, 4, 5, or 6, and the like. In some examples, snap fits 120 can include a geometry designed to reduce stress in snap fits 120 during installation, such as a tapered rectangular extension including a radially extending projection, for example.

[0069] Sensor module 106 includes PCB 132, which can be a printed circuit board configured to support and electrically connect the components of sensor module 106. As discussed above, internal connector 126 connects to external connector 124, which connects to coil connector 122. Internal connector 126 is also electrically connected to PCB 132 at a proximal end of PCB 132.

[0070] Capacitor 128, communication chip 130, first sensor 134, second sensor 135, and third sensor 136 can also be electrically connected to PCB 132 and supported by PCB 132. First sensor 134, second sensor 135, and third sensor 136 can be connected to optical fibers 143 to place first sensor 134 and/or second sensor 135 and/or third sensor 136 in communication with an environment outside of sensor implant 100, such as synovial fluid that can be found in a distal portion of femur 204. First sensor 134, second sensor 135, and third sensor 136 can be electrochemical, amperometric, potentiometric, conduct metric, thermometric, optical, luminescent, such as sensor configured to produce a signal as a function of glucose, temperature, oxygen (O₂), carbon dioxide (CO₂), or Ph. In one example, an optical sensor can be configured to convert an optical signal into a sensor signal that is a function of a measured optical condition, as discussed further below.

[0071] Cap 108 can be releasably securable to secondary insert 104, and in some examples can be releasably securable to secondary insert bore 146. In some examples, cap 108 can include threaded portion 142 having a diameter smaller than a distal portion of cap 108. Threaded portion 142 can extend towards proximal end 114. Secondary insert bore 146 can include internal threaded portion 148 configured to receive threaded portion 142 of cap 108. In some

examples, inner ring 137 can be a seal such as an o-ring or other annular seal. In some examples, inner ring 137 can be configured to surround arms 138 and abut threaded portion 142 of cap 108 and internal threaded portion 148, creating a seal between cap 108 and secondary insert bore 146.

[0072] Arms 138 can extend axially in a generally proximal direction from a proximal surface of cap 108. Each of arms 138 can include PCB slots 140, which can be sized to receive and retain PCB 132. As discussed below, in some examples, arms 138 can be diametrically spaced to accommodate first sensor 134, second sensor 135, and third sensor 136 between arms 138. In some examples, cap 108 can be configured to receive optical fibers 143, which can connect to PCB 132 and/or first sensor 134 and/or second sensor 135 and/or third sensor 136, as discussed further below.

[0073] In operation of some examples, first sensor 134, second sensor 135, and third sensor 136 can be inactive (or passive) while installed in a patient. A physician or other user can then use an external device to transmit power to antenna coil 118 through induction of electromagnetic field powers. Antenna coil 118 can distribute the power to sensor module 106, and more specifically to communication chip 130. Communication chip 130 can distribute power to first sensor 134, second sensor 135, and third sensor 136, which can initiate their individual measurement sequences. The external device can then remain active, awaiting a return signal from antenna coil 118. Antenna coil 118 also can communicate through load modulation of an externally applied electromagnetic field.

[0074] In operation of some examples, optical fibers 143 can transmit to first sensor 134 and/or second sensor 135 and/or third sensor 136 an optical condition of the environment of a distal portion of femur 204, such as the joint cavity. The sensed condition can be converted and/or correlated to conditions of the environment such as temperature, Ph, and glucose by any of the sensors. First sensor 134 and/or second sensor 135 and/or third sensor 136 can produce sensor signals as a function of sensed conditions that can be transmitted from implantable sensor 100 to an external device (as described further below).

[0075] In some examples, glucose, Ph, and temperature can be used to detect conditions indicative of infection. For example, an elevated temperature can be indicative of the presence of an infection. In other examples, a deviation in glucose or Ph may indicate an infection. The external device can be configured to determine whether or not an infection exists in the sampled environment as a function of the signals received from implantable sensor 100. In addition, a combination of multiple sensors readings can provide a risk indication of local early infection, which can save cost and improve quality of a patient's life. Because sensor 100 is externally powered, sensor 100 does not require internal power, reducing the need for internal capacitors and power, which can have regulatory advantages.

[0076] FIG. 5A illustrates a side view of a cap for an implantable sensor, in accordance with at least one example of this disclosure. FIG. 5B illustrates an isometric view of a cap for a sensor module from a distal perspective, in accordance with at least one example of this disclosure. FIGS. 5A and 5B are discussed concurrently. FIGS. 5A and 5B show cap 108, which can include inner ring 137, arms 138, PCB slots 140, threaded portion 142, optical fibers 143, head portion 150, and passageways 152.

[0077] FIGS. 5A and 5B are consistent with FIGS. 1-4, but show further detail of cap 108, such as head portion 150, which has a diameter that is larger than threaded portion 142 and arms 138. Head portion 150 can include passageways 152, which can be bores, ports, and the like, passing through head portion 150 and part or all of threaded portion 142 to expose passageways 152 to a distal side of cap 108 and an internal portion of secondary insert 104.

[0078] Head portion can have a non-planar surface at a distal end, such that a thickness T of a portion of head portion 150 can be larger than a thickness t of another portion of head portion 150. In one example, ports 152 can be positioned at the portion of head portion 150 having thickness t, which can have the benefit of reducing a length of optical fibers 143.

[0079] FIG. 6 illustrates implantable sensor 100 installed in femoral intramedullary canal 202 of femur 204, and surrounded by femoral implant 212. FIG. 6 shows cap 108, which can include optical fibers 143, head portion 150, and passageways 152. Cap 108 of implantable sensor 100, as shown in FIG. 6, can be connected and operate consistently with FIGS. 1-5. FIG. 6 further shows how cap 108 can be accessed when installed in intramedullary canal 202 of femur 204, even after femoral implant 212 has been installed on femur 204.

[0080] Because cap 108 is accessible when installed in intramedullary canal 202 and because cap 108 is removably threaded to secondary insert 104 (shown in FIG. 3, for example), cap 108 can be removed from secondary insert 104 when implantable sensor is installed in femoral intramedullary canal 202. In some examples, cap 108 can be removed from secondary insert 104 when implantable sensor 100 is installed in femoral intramedullary canal 202 and while femoral implant 212 is installed. By removing cap 108, sensor module 106 can also be removed to allow for replacement or repair of components, such as capacitor 128, without removal of the entirety of implantable sensor 100.

[0081] FIG. 6 also shows how optical fibers 143 pass through passageways 152 to reach an environment around the joint cavity and an environment generally surrounding the distal portion of femur 204. This way, optical fibers 143 can transmit optical information sensed from the environment near the distal area of femur 204, such as synovial fluid, to sensors within implantable sensor 100, such as first sensor 134, second sensor 135, and third sensor 136 (of FIGS. 3 and 4). In some examples, optical fibers 143 may not be included and passageways 152 can act as conduits for synovial fluid (or other fluid), drawing fluid through cap 108 for sensing.

[0082] In operation of some examples, optical fibers 143 can transmit to first sensor 134 an optical condition of the environment of the joint cavity or the environment around the distal termination of femur 204. First sensor 134 can then convert the optical condition into a sensor signal that can be correlated to Ph or glucose of the sensed environment. In some examples, second sensor 135 can produce a second sensor signal as a function of a second sensed condition. Second sensor 135 can also be connected to one or more optical fibers 143 for producing a second sensor signal that can be correlated to Ph or glucose of the sensed environment. In some examples, third sensor 136 can be a temperature sensor, such as a thermistor, for producing a third sensor signal as a function of the temperature around third sensor 136. Because implantable sensor 100 is implanted in

intramedullary canal, the internal temperature of implantable sensor **100** can be similar to the temperature of the environment surrounding implantable sensor **100**, such as the temperature of intramedullary canal **202**, joint cavity, or the environment around the distal portion of femur **204**. Any of first sensor **134**, second sensor **135**, and third sensor **136** can be configured similarly to any other of these sensors described above.

[0083] The sensor signals produced by first sensor **134**, second sensor **135**, and third sensor **136** can be transmitted from implantable sensor **100** (as described further below) to an external device that can be configured to determine whether or not an infection exists in the sampled environment. Not only can infections be harmful to a patient's health, infections can lead to repeated surgery and/or replacement of knee prostheses, sometimes called revision surgeries. By detecting early signs of infection, implantable sensor **100** can alert a patient and/or medical personnel to the existence of an infection, which can help to prevent worsening of infections and can therefore prevent future procedures, such as revisions, saving cost and improving quality of life.

[0084] FIG. 7A illustrates implantable sensor **100A** with antenna coil **118A** installed in femoral intramedullary canal **202** of femur **204** at a first coil angle θ_1 . FIG. 7B illustrates implantable sensor **100B** with antenna coil **118B** installed in femoral intramedullary canal **202** of femur **204** at such that antenna coil **118B** does not have a coil angle. FIG. 7C illustrates implantable sensor **100C** with antenna coil **118C** installed in femoral intramedullary canal **202** of femur **204** at a second coil angle θ_2 .

[0085] Wireless signals transmitted to and from antenna coils **106A-C** can be affected by soft tissues, bones, and femoral implant **212**. In one example, antenna coils **106A-106C** can be optimized to transmit wireless signals by varying an angle of antenna coils **106A-106C**. In some examples, such as the example shown in FIG. 6A, antenna coil **118A** can be placed within proximal portion **110** at first coil angle θ_1 , which can be an angle of 1° through 90° , in some examples. In some other examples, first coil angle θ_1 can be an angle between about 8° and about 10° , such as 9° .

[0086] In some examples, such as the example shown in FIG. 7B, antenna coil **118B** can be placed within proximal portion **110** to have a coil angle of 0° . In some examples, such as the example shown in FIG. 7B, antenna coil **118C** can be placed within proximal portion **110** at second coil angle θ_2 , which can be an angle of -1° through -90° , in some examples. In some other examples, first coil angle θ_1 can be an angle between about -8° and about -10° , such as -9° .

[0087] FIG. 8 illustrates a schematic of sensor module **104**, which can include antenna coil **118**, capacitor **128**, communication chip **130**, PCB **132**, first sensor **134**, second sensor **135**, third sensor **136**, optical fibers **143**, and tuning capacitor **156**.

[0088] Capacitor **128**, communication chip **130**, first sensor **134**, second sensor **135**, third sensor **136**, and tuning capacitor **156** can be soldered to or otherwise coupled to PCB **132**. PCB **132** can include a non-conductive substrate with an etched copper plate as a laminated layer that can provide the electrical connections of PCB **132**.

[0089] Communication chip **130** can be a communication processor configured to receive inputs, process input, and produce output formatted for wireless transmission. For

example, communication chip **130** can be a near field contact chip (NFC) including a low-power microcontroller.

[0090] In some examples, capacitor **128** can be configured to store power received from antenna coil **118**, which can be distributed to power communication chip **130**, which can then be distributed by communication chip **130** to other components of sensor module **104**, as necessary. In some examples, capacitor **128** can be a replaceable battery, and the like, configured to provide power to communication chip **130**, which can then be distributed by communication chip **130** to other components of sensor module **104**, as necessary.

[0091] In some examples, tuning capacitor **156** can be connected in parallel to antenna coil **118** and electrically connected to communication chip **130**. Tuning capacitor **156** can be used for radio frequency (RF) tuning of antenna coil **118** to optimize sending and receiving of wireless signals from and to antenna coil **118**.

[0092] As shown in FIG. 8, first sensor **134** and second sensor **135** can be connected to receive power and control signals from communication chip **130**. First sensor **134** and second sensor **135** can also be communicatively coupled to communication chip **130**. In some examples, optical fibers **143** can connect directly to first sensor **134** and second sensor **135**, as shown in FIG. 8. In some examples, optical fibers **143** can be other types of conductors, such as wires.

[0093] Third sensor **136** is shown as being a resistive temperature sensor, such as a thermistor, and the like. In some other examples, third sensor **136** can be configured similarly to first sensor **134** and second sensor **135**.

[0094] In operation of one embodiment, sensor **100** can be inactive. Then, an external device can transmit power using induction to antenna coil **118**, which can be distributed to communication chip **130** and then on to first sensor **134**, second sensor **135**, and third sensor **136**. Thereafter, first sensor **134**, second sensor **135**, and third sensor **136** can be controlled to take individual measurements by communication chip **130**, as may be instructed by the external device.

[0095] Then, communication chip **130** can receive a first sensor signal from first sensor **134**, a second sensor signal from second sensor **135**, and a third sensor signal from third sensor **136**. Communication chip **130** can analyze and/or format the received sensor signals for wireless transmission via antenna coil **118**. Because first sensor **134**, second sensor **135**, and third sensor **136** can be configured to produce sensor signals indicative of the presence of an infection in an environment surrounding implantable sensor **100**, such as the environment of a human knee, sensor module **104** can enable implantable sensor **100** to transmit wireless signals via communication chip **130** and antenna coil **118** to an external device to help detect the existence of an infection.

[0096] To reduce power consumption, communication chip may send and receive signals to and from first sensor **134**, second sensor **135**, and third sensor **136** in predetermined time intervals. Similarly, communication chip can send and receive signals to and from antenna coil **118** in predetermined time intervals.

[0097] FIG. 9A illustrates an isometric view of secondary insert **104**. FIG. 9B illustrates a plan view of secondary insert **104**. FIG. 9C illustrates a proximal end view of secondary insert **104**. FIG. 9D illustrates a distal end view of primary insert **104**. FIG. 9E illustrates a cross-section view of secondary insert **104** across indicators 9E-9E of FIG. 9A.

FIG. 9F illustrates a cross-section view of secondary insert **104** across indicators **9F-9F** of FIG. 9E. FIGS. 9A-9F are discussed concurrently.

[0098] FIGS. 9A-9F are consistent with FIGS. 1, 3, and 4 discussed above, but show additional details of secondary insert **104**, which can include snap fits **120** having projections **123**, and can include coil connector **122**, secondary insert bore **146**, internal threaded portion **148**, ribs **158**, rib channels **160**, and distal channels **162**.

[0099] As shown in FIG. 9E, secondary insert bore **146** can extend from a distal end of secondary insert **104** towards and through a proximal end. Secondary insert bore **146** can have a diameter that varies. For example, a diameter of secondary insert bore **146** can be larger between the proximal and distal ends of secondary insert **104** to accommodate sensor module **106**, as shown in FIGS. 3 and 4. Secondary insert bore **146** can be smaller at the proximal end of secondary insert **104** to provide a passage sized to secure coil connector **122**. Further, secondary insert bore **146** can be smaller at the proximal end of secondary insert **104** to provide additional material thickness for snap fits **120**. At the distal end of secondary insert **104**, secondary insert bore **146** can include internal threaded portion **148** that can be configured to threadably engage threaded portion **142** of cap **108**, as shown in FIGS. 3 and 4.

[0100] In some examples, secondary insert **104** can include ribs **158**, which can extend axially along an outer surface of secondary insert **104** between the distal and proximal ends of secondary insert **104**. As shown in FIG. 9E, ribs **158** can have radial projections having a geometric shape similar to a triangular prism, in some examples, but can have other geometric shapes in some other examples. Ribs **158** can be placed around an entirety of the circumference of secondary insert **104**, in some examples. In some other examples, ribs **158** can be interrupted by rib channels **160**, as described further below. Ribs **158** can be spaced by angle A, as shown in FIG. 9F. Angle A can be an angle of about 5° to about 180° in some examples. In some examples, angle A can be an angle of about 10° to about 20° in other examples, such as 15°, for example. The geometric shape and spacing of ribs **158** can dictate a quantity of ribs **158** disposed around the circumference of secondary insert **104**. In the example of FIG. 9F, the ribs can be spaced at 15°, except for where rib grooves create a larger space between ribs **158**, such that 20 of ribs **158** are spaced around the circumference of secondary insert **104**.

[0101] In operation of some examples, ribs **158** can engage with grooves of primary insert **102** (shown in later figures), to circumferentially secure secondary insert **104** within primary insert **102**. In some examples, the consistent spacing between ribs **158** and the uniform geometry of ribs **158** can allow secondary insert **104** to be inserted and secured in primary insert **102** in a variety of positions, as discussed further below.

[0102] In some examples, secondary insert **104** can include rib channels **160**, which can extend axially along an outer surface of secondary insert **104** between the distal and proximal ends. Rib channels **160** can be approximately the same length as ribs **158**. In some examples, rib channels can be a space between ribs **158**, and in some examples, rib channels **160** can be a groove or channel in the outer surface of secondary insert **104**.

[0103] In some examples, secondary insert **104** can include distal channels **162**, which can be a groove or

channel formed in the outer surface of secondary insert **104** proximate the distal end. Distal channels **162** can have a quantity equal to the quantity of rib channels **160**, and can be circumferentially aligned with rib channels **160**. In operation of some examples, rib channels **160** and distal channels **162** can be configured to allow air to escape from primary insert **102** when secondary insert **104** is inserted into primary insert **102**. This can prevent a pressure from building within primary insert **102** during installation of secondary insert **104**.

[0104] FIG. 10A illustrates a plan view of primary insert **102**, in accordance with at least one example of this disclosure. FIG. 10B illustrates a cross-section view of primary insert **102** across indicators **10B-10B** of FIG. 10A, in accordance with at least one example of this disclosure. FIG. 10C illustrates a cross-section view of primary insert **102** across indicators **10C-10C** of FIG. 10B, in accordance with at least one example of this disclosure. FIGS. 10A-10C are discussed concurrently.

[0105] FIGS. 10A-10C are consistent with FIGS. 1, 3, and 4 below, but show additional details of primary insert **102**, which can include proximal portion **110**, distal portion **112**, proximal end **114**, distal end **116**, central bore **144**, fins **164**, distal opening **166**, alignment grooves **168**, and distal flange **170**.

[0106] Central bore **144** can be a bore beginning at distal opening **166** proximate distal end **116** and extending through distal portion **112** and proximal portion **110**, terminating in proximal portion **110** prior to proximal end **114**. In some examples, central bore **144** can have a diameter in proximal portion **110** that is larger than a second diameter in distal portion **112**.

[0107] Fins **164** can be radial projections extending axially along an outer surface of distal portion **112** of primary insert **102**. Fins **164** can be circumferentially disposed around distal portion **112** and can include a quantity of fins **164** such as 1, 2, 3, 4, 5, 6, 10, 15, and the like. Fins **164** can be configured to engage an intramedullary canal of a femur, such as intramedullary canal **202** of FIG. 2, to prevent axial and rotational movement of primary insert **102** relative to intramedullary canal **202** and femur **204**, for example.

[0108] Distal flange **170** can be integral to distal portion **112** and can be located at distal end **116**. Distal flange **170** can have an outer diameter that is larger than a diameter of distal portion **112** and equal to an outer diametric dimension of fins **164**. In operation of some examples, distal flange **170** can provide a mating surface for cap **108**.

[0109] Alignment grooves **168** can be grooves formed in an inner surface of distal portion **112**, that extend radially into central bore **144** and extend axially along bore **144** beginning proximate distal end **116** and terminating prior to proximal portion **110**. Alignment grooves **168** can be spaced by angle B, as shown in FIG. 10C. Angle B can be an angle of about 5° to about 180° in some examples. In some examples, angle B can be an angle of about 10° to about 20° in other examples, such as 15°, for example.

[0110] The geometric shape and spacing of alignment grooves **168** can be designed to mate with ribs **158** of FIGS. 9A-9F. In this way, ribs **158** can be required to align with alignment grooves **168** for secondary insert **104** to be inserted into primary insert **102**. Alignment grooves **168** can be configured to have a relatively tight fit with ribs **158** so that secondary insert **104** can be easily inserted into and removed from primary insert **102** while preventing second-

ary insert **104** from rotating relative to primary insert **102** while secondary insert **104** is within primary insert **102**.

[0111] Because alignment grooves **168** are of the same shape and size as ribs **158**, secondary insert **104** can be inserted into primary insert **102** in many orientations. In operation of some examples, the exposure of optical fibers **143** (of FIG. 3, for example) to synovial fluid around femur **204** (of FIG. 2, for example) can be improved by altering an orientation of secondary insert **104** relative to primary insert **102** during a procedure. That is, once cap **108** (of FIG. 3, for example) is secured to secondary insert **104**, the position of optical fibers **143** are fixed relative to cap **108** and secondary insert **104**. And, once primary insert **102** is installed into a femur, such as femur **204** (of FIG. 2, for example), a position of primary insert **102** is fixed relative to femur **204**. Therefore, after primary insert **102** has been installed in intramedullary canal **102**, secondary insert **104** can be rotated to optimize exposure of optical fibers **143** to their surrounding environment, such as the joint cavity, which can improve sensor performance.

[0112] FIGS. 11A-11C illustrate steps of a surgical procedure, in accordance with at least one example of this disclosure. In the step shown in FIG. 11A, a bore can be drilled using drill **1100** in intramedullary canal **202** of femur **204**. In the step shown in FIG. 11B, each of trial rods **1104A-1104D** can be inserted into the bore drilled in intramedullary canal **204** for the purpose of selecting a size of implantable sensor **100** that will have an appropriate fit within intramedullary canal **202**. In the step shown in FIG. 11C, implantable sensor **100** having an appropriate size can be inserted into intramedullary canal **202**, where mallet **1106** can be used to apply the force necessary to entirely insert and secure implantable sensor **100** into intramedullary canal **202** of femur **204**.

[0113] FIG. 12 illustrates a schematic of components of sensor system **1200**, in accordance with at least one example of this disclosure. Sensor system **1200** includes sensor **1202**, external device **1204**, central device **1206**, central device database **1208**, expert device **1210**, and connection medium **1212**.

[0114] Sensor **1202** can be an implantable sensor consistent with FIGS. 1-10. External device **1204** can be a portable device, such as a handheld computer, for example, a smart phone, a tablet, a laptop with a connected sensor, or any other portable computing device including a processor and wireless communication capabilities. In yet other examples, expert device **1204** can include only transmitting and energy transmitting functionalities. Central device **1206** and expert device **1210** can be a portable device, as described above, or can be a stationary device or devices, such as a desktop computer or a central server system accessible through a program or online interface, such as a web page. Central device database **1208** can be a database for storing measurements and analysis from external device **1204**, central device **1206**, and expert device **1210**. Central device database **1208**, external device **1204**, central device **1206**, and expert device **1210** can include machine readable medium. The terms "machine readable medium" may include any medium that is capable of storing, encoding, or carrying instructions for execution by the device and that cause the device to perform any one or more of the techniques of the present disclosure, or that is capable of storing, encoding or carrying data structures used by or associated with such instructions. Non-limiting machine readable medium

examples may include solid-state memories, and optical and magnetic media. Specific examples of machine readable media may include: non-volatile memory, such as semiconductor memory devices (e.g., Electrically Programmable Read-Only Memory (EPROM), Electrically Erasable Programmable Read-Only Memory (EEPROM)) and flash memory devices; magnetic disks, such as internal hard disks and removable disks; magneto-optical disks; and CD-ROM and DVD-ROM disks.

[0115] Connection medium **1212** can be a communication network utilizing any one of a number of transfer protocols (e.g., frame relay, internet protocol (IP), transmission control protocol (TCP), user datagram protocol (UDP), hypertext transfer protocol (HTTP), etc.). Example communication networks may include a local area network (LAN), a wide area network (WAN), a packet data network (e.g., the Internet), mobile telephone networks (e.g., cellular networks), Plain Old Telephone (POTS) networks, and wireless data networks (e.g., Institute of Electrical and Electronics Engineers (IEEE) 802.11 family of standards known as Wi-Fi® or IEEE 802.15.4 family of standards known as ZigBee®), as the personal area network family of standards known as Bluetooth® that are promulgated by the Bluetooth Special Interest Group, peer-to-peer (P2P) networks, among others. Connection medium **1212** can also be a combination of networks.

[0116] Sensor **1202** can be in communication with external device **1204** through a wireless connection, such as Bluetooth, NFC, wi-fi, other electromagnetic based communication protocols, and the like. External device **1204**, central device **1206**, central device database **1208**, and expert device **1210** can be in wireless or wired communication with connection medium **1212**. Sensor system **1200** can operate as described in the FIGS. above, and in the method described below in FIG. 13.

[0117] FIG. 13 illustrates a method **1300** of using sensor system **1200** of FIG. 12, in accordance with at least one example of this disclosure. The steps or operations of method **1300** are illustrated in a particular order for convenience and clarity; many of the discussed operations can be performed in a different sequence or in parallel without materially impacting other operations. Method **1300** as discussed includes operations performed by multiple different actors, devices, and/or systems. It is understood that subsets of the operations discussed in method **1300** attributable to a single actor, device, or system could be considered a separate standalone process or method. At step **1302**, the method **1300** can begin with an intramedullary canal being drilled, so that an implantable sensor can be inserted into the intramedullary canal at step **1304**. At step **1306**, the method **1300** can continue with a computing device, such as external device **1204** of FIG. 12, connecting to the sensor. At this time, a communicative link can be confirmed and transmission of power and data can occur between the external device and sensor to functionally test the connection.

[0118] After completion of the surgical procedure at step **1308**, the external device can distribute power to sensor **1202**, enabling communication between the external device and sensor **1202**, which is implanted into the patient. For example, sensor data, such as temperature, Ph, and glucose readings, can be transmitted from sensor **1202** to external device **1204**. External device **1204** can perform analysis and then communicate with central device **1206** at step **1312**.

Central device **1206** can perform further analysis at step **1314**, before communicating with expert device **1210** at step **1316**. In some examples, analysis can be performed in external device **1204** at step **1310** prior to communication with central device **1206**.

[0119] Analysis performed at steps **1314** and **1318** can include analyzing data from sensor **1202** to determine the presence of an infection. Other analysis such as determining remaining capacitor health, signal strength, and component functionality may also be performed. In some examples, where the device is battery-powered, wireless charging of the battery can be performed.

[0120] At step **1318** an expert may perform analysis outside of expert device **1210**, which can then be entered into expert device **1210**. Thereafter, expert device **1210** can then communicate with central device **1206** at step **1320** to relay any additional data and/or analysis performed at step **1318**. Thereafter, all of the analysis and data derived from central device **1206**, central device database **1208**, and expert device **1210** can be communicated to external device **1204** at step **1322**, where a user can view the data and analysis to make a decision regarding the joint in which sensor **1202** is installed, or can receive an instruction containing a decision.

[0121] This method offers the benefit of providing measurement data from within a joint containing a prosthesis that can be used to detect the presence of an infection. Moreover, the data can be sent to multiple devices, such as an external device, a central device, a central device database, and an expert device, to provide detailed and in-depth analysis on the data retrieved, such as comparing the data to data received from other sensors, and analysis performed by experts possessing knowledge not readily available, to determine the presence of an infection or other problem.

[0122] Method examples described herein may be machine or computer-implemented at least in part. Some examples may include a computer-readable medium or machine-readable medium encoded with instructions operable to configure an electronic device to perform methods as described in the above examples. An implementation of such methods may include code, such as microcode, assembly language code, a higher-level language code, or the like. Such code may include computer readable instructions for performing various methods. The code may form portions of computer program products. Further, in an example, the code may be tangibly stored on one or more volatile, non-transitory, or non-volatile tangible computer-readable media, such as during execution or at other times. Examples of these tangible computer-readable media may include, but are not limited to, hard disks, removable magnetic disks, removable optical disks (e.g., compact disks and digital video disks), memory cards or sticks, random access memories (RAMs), read only memories (ROMs), and the like.

[0123] The above detailed description includes references to the accompanying drawings, which form a part of the detailed description. The drawings show, by way of illustration, specific embodiments in which the invention can be practiced. These embodiments are also referred to herein as “examples.” Such examples can include elements in addition to those shown or described. However, the present inventors also contemplate examples in which only those elements shown or described are provided. Moreover, the present inventors also contemplate examples using any combination or permutation of those elements shown or

described (or one or more aspects thereof), either with respect to a particular example (or one or more aspects thereof), or with respect to other examples (or one or more aspects thereof) shown or described herein.

[0124] In the event of inconsistent usages between this document and any documents so incorporated by reference, the usage in this document controls.

[0125] In this document, the terms “a” or “an” are used, as is common in patent documents, to include one or more than one, independent of any other instances or usages of “at least one” or “one or more.” In this document, the term “or” is used to refer to a nonexclusive or, such that “A or B” includes “A but not B,” “B but not A,” and “A and B,” unless otherwise indicated. In this document, the terms “including” and “in which” are used as the plain-English equivalents of the respective terms “comprising” and “wherein.” Also, in the following claims, the terms “including” and “comprising” are open-ended, that is, a system, device, article, composition, formulation, or process that includes elements in addition to those listed after such a term in a claim are still deemed to fall within the scope of that claim. Moreover, in the following claims, the terms “first,” “second,” and “third,” etc. are used merely as labels, and are not intended to impose numerical requirements on their objects.

[0126] The above description is intended to be illustrative, and not restrictive. For example, the above-described examples (or one or more aspects thereof) may be used in combination with each other. Other embodiments can be used, such as by one of ordinary skill in the art upon reviewing the above description. The Abstract is provided to comply with 37 C.F.R. § 1.72(b), to allow the reader to quickly ascertain the nature of the technical disclosure. It is submitted with the understanding that it will not be used to interpret or limit the scope or meaning of the claims. Also, in the above Detailed Description, various features may be grouped together to streamline the disclosure. This should not be interpreted as intending that an unclaimed disclosed feature is essential to any claim. Rather, inventive subject matter may lie in less than all features of a particular disclosed embodiment. Thus, the following claims are hereby incorporated into the Detailed Description as examples or embodiments, with each claim standing on its own as a separate embodiment, and it is contemplated that such embodiments can be combined with each other in various combinations or permutations. The scope of the invention should be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled.

1. An implantable sensor configured to be inserted in an intramedullary canal, the implantable sensor comprising:
 - a primary insert including a distal end, a proximal end opposite the distal end, and a central bore extending from an opening in the distal end towards the proximal end;
 - a secondary insert receivable within the central bore through the opening, the secondary insert comprising:
 - a body removably engageable with an inside surface of the central bore; and
 - a sensor module disposable within the body and configured to produce a sensor signal as a function of a first sensed parameter indicative of infection; and
- an antenna disposed in the central bore, the antenna configured to:

- transmit a wireless signal as a function of the sensor signal.
2. The implantable sensor of claim 1, wherein the sensor comprises one of a temperature sensor, a pH sensor, an oxygen sensor, a carbon dioxide sensor, and a glucose sensor.
 3. The implantable sensor of claim 1, wherein the antenna is configured to receive power from an external source and distribute the power to the sensor.
 4. The implantable sensor of claim 1, wherein the secondary insert further comprises:
 - a cap releasably securable to the secondary insert.
 5. The implantable sensor of claim 4, wherein the cap and sensor module are releasable from the secondary insert while the secondary insert is inserted in the intramedullary canal.
 6. The implantable sensor of claim 4, wherein the cap further comprises:
 - a plurality of legs projecting proximally from a proximal surface of the cap and configured to retain the sensor capsule.
 7. The implantable sensor of claim 1, wherein the secondary insert further comprises:
 - a second sensor configured to produce a second sensor signal as a function of a second sensed parameter indicative of infection.
 8. The implantable sensor of claim 7, wherein the secondary insert further comprises:
 - a third sensor configured to produce a third sensor signal as a function of a third sensed parameter indicative of infection.
 9. The implantable sensor of claim 1, wherein the secondary insert further comprises:
 - an optical fiber connected to the sensor and extending through a periphery of the secondary insert to expose the optical fiber to a joint cavity adjacent to the intramedullary canal to send an optical signal to the sensor as a function of sensed optical conditions of the joint cavity.
 10. The implantable sensor of claim 9, further comprising:
 - a cap releasably securable to the secondary insert, the cap comprising:
 - a passage exposing the sensor module to the joint cavity, the passage receivable of the optical fiber.
 11. The implantable sensor of claim 1, wherein the central bore further comprises a plurality of grooves extending axially along a surface of the central bore, and wherein the secondary insert further comprises a plurality of ribs projecting radially outward from an outer surface of the secondary insert and extending axially along the outer surface, the plurality of ribs mateable with the plurality of grooves to prevent rotation of the secondary insert relative to the primary insert.
 12. A system for monitoring a joint cavity, the system comprising:
 - an implantable sensor comprising:
 - a femoral insert implantable in a femoral intramedullary canal adjacent to the joint cavity, the femoral insert comprising:
 - a proximal end and a distal end; and
 - a central bore extending from the distal end through the distal portion and terminating prior to the proximal end;
 - a sensor insertable into the central bore through the distal end, the sensor configured to produce a sensor signal as a function of a sensed condition of the joint cavity; and
 - an antenna disposed in the central bore, the antenna configured to:
 - transmit a wireless signal as a function of the sensor signal; and
 - receive power and distribute the power to the sensor.
 - an external computing device comprising:
 - a communication circuit configured to wirelessly receive the sensor signal transmitted via the antenna and deliver power to the antenna;
 - a processor communicatively coupled to the communication circuit and configured to process the sensor signal and generate a graphical user-interface as a function of the sensor signal; and
 - a display device communicatively coupled to the processor and configured to display the graphical user-interface.
 13. The system of claim 12, further comprising:
 - a central device in communication with the external computing device, the central device configured to analyze data received from the external computing device and return analysis to the external computing device.
 14. The system of claim 13, further comprising:
 - an expert device in communication with at least one of the external computing device and the central device, the expert device configured to:
 - analyze data received from at least one of the external computing device the central device; and
 - analyze analysis received from the central device.
 15. The sensor module of claim 12, wherein the secondary insert further comprises:
 - a communication chip connected to the antenna and the sensor, the communication chip configured to process the sensor signal and distribute power from the antenna to the sensor.
 16. The sensor module of claim 15, wherein the communication chip comprises a near field communication chip.
 17. An intramedullary implant configured to be inserted in a femoral intramedullary canal, the intramedullary implant comprising:
 - a housing insertable into a femoral intramedullary canal, the housing comprising:
 - a proximal portion including a proximal end;
 - a distal portion including a distal end; and
 - a bore extending from the distal end towards the proximal end;
 - a secondary insert receivable in the bore, the secondary insert engageable with an internal surface of the bore, and including a sensor configured to produce a sensor signal as function of a first sensed parameter of a joint cavity adjacent the intramedullary canal, the first sensed parameter indicative of infection; and
 - an antenna coil disposed in the proximal portion, the antenna configured to transmit a wireless signal as a function of the sensor signal.
 18. The implantable sensor of claim 17, wherein the secondary insert comprises a snap fit connection securable to the central bore.
 19. The implantable sensor of claim 18, wherein the snap fit connection comprises a plurality of straight arms, each

arm of the plurality of arms including a projection extending radially from a proximal termination of each arm.

20. The implantable sensor of claim 17, wherein the antenna coil is positionable within the proximal portion to change a coil angle relative to the sensor module.

* * * * *

专利名称(译)	植入式膝关节传感器及使用方法		
公开(公告)号	US20180184944A1	公开(公告)日	2018-07-05
申请号	US15/399131	申请日	2017-01-05
[标]申请(专利权)人(译)	拜欧米特制造有限责任公司		
申请(专利权)人(译)	BIOMET制造有限责任公司		
当前申请(专利权)人(译)	BIOMET制造有限责任公司		
[标]发明人	BODEWES HILBRANDUS H KHAN MOHAMMED IMRAN LASZLO DELI DANIEL HOEBOER MAX ABDEL ALIM VAN DEN BERG LISA VAN OPSTAL SIEMON KOPERDRAAT BONITA KRIJGSMAN BART HEERINK JURRIT		
发明人	BODEWES, HILBRANDUS H. KHAN, MOHAMMED IMRAN LASZLO-DELI, DANIEL HOEBOER, MAX ABDEL ALIM-VAN DEN BERG, LISA VAN OPSTAL, SIEMON KOPERDRAAT, BONITA KRIJGSMAN, BART HEERINK, JURRIT		
IPC分类号	A61B5/07 A61B5/01 A61B5/145 A61B5/1455 A61B5/00 A61B5/1459		
CPC分类号	A61B5/076 A61B5/01 A61B5/14539 A61B5/14551 A61B2560/0219 A61B5/0031 A61B5/6878 A61B5/1459 A61B5/14532 A61B5/0008 A61B5/4504 A61B5/4528 A61F2/30721 A61F2/38 A61F2002/30668 A61F2002/30878		
外部链接	Espacenet USPTO		

摘要(译)

配置成插入髓内管的可植入传感器可包括主插入件，辅助插入件和天线。主插入件可包括远端，与远端相对的近端，以及可从远端中的开口朝向近端延伸的中心孔。辅助插入件可以通过开口容纳在中心孔内。辅助插入件可包括主体和传感器模块。主体可以与中心孔的内表面可拆卸地接合。传感器模块可以在身体内是一次性的，并且可以配置成根据指示感染的第一感测参数产生传感器信号。天线可以设置在中心孔中。天线可以被配置为根据传感器信号发送无线信号。

