



US010165946B2

(12) **United States Patent**
Bardy et al.

(10) **Patent No.:** **US 10,165,946 B2**
(45) **Date of Patent:** **Jan. 1, 2019**

(54) **COMPUTER-IMPLEMENTED SYSTEM AND METHOD FOR PROVIDING A PERSONAL MOBILE DEVICE-TRIGGERED MEDICAL INTERVENTION**

(71) Applicant: **Bardy Diagnostics, Inc.**, Vashon, WA (US)

(72) Inventors: **Gust H. Bardy**, Carnation, WA (US);
Jason Felix, Vashon Island, WA (US);
Jon Mikalson Bishay, Seattle, WA (US)

(73) Assignee: **Bardy Diagnostics, Inc.**, Seattle, WA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **14/217,402**

(22) Filed: **Mar. 17, 2014**

(65) **Prior Publication Data**
US 2015/0088007 A1 Mar. 26, 2015

Related U.S. Application Data
(63) Continuation-in-part of application No. 14/082,071, filed on Nov. 15, 2013, now Pat. No. 9,433,367, (Continued)

(51) **Int. Cl.**
A61B 5/02 (2006.01)
A61B 5/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/0022** (2013.01); **A61B 5/024** (2013.01); **A61B 5/0205** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC G06F 19/3406; G06F 19/3412; G06F 19/3418; G06F 19/3475; G06F 19/3456; A61B 5/0022; A61B 5/0002
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,215,136 A 11/1965 Holter et al.
3,569,852 A 3/1971 Berkovits
(Continued)

FOREIGN PATENT DOCUMENTS

DE 19955211 5/2001
EP 1859833 11/2007
(Continued)

OTHER PUBLICATIONS

US 6,527,714, 03/2003, Bardy (withdrawn)
(Continued)

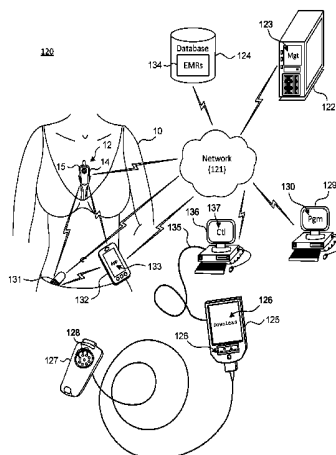
Primary Examiner — Niketa Patel

Assistant Examiner — Nathan A Baldwin

(74) *Attorney, Agent, or Firm* — Patrick J. S. Inouye;
Krista A. Wittman

(57) **ABSTRACT**

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. The wearable monitor sits centrally on the patient's chest along the sternum oriented top-to-bottom. The placement of the wearable monitor in a location at the sternal midline (or immediately to either side of the sternum) benefits extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. The wearable monitor can interoperate wirelessly with other physiology and activity sensors and mobile devices. An application executed by the sensor or device can trigger the dispatch of a wearable monitor to the patient upon detecting potentially medically-significant events. The dispatched wearable monitor would then be capable of providing precise medically-actionable data, not merely an alert that some abnormality may be present. The patient can then use the sensor or device to physically record the placement and use of the
(Continued)



medically-actionable wearable monitor, thereby facilitating the authentication of the data recorded.

20 Claims, 8 Drawing Sheets

Related U.S. Application Data

which is a continuation-in-part of application No. 14/080,717, filed on Nov. 14, 2013, now Pat. No. 9,545,204, which is a continuation-in-part of application No. 14/080,725, filed on Nov. 14, 2013, now Pat. No. 9,730,593.

(60) Provisional application No. 61/882,403, filed on Sep. 25, 2013.

(51) Int. Cl.

A61B 5/0205 (2006.01)

A61B 5/024 (2006.01)

G06F 19/00 (2018.01)

(52) U.S. Cl.

CPC **A61B 5/7282** (2013.01); **G06F 19/00** (2013.01); **G06F 19/3418** (2013.01)

(56) References Cited

U.S. PATENT DOCUMENTS

3,699,948 A 10/1972 Ota et al.
3,893,453 A 7/1975 Goldberg
4,123,785 A 10/1978 Cherry et al.
4,328,814 A 5/1982 Arkans
4,441,500 A 4/1984 Sessions et al.
4,532,934 A 8/1985 Kelen
4,546,342 A 10/1985 Weaver et al.
4,550,502 A 11/1985 Grayzel
4,580,572 A 4/1986 Granek et al.
4,635,646 A 1/1987 Gilles et al.
4,653,022 A 3/1987 Koro
4,716,903 A 1/1988 Hansen
4,809,705 A 3/1989 Ascher
4,915,656 A 4/1990 Alferness
5,007,429 A 4/1991 Treatch et al.
5,025,794 A 6/1991 Albert et al.
5,107,480 A 4/1992 Naus
5,168,876 A 12/1992 Quedens et al.
5,215,098 A 6/1993 Steinhaus
D341,423 S 11/1993 Bible
5,265,579 A 11/1993 Ferrari
5,333,615 A 8/1994 Craelius et al.
5,341,806 A 8/1994 Gadsby et al.
5,355,891 A 10/1994 Wateridge et al.
5,365,934 A 11/1994 Leon et al.
5,365,935 A 11/1994 Righter et al.
5,392,784 A 2/1995 Gudaitis
D357,069 S 4/1995 Plahn et al.
5,402,780 A 4/1995 Faasse, Jr.
5,402,884 A 4/1995 Gilman et al.
5,450,845 A 9/1995 Axelgaard
5,458,141 A 10/1995 Neil
5,473,537 A 12/1995 Glazer et al.
5,483,969 A 1/1996 Testerman et al.
5,511,553 A 4/1996 Segalowitz
5,540,733 A 7/1996 Testerman et al.
5,546,952 A 8/1996 Erickson
5,549,655 A 8/1996 Erickson
5,579,919 A 12/1996 Gilman et al.
5,582,181 A 12/1996 Ruess
D377,983 S 2/1997 Sabri et al.
5,601,089 A 2/1997 Bledsoe et al.
5,623,935 A 4/1997 Faisandier
5,682,901 A 11/1997 Kamen
5,697,955 A 12/1997 Stolte

5,749,902 A 5/1998 Olsen et al.
5,788,633 A 8/1998 Mahoney
5,817,151 A 10/1998 Olsen et al.
5,819,741 A 10/1998 Karlsson et al.
5,850,920 A 12/1998 Gilman et al.
D407,159 S 3/1999 Roberg
5,876,351 A 3/1999 Rohde
5,906,583 A 5/1999 Rogel
5,951,598 A 9/1999 Bishay et al.
5,957,857 A 9/1999 Hartley
5,984,102 A 11/1999 Tay
6,032,064 A 2/2000 Devlin et al.
6,038,469 A 3/2000 Karlsson et al.
6,101,413 A 8/2000 Olsen et al.
6,115,638 A 9/2000 Groenke
6,117,077 A 9/2000 Del Mar et al.
6,134,479 A 10/2000 Brewer et al.
6,148,233 A 11/2000 Owen et al.
6,149,602 A 11/2000 Arcelus
6,149,781 A 11/2000 Forand
6,188,407 B1 2/2001 Smith et al.
D443,063 S 5/2001 Pisani et al.
6,245,025 B1 6/2001 Torok et al.
6,246,330 B1 6/2001 Nielsen
6,249,696 B1 6/2001 Olson et al.
D445,507 S 7/2001 Pisani et al.
6,269,267 B1 7/2001 Bardy et al.
6,272,385 B1 8/2001 Bishay et al.
6,298,255 B1 10/2001 Cordero et al.
6,301,502 B1 10/2001 Owen et al.
6,304,773 B1 10/2001 Taylor et al.
6,304,780 B1 10/2001 Owen et al.
6,304,783 B1 10/2001 Lyster et al.
6,374,138 B1 4/2002 Owen et al.
6,381,482 B1 4/2002 Jayaraman et al.
6,416,471 B1 7/2002 Kumar et al.
6,418,342 B1 7/2002 Owen et al.
6,424,860 B1 7/2002 Karlsson et al.
6,427,083 B1 7/2002 Owen et al.
6,454,708 B1 9/2002 Ferguson et al.
6,456,872 B1 9/2002 Faisandier
6,463,320 B1 10/2002 Xue et al.
6,546,285 B1 4/2003 Owen et al.
6,605,046 B1 8/2003 Del Mar
6,607,485 B2 8/2003 Bardy
6,611,705 B2 8/2003 Hopman et al.
6,671,545 B2 12/2003 Fincke
6,671,547 B2 12/2003 Lyster et al.
6,694,186 B2 2/2004 Bardy
6,704,595 B2 3/2004 Bardy
6,705,991 B2 3/2004 Bardy
6,719,701 B2 4/2004 Lade
6,754,523 B2 6/2004 Toole
6,782,293 B2 8/2004 Dupelle et al.
6,856,832 B1 2/2005 Matsumura et al.
6,860,897 B2 3/2005 Bardy
6,866,629 B2 3/2005 Bardy
6,887,201 B2 5/2005 Bardy
6,893,397 B2 5/2005 Bardy
6,904,312 B2 6/2005 Bardy
6,908,431 B2 6/2005 Bardy
6,913,577 B2 7/2005 Bardy
6,944,498 B2 9/2005 Owen et al.
6,960,167 B2 11/2005 Bardy
6,970,731 B1 11/2005 Jayaraman et al.
6,978,169 B1 12/2005 Guerra
6,993,377 B2 1/2006 Flick et al.
7,020,508 B2 3/2006 Stivoric et al.
7,027,864 B2 4/2006 Snyder et al.
7,065,401 B2 6/2006 Worden
7,085,601 B1 8/2006 Bardy et al.
7,104,955 B2 9/2006 Bardy
7,134,996 B2 11/2006 Bardy
7,137,389 B2 11/2006 Berthon-Jones
7,147,600 B2 12/2006 Bardy
7,215,991 B2 5/2007 Besson et al.
7,248,916 B2 7/2007 Bardy
7,257,438 B2 8/2007 Kinast
7,277,752 B2 10/2007 Matos

(56)

References Cited

U.S. PATENT DOCUMENTS

D558,882	S	1/2008	Brady		2003/0004547	A1	1/2003	Owen et al.
7,328,061	B2	2/2008	Rowlandson et al.		2003/0073916	A1	4/2003	Yonce
7,412,395	B2	8/2008	Rowlandson et al.		2003/0083559	A1	5/2003	Thompson
7,429,938	B1	9/2008	Corndorf		2003/0097078	A1	5/2003	Maeda
7,552,031	B2	6/2009	Vock et al.		2003/0139785	A1	7/2003	Riff et al.
D606,656	S	12/2009	Kobayashi et al.		2003/0176802	A1	9/2003	Galen et al.
7,706,870	B2	4/2010	Shieh et al.		2003/0211797	A1	11/2003	Hill et al.
7,756,721	B1	7/2010	Falchuk et al.		2004/0008123	A1	1/2004	Carrender
7,787,943	B2	8/2010	McDonough		2004/0019288	A1	1/2004	Kinast
7,874,993	B2	1/2011	Bardy		2004/0034284	A1	2/2004	Aversano et al.
7,881,785	B2	2/2011	Nassif et al.		2004/0049132	A1	3/2004	Barron et al.
D639,437	S	6/2011	Bishay et al.		2004/0073127	A1	4/2004	Istvan et al.
7,959,574	B2	6/2011	Bardy		2004/0087836	A1	5/2004	Green et al.
8,116,841	B2	2/2012	Bly et al.		2004/0088019	A1	5/2004	Rueter et al.
8,172,761	B1 *	5/2012	Rulkov	A61B 5/01	2004/0093192	A1	5/2004	Hasson et al.
				600/301	2004/0148194	A1	7/2004	Wellons et al.
					2004/0207530	A1	10/2004	Nielsen
8,180,425	B2	5/2012	Selvitelli et al.		2004/0236202	A1	11/2004	Burton
8,200,320	B2	6/2012	Kovacs		2004/0243435	A1	12/2004	Williams
8,231,539	B2	7/2012	Bardy		2004/0256453	A1	12/2004	Lammle
8,231,540	B2	7/2012	Bardy		2004/0260188	A1	12/2004	Syed et al.
8,239,012	B2	8/2012	Felix et al.		2004/0260192	A1	12/2004	Yamamoto
8,249,686	B2	8/2012	Libbus et al.		2005/0096717	A1	5/2005	Bishay et al.
8,260,414	B2	9/2012	Nassif et al.		2005/0108055	A1	5/2005	Ott et al.
8,266,008	B1	9/2012	Siegal et al.		2005/0154267	A1	7/2005	Bardy
8,277,378	B2	10/2012	Bardy		2005/0182308	A1	8/2005	Bardy
8,285,356	B2	10/2012	Bly et al.		2005/0182309	A1	8/2005	Bardy
8,285,370	B2	10/2012	Felix et al.		2005/0215918	A1	9/2005	Frantz et al.
8,308,650	B2	11/2012	Bardy		2005/0222513	A1	10/2005	Hadley et al.
8,366,629	B2	2/2013	Bardy		2005/0228243	A1	10/2005	Bardy
8,374,688	B2	2/2013	Libbus et al.		2005/0245839	A1	11/2005	Stivoric et al.
8,412,317	B2	4/2013	Mazar		2006/0025696	A1	2/2006	Kurzweil et al.
8,460,189	B2	6/2013	Libbus et al.		2006/0025824	A1	2/2006	Freeman et al.
8,473,047	B2	6/2013	Chakravarthy et al.		2006/0030767	A1	2/2006	Lang et al.
8,478,418	B2	7/2013	Fahey		2006/0041201	A1	2/2006	Behbehani et al.
8,554,311	B2	10/2013	Warner et al.		2006/0122469	A1	6/2006	Martel
8,591,430	B2	11/2013	Amurthur et al.		2006/0124193	A1	6/2006	Orr et al.
8,594,763	B1	11/2013	Bibian et al.		2006/0224072	A1	10/2006	Shennib
8,600,486	B2	12/2013	Kaib et al.		2006/0235320	A1	10/2006	Tan et al.
8,613,708	B2	12/2013	Bishay et al.		2006/0253006	A1	11/2006	Bardy
8,613,709	B2	12/2013	Bishay et al.		2006/0264730	A1	11/2006	Stivoric et al.
8,620,418	B1	12/2013	Andover		2006/0264767	A1	11/2006	Shennib
8,626,277	B2	1/2014	Felix et al.		2007/0003115	A1	1/2007	Patton et al.
8,628,020	B2	1/2014	Beck		2007/0038057	A1	2/2007	Nam et al.
8,668,653	B2	3/2014	Nagata et al.		2007/0050209	A1	3/2007	Yered
8,684,925	B2	4/2014	Manicka et al.		2007/0078324	A1	4/2007	Wijisiriwardana
8,688,190	B2	4/2014	Libbus et al.		2007/0078354	A1	4/2007	Holland
8,718,752	B2	5/2014	Libbus et al.		2007/0089800	A1	4/2007	Sharma
8,744,561	B2	6/2014	Fahey		2007/0093719	A1	4/2007	Nichols, Jr. et al.
8,774,932	B2	7/2014	Fahey		2007/0100248	A1	5/2007	Van Dam et al.
8,790,257	B2	7/2014	Libbus et al.		2007/0100667	A1	5/2007	Bardy
8,790,259	B2	7/2014	Katra et al.		2007/0123801	A1	5/2007	Goldberger et al.
8,795,174	B2	8/2014	Manicka et al.		2007/0131595	A1	6/2007	Jansson et al.
8,798,729	B2	8/2014	Kaib et al.		2007/0136091	A1	6/2007	McTaggart
8,798,734	B2	8/2014	Kuppuraj et al.		2007/0179357	A1	8/2007	Bardy
8,818,478	B2	8/2014	Scheffler et al.		2007/0185390	A1	8/2007	Perkins et al.
8,818,481	B2	8/2014	Bly et al.		2007/0203415	A1	8/2007	Bardy
8,823,490	B2	9/2014	Libbus et al.		2007/0203423	A1	8/2007	Bardy
8,938,287	B2	1/2015	Felix et al.		2007/0208232	A1	9/2007	Kovacs
8,965,492	B2	2/2015	Baker et al.		2007/0208233	A1	9/2007	Kovacs
9,066,664	B2	6/2015	Karjalainen		2007/0208266	A1	9/2007	Hadley
9,155,484	B2	10/2015	Baker et al.		2007/0225611	A1	9/2007	Kumar et al.
9,204,813	B2	12/2015	Kaib et al.		2007/0244405	A1	10/2007	Xue et al.
9,277,864	B2	3/2016	Yang et al.		2007/0249946	A1	10/2007	Kumar et al.
9,339,202	B2	5/2016	Brockway et al.		2007/0255153	A1	11/2007	Kumar et al.
9,439,566	B2	9/2016	Arne et al.		2007/0265510	A1	11/2007	Bardy
2002/0013538	A1	1/2002	Teller		2007/0276270	A1	11/2007	Tran
2002/0013717	A1 *	1/2002	Ando	A61B 5/0002	2007/0276275	A1	11/2007	Proctor et al.
				705/4	2007/0293738	A1	12/2007	Bardy
					2007/0293739	A1	12/2007	Bardy
2002/0103422	A1	8/2002	Harder et al.		2007/0293740	A1	12/2007	Bardy
2002/0109621	A1	8/2002	Khair et al.		2007/0293741	A1	12/2007	Bardy
2002/0120310	A1	8/2002	Linden et al.		2007/0293772	A1	12/2007	Bardy
2002/0128686	A1	9/2002	Minogue et al.		2007/0299325	A1	12/2007	Farrell et al.
2002/0184055	A1 *	12/2002	Naghavi	G06F 19/3406	2007/0299617	A1	12/2007	Willis
				705/2	2008/0027339	A1	1/2008	Nagai et al.
					2008/0051668	A1	2/2008	Bardy
2002/0193668	A1	12/2002	Munneke		2008/0058661	A1	3/2008	Bardy
					2008/0091097	A1	4/2008	Linti et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0108890	A1	5/2008	Teng et al.	
2008/0114232	A1	5/2008	Gazit	
2008/0139953	A1*	6/2008	Baker	A61B 5/0006 600/509
2008/0143080	A1	6/2008	Burr	
2008/0177168	A1	7/2008	Callahan et al.	
2008/0194927	A1	8/2008	KenKnight et al.	
2008/0208009	A1*	8/2008	Shklarski	A61B 5/0022 600/301
2008/0208014	A1	8/2008	KenKnight et al.	
2008/0284599	A1	11/2008	Zdeblick et al.	
2008/0288026	A1	11/2008	Cross et al.	
2008/0294024	A1	11/2008	Cosentino et al.	
2008/0306359	A1	12/2008	Zdeblick et al.	
2008/0312522	A1	12/2008	Rowlandson	
2009/0012979	A1	1/2009	Bateni et al.	
2009/0054952	A1	2/2009	Glukhovskiy et al.	
2009/0062897	A1	3/2009	Axelgaard	
2009/0069867	A1	3/2009	KenKnight et al.	
2009/0073991	A1	3/2009	Landrum et al.	
2009/0076336	A1	3/2009	Mazar et al.	
2009/0076341	A1	3/2009	James et al.	
2009/0076342	A1	3/2009	Amurthur et al.	
2009/0076343	A1	3/2009	James et al.	
2009/0076346	A1	3/2009	James et al.	
2009/0076349	A1	3/2009	Libbus et al.	
2009/0076397	A1	3/2009	Libbus et al.	
2009/0076401	A1	3/2009	Mazar et al.	
2009/0076559	A1	3/2009	Libbus et al.	
2009/0088652	A1	4/2009	Tremblay	
2009/0112116	A1	4/2009	Lee et al.	
2009/0131759	A1	5/2009	Sims et al.	
2009/0156908	A1	6/2009	Belalcazar et al.	
2009/0216132	A1	8/2009	Orbach	
2009/0270708	A1	10/2009	Shen et al.	
2009/0270747	A1	10/2009	Van Dam et al.	
2009/0292194	A1	11/2009	Libbus et al.	
2010/0007413	A1	1/2010	Herleikson	
2010/0022897	A1	1/2010	Parker et al.	
2010/0056881	A1	3/2010	Libbus et al.	
2010/0081913	A1	4/2010	Cross et al.	
2010/0174229	A1	7/2010	Hsu et al.	
2010/0177100	A1	7/2010	Carnes et al.	
2010/0185063	A1	7/2010	Bardy	
2010/0185076	A1	7/2010	Jeong et al.	
2010/0191154	A1	7/2010	Berger et al.	
2010/0191310	A1	7/2010	Bly	
2010/0223020	A1	9/2010	Goetz	
2010/0234715	A1	9/2010	Shin et al.	
2010/0234716	A1	9/2010	Engel	
2010/0280366	A1	11/2010	Arne et al.	
2010/0312188	A1	12/2010	Robertson et al.	
2010/0324384	A1	12/2010	Moon et al.	
2011/0021937	A1	1/2011	Hugh et al.	
2011/0054286	A1	3/2011	Crosby et al.	
2011/0060215	A1	3/2011	Tupin et al.	
2011/0066041	A1	3/2011	Pandia et al.	
2011/0077497	A1*	3/2011	Oster	A61B 5/0002 600/372
2011/0105861	A1	5/2011	Derchak et al.	
2011/0144470	A1	6/2011	Mazar et al.	
2011/0160548	A1	6/2011	Forster et al.	
2011/0224564	A1	9/2011	Moon et al.	
2011/0237922	A1	9/2011	Parker, III et al.	
2011/0237924	A1	9/2011	McGusty et al.	
2011/0245699	A1	10/2011	Snell et al.	
2011/0245711	A1	10/2011	Katra et al.	
2011/0288605	A1	11/2011	Kaib et al.	
2012/0003933	A1*	1/2012	Baker	A61B 5/0002 455/41.2
2012/0029306	A1	2/2012	Paquet et al.	
2012/0029315	A1	2/2012	Raptis et al.	
2012/0029316	A1	2/2012	Raptis et al.	
2012/0035432	A1	2/2012	Katra et al.	
2012/0078127	A1	3/2012	McDonald et al.	

2012/0088998	A1	4/2012	Bardy et al.	
2012/0088999	A1	4/2012	Bishay et al.	
2012/0089000	A1	4/2012	Bishay et al.	
2012/0089001	A1	4/2012	Bishay et al.	
2012/0089037	A1*	4/2012	Bishay	A61B 5/0404 600/509
2012/0089412	A1	4/2012	Bardy et al.	
2012/0089417	A1	4/2012	Bardy et al.	
2012/0095352	A1	4/2012	Tran	
2012/0101358	A1	4/2012	Boettcher et al.	
2012/0101396	A1*	4/2012	Solosko	A61B 5/0006 600/509
2012/0165645	A1	6/2012	Russell et al.	
2012/0306662	A1	6/2012	Vosch et al.	
2012/0172695	A1	7/2012	Ko et al.	
2012/0238910	A1	9/2012	Nordstrom	
2012/0253847	A1	10/2012	Dell'Anno et al.	
2012/0302906	A1	11/2012	Felix et al.	
2012/0323132	A1	12/2012	Warner et al.	
2012/0330126	A1	12/2012	Hoppe et al.	
2013/0041272	A1	2/2013	Guillen Arredondo et al.	
2013/0077263	A1	3/2013	Oleson et al.	
2013/0079611	A1	3/2013	Besko	
2013/0085347	A1	4/2013	Manicka et al.	
2013/0085403	A1	4/2013	Gunderson et al.	
2013/0096395	A1	4/2013	Katra et al.	
2013/0116533	A1	5/2013	Lian et al.	
2013/0123651	A1	5/2013	Bardy	
2013/0158361	A1	6/2013	Bardy	
2013/0197380	A1	8/2013	Oral et al.	
2013/0225963	A1	8/2013	Kodandaramaiah et al.	
2013/0225966	A1	8/2013	Macia Barber et al.	
2013/0243105	A1	9/2013	Lei et al.	
2013/0274584	A1	10/2013	Finlay et al.	
2013/0275158	A1	10/2013	Fahey	
2013/0324809	A1	12/2013	Lisogurski et al.	
2013/0324855	A1	12/2013	Lisogurski et al.	
2013/0324856	A1	12/2013	Lisogurski et al.	
2013/0325359	A1	12/2013	Jarverud et al.	
2013/0331665	A1	12/2013	Libbus et al.	
2013/0338448	A1	12/2013	Libbus et al.	
2013/0338472	A1	12/2013	Macia Barber et al.	
2014/0012154	A1	1/2014	Mazar et al.	
2014/0056452	A1	2/2014	Moss et al.	
2014/0140359	A1	5/2014	Kalevo et al.	
2014/0180027	A1	6/2014	Buller	
2014/0189928	A1	7/2014	Oleson et al.	
2014/0206977	A1	7/2014	Bahney et al.	
2014/0215246	A1	7/2014	Lee et al.	
2014/0249852	A1	9/2014	Proud	
2014/0296651	A1	10/2014	Stone	
2014/0358193	A1	12/2014	Lyons et al.	
2014/0364756	A1	12/2014	Brockway et al.	
2015/0048836	A1	2/2015	Guthrie et al.	
2015/0065842	A1	3/2015	Lee et al.	
2015/0165211	A1	6/2015	Navqi et al.	
2015/0177175	A1	6/2015	Elder et al.	
2015/0250422	A1	9/2015	Bay	
2015/0257670	A1	9/2015	Ortega et al.	
2015/0305676	A1	11/2015	Shoshani	
2015/0359489	A1	12/2015	Baudenbacher et al.	
2016/0217691	A1*	7/2016	Kadobayashi	G06Q 50/22

FOREIGN PATENT DOCUMENTS

EP	2438851	4/2012
EP	2438852	4/2012
EP	2465415	6/2012
EP	2589333	5/2013
JP	H06319711	11/1994
JP	H11188015	7/1999
JP	2004129788	4/2004
JP	2007082938	4/2007
JP	2009219554	10/2009
WO	0078213	12/2000
WO	2003032192	4/2003
WO	2006009767	1/2006
WO	2006014806	2/2006
WO	2007066270	6/2007

(56) References Cited

FOREIGN PATENT DOCUMENTS

WO	2007092543	8/2007
WO	2008010216	1/2008
WO	2008057884	5/2008
WO	2009036306	3/2009
WO	2009036313	3/2009
WO	2009036327	3/2009
WO	2009112976	9/2009
WO	2009112978	9/2009
WO	2009112979	9/2009
WO	2009142975	11/2009
WO	2010066507	6/2010
WO	2010105045	9/2010
WO	2011047207	4/2011
WO	2012140559	10/2012
WO	2012146957	11/2012

OTHER PUBLICATIONS

Saadi et al. "Heart Rhythm Analysis Using ECG Recorded With a Novel Sternum Based Patch Technology—A Pilot Study." Cardio technix 2013—Proceedings of the International Congress on Cardiovascular Technologies, Sep. 20, 2013.

Anonymous. Omegawave Launches Consumer App 2.0 in U.S. "Endurance Sportswire—Endurance Sportswire." Jul. 11, 2013. URL: <http://endurancesportswire.com/omegawave-launches-consumer-app-2-0-in-u-s/>.

Chan et al. "Wireless Patch Sensor for Remote Monitoring of Heart Rate, Respiration, Activity, and Falls." pp. 6115-6118. 2013 35th Annual International Conference of the IEEE Engineering in Medical and Biology Society. Jul. 1, 2013.

Daoud et al. "Fall Detection Using Shimmer Technology and Multiresolution Analysis." Aug. 2, 2013. URL: <https://decibel.ni.com/content/docs/DOC-26652>.

Libbus. "Adherent Cardiac Monitor With Wireless Fall Detection for Patients With Unexplained Syncope." Abstracts of the First AMA-IEEE Medical Technology Conference on Individualized Healthcare. May 22, 2010.

15 of the Hottest Wearable Gadgets, URL <<http://thehottestgadgets.com/2008/09/the-15-hottest-wearable-gadgets-001253>> (Web page cached on Sep. 27, 2008).

Alivecor's Heart Monitor for iPhone Receives FDA Clearance, URL <<http://www.businesswire.com/news/home/20121203005545/en/AliveCor%E2%80%99s-Heart-Monitor-iPhone-Receives-FDA-Clearance#.U7rtq7FVtyF>> (Dec. 3, 2012).

Bharadwaj et al., Techniques for Accurate ECG signal processing, EE Times, URL <www.eetimes.com/document.asp?doc_id=1278571> (Feb. 14, 2011).

Chen et al., "Monitoring Body Temperature of Newborn Infants at Neonatal Intensive Care Units Using Wearable Sensors," BodyNets 2010, Corfu Island, Greece. (Sep. 10, 2010).

Epstein, Andrew E. et al.; ACC/AHA/HRS 2008 Guidelines for Device-Based Therapy of Cardiac Rhythm Abnormalities. J. Am. Coll. Cardiol. 2008; 51; e1-e62, 66 Pgs.

Fitbit automatically tracks your fitness and sleep, URL <<http://www.fitbit.com/>> (Web page cached on Sep. 10, 2008).

Smith, Kevin, "Jawbone Up VS. Fitbit Flex: Which Is the Best Fitness Band?" URL <<http://www.businessinsider.com/fitbit-flex-vs-jawbone-up-2013-5?op=1>> (Jun. 1, 2013).

Kligfield, Paul et al., Recommendations for the Standardization and Interpretation of the Electrocardiogram: Part I. J. Am. Coll. Cardiol. 2007; 49; 1109-27, 75 Pgs.

Lauren Gravit, "When Your Diet Needs a Band-Aid," Technology Review, MIT. (May 1, 2009).

Lieberman, Jonathan, "How Telemedicine Is Aiding Prompt ECG Diagnosis in Primary Care," British Journal of Community Nursing, vol. 13, No. 3, Mar. 1, 2008 (Mar. 1, 2008), pp. 123-126, XP009155082, ISSN: 1462-4753.

McManus et al., "A Novel Application for the Detection of an Irregular Pulse using an iPhone 4S in Patients with Atrial Fibrillation," vol. 10(3), pp. 315-319 (Mar. 2013).

Nike+ Fuel Band, URL <http://www.nike.com/us/en_us/c/nikeplus-fuelband> (Web page cached on Jan. 11, 2013).

P. Libby et al., "Braunwald's Heart Disease—A Textbook of Cardiovascular Medicine," Chs. 11, pp. 125-148 and 12, pp. 149-193 (8th ed. 2008), American Heart Association.

Initial hands-on with Polar Loop activity tracker, URL <<http://www.drainmaker.com/2013/09/polar-loop-firstlook.html>> (Sep. 17, 2013).

Sittig et al., "A Computer-Based Outpatient Clinical Referral System," International Journal of Medical Informatics, Shannon, IR, vol. 55, No. 2, Aug. 1, 1999, pp. 149-158, X0004262434, ISSN: 1386-5056(99)00027-1.

Sleepview, URL <<http://www.clevemed.com/sleepview/overview.shtml>> (Web pages cached on Feb. 23, 2010, Dec. 29, 2012 and Sep. 4, 2013).

Actigraphy/ Circadian Rhythm SOMNObatch, URL <<http://www.somnomedics.eu/news-events/publications/somnowatchtm.html>> (Web page cached on Jan. 23, 2010).

Zio Event Card, URL <<http://www.irhythmtech.com/zio-solution/zio-event/>> (Web page cached on Mar. 11, 2013).

Zio Patch System, URL <<http://www.irhythmtech.com/zio-solution/zio-system/index.html>> (Web page cached on Sep. 8, 2013).

Seifert, Dan, "Samsung dives into fitness wearable with the Gear Fit/ The Verge," URL <<http://www.theverge.com/2014/2/24/5440310/samsung-dives-into-fitness-wearables-with-the-gear-fit>> (Feb. 24, 2014).

Soper, Taylor, "Samsung's new Galaxy S5 flagship phone has fingerprint reader, heart rate monitor," URL <<http://www.geekwire.com/2014/samsung-galaxy-s5-fingerprint/>> (Feb. 24, 2014).

Dolcourt, Jessica, "See the Samsung Galaxy S5's Heart rate monitor in action," URL <<http://www.cnet.com/news/see-the-samsung-galaxy-s5s-heart-rate-monitor-in-action/>> (Feb. 25, 2014).

A Voss et al., "Linear and Nonlinear Methods for Analyses of Cardiovascular Variability in Bipolar Disorders," Bipolar Disorders, vol. 8, No. 5p1, Oct. 1, 2006, pp. 441-452, XP55273826, DK ISSN: 1398-5647, DOI: 10.1111/i.1399-5618.2006.00364.x.

"VARICRAD-KARDI Software User's Manual Rev. 1.1", Jul. 8, 2009 (Jul. 8, 2009), XP002757888, retrieved from the Internet: URL: <http://www.ehrlich.tv/KARDIVAR-Software.pdf> [retrieved on May 20, 2016].

"Vedapulse UK," Jan. 1, 2014 (Jan. 1, 2014), XP002757887, Retrieved from the Internet: URL: <http://www.vedapulseuk.com/diagnostic/> [retrieved on May 19, 2016].

Duttweiler et al., "Probability Estimation in Arithmetic and Adaptive-Huffman Entropy Coders," IEEE Transactions on Image Processing, vol. 4, No. 3, Mar. 1, 1995, pp. 237-246.

Gupta et al., "An ECG Compression Technique for Telecardiology Application," India Conference (INDICON), 2011 Annual IEEE, Dec. 16, 2011, pp. 1-4.

Nave et al., "ECG Compression Using Long-Term Prediction," IEEE Transactions on Biomedical Engineering, IEEE Service Center, NY, USA, vol. 40, No. 9, Sep. 1, 1993, pp. 877-885.

Skretting et al., "Improved Huffman Coding Using Recursive Splitting," NORSIG, Jan. 1, 1999.

<https://web.archive.org/web/20130831204020/http://www.biopac.com/research.asp?CatID=37&Main=Software> (Aug. 2013).

<http://www.gtcc.at/Products/Software/g.BSAnalyze-Specs-Features> (2014).

ADINSTRUMENTS: ECG Analysis Module for LabChart & PowerLab, 2008.

BIOPAC Systems, Inc. #AS148-Automated ECG Analysis, Mar. 24, 2006.

* cited by examiner

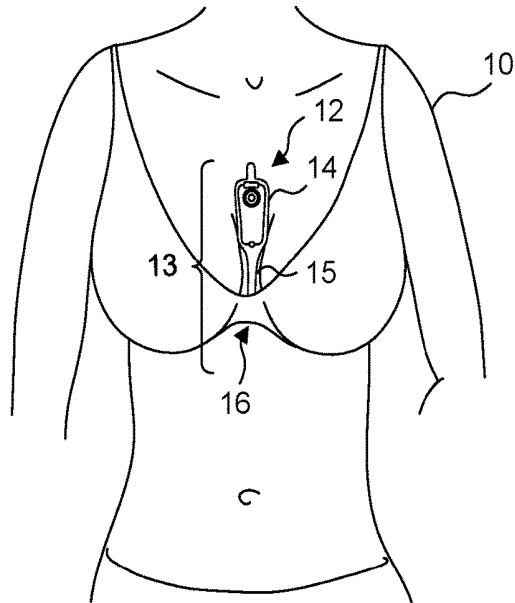
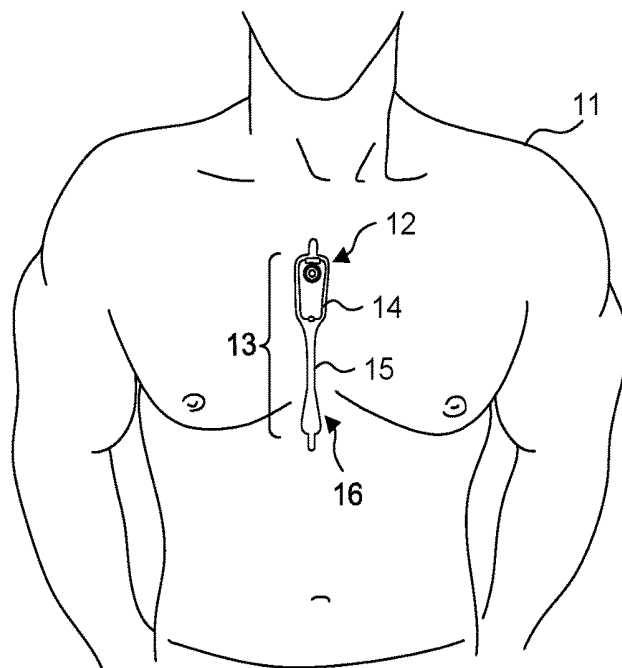
Fig. 1.**Fig. 2.**

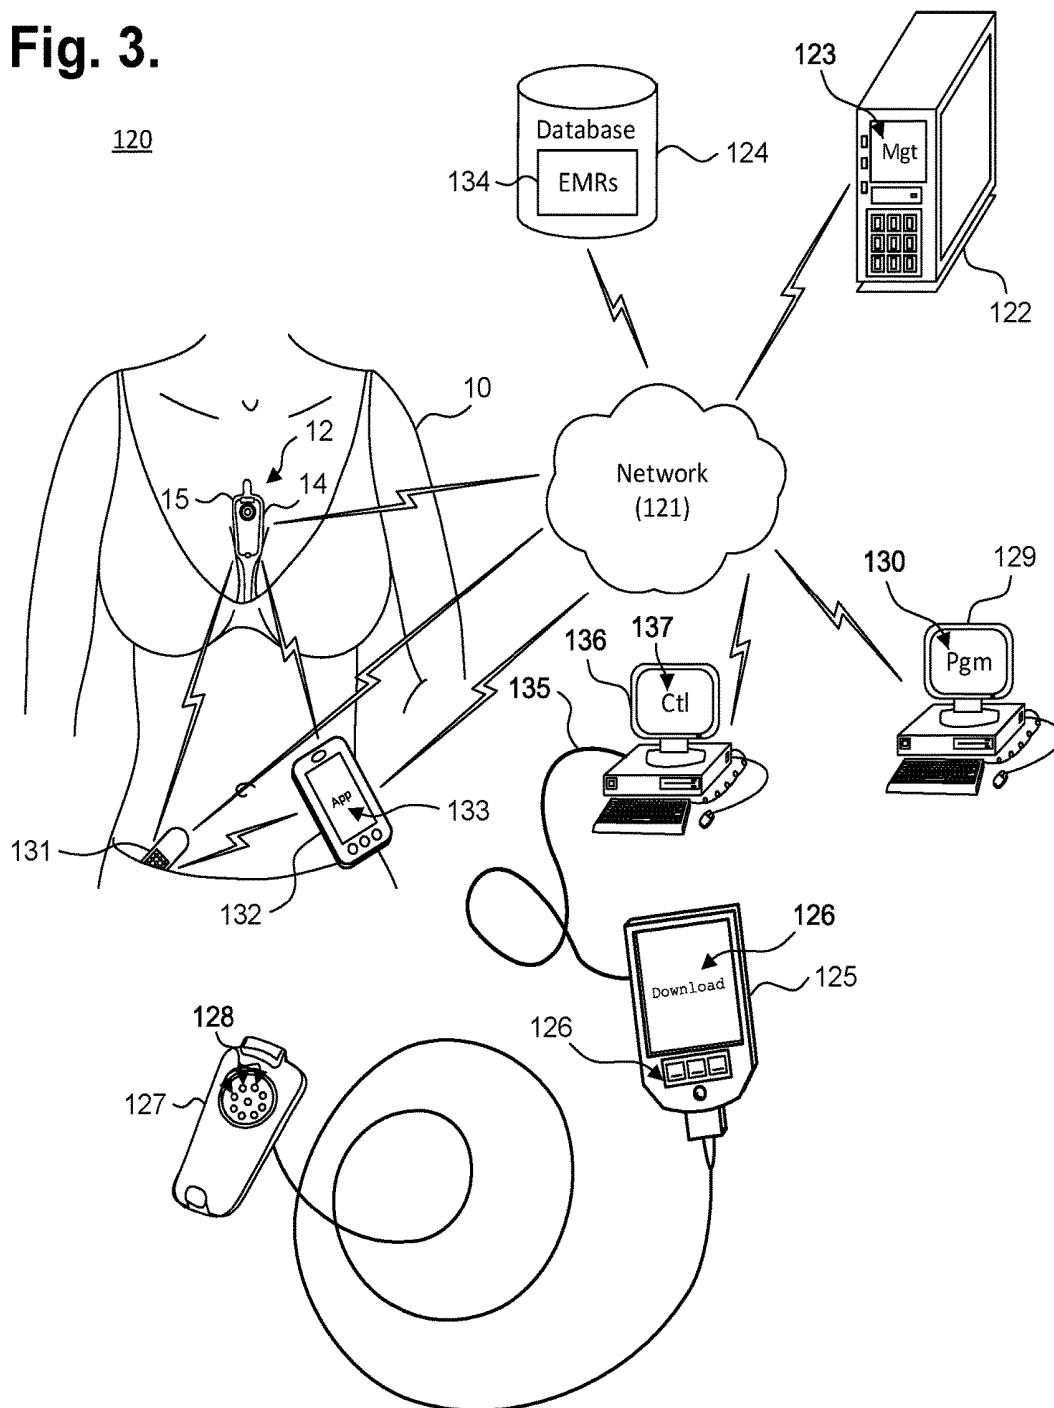
Fig. 3.

Fig. 4.

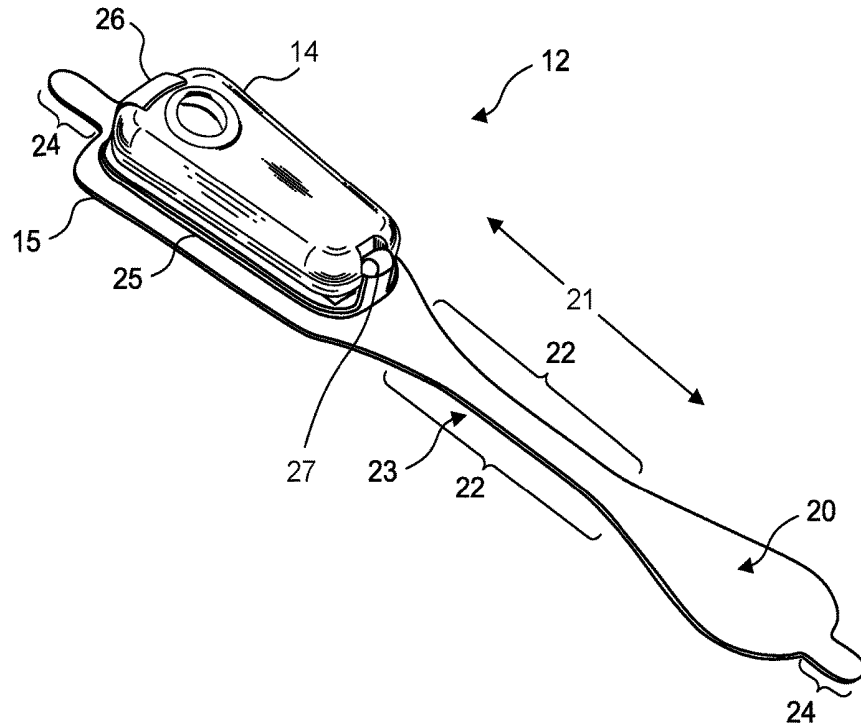


Fig. 5.

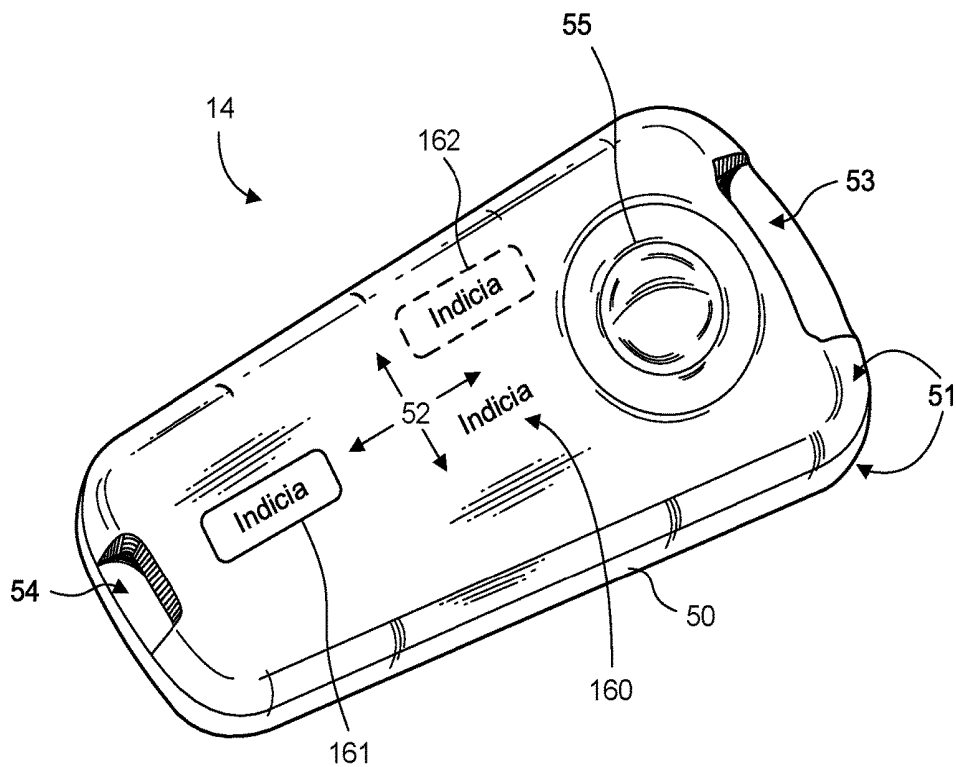


Fig. 6.

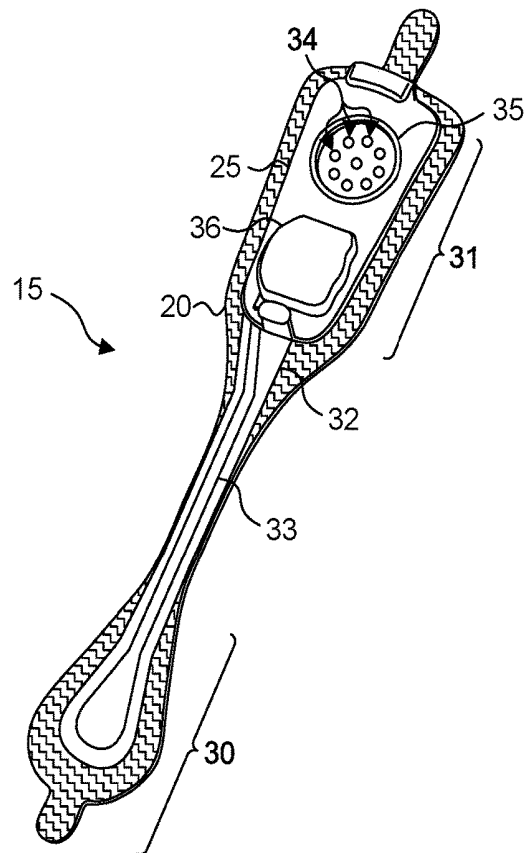


Fig. 7.

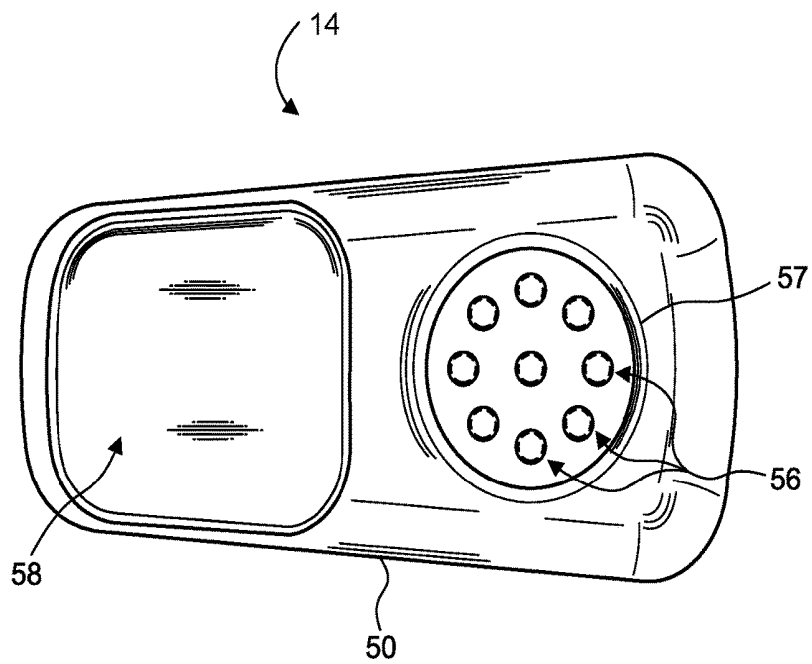


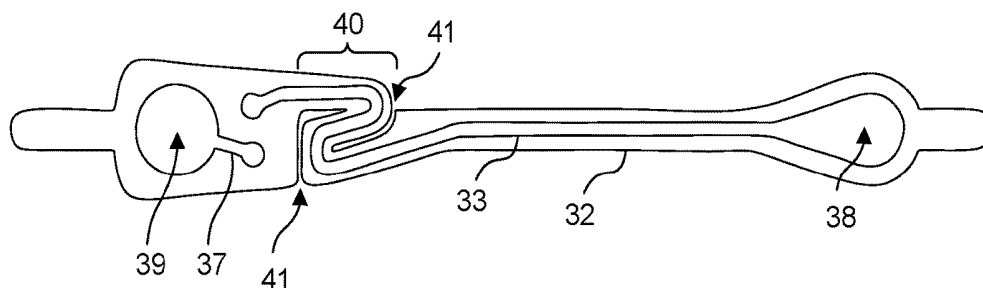
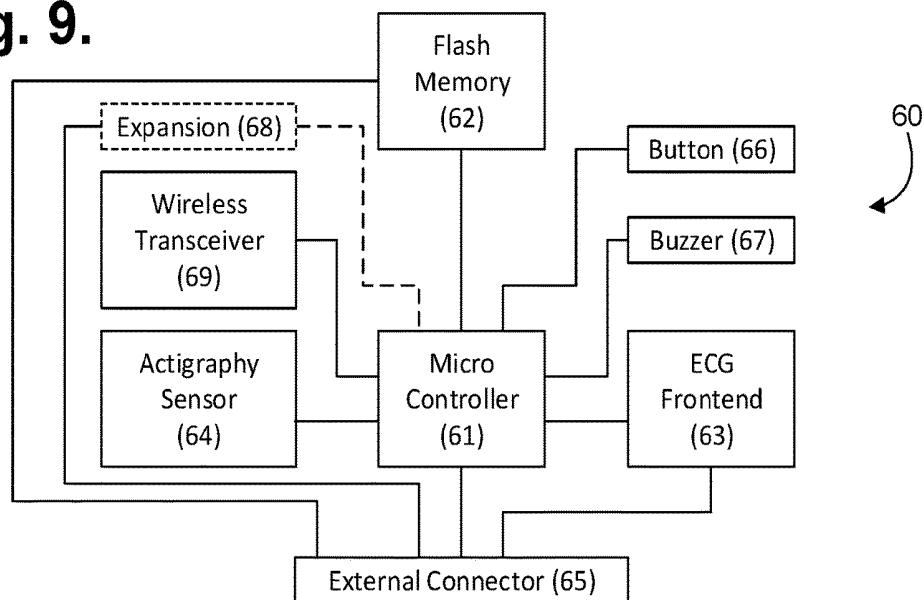
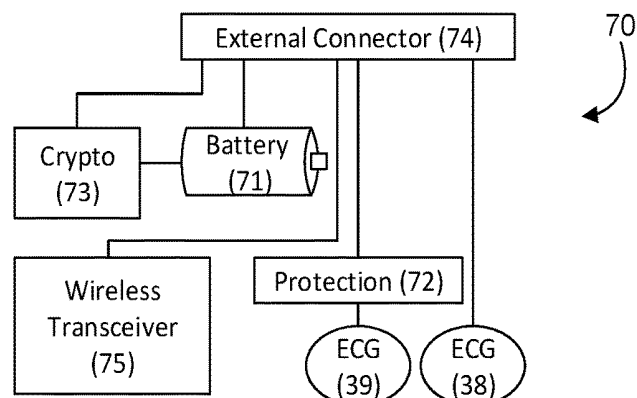
Fig. 8.**Fig. 9.****Fig. 10.**

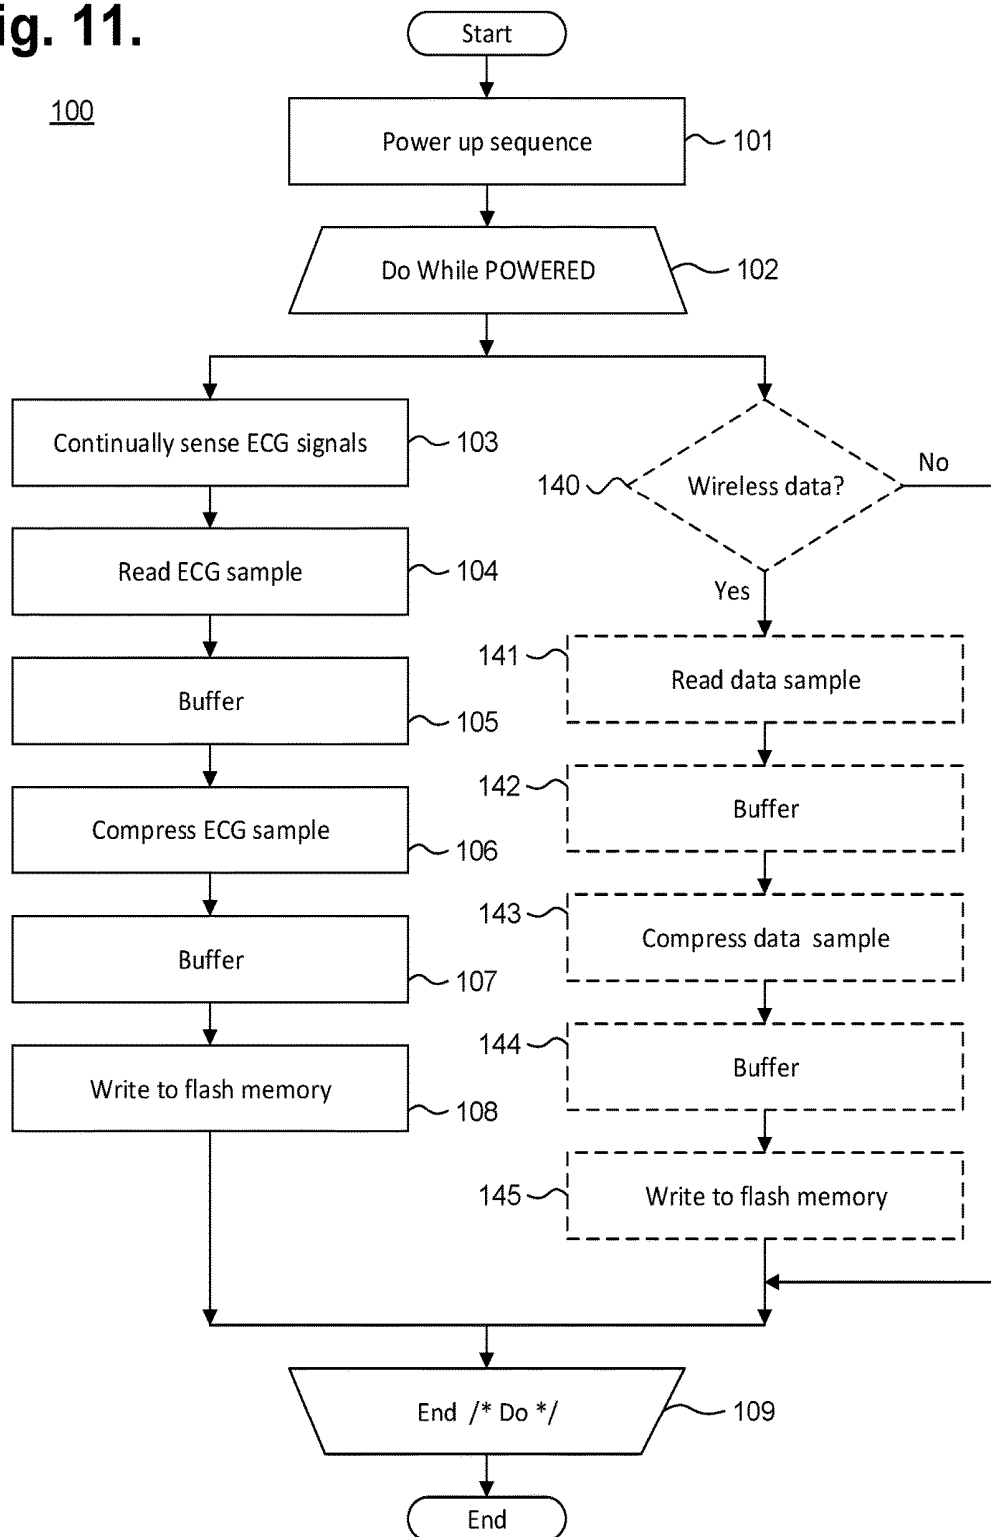
Fig. 11.

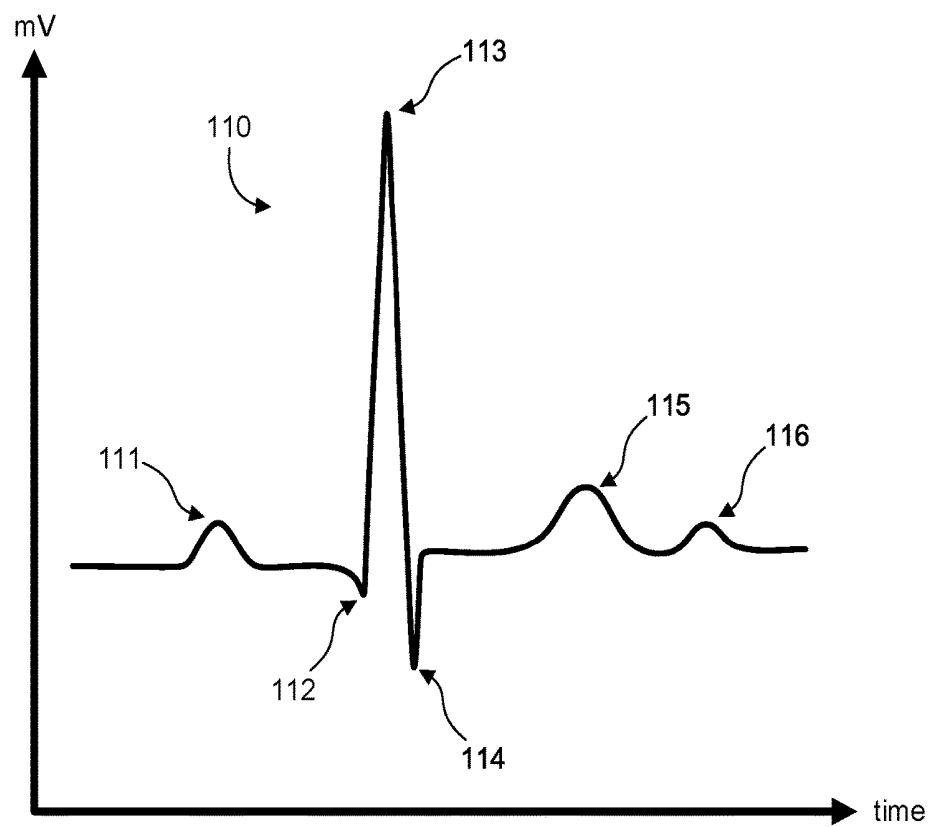
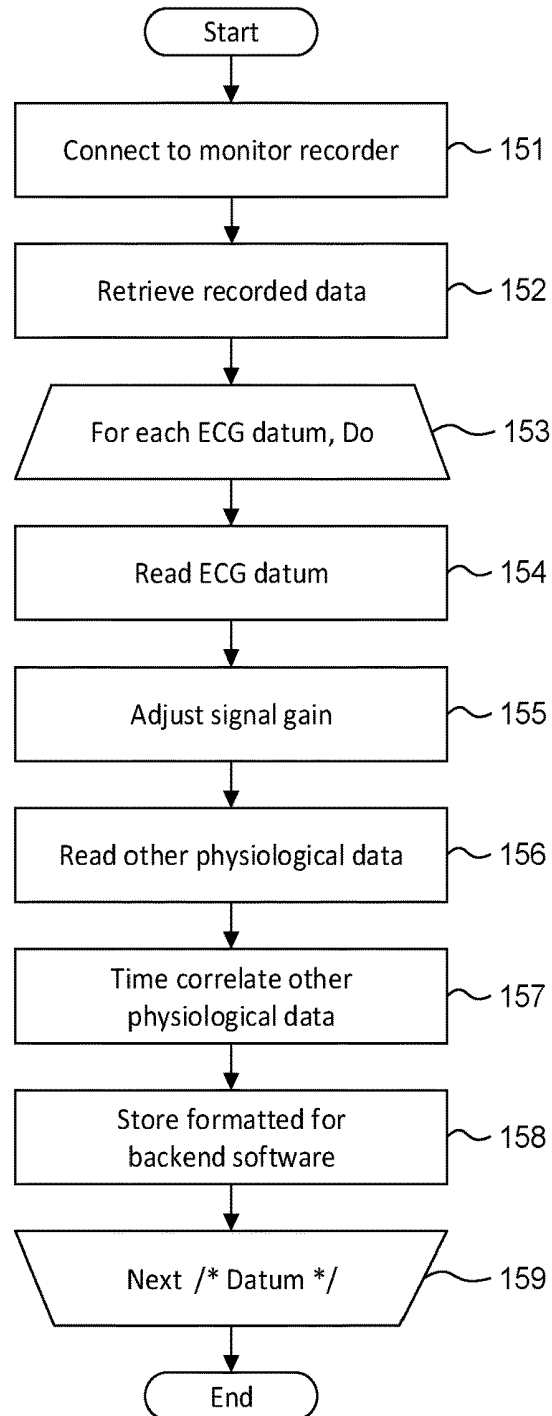
Fig. 12.

Fig. 13.150

COMPUTER-IMPLEMENTED SYSTEM AND METHOD FOR PROVIDING A PERSONAL MOBILE DEVICE-TRIGGERED MEDICAL INTERVENTION

CROSS-REFERENCE TO RELATED APPLICATION

This non-provisional patent application is a continuation-in-part of U.S. Pat. No. 9,433,367, issued Sep. 6, 2016; which is a continuation-in-part of U.S. Pat. No. 9,545,204, issued Jan. 17, 2017, and a continuation-in-part of U.S. Pat. No. 9,730,593, issued Aug. 15, 2017; and which further claims priority under 35 U.S.C. § 119(e) to U.S. Provisional Patent application, Ser. No. 61/882,403, filed Sep. 25, 2013, the disclosures of which are incorporated by reference.

FIELD

This application relates in general to electrocardiographic monitoring and, in particular, to a computer-implemented system and method for providing a personal mobile device-triggered medical intervention.

BACKGROUND

An electrocardiogram (ECG) records electrical potentials in the heart using a standardized set format 12-lead configuration to record cardiac electrical signals from well-established chest locations. Electrodes are placed on the skin over the anterior thoracic region of the body to the lower right and to the lower left of the sternum, on the left anterior chest, and on the limbs. The recorded cardiac electrical activity, represented by PQRSTU waveforms, can be interpreted to derive heart rate and physiology, where each P-wave represents atrial electrical activity and the QRSTU components represent ventricular electrical activity.

An ECG is a snapshot of heart function, typically recorded over 12 seconds, that can help diagnose rate and regularity of heartbeats, effect of drugs or implantable cardiac devices, and whether a patient has heart disease. ECGs are limited to recording those heart-related aspects present at the time of recording. Thus, an ECG only provides a partial picture and can be insufficient for complete patient diagnosis of many cardiac disorders. Sporadic conditions that may not show up during a spot ECG recording, including fainting or syncope; rhythm disorders, such as tachyarrhythmias and bradyarrhythmias; asystolic episodes; and other cardiac and related disorders, require other means of diagnosis.

Diagnostic efficacy of cardiac rhythm disorders in particular can be improved, when appropriate, through long-term extended ECG monitoring. Recording cardiac physiology over an extended period can be challenging, yet is often essential to enabling a physician to identify events of potential concern. Although a 30-day observation period is considered the “gold standard” of ECG monitoring, achieving 30-day coverage has proven unworkable because conventional ambulatory ECG monitoring systems are arduous to employ, cumbersome to wear, and excessively costly. Nevertheless, if a patient’s ECG could be recorded in an ambulatory setting over long periods of time, thereby allowing the patient to engage in activities of daily living, the chances of acquiring meaningful information and capturing an abnormal cardiac rhythm event becomes more likely to be achieved.

For instance, the long-term wear of ECG electrodes is complicated by skin irritation and the inability of conventional ECG electrodes to maintain continual skin contact after a day or two. Moreover, time, dirt, moisture, and other environmental contaminants, as well as perspiration, skin oil, and dead skin cells from the patient’s body, can get between an ECG electrode, the non-conductive adhesive used to adhere the ECG electrode, and the skin’s surface. These factors adversely affect electrode adhesion and the quality of cardiac signal recordings. Moreover, physical movement and clothing impart compressional, tensile, and torsional forces on electrode contact points decreasing signal quality, especially over long recording times. In addition, an inflexibly fastened ECG electrode is prone to dislodgement that often occurs unbeknownst to the patient, making the ECG recordings worthless. Further, some patients may have skin conditions, such as itching and irritation, aggravated by the wearing of most ECG electrodes. A patient may have to periodically remove or replace electrodes during a long-term monitoring period, whether to replace a dislodged electrode, reestablish better adhesion, alleviate itching or irritation, allow for cleansing of the skin, allow for showering and exercise, or for other purpose. Such replacement or slight alteration in electrode location can interfere with the goal of recording the ECG signal for long periods of time. Finally, such recording devices are often ineffective at recording atrial electrical activity, which is critical in the accurate diagnosis of heart rhythm disorders, because of the use of traditional ECG recording electronics or due to the location of the monitoring electrodes far from the origin of the atrial signal, for instance, the P-wave.

Conventionally, Holter monitors are widely used for long-term extended ECG monitoring, typically, for only 24-48 hours. A typical Holter monitor is a wearable and portable version of an ECG that includes cables for each electrode placed on the skin and a separate battery-powered ECG recorder. Similar to standard in-clinic ECG practice, the cable and electrode combination (or leads) are placed in the anterior thoracic region. The duration of a Holter monitoring recording depends on the sensing and storage capabilities of the monitor, as well as battery life. A “looping” Holter (or event) monitor can operate for a longer period of time by overwriting older ECG tracings, thence “recycling” storage in favor of extended operation, yet at the risk of losing crucial event data. Holter monitors remain cumbersome, expensive and typically for prescriptive use only, which limits their usability. Further, the skill required to properly place the ECG leads on the patient’s chest hinders or precludes a patient from replacing or removing the electrodes.

The ZIO XT Patch and ZIO Event Card devices, manufactured by iRhythm Tech., Inc., San Francisco, Calif., are wearable stick-on monitoring devices that are typically worn on the upper left pectoral region to respectively provide continuous and looping ECG recordings. The location is used to simulate surgically implanted monitors. These devices are prescription-only for single patient use. The ZIO XT Patch device is limited to 14-day monitoring, while the ZIO Event Card device’s electrodes can be worn for up to 30 days. The ZIO XT Patch device combines electronic recording components, including battery, and physical electrodes into a unitary assembly that adheres to the skin. The ZIO XT Patch device uses adhesive strong enough to support the weight of both the monitor and the electrodes over an extended period of time. During monitoring, the battery is continually depleted and can potentially limit overall monitoring duration. The ZIO Event Card device is

a form of downsized Holter monitor with a recorder component that must be removed during activities that could damage the non-waterproof electronics. These patches have a further limitation because of a small inter-electrode distance coupled to its designed location of application, high on the left chest. The electrical design of the ZIO patch and its location make recording high quality atrial signals (P-waves) difficult, as the location is relatively far from the origin of these low amplitude signals. As well, the location is suboptimal for identification of these signals. Furthermore, this patch is problematical for woman by being placed in a location that may limit signal quality, especially in woman with large breasts or bosoms. Both ZIO devices represent compromises between length of wear and quality of ECG monitoring, especially with respect to ease of long term use, female-friendly fit, and quality of atrial (P-wave) signals.

Personal ambulatory monitoring, both with smartphones or via adjuncts to smartphones, such as with a wirelessly-connected monitor or activity tracker, of varying degrees of sophistication and interoperability, have become increasingly available. For instance, McManus et al., "A Novel Application for the Detection of an Irregular Pulse using an iPhone 4S in Patients with Atrial Fibrillation," Vol. 10(3), pp. 315-319 (March 2013), the disclosure of which is incorporated by reference, discloses obtaining pulsatile time series recordings before and after cardioversion using the digital camera built into a smartphone. An algorithm implemented as an app executed by the smartphone analyzed recorded signals to accurately distinguish pulse recordings during atrial fibrillation from sinus rhythm, although such a smartphone-based approach provides non-continuous observation and would be impracticable for long term physiological monitoring. Further, the smartphone-implemented app does not provide continuous recordings, including the provision of pre-event and post-event context, critical for an accurate medical diagnosis that might trigger a meaningful and serious medical intervention. In addition, a physician would be loath to undertake a surgical or serious drug intervention without confirmatory evidence that the wearer in question was indeed the subject of the presumed rhythm abnormality. Validation of authenticity of the rhythm disorder for a specified patient takes on critical legal and medical importance.

The AliveCor heart monitor, manufactured by AliveCor, Inc., San Francisco, Calif., provides a non-continuous, patient-triggered event monitor, which is worn on the fingertip. Heart rate is sensed over a single lead (comparable to Lead I on a conventional ECG) and recorded by an app running on a smartphone, such as an iOS operating system-based smartphone, such as the iPhone, manufactured by Apple Inc., Cupertino, Calif., or an Android operating system-based smartphone, manufactured and offered by various companies, including Google Inc., Mountain View, Calif.; Samsung Electronics Co., Ltd., Suwon, S. Korea; Motorola Mobility LLC, a subsidiary of Google Inc., Libertyville, Ill.; and LG Electronics Inc., Seoul, S. Korea. The Android operating system is also licensed by Google Inc. The app can send the data recorded by an AliveCor heart monitor from the smartphone to healthcare providers, who ultimately decide whether to use the data for screening or diagnostic purposes. Furthermore, as explained supra with respect to the McManus reference, none of these devices provides the context of the arrhythmia, as well as the medico-legal confirmation that would otherwise allow for a genuine medical intervention.

Similarly, adherents to the so-called "Quantified Self" movement combine wearable sensors and wearable computing to self-track activities of their daily lives. The Fitbit Tracker, manufactured by Fitbit Inc., San Francisco, Calif.; the Jawbone UP, manufactured by Jawbone, San Francisco, Calif.; the Polar Loop, manufactured by Polar Electro, Kempele, Finland; and the Nike+ FuelBand, manufactured by Nike Inc., Beaverton, Oreg., for instance, provide activity trackers worn on the wrist or body with integrated fitness tracking features, such as a heart rate monitor and pedometer to temporally track the number of steps taken each day with an estimation calories burned. The activity tracker can interface with a smartphone or computer to allow a wearer to monitor their progress towards a fitness goal. These activity trackers are accessories to smartphones, including iOS operating system-based smartphones, Android operating system-based smartphones, and Windows Phone operating-system based smartphones, such as manufactured by Microsoft Corporation, Redmond, WA, to which recorded data must be offloaded for storage and viewing.

The features of activity trackers can also be increasingly found in so-called "smart" watches that combine many of the features of activity trackers with smartphones. Entire product lines are beginning to be offered to provide a range of fitness- and health-tracking solutions. As one example, Samsung Electronics Co., Ltd., offers a line of mobile products with fitness-oriented features, including the Galaxy S5 smartphone, which incorporates a biometric fingerprint reader and heart rate monitor; the Gear 2 smart watch, which also incorporates a heart rate monitor; and the Gear Fit wearable device, which incorporates a heart rate monitor, real time fitness coaching, and activity tracker. The Galaxy S5 smartphone's heart rate monitor is not meant for continuous tracking, while the both the Gear 2 smart watch and Gear Fit wearable device must be paired with a smartphone or computer to offload and view the recorded data.

With all manner of conventional "fitness-oriented" device, whether smartphone, smart watch, or activity tracker, quantified physiology is typically tracked for only the personal use of the wearer. Monitoring can be either continuous or non-continuous. The wearer must take extra steps to route recorded data to a health care provider; thus, with rare exception, the data is not time-correlated to physician-supervised monitoring nor validated. Furthermore, the monitoring is strictly informational and medically-significant events, such as serious cardiac rhythm disorders, including tachyarrhythmias and bradyarrhythmias, while potentially detectable, are neither identified nor acted upon.

In today's medical and legal environment, a mobile device, such as a smartphone, provides information that cannot be translated into data that triggers surgery or drug therapy by a physician. In the case of a smartphone detecting a fast heartbeat, for example, such a detection and the information on the smartphone would neither be identified as truly related to the patient in question or would be deemed sufficient for subjecting a patient to surgery or potentially toxic drug therapy. Thus, such data that is available today is not actionable in a medically therapeutic relevant way. To make such data actionable, one must have recorded data that allows a specific rhythm diagnosis, and a vague recording hinting that something may be wrong with the heart will not suffice. Further, the recorded data must not only identify the heart-related event of concern, but the signals before and after the event, which provides critical medical information for a physician to diagnose the disorder specifically. Finally, the recorded data must be made certifiable, so that the relationship of the recorded data to the patient that the

physician is seeing is clear and appropriately identifiable as an event originating in the patient being examined. Establishing this relationship of data-to-patient has become a legally mandatory step in providing medical care, which heretofore has been impracticable insofar as one cannot merely rely upon a smartphone to provide legally sufficient identification of an abnormality with actionable data such that a patient undergoes a serious medical intervention.

Therefore, a need remains for an extended wear continuously recording ECG monitor practicably capable of being worn for a long period of time in both men and women and capable of recording high quality atrial and ventricular signals reliably.

A further need remains for facilities to integrate wider-ranging physiological and "life tracking"-type data into long-term ECG and physiological data monitoring coupled with an onboard ability to cascade into the medical records and to the medical authorities appropriate medical intervention upon detection of a condition of potential medical concern.

SUMMARY

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. The wearable monitor sits centrally (in the midline) on the patient's chest along the sternum oriented top-to-bottom. The placement of the wearable monitor in a location at the sternal midline (or immediately to either side of the sternum), with its unique narrow "hourglass"-like shape, benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch anywhere within the general region of the sternum, the area most likely to record high quality atrial signals or P-waves. Moreover, the wearable monitor is worn in such a location that is comfortable to woman and allows wear during activity.

In a further embodiment, the wearable monitor can interoperate wirelessly with other wearable physiology monitors and activity sensors and with mobile devices, including so-called "smartphones," as well as with personal computers and tablet or handheld computers, to download monitoring data either in real-time or in batches. Where a wearable physiology monitor, activity sensor, or mobile device worn or held by the patient includes the capability to sense cardiac activity, particularly heart rate, or other physiology, an application executed by the monitor, sensor, or device can trigger the dispatch of a medically-actionable wearable monitor to the patient upon detecting potentially medically-significant events, such as cardiac rhythm disorders, including tachyarrhythmias and bradyarrhythmias. Upon receipt of the wearable monitor, the patient can use the sensor or device, if appropriately equipped with photographic, fingerprint or thumbprint, or other recording features, to physically record the placement and use of the wearable monitor, thereby facilitating the authentication of the data recorded by the wearable monitor. Finally, the monitor recorder can also be equipped with a wireless transceiver to either provide data or other information to, or receive data or other information from, an interfacing wearable physiology monitor, activity sensor, or mobile device for relay to an external system or further device, such as a server, analysis, or for further legal validation of the relationship of the monitor to the patient, or for other purpose.

One embodiment provides a remotely-interfaceable extended wear electrocardiography and physiological sensor monitor recorder. A sealed housing is adapted to be removably secured into the non-conductive receptacle on a disposable extended wear electrode patch. Electronic circuitry is included within the sealed housing. An externally-powered micro-controller is operable to execute under micro programmable control. An electrocardiographic front end circuit is electrically interfaced to the micro-controller and is operable to sense electrocardiographic signals through electrocardiographic electrodes provided on the disposable extended wear electrode patch. A wireless transceiver is electrically interfaced with the micro-controller and is operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals. Externally-powered flash memory is electrically interfaced with the micro-controller and is operable to store the samples of the electrocardiographic signals.

A further embodiment provides a remotely-interfaceable extended wear electrocardiography and physiological sensor monitor. A disposable extended wear electrode patch includes a flexible backing formed of an elongated strip of stretchable material with a narrow longitudinal midsection and, on each end, a contact surface at least partially coated with an adhesive dressing provided as a crimp relief. A pair of electrocardiographic electrodes is conductively exposed on the contact surface of each end of the elongated strip. A non-conductive receptacle is adhered to an outward-facing end of the elongated strip and includes a plurality of electrical pads. A flexible circuit is affixed on each end of the elongated strip as a strain relief and includes a pair of circuit traces electrically coupled to the pair of electrocardiographic electrodes and a pair of the electrical pads. A reusable electrocardiography monitor has a sealed housing adapted to be removably secured into the non-conductive receptacle. A micro-controller is operable to execute under micro programmable control and is electrically interfaced to an electrocardiographic front end circuit that is operable to sense electrocardiographic signals through the electrocardiographic electrodes via the pair of electrical pads. A wireless transceiver is electrically interfaced with the micro-controller and is operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals. Flash memory is electrically interfaced with the micro-controller and is operable to store the samples of the electrocardiographic signals.

A still further embodiment provides a computer-implemented system and method for providing a personal mobile device-triggered medical intervention. An activity monitor is adapted to be used proximal to a patient's body and includes a physiology sensor operable to sense physiological data of the body. A personal mobile device includes an application executable by the mobile device that is configured to detect an event of potential medical significance within the sensed physiological data. The mobile device also includes a wireless transceiver operable to interface the mobile device with an external system and to send notification of a detection of the event. An extended wear electrocardiography and physiological sensor monitor recorder is dispatched by the external system upon receipt of the notification.

The monitoring patch is especially suited to the female anatomy. The narrow longitudinal midsection can fit nicely within the intermammary cleft of the breasts without inducing discomfort, whereas conventional patch electrodes are wide and, if adhered between the breasts, particularly hypertrophic or pendulous breasts, would cause chafing, irritation, frustration, and annoyance, leading to low patient compli-

ance and possibly premature removal of the monitoring patch. Furthermore, such conventional patches do not have the electrical design and signal processing that would allow recording of the P-wave, given the close spacing of the bipolar electrodes.

The foregoing aspects enhance ECG monitoring performance and quality, facilitating long-term ECG recording, critical to accurate arrhythmia diagnosis.

In addition, the foregoing aspects enhance comfort in women (and certain men), but not irritation of the breasts, by placing the monitoring patch in the best location possible for optimizing the recording of cardiac signals from the atrium, another feature critical to proper arrhythmia diagnosis.

Finally, the foregoing aspects as relevant to monitoring are equally applicable to recording other physiological data, such as heart rate, temperature, blood pressure, respiratory rate, blood pressure, blood sugar (with appropriate subcutaneous probe), oxygen saturation, minute ventilation, as well as other measures of body chemistry and physiology.

Still other embodiments will become readily apparent to those skilled in the art from the following detailed description, wherein are described embodiments by way of illustrating the best mode contemplated. As will be realized, other and different embodiments are possible and the embodiments' several details are capable of modifications in various obvious respects, all without departing from their spirit and the scope. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor respectively fitted to the sternal region of a female patient and a male patient.

FIG. 3 is a functional block diagram showing a system for remote interfacing of an extended wear electrocardiography and physiological sensor monitor in accordance with one embodiment.

FIG. 4 is a perspective view showing an extended wear electrode patch with a monitor recorder inserted.

FIG. 5 is a perspective view showing the monitor recorder of FIG. 4.

FIG. 6 is a perspective view showing the extended wear electrode patch of FIG. 4 without a monitor recorder inserted.

FIG. 7 is a bottom plan view of the monitor recorder of FIG. 4.

FIG. 8 is a top view showing the flexible circuit of the extended wear electrode patch of FIG. 4 when mounted above the flexible backing

FIG. 9 is a functional block diagram showing the component architecture of the circuitry of the monitor recorder of FIG. 4.

FIG. 10 is a functional block diagram showing the circuitry of the extended wear electrode patch of FIG. 4.

FIG. 11 is a flow diagram showing a monitor recorder-implemented method for monitoring ECG data for use in the monitor recorder of FIG. 4.

FIG. 12 is a graph showing, by way of example, a typical ECG waveform.

FIG. 13 is a flow diagram showing a method for offloading and converting ECG and other physiological data from

an extended wear electrocardiography and physiological sensor monitor in accordance with one embodiment.

DETAILED DESCRIPTION

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor 12, including a monitor recorder 14 in accordance with one embodiment, respectively fitted to the sternal region of a female patient 10 and a male patient 11. The wearable monitor 12 sits centrally (in the midline) on the patient's chest along the sternum 13 oriented top-to-bottom with the monitor recorder 14 preferably situated towards the patient's head. In a further embodiment, the orientation of the wearable monitor 12 can be corrected post-monitoring, as further described infra. The electrode patch 15 is shaped to fit comfortably and conformal to the contours of the patient's chest approximately centered on the sternal midline 16 (or immediately to either side of the sternum 13). The distal end of the electrode patch 15 extends towards the Xiphoid process and, depending upon the patient's build, may straddle the region over the Xiphoid process. The proximal end of the electrode patch 15, located under the monitor recorder 14, is below the manubrium and, depending upon patient's build, may straddle the region over the manubrium.

The placement of the wearable monitor 12 in a location at the sternal midline 16 (or immediately to either side of the sternum 13) significantly improves the ability of the wearable monitor 12 to cutaneously sense cardiac electric signals, particularly the P-wave (or atrial activity) and, to a lesser extent, the QRS interval signals in the ECG waveforms that indicate ventricular activity, while simultaneously facilitating comfortable long-term wear for many weeks. The sternum 13 overlies the right atrium of the heart and the placement of the wearable monitor 12 in the region of the sternal midline 13 puts the ECG electrodes of the electrode patch 15 in a location better adapted to sensing and recording P-wave signals than other placement locations, say, the upper left pectoral region or lateral thoracic region or the limb leads. In addition, placing the lower or inferior pole (ECG electrode) of the electrode patch 15 over (or near) the Xiphoid process facilitates sensing of ventricular activity and provides superior recordation of the QRS interval.

When operated standalone, the monitor recorder 14 of the extended wear electrocardiography and physiological sensor monitor 12 senses and records the patient's ECG data into an onboard memory. In addition, the wearable monitor 12 can interoperate with other devices. FIG. 3 is a functional block diagram showing a system 120 for remote interfacing of an extended wear electrocardiography and physiological sensor monitor 12 in accordance with one embodiment. The monitor recorder 14 is a reusable component that can be fitted during patient monitoring into a non-conductive receptacle provided on the electrode patch 15, as further described infra with reference to FIG. 4, and later removed for offloading of stored ECG data or to receive revised programming. The monitor recorder 14 can then be connected to a download station 125, which could be a programmer or other device that permits the retrieval of stored ECG monitoring data, execution of diagnostics on or programming of the monitor recorder 14, or performance of other functions. The monitor recorder 14 has a set of electrical contacts (not shown) that enable the monitor recorder 14 to physically interface to a

set of terminals **128** on a paired receptacle **127** of the download station **125**. In turn, the download station **125** executes a communications or offload program **126** (“Of-fload”) or similar program that interacts with the monitor recorder **14** via the physical interface to retrieve the stored ECG monitoring data. The download station **125** could be a server, personal computer, tablet or handheld computer, smart mobile device, or purpose-built programmer designed specific to the task of interfacing with a monitor recorder **14**. Still other forms of download station **125** are possible.

Upon retrieving stored ECG monitoring data from a monitor recorder **14**, middleware first operates on the retrieved data to adjust the ECG capture quality, as necessary, and to convert the retrieved data into a format suitable for use by third party post-monitoring analysis software, as further described infra with reference to FIG. **13**. The formatted data can then be retrieved from the download station **125** over a hard link **135** using a control program **137** (“Ctl”) or analogous application executing on a personal computer **136** or other connectable computing device, via a communications link (not shown), whether wired or wireless, or by physical transfer of storage media (not shown). The personal computer **136** or other connectable device may also execute middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program, as further described infra with reference to FIG. **13**. Note that formatted data stored on the personal computer **136** would have to be maintained and safeguarded in the same manner as electronic medical records (EMRs) **134** in the secure database **124**, as further discussed infra. In a further embodiment, the download station **125** is able to directly interface with other devices over a computer communications network **121**, which could be some combination of a local area network and a wide area network, including the Internet, over a wired or wireless connection.

A client-server model could be used to employ a server **122** to remotely interface with the download station **125** over the network **121** and retrieve the formatted data or other information. The server **122** executes a patient management program **123** (“Mgt”) or similar application that stores the retrieved formatted data and other information in a secure database **124** cataloged in that patient’s EMRs **134**. In addition, the patient management program **123** could manage a subscription service that authorizes a monitor recorder **14** to operate for a set period of time or under pre-defined operational parameters.

The patient management program **123**, or other trusted application, also maintains and safeguards the secure database **124** to limit access to patient EMRs **134** to only authorized parties for appropriate medical or other uses, such as mandated by state or federal law, such as under the Health Insurance Portability and Accountability Act (HIPAA) or per the European Union’s Data Protection Directive. For example, a physician may seek to review and evaluate his patient’s ECG monitoring data, as securely stored in the secure database **124**. The physician would execute an application program **130** (“Pgm”), such as a post-monitoring ECG analysis program, on a personal computer **129** or other connectable computing device, and, through the application **130**, coordinate access to his patient’s EMRs **134** with the patient management program **123**. Other schemes and safeguards to protect and maintain the integrity of patient EMRs **134** are possible.

The wearable monitor **12** can interoperate wirelessly with other wearable physiology monitors and activity sensors **131**, such as activity trackers worn on the wrist or body, and

with mobile devices **133**, including smart watches and smartphones. Wearable physiology monitors and activity sensors **131** encompass a wide range of wirelessly interconnectable devices that measure or monitor a patient’s physiological data, such as heart rate, temperature, blood pressure, respiratory rate, blood pressure, blood sugar (with appropriate subcutaneous probe), oxygen saturation, minute ventilation, and so on; physical states, such as movement, sleep, footsteps, and the like; and performance, including calories burned or estimated blood glucose level. The physiology sensors in non-wearable mobile devices, particularly smartphones, are generally not meant for continuous tracking and do not provide medically precise and actionable data sufficient for a physician to prescribe a surgical or serious drug intervention; such data can be considered screening information that something may be wrong, but not data that provides the highly precise information that may allow for a surgery, such as implantation of a pacemaker for heart block or a defibrillator for ventricular tachycardia, or the application of serious medications, like blood thinners for atrial fibrillation or a cardiac ablation procedure. Such devices, like smartphones, are better suited to pre- and post-exercise monitoring or as devices that can provide a signal that something is wrong, but not in the sufficient detail and validation to allow for medical action. Conversely, medically actionable wearable sensors and devices sometimes provide continuous recording for relatively short time periods, but must be paired with a smartphone or computer to offload and evaluate the recorded data, especially if the data is of urgent concern.

Wearable physiology monitors and activity sensors **131**, also known as “activity monitors,” and to a lesser extent, “fitness” sensor-equipped mobile devices **133**, can trace their life-tracking origins to ambulatory devices used within the medical community to sense and record traditional medical physiology that could be useful to a physician in arriving at a patient diagnosis or clinical trajectory, as well as from outside the medical community, from, for instance, sports or lifestyle product companies who seek to educate and assist individuals with self-quantifying interests. Data is typically tracked by the wearable physiology monitors or activity sensors **131** and mobile device **133** for only the personal use of the wearer. The physiological monitoring is strictly informational, even where a device originated within the medical community, and the data is generally not time-correlated to physician-supervised monitoring. Importantly, medically-significant events, such as cardiac rhythm disorders, including tachyarrhythmias, like ventricular tachycardia or atrial fibrillation, and bradyarrhythmias, like heart block, while potentially detectable with the appropriate diagnostic heuristics, are neither identified nor acted upon by the wearable physiology monitors and activity sensors **131** and the mobile device **133**.

Frequently, wearable physiology monitors and activity sensors **131** are capable of wirelessly interfacing with mobile devices **133**, particularly smart mobile devices, including so-called “smartphones” and “smart watches,” as well as with personal computers and tablet or handheld computers, to download monitoring data either in real-time or in batches. The wireless interfacing of such activity monitors is generally achieved using transceivers that provide low-power, short-range wireless communications, such as Bluetooth, although some wearable physiology monitors and activity sensors **131**, like their mobile device cohorts, have transceivers that provide true wireless communications services, including 4G or better mobile telecommunications,

over a telecommunications network. Other types of wireless and wired interfacing are possible.

Where the wearable physiology monitors and activity sensors **131** are paired with a mobile device **133**, the mobile device **133** executes an application (“App”) that can retrieve the data collected by the wearable physiology monitor and activity sensor **131** and evaluate the data to generate information of interest to the wearer, such as an estimation of the effectiveness of the wearer’s exercise efforts. Where the wearable physiology monitors and activity sensors **131** has sufficient onboard computational resources, the activity monitor itself executes an app without the need to relay data to a mobile device **133**. Generally, such more computationally-capable wearable physiology monitors and activity sensors are also equipped with wireless communications services transceivers, such as found in some smart watches that combine the features of activity monitors with mobile devices. Still other activity monitor and mobile device functions on the collected data are possible.

In a further embodiment, a wearable physiology monitor, activity sensor **131**, or mobile device **133** worn or held by the patient **10**, or otherwise be used proximal to the patient’s body, can be used to first obtain and then work collaboratively with a more definitive monitor recorder **14** to enable the collection of physiology by the monitor recorder **14** before, during, and after potentially medically-significant events. The wearable physiology monitor, activity sensor **131**, or mobile device **133** must be capable of sensing cardiac activity, particularly heart rate or rhythm, or other types of physiology or measures, either directly or upon review of relayed data. Where the wearable physiology monitor or activity sensor **131** is paired with a mobile device **133**, the mobile device **133** serves as a relay device and executes an application that will trigger the dispatch of a monitor recorder **14** to the patient **10** upon detecting potentially medically-significant events in the data provided by the paired activity monitor, such as cardiac rhythm disorders, including tachyarrhythmias and bradyarrhythmias. If the mobile device **133** is itself performing the monitoring of the patient’s physiology, the mobile device **133** executes an application that will trigger the dispatch of a monitor recorder **14** to the patient **10** in near-real time upon detecting potentially medically-significant events, thereby avoiding the delay incurred by data relay from an activity monitor. Finally, if the wearable physiology monitor or activity sensor **131** has sufficient onboard computational resources and also is equipped with a wireless communications services transceiver, the wearable physiology monitor or activity sensor **131** effectively becomes the mobile device **133** and executes an application that will trigger the dispatch of a monitor recorder **14** to the patient **10** in near-real time upon detecting potentially medically-significant events without the need to first interface with a mobile device **133**. Still other configurations of the detection app are possible.

The act of triggering the dispatch of a monitor recorder **14** represents the first step in a cascade of possible medical interventions of potentially increasing seriousness and urgency. Sensors **131** and devices **133** are generally not capable of detecting and recording medically precise and actionable data, whereas, as a device designed for extended wear, the monitor recorder **14** continually monitors the patient’s physiology over a long time period and will capture any medically-actionable data leading up to, throughout the occurrence of, and following an event of potential medical concern.

The monitoring data recorded by the monitor recorder **14** can be uploaded directly into the patient’s EMRs **134**, either

by using a mobile device **133** as a conduit for communications with a server **122** coupled to a secure database **124** within which the patient’s EMRs **134** are stored, or directly to the server **122**, if the monitor recorder **14** is appropriately equipped with a wireless transceiver or similar external data communications interface, as further described infra. Thus, the data recorded by the monitor recorder **14** would directly feed into the patient’s EMRs **134**, thereby allowing the data to be made certifiable for immediate use by a physician or healthcare provider. No intermediate steps would be necessary when going from cutaneously sensing cardiac electric signals and collecting the patient’s physiology using a monitor recorder **14** to presenting that recorded data to a physician or healthcare provider for medical diagnosis and care. The direct feeding of data from the monitor recorder **14** to the EMRs **134** clearly establishes the relationship of the data, as recorded by the monitor recorder **14**, to the patient **10** that the physician is seeing and appropriately identifies any potentially medically-significant event recorded in the data as originating in the patient **10** and nobody else. Based on the monitoring data, physicians and healthcare providers can rely on the data as certifiable and can directly proceed with determining the appropriate course of treatment for the patient **10**, including undertaking further medical interventions as appropriate. In a further embodiment, the server **122** can evaluate the recorded data, as fed into the patient’s EMRs **134**, to refer the patient **10** for medical care to a general practice physician or medical specialist, for instance, a cardiac electrophysiologist referral from a cardiologist when the recorded data indicates an event of sufficient potential severity to warrant the possible implantation of a pacemaker for heart block or a defibrillator for ventricular tachycardia. Other uses of the data recorded by the monitor recorder **14** are possible.

For instance, a patient **10** who has previously suffered heart failure is particularly susceptible to ventricular tachycardia following a period of exercise or strenuous physical activity. A wearable sensor **131** or device **133** that includes a heart rate monitor would be able to timely detect an irregularity in heart rhythm. The application executed by the sensor **131** or device **133** allows those devices to take action by triggering the dispatch of a monitor recorder **14** to the patient **10**, even though the data recorded by the sensor **131** or device **133** is itself generally medically-insufficient for purposes of diagnosis and care. Thus, rather than passively recording patient data, the sensor **131** or device **133** takes on an active role in initiating the provisioning of medical care to the patient **10** and starts a cascade of appropriate medical interventions under the tutelage of and followed by physicians and trained healthcare professionals.

In a still further embodiment, the monitor recorder **14** could upload an event detection application to the sensor **131** or device **133** to enable those devices to detect those types of potentially medically-significant events, which would trigger the dispatch of a monitor recorder **14** to the patient **10**. Alternatively, the event detection application could be downloaded to the sensor **131** or device **133** from an online application store or similar online application repository. Finally, the monitor recorder **14** could use the sensor **131** or device **133** to generate an appropriate alert, including contacting the patient’s physician or healthcare services, via wireless (or wired) communications, upon detecting a potentially medically-significant event or in response to a patient prompting.

The patient **10** could be notified by the sensor **131** or device **133**, through the sensor’s or device’s user interface, that an event of potential medical concern has been detected

13

coupled with an offer to have a monitor recorder **14** sent out to the patient **10**, assuming that the patient **10** is not already wearing a monitor recorder **14**. Alternatively, the sensor **131** or device **133** could unilaterally send out a request for a monitor recorder **14**. The request for a monitor recorder **14** could be sent via wireless (or wired) communications to the patient's physician, a medical service provider organization, a pharmacy, an emergency medical service, or other appropriate healthcare entity that would, in turn, physically provide the patient with a monitor recorder **14**. The patient **10** could also be told to pick up a monitor recorder **14** directly from one of the above-identified sources.

Conventional Holter monitors, as well as the ZIO XT Patch and ZIO Event Card devices, described supra, are currently available only by a physician's prescription for a specific patient **10**. As a result, the physiological data recorded by these monitors and devices are assumed by healthcare professional to belong to the patient **10**. In this prescriptive medicine context, grave questions as to the authenticity of the patient's identity and the data recorded do not generally arise, although current medical practice still favors requesting affirmative patient and caregiver identification at every step of healthcare provisioning. As a device intended for adoption and usage broader than prescriptive medicine, the monitor recorder **14** carries the potential to be used by more than one individual, which can raise concerns as to the veracity of the data recorded.

In a still further embodiment, the mobile device **133**, or, if properly equipped, the activity monitor, can be used to help authenticate the patient **10** at the outset of and throughout the monitoring period. The mobile device **133** (or activity monitor) must be appropriately equipped with a digital camera or other feature capable of recording physical indicia located within the proximity of the mobile device **133**. For instance, the Samsung Galaxy S5 smartphone has both a biometric fingerprint reader and autofocus digital camera built in. Upon receipt of a monitor recorder **14**, the patient **10** can use the photographic or other recording features of the mobile device **133** (or activity monitor) to physically record the placement and use of the monitor recorder **14**. For instance, the patient **10** could take a picture or make a video of the monitor recorder **14** using as applied to the chest using the built-in digital camera. The patient **10** could also swipe a finger over the biometric fingerprint reader. Preferably, the patient **10** would include both his or her face or similar uniquely-identifying marks or indicia, such as a scar, tattoo, body piercing, or RFID chip, plus any visible or electronic indicia on the outside of the monitor recorder's housing, as further described infra with reference to FIG. 5, in the physical recording. The physical recording would then be sent by the mobile device **133** (or activity monitor) via wireless (or wired) communications to the patient's physician's office or other appropriate caregiver, thereby facilitating the authentication of the data recorded by the monitor recorder **14**. Alternatively, the physical recording could be securely stored by the monitor recorder **14** as part of the monitoring data set.

The mobile device **133** could also serve as a conduit for providing the data collected by the wearable physiology monitor or activity sensor **131** to a server **122**, or, similarly, the wearable physiology monitor or activity sensor **131** could itself directly provide the collected data to the server **122**. The server **122** could then merge the collected data into the wearer's EMRs **134** in the secure database **124**, if appropriate (and permissible), or the server **122** could perform an analysis of the collected data, perhaps based by comparison to a population of like wearers of the wearable

14

physiology monitor or activity sensor **131**. Still other server **122** functions on the collected data are possible.

Finally, the monitor recorder **14** can also be equipped with a wireless transceiver, as further described infra with reference to FIGS. 9 and 10. Thus, when wireless-enabled, both wearable physiology monitors, activity sensors **131**, and mobile devices **133** can wirelessly interface with the monitor recorder **14**, which could either provide data or other information to, or receive data or other information from an interfacing device for relay to a further device, such as the server **122**, analysis, or other purpose. In addition, the monitor recorder **14** could wirelessly interface directly with the server **122**, personal computer **129**, or other computing device connectable over the network **121**, when the monitor recorder **14** is appropriately equipped for interfacing with such devices. Still other types of remote interfacing of the monitor recorder **14** are possible.

During use, the electrode patch **15** is first adhered to the skin along the sternal midline **16** (or immediately to either side of the sternum **13**). A monitor recorder **14** is then snapped into place on the electrode patch **15** to initiate ECG monitoring. FIG. 4 is a perspective view showing an extended wear electrode patch **15** with a monitor recorder **14** in accordance with one embodiment inserted. The body of the electrode patch **15** is preferably constructed using a flexible backing **20** formed as an elongated strip **21** of wrap knit or similar stretchable material with a narrow longitudinal mid-section **23** evenly tapering inward from both sides. A pair of cut-outs **22** between the distal and proximal ends of the electrode patch **15** create a narrow longitudinal midsection **23** or "isthmus" and defines an elongated "hourglass"-like shape, when viewed from above.

The electrode patch **15** incorporates features that significantly improve wearability, performance, and patient comfort throughout an extended monitoring period. During wear, the electrode patch **15** is susceptible to pushing, pulling, and torquing movements, including compressional and torsional forces when the patient bends forward, and tensile and torsional forces when the patient leans backwards. To counter these stress forces, the electrode patch **15** incorporates strain and crimp reliefs, such as described in commonly-assigned U.S. Pat. No. 9,545,204, issued Jan. 17, 2017, the disclosure of which is incorporated by reference. In addition, the cut-outs **22** and longitudinal midsection **23** help minimize interference with and discomfort to breast tissue, particularly in women (and gynecomastic men). The cut-outs **22** and longitudinal midsection **23** further allow better conformity of the electrode patch **15** to sternal bowing and to the narrow isthmus of flat skin that can occur along the bottom of the intermammary cleft between the breasts, especially in buxom women. The cut-outs **22** and longitudinal midsection **23** help the electrode patch **15** fit nicely between a pair of female breasts in the intermammary cleft. Still other shapes, cut-outs and conformities to the electrode patch **15** are possible.

The monitor recorder **14** removably and reusably snaps into an electrically non-conductive receptacle **25** during use. The monitor recorder **14** contains electronic circuitry for recording and storing the patient's electrocardiography as sensed via a pair of ECG electrodes provided on the electrode patch **15**, such as described in commonly-assigned U.S. Pat. No. 9,730,593, issued Aug. 15, 2017, the disclosure which is incorporated by reference. The non-conductive receptacle **25** is provided on the top surface of the flexible backing **20** with a retention catch **26** and tension clip **27**

molded into the non-conductive receptacle **25** to conformably receive and securely hold the monitor recorder **14** in place.

The monitor recorder **14** includes a sealed housing that snaps into place in the non-conductive receptacle **25**. FIG. **5** is a perspective view showing the monitor recorder **14** of FIG. **4**. The sealed housing **50** of the monitor recorder **14** intentionally has a rounded isosceles trapezoidal-like shape **52**, when viewed from above, such as described in commonly-assigned U.S. Design Patent No. D717,955, issued Nov. 18, 2014, the disclosure of which is incorporated by reference. In addition, a label, barcode, QR code, or other visible or electronic indicia is printed **160** on the outside of, applied **161** to the outside of, or integrated **162** into the sealed housing **50** to uniquely identify the monitor recorder **14** and can include a serial number, manufacturing lot number, date of manufacture, and so forth. The edges **51** along the top and bottom surfaces are rounded for patient comfort. The sealed housing **50** is approximately 47 mm long, 23 mm wide at the widest point, and 7 mm high, excluding a patient-operable tactile-feedback button **55**. The sealed housing **50** can be molded out of polycarbonate, ABS, or an alloy of those two materials. The button **55** is waterproof and the button's top outer surface is molded silicon rubber or similar soft pliable material. A retention detent **53** and tension detent **54** are molded along the edges of the top surface of the housing **50** to respectively engage the retention catch **26** and the tension clip **27** molded into non-conductive receptacle **25**. Other shapes, features, and conformities of the sealed housing **50** are possible.

The electrode patch **15** is intended to be disposable. The monitor recorder **14**, however, is reusable and can be transferred to successive electrode patches **15** to ensure continuity of monitoring. The placement of the wearable monitor **12** in a location at the sternal midline **16** (or immediately to either side of the sternum **13**) benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch **15** anywhere within the general region of the sternum **13**.

As a result, at any point during ECG monitoring, the patient's skin is able to recover from the wearing of an electrode patch **15**, which increases patient comfort and satisfaction, while the monitor recorder **14** ensures ECG monitoring continuity with minimal effort. A monitor recorder **14** is merely unsnapped from a worn out electrode patch **15**, the worn out electrode patch **15** is removed from the skin, a new electrode patch **15** is adhered to the skin, possibly in a new spot immediately adjacent to the earlier location, and the same monitor recorder **14** is snapped into the new electrode patch **15** to reinitiate and continue the ECG monitoring.

During use, the electrode patch **15** is first adhered to the skin in the sternal region. FIG. **6** is a perspective view showing the extended wear electrode patch **15** of FIG. **4** without a monitor recorder **14** inserted. A flexible circuit **32** is adhered to each end of the flexible backing **20**. A distal circuit trace **33** and a proximal circuit trace (not shown) electrically couple ECG electrodes (not shown) to a pair of electrical pads **34**. The electrical pads **34** are provided within a moisture-resistant seal **35** formed on the bottom surface of the non-conductive receptacle **25**. When the monitor recorder **14** is securely received into the non-conductive receptacle **25**, that is, snapped into place, the electrical pads **34** interface to electrical contacts (not shown) protruding from the bottom surface of the monitor recorder **14**, and the

moisture-resistant seal **35** enables the monitor recorder **14** to be worn at all times, even during bathing or other activities that could expose the monitor recorder **14** to moisture.

In addition, a battery compartment **36** is formed on the bottom surface of the non-conductive receptacle **25**, and a pair of battery leads (not shown) electrically interface the battery to another pair of the electrical pads **34**. The battery contained within the battery compartment **35** can be replaceable, rechargeable or disposable.

The monitor recorder **14** draws power externally from the battery provided in the non-conductive receptacle **25**, thereby uniquely obviating the need for the monitor recorder **14** to carry a dedicated power source. FIG. **7** is a bottom plan view of the monitor recorder **14** of FIG. **4**. A cavity **58** is formed on the bottom surface of the sealed housing **50** to accommodate the upward projection of the battery compartment **36** from the bottom surface of the non-conductive receptacle **25**, when the monitor recorder **14** is secured in place on the non-conductive receptacle **25**. A set of electrical contacts **56** protrude from the bottom surface of the sealed housing **50** and are arranged in alignment with the electrical pads **34** provided on the bottom surface of the non-conductive receptacle **25** to establish electrical connections between the electrode patch **15** and the monitor recorder **14**. In addition, a seal coupling **57** circumferentially surrounds the set of electrical contacts **56** and securely mates with the moisture-resistant seal **35** formed on the bottom surface of the non-conductive receptacle **25**.

The placement of the flexible backing **20** on the sternal midline **16** (or immediately to either side of the sternum **13**) also helps to minimize the side-to-side movement of the wearable monitor **12** in the left- and right-handed directions during wear. To counter the dislodgment of the flexible backing **20** due to compressional and torsional forces, a layer of non-irritating adhesive, such as hydrocolloid, is provided at least partially on the underside, or contact surface of the flexible backing **20**, but only on the distal end **30** and the proximal end **31**. As a result, the underside, or contact surface of the longitudinal midsection **23** does not have an adhesive layer and remains free to move relative to the skin. Thus, the longitudinal midsection **23** forms a crimp relief that respectively facilitates compression and twisting of the flexible backing **20** in response to compressional and torsional forces. Other forms of flexible backing crimp reliefs are possible.

Unlike the flexible backing **20**, the flexible circuit **32** is only able to bend and cannot stretch in a planar direction. The flexible circuit **32** can be provided either above or below the flexible backing **20**. FIG. **8** is a top view showing the flexible circuit **32** of the extended wear electrode patch **15** of FIG. **4** when mounted above the flexible backing **20**. A distal ECG electrode **38** and proximal ECG electrode **39** are respectively coupled to the distal and proximal ends of the flexible circuit **32**. A strain relief **40** is defined in the flexible circuit **32** at a location that is partially underneath the battery compartment **36** when the flexible circuit **32** is affixed to the flexible backing **20**. The strain relief **40** is laterally extendable to counter dislodgment of the ECG electrodes **38**, **39** due to tensile and torsional forces. A pair of strain relief cutouts **41** partially extend transversely from each opposite side of the flexible circuit **32** and continue longitudinally towards each other to define in 'S'-shaped pattern, when viewed from above. The strain relief respectively facilitates longitudinal extension and twisting of the flexible circuit **32** in response to tensile and torsional forces. Other forms of circuit board strain relief are possible.

ECG monitoring and other functions performed by the monitor recorder 14 are provided through a micro controlled architecture. FIG. 9 is a functional block diagram showing the component architecture of the circuitry 60 of the monitor recorder 14 of FIG. 4. The circuitry 60 is externally powered through a battery provided in the non-conductive receptacle 25 (shown in FIG. 6). Both power and raw ECG signals, which originate in the pair of ECG electrodes 38, 39 (shown in FIG. 8) on the distal and proximal ends of the electrode patch 15, are received through an external connector 65 that mates with a corresponding physical connector on the electrode patch 15. The external connector 65 includes the set of electrical contacts 56 that protrude from the bottom surface of the sealed housing 50 and which physically and electrically interface with the set of pads 34 provided on the bottom surface of the non-conductive receptacle 25. The external connector includes electrical contacts 56 for data download, microcontroller communications, power, analog inputs, and a peripheral expansion port. The arrangement of the pins on the electrical connector 65 of the monitor recorder 14 and the device into which the monitor recorder 14 is attached, whether an electrode patch 15 or download station (not shown), follow the same electrical pin assignment convention to facilitate interoperability. The external connector 65 also serves as a physical interface to a download station that permits the retrieval of stored ECG monitoring data, communication with the monitor recorder 14, and performance of other functions.

Operation of the circuitry 60 of the monitor recorder 14 is managed by a microcontroller 61. The micro-controller 61 includes a program memory unit containing internal flash memory that is readable and writeable. The internal flash memory can also be programmed externally. The microcontroller 61 draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. The microcontroller 61 connects to the ECG front end circuit 63 that measures raw cutaneous electrical signals and generates an analog ECG signal representative of the electrical activity of the patient's heart over time.

The circuitry 60 of the monitor recorder 14 also includes a flash memory 62, which the micro-controller 61 uses for storing ECG monitoring data and other physiology and information. The flash memory 62 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. Data is stored in a serial flash memory circuit, which supports read, erase and program operations over a communications bus. The flash memory 62 enables the microcontroller 61 to store digitized ECG data. The communications bus further enables the flash memory 62 to be directly accessed externally over the external connector 65 when the monitor recorder 14 is interfaced to a download station.

The circuitry 60 of the monitor recorder 14 further includes an actigraphy sensor 64 implemented as a 3-axis accelerometer. The accelerometer may be configured to generate interrupt signals to the microcontroller 61 by independent initial wake up and free fall events, as well as by device position. In addition, the actigraphy provided by the accelerometer can be used during post-monitoring analysis to correct the orientation of the monitor recorder 14 if, for instance, the monitor recorder 14 has been inadvertently installed upside down, that is, with the monitor recorder 14 oriented on the electrode patch 15 towards the patient's feet, as well as for other event occurrence analyses, such as described in commonly-assigned U.S. Pat. No. 9,737,224, issued Aug. 22, 2017, the disclosure of which is incorporated by reference.

The circuitry 60 of the monitor recorder 14 includes a wireless transceiver 69 that can provides wireless interfacing capabilities. The wireless transceiver 69 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. The wireless transceiver 69 can be implemented using one or more forms of wireless communications, including the IEEE 802.11 computer communications standard, that is Wi-Fi; the 4G mobile phone mobile standard; the Bluetooth data exchange standard; or other wireless communications or data exchange standards and protocols. The type of wireless interfacing capability could limit the range of interoperability of the monitor recorder 14; for instance, Bluetooth-based implementations are designed for low power consumption with a short communications range.

The microcontroller 61 includes an expansion port that also utilizes the communications bus. External devices, separately drawing power externally from the battery provided on the electrode patch 15 or other source, can interface to the microcontroller 61 over the expansion port in half duplex mode. For instance, an external physiology sensor can be provided as part of the circuitry 60 of the monitor recorder 14, or can be provided on the electrode patch 15 with communication with the micro-controller 61 provided over one of the electrical contacts 56. The physiology sensor can include an SpO₂ sensor, blood pressure sensor, temperature sensor, respiratory rate sensor, glucose sensor, airflow sensor, volumetric pressure sensing, or other types of sensor or telemetric input sources. For instance, the integration of an airflow sensor is described in commonly-assigned U.S. Pat. No. 9,364,155, issued Jun. 14, 2016, the disclosure of which is incorporated by reference.

Finally, the circuitry 60 of the monitor recorder 14 includes patient-interfaceable components, including a tactile feedback button 66, which a patient can press to mark events or to perform other functions, and a buzzer 67, such as a speaker, magnetic resonator or piezoelectric buzzer. The buzzer 67 can be used by the microcontroller 61 to output feedback to a patient such as to confirm power up and initiation of ECG monitoring. Still other components as part of the circuitry 60 of the monitor recorder 14 are possible.

While the monitor recorder 14 operates under micro control, most of the electrical components of the electrode patch 15 operate passively. FIG. 10 is a functional block diagram showing the circuitry 70 of the extended wear electrode patch 15 of FIG. 4. The circuitry 70 of the electrode patch 15 is electrically coupled with the circuitry 60 of the monitor recorder 14 through an external connector 74. The external connector 74 is terminated through the set of pads 34 provided on the bottom of the non-conductive receptacle 25, which electrically mate to corresponding electrical contacts 56 protruding from the bottom surface of the sealed housing 50 to electrically interface the monitor recorder 14 to the electrode patch 15.

The circuitry 70 of the electrode patch 15 performs three primary functions. First, a battery 71 is provided in a battery compartment formed on the bottom surface of the non-conductive receptacle 25. The battery 71 is electrically interfaced to the circuitry 60 of the monitor recorder 14 as a source of external power. The unique provisioning of the battery 71 on the electrode patch 15 provides several advantages. First, the locating of the battery 71 physically on the electrode patch 15 lowers the center of gravity of the overall wearable monitor 12 and thereby helps to minimize shear forces and the effects of movements of the patient and clothing. Moreover, the housing 50 of the monitor recorder 14 is sealed against moisture and providing power externally

avoids having to either periodically open the housing **50** for the battery replacement, which also creates the potential for moisture intrusion and human error, or to recharge the battery, which can potentially take the monitor recorder **14** off line for hours at a time. In addition, the electrode patch **15** is intended to be disposable, while the monitor recorder **14** is a reusable component. Each time that the electrode patch **15** is replaced, a fresh battery is provided for the use of the monitor recorder **14**, which enhances ECG monitoring performance quality and duration of use. Finally, the architecture of the monitor recorder **14** is open, in that other physiology sensors or components can be added by virtue of the expansion port of the microcontroller **61**. Requiring those additional sensors or components to draw power from a source external to the monitor recorder **14** keeps power considerations independent of the monitor recorder **14**. Thus, a battery of higher capacity could be introduced when needed to support the additional sensors or components without effecting the monitor recorders circuitry **60**.

Second, the pair of ECG electrodes **38, 39** respectively provided on the distal and proximal ends of the flexible circuit **32** are electrically coupled to the set of pads **34** provided on the bottom of the non-conductive receptacle **25** by way of their respective circuit traces **33, 37**. The signal ECG electrode **39** includes a protection circuit **72**, which is an inline resistor that protects the patient from excessive leakage current.

Last, in a further embodiment, the circuitry **70** of the electrode patch **15** includes a cryptographic circuit **73** to authenticate an electrode patch **15** for use with a monitor recorder **14**. The cryptographic circuit **73** includes a device capable of secure authentication and validation. The cryptographic device **73** ensures that only genuine, non-expired, safe, and authenticated electrode patches **15** are permitted to provide monitoring data to a monitor recorder **14**, such as described in commonly-assigned U.S. Pat. No. 9,655,538, issued May 23, 2017, the disclosure which is incorporated by reference.

In a further embodiment, the circuitry **70** of the electrode patch **15** includes a wireless transceiver **75**, in lieu the including of the wireless transceiver **69** in the circuitry **60** of the monitor recorder **14**, which interfaces with the microcontroller **61** over the microcontroller's expansion port via the external connector **74**.

The monitor recorder **14** continuously monitors the patient's heart rate and physiology. FIG. **11** is a flow diagram showing a monitor recorder-implemented method **100** for monitoring ECG data for use in the monitor recorder **14** of FIG. **4**. Initially, upon being connected to the set of pads **34** provided with the non-conductive receptacle **25** when the monitor recorder **14** is snapped into place, the microcontroller **61** executes a power up sequence (step **101**). During the power up sequence, the voltage of the battery **71** is checked, the state of the flash memory **62** is confirmed, both in terms of operability check and available capacity, and microcontroller operation is diagnostically confirmed. In a further embodiment, an authentication procedure between the microcontroller **61** and the electrode patch **15** are also performed.

Following satisfactory completion of the power up sequence, an iterative processing loop (steps **102-109**) is continually executed by the microcontroller **61**. During each iteration (step **102**) of the processing loop, the ECG frontend **63** (shown in FIG. **9**) continually senses the cutaneous ECG electrical signals (step **103**) via the ECG electrodes **38, 29** and is optimized to maintain the integrity of the P-wave. A sample of the ECG signal is read (step **104**) by the micro-

controller **61** by sampling the analog ECG signal output front end **63**. FIG. **12** is a graph showing, by way of example, a typical ECG waveform **110**. The x-axis represents time in approximate units of tenths of a second. The y-axis represents cutaneous electrical signal strength in approximate units of millivolts. The P-wave **111** has a smooth, normally upward, that is, positive, waveform that indicates atrial depolarization. The QRS complex usually begins with the downward deflection of a Q wave **112**, followed by a larger upward deflection of an R-wave **113**, and terminated with a downward waveform of the S wave **114**, collectively representative of ventricular depolarization. The T wave **115** is normally a modest upward waveform, representative of ventricular depolarization, while the U wave **116**, often not directly observable, indicates the recovery period of the Purkinje conduction fibers.

Sampling of the R-to-R interval enables heart rate information derivation. For instance, the R-to-R interval represents the ventricular rate and rhythm, while the P-to-P interval represents the atrial rate and rhythm. Importantly, the PR interval is indicative of atrioventricular (AV) conduction time and abnormalities in the PR interval can reveal underlying heart disorders, thus representing another reason why the P-wave quality achievable by the extended wear ambulatory electrocardiography and physiological sensor monitor described herein is medically unique and important. The long-term observation of these ECG indicia, as provided through extended wear of the wearable monitor **12**, provides valuable insights to the patient's cardiac function and overall well-being.

Each sampled ECG signal, in quantized and digitized form, is temporarily staged in buffer (step **105**), pending compression preparatory to storage in the flash memory **62** (step **106**). Following compression, the compressed ECG digitized sample is again buffered (step **107**), then written to the flash memory **62** (step **108**) using the communications bus. Processing continues (step **109**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

In a further embodiment, the monitor recorder **14** also continuously receives data from wearable physiology monitors or activity sensors **131** and mobile devices **133** (shown in FIG. **3**). The data is received in a conceptually-separate execution thread as part of the iterative processing loop (steps **102-109**) continually executed by the microcontroller **61**. During each iteration (step **102**) of the processing loop, if wireless data is available (step **140**), a sample of the wireless is read (step **141**) by the microcontroller **61** and, if necessary, converted into a digital signal by the onboard ADC of the microcontroller **61**. Each wireless data sample, in quantized and digitized form, is temporarily staged in buffer (step **142**), pending compression preparatory to storage in the flash memory **62** (step **143**). Following compression, the compressed wireless data sample is again buffered (step **144**), then written to the flash memory **62** (step **145**) using the communications bus. Processing continues (step **109**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

The monitor recorder **14** stores ECG data and other information in the flash memory **62** (shown in FIG. **9**) using a proprietary format that includes data compression. As a result, data retrieved from a monitor recorder **14** must first

be converted into a format suitable for use by third party post-monitoring analysis software. FIG. 13 is a flow diagram showing a method 150 for offloading and converting ECG and other physiological data from an extended wear electrocardiography and physiological sensor monitor 12 in accordance with one embodiment. The method 150 can be implemented in software and execution of the software can be performed on a download station 125, which could be a programmer or other device, or a computer system, including a server 122 or personal computer 129, such as further described supra with reference to FIG. 3, as a series of process or method modules or steps. For convenience, the method 150 will be described in the context of being performed by a personal computer 136 or other connectable computing device (shown in FIG. 3) as middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program. Execution of the method 150 by a computer system would be analogous mutatis mutandis.

Initially, the download station 125 is connected to the monitor recorder 14 (step 151), such as by physically interfacing to a set of terminals 128 on a paired receptacle 127 or by wireless connection, if available. The data stored on the monitor recorder 14, including ECG and physiological monitoring data, other recorded data, and other information are retrieved (step 152) over a hard link 135 using a control program 137 ("Ctl") or analogous application executing on a personal computer 136 or other connectable computing device.

The data retrieved from the monitor recorder 14 is in a proprietary storage format and each datum of recorded ECG monitoring data, as well as any other physiological data or other information, must be converted, so that the data can be used by a third-party post-monitoring analysis program. Each datum of ECG monitoring data is converted by the middleware (steps 153-159) in an iterative processing loop. During each iteration (step 153), the ECG datum is read (step 154) and, if necessary, the gain of the ECG signal is adjusted (step 155) to compensate, for instance, for relocation or replacement of the electrode patch 15 during the monitoring period.

In addition, depending upon the configuration of the wearable monitor 12, other physiological data (or other information), including patient events, such as a fall, peak activity level, sleep detection, Detection of patient activity levels and states, and so on, may be recorded along with the ECG monitoring data. For instance, actigraphy data may have been sampled by the actigraphy sensor 64 based on a sensed event occurrence, such as a sudden change in orientation due to the patient taking a fall. In response, the monitor recorder 14 will embed the actigraphy data samples into the stream of data, including ECG monitoring data, that is recorded to the flash memory 62 by the micro-controller 61. Post-monitoring, the actigraphy data is temporally matched to the ECG data to provide the proper physiological context to the sensed event occurrence. As a result, the three-axis actigraphy signal is turned into an actionable event occurrence that is provided, through conversion by the middleware, to third party post-monitoring analysis programs, along with the ECG recordings contemporaneous to the event occurrence. Other types of processing of the other physiological data (or other information) are possible.

Thus, during execution of the middleware, any other physiological data (or other information) that has been embedded into the recorded ECG monitoring data is read (step 156) and time-correlated to the time frame of the ECG signals that occurred at the time that the other physiological

data (or other information) was noted (step 157). Finally, the ECG datum, signal gain adjusted, if appropriate, and other physiological data, if applicable and as time-correlated, are stored in a format suitable to the backend software (step 158) used in post-monitoring analysis.

In a further embodiment, the other physiological data, if apropos, is embedded within an unused ECG track. For example, the SCP-ENG standard allows multiple ECG channels to be recorded into a single ECG record. The monitor recorder 14, though, only senses one ECG channel. The other physiological data can be stored into an additional ECG channel, which would otherwise be zero-padded or altogether omitted. The backend software would then be able to read the other physiological data in context with the single channel of ECG monitoring data recorded by the monitor recorder 14, provided the backend software implemented changes necessary to interpret the other physiological data. Still other forms of embedding of the other physiological data with formatted ECG monitoring data, or of providing the other physiological data in a separate manner, are possible.

Processing continues (step 159) for each remaining ECG datum, after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

While the invention has been particularly shown and described as referenced to the embodiments thereof, those skilled in the art will understand that the foregoing and other changes in form and detail may be made therein without departing from the spirit and scope.

What is claimed is:

1. A computer-implemented system for providing a personal mobile device-triggered medical intervention, comprising:

a wearable ambulatory sensor monitor comprising:

a disposable extended wear electrode patch configured for positioning along a sternal midline of a patient, comprising:

a non-conductive receptacle comprising a first set of electrical contact mating pads and a second set of electrical contact mating pads;

a pair of electrocardiographic electrodes, a first electrocardiographic electrode configured for positioning under the non-conductive receptacle on one end of the disposable extended wear electrode patch below the manubrium of a patient and the other electrocardiographic electrode configured for positioning on the other end of the disposable extended wear electrode patch that extends over the Xiphoid process of the patient, wherein the extension over the Xiphoid process facilitates sensing of ventricular activity and provides improved recollection of QRS intervals;

a battery electrically interfaced to the first set of electrical contact mating pads and located between and in alignment with the electrodes, wherein the battery is configured for positioning in a battery compartment provided in the non-conductive receptacle on the electrode patch; and

a flexible circuit connecting each of the electrocardiographic electrodes to one of the electrical contact mating pads of the second set of electrical contact mating pads;

a reusable sealed housing adapted to be removably secured into the non-conductive receptacle and comprising electronic circuitry operable to sense electrocardiographic signals through the electrocardiographic electrodes and a set of electrical contacts

23

protruding from a surface of the sealed housing and contacting the first set of electrical mating pads that connect the battery on the electrode patch and the second set of electrical contact mating pads that connect each of the electrocardiographic electrodes; 5
 an activity monitor adapted to be used proximal to the patient's body comprising a physiology sensor operable to sense physiological data of the body;
 a personal mobile device, comprising:
 a wireless transceiver operable to interface the mobile device with a wirelessly-interfaceable server; 10
 a non-transitory readable storage medium comprising program code; and
 a processor and memory with the processor coupled to the wireless transceiver and the storage medium, 15
 wherein the processor is configured to execute the program code to perform steps to:
 detect an event of potential medical significance comprising a cardiac rhythm disorder within the physiological data as sensed by the physiology 20
 sensor comprised in the activity monitor; and
 trigger dispatch of the wearable ambulatory sensor monitor with the wireless transceiver through a request sent to the server upon the detection of the event of potential medical significance based on 25
 the physiological data; and
 the server operable to dispatch the wearable ambulatory sensor monitor comprising the extended wear electrode patch and the sealed housing to the patient upon receipt of the request as sent from the mobile device after 30
 obtaining the physiological data via the activity monitor, for further monitoring of the patient via the wearable ambulatory sensor monitor.

2. A system according to claim 1, further comprising at least one of: 35
 the activity monitor further adapted to sense the physiological data continuously;
 the activity monitor further adapted to sense the physiological data non-continuously; and
 the activity monitor further adapted to sense the physiological data upon patient triggering. 40

3. A system according to claim 1, the mobile device further comprising:
 the activity monitor.

4. A system according to claim 1, wherein the activity 45
 monitor comprises a device physically independent from the mobile device,
 the activity monitor further comprising:
 a short-range wireless transceiver coupled to the physiology sensor and operable to wirelessly interface the 50
 activity monitor with the wireless transceiver comprised in the mobile device and relay the physiological data as sensed by the physiology sensor comprised in the activity monitor to the mobile device.

5. A system according to claim 1, wherein the physiological 55
 data is selected from the group comprising heart rate, temperature, blood pressure, respiratory rate, blood pressure, blood sugar, oxygen saturation, and minute ventilation.

6. A system according to claim 1, the electronic circuitry further comprising: 60
 an externally-powered micro-controller operable to execute under micro programmable control;
 an electrocardiographic front end circuit electrically interfaced to the micro-controller and operable to sense electrocardiographic signals through electrocardiographic electrodes provided on the disposable extended 65
 wear electrode patch; and

24

externally-powered flash memory electrically interfaced with the micro-controller and operable to store the samples of the electrocardiographic signals.

7. A system according to claim 6, further comprising:
 a recorder wireless transceiver electrically interfaced with the micro-controller and operable to interface the mobile device with a telecommunications network upon which electronic medical records are located; and the micro-controller comprising an upload module as part of the micro programmable control that is configured to send the samples of the electrocardiographic signals directly to the electronic medical records via the recorder wireless transceiver.

8. A system according to claim 7, further comprising:
 a server coupled to the electronic medical records, further comprising:
 a data retrieval module configured to retrieve the samples of the electrocardiographic signals from the electronic medical records; and
 an evaluation module configured to evaluate the samples of the electrocardiographic signals and to refer the patient for medical care.

9. A system according to claim 7, further comprising:
 a recording feature comprised in the mobile device operable to record physical indicia proximal to the mobile device,
 wherein a recording of both the placement of the sensor monitor on the patient's body and indicia uniquely identifying the patient are provided to the electronic medical records with the samples of the electrocardiographic signals as certification.

10. A system according to claim 9, further comprising:
 the sealed housing further comprising indicia uniquely identifying the sealed housing,
 wherein the recording further comprises the indicia uniquely identifying the sealed housing.

11. A system according to claim 10, wherein the indicia uniquely identifying the sealed housing is selected from the group comprising visible indicia printed on the outside of the sealed housing, visible indicia applied to the outside of the sealed housing, and electronic indicia integrated into the sealed housing.

12. A system according to claim 7, further comprising:
 a recording feature comprised in the mobile device operable to record physical indicia proximal to the mobile device,
 wherein a recording of the placement of the sensor monitor on the patient's body and indicia uniquely identifying the patient are securely stored as part of the samples of the electrocardiographic signals as certification.

13. A system according to claim 12, further comprising:
 the sealed housing further comprising indicia uniquely identifying the sealed housing,
 wherein the recording further comprises the indicia uniquely identifying the sealed housing.

14. A system according to claim 13, wherein the indicia uniquely identifying the sealed housing is selected from the group comprising visible indicia printed on the outside of the sealed housing, visible indicia applied to the outside of the sealed housing, and electronic indicia integrated into the sealed housing.

15. A system according to claim 6, further comprising:
 a download station comprising:
 a non-conductive receptacle adapted to removably receive the sealed housing; and

25

a download station controller operable to retrieve the samples of the electrocardiographic signals; and
 a computer system operatively coupled to the download station controller and centrally accessible over a data communications network and operable to maintain the samples of the electrocardiographic signals upon retrieval.

16. A system according to claim 6, wherein a pair of the electrical contacts are connected to at least one of the micro-controller, the wireless transceiver, and the flash memory.

17. A system according to claim 1, the disposable extended wear electrode patch further comprising:

a flexible backing formed of an elongated strip of stretchable material with a narrow longitudinal midsection evenly tapering inward from both ends of the elongated strip and, on each end, a contact surface coated with an adhesive dressing only on each end provided as a crimp relief;

one of the electrocardiographic electrodes conductively exposed on the contact surface of each end of the elongated strip;

the non-conductive receptacle adhered to an outward-facing end of the elongated strip; and

26

the flexible circuit affixed on each end of the elongated strip and comprising a pair of circuit traces electrically coupled to the electrocardiographic electrodes and the electrical pads.

18. A system according to claim 1, wherein the activity tracker is selected from the group comprising a wearable physiology sensor, a wearable activity sensor, a smart watch, and a smartphone.

19. A system according to claim 1, further comprising at least one of:

a server computer system centrally accessible over a data communications network and operable to wirelessly interface with the wireless transceiver to receive samples of electrocardiographic signals; and

a client computer system interconnected to the data communications network and operable to wirelessly interface with the wireless transceiver to access the samples of the electrocardiographic signals.

20. A system according to claim 19, further comprising: a secure database interconnected to the data communications network and operable to maintain the samples of the electrocardiographic signals on behalf of one or more of the server computer system and the client computer system in the patient's electronic medical records.

* * * * *

专利名称(译)	用于提供个人移动设备触发的医疗干预的计算机实现的系统和方法		
公开(公告)号	US10165946	公开(公告)日	2019-01-01
申请号	US14/217402	申请日	2014-03-17
[标]申请(专利权)人(译)	BARDY诊断		
申请(专利权)人(译)	BARDY诊断, INC.		
当前申请(专利权)人(译)	BARDY诊断, INC.		
[标]发明人	BARDY GUST H FELIX JASON BISHAY JON MIKALSON		
发明人	BARDY, GUST H. FELIX, JASON BISHAY, JON MIKALSON		
IPC分类号	A61B5/02 A61B5/024 A61B5/0205 A61B5/00		
CPC分类号	A61B5/0022 A61B5/024 G16H40/63 A61B5/7282 G06F19/00 A61B5/0205 G06F19/3418		
审查员(译)	帕特尔NIKETA		
优先权	61/882403 2013-09-25 US		
其他公开文献	US20150088007A1		
外部链接	Espacenet		

摘要(译)

可以通过可穿戴式监视器提供生理监测，该监视器包括两个组件，一个灵活的扩展耐磨电极贴片和一个可拆卸的可重复使用的监视器记录器。可穿戴式监视器位于患者胸部的中央，沿着胸骨从上到下。将可穿戴式监视器放置在胸骨中线（或紧邻胸骨的任一侧）的位置，通过消除在整个监视期间将ECG电极连续放置在皮肤上的相同斑点中的要求，有利于延长佩戴。可穿戴式监视器可以与其他生理和活动传感器以及移动设备进行无线互操作。由传感器或设备执行的应用程序可以在检测到潜在的医学上重要的事件时触发将可穿戴监视器发送给患者。然后，调度的可穿戴监视器将能够提供精确的可医学操作的数据，而不仅仅是可能存在某些异常的警报。然后，患者可以使用传感器或设备物理地记录可医疗操作的可穿戴监视器的放置和使用，从而便于对所记录的数据进行认证。

