



US010201298B2

(12) **United States Patent**
Al-Ali et al.

(10) **Patent No.:** **US 10,201,298 B2**
(45) **Date of Patent:** ***Feb. 12, 2019**

(54) **NONINVASIVE OXIMETRY OPTICAL
SENSOR INCLUDING DISPOSABLE AND
REUSABLE ELEMENTS**

(71) Applicant: **MASIMO CORPORATION**, Irvine,
CA (US)

(72) Inventors: **Ammar Al-Ali**, San Juan Capistrano,
CA (US); **Yassir Abdul-Hafiz**, Irvine,
CA (US)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **15/642,162**

(22) Filed: **Jul. 5, 2017**

(65) **Prior Publication Data**

US 2017/0367632 A1 Dec. 28, 2017

Related U.S. Application Data

(63) Continuation of application No. 14/332,004, filed on
Jul. 15, 2014, now Pat. No. 9,693,719, which is a
continuation of application No. 13/585,669, filed on
Aug. 14, 2012, now Pat. No. 8,781,549, which is a
continuation of application No. 11/754,972, filed on
May 29, 2007, now Pat. No. 8,244,325, which is a
continuation of application No. 11/172,587, filed on
Jun. 30, 2005, now Pat. No. 7,225,007, which is a
continuation of application No. 10/351,645, filed on
Jan. 24, 2003, now Pat. No. 6,920,345.

(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 5/14552** (2013.01); **A61B 5/6826**
(2013.01); **A61B 5/6833** (2013.01); **A61B**
5/6838 (2013.01); **Y10T 29/49826** (2015.01)

(58) **Field of Classification Search**
CPC A61B 5/1455; A61B 5/14551; A61B
5/14552; A61B 5/6826; A61B 5/6833;
A61B 5/6838
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,960,128 A	10/1990	Gordon et al.
4,964,408 A	10/1990	Hink et al.
5,041,187 A	8/1991	Hink et al.
5,069,213 A	12/1991	Polczynski
5,163,438 A	11/1992	Gordon et al.
5,319,355 A	6/1994	Russek
5,337,744 A	8/1994	Branigan
5,341,805 A	8/1994	Stavridi et al.
D353,195 S	12/1994	Savage et al.
D353,196 S	12/1994	Savage et al.
5,377,676 A	1/1995	Vari et al.
D359,546 S	6/1995	Savage et al.

(Continued)


Primary Examiner — Eric Winakur

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson
& Bear, LLP

(57) **ABSTRACT**

A pulse oximetry sensor includes reusable and disposable
elements. To assemble the sensor, members of the reusable
element are mated with assembly mechanisms of the dis-
posable element. The assembled sensor provides indepen-
dent movement between the reusable and disposable ele-
ments.

19 Claims, 10 Drawing Sheets

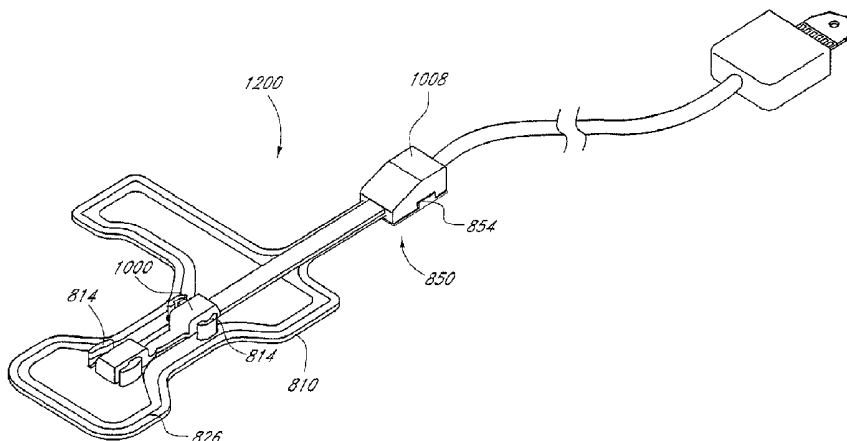

(56)

References Cited

U.S. PATENT DOCUMENTS

5,431,170	A	7/1995	Mathews	6,317,627	B1	11/2001	Ennen et al.
D361,840	S	8/1995	Savage et al.	6,321,100	B1	11/2001	Parker
D362,063	S	9/1995	Savage et al.	6,325,761	B1	12/2001	Jay
5,452,717	A	9/1995	Branigan et al.	6,334,065	B1	12/2001	Al-Ali et al.
D363,120	S	10/1995	Savage et al.	6,343,224	B1	1/2002	Parker
5,456,252	A	10/1995	Vari et al.	6,349,228	B1	2/2002	Kiani et al.
5,479,934	A	1/1996	Imran	6,360,114	B1	3/2002	Diab et al.
5,482,036	A	1/1996	Diab et al.	6,368,283	B1	4/2002	Xu et al.
5,490,505	A	2/1996	Diab et al.	6,371,921	B1	4/2002	Caro et al.
5,494,043	A	2/1996	O'Sullivan et al.	6,377,829	B1	4/2002	Al-Ali
5,533,511	A	7/1996	Kaspari et al.	6,388,240	B2	5/2002	Schulz et al.
5,534,851	A	7/1996	Russek	6,397,091	B2	5/2002	Diab et al.
5,561,275	A	10/1996	Savage et al.	6,430,437	B1	8/2002	Marro
5,562,002	A	10/1996	Lalin	6,430,525	B1	8/2002	Weber et al.
5,590,649	A	1/1997	Caro et al.	6,463,311	B1	10/2002	Diab
5,602,924	A	2/1997	Durand et al.	6,470,199	B1	10/2002	Kopotic et al.
5,632,272	A	5/1997	Diab et al.	6,501,975	B2	12/2002	Diab et al.
5,638,816	A	6/1997	Kiani-Azarbayjany et al.	6,505,059	B1	1/2003	Kollias et al.
5,638,818	A	6/1997	Diab et al.	6,515,273	B2	2/2003	Al-Ali
5,645,440	A	7/1997	Tobler et al.	6,519,487	B1	2/2003	Parker
5,685,299	A	11/1997	Diab et al.	6,525,386	B1	2/2003	Mills et al.
D393,830	S	4/1998	Tobler et al.	6,526,300	B1	2/2003	Kiani et al.
5,743,262	A	4/1998	Lepper, Jr. et al.	6,541,756	B2	4/2003	Schulz et al.
5,758,644	A	6/1998	Diab et al.	6,542,764	B1	4/2003	Al-Ali et al.
5,760,910	A	6/1998	Lepper, Jr. et al.	6,580,086	B1	6/2003	Schulz et al.
5,769,785	A	6/1998	Diab et al.	6,584,336	B1	6/2003	Ali et al.
5,782,757	A	7/1998	Diab et al.	6,595,316	B2	7/2003	Cybulski et al.
5,785,659	A	7/1998	Caro et al.	6,597,932	B2	7/2003	Tian et al.
5,791,347	A	8/1998	Flaherty et al.	6,597,933	B2	7/2003	Kiani et al.
5,810,734	A	9/1998	Caro et al.	6,606,511	B1	8/2003	Ali et al.
5,823,950	A	10/1998	Diab et al.	6,632,181	B2	10/2003	Flaherty et al.
5,830,131	A	11/1998	Caro et al.	6,639,668	B1	10/2003	Trepagnier
5,833,618	A	11/1998	Caro et al.	6,640,116	B2	10/2003	Diab
5,860,919	A	1/1999	Kiani-Azarbayjany et al.	6,643,530	B2	11/2003	Diab et al.
5,890,929	A	4/1999	Mills et al.	6,650,917	B2	11/2003	Diab et al.
5,904,654	A	5/1999	Wohltmann et al.	6,654,624	B2	11/2003	Diab et al.
5,919,134	A	7/1999	Diab	6,658,276	B2	12/2003	Kiani et al.
5,934,925	A	8/1999	Tobler et al.	6,661,161	B1	12/2003	Lanzo et al.
5,940,182	A	8/1999	Lepper, Jr. et al.	6,671,531	B2	12/2003	Al-Ali et al.
5,987,343	A	11/1999	Kinast	6,678,543	B2	1/2004	Diab et al.
5,995,855	A	11/1999	Kiani et al.	6,684,090	B2	1/2004	Ali et al.
5,997,343	A	12/1999	Mills et al.	6,684,091	B2	1/2004	Parker
6,002,952	A	12/1999	Diab et al.	6,697,656	B1	2/2004	Al-Ali
6,011,986	A	1/2000	Diab et al.	6,697,657	B1	2/2004	Shehada et al.
6,027,452	A	2/2000	Flaherty et al.	6,697,658	B2	2/2004	Al-Ali
6,036,642	A	3/2000	Diab et al.	RE38,476	E	3/2004	Diab et al.
6,045,509	A	4/2000	Caro et al.	6,699,194	B1	3/2004	Diab et al.
6,061,584	A *	5/2000	Lovejoy A61B 5/14552 600/310	6,714,804	B2	3/2004	Al-Ali et al.
6,067,462	A	5/2000	Diab et al.	RE38,492	E	4/2004	Diab et al.
6,081,735	A	6/2000	Diab et al.	6,721,582	B2	4/2004	Trepagnier et al.
6,088,607	A	7/2000	Diab et al.	6,721,585	B1	4/2004	Parker
6,110,522	A	8/2000	Lepper, Jr. et al.	6,725,075	B2	4/2004	Al-Ali
6,124,597	A	9/2000	Shehada	6,728,560	B2	4/2004	Kollias et al.
6,128,521	A	10/2000	Marro et al.	6,735,459	B2	5/2004	Parker
6,129,675	A	10/2000	Jay	6,745,060	B2	6/2004	Diab et al.
6,144,868	A	11/2000	Parker	6,760,607	B2	7/2004	Al-Ali
6,151,516	A	11/2000	Kiani-Azarbayjany et al.	6,770,028	B1	8/2004	Ali et al.
6,152,754	A	11/2000	Gerhardt et al.	6,771,994	B2	8/2004	Kiani et al.
6,157,850	A	12/2000	Diab et al.	6,792,300	B1	9/2004	Diab et al.
6,165,005	A	12/2000	Mills et al.	6,813,511	B2	11/2004	Diab et al.
6,184,521	B1	2/2001	Coffin, IV et al.	6,816,741	B2	11/2004	Diab
6,206,830	B1	3/2001	Diab et al.	6,822,564	B2	11/2004	Al-Ali
6,229,856	B1	5/2001	Diab et al.	6,826,419	B2	11/2004	Diab et al.
6,232,609	B1	5/2001	Snyder et al.	6,830,711	B2	12/2004	Mills et al.
6,236,872	B1	5/2001	Diab et al.	6,850,787	B2	2/2005	Weber et al.
6,241,683	B1	6/2001	Macklem et al.	6,850,788	B2	2/2005	Al-Ali
6,253,097	B1	6/2001	Aronow et al.	6,852,083	B2	2/2005	Caro et al.
6,256,523	B1	7/2001	Diab et al.	6,861,639	B2	3/2005	Al-Ali
6,263,222	B1	7/2001	Diab et al.	6,898,452	B2	5/2005	Al-Ali et al.
6,278,522	B1	8/2001	Lepper, Jr. et al.	6,920,345	B2	7/2005	Al-Ali et al.
6,280,213	B1	8/2001	Tobler et al.	6,931,268	B1	8/2005	Kiani-Azarbayjany et al.
6,285,896	B1	9/2001	Tobler et al.	6,934,570	B2	8/2005	Kiani et al.
6,301,493	B1	10/2001	Marro et al.	6,939,305	B2	9/2005	Flaherty et al.
6,308,089	B1	10/2001	von der Ruhr et al.	6,943,348	B1	9/2005	Coffin, IV
				6,950,687	B2	9/2005	Al-Ali
				6,961,598	B2	11/2005	Diab
				6,970,792	B1	11/2005	Diab
				6,979,812	B2	12/2005	Al-Ali
				6,985,764	B2	1/2006	Mason et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,993,371 B2	1/2006	Kiani et al.	7,510,849 B2	3/2009	Schurman et al.
6,996,427 B2	2/2006	Ali et al.	7,526,328 B2	4/2009	Diab et al.
6,999,904 B2	2/2006	Weber et al.	7,530,942 B1	5/2009	Diab
7,003,338 B2	2/2006	Weber et al.	7,530,949 B2	5/2009	Al Ali et al.
7,003,339 B2	2/2006	Diab et al.	7,530,955 B2	5/2009	Diab et al.
7,015,451 B2	3/2006	Dalke et al.	7,563,110 B2	7/2009	Al-Ali et al.
7,024,233 B2	4/2006	Ali et al.	7,596,398 B2	9/2009	Al-Ali et al.
7,027,849 B2	4/2006	Al-Ali	7,618,375 B2	11/2009	Flaherty
7,030,749 B2	4/2006	Al-Ali	D606,659 S	12/2009	Kiani et al.
7,039,449 B2	5/2006	Al-Ali	7,647,083 B2	1/2010	Al-Ali et al.
7,041,060 B2	5/2006	Flaherty et al.	D609,193 S	2/2010	Al-Ali et al.
7,044,918 B2	5/2006	Diab	D614,305 S	4/2010	Al-Ali et al.
7,048,687 B1	5/2006	Reuss et al.	RE41,317 E	5/2010	Parker
7,067,893 B2	6/2006	Mills et al.	7,729,733 B2	6/2010	Al-Ali et al.
7,096,052 B2	8/2006	Mason et al.	7,734,320 B2	6/2010	Al-Ali
7,096,054 B2	8/2006	Abdul-Hafiz et al.	7,761,127 B2	7/2010	Al-Ali et al.
7,132,641 B2	11/2006	Schulz et al.	7,761,128 B2	7/2010	Al-Ali et al.
7,142,901 B2	11/2006	Kiani et al.	7,764,982 B2	7/2010	Dalke et al.
7,149,561 B2	12/2006	Diab	D621,516 S	8/2010	Kiani et al.
7,186,966 B2	3/2007	Al-Ali	7,791,155 B2	9/2010	Diab
7,190,261 B2	3/2007	Al-Ali	7,801,581 B2	9/2010	Diab
7,215,984 B2	5/2007	Diab	7,822,452 B2	10/2010	Schurman et al.
7,215,986 B2	5/2007	Diab	RE41,912 E	11/2010	Parker
7,221,971 B2	5/2007	Diab	7,844,313 B2	11/2010	Kiani et al.
7,225,006 B2	5/2007	Al-Ali et al.	7,844,314 B2	11/2010	Al-Ali
7,225,007 B2	5/2007	Al-Ali	7,844,315 B2	11/2010	Al-Ali
RE39,672 E	6/2007	Shehada et al.	7,865,222 B2	1/2011	Weber et al.
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	7,873,497 B2	1/2011	Weber et al.
7,245,953 B1	7/2007	Parker	7,880,606 B2	2/2011	Al-Ali
7,254,429 B2	8/2007	Schurman et al.	7,880,626 B2	2/2011	Al-Ali et al.
7,254,431 B2	8/2007	Al-Ali	7,891,355 B2	2/2011	Al-Ali et al.
7,254,433 B2	8/2007	Diab et al.	7,894,868 B2	2/2011	Al-Ali et al.
7,254,434 B2	8/2007	Schulz et al.	7,899,507 B2	3/2011	Al-Ali et al.
7,272,425 B2	9/2007	Al-Ali	7,899,518 B2	3/2011	Trepagnier et al.
7,274,955 B2	9/2007	Kiani et al.	7,904,132 B2	3/2011	Weber et al.
D554,263 S	10/2007	Al-Ali	7,909,772 B2	3/2011	Popov et al.
7,280,858 B2	10/2007	Al-Ali et al.	7,910,875 B2	3/2011	Al-Ali
7,289,835 B2	10/2007	Mansfield et al.	7,919,713 B2	4/2011	Al-Ali et al.
7,292,883 B2	11/2007	De Felice et al.	7,937,128 B2	5/2011	Al-Ali
7,295,866 B2	11/2007	Al-Ali	7,937,129 B2	5/2011	Mason et al.
7,328,053 B1	2/2008	Diab et al.	7,937,130 B2	5/2011	Diab et al.
7,332,784 B2	2/2008	Mills et al.	7,941,199 B2	5/2011	Kiani
7,340,287 B2	3/2008	Mason et al.	7,951,086 B2	5/2011	Flaherty et al.
7,341,559 B2	3/2008	Schulz et al.	7,957,780 B2	6/2011	Lamego et al.
7,343,186 B2	3/2008	Lamego et al.	7,962,188 B2	6/2011	Kiani et al.
D566,282 S	4/2008	Al-Ali et al.	7,962,190 B1	6/2011	Diab et al.
7,355,512 B1	4/2008	Al-Ali	7,976,472 B2	7/2011	Kiani
7,356,365 B2	4/2008	Schurman	7,988,637 B2	8/2011	Diab
7,371,981 B2	5/2008	Abdul-Hafiz	7,990,382 B2	8/2011	Kiani
7,373,193 B2	5/2008	Al-Ali et al.	7,991,446 B2	8/2011	Ali et al.
7,373,194 B2	5/2008	Weber et al.	8,000,761 B2	8/2011	Al-Ali
7,376,453 B1	5/2008	Diab et al.	8,008,088 B2	8/2011	Bellott et al.
7,377,794 B2	5/2008	Al Ali et al.	RE42,753 E	9/2011	Kiani-Azarbayjany et al.
7,377,899 B2	5/2008	Weber et al.	8,019,400 B2	9/2011	Diab et al.
7,383,070 B2	6/2008	Diab et al.	8,028,701 B2	10/2011	Al-Ali et al.
7,415,297 B2	8/2008	Al-Ali et al.	8,029,765 B2	10/2011	Bellott et al.
7,428,432 B2	9/2008	Ali et al.	8,036,727 B2	10/2011	Schurman et al.
7,438,683 B2	10/2008	Al-Ali et al.	8,036,728 B2	10/2011	Diab et al.
7,440,787 B2	10/2008	Diab	8,046,040 B2	10/2011	Ali et al.
7,454,240 B2	11/2008	Diab et al.	8,046,041 B2	10/2011	Diab et al.
7,467,002 B2	12/2008	Weber et al.	8,046,042 B2	10/2011	Diab et al.
7,469,157 B2	12/2008	Diab et al.	8,048,040 B2	11/2011	Kiani
7,471,969 B2	12/2008	Diab et al.	8,050,728 B2	11/2011	Al-Ali et al.
7,471,971 B2	12/2008	Diab et al.	RE43,169 E	2/2012	Parker
7,483,729 B2	1/2009	Al-Ali et al.	8,118,620 B2	2/2012	Al-Ali et al.
7,483,730 B2	1/2009	Diab et al.	8,126,528 B2	2/2012	Diab et al.
7,489,958 B2	2/2009	Diab et al.	8,128,572 B2	3/2012	Diab et al.
7,496,391 B2	2/2009	Diab et al.	8,130,105 B2	3/2012	Al-Ali et al.
7,496,393 B2	2/2009	Diab et al.	8,145,287 B2	3/2012	Diab et al.
D587,657 S	3/2009	Al-Ali et al.	8,150,487 B2	4/2012	Diab et al.
7,499,741 B2	3/2009	Diab et al.	8,175,672 B2	5/2012	Parker
7,499,835 B2	3/2009	Weber et al.	8,180,420 B2	5/2012	Diab et al.
7,500,950 B2	3/2009	Al-Ali et al.	8,182,443 B1	5/2012	Kiani
7,509,154 B2	3/2009	Diab et al.	8,185,180 B2	5/2012	Diab et al.
7,509,494 B2	3/2009	Al-Ali	8,190,223 B2	5/2012	Al-Ali et al.
			8,190,227 B2	5/2012	Diab et al.
			8,203,438 B2	6/2012	Kiani et al.
			8,203,704 B2	6/2012	Merritt et al.
			8,204,566 B2	6/2012	Schurman et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,219,172 B2	7/2012	Schurman et al.	8,634,889 B2	1/2014	Al-Ali et al.
8,224,411 B2	7/2012	Al-Ali et al.	8,641,631 B2	2/2014	Sierra et al.
8,228,181 B2	7/2012	Al-Ali	8,652,060 B2	2/2014	Al-Ali
8,229,533 B2	7/2012	Diab et al.	8,663,107 B2	3/2014	Kiani
8,233,955 B2	7/2012	Al-Ali et al.	8,666,468 B1	3/2014	Al-Ali
8,244,325 B2	8/2012	Al-Ali et al.	8,667,967 B2	3/2014	Al-Ali et al.
8,255,026 B1	8/2012	Al-Ali	8,670,811 B2	3/2014	O'Reilly
8,255,027 B2	8/2012	Al-Ali et al.	8,670,814 B2	3/2014	Diab et al.
8,255,028 B2	8/2012	Al-Ali et al.	8,676,286 B2	3/2014	Weber et al.
8,260,577 B2	9/2012	Weber et al.	8,682,407 B2	3/2014	Al-Ali
8,265,723 B1	9/2012	McHale et al.	RE44,823 E	4/2014	Parker
8,274,360 B2	9/2012	Sampath et al.	RE44,875 E	4/2014	Kiani et al.
8,280,473 B2	10/2012	Al-Ali	8,690,799 B2	4/2014	Telfort et al.
8,301,217 B2	10/2012	Al-Ali et al.	8,700,112 B2	4/2014	Kiani
8,306,596 B2	11/2012	Schurman et al.	8,702,627 B2	4/2014	Telfort et al.
8,310,336 B2	11/2012	Muhsin et al.	8,706,179 B2	4/2014	Parker
8,315,683 B2	11/2012	Al-Ali et al.	8,712,494 B1	4/2014	MacNeish, III et al.
RE43,860 E	12/2012	Parker	8,715,206 B2	5/2014	Telfort et al.
8,337,403 B2	12/2012	Al-Ali et al.	8,718,735 B2	5/2014	Lamego et al.
8,346,330 B2	1/2013	Lamego	8,718,737 B2	5/2014	Diab et al.
8,353,842 B2	1/2013	Al-Ali et al.	8,718,738 B2	5/2014	Blank et al.
8,355,766 B2	1/2013	MacNeish, III et al.	8,720,249 B2	5/2014	Al-Ali
8,359,080 B2	1/2013	Diab et al.	8,721,541 B2	5/2014	Al-Ali et al.
8,364,223 B2	1/2013	Al-Ali et al.	8,721,542 B2	5/2014	Al-Ali et al.
8,364,226 B2	1/2013	Diab et al.	8,723,677 B1	5/2014	Kiani
8,374,665 B2	2/2013	Lamego	8,740,792 B1	6/2014	Kiani et al.
8,385,995 B2	2/2013	Al-Ali et al.	8,754,776 B2	6/2014	Poeze et al.
8,385,996 B2	2/2013	Smith et al.	8,755,535 B2	6/2014	Telfort et al.
8,388,353 B2	3/2013	Kiani et al.	8,755,856 B2	6/2014	Diab et al.
8,399,822 B2	3/2013	Al-Ali	8,755,872 B1	6/2014	Marinow
8,401,602 B2	3/2013	Kiani	8,761,850 B2	6/2014	Lamego
8,405,608 B2	3/2013	Al-Ali et al.	8,764,671 B2	7/2014	Kiani
8,414,499 B2	4/2013	Al-Ali et al.	8,768,423 B2	7/2014	Shakespeare et al.
8,418,524 B2	4/2013	Al-Ali	8,771,204 B2	7/2014	Telfort et al.
8,423,106 B2	4/2013	Lamego et al.	8,777,634 B2	7/2014	Kiani et al.
8,428,967 B2	4/2013	Olsen et al.	8,781,543 B2	7/2014	Diab et al.
8,430,817 B1	4/2013	Al-Ali et al.	8,781,544 B2	7/2014	Al-Ali et al.
8,437,825 B2	5/2013	Dalvi et al.	8,781,549 B2	7/2014	Al-Ali et al.
8,455,290 B2	6/2013	Siskavich	8,788,003 B2	7/2014	Schurman et al.
8,457,703 B2	6/2013	Al-Ali	8,790,268 B2	7/2014	Al-Ali
8,457,707 B2	6/2013	Kiani	8,801,613 B2	8/2014	Al-Ali et al.
8,463,349 B2	6/2013	Diab et al.	8,821,397 B2	9/2014	Al-Ali et al.
8,466,286 B2	6/2013	Bellot et al.	8,821,415 B2	9/2014	Al-Ali et al.
8,471,713 B2	6/2013	Poeze et al.	8,830,449 B1	9/2014	Lamego et al.
8,473,020 B2	6/2013	Kiani et al.	8,831,700 B2	9/2014	Schurman et al.
8,483,787 B2	7/2013	Al-Ali et al.	8,840,549 B2	9/2014	Al-Ali et al.
8,489,364 B2	7/2013	Weber et al.	8,847,740 B2	9/2014	Kiani et al.
8,498,684 B2	7/2013	Weber et al.	8,849,365 B2	9/2014	Smith et al.
8,504,128 B2	8/2013	Blank et al.	8,852,094 B2	10/2014	Al-Ali et al.
8,509,867 B2	8/2013	Workman et al.	8,852,994 B2	10/2014	Wojtczuk et al.
8,515,509 B2	8/2013	Bruinsma et al.	8,868,147 B2	10/2014	Stippick et al.
8,523,781 B2	9/2013	Al-Ali	8,868,150 B2	10/2014	Al-Ali et al.
8,529,301 B2	9/2013	Al-Ali et al.	8,870,792 B2	10/2014	Al-Ali et al.
8,532,727 B2	9/2013	Ali et al.	8,886,271 B2	11/2014	Kiani et al.
8,532,728 B2	9/2013	Diab et al.	8,888,539 B2	11/2014	Al-Ali et al.
D692,145 S	10/2013	Al-Ali et al.	8,888,708 B2	11/2014	Diab et al.
8,547,209 B2	10/2013	Kiani et al.	8,892,180 B2	11/2014	Weber et al.
8,548,548 B2	10/2013	Al-Ali	8,897,847 B2	11/2014	Al-Ali
8,548,549 B2	10/2013	Schurman et al.	8,909,310 B2	12/2014	Lamego et al.
8,548,550 B2	10/2013	Al-Ali et al.	8,911,377 B2	12/2014	Al-Ali
8,560,032 B2	10/2013	Al-Ali et al.	8,912,909 B2	12/2014	Al-Ali et al.
8,560,034 B1	10/2013	Diab et al.	8,920,317 B2	12/2014	Al-Ali et al.
8,570,167 B2	10/2013	Al-Ali	8,921,699 B2	12/2014	Al-Ali et al.
8,570,503 B2	10/2013	Vo et al.	8,922,382 B2	12/2014	Al-Ali et al.
8,571,617 B2	10/2013	Reichgott et al.	8,929,964 B2	1/2015	Al-Ali et al.
8,571,618 B1	10/2013	Lamego et al.	8,942,777 B2	1/2015	Diab et al.
8,571,619 B2	10/2013	Al-Ali et al.	8,948,834 B2	2/2015	Diab et al.
8,577,431 B2	11/2013	Lamego et al.	8,948,835 B2	2/2015	Diab
8,581,732 B2	11/2013	Al-Ali et al.	8,965,471 B2	2/2015	Lamego
8,584,345 B2	11/2013	Al-Ali et al.	8,983,564 B2	3/2015	Al-Ali
8,588,880 B2	11/2013	Abdul-Hafiz et al.	8,989,831 B2	3/2015	Al-Ali et al.
8,600,467 B2	12/2013	Al-Ali et al.	8,996,085 B2	3/2015	Kiani et al.
8,606,342 B2	12/2013	Diab	8,998,809 B2	4/2015	Kiani
8,626,255 B2	1/2014	Al-Ali et al.	9,028,429 B2	5/2015	Telfort et al.
8,630,691 B2	1/2014	Lamego et al.	9,037,207 B2	5/2015	Al-Ali et al.
			9,060,721 B2	6/2015	Reichgott et al.
			9,066,666 B2	6/2015	Kiani
			9,066,680 B1	6/2015	Al-Ali et al.
			9,072,474 B2	7/2015	Al-Ali et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,078,560 B2	7/2015	Schurman et al.	9,566,019 B2	2/2017	Al-Ali et al.
9,084,569 B2	7/2015	Weber et al.	9,579,039 B2	2/2017	Jansen et al.
9,095,316 B2	8/2015	Welch et al.	9,591,975 B2	3/2017	Dalvi et al.
9,106,038 B2	8/2015	Telfort et al.	9,622,692 B2	4/2017	Lamego et al.
9,107,625 B2	8/2015	Telfort et al.	9,622,693 B2	4/2017	Diab
9,107,626 B2	8/2015	Al-Ali et al.	D788,312 S	5/2017	Al-Ali et al.
9,113,831 B2	8/2015	Al-Ali	9,636,055 B2	5/2017	Al-Ali et al.
9,113,832 B2	8/2015	Al-Ali	9,636,056 B2	5/2017	Al-Ali
9,119,595 B2	9/2015	Lamego	9,649,054 B2	5/2017	Lamego et al.
9,131,881 B2	9/2015	Diab et al.	9,662,052 B2	5/2017	Al-Ali et al.
9,131,882 B2	9/2015	Al-Ali et al.	9,668,679 B2	6/2017	Schurman et al.
9,131,883 B2	9/2015	Al-Ali	9,668,680 B2	6/2017	Bruinsma et al.
9,131,917 B2	9/2015	Telfort et al.	9,668,703 B2	6/2017	Al-Ali
9,138,180 B1	9/2015	Coverston et al.	9,675,286 B2	6/2017	Diab
9,138,182 B2	9/2015	Al-Ali et al.	9,687,160 B2	6/2017	Kiani
9,138,192 B2	9/2015	Weber et al.	9,693,719 B2	7/2017	Al-Ali et al.
9,142,117 B2	9/2015	Muhsin et al.	9,693,737 B2	7/2017	Al-Ali
9,153,112 B1	10/2015	Kiani et al.	9,697,928 B2	7/2017	Al-Ali et al.
9,153,121 B2	10/2015	Kiani et al.	9,717,425 B2	8/2017	Kiani et al.
9,161,696 B2	10/2015	Al-Ali et al.	9,717,458 B2	8/2017	Lamego et al.
9,161,713 B2	10/2015	Al-Ali et al.	9,724,016 B1	8/2017	Al-Ali et al.
9,167,995 B2	10/2015	Lamego et al.	9,724,024 B2	8/2017	Al-Ali
9,176,141 B2	11/2015	Al-Ali et al.	9,724,025 B1	8/2017	Kiani et al.
9,186,102 B2	11/2015	Bruinsma et al.	9,730,640 B2	8/2017	Diab et al.
9,192,312 B2	11/2015	Al-Ali	9,743,887 B2	8/2017	Al-Ali et al.
9,192,329 B2	11/2015	Al-Ali	9,749,232 B2	8/2017	Sampath et al.
9,192,351 B1	11/2015	Telfort et al.	9,750,442 B2	9/2017	Olsen
9,195,385 B2	11/2015	Al-Ali et al.	9,750,443 B2	9/2017	Smith et al.
9,211,072 B2	12/2015	Kiani	9,750,461 B1	9/2017	Telfort
9,211,095 B1	12/2015	Al-Ali	9,775,545 B2	10/2017	Al-Ali et al.
9,218,454 B2	12/2015	Kiani et al.	9,775,546 B2	10/2017	Diab et al.
9,226,696 B2	1/2016	Kiani	9,775,570 B2	10/2017	Al-Ali
9,241,662 B2	1/2016	Al-Ali et al.	9,778,079 B1	10/2017	Al-Ali et al.
9,245,668 B1	1/2016	Vo et al.	9,782,077 B2	10/2017	Lamego et al.
9,259,185 B2	2/2016	Abdul-Hafiz et al.	9,782,110 B2	10/2017	Kiani
9,267,572 B2	2/2016	Barker et al.	9,787,568 B2	10/2017	Lamego et al.
9,277,880 B2	3/2016	Poeze et al.	9,788,735 B2	10/2017	Al-Ali
9,289,167 B2	3/2016	Diab et al.	9,788,768 B2	10/2017	Al-Ali et al.
9,295,421 B2	3/2016	Kiani et al.	9,795,300 B2	10/2017	Al-Ali
9,307,928 B1	4/2016	Al-Ali et al.	9,795,310 B2	10/2017	Al-Ali
9,323,894 B2	4/2016	Kiani	9,795,358 B2	10/2017	Telfort et al.
D755,392 S	5/2016	Hwang et al.	9,795,739 B2	10/2017	Al-Ali et al.
9,326,712 B1	5/2016	Kiani	9,801,556 B2	10/2017	Kiani
9,333,316 B2	5/2016	Kiani	9,801,588 B2	10/2017	Weber et al.
9,339,220 B2	5/2016	Lamego et al.	9,808,188 B1	11/2017	Perea et al.
9,341,565 B2	5/2016	Lamego et al.	9,814,418 B2	11/2017	Weber et al.
9,351,673 B2	5/2016	Diab et al.	9,820,691 B2	11/2017	Kiani
9,351,675 B2	5/2016	Al-Ali et al.	9,833,152 B2	12/2017	Kiani et al.
9,364,181 B2	6/2016	Kiani et al.	9,833,180 B2	12/2017	Shakespeare et al.
9,368,671 B2	6/2016	Wojtczuk et al.	9,839,379 B2	12/2017	Al-Ali et al.
9,370,325 B2	6/2016	Al-Ali et al.	9,839,381 B1	12/2017	Weber et al.
9,370,326 B2	6/2016	McHale et al.	9,847,002 B2	12/2017	Kiani et al.
9,370,335 B2	6/2016	Al-Ali et al.	9,847,749 B2	12/2017	Kiani et al.
9,375,185 B2	6/2016	Ali et al.	9,848,800 B1	12/2017	Lee et al.
9,386,953 B2	7/2016	Al-Ali	9,848,806 B2	12/2017	Al-Ali et al.
9,386,961 B2	7/2016	Al-Ali et al.	9,848,807 B2	12/2017	Lamego
9,392,945 B2	7/2016	Al-Ali et al.	9,861,298 B2	1/2018	Eckerbom et al.
9,397,448 B2	7/2016	Al-Ali et al.	9,861,304 B2	1/2018	Al-Ali et al.
9,408,542 B1	8/2016	Kinast et al.	9,861,305 B1	1/2018	Weber et al.
9,436,645 B2	9/2016	Al-Ali et al.	9,867,578 B2	1/2018	Al-Ali et al.
9,445,759 B1	9/2016	Lamego et al.	9,872,623 B2	1/2018	Al-Ali
9,466,919 B2	10/2016	Kiani et al.	9,876,320 B2	1/2018	Coverston et al.
9,474,474 B2	10/2016	Lamego et al.	9,877,650 B2	1/2018	Muhsin et al.
9,480,422 B2	11/2016	Al-Ali	9,877,686 B2	1/2018	Al-Ali et al.
9,480,435 B2	11/2016	Olsen	9,891,079 B2	2/2018	Dalvi
9,492,110 B2	11/2016	Al-Ali et al.	9,895,107 B2	2/2018	Al-Ali et al.
9,510,779 B2	12/2016	Poeze et al.	9,924,893 B2	3/2018	Schurman et al.
9,517,024 B2	12/2016	Kiani et al.	9,924,897 B1	3/2018	Abdul-Hafiz
9,532,722 B2	1/2017	Lamego et al.	2006/0161054 A1	7/2006	Reuss et al.
9,538,949 B2	1/2017	Al-Ali et al.	2007/0282478 A1	12/2007	Al-Ali et al.
9,538,980 B2	1/2017	Telfort et al.	2009/0247984 A1	10/2009	Lamego et al.
9,549,696 B2	1/2017	Lamego et al.	2009/0275813 A1	11/2009	Davis
9,554,737 B2	1/2017	Schurman et al.	2009/0275844 A1	11/2009	Al-Ali
9,560,996 B2	2/2017	Kiani	2010/0004518 A1	1/2010	Vo et al.
9,560,998 B2	2/2017	Al-Ali et al.	2010/0030040 A1	2/2010	Poeze et al.
			2011/0082711 A1	4/2011	Poeze et al.
			2011/0105854 A1	5/2011	Kiani et al.
			2011/0125060 A1	5/2011	Telfort et al.
			2011/0208015 A1	8/2011	Welch et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0230733	A1	9/2011	Al-Ali	2016/0029932	A1	2/2016	Al-Ali
2012/0165629	A1	6/2012	Merritt et al.	2016/0058347	A1	3/2016	Reichgott et al.
2012/0209082	A1	8/2012	Al-Ali	2016/0066824	A1	3/2016	Al-Ali et al.
2012/0209084	A1	8/2012	Olsen et al.	2016/0081552	A1	3/2016	Wojtczuk et al.
2012/0283524	A1	11/2012	Kiani et al.	2016/0095543	A1	4/2016	Telfort et al.
2012/0319816	A1	12/2012	Al-Ali	2016/0095548	A1	4/2016	Al-Ali et al.
2013/0023775	A1	1/2013	Lamego et al.	2016/0103598	A1	4/2016	Al-Ali et al.
2013/0041591	A1	2/2013	Lamego	2016/0143548	A1	5/2016	Al-Ali
2013/0060147	A1	3/2013	Welch et al.	2016/0166182	A1	6/2016	Al-Ali et al.
2013/0096405	A1	4/2013	Garfio	2016/0166183	A1	6/2016	Poeze et al.
2013/0096936	A1	4/2013	Sampath et al.	2016/0192869	A1	7/2016	Kiani et al.
2013/0243021	A1	9/2013	Siskavich	2016/0196388	A1	7/2016	Lamego
2013/0253334	A1	9/2013	Al-Ali et al.	2016/0197436	A1	7/2016	Barker et al.
2013/0296672	A1	11/2013	O'Neil et al.	2016/0213281	A1	7/2016	Eckerbom et al.
2013/0296713	A1	11/2013	Al-Ali et al.	2016/0228043	A1	8/2016	O'Neil et al.
2013/0324808	A1	12/2013	Al-Ali et al.	2016/0233632	A1	8/2016	Scruggs et al.
2013/0331660	A1	12/2013	Al-Ali et al.	2016/0234944	A1	8/2016	Schmidt et al.
2014/0012100	A1	1/2014	Al-Ali et al.	2016/0270735	A1	9/2016	Diab et al.
2014/0051953	A1	2/2014	Lamego et al.	2016/0283665	A1	9/2016	Sampath et al.
2014/0081175	A1	3/2014	Telfort	2016/0287090	A1	10/2016	Al-Ali et al.
2014/0120564	A1	5/2014	Workman et al.	2016/0287786	A1	10/2016	Kiani
2014/0121482	A1	5/2014	Merritt et al.	2016/0296169	A1	10/2016	McHale et al.
2014/0127137	A1	5/2014	Bellott et al.	2016/0310052	A1	10/2016	Al-Ali et al.
2014/0135588	A1	5/2014	Al-Ali et al.	2016/0314260	A1	10/2016	Kiani
2014/0163344	A1	6/2014	Al-Ali	2016/0324486	A1	11/2016	Al-Ali et al.
2014/0163402	A1	6/2014	Lamego et al.	2016/0324488	A1	11/2016	Olsen
2014/0166076	A1	6/2014	Kiani et al.	2016/0327984	A1	11/2016	Al-Ali et al.
2014/0171763	A1	6/2014	Diab	2016/0328528	A1	11/2016	Al-Ali et al.
2014/0180038	A1	6/2014	Kiani	2016/0331332	A1	11/2016	Al-Ali
2014/0180154	A1	6/2014	Sierra et al.	2016/0367173	A1	12/2016	Dalvi et al.
2014/0180160	A1	6/2014	Brown et al.	2017/0000394	A1	1/2017	Al-Ali et al.
2014/0187973	A1	7/2014	Brown et al.	2017/0007134	A1	1/2017	Al-Ali et al.
2014/0213864	A1	7/2014	Abdul-Hafiz et al.	2017/0007198	A1	1/2017	Al-Ali et al.
2014/0266790	A1	9/2014	Al-Ali et al.	2017/0014083	A1	1/2017	Diab et al.
2014/0275808	A1	9/2014	Poeze et al.	2017/0014084	A1	1/2017	Al-Ali et al.
2014/0275835	A1	9/2014	Lamego et al.	2017/0027456	A1	2/2017	Kinast et al.
2014/0275871	A1	9/2014	Lamego et al.	2017/0042488	A1	2/2017	Muhsin
2014/0275872	A1	9/2014	Merritt et al.	2017/0055851	A1	3/2017	Al-Ali
2014/0276115	A1	9/2014	Dalvi et al.	2017/0055882	A1	3/2017	Al-Ali et al.
2014/0288400	A1	9/2014	Diab et al.	2017/0055887	A1	3/2017	Al-Ali
2014/0316217	A1	10/2014	Purdon et al.	2017/0055896	A1	3/2017	Al-Ali et al.
2014/0316218	A1	10/2014	Purdon et al.	2017/0079594	A1	3/2017	Telfort et al.
2014/0316228	A1	10/2014	Blank et al.	2017/0086723	A1	3/2017	Al-Ali et al.
2014/0323825	A1	10/2014	Al-Ali et al.	2017/0143281	A1	5/2017	Olsen
2014/0323897	A1	10/2014	Brown et al.	2017/0147774	A1	5/2017	Kiani
2014/0323898	A1	10/2014	Purdon et al.	2017/0156620	A1	6/2017	Al-Ali et al.
2014/0330092	A1	11/2014	Al-Ali et al.	2017/0173632	A1	6/2017	Al-Ali
2014/0330098	A1	11/2014	Merritt et al.	2017/0187146	A1	6/2017	Kiani et al.
2014/0357966	A1	12/2014	Al-Ali et al.	2017/0188919	A1	7/2017	Al-Ali et al.
2015/0005600	A1	1/2015	Blank et al.	2017/0196464	A1	7/2017	Jansen et al.
2015/0011907	A1	1/2015	Purdon et al.	2017/0196470	A1	7/2017	Lamego et al.
2015/0012231	A1	1/2015	Poeze et al.	2017/0202490	A1	7/2017	Al-Ali et al.
2015/0032029	A1	1/2015	Al-Ali et al.	2017/0224262	A1	8/2017	Al-Ali
2015/0038859	A1	2/2015	Dalvi et al.	2017/0228516	A1	8/2017	Sampath et al.
2015/0080754	A1	3/2015	Purdon et al.	2017/0245790	A1	8/2017	Al-Ali et al.
2015/0087936	A1	3/2015	Al-Ali et al.	2017/0251974	A1	9/2017	Shreim et al.
2015/0094546	A1	4/2015	Al-Ali	2017/0251975	A1	9/2017	Shreim et al.
2015/0097701	A1	4/2015	Al-Ali et al.	2017/0258403	A1	9/2017	Abdul-Hafiz et al.
2015/0099950	A1	4/2015	Al-Ali et al.	2017/0311891	A1	11/2017	Kiani et al.
2015/0099955	A1	4/2015	Al-Ali et al.	2017/0325728	A1	11/2017	Al-Ali et al.
2015/0101844	A1	4/2015	Al-Ali et al.	2017/0332976	A1	11/2017	Al-Ali et al.
2015/0106121	A1	4/2015	Muhsin et al.	2017/0340293	A1	11/2017	Al-Ali et al.
2015/0112151	A1	4/2015	Muhsin et al.	2017/0360310	A1	12/2017	Kiani et al.
2015/0116076	A1	4/2015	Al-Ali et al.	2017/0367632	A1	12/2017	Al-Ali et al.
2015/0165312	A1	6/2015	Kiani	2018/0008146	A1	1/2018	Al-Ali et al.
2015/0196249	A1	7/2015	Brown et al.	2018/0014752	A1	1/2018	Al-Ali et al.
2015/0216459	A1	8/2015	Al-Ali et al.	2018/0028124	A1	2/2018	Al-Ali et al.
2015/0238722	A1	8/2015	Al-Ali	2018/0055385	A1	3/2018	Al-Ali
2015/0245773	A1	9/2015	Lamego et al.	2018/0055390	A1	3/2018	Kiani et al.
2015/0245794	A1	9/2015	Al-Ali	2018/0055430	A1	3/2018	Diab et al.
2015/0257689	A1	9/2015	Al-Ali et al.	2018/0064381	A1	3/2018	Shakespeare et al.
2015/0272514	A1	10/2015	Kiani et al.	2018/0069776	A1	3/2018	Lamego et al.
2015/0351697	A1	12/2015	Weber et al.	2018/0103874	A1	4/2018	Lee et al.
2015/0359429	A1	12/2015	Al-Ali et al.	2018/0116575	A1	5/2018	Perea et al.
2015/0366507	A1	12/2015	Blank	2018/0125368	A1	5/2018	Lamego et al.
				2018/0125430	A1	5/2018	Al-Ali et al.
				2018/0130325	A1	5/2018	Kiani et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2018/0132769 A1 5/2018 Weber et al.
2018/0132770 A1 5/2018 Lamego

* cited by examiner

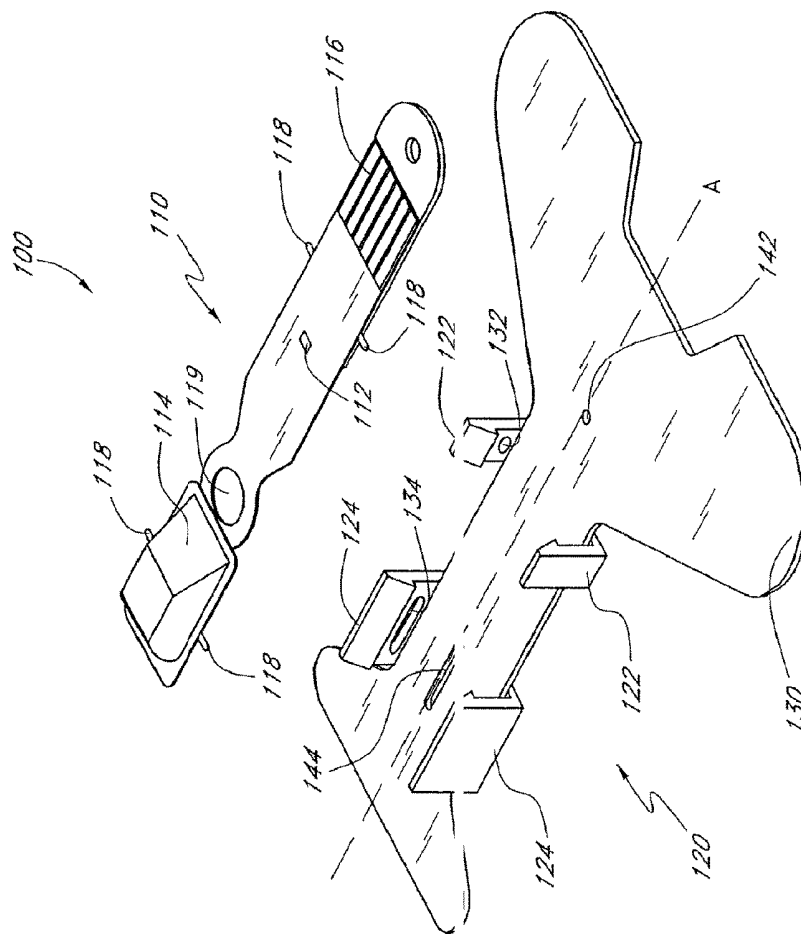
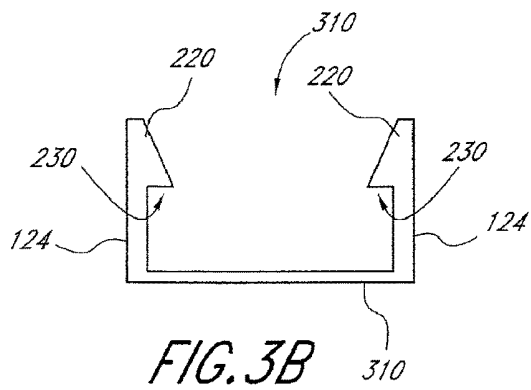
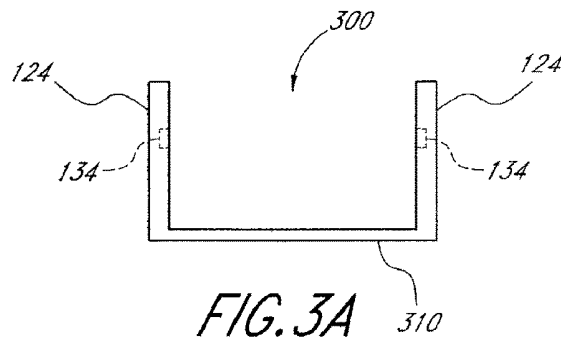
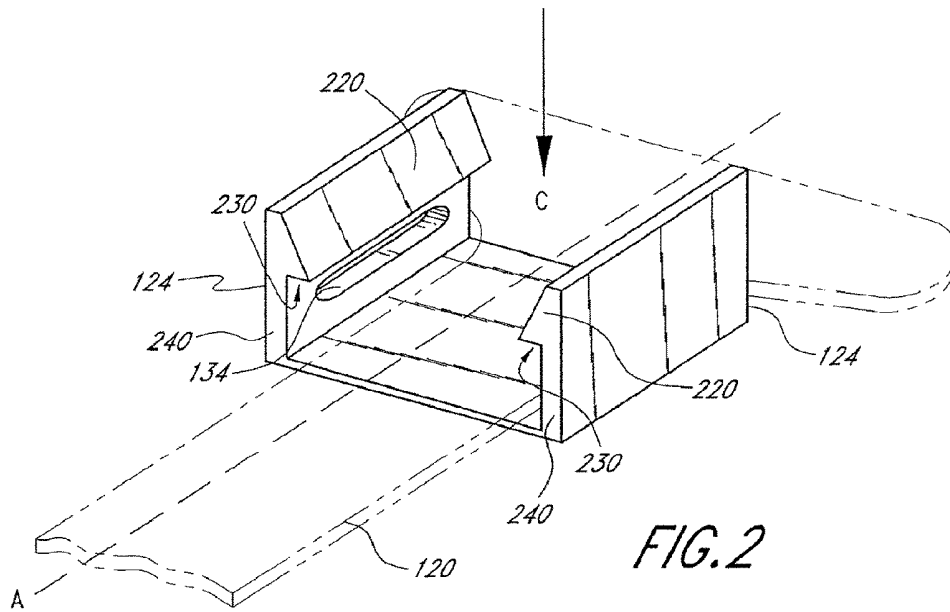
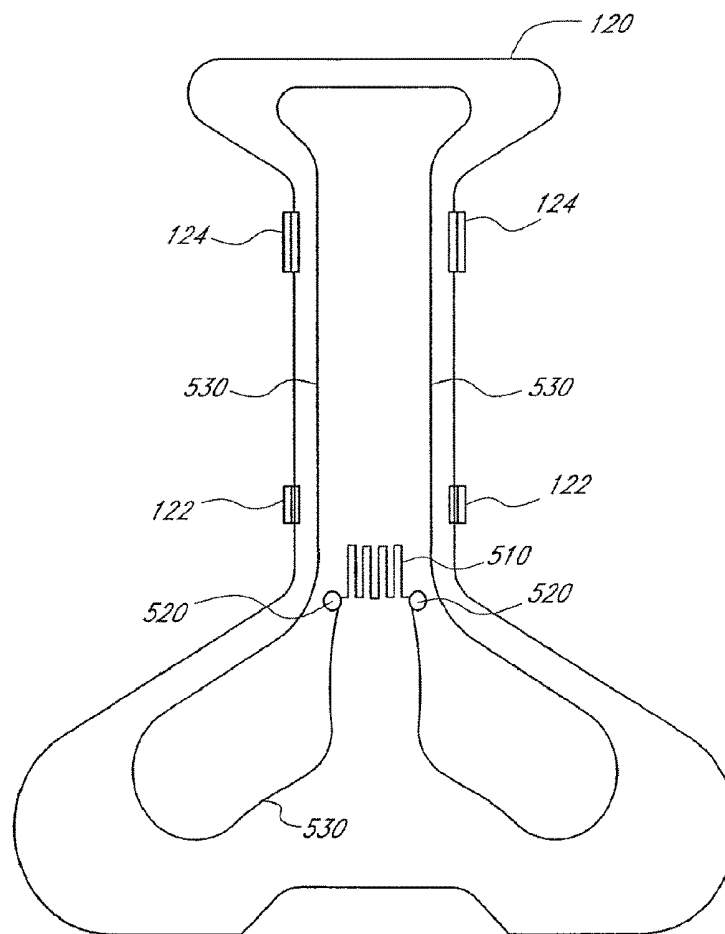
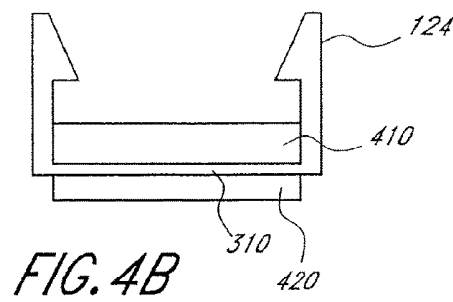
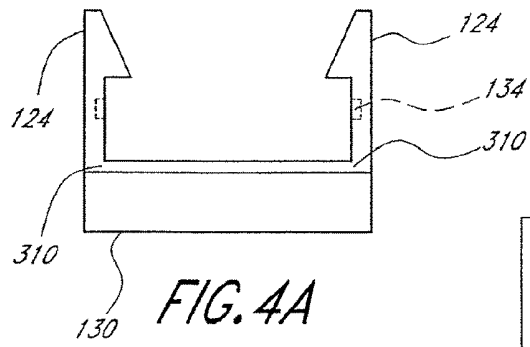
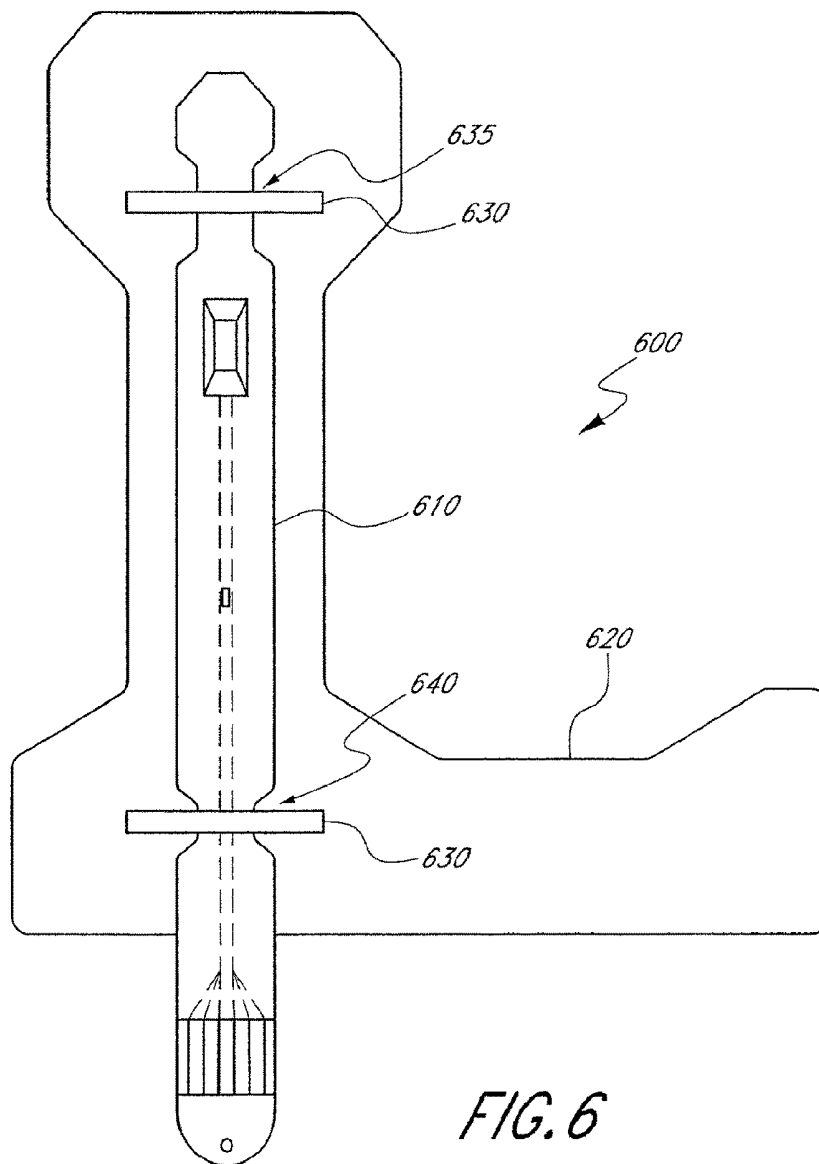
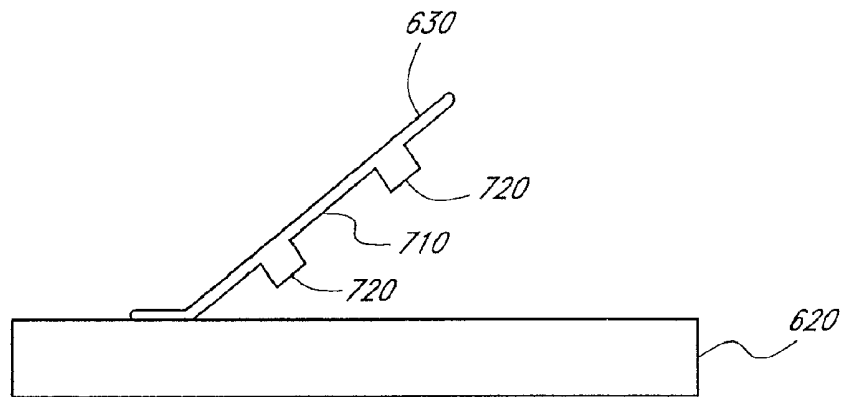
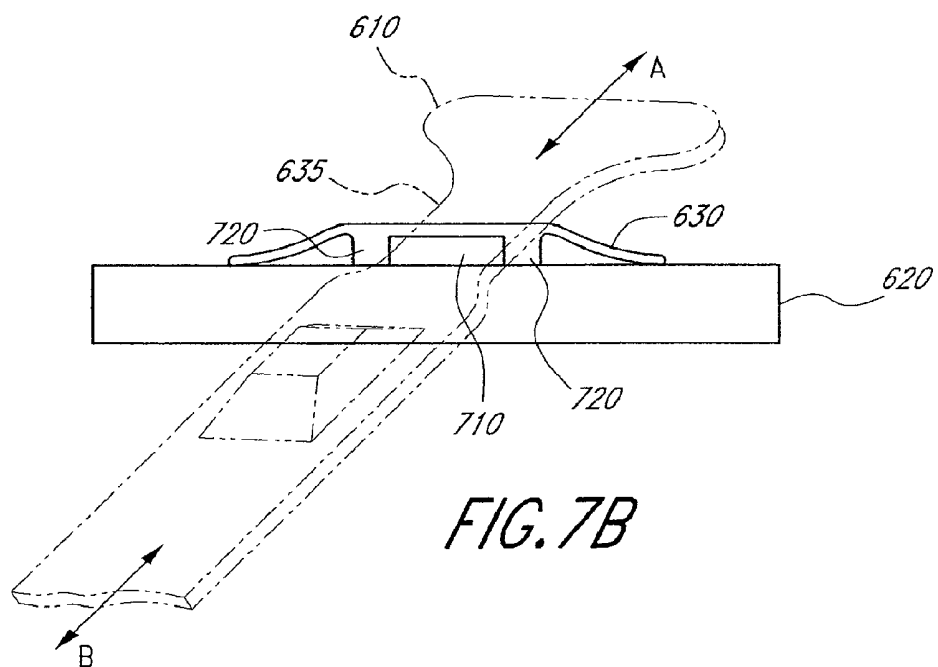



FIG. 1











*FIG. 7A**FIG. 7B*

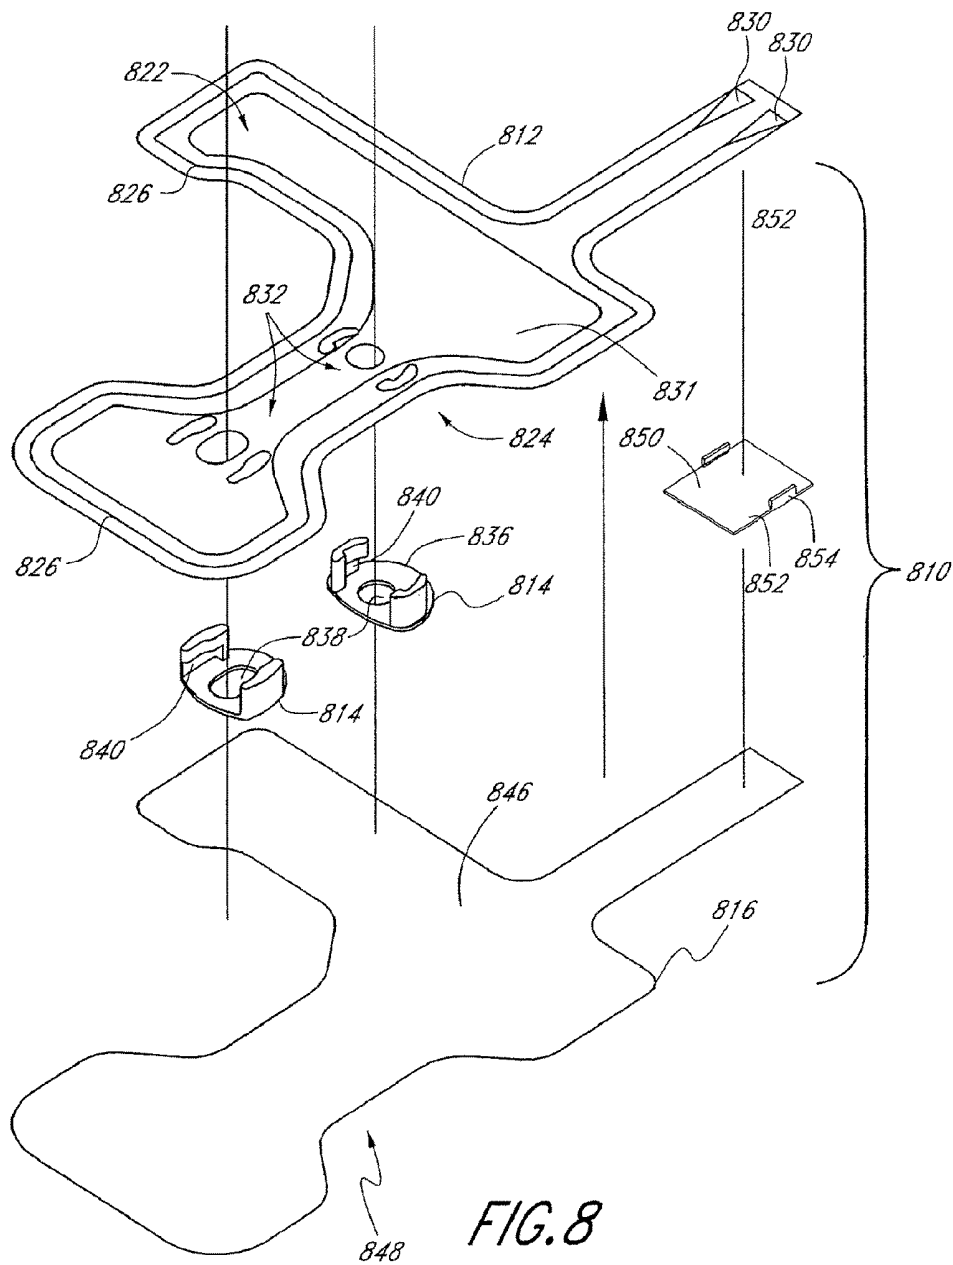

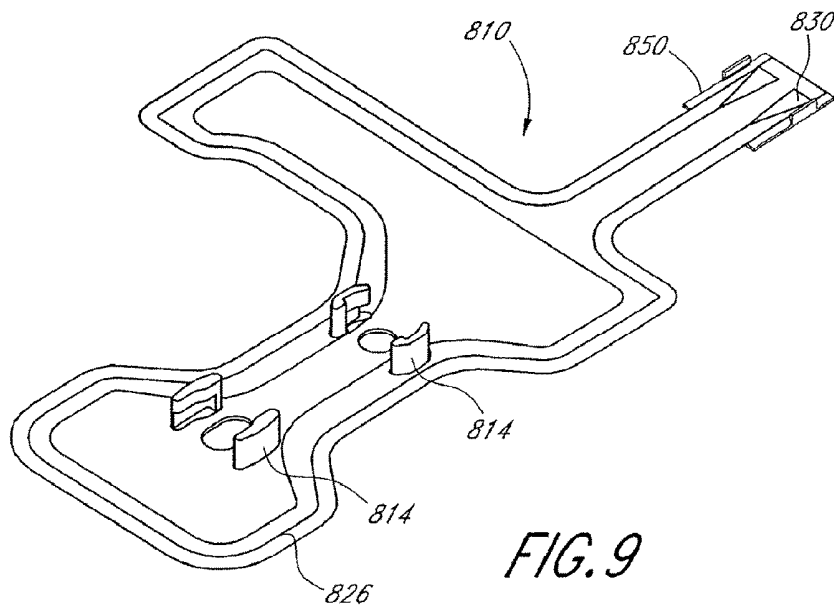

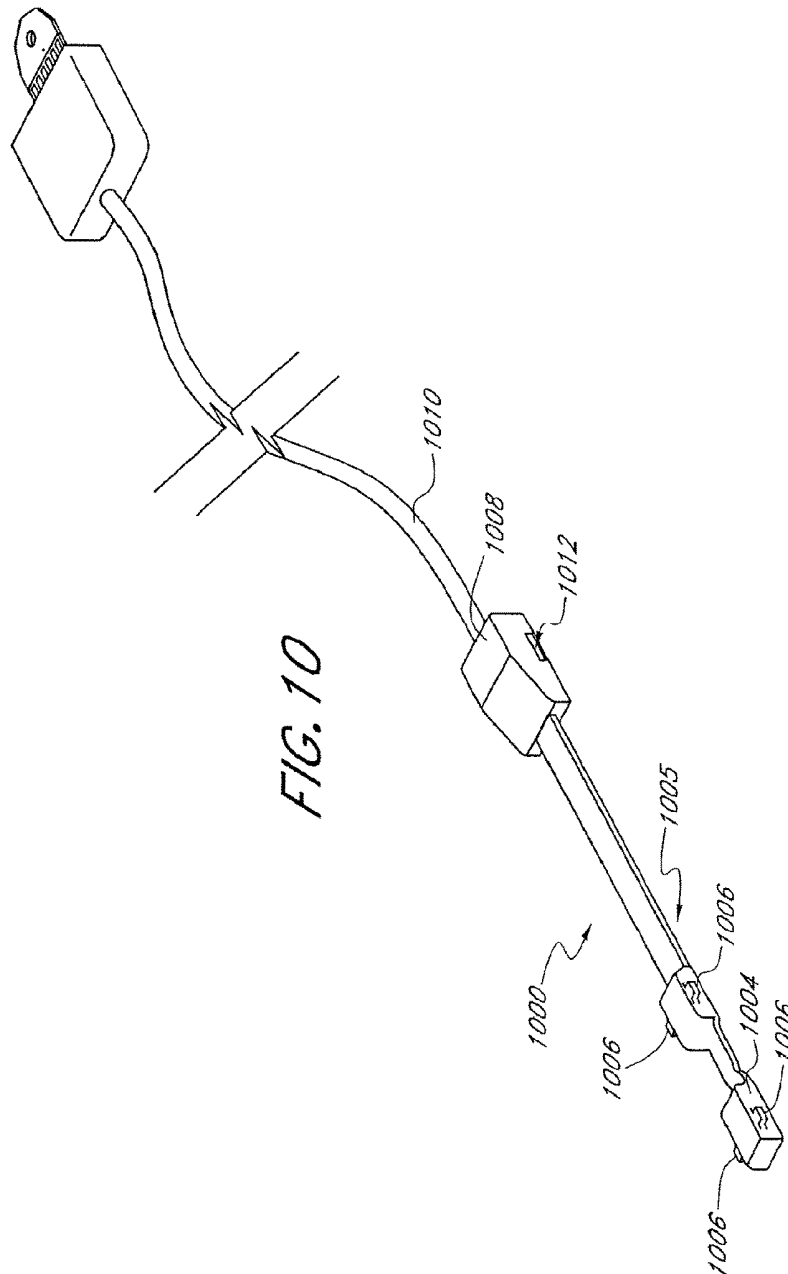

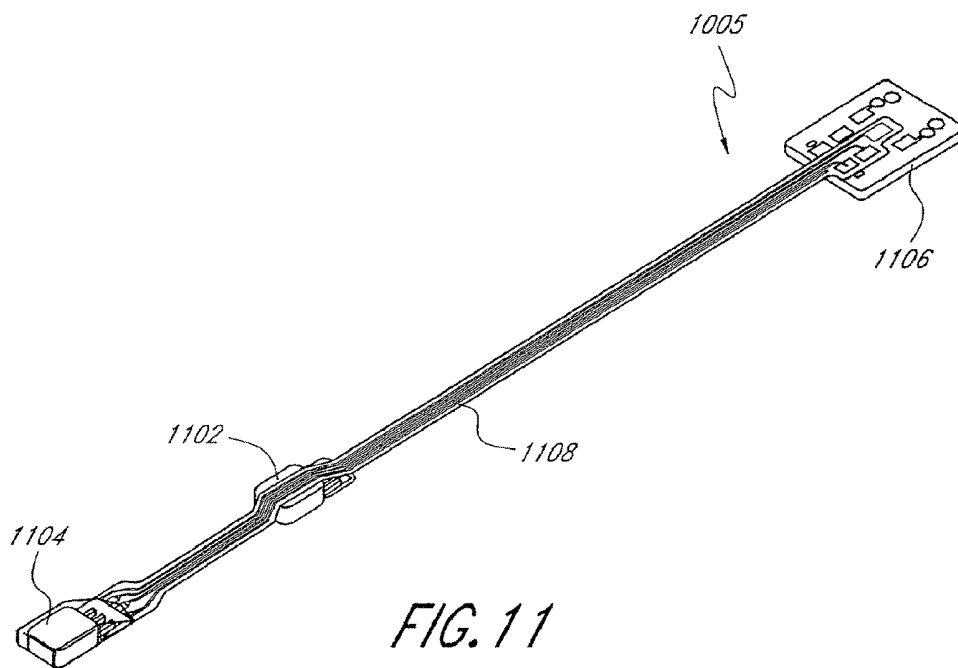

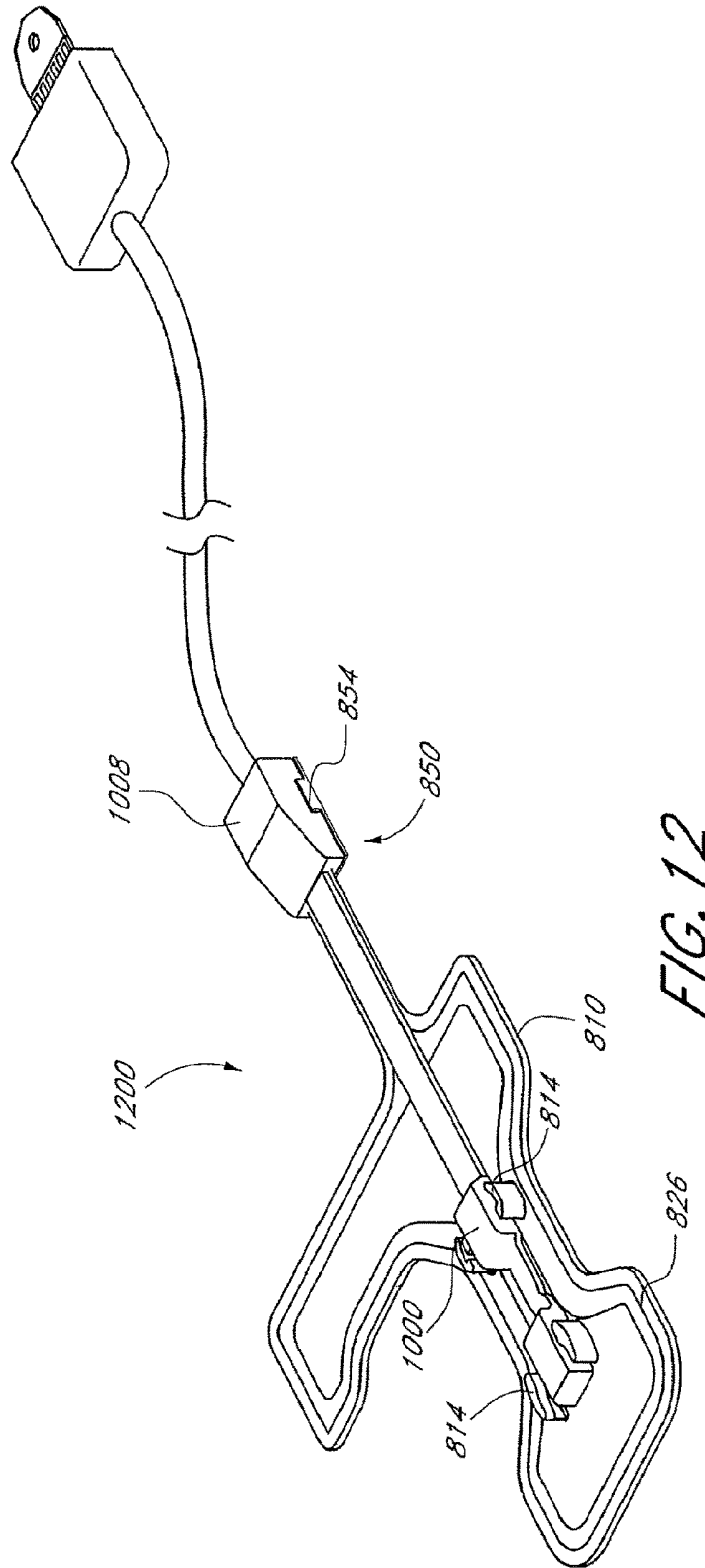

1

NONINVASIVE OXIMETRY OPTICAL SENSOR INCLUDING DISPOSABLE AND REUSABLE ELEMENTS

RELATED APPLICATIONS

The present application is a continuation of U.S. patent application Ser. No. 14/332,004, filed Jul. 15, 2014, entitled "Noninvasive Oximetry Optical Sensor Including Disposable and Reusable Elements," which is a continuation of U.S. patent application Ser. No. 13/585,669, filed Aug. 14, 2012, entitled "Noninvasive Oximetry Optical Sensor Including Disposable and Reusable Elements," now U.S. Pat. No. 8,781,549, which is a continuation of U.S. patent application Ser. No. 11/754,972, filed May 29, 2007, entitled "Noninvasive Oximetry Optical Sensor Including Disposable and Reusable Elements," now U.S. Pat. No. 8,244,325, which is a continuation of U.S. patent application Ser. No. 11/172,587, filed Jun. 30, 2005, entitled "Optical Sensor Including Disposable and Reusable Elements," now U.S. Pat. No. 7,225,007, which is a continuation of U.S. patent application Ser. No. 10/351,645, filed Jan. 24, 2003, entitled "Optical Sensor Including Disposable and Reusable Elements," now U.S. Pat. No. 6,920,345, and claims priority benefit under 35 U.S.C. § 120 to the same. The present application incorporates the foregoing disclosures herein by reference.

FIELD OF THE INVENTION

The present invention relates to the field of sensors that measure oxygen content in a patient's blood. More specifically, the invention relates to a sensor that assembles reusable and disposable elements and/or allows longitudinal displacement between the reusable and disposable elements.

BACKGROUND OF THE INVENTION

Early detection of low blood oxygen is important in a wide variety of medical applications, and oximetry was developed to study and to measure, among other things, the oxygen status of blood. One type of oximetry, pulse oximetry, employs a sensor attached to a patient in order to output a signal indicative of a physiological parameter of the patient, such as, for example, the patient's blood oxygen saturation.

A pulse oximeter sensor generally uses a number of sensor components, such as one or more energy emission devices like red and infrared LED emitters, and an energy detection device like a photodiode detector. The sensor is generally attached to a measurement site such as a patient's finger, toe, ear, forehead, foot, hand, heel or the like, using an attachment mechanism such as a disposable tape, reusable housing, Velcro strap, or the like. The attachment mechanism positions the emitter and detector in proximity to the measurement site, such that the emitter projects energy into the blood vessels and capillaries of the measurement site, and the photodiode detector then detects the attenuated energy. The emitted energy can be light or other forms of energy. The detector communicates a signal indicative of the detected attenuated energy to a signal processing device such as an oximeter. The oximeter generally calculates, among other things, one or more physiological parameters of the measurement site.

In sensors where the detector detects emissions through the measurement site, it is generally desirable to position the detector opposite the emitter around the measurement site,

2

such as, for example, above and below a finger. However, sensors are produced in a limited number of sizes and shape configurations, while patients have, for example, fingers and toes of many different sizes and shapes.

In addition, the attachment mechanism and the electronic components of a sensor are generally curved around a measurement site in a manner detrimental to one or more elements of the sensor. For example, the attachment mechanism generally wraps around the measurement site at an approximate "inner circle" having a first radius, while the electronic components such as the flexible circuits are generally fixedly attached to the attachment mechanism. Accordingly, the electronic components can form an approximate "outer circle" having a second radius unequal to the first radius. However, because the attachment mechanism generally does not move independently with respect to the electrical components, attachment of the sensor to the measurement site can exert forces on the electrical components, such as, for example, exerting forces which try to lengthen, or longitudinally stretch the electrical components to account for an increased radius thereof. The forced stretching can damage the electrical components of a flexible circuit, such as the conductive traces.

SUMMARY OF THE INVENTION

Based on the foregoing, embodiments of the present invention include a sensor comprising reusable and disposable sensor elements that permit longitudinal displacement with respect to one another when the sensor is attached to a measurement site. For example, in one embodiment the sensor includes a reusable element and a disposable element configured to receive the reusable element in a releasable attachment assembly providing longitudinal displacement between the disposable and reusable elements. The longitudinal displacement advantageously allows the sensor elements to self-adjust with respect to one another during attachment to the measurement site. The self-adjustment or independent movement advantageously reduces the forces caused by longitudinal stretching, thereby reducing damage to the reusable element.

One aspect of the invention relates to an optical probe including a reusable element and a disposable element that can be attached together by placing or snapping protrusions on one element into apertures and receiving slots on the other element. For example, the reusable element can be fitted with protrusions made of plastic, and the disposable element can be fitted with detents or tabs, which include apertures or receiving slots. The reusable element attaches to the disposable element by inserting, or snapping, the protrusions into the apertures and the receiving slots of the tabs. When assembled, at least some of the protrusions are slidable within the receiving slots to independently move along a longitudinal axis of the sensor, thereby providing some longitudinal decoupling between the reusable element and the disposable element.

Another aspect of the invention relates to a sensor with a reusable element and a disposable element where the reusable element is made of a flexible or pliable material and includes one or more neck sections. The disposable element includes two straps, each of which is configured to receive a neck section. The reusable element and the disposable element are attached together by placing the neck sections within the straps. In one embodiment, the neck sections include a long neck section and a short neck section. The long neck section has a sufficient length to allow longitudi-

3

nal movement of the reusable element within the strap, thus permitting movement of the reusable element with respect to the disposable element.

Another aspect of the invention relates to a sensor with a reusable element and a disposable element where the reusable element is secured by guides or tabs affixed to the disposable element. The guides allow limited longitudinal motion of the reusable element and thereby allow the reusable element to flex independently of the disposable element as the device is positioned on a patient.

Another aspect of the invention relates to a sensor with a reusable element and a disposable element where the reusable element is encased in a protective cover. In one embodiment, the protective cover is made of a pliable material and prevents any sharp edges from scratching or poking a patient or caregiver. The protective cover also advantageously prevents damage to the reusable element that could occur from dirt, dust, liquids, or other elements of the environment.

Yet another aspect of the invention relates to a sensor with a reusable element and a disposable element where the disposable element includes a breakable element. After an approximate predetermined number of safe uses, the breakable element breaks and the disposable element is rendered inoperable or otherwise indicates its over use.

For purposes of summarizing the invention, certain aspects, advantages and novel features of the invention have been described herein. Of course, it is to be understood that not necessarily all such aspects, advantages or features will be embodied in any particular embodiment of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

A general architecture that implements the various features of the invention will now be described with reference to the drawings. The drawings and the associated descriptions are provided to illustrate embodiments of the invention and not to limit the scope of the invention. The drawings are not necessarily drawn to scale. Throughout the drawings, reference numbers are re-used to indicate correspondence between referenced elements. In addition, the first digit of each reference number indicates the figure in which the element first appears.

FIG. 1 illustrates a perspective view of an embodiment of an unassembled sensor that includes reusable and disposable elements.

FIG. 2 illustrates a perspective view of tabs of the disposable element of FIG. 1.

FIG. 3A illustrates a cross-sectional view of another embodiment of tabs of a disposable element.

FIG. 3B illustrates a cross-sectional view of yet another embodiment of tabs of a disposable element.

FIG. 4A illustrates a cross-sectional view of the two tabs of FIG. 2, adhesively attached to the disposable element.

FIG. 4B illustrates a cross-sectional view of the two tabs of FIG. 2, attached between layers of the disposable element.

FIG. 5 illustrates a top view of the disposable element of FIG. 1, including an information element and breakable conductor.

FIG. 6 illustrates a top view of another embodiment of an assembled sensor that includes reusable and disposable elements.

FIGS. 7A and 7B illustrate simplified cross-sectional views of an embodiment of a strap of the disposable element of FIG. 6.

FIG. 8 illustrates an exploded view of a disposable element according to another embodiment of an optical sensor.

4

FIG. 9 illustrates a perspective view of the disposable element of FIG. 8.

FIG. 10 illustrates a perspective view of an embodiment of a reusable element according to an embodiment of the optical sensor of FIG. 8.

FIG. 11 illustrates a perspective view of a flex circuit of the reusable element of FIG. 10.

FIG. 12 illustrates a perspective view of the assembled optical sensor including the disposable element of FIG. 8 and the reusable element of FIG. 10.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

FIG. 1 illustrates an embodiment of a sensor 100. The sensor 100 includes a reusable element 110 and a disposable element 120. According to one embodiment, the reusable element 110 generally includes those components of the sensor 100 that are more expensive, such as, for example, one or more energy emitters, one or more energy detectors, one or more breakable conductors, one or more information elements, some or all of the same, or the like. In addition, the reusable element 110 includes an assembly mechanism generally shaped to mate with a corresponding component of the disposable element 120, as will be disclosed in greater detail below.

The disposable element 120 generally includes those components of the sensor 100 that are less expensive, such as, for example, face tape, bandages, or other mechanisms for removably attaching the reusable element 110 to a measurement site. Moreover, the disposable element 120 includes a mating assembly mechanism generally shaped to mate with assembly mechanism of the reusable element 110, thereby attaching the reusable element 110 to the disposable element 120 in a manner that provides for at least some self adjustment or displacement between the elements.

When the disposable element 120 attaches the reusable element 110 to tissue of a measurement site, a signal processing device, such as an oximeter, activates the energy emitters to transmit light energy into the tissue. The tissue attenuates the light energy, which is then detected by the detector. A signal indicative of the detected light energy is then generally forwarded back to the signal processing device for determination of one or more physiological parameters of the tissue, such as, for example, oxygen saturation, pulse rate, or the like.

A skilled artisan will recognize from the disclosure herein that there are many combinations of differing shapes and circuit configurations for the reusable and disposable elements, 110 and 120, respectively, such as, for example, those disclosed in U.S. Pat. No. 6,377,829, and U.S. patent application Ser. No. 10/020,664, filed on Dec. 11, 2001, both of which are hereby incorporated by reference.

As shown in the exemplary embodiment of FIG. 1, the reusable element 110 can include one or more energy emitters 112, an energy detector 114, and an electrical connector 116 electrically communicating with the emitters 112 and the detector 114 through a flexible circuit. According to one embodiment, the flexible circuit comprises material of a generally flexible or pliable construction.

The reusable element 110 also includes the foregoing assembly mechanism, such as, for example, the one or more protrusions 118. According to one embodiment, the protrusions 118 comprise approximately cylindrical-shaped or tab-shaped extensions made of plastic or other durable materials. FIG. 1, shows the reusable element 110 including four protrusions 118, two opposing protrusions proximate a

front portion and extending in opposite generally horizontal directions, and two opposing protrusions proximate a back portion and extending in opposite generally horizontal directions. According to one embodiment, the protrusions 118 roughly align with one or more of the electronic components of the sensor 100. As described below, the protrusions 118 each advantageously mate with the mating assembly mechanism of the disposable element 120 in a manner providing for at least some displacement of the reusable element 110 with respect to the disposable element 120, thereby avoiding damage or harmful wear of the reusable element 110.

FIG. 1 also shows the flexible circuit including an optical barrier, such as, for example, an aperture or gap 119 to reduce light energy from traveling from the emitter 112 to the detector 114 without first passing through tissue at the measurement site (i.e., light piping). A skilled artisan will recognize from the disclosure herein that the gap 119 could be replaced with opaque materials, protrusions, pads, tabs, or other light blocking mechanisms.

Although disclosed with reference to preferred embodiments, a skilled artisan will recognize from the disclosure herein, a number of other embodiments of the reusable element 110. For example, one or more of the emitters 112 or the detector 114 can be located on the disposable element 120. Moreover, the flexible circuit may comprise plastic, electric wires, polyester substrates, or the like.

FIG. 1 also shows the disposable element 120. According to an embodiment, the disposable element 120 generally comprises a base 130 comprising a face tapestock material similar to that of an adhesive bandage shaped to position the reusable element proximate the measurement site. The face tape can include an adhesive covered base protected by one or more conveniently shaped release liners or layers. Although illustrated in a conventional elongated surface with opposing wings style shape, an artisan will recognize from the disclosure herein that the tape may comprise virtually any shape, including those disclosed in U.S. patent application Ser. No. 10/020,664, referenced above. Moreover, the disposable element 120 may comprise a Velcro strap, a foam wrap, a reusable plastic housing or the like.

The disposable element 120 also includes the assembly mechanism, illustrated as tabs 122 and 124. Each of the tabs 122 include an aperture 132, while each of the tabs 124 include a receiving slot 134. In one embodiment, the apertures 132 and the receiving slots 134 have sufficient depth to receive the protrusions 118. In other embodiments, the apertures 132 and receiving slots 134 extend through the tabs 122 and 124. As shown in FIG. 1, the tabs 122 and 124 are shaped to removably receive the reusable element 110. For example, the tabs 122 and 124 can include sloped surfaces that cause the tabs 122 and 124 to displace outwardly during assembly of the sensor 100. For example, when the reusable element 110 is properly positioned within the tabs 122 and 124, the tabs 122 and 124 snap inwardly over the reusable element 110 such that the protrusions 118 are within the apertures 132 and the receiving slots 134. When assembled, vertical and horizontal movement between the reusable and disposable elements, 110 and 120 respectively, is substantially prevented by the relationship between the tabs 122 and 124, the apertures 132, the slots 134 and the protrusions 118. However, the slots 134 provide for displacement between elements along longitudinal axis A when the disposable portion 120 is wrapped around a measurement site by allowing the protrusions 118 to slide back and forth within the slots 134. Thus, the assembly mechanisms of the reusable and disposable elements, 110 and 120, provide independent movement between the ele-

ments, thereby allowing self-adjustment of the sensor 100 to the differing radiuses of each element. Such construction advantageously reduces the harmful stressing effects applied to components of the reusable element 110.

FIG. 1 also shows that a gap 142, slot or aperture, or otherwise transparent area can be included on the disposable element 120 to permit light from the emitter 112 to travel through the disposable element 120 to the tissue of the measurement site. Moreover, another gap 144 can be included on the disposable element 120 to permit attenuated light from the measurement site tissue to travel through the disposable element 120 to the detector 114. In another embodiment, some or all of the base 130 of the disposable element 120 is made of a transparent material, and the gaps 142 and 144 can be omitted.

A skilled artisan will recognize from the disclosure herein that the tabs 122 and 124 of the disposable element 120 can be implemented in a wide variety of embodiments. For example, an embodiment can include each of the tabs 122 and 124 having a receiving slot 134 while another embodiment can include each of the tabs 122 and 124 having an aperture 132.

FIG. 2 illustrates a perspective view of the tabs 124 including the receiving slots 134. As disclosed, the tabs 124 can be shaped to include a sloped surface 220 configured to displace a ledge or catch 230 during sensor assembly. For example, the sloped surface 220 displaces outwardly when protrusions 118 are pressed in the direction of the arrow C. Then when the reusable element 110 is properly positioned, the protrusions 118 snap into the receiving slots 134 and the catch 230 snaps over a top surface of the reusable element 110.

The receiving slots 134 are longer than the cross sectional width of the protrusions 118 so that the protrusions 118 can move within the receiving slots 134 to different positions along the longitudinal axis A of the disposable element 120. The apertures 132, on the other hand, are sized to allow protrusions 118 to be located within the apertures 132 but to prevent substantial movement along the longitudinal axis A of the disposable element 120, thus ensuring proper positioning of the sensor elements, with respect to the tissue and one another.

In an embodiment, the reusable element 110 and the disposable element 120 are assembled into the sensor 100 when the protrusions 118 are snapped into the apertures 132 and the receiving slots 134 of the tabs 122 and 124. The assembled sensor 100 is then attached to a measurement site, through, for example, application of the adhesive covered side of the face tape to tissue at the measurement site. During application, the protrusions 118 within the receiving slots 134 move along the receiving slot 134, while the protrusions 118 remain positioned within the aperture 132. This type of flexibility advantageously reduces the stretching force placed on conventional reusable elements.

FIG. 2 also shows receiving slots 134 as grooves in the walls 240 of the tabs 124, where the grooves do not extend all the way through the walls 240. In other embodiments, the receiving slots 134 can be open slots that extend through the walls 240. Likewise, the aperture 132 can be straightforward depressions, or punch through holes.

FIG. 3A illustrates a cross-sectional view of tabs 300 of another embodiment of a disposable element, such as disposable element 120 of FIG. 1. The tabs 300 include the receiving slot 134 for receiving the protrusions 118, but does not include the sloped surface 220 or the catch 230 of FIG. 2. Thus, the reusable element 110 is assembled relying on

the interaction described in the foregoing between the protrusions 118 and the apertures 132 and the slots 134.

FIG. 3B illustrates a cross-sectional view of tabs 310 of another embodiment of a disposable element, such as the disposable element of FIG. 1. The tabs 310 include the sloped surface 220 and the catch 230, but do not include the receiving slot 134 or aperture 132. Thus, the sensor 100 is assembled relying on the interaction between the catch 230 and the surface of the reusable element 110.

FIG. 4A illustrates a cross-sectional view of the tabs 124 of FIG. 1 adhesively attached to the disposable element 120, according to an embodiment. In FIG. 4A, the tabs 124 are attached to the base 130 by adhesive. In a preferred arrangement, the tabs 124 share a common substrate 310, and an adhesive is applied between the substrate 310 and the base 130 to attach the tabs 124 to the disposable element 120.

FIG. 4B illustrates a cross-sectional view of the tabs 124 of FIG. 1 attached between layers of the disposable element 120 of FIG. 1, according to another embodiment. In FIG. 4B, the tabs 124 are attached between two layers 410 and 420 of the base 130. In a preferred arrangement, the two tabs 124 share a common substrate 310, and the substrate 310 is sandwiched between the layers 410 and 420.

A skilled artisan will recognize from the disclosure herein that the embodiments disclosed with reference to FIGS. 3 and 4 can be applied to one or both sets of the tabs 122 and 124. Moreover, a skilled artisan will recognize from the disclosure herein that the protrusions 118 can be attached to the reusable element 110 in a number of ways, such as, for example, attached by adhesive to the reusable element 110, manufactured as integral parts of the reusable element 110, sandwiched between a top layer and a bottom layer of the reusable element 110, or the like.

FIG. 5 illustrates a top view of the disposable element of FIG. 1, including an information element 510, contacts 520, and a breakable conductor 530, according to yet another embodiment. The contacts 520 can electrically connect with contacts on the flexible circuit of the reusable element 120, thereby adding the information element 510 and/or the breakable conductor 530 into the electric circuit of the sensor 100. As is understood in the art, the information element 510 can provide an indication of the sensor or patient type, operating characteristics or the like, or that the sensor 100 is from an authorized supplier. In an embodiment, the information element 510 is a resistive element made by depositing a conductive ink trace having a predetermined length and width. The information element 510 is disposed between contacts 520, which can also be implemented with conductive ink. As an artisan will recognize from the disclosure herein, many type of information elements can be included, such as, for example, passive or active elements, accessible memory elements, or the like.

The breakable conductor 530 is configured to break after a predetermined number of safe uses, thus providing quality control to ensure that the disposable element 120 is not over used. Various embodiments of information element 510, contacts 520, and breakable conductor 530 can be found in U.S. Pat. No. 6,377,829.

FIG. 6 illustrates a top view of an assembled sensor 600 that includes reusable and disposable elements, according to another embodiment. As shown in FIG. 6, the sensor 600 includes a reusable element 610 and a disposable element 620. The disposable element 620 includes straps 630 which position the reusable element 610 as described below. As shown in FIG. 6, the reusable element 610 can be similar to the reusable element 110 of the foregoing embodiments, generally including, for example, the more expensive com-

ponents of the sensor 600. Moreover, disposable element 620 can be similar to the disposable element 120 of the foregoing embodiments, generally including for example, a disposable tape. The disposable tape can be virtually any suitable shape, and is shown in FIG. 6 in a generally "L" shaped configuration.

FIG. 6 also shows the reusable portion 610 including an extended narrow neck or notch 635 and a neck or notch 640, each narrower in width than the general width of the reusable element 610. The straps 630 attached to the disposable element 620 extend over the necks 635 and 640 to position the reusable element 610 with respect to and proximate the disposable element 620. The straps 630 provide for longitudinal movement between the elements of the sensor 600 similar to that disclosed in the foregoing.

FIG. 7A illustrates a simplified cross-sectional view of one of the straps 630 of the disposable element 620 of FIG. 6, according to an embodiment. The strap 630 may comprise a hook-and-loop device such as Velcro. The strap 630 may alternatively be an integral part of the structure of the disposable element 620. According to an embodiment, the strap 630 includes blocks 720 forming a gap 710 therebetween. As shown in FIG. 7A, an embodiment of the strap 620 can be removed from the disposable element 620 to permit the neck 630 of the reusable element 610 to be placed within the gap 710, as shown in FIG. 7B an artisan will also recognize from the disclosure herein that the pliable material of the reusable portion 610 can alternatively or concurrently be compressed together and guided through attached straps 630.

According to one embodiment, the gap 710 is as wide or slightly wider than the necks 635 and 640, but narrower than other adjacent portions of the reusable element 610. Therefore, once placed in the gaps 710 and attached to the disposable element 620, the reusable element 610 can be moved along its longitudinal axis along the arrows A and B (FIG. 7B), but only to the extent that the necks 635 and 640 remain in the gaps 710.

In one embodiment shown in FIG. 6, the reusable element 610 includes the relatively "long" neck 635 shown near the top of the figure and a relatively "short" neck 640 shown near the bottom of the figure. Once the two necks 635 and 640 are placed within the straps 650, the long neck 635 allows the reusable element 610 to be moved along a longitudinal axis of the disposable element 120. In contrast, the short neck 640 prevents substantial movement along the longitudinal axis. Thus, similar to embodiments disclosed in the foregoing, the sensor 600 allows the neck 630 to self adjust during application to a measurement site, thereby avoiding damaging the reusable element 610.

FIG. 8 illustrates an exploded view of a disposable element 810 according to another embodiment of an optical sensor. The disposable element 810 includes a top layer 812, at least one attachment mechanism, tab, or positioning guide 814, and an adhesive, preferably transparent, tape layer 816. FIG. 8 shows tabs 814 positioned in a back-to-back or opposing manner, as will be described in greater detail below.

FIG. 8 shows the top layer 812 as a generally L shaped tape or other pliable substrate including a first side 822 and a second side 824, although an artisan will recognize from the disclosure herein that the virtually any shape can be used which provides attachment to tissue of a patient. According to an embodiment, the first side 822 includes a breakable element 826, such as the conductive trace disclosed in U.S. Pat. No. 6,377,829, discussed in the foregoing. The breakable element 826 is included into the electrical circuit of the

optical sensor through electrical leads or contacts **830** configured to electrically communicate with contacts of a reusable element of the optical sensor. Moreover, the first side **822** of the top layer **812** can optionally include an optical barrier layer **831**, such as a layer of material opaque or substantially opaque to light. The optical barrier layer **831** is generally designed to help prevent ambient light or light piping from interfering with the optical signals before or after they are passed through the tissue of the patient. In one embodiment, the barrier layer **831** comprises conductive trace material similar to that of the breakable element **826**.

According to an embodiment, the top layer **812** also includes a plurality of apertures **832**, which when the optical sensor is assembled, accept portions of the tabs **814** in a manner designed to provide proper placement, positioning, and support of the tabs **814**. However, an artisan will recognize from the disclosure herein that top layer **812** may use ink outlines combined with adhesive, or the like to help an assembler properly place and support the tabs **814** on the first side **822** of the top layer **812**.

Each tab **814** includes a base **836**, a signal aperture **838**, and grooves or slots **840**. The base **836** connects and supports each of two raised side members forming a generally U shaped structure. The signal apertures **838** comprise holes through which a properly positioned sensor element can emit or detect optical signals, and the raised side members each include the slot **840**, similar to the grooves **134** of the tabs **124** of FIG. 1. However, unlike FIG. 1, an embodiment of each of the slots **840** opens from one side of the raised side member, extends along the side member, and ends before the other side of the raised side member. Thus, the slot **840** accepts a protrusion or the like from an insertion side, and allows the protrusion to slide within the slot **840** to the end thereof, proximate a blocked side. Moreover, according to one embodiment, the blocked sides of the tabs **814** approximately adjacently oppose one another, such that protrusions inserted into the insertion sides, are at one point blocked from sliding closer than a predetermined distance from one another by the blocked sides.

According to one embodiment, the tape layer **816** comprises a transparent tape or other substrate layer. The tape layer **816** has a first side **846** and a second side **848**. When assembled, the first side **846** adheres to the top layer **812** and sandwiches the tabs **814** therebetween. The second side **848** includes an adhesive, hook-and-loop, similar or combination structure configured to secure the disposable element **810** to tissue of a patient.

FIG. 8 also shows the disposable element **810** including a cable connector **850**. The cable connector **850** generally provides for connection of the disposable element **810** to the remainder of a sensor, such as, for example, the reusable elements. According to the exemplary embodiment, the cable connector **850** comprises a plastic plate **852** including mating portions **854**, such as, for example, raised pliable detents that each including a catch. However, an artisan will recognize from the disclosure herein any suitable mating mechanism can be used to connect the disposable element **810**, including virtually any mechanical-type mating mechanism, adhesives, hook-and-loop materials, combinations, or the like.

When the disposable element **810** is assembled as shown in FIG. 9, the bases **836** of the tabs **814** and the plate **852** communicate with the second side **824** of the top layer **812** and first side **846** of the tape layer **816** such that the bases **836** of the tabs **814** and the plate **852** are secured in position between the top layer **812** and the tape layer **816**. The raised side members of the tabs **814** extend through the plurality of

apertures **832** in the top layer **812**, thereby aligning the signal apertures **838** with apertures in the top layer **812**. Moreover, as shown in the illustrated embodiment, the mating portions **854** of the cable connector **850** extend above the top layer **812**.

FIG. 10 shows a perspective view of an embodiment of a reusable element **1000**. The reusable element **1000** preferably includes a protective cover or coating **1004** covering a plurality of electronic sensor elements **1005** and a plurality of protrusions **1006**. The reusable element **1000** also includes a cable connection housing **1008**, and cord or cable **1010**. According to one embodiment, the protective cover **1004** comprises a soft material, such as a pliable rubber, plastic or the like, which preferably encapsulates and protects the electronic sensor elements **1005** from damage and advantageously protects caregivers and patients from sharp corners often associated with the reusable element **1000**, such as, for example, the protrusions **1006** or the sensor elements **1005**.

The protrusions **1006** extend from opposing sides of the reusable element **1000** in generally horizontal and opposing directions. To assemble the optical sensor, the protrusions are aligned with the outside-facing insertion side of each of the slots **840** of the disposable element **810**, shown in FIG. 8, and are slid toward one another on each side. As can be seen in FIG. 12, an embodiment of the assembled sensor includes one or more of the protrusions **1006** abutting the blocked side of one pair of the slots **810**, while the other protrusions **1006** are proximate the blocked side of the other pair of slots **810**, thereby allowing the reusable element **1000** to self adjust and avoid the detrimental stretching forces caused from application to a measurement site.

FIG. 10 also shows the cable connection housing **1008** including insertion slots **1012** configured to receive and mate with the mating portions **854** of the cable connector **850** shown in FIG. 8. When mated, the cable connection housing **1008** provides electrical contact between the electrical leads **830** of the disposable element **810** and the sensor circuitry.

FIG. 11 illustrates a perspective view of portions of the electronic sensor elements **1005** of the reusable element **1100** without the protective cover or coating **1004**. The elements **1005** include one or more energy emitters **1102**, such as one or more LEDs, an energy detector **1104**, such as a photodetector, electrically connected to a connector **1106** through a flexible circuit **1108**. The connector **1106** is configured to electrically communicate with the leads **830** of the disposable element **810** when the sensor is assembled. Moreover, the connector **1106** is configured to electrically attach the conductive traces of the flexible circuit **1108** to the conductors of the cable **1010**.

FIG. 12 shows a perspective view of an assembled sensor **1200**. The sensor **1200** includes the reusable element **1000**, including the disposable element **810** connected to the connection housing **1008** through the mating portions **854** of the cable connector **850**, such that the breakable element **826** is part of the electrical circuitry of the sensor. In one embodiment, the sensor is inoperative or otherwise provides an indication of overuse or misuse when the breakable element **826** is broken or otherwise becomes an open circuit.

As disclosed, when connected to the disposable element **810**, the protrusions **1006** have a limited range of motion within the tabs **814**, thereby giving the reusable element **1000** a limited range of longitudinal motion independent of the disposable element **810**. As described with other embodiments, this longitudinal motion allows the disposable element **810** and the reusable element **1000** to flex indepen-

dently as the sensor **1200** is attached to tissue of a user, such as a finger, toe, ear, or the like, thereby avoiding damage or unnecessarily harmful wear of the reusable element **1000**. Also, this limited range of motion ensures at least approximate proper alignment of various sensor components.

After use, as with embodiments described above, the disposable element **810** is removed and discarded, while the reusable element **812** can be sterilized and reused.

Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. For example, although the above sections describe a reusable element fitted with protrusions or necks and a disposable element fitted with apertures and receiving slots or straps, the embodiments can be reversed having, for example, the reusable element fitted with the apertures, receiving slots, or straps, and with the disposable element fitted with the protrusions or necks.

Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the reaction of the preferred embodiments, but is to be defined by reference to the appended claims.

What is claimed is:

1. A reusable portion of a noninvasive optical oximetry sensor, the sensor when assembled configured to attach to a measurement site of a monitored patient and to output signals responsive to light absorption by tissue at the measurement site, wherein an oximeter receiving the signals or data responsive to the signals is configured to determine one or more physiological parameters of the patient including at least oxygen saturation or pulse rate, the oximeter including a front end in electrical communication with the sensor, the reusable portion comprising:

a sensor connector;

at least one light source;

at least one detector configured to detect light from the at least one light source after attenuation by the tissue and output the signals responsive to the detected light;

a plurality of first mating elements mechanically matable with second mating elements of a disposable portion of the sensor, wherein the first and second mating elements move with respect to one another to provide independent flexion of the reusable portion and the disposable portion during attachment of the sensor to the patient, the first and second mating elements configured to cause proper alignment in the sensor between the reusable portion and the disposable portion, wherein the disposable portion includes:

an electrical circuit element other than the at least one light source, the at least one light detector, or other light emitting or detecting device, and

first electrical contacts in electrical communication with the electrical circuit element; and

second electrical contacts configured to electrically connect to the first electrical contacts when the reusable portion is mated with the disposable portion, the sensor being inoperative when the first and second electrical contacts are not sufficiently proximate to one another to form a completed circuit, the completed circuit including at least the second electrical contacts, the first electrical contacts, the electrical circuit element, the sensor connector, and the front end of the oximeter.

2. The reusable portion of claim 1, wherein the disposable portion is a first disposable portion of a plurality of identical

disposable portions, the reusable portion configured to mate with each of the plurality of identical disposable portions at distinct time intervals.

3. The reusable portion of claim 1, wherein the electrical circuit element is configured to at least temporarily prevent the first and second electrical contacts from forming the completed circuit after a threshold number of uses of the sensor.

4. The reusable portion of claim 3, wherein the electrical circuit element comprises a breakable conductor.

5. The reusable portion of claim 4, wherein discontinuity of the breakable conductor prevents the first and second electrical contacts from forming the completed circuit.

6. The reusable portion of claim 1, wherein the first and second electrical contacts are sufficiently proximate to one another to form the completed circuit when the reusable portion is mated with the disposable portion.

7. The reusable portion of claim 1, wherein the first and second mating elements comprise at least some tabs and at least some slots, wherein the at least some slots are shaped to allow the at least some tabs to move within the at least some slots to allow the independent flexion.

8. The reusable portion of claim 1, wherein the first mating elements comprise one or more straps and the second mating elements comprise one or more neck sections, wherein each strap includes a gap adapted to receive one of the neck sections, wherein the gap is narrower in cross section than adjacent sections of the reusable portion, wherein at least a portion of the reusable portion is slidable within at least one or the gaps to allow the independent flexion.

9. A disposable portion of a noninvasive optical oximetry sensor, the sensor when assembled configured to attach to a measurement site of a monitored patient and to output signals responsive to light absorption by tissue at the measurement site, wherein an oximeter receiving the signals or data responsive to the signals is configured to determine one or more physiological parameters of the patient including at least oxygen saturation or pulse rate, the oximeter including a front end in electrical communication with the sensor, the reusable portion comprising:

a plurality of first mating elements mechanically matable with second mating elements of a reusable portion of the sensor, wherein the first and second mating elements move with respect to one another to provide independent flexion of the disposable portion and the reusable portion during attachment of the sensor to the patient, the first and second mating elements configured to cause proper alignment in the sensor between the disposable portion and the reusable portion, wherein the reusable portion includes first electrical contacts, at least one light source, a sensor connector, and at least one light detector;

an electrical circuit element other than the at least one light source, the at least one light detector, or other light emitting or detecting device; and

second electrical contacts configured to electrically connect to the first electrical contacts when the disposable portion is mated with the reusable portion, the sensor being inoperative when the first and second electrical contacts are not sufficiently proximate to one another to form a completed circuit, the completed circuit including at least the second electrical contacts, the first electrical contacts, the electrical circuit element, the sensor connector, and the front end of the oximeter.

10. The disposable portion of claim 9, wherein the electrical circuit element is configured to at least temporarily

13

prevent the first and second electrical contacts from forming the completed circuit after a threshold number of uses of the sensor.

11. The disposable portion of claim 10, wherein the electrical circuit element comprises a breakable conductor. 5

12. The disposable portion of claim 11, wherein the breakable element loses continuity after a threshold number of uses of the sensor, the loss of continuity rendering the disposable portion inoperative.

13. The disposable portion of claim 11, wherein a loss of continuity in the breakable conductor prevents the first and second electrical contacts from forming the completed circuit. 10

14. The disposable portion of claim 9, wherein the electrical circuit element comprises conductive ink.

15. The disposable portion of claim 9, wherein the electrical circuit element comprises an information element. 15

16. The disposable portion of claim 15, wherein the information element is configured to provide at least one of an indication of sensor type, patient type, sensor operating characteristics, or that sensor is from an authorized supplier.

14

17. The disposable portion of claim 9, wherein the first and second electrical contacts are sufficiently proximate to one another to form the completed circuit when the disposable portion is mated with the reusable portion.

18. The disposable portion of claim 9, wherein the first and second mating elements comprise at least some tabs and at least some slots, wherein the at least some slots are shaped to allow the at least some tabs to move within the at least some slots to allow the independent flexion.

19. The disposable portion of claim 9, wherein the first mating elements comprise one or more straps and the second mating elements comprise one or more neck sections, wherein each strap includes a gap adapted to receive one of the neck sections, wherein the gap is narrower in cross section than adjacent sections of the reusable portion, wherein at least a portion of the reusable portion is slidable within at least one of the gaps to allow the independent flexion.

* * * * *

专利名称(译)	无创血氧测定光学传感器，包括一次性和可重复使用的元件		
公开(公告)号	US10201298	公开(公告)日	2019-02-12
申请号	US15/642162	申请日	2017-07-05
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR ABDUL HAFIZ YASSIR		
发明人	AL-ALI, AMMAR ABDUL-HAFIZ, YASSIR		
IPC分类号	A61B5/1455 A61B5/00		
CPC分类号	A61B5/14552 A61B5/6826 A61B5/6838 A61B5/6833 Y10T29/49826		
优先权	11/172587 2007-05-29 US		
其他公开文献	US20170367632A1		
外部链接	Espacenet		

摘要(译)

脉搏血氧饱和度传感器包括可重复使用和一次性元件。为了组装传感器，可重复使用元件的构件与一次性元件的组装机构配合。组装好的传感器在可重复使用和一次性元件之间提供独立的运动。

