



US 20180184901A1

(19) **United States**

(12) **Patent Application Publication**
Akmandor et al.

(10) **Pub. No.: US 2018/0184901 A1**

(43) **Pub. Date: Jul. 5, 2018**

(54) **STRESS DETECTION AND ALLEVIATION
SYSTEM AND METHOD**

Publication Classification

(51) **Int. Cl.**

A61B 5/00 (2006.01)

A61B 5/16 (2006.01)

A61B 5/024 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/0006* (2013.01); *A61B 5/165*

(2013.01); *G16H 50/30* (2018.01); *A61B*

5/0024 (2013.01); *A61B 5/4884* (2013.01);

A61B 5/02405 (2013.01)

(71) Applicant: **The Trustees of Princeton University,**
Princeton, NJ (US)

(72) Inventors: **Ayten Ozge Akmandor,** Princeton, NJ
(US); **Niraj K. Jha,** Princeton, NJ (US)

(73) Assignee: **The Trustees of Princeton University,**
Princeton, NJ (US)

(21) Appl. No.: **15/857,981**

(22) Filed: **Dec. 29, 2017**


Related U.S. Application Data

(60) Provisional application No. 62/442,517, filed on Jan.
5, 2017.

(57)

ABSTRACT

According to various embodiments, a stress detection and alleviation (SoDA) system for a user is disclosed. The system includes a SoDA device configured with one or more processors that receive wearable medical sensor (WMS) data from a plurality of WMSs. The processors are programmed to remove one or more artifacts from the WMS data, extract a set of features from the WMS data, remove correlated features from the extracted features to obtain a reduced set of features, classify the reduced set of features in order to determine whether the user is stressed, and generate a response based on whether the user is stressed.

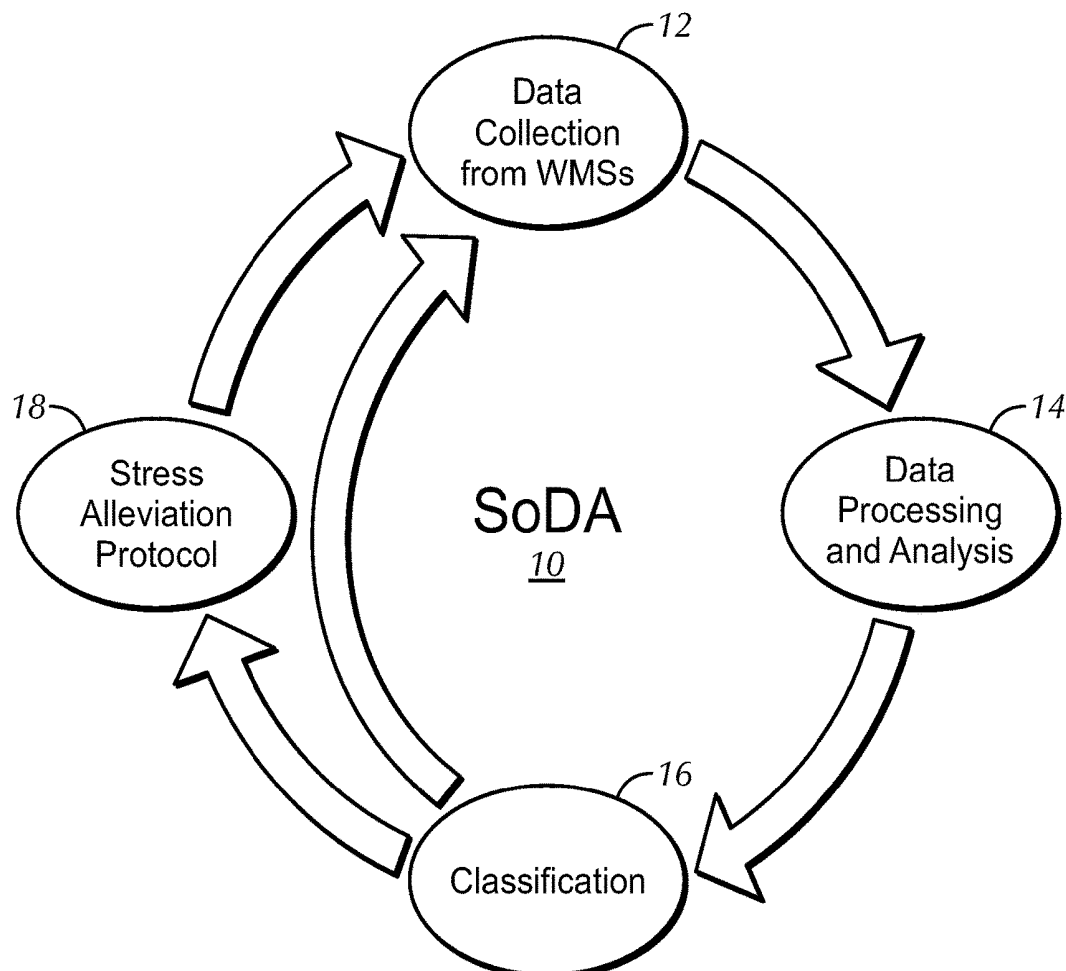

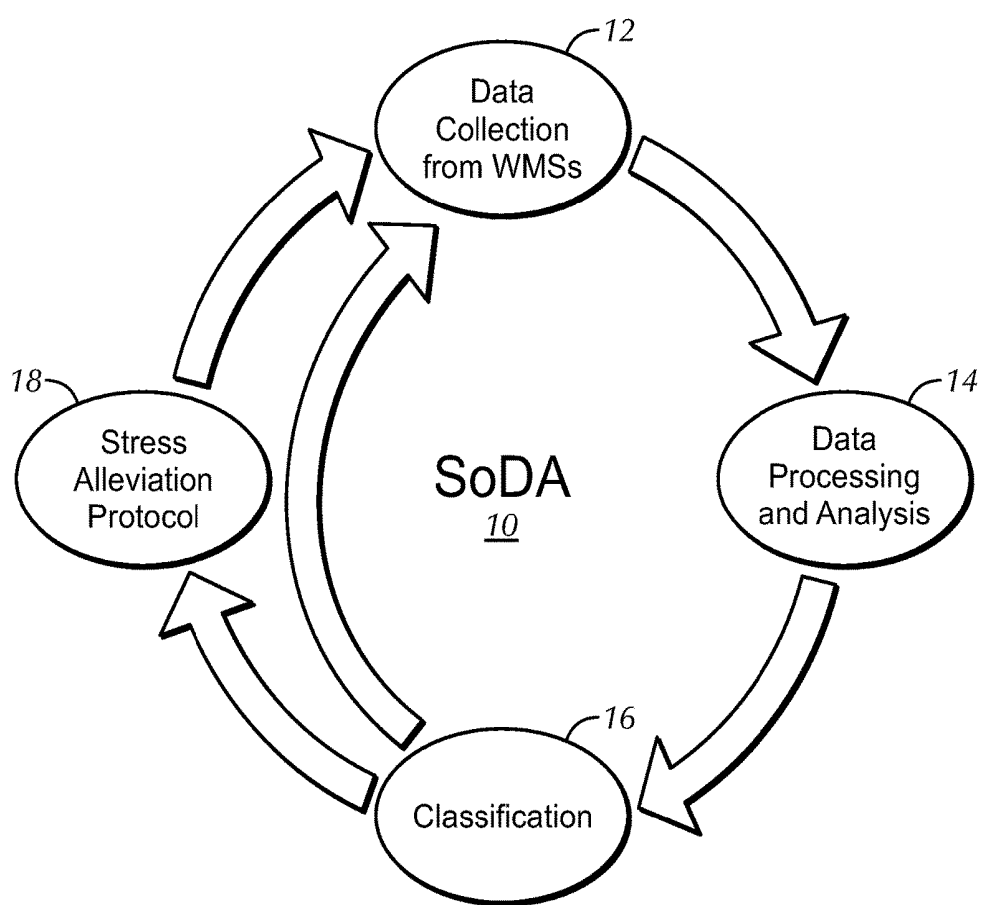
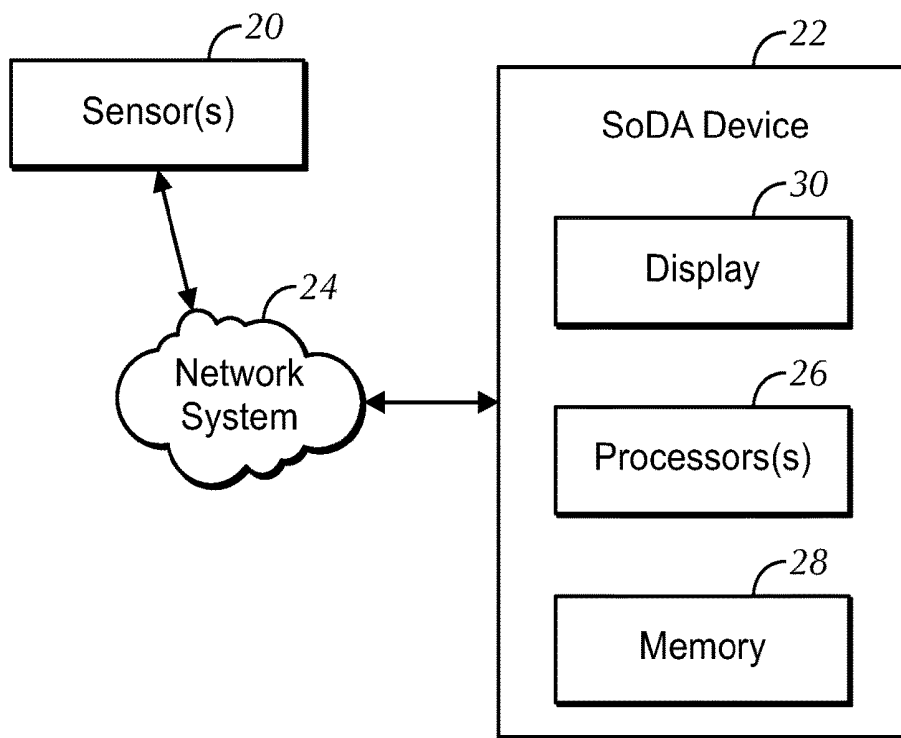


FIG. 1

**FIG. 2**

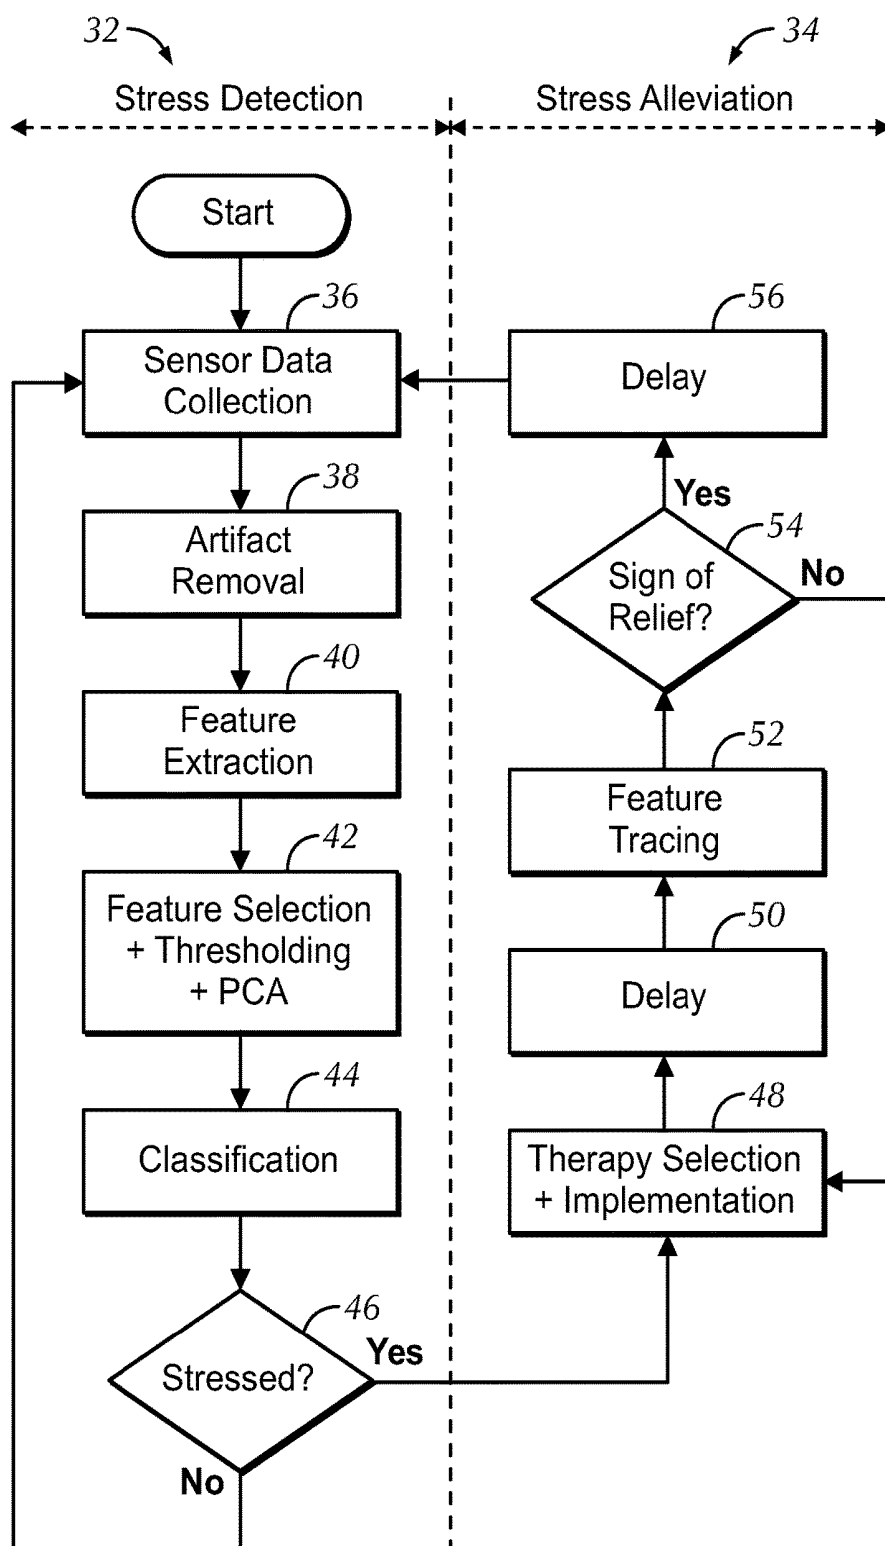


FIG. 3

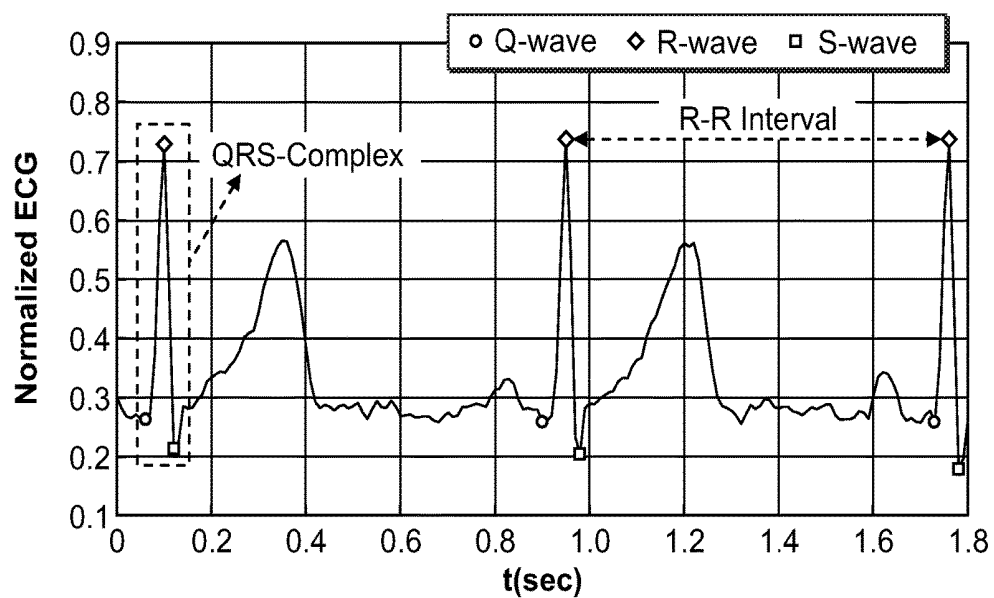


FIG. 4

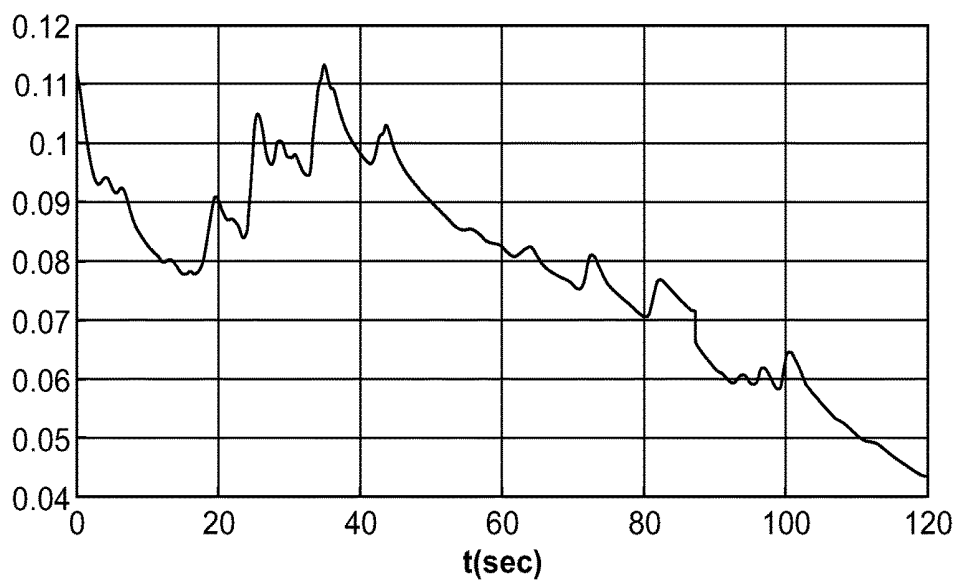


FIG. 5

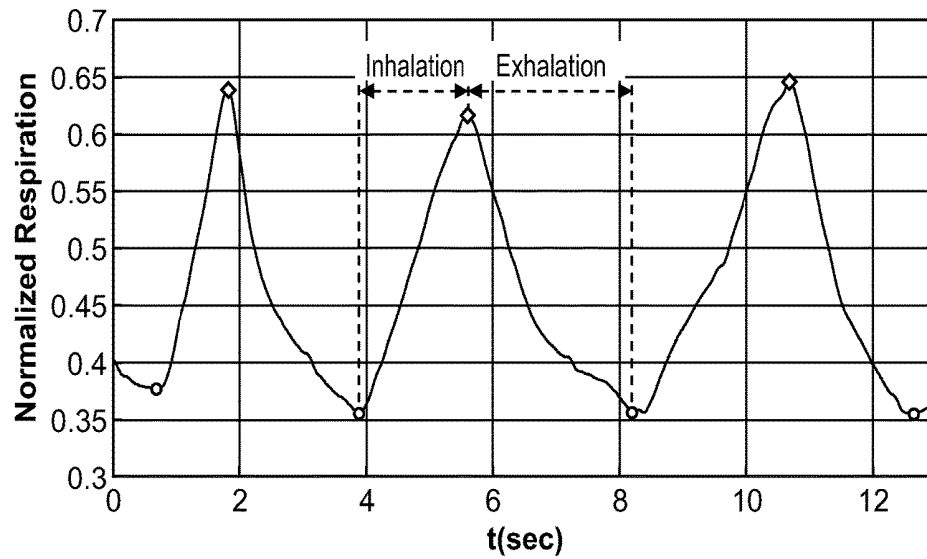


FIG. 6

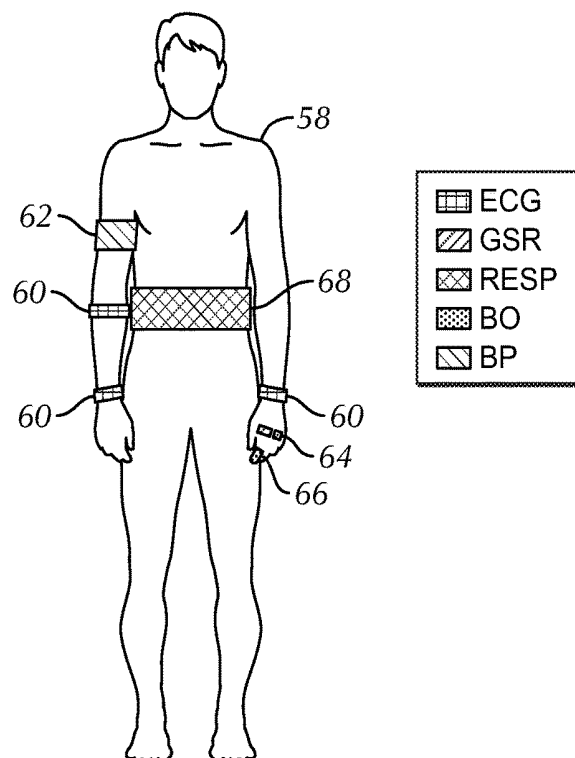


FIG. 7

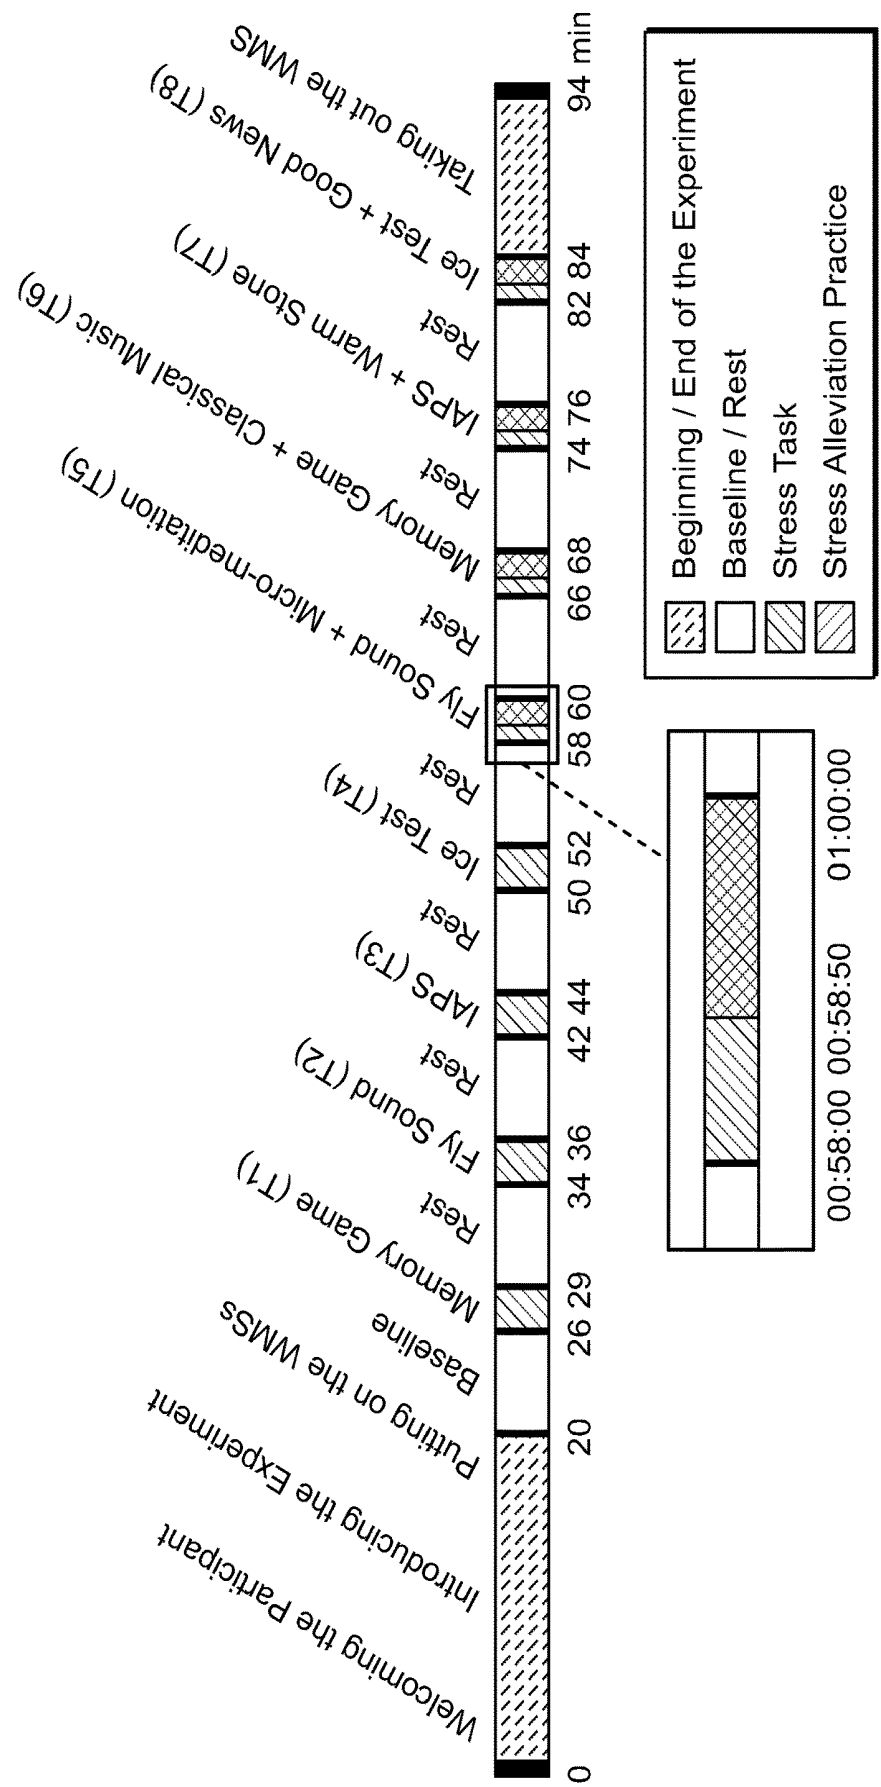


FIG. 8

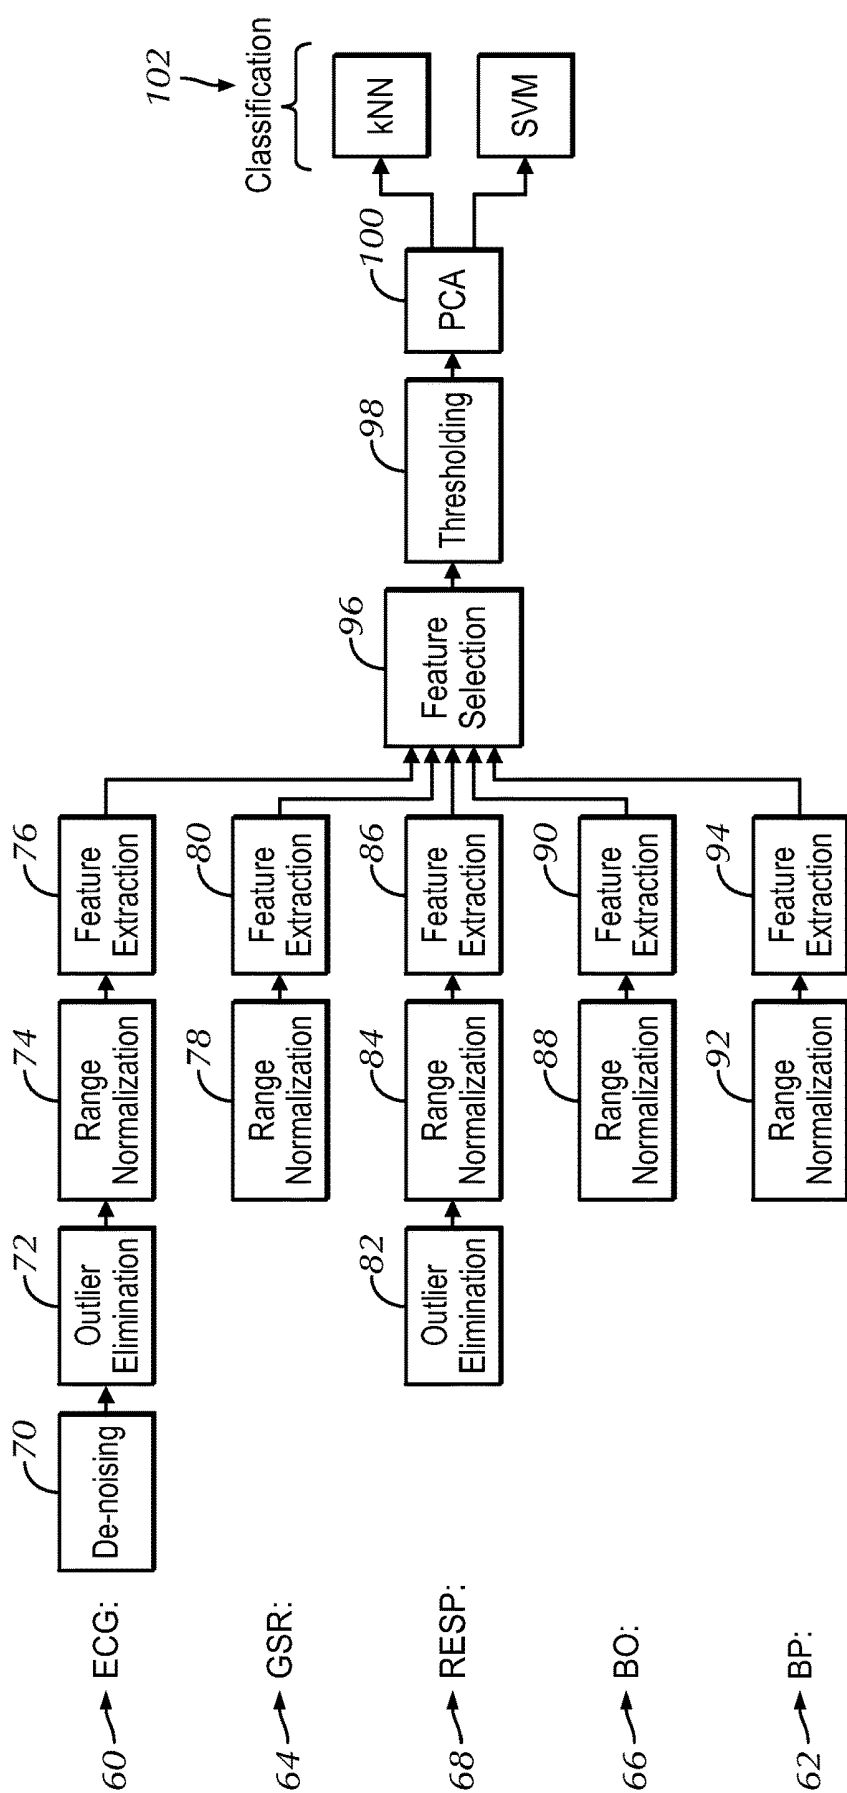
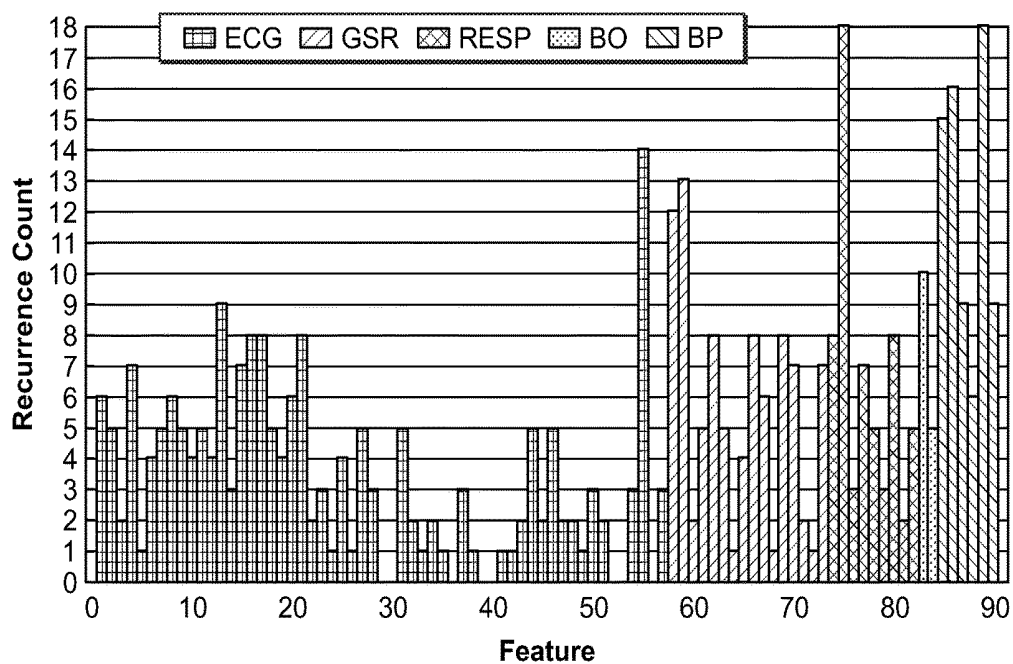


FIG. 9

Sensor	Abbreviation	Unit	Number of Features
Electrocardiogram	ECG	mV	57
Galvanic Skin Response	GSR	mS	16
Respiration	RESP	1/min	9
Blood Oximeter	BO	%	2
Blood Pressure	BP	mmHg	6

FIG. 10**FIG. 11**

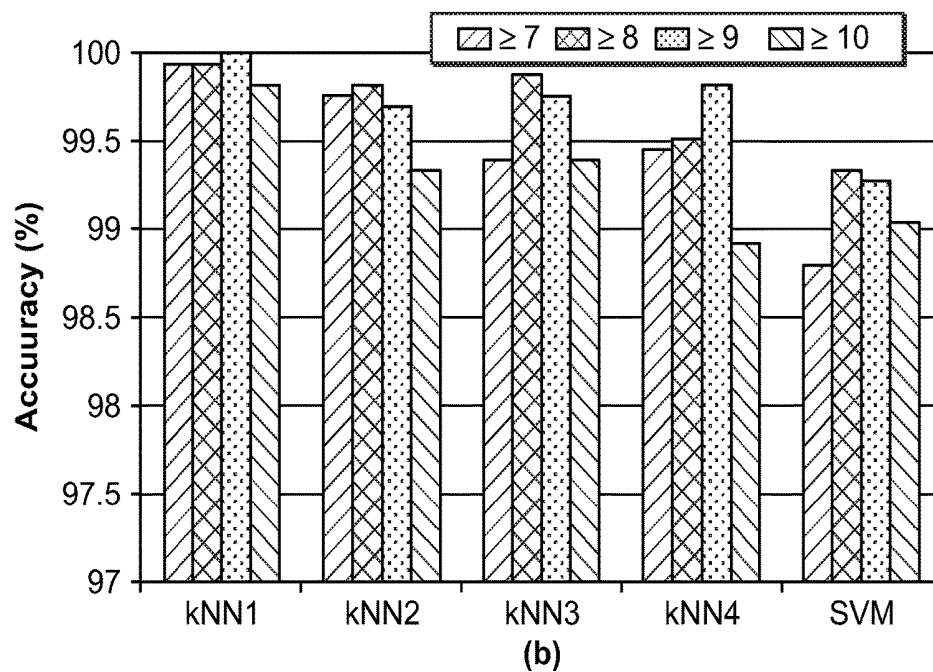
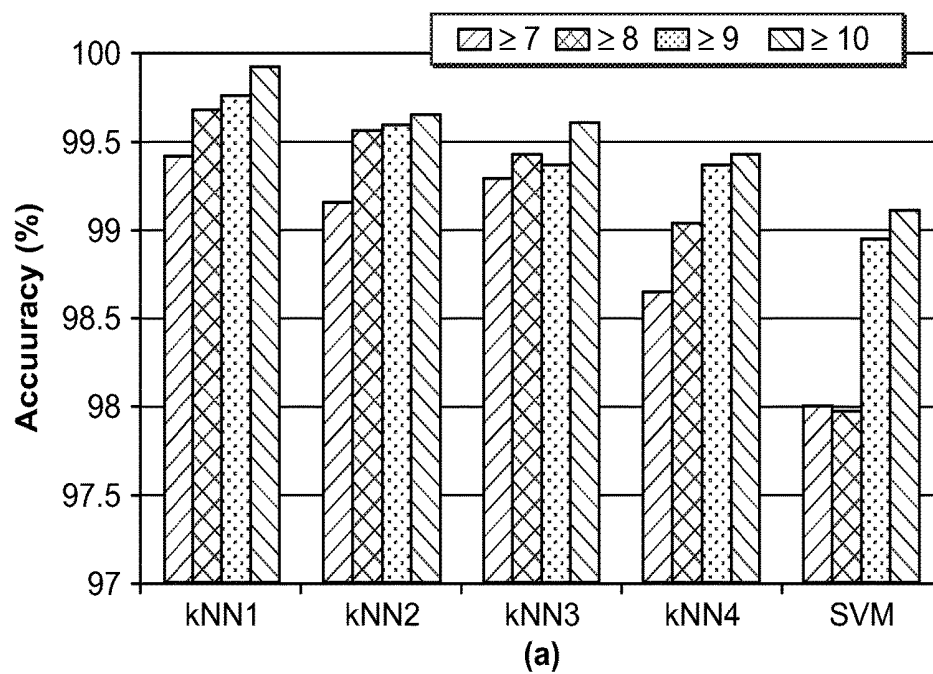



FIG. 12




	Feature	Sensor	Threshold
1	ECG-derived respiration rate	ECG	8.9
2	Mean of skin conductance amplitude	GSR	8.9
3	Standard deviation of skin conductance amplitude	GSR	8.9
4	Sum of amplitudes of skin conductance responses above the threshold (continuous decomposition analysis)	GSR	8
5	Mean of tonic activity	GSR	8
6	Maximum positive deflection	GSR	8
7	Mean of respiration duration	RESP	8
8	RMS of respiration signal	RESP	8.9
9	Median of respiration duration	RESP	8
10	Mean of blood oxygen level	BO	8.9
11	Mean of systolic blood pressure	BP	8.9
12	Variance of systolic blood pressure	BP	8.9
13	Mean of diastolic blood pressure	BP	8.9
14	Mean of MAP	BP	8.9
15	Varaince of MAP	BP	8.9

FIG. 13

	Generalized Model		Individualized Model			
	(≥ 8)	(≥ 9)	(≥ 8)		(≥ 9)	
			Mean	Median	Mean	Median
kNN1	11.0	9.0	8.4	9.0	6.5	6.0
kNN2	11.0	9.0	8.5	9.0	6.7	6.0
kNN3	11.0	9.0	8.5	9.0	6.6	6.0
kNN4	11.0	9.0	8.0	9.0	6.5	6.0
SVM	11.0	9.0	6.7	7.0	6.7	7.0

FIG. 14

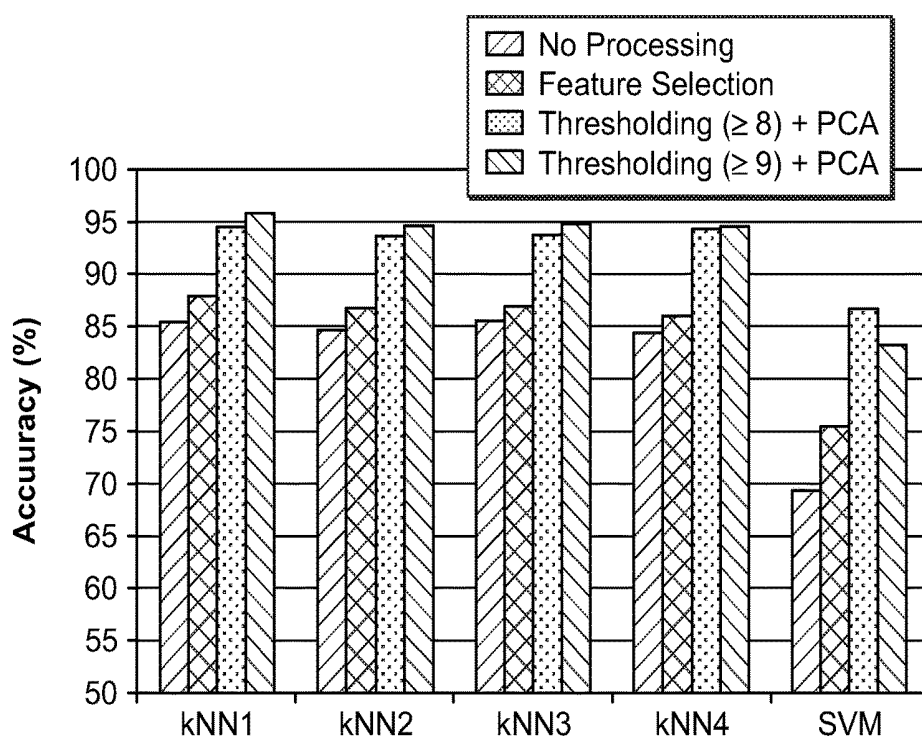**FIG. 15**

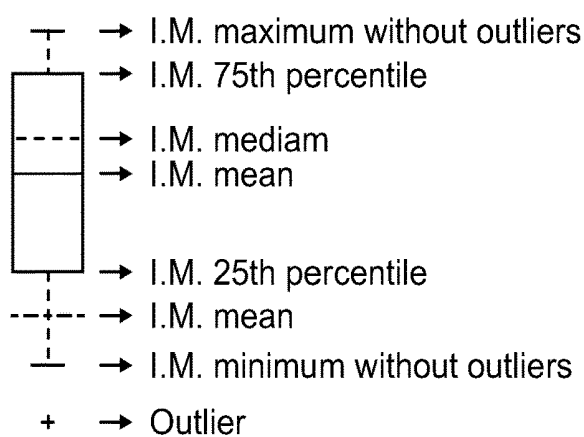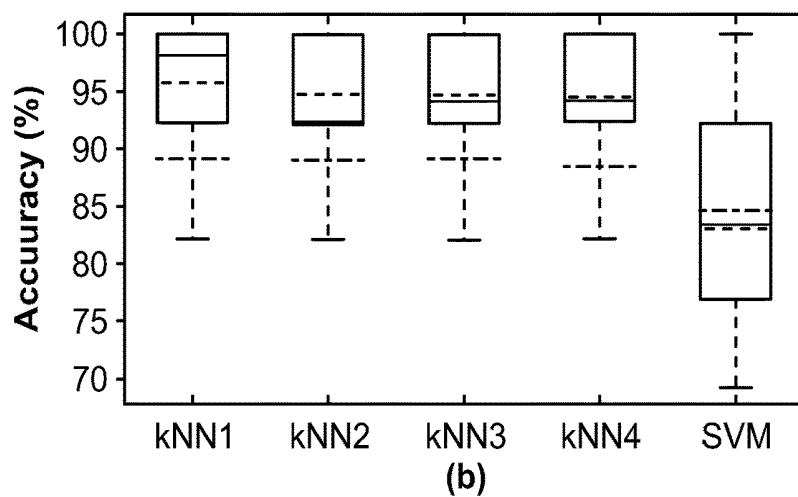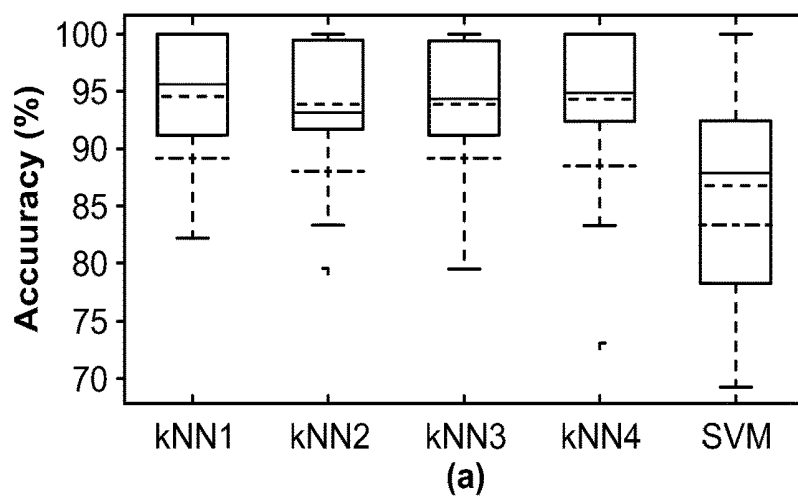

I.M. → Individual Model
G.M. → General Model

(c)

FIG. 16

Sensor	#Features		Timp Elapsed (<i>ms</i>)	
	(≥ 8)	(≥ 9)	Feature Extractionin (≥ 8)	(≥ 9)
ECG	1	1	1.5	1.5
GSR	5	2	11.4	9.9
RESP	3	1	46.1	38.3
BO	1	1	35.3	35.3
BP	5	5	205.2	205.2
Total	15	10	299.5	290.2

FIG. 17

Stress Alleviation Protocol

Given: *therapySet*, set of the stress alleviation techniques.

```

1: therapy  $\leftarrow$  null, k  $\leftarrow$  0, flag  $\leftarrow$  0
2: for i = 1, ..., length(therapySet)
3:   therapy  $\leftarrow$  therapySet(i)
4:   Delay (30sec.)
5:   Compute selected N feature values
6:   Compute k, number of features showing stress
   relief
7:   if k  $\geq$  N/2
8:     Delay (30sec.)
9:     Compute selected N feature values
10:    Compute k
11:    if k  $\geq$  N/2
12:      flag  $\leftarrow$  1
13:    return
14:  end
15: end
16: end
17: if flag = 0, when none of the stress alleviation
   techniques is effective
18: Give warning to the user
19: return
20: end

```

FIG. 18

	Mean		Median		25th		75th	
	T2	T5	T2	T5	T2	T5	T2	T5
R-R	0.52	0.51	0.51	0.48	0.43	0.41	0.59	0.60
HR	0.18	0.19	0.18	0.18	0.13	0.13	0.22	0.24
LF/HF	0.06	0.06	0.03	0.03	0.01	0.01	0.06	0.08
	T3	T7	T3	T7	T3	T7	T3	T7
R-R	0.54	0.52	0.53	0.51	0.42	0.44	0.64	0.62
HR	0.17	0.18	0.16	0.17	0.11	0.12	0.22	0.21
LF/HF	0.06	0.10	0.02	0.03	0.01	0.01	0.06	0.06
	T4	T8	T4	T8	T4	T8	T4	T8
R-R	0.51	0.52	0.49	0.49	0.41	0.42	0.61	0.58
HR	0.19	0.18	0.18	0.18	0.13	0.14	0.23	0.23
LF/HF	0.05	0.07	0.03	0.03	0.01	0.01	0.05	0.07

FIG. 19

	Mean		Median		25th		75th	
	T2	T5	T2	T5	T2	T5	T2	T5
R-R	0.51	0.55	0.47	0.53	0.40	0.42	0.57	0.62
HR	0.21	0.19	0.21	0.18	0.15	0.13	0.26	0.24
LF/HF	0.05	0.05	0.02	0.02	0.01	0.01	0.05	0.04
	T3	T7	T3	T7	T3	T7	T3	T7
R-R	0.54	0.55	0.53	0.55	0.43	0.46	0.62	0.64
HR	0.18	0.19	0.18	0.17	0.13	0.12	0.24	0.22
LF/HF	0.09	0.07	0.03	0.02	0.01	0.01	0.10	0.05
	T4	T8	T4	T8	T4	T8	T4	T8
R-R	0.52	0.55	0.50	0.51	0.40	0.43	0.63	0.68
HR	0.21	0.19	0.20	0.19	0.13	0.11	0.26	0.25
LF/HF	0.05	0.05	0.03	0.03	0.02	0.01	0.07	0.07

FIG. 20

	Mean		Median		25th		75th	
	T2	T5	T2	T5	T2	T5	T2	T5
R-R	0.93	0.93	0.93	0.93	0.86	0.92	1.00	0.94
HR	0.04	0.04	0.04	0.04	0.00	0.04	0.08	0.05
LF/HF	0.00	0.28	0.00	0.28	0.00	0.03	0.01	0.54
Inh	0.34	0.24	0.34	0.24	0.29	0.14	0.40	0.34
	T3	T7	T3	T7	T3	T7	T3	T7
R-R	0.98	1.03	0.98	1.03	0.97	1.00	0.99	1.06
HR	0.02	-0.02	0.02	-0.02	0.01	-0.03	0.02	0.00
LF/HF	0.84	0.13	0.84	0.13	0.69	0.08	1.00	0.19
Inh	0.70	0.55	0.70	0.55	0.39	0.44	1.00	0.65
	T4	T8	T4	T8	T4	T8	T4	T8
R-R	0.82	1.02	0.82	1.02	0.81	0.96	0.83	1.07
HR	0.11	-0.01	0.11	-0.01	0.10	-0.04	0.12	0.02
LF/HF	0.05	0.16	0.05	0.16	0.04	0.09	0.06	0.24
Inh	0.04	0.74	0.04	0.74	0.00	0.60	0.08	0.87

FIG. 21

	Mean		Median		25th		75th	
	T2	T5	T2	T5	T2	T5	T2	T5
R-R	0.93	0.98	0.93	0.98	0.85	0.93	1.00	1.04
HR	0.04	0.01	0.04	0.01	0.00	-0.02	0.09	0.04
LF/HF	0.12	0.31	0.12	0.31	0.04	0.11	0.20	0.51
Inh	0.55	0.28	0.55	0.28	0.09	0.01	1.00	0.55
	T3	T7	T3	T7	T3	T7	T3	T7
R-R	0.97	1.21	0.97	1.21	0.96	1.14	0.98	1.29
HR	0.02	-0.11	0.02	-0.11	0.01	-0.15	0.03	-0.08
LF/HF	0.19	0.06	0.19	0.06	0.00	-0.01	0.38	0.13
Inh	0.52	1.19	0.52	1.19	0.11	0.79	0.92	1.59
	T4	T8	T4	T8	T4	T8	T4	T8
R-R	0.93	1.01	0.93	1.01	0.91	0.96	0.95	1.06
HR	0.04	0.00	0.04	0.00	0.03	-0.03	0.05	0.03
LF/HF	0.10	0.14	0.10	0.14	0.09	0.09	0.10	0.20
Inh	0.27	0.71	0.27	0.71	0.00	0.26	0.53	1.17

FIG. 22

	Generalized Model	Individualized Model
1	Micro-meditation	Warm Stone
2	Good News	Good News
3	Warm Stone	Micro-meditation

FIG. 23

STRESS DETECTION AND ALLEVIATION SYSTEM AND METHOD

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to provisional application 62/442,517, filed on Jan. 5, 2017, which is herein incorporated by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] The present invention relates generally to stress detection and alleviation systems and, more particularly, to a stress relief system that continuously monitors stress levels via data from wearable medical sensors and utilizes machine learning systems based on supervised feature selection, unsupervised dimensionality reduction, and classification to detect and mitigate stress as it arises without the need for user intervention.

[0003] Stress is a serious health problem that afflicts a large fraction of humanity. In the United States, three out of four visits to the doctor are due to stress-related disorders. In Europe, stress is reported to be the second most common health problem. Stress also has a severe adverse impact on the United States' economy. According to the American Institute of Stress (AIS), each year \$300 billion is spent on the treatment of stress-induced disorders.

[0004] Stress can be divided into two parts: stressor and reaction. Stressor is the activity or effect that triggers a change in the physiological parameter values of the human body. Reaction is the deviation of these parameter values from their normal levels. When confronted with a stressor, the body raises an alarm that results in a stress response. The stress response of the body depends on the duration for which the stressor is active. With long and frequent stress responses, a person becomes more likely to develop one or more serious health problems. For example, excessive exposure to stress may result in depression, cardiovascular diseases, sleep disorders, degradation in the immune system, or cancer, as nonlimiting examples. In addition to stressor duration, personal traits also play a significant role in stress response. These traits have an impact on physiological signals, and indirectly on the emotional condition.

[0005] As such, it is desirable to have immediate stress alleviation when a stress response is detected. Stress alleviation should ideally be tailored to the individual to have maximum impact.

SUMMARY OF THE INVENTION

[0006] According to various embodiments, a stress detection and alleviation (SoDA) system for a user is disclosed. The system includes a SoDA device configured with one or more processors that receive wearable medical sensor (WMS) data from a plurality of WMSs. The processors are programmed to remove one or more artifacts from the WMS data, extract a set of features from the WMS data, remove correlated features from the extracted features to obtain a reduced set of features, classify the reduced set of features in order to determine whether the user is stressed, and generate a response based on whether the user is stressed.

[0007] According to various embodiments, a method for stress detection and alleviation (SoDA) for a user of a SoDA device is disclosed. The SoDA device includes one or more processors. The method includes receiving wearable medi-

cal sensor (WMS) data from a plurality of WMSs, removing one or more artifacts from the WMS data, extracting a set of features from the WMS data, removing correlated features from the extracted features to obtain a reduced set of features, classifying the reduced set of features in order to determine whether the user is stressed, and generating a response based on whether the user is stressed.

[0008] According to various embodiments, a non-transitory computer-readable medium having stored thereon a computer program for execution by a processor configured to perform a method for stress detection and alleviation of a user is disclosed. The method includes receiving wearable medical sensor (WMS) data from a plurality of WMSs, removing one or more artifacts from the WMS data, extracting a set of features from the WMS data, removing correlated features from the extracted features to obtain a reduced set of features, classifying the reduced set of features in order to determine whether the user is stressed, and generating a response based on whether the user is stressed.

[0009] Various other features and advantages will be made apparent from the following detailed description and the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] In order for the advantages of the invention to be readily understood, a more particular description of the invention briefly described above will be rendered by reference to specific embodiments that are illustrated in the appended drawings. Understanding that these drawings depict only exemplary embodiments of the invention and are not, therefore, to be considered to be limiting its scope, the invention will be described and explained with additional specificity and detail through the use of the accompanying drawings, in which:

[0011] FIG. 1 is a flowchart of the stress detection and alleviation system according to an embodiment of the present invention;

[0012] FIG. 2 is a block diagram of the stress detection and alleviation system according to an embodiment of the present invention;

[0013] FIG. 3 is a flowchart of the stress detection and alleviation system according to an embodiment of the present invention;

[0014] FIG. 4 is an example of an ECG signal according to an embodiment of the present invention;

[0015] FIG. 5 is an example of a normalized GSR signal according to an embodiment of the present invention;

[0016] FIG. 6 is an example waveform of a respiration signal according to an embodiment of the present invention;

[0017] FIG. 7 is a diagram showing an example of on-body positions of WMSs according to an embodiment of the present invention;

[0018] FIG. 8 is a diagram showing an example experimental procedure according to an embodiment of the present invention;

[0019] FIG. 9 is a flowchart showing data processing according to an embodiment of the present invention;

[0020] FIG. 10 is a table summarizing various details of the WMSs including features extracted according to an embodiment of the present invention;

[0021] FIG. 11 is a graph showing the recurrence count of features according to an embodiment of the present invention;

[0022] FIG. 12 is a graph showing accuracy with respect to recurrence count limits according to an embodiment of the present invention;

[0023] FIG. 13 is a table showing selected feature sets for input to the principal component analysis (PCA) stage according to an embodiment of the present invention;

[0024] FIG. 14 is a table showing PCA reduced dimensions for the generalized embodiment and statistics of reduced dimensions for the individualized embodiment according to embodiments of the present invention;

[0025] FIG. 15 is a chart showing the effect of feature selection, thresholding, and PCA on the accuracy of different classifiers according to an embodiment of the present invention;

[0026] FIG. 16 is a chart showing classification accuracy according to an embodiment of the present invention;

[0027] FIG. 17 is a table showing time elapsed during feature extraction according to an embodiment of the present invention;

[0028] FIG. 18 is a protocol for stress alleviation according to an embodiment of the present invention;

[0029] FIG. 19 is a table showing statistics of physiological signals in a generalized embodiment for 0-50 seconds according to an embodiment of the present invention;

[0030] FIG. 20 is a table showing statistics of physiological signals in a generalized embodiment for 60-120 seconds according to an embodiment of the present invention;

[0031] FIG. 21 is a table showing statistics of physiological signals in an individualized embodiment for 0-50 seconds according to an embodiment of the present invention;

[0032] FIG. 22 is a table showing statistics of physiological signals in an individualized embodiment for 60-120 seconds according to an embodiment of the present invention; and

[0033] FIG. 23 is a table showing the order of stress reduction techniques according to an embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0034] According to various embodiments, disclosed herein is a stress detection and alleviation system (referred to herein as “SoDA”). As shown broadly in FIG. 1, SoDA 10 detects stress and then employs a stress alleviation technique based on the stress characteristics of the person. First, data is collected from wearable medical sensors in block 12, then the data is processed and analyzed in block 14, and then classified in block 16 in order to provide a particular stress alleviation protocol in block 18. The process can continuously repeat itself as stress levels are monitored, as illustrated by the arrows shown in FIG. 1.

[0035] Stress characteristics are deduced from physiological signals obtained through wearable medical sensors (WMSs). WMSs may be utilized for ECG, GSR, respiration rate, blood pressure, and blood oximeter, as nonlimiting examples. However, more sophisticated and other types of WMSs can be easily incorporated into SoDA as and when they become available. Use of WMSs offers several advantages. First, WMSs continuously collect data from the human body, making it possible to detect a stress response quickly. Second, they also enable real-time stress mitigation. Alternatively, since the WMS data are typically communicated to an on-body device, such as a smartphone, and thereon to a health server that is accessible to a doctor, it has

the potential to enhance the ability of a doctor to intervene significantly faster than currently possible. Third, if stress-induced disorders can be significantly reduced, it may bend the national health expenditure curve downwards.

[0036] The stress detection and mitigation system disclosed herein can offer two options to the user: “generalized” and “individualized”. In the generalized embodiment, the system detects and alleviates stress by using a predetermined stress model based on data obtained from a population of individuals. The individualized embodiment is configured based on the particular user’s stress response. The generalized embodiment becomes active just after turning on the system, whereas the individualized embodiment requires training data from the user for modeling purposes. However, the individualized embodiment is more accurate in discerning if the user is stressed since it is trained on WMS data obtained from the user.

[0037] System Overview

[0038] A simplified block diagram of a SoDA system 10 is shown in FIG. 2 according to an embodiment of the present invention. Each element will be discussed in greater detail in the forthcoming sections. SoDA 10 includes one or more wearable medical sensors (WMSs) shown generally by reference number 20. The WMSs may be utilized for ECG, GSR, respiration rate, blood pressure, and blood oximeter, as nonlimiting examples.

[0039] The sensors 20 may be connected to a SoDA device 22 via a network system 24. The sensors 20 may also be integrated into the SoDA device 22 in alternative embodiments. If the sensors 20 are integrated into the SoDA device 22, then a network system 24 is not required. The SoDA device 22 may be implemented in a variety of configurations including general computing devices such as desktop computers, laptop computers, tablets, network appliances, or mobile devices such as mobile phones, smart phones, or smart watches. The SoDA device 22 includes one or more processors 26 for performing specific functions and memory 28 for storing those functions. Particularly, the processors 26 process data received from the sensors 20 to generate stress mitigation data, to be discussed in greater detail in the forthcoming sections. This data may be output via a display 30 on the SoDA device 22.

[0040] The network system 24 may be implemented as a single network or a combination of multiple networks. Network system 24 may include but is not limited to wireless telecommunications networks, WiFi, Bluetooth, Zigbee, or other communications networks. Network system 24 may be a wired network as well.

[0041] A simplified flow chart of the SoDA system 10 is shown in FIG. 3, where each step will be discussed in greater detail in the forthcoming sections. SoDA 10 includes a stress detection section 32 and a stress alleviation section 34. SoDA 10 starts at step 36 with sensor data collection from the one or more sensors 20. After collecting physiological signals from the sensors 20, the SoDA device 22 removes artifacts from the data, i.e., de-noises the data, at step 38. Then, various features are extracted from the data at step 40. Since some of these features may be correlated, not all of them are used for stress classification, since correlations lead to redundancy and may impact stress classification performance negatively. Therefore, at step 42, a reduced set of features is obtained via feature selection, thresholding, and principal component analysis. At step 44, the reduced set of features is classified via machine-learning systems, such as

support vector machine or k-nearest neighbor, as nonlimiting examples. Based on the classified features, at step 46, SoDA 10 queries whether the user is stressed. If no, SoDA 10 returns to the sensor data collection step 36. If yes, SoDA moves to the stress alleviation section 34.

[0042] The stress alleviation section 34 starts with step 48, where a particular stress relief therapy is selected and implemented. Stress relief therapy includes but is not limited to micro-meditation, reading good news, listening to classical music, deep breathing, and repeating words/suggestions in the mind. A brief delay is then implemented at step 50, because stress relief is not instantaneous. After the delay, at step 52, relevant feature values are traced to determine if the user is still stressed. This leads to a query at step 54 whether the user shows signs of stress relief. If, no SoDA 10 returns to step 48 to select and implement a different stress relief therapy. If yes, after a brief delay at 56, SoDA 10 returns to the stress detection section 32 by continuing to collect sensor data at step 36.

[0043] Motivation

[0044] Stress is unavoidable and can be triggered by various events. For example, stressors may lurk at work, in expectations, or simply in various ordinary circumstances, e.g., traffic jams, time pressure, lack of sleep, pollution, inconsiderate people, and excess noise. When exposed to long periods of stress or excessive stress, an individual's health is impacted negatively, becoming more susceptible to lifelong health problems, such as diabetes, hypertension, heart disease, etc. Thus, it is important to detect and alleviate stress as quickly as possible.

[0045] As such, the aim of the system disclosed herein is to continuously track the human stress level and try to maintain it within normal levels. Continuous stress measurement is made possible through inference on WMS data. Based on user preference (generalized or individualized), upon detection of stress, an appropriate sequence of stress reduction techniques is selected and suggested to the user. If the feature values extracted from the WMS data collected after the application of the first stress alleviation technique show a tendency towards a relaxed state, the system stays with the technique; otherwise, it suggests the next technique and reevaluates.

[0046] In the system disclosed herein, SoDA, stress characteristics of the user are modeled with the help of four different stressors. With a distinctive feature selection performed based on WMS data, when the individual is subjected to these stressors, high accuracy in stress detection is obtained. All four stressors are evaluated with and without the stress alleviation techniques. Their impact is evaluated after the participant's stress level attains approximately the same level as just before the application of stress alleviation. While performing the task, the stressor is not removed in the alleviation stage. This enables more realistic and reliable comparisons among the stress alleviation techniques. Moreover, since different individuals may respond in different degrees to various stress alleviation techniques, the system responds to a user's needs adaptively and quickly by selecting the best sequence of such techniques.

[0047] Stress and Health

[0048] Stress is a wide-ranging and complex topic that does not have a specific definition. According to one definition, stress may be the relationship between the person and a situation, which adversely impacts the happiness and health of the sufferer. Another definition of stress is that it is

a physiological reaction that aims to protect the individual from possible threats emanating from the environment. These definitions indicate that stress arises from a threatening situation. An individual's body activates its defense mechanism to adapt to or overcome the stressful circumstance. When the stressor disappears, our body returns to normal operation. However, this recovery takes some time since stress results in chemical changes in the individual's body. Thus, continuous exposure to stress prevents the body from returning to normal, and thus has long-term health consequences, ranging from cardiovascular to psychological problems.

[0049] WMSs and Physiological Parameters

[0050] WMSs are noninvasive and autonomous devices that are used to monitor human health. They are called wearable since they are placed on the human body or clothing. They come in various forms: patches, bandages, glasses, rings, bracelets, as nonlimiting examples. WMSs can monitor posture, fetal health, heart disease, obesity, diabetes, epilepsy, sleep quality, cigarette smoking, etc.

[0051] The physiological parameters related to stress include but are not limited to heart rate, blood pressure, skin conductivity, respiration rate, blood oxygen level, electromyograph (EMG) of trapezius muscles, pupil diameter, and cortisol level. Obtaining heart rate, blood pressure, skin conductivity, respiration rate, and blood oxygen level requires minimal obtrusion. As such, they are the parameters for the preferred embodiment of the disclosed system. However, other parameters may still be utilized in other embodiments.

[0052] Electrocardiogram (ECG):

[0053] An ECG sensor measures the electrical activity of the heart during a cardiac cycle. It is noninvasively obtained by relying on body fluids as conductors and comparing the potential difference between the electrodes. An example of an ECG signal is shown in FIG. 4. A cardiac cycle is composed of P-Q-R-S-T waves. The most detectable part of the ECG signal is the Q-R-S complex. In this complex, the first negative deflection is called the Q-wave, which is followed by a large positive deflection called the R-wave, and the next negative deflection called the S-wave. Generally, the Q-R-S complex lasts for 60-100 milliseconds in adults. From the ECG signal, values for various parameters, such as the heart rate (HR), heart rate variability (HRV), R-R interval, etc., can be derived. Deviations in the values of these parameters in consecutive cycles may indicate stress.

[0054] Galvanic Skin Response (GSR):

[0055] GSR indicates the change in electrical characteristics of the skin due to perspiration from the body. It measures skin conductance (SC) noninvasively by applying a low constant voltage through the electrodes. An example of a normalized GSR signal is shown in FIG. 5. The measured SC is composed of two electrodermal activities: phasic and tonic. Phasic activity is the high frequency component and thus varies quickly, whereas tonic activity is the low frequency component and thus changes more slowly. Stressful situations can cause sweat production, which changes skin conductance.

[0056] Respiration Monitor:

[0057] Respiration is composed of inhalation and exhalation. An example waveform of the respiration signal is shown in FIG. 6. During respiration, oxygen is transmitted to the cells and the accumulated carbon dioxide is removed. The normal respiration rate for adults is 12-16 breaths per

minute. Although respiration rate can be obtained through different methods, the respiration monitor utilized herein measures thoracic expansion to obtain respiratory information. Stressors influence the duration and amplitude of inhalation and exhalation.

[0058] Blood Oximeter:

[0059] A blood oximeter noninvasively measures the blood oxygen level with the help of light-emitting diodes (LEDs). Blood consists of hemoglobin molecules. When these molecules have different oxygen levels, they lead to different levels of absorption of the light emitted through the LEDs. The blood oximeter uses this property to emit light from one side of a fingertip or earlobe and analyzes the received signal emanating from the other side to assess the blood oxygen level. Stress also has an impact on this level.

[0060] Blood Pressure Monitor:

[0061] Blood pressure is the force exerted on blood vessels of the circulatory system. It has two components: systolic and diastolic. Systolic blood pressure indicates the pressure when the heart pumps blood into the arteries, whereas diastolic blood pressure indicates the pressure when the arteries withstand the blood flow. Both systolic and diastolic blood pressures can be obtained through the blood pressure monitor. The normal range for the systolic blood pressure is 90-120 mmHg, and the normal range for the diastolic blood pressure is 60-80 mmHg. In the presence of a stressor, systolic and diastolic blood pressures deviate from their baseline levels.

[0062] Physiological signals may be collected through the five WMSs discussed above: ECG, blood pressure monitor, GSR, respiration monitor, and blood oximeter, in a preferred embodiment of the present invention. However, alternative embodiment may utilize other WMSs. ECG, GSR, and respiration monitor has a sampling rate of 100 Hz, whereas blood oximeter has a sampling rate of 1 Hz. However, other sampling rates may be used in alternative embodiments. Blood pressure is not measured continuously. When the individual performs a stress-inducing task, blood pressure measurements are taken in the beginning, middle, and end. However, for the baseline and individual-under-rest parts of the experiments, to be discussed in further detail below, blood pressure is measured in the beginning and at the end. The body placement of the chosen WMSs takes into account both the comfort of the individual and the accuracy of the measurements. An example of on-body positions of WMSs on an individual **58** are shown in FIG. 7. The ECG **60** and blood pressure monitor **62** are placed on the arms of the individual **58**. The GSR **64** and blood oximeter **66** are placed on the fingers of the individual **58**. The respiratory monitor **68** is placed around the waist of the individual **58**.

[0063] It should be noted that alternative embodiments may have different WMSs, different WMS positions, or have all WMSs integrated into a single WMS sensor platform. Furthermore, alternative embodiments may utilize different physiological signal data as inputs.

[0064] Experimental Procedure for Feature Extraction

[0065] For each participant, the laboratory session took approximately 90 minutes. FIG. 8 summarizes the experimental procedure. The session starts by welcoming and asking the participant to sit on a comfortable chair. Then, the experimental procedure and on-body positions of WMSs are explained to the participant in detail. Once wearing the sensors, the participant is reminded of the importance of silence and correct body posture. The participant is encour-

aged to ask questions. Upon ensuring that the participant is comfortable with the experimental setup and procedure, the experiment commences.

[0066] Baseline:

[0067] This is the first stage of the experiment. It is performed to obtain the original levels of the physiological signals. In this stage, the participant is asked to look at the black screen and relax.

[0068] Rest:

[0069] A rest period is introduced in between two tests to calm the participant down. A stressful task pushes the physiological signals to deviate from their original levels, thus requiring a rest period to recover. As in the baseline stage, the participant is asked to look at the black screen and relax.

[0070] Memory Game:

[0071] This game is played on a computer. The participant is shown 40 cards that are flipped back. Two cards are selected in every round. If the cards match, they remain in the face-up position. If they do not match, then both cards are flipped back and another round commences. The participant is given two minutes to complete this task.

[0072] Fly Sound:

[0073] In this stage, the participant is asked to listen to the sound of a fly buzzing around, with a black screen shown to prevent distraction.

[0074] International Affective Picture System (IAPS):

[0075] In this task, the participant is shown pictures from the IAPS Database. The pictures are selected based on the affective ratings specified in the IAPS Technical Manual. Before displaying the pictures, an informative slide ("Get Ready for the Next Slide") is shown for five seconds. Then, the picture is displayed for seven seconds. This procedure is repeated for a total of 10 pictures. Two sets of tests are performed without (T3) and with (T7) stress mitigation techniques. The corresponding picture numbers for the two sets are as follows:

[0076] Set 1: 1304, 3060, 3170, 3266, 6260, 6313, 9040, 9300, 9413, 9635.

[0077] Set 2: 1525, 3053, 3080, 6520, 9220, 9405, 9410, 9570, 9921, 9940.

[0078] Ice Test:

[0079] In this test, the participant is asked to place the right hand on top of an ice-filled container. In the event of discomfort, the participant is encouraged to raise the hand and place it back on the ice or finish the test. The test is not started until the ice has melted partially.

[0080] Stress Mitigation Techniques

[0081] SoDA offers various stress mitigation techniques: classical music, micro-meditation, warm stone, and good news, as nonlimiting examples. Alternative embodiments may incorporate other stress mitigation techniques as well. In the individualized embodiment, an individual-specific order of these techniques is employed, whereas in the generalized embodiment, a fixed sequence is used for each individual. In order to obtain the most effective sequence, the four stress-inducing tasks are carried out with and without stress alleviation techniques.

[0082] As shown in FIG. 8, in tasks T1-T8, stressors are applied for 0-120 seconds; however, in tasks T5-T8, in addition to the stressors, the alleviation techniques are also employed in the 50-120 second range.

[0083] Classical Music:

[0084] During the memory game (T6), classical music is played starting at the 50th second. The composition set includes but is not limited to Benjamin Godard's "Berceuse" and Frederic Chopin's "Il. Romance".

[0085] Micro-Meditation:

[0086] Micro-meditation is a short-duration practice for nurturing self-awareness. It can be employed in various forms. In the experiment, in the presence of the fly sound stressor (T5), the participant is asked to close the eyes and relax various body parts starting from the feet to face. As before, this technique is employed starting at the 50th second of the task and instructions related to body parts that need to be relaxed are provided during the meditation.

[0087] Warm Stone:

[0088] In this stress mitigation technique, using IAPS pictures as stressors (T7), the participant is asked to hold in the palm a warm stone of size approximately 9×8×2 cm. The stone may be other sizes in other embodiments. The stone is warmed up by placing it in boiling water for two minutes. Then, it is taken out, dried, and placed on its side for another two minutes. At the 50th second of the task, the participant is given the warm stone, with continuing display of selected IAPS pictures on the screen.

[0089] Good News:

[0090] While the participant is performing the ice test, positive and optimistic news are displayed on the screen. Task T8 is started with a black screen. Starting at the 50th second, good news accompanied by a corresponding picture is shown for 10 seconds. A total of seven news items are displayed.

[0091] Preprocessing and Feature Extraction

[0092] To obtain the performance measures, the data obtained from the participants is analyzed. The dataset for each participant is composed of 24×2 minutes of measurements collected through the five WMSs. FIG. 9 shows how the data from these WMSs are processed, as described below.

[0093] ECG 60:

[0094] Processing from the ECG 60 includes the following steps: de-noising 70, outlier elimination 72, range normalization 74, and feature extraction 76.

[0095] The ECG signal needs to be de-noised first at step 70. The de-noising steps target baseline wander, power-line interference, muscle noise, etc. Baseline wander is a very low frequency component that can be caused by perspiration, respiration, and body movements. Given that the lowest observed heart rate is approximately 40 bpm (0.67 Hz), a cut-off frequency of 0.5 Hz is selected. A zero-phase high-pass filter is employed based on this cut-off frequency. In order to remove muscle noise and the aliased components of power-line interference, the FFT of the ECG signal is plotted. When a peak is observed in the absolute FFT, a notch filter is used to remove the noise. The frequency corresponding to the highest amplitude in the peak is selected as the center frequency of the notch filter.

[0096] Following the de-noising step 70, the outliers are replaced with the upper/lower thresholds that are derived from the data in step 72. Moreover, at step 74, range normalization shown in the following equation is carried out to eliminate the variability in the physiological signal levels of the participants.

$$d'_i = \frac{d_i - \min(d)}{\max(d) - \min(d)}$$

[0097] After signal preprocessing is complete, at step 76, a total of 57 ECG features are extracted. This is done by detecting the Q-R-S complex and calculating the corresponding features (e.g., mean, variance, quartile deviation, 80th percentile, etc.) using code implemented in MatLab. For heart rate variability related features, Kubios HRV is utilized. Intervals for frequency domain computations are determined as very low frequency (VLF, 0-0.04 Hz), low frequency (LF, 0.04-0.15 Hz), and high frequency (HF, 0.15-0.4 Hz). Following the computations in MatLab and Kubios, the extracted feature values are combined and stored with the ones obtained through other WMSs.

[0098] GSR 64:

[0099] Processing from the GSR 64 includes the following steps: range normalization 78, and feature extraction 80.

[0100] The data obtained from the GSR sensor 64 are first subjected to range normalization via the same equation above at step 78. Then, mean, median, and standard deviation of the data are calculated using MatLab. Moreover, continuous and discrete decomposition analyses are carried out using Ledalab. A total of 16 features are extracted from GSR data at step 80.

[0101] Respiration Monitor 68:

[0102] Processing from the respiration monitor 68 includes the following steps: outlier elimination 82, range normalization 84, and feature extraction 86.

[0103] The outliers of the data obtained from the respiration monitor are replaced with upper or lower thresholds at step 82. After removing the data artifacts, range normalization is performed with the same equation above at step 84. Then, feature values are calculated using MatLab. From the respiration data, a total of nine features are extracted at step 86: mean, median, and quartile deviation of the respiration duration, root mean square (RMS) of the respiration signal, mean of inhalation and exhalation durations, mean and median of the ratio of inhalation-to-exhalation duration, and mean of stretch.

[0104] Blood Oximeter 66:

[0105] Processing from the blood oximeter 66 includes the following steps: range normalization 88 and feature extraction 90.

[0106] The data obtained from the blood oximeter are also first range-normalized by the above equation at step 88. Then, two features are extracted at step 90: mean and variance.

[0107] Blood Pressure Monitor 62:

[0108] Processing from the blood pressure monitor 62 includes the following steps: range normalization 92 and feature extraction 94.

[0109] This monitor 62 measures the systolic/diastolic pressures and derives the mean arterial pressure (MAP). In order to get comparable feature values across the participants, range normalization as shown above is used in step 92. Then, the corresponding mean and variance are calculated. A total of six features are obtained from the blood pressure measurements at step 94.

[0110] Various details of the WMSs are summarized in FIG. 10, including their abbreviations, units, and the total number of features extracted.

[0111] Feature Selection, Thresholding, PCA, and Classification

[0112] After preprocessing, a total of 90 features from the physiological signals collected by the five WMSs are extracted. Since some of these features may be correlated and correlations lead to redundancy, which impacts classification performance negatively, not all of them are used for stress detection. Hence, the data is divided into three parts: first part for training, second part for validation of chosen parameters, and third part for testing. Supervised attribute selection is applied to the training part using Weka 3.8.0 at step **96**. This includes the steps of forward feature selection and subset evaluation. In forward feature selection, the system starts with an empty set and searches for features in the forward direction in a greedy fashion. In subset evaluation, each feature is analyzed in terms of its individual contribution to accuracy and its redundancy with respect to the other features. The output of attribute selection **96** is a set of features that minimizes redundancy while improving accuracy. This procedure **96** is carried out for each of the participants.

[0113] The reduced set of features obtained thus far is then subjected to principal component analysis (PCA) at step **100**. PCA **100** transforms the input information into a group of new orthogonal variables that are linearly uncorrelated. These variables are called principal components. The first principal component has the largest variance, hence includes the largest amount of information about the input data. The second principal component is orthogonal to the first one and has the second largest possible variance. Under the condition of orthogonality, the remaining components are then calculated. Since the majority of data can be represented by the first n components, the remaining ones can be ignored. This enables compression of the data. Thus, PCA **100** is used to extract the most relevant information from the data, and shown to have a positive effect on classification accuracy.

[0114] For the present embodiment, the most important information has already been extracted through supervised attribute selection. However, due to the finite size of training data available, the optimal feature set obtained based on the training dataset may not be optimal for the testing dataset. In order to address this problem, a thresholding step **98** is included prior to the PCA step **100**. The reduced sets of features from all participants' data are combined and the number of times each feature appears calculated. Only features that appear more than a predefined threshold are selected and provided as input to PCA **100** for dimensionality reduction. This helps to eliminate features that do not carry too much information.

[0115] However, the combined set may include redundant features and the training data may not be enough to determine the optimal feature set. Since PCA **100** is an unsupervised method, it does not take into account the labels of the training data. By calculating orthogonal components and choosing the first n that represent a majority of the data, the negative impact on supervised feature selection of the finite-sized training data is abated. In other words, supervised feature selection **96** is used as a coarse sieve, then PCA **100** is employed as a fine sieve. The number of principal components, n , is determined based on each participant's data separately. The principal components are added one by one to the training data. At the $(n+1)$ -th component, if the

classification accuracy on the validation data does not increase, then n is taken to be the optimal number of principal components.

[0116] The data obtained after the PCA step **100** are fed to the classification stage **102** for each of the participants. Due to their widespread applicability and excellent performance, support vector machine (SVM) and k-nearest neighbor (kNN) are employed for binary classification. However, other classification methods may be implemented in alternative embodiments. In SVM, classification is done by finding a hyperplane that separates the n -dimensional data into two classes and maximizes the margin. However, since the data is not linearly separable here, a radial basis function (RBF) kernel is utilized. The RBF kernel maps the data to a higher-dimensional space where they are linearly separable.

[0117] In kNN, the k-nearest neighbors are determined based on a distance metric (e.g., Euclidean, Minkowski, etc.) and classification is performed using majority voting. In the present embodiment, Euclidean distance is used as the distance measure. Moreover, since the generalized embodiment is obtained by combining each individual's data, the optimal k is different for the individualized and generalized embodiments. Thus, to have comparable results, kNN is performed for a k value spanning **1** to **4**. It should be noted alternative embodiments are not limited to kNN with $k=1, 2, 3$, or 4 . Analysis based on different k values demonstrates the consistent performance of SoDA.

[0118] As such, 90 features were obtained from the physiological data collected by the WMSs and the best subset for each of the participants is obtained. The number of features in this subset ranged from 8 to 22. These reduced sets are combined and the number of times each feature appears is counted. The recurrence count of the features is shown in FIG. **11**. This figure indicates that all five physiological signals are indicators of stress. However, compared with the others, the recurrence count of the ECG features is smaller. This is because the total number of features extracted from ECG outnumbered the number of features extracted from the other four physiological signals. In other words, since ECG features provide more options to choose from, the result is a more spread distribution. To get around this problem, different recurrence count thresholds are used for ECG and GSR+RESP+BO+BP derived features. Only the features that are above these thresholds are found to be useful for a larger set of participants and selected for the modeling of stress.

[0119] In FIG. **12**, the accuracy of the stress detection stage is analyzed for various thresholds of ECG (in FIG. **12(a)**) and GSR+RESP+BO+BP (in FIG. **12(b)**), respectively. Since a threshold of ten for ECG and eight/nine for GSR+RESP+BO+BP lead to the best or near-best accuracy in all the cases, they are chosen as the thresholds. Thus, features with ECG recurrence count of ten or above and GSR+RESP+BO+BP recurrence count of eight/nine or above are selected. However, other thresholds may be chosen in alternative embodiments. The corresponding feature sets are shown in FIG. **13**.

[0120] The selected features are subjected to PCA for dimensionality reduction. In the individualized embodiment, dimensionality reduction is carried out for each participant separately, whereas in the generalized embodiment, the combined dataset is used. After computing the corresponding principal components, the first n components are kept and classification accuracy on the validation data is com-

puted. If the inclusion of the (n+1)th component does not improve the accuracy, n is taken to be the reduced dimension. The reduced dimensions for the generalized embodiment and statistics of reduced dimensions for 32 individualized embodiments are shown in FIG. 14.

[0121] The impact of forward feature selection with subset evaluation and PCA on the classification accuracy is demonstrated in FIG. 15 for kNN (k=1-4) and SVM. The first bar for each classifier represents the case when all 90 features were selected, hence, when no processing was done. Forward feature selection with subset evaluation followed by thresholding and PCA (third and fourth bars) can be seen to have the highest accuracies in all the cases. This is because forward feature selection with subset evaluation and PCA complement each other. Forward feature selection with subset evaluation is a supervised attribute selection method. It takes training data with labels as input and obtains the corresponding feature set.

[0122] However, due to the finite size of the training dataset, this method may eliminate some features that are indicators of stress. In order to overcome this problem, the advantage offered by unsupervised dimensionality reduction is exploited. After combining the reduced feature sets and selecting the ones above the threshold, PCA is applied. In PCA, the labels are not taken into account. Hence, the method is not adversely impacted by the training dataset size.

[0123] Using reduced dimensions, the performance of both the individualized and generalized embodiments are analyzed. The classification accuracy results are shown in boxplots in FIG. 16. FIG. 16(c) shows the definitions of the various boxplot parameters. For the individualized embodiment, the top and bottom of the boxplot indicates 75th and 25th percentiles, respectively. The whiskers show the maximum and minimum values without the outliers. The solid and dashed lines depict the median and mean of the individualized embodiments, respectively. The dotted line depicts the accuracy value for the generalized embodiment. FIGS. 16(a) and 16(b) show the classification results for ECG threshold of ten and GSR+RESP+BO+BP threshold of eight and nine, respectively.

[0124] FIG. 16(a) shows the classification results obtained from kNN1 ($\mu=94.5\%$), kNN2 ($\mu=93.7\%$), kNN3 ($\mu=93.8\%$), kNN4 ($\mu=94.2\%$), and SVM ($\mu=86.7\%$) for an ECG threshold of ten and GSR+RESP+BO+BP threshold of eight. FIG. 16(b) shows the classification results obtained from kNN1 ($\mu=95.8\%$), kNN2 ($\mu=94.7\%$), kNN3 ($\mu=94.8\%$), kNN4 ($\mu=94.5\%$), and SVM ($\mu=83.2\%$) for an ECG threshold of ten and GSR+RESP+BO+BP threshold of nine. For the individualized embodiment, the mean of kNN classification accuracy varies between 93.7 and 94.5 percent in FIG. 16(a), and 94.5 and 95.8 percent in FIG. 16(b). The maximum accuracy (95.8 percent) is obtained when k=1. For SVM, the mean of the classification accuracy is 86.7 percent in FIG. 16(a) and 83.2 percent in FIG. 16(b). However, for the generalized embodiment, the corresponding maximum accuracies are 89.2 and 83.1 percent in FIG. 16(a), and 89.3 and 84.6 percent in FIG. 16(b) for kNN and SVM, respectively. Except for the result for SVM in FIG. 16(b), the individualized embodiment is observed to detect stress with higher accuracy relative to the generalized embodiment. Considering the negative effect of choosing a GSR+RESP+BO+BP threshold of nine in FIG. 15, this result is expected.

[0125] In addition to boxplots in FIG. 10, the 95 percent confidence interval (CI) was also computed for classification accuracies of the individualized embodiment. With an ECG threshold of ten and GSR+RESP+BO+BP threshold of eight, the corresponding 95 percent CIs are (92.5, 96.5 percent) for kNN1, (91.8, 95.6 percent) for kNN2, (91.8, 95.9 percent) for kNN3, (92.0, 96.5 percent) for kNN4, and (83.6, 89.7 percent) for SVM. With an ECG threshold of ten and GSR+RESP+BO+BP threshold of nine, the corresponding 95 percent CIs are (94.0, 97.5 percent) for kNN1, (92.8, 96.5 percent) for kNN2, (92.8, 96.7 percent) for kNN3, (92.4, 96.6 percent) for kNN4, and (79.9, 86.5 percent) for SVM. Both FIG. 16 and the CIs indicate that SoDA provides high stress detection accuracy. The accuracy difference between the two embodiments is due to the fact that stress impacts different individuals in slightly different ways. Thus, a model derived from a population of individuals cannot be expected to be as accurate as the model derived from just the individual.

[0126] SoDA enables stress detection in real-time. As shown in FIG. 17, the stress detection stage requires approximately 0.3 s for computing the feature values from WMS data. The measurements are based on a MacBook Pro with a 2.5 GHz Intel Core i7 processor. Since WMS data are continuously collected, this enables the system to provide real-time stress tracking.

[0127] Stress Alleviation

[0128] If stress is detected, SoDA offers stress therapy and modifies the stress alleviation protocol based on the data collected. FIG. 18 shows the stress alleviation protocol. After the user makes use of the suggested stress mitigation technique, the relevant feature values are traced. If these newly obtained feature values have a tendency towards the 'no stress' case, SoDA continues to suggest the current stress mitigation technique for a period of time; otherwise, it suggests the next technique. This period of time can be modified by the user. According to the protocol in FIG. 18, when the stress alleviation technique is observed to reduce stress level for 60 s, the system transitions to the stress detection stage, and checks the user's stress level. If the user is classified as 'stressed' again, then the stress alleviation stage continues with the stress reduction technique.

[0129] To determine whether the proposed technique is working or not, a majority vote based on all the selected feature value trends is carried out. The feature set used in this stage is not the same with the features used for stress detection. This is because not all features behave the same way when a stressor is applied versus when stress mitigation is applied. For example, even when the body begins to relax, the impact on blood pressure is not immediate. Hence, features derived from blood pressure are not used in the stress alleviation step. In this case, feature values should have an immediate response and should be robust to biological differences. Thus, the features that are appropriate for indicating stress alleviation are selected separately using a feature selection process similar to the one used for stress detection. The aim of stress mitigation techniques is to help the user reach a relaxed state faster than when no such therapeutic technique is employed.

[0130] The features that were found to be the most reliable and robust to biological differences at this stage were: R-R interval, heart rate (HR), and ratio of low frequency to high frequency band power (LF/HF) of the ECG signal. Hence, they were chosen for the generalized embodiment. However,

for the individualized embodiment, the system is designed to be more flexible. It allows the choice of additional features to respond to the needs of the user more effectively. After the application of stress therapy, if SoDA finds the traced values of the selected features indicate recovery from stress, the therapy is continued. Otherwise, the next stress reduction technique is suggested to the user.

[0131] FIGS. 19 and 20 show various statistics derived from the physiological signals for the generalized embodiment. For the three selected features, the statistics are derived over the 0-50 s and 60-120 s intervals. In the case of tasks T1-T4, no stress therapy is employed for the duration (120 s) of the stressful task. However, in the case of tasks T5-T8, starting from the 50th second, stress alleviation technique is used, however, without removing the stressor from the environment. Since stress mitigation needs some time to have an impact, the feature values are calculated 10 s after the start of the therapy.

[0132] First, in order to compare the effectiveness of the stress mitigation techniques, feature values are calculated for the 0-50 s duration for both without and with therapy cases. Since the therapy does not start until the 50th second, these values can be expected to be approximately equal for the same tasks. In other words, the same tasks should stress the participant to the same degree. Fly sound, IAPS, and ice test were verified to satisfy this condition. However, when the physiological signals were analyzed for task T1 (memory game), it was observed that the participants had an excessive stress response. This may have been because memory game was the first task the participants carried out. Even though the participants wore the sensors for some time to become comfortable with them and were given practice tests, their stress levels were different for the practice and real tests. Thus, their stress responses were different the first time they were asked to play the memory game (task T1) and the second time (task T6). Due to this reason, the effectiveness of the corresponding stress alleviation technique (classical music) could not be analyzed.

[0133] For the remaining therapies, when the stress mitigation techniques provide better results than the 'no therapy' case, the data are shown in non-italicized form, else in italicized, in FIGS. 19 and 20. Increase in the R-R interval and decrease in HR and LF/HF indicate a more relaxed state. Within the same time interval, if the stress mitigation techniques bring these feature values to a more relaxed state, then the corresponding techniques can be concluded to be more effective than the 'no therapy' case. In general, the remaining three stress mitigation techniques were verified to be effective.

[0134] Next, the order of effectiveness for the stress mitigation techniques was analyzed. Considering the mean of the feature values, FIGS. 19 and 20 show that both micro-meditation (T5) and good news (T8) are effective. In the case of warm stone therapy, the heart rate is not observed to indicate fast relief compared to 'no therapy' even though the other two feature values do. Hence, warm stone is rated (at least for the generalized embodiment) the lowest. Between micro-meditation and good news, since micro-meditation increases the R-R interval more, it is ranked higher.

[0135] A similar analysis is performed for the individualized embodiment. The results for one of the participants are shown in FIGS. 21 and 22. As in the generalized embodiment, the corresponding feature values are expected to be close to each other for 0-50 s (in columns T2-T5, T3-T7, and

T4-T8). However, due to the smaller amount of data available for a sole individual in the individualized embodiment, the corresponding feature values are not as close as in the case of the generalized embodiment. Still, since the corresponding values are comparable, the analysis of stress reduction techniques is carried out. In the individualized embodiment, as the system collects more data, it models the stress characteristics of the user more precisely. The individualized embodiment also provides an opportunity to include more features that are suitable to the individual in question. This also means that the therapy order can now be tailored to the individual. For example, inhalation duration was an additional feature that was found to be useful for this individual. Increase in the inhalation duration indicates reduced stress. Based on the bolded values in FIGS. 21 and 22, the best order for this individual can be concluded to be: warm stone (T7), good news (T8), and micro-meditation (T5).

[0136] As shown in FIG. 23, since the order is different from the generalized embodiment, the advantage of personalized stress therapy is evident. In other words, if the user selects the individualized embodiment, the recovery becomes faster than if the generalized embodiment is selected. However, as can be seen from FIGS. 19-22, either of the options provides faster relief than the 'no therapy' alternative.

ADVANTAGES

[0137] SoDA includes both stress detection and alleviation stages. The overall system is shown to respond in real-time with 95.8% stress detection accuracy. For the stress alleviation stage, the system is compared with the 'no therapy' baseline. For both the 'no therapy' baseline and stress alleviation stages, the same stressors are applied for the same time interval. Since the stress alleviation stage is found to provide faster relief, its effectiveness is verified. SoDA enables both automatic stress detection and alleviation in a user-transparent manner, and provides quantitative evaluations using multiple WMSs, stressors, and therapies. It also offers high classification accuracy.

[0138] As such, disclosed herein is an automatic stress detection and alleviation system that is adaptive and requires minimum user involvement. The system was designed, implemented, and analyzed with multiple options and stress mitigation techniques. The system was shown to be capable of responding to and reducing the stress level of its user more effectively than when 'no therapy' option is used. SoDA can provide two options to its user: 'individualized' and 'generalized'. The 'individualized' embodiment is more accurate (95.8% as opposed to 89.3% for the 'generalized' embodiment). However, it requires physiological training data to be collected from the user for the derivation of the model. The 'generalized' embodiment can be used as is.

[0139] It is understood that the above-described embodiments are only illustrative of the application of the principles of the present invention. The present invention may be embodied in other specific forms without departing from its spirit or essential characteristics. All changes that come within the meaning and range of equivalency of the claims are to be embraced within their scope. Thus, while the present invention has been fully described above with particularity and detail in connection with what is presently deemed to be the most practical and preferred embodiment of the invention, it will be apparent to those of ordinary skill

in the art that numerous modifications may be made without departing from the principles and concepts of the invention as set forth in the claims.

What is claimed is:

1. A stress detection and alleviation (SoDA) system for a user comprising a SoDA device configured with one or more processors that receive wearable medical sensor (WMS) data from a plurality of WMSs, the processors being programmed to:

remove one or more artifacts from the WMS data;
extract a set of features from the WMS data;
remove correlated features from the extracted features to obtain a reduced set of features;
classify the reduced set of features in order to determine whether the user is stressed; and
generate a response based on whether the user is stressed.

2. The system of claim 1, wherein the WMS data comprises electrocardiogram (ECG) data, Galvanic skin response (GSR) data, respiration rate data, blood pressure data, and blood oximeter data.

3. The system of claim 1, wherein the removing the correlated features further comprises thresholding and principal component analysis.

4. The system of claim 1, wherein classifying the reduced set of features comprises utilizing support vector machine (SVM) or k-nearest neighbor (kNN) techniques.

5. The system of claim 1, wherein generating a response further comprises selecting a stress mitigation technique.

6. The system of claim 5, wherein the stress mitigation technique comprises one of listening to classical music, practicing micro-meditation, holding a warm stone, and receiving good news.

7. The system of claim 5, wherein generating a response further comprises monitoring the user's response to the selected stress mitigation technique.

8. The system of claim 7, wherein generating a response further comprises selecting a new stress mitigation technique based on the user's response to the first selected stress mitigation technique.

9. A method for stress detection and alleviation (SoDA) for a user of a SoDA device, the SoDA device including one or more processors, the method comprising:

receiving wearable medical sensor (WMS) data from a plurality of WMSs;
removing one or more artifacts from the WMS data;
extracting a set of features from the WMS data;
removing correlated features from the extracted features to obtain a reduced set of features;
classifying the reduced set of features in order to determine whether the user is stressed; and
generating a response based on whether the user is stressed.

10. The method of claim 9, wherein the WMS data comprises electrocardiogram (ECG) data, Galvanic skin response (GSR) data, respiration rate data, blood pressure data, and blood oximeter data.

11. The method of claim 9, wherein the removing the correlated features further comprises thresholding and principal component analysis.

12. The method of claim 9, wherein classifying the reduced set of features comprises utilizing support vector machine (SVM) or k-nearest neighbor (kNN) techniques.

13. The method of claim 9, wherein generating a response further comprises selecting a stress mitigation technique.

14. The method of claim 13, wherein the stress mitigation technique comprises one of listening to classical music, practicing micro-meditation, holding a warm stone, and receiving good news.

15. The method of claim 13, wherein generating a response further comprises monitoring the user's response to the selected stress mitigation technique.

16. The method of claim 15, wherein generating a response further comprises selecting a new stress mitigation technique based on the user's response to the first selected stress mitigation technique.

17. A non-transitory computer-readable medium having stored thereon a computer program for execution by a processor configured to perform a method for stress detection and alleviation of a user, the method comprising:

receiving wearable medical sensor (WMS) data from a plurality of WMSs;
removing one or more artifacts from the WMS data;
extracting a set of features from the WMS data;
removing correlated features from the extracted features to obtain a reduced set of features;
classifying the reduced set of features in order to determine whether the user is stressed; and
generating a response based on whether the user is stressed.

18. The medium of claim 17, wherein the WMS data comprises electrocardiogram (ECG) data, Galvanic skin response (GSR) data, respiration rate data, blood pressure data, and blood oximeter data.

19. The medium of claim 17, wherein the removing the correlated features further comprises thresholding and principal component analysis.

20. The medium of claim 17, wherein classifying the reduced set of features comprises utilizing support vector machine (SVM) or k-nearest neighbor (kNN) techniques.

21. The medium of claim 17, wherein generating a response further comprises selecting a stress mitigation technique.

22. The medium of claim 21, wherein the stress mitigation technique comprises one of listening to classical music, practicing micro-meditation, holding a warm stone, and receiving good news.

23. The medium of claim 21, wherein generating a response further comprises monitoring the user's response to the selected stress mitigation technique.

24. The medium of claim 23, wherein generating a response further comprises selecting a new stress mitigation technique based on the user's response to the first selected stress mitigation technique.

* * * * *

专利名称(译)	压力检测和缓解系统和方法		
公开(公告)号	US20180184901A1	公开(公告)日	2018-07-05
申请号	US15/857981	申请日	2017-12-29
[标]申请(专利权)人(译)	普林斯顿大学		
申请(专利权)人(译)	普林斯顿大学的受托人		
当前申请(专利权)人(译)	普林斯顿大学的受托人		
[标]发明人	AKMANDOR AYTEN OZGE JHA NIRAJ K		
发明人	AKMANDOR, AYTEN OZGE JHA, NIRAJ K.		
IPC分类号	A61B5/00 A61B5/16 A61B5/024		
CPC分类号	A61B5/0006 A61B5/165 A61B5/02405 A61B5/0024 A61B5/4884 G16H50/30 A61B5/02438 G16H10/60 A61B5/0205 A61B5/4836 A61B5/4848 G16H20/70 G16H40/63 G16H40/67 G16H50/20 G16H50/70		
优先权	62/442517 2017-01-05 US		
外部链接	Espacenet USPTO		

摘要(译)

根据各种实施例，公开了一种用于用户的压力检测和缓解（SoDA）系统。该系统包括配置有一个或多个处理器的SoDA设备，所述处理器从多个WMS接收可穿戴医疗传感器（WMS）数据。处理器被编程为从WMS数据中移除一个或多个工件，从WMS数据中提取一组特征，从提取的特征中移除相关特征以获得减少的特征集，对减少的特征集进行分类以便确定用户是否有压力，并根据用户是否有压力生成响应。

