



(11) **EP 2 097 010 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
05.10.2011 Bulletin 2011/40

(51) Int Cl.:
A61B 8/14 ^(2006.01) **G01N 21/17** ^(2006.01)
A61B 5/00 ^(2006.01) **A61B 8/08** ^(2006.01)
G01S 7/52 ^(2006.01)

(21) Application number: **07859456.1**

(86) International application number:
PCT/IB2007/055231

(22) Date of filing: **19.12.2007**

(87) International publication number:
WO 2008/075299 (26.06.2008 Gazette 2008/26)

(54) **COMBINED PHOTOACOUSTIC AND ULTRASOUND IMAGING SYSTEM**

KOMBINIERTES PHOTOAKUSTISCHES UND ULTRASCHALL-DARSTELLUNGSSYSTEM
SYSTÈME D'IMAGERIE PHOTOACOUSTIQUE ET ULTRASONORE COMBINÉE

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE
SI SK TR**

(30) Priority: **19.12.2006 US 870713 P**

(43) Date of publication of application:
09.09.2009 Bulletin 2009/37

(73) Proprietor: **Koninklijke Philips Electronics N.V.
5621 BA Eindhoven (NL)**

(72) Inventor: **BURCHER, Michael
Briarcliff Manor, NY 10510-8001 (US)**

(74) Representative: **Kroeze, Johannes Antonius
Philips
Intellectual Property & Standards
P.O. Box 220
5600 AE Eindhoven (NL)**

(56) References cited:
EP-A- 1 561 424

- **SIMON CLAUDIO ET AL: "Motion compensation algorithm for non-invasive two-dimensional temperature estimation using diagnostic pulse-echo ultrasound" PROC SPIE INT SOC OPT ENG; PROCEEDINGS OF SPIE - THE INTERNATIONAL SOCIETY FOR OPTICAL ENGINEERING 1998, vol. 3249, 1998, pages 182-192, XP002479483**
- **FRENZ M ET AL: "Combined Ultrasound and Optoacoustic System for Real-Time High-Contrast Vascular Imaging in Vivo" IEEE TRANSACTIONS ON MEDICAL IMAGING, IEEE SERVICE CENTER, PISCATAWAY, NJ, US, vol. 24, no. 4, 1 April 2005 (2005-04-01), pages 436-440, XP011129441 ISSN: 0278-0062**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 097 010 B1

Description

[0001] The present disclosure relates to systems and methods related to photoacoustic and ultrasound imaging.

[0002] Photoacoustic (PA) tomography is an emerging medical imaging modality. (See, e.g., S. Manohar, A. Kharine, J. C. G. van Hespén, W. Steenbergen, and T. G. van Leeuwen, "The Twente Photoacoustic Mammoscope: System Overview and Performance," *Physics in Medicine and Biology*, Vol. 50, No. 11, pp. 2543-2557, June 2005; M. Xu and L. Wang, "Universal back-projection algorithm for photoacoustic computer tomography," *Physical Review E*, Vol. 71, No. 1, pp. 16706, 2005.) Typically, a short laser pulse is fired at an object of interest (for example, human or animal tissue). Laser energy is absorbed by structures within the object, causing a rapid temperature increase and thermal expansion. This thermal expansion causes ultrasound waves to propagate through the object, where they are received by ultrasound transducers positioned on the surface of the object. These signals can be beamformed in order to produce an image of the object's absorption at the wavelength of the laser. Since the laser radiation is scattered within the object, the illumination is not strongly focused, and an image can be formed from a single laser pulse. In order to increase the signal to noise ratio (SNR), several of these images may be averaged.

[0003] Ultrasound imaging is an established medical imaging modality. Images are formed by transmitting focused pulses of ultrasound energy into the body. The pulses are reflected by boundaries between structures within the body. The reflections propagate back to the ultrasound transducer and are then beamformed to create one A-line. Each transmission is used to form one line of the ultrasound image. An ultrasound image is therefore formed by multiple transmissions.

[0004] Recently, there has been an interest in performing photoacoustic imaging combined with ultrasound imaging. (J. Niederhauser, M. Jaeger, R. Lemor, P. Weber, and M. Frenz, "Combined Ultrasound and Optoacoustic System for Real-Time High-Contrast Vascular Imaging In Vivo," *IEEE Transactions on Medical Imaging*, Vol. 24, No. 4, pp. 436-440, April 2005.) So far, these systems have operated in two modes: producing either photoacoustic or ultrasound images, depending on the selected mode, even though much of the hardware and processing is common to both types of imaging.

[0005] Researchers have described systems where the images from the two modalities are displayed side-by-side. (See, e.g., J. Niederhauser, M. Jaeger, R. Lemor, P. Weber, and M. Frenz, "Combined Ultrasound and Optoacoustic System for Real-Time High-Contrast Vascular Imaging In Vivo," *IEEE Transactions on Medical Imaging*, vol. 24, no. 4, pp. 436-440, April 2005.) The problem with this arrangement is that it can be hard to identify features in the two images which originate from the same anatomical structure.

[0006] The frame rate of the PA image is limited by the pulse repetition rate of the laser and the (possible) need to average several pulses to achieve a sufficient signal-to-noise ratio. The pulse repetition rate for a typical laser is 10 Hz. This is therefore the maximum frame rate of the PA images. Averaging will reduce it. This is a significantly lower rate than the ultrasound. Ultrasound frame rates are typically 60 Hz for an imaging depth of 10 cm and 128 image lines. If the PA images and ultrasound images are acquired in an interleaved fashion, then the rates may be reduced accordingly. For example, if PA images are acquired at 10Hz, then the ultrasound frame rate would be reduced by 5Hz to 55 Hz.

[0007] The relatively low frame rate of PA images can make combining different PA frames difficult. This needs to occur when several PA frames are averaged, or PA frames acquired with different wavelengths are compared. (See, e.g., X. Wang, Y. Pang, G. Ku, X. Xie, G. Stoica, and L. Wang, "Noninvasive laser-induced photoacoustic tomography for structural and functional in vivo imaging of the brain," *Nature Biotechnology*, Vol. 21, No. 7, pp. 803-806, July 2003.) The object being imaged (for example, the human body or a small animal) may move between the times when the two frames are acquired. If the frames are being averaged, this will reduce the spatial resolution of the resulting image. If the frames correspond to different laser wavelengths, then the motion will cause misregistration and possibly artifacts, as shown in Figure 1(b).

[0008] Referring to Figures 1(a) and 1(b), artifacts resulting from incorrect registration of PA frames acquired with different wavelengths (λ_1 and λ_2) are displayed. The graphs represent a cross-section through an image. The abscissa is the pixel value. In Figure 1(a), the two frames are correctly registered. The correct ratio between the images at the two wavelengths is shown in black. In Figure 1(b), the λ_2 frame has been shifted due to motion during the time between frames. The ratio is now incorrect and shows a large artifactual value at the 4th and 5th samples.

[0009] EP 1 561 424 discloses a non-invasive diagnostic imaging method and apparatus with light containing a specific wavelength and ultrasonic waves.

[0010] "Motion compensation algorithm for non-invasive two-dimensional temperature estimation using diagnostic pulse-echo ultrasound", by C. Simon, P. Van-Baren, and E. Ebbini, SPIE Vol. 3249, pp. 182-192, discloses an imaging system based on pulse-echo ultrasound scanning.

[0011] Accordingly, a need exists for an effective image combining system for PA and ultrasound images. These and other needs are addressed and/or overcome by the assemblies and methods of the present disclosure.

[0012] The present disclosure provides systems and methods for generating photoacoustic images and ultrasound images in real time. A system associated with the present disclosure includes: (a) a means for generating photoacoustic signals; (b) at least a first transducer

adapted to: (i) transmit ultrasound waves; (ii) receive ultrasound signals generated from the ultrasound waves; and (iii) receive photoacoustic signals generated from the photoacoustic signal means; (c) a motion estimator adapted to estimate motion based on the ultrasound signals; and (d) an image combiner adapted to receive and combine ultrasound data, photoacoustic data and motion estimator data generated from the received ultrasound and photoacoustic signals and the motion estimator and correct for motion to generate at least a photoacoustic image. The photoacoustic image may be corrected for motion by the image combiner using the motion estimator data. An exemplary image combiner is adapted to receive and combine ultrasound data, photoacoustic data and motion estimator data generated from the received ultrasound and photoacoustic signals and the motion estimator to generate a combined image.

[0013] In an exemplary system according to the present disclosure, combined images are received by a frame buffer adapted: (i) to store combined image output generated from the image combiner, and (ii) transmit the combined image to a display means. Typically, the photoacoustic signal means is accomplished by an illumination system adapted to generate a photoacoustic signal within a sample. Generally, the illumination system is characterized by an energy beam, such as a laser. The display means can be any display system, typically used for medical imaging such as an LCD or a CRT.

[0014] In an exemplary embodiment, the frame buffer is adapted to transmit a series of combined images at a rate of about 55 Hz. Typically, the received ultrasound signals are beamformed by an ultrasound beamformer to create a series of radio frequency signals. A portion of the radio frequency signals are received by the motion estimator and the remaining portion are detected and pass through an ultrasound scan converter to generate an ultrasound image adapted to be received by the image combiner. In an exemplary embodiment, all the radio frequency signals are received by the motion estimator when generating only PA images to correct for motion distortion in the PA imaging. Generally, the ultrasound signal pathway includes passing through a series of stages including filtering, detection and compounding. The motion estimator is adapted to generate a compensation signal to be received by the image combiner. An exemplary image combiner associated with the present disclosure is adapted to receive ultrasound image signals at a rate of about 55 Hz.

[0015] In an exemplary embodiment, the received photoacoustic signals pass through a photoacoustic scan converter adapted to generate a photoacoustic image to be received by the image combiner. An exemplary image combiner according to the present disclosure is adapted to receive photoacoustic image signals at a rate of about 10 Hz. Typically, the motion estimator is adapted to estimate motion of an object based on the portion of radio frequency signals. In an exemplary embodiment, ultrasound signals can be generated in a pulsed Doppler

mode.

[0016] An exemplary image combiner according to the present disclosure is adapted to generate a sequence of combined frames containing data resulting from the received ultrasound signals and data resulting from the received photoacoustic signals. The sequence of combined frames is transmitted to a frame buffer. The image combiner should be adapted to perform spatial and temporal interpolation and resampling of the received photoacoustic signals. Typically, the image combiner is adapted to generate an output frame based on a combination of pixel values of at least one ultrasound image and at least one photoacoustic image.

[0017] In an exemplary embodiment, the display means is adapted to allow different images to be spatially registered, such that corresponding anatomical features in each image can be identified. The display means is adapted to display images in a displaying option selected from the group consisting of: displaying photoacoustic images only, displaying photoacoustic images and ultrasound images next to one another, overlaying a photoacoustic image on to an ultrasound image, using Doppler information to select which photoacoustic pixels are displayed, and combining Doppler and photoacoustic oxygenation information.

[0018] The present disclosure describes a method of combining images of a sample including: (a) illuminating a sample with an illumination system adapted to generate photoacoustic signals; (b) transmitting ultrasound waves to the sample with an ultrasound transmitting means adapted to receive ultrasound signals and photoacoustic signals; (c) generating ultrasound images from a portion of the received ultrasound signals via an ultrasound imaging means; (d) generating a motion estimation from a remaining portion of the received ultrasound signals via a motion estimator; (e) generating photoacoustic images from the received photoacoustic signals via a photoacoustic imaging means; and (f) combining the ultrasound images, the motion estimation and the photoacoustic images in an image combiner adapted to transmit the combined image to a display means.

[0019] Additional features, functions and benefits of the disclosed systems and methods will be apparent from the description which follows, particularly when read in conjunction with the appended figures.

[0020] To assist those of ordinary skill in the art in making and using the disclosed systems and methods, reference is made to the appended figures, wherein:

Figure 1(a) and Figure 1(b) are graphs illustrating artifacts resulting from incorrect registration of PA frames acquired with different wavelengths;
Figure 2 is a schematic illustrating a combined PA and ultrasound imager system associated with the present disclosure.

[0021] The present disclosure relates to systems and methods that combine photoacoustic (PA) and ultra-

sound images. Such systems and methods are capable of generating images using PA or ultrasound image generating means. The acquisition of these images can be interleaved so that, from the point-of-view of the user, they appear to be acquired simultaneously. The two imaging modalities rely on different contrast mechanisms, and they will therefore generate different information. For example, an ultrasound image shows boundaries between different tissues with different acoustic impedances, whereas a PA image shows absorption of laser energy at the associated optical wavelength used.

[0022] Systems according to the present disclosure are used to simultaneously display PA and ultrasound images of the same object. An exemplary embodiment of a system associated with the present disclosure includes an image combiner that performs spatial and temporal interpolation of two images (PA and ultrasound) before generating a combined image. The combined image is then displayed on a display means such as a CRT and/or an LCD. In an exemplary embodiment the combined image can also be transmitted as data to a data storage or processing means such as a printer, a hard disk, a compact disk, and/or a flash drive. An exemplary image combiner according to the present disclosure is able to use motion estimates obtained from ultrasound data to enhance a photoacoustic image: increasing its apparent frame rate, registering consecutive frames in order to reduce artifacts. An exemplary combined system may be capable of generating combined ultrasound and PA images that are registered spatially and temporally.

[0023] Referring to Figure 2, a schematic of an exemplary image combiner for a combined PA and ultrasound imaging system is shown. An exemplary system according to the present disclosure is used in conjunction with an ultrasound signal pathway, a PA signal pathway, a motion estimator, a frame buffer and a display. Ultrasound images are typically formed using a transducer, ultrasound beamformer and an ultrasound scan converter. These components may be the same as those typically found in an existing modem ultrasound machine. Ultrasound energy is transmitted in a series of focused beams using an ultrasound beamformer and a transducer. The energy received by the transducer is then beamformed to create a corresponding series of radio frequency (RF) signals, known as A-lines. These signals are detected and then scan converted to form a B-mode ultrasound image. The same components can also be used in a pulsed Doppler mode to detect and measure motion.

[0024] PA signals are generated by illuminating an object with a short laser pulse. The signals are received by a transducer that is common to PA and ultrasound signal pathways. The signals pass through a PA beamformer, which allows them to be spatially localized. The PA scan converter is then used to resample the signals and produce a PA image. In an exemplary embodiment, a single transducer is deployed to transmit ultrasound waves, receive ultrasound signals generated by the transmitted ultrasound waves and receive PA signals. However, sys-

tems associated with the present disclosure also include embodiments having multiple transducers. In an exemplary embodiment, a first transducer transmits ultrasound waves and a second transducer receives ultrasound signals generated by the transmitted ultrasound waves and receives the PA signals.

[0025] A motion estimator is used to estimate the motion of the object using the ultrasound data. To accomplish motion estimation, it is necessary to compare the signals received at different times from the same image location. This can be done using the RF A-line signals before they are detected and scan converted. Accordingly, it is possible to estimate the axial motion very accurately. Such motion estimation methods have previously been used in elastography. (See, e.g., E. E. Konofagou, T. Harrigan, and J. Ophir, "Shear strain estimation and lesion mobility assessment in elastography," *Ultrasonics*, Vol. 38, No. 1-8, pp. 400-4, 2000; J. Ophir, S. K. Alam, B. Garra, F. Kallel, E. Konofagou, T. Krouskop, and T. Varghese, "Elastography: ultrasonic estimation and imaging of the elastic properties of tissues," *Proceedings of the Institution of Mechanical Engineers. Part H, Journal of Engineering in Medicine*, Vol. 213, No. 3, pp. 203-33, 1999; J. Ophir, I. Cespedes, H. Ponnekanti, Y. Yazdi, and X. Li, "Elastography: a quantitative method for imaging the elasticity of biological tissues," *Ultrasonic Imaging*, Vol. 13, No. 2, pp. 111-34, 1991.)

[0026] It is also possible to estimate the motion from a series of ultrasound images (after detection and scan conversion) using speckle tracking. (See, e.g., E. J. Chen, R. S. Adler, P. L. Carson, W. K. Jenkins, and W. D. O'Brien, Jr., "Ultrasound tissue displacement imaging with application to breast cancer," *Ultrasound in Medicine and Biology*, Vol. 21, No. 9, pp. 1153-62, 1995; M. O'Donnell, A. R. Skovoroda, B. M. Shapo, and S. Y. Emelianov, "Internal displacement and strain imaging using ultrasonic speckle tracking," *IEEE Transactions on Ultrasonics, Ferroelectrics and Frequency Control*, Vol. 41, No. 3, pp. 314-25, May 1994.) In an exemplary embodiment, the motion estimator receives signals from the ultrasound beamformer and the ultrasound images to generate motion estimation.

[0027] A further alternative estimation method includes using Doppler information derived from specific Doppler sequences. (See, e.g., D. A. Christensen, *Ultrasonic Bioinstrumentation*: John Wiley & Sons, 1988.) It is understood that ultrasound image generators do not need to contain contrasting structures in order to perform motion estimation. The motion estimation can be performed on regions of uniform speckle texture.

[0028] Motion information extracted from the ultrasound signals may be displayed on the ultrasound image. Commercial ultrasound scanners typically include continuous wave Doppler, color Doppler, power Doppler and pulsed Doppler modes. Some also feature elastography, Doppler strain rate imaging and tissue Doppler imaging.

[0029] An exemplary image combiner according to the present disclosure may perform at least the following two

functions:

1. Spatial and temporal interpolation and resampling of a PA image sequence, thus making use of the motion estimates derived from the ultrasound signals; and
2. Generating an output frame based on a combination of the pixel values in one of more ultrasound images and one or more PA images.

[0030] The output of the image combiner is typically a sequence of combined frames containing both ultrasound and PA information. This information is typically stored in a frame buffer. The frame buffer includes a plurality of frames adapted to be sequentially displayed on a display means. Exemplary display means include but are not limited to a CRT, LCD, or any other type of information display system.

[0031] Systems according to the present disclosure are adapted to allow for images acquired by ultrasound and PA modalities to be displayed on a single displaying means. Moreover, exemplary systems allow these images to be displayed at the same rate, even though they are acquired at different rates. Exemplary systems allow for different images to be spatially registered, such that corresponding anatomical features in the two images can be identified. Further aspects associated with the present disclosure include allowing for different PA images to be registered before being combined, thus reducing misregistration artifacts.

[0032] Spatial and temporal resampling of a PA image sequence functions as follows:

1. Spatial resampling: A PA image may be reconstructed on a different spatial grid from an ultrasound image. Spatial interpolation and resampling of a PA image is therefore required before it can be overlaid on an ultrasound image. This functionality may be performed within a PA scan conversion module. However, it may be desirable to perform certain operations, such as combining multiple PA frames, before spatial resampling (for increased accuracy, or less computation). (See, e.g., P. Thevenaz, T. Blu, and M. Unser, "Interpolation revisited [medical images application]," *Medical Imaging, IEEE Transactions*, Vol. 19, No. 7, pp. 739-758, 2000.)

2. Temporal up-sampling without ultrasound: PA frames can be temporally up-sampled using standard techniques developed for video. (See, e.g., H. A. Karim, M. Bister, and M. U. Siddiqi, "Low rate video frame interpolation - challenges and solution," in *Proc. Acoustics, Speech, and Signal Processing*, 2003. *Proceedings. (ICASSP'03)*, 2003 IEEE International Conference on, 2003, Vol. 3, pp. III-117-20 vol.3.) This allows a PA frame to be interpolated for each ultrasound frame. Alternatively, both PA frames and ultrasound frames can be interpolated to a video display rate.

3. Using ultrasound motion information to increase perceived PA refresh rate: Typical a maximum frame rate for an exemplary PA imaging system is about 10 Hz. An image that is refreshed at this rate, will appear to be "jerky" to a user. Using an exemplary system associated with the present disclosure, the motion and deformation of objects within the image can be detected and estimated by a motion estimator. The ultrasound motion field (which is typically measured at 55 Hz) can then be used to warp the PA image. The warped PA image can then be displayed at a 65 Hz rate.

4. Using ultrasound motion information to register PA images before combining: As mentioned above, combining two PA frames that are not properly registered can lead to blurring or other artifacts. The ultrasound motion field can be used to estimate the deformation of an object that occurred during the interval between the PA frame acquisitions. The motion field can then be used to warp one of the PA frames, such that both frames correspond to the same configuration of the object. This will reduce the blurring and artifacts.

5. Using ultrasound motion information to decide which parts of PA images to combine: It is possible that some structures within a field-of-view of a particular PA image will be moving too fast to be tracked accurately by an ultrasound motion estimator. This fast motion may still be indicated by the motion estimator. For example, the correlation values in a speckle tracking algorithm may be below a certain threshold. Rather than trying to register these parts of an image by warping, it may be advantageous to not combine these parts of the PA frames.

6. Using ultrasound information to detect when a large change in probe position has occurred and stop averaging: As mentioned above, it may be necessary to average several PA frames in order to achieve sufficient signal-to-noise ratio (SNR). This decreases the temporal resolution of an exemplary system and gives persistence to the image. This has a disadvantage in that, when a probe is moved to a different part of the body, or a different orientation, the previous image will persist, even though it corresponds to very different anatomy. The ultrasound can be used to detect this condition and reset the averaging, such that the previous image is not overlaid on a new image. In this scenario, it may also be appropriate to stop the display of the PA image for a few frames until enough (registered) images are available to average and produce a good image with sufficient SNR.

[0033] A combined imaging system according to the present disclosure can be adapted to accomplish several displaying options including but not limited to:

1. Displaying PA image only: A PA image can still

be enhanced by ultrasound motion information as described above.

2. Displacing PA and ultrasound images next to one another: Images are displayed at the same (video) rate, even though they are acquired at different rates.

3. Overlaying a PA image on to an ultrasound image: PA images can be displayed using a different color-map than that used to display ultrasound images. The PA image can be set at a threshold such that pixels below the threshold appear transparent and the user can "see through" to the ultrasound image behind. The roles of the images can be reversed so that the ultrasound image is overlaid on the PA image.

4. Using Doppler information to select which PA pixels are displayed: Doppler signals from the ultrasound (color Doppler, or power Doppler) can be used to detect where there is motion within an image scan. PA images will only be displayed as a color overlay on pixels where the Doppler signal exceeded a certain threshold setting. Blood, for example, is a strong absorber for wavelengths of light normally used for PA imaging. The resulting image would thus be an image of blood moving above a certain speed.

5. Combining Doppler and PA oxygenation information: By comparing PA images at two different wavelengths, it is possible to determine the oxygenation of blood. The oxygenation value can be multiplied by the velocity derived from the Doppler signal, and the result displayed as an image to a user. The image would be a measure of the rate at which oxygen was being transported in the blood vessels being imaged.

[0034] Examples of possible uses for an exemplary system associated with the present disclosure include but are not limited to medical imaging of humans, or small animals. An exemplary imaging system can be added to an existing modem ultrasound machine, such as, for example, a Philips iU22 or iE33.

Claims

1. A combined imaging system, comprising:

- (a) means for generating photoacoustic signals;
- (b) at least a first transducer adapted to: (i) transmit ultrasound waves; (ii) receive ultrasound signals generated from the ultrasound waves; and (iii) receive photoacoustic signals generated from the photoacoustic signal means;

characterized in that

the system further comprises

- (c) a motion estimator adapted to estimate motion based on the ultrasound signals; and
- (d) an image combiner adapted to receive and combine ultrasound data, photoacoustic data and motion estimator data generated from the

received ultrasound and photoacoustic signals and the motion estimator and correct for motion to generate a combined image.

2. A system according to claim 1, wherein the combined image is received by a frame buffer adapted: (i) to store combined image output generated from the image combiner; and (ii) transmit the combined image to a display means and/or data storage means.

3. A system according to claim 1, wherein the photoacoustic signal means is accomplished by an illumination system adapted to generate a photoacoustic signal within a sample.

4. A system according to claim 3, wherein the illumination system is **characterized by** an energy beam.

5. A system according to claim 2, wherein the display means is selected from the group consisting of an LCD and a CRT and the data storage means are selected from the group consisting of a printer, a hard disc, a compact disc, and a flash drive.

6. A system according to claim 2, wherein the frame buffer is adapted to transmit a series of combined images at a rate of about 55 Hz.

7. A system according to claim 3, wherein the received ultrasound signals are beamformed by an ultrasound beamformer to create a series of radio frequency signals.

8. A system according to claim 3, wherein the received photoacoustic signals pass through a photoacoustic scan converter adapted to generate a photoacoustic image to be received by the image combiner.

9. A system according to claim 1, wherein the ultrasound signals are generated in a pulsed Doppler mode.

10. A system according to claim 2, wherein the image combiner is adapted to generate a sequence of combined frames containing data resulting from the received ultrasound signals and data resulting from the received photoacoustic signals to be transmitted to the frame buffer.

11. A system according to claim 1, wherein the image combiner is adapted to perform spatial and/or temporal interpolation and resampling of the received photoacoustic signals.

12. A system according to claim 2, wherein the display means is adapted to allow different images to be spatially registered, such that corresponding anatomical features in each image can be identified.

13. A system according to claim 2, wherein the display means is adapted to display images in a displaying option selected from the group consisting of: displaying photoacoustic images only, displaying photoacoustic images and ultrasound images next to one another, overlaying a photoacoustic image on to an ultrasound image, using Doppler information to select which photoacoustic pixels are displayed, and combining Doppler and photoacoustic oxygenation information.

14. A method of combining images of a sample comprising:

- (a) illuminating a sample with an illumination system adapted to generate photoacoustic signals;
- (b) transmitting ultrasound waves to the sample with an ultrasound transmitting means adapted to receive ultrasound signals and photoacoustic signals;
- (c) generating at least one ultrasound image from a portion of the received ultrasound signals via an ultrasound imaging means;
- (d) generating a motion estimation from a remaining portion of the received ultrasound signals via a motion estimator;
- (e) generating at least one photoacoustic image from the received photoacoustic signals via a photoacoustic imaging means; and
- (f) combining the ultrasound image, the motion estimation and the photoacoustic image and correcting for motion in an image combiner adapted to transmit the combined image to a display means.

15. A combined imaging system, comprising:

- (a) means for generating photoacoustic signals;
- (b) at least a first transducer adapted to transmit ultrasound waves
- (c) at least a second transducer adapted to: (i) receive ultrasound signals generated from the ultrasound waves; and (ii) receive photoacoustic signals generated from the photoacoustic signal means;
- (c) a motion estimator adapted to estimate motion based on the ultrasound signals; and
- (d) an image combiner adapted to receive and combine ultrasound data, photoacoustic data and motion estimator data generated from the received ultrasound and photoacoustic signals and the motion estimator and correct for motion to generate a combined image.

Patentansprüche

1. Kombiniertes Bildgebungssystem, das Folgendes umfasst:

- (a) Mittel zum Erzeugen von photoakustischen Signalen;
- (b) mindestens einen ersten Wandler, der vorgesehen ist, um (i) Ultraschallwellen auszusenden; (ii) von den Ultraschallwellen erzeugte Ultraschallsignale zu empfangen; und (iii) von den photoakustischen Signalmitteln erzeugte photoakustische Signale zu empfangen;

dadurch gekennzeichnet, dass

das System weiterhin Folgendes umfasst:

- (c) eine Bewegungsschätzeinheit, die vorgesehen ist, um Bewegung basierend auf Ultraschallsignalen zu schätzen; und
- (d) eine Bildkombiniereinheit, die vorgesehen ist, um Ultraschalldaten, photoakustische Daten und Bewegungsschätzeinheitdaten zu empfangen und zu kombinieren, die von den empfangenen Ultraschallsignalen und photoakustischen Signalen und der Bewegungsschätzeinheit erzeugt wurden und bezüglich Bewegung zu korrigieren, um ein kombiniertes Signal zu erzeugen.

2. System nach Anspruch 1, wobei das kombinierte Signal durch einen Einzelbildpuffer empfangen wird, der vorgesehen ist, um (i) von der Bildkombiniereinheit erzeugte kombinierte Bildausgabe zu speichern und (ii) das kombinierte Bild an ein Anzeigemittel und/oder Datenspeichermittel zu senden.

3. System nach Anspruch 1, wobei das photoakustische Signalmittel durch ein Beleuchtungssystem geschaffen wird, das vorgesehen ist, um ein photoakustisches Signal innerhalb einer Probe zu erzeugen.

4. System nach Anspruch 3, wobei das Beleuchtungssystem durch ein Energiestrahlenbündel gekennzeichnet ist.

5. System nach Anspruch 2, wobei das Anzeigemittel ausgewählt wird aus der Gruppe bestehend aus einer Flüssigkristallanzeige (LCD) und einer Kathodenstrahlröhre (CRT) und die Datenspeichermittel ausgewählt werden aus der Gruppe bestehend aus einem Drucker, einer Festplatte, einer Compact Disc und einem Flash-Laufwerk.

6. System nach Anspruch 2, wobei der Einzelbildpuffer vorgesehen ist, um eine Reihe von kombinierten Bildern mit einer Rate von ca. 55 Hz zu senden.

7. System nach Anspruch 3, wobei die empfangenen Ultraschallsignale durch einen Ultraschall-Strahlfor-

mer strahlgeformt werden, um eine Reihe von Hochfrequenzsignalen zu erzeugen.

8. System nach Anspruch 3, wobei die empfangenen photoakustischen Signale durch einen photoakustischen Abtastumsetzer geleitet werden, der vorgesehen ist, um ein durch die Bildkombiniereinheit zu empfangendes photoakustisches Bild zu erzeugen. 5
9. System nach Anspruch 1, wobei die Ultraschallsignale in einem gepulsten Dopplermodus erzeugt werden. 10
10. System nach Anspruch 2, wobei die Bildkombiniereinheit vorgesehen ist, um eine an den Einzelbildpuffer zu sendende Folge von kombinierten Einzelbildern zu erzeugen, welche aus den empfangenen Ultraschallsignalen resultierende Daten und aus den empfangenen photoakustischen Signalen resultierende Daten enthalten. 15 20
11. System nach Anspruch 1, wobei die Bildkombiniereinheit vorgesehen ist, um räumliche und/oder zeitliche Interpolation durchzuführen und die empfangenen photoakustischen Signale erneut abzutasten. 25
12. System nach Anspruch 2, wobei das Anzeigemittel vorgesehen ist, um die räumliche Registrierung von verschiedenen Bildern zu ermöglichen, so dass entsprechende anatomische Merkmale in jedem Bild identifiziert werden können. 30
13. System nach Anspruch 2, wobei das Anzeigemittel vorgesehen ist, um Bilder in einer Anzeigeoption anzuzeigen, die ausgewählt wird aus der Gruppe bestehend aus: Anzeigen von nur photoakustischen Bildern, Anzeigen von photoakustischen Bildern und Ultraschallbildern nebeneinander, Überlagern eines Ultraschallbildes durch ein photoakustisches Bild, Nutzen von Dopplerinformationen, um auszuwählen, welche photoakustischen Pixel angezeigt werden, und Kombinieren von Doppler- und photoakustischen Oxygenationsinformationen. 35 40
14. Verfahren zum Kombinieren von Bildern einer Probe, das Folgendes umfasst: 45
 - (a) Beleuchten einer Probe mit einem Beleuchtungssystem, das vorgesehen ist, um photoakustische Signale zu erzeugen; 50
 - (b) Senden von Ultraschallwellen an die Probe mit einem Ultraschallsendemittel, das vorgesehen ist, um Ultraschallsignale und photoakustische Signale zu empfangen;
 - (c) Erzeugen von mindestens einem Ultraschallbild anhand von einem Teil der empfangenen Ultraschallsignale über ein Ultraschallbildgebungsmittel; 55

- (d) Erzeugen einer Bewegungsschätzung anhand von einem verbleibenden Teil der empfangenen Ultraschallsignale über eine Bewegungsschätzeinheit;
- (e) Erzeugen von mindestens einem photoakustischen Bild anhand der empfangenen photoakustischen Signale über ein photoakustisches Bildgebungsmittel; und
- (f) Kombinieren des Ultraschallbildes, der Bewegungsschätzung und des photoakustischen Bildes und Korrigieren bezüglich Bewegung in einer Bildkombiniereinheit, die vorgesehen ist, um das kombinierte Bild an ein Anzeigemittel zu senden.

15. Kombiniertes Bildgebungssystem, das Folgendes umfasst:

- (a) Mittel zum Erzeugen von photoakustischen Signalen;
- (b) mindestens einen ersten Wandler, der vorgesehen ist, um Ultraschallwellen zu senden;
- (c) mindestens einen zweiten Wandler, der vorgesehen ist, um (i) von den Ultraschallwellen erzeugte Ultraschallsignale zu empfangen; und (ii) von den photoakustischen Signalmitteln erzeugte photoakustische Signale zu empfangen;
- (d) eine Bewegungsschätzeinheit, die vorgesehen ist, um Bewegung basierend auf Ultraschallsignalen zu schätzen; und
- (e) eine Bildkombiniereinheit, die vorgesehen ist, um Ultraschalldaten, photoakustische Daten und Bewegungsschätzeinheitdaten zu empfangen und zu kombinieren, die von den empfangenen Ultraschallsignalen und photoakustischen Signalen und der Bewegungsschätzeinheit erzeugt wurden und bezüglich Bewegung zu korrigieren, um ein kombiniertes Signal zu erzeugen.

Revendications

1. Système d'imagerie combinée, comprenant :

- (a) des moyens destinés à générer des signaux photoacoustiques ;
- (b) au moins un premier transducteur adapté pour : (i) transmettre des ondes ultrasonores ; (ii) recevoir des signaux ultrasonores générés à partir des ondes ultrasonores ; et (iii) recevoir des signaux photoacoustiques générés à partir des moyens de signaux photoacoustiques ;
- caractérisé en ce que**
- le système comprend en outre :
- (c) un estimateur de mouvement adapté pour estimer un mouvement en fonction des signaux ultrasonores ; et

- (d) un combineur d'image adapté pour recevoir et combiner des données ultrasonores, des données photoacoustiques et des données d'estimateur de mouvement générées à partir des signaux ultrasonores et photoacoustiques reçus et de l'estimateur de mouvement et réaliser une correction de mouvement pour générer une image combinée.
2. Système selon la revendication 1, dans lequel l'image combinée est reçue par une mémoire tampon d'image adaptée : (i) pour stocker une sortie d'image combinée générée à partir du combineur d'image ; et (ii) transmettre l'image combinée à des moyens d'affichage et/ou des moyens de stockage de données.
 3. Système selon la revendication 1, dans lequel les moyens de signaux photoacoustiques sont accomplis par un système d'éclairage adapté pour générer un signal photoacoustique au sein d'un échantillon.
 4. Système selon la revendication 3, dans lequel le système d'éclairage est **caractérisé par** un faisceau d'énergie.
 5. Système selon la revendication 2, dans lequel les moyens d'affichage sont sélectionnés parmi le groupe constitué d'un LCD et d'un CRT et les moyens de stockage de données sont sélectionnés parmi le groupe constitué d'une imprimante, d'un disque dur, d'un disque compact, et d'un disque flash.
 6. Système selon la revendication 2, dans lequel la mémoire tampon d'image est adaptée pour transmettre une série d'images combinées à une fréquence d'environ 55 Hz.
 7. Système selon la revendication 3, dans lequel les signaux ultrasonores reçus subissent une formation de faisceau par un formeur de faisceau ultrasonore pour créer une série de signaux de radiofréquence.
 8. Système selon la revendication 3, dans lequel les signaux photoacoustiques reçus passent à travers un convertisseur de balayage photoacoustique adapté pour générer une image photoacoustique destinée à être reçue par le combineur d'image.
 9. Système selon la revendication 1, dans lequel les signaux ultrasonores sont générés dans un mode à impulsions à effet Doppler.
 10. Système selon la revendication 2, dans lequel le combineur d'image est adapté pour générer une séquence d'images combinées contenant des données résultant des signaux ultrasonores reçus et des données résultant des signaux photoacoustiques reçus, destinée à être transmise à la mémoire tampon d'image.
 11. Système selon la revendication 1, dans lequel le combineur d'image est adapté pour réaliser une interpolation et un ré-échantillonnage spatial et/ou temporel des signaux photoacoustiques reçus.
 12. Système selon la revendication 2, dans lequel les moyens d'affichage sont adaptés pour permettre à des images différentes d'être repérées spatialement, de sorte que des caractéristiques anatomiques correspondantes dans chaque image puissent être identifiées.
 13. Système selon la revendication 2, dans lequel les moyens d'affichage sont adaptés pour afficher des images dans une option d'affichage sélectionnée parmi le groupe constitué de : un affichage d'images photoacoustiques seules, un affichage d'images photoacoustiques et d'images ultrasonores les unes à côté des autres, une superposition d'une image photoacoustique sur une image ultrasonore, une utilisation d'informations à effet Doppler pour sélectionner les pixels photoacoustiques qui sont affichés, et une combinaison d'informations à effet Doppler et d'oxygénation photoacoustique.
 14. Procédé de combinaison d'images d'un échantillon, comprenant les étapes consistant à :
 - (a) éclairer un échantillon avec un système d'éclairage adapté pour générer des signaux photoacoustiques ;
 - (b) transmettre des ondes ultrasonores à l'échantillon avec des moyens de transmission ultrasonore adaptés pour recevoir des signaux ultrasonores et des signaux photoacoustiques ;
 - (c) générer au moins une image ultrasonore à partir d'une partie des signaux ultrasonores reçus par l'intermédiaire de moyens d'imagerie ultrasonore ;
 - (d) générer une estimation de mouvement à partir d'une partie restante des signaux ultrasonores reçus par l'intermédiaire d'un estimateur de mouvement ;
 - (e) générer au moins une image photoacoustique à partir des signaux photoacoustiques reçus par l'intermédiaire de moyens d'imagerie photoacoustique ; et
 - (f) combiner l'image ultrasonore, l'estimation de mouvement et l'image photoacoustique et réaliser une correction de mouvement dans un combineur d'image adapté pour transmettre l'image combinée à des moyens d'affichage.
 15. Système d'imagerie combinée, comprenant :

- (a) des moyens destinés à générer des signaux photoacoustiques ;
- (b) au moins un premier transducteur adapté pour transmettre des ondes ultrasonores ;
- (c) au moins un second transducteur adapté pour : (i) recevoir des signaux ultrasonores générés à partir des ondes ultrasonores ; et (ii) recevoir des signaux photoacoustiques générés à partir des moyens de signaux photoacoustiques ;
- (d) un estimateur de mouvement adapté pour estimer un mouvement en fonction des signaux ultrasonores ; et
- (e) un combineur d'image adapté pour recevoir et combiner des données ultrasonores, des données photoacoustiques et des données d'estimateur de mouvement générées à partir des signaux ultrasonores et photoacoustiques reçus et de l'estimateur de mouvement et réaliser une correction de mouvement pour générer une image combinée.

25

30

35

40

45

50

55

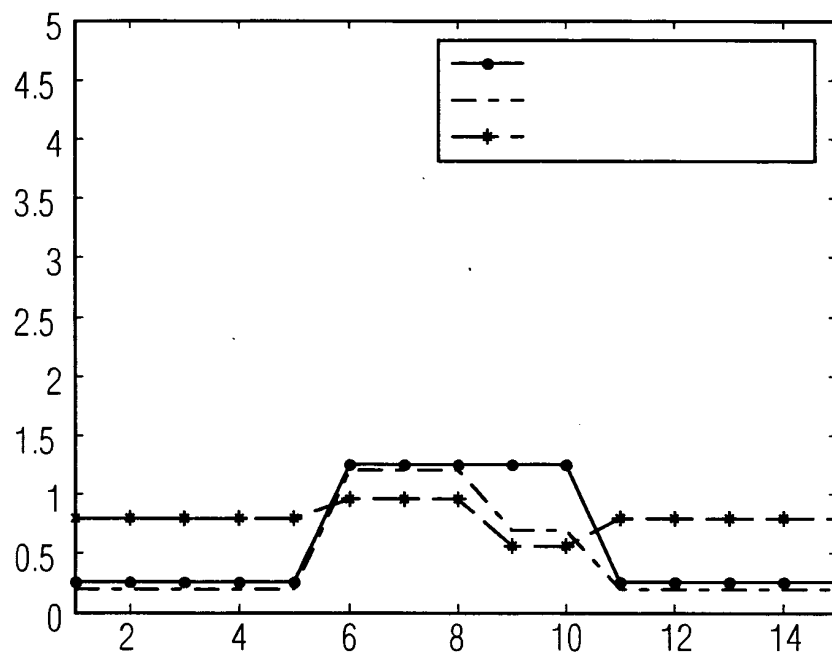


FIG. 1A

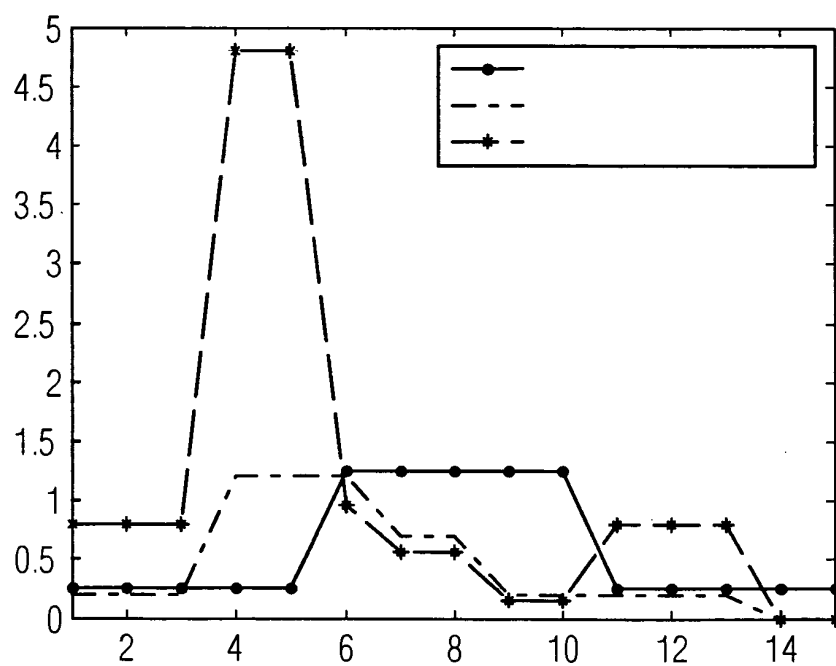


FIG. 1B

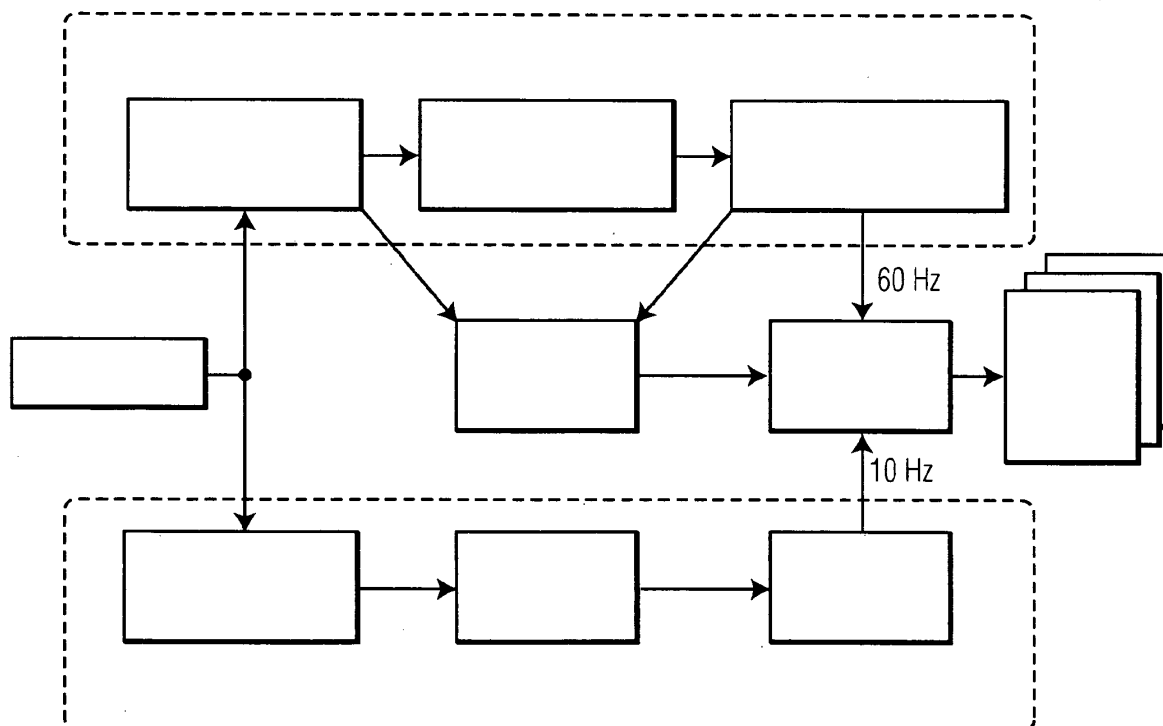


FIG. 2

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- EP 1561424 A [0009]

Non-patent literature cited in the description

- **S. MANOHAR ; A. KHARINE ; J. C. G. VAN HESPEL ; W. STEENBERGEN ; T. G. VAN LEEUWEN.** The Twente Photoacoustic Mammoscope: System Overview and Performance. *Physics in Medicine and Biology*, June 2005, vol. 50 (11), 2543-2557 [0002]
- **M. XU ; L. WANG.** Universal back-projection algorithm for photoacoustic computer tomography. *Physical Review E*, 2005, vol. 71 (1), 16706 [0002]
- **J. NIEDERHAUSER ; M. JAEGER ; R. LEMOR, P. WEBER ; M. FRENZ.** Combined Ultrasound and Photoacoustic System for Real-Time High-Contrast Vascular Imaging In Vivo. *IEEE Transactions on Medical Imaging*, April 2005, vol. 24 (4), 436-440 [0004]
- **J. NIEDERHAUSER ; M. JAEGER ; R. LEMOR ; P. WEBER ; M. FRENZ.** Combined Ultrasound and Photoacoustic System for Real-Time High-Contrast Vascular Imaging in Vivo. *IEEE Transactions on Medical Imaging*, April 2005, vol. 24 (4), 436-440 [0005]
- **X. WANG ; Y. PANG ; G. KU ; X. XIE ; G. STOICA ; L. WANG.** Noninvasive laser-induced photoacoustic tomography for structural and functional in vivo imaging of the brain. *Nature Biotechnology*, July 2003, vol. 21 (7), 803-806 [0007]
- **C. SIMON ; P. VANBAREN ; E. EBBINI.** Motion compensation algorithm for non-invasive two-dimensional temperature estimation using diagnostic pulse-echo ultrasound. *SPIE*, vol. 3249, 182-192 [0010]
- **E. E. KONOFAGOU ; T. HARRIGAN ; J. OPHIR.** Shear strain estimation and lesion mobility assessment in elastography. *Ultrasonics*, 2000, vol. 38 (1-8), 400-4 [0025]
- **J. OPHIR ; S. K. ALAM ; B. GARRA ; F. KALLEL ; E. KONOFAGOU ; T. KROUSKOP ; T. VARGHESE.** Elastography: ultrasonic estimation and imaging of the elastic properties of tissues. *Proceedings of the Institution of Mechanical Engineers. Part H, Journal of Engineering in Medicine*, 1999, vol. 213 (3), 203-33 [0025]
- **J. OPHIR ; I. CESPEDES ; H. PONNEKANTI ; Y. YAZDI ; X. LI.** Elastography: a quantitative method for imaging the elasticity of biological tissues. *Ultrasonic Imaging*, 1991, vol. 13 (2), 111-34 [0025]
- **E. J. CHEN ; R. S. ADLER ; P. L. CARSON ; W. K. JENKINS ; W. D. O'BRIEN, JR.** Ultrasound tissue displacement imaging with application to breast cancer. *Ultrasound in Medicine and Biology*, 1995, vol. 21 (9), 1153-62 [0026]
- **M. O'DONNELL ; A. R. SKOVORODA ; B. M. SHAPO ; S. Y. EMELIANOV.** Internal displacement and strain imaging using ultrasonic speckle tracking. *IEEE Transactions on Ultrasonics, Ferroelectrics and Frequency Control*, May 1994, vol. 41 (3), 314-25 [0026]
- **D. A. CHRISTENSEN.** Ultrasonic Bioinstrumentation. John Wiley & Sons, 1988 [0027]
- **P. THEVENAZ ; T. BLU ; M. UNSER.** Interpolation revisited [medical images application]. *Medical Imaging, IEEE Transactions*, 2000, vol. 19 (7), 739-758 [0032]
- **H. A. KARIM ; M. BISTER ; M. U. SIDDIQI.** Low rate video frame interpolation - challenges and solution. *Proc. Acoustics, Speech, and Signal Processing, 2003. Proceedings. (ICASSP'03), 2003 IEEE International Conference*, 2003, vol. 3, III-117-20 [0032]

专利名称(译)	结合光声和超声成像系统		
公开(公告)号	EP2097010B1	公开(公告)日	2011-10-05
申请号	EP2007859456	申请日	2007-12-19
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦电子N.V.		
[标]发明人	BURCHER MICHAEL		
发明人	BURCHER, MICHAEL		
IPC分类号	A61B8/14 G01N21/17 A61B5/00 A61B8/08 G01S7/52		
CPC分类号	A61B5/0035 A61B5/0059 A61B5/0095 A61B5/7207 A61B8/08 A61B8/14 A61B8/4416 A61B8/488 A61B8/5238 A61B8/5276 G01N21/1702 G01S7/52074 G01S15/899 A61B8/5261		
代理机构(译)	kroeze antonius , 约翰		
优先权	60/870713 2006-12-19 US		
其他公开文献	EP2097010A1		
外部链接	Espacenet		

摘要(译)

本公开提供了一种适于同时显示相同对象的光声和超声图像的系统。图像组合器可以在生成组合图像之前执行两个图像的空间和时间内插。然后将组合图像显示在诸如LCD或CRT的显示器上。该系统能够使用从超声数据获得的运动估计来增强光声图像，从而增加其表现帧速率，记录连续帧以减少伪像。该系统能够产生在空间和时间上记录的组合超声和光声图像。

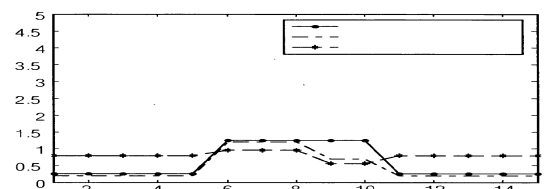


FIG. 1A

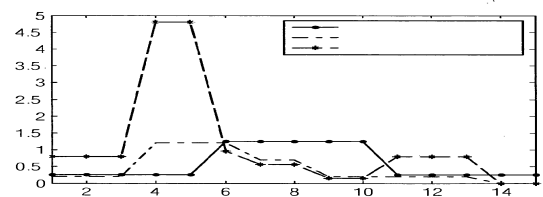


FIG. 1B