


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : A61B 8/13, 8/04	A1	(11) International Publication Number: WO 00/62677 (43) International Publication Date: 26 October 2000 (26.10.00)
<p>(21) International Application Number: PCT/IL00/00223</p> <p>(22) International Filing Date: 14 April 2000 (14.04.00)</p> <p>(30) Priority Data: 129461 15 April 1999 (15.04.99) IL</p> <p>(71) Applicant (for all designated States except US): F.R.A.Y. PROJECT LTD. [IL/IL]; Ibn Gvirol St. 20, 46482 Herzliya (IL).</p> <p>(72) Inventor; and (75) Inventor/Applicant (for US only): LEVKOVITZ, Zeev [IL/IL]; Rambam Street 28/19, 43602 Raanana (IL).</p> <p>(74) Agent: REINHOLD COHN AND PARTNERS; P.O. Box 4060, 61040 Tel-Aviv (IL).</p>	<p>(81) Designated States: AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</p>	

(54) Title: ULTRASOUND IMAGING DEVICE

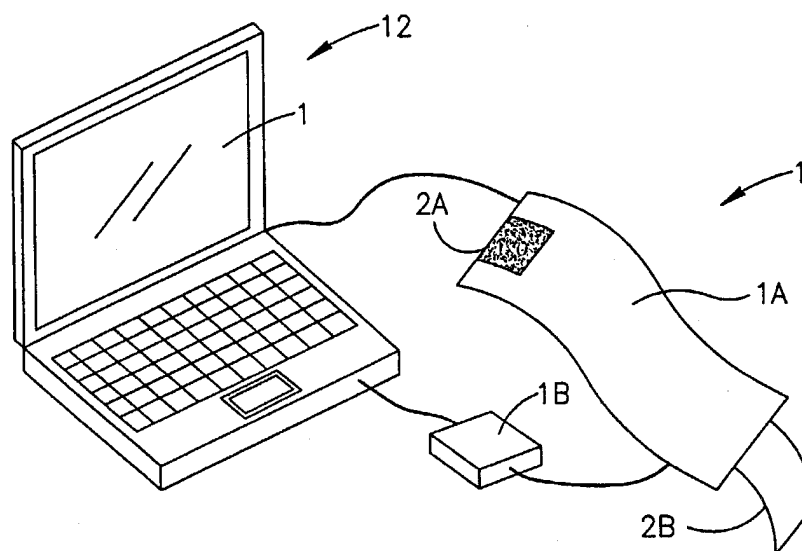

(57) Abstract

Ultrasound-based imaging device (1) and software operated method are presented for monitoring a body part and generating data indicative of a three-dimensional image of an internal structure of the body part. The device (1) is portable and comprises a substantially elastic cover (1A) for covering the body part, wherein the cover is coupled to a control unit (1B) and is connectable to a computer device. The cover carries an array of ultrasonic transceivers (5), each of a kind emitting a beam of ultrasonic waves for irradiating an area within a region covered by the cover, and detecting signal response of the irradiated area. The transceivers (5) are arranged in at least two spaced parallel groups. The transceivers of each group are arranged in a spaced-apart relationship, the space between each two adjacent transceivers in the group being such that an overlap exists between the areas irradiated by the adjacent transceivers.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

Ultrasound Imaging Device

FIELD OF THE INVENTION

The present invention is in the field of imaging techniques, and relates to ultrasound imaging device for monitoring an organ of a patient and displaying an image of its internal structure.

5 BACKGROUND OF THE INVENTION

Ultrasound-based imaging techniques are known and widely used for observing organs in the human body for medical diagnosis. Some ultrasound systems utilize a hand-held probe containing an array of transducers that convert electrical signals into ultrasonic waves, and appropriate signal reception means.
10 The probe is appropriately placed on the patient's body and an ultrasound beam is directed towards a location within the region of interest. To image the entire region, the probe is displaced with respect to the body thereby providing the scanning of the region. This enables to construct a two-dimensional image of the region.

Various methods and devices have been developed aimed at improving the
15 performance of ultrasound imaging systems, and are disclosed, for example, in the following US Patents: 4,625,555; 5,235,857; and 5,435,312.

US Patent 4,625,555 discloses a measurement apparatus utilizing three ultrasonic transducers, wherein first and second transducers are arranged opposite to each other across an object interposed therebetween, and a ray from the third
20 transducer intersects a ray connecting the first and second transducers. The second transducer receives ultrasonic waves emitted by the first and third transducer after corresponding time periods, and the first transducer receives an ultrasonic wave emitted by the third transducer after a respective time interval. On the basis of these time periods, a distribution of propagation velocity of sound internally of the object
25 is measured.

- 2 -

US Patent 5,235,857 discloses a real-time 3D medical ultrasound imaging machine, wherein either a single transducer or a two-dimensional array of transducer is associated with an array of receivers. A body to be imaged is located outside a plane defined by the transducer(s) and receivers.

5 US Patent 5,435,312 discloses an acoustic imaging device, in which several transducer and detector means are arranged in a ring so as to at least partly encircle a body to be imaged. Each of the transducers is operated for transmitting signals with subsequent reception of scattered waves by remaining transducers. This technique enables the imaging of a single slice of the organ.

10 SUMMARY OF THE INVENTION

There is accordingly a need in the art to facilitate real-time 3D imaging with ultrasonic radiation, by providing a novel method and device for ultrasound-based imaging.

The device according to the invention, in distinguish to the conventional
15 devices of the kind specified, has a simple and portable construction, and is easy to operate (generally similar to the known blood-pressure measuring device). This enables the use of the device for the immediate monitoring of an injured patient in outdoor conditions or at the patient's home. To this end, the device is connected to a conventional computer, for example a portable computer (laptop), typically
20 available at the user's home, ambulance, physician's office, or hospital. The computer device is installed with a predetermined software application capable of processing data coming from the imaging device. This image processing does not require a complicated sampling procedure, due to the specific arrangement of transceivers provided in the imaging device.

25 The term "*transceiver*" signifies a unit composed of a transmitter of radiation (of ultrasonic waves in this case) and a detector (receiver) of returned radiation.

The main idea of the present invention is aimed at 3D mapping of an internal structure of a body part, and is based on the provision of an array (matrix)

- 3 -

of transceivers mounted on an elastic cover for covering or wrapping a patient's organ (limb) when putting the device in operation. The transceivers are arranged in spaced parallel groups, each group including several spaced-apart transceivers. Each pair of adjacent transceivers in the group (which form a circle when in an operative position of the cover) provides stereoscopic imaging of an area within the entire region imaged by all the transceivers. Consequently, each such group of transceivers provides a 360-degree section image of the organ, at least two groups of transceivers being thereby sufficient for constructing a three-dimensional image of the structure performing a data processing procedure by the software application.

10 The transceivers are connected to a control unit, which is operated by the software application for electrically operating the transceivers in a predetermined manner. By coupling output circuits of the transceivers to the computer device, either directly, or through a communication link, data coming from the transceivers is processed and a 3D image is constructed and displayed on a monitor of the

15 computer device.

The image can be stored in the memory of the computer, thereby enabling to detect changes in the internal structure of the patient's body part, that may be caused by drugs, as well as enabling the timely detection of blood thromboses.

The transceivers transmit and receive signals in accordance with the following parameters predefined by the software application: timing (sequence), signal intensity and pulse duration. The software application, in response to data coming from the transceivers, processes data indicative of the collected samples and determines whether the collected data is sufficient for constructing the 3D image of the structure. If the received data is insufficient, the software application

25 operates the transceivers for further collection of samples until the complete 3D image can be constructed.

There is thus provided according to one broad aspect of the present invention, an imaging device for monitoring a body part and generating data indicative of a three-dimensional image of an internal structure of the body part, the

30 device comprising:

- 4 -

- (i) a substantially elastic cover for covering the body part when in an operative position of the device;
- (ii) a control unit coupled to the cover;
- (iii) an array of ultrasonic transceivers mounted on the cover each for emitting a beam of ultrasonic waves for irradiating an area within a region covered by the cover, and for detecting a signal response of the irradiated area, the array of the transceivers being composed of at least two spaced-apart parallel groups of the transceivers, wherein the transceivers of each group are arranged in a spaced-apart relationship, and the space between each two adjacent transceivers in the group is such that an overlap exists between the areas irradiated by the adjacent transceivers.

The cover when in an inoperative position thereof may be in the form of a circle so as to form a spherical part when in the operative position thereof. This design of the cover may be applied to a woman's abdomen or breast. The cover may be in the form of an open sleeve provided with two fasteners at its opposite ends for securing the cover on the body part wrapped by the cover. The cover may be in the form of sleeve (cuff) open at opposite ends so as to put onto the body part.

Generally speaking, the device according to the present invention provides for acquiring 2D images of the sections, and creating a 3D structure of the inside of the body part (limb). The 3D image will be presented on a conventional PC monitor or a laptop monitor. Generally, the image can be displayed in a regular way (i.e., on the computer monitor), or by virtual reality or holograms-based technique. Additionally, the obtained picture (3D image) can be rotated on the display by simply operating a computer mouse or the like. The use of the flexible cover allows the system high mobility in emergencies, either in the field or at the scene of an event.

The present invention enables examination (monitoring) without having to move the patient (in severe accidents), and enables the accurate and reliable reporting of the severity of the injury in the field. The use of 3D display, spatial

– 5 –

display or any other conventional monitor enables certain rapid identification of types and natures of fractures within limbs, without the need for prior surgical intervention. The present invention can be used for the identification of blood vessels and their location, and the introduction of a needle for purposes of IV, blood testing, etc., and is assured to locate the vein on the first attempt. The present invention enables early identification of irregularities in the limbs and in the anatomical or tissue structure of the internal array, without surgical intervention.

The invention can be advantageously useful for monitoring the health condition of an injured patient in outdoor conditions or at the patient's home, e.g., for monitoring osteoporosis, arteriosclerosis or tumors, and for taking blood samples. Specifically, the present invention provides a facile method and a flexible device for monitoring changes in a patient's organ so as to monitor significant parameters of the patient's health. Further, such a device may be used for treating injured soldiers in battle when the mobility and the compactness of the device are of great importance.

According to another aspect of the present invention, there is provided an imaging system comprising the above imaging device connectable to a computer device.

Preferably, the transceivers are sequentially operated, so as to significantly simplify the image processing. To this end, the control unit comprises a synchronizer block for operating a power supply of the transceivers accordingly. First, the transceivers of the first group are sequentially activated to irradiate the plurality of areas within a slice and generate data indicative thereof. This data is stored in a memory of the computer device, until all other groups of the transceivers are sequentially operated, and then used by a suitable software application for providing a 3D image of the entire structure covered by the cover.

Thus, according to yet another aspect of the present invention, there is provided an imaging method for obtaining a three-dimensional image of an internal structure of a body part utilizing an imaging device having a cover for covering said body part and carrying at least two groups of ultrasonic transceivers, wherein

– 6 –

each an overlap exists between areas irradiated by each two locally adjacent transceivers in the group, the method comprising the steps of:

- 5 (a) sequentially operating each of the transceivers in one group for irradiating corresponding areas within a region covered by the cover, and generating data indicative of 360-degree section of the body part;
- (b) repeating step (a) with respect to at least one other group of the transceivers, so as to generate data indicative of at least one further 360-degree section; and
- 10 (c) processing the generated data to construct said three-dimensional image of the internal structure of the body part.

BRIEF DESCRIPTION OF THE DRAWINGS

In order to understand the invention and to see how it may be carried out in practice, a preferred embodiment will now be described, by way of non-limiting example only, with reference to the accompanying drawings, in which:

15 **Fig. 1a and 1b** schematically illustrate one example of an imaging device according to the present invention;

Fig. 2 more specifically illustrate an arrangement of transceivers when in an operational position of the device of Figs 1a-1b;

20 **Fig. 3** is a schematic illustration of an imaging device according to another example of the present invention;

Fig. 4 is a schematic illustration of an imaging system utilizing the imaging device of the present invention;

25 **Fig. 5** shows the imaging device of the present invention applied to locate the patient's blood vessels and to guide a needle of a syringe towards the patient's vein;

Fig. 6 illustrates yet another example of an imaging device of the present invention utilizing an inflatable cover for covering a body part to be imaged; and

Fig. 7 illustrates an imaging device of the present invention designed to be uses for monitoring a woman's abdomen.

DETAILED DESCRIPTION OF A PREFERRED EMBODIMENT

Referring to Fig.1a and 1b, there is schematically illustrated an imaging device 1 constructed and operated according to the invention. The device 1 is composed of a light elastic cover 1A associated with a control unit 1B (adaptor).
5 The cover 1A, when in an inoperative position thereof (Fig. 1a) is a strap formed with two connectors 2A and 2B (e.g., Velcro fasteners) at its opposite ends, so as to form an open sleeve (Fig. 1b) capable of wrapping a patient's organ (not shown here) when in the operative position of the device. The sleeve resembles a sphygmomanometer cuff, being made of several layers of cloth or other flexible
10 material. The sleeve is easy to wear and can be adapted to a wide range of limbs of various sizes.

Mounted on the strap 1A (i.e., built-in between the layers) is a two-dimensional array of transceivers, generally designated as 5, each transceiver being composed of a piezoelectric transducer and a receiver for, respectively,
15 transmitting and receiving ultrasonic waves. In the present example, the 2D array 5 is formed by four parallel spaced-apart groups (rows) R_1 - R_4 extending along the strap 1A, each group including six transceivers aligned in a spaced-apart relationship. As shown, transceivers $T_1^{(1)}$ - $T_6^{(1)}$ form the group R_1 , transceivers $T_1^{(2)}$ - $T_6^{(2)}$ form the group R_2 , etc.

20 It should be noted, although not specifically shown, that the control unit 1B comprises such main constructional parts as a power source for electrically operating the transducers, and a synchronizer block, the purpose of which will be described further below.

As better shown in Fig. 2, when rolling the strap 1 into its operational
25 position forming an open sleeve (for placing the device onto a patient's organ, such as his limb), the transceivers of each row become arranged along the circumferential region of the sleeve, thereby forming a circular array around the patient's limb.

The operation of the transceivers of each group enables the creation of a
30 360-degree section of the limb under examination. Each of the transceivers emits a

- 8 -

beam **B** (solid angle) of ultrasonic radiation (wave) propagating towards an area located within a region to be imaged, and receives a signal response **B'** of this area. This is exemplified in the figure in a self-explanatory manner with respect to the transceiver $T_1^{(1)}$, $T_1^{(3)}$ - $T_6^{(3)}$. As also shown in the figure, the transceivers in each row are spaced from each other such that the beams emitted by two locally adjacent transceivers provides a certain overlap between the irradiated areas. Generally speaking, each two locally adjacent transceivers in the group enables the stereoscopic imaging of the same location (overlapped region).

Fig. 3 illustrates the device 1 in operation, being worn by a patient on his arm. In this example, the strap **1A** of Figs. 1a-1b is replaced by an elastic cuff (the so-called "close sleeve") **10**, which is open at both ends **10A** and **10B**, so as to be placed on the patient's extreme organ, without the need for any fasteners.

Turning back to Fig. 2, the operation of all the transceivers in the group creates a plurality of imaging sectors, thereby enabling the creation of a 360-degree section. The provision of at least two groups of transceivers enables simultaneous (i.e., at the same current position of the device with respect to the patient's organ) imaging of two such 360-degree sections, which may be processed by a suitable image processing technique to reconstruct a 3D image of the internal structure of the patient's organ covered by the sleeve.

The above construction of the imaging device enables to maintain the distances between the transceivers, and the transceivers and the region to be imaged. Accordingly, movements, position shifts and the involuntary tremor of the patient do not affect the course of the examination. This makes the device suitable for examining babies and children. Moreover, the sleeve structure of the device solves the problem of repeat examination. Indeed, since the relative location of the transceivers does not change (neither relative to themselves nor relative to the body part under examination), the examination conditions are identical in all respects and enable true comparison. The flexibility and mobility of the sleeve eliminate the need to move the patient's body, or the limb under examination. The sleeve is simply placed around the body part to be examined (e.g., supposedly damaged

part). This makes the device suitable for field casualties and road accidents, when the extent and severity of the internal injuries are not known.

Fig. 4 illustrates an imaging system composed of the imaging device **1** connected to a conventional computer device (laptop) **12** installed with a suitable software application, which is capable of collecting and processing data generated by the device **1**.

As indicated above, the control unit **1B** (Fig. 1a) includes the synchronizer block (i.e., a timing system) that operates the power source so as to provide a sequential imaging. More specifically, each transceiver (composed of a transmitter and receiver) transmits and receives ultrasonic waves within a given time, and generates data indicative of the received signal. This data is transmitted to a storage utility (database or memory) in the computer device **12**. The synchronizer block operates the power supply to sequentially operate all the transceivers in the first group **R₁** (six transceivers in the present example), and data indicative of an acoustic response of all the imaged areas are transmitted to the storage utility. Then, an image processing utility (a suitable software application) installed in the computer device operates to build an image of the first section (using the previously stored data). In the same way, the software application processes data generated by the transceivers of the groups **R₂**, **R₃** and **R₄** collected in a sequential manner.

Hence, information about the four image sections is created and stored in the memory of the computer device. At a next operational step, a 3D image is constructed using the stored information on the four sections, and the image is displayed on a monitor of the computer device. This sequence of operations is fast enough to generate a continuous flow of 3D images of the sections, in order to create the illusion of motion in real time (if any) within the organ/limb under examination.

Thus, the technique of the present invention provides the creation of a three dimensional image (picture) of an internal structure of an organ from a series of

slice images, each of the slice images being in the form of a 360-degree section image.

It should be noted that if some of the transceivers overlap when wrapping the strap around the patient's organ, the system will disregard the uppermost of the overlapping receivers. This is determined during self-calibration of the system.

It should also be noted that data indicative of a constructed image may be transmitted from the computer **12** to a central medical station through a computer network. Alternatively, the control unit of the imaging device may include a suitable communication utility for transmitting the collected data to the central station through a telephone communication link.

Referring to Fig. 5, there is illustrated an example of applying the imaging device **1** of the present invention to locate the patient's blood vessels and to guide a needle **14** of a syringe **16** towards the patient's vein via an aperture **18** provided in the sleeve **1A.**, while continuously imaging the structure of the veins of the patient. A 3D image **IM** of the structure is displayed on the computer's monitor **19** showing the needle and vein (which are not illustrated here). Such a device is particularly useful when the veins of the patient are hidden, and may be regularly used in hospitals for setting an infusion system or any other treatment, for the convenience of the patient and the nurse.

It should be noted, although not specifically shown, that the sleeve may include an inner disposable sterile element.

As shown in the example of Fig. 6, a sleeve **20** may be inflatable. To this end, the sleeve **20** is constructed generally similar to the above described sleeve **1A** (Figs. 1a-1b) or sleeve **10** (Fig. 3), but is additionally provided with a hollow layer that enables the introduction of air (inflation) by means of a conventional pneumatic assembly (pump) **22** typically used with a sphygmomanometer cuff.

According to another example of the present invention shown in Fig. 7, an elastic cover of the imaging device is in the form of a dome-shape open sleeve (cup) **30** adapted to cover the abdominal portion of a pregnant woman or a woman's breast. Cup **30** is made of a substantially flexible/elastic material which

- 11 -

adapts to the varying sizes, and, when intended for covering the woman's abdomen, is formed with strips 32 for tying behind the back and securing the cup. This enables to achieve the optimum positioning of sensors (transceivers), generally at T, which are in the present example arranged in several groups, extending radially
5 from the top of the cup.

Those skilled in the art will readily appreciate that various modifications and changes can be applied to the embodiments of the invention as hereinbefore exemplified, without departing from its scope defined in and by the appended claims.

10

CLAIMS:

1. An imaging device for monitoring a body part and generating data indicative of a three-dimensional image of an internal structure of the body part, the device comprising:

- 5 (i) a substantially elastic cover for covering the body part when in an operative position of the device;
- (ii) a control unit coupled to the cover;
- 10 (iii) an array of ultrasonic transceivers mounted on the cover each for emitting a beam of ultrasonic waves for irradiating an area within a region covered by the cover, and for detecting a signal response of the irradiated area, the array of the transceivers being composed of at least two spaced-apart parallel groups of the transceivers, wherein the transceivers of each group are arranged in a spaced-apart relationship, and the space between each two adjacent transceivers in the group is such that an overlap exists between the areas irradiated
- 15 by the adjacent transceivers.

2. The device according to Claim 1, wherein the cover, when in an inoperative position thereof, is in the form of a strap provided with two fasteners at its opposite ends for securing the cover on the body part when wrapped by the

20 cover, while in the operational position thereof.

3. The device according to Claim 1, wherein the cover is in the form of a sleeve open at opposite ends thereof so as to be put onto the body part.

4. The device according to Claim 1, wherein the cover, when in an inoperative position thereof is in the form of a circle capable of forming a spherical

25 part, when in the operative position of the cover.

5. The device according to Claim 1, wherein each of the transceivers comprises a piezoelectric transducer.

– 13 –

6. The device according to claim 1, wherein said cover is formed with an inner disposable layer contacting the surface of the body during the operation of the device.

7. The device according to Claim 1, wherein the control unit comprises a power source for activating the transceivers, and a synchronizer block for sequentially operating the transceivers.

8. An imaging system comprising an imaging device for monitoring a body part and generating data indicative of a three-dimensional image of an internal structure of the body part, a control unit for operating the imaging device, and a computer device connectable to the imaging device for processing data generated by the imaging device and constructing and displaying said three-dimensional image, wherein the imaging device comprises:

- (i) a substantially elastic cover for covering the body part when in an operative position of the device;
- (ii) a control unit coupled to the cover;
- (iii) an array of ultrasonic transceivers mounted on the cover each for emitting a beam of ultrasonic waves for irradiating an area within a region covered by the cover, and for detecting a signal response of the irradiated area, the array of the transceivers being composed of at least two spaced-apart parallel groups of the transceivers, wherein the transceivers of each group are arranged in a spaced-apart relationship, and the space between each two adjacent transceivers in the group is such that an overlap exists between the areas irradiated by the adjacent transceivers.

9. An imaging method for obtaining a three-dimensional image of an internal structure of a body part utilizing an imaging device having a cover for covering said body part and carrying at least two groups of ultrasonic transceivers, wherein each an overlap exists between areas irradiated by each two locally adjacent transceivers in the group, the method comprising the steps of:

– 14 –

- (a) sequentially operating each of the transceivers in one group for irradiating corresponding areas within a region covered by the cover, and generating data indicative of 360-degree section of the body part;
- 5 (b) repeating step (a) with respect to at least one other group of the transceivers, so as to generate data indicative of at least one further 360-degree section; and
- (c) processing the generated data to construct said three-dimensional image of the internal structure of the body part.

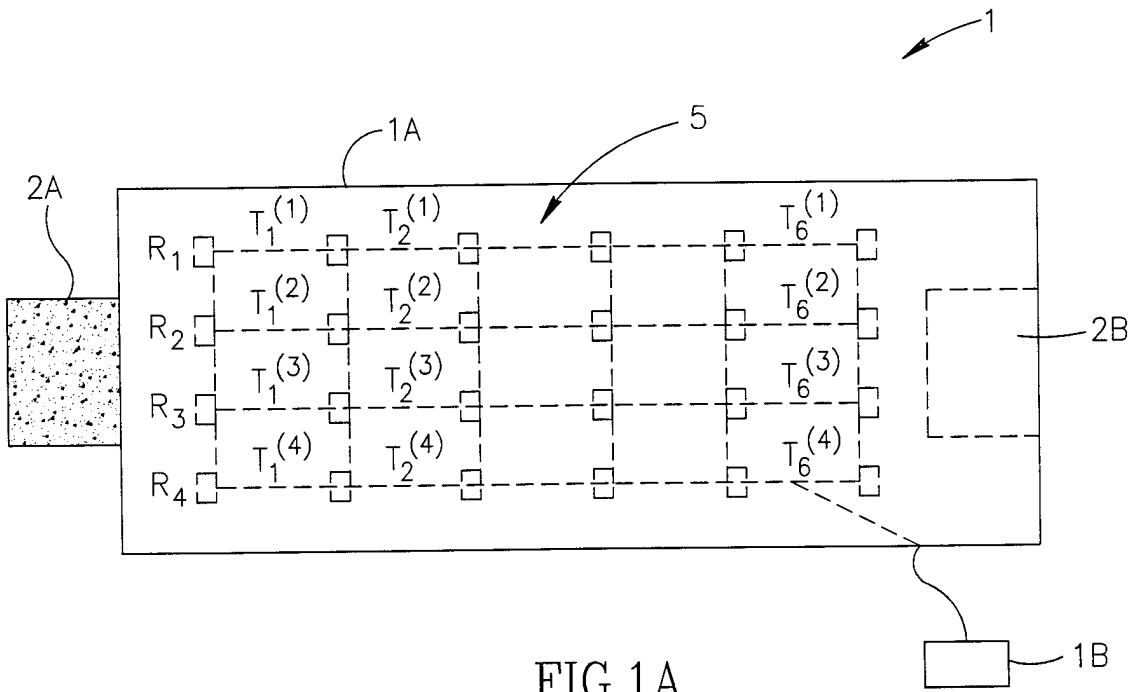


FIG. 1A

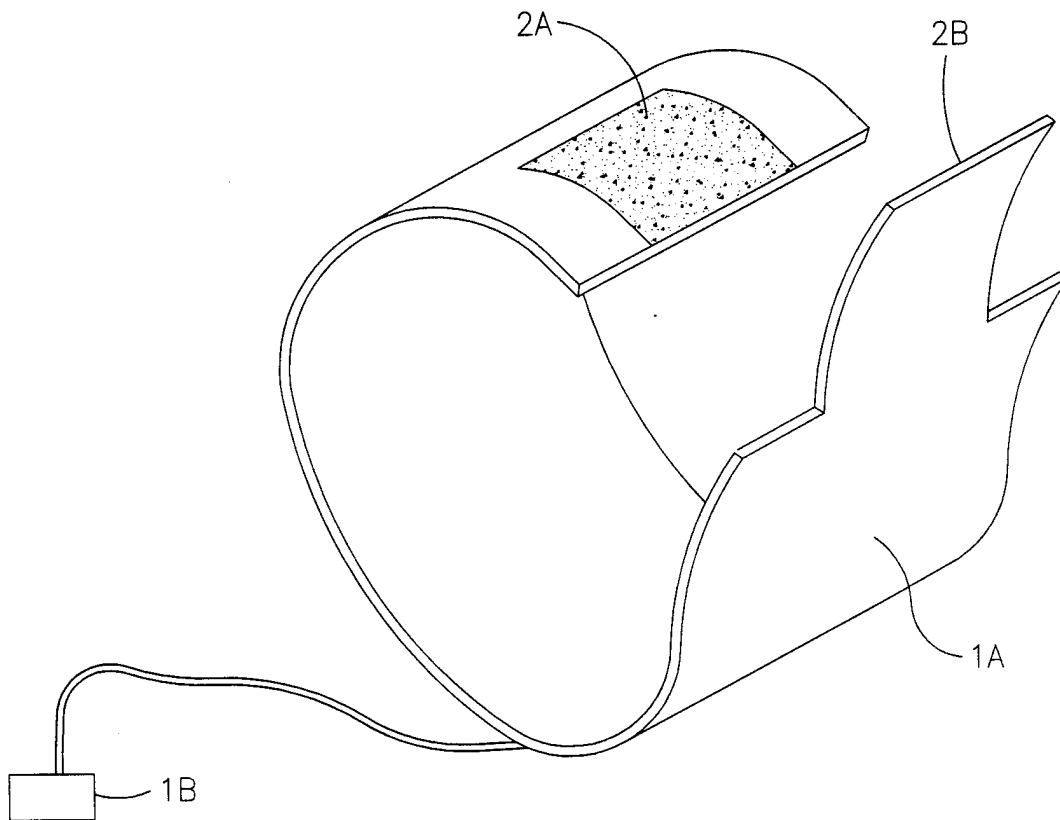


FIG. 1B

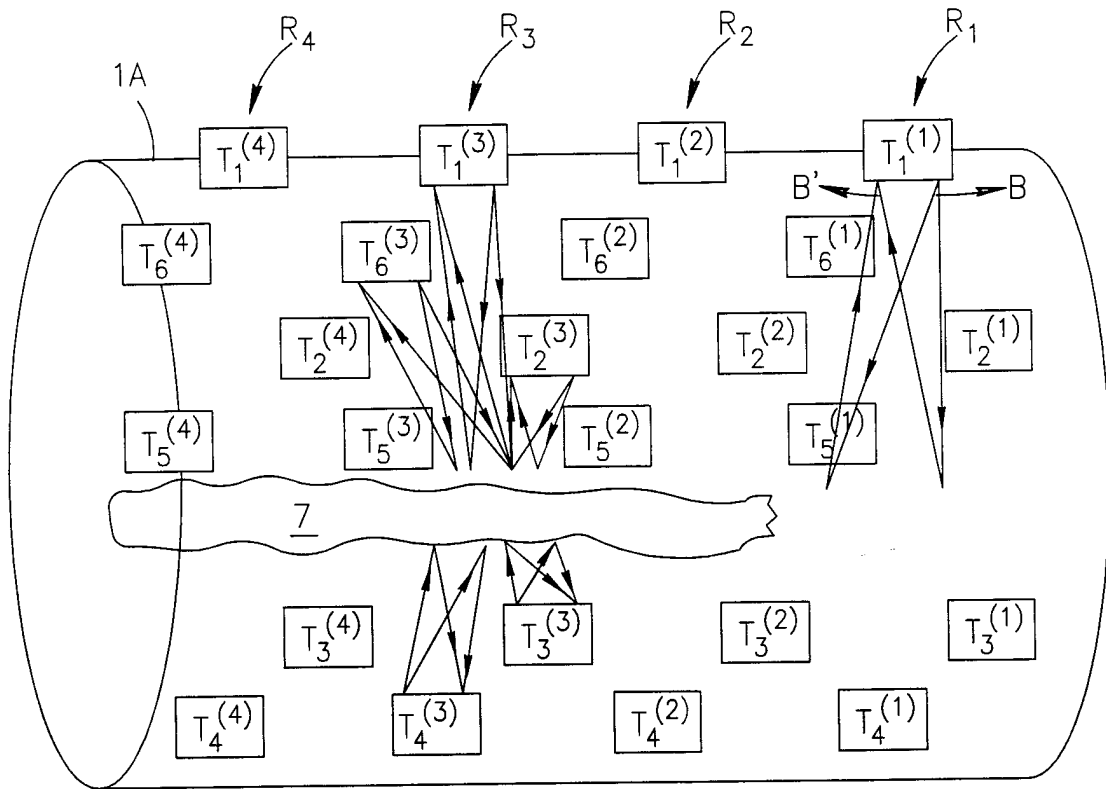


FIG. 2

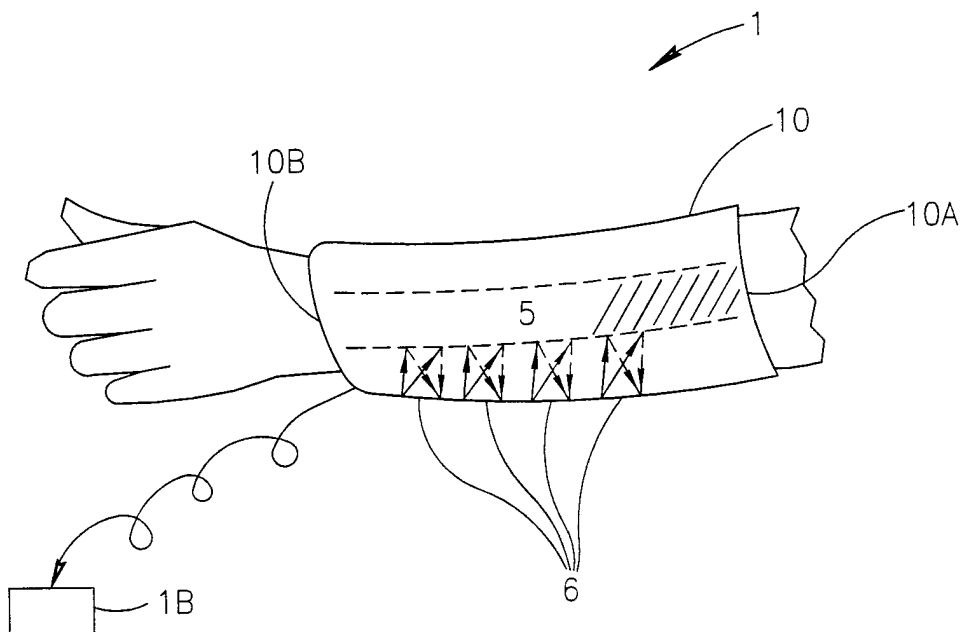


FIG. 3

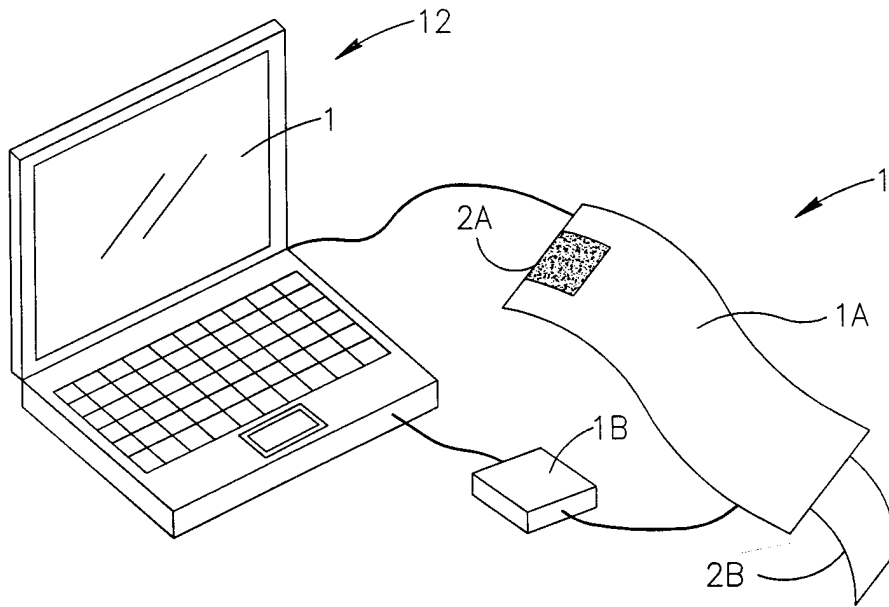


FIG. 4

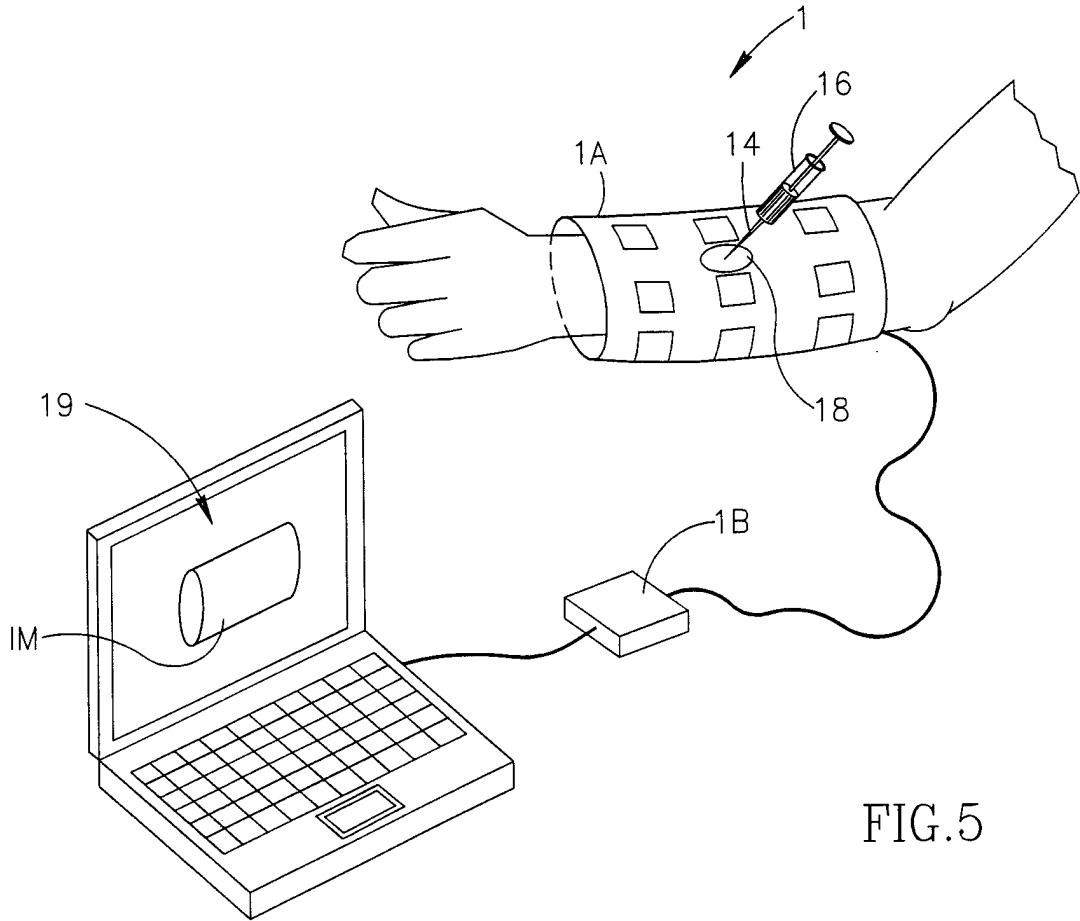


FIG. 5

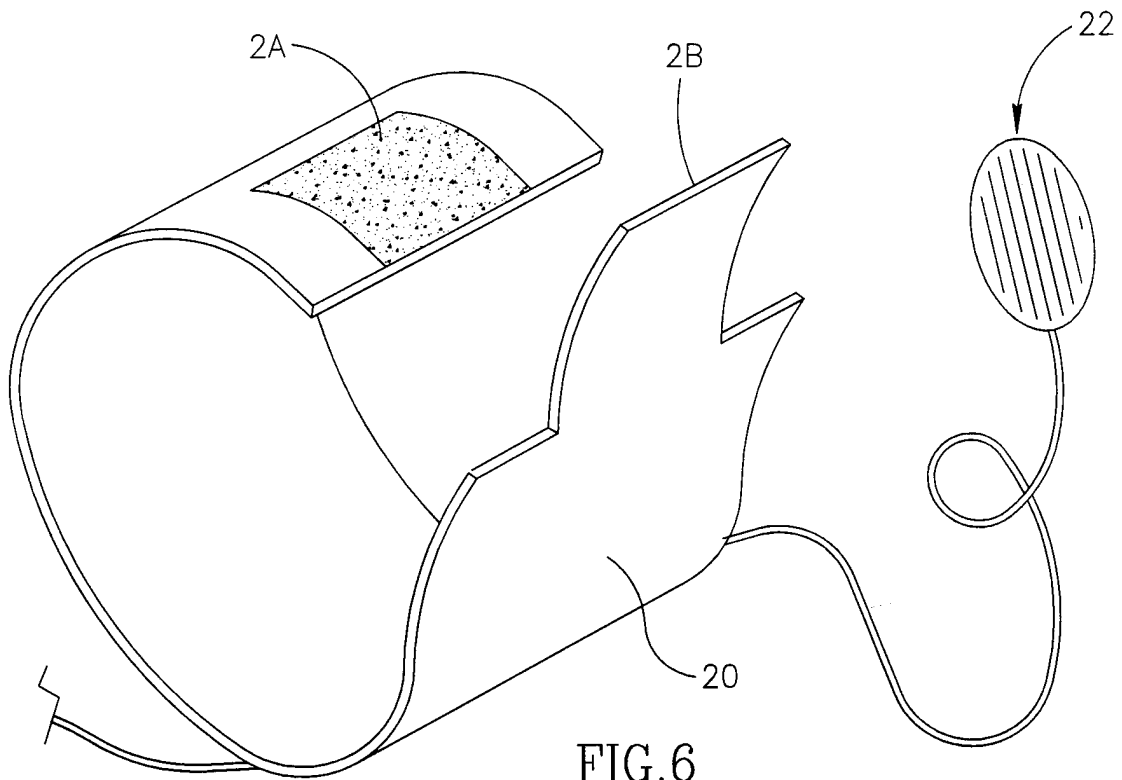


FIG. 6

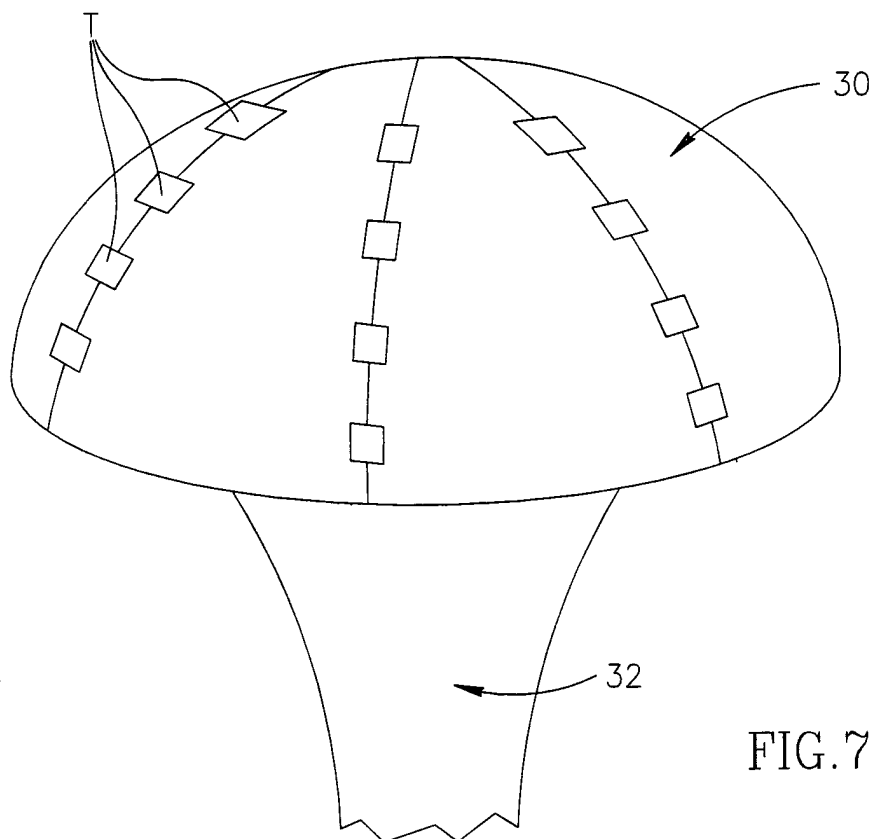


FIG. 7

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IL 00/00223

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61B8/13 A61B8/04

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 074 564 A (W.A. ANDERSON) 21 February 1978 (1978-02-21) column 1, line 46 -column 2, line 15 column 2, line 38 - line 50 column 5, line 58 -column 6, line 67 -----	1,5,7-9
A	FR 2 477 404 A (THOMSON-CSF) 11 September 1981 (1981-09-11) page 2, line 23 - line 33 -----	1,3-5
A	US 4 206 653 A (C.A.M. LE MAY) 10 June 1980 (1980-06-10) column 9, line 39 -column 10, line 9 -----	1,7-9

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search <p style="text-align: center;">7 August 2000</p>	Date of mailing of the international search report <p style="text-align: center;">14/08/2000</p>
Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo.nl, Fax: (+31-70) 340-3016	Authorized officer <p style="text-align: center;">Rieb, K.D.</p>

INTERNATIONAL SEARCH REPORT

Information on patent family members

Inte: onal Application No PCT/IL 00/00223
--

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
US 4074564	A	21-02-1978	CA	1050654 A		13-03-1979
			GB	1511023 A		17-05-1978
FR 2477404	A	11-09-1981	DE	3008975 A		01-10-1981
US 4206653	A	10-06-1980	GB	1554722 A		31-10-1979
			DE	2644889 A		18-08-1977
			FR	2326704 A		29-04-1977
			JP	52044684 A		07-04-1977
			US	4137775 A		06-02-1979

专利名称(译)	超声成像设备		
公开(公告)号	EP1168963A1	公开(公告)日	2002-01-09
申请号	EP2000919110	申请日	2000-04-14
[标]申请(专利权)人(译)	由于F R A Y项目		
申请(专利权)人(译)	磨损. PROJECT LTD.		
当前申请(专利权)人(译)	磨损. PROJECT LTD.		
[标]发明人	LEV KOVITZ ZEEV		
发明人	LEV KOVITZ, ZEEV		
IPC分类号	A61B8/00 A61B8/04 A61B8/13		
CPC分类号	A61B8/4483 A61B8/04 A61B8/13 A61B8/4227 A61B8/4427 Y10S128/916		
优先权	129461 1999-04-15 IL		
外部链接	Espacenet		

摘要(译)

提出了基于超声的成像装置(1)和软件操作的方法,用于监测身体部分并产生指示身体部分的内部结构的三维图像的数据。该装置(1)是便携式的,并且包括用于覆盖身体部分的基本上弹性的盖(1A),其中,盖连接到控制单元(1B)并且可连接到计算机装置。盖子承载超声波收发器(5)阵列,每个超声波收发器发射超声波束,用于照射由盖子覆盖的区域内的区域,并检测照射区域的信号响应。收发器(5)布置在至少两个间隔开的平行组中。每组的收发器以间隔开的关系布置,组中的每两个相邻收发器之间的空间使得在由相邻收发器照射的区域之间存在重叠。