

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
25 September 2003 (25.09.2003)

PCT

(10) International Publication Number
WO 03/077766 A1

(51) International Patent Classification⁷: **A61B 8/08**, 8/12,
G01N 29/00, G01S 15/00

(74) Agent: **ABC-PATENT, SIVILING. ROLF CHR. B. LARSEN A.S.**; Postboks 6150 Etterstad, N-0602 Oslo (NO).

(21) International Application Number: PCT/NO03/00089

(22) International Filing Date: 13 March 2003 (13.03.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/364,747 15 March 2002 (15.03.2002) US

(71) Applicants and


(72) Inventors: **ANGELSEN, Bjørn, A., J.** [NO/NO]; Bugges
veg 4B, N-7051 Trondheim (NO). **JOHANSEN, Tonni, F.**
[NO/NO]; Osloveien 6, N-7018 Trondheim (NO).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,

[Continued on next page]

(54) Title: MULTIPLE SCAN-PLANE ULTRASOUND IMAGING OF OBJECTS

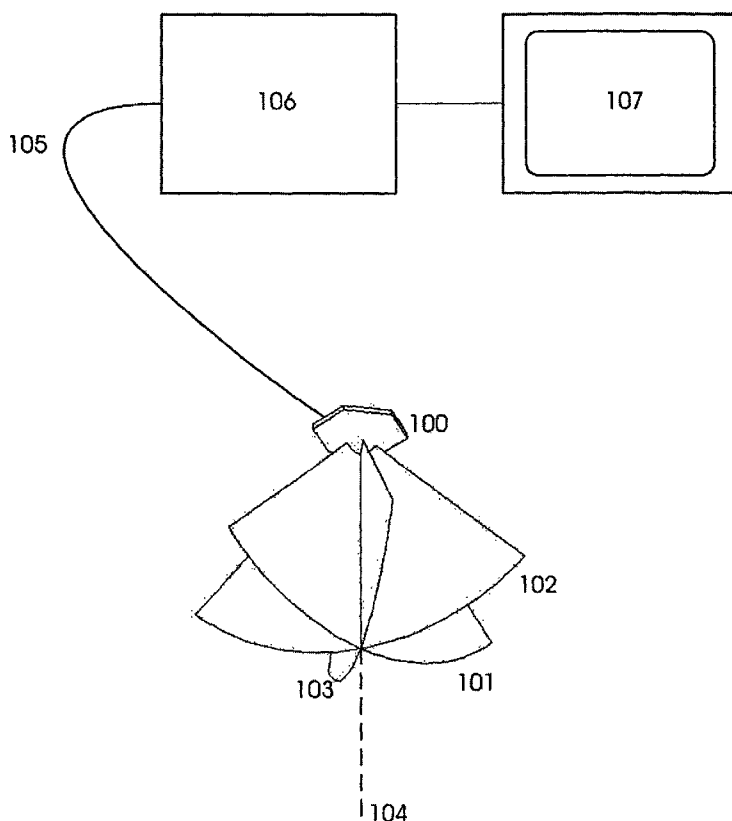

(57) Abstract: A method of real time ultrasound imaging of an object in at least three two-dimensional scan planes that are rotated around a common axis, is given, together with designs of ultrasound transducer arrays that allows for such imaging. The method is also introduced into a monitoring situation of cardiac function where, combined with other measurements as for example the LV pressure, physiological parameters like ejection fraction and muscular fiber stress is calculated.



WO 03/077766 A1



SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— *with international search report*

MULTIPLE SCAN-PLANE ULTRASOUND IMAGING OF OBJECTS

1. Field of the invention

5 The present invention is directed to real time ultrasound imaging of an object, like a biological structure, in multiple scan planes. Designs of efficient ultrasound phased array bulk wave transducers for two-dimensional ultrasound imaging, with several, electronically selectable 2D scan planes, are given.
10 The electronic selection of the 2D scan plane direction allows so rapid switching of the direction that practically real time observation of moving objects like the heart, can be obtained simultaneously in several scan planes. The invention also addresses real time ultrasound monitoring of the cardiac
15 function.

2. Background of the invention

In medical ultrasound imaging, one often examines an object through a variety of two-dimensional (2D) scan plane
20 directions to observe the form, regional variations, and volume of the object. In particular one uses such multiple scan plane imaging of the heart to assess regional variations in the wall motion and myocardial contraction/relaxation, as well as to calculate the time varying volume of the heart, or
25 the temporal variation of the fiber stress and strain in the heart. Other situations are observations of fetuses, tumors, etc., especially for calculating the volume to study growth.

In practical clinical examinations, such multiple 2D scan
30 planes are generally obtained through manual movement of the 2D ultrasound probe, where for example with transesophageal measurements of the heart with a 2D phased array probe, special mechanisms have been designed for rotation of the ultrasound array through remote control. A phased array
35 transducer for electronic selection of the ultrasound scan planes in two angular directions has been presented in [1], but this solution has found limited practical use, mainly because one wants to observe the object in more than two planes, generally at least three or four angular directions of
40 the 2D scan plane.

The present invention presents a solution to this problem, with the design of a phased array transducer that allows free electronic selection of the 2D scan plane in more than 2
45 angular directions, for example 3 or 4 angular directions.

3. Summary of the invention

The invention presents methods for practically real time ultrasound imaging of objects in 3 or more 2D ultrasound scan

planes, where the 2D scan-planes are rotated around a common axis. With practically real time is here meant that the image data is collected along a set of sample beams within said 2D scan planes, and the sample beam data collection occurs so frequently of the object that all the sample beam data defining the image is collected within so short time period in relation to movements of the object, that the collected data captures a for practical purposes frozen frame the moving object. The image data can in addition be displayed on an image screen with so slow delay that one for practical purposes can view the object as it moves.

Such multiple 2D real time imaging is useful to study regional variations in cardiac wall motion. Using image analysis for automatic selection of the edges of for example a heart cavity or a tumor, one can study dimension and volume variations of the object to study tumor growth or ventricular volumes and ejection fraction. Based on ventricular dimensions, one can calculate myocardial strain, and with Doppler analysis one can quantitate regional wall velocity and strain velocity of the myocardium in each beam direction. Doppler analysis can also be used with forced deformation of tissue to study regional variations in tissue elasticity with methods referred to as elastography. With added input of the left ventricular pressure, as for example during anesthesia or critical care monitoring, the invention also presents methods for real time calculation of the left ventricular fiber stress, for accurate observation of the physiological function of the myocardium. The invention hence devices the use of such imaging for monitoring of cardiac performance, for example during anaesthesia or other critical care monitoring.

The invention further presents detailed designs of ultrasound transducer arrays that allows sector scanning of an ultrasound beam in three or four 2D scan planes that are rotated around a common axis. The design is composed of at least two active piezoelectric, phased array transducer layers mounted face to face in a sandwich structure that is mounted on a backing material. The piezoelectric sandwich front face is connected to the load material through a set of elastic impedance interfacing layers for improving the acoustic power coupling between the piezoelectric layers and the load material. In a special wide band design, the impedance interfacing layer closest to the piezoelectric layers has the same characteristic impedance as the piezoelectric layers, as described in [5].

Both the front and back side electrodes of each array layer are formed as a set of isolated, parallel finger/element electrodes that are connected to a switching circuit. The finger/element directions on the front and back side of each layer form angles to each other. The finger/element directions of the different piezoelectric layers are arranged so that the

finger directions of at least one set of electrodes of one layer form an angle to the finger directions of at least one set of electrodes of other layers.

- 5 The switching circuit is electronically controlled so that the full set of finger electrodes of each piezoelectric layer surface can selectively be connected either to the hot wires of a phased array ultrasound imaging instrument, or connected to signal ground. This allows electronic selection of one of a
10 set of 2D scan plane directions for each transmitted pulse. With limited number of beams in each 2D image, one can get so high frame rate that when switching the scan planes sequentially, the images in the different scan planes show practically real time display of the object. Hence, the
15 imaging instrument can show real time display of 3 or 4 scan plane directions, for example to observe regional contraction abnormalities of the myocardium.

- Transmitting a wide beam and covering it with several narrow
20 receive beams in parallel, one can increase the frame rate by a factor of order 2 - 6. Other increase in the frame rate is obtained by reducing the beam density where the scan planes intersect, and where the beams have limited information about the object, for example internal in the left ventricle while
25 the ventricular walls are covered with high density of beams for ventricular wall motion analysis. For special high frame rate observation of the heart in the different scan planes, one can keep the same scan plane direction for a whole cardiac cycle, and change direction of the scan plane right before the
30 onset of the myocardial contraction, for example triggered by the ECG signal from the heart.

- The invention also shows a special embodiment where the multi-scan plane phased array is mounted at the tip of an endoscope
35 for imaging of objects from internal in the body. In particular, such a method is useful for transesophageal imaging of the heart in many scan planes, for example to assist anesthesia monitoring during surgery. The transesophageal array can further be rotated mechanically in
40 the endoscope for detailed alignment of the scan planes with interesting areas, or to increase the number of scan planes that are imaged.

- Ultrasound contrast agents can be used to observe regional
45 variations of myocardial blood perfusion. Such contrast agent can also be administered for efficient determination of the ventricular volumes. An example of an array embodiment is given that allows imaging in multiple frequency bands. This embodiment is well adapted for transmission of ultrasound
50 pulses within one band of frequencies, and reception in sub, 2nd, 3rd, or 4th harmonic component of the transmit band. Such harmonic imaging is especially useful for the detection of ultrasound contrast agent, both to assess regional variations

in the myocardial blood perfusion, and for automatic detection of the volume of ventricular cavities, and for detection of regions of tumors with increased vascularization.

5 4. Summary of the drawings

- Figure 1 shows in Figure 1a an example of an imaging system that allows real time imaging of an object simultaneously in three 2D scan planes, while Figure 1b
10 shows an example display of 3 real time 2D images, and Figure 1c illustrates a spiral scanning of ultrasound beam for observation of the myocardium with minimal lag between beams across the myocardium.
- 15 Figure 2 shows a cross section in the thickness direction of a typical layer structure of the transducer array, according to the invention,
- 20 Figure 3 shows a two-layer array with finger electrode structure that allows for electronic selection of three 2D scan planes as in Figure 1a,
- 25 Figure 4 shows transmit transfer functions that can be obtained with the transducer structure in Figure 3,
- 30 Figure 5 shows yet another transducer array structure with two piezoelectric layers according to the invention that allows for electronic selection of 4 scan planes,
- 35 Figure 6 shows example scan planes that can be selected with the transducer array structure in Figure 5,
- 40 Figure 7 shows how the scan planes can be selected with an electronic switching circuit located in the ultrasound probe close to the array, to minimize the number of cables connecting the probe to the imaging instrument,
- 45 Figure 8 shows a transesophageal probe with an ultrasound array and electronic switching circuit mounted at a tip of a gastroscope according to the invention,
- 50 Figure 9 shows transmission of the ultrasound beam within three selectable 2D scan planes rotated around a common axis with a 2D matrix array,
- Figure 10 shows by example displays of the image data, where Figure 10a shows example display of 4 simultaneous, real time 2D images, and Figure 10b shows a bullet display of myocardial strain data in three 2D images,
- Figure 11 shows temporal displays of cardiac physiological variables obtained with a cardiac monitoring instrument

according to the invention, showing both a fast time which displays variations within a heart beat, and a slow time frame that shows variation of parameters from beat to beat.

5

5. Detailed description of the invention

Several example embodiments according to the invention is presented in the following. It is clear that this
10 presentation is meant for illustration purposes only, and by no means represents limitations of the invention, which in its broadest aspect is defined by the claims appended hereto.

As an example embodiment of the invention, Figure 1a shows a
15 transducer array 100 that is capable of transmitting pulsed ultrasound beams with directions freely and electronically steerable within for example three 2D sector scan planes 101, 102, and 103, that are rotated with different angular
20 directions around a common axis 104. The transducer array is connected via a cable 105 to an ultrasound imaging instrument 106 with image outputs given to a display screen 107.

In a typical imaging situation, the ultrasound imaging
25 instrument 106 directs signals to the transducer that transmit ultrasound beams in selected directions within the 2D scan planes 101 - 103. The back scattered signal is for each beam direction analyzed in the instrument to generate a set of image parameters for a set of range samples along the beam
30 directions. Typical image parameters can be a compressed version of the backscattered amplitude for imaging of tissue structures, or Doppler frequency parameters for imaging of blood velocities, velocities of tissue movement, or strain of
35 tissue regions, for example myocardial strain, or enforced strain on a tumor for elastography imaging, all according to known methods.

The beam scanning can be done in many ways, for example sequentially for each 2D scan plane in turn, or in a spiral
40 pattern as described below. The image parameters for the beam directions that belong to each scan plane are then grouped together to form 2D images of the image parameters for the scan planes. These 2D images are then shown in real time on a display screen, for example as the images 111, 112, 113 in
45 Figure 1b. This Figure also illustrates a time trace 114 of a cardiac ECG to be used as timing reference, with an area 115 for display of alphanumeric data extracted from the images or other measurements.

- With 64 beams per 2D image with an image range of 15 cm, one typically obtains 72 2D images per second. With 3 sequential 2D scan planes one hence gets 24 full updates of the three 2D scan-planes per second. Increasing to 4 sequential scan
- 5 planes, one gets 18 full updates per second of the four 2D scan-planes. 64 beams with a 16 mm aperture array at 3 MHz give a total opening angle of the 2D image around ~ 60 deg with full angular sampling of the 2D image.
- 10 Transmitting a wide transmit beam and covering it with several (for example 2 - 6) narrow receive beams in parallel, allows an increase of the image rate by a factor 2 - 6. This also gives time for expanding the scan angle of each 2D scan-plane, for example to 90 deg. The image rate and/or the width of the
- 15 2D scan can also be increased by reduced beam density, especially in the overlap region of the planes close to the axis 104, and in regions with little information about the object, like the middle of the ventricle with apical long axis imaging of the heart. If faster 2D image rate is needed, for
- 20 example to study details in the onset of cardiac contraction and relaxation, one can image a full cardiac cycle for each scan plane, and change the scan plane at the end of the cardiac cycle, for example triggered by the ECG signal.
- 25 For assessment of regional wall motion abnormalities of the heart, it is important that the time delay is minimal between the beams that samples the wall in different regions. A useful cardiac scanning is then obtained by apical imaging of the ventricle, locating the array center axis 104 along the left
- 30 ventricle long axis, which in Figure 1c is shown as normal to the Figure in the center. A typical myocardium cross section is shown as the area 125 in this image. Cross sections of the scan planes 101, 102, 103 are shown as 121, 122, 123. In this particular beam scanning pattern, the scan plane direction is
- 35 switched in a circle for each sequential beam direction, so that the beam scanning occurs in a spiral cone with steadily increasing/decreasing angle of the beam to the axis 104. The crosses indicates some of the interrogating beams, where a selection 126, 127, 128, indicate a subset of the beams that
- 40 follow each other in a sequence in the direction 129. At the last beam 130 with this beam angle to the axis 104, the beam angle is increased so that the next beam cross section is 131 in the same scan plane 121 as the beam 126, but with larger (or possibly smaller) beam angle to the center axis 104. The
- 45 beam direction 130 is in this example followed by the beam direction 132 in 2D scan plane 122 and so on as indicated by the arrows. As the myocardium 125 with this scanning pattern is imaged with beams of close to the same opening angle between the beam and axis 104, one can cover the whole
- 50 myocardium in a limited time interval. Typically, the myocardium is covered with around $10 \times 6 \sim 60$ consecutive beams that can be collected in a time interval of 10 - 15 msec with a frame rate of ~ 80 frames per second. This provides a

highly adequate volume frame rate to study regional variations in the contraction, relaxation pattern of the myocardium.

5 For display, the image data from the beam directions belonging to each 2D scan plane are grouped together to form 2D images that are displayed in real time as exemplified in Figure 1b. The multiple scan planes can then be used for real time observation of regional wall motion in the heart and volume calculations of the heart cavities, both for diagnosis and for
10 peri and post surgical monitoring, and monitoring in other critical care situations, as discussed below.

Two embodiments of transducer arrays that provide the beam scanning according to the invention, is now presented.
15

Figure 2 shows a cross section in the thickness direction of a phased array according to the invention, where 201 and 202 show two piezoelectric array layers mounted on a backing structure 203 with so high acoustic power absorption that
20 reflected waves in the backing material can be neglected. The piezoelectric layers are covered with phased array finger/element electrodes 208, 209, 210, and 211. The front electrodes 209 of the back layer and the back electrodes 210 of the front layer are electrically isolated from each other
25 with the thin layer 212, for example a glue film. Between the piezoelectric layers and the acoustic load material 204, the structure contains a set of elastic layers 205 to interface the characteristic impedance of the piezoelectric layers (201, 202) to that of the load material 204.
30

A method for such impedance interfacing that gives a particularly wide bandwidth, is given in [5], where the first layer of structure 205 in contact with the piezoelectric layers contains an elastic layer with close to the same
35 characteristic impedance as the piezoelectric layers, followed by layers with falling characteristic impedance towards the load. Such an impedance interfacing is particularly useful when using the two piezoelectric layers in electrical parallel coupling to transmit a low frequency pulse, and then receive
40 higher harmonic components (2^{nd} to 4^{th}) of this pulse on for example the back layer 201, as described below. One might also transmit a pulse on layer 201 and receive a sub-harmonic pulse on the electrical parallel of layers 201 and 202, as described below. In other situations one can use more narrow-band
45 impedance interfacing layers 205, according to standard methods.

An example of dicing of the piezoelectric plates to obtain a reduced characteristic impedance ceramic/polymer composite,
50 with an arrangement of electrodes that allows phased steering of an ultrasound beam in three 2D planes, is shown in Figure 3, which shows the piezoelectric layers and electrodes from the faces. In Figure 3a, 301 shows dicing grooves of the ceramic

piezoelectric layers, the same for both layers, with the remaining ceramic posts/islands as 302. The dicing grooves 301 are filled with polymer to produce a ceramic/polymer composite structure with characteristic impedance reduced from that of the bulk ceramic material by a factor around 0.5, depending on the relative volume fill of ceramic.

In a particular embodiment according to the invention, the back face of the piezoelectric layer 201 is covered with a set of divided finger/element electrodes 303 as shown in Figure 3b, while the front face of the back layer 201 and the back face of the front layer 202 are covered with divided finger electrodes 304 and 305 that have the same shape and direction, as shown in Figure 3c. The front face of piezoelectric layer 202 is covered with divided finger electrodes 306 shown in Figure 3d. The electrode sets 303 - 306 corresponds to the electrodes 208 - 211 in Figure 2, where the finger electrodes 304 and 305 are electrically isolated from each other by the layer 212 as illustrated in Figure 2.

A principle drawing of the 2D scan planes that can be obtained with the array in Figure 3, is shown in Figure 1a, where the array is illustrated as 100. Grounding electrode sets 304/209, 305/210, and 306/211, and operating the back electrodes 303/208 as the hot electrodes of the elements of a linear phased array transducer, one will obtain a 2D image scan plane shown as 101 in Figure 1a. Grounding electrode sets 303/208, 305/210, and 306/211, and operating the electrodes 304/209 as the hot element electrodes of a phased array, one obtains a 2D image scan plane shown as 102 in Figure 1a. Grounding electrode sets 303/208, 304/209, and 305/210, and operating the front electrodes 306/211 as the hot element electrodes of a phased array, one obtains a 2D image scan plane shown as 103 in Figure 1a.

Choosing the dicing and electrode directions at 60 deg angle to each other as shown in Figure 2a - 2d, one gets an equilateral triangle of the ceramic islands, and 60 degrees angle between the 2D scan planes in Figure 1a, which gives an even angular sampling of the object. With such angles, one gets equal dimensions of the ceramic islands of the composite allowing equal width of the electrodes/elements of the array. Other angular divisions of the array/electrodes is also possible, for example to sample the left ventricle closer to other, wanted image planes.

The transduction capabilities of the array are conveniently described by the transmit transfer functions $H_{tt}(\omega)$ of the array elements, defined as the transfer function from the transmit voltage on the electrodes to the vibration velocity on the element front surface. Typical transmit transfer functions for the back layer 201 and the front layer 202, with the other layer electrically shorted, are shown as 401 and 402

in Figure 4, respectively. Both scan planes 101 and 102 in Figure 1a are using the back piezoelectric layer 201 of Figure 2 with the transfer function 401 with close to flat response in a wide frequency range of 1.5 - 4.2 MHz. Scan plane 103 of Figure 1a is using the front piezoelectric layer 202 of Figure 2 with the transfer function 402 of Figure 4. We see that both layers have similar transfer function (401 and 402) in the 2.8 - 4.2 MHz frequency range. Hence, within this frequency band, the pulses for the third scan plane 103 obtained with the front layer can be made similar to the pulses for the scan planes 101 and 102 obtained with the back layer.

In Figure 2, the polarizations of the piezoelectric layers are shown as P1 (206) and P2 (207). With opposite directions of the polarizations as shown in this example, one obtains electrical parallel coupling of the layers by grounding the front (211/306) and back (208/303) electrodes and operating the mid electrodes (209/304 and 210/305) as the hot electrodes of a phased array. The transmit transfer function for such electrical parallel coupled operation of the piezoelectric layers, is shown as 403 in Figure 4. We notice that this transfer function covers a lower band of frequencies from 0.8 - 2.2 MHz.

Hence, aside from the ability to electronically select three scan planes, the structure allows for operations in multiple frequency bands in scan plane 102, both for regular 1st harmonic imaging in multiple frequency bands and for harmonic imaging. For example, with electric parallel coupling of the layers as described above, one can transmit in a low frequency band 403. Grounding electrodes 208/303, 210/305, and 211/306 while operating 209/304 as the hot element electrodes of a phased array, one can receive 2nd, 3rd, or 4th harmonic components of the transmit band 401 with the back layer. Similarly, one can transmit in a high frequency band with grounded electrodes 208/303, 210/305, 211/306 and operating electrodes 209/304 as the hot element electrodes of a phased array, and receive sub harmonics of the transmit band by grounding electrodes 208/303 and 211/306, and connecting electrodes 209/304 and 210/305 to operate the two layers electrically in parallel for a low frequency band.

A dual piezoelectric layer structure that provides free selection of 4 scan planes, is shown in Figure 5, which shows the piezoelectric layers and electrodes from the faces as in Figure 3. In the thickness direction, the structure contains two piezoelectric layers, with an impedance interface of elastic layers to the load, as shown in Figure 2. In Figure 5a is shown an example of dicing of the ceramic piezoelectric layers, where 501 shows the dicing grooves and 502 shows the ceramic posts/island. The difference to the structure in Figure 3 is found in the ceramic dicing to form the ceramic/polymer composite, and the directions of the

finger/element electrodes. In particular, for the structure in Figure 5 the two sets of intermediate electrodes 504/209 and 505/210 between layers 201 and 202 have different directions as shown in Figures 5c and 5d. The back side of layer 201 is
5 furnished with a set of finger electrodes 503/208 shown in Figure 5b, and the front side of layer 202 is furnished with a set of finger electrodes 506/211 shown in Figure 5e.

We see that by grounding the electrodes 504/209, 505/210 and 506/211, and operating the back electrodes 503/208 as the hot
10 element electrodes of a linear phased array, we obtain a 2D scan plane shown as 601 in Figure 6. Grounding the electrodes 503/208, 505/210 and 506/211, and operating the electrodes 504/209 as the hot element electrodes of the phased array, we
15 get the 2D scan plane 602 in Figure 6. Grounding the electrodes 503/208, 504/209 and 505/210, and operating the electrodes 506/211 as the hot element electrodes of the phased array, we get the 2D scan plane 603 in Figure 6. Grounding the electrodes 506/211, 503/208 and 504/209, and operating the
20 electrodes 505/210 as the hot electrodes of a phased array, we get the 2D scan plane 604 in Figure 6. The transfer function for the back and the front layers will be the same as 401 and 402 shown in Figure 4, while this structure will not allow phased array scanning with electric parallel coupling of
25 the layers in the low frequency band 403.

Electronic selection of the illustrated scan planes can be done with an integrated circuit as for example illustrated in Figure 7. This Figure shows by example as 701 the multi
30 layer/multi electrode transducer array of Figure 3. Wire sets 703, 704, 705, and 706 connects the electrode sets 303, 304, 305, and 306 to the electronic switching circuit 702, which by the control signals 707 selects the set of electrodes to be connected to the hot wires of the set of coaxial cables 708
35 that are fed to the imaging instrument 710, and the set of electrodes that are connected to the signal ground level 709. Such an electronic circuit can be mounted close to the array, so that only the cables 708 and the control signals 707 for the scan plane selection is connecting to the imaging
40 instrument.

The transducer array and the scan plane selection circuit is then typically mounted at the tip of a hand held probe for
45 imaging from the body surface, or at the tip of an endoscope, like a gastroscope, for imaging of objects from inside the body, for example transesophageal imaging of the heart or endoscopic imaging of a tumor.

Figure 8 shows by way of example a transesophageal probe 800
50 with an array 801 according to this invention mounted at the tip of the gastroscope that is inserted into the body. The angular directions of the steerable tip 802 of the probe are controlled via wires by the rotation handles 803 and 804,

according to standard methods for wire control of the tip of endoscopes. This particular embodiment contains an additional control 805 for rotation as indicated by the arrow 806 of the array 801 within the gastroscope tip 802, for example to
5 adjust one of the scan planes to follow the long axis of the heart. The other scan planes are then grouped around this long axis according to the design of the array. This adjustment can be used for standardized observation of regional wall motion of the heart or accurate calculation of the volume of heart
10 cavities or other objects like tumors. The endoscope probe is connected to the imaging instrument through the cable 807.

Electronic steering of the beam within a selected set of 2D scan planes, can also be done with a two-dimensional matrix
15 array illustrated as 900 in Figure 9. This array is composed of a set of small elements 905 located in a 2D matrix, and where the signal for each element can be individually delayed. By delaying the signals of the individual elements, the beam can be steered and focused in a selected directions within a
20 cone 906, according to known principles. In particular one can select beam directions within a set of 2D scan planes 901, 902, 903 which allows scanning of the ultrasound beam as described above. However, the 2D matrix array severely increases the complexity of the ultrasound scanning system,
25 compared to the arrays in Figures 3 and 5.

Electronic selection of the 2D scan planes from a set, allows practically simultaneous imaging of the heart in 3 or 4 scan planes with the above described arrays, as discussed in
30 relation to Figure 1. Here, Figure 1b shows by way of example a display of real time imaging with three 2D scan planes that for example could be obtained with the array in Figure 3. Similarly Figure 10a shows the display of 4 real time scan planes for example obtained with the array in Figure 5. In
35 this example the 2D image displays 1001-1004 could correspond to the 2D scan planes 601 - 604 in Figure 6. A time trace 1005 showing the ECG for timing references, is included in the display together with a region 1006 for display of
40 alphanumeric data, like the end diastolic and end systolic ventricular volumes, the ejection fraction, etc. The images in Figure 1a and 10 can typically be used for wall motion scoring, where the score data can be presented in a bullet image, according to well known principles.

45 Through automatic detection of the ventricular cavities in the 2D images, one can do real time calculation of the volumes of the heart cavities, especially the left ventricle as shown in [6], to study filling and ejection patterns, and also the ejection fraction of the left ventricle. Ultrasound contrast
50 agent can be used to study regional perfusion variations in the myocardium, where harmonic imaging of the contrast agent improves the contrast to tissue power ratio. Ultrasound

contrast agent can also be used in difficult to image patients for improved determination of the cavity regions.

In many monitoring situations, a measured left ventricular pressure $p_{LV}(t)$ is available throughout the whole cardiac cycle. In critical situations, like peri and post surgery, $p_{LV}(t)$ can be obtained with a catheter in the left ventricle. In other situations, one can obtain $p_{LV}(t)$ from the aortic pressure throughout systole when the aortic valves are open. The aortic pressure can be obtained from a catheter in a central vessel, or through diameter measurements of the subclavian or carotid vessels. Combined with ultrasound measurements of the left ventricular diameter, $D(t)$, and wall thickness, $H(t)$, one can calculate the fiber stress $\sigma_f(t)$ in the myocardium according to known methods [7] as

$$\sigma_f(t) = \frac{H(t)}{(D(t)+H(t)) \left(3 - \left(\frac{D(t)+H(t)}{2L(t)} \right)^2 \right)} p_{LV}(t) \quad (1)$$

where $L(t)$ is the length of the left ventricular cavity. $L(t)$ can in most situations be approximated by a constant average value. As the myocardial muscle volume is constant, one can also obtain the temporal variations of the wall thickness $H(t)$ from $D(t)$ and $L(t)$. The left ventricular volume V_{LV} can then be approximated by the truncated ellipsoid and calculated based on $D(t)$ and $L(t)$.

There also exists a formula for calculating the fiber stress from the left ventricular cavity volume, V_{LV} , and the myocardial wall volume V_w [8] as

$$\sigma_f(t) = \frac{3}{\ln \left(1 - \frac{V_w}{V_{LV}(t)} \right)} p_{LV}(t) \quad (2)$$

Such calculations hence allows, according to the invention, real time displays of advanced physiological contraction/relaxation parameters of the myocardium. Temporal differentiation of the parameter wave-forms, including the volume traces, enhances information about the physiological function during the rapid changes at the onset and the end of the contraction.

The average relative strain in the myocardial fibers in a ventricle with close to uniform contraction of the myocardium in all regions, can be approximated as equal to the relative variation in the cardiac diameter, $\epsilon_a(t) = D(t)/D_{max}$. With

regional variations in the strain, as found with ischemic heart disease, the average strain is still an interesting measure of the cardiac performance, but in this situation one would also like to see an image of the regionally variable

5 strain $\varepsilon(\underline{r}, t)$, where \underline{r} is a vector coordinate of the of the myocardial surface. Based on Doppler measurements along each beam direction, one can estimate the local strain rate in the myocardium, which can be displayed in different ways, for
 10 example as color or grey scale indications in the bullet image 1007 in Figure 10b, where the angular direction in the bullet image indicates the angular direction of the scan planes of 101, 102, and 103 Figure 1, and the radial direction in the bullet image indicates the distance from the apex of the heart.

15 To further illustrate the monitoring situation, Figure 11 shows an example display according to the invention, where the dimensional measurement of the heart obtained with the arrays according to the invention is used to calculate contractile
 20 parameters of the left ventricle. The display shows from the top to bottom, the ECG traces 1101, the left ventricular pressure 1102, the fiber stress 1103 and average, relative fiber strain 1104, and the left ventricular volume traces 1105. For trend information over a longer time period, one can
 25 show in a slower time scale the end systolic volume, ESV (1106), as the minimum of V_{LV} per beat, the end diastolic volume, EDV (1107), as the maximum of V_{LV} per beat, the stroke volume, SV (1108), cardiac output, EF (1109), and the ejection fraction, CO (1110), calculated as

30
$$\begin{array}{lll} SV = EDV - ESV & CO = SV * HR & EF = SV / EDV \\ & & (3) \end{array}$$

35 where $HR = 60 / THR$ is the number of beats per minute calculated from the duration THR of the cardiac cycle per beat in seconds, for example measured for each heart beat from the ECG. These parameters together with HR (1111) and other parameters as for example $\max(dV/dt)$, $\max(\sigma_f)$, $\max(d\sigma_f/dt)$, $\max(\varepsilon_a)$, $\max(d\varepsilon_a/dt)$, etc. can conveniently be displayed as
 40 numbers for each heart beat along each trace or in an alphanumeric area 1112.

Thus, while there have shown and described and pointed out fundamental novel features of the invention as applied to a
 45 preferred embodiment thereof, it will be understood that various omissions and substitutions and changes in the form and details of the devices illustrated, and in their operation, may be made by those skilled in the art without departing from the spirit of the invention. For example, it is
 50 expressly intended that all combinations of those elements and/or method steps which perform substantially the same function in substantially the same way to achieve the same

results are within the scope of the invention. Moreover, it should be recognized that structures and/or elements and/or method steps shown and/or described in connection with any disclosed form or embodiment of the invention may be
5 incorporated in any other disclosed or described or suggested form or embodiment as a general matter of design choice. It is the intention, therefore, to be limited only as indicated by the scope of the claims appended hereto.

10 References:

[1] US Pat 4,640,291 Feb. 3, 1987: "B-plane phased array for ultrasound medical imaging" Inventor: Pieter 't Hoen.
Assignee: North American Philips Corporation

15 [2] US Pat 5,724,976, Mar. 10, 1998: "Ultrasound Imaging Preferable to Ultrasound Contrast Echography" Inventors: Yoshitaka Mine, Makota Hiramata, Hiroyuki Tsujino, Shiro Saito.
Assignee: Kabushiki Kaisha Toshiba, Kawasaki, Japan

20 [3] US Pat 5,825,117 Oct. 20, 1998: "Second Harmonic Imaging Transducers" Inventors: William J. Ossmann, Larry Pendergass, Martin K. Mason. Assignee: Hewlett-Packard Company, Palo Alto Calif.

25 [4] US Pat 5,957,851 Sep. 28, 1999: "Extended Bandwidth Ultrasonic Transducer" Inventor: John Hossack. Assignee: Acuson Corporation, Mountain View, Calif.

30 [5] US Pa Appl 60/260,023 Filed Jan 05 2001: "Wide or Multiple Frequency Band Transducer and Transducer Arrays". Inventors: Bjørn A. J. Angelsen and Tonni F. Johansen

35 [6] Aakhus S., Mæhle J., Bjørnstad K.: "A new method for echocardiographic computerized three-dimensional reconstruction of left ventricular endocardial surface: In vitro accuracy and clinical repeatability of volumes." J Am Soc Echocard, Vol 7, No6, 1994:571-581

40 [7] Rabben S.I., Irgens F., Angelsen B. : "Equations for estimating muscle fiber stress in the left ventricular wall", Heart and Vessels 1999, 14:189-196

45 [8] Arts T, Bovendeerd PHM, Prinzen FW, Reneman RS: "Relation between left ventricular cavity pressure and volume and systolic fiber stress and strain in the wall." J Biophys 59, 1991:93-102

We claim:

1. A method for practically real time ultrasound imaging of an object in at least 3 different 2D image planes, the method
5 contains the steps of
 - electronically scanning with an ultrasound transducer array a pulsed ultrasound beam with electronically and freely selectable beam directions within at least 3
10 different sector scan planes that are located with different angular directions around a common axis, the beam direction being switchable both within and between the 2D scan planes from pulse to pulse, and
 - 15 - using the back scattered signal from the pulses in each beam direction to form image data as a function of depth along image sample beam directions,
 - 20 - grouping the image data from each said image sample beam directions together to form 2D images of the object from each scan plane that are obtained with such high frame rate,
 - 25 - so that for practical purposes related to object movements, real time 2D images from said at least 3 different 2D scan planes can be shown on a display screen.
2. A method according to claim 1, where the ultrasound
30 transducer array allows sector scanning of the ultrasound beam within a fixed number of 2D scan planes, where the number of 2D scan planes is at least 3, and a particular 2D scanplane of the said fixed number of 2D scan planes can be selected electronically with negligible switching time for each transmitted pulse.
35
3. A system for ultrasound imaging of an object in at least 3 different 2D image scan planes according to claim 1, the system comprising
 - 40 - an ultrasound transducer array that allows sector scanning of the ultrasound beam within at least 3 different 2D scan planes, where the beam direction can be electronically selected from pulse to pulse, freely between the 2D scan planes and within each 2D scan plane,
 - 45 - the transducer array being connected to an imaging instrument that comprises:
 - 50 - means for analyzing the back scattered signal from the beam directions to form image data as a function of depth along the beam directions,
 - means for grouping the image data from said beam

directions to form 2D images of the object from said at least three 2D scan planes,

5 - means for displaying said 2D images of the object on a common display screen in real time,

10 - selecting a scanning pattern of said beams in relation to number of 2D scan planes and movements of the object so that the ultrasound images can be presented with so high frame rate,

15 - that for practical purposes related to the object movements, real time imaging of the moving object in said 2D scan planes is obtained.

4. An ultrasound imaging system according to claim 3, where the 2D scan plane is changed in a circle for each 2D beam sampling, so that a 3D scanning of the object in a spiral cone is obtained, for observation of the object with
20 minimal delays between sampling beams in neighboring 2D scan planes.

5. An ultrasound monitoring system for cardiac function, including an ultrasound 2D imaging system according to
25 claim 1 and also several cardiac physiological measurements.

6. An ultrasound monitoring system for cardiac function according to claim 5, where automatic edge detection is
30 done in the ultrasound images for automatic calculation of the volume of heart cavities, and/or calculation of relative strain in the myocardial fibers.

7. An ultrasound monitoring system for cardiac function according to claim 6, where ventricular dimensions or
35 volume are combined with ventricular pressure measurements to calculate the fiber stress in the cavity walls.

8. An ultrasound monitoring system for cardiac function according to claim 6 or 7, where simultaneous visualization
40 of the multiple scan planes of the heart is done on one part of the display screen, or on a separate display screen, while temporal variation of parameters derived from the ultrasound images and other physiological measurements
45 are shown as a function of time on other parts of the display screen, or on a separate display screen.

9. An ultrasound monitoring instrument for cardiac function according to claim 8, where minimum and maximum values of
50 the temporal traces for each cardiac cycle, are shown in a slow time scale on the same monitor or on a separate monitor.

10. An ultrasound transducer array capable of phased array direction steering and focusing of an ultrasound beam within a set of 2D scan planes that can be electronically selected, where the number of 2D scan planes is at least 3, characterized by that
- 5
- the array is build up of at least two piezoelectric array layers mounted face to face in a sandwich structure with a front and a back direction,
 - 10
 - the back face of the piezoelectric sandwich is mounted on a backing material and the front face of the sandwich is adapted to be connected to the acoustic load material through at least one elastic layer for acoustic impedance
 - 15 interfacing between the piezoelectric layers and the load material,
 - on each face of the piezoelectric layers is attached a set of parallel finger electrodes where the electrodes are electrically isolated from each other, the directions of
 - 20 the fingers on the front and the back face for each piezoelectric layer forms a non-zero angle to each other,
 - each set of finger electrodes on said faces are adapted to selectively be connected as the hot element electrodes to a phased array beam former, or connected to the beam
 - 25 former signal ground,
 - so that selectively connecting the whole set of finger/element electrodes on one side of at least one piezoelectric layer as the hot element electrodes to the beam former, and grounding all other sets of finger
 - 30 electrodes on the other faces of the piezoelectric layers, one obtains a linear phased array transducer where the angular direction of the 2D scan plane around a common
 - 35 axis, is determined by the set of the finger electrodes that are selected as the hot electrodes of the array.
11. An ultrasound transducer array according to claim 10, where the piezoelectric layers are made as a composite of ferroelectric ceramic and polymer, where
- 40
- the composite structure is the same through all piezoelectric array layers in the sandwich and the ceramic posts of the composite are separated from each other with
 - 45 at least some linear grooves filled with polymer,
 - said linear grooves conforms with the separations between said finger electrodes on the face of the piezoelectric layers, and hence also the active phased array elements defined by the electrodes connected the hot element wires
 - 50 of said beam former.

12. An ultrasound transducer array composed of two piezoelectric array layers according to claim 11, where
- 5 - the ceramic posts in said composite structure has a triangular cross section, the triangles being arranged so that the dicing of the ceramic can be done to form straight grooves,
 - 10 - some of said straight grooves filled with polymer defines the separation between the finger electrodes and hence also the selected, active phased array elements,
 - 15 - the finger electrodes of one face of each piezoelectric layer having the same, first direction, while the direction of the finger electrodes of the other faces are different from each other and different from said first direction.
13. An ultrasound transducer array composed of two piezoelectric array layers according to claim 12, where
- 20 - the ceramic posts in the composite structure has a cross section of an equilateral triangle, the triangles being arranged so that the dicing of the ceramic can be done in straight lines with 60 deg inclination to each other,
 - 25 - the separation of the finger/element electrodes on the piezoelectric layer surface, conforms with straight lines of polymer in the composite, so that the directions of the finger electrodes forms angles of 60 deg with each other.
14. An ultrasound transducer array according to claim 12, where the piezoelectric layers have opposite polarization directions, and
- 35 - for operation in a lower frequency band in one 2D scan plane normal to said, first direction, the two set of finger electrodes having the same, first direction are connected to each other to form the hot electrodes of a phased array,
 - 40 - while the other set of electrodes are coupled to signal ground so that electric parallel operation of the layers is obtained for operation in a lower frequency band, and
 - 45 - for operation in a higher frequency band with the 2D scan plane also normal to said, first direction, only the electrodes of the front or the back layer with the said, first direction are used as the hot electrodes of the phased array, while all the other sets of finger electrodes
 - 50 are connected to signal ground.
15. An ultrasound transducer array composed of two piezoelectric layers according to claim 10, where the

- 5 directions of the front and back face finger electrodes for each piezoelectric layer form an angle with each other, and the directions of the back finger electrodes of the front piezoelectric layer and the front finger electrodes of the back piezoelectric layer form an angle with each other, so that all the four sets of finger electrodes on the four faces of the piezoelectric layers forms non-zero angles to each other.
- 10 16. An ultrasound transducer array composed of two piezoelectric layers according to claim 15, where the directions of the front and back face finger electrodes for each piezoelectric layer form 90 deg angle with each other, and the directions of the back finger electrodes of the front piezoelectric layer and the front finger electrodes of the back piezoelectric layer form an angle of 45 deg with each other.
- 15 17. An ultrasound transducer array according to claim 11 and 16, where the ceramic posts in the composite structure has a cross section of an isosceles triangle with top angles of 90 deg, the triangles being arranged so that the dicing of the ceramic can be done in straight lines with 45 deg inclination to each other.
- 20 18. An ultrasound transducer array for phased array imaging with electronic selection of multiple scan plane directions according to claim 10, where
- 25 - close to the transducer array there is mounted an electronic switching circuit,
- 30 - the individual finger electrodes of the electrode sets of each piezoelectric layer face are electrically connected to the switching circuit,
- 35 - the switching circuit being able to connect the electrode set of one freely selectable face of the piezoelectric layers to the hot wires of the ultrasound beam former, while the electrode sets of the other faces of the piezoelectric layers are connected to signal ground.
- 40 19. An ultrasound transducer probe composed of an endoscope with an ultrasound array according to claim 10 mounted at the tip of the endoscope to be inserted into an object, for ultrasound imaging of internal structures in the object.
- 45 20. An ultrasound transducer probe according to claim 19, where the tip of the endoscope is flexible and where the flex of the tip can be steered by control at the external end of the endoscope.
- 50

21. An ultrasound transducer probe according to claim 19,
where the array can be rotated in the endoscope tip
controlled by means at the external end of the endoscope,
or in the imaging instrument.
- 5
22. An ultrasound 2D phased array imaging system according to
claim 3 capable for operating the multiple set of parallel
finger electrodes of a phased array transducer according to
claim 10, the ultrasound imaging instrument also providing
10 electronic selection signals to control the electronic
selection of which element set is connected to the hot
wires of the system, and which element sets are connected
to signal ground, for selection of the ultrasound scan
planes for 2D imaging, either through manual control from
15 the instrument control panel, or through automatic
selection of the scan planes in a sequence, for example
changing the scan plane for each beam, or from 2D frame to
2D frame, or changing the scan plane in a slower manner,
for example triggered by a signal derived from a
20 physiological signal like the ECG.

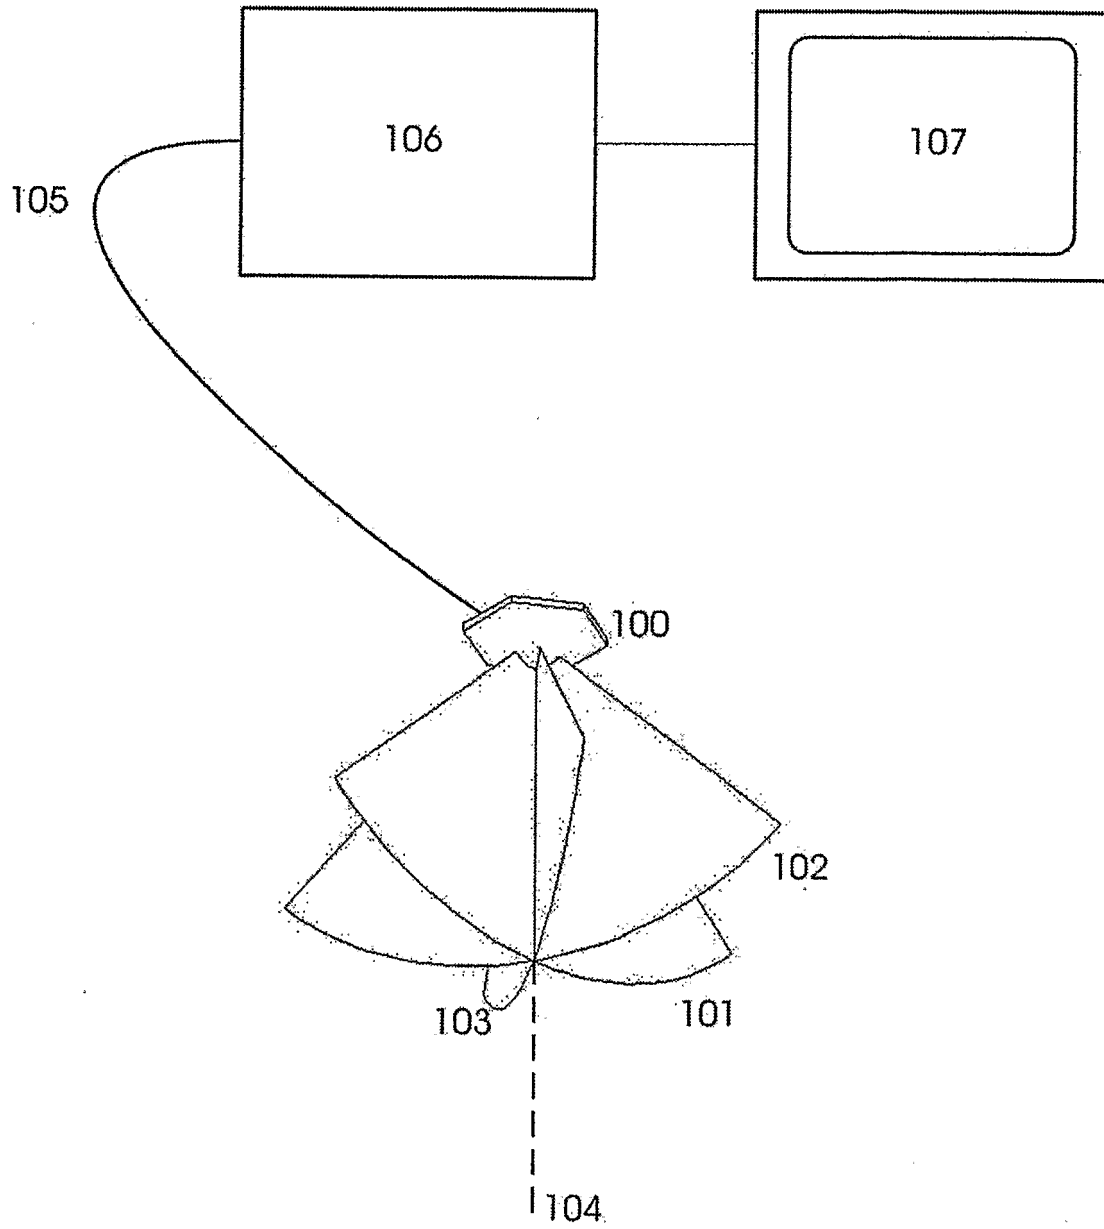


Figure 1a

2/21

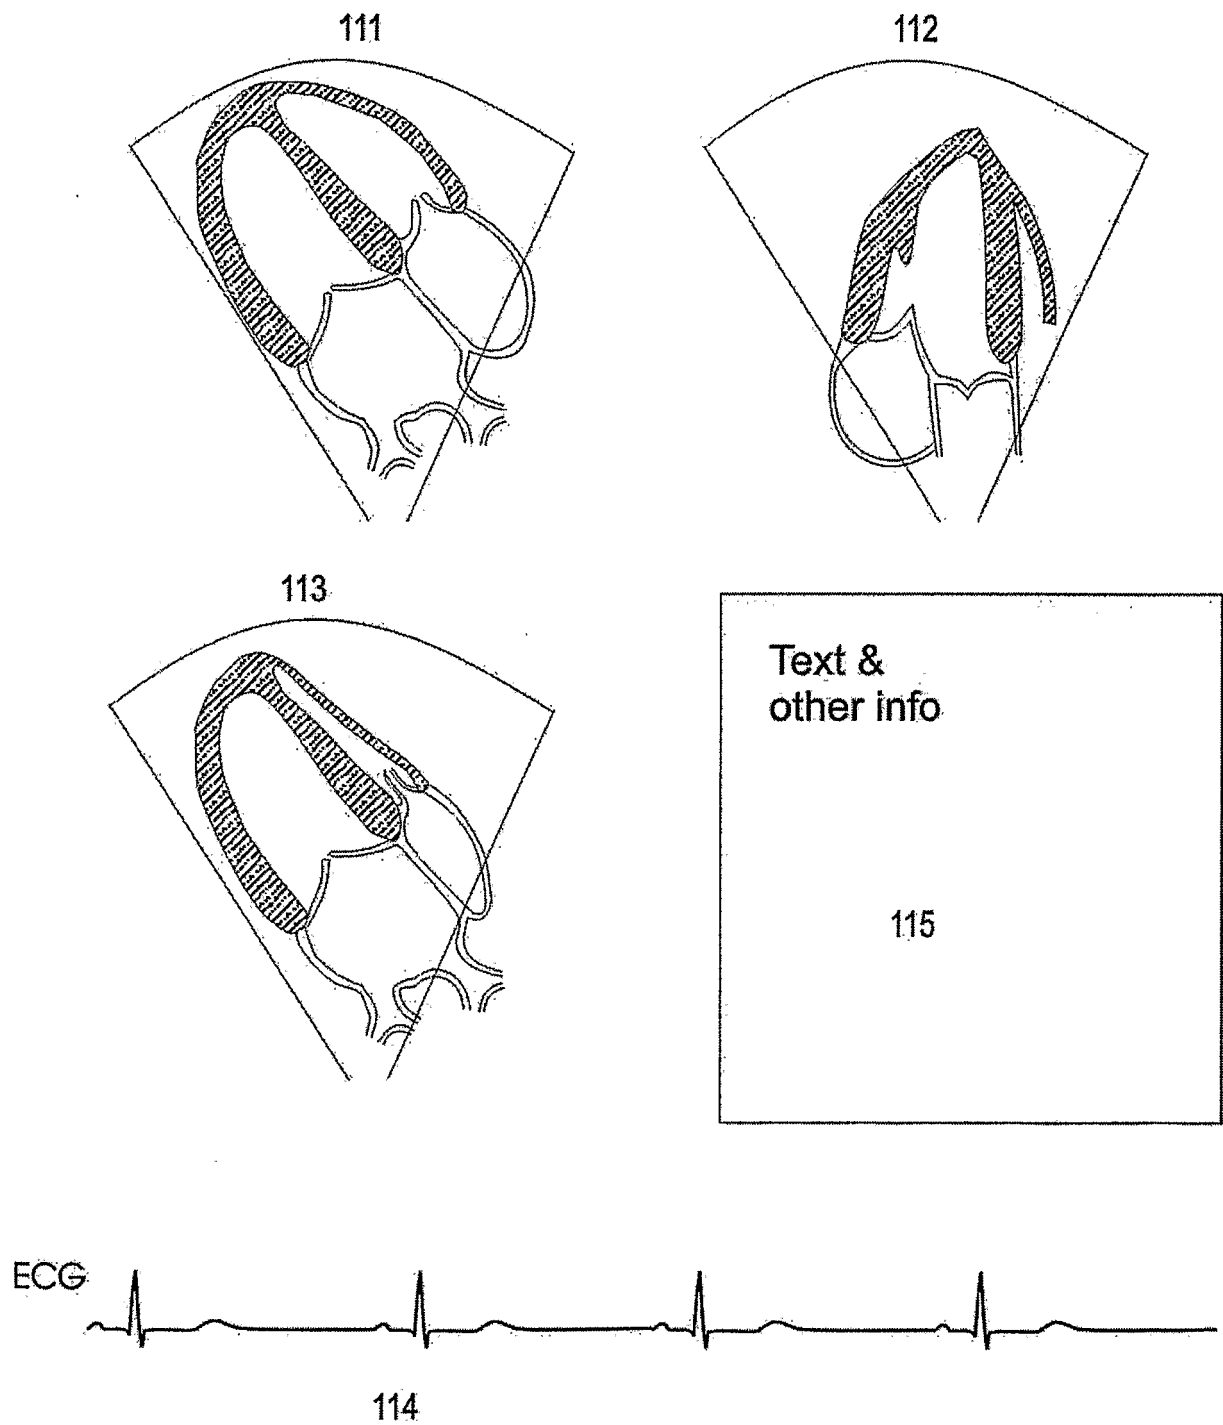


Figure 1b

3/21

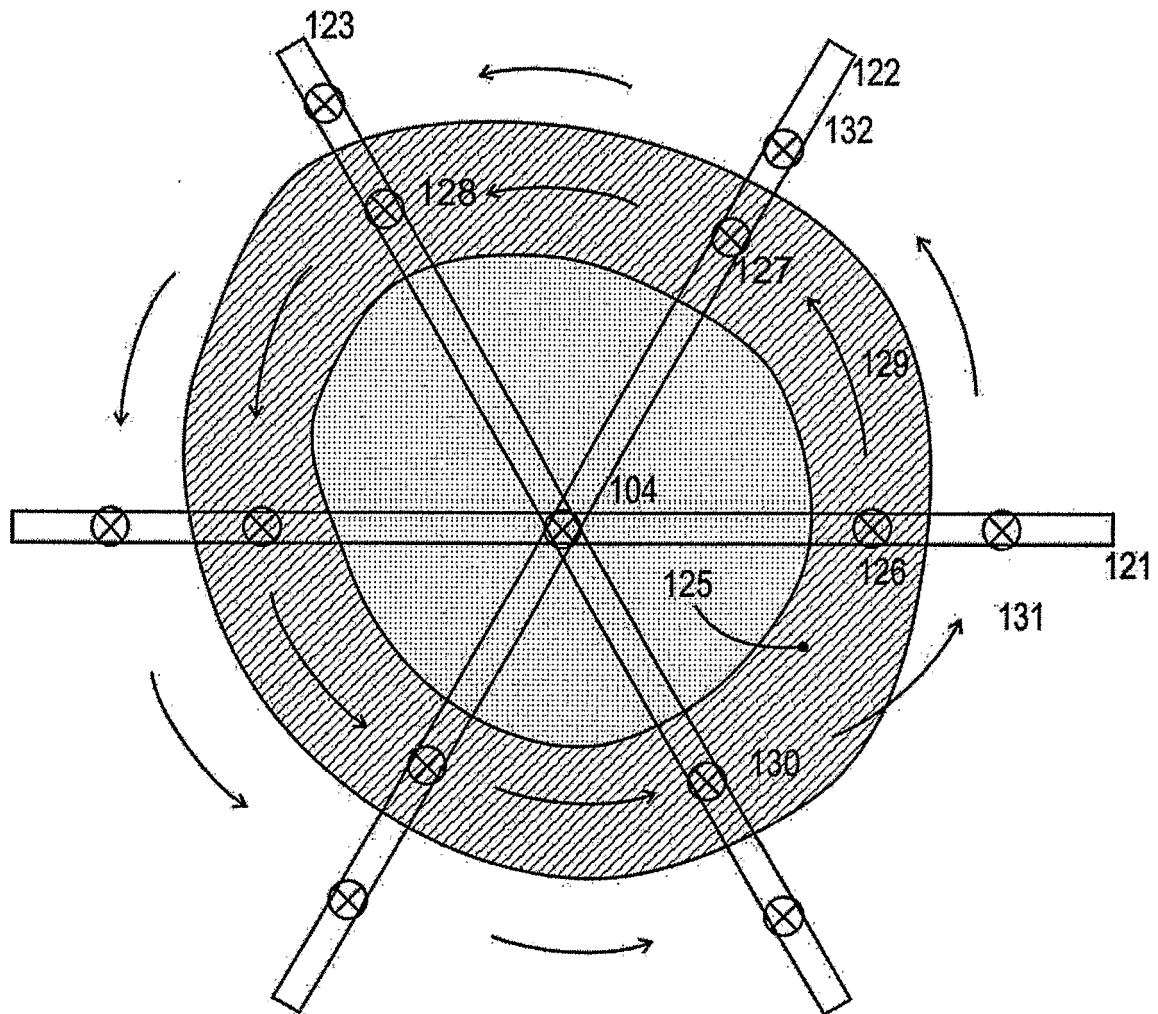


Figure 1c

4/21

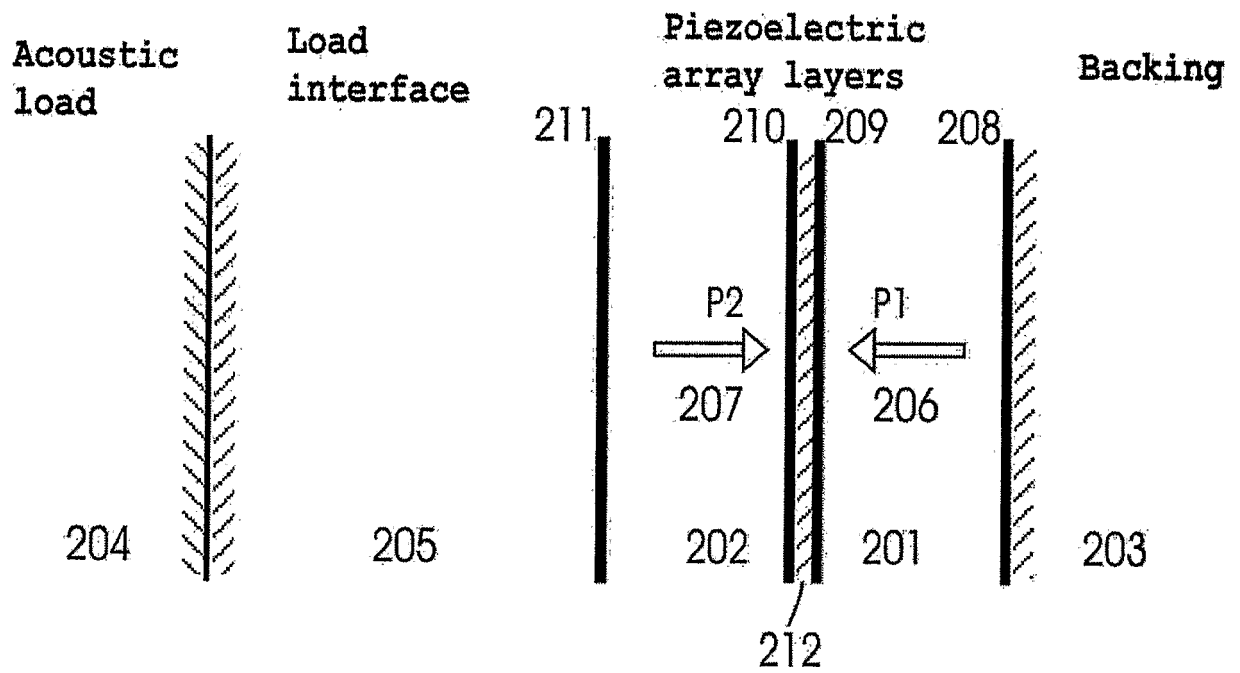


Figure 2

5/21

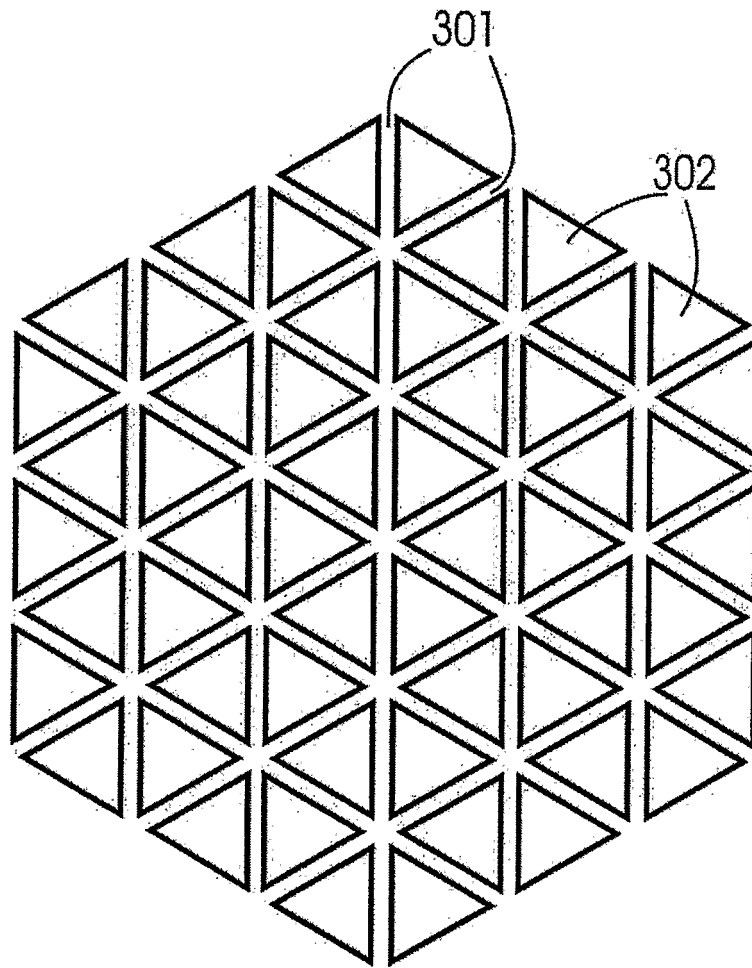


Figure 3a

6/21

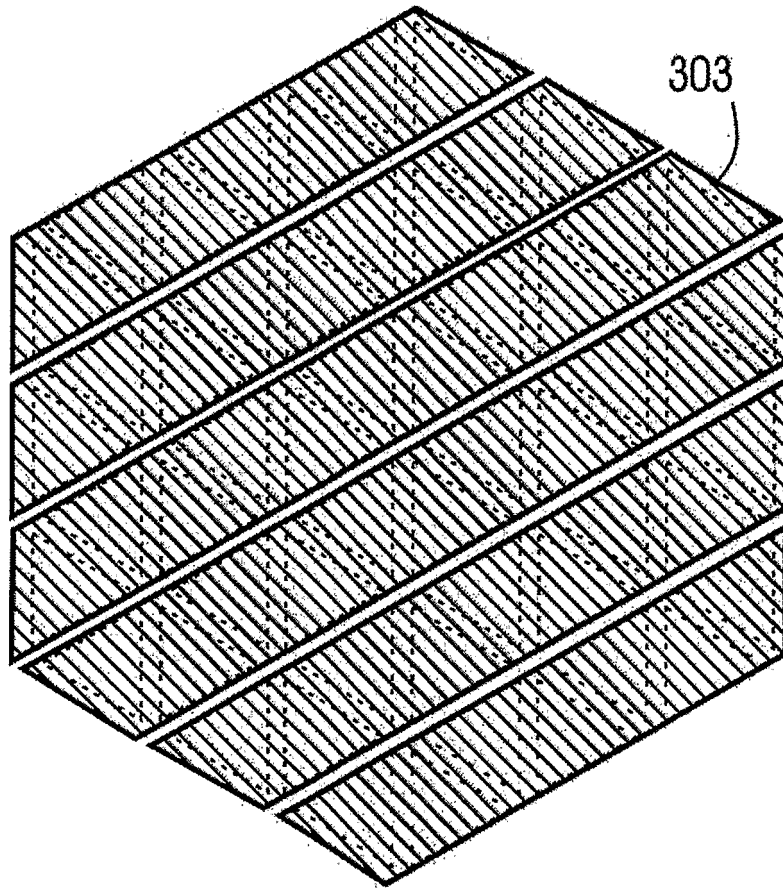


Figure 3b

7/21

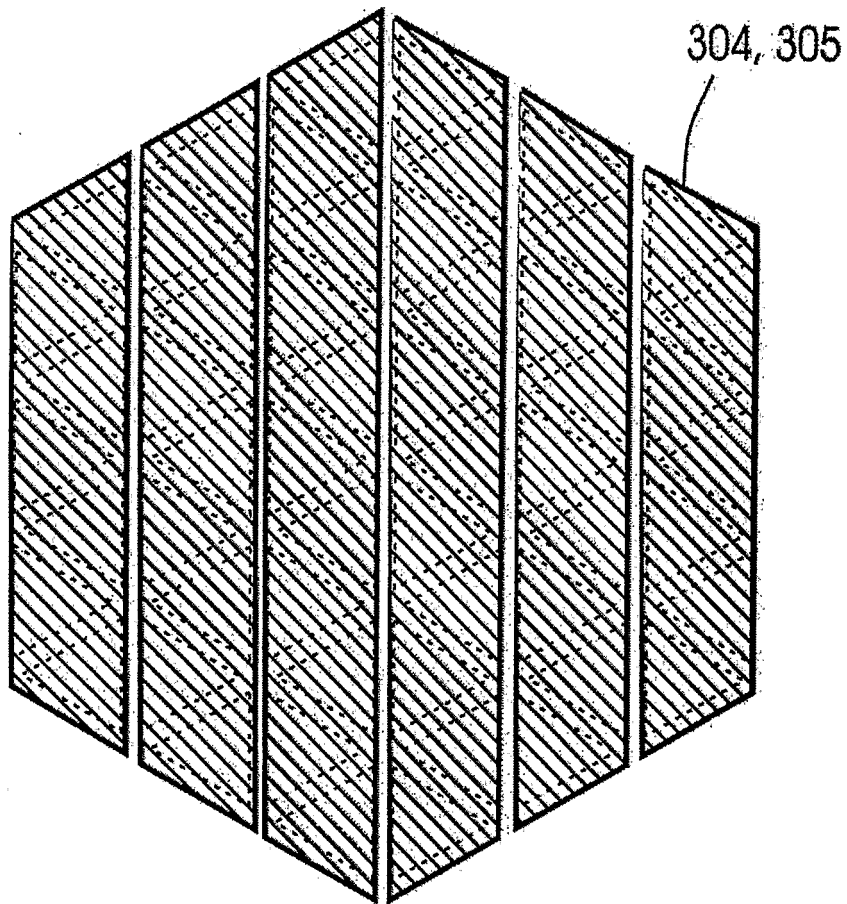


Figure 3c

8/21

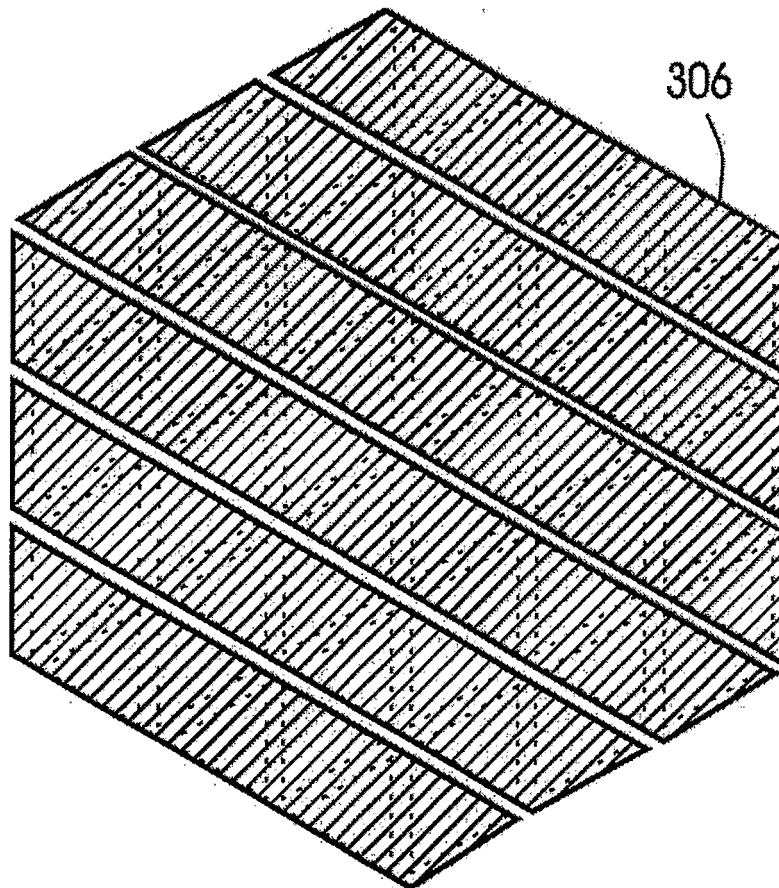


Figure 3d

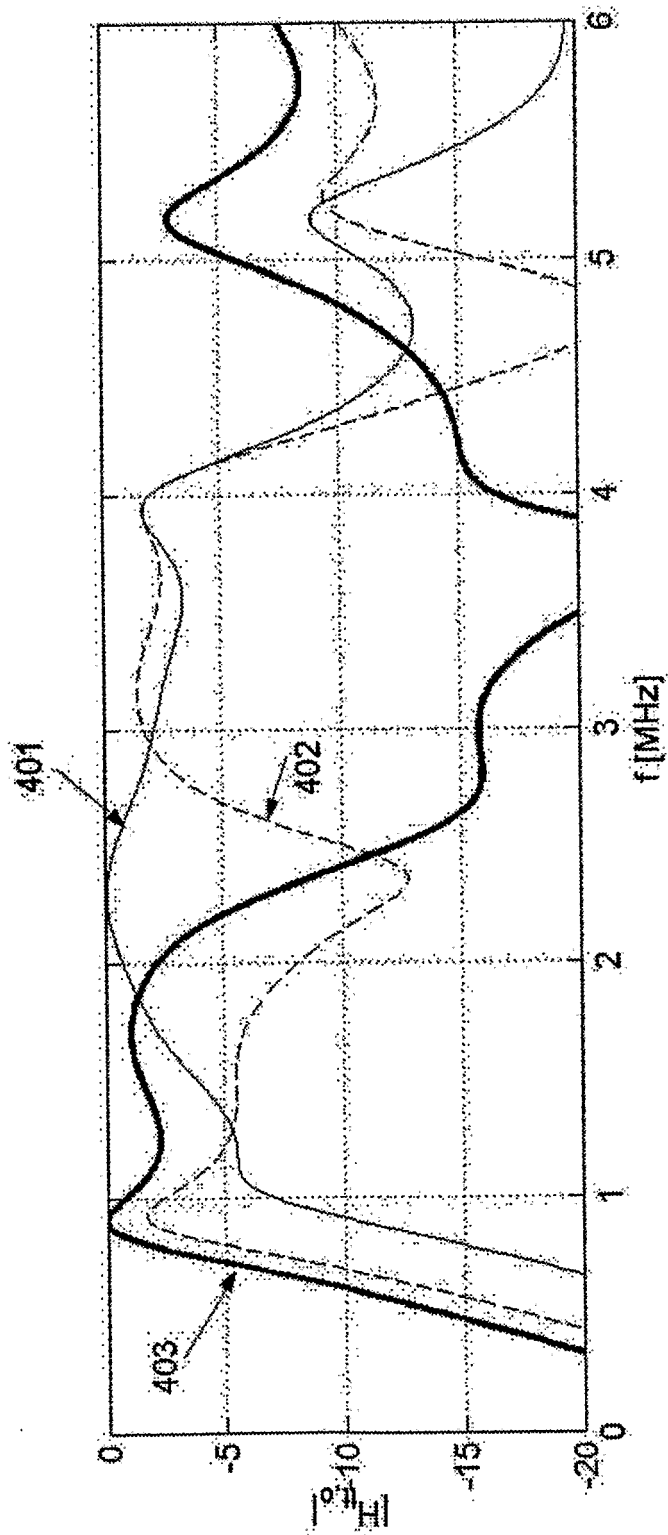


Figure 4

10/21

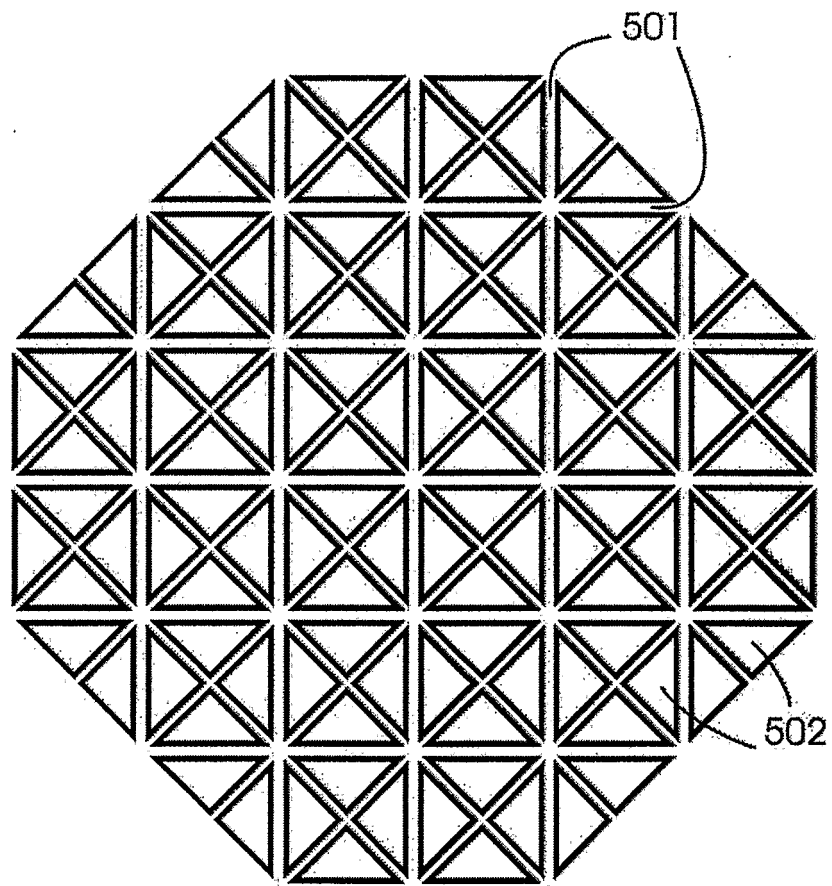


Figure 5a

11/21

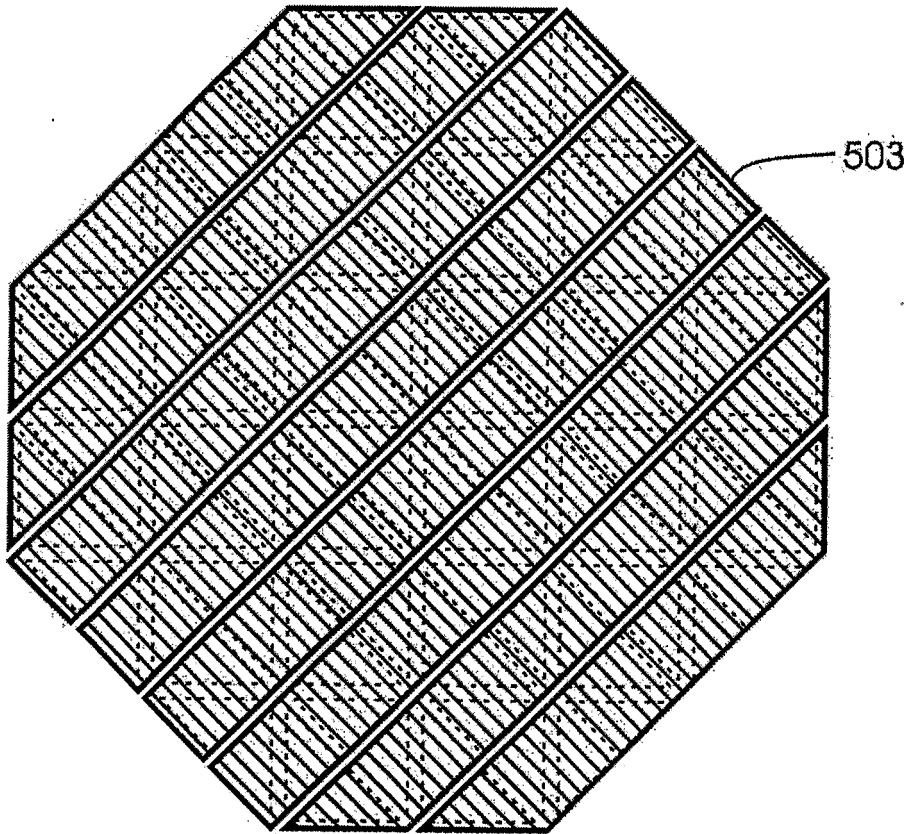


Figure 5b

12/21

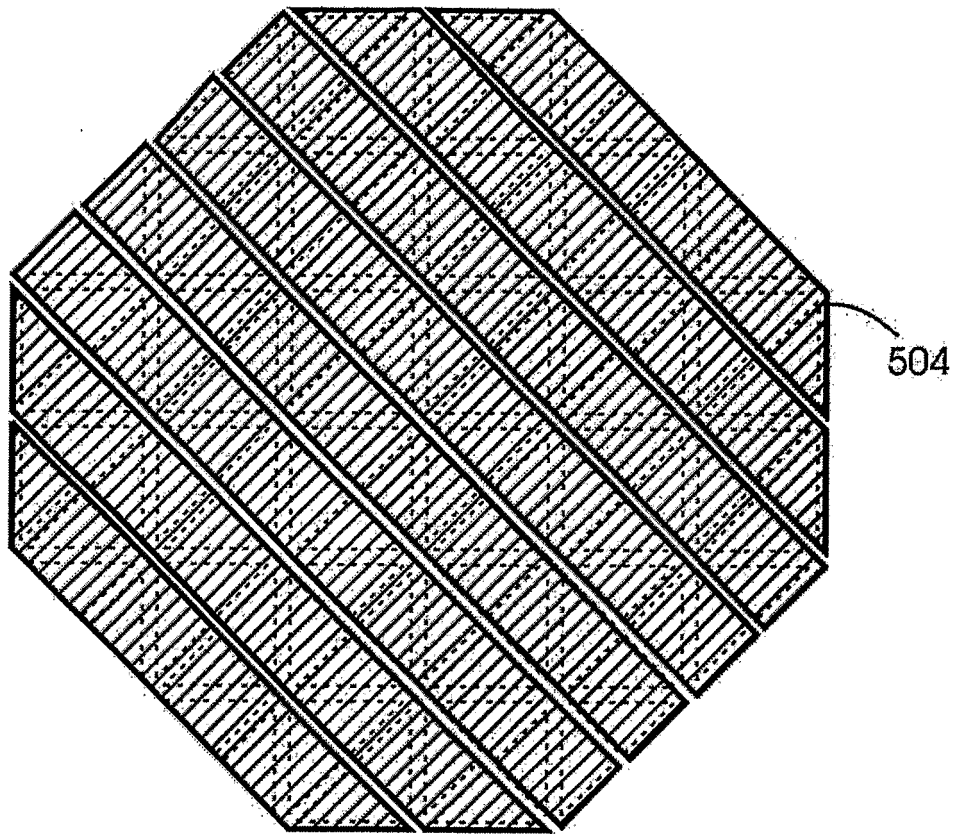


Figure 5c

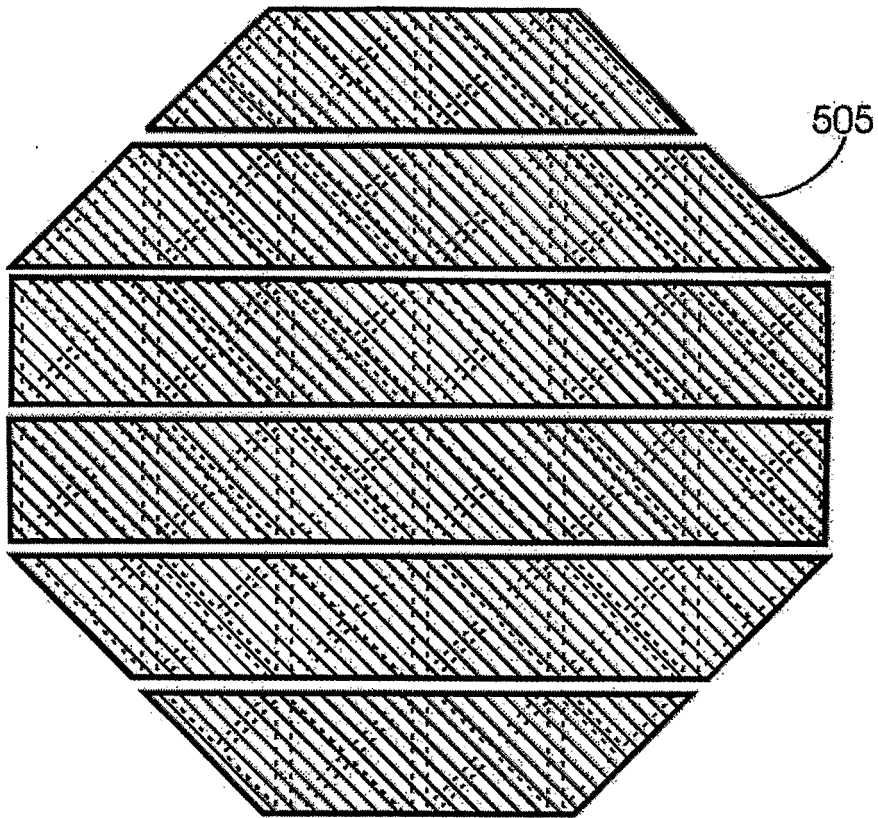


Figure 5d

14/21

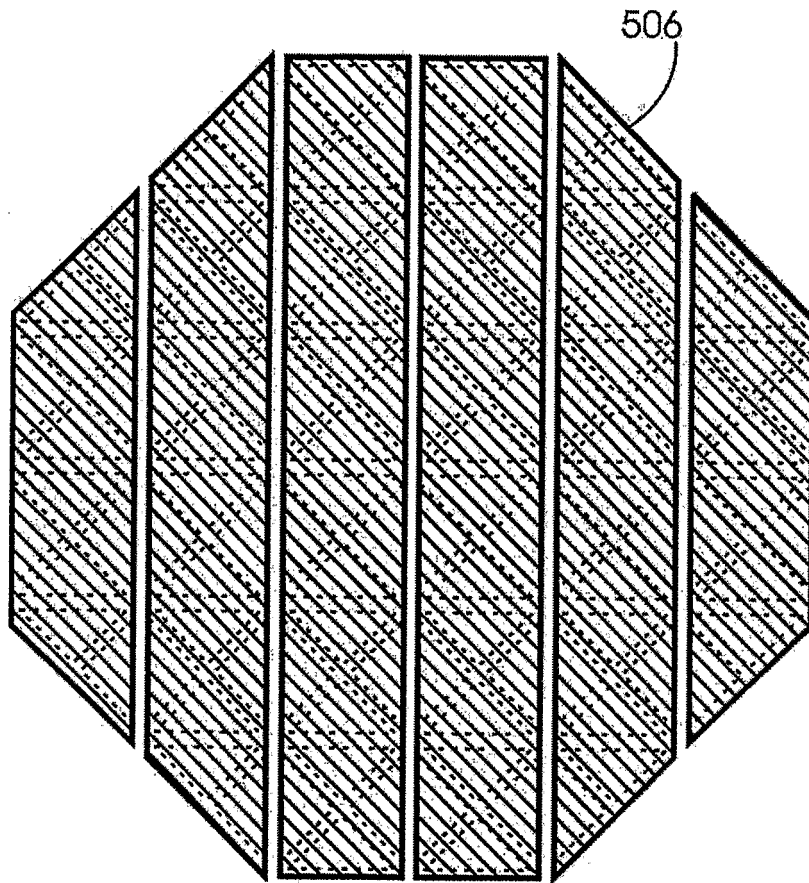


Figure 5e

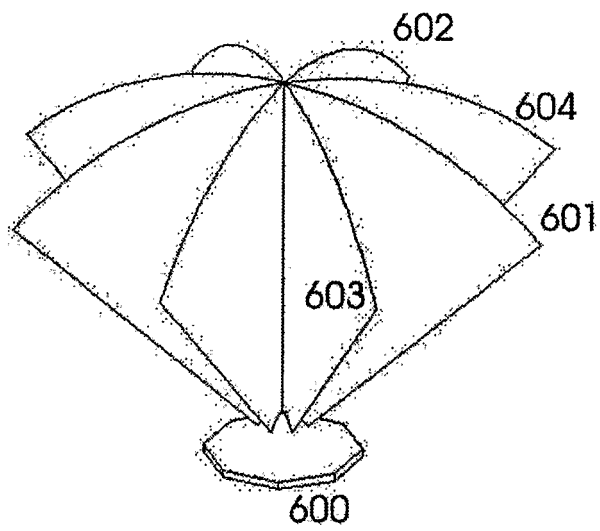


Figure 6

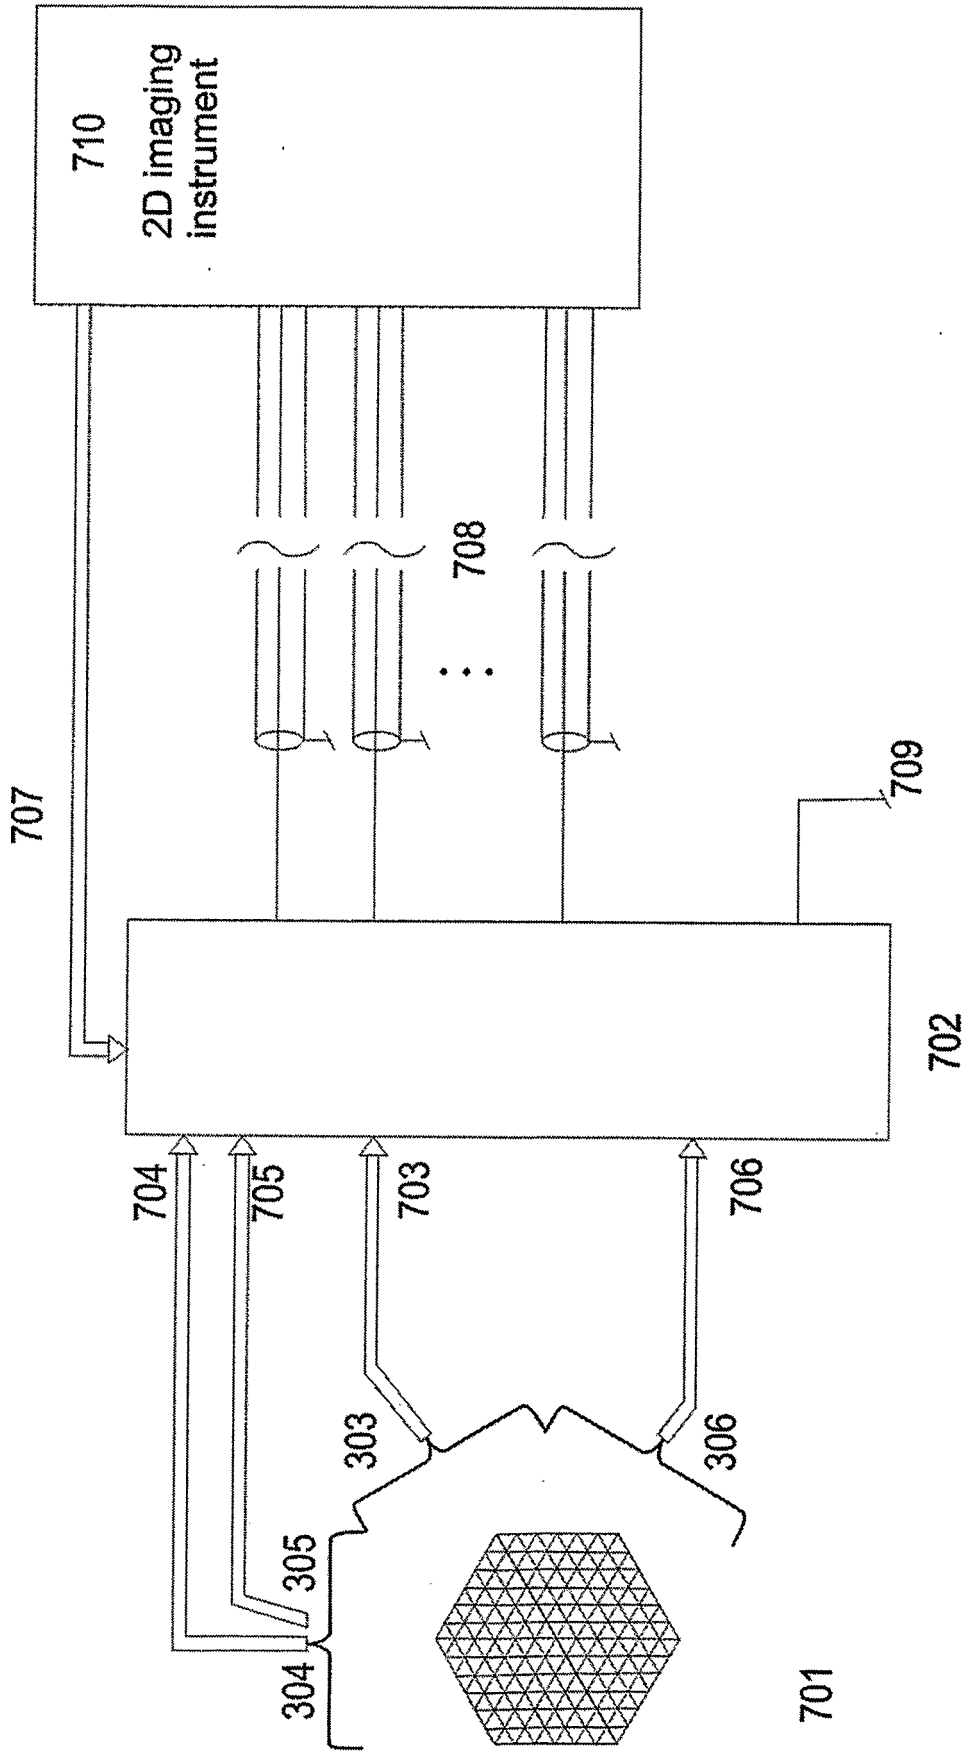


Figure 7

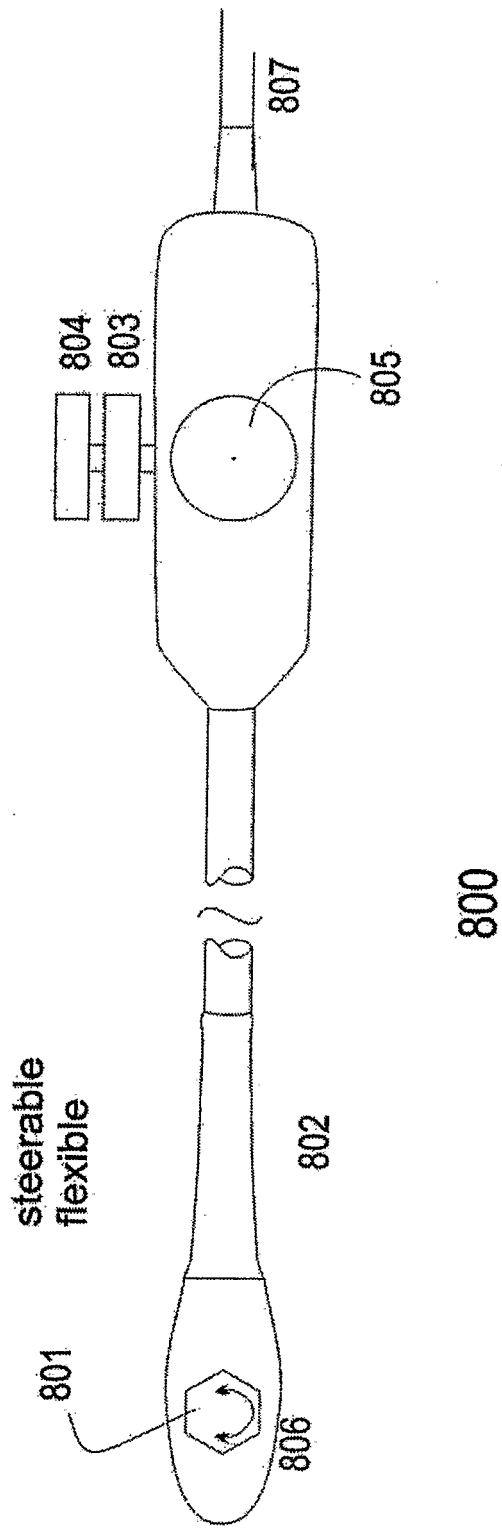


Figure 8

18/21

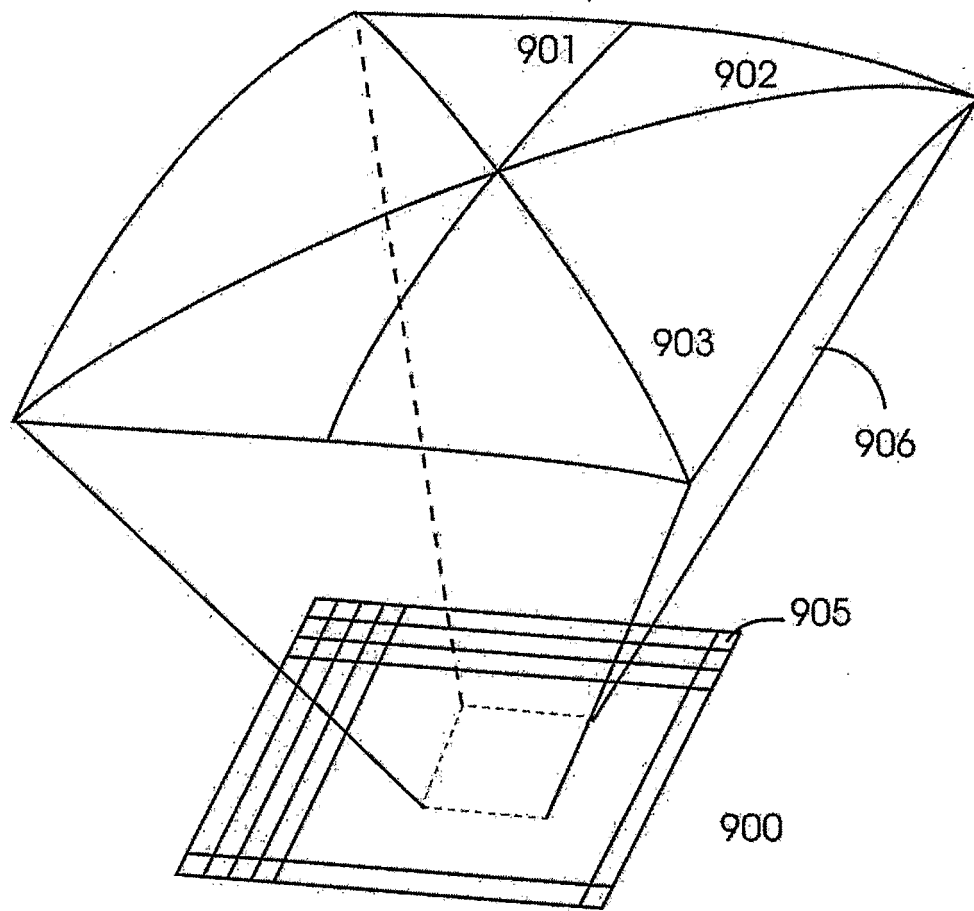


Figure 9

19/21

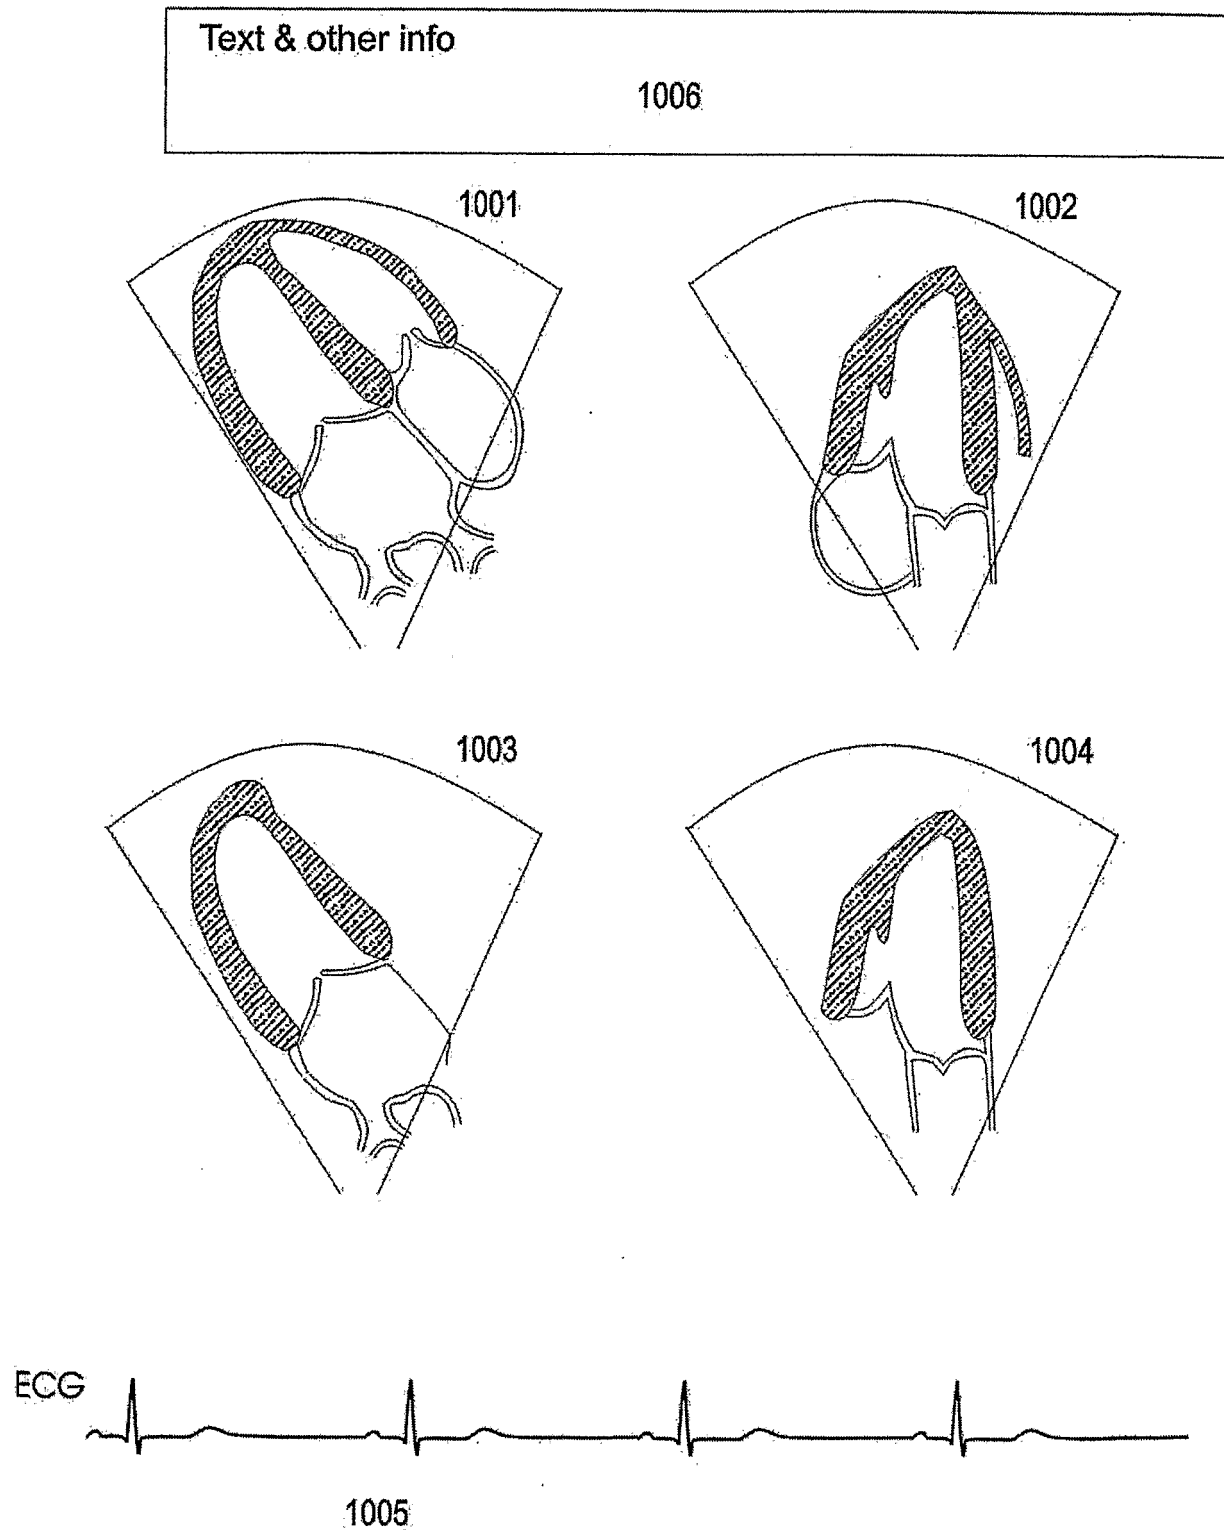


Figure 10a

20/21

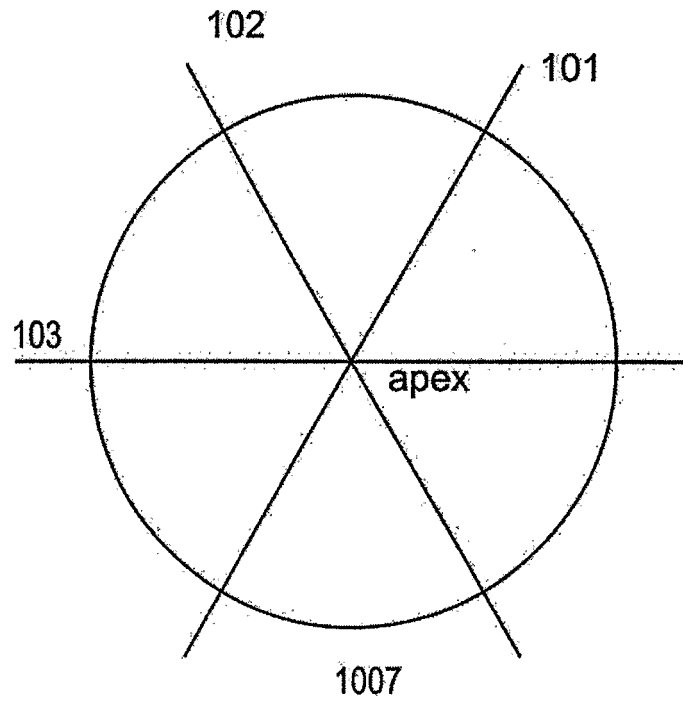


Figure 10b

21/21

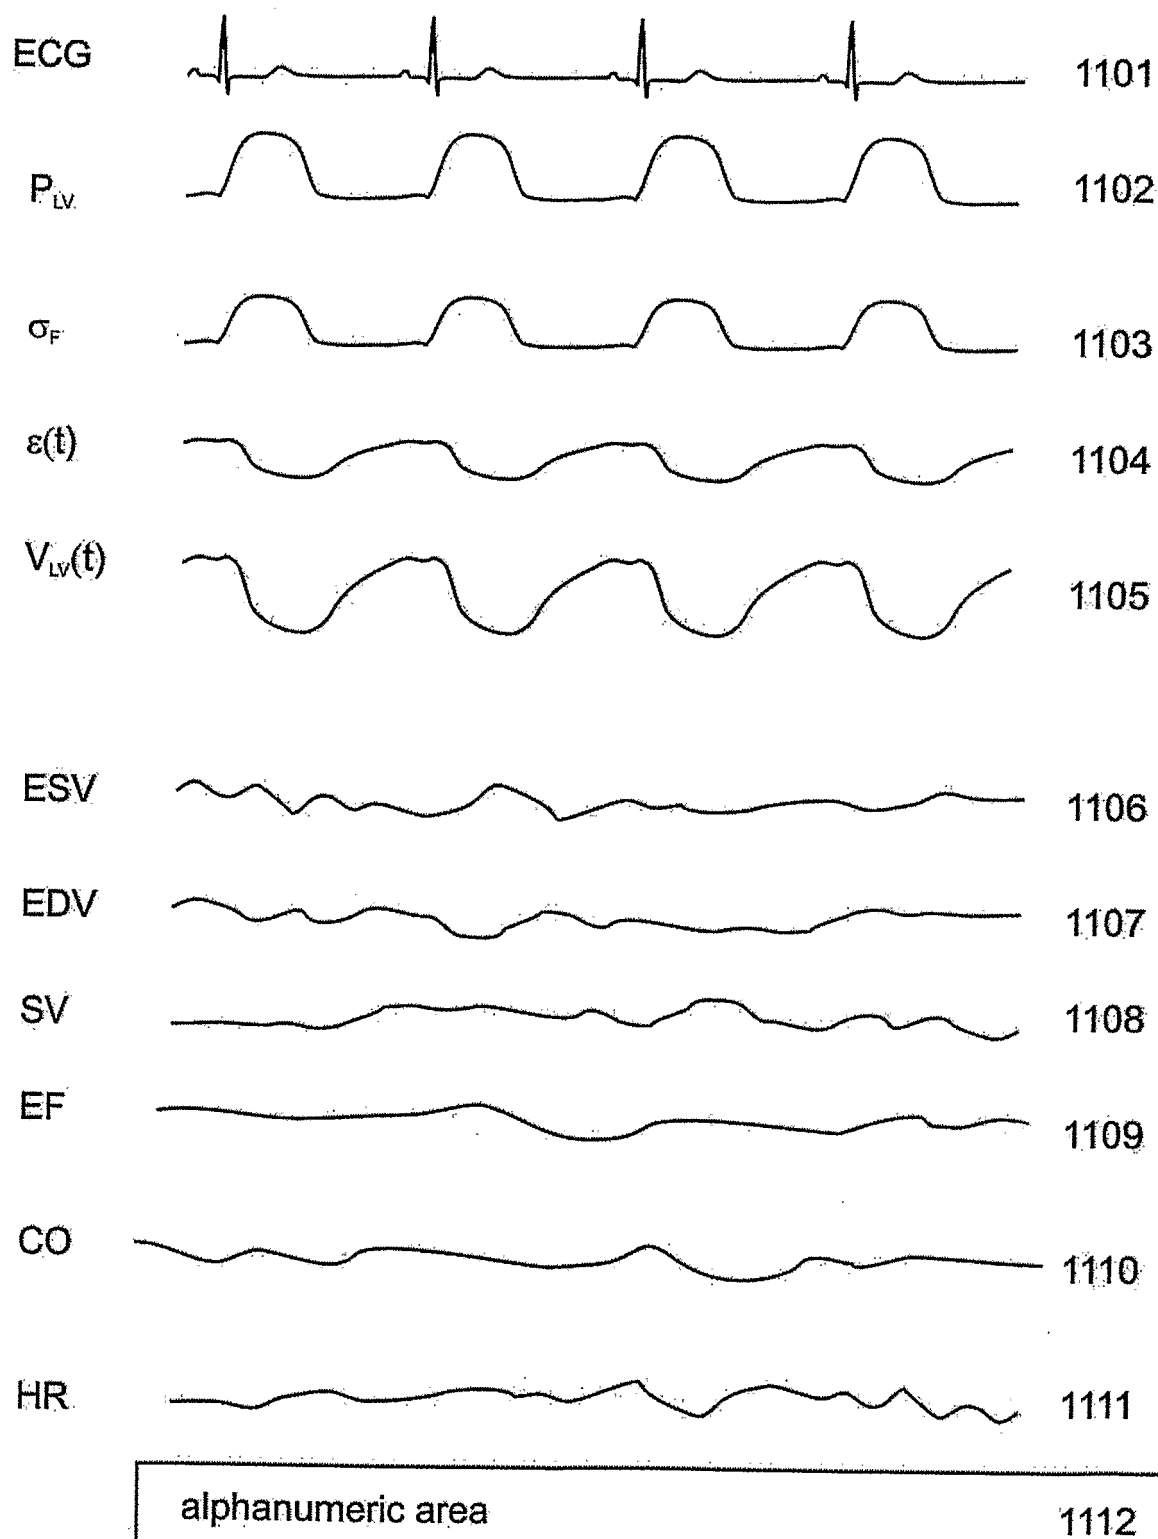


Figure 11

INTERNATIONAL SEARCH REPORT

International application No.

PCT/NO 03/00089

A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61B 8/08, A61B 8/12, G01N 29/00, G01S 15/00
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61B, A61N, G01N, G01S

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

WPI DATA, INSPEC, MEDLINE, BIOSIS

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 0754957 A2 (ALOKA CO.LTD.), 22 January 1997 (22.01.97), figure 1, abstract --	1-22
A	US 4817616 A (ALBERT GOLDSTEIN), 4 April 1989 (04.04.89), figure 1, abstract --	1-22
A	US 5724976 A (YOSHITAKA MINE ET AL), 10 March 1998 (10.03.98), figure 1, abstract --	1-22
A	US 5295486 A (HELMUT WOLLSCHLÄGER ET AL), 22 March 1994 (22.03.94), figure 2, abstract -- -----	1-22

☐ Further documents are listed in the continuation of Box C.

☒ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance
"E" earlier application or patent but published on or after the international filing date
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
"O" document referring to an oral disclosure, use, exhibition or other means
"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

19 May 2003

Date of mailing of the international search report

21 -05- 2003

Name and mailing address of the ISA/
Swedish Patent Office
Box 5055, S-102 42 STOCKHOLM
Facsimile No. +46 8 666 02 86

Authorized officer

Patrik Widerdal/Els
Telephone No. +46 8 782 25 00

INTERNATIONAL SEARCH REPORT

Information on patent family members

29/04/03

International application No.

PCT/NO 03/00089

Patent document cited in search report				Publication date		Patent family member(s)		Publication date	
EP	0754957	A2	22/01/97	CA	2181326	A		18/01/97	
				DE	69612148	D,T		19/07/01	
				JP	2883584	B		19/04/99	
				JP	10033538	A		10/02/98	
				US	5706816	A		13/01/98	

US	4817616	A	04/04/89	NONE					

US	5724976	A	10/03/98	DE	19548988	A,C		11/07/96	
				JP	8187245	A		23/07/96	
				JP	8182680	A		16/07/96	

US	5295486	A	22/03/94	AT	102807	T		15/04/94	
				DE	3914619	A		08/11/90	
				DE	58907254	D		00/00/00	
				EP	0470954	A,B		19/02/92	
				JP	2842911	B		06/01/99	
				JP	7500506	T		19/01/95	
				WO	9013259	A		15/11/90	
				DE	8900550	U		09/03/89	

专利名称(译)	物体的多个扫描平面超声成像		
公开(公告)号	EP1489972A1	公开(公告)日	2004-12-29
申请号	EP2003708748	申请日	2003-03-13
[标]申请(专利权)人(译)	ANGELSEN BJORN第] JOHANSEN TONNI F		
申请(专利权)人(译)	ANGELSEN , BJORN A. J. JOHANSEN , TONNI F.		
当前申请(专利权)人(译)	ANGELSEN , BJORN A. J. JOHANSEN , TONNI F.		
[标]发明人	ANGELSEN BJORN A J JOHANSEN TONNI F		
发明人	ANGELSEN, BJORN A. J. JOHANSEN, TONNI F.		
IPC分类号	A61B8/08 A61B8/06 G01S7/52 G01S15/89 H01L41/08 H01L41/09 H04R17/00 A61B8/12 G01N29/00 G01S15/00		
CPC分类号	A61B8/145 A61B8/06 A61B8/13 G01S7/52074 G01S15/8925 G01S15/8927		
代理机构(译)	HOWE , 史蒂芬		
优先权	60/364747 2002-03-15 US		
其他公开文献	EP1489972B1 EP1489972B2		
外部链接	Espacenet		

摘要(译)

给出了围绕公共轴旋转的至少三个二维扫描平面中的对象的实时超声成像方法，以及允许这种成像的超声换能器阵列的设计。该方法还被引入到心脏功能的监测情况中，其中结合其他测量结果例如LV压力，计算诸如射血分数和肌肉纤维应力的生理参数。