(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau

(43) International Publication Date
28 December 2006 (28.12.2006)

PCT

(10) International Publication Number
WO 2006/136988 A2

(54) Title: METHOD AND APPARATUS FOR 3D ULTRASOUND IMAGING USING A STATIONARY BEAM TO ESTIMATE A PARAMETER
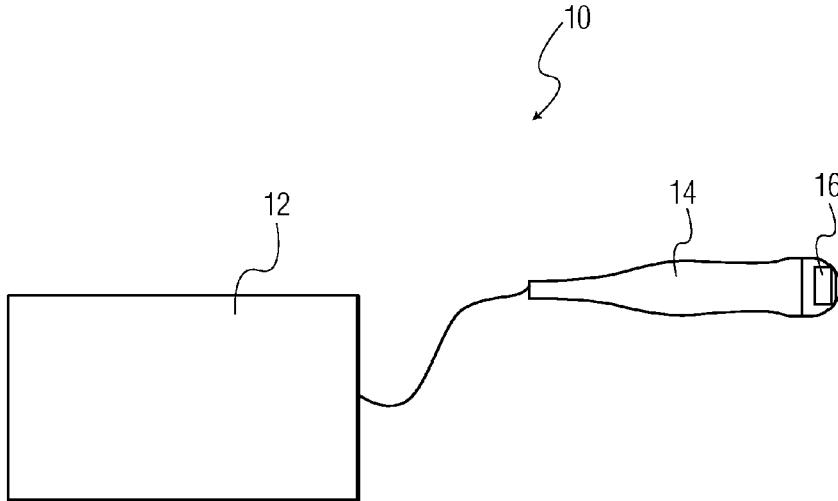
(57) Abstract: A method of three-dimensional (3D) ultrasound imaging comprises acquiring ultrasound data representative of an imaging volume as a function of time, from which can be obtained a plurality of two-dimensional images, and acquiring data from a stationary ultrasound beam concurrently with the acquiring of the ultrasound data representative of the imaging volume. The stationary ultrasound beam data is analyzed to derive a parameter from the stationary ultrasound beam data. The method further includes rearranging a plurality of 2D ultrasound images obtained from the acquired ultrasound data for 3D processing as a function of the derived parameter. In one embodiment, acquiring data from the stationary ultrasound beam comprises one or more of an M-mode acquisition, a Doppler mode acquisition, or an acquisition tailored to a specific ultrasound imaging application.

METHOD AND APPARATUS FOR 3D ULTRASOUND IMAGING
USING A STATIONARY BEAM TO ESTIMATE A PARAMETER

The present embodiments relate generally to medical ultrasound systems and more particularly, to a method and apparatus for 3D ultrasound imaging, for example, ultrasonic 3D fetal heart imaging.

In known methods for fetal heart imaging, an electrocardiogram (ECG) is not available. As a result, an ultrasound system uses spatial-temporal image correlation (STIC) to derive the cardiac phase from a spectral analysis of two-dimensional (2D) images while an imaging plane is being swept across an imaging volume. Using the cardiac phase derived from STIC, the ultrasound system rearranges the 2D images for three-dimensional (3D) processing. However, the accuracy of the STIC analysis varies from one imaging plane to another, especially if the heart rate does not remain steady.

With prior known methods, Fetal STIC imaging includes constructing 3D views of the fetal heart from images acquired over many heart beats. In addition, the current data processing techniques for Fetal STIC imaging require that the heart rate remain steady. However, odd beats or heart rate changes can degrade the 3D views by causing information from different cardiac phases to be intermingled in views that should represent single cardiac phases.

Accordingly, an improved method and ultrasound system for overcoming the problems in the art is desired.

According to an embodiment of the present disclosure, a method of three-dimensional (3D) ultrasound imaging comprises acquiring ultrasound data representative of an imaging volume as a function of time, from which can be obtained a plurality of two-dimensional images, and acquiring data from a stationary ultrasound beam concurrently with the acquiring of the ultrasound data representative of the imaging volume. The stationary ultrasound beam data is analyzed to derive a parameter from the stationary ultrasound beam data. The method further includes rearranging a plurality of 2D ultrasound images obtained from the acquired ultrasound data for 3D processing as a function of the derived parameter. In one embodiment, acquiring data from the stationary ultrasound beam comprises one or more of an M-mode acquisition, a Doppler mode acquisition, or an acquisition tailored to a specific ultrasound imaging application. The method can also be

implemented by an ultrasound imaging system, as well as in the form of a computer program product.

Figure 1 is a partial block diagram view of an ultrasound system according to an embodiment of the present disclosure;

Figure 2 is a simplified schematic diagram view illustrating 3D ultrasound imaging of a target volume with use of the ultrasound imaging system and method according to an embodiment of the present disclosure; and

Figure 3 is a flow diagram view illustrating a method of 3D ultrasound imaging according to another embodiment of the present disclosure.

In the figures, like reference numerals refer to like elements. In addition, it is to be noted that the figures may not be drawn to scale.

As discussed herein above, prior known methods of Fetal STIC imaging have involved constructing 3D views of the fetal heart from images acquired over many heart beats. In addition, the data processing techniques for the prior Fetal STIC imaging methods required that the heart rate remain steady, however, odd beats or heart rate changes degrade the 3D views by causing information from different cardiac phases to be intermingled in views that should represent single cardiac phases. In contrast, according to one embodiment of 3D ultrasound imaging of the present disclosure, the method includes (i) monitoring the heart to determine the actual cardiac phase of each 2D image and (ii) using the determined cardiac phase information to avoid mixing different phases within a single 3D view. Monitoring of the heart is accomplished by using ultrasound, and more particularly, using a stationary ultrasound beam and wherein the transducer remains stationary. Accordingly, Doppler mode or M-mode acquisition can be used to monitor a chosen anatomical location on a fine time scale.

It is further noted that use of Doppler mode or M-mode acquisition is not possible with prior Fetal STIC imaging methods which use mechanical transducer motion to acquire the 3D volume for Fetal STIC. In other words, moving the transducer makes it impossible to hold a Doppler or M-mode line on the chosen anatomical location. The methods according to the embodiments of the present disclosure include a realization that new transducers that scan 3D volumes without mechanical motion (for example, 2D array or matrix transducers) allow for overcoming this limitation. That is, a transducer that scans 3D volumes without mechanical motion can be configured to transmit lines throughout a

2

3D volume. In addition, the transducer capable of 3D scanning without mechanical movement, hereinafter referred to as a transducer with 3D electronic steering, can further be configured to interleave a stationary monitor pulse with pulses used to acquire a 3D volume, for example, in connection with fetal STIC.

In order to scan a 3D volume using a transducer that cannot electronically steer throughout the volume, hereinafter referred to as a transducer without 3D electronic steering, the transducer must be mechanically moved. For example, a 3D volume can be scanned using a 1D phased array transducer by moving the transducer so that its 2D scan plane moves across the volume being scanned. As indicated herein above, moving the transducer without 3D electronic steering in this way makes it impossible to maintain a stationary monitor beam. The situation is much the same with so-called 1.5D transducers, which have some ability to control elevation focusing or elevation steering or both. In contrast, a transducer with 3D electronic steering remains stationary and uses electronic steering to sweep through a 3D volume, whereas a transducer without 3D electronic steering must move to sweep through the 3D volume.

A review of 2D ultrasound imaging, M-mode, and Doppler data acquisition is provided below. It is noted that the numbers included herein represent but a single example of how this may be done, and other numbers may be used. For simple 2D ultrasound imaging, image data can be acquired from 50 transmit lines spanning a 90 degree wedge. The frame rate can be 50 Hz, or 20 ms per frame. Time between adjacent lines is 0.4 ms. In addition, time between repeated views of the same line is the frame time, 20 ms.

With respect to M-mode acquisition, M-mode is used to see motion on finer time scales. For example, a system operator selects one line from a 2D frame. The selected line is thereafter acquired 5 times evenly spaced (in time) among the 50 lines of the 2D frame. The scanner will acquire ten 2D lines and then re-acquire the M-mode line, so that the M-mode view is updated every 4 ms. Accordingly, the M-mode acquisition enables seeing motion on smaller time scales than with 2D imaging alone, in which the image updates only once every 20 ms. An M-mode trace is composed by displaying the acquired M-mode lines side-by-side. The M-mode trace includes a scrolling trace, similar to a strip-chart recorder. In addition, with respect to the M-mode trace, the vertical axis represents depth and the horizontal axis represents time.

Duplex Doppler uses a similar acquisition strategy to that of M-mode acquisition; however, a duplex Doppler line would typically be acquired after every 2D image line. In addition, for Doppler acquisition, the acquired data is used to determine blood flow rather than being used to form a spatial image. The vertical axis of a Doppler acquisition trace represents velocity (of the moving blood) and the horizontal axis represents time. In addition, it is noted that a cardiac cycle is evident in both M-mode and Doppler traces.

Furthermore, while using duplex Doppler drops the 2D frame rate by about half, it would almost certainly be unacceptable for use with known fetal STIC imaging methods. However, with the method of 3D imaging according to the embodiments of the present disclosure, duplex Doppler provides for a fetal STIC improvement, by employing acquisition timing similar to M-mode.

According to one embodiment of the present disclosure, a method of 3D ultrasound imaging includes using a transducer with 3D electronic steering (for example, a 2D array transducer) without additional steering via mechanical movement, wherein derivation of cardiac phase is improved by analyzing a stationary ultrasound beam instead of a collection of imaging planes (comprising a 3D volume). The same stationary ultrasound beam can be used for all image planes, for example, during a particular fetal heart imaging procedure, so that consistent results are obtained for all imaging planes. In other words, the embodiments of the present disclosure correctly determine the cardiac phase of each image even if the heart rate changes during the cardiac acquisition. According to one embodiment, the stationary beam can include an M-mode acquisition, a Doppler acquisition, or an acquisition tailored specifically to fit the ultrasound imaging requirements of a particular imaging procedure. The monitor beam may be acquired less often than is typical for either M-mode or Doppler, perhaps only once per 2D image frame, and perhaps even less often.

According to one embodiment of the present disclosure, an ultrasound system comprises a transducer with 3D electronic steering configured to interleave a sweep of 2D data acquisitions with a stationary acquisition, wherein the stationary acquisition comprises an M-mode acquisition or a Doppler acquisition. As noted herein, transducers that are mechanically swept to perform 3D acquisitions, either by motorization or by other manipulation, are not able to interleave a sweep of 2D data acquisitions with a stationary acquisition.

The embodiments of the present disclosure can be implemented by deriving the cardiac phase from a STIC analysis of the M-mode and/or Doppler data streams obtained with the use of the stationary ultrasound beam. Alternatively, the STIC algorithms may be modified for better performance with M-mode and/or Doppler data streams. Furthermore, an additional new approach to the analysis can be implemented for better performance with M-mode and/or Doppler data streams. Moreover, a novel form of acquisition tailored specifically to fit the 3D ultrasound imaging application may be used either in place of or in addition to M-mode and/or Doppler data streams. Furthermore, as discussed herein, the embodiments of the present disclosure can be implemented in ultrasound systems that support both 3D fetal heart imaging and matrix (2D array) ultrasound transducers.

According to another embodiment, a method of three-dimensional (3D) ultrasound imaging comprises acquiring ultrasound data representative of an imaging volume as a function of time, from which can be obtained a plurality of two dimensional (2D) ultrasound images. The method further comprises acquiring data from a stationary ultrasound beam concurrently with the acquiring of the ultrasound data representative of the imaging volume. The stationary ultrasound beam data is analyzed to derive a parameter from the stationary ultrasound beam data. In addition, the acquired ultrasound data is rearranged for 3D processing as a function of the derived parameter. From the rearranged ultrasound data one or more 2D images ordered according to the derived parameter may be obtained. Likewise, from the rearranged ultrasound data one or more 3D surface rendered images ordered according to the derived parameter may be obtained. Acquiring of the ultrasound data can further comprise one or more of (i) a consecutive acquisition order across the imaging volume, (ii) a non-consecutive acquisition order across the imaging volume, or (iii) a prescribed acquisition order across the imaging volume. The prescribed acquisition order can include any arbitrary order selected according to the requirements of a particular acquisition.

Referring now to the drawings, Figure 1 is a block diagram view of a three-dimensional (3D) ultrasound imaging system 10 according to an embodiment of the present disclosure. The 3D ultrasound imaging system 10 includes a control or base unit 12 configured for use with an ultrasound transducer probe 14, further for carrying out the ultrasound imaging methods as discussed herein according to the embodiments of the present disclosure. The probe 14 contains an ultrasound transducer 16. In one embodiment,

the control unit 12 is configured for (i) controlling the ultrasound transducer 16 and (ii) performing 3D ultrasound imaging according to the 3D ultrasound imaging methods of the present disclosure.

In one embodiment, ultrasound transducer 16 comprises a matrix transducer, also
5   referred to as a two-dimensional array transducer. Furthermore, base unit 12 includes suitable control electronics for performing 3D ultrasound imaging as discussed herein. For example, in one embodiment, base unit 12 can comprise a computer as discussed further herein. Ultrasound transducer probe 14 couples to base unit 12 via a suitable connection, for example, an electronic cable, a wireless connection, or other suitable means.

10   Figure 2 is a simplified schematic diagram view illustrating 3D ultrasound imaging of a target volume with use of the ultrasound imaging system 10 according to an embodiment of the present disclosure. In particular, ultrasound transducer 16 produces a sweep 20 of ultrasound beams of a 2D imaging plane directed into an imaging volume (not shown) in response to an activation signal from base unit 12. For example, the sweep 20
15   can comprise a sweep from an initial 2D imaging plane 22 to a final 2D imaging plane 24. The ultrasound energy can be adjusted as needed, for example by a repositioning of the ultrasound transducer 16 (via repositioning of probe 14) with respect to the target location or imaging volume and/or through appropriate activation signals from base unit 12, according to the requirements of a particular 3D ultrasound imaging application. In
20   addition, the imaging volume is disposed in a region of interest within a subject to be imaged according to the methods of the present disclosure.

According to one embodiment of the present disclosure, the method of three-dimensional (3D) ultrasound imaging comprises acquiring a plurality of two-dimensional (2D) ultrasound images 28 as a 2D imaging plane is swept across an imaging volume. For
25   example, the 2D ultrasound images 28 include images from an initial image 30 to a final image 32, corresponding to the sweep 20 from the initial 2D imaging plane 22 to the final imaging plane 24. Concurrently with the acquiring of the plurality of 2D ultrasound images, data from a stationary ultrasound beam 26 is acquired. The stationary ultrasound beam data is analyzed to derive a parameter 34 from the stationary ultrasound beam data.
30   Furthermore, the 2D ultrasound images are rearranged into new groups of images, as indicated by reference numeral 36 in Figure 2, for 3D processing as a function of the derived parameter. Within the new groups there are a number of images. As shown in

Figure 2, for illustration only, the new groups include eleven 2D images. The base unit 12 of 3D ultrasound system is configured for arranging the images spatially within the new groups because the images have all occurred at different positions in space with known positional co-ordinates. In the example of Figure 2, two volumes 38 and 49 are shown. One volume 38 at systole and another volume 40 at diastole. In addition, there can exist additional volumes between these two volumes (38,40) and their corresponding locations, as illustrated by reference numeral 42.

In one embodiment, the derived parameter comprises a cardiac phase. In other words, the imaging volume contains a cardiac source, the cardiac source having a number of cardiac phases. For example, the cardiac source can comprise a fetal heart.

According to another embodiment, acquiring the plurality of 2D ultrasound images comprises using a matrix transducer. The matrix transducer can be configured (i) for electronically steering ultrasound beams to acquire 2D ultrasound images and (ii) for sweeping the 2D imaging plane across the imaging volume. In addition, acquiring the stationary ultrasound beam data can also comprise using the matrix transducer, wherein the matrix transducer is further configured for (iii) interleaving the acquiring of the 2D ultrasound images with stationary ultrasound beam data acquisition.

In one embodiment, the transducer with 3D electronic steering 16 is configured for steering the stationary ultrasound beam 26 to occur within the imaging volume at a position for obtaining an optimal signal. That is, the stationary ultrasound beam 26 can be steered, and a positioning of the stationary ultrasound beam can be adjusted as may be necessary, to an optimal or other suitable location within the imaging volume to improve derivation of the parameter for the acquiring of the ultrasound data representative of the imaging volume and the obtaining of the plurality of 2D ultrasound images 28. For example, a positioning of the stationary ultrasound beam may be adjusted during an imaging volume acquisition sequence to provide a desired tracking of a cardiac phase. Furthermore, acquiring of the stationary ultrasound beam data can comprise, for example, an M-mode acquisition or a Doppler mode acquisition. In another embodiment, acquiring the stationary ultrasound beam data can comprise an acquisition tailored to a specific ultrasound imaging application.

In another embodiment, acquiring the stationary ultrasound beam data comprises acquiring the stationary ultrasound beam data concurrently with the acquiring of each of

the plurality of 2D ultrasound images 28. Accordingly, analyzing the stationary ultrasound beam data includes analyzing data from each respective stationary ultrasound beam data acquisition to derive the parameter 34 for a corresponding 2D ultrasound image. In one embodiment, analyzing further includes performing a spatial-temporal image correlation

5   (STIC) analysis of the stationary ultrasound beam data, with appropriate adaptation of the STIC methods to the acquired data. The stationary ultrasound beam data can comprise, for example, one or more of an M-mode data stream, a Doppler mode data stream, or other data stream. In addition, a same stationary ultrasound beam 26 can be used concurrently for all 2D imaging planes to enable a consistent derivation of the parameter for the plurality of

10 2D ultrasound images.

In another embodiment, a method of three-dimensional (3D) ultrasound imaging comprises acquiring a plurality of two-dimensional (2D) ultrasound images as a 2D imaging plane is swept across an imaging volume that contains a cardiac source, the cardiac source having a number of cardiac phases, and wherein acquiring the plurality of

15 2D ultrasound images comprises using a transducer with 3D electronic steering configured (i) for electronically steering ultrasound beams to acquire 2D ultrasound images and (ii) for sweeping the 2D imaging plane across the imaging volume. The method further comprises acquiring data from a stationary ultrasound beam concurrently with the acquiring of the plurality of 2D ultrasound images, wherein acquiring the stationary ultrasound beam data

20 further comprises using the matrix transducer, wherein the transducer with 3D electronic steering is further configured for (iii) interleaving the acquiring of the 2D ultrasound images with stationary ultrasound beam data acquisition. In addition, the stationary ultrasound beam data is analyzed to derive a cardiac phase from the stationary ultrasound beam data. Furthermore, the 2D ultrasound images are rearranged for 3D processing as a

25 function of the derived cardiac phase.

In the embodiment of the preceding paragraph, the acquiring of the stationary ultrasound beam data can comprise one or more of an M-mode acquisition, a Doppler mode acquisition, or an acquisition tailored to a specific ultrasound imaging application. In addition, in another embodiment, the analyzing includes performing a spatial-temporal

30 image correlation (STIC) analysis of the stationary ultrasound beam data. Still further, in another embodiment a same stationary ultrasound beam is used concurrently for all 2D imaging planes to enable a consistent derivation of the cardiac phase for the plurality of 2D

ultrasound images. Furthermore, the stationary ultrasound beam is selectively positioned for obtaining an optimal signal to improve derivation of the cardiac phase for the plurality of 2D ultrasound images.

Figure 3 is a flow diagram view illustrating a method of 3D ultrasound imaging,
5   generally indicated by reference numeral 50, according to another embodiment of the present disclosure. The method begins with step 52, wherein initial actions are taken by a system operator in setting up the ultrasound imaging equipment in preparation for acquiring a 3D ultrasound image of a desired imaging volume. At step 54, the method includes acquiring a plurality of two-dimensional (2D) ultrasound images as a 2D imaging
10   plane is swept across an imaging volume. At step 56, concurrently with the acquiring of the plurality of 2D ultrasound images, the method includes acquiring data from a stationary ultrasound beam. At step 58, the stationary ultrasound beam data is analyzed to derive a parameter from the stationary ultrasound beam data. In one embodiment, the parameter includes a cardiac phase. At step 60, the method includes rearranging the 2D ultrasound
15   images for 3D processing as a function of the derived parameter. Additional processing, as may be appropriate for a particular 3D ultrasound imaging application, continues and/or occurs with step 62.

In addition to the above, the embodiments of the present disclosure also include computer software or a computer program product. The computer program product
20   includes a computer readable media having a set of instructions executable by a computer for carrying out the methods of 3D ultrasound imaging as described and discussed herein. The computer readable media can include any suitable computer readable media for a given ultrasound imaging system application. Still further, the computer readable media may include a network communication media. Examples of network communication media
25   include, for example, an intranet, the Internet, or an extranet. In one embodiment, control unit 12 can comprise a computer.

Although only a few exemplary embodiments have been described in detail above, those skilled in the art will readily appreciate that many modifications are possible in the exemplary embodiments without materially departing from the novel teachings and
30   advantages of the embodiments of the present disclosure. For example, the embodiments of the present disclosure can be applied to 3D ultrasound imaging such as 3D fetal heart ultrasound imaging. Accordingly, all such modifications are intended to be included within

the scope of the embodiments of the present disclosure as defined in the following claims. In the claims, means-plus-function clauses are intended to cover the structures described herein as performing the recited function and not only structural equivalents, but also equivalent structures.

5   In addition, any reference signs placed in parentheses in one or more claims shall not be construed as limiting the claims. The word "comprising" and "comprises," and the like, does not exclude the presence of elements or steps other than those listed in any claim or the specification as a whole. The singular reference of an element does not exclude the plural references of such elements and vice-versa. One or more of the embodiments may be

10   implemented by means of hardware comprising several distinct elements, and/or by means of a suitably programmed computer. In a device claim enumerating several means, several of these means may be embodied by one and the same item of hardware. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to an advantage.

15

CLAIMS:

1.   A method of three-dimensional (3D) ultrasound imaging comprising:

acquiring ultrasound data representative of an imaging volume as a function of time, from which can be obtained a plurality of two dimensional (2D) ultrasound images;

acquiring data from a stationary ultrasound beam concurrently with the acquiring of the ultrasound data representative of the imaging volume;

analyzing the stationary ultrasound beam data to derive a parameter from the stationary ultrasound beam data; and

rearranging a plurality of 2D ultrasound images obtained from the acquired ultrasound data for 3D processing as a function of the derived parameter.

2.   The method of claim 1, wherein the derived parameter comprises a cardiac phase.

3.   The method of claim 1, wherein the imaging volume contains a cardiac source, the cardiac source having a number of cardiac phases.

4.   The method of claim 3, further wherein the cardiac source comprises a fetal heart.

5.   The method of claim 1, wherein acquiring ultrasound data comprises using a transducer with 3D electronic steering configured (i) for electronically steering ultrasound beams to acquire data representative of a 2D ultrasound image within a 2D imaging plane of the imaging volume and (ii) for sweeping the 2D imaging plane across the imaging volume, and

wherein acquiring the stationary ultrasound beam data further comprises using the transducer with 3D electronic steering, wherein the transducer with 3D electronic steering is further configured for (iii) interleaving the acquiring of the 2D ultrasound image data with the stationary ultrasound beam data acquisition.

6.   The method of claim 5, further wherein acquiring the stationary ultrasound beam data comprises an M-mode or a Doppler mode acquisition.

7.   The method of claim 5, further wherein acquiring the stationary ultrasound beam data comprises an acquisition tailored to a specific ultrasound imaging application.

8.   The method of claim 1, wherein acquiring the stationary ultrasound beam data comprises one or more of an M-mode acquisition, a Doppler mode acquisition, or an acquisition tailored to a specific ultrasound imaging application.

9.   The method of claim 1, wherein acquiring the stationary ultrasound beam data comprises acquiring the stationary ultrasound beam data concurrently with the acquiring of ultrasound data for each of the plurality of 2D ultrasound images, and wherein analyzing the stationary ultrasound beam data comprises analyzing data from each respective stationary ultrasound beam data acquisition to derive the parameter for a corresponding 2D ultrasound image.

10.   The method of claim 9, wherein analyzing further includes performing a spatial-temporal image correlation (STIC) analysis of the stationary ultrasound beam data.

11.   The method of claim 9, further wherein the stationary ultrasound beam data comprises one or more of an M-mode data stream, a Doppler mode data stream, or other data stream.

12.   The method of claim 9, wherein a same stationary ultrasound beam is used concurrently for all 2D imaging planes of the plurality of 2D ultrasound images to enable a consistent derivation of the parameter for the plurality of 2D ultrasound images.

13.   The method of claim 1, further comprising:
        adjusting a positioning of the stationary ultrasound beam for obtaining an optimal signal to improve derivation of the parameter for the plurality of 2D ultrasound images.

14.   The method of claim 1, wherein acquiring the ultrasound data comprises one or more of (i) a consecutive acquisition order across the imaging volume, or (ii) a non-

consecutive acquisition order across the imaging volume, or (iii) a prescribed acquisition order across the imaging volume.

15.   A three-dimensional (3D) ultrasound imaging apparatus comprising:
        a control unit; and
        an ultrasound transducer coupled to the control unit, wherein said control unit is configured for (i) controlling the ultrasound transducer and (ii) performing 3D ultrasound imaging according to the method of claim 1.

16.   A computer program product comprising computer readable media having a set of instructions executable by a computer, wherein the instructions are configured for carrying out three-dimensional (3D) ultrasound imaging according to the method of claim 1.

17.   A method of three-dimensional (3D) ultrasound imaging comprising:
        acquiring a plurality of two-dimensional (2D) ultrasound images as a 2D imaging plane is swept across an imaging volume that contains a cardiac source, the cardiac source having a number of cardiac phases, and wherein acquiring the plurality of 2D ultrasound images comprises using a transducer with 3D electronic steering configured (i) for electronically steering ultrasound beams to acquire 2D ultrasound images and (ii) for sweeping the 2D imaging plane across the imaging volume;
        acquiring data from a stationary ultrasound beam concurrently with the acquiring of the plurality of 2D ultrasound images, wherein acquiring the stationary ultrasound beam data further comprises using the transducer with 3D electronic steering, wherein the transducer with 3D electronic steering is further configured for (iii) interleaving the acquiring of the 2D ultrasound images with stationary ultrasound beam data acquisition;
        analyzing the stationary ultrasound beam data to derive a cardiac phase from the stationary ultrasound beam data; and
        rearranging the 2D ultrasound images for 3D processing as a function of the derived cardiac phase.

18.   The method of claim 17, wherein acquiring the stationary ultrasound beam data comprises one or more of an M-mode acquisition, a Doppler mode acquisition, or an acquisition tailored to a specific ultrasound imaging application.

19.   The method of claim 17, wherein analyzing includes performing a spatial-temporal image correlation (STIC) analysis of the stationary ultrasound beam data.

20.   The method of claim 17, wherein a same stationary ultrasound beam is used concurrently for all 2D imaging planes to enable a consistent derivation of the cardiac phase for the plurality of 2D ultrasound images.

21.   The method of claim 17, further comprising:
        adjusting a positioning of the stationary ultrasound beam for obtaining an optimal signal to improve derivation of the cardiac phase for the plurality of 2D ultrasound images.

22.   The method of claim 1, wherein the acquired ultrasound data is rearranged as a function of the derived parameter.

23.   Method of claim 22, wherein 3D surface images are obtained from the rearranged ultrasound data.

24.   Method of claim 22, wherein one or more 2D images are obtained from the rearranged data.

25.   Method of claim 22, wherein one or more other metrics, descriptors, or renderings are obtained from the rearranged data.
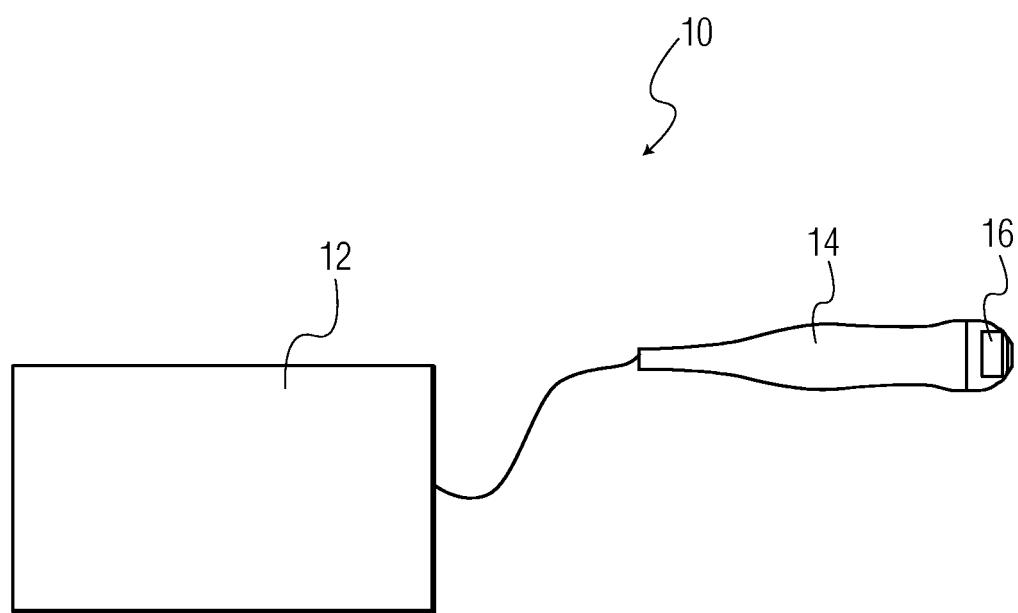
FIG. 1
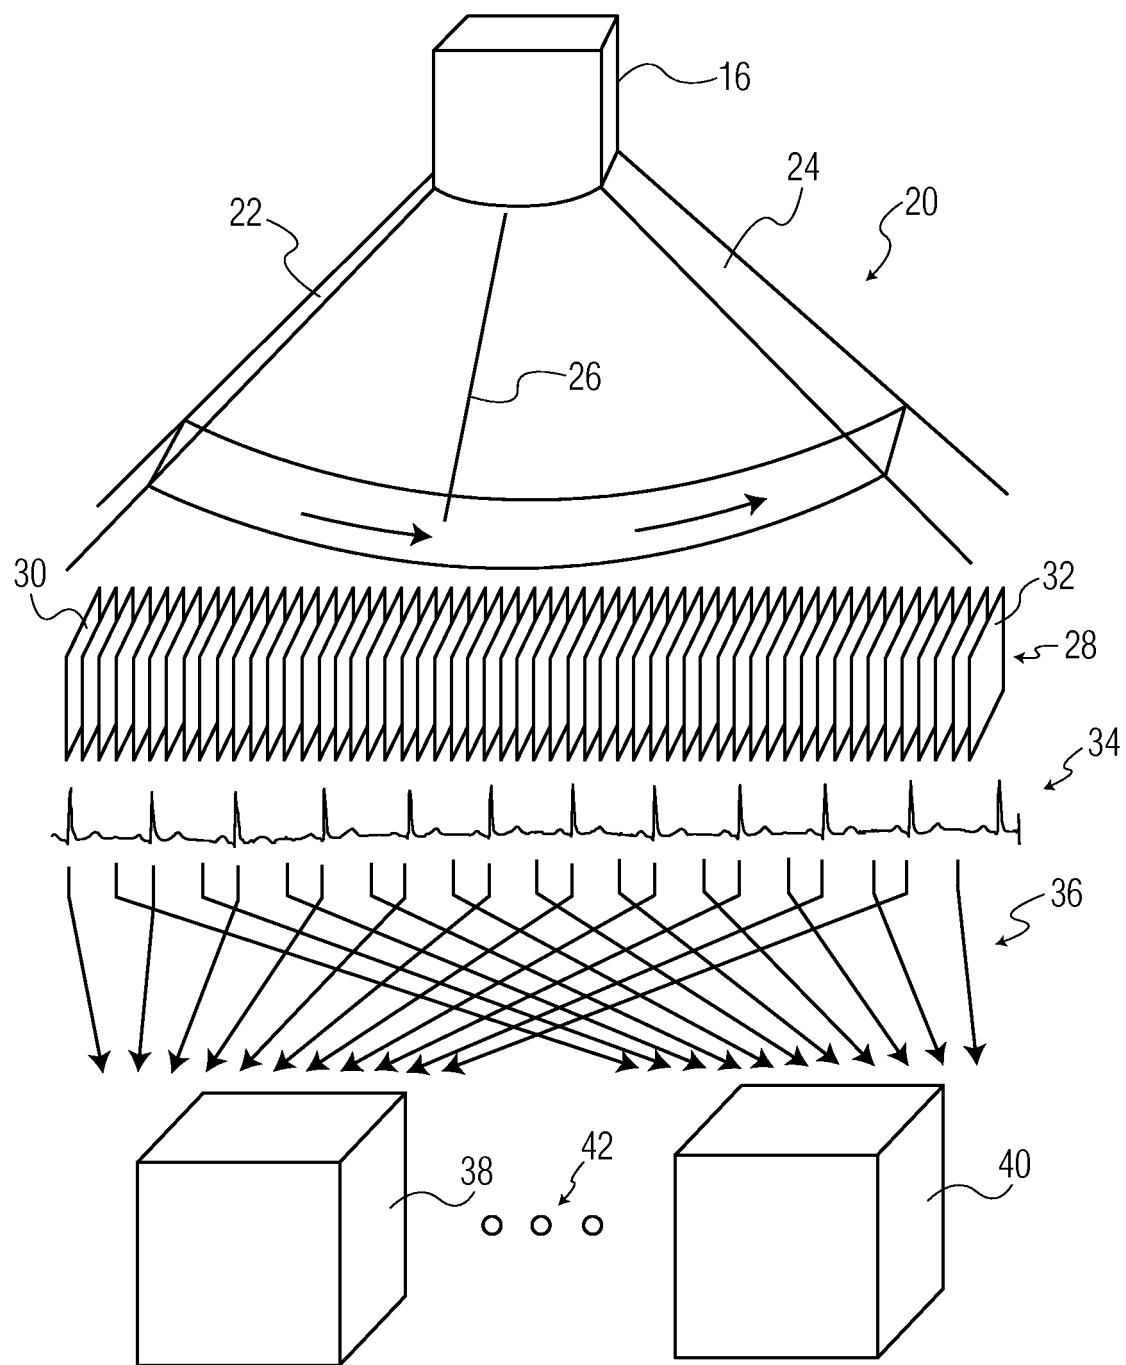
FIG. 2

3/3
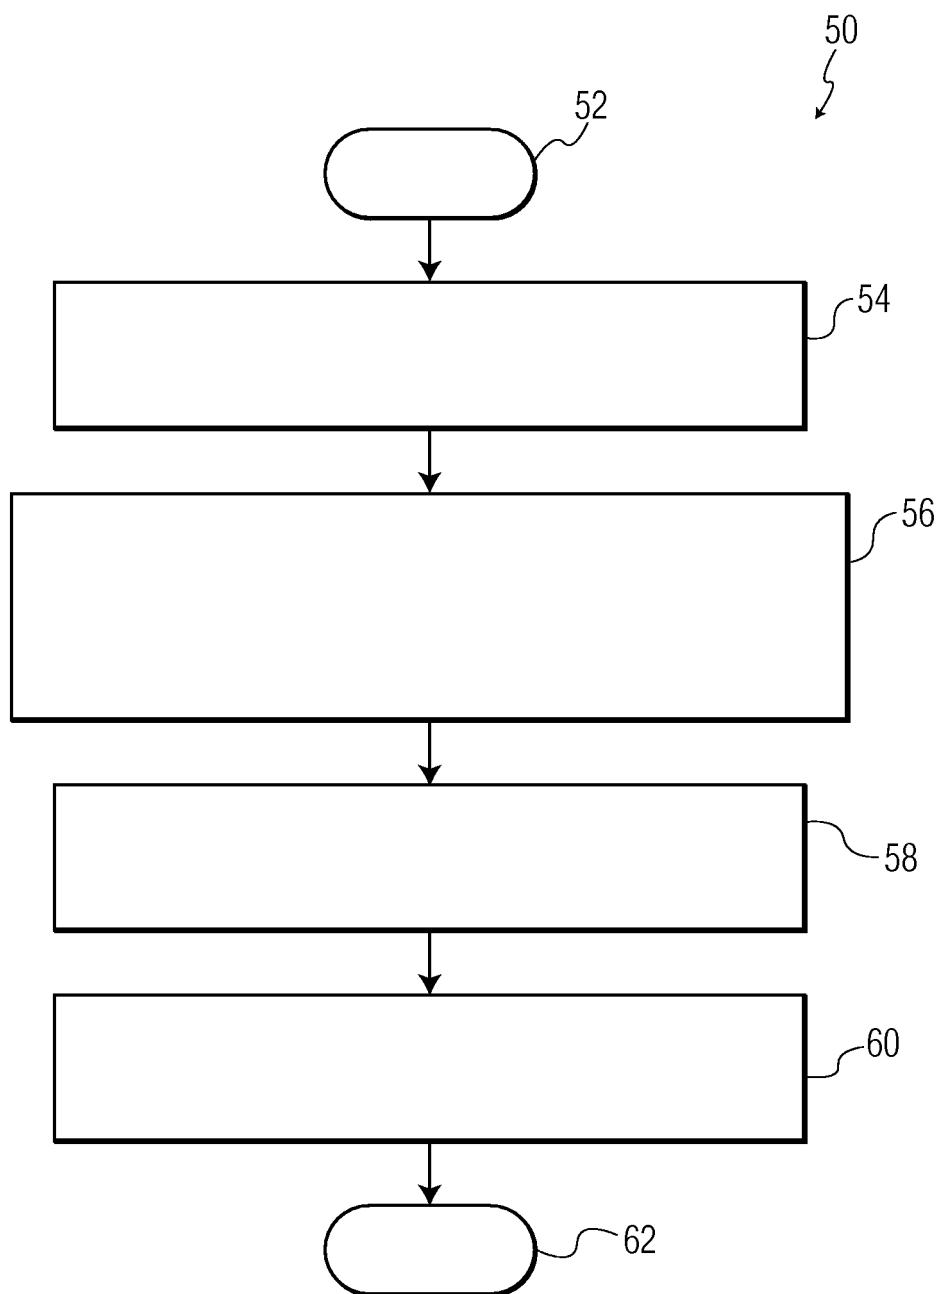
FIG. 3

专利名称(译)	使用固定光束估计参数的3D超声成像的方法和装置		
公开(公告)号	EP1895909A2	公开(公告)日	2008-03-12
申请号	EP2006765766	申请日	2006-06-15
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	SHERRILL DAVID S		
发明人	SHERRILL, DAVID S.		
IPC分类号	A61B8/14		
CPC分类号	A61B8/14 A61B8/0883 A61B8/483 A61B2562/0204 A61B2562/046 G01S7/52088 G01S15/8979 G01S15/8993		
优先权	60/693469 2005-06-23 US		
其他公开文献	EP1895909B1		
外部链接	Espacenet		

摘要(译)

一种三维（3D）超声成像方法包括获取表示成像体积的超声数据作为时间的函数，从中可以获得多个二维图像（28），并从静止超声波束获取数据（26）与获取代表成像体积的超声数据同时进行。分析静止超声波束数据以从静止超声波束数据导出参数（34）。该方法还包括根据导出的参数重新排列（36）从获取的超声数据获得的多个2D超声图像以进行3D处理。在一个实施例中，从静止超声波束获取数据包括M模式采集，多普勒模式采集或针对特定超声成像应用定制的采集中的一个或多个。优选地，该方法应用于三维胎儿心脏成像。