



(51) International Patent Classification:

G01N 29/44 (2006.01) *G01N 29/265* (2006.01)
A61B 8/00 (2006.01) *G06T 17/00* (2006.01)
A61B 8/14 (2006.01)

(21) International Application Number:

PCT/CA2013/000302

(22) International Filing Date:

28 March 2013 (28.03.2013)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/617,031 28 March 2012 (28.03.2012) US

(71) Applicant: **UNIVERSITY OF WESTERN ONTARIO**
[CA/CA]; The Gordon Mogenson Bldg., Suite 105, 100
Collip Circle, London, Ontario N6G 4X8 (CA).

(72) Inventors: **BARKER, Kevin**; 1740 Baystreet Crescent,
London, Ontario N6G 5M9 (CA). **FENSTER, Aaron**; 107
Ambleside Drive, London, Ontario N6G 4N9 (CA). **NE-
SHAT, Hamid**; #1508, 190 Cherry Hill Circle, London,
Ontario N6H 2M3 (CA). **KAKANI, Nirmal**; P.O. Box
5339, 339 Windermere Road, London, Ontario N6A 5A5
(CA).


(74) Agents: **RUSTON, David, A.** et al.; Sim & McBurney,
330 University Avenue 6th Floor, Toronto, Ontario M5G
1R7 (CA).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,
NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU,
RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,
ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: ACTUATOR FOR MOVING AN ULTRASOUND PROBE

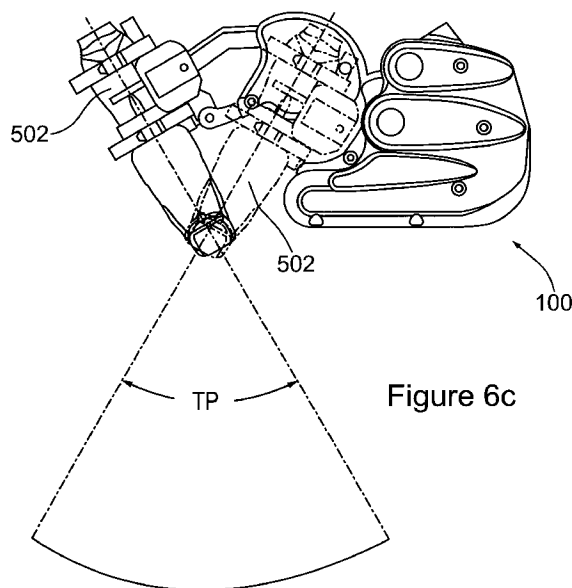

(57) Abstract: An actuator for an ultrasound probe comprises a housing assembly configured to accommodate an ultrasound probe and to be positioned adjacent to a target region of interest to be examined, and a motor assembly coupled to the housing assembly, the motor assembly configured to move the housing assembly in a manner to allow an ultrasound probe when accommodated by the housing assembly to perform a compound scan of the target region of interest.



Published:

— *with international search report (Art. 21(3))*

ACTUATOR FOR MOVING AN ULTRASOUND PROBE

Cross-Reference To Related Application

[0001] This application claims the benefit of U.S. Provisional Application No. 61/617, 031 to Barker et al. filed on March 28, 2012, the entire disclosure of which is incorporated herein by reference.

5 Field of the Invention

[0002] The present invention relates to ultrasound imaging and in particular, to an actuator for moving an ultrasound probe and to an ultrasound imaging system employing the same.

Background of the Invention

10 [0003] A wide variety of approaches have been developed to produce three-dimensional (3D) ultrasound images using both one-dimensional (1D) ultrasound arrays and two-dimensional (2D) ultrasound arrays. The use of 1D ultrasound arrays to produce 3D ultrasound images requires methods to determine the position and orientation of acquired 2D ultrasound images within the 3D ultrasound image volume.

15 The use of 2D ultrasound arrays to produce 3D ultrasound images requires a 3D scan-converter to build the 3D ultrasound images from the sequence of transmit acoustic signals.

[0004] U.S. Patent No. 5,562,095 to Downey et al., the entire disclosure of which is incorporated herein by reference, discloses a 3D ultrasound imaging system for
20 the eye, prostate and other organs, comprising an assembly onto which an ultrasound probe may be mounted, a motor and drive for either rotating or scanning the ultrasound probe relative to the human organ under investigation, and a computer for executing software for controlling movement of the assembly to rotate or scan the ultrasound probe. Ultrasound signals from the probe are processed via a clinical ultrasound
25 machine for generating multiple 2D ultrasound images of the organ. The software executed on the computer collects the 2D ultrasound images of the clinical ultrasound machine and reconstructs the 2D ultrasound images to form a 3D ultrasound image which can be viewed and manipulated in real time, or stored for later retrieval.

- 2 -

[0005] Improvements in 3D ultrasound imaging are generally desired. It is therefore an object at least to provide a novel actuator for moving an ultrasound probe and a novel ultrasound imaging system employing the same.

Summary of the Invention

5 [0006] Accordingly, in one aspect there is provided an actuator for an ultrasound probe comprising a housing assembly configured to accommodate an ultrasound probe and to be positioned adjacent a target region of interest to be examined, and a motor assembly coupled to the housing assembly, the motor assembly configured to move the housing assembly in a manner to allow an ultrasound probe when accommodated by the
10 housing assembly to perform a compound scan of the target region of interest.

[0007] In one embodiment, during the compound scan, the motor assembly is configured to move the housing assembly along a linear path and to tilt the housing assembly during its movement along the linear path. The motor assembly comprises a first motor system and a second motor system, the first motor system being configured to
15 move the housing assembly along the linear path and the second motor system being configured to tilt the housing assembly. The first motor system comprises a motor coupled to a linear slide for moving the housing assembly along the linear path. The second motor system comprises a motor coupled to a plurality of linkage arms for tilting the housing assembly between first and second boundaries.

20 [0008] In one embodiment, the motor assembly is further configured to move the housing assembly along the linear path to allow the ultrasound probe when accommodated by the housing assembly to perform a linear scan of the target region of interest or to tilt the housing assembly to allow the ultrasound probe when accommodated by the housing assembly to perform a tilt scan of the target region.

25 [0009] In one embodiment, the housing assembly comprises a harness to retain the ultrasound probe therein. A casing encloses at least the motor assembly and has user actuatable controls thereon. Formations are provided in the casing to accommodate a user's fingers and the user actuatable controls are positioned approximate the formations.

[0010] According to another aspect there is provided an ultrasound imaging
30 system comprising the above actuator, an ultrasound probe accommodated by the housing assembly of the actuator, and processing structure configured to process

- 3 -

ultrasound signals output by the ultrasound probe and to control the motor assembly of the actuator.

[0011] According to another aspect there is provided a method of reconstructing a three-dimensional ultrasound image of a target region of interest, the method comprising: receiving a plurality of 2D ultrasound images captured during a compound scan of the target region of interest; and mapping pixels of each of the received 2D ultrasound images to a corresponding voxel within a reconstruction matrix.

[0012] In one embodiment, the 2D ultrasound images are received in succession. Each pixel of each 2D ultrasound image is mapped to a corresponding voxel within the reconstruction matrix. The reconstruction matrix is displayed on a display device. A mapping matrix is calculated to map pixels of each received 2D ultrasound image to the corresponding voxel within the reconstruction matrix.

[0013] According to yet another aspect there is provided a method of reconstructing a three-dimensional ultrasound image of a target region of interest, the method comprising: calculating a mapping matrix to map pixels within an acquisition matrix to a corresponding voxel within a reconstruction matrix; receiving a plurality of 2D ultrasound images captured during a compound scan of the target region of interest and storing pixels of each of the plurality of 2D ultrasound images within the acquisition matrix; mapping each pixel within the acquisition matrix with a corresponding voxel within the reconstruction matrix using the mapping matrix; and storing a pixel value associated with each pixel within the acquisition matrix at the corresponding voxel within the reconstruction matrix.

Brief Description of the Drawings

[0014] Embodiments will now be described more fully with reference to the accompanying drawings in which:

[0015] Figure 1 is a schematic block diagram of a 3D ultrasound imaging system;

[0016] Figure 2a is an isometric view of a motor assembly and a housing assembly forming part of an actuator of the 3D ultrasound imaging system of Figure 1;

[0017] Figure 2b is a top plan view of the motor assembly and the housing assembly of Figure 2a;

- 4 -

- [0018] Figure 2c is a front elevational view of the motor assembly and the housing assembly of Figure 2a;
- [0019] Figure 2d is a side elevational view of the motor assembly and the housing assembly of Figure 2a;
- 5 [0020] Figure 2e is a top plan view of the motor assembly disassembled;
- [0021] Figure 3a is an isometric view of the motor assembly, the housing assembly, an ultrasound probe and a casing;
- [0022] Figure 3b is a top plan view of the motor assembly, the housing assembly, the ultrasound probe and the casing;
- 10 [0023] Figure 3c is a front elevational view of the motor assembly, the housing assembly, the ultrasound probe and the casing;
- [0024] Figure 3d is a side elevational view of the motor assembly, the housing assembly, the ultrasound probe and the casing;
- [0025] Figure 4 is a flowchart showing a 3D ultrasound imaging system operation method;
- 15 [0026] Figures 5a to 5c are side elevational views of the 3D ultrasound imaging system of Figure 1 during operation in a linear scanning mode;
- [0027] Figures 6a to 6c are side elevational views of the 3D ultrasound imaging system of Figure 1 during operation in a tilt scanning mode;
- 20 [0028] Figures 7a to 7c are side elevational views of the 3D ultrasound imaging system of Figure 1 during operation in a compound scanning mode;
- [0029] Figure 8 is a flowchart showing a method for reconstructing a 3D ultrasound image during the compound scanning mode; and
- [0030] Figure 9 is an exemplary ultrasound image reconstructed according to the method of Figure 8.
- 25

Detailed Description of the Embodiments

- [0031] In the following, an actuator for an ultrasound probe and an ultrasound imaging system employing the same are described. The actuator comprises a housing assembly configured to accommodate an ultrasound probe and to be positioned adjacent
- 30 to a target region of interest to be examined. The region of interest may be a human organ or tissue such as for example a liver, a kidney, a breast, etc. A motor assembly is

- 5 -

coupled to the housing assembly and is configured to move the housing assembly and hence the ultrasound probe, in a manner to allow the ultrasound probe when accommodated by the housing assembly to perform a compound scan of the target region of interest.

5 **[0032]** Turning now to Figure 1, a schematic block diagram of a 3D ultrasound imaging system 100 is shown. In this embodiment, the 3D ultrasound imaging system 100 is operable in a plurality of modes including a linear scanning mode, a tilt scanning mode, and a compound scanning mode, as will be described. The 3D ultrasound imaging system 100 comprises a general purpose computing device 200 that is
10 communicatively coupled to an actuator 250. The actuator 250 comprises a motor assembly 300 and a housing assembly 400. The motor assembly 300 receives control commands from the general purpose computing device 200 and in response, moves the housing assembly 400. The housing assembly 400 accommodates an ultrasound probe 502 (see Figures 3a to 3d) that communicates with a clinical ultrasound machine 500.
15 The clinical ultrasound machine 500 processes ultrasound signals received from the ultrasound probe 502 during scanning of a target region of interest to generate 2D ultrasound images of the region of interest. The clinical ultrasound machine 500 is communicatively coupled to the general purpose computing device 200 and sends generated 2D ultrasound images thereto. The general purpose computing device 200 in
20 turn processes the received 2D ultrasound images to reconstruct a 3D ultrasound image of the target region of interest, which is communicated to a user interface 600 for display thereon.

[0033] The general purpose computing device 200 in this embodiment is a personal computer or other suitable processing device comprising, for example, a
25 processing unit, system memory (volatile and/or non-volatile memory), other non-removable or removable memory (e.g., a hard disk drive, RAM, ROM, EEPROM, CD-ROM, DVD, flash memory, etc.) and a system bus coupling the various computing device components to the processing unit. The general purpose computing device 200 may also comprise networking capability using Ethernet, WiFi, and/or other network
30 format, to access shared or remote drives, one or more networked computers, or other networked devices.

- 6 -

[0034] Figures 2a to 2e illustrate the motor assembly 300 and the housing assembly 400 and Figures 3a and 3d illustrate the motor assembly 300, the housing assembly 400, the ultrasound probe 502, and a casing 700 enclosing the motor assembly 300 and a portion of the housing assembly 400.

5 [0035] In this embodiment, motor assembly 300 comprises a linear motor system 302 and a tilt motor system 304. The linear motor system 302 comprises a motor 306 coupled to a linear slide carriage 310 via a lead screw 312. Each side of the linear carriage 310 is connected to a linear slide 308. Each linear slide 308 is slidably mounted to a respective stationary rail which is connected to an interior surface of the casing 700,
10 as will be described. As the motor 306 rotates the lead screw 312, the linear slide carriage 310 moves along a linear path. The movement of the linear slide carriage 310 causes movement of each linear slide 308 along its respective stationary rail. As such, the linear motor system 302 moves the housing assembly 400 along the linear path. In this embodiment, the motor 306 has a gear ratio of about 112:1 and a maximum no load
15 output speed of about 59 revolutions-per-minute (RPM). The lead screw 312 has a pitch of about 1/2.7 inches. The linear motor system 302 is configured to move the linear slides 308 a total of about 3cm along the linear path at a speed of about 0.75cm/s.

[0036] The tilt motor system 304 comprises a motor 314 and a plurality of linkage arms 316, 318 and 320 formed of aluminum or other suitable material. The tilt
20 motor system 304 is shown disassembled in Figure 2e together with linear slide carriage 310. The linkage arms 316, 318 and 320 and linear slide carriage 310 are connected to one another, as will be described, via a polyether ether ketone (PEEK) bushing on a stainless steel shaft. A first connection point 316-1 of linkage arm 316 is connected to a first connection point 318-1 of linkage arm 318. A second connection point 316-2 of
25 linkage arm 316 is connected to the linear slide carriage 310 at connection point 310-1. A front end defined by connection points 320-1 and 320-2 of linkage arm 320 is connected to the linear slide carriage 310 at connection points 310-2 and 310-3, respectively. A back end of linkage arm 320 defined by connection points 320-3 and 320-4 is connected to housing assembly 400. A connection point 318-2 of linkage arm
30 318 is connected to a driving shaft (not shown) of motor 314. Linkage arm 318 is connected to a lower portion of housing assembly 400 at connection points 318-3 and 318-4. As will be appreciated, motor 314, when actuated, imparts rotation of linkage

- 7 -

arm 318. As a result of the rotation, linkage arms 316 and 320 rotate and thus, the tilt motor system 304 provides tilt motion to housing assembly 400 between a range of about -30° and 30° . In this embodiment, the motor 314 has a gear ratio of about 207:1 and a maximum no load output speed of about 32 RPM. The tilt motor system 304 is
5 configured to complete a 60° sweep in about 4 seconds.

[0037] Housing assembly 400 comprises a linkage arm 402 connected to the connection points 320-3 and 320-4 of linkage arm 320. A bottom portion 404 of the housing assembly 400 is connected to connection points 318-3 and 318-4 of linkage arm 318. The housing assembly 400 has a housing port 406 dimensioned to securely hold a
10 harness 410 that is configured to retain the ultrasound probe 502. A handle 408 is tangentially connected to a side of the housing assembly 400. The top of the handle 408 comprises a locking button for locking the harness 410 therein. The bottom of the handle 408 comprises an unlocking button for unlocking the harness 410 therefrom. In this embodiment, the housing assembly 400, including the linkage arm 402 and handle
15 408, is made of a polyether ether ketone (PEEK) material. Harness 410 is positioned around a top portion of the ultrasound probe 502 and retains the ultrasound probe 502. The harness 410 is custom made for different types of ultrasound probes. The harness 410 is opened by loosening a screw associated therewith and when opened, the harness 410 is able to receive the ultrasound probe 502.

20 [0038] The casing 700 in this embodiment is made of a molded plastic material such as for example ABS-M30 manufactured by Stratasys®. The interior surface of the casing 700 comprises a pair of stationary rails (not shown). Each stationary rail extends along a respective side of the interior surface of the casing 700 and is configured to support a respective linear slide 308. Each side of the exterior surface of the casing 700
25 has a pair of grooves 702 formed therein, each of which is dimensioned to receive a finger of a user. A plurality of operational buttons is positioned within the grooves 702. The buttons can be user actuated to allow the user to control and operate the 3D ultrasound imaging system 100. Exemplary functions associated with the operational buttons include start scan, stop scan, jog, etc.

30 [0039] The user interface 600 in this embodiment comprises a display monitor such as for example a liquid crystal display (LCD) panel or other suitable display panel or device connected to the general purpose computing device 200 via a cable such as for

- 8 -

example a high-definition multimedia interface (HDMI) cable or a video graphics array (VGA) cable or other suitable wired or wireless communications link. The user interface 600 displays the graphical user interface of an application program executed by the general purpose computing device 200. The user interface 600 further comprises a keyboard and a mouse and/or other suitable user input devices, which are connected to the general purpose computing device 200 via a universal serial bus (USB) cable or other suitable wired or wireless connection.

[0040] Turning now to Figure 4, a method of operating the 3D ultrasound imaging system 100 is shown and is generally identified by reference numeral 800.

During operation, when the general purpose computing device 200 receives a mode selection from the user interface 600 (step 802), a check is performed to determine which mode has been selected (step 804). If the linear scanning mode has been selected, when a start scan command has been input via actuation of the associated operational button, the linear motor system 302 is actuated by the general purpose computing device 200 (step 806) and thus, a linear scan of the target region of interest is performed by the 3D ultrasound imaging system 100, and the method ends. If the tilt scanning mode has been selected, when a start scan command has been input via actuation of the associated operational button, the tilt motor system 304 is actuated by the general purpose computing device 200 (step 808) and thus, a tilt scan of the target region of interest is performed by the 3D ultrasound imaging system 100, and the method ends. If the compound scanning mode has been selected, when a start scan command has been input via actuation of the associated operational button, both the linear motor system 302 and the tilt motor system 304 are actuated by the general purpose computing device 200 (step 810) and thus a compound scan of the target region of interest is performed by the 3D ultrasound imaging system 100, and the method ends.

[0041] Turning to Figure 5a, the start position of the actuator 250 in the linear scanning mode is shown. As can be seen, ultrasound probe 502 is positioned such that its longitudinal axis is generally normal to the surface of the target region of interest to be scanned. Each linear slide 308 is at its rearward most position on the respective stationary rail. As will be appreciated, each linear slide 308 is contained within casing 700, and thus is not visible in Figure 5a.

- 9 -

[0042] Figure 5b shows the finish position of the actuator 250 in the linear scanning mode. As can be seen, ultrasound probe 502 remains positioned such that its longitudinal axis is generally normal to the surface of the target region of interest to be scanned. Each linear slide 308 is at its forward most position on the respective stationary rail. As such, the linear slide carriage 310 extends out of casing 700. Again, as each linear slide 308 is contained within casing 700, it is not visible in Figure 5b.

[0043] Figure 5c shows both the start position and the finish position of the actuator 250 in the linear scanning mode. As can be seen, the ultrasound probe 502 moves from the start position to the finish position along a linear path indicated by arrow LP. The linear path LP is defined by movement of the linear slide carriage 310 and the resultant movement of each linear slide 308 along its respective stationary rail. As such, the ultrasound probe 502 performs a linear scan of the target region of interest when moved along linear path LP. It will be appreciated that in the linear scanning mode, there is no tilt movement of the ultrasound probe 502.

[0044] During operation in the linear scanning mode, the ultrasound probe 502 scans the target region of interest as it moves along the linear path LP and outputs ultrasound signals to the clinical ultrasound machine 500. The ultrasound signals from the ultrasound probe 502 are processed via the clinical ultrasound machine 500 to generate a plurality of 2D ultrasound images of the target region of interest at the desired frame rate (typically 15 or 30 frames per second). The 2D ultrasound images are then communicated to the general purpose computing device 200 for processing. The general purpose computing device 200 processes the 2D ultrasound images to reconstruct a 3D ultrasound image covering a rectangular volume of the scanned target region of interest according to a known method such as that described in above-incorporated U.S. Patent No. 5,562,095 to Downey et al.

[0045] Turning to Figure 6a, the start position of the actuator 250 in the tilt scanning mode is shown. As can be seen, ultrasound probe 502 is positioned such that its longitudinal axis is approximately 30° to the normal of the surface of the target region of interest to be scanned. Each linear slide 308 is at its rearward most position on the respective stationary rail. As will be appreciated, each linear slide 308 is contained within casing 700, and thus is not visible in Figure 6a.

- 10 -

[0046] Figures 6b shows the finish position of the actuator 250 in the tilt scanning mode. As can be seen, ultrasound probe 502 is positioned such that its longitudinal axis is approximately -30° to the normal of the surface of the target region of interest to be scanned. Each linear slide 308 is at its rearward most position on the
5 respective stationary rail. As will be appreciated, each linear slide 308 is contained within casing 700, and thus is not visible in Figure 6b.

[0047] Figure 6c shows both the start position and the finish position of the actuator 250 in the tilt scanning mode. As can be seen, the ultrasound probe 502 moves from the start position to the finish position along a path indicated by arrow TP. As
10 such, the ultrasound probe 502 performs a tilt scan of the target region of interest when moved along path TP. It will be appreciated that in the tilt scanning mode, there is no linear movement of the ultrasound probe 502.

[0048] During operation in the tilt scanning mode, the ultrasound probe 502 scans the target region of interest as it moves along path TP and outputs ultrasound
15 signals to the clinical ultrasound machine 500. The ultrasound signals from the ultrasound probe 502 are processed via the clinical ultrasound machine 500 to generate a plurality of 2D ultrasound images of the target region of interest at the desired frame rate (typically 15 or 30 frames per second). The 2D ultrasound images are communicated to the general purpose computing device 200 for processing. The general purpose
20 computing device 200 in turn processes the 2D ultrasound images to reconstruct a 3D ultrasound image covering a pie-shaped volume of the scanned target region of interest according to a known method such as that described in above-incorporated U.S. Patent No. 5,562,095 to Downey et al.

[0049] Turning to Figure 7a, the start position of the actuator 250 in the
25 compound scanning mode is shown. As can be seen, ultrasound probe 502 is positioned such that its longitudinal axis is approximately -30° to the normal of the surface of the target region of interest to be scanned. Each linear slide 308 is at its rearward most position on the respective stationary rail. As will be appreciated, each linear slide 308 is contained within casing 700, and thus is not visible in Figure 7a.

30 [0050] Figure 7b shows the finish position of the actuator 250 in the tilt scanning mode. As can be seen, ultrasound probe 502 is positioned such that its longitudinal axis is approximately 30° to the normal of the surface of the target region of interest to be

- 11 -

scanned. Each linear slide 308 is also at its forward most position on the respective stationary rail. Again, as each linear slide 308 is contained within casing 700, it is not visible in Figure 7b.

[0051] Figure 7c shows both the start position and the finish position of the actuator 250 in the compound scanning mode. As can be seen, the ultrasound probe 502 moves from the start position to the finish position along a path indicated by arrow CP. As such, the ultrasound probe 502 performs a compound scan of the target region of interest when moved along path CP. Comparing the scan path of the ultrasound probe 502 during operation in the compound scanning mode (Figure 7c) to the scan paths of the ultrasound probe 502 during operation in the linear scanning mode (Figure 5c) and tilt scanning mode (Figure 6c), a larger volume is covered by the ultrasound probe 502 during operation in the compound scanning mode.

[0052] During operation in the compound scanning mode, the ultrasound probe 502 scans the target region of interest as it moves along path CP. The ultrasound signals output by the ultrasound probe 502 are processed via the clinical ultrasound machine 500 to generate a plurality of 2D ultrasound images of the target region of interest at the desired frame rate (typically 15 or 30 frames per second). The 2D ultrasound images are communicated to the general purpose computing device 200 for processing. The general purpose computing device 200 in turn processes the 2D ultrasound images to reconstruct a 3D ultrasound image covering a frusto-conical shaped volume of the scanned target region of interest as will now be described below.

[0053] As will be appreciated, in the compound scanning mode, reconstructing a 3D ultrasound image from the plurality of 2D ultrasound images must take into account both the linear and tilt movements of the ultrasound probe 502. For this purpose, two 3D matrices are created within memory associated with the general purpose computing device 200 and mapped to one another.

[0054] The first 3D matrix, hereinafter referred to as an acquisition matrix, holds pixel values of each acquired 2D ultrasound image. The size of the acquisition matrix is expressed as:

$$h \times w \times n \quad (1)$$

where h is the number of pixels in each 2D ultrasound image along the Y-direction, w is the number of pixels in each 2D ultrasound image along the X-direction, and n is the

- 12 -

number of 2D ultrasound images to be captured during the compound scan. It should be noted that the number of pixels in each 2D ultrasound image along the Y-direction h and X-direction w are fixed for the compound scan. The number of 2D ultrasound images to be captured n is determined by dividing the maximum sweeping angle of the ultrasound probe 502 by a desired angle between two consecutive 2D ultrasound images. The desired angle between two consecutive 2D ultrasound images is set by the user prior to ultrasound image acquisition via the user interface 600. As will be appreciated, the grey-value of each pixel may be one or two bytes depending on the number of bits selected to represent the grey-values. Prior to scanning, each pixel within the acquisition matrix is set to a value of zero, and thus is set to the color black.

[0055] The second 3D matrix, hereinafter referred to as a reconstruction matrix, holds grey-values of each voxel of the reconstructed 3D ultrasound image. The size of the reconstruction matrix is determined by the acquired image parameters, scanning mode, and maximum sweep either set as default values within the 3D ultrasound imaging system 100 or set by the user via the user interface 600. Specifically, the size of the reconstruction matrix is expressed as:

$$h \times w \times z \quad (2)$$

where h is the number of pixels in each 2D ultrasound image along the Y-direction and w is the number of pixels in each 2D ultrasound image along the X-direction. The value of z is calculated as:

$$z = (n - 1) \left(1 + \frac{2h}{L} \sin(\theta) \right) \quad (3)$$

where n is the number of 2D ultrasound images to be captured, h is the number of pixels in each 2D ultrasound image along the Y-direction, L is the extent of the linear motion during the compound scan, and θ is the maximum angle of the tilt motion during the compound scan.

[0056] To determine an association between a voxel in the reconstruction matrix and a corresponding pixel in the acquisition matrix, a mapping matrix is used. In this embodiment, the mapping matrix is calculated using a closest point method, wherein a particular voxel within the reconstruction matrix is mapped to a pixel within the acquisition matrix that has coordinates closest thereto. The mapping matrix is calculated before the compound scan is performed and is used to fill each voxel within the

- 13 -

reconstruction matrix as corresponding pixels within the acquisition matrix are filled based on the captured 2D ultrasound images. The mapping matrix is stored within memory associated with the general purpose computing device 200 and may be used with future compound scans comprising the same parameters (i.e. angular step angle, linear step distance, linear extent of scan L , maximum angle θ , size of image in X-direction, number of pixels in X-direction, and number of pixels in Y-direction). During the compound scan, the reconstruction matrix is displayed by the user interface 600 such that a user can follow the scanning and reconstructing process.

[0057] Turning to Figure 8, a flowchart showing a method for reconstructing a 3D ultrasound image from a plurality of 2D ultrasound images obtained during a compound scan of the target region of interest is shown and is generally identified by reference numeral 900. Method 900 begins by calculating the mapping matrix (step 902). The mapping matrix is calculated by first transferring each pixel in the acquisition matrix according to corresponding 3D scanning geometry, and then using each transferred pixel to find a reverse map according to the closest point method. Each pixel ($X_{im(i)}, Y_{im(i)}$) in acquired 2D ultrasound image i in the acquisition matrix (containing a total number of acquired 2D ultrasound images n) is transferred to 3D geometry using the following equations:

$$X = X_{im(i)} \quad (4)$$

$$Y = Y_{im(i)} dx \cos(\theta_i) \quad (5)$$

$$Z = i \times dL + Y_{im(i)} dy \sin \theta_i \quad (6)$$

where the transformed 3D coordinates $[X, Y, Z]$ represent the corresponding location in the 3D ultrasound image, θ_i is the angle of the ultrasound probe 502 at which 2D ultrasound image i is acquired, and dL is the linear scanning distance between two consecutive captured 2D ultrasound images. It is noted that the transformed 3D coordinates $[X, Y, Z]$ do not necessarily contain integer values and do not directly correspond to a location within the reconstruction matrix, since coordinates within the reconstruction matrix are integer values. As will be appreciated, if only the integer part of the transformed 3D coordinates $[X, Y, Z]$ is used, depending on the linear scanning distance between two consecutive captured 2D ultrasound images, there may be gaps between the planes in the reconstruction matrix that must be filled. Further, there may

- 14 -

be cases wherein two or more pixels in the acquired 2D ultrasound images contain the same integer values.

[0058] Once the 3D transformation for each pixel ($X_{im(i)}$, $Y_{im(i)}$) in the acquisition matrix has been calculated according to Equations (4), (5) and (6), each voxel within the reconstruction matrix that falls within the boundaries of the scanned target region of interest is evaluated. In this embodiment, any voxel within the reconstruction matrix that is outside of the boundaries of the scanned target region of interest will have a grey-value that results in a black colored voxel. For each of these voxels, a pixel within the acquisition matrix that has coordinates closest to each particular pixel within the reconstruction matrix is identified, and the transformed 3D coordinates [X, Y, Z] of that pixel are recorded within the mapping matrix.

[0059] To minimize processing, given the geometry of the scanned volumes, once a single slice perpendicular to the compound scan direction within the mapping matrix is calculated, the remaining slices within the mapping matrix are determined by changing the value of X . To further minimize processing, given the symmetry about the mid-line of the compound scan, that is, when the ultrasound probe 502 is positioned such that its longitudinal axis is generally perpendicular to the surface of the target region of interest to be scanned, once half of the pixels in a slice have been calculated for the mapping matrix, the second half of the pixels can be readily determined by mirroring the Y value of the calculated pixels. As will be appreciated, each element within the mapping matrix has three components represented by $X_{im(i)}$, $Y_{im(i)}$ and the acquired 2D ultrasound image number i .

[0060] Once the mapping matrix has been calculated, the compound scan begins (step 904). A 2D ultrasound image of the target region of interest is acquired (step 906) and stored in the acquisition matrix (step 908). The pixels of the acquired 2D ultrasound image are mapped to corresponding voxels within the reconstruction matrix using the mapping matrix, and the resulting reconstruction matrix is displayed on the user interface 600 (step 910). A check is performed to determine if the compound scan is complete (step 912). If the compound scan is not complete, the method returns to step 906 to acquire another 2D ultrasound image of the region of interest. Once all of the 2D ultrasound images of the compound scan have been acquired and processed as described above, the method ends.

[0061] A side view of an exemplary ultrasound image 1000 reconstructed according to method 900 is shown in Figure 9. Reconstructed image 1000 was acquired using a linear scanning distance L of 25cm and a maximum angle θ of 27° . As can be seen, reconstructed image 1000 is symmetric about center line 1002, which is shown for illustrative purposes. Each line 1004 represents the side view of a single 2D ultrasound image stored within the reconstruction matrix.

[0062] Although the mapping matrix is calculated above using a closest point method, in another embodiment the mapping matrix may be calculated using an interpolation method, wherein the grey-value of a particular voxel within the reconstruction matrix is determined using the grey-value of a combination of pixels within the acquisition matrix that have coordinates closest to the particular voxel within the reconstruction matrix. In this embodiment, once the 3D transformation for each pixel $(X_{im(i)}, Y_{im(i)})$ in the acquisition matrix has been calculated according to Equations (4), (5) and (6), a linear combination of 2, 4 or 6 pixels within the acquisition matrix that have coordinates closest to each particular voxel within the reconstruction matrix are identified, the grey-value of each of these pixels is used to calculate the grey-value of the corresponding voxel in the reconstruction matrix, and the transformed 3D coordinates $[X, Y, Z]$ of each of the 2, 4 or 6 pixels are stored in the mapping matrix. As will be appreciated, if 2 pixels are used, each pixel within the mapping matrix will contain 8 components represented by $X_{im(i)}, Y_{im(i)}$ and the acquired 2D ultrasound image number i for each of the 2 pixels identified in the acquisition matrix, as well as 2 values associated with the weighting factors of the 2 pixels. If 4 pixels are used, each pixel within the mapping matrix will contain 16 components represented by $X_{im(i)}, Y_{im(i)}$ and the acquired 2D ultrasound image number i for each of the 4 pixels identified in the acquisition matrix, as well as 4 values associated with the weighting factors of the 4 pixels. Similarly, if 6 pixels are used, each pixel within the mapping matrix will contain 24 components represented by $X_{im(i)}, Y_{im(i)}$ and the acquired 2D ultrasound image number i for each of the 6 pixels identified in the acquisition matrix, as well as 6 values associated with the weighting factors of the 6 pixels.

[0063] Those skilled in the art will appreciate that virtually any type of ultrasound probe may be used and virtually any type of clinical ultrasound machine that is compatible with the selected ultrasound probe may be used. For example, clinical

- 16 -

ultrasound machines utilizing B-mode ultrasound, Doppler imaging ultrasound, or power Doppler imaging ultrasound may be used.

[0064] Although the linkage arms are described above as being made of aluminum, those skilled in the art will appreciate that other types of material may be used such as for example stainless steel, plastic materials, etc.

[0065] Although the linear motor system is described above as comprising a linear slide to provide movement along a single axis, those skilled in the art will appreciate that other arrangements may be used. For example, a box slide or dovetail may be used. Similarly, the linear movement may be achieved through use of rods or round rails. Also, although the linear motor system is described above as comprising a motor driven lead screw to provide movement along a single axis, those skilled in the art will appreciate that other arrangements may be used. For example, devices such as a belt, chain, rack and pinion gearing may be used.

[0066] Although the tilt motor system is described above as comprising a motor directly connected to one or more linkage arms, the tilt motor system may alternatively use one or more gears to adjust the speed of the tilt motor system.

[0067] Although the linear motor system and tilt motor system are described above as comprising separate motors, those skilled in the art will appreciate that one motor may be used. For example, a single motor may be used in combination with a specific orientation of linkage arms to operate within tilt and linear motion parameters, thereby achieving proper motion for a compound scan. It will also be appreciated that different types of motors may be used such as for example brushed DC motors.

[0068] Although the ultrasound probe is described above as being retained within the housing assembly via a harness, those skilled in the art will appreciate that other types of mechanical retaining devices may be used. For example, a quick release mechanism or spring-loaded quick release mechanism may be used to retain the ultrasound probe within the housing assembly.

[0069] Although voxels within the reconstruction matrix are considered to be outside of the scanned target region of interest if they are black in color, those skilled in the art will appreciate that the voxels to be evaluated may be selectable by a user via user interface 600.

- 17 -

[0070] In embodiments described above, particular motor gear ratios and output speeds, lead screw pitches, path distances, sweeps and speeds as well as particular component materials have been specified. Those of skill in the art will appreciate that these specifics are exemplary and that alternatives are available.

- 5 [0071] Although embodiments have been described with reference to the drawings, those of skill in the art will appreciate that variations and modifications may be made without departing from the scope thereof as defined by the appended claims.

- 18 -

What is claimed is:

1. An actuator for an ultrasound probe comprising:
a housing assembly configured to accommodate an ultrasound probe
5 and to be positioned adjacent to a target region of interest to be examined; and
a motor assembly coupled to the housing assembly, the motor
assembly configured to move the housing assembly in a manner to allow an
ultrasound probe when accommodated by the housing assembly to perform a
compound scan of the target region of interest.
10
2. The actuator of claim 1 wherein during the compound scan, the motor
assembly is configured to move the housing assembly along a linear path and to tilt
the housing assembly during its movement along the linear path.
- 15 3. The actuator of claim 2 wherein the motor assembly comprises a first
motor system and a second motor system, the first motor system being configured to
move the housing assembly along the linear path and the second motor being system
configured to tilt the housing assembly.
- 20 4. The actuator of claim 3 wherein the first motor system comprises a
motor coupled to a linear slide for moving the housing assembly along the linear path.
5. The actuator of claim 3 or 4 wherein the second motor system
comprises a motor coupled to a plurality of linkage arms for tilting the housing
25 assembly between first and second boundaries.
6. The actuator of claim 5 wherein the first and second boundaries are
defined by first and second angles measured with respect to the normal to a surface of
the target region of interest.
30
7. The actuator of claim 6 wherein the first and second angles are
complimentary.

- 19 -

8. The actuator of claim 6 or 7 wherein the first angle is equal to approximately 30° and the second angle is equal to approximately -30° .
- 5 9. The actuator of any one of claims 2 to 8 wherein the motor assembly is further configured to move the housing assembly along the linear path to allow the ultrasound probe when accommodated by the housing assembly to perform a linear scan of the target region of interest or to tilt the housing assembly to allow the ultrasound probe when accommodated by the housing assembly to perform a tilt scan
10 of the target region of interest.
10. The actuator of any one of claims 1 to 9 wherein the housing assembly comprises a harness to retain the ultrasound probe therein.
- 15 11. The actuator of any one of claims 1 to 10 further comprising a casing enclosing at least the motor assembly.
12. The actuator of claim 11 further comprising user actuatable controls on the casing.
20
13. The actuator of claim 12 wherein the casing has formations therein shaped to accommodate a user's fingers and wherein the user actuatable controls are positioned proximate the formations.
- 25 14. An ultrasound imaging system comprising:
an actuator according to any one of claims 1 to 13;
an ultrasound probe accommodated by the housing assembly of the actuator; and
processing structure configured to process ultrasound signals output by
30 the ultrasound probe and to control the motor assembly of the actuator.

- 20 -

15. The ultrasound imaging system of claim 14 wherein the processing structure comprises a clinical ultrasound machine to which the ultrasound probe is connected, the clinical ultrasound machine being configured to generate a succession of two-dimensional ultrasound images during the compound scan, and a processing
5 device configured to reconstruct the two-dimensional ultrasound images to form a three-dimensional ultrasound image of the target region of interest.

16. A method of reconstructing a three-dimensional ultrasound image of a target region of interest, the method comprising:
10 receiving a plurality of 2D ultrasound images captured during a compound scan of the target region of interest; and
 mapping pixels of each of the received 2D ultrasound images to a corresponding voxel within a reconstruction matrix.

15 17. The method of claim 16 wherein the 2D ultrasound images are received in succession.

18. The method of claim 16 or 17 wherein each pixel of each 2D ultrasound image is mapped to a corresponding voxel within the reconstruction
20 matrix.

19. The method of any one of claims 16 to 18 further comprising displaying the reconstruction matrix on a display device.

25 20. The method of claim 18 further comprising calculating a mapping matrix to map pixels of each received 2D ultrasound image to the corresponding voxel within the reconstruction matrix.

21. The method of claim 20 wherein the mapping matrix is calculated prior
30 to receiving the 2D ultrasound images.

- 21 -

22. A method of reconstructing a three-dimensional ultrasound image of a target region of interest, the method comprising:

calculating a mapping matrix to map pixels within an acquisition matrix to a corresponding voxel within a reconstruction matrix;

5 receiving a plurality of 2D ultrasound images captured during a compound scan of the target region of interest and storing pixels of each of the plurality of 2D ultrasound images within the acquisition matrix;

mapping each pixel within the acquisition matrix with a corresponding voxel within the reconstruction matrix using the mapping matrix; and

10 storing a pixel value associated with each pixel within the acquisition matrix at the corresponding voxel within the reconstruction matrix.

23. The method of claim 22 further comprising displaying the reconstruction matrix on a display device.

15

1/12

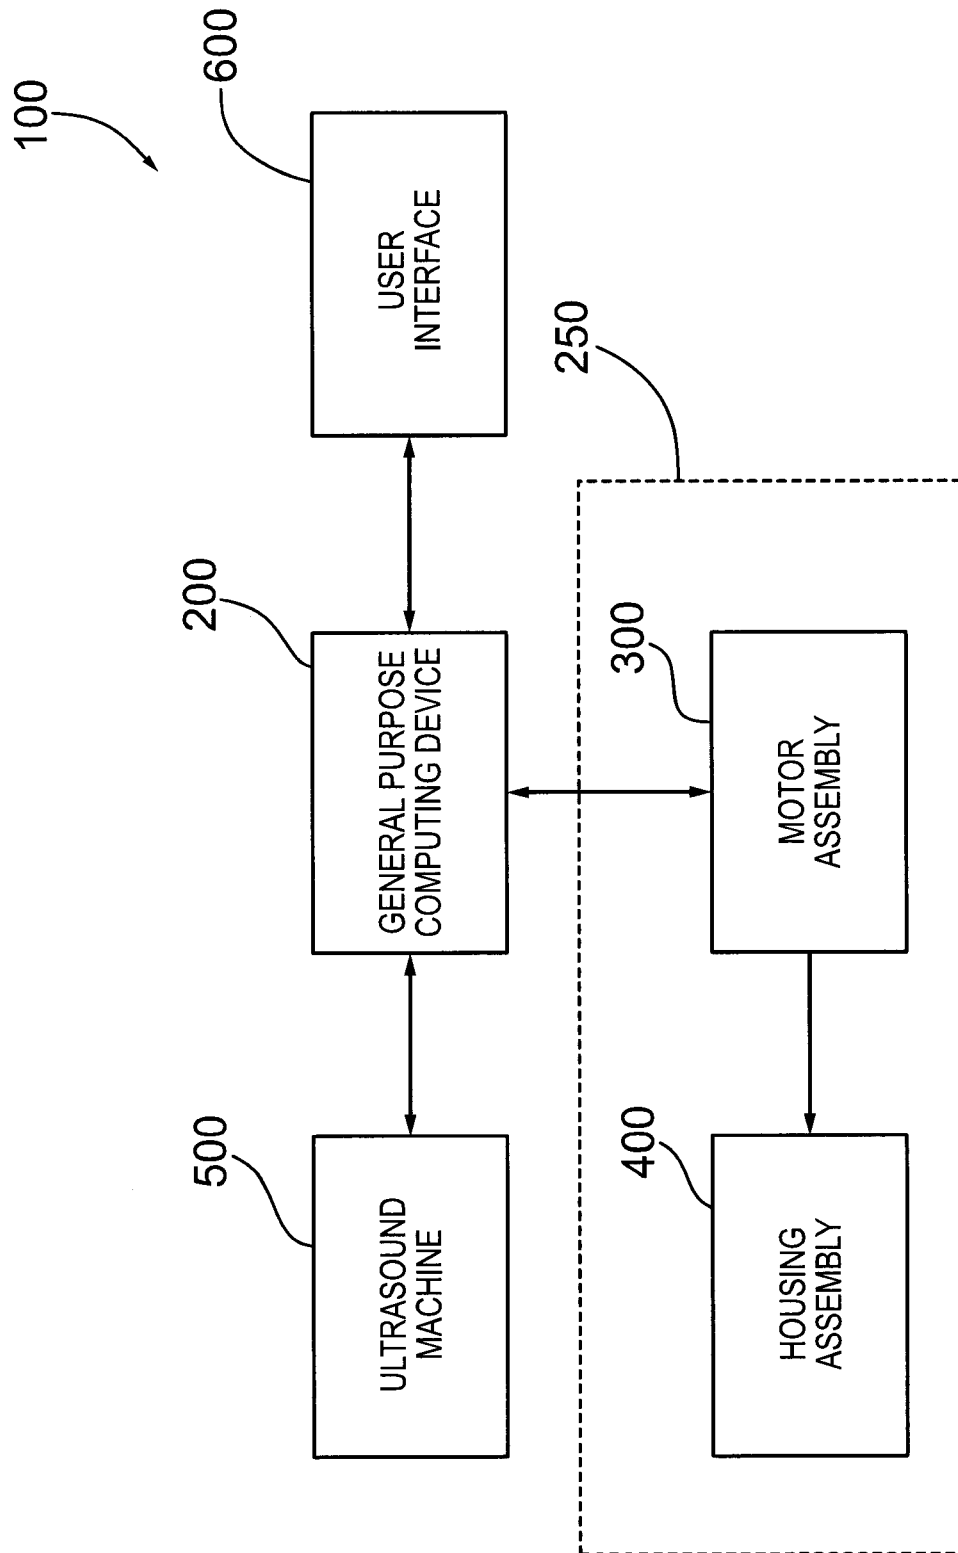


Figure 1

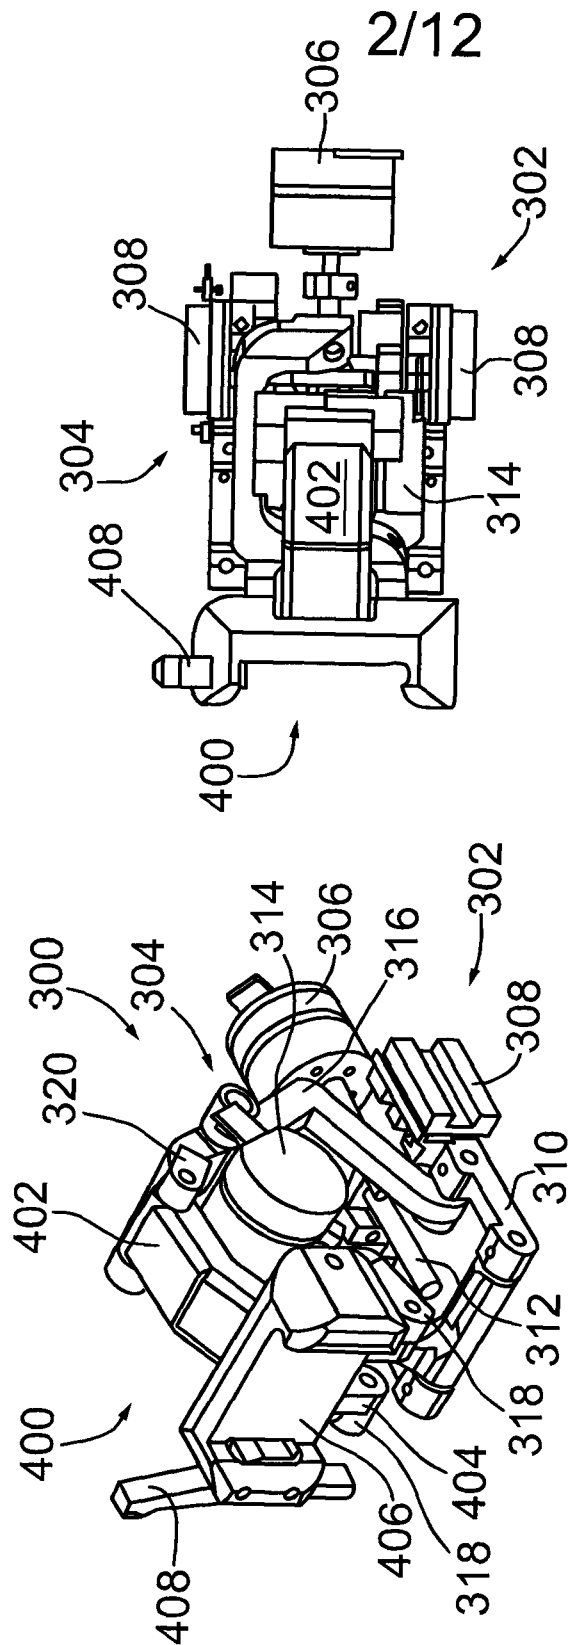
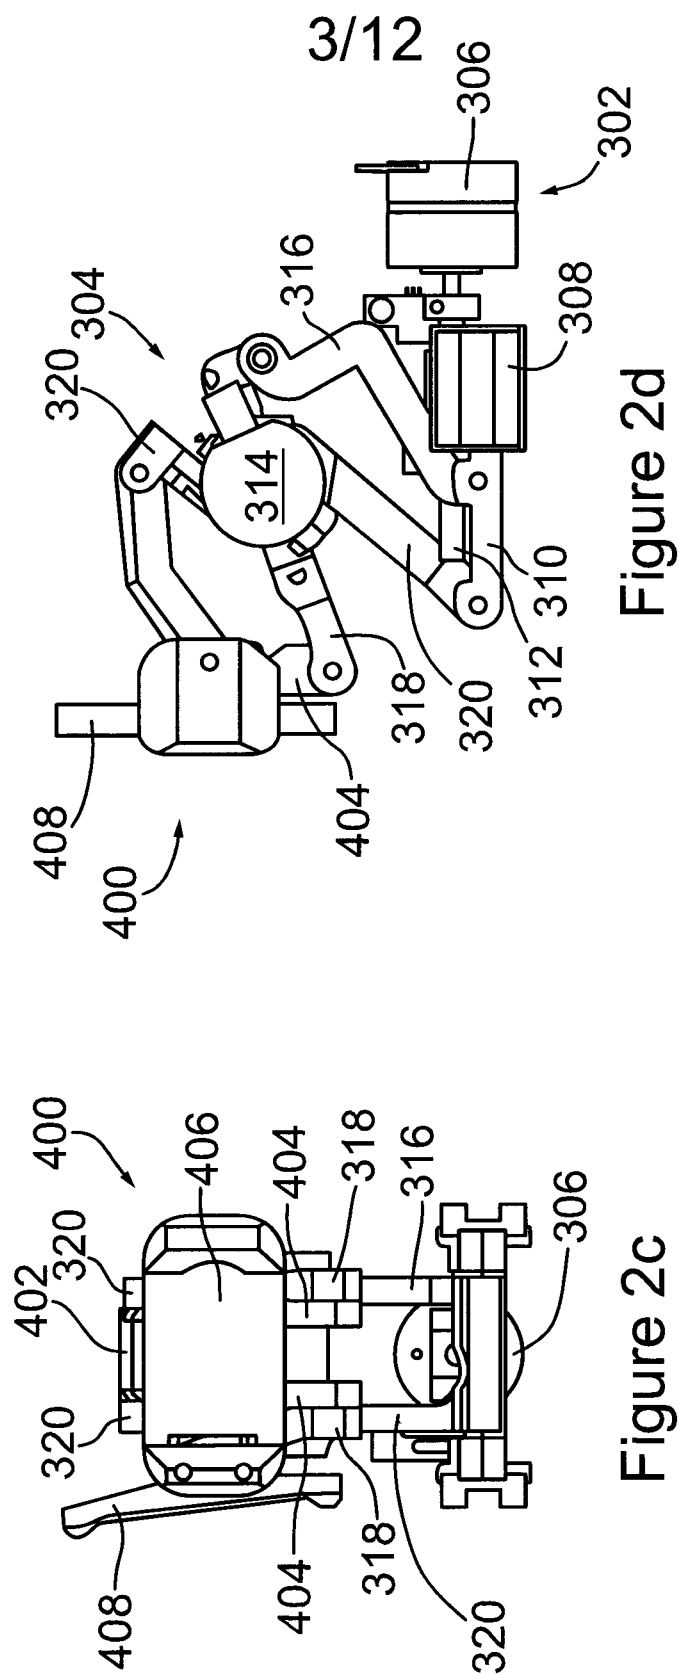


Figure 2b

Figure 2a



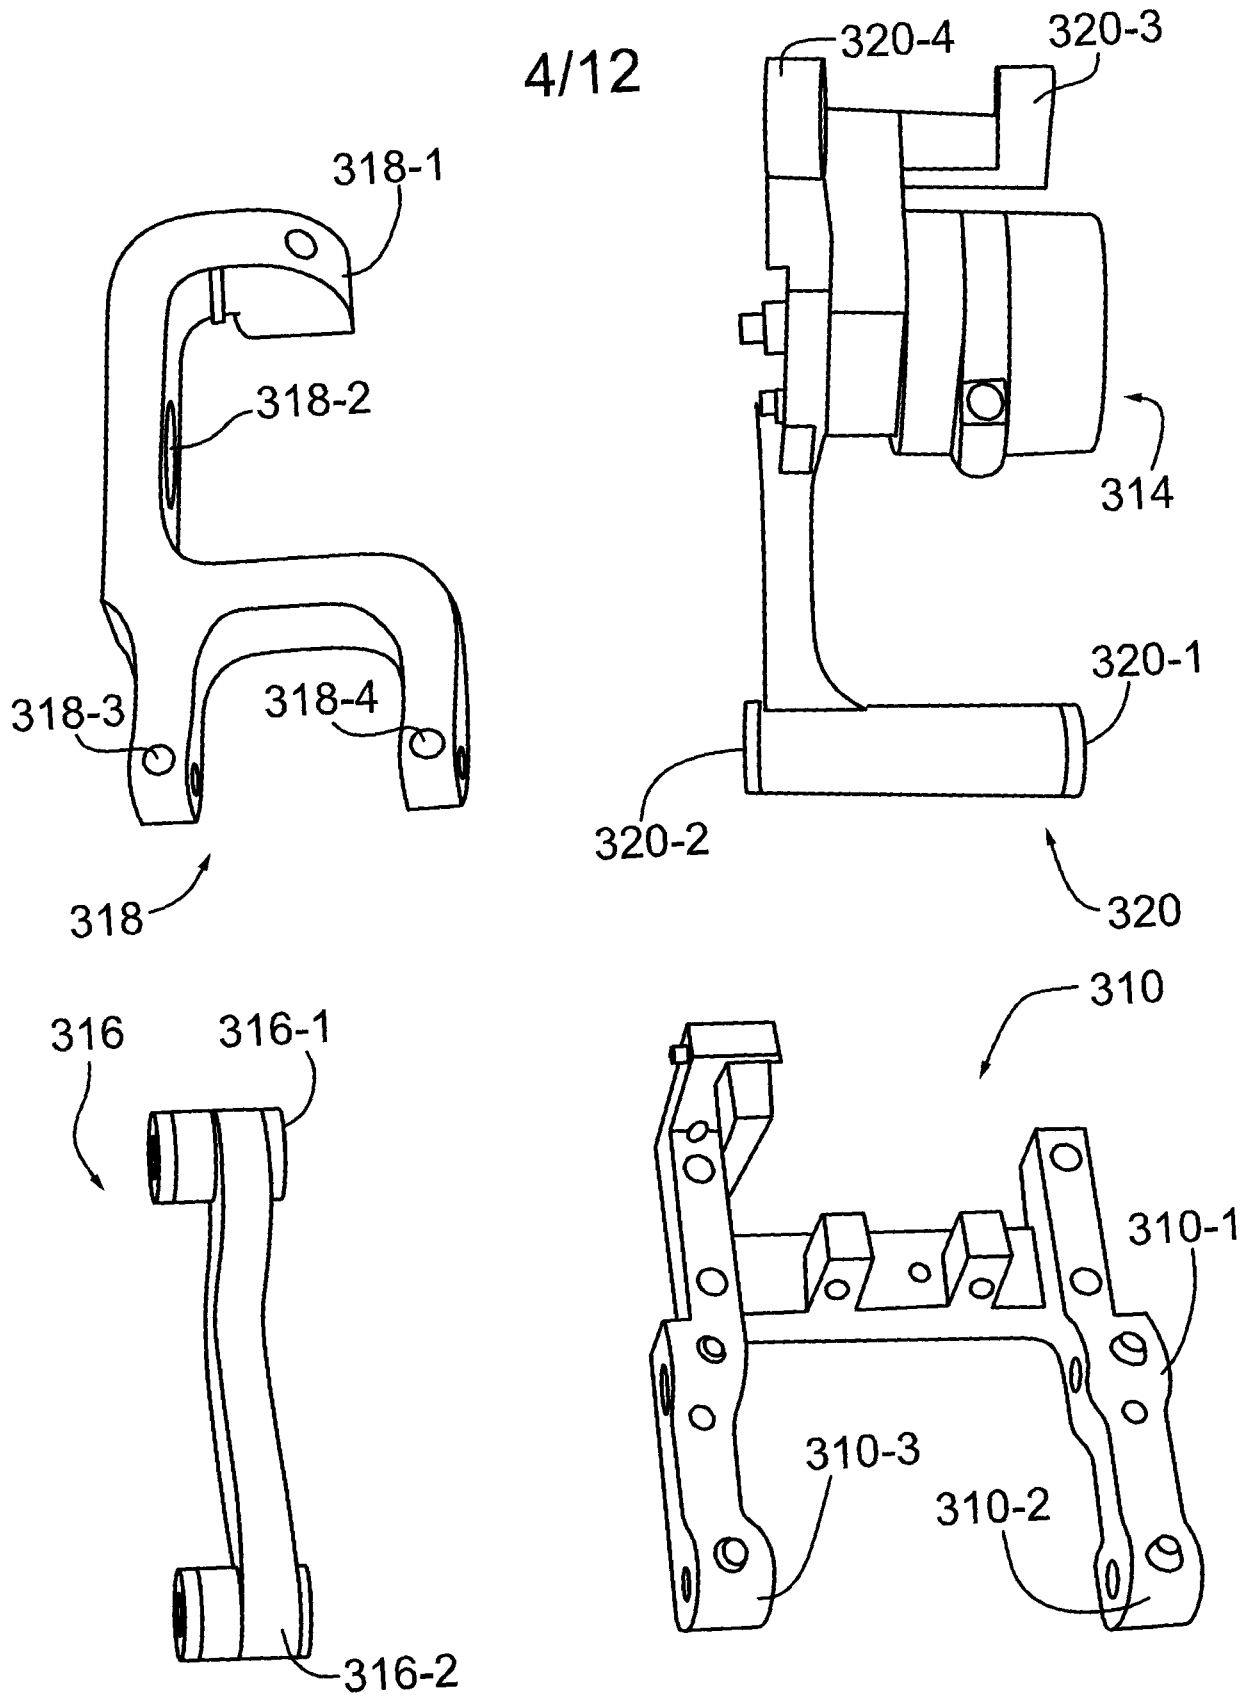


Figure 2e

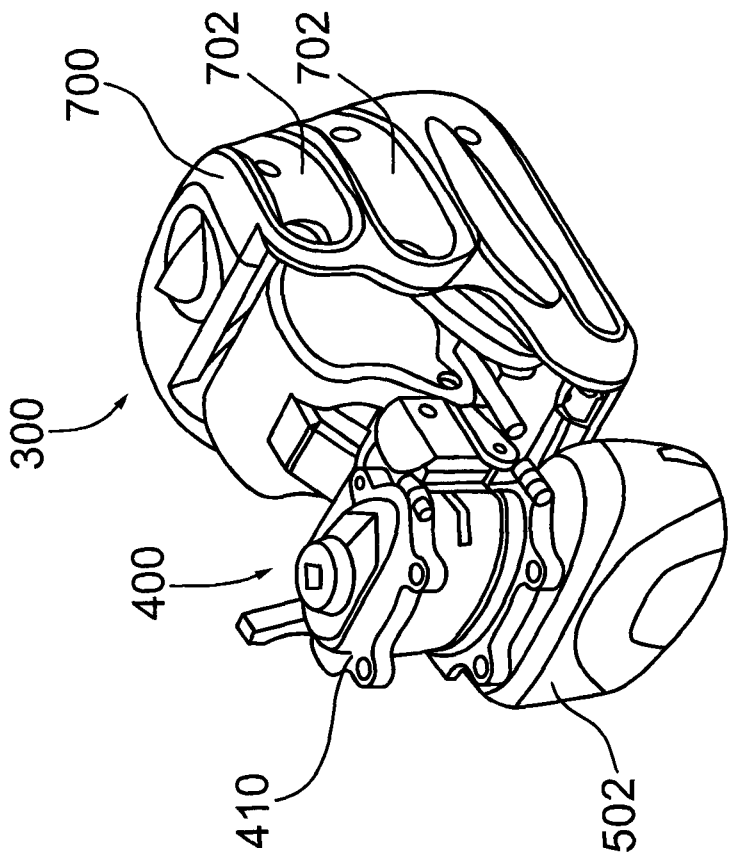


Figure 3a

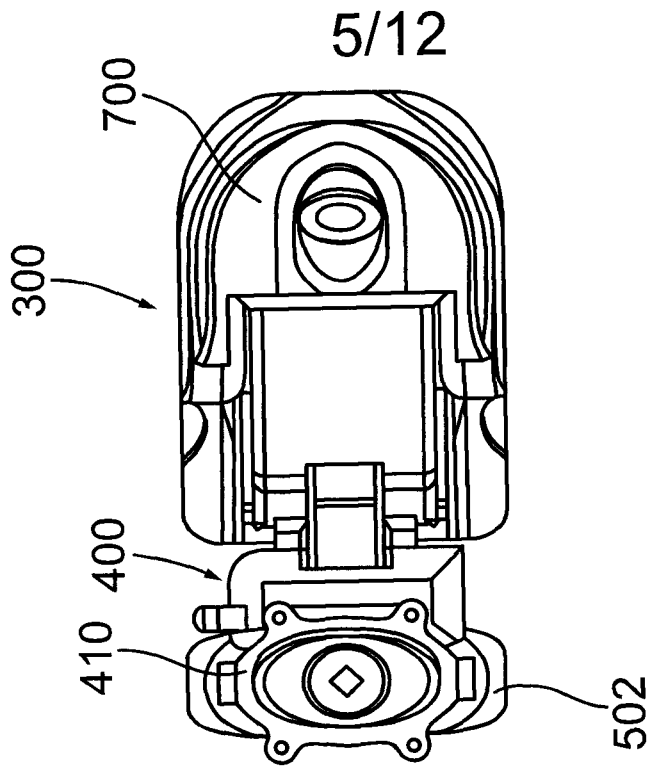


Figure 3b

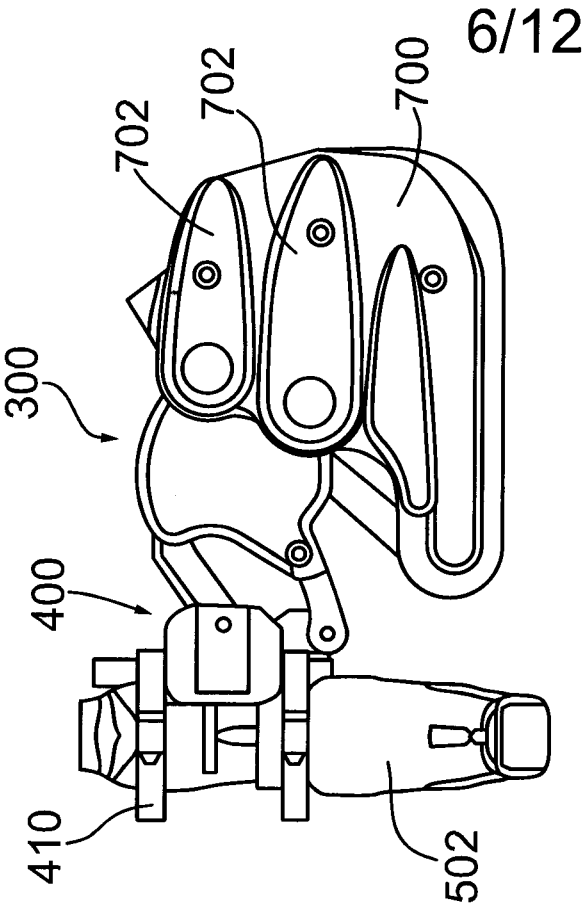


Figure 3d


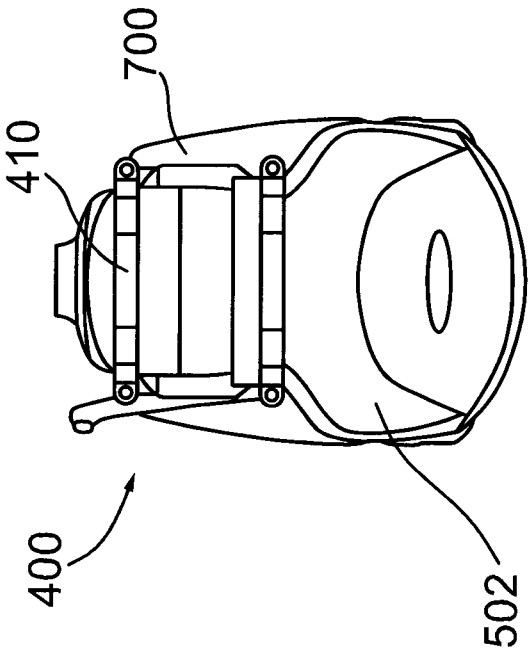


Figure 3c

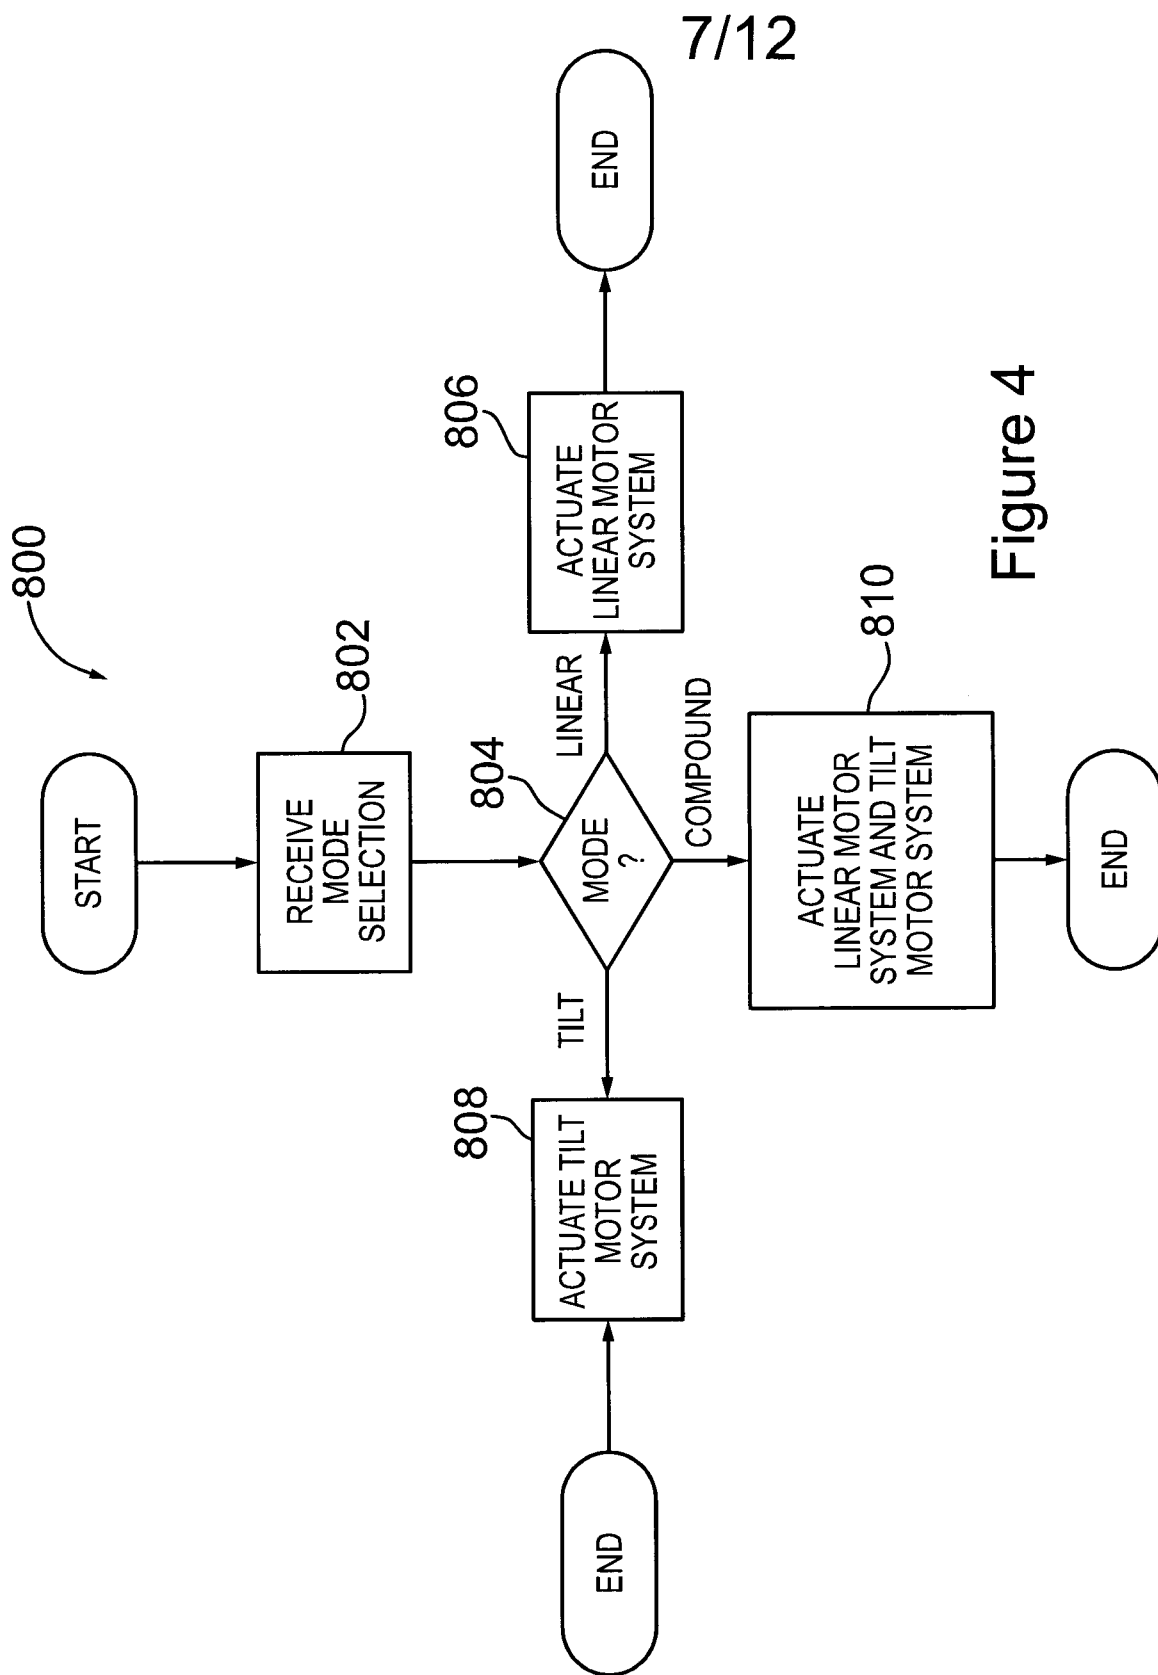

8/12

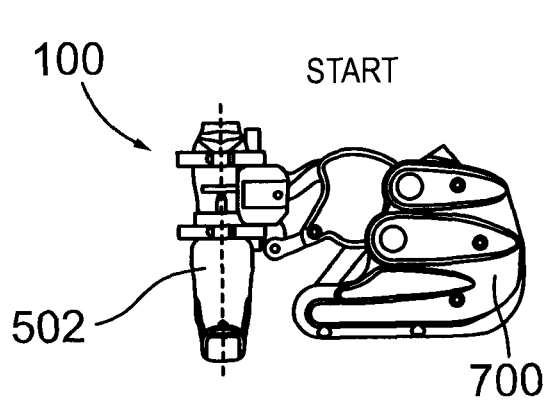


Figure 5a

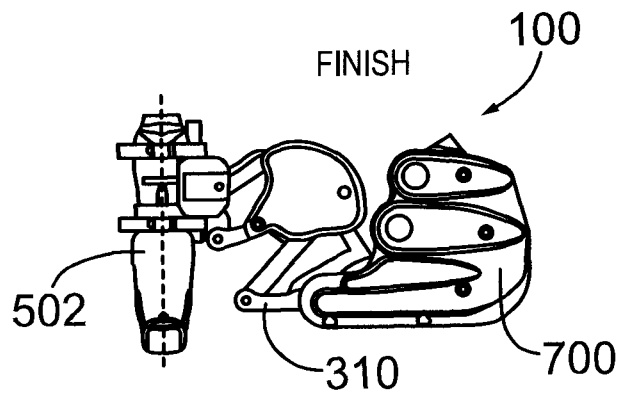


Figure 5b

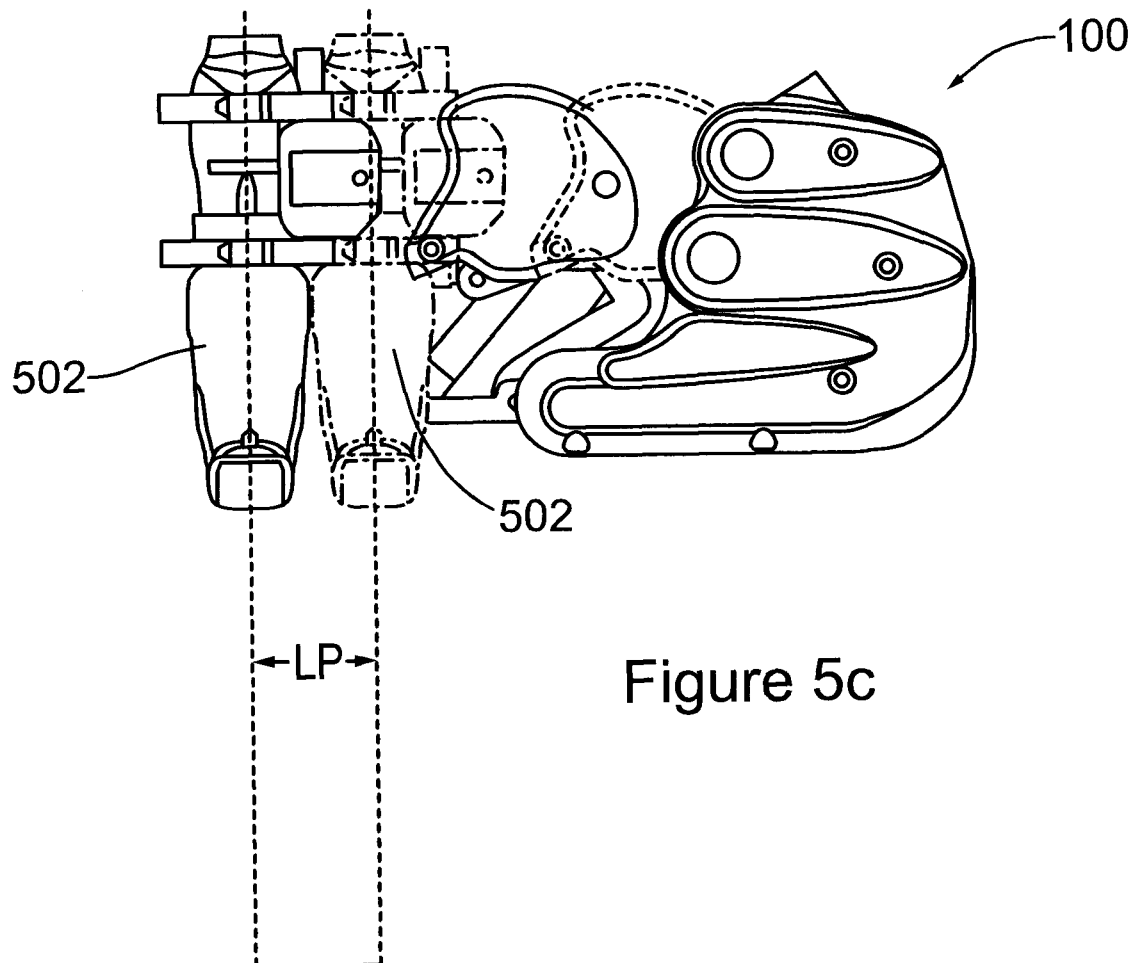


Figure 5c

9/12

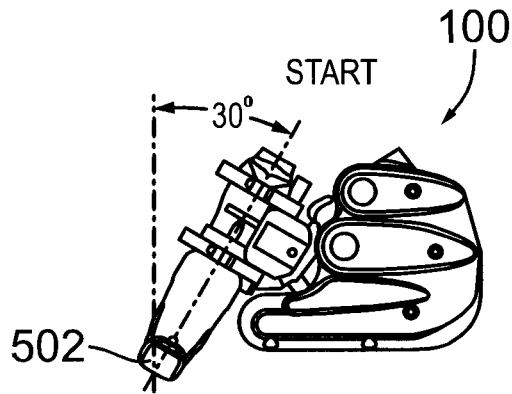


Figure 6a

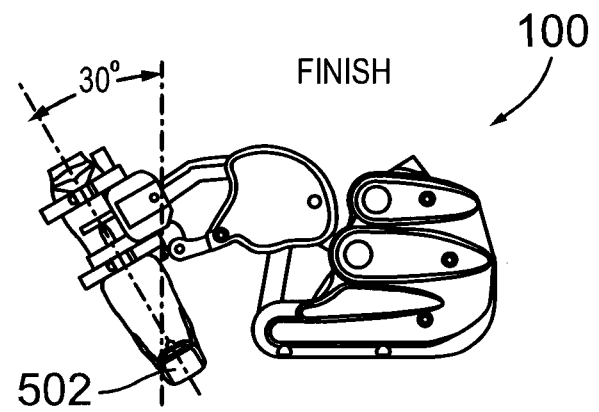


Figure 6b

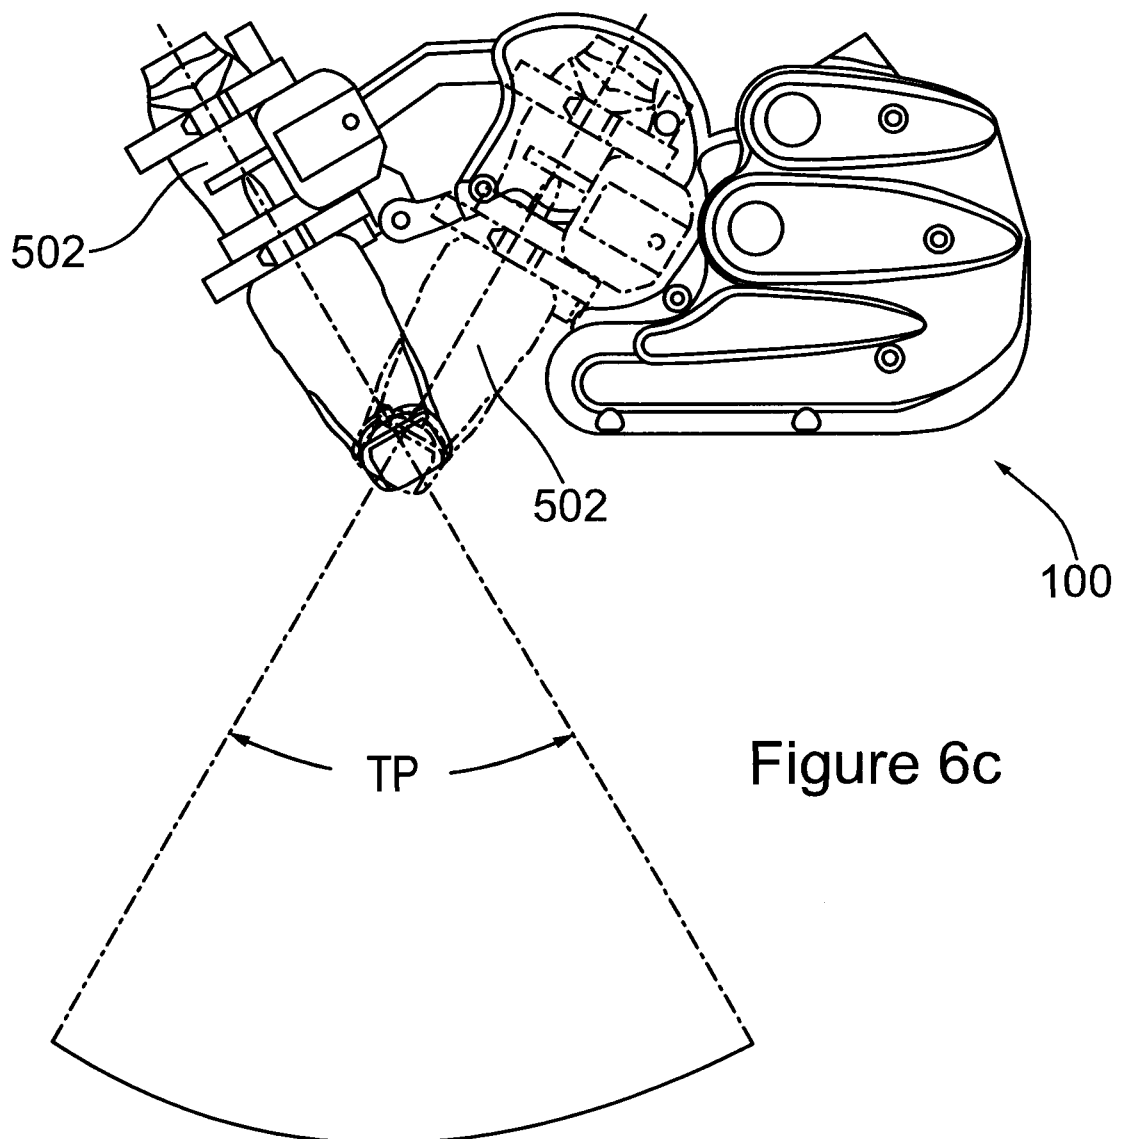


Figure 6c

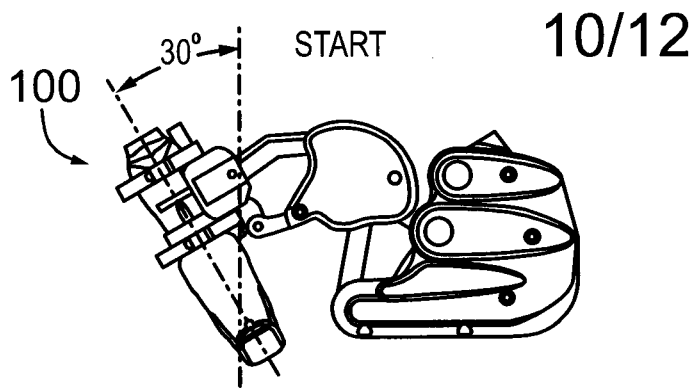


Figure 7a

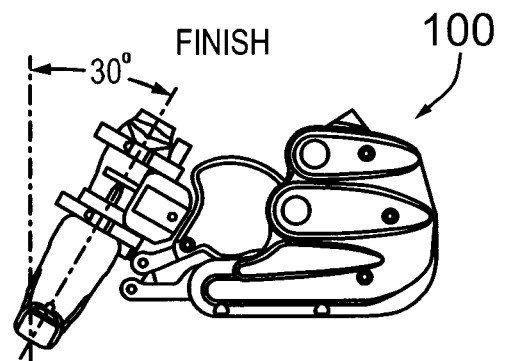


Figure 7b


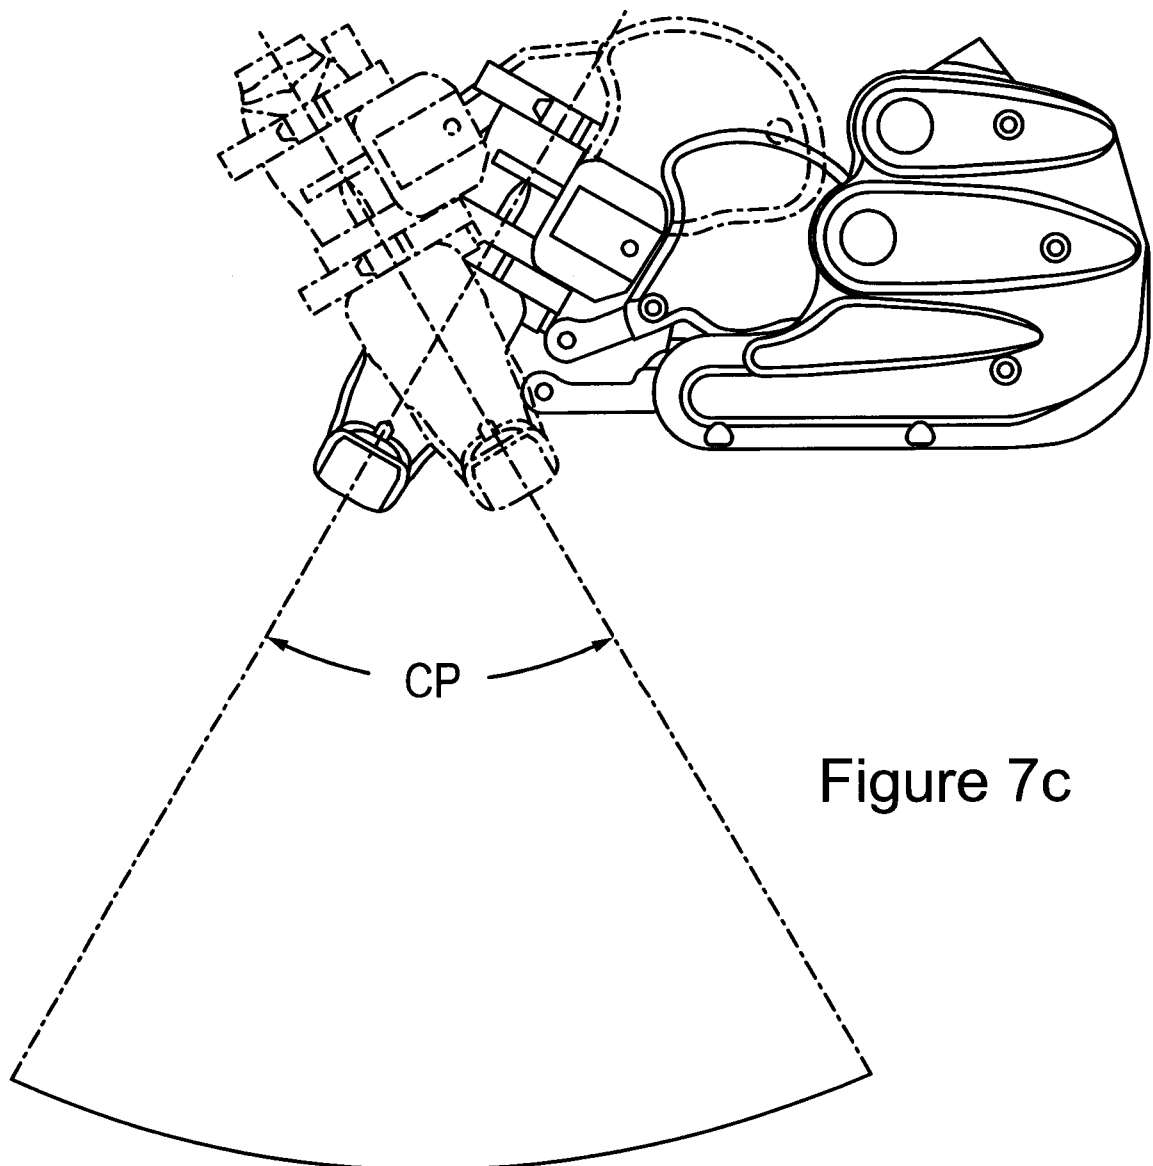


Figure 7c

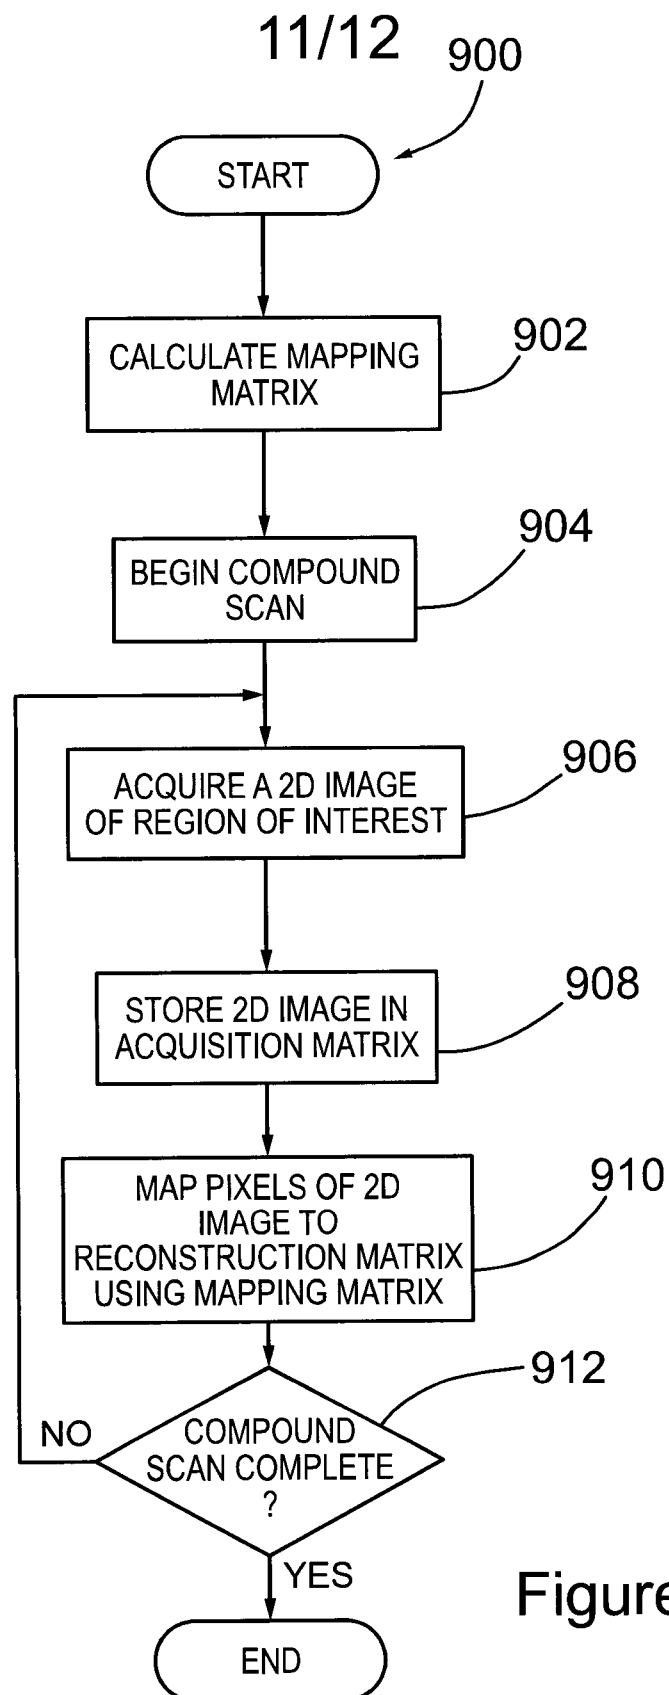

12/12

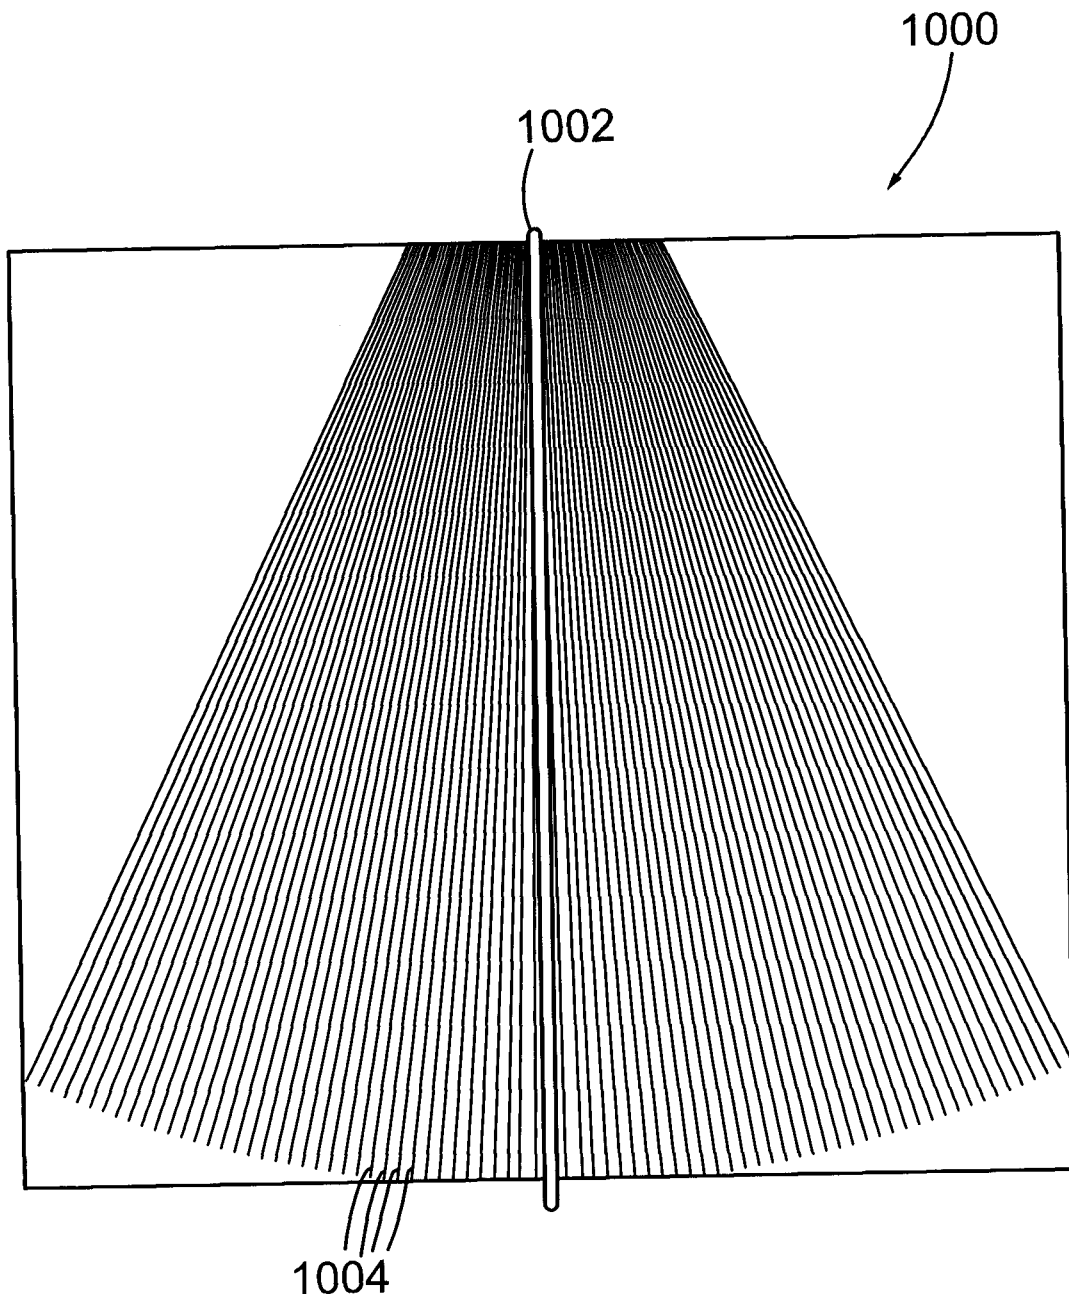


Figure 9

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CA2013/000302

A. CLASSIFICATION OF SUBJECT MATTER IPC: <i>G01N 29/44</i> (2006.01) , <i>A61B 8/00</i> (2006.01) , <i>A61B 8/14</i> (2006.01) , <i>G01N 29/265</i> (2006.01) , <i>G06T 17/00</i> (2006.01) According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) IPC: <i>G01N</i> (2006.01) , <i>A61B</i> (2006.01) , <i>G06T</i> (2006.01) (using keywords) Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used) Canadian Patent Database, Esp@cenet, TotalPatent, United States Patent Database (USPTO), Google Patents. Keywords: actuator, housing or container, motor, scan, sensor, target, ultrasound probe.		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	CA2749465 (Griffin et al.) 29 February 2012 (29-02-2012) - abstract - page 2, line 24 - page 3, line 9 - page 4, line 24 - page 10, line 11 - page 14, line 1 - page 15, line 2 - claims 1-4 - figures 2-8	1-9, 11-15
Y	US5456256 (Schneider et al.) 10 October 1995 (10-10-1995) - abstract - col. 1, line 39 - col. 2, line 18 - col. 3, lines 31-51 - col. 5, line 7 - col. 6, line 27 - col. 8, line 46 - col. 10, line 20 - col. 14, line 41 - col. 15, line 10 - claims 1, 4-7	1-9, 11-15
☒ Further documents are listed in the continuation of Box C. ☒ See patent family annex.		
* Special categories of cited documents : "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family	
Date of the actual completion of the international search 09 July 2013 (09-07-2013)	Date of mailing of the international search report 12 July 2013 (12-07-2013)	
Name and mailing address of the ISA/CA Canadian Intellectual Property Office Place du Portage I, C114 - 1st Floor, Box PCT 50 Victoria Street Gatineau, Quebec K1A 0C9 Facsimile No.: 001-819-953-2476	Authorized officer Tung Nguyen (819) 956-3859	

INTERNATIONAL SEARCH REPORTInternational application No.
PCT/CA2013/000302**Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of the first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons :

1. ☐ Claim Nos. :
because they relate to subject matter not required to be searched by this Authority, namely :
2. ☐ Claim Nos. :
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically :
3. ☐ Claim Nos. :
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows :

see extra sheet.

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claim Nos. :
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claim Nos. : 1-15

Remark on Protest ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.

☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.

☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORTInternational application No.
PCT/CA2013/000302

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO9600402 (Fenster et al.) 4 January 1996 (04-01-1996) - see entire document	1-15
A, P	CN102497131 (Hai et al.) 13 June 2012 (13-06-2012) - see entire document	1-15
A	US20090326554 (Vohra et al.) 31 December 2009 (31-12-2009) - see entire document	1-15
A	US20110152690 (Anthony et al.) 23 June 2011 (23-06-2011) - see entire document	1-15
A	US5445154 (Larson et al.) 29 August 1995 (29-08-1995) - see entire document	1-15

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/CA2013/000302

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
CA2749465A1	29 February 2012 (29-02-2012)	CA2749465A1 EP2422708A1 JP2012050824A US2012053468A1 US8409102B2	29 February 2012 (29-02-2012) 29 February 2012 (29-02-2012) 15 March 2012 (15-03-2012) 01 March 2012 (01-03-2012) 02 April 2013 (02-04-2013)
US5456256A	10 October 1995 (10-10-1995)	AT297158T BR9407982A CA2175691A1 CA2175691C CN1140982A CN1297234C DE69434400D1 EP0727963A1 EP0727963A4 EP0727963B1 JPH09507031A WO9512354A1	15 June 2005 (15-06-2005) 03 December 1996 (03-12-1996) 11 May 1995 (11-05-1995) 23 March 2010 (23-03-2010) 22 January 1997 (22-01-1997) 31 January 2007 (31-01-2007) 14 July 2005 (14-07-2005) 28 August 1996 (28-08-1996) 20 October 1999 (20-10-1999) 08 June 2005 (08-06-2005) 15 July 1997 (15-07-1997) 11 May 1995 (11-05-1995)
WO9600402A1	04 January 1996 (04-01-1996)	AT195599T AT213351T AU2730495A AU7117894A AU7615496A CA2110148A1 CA2110148C CA2193485A1 CA2193485C CA2238184A1 CA2238184C CA2277723C DE4344312A1 DE4344312C2 DE69518421D1 DE69518421T2 DE69619262D1 DE69619262T2 EP0766857A2 EP0766857B1 EP0862766A1 EP0862766B1 EP0997851A2 EP0997851A3 FR2709392A1 FR2709392B1 GB9700844D0 GB2308661A GB2308661B GB9226935D0 GB9304112D0 JPH06233765A JPH10502194A JP2000500679A US5454371A US5562095A US5842473A US5964707A	15 September 2000 (15-09-2000) 15 February 2002 (15-02-2002) 19 January 1996 (19-01-1996) 19 January 1996 (19-01-1996) 19 June 1997 (19-06-1997) 25 June 1994 (25-06-1994) 05 October 1999 (05-10-1999) 04 January 1996 (04-01-1996) 14 September 1999 (14-09-1999) 05 June 1997 (05-06-1997) 23 November 2004 (23-11-2004) 12 September 2000 (12-09-2000) 14 July 1994 (14-07-1994) 23 November 2000 (23-11-2000) 21 September 2000 (21-09-2000) 01 March 2001 (01-03-2001) 21 March 2002 (21-03-2002) 17 October 2002 (17-10-2002) 09 April 1997 (09-04-1997) 16 August 2000 (16-08-2000) 09 September 1998 (09-09-1998) 13 February 2002 (13-02-2002) 03 May 2000 (03-05-2000) 03 November 2004 (03-11-2004) 03 March 1995 (03-03-1995) 31 October 1997 (31-10-1997) 05 March 1997 (05-03-1997) 02 July 1997 (02-07-1997) 29 July 1998 (29-07-1998) 17 February 1993 (17-02-1993) 14 April 1993 (14-04-1993) 23 August 1994 (23-08-1994) 24 February 1998 (24-02-1998) 25 January 2000 (25-01-2000) 03 October 1995 (03-10-1995) 08 October 1996 (08-10-1996) 01 December 1998 (01-12-1998) 12 October 1999 (12-10-1999)

INTERNATIONAL SEARCH REPORTInternational application No.
PCT/CA2013/000302

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
		WO9600425A2 WO9600425A3 WO9720288A1	04 January 1996 (04-01-1996) 07 March 1996 (07-03-1996) 05 June 1997 (05-06-1997)
CN102497131A	13 June 2012 (13-06-2012)	None	
US2009326554A1	31 December 2009 (31-12-2009)	US2009326554A1 US7875039B2 US2009326555A1	31 December 2009 (31-12-2009) 25 January 2011 (25-01-2011) 31 December 2009 (31-12-2009)
US2011152690A1	23 June 2011 (23-06-2011)	US2011166453A1 US8328725B2 US8333704B2 US2011172541A1 US8382671B2 US2012172710A1 WO2011075713A1 WO2012094308A1	07 July 2011 (07-07-2011) 11 December 2012 (11-12-2012) 18 December 2012 (18-12-2012) 14 July 2011 (14-07-2011) 26 February 2013 (26-02-2013) 05 July 2012 (05-07-2012) 23 June 2011 (23-06-2011) 12 July 2012 (12-07-2012)
US5445154A	29 August 1995 (29-08-1995)	None	

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CA2013/000302

There are 2 inventions claimed in the international application covered by the claims indicated below:

Group A: Claims 1-15 are directed to an actuator for an ultrasound probe comprising a housing assembly and a motor assembly.

Group B: Claims 16-23 are directed to a method of reconstructing a three-dimensional ultrasound image of a target region of interest.

It is considered that **the international application does not comply with the requirements of unity of invention** (Rules 13.1, 13.2 and 13.3) since the inventions listed as Groups A and B do not relate to a single inventive concept under PCT Rule 13.1 and they lack the same or corresponding technical features under PCT Rule 13.2.

专利名称(译)	用于移动超声探头的致动器		
公开(公告)号	EP2831573A1	公开(公告)日	2015-02-04
申请号	EP2013767924	申请日	2013-03-28
[标]申请(专利权)人(译)	西安大略大学		
申请(专利权)人(译)	加拿大西安大略大学		
当前申请(专利权)人(译)	加拿大西安大略大学		
[标]发明人	BARKER KEVIN FENSTER AARON NESHAT HAMID KAKANI NIRMAL		
发明人	BARKER, KEVIN FENSTER, AARON NESHAT, HAMID KAKANI, NIRMAL		
IPC分类号	G01N29/44 A61B8/00 A61B8/14 G01N29/265 G06T17/00 A61B8/08 G01N29/22		
CPC分类号	A61B8/4461 A61B8/13 A61B8/4218 A61B8/466 A61B8/483 A61B8/5207 A61B8/5253 A61B8/54 G01N29/225 G01N29/265		
代理机构(译)	TURNER , STEPHEN		
优先权	61/617031 2012-03-28 US		
其他公开文献	EP2831573A4 EP2831573B1		
外部链接	Espacenet		

摘要(译)

用于超声探头的致动器包括：壳体组件，被配置为容纳超声探头并且被定位在待检查的目标感兴趣区域附近；以及马达组件，被联接到壳体组件，马达组件被配置为移动壳体组件。以一种方式允许超声探头在被壳体组件容纳时执行目标感兴趣区域的复合扫描。