



(43) International Publication Date
14 November 2013 (14.11.2013)

- (51) International Patent Classification:
A61B 8/00 (2006.01) *A61B 19/00* (2006.01)
A61B 8/08 (2006.01)
- (21) International Application Number:
PCT/IB2013/053615
- (22) International Filing Date:
6 May 2013 (06.05.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/645,674 11 May 2012 (11.05.2012) US
- (71) Applicant: **KONINKLIJKE PHILIPS N.V.** [NL/NL];
High Tech Campus 5, NL-5656 AE Eindhoven (NL).
- (72) Inventors: **VIGNON, Francois, Guy, Gerard, Marie**; c/o
High Tech Campus, Building 5, NL-5656 AE Eindhoven
(NL). **CHANG, Jin**; c/o High Tech Campus, Building 5,
NL-5656 AE Eindhoven (NL). **DANIELS, Allison, Ar-**
den; c/o High Tech Campus, Building 5, NL-5656 AE
Eindhoven (NL). **JAIN, Ameet, Kumar**; c/o High Tech
Campus, Building 5, NL-5656 AE Eindhoven (NL).
- (74) Agents: **STEFFEN, Thomas** et al.; High Tech Campus,
Building 5, NL-5656 AE Eindhoven (NL).
- (81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,

BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,
NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU,
RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,
ZM, ZW.

- (84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

Published:

- with international search report (Art. 21(3))

(54) Title: AN ULTRASONIC IMAGING APPARATUS AND A METHOD FOR IMAGING A SPECULAR OBJECT AND A TARGET ANATOMY IN A TISSUE USING ULTRASOUND

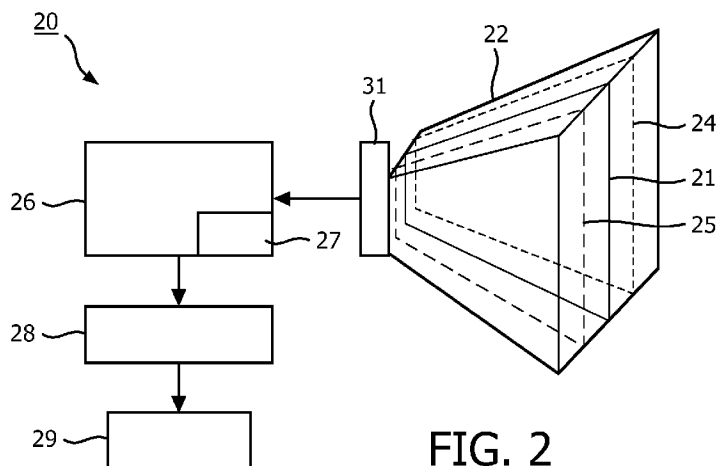


FIG. 2

(57) Abstract: The invention relates to a method and an ultrasonic imaging apparatus (20) for imaging a specular object (such as a biopsy needle) and a target anatomy in a tissue, whereby the specular object remains visible even when its location deviates from a target plane (21) including the target anatomy.

An ultrasonic imaging apparatus and a method for imaging a specular object and a target anatomy in a tissue using ultrasound

FIELD OF THE INVENTION

The invention relates to a method of imaging a specular object, such as for example a needle-like instrument, and a target anatomy in a tissue using ultrasound, the method comprising a tissue imaging step of transmitting first sound waves into a volumetric region of the tissue, the volumetric region including the target anatomy located in a target plane, of receiving echoes of said first sound waves from the target plane, and of processing said received echoes to produce a tissue image, said tissue imaging step using a tissue mode specific set of parameters, and a specular object imaging step of transmitting second sound waves into said volumetric region of the tissue, the volumetric region including the specular object, of receiving echoes of said second sound waves from the target plane, and of processing said received echoes to produce a specular object image, said specular object imaging step using a specular object mode specific set of parameters, and a display step of displaying a combined tissue image and specular object image.

The invention further relates to an apparatus implementing the method according to the invention.

More specifically the invention relates to a method of imaging a biopsy needle using ultrasound and to an ultrasonic imaging apparatus for imaging a biopsy needle.

BACKGROUND OF THE INVENTION

Ultrasound is commonly used for imaging needle insertion during interventional surgical procedures. Such needles may, for example, be paracentetic needles for withdrawal of fluid from a target anatomy in a body or biopsy needles for the removal of samples from a target anatomy in a body. Needles may also be used to administer drugs or other substances into a specific location relative to a target anatomy in the body.

During such procedures the precision of needle trajectory is highly important. The needle should not disturb or damage anatomy not connected with the procedure being undertaken. Some procedures may be directed towards small regions in the body e.g. artery or an area close to a major anatomy, such as the heart. Accuracy of needle placement is therefore vital.

Ultrasound is often used as an imaging method for imaging a needle and a target anatomy in support of the interventional procedure. Other imaging alternatives, such as Xray or EM (electromagnetic) guidance, suffer from drawbacks such as risk of radiation exposure, 2D view only, additional set-up time, tracking errors or lack of visibility of the specular object, such as a biopsy needle.

A method according to the preamble for imaging a specular needle together with a target anatomy in a tissue is described in "Enhancement of needle visibility in ultrasound-guided percutaneous procedures"; Cheung and Rohling's; *Ultr. Med. Biol.* (2004) 30: 617-624. Here the visualization of a needle in the ultrasound image is enhanced, without compromising the quality of the visualization of the target anatomy in the tissue, by displaying the combination of a specular object image (also referred to as a needle-specific image) and a tissue image. The tissue image, obtained using a tissue mode specific set of parameters, depicts the target anatomy in the tissue but may depict the needle in a poor quality, or even do not depict the needle at all, whereas the specular object image, obtained using a specular object mode specific set of parameters, depicts the needle with great contrast, but may depict almost no background tissue. Combining both images, by taking their weighted average, yield an image (often referred to as a needle-enhanced image) showing both the needle and the target anatomy.

The characteristics of the ultrasound imaging in the tissue imaging step and in the specular object imaging step are optimized to allow the best possible responses. These characteristics are set by using respectively the tissue mode specific set of parameters or the specular object mode specific set of parameters. These sets of parameters may comprise, for example, the frequency of the ultrasound waves, beam steering and beam density related parameters, the focal depth, the rate at which the echoes are received (the frame rate), and parameters controlling the type of processing of the received echoes, such as for example aperture processing and temporal filtering.

In the above described method the favored geometry for the needle to be displayed is the so-called "in-plane" geometry wherein the long axis of the needle is contained in the target plane including the target anatomy. However, in a significant number of cases the needle location deviates from the target plane due to, for example, tissue heterogeneities and bevel asymmetry.

It is now a problem of the known method that such an out-of-plane needle is not shown (or not sufficiently shown) in the combined (needle-enhanced) images. The clinician has to move the imaging transducer, transmitting and receiving the sound waves, to

locate the needle, but then loses the target anatomy located in the original target plane.

Furthermore, since the clinician does not know where the needle is located in relation to the original target plane, he has no indication how to move the transducer to find the needle.

5 SUMMARY OF THE INVENTION

It is an object of the present invention to overcome the above problems of the prior art. According to the present invention this object is achieved by providing a method according to the preamble in which the specular object imaging step is adapted i) to receive echoes of said second sound waves from a plurality of image planes, said plurality of image
10 planes separated in an elevation direction at selected elevations around the target plane, and ii) to process the echoes received from the target plane and from the plurality of image planes to produce the specular object image.

The inventors have realized that it is important to keep imaging the target plane including the target anatomy in the tissue imaging step, and at the same time image a
15 volumetric region of the tissue surrounding that target anatomy without a need to move the transducer in the specular object imaging step.

According to the invention a plurality of image planes separated in an elevation direction is acquired in the specular object imaging step using the specular object mode specific set of parameters. This gives a 3-dimensional set of (needle-specific) images.
20 From this 3-dimensional set of (needle-specific) images the specular object image is obtained providing a detailed image of the object (such as a needle) which can be pinpointed in three dimensions and quantified in length and direction.

The plurality of image planes may comprise the target plane including the target anatomy. This target plane may fall in the centre of the plurality of image planes, but
25 this is not essential. Nor it is essential to centre an apex of the elevation planes at the centre of the array transducer producing the ultrasound waves, or for the elevation planes to be parallel.

In the tissue imaging step a 2-dimensional tissue image of the target anatomy located in a target plane is obtained, while in the specular object imaging step the specular
30 object image (such a a needle) is obtained from a 3-dimensional set of (needle-specific) images. Thus the relation between them allows combining of these images to display the combined (needle-enhanced) image in which the object (such as a needle) is shown in relation to the target anatomy. Such a combined image allows the operator to see the object (such as a needle) even when it does not directly coincide with the target plane. It should be

noted that it is advantageous that these images have been obtained without moving the transducer.

In the display step the planar tissue image (showing the target anatomy) is combined with a volumetric rendering of the specular object. In this way a simultaneous display of the specular object together with the target anatomy is maintained, even when the specular object moves away from the target plane.

The data from the individual planes in the plurality of image planes may be combined by averaging to form the specular object image. However, in an embodiment a 3-dimensional segmentation algorithm is used to segment the specular object (such as a needle) out of the plurality of image planes to create a specular object image only showing that object. In a further embodiment each of the planes in the plurality of image planes are used as individual snapshots to produce separate images showing (part of) the specular object which are then fitted together in jigsaw-like fashion.

According to the invention a plurality of image planes separated in an elevation direction at selected elevations around the target plane are acquired in the specular object imaging step. It is noted that the target plane may fall in the centre of the plurality of image planes (resulting in image planes symmetrically arranged about the target plane), but that this is not essential to the present invention. The angular range of elevation of many commercially available array transducers may be as much wide as +45 to -45 degrees. If the elevation planes are parallel to each other, the lateral range spanned by all the planes may be as wide as the elevational probe footprint. According to an embodiment of the present invention a range between -10 degrees and +10 degrees in relation to the target plane is preferred. Such a range has been found to be most efficient in terms of imaging quality and imaging rate, while at the same time being large enough to capture the specular object. For the same reasons an imaging range between -15 mm to +15 mm is preferred when a plurality of parallel image planes is acquired (using, for example, a linear array transducer) in the specular object imaging step.

In a further embodiment of the present invention the image planes in the plurality of image planes are being imaged in the specular object imaging step at a lower imaging rate than the imaging rate at which the target plane is being imaged in the tissue imaging step. This allows for maintaining an optimized frame rate for displaying the combined tissue and specular object image without undue burden on the image processor hardware. The tissue image is preferably imaged at a high imaging rate to give a real-time and most detailed image of the tissue in the target plane. The specular object image needs

less detail and thus a lower imaging rate of the plurality of images from which this specular object image is derived is possible.

A further embodiment of the present invention involves multiple tissue imaging steps and multiple specular object imaging steps which are performed in an interleaved manner. This embodiment has the advantage that it reduces any temporal lag between the tissue image and the specular object image.

The object of the present invention is further achieved by providing an ultrasonic imaging apparatus for of imaging a specular object and a target anatomy in a tissue, the apparatus comprising

an array transducer for transmitting sound waves into a volumetric region of the tissue and for receiving echoes of said sound waves, said array transducer adapted to have elevation steering capabilities;
a beamformer for controlling the transmission of sound waves by the array transducer such that first sound waves are transmitted into the volumetric region including the target anatomy located in a target plane and echoes are received of said first sound waves from the target plane, and for controlling the transmission of sound waves by the array transducer such that second sound waves are transmitted into the volumetric region including the specular object and echoes are received of said second sound waves from the target plane, said beamformer adapted to control the reception of said second sound waves from a plurality of image planes, said plurality of image planes separated in an elevation direction at selected elevations around the target plane;
a data processor for processing said received echoes of said first sound waves to produce a tissue image and for processing said received echoes of said second sound waves to produce a specular object image, said data processor adapted to process the echoes received from the target plane and from the plurality of image planes to produce the specular object image; and
an image processor for displaying a combined tissue image and specular object image.

It is noted that the data processor and the image processor may be formed by dedicated hardware as well as by a generic processor implementing the required functions through appropriate firmware.

It is noted that international patent application WO 2008/126015 describes an ultrasonic diagnostic imaging system that scans a plurality of planar slices in a volumetric region which are parallel to each other. The image data of the individual slices is combined by projecting the data in the elevation dimension to produce a so-called "thick slice" image. The thick slice image is then displayed at a high frame rate by combining a single newly

acquired slice with slices previously acquired. The described method thus aims at providing, in the tissue imaging step, spatially compounded images which can be generated at a high frame rate.

5 BRIEF DESCRIPTION OF THE FIGURES

The principle of the invention and preferred embodiments thereof will be further elucidated with reference to the figures, where

Fig 1A and 1B show flowcharts of embodiments of the method according to the invention;

10 Fig 2 schematically illustrates part of an ultrasound imaging apparatus according to the invention; and

Fig 3A, 3B and 3C illustrate how the various images are obtained according to an embodiment of the invention

15 DETAILED DESCRIPTION OF THE INVENTION

Fig 1A illustrates an embodiment 10 of the method according to the invention. The embodiment 10 comprises a tissue imaging step 11 of transmitting first sound waves into a volumetric region 22, of receiving echoes of said first sound waves from a target plane 21 (said target plane including the target anatomy), and of processing said received echoes to
20 produce a tissue image. In this tissue imaging step 11 a tissue mode specific set of parameters is used, thereby ensuring the optimal imaging of the target anatomy in the tissue. The embodiment 10 further comprises a specular object imaging step 12 of transmitting second sound waves into said volumetric region 22, of receiving echoes of said second sound waves from a plurality of image planes 24, 25 separated in an elevation direction at selected
25 elevations around the target plane 21, and of processing the echoes received from the target plane and from the plurality of image planes to produce a specular object image. In this specular object imaging step 12 a specular object mode specific set of parameters is used, thereby ensuring the optimal imaging of the specular object, such as for example a needle. In a display step 13 of the embodiment 10 both the tissue image and the specular object image
30 (often referred to as a so-called needle-specific image) are combined into a single image (often referred to as a so-called needle-enhanced image) for display.

In a further embodiment the specular object imaging step 12 comprises a segmentation sub-step 121. In this segmentation sub-step the specular object is segmented

out of each individual plane of the plurality of image planes. In the specular object imaging step 12 the specular object image is then created out of the segmented individual planes.

Fig 1B illustrates an alternative embodiment 101 of the method according to the invention. This embodiment 101 comprises the tissue imaging step 11, the specular object imaging step 12 and the display step 13 as described above with reference to Fig 1A.

However, the tissue imaging step 11 and the specular object imaging step 12 are performed multiple times and in an interleaved manner, as is indicated by loop 111. First a tissue image of the target plane 21 is imaged. Next a first plurality of image planes is imaged. This first plurality of images planes consist, for example, of the three image planes around the target plane 21. Next a subsequent tissue image of the target plane 21 is imaged, after which a second plurality of image planes is imaged. This second plurality of images planes consisting, for example, of three image planes adjacent to the first plurality of image planes. This loop 111 continues until all of the planes in the plurality of images planes are imaged. It is noted that the plurality of image planes may be subdivide in alternative ways and that it is even not necessary that the planes in the plurality of images planes are imaged sequentially. In a further embodiment the tissue image of the target plane 21 is combined in display step 13 with the last available specular object image each time such a tissue image is imaged in one of the tissue imaging steps 11.

Fig 2 illustrates part of an ultrasound imaging apparatus according to the invention implementing an embodiment of the above described method according to the invention. An array transducer 31 insonifies a volumetric region 22 including a target anatomy with ultrasound. The volumetric region 22 comprises a two dimensional target plane 21 and a plurality of image planes, here illustrated by two image planes 24, 25 located immediately adjacent to and on opposite sides of the target plane 21. The incident ultrasound from the array transducer 31 is shaped and controlled by a beamformer 26. The beamformer 26 provides capability for generating a 2-dimensional tissue image of the target plane 21 by using parameters from a tissue mode specific set of parameters and capability for generating a 3-dimensional plurality of image planes 24, 25 by using parameters from a specular object mode specific set of parameters. The beamformer comprises a module 27 which provides the capability to image elevation planes, such as planes 24 and 25, at different angular and / or lateral elevations. Ultrasound returned and received by the ultrasound array transducer 31 is fed to a data processor 28 for producing a tissue image and for producing a specular object image. These two images are fed to an image processor 29 for displaying a combined tissue image and specular object image.

In an embodiment the data processor 28 is adapted to segment the specular object out of the plurality of image planes to produce a specular object image only showing that object. To this end the data processor 28 may include dedicated hardware tailored to this segmentation process.

5 Fig 3A shows an array transducer 31 and the target plane 21 and the plurality of image planes 24, 25, 34 and 35. The target plane 21 is imaged in the tissue imaging step 11 to produce the tissue image. The plurality of image planes 24, 25, 34 and 35 are imaged in the specular object imaging step 12. According to this embodiment the target plane 21 is also imaged in the specular object imaging step, now using the specular object specific set of
10 parameters. This is represented by the further image plane 36, which coincident with the target plane 21.

Fig 3B shows the array transducer 31 and the target plane 21 in relation to a needle 37. It can be seen from the figure that the needle is not aligned with the target plane 21 and does not lie completely along the target plane 21, but sits at an angle relative to it. The
15 solid line of the needle 37 is indicative of the part of the needle in front of the target plane 21, while the dashed line is indicative of the part of the needle lying behind the target plane 21.

Fig 3C illustrates the images obtained in the various steps according to the invention when visualizing such an out-of-plane needle as is depicted in Fig. 2B. In the tissue imaging step 11 a tissue image 39 of the target plane 21 is obtained. Next a plurality
20 of image planes is obtained for several elevations in the specular object imaging step 12. Here it has been chosen to have the target plane itself (represented by the further image plane 36) and three elevations in the positive angular direction and three in the negative angular direction with respect to the target plane 21. The target plane location represented by the further image plane 36 is labeled with a zero in the figure and the elevated image planes with
25 a positive or negative one, two or three. It is noted that this number of elevated image planes is merely an example and should not be construed as limiting. In display step 13 the tissue image 39 and the plurality 40 of image planes are combined into a final image 38 to be displayed. This combination can be done by overlaying the 3-dimensional image information from the plurality 40 of image planes on the 2-dimensional tissue image. Alternatively, this
30 combination can be done by first combining the 3-dimensional image information from the plurality 40 of image planes into a specular object image and subsequently overlaying this specular object image on the tissue image. The information from the individual planes in the plurality 40 of image planes may, for example, be combined by averaging to form the specular object image. It is noted that the combination of the images into a final image 38 to

be displayed is not limited to overlay techniques only, but that other techniques, including showing the tissue image and the specular object image alongside each other, may be used as well.

An embodiment of the invention involves an optional segmentation sub-step

5 121. In this sub-step a plurality 41 of segmentation images is made available over the same range as for the plurality 40 of image planes. Known segmentation algorithms can be used to segment the specular object (such as the needle in this example) out of the plurality 40 of image planes to form the plurality 41 of segmentation images. In the display step 13 the tissue image 39 and the plurality 41 of segmentation image are now combined into the final
10 image 38. Alternatively, the plurality 41 of segmentation images are combined into a specular object image only showing that object (such as the needle in this example).

As can be seen in Fig 3B the needle does not lie completely along the target plane 21, but sits at an angle relative to it. Part of the needle is in front of the target plane 21, while part of the needle is behind the target plane 21. This results in each individual image
15 plane in the plurality 40 of image planes showing (part of) the needle in a different location in said individual image plane, as is shown in FIG 3C.

In an embodiment of the invention the needle (more in general, the specular object) as shown in the combined final image 38 is coded depending on the position deviation of the individual image planes from the target plane 21. Each part of the needle
20 originating from a different individual image plane has a different coding in the reconstructed needle shown in the combined final image 38. A preferred coding technique is color coding the needle, since the use of color is easy to absorb and understand by an operator. A an example, the part of the needle shown in the combined final image 38 originating from the individual image planes in front of the target plane 21 may be colored in red while the part of
25 the needle originating from the individual image planes behind the target plane 21 may be colored in blue.

CLAIMS:

1. A method of imaging a specular object and a target anatomy in a tissue using ultrasound, the method comprising

- a tissue imaging step (11)

- of transmitting first sound waves into a volumetric region (22) of the tissue, the volumetric region including the target anatomy located in a target plane (21),

- of receiving echoes of said first sound waves from the target plane, and

- of processing said received echoes to produce a tissue image,

- said tissue imaging step using a tissue mode specific set of parameters, and

- a specular object imaging step (12)

- of transmitting second sound waves into said volumetric region of the tissue, the volumetric region including the specular object,

- of receiving echoes of said second sound waves from the target plane, and

- of processing said received echoes to produce an specular object image,

- said specular object imaging step using a specular object mode specific set of parameters, and

- a display step (13) of displaying a combined tissue image and specular object image, characterized in that

- the specular object imaging step is adapted to

- receive echoes of said second sound waves from a plurality of image planes (24, 25), said plurality of image planes separated in an elevation direction at selected elevations around the target plane (21), and

- to process the echoes received from the target plane and from the plurality of image planes to produce the specular object image.

2. A method as claimed in claim 1, wherein the specular object imaging step is further adapted to segment the specular object out of each individual plane of the plurality of image planes, and to create the specular object image out of the thus segmented individual planes.

3. A method as claimed in claim 1, comprising at least two tissue imaging steps (11) and a least two specular object imaging steps (12), wherein the tissue imaging steps are performed interleaved with the specular object imaging steps.

5

4. An ultrasonic imaging apparatus (20) for imaging a specular object and a target anatomy in a tissue, the apparatus comprising

- an array transducer (31) for transmitting sound waves into a volumetric region (22) of the tissue and for receiving echoes of said sound waves;

10 -a beamformer (26) for controlling the transmission of sound waves by the array transducer such that first sound waves are transmitter into the volumetric region including the target anatomy located in a target plane (21) and echoes are received of said first sound waves from the target plane, and for controlling the transmission of sound waves by the array transducer such that second sound waves are transmitter into the volumetric region including the

15 specular object and echoes are received of said second sound waves from the target plane;
- a data processor (28) for processing said received echoes of said first sound waves to produce a tissue image and for processing said received echoes of said second sound waves to produce a specular object image; and

-an image processor (29) for displaying a combined tissue image and specular object image;
20 characterized in that

- the array transducer (31) is adapted to have elevation steering capabilities,

- the beamformer (26) is adapted to control the reception of said second sound waves from a plurality of image planes(24,25), said plurality of image planes separated in an elevation direction at selected elevations around the target plane (21), and

25 - the data processor (28) is adapted to process the echoes received from the target plane and from the plurality of image planes to produce the specular object image.

5. An ultrasonic imaging apparatus as claimed in claim 4, wherein the data processor (28) is further adapted to segment the specular object out of the plurality of image
30 planes.

1/4

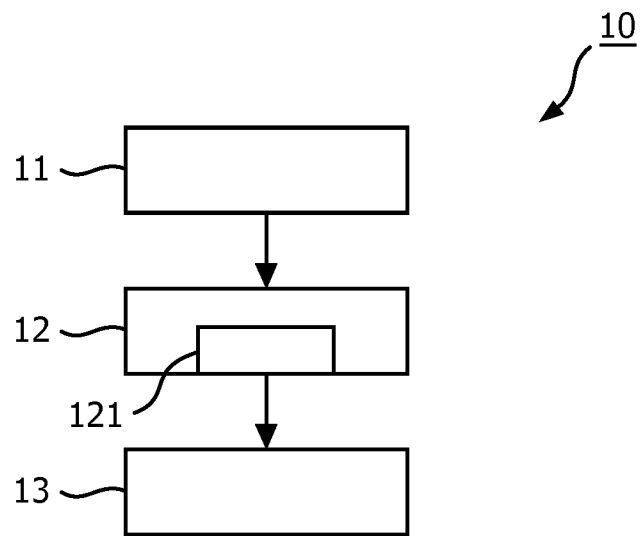


FIG. 1A

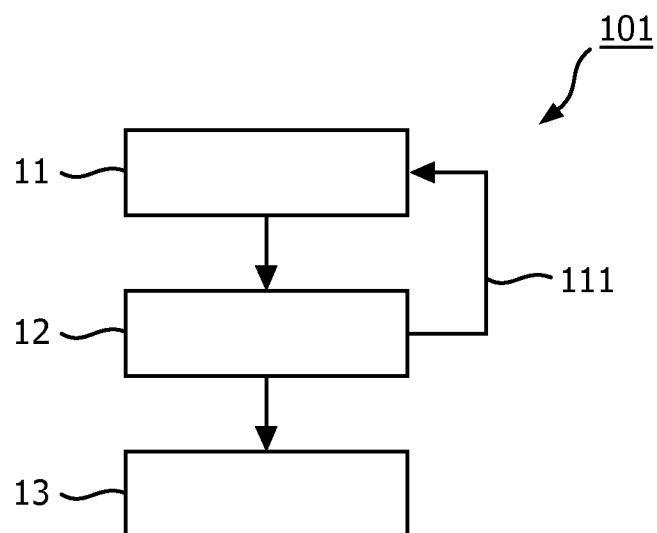


FIG. 1B

2/4

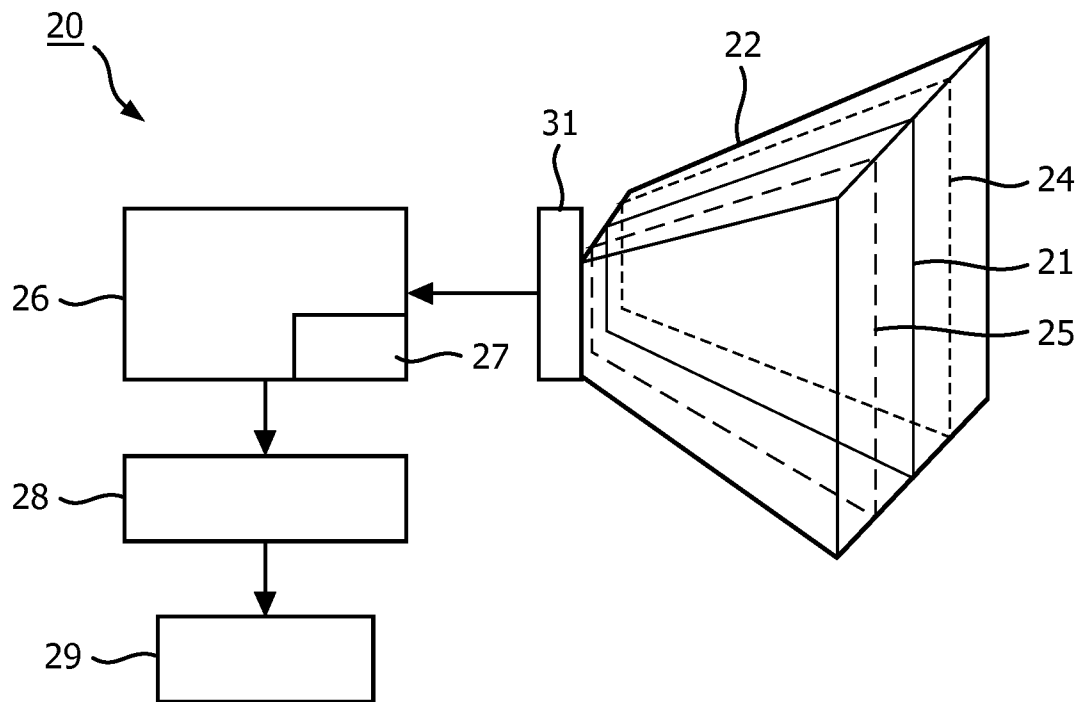


FIG. 2

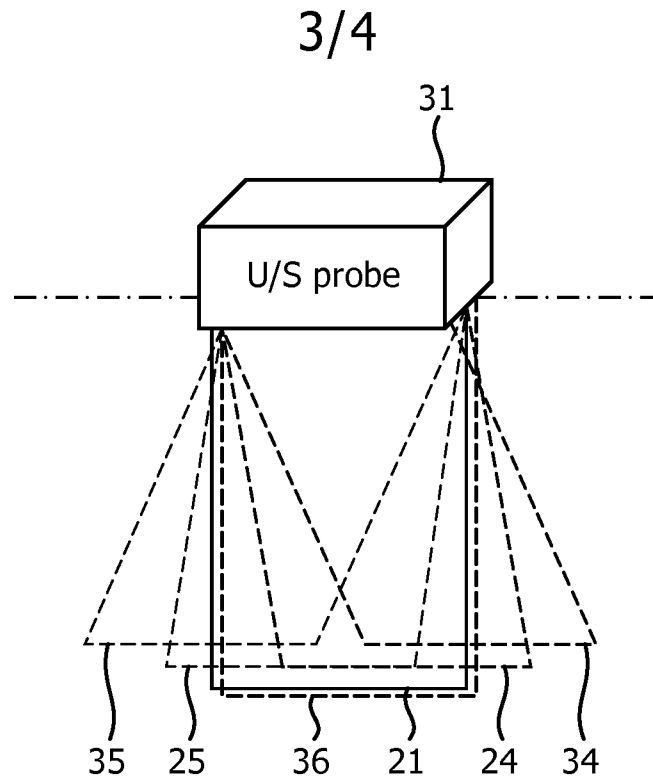


FIG. 3A

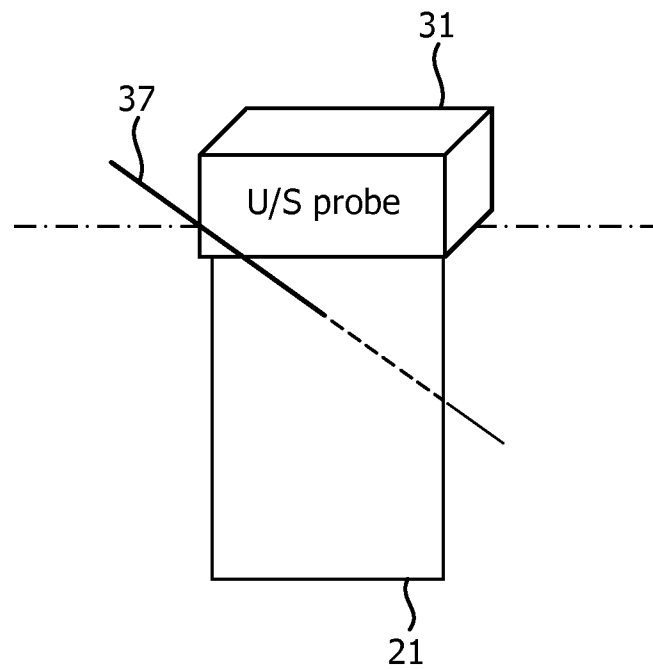


FIG. 3B

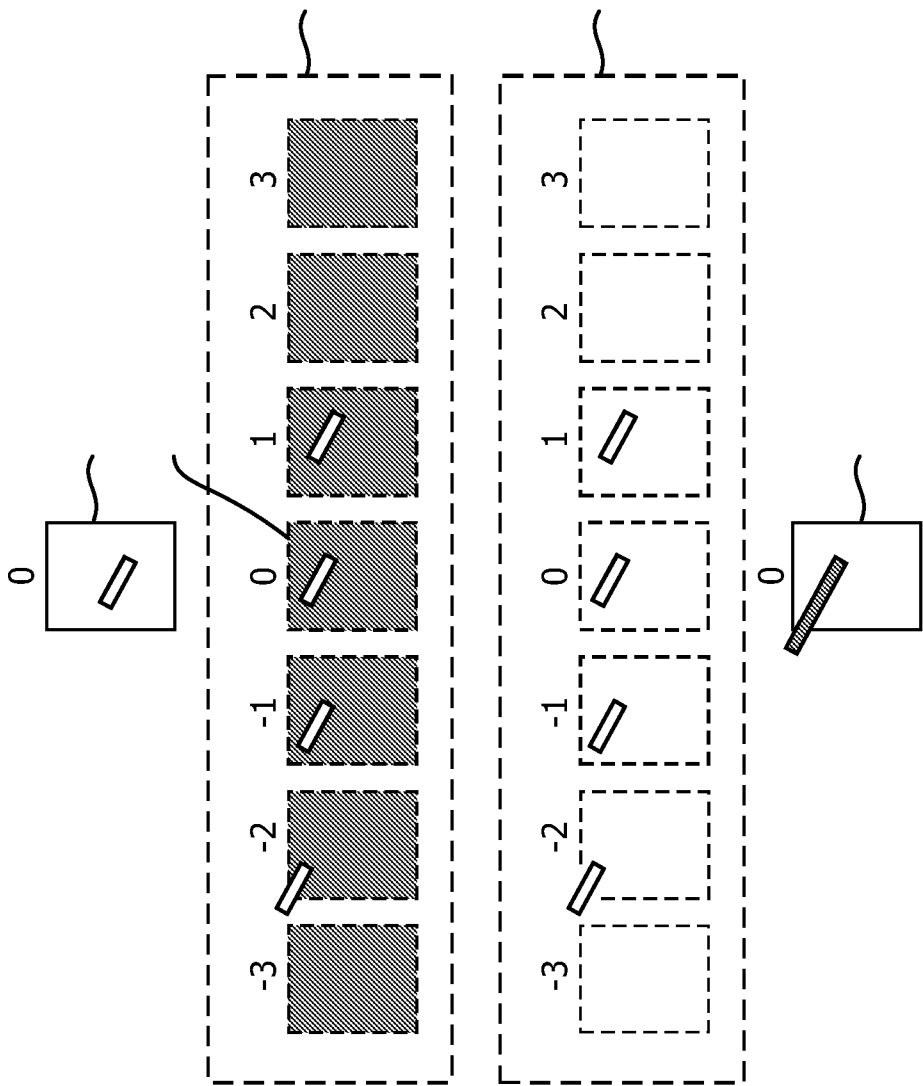


FIG. 3C

INTERNATIONAL SEARCH REPORT

International application No

PCT/IB2013/053615

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61B8/00 A61B8/08 A61B19/00
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 1 281 368 A2 (ESAOTE SPA [IT]) 5 February 2003 (2003-02-05) abstract figure 1 paragraph [0047] - paragraph [0072] -----	1,3,4
X	US 2002/173719 A1 (ZHAO DANHUA [US] ET AL) 21 November 2002 (2002-11-21) abstract figures 1-8 paragraph [0026] - paragraph [0053] -----	1,2,4,5



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

7 August 2013

Date of mailing of the international search report

19/08/2013

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Moehrs, Sascha

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/IB2013/053615

Patent document cited in search report	Publication date	Patent family member(s)	Publication date	
EP 1281368	A2	05-02-2003	EP 1281368 A2	05-02-2003
			IT SV20010025 A1	30-12-2002

US 2002173719	A1	21-11-2002	NONE	

专利名称(译)	一种超声成像设备和使用超声波对组织中的镜面物体和目标解剖结构成像的方法		
公开(公告)号	EP2846697A1	公开(公告)日	2015-03-18
申请号	EP2013729463	申请日	2013-05-06
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	VIGNON FRANCOIS GUY GERARD MARIE CHANG JIN DANIELS ALLISON ARDEN JAIN AMEET KUMAR		
发明人	VIGNON, FRANCOIS, GUY, GERARD, MARIE CHANG, JIN DANIELS, ALLISON, ARDEN JAIN, AMEET, KUMAR		
IPC分类号	A61B8/00 A61B8/08 A61B19/00		
CPC分类号	A61B8/0841 A61B8/14 A61B8/4416 A61B8/463 A61B8/466 A61B8/483 A61B8/523 A61B8/5246 A61B2034/2063 A61B2090/378 G06T2207/10132 G06T2207/30004 G09G5/38 G09G2340/12		
代理机构(译)	STEFFEN , THOMAS		
优先权	61/645674 2012-05-11 US		
外部链接	Espacenet		

摘要(译)

本发明涉及一种用于对组织中的镜面对象（例如活检针）和目标解剖结构进行成像的方法和超声成像设备（20），由此镜面对象即使在其位置偏离目标平面时也保持可见（21）包括目标解剖结构。