




- (51) International Patent Classification:  
A61B 8/12 (2006.01) A61B 8/00 (2006.01)
- (21) International Application Number:  
PCT/US2017/016471
- (22) International Filing Date:  
3 February 2017 (03.02.2017)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
15/063,654 8 March 2016 (08.03.2016) US
- (71) Applicant: COVIDIEN LP [US/US]; 15 Hampshire Street, Mansfield, Massachusetts 02048 (US).
- (72) Inventors: JASPERSON, Keith E.; 13993 Magnolia Street NW, Andover, Minnesota 55304 (US). CHRISTMANN, H. Aaron; 4356 Cottage Park Road, White Bear Lake, Minnesota 55110 (US). WEISENBERGER, Michael R.; 2944 Zarthan Avenue South, Minneapolis, Minnesota 55416 (US).
- (74) Agent: BELENCHIA, Giordana M.; Medtronic, IP Legal, 5920 Longbow Drive, A36, Boulder, Colorado 80301 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:  
— with international search report (Art. 21(3))

(54) Title: SURGICAL TOOL WITH FLEX CIRCUIT ULTRASOUND SENSOR

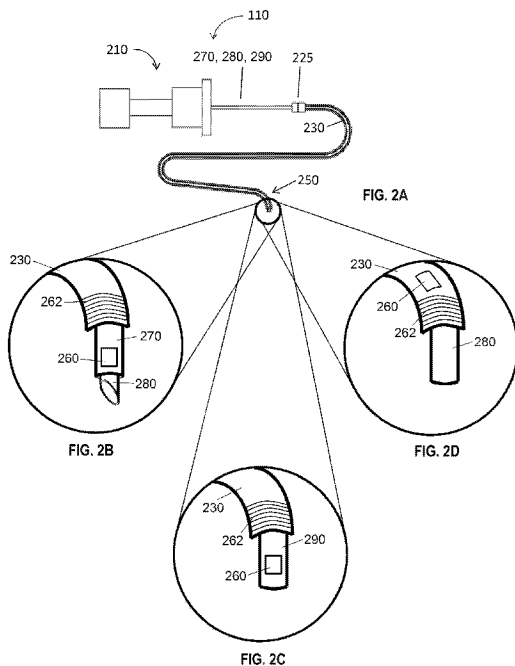

(57) Abstract: A medical instrument includes a printed ultrasound sensor, a surface, at least one non-conductive material, and at least one pair of contacts. The ultrasound sensor includes an array of ultrasound transducers printed on a non-conductive surface of the medical instrument. The medical instrument contains multiple conductive and nonconductive layers. The at least one pair of contacts are electrically coupled to the ultrasound sensor and operably coupled to the conductive layer, the conductive layer coupled to a measurement device, which converts electrical signals from the ultrasound sensor into images displayed on a display unit. The location of the medical instrument can be visualized in real time on the display unit.



**SURGICAL TOOL WITH FLEX CIRCUIT ULTRASOUND SENSOR****BACKGROUND****Technical Field**

[0001] The present disclosure relates to a medical instrument including an ultrasound sensor. More particularly, the present disclosure relates to systems and methods that confirm a location of a medical instrument having an ultrasound transducer.

**Discussion of Related Art**

[0002] Electromagnetic navigation (EMN) has helped expand the possibilities of treatment to internal organs and diagnosis of diseases. EMN relies on non-invasive imaging technologies, such as computed tomography (CT) scanning, magnetic resonance imaging (MRI), or fluoroscopic technologies. These images may be registered to a location of a patient within a generated magnetic field, and as a result the location of a sensor placed in that field can be identified with reference to the images. As a result, EMN in combination with these non-invasive imaging technologies is used to identify a location of a target and to help clinicians navigate inside of the patient's body to the target.

[0003] In one particular example of currently marketed systems in the area of locating the position of medical instruments in a patient's airway, a sensor is placed at the end of a probe referred to as a locatable guide and passed through an extended working channel (EWC) or catheter, and the combination is inserted into the working channel of a bronchoscope. The EWC and probe with the sensor is then navigated to the target within the patient. Once the target is reached, the locatable guide (i.e., sensor and probe) can be removed and one or more instruments, including biopsy needles, biopsy brushes, ablation catheters, and the like can be passed through the working channel and EWC to obtain samples and/or treat the target. At this point, however, because the locatable guide with the sensor has been removed, the exact location of a distal end of the EWC, and by

extension any instrument which might be passed there through is not precisely known. In addition, the precise location within the target tissue is not entirely clear.

[0004] Images generated by the non-invasive imaging technologies described above do not provide the resolution of live video imaging. To achieve live video, a clinician may utilize the features of an endoscope. However, an endoscope is limited by its size and as a result cannot be navigated to the pleura boundaries of the lungs and other very narrow passageways as is possible with tools typically utilized in EMN. An alternative is a visualization instrument that is inserted through the EWC and working channel of the endoscope, which can be sized to reach areas such as the pleura boundaries.

[0005] As with the locatable guide, however, once the visualization instrument is removed the location of the distal end of the EWC is unclear. One technique that is used is the placement of one or more markers into the tissue near the target and the use of fluoroscopy to confirm location of the EWC and the markers, and any subsequent instruments passed through the EWC. Due to the small diameter of the EWC, simultaneous insertion of more than one instrument may be impractical. Thus, repeated insertions and removals of instruments for visualization, diagnosis, and surgeries are necessitated. Such repeated insertions and removals lengthen diagnostic or surgical time and efforts, and increase costs on patients correspondingly. Thus, it is desirable to make a fewer insertion and/or removal of instruments to shorten times necessary for diagnosis and surgeries while at the same time increasing the certainty of the location of the EWC and instruments passed through the EWC, including imaging modalities.

## SUMMARY

[0006] Provided in accordance with the present disclosure is a medical instrument including a printed ultrasound sensor. In particular, the medical instrument includes a conductive layer printed circumferentially around at least a portion of a catheter and a

nonconductive layer printed on top of the conductive layer. An ultrasound sensor is printed on a distal portion of the nonconductive layer. The ultrasound sensor is adapted to transmit and receive signals. At least one pair of vias are formed in the conductive layer and nonconductive layer and enable an electrical connection between the ultrasound sensor and the conductive layer. In embodiments, the conductive layer is copper, silver, gold, conductive alloys, or conductive polymer. The medical instrument also includes a connector formed on a proximal end of the catheter for connection to an ultrasound image resolution device.

[0007] According to aspects of the disclosure, the medical instrument also includes an electromagnetic sensor disposed on a distal portion of the catheter. The medical instrument further includes a base non-conductive layer on the distal portion of the medical instrument on which the electromagnetic sensor is printed.

[0008] In embodiments, the ultrasound sensor includes an array of ultrasound transducers. The ultrasound transducers are formed of piezoelectric material. In embodiments, the ultrasound transducers are made at least in part of silicon diaphragms, wherein the piezoelectric material is printed on the silicon diaphragms. The piezoelectric material may be perovskite phase lead zirconate titanate (PZT), quartz, lead titanate, barium titanate, or polyvinylidene fluoride (PVDF). In embodiments, the array of ultrasound transducers are printed in parallel rows of ultrasound transducers.

[0009] In another embodiment, the medical instrument is an extended working channel, a biopsy forceps, a biopsy brush, a biopsy needle, or a microwave ablation probe. In further embodiments, the medical instrument includes an outer surface formed of ethylene tetrafluoroethylene (ETFE), polytetrafluoroethylene (PTFE), polyimide, or non-conductive polymer.

[0010] According to aspects of the disclosure, the ultrasound sensor, conductive layer, and the non-conductive layer are printed using drop-on-demand (DOD) or ink-jet printing. Additionally, the electromagnetic sensor is printed on a distal portion of the medical instrument.

[0011] In another embodiment, the electromagnetic sensor includes at least one pair of contacts electrically connected to the electromagnetic sensor, wherein at least one pair of contacts is coupled to the conductive layer. According to aspects of the disclosure, the conductive layer is connectable to a measurement device configured to sense an induced electrical signal based on a magnetic flux change of an electromagnetic field, wherein a location of the medical instrument in a coordinate system of the electromagnetic field is identified based on the induced electrical signal in the electromagnetic sensor.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

[0012] Objects and features of the presently disclosed systems and methods will become apparent to those of ordinary skill in the art when descriptions of various embodiments are read with reference to the accompanying drawings, of which:

[0013] FIG. 1 is a perspective schematic view of a system for identifying a location of a medical instrument in accordance with an embodiment of the present disclosure;

[0014] FIG. 2A is a schematic view of a catheter guide assembly and medical instrument in accordance with the present disclosure;

[0015] FIG. 2B is an enlarged view of one embodiment of the indicated area of detail of FIG. 2A;

[0016] 2C is an enlarged view of another embodiment of the indicated area of detail of FIG. 2A;

[0017] 2D is an enlarged view of yet another embodiment of the indicated area of detail of FIG. 2A;

[0018] FIG. 3 depicts a partial perspective view, which illustrates one embodiment of an ultrasound sensor printed at the distal portion of a medical instrument in accordance with an embodiment of the present disclosure;

[0019] FIG. 4 is a partial perspective side view of an illustrative design of a proximal portion of a medical instrument around which a series of conductive and nonconductive layers are printed;

[0020] FIGS. 5A-5D are partial side views of a plurality of medical instruments in accordance with an embodiment of the present disclosure;

[0021] FIG. 6 is schematic illustration of a printer that prints an ultrasound sensor on a surface of a medical instrument in accordance with an embodiment of the present disclosure; and

[0022] FIG. 7 is a flowchart of a method for printing an ultrasound sensor on a medical instrument in accordance with an embodiment of the present disclosure.

### **DETAILED DESCRIPTION**

[0023] The present disclosure is related to medical instruments, systems and methods for identifying a location of medical instruments by using an ultrasound sensor. The ultrasound sensor may be printed directly on or separately fabricated and then affixed to the medical instruments. Since the ultrasound sensor may be inserted inside of patient's body with medical instruments, the location of the medical instrument can be determined in real-time. Further, the sensor may work in conjunction with and/or supplement other imaging modalities. Due to the small size of the ultrasound sensor, medical instruments may incorporate the sensor within the medical instruments, to facilitate continuous navigation. Although the present disclosure will be described in terms of specific

illustrative embodiments, it will be readily apparent to those skilled in this art that various modifications, rearrangements, and substitutions may be made without departing from the spirit of the present disclosure. The scope of the present disclosure is defined by the claims appended to this disclosure.

[0024] As used herein, the term “distal” refers to the portion that is being described which is further from a user, while the term “proximal” refers to the portion that is being described which is closer to a user. Further, to the extent consistent, any of the aspects and features detailed herein may be used in conjunction with any or all of the other aspects and features detailed herein.

[0025] FIG. 1 illustrates one illustrative embodiment of a system and method for identifying a location of medical instruments in an electromagnetic field. In particular, an electromagnetic navigation (EMN) system 100, which is configured to utilize CT, MRI, or fluoroscopic images, is shown. One such EMN system may be the ELECTROMAGNETIC NAVIGATION BRONCHOSCOPY<sup>®</sup> system currently sold by Medtronic Inc. The EMN system 100 includes a catheter guide assembly 110, a bronchoscope 115, a computing device 120, a monitoring device 130, an electromagnetic (EM) board 145, a tracking device 160, and reference sensors 170. The bronchoscope 115 is operatively coupled to the computing device 120 and the monitoring device 130 via a wired connection (as shown in FIG. 1) or wireless connection (not shown).

[0026] FIG. 2A illustrates a schematic illustration of the catheter guide assembly 110 of FIG. 1. The catheter guide assembly 110 includes a control handle 210, which enables advancement and steering of the distal end 250 of the catheter guide assembly 110. The catheter guide assembly 110 may include a catheter 270 inserted in the EWC 230, as shown in FIG. 2B, a locatable guide catheter (LG) 290 inserted in the EWC 230, as

shown in FIG. 2C, or a medical instrument 280 inserted in the EWC 230, as shown in FIG. 2D. The catheter 270 may further be configured to receive a medical instrument 280.

[0027] In embodiments, the EM sensor 262 can be directly integrated into the distal end of the catheter 270, LG 290, or the EWC 230, as depicted in FIGS. 2B-2D, respectively. In all three embodiments shown in FIGS. 2B-2D, the catheter guide assembly 110 contains an ultrasound sensor (US) 260 at its distal end. Alternatively, in some embodiments, the US sensor 260 may be integrated into the distal end of the catheter 270 or directly on the medical instrument 280. A locking mechanism 225 may secure the catheter 270, the LG 220, or the medical instrument 280 to the EWC 230. The locking mechanism 225 allows a user to know the rotational orientation of the catheter 270, the LG 220, or the medical instrument 280 in addition to its 3-dimensional position. Catheter guide assemblies usable with the instant disclosure may be currently marketed and sold by Medtronic Inc. under the name SUPERDIMENSION<sup>®</sup> Procedure Kits and EDGE<sup>™</sup> Procedure Kits.

[0028] For a more detailed description of the catheter guide assemblies, reference is made to commonly-owned U.S. Patent Application Publication Number 2014/0046315 filed on March 15, 2013, by Ladtkow et al. and U.S. Patent No. 7,233,820, the entire contents of which are incorporated in this disclosure by reference. As will be described in greater detail below, the EM sensor 262 on the distal portion of the LG 290 or EWC 230 senses the electromagnetic field, and is used to identify the location of the LG 290 or EWC 230 in the electromagnetic field, and the US sensor 260 may be used to image the target and confirm the position of the EWC 230, LG 290, and/or the medical instrument 280.

[0029] In use, the bronchoscope 115 is inserted into the mouth or through an incision of a patient 150 to capture images of the internal organ. In one embodiment of

the EMN system 100, inserted into the bronchoscope 115 is a catheter guide assembly 110 for achieving an access to the lung of the patient 150. The catheter guide assembly 110 may include an extended working channel (EWC) 230 into which a catheter 270 or LG 290 with the EM sensor 262 at its distal portion is inserted. Alternatively, the EWC 230 may have an EM sensor 262 integrated at its distal portion. The EM sensor 262 is used to navigate the EWC 230 through the lung described in greater detail below. Additionally, an US sensor 260 may be integrated at a distal portion of the EWC 230 (as shown in FIGS. 2B-2D) and/or the catheter 270 (not shown) and is used to provide differential imaging information of the surrounding tissue.

[0030] In an alternative embodiment, instead of a bronchoscope 115 inserted via a natural orifice, the catheter guide assembly 110 is inserted into the patient 150 via an incision. The catheter guide assembly 110 including the EWC 230 may be inserted through the incision to navigate any luminal network including the airways of a lung and a cardiac luminal network.

[0031] The computing device 120, such as, a laptop, desktop, tablet, or other similar computing device, includes a display 122, one or more processors 124, memory 126, a network card 128, and an input device 129. The EMN system 100 may also include multiple computing devices, wherein the separate computing devices are employed for planning, treatment, visualization, and other aspects of assisting clinicians in a manner suitable for medical operations. The display 122 may be touch-sensitive and/or voice-activated, enabling the display 122 to serve as both input and output devices. The display 122 may display two dimensional (2D) images or a three dimensional (3D) model of an internal organ, such as the lung, prostate, kidney, colon, liver, etc., to locate and identify a portion of the internal organ that displays symptoms of diseases.

[0032] The display 122 may further display options to select, add, and remove a target to be treated and settable items for the visualization of the internal organ. In an aspect, the display 122 may also display the location of the catheter guide assembly 110 in the electromagnetic field based on the 2D images or 3D model of the internal organ. In another aspect, the display 122 may also display a live ultrasound image captured by the US sensor 260. This live ultrasound image may be superimposed over the 2D images or 3D model of the organs or over a virtual bronchoscopy image, or over a fluoroscopy image, or it may be displayed in a side-by-side configuration. In another embodiment, a separate display 122 may be used to display the ultrasound image.

[0033] The one or more processors 124 execute computer-executable instructions. The processors 124 may perform image-processing functions so that the 3D model of the internal organ and/or the ultrasound image can be displayed on the display 122. In embodiments, the computing device 120 may further include a separate graphic accelerator (not shown) that performs only the image-processing functions so that the one or more processors 124 may be available for other programs. The memory 126 stores data and programs. For example, data may be image data for the 3D model, ultrasound imaging, or any other related data such as patients' medical records, prescriptions and/or history of the patient's diseases.

[0034] One type of program stored in the memory 126 is a 3D model and pathway planning software module (planning software). An example of the 3D model generation and pathway planning software may be the EMN planning software currently sold by Medtronic Inc. When image data of a patient, which is typically in digital imaging and communications in medicine (DICOM) format, from for example a CT image data set (or an image data set by other imaging modality) is imported into the planning software, a 3D model of the internal organ is generated. In an aspect, imaging may be done by CT

imaging, magnetic resonance imaging (MRI), functional MRI, X-ray, and/or any other imaging modalities. To generate the 3D model, the planning software employs segmentation, surface rendering, and/or volume rendering. The planning software then allows for the 3D model to be sliced or manipulated into a number of different views including axial, coronal, and sagittal views that are commonly used to review the original image data. These different views allow the user to review all of the image data and identify potential targets in the images.

[0035] Once a target is identified, the software enters into a pathway planning module. The pathway planning module develops a pathway plan to achieve access to the targets and the pathway plan pin-points the location and identifies the coordinates of the target such that they can be arrived at using the EMN system 100, and particularly the catheter guide assembly 110 together with the EWC 230 and the LG 290,. The pathway planning module guides a clinician through a series of steps to develop a pathway plan for export and later use during navigation to the target in the patient 150. The term, clinician, may include doctor, surgeon, nurse, medical assistant, or any user of the pathway planning module involved in planning, performing, monitoring and/or supervising a medical procedure.

[0036] Details of these processes and the pathway planning module can be found in U.S. Patent Application Publication Number 2014/0281961 filed by Medtronic Inc. on June 21, 2013, and entitled "Pathway Planning System and Method," the entire contents of which are incorporated in this disclosure by reference. Such pathway planning modules permit clinicians to view individual slices of the CT image data set and to identify one or more targets. These targets may be, for example, lesions or the location of a nerve which affects the actions of tissue where the disease has rendered the internal organ's function compromised.

[0037] The memory 126 may store navigation and procedure software which interfaces with the EMN system 100 to provide guidance to the clinician and provide a representation of the planned pathway on the 3D model and 2D images derived from the 3D model. An example of such navigation software is the ILOGIC<sup>®</sup> navigation and procedure suite sold by Medtronic, Inc. In practice, the location of the patient 150 in the EM field generated by the EM field generating device 145 must be registered to the 3D model and the 2D images derived from the 3D model. Such registration may be manual or automatic and is described in detail and commonly assigned U.S. Patent Application No. 14/753,288 entitled "System and method for navigating within the lung," the entire contents of which are incorporated in this disclosure by reference.

[0038] As shown in FIG. 1, the patient surface or bed 140 is configured to provide a flat surface for the patient to lie down and includes an EM field generating device 145. When the patient 150 lies down on the EM board 145, the EM field generating device in the EM board 145 generates an EM field sufficient to surround a portion of the patient 150. The EM sensor 262 at the end of the LG 290 is used to determine the location of the distal end of the LG 290 and therewith the EWC 230 within the patient. In an aspect, a separate EM sensor 262 may be located at the distal end of the EWC 230 and therewith the exact location of the EWC 230 in the EM field generated by the EM field generating device 145 can be identified within the patient 150.

[0039] In yet another aspect, the EM board 145 may be configured to be operatively coupled with the reference sensors 170 which are located on the chest of the patient 150. The reference sensors 170 move up following the chest while the patient 150 is inhaling and move down following the chest while the patient 150 is exhaling. The movement of the chest of the patient 150 in the EM field is captured by the reference sensors 170 and transmitted to the tracking device 160 so that the breathing pattern of the

patient 150 may be recognized. The tracking device 160 also receives the output of the EM sensor 262, combines both outputs, and compensates the breathing pattern for the location of the EM sensor 262. In this way, the location identified by the EM sensor 262 may be compensated for such that the compensated location of the EM sensor 262 may be synchronized with the 3D model of the internal organ. As noted above, however, the use of an LG 290 with an EM sensor 262 at its distal end 250 can result in challenges surrounding instrument swaps, loss of location information, and a general prolongation of the time needed for a procedure. To alleviate these issues, the EM sensor 262 may be printed directly on the distal portion of a medical instrument 280 or the EWC 230 as described in U.S. Provisional Patent Application No. 62/170,383 filed by Medtronic Inc. on June 3, 2015, and entitled "Medical Instrument with Sensor for use in a System and Method for Electromagnetic Navigation," the entire contents of which are incorporated in this disclosure by reference. Additionally, a US sensor 260 may be printed directly on the distal portion of a medical instrument 280, catheter 270, and/or EWC 230. When used in conjunction with the EM sensor 262, the US sensor 260 improves accuracy and precision when navigating to a target tissue by providing real time imaging of the distal end of the medical instrument 280, catheter 270, and/or EWC 230.

[0040] FIG. 3 depicts an embodiment of an US sensor 260 printed on an instrument 300. The instrument 300 may be an EWC 230, a catheter 270, a medical instrument 280, a biopsy instrument, an ablation instrument, a monopolar or bipolar electrosurgical instrument, a marking instrument, or a needle, in short any instrument capable of being inserted into the luminal network (e.g., the airways or vasculature of a patient). In one embodiment the instrument 300 is sized to pass through the EWC 230. Alternatively, the instrument 300 may be the EWC 230. Other exemplary instruments 300 are shown in FIGS. 5A-5D, depicting biopsy forceps 570, a biopsy brush 575, a biopsy

needle 580, and a microwave ablation probe 585, each having an US sensor 260 applied by the methods of the present disclosure. The US sensor 260 can provide ultrasound imaging of tissue at the distal end of instrument 300. When used in conjunction with an EM sensor 262, a user is able to identify the location of the instrument 300 (through the EM sensor 262) and obtain a visual image of the precise location of the instrument 300 (through the US sensor 260). Any number of combinations for the location of the US sensor 260 and EM sensor 262 are envisioned. For example, some of which have been discussed above, the US sensor 260 may be located on the EWC 230 and the EM sensor 262 on the instrument 300, or the US sensor 260 may be located on the instrument 300 and the EM sensor 262 on the EWC 230. Alternatively, both the US sensor 260 and the EM sensor 262 may be located on either the EWC 230 or the instrument 300.

[0041] As will be described in greater detail below, the distal portion of the instrument 300 may be made of or covered by Ethylene tetrafluoroethylene (ETFE), Polytetrafluoroethylene (PTFE), polyimide, or another suitable material to form a non-conductive base for the US sensor 260. If the distal portion of the instrument 300 is not covered or made of a non-conductive material, a non-conductive material may be applied to the distal portion first to form an insulating base for the US sensor 260. In embodiments, instrument 300 may comprise a hollow tube consisting of an inner PTFE liner. The PTFE liner provides lubricity for easy sliding of tools down the center of the instrument 300. In one embodiment, the EM sensor 262 is printed directly on the PTFE layer. Radially outward of the PTFE layer is a wire braid layer (not shown). The wire braid helps provide structural integrity and torquability to allow for easy maneuverability of the instrument 300. The final layer is a thermal plastic layer which, through a heat process, bonds all three layers together to provide durability.

[0042] With respect to the US sensor 260 depicted in FIG. 3, the US sensor 260 may be printed in an array. Although FIG. 3 depicts the US sensor 260 printed in perpendicular rows, other configurations are envisioned. For example, the US sensor 260 may be printed in non-overlapping parallel rows (as depicted in FIGS. 2B-2D) or in non-perpendicular rows. The US sensor 260 is printed from piezoelectric material. In embodiments, an EM sensor 262 (shown in FIGS. 2B-D) is also printed on the instrument 300 adjacent to the US sensor 260. PZT is a preferred material due to its strong mechanical to electrical coupling. The US sensor 260 may be fabricated and printed on the medical instrument 300 using known microelectromechanical system (MEMS) and/or nanoelectromechanical system (NEMS) techniques. In one embodiment, the US sensor 260 includes an array of clamped silicon diaphragms (not shown), which are a common component of US sensors. In particular, a thin layer of piezoelectric material, sandwiched between two electrodes, is printed on the silicon diaphragms.

[0043] In embodiments, the radius of the electrodes is smaller than the radius of the diaphragm. When an AC driving signal is applied between the electrodes, the resulting strain on the piezoelectric material vibrates the structure and diaphragm sending ultrasonic pressure waves into its surroundings. Alternatively, the US sensor 260 may be exposed to ultrasonic pressure waves from its surrounding environment, and these waves are translated into electrical signals.

[0044] In embodiments, the US sensor 260 may be printed in an array of US sensors coupled together using known printing techniques, such as drop-on-demand (DOD) or ink-jet printing. The US sensor 260 and the EM sensor 262 may be printed adjacent each other or they may be printed in layers. Specifically, the EM sensor 262 is first printed on the instrument 300, a non-conductive material is then applied over the EM sensor 262, and the US sensor 260 is printed on the non-conductive material. It is

envisioned that any number of layers and/or combination of sensors may be printed on the instrument 300. Each sensor may have a different configuration or location, e.g., a different orientation, a different length L, and a different distance from the distal end of the instrument 300.

[0045] In accordance with the present disclosure, US sensor 260 may be printed directly onto the instrument 300. That is, during the manufacture of the instrument 300, one of the processing steps is to apply one or more conductive inks, piezoelectric material, or other materials to the instrument 300. This printing may be performed by a number of processes including ink jet printing, flexographic printing, vapor deposition, etching, and others known to those of skill in the art without departing from the scope of the present disclosure. The US sensor 260 may have a thickness of about 0.01 to about 0.05 millimeter (mm) so that the sensor can be printed on an instrument 300 without appreciably increasing its dimensions. In accordance with one embodiment, a final non-conductive layer covers the US sensor 260, thereby protecting the top layer of the US sensor 260. In some embodiments, the non-conductive material may be Kapton, ETFE, PTFE, non-conductive polymer, or polyimide.

[0046] As depicted in FIG. 3, the US sensor 260 contains vias 302, 304 connected to the terminals of US sensor 260. In embodiments, each via is electrically coupled to a different conductive layer on the proximal portion of the instrument 300, as shown in more detail in FIG. 4. Although not shown, EM sensor 262 may also contain one or more respective vias.

[0047] FIG. 4 depicts an embodiment of a proximal portion of an instrument 300 and the various layers of conductive and/or nonconductive material printed directly onto the instrument. FIG. 4 is not drawn to scale and is meant for illustrative purposes only.

Each layer of conductive and/or nonconductive material may range in thickness from 9 microns to 0.05 millimeters (mm).

[0048] As described above, the EM sensor 262 and US sensor 260 printed on the distal portion of instrument 300. On the proximal portion of the instrument 300, nonconductive layers 400 and conductive layers 402, 404, 406, 408 are printed directly on the PTFE layer in layers in alternating fashion. In other words, a base nonconductive layer 400 is printed on top of the PTFE layer followed by a conductive layer 402 printed on top of the base nonconductive layer. Another nonconductive layer is then printed on top of conductive layer 402 and another conductive layer 404 is printed on top of the nonconductive layer. This process is then repeated until a desired number of nonconductive and conductive layers are achieved. In embodiments, the final layer is a nonconductive layer and a thermal plastic layer is then placed on top of the final nonconductive layer. The embodiment shown in FIG. 4 illustrates a total of four conductive layers 402, 404, 406, 408 and four nonconductive layers 400. A final nonconductive layer (not shown) may be printed on the final conductive layer 408. In aspects, the conductive material may be copper, silver, gold, conductive alloys, or conductive polymer, and the non-conductive material may be Kapton, ETFE, PTFE, non-conductive polymer, or polyimide.

[0049] The conductive layers function as wires and form a return path for the US sensor 260 and EM sensor 262, connecting the sensors to tracking device 160 and/or computing device 120. For example, in one embodiment, conductive layer 402 is connected to via 302, conductive layer 404 is connected to via 304 of US sensor 260, and conductive layer 402 and conductive layer 404 are coupled to the EM sensor 262 through vias (not shown).

[0050] Since the US sensor 260 and EM sensor 262 are very thin, they have a high resistance, however, a low resistance is desired for the return path. In one embodiment, each conductive layer 402, 404, 406, 408 is printed 360 degrees around the instrument 300 and along the length of the instrument 300 back to the proximal end in order to reduce the resistance on the return path.

[0051] As described above, one methodology for applying US sensors to instruments is via printing directly on the instruments. FIG. 6 shows a printing apparatus 600 that prints conductive material, non-conductive material, and piezoelectric material directly to the desired locations of the instruments. The printing apparatus 600 includes a reservoir 610, a printing nozzle 620, and an actuating arm 630. The reservoir 610 includes a first tank 640, which contains a conductive material or a piezoelectric material, and a second tank 650, which contains a non-conductive material. The printing apparatus 600 can print a circuit on any instrument 660, which can be locked into the distal end of the actuating arm 630. In an aspect, the printing apparatus may print a sensor over a polymer.

[0052] A controller (not shown) of the printing apparatus 600 controls an actuating motor (not shown) to move the actuating arm 630. The actuating motor is fixedly connected to the proximal end of the actuating arm 630. The actuating motor can index forward and backward and rotate the actuating arm 630. In an aspect, the actuating motor may move the reservoir 610 while printing. For example, the actuating motor may index forward or backward the reservoir 610 while rotating the actuating arm 630. Still further, the reservoir 610 and instrument 660 may be held motionless while the printing nozzle 620, which is fluidly connected to the reservoir 610, moves about the instrument 660. Further, combinations of these techniques may be employed by those of skill in the art without departing from the scope of the present disclosure.

[0053] In an aspect, the printing may be started from the distal end of the instrument 660 or the proximal end of the instrument 660. In a case when the printing is started from the distal end of the instrument 660, the actuating arm 630 indexes the instrument 660 forward so that the printing nozzle 620 can print the conductive material toward the proximal end of the instrument 660. In another case when the printing is started from the proximal end of the instrument 660, the actuating arm 630 indexes the instrument 660 backward so that the printing nozzle 620 can print the conductive material toward the distal end of the instrument 660. After completion of printing the non-conductive material, the printing nozzle 620 may print the conductive material or piezoelectric material over the instrument 660 again. By repeating these steps, the instrument 660 may have several types of sensors.

[0054] FIG. 7 shows a method 700 of printing the conductive layers 402, 404, 406, 408 which form the return paths for the US sensor 260 and EM sensor 262 on a surface of the instrument 660. The method 700 starts from setting a counter N as zero in step 710. In step 720, the printer prints the conductive material for the vias 302, 304 or for the electrical contacts which couple to an external computing device or ultrasound image resolution device. In step 730, the printer prints a conductive material on the tube. While printing, in step 740, an indexing arm of the printer, which holds the tube, indexes forward or backward, and rotates the tube.

[0055] In step 750, the printer prints the conductive material for another electrical contact. The contacts printed in steps 710 and 750 are to be used to connect to wires which lead to and connect with an external apparatus such as the tracking device 160 of FIG. 1 or an ultrasound image resolution device.

[0056] In step 760, the printer prints a non-conductive material to form a non-conductive film over the printed conductive material. While printing the non-conductive

material, in step 770, the actuating arm of the printer indexes forward or backward and rotates in a direction reverse from the direction of printing the conductive material. In this way, the printed conductive material is insulated from or protected from other environments.

[0057] In step 780, the counter N is incremented by one. In step 790, the counter N is compared with a predetermined number of layers. If the counter N is less than the predetermined number of layers, the method 700 repeats steps 720 through 790. If the counter N is not less than the predetermined number of layers, the method is ended.

[0058] Although embodiments have been described in detail with reference to the accompanying drawings for the purpose of illustration and description, it is to be understood that the inventive processes and apparatus are not to be construed as limited. It will be apparent to those of ordinary skill in the art that various modifications to the foregoing embodiments may be made without departing from the scope of the disclosure.

**WHAT IS CLAIMED IS:**

1. A medical instrument comprising:

- a catheter;
- a conductive layer printed circumferentially around at least a portion of the catheter;
- a nonconductive layer printed on top of the conductive layer;
- an ultrasound sensor printed on a distal portion of the nonconductive layer, the ultrasound sensor adapted to transmit and receive signals;
- at least one pair of vias formed in the conductive layer and nonconductive layer enabling electrical connection of the ultrasound sensor and the conductive layer; and
- a connector formed on a proximal end of the catheter for connection to an ultrasound image resolution device.

2. The medical instrument according to claim 1, further comprising an electromagnetic sensor disposed on a distal portion of the catheter.

3. The medical instrument according to claim 2, further comprising a base non-conductive layer on the distal portion of the medical instrument on which the electromagnetic sensor is printed.

4. The medical instrument according to claim 1, wherein the ultrasound sensor comprises an array of ultrasound transducers.

5. The medical instrument according to claim 4, wherein the ultrasound transducers comprise of piezoelectric material.

6. The medical instrument according to claim 5, wherein the ultrasound transducers further comprise of silicon diaphragms, wherein the piezoelectric material is printed on the silicon diaphragms.
7. The medical instrument according to claim 5, wherein the piezoelectric material is selected from the group consisting of perovskite phase lead zirconate titanate (PZT), quartz, lead titanate, barium titanate, and polyvinylidene fluoride (PVDF).
8. The medical instrument according to claim 4, wherein the array of ultrasound transducers comprises printed parallel rows of ultrasound transducers.
9. The medical instrument according to claim 1, wherein the medical instrument is selected from the group consisting of an extended working channel, a biopsy forceps, a biopsy brush, a biopsy needle, and a microwave ablation probe.
10. The medical instrument according to claim 1, wherein the conductive layer is formed from a material selected from the group of copper, silver, gold, conductive alloys, and conductive polymer.
11. The medical instrument according to claim 1, further comprising an outer surface formed of a material selected from the group consisting of ETFE, PTFE, polyimide, and non-conductive polymer.

12. The medical instrument according to claim 1, wherein the ultrasound sensor, conductive layer, and the non-conductive layer are printed using drop-on-demand (DOD) or ink-jet printing.

13. The medical instrument according to claim 2, wherein the electromagnetic sensor is printed on a distal portion of the medical instrument.

14. The medical instrument according to claim 2, wherein the electromagnetic sensor includes at least one pair of contacts electrically connected to the electromagnetic sensor.

15. The medical instrument according to claim 14, wherein at least one pair of contacts is coupled to the conductive layer.

16. The medical instrument according to claim 15, wherein the conductive layer is connectable to a measurement device configured to sense an induced electrical signal based on a magnetic flux change of an electromagnetic field, wherein a location of the medical instrument in a coordinate system of the electromagnetic field is identified based on the induced electrical signal in the electromagnetic sensor.

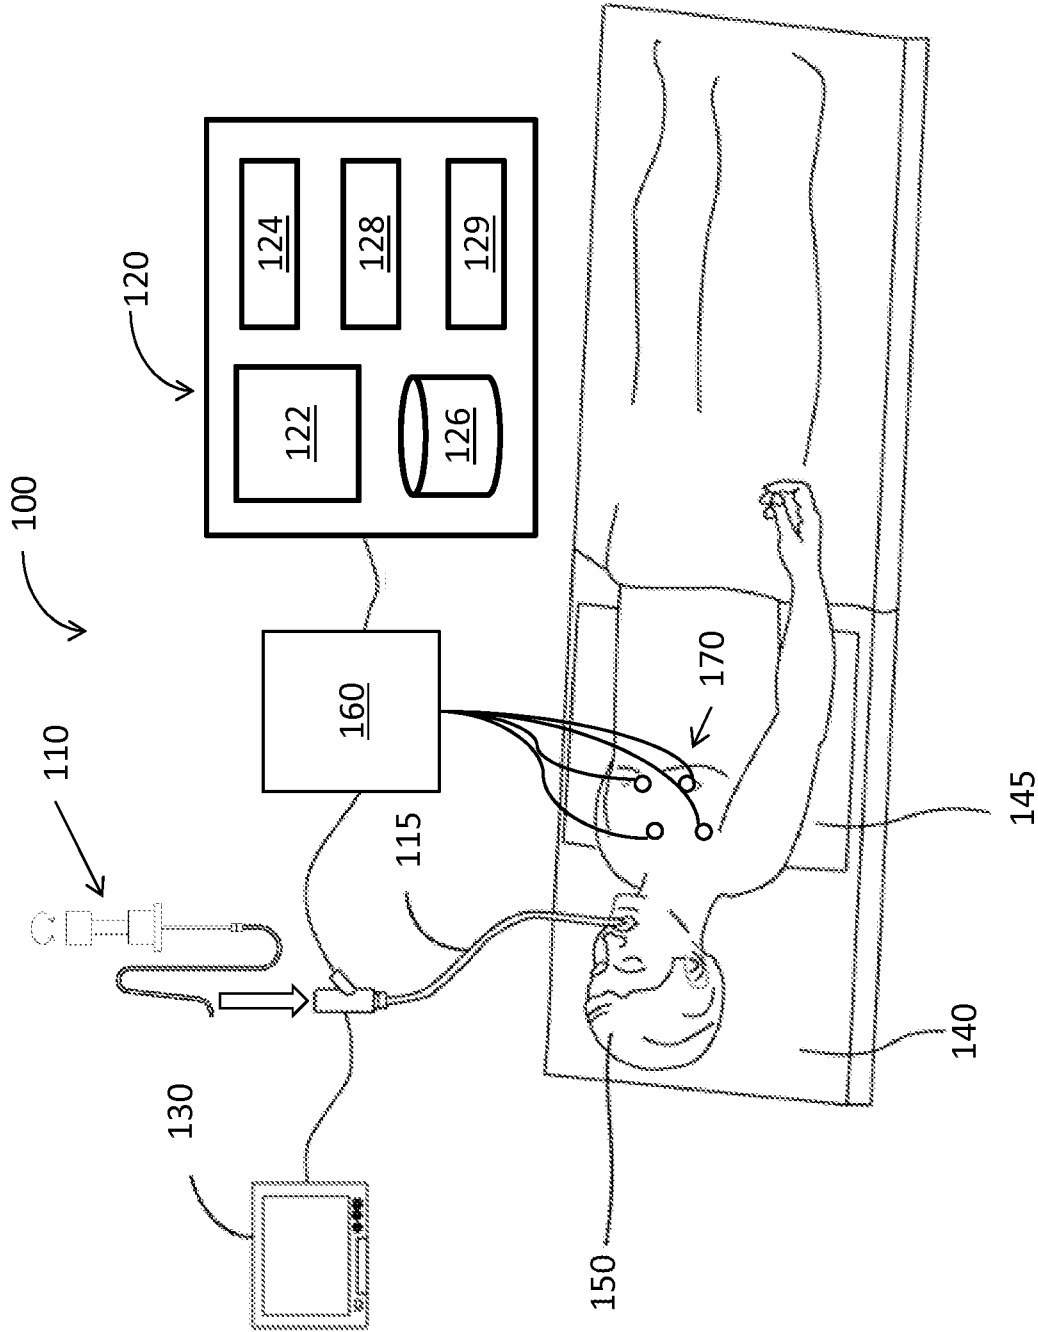


FIG. 1

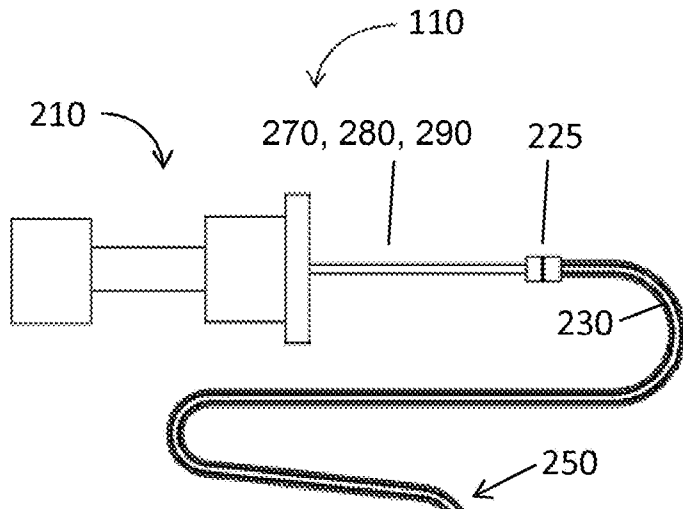


FIG. 2A

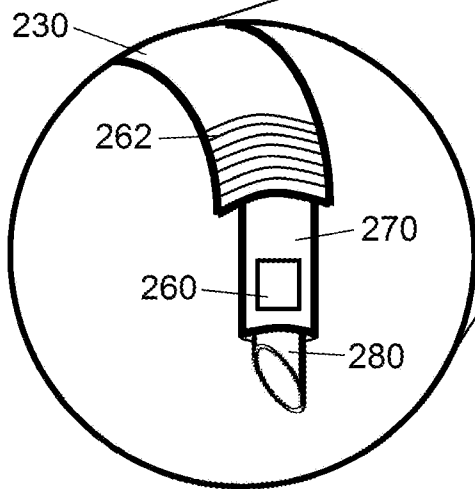


FIG. 2B

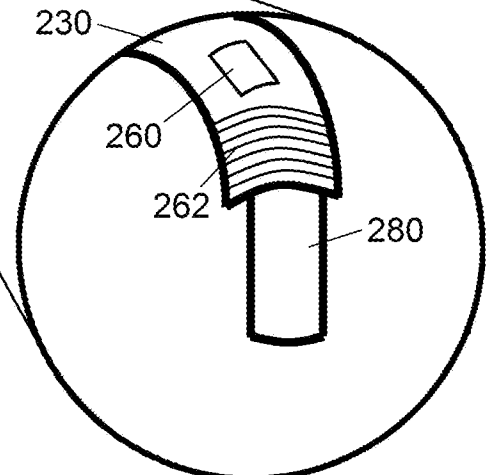


FIG. 2D

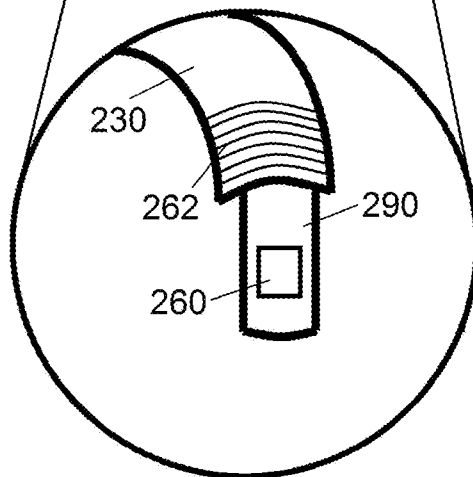
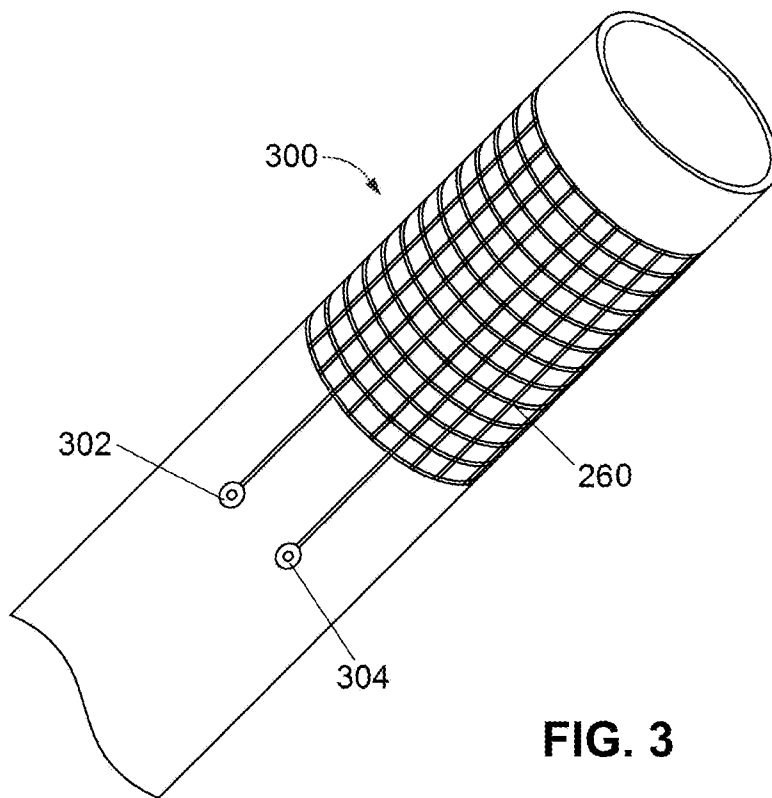


FIG. 2C



**FIG. 3**

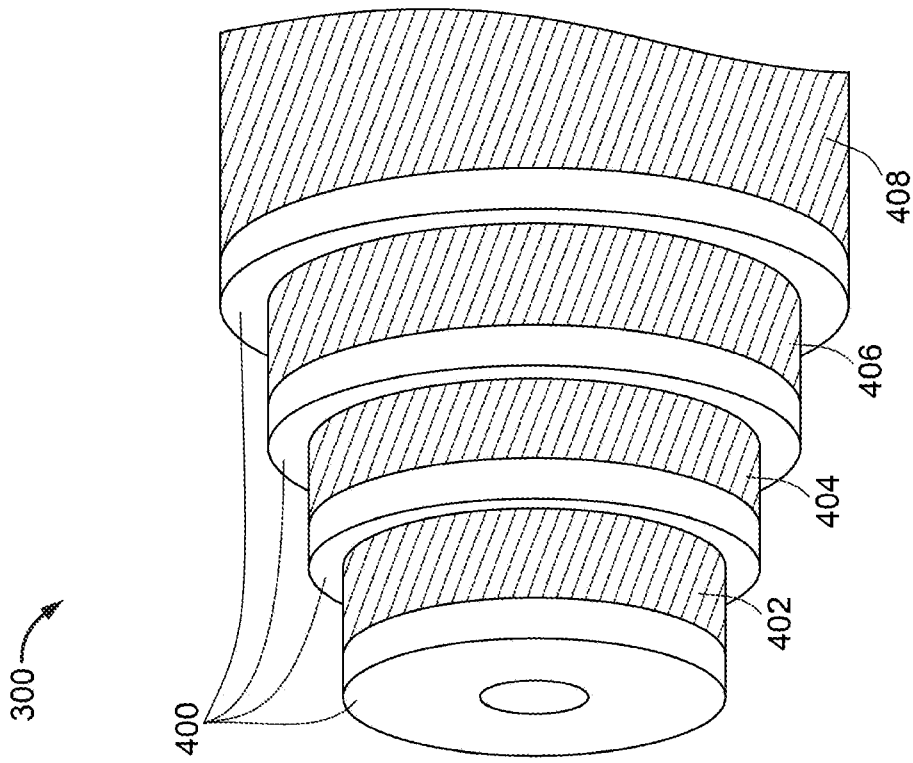


FIG. 4

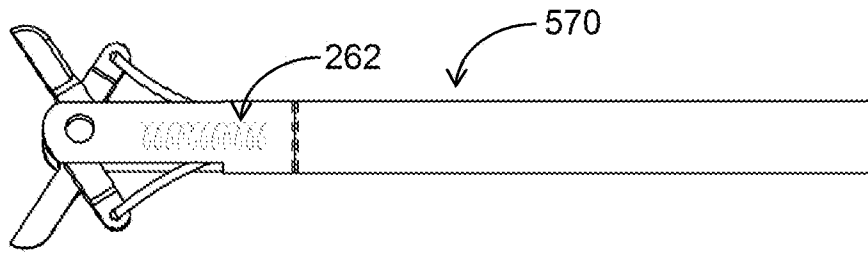


FIG. 5A

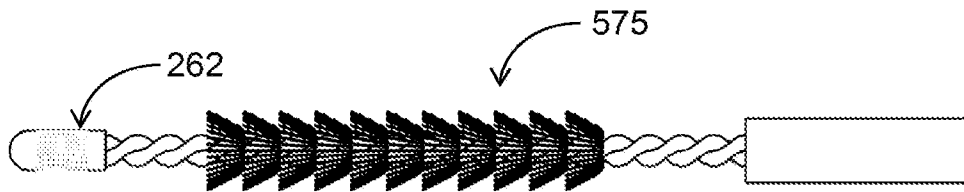


FIG. 5B

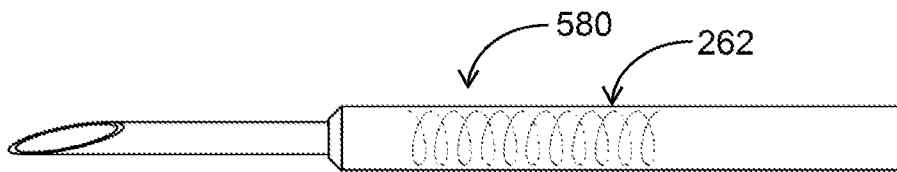


FIG. 5C

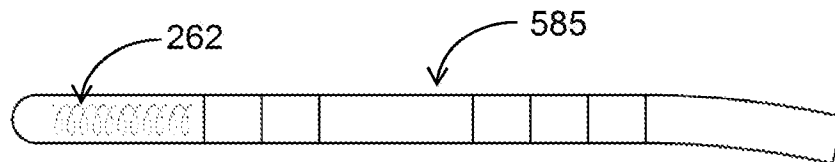


FIG. 5D

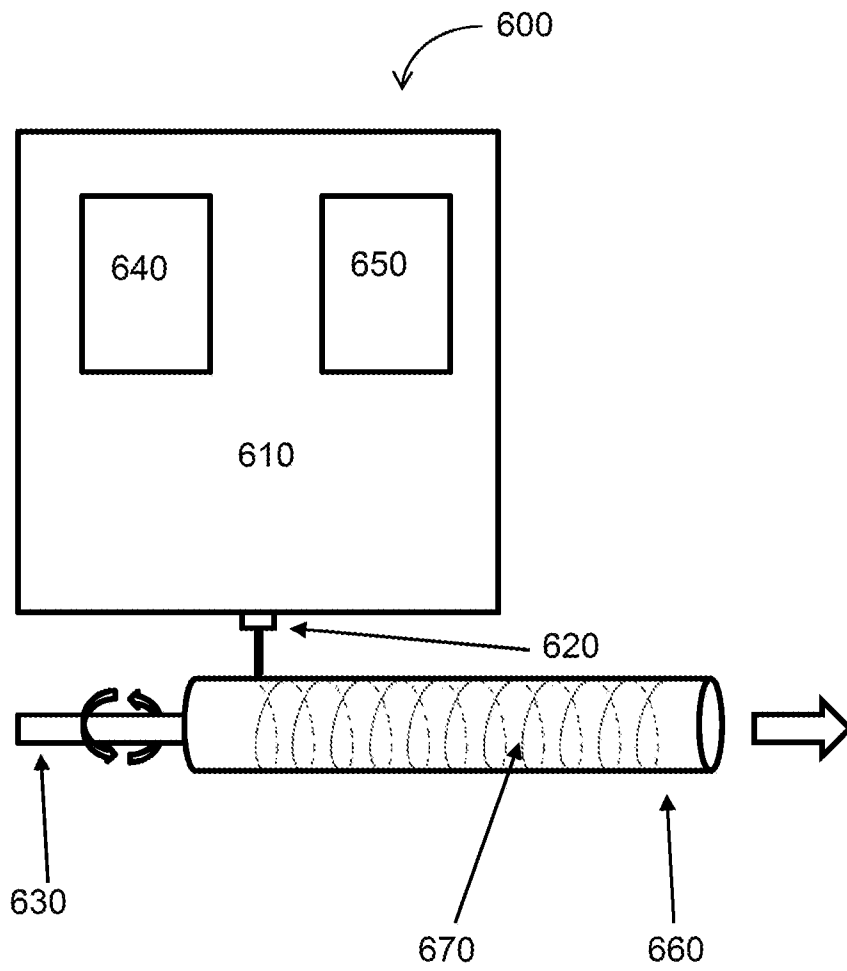
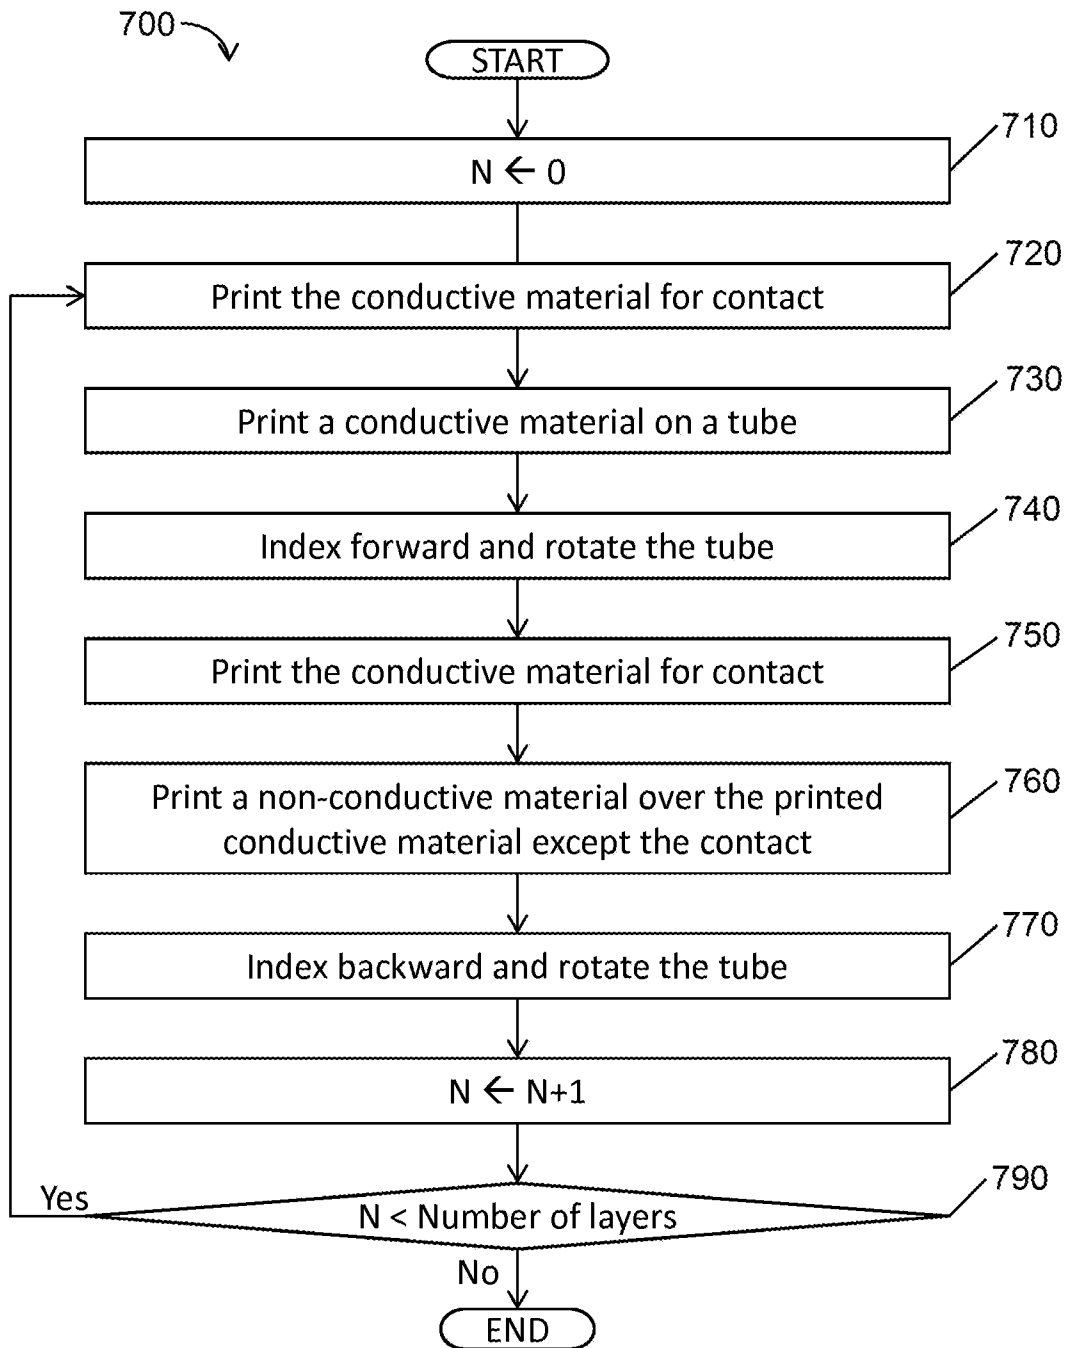


FIG. 6



**FIG. 7**

**A. CLASSIFICATION OF SUBJECT MATTER****A61B 8/12(2006.01)i, A61B 8/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**Minimum documentation searched (classification system followed by classification symbols)  
A61B 8/12; A61B 18/14; A61B 8/14; B32B 38/08; A61B 8/00; A61B 5/00Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched  
Korean utility models and applications for utility models  
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)  
eKOMPASS(KIPO internal) & Keywords: catheter, conductive, nonconductive, ultrasound, layer, sensor**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 2016-010934 A1 (CABRERA-MUNOZ, NESTOR, E. et al.) 21 January 2016 See page 10, line 2-page 27, line 5, claims 2-16 and figures 1-3.	1,4-12
Y		2,3,13-16
Y	US 2004-0193057 A1 (BARBATO et al.) 30 September 2004 See paragraph [32] and claims 25-27.	2,3,13-16
A	US 2015-0032104 A1 (ST. JUDE MEDICAL, ATRIAL FIBRILLATION DIVISION, INC.) 29 January 2015 See claims 1-23 and figures 1-5.	1-16
A	WO 2009-073752 A1 (KOLO TECHNOLOGIES, INC.) 11 June 2009 See claims 1-29 and figures 1-3.	1-16
A	WO 2004-093670 A1 (SCIMED LIFE SYSTEMS, INC.) 04 November 2004 See claims 1-41 and figures 3A,3B.	1-16

 Further documents are listed in the continuation of Box C. See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

27 April 2017 (27.04.2017)

Date of mailing of the international search report

**27 April 2017 (27.04.2017)**

Name and mailing address of the ISA/KR

International Application Division  
Korean Intellectual Property Office  
189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea

Facsimile No. +82-42-481-8578

Authorized officer

KIM, Yeon Kyung

Telephone No. +82-42-481-3325



## INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2017/016471

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2016-010934 A1	21/01/2016	None	
US 2004-0193057 A1	30/09/2004	AU 2003-300403 A1 CA 2520526 A1 CA 2520526 C EP 1608260 A1 EP 1608260 B1 JP 2006-513801 A US 2004-0193041 A1 US 2006-0106314 A1 US 7081094 B2 US 7314448 B2 US 8506493 B2 WO 2004-093670 A1 WO 2005-067801 A1	19/11/2004 04/11/2004 11/12/2012 28/12/2005 01/06/2011 27/04/2006 30/09/2004 18/05/2006 25/07/2006 01/01/2008 13/08/2013 04/11/2004 28/07/2005
US 2015-0032104 A1	29/01/2015	EP 2382002 A1 EP 2382002 A4 EP 2382002 B1 JP 2012-518487 A JP 5572171 B2 US 2010-217257 A1 US 2015-374433 A1 US 8864744 B2 US 9060785 B2 WO 2010-099096 A1	02/11/2011 31/10/2012 20/11/2013 16/08/2012 13/08/2014 26/08/2010 31/12/2015 21/10/2014 23/06/2015 02/09/2010
WO 2009-073752 A1	11/06/2009	CN 101746707 A CN 101750609 A CN 101861127 A CN 101868185 A CN 101868185 B CN 101868981 A CN 101868981 B CN 101874287 A CN 101874287 B CN 101874343 A CN 101874343 B EP 2214560 A1 EP 2215710 A1 EP 2215854 A1 EP 2217151 A1 EP 2218094 A1 JP 2011-505205 A JP 2011-505206 A JP 2011-505765 A JP 2011-507561 A JP 2011-523544 A JP 5269090 B2	23/06/2010 23/06/2010 13/10/2010 20/10/2010 11/12/2013 20/10/2010 07/05/2014 27/10/2010 29/08/2012 27/10/2010 10/09/2014 11/08/2010 11/08/2010 11/08/2010 18/08/2010 18/08/2010 24/02/2011 24/02/2011 24/02/2011 10/03/2011 11/08/2011 21/08/2013

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2017/016471**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		JP 5497657 B2	21/05/2014
		JP 5529749 B2	25/06/2014
		JP 5611830 B2	22/10/2014
		US 2009-0140019 A1	04/06/2009
		US 2009-0140609 A1	04/06/2009
		US 2009-0141592 A1	04/06/2009
		US 2010-0246332 A1	30/09/2010
		US 2010-0251537 A1	07/10/2010
		US 2010-0255623 A1	07/10/2010
		US 2010-0262014 A1	14/10/2010
		US 2010-0280388 A1	04/11/2010
		US 8345513 B2	01/01/2013
		US 8429808 B2	30/04/2013
		US 8483014 B2	09/07/2013
		US 8767514 B2	01/07/2014
		US 8815653 B2	26/08/2014
		US 9408588 B2	09/08/2016
		WO 2009-073692 A1	11/06/2009
		WO 2009-073706 A1	11/06/2009
		WO 2009-073748 A1	11/06/2009
		WO 2009-073753 A1	11/06/2009
WO 2004-093670 A1	04/11/2004	AT 511383 T	15/06/2011
		AU 2003-300403 A1	19/11/2004
		CA 2520526 A1	04/11/2004
		CA 2520526 C	11/12/2012
		EP 1608260 A1	28/12/2005
		EP 1608260 B1	01/06/2011
		ES 2364553 T3	06/09/2011
		JP 2006-513801 A	27/04/2006
		US 2004-0193041 A1	30/09/2004
		US 2004-0193057 A1	30/09/2004
		US 2006-0106314 A1	18/05/2006
		US 7081094 B2	25/07/2006
		US 7314448 B2	01/01/2008
		US 8506493 B2	13/08/2013
		WO 2005-067801 A1	28/07/2005

专利名称(译)	具有柔性电路超声传感器的手术工具		
公开(公告)号	<a href="#">EP3426161A1</a>	公开(公告)日	2019-01-16
申请号	EP2017763707	申请日	2017-02-03
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	COVIDIEN LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	JASPERSON KEITH E CHRISTMANN H AARON WEISENBERGER MICHAEL R		
发明人	JASPERSON, KEITH E. CHRISTMANN, H. AARON WEISENBERGER, MICHAEL R.		
IPC分类号	A61B8/12 A61B8/00		
CPC分类号	A61B8/0841 A61B8/12 A61B8/445 B06B1/0688		
优先权	15/063654 2016-03-08 US		
其他公开文献	EP3426161A4		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

医疗器械包括印刷的超声传感器，表面，至少一种非导电材料和至少一对触头。超声传感器包括印刷在医疗器械的非导电表面上的超声换能器阵列。医疗器械包含多个导电和非导电层。所述至少一对触头电耦合到超声传感器并且可操作地耦合到导电层，导电层耦合到测量装置，测量装置将来自超声传感器的电信号转换成显示在显示单元上的图像。可以在显示单元上实时显示医疗器械的位置。