



(11) **EP 1 720 039 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
03.12.2014 Bulletin 2014/49

(51) Int Cl.:
G01S 15/89 ^(2006.01) **A61B 8/12** ^(2006.01)
A61B 8/14 ^(2006.01)

(21) Application number: **06252210.7**

(22) Date of filing: **25.04.2006**

(54) **Display of a two-dimensional fan shaped ultrasound field**

Darstellung eines zweidimensionalen fächerförmigen Ultraschallfeldes

Représentation d'un champ ultrasonore de deux dimensions en forme d'éventail

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI
SK TR**

(30) Priority: **26.04.2005 US 114680**

(43) Date of publication of application:
08.11.2006 Bulletin 2006/45

(73) Proprietor: **Biosense Webster, Inc.
Diamond Bar, CA 91765 (US)**

(72) Inventors:
• **Altmann, Andres Claudio
Haifa 34614 (IL)**
• **Govari, Assaf
Haifa 34400 (IL)**

(74) Representative: **Small, Gary James et al
Carpmaels & Ransford LLP
One Southampton Row
London WC1B 5HA (GB)**

(56) References cited:
**EP-A- 1 815 797 WO-A-96/25881
US-A- 6 049 622 US-A1- 2002 165 448
US-A1- 2003 199 748 US-A1- 2003 231 789**

- **NOVAK P G ET AL: "Enhanced left atrial mapping using digitally synchronized NavX three-dimensional nonfluoroscopic mapping and high-resolution computed tomographic imaging for catheter ablation of atrial fibrillation" HEART RHYTHM, ELSEVIER, vol. 1, no. 4, October 2004 (2004-10), pages 521-522, XP004608388 ISSN: 1547-5271**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates generally to medical imaging systems, and particularly systems for constructing three-dimensional organ models from multiple ultrasonic images.

BACKGROUND OF THE INVENTION

[0002] Methods for three-dimensional (3-D) mapping of the endocardium (i.e., the inner surfaces of the heart) are known in the art. For example, U.S. Patent 5,738,096 describes a method for constructing a map of the heart. An invasive probe is brought into contact with multiple locations on the wall of the heart. The position of the invasive probe is determined for each location, and the positions are combined to form a structural map of at least a portion of the heart.

[0003] In some systems, such as the one described by U.S. Patent 5,738,096 cited above, additional physiological properties, as well as local electrical activity on the surface of the heart, are also acquired by the catheter. A corresponding map incorporates the acquired local information.

[0004] Some systems use hybrid catheters that incorporate position sensing. For example, U.S. Patent 6,690,963 describes a locating system for determining the location and orientation of an invasive medical instrument.

[0005] A catheter with acoustic transducers may be used for non-contact imaging of the endocardium. For example, U.S. Patents 6,716,166 and 6,773,402 describe a system for 3-D mapping and geometrical reconstruction of body cavities, particularly of the heart. The system uses a cardiac catheter comprising a plurality of acoustic transducers. The transducers emit ultrasonic waves that are reflected from the surface of the cavity and are received again by the transducers. The distance from each of the transducers to a point or area on the surface opposite the transducer is determined, and the distance measurements are combined to reconstruct the 3-D shape of the surface. The catheter also comprises position sensors, which are used to determine position and orientation coordinates of the catheter within the heart.

[0006] U.S. Patent 5,846,205 describes a phased-array ultrasonic transducer assembly that includes a catheter. An end portion is mounted to the catheter around a transducer array, and the end portion defines an acoustic window, which is essentially non-focusing to ultrasonic energy passing therethrough. Because the acoustic window is non-focusing, the inventors claim that a relatively small radius of curvature can be used on the radial outer surface of this window.

[0007] U.S. Patent No. 6,066,096 describes an imaging probe for volumetric intraluminal ultrasound imaging. The probe, configured to be placed inside a patient body, includes an elongated body having proximal and distal

ends. An ultrasonic transducer phased array is connected to and positioned on the distal end of the elongated body. The ultrasonic transducer phased array is positioned to emit and receive ultrasonic energy for volumetric forward scanning from the distal end of the elongated body. The ultrasonic transducer phased array includes a plurality of sites occupied by ultrasonic transducer elements. At least one ultrasonic transducer element is absent from at least one of the sites, thereby defining an interstitial site. A tool is positioned at the interstitial site. In particular, the tool can be a fiber optic lead, a suction tool, a guide wire, an electrophysiological electrode, or an ablation electrode.

[0008] U.S. Patent 6,059,731 describes a simultaneous side-and-end viewing ultrasound imaging catheter system. The system includes at least one side array and at least one end array. Each of the arrays has at least one row of ultrasonic transducer elements. The elements are operable as a single ultrasound transducer and are phased to produce different views.

[0009] U.S. Patent 5,904,651 describes a catheter tube that carries an imaging element for visualizing tissue. The catheter tube also carries a support structure, which extends beyond the imaging element, for contacting surrounding tissue away from the imaging element. The support element stabilizes the imaging element, while the imaging element visualizes tissue in the interior body region. The support structure also carries a diagnostic or therapeutic component to contact surrounding tissue.

[0010] U.S. Patent 5,876,345 describes an ultrasonic catheter for two-dimensional (2-D) imaging or 3-D reconstruction. The ultrasonic catheter includes at least two ultrasonic arrays having good near and far field resolutions. The catheter provides an outline of a heart chamber, in order to assist in interpreting images obtained by the catheter.

[0011] U.S. Patent 6,228,032 describes a steering mechanism and steering line for a catheter-mounted phased linear array of ultrasonic transducer elements.

[0012] U.S. Patent 6,226,546 describes a catheter location system for generating a 3-D map of a part of a human body, from which a position of the catheter may be determined. A plurality of acoustic transducers is disposed about the catheter head at predetermined locations. Acoustic signals are generated by the acoustic transducers acting as sources. A signal processing unit generates the 3-D map responsive to signals received by the acoustic transducers acting as acoustic receivers.

[0013] U.S. Patent 6,171,248 describes an ultrasonic probe for 2-D imaging or 3-D reconstruction. The patent describes an ultrasonic probe that includes at least two ultrasonic arrays. The probe allows 3-D images to be constructed and examined.

[0014] Several methods are known in the art for non-contact reconstruction of the endocardial surface using intracardial ultrasonic imaging. For example, PCT Patent Publication WO 00/19908 describes a steerable trans-

ducer array for intracardial ultrasonic imaging. The array forms an ultrasonic beam, which is steered in a desired direction by an active aperture. U.S. Patent 6,004,269 describes an acoustic imaging system based on an ultrasound device that is incorporated into a catheter. The ultrasound device directs ultrasonic signals toward an internal structure in the heart to create an ultrasonic image. PCT Patent Publications WO 99/05971 and WO 00/07501 describe the use of ultrasound transducers on a reference catheter to locate ultrasound transducers on other catheters (e.g., mapping or ablation catheters) which are brought into contact with the endocardium.

[0015] Further examples of intracardial ultrasonic imaging are presented in U.S. Patent 5,848,969. This publication describes systems and methods for visualizing interior tissue regions using expandable imaging structures.

[0016] PCT Patent Publication WO 99/55233 describes a method for delineating a 3-D surface of a patient's heart. A 3-D mesh model is developed using training data, to serve as an archetypal shape for a population of patient hearts. Multiple ultrasound images of the patient's heart are taken in different image planes. Anatomical locations are manually identified in each of the images. The mesh model is rigidly aligned with the images, in respect to the predefined anatomical locations.

[0017] Other methods of contour extraction and 3-D modeling using ultrasonic images are described in European Patent Application EP 0961135. As another example, PCT Patent Publication WO 98/46139 describes a method for combining Doppler and B-mode ultrasonic image signals into a single image using a modulated non-linear mapping function.

[0018] U.S. Patent 5,797,849 describes a method for carrying out a medical procedure using a 3-D tracking and imaging system. A surgical instrument is inserted into a patient body. The position of the surgical instrument is tracked as it moves through a bodily structure. The location of the surgical instrument relative to its immediate surroundings is displayed to improve a physician's ability to precisely position the surgical instrument.

[0019] U.S. Patent 5,391,199 describes a method for ablating a portion of an organ or bodily structure of a patient. The method includes obtaining a perspective image of an organ or structure to be mapped, and advancing one or more catheters to sites adjacent to or within the organ or structure. The location of each catheter distal tip is sensed using a non-ionizing field. At the distal tip of one or more catheters, local information of the organ or structure is sensed, and the sensed information is processed to create one or more data points. The data points are superimposed on a perspective image of the organ or structure, to facilitate the ablating of a portion of the organ or structure.

[0020] Some medical imaging systems apply methods for reconstructing 3-D models, based on acquired imaging information. For example, U.S. Patent 5,568,384 describes a method for synthesizing 3-D multimodality im-

age sets into a single composite image. Surfaces are extracted from two or more different images and matched using semi-automatic segmentation techniques.

[0021] U.S. Patent 6,226,542 describes a method for 3-D reconstruction of intrabody organs. A processor reconstructs a 3-D map of a volume or cavity in a patient's body from a plurality of sampled points on the volume whose position coordinates have been determined. Reconstruction of a surface is based on a limited number of sampled points.

[0022] U.S. Patents 4,751,643 and 4,791,567 describe a method for determining connected substructures within a body. 3-D regions exhibiting the same tissue type are similarly labeled. Using the label information, all similarly labeled connected data points are determined.

[0023] Some systems use image processing methods for analyzing and modeling body tissues and organs based on information acquired by imaging. One such technique is described by McInerney and Terzopoulos in "Deformable Models in Medical Image Analysis: A Survey," Medical Image Analysis, (1:2), June 1996, pages 91-108. The authors describe a computer-assisted medical image analysis technique for segmenting, matching, and tracking anatomic structures by exploiting (bottom-up) constraints derived from the image data together with (top-down) *a priori* knowledge about the location, size, and shape of these structures.

[0024] Another analysis technique is described by Neubauer and Wegenkittl in "Analysis of Four-Dimensional Cardiac Data Sets Using Skeleton-Based Segmentation," the 11th International Conference in Central Europe on Computer Graphics, Visualization and Computer Vision, University of West Bohemia, Plzen, Czech Republic, February 2003. The authors describe a computer-aided method for segmenting parts of the heart from a sequence of cardiac CT (Computerized Tomography) images, taken at a number of time points over the cardiac cycle.

SUMMARY OF THE INVENTION

[0025] Three-dimensional images of the heart are useful in many catheter-based diagnostic and therapeutic applications. Real-time imaging improves physician performance and enables even relatively inexperienced physicians to perform complex surgical procedures more easily. 3-D imaging also helps to reduce the time needed to perform some surgical procedures. Additionally, 3-D ultrasonic images can be used in planning complex procedures and catheter maneuvers.

[0026] Embodiments of the present invention provide improved systems for performing 3-D cardiac imaging. A probe that comprises an array of ultrasound transducers and a position sensor is used to image a target organ or structure in the patient's body. In one embodiment, the probe comprises a catheter, which is inserted into the patient's heart. The probe acquires multiple 2-D ultrasound images of the target organ and sends them to

an image processor. For each image, location and orientation coordinates of the probe are measured using the position sensor.

[0027] The invention is defined in claim 1. Further aspects are defined in the dependent claims.

[0028] A user of the system, typically a physician, examines the images on an interactive display. The user employs the display to manually mark (also referred to as "tagging") contours of interest that identify features of the organ, on one or more of the images. Additionally the contours can be tagged automatically using a contour detection software. An image processor can automatically identify and reconstruct the corresponding contours in at least some of the remaining, untagged images. The image processor then constructs a 3-D structural model based on the multiple ultrasound images and the corresponding probe coordinates at which each of the images was captured, using the contours to segment the 3-D structures in the model.

[0029] Document US2003231789 A1 discloses a system according to the preamble of claim 1.

BRIEF DESCRIPTION OF THE DRAWINGS

[0030] The present invention will be more fully understood from the following detailed description of the embodiments thereof, taken together with the drawings in which:

Fig. 1 is a schematic, pictorial illustration of a system for cardiac mapping and imaging, in accordance with an embodiment of the present invention;

Fig. 2 is a schematic, pictorial illustration of a catheter, in accordance with an embodiment of the present invention;

Fig. 3 is a flow chart that schematically illustrates a method for cardiac mapping and imaging, in accordance with an embodiment of the present invention;

Figs. 4-8 are images that visually demonstrate a method for cardiac mapping and imaging, in accordance with an embodiment of the present invention;

Figs. 9 and 10 are images that visually demonstrate a modeled cardiac chamber, in accordance with an embodiment of the present invention; and

Fig. 11 is an image that visually demonstrates an ultrasound image registered with a pre-acquired image, in accordance with an embodiment of the present invention.

DETAILED DESCRIPTION OF EMBODIMENTS

SYSTEM DESCRIPTION

[0031] Fig. 1 is a schematic, pictorial illustration of a system 20 for imaging and mapping a heart 24 of a patient, in accordance with an embodiment of the present invention. The system comprises a catheter 28, which is inserted by a physician into a chamber of the heart

through a vein or artery. Catheter 28 typically comprises a handle 29 for operation of the catheter by the physician. Suitable controls on the handle enable the physician to steer, position and orient the distal end of the catheter as desired.

[0032] System 20 comprises a positioning sub-system that measures location and orientation coordinates of catheter 28. (Throughout this patent application, the term "location" refers to the spatial coordinates of the catheter, and the term "orientation" refers to its angular coordinates. The term "position" refers to the full positional information of the catheter, comprising both location and orientation coordinates).

[0033] In one embodiment, the positioning sub-system comprises a magnetic position tracking system that determines the position and orientation of catheter 28. The positioning sub-system generates magnetic fields in a predefined working volume its vicinity and senses these fields at the catheter. The positioning sub-system typically comprises a set of external radiators, such as field generating coils 30, which are located in fixed, known positions external to the patient. Coils 30 generate fields, typically electromagnetic fields, in the vicinity of heart 24. The generated fields are sensed by a position sensor 32 inside catheter 28.

[0034] In an alternative embodiment, a radiator, such as a coil, in the catheter generates electromagnetic fields, which are received by sensors outside the patient's body.

[0035] The position sensor transmits, in response to the sensed fields, position-related electrical signals over cables 33 running through the catheter to a console 34. Alternatively, the position sensor may transmit signals to the console over a wireless link. The console comprises a positioning processor 36 that calculates the location and orientation of catheter 28 based on the signals sent by position sensor 32. Positioning processor 36 typically receives, amplifies, filters, digitizes, and otherwise processes signals from catheter 28.

[0036] Some position tracking systems that may be used for this purpose are described, for example, in U.S. Patents 6,690,963, 6,618,612 and 6,332,089, and U.S. Patent Application Publications 2002/0065455 A1, 2004/0147920 A1 and 2004/0068178 A1. Although the positioning sub-system shown in Fig. 1 uses magnetic fields, the methods described below may be implemented using any other suitable positioning sub-system, such as systems based on electromagnetic fields, acoustic or ultrasonic measurements.

[0037] As will be explained and demonstrated below, system 20 enables the physician to perform a variety of mapping and imaging procedures. These procedures comprise, for example, the following:

- Display real-time or near real-time (NRT) 2-D ultrasound images (See Figs. 4 and 6 below).
- Reconstruct 3-D models of a target structure in the patient's body, based on 2-D ultrasound images (See Figs. 4-10 below).

- Register, overlay and display a parametric map, such as an electro-physiological information map or an electro-anatomical map on the reconstructed 3-D model (See Fig. 8 below).
- Register, overlay and display a 3-D image acquired from an external system on the reconstructed 3-D model.
- Register and display 2-D ultrasound images on a 3-D image acquired from an external system (See Fig. 11 below).

[0038] Fig. 2 is a schematic, pictorial illustration that shows the distal end of catheter 28, in accordance with an embodiment of the present invention. The catheter comprises an ultrasonic imaging sensor. The ultrasonic sensor typically comprises an array of ultrasonic transducers 40. In one embodiment, the transducers are piezo-electric transducers. The ultrasonic transducers are positioned in or adjacent to a window 41, which defines an opening within the body or wall of the catheter.

[0039] Transducers 40 operate as a phased array, jointly transmitting an ultrasound beam from the array aperture through window 23. (Although the transducers are shown arranged in a linear array configuration, other array configurations can be used, such as circular or convex configurations.) In one embodiment, the array transmits a short burst of ultrasound energy and then switches to a receiving mode for receiving the ultrasound signals reflected from the surrounding tissue. Typically, transducers 40 are driven individually in a controlled manner in order to steer the ultrasound beam in a desired direction. By appropriate timing of the transducers, the produced ultrasound beam can be given a concentrically curved wave front, so as to focus the beam at a given distance from the transducer array. Thus, system 20 uses the transducer array as a phased array and implements a transmit/receive scanning mechanism that enables the steering and focusing of the ultrasound beam, so as to produce 2-D ultrasound images.

[0040] In one embodiment, the ultrasonic sensor comprises between sixteen and sixty-four transducers 40, preferably between forty-eight and sixty-four transducers. Typically, the transducers generate the ultrasound energy at a center frequency in the range of 5-10 MHz, with a typical penetration depth of 14 cm. The penetration depth typically ranges from several millimeters to around 16 centimeters, and depends upon the ultrasonic sensor characteristics, the characteristics of the surrounding tissue and the operating frequency. In alternative embodiments, other suitable frequency ranges and penetration depths can be used.

[0041] After receiving the reflected ultrasound echoes, electric signals based on the reflected echoes are sent by transducers 40 over cables 33 through catheter 28 to an image processor 42 in console 34, which transforms them into 2-D, typically sector-shaped ultrasound images. Image processor 42 typically computes or determines position and orientation information, displays real-time

ultrasound images, performs 3-D image or volume reconstructions and other functions which will all be described in greater detail below.

[0042] In some embodiments, the image processor uses the ultrasound images and the positional information to produce a 3-D model of a target structure of the patient's heart. The 3-D model is presented to the physician as a 2-D projection on a display 44.

[0043] In some embodiments, the distal end of the catheter also comprises at least one electrode 46 for performing diagnostic and/or therapeutic functions, such as electro-physiological mapping and/or radio frequency (RF) ablation. In one embodiment, electrode 46 is used for sensing local electrical potentials. The electrical potentials measured by electrode 46 may be used in mapping the local electrical activity on the endocardial surface. When electrode 46 is brought into contact or proximity with a point on the inner surface of the heart, it measures the local electrical potential at that point. The measured potentials are converted into electrical signals and sent through the catheter to the image processor for display. In other embodiments, the local electrical potentials are obtained from another catheter comprising suitable electrodes and a position sensor, all connected to console 34.

[0044] In alternative embodiments, electrode 46 can be used to measure different parameters, such as various tissue characteristics, temperature and/or blood flow. Although electrode 46 is shown as being a single ring electrode, the catheter may comprise any number of electrodes 46 in any form. For example, the catheter may comprise two or more ring electrodes, a plurality or array of point electrodes, a tip electrode, or any combination of these types of electrodes for performing the diagnostic and/or therapeutic functions outlined above.

[0045] Position sensor 32 is typically located within the distal end of catheter 28, adjacent to electrode 46 and transducers 40. Typically, the mutual positional and orientational offsets between position sensor 32, electrode 46 and transducers 40 of the ultrasonic sensor are constant. These offsets are typically used by positioning processor 36 to derive the coordinates of the ultrasonic sensor and of electrode 46, given the measured position of position sensor 32. In another embodiment, catheter 28 comprises two or more position sensors 32, each having constant positional and orientational offsets with respect to electrode 46 and transducers 40. In some embodiments, the offsets (or equivalent calibration parameters) are pre-calibrated and stored in positioning processor 36. Alternatively, the offsets can be stored in a memory device (such as an electrically-programmable read-only memory, or EPROM) fitted into handle 29 of catheter 28.

[0046] Position sensor 32 typically comprises three non-concentric coils (not shown), such as described in U.S. Patent 6,690,963 cited above. Alternatively, any other suitable position sensor arrangement can be used, such as sensors comprising any number of concentric or

non-concentric coils, Hall-effect sensors and/or magneto-resistive sensors.

[0047] Typically, both the ultrasound images and the position measurements are synchronized with the heart cycle, by gating signal and image capture relative to a body-surface electrocardiogram (ECG) signal or intracardiac electrocardiogram. (In one embodiment, the ECG signal can be produced by electrode 46.) Since features of the heart change their shape and position during the heart's periodic contraction and relaxation, the entire imaging process is typically performed at a particular timing with respect to this period. In some embodiments, additional measurements taken by the catheter, such as measurements of various tissue characteristics, temperature and blood flow measurements, are also synchronized to the electrocardiogram (ECG) signal. These measurements are also associated with corresponding position measurements taken by position sensor 32. The additional measurements are typically overlaid on the reconstructed 3-D model, as will be explained below.

[0048] In some embodiments, the position measurements and the acquisition of the ultrasound images are synchronized to an internally-generated signal produced by system 20. For example, the synchronization mechanism can be used to avoid interference in the ultrasound images caused by a certain signal. In this example, the timing of image acquisition and position measurement is set to a particular offset with respect to the interfering signal, so that images are acquired without interference. The offset can be adjusted occasionally to maintain interference-free image acquisition. Alternatively, the measurement and acquisition can be synchronized to an externally-supplied synchronization signal.

[0049] In one embodiment, system 20 comprises an ultrasound driver (not shown) that drives the ultrasound transducers 40. One example of a suitable ultrasound driver, which can be used for this purpose is an AN2300™ ultrasound system produced by Analogic Corp. (Peabody, Massachusetts). In this embodiment, the ultrasound driver performs some of the functions of image processor 42, driving the ultrasonic sensor and producing the 2-D ultrasound images. The ultrasound driver may support different imaging modes such as B-mode, M-mode, CW Doppler and color flow Doppler, as are known in the art.

[0050] Typically, the positioning and image processors are implemented using a general-purpose computer, which is programmed in software to carry out the functions described herein. The software may be downloaded to the computer in electronic form, over a network, for example, or it may alternatively be supplied to the computer on tangible media, such as CD-ROM. The positioning processor and image processor may be implemented using separate computers or using a single computer, or may be integrated with other computing functions of system 20. Additionally or alternatively, at least some of the positioning and image processing functions may be performed using dedicated hardware.

3-D IMAGING METHOD

[0051] Fig. 3 is a flow chart that schematically illustrates a method for cardiac mapping and imaging, in accordance with an embodiment of the present invention. In principle, the disclosed method combines multiple 2-D ultrasound images, acquired at different positions of the catheter, into a single 3-D model of the target structure. In the context of the present patent application and in the claims, the term "target structure" or "target" may refer to a chamber of the heart, in whole or in part, or to a particular wall, surface, blood vessel or other anatomical feature. Although the embodiments described herein refer particularly to structures in and around the heart, the principles of the present invention may similarly be applied, *mutatis mutandis*, in imaging of bones, muscles and other organs and anatomical structures.

[0052] The method begins with acquisition of a sequence of 2-D ultrasound images of the target structure, at an ultrasound scanning step 50. Typically, the physician inserts catheter 28 through a suitable blood vessel into a chamber of the heart, such as the right atrium, and then scans the target structure by moving the catheter between different positions inside the chamber. The target structure may comprise all or a part of the chamber in which the catheter is located or, additionally or alternatively, a different chamber, such as the left atrium, or vascular structures, such as the aorta. In each catheter position, the image processor acquires and produces a 2-D ultrasound image, such as the image shown in Fig. 4 below.

[0053] In parallel, the positioning sub-system measures and calculates the position of the catheter. The calculated position is stored together with the corresponding ultrasound image. Typically, each position of the catheter is represented in coordinate form, such as a six-dimensional coordinate (X, Y, Z axis positions and pitch, yaw and roll angular orientations).

[0054] In some embodiments, the catheter performs additional measurements using electrode 46. The measured parameters, such as local electrical potentials, are optionally overlaid and displayed as an additional layer on the reconstructed 3-D model of the target structure, as will be explained below.

[0055] After obtaining the set of ultrasound images, the image processor displays one or more of these images to the physician, at a manual tagging step 52. Alternatively, step 52 may be interleaved with step 50. The gray levels in the images enable the physician to identify structures, such as the walls of heart chambers, blood vessels and valves. The physician examines the ultrasound images and identifies contours-of-interest that represent walls or boundaries of the target structure. The physician marks the contours on display 44, typically by "tagging" them using a pointing device 45, such as a trackball. (An exemplary tagged 2-D image is shown in Fig. 5 below.) The pointing device may alternatively comprise a mouse, a touch-sensitive screen or tablet coupled to display 44,

or any other suitable input device. The combination of display 44 and pointing device 45 is an example of an interactive display, i.e., means for presenting an image and permitting the user to mark on the image in such a way that a computer is able to locate the marks in the image. Other types of interactive displays will be apparent to those skilled in the art.

[0056] The physician may tag the contours on one or several images out of the set in this manner. The physician may also tag various anatomical landmarks or artifacts, as relevant to the medical procedure in question. The physician may similarly identify "keep away" areas that should not be touched or entered in a subsequent therapeutic procedure, such as ablation.

[0057] In some embodiments, the contours-of-interest are tagged in a semi-automatic manner. For example, the image processor may run suitable contour detection software. In this embodiment, the software automatically detects and marks contours in one or more of the 2-D images. The physician then reviews and edits the automatically-detected contours using the interactive display.

[0058] The image processor may use the tagged contours to automatically reconstruct the contours in the remaining, untagged ultrasound images, at an automatic tagging step 54. (In some embodiments, the physician may tag all 2-D ultrasound images at step 52. In this case, step 54 is omitted.) The image processor traces the structures tagged by the physician, and reconstructs them in the remaining ultrasound images. This identification and reconstruction process may use any suitable image processing method, including edge detection methods, correlation methods, motion detection methods and other methods known in the art. The position coordinates of the catheter that are associated with each of the images may also be used by the image processor in correlating the contour locations from image to image. Additionally or alternatively, step 54 may be implemented in a user-assisted manner, in which the physician reviews and corrects the automatic contour reconstruction carried out by the image processor. The output of step 54 is a set of 2-D ultrasound images, tagged with the contours-of-interest.

[0059] The image processor subsequently assigns 3-D coordinates to the contours-of-interest identified in the set of images, at a 3-D coordinate assignment step 56. Although in step 52 the physician marks the tags on 2-D images, the location and orientation of the planes of these images in 3-D space are known by virtue of the positional information, stored together with the images at step 50. Therefore, the image processor is able to determine the 3-D coordinates for each pixel or of any pixel in the 2-D images, and in particular those corresponding to the tagged contours. When assigning the coordinates, the image processor typically uses the stored calibration data comprising the position and orientation offsets between the position sensor and the ultrasonic sensor, as described above.

[0060] In some embodiments, the contours-of-interest

comprise discrete points. In these embodiments, the positioning processor assigns a 3-D coordinate to each such discrete point. Additionally, the positioning processor assigns a 3-D coordinate to discrete points of a surface or a volume (defined by surfaces) such as a chamber of a heart. Thus, registration of the pre-acquired image to the one or more 2-D ultrasound images or 3-D model of the ultrasound images can be performed using contours, discrete points, surfaces or volumes.

[0061] In some embodiments, the image processor displays one or more of the 2-D ultrasound images, appropriately oriented in 3-D space. (See, for example, Fig. 6 below.) The contours-of-interest may optionally be marked on the oriented 2-D image.

[0062] The image processor produces a 3-D skeleton model of the target structure, at a 3-D reconstruction step 58. The image processor arranges the tagged contours from some or all of the 2-D images in 3-D space to form the skeleton model. (See an exemplary skeleton model in Fig. 7 below.) In some embodiments, the image processor uses a "wire-mesh" type process to generate surfaces over the skeleton model and produce a solid 3-D shape of the target structure. The image processor projects the contours-of-interest on the generated 3-D model. The model is typically presented to the physician on display 44. (See exemplary 3-D models in Figs. 8-10 below).

[0063] As described above, in some embodiments system 20 supports a measurement of local electrical potentials on the surfaces of the target structure. In this measurement, each electrical activity data-point acquired by catheter 28 comprises an electrical potential or activation time value measured by electrode 46 and the corresponding position coordinates of the catheter measured by the positioning sub-system for creation or generation of an electrophysiological map (by the image processor). The image processor registers the electrical activity data-points with the coordinate system of the 3-D model and overlays them on the model, at an overlaying step 60. Step 60 is optional in the method and is performed only if system 20 supports this type of measurement and if the physician has chosen to use this feature. The electrical activity data-points are typically measured when electrode 46 is in contact with, or in close proximity to, the wall of the target structure. Therefore, the data-points are typically superimposed on the 3-D model of the structure.

[0064] Alternatively, a separate 3-D electrical activity map (often referred to as an electro-anatomical map) can be generated and displayed. For example, a suitable electro-anatomical map can be produced by a CARTO™ navigation and mapping system, manufactured and sold by Biosense Webster, Inc. (Diamond Bar, California). The electrical potential values may be presented using a color scale, for example, or any other suitable visualization method. In some embodiments, the image processor may interpolate or extrapolate the measured electrical potential values and display a full color map that

describes the potential distribution across the walls of the target structure. As defined herein, the term "electro-physiological map" means a map of electrical activity data-points or an electro-anatomical map.

[0065] As noted above, information imported from other imaging applications may be registered with the 3-D model and overlaid on the model for display. For example, pre-acquired computerized tomography (CT), magnetic resonance imaging (MRI) or x-ray information may be registered with the 3-D ultrasound-based model and displayed together with the 3-D model and/or with 2-D ultrasound images on display 44. (See an exemplary overlay of a 2-D image and a pre-acquired CT image in Fig. 11 below.)

[0066] Additionally or alternatively, if additional parametric measurements were taken at step 50 above, these measurements can be registered with the 3-D model and displayed as an additional layer (often referred to as a "parametric map").

[0067] When implementing the disclosed method, the order of steps 50-60 may be modified, and steps may be repeated in an interactive manner. For example, the physician may acquire a first sequence 2-D images and tag them manually. Then, the physician may go back and acquire additional images and have the system tag them automatically, using the tagged contours in the first sequence of images. The physician may then generate the full 3-D model and examine it. If the model is not accurate enough in some areas, the physician may decide to acquire an additional set of images in order to refine the 3-D model. Additionally or alternatively, the physician may decide, after examining the images or the 3-D model, to change the manual tagging of one or more of the images, or to override the automatic tagging process. Other sequences of applying steps 50-60, in order to reach a high quality 3-D model of the target structure, may also be followed by the physician. Additionally or alternatively, some of these steps may be carried out automatically, under robotic control, for example.

[0068] In some embodiments, features from the 2-D ultrasound images are selectively displayed as part of the 3-D model. For example, features that are located outside the volume defined by the contours-of-interest may be discarded or hidden from the displayed model. Alternatively or additionally, only the skeleton model or the wire-mesh model can be displayed. Other suitable criteria can be used for filtering the information to be displayed. For example, "keep away" areas marked in one or more of the 2-D images, as described above, may be suitably drawn and highlighted in the 3-D model.

[0069] In some embodiments, system 20 can be used as a real-time or near real-time imaging system. For example, the physician can reconstruct a 3-D model of the target structure using the methods described above, as a preparatory step before beginning a medical procedure. The physician can tag any desired anatomical landmarks or features of interest, which are displayed on the 3-D model. During the procedure, system 20 can contin-

uously track and display the 3-D position of the catheter with respect to the model and the tagged contours. The catheter used for performing the medical procedure may be the same catheter used for generating the 3-D model, or a different catheter fitted with a suitable position sensor.

CARDIAC IMAGING EXAMPLE

[0070] Figs. 4-8 are images that visually demonstrate the 3-D imaging method described above, in accordance with an embodiment of the present invention. The figures were produced from ultrasound images generated by a cardiac imaging system implemented by the inventors.

The images were produced during a real-life experiment that imaged the heart of a pig using a catheter similar to the catheter shown in Fig. 2 above.

[0071] Fig. 4 shows a 2-D ultrasound image acquired by the ultrasonic transducers at a particular position of catheter 28. The image shows two distinct features 80 and 82 of the heart. Multiple ultrasound images of this form were acquired at different positions of the catheter, in accordance with ultrasound scanning step 50 of the method of Fig. 3 above.

[0072] Fig. 5 shows the ultrasound image of Fig. 4, with features 80 and 82 marked with contours 84 and 86, respectively. Fig 4 was taken with the catheter positioned in the right atrium. In this 2-D ultrasound image, feature 80 represents the mitral valve and feature 82 represent the aortic valve. The contours were manually tagged by a user, in accordance with manual tagging step 52 of the method of Fig. 3 above. Contours 84 and 86 mark the anatomical structures in the 3-D working volume and assist the physician to identify these structures during the procedure.

[0073] Fig. 6 shows a 2-D ultrasound image 85 oriented and projected in 3-D space. The figure shows an exemplary split-screen display, as can be produced by image processor 42 and displayed on display 44 of system 20. The "raw" 2-D image is displayed in a separate window on the right hand side of the figure.

[0074] An isometric display at the center of the figure shows a projected image 87, produced by orienting and projecting the plane of image 85 in 3-D space, in accordance with the position measurement of position sensor 32. An orientation icon 81, typically having the shape of the imaged anatomical structure (a heart in this example), is displayed with the same orientation as projected image 87 in real-time as catheter 28 is moved within the patient's body. Icon 81 assists the physician in understanding the 3-D orientation of the projected image.

[0075] A beam icon 83 is used in association with projected 2-D image 87 to mark the area scanned by the ultrasound beam. As such, icon 83 is oriented and displayed in the same plane (same orientation) as projected image 87 in real-time as catheter 28 is moved within the patient's body. Icon 83 may comprise a web-like or fan-like linear depiction, preferably in color, such as red. Al-

ternatively, icon 83 may comprise a colored line marking the perimeter of the area scanned by the beam to produce image 87, or any other suitable means for visualizing the position and orientation of the ultrasound beam. In the example of Fig. 6, icon 83 comprises two straight lines indicating the angular sector defined by the ultrasound beam. In some embodiments, an additional icon 99 marking the location and position of the distal end of catheter 28 is also displayed. For example, the distal end of catheter 28 is displayed as a catheter tip icon 99 that permits the physician or user of system 20 to understand the location and orientation of ultrasound images captured by the catheter 28, independently of whether any other image processing is used to orient the 2-D ultrasound image or fan 87 or to superimpose the 2-D image on a 3-D image or frame. The physician or user of system 20 may also use the icon 99 for aiming or directing the ultrasound beam in a desired direction and/or orientation. For example, the catheter tip icon 99 may be used in positioning the tip of catheter 28 adjacent to a known landmark in the heart in order to facilitate a more accurate estimation of the direction of the ultrasound beam.

[0076] Projected image 87 is typically displayed inside a cube that marks the boundaries of the working volume. The working volume is typically referenced to the coordinate system of field radiating coils 30 of the positioning sub-system shown in Fig. 1 above. In one embodiment, each side of the cube (i.e., the characteristic dimension of the working volume) measures approximately 12 cm. Alternatively, any other suitable size and shape can be chosen for the working volume, typically depending upon the tissue penetration capability of the ultrasound beam.

[0077] A signal display 91 at the bottom of the figure shows the ECG signal, to which the measurements are synchronized, as explained above.

[0078] When system 20 operates in real time, the position and orientation of the projected image and of icon 83 change with the movements of catheter 28. In some embodiments, the physician can change the angle of observation, zoom in and out and otherwise manipulate the displayed images using the interactive display. The user interface features described herein are shown as an exemplary configuration. Any other suitable user interface can be used.

[0079] In some embodiments, system 20 and the associated user interface can be used for 3-D display and projection of 2-D ultrasound images, without reconstructing a 3-D model. For example, the physician can acquire a single 2-D ultrasound image and tag contours-of-interest on this image. System 20 can then orient and project the ultrasound image in 3-D space, in a manner similar to the presentation of projected image 87. If desired, during the medical procedure the system can continuously track and display the 3-D position of the catheter performing the procedure (which may be different from the catheter acquiring image 87) with respect to the projected ultrasound image and the tagged contours.

[0080] Fig. 7 shows a skeleton model of the target

structure, in this example comprising the right ventricle, produced by the image processor in accordance with 3-D reconstruction step 58 of the method of Fig. 3 above. Prior to generating the skeleton model, the image processor traced and reconstructed contours 84 and 86 in the untagged ultrasound images, in accordance with automatic tagging step 54. Fig. 7 shows the original contours 84 and 86 projected onto 3-D space. Contours 88 were automatically reconstructed by the image processor from other contours tagged by the physician.

[0081] Fig. 8 shows a solid 3-D model of the right ventricle, generated by the image processor. Some of contours 88 are overlaid on the solid model. In addition, contours 89 showing the left ventricle can also be seen in the figure. The surface of the right ventricle is overlaid with an electrical activity map 90, as measured by electrode 46 in accordance with overlaying step 60 of the method of Fig. 3 above. The map presents different electrical potential values using different colors (shown as different shading patterns in Fig. 8).

[0082] Figs. 9 and 10 are images that visually demonstrate modeled left atria, in accordance with an embodiment of the present invention. In both figures, the atrium is shown as a solid model 92. A contour 94 tagged by the physician marks the location of the fossa ovalis. Contours 96 mark additional contours of interest used to construct solid model 92. In Fig. 10, a 2-D ultrasound image 98 is registered with the coordinate system of model 92 and displayed together with the model.

[0083] Fig. 11 is an image that visually demonstrates an ultrasound image 102 registered with a pre-acquired image 100, in accordance with an embodiment of the present invention. In this example, a pre-acquired CT image is registered with the coordinate system of the 3-D model. The pre-acquired image and the 2-D ultrasound image are displayed together on display 44.

[0084] Although the embodiments described above relate specifically to ultrasound imaging using an invasive probe, such as a cardiac catheter, the principles of the present invention may also be applied in reconstructing 3-D models of organs using an external or internal ultrasound probe (such as a trans-thoracic probe), fitted with a positioning sensor. Additionally or alternatively, as noted above, the disclosed method may be used for 3-D modeling of organs other than the heart. Further additionally or alternatively, other diagnostic or treatment information, such as tissue thickness and ablation temperature, may be overlaid on the 3-D model in the manner of the electrical activity overlay described above. The 3-D model may also be used in conjunction with other diagnostic or surgical procedures, such as ablation catheters. The 3-D model may also be used in conjunction with other procedures, such as an atrial septal defect closing procedure, spine surgery, and particularly minimally-invasive procedures.

[0085] It will thus be appreciated that the embodiments described above are cited by way of example, and that the present invention is not limited to what has been par-

ticularly shown and described hereinabove.

Claims

1. A medical imaging system (20) for imaging a target in a patient's body, the target having one or more features, the system comprising:

a catheter (28) comprising a position sensor (32) and an ultrasonic imaging sensor (40), the position sensor configured to transmit electrical signals indicative of positional information of a portion of the catheter in the patient's body, and the ultrasonic imaging sensor configured to transmit ultrasonic energy at the target in the patient's body, receive ultrasonic echoes reflected from the target in the patient's body and transmit signals relating to the ultrasonic echoes reflected from the target in the patient's body; **characterised by** a positioning processor (36) operatively connected to the catheter for determining positional information of the portion of the catheter based on the electrical signals transmitted by the position sensor; a display (44) configured to allow a user of the system to tag contours of interest on one or more two-dimensional ultrasonic images shown on the display, said contours identifying the features of the target; and an image processor (42) operatively connected to the catheter, the positioning processor and the display, the image processor configured to:

- (i) generate a plurality of two-dimensional ultrasonic images (102) of the target based on the signals transmitted by the ultrasonic sensor; to determine three-dimensional coordinates for any pixel of the ultrasonic image of the target by virtue of the positional information and to output a set of two-dimensional ultrasonic images tagged with contours-of-interest;
- (ii) reconstruct a three-dimensional skeleton model using the plurality of two-dimensional ultrasonic images by subsequently assigning three-dimensional coordinates to the tagged contours of interest identified in the set of two-dimensional ultrasound images and arranging the tagged contours from some or all of the two-dimensional ultrasonic images in three-dimensional space to form a skeleton model; and
- (iii) depict a real-time two-dimensional ultrasonic image on the three-dimensional model on the display in a same orientation as an orientation of the portion of the catheter in the patient's body based on positional in-

formation derived from the position sensor.

2. The system according to Claim 1, wherein the contours of interest are tagged in a first one of the plurality of two-dimensional ultrasonic images and the image processor is further configured to automatically identify and reconstruct corresponding contours in at least some of the untagged remaining plurality of two-dimensional ultrasonic images.
3. The system according to Claim 2, wherein the image processor is further configured to reconstruct corresponding contours based on a user input of one or more of: approval, deletion, correction, and modification.
4. The system according to Claim 1, further comprising a pre-acquired image (100); and wherein:
 - the image processor is further configured to register the pre-acquired image with one of the ultrasonic image transmitted by the ultrasonic sensor and the three dimensional model.
5. The system according to any one of Claims 1 to 4, wherein the orientation of the real-time two-dimensional ultrasonic image is depicted on the display in real-time as the same orientation of the portion of the catheter as the catheter is moved within the patient's body.
6. The system according to Claim 5, further comprising using a beam icon (83) to depict the orientation of the real-time two-dimensional ultrasonic image in real-time in the same orientation of the portion of the catheter.
7. The system according to Claim 6, further comprising an orientation icon (81) depicted on the display in a same orientation as the real-time two-dimensional ultrasonic image depicted on the display.
8. The system according to Claim 6, wherein the beam icon is depicted on the display in a color.
9. The system according to Claim 8, wherein the beam icon is a web-like depiction.
10. The system according to Claim 8, wherein the beam icon is a fan-like depiction.
11. The system according to Claim 7, wherein the orientation icon comprises a shape of the target imaged with the catheter.
12. The system according to Claim 11, wherein the target comprises an anatomical structure.

13. The system according to any preceding claim, wherein the image processor is further configured to generate surfaces over the skeleton model using a wire-mesh process to produce a solid three-dimensional shape.

5

Patentansprüche

1. Medizinisches Bildgebungssystem (20) zum Abbilden eines Zielobjekts in dem Körper eines Patienten, wobei das Zielobjekt eine oder mehrere Eigenschaften besitzt, wobei das System Folgendes umfasst:

10

einen Katheter (28), der einen Positionssensor (32) und einen Ultraschallbildgebungssensor (40) umfasst, wobei der Positionssensor konfiguriert ist, elektrische Signale, die Positionsinformationen eines Teils des Katheters in dem Körper des Patienten angeben, zu übertragen, und der Ultraschallbildgebungssensor konfiguriert ist, Ultraschallenergie an das Zielobjekt in dem Körper des Patienten zu übertragen, von dem Zielobjekt in dem Körper des Patienten reflektierte Ultraschallechos zu empfangen und Signale bezüglich der von dem Zielobjekt in dem Körper des Patienten reflektierten Ultraschallechos zu übertragen;

15

20

gekennzeichnet durch

einen Positionierungsprozessor (36), der mit dem Katheter betriebstechnisch verbunden ist, um Positionsinformationen des Teils des Katheters aufgrund der durch den Positionssensor übertragenen elektrischen Signale zu bestimmen;

30

eine Anzeige (44), die konfiguriert ist, einem Anwender des Systems zu ermöglichen, interessierende Konturen auf einem oder mehreren zweidimensionalen auf der Anzeige gezeigten Ultraschallbildern zu markieren, wobei die Konturen die Eigenschaften des Zielobjekts identifizieren; und

35

einen Bildprozessor (42), der mit dem Katheter, dem Positionierungsprozessor und der Anzeige betriebstechnisch verbunden ist, wobei der Bildprozessor konfiguriert ist:

40

45

- (i) mehrere zweidimensionale Ultraschallbilder (102) des Zielobjekts aufgrund der durch den Ultraschallsensor übertragenen Signale zu erzeugen; dreidimensionale Koordinaten für jedes Pixel des Ultraschallbildes des Zielobjekts aufgrund der Positionsinformationen zu bestimmen und eine Gruppe von zweidimensionalen Ultraschallbildern, die mit interessierenden Konturen markiert sind, auszugeben;
- (ii) ein dreidimensionales Skelettmodell un-

50

55

ter Verwendung der mehreren zweidimensionalen Ultraschallbilder zu rekonstruieren, indem anschließend dreidimensionale Koordinaten den markierten interessierenden Konturen, die in der Gruppe der zweidimensionalen Ultraschallbilder identifiziert wurden, zugeordnet werden und die markierten Konturen von einigen oder allen der zweidimensionalen Ultraschallbilder in einem dreidimensionalen Raum angeordnet werden, um ein Skelettmodell zu bilden; und
(iii) ein zweidimensionales Echtzeit-Ultraschallbild auf dem dreidimensionalen Modell auf der Anzeige in derselben Orientierung wie eine Orientierung des Teils des Katheters in dem Körper des Patienten aufgrund von von dem Positionssensor abgeleiteten Positionsinformationen darzustellen.

2. System nach Anspruch 1, wobei die interessierenden Konturen in einem ersten der mehreren zweidimensionalen Ultraschallbilder markiert sind und der Bildprozessor ferner konfiguriert ist, entsprechende Konturen in zumindest einigen der nicht markierten verbleibenden mehreren zweidimensionalen Ultraschallbilder automatisch zu identifizieren und zu rekonstruieren.

3. System nach Anspruch 2, wobei der Bildprozessor ferner konfiguriert ist, entsprechende Konturen aufgrund einer Anwendereingabe von einer oder mehreren von: Genehmigung, Löschung, Korrektur und Änderung zu rekonstruieren.

4. System nach Anspruch 1, das ferner ein vorerfasstes Bild (100) umfasst; wobei:

der Bildprozessor ferner konfiguriert ist, das vorerfasste Bild mit einem der durch den Ultraschallsensor übertragenen Ultraschallbilder und dem dreidimensionalen Modell zu registrieren.

5. System nach einem der Ansprüche 1 bis 4, wobei die Orientierung des zweidimensionalen Echtzeitultraschallbildes als dieselbe Orientierung des Teils des Katheters in Echtzeit auf der Anzeige dargestellt wird, wenn der Katheter innerhalb des Körpers des Patienten bewegt wird.

6. System nach Anspruch 5, das ferner ein Strahlsymbol (83) umfasst, um die Orientierung des zweidimensionalen Echtzeit-Ultraschallbildes in derselben Orientierung des Teils des Katheters in Echtzeit darzustellen.

7. System nach Anspruch 6, das ferner ein Orientierungssymbol (81) umfasst, das auf der Anzeige in derselben Orientierung wie das auf der Anzeige dargestellte zweidimensionale Echtzeit-Ultraschallbild dargestellt wird. 5
8. System nach Anspruch 6, wobei das Strahlsymbol auf der Anzeige in einer Farbe dargestellt wird.
9. System nach Anspruch 8, wobei das Strahlsymbol eine netzartige Darstellung ist. 10
10. System nach Anspruch 8, wobei das Strahlsymbol eine fächerartige Darstellung ist. 15
11. System nach Anspruch 7, wobei das Orientierungssymbol eine Form des Zielobjekts, das mit dem Katheter dargestellt ist, umfasst.
12. System nach Anspruch 11, wobei das Zielobjekt eine anatomische Struktur umfasst. 20
13. System nach einem vorhergehenden Anspruch, wobei der Bildprozessor ferner konfiguriert ist, Flächen über dem Skelettmodell unter Verwendung eines Drahtnetzvorgangs zu erzeugen, um eine dreidimensionale Vollform zu erzeugen. 25

Revendications 30

1. Système d'imagerie médicale (20) pour imager une cible dans le corps d'un patient, la cible possédant une ou plusieurs caractéristiques, le système comprenant : 35

un cathéter (28) comprenant un capteur de position (32) et un capteur imageur ultrasonore (40), le capteur de position étant conçu pour émettre des signaux électriques indiquant des informations sur la position d'une partie du cathéter dans le corps du patient, et le capteur imageur ultrasonore étant conçu pour émettre de l'énergie ultrasonore au niveau de la cible dans le corps du patient, recevoir des échos ultrasonores réfléchis par la cible dans le corps du patient et émettre des signaux relatifs aux échos ultrasonores réfléchis par la cible dans le corps du patient ; 40

caractérisé par 45

un processeur de positionnement (36) relié fonctionnellement au cathéter pour déterminer des informations sur la position de la partie du cathéter à partir des signaux électriques émis par le capteur de position ; 50

un affichage (44) conçu pour permettre à un utilisateur du système de marquer des contours présentant un intérêt sur une ou plusieurs ima-

ges ultrasonores bidimensionnelles présentées sur l'affichage, lesdits contours identifiant les caractéristiques de la cible ; et
un processeur d'images (42) relié fonctionnellement au cathéter, au processeur de positionnement et à l'affichage, le processeur d'images étant conçu pour :

- (i) générer une pluralité d'images ultrasonores bidimensionnelles (102) de la cible à partir des signaux émis par le capteur ultrasonore ; déterminer des coordonnées tridimensionnelles pour tout pixel de l'image ultrasonore de la cible au moyen des informations sur la position et produire un ensemble d'images ultrasonores bidimensionnelles marquées par des contours présentant un intérêt ;
- (ii) reconstituer un modèle de squelette tridimensionnel à l'aide de la pluralité d'images ultrasonores bidimensionnelles en assignant ensuite des coordonnées tridimensionnelles aux contours présentant un intérêt marqués identifiés dans l'ensemble d'images ultrasonores bidimensionnelles et en agençant les contours marqués issus de certaines ou de la totalité des images ultrasonores bidimensionnelles dans un espace tridimensionnel pour former un modèle de squelette ; et
- (iii) représenter une image ultrasonore bidimensionnelle en temps réel sur le modèle tridimensionnel sur l'affichage selon une même orientation qu'une orientation de la partie du cathéter dans le corps du patient à partir d'informations sur la position obtenues du capteur de position.

2. Système selon la revendication 1, dans lequel les contours présentant un intérêt sont marqués dans une première de la pluralité d'images ultrasonores bidimensionnelles et le processeur d'images est conçu en outre pour identifier et reconstituer automatiquement des contours correspondants dans certaines au moins de la pluralité non marquée restante d'images ultrasonores bidimensionnelles.
3. Système selon la revendication 2, dans lequel le processeur d'images est conçu en outre pour reconstituer des contours correspondants à partir d'une entrée utilisateur représentant au moins une des actions suivantes : une approbation, une suppression, une correction et une modification.
4. Système selon la revendication 1, comprenant en outre une image acquise au préalable (100) ; et dans lequel :

le processeur d'images est conçu en outre pour caler l'image acquise au préalable sur l'image ultrasonore émise par le capteur ultrasonore ou bien sur le modèle tridimensionnel.

5

5. Système selon l'une quelconque des revendications 1 à 4, dans lequel l'orientation de l'image ultrasonore bidimensionnelle en temps réel est représentée sur l'affichage en temps réel comme la même orientation que celle de la partie du cathéter à mesure qu'on déplace le cathéter dans le corps du patient. 10
6. Système selon la revendication 5, comprenant en outre une icône de faisceau (83) servant à représenter en temps réel l'orientation de l'image ultrasonore bidimensionnelle en temps réel selon la même orientation que celle de la partie du cathéter. 15
7. Système selon la revendication 6, comprenant en outre une icône d'orientation (81) représentée sur l'affichage selon une même orientation que celle de l'image ultrasonore bidimensionnelle en temps réel représentée sur l'affichage. 20
8. Système selon la revendication 6, dans lequel l'icône de faisceau est représentée sur l'affichage avec une couleur. 25
9. Système selon la revendication 8, dans lequel l'icône de faisceau est une représentation en forme de bande. 30
10. Système selon la revendication 8, dans lequel l'icône de faisceau est une représentation en forme d'éventail. 35
11. Système selon la revendication 7, dans lequel l'icône d'orientation comprend une forme de la cible imagée avec le cathéter. 40
12. Système selon la revendication 11, dans lequel la cible comprend une structure anatomique. 45
13. Système selon l'une quelconque des revendications précédentes, dans lequel le processeur d'images est conçu en outre pour générer des surfaces par-dessus le modèle de squelette à l'aide d'un processus de maillage pour produire une forme tridimensionnelle pleine. 50

50

55

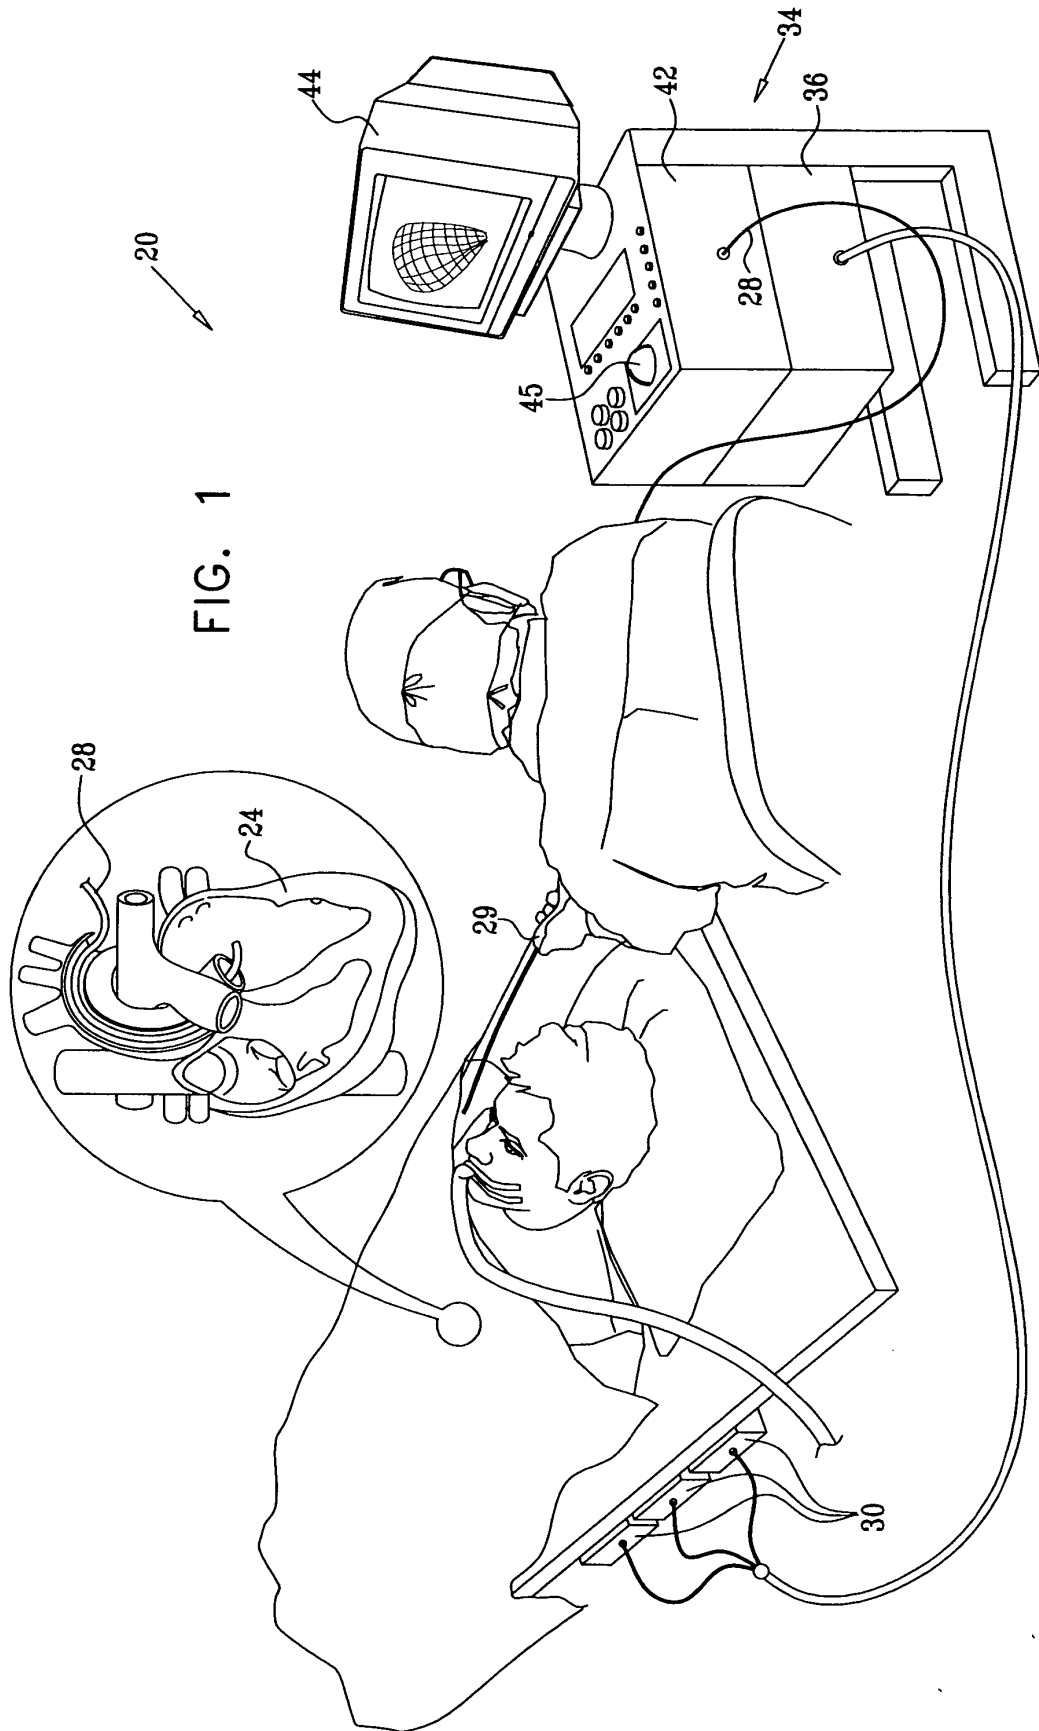


FIG. 2

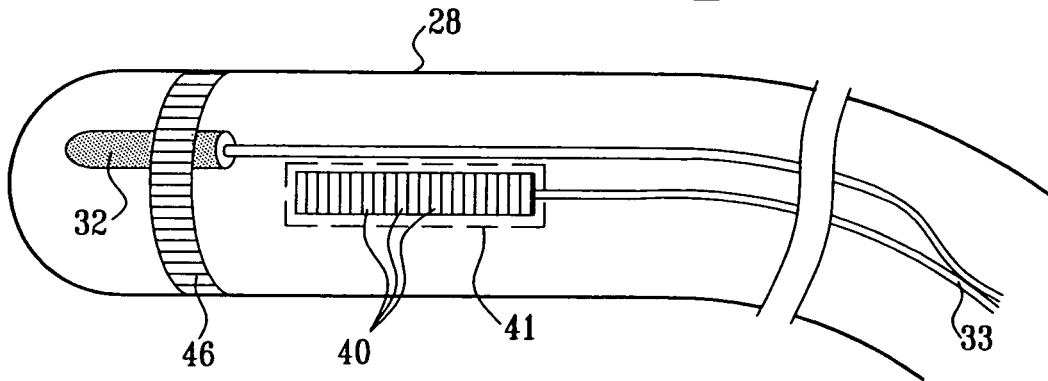


FIG. 3

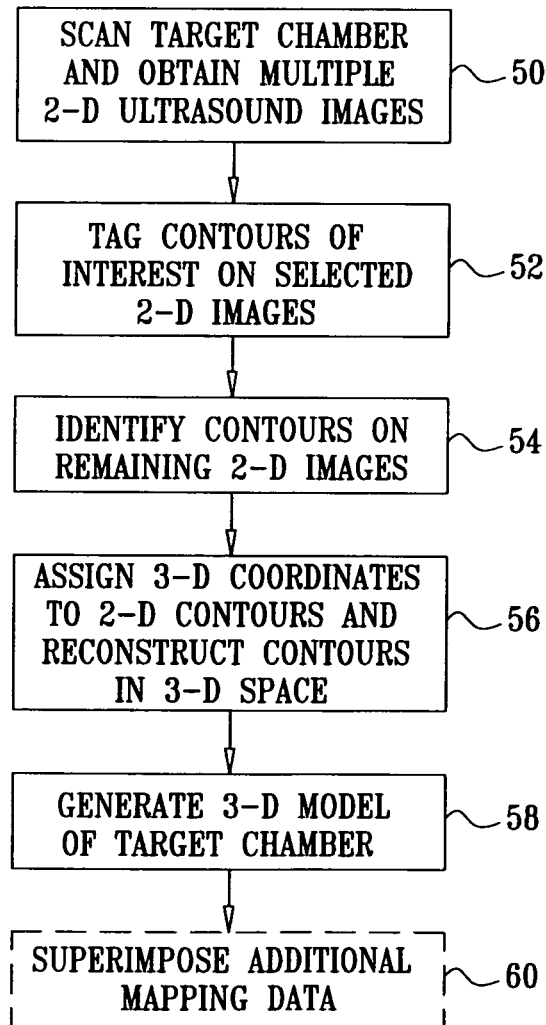


FIG. 4

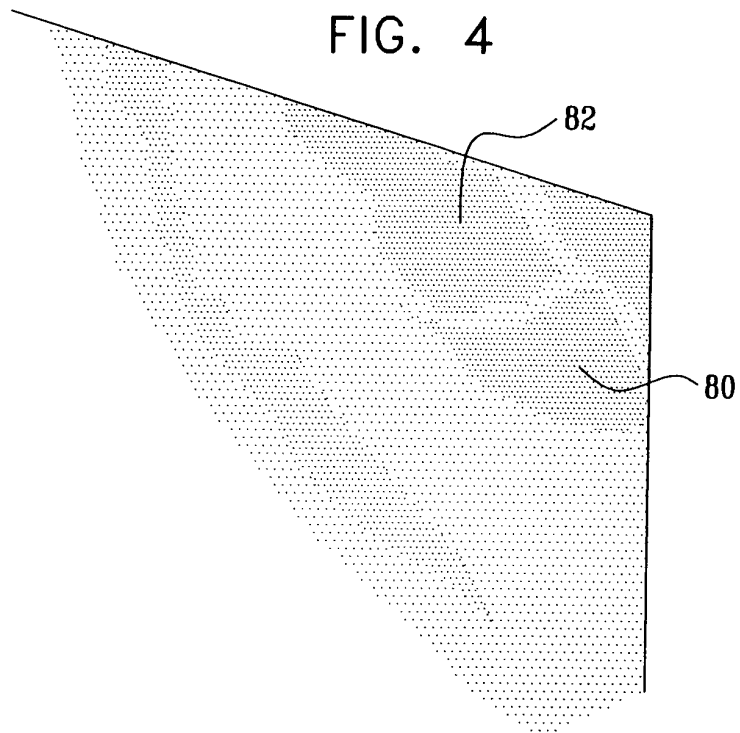
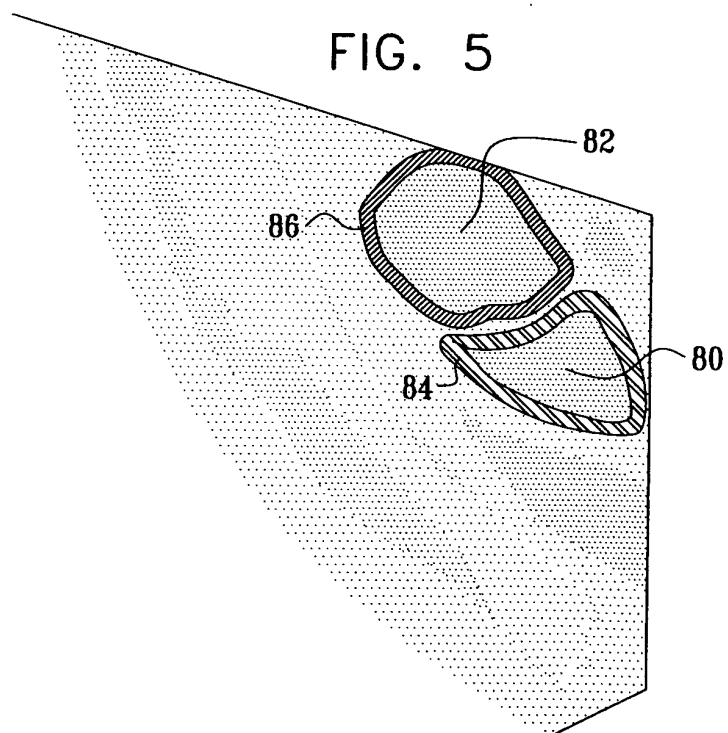


FIG. 5



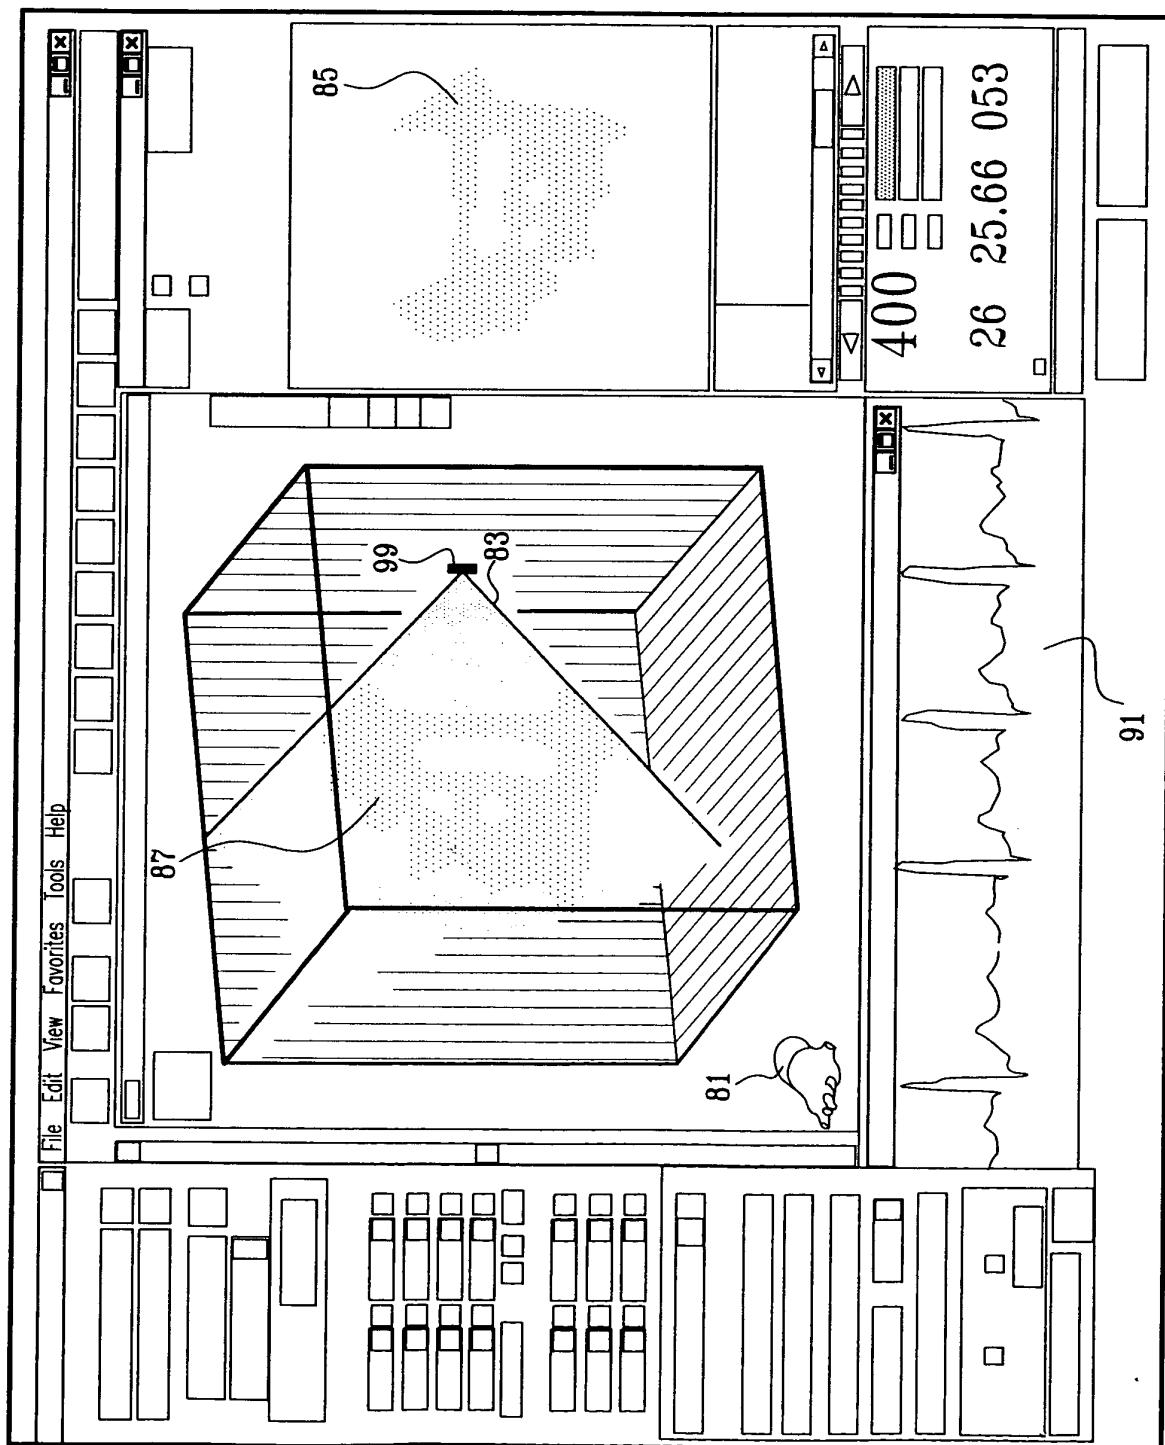


FIG. 6

FIG. 7

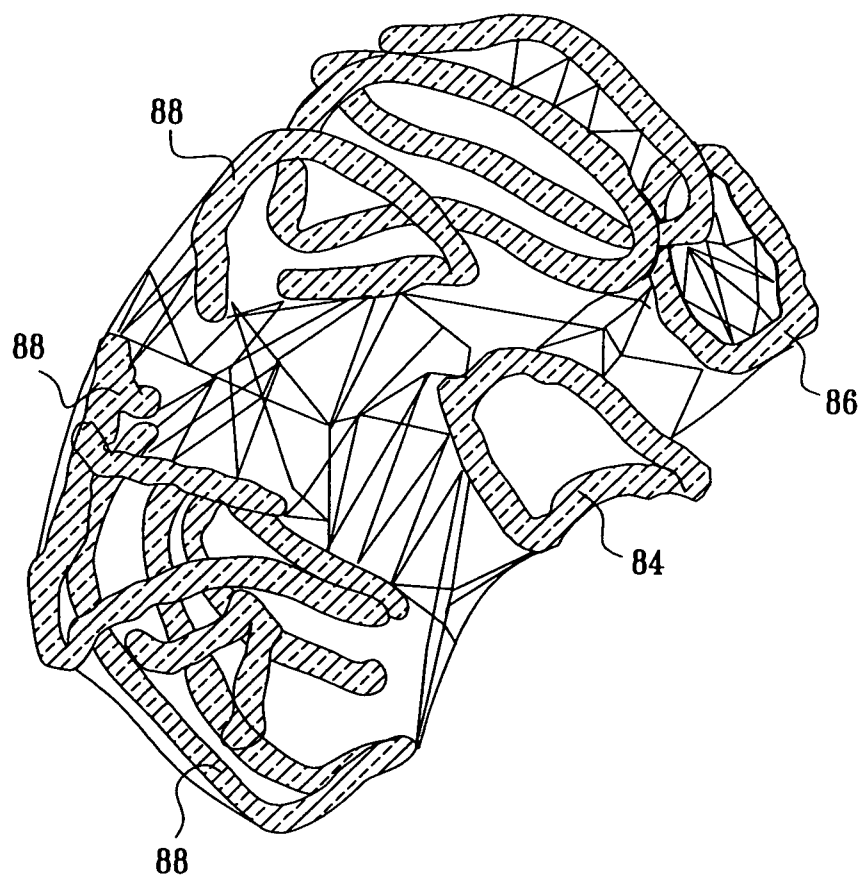


FIG. 8

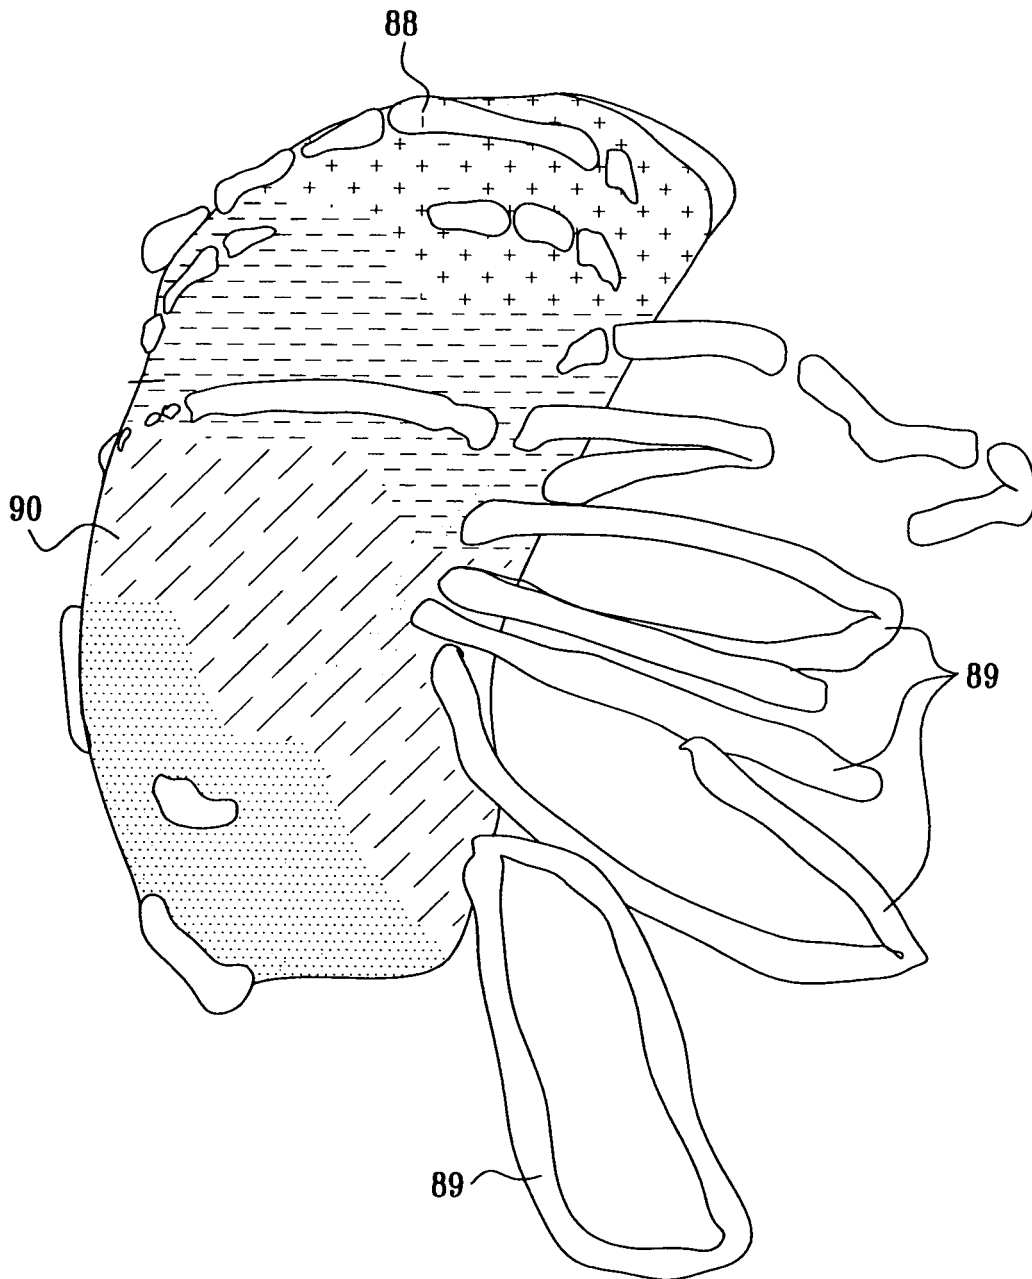


FIG. 9

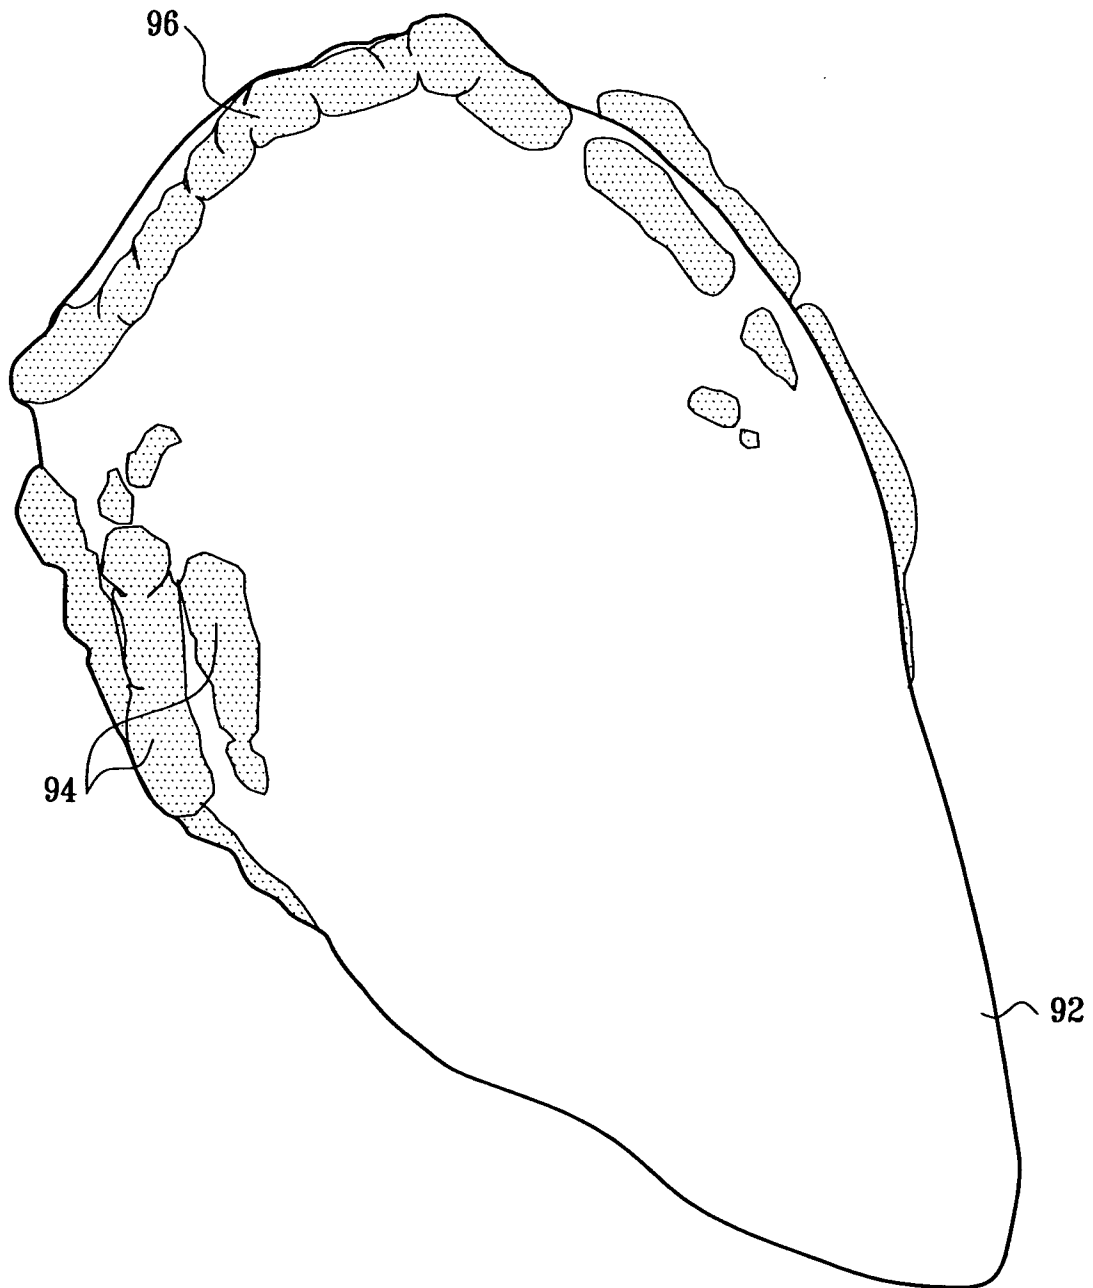


FIG. 10


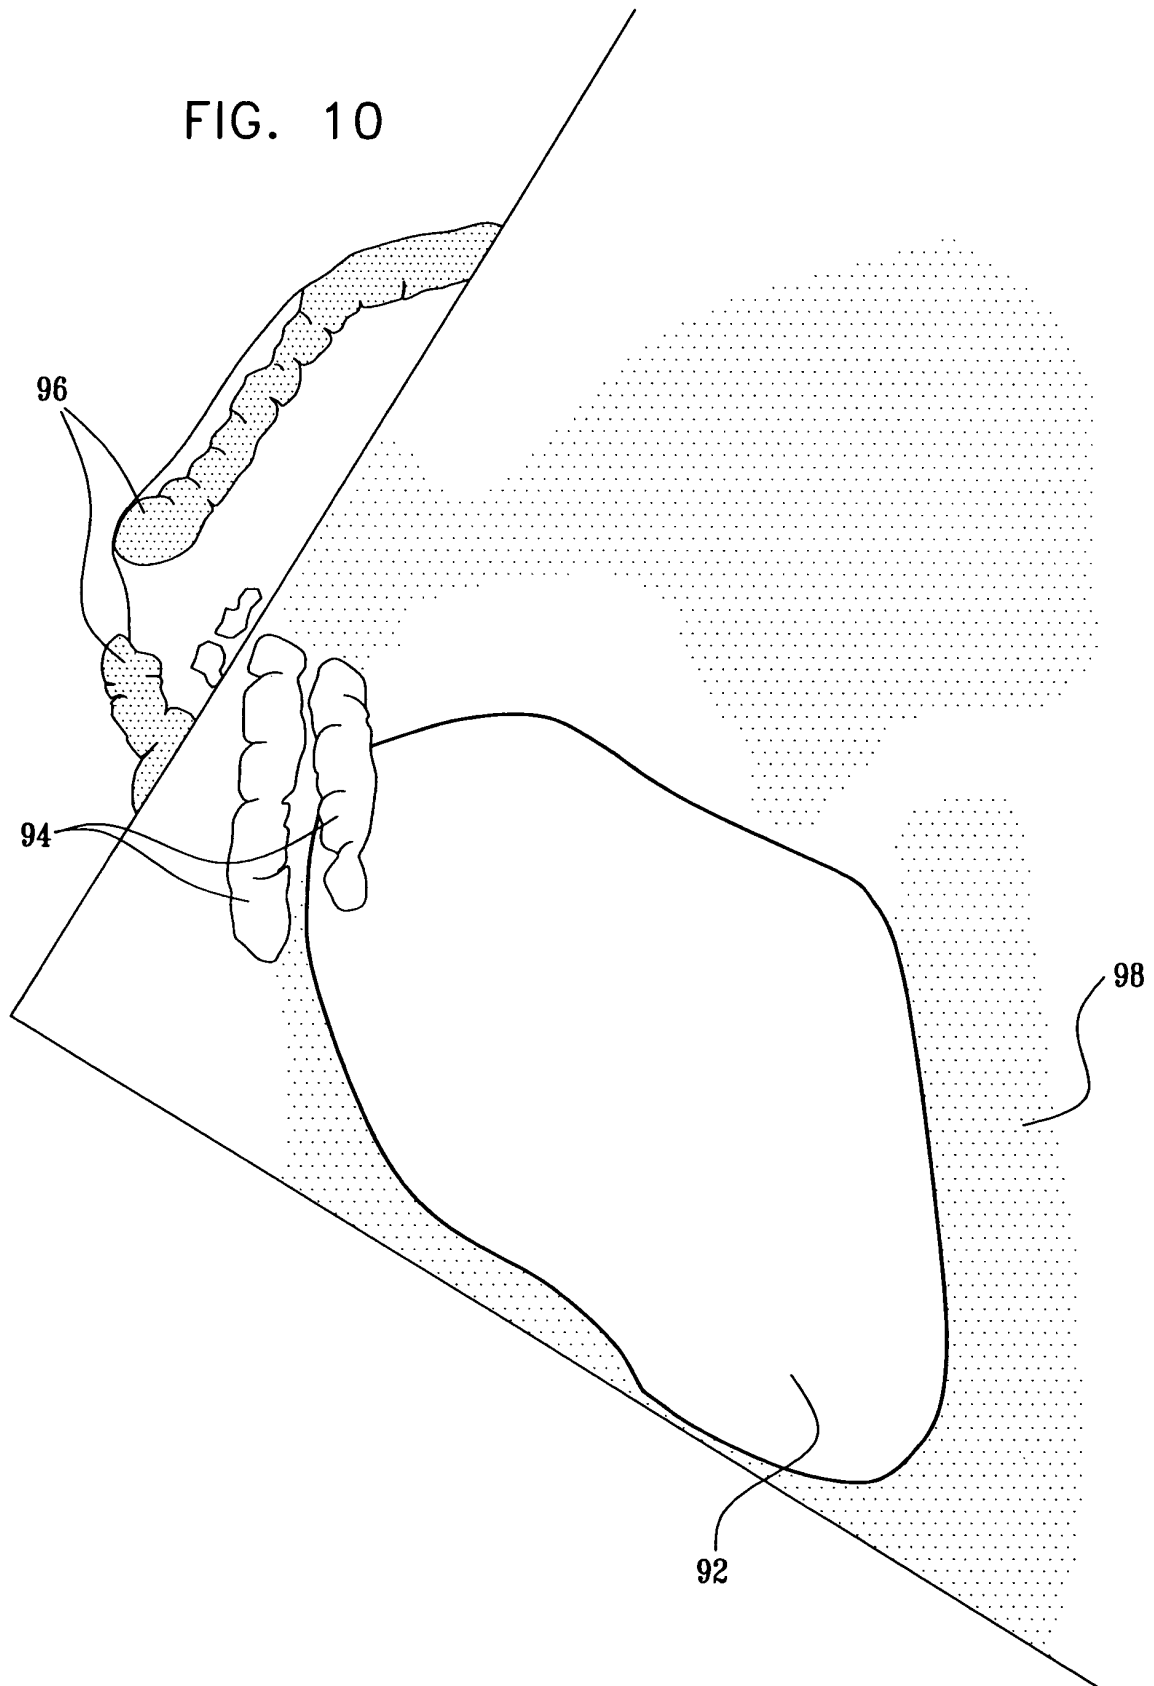


FIG. 11

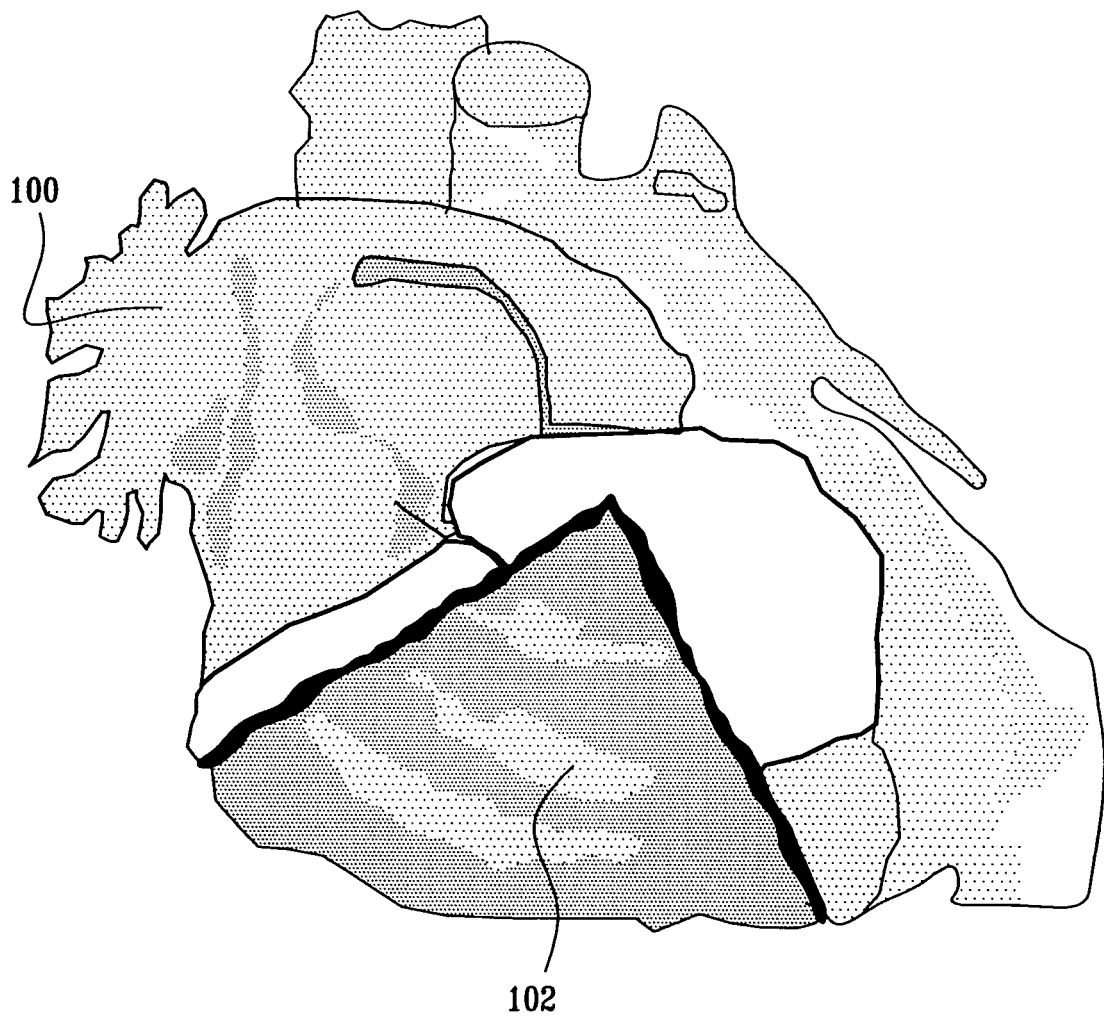

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5738096 A [0002] [0003]
- US 6690963 B [0004] [0036] [0046]
- US 6716166 B [0005]
- US 6773402 B [0005]
- US 5846205 A [0006]
- US 6066096 A [0007]
- US 6059731 A [0008]
- US 5904651 A [0009]
- US 5876345 A [0010]
- US 6228032 B [0011]
- US 6226546 B [0012]
- US 6171248 B [0013]
- WO 0019908 A [0014]
- US 6004269 A [0014]
- WO 9905971 A [0014]
- WO 0007501 A [0014]
- US 5848969 A [0015]
- WO 9955233 A [0016]
- EP 0961135 A [0017]
- WO 9846139 A [0017]
- US 5797849 A [0018]
- US 5391199 A [0019]
- US 5568384 A [0020]
- US 6226542 B [0021]
- US 4751643 A [0022]
- US 4791567 A [0022]
- US 2003231789 A1 [0029]
- US 6618612 B [0036]
- US 6332089 B [0036]
- US 20020065455 A1 [0036]
- US 20040147920 A1 [0036]
- US 20040068178 A1 [0036]

Non-patent literature cited in the description

- **MCINERNEY ; TERZOPOULOS.** Deformable Models in Medical Image Analysis: A Survey. *Medical Image Analysis*, 1996, 91-108 [0023]
- **NEUBAUER ; WEGENKITTL.** Analysis of Four-Dimensional Cardiac Data Sets Using Skeleton-Based Segmentation. *the 11th International Conference in Central Europe on Computer Graphics, Visualization and Computer Vision*, February 2003 [0024]

专利名称(译)	显示二维扇形超声场		
公开(公告)号	EP1720039B1	公开(公告)日	2014-12-03
申请号	EP2006252210	申请日	2006-04-25
[标]申请(专利权)人(译)	韦伯斯特生物官能公司		
申请(专利权)人(译)	生物传感韦伯斯特, INC.		
当前申请(专利权)人(译)	生物传感韦伯斯特, INC.		
[标]发明人	ALTMANN ANDRES CLAUDIO GOVARI ASSAF		
发明人	ALTMANN, ANDRES CLAUDIO GOVARI, ASSAF		
IPC分类号	G01S15/89 A61B8/12 A61B8/14		
CPC分类号	G06T17/10 A61B5/02055 A61B5/042 A61B5/06 A61B5/062 A61B8/12 A61B8/14 A61B8/145 A61B8/4254 A61B8/463 A61B8/543 A61B2090/364 A61B2090/3958 G01S15/8993 G06T7/30 G06T2207/30048 G06T2210/41		
优先权	11/114680 2005-04-26 US		
其他公开文献	EP1720039A2 EP1720039A3		
外部链接	Espacenet		

摘要(译)

用于对患者身体成像的医学成像系统包括具有位置传感器和超声成像传感器的导管，其中位置传感器发送指示导管的一部分在患者体内的位置信息的电信号，并且超声成像传感器发送超声能量在患者体内的目标处，接收从患者体内的目标反射的超声回波，并发送与从患者体内的目标反射的超声回波有关的信号。定位处理器可操作地连接到导管，用于基于由位置传感器发送的电信号确定导管的一部分的位置信息。该系统还包括显示器和可操作地连接到导管，定位处理器和显示器的图像处理器。图像处理器基于由超声波传感器发送的信号生成目标的超声图像，并且在显示器上以与基于患者体内的导管部分的取向相同的取向实时描绘所生成的超声图像。来自位置传感器的位置信息。

