

(19)



(11)

EP 3 099 244 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
13.03.2019 Bulletin 2019/11

(51) Int Cl.:
A61B 8/08 (2006.01) **A61B 8/00** (2006.01)
G01S 7/52 (2006.01) **A61B 8/14** (2006.01)

(21) Application number: **15708583.8**

(86) International application number:
PCT/IB2015/050384

(22) Date of filing: **19.01.2015**

(87) International publication number:
WO 2015/114484 (06.08.2015 Gazette 2015/31)

(54) **ULTRASOUND SYSTEMS FOR MULTI-PLANE ACQUISITION WITH SINGLE- OR BI-PLANE
REAL-TIME IMAGING, AND METHODS OF OPERATION THEREOF**

ULTRASCHALLSYSTEME FÜR MULTIPLANARE ERFASSUNG MIT MONO- ODER BIPLANARER
ECHTZEIT-BILDGEBUNG UND VERFAHREN ZUM BETRIEB DAVON

SYSTÈMES À ULTRASONS POUR ACQUISITION MULTI-PLAN AVEC IMAGERIE EN TEMPS RÉEL
MONO- OU BI-PLAN ET LEURS PROCÉDÉS DE FONCTIONNEMENT

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **28.01.2014 US 201461932312 P**

(43) Date of publication of application:
07.12.2016 Bulletin 2016/49

(73) Proprietor: **Koninklijke Philips N.V.
5656 AE Eindhoven (NL)**

(72) Inventors:
• **GAUTHIER, Thomas Patrice Jean Arsene
NL-5656 AE Eindhoven (NL)**
• **OLSSON, Lars Jonas
NL-5656 AE Eindhoven (NL)**

(74) Representative: **Gravendeel, Cornelis
Philips Intellectual Property & Standards
High Tech Campus 5
5656 AE Eindhoven (NL)**

(56) References cited:
**WO-A1-2009/044316 US-A1- 2012 230 575
US-A1- 2014 013 849 US-B2- 8 012 090**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 3 099 244 B1

Description

[0001] An accurate and early assessment of cancer treatment response is desirable for efficient cancer management and for the evaluation of new therapeutic compounds for cancer patients. Histological determination of a mean intra tumor micro vascular density (MVD) is the most commonly used method for assessing angiogenesis. However, MVD methods do not provide an accurate assessment of the functionality of tumor vessels because many poorly functioning or collapsed vessels have endothelial cells that are stained and counted and rely upon invasive techniques to obtain tissue samples for diagnosis. Therefore, determination of changes in MVD may not accurately reflect the effectiveness of an anti-angiogenic therapy. For many years, the standard way to assess tumor response to treatment has been to measure tumor size using axial computed tomography (CT) or magnetic resonance imaging (MRI) imaging methods, and following a Response Evaluation Criteria in Solid Tumors (RECIST) guidelines and/or World Health Organization (WHO) guidelines. However, it may take several weeks to months for tumor morphology to noticeably change, hence diagnostic information based upon a change in tumor size may take from weeks to months to obtain. Thus, delay is undesirable and is frequently encountered when using image-based diagnostic methods to assess cancer treatments.

[0002] Newly introduced biological anti-cancer compounds, such as anti-angiogenic agents, can cause tumor enlargement before shrinkage, or may stabilize tumor growth to allow patients to live in symbiosis with their cancer. However, diagnosis based upon size criteria (e.g., change of tumor size over time) may not work in such cases. There is therefore clearly a need for a new imaging biomarker to assess tumor response. Such a new imaging biomarker may be used to assess early whether a particular therapeutic regimen is appropriate or effective following initiation of therapy, and it would have implications for both patient management and for drug development to support "go/no-go" decisions and accelerate, for example, clinical trials. Most cancer treatments currently available do not work immediately, do not cause complete necrosis, and/or may not dramatically affect tissue characteristics (compared with ablation therapy). It is therefore not straightforward to detect tumor change by current imaging methods unless the tumor size changes. Quantification of function of the tumor either by blood flow or by metabolism is therefore an attractive method to assess response to therapy such as such as anti-angiogenic therapy.

[0003] For example, a method known as contrast-enhanced ultrasound (CEUS) is one of three (together with Fludeoxyglucose-positron emission tomography (FDG-PET) and dynamic contrast enhanced magnetic resonance imaging (DCE-MRI)) leading functional imaging methods which may be used to assess tumor response to anti-angiogenic therapy or the like. However, conventional CEUS methods can be inaccurate and difficult to perform. There is need for improved systems and methods that provide more accurate measurements and simpler image acquisition workflows.

[0004] Patent application publication US 2014/013849 A1 describes an ultrasound imaging system and method that comprises acquiring data including a first plane and a second plane, adjusting a first orientation of the first plane and, automatically, adjusting a second orientation of the second plane in order to maintain a fixed relationship between the second plane and the first plane.

[0005] US 2012/230575 A1 relates to ultrasound medical imaging for providing information about a region of interest of an object. In order to improve the quantification information provided to a user, a method is provided comprising the following steps: acquiring at least a first and a second ultrasound image plane of an object; determining a region of interest in the at least first and second image planes of the object is; determining first quantification data for the region of interest from the first image plane and second quantification data for the region of interest from the second image plane; and generating a composite quantification measurement by combining the determined first quantification data and second quantification data.

[0006] In patent document US 8,012,090 B2, it is there disclosed an ultrasound system that includes a probe for successively acquiring ultrasound information from an object along at least three distinct scan planes. The scan planes intersect one another along an axis extending from the probe through the object. A memory is included for storing data slices corresponding to the at least three distinct scan planes based on the ultrasound information. Also included is a processor that accesses the memory to select and obtain the data slices and generates ultrasound images based on the data slices. A display is included for co-displaying the ultrasound images.

[0007] Document WO 2009/044316 A1 discloses an ultrasound imaging system for real-time creation and display of a number of images corresponding to parallel slices of a target region in a patient. The system also includes a user interface capable of allowing the user to control the number, orientation, and spacing of the multiple acquired planes.

[0008] The above objects are solved by the independent claims. Advantageous embodiments are defined in the dependent claims.

[0009] The system(s), device(s), method(s), arrangements(s), user interface(s), computer program(s), processes, etc. (hereinafter each of which will be referred to as system, unless the context indicates otherwise), described herein address problems in prior art systems.

[0010] There is disclosed an ultrasound imaging system for imaging a region of interest of a subject. The system may include a controller that is configured to determine a number N of a plurality of image planes to scan through the region of interest, acquire echo information corresponding to each of the image planes in the plurality,

generate image information for each of the image planes based upon the acquired echo information, store the image information corresponding to each of the image planes in a memory of the system; and render, in real time on a display, an ultrasound image comprising the region of interest, wherein the ultrasound image is rendered from generated image information for a single selected image plane of the plurality of image planes or a bi-plane that is orthogonal to the plurality of image planes.

[0011] Further, the controller may render, in real time on the display, lines or other characters or symbols that are overlaid on or positioned at the top and/or bottom of the ultrasound image rendered from the generated image information, the lines or other characters or symbols being indicative of the plurality of image planes scanned through the region of interest.

[0012] In addition, the controller may also render another ultrasound image on the display in real-time based on image information from one of the plurality of image planes and a selected line corresponding to the single selected image plane is displayed differently from remaining lines on the display, and wherein the selected line corresponds to an image plane that is at an angle (e.g., orthogonal) to the plurality of image planes.

[0013] It is also envisioned that the stored image information may include image information corresponding to the selected single image plane, which is rendered in real time, and image information corresponding to image planes, which are not displayed in real time, of the plurality of image planes. It is also envisioned that the controller may generate a time-intensity curve which represents contrast uptake based upon image information corresponding to the image planes which are not rendered in real time and the selected single image plane which is rendered in real time. Moreover, the controller may determine parameters including one or more of peak intensity, area under the curve, rise time, and mean transit time based upon the generated time intensity curve. It is also envisioned that a number of image planes rendered in real-time is independent of N . Moreover, N may be $2 < N < N_{3D}$, where N_{3D} is a typical number of planes acquired in real-time 3D imaging.

[0014] There is also disclosed a method of displaying ultrasound images, and a computer program stored on a non-transitory computer readable memory medium, the computer program and the method being provided to perform the steps and features described for the ultrasound system.

[0015] The present invention is explained in further detail in the following exemplary embodiments and with reference to the figures, where identical or similar elements are partly indicated by the same reference numerals, and the features of various exemplary embodiments being combinable.

[0016] In the drawings:

FIG. 1 shows a flow diagram that illustrates a process performed in accordance with embodiments of the present system;

FIG. 2 shows a portion of a screenshot of a real-time display frame (RTDF) including a graph of image information for the selected single-plane (SSP) in accordance with embodiments of the present system;

FIG. 3 shows a portion of a screenshot of the RTDF including the graph of the image information of the SSP and a graph including image information of an orthogonal scan plane in accordance with embodiments of the present system;

FIG. 4 shows a portion of a screen shot of a graphical user interface (GUI) including the RTDF in accordance with embodiments of the present system; and

FIG. 5 illustrates in block diagram form an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention.

[0017] The following are descriptions of illustrative embodiments that when taken in conjunction with the following drawings will demonstrate the above noted features and advantages, as well as further ones. In the following description, for purposes of explanation rather than limitation, illustrative details are set forth such as architecture, interfaces, techniques, element attributes, etc. However, it will be apparent to those of ordinary skill in the art that other embodiments that depart from these details would still be understood to be within the scope of the appended claims. Moreover, for the purpose of clarity, detailed descriptions of well known devices, circuits, tools, techniques, and methods are omitted so as not to obscure the description of the present system. It should be expressly understood that the drawings are included for illustrative purposes and do not represent the entire scope of the present invention. In the accompanying drawings, like reference numbers in different drawings may designate similar elements.

[0018] In accordance with embodiments of the present system, there is disclosed an ultrasound system (e.g., a real-time two-dimensional (2D) and three-dimensional (3D) contrast-enhanced ultrasound (CEUS) system), which may perform off-line quantitative analysis of acquired image information. In some embodiments, ultrasound images from multiple scan planes or slices may be acquired in real-time, stored, and thereafter used for quantitative analysis. In one embodiment, quantification of tumor blood flow and tumor fractional blood volume may be performed off-line using, for example, cine loops of the acquired ultrasound images where data over the volume of the tumor can be collected and used for quantification. In this scenario, a user (e.g., an operator such as a sonographer, a doctor, etc.) may control an ultrasound

imaging system to scan a plurality of image planes in an object-of-interest, such as a tumor, to acquire image information for each of the image planes to generate a plurality of ultrasound images of the object of interest. In certain embodiments, the collective image data for each of the plurality of image planes may form an image volume or 2D ultrasound images of the object-of-interest (e.g., the tumor) that can be used for various quantitative analyses. For example, image information from one or more of the image planes, which form the image volume, may be stored in a memory of the system for later use such as for post-processing. During post processing, the user may then position a region-of-interest (ROI) in the image volume for quantification and further analysis.

[0019] As will be described further herein, the plurality of images planes can be referred to as N image planes or N' image planes. N image planes are at an angle to N' image planes, e.g., at a 30°, 45°, 90°, or other desired angle. In some embodiments, the N (or N') image planes can be generated to be parallel to each other or at any angle relative (e.g., 90 degrees or orthogonal) to each other. In certain embodiments, a 2D array transducer can generate N image planes that fan out at a predetermined angle relative to each other. In some embodiments, the N image planes are orthogonal to at least one N' image plane. Sets of planes that are generated at an angle relative to each other may be spaced to capture data over about 90-110 degrees. In some embodiments, with a 2D matrix transducer the N image planes may correspond to azimuthal image planes and the N' image planes may correspond to elevational image planes or vice versa. The plurality of image planes may include N or N' image planes where N or N' is an integer greater than two. In some embodiments, a plurality of N image planes may be acquired and stored while only one N' image plane, i.e., a bi-plane image is displayed and/or stored during a scanning operation.

[0020] In accordance with some embodiments, each of the plurality of image planes (e.g., the image slices) may have a user-defined or default thickness (e.g., a slice thickness). The user may also control the location and/or orientation of one or more of the plurality of image planes. For example, the plurality of N (or N') image planes may be parallel to each other or at an angle to each other. The density or spacing between the image planes can also be defined. In some embodiments, an N' image plane orthogonal to the plurality of N image planes, can also be scanned and rendered for display. In certain embodiments, both sets of the plurality of N image planes and the plurality of N' image planes are used to generate ultrasound images,. For example, a first set includes a plurality of N image planes, and a second set includes N' image planes that are orthogonal to the planes of the first set. In certain embodiments, a first set of a plurality of N image planes are fanned out in space and a second set of N' image planes are at an angle (e.g., orthogonal) to the N image planes.

[0021] In accordance with other embodiments, during the acquisition process, a single image plane of the plurality of image planes (e.g., the N image planes) will be displayed on the imaging system in real-time. In certain embodiments, a bi-plane (e.g., an orthogonal image plane) to the plurality of image planes (e.g., the N image planes) will be displayed on the imaging system in real-time. However, image information for each of the plurality of N image planes will be acquired and stored in a memory of the system for later use, such as for post processing off-line and/or for selection and display of one N image plane or an N' image plane at an angle (e.g., orthogonal) to the N image plane.

[0022] With regard to the post-processing, off-line post-processing for, e.g., a contrast-enhanced ultrasound application may be performed to determine parameters such as peak intensity area under a time-intensity curve, as well as other parameters such as rise time and mean transit time and other derived parameters which correlate with tumor blood flow and tumor fractional blood volume, and thus represent contrast uptake by the tumor. Using such a protocol, image information of each image plane (e.g., each image slice or scan plane) from the plurality of scanned image planes may be used to reduce or otherwise minimize errors due to slight changes of a location of an image plane and/or adjustments to the position of the region-of-interest. This may significantly reduce inaccuracy in the time-intensity curve and therefore derived parameters which are thought to correlate with tumor blood flow and tumor fractional blood volume due to changes of position of an image plane and/or adjustments to the region-of-interest.

[0023] Further, as tumors are never homogeneous, by providing quantitative information which may be derived from a plurality of scanned image planes of the tumor, embodiments of the present system may determine overall tumor vascularity with greater accuracy than may be derived from a single scanned image plane. Moreover, as embodiments of the present system may determine a balance between spatial and temporal contrast and determine a plurality of scan planes N based upon this balance, overall accuracy may surpass full 3D scans which may have limited temporal contrast.

[0024] FIG. 1 shows a flow diagram that illustrates a process 100 performed in accordance with embodiments of the present system. The process may perform a multi-slice acquisition in real time. The process 100 may be performed using one or more computers communicating over a network and may obtain information from, and/or store information to one or more memories which may be local and/or remote from each other. The process 100 can include one or more of the following acts performed by a processor or other device configured to perform the following acts. In some embodiments, the acts of process 100 may be performed using an ultrasound imaging system including the processor operating in accordance with embodiments of the present system. Further, one or more of these acts may be combined and/or separated into sub-acts, if desired, or one or more of these acts may be skipped depending upon settings. In operation, the process may start during act 101 and then proceed to act 105. It is noted that the process of FIG. 1 is one example embodiment of processes provided in the present disclosure. The process steps described further herein can be carried

out, e.g., in a non-sequential fashion and in any desired order for producing a useful result in an imaging procedure. For example, the image planes that will be displayed can be changed while acquiring and displaying the image data. The number N of image planes being acquired can also be changed in real-time during imaging. Moreover, the image planes being stored can be changed and modified during imaging. For instance, a single set of planes or a loop of sets of image planes can be selected during an imaging procedure, or prior to using presets in the system.

[0025] Moving to act 105, the process can include determining a number of image planes to be scanned as the plurality of image planes. The discussion below will describe N image planes, but it can also apply to N' image planes. The value of the number of image planes used is represented by N, where N is an integer that can be greater than two. The value of N may be selected by the user of the system and defines a number of image planes (e.g., a plurality of fanned out image planes) to be acquired in a multi-slice image acquisition of an anatomical object of interest, such as a tumor. The N image planes may be at an angle to each other (e.g., fanned out) and may intersect the object-of-interest to be acquired. The N image planes that are at an angle to each other may be arranged in spacing that is representative of a sector image that is typically displayed in B-mode ultrasound imaging. The N planes may also be equidistant or not equidistant from each other.

[0026] In some embodiments, the number N of image planes used for a scanning procedure can abide by the following equation:

$$2 < N < N_{3D}, \quad \dots \quad \text{Eq. (1)}$$

where N_{3D} is a typical number of planes acquired in real-time 3D imaging. Accordingly, the scan time using the present system is less than scan times used in typical 3D imaging. In some embodiments, a value of N may be set to about 5 to 10, and N_{3D} could be between 32 to 160 frames. However, the number of N or N' image planes can be readily set by a user or provided, e.g., in a preset or default configuration for a given procedure. For example, in some embodiments, a number for N may be directly input from a user depending on the desired application. Accordingly, the process can include employing a user interface (UI) such as a menu or input keys which may be physical keys or software keys displayed on a touch sensitive display (e.g., a rotating knob, or other switches, such as a sliding switch, up-down arrows, menu list for selection etc.) with which a user may interact to enter or otherwise select a value of N. In some embodiments, physical keys and knobs associated with traditional ultrasound cart-based systems can be used.

[0027] In some embodiments, the value of N may be determined based upon, for example, a desired temporal or spatial resolution of an imaging volume. Thus, for example, as a user increases the temporal resolution, N may be decreased. In yet other embodiments, a default value for N may be obtained from a memory of the system. For example, N may have a default value of 8. Further, in yet other embodiments, the value of N may be set in accordance with user preferences obtained from a memory of the system. Accordingly, the process may identify a current user and obtain user settings corresponding with the identified user from a memory of the system. Thus, for a first user, the process may set the value of N = 7 while for second user, the process may set the value of N = 9. However, N may also be an even number.

[0028] In yet other embodiments, it is envisioned that the value of N may be determined in accordance with patient parameters such as a patient's age, height, weight, etc. In yet other embodiments, a value of N may be determined based upon differences in size of tissue being imaged for a given scan (e.g., a heart scan, a liver scan, a gallbladder scan, a pancreas scan, a kidney scan, a general intestinal scan, etc. and/or combinations thereof). For larger tissue structures, N may be greater.

[0029] Further, in yet other embodiments, the process may include determining whether previous scan information (e.g. from a previous scan of the current patient and which includes a value of N) is available. Accordingly, if it is determined that previous scan information is available, the system may use the same value for N as was used in the previous scan information (if N is available). This may provide for matching of the N scan planes in the current and previous scans for the same patient. However, if it is determined that that previous scan information is not available, the system may use a default value of N (e.g., 5). Further, if it is determined that N from the previous scan information is equal to 1 (e.g., only a single scan plane was obtained), the process may set N equal to a default value, e.g., 5.

[0030] In yet other embodiments, N may be determined based upon a look-up table. For example, parameters may be stored in a memory of the system in any suitable form such as a scan parameter table. Thereafter, the process may include using the scan parameter table to determine a value of N in accordance with entries of the scan parameter table. The scan parameter table may be set and/or reset by the system and/or user. Accordingly, the process may include providing the user with user interface with which the user may interact to set and/or reset the parameters of the scan parameter table, if desired.

[0031] As described herein, a single image plane of the plurality of image planes (e.g., the N image planes) can be rendered on a display of the imaging system in real-time, while a bi-plane (e.g., an orthogonal image plane of the plurality

of image planes (e.g., the N image planes)) can also be rendered on the display in real-time. As will be referred to herein, a selected scan plane (SSP) (selected image plane) refers to a single selected image plane that is displayed among the plurality of image planes that are acquired. A selected scan plane (SSP) may also refer to two selected bi-plane (e.g., orthogonal) image planes that are displayed. For example, a selected N image plane and a respective N' image plane can be displayed in real-time. While the following description will mostly refer to acquiring and storing N image planes and displaying a single selected plane, it is equally applicable to embodiments where N, N' image planes are acquired and stored (e.g., where the N image planes are orthogonal to the N' image planes) and only two image planes of the acquired and stored N, N' image planes are actually displayed.

[0032] As will be described further below with reference to acts 117 and 119, the DNSP refers to scan planes which are not to be displayed and may be optionally included in some embodiments, if desired. For example, with regard to imaging a tissue of interest (e.g. a tumor or organ), six image planes (N=6) may intersect the tissue of interest during imaging. Scan plan 4 will be displayed during the scan. Scan planes that are not to be displayed (e.g., the DNSPs) are scan planes 1, 2, 3, 5, and 6. Any suitable format may be used. In some embodiments, the values of N, SSP, DNSPs, may be set in accordance with a user's settings. After completing act 105, the process may continue to act 109.

[0033] During act 109, the process may include acquiring echo information from the N image planes that intersect the object-of-interest (e.g., a tumor of the patient in the present example). Alternatively, N image planes that intersect at an angle (e.g., orthogonally) with N' image planes are acquired during act 109. Accordingly, the process may include controlling an ultrasonic probe including a transducer array (e.g., a 2D matrix array transducer) to transmit ultrasonic pulses which intersect object of interest the N planes and to acquire echo information for each of the N planes in return. More particularly, the process may include controlling the probe(s) to obtain echo information corresponding with a real-time acquisition of the N scan planes.

[0034] During act 109, the process may further include obtaining echo information for at least one N' image plane (e.g., a bi-plane) that is at an angle (e.g., orthogonal) to the group of N image planes. If it is determined that only N image planes will be scanned, then the process will not obtain any N' image planes. If it is determined that a bi-plane image is to be acquired, the process may include obtaining the at least one N' image plane and, therefore, may include obtaining echo information for the at least one N' image plane. After completing act 109, the process may continue to act 113.

[0035] During act 113, the process may include generating image information for each of the N image planes based upon the acquired echo information received for each of the N image planes, respectively. The process may include generating the image information using any suitable methods generally well known in the art. In one embodiment, the process may include acquiring and generating multi-frame data using a Live-iSlice™ environment. The image information for each of the N scan planes may also be used to generate volume data. Further, the process may generate image information for the at least one N' image plane based upon the acquired echo information for the N' scan plane. After completing act 113, the process may continue to act 117.

[0036] During act 117, the process may include selecting images for real-time display during a scanning operation. In some embodiments, a single image plane of the N image planes is selected and displayed. In certain embodiments, a bi-plane image plane is displayed that is at an angle (e.g., orthogonal) to the N image planes, and if a plurality of N' image planes are acquired then one of the N' image planes is selected for display. The N image or bi-plane image (e.g., an N' image) selected for display can be displayed to a user in a suitable format, e.g., as a square, rectangle or as a sector image. The N image or bi-plane image (e.g., an N' image) may be selected by the process and/or user. For example, a default setting for which selected N or N' image may be obtained from a memory of the system and/or from a user through selection. Accordingly, the process may include providing a user with a user interface with which the user may interact (e.g., a knob, a menu, etc.) to select an image to display (e.g., before or during a scan, if desired).

[0037] In some embodiments, a process of elimination may be used to select the N image and/or N' image to display. For example, the displayed image may be selected among the N or N' image planes being acquired and stored. The other remaining N or N' image planes that are not displayed are referred to as DNSPs. In one embodiment, assuming that N=6, and the slices that are not to be displayed (e.g., DNSPs) are slices 1, 2, 3, 5, and 6, the process may determine that the image plane to display is the 4th slice. Thus, in some embodiments, the DNSPs are determined first and, thereafter, the image plane to display may be determined. In yet other embodiments the N image or N' image to display may be determined based upon a user's ID. Accordingly, in these embodiments, the process may identify the user, obtain the user's settings from a memory of the system, and thereafter set the N image planes or N' image planes in accordance with the user's settings. After completing act 117, the process may continue to act 119. It is also noted that acts 117 and 119 can be carried out in a different order of the process. For example, act 117 and/or 119 can be implemented after act 105 when the number of slices or image planes to be acquired is determined.

[0038] During act 119, the process may select the DNSPs. The DNSPs may include (N-1) of the N image planes, or (N'-1) of the N' image planes being acquired during a scan. The DNSPs are image planes that are stored but not displayed (e.g., non-display slices) in real time. The DNSPs may be selected using any suitable method such as from a memory of the system and/or from a user input. It is further envisioned that the DNSPs may further be set in accordance with the type of tissue being scanned (e.g., liver scan, heart scan, etc.). In yet other embodiments, once the value of N and

the image plane to be displayed are determined the DNSPs may be determined using a process of elimination. Thus, if it is determined that $N=7$ and the image plane to be displayed is 4, then the process may determine that the DNSPs are 1, 2, 3, 5, 6, and 7. A similar process applies to selection among N' image planes that are orthogonal to the N image planes. In one embodiment, a single bi-plane image is selected, but other N' image planes can also be selected and displayed.

[0039] Referring back to the N image plane slices, in accordance with some embodiments, it is envisioned that the location, spacing, thickness, depth and/or orientation of the DNSPs slices may be set by the process and/or user. In some embodiments, if other values, settings, and/or parameters are necessary, the process may include obtaining corresponding default values from a memory of the system. After completing act 119, the process may continue to act 121.

[0040] During act 121, the process may include forming a real-time display frame (RTDF) for rendering on a display of the system. All ultrasound images generated of the object-of-interest which are to be displayed in real time, such as the SSP and, e.g., an orthogonal image plane to the SSP, are to populate the RTDF. However, images planes which are not to be displayed, such as the DNSPs, are not to populate the RTDF.

[0041] During act 123, the process may include determining whether only N image planes are to be acquired during imaging. This is referred to FIG. 1 as a 2D scan. If it is determined that only N image planes will be acquired, the process may continue to act 137. However, if it is determined that at least one N' image plane will be displayed and/or acquired, then the process may continue to act 133 in which the real-time display frame will display at least one of the N' image planes, such as an N' image plane orthogonal to the N image planes in the 2D scan. The system and/or user may select whether N and/or N' image planes will be stored and/or displayed. For example, in some embodiments, the process may provide a user with a user interface (e.g., knobs, menus) with which to interact with the system to select which image planes will be stored and/or displayed. This setting may be performed at any time such as during an initial setup process. In yet other embodiments, depending upon a type of scan being performed (e.g., liver CEUS, etc.), the process may select a default configuration or user preferences for N and/or N' image planes to be stored and/or displayed.

[0042] The RTDF may include a continuous or discontinuous area(s) and may have a shape and/or size which may be selected by the system (e.g., default, by test type, by test parameters, etc.) or the user. Thus, the RTDF may be populated with image information for a selected N image plane (e.g., including a region-of-interest, if desired) and the image information for an N' image plane (e.g., an orthogonal N' image plane), and any associated information such as measurements, axes, slice locations, highlighting, etc. In some embodiments, the RTDF may include null information. For example, FIG. 2 shows a portion of a screenshot of the RTDF 200 including an ultrasound image 202 that corresponds to an N image plane (e.g., a slice within the region-of-interest, if desired), where image 202 includes image information of the region of interest, e.g., a tumor 14, in accordance with embodiments of the present system. The RTDF 200 may further include an ultrasound image 204 corresponding to an N' image plane that is at an angle (e.g., orthogonal) to the N image plane corresponding ultrasound image 202. A line 204a may be overlaid over the N image plane ultrasound image 202 to identify where the bi-plane ultrasound image 204 is located in relation. Other lines 206a, 206b, 206c, and 206d can be overlaid and displayed to show where other N' image planes are being imaged and stored, but not displayed. FIG. 2 shows solid and dashed lines over the image, but other indicators can be used to tell a user which lines are being displayed and which are just being stored. For example, opposing carats, stars, or other icons could be positioned on the outer edge of the image and shown, e.g., with different colors. The lines or other markings over the image could also be removed from the display to allow for better image viewing. In general, this information indicates to a user the number of the N of planes being acquired and their locations relative to each other. Of course, because the N image planes are orthogonal to the N' image planes, ultrasound image 202 could correspond to an N' image plane and ultrasound image 204 could correspond to an orthogonal N image plane. Similarly, the lines 204a and 206a-206d could correspond to N image planes. The ultrasound image 202 may be formed by the process using any suitable imaging method known in the art and could be displayed in a modified iSlice™ environment operating in accordance with embodiments of the present system. Also shown in FIG. 2, a distance d_s indicates an angular distance between adjacent imaging planes of the N or N' imaging planes. In some embodiments, the image planes may be parallel in which d_s may refer to units in mm. The angular distance d_s between each of the imaging planes may be equal (e.g., N imaging planes may be equidistant from each other). However, in yet other embodiments, the imaging planes may be unequally spaced as may be set by the system and/or user. N and d_s may be (inversely) related. For example, increasing N may cause d_s to decrease and vice versa. After completing act 121, the process may continue to act 123.

[0043] In some embodiments, act 133 can include populating the RTDF 300 with image information for both an ultrasound image 304 corresponding to an N image plane and an ultrasound image 304' corresponding to an N' image plane, as shown in FIG. 3. Further, the process may determine locations of each of the N image planes and show them as lines 306a-306d. Lines 306'a-306'd correspond to N' image planes that are orthogonal to the N image planes. The projection of the lines 304, 304', 306a-d, and 306'a-d can be shown in the RTDF 300 in a direction that is oriented orthogonal from the face of a 2D array transducer, such as an X-matrix transducer. This view can give the user an idea of how the image planes are oriented in respect to the azimuthal and elevational dimensions of the probe. In FIG. 3, the RTDF 300 includes the display of an N' image plane 304 and an orthogonal N' image plane 304'. As shown the images are displayed in

rectangular form, but the sector shape image format shown in FIG. 2 can also be used. The solid lines 304 and 304' indicate the image plane that is being displayed, and the dotted lines (e.g., 306'a) indicate the DNSPs.

[0044] After completing act 133, the process may continue to act 137. In some embodiments, the process may fit the RTDF to information to be displayed therein, to a desired format, and/or to a rendering device such as a display of the system. During act 137, the process may render the ultrasound image 202 on a display of the system in real-time, or render at least one N' image plane (e.g., the two orthogonal ultrasound images 304, 304').

[0045] FIG. 4 shows a portion of a screen shot 400 of a graphical user interface (GUI) 402 including an RTDF 404. As shown in FIG. 4, the RTDF 404 includes two 2D images next to each other 10 and 12. Image 12 on the right side of FIG. 4 is an orthogonal image plane to the image plane acquired to display image 10. In this embodiment, the images 10 and 12 can be used to tell the user that they are aligned in the middle of the tumor 14. Dashed lines 16 in FIG. 4 are tissue structures. As shown, the lines overlaid on image 10 are numbered 1-5, where scan line 3 corresponds to the position of the image plane that is used to generate image 12. Lines 1, 2, 4, 5 correspond to other image planes that are orthogonal to the image plane used to generate image 10 (similar to 206a-206d in FIG. 2). Typically, lines 1, 2, 4 and 5 are stored by the system, but not shown for display. Only image 12, which corresponds to line 3, is displayed. In FIG. 4, the images corresponding to lines 1-5 are also shown as five smaller images 18 showing the different slices or cross sections of the tumor 14 in space. The cross section at the center of the tumor 14 is shown in images 12 and 3, where the center cross tumor section shown in image 3 is larger than the side or off-center cross sections shown in images of the tumor slices 1, 2, 4, 5.

[0046] The solid line 3 in image 10 indicates the location of cross section within the tumor 14 (namely, though the center of the tumor 14) shown in an adjacent image that is being displayed in real-time as image 12 in the right panel of the interface. The dashed lines 1, 2, 4, 5 in image 10 indicate that these off-center tumor slices are available for selection by the user for display on the right panel of the interface (i.e., the side of FIG. 4) instead of the currently displayed image 12. Of course, if desired, more than one tumor slice may be displayed next to image 10, where even all the available tumor slices 1-5 may be simultaneously displayed. However, this clutters the GUI and may cause confusion. Accordingly, only the single ultrasound image corresponding to line 3 is displayed in image 12.

[0047] The dashed lines for 1, 2, 4, 5 also show the user what other images (besides the displayed image 12) are being acquired during the scan but not shown, as currently the selected image shown in the image 12 is the center tumor slice as this center slice is selected by the user as indicated by the solid line 3 in image 10. That is, the various cross-sections of the tumor 14 along image planes 1-5 are stored, while only image plane 3 (selected by the user) is being shown as the orthogonal image 12. The stored cross-section images can then be reviewed offline and used for quantification, for example, and/or also displayed in additional images next to currently images 10, 12 shown in FIG. 4.

[0048] It should be noted that while the user can also select the scan density or number of planes or slices of the object of interest, e.g., a tumor to be acquired in real time. Thus, instead of the 5 planes or slices shown in FIG. 4, the user may change the scan density, such as increase the real-time acquired slices from 5 to 10 for example. Further, additional slices may be acquired in real-time at different angles. For example, in addition to the 5 planes or slices 1-5, further 5 planes or slices 1'-5' (not shown) may also be acquired and displayed as an image, where the further slices 1'-5' are orthogonal to the slices 1-5. The two orthogonal middle slices 3, 3' may be used to better define the center of the tumor 14, as shown by a bulls-eye center. An additional image can be displayed next to image 12, similar to image 304' shown displayed next to image 304 in FIG. 3, where the two images 304, 304' are orthogonal to each other for example.

[0049] The GUI 402 may include the RTDF 404 and a menu with which the user may interact with the process and/or system. Accordingly, the menu may include information such as values of N, and SSP, DNSPs, a type of scan, Region of Interest, etc. which may be listed in boxes 422, 418, 416, 423, 424, respectively. Further, the UI 402 may include day, date, time information 408, information related to the scanner such as machine ID 410, information related to professionals who run and/or ordered the scan such as doctor ID 406 and user ID (e.g., sonographer) 412. The GUI 402 may further include information which may identify a patient such as patient ID 414. A soft key 420 may be selected to change a value the SSP, if desired. In yet further embodiments, a user may, for example, control the position and/or number of underlying acquired scan planes corresponding with the N and/or N' image slices using, for example, rotary knobs on the ultrasound scanner control panel, as may be desired. Alternatively, a touch panel may also be integrated into the system for user controls.

[0050] In some embodiments, selecting N image planes may automatically result in selection of N' image planes. For example, if N is selected to be 2 (i.e., SSP=2), then image information is displayed for both orthogonal slices 2 and 2' (i.e., SSP'=2), for display as two images, such as images 304, 304' shown in FIG. 3. After completing act 137, the process may continue to act 141.

[0051] During act 141, the process may include storing any or select information generated and/or otherwise used by the process in a memory of the system for later use. For example, the echo information, the generated image information for each of N image planes, the image information for the orthogonal frame, the RTDF, parameter settings such as N, SSP, DNSPs, a patient's name, the professional performing the scan, the type of scan, the date of scan, a doctor's name (who ordered the scan), etc., may be stored in a memory of the system for later use such as for off-line quantification

or other post-processing. Additionally, the stored information may be used for determining parameters for later scans such as for later CEUS scans, etc. Data used by, obtained by, and/or otherwise generated by, the present system may be stored in any suitable archiving system such as a Picture Archiving System. Moreover, by controlling the value of N to be less than N_{3D} , the number of scan planes is reduced which can conserve system resources and reduce or prevent data workflow challenges. After completing act 141, the process may repeat act 105 or may continue to act 145, where it ends, if desired.

[0052] An off-line process operating in accordance with embodiments of the present system may also be used to perform quantitative analysis on the data generated by the process such as the image information for the N image planes. For example, quantification analysis could be used to sum up intensity in a region (e.g., a tumor) of an image during a CEUS procedure. The intensity quantification could be used to indicate an amount of vasculature present in the tumor, especially in applications where intensity is related to presence of contrast media in blood in the tissue. It is further envisioned that a modified Live-iSlice™ method operating in accordance with embodiments of the present system may be performed using a matrix transducer to provide enhanced frame rate and workflow over conventional methods.

[0053] Embodiments of the present system may perform data imaging in real-time for N image planes, where $2 < N < N_{3D}$, where N_{3D} is a typical number of planes acquired in real-time 3D imaging. Further, embodiments of the present system may allow the operator to control the number of scan planes N, so that the operator can adjust N to reach an acceptable trade-off between spatial sampling of the tumor and frame rate. However, during use, embodiments of the present system may render only a single scan plane of the N scan planes in real-time. Accordingly, as a user has to follow only a single scan plane in an enhanced user interface (UI) real time (as opposed to a plurality of scan planes in real-time), user distraction and confusion may be reduced or entirely prevented.

[0054] Embodiments of the present system may provide data at a higher volume rate than conventional real-time 3D systems. This may be advantageous when performing CEUS methods and may result in increased result accuracy. Further, by providing a user interface (UI) operating in accordance with embodiments of the present system, undue distraction at a critical time may be prevented. This may result in more accurate test results and/or fewer failed exams.

[0055] As analysis of a three-dimensional (3D) structure such as a tumor, based upon information obtained from using single scan plane may be unreliable, and as full 3D scans may have temporal and spatial limitations, embodiments of the present system provide advantages both of these methods. For example, by providing N scan planes wherein N is greater than 2 and less than a number (e.g., N_{3D}) of scan planes obtained using a full 3D scan, embodiments of the present system may enhance temporal and spatial contrast over existing systems thus allowing faster and more accurate scan analysis. This enhancement may be desirable for clinical validation and broad adoption of methods used by embodiments of the present system.

[0056] Moreover, by providing image information related to a plurality of scanned image planes (e.g., the N scan planes), it may be easier to match image information obtained from at least one currently-derived scan plane with image information of a scan plane from a previous scan (e.g., obtained earlier and stored in a memory of the system) for comparison using, for example image processing methods. Accordingly, by more closely matching current and previous scan planes, CEUS methods to determine parameters operating in accordance with embodiments of the present method may provide increased accuracy over conventional CEUS methods. This may be beneficial for therapy monitoring. Moreover, similar benefits may be obtained using embodiments of the present system for characterization studies using 2D CUES methods to collect information from a plurality of scan planes (such as N scan planes) of a tumor so as to characterize the tumor. For example, by obtaining information about a plurality of scan planes in the tumor, a characterization of the tumor which is more representative of characteristics of the overall tumor may be obtained as opposed to information collected using a single plane.

[0057] Referring to FIG. 5, an ultrasound system 510 constructed in accordance with the principles of the present invention is shown in block diagram form. The ultrasound system is configured by two subsystems, a front end acquisition subsystem 510A and a display subsystem 510B. An ultrasound probe is coupled to the acquisition subsystem which includes a two-dimensional matrix array transducer 570 and a micro-beamformer 572. The micro-beamformer contains circuitry which control the signals applied to groups of elements ("patches") of the array transducer 570 and does some processing of the echo signals received by elements of each group. Micro-beamforming in the probe advantageously reduces the number of conductors in the cable between the probe and the ultrasound system and is described in U.S. Pat. No. 5,997,479 (Savord et al.) and in U.S. Pat. No. 6,436,048 (Pesque), and provides electronic steering of beams on transmit and receive for high frame rate real-time (live) imaging.

[0058] The probe is coupled to the acquisition subsystem 510A of the ultrasound system. The acquisition subsystem includes a beamform controller 574 which is responsive to a user control 536 and provides control signals to the microbeamformer 572, instructing the probe as to the timing, frequency, direction and focusing of transmit beams. The beamform controller also controls the beamforming of echo signals received by the acquisition subsystem by its control of analog-to-digital (A/D) converters 518 and a beamformer 520. Partially beamformed echo signals received by the probe are amplified by preamplifier and TGC (time gain control) circuitry 516 in the acquisition subsystem, then digitized by the A/D converters 518. The digitized echo signals are then formed into fully steered and focused beams by a main

system beamformer 520. The echo signals are then processed by an image processor 522 which performs, e.g., digital filtering, B mode detection, and can also perform other signal processing such as harmonic separation, speckle reduction, and other desired image signal processing.

[0059] The echo signals produced by the acquisition subsystem 510A are coupled to the display subsystem 510B, which processes the echo signals for display in the desired image format. The echo signals are processed by an image line processor 524, which is capable of sampling the echo signals, splicing segments of beams into complete line signals, and averaging line signals for signal-to-noise improvement or flow persistence. The image lines for a 2D image are scan converted into the desired image format by a scan converter 526 which performs R-theta conversion as is known in the art. The scan converter can thus format rectilinear or sector image formats. The image is then stored in an image memory 528 from which it can be displayed on a display 538. The image in memory is also overlaid with graphics to be displayed with the image, which are generated by a graphics generator 534 which is responsive to the user control 536 so that the graphics produced are associated with the images of the display. Individual images or image sequences can be stored in a cine memory 530 during capture of image loops or sequences. With respect to FIG. 2, for example, the ultrasound imaging system is configured to display an ultrasound image 202 corresponding the selected N image plane and/or an ultrasound image 204 corresponding to an N' image plane as acquired by the matrix array transducer. The lines (e.g. 206a) can be displayed over the displayed image through the graphics generator.

[0060] The 2D array transducer can be operated to acquire image data from at least one N or N' image plane. For example, the 2D array transducer can be used to generate images that correspond to image planes 206a, 206b, 204a, 206c, and 206d of FIG. 2. When the matrix array probe is operated to scan both N image planes and N' image planes (e.g., as in FIG. 3), selected by the controls of the control panel 536, the beamform controller 574 is controlled to alternately acquire images of two different image planes in rapid, real-time succession. The controls of the control panel 536 can also be used to select the desired angle and orientation of the various imaging planes that are being scanned, e.g., the rotate, tilt, or elevation tilt can be modified. The live images of the two N and N' image planes can be displayed side-by-side as shown in FIG. 2. In one embodiment, the sonographer can hold the matrix array probe steady so that the target anatomy is constantly displayed in the N' plane image 202, and then manipulate a control of the control panel to tilt, rotate, or elevate the N' image plane to generate the image 204. In accordance with the principles of the present invention, the biplane images may be displayed, stored, and/or exported either in the standard format with both images in the same display frame, or as independent images. Moreover, while not shown, the system can further include a 3D processor, which can be used to display 3D volumes if desired.

[0061] Embodiments of the present system may be compatible with ultrasound systems having a matrix transducer such as Philips™ X5-1, X6-1, X7-2, and X7-2t matrix transducers and the like. It is further envisioned that embodiments of the present system may provide improved systems and methods for applications which may require (on-line or off-line) visualization and/or quantification of multiple scan planes such as tumor therapy monitoring.

[0062] While the present invention has been shown and described with reference to particular exemplary embodiments, it will be understood by those skilled in the art that present invention is not limited thereto, but that various changes in form and details, including the combination of various features and embodiments, may be made therein without departing from the spirit and scope of the invention.

[0063] Further variations of the present system would readily occur to a person of ordinary skill in the art and are encompassed by the following claims.

[0064] Finally, the above-discussion is intended to be merely illustrative of the present system and should not be construed as limiting the appended claims to any particular embodiment or group of embodiments. Thus, while the present system has been described with reference to exemplary embodiments, it should also be appreciated that numerous modifications and alternative embodiments may be devised by those having ordinary skill in the art without departing from the broader and intended spirit and scope of the present system as set forth in the claims that follow. The specification and drawings are to be regarded in an illustrative manner and are not intended to limit the scope of the appended claims.

[0065] In interpreting the appended claims, it should be understood that:

- a) the word "comprising" does not exclude the presence of other elements or acts than those listed in a given claim;
- b) the word "a" or "an" preceding an element does not exclude the presence of a plurality of such elements;
- c) any reference signs in the claims do not limit their scope;
- d) several "means" may be represented by the same item or hardware or software implemented structure or function;
- e) any of the disclosed elements may be comprised of hardware portions (e.g., including discrete and integrated electronic circuitry), software portions (e.g., computer programming), and any combination thereof;
- f) hardware portions may be comprised of one or both of analog and digital portions;
- g) any of the disclosed devices or portions thereof may be combined together or separated into further portions unless specifically stated otherwise;
- h) no specific sequence of acts or steps is intended to be required unless specifically indicated; and

i) the term "plurality of" an element includes two or more of the claimed element, and does not imply any particular range of number of elements; that is, a plurality of elements may be as few as two elements, and may include an immeasurable number of elements.

Claims

1. An ultrasound imaging system (510) for imaging a region of interest (14) of a subject, comprising a controller configured to:

- determine a number (N, N') of a plurality of image planes to scan through the region of interest (14);
- acquire echo information corresponding to each of the image planes in the plurality;
- generate image information for each of the image planes based upon the acquired echo information; and
- store the image information corresponding to each of the image planes in a memory (528) of the system;

wherein the controller is further configured to:

- display an ultrasound image (202, 204) comprising the region of interest (14), wherein the ultrasound image is rendered for display from generated image information for a single selected image plane of the plurality of image planes, wherein the selected image plane is one of a first plurality of the plurality of image planes, the first plurality of the plurality of image planes being at an angle to a second plurality of the plurality of image planes, the remaining image planes of the first plurality of the plurality of image planes not being displayed; and
- render, in real time on the display (538), a plurality of lines (204a, 206a-206d) that are overlaid on the ultrasound image (202) rendered from the generated image information for the selected image plane, the plurality of lines (204a, 206a-206d) being indicative of the second plurality of the plurality of image planes scanned through the region of interest (14).

2. The system of claim 1, wherein the controller is further configured to render another ultrasound image (204) on the display (538) in real-time based on image information from a single image plane of the second plurality of the plurality of image planes corresponding to a selected line (204a) of the plurality of lines, and wherein the selected line (204a) is displayed differently from the remaining lines (206a-206d) of said plurality of lines on the display (538), the remaining lines (206a-206d) corresponding to the remaining image planes of the second plurality of the plurality of image planes that are acquired and stored but not displayed.

3. The system of claim 1, wherein the controller is further configured to render a plurality of smaller images (18) on the display (538), each of the plurality of smaller images (18) corresponding to an image plane of the second plurality of the plurality of image planes.

4. The system of claim 1, wherein the stored image information comprises image information corresponding to the selected image plane, which is rendered in real time, and image information corresponding to image planes, which are not rendered in real time.

5. The system of claim 1, wherein the controller is further configured to generate a time-intensity curve which represents contrast uptake based upon image information corresponding to the plurality of image planes.

6. The system of claim 5, wherein the controller is further configured to determine parameters comprising one or more of peak intensity, area under the time-intensity curve, rise time, and mean transit time based upon the generated time-intensity curve.

7. The system of claim 1, further comprising a user interface (536) configured to enable a user to select an image plane of the plurality of image planes.

8. The system of claim 1, wherein the number (N) of the first plurality of the plurality of image planes is between 2 and N_{3D} , wherein N_{3D} is between 32 and 160.

9. A method (100) of displaying ultrasound images, the method comprising:

- determining (105) a number (N, N') of a plurality of image planes to scan through a region of interest (14) of

a subject;

- acquiring (109) echo information corresponding to each of the image planes in the plurality;
- generating (113) image information for each of the image planes based upon the acquired echo information; and
- storing (141) the image information corresponding to each of the image planes in a memory (528);

wherein the method further comprises:

- displaying (137) an ultrasound image (202, 204) comprising the region of interest (14), wherein the ultrasound image is rendered (121) for display from generated image information for a single selected image plane of the plurality of image planes, wherein the selected image plane is one of a first plurality of the plurality of image planes, the first plurality of the plurality of image planes being at an angle to a second plurality of the plurality of image planes, the remaining image planes of the first plurality of the plurality of image planes not being displayed; and
- rendering, in real time on the display (538), a plurality of lines (204a, 206a-206d) that are overlaid on the ultrasound image (202) rendered from the generated image information for the selected image plane, the plurality of lines (204a, 206a-206d) being indicative of the second plurality of the plurality of image planes scanned through the region of interest (14).

10. The method of claim 9, comprising rendering (133) another ultrasound image (204) on the display (538) in real-time based on image information from a single image plane of the second plurality of the plurality of image planes corresponding to a selected line (204a) of the plurality of lines, and wherein the selected line (204a) is displayed differently from the remaining lines (206a-206d) of said plurality of lines on the display (538), the remaining lines (206a-206d) corresponding to the remaining image planes of the second plurality of the plurality of image planes that are acquired and stored but not displayed.

11. The method of claim 9, wherein the stored image information comprises image information corresponding to the selected image plane, which is rendered in real time, and image information corresponding to image planes, which are not rendered in real time.

12. The method of claim 9, comprising generating a time-intensity curve which represents contrast uptake based upon image information corresponding to the plurality of image planes.

13. The method of claim 12, comprising determining parameters comprising one or more of peak intensity, area under the time-intensity curve, rise time, and mean transit time based upon the generated time-intensity curve.

14. The method of claim 9, wherein the first plurality of the plurality of image planes are parallel to each other or fanned out in space, and wherein first plurality of the plurality of image planes are orthogonal to the second plurality of the plurality of image planes.

15. A computer program stored on a non-transitory computer readable memory medium, the computer program being configured to render ultrasonic image information and comprising program portions which, when executed by a processor, configure the processor to perform the method of any of claims 9-14.

Patentansprüche

1. Ultraschallbildgebungssystem (510) zur bildgebenden Darstellung einer interessierenden Region (14) eines Patienten, umfassend eine Steuereinheit, die konfiguriert ist zum:

- Ermitteln einer Anzahl (N, N') von einer Vielzahl von Bildebenen, die durch die interessierende Region (14) zu scannen sind;
- Erfassen von Echoinformationen, die jeder der Bildebenen in der Vielzahl entsprechen;
- Erzeugen von Bildinformationen für jede der Bildebenen basierend auf den erfassten Echoinformationen; und
- Speichern der Bildinformationen, die jeder der Bildebenen entsprechen, in einem Speicher (528) des Systems;

wobei die Steuereinheit ferner konfiguriert ist zum:

- Anzeigen eines die interessierende Region (14) umfassenden Ultraschallbilds (202, 204), wobei das Ultra-

schallbild anhand der erzeugten Bildinformationen für eine einzelne ausgewählte Bildebene der Vielzahl von Bildebenen zur Anzeige gerendert wird, wobei die ausgewählte Bildebene eine von einer ersten Vielzahl der Vielzahl von Bildebenen ist, wobei die erste Vielzahl der Vielzahl von Bildebenen in einem Winkel zu einer zweiten Vielzahl der Vielzahl von Bildebenen angeordnet ist, wobei die restlichen Bildebenen der ersten Vielzahl der Vielzahl von Bildebenen nicht angezeigt werden; und

- Rendern, in Echtzeit auf der Anzeige (538), einer Vielzahl von Linien (204a, 206a-206d), die dem anhand der erzeugten Bildinformationen für die ausgewählte Bildebene gerenderten Ultraschallbild (202) überlagert sind, wobei die Vielzahl von Linien (204a, 206a-206d) die zweite Vielzahl der Vielzahl von Bildebenen angibt, welche durch die interessierende Region (14) gescannt werden.

2. System nach Anspruch 1, wobei die Steuereinheit ferner konfiguriert ist, um ein weiteres Ultraschallbild (204) auf der Anzeige (538) in Echtzeit basierend auf Bildinformationen aus einer einzelnen Bildebene der zweiten Vielzahl der Vielzahl von Bildebenen zu rendern, die einer ausgewählten Linie (204a) der Vielzahl von Linien entspricht, und wobei die ausgewählte Linie (204a) anders als die restlichen Linien (206a-206d) der genannten Vielzahl von Linien auf der Anzeige (538) angezeigt wird, wobei die restlichen Linien (206a-206d) den restlichen Bildebenen der zweiten Vielzahl der Vielzahl von Bildebenen entsprechen, welche erfasst und gespeichert, aber nicht angezeigt werden.

3. System nach Anspruch 1, wobei die Steuereinheit ferner konfiguriert ist, um eine Vielzahl von kleineren Bildern (18) auf der Anzeige (538) zu rendern, wobei jedes der Vielzahl von kleineren Bildern (18) einer Bildebene der zweiten Vielzahl der Vielzahl von Bildebenen entspricht.

4. System nach Anspruch 1, wobei die gespeicherten Bildinformationen Bildinformationen, die der ausgewählten in Echtzeit gerenderten Bildebene entsprechen, und Bildinformationen, die den nicht in Echtzeit gerenderten Bildebenen entsprechen, umfassen.

5. System nach Anspruch 1, wobei die Steuereinheit ferner konfiguriert ist, um eine Zeit-Intensität-Kurve, die die Kontrastmittelaufnahme darstellt, basierend auf den Bildinformationen zu erzeugen, die der Vielzahl von Bildebenen entsprechen.

6. System nach Anspruch 5, wobei die Steuereinheit ferner konfiguriert ist, um Parameter umfassend eines oder mehreres von Peak-Intensität, Fläche unter der Zeit-Intensität-Kurve, Anstiegszeit und mittlere Durchgangszeit basierend auf der erzeugten Zeit-Intensität-Kurve zu ermitteln.

7. System nach Anspruch 1, ferner umfassend eine Benutzeroberfläche (536), die konfiguriert ist, um einem Benutzer zu ermöglichen, eine Bildebene von der Vielzahl von Bildebenen auszuwählen.

8. System nach Anspruch 1, wobei die Anzahl (N) der ersten Vielzahl der Vielzahl von Bildebenen zwischen 2 und N_{3D} beträgt, wobei N_{3D} zwischen 32 und 160 beträgt.

9. Verfahren (100) zum Anzeigen von Ultraschallbildern, wobei das Verfahren Folgendes umfasst:

- Ermitteln (105) einer Anzahl (N, N') von einer Vielzahl von Bildebenen, die durch eine interessierende Region (14) eines Patienten zu scannen sind;
- Erfassen (109) von Echoinformationen, die jeder der Bildebenen in der Vielzahl entsprechen;
- Erzeugen (113) von Bildinformationen für jede der Bildebenen basierend auf den erfassten Echoinformationen; und
- Speichern (141) der Bildinformationen, die jeder der Bildebenen entsprechen, in einem Speicher (528);

wobei das Verfahren ferner Folgendes umfasst:

- Anzeigen (137) eines die interessierende Region (14) umfassenden Ultraschallbilds (202, 204), wobei das Ultraschallbild anhand der erzeugten Bildinformationen für eine einzelne ausgewählte Bildebene der Vielzahl von Bildebenen zur Anzeige gerendert wird (121), wobei die ausgewählte Bildebene eine von einer ersten Vielzahl der Vielzahl von Bildebenen ist, wobei die erste Vielzahl der Vielzahl von Bildebenen in einem Winkel zu einer zweiten Vielzahl der Vielzahl von Bildebenen angeordnet ist, wobei die restlichen Bildebenen der ersten Vielzahl der Vielzahl von Bildebenen nicht angezeigt werden; und
- Rendern, in Echtzeit auf der Anzeige (538), einer Vielzahl von Linien (204a, 206a-206d), die dem anhand der erzeugten Bildinformationen für die ausgewählte Bildebene gerenderten Ultraschallbild (202) überlagert sind,

wobei die Vielzahl von Linien (204a, 206a-206d) die zweite Vielzahl der Vielzahl von Bildebenen angibt, welche durch die interessierende Region (14) gescannt werden.

10. Verfahren nach Anspruch 9, umfassend das Rendern (133) eines weiteren Ultraschallbilds (204) auf der Anzeige (538) in Echtzeit basierend auf Bildinformationen aus einer einzelnen Bildebene der zweiten Vielzahl der Vielzahl von Bildebenen, die einer ausgewählten Linie (204a) der Vielzahl von Linien entspricht, und wobei die ausgewählte Linie (204a) anders als die restlichen Linien (206a-206d) der genannten Vielzahl von Linien auf der Anzeige (538) angezeigt wird, wobei die restlichen Linien (206a-206d) den restlichen Bildebenen der zweiten Vielzahl der Vielzahl von Bildebenen entsprechen, welche erfasst und gespeichert, aber nicht angezeigt werden.
11. Verfahren nach Anspruch 9, wobei die gespeicherten Bildinformationen Bildinformationen, die der ausgewählten in Echtzeit gerenderten Bildebene entsprechen, und Bildinformationen, die den nicht in Echtzeit gerenderten Bildebenen entsprechen, umfassen.
12. Verfahren nach Anspruch 9, umfassend das Erzeugen einer Zeit-Intensität-Kurve, die die Kontrastmittelaufnahme darstellt, basierend auf den Bildinformationen zu erzeugen, die der Vielzahl von Bildebenen entsprechen.
13. Verfahren nach Anspruch 12, umfassend das Ermitteln von Parametern umfassend eines oder mehreres von Peak-Intensität, Fläche unter der Zeit-Intensität-Kurve, Anstiegszeit und mittlere Durchgangszeit basierend auf der erzeugten Zeit-Intensität-Kurve.
14. Verfahren nach Anspruch 9, wobei die erste Vielzahl der Vielzahl von Bildebenen parallel zueinander oder im Raum aufgefächert sind, und wobei die erste Vielzahl der Vielzahl von Bildebenen orthogonal zu der zweiten Vielzahl der Vielzahl von Bildebenen angeordnet ist.
15. In einem nichtflüchtigen computerlesbaren Speichermedium gespeichertes Computerprogramm, wobei das Computerprogramm konfiguriert ist, um Ultraschallbildinformationen zu rendern, und Programmabschnitte umfasst, die bei Ausführung durch einen Prozessor den Prozessor dafür konfigurieren, das Verfahren nach einem der Ansprüche 9 bis 14 durchzuführen.

Revendications

1. Système d'imagerie ultrasonique (510) pour imager une région d'intérêt (14) d'un sujet, comprenant un dispositif de commande configuré pour :
 - déterminer un nombre (N, N') d'une pluralité de plans images à balayer à travers la région d'intérêt (14) ;
 - acquérir des informations d'écho correspondant à chacun des plans images de la pluralité ;
 - générer des informations d'image pour chacun des plans images sur la base des informations d'écho acquises ;
 - et
 - stocker les informations d'image correspondant à chacun des plans images dans une mémoire (528) du système ;
 dans lequel le dispositif de commande est en outre configuré pour :
 - afficher une image ultrasonique (202, 204) comprenant la région d'intérêt (14), dans lequel l'image ultrasonique est rendue pour un affichage à partir d'informations d'image générées pour un seul plan image sélectionné de la pluralité de plans images, dans lequel le plan image sélectionné est l'un d'une première pluralité de la pluralité de plans images, la première pluralité de la pluralité de plans images faisant un angle avec une seconde pluralité de la pluralité de plans images, les plans images restants de la première pluralité de la pluralité de plans images n'étant pas affichés ; et
 - rendre, en temps réel sur l'appareil d'affichage (538), une pluralité de lignes (204a, 206a-206d) qui sont superposées sur l'image ultrasonique (202) rendue à partir des informations d'image générées pour le plan image sélectionné, la pluralité de lignes (204a, 206a-206d) étant indicatives de la seconde pluralité de la pluralité de plans images balayés à travers la région d'intérêt (14).
2. Système selon la revendication 1, dans lequel le dispositif de commande est en outre configuré pour rendre une autre image ultrasonique (204) sur l'appareil d'affichage (538) en temps réel sur la base d'informations d'image

provenant d'un plan image unique de la seconde pluralité de la pluralité de plans images correspondant à une ligne sélectionnée (204a) de la pluralité de lignes et dans lequel la ligne sélectionnée (204a) est affichée différemment des lignes restantes (206a-206d) de ladite pluralité de lignes sur l'appareil d'affichage (538), les lignes restantes (206a-206d) correspondant aux plans images restants de la seconde pluralité de la pluralité de plans images qui sont acquis et stockés, mais non affichés.

3. Système selon la revendication 1, dans lequel le dispositif de commande est en outre configuré pour rendre une pluralité d'images plus petites (18) sur l'appareil d'affichage (538), chacune de la pluralité d'images plus petites (18) correspondant à un plan image de la seconde pluralité de la pluralité de plans images.

4. Système selon la revendication 1, dans lequel les informations d'image stockées comprennent des informations d'image correspondant au plan image sélectionné qui est rendu en temps réel et des informations d'image correspondant à des plans images qui ne sont pas rendus en temps réel.

5. Système selon la revendication 1, dans lequel le dispositif de commande est en outre configuré pour générer une courbe d'intensité dans le temps qui représente une prise de contraste sur la base d'informations d'image correspondant à la pluralité de plans images.

6. Système selon la revendication 5, dans lequel le dispositif de commande est en outre configuré pour déterminer des paramètres comprenant un(e) ou plusieurs d'une intensité de pic, d'une zone en dessous de la courbe d'intensité dans le temps, d'un temps d'augmentation et d'un temps de transit moyen sur la base de la courbe d'intensité dans le temps générée.

7. Système selon la revendication 1, comprenant en outre une interface utilisateur (536) configurée pour permettre à un utilisateur de sélectionner un plan image de la pluralité de plans images.

8. Système selon la revendication 1, dans lequel le nombre (N) de la première pluralité de la pluralité de plans images se situe entre 2 et N_{3D} , où N_{3D} se situe entre 32 et 160.

9. Procédé (100) d'affichage d'une image ultrasonique, le procédé comprenant :

- la détermination (105) d'un nombre (N, N') d'une pluralité de plans images à balayer à travers une région d'intérêt (14) d'un sujet ;
- l'acquisition (109) d'informations d'écho correspondant à chacun des plans images de la pluralité ;
- la génération (113) d'informations d'image pour chacun des plans images sur la base des informations d'écho acquises ; et
- le stockage (141) des informations d'image correspondant à chacun des plans images dans une mémoire (528) ;

dans lequel le procédé comprend en outre :

- l'affichage (137) d'une image ultrasonique (202, 204) comprenant la région d'intérêt (14), dans lequel l'image ultrasonique est rendue (121) pour un affichage à partir d'informations d'image générées pour un plan image sélectionné unique de la pluralité de plans images, dans lequel le plan image sélectionné est l'un d'une première pluralité de la pluralité de plans images, la première pluralité de la pluralité de plans images faisant un angle avec une seconde pluralité de la pluralité de plans images, les plans images restants de la première pluralité de la pluralité de plans images n'étant pas affichés ; et
- le rendu, en temps réel sur l'appareil d'affichage (538), d'une pluralité de lignes (204a, 206a-206d) qui sont superposées sur l'image ultrasonique (202) rendue à partir des informations d'image générées pour le plan image sélectionné, la pluralité de lignes (204a, 206a-206d) étant indicative de la seconde pluralité de la pluralité de plans images balayés à travers la région d'intérêt (14).

10. Procédé selon la revendication 9, comprenant le rendu (133) d'une autre image ultrasonique (204) sur l'appareil d'affichage (538) en temps réel sur la base d'informations d'image issues d'un plan image unique de la seconde pluralité de la pluralité de plans images correspondant à une ligne sélectionnée (204a) de la pluralité de lignes et dans lequel la ligne sélectionnée (204a) est affichée différemment des lignes restantes (206a-206d) de ladite pluralité de lignes sur l'affichage (538), les lignes restantes (206a-206d) correspondant aux plans images restants de la seconde pluralité de la pluralité de plans images qui sont acquis et stockés, mais non affichés.

11. Procédé selon la revendication 9, dans lequel les informations d'image stockées comprennent des informations d'image correspondant au plan image sélectionné qui est rendu en temps réel et des informations d'image correspondant à des plans image qui ne sont pas rendus en temps réel.

5 12. Procédé selon la revendication 9, comprenant la génération d'une courbe d'intensité dans le temps qui représente une prise de contraste sur la base d'informations d'image correspondant à la pluralité de plans images.

10 13. Procédé selon la revendication 12, comprenant la détermination de paramètres comprenant un(e) ou plusieurs d'une intensité de pic, d'une zone en dessous de la courbe d'intensité dans le temps, d'un temps de croissance et d'un temps de transit moyen sur la base de la courbe d'intensité dans le temps générée.

15 14. Procédé selon la revendication 9, dans lequel la première pluralité de la pluralité de plans images est parallèle les uns aux autres ou dispersée dans l'espace et dans lequel la première pluralité de la pluralité de plans images est orthogonale à la seconde pluralité de la pluralité de plans images.

20 15. Programme d'ordinateur stocké sur un support de mémoire lisible par ordinateur non transitoire, le programme d'ordinateur étant configuré pour rendre des informations d'image ultrasoniques et comprenant des parties de programme qui, lorsqu'elles sont exécutées par un processeur, configurent le processeur pour effectuer le procédé de l'une quelconque des revendications 9 à 14.

25

30

35

40

45

50

55

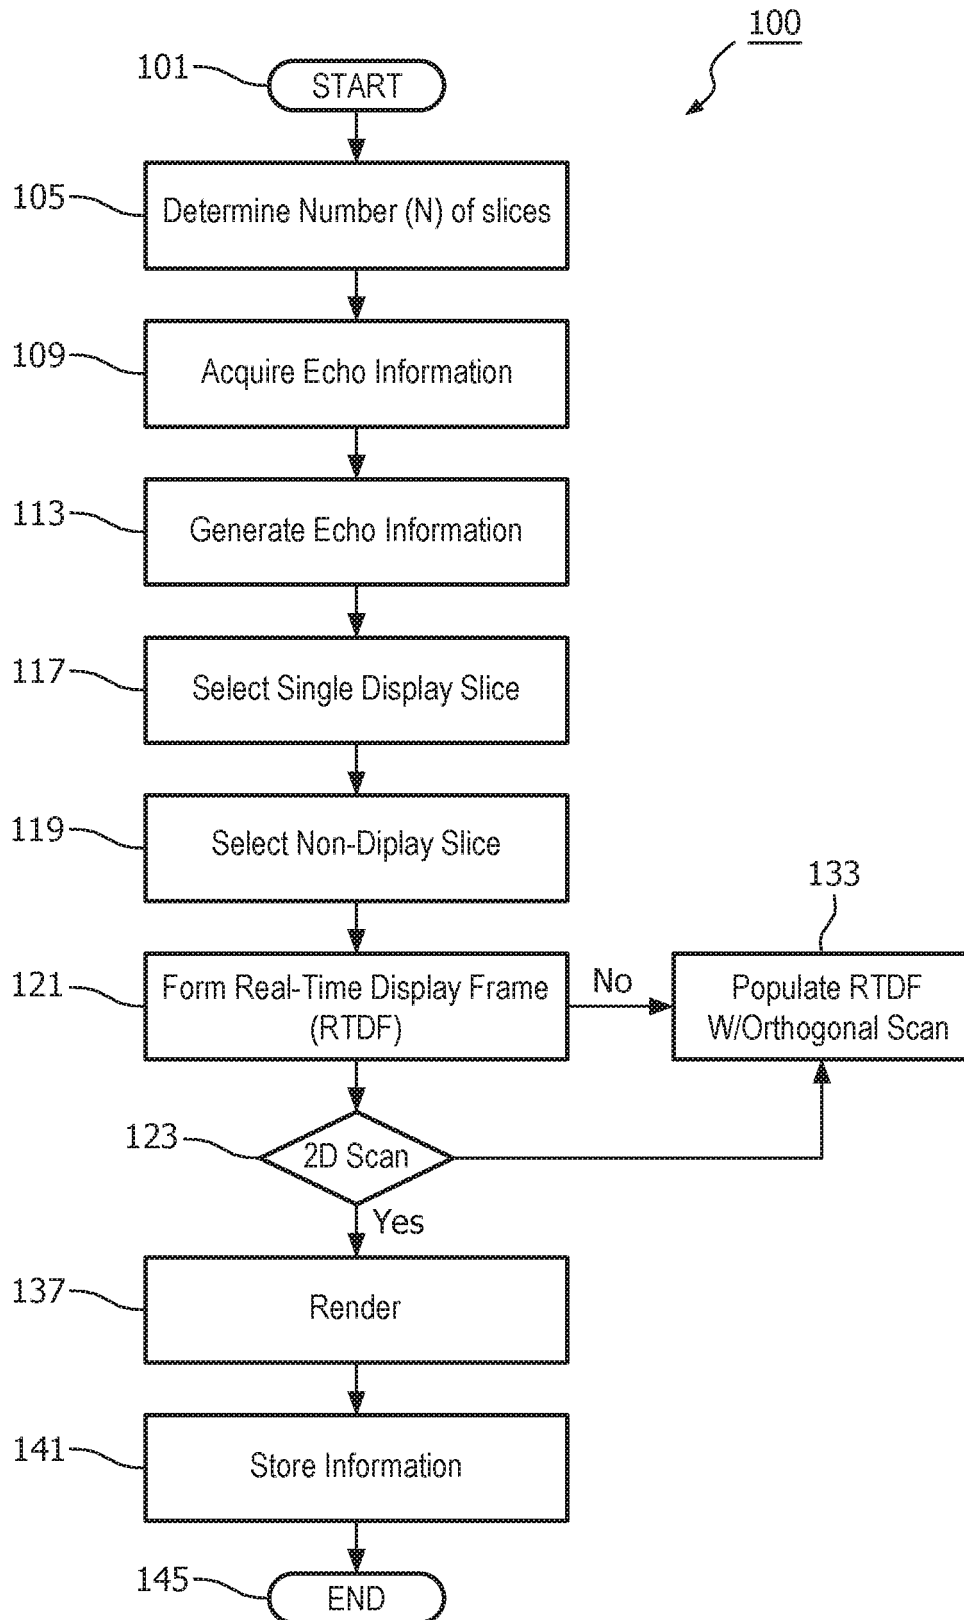


FIG. 1

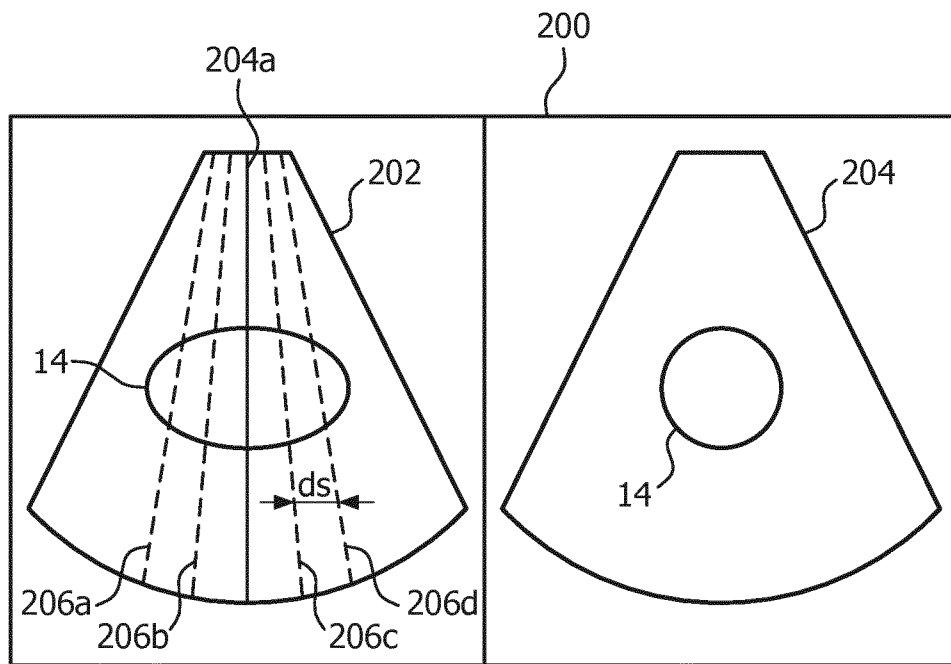


FIG. 2

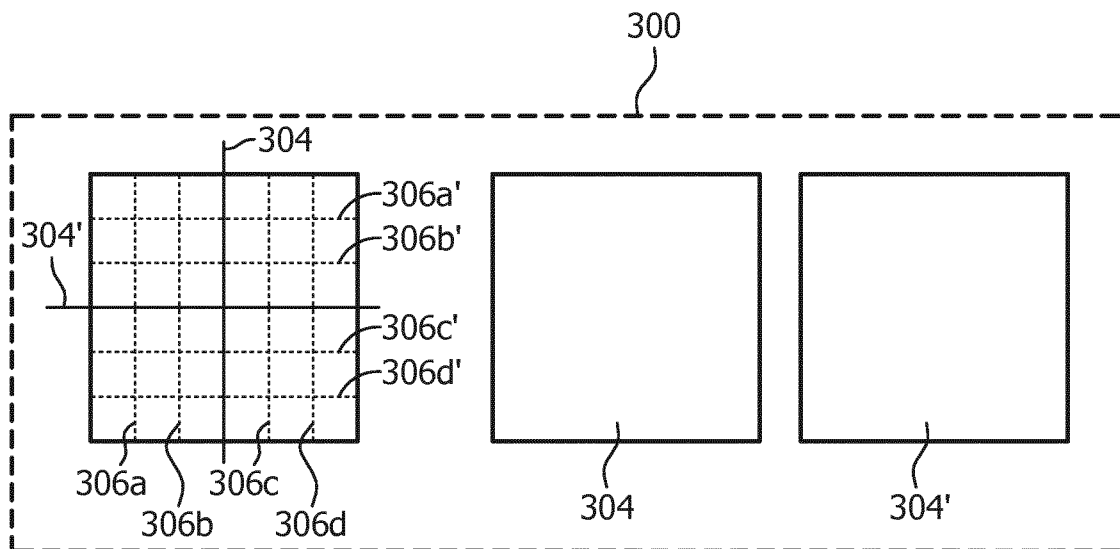
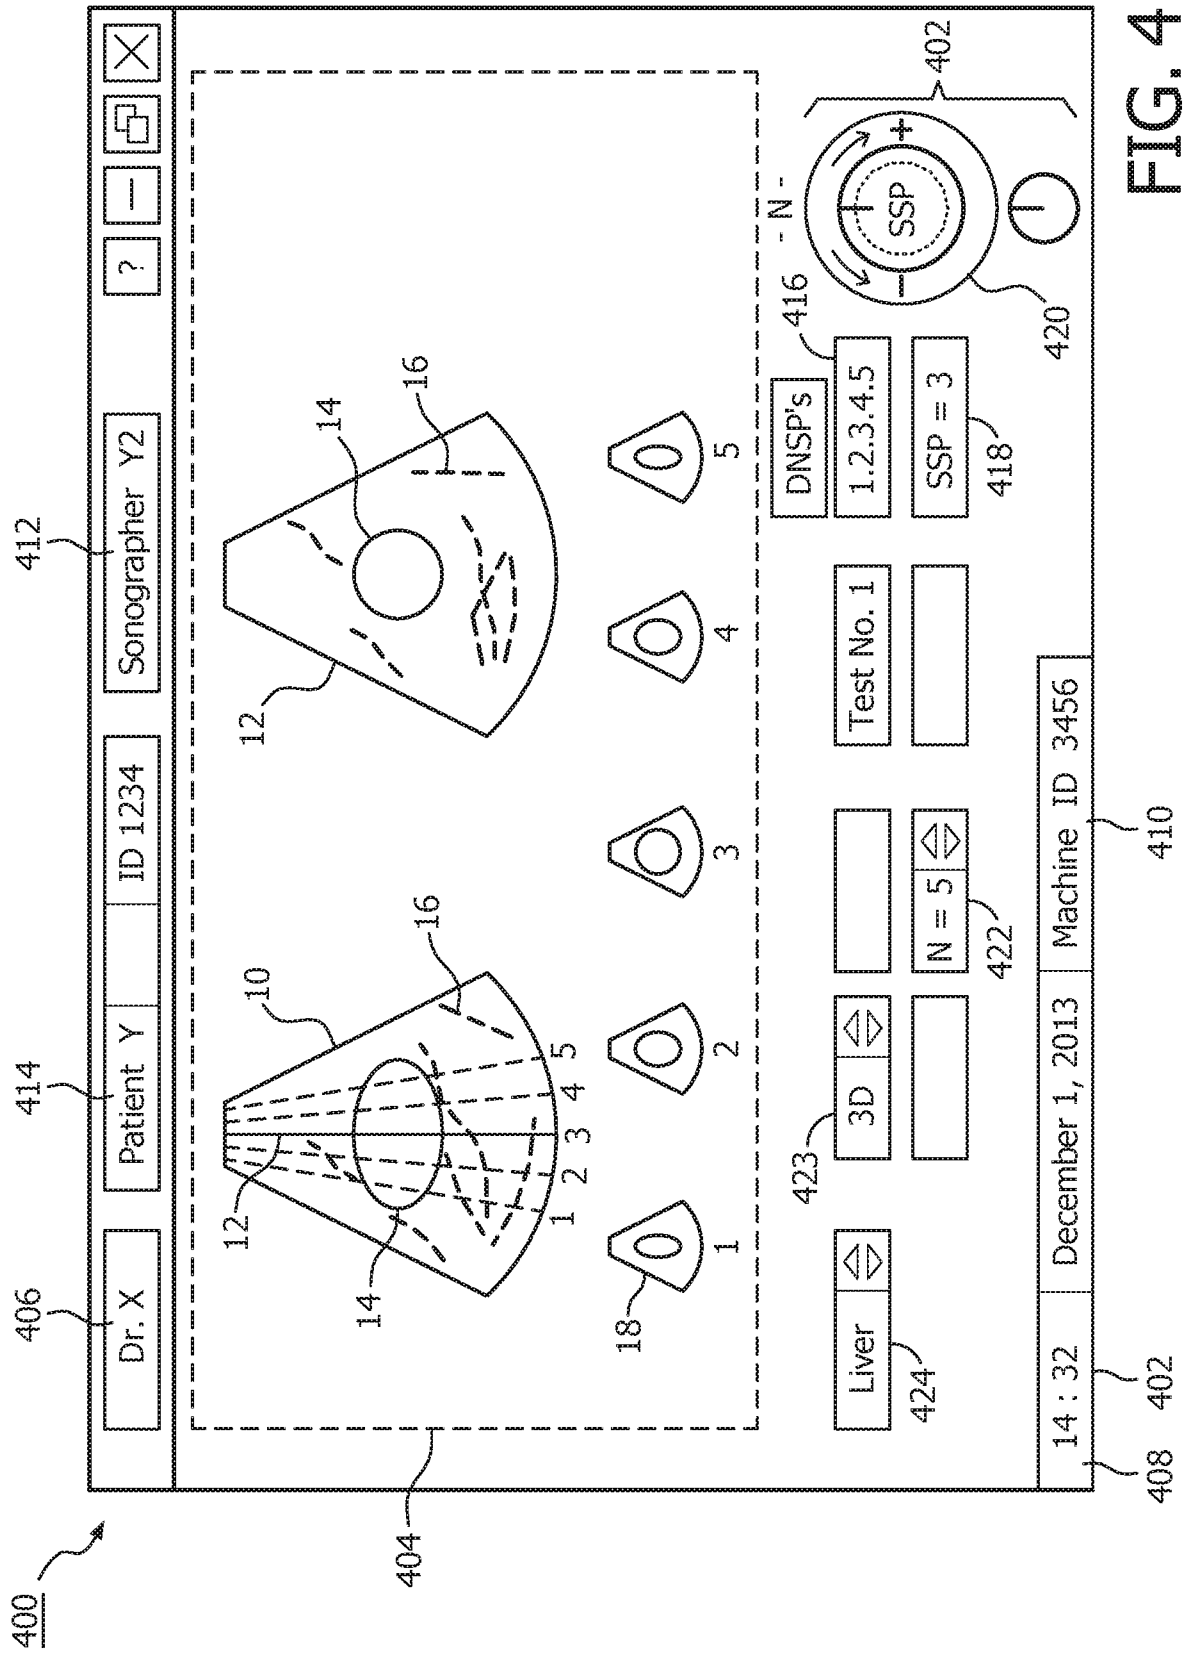


FIG. 3



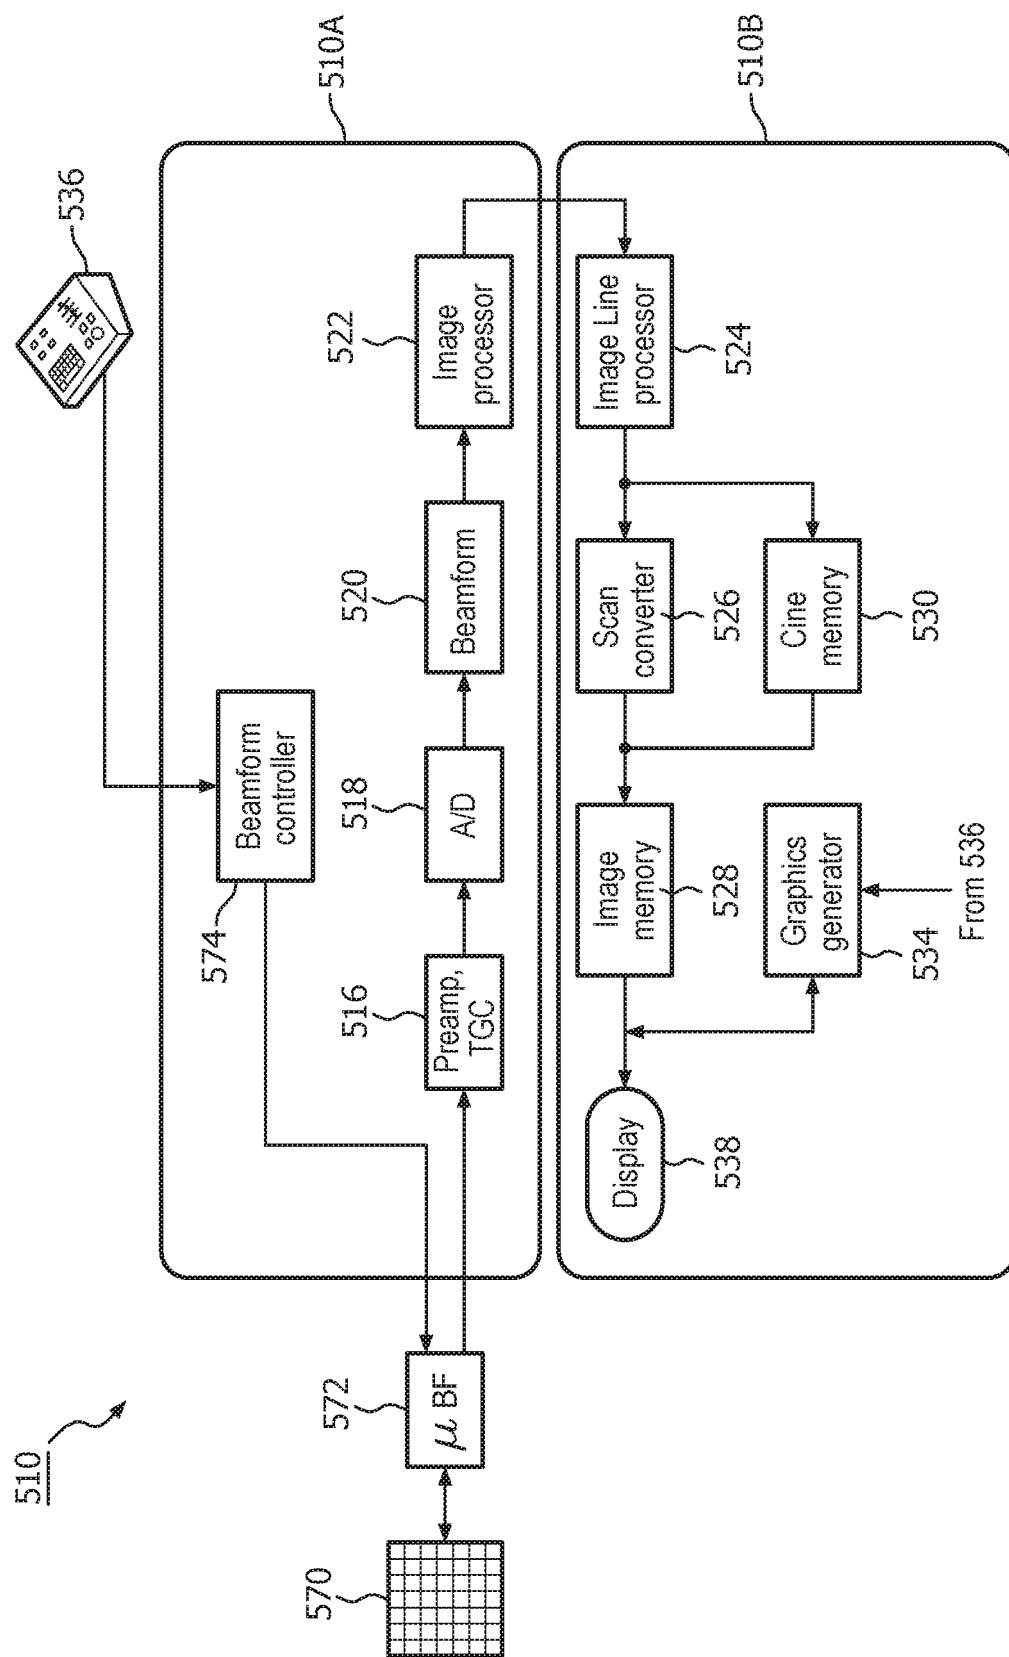


FIG. 5

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2014013849 A1 [0004]
- US 2012230575 A1 [0005]
- US 8012090 B2 [0006]
- WO 2009044316 A1 [0007]
- US 5997479 A, Savord [0057]
- US 6436048 B, Pesque [0057]

专利名称(译)	用于具有单平面或BI平面实时成像的多平面采集的超声系统及其操作方法		
公开(公告)号	EP3099244A1	公开(公告)日	2016-12-07
申请号	EP2015708583	申请日	2015-01-19
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	GAUTHIER THOMAS PATRICE JEAN ARSENE OLSSON LARS JONAS		
发明人	GAUTHIER, THOMAS PATRICE JEAN ARSENE OLSSON, LARS JONAS		
IPC分类号	A61B8/08 A61B8/00 G01S7/52 A61B8/14		
CPC分类号	A61B8/0891 A61B8/145 A61B8/463 A61B8/481 A61B8/5223 A61B8/523 G01S7/52074 G01S7/52084 G16H50/30 A61B8/085 A61B8/5207 A61B8/469 A61B8/54		
优先权	61/932312 2014-01-28 US		
其他公开文献	EP3099244B1		
外部链接	Espacenet		

摘要(译)

超声成像系统和方法技术领域本发明涉及超声成像系统和方法，更具体地，涉及用于适用于超声成像应用的单平面或双平面实时成像模式的多平面采集的超声成像系统和方法，例如肿瘤血液的量化流量和肿瘤分数血容量。超声成像设备可以确定多个图像平面以扫描感兴趣区域，获取对应于每个图像平面的回波信息，生成每个图像平面的图像信息，存储对应于每个图像的图像信息飞机;显示包括感兴趣区域的超声图像，其中超声图像是从所生成的图像信息中呈现的，所述图像信息用于所述多个图像平面中的所选图像平面或与所述多个图像平面成角度的双平面。