



(12) **EUROPEAN PATENT APPLICATION**
published in accordance with Art. 153(4) EPC

(43) Date of publication:
06.06.2018 Bulletin 2018/23

(51) Int Cl.:
A61B 8/00 (2006.01)

(21) Application number: **16829606.9**

(86) International application number:
PCT/CN2016/078835

(22) Date of filing: **08.04.2016**

(87) International publication number:
WO 2017/016239 (02.02.2017 Gazette 2017/05)

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
MA MD

(71) Applicant: **Telefield Medical Imaging Limited Hong Kong (CN)**

(72) Inventor: **ZHENG, Yongping Hong Kong (CN)**

(74) Representative: **Hellmich, Wolfgang European Patent and Trademark Attorney Lortzingstrasse 9 / 2. Stock 81241 München (DE)**

(30) Priority: **28.07.2015 CN 201510452165**

(54) **THREE-DIMENSIONAL IMAGING ULTRASONIC SCANNING METHOD**

(57) A three-dimensional imaging ultrasonic scanning method is applied to ultrasonic diagnostic instruments. The method comprises the following steps: S0, generating a high-frequency voltage pulse to drive a plurality of ultrasonic arrays and power a spatial locator to put the spatial location into service (S100); S1, using the plurality of ultrasonic arrays to acquire different ultrasonic image information of a tested object (S101); S2, using the spatial locator to acquire the positional information of the plurality of ultrasonic arrays (S102). The three-dimensional imaging ultrasonic scanning method can simultaneously satisfy different requirements for images during three-dimensional ultrasonic scanning, so that with just one scanning, a series of B-mode ultrasound images corresponding to each of the ultrasonic arrays can be obtained, and further three-dimensional images for the tested object can be constructed by a main body portion of ultrasonic diagnosis, laying a better foundation for ultrasonic diagnosis.

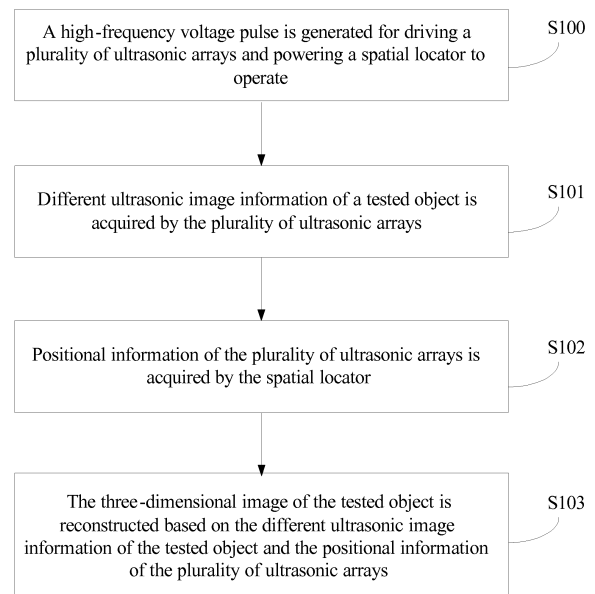


FIG. 1

Description

TECHNICAL FIELD

[0001] The present application relates to the technical field of the ultrasonic scanning used in ultrasonic diagnostic instruments, and more particularly relates to a three-dimensional imaging ultrasonic scanning method.

BACKGROUND

[0002] At present, in the ultrasonic diagnostic instruments, the three-dimensional ultrasound imaging can be accomplished by moving the B-ultrasound probe to a series of spatial positions for recording the B-ultrasound images (2D) at these spatial positions and reconstructing the three-dimensional ultrasound images based on the simultaneously recorded B-ultrasound images (2D). However, in the existing technology just a single one B-ultrasound probe is moved to do this, that is, the resulting ultrasound image is completely determined by the characteristics of the single one B-ultrasound probe, among them, which characteristics include ultrasound frequency, resolution, penetration depth, image width, image shape, focus mode, and image direction. However, in the three-dimensional ultrasound scanning, different organizations, different parts, different patients, different requirements, often have different requirements for these parameters, and meanwhile different requirements may need to be satisfied. For example, in the three-dimensional ultrasound imaging of the spine, an ultrasound probe with a higher frequency should be employed for the muscle tissue which may need high resolution, while an ultrasound probe with a lower frequency should also be employed for the deep tissue imaging. In this case, using a single one ultrasonic probe for the three-dimensional ultrasound imaging cannot meet the actual requirements.

SUMMARY

[0003] The object of the present application is to provide a three-dimensional imaging ultrasonic scanning method, aiming at the above defects of the prior art that a single one ultrasonic probe cannot satisfy the different requirements of the three-dimensional imaging in the three-dimensional ultrasonic scanning at the same time. In one aspect, a three-dimensional imaging ultrasonic scanning method is provided for solving above technical problem, which including following steps:

S0, generating a high-frequency voltage pulse for driving a plurality of ultrasonic arrays and powering a spatial locator to operate;

S1, acquiring different ultrasonic image information of a tested object by the plurality of ultrasonic arrays;

S2, acquiring positional information of the plurality of ultrasonic arrays by the spatial locator.

[0004] Advantageously, in the step S1, the plurality of ultrasonic arrays implement a scanning at the same time, or at different times or at fixed relative positions.

[0005] Advantageously, in the step S2, the spatial locator is a positioner based on electromagnetic field measurements.

[0006] Advantageously, in the step S2, the spatial locator is a motor driving device with a positioning function, wherein the plurality of ultrasonic arrays are mounted on the motor driving device.

[0007] Advantageously, the motor driving device with the positioning function is a linear scanning device, wherein the plurality of ultrasonic arrays are mounted on the linear scanning device.

[0008] Advantageously, the motor driving device with the positioning function is a circular scanning device, wherein the plurality of ultrasonic arrays are mounted on the circular scanning device.

[0009] Advantageously, the plurality of ultrasonic arrays have different frequencies/sizes/focus modes/shapes/mounting orientations.

[0010] Advantageously, the plurality of ultrasonic arrays include at least a first ultrasound array and a second ultrasound array, wherein, the first ultrasonic array and the second ultrasonic array have the same mounting orientation but different frequencies for acquiring different image information of a same part of the tested object.

[0011] Advantageously, the first ultrasonic array is arranged as a linear array while the second ultrasonic array is arranged as an arc-shaped array for acquiring different scanning ranges of the tested object.

[0012] Advantageously, the three-dimensional imaging ultrasonic scanning method of the present application further includes a following step:
S3, reconstructing a three-dimensional image of the tested object based on the different ultrasonic image information of the tested object and the positional information of the plurality of ultrasonic arrays.

[0013] The three-dimensional imaging ultrasound scanning method of the present invention employs at least two ultrasound B-ultrasound arrays having different parameters so that with just one time of scanning, a series of B-mode ultrasound images corresponding to each of the ultrasonic arrays can be obtained. According to the actual needs, the series of images meeting the requirements can be selected for the image three-dimensional ultrasound imaging. For example, two ultrasonic arrays with different frequencies are mounted in parallel, such that images obtained from the ultrasonic arrays with a higher frequency may be used for the superficial tissues to obtain a higher image resolution, while images obtained from the ultrasonic arrays with a lower frequency may be used for the deeper tissues to ensure a sufficient penetration depth. Two ultrasound probes with different shapes may be used, for example one of which can be

a linear array and the other one can be an arc-shaped array. A higher resolution may be obtained by the linear array, while a larger scanning range may be obtained by the arc-shaped array. Different ultrasonic arrays can also be installed in different directions so that three-dimensional images of multiple interested regions or three-dimensional images of the same interested region in different directions, such as the images of the spinous processes in different directions, can be obtained by one time of three-dimensional scanning. In addition to satisfying different requirements by selecting images from different series of ultrasound images obtained by the different ultrasonic arrays, the corresponding images in different series can also be used for image fusion processing to achieve higher image quality, for example, the high signal to noise ratio of the image, thus providing a good foundation for the ultrasound diagnosis.

BRIEF DESCRIPTION OF THE DRAWINGS

[0014]

FIG. 1 is a flowchart of the three-dimensional imaging ultrasonic scanning method according to a first embodiment of the present application.

FIG. 2 is a schematic diagram of the structure of the motor driving device with a positioning function in FIG. 1, wherein the motor driving device is a circular scanning device.

FIG. 3 is a flowchart of the three-dimensional imaging ultrasonic scanning method according to a second embodiment of the present application.

FIG. 4 is an external view of a preferred embodiment of the first ultrasonic array and the second ultrasonic array in FIG. 3.

FIG. 5 is an external view of another preferred embodiment of the first ultrasonic array and the second ultrasonic array in FIG. 3.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0015] The present application provides a three-dimensional imaging ultrasonic scanning method applicable to the ultrasonic diagnostic instruments. The three-dimensional imaging ultrasonic scanning method can simultaneously satisfy different requirements for images during three-dimensional ultrasonic scanning. A specific solution is to simultaneously move at least two ultrasound B-ultrasound arrays with different parameters in a three-dimensional imaging scanning, so that a series of B-ultrasound images corresponding to each ultrasound array can be obtained in a single one time of scanning. At the same time, combining with the spatial locator, the series

of images meeting the requirements can be selected for the image three-dimensional ultrasound imaging. In addition to satisfying different requirements by selecting images from different series of ultrasound images obtained by the different ultrasonic arrays, the corresponding images in different series can also be used for image fusion processing to achieve higher image quality, for example, the high signal to noise ratio of the image, thus providing a good foundation for ultrasonic diagnosis.

[0016] To make the object, the technical solution, and the advantage of the present application more clearly, the present application is further described in detail below with reference to the accompanying drawings and embodiments. It should be understood that the specific embodiments described herein are merely used to explain the present invention and are not intended to the present application.

[0017] As shown in FIG. 1, a flowchart of the three-dimensional imaging ultrasonic scanning method according to a first embodiment of the present application is disclosed. The three-dimensional imaging ultrasonic scanning method comprises the following steps.

[0018] In step S100, a high-frequency voltage pulse is generated for driving a plurality of ultrasonic arrays and powering a spatial locator to operate.

[0019] In this step, the high-frequency voltage pulse is generated by a transmission circuit which is positioned in the ultrasonic diagnostic instrument.

[0020] In this embodiment, the transmission circuit can be composed of a clock generator, a frequency divider, a transmission delay circuit, and a pulse generator. The clock pulse generated by the clock generator is passed through the frequency divider to be lowered to a rate pulse with a certain frequency which is then passed through the transmission delay circuit to the pulse generator for generating a high frequency voltage pulse to drive the plurality of ultrasound arrays. That is, the transmission circuit transmits the electric signals to the plurality of ultrasonic arrays and drives the plurality of ultrasonic arrays, so that the plurality of ultrasonic arrays transmit the ultrasonic beams to the tested object, which belongs to the prior art and is not described herein again.

[0021] In step S101, different ultrasonic image information of a tested object is acquired by the plurality of ultrasonic arrays.

[0022] In this step, the plurality of ultrasonic arrays implement a scanning at the same time, or at different times or at fixed relative positions. During the scanning, the plurality of ultrasonic arrays respectively send ultrasonic waves to the tested object, receive the ultrasonic echo, and output corresponding electric signals according to the ultrasonic echo. Among them, the plurality of ultrasonic arrays have different frequencies, sizes, focus modes, shapes, mounting orientations, and the combinations thereof.

[0023] The above electrical signal is also needed to go through the amplifying circuit, the delay circuit and the addition circuit for further processing, so that the main

part of the ultrasonic diagnostic instrument can better receive the electrical signal that represents the different information of the tested object. Wherein, the amplifying circuit is configured to perform low-noise amplification or buffering operation on the received or transmitted ultrasonic signals to better transmit the ultrasonic signals. The delay circuit and the addition circuit are respectively used to delay and add the electric signal of the ultrasonic wave.

[0024] In this embodiment, the ultrasonic arrays are arranged in different shapes to acquire images of different scanning ranges. The shapes of the ultrasonic arrays include a line array, an arc-shaped array, and a two-dimensional array. Wherein, an image of higher resolution is obtained when using the linear array for scanning, while an image of larger scanning range is obtained when using the arc-shaped array for scanning.

[0025] In this embodiment, when the mounting orientations of the plurality of ultrasonic arrays are the same, different frequencies can be set, so that images of the same tested object at different depths can be obtained according to the different frequencies. When the mounting orientations of the plurality of ultrasonic arrays are different, images of multiple desired scanning areas or images of the same scanning area in different directions can be obtained by one time of scanning.

[0026] In step S102, positional information of the plurality of ultrasonic arrays is acquired by the spatial locator.

[0027] In this step, the positional information of the plurality of ultrasonic arrays during the scanning is acquired by the spatial locator. During the scanning, the electric signals outputted by the ultrasonic arrays and the corresponding positional information are outputted to the main part of the ultrasonic diagnostic instrument. According to the scanning process, the spatial locator locates the positional information of the plurality of ultrasonic arrays to transmit the positional information to the main part of the ultrasonic diagnostic instrument for image-related processing.

[0028] Wherein, the spatial locator may be a positioner based on electromagnetic field measurement or a motor driving device with a positioning function. When the spatial locator is the motor driving device with a positioning function, the plurality of ultrasonic arrays are mounted at corresponding positions according to different forms of the motor driving device with a positioning function. When the motor driving device with a positioning function is a linear scanning device, the plurality of ultrasonic arrays are mounted on the linear scanning device. When the motor driving device with a positioning function is a circular scanning device, the plurality of ultrasonic arrays are mounted on the circular scanning device. As shown in FIG.2, the circular scanning device includes a motor driver 23 and a supporting body 24 driven by the motor driver 23 to rotate. The supporting body 24 has a circular shape. The tested object 21 is placed at the center of the supporting body 24. The plurality of ultrasonic arrays 22 are mounted on the supporting body 24 and equally spaced along the circumference of the supporting body

24.

[0029] In step S103, the three-dimensional image of the tested object is reconstructed based on the different ultrasonic image information of the tested object and the positional information of the plurality of ultrasonic arrays.

[0030] In this step, the main part of the ultrasonic vibration apparatus can acquire a scanned three-dimensional image based on the positional information acquired by the spatial locator and the electric signal of the different ultrasonic image information outputted by the ultrasonic arrays after image processing.

[0031] Specifically, a plurality of three-dimensional images of the tested object are reconstructed by performing image processing on the different ultrasonic image information of the tested object and the positional information of the plurality of ultrasonic arrays, wherein each three-dimensional image is reconstructed from the ultrasound image information obtained from each ultrasound array.

[0032] Alternatively, the three-dimensional image of the tested object is reconstructed by performing comprehensive image processing on the different ultrasonic image information of the tested object and the positional information of the plurality of ultrasonic arrays. Wherein, the three-dimensional image is obtained by reconstructing and fusing the different ultrasonic image information obtained by the plurality of ultrasonic arrays.

[0033] As shown in FIG.3, a flowchart of the three-dimensional imaging ultrasonic scanning method according to a second embodiment of the present application is disclosed, in which the plurality of ultrasonic arrays include a first ultrasonic array and a second ultrasonic array.

[0034] In this embodiment, the method comprises the following steps.

[0035] In step S200, the high-frequency voltage pulse is generated for driving a plurality of ultrasonic arrays and powering a spatial locator to operate.

[0036] In this step, the high-frequency voltage pulse is generated by a transmission circuit which is positioned in the ultrasonic diagnostic instrument.

[0037] In this embodiment, the transmission circuit can be composed of a clock generator, a frequency divider, a transmission delay circuit, and a pulse generator. The clock pulse generated by the clock generator is passed through the frequency divider to be lowered to a rate pulse with a certain frequency which is then passed through the transmission delay circuit to the pulse generator for generating a high frequency voltage pulse to drive the plurality of ultrasound arrays. That is, the transmission circuit transmits the electric signals to the plurality of ultrasonic arrays and drives the plurality of ultrasonic arrays, so that the plurality of ultrasonic arrays transmit the ultrasonic beams to the tested object, which belongs to the prior art and is not described herein again.

[0038] In step S201, the superficial tissue information of the tested object is acquired by the first ultrasonic array and the deeper tissue information of the corresponding part of the tested object is acquired by the second ultra-

sonic array.

[0039] In this step, the first ultrasonic array and the second ultrasonic array may implement a scanning at the same time, or at different times or at fixed relative positions. During the scanning, the first ultrasonic array and the second ultrasonic array respectively send ultrasonic waves to the tested object, receive the ultrasonic echo, and output corresponding electric signals according to the ultrasonic echo. Wherein, both the first ultrasonic array and the second ultrasonic array are linear arrays having the same mounting orientation but different frequencies.

[0040] In step S202, the positional information of the first ultrasonic array and the second ultrasonic array is acquired by the spatial locator.

[0041] In this step, the positional information of the first ultrasonic array and the second ultrasonic array during the scanning is acquired by the spatial locator. During the scanning, the electric signals outputted by the ultrasonic arrays and the corresponding positional information are outputted to the main part of the ultrasonic diagnostic instrument. According to the scanning process, the spatial locator locates the positional information of the plurality of ultrasonic arrays to transmit the positional information to the main part of the ultrasonic diagnostic instrument for image-related processing.

[0042] Wherein, the spatial locator may be a positioner based on electromagnetic field measurement or a motor driving device with a positioning function. When the spatial locator is the motor driving device with a positioning function, the first ultrasonic array and the second ultrasonic array are mounted at corresponding positions according to different forms of the motor driving device with a positioning function. When the motor driving device with a positioning function is a linear scanning device, the first ultrasonic array and the second ultrasonic arrays are mounted on the linear scanning device. When the motor driving device with a positioning function is a circular scanning device, the first ultrasonic array and the second ultrasonic array are mounted on the circular scanning device.

[0043] In step S203, the three-dimensional image of the tested object is reconstructed based on the different ultrasonic image information of the tested object and the positional information of the first ultrasonic array and the second ultrasonic array.

[0044] In this step, the main part of the ultrasonic vibration apparatus can acquire a scanned three-dimensional image based on the positional information acquired by the spatial locator and the electric signals for the same part of the tested object at the different depths outputted by the first ultrasonic array and the second ultrasonic array after image processing.

[0045] Specifically, two three-dimensional images of the tested object are reconstructed by performing image processing on the different ultrasonic image information of the tested object and the positional information of the first ultrasonic array and the second ultrasonic array,

wherein one three-dimensional image is reconstructed from the ultrasound image information obtained from the first ultrasound array, and the other three-dimensional image is reconstructed from the ultrasound image information obtained from the second ultrasound array.

[0046] Alternatively, the three-dimensional image of the tested object is reconstructed by performing comprehensive image processing on the different ultrasonic image information of the tested object and the positional information of the first ultrasonic array and the second ultrasonic array. Wherein, the three-dimensional image is obtained by reconstructing and fusing different ultrasonic image information obtained by the first ultrasonic array and the second ultrasonic array.

[0047] As shown in FIG.4, an external view of a preferred embodiment of the first ultrasonic array and the second ultrasonic array in FIG. 3 is disclosed. In this embodiment, both the first ultrasonic array 31 and the second ultrasonic array 32 are linear arrays arranged in parallel, that is, the mounting orientations of the first ultrasonic array 31 and the second ultrasonic array 32 are the same. During the scanning, the areas scanned by the first ultrasonic array 31 and the second ultrasonic array 32 are the same. The frequency of the first ultrasonic array 31 is f_0 , and the frequency of the second ultrasonic array 32 is f_1 . When f_0 and f_1 are not equal, the images of the same tested object at the different depths can be obtained according to the different frequencies. In the present application, the mounting orientations of the first ultrasonic array 31 and the second ultrasonic array 32 are not limited to this. In actual use, the ultrasonic arrays may adopt other mounting orientations. Meanwhile, other parameters of the ultrasonic arrays, such as the shape and the size, may also be different according to practical needs.

[0048] As shown in FIG.5, an external view of another preferred embodiment of the first ultrasonic array and the second ultrasonic array in FIG. 3 is disclosed. In this embodiment, the first ultrasonic array 41 is arranged as a linear array, while the second ultrasonic array 42 is arranged as an arc-shaped array. The mounting orientations of the first ultrasonic array 41 and the second ultrasonic array 42 are the same. During scanning, a higher resolution is obtained by the scanning of the first ultrasonic array 41, and a larger scanning area is obtained by the scanning of the second ultrasonic array 42. In the present application, the mounting orientations of the first ultrasonic array 41 and the second ultrasonic array 42 are not limited to this. In actual use, the ultrasonic arrays may adopt other mounting orientations. Meanwhile, other parameters of the ultrasonic arrays, such as the shape and the size, may also be different according to practical needs.

[0049] In summary, the present application provides a three-dimensional imaging ultrasonic scanning method applicable to ultrasonic diagnostic instruments. The three-dimensional imaging ultrasonic scanning method can simultaneously satisfy different requirements for im-

ages during three-dimensional ultrasonic scanning. A specific solution is to simultaneously move at least two ultrasound B-ultrasound arrays with different parameters in a three-dimensional imaging scanning. Combining with the spatial locator, a series of B-ultrasound images corresponding to each ultrasound array can be obtained in a single one time of scanning, so that the main part of the ultrasound diagnosis can construct a three-dimensional image of the tested object, thus providing a good foundation for the ultrasound diagnosis .

[0050] As described above, it is only a better specific implementation method of the application, but the scope of protection of the application is not limited to this. Any variation or replacement that can be easily thought of by persons skilled in the art within the technical scope disclosed by the present application shall fall within the protection scope of the present application. Therefore, the protection scope of the present application should be subject to the protection scope of the claims.

Claims

1. A three-dimensional imaging ultrasonic scanning method applicable to ultrasonic diagnostic instruments, **characterised in that** including following steps:

S0, generating a high-frequency voltage pulse for driving a plurality of ultrasonic arrays and powering a spatial locator to operate;
S1, acquiring different ultrasonic image information of a tested object by the plurality of ultrasonic arrays;
S2, acquiring positional information of the plurality of ultrasonic arrays by the spatial locator.

2. The three-dimensional imaging ultrasonic scanning method according to claim 1, **characterised in that** in the step S1, the plurality of ultrasonic arrays implement a scanning at the same time, or at different times or at fixed relative positions.
3. The three-dimensional imaging ultrasonic scanning method according to claim 1, **characterised in that** in the step S2, the spatial locator is a positioner based on electromagnetic field measurements.
4. The three-dimensional imaging ultrasonic scanning method according to claim 1, **characterised in that** in the step S2, the spatial locator is a motor driving device with a positioning function, wherein the plurality of ultrasonic arrays are mounted on the motor driving device.
5. The three-dimensional imaging ultrasonic scanning method according to claim 4, **characterised in that** the motor driving device with the positioning function

is a linear scanning device, wherein the plurality of ultrasonic arrays are mounted on the linear scanning device.

6. The three-dimensional imaging ultrasonic scanning method according to claim 4, **characterised in that** the motor driving device with the positioning function is a circular scanning device, wherein the plurality of ultrasonic arrays are mounted on the circular scanning device.
7. The three-dimensional imaging ultrasonic scanning method according to any one of claims 1 to 6, **characterised in that** the plurality of ultrasonic arrays have different frequencies/sizes/focus modes/shapes/mounting orientations.
8. The three-dimensional imaging ultrasonic scanning method according to claim 7, **characterised in that** the plurality of ultrasonic arrays include at least a first ultrasound array and a second ultrasound array, wherein, the first ultrasonic array and the second ultrasonic array have the same mounting orientation but different frequencies for acquiring different image information of a same part of the tested object.
9. The three-dimensional imaging ultrasonic scanning method according to claim 8, **characterised in that** the first ultrasonic array is arranged as a linear array while the second ultrasonic array is arranged as an arc-shaped array for acquiring different scanning ranges of the tested object.
10. The three-dimensional imaging ultrasonic scanning method according to claim 1, **characterised in that** further including a following step:
S3, reconstructing a three-dimensional image of the tested object based on the different ultrasonic image information of the tested object and the positional information of the plurality of ultrasonic arrays.

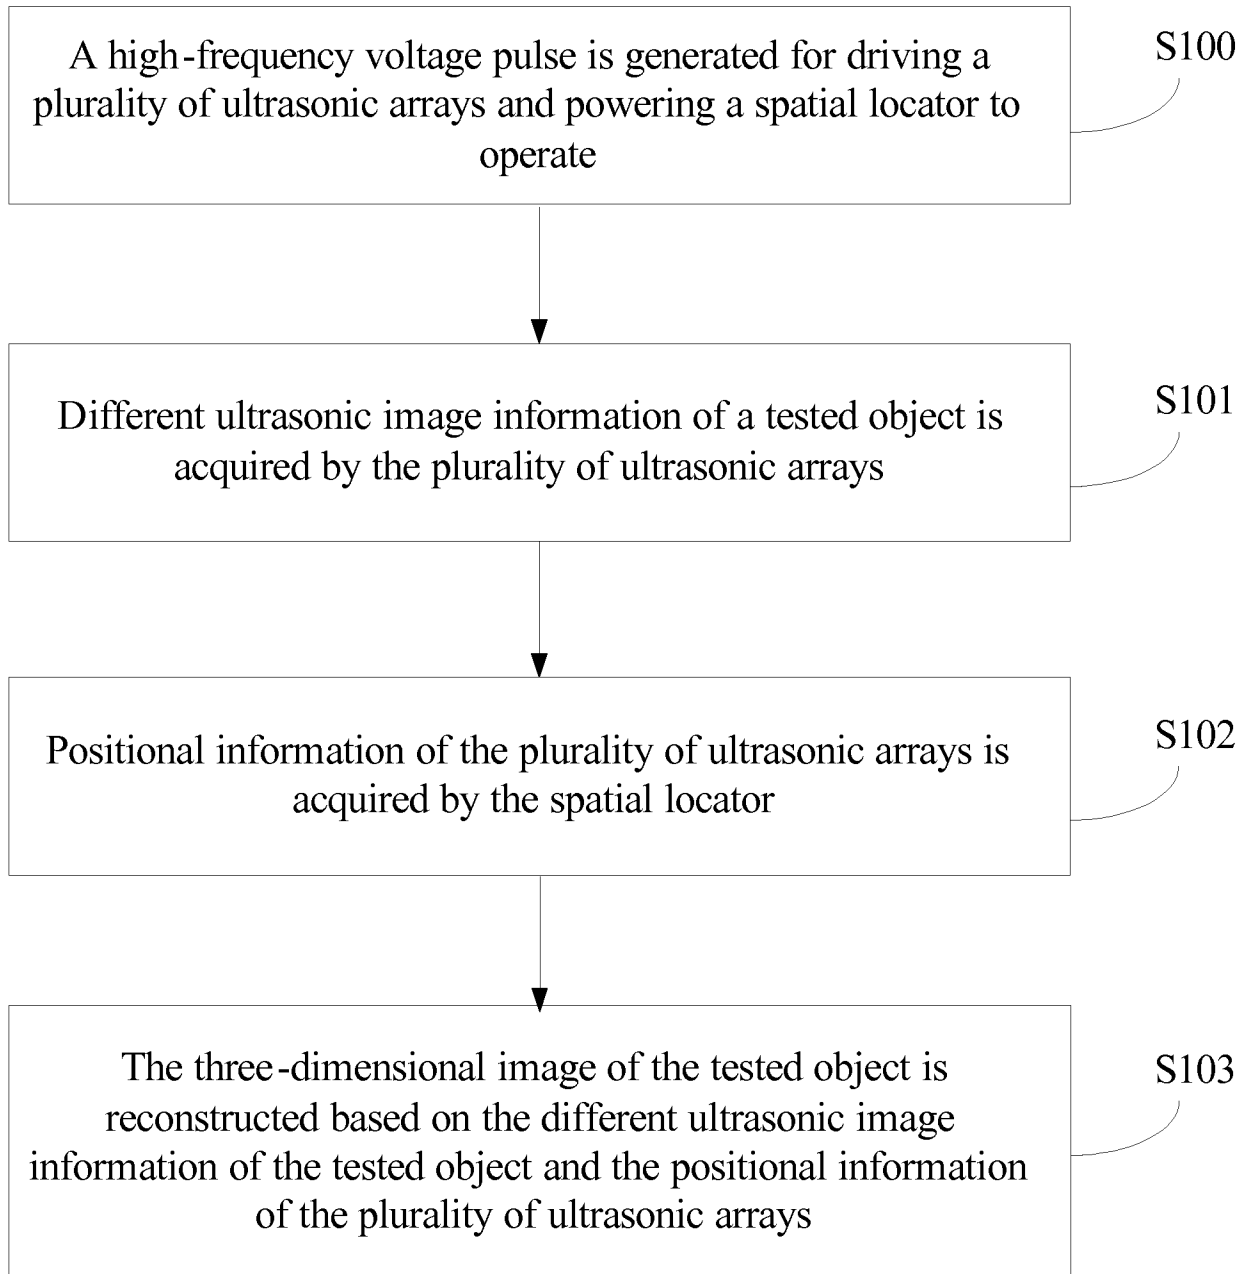


FIG. 1

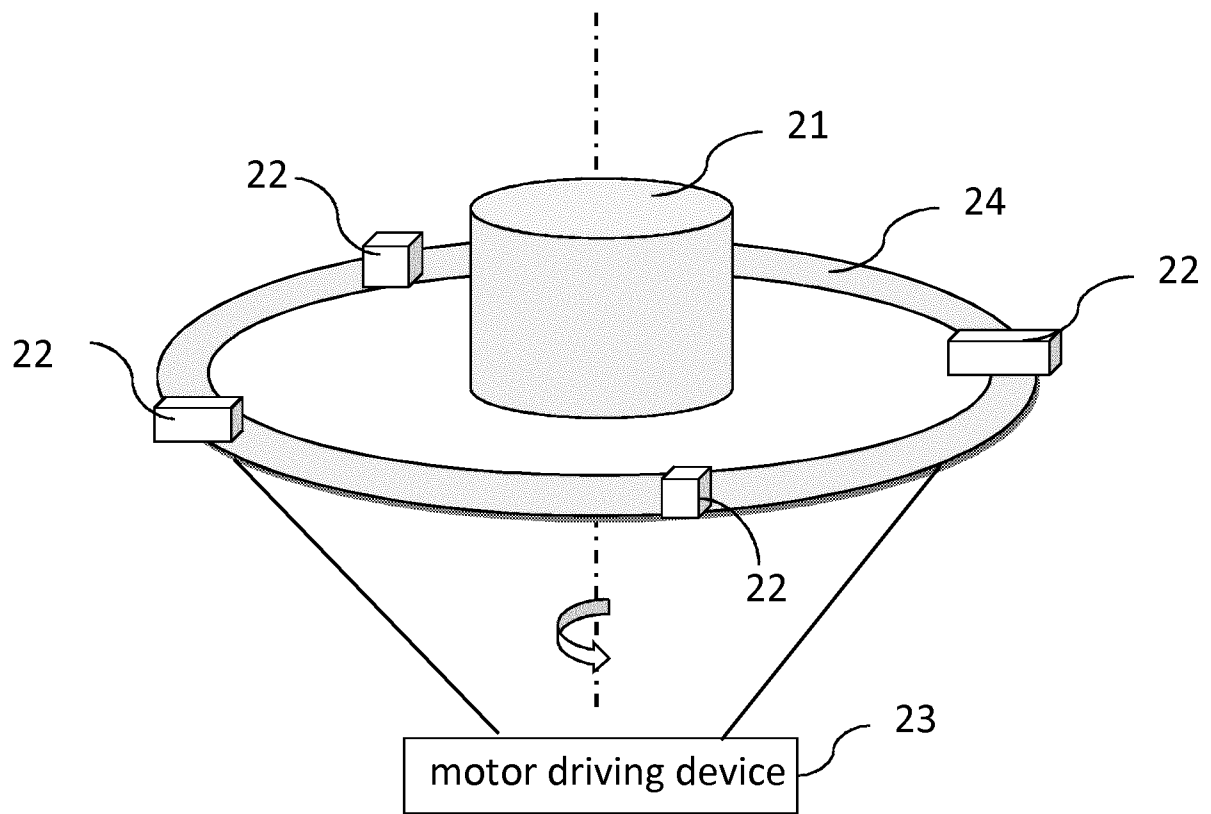


FIG. 2





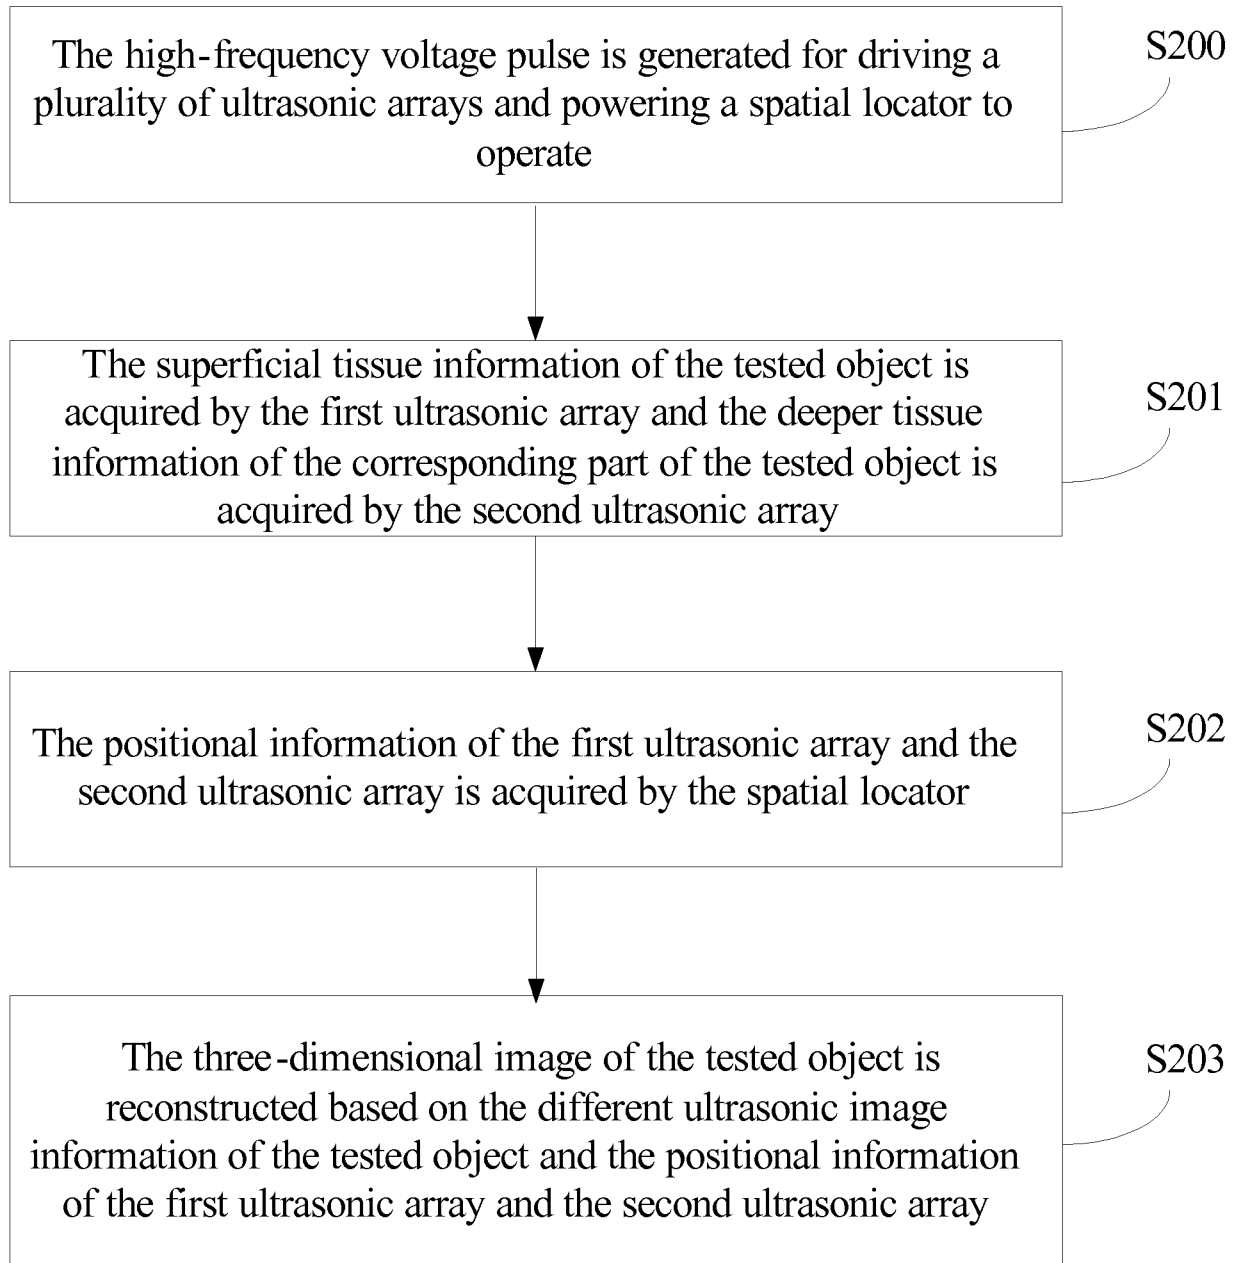


FIG. 3

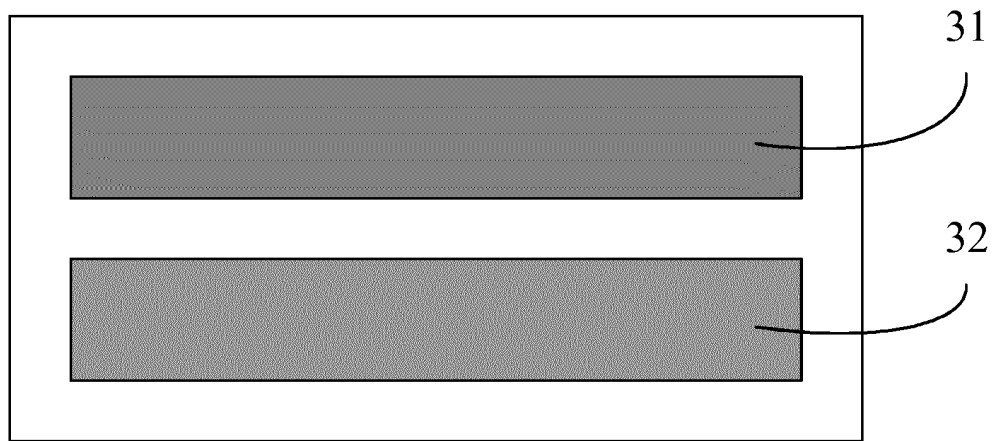

Scanning direction
FIG. 4

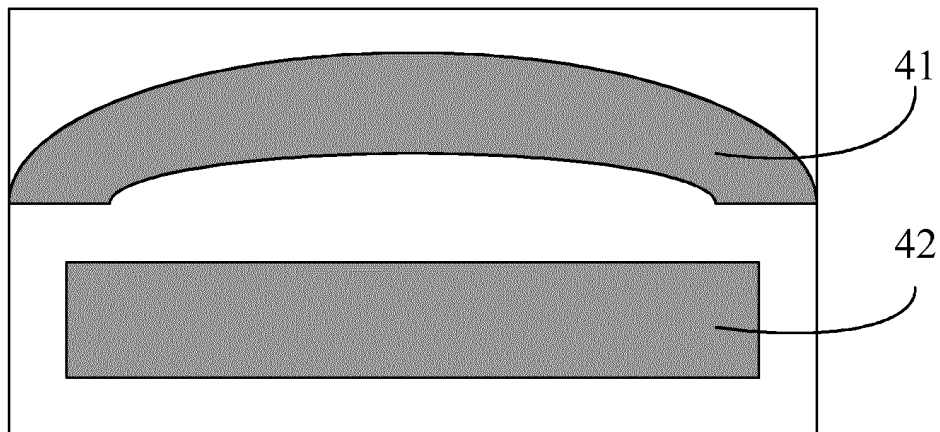

Scanning direction
FIG. 5

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CN2016/078835

A. CLASSIFICATION OF SUBJECT MATTER

A61B 8/00 (2006.01) i

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 8/-

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

CNPAT, CNKI, WPI, EPODOC: TELEFIELD MEDICAL IMAGING LIMITED; ZHENG, Yongping; synchronization, asynchronism, multi, sense, three, image, move, transducer, ultrasonic, position, detect?, array?, probe?, direction, rebuild, two, frequency, scan

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	CN 102068275 A (SIEMENS MEDICAL SOLUTIONS USA, INC.), 25 May 2011 (25.05.2011), description, paragraphs [0017]-[0032], [0038]-[0064] and [0067]-[0089], and figures 1-3	1-10
X	CN 102793562 A (SONY CORPORATION), 28 November 2012 (28.11.2012), description, paragraphs [0048]-[0068], and figures 1-8	1-10
X	CN 102626324 A (SAMSUNG SDI CO., LTD.), 08 August 2012 (08.08.2012), description, paragraphs [0028]-[0043] and [0050]-[0056], and figures 1-5	1-10
X	JP 2008307087 A (TOSHIBA K.K. et al.), 25 December 2008 (25.12.2008), description, paragraphs [0015]-[0075], and figures 1-5	1-10
A	CN 103142246 A (TOSHIBA CORPORATION et al.), 12 June 2013 (12.06.2013), the whole document	1-10
A	CN 103954966 A (SOUTH CHINA UNIVERSITY OF TECHNOLOGY), 30 July 2014 (30.07.2014), the whole document	1-10

☐ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	
"E" earlier application or patent but published on or after the international filing date	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	"&" document member of the same patent family

Date of the actual completion of the international search
13 June 2016 (13.06.2016)Date of mailing of the international search report
01 July 2016 (01.07.2016)Name and mailing address of the ISA/CN:
State Intellectual Property Office of the P. R. China
No. 6, Xitucheng Road, Jimenqiao
Haidian District, Beijing 100088, China
Facsimile No.: (86-10) 62019451Authorized officer
HUANG, Xi
Telephone No.: (86-10) **61648421**

INTERNATIONAL SEARCH REPORT **Information on patent family members**

International application No.
PCT/CN2016/078835

Patent Documents referred in the Report	Publication Date	Patent Family	Publication Date
CN 102068275 A	25 May 2011	DE 102010047155 A1	26 May 2011
		US 2011125022 A1	26 May 2011
		JP 2011110432 A	09 June 2011
		KR 20110058723 A	01 June 2011
CN 102793562 A	28 November 2012	EP 2527830 A2	28 November 2012
		JP 2012239813 A	10 December 2012
		US 2012300578 A1	29 November 2012
		US 9182380 B2	10 November 2015
CN 102626324 A	08 August 2012	US 2012203107 A1	09 August 2012
		KR 20120090170 A	17 August 2012
JP 2008307087 A	25 December 2008	None	
CN 103142246 A	12 June 2013	US 2013144168 A1	06 June 2013
		JP 2013138841 A	18 July 2013
		CN 103142246 B	17 December 2014
CN 103954966 A	30 July 2014	WO 2015154486 A1	15 October 2015

Form PCT/ISA/210 (patent family annex) (July 2009)

专利名称(译)	三维成像超声扫描方法		
公开(公告)号	EP3329854A4	公开(公告)日	2019-05-08
申请号	EP2016829606	申请日	2016-04-08
[标]申请(专利权)人(译)	中慧医学成像有限公司		
申请(专利权)人(译)	慧医学影像有限公司		
当前申请(专利权)人(译)	中慧医学影像有限公司		
[标]发明人	ZHENG YONGPING		
发明人	ZHENG, YONGPING		
IPC分类号	A61B8/00		
CPC分类号	A61B8/466 A61B8/00 A61B8/0875 A61B8/4218 A61B8/4254 A61B8/4461 A61B8/4477 A61B8/483 A61B8/5207 A61B8/54 G01S15/8915 G01S15/894 G01S15/8952 G01S15/8993		
代理机构(译)	HELLMICH , WOLFGANG		
优先权	201510452165.7 2015-07-28 CN		
其他公开文献	EP3329854A1		
外部链接	Espacenet		

摘要(译)

三维成像超声扫描方法应用于超声诊断仪器。该方法包括以下步骤：
S0，产生高频电压脉冲以驱动多个超声阵列，并为空间定位器供电以使空间位置投入使用（S100）；S1，使用多个超声阵列获取被测对象的不同超声图像信息（S101）；S2，使用空间定位器获取多个超声阵列的位置信息（S102）。三维成像超声扫描方法可以同时满足三维超声扫描期间图像的不同要求，因此只需一次扫描，就可以获得与每个超声阵列对应的一系列B模式超声图像，并且测试对象的三维图像可以通过超声诊断的主体部分构建，为超声诊断奠定更好的基础。