



(51) International Patent Classification:

H04W 80/12 (2009.01) *G01S 15/89* (2006.01)
A61B 8/13 (2006.01) *H04W 12/06* (2009.01)

(21) International Application Number:

PCT/CA2016/050343

(22) International Filing Date:

23 March 2016 (23.03.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

14/671,773 27 March 2015 (27.03.2015) US

(71) Applicant: **CLARIUS MOBILE HEALTH CORP.**
[CA/CA]; Attention : Julian Ho, 350 - 3605 Gilmore Way,
Burnaby, BC V5G 4X5 (CA).

(72) Inventors: **PELISSIER, Laurent**; 171 West Kings Road,
North Vancouver, British Columbia V7N 2L7 (CA).
DICKIE, Kris; 928 East 20th Avenue, Vancouver, British
Columbia V5V 1N6 (CA). **HANSEN, Trevor**; #212-825

East 7th Avenue, Vancouver, British Columbia V5T 1P4
(CA).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,

[Continued on next page]

(54) Title: SYSTEM AND METHOD FOR CONNECTING AND CONTROLLING WIRELESS ULTRASOUND IMAGING SYSTEM FROM ELECTRONIC DEVICE

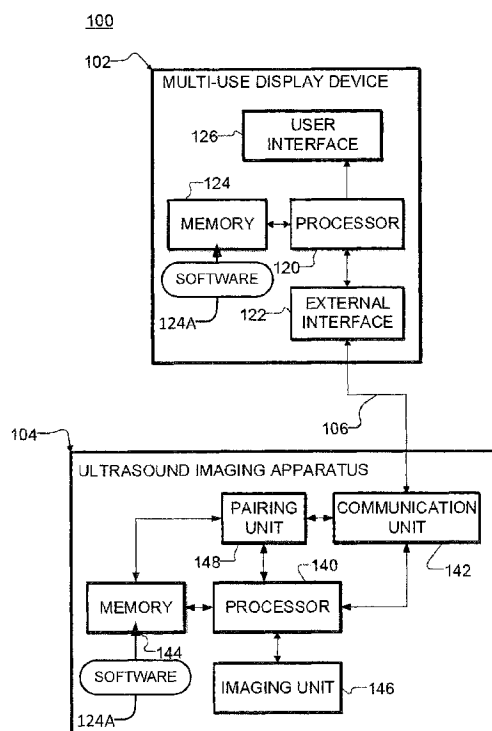


FIG. 1

(57) Abstract: An ultrasound imaging system comprising a multi-use electronic display device and an ultrasound imaging device. The multi-use electronic display device is capable of communicating with one or more ultrasound imaging devices and selecting which to connect with based on at least one of previously store information, user input, and information gathered from the ultrasound imaging devices. The multi-use electronic display device may communicate with the ultrasound imaging devices while they are in a low power standby state. This approach reduces the complexity of the pairing process and provides a means for quickly and easily selecting between multiple ultrasound imaging devices.



SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, **Published:**
GW, KM, ML, MR, NE, SN, TD, TG).

— *with international search report (Art. 21(3))*

SYSTEM AND METHOD FOR CONNECTING AND CONTROLLING WIRELESS ULTRASOUND IMAGING SYSTEM FROM ELECTRONIC DEVICE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority from US Application No. 14/671773, filed 27 March 2015. For purposes of the United States, this application claims the benefit under 35 U.S.C. §119 of US Application No. 14/671773, filed 27 March 2015, and entitled SYSTEM AND METHOD FOR CONNECTING AND CONTROLLING WIRELESS ULTRASOUND IMAGING SYSTEM FROM ELECTRONIC DEVICE which is hereby incorporated herein by reference for all purposes.

FIELD

[0002] This invention generally relates to ultrasound imaging systems. In particular, the invention relates to ultrasound imaging systems comprising an ultrasound imaging apparatus and a multi-use electronic display device, and to methods for communication between ultrasound imaging apparatus and multi-use display devices.

BACKGROUND

[0003] Ultrasound imaging systems are an important tool for diagnosis and therapy in a wide range of medical applications. Conventionally, ultrasound systems were large, expensive units used only in radiology departments by highly trained specialists. To improve portability and usability and enable ultrasound to be used at the point-of-care and by more users, various attempts have been made to reduce the size and cost of these systems and avoid the ergonomically troublesome cables that are typically used to attach handheld transducers to processing hardware.

[0004] For example, U.S. Pat. No. 6780154 discloses a handheld medical diagnostic ultrasound imaging system that wirelessly communicates ultrasound data to a multi-use display device such as a commercially available PDA or tablet computer.

[0005] In addition to size and cost, wireless ultrasound systems may also face challenges related to bandwidth and power. A high bandwidth is desirable in order to support high quality images and high frame rates. However, high bandwidth wireless connections typically have high power consumption, which can quickly drain the battery of a wireless imaging device.

[0006] Some applications, like emergency medicine, may be time-critical. In such applications, users may need to begin imaging without delay. Some ultrasound systems can take a long time, on the order of 30-45 seconds, to boot up. It may not be practical for a battery-powered device to remain on when not in use. Wireless communication links generally require some sort of initialization procedure in order to establish communication. This pairing process can take a long time and be prone to errors, further delaying the start of imaging.

[0007] There remains a need for wireless ultrasound imaging systems that enable users of multi-use display devices to connect to ultrasound imaging devices quickly, easily, and securely. There is a particular need for such systems that provide multiple ultrasound imaging devices and allow users to rapidly select and commence imaging using a selected one of the ultrasound imaging devices.

SUMMARY

[0008] The description of the invention which follows, together with the accompanying drawings should not be construed as limiting the invention to the examples shown and described, because those skilled in the art to which this invention pertains will be able to devise other forms thereof within the scope of the appended claims.

[0009] In accordance with one or more embodiments, a wireless ultrasound imaging system comprises a multi-use display device and an ultrasound imaging device. The multi-use display device is configured to acquire ultrasound imaging device selection data from one or more ultrasound imaging devices, select an ultrasound imaging device, direct the selected ultrasound imaging device to acquire ultrasound data, receive the ultrasound data from the selected ultrasound imaging device and display the ultrasound data.

[0010] One aspect provides an ultrasound imaging method. The method comprises, by a multi-use electronic display device: using a first wireless communication protocol to acquire imaging device selection information from each of one or more ultrasound imaging devices. The method selects one of the one or more ultrasound imaging devices for use in an ultrasound procedure based on the selection information. The method then establishes a primary wireless communication link with the selected one of the ultrasound imaging devices according to a second wireless communication protocol different from the first wireless communication protocol. The method commands the selected one of the ultrasound imaging devices to acquire ultrasound image data. Subsequently, the method receives the ultrasound image data by way of the primary wireless communication link; and displays the received ultrasound image data on a screen of the multi-use electronic display device. The first wireless communication protocol may, for example, comprise a Bluetooth protocol.

[0011] In some embodiments the method comprises, by the multi-use electronic display device: determining from the selection information a controllable function of the ultrasound imaging device; and in response to determining the controllable function, configuring the multi-use electronic display device to provide at least one user interface control for the controllable function.

[0012] In some embodiments the selection information comprises link information for each of the one or more ultrasound imaging devices and establishing the primary wireless communication link with the selected one of the ultrasound imaging devices comprises using the link information to establish data communication between the multi-use display device and the selected ultrasound imaging device according to the second wireless data communication protocol. The link information may include, for example an address, name, ID or other information identifying the selected ultrasound imaging device. The link information may optionally include other information useful for setting up the primary wireless communication link such as encryption keys or other encryption information, protocol information, etc.

[0013] In some embodiments the selection information comprises battery charge information indicative of a state of charge of batteries of the ultrasound imaging devices.

In some embodiments the first wireless communication protocol is a protocol that does not require the ultrasound imaging devices to be powered. For example, the first wireless communication protocol may comprise an RFID protocol. In some embodiments the method comprise, at the multi-use electronic display device, determining the ultrasound procedure to perform on a patient and selecting one of the one or more ultrasound imaging devices comprises limiting the selection to those of the ultrasound imaging devices that possess an adaptation necessary for the ultrasound procedure. The adaptation may comprise, for example one or more of, a Doppler imaging mode or other special imaging mode; a transducer having a configuration required for the determined ultrasound procedure; a needle guide or other structural adaptation; a data transceiver providing a desired bandwidth, etc.

[0014] In some embodiments selecting one of the one or more ultrasound imaging devices comprises a filtering stage in which those of the ultrasound imaging devices potentially suitable for the ultrasound procedure are identified and a selection stage comprising, if more than one of the ultrasound imaging devices are potentially suitable for the procedure, selecting one of the more than one of the ultrasound imaging devices that are potentially suitable for the procedure.

[0015] In some embodiments acquiring imaging device selection information from each of one or more ultrasound imaging devices is performed while some or all of the ultrasound imaging devices are in a low-power standby state and the method comprises commanding the selected one of the ultrasound imaging devices to switch to an active or power on state.

[0016] In some embodiments, the method comprises, by way of the first wireless communication protocol commanding the selected one of the ultrasound imaging devices to issue a human-perceptible visual or audible signal. The visual or audible signal may be used to locate the selected ultrasound imaging device or to distinguish the selected ultrasound imaging device from other similar-looking ultrasound imaging devices. In some embodiments the method comprises, before selecting one of the one or more ultrasound imaging devices, displaying at the multi-use display device at least some of the selection information for each of a plurality of the ultrasound imaging devices, the

displayed selection information including one or more of: type of an ultrasound transducer type of the ultrasound imaging device; nickname of the ultrasound imaging device; battery state of charge of the ultrasound imaging device; and strength of signals in the first wireless communication protocol received at the multi-use display device from the ultrasound imaging device.

[0017] The above-noted features may be combined in any combinations and sub-combinations to yield various non-limiting example embodiments.

[0018] Another aspect provides an ultrasound imaging system comprising an ultrasonic imaging apparatus which wirelessly communicates with a multi-use electronic display device for display of ultrasound image data acquired by the ultrasonic imaging device. The ultrasonic imaging apparatus comprises: an imaging unit operable to transmit ultrasound energy and acquire ultrasound data; a processor, coupled to and configured to control the imaging unit; a pairing unit, coupled to the processor and configured to establish a preliminary data connection with the multi-use electronic display device; a communication unit, coupled to the processor and configured to communicate ultrasound image data to the multi-use electronic display device. The processor is coupled to the first communication interface, imaging unit, and pairing unit and is operable to receive imaging configuration data from the multi-use electronic display device. The multi-use electronic display device comprises: an external interface configured to communicate with the communication interface and receive said transmitted ultrasound image data information, a second processor, configured to convert said ultrasound image data information into an ultrasound image, a memory, coupled to said second processor; and a user interface, coupled to the second processor and operable to display the ultrasound image.

[0019] In some embodiments the external interface comprises first and second wireless transceivers and the communication unit comprises a third wireless transceiver, configured to form a first data connection with the first wireless transceiver; and a fourth wireless transceiver, configured to form a second data connection with the second wireless transceiver. The first and second wireless transceivers may operate according to distinct communication protocols. In some embodiments, information for setting up said second data connection is communicated via the first data connection. In an example embodiment

the first wireless transceiver is provided by a Bluetooth module. In the example embodiment the second wireless transceiver may be provided by a Wi-Fi module.

[0020] In some embodiments the ultrasound imaging device comprises a sensing unit. The sensing unit may, for example, comprise one or more of an inertial measurement unit and a global positioning sensor. One or both of the ultrasound imaging device and multi-use display device may be battery powered portable devices.

[0021] In some embodiments, commanding the selected one of the ultrasound imaging devices to acquire ultrasound image data comprises transmitting imaging parameters to the selected one of the ultrasound imaging devices and the method comprises automatically establishing initial values for the imaging parameters at the multi-use imaging device based on the ultrasound procedure.

[0022] Another aspect of the invention provides a diagnostic ultrasound imaging system. The diagnostic ultrasound imaging system according to this aspect comprises a multi-use display device operable to wirelessly connect with at least one ultrasound imaging device. The multi-use display device may comprise an off-the-shelf device such as a smart phone, tablet computer, personal digital assistant (PDA) or portable computer configured with software (e.g. an app) which provides functions for establishing a data connection to an ultrasound imaging device, receiving ultrasound image data from the ultrasound imaging device and displaying an ultrasound image on a display of the multi-use display device. The multi-use display device may be operable for uses other than ultrasound imaging.

[0023] The multi-use display device comprises a processor, a user interface, a memory, and an external interface. The multi-use display device is operable to wirelessly communicate with the ultrasound imaging device through the external interface to configure imaging parameters and receive ultrasound data.

[0024] In some embodiments, the external interface of the multi-use display device may comprise one or more wireless transceivers that provide wireless communications with other devices using a plurality of different wireless communication protocols.

[0025] In an example embodiment the ultrasound imaging device comprises a processor, an imaging unit, a pairing unit, a memory, and a communication unit operable to connect with the multi-use display device.

[0026] In some embodiments, the ultrasound imaging device may further comprise a sensing unit to generate ultrasound imaging device selection information on the current state of the ultrasound imaging device.

[0027] In some embodiments, the ultrasound imaging device may operate in at least a standby state and an active state. The ultrasound imaging device may consume less power in the standby state.

[0028] In some embodiments, the ultrasound imaging device is a handheld or hand-carried system. The ultrasound imaging device may be a laptop or cart-based system in the alternative.

[0029] Another aspect of the present invention provides a method for using a multi-use display device to wirelessly control and receive data from an ultrasound imaging device. The method comprises: acquiring ultrasound imaging device selection information from one or more ultrasound imaging devices, selecting an ultrasound imaging device based on the plurality of ultrasound imaging device selection information, establishing communication with the selected ultrasound imaging device, directing the selected ultrasound imaging device to acquire ultrasound data, receiving the acquired ultrasound data from the ultrasound imaging device, and displaying the ultrasound data acquired by the ultrasound imaging device on the multi-use display device.

[0030] In some embodiments, the ultrasound imaging device selection information may comprise at least one of the following: information gathered from one or more available ultrasound imaging devices, information from the user, and previously stored information.

[0031] In some embodiments, the plurality of ultrasound imaging device selection information from one or more ultrasound imaging devices may be acquired while one or more of the ultrasound imaging devices are in a standby state. A selected one of the ultrasound imaging devices may subsequently be transitioned from a standby state to an

active state by a user control input or automatically. In some embodiments, the user control input is received at the user interface of a multi-use display device and software on the multi-use display device causes the multi-use display device to transmit a signal to the ultrasound imaging device that causes the ultrasound imaging device to transition to the active state.

[0032] In some embodiments an ultrasound device list may be generated based at least in part on the ultrasound imaging device selection information. This list may also be displayed on multi-use display device **102**.

[0033] In some embodiments, selecting an ultrasound imaging device may comprise receiving an input from a user via a user interface on the multi-use display device.

[0034] In some embodiments, selecting an ultrasound imaging device may comprise an automated step performed by the multi-use display device based on the plurality of pieces of ultrasound imaging device selection information. For example, the multi-use display device may be configured to automatically select the closest ultrasound imaging device, or automatically select the ultrasound imaging device that was previously connected.

[0035] Another aspect of the invention provides ultrasound imaging devices as described herein.

[0036] Further aspects and example embodiments are illustrated in the accompanying drawings and/or described in the following description.

BRIEF DESCRIPTION OF THE DRAWINGS

[0037] The accompanying drawings illustrate non-limiting example embodiments of the invention.

[0038] FIG. 1 is a schematic diagram of an ultrasound imaging system according to an example embodiment of the present disclosure.

[0039] FIG. 2 is a process diagram that illustrating an operation of the multi-use electronic display device in the communication method according to an example embodiment of the present disclosure.

[0040] FIG. 3 is a diagram illustrating a preliminary connection between an ultrasound imaging device and multi-use display device and a primary connection via a wireless local area network according to an example embodiment of the present disclosure.

[0041] FIG. 4 is a diagram illustrating a preliminary connection between an ultrasound imaging device and multi-use display device and a primary connection via a personal area network according to an example embodiment of the present disclosure.

[0042] FIG. 5 is a signal flow diagram illustrating signal flows between devices in the communication method according to an example embodiment of the present disclosure.

[0043] FIG. 6 is an example of a screen shown on the multi-use display device of FIG 1.

[0044] FIG. 7 is an example of a screen shown on multi-use display device of FIG 1.

[0045] FIG. 8 is an example of a screen shown on multi-use display device of FIG 1.

[0046] FIG. 9 is schematic diagram of an example embodiment of the ultrasound imaging system.

DETAILED DESCRIPTION

[0047] Throughout the following description, specific details are set forth in order to provide a more thorough understanding of the invention. However, the invention may be practiced without these particulars. In other instances, well known elements have not been shown or described in detail to avoid unnecessarily obscuring the invention. Accordingly, the specification and drawings are to be regarded in an illustrative, rather than a restrictive sense.

[0048] Throughout the following description, a “target object” may be a target inanimate object or a target animate object, which is displayed via an image. Also, the target object

may be a part of a human body and may include the liver, the heart, the womb, the brain, the breast, the abdominal region, or the like, a fetus, or a cross-section of a part of the human body. Throughout the following description, a “user” may be a medical expert including a doctor, a nurse, a medical laboratory technologist, a sonographer, or the like.

[0049] FIG. 1 is a schematic diagram of an ultrasound imaging system **100** in accordance with an embodiment of the disclosure. Ultrasound imaging system **100** comprises a multi-use display device **102** and an ultrasound imaging device **104**.

[0050] A communication link **106** between multi-use display device **102** and ultrasound imaging device **104** may be established. Multi-use display device **102** may gather information about ultrasound imaging device **104** by way of link **106**. Multi-use display device **102** may establish communication link **106** with one or more other ultrasound imaging devices **104** (not shown in Figure 1) and may obtain and use information about the ultrasound imaging devices **104** to select among two or more ultrasound imaging devices **104**.

[0051] Ultrasound imaging device **104** may be wirelessly connected with multi-use display device **102**. Ultrasound imaging device **104** may transmit an ultrasound signal to a target object according to a control signal that is transmitted from multi-use display device **102**.

[0052] Still referring to FIG. 1, multi-use display device **102** may comprise a processor **120**, memory **124**, user interface **120**, and an external interface **122**. Processor **120** may be a general purpose CPU or may be a low power/mobile specific processor. Processor **120** is coupled with memory **124**. Memory **124** includes storage for program and program operating code. One or more programs **124A** in memory **124** coordinates interactions of multi-use display device **102** with ultrasound imaging devices **104** as described herein.

[0053] User interface **120** is coupled with processor **120** and may comprise both the software and hardware components necessary to interface with a user of the multi-use display device. User interface **120** may comprise physical input devices such as a touch-sensitive display screen, keyboard, microphone, or function buttons. User interface **120**

may further comprise output devices such as a color, grayscale, or black and white display screen, audio speaker/output, vibrating or LED indicators.

[0054] External interface **122** is coupled with processor **120** and provides connectivity of multi-use display device **102** with ultrasound imaging device(s) **104** through communication link(s) **106**. External interface **122** may also be operable to communicate with another device, such as a web server.

[0055] Processor **120** may generate control signals to control an operation of ultrasound imaging device **104** according to information that is provided via user interface **126**. The control signals may include control signals that control ultrasound imaging device **104** to generate ultrasound signals, and control signals that control how ultrasound imaging device **104** handles transmission and reception of the ultrasound signal. In addition, processor **120** may control wireless communication with ultrasound imaging device **104**, and may control generation and display of an ultrasound image on a display of user interface **126** based on ultrasound image data provided from ultrasound imaging device **104**.

[0056] Still referring to FIG. 1, ultrasound imaging device **104** may comprise a processor **140**, memory **144**, imaging unit **146**, pairing unit **148**, and a communication unit **142**. Processor **140** may comprise a general purpose CPU, a low power/mobile specific processor, a field programmable gate array, a combination of two or more of these or the like.

[0057] Imaging unit **146** is operable to acquire ultrasound image data of a target object based on control signals from processor **140**. Imaging unit **146** may comprise a transmitter for generating ultrasound energy and a receiver for receiving ultrasound energy reflected from the target object. Imaging unit **146** may further comprise an analog-to-digital converter for digitizing the received ultrasound energy into digital ultrasound data. Imaging unit **146** may further comprise one or more beamformers to combine and focus the received ultrasound energy along a desired scanline. Imaging unit **146** may further comprise a signal processor to apply filtering or compression to the ultrasound image data.

Imaging unit **146** may also comprise a scan converter for converting the ultrasound image data into a specific display format.

[0058] Processor **120** is coupled with memory **124**. Memory **124** includes storage for program and program operating code. One or more programs in memory **124** coordinates the operation of ultrasound imaging device **104** as described herein. Memory **124** may also be used to store information about ultrasound imaging device **104** and/or ultrasound image data.

[0059] Pairing unit **148** is operable to establish communication link **106** between communication unit **142** and external interface **122** of multi-use display device **102**. Communication unit **142** may comprise one or more wireless transceivers.

[0060] In some embodiments, ultrasound imaging device **104** may function in at least a standby state and an active state. In the standby state, some of the internal subsystems of ultrasound imaging device **104** may be powered and thus functional while others are powered down. For example, in the standby state all subsystems may be powered down except for pairing unit **148** and communication unit **142**. In the standby state, ultrasound imaging device **102** is able conserve power, which may extend battery life. In the active state, all subsystems of ultrasound imaging device **102** may be powered. Ultrasound imaging devices **104** may be transitioned from a standby state to an active state by activating a control on the ultrasound imaging device **104**. Alternatively, ultrasound imaging devices **104** may be transitioned from a standby state to an active state in response to a signal or command received through communication unit **142**.

[0061] Ultrasound imaging devices **104** may have any of a wide range of various sizes and configurations. For example, ultrasound imaging device **104** may be handheld or hand carried. Alternatively, ultrasound imaging device **104** may be in a laptop form factor or a more traditional cart-based device. In some preferred embodiments, ultrasound imaging devices **104** have the form of hand-held battery-powered probes.

[0062] Communication link **106** may comprise more than one communication protocol. In some embodiments, a first protocol is applied for initial discovery of an ultrasound imaging device **104** by multi-use display device **102** as well as acquisition of data useful

for selecting the ultrasound imaging device **104** and information useful for establishing a communications link according to a second protocol with the ultrasound imaging device **104**. The second protocol may provide a longer range and/or higher bandwidth connection than the first protocol.

[0063] For example, a preliminary connection may be a Bluetooth™ low energy (BLE) connection and a primary connection may be a Wi-Fi connection. Alternatively, one or more of the following protocols may be used: wireless local area network (LAN), Bluetooth, ZigBee™, Wi-Fi Direct (WFD), ultra wideband (UWB), infrared data association (IrDA), Bluetooth low energy (BLE), near field communication (NFC), wireless broadband internet (Wibro), world interoperability for microwave access (WiMAX), shared wireless access protocol (SWAP), radio frequency (RF) communications and the like.

[0064] Once the desired ultrasound imaging device **104** is selected, the preliminary connection may be operable to setup a primary connection for communication and data transfer between multi-use display device **102** and ultrasound imaging device **104**.

[0065] In some embodiments, software processes running on multi-use display device **102** play a role in selection of an ultrasound imaging device **104**. To give three examples, selection may be based on one or more of: capabilities of the ultrasound imaging device **104**; proximity to multi-use display device **102**; and rights of a user of multi-use display device **102**. Selection may also be based on combinations of two or more of these or other factors with one another.

[0066] In a first example, a user selects an ultrasound imaging procedure to perform. Not all of ultrasound imaging devices **104** are suitable for the procedure. Multi-use display device **102** may display for selection only those available ultrasound imaging devices **104** that are suitable for the procedure. This filtering may be based on information regarding the configuration and/or capabilities of the ultrasound imaging devices **104** provided by way of preliminary connections to those devices.

[0067] As a second example, multi-use display device **102** determines distance to each of ultrasound imaging devices **104** and sorts a list of available ultrasound imaging devices

104 by distance. Distance may be measured by monitoring signal strength of signals from the ultrasound imaging devices on the preliminary communication channel.

[0068] As a third example, different multi-use display devices **102** may have rights to access different ultrasound imaging devices. Some ultrasound imaging devices may be available only to physicians. Others may be available only to members of a certain department. Others may be available only to certain individuals, and so on. Multi-use display device **102** may use information obtained from the preliminary data connection to determine whether it is authorized for use with the ultrasound imaging device **104** and may display for selection only those ultrasound imaging devices **104** for which the multi-use display device **102** is authorized.

[0069] In some embodiments, the preliminary protocol is a protocol that does not require the ultrasonic imaging device to be powered. For example, the preliminary protocol may comprise an RFID protocol. An RFID chip on the ultrasonic imaging device **104** may contain information identifying the ultrasonic imaging device **104**, describing capabilities of the ultrasonic imaging device **104**, and/or describing how to establish a second (primary) data connection to the ultrasonic imaging device **104**. In such embodiments, multi-use display device **102** may incorporate an RFID reader or system **100** may include a separate RFID reader with which multi-use display device **102** communicates by a suitable protocol, for example Bluetooth.

[0070] FIG. 2 is a flowchart illustrating an operation procedure **S200** of the multi-use electronic display device in the communication method according to an embodiment of the present disclosure.

[0071] In operation **S202**, multi-use display device **102** acquires a plurality of pieces of ultrasound imaging device selection information. The plurality of pieces of information may be acquired from one or more ultrasound imaging devices, from the user, or from memory **124**.

[0072] In order to obtain ultrasound imaging device selection information from one or more ultrasound imaging devices, multi-use display device **102** may search for ultrasound

imaging devices **104** that are within range and may establish a preliminary connection with each of them.

[0073] In some embodiments, ultrasound imaging devices **104** advertise their presence. For example, communication unit **142** may include a Bluetooth Low Energy module that is configured to periodically advertise the presence of ultrasound imaging device **104**. Upon reception of one of these advertisements, multi-use display device **102** may attempt to establish a preliminary connection with ultrasound imaging device **104** in order to request ultrasound imaging device selection information. Alternatively, the advertisements may also contain some or all of the ultrasound imaging device selection information.

[0074] As part of the preliminary connection process, multi-use display device **102** and/or ultrasound imaging device **104** may perform an authentication step. An authentication step may involve the exchange of credentials (e.g. username/password or digital certificate information) between multi-use display device **102** and ultrasound imaging device **104**. In some embodiments, an authentication server, which may be network-based or cloud-based, mediates the authentication. The authentication step may block further execution of method **S200** if the multi-use display device **102** is not authorized to work with the ultrasound imaging device **104** or *vice versa*.

[0075] Ultrasound imaging device selection information received from an ultrasound imaging device **104** may include at least one of identity information of the ultrasound imaging device, function information about the ultrasound imaging device, and status information about the ultrasound imaging device.

[0076] The identity information of the ultrasound imaging device may include a universally unique identifier (UUID), a name determined by the manufacturer and/or a user-defined device name. For example, a user-defined device name could be “DrSeymourConvex”.

[0077] The function information about the ultrasound imaging device may include, for example, one or more of the following: power information (e.g. state of charge of an onboard battery), transducer information, or imaging capabilities. Power information may

include power type, such as line or battery or information on the battery. For example, battery information may include type, capacity, state of charge, and/or an estimated life. Transducer information may include the geometry, such as convex or linear, the number of elements, and the number of channels. Imaging capabilities may include available imaging modes such as B-Mode, M-Mode, Color Doppler, Power Doppler, and the like. Transducer information may also include physical features of the probe, such as whether or not a needle guide is present.

[0078] The status information about the ultrasound imaging device may include one of the following: connection state, boot state. For example, the connection state may include the presence and/or identity of a different multi-use display device connected to the ultrasound imaging device. The boot state may indicate the power state of the ultrasound imaging device, such as a standby state or an active state.

[0079] Multi-use display device **102** may also acquire ultrasound device selection information for ultrasound imaging device **104** based on characteristics of its connection to the ultrasound imaging device **104**. For example, the strength of the wireless connection, or an estimate of proximity based at least in part on the strength of the wireless connection.

[0080] In some embodiments, ultrasound imaging device **104** may comprise additional sensors to report other status information such as temperature, orientation, or position. For example, an inertial measurement sensor may report the 3D orientation of the probe relative to the ground. In another example, a global positioning sensor may indicate the global position of the ultrasound imaging system.

[0081] In some embodiments, the ultrasound device selection information is retrieved from available ultrasound imaging devices **104** in two or more steps. A first step may be used to identify those of ultrasound imaging devices **104** that have a first characteristic. This first characteristic could be a configuration or capability (e.g. transducer type or available imaging modes). Further ultrasound device selection information could then be obtained via the preliminary data connection only for those available ultrasound imaging devices **104** that have the desired characteristic (e.g. only those with curved transducers or

only those capable of colour Doppler imaging or only those with at least 50% battery capacity, etc.).

[0082] Still referring to operation **S202**, multi-use display device **102** may acquire ultrasound imaging selection information by receiving an input from the user. For example, the user may request a particular type of exam or a particular time of day they would like to perform an exam. This input may be received through user interface **126**, for example by input via a touchscreen or based on voice command.

[0083] Multi-use display device **102** may also acquire certain ultrasound imaging device selection information from memory **124**. For example, information specifying which ultrasound imaging devices the user is authorized to operate and which ultrasound imaging device was last used by the user may be stored in memory **124**.

[0084] In operation **S204**, multi-use display device **102** selects an ultrasound imaging device based on the ultrasound imaging device selection information acquired in operation **S202**. The selection may be based on an input from the user received through user interface **126** or may be automated.

[0085] Multi-use display device **102** may generate and display an ultrasound imaging device list based on the plurality of pieces of ultrasound imaging device selection information. The ultrasound imaging device list may display identifiers (e.g. names, allocated numbers, allocated letters or allocated symbols of the ultrasound imaging devices) that correspond to the ultrasound imaging device, and the plurality of pieces of ultrasound imaging device selection information acquired in operation **S202**.

[0086] The ultrasound imaging device list may be filtered or ranked based on the ultrasound imaging device selection information. For example, if the user has indicated that an abdominal exam is desired, the ultrasound imaging device list may display only ultrasound imaging devices with a transducer geometry suitable for abdominal examinations (e.g. convex). In another example, the ultrasound imaging device list may be ranked by physical proximity. In yet another example, the ultrasound imaging device list may be ranked by estimated battery life. Combinations of these are also possible. One

skilled in the art can envision that various criteria could be used and/or combined to match the preference of the user.

[0087] Processor **120** may be configured to automate part or all of the selection. For example, if there is only one device on the ultrasound imaging device list, processor **120** may be configured to skip displaying the list to the user and proceed to the next step. Processor **120** may also be configured to automatically select an ultrasound imaging device based on predetermined or user-selectable criteria. For example, processor **120** may preferentially select the ultrasound imaging device that was used in a preceding session.

[0088] The ultrasound imaging device list may optionally provide a means for locating or identifying a particular ultrasound imaging device. For example, multi-use display device **102** may receive an input from the user through user interface **126** for one or more of the ultrasound imaging devices on the ultrasound imaging device list. In response to receiving the input, multi-use display device **102** may transmit a page signal to the corresponding ultrasound imaging devices via the preliminary connection. Upon reception of the page signal, the ultrasound imaging device may generate an indication for the user. The indication may include a visible, audible, and/or tactile signal, such as a flashing light, audible tone, or a vibration.

[0089] In operation **S206**, multi-use display device **102** establishes a primary communication channel with the ultrasound imaging device selected in **S206**.

[0090] Operation **S206** may involve transmitting information to setup the primary communication channel through the preliminary communication channel. For example, information such as an SSID and a password to setup a WIFI connection may be transmitted through a preliminary Bluetooth connection.

[0091] As part of establishing communication to a particular ultrasound imaging device **104**, multi-use display device **102** may transmit a signal to the ultrasound imaging device selected in operation **S204** to transition it from a standby state to an active state.

[0092] Operation **S206** may additionally configure multi-use display device **102** to work with the selected ultrasonic imaging device **104**. This configuration may involve one or more of:

- configuring multi-use display device **102** to perform any steps required to further process for display ultrasound data to be received from the ultrasound imaging device **104**;
- configuring user interface **126** to provide controls for the various functions of ultrasound imaging device **104**. Optionally, only a subset of the available controls which are required for a procedure specified by the ultrasound imaging device selection information are initially displayed on multi-use display device **102**;
- sizing buffers to accommodate the expected ultrasound imaging data;
- configuring user interface **126** to display ultrasound images from the selected ultrasound imaging device **104**;
- etc.

[0093] In operation **S208**, multi-use display device **102** transmits a control signal to the ultrasound imaging device selected in **S204**. The control signal may contain commands to set the selected ultrasound imaging device **104** into a particular imaging mode. For example, the commands may control values for a number of imaging parameters that are to be used to acquire ultrasound data. In some embodiments initial values for the imaging parameters are set based on an ultrasound procedure to be performed on a patient. The imaging parameters may comprise parameters that relate to aspects of ultrasound imaging such as the nature of ultrasound signals to be transmitted (e.g. waveform, intensity, aperture, frequency, etc.); the nature of beamforming to be applied to the transmit signals; the nature of beamforming to apply to received ultrasound echo signals; the nature of processing to be applied to received ultrasound signals (e.g. gain, filtering etc.); the nature of an image to acquire (e.g. number of scanlines, depth of scanlines, compounding, etc.).

[0094] In operation **S210**, multi-use display device **102** receives ultrasound data acquired by the ultrasound imaging device in response to the control signal transmitted in operation **S208**.

[0095] In operation **S212**, multi-use electronic display device **102** displays the ultrasound image data generated in operation **S214** via user interface **126**.

[0096] Additional processing steps may be performed on the ultrasound data on multi-use electronic display device **102** before it is displayed as an image. For example, the ultrasound data may be scan converted.

[0097] FIG. 3 is a diagram illustrating a preliminary connection between ultrasound imaging device **104** and multi-use display device **102** and a primary connection between the ultrasound imaging device **104** and the multi-use display device **102** via a wireless local area network. In this embodiment, preliminary connection **310** is a Bluetooth connection and primary connection **314** is a Wi-Fi connection. Multi-use display device **102** establishes Bluetooth connection **310** with ultrasound imaging device **104** within a personal area network **306**. Multi-use display device **102** may then transmit configuration information via Bluetooth to ultrasound imaging device **104** in order to establish a Wi-Fi connection **314**.

[0098] Configuration information to setup Wi-Fi connection **314** may comprise an SSID and a password. This configuration information may be encrypted. Alternatively, configuration information may comprise a reference to previously stored information in ultrasound imaging device memory **144**.

[0099] In some embodiments, communications between ultrasound imaging apparatus **104** and multi-use display apparatus **102** are encrypted. In some embodiments, encryption is provided by the wireless protocol used for the primary connection. For example, where the primary connection is a Wi-Fi connection, the connection may be secured by WEP or WPA. In some embodiments, to ensure better security, ultrasound imaging device **104** encrypts ultrasound image data using a separate encryption protocol and multi-use display data **102** decrypts the ultrasound image data before displaying it. In such embodiments, information regarding the encryption (such as a public key from multi-use display device **102**) may be exchanged by way of the preliminary connection or by way of the primary data connection.

[0100] FIG. 4 is a diagram illustration of a preliminary connection between an ultrasound imaging device and multi-use display device and a primary connection via a personal area network. In this embodiment, preliminary connection **310** is a Bluetooth connection and primary connection **416** is a Wi-Fi direct connection. In a similar fashion, Bluetooth connection **310** is established first, and used to establish Wi-Fi direct connection **416**.

[0101] FIG. 5 is signal flow diagram for an example procedure in which multi-use display **102** selects an ultrasound imaging device **104** and performs wireless communication, according to an embodiment of the present disclosure.

[0102] At least one ultrasound imaging device **104** may be in a broadcast state **S500**, and will periodically send a Bluetooth Device Advertisement signal in operation **S504**.

[0103] In operation **S502**, multi-use display device **102** initiates a discovery process. If an advertisement signal is received, multi-use display **102** transmits an Information Request signal (Information REQ) at operation **S506**. Ultrasound imaging device **104** then responds by transmitting an Information Response signal (Information RES) in operation **S508**.

[0104] In operation **S510**, multi-use display device **102** transmits a Bluetooth Connection Request signal (Bluetooth Connection REQ). If the signal is received, ultrasound imaging device **104** sends multi-use display device **102** a Bluetooth Connection Response signal (Bluetooth Connection RES) at operation **S512**. Then multi-use display device **102** and ultrasound imaging device **104** establish a Bluetooth communication channel at operation **S514**.

[0105] In operation **S516**, multi-use display device **102** generates an ultrasound imaging device list from the information acquired during operation **S508** from one or more ultrasound imaging devices **104** and displays an ultrasound imaging device list.

[0106] In operation **S518**, multi-use display device **102** select an ultrasound imaging device from the list of ultrasound imaging devices. This selection may be based on an input received from user interface **126**.

[0107] If the ultrasound imaging device **104** selected in operation **S518** is determined to be in a standby state, multi-use display device **102** will send a Boot Request signal (Boot REQ) at operation **S520**. Ultrasound imaging device **104** then transitions from a standby state to an active state in operation **S522Te**. When the boot process is complete, ultrasound imaging device **104** transmits a Boot Response signal (Boot RES) in operation **S524**.

[0108] In operation **S526** multi-use display device **102** transmits Wi-Fi connection information via the Bluetooth connection. In operation **528**, multi-use display device **102** prepares for a Wi-Fi connection. Similarly, ultrasound imaging devices **104** prepares for Wi-Fi connection in operation **S530** and then transmits a Wi-Fi Connection Request signal (Wi-Fi Connect REQ) in operation **S532**. If multi-use display device **102** receives the Wi-Fi Connection Request signal, multi-use display device **102** transmits a Wi-Fi Connection Response signal (Wi-Fi Connection RES) in operation **S534**. Afterwards, multi-use display device **102** and ultrasound imaging device **104** establish a Wi-Fi communication channel at operation **S536**.

[0109] Next, in operation **S538**, multi-use display device **102** transmits imaging configuration information via the Wi-Fi communication channel. If ultrasound imaging devices **104** receives the imaging configuration information, it prepares for imaging at operation **S540**.

[0110] In operation **S542**, multi-use display device **102** transmits a Start Imaging Request signal (Start Imaging REQ). Ultrasound imaging devices **104** sends a Start Imaging Response signal (Start Imaging RES) in response to the Start Imaging Request signal at operation **S544**. Then ultrasound imaging devices **104** starts imaging in operation **S546**. Ultrasound data is sent from ultrasound imaging devices **104** to multi-use display device **102** multi-use display device **102** via the Wi-Fi communication channel in operation **S548**.

[0111] In operation **S550**, multi-use display device **102** displays the ultrasound data received from ultrasound imaging devices **104**. The ultrasound data may be displayed on user interface **126** or on a secondary display.

[0112] FIG. 6 illustrates an example of a screen that may be shown on ultrasound imaging device **104** during selection operation **S204** of FIG 2. In this example, user interface **126** displays an ultrasound imaging device list comprising an ID indicator **610**, a type indicator **612**, a state indicator **614**, a power indicator **616**, and a page control **618** for ultrasound imaging devices **104A-C**. In this example, the ultrasound imaging device list on the user interface shows that System A and System B are in a standby state, while System C is in an active state.

[0113] FIG. 7 illustrates an example of a screen that may be shown on ultrasound imaging device **104** during selection operation **S204** of FIG. 2 in which an ultrasound imaging device is already connected to another multi-use display device. In this example, System A is already connected so it is moved to the bottom of the list and marked as unavailable on the user interface.

[0114] FIG. 8 illustrates an example of a screen that may be shown on ultrasound imaging device **104** during selection operation **S204** of FIG 2 in which the ultrasound imaging device list is ranked based on the proximity of the ultrasound imaging devices to multi-use display device **102**. In this example, System B is the ultrasound imaging devices with the strongest signal and is displayed at the top of the list.

[0115] FIG. 9 illustrates an ultrasound imaging system in accordance with another embodiment of the present disclosure. In this embodiment, ultrasound imaging device **104** further comprises a sensing unit **900** in communication with processor **140**. Sensing unit **900** is configured to measure ultrasound imaging device state information.

[0116] Sensing unit **900** may also comprise a battery monitor capable of reporting at least one of the following: battery type, state of charge, estimated run-time, battery voltage, battery temperature, battery current.

[0117] Sensing unit **900** may also comprise one or more environmental sensors such as an inertial measurement unit, an accelerometer, a compass, a magnetometer, temperature sensor, or a global positioning sensor.

[0118] In one embodiment, sensing unit **900** comprises a contact sensor able to sense when ultrasound imaging device **104** is in physical contact with a patient or user. For example, a capacitive touch sensor may sense when the transducer is being held by a user's hand.

[0119] An ultrasound imaging system that does not require a display or a user interface can be much more cost effective than traditional ultrasound machines which include dedicated displays and extensive user interfaces.

[0120] The simpler and/or partially automated ultrasound imaging device selection process and simplified pairing process as described herein may reduce the time required to start scanning and make the workflow easier.

[0121] The ability of a multi-user display device to acquire ultrasound imaging device selection information while the ultrasound imaging device is in a low-power standby state may help reduce power consumption and extend battery life.

[0122] In an example use case, an ultrasound department in a hospital has acquired a set of ultrasound imaging devices **104** as described herein. The ultrasound imaging devices **104** are of different types. In this example, some, but not all, of the ultrasound imaging devices **104** incorporate colour Doppler imaging functions. Another difference between the different ultrasound imaging devices **104** is that different ones of the ultrasound imaging devices **104** are equipped with different probes. Some of the ultrasound imaging devices **104** have general purpose linear or convex transducers. Others of the ultrasound imaging devices **104** have special-purpose probes such as probes specialized for trans-vaginal imaging. Others of the imaging devices may be equipped with hardware features such as guides for conducting needle biopsies. In this use example, the hospital acquired ultrasound imaging devices **104** for a cost significantly less than it would have cost to equip the ultrasound imaging suite with conventional ultrasound imaging machines.

[0123] A number of ultrasound technicians work in the hospital. Each of the ultrasound technicians has a tablet computer which runs an ultrasound imaging application. Each of the ultrasound technicians has a full caseload and therefore must be efficient in going about their work. When ultrasound devices **104** are not being used, they are normally

stored in a charging dock so that their internal batteries may be kept charged. As different ultrasound imaging devices **104** are used in different amounts during the day, different ultrasound imaging devices **104** may be at different charge levels. These ultrasound imaging devices **104** that have not been used very much or which have been on the charger for a sufficient period of time will be fully charged or nearly fully charged. Others may be partially discharged. Others still may be nearing the end of their battery life.

[0124] As each ultrasound technician goes about his or her business, the software on his or her tablet computer causes the tablet computer to interrogate ultrasound imaging devices **104** by way of a preliminary communication channel, such as Bluetooth. Thus, each ultrasound technician's tablet computer has, at any given time, information about the available ultrasound imaging devices **104**. When a technician is available to take a new patient, the technician can cause the software to display a list of the available ultrasound imaging devices **104**. Those ultrasound imaging devices **104** that are currently in use by somebody else or currently have very low levels of battery charge may be either excluded from the list or marked as being unavailable. The ultrasound technician may select one of the available ultrasound imaging devices **104**. The selection causes the ultrasound technician's tablet computer to commence pairing with the selected ultrasound imaging device **104**. The pairing may establish a primary data connection such as a Wi-Fi wireless connection. If the selected ultrasound imaging device **104** is not in the place where it should be, or if it is in the midst of one or more other very similar looking ultrasound imaging devices **104**, then the technician may, by activating a control on his or her tablet computer, cause the selected ultrasound imaging device **104** to identify itself.

[0125] In some cases the ultrasound technician may prepare for selecting an ultrasound device **104** by operating software on the tablet computer to identify a type of ultrasound procedure for which the next patient is scheduled. Information about the type of ultrasound procedure may be retrieved from a patient record or appointment booking system or entered by the technician into the tablet computer. In some cases software running on the tablet computer provides a user interface which allows the user to select from among a number of predefined types of ultrasound examination. In such embodiments the selection step may include identifying those of available ultrasound

imaging devices 104 that are suitable for the selected type of ultrasound examination. The software may suppress display of those ultrasound imaging devices **104** that are not suitable for the selected type of ultrasound examination or in some other manner indicate their non-suitability.

[0126] Software on the multi-use display device determines an initial set of imaging parameters to be used by the selected ultrasound imaging device. This initial set of imaging parameters may be predefined and associated with a selected predefined type of ultrasound examination. In some embodiments the imaging parameters are transmitted to the selected ultrasound imaging device before the ultrasound imaging device is initialized (e.g. booted) and an initialization sequence of the ultrasound imaging device configures the ultrasound imaging device according to the imaging parameters while the ultrasound imaging device is being initialized such that the ultrasound imaging device is already configured according to the imaging parameters as soon as it has completed its initialization (e.g. as soon as it is booted up).

[0127] Having identified and taken the selected ultrasound imaging device **104**, the technician proceeds to perform the desired ultrasound examination of the patient. By the time the ultrasound technician has reached the patient's bedside, the pairing process has been completed, the ultrasound imaging device has been configured with imaging parameters suitable for the type of ultrasound examination to be performed and so ultrasound examination can proceed without delay. Ultrasound data from the ultrasound imaging device **104** is provided to the technician's tablet computer. Ultrasound images may be stored on the tablet computer and/or uploaded to a server to be reviewed by a radiologist and/or stored in a medical record.

[0128] When the technician is done with the ultrasound imaging device **104**, the technician may unpair the ultrasound imaging device with his or her tablet computer, for example, by activating a control on the tablet computer and may return the ultrasound imaging device to a charging station for later use.

[0129] In some embodiments, an ultrasound technician may know that he or she will need to use a particular ultrasound imaging apparatus **104** in a short while. Some embodiments

permit the user to reserve the ultrasound imaging device by inputting a command on his or her computer. The tablet computer may confirm the reservation to the ultrasound imaging device, for example, by way of the preliminary communication link. The ultrasound imaging device itself may record the reservation request and start a countdown timer for a reservation time. For example, the system may be set up to allow ultrasound technicians to reserve ultrasound imaging devices 15 minutes in advance only. When such a reservation has been made, the ultrasound imaging device **104** may communicate the reservation information to other multi-use display devices **102** (e.g. the tablet computers of other technicians) such that the other technicians can see that the particular ultrasound imaging device **104** has been reserved and optionally by whom. These communications are made by way of the preliminary data connection in some embodiments.

[0130] Although it is not mandatory, it is convenient that multi-use display devices **102** may be provided by standard off-the-shelf hardware such as smart phones or tablet computers which are customized by the addition of application software having functions for interacting with ultrasound imaging devices **104** and displaying ultrasound images as described herein. It is also convenient and cost effective but not mandatory for ultrasound imaging devices **104** to have no user interface or only minimal user interfaces.

[0131] While the above description contains many specifications, these should not be construed as limitations on the scope of any embodiment, but as exemplifications of various embodiments thereof. Many other ramifications and variations are possible within the teachings of the various embodiments.

[0132] Thus the scope should be determined by the appended claims and their legal equivalents, and not by the examples given.

INTERPRETATION OF TERMS

[0133] Unless the context clearly requires otherwise, throughout the description and the claims:

- “comprise”, “comprising”, and the like are to be construed in an inclusive sense, as opposed to an exclusive or exhaustive sense; that is to say, in the sense of “including, but not limited to”;
- “connected”, “coupled”, or any variant thereof, means any connection or coupling, either direct or indirect, between two or more elements; the coupling or connection between the elements can be physical, logical, or a combination thereof;
- “herein”, “above”, “below”, and words of similar import, when used to describe this specification, shall refer to this specification as a whole, and not to any particular portions of this specification;
- “or”, in reference to a list of two or more items, covers all of the following interpretations of the word: any of the items in the list, all of the items in the list, and any combination of the items in the list;
- the singular forms “a”, “an”, and “the” also include the meaning of any appropriate plural forms.

[0134] Words that indicate directions such as “vertical”, “transverse”, “horizontal”, “upward”, “downward”, “forward”, “backward”, “inward”, “outward”, “vertical”, “transverse”, “left”, “right”, “front”, “back”, “top”, “bottom”, “below”, “above”, “under”, and the like, used in this description and any accompanying claims (where present), depend on the specific orientation of the apparatus described and illustrated. The subject matter described herein may assume various alternative orientations. Accordingly, these directional terms are not strictly defined and should not be interpreted narrowly.

[0135] Embodiments of the invention may be implemented using specifically designed hardware, configurable hardware, programmable data processors configured by the provision of software (which may optionally comprise “firmware”) capable of executing on the data processors, special purpose computers or data processors that are specifically programmed, configured, or constructed to perform one or more steps in a method as explained in detail herein and/or combinations of two or more of these. Examples of specifically designed hardware are: logic circuits, application-specific integrated circuits (“ASICs”), large scale integrated circuits (“LSIs”), very large scale integrated circuits (“VLSIs”), and the like. Examples of configurable hardware are: one or more

programmable logic devices such as programmable array logic (“PALs”), programmable logic arrays (“PLAs”), and field programmable gate arrays (“FPGAs”). Examples of programmable data processors are: microprocessors, digital signal processors (“DSPs”), embedded processors, graphics processors, math co-processors, general purpose computers, server computers, cloud computers, mainframe computers, computer workstations, and the like. For example, one or more data processors in a control circuit for a device may implement methods as described herein by executing software instructions in a program memory accessible to the processors.

[0136] While processes or blocks are presented in a given order, alternative examples may perform routines having steps, or employ systems having blocks, in a different order, and some processes or blocks may be deleted, moved, added, subdivided, combined, and/or modified to provide alternative or sub-combinations. Each of these processes or blocks may be implemented in a variety of different ways. Also, while processes or blocks are at times shown as being performed in series, these processes or blocks may instead be performed in parallel, or may be performed at different times.

[0137] In addition, while elements are at times shown as being performed sequentially, they may instead be performed simultaneously or in different sequences. It is therefore intended that the following claims are interpreted to include all such variations as are within their intended scope.

[0138] Certain aspects of the invention may also be provided in the form of a program product. The program product may comprise any non-transitory medium which carries a set of computer-readable instructions which, when executed by a data processor, cause the data processor to execute a method of the invention. Program products according to the invention may be in any of a wide variety of forms. The program product may comprise, for example, non-transitory media such as magnetic data storage media including floppy diskettes, hard disk drives, optical data storage media including CD ROMs, DVDs, electronic data storage media including ROMs, flash RAM, EPROMs, hardwired or preprogrammed chips (e.g., EEPROM semiconductor chips), nanotechnology memory, or the like. The computer-readable signals on the program product may optionally be compressed or encrypted.

[0139] In some embodiments, some aspects of the invention may be implemented in software. For greater clarity, “software” includes any instructions executed on a processor, and may include (but is not limited to) firmware, resident software, microcode, and the like. Both processing hardware and software may be centralized or distributed (or a combination thereof), in whole or in part, as known to those skilled in the art. For example, software and other modules may be accessible via local memory, via a network, via a browser or other application in a distributed computing context, or via other means suitable for the purposes described above.

[0140] Where a component (e.g. a software module, processor, assembly, device, circuit, etc.) is referred to above, unless otherwise indicated, reference to that component (including a reference to a “means”) should be interpreted as including as equivalents of that component any component which performs the function of the described component (i.e., that is functionally equivalent), including components which are not structurally equivalent to the disclosed structure which performs the function in the illustrated exemplary embodiments of the invention.

[0141] Specific examples of systems, methods and apparatus have been described herein for purposes of illustration. These are only examples. The technology provided herein can be applied to systems other than the example systems described above. Many alterations, modifications, additions, omissions, and permutations are possible within the practice of this invention. This invention includes variations on described embodiments that would be apparent to the skilled addressee, including variations obtained by: replacing features, elements and/or acts with equivalent features, elements and/or acts; mixing and matching of features, elements and/or acts from different embodiments; combining features, elements and/or acts from embodiments as described herein with features, elements and/or acts of other technology; and/or omitting combining features, elements and/or acts from described embodiments.

[0142] It is therefore intended that the following appended claims and claims hereafter introduced are interpreted to include all such modifications, permutations, additions, omissions, and sub-combinations as may reasonably be inferred. The scope of the claims

should not be limited by the preferred embodiments set forth in the examples, but should be given the broadest interpretation consistent with the description as a whole.

WHAT IS CLAIMED IS:

1. An ultrasound imaging method comprising, by a multi-use electronic display device:
 - using a first wireless communication protocol, acquiring imaging device selection information from each of one or more ultrasound imaging devices;
 - selecting one of the one or more ultrasound imaging devices for use in an ultrasound procedure based on the selection information;
 - establishing a primary wireless communication link with the selected one of the ultrasound imaging devices according to a second wireless communication protocol different from the first wireless communication protocol;
 - commanding the selected one of the ultrasound imaging devices to acquire ultrasound image data;
 - receiving the ultrasound image data by way of the primary wireless communication link; and
 - displaying the received ultrasound image data on a screen of the multi-use electronic display device.
2. A method according to claim 1 comprising, by the multi-use electronic display device:
 - determining from the selection information a controllable function of the ultrasound imaging device; and
 - in response to determining the controllable function, configuring the multi-use electronic display device to provide at least one user interface control for the controllable function.
3. A method according to either of claim 1 or 2, wherein the selection information comprises battery charge information indicative of states of charge of batteries of the ultrasound imaging devices.

4. A method according to claim 3 wherein selecting one of the one or more ultrasound imaging devices is based at least in part on the battery charge information.
5. A method according to either of claim 1 or 2, wherein selecting one of the one or more ultrasound imaging devices comprises a filtering stage in which those of the ultrasound imaging devices potentially suitable for the ultrasound procedure are identified and a selection stage comprising, if more than one of the ultrasound imaging devices are potentially suitable for the procedure, selecting one of the more than one of the ultrasound imaging devices that are potentially suitable for the procedure.
6. A method according to claim 5 wherein the selection information comprises battery charge information indicative of states of charge of batteries of the ultrasound imaging devices.
7. A method according to claim 6 wherein selecting one of the one or more ultrasound imaging devices is based at least in part on the battery charge information.
8. A method according to any one of claims 5 to 7, wherein the filtering stage comprises selecting those of the ultrasound imaging devices for which the state of charge has at least a threshold value.
9. A method according to any one of claims 5 to 8, wherein:
 - the selection information comprises a reservation status; and
 - the filtering stage comprises selecting those of the ultrasound imaging devices that have a certain reservation status.
10. A method according to any one of claims 5 to 9, wherein:

the selection information comprises an access requirement for each of the one or more ultrasound imaging devices;

the multi-use electronic display is associated with an access right; and

the filtering stage comprises selecting those of the ultrasound imaging devices of which the access right meets or exceeds the access requirement.

11. A method according to any one of claims 5 to 10 wherein:

the selection information comprises a first authentication credential for each of the one or more ultrasound imaging devices; and

the filtering stage comprises:

authenticating the first authentication credential of each of the ultrasound imaging devices; and

selecting those of the ultrasound imaging devices of which the first authentication credential has been successfully authenticated.

12. A method according to any one of claims 5 to 11 wherein:

the multi-use electronic display device has a second authentication credential; and

the filtering stage comprises:

each of the ultrasound imaging devices authenticating the second authentication credential; and

selecting those of the ultrasound imaging devices for which the second authentication credential was successfully authenticated.

13. A method according to any one of claims 1 to 12 wherein the selection information comprises link information for each of the one or more ultrasound imaging devices and establishing the primary wireless communication link with the selected one of the ultrasound imaging devices comprises using the link information to establish data communication between the multi-use display device and the selected ultrasound imaging device according to the second wireless data communication protocol.

14. A method according to any one of claims 1 to 12 further comprising, using the first wireless protocol, acquiring link information for establishing the primary wireless communication link with one or more of the ultrasound imaging devices and establishing the primary wireless communication link with the selected ultrasound imaging device using the link information.
15. A method according to any one of claims 1 to 14, wherein the selection information comprises a size and a configuration of the one or more ultrasound imaging devices.
16. A method according to any one of claims 1 to 15, wherein:
 - each of the one or more ultrasound imaging devices comprises one or more sensors; and
 - the selection information comprises one or more outputs from the one or more sensors.
17. A method according to any one of claims 1 to 16, comprising, before selecting one of the one or more ultrasound imaging devices, displaying at the multi-use display device at least some of the selection information for each of a plurality of the ultrasound imaging devices, the displayed selection information including one or more of:
 - type of an ultrasound transducer type of the ultrasound imaging device;
 - nickname of the ultrasound imaging device;
 - battery state of charge of the ultrasound imaging device; and
 - strength of signals in the first wireless communication protocol received at the multi-use display device from the ultrasound imaging device.
18. A method according to any one of claims 1 to 17, comprising, at the multi-use electronic display device, determining the ultrasound procedure to perform on a patient wherein selecting one of the one or more ultrasound imaging devices

comprises limiting the selection to those of the ultrasound imaging devices that possess an adaptation necessary for the ultrasound procedure.

19. A method according to claim 18 wherein the adaptation comprises a Doppler imaging mode.
20. A method according to claim 18 wherein the adaptation comprises a transducer having a configuration suitable for the determined ultrasound procedure.
21. A method according to claim 18 wherein the adaptation comprises a needle guide.
22. A method according to any one of claims 1 to 21, comprising determining at the multi-use display device a proximity of each of the ultrasound imaging devices to the multi-use electronic display device based on signals received by the multi-use display device from the ultrasound imaging devices according to the first wireless communication protocol and selecting one of the one or more ultrasound imaging devices is based at least in part on the proximities of the ultrasound imaging devices to the multi-use display device.
23. A method according to claim 22 wherein the proximity of each of the ultrasound imaging devices is determined by a strength of the signals received by the multi-use display device from the ultrasound imaging devices.
24. A method according to any one of claims 1 to 23, wherein acquiring imaging device selection information from each of the one or more ultrasound imaging devices is performed while some or all of the ultrasound imaging devices are in a low-power standby state and the method comprises commanding the selected one of the ultrasound imaging devices to switch to a power on state.
25. A method according to any one of claims 1 to 24, wherein commanding the selected one of the ultrasound imaging devices to acquire ultrasound image data

comprises transmitting imaging parameters to the selected one of the ultrasound imaging devices and the method comprises automatically establishing initial values for the imaging parameters at the multi-use imaging device based on the ultrasound procedure.

26. A method according to any one of claims 1 to 25, wherein the multi-use electronic display device comprises a smartphone, laptop computer or tablet computer.
27. A method according to any one of claims 1 to 26, comprising, by way of the first wireless communication protocol commanding the selected one of the ultrasound imaging devices to issue a human-perceptible visual or audible signal.
28. A method according to any one of claims 1 to 27, wherein the first wireless communication protocol is a Bluetooth protocol.
29. A method according to any one of claims 1 to 28, wherein the first wireless communication protocol is a protocol that does not require the ultrasound imaging devices to be powered.
30. A method according to any one of claims 1 to 29, wherein the first wireless communication protocol comprises an RFID protocol.
31. A method according to any one of claims 1 to 30, wherein the selection information comprises a set of image filtering and data compression capabilities of each of the ultrasound imaging devices, and establishing a primary wireless communication link comprises commanding the selected one of the ultrasound imaging devices to use a specified filter and data compression capability.
32. A method according to any one of claims 1 to 31, wherein establishing the primary wireless communication link comprises:

the multi-use electronic display device transmitting a first encryption key to the ultrasound imaging device over the first wireless communication protocol;

the ultrasound imaging device transmitting a second encryption key to the multi-use electronic display device over the first wireless communication protocol;

the multi-use electronic display device encrypting transmissions over the second wireless communication protocol with the second encryption key; and

the ultrasound imaging display device encrypting transmissions over the second wireless communication protocol with the first encryption key.

33. An apparatus for ultrasound imaging, the apparatus comprising:

a multi-use electronic display device comprising:

a first communications system operative to wirelessly communicate data according to a first and a second wireless communication protocol;

a processor;

a first data store containing a program executable by the processor and parameters for one or more ultrasound imaging procedures; and

a screen;

wherein:

the program is configured to:

cause the first communications system to retrieve device selection information from one or more ultrasound imaging devices using the first wireless communication protocol and to store the selection information on the first data store;

cause the processor to select one of the ultrasound imaging devices based on a selected one of the one or more ultrasound imaging procedures and the selection information;

cause the first communications system to establish a primary wireless communication link with the selected one of the ultrasound imaging devices using the second wireless communication protocol;

cause the first communications system to command the selected one of the ultrasound imaging devices to acquire ultrasound image data;

cause the first communications system to receive the ultrasound image data over the primary wireless communication link; and
cause the screen to display the ultrasound image data.

34. An apparatus for ultrasound imaging, the apparatus comprising:
- a multi-use electronic display device comprising:
 - a first communications system operative to wirelessly communicate data according to a first and a second wireless communication protocol;
 - a processor;
 - a first data store containing a program executable by the processor and parameters for one or more ultrasound procedures; and
 - a screen;
 - one or more ultrasound imaging devices, each of the one or more ultrasound imaging devices comprising:
 - a second communications system operative to wirelessly communicate data according to the first and the second wireless communication protocol; and
 - a second data store containing device selection information;
- wherein:
- the program is configured to cause:
 - the first communications system to connect to the second communications system of each of the one or more ultrasound imaging devices using the first wireless communication protocol, retrieve the device selection information stored on the corresponding second data store, and store the device selection information in the first data store;
 - the processor to select one of the ultrasound imaging devices based on a selected one of the one or more ultrasound procedures and the selection information stored on the first data store;
 - the first communications system to establish a primary wireless communication link with the second communications system on the

selected one of the ultrasound imaging devices using the second wireless communication protocol;

the first communications system to cause the selected one of the ultrasound imaging devices to acquire ultrasound image data;

the first communications system to retrieve the ultrasound image data over the primary wireless communication link; and

the screen to display the ultrasound image data.

35. An apparatus according to either of claims 33 or 34, wherein the program is configured to cause the processor to determine from the selection information a controllable function of the ultrasound imaging device, and to configure the display to provide at least one user interface control for the controllable function.
36. An apparatus according to any one of claims 33 to 35, wherein the selection information comprises battery charge information indicative of states of charge of batteries of the ultrasound imaging devices.
37. An apparatus according to claim 36 wherein the program is configured to cause the processor to select one of the one or more ultrasound imaging devices based at least in part on the battery charge information.
38. An apparatus according to either of claims 33 or 34, wherein the program configures the processor to select one of the one or more ultrasound imaging devices by filtering those of the ultrasound imaging devices potentially suitable for the selected ultrasound procedure, and then performing a selection stage comprising, if more than one of the ultrasound imaging devices are potentially suitable for the selected ultrasound procedure, selecting one of the more than one of the ultrasound imaging devices that are potentially suitable for the procedure.

39. An apparatus according to claim 38 wherein the selection information comprises battery charge information indicative of states of charge of batteries of the ultrasound imaging devices.
40. An apparatus according to claim 39 wherein the program is configured to cause the processor to select one of the one or more ultrasound imaging devices based at least in part on the battery charge information.
41. An apparatus according to either of claims 39 or 40, wherein the filtering comprises selecting those of the ultrasound imaging devices for which the state of charge has at least a threshold value.
42. An apparatus according to any one of claims 38 to 41, wherein:
 - the selection information comprises a reservation status; and
 - the filtering comprises selecting those of the ultrasound imaging devices that have a certain reservation status.
43. An apparatus according to any one of claims 38 to 42, wherein:
 - the selection information comprises an access requirement for each of the one or more ultrasound imaging devices;
 - an access right is stored on the first data store; and
 - the filtering comprises selecting those of the ultrasound imaging devices of which the access right meets or exceeds the access requirement.
44. An apparatus according to any one of claims 38 to 43 wherein:
 - the selection information comprises a first authentication credential for each of the one or more ultrasound imaging devices; and
 - the filtering comprises:
 - authenticating the first authentication credential of each of the ultrasound imaging devices; and

selecting those of the ultrasound imaging devices of which the first authentication credential has been successfully authenticated.

45. An apparatus according to any one of claims 38 to 44 wherein:
 - a second authentication credential is stored on the first data store;
 - the program is configured to cause:
 - the first communications system to transmit the second authentication credential to each of the ultrasound imaging devices;
 - the first communications system to retrieve an authentication result from each of the ultrasound imaging devices; and
 - the filtering comprises selecting those of the ultrasound imaging devices for which the retrieved authentication result was successful.
46. An apparatus according to any one of claims 33 to 45 wherein the selection information comprises link information for each of the one or more ultrasound imaging devices and the program is configured to cause the processor to establish the primary wireless communication link with the selected one of the ultrasound imaging devices using the link information to establish data communication with the selected ultrasound imaging device according to the second wireless data communication protocol.
47. An apparatus according to any one of claim 33 to 46, wherein the selection information comprises information for establishing the primary wireless communication link with the selected ultrasound imaging device.
48. An apparatus according to any one of claims 33 to 47, wherein the selection information comprises a size and a configuration of the one or more ultrasound imaging devices.
49. An apparatus according to any one of claims 33 to 48, wherein:

each of the one or more ultrasound imaging devices comprises one or more sensors; and

the selection information comprises one or more outputs from the one or more sensors.

50. An apparatus according to any one of claims 33 to 49, wherein the program is configured to cause the display to display at least some of the selection information for each of a plurality of the ultrasound imaging devices, before causing the processor to select one of the one or more ultrasound imaging devices based at least in part on user input to the multi-use electronic display device, wherein displayed selection information comprises one or more of:
 - type of an ultrasound transducer type of the ultrasound imaging device;
 - nickname of the ultrasound imaging device;
 - battery state of charge of the ultrasound imaging device; and
 - strength of signals in the first wireless communication protocol received at the first communications system from the ultrasound imaging device.
51. An apparatus according to any one of claims 33 to 50, wherein the program is configured to cause the processor to select one of the one or more ultrasound imaging devices by steps comprising limiting the selection to those of the ultrasound imaging devices that possess an adaptation necessary for the ultrasound procedure.
52. An apparatus according to claim 51 wherein the adaptation comprises a Doppler imaging mode.
53. An apparatus according to claim 51 or 52 wherein the adaptation comprises a transducer having a configuration required for the determined ultrasound procedure.

54. An apparatus according to anyone of claims 51 to 53 wherein the adaptation comprises a needle guide.
55. An apparatus according to any one of claims 33 to 54 wherein the program is configured to cause the processor to determine a proximity of each of the ultrasound imaging devices based on signals received by the first communications system from the ultrasound imaging devices according to the first wireless communication protocol and to select one of the one or more ultrasound imaging devices based at least in part on the proximities of the ultrasound imaging devices to the multi-use display device.
56. An apparatus according to claim 55 wherein the program is configured to cause the processor to determine the proximity of each of the ultrasound imaging devices by a strength of the signals received by the first communications system from the ultrasound imaging devices.
57. An apparatus according to any one of claims 33 to 56, wherein retrieving selection information from each of the one or more ultrasound imaging devices is performed while some or all of the ultrasound imaging devices are in a low-power standby state and the program is configured to cause the first communications system to command the selected one of the ultrasound imaging devices to switch to a power on state.
58. An apparatus according to any one of claims 33 to 57, wherein causing the selected one of the ultrasound imaging devices to acquire ultrasound image data comprises the first communications system transmitting imaging parameters to the selected one of the ultrasound imaging devices, and the program is configured to cause the processor to establish initial values for the imaging parameters based on the selected ultrasound procedure.

59. An apparatus according to any one of claims 33 to 58, wherein the multi-use electronic display device comprises a smartphone, laptop computer or tablet computer.
60. An apparatus according to any one of claims 33 to 59, wherein the program is configured to cause the first communications system to transmit by way of the first wireless communication protocol to the selected one of the ultrasound imaging devices a command for an audio-visual module to emit a human-perceptible visual or audible signal.
61. An apparatus according to any one of claims 33 to 60, wherein the first wireless communication protocol is a Bluetooth protocol.
62. An apparatus according to any one of claims 33 to 61, wherein the first wireless communication protocol is a protocol that does not require the ultrasound imaging devices to be powered.
63. An apparatus according to any one of claims 33 to 62, wherein the first wireless communication protocol comprises an RFID protocol.
64. An apparatus according to any one of claims 33 to 63, wherein the selection information comprises a set of image filtering and data compression capabilities of each of the ultrasound imaging devices, and establishing a primary wireless communication link comprises commanding the selected one of the ultrasound imaging devices to use a specified filter and data compression capability.
65. An ultrasound imaging devices comprising:
 - a communications system configured to send and receive data over a first and a second wireless communication protocol;
 - a data store containing device selection information; and
 - an ultrasound imaging module;

wherein:

the ultrasound imaging device is configured to transmit the device selection information to a multi-use electronic display device in response to a request received at the communications system using the first wireless communication protocol and to acquire ultrasound image data using the ultrasound imaging module and transmit the ultrasound image data using the second wireless communication protocol in response to a command received at the communications system.

66. An ultrasound imaging device according to claim 65, wherein the selection information comprises battery charge information indicative of a state of charge of batteries of the ultrasound imaging device.
67. An ultrasound imaging device according to either of claim 65 or 66, wherein the selection information comprises a reservation status.
68. An ultrasound imaging device according to any one of claims 65 to 67, wherein the selection information comprises an access requirement for the ultrasound imaging device.
69. An ultrasound imaging device according to any one of claims 65 to 68, wherein the selection information comprises a first authentication credential for the ultrasound imaging device.
70. An ultrasound imaging device according to any one of claims 65 to 69, wherein:
 - the ultrasound imaging device comprises a processor configured to authenticate an authentication credential received by the communications system and to;
 - and
 - cause the communications system to transmit results of the authentication to a multi-use electronic display device.

71. An apparatus according to any one of claims 65 to 70, wherein the selection information comprises a size and a configuration of the ultrasound imaging device.
72. An ultrasound imaging device according to any one of claims 65 to 71, wherein:
 - the ultrasound imaging device comprises one or more sensors; and
 - the selection information comprises one or more outputs from the one or more sensors.
73. An ultrasound imaging device according to any one of claims 65 to 72, wherein transmitting the device selection information is performed while the ultrasound imaging device is in a low-power standby state and the ultrasound imaging device is configured to switch to a power on state in response to a command received by the communications system.
74. An ultrasound imaging device according to any one of claims 65 to 73, comprising an audio and/or video module connected to emit a human-perceptible visual or audible signal in response to a command received by way of the first wireless communication protocol.
75. An ultrasound imaging device according to any one of claims 65 to 74, wherein the first wireless communication protocol is a Bluetooth protocol.
76. An ultrasound imaging device according to any one of claims 65 to 75, wherein the first wireless communication protocol is a protocol that does not require the ultrasound imaging device to be powered.
77. An ultrasound imaging device according to any one of claims 65 to 76, wherein the first wireless communication protocol comprises an RFID protocol.

78. An ultrasound imaging device according to any one of claims 65 to 77 comprising an image filtering and data compression module, wherein:

the selection information comprises a set of image filtering and compression capabilities; and

the communications system is configured to cause the image filtering and compression module to use an image filter and compression specified by a command received at the communications system.

1/8

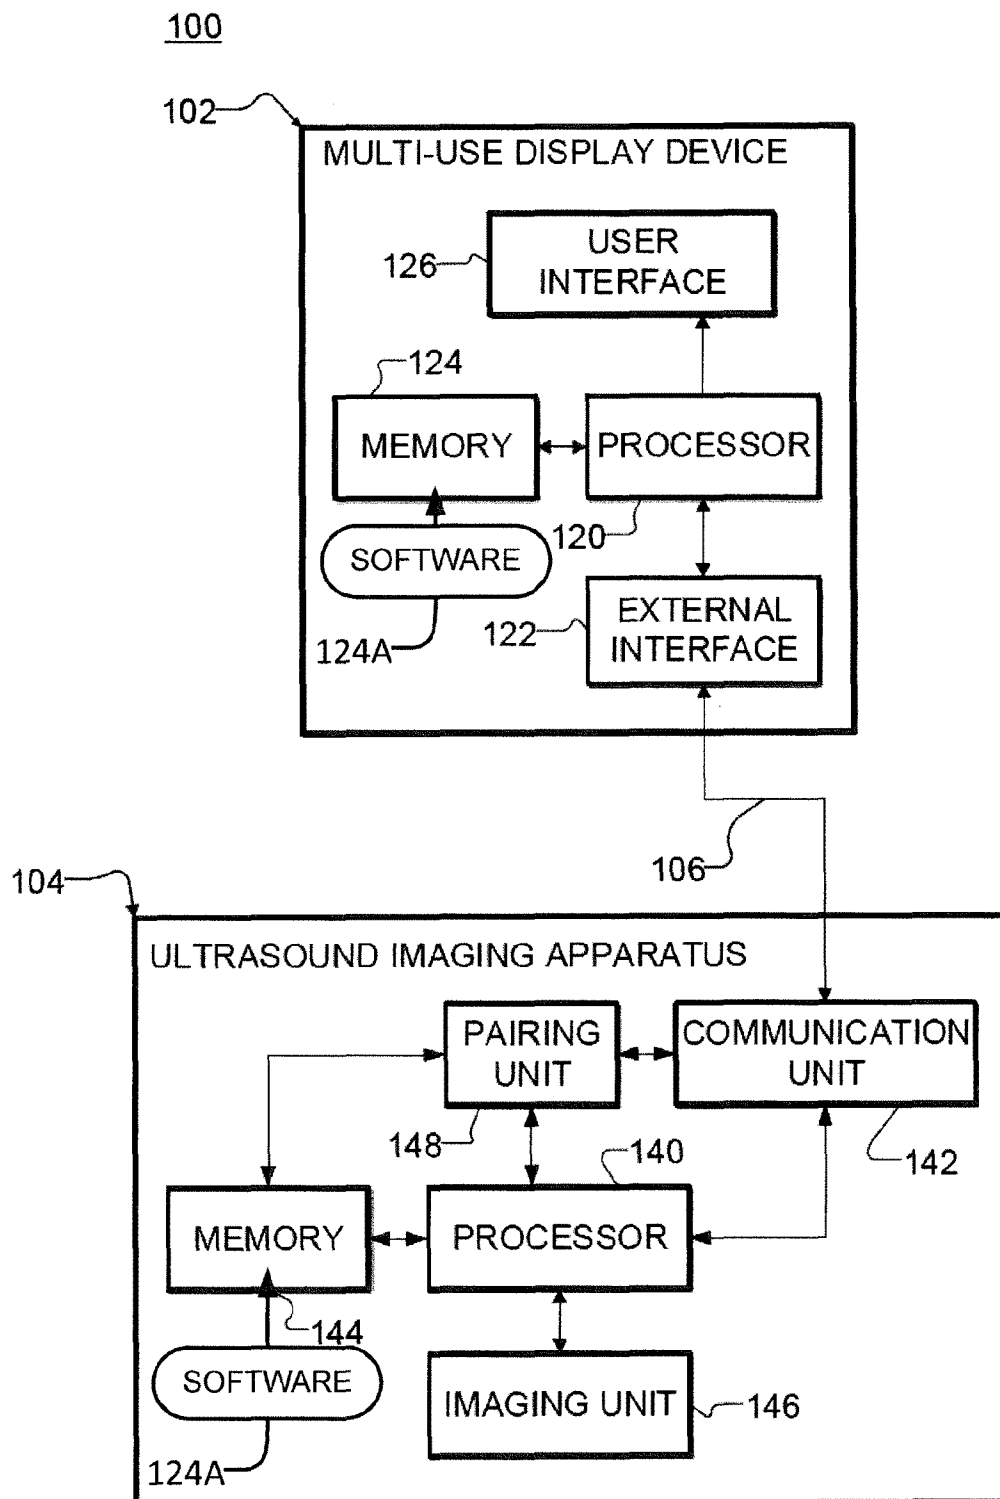


FIG. 1

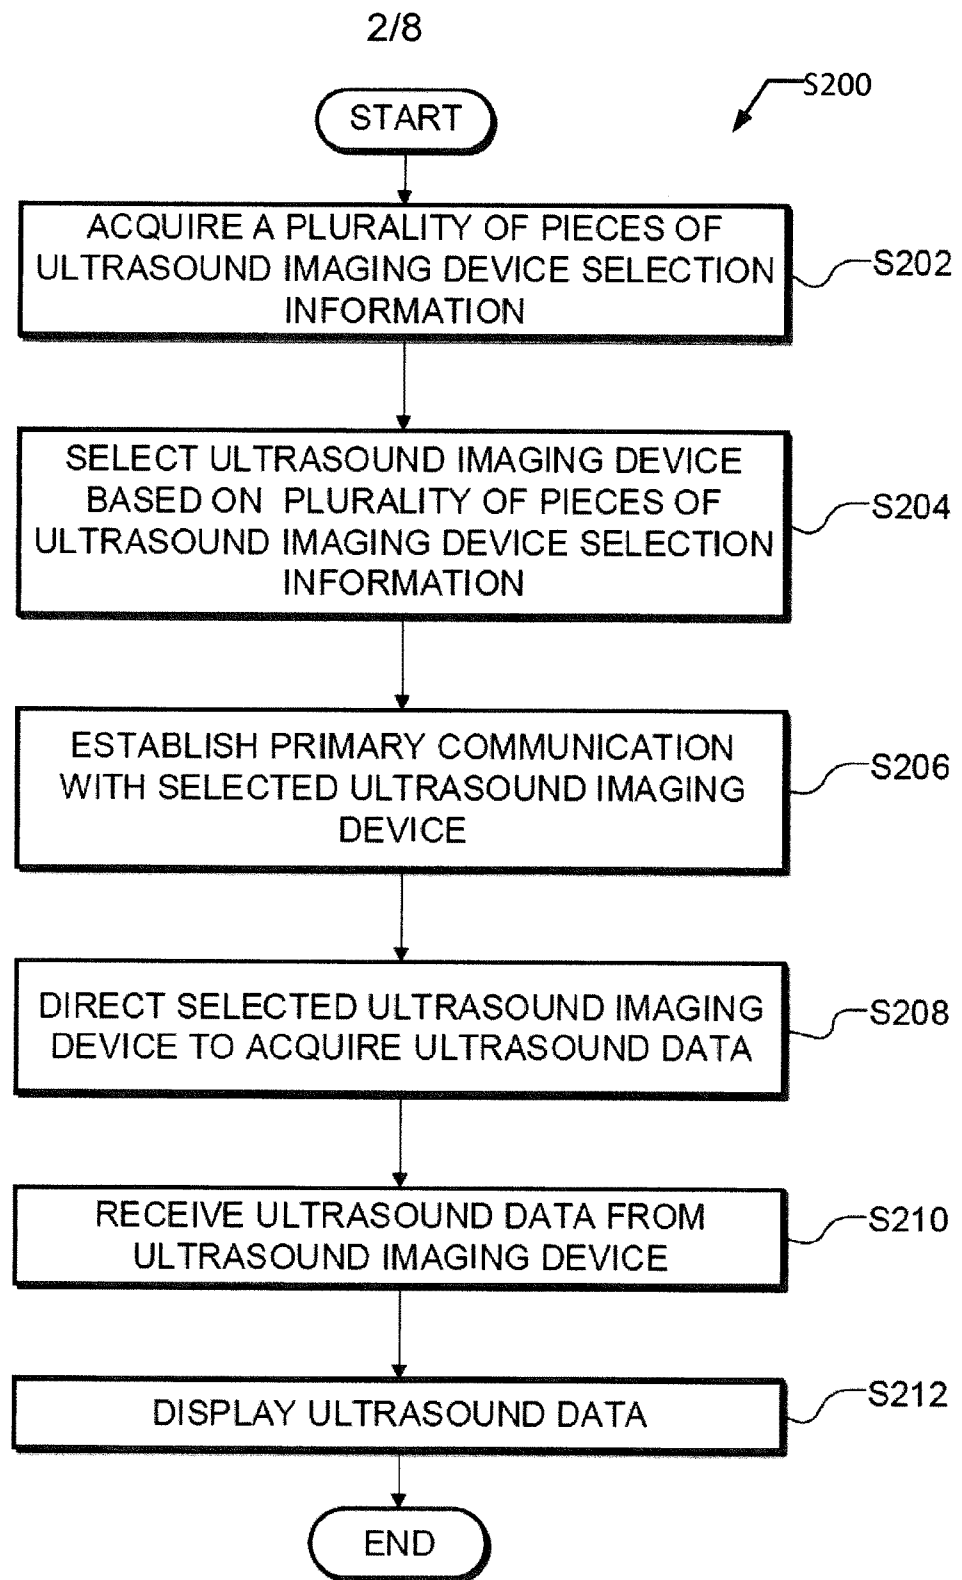


FIG. 2

3/8

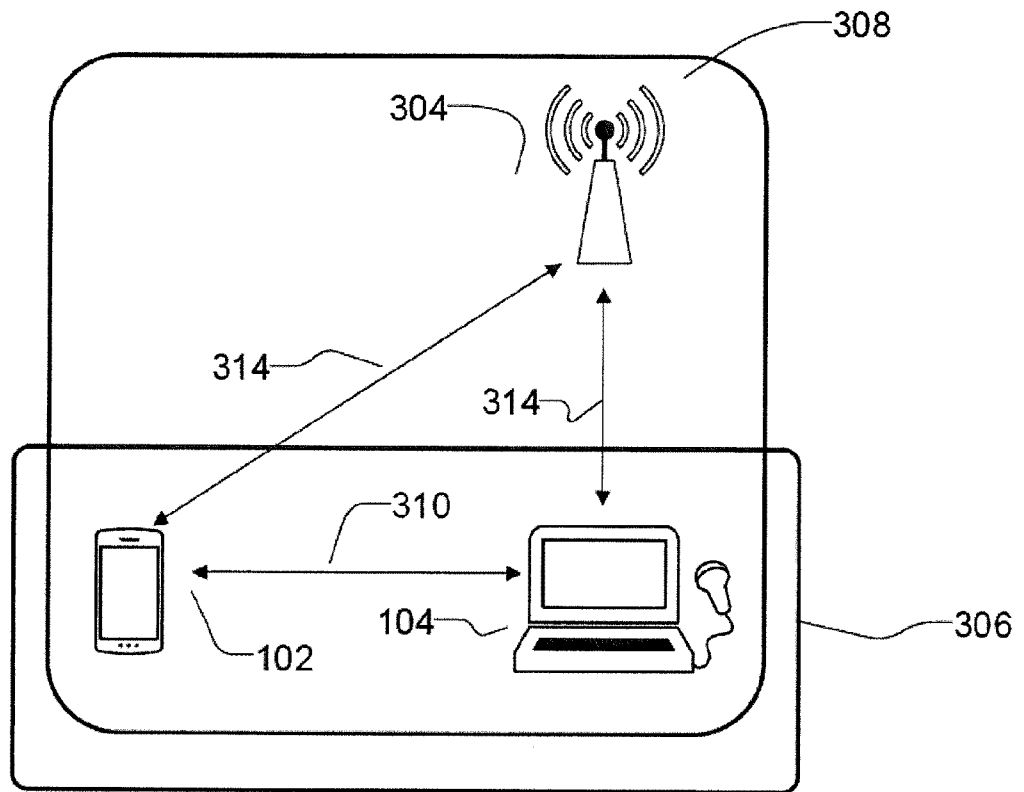


FIG. 3

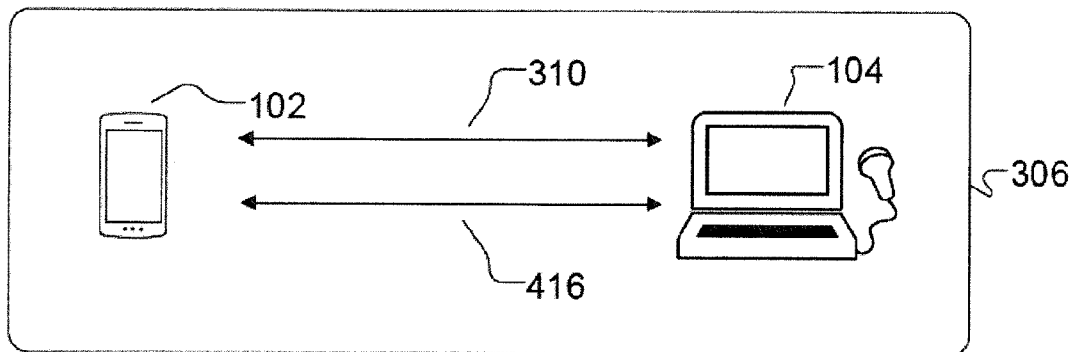


FIG. 4

4/8

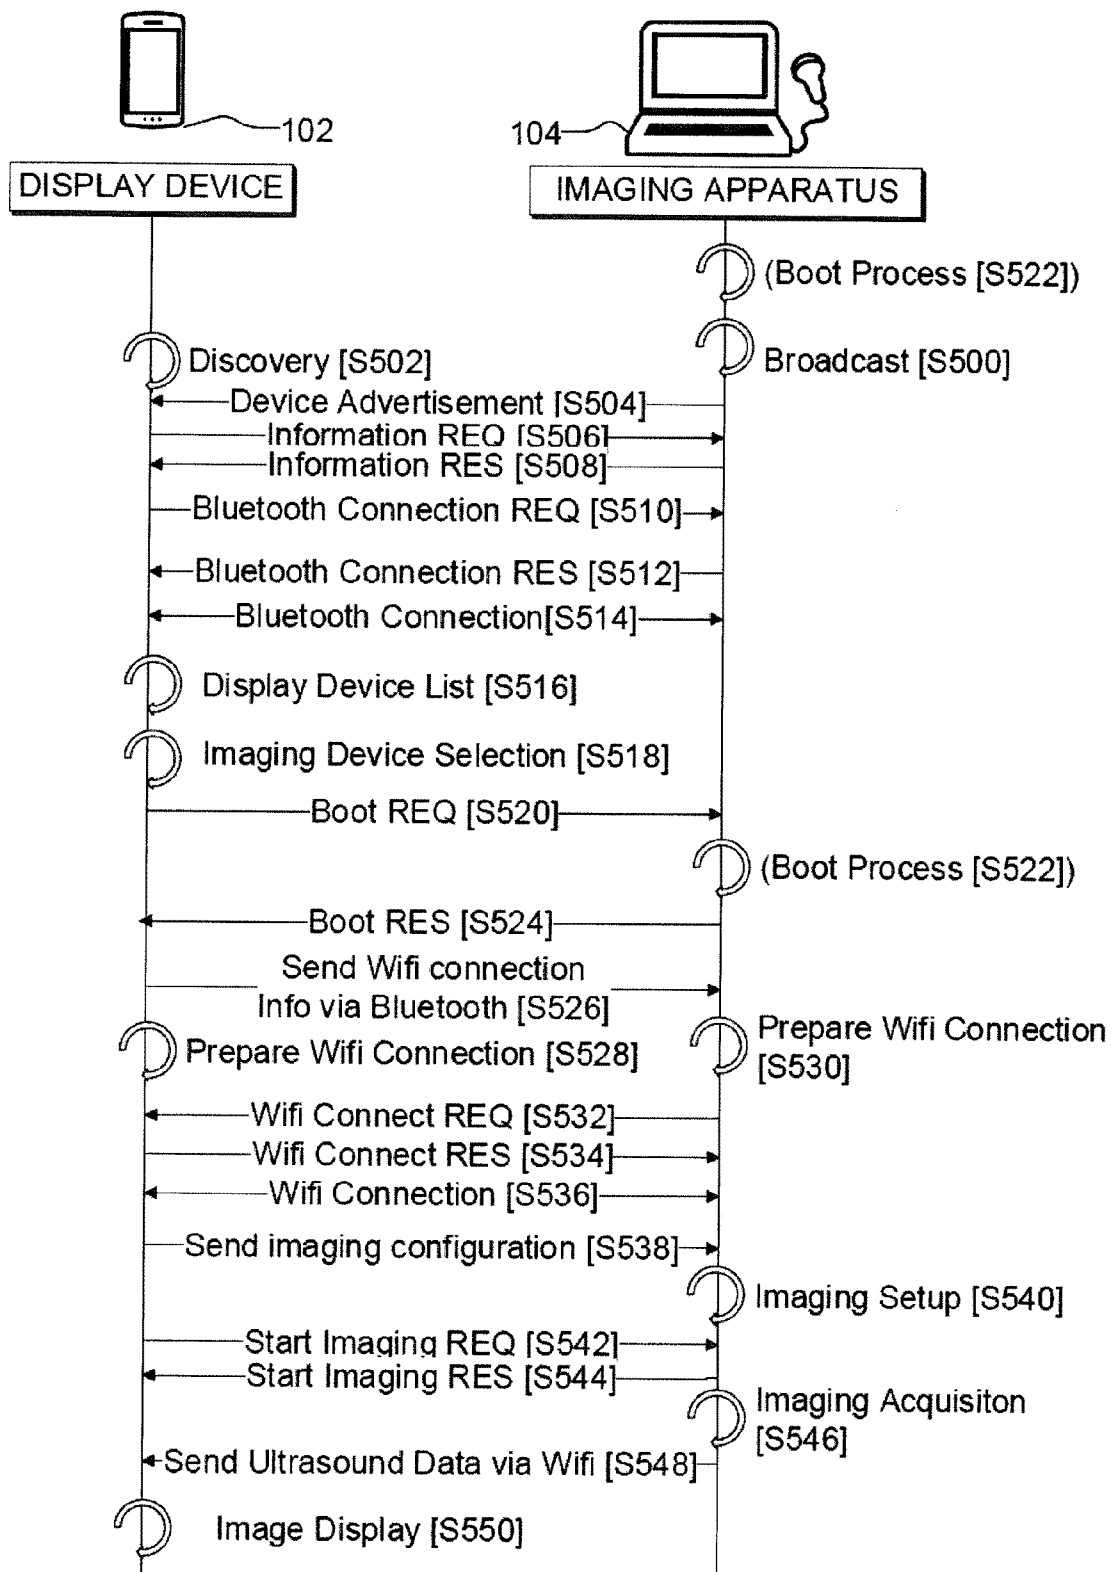


FIG. 5

5/8

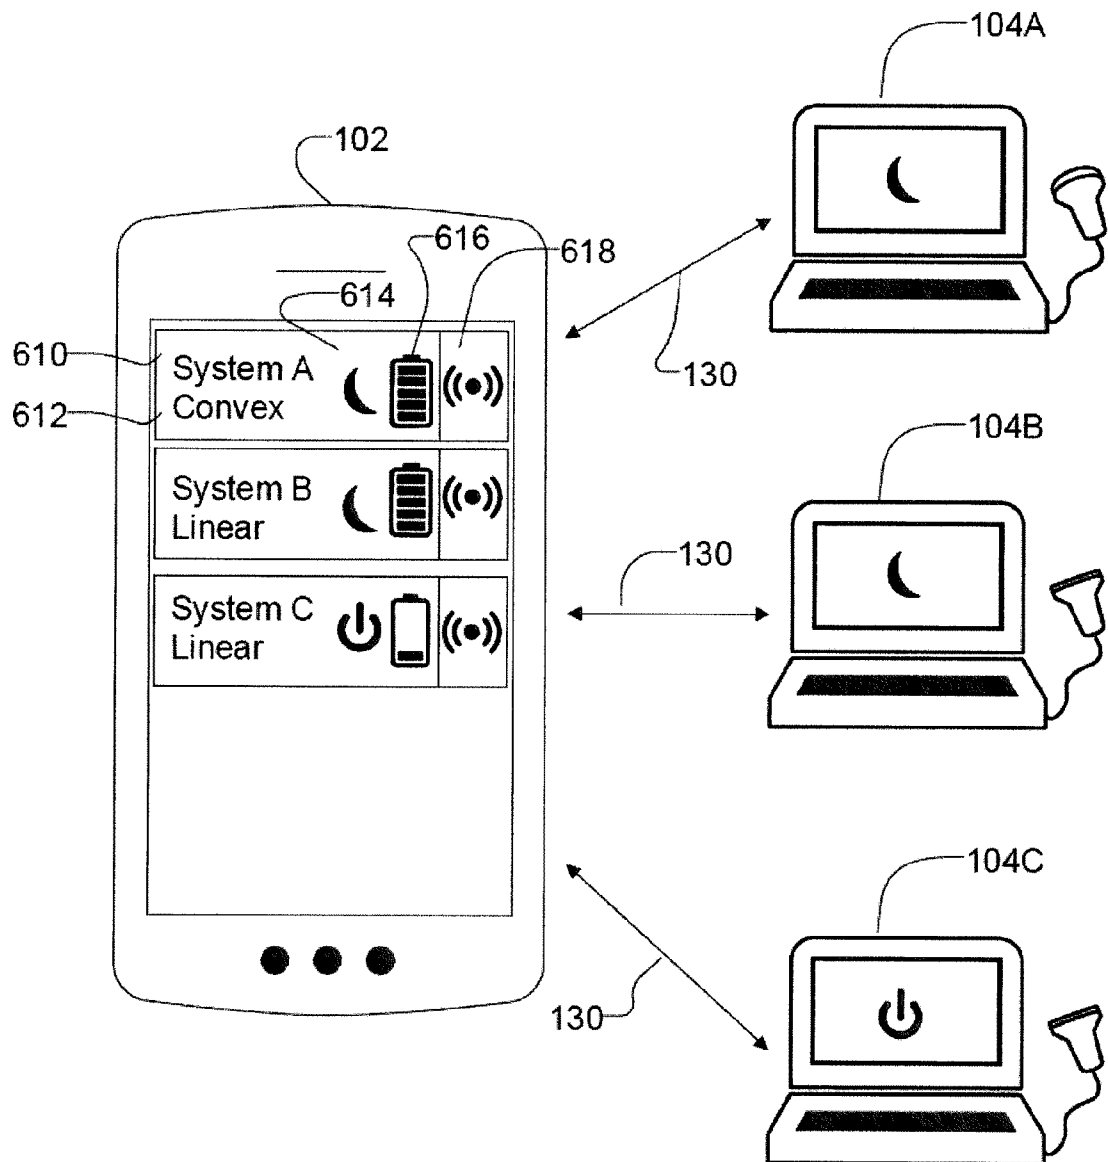


FIG. 6

6/8

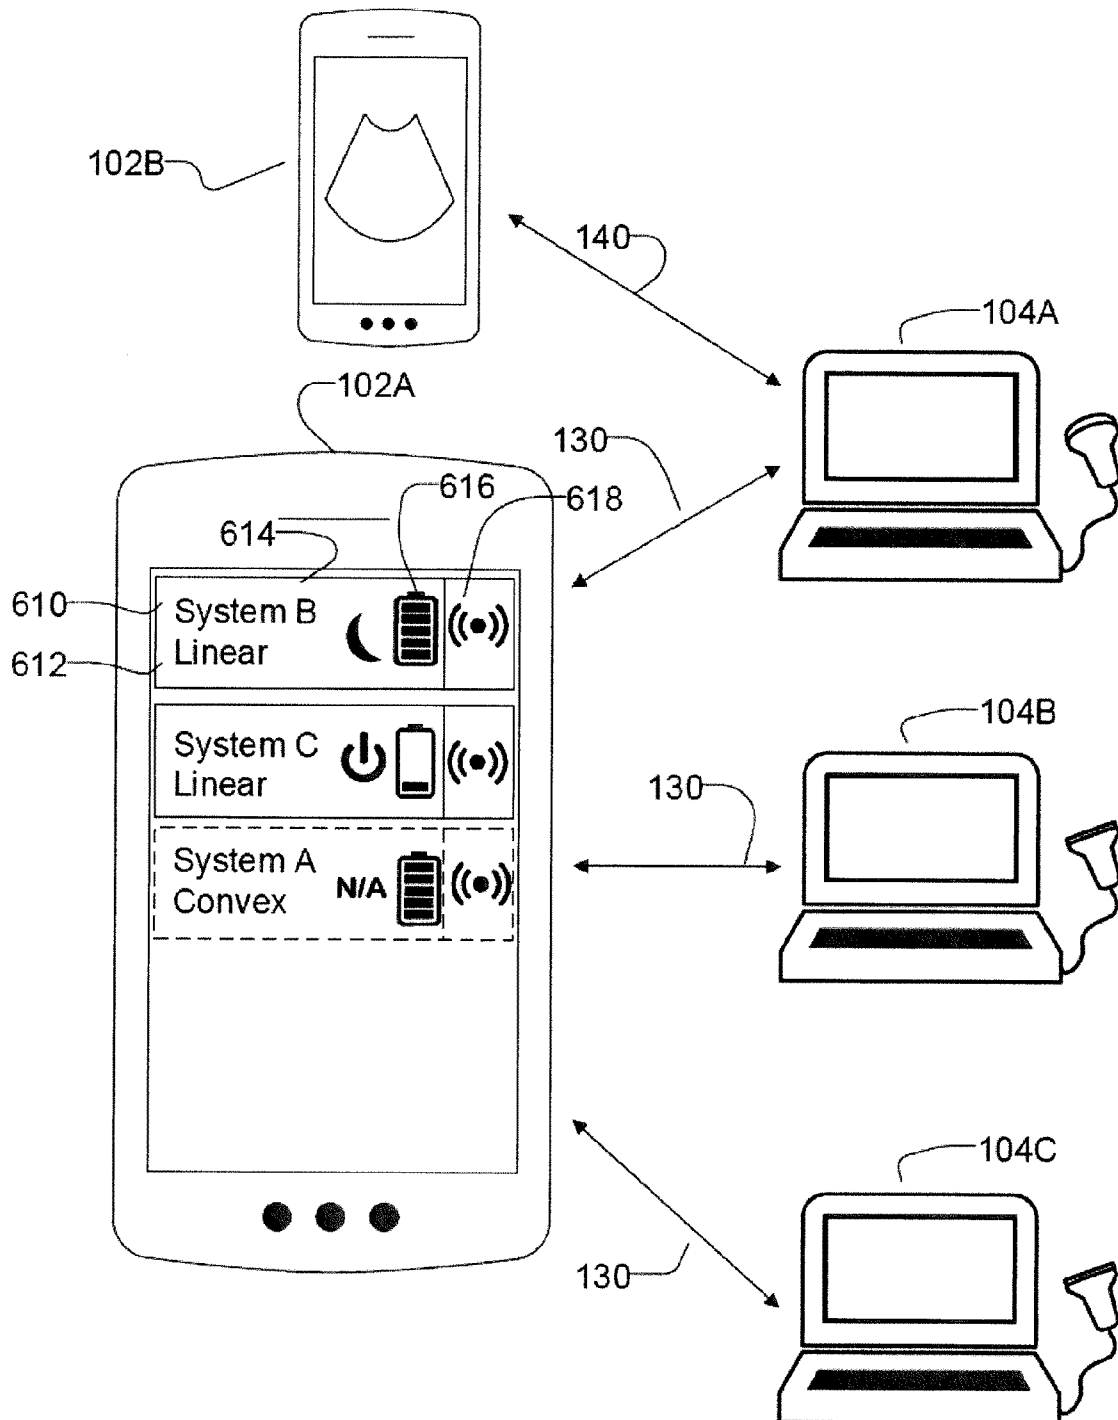


FIG. 7

7/8

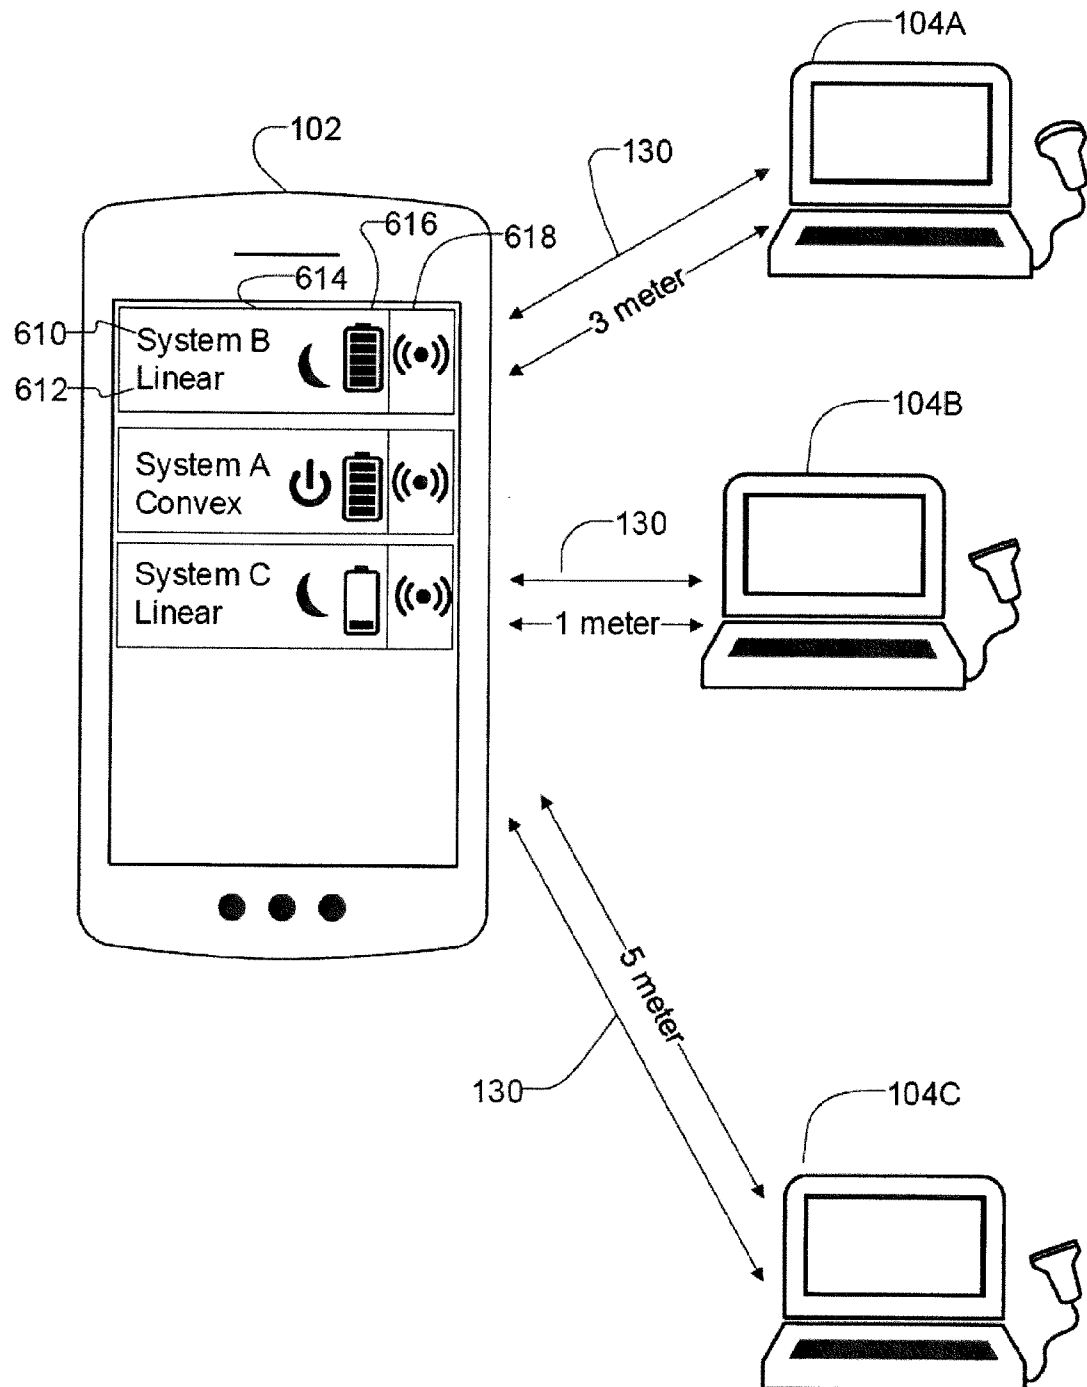


FIG. 8

8/8

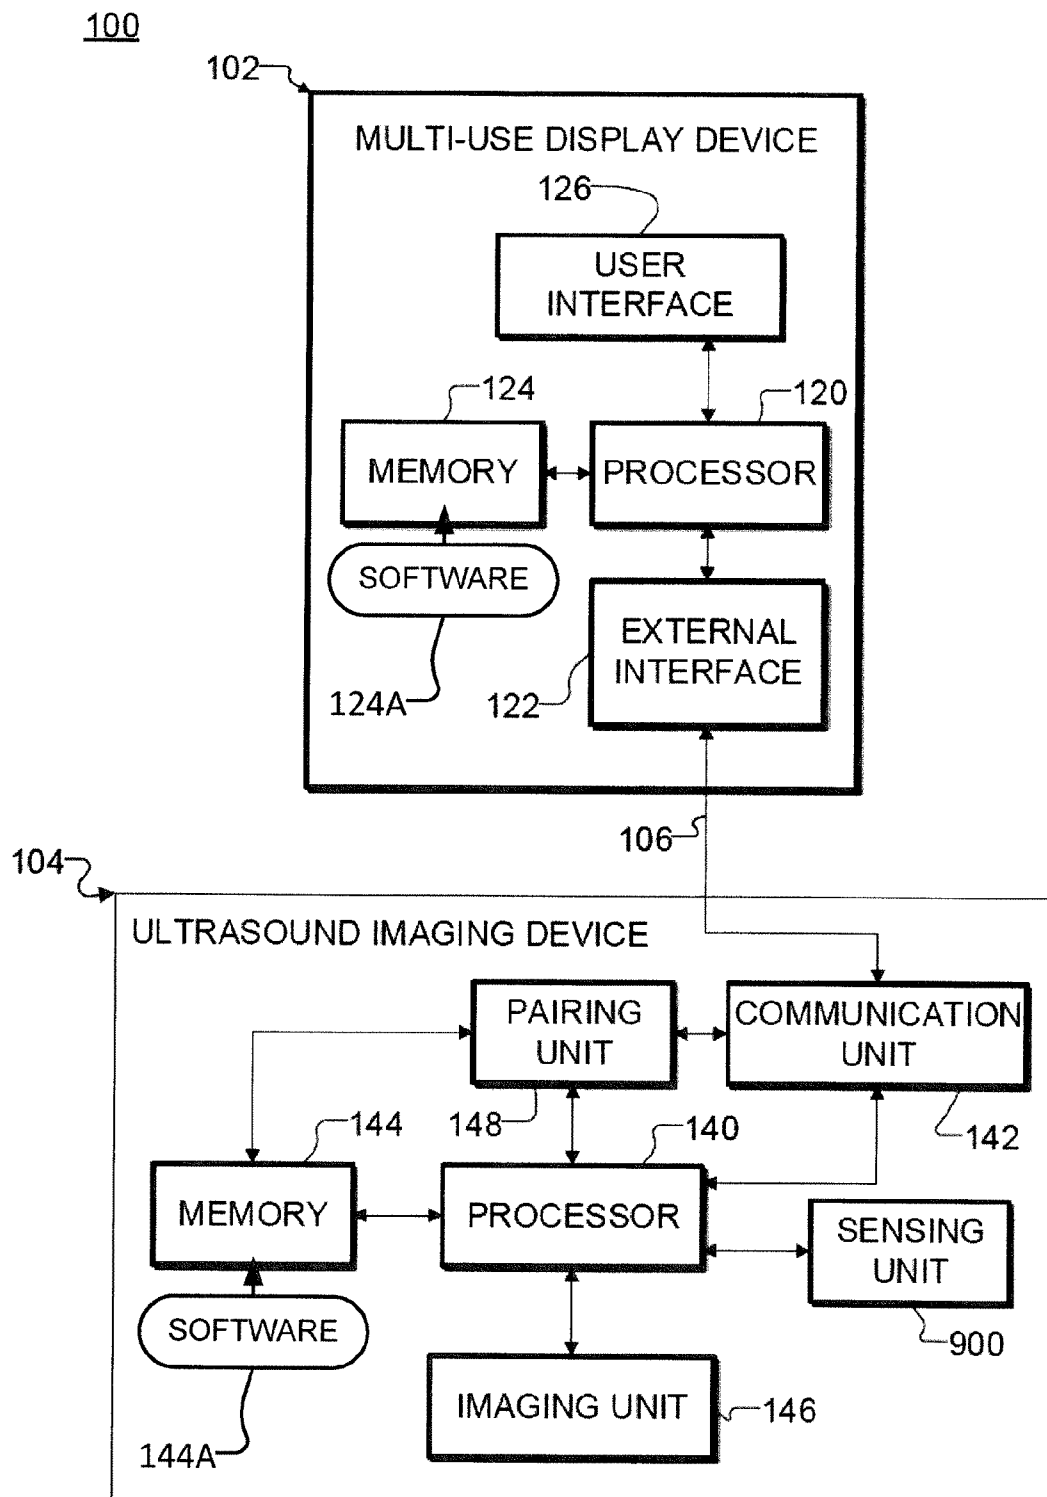


FIG. 9

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/050343

A. CLASSIFICATION OF SUBJECT MATTER

IPC: **H04W 80/12** (2009.01), **A61B 8/13** (2006.01), **G01S 15/89** (2006.01), **H04W 12/06** (2009.01), **H04W 80/00** (2009.01)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
keywords used across the whole IPC

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used)
Databases: Questel Orbit, Canadian Patent Database, CIPO Library Discovery Tool, Google, Google Patent, Google Scholar, IEEE Xplore
ACM Digital Library
Search terms: ultrasound imaging mobile bluetooth wi-fi wifi power battery proximity establish* session connect* link

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	(AGARWAL et al.) "Dynamic power management using on demand paging for networked embedded systems", Proceedings of the ASP-DAC 2005, Asia and South Pacific Design Automation Conference, 2005, Volume: 2, Pages: 755 – 759, 18-21 January 2005 (18-01-2005) [retrieved on 15 July 2016 (15-07-2016) Retrieved from: http://ieeexplore.ieee.org/stamp/stamp.jsp?tp=&arnumber=1466450 , also available at http://synergy.cs.cmu.edu/files/Agarwal_ASPDAC05_OnDemandPaging.pdf] *entire document*	1-78
A	US20120213136 A1 (WOO et al.) 23 August 2012 (23-08-2012) *entire document*	1-78
A	US20120214417 A1 (WOO et al.) 23 August 2012 (23-08-2012) *entire document*	1-78

☒ Further documents are listed in the continuation of Box C.

☒ See patent family annex.

* "A" "E" "L" "O" "P"	Special categories of cited documents: document defining the general state of the art which is not considered to be of particular relevance earlier application or patent but published on or after the international filing date document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) document referring to an oral disclosure, use, exhibition or other means document published prior to the international filing date but later than the priority date claimed	"T" "X" "Y" "&"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art document member of the same patent family
--------------------------------------	--	--------------------------	--

Date of the actual completion of the international search
15 July 2016 (15-07-2016)

Date of mailing of the international search report
18 July 2016 (18-07-2016)

Name and mailing address of the ISA/CA
Canadian Intellectual Property Office
Place du Portage I, C114 - 1st Floor, Box PCT
50 Victoria Street
Gatineau, Quebec K1A 0C9
Facsimile No.: 819-953-2476

Authorized officer

Tatjana Kremer (819) 639-8189

INTERNATIONAL SEARCH REPORT

International application No.

PCT/CA2016/050343

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US6780154 B2 (HUNT et al.) 24 August 2004 (24-08-2004) *entire document*	1-78
A	US20050124890 A1 (HALMANN et al.) 9 June 2005 (09-06-2005) *entire document*	1-78

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/CA2016/050343

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
US2012213136A1	23 August 2012 (23-08-2012)	US2012213136A1	23 August 2012 (23-08-2012)
		US8918148B2	23 December 2014 (23-12-2014)
		CN102651785A	29 August 2012 (29-08-2012)
		CN102651785B	04 February 2015 (04-02-2015)
		CN102882241A	16 January 2013 (16-01-2013)
		CN102882241B	07 January 2015 (07-01-2015)
		EP2492776A2	29 August 2012 (29-08-2012)
		EP2493051A2	29 August 2012 (29-08-2012)
		KR20120096858A	31 August 2012 (31-08-2012)
		KR20120096864A	31 August 2012 (31-08-2012)
		KR20120096865A	31 August 2012 (31-08-2012)
		KR20120096866A	31 August 2012 (31-08-2012)
		US2012214418A1	23 August 2012 (23-08-2012)
		US8743856B2	03 June 2014 (03-06-2014)
		US2012213134A1	23 August 2012 (23-08-2012)
		US8824346B2	02 September 2014 (02-09-2014)
		US2012214417A1	23 August 2012 (23-08-2012)
		US8830889B2	09 September 2014 (09-09-2014)
		US2012213135A1	23 August 2012 (23-08-2012)
		US9059597B2	16 June 2015 (16-06-2015)
US2012214417A1	23 August 2012 (23-08-2012)	US2012214417A1	23 August 2012 (23-08-2012)
		US8830889B2	09 September 2014 (09-09-2014)
		CN102651785A	29 August 2012 (29-08-2012)
		CN102651785B	04 February 2015 (04-02-2015)
		CN102882241A	16 January 2013 (16-01-2013)
		CN102882241B	07 January 2015 (07-01-2015)
		EP2492776A2	29 August 2012 (29-08-2012)
		EP2493051A2	29 August 2012 (29-08-2012)
		KR20120096858A	31 August 2012 (31-08-2012)
		KR20120096864A	31 August 2012 (31-08-2012)
		KR20120096865A	31 August 2012 (31-08-2012)
		KR20120096866A	31 August 2012 (31-08-2012)
		US2012214418A1	23 August 2012 (23-08-2012)
		US8743856B2	03 June 2014 (03-06-2014)
		US2012213134A1	23 August 2012 (23-08-2012)
		US8824346B2	02 September 2014 (02-09-2014)
		US2012213136A1	23 August 2012 (23-08-2012)
		US8918148B2	23 December 2014 (23-12-2014)
		US2012213135A1	23 August 2012 (23-08-2012)
		US9059597B2	16 June 2015 (16-06-2015)
US6780154B2	24 August 2004 (24-08-2004)	US2003139664A1	24 July 2003 (24-07-2003)
		US2003139671A1	24 July 2003 (24-07-2003)
		US7371218B2	13 May 2008 (13-05-2008)
US2005124890A1	09 June 2005 (09-06-2005)	US2005124890A1	09 June 2005 (09-06-2005)
		US8535227B2	17 September 2013 (17-09-2013)
		DE10254191A1	18 June 2003 (18-06-2003)
		JP2003190159A	08 July 2003 (08-07-2003)
		US2003097071A1	22 May 2003 (22-05-2003)
		US7115093B2	03 October 2006 (03-10-2006)
		US2014024942A1	23 January 2014 (23-01-2014)
		US2014243669A1	28 August 2014 (28-08-2014)

专利名称(译)	用于从电子设备连接和控制无线超声成像系统的系统和方法		
公开(公告)号	EP3275279A4	公开(公告)日	2018-12-19
申请号	EP2016771129	申请日	2016-03-23
[标]申请(专利权)人(译)	CLARIUS移动医疗		
申请(专利权)人(译)	Clarius移动健康公司		
[标]发明人	PELISSIER LAURENT DICKIE KRIS HANSEN TREVOR		
发明人	PELISSIER, LAURENT DICKIE, KRIS HANSEN, TREVOR		
IPC分类号	H04W80/12 A61B8/13 G01S15/89 H04W12/06		
CPC分类号	A61B8/465 A61B8/0841 A61B8/4245 A61B8/4411 A61B8/4427 A61B8/4438 A61B8/4472 A61B8/4477 A61B8/461 A61B8/488 A61B8/54 A61B8/56 A61B8/565 G01S7/52082 G01S7/52096 G06F19/321 G16H30/20 G16H40/20 G16H40/63 G16H40/67 G16H50/20		
优先权	14/671773 2015-03-27 US		
其他公开文献	EP3275279A1		
外部链接	Espacenet		

摘要(译)

一种超声成像系统，包括多用途电子显示设备和超声成像设备。多用途电子显示设备能够与一个或多个超声成像设备通信，并基于先前存储信息，用户输入和从超声成像设备收集的信息中的至少一个来选择连接哪个。多用途电子显示设备可以在超声成像设备处于低功率待机状态时与超声成像设备通信。该方法降低了配对过程的复杂性，并提供了在多个超声成像设备之间快速且容易地进行选择的手段。