



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
27.01.2016 Bulletin 2016/04

(51) Int Cl.:
A61B 8/00 (2006.01)

(21) Application number: **15153428.6**

(22) Date of filing: **02.02.2015**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(72) Inventors:
• **Jin, Gil Ju**
Seoul (KR)
• **Ahn, Mi Jeoung**
Seoul (KR)
• **Byun, Mi Ae**
Gyeonggi-do (KR)

(30) Priority: **24.07.2014 KR 20140094214**

(71) Applicant: **Samsung Medison Co., Ltd.**
Gangwon-do 250-870 (KR)


(74) Representative: **Frey, Sven Holger**
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft mbB
Alte Ulmer Strasse 2
89522 Heidenheim (DE)

(54) **Ultrasound imaging apparatus and controlling method thereof**

(57) Disclosed herein is an ultrasound imaging apparatus and a controlling method thereof, the ultrasound imaging apparatus includes a receiving unit receiving an imaging signal of an object, a display unit displaying a diagnostic imaging on a first section based on the imaging

signal and displaying an image indicator indicating a target part of the object on a second section, and a controlling unit synchronizing the diagnostic imaging with a reference image corresponding to the diagnostic imaging.

FIG. 3

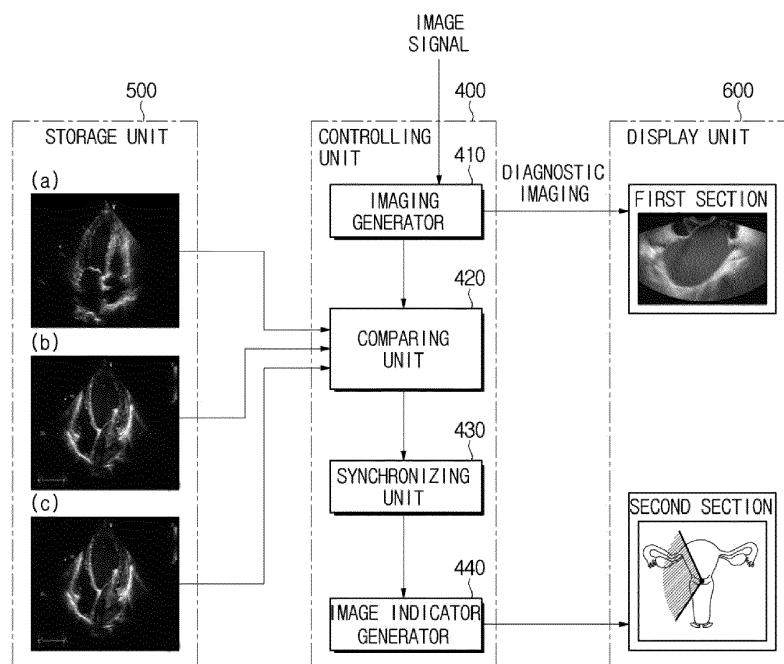

Description

BACKGROUND

1. Field

[0001] Embodiments of the present disclosure relate to an ultrasound imaging apparatus for processing an ultrasonic image and a controlling method thereof.

2. Description of Related Art.

[0002] An ultrasound imaging apparatus irradiates ultrasounds to a target part in an object through the surface of the object, detects echo ultrasounds reflected from the object and then noninvasively provides images about an examined part, such as a tomogram of a soft tissue or bloodstream.

[0003] The ultrasound imaging apparatus is compact, inexpensive, and displaying a diagnostic imaging immediately as compared with another type of diagnostic imaging apparatus, e.g., X-ray device, Computerized Tomography (CT) scanner, Magnetic Resonance Image (MRI), diagnostic nuclear medical apparatus. In addition, the ultrasound imaging apparatus is safe because there is not risk of radiation exposure. Therefore, the ultrasound imaging apparatus is widely used in medical examination at maternity, cardiology, abdomen, urology clinics.

[0004] In general, a diagnostic imaging generated by an ultrasound imaging apparatus displays a portion of an object, thus it is difficult for an operator to recognize intuitively a target part of the object or a ultrasound probe direction toward an examined position. Together with the diagnostic imaging, an image indicator indicating a target part of the object may be displayed, wherein the image indicator may be letters or icons similar with a shape of the object.

SUMMARY

[0005] Therefore, it is an aspect of the present disclosure to provide an ultrasound imaging apparatus capable of displaying a diagnostic imaging together with an image indicator indicating a target part by synchronizing the diagnostic imaging of the ultrasound imaging apparatus with a reference imaging, and a method of controlling the same.

[0006] Additional aspects of the present disclosure will be set forth in part in the description which follows and, in part, will be obvious from the description, or may be learned by practice of the invention.

[0007] In accordance with one aspect of the present disclosure, an ultrasound imaging apparatus includes a receiving unit receiving an imaging signal of an object, a display unit displaying a diagnostic imaging on a first section based on the imaging signal and displaying an image indicator indicating a target part of the object on a second

section, and a controlling unit synchronizing the diagnostic imaging with a reference image corresponding to the diagnostic imaging.

[0008] The display unit may display at least one reference images similar to the diagnostic imaging on a third section, the ultrasound imaging apparatus may further include an input unit receiving a selection of one reference image among the at least one reference images from users, and the control unit may synchronize the diagnostic imaging with the selected reference image.

[0009] The image indicator may include a target organ marker of the object.

[0010] The image indicator may include a beam direction marker indicating a direction of an ultrasound probe beam.

[0011] The image indicator may include a beam direction marker in two dimensions or in three dimensions according to types of image signals.

[0012] The image indicator may further include a body axis marker indicating an anatomical location of the object.

[0013] The ultrasound imaging apparatus may further include an input unit receiving user requests including a selection of a target part and a diagnostic location from users, and the display unit may further display a different target organ marker the second section according to the selection of the target part and the diagnostic location.

[0014] The reference image may include a cross-sectional image according to a diagnostic mode of a three dimensional volume image.

[0015] The ultrasound imaging apparatus may further include a storage unit storing the reference images according to target parts and diagnostic locations of an object, and an input unit receiving a selection of the target part and the diagnostic location from the user.

[0016] The control unit may set the image indicator as at least one of a reference position and a reference location when the diagnostic imaging is synchronized with the reference image.

[0017] The receiving unit may receive signals of a relative position and a relative location of the ultrasound probe based on the reference position and the reference location, and the control unit may move the image indicator according to the relative position and the relative location.

[0018] The receiving unit may receive a first image signal and a second image signal of the object, the display unit may display a first diagnostic imaging based on the first image signal and a second diagnostic imaging based on the second image signal on the first section, and the control unit may move the image indicator according to a relative position and a relative location of the second diagnostic imaging based on the first diagnostic imaging.

[0019] The display unit may display the target part on the second section by moving the target organ marker.

[0020] The ultrasound imaging apparatus may further include an ultrasound probe transmitting an ultrasound to the object, receiving an echo ultrasound reflected from

the object, and transforming the echo ultrasound to an electrical signal, and the display unit may display a target part of the object on a first section based on the electrical signal.

[0021] The ultrasound probe may include a detecting unit, wherein the detecting unit may detect a relative position and a relative location of the ultrasound probe based on a reference position and a reference location, and the controlling unit may move the image indicator according to the relative position and the relative location.

[0022] The detecting unit may include at least one of an angular velocity sensor, a magnetic sensor, an acceleration sensor, a gravity sensor, and a gyro sensor.

[0023] The ultrasound imaging apparatus may further include a storage unit storing at least one reference image.

[0024] The ultrasound imaging apparatus may further include an input unit receiving a change signal for changing the reference image from users, and the controlling unit may synchronize the changed reference image based on the change signal.

[0025] In accordance with another aspect of the present disclosure, a controlling method of an ultrasound imaging apparatus includes receiving an image signal of an object, displaying a diagnostic imaging on a first section based on the image signal, synchronizing the diagnostic imaging with a reference image corresponding to the diagnostic imaging, and displaying an image indicator indicating a target part of the object on a second section.

[0026] The method may further include displaying at least one reference images similar to the diagnostic imaging on a third section before the synchronizing, and receiving a selection of one reference image among the at least one reference images from the user, wherein the synchronizing is that the selected reference image by the user is synchronized with the diagnostic imaging.

[0027] The reference image may include a cross-sectional image according to a diagnostic mode of a three dimensional volume image.

BRIEF DESCRIPTION OF THE DRAWINGS

[0028] These and/or other aspects of the disclosure will become apparent and more readily appreciated from the following description of embodiments, taken in conjunction with the accompanying drawings of which:

FIG. 1 is a perspective view illustrating an ultrasound imaging apparatus according to an embodiment of the present disclosure;

FIG. 2 is a control block diagram illustrating the ultrasound imaging apparatus according to an embodiment of the present disclosure;

FIGS. 3 and 4 are views illustrating a control operation by a controlling unit;

FIGS. 5 (a) and (b) are views illustrating a reference image stored in a storage unit according to an embodiment of the present disclosure;

FIGS. 6 and 7 (a) and (b) are views illustrating an image indicator displayed on a second section of a display unit;

FIGS. 8 (a) to (d) and 9 (a) to (d) are views illustrating a diagnostic imaging and an image according to changing a location and a position of an ultrasound probe; and

FIG. 10 is a flow chart illustrating a control method of an ultrasound imaging apparatus according to another embodiment of the present disclosure.

DETAILED DESCRIPTION

[0029] The present disclosure will now be described more fully with reference to the accompanying drawings, in which exemplary embodiments of the disclosure are shown. The disclosure may, however, be embodied in many different forms and should not be construed as being limited to the embodiments set forth herein; rather, these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey the concept of the disclosure to those skilled in the art. Like reference numerals in the drawings denote like elements, and thus their description will be omitted. In the description of the present disclosure, if it is determined that a detailed description of commonly-used technologies or structures related to the embodiments of the present disclosure may unnecessarily obscure the subject matter of the invention, the detailed description will be omitted. It will be understood that, although the terms first, second, third, etc., may be used herein to describe various elements, components, regions, layers and/or sections, these elements, components, regions, layers and/or sections should not be limited by these terms. These terms are only used to distinguish one element, component, region, layer or section from another region, layer or section.

[0030] Embodiments of the present disclosure will now be described with reference to accompanying drawings.

[0031] FIG. 1 is a perspective view illustrating an ultrasound imaging apparatus according to an embodiment of the present disclosure.

[0032] As illustrated in FIG. 1, an ultrasound imaging apparatus 100 may include an ultrasound probe 200, a main body 300, a display unit 600 and an input unit 700.

[0033] The ultrasound probe 200 is connected to an end of a cable and the other end of the cable may be connected to a male connector (not shown). The male connector may be physically coupled with a female connector (not shown) of the main unit 300.

[0034] The ultrasound probe 200 may include at least one transducer T, and use them to transmit ultrasound

signals to an object and receive echo ultrasounds reflected from the object. The at least one transducer T may form at least one row at one end of the ultrasound probe 200, as shown in FIG. 1.

[0035] The object may be a living body of a human or animal, an organ in the living body, such as blood vessels, bones, muscles, etc., but is not limited thereto. Therefore, anything whose internal structure may be imaged by the ultrasound imaging apparatus 100 may be the object.

[0036] Three directions perpendicular to one and another based on a center of the transducer may be defined as an axis direction (A), a lateral direction (L), and an elevation direction (E). Particularly, a direction in which an ultrasound is radiated may be defined as the axis direction (A), a direction in which transducers are formed in a row may be defined as the lateral direction (L), and a direction perpendicular to the axis direction and the lateral direction may be defined as the elevation direction (E).

[0037] The main body 300 may include a main component of the ultrasound imaging apparatus 100, such as a transmit signal generator (not shown). When an examiner inputs an ultrasound diagnosis command, the transmit signal generator (not shown) may generate a transmit signal and transmit the transmit signal to the ultrasound probe 200.

[0038] The main body 300 may include at least one female connectors (not shown), which are physically coupling to male connectors (not shown) connected to cables so that the main body 300 and the ultrasound probe 200 may communicate signals. For example, a transmit signal generated by the transmit signal generator may be sent to the ultrasound probe 200 through the male connector connected to the female connector of the main body 300 and the cable.

[0039] In addition, a plurality of casters configured to fix or move the ultrasound imaging apparatus 100 to a certain place may be mounted on a lower portion of the main body 300.

[0040] The input unit 700 may receive commands related to an operation of the ultrasound imaging apparatus 100 from users. For example, the user may input a command to start ultrasonic examination, select a target part, select a diagnostic position, select a mode for an output ultrasonic image, select a reference imaging, etc., through the input unit 700. The command may be performed by selecting one of user interfaces displayed on the display unit 600.

[0041] The input unit 700 may receive changing geometry information from the user, wherein the changing geometry information may be changing zoom, inversing, reversing, rotating, or changing focus of an ultrasound image. To match a reference image with a diagnostic imaging, the reference image displayed on a third section of the display unit 600, which is described later, may be changed zoom thereof, inversed, reversed, rotated or changed focus thereof according to the changing geometry information input by the user.

[0042] The target part may be referred to as a part of an object related to image signals currently receiving, and may include all organs, e.g., a heart, a brain, a breast, which are examined by the ultrasound imaging apparatus. By inputting a part to be examined in advance, the user may easily obtain information related to a diagnostic imaging such as a reference image corresponding to the diagnostic imaging.

[0043] The diagnostic position may be information about the target part of the object is examined from where, which is input by the user through the input unit 700. For example, through the input unit 700, the user may input whether a heart is examined from an esophagus or from ribs. Particularly, when examining a brain, a diagnostic position may be Mid-Sagittal plane, Trans-ventricular plane, Trans-thalamic plane, and Trans-cerebellar plane, and when examining a heart, a diagnostic position may be Four-chamber view, Five chamber view, three vessel view (3VT), Right ventricular outflow tract (RVOT), Left ventricular outflow tract, (LVOT), Bicaaval View, Aortic Arch, Ductal Arch, Short Axis View, and Long Axis view.

[0044] Modes for an ultrasound imaging may include an Amplitude mode (A-mode), a Brightness mode (B-mode), a Doppler mode (D-mode), an Elastography mode (E-mode), a Motion mode (M-mode), etc.,.

[0045] A reference image may be a reference for a target part of an object and a diagnostic position, and the user may guess where are the target part and the diagnostic position on the basis of the reference image. The reference image may be a cross-sectional view of a three dimensional volume image of the target part, which is described later with reference with FIG. 5. At least one reference images may be provided to the user through the display unit 600, and the user may select one reference image through the input unit 700. The selected reference image may be synchronized with the diagnostic imaging.

[0046] Commands input through the input unit 700 may be transmitted to the main body 300 through wired/wireless communication.

[0047] The 'user' as used herein may be a medical person who performs diagnosis with the ultrasound imaging apparatus 100, including a doctor, a radiographer, a nurse, etc., but is not limited thereto and thus may be anyone who uses the ultrasound imaging apparatus 100.

[0048] The input unit 700 may include at least one of a keyboard, mouse, trackball, touch screen, foot switch, and foot pedal, but is not limited thereto.

[0049] The input unit 700 may be provided on an upper portion of the main body 300 as shown in FIG. 1, or may be provided on a lower portion of the main body 300 when the input unit 700 is implemented with a foot switch or a foot pedal.

[0050] If the input unit 700 is implemented in a Graphical User Interface (GUI), i.e., in software like a touch screen, the input unit 700 may be displayed on the display unit 600, which will be described later.

[0051] At least one ultrasound probe holders may be provided on around the input unit 700 to hold the ultrasound probe 200. Therefore, the user may keep the ultrasound probe 200 in the ultrasound probe holder while the ultrasound imaging apparatus 100 is not used.

[0052] The display unit 600 displays an image obtained in an ultrasonic diagnostic process. The display unit 600 displays the image according to a mode selected by the user. If no mode is selected, the image may be displayed in a default mode set by the user in advance, e.g., B mode.

[0053] Particularly, the display unit 600 may display a diagnostic imaging on a first section, and display an image indicator showing a target part of the object on a second section. The display unit 600 may display at least one reference images similar to the diagnostic imaging on a third section.

[0054] The first section may be a section for displaying the diagnostic imaging of the object being diagnosed currently, and other images may be displayed according to ultrasound imaging modes, the type of ultrasound probe. The diagnostic imaging may include a three-dimensional (3D) image.

[0055] The second section may be a section for displaying an image indicator for indicating the target part. For example, an organ imaging virtually formed and a beam direction marker showing a direction of an ultrasound probe beam may be displayed. A target part may be directly displayed to the user, which is will be described later with reference with FIGS. 6 and 7.

[0056] The third section may be a section for displaying at least one reference imaging, which is determined to be similar to the diagnostic imaging. The user may select a single reference imaging among the displayed reference imaging through the input unit 700.

[0057] The user may input a change signal for a reference imaging through the input unit 700. The change signal for a reference imaging may allow a control unit 400 to change a reference imaging determined to be most similar to the diagnostic imaging or a reference imaging selected by the user to another reference imaging. Therefore, the control unit 400 may synchronize a changed reference imaging according to the signal for changing. The change signal may serve as a revise signal and input by the user even after the synchronization. The changed reference imaging may be the second most similar reference imaging next to the most similar reference imaging, or a reference imaging selected by the user.

[0058] The display unit 600 may be mounted by coupling to the main body 300. However, the display unit 600 may be separated from the main body 300. Although not illustrated in FIG. 1, a sub display for displaying an application (e.g., menus and guidance needed for ultrasonic diagnosis) related to operations of the ultrasound imaging apparatus 100 may be provided.

[0059] The display unit 600 may employ a Liquid Crystal Display (LCD), a Light Emitting Diodes (LED), an Organic Light Emitting Diodes (OLED), an Active Matrix Or-

ganic Light Emitting Diodes (AMOLED), a flexible display, a three dimensional 3D display (3D) and a touch screen having a display function and an input function.

[0060] FIG. 2 is a control block diagram illustrating the ultrasound imaging apparatus according to an embodiment of the present disclosure, and FIGS. 3 and 4 are views illustrating a control operation by a controlling unit.

[0061] Referring to FIG. 2, the ultrasound imaging apparatus 100 may image an inside or an outside of an object by the ultrasound probe 200, a beamformer 350, a controlling unit 400, a storage unit 500, the input unit 700, and the display unit 600.

[0062] The ultrasound probe 200 may include at least one transducer T to transmit ultrasounds to an object, receive echo ultrasounds reflected from the object, and perform transformation between electric signals and ultrasounds.

[0063] Particularly, when the ultrasound probe 200 is supplied with power from an external power supply or an internal electricity storage device, e.g., battery, the transducers generate ultrasounds while vibrating due to the applied current and irradiate the ultrasounds to an external object. Each transducer receives an echo ultrasound reflected and returned from the object, and generates a current while vibrating due to the echo ultrasound, the current having a frequency corresponding to the vibration frequency.

[0064] The transducer T may be a Magnetostrictive Ultrasound Transducer (MUT) that uses magnetostrictive effects of a magnetic substance, a Capacitive Micromachined Ultrasonic Transducer (cMUT) that uses vibration of hundreds or thousands of microfabricated thin films, or a Piezoelectric Ultrasonic Transducer (PUT) that uses piezoelectric effects of a piezoelectric substance.

[0065] The transducers T may be linear array, convex array, phased array, sector array transducers, etc., which may be arranged in a form of a row or a matrix. When the transducers T are arranged in a row, they may be swung in the elevation direction to obtain multiple ultrasonic images; and when they are arranged in a form of a matrix, multiple ultrasonic images may be obtained only with a single transmission of ultrasounds.

[0066] However, the transducers are not limited thereto, but may be implemented with any other types of transducers known to skilled people in the art.

[0067] Although not shown, the ultrasound probe 200 may further include a detecting unit (not shown), and the detecting unit may be disposed in the case of the ultrasound probe 200. The detecting unit may generate information about position and location of the ultrasound probe 200 by detecting a position and a location of the ultrasound probe 200. The detecting unit may employ an angular velocity sensor, a magnetic sensor, an acceleration sensor, a gravity sensor, and a gyro sensor, but is not limited thereto. That is, the detecting unit may employ any kind of sensor capable of detecting a second or a three dimensional position and location of the ultrasound probe 200.

[0068] The beamformer 350 may include a transmit beamformer 360 and a receive beamformer 370 to perform transformation between analog and digital signals and to adjust time differences of ultrasounds transmitted by or received from the at least one transducers T.

[0069] Ultrasounds adjusted time differences may be focused as a receive signal (S), and the focused receive signal (S) may be supplied to the controlling unit 400. As mentioned above, the signal supplied to the controlling unit 400 may be defined as an imaging signal.

[0070] The storage unit 500 may store reference images according to target parts and diagnostic location. Particularly, the storage unit 500 may store various reference images according to diagnostic locations based on one target part or may store various reference images according to target parts. In addition, the storage unit 500 may store image indicators set up according to each reference images.

[0071] FIG. 5 is a view illustrating a reference image stored in a storage unit according to an embodiment of the present disclosure.

[0072] A reference image may be a reference for a target part of an object and a diagnostic position, and the user may guess where are the target part and the diagnostic position on the basis of the reference image. When referring to FIG. 5a, the reference image stored in the storage unit 500 may be a cross-sectional view of the target part and the diagnostic position, and when referring to FIG. 5b, the reference image stored in the storage unit 500 may be a cross-sectional view of a three dimensional volume image of the target part and the diagnostic position, wherein the three dimensional volume image may correspond to the target part and the cross-sectional view may correspond to the diagnostic location. That is, the storage unit 500 may store a cross-sectional view, such as FIG. 5a, a three dimensional volume image and a cross-sectional view of a three dimensional volume image, such as FIG. 5b.

[0073] FIGS. 6 and 7 are views illustrating an image indicator displayed on a second section of a display unit.

[0074] As illustrated in FIG. 6, the image indicator may include a target organ marker, a body axis marker, and an ultrasound beam direction marker. The display unit 600 may virtually display a target part by these markers.

[0075] The target organ marker may display a target part of an object, such as a chest, a liver, an abdomen, an uterus, an anus, etc., and may be identical to a three dimensional volume image of a reference image. The body axis marker may display an anatomical location, such as Cranial (Cr), Caudal (Ca), Anterior (A), Posterior (P), Right (R) and Left (L), by using a three dimensional coordinate system. Hereinafter, the body axis marker may be displayed by using a three dimensional rectangular coordinate system, but is not limited thereto. The body axis marker may be displayed in various shapes. The ultrasound beam direction marker may display a direction of an ultrasound beam. The ultrasound beam direction marker may have a square shape in a leaner ul-

trasound probe, a fan shape having trapezoid shaped in a convex ultrasound probe or a vaginal ultrasound probe, a fan shape in a phased array ultrasound probe, and a three-dimensional shape of a cross-sectional beam of each ultrasound probe in a two-dimensional matrix ultrasound probe (2D Matrix ultrasound probe), and may display the transmission direction of the ultrasound beam. According to one embodiment, the ultrasound beam direction marker may be displayed with the body axis marker so that a vertex of a triangle in the ultrasound beam direction marker is to be located at an origin of a coordinate system of the body axis marker. In addition, when the ultrasound probe 200 is a one dimensional array ultrasound probe (1 D), the ultrasound beam direction marker may be displayed in two dimensions, and when the ultrasound probe 200 is a two dimensional array ultrasound probe or a three dimensional mechanical ultrasound probe, the ultrasound beam direction marker may be displayed in three dimensional volume.

[0076] The storage unit 500 may store reference images according to a target part and a diagnostic position in advance. A diagnostic imaging and the stored reference image may be subject to be compared by a comparing unit 430 of the control unit, which is described later.

[0077] The storage unit 500 may store the image indicator in association with the target part and the diagnostic location of the object. For example, the storage unit 500 may store the image indicator including a target organ marker, a body axis marker and an ultrasound beam direction marker, wherein the image indicator correspond to the target part and the diagnostic location of the object, as illustrated in FIG. 6. When the target organ marker and the ultrasound beam direction marker may be displayed in a two dimensional when using a two dimensional coordinate system, as illustrated in FIG. 7a. When the target organ marker and the body axis marker may be displayed in three dimensions when using a three dimensional coordinate system, as illustrated in FIG. 7b. The storage unit 500 may store reference images in association with image indicators.

[0078] The storage unit 500 may include a program part and a data part.

[0079] The program part may include Operating system (OS) booting programs to control overall operations of the ultrasound imaging apparatus 100. The program part may include programs related to the operation of the control unit 400. The data part may be a place where data generated according to the operation of the ultrasound imaging apparatus 100, such as the reference image and the image indicator, is stored.

[0080] The storage unit 500 may employ volatile memory, such as, cache memory, Read Only Memory (ROM), Programmable ROM (PROM), Erasable Programmable ROM (EPROM), Electrically Erasable Programmable ROM (EEPROM) and Flash memory, nonvolatile memory, such as, Random Access Memory (RAM), Hard Disk Drive (HDD), or CD-ROM, but is not limited thereto.

[0081] The control unit 400 may control overall opera-

tions of the ultrasound imaging apparatus 100. Particularly, the control unit 400 may generate control signals to control at least one of the transmit beamformer 360, the receive beamformer 370, the storage unit 500, and the display unit 600 to response commands input through the input unit 700. The control unit 400 may generate control signals to control compartments to response commands received from outside devices through wired/wireless communication.

[0082] Referring to FIGS. 3 and 4, the control unit 400 may include an imaging generator 410, a comparing unit 420, a synchronizing unit 430, and an image indicator generator 440.

[0083] The imaging generator 410 may generate a diagnostic imaging based on an electrical signal, hereinafter, an imaging signal, received from the beamformer 350, and may allow the display unit 600 to display the diagnostic imaging on the first section of the display unit 600. The generated diagnostic imaging may be an Amplitude mode (A-mode), a Brightness mode (B-mode), a Doppler mode (D-mode), an Elastography mode (E-mode), and a Motion mode (M-mode), but is not limited thereto. Hereinafter, an image in Brightness mode (B-mode) will be described as an example. The B-mode may be a diagnosis mode in which size of echo ultrasounds reflected from the object is converted to brightness and displayed. According to embodiments, diagnostic imaging may be displayed in various modes. In addition, the diagnostic imaging may be generated in two or three dimensional image. Particularly, the image generator 410 may generate diagnostic imaging based on focused ultrasound signal through the receive beamformer 370.

[0084] The comparing unit 420 may compare the generated diagnostic imaging with at least one reference image stored in the storage unit 500. Referring to FIG. 3, the comparing unit 420 may select a reference image which is the most similar with a diagnostic imaging after comparing a diagnostic imaging with at least one reference image (a, b, c) corresponding to a target part and a diagnostic location, both of which are input by the user. In addition, the comparing unit 420 may automatically select the most similar reference image, as illustrated in FIG. 3. However, the comparing unit 420 may allow the user to select the most similar image after displaying at least one reference image (a, c) determined to be the most similar image among the reference image (a, b, c) corresponding to the target part and the diagnostic location, as illustrated in FIG. 4.

[0085] The synchronizing unit 430 may synchronize the selected reference image with the diagnostic imaging, and may set a diagnostic area of the image indicator as a reference position and a reference location. The synchronizing may be defined as associating the selected reference image with the diagnostic imaging. Particularly, the synchronizing unit 430 may synchronize the selected reference image with the diagnostic imaging, and may set a position and a location of the ultrasound probe 200 at synchronizing point as a reference position

and reference location of the ultrasound probe 200. The set reference location may be a location to allow the center of gravity of the ultrasound probe 200 to be an original point of a coordinate system of the body axis marker, and the set reference position may be an angle according to an orientation of the ultrasound probe 200 detected by the detecting unit. The reference position and the reference location may be stored in the storage unit 500.

[0086] The image indicator generator 440 may generate an image indicator displayed on the second section based on the reference position and the reference location.

[0087] FIGS. 8 and 9 are views illustrating a diagnostic imaging and an image according to changing a location and a position of an ultrasound probe.

[0088] Particularly, referring to FIG. 8, when a diagnostic imaging, as illustrated in (a), may be set as a reference position and a reference location, the image indicator generator 440 may generate an image indicator, as illustrated in (c). When a position and location of the ultrasound probe 200 is changed, the diagnostic imaging may be displayed in the first section, as illustrated in (b) and the image indicator generator 440 may generate an image indicator, as illustrated in (d), according to a relative position and a relative location of the ultrasound probe 200 based on the reference position and the reference location. That is, an image indicator may be moved according to a relative position and a relative location based on the reference position and the reference location of the ultrasound probe 200.

[0089] The relative position and the relative location based on the reference position and the reference location of the ultrasound probe 200 may be detected by a sensor of the detecting unit of the ultrasound probe 200, and a relative position and a relative location estimated from a diagnostic imaging, as illustrated in FIG. 9.

[0090] The image indicator generator 440 may generate an image indicator in a way that the beam direction marker is displayed in the body marker coordinate system, as illustrated in FIG. 8, in a way that a direction of the target organ marker may be changed, as illustrated in (a, b) of FIG. 9, or in a way that a point of the beam direction marker is changed, as illustrated in (c, d) of FIG. 9, but is not limited thereto. The image indicator may be displayed in various ways capable of showing a position and location of an ultrasound probe.

[0091] The control unit 400 may include a processor, a ROM in which control programs are stored, and a RAM in which signals or data input from the outside are stored or which is used as a storage area to correspond to various operations

[0092] The control unit 400 may control overall operations of the ultrasound imaging apparatus 100 and a flow of signal between compartments disposed inside the ultrasound imaging apparatus 100, and may process data. The control unit 400 may control power supplied to the internal compartments.

[0093] When conditions input by the user or stored in

advance are met, the control unit 400 may perform Operation System (OS) and various applications. Operations of the control unit 400 may be performed by being programmed by the storage unit 500. The description about the storage unit 500 is mentioned above, so it is omitted.

[0094] The processor may be realized in a shape of System on Chip (SoC) including core and GPU. The processor may include a single core, a dual core, a triple core, a quad core and various multiple cores. The control unit 400 may include a graphic processing board which is a circuit board electrically connected includes a processor, and RAM or ROM. The process, a ROM, and RAM may be connected to each other through an internal bus. The control unit 400 may be referred as a compartment including a processor, a ROM, and a RAM. The control unit 400 may be referred as a compartment including a processor, a ROM, a RAM, and a processing board.

[0095] FIG. 10 is a flow chart illustrating a control method of an ultrasound imaging apparatus according to another embodiment of the present disclosure.

[0096] The ultrasound imaging apparatus 100 may irradiate ultrasounds to the object, detect reflected signals from the object, and then obtain imaging signals (S 1110).

[0097] The reflected signals may be ultrasound signals received from the transducer, and may be changed to electronic signals by the beamformer. The electrical signals may be input to the control unit as imaging signals and then may be displayed on the first section of the display unit as a diagnostic imaging (S1120).

[0098] The diagnostic imaging and a reference image may be synchronized (S1130), and during the synchronization, the diagnostic imaging may be compared with at least one reference images stored in the storage unit, and then the most similar reference image to the diagnostic imaging, which is identical to the diagnostic imaging, may be selected. In this case, the selection of the reference image may be performed by estimating by ultrasound imaging apparatuses, or by selecting a single reference image through the input unit by displaying at least one reference images on the display unit.

[0099] A reference image may be a reference for a target part of an object and a diagnostic position, and the user may guess where are the target part and the diagnostic position on the basis of the reference image. The reference image may be a cross-sectional view of a three dimensional volume image of the target part or may be stored to correspond to the target part and the diagnostic location of the object.

[0100] The synchronization may represent associating the selected reference image with the diagnostic imaging.

[0101] After the synchronization of the selected reference image and the diagnostic imaging, a position and location of the ultrasound probe at a time of the synchronization may be set as the reference position and location of the ultrasound probe. The set reference position may allow the center of gravity of the ultrasound probe to be an origin of the body axis marker coordinate system, the

reference position may be an angle according an orientation of the ultrasound probe detected by the detecting unit, and then the image indicator may be displayed on the second section of the display unit (S 1140). At this time, the ultrasound beam direction marker may be displayed together with the body axis marker to allow a start point of an ultrasound to be placed on the origin of the body axis marker coordinate system. The beam direction marker and the body axis marker, which is information to virtually display the diagnostic area in the second section, may be displayed together with the target organ marker displaying the target part of the object in two dimensions or three dimensions.

[0102] When the target part of the object is changed according to the movement of the ultrasound probe (S 1150), the diagnostic imaging displayed on the first section may be changed. Accordingly, the image indicator may be moved (S1160). In this case, the position and the location of the ultrasound probe may be determined based on a detected signal by the detecting unit provided in the ultrasound probe and may be determined based on the changed diagnostic imaging of the object. Particularly, when the position and the location of the ultrasound probe are detected by an angular velocity sensor, a magnetic sensor, an acceleration sensor, a gravity sensor, and a gyro sensor, all of which are provided in the ultrasound probe, the image indicator may be changed from the reference position and the relative location to a relative position and a relative location. In addition, as mentioned above, the reference image, which is the most similar to the changed diagnostic imaging, may be selected, and the ultrasound imaging apparatus may estimate the relative position and the relative location based on the relation between reference information about the reference image of the changed diagnostic imaging and a preset reference position and location, and accordingly the image indicator may be moved. According to one exemplary embodiment of the movement of the image indicator, a beam direction of the beam direction marker may be changed.

[0103] As is apparent from the above description, the ultrasound imaging apparatus and a control method thereof may provide an accurate position and direction of the ultrasound probe diagnosing the object to the user by using the image indicator.

[0104] Without requiring the user's judgment, a target part virtually displayed is synchronized with a reference image so that the convenience may be provided to the user.

[0105] By matching the target organ marker configured to display the target part of the object, the body axis marker configured to display the diagnostic position of the object, and the beam direction marker configure to display a direction of an ultrasound probe beam received from the ultrasound probe with the target part currently examined by the user, the user may intuitively and accurately recognize the position of the ultrasound probe.

[0106] According to embodiments of the present dis-

closure, some components provided in the ultrasound imaging apparatus 100 may be implemented as modules. Here, the term "module" may represent a software element or a hardware element, such as a Field Programmable Gate Array (FPGA) or an Application Specific Integrated Circuit (ASIC), and the module may perform a predetermined role. However, the module is not limited to software or hardware. Further, the module may be constructed to exist in an addressable storage module, or to play one or more processors.

[0107] The module may include elements (e.g., software elements, object-oriented software elements, class elements and task elements), processors, functions, properties, procedures, subroutines, segments of a program code, drivers, firmware, a microcode, a circuit, data, a database, data structures, tables, arrays, and variables. Herein, functions provided by components and modules may be provided by a smaller number of combined larger components and modules, or by a larger number of divided smaller components and modules. In addition, the components and modules may be realized to operate one or more CPUs in a device.

[0108] The ultrasound imaging apparatus 100 and the control method thereof may be implemented as a computer code on a computer readable recording medium. The computer readable recording medium may include various kinds of recording medium stored data decrypted by the computer system. For example, there may be a Read Only Memory (ROM), a Random Access Memory (RAM), a magnetic tape, a magnetic disk, a flash memory, and an optical data storage device. In addition, the medium may be distributed to computer systems over a network, in which computer-readable code may be stored and executed in a distributed manner.

[0109] Although a few embodiments of the present disclosure have been shown and described, it would be appreciated by those skilled in the art that changes may be made in these embodiments without departing from the principles and spirit of the disclosure, the scope of which is defined in the claims and their equivalents.

Claims

1. An ultrasound imaging apparatus comprising:

a receiving unit receiving an imaging signal of an object;
a display unit displaying a diagnostic imaging on a first section based on the imaging signal, and displaying an image indicator indicating a target part of the object on a second section; and
a controlling unit synchronizing the diagnostic imaging with a reference image corresponding to the diagnostic imaging.

2. The ultrasound imaging apparatus of claim 1, wherein

the display unit displays at least one reference images similar to the diagnostic imaging on a third section, the ultrasound imaging apparatus further comprises an input unit receiving a selection of one reference image among the at least one reference images from users, and the control unit synchronizes the diagnostic imaging with the selected reference image.

3. The ultrasound imaging apparatus of claim 1, wherein the image indicator comprises a target organ marker of the object.

4. The ultrasound imaging apparatus of claim 1, wherein the image indicator comprises a beam direction marker indicating a direction of a ultrasound probe beam.

5. The ultrasound imaging apparatus of claim 1, wherein the image indicator comprises a beam direction marker in two dimensions or in three dimensions according to types of image signals.

6. The ultrasound imaging apparatus of claim 1, wherein the image indicator further comprises a body axis marker indicating an anatomical location of the object.

7. The ultrasound imaging apparatus of claim 1, further comprising:

an input unit receiving user requests including a selection of a target part and a diagnostic location from users, wherein the display unit further displays a different target organ marker on the second section according to the selection of the target part and the diagnostic location.

8. The ultrasound imaging apparatus of claim 1, wherein the reference image comprises a cross-sectional image according to a diagnostic mode of a three dimensional volume image.

9. The ultrasound imaging apparatus of claim 1, further comprising:

a storage unit storing the reference images according to target parts and diagnostic locations of an object, and an input unit receiving a selection of the target part and the diagnostic location from the user.

10. The ultrasound imaging apparatus of claim 1, where-

in
the control unit sets the image indicator as at least one of a reference position and a reference location when the diagnostic imaging is synchronized with the reference image.

11. The ultrasound imaging apparatus of claim 10, wherein
the receiving unit receives signals of a relative position and a relative location of the ultrasound probe based on the reference position and the reference location, and the control unit moves the image indicator according to the relative position and the relative location.

12. The ultrasound imaging apparatus of claim 10, wherein
the receiving unit receives a first image signal and a second image signal of the object, the display unit displays a first diagnostic imaging based on the first image signal and a second diagnostic imaging based on the second image signal on the first section, and the control unit moves the image indicator according to a relative position and a relative location of the second diagnostic imaging based on the first diagnostic imaging.

13. The ultrasound imaging apparatus of claim 3, wherein
the display unit displays the target part on the second section by moving the target organ marker.

14. The ultrasound imaging apparatus of claim 1, further comprising:

an ultrasound probe transmitting an ultrasound to the object, receiving an echo ultrasound reflected from the object, and transforming the echo ultrasound to an electrical signal, wherein the display unit displays a target part of the object on a first section based on the electrical signal.

15. The ultrasound imaging apparatus of claim 14, wherein
the ultrasound probe comprises a detecting unit, wherein the detecting unit detects a relative position and a relative location of the ultrasound probe based on a reference position and a reference location, and the controlling unit moves the image indicator according to the relative position and the relative location.

16. The ultrasound imaging apparatus of claim 15, wherein
the detecting unit comprises at least one of an angular velocity sensor, a magnetic sensor, an acceleration sensor, a gravity sensor, and a gyro sensor.

17. The ultrasound imaging apparatus of claim 1, further comprising:

a storage unit storing at least one reference image.

18. The ultrasound imaging apparatus of claim 1, further comprising an input unit receiving a change signal for changing the reference image from users, wherein the controlling unit synchronizes the changed reference image based on the change signal.

19. a controlling method of an ultrasound imaging apparatus comprising:

receiving an image signal of an object;
displaying a diagnostic imaging on a first section based on the image signal;
synchronizing the diagnostic imaging with a reference image corresponding to the diagnostic imaging; and
displaying an image indicator indicating a target part of the object on a second section.

20. The method of claim 19, further comprising:

displaying at least one reference images similar to the diagnostic imaging on a third section before the synchronizing; and
receiving a selection of one reference image among the at least one reference images from the user, wherein the synchronizing is that the selected reference image by the user is synchronized with the diagnostic imaging.

FIG. 1

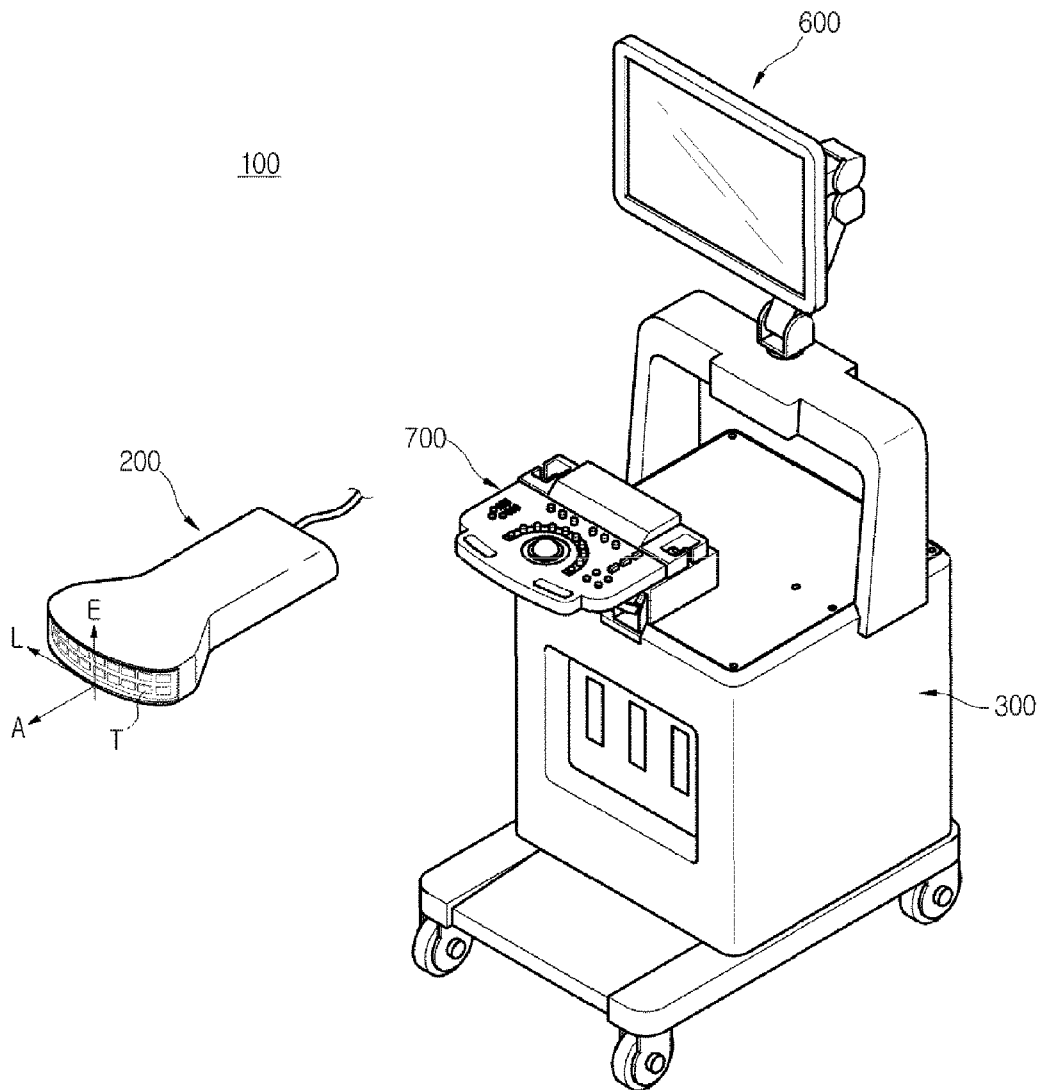


FIG. 2

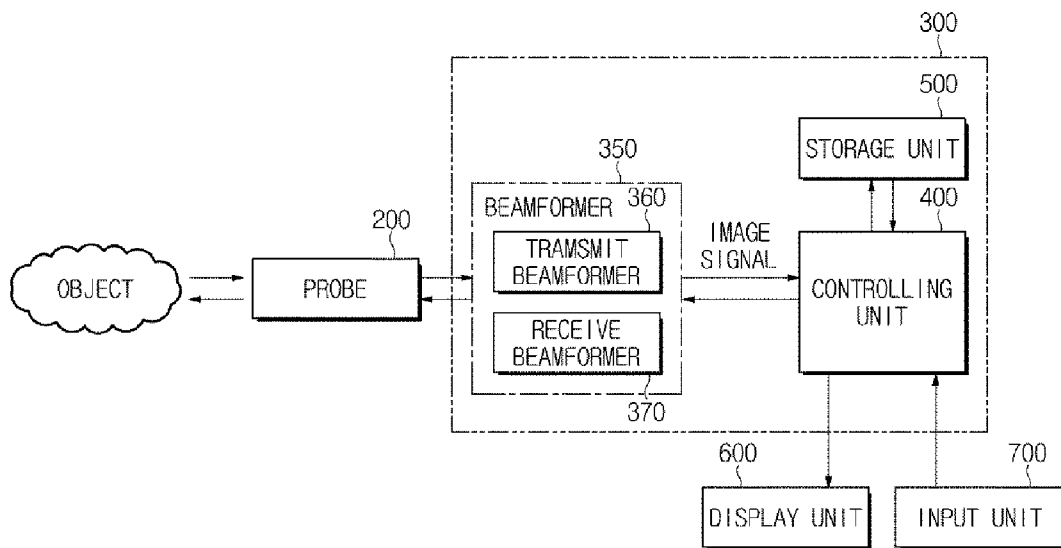


FIG. 3

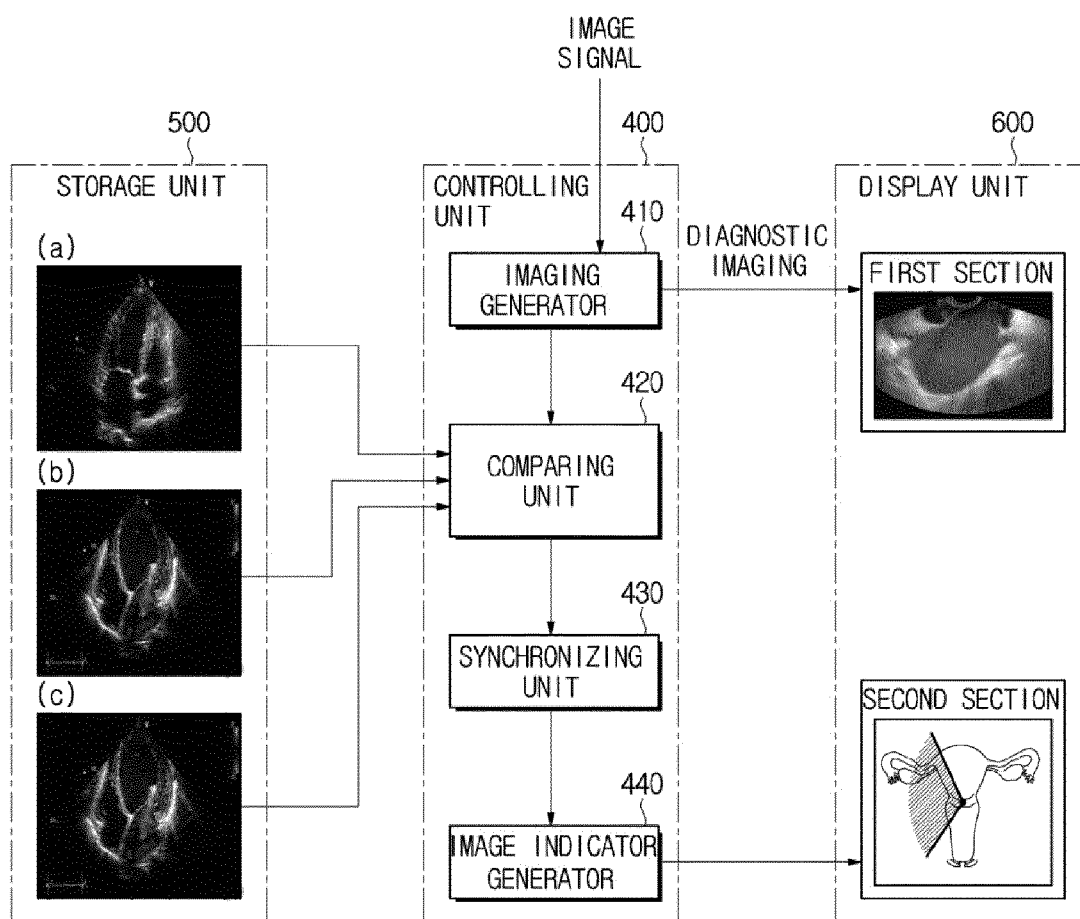


FIG. 4

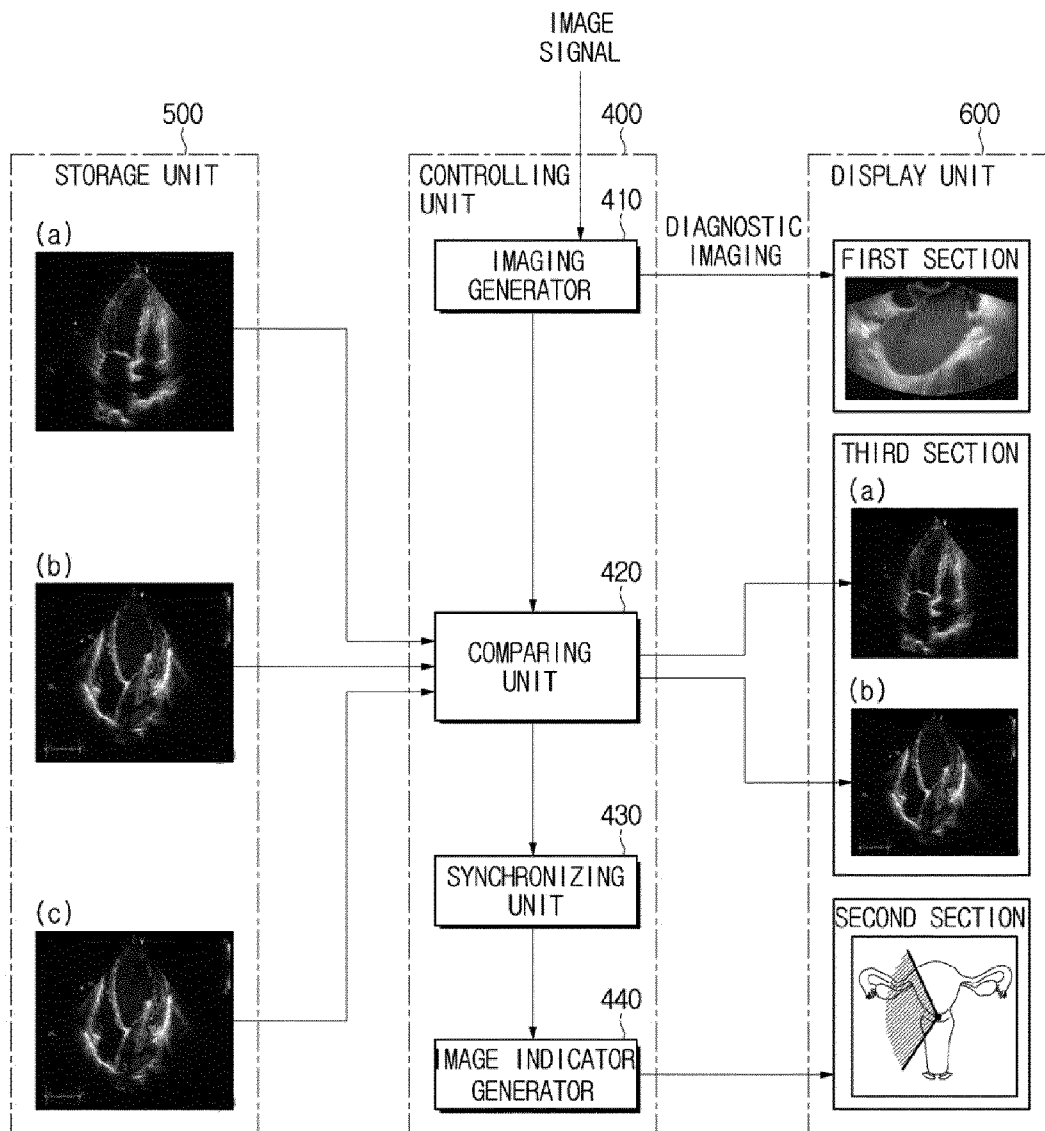


FIG. 5

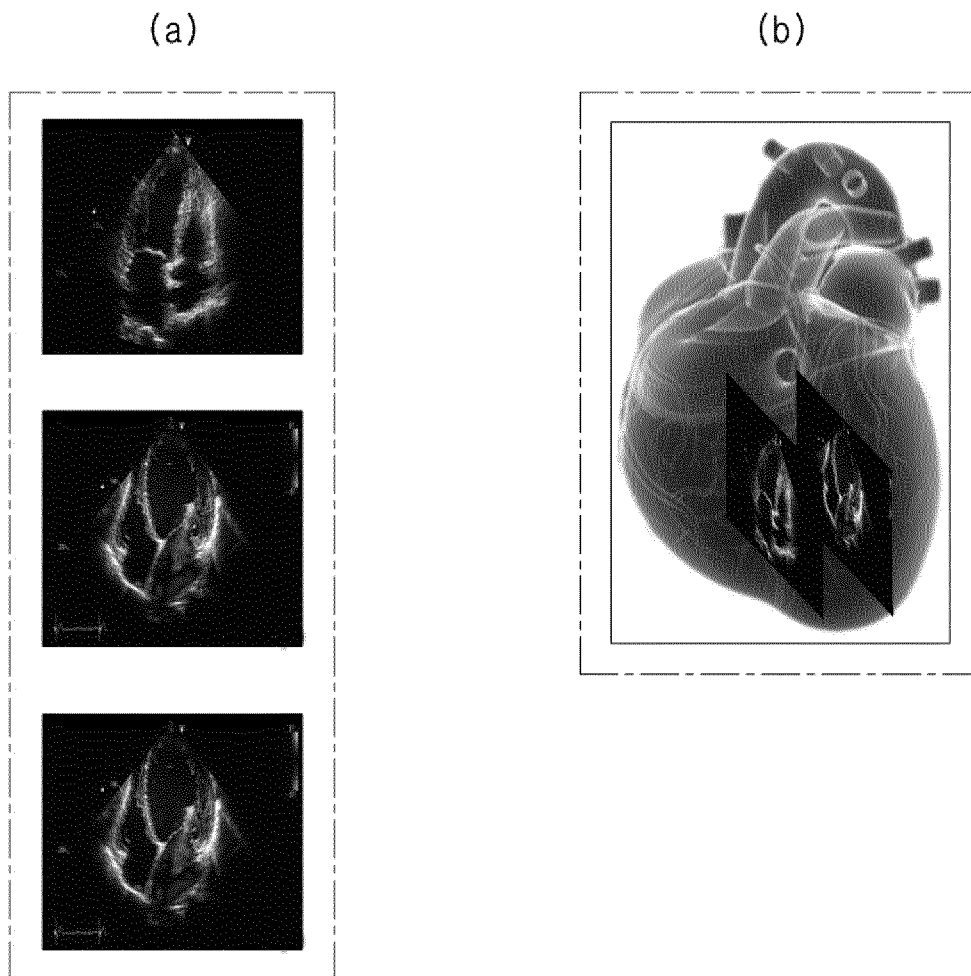


FIG. 6

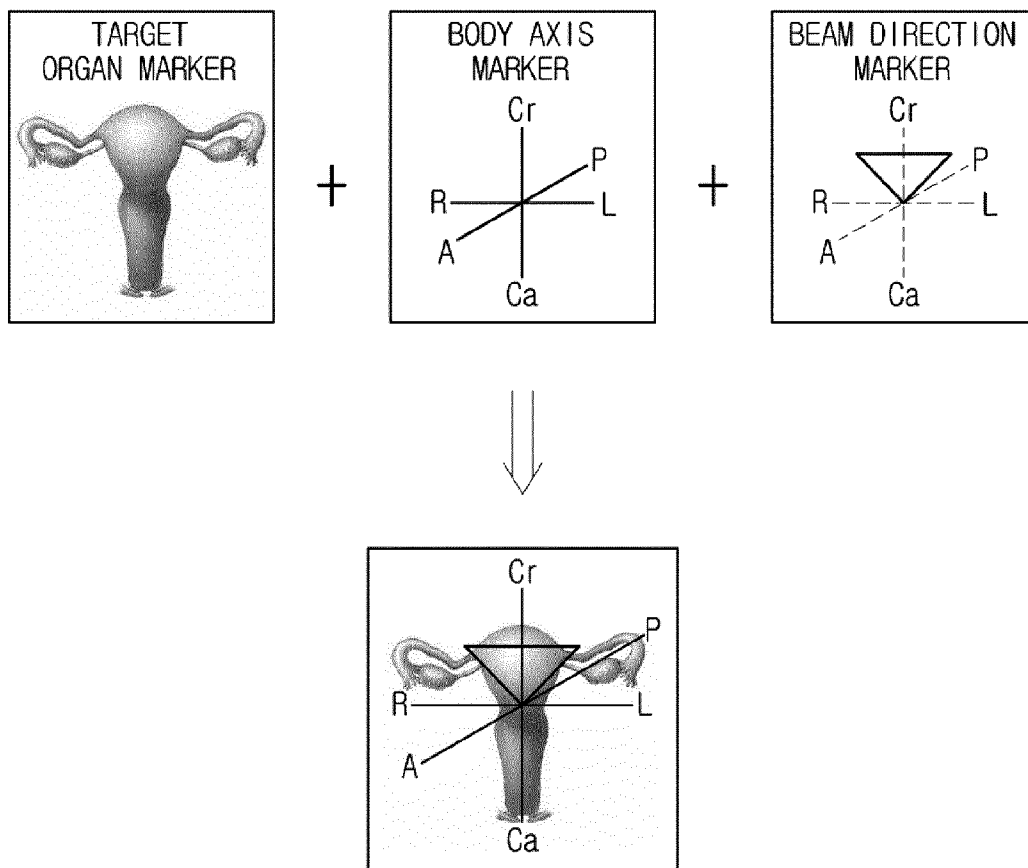


FIG. 7

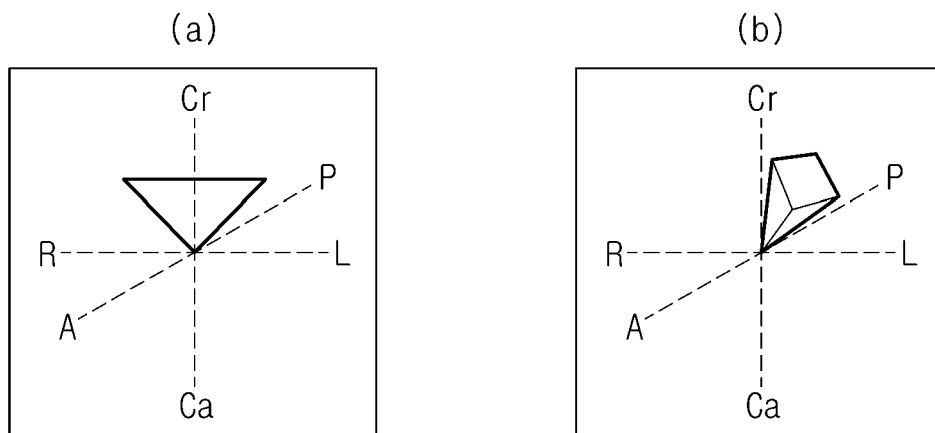


FIG. 8

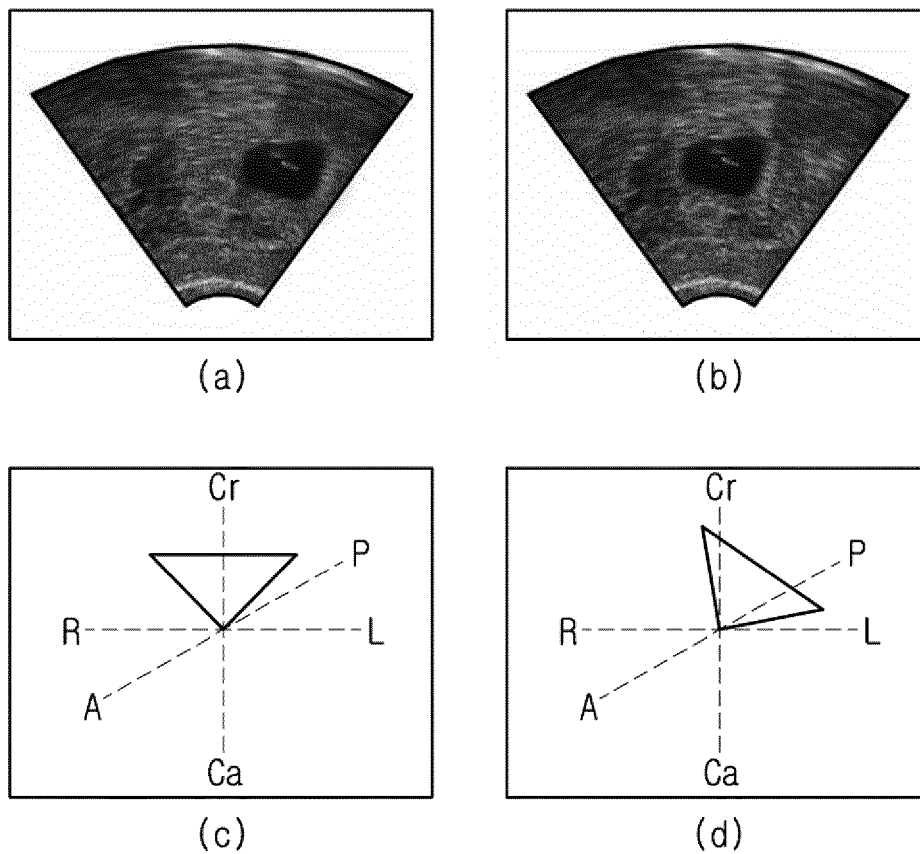


FIG. 9


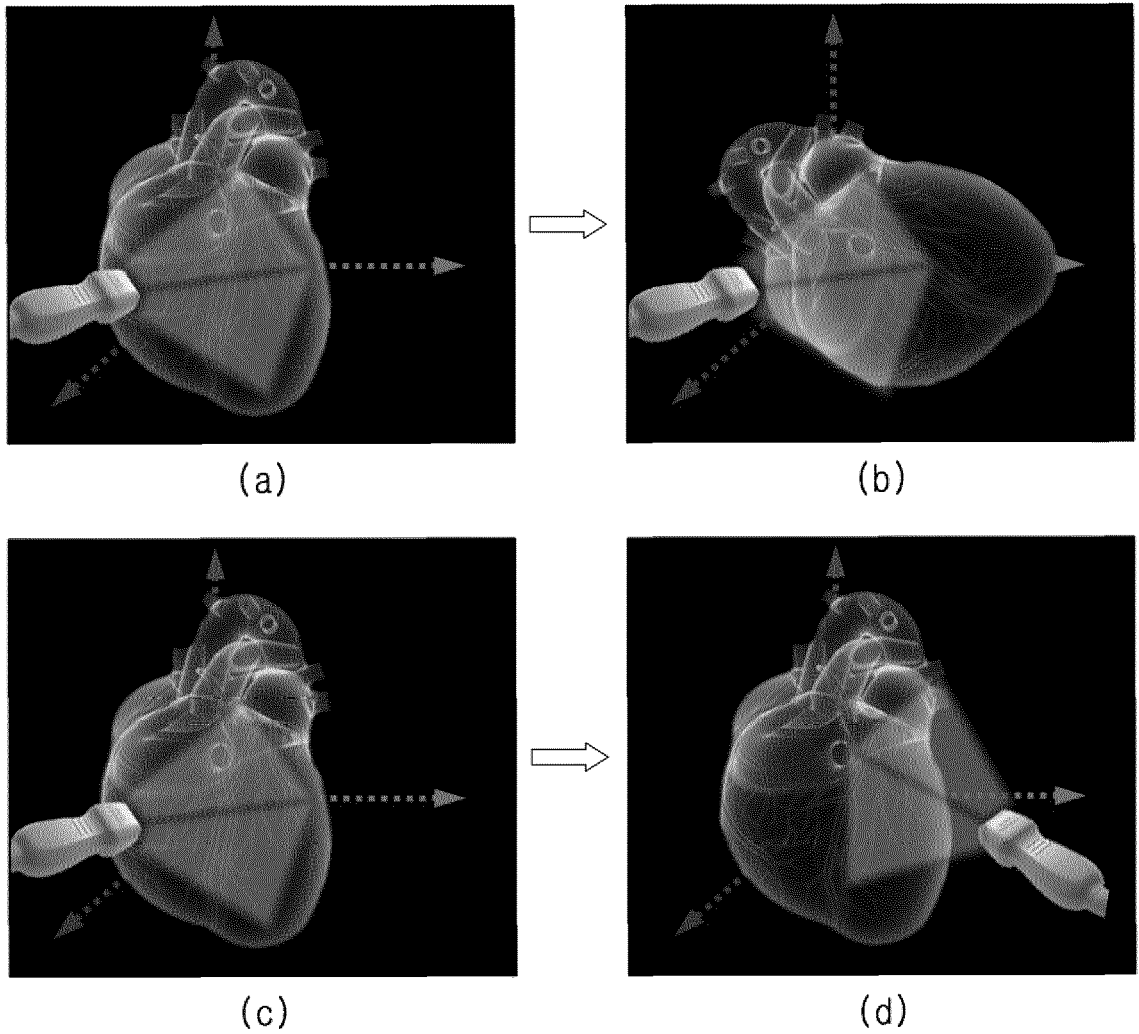


FIG. 10

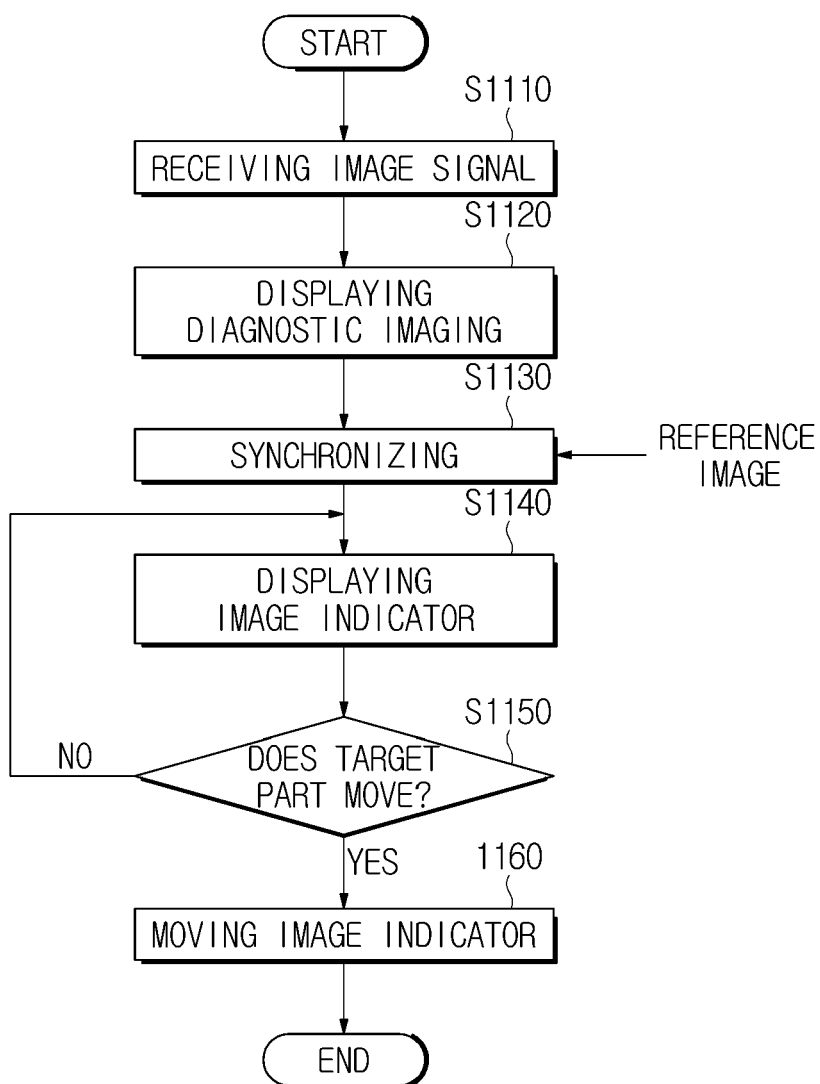

EUROPEAN SEARCH REPORT

Application Number
EP 15 15 3428

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2012/310092 A1 (YAWATA TSUTOMU [JP]) 6 December 2012 (2012-12-06)	1,2,5, 7-20	INV. A61B8/00
Y	* paragraph [0028] - paragraph [0053]; figures 1-8 *	3,4,6	
Y	----- US 2012/220873 A1 (HYUN DONG GYU [KR]) 30 August 2012 (2012-08-30) * figure 4 *	3,4,6	
X	----- EP 2 754 396 A1 (HITACHI MEDICAL CORP [JP]) 16 July 2014 (2014-07-16) * paragraph [0012]; figure 4 *	1,2,5, 7-20	
A	----- US 5 938 607 A (JAGO JAMES R [US] ET AL) 17 August 1999 (1999-08-17) * the whole document *	1-20	
A	----- US 2010/191114 A1 (HYUN DONG GYU [KR] ET AL) 29 July 2010 (2010-07-29) * the whole document *	1-20	TECHNICAL FIELDS SEARCHED (IPC)
			A61B
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 26 November 2015	Examiner Koprinarov, Ivaylo
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03 82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 15 15 3428

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

26-11-2015

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 2012310092	A1	06-12-2012	JP 5717543 B2	13-05-2015
			JP 2012245230 A	13-12-2012
			US 2012310092 A1	06-12-2012

US 2012220873	A1	30-08-2012	EP 2491865 A1	29-08-2012
			JP 2012176239 A	13-09-2012
			US 2012220873 A1	30-08-2012
			US 2014316271 A1	23-10-2014

EP 2754396	A1	16-07-2014	CN 103781426 A	07-05-2014
			EP 2754396 A1	16-07-2014
			JP 5775164 B2	09-09-2015
			JP WO2013035393 A1	23-03-2015
			US 2014236001 A1	21-08-2014
			WO 2013035393 A1	14-03-2013

US 5938607	A	17-08-1999	NONE	

US 2010191114	A1	29-07-2010	EP 2213240 A1	04-08-2010
			JP 2010172701 A	12-08-2010
			KR 20100087521 A	05-08-2010
			US 2010191114 A1	29-07-2010

专利名称(译)	超声成像设备及其控制方法		
公开(公告)号	EP2977012A1	公开(公告)日	2016-01-27
申请号	EP2015153428	申请日	2015-02-02
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星麦迪逊有限公司		
[标]发明人	JIN GIL JU AHN MI JEOUNG BYUN MI AE		
发明人	JIN, GIL JU AHN, MI JEOUNG BYUN, MI AE		
IPC分类号	A61B8/00		
CPC分类号	A61B8/463 A61B8/14 A61B8/4245 A61B8/467 A61B8/5238		
审查员(译)	KOPRINAROV , IVAYLO		
优先权	1020140094214 2014-07-24 KR		
其他公开文献	EP2977012B1		
外部链接	Espacenet		

摘要(译)

本发明公开了一种超声成像设备及其控制方法，所述超声成像设备包括：接收单元，接收对象的成像信号；显示单元，基于所述成像信号在第一部分上显示诊断成像；以及显示图像指示器指示第二部分上的对象的目标部分，以及控制单元使诊断成像与对应于诊断成像的参考图像同步。

