



- (51) International Patent Classification:
A61B 8/00 (2006.01)
- (21) International Application Number:
PCT/US2015/020279
- (22) International Filing Date:
12 March 2015 (12.03.2015)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/952,086 12 March 2014 (12.03.2014) US
- (71) Applicant: FUJIFILM SONOSITE, INC. [US/US];
21919 30th Drive SE, Bothell, WA 98021 (US).
- (72) Inventor: CHAGGARES, N., Chris; 700 Garden Street,
Whitby, Ontario, L7G 7B3 (CA).
- (74) Agents: BELLO, Ryan, M. et al.; Perkins Coie LLP, P.O.
Box 1247, Seattle, WA 98111-1247 (US).
- (81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG,
MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM,
PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC,
SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ,
TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU,
TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE,
DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU,
LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,
SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ,
GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: HIGH FREQUENCY ULTRASOUND TRANSDUCER HAVING AN ULTRASONIC LENS WITH INTEGRAL CENTRAL MATCHING LAYER

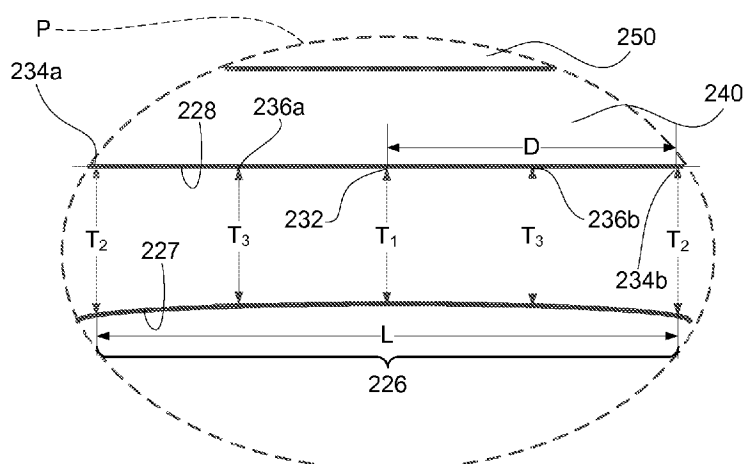


FIG. 2B

(57) Abstract: High frequency ultrasound transducers configured for use with high frequency ultrasound diagnostic imaging systems are disclosed herein. In one embodiment, an ultrasound transducer includes a concave lens having an average thickness in a center portion that that is substantially equal to an odd multiple a 1/4- wavelength of the center frequency of the ultrasound transducer.

HIGH FREQUENCY ULTRASOUND TRANSDUCER HAVING AN ULTRASONIC LENS WITH INTEGRAL CENTRAL MATCHING LAYER

TECHNICAL FIELD

[0001] The disclosed technology generally relates to the fields of ultrasonic transducers and medical diagnostic imaging. More specifically, the disclosed technology relates to high frequency ultrasonic transducers and acoustic lenses configured for use therewith.

PATENTS AND PATENT APPLICATIONS INCORPORATED BY REFERENCE

[0002] The following patents are also incorporated by reference herein in their entireties: U.S. Patent No. 7,052,460, titled "SYSTEM FOR PRODUCING AN ULTRASOUND IMAGE USING LINE-BASED IMAGE RECONSTRUCTION," and filed December 15, 2003; U.S. Patent No. 7,255,648, titled "HIGH FREQUENCY, HIGH FRAME-RATE ULTRASOUND IMAGING SYSTEM," and filed October 10, 2003; U.S. Patent No. 7,230,368, titled "ARRAYED ULTRASOUND TRANSDUCER," and filed April 20, 2005; U.S. Patent No. 7,808,156, titled "ULTRASONIC MATCHING LAYER AND TRANSDUCER," and filed March 2, 2006; U.S. Patent No. 7,901,358, titled "HIGH FREQUENCY ARRAY ULTRASOUND SYSTEM," and filed November 2, 2006; and U.S. Patent No. 8,316,518, titled "METHODS FOR MANUFACTURING ULTRASOUND TRANSDUCERS AND OTHER COMPONENTS," and filed September 18, 2009.

BRIEF DESCRIPTION OF THE DRAWINGS

[0003] The invention may be more completely understood in consideration of the accompanying drawings, which are incorporated in and constitute a part of this specification, and together with the description, serve to illustrate the disclosed technology.

[0004] FIG. 1 is a schematic view of an ultrasound imaging system configured in accordance with one or more embodiments of the disclosed technology.

[0005] FIG. 2A is a cross-sectional schematic view of an ultrasound transducer stack configured in accordance with one or more embodiments of the disclosed technology.

[0006] FIG. 2B is an enlarged view of a portion P of FIG. 2A.

[0007] FIG. 3 is a schematic side view of a prior art transducer.

[0008] FIG. 4 is a schematic side view of a transducer configured in accordance with one or more embodiments of the disclosed technology.

DETAILED DESCRIPTION

[0009] Ultrasonic transducers provide a means for converting electrical energy into acoustic energy and vice versa. When the electrical energy is in the form of a radio frequency (RF) signal, a transducer can produce ultrasonic signals with the same frequency characteristics as the driving electrical RF signal. Conventional clinical ultrasound transducers are typically operated at center frequencies ranging from less than 1 Megahertz (MHz) to about 10 MHz. Ultrasound in the frequency spectrum of 1-10 MHz generally provides a means of imaging biological tissue with a resolution ranging from several millimeters to generally greater than 150 microns and at depths from a few millimeters to greater than 10 centimeters.

[0010] In contrast, high frequency ultrasonic (HFUS) transducers are generally ultrasonic transducers with center frequencies above 15 MHz and ranging to over 60 MHz (e.g., 15 MHz, 20 MHz, 25 MHz, 30 MHz, 40 MHz, 50 MHz, 60 MHz). HFUS transducers provide higher resolution than transducers that operate at lower frequencies (e.g., less than 15 MHz.) while limiting a maximum depth of penetration. As a result, HFUS transducers can image biological tissue at depths ranging from, for example, a fraction of a millimeter (e.g., 0.25mm, 0.5mm, 0.75mm) to 3 cm or greater (e.g., 4cm) with resolutions ranging, for example, from about 20 microns to about 200 microns.

[0011] For transducers operating at frequencies less than 10 MHz, for example, a wide variety of lens materials are available to produce convex lenses that are substantially acoustically impedance-matched to a medium (e.g., tissue in a subject) to be imaged. Acoustic energy received at these transducers is typically almost

completely transmitted through the lens material to be received by the transducer, with almost no energy reflected back into the medium, and thus no multipath artifacts are created. In addition, one skilled in the art will understand that a well-designed transducer, having a well matched lens material will not exhibit multiple reflections within the lens itself. In the case of HFUS transducers, however, very few materials are suitable for constructing acoustic lenses due to significantly higher acoustic attenuation. As those of ordinary skill in the art will appreciate, acoustic attenuation in polymers tends to increase exponentially with frequency. Accordingly, an acoustic attenuation of ultrasound energy at 20 MHz in a polymer can be an order of magnitude (e.g., 10 times greater, 20 times greater, 100 times greater) than an acoustic attenuation of ultrasound energy of 10 MHz and below in the same polymer.

[0012] There can be many challenges associated with fabricating HFUS transducers that do not arise when working with traditional clinical ultrasonic transducers that operate at frequencies below about 10 MHz. Those of ordinary skill in the art will appreciate that structures (e.g., transducer layers, matching layers, lenses) associated with an ultrasound transducer generally scale in a manner that is inversely proportional to an operating frequency of the transducer. For example, a 50 MHz transducer will have structures about 10 times smaller than a 5 MHz transducer. In many cases, materials or techniques used with lower frequency transducers (e.g., less than about 10 MHz.) cannot be scaled down to sizes and/or shapes suitable for use in HFUS transducers. Accordingly, new technologies may need to be developed or adapted in the fabrication of HFUS transducers. In other cases, entirely new requirements exist when dealing with the higher radio frequency electronic and acoustic signals associated with HFUS transducers.

[0013] Conventional HFUS transducers typically include hard plastic acoustic lenses shaped and/or formed into concave lenses in order to focus an elevation dimension of the transducer. Suitable HFUS lens materials may include, for example, polymethylpentene (e.g., TPX®), cross-linked polystyrene (e.g., Rexolite®), and polybenzimidazole (e.g., Celazole®), all of which have relatively low attenuation at frequencies greater than about 15 MHz. Acoustic lenses made from materials suited for HFUS use, however, may also have acoustic impedances significantly or substantially different (e.g., 10% different, 25% different, 50% different) from an

acoustic impedance of a subject to be imaged. The resulting acoustic impedance mismatch (e.g., a difference of 0.1 MRayl, 0.3 MRayl, 0.5 MRayl, 1 MRayl, 2 MRayls) between the lens and the subject can cause multipath imaging artifacts when ultrasound energy is transmitted from the transducer and received at the transducer to form an ultrasound image. An acoustic impedance mismatch at the front of the lens with respect to the coupling medium or the subject can also result in intra-lens reflections and/or lens reverberation artifacts that can degrade the axial resolution of the ultrasound transducer.

[0014] The multipath or multi-bounce artifacts can cause a ghost image of bright specular reflectors appearing an equal depth below the true image of the specular reflector. A skin line of a subject, for example, may be imaged at a depth of 4mm in the image and cause a multipath artifact at a depth of 8mm. Those of ordinary skill in the art will appreciate that such an artifact may be produced when ultrasonic energy emitted from the transducer strikes a strong specular reflector (e.g., a skin line of a subject) roughly normal to the path of the ultrasound. A portion (e.g., 5%, 10%) of the emitted ultrasonic energy may be reflected back from the specular reflector toward the transducer lens, whereupon a second reflection may occur if the lens is not substantially acoustically matched to the transmission medium (e.g., gel, water). The second reflection may then propagate back to the specular reflector a second time, where again, a specular reflection occurs and acoustic energy is once again received by the transducer. A cascade of such reflections can cause a series of multipath artifacts to appear in an ultrasound image. Such partial reflections can occur repeatedly until no significant energy remains in the reflections. One approach to mitigating imaging artifacts may include positioning an acoustic matching layer on an outer surface of an acoustic lens. Lenses having matching layers on their outer surfaces, however, can be very difficult to fabricate and, in many cases, are impractical for use with ultrasound transducers that operate at higher frequencies (e.g., greater than about 15 MHz.).

[0015] Lens reverberation artifacts caused by, for example, intra-lens multiple reflections can be similar to the multipath artifacts described above. Intra-lens reflections, however, occur entirely within the lens material and may be caused by an acoustic mismatch between the outer surface of the lens and the acoustic coupling

medium or the subject being imaged. A partial echo is produced at the front face of the lens as the acoustic pulse exits the transducer and enters the subject. This echo can then reverberate between any internal acoustic mismatch in the transducer acoustic stack, such as the back surface of the lens for example. As those of ordinary skill in the art will appreciate, every effort will be made to acoustically match the back surface of the lens to the acoustic stack of the transducer, typically through the use of some form of acoustic matching layer. However, due to the low attenuation of HFUS lens materials, even a small reflection from the back surface/stack interface can give rise to a lens reverb artifact. The effect of the lens reverb artifact is to effectively lengthen the pulse of the transducer as each reverb echo become part of the main transducer pulse and thus any echoes received by the transducer.

[0016] FIG. 3 is a schematic view of a prior art transducer 380 that illustrates one example of the intra-lens reflections and reverberation artifacts described above. The transducer 380 includes a transducer layer 382, a matching layer 384 and an acoustic lens 386 having a lower surface 388 and a thickness T. The transducer 380 transmits and receives ultrasound energy (e.g., high frequency ultrasound of 15 MHz or greater) through a skin line 392 of a subject 390 (e.g., a human patient, an animal). The transducer layer 382 is configured to transmit a primary ultrasound signal S into the subject 390 and receives ultrasound echoes S', which are used to form an ultrasound image.

[0017] First, second and third reflections R1, R1' and R1'' illustrate one example of the multipath artifacts described above. The skin line 392 reflects a portion (e.g., 5%, 10%, 20%) of the signal S thereby forming the first reflection R1. The first reflection R1 propagates back toward the transducer layer 382, which reflects a portion (e.g., 5%, 10%, 20%) of the first reflection R1 back toward the subject thereby forming the second reflection R1'. The skin line 392 reflects a portion of the second reflection R1' back toward the transducer layer 382 thereby forming the third reflection R1''. The transducer layer 382 receives the echoes S' along with portions of the first reflection R1 and third reflection R1'', all of which are combined by an image processor (not shown) to form an ultrasound image. As those of ordinary skill in the art will appreciate, the reflections R1 and R1'' can cause undesirable artifacts in the ultrasound image.

[0018] First, second and third reflections R2, R2' and R2'' illustrate one example of the intra-lens reverberation artifacts described above. The lower surface 388 of the lens 386 reflects a portion (e.g., 5%, 10%, 20%) of the signal S thereby forming the first reflection R2. The first reflection R2 propagates back toward the transducer layer 382, which reflects a portion (e.g., 5%, 10%, 20%) of the first reflection R2 back toward the subject thereby forming the second reflection R2'. The lower surface 388 of the lens 386 reflects a portion of the second reflection R2' back toward the transducer layer 382 thereby forming the third reflection R2''. The transducer layer 382 receives a combination of the echoes S' along with portions of the first reflection R2 and the third reflection R2'' to form an ultrasound image. The reflections R2 and R2'' can cause undesirable artifacts in the ultrasound image. In many instances, reflections similar to R1, R1'', R2 and R2'' can cause artifacts in the same ultrasound image, which can significantly reduce image quality.

[0019] FIG. 4 is a schematic side view of a transducer 480 configured in accordance with one or more embodiments of the disclosed technology. The transducer 480 includes an lens 486 having a curved surface 422 and a center portion 426. The center portion 426 has an average thickness approximately equal to an odd multiple of a quarter wavelength (e.g., 1/4-wavelength, 3/4-wavelength, 5/4-wavelength, 7/4-wavelength) of the center frequency of the transducer 480. A signal S2 is transmitted into the subject 390. The skin line 392 reflects a portion of the signal S2 to form a first reflection R3, and the curved portion 422 reflects a portion of the signal S2 to form second reflections R4. In contrast to reflections R1 and R2 discussed above, the first reflection R3 and the second reflections R4 are not specular reflections and thus do not travel back to the transducer 382. Accordingly the lens 486 can significantly reduce artifacts in a HFUS image, such as the intra-lens and multipath reflections discussed above with reference to FIG. 3.

[0020] The disclosed technology can provide a reduction of multipath artifacts (e.g., intra-lens reverberation artifacts, external multi-bounce artifacts) in HFUS transducers described above. In one aspect of the present disclosure, an ultrasound transducer includes an acoustical lens in which a center portion of the lens (e.g., the thinnest part of the concave shape of the lens between two end portions of the lens) has a thickness of about a fractional portion of a wavelength of the transducer center

frequency. In some embodiments, for example, the lens center portion can have an average thickness approximately equal to an odd multiple of a quarter wavelength (e.g., 1/4-wavelength, 3/4-wavelength, 5/4-wavelength, 7/4-wavelength) of the transducer center frequency (e.g., 15 MHz, 20 MHz, 25 MHz, 30 MHz). Incorporating the lens described above onto an ultrasound transducer results in the central portion of the lens effectively adding an additional matching layer (e.g., a quarter wavelength matching layer) to the front of the transducer. The disclosed technology therefore provides a lens having reduced acoustic reflectivity to normal incident plane waves, thus mitigating multipath acoustic artifacts in the image, and reducing intra lens reverb artifacts as well. In some embodiments, for example, the disclosed technology can increase the transmission coefficient of an HFUS transducer lens from 85% to about 95%. Stated differently, the disclosed technology can reduce the reflection coefficient of an HFUS transducer lens from 15% to less than between 5% and 10% or less, thereby significantly increasing sensitivity of the HFUS transducer (e.g., an increase between 1dB and 2.5dB).

[0021] In another aspect of the disclosed technology, an ultrasound transducer stack includes a transducer layer and a lens layer. The transducer layer is configured to transmit ultrasound energy at a center frequency (e.g., 15 MHz or higher). The lens layer has an upper surface underlying the transducer layer. At least a portion of the lens layer has a concave curvature in a direction normal to an axial direction of the transducer. A center portion of the lens layer has an average thickness that is substantially equal to an odd multiple (e.g., 1, 3, 5) of a 1/4 wavelength of the center frequency of the transducer layer. In some embodiments, a matching layer is disposed between the lens layer and the transducer layer. In one embodiment, for example, the matching layer is attached to the lens layer by another matching layer that comprises cyanoacrylate. In some embodiments, the lens layer has an acoustic impedance substantially different (e.g., 10% different, 25% different, 50% different) than an acoustic impedance of water.

[0022] In yet another aspect of the disclosed technology, an ultrasound system includes an ultrasound imaging system coupled to an ultrasound transducer probe. The ultrasound transducer probe is configured to transmit ultrasound toward a subject and receive ultrasound energy from the subject. The transducer probe includes a lens

layer and one or more transducer elements configured to operate at a center frequency (e.g., between about 15 MHz and about 60 MHz). A portion of the lens layer has a concave curvature in a direction normal to an axial direction of the transducer. A center portion of the concave curvature has an average thickness substantially equal to (e.g., within about 1%, within about 2%, within about 5%) an odd multiple (e.g., 1, 3, 5, 7, 9) of a $1/4$ wavelength of the center frequency of the one or more transducer elements. In some embodiments, a reflection coefficient of the lens layer is less than about 5%. In some embodiments, the reflection coefficient is between, for example, about 1% and 15%.

[0023] In still another aspect of the disclosed technology, a method of constructing an ultrasound transducer includes fabricating an acoustic lens layer and attaching or bonding the lens layer to a first matching layer operationally coupled to a transducer layer. The lens layer is fabricated to have a center curved section and two flat side sections. Fabricating the curved section includes fabricating a center portion having a midpoint and two endpoints such that the center portion has a first thickness at the midpoint and a second thickness at each of the two endpoints. An average of the first thickness and the second thickness is substantially equal to (e.g., within about 1%, within about 2%, within about 5%) an odd multiple of a $1/4$ wavelength (e.g., $1/4$ -wavelength, $3/4$ wavelength, $5/4$ -wavelength) of the center frequency (e.g., between about 15 MHz and about 60 MHz) of the ultrasound transducer. In some embodiments, the method further includes bonding or attaching a second matching layer to the lens layer with the first matching layer such that the second matching layer is positioned between the first matching layer and the transducer layer. In some embodiments, the lens layer has a speed of sound significantly different (e.g., 100% different, 200% different) than a speed of sound in water.

[0024] In another aspect of the disclosed technology, an ultrasound transducer stack includes a transducer layer comprising one or more ultrasound transducer elements configured to operate at a center frequency of 15 MHz or greater (e.g., between about 15 MHz and about 60 MHz). The transducer stack further includes an acoustic lens having a rear surface attached to a matching layer operationally coupled to the transducer layer. A front surface of the acoustic lens includes two flat side sections and a center curved section extending therebetween in an elevation direction

relative to the transducer stack. A first thickness of the center curved section in an axial direction relative to the transducer stack is less than an odd multiple of 1/4-wavelength of the center frequency. The thickness of the center curved section increases outwardly a first distance in the elevation direction to an endpoint having a second thickness in the axial direction that is greater than an odd multiple of 1/4-wavelength of the center frequency such that the average thickness in the axial direction of the center curved section between the midpoint and the endpoint is substantially an odd multiple of 1/4-wavelength of the center frequency. In some embodiments, a length of the center curved section is twice the first distance. In some embodiments, the length of the center curved section is about 10% or less of a total length of the transducer stack in the elevation direction. In some embodiments, the first thickness is between about 95% and 99.5% of the odd multiple of the 1/4-wavelength of the center frequency, and the second thickness is between about 100.5% and 105% of the odd multiple of the 1/4-wavelength of the center frequency.

Suitable Systems

[0025] FIG. 1 is a schematic view of an ultrasound system 100 configured in accordance with an embodiment of the disclosed technology. The ultrasound system 100 includes an ultrasound probe 104 coupled to an image processing system 102 via a link 106 (e.g., a wire, a wireless connection). The probe 104 includes a transducer 110 (e.g., an HFUS stack). The transducer 110 can transmit ultrasound energy (e.g., HFUS energy) into a subject and receive at least a portion of the reflected ultrasound energy from the subject. The received ultrasound energy can be converted into a corresponding electrical signal and transmitted electrically to the image processing system 102, which can form one or more ultrasound images based on the received ultrasound energy.

[0026] FIG. 2A is a cross section schematic view of an ultrasound transducer stack 210 (e.g., the transducer 110 of FIG. 1) configured in accordance with one or more embodiments of the disclosed technology. The transducer stack 210 includes an acoustic lens 220, a first matching layer 240, a second matching layer 250, a third matching layer 255 and a transducer layer 260 (e.g., a piezoelectric transducer layer, a PMUT layer, a CMUT layer). In some embodiments, the first matching layer 240 can

include a bonding material (e.g., cyanoacrylate, a polymer, an epoxy) having a 1/4-wavelength thickness and can be configured to bond or otherwise attach a front surface of the second matching layer 250 to a rear surface 228 of the lens 220. A rear surface of the matching layer 250 is bonded or otherwise attached to a front surface of the third matching layer 255. A rear surface of the third matching layer 255 is attached to a front surface of the transducer layer 260. A centerline 221 extends along an axial direction (i.e., along the y-axis shown in FIG. 2A) of the transducer stack 210. In the illustrated embodiment, the transducer stack 210 includes a three matching layers—the first matching layer 240, the second matching layer 250 and the third matching layer 255. In some embodiments, however, the transducer stack 210 may include one or more additional matching layers as disclosed, for example, in U.S. Patent No. 7,808,156, incorporated by reference above. Other embodiments of the transducer stack 210 may not include one or more of the first matching layer 240, the second matching layer 250 and the third matching layer 255.

[0027] The lens 220 includes a curved section 222 that has a concave curvature (e.g., cylindrical, parabolic or hyperbolic curvature) in an elevation direction (i.e., along the x-axis shown in FIG. 2) of the transducer stack 210. The curved section 222 is bounded by side section 224 (identified individually as a first side section 224a and a second side section 224b). The curved section 222 has a curved outer surface 227 and the flat side portions 224 have outer surfaces 229 (identified individually as a first outer surface 229a and a second outer surface 229b). The curved section 222 includes a center portion 226 centered at the centerline 221. As discussed in more detail with reference to FIG. 2A, the center portion 226 has a first thickness T_1 at a midpoint and a second thickness T_2 at two endpoints. The center portion 222 has a length L (e.g., less than 0.5mm, 0.5mm, 0.7mm, 1mm, greater than 1mm) in the elevation direction of the transducer. In some embodiments, the length L can extend between about 1% and 10% of the length of the transducer in the elevation direction. In some embodiments, the length L and a radius of curvature of the center portion 226 can be determined by the focal number (e.g., F_2 , F_5 , F_8 , F_{10}) of the lens and the focal depth of the transducer. As those of ordinary skill in the art will appreciate, the focal number of the lens is proportional to a ratio of the focal depth of the transducer and a length of the curved section 222 of the lens.

[0028] The lens 220 can comprise, for example, polymethylpentene, cross-linked polystyrene and/or polybenzimidazole. In other embodiments, however, the lens 220 can comprise any suitable material (e.g., metals, such as aluminum or stainless steel, or ceramic materials, such as PZT or alumina) having a speed of sound higher than a speed of sound of a medium being imaged (e.g., water, tissue in a subject). Moreover, in some embodiments, the first thickness T_1 of the center portion 226 may be slightly less than an odd multiple of $1/4$ of the wavelength (e.g., between approximately 95% and 99.5% of an odd multiple of the $1/4$ wavelength thickness) of a center frequency (e.g., 15 MHz or greater) of the transducer layer 260. Correspondingly, the second thickness T_2 may be slightly more than an odd multiple of $1/4$ of the wavelength (e.g., between approximately 100.5% and 105% of an odd multiple of the $1/4$ wavelength thickness) of the center frequency. The center portion 226 of the curved section 222 therefore has a substantially average thickness of approximately an odd multiple of $1/4$ of the wavelength (within a $\pm 5\%$ of an odd multiple of $1/4$ wavelength). Fabricating the center portion 226 to have an average thickness substantially equal to a fractional wavelength of the center frequency of the transducer layer 260 can provide an improved acoustic match to a subject being imaged and therefore can significantly reduce multipath reflections compared to an acoustic lens having an arbitrary thickness.

[0029] FIG. 2B is an enlarged view of a portion P of FIG. 2A showing the center portion 226 in more detail. The center portion 222 has a midpoint 232 and extends between a first endpoint 234a and second endpoint 234b in the elevation direction. The midpoint 232 is spaced apart from each of the first and second midpoints 234a and 234b a distance D in the elevation direction (i.e., one-half the length L). The thickness of the center portion 222 in the axial direction increases outwardly from T_1 at the midpoint 232 to the thickness T_2 at each of the first and second midpoints 234a and 234b. The average thickness of the center portion 222 substantially equal to an odd multiple (e.g., 1, 3, 5, 7) of a $1/4$ -wavelength of the center frequency of the transducer layer 260 (FIG. 2A). Further, at intermediate points 236a and 236b, the center portion 222 has a thickness T_3 generally corresponds to the average thickness of the center portion 222 between midpoint 232 and each of the first and second midpoints 234a and 234b.

[0030] In some embodiments, however, the center portion 226 can be configured to have an average $\frac{3}{4}$ -wavelength thickness to provide adequate dielectric strength to meet desired medical electrical safety standards. In other embodiments, the center portion 226 may have an average thickness less than $\frac{3}{4}$ wavelength. In some embodiments, for example, the center portion 226 can be fabricated to have an average thickness of the $\frac{1}{4}$ of the wavelength of an operational center frequency (e.g., 20 MHz, 25 MHz, 30 MHz) of the transducer layer 260. In some embodiments, the average thickness of the center portion 226 can be any odd multiple (e.g., 1, 3, 5, 7, 9) of $\frac{1}{4}$ of the wavelength of the operational center frequency of the transducer layer 260 (FIG. 2A). In other embodiments, however, the average thickness can be any suitable fraction of the wavelength of the operational center frequency of the transducer layer 260 (FIG. 2A). Those of ordinary skill in the art will appreciate, for example, that for broadband ultrasound transducers, a $\frac{1}{4}$ wavelength lens thickness will generally perform better than a $\frac{3}{4}$ wavelength lens thickness, and increasing odd multiples of $\frac{1}{4}$ -wavelength generally perform progressively worse. In contrast, narrowband transducers (e.g., CW Doppler transducers) can have acoustic lenses with increasing odd multiples of the $\frac{1}{4}$ -wavelength without a significant reduction in performance.

[0031] Fabricating the center portion 226 to have of an average thickness corresponding generally to a fractional portion (e.g., $\frac{1}{4}$, $\frac{3}{4}$) of the wavelength can, in addition to minimizing multi-path artifacts, acoustically enhance a central part of the elevation dimension (i.e., along the x-axis of FIG. 2A) of the transducer layer 260 (FIG. 2A), thereby providing a desirable boost to a normal component of the elevation beam. This can be viewed as achieving the equivalent of mild apodization of the elevation beam by enhancing the central part of the beam relative to the edges, as opposed to attenuating the edges relative to the center of the beam. The apodization of the elevation beam can lead to a reduction in sidelobes in the elevation beam.

[0032] From the foregoing, it will be appreciated that specific embodiments of the invention have been described herein for purposes of illustration, but that various modifications may be made without deviating from the scope of the invention. Accordingly, the invention is not limited except as by the appended claims.

CLAIMS

I/We claim:

1. An ultrasound transducer stack comprising:
a transducer layer configured to transmit ultrasound energy at a center frequency; and
an lens layer having an upper surface underlying the transducer layer, wherein at least a portion of the lens layer has a concave curvature in a direction normal to an axial direction of the transducer, and wherein a center portion of the lens layer has an average thickness that is substantially equal to an odd multiple of a $1/4$ wavelength of the center frequency of the transducer layer.
2. The ultrasound transducer of claim 1 wherein the center frequency of the transducer layer is greater than 15 MHz, and wherein the lens layer is acoustically penetrable at frequencies greater than 15 MHz.
3. The ultrasound transducer of claim 1 wherein the average thickness of the center portion of the lens layer is $1/4$ of the wavelength of the center frequency of the transducer layer.
4. The ultrasound transducer of claim 1 wherein the average thickness of the center portion of the lens layer is $3/4$ of the wavelength of the center frequency of the transducer layer.
5. The ultrasound transducer of claim 1, further comprising a matching layer disposed between the transducer layer and the lens layer.
6. The ultrasound transducer of claim 5 wherein the matching layer is a first matching layer, further comprising a second matching layer between the lens layer and the first matching layer, wherein the second matching layer comprises cyanoacrylate,

and wherein the first matching layer and the second matching layer each have a thickness approximately $1/4$ -wavelength of the center frequency of the transducer layer.

7. The ultrasound transducer of claim 1 wherein the lens layer has an acoustic impedance substantially different than an acoustic impedance of water.

8. An ultrasound system, comprising:
an ultrasound imaging system; and
an ultrasound transducer probe coupled to the imaging system and configured to transmit ultrasound toward a subject and receive ultrasound energy from the subject, wherein the ultrasound transducer probe includes:
one or more transducer elements configured to operate at a center operating frequency; and
a lens layer, wherein at least a portion of the lens layer has a concave curvature in a direction normal to an axial direction of the transducer, and wherein a center portion of the concave curvature has an average thickness substantially equal an odd multiple of $1/4$ wavelength of the center operating frequency of the one or more transducer elements.

9. The ultrasound transducer of claim 8 wherein the center operating frequency of the one or more transducer elements is greater than 15 MHz, and wherein the lens layer is acoustically penetrable at frequencies greater than 15 MHz.

10. The ultrasound transducer of claim 9 wherein a reflection coefficient of the lens layer is less than 10%.

11. The ultrasound transducer of claim 8 wherein the average thickness of the center portion of the lens layer is $1/4$ of the wavelength of the center frequency.

12. The ultrasound transducer of claim 8 wherein the average thickness of the center portion of the lens layer is $3/4$ of the wavelength of the center frequency.

13. A method of constructing an ultrasound transducer, comprising:
fabricating an acoustic lens layer having a center curved section and two flat side sections, wherein fabricating the curved section includes fabricating a center portion having a midpoint and two endpoints such that the center portion has a first thickness at the midpoint and a second thickness at each of the two endpoints, and wherein an average of the first thickness and the second thickness is substantially equal to an odd multiple of a $1/4$ wavelength of the center frequency of the ultrasound transducer; and
bonding the lens layer to a matching layer operationally coupled to a transducer layer.

14. The method of claim 13 wherein the matching layer is a first matching layer comprising an epoxy, and wherein bonding the lens layer comprises bonding a second matching layer to the lens layer using the first matching layer that comprises an epoxy such that the second matching layer is positioned between the first matching layer and the transducer layer.

15. The method of claim 13 wherein bonding the lens layer comprises bonding the lens layer to a matching layer operationally coupled to a transducer layer configured to operate at a center frequency of 15 MHz or greater.

16. The method of claim 13 wherein a speed of sound of the lens layer is significantly different than the speed of sound in water.

17. An ultrasound transducer stack, comprising:
a transducer layer comprising one or more ultrasound transducer elements configured to operate at a center frequency of 15 MHz or greater;
a matching layer spaced apart from the transducer layer in an axial direction relative to the transducer stack; and
an acoustic lens having a front surface and a rear surface, wherein the rear surface of the lens is attached to the matching layer, wherein the front surface includes two flat side sections and a center curved section

extending therebetween in an elevation direction relative to the transducer stack, wherein a first thickness of the center curved section in an axial direction relative to the transducer stack is less than an odd multiple of $1/4$ -wavelength of the center frequency, wherein the thickness of the center curved section increases outwardly a first distance in the elevation direction to an endpoint having a second thickness in the axial direction that is greater than an odd multiple of $1/4$ -wavelength of the center frequency, and wherein the average thickness in the axial direction of the center curved section between the midpoint and the endpoint is substantially an odd multiple of $1/4$ -wavelength of the center frequency.

18. The ultrasound transducer stack of claim 17 wherein the center curved section has a length that is approximately two times greater than the first distance.

19. The ultrasound transducer stack of claim 18 wherein the length is about 10% or less of a total length of the transducer stack in the elevation direction.

20. The ultrasound transducer stack of claim 17 wherein the first thickness is between about 95% and 99.5% of the odd multiple of the $1/4$ -wavelength of the center frequency, and wherein the second thickness is between about 100.5% and 105% of the odd multiple of the $1/4$ -wavelength of the center frequency.

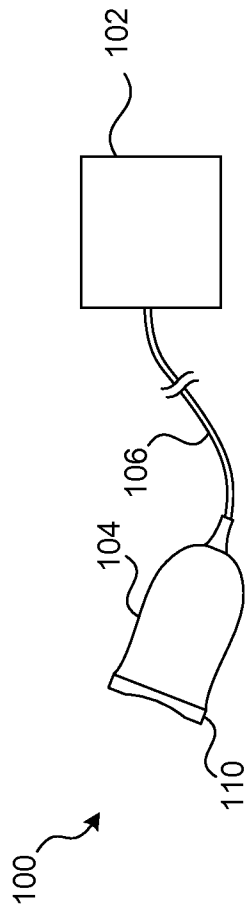


FIG. 1

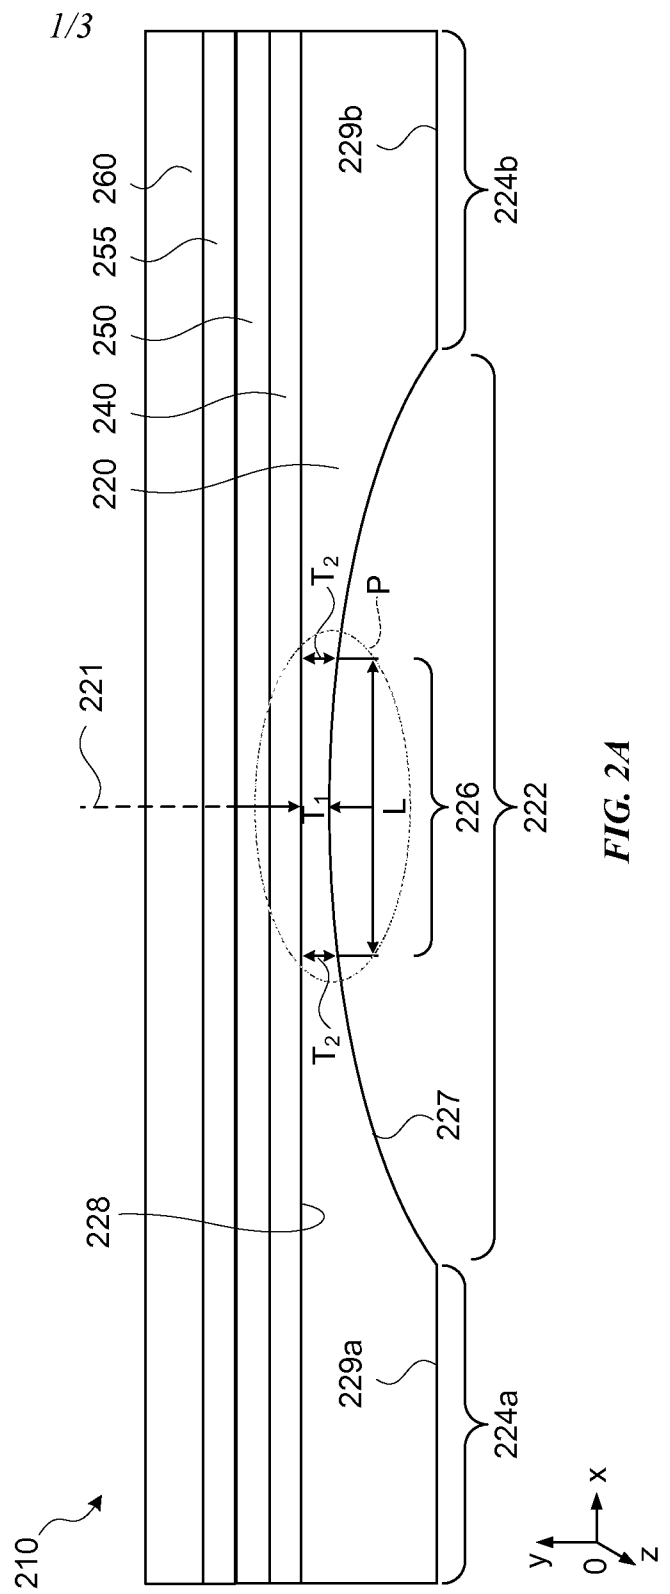
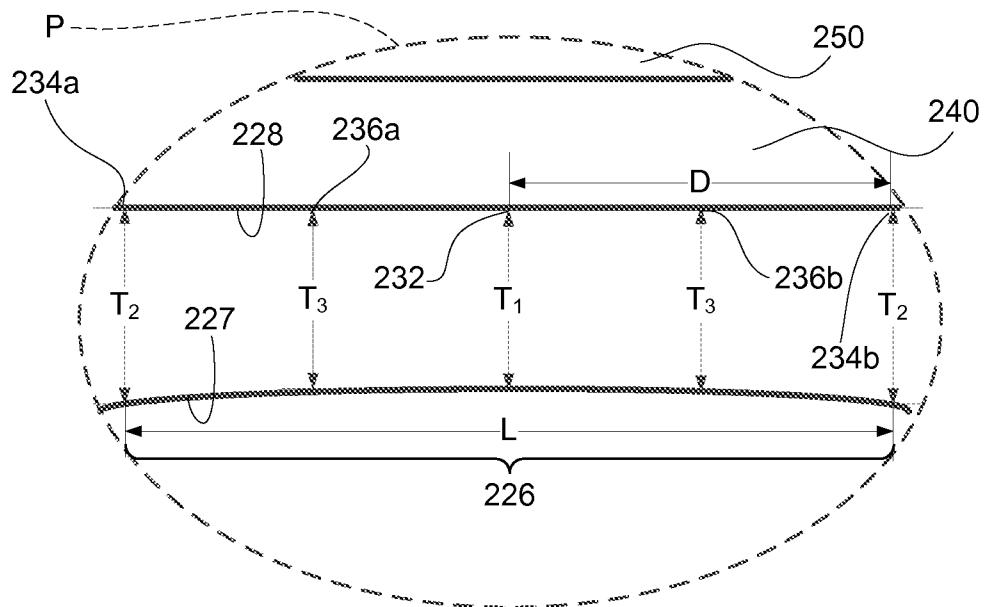


FIG. 2A

2/3

**FIG. 2B**

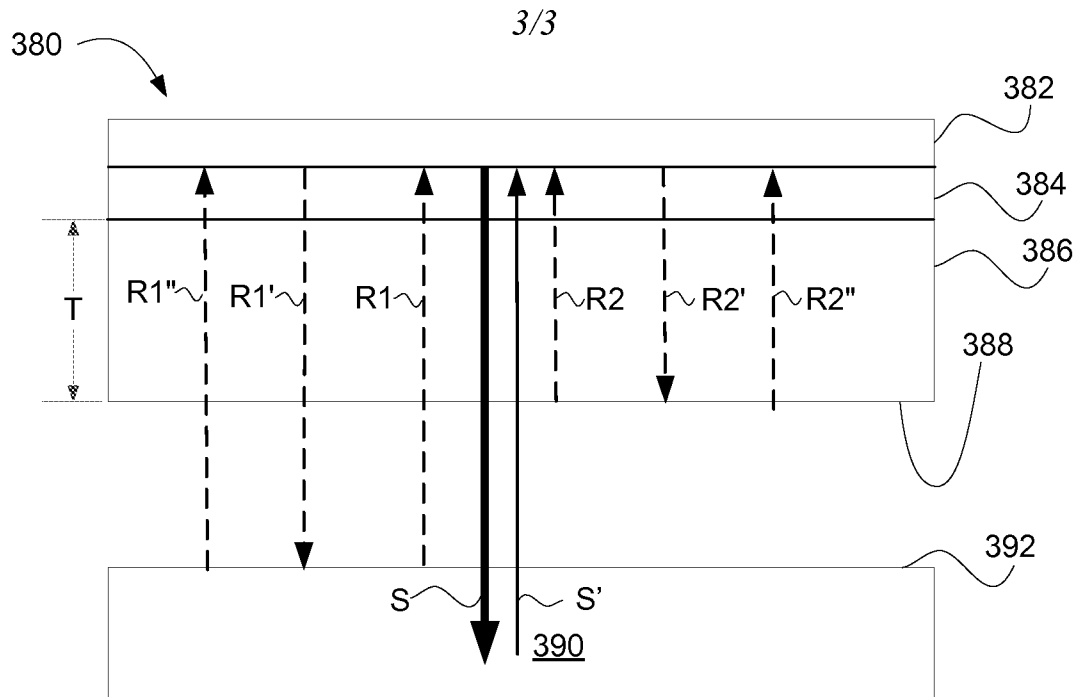


FIG. 3
(PRIOR ART)

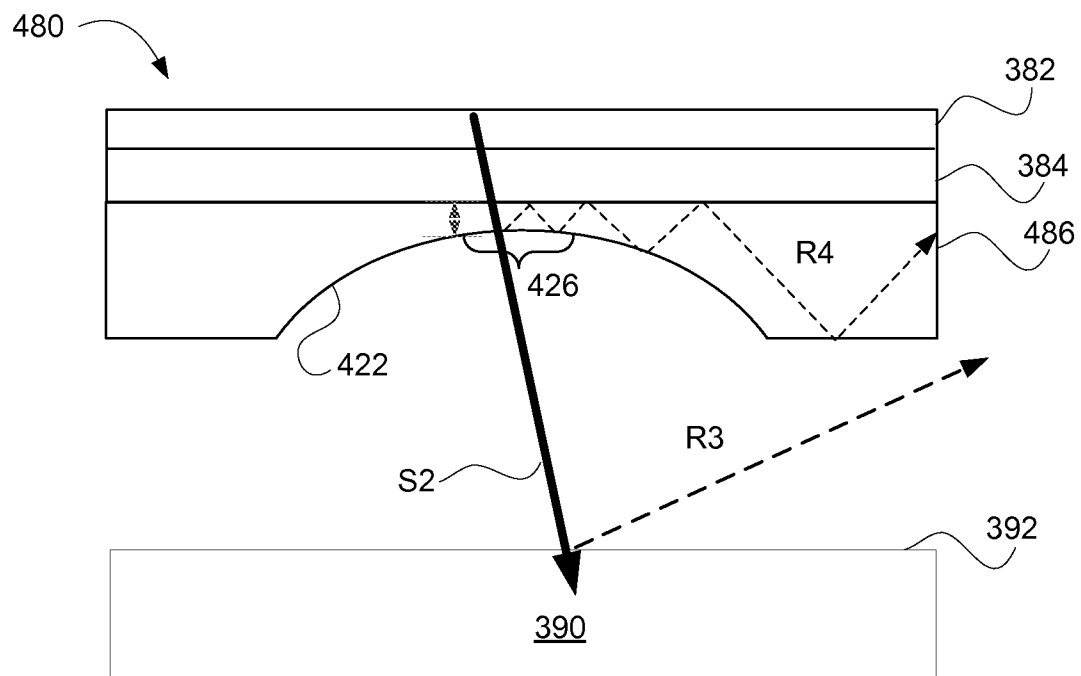


FIG. 4

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2015/020279**A. CLASSIFICATION OF SUBJECT MATTER****A61B 8/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 8/00; B06B 1/06; A61B 17/00; H01L 41/22; H01L 41/00; G01N 29/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & keywords: ultrasound, transducer, stack, lens, concave, 1/4-wavelength, center frequency

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2010-0156244 A1 (MARC LUKACS et al.) 24 June 2010 See abstract, paragraphs [0006]-[0082], claims 1-26 and figures 1-4.	1-7,9,10,13-16
A		8,11,12,17-20
X	US 6443900 B2 (HIDEO ADACHI et al.) 03 September 2002 See abstract, column 1, lines 14-20, column 13, lines 5-40, column 24, lines 32-40 and figures 9A,9B.	8,11,12
Y		1-7,9,10,13-16
A	US 2007-0205697 A1 (N. CHRIS CHAGGARES et al.) 06 September 2007 See abstract, paragraphs [0067]-[0078] and figure 4.	1-20
A	US 2008-0194965 A1 (JOHN W. SLIWA et al.) 14 August 2008 See abstract, paragraphs [0074]-[0103] and figures 4-12.	1-20
A	WO 2008-097527 A1 (BROWN UNIVERSITY et al.) 14 August 2008 See abstract, pages 8-12 and figures 1A,1B.	1-20



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

18 June 2015 (18.06.2015)

Date of mailing of the international search report

19 June 2015 (19.06.2015)

Name and mailing address of the ISA/KR


International Application Division
Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City, 302-701,
Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

KIM, Tae Hoon

Telephone No. +82-42-481-8407



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2015/020279

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2010-0156244 A1	24/06/2010	CN 102308375 A	04/01/2012
		CN 102308375 B	28/01/2015
		CN 103811366 A	21/05/2014
		EP 2344042 A1	20/07/2011
		EP 2345066 A1	20/07/2011
		JP 2012-503370 A	02/02/2012
		JP 2014-131357A	10/07/2014
		JP 5723775 B2	27/05/2015
		US 2011-0144494 A1	16/06/2011
		US 2013-096434 A1	18/04/2013
		US 8316518 B2	27/11/2012
		WO 2010-031192 A1	25/03/2010
		WO 2010-031192 A8	17/06/2010
		WO 2010-033867 A1	25/03/2010
US 6443900 B2	03/09/2002	JP 2001-258879 A	25/09/2001
		JP 2002-248100 A	03/09/2002
		JP 4602574 B2	22/12/2010
		US 2002-0007118 A1	17/01/2002
US 2007-0205697 A1	06/09/2007	CA 2644227 A1	13/09/2007
		CN 101442940 A	27/05/2009
		CN 101442940 B	17/12/2014
		CN 103861796 A	18/06/2014
		EP 2004064 A2	24/12/2008
		EP 2004064 A4	02/05/2012
		JP 2009-528784 A	06/08/2009
		JP 2012-235524 A	29/11/2012
		JP 2013-081241 A	02/05/2013
		JP 5415086 B2	12/02/2014
		JP 5634452 B2	03/12/2014
		US 7808156 B2	05/10/2010
		WO 2007-103144 A2	13/09/2007
		WO 2007-103144 A3	24/04/2008
US 2008-0194965 A1	14/08/2008	CN 101652102 A	17/02/2010
		EP 2112906 A2	04/11/2009
		EP 2112906 A4	30/03/2011
		EP 2112906 B1	11/09/2013
		JP 2010-517695 A	27/05/2010
		JP 5352475 B2	27/11/2013
		US 8382689 B2	26/02/2013
		WO 2008-098101 A2	14/08/2008
		WO 2008-098101 A3	20/11/2008
WO 2008-097527 A1	14/08/2008	EP 2115450 A1	11/11/2009
		EP 2115450 A4	04/03/2015
		JP 2010-518396 A	27/05/2010
		JP 5406729 B2	05/02/2014

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2015/020279

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 2011-0036171 A1	17/02/2011
		US 8302480 B2	06/11/2012

专利名称(译)	具有带有整体中心匹配层的超声透镜的高频超声换能器		
公开(公告)号	EP3116405A1	公开(公告)日	2017-01-18
申请号	EP2015762059	申请日	2015-03-12
[标]申请(专利权)人(译)	富士胶片索诺声公司		
申请(专利权)人(译)	FUJIFILM SONOSITE , INC.		
当前申请(专利权)人(译)	FUJIFILM SONOSITE , INC.		
[标]发明人	CHAGGARES N CHRIS		
发明人	CHAGGARES, N., CHRIS		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4272 B06B1/067 G10K11/30 Y10T156/10		
优先权	61/952086 2014-03-12 US		
其他公开文献	EP3116405A4		
外部链接	Espacenet		

摘要(译)

本文公开了配置用于高频超声诊断成像系统的高频超声换能器。在一个实施例中，超声换能器包括凹透镜，该凹透镜在中心部分具有平均厚度，该凹透镜基本上等于超声换能器的中心频率的奇数倍1/4波长。