



(51) International Patent Classification:

A61B 8/00 (2006.01) A61B 8/13 (2006.01)

A61B 8/12 (2006.01) A61B 8/14 (2006.01)

(21) International Application Number:

PCT/US2018/038788

(22) International Filing Date:

21 June 2018 (21.06.2018)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/524,196 23 June 2017 (23.06.2017) US

(71) Applicant: ORAL DIAGNOSTIX, LLC [US/US]; 101 Calvert Avenue, Clinton, South Carolina 29325 (US).

(72) Inventor: KATZBERG, Richard W. (deceased).

(74) Agent: MARCUS, Tara L.; BLANK ROME LLP, 1825 Eye Street NW, Washington, District of Columbia 20006 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP,

KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))

Published:

— with international search report (Art. 21(3))

(54) Title: TRANSORAL ULTRASOUND PROBE AND METHOD OF USE

(57) Abstract: A transoral ultrasound probe for imaging a temporomandibular joint and a method of imaging a temporomandibular joint using a transoral probe.

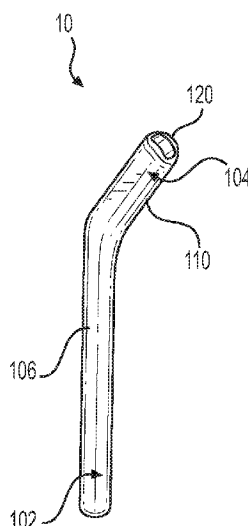


FIG. 2A



TRANSORAL ULTRASOUND PROBE AND METHOD OF USE

RELATED APPLICATION

[0001] The present application claims priority to U.S. provisional application no. 62/524,196, filed June 23, 2017, the entire disclosure of which is incorporated herein by reference.

FIELD OF THE INVENTION

[0002] The present invention relates to a transoral probe for ultrasound imaging of the jaw, namely the temporomandibular joint.

BACKGROUND

[0003] Temporomandibular disorders (TMD) are a significant public health problem that represents a group of potentially debilitating conditions affecting approximately 5% to 12% of the population in the U.S. TMD is the second most common musculoskeletal condition (after chronic low back pain) that is associated with pain and disability and is often the result of disc displacement and the resulting mechanical temporomandibular joint (TMJ) dysfunction. Pain-related TMD can impact an individual's daily activities, psychosocial function, and quality of life. Research regarding disc displacement has indicated that the clinical approaches for assessing disc displacement can lead to diagnoses that exhibit sensitivities as low as 0.34-0.54 Volts p-p. Consequently, improved clinical diagnosis, treatment decision-making in specific presentations, and confirmation of the diagnosis of disc displacement, requires imaging.

[0004] Current TMJ imaging technologies include panoramic radiographs, cone beam CT (CBCT) for hard tissues only, and magnetic resonance imaging (MRI). There are several barriers to the widespread use of these technologies and effectiveness for TMD diagnosis, such as the medical risk of exposure to ionizing radiation with panoramic radiographs and CBCT, high cost of both CBCT and MRI, limited accessibility of MRI systems that are located in hospitals and medical imaging laboratories, and patient-related claustrophobic concerns and the consequent management requirements for anxiolytics. Arthrography has also been previously used for imaging but was abandoned due to its invasive nature.

[0005] Prior attempts at developing ultrasound imaging of the TMJ have been suboptimal due to the utilization of large-sized imaging probes that are constrained to imaging approaches of only the axial and coronal anatomical planes because the images can only be acquired externally from the side of the patient's face. Bone barriers restrict sound penetration to only the superficial aspect of the entire TMJ soft tissue anatomy. Even if ultrasound energy had the penetrating ability to image the entire axial and coronal TMJ anatomy, these two anatomical planes of imaging are not adequate to depict disc displacement. Research has shown that the external imaging approach, as shown in FIG. 1, achieved only a 22.8% specificity for disc displacement in the closed-mouth position and zero specificity for disc displacement in the opened-mouth position.

[0006] FIG. 1 illustrates such suboptimal ultrasound imaging approached externally with large probes. The external facial approach has not gained clinical acceptance because: 1) the sound penetration is severely limited by the markedly contoured anatomy of the bones of the condyle, tubercle and zygomatic arch of the TMJ; and 2) of being limited to the depiction of only the axial (transverse) and coronal (longitudinal) planes of imaging. The external bone barriers restrict sound penetration to only the superficial aspects of the TMJ anatomy. Extensive literature and extensive clinical experiences derived from TMJ arthrotomography, CT and MRI, have proven that the sagittal plane of imaging is preferred for the effective and accurate depiction of TMJ disc displacement.

[0007] Therefore, there is a need for imaging modality that can accurately depict dynamic TMJ function as an integral characteristic of routine medical ultrasound imaging.

SUMMARY

[0008] A transoral ultrasound probe for imaging a temporomandibular joint, comprising a handle section that has a longitudinal axis, the handle section being configured for connection to a power source; and an intraoral section that has a cephalad angulation such that the intraoral section is positioned at an operative angle with respect to the longitudinal axis of the handle section, and the intraoral section is configured to emit and receive sound waves. The operative angle of the intraoral section is preferably an acute angle.

[0009] In one embodiment, the operative angle is less than 45 degrees and/or is about 30 degrees. In a certain embodiment, the handle section has a longitudinal length and the intraoral section has a length that is about one-third shorter than the longitudinal length of the handle section; the handle section has a first width and the intraoral section has a second width, and the second width is greater than the first width; the handle section and the intraoral section have substantially the same thickness and the thickness is less than or equal to the first width; the handle and intraoral sections define substantially flat side surfaces and the thickness extends between the side surfaces; a distal end of the intraoral section is rounded; the intraoral section includes a transducer aperture at a distal end thereof configured to emit and receive the sound waves; the handle section is connected to the power source via a power cable or the power source is at least one battery connected to the handle section; and/or the power source is either coupled to or is part of a control unit.

[0010] A method of imaging a temporomandibular joint using a transoral probe that has a handle section and an intraoral section with a cephalad angulation, that comprises the steps of holding the handle section of the transoral probe; inserting the intraoral section of the transoral probe into a patient's mouth in a recess between the cheek and gum such that a transducer aperture of the intraoral section generally faces the temporomandibular joint; and emitting and receiving sound waves via the transducer aperture on the intraoral section of the transoral probe thereby producing images of the temporomandibular joint in at least the sagittal anatomical plane.

[0011] In one embodiment of the method, the step of emitting and receiving sound waves produces images of the temporomandibular joint in all anatomical planes, including the axial, coronal, and sagittal planes. In other embodiments, the method further comprises the step of controlling the amplitude, frequency, and duration of the sound waves emitted from the transducer aperture of the transoral probe; and/or the step of connecting the transoral probe to a power source. In certain embodiments of the method, the intraoral section of the transoral probe is positioned at an operative angle with respect to a longitudinal axis of the handle section, and the operative angle is an acute angle; the operative angle of the intraoral section is about 30 degrees; the handle and intraoral sections define substantially flat side surfaces and a thickness that extends between the side surfaces; the handle section has a first width and the intraoral section has a second width that is larger than the first width; and/or a distal end of the intraoral section of the transoral probe is rounded.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] A more complete appreciation of the invention and many of the attendant advantages thereof will be readily obtained as the same becomes better understood by reference to the following detailed description when considered in connection with the accompanying drawings, wherein:

[0013] FIG. 1 is a diagrammatic view of a prior art method of imaging the temporomandibular joint;

[0014] FIGS. 2A thru 2C are perspective and elevational views of a transoral probe according to an exemplary embodiment of the present invention;

[0015] FIGS. 3A thru 3C are diagrammatic views of an exemplary probe orientation and window of imaging into the temporomandibular joint inside of a patient's mouth in accordance with the present invention; and

[0016] FIG. 4 is an exemplary sonogram image of the temporomandibular joint produced in accordance with the present invention and method.

DETAILED DESCRIPTION

[0017] The present invention generally relates to a transoral ultrasound probe 10 and use thereof for imaging inside of a patient's mouth, such as the temporomandibular joint, for diagnosis and treatment of disc displacement disorders. The present invention preferably provides transoral sagittal high resolution dynamic ultrasound as an effective imaging modality to depict temporomandibular joint (TMJ) structure and function. The present invention may be an imaging tool that can detect TMJ disc displacement, assess the onset and progression of disease, and facilitate longitudinal diagnostics to monitor treatment outcomes. The present invention, among other things, advances imaging of TMJ disc displacement to complement the medical history and clinical examination of the patient; provides dynamic TMJ imaging for clinical research and improved imaging capabilities for practicing clinicians in the diagnosis and treatment of TMJ disorders; permits multidimensional joint visualization, particularly useful for routine screening of patients with joint dysfunction; provides images that clearly show the structure of the disc or as a part of the joint capsule or joint effusion; and is ergonomically designed for optimal patient comfort.

[0018] TMJ imaging in the clinical setting that is achieved with the transoral ultrasound imaging of the present invention, may be used for screening protocols to establish the presence or absence and severity of disc displacement in TMD patients. Other advantages of the present invention include that it provides non-invasive procedure; there is no ionizing radiation risk; it is capable of 3-D and 4-D imaging of joint function and mechanics; it is accessible and has ease of portability; it is interactive, point-to-care clinical adjunct; and it has a low expense.

[0019] Ultrasound imaging is a highly sophisticated medical technology that eliminates and minimizes many of the negatives currently found in TMJ diagnostics. A benefit of the present invention is that ultrasound imaging of TMD will be more readily accessible and have widespread utilization for expanded clinical diagnosis, screening for asymptomatic disease, and research.

[0020] The transoral probe 10 of the present invention is designed to acquire ultrasound images of the TMJ via a transoral soft tissue window 200 that depicts the anatomic sagittal plane and is of adequate imaging depth to encompass the entire joint anatomy. The probe 10 of the present invention preferably provides transoral sagittal imaging for impacting this field of research and for point-to-care clinical diagnostics.

[0021] The ultrasound probe (or transducer) 10 produces sound waves that bounce off body tissues and make echoes, and also receives the echoes and sends them to a control unit or computer 12 that uses them to create an image or sonogram. The probe 10 is configured to be connected to a power source 14, which may be separate from or part of the control unit 12. The control unit 12 does the calculations and can display and/or print the processed images. In one embodiment, the probe 10 is connected to the power source 14 via a power cable C. Alternatively, the power source 14 may be one or more batteries connected to or received in the probe 10. The control unit 12 may also include pulse control for changing the amplitude, frequency and duration of the sound waves emitted from the probe 10.

[0022] The probe 10 is designed for acoustic, mechanical and electrical optimization thereof. The probe 10 may have, for example, about an 8-10 MHz center frequency-wide band (minimum 70%+ bandwidth), 32 elements, about 0.3 mm pitch, and about 3.5 mm elevation. The acoustic design of probe 10 may integrate a piezo-composite, for example, with matching layer and backing components optimized for the high resolution for a shallow depth range (e.g. 40-45 mm). The electrical design of the probe 10 may be composed of specialized circuitry to allow construction of the smallest probe size possible. The probe cable exit 122 may be reduced to a circumference as small as possible.

[0023] As seen in FIGS. 2A-2C, the transoral probe 10 generally includes a handle section 102 configured to facilitate gripping and manipulation of the probe 10 and an intraoral section 104 configured for insertion into the patient's mouth for ultrasound imaging of the temporomandibular joint. The probe 10 preferably has an ergonomic configuration for patient comfort when the probe 10 is inserted into the patient's mouth. The probe 10 may be

ergonomically optimized particularly to fit inside the mouth between the cheek and gum of the soft tissue recess of the posterior maxillary region. The ergonomic configuration of the probe 10 may include substantially flat side surfaces 106 and 108 with opposing generally rounded margins 110 and 112 extending between the side surfaces 106 and 108. In a preferred embodiment, the thickness T of the probe 10 at the margins 110 and 112 is relatively thin, thereby giving the probe 10 a generally flat shape (particularly as compared to the rounded configuration of traditional probes) similar to a spatula.

[0024] The ergonomic configuration of the probe 10 is also preferably compact and not bulky or rectangular with squared off edges, like in some conventional probes. The distal end 118 of the intraoral section 104 may be rounded for additional patient comfort. The length of the intraoral section 104 is preferably shorter than the length of the handle section 102. For example, the intraoral section 104 may be about one-third shorter than the handle section 102. In one embodiment, the intraoral section 104 is about 1.88 inches or about 4.5cm long and the handle section 102 is about 3.77 inches or about 9.5cm long for a total length of the probe 10 being about 5.66 inches or about 14cm. The width W_1 of the intraoral section 104 is preferably greater or larger than the width W_2 of the handle section 102. The width W_1 of the intraoral section 104 may be, for example, about 0.45 inches or about 1.1 cm. The thickness T of the probe 10 is preferably the same at both the handle and intraoral sections 102 and 104 and is preferably the same as or less than the width W_2 of the handle section 102. The thickness T may be, for example, about 0.35 inches or about 0.9 cm. The ergonomic and compact design of the probe 10 also allows unrestricted movement of the patient's jaw while imaging the same, thereby producing more accurate images of the TMJ movement and also adding to the patient's comfort.

[0025] The intraoral section 104 has a cephalad angulation (also known as toward-the-head) such that it is positioned at an operative angle α with respect to a longitudinal axis 114 of the handle section 102 for optimal imaging of the temporomandibular joint and patient comfort when the intraoral section 104 is inserted into the patient's mouth. The operative angle α is preferably less than 90 degrees, more preferably less than 45 degrees, and most preferably about 30 degrees. The intraoral section 104 is configured to emit and receive sound waves via a

transducer aperture 120. In a preferred embodiment, the transducer aperture 120 is located at or near the distal end 118 of the intraoral section 104, as best seen in FIGS. 2A and 2C.

[0026] Ultrasound imaging according to the present invention may be performed by using a pulse-echo technique, for example, that sends and receives sound waves/energy via the intraoral section 104 and aperture 120. The transoral probe 10 converts electrical energy into a brief pulse of high-frequency sound energy that is transmitted into the patient's tissue. The probe 10 then becomes a receiver, detecting echoes of sound energy reflected from the tissue. Real-time images of moving patient tissues may be produced and displayed via control unit 12 depicting TMJ condyle, disc and muscle movement. In accordance with the present invention, images may be produced in any anatomical (hypothetical) plane, i.e. the axial (or horizontal) plane, the coronal (or vertical) plane, and the sagittal (or median) plane. The axial anatomical plane divides the body into cranial and caudal (head and feet) portions; the coronal anatomical plane divides the body into dorsal and ventral (back and front) portions; and the sagittal anatomical plane divides the body into left and right portions. The transoral probe 10 is designed to allow for images of the TMJ in the sagittal plane, in addition to the axial and coronal planes, which provides the most effective and accurate depiction of the TMJ, including the TMJ disc, condyle, and fossa (and movement thereof).

[0027] Optimal visualization of the TMJ may be performed through a transoral window (between the cheek and gum) 200 that is devoid of bone to allow adequate sound transmission. FIGS. 3A-3C are diagrammatic views of a preferred orientation of the transoral probe 10 of the present invention, showing how the probe 10 is to be positioned in the window 200 between the cheek and gum of the upper maxillary arch to acquire sagittal ultrasound images of the condyle and disc of the temporomandibular joint therethrough without bone hindrance.

[0028] A method of imaging a temporomandibular joint according to the present invention using the transoral probe 10 generally comprises the steps of, once connected to a power source, holding and manipulating the handle section 102 of the transoral probe 10 and inserting the intraoral section 104 into a patient's mouth in the window 200 between the cheek and gum such

that the transducer aperture 120 thereof generally faces the temporomandibular joint. Once properly inserted and positioned in the patient's mouth, the probe 10 is activated to emit and receive sound waves via the transducer aperture 120, thereby producing images (via software and control unit 12) of the temporomandibular joint in at least the sagittal anatomical plane and preferably in all of the anatomical planes, i.e. the axial, coronal, and sagittal planes. The amplitude, frequency, and duration of the sound waves emitted from the transducer aperture 120 of the transoral probe 10 may be controlled and adjusted by the control unit 12.

[0029] In unblinded preliminary observations, the present invention provided the first TMJ images acquired by sagittal transoral sonography. The condyle and its subcondylar surface, as seen in FIG. 4, were visible in all subject joints. The condyle (C), which is the rounded protuberance at the end of the bone for articulation with another bone, is vertically oriented and hypoechoic; whereas, the subcondylar surface is arc-shaped and echogenic, having a cap-like appearance (small arrowheads in FIG. 4). The condyle is also identifiable by its translational and rotational motion with jaw opening and closing.

[0030] While particular embodiments have been chosen to illustrate the invention, it will be understood by those skilled in the art that various changes and modifications can be made therein without departing from the scope of the invention as defined in the appended claims.

WHAT IS CLAIMED IS:

1. A transoral ultrasound probe for imaging a temporomandibular joint, comprising:

a handle section having a longitudinal axis, the handle section being configured for connection to a power source; and

an intraoral section having a cephalad angulation such that the intraoral section is positioned at an operative angle with respect to the longitudinal axis of the handle section, the intraoral section being configured to emit and receive sound waves,

wherein the operative angle of the intraoral section is an acute angle.
2. The transoral ultrasound probe of claim 1, wherein the operative angle is less than 45 degrees.
3. The transoral ultrasound probe of claim 1, wherein the operative angle is about 30 degrees.
4. The transoral ultrasound probe of claim 1, wherein the handle section has a longitudinal length and the intraoral section has a length that is about one-third shorter than the longitudinal length of the handle section.
5. The transoral ultrasound probe of claim 1, wherein the handle section has a first width and the intraoral section has a second width, and the second width is greater than the first width.
6. The transoral ultrasound probe of claim 5, wherein the handle section and the intraoral section have substantially the same thickness and the thickness is less than or equal to the first width.

7. The transoral ultrasound probe of claim 6, wherein the handle and intraoral sections define substantially flat side surfaces and the thickness extends between the side surfaces.
8. The transoral ultrasound probe of claim 7, wherein a distal end of the intraoral section is rounded.
9. The transoral ultrasound probe of claim 1, wherein the intraoral section includes a transducer aperture at a distal end thereof configured to emit and received the sound waves.
10. The transoral ultrasound probe of claim 1, wherein the handle section is connected to the power source via a power cable or the power source is at least one battery connected to the handle section.
11. The transoral ultrasound probe of claim 10, wherein the power source is either coupled to or is part of a control unit.
12. A method of imaging a temporomandibular joint using a transoral probe that has a handle section and an intraoral section with a cephalad angulation, comprising the steps of:
- holding the handle section of the transoral probe;
- inserting the intraoral section of the transoral probe into a patient's mouth in a recess between the cheek and gum such that a transducer aperture of the intraoral section generally faces the temporomandibular joint; and
- emitting and receiving sound waves via the transducer aperture on the intraoral section of the transoral probe thereby producing images of the temporomandibular joint in at least the sagittal anatomical plane.
13. The method of claim 12, wherein the step of emitting and receiving sound waves produces images of the temporomandibular joint in all anatomical planes, including the axial, coronal, and sagittal planes.

14. The method of claim 12, further comprising the step of controlling the amplitude, frequency, and duration of the sound waves emitted from the transducer aperture of the transoral probe.
15. The method of claim 12, further comprising the step of connecting the transoral probe to a power source.
16. The method of claim 12, wherein the intraoral section of the transoral probe is positioned at an operative angle with respect to a longitudinal axis of the handle section, and the operative angle is an acute angle.
17. The method of claim 16, wherein the operative angle of the intraoral section is about 30 degrees.
18. The method of claim 12, wherein the handle and intraoral sections define substantially flat side surfaces and a thickness that extends between the side surfaces.
19. The method of claim 18, wherein the handle section has a first width and the intraoral section has a second width that is larger than the first width.
20. The method of claim 12, wherein a distal end of the intraoral section of the transoral probe is rounded.

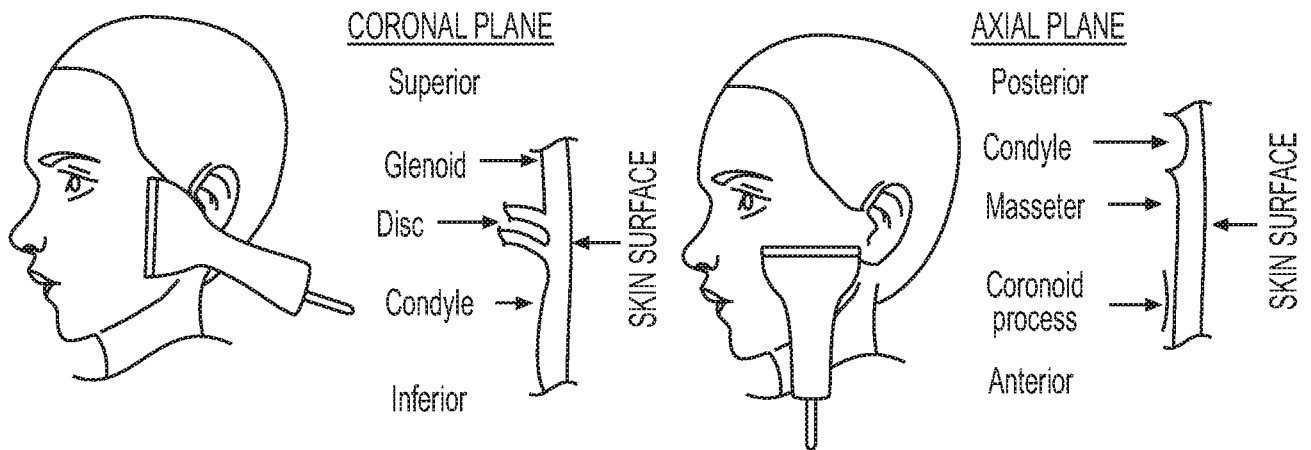


FIG. 1
PRIOR ART

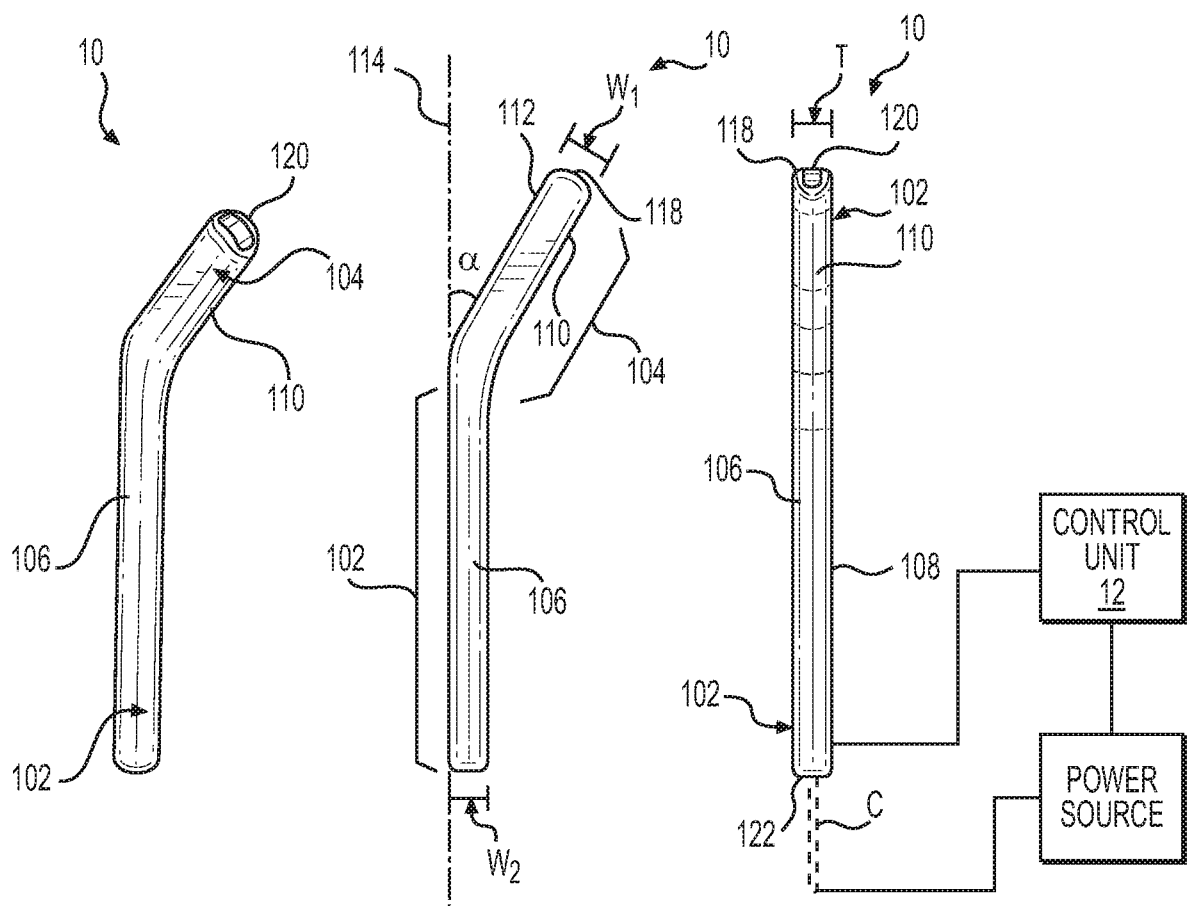


FIG. 2A

FIG. 2B

FIG. 2C

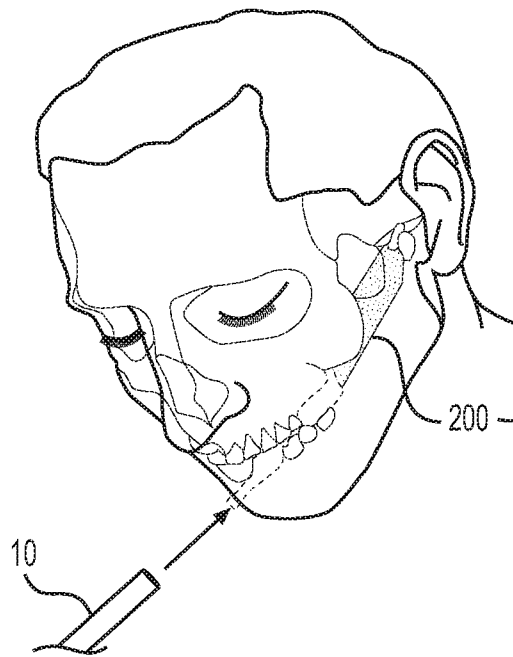


FIG. 3A

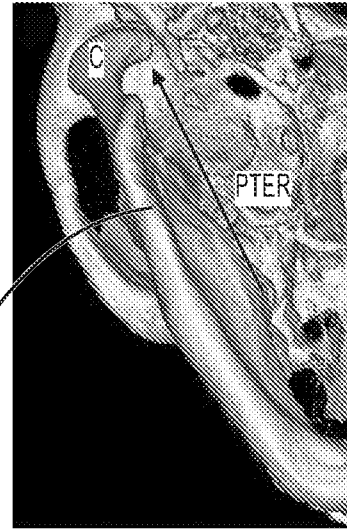


FIG. 3B

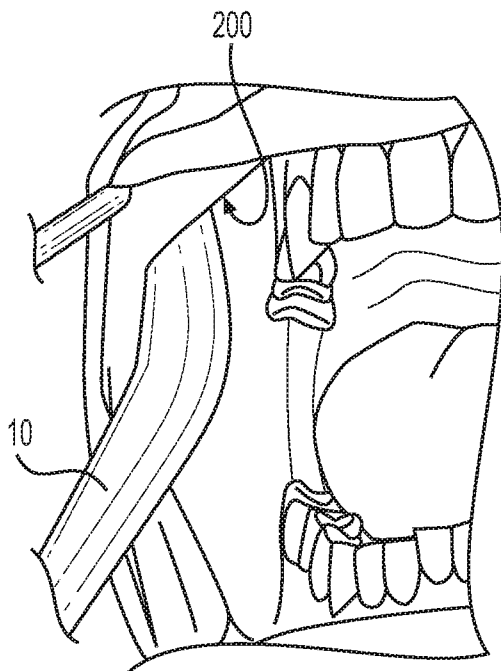


FIG. 3C

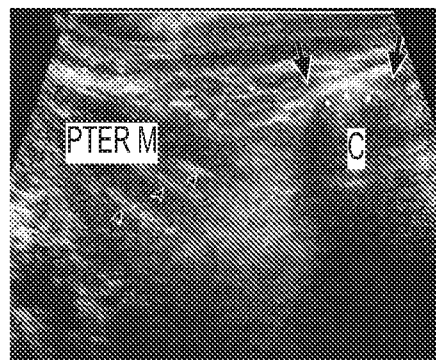


FIG. 4

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US18/38788

A. CLASSIFICATION OF SUBJECT MATTER

IPC - A61B 8/00, 8/12, 8/13, 8/14 (2018.01)

CPC - A61B 5/4542, 8/00, 8/0875, 8/12, 8/13, 8/14, 8/145, 8/44, 8/4455

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X -- Y	US 2015/03/4331 A1 (CHU, W-J et al.) 31 December 2015, figures 1-2, paragraphs [0015], [0042], [0045], [0047]	1-4 --- 5-8
X	US 5,779,639 A (YEUNG, HK) 14 July 1998; figure 1; column 4, lines 14-33, 53-65; column 5, lines 10-17	1-3, 9-11
Y	US 5,931,788 A (KEEN, RR et al.) 03 August 1999; figures 1-2; column 3, lines 63-67	5-8
A	US 2004/0143186 A1 (ANISIMOV, V et al.) 22 July 2004; paragraphs [0101], [0106]	12-20
A	US 2010/0198069 A1 (KAFAI EL-KHORASSANI, H) 05 August 2010; figure 3; paragraph [0016]	12-20
A	US 2013/0060144 A1 (CULJAT, M et al.) 07 March 2013; figure 3; paragraph [0042]	12-20
A	US 5,690,113 A (SLIWA, JW et al.) 25 November 1997; entire document	1-20



Further documents are listed in the continuation of Box C.



See patent family annex.

*

Special categories of cited documents:

"A"

document defining the general state of the art which is not considered to be of particular relevance

"E"

earlier application or patent but published on or after the international filing date

"L"

document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O"

document referring to an oral disclosure, use, exhibition or other means

"P"

document published prior to the international filing date but later than the priority date claimed

"T"

later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X"

document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y"

document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&"

document member of the same patent family

Date of the actual completion of the international search

14 August 2018 (14.08.2018)

Date of mailing of the international search report

31 AUG 2018

Name and mailing address of the ISA/

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents

P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Shane Thomas

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774

专利名称(译)	经鼻超声探头和使用方法		
公开(公告)号	EP3641655A1	公开(公告)日	2020-04-29
申请号	EP2018820272	申请日	2018-06-21
[标]发明人	KATZBERG RICHARD W		
发明人	KATZBERG, RICHARD W.		
IPC分类号	A61B8/00 A61B8/12 A61B8/13 A61B8/14		
CPC分类号	A61B8/0875 A61B8/12 A61B8/4281 A61B8/4444 A61B8/4209 A61B18/1477		
优先权	62/524196 2017-06-23 US		
外部链接	Espacenet		

摘要(译)

用于对颞下颌关节进行成像的经口超声探头以及使用经口腔探头对颞下颌关节进行成像的方法。