

(19)



(11)

EP 2 663 237 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

31.12.2014 Bulletin 2015/01

(51) Int Cl.:

A61B 6/12 (2006.01)

A61B 8/08 (2006.01)

(86) International application number:

PCT/IB2012/050109

(21) Application number: **12701029.6**

(22) Date of filing: **10.01.2012**

(87) International publication number:

WO 2012/095784 (19.07.2012 Gazette 2012/29)

(54) VISUALIZATION OF CATHETER IN THREE-DIMENSIONAL ULTRASOUND

VISUALISIERUNG EINES KATHETERS IN DREIDIMENSIONALEM ULTRASCHALL

VISUALISATION DE CATHÉTER EN ÉCHOGRAPHIE TRIDIMENSIONNELLE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **13.01.2011 US 201161432327 P**

(43) Date of publication of application:

20.11.2013 Bulletin 2013/47

(73) Proprietor: **Koninklijke Philips N.V.**

5656 AE Eindhoven (NL)

(72) Inventors:

- **YAN, Pingkun**
NY 10510 (US)

- **PARTHASARATHY, Vijay**

NY 10510 (US)

- **MANZKE, Robert**

NY 10510 (US)

- **JAIN, Ameet Kumar**

NY 10510 (US)

(74) Representative: **Steffen, Thomas**

Philips

Intellectual Property & Standards

P.O. Box 220

5600 AE Eindhoven (NL)

(56) References cited:

WO-A1-2005/092198 DE-A1- 10 210 648

US-A1- 2001 029 334 US-A1- 2003 199 748

US-A1- 2009 136 103 US-B1- 6 389 104

EP 2 663 237 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention generally relates to accurate image guidance for an interventional procedure, particularly an interventional cardiac procedure. The present invention specifically relates to visualization of an interventional tool (e.g., a catheter) in an ultrasound image ("3D US").

[0002] Knowing a relative position of an interventional tool (e.g., a catheter) with respect to a pre-procedural planning scan (e.g., a magnetic resonance imaging ("MRI") scan or a computed tomography ("CT") scan) is important for accurate guidance in an interventional procedure, particularly an interventional cardiac procedure. Since X-ray fluoroscopic images provide very highly resolved images of the interventional tool during the procedure, image-guided systems known in the art for providing visual aid in guiding the interventional tool have concentrated on tracking a tip of the tool in fluoroscopic images and overlaying in the pre-procedural scan. It is also well known, for visualization of a 3D shape of the interventional tool in real time, to mount a multitude of position sensors and/or shape sensing sensors on the interventional tool in order to track the 3D shape of the interventional tool.

[0003] Increasingly, registering an ultrasound image ("2D US") or 3D US with X-ray imaging has augmented X-ray fluoroscopy as an aid for guiding an interventional procedure. The key role of the 2D US or the 3D US is to augment the pre-procedural scan with real time motion information, while the X-ray fluoroscopic image(s) provide high resolution visualization of the interventional tool in real time. Moreover, with the introduction of 3D US in real time, it is becoming possible to visualize the interventional tool more clearly in ultrasound, thereby enabling ultrasound-only guided interventions.

[0004] In cardiac interventional procedures, it is important to visualize the tip of a catheter as well as the orientation of the tip of the catheter. The identification of the catheter tip is difficult in 3D US, especially in a cardiac interventional setting. Therefore, methods for identifying the catheter tip in X-ray images and mapping these points into 3D US for extraction and fusing in a pre-procedural scan is beneficial for the interventional procedure.

[0005] One form of the present invention is defined in claims 1 and 7.

[0006] A second form of the present invention is defined in claim 12.

[0007] The foregoing forms and other forms of the present invention as well as various features and advantages of the present invention will become further apparent from the following detailed description of various exemplary embodiments of the present invention read in conjunction with the accompanying drawings. The detailed description and drawings are merely illustrative of the present invention rather than limiting, the scope of the present invention being defined by the appended claims.

[0008] Document DE10210648 A1 discloses a system, device and method according to the preambles of claims 1, 7 and 12 respectively.

FIG. 1 illustrates an exemplary embodiment of an image-guided system in accordance with present invention.

FIG. 2 illustrates a flowchart representative of an image-guided method in accordance with the present invention.

FIG. 3 illustrates an exemplary implementation of the image-guided method of FIG. 2 by the image-guided system of FIG. 1.

FIGS. 4-6 illustrate various embodiments of a tool tracking device in accordance with the present invention.

FIG. 7 illustrates an exemplary geometric relationship between an X-ray image and an ultrasound image in accordance with the present invention.

FIG. 8 illustrates an exemplary tool tip movement within an ultrasound image in accordance with the present invention.

FIG. 9 illustrates a flowchart representative of one embodiment of a cardiac interventional procedure incorporating one embodiment of a tool tracking method in accordance with the present invention.

FIG. 10 illustrates a flowchart representative of a second embodiment of a tool tracking method in accordance with the present invention.

FIG. 11 illustrates a flowchart representative of one embodiment of a tool localization method in accordance with the present invention.

FIG. 12 illustrates a flowchart representative of one embodiment of a weighted graph construction method in accordance with the present invention.

FIG. 13 illustrates an exemplary weighted graph corresponding to an energy function in accordance with the present invention.

FIG. 14 illustrates a flowchart representative of one embodiment of an image segmentation method in accordance with the present invention.

[0009] As previously stated, the present invention provides various methods for visualizing a three-dimensional shape of the interventional tool in real time inside of a three-dimensional pre-procedural planning scan. As will be appreciated by those having ordinary skill in the art from the following descriptions of FIGS. 1-13, these methods are implemented by a tool tracking device of the present invention utilizing X-ray images and ultrasound images. For purposes of facilitating

an understanding of the present invention, the tool tracking device will be described herein for tracking a catheter during a cardiac interventional procedure.

[0010] Specifically, FIG. 1 illustrates an image-guiding system employing an X-ray imaging system, a 3D US imaging system and a tool tracking device in the form of a catheter tracking device 50.

[0011] For purposes of the present invention, the X-ray imaging system is broadly defined herein as including an X-ray imaging device 20 for controlling an operation of an X-ray source 21 and an X-ray detector 22 structurally configured for generating a X-ray image ("XRI") 25 of an anatomical region (e.g., a cardiac region) represented by a volume 40 and/or for controlling an operation of an X-ray source 23 and an X-ray detector 24 structurally configured for generating a X-ray image ("XRI") 26 of anatomical region 40. In practice, components 20-22 exclusive of components 23 and 24 represent a monoplane X-ray system of any type, and components 21-24 collectively represent a bi-plane X-ray system of any type. Examples of the X-ray imaging system include, but are not limited to, any type of X-ray system for performing a cardiac interventional procedure. In one embodiment, an X-ray system from the Allure Xper series commercially sold by Philips Medical Systems may serve as the X-ray imaging system.

[0012] For purposes of the present invention, the 3D US imaging system is broadly defined herein as including 3D US imaging device 30 for controlling an operation of 3D US probe 31 structurally configured for generating an ultrasound image ("USI") 32 of anatomical region 40. Examples of the 3D US imaging system include, but are not limited to, any type of ultrasound imaging system, particularly one utilizing a 3D TEE probe. In one embodiment, the iEEE intelligent echo system commercially sold by Philips Medical Systems may serve as 3D US imaging system.

[0013] For purposes of the present invention, catheter tracking device 50 is broadly defined herein as any device structurally configured for registering X-ray image(s) 25/26 and ultrasound image 32 for purposes of identifying a tip of a catheter 41 within anatomical region 40, and for visualizing a 3D shape of catheter 41 in real time inside of a 3D pre-procedural planning scan inclusive of anatomical region 40. To this end, catheter tracking device 50 executes an image-guided method represented by a flowchart 60 as shown in FIG. 2.

[0014] Referring to FIG. 2, a stage S61 of flowchart 60 encompasses a pre-operative planning of an interventional procedure involving a 3D scan (e.g., a MRI scan or a CT scan) of an anatomical region of a patient. For example, as shown in FIG. 3, stage S61 may encompass a 3D pre-procedural scan 72 of a cardiac region 71 of a patient 70 and a storage of 3D pre-procedural scan 72 within a database 73.

[0015] A stage S62 of flowchart 60 encompasses a registration by catheter tracking device 50 of X-ray image(s) and an ultrasound image of the anatomical region of the patient. For example, as shown in FIG. 3, X-ray image 25 and/or X-ray image 26 of cardiac region 71 as well as ultrasound image 32 of cardiac region 71 are generated by the X-ray imaging system and the 3D US imaging system, respectively, whereby catheter tracking device 50 registers X-ray image 25 and/or X-ray image 26 to ultrasound image 31. In practice, the registration may be involved a conversion of X-ray coordinates into 3D US real-time coordinates using a combination of system calibration and real-time tracking as known in the art. For example, the registration may include manual alignment or an electromagnetic tracking technique.

[0016] A stage S63 of flowchart 60 encompasses an identification of a portion of the catheter (e.g., a tip of the catheter) within the ultrasound image. In one embodiment as related to FIG. 3, stage S63 involves an automatic or a manual identification of the tip of catheter 41 within X-ray image 25 and/or X-ray image 26 and a localization of the tip of catheter 41 within ultrasound image 32 derived the X-ray/3D US registration as known in the art.

[0017] A stage S64 of flowchart 60 encompasses an image segmentation of catheter 41 within ultrasound image 32 with the catheter tip serving as an initialization point for the image segmentation process.

[0018] A stage S65 of flowchart 60 encompasses a tracking of the catheter within a pre-procedural scan of the anatomical region derived from the image segmentation of the 3D shape of the catheter within the ultrasound image. For example, as shown in FIG. 3, stage S65 involves catheter tracking device 50 displaying 3D pre-procedural scan 72 on a display 80 with a tracking overlay 75 of catheter 41 projected within scan 72 as derived from previous image segmentation of the 3D shape of catheter 41 within the ultrasound image 32.

[0019] A description of FIGS. 4-13 will now be provided herein to provide a detailed explanation of various embodiments of a catheter tracking device of the present invention including modules structurally configured with hardware, software and/or firmware for implementing stages S63 and S64 of flowchart 60 (FIG. 2).

[0020] Specifically, FIG. 4 illustrates a catheter image tracking module 51a for implementing stages S63 and S64 in accordance with a process known herein as "tip detection mode" in view of the fact the manner by which the tip is detected may serve as a boundary constraint for subsequent image segmentation.

[0021] Generally, the "tip detection mode" utilizes a geometric relationship of an X-ray image and an ultrasound volume whereby a tool tip in the X-ray image corresponds to a line or a line set going through the ultrasound image after transformation using an X-ray/3D US registration. For example, as shown in FIG. 7, an X-ray projection 90 of a catheter 41 onto X-ray detector 22 via X-ray source 21 corresponds to a line set 91 of three (3) lines going through an ultrasound volume 33 after transformation using an X-ray/3D US registration. By using the illustrated geometric constraint, a six (6) degree of freedom ("DOF") catheter tracking problem $[x, y, z, a, b, c]$, where xyz are translations and a, b , and c are rotations, is reduced into a four (4) DOF problem with $[r, a, b, c]$, where r is a translation along a tracing line 92 associated

with the catheter tip shown in FIG. 7. In practice, this catheter tracking problem may be efficiently solved by using a Kalman filter or particle filter based visual tracker, which has been extensively studied in computer vision. The reduction of search space to four (4) DOF significantly improves the step of the visual tracking algorithms as described below.

[0022] For example, a particle filter is used to illustrate how to build the catheter tracking module 51. Specifically, let $X = [r, a, b, c]$ denote the state vector representing the location and the pose of catheter 41. The catheter tracking problem may be described by i.e., to estimate state vector X using the ultrasound volume history. By using Bayes' rule, the following equation [1] is derived for tracking purposes:

$$p(X_t | \mathbf{V}_{us}^t) = p(\mathbf{V}_{us}^t | X_t) \int p(X_t | X_{t-1}) p(X_{t-1} | \mathbf{V}_{us}^{t-1}) dX_{t-1} \quad [1]$$

[0023] By assuming the dynamic change from X_{t-1} to X_t as shown in FIG. 8 from a point 93 to a point 94 in 3D US volume 33 follows some distribution $p(X_t | X_{t-1})$, the particles sampled from the previous 3D US volume $p(X_{t-1} | \mathbf{V}_{us}^{t-1})$ may be propagated to the next frame, where the fitness of an estimated tool tip to the current 3D US frame is measured by $p(\mathbf{V}_{us}^t | X_t)$. By applying the geometric constraint from a single X-ray image 25 as shown in FIG. 8, the number of variables in the state vector X is reduced from six (6) to (4), which in turn reduces the number of samples used in the particle filter and shortens the tracking time by one-third (1/3) for an equivalent tracking accuracy compared to the unconstrained tracking in 3D US. In other words, with the same computational time, the proposed scheme can use more samples to make the catheter visualization in 3D US volume 33 more accurate and more robust.

[0024] FIG. 9 illustrates a flowchart 100 representative of a cardiac interventional procedure incorporating the "tip detection mode" of the present invention via a tracking loop including stages S104-S106 of flowchart 100.

[0025] Specifically, stage S104 encompasses a generation of a single X-ray image of the heart cavity during a 3D US probe of the heart cavity. The single X-ray image is utilized by tool identification module 52a during stage S105 to identify the tip of the catheter in an ultrasound image of the heart cavity in one time phase or ECG phase.

[0026] In one embodiment of stage S105, the tip of the catheter is manually identified in a ultrasound image via a user input of the 3D US imaging system and a line extending from the X-ray source through 3D US volume to the catheter tip as projected on the X-ray detector is determined. In a second embodiment of stage S105, the tip of the catheter is manually identified in the X-ray image via a user input of the X-ray image system and then mapped to the ultrasound image based on the X-ray/3D US registration. Additionally, a line extending from the X-ray source through 3D US volume to the catheter tip as projected on the X-ray detector is determined.

[0027] In a third embodiment of stage S105, the tip of the catheter is automatically identified in the X-ray image via a known template matching algorithm and then mapped to the ultrasound image based on the X-ray/3D US registration. Again, a line extending from the X-ray source through 3D US volume to the catheter tip as projected on the X-ray detector is determined.

[0028] In a fourth embodiment of stage S105, the catheter tip may be automatically detected in the ultrasound image using learning based techniques, where the appearance model can come from manual identification of catheter tip in sample 3D US images or from biplane X-ray images. In this appearance modelling process, 3D image patches are first extracted from the training 3D US volumes around the identified catheter tip. Each patch is reshaped into a vector and may be considered as a column of a matrix M . The singular value decomposition ("SVD") may be applied to the constructed matrix to extract the principal components U of the training patches. That is $M = U \Sigma V^T$.

[0029] During the detection process, the search is performed along the line back projected from the identified catheter tip in X-ray image to the 3D US volume. For each search location, a patch I_p with the same size as the training patch is extracted. The patch can then be decomposed into $b = U^T I_p$ and the distance from the patch to the learned model is measured by $\|b\|^2$. The catheter tip location may be detected as the point with the smallest distance.

[0030] Stage S106 encompasses image segmentation module 53a visualizing the 3D shape of the catheter within the ultrasound image. In practice, the present invention does not impose any restrictions or limitations to the segmentation of the catheter for visualization purposes. Nonetheless, during stage S106, the back-projected line or line set may serve as a boundary constraint for the catheter segmentation in the ultrasound image, i.e. the catheter tip has to be located somewhere along this line or line set. The catheter segmentation may be further constraint by the dimensions of the ultrasound image. Additionally, a priori knowledge of the catheter shape may be further used to determine statistically likely poses given the before mentioned boundary conditions.

[0031] One advantage of the execution of the tracking loop stages S104-S106 is the use of a monoplane X-ray imaging system.

[0032] Referring to on overall execution of flowchart 100, a stage S101 of flowchart 100 encompasses an insertion of

a catheter into a heart cavity. Upon the insertion, a 3D US probe (e.g., probe 31 shown in FIG. 1) is utilized to selectively trigger the tracking loop as needed. Specifically, if the 3D US probe illustrates the catheter is at the heart wall and on target, then flowchart 100 from stage S101 through stages S102 and S103 to termination. Otherwise, if the 3D US probe illustrates the catheter is not at the heart wall during stage S102, then tracking loop stages S104-S106 are executed. Alternatively, if the 3D US probe illustrates the catheter is not on target at the heart wall during stage S103, then the catheter is retracted during a stage S107 prior to an execution of tracking loop stages S104-S106.

[0033] FIG. 5 illustrates a catheter image tracking module 51b for implementing stages S63 and S64 (FIG. 2) in accordance with a process known herein as "graph-cut segmentation mode" in view of the fact the manner by which catheter is segmented is based on a graph-cut method.

[0034] Generally, the "graph-cut segmentation mode" implements a flowchart 110 shown in FIG. 10 involving a catheter tip location in 3D US volume space during a stage S111 and a catheter segmentation in 3D US volume space during a stage S112.

[0035] In one embodiment of stage S111, the catheter tip may be manually identified in the 3D US volume space.

[0036] In a more reliable second embodiment of stage S111, a flowchart 120 representative of a catheter tip localization method of the present invention as shown in FIG. 11 is executed.

[0037] Referring to FIG. 11, upon the catheter being inserted within an anatomical region, a stage S121 of flowchart 120 encompasses an X-ray image acquisition of the catheter at a 1st gantry angle during a specified cardiac phase (e.g., an end diastole phase) and a specified respiratory phase (e.g., an end respiratory phase) using known cardiac and respiratory gating techniques and a stage S122 of flowchart 120 encompasses a manual or automatic segmentation of the catheter tip in the X-ray image acquired during stage S121.

[0038] For a monoplane X-ray imaging system, a stage S123 of flowchart 120 encompasses an X-ray image acquisition of the catheter at a 2nd gantry angle during the same specified cardiac phase and the same specified respiratory phase using known cardiac and respiratory gating techniques and a stage S124 of flowchart 120 encompasses a manual or automatic segmentation of the catheter tip in the X-ray image acquired during stage S123.

[0039] For a biplane X-ray imaging system, stages S121/S122 and stages S123/S124 may be executed simultaneously.

[0040] For either X-ray imaging system, a corresponding 3D location of the catheter tip in the 2D X-ray coordinate system is reconstructed during a stage S125 of flowchart 120. In one embodiment of stage S125, a known epipolar constraint is utilized to reconstruct the 3D location of the catheter tip in the 2D X-ray coordinate system.

[0041] Thereafter, during a stage S126 of flowchart 120, a reconstructed 2D X-ray coordinate location of the catheter tip is converted into a 3D US real-time coordinate location using system calibration and real-time tracking. In one embodiment of stage S126, a manual alignment is used as the basis for the conversion. In a second embodiment of stage S126, a known electromagnetic tracking technique is used as the basis for the conversion.

[0042] Referring back to FIG. 10, flowchart 120 facilitates an execution of a flowchart 150 (FIG. 14) during stage S112.

[0043] Flowchart 150 is premised on a minimization of the following energy functional [2]:

$$\{x_p\} = \min_{\{x_p\}} \sum_p D_p(x_p) + \sum_{p \sim q} w_{pq} [x_p \neq x_q] \quad [2]$$

where x_p is the label of the pixel p and $p \sim q$ indicates that the pixel p and q are neighbors. The first term of the energy functional $D_p(x_p)$ describes the cost of assigning a pixel to foreground or to background based on its label. The cost of assigning a pixel to the foreground is chosen as the absolute difference between the filter response f_p at that pixel and the minimum filter response ε of the image. This cost gets its minimum value at the pixels inside the catheter as the filter that highlights the catheter gives its lowest response at those pixels. In a similar way, the cost of assigning a pixel to background is chosen as the absolute difference between the filter response f_p at that pixel and the mean filter response μ of the image.

[0044] On the other hand, the second pair wise part works as a regularization term. When two neighboring pixels p and q , have different labels x_p and x_q , the predicate $[x_p \neq x_q]$ takes the value 1 and w_{pq} accumulates to the energy, otherwise it takes the value 0 and w_{pq} has no contribution to the energy. As a natural choice for w_{pq} that favors the assignment of the same label to the nearby pixels with similar filter response, the similarity measure $w_{pq} = e^{-B|f_p - f_q|}$ may be utilized.

[0045] To find the global minimum of equation [2], a flowchart 130 as shown in FIG. 12 is executed for constructing a weighted graph, such as, for example, a weighted graph 140 shown in FIG. 13. Referring to FIGS. 12 and 13, a stage S131 of flowchart 130 encompasses a construction of a node to the graph for each pixel. As this is a binary optimization problem, a stage S132 of flowchart 130 encompasses an addition of two (2) terminal nodes s and t representing background and foreground, respectively. Next, a stage S133 of flowchart 130 encompasses a connection of terminal

node s to each node representing pixels and assignment of the weight, and a connection of terminal node t to, each node and assignment of the weight $|f_p - \mu|$ to those edges. Finally, a stage S134 of flowchart 130 encompasses an addition of edges that connect the nodes representing neighboring pixels, and assignment of the weight w_{pq} to the edges.

[0046] Referring now to FIG. 14, flowchart 150 is executed for segmenting the catheter in the 3D US volume space. Specifically, a localized tool tip in 3D US volume space as determined by flowchart 120 (FIG. 11) is utilized as the initial seed point and a stage S151 of flowchart 150 encompasses a generation of a small neighborhood around the identified tool tip to compute a probability distribution function (PDF) of the catheter intensity. Next, a stage S152 of flowchart 150 encompasses a computation of the term $D_p(x_p)$ for equation [2] to assign the weight to each terminal link for purposes of constructing the weighted graph, and a stage S153 of flowchart 150 encompasses an application of a graph-cut to the constructed graph to obtain an initial segmentation.

[0047] The initial segmentation may not be ideal, because not only the catheter itself but also some other structure around it with similar appearance may be included into the segmentation. Thus, a stage S154 of flowchart 150 encompasses an application of a catheter shape filter to refine the initial segmentation. The catheter shape filter is designed to exploit the tubular structure of the catheter and may be a 2nd derivative of 2D Gaussian kernel with 3D orientation in the design. In one embodiment, an orientation of the filter is set by computing the principal direction of the initial segmentation.

[0048] Upon completion of stage S154, a stage S155 of flowchart 150 encompasses a construction of a new 3D graph the same manner as stage S152. A final catheter segmentation is done by applying graph-cut again on this new graph during a stage S156 of flowchart 150.

[0049] From the description of FIGS. 7-14, those having ordinary skill in the art will appreciate the "tip detection mode" and the "graph-cut segmentation mode" of catheter tracking device 51a (FIG. 4) and catheter tracking device 51b (FIG. 5), respectively. FIG. 6 illustrates a catheter image tracking module 51c for implementing stages S63 and S64 in accordance with a combination of "tip detection mode" as executed by a tool detection module 52c and the "graph-cut segmentation mode" as executed by the image segmentation module 53c.

[0050] From the description of FIGS. 1-14, those having skill in the art will have a further appreciation on how to implement a tool tracking method for any application in accordance with the present invention.

[0051] In practice, any number of X-ray imaging device 20, 3D US imaging device 30 and a tool tracking device may be integrated into a single device.

[0052] While various exemplary embodiments of the present invention have been illustrated and described, it will be understood by those skilled in the art that the exemplary embodiments of the present invention as described herein are illustrative. Therefore, it is intended that the present invention not be limited to the particular embodiments disclosed as the best mode contemplated for carrying out the present invention, but that the present invention includes all embodiments falling within the scope of the claims.

Claims

1. An image-guided system, comprising:

an X-ray imaging device (20) for generating at least one X-ray image (25, 26) illustrating a tool (41) within an anatomical region (40);
an ultrasound imaging device (30) for generating an ultrasound image (32) illustrating the tool (41) within the anatomical region (40); and
a tool tracking device (50) for tracking the tool (41) within the anatomical region (40),

wherein the tool tracking device (50) is operable to localize a portion of the tool (41) as located within the ultrasound image (32) based on an identification of the portion of the tool (41) as located within the at least one X-ray image (25, 26) and is **characterised in that** the tool tracking device is operable to localize said portion of the tool by localizing the portion of the tool (41) along at least one line extending from an X-ray source (21) to an X-ray detector (22) through an ultrasound volume (33) after registration of the ultrasound image (32) with the X-ray image (25, 26), and

wherein the tool tracking device (50) is further operable to execute an image segmentation of an entirety of the tool (41) as located within the ultrasound image (32) relative to a localization of the portion of the tool (41) as located within the ultrasound image (32).

2. The image-guided system of claim 1, wherein the tool (41) is a catheter, and wherein a portion of the tool (41) is a tip of the tool (41).

3. The image-guided system of claim 1, wherein the X-ray imaging device (20) is one of a group including a monoplane X-ray imaging device and a bi-plane X-ray imaging device.

5 4. The image-guided system of claim 1, wherein the at least one line serves as at least one boundary constraint for an execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32).

5. The image-guided system of claim 1, wherein an execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32) relative to the localization of the portion of the tool (41) as located within the ultrasound image (32) includes:

10 constructing an initial weighted energy graph (140); and
executing a graph-cut segmentation of the initial weighted energy graph (140).

15 6. The image-guided system of claim 5, wherein the execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32) relative to the localization of the portion of the tool (41) as located within the ultrasound image (32) further includes:

20 applying a shape filter to the graph-cut segmentation of the initial weighted energy graph (140);
constructing a final weighted energy graph (140) as a function of the application of the shape filter to the graph-cut segmentation of the initial weighted energy graph (140); and
executing a graph-cut segmentation of the final weighted energy graph (140).

25 7. A tool tracking device (50) for tracking a tool (41) within an anatomical region (40), the tool tracking device (50) comprising:

30 a tool (41) identification module (51, 51a, 51b, 51c, 52a) operable to localize a portion of the tool (41) as located within an ultrasound image (32) illustrating the tool (41) within the anatomical region (40) based on an identification of the portion of the tool (41) as located within the at least one X-ray image (25, 26) illustrating the tool (41) within the anatomical region (40) **characterised in that** the tool identification module is operable to localize said portion of the tool by localizing the portion of the tool (41) along at least one line extending from an X-ray source (21) to an X-ray detector (22) through an ultrasound volume (33) after registration of the ultrasound image (32) with the X-ray image (25, 26), and
an image segmentation module operable to execute an image segmentation of an entirety of the tool (41) as located within the ultrasound image (32) relative to a localization of the portion of the tool (41) as located within the ultrasound image (32).

8. The tool tracking device (50) of claim 7, wherein the tool (41) is a catheter, and wherein a portion of the tool (41) is a tip of the tool (41).

40 9. The tool tracking device (50) of claim 7, wherein the at least one line serves as at least one boundary constraint for an execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32).

45 10. The tool tracking device (50) of claim 7, wherein an execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32) relative to the localization of the portion of the tool (41) as located within the ultrasound image (32) further includes:

constructing an initial weighted energy graph (140); and
executing a graph-cut segmentation of the initial weighted energy graph (140).

50 11. The tool tracking device (50) of claim 10, wherein the execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32) relative to the localization of the portion of the tool (41) as located within the ultrasound image (32) further includes:

55 applying a shape filter to the graph-cut segmentation of the initial weighted energy graph (140);
constructing a final weighted energy graph (140) as a function of the application of the shape filter to the graph-cut segmentation of the initial weighted energy graph (140); and
executing a graph-cut segmentation of the final weighted energy graph (140).

12. An image-guided method for tracking a tool (41) within an anatomical region (40), comprising:

generating at least one X-ray image (25, 26) illustrating the tool (41) within an anatomical region (40);
 generating an ultrasound image (33) illustrating the tool (41) within the anatomical region (40);
 localizing a portion of the tool (41) as located within the ultrasound image (32) based on an identification of the
 portion of the tool (41) as located within the at least one X-ray image (25, 26) **characterised by** said localizing
 said portion of the tool being done by localizing the portion of the tool (41) along at least one line extending
 from an X-ray source (21) to an X-ray detector (22) through an ultrasound volume (33) after registration of the
 ultrasound image (32) with the X-ray image (25, 26); and
 executing an image segmentation of an entirety of the tool (41) as located within the ultrasound image (32)
 relative to a localization of the portion of the tool (41) as located within the ultrasound image (32).

13. The image-guided method of claim 12, wherein the at least one line serves as at least one boundary constraint for
 an execution of the image segmentation of the entirety of the tool (41) as located within the ultrasound image (32).

14. The image-guided method of claim 12, wherein an execution of the image segmentation of the entirety of the tool
 (41) as located within the ultrasound image (32) relative to the localization of the portion of the tool (41) as located
 within the ultrasound image (32) further includes:

constructing an initial weighted energy graph (140); and
 executing a graph-cut segmentation of the initial weighted energy graph (140).

15. The image-guided method of claim 14, wherein the execution of the image segmentation of the entirety of the tool
 (41) as located within the ultrasound image (32) relative to the localization of the portion of the tool (41) as located
 within the ultrasound image (32) further includes:

applying a shape filter to the graph-cut segmentation of the initial weighted energy graph (140);
 constructing a final weighted energy graph (140) as a function of the application of the shape filter to the graph-
 cut segmentation of the initial weighted energy graph (140); and
 executing a graph-cut segmentation of the final weighted energy graph (140).

Patentansprüche

1. Bildgeführtes System, das Folgendes umfasst:

eine Röntgenbildgebungsvorrichtung (20) zum Erzeugen von mindestens einem Röntgenbild (25, 26), das ein
 Instrument (41) innerhalb einer anatomischen Region (40) darstellt;
 eine Ultraschallbildgebungsvorrichtung (30) zum Erzeugen eines Ultraschallbilds (32), das das Instrument (41)
 innerhalb der anatomischen Region (30) darstellt; und
 eine Instrumentverfolgungsvorrichtung (50) zum Verfolgen des Instruments (41) innerhalb der anatomischen
 Region (40),

wobei die Instrumentverfolgungsvorrichtung (50) betriebsfähig ist, um einen Teil des Instruments (41), wie er inner-
 halb des Ultraschallbilds (32) lokalisiert wurde, basierend auf einer Identifikation des Teils des Instruments (41),
 wie er innerhalb des mindestens einen Röntgenbilds (25, 26) lokalisiert wurde, zu lokalisieren, und **dadurch ge-
 kennzeichnet ist, dass** die Instrumentverfolgungsvorrichtung betriebsfähig ist, um den genannten Teil des Instru-
 ments zu lokalisieren, indem sie den Teil des Instruments (41) entlang mindestens einer Linie, die von einer Rönt-
 genquelle (21) durch ein Ultraschallvolumen (33) zu einem Röntgendetektor (22) verläuft, nach der Registrierung
 des Ultraschallbilds (32) mit dem Röntgenbild (25, 26) lokalisiert, und
 wobei die Instrumentverfolgungsvorrichtung (50) weiterhin betriebsfähig ist, um eine Bildsegmentierung einer Ge-
 samtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu einer Lokali-
 sierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, durchzuführen.

2. Bildgeführtes System nach Anspruch 1, wobei das Instrument (41) ein Katheter ist, und wobei ein Teil des Instruments
 (41) eine Spitze des Instruments (41) ist.

3. Bildgeführtes System nach Anspruch 1, wobei die Röntgenbildgebungsvorrichtung (20) eine Vorrichtung aus einer

Gruppe ist, die eine Einebenen-Röntgenbildgebungsvorrichtung und eine Zweiebenen-Röntgenbildgebungsvorrichtung umfasst.

4. Bildgeführtes System nach Anspruch 1, wobei die mindestens eine Linie als mindestens eine Randbedingung für eine Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, dient.

5. Bildgeführtes System nach Anspruch 1, wobei die Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu der Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, Folgendes umfasst:

Konstruieren eines anfänglichen gewichteten Energiegraphen (140); und
Durchführen einer Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140).

6. Bildgeführtes System nach Anspruch 5, wobei die Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu der Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, weiterhin Folgendes umfasst:

Anwenden eines Formfilters auf die Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140);
Konstruieren eines endgültigen gewichteten Energiegraphen (140) als Funktion der Anwendung des Formfilters auf die Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140); und
Durchführen einer Graph-Cut-Segmentierung des endgültigen gewichteten Energiegraphen (140).

7. Instrumentverfolgungsvorrichtung (50) zum Verfolgen eines Instruments (41) innerhalb einer anatomischen Region (40), wobei die Instrumentverfolgungsvorrichtung (50) Folgendes umfasst:

ein Identifikationsmodul (51, 51a, 51b, 51c, 52a) für das Instrument (41), das betriebsfähig ist, um einen Teil des Instruments (41), wie er innerhalb eines Ultraschallbilds (32) lokalisiert wurde, das das Instrument (41) innerhalb der anatomischen Region (40) darstellt, basierend auf einer Identifikation des Teils des Instruments (41) zu lokalisieren, wie er innerhalb des mindestens einen Röntgenbilds (25, 26) lokalisiert wurde, das das Instrument (41) innerhalb der anatomischen Region (40) darstellt, **dadurch gekennzeichnet, dass** das Instrumentidentifikationsmodul betriebsfähig ist, um den genannten Teil des Instruments (41) zu lokalisieren,

indem es den Teil des Instruments (41) entlang mindestens einer Linie, die von einer Röntgenquelle (21) durch ein Ultraschallvolumen (33) zu einem Röntgendetektor (22) verläuft, nach der Registrierung des Ultraschallbilds (32) mit dem Röntgenbild (25, 26) lokalisiert, und
wobei ein Bildsegmentierungsmodul betriebsfähig ist, um eine Bildsegmentierung einer Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu einer Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, durchzuführen.

8. Instrumentverfolgungsvorrichtung (50) nach Anspruch 7, wobei das Instrument (41) ein Katheter ist und wobei der Teil des Instruments (41) eine Spitze des Instruments (41) ist.

9. Instrumentverfolgungsvorrichtung (50) nach Anspruch 7, wobei die mindestens eine Linie als mindestens eine Randbedingung für eine Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, dient.

10. Instrumentverfolgungsvorrichtung (50) nach Anspruch 7, wobei die Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu der Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, weiterhin Folgendes umfasst:

Konstruieren eines anfänglichen gewichteten Energiegraphen (140); und
Durchführen einer Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140).

11. Instrumentverfolgungsvorrichtung (50) nach Anspruch 10, wobei die Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu der Lokalisierung

des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, weiterhin Folgendes umfasst:

Anwenden eines Formfilters auf die Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140);
Konstruieren eines endgültigen gewichteten Energiegraphen (140) als Funktion der Anwendung des Formfilters auf die Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140); und
Durchführen einer Graph-Cut-Segmentierung des endgültigen gewichteten Energiegraphen (140).

12. Bildgeführtes Verfahren zum Verfolgen eines Instruments (41) innerhalb einer anatomischen Region (40), wobei das Verfahren Folgendes umfasst:

Erzeugen von mindestens einem Röntgenbild (25, 26), das das Instrument (41) innerhalb einer anatomischen Region (40) darstellt;
Erzeugen eines Ultraschallbilds (32), das das Instrument (41) innerhalb der anatomischen Region (40) darstellt;
Lokalisieren eines Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, basierend auf einer Identifikation des Teils des Instruments (41), wie er innerhalb des mindestens einen Röntgenbilds (25, 26) lokalisiert wurde, **dadurch gekennzeichnet, dass** das genannte Lokalisieren des genannten Teils des Instruments erfolgt, indem der Teil des Instruments (41) entlang mindestens einer Linie, die von einer Röntgenquelle (21) durch ein Ultraschallvolumen (33) zu einem Röntgendetektor (22) verläuft, nach der Registrierung des Ultraschallbilds (32) mit dem Röntgenbild (25, 26) lokalisiert wird; und
eine Bildsegmentierung einer Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu einer Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, durchgeführt wird.

13. Bildgeführtes Verfahren nach Anspruch 12, wobei die mindestens eine Linie als mindestens eine Randbedingung für eine Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, dient.

14. Bildgeführtes Verfahren nach Anspruch 12, wobei die Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu der Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, weiterhin Folgendes umfasst:

Konstruieren eines anfänglichen gewichteten Energiegraphen (140); und
Durchführen einer Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140).

15. Bildgeführtes Verfahren nach Anspruch 14, wobei die Durchführung der Bildsegmentierung der Gesamtheit des Instruments (41), wie es innerhalb des Ultraschallbilds (32) lokalisiert wurde, relativ zu der Lokalisierung des Teils des Instruments (41), wie er innerhalb des Ultraschallbilds (32) lokalisiert wurde, weiterhin Folgendes umfasst:

Anwenden eines Formfilters auf die Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140);
Konstruieren eines endgültigen gewichteten Energiegraphen (140) als Funktion der Anwendung des Formfilters auf die Graph-Cut-Segmentierung des anfänglichen gewichteten Energiegraphen (140); und
Durchführen einer Graph-Cut-Segmentierung des endgültigen gewichteten Energiegraphen (140).

Revendications

1. Système guidé par image, comprenant :

un dispositif d'imagerie à rayons X (20) pour générer au moins une image à rayons X (25, 26) illustrant un outil (41) à l'intérieur d'une région anatomique (40) ;
un dispositif d'imagerie à ultrasons (30) pour générer une image à ultrasons (32) illustrant l'outil (41) à l'intérieur de la région anatomique (40) ; et
un dispositif de suivi d'outil (50) pour assurer le suivi de l'outil (41) à l'intérieur de la région anatomique (40),

dans lequel le dispositif de suivi d'outil (50) est utilisable pour localiser une portion de l'outil (41) qui est située à

l'intérieur de l'image à ultrasons (32) sur la base d'une identification de la portion de l'outil (41) qui est située à l'intérieur de l'au moins une image à rayons X (25, 26), **caractérisé en ce que** le dispositif de suivi d'outil est utilisable pour localiser ladite portion de l'outil en localisant la portion de l'outil (41) le long d'au moins une ligne s'étendant à partir d'une source de rayons X (21) jusqu'à un détecteur de rayons X (22) à travers un volume d'ultrasons (33) après l'alignement de l'image à ultrasons (32) avec l'image à rayons X (25, 26), et dans lequel le dispositif de suivi d'outil (50) est en outre utilisable pour exécuter une segmentation d'image d'une intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à une localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32).

2. Système guidé par image selon la revendication 1, dans lequel l'outil (41) est un cathéter, et dans lequel une portion de l'outil (41) est une pointe de l'outil (41).

3. Système guidé par image selon la revendication 1, dans lequel le dispositif d'imagerie à rayons X (20) est l'un d'un groupe se composant d'un dispositif d'imagerie à rayons X à plan unique et d'un dispositif d'imagerie à rayons X à plan double.

4. Système guidé par image selon la revendication 1, dans lequel l'au moins une ligne sert d'au moins une contrainte de frontière pour une exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32).

5. Système guidé par image selon la revendication 1, dans lequel une exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à la localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) comprend :

la construction d'un graphique d'énergie pondérée initial (140) ; et
l'exécution d'une segmentation à découpage de graphique du graphique d'énergie pondérée initial (140).

6. Système guidé par image selon la revendication 5, dans lequel l'exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à la localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) comprend en outre :

l'application d'un filtre de forme à la segmentation à découpage de graphique du graphique d'énergie pondérée initial (140) ;

la construction d'un graphique d'énergie pondérée final (140) en fonction de l'application du filtre de forme à la segmentation à découpage de graphique du graphique d'énergie pondérée initial (140) ; et
l'exécution d'une segmentation à découpage de graphique du graphique d'énergie pondérée final (140).

7. Dispositif de suivi d'outil (50) pour assurer le suivi d'un outil (41) à l'intérieur d'une région anatomique (40), le dispositif de suivi d'outil (50) comprenant :

un module d'identification (51, 51a, 51b, 51c, 52a) d'outil (41) utilisable pour localiser une portion de l'outil (41) qui est située à l'intérieur d'une image à ultrasons (32) illustrant l'outil (41) à l'intérieur de la région anatomique (40) sur la base d'une identification de la portion de l'outil (41) qui est située à l'intérieur de l'au moins une image à rayons X (25, 26) illustrant l'outil (41) à l'intérieur de la région anatomique (40), **caractérisé en ce que** le module d'identification d'outil est utilisable pour localiser ladite portion de l'outil (41) en localisant la portion de l'outil (41) le long d'au moins une ligne s'étendant à partir d'une source de rayons X (21) jusqu'à un détecteur de rayons X (22) à travers un volume d'ultrasons (33) après l'alignement de l'image à ultrasons (32) avec l'image à rayons X (25, 26), et

un module de segmentation d'image utilisable pour exécuter une segmentation d'image d'une intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à une localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32).

8. Dispositif de suivi d'outil (50) selon la revendication 7, dans lequel l'outil (41) est un cathéter, et dans lequel une portion de l'outil (41) est une pointe de l'outil (41).

9. Dispositif de suivi d'outil (50) selon la revendication 7, dans lequel l'au moins une ligne sert d'au moins une contrainte de frontière pour une exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32).

10. Dispositif de suivi d'outil (50) selon la revendication 7, dans lequel une exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à la localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) comprend en outre :

la construction d'un graphique d'énergie pondérée initial (140) ; et
l'exécution d'une segmentation à découpage de graphique du graphique d'énergie pondérée initial (140).

11. Dispositif de suivi d'outil (50) selon la revendication 10, dans lequel l'exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à la localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) comprend en outre :

l'application d'un filtre de forme à la segmentation à découpage de graphique du graphique d'énergie pondérée initial (140) ;
la construction d'un graphique d'énergie pondérée final (140) en fonction de l'application du filtre de forme à la segmentation à découpage de graphique du graphique d'énergie pondérée initial (140) ; et
l'exécution d'une segmentation à découpage de graphique du graphique d'énergie pondérée final (140).

12. Procédé guidé par image pour assurer le suivi d'un outil (41) à l'intérieur d'une région anatomique (40), comprenant :

la génération d'au moins une image à rayons X (25, 26) illustrant l'outil (41) à l'intérieur d'une région anatomique (40) ;
la génération d'une image à ultrasons (33) illustrant l'outil (41) à l'intérieur de la région anatomique (40) ;

la localisation d'une portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) sur la base d'une identification de la portion de l'outil (41) qui est située à l'intérieur de l'au moins une image à rayons X (25, 26), **caractérisé en ce que** ladite localisation de ladite portion de l'outil est effectuée en localisant la portion de l'outil (41) le long d'au moins une ligne s'étendant à partir d'une source de rayons X (21) jusqu'à un détecteur de rayons X (22) à travers un volume d'ultrasons (33) après l'alignement de l'image à ultrasons (32) avec l'image à rayons X (25, 26) ; et l'exécution d'une segmentation d'image d'une intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à une localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32).

13. Procédé guidé par image selon la revendication 12, dans lequel l'au moins une ligne sert d'au moins une contrainte de frontière pour une exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32).

14. Procédé guidé par image selon la revendication 12, dans lequel une exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à la localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) comprend en outre :

la construction d'un graphique d'énergie pondérée initial (140) ; et
l'exécution d'une segmentation à découpage de graphique du graphique d'énergie pondérée initial (140).

15. Procédé guidé par image selon la revendication 14, dans lequel l'exécution de la segmentation d'image de l'intégralité de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) par rapport à la localisation de la portion de l'outil (41) qui est située à l'intérieur de l'image à ultrasons (32) comprend en outre :

l'application d'un filtre de forme à la segmentation à découpage de graphique du graphique d'énergie pondérée initial (140) ;
la construction d'un graphique d'énergie pondérée final (140) en fonction de l'application du filtre de forme à la segmentation à découpage de graphique du graphique d'énergie pondérée initial (140) ; et
l'exécution d'une segmentation à découpage de graphique du graphique d'énergie pondérée final (140).

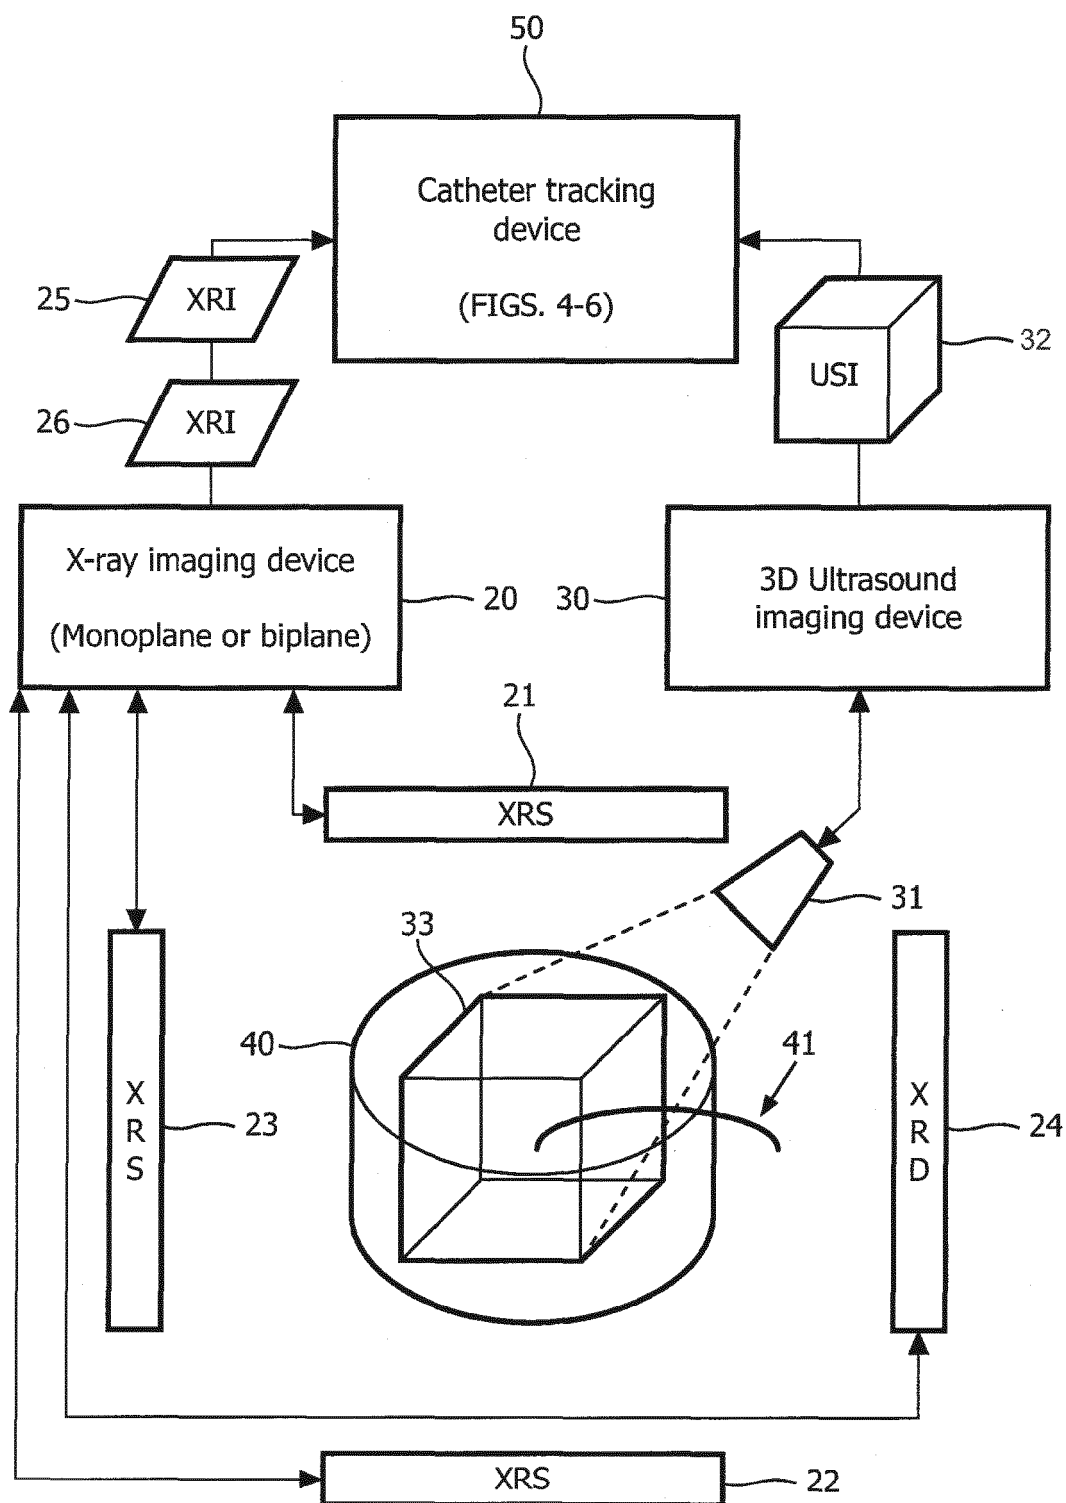


FIG. 1


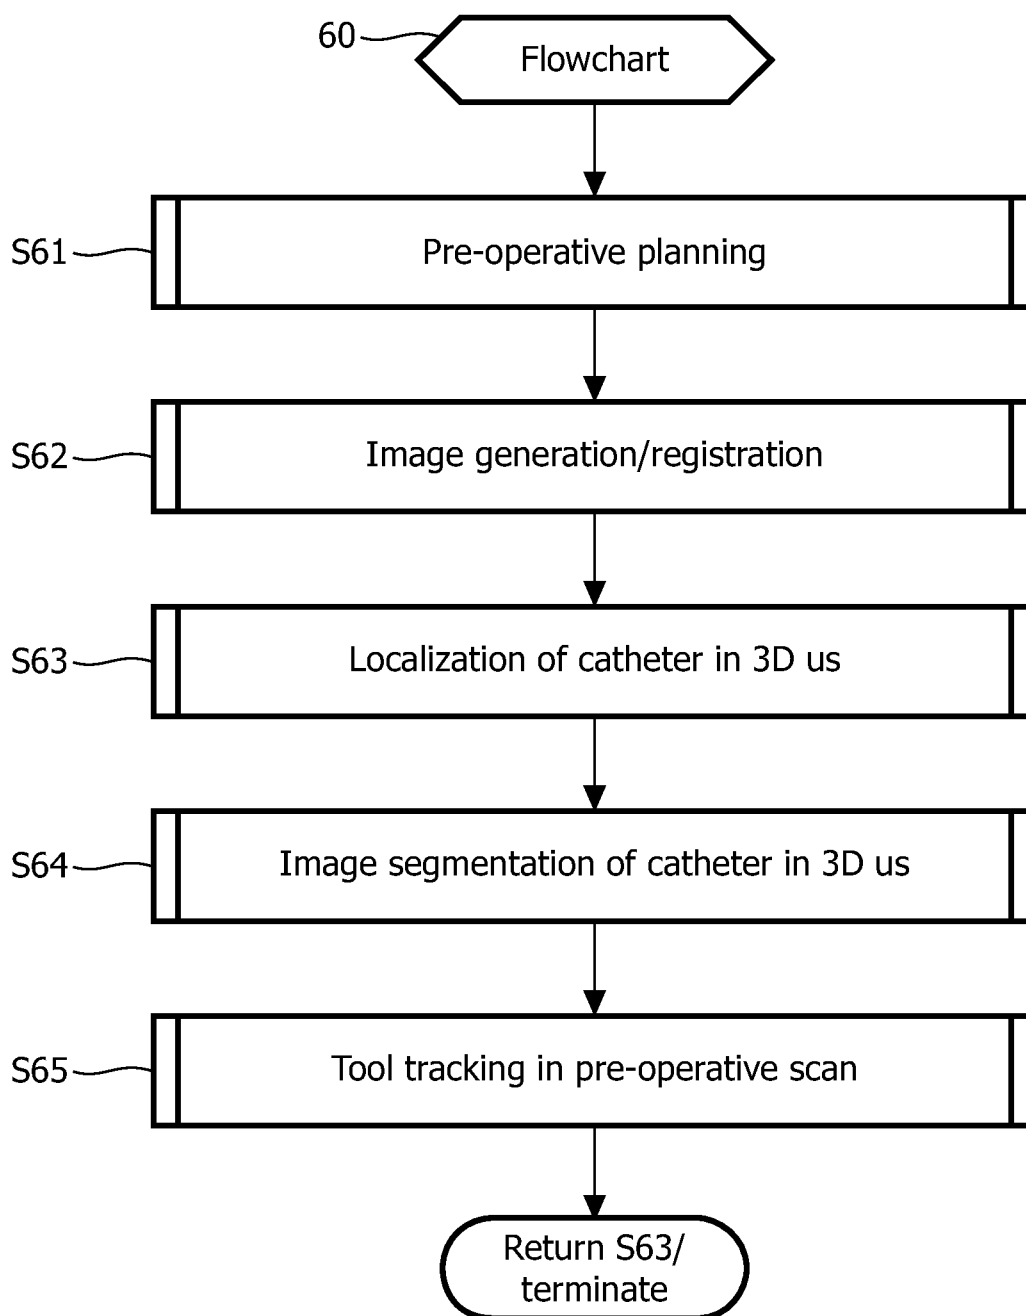


FIG. 2

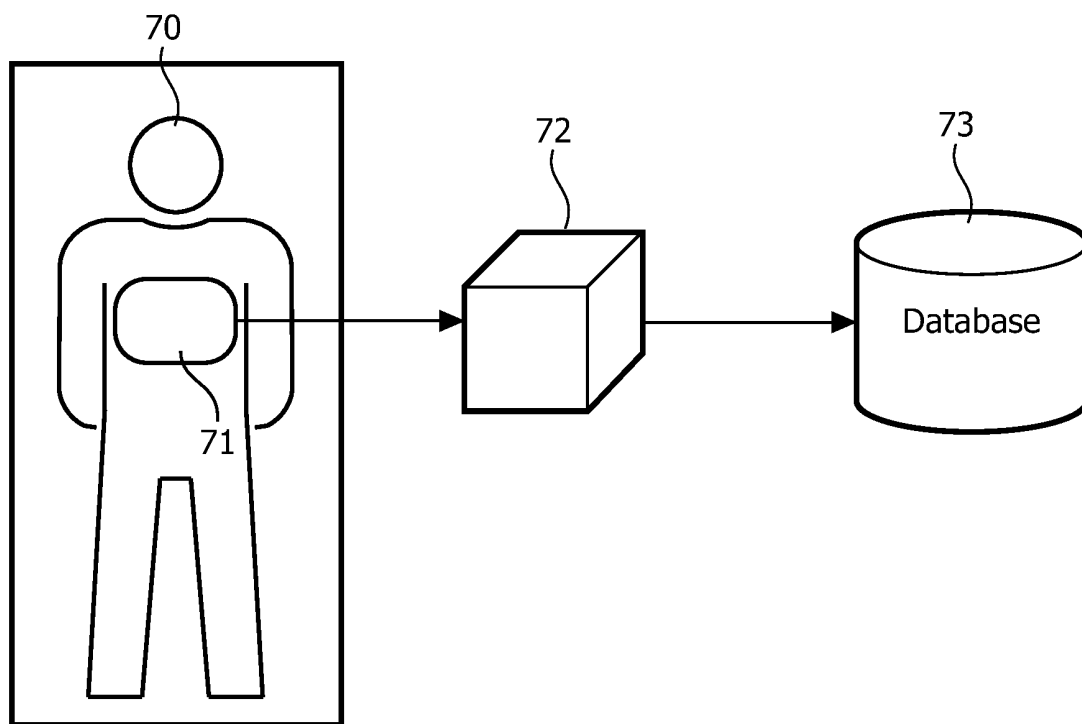

PRE-OPERATIVE

INTRA-OPERATIVE

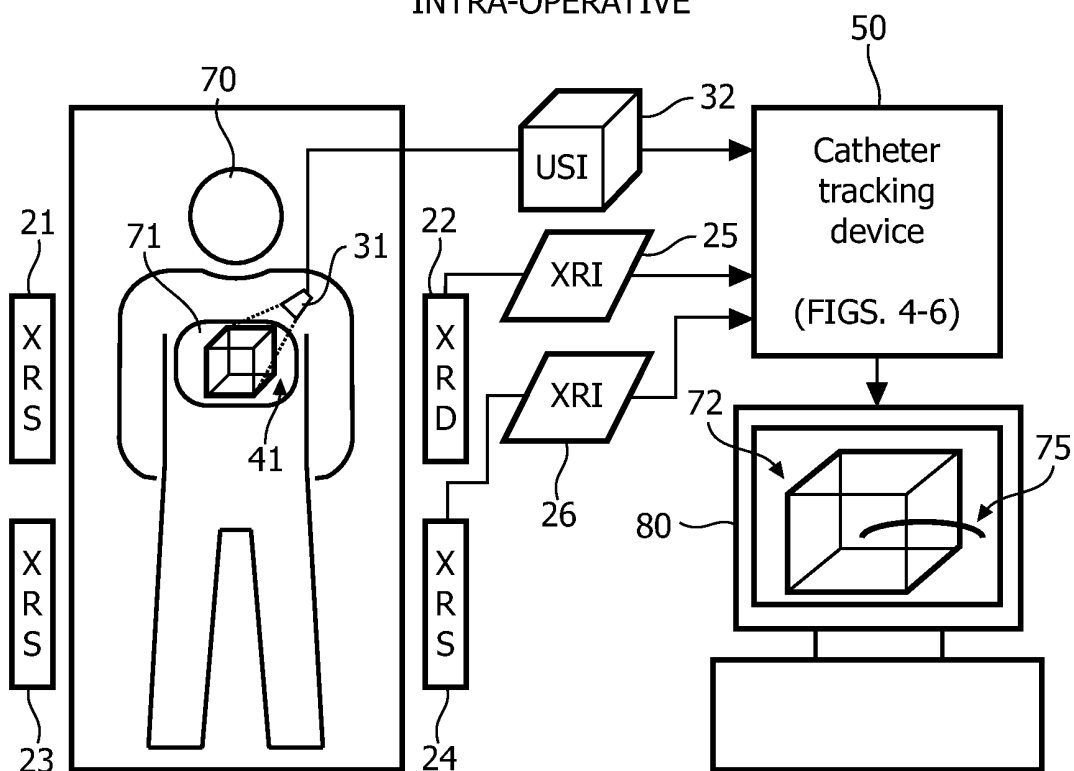


FIG. 3

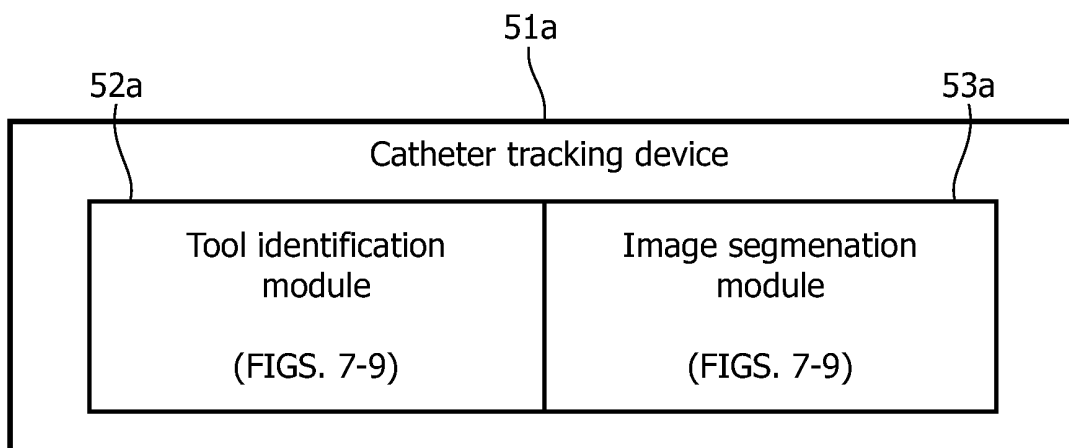


FIG. 4

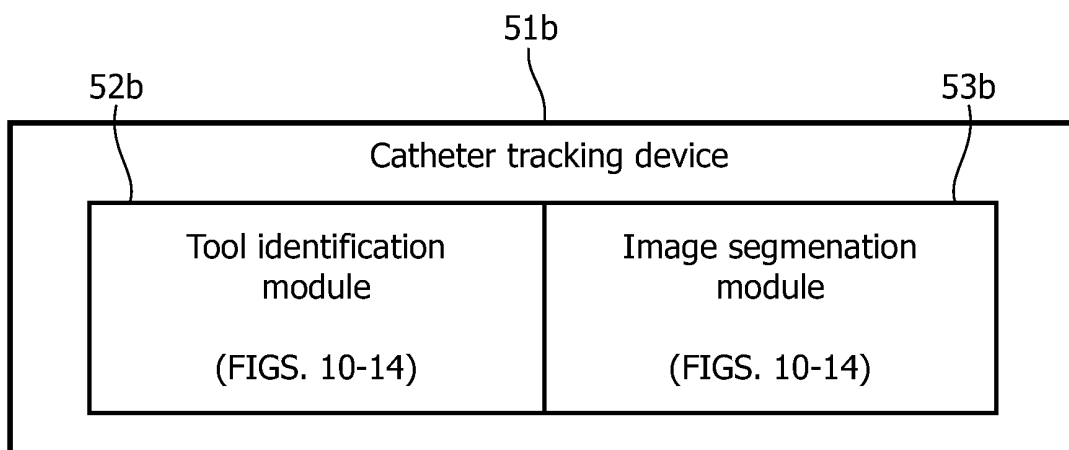


FIG. 5

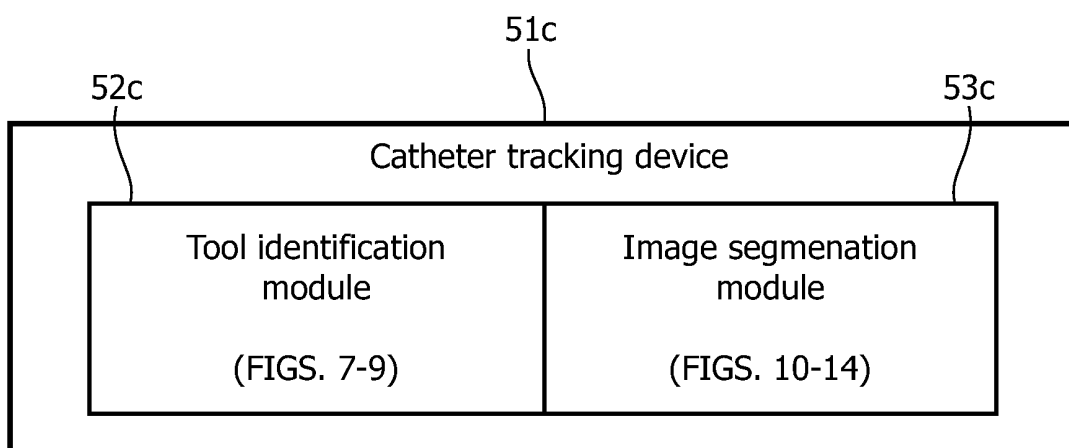


FIG. 6

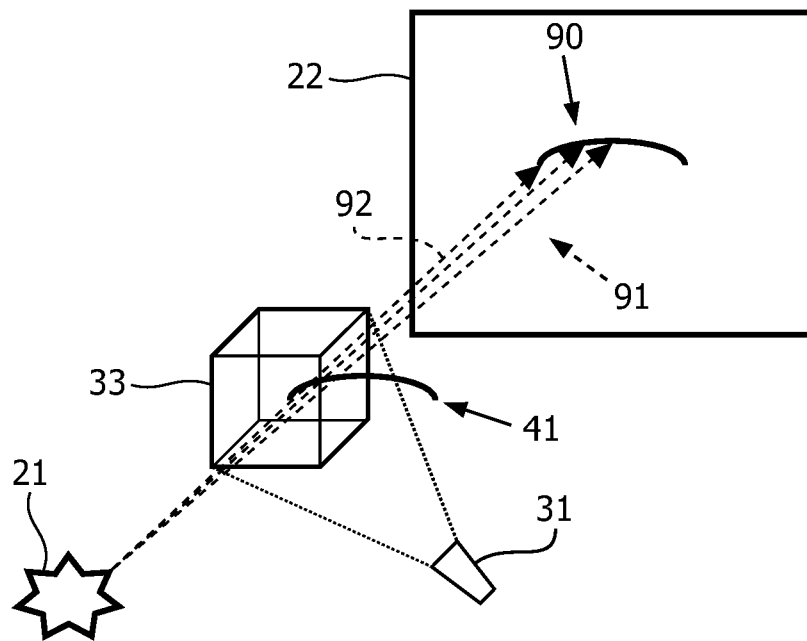


FIG. 7

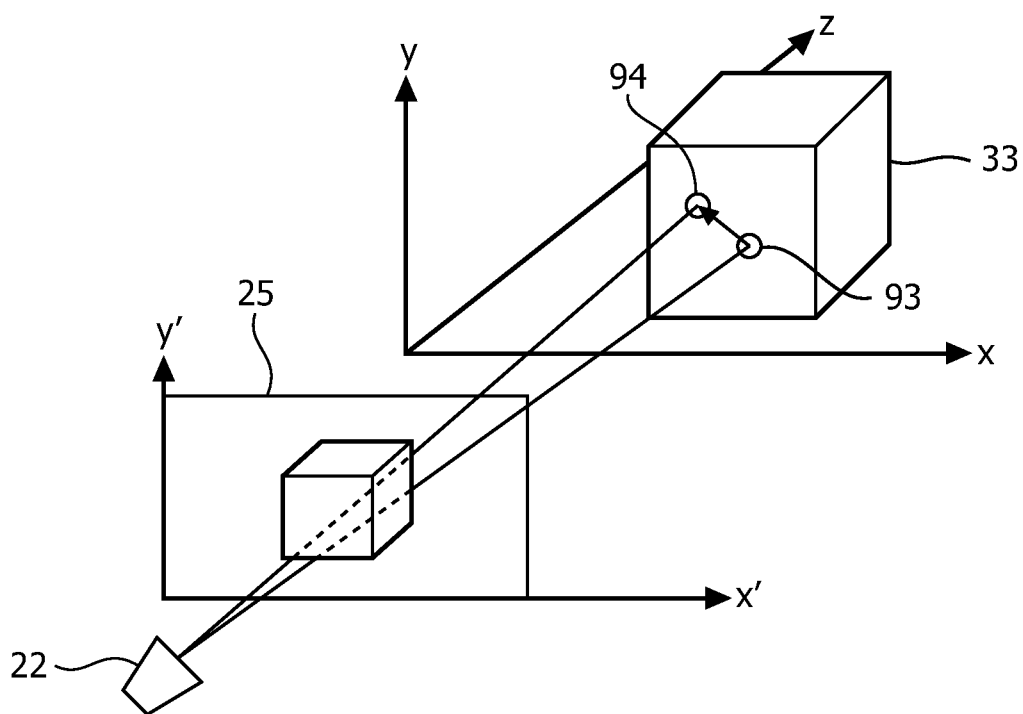


FIG. 8

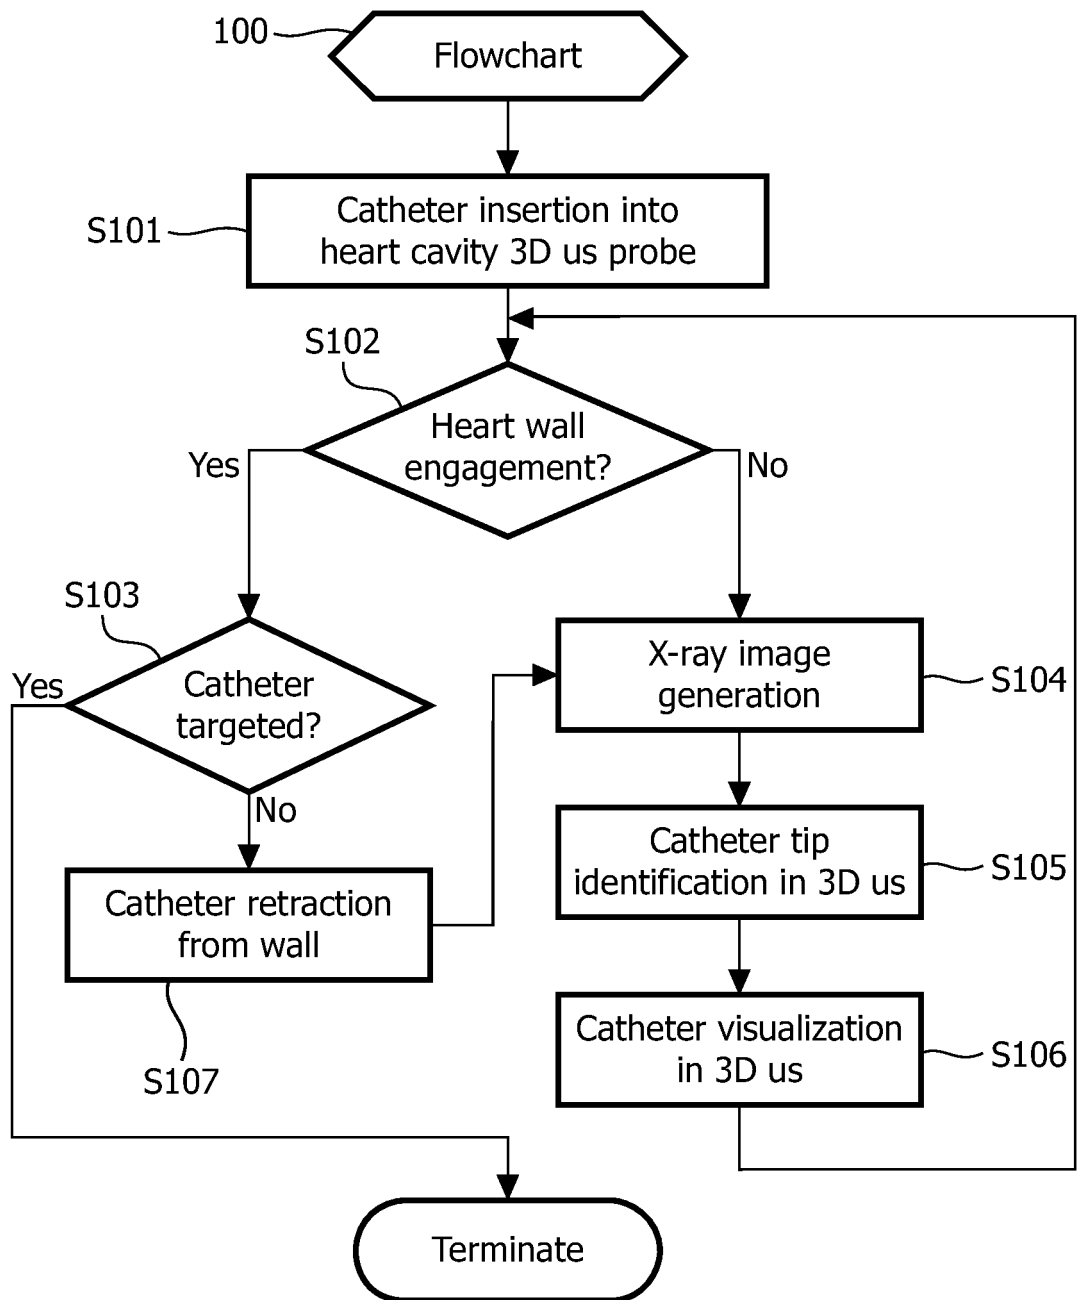


FIG. 9

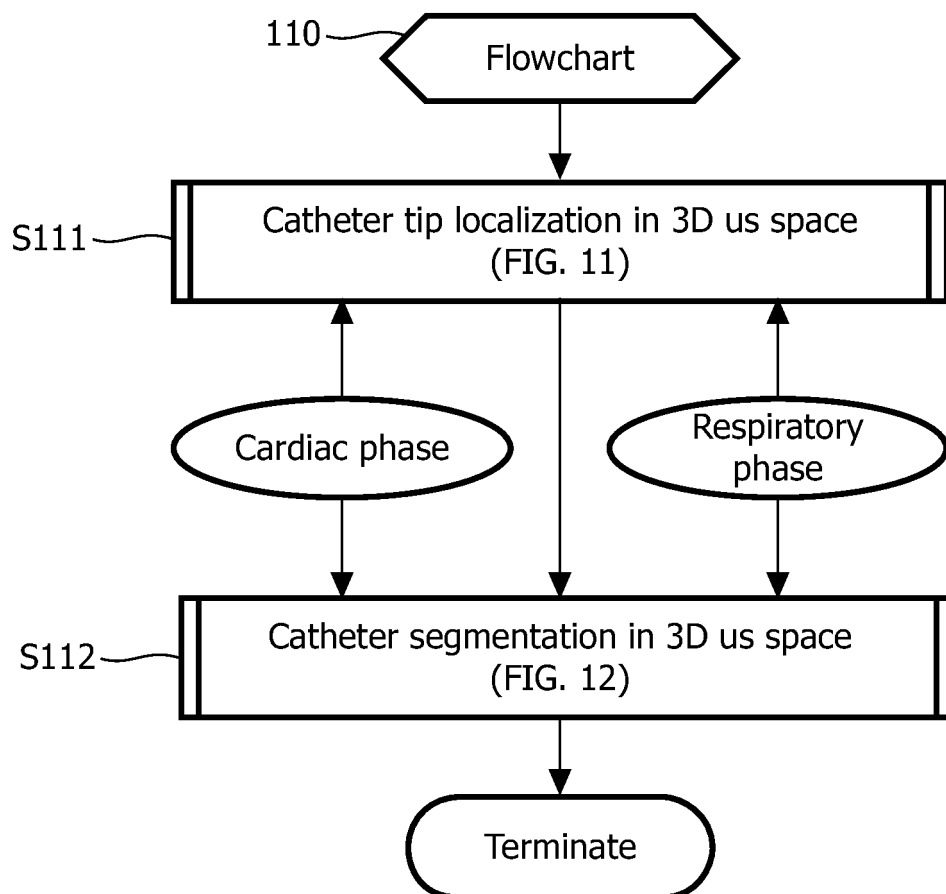


FIG. 10

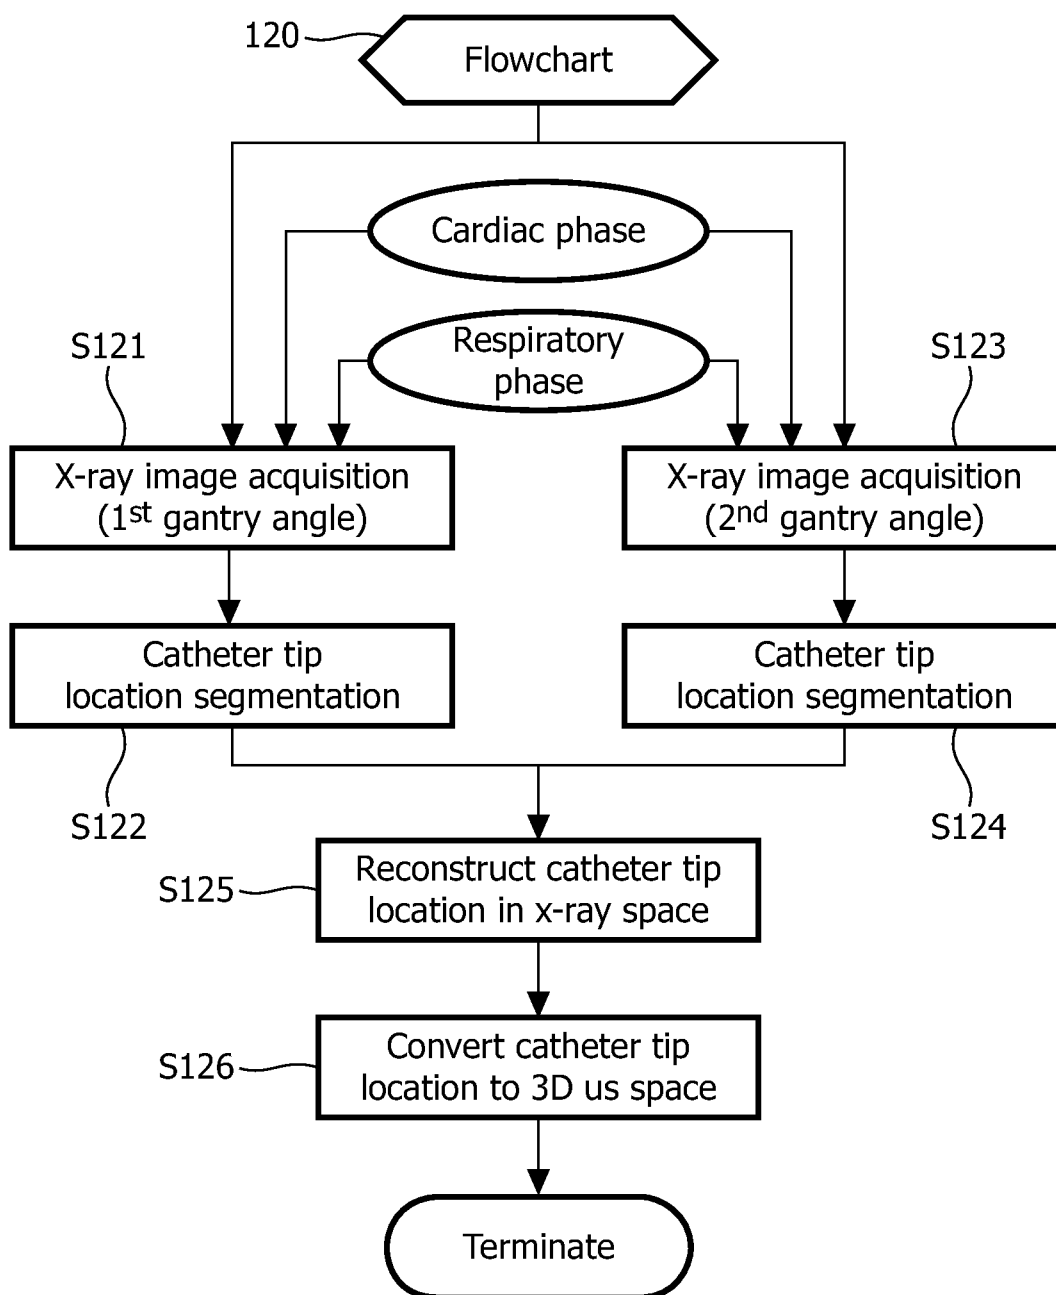


FIG. 11

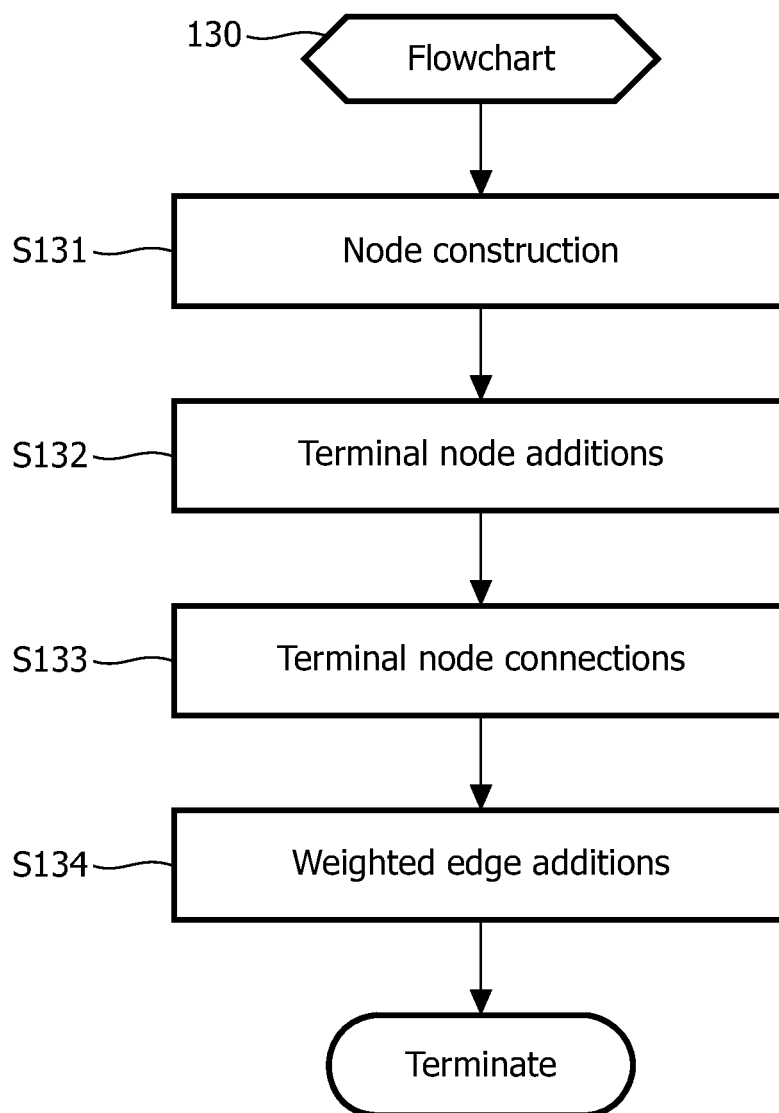


FIG. 12

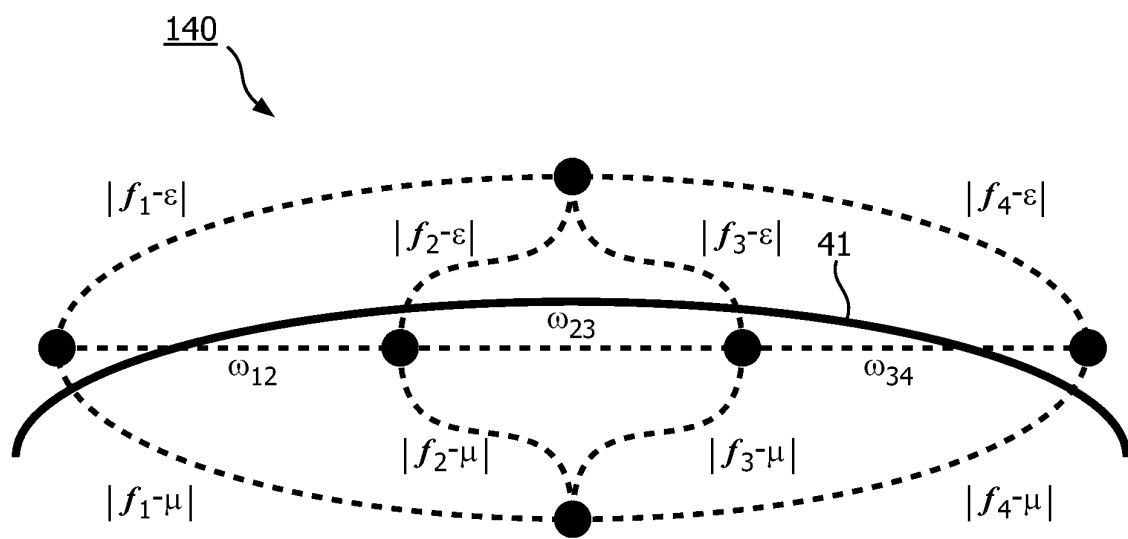


FIG. 13

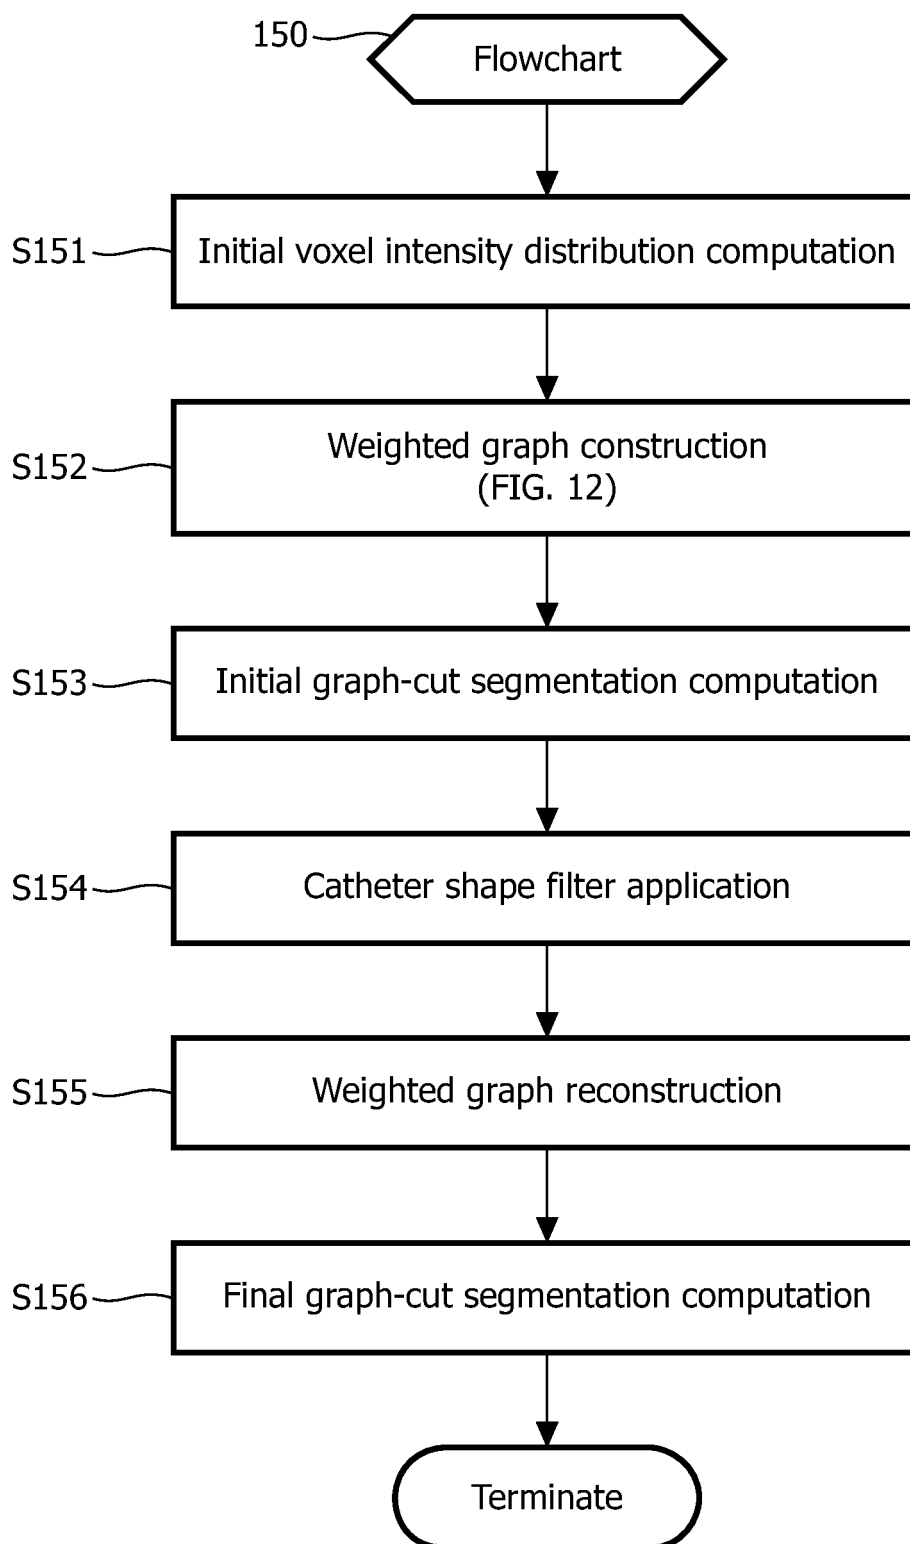


FIG. 14

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- DE 10210648 A1 [0008]

专利名称(译)	三维超声中导管的可视化		
公开(公告)号	EP2663237B1	公开(公告)日	2014-12-31
申请号	EP2012701029	申请日	2012-01-10
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	YAN PINGKUN PARTHASARATHY VIJAY MANZKE ROBERT JAIN AMEET KUMAR		
发明人	YAN, PINGKUN PARTHASARATHY, VIJAY MANZKE, ROBERT JAIN, AMEET KUMAR		
IPC分类号	A61B6/12 A61B8/08		
CPC分类号	A61B34/20 A61B6/12 A61B8/0883 A61B8/466 A61B8/483		
代理机构(译)	STEFFEN , THOMAS		
优先权	61/432327 2011-01-13 US		
其他公开文献	EP2663237A1		
外部链接	Espacenet		

摘要(译)

图像引导系统采用X射线成像装置 (20) 产生一个或多个X射线图像 (25,26) , 示出解剖区域 (40) 内的工具 (41) 和超声成像装置 (30) 用于产生描绘解剖区域 (40) 内的工具 (41) 的超声图像 (33) 。图像引导系统还采用工具跟踪装置 (50) , 用于在视觉上跟踪解剖区域 (40) 内的工具 (41) 。在操作中, 工具跟踪装置 (50) 响应于工具 (41) 的部分的识别位于X射线图像内而将工具 (41) 的一部分定位在超声图像 (33) 内 (s) (25,26) , 并且相对于位于超声图像内的工具 (41) 的部分的定位, 执行位于超声图像 (33) 内的整个工具 (41) 的图像分割。 (33) 。

