


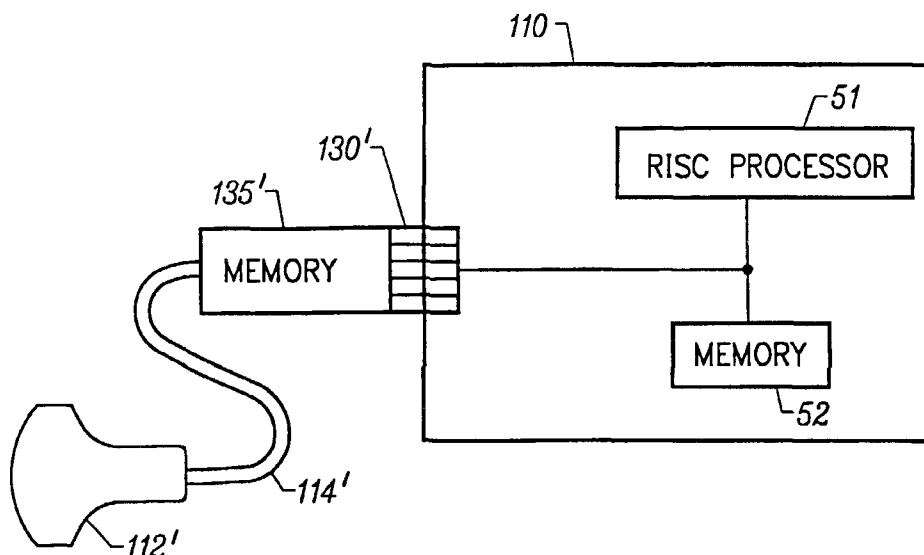

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : A61B 8/00	A1	(11) International Publication Number: WO 00/66002 (43) International Publication Date: 9 November 2000 (09.11.00)
(21) International Application Number: PCT/US00/12422 (22) International Filing Date: 4 May 2000 (04.05.00) (30) Priority Data: 60/132,421 4 May 1999 (04.05.99) US 09/564,601 3 May 2000 (03.05.00) US (71) Applicant: SONOSITE, INC. [US/US]; Suite 200, 19807 North Creek Parkway, Bothell, WA 98011-8214 (US). (72) Inventors: LITTLE, Blake, W.; 2505 241st Street S.E., Bothell, WA 98021 (US). CATALLO, Leo, R.; 5021 E. Mercer Way, Mercer Island, WA 98040 (US). QUISTGAARD, Jens, U.; 4716 N.E. 187th Place, Seattle, WA 98155 (US). (74) Agents: AKA, Gary, T. et al.; Townsend and Townsend and Crew LLP, 8th Floor, Two Embarcadero Center, San Francisco, CA 94111-3834 (US).	(81) Designated States: AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i>	

(54) Title: ULTRASOUND DIAGNOSTIC INSTRUMENT HAVING SOFTWARE IN DETACHABLE SCANHEAD

**(57) Abstract**

An ultrasound diagnostic instrument includes a console (110) having electronic circuitry for processing electrical signals for display including a digital processor (40), a memory (32, 42) for storing software for use with the processor (40), and a first connector (130) coupled to the memory, and processor. A transducer scanhead (112) for generating ultrasound waves, for receiving reflected ultrasound waves is connected through a cable (114), a second connector to the first connector, and to the digital processor. A second memory (42) external to the console (110) is provided for communicating with the digital processor (40) through the second connector, the second memory storing software, and data necessary for use of the transducer scan head (112) in the ultrasound diagnostic instrument.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

ULTRASOUND DIAGNOSTIC INSTRUMENT HAVING SOFTWARE IN DETACHABLE SCANHEAD

5

This invention claims priority from Provisional Application 60/132,421 filed May 4, 1999 and is related to co-pending Provisional Application 60/132,558 filed May 5, 1999 for Low Power Portable Ultrasound Diagnostic Instrument and Provisional Application 60/132,515 filed May 4, 1999 for Mobile Ultrasound Diagnostic Instrument and Docking Stand.

10

BACKGROUND OF THE INVENTION

This invention relates generally to medical ultrasonic diagnostic systems, and more particularly this invention relates to ultrasonic diagnostic instruments which employ detachable ultrasound transducer scanheads.

15

Modern ultrasonic diagnostic systems are large, complex instruments. Today's premium ultrasound systems, while mounted in carts for portability, continue to weigh several hundred pounds. In the past, ultrasound systems such as the ADR 4000 ultrasound system produced by Advanced Technology Laboratories, Inc., were smaller desktop units about the size of a personal computer. However, such instruments lack many of the advanced features of today's premium ultrasound systems such as color Doppler imaging and three dimensional display capabilities. As ultrasound systems become more sophisticated they also become bulkier.

20

Disclosed in U.S. Patent No. 5,722,412 is a diagnostic ultrasound instrument which exhibits many of the features of a premium ultrasound system in an hand-held unit. The instrument can be produced as a single unit or in a preferred embodiment the instrument is a two-part unit one including a transducer, beamformer, and image processor and the other including a display and power source for both units. In such a configuration the transducer/processor unit can be manipulated with one hand while a cable between the two units enables the video to be shown on the display unit

25

30

while the lateral unit is held or positioned for optimal viewing of the ultrasound image. The cable also provides energy for the transducer/processor unit from the display unit.

Co-pending application Serial No. 19162-3 discloses a portable ultrasound diagnostic instrument in which a power monitor and control function are incorporated to
5 limit power consumption. Co-pending application Serial No. 19162-8 discloses a docking stand which can be employed with the instrument of Serial No. 19162-3.

Heretofore, the operating software and any special function software have been stored in memory with the system processor in a console of the instrument. Since various special application scanheads can be used with the instrument, the operating
10 software for implementing the special applications has been stored in the console, thus necessitating a large memory. This can be inconvenient when new scanheads are introduced or when system software is upgraded since the console often must be returned to a central service facility for software update or the expense of having trained field personnel is required for field upgrade.

15 The present invention is directed to facilitating software update and special operating software without the need for a large module memory or for module retrofitting at a centralized service facility.

SUMMARY OF THE INVENTION

20

The present invention overcomes limitations in the prior art by providing memory in association with the transducer scanhead separate from the console of an ultrasound diagnostic instrument with the memory providing transducer specific data required for system setup, drive, and data image with transducers for various applications,
25 and depths, and optimization settings that are unique for each. The external memory also provides a means to update and upgrade the system executable code and thereby allow the use of future transducer scanheads and to provide for future applications of the instrument. By so providing a memory outside of the console, manual field upgrade or system swap is obviated when a new function, application, or transducer scanhead is
30 introduced.

The invention and objects and features thereof will be more readily apparent from the following detailed description and appended claims when taken with the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a functional block diagram of an ultrasonic diagnostic instrument
5 as disclosed in application Serial No. 19162-3.

Fig. 2 is a perspective view illustrating an ultrasound diagnostic instrument
and docking stand as disclosed in application Serial No. 19162-8.

Fig. 3 is a functional block diagram of the ultrasound diagnostic
instruments of Figs. 1 and 2 as modified in accordance with the present invention.

10 Fig. 4 is a functional block diagram of a memory in an ultrasound
diagnostic instrument in accordance with the invention and contents of the memory.

DETAILED DESCRIPTION OF ILLUSTRATIVE EMBODIMENTS

15 Fig. 1 is a detailed functional block diagram of an ultrasonic diagnostic
instrument as disclosed in co-pending application Serial No. 19162-3. The instrument is
described in more detail in U.S. Patent No. 5,722,412, which is incorporated herein by
reference. In this instrument a transducer array 10 is used for a solid state, electronic
control capabilities, variable aperture, image performance and reliability. Either a flat or
20 curved linear array can be used. In a preferred embodiment the array is a curved array,
which affords a broad sector scanning field. While the preferred embodiment provides
sufficient delay capability to both steer and focus a flat array such as a phased array, the
geometric curvature of the curved array reduces the delay requirements on the
beamformer. The elements of the array are connected to a transmit/receive ASIC 20
25 which drives the transducer elements and receives echoes received by the elements. The
transmit/receive ASIC 30 also controls the transmit and receive apertures of the array 10
and the gain of the received echo signals. The transmit/receive ASIC is preferably
located within inches of the transducer elements, preferably in the same enclosure, and
just behind the transducer.

30 Echoes received by the transmit/receive ASIC 20 are provided to the
adjacent front end ASIC 30, which beamforms the echoes from the individual transducer
elements into scanline signals. The front end ASIC 30 also controls the transmit
waveform, timing, aperture and focusing. In the illustrated embodiment the front end

ASIC 30 provides timing signals for the other ASICs, time gain control, and monitors and controls the power applied to the transducer array, thereby controlling the acoustic energy which is applied to the patient and minimizing power consumption of the unit. A memory device 32 is connected to the front end ASIC 30, which stores data used by the
5 beamformer.

Beamformer scanline signals are coupled from the front end ASIC 30 to the adjacent digital signal processing ASIC 40. The digital signal processing ASIC 40 filters the scanline signals and in the preferred embodiment also provides several advanced features including synthetic aperture formation, frequency compounding.
10 Doppler processing such as power Doppler (color power angio) processing, and speckle reduction.

The ultrasound B mode and Doppler information is then coupled to the adjacent back end ASIC 50 for scan conversion and the production of video output signals. A memory device 42 is coupled to the back end ASIC 50 to provide storage used
15 in three dimensional power Doppler (3D CPA) imaging. The back end ASIC also adds alphanumeric information to the display such as the time, date, and patient identification. A graphics processor overlays the ultrasound image with information such as depth and focus markers and cursors. Frames of ultrasonic images are stored in a video memory 54 coupled to the back end ASIC 50, enabling them to be recalled and replayed in a live
20 realtime sequence. Video information is available at a video output in several formats, including NTSC and PAL television formats and RGB drive signals for an LCD display 60 or a video monitor.

The back end ASIC 50 also includes the central processor for the ultrasound system, a RISC (reduced instruction set computer) processor. The RISC
25 processor is coupled to the front end and digital signal processing ASICs to control and synchronize the processing and control functions throughout the hand-held unit. A program memory 52 is coupled to the back end ASIC 50 to store program data which is used by the RISC processor to operate and control the unit. The back end ASIC 50 is also coupled to a data port configured as a PCMCIA interface 56. This interface allows other
30 modules and functions to be attached to the hand-held ultrasound unit. The interface 56 can connect to a modem or communications link to transmit and receive ultrasound information from remote locations. The interface can accept other data storage devices to add new functionality to the unit, such as an ultrasound information analysis package.

The RISC processor is also coupled to the user controls 70 of the unit to accept user inputs to direct and control the operations of the hand-held ultrasound system.

Power for the hand-held ultrasound system in a preferred embodiment is provided by a rechargeable battery. Battery power is conserved and applied to the components of the unit from a power subsystem 80. The power subsystem 80 includes a DC converter to convert the low battery voltage to a higher voltage which is applied to the transmit/receive ASIC 20 to drive the elements of the transducer array 10. In order to limit power consumption, the power monitor and control unit 80 controls the operating mode of the LCD display 60 and video circuitry in unit 50 along with the clock frequency of the RISC processor in unit 50 and the clock frequencies of the DAC and ADC units in beamformer circuitry 30. The color angiography function unit and 3D signal processing DSP unit 40 are similarly controlled by the power monitor and control.

Fig. 2 is a perspective view of a mobile ultrasound diagnostic instrument and docking stand as disclosed in application Serial No. 19162-8. The diagnostic instrument includes a console 110 and transducer scanhead 112 which is connected to console 110 through cable 114. The instrument can be of the type disclosed in U.S. Patent No. 5,722,412 and in co-pending application Serial No. 19162-3, as illustrated in Fig. 1.

Console 110 is received within a sleeve receptacle 116 which is supported in a raised position by means of a vertical support 118 that mounts to a base 120 having a plurality of wheels 122 for movement. Cable 114 connects a scanhead 112 to console 110 and includes a connector 130 which plugs into console 110. Alternatively, scanhead 112 can communicate with console 112 by wireless transmission of signals from a transceiver in the scanhead to and from a transceiver in console 112.

In using the instrument of Fig. 2 it is often expeditious to connect any one of a plurality of scanheads 112 to the console for specific applications. Arm 160 is attached to the vertical support 118 for receiving a plurality of scanheads 112', cables 114', and connectors 130'.

In accordance with the invention, and as shown in Fig. 3 a memory 135' is provided with each scanhead 112' and connector 130' which includes software and data necessary for use of the specific scanhead in the ultrasound diagnostic instrument. The memory can be located in connector 130' in cable 114', or in the scanhead 112'. Cable 114' and connector 130' connect the memory with the processor 51 and memory 52 within

module 110. Fig. 4 is a functional block diagram illustrating one embodiment in which the memory 135' is located within connector 130' and interfaces with program memory 52 and RISC processor 51 within module 110. Memory 135' stores operational data unique to a specific transducer scanhead which may be designed for specific applications such as cardiac analysis, neo-natal analysis, gynecology analysis, and prostate analysis. The stored data unique to the scanhead can include signal processing tables and beamforming tables along with filter coefficients, scan conversion coefficients, focusing tables, and compression tables. Calculations necessary for a specific application can also be included.

In addition to transducer scanhead data and application software, the memory can include system executable code which permits update and upgrade of the system executable code resident in memory 52 of the console. Thus software for future applications as well as operational data for various transducer scanheads can be provided in memory without the need for a manual field upgrade of the software stored in the console memory or the need for a system swap when a new function or application is required.

By providing a secondary memory external to the console and in association with a specific transducer scanhead, the memory requirements of the console can be greatly reduced since all the software necessary for a specific function and particular scanheads need not be stored therein. The inclusion of this system executable code obviates the need for field upgrade and provides greater versatility when using a plurality of special purpose transducer scanheads with the ultrasound instrument console. Thus instrument size, weight, and required power are reduced. Further reduction can be provided through use of the instrument as a data gathering instrument with the data being used at a centralized location for imaging. In this connection, memory 135' can include data encryption so that the process signals can be viewed only by an authorized party.

There has been described an ultrasound diagnostic instrument which achieves greater versatility in use by the provision of memory external to an instrument console and in association with a particular transducer scanhead. While the invention has been described with reference to a specific embodiment, the description is illustrative of the invention and is not to be construed as limiting the invention. For example, the memory within the console can be eliminated with the external memory providing all memory functions for the processor as well as the scanhead. Thus, various modifications

and applications may occur to those skilled in the art without departing from the true spirit and scope of the invention as defined by the appended claims.

WHAT IS CLAIMED IS:

- 1 1. An ultrasound diagnostic instrument comprising
2 a) a console including display electronic circuitry for processing
3 electrical signals for display including a digital processor, a first memory and a first
4 connector coupled to the processor and first memory,
5 b) a transducer scanhead for generating ultrasound waves and
6 receiving reflected or scattered ultrasound waves,
7 c) means for coupling the transducer scanhead for transmitting
8 electrical signals to and from the scanhead, and
9 d) a second memory for communicating with the console through the
10 second connector, the second memory storing software and data necessary for use of the
11 transducer scanhead in the ultrasound diagnostic instrument.
- 1 2. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the software and data stored in the second memory include operational data
3 unique to the transducer scanhead.
- 1 3. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the software and data include at least one of physical parameters, operational
3 data for the scanhead, and executable code.
- 1 4. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the software and data include operational software for executing unique
3 functions with the transducer scanhead.
- 1 5. The ultrasound diagnostic instrument as defined by claim 4
2 wherein the operational software provides unique diagnostic analysis.
- 1 6. The ultrasound diagnostic instrument as defined by claim 5
2 wherein the unique diagnostic analysis is selected from a group including cardiac
3 analysis, neo-natal analysis, gynecology analysis and prostate analysis.

- 1 7. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the software and data stored in the second memory includes system executable
3 code for the digital processor.
- 1 8. The ultrasound diagnostic instrument as defined by claim 7
2 wherein the system executable code comprises a software update and upgrade of system
3 executable code in the first memory.
- 1 9. The ultrasound diagnostic instrument as defined by claim 8
2 wherein the system executable code permits new applications of the instrument.
- 1 10. The ultrasound diagnostic instrument as defined by claim 8
2 wherein system executable code permits use of a new transducer scanhead in the
3 instrument.
- 1 11. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the memory resides in the transducer scanhead.
- 1 12. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the memory resides in a second connector connected to the means for coupling
3 for mating with the first connector in the console.
- 1 13. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the memory resides in the means for coupling.
- 1 14. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the console further includes a display for processed electrical signals.
- 1 15. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the console includes memory for storing processed electrical signals for display
3 at a remote facility.
- 1 16. The ultrasound diagnostic instrument as defined by claim 14
2 wherein the console memory includes data encryption for data from the transducer
3 scanhead to the console.

1 17. The ultrasound diagnostic instrument as defined by claim 1 and
2 further including a console memory within the console for storing software for use with
3 the processor.

1 18. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the means for coupling comprises a cable.

1 19. The ultrasound diagnostic instrument as defined by claim 1
2 wherein the means for coupling is wireless.

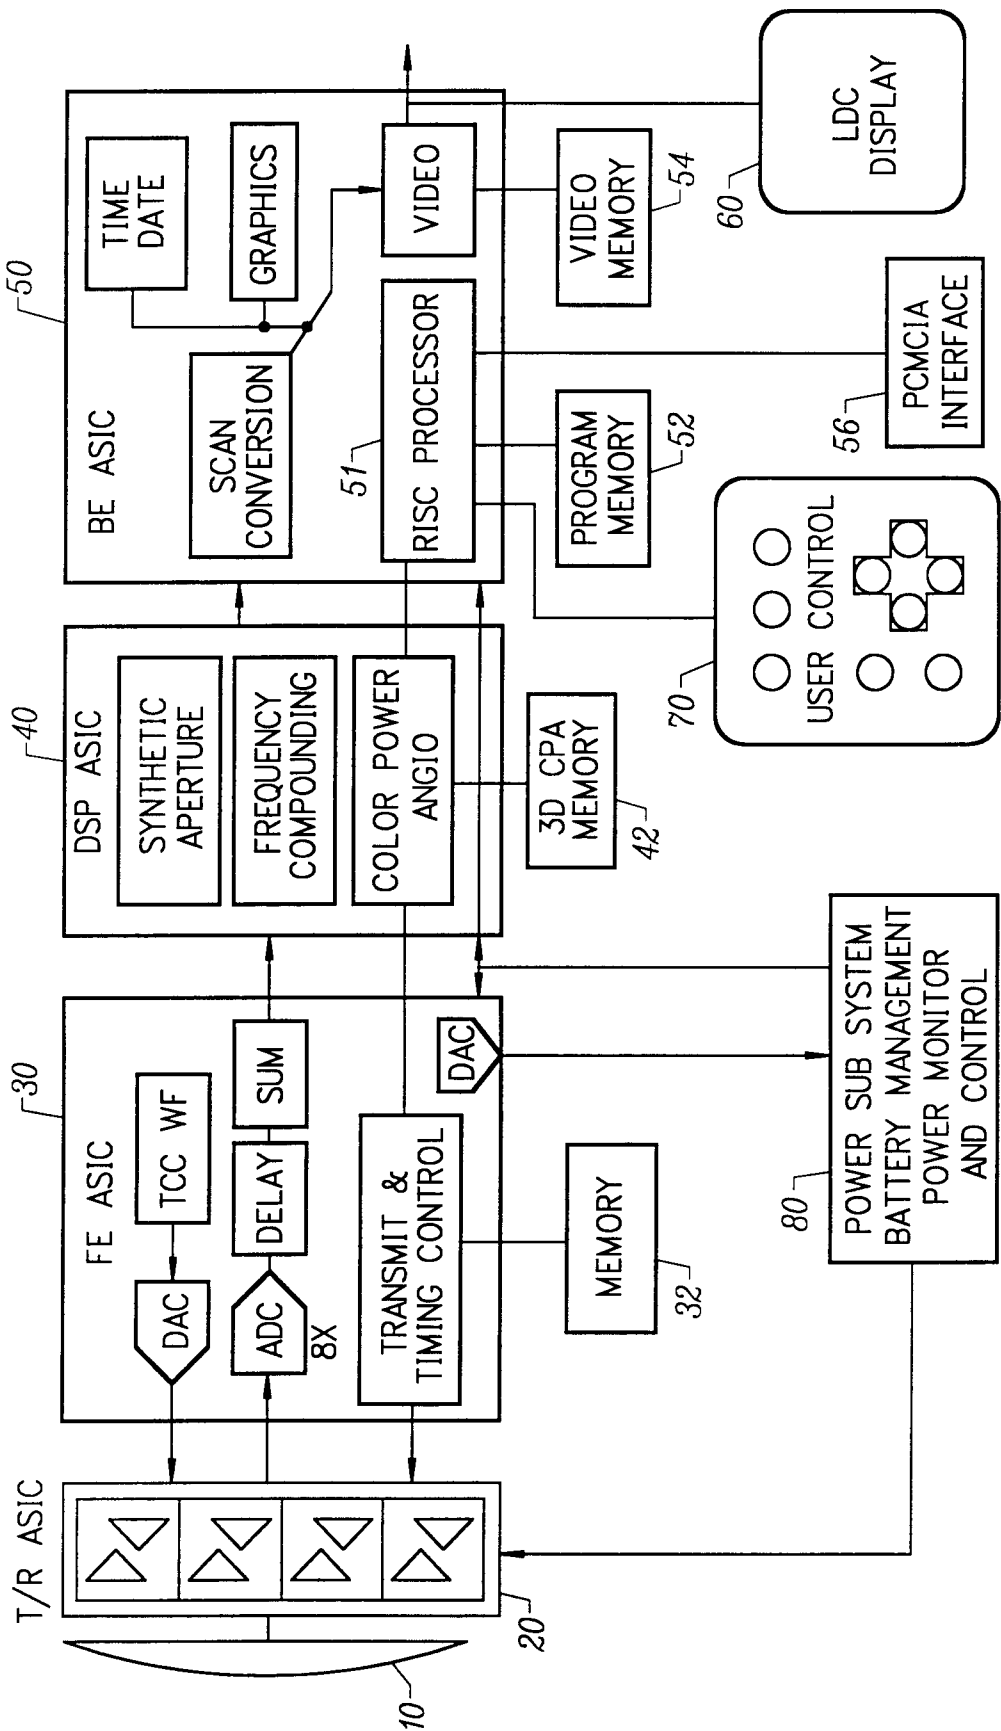
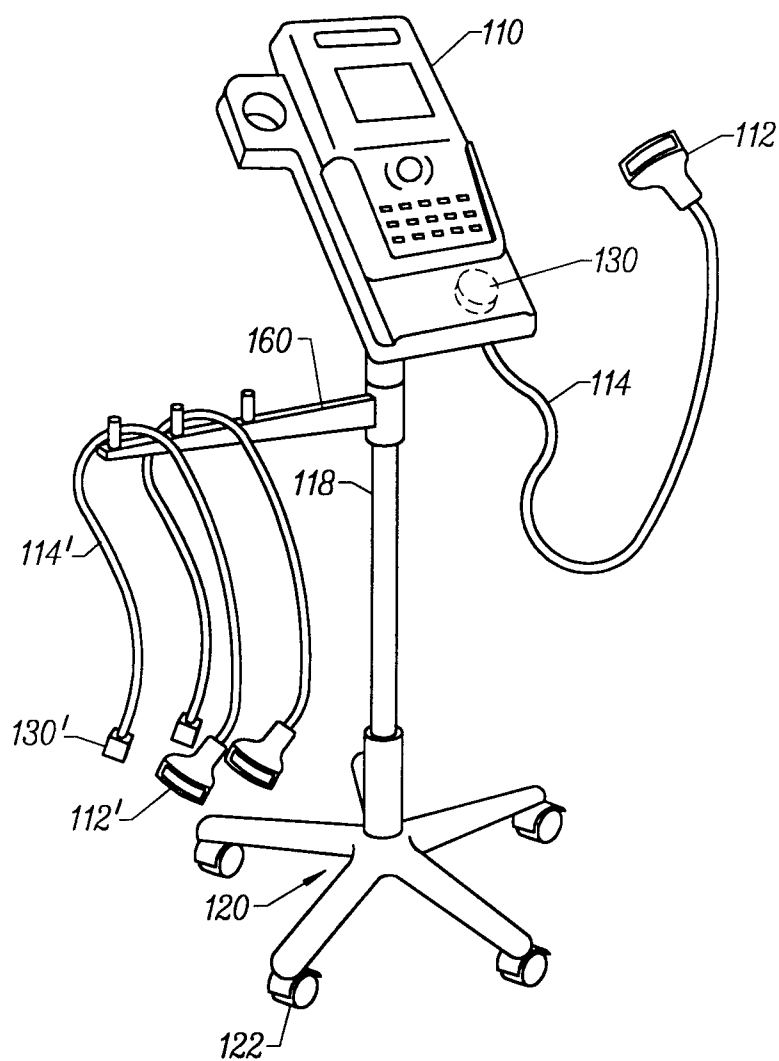
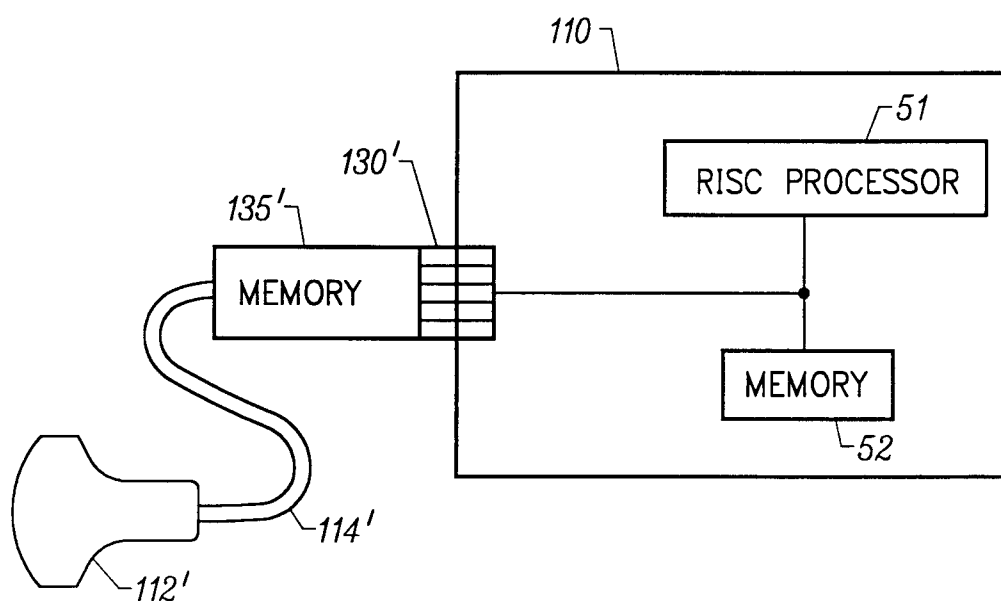
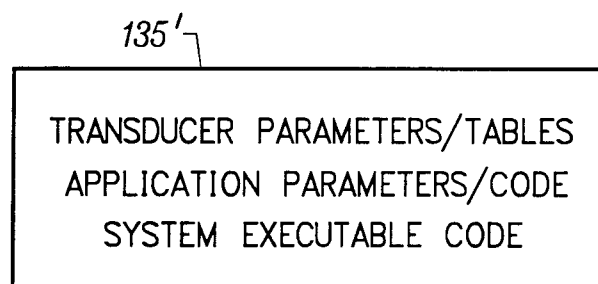


FIG. 1

*FIG. 2*

*FIG. 3**FIG. 4*

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US00/12422

A. CLASSIFICATION OF SUBJECT MATTER IPC(7) : A61B 8/00 US CL : 600/447 According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) U.S. : 128.903, 916; 364/708.1; 600/437, 443-447 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) WEST 2.0, EAST Search Terms: diagnostic, console, display, digital processor, ultrasound, memory		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5,690,114 A (CHIANG et al.) 25 November 1997, cols. 12-17.	1-19
Y	US 5,235,984 A (D'SA) 17 April 1993, Abstract.	1-19
Y	US 4,972,838 A (YAMAZAKI) 27 November 1990, entire document.	1-19
☐ Further documents are listed in the continuation of Box C. ☐ See patent family annex		
*	Special categories of cited documents:	
"A"	document defining the general state of the art which is not considered to be of particular relevance	"T"
"E"	earlier document published on or after the international filing date	"X"
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y"
"O"	document referring to an oral disclosure, use, exhibition or other means	"Z"
"P"	document published prior to the international filing date but later than the priority date claimed	"&"
		later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
		document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
		document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
		document member of the same patent family
Date of the actual completion of the international search	Date of mailing of the international search report	
12 JULY 2000	02 AUG 2000	
Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. (703) 305-3230	Authorized officer ALI IMAM Telephone No. 703-305-6933	

专利名称(译)	具有可拆卸扫描头软件的超声诊断仪器		
公开(公告)号	EP1180970A1	公开(公告)日	2002-02-27
申请号	EP2000928891	申请日	2000-05-04
[标]申请(专利权)人(译)	索诺塞特公司		
申请(专利权)人(译)	SONOSITE INC.		
当前申请(专利权)人(译)	SONOSITE INC.		
[标]发明人	LITTLE BLAKE W CATALLO LEO R QUISTGAARD JENS U		
发明人	LITTLE, BLAKE, W. CATALLO, LEO, R. QUISTGAARD, JENS, U.		
IPC分类号	A61B8/14 G01S7/52 G01S7/521 A61B8/00		
CPC分类号	G01S7/52079 A61B8/14 A61B8/4405 A61B8/4433 G01S7/52017		
优先权	09/564601 2000-05-03 US 60/132421 1999-05-04 US		
其他公开文献	EP1180970B1 EP1180970A4		
外部链接	Espacenet		

摘要(译)

超声诊断仪器包括控制台 (110) , 其具有用于处理用于显示的电信号的电子电路, 包括数字处理器 (40) , 用于存储与处理器 (40) 一起使用的软件的存储器 (32,42) , 以及第一连接器。 (130) 耦合到存储器和处理器。用于产生超声波的换能器扫描头 (112) 用于接收反射的超声波, 其通过电缆 (114) , 第二连接器连接到第一连接器, 并连接到数字处理器。控制台 (110) 外部的第二存储器 (42) 用于通过第二连接器与数字处理器 (40) 通信, 第二存储器存储软件, 以及使用转换器扫描头 (112) 所需的数据。超声诊断仪。