

(19)



(11)

EP 2 272 435 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

07.06.2017 Bulletin 2017/23

(51) Int Cl.:

A61B 8/08 (2006.01)

(86) International application number:

PCT/JP2009/057469

(21) Application number: **09734414.7**

(22) Date of filing: **14.04.2009**

(87) International publication number:

WO 2009/131027 (29.10.2009 Gazette 2009/44)

(54) REFERENCE DEFORMABLE BODY AND ULTRASONIC DIAGNOSTIC APPARATUS

DEFORMIERBARER BEZUGSKÖRPER UND ULTRASCHALLDIAGNOSEGERÄT

CORPS DE RÉFÉRENCE DÉFORMABLE ET APPAREIL DE DIAGNOSTIC À ULTRASONS

(84) Designated Contracting States:

**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL
PT RO SE SI SK TR**

(74) Representative: **Strehl Schübel-Hopf & Partner**

**Maximilianstrasse 54
80538 München (DE)**

(30) Priority: **25.04.2008 JP 2008114869**

(56) References cited:

**WO-A1-2005/120358 JP-A- 5 076 528
JP-A- 6 154 215 JP-A- 7 178 089
JP-A- H0 576 528 JP-A- 2003 070 788
JP-A- 2005 066 041 JP-A- 2005 066 041
JP-A- 2007 014 485 JP-A- 2007 215 672
JP-A- 2007 236 823 JP-U- 3 027 214
US-A1- 2007 239 006**

(43) Date of publication of application:
12.01.2011 Bulletin 2011/02

(73) Proprietor: **Hitachi, Ltd.**
Chiyoda-ku
Tokyo 100-8280 (JP)

(72) Inventor: **MATSUMURA, Takeshi**
Tokyo 101-0021 (JP)

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 272 435 B1

Description

Field of the Invention

[0001] The present description relates to a reference deformable body to be attached on an ultrasonic wave transmission/ reception surface of an ultrasonic probe, an ultrasonic diagnostic apparatus and ultrasonic diagnostic method for displaying a tomographic image of an imaging target portion in an object to be examined using ultrasonic waves or an elasticity image which presents hardness or softness of biological tissues. The present invention is set out in the appended claims.

Description of Related Art

[0002] An ultrasonic diagnostic apparatus transmits an ultrasonic wave to the inside of an object to be examined using an ultrasonic probe, receives the reflected echo signal of the ultrasonic wave from the inside of the object according to the structure of the biological tissue, and constructs a tomographic image such as a B-mode image to display for diagnosis.

[0003] Ultrasonic diagnostic apparatuses of recent years measure an ultrasonic wave receiving signal by pressing an object using an ultrasonic probe manually or mechanically, acquire displacement of the tissues, and display an elasticity image of the biological tissues based on the acquired displacement data. At this time, the method has been disclosed wherein a reference deformable body is attached to the ultrasonic probe via a fixing member, the border between the object and the reference deformable body is detected from the RF signal frame data acquired by transmission and reception of the ultrasonic waves, and the pressure applied to the object is measured from the positional information of the border (for example, Patent Document 1).

Prior Art Document

Patent Document

[0004] Patent Document 1: WO2005/120358

[0005] US 2007/0239006 A1 discloses an apparatus with the features in the preamble of present claim 1. Other conventional ultrasonic devices are described in JP H5 76528 A and JP 2005 66041 A.

[0006] There are various types of reference deformable bodies to be attached to an ultrasonic probe. For example, since there are different sizes or shapes of ultrasonic probes, the size or shape of the reference deformable body best suited to each of those probes would be also different. For a linear-type ultrasonic probe, a linear-type reference deformable body is to be attached. For a convex-type of ultrasonic probe, a curved reference deformable body is to be attached. Also, when depth or size of a measuring portion or physical attribute of the object is different, hardness or thickness of the reference deformable body needs to be changed. In this manner, it is necessary to switch types of the reference deformable body to have optimal feature according to the measurement condition.

[0007] However, if the type of the reference deformable body is not identified, elasticity modulus calculation or ultrasonic wave transmission/reception setting cannot be executed properly.

[0008] The objective of the present invention is to identify the type of a reference deformable body to be attached to an ultrasonic probe.

Summary of the Invention

[0009] In order to achieve the objective, the present invention provides the ultrasonic diagnostic apparatus defined in present claim 1. It comprises:

an ultrasonic probe having the ultrasonic wave transmitting/receiving surface on which a reference deformable body is attached;

a tomographic image constructing unit configured to transmit/receive an ultrasonic wave to/from an object to be examined via the reference deformable body, and generate a tomographic image based on the RF signal frame data of the cross-sectional region of the object;

a display unit configured to display the tomographic image;

a storing unit configured to store the relationship between an ID given to the reference deformable body and the type of the reference deformable body; and

a type identifying unit configured to read out the type of the reference deformable body corresponding to the ID of the reference deformable body attached to the ultrasonic probe and to identify the type of the reference deformable body. Consequently, the type of the reference deformable body can be identified.

[0010] It also comprises an image analyzing unit configured to analyze feature quantity of the reference deformable body in the tomographic image, wherein:

the storing unit stores the relationship between the analyzed feature quantity of the reference deformable body and the type of the reference deformable body; and
the type identifying unit reads out the type of the reference deformable body corresponding to the feature quantity of the reference deformable body in the newly-obtained tomographic image, and identifies the type of the reference deformable body. Consequently, the type of the reference deformable body can be identified.

[0011] Furthermore, it may comprise an image processing means configured to shift a tomographic image or an elasticity image toward the ultrasonic probe side in accordance with the thickness of the reference deformable body identified in the type identifying means. Furthermore, it may comprise an ultrasonic wave transmission/reception control unit configured to control the focus of the ultrasonic wave in accordance with the thickness of the reference deformable body identified by the type identifying means, so that the ultrasonic wave will not be focused on the reference deformable body.

[0012] In the present invention, the type of a reference deformable body can be identified, and the information thereof can be reflected to calculation of elasticity or displayed. The present invention is set out in the appended claims. The embodiments, aspects or examples according to the present description that do not fall within the scope of said claims are provided for illustrative purposes only and do not form part of the present invention.

Brief Description of the Drawings

[0013]

Fig. 1 shows the general configuration of the present description.

Fig. 2 shows the attachment pattern of a reference deformable body related to the present description.

Fig. 3 shows the display pattern of an ID related to the present description.

Fig. 4 shows the first embodiment of the present description.

Fig. 5 shows an embodiment of pressure measurement related to the present description.

Fig. 6 shows the second embodiment of the present description.

Fig. 7 shows a tomographic image of a reference deformable body in which scatterer is included, which is related to the present description.

Fig. 8 shows a tomographic image of a reference deformable body formed by a plurality of different layers, which is related to the present description.

Fig. 9 shows a tomographic image of a reference deformable body including bar code, which is related to the present description.

Fig. 10 shows the third embodiment of the present description.

Fig. 11 shows tomographic images before and after receiving correction process.

Description of Reference Numerals

[0014] 1: ultrasonic wave transmission/reception control circuit, 2: transmitting circuit, 3: ultrasonic probe, 4: receiving circuit, 5: phasing and adding circuit, 6: signal processing unit, 7: black and white scan converter, 8: RF signal frame data selecting unit, 9: displacement/strain calculating unit, 10: elasticity modulus calculating unit, 11: elasticity data processing unit, 12: color scan converter, 13: switching and adding unit, 14: image display unit, 15: pressure calculating unit, 16: reference deformable body, 30: reference deformable body information acquiring unit, 32: control unit, 34: input unit, 36: cine memory

Detailed Description of the Invention

[0015] An embodiment of the present description will be described referring to the diagrams. Fig. 1 shows a block diagram of the ultrasonic diagnostic apparatus related to the present description. An ultrasonic diagnostic apparatus is for acquiring a tomographic image of a measuring portion in an object to be examined using ultrasonic waves and displaying an elasticity image that presents hardness or softness of biological tissues.

[0016] The ultrasonic diagnostic apparatus is configured comprising ultrasonic wave transmission/reception control circuit 1, transmitting circuit 2, ultrasonic probe 3, receiving circuit 4, phasing and adding circuit 5, signal processing unit 6, black and white scan converter 7, RF signal frame data selecting unit 8, displacement/strain calculating unit 9, elasticity modulus calculating unit 10, elasticity data processing unit 11, color scan converter 12, switching and adding unit 13, image display unit 14, pressure calculating unit 15, reference deformable body 16, reference deformable body information acquiring unit 30, control unit 32, input unit 34 and cine memory 36 as shown in Fig. 1.

[0017] Ultrasonic probe 3 is formed by disposing multiple strips of transducers therein, for transmitting and receiving ultrasonic waves to/from an object by scanning beams mechanically or electronically. Each transducer generally has the function that converts incoming pulse waves or continuous transmitting signals into ultrasonic waves and discharges the converted ultrasonic waves, and the function that converts the reflected echoes discharged from inside of the object into electronic signals (reflected echo signals) and outputs the converted signals.

[0018] Reference deformable body 16 is attached on the ultrasonic wave transmitting/receiving surface of ultrasonic probe 3. Reference deformable body 16 is to be applied on the body surface of the object to give compression. Compressing motion renders transmission/reception of ultrasonic waves via ultrasonic probe, and provides stress distribution to the measuring portion in the body cavity.

[0019] Ultrasonic wave transmission/reception control circuit 1 controls the timing or focus for transmitting and receiving ultrasonic waves. Transmitting circuit 2 produces transmission pulses for generating ultrasonic waves by driving ultrasonic probe 3, and sets the convergent point (focus) of the ultrasonic waves transmitted by an internal transmission phasing and adding circuit at a certain depth. Receiving circuit 4 amplifies the reflected echo signal received by ultrasonic probe 3 at a predetermined gain. The number of reflected echo signals which corresponds to the number of the amplified respective transducers is inputted to phasing and adding circuit 5. Phasing and adding circuit 5 controls the phase of the reflected echo signal amplified in receiving circuit 4, and forms RF signal frame data.

[0020] Signal processing unit 6 and black and white scan converter 7 are provided on one end of the output side of phasing and adding circuit 5. Signal processing unit 6 inputs the RF signal frame data from phasing and adding circuit 5, and executes various signal processing such as gain compensation, log compensation, detection, edge enhancement and filtering.

[0021] Black and white scan converter 7 obtains the RF signal frame data signal processed in signal processing unit 6 at a predetermined cycle, and reads out the tomographic image data based on the RF signal frame data at TV system cycle.

[0022] Also, RF signal frame data selecting unit 8, displacement/strain calculating unit 9, pressure calculating unit 15 and elasticity modulus calculating unit 10 are comprised on the output side of the other end of phasing and adding circuit 5. Also, elasticity data processing unit 11 and color scan converter 12 are comprised on the latter part of elasticity modulus calculating unit 10.

[0023] On the output side of black and white scan converter 7 and color scan converter 12, switching and adding unit 13 is comprised. Image display unit 14 is a monitor for displaying a tomographic image based on the tomographic image data obtained by black and white converter 7 and an elasticity image based on the elasticity image data obtained by the color scan converter. Cine memory 36 on the output side of switching and adding unit 13 is for storing tomographic image data and elasticity image data with time information. The tomographic image data and elasticity image data stored in cine memory 36 are displayed on image display unit 14 according to the command from input unit 34.

[0024] RF signal frame data selecting 8 sequentially stores the RF signal frame data outputted from phasing and adding circuit 5 (the currently stored RF signal frame data is set as RF signal frame data N) in the frame memory provided in RF frame data selecting unit 8, selects one set of RF signal frame data from among the past RF signal frame data N-1, N-2, N-3, ... N-M (the selected data is set as RF signal frame data X), and outputs a pair of RF signal frame data N and RF signal frame data X to displacement/strain calculating unit 9. While RF signal frame data is described above as the signal to be outputted from phasing and adding circuit 5, it may also be the form of I,Q signal which is the complex-demodulated RF signal.

[0025] Displacement/strain calculating unit 9 executes one-dimensional or two-dimensional correlation process based on the pair of RF signal frame data selected by RF signal frame data selecting unit 8, measures displacement or moving vector (direction and size of displacement) of the respective measurement points on a tomographic image, generates displacement frame data, and calculates the strain from the generated strain frame data. The strain is to be calculated, for example, by performing spatial differentiation on the displacement. The moving vector is to be detected, for example, using the block matching method or the gradient method. Block matching method divides an image into

blocks formed by, for example, $N \times N$ pixels, searches the block which is most approximated to the target block in the current frame from the previous frame, and performs encoding referring to the searched blocks.

[0026] Elasticity modulus calculating unit 10 calculates elasticity modulus from the strain information outputted from displacement/strain calculating unit 9 and from the pressure information outputted from pressure calculating unit 15, generates numerical data of the elasticity modulus (elasticity frame data), and outputs the generated data to elasticity data processing unit 11 and color scan converter 12. One of elasticity modulus, for example, Young's modulus Y_m is to be obtained by dividing the stress (pressure) in each calculation point by the strain in each calculation point, as shown in the equation below. In the equation below, the index of i, j represents the coordinate of the frame data.

[Equation 1]

$$Y_{mi,j} = \text{pressure}(\text{stress})_{i,j} / (\text{strain } i,j)$$

$$(i,j = 1, 2, 3 \dots)$$

[0027] Here, the pressure given to the object is measured in pressure measuring unit 15. Pressure measuring unit 15 obtains the pressure given to reference deformable body 16 by calculation, and outputs it as the pressure given to the object. The detail on this step will be described later.

[0028] Elasticity data processing unit 11 executes various image processing such as smoothing process in the coordinate plane of the calculated elasticity frame data, contrast optimization process, or smoothing process among the frames in the time axis direction.

[0029] Color scan converter 12 provides color information on light's three primary colors that are red(R), green(G) and blue (B) to the elasticity frame data outputted from elasticity data processing unit 11. For example, large elasticity modulus is converted into red color code, and small elasticity modulus is converted into blue color code.

[0030] Also, object pressing mechanism 18 moves ultrasonic probe 3 in vertical directions using a device such as motor or wire so as to press the object, or an operator may manually move ultrasonic probe 3 in vertical direction.

(First Embodiment: Manual Input of ID)

[0031] Here, the first embodiment will be described referring to Figs. 1 ~ 5. In the first embodiment, an operator inputs an ID to make an ultrasonic diagnostic apparatus to identify the type of a reference deformable body, for reflecting the type to elasticity calculation or displaying the type. This ID is to be the index for identifying the type of the reference deformable body.

[0032] The ultrasonic diagnostic apparatus of the first embodiment mainly comprises input unit 34 configured to input an ID of reference deformable body 16, control unit 32 configured to make the ID inputted by input unit 34 to be outputted to reference deformable body information acquiring unit 30, reference deformable information acquiring unit 30 configured to acquire the type of reference deformable body 16 corresponding to the outputted ID and to reflect the type of reference deformable body 16 to calculation in pressure calculating unit 15 or elasticity modulus calculating unit 10.

[0033] First, attachment pattern of reference deformable body 16 will be described using Fig. 2. As shown in Fig. 2(a), fixing member 17 is formed by frame body 20 having airspace in the center thereof and a pair of holding units 21 extended downward from the bottom surface of frame body 20. Frame body 20 and holding units 21 are formed being integrated with each other. On holding unit 21, a protruded portion is provided so as to fit in the slot on the side portion of ultrasonic probe 3 (not illustrated in the diagram). Accordingly, fixing member 17 can be mounted to ultrasonic probe 3 through one-touch operation. Also, on the inner-peripheral surface of the airspace in frame body 20, slot portion 22 is provided for holding reference deformable body 16. The width of slot portion 22 is about 3mm, and the depth thereof is about 5mm.

[0034] As shown in Fig. 2(b), reference deformable body 16 has a form wherein rectangle body 26 is provided to the central portion on the upper surface of a square-shaped flat-plate body 25. Rectangle body 26 of reference deformable body 16 has the size which can be protruded from the airspace in fixing member 17. Also, flat-plate body 25 has about 3mm of thickness which can be fit in slot portion 22 of fixing member 17.

[0035] Reference deformable body 16 is formed based on oil-based gel material, water-based gel material such as acrylamide or silicon, etc. Acrylamide is formed as acrylamide gel wherein cross-linking agent (BIS) is polymerized in the presence of catalytic agent. This is polymer gel having 3-dimensional meshed structure, and has texture like agar or gelatin. In this manner, the material that is a liquid solution and gets coagulated over time into a gel after coagulating agent is mixed in is preferable for reference deformable body 16. If it is constituted by the material such as acrylamide having low viscosity, it is suited for pressure measurement since it responds to pressing operation quickly. Also, reference deformable body 16 may also be formed by a material based on aqueous resin gelled substance which is to be used as a phantom for diagnosis using ultrasonic waves.

[0036] Fig. 2(c) shows a pattern wherein reference deformable body 16 is attached to fixing member 17. The end portion of flat-plate body 25 is inserted into slot portion 22 formed on the inner-peripheral surface of frame body 20, and reference deformable body 16 is attached to fixing member 17. Since flat-plate body 25 which is reference deformable body 16 is an elastic body, flat-plate body 25 can be mounted in slot portion 22 using the elasticity. Accordingly, when reference deformable body 16 is attached to fixing member 17, rectangle body 26 of reference deformable body 16 is protruded from frame body 20 of fixing member 17.

[0037] Fig. 2(d) shows the cross-sectional view in the longitudinal direction of the condition that reference deformable body 16 and fixing member 17 are fixed on ultrasonic probe 3. In the condition that reference deformable body 16 is attached to fixing member 17 as shown in Fig. 2(c), fixing member 17 is fixed on ultrasonic probe 3 via holding unit 22. When fixing member 17 is fixed on ultrasonic probe 3, reference deformable body 16 comes to contact transducers 19 provided on the upper part of ultrasonic probe 3. In this condition, the upper surface of reference deformable body 16 is applied to an object, and executes transmission/reception of ultrasonic waves from/to transducers 19.

[0038] Also, as shown in Fig. 3, reference deformable body 16 or package 40 of reference deformable body 16 has ID 40.

(1-1: ID on a reference deformable body)

[0039] Concretely, as shown in Fig. 3(a), ID 40 formed by letters is appended on the side surface of reference deformable body 16. ID 40 is, for example, "BBAC" formed by four alphabetical letters. ID 40 is appended on the side surface (the part which does not contact the object) of reference deformable body 16 to avoid the influence thereof in transmission and reception of ultrasonic waves to/from the object. An operator can identify ID 40 by the order of alphabetical letters through checking ID 40 on the side surface of reference deformable body 16. ID 40 may be presented also by numbers, symbols, figures, colors, and so on.

[0040] Also, as shown in Fig. 3(b), by providing concavity and convexity for imprinting ID40 in advance on a metal mold to form reference deformable body 16 and inpouring gel material of reference deformable body in the metal mold, ID 40 formed by concavity and convexity can be formed on the side surface of reference deformable body 16. The operator can identify ID 40 by seeing or touching the concavity and convexity of ID 40 formed on the side surface of reference deformable body 16. Also, surface treatment such as sawtooth or wave pattern may be worked on the side surface of reference deformable body 16.

[0041] Also, ID 40 may be identified by dyeing reference deformable body 16. For example, if reference deformable body 16 is white ID 40 is set as "BBAC", and if reference deformable body 16 is yellow ID 40 is set as "AAAA".

(1-2: ID on a package)

[0042] As shown in Fig. 3(c), ID 40 may be appended on case 42 which is for packaging reference deformable body 16. Case 42 has case part 46 having airspace therein and cover part 44, and reference deformable body 16 is contained and sealed between case part 46 and cover part 44. By sealing and containing reference deformable body 16 inside of case 42, deterioration of reference deformable body 16 can be minimized by keeping out dust or air.

[0043] The operator can identify the alphabetical letters, i.e. ID 40 of reference deformable body by seeing ID 40 on the case for packaging reference deformable body 16.

(1-3: Manual Input of ID)

[0044] Next, as shown in Fig. 4, the operator inputs ID 40 of reference deformable body 16 or ID 40 described on case 42 for containing reference deformable body 16 to input unit 34. Control unit 32 outputs ID 40 inputted by input unit 34 to reference deformable body information acquiring unit 30, and gives a command to identify the type of reference deformable body 16. Then reference deformable body information acquiring unit 30 identifies the type of reference deformable body 16 from the outputted ID 40, and reflects the type of reference deformable body 16 to calculation to be executed by pressure calculating unit 16 and elasticity modulus calculating unit 10. Also, reference deformable body information acquiring unit 30 displays the type of reference deformable body 16 on image display unit 14.

[0045] In concrete terms, reference deformable body information acquiring unit 30 is formed by ID information receiving unit 50 for receiving the inputted ID 40 of reference deformable body 16, memory 52 for storing a plurality of relationships between IDs 40 of reference deformable body 16 and types of reference deformable body 16 in advance, and type identifying unit 54 for identifying the type of reference deformable body 16 corresponding to the inputted ID 40 based on the information stored in memory 52. Also, in memory 52, one type of reference deformable body (such as thickness, elasticity characteristic, acoustic characteristic and type of the probe) is stored corresponding to one ID 40 as shown in chart 1 below.

[Chart 1]

ID	Thickness (mm)	Elasticity characteristics (N/m)	Acoustic characteristics (N • s/m ³)	Kind of probe (Applying part)
AAAA	8	100	1.5×10^6	Linear type
BAAA	7	100	1.5×10^6	Linear type
BBAA	7	50	1.5×10^6	Linear type
•	•	•	•	•
•	•	•	•	•
DDDD	5	30	1.0×10^6	Intracavitary type

[0046] Here, the thickness of reference deformable body 16 is the thickness of reference deformable body in the transmitting/ receiving direction of ultrasonic waves, and is the initial thickness before applying pressure. Elasticity characteristics indicate elasticity modulus, viscoelasticity modulus, nonlinearity, Poisson's ratio, etc. of reference deformable body 16. In the present embodiment, elasticity modulus is used as elasticity characteristic. Also, acoustic characteristics indicate acoustic velocity, rate of decrease, acoustic impedance, etc. of reference deformable body 16. In the present embodiment, acoustic impedance is used as acoustic characteristic. The type of probe indicates the type of ultrasonic probe 3 to which reference deformable body 16 is attached. For example, there are different types such as linear type of ultrasonic probe 3 for pressing from outside of the body or a convex type of ultrasonic probe 3, or an intracavitary type of ultrasonic probe 3 for pressing from inside of the object's body, and the applying part is to be determined.

[0047] The four alphabetical letters which indicate ID 40 respectively correspond to the type of each reference deformable body 16. The far-left alphabet corresponds to the thickness of each reference deformable body 16. For example, if the far left alphabet is A, it means that the thickness of the reference deformable body is 8mm, B indicates that the thickness of the reference deformable body is 7mm, C indicates that the thickness of the reference deformable body is 6mm, and D indicates that the thickness of the reference deformable body is 5mm. In this manner, the operator can recognize the thickness of reference deformable body 16 by only looking at ID 40. In the same manner, the second left alphabet corresponds to the elasticity characteristics. The third left alphabet corresponds to the acoustic characteristic, and the far-right alphabet corresponds to the type of ultrasonic probe to which reference deformable body 16 is attached.

[0048] Then kind identifying unit 54 identifies the kind of reference deformable body 16 corresponding to the inputted ID 40 by reading it out from memory 52. Input unit 34 may also input the information on characteristics (for example, elasticity characteristics, etc. of reference deformable body 16) of reference deformable body 16 instead of ID 40.

(1-4: Pressure Measurement)

[0049] Type identifying unit 54 outputs the type of reference deformable body 16 to pressure calculating unit 15. Pressure calculating unit 15 detects the thickness and the elasticity modulus in particular from among the types of reference deformable body 16 (thickness, elasticity characteristics, acoustic characteristics, type of probe, etc.) outputted from reference deformable body information acquiring unit 30. The detected thickness is the initial thickness of reference deformable body 16 before pressure is applied to the object.

[0050] Pressure calculating unit 15 obtains the strain of reference deformable body 16 deformed by the pressure applied to the object, from the RF signal frame data outputted from RF signal frame data selecting unit 8. In concrete terms, pressure calculating unit 15 first extracts the RF signal frame data in the region including the border between the object and reference deformable body 16. Then it obtains the coordinate of the border between the object and reference deformable body 16 based on the extracted RF signal frame data. For example, the threshold value is set with respect to the amplitude of the signal wave pattern of the RF signal frame data including the border, the threshold value is set as original point 0 in the depth direction (contact plane of the transducer and reference deformable body 16), and the coordinate wherein the amplitude of the waveform of the RF signal frame data first surpasses the threshold value from in the depth direction from the original point is detected as the coordinate of the border.

[0051] While the border between the object and reference deformable body 16 is detected above based on the RF signal frame data, the tomographic image data outputted from black and white scan converter 16 may also be used for detecting the border. Fig. 5(a) shows the condition of reference deformable body 16 before pressure is applied on the object. Fig. 5(b) shows the condition of reference deformable body 16 after pressure is applied on the object. Pressure calculating unit 15 detects the coordinate of the border in the tomographic image based on the difference of the acoustic

characteristics (acoustic velocity, rate of decrease and acoustic impedance) between tissue 1 and reference deformable body 16.

[0052] Then pressure calculating unit 15 associates the initial thickness of reference deformable body 16 before pressure is applied with the coordinate of the border. Also, pressure calculating unit 15 calculates the displacement of reference deformable body 16 from the coordinate of the border after pressure is applied, based on the association between the initial thickness and the coordinate of the border. Pressure calculating unit 15 then calculates the strain from the calculated displacement and the initial thickness.

[0053] Also, elasticity modulus (a part of elasticity characteristics) of reference deformable body 16 is identified by type identifying unit 54 based on ID 40. Consequently, by setting P as (pressure (stress)), Y as (elasticity modulus) and δd as (strain), their relationship can be expressed by the following equation.

[Equation 2]

$$P(\text{pressure}(\text{stress})) = Y(\text{elasticity modulus}) \times \delta d(\text{strain})$$

[0054] Pressure calculating unit 15 can obtain the pressure in the border between the object and reference deformable body 16 based on the above-mentioned equation 2.

(1-5: Calculation of Elasticity Modulus)

[0055] Elasticity modulus calculating unit 10 calculates elasticity modulus based on the above equation 1 from the strain information outputted from displacement/strain calculating unit 9 and the pressure information outputted from pressure calculating unit 15, and generates numerical data (elasticity frame data) of the elasticity modulus. Elasticity modulus calculating unit 10 outputs the elasticity frame data to elasticity data processing unit 11.

[0056] Color scan converter 12 appends hue information to the elasticity frame data outputted from elasticity data processing unit 11, and image display unit 14 displays the elasticity image based on the elasticity image data acquired by the color scan converter. Though not shown in the diagram, image display unit 14 may also display the elasticity modulus outputted from elasticity modulus calculating unit 10 by numerical values.

[0057] As described above, in accordance with the present embodiment, it is possible to identify the type of reference deformable body 16 by ID 40, and to reflect the identified information on elasticity calculation, whereby calculation of elasticity can be more stable.

(1-6: ID Display)

[0058] Also, type identifying unit 54 outputs the type of reference deformable body 16 or ID 40 to cine memory 36. Cine memory 36 stores the type of reference deformable body 16 or the information on ID 40 along with the elasticity image or tomographic image. Image display unit 14 outputs the type of reference deformable body 16 or the information on ID 40 along with the elasticity image or tomographic image from cine memory 36 and displays them. In this manner, the type of the reference deformable body or ID 40 can be displayed.

[0059] The operator can execute the setting of ultrasonic waves properly since the type of reference deformable body 16 or ID 40 can be identified. Also, after performing the ultrasonic diagnosis, he/she can identify which type of reference deformable body was used for obtaining the elasticity image or tomographic image upon reviewing the elasticity image or tomographic image obtained by applying reference deformable body 16.

[0060] Also, dedicated information on ultrasonic probe 3 is appended to ID 40 as shown in chart 1. Though not shown in the diagram, it is possible to set the procedure to display the warning or to make sounds when reference deformable body 16 is applied to a nondedicated ultrasonic probe 3 and transmission/ reception of ultrasonic waves is executed.

(Second Embodiment: ID Automatic Identification)

(2-1: Echo Luminance)

[0061] Here, the second embodiment will be described using Fig. 6 ~ Fig. 9. The difference from the first embodiment is that ID 40 of reference deformable body 16 is automatically identified.

[0062] Reference deformable body information identifying unit 30 is formed by image analyzing unit 60 configured to the tomographic image stored in cine memory 36, memory 52 configured to store the relationship between a plurality of IDs 40 of reference deformable body 16 and feature quantity of the tomographic image of reference deformable body 16 in advance, and type identifying unit 54 configured to identify the type of reference deformable body 16 corresponding

to the inputted tomographic image based on the information stored in memory 52.

[0063] Reference deformable body 16 includes, for example, a scatterer. Image analyzing unit 60 analyses the echo luminance in the tomographic image of reference deformable body 16 in which the scatterer outputted from cine memory 36 is included. The memory 52 stores plural echo luminance (0 ~ 255) of reference deformable body 16 by associating them with ID 40 respectively. For example, as shown in chart 2, it is assumed that there are two kinds (ID 40: α, β) of reference deformable bodies 16 having different elasticity modulus or scatterer concentration that are stored in memory 52. It is also assumed that the ultrasonic waves are transmitted/received to/from the respective reference deformable bodies 16 in the same condition.

[Chart 2]

ID	Elasticity modulus (kPa)	Scatterer concentration (%)	Echo luminance (0~255)	Thickness (mm)
α	10	1	50	8
β	20	3	100	7

[0064] Figs. 7 are tomographic images in the case that reference deformable body 16 (α, β) in which scatterer is included is attached. Fig. 7(a) is a tomographic image in the case that reference deformable body 16 having α as ID 40 is attached, and Fig. 7(b) is a tomographic image in the case reference deformable body 16 having β as ID 40 is attached.

[0065] The echo luminance of reference deformable body 16 is displayed in the region where is shallow in depth (for example, 0 ~ 5mm) in the tomographic image. Image analyzing unit 60 analyzes the echo luminance in the shallow region of the tomographic image stored in cine memory 36. For example, image analyzing unit 60 sets ROI 70 in reference deformable body 16 of the tomographic image, and analyzes the luminance information in ROI 70. This ROI 70 is set via input unit 34 as one chooses. Also, it may be set so that ROI 70 is automatically set in the region which is shallow in depth (for example, 0 ~ 5mm) in the tomographic image.

[0066] Image analyzing unit 60 analyzes statistical characteristics of the echo luminance such as the average value or dispersion value of the echo luminance in ROI 70. Then type identifying unit 54 reads out the type of reference deformable body 16 corresponding to the characteristics of the echo luminance in the analyzed tomographic image from memory 52 and identifies it.

[0067] In concrete terms, if the average value of the echo luminance in ROI 70 is "50", type identifying unit 54 identifies that ID 40 of reference deformable 16 is α . Also, if the average value of the echo luminance in ROI 70 is "100", type identifying unit 54 identifies that ID 40 of the reference deformable body is β .

[0068] Then type identifying unit 54 outputs the type (here, elasticity modulus, scatterer concentration, echo luminance and thickness) or ID 40 of reference deformable body 16 to cine memory 36. Cine memory 36 stores the information on the type or ID 40 of reference deformable body 16 along with the elasticity image or tomographic image. Image display unit 14 outputs the information on the type or ID 40 of reference deformable body 16 along with the elasticity image or tomographic image from cine memory 36, and displays them. Accordingly, the operator can identify the type or ID 40 of reference deformable body, and set ultrasonic waves appropriately. Also, he/she can identify the type of reference deformable body 16 used for obtaining the elasticity image or tomographic image.

[0069] Also, as in the same manner as the first embodiment, elasticity modulus may be calculated based on the type of reference deformable body 16. Type identifying unit 54 outputs the type of reference deformable body 16 to pressure calculating unit 15, and pressure calculating unit 15 calculates the pressure. Then elasticity modulus calculating unit 10 calculates elasticity modulus from the strain information outputted from displacement/strain calculating unit 9 and the pressure information outputted from pressure calculating unit 15, and generates the numerical data (elasticity frame data) of the elasticity modulus. Image display unit 14 displays the elasticity image or elasticity modulus based on the generated elasticity frame data.

(2-2: Attenuation Characteristics)

[0070] While the type of reference deformable body 16 is identified above from the average value of the echo luminance in reference deformable body 16, there are cases, for example, that approximately average echo luminance is distributed even when the scatterer concentration of reference deformable body 16 is greatly different.

[0071] Given this factor, type identifying unit 54 may identify the type of reference deformable body 16 from attenuation characteristic of reference deformable body 16. Attenuation characteristic is the feature that ultrasonic waves attenuate in proportion to the scatterer concentration. Image analyzing unit 60 analyzes the attenuation characteristics from distribution of the intensity of echo luminance in reference deformable body 16. The intensity of echo luminance in reference deformable body 16 has the characteristic that it attenuates as moving from the shallow depth portion to the deep portion.

[0072] When the ultrasonic waves having low transmitting voltage are transmitted/received to/from ultrasonic probe

3 and the scatterer concentration of reference deformable body 16 is high, attenuation rate is great and the intensity of echo luminance attenuates drastically. ID 40 in this condition is set as α . Also, when the ultrasonic waves having high transmitting voltage are transmitted/received to/from ultrasonic probe 3 and the scatterer concentration is low, attenuation rate is small and the intensity of echo luminance attenuates gradually. ID 40 of this reference deformable body 16 is set as β . The relationship between the attenuation of reference deformable body 16 and ID 40 is stored in memory 52.

[0073] Image analyzing unit 60 analyzes the attenuation rate from the distribution of the intensity in echo luminance of the scatterer in ROI 70. Then type identifying unit 54 reads out and identifies the type of reference deformable body 16 corresponding to the attenuation rate from memory 52. Type identifying unit 54, in the case that the attenuation rate in ROI 70 is high, identifies that ID 40 of reference deformable body 16 is α . In the case that the attenuation rate in ROI is low, it identifies that ID 40 of reference deformable body 16 is β .

(2-3: Pattern of Scatterer)

[0074] Also, type identifying unit 54 may identify the type of reference deformable body 16 from density distribution (rarefaction density) of scatterer in reference deformable body 16.

[0075] For example, in the case that density distribution of the scatterer of reference deformable body 16 gets higher as it moves from the shallow region to the deep region, ID 40 of reference deformable body 16 is set as α . In the case that the density distribution of the scatterer of reference deformable body 16 gets lower as it moves from the shallow region to the deep region, ID 40 of reference deformable body 16 is set as β . The relationship between the scatterer distribution of reference deformable body 16 and ID 40 is to be stored in memory 52.

[0076] Image analyzing unit 60 analyzes density distribution of the scatterer from the echo luminance in ROI 70. Then type identifying unit 54 reads out and identifies the type of reference deformable body 16 corresponding to the density distribution of the analyzed scatterer from memory 52.

[0077] Type identifying unit 54, in the case that the echo luminance in ROI 70 gets lower as it moves from the shallow region to the deep region, identifies that ID 40 of reference deformable body 16 is α . Type identifying unit 54, in the case that the echo luminance in ROI 70 gets higher as it moves from the shallow region to the deep region, identifies that ID 40 of reference deformable body 16 is β . Type identifying unit 54 may also identify the type of reference deformable body 16 based on discreteness (dispersion in normal distribution) of the echo luminance distribution in the scatterer of reference deformable body 16.

(2-4: Size and Form of Scatterer)

[0078] Also, deformable body type identifying unit 54 may identify the type of reference deformable body 16 from the size of the scatterer. For example, when the size of the scatterer included in reference deformable body 16 is $5\mu\text{m}$, ID 40 of reference deformable body 16 is set as α . When the size of the scatterer included in reference deformable body 16 is $10\mu\text{m}$, ID 40 of reference deformable body is set as β . At this time, it is to be assumed that a plurality of scatterers having even size are included in reference deformable body 16. The relationship between the size of the scatterer in reference deformable body 16 and ID 40 is stored in memory 52.

[0079] Image analyzing unit 60 analyzes the size of the scatterer from echo luminance in ROI 70. Then type identifying unit 54 reads out and identifies the type of reference deformable body 16 corresponding to the size ($5\mu\text{m}$ or $10\mu\text{m}$) of the analyzed scatterer. Also, deformable body type identifying unit 54 can also identify the form of the scatterer in reference deformable body 16 using the pattern matching method. It is set so that the form of the scatterer is different for each ID 40 of reference deformable body 16.

[0080] The relationship between the form of the scatterer of reference deformable body and ID 40 is stored in memory 52. Image analyzing unit 60 analyzes the form of the scatterer from the echo luminance in ROI 70. Then type specifying unit 54 executes the pattern matching method between the form of the scatterer stored in memory 54 and the form of the analyzed scatterer. Type identifying unit 54 reads out and identifies the type of reference deformable body 16 including the best matched scatterer stored in the memory.

(2-5: Layer and Barcode)

[0081] Also, deformable body type identifying unit 54 may identify the type by the pattern or barcode of reference deformable body 16. As shown in Fig. 8, reference deformable body 16 is assumed to be formed by a plurality of different kinds of layers (layer 1 and layer 2). Layer 1 is on the side of ultrasonic probe 3, and layer 2 is on the side of the object.

[0082] As shown in Fig. 8(a), in the case that the ratio between layer 1 and layer 2 of reference deformable body 16 is (layer 1:layer 2 = 1:2), ID 40 of reference deformable body 16 is set as α . As shown in Fig. 8(b), in the case that the ratio thereof is (layer 1:layer 2 = 1:1), ID 40 of reference deformable body is set as β . The relationship between the ratio between the layers of reference deformable body 16 and ID 40 is stored in memory 52.

[0083] Image analyzing unit 60 analyzes the ratio between layer 1 and layer 2 of reference deformable body 16 from the echo luminance of an elasticity image. In concrete terms, image analyzing unit 60 detects the border between layer 1 and layer 2, and the border between layer 2 and tissue 1 based on the echo luminance. Then image analyzing unit 60 detects the height of layer 1 and layer 2 in the depth direction from the respective borders. Type identifying unit 54 then reads out and identifies ID 40 of reference deformable body 16 corresponding to the detected ratio between layer 1 and layer 2 from memory 52.

[0084] Also, as shown in Fig. 9, it is assumed that mark 72 formed by barcodes is appended to the side of reference deformable body 16. As shown in Fig. 9(a), in the case that reference deformable body 16 includes one strip of barcode, ID 40 of reference deformable body 16 is set as α . As shown in Fig. 9(b), in the case that reference deformable body 16 includes two strips of barcodes, ID 40 of reference deformable body 16 is set as β . The relationship between the number of strips in barcode and ID 40 of reference deformable body 16 is stored in memory 52. The echo luminance of barcode should be different from the echo luminance of reference deformable body 16. The array direction of the barcode is the major-axis direction or minor-axis direction of reference deformable body 16.

[0085] Image analyzing unit 60 analyzes the number of strips of barcode in reference deformable body 16 from the echo luminance of the elasticity image. Then type identifying unit 54 reads out and identifies ID 40 of reference deformable body 16 corresponding to the analyzed number of strips of barcode from memory 52.

[0086] While barcode is used as mark 72 here, a concave portion or notch may also be used. Also, by stretching a very thin string (for example, a fish line) inside of reference deformable body 16 along the minor-axis direction of reference deformable body 16, the information on the number of the strings or interval between the strips may be also used as mark 72.

(Third Embodiment: Image Processing)

[0087] The third embodiment will now be described referring to Figs. 10 and 11. The difference from the first embodiment and the second embodiment is that image processing is executed by identifying the type of reference deformable unit 16.

[0088] As shown in Fig. 10, reference deformable body information acquiring unit 30 has image processing unit 62 for executing image processing with respect to the tomographic image (or elasticity image) stored in cine memory 36, in addition to the above-described image analyzing unit 60, memory 52 and type identifying unit 54.

[0089] Type identifying unit 54 outputs ID 40 of reference deformable body 16 (includes thickness, elasticity characteristics, acoustic characteristics, kind of probe, etc.) to image processing unit 62. Image processing unit 62 detects thickness from ID 40.

[0090] As shown in Fig. 11, image processing unit 62 shifts the tomographic image toward the upper direction (the side of ultrasonic probe 3) according to the "thickness" of reference deformable body 16 so as not to display reference deformable body 16. Fig. 11(a) shows the tomographic image before the correction, and Fig. 11(b) shows the tomographic image after the correction.

[0091] In concrete terms, as shown in Chart 1, if ID 40 identified in type identifying unit 54 is AAAA, the thickness of reference deformable body 16 is 8mm. Image processing unit 62 loads the thickness information of the reference deformable body from type identifying unit 54, and shifts the tomographic image stored in cine memory 36 in the upper direction by 8mm. If ID 40 is BAAA, the thickness of reference deformable unit 16 is 7mm. Image processing unit 62 loads thickness information of the reference deformable body from type identifying unit 54, and shifts the tomographic image stored in cine memory 36 in the upper direction by 7mm.

[0092] In this manner, as shown in Fig. 11(b), since reference deformable body 16 is not displayed on image display unit 14, it is possible to broaden the display region of tissue 5 in the deep portion.

(Fourth Embodiment: Focus only on the Thickness Portion)

[0093] Here, the fourth embodiment will be described. The difference from the first embodiment ~ the third embodiment is that transmission and reception of ultrasonic waves is controlled by identifying ID 40 of reference deformable body 16.

[0094] In the present embodiment, though not shown in the diagram, reference deformable body information acquiring unit 30 is connected with ultrasonic-wave transmission/reception control circuit 1.

[0095] Type identifying unit 54 outputs ID 40 of reference deformable body 16 (includes thickness, elasticity characteristics, acoustic characteristics, kind of probe, etc.) to ultrasonic-wave transmission/reception control circuit 1. Ultrasonic-wave transmission/reception control circuit 1 detects "thickness" from ID 40. Then ultrasonic-wave transmission/reception control circuit 1 controls focus of the ultrasonic waves according to the thickness so that the ultrasonic waves will not be focused on reference deformable body 16.

[0096] In concrete terms, as shown in Chart 1, if ID 40 identified in type identifying unit 54 is AAAA, the thickness of reference deformable body 16 is 8mm. Ultrasonic-wave transmission/reception circuit 1 loads the thickness information of the reference deformable body from type identifying unit 54, and controls transmission circuit 2 and receiving circuit

4 so that ultrasonic waves will be focused at the depth deeper than 8mm to avoid ultrasonic waves from being focused on reference deformable body 16.

[0097] Accordingly, since ultrasonic waves are focused on tissues 1~5 of the object, image display unit 14 can display the tomographic image appropriately. The invention is set out in the following claims:

Claims

1. An ultrasonic diagnostic apparatus comprising:

an ultrasonic probe (3) comprising an ultrasonic transmitting and receiving surface and a reference deformable body (16) attached on said surface and including a scatterer;
 a tomographic image constructing unit configured to transmit and receive ultrasonic waves to and from an object to be examined via the reference deformable body (16), and generate a tomographic image based on a RF signal frame data of a cross-sectional region of the object;
 a display unit (14) configured to display the tomographic image;
 a storing unit (52) configured to store the relationship between an ID (40) appended to the reference deformable body (16) and a type of the reference deformable body (16);
 a type identifying unit (54) configured to read out a type of the reference deformable body (16) corresponding to the ID (40) of the reference deformable body (16) which is attached to the ultrasonic probe (3), and identify the type of the reference deformable body (16); and
 an image analyzing unit (60) configured to analyze a feature quantity of the reference deformable body (16) in the tomographic image, **characterized in that:**
 the storing unit (52) is adapted to store the relationship between the analyzed feature quantity of the reference deformable body (16) and a type of the reference deformable body (16), and
 the type identifying unit (54) is adapted to read out the type of the reference deformable body (16) corresponding to the feature quantity of the reference deformable body (16) in a newly-obtained tomographic image, and identify the type of the reference deformable body (16), and **in that:**

the feature quantity is the average value of the echo luminance in the tomographic image, and the type identifying unit (54) is adapted to identify the type of the reference deformable body (16) based on the average value of the echo luminance in a newly-obtained tomographic image; or
 the feature quantity is the echo luminance of the scatterer included in the reference deformable body (16), and the type identifying unit (54) is adapted to identify the type of the reference deformable body (16) based on the pattern, size or form of the scatterer in a newly-obtained tomographic image.

2. The ultrasonic diagnostic apparatus according to claim 1, wherein a type of the reference deformable body (16) includes at least one of thickness of the reference deformable body (16), elasticity characteristics including elasticity modulus, acoustic characteristics, scatterer concentration and the ultrasonic probe (3) to be attached.

3. The ultrasonic diagnostic apparatus according to claim 1, wherein the display unit (14) is adapted to display at least one of an ID (40) of the reference deformable body (16) which is identified in the type identifying unit (54) or type of the reference deformable body (16).

4. The ultrasonic diagnostic apparatus according to claim 1, **characterized in that** the ID (40) is appended at least to one of the reference deformable body (16).

5. The ultrasonic diagnostic apparatus according to claim 1, **characterized in** further comprising:

a pressure calculating unit (15) configured to read out information on thickness and elasticity modulus from among the types of the reference deformable body (16) stored in the type identifying unit (54), and calculate the pressure applied on the reference deformable body (16);
 a strain calculating unit (9) configured to calculate strain of a tissue in the cross-sectional region based on the RF signal frame data; and
 an elasticity modulus calculating unit (10) configured to calculate elasticity modulus of the tissue based on the calculated pressure and strain.

6. The ultrasonic diagnostic apparatus according to claim 5, wherein the pressure calculating unit (15) is adapted to

calculate the pressure applied to the reference deformable body (16) based on the strain and the elasticity modulus obtained from the thickness and displacement of the reference deformable body (16).

7. The ultrasonic diagnostic apparatus according to claim 5, **characterized in** further comprising an elasticity image constructing unit (11) configured to generate an elasticity image based on the elasticity modulus of a tissue calculated by the elasticity modulus calculating unit (10).
8. The ultrasonic diagnostic apparatus according to claim 1, **characterized in** further comprising an image processing unit (62) configured to shift a tomographic image or elasticity image toward the side of the ultrasonic probe (3), in accordance with the thickness of the reference deformable body (16) identified by the type identifying unit (54).
9. The ultrasonic diagnostic apparatus according to claim 1, **characterized in** further comprising an ultrasonic-wave transmission/reception control unit (1) configured to control focus of the ultrasonic wave so that the ultrasonic wave is not focused on the reference deformable body (16), in accordance with the thickness of the reference deformable body (16) identified by the type identifying unit (54).

Patentansprüche

1. Ultraschall Diagnosegerät mit einer Ultraschallsonde (3) mit einer Ultraschallsende- und -empfangsfläche und einem deformierbaren Referenzkörper (16), der auf der Fläche befestigt ist und ein Streuelement aufweist, einer Tomographiebild-Erstelleinheit, die dazu eingerichtet ist, Ultraschallwellen über den deformierbaren Referenzkörper (16) zu einem zu untersuchenden Objekt zu senden und von diesem zu empfangen, und basierend auf HF-Signalrahmendaten eines Querschnittsbereichs des Objekts ein Tomographiebild zu erzeugen, einer Anzeigeeinheit (14), die dazu eingerichtet ist, das Tomographiebild anzuzeigen, einer Speichereinheit (52), die dazu eingerichtet ist, das Verhältnis zwischen einer an dem deformierbaren Referenzkörper (16) angebrachten ID (40) und eines Typs des deformierbaren Referenzkörpers (16) zu speichern, einer Typenidentifikationseinheit (54), die dazu eingerichtet ist, einen Typ des deformierbaren Referenzkörpers (16) auszulesen, der der ID (40) des deformierbaren Referenzkörpers (16) entspricht, der an der Ultraschallsonde (3) befestigt ist, und den Typ des deformierbaren Referenzkörpers (16) zu identifizieren, und einer Bildanalyseeinheit (60), die dazu eingerichtet ist, eine Merkmalsgröße des deformierbaren Referenzkörpers (16) in dem Tomographiebild zu analysieren, **dadurch gekennzeichnet, dass** die Speichereinheit (52) dazu ausgelegt ist, die Beziehung zwischen der analysierten Merkmalsgröße des deformierbaren Referenzkörpers (16) und eines Typs des deformierbaren Referenzkörpers (16) zu speichern, und die Typenidentifikationseinheit (54) dazu ausgelegt ist, den Typ des deformierbaren Referenzkörpers (16) auszulesen, der der Merkmalsgröße des deformierbaren Referenzkörpers (16) in einem neu erhaltenen Tomographiebild entspricht, und den Typ des deformierbaren Referenzkörpers (16) zu identifizieren, und dadurch, dass die Merkmalsgröße der Durchschnittswert der Echo-Luminanz in dem Tomographiebild ist, und die Typenidentifikationseinheit (54) dazu ausgelegt ist, den Typ des deformierbaren Referenzkörpers (16) basierend auf dem Durchschnittswert der Echo-Luminanz in einem neu erhaltenen Tomographiebild zu identifizieren, oder die Merkmalsgröße die Echo-Luminanz des in dem deformierbaren Referenzkörper (16) enthaltenen Streuelements ist, und die Typenidentifikationseinheit (54) dazu ausgelegt ist, den Typ des deformierbaren Referenzkörpers (16) basierend auf Muster, Größe oder Form des Streuelements in einem neu erhaltenen Tomographiebild zu identifizieren.
2. Ultraschall Diagnosegerät nach Anspruch 1, wobei ein Typ des deformierbaren Referenzkörpers (16) die Dicke des deformierbaren Referenzkörpers (16), eine das Elastizitätsmodul einschließende Elastizitätscharakteristik, eine Akustikcharakteristik, eine Streuelementkonzentration und/oder die zu befestigende Ultraschallsonde (3) einschließt.
3. Ultraschall Diagnosegerät nach Anspruch 1, wobei die Anzeigeeinheit (14) dazu ausgelegt ist, eine ID (40) des deformierbaren Referenzkörpers (16), der in der Typenidentifikationseinheit (54) identifiziert ist, und/oder den Typ des deformierbaren Referenzkörpers (16) anzuzeigen.
4. Ultraschall Diagnosegerät nach Anspruch 1, **dadurch gekennzeichnet, dass** die ID (40) an dem deformierbaren Referenzkörper (16) angebracht ist.

5. Ultraschall Diagnosegerät nach Anspruch 1, **dadurch gekennzeichnet, dass** es ferner aufweist:

eine Druckberechnungseinheit (15), die dazu eingerichtet ist, Information über die Dicke und das Elastizitätsmodul unter den Typen des deformierbaren Referenzkörpers (16) auszulesen, die in der Typenidentifikationseinheit (54) gespeichert sind, und den auf den deformierbaren Referenzkörper (16) ausgeübten Druck zu berechnen,

eine Spannungsberechnungseinheit (9), die dazu eingerichtet ist, die Spannung eines Gewebes in dem Querschnittsbereich basierend auf den HF-Signalrahmendaten zu berechnen, und

eine Elastizitätsmodul-Berechnungseinheit (10), die dazu eingerichtet ist, das Elastizitätsmodul des Gewebes basierend auf dem berechneten Druck und der berechneten Spannung zu berechnen.

6. Ultraschall Diagnosegerät nach Anspruch 5, wobei die Druckberechnungseinheit (15) dazu ausgelegt ist, den auf den deformierbaren Referenzkörper (16) ausgeübten Druck basierend auf der Spannung und dem Elastizitätsmodul zu berechnen, die aus der Dicke und der Verschiebung des deformierbaren Referenzkörpers (16) erhalten wurden.

7. Ultraschall Diagnosegerät nach Anspruch 5, **dadurch gekennzeichnet, dass** es ferner eine Elastizitätsbild-Erstellungseinheit (11) aufweist, die dazu eingerichtet ist, ein Elastizitätsbild basierend auf dem Elastizitätsmodul eines Gewebes zu erzeugen, das durch die Elastizitätsmodul-Berechnungseinheit (10) berechnet wurde.

8. Ultraschall Diagnosegerät nach Anspruch 1, **dadurch gekennzeichnet, dass** es ferner eine Bildverarbeitungseinheit (62) aufweist, die dazu eingerichtet ist, ein Tomographiebild oder ein Elastizitätsbild gemäß der Dicke des deformierbaren Referenzkörpers (16), der durch die Typenidentifikationseinheit (54) identifiziert wurde, hin zu der Seite der Ultraschallsonde (3) zu verschieben.

9. Ultraschall Diagnosegerät nach Anspruch 1, **dadurch gekennzeichnet, dass** es ferner eine Ultraschallwellen-Sende/Empfangs-Steuereinheit (1) aufweist, die dazu eingerichtet ist, gemäß der Dicke des deformierbaren Referenzkörpers (16), der durch die Typenidentifikationseinheit (54) identifiziert wurde, den Fokus der Ultraschallwellen so zu steuern, dass die Ultraschallwelle nicht auf den deformierbaren Referenzkörper (16) fokussiert ist.

Revendications

1. Appareil de diagnostic à ultrasons comprenant :

une sonde (3) à ultrasons comprenant une surface de transmission et de réception d'ultrasons et un corps déformable de référence (16) fixé sur ladite surface et incluant un diffuseur ;

une unité de construction d'image tomographique configurée pour transmettre et recevoir des ondes ultrasonores vers un et d'un objet à examiner par l'intermédiaire du corps déformable de référence (16), et générer une image tomographique sur la base de données de trames de signal RF d'un région en coupe transversale de l'objet ;

une unité (14) d'affichage configurée pour afficher l'image tomographique ;

une unité (52) de stockage configurée pour stocker la relation entre un ID (40) annexé au corps déformable de référence (16) et un type du corps déformable de référence (16) ;

une unité (54) d'identification de type configurée pour lire un type du corps déformable de référence (16) correspondant à l'ID (40) du corps déformable de référence (16) qui est fixé à la sonde (3) à ultrasons, et identifier le type du corps déformable de référence (16) ; et

une unité (60) d'analyse d'image configurée pour analyser une quantité de caractéristiques du corps déformable de référence (16) dans l'image tomographique,

caractérisé en ce que :

l'unité (52) de stockage est adaptée à stocker la relation entre la quantité de caractéristiques analysée du corps déformable de référence (16) et un type du corps déformable de référence (16), et

l'unité (54) d'identification de type est adaptée à lire le type du corps déformable de référence (16) correspondant à la quantité de caractéristiques du corps déformable de référence (16) dans une image tomographique nouvellement obtenue, et identifier le type du corps déformable de référence (16),

et **en ce que :**

la quantité de caractéristiques est la valeur moyenne de la luminance d'échos dans l'image tomogra-

phique, et l'unité (54) d'identification de type est adaptée à identifier le type du corps déformable de référence (16) sur la base de la valeur moyenne de la luminance d'échos dans une image tomographique nouvellement obtenue ; ou

la quantité de caractéristiques est la luminance d'échos du diffuseur inclus dans le corps déformable de référence (16), et l'unité (54) d'identification de type est adaptée à identifier le type du corps déformable de référence (16) sur la base du motif, de la taille ou de la forme du diffuseur dans une image tomographique nouvellement obtenue.

2. Appareil de diagnostic à ultrasons selon la revendication 1, dans lequel un type du corps déformable de référence (16) inclut au moins une parmi l'épaisseur du corps déformable de référence (16), des caractéristiques d'élasticité incluant un module d'élasticité, des caractéristiques acoustiques, une concentration de diffuseur et la sonde (3) à ultrasons devant être fixée.

3. Appareil de diagnostic à ultrasons selon la revendication 1, dans lequel l'unité (14) d'affichage est adaptée à afficher au moins un parmi un ID (40) du corps déformable de référence (16) qui est identifié dans l'unité (54) d'identification de type ou un type du corps déformable de référence (16).

4. Appareil de diagnostic à ultrasons selon la revendication 1, **caractérisé en ce que** l'ID (40) est annexé au corps déformable de référence (16).

5. Appareil de diagnostic à ultrasons selon la revendication 1, **caractérisé en ce que** comprenant en outre :

une unité (15) de calcul de pression configurée pour lire des informations sur l'épaisseur et le module d'élasticité parmi les types du corps déformable de référence (16) stockés dans l'unité (54) d'identification de type, et calculer la pression appliquée sur le corps déformable de référence (16) ;

une unité (9) de calcul de déformation configurée pour calculer une déformation d'un tissu dans la région en coupe transversale sur la base des données de trames de signal RF ; et

une unité (10) de calcul de module d'élasticité configurée pour calculer le module d'élasticité du tissu sur la base de la pression et de la déformation calculées.

6. Appareil de diagnostic à ultrasons selon la revendication 5, dans lequel l'unité (15) de calcul de pression est adaptée à calculer la pression appliquée au corps déformable de référence (16) sur la base de la déformation et du module d'élasticité obtenus à partir de l'épaisseur et du déplacement du corps déformable de référence (16).

7. Appareil de diagnostic à ultrasons selon la revendication 5, **caractérisé en ce que** comprenant en outre une unité (11) de construction d'image d'élasticité configurée pour générer une image d'élasticité sur la base du module d'élasticité d'un tissu calculé par l'unité (10) de calcul de module d'élasticité.

8. Appareil de diagnostic à ultrasons selon la revendication 1, **caractérisé en ce que** comprenant en outre une unité (62) de traitement d'image configurée pour décaler une image tomographique ou une image d'élasticité vers le côté de la sonde (3) à ultrasons, en fonction de l'épaisseur du corps déformable de référence (16) identifié par l'unité (54) d'identification de type.

9. Appareil de diagnostic à ultrasons selon la revendication 1, **caractérisé en ce que** comprenant en outre une unité (1) de commande de transmission/réception d'onde ultrasonore configurée pour commander une focalisation de l'onde ultrasonore de manière à ce que l'onde ultrasonore ne soit pas focalisée sur le corps déformable de référence (16), en fonction de l'épaisseur du corps déformable de référence (16) identifié par l'unité (54) d'identification de type.

FIG. 1

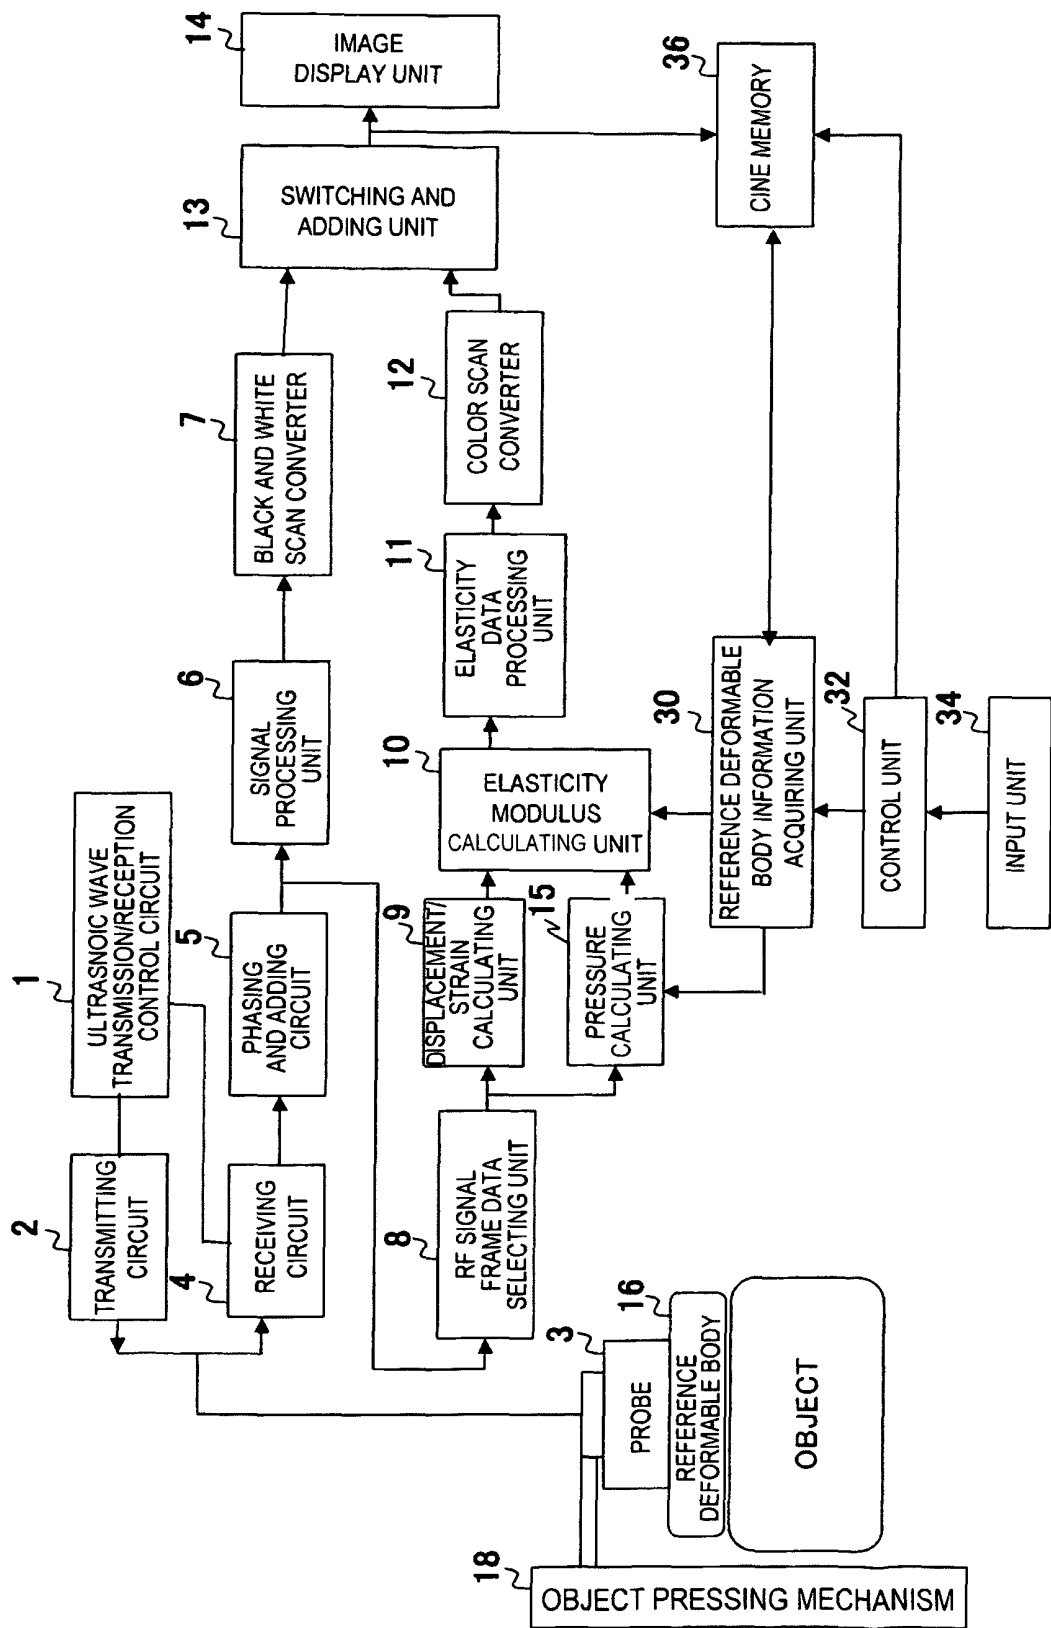


FIG. 2

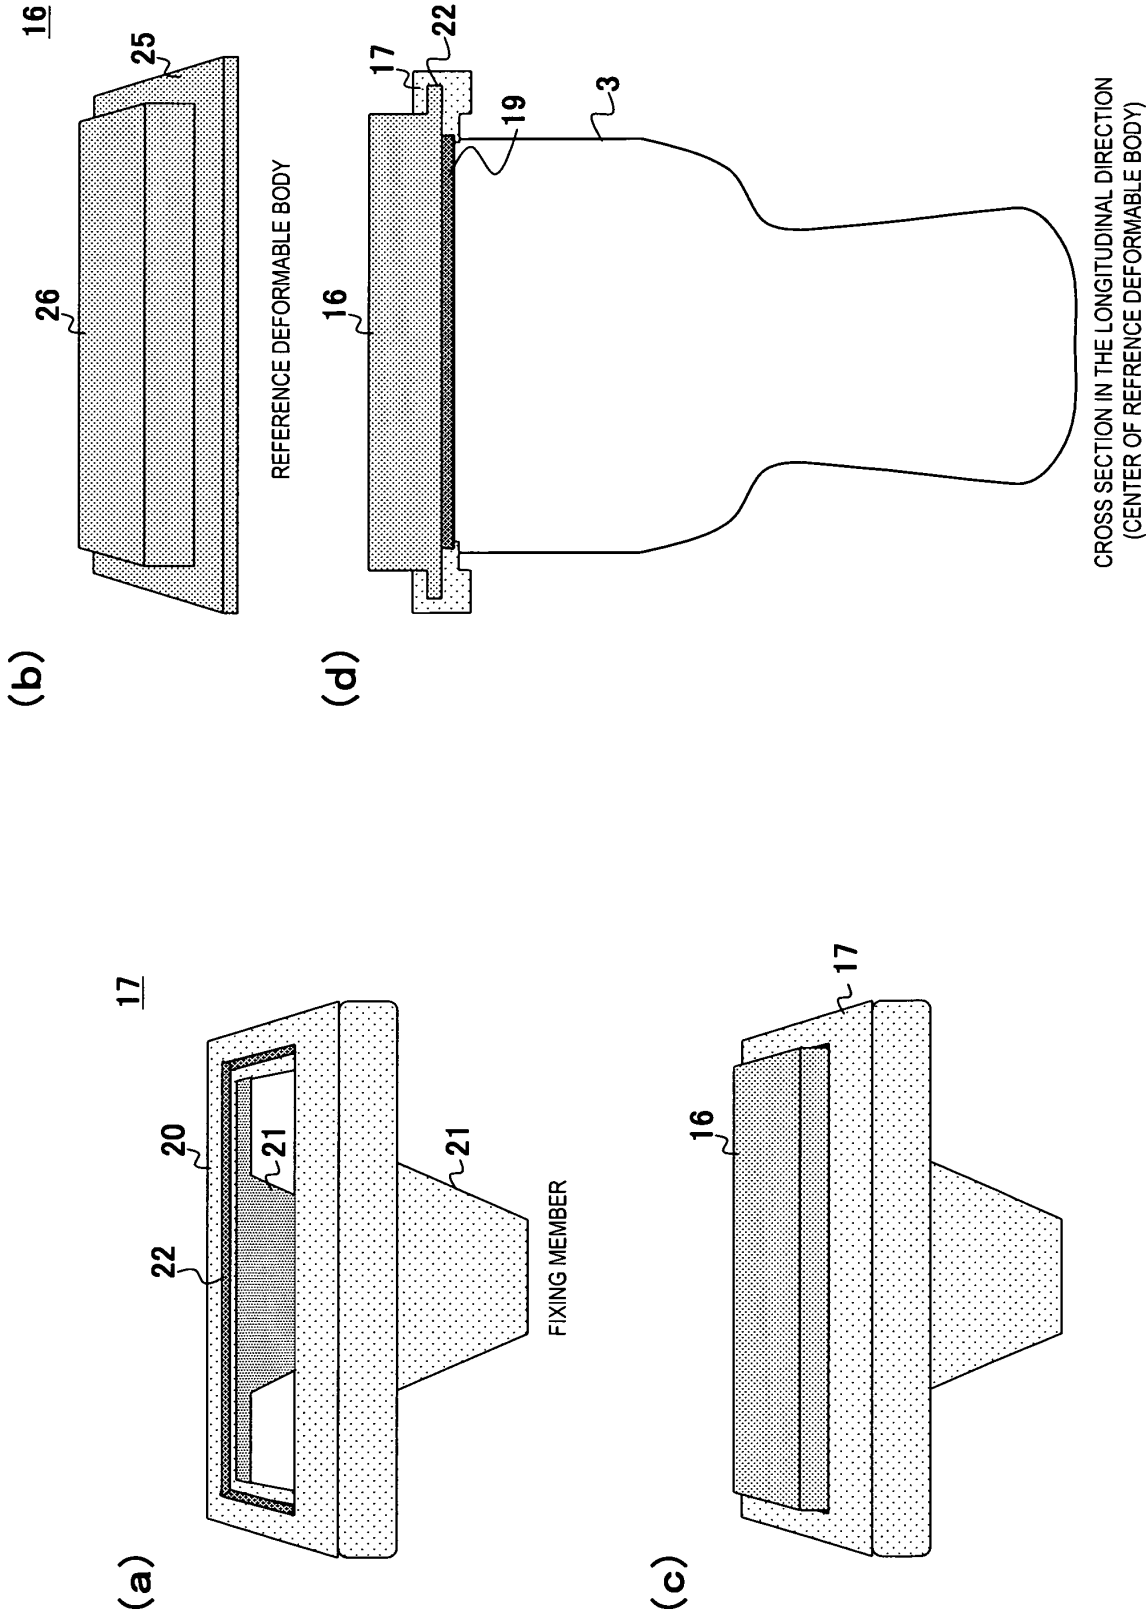


FIG. 3

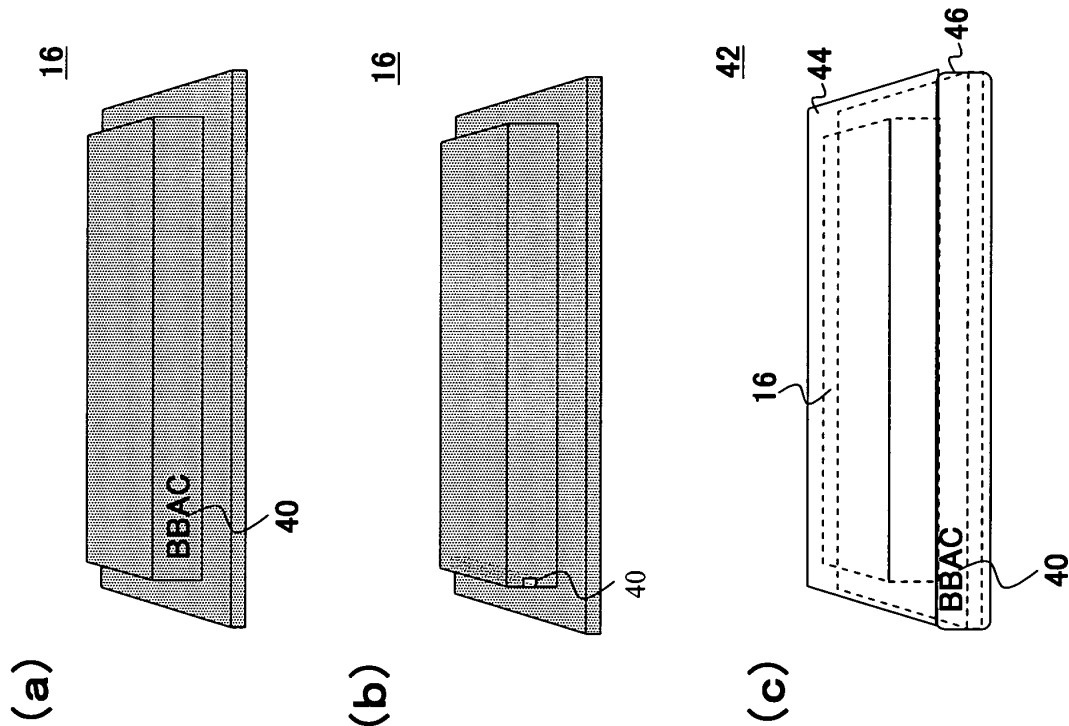


FIG. 4



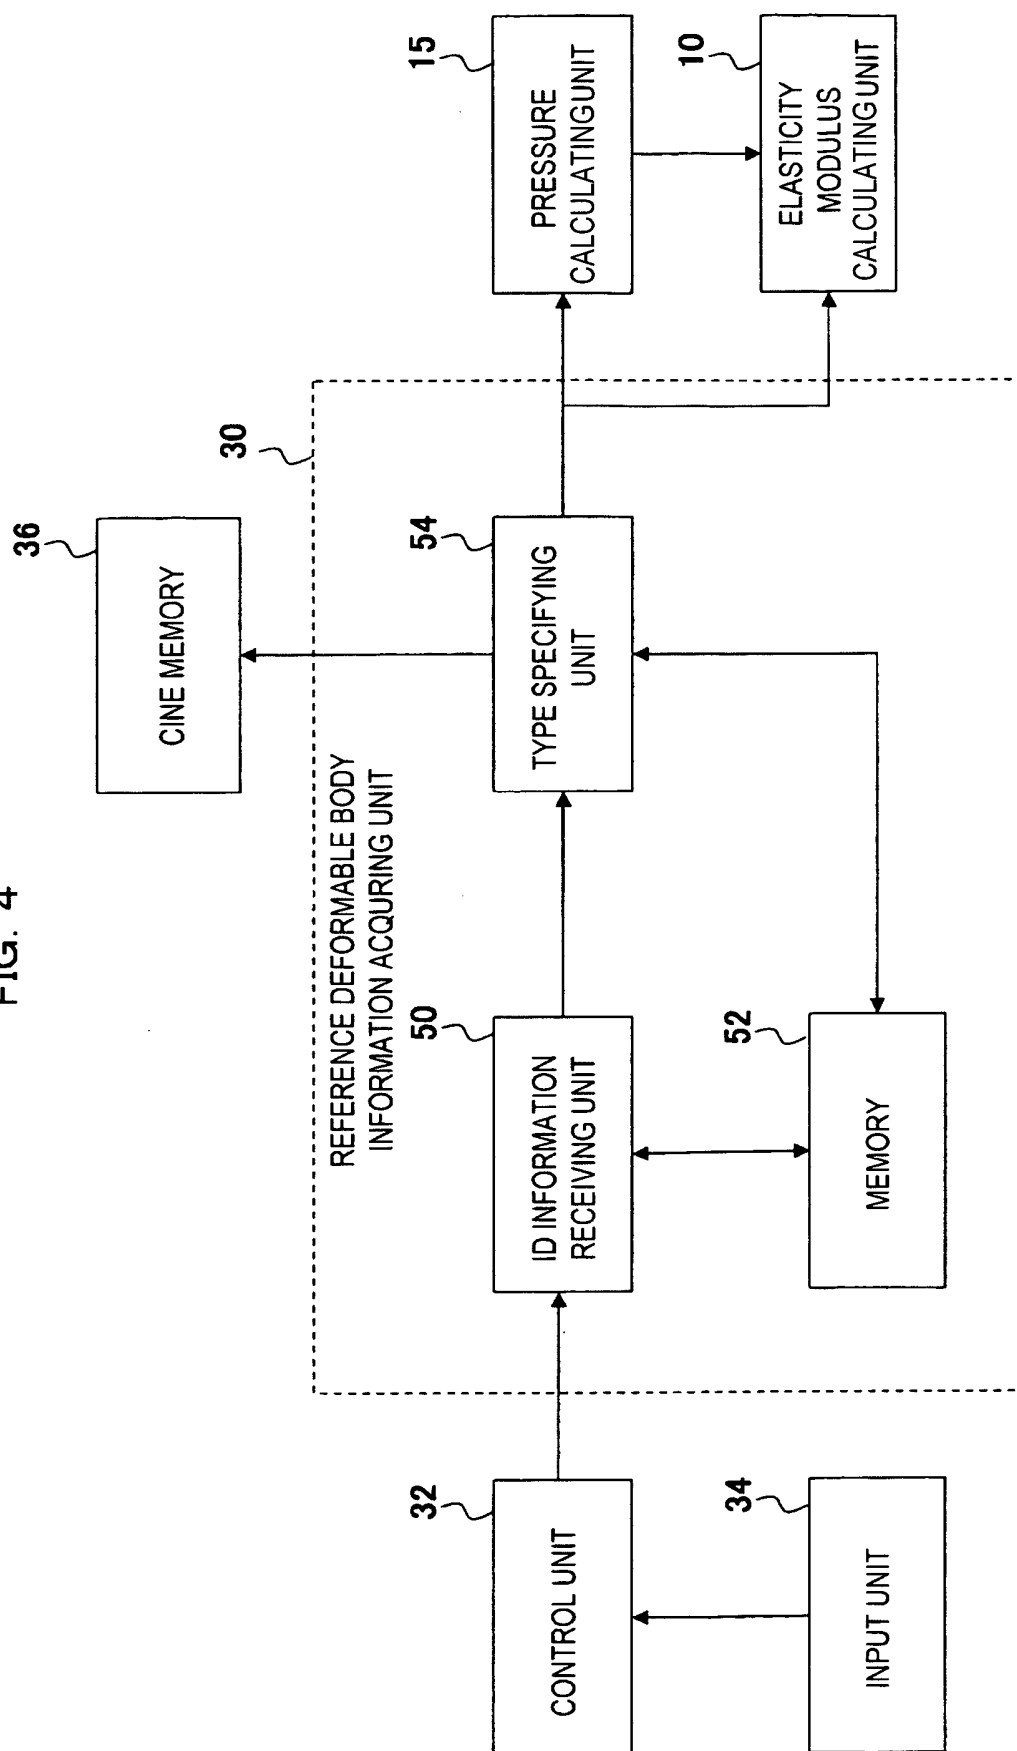


FIG. 5

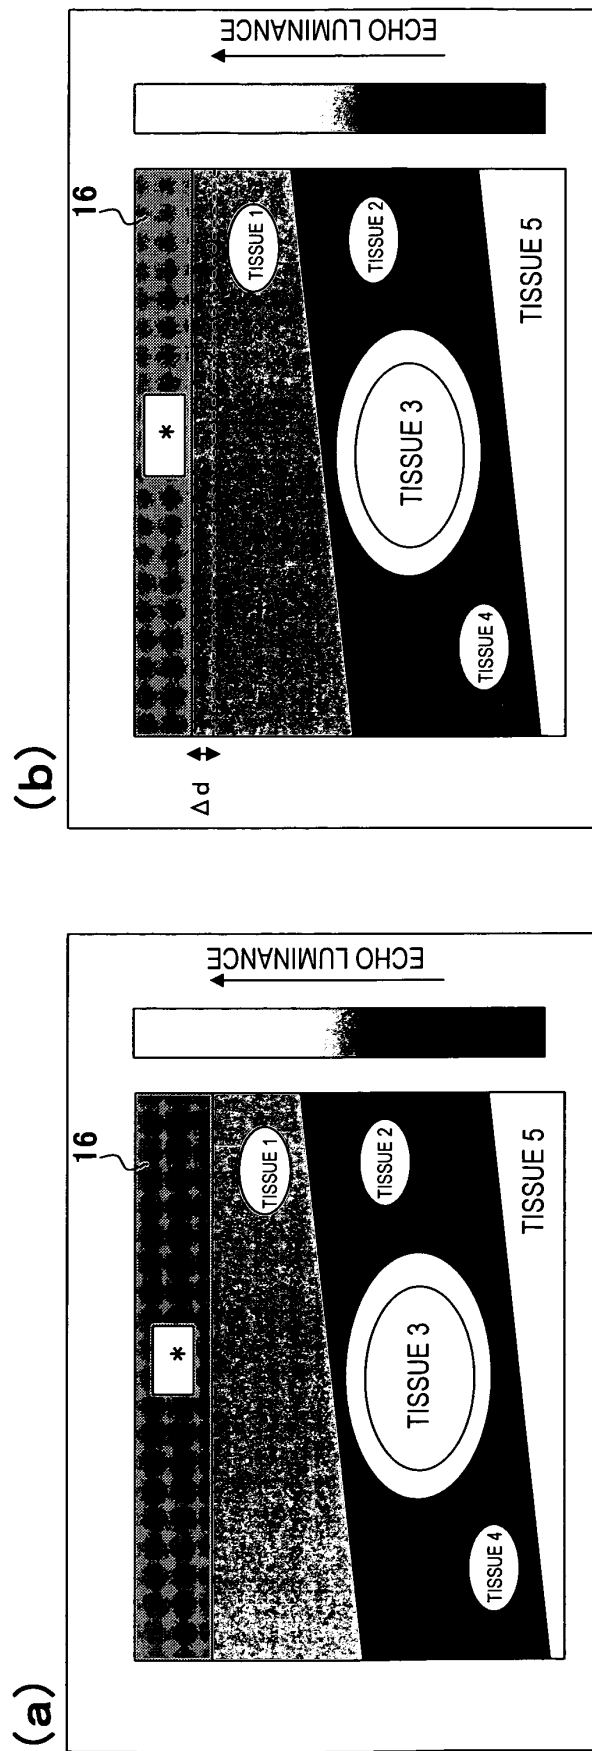


* : REFERENCE DEFORMABLE BODY

FIG. 6

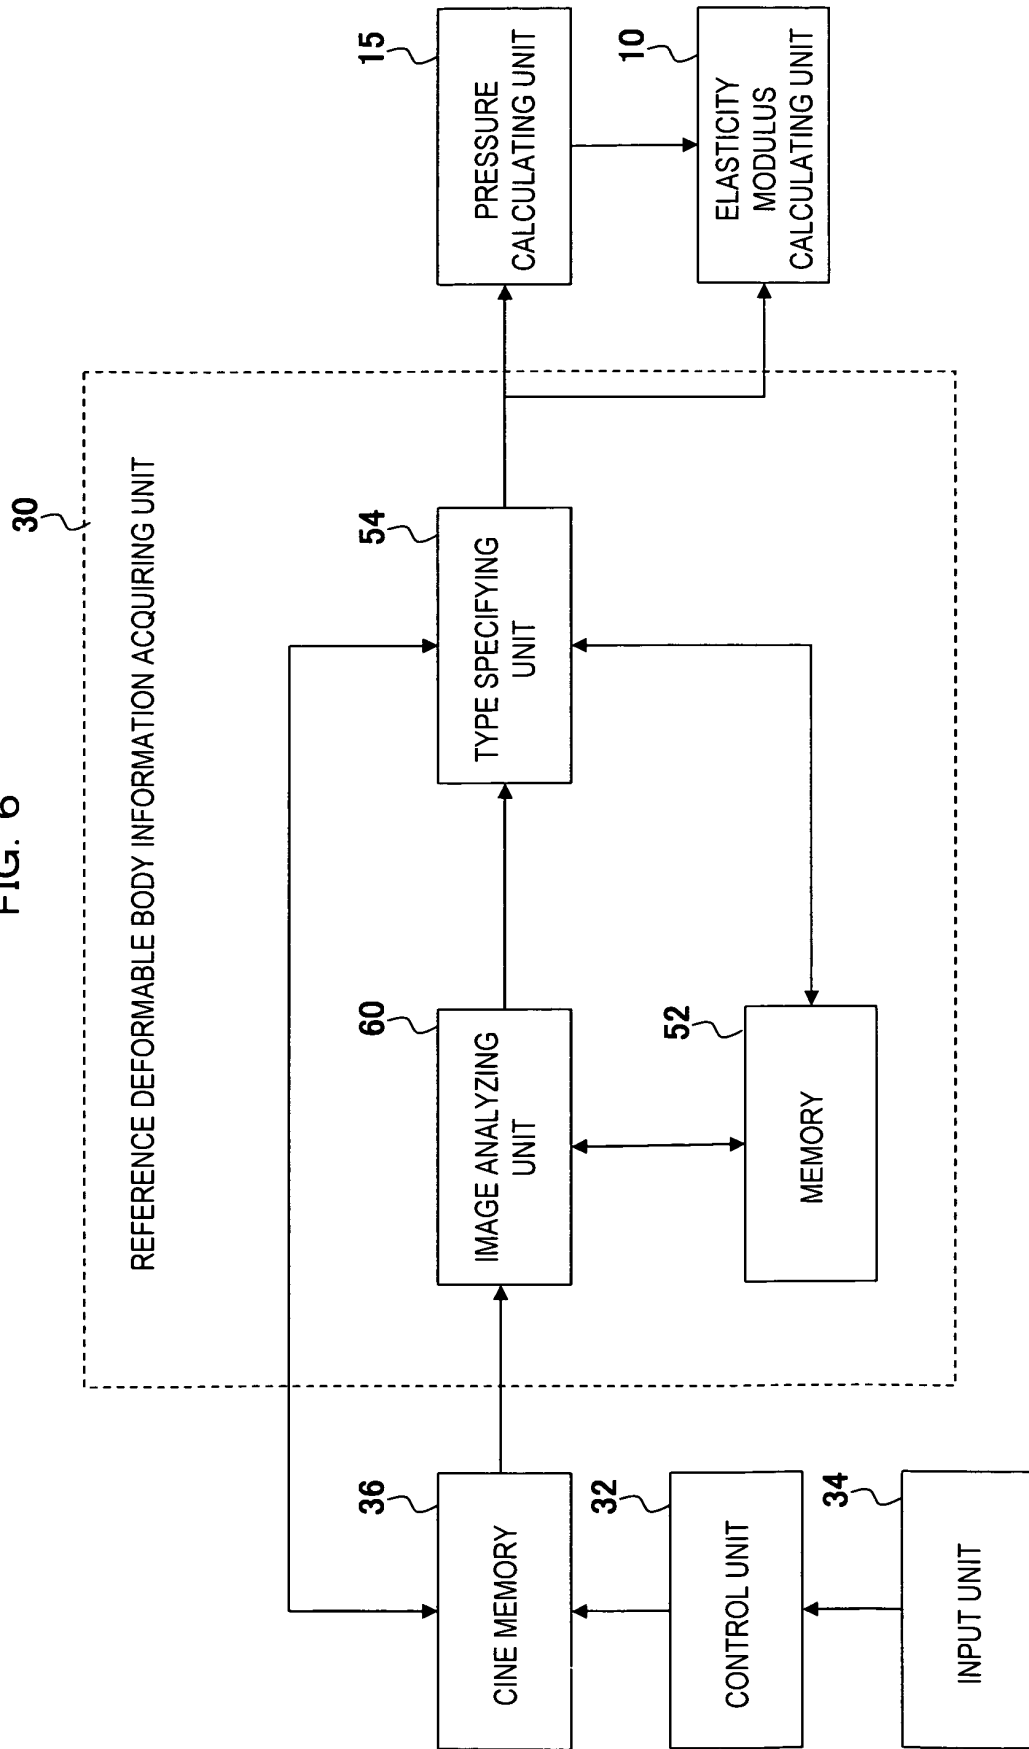


(a)

ID : α (SCATTERER CONCENTRATION 1%)

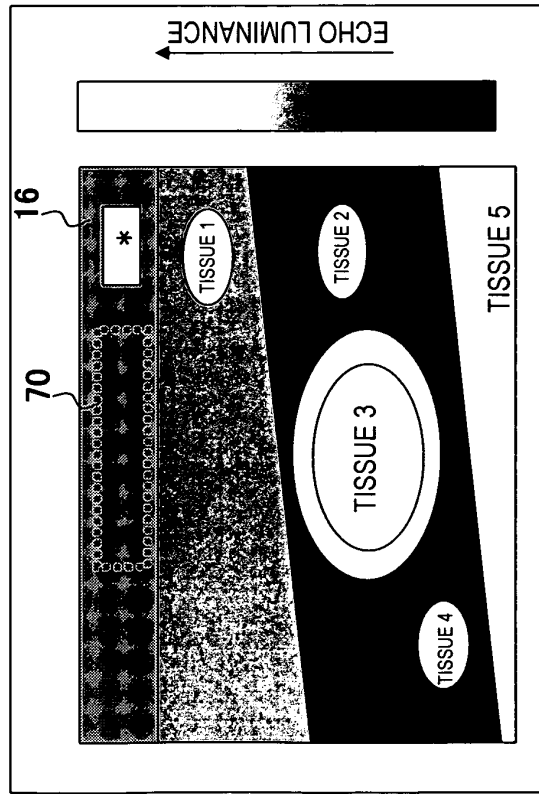

(b)

ID : β (SCATTERER CONCENTRATION 3%)

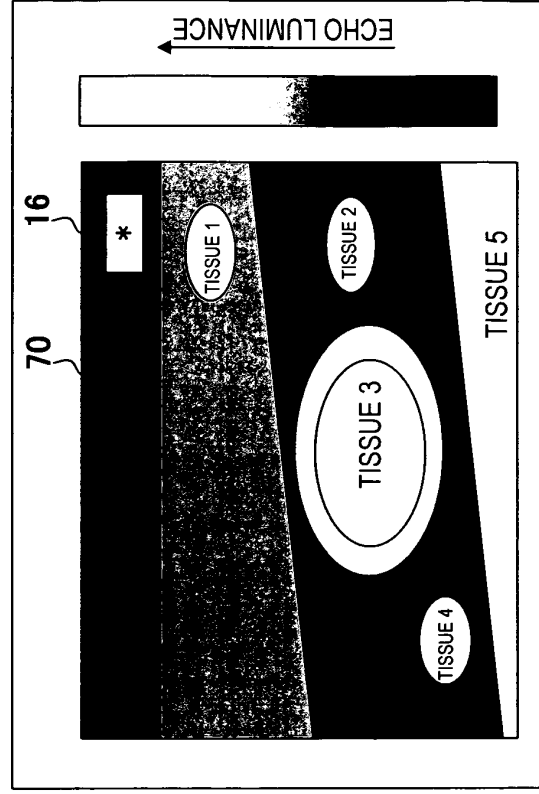


* : REFERENCE DEFORMABLE BODY

FIG. 7

FIG. 8


(a)

ID : α (LAYER1 : LAYER2=1 : 2)

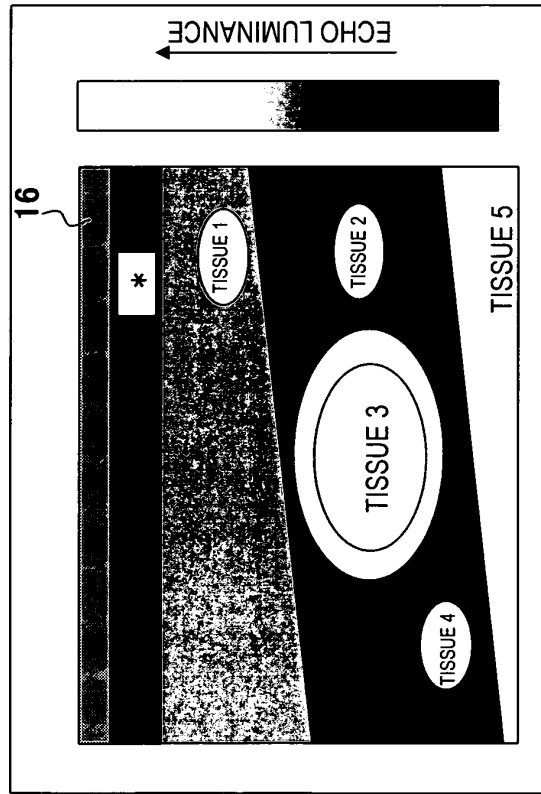


(b)

ID : β (LAYER1 : LAYER2=1 : 1)

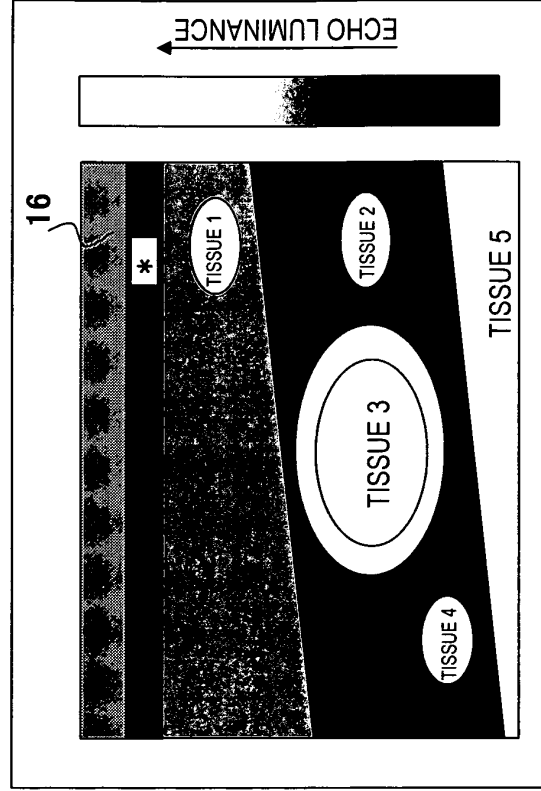

* : REFERENCE DEFORMABLE BODY

FIG. 9

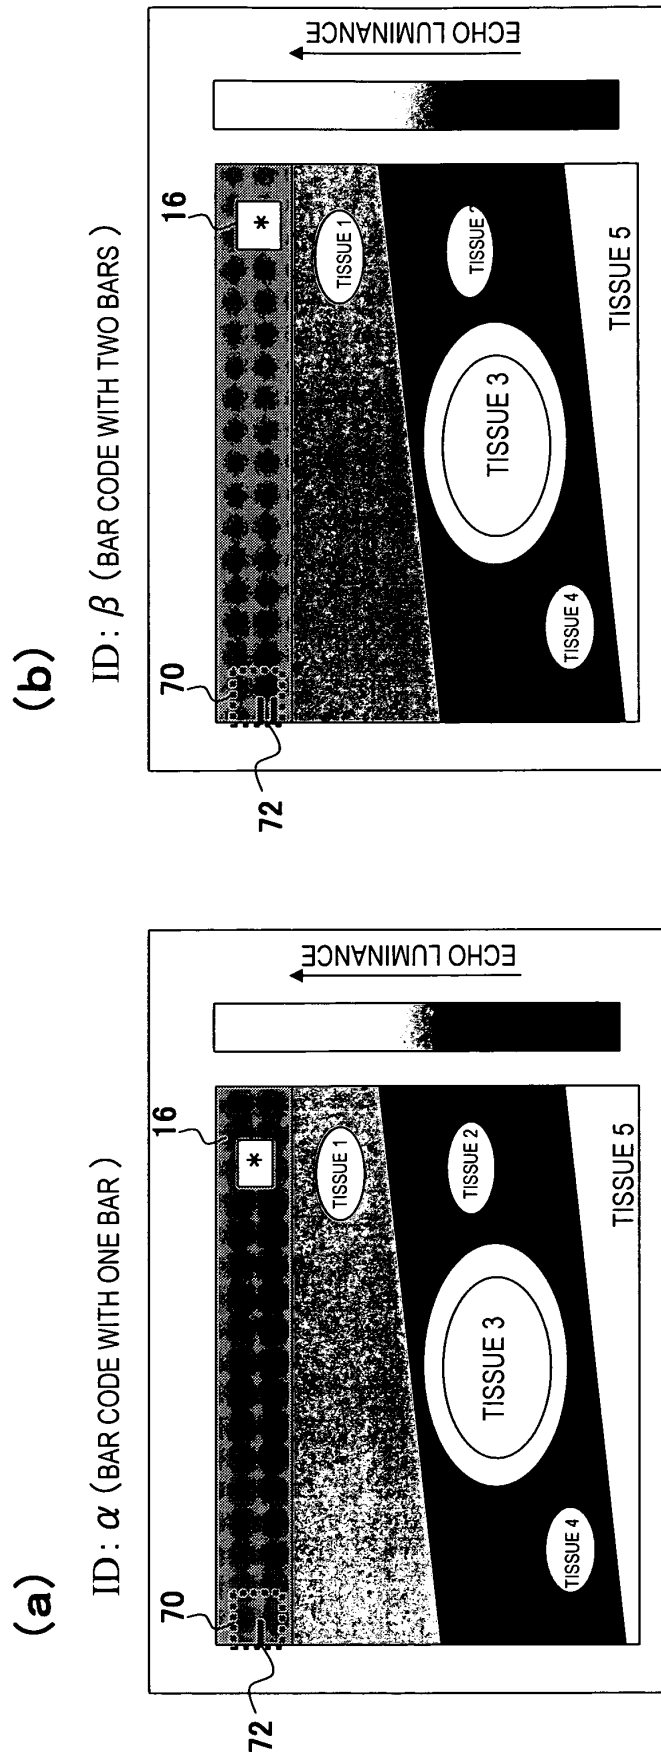

* : REFERENCE DEFORMABLE BODY


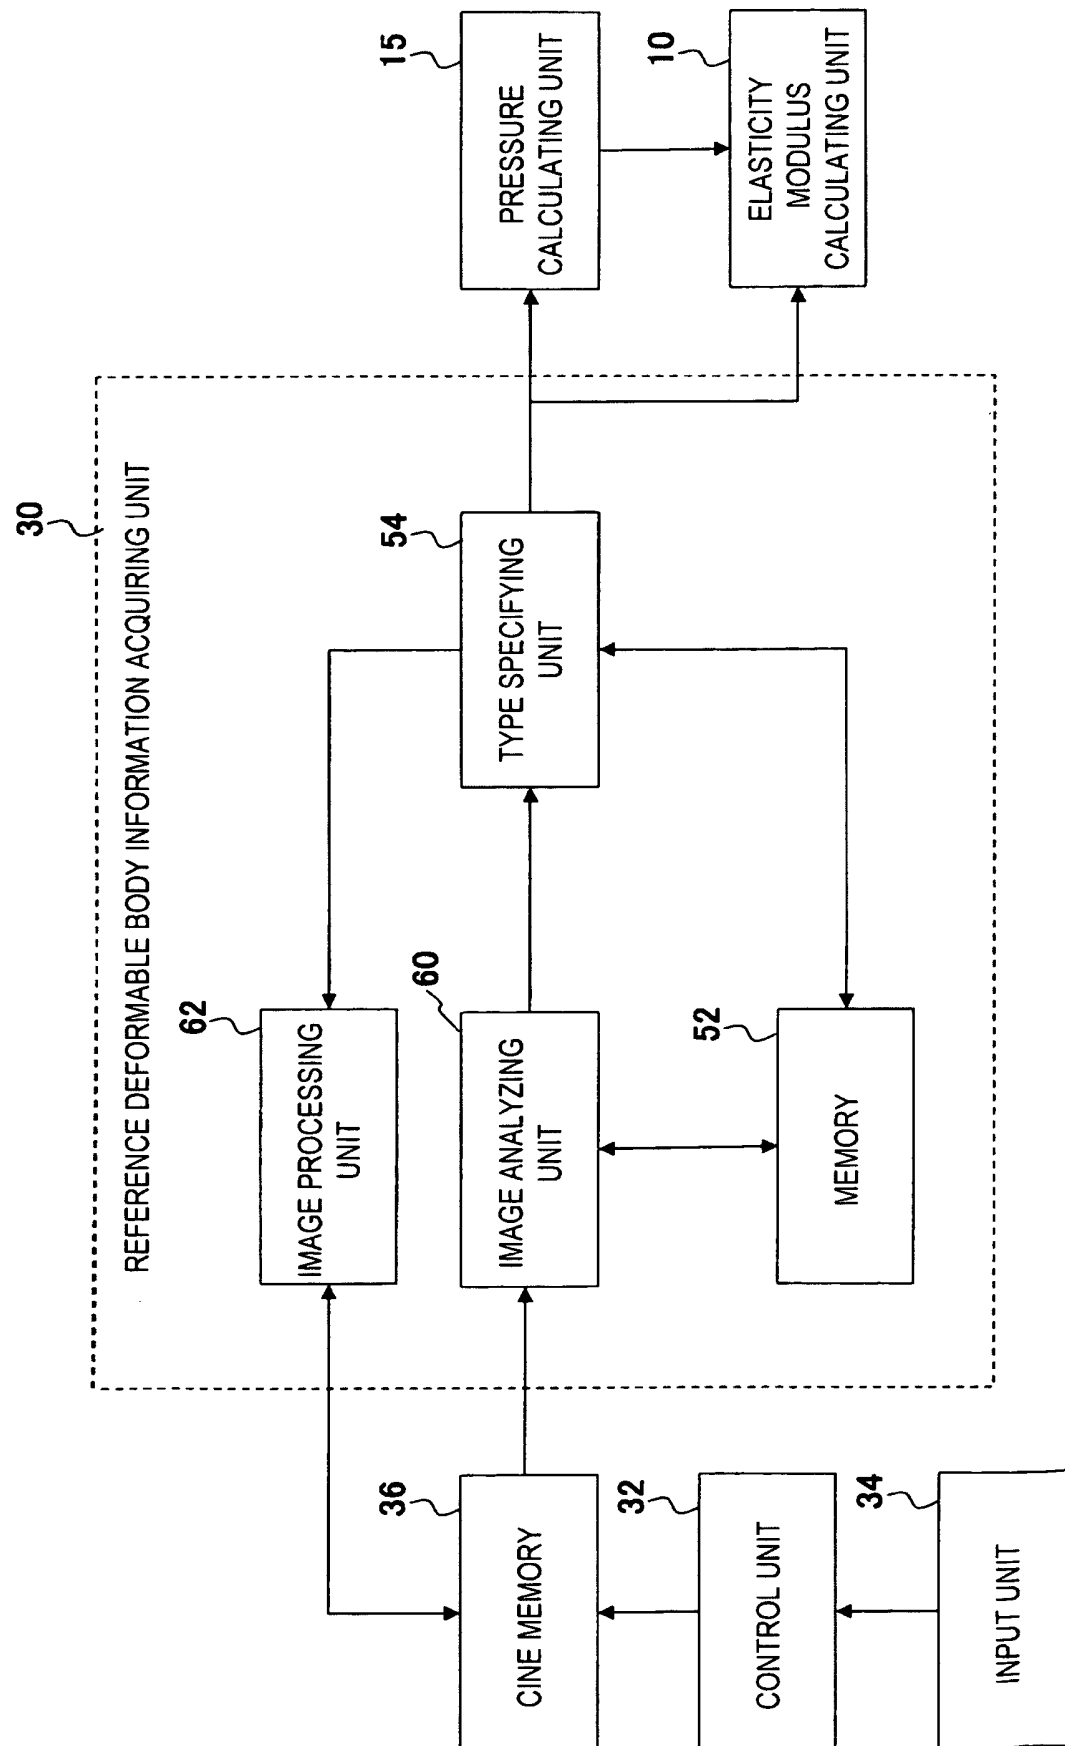



FIG. 10

FIG. 1 1

(a) BEFORE CORRECTION

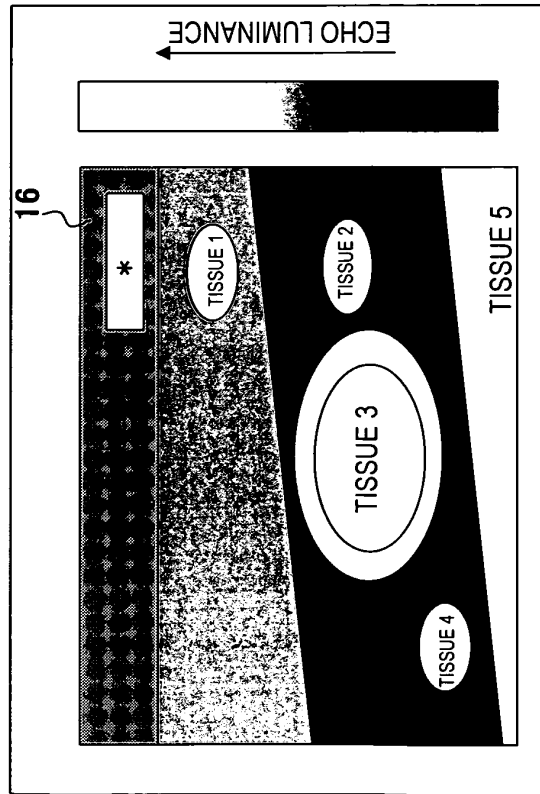

(b) AFTER CORRECTION

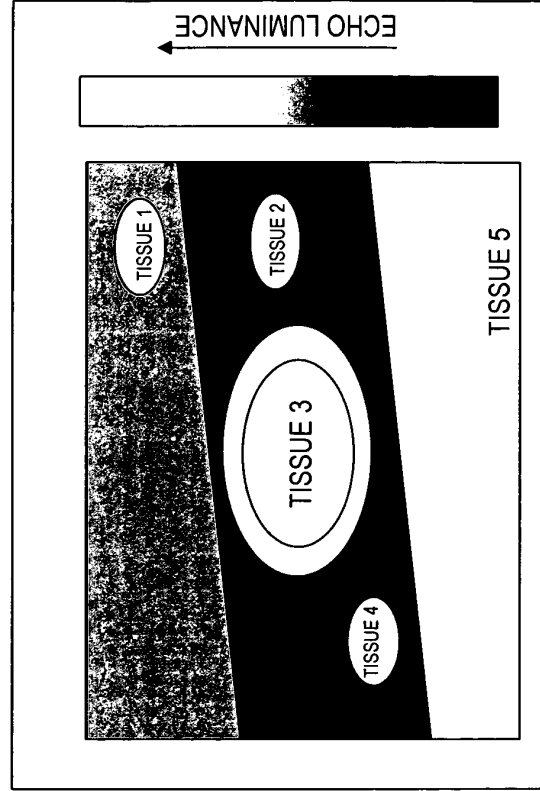

* : REFERENCE DEFORMABLE BODY

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 2005120358 A [0004]
- US 20070239006 A1 [0005]
- JP H576528 A [0005]
- JP 2005066041 A [0005]

专利名称(译)	参考可变形体和超声诊断设备		
公开(公告)号	EP2272435B1	公开(公告)日	2017-06-07
申请号	EP2009734414	申请日	2009-04-14
[标]申请(专利权)人(译)	株式会社日立医药		
申请(专利权)人(译)	日立医疗器械股份有限公司		
当前申请(专利权)人(译)	HITACHI , LTD.		
[标]发明人	MATSUMURA TAKESHI		
发明人	MATSUMURA, TAKESHI		
IPC分类号	A61B8/08		
CPC分类号	A61B8/00 A61B8/4281 A61B8/4438 A61B8/4455 A61B8/485		
优先权	2008114869 2008-04-25 JP		
其他公开文献	EP2272435A1 EP2272435A4		
外部链接	Espacenet		

摘要(译)

提供了一种可以识别其类型的参考可变形体，一种能够识别参考可变形体的类型的超声诊断设备，以及一种超声诊断方法。超声诊断设备包括超声探头（3），其中附接有参考可变形体（16），断层图像构建单元（6,7）和显示单元（14）。超声波诊断装置的特征在于，还包括：存储单元，被配置为存储给予参考可变形体（16）的ID与参考可变形体（16）的类型之间的关系，以及配置的类型识别单元（54）。读出与从存储单元（52）安装在超声波探头（3）上的基准可变形体（16）的ID对应的基准可变形体（16）的种类，确定基准可变形体的种类。

[Equation 1]

$$Y_{mi,j} = \text{pressure}(\text{stress})_{i,j} / (\text{strain } i,j)$$

$$(i,j = 1, 2, 3 \dots)$$