

(19)



(11)

**EP 2 434 957 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:

**01.01.2020 Bulletin 2020/01**

(51) Int Cl.:

**A61B 8/00 (2006.01)**

(21) Application number: **10780130.0**

(86) International application number:

**PCT/IB2010/001793**

(22) Date of filing: **25.05.2010**

(87) International publication number:

**WO 2010/136905 (02.12.2010 Gazette 2010/48)**

**(54) PULSE OFFSET ULTRASONIC IMAGING**

ULTRASCHALLBILDGEBUNG MIT VERSETZTEM IMPULS

IMAGERIE ULTRASONORE À DÉCALAGE D'IMPULSION

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO SE SI SK SM TR**

• **LI, Shuangshuang**

**P.R. China 518057 (CN)**

• **LI, Yong**

**P.R. China 518057 (CN)**

(30) Priority: **25.05.2009 CN 200910133494**

(74) Representative: **KIPA AB et al**

**P O Box 1065**

**251 10 Helsingborg (SE)**

(43) Date of publication of application:

**04.04.2012 Bulletin 2012/14**

(56) References cited:

**EP-A2- 0 948 931 EP-A2- 2 000 096**

**WO-A1-01/64108 CN-A- 1 976 635**

**CN-A- 101 357 068 US-A- 4 809 184**

**US-A- 5 685 308 US-A1- 2005 131 298**

**US-B1- 6 221 018 US-B1- 6 221 018**

**US-B1- 6 599 245**

(72) Inventors:

• **FAN, Rui**

**P.R. China 518057 (NA)**

**EP 2 434 957 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description****TECHNICAL FIELD**

5 [0001] The invention relates to diagnostic medical ultrasonic imaging.

**BACKGROUND ART**

10 [0002] Ultrasonic imaging is a well-known diagnostic medical technique that can generate a visible image of a region of interest (ROI) by transmitting ultrasound into a patient's body, and then receiving and processing reflected ultrasonic echoes, whose characteristics carry information about the body tissues exposed to the sound waves.

[0003] In a conventional ultrasonic imaging system, a transmit circuit energizes an array of piezoelectric elements to generate ultrasonic transmit pulses along focused beams into the ROI of the body. Many body tissues of interest are typically nonlinear media such that non-linear distortion is created as the ultrasonic pulses propagate through them. The nature of this distortion indicates characteristics of the tissues that can be extracted for display.

15 [0004] There is a continual effort to improve the quality of these diagnostic images, with "quality" being defined in several different ways. As with many other forms of signal processing, the effort often involves trying to get as much information as possible from the received signals while rejecting as much unwanted signal energy ("noise") as possible.

20 [0005] One known and common method is often referred to as "harmonic imaging." As the name implies, instead of processing only the echo signal at the fundamental transmit frequency, this technique involves isolating and extracting information from one or more harmonics of this fundamental frequency either in addition to or instead of at the fundamental frequency alone. Such a technique is disclosed in:

25 United States Patent No. 6,206,833;  
United States Patent No. 7,004,905;  
United States Patent No. 7,104,956; and  
United States Patent No. 7,513,870.

30 [0006] Echoes reflected from the ROI will typically include a linear component, which is associated with the ultrasonic pulses, and a nonlinear component, associated with the characteristic of tissues and structures of the body. The nonlinear component is extracted from the echoes, and the visible image is generated by processing and analyzing the nonlinear component.

35 [0007] One other known method for improving imaging quality is often referred to as "phase inversion" or "pulse inversion." This technique exploits the linearity of much of the medium through which the ultrasound pressure waves propagate through the ROI by transmitting and receiving a first ultrasound pulse, and then soon thereafter transmitting and receiving a second ultrasound pulse with a polarity opposite that of the first. Stated differently but equivalently, the two paired pulses differ in phase by 180 degrees. The combined (typically, summed) return signals will therefore "cancel" each other out (sum to zero) with respect to all linear propagation. The remaining signal is then either processed as is, or a harmonic of it is processed to create the displayed image (thereby using *both* the "phase inversion" and "harmonic imaging" techniques). United States Patent No. 5,632,277 and United States Patent No. 5,951,478 disclose examples of systems that use the "phase inversion" technique. WO01/64108 discloses medical diagnostic ultrasound imaging method fires a sequence of pulses which may be interleaved into a body and then receives, beam forms, weights and sums the resulting echo signals to suppress first order echoes.

**SUMMARY OF THE INVENTION**

45 [0008] The invention is defined in independent claims 1 and 10. A diagnostic ultrasound image of a region of interest (ROI) of a body is formed by transmitting into the ROI at least a first and a second ultrasound pulse, in which the second pulse is phase-shifted relative to the first pulse by an amount other than 0 or 180 degrees. Discrete (quantized) received signals from the pulses are interleaved to form a resultant operating signal that is detected and beamformed as the operating signal.

**BRIEF DESCRIPTION OF THE DRAWINGS**

55 [0009]

Figure 1 is a block diagram of an offset pulse ultrasonic imaging system in accordance with an embodiment;

Figure 2 is a flowchart of an offset pulse ultrasonic imaging method in accordance with an embodiment;

Figure 3 is a block diagram of an offset pulse ultrasonic imaging system in accordance with another embodiment;

5 Figure 4 is a flowchart of an offset pulse ultrasonic imaging method in accordance with another embodiment;

Figure 5a-5(d) are graphs of waveforms for ultrasonic pulses and echoes in accordance with another embodiment;

10 Figure 6a-6(d) are graphs of echo waveforms at sample rates of 40MHz, shown in a conventional ultrasonic imaging system and an ultrasonic imaging system in accordance with an embodiment respectively; and

Figure 7a-7(d) are graphs of echo waveforms at sample rates of 30MHz, shown in a conventional ultrasonic imaging system and an ultrasonic imaging system in accordance with an embodiment respectively.

15 Figure 8 illustrates a two-pulse embodiment and how a second pulse is offset from a first.

Figures 9a and 9b illustrate how the pulses shown in Figure 8 may be quantized.

20 Figure 10 illustrates echo pulse interleaving.

Figure 11 illustrates how pulse offsetting and interleaving affect the spectrum of received signals.

## DETAILED DESCRIPTION

25 **[0010]** The following detailed description refers to the accompanying drawings. The same reference numbers may be used in different drawings to identify the same or similar elements. In the following description specific details may be set forth such as particular structures, techniques, etc. in order to provide a thorough understanding of the various aspects of the claimed invention. However, such details are provided for purposes of explanation and should not be viewed as limiting with respect to the claimed invention. With benefit of the present disclosure it will be apparent to those skilled in the art that the various aspects of the invention claimed may be practiced in other examples that depart from these specific details. Moreover, in certain instances, descriptions of well known devices, circuits, and methods are omitted so as not to obscure the description of the present invention with unnecessary detail.

30 **[0011]** Figure 1 shows a block diagram of an offset pulse ultrasonic imaging system 100 in accordance with an embodiment. As shown in Figure 1, a transmit circuit 10 generates a plurality of ultrasonic pulse signals for each scan line in a scan plane. The plurality of ultrasonic pulse signals is converted into a plurality of ultrasonic pulses by a probe/transducer 20, which includes an array of piezoelectric elements. The structure and operation of an ultrasound probe/transducer are well understood and can be summarized by saying that it functions as a phased array of piezoelectric transmit/receive elements that generate and respond to pressure waves at ultrasonic frequencies. The ultrasonic pulses are offset relative to each other, which will be explained in detail later. The converted ultrasonic pulses are transmitted into a region of interest (ROI) 30 of a body. Since tissues of the body are nonlinear media, the echoes, reflected from the ROI 30, include a linear component associated with the ultrasonic pulses, and a nonlinear component associated with the characteristics of the various body tissues and other structures.

35 **[0012]** The ultrasound echoes reflected back from these body tissues and structures are then converted into echo signals by the probe 20. Conventional sampling, analog-to-digital and other circuitry is then used to convert the electrical signals created by the piezoelectric elements in the probe into a series of digital equivalent values, which are then supplied to an interleaver 40. As is explained in greater detail below, the interleaver 40 interleaves the values into a sequence of samples to form an operating signal. The operating signal is supplied to a detector 50. An explanation of the operating signal will be given in detail later. The nonlinear component is extracted from the operating signal in the detector 50 and is then beamformed in a beamformer 60 to generate a scan line, a collection of which is then converted in any known manner into a form suitable for display or recording or other processing by a user.

40 **[0013]** Figure 2 is a flowchart of an offset pulse ultrasonic imaging method in accordance with an embodiment. In one embodiment, the method can be performed by the offset pulse ultrasonic imaging system 100 in Figure 1.

45 **[0014]** First, at step 10, a transmit circuit 10 generates a plurality K of ultrasonic pulse signals for each scan line in a scan plane. That is, K ultrasonic pulse signals are emitted by the transmit circuit 10. For the K ultrasonic pulse signals, each ultrasonic pulse signal is time-shifted relative to an immediately preceding ultrasonic pulse signal by a predetermined amount. In one embodiment, the time-shift is  $\tau=1/(K \cdot f_s)$  where  $f_s$  is an initial sample rate for each scan line.

50 **[0015]** Each of the K ultrasonic pulse signals may optionally be weighted by a corresponding weight coefficient

$\cos(\frac{(k-1) \cdot 2\pi}{K} \cdot \alpha)$ , where  $K=1, 2 \dots K$ , and  $\alpha$  is positive integer. If the  $K^{th}$  ultrasonic pulse signal is represented by  $P_K$ , ultrasonic pulse signals  $P_1, P_2, \dots, P_K$  can be represented as:

$$\begin{aligned} P_1 &= A(t) \sin(\omega t + \Phi_p) \\ P_2 &= A(t + \tau) \cos(\frac{2\pi}{K} \cdot \alpha) \sin(\omega(t + \tau) + \Phi_p) \\ &\dots \\ P_K &= A(t + (k-1)\tau) \cos(\frac{(k-1)2\pi}{K} \cdot \alpha) \sin(\omega(t + (k-1)\tau) + \Phi_p) \end{aligned}$$

The absolute ratio of two weight coefficients represents the amplitude ratio of the two corresponding ultrasonic pulse signals. In the condition where the weight coefficient is positive, the waveform polarity of the corresponding ultrasonic pulse signal is positive; on the other hand, if the weight coefficient is negative, the polarity is negative.

**[0016]** At step 20, the  $K$  ultrasonic pulse signals are converted into  $K$  corresponding ultrasonic pulses by the probe 20, wherein each ultrasonic pulse is time-shifted relative to an immediately preceding ultrasonic pulse by the predetermined amount  $\tau$ . The  $K$  ultrasonic pulses are transmitted into the ROI 30 of the body. Because each of the  $K$  ultrasonic pulses is time-shifted relative to an immediately preceding ultrasonic pulse by  $\tau$ , the  $K$  ultrasonic pulses are relatively offset pulses emitted to the ROI 30.

**[0017]** Since many body tissues of interest comprise acoustically nonlinear media, the echoes, reflected from the ROI 30, include a linear component associated with the ultrasonic pulses and a nonlinear component associated with characteristics of tissues of the body. At step 30, the probe 20 receives  $K$  echoes and converts the  $K$  echoes into  $K$  echo signals. If the  $K^{th}$  echo signal is represented by  $E_K$ , echo signals  $E_1, E_2, \dots, E_K (K=1, 2 \dots K)$  can be represented as:

$$\begin{aligned} E_1 &= A(t) \sin(\omega t + \Phi_e) + H(t) \\ E_2 &= A(t + \tau) \cos(\frac{2\pi}{K} \cdot \alpha) \sin(\omega(t + \tau) + \Phi_e) + \cos^2(\frac{2\pi}{K} \cdot \alpha) H(t + \tau) \\ &\dots \\ E_K &= A(t + (k-1)\tau) \cos(\frac{(k-1)2\pi}{K} \cdot \alpha) \sin(\omega(t + (k-1)\tau) + \Phi_e) + \cos^2(\frac{(k-1)2\pi}{K} \cdot \alpha) H(t + (k-1)\tau) \end{aligned}$$

where  $H(t)$  represents the nonlinear component which carries information on characteristic of tissues of the body.

**[0018]** In this embodiment,  $K$  ultrasonic pulse signals are emitted by the transmit circuit 10 for each scan line in the scan plane associated with the initial sample rate  $f_s$ . The interleaver 40 thus may receive  $K$  echo signals converted by the probe 20 in the period of  $\tau=1/f_s$ . That is, in each sample interval of  $1/f_s$ ,  $K$  echo signals ( $E_1, E_2 \dots E_K$ ) can be received by the interleaver 40. These echo signals ( $E_1, E_2 \dots E_K$ ) make up  $K$  samples in the sample interval of  $1/f_s$ .

**[0019]** Where the initial sample interval is  $1/f_s$ , the number of initial samples is  $N$  for each scan line in the scan plane. As mentioned above, there are  $K$  signals in the sample interval of  $1/f_s$ . The sampled values of the  $K$  signals in each sample interval of  $1/f_s$  may then be interleaved in a sequence of the initial samples  $1, 2 \dots N$ , to form the operating signal for generating the scan line, the number of current samples is  $N \cdot K$ . If the operating signal is represented by  $W(t)$ ,  $W(t)$  may be made up of echo signals  $E_{11} E_{12} \dots E_{1K} E_{21} E_{22} \dots E_{2K} \dots E_{i1} E_{i2} \dots E_{ij} \dots E_{iK} \dots E_{N1} E_{N2} \dots E_{Nj} \dots E_{NK}$ ,  $i = 1, 2 \dots N$ ,  $j = 1, 2 \dots K$ .

$$\begin{aligned} W(t) &= A(t) \sin(\omega t + \Phi_e) \cos(2\pi\alpha f_s \cdot t) + H(t) \cos^2(2\pi\alpha f_s \cdot t) \\ &= A(t) \sin(\omega t + \Phi_e) \cos(2\pi\alpha f_s \cdot t) + \frac{1}{2} H(t) + \frac{1}{2} H(t) \cos(4\pi\alpha f_s \cdot t) \end{aligned}$$

Where  $t = m\tau$ ,  $m = 0, 1, 2, \dots, (N \cdot K - 1)$ ,  $\tau = \frac{1}{Kf_s}$

**[0020]** The K echo signals are interleaved in the sequence of the initial samples (1, 2...N) to form the operating signal  $W(t)$  in the interleaver 40. The operating signal  $W(t)$  is supplied to a detector 50 at step 40. Then, at step 50, the nonlinear component is extracted from the operating signal  $W(t)$  in the detector 50, and at step 60, the nonlinear component is beamformed in a beamformer 60 to generate the scan line. Since the nonlinear component carries information about characteristics of tissues of the body, a visible image of the ROI 30 is generated by analyzing the nonlinear component using known scan conversion and display algorithms.

**[0021]** It can be concluded from the expression of  $W(t)$ : (1) the sample interval of the operating signal is  $\tau$ , so the effective sample rate of the operating signal is  $K \cdot f_s$  which is K times the initial sample rate  $f_s$ ; (2) the linear component of the operating signal is modulated to  $\alpha$  times  $f_s$ , i.e. the linear component is moved to both sides of  $\alpha \cdot f_s$  in the frequency domain; whereas, for the nonlinear component, half is not modulated and the other half is modulated to  $2\alpha f_s$ . That is, in the frequency domain, half of the nonlinear component is maintained at its original frequency and the other half is moved to both sides at  $2 \cdot \alpha \cdot f_s$ .

**[0022]** Detection of the nonlinear component at either side of  $2 \cdot \alpha \cdot f_s$  may avoid frequency overlap, or at least cause less overlap than in known methods. It is preferable to select  $\alpha$  and K by considering the following equation. In accordance with Nyquist theorem:

$$Kf_s \geq 2 \cdot \left( \frac{4\pi\alpha f_s}{2\pi} \right), \quad \text{i.e.} \quad \frac{K}{\alpha} \geq 4$$

**[0023]** In this embodiment, each of the K ultrasonic pulse signals may be weighted by a corresponding weight coefficient, which causes the linear component to move to either side of  $\alpha f_s$  in the frequency spectrum; as for the nonlinear component, half is maintained at the original fundamental frequency and the other half is moved to either side of  $2\alpha f_s$ . Accordingly, when the operating signal is analyzed in the detector 50, the nonlinear component is extracted efficiently because the linear component and the nonlinear component are separated in the frequency domain.

**[0024]** In another embodiment, the linear component may be overlapped by part of the nonlinear component (e.g. the nonlinear component moved to  $2 \cdot \alpha \cdot f_s$ ) in the frequency domain while the nonlinear component is maintained at the original fundamental frequency (i.e. non-modulated nonlinear component) instead of the nonlinear component being moved to both sides of  $2 \cdot \alpha \cdot f_s$  (i.e. modulated nonlinear component). The relevant information-bearing nonlinear signal component, can be extracted using known filtering methods provided that the non-modulated nonlinear component is sufficiently separated from the linear component and the non-modulated nonlinear component.

**[0025]** Figure 3 shows a block diagram of an offset pulse ultrasonic imaging system 200 in accordance with another embodiment. As compared with the offset pulse ultrasonic imaging system 100, the system 200 further comprises a selector 5. The selector 5 may select suitable K and  $\alpha$  for enabling the non-modulated nonlinear component to be separated from the linear component in the frequency domain and not be interfered with due to frequency overlap caused by the linear component and the modulated nonlinear component.

**[0026]** As shown in Figure 3, a transmit circuit 10', based on the selected K and  $\alpha$ , generates a plurality of ultrasonic pulse signals for each scan line in a scan plane. The probe 20, interleaver 40, detector 50 and beamformer 60, can be implemented using the same or similar devices and programming as shown in Figure 1.

**[0027]** Figure 4 is a flowchart of an offset pulse ultrasonic imaging method in accordance with an embodiment. In this embodiment, the method can be performed by the offset pulse ultrasonic imaging system 200 shown in Figure 3. First, at step 5, a selector 5 selects suitable K and  $\alpha$  values. The selected K and  $\alpha$  may enable the non-modulated nonlinear component to be separated from the linear component, thereby reducing interference due to frequency overlap of the linear and nonlinear components in frequency domain. At step 10', a transmit circuit 10', based on the selected K and  $\alpha$ , generates a plurality of ultrasonic pulse signals, for example K, for each scan line in a scan plane. The following steps 20-60 may be the same or similar as those shown in Figure 2.

**[0028]** The system and the method as shown in Figure 3 and Figure 4 will be illustrated further by providing a group of particular values of K and  $\alpha$ . In one embodiment,  $K=2$  and  $\alpha=1$ . In accordance with the expression for  $P_K$  above, the ultrasonic pulse signals  $P_1$  and  $P_2$  can be represented as:

$$P_1 = A(t) \sin(\omega t + \Phi_p)$$

$$P_2 = A(t + \tau) \cos\left(\frac{2\pi}{K} \cdot \alpha\right) \sin(\omega(t + \tau) + \Phi_p)$$

$$= -A(t + \tau) \sin(\omega(t + \tau) + \Phi_p)$$

5  
**[0029]** In this example, the polarities of waveforms of ultrasonic pulse signals  $P_1$  and  $P_2$  are positive and negative respectively, and the amplitude ratio of  $P_1$  and  $P_2$  is 1:1. The ultrasonic pulse signal  $P_2$  is time-shifted relative to the ultrasonic pulse signal  $P_1$  by a predetermined amount  $\tau = 1/(2f_s)$ . The waveforms for the ultrasonic pulses  $P_1$  and  $P_2$  are illustrated in Figure 5a.

10  
**[0030]** The ultrasonic pulses  $P_1$  and  $P_2$  are transmitted into the ROI 30 and echo signals are reflected back to the transducer as usual. In accordance with the expression of echo signal  $E_K$  above, the echo signals  $E_1$  and  $E_2$  can be represented as:

$$E_1 = A(t) \sin(\omega t + \Phi_e) + H(t)$$

$$E_2 = A(t + \tau) \cos\left(\frac{2\pi}{K} \cdot \alpha\right) \sin(\omega(t + \tau) + \Phi_e) + \cos^2\left(\frac{2\pi}{K} \cdot \alpha\right) H(t + \tau)$$

$$= -A(t + \tau) \sin(\omega(t + \tau) + \Phi_e) + H(t + \tau)$$

15  
**[0031]** The waveforms for the echo signals  $E_1$  and  $E_2$  are illustrated in Figure 5b, where the echo signal  $E_1$  is illustrated with small circles and the echo signal  $E_2$  is illustrated as small squares. The two echo signals  $E_1$  and  $E_2$  in each sample interval of  $1/f_s$  are interleaved to form an operating signal  $W(t)$ . In accordance with the expression of the operating signal  $W(t)$  as above mentioned,  $W(t)$  can be represented as:

$$W(t) = A(t) \sin(\omega t + \Phi_e) \cos(2\pi f_s \cdot t) + \frac{1}{2} H(t) + \frac{1}{2} H(t) \cos(4\pi f_s \cdot t)$$

20  
 In this embodiment, the sample rate of the nonlinear component is  $2f_s$  ( $K=2$ ), so the operating signal  $W(t)$  can be further expressed as:

$$W(t) = A(t) \sin(\omega t + \Phi_e) \cos(2\pi f_s \cdot t) + H(t)$$

25  
**[0032]** It can be concluded from the expression of  $W(t)$ : (1) the sample rate of the operating signal is two times of the initial sample rate  $f_s$ , i.e.  $2 \cdot f_s$ , as shown in Figure 5c; (2) the linear component is moved to either side of  $f_s$  in frequency domain, the two central frequencies are located at  $(f_s - \omega/2\pi)$  and at  $(f_s + \omega/2\pi)$  respectively; and the nonlinear component is maintained at the fundamental frequency. Since the linear component and the nonlinear component are separated in the frequency domain, and the sample rate of the nonlinear component is two times the initial sample rate  $f_s$ , the linear component can be efficiently filtered using known filtering methods, for example, and the nonlinear component  $H(t)$  can be extracted efficiently as shown in Figure 5d.

30  
**[0033]** Further, in one illustrative embodiment, the initial sample rate  $f_s$  is 40MHz, the central frequency of the linear component is 6MHz and the central frequency of the nonlinear component is 12MHz. The waveforms of the operating signal  $W(t)$  are illustrated in Figure 6c and Figure 6(d); whereas the waveforms of echoes in a conventional ultrasonic imaging system are shown in Figure 6a and Figure 6b. There will be significant frequency overlap in conventional ultrasonic imaging systems; however, according to the embodiment of the invention ( $K=2$ ,  $\alpha=1$ ), not only the effective sample rate is increased to two times the initial sample rate  $f_s$  (i.e. 80MHz), but the linear component is much more completely separated from the nonlinear component in the frequency domain.

35  
**[0034]** According to embodiments of the present invention, the sample rate of the nonlinear component is increased by virtue of the parameter  $K$ . Thus, almost all frequencies in the frequency band of the nonlinear component can be more efficiently detected even if the initial sample rate  $f_s$  is not high.

40  
**[0035]** In another embodiment, the initial sample rate  $f_s$  is 30MHz. The waveforms of the operating signal  $W(t)$  are

shown in Figure 7c and Figure 7(d); the waveforms of echoes in a conventional ultrasonic imaging system are shown in Figure 7a and Figure 7b. As can be seen, because of significant frequency overlap in the conventional ultrasonic imaging system, the information at the frequencies in the frequency band of the nonlinear component cannot be detected completely; however, according to the embodiment of the present invention, not only the linear component can be separated from the nonlinear component in the frequency domain, but the sample rate can be increased to two times of the initial sample rate  $f_s$  (in this example, 60MHz), which enables almost all signal at frequencies in the frequency band of the nonlinear component to be much easier to isolate and detect.

[0036] Other groups of particular values of  $K$  and  $\alpha$  can be selected. With the selected  $K$  and  $\alpha$ , the effective sample rate of the operating signal is increased to  $K$  times the initial sample rate  $f_s$ , and the linear component is modulated to a location as far as possible from the nonlinear component in the frequency domain.

[0037] According to another illustrative embodiment,  $K=6$ ,  $\alpha=2$ , such that six ultrasonic pulse signals  $P_1, P_2 \dots P_6$  are generated for each scan line in the scan plane. The corresponding weight coefficients of the six ultrasonic pulse signals may then be 1,  $-1/2$ ,  $-1/2$ , 1,  $-1/2$ ,  $-1/2$ . The polarities of the waveforms for the six ultrasonic pulse signals are thus positive, negative, negative, positive, negative, negative, and the amplitude ratios of the six ultrasonic pulse signals are 1:0.5:0.5:1:0.5:0.5. For the six ultrasonic pulse signals, an ultrasonic pulse signal is time-shifted relative to an immediately preceding ultrasonic pulse signal by a predetermined amount  $\tau = 1/(2f_s)$ .

[0038] The ultrasonic pulses  $P_1, P_2 \dots P_6$  are transmitted into the ROI 30, and the echoes reflected from the region 30 and sensed by the transducer as usual. The six echo signals  $E_1, E_2 \dots E_6$  are then interleaved in a sequence of initial samples to form an operating signal  $W(t)$ . In accordance with the expression of the operating signal  $W(t)$  as above,  $W(t)$  can be represented:

$$W(t) = A(t) \sin(\omega t + \Phi_e) \cos(4\pi f_s \cdot t) + \frac{1}{2} H(t) + \frac{1}{2} H(t) \cos(8\pi f_s \cdot t)$$

[0039] It can be concluded from the expression of  $W(t)$ : the linear component is moved to either side of  $2 \cdot f_s$  in frequency domain; the two central frequencies are located at  $(2f_s - \omega/2\pi)$  and  $(2f_s + \omega/2\pi)$  respectively; for the nonlinear component, half of which is maintained at the original fundamental frequency and the other half of which is moved to either side of  $4 \cdot f_s$ ; and the two central frequencies are located at  $(4f_s - \omega/\pi)$  and  $(4f_s + \omega/\pi)$ . In this embodiment, the effective sampling rate of the operating signal is increased to six times the initial sampling rate, that is, to  $6 \cdot f_s$  ( $K=6$ ). Due to the interference of frequency overlap, within an active range of  $0 \sim 3 f_s$  for frequency detection, the linear component, which is moved to both sides of  $2 \cdot f_s$ , is overlapped or partly overlapped with the nonlinear component, which is moved to both sides of  $4f_s$  ( $-4f_s + 6f_s = 2f_s$ ) at  $2 \cdot f_s$  in the frequency domain. However, the other half of the nonlinear component, which is maintained at original fundamental frequency, is not significantly affected by the frequency overlap. Since half of the nonlinear component, which is maintained at original frequency, is separated from the linear component, which is moved to either side of  $2 \cdot f_s$  in the frequency domain, and the half of the nonlinear component, which is maintained at original frequency, is not interfered with significantly by the frequency overlap, the linear component can be filtered out using conventional filtering methods and the nonlinear component  $H(t)$  can be extracted from the operating signal  $W(t)$ .

[0040] In an ultrasonic imaging system according to a preferred embodiment,  $K$  ultrasonic pulse signals are emitted into a region of interest of a body for each scan line in a scan plane. Accordingly,  $K$  echoes are reflected by the region of interest. An operating signal is formed by interleaving  $K$  echoes signals. When the operating signal is detected to extract the information from the nonlinear component of the echoes, the frequency of the linear component of the echoes is modulated away so as to enable more efficient separation from the nonlinear component in frequency domain.

[0041] The offset pulse ultrasonic imaging system and method thereof should not be limited to embodiments mentioned above. It will be apparent to those skilled in the art that the various aspects of the invention claimed may be practiced in other examples that depart from these specific details.

[0042] In an alternative embodiment of the ultrasonic imaging method, a plurality of groups of ultrasonic pulses are transmitted into a region of interest of a body for each scan line in a scan plane, wherein each group of ultrasonic pulses comprises  $K$  ultrasonic pulses. For example, a transmit circuit may generate three groups of ultrasonic pulses for each scan line in a scan plane, each group of ultrasonic pulses comprising two ultrasonic pulses  $P_1$  and  $P_2$ , wherein  $P_2$  is time-shifted relative to  $P_1$  by a predetermined amount, and the two ultrasonic pulses  $P_1$  and  $P_2$  are optionally weighted by corresponding weight coefficients. The predetermined amount and the corresponding weight coefficients may adopt parameters disclosed in above embodiments. The three groups of ultrasonic pulses ( $P_1, P_2, P_1, P_2, P_1, P_2$ ) are emitted into the region of interest. The echoes reflected from the region of interest are received by the probe/transducer as usual. The received echoes accordingly include six echo signals ( $E_1, E_2, E_1, E_2, E_1, E_2$ ). Each group of echo signals ( $E_1, E_2$  pair) is interleaved in a sequence of initial samples to form an operating signal associated with the group of echo signals. Therefore, three groups of echo signals ( $E_1, E_2$  pairs) are interleaved to form three operating signals  $W_1, W_2, W_3$ . The nonlinear component associated with each of the groups of echo signals is then extracted from the corresponding

operating signal; that is, nonlinear components  $h_1$ ,  $h_2$  and  $h_3$  are extracted from  $W_1$ ,  $W_2$ ,  $W_3$  respectively. In a module such as the detector in above embodiments, the extracted nonlinear components  $h_1$ ,  $h_2$  and  $h_3$  can be combined, for example, as a resultant of the extracted nonlinear components, by summing the nonlinear components, i.e.  $H = h_1 + h_2 + h_3$ . The SNR (signal-to-noise ratio) of  $H$  may thereby be improved in comparison with the SNR of each of linear components  $h_1$ ,  $h_2$  and  $h_3$ .

**[0043]** In addition, the selector described above may be configured to allow for user adjustment. The selector may select suitable  $K$  and  $\alpha$  values based on the active range of frequency detection. With the selected  $K$  and  $\alpha$ , a transmit circuit generates  $K$  ultrasonic pulse signals for each scan line in a scan plane. In an alternative embodiment, a particular transmit circuit may generate a predetermined plurality of ultrasonic pulse signals for each scan line in a scan plane.

**[0044]** Further, as in other embodiments, the amplitude of each of the  $K$  ultrasonic pulse signals may be weighted by a corresponding weight coefficient. In an alternative embodiment,  $K$  ultrasonic pulse signals are emitted to a region of interest of a body for each scan line in a scan plane, wherein the amplitude of each of the  $K$  ultrasonic pulse signals is not weighted.  $K$  echoes are reflected by the region of interest accordingly. An operating signal is formed by interleaving  $K$  echoes signals. When the operating signal is detected to extract nonlinear component of the echoes, the effective sampling rate of the operating signal is increased to  $K$  times the initial sample rate  $f_s$ . Since the linear component is not modulated, the linear component may be overlapped with the nonlinear component in the frequency domain. A narrow-band filter that passes narrowband ultrasonic pulse signals may then be used to extract the nonlinear component in this embodiment.

**[0045]** Also, an ultrasonic pulse signal is time-shifted relative to an immediately preceding ultrasonic pulse signal by a predetermined amount. In some of the above-mentioned embodiments, the time-shift  $\tau = 1/(K \cdot f_s)$  wherein  $f_s$  is the initial sample rate for each scan line. In an alternative embodiment, the time-shift  $\tau$  may be set another predetermined value, for example  $1/(2 \cdot K \cdot f_s)$ . Correspondingly, some modifications might be made to the ultrasonic imaging system. For example, a synchronizer may be added into the system as needed to keep the ultrasonic pulse signals emitted by the transmit circuit and the received echoes synchronized so as to form an operating signal.

**[0046]** Figures 8-11 illustrate in a different and perhaps more visible way the two-pulse embodiment of the invention described above. The illustrated example also shows the principle of the invention in terms of phase shift instead of time shift, although these two representations are of course equivalent mathematically. In the illustrated example, two transmit pulses  $P1(t)$  and  $P2(t)$  are shown in greatly simplified form for the sake of clarity; all skilled in medical ultrasound engineering realize that actual transmit pulses from a modern ultrasound imaging transducer - especially with the usual multi-element phased piezoelectric array - may have a much more complicated waveform.

**[0047]** The main point to be illustrated in Figure 8 is that the second pulse in the series is generated so as to be offset in phase from  $P1$  by  $\Delta\theta$ , which is neither 0 degrees nor 180 degrees. In other words, in this invention, the second pulse  $P2$  is not just a "repeat" (0° phase shift or a multiple of 360°) of the first pulse  $P1$ , nor is it the "inverse" (180° phase shift or a multiple thereof) of  $P1$ , but is rather offset from  $P1$  by an amount that is other than 0° or 180°.

**[0048]** Sampling of analog signals to generate corresponding numerical representations is of course a well-known feature of almost all digital signal processing. In Figures 9a and 9b, receive/echo signals  $E1$ ,  $E2$  corresponding to transmit pulses  $P1$ ,  $P2$ , respectively, are illustrated in discrete form, such that  $E1 = E1(i)$ ,  $i = 0, 1, \dots$  and  $E2 = E2(j)$ ,  $j = 0, 1, \dots$

**[0049]** Figure 10 illustrates graphically how  $E1$  and  $E2$  may be interleaved such that the values  $E2(j)$  are aligned "in between" temporally adjacent values of  $E1(i)$ . If  $P2$  is sampled at the same frequency as  $P1$ , then each  $E2(j)$  value can be interleaved temporally in the middle of the adjacent  $E1(i)$  values. The combined, that is, interleaved resultant operating signal  $W$  will thereby have twice as many values per cycle as either  $E1$  or  $E2$  alone; in other words, the effective sampling rate of the interleaved resultant signal is twice the actual sampling rate used to quantize each of the return signals from  $P1$  and  $P2$ . The combined, interleaved operating signal  $W$  can then be processed as if it were a single discrete received signal

**[0050]** Those skilled in the art will readily see how the two-pulse embodiment illustrated in Figures 8-10 can be extended to even more pulses with suitable relative offsets. In other words, although Figures 8-10 illustrate an example with  $K=2$ , the principle can be extended to embodiments in which  $K>2$ .

**[0051]** Figure 11 illustrates the effect of transmit pulse offsetting and receive pulse interleaving. Assume first that there were no such offsetting and interleaving. The spectral component at the fundamental frequency  $f_0$  (shown with the dashed line) and the spectral component at the first harmonic (centered on  $2f_0$ ) will overlap (shown with hatched shading); moreover, even a narrow-band filter will typically also pass energy from the fundamental component in addition to the harmonic information, noise, and non-linear information  $N$ . One prior art way to try to overcome this inherent problem is to then try to extract even higher-order harmonic information, but as is well known, the amplitude of such higher-order harmonics becomes lower and lower, thereby making it more and more difficult to maintain a good signal-to-noise ratio.

**[0052]** The effect of transmit pulse offsetting and return signal interleaving and compounding is that the spectral component at the fundamental frequency  $f_0$  is shifted both upward and downward relative to the origin, with the positive shift (illustrated by the arrow arc from the dashed  $f_0$  "curve" to the solid  $f_s + f_0$  curve). One advantage of this is that a band-

pass filter narrowly tuned to the harmonic  $2f_0$  is not necessary; rather, even a broader-spectrum filter  $f$  can suffice; alternatively, the signal from a band-pass filter will not be as degraded by component overlap.

[0053] The amount of offset, that is,  $\Delta\theta$  may be adjusted according to the needs of any given implementation of the invention and could even be made user-adjustable during scans to find a "best" image result. In general, as  $\Delta\theta$  increases, the degree of separation, that is, fundamental component up-shift, will increase, but accuracy will decrease. For  $K=2$ , a suitable value for  $\Delta\theta$  will typically be  $\Delta\theta = (f_s/2f_0) (1/360)$ .

## Claims

1. A method for creating an image of a region of interest (30) of a body comprising:

transmitting a first ultrasonic pulse (P1) into the region of interest;  
 sensing first received signals (E1) corresponding to ultrasonic energy from the first ultrasonic pulse reflected from within the region of interest;  
 transmitting a second ultrasonic pulse (P2) into the region of interest;  
 sensing second received signals (E2) corresponding to ultrasonic energy from the second ultrasonic pulse reflected from within the region of interest; and  
 creating the image of the region of interest as a function of the first and second received signals;  
 in which the second ultrasonic pulse is phase-shifted relative to the first ultrasonic pulse by an amount other than zero degrees and 180 degrees the method being **CHARACTERISED BY:**

interleaving discrete representations of the first and second received signals to form a resultant operating signal (W); and  
 creating the image as a function of the resultant operating signal.

2. The method of claim 1, further comprising:

extracting a nonlinear component from the operating signal; and  
 beamforming the nonlinear component to generate a scan line, whereby a series of scan lines form the image.

3. The method of claim 1, in which K received signals, corresponding to echo signals from respective, relatively phase-offset transmitted ultrasonic pulses, are quantized and interleaved to form the resultant operating signal.

4. The method of claim 3, in which K is greater than two.

5. The method of claim 3, in which:

the phase shift is chosen such that the second ultrasonic pulse is transmitted with a time delay of  $1/K \cdot f_s$ ; and the received signals are quantized with an initial sampling rate of  $f_s$ .

6. The method of claim 3, wherein amplitudes of the K ultrasonic pulses are weighted by corresponding weight coefficients.

7. The method of claim 6, wherein the weight coefficient for the amplitude of a  $k^{\text{th}}$  ultrasonic pulse is

$$\cos\left(\frac{2\pi(k-1)}{K} \cdot \alpha\right), \quad k = 1, 2 \dots K,$$

$\alpha$  is positive integer and the center frequency of the linear component is moved to  $\alpha f_s$ .

8. The method of claim 7, wherein the  $(K, \alpha)$  is selected from any one of groups of (2, 1) and (6, 2).

9. The method of claim 2, further comprising frequency filtering the operating signal using a filter than passes not only

a frequency that is a harmonic of a fundamental signal frequency, but also energy at the fundamental signal frequency itself.

10. A system for creating an image of a region of interest (30) of a body comprising:

an ultrasound transducer (20) for transmitting a first ultrasonic pulse (P1) and at least a second ultrasonic pulse (P2) into the region of interest;  
 the ultrasound transducer being arranged to sense first and second received signals (E1, E2) corresponding to ultrasonic energy from the first and ultrasonic pulses, respectively, from within the region of interest;  
 transmit control circuitry (10) for causing the ultrasound transducer to generate the second ultrasonic pulse phase-shifted relative to the first ultrasonic pulse by an amount other than zero degrees and 180 degrees  
 reception circuitry (40, 50, 60) for creating the image of the region of interest as a function of the first and second received signals,

**CHARACTERIZED in that**

the reception circuitry includes an interleaver (40) provided for interleaving discrete representations of the first and second received signals to form a resultant operating signal; and  
 detection (50) and beamforming (60) circuitry is provided for creating the image as a function of the resultant operating signal.

11. The system of claim 10, in which the detection and beamforming circuitry comprises:

a detector (50) configured to extract a nonlinear component from the operating signal for each group of ultrasonic pulses and to generate a resultant of the nonlinear component for each group of transmitted ultrasonic pulses; and  
 a beamformer (60) configured to beamform the resultant of the nonlinear component for each group of ultrasonic pulses to generate a scan line, whereby a series of scan lines form the image.

12. The system of claim 10, in which the reception circuitry is configured to quantize and interleave  $K$  received signals, corresponding to echo signals from respective, relatively phase-offset transmitted ultrasonic pulses, to form the resultant operating signal.

13. The system of claim 12, in which  $K$  is greater than two.

14. The system of claim 12, in which:

$K$  is two or greater;  
 the transmit control circuitry (10) is configured to choose the phase shift such that the second ultrasonic pulse is transmitted with a time delay of  $1/K \cdot f_s$ ; and  
 the reception circuitry (40, 50, 60) is configured to quantize the received signals with an initial sampling rate of  $f_s$ .

15. The system of claim 14, wherein the transmit control circuitry (10) is configured to weight the amplitudes of the  $K$  ultrasonic pulses by corresponding weight coefficients.

16. The system of claim 15, wherein  
 the weight coefficient for the amplitude of a  $k^{\text{th}}$  ultrasonic pulse is

$$\cos\left(\frac{2\pi(k-1)}{K} \cdot \alpha\right), k = 1, 2 \dots K,$$

$\alpha$  is positive integer and  
 the center frequency of the linear component is moved to  $\alpha f_s$ .

**Patentansprüche**

1. Ein Verfahren zur Erstellung eines Bildes eines Untersuchungsbereichs (30) eines Körpers mit:

der Übertragung eines ersten Ultraschallimpulses (P1) in den Untersuchungsbereich,

## EP 2 434 957 B1

der Erfassung erster Empfangssignale (E1), die der Ultraschallenergie des ersten Ultraschallimpulses entsprechen, der vom Untersuchungsgebiet reflektiert wird,  
der Übertragung eines zweiten Ultraschallimpulses (P2) in den Untersuchungsbereich,  
der Erfassung zweiter Empfangssignale (E2), die der Ultraschallenergie des zweiten Ultraschallimpulses entsprechen, der vom Untersuchungsgebiet reflektiert wird, und  
der Erstellung einer Aufnahme des Untersuchungsbereichs als Funktion der ersten und zweiten Empfangssignale,  
wobei der zweite Ultraschallimpuls im Vergleich zum ersten um einen Betrag phasenverschoben ist, der ungleich 0 und 180 Grad ist,  
ein Verfahren **DADURCH GEKENNZEICHNET, DASS:**

diskrete Abbildungen der ersten und zweiten Empfangssignale überlappt werden, um ein daraus resultierendes Arbeitssignal (W) zu bilden, und  
die Aufnahme als Funktion des resultierenden Arbeitssignals erstellt wird.

2. Das Verfahren gemäß Anspruch 1, das weiterhin Folgendes aufweist:  
die Extraktion einer nichtlinearen Komponente des Arbeitssignals und die Strahlformung der nichtlinearen Komponente zur Generierung einer Abtastlinie wobei eine Reihe von Abtastlinien die Aufnahme ergibt.

3. Das Verfahren gemäß Anspruch 1, bei dem K Empfangssignale, die den Echosignalen der entsprechenden, phasenversetzt ausgesendeten Ultraschallimpulse entsprechen, quantisiert und überlappt werden, um das sich ergebende Arbeitssignal zu bilden.

4. Das Verfahren gemäß Anspruch 3, wobei K größer 2 ist.

5. Das Verfahren gemäß Anspruch 3, wobei:

die Phasenverschiebung so gewählt wird, dass der zweite Ultraschallimpuls mit einer Zeitverzögerung von  $1/K \cdot f_s$  übertragen wird, und  
die empfangenden Signale mit einer anfänglichen Abtastrate von  $f_s$  quantisiert werden.

6. Das Verfahren gemäß Anspruch 3, wobei die Amplituden der K Ultraschallimpulse durch entsprechende Gewichtungskoeffizienten gewichtet werden.

7. Das Verfahren gemäß Anspruch 6, wobei für den Gewichtungskoeffizient der Amplitude des k-ten Ultraschallimpulses gilt:

$$\cos\left(\frac{2\pi(k-1)}{K} \cdot \alpha\right), \quad k = 1, 2 \dots K,$$

$\alpha$  ist eine positive Ganzzahl, und die Mittenfrequenz der linearen Komponente wird zu  $\alpha f_s$  verschoben.

8. Das Verfahren gemäß Anspruch 7, wobei  $(K, \alpha)$  aus einer der Gruppen (2, 1) und (6, 2) gewählt werden.

9. Das Verfahren gemäß Anspruch 2, das weiterhin eine Frequenzfilterung des Arbeitssignals mit einem Filter enthält, der nicht nur eine Frequenz überträgt, die eine Harmonische der Grundsignalfrequenz ist, sondern auch Energie mit der Grundsignalfrequenz selbst.

10. Ein System zur Erstellung einer Aufnahme eines Untersuchungsbereichs (30) eines Körpers mit:

einem Ultraschallwandler (20) zur Übertragung eines ersten Ultraschallimpulses (P1) und mindestens eines zweiten Ultraschallimpulses (P2) in den Untersuchungsbereich,  
wobei der Ultraschallwandler zur Erfassung der ersten und zweiten Empfangssignale (E1, E2) ausgelegt ist, die der Ultraschallenergie des ersten und zweiten Ultraschallimpulses entsprechen, die vom Untersuchungsgebiet reflektiert werden,  
einem Übertragungssteuerkreis (10), um den Ultraschallwandler zur Generierung des zum ersten Ultraschallimpuls um einen Betrag, der weder 0 noch 180 Grad entspricht, phasenversetzten zweiten Ultraschallimpulses

zu bringen, wobei der Steuerkreis (40, 50, 60) der Erstellung der Aufnahme des Untersuchungsbereichs als Funktion der ersten und zweiten Empfangssignale dient,

**DADURCH GEKENNZEICHNET, dass**

der Empfangskreis einen Interleaver (40) enthält, der dem Überlappen der diskreten Abbildungen der ersten und zweiten Empfangssignale dient, um ein daraus resultierendes Arbeitssignal zu bilden, und der Erfassungs- (50) und Strahlenformungskreis (60) der Erstellung der Aufnahme als Funktion des resultierenden Arbeitssignals dient.

11. Das System gemäß Anspruch 10, bei dem der Erfassungs- und Strahlenformungskreis Folgendes enthält:

einen Sensor (50), der zur Extraktion einer nichtlinearen Komponente des Arbeitssignals für jede Ultraschallimpulsgruppe und zur Generierung der Resultierenden der nichtlinearen Komponente jeder Gruppe übertragener Ultraschallimpulse ausgelegt ist und

einen Strahlformer (60), der zur Strahlformung der Resultierenden der nichtlinearen Komponente jeder Gruppe übertragener Ultraschallimpulse ausgelegt ist, um eine Abtastlinie zu generieren, wobei eine Serie von Abtastlinien die Aufnahme ergibt.

12. Das System gemäß Anspruch 10, bei dem der Empfangskreis zur Quantisierung und Überlappung der K Empfangssignale dient, die den Echosignalen der entsprechenden, phasenversetzt ausgesendeten Ultraschallimpulse entsprechen, um das sich ergebende Arbeitssignal zu bilden.

13. Das System gemäß Anspruch 12, wobei K größer 2 ist.

14. Das System gemäß Anspruch 12, wobei:

K 2 oder größer ist,

der Übertragungssteuerkreis (10) so ausgelegt ist, dass die Phasenverschiebung so gewählt wird, dass der zweite Ultraschallimpuls mit einer Zeitverzögerung von  $1/K \cdot f_s$  übertragen wird, und

der Empfangskreis (40, 50, 60) so ausgelegt ist, dass die empfangenden Signale mit einer anfänglichen Abtastrate von  $f_s$  quantisiert werden.

15. Das System gemäß Anspruch 14, wobei der Übertragungssteuerkreis (10) so ausgelegt ist, dass die Amplituden der K Ultraschallimpulse durch entsprechende Gewichtungskoeffizienten gewichtet werden.

16. Das System gemäß Anspruch 15, wobei für den Gewichtungskoeffizient der Amplitude des k-ten Ultraschallimpulses gilt:

$$\cos\left(\frac{2\pi(k-1)}{K} \cdot \alpha\right), k = 1, 2 \dots K,$$

$\alpha$  ist eine positive Ganzzahl, und die Mittenfrequenz der linearen Komponente wird zu  $af_s$  verschoben.

## Revendications

1. Procédé de création d'une image d'une zone d'intérêt (30) d'un corps comprenant les étapes consistant à :

transmettre une première impulsion ultrasonore (P1) dans la zone d'intérêt ;

détecter des premiers signaux reçus (E1) correspondant à l'énergie ultrasonore de la première impulsion ultrasonore réfléchiée par l'intérieur de la zone d'intérêt ;

transmettre une deuxième impulsion ultrasonore (P2) dans la zone d'intérêt ;

détecter des deuxièmes signaux reçus (E2) correspondant à l'énergie ultrasonore de la deuxième impulsion ultrasonore réfléchiée par l'intérieur de la zone d'intérêt ; et

créer l'image de la zone d'intérêt sous la forme d'une fonction des premiers et deuxièmes signaux reçus ;

dans lequel la deuxième impulsion ultrasonore est déphasée par rapport à la première impulsion ultrasonore d'une quantité autre que zéro degré et 180 degrés, le procédé étant **CARACTERISE PAR** :

## EP 2 434 957 B1

le fait d'entrelacer des représentations discrètes des premiers et deuxièmes signaux reçus afin de former un signal de fonctionnement résultant (W) ; et  
le fait de créer l'image sous la forme d'une fonction du signal de fonctionnement résultant.

5 2. Procédé selon la revendication 1, comprenant en outre :

le fait d'extraire une composante non linéaire du signal de fonctionnement ; et  
le fait de réaliser un beamforming (formation de voies) sur la composante non linéaire afin de générer une ligne de balayage, grâce à quoi une série de lignes de balayage forment l'image.

10 3. Procédé selon la revendication 1, dans lequel K signaux reçus, correspondant aux signaux d'écho des impulsions ultrasonores transmises, déphasées les unes par rapport aux autres, respectives sont quantifiés et entrelacés pour former le signal de fonctionnement résultant.

15 4. Procédé selon la revendication 3, où K est supérieur à deux.

5. Procédé selon la revendication 3, dans lequel :

20 le déphasage est choisi de telle sorte que la deuxième impulsion ultrasonore est transmise avec un retard de  $1/K \cdot f_s$ ; et  
les signaux reçus sont quantifiés avec une fréquence d'échantillonnage initiale de  $f_s$ .

25 6. Procédé selon la revendication 3, dans lequel les amplitudes des K impulsions ultrasonores sont pondérées par des coefficients de pondération correspondants.

7. Procédé selon la revendication 6, dans lequel  
le coefficient de pondération pour l'amplitude d'une  $k^{\text{ième}}$  impulsion ultrasonore est

$$30 \cos\left(\frac{2\pi(k-1)}{K} \cdot \alpha\right), \quad k = 1, 2 \dots K,$$

$\alpha$  est un entier positif et  
la fréquence centrale de la composante linéaire est déplacée à  $\alpha f_s$ .

35 8. Procédé selon la revendication 7, dans lequel le  $(K, \alpha)$  est un groupe quelconque sélectionné parmi les groupes de  $(2, 1)$  et  $(6, 2)$ .

40 9. Procédé selon la revendication 2, comprenant en outre le fait de filtrer en fréquence le signal de fonctionnement en utilisant un filtre qui ne laisse passer qu'une fréquence qui est une harmonique d'une fréquence de signal fondamentale, mais également l'énergie à la fréquence de signal fondamentale elle-même.

10. Système de création d'une image d'une zone d'intérêt (30) d'un corps comprenant :

45 un transducteur ultrasonore (20) destiné à transmettre une première impulsion ultrasonore (P1) et au moins une deuxième impulsion ultrasonore (P2) dans la zone d'intérêt ;  
le transducteur ultrasonore étant agencé pour détecter des premiers et deuxièmes signaux reçus (E1, E2) correspondant à l'énergie ultrasonore des première et deuxième impulsions ultrasonores, respectivement, provenant de l'intérieur de la zone d'intérêt ;

50 un circuit de commande de transmission (10) destiné à amener le transducteur ultrasonore à générer la deuxième impulsion ultrasonore déphasée par rapport à la première impulsion ultrasonore d'une quantité autre que zéro degré et 180 degrés,

un circuit de réception (40, 50, 60) destiné à créer l'image de la zone d'intérêt sous la forme d'une fonction des premiers et deuxièmes signaux reçus,

55 **CARACTERISE en ce que**

le circuit de réception inclut un entrelaceur (40) prévu pour entrelacer des représentations discrètes des premiers et deuxièmes signaux reçus afin de former un signal de fonctionnement résultant ; et

un circuit de détection (50) et de beamforming (60) est prévu pour créer l'image sous la forme d'une fonction

du signal de fonctionnement résultant.

11. Système selon la revendication 10, dans lequel le circuit de détection et de beamforming comprend :

5 un détecteur (50) configuré pour extraire une composante non linéaire du signal de fonctionnement pour chaque groupe d'impulsions ultrasonores et pour générer une résultante de la composante non linéaire pour chaque groupe d'impulsions ultrasonores transmises ; et  
 un récepteur de beamforming (60) configuré pour réaliser un beamforming sur la résultante de la composante non linéaire pour chaque groupe d'impulsions ultrasonores afin de générer une ligne de balayage, grâce à quoi  
 10 une série de lignes de balayage forment l'image.

12. Système selon la revendication 10, dans lequel le circuit de réception est configuré pour quantifier et entrelacer K signaux reçus, correspondant aux signaux d'écho des impulsions ultrasonores transmises, déphasées les unes par rapport aux autres, respectives pour former le signal de fonctionnement résultant.

15 13. Système selon la revendication 12, où K est supérieur à deux.

14. Système selon la revendication 12, où :

20 K est supérieur ou égal à deux ;  
 le circuit de commande de transmission (10) est configuré pour choisir le déphasage de telle sorte que la deuxième impulsion ultrasonore est transmise avec un retard de  $1/K \cdot f_s$ ; et  
 le circuit de réception (40, 50, 60) est configuré pour quantifier les signaux reçus avec une fréquence d'échantillonnage initiale de  $f_s$ .

25 15. Système selon la revendication 14, dans lequel le circuit de commande de transmission (10) est configuré pour pondérer les amplitudes des K impulsions ultrasonores par des coefficients de pondération correspondants.

30 16. Système selon la revendication 15, dans lequel le coefficient de pondération pour l'amplitude d'une  $k^{\text{ième}}$  impulsion ultrasonore est

$$\cos\left(\frac{2\pi(k-1)}{K} \cdot \alpha\right), \quad k = 1, 2, \dots, K,$$

35  $\alpha$  est un entier positif et  
 la fréquence centrale de la composante linéaire est déplacée à  $\alpha f_s$ .

40

45

50

55

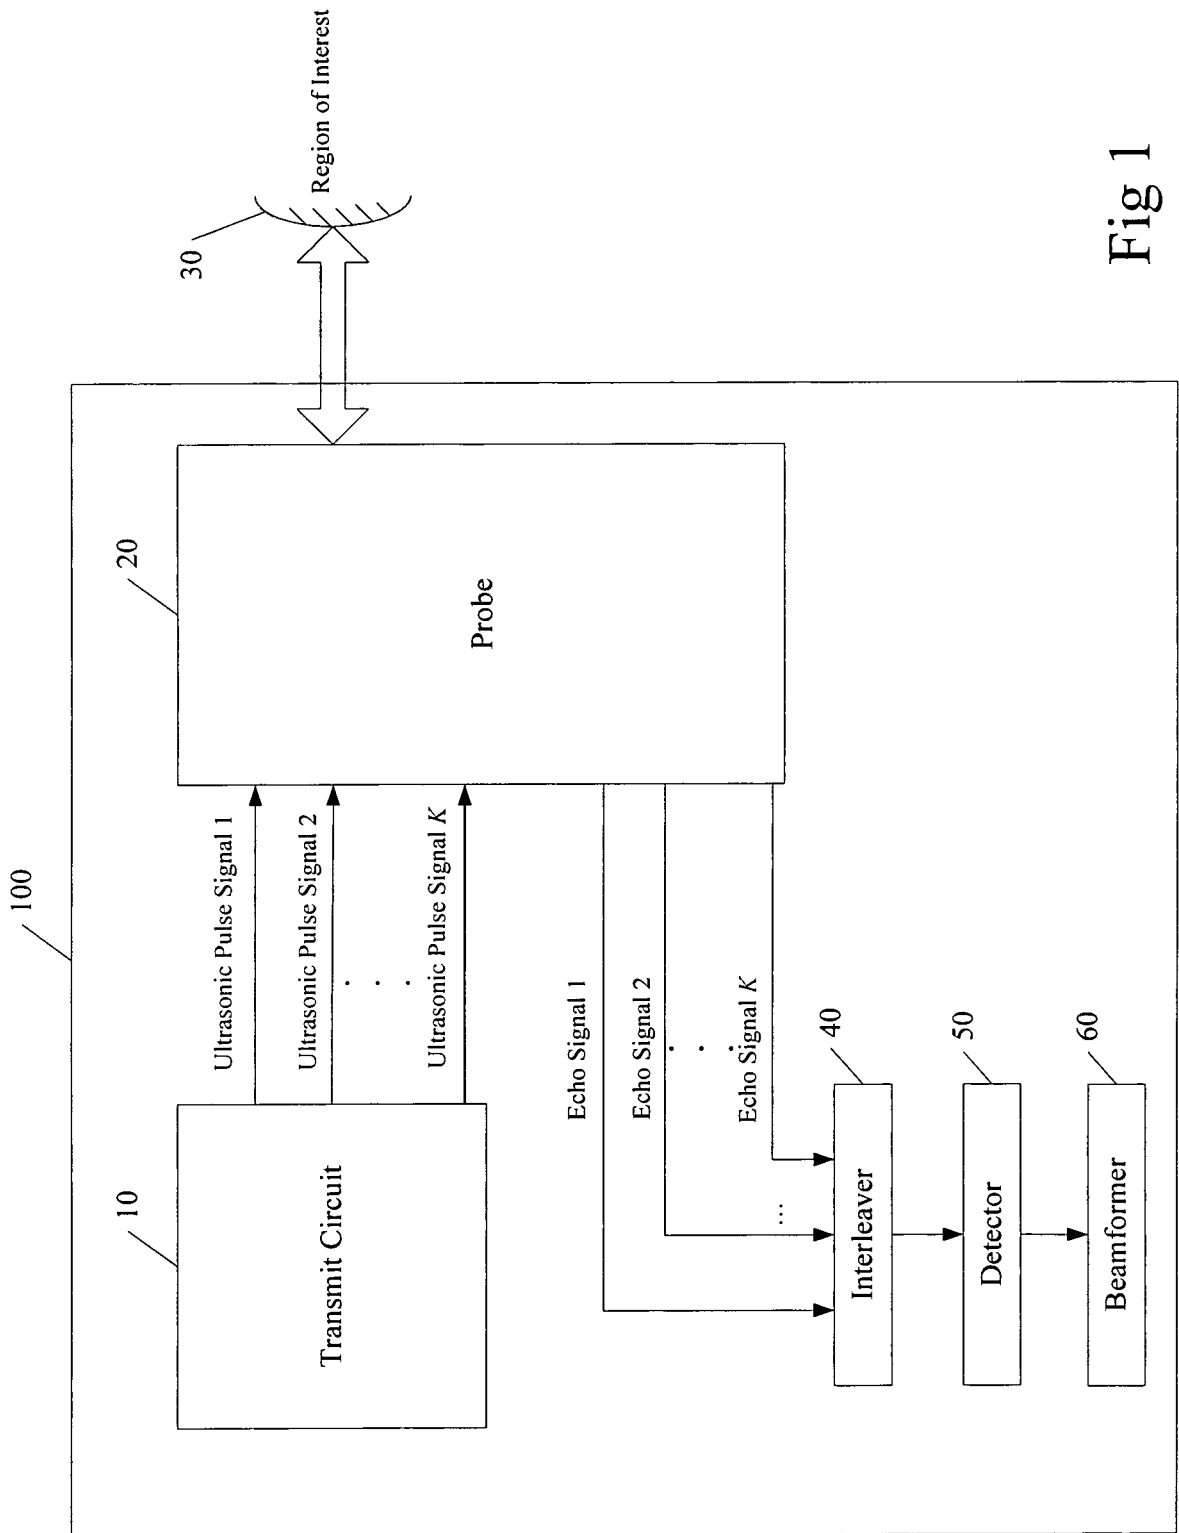


Fig 1

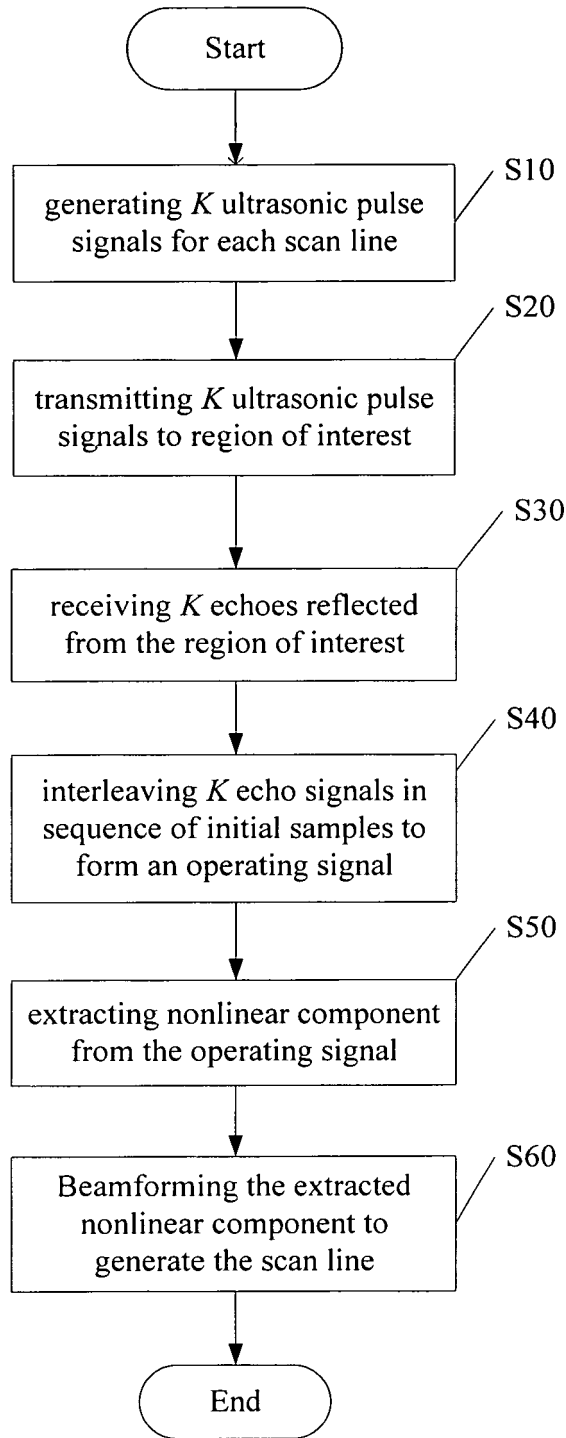


Fig 2

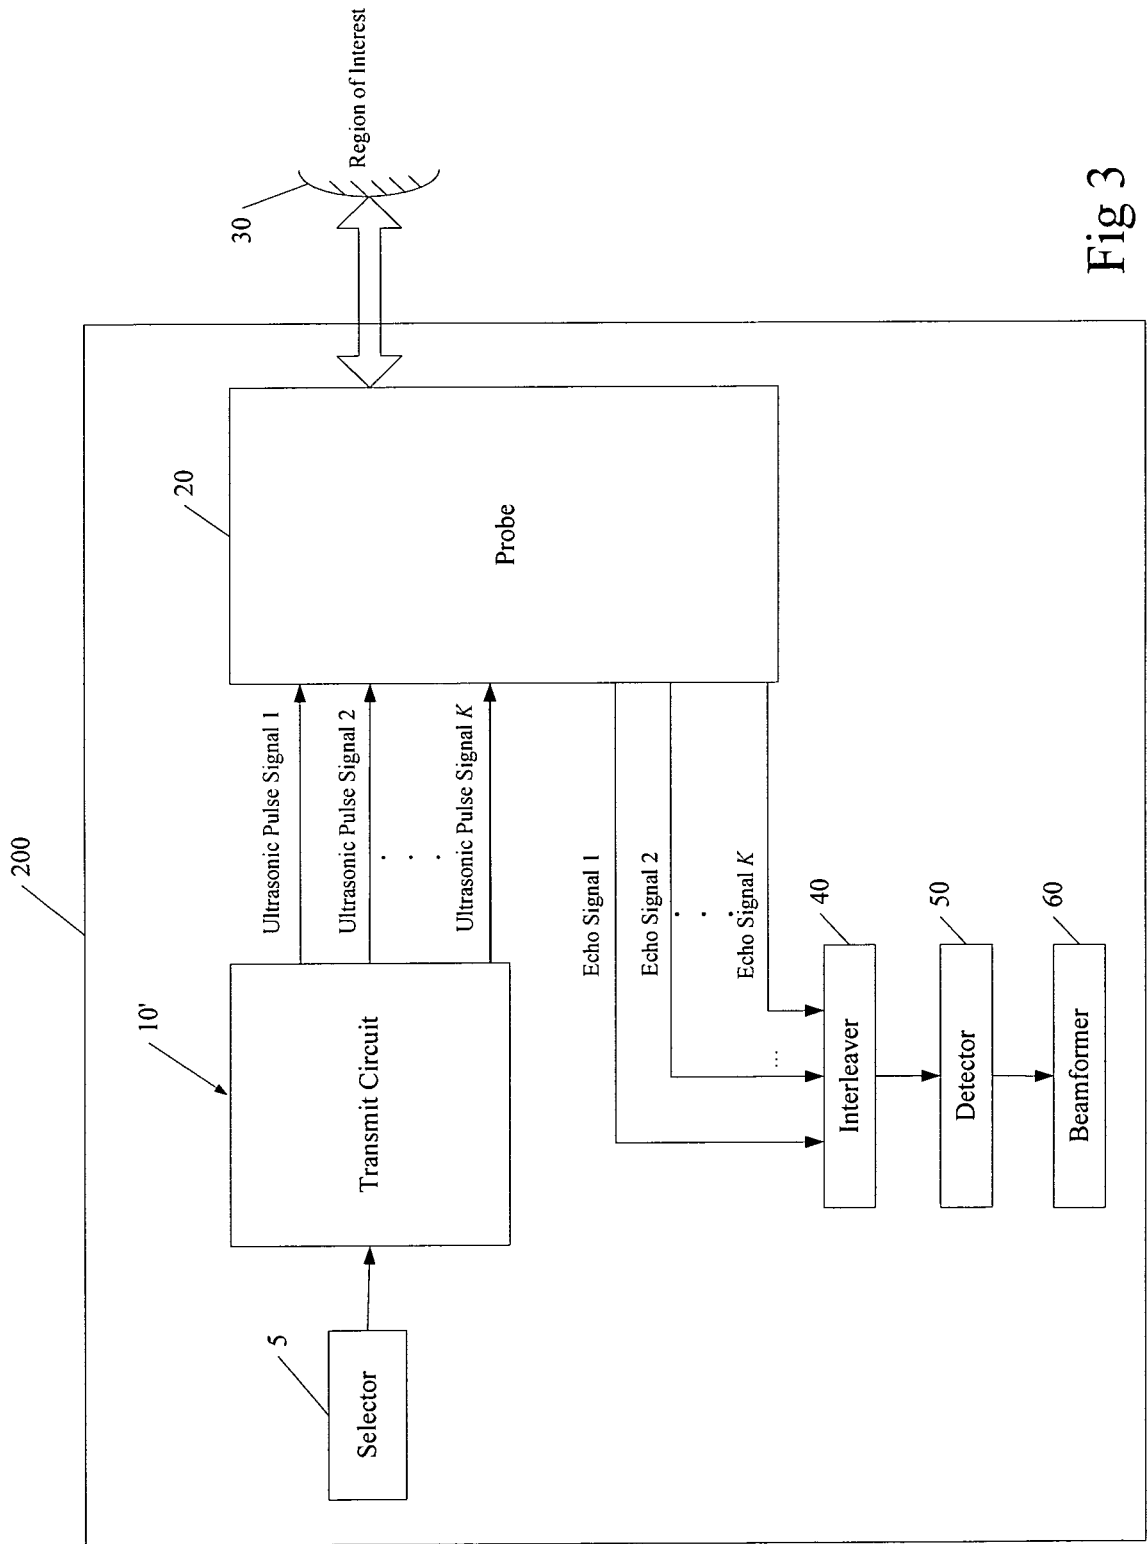


Fig 3

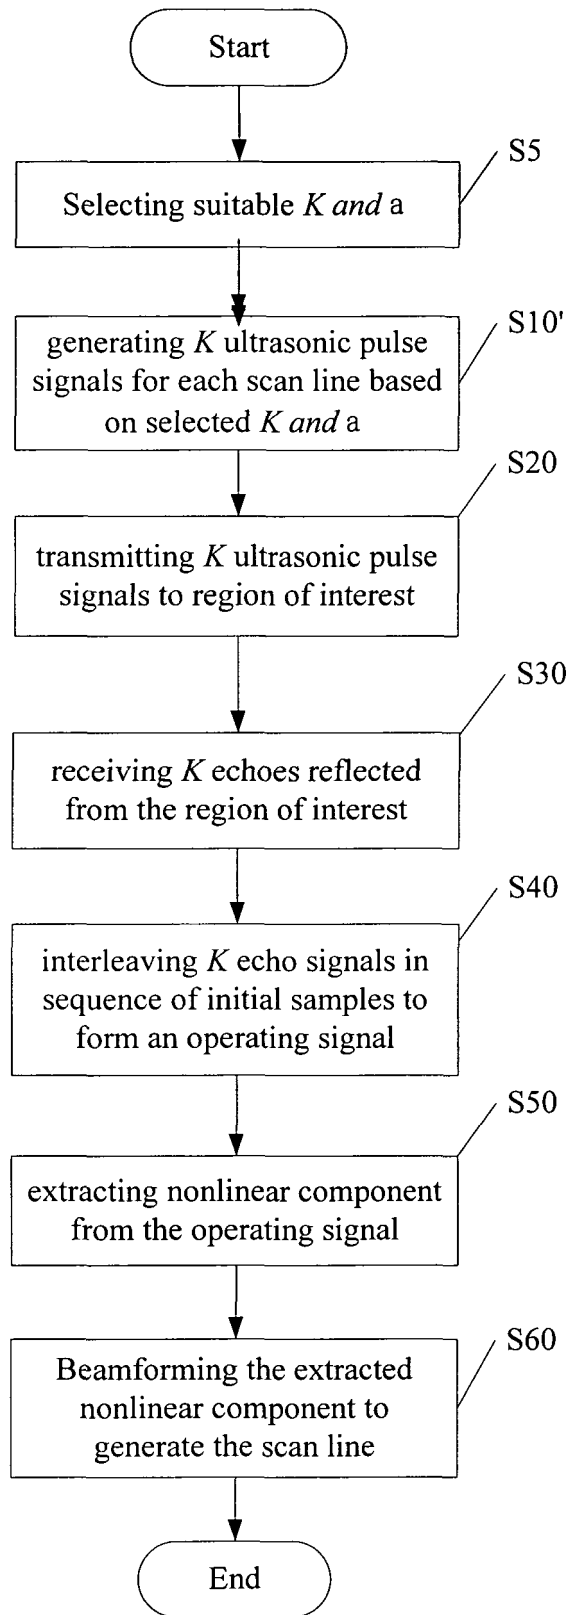


Fig 4

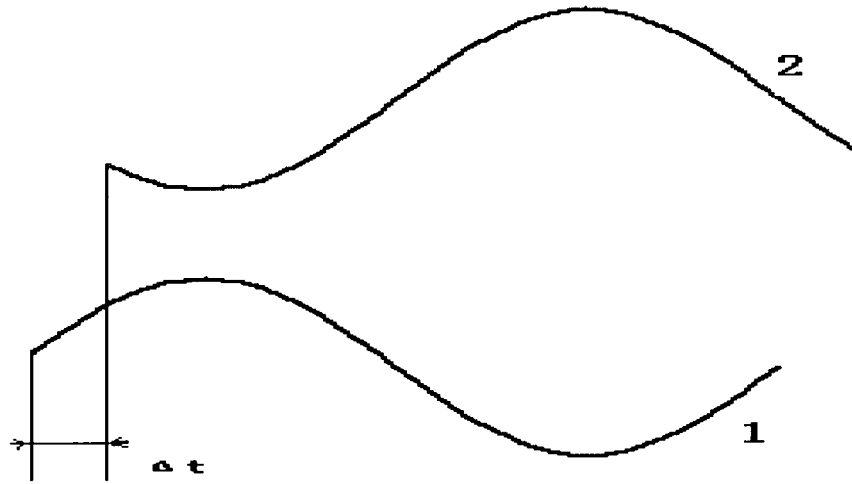


Fig 5a

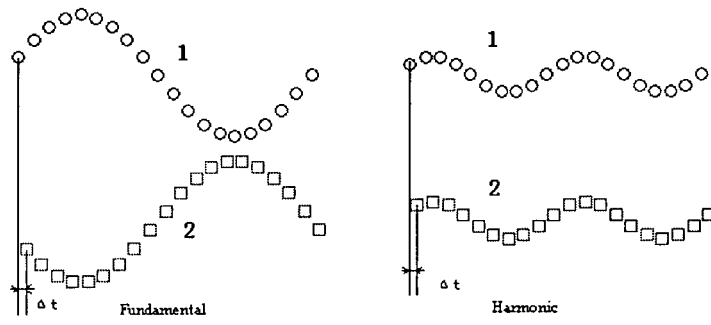


Fig 5b

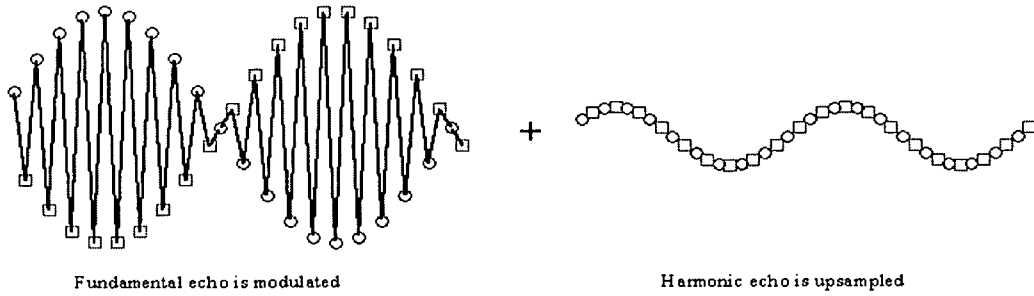


Fig 5c

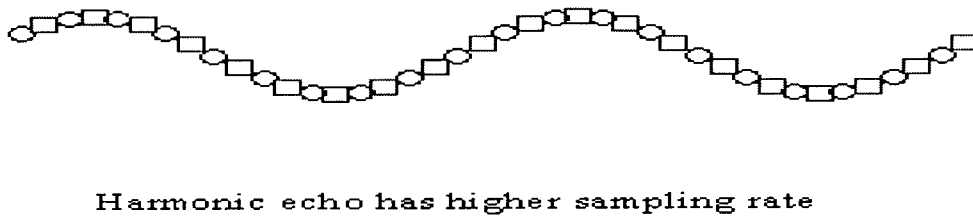


Fig 5d

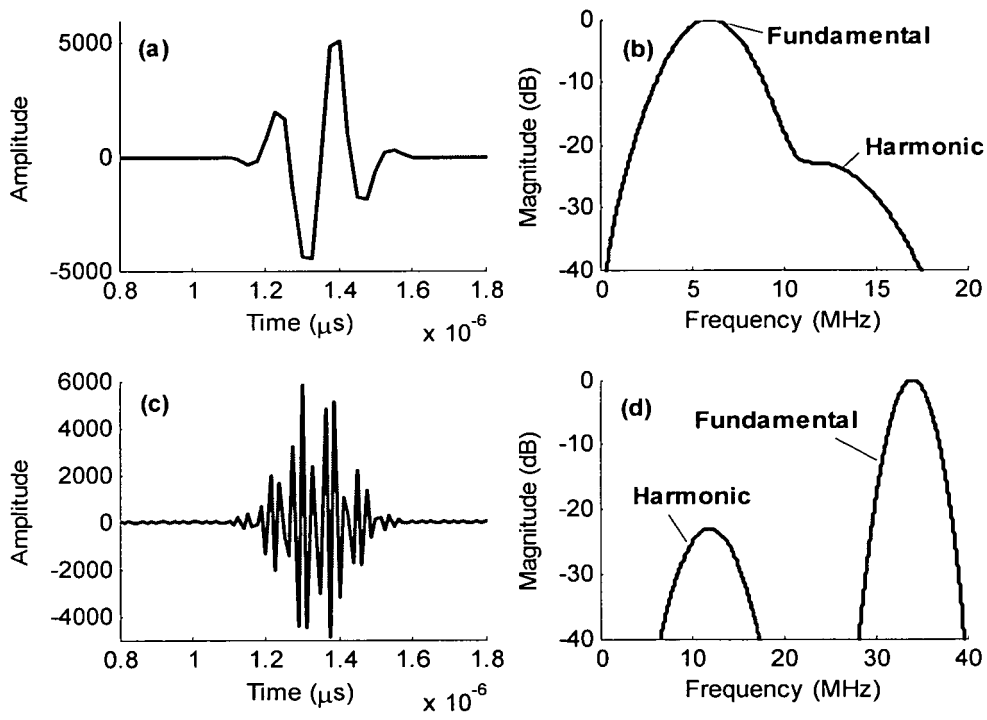


Fig 6

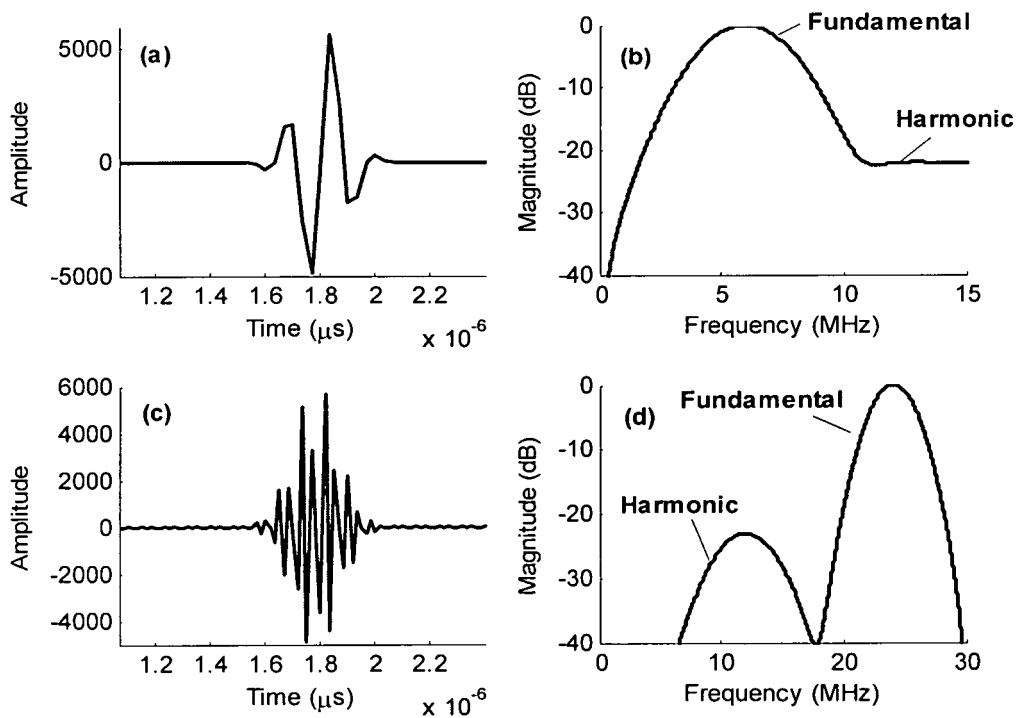


Fig 7

FIG. 8

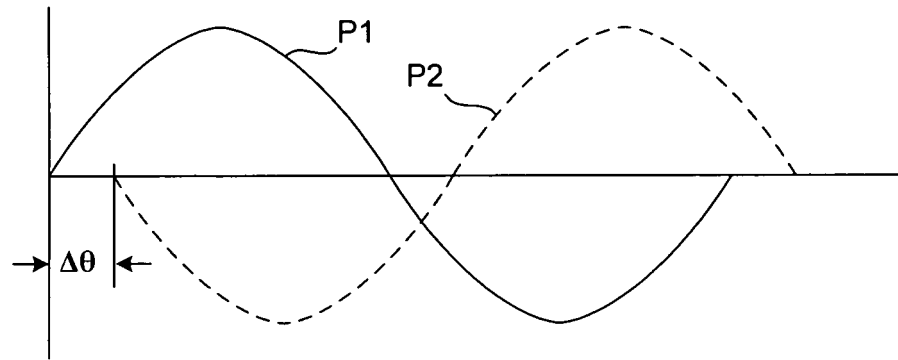


FIG. 9a

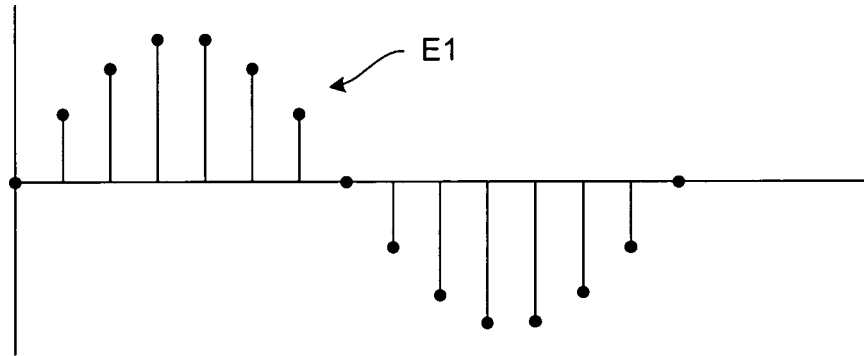


FIG. 9b

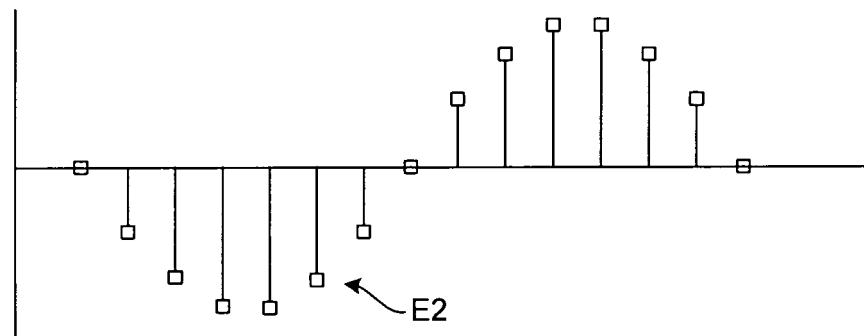


FIG. 10


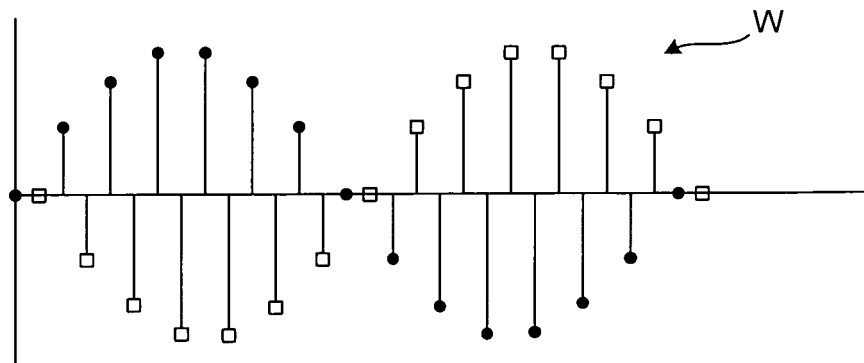


FIG. 11

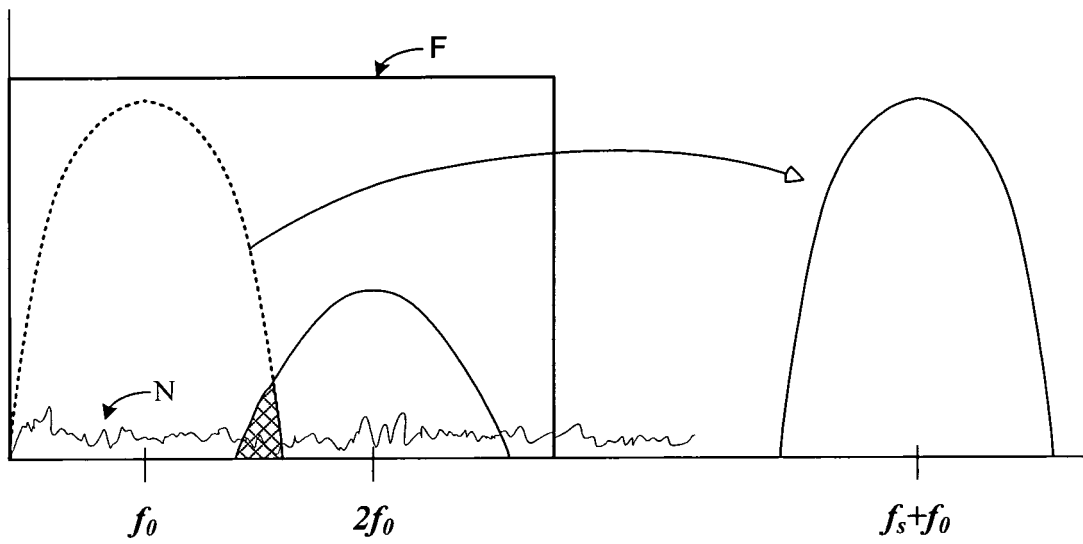

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 6206833 B [0005]
- US 7004905 B [0005]
- US 7104956 B [0005]
- US 7513870 B [0005]
- US 5632277 A [0007]
- US 5951478 A [0007]
- WO 0164108 A [0007]

专利名称(译)	脉冲移位超声成像		
公开(公告)号	<a href="#">EP2434957B1</a>	公开(公告)日	2020-01-01
申请号	EP2010780130	申请日	2010-05-25
[标]申请(专利权)人(译)	深圳迈瑞生物医疗电子股份有限公司		
申请(专利权)人(译)	深圳迈瑞生物医疗电子股份有限公司.		
当前申请(专利权)人(译)	深圳迈瑞生物医疗电子股份有限公司.		
[标]发明人	FAN RUI LI SHUANGSHUANG LI YONG		
发明人	FAN, RUI LI, SHUANGSHUANG LI, YONG		
IPC分类号	A61B8/00		
CPC分类号	A61B8/08 A61B8/14 G01S7/52038 G01S7/52046 G01S15/108 G01S15/8959 A61B8/5207		
代理机构(译)	KIPA AB		
优先权	200910133494.X 2009-05-25 CN		
其他公开文献	EP2434957A2 EP2434957A4		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

通过将至少第一超声脉冲和第二超声脉冲传送到ROI中来形成身体的感兴趣区域 ( ROI ) 的诊断超声图像，其中第二脉冲相对于第一脉冲相移了其数量的量。大于0或180度的倍数。来自脉冲的离散接收信号被交织以形成最终的操作信号，该操作信号被检测并被波束成形为操作信号。

$$\cos\left(\frac{(k-1) \cdot 2\pi}{K} \cdot \alpha\right),$$