



(11) **EP 3 089 671 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
22.05.2019 Bulletin 2019/21

(51) Int Cl.:
A61B 8/12 (2006.01) A61B 34/20 (2016.01)
A61B 8/08 (2006.01) A61B 8/00 (2006.01)
A61B 17/34 (2006.01) A61B 90/00 (2016.01)

(21) Application number: **15704590.7**

(86) International application number:
PCT/IB2015/050023

(22) Date of filing: **02.01.2015**

(87) International publication number:
WO 2015/101949 (09.07.2015 Gazette 2015/27)

(54) **INSTRUMENT ALIGNMENT AND TRACKING WITH ULTRASOUND IMAGING PLANE**

**INSTRUMENTENAUSRICHTUNG UND -VERFOLGUNG MIT
ULTRASCHALLBILDGEBUNGSEBENE**

ALIGNEMENT ET POURSUITE D'INSTRUMENT AVEC PLAN D'IMAGERIE ÉCHOGRAPHIQUE

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(72) Inventors:
• **VIGNON, Francois Guy Gerard Marie**
NL-5656 AE Eindhoven (NL)
• **JAIN, Ameet Kumar**
NL-5656 AE Eindhoven (NL)

(30) Priority: **02.01.2014 US 201461922882 P**

(43) Date of publication of application:
09.11.2016 Bulletin 2016/45

(74) Representative: **Philips Intellectual Property &
Standards**
High Tech Campus 5
5656 AE Eindhoven (NL)

(60) Divisional application:
19153574.9

(73) Proprietor: **Koninklijke Philips N.V.**
5656 AE Eindhoven (NL)

(56) References cited:
US-A1- 2010 298 704 US-A1- 2011 245 659
US-A1- 2013 041 252 US-A1- 2013 211 243

EP 3 089 671 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention generally relates to a three-dimensional ("3D") alignment and tracking of a relative position of an interventional tool (e.g., a needle, a catheter, etc.) to an acoustic image plane generated by an acoustic imaging device (e.g., a two-dimensional ("2D") ultrasound imaging probe having a one-dimensional ("1D") transducer array). The present invention specifically relates to acoustic sensors spatially aligned relative to the interventional tool (e.g., attached to or embedded in a distal tip of a needle or a catheter) for facilitating the relative alignment and position tracking of the interventional tool to the acoustic image plane.

[0002] A 2D ultrasound probe having a 1D transducer array is commonly used for visualization of a target anatomical plane in a wide range of clinical interventions. However, it is a challenge to assess a position of an interventional tool (e.g., a needle, a catheter, etc.) outside of an acoustic imaging of the target anatomical plane generated by the 2D ultrasound probe. Consequently, a clinician may spend a lot of effort and time in trying to exactly position the interventional tool inside the acoustic image of the target anatomical plane, particularly a distal tip of the interventional tool. More particularly, for interventions involving oblique/orthogonal injection of the interventional tool into the target anatomical plane, it has proven difficult to establish an exact time and position of an entry of the interventional tool inside the acoustic image of the target anatomical plane.

[0003] For example, needle insertion under ultrasound guidance is commonly performed for various interventions (e.g., biopsies, fluid drainage, nerve blocks, vascular access, etc.). While needle visualization techniques based on steering imaging beams approximately perpendicular to the needle shaft have been implemented, in a significant number of cases the needle deviates from the acoustic image plane due to tissue heterogeneities and/or bevel asymmetry. Essentially, an out-of-plane needle disappears from the acoustic image plane irrespective of the sophistication of the smart needle visualization enhancement software. The clinician then has to move the acoustical image plane to reacquire an image of the needle, but as a result loses the acoustic image of the target anatomical plane. Furthermore, the clinician does not know where the needle is in relation to the acoustic image plane and therefore the clinician has no indication how to move the 2D ultrasound probe to find the needle.

[0004] In summary, for acoustic imaging, it is an imperative operating principle to keep imaging the target anatomical plane and at the same time know the relative position of the needle with respect to the target anatomical plane. However, one major technical difficulty for acoustic imaging is to correctly align the needle and the ultrasound imaging plane for an in-plane approach and to visualize the needle tip as opposed to the shaft for an out-of-plane approach. Small probe and needle movements lead to misalignment of the needle and image plane which in turn may result in poor needle visualization, frustration, stress, loss of time, multiple needle punctures resulting in patient discomfort, and possibly bad procedure outcomes (e.g., false-negative in biopsies, unsuccessful blocks in regional anesthesia or pain management, and vessel and nerve damage).

[0005] For example, FIGS. 1A and 1B illustrate a small Y movement of a needle 30 toward an acoustic image plane 11. This small Y movement may lead to a Y misalignment of needle 30 and acoustic image plane 11 as demonstrated by the white graphical icon identically shown in an ultrasound image 10. Additionally, needles are often poorly visualized under ultrasound, because they are specular reflectors that reflect the sound away from the imaging probe with a degree of reflection depending upon the insertion angle of the needle with in the imaging plane. Nonetheless, there is value in displaying the needle tip and expected trajectory when the needle is in plane and invisible or out of plane.

[0006] A document US 2011/0245659 A1 discloses a system which facilitates the placement of an instrument internal to an object aided by an overlay superimposed on an image. The placement of a needle tip within a patient's body using an overlay superimposed on a sonographic image is facilitated. A superimposed overlay of embodiments is created by monitoring a fixed point of an external portion of the instrument in relation to an imaging transducer.

[0007] A document US 2013/0041252 A1 discloses an ultrasound receive beamformer configured for one-way only beamforming of transmissive ultrasound using one-way delays. The receive beamforming in some embodiments is used to track, in real time, a catheter, needle or other surgical tool within an image of a region of interest. The tool can have embedded at its tip a small ultrasound transmitter or receiver for transmitting or receiving the transmissive ultrasound.

[0008] A document US 2013/0211243 A1 discloses an ultrasound imaging system that has a 3D location system and a data store for recording locations within a patient. Navigation to target locations is facilitated by providing graphical elements superposed on a 2-dimensional image.

[0009] A document US 2010/0298704 A1 discloses an ultrasound system having an ultrasound transducer equipped with a position marker and a needle equipped with a position marker. The position markers allow the position and orientation of the transducer and needle to be determined.

[0010] The present invention adheres to the operating principle of acoustic imaging by facilitating a tracking and visualization of the interventional tool via an overlay of a graphical icon (e.g., a marker) indicating the interventional tool on the ultrasound image. One or more features/aspects of the graphical icon (e.g., size, color, shape, etc.) is modulated as a function of a distance of the interventional tool (e.g., the tip of the interventional tool) to the ultrasound imaging plane. For example, as shown in FIGS. 2A and 2B, a size of a graphical icon illustrated as a white X marker overlain on

ultrasound image 10 increases as interventional tool is moved in a Y direction of acoustic image plane 11 as shown in FIGS. 1A and 1B. This will significantly help a physician align the interventional tool with the imaging probe, which results in good confidence, fast procedures and good outcomes, particularly even when the interventional tool is invisible to conventional imaging (i.e., out of plane).

[0011] One form of the present invention is tool navigation system employing an ultrasound probe, an ultrasound scanner, an interventional tool (e.g., a needle or a catheter), a plurality of ultrasound transducers, a tool tracker and an image navigator. In operation, the ultrasound probe generates an acoustic image plane for scanning an anatomical region, and the ultrasound scanner generates an ultrasound image of the anatomical region from a scan of the anatomical region. During the scan, the interventional tool is navigated within the anatomical region relative to the acoustic image plane, and the ultrasound transducers facilitate a tracking by the tool tracker of a distance of the interventional tool relative to the acoustic image plane. The image navigator displays a graphical icon within the ultrasound image of the anatomical region as generated by the ultrasound scanner for illustrating a tracking of the interventional tool relative to the acoustic image plane by the tool tracker. One or more aspects of the graphical icon are modulated by the image navigator responsive to a distance of the interventional tool relative to the acoustic image plane as the interventional tool is navigated within the anatomical region.

[0012] The foregoing form and other forms of the present invention as well as various features and advantages of the present invention will become further apparent from the following detailed description of various embodiments of the present invention read in conjunction with the accompanying drawings. The detailed description and drawings are merely illustrative of the present invention rather than limiting, the scope of the present invention being defined by the appended claims and equivalents thereof.

FIGS. 1A and 1B respectively illustrate exemplary views of an ultrasound images as known in the art.

FIGS. 2A and 2B respectively illustrate an exemplary modulation of a graphical icon of the present invention of the ultrasound images shown in FIGS. 1A and 1B.

FIG. 3 illustrates an exemplary embodiment of a tool tracking system of the present invention.

FIG. 4 illustrates an exemplary interventional procedure involving the tool tracking system shown in FIG. 3.

FIG. 5 illustrates an exemplary execution of a trilateration as known in the art.

FIG. 6 illustrates a flowchart representative of a first exemplary embodiment of a graphical icon modulation method in accordance with the present invention.

FIG. 7 illustrates a flowchart representative of a second exemplary embodiment of a graphical icon modulation method in accordance with the present invention.

FIG. 8 illustrates a flowchart representative of a third exemplary embodiment of a graphical icon modulation method in accordance with the present invention.

[0013] To facilitate an understanding of the present invention, exemplary embodiments of the present invention will be provided herein directed to a tool navigation system shown in FIG. 3.

[0014] Referring to FIG. 3, the tool navigation system employs an ultrasound probe 20, an interventional tool 30, an ultrasound scanner 60, a tool tracker 70, and an image navigator 80.

[0015] Ultrasound probe 20 is any device as known in the art for scanning an anatomical region of a patient via acoustic energy to visualize subcutaneous body structures (e.g., tendons, muscles, joints, vessels and internal organ, etc.), such as, for example, a scanning an anatomical region 12 of a patient 11 as shown in FIG. 3. Examples of ultrasound probe 20 include, but are not limited to, a two-dimensional ("2D") ultrasound probe having a one-dimensional ("1D") transducer array, linear or curved.

[0016] Ultrasound scanner 60 is a structural configuration of hardware, software, firmware and/or circuitry as known in the art for generating an ultrasound image of the anatomical region of the patient as scanned by ultrasound probe 20 (e.g., an ultrasound image 10 of a fetus as shown in FIGS. 1-3).

[0017] Interventional tool 30 is any tool as known in the art for performing interventional procedures involving a navigation of interventional tool 30 within the anatomical region. Examples of interventional tool 30 include, but are not limited to, a needle and a catheter, and examples of interventional procedures include, but are not limited to, biopsies, fluid drainage, nerve blocks, vascular access, etc.

[0018] To facilitate the navigation in practice, interventional tool 30 may be equipped with one or more ultrasound transducers in the form of transmitters, receivers and/or transceivers as known in the art. More particularly, one ultrasound transducer provides information in a position of a designated area of interventional tool 30 (e.g., a distal tip of interventional tool 30), and two or more ultrasound transducers provide orientation information that facilitates a displaying of a projected path of interventional tool 30 and a projected intersection point with the ultrasound imaging plane 11, thus further facilitating out-of-plane approaches (which are otherwise blind).

[0019] In one embodiment as shown in FIG. 4, a pair of ultrasound transducers 31 are embedded in a known configuration adjacent a distal tip on interventional tool 30. When operating as transmitters, ultrasound transducers 31 may

either be separated by non-overlapping frequency ranges, and/or be fired one after the other to facilitate an individual tracking of ultrasound transducers 31. Similarly, when operated as receivers, signals for each ultrasound transducer 31 needs to be individualized (e.g., with non-overlapping bandwidths, a switch, two (2) independent cables, or signal processing methods for signal separation).

5 **[0020]** For this embodiment of interventional tool 30 as shown in FIG. 4, ultrasound probe 20 may be equipped with one or more ultrasound transducers 21 for tracking ultrasound transducers 31. More particularly, three (3) or more ultrasound transducers 21 yield satisfactory position estimates of ultrasound transducers 31. In practice, ultrasound transducers 21 are disposed on ultrasound probe 20 in a manner providing a wide acceptance angle in order to efficiently track ultrasound transducers 31 within a wide field of view.

10 **[0021]** In one embodiment of ultrasound probe 20 as shown in FIG. 4, six (6) ultrasound transducers 21 are disposed on a 2D surface around the array perimeter of ultrasound probe 20. In practice for this embodiment, ultrasound transducers 21 may be mounted on ultrasound probe 20 as a clip-on device or embedded in a design of ultrasound probe 20. In either case, a simple calibration between the tracked position and the image may be needed. Such a calibration may involve a clicking on tip of interventional tool 30 on a pulse-echo image under a controlled imaging environment.

15 **[0022]** Tool tracker 70 is a structural configuration of hardware, software, firmware and/or circuitry as known in the art for executing technique(s) for tracking a position of interventional tool 30 relative to the ultrasound image of the anatomical region. For the ultrasound tracking embodiment of ultrasound probe 20 and interventional tool 30 as shown in FIG. 4, tool tracker 70 executes a trilateration algorithm for determining a 3D position of ultrasound transducers 31 based on a time of flight of signals between ultrasound transducers 21 and ultrasound transducers 31.

20 **[0023]** In practice, three (3) pairs of location-distance are necessary to perform 3D localization and any additional pairs of location-distance increase robustness. In one embodiment, as supported by FIG. 5, a linear least-squares estimate for location of ultrasound transducers 31 may be obtained with the following equation:

25
$$\hat{\mathbf{x}}_s = (S^T S)^{-1} A^T \mathbf{b}$$

30 where $S = \begin{bmatrix} \mathbf{x}_2 \\ \mathbf{x}_3 \\ \vdots \\ \mathbf{x}_N \end{bmatrix}$, $\mathbf{b} = \frac{1}{2} \begin{bmatrix} R_2^2 - D_2^2 + D_1^2 \\ R_3^2 - D_3^2 + D_1^2 \\ \vdots \\ R_N^2 - D_N^2 + D_1^2 \end{bmatrix}$,

35 $\mathbf{x}_i = [x_i \ y_i \ z_i]$ denotes a location of an i^{th} ($i = 1, \dots, N$) transducers 21,
 $R_i = \|\mathbf{x}_i\|$ is a distance from virtual transducer 21 to a coordinate frame origin,
 $D_i = \|\mathbf{x}_i - \mathbf{x}_s\|$ is a distance between each transducer 21 and sensor 31, and
 $\mathbf{x}_1 = [0 \ 0 \ 0]$ is the location of each transducer 21 designated as the origin.

40 **[0024]** In an alternative embodiment utilizing ultrasound transducers 31 and omitting ultrasound transducers 21, tool tracker 70 executes an algorithm for computing sensor position with respect to the imaging frame of reference. More particularly, tool tracker 70 determines a projection of a 3D position (X-azimuth, Z-depth, Y-elevation) onto a 2D position in the imaging plane 12 (x-z or r-theta). For this embodiment, a Z-depth (or range) coordinate is obtained by measuring a time of flight of ultrasound signals from ultrasound probe 20 to ultrasound transducers 31, and an X-azimuth (or angular) position is obtained by searching for a maximum received amplitude across received beams at ultrasound transducers 31. A qualitative estimate of the Y coordinate (distance of the sensors 31 to imaging plane 11) is obtained by recording the received amplitude of the signals at transducers 31 and comparing it to a past history: increasing amplitude generally means that the sensors 31 are approaching imaging plane 11, whereas a decreasing amplitude means that the sensors 31 are going further away from imaging plane 11.

45 **[0025]** Image navigator 80 is a structural configuration of hardware, software, firmware and/or circuitry as known in the art for executing technique(s) for displaying an ultrasound image as generated by ultrasound scanner 60 and in accordance with the present invention for generating a graphical icon for illustrating a tracking of interventional tool 30 relative to the acoustic image plane 11 by tool tracker 70. More particularly, as interventional tool 30 is navigated within the anatomical region, image navigator 80 modulates one or more aspects of the graphical icon (e.g., size, color, shape) to qualitatively indicate a tracked distance of the interventional tool 30 relative to the acoustic image plane 11. To this end, image navigator 80 inputs data 61 from ultrasound scanner 60 representative of ultrasound image 10 and inputs
55 data 71 from tool tracker 70 representative of a 3D position (X-azimuth, Z-depth) of interventional tool 30 relative to acoustic image plane 11.

[0026] To facilitate an understanding of the graphical icon modulation, exemplary embodiments of image navigator

80 will be provided herein directed to a size modulation of a marker as shown in FIGS. 6-8 to qualitatively indicate a distance of the ultrasound transducers 31 to ultrasound image plane 11. While these exemplary embodiments use the amplitudes or signal-to-noise ratios SNRs of received signals and compares them to a history of received amplitudes or SNRs to modulate the marker appearance, those having ordinary skill in the art will appreciate how to apply the principles of these exemplary embodiments to other modulated aspects (e.g., shape, color, bar graph, etc.) and signals quantifying of the Y-elevation distance. Those having ordinary skill in the art will also appreciate various modifications and variations of these exemplary embodiments of graphical icon modulation.

[0027] Generally, it is desired that the size of the marker (the variable 'markerSize') is maximum (to a fixed maximum size 'maxSize') when the signal level (V) at ultrasound transducer 31 drops below a certain voltage or a certain SNR, and minimum (to a fixed minimum size 'minSize') when an ultrasound transducer 31 is on imaging plane 11 at any depth. At intermediate levels, the size of the marker is intermediate. In practice, the size of the marker may be the size of the marker (the variable 'markerSize') is maximum (to a fixed maximum size 'maxSize') when an ultrasound transducer 31 is on imaging plane 11 at any depth, and minimum (to a fixed minimum size 'minSize') when the signal level (V) at ultrasound transducer 31 drops below a certain voltage or a certain SNR.

[0028] Also in practice, a curve $\text{markerSize} = f(V)$ or $\text{markerSize} = f(\text{SNR})$ should be monotonically increasing or decreasing, but may be linear as described herein or nonlinear (e.g. logarithmic). When the signal levels drop below the set minimum acceptable signal level (minV or minSNR), the marker is not displayed on the screen. In all embodiments as shown in FIGS. 608, the minimum marker size ('minSize') corresponds to the minimum acceptable received voltage or received SNR, which is a fixed parameter ('minV'/minSNR'). At lower received signal levels, the marker is no longer displayed. This eliminates the possibility to display potentially wrong sensor locations in low-SNR scenarios.

[0029] In a fixed max voltage embodiment, from the minimum marker size 'minSize', a monotonically increasing curve of size versus received signal amplitude or SNR is implemented. The marker size "markerSize" is thus directly representing the received signal strength, which increases at a given depth as ultrasound transducer 31 approaches the imaging plane 11 and decreases as it goes away from the imaging plane 11. In order to limit the maximum size of the marker, it may be decided that the marker stops to grow beyond 'maxSize' after a maximum acceptable signal strength 'maxV'.

[0030] FIG. 6 illustrates a flowchart 90 representative of an exemplary fixed max voltage embodiment. Referring to FIG. 6, a stage S91 of flowchart 90 encompasses image navigator 80 acquiring parameters necessary for a calculation by image navigator 80 of 'markerSize_C' during a stage S92 of flowchart 90 as a function of the measured voltage V indicative of the received signal amplitude in accordance with the following equation:

$$\text{markerSize}_C = (V - \text{minV}) / (\text{maxV} - \text{minV}) * (\text{maxSize} - \text{minSize}) + \text{minSize}$$

[0031] A stage S93 of flowchart 90 encompasses image navigator 80 displaying a 'markerSize_D' in accordance with the following equations:

$$\begin{aligned} \text{markerSize}_D &= 0 \text{ if } \text{markerSize}_C < \text{minSize} \\ \text{markerSize}_D &= \text{maxSize} \text{ if } \text{markerSize}_C > \text{maxSize} \end{aligned}$$

[0032] Image navigator 80 returns to stage S92 to repeat stages S92 and S93 as needed.

[0033] In a variable max voltage embodiment, the maximum marker size ('maxSize') is variable and corresponds to the maximum signal strength received by ultrasound transducer 31 since the experiment was started (variable 'maxV'). Each time a signal is received, its strength is compared to the maximum past received signal. If it exceeds it, the signal 'maxV' corresponding to the maximum marker size is updated. This embodiment ensures a maximum marker size excursion as interventional tool 30 is advanced within the anatomical region.

[0034] FIG. 7 illustrates a flowchart 100 representative of an exemplary variable max voltage embodiment. Referring to FIG. 7, a stage S101 of flowchart 100 encompasses image navigator 80 acquiring parameters necessary for a calculation by image navigator 80 of 'markerSize_C' during a stage S102 of flowchart 100 as a function of the measured voltage V indicative of the received signal amplitude compared to variable 'maxV_V'. Specifically, an initial implementation of stage S101 involves setting 'maxV' to 0 and markerSize to a 'defaultSize', and stage S102 involves a setting of 'maxV_V' to the measured voltage V if measured voltage V is greater than 'maxV' or otherwise setting 'maxV_V' = "maxV". The setting of 'maxV_V' is inputted to the calculation of 'markerSize_C' in accordance with the following equation:

$$\text{markerSize}_C = (V - \text{minV}) / (\text{maxV}_V - \text{minV}) * (\text{maxSize} - \text{minSize}) + \text{minSize}$$

[0035] Thereafter, 'maxV' = "maxV_V'.

[0036] A stage S93 of flowchart 90 encompasses image navigator 80 displaying a 'markerSize_D' in accordance with the following equations:

$$\begin{aligned} \text{markerSize}_D &= 0 \text{ if } \text{markerSize}_C < \text{minsize} \\ \text{markerSize}_D &= \text{maxSize} \text{ if } \text{markerSize}_C > \text{maxSize} \end{aligned}$$

[0037] Image navigator 80 returns to stage S102 to repeat stages S102 and S103 as needed.

[0038] The fixed max voltage and the variable max voltage embodiments ensure displaying a growing marker as ultrasound transducer 31 is moved toward the imaging plane 11 at a given imaging depth. However, as known in the art, the received signal amplitude also depends on depth so that the variation of marker size as a function of out-of-plane distance is depth-dependent, and changes in sensor depth also will result in changes in marker size.

[0039] In order to mitigate or eliminate this effect, in a minimal movement embodiment, the current received signal amplitude is compared to a short history of signal amplitudes. The history length is a set parameter typically set to a few seconds of data, or a characteristic time for sensor advancement into the ultrasound field. The maximum marker size (a set parameter) is set to correspond to the maximum received signal or SNR during this history. As a further refinement, the history file is updated each time ultrasound transducer 31 is measured to move significantly (over a set distance threshold) as measured by its tracked position. This guarantees that the maximum set marker size will be displayed when ultrasound transducer 31 is in plane at any depth, provided that the characteristic time of cross-plane motion is faster than that of depth motion.

[0040] FIG. 8 illustrates a flowchart 110 representative of the minimal movement embodiment. Referring to FIG. 8, a stage S111 of flowchart 110 encompasses image navigator 80 acquiring parameters necessary for a calculation by image navigator 80 of 'markerSize_C' during a stage S113 of flowchart 110 as a function of a history of measured voltage V indicative of the received signal amplitude as related to movement of interventional tool 30. Specifically, an initial implementation of stage S111 involves setting 'maxV' to 0; markerSize to a 'defaultSize', and a history to zeros.

[0041] A stage S112 of flowchart 110 encompasses image navigator 80 determining whether interventional tool 30 has been moved beyond a threshold distance. If so, image navigator 80 proceeds to stage S113 to update the history with measured voltage V in accordance with the following equations:

$$\begin{aligned} \text{history}(1:N-1) &= \text{history}(2:N) \\ \text{history}(N) &= V \\ \text{maxV} &= \text{max}(\text{history}) \end{aligned}$$

$$\text{markerSize}_C = (V - \text{minV}) / (\text{maxV} - \text{minV}) * (\text{maxSize} - \text{minSize}) + \text{minSize}$$

[0042] A stage S113 of flowchart 110 encompasses image navigator 80 displaying a 'markerSize_D' in accordance with the following equations:

$$\begin{aligned} \text{markerSize}_D &= 0 \text{ if } \text{markerSize}_C < \text{minsize} \\ \text{markerSize}_D &= \text{maxSize} \text{ if } \text{markerSize}_C > \text{maxSize} \end{aligned}$$

[0043] Image navigator 80 returns to stage S112 to repeat stages S112- S114 as needed.

[0044] All the above embodiments may advantageously modified by taking into account the measured current spatial position, especially the depth, of interventional tool 30. Specifically, as known in the art, a field amplitude varies with depth and out-of-plane distance (and to a lesser extent with azimuth). The goal is to eliminate the variation in displayed marker size as a function of depth, but keep the variations on marker size as a function of out-of-plane distance at a given depth.

[0045] The following is a discussion on various possible schemes to incorporate depth (and azimuth) information in the display flowcharts of FIGS. 6-8 .

[0046] First for the fixed maximum voltage embodiment of FIG. 6, instead of a fixed maximum marker size (variable 'maxSize'), a look-up table of marker sizes as a function of depth (and possibly azimuth or azimuth angle as well) is established. This table is built based on some calibration of the spatial field which is achieved beforehand by simulation or/and measurement or on-the-fly by simulation. Different look-up tables may be used for different probes, imaging modes, settings (e.g. beam density) and transmit focal depth, for varying degrees of accuracy. The bulk attenuation within the anatomical region may be measured by fitting an exponential to the curve giving backscattered data amplitude as a function of depth (on the pulse-echo data), and added as an input to the simulation. Further, the maximum marker

size may be a function of interventional tool 30.

[0047] Second, in embodiments setting maxV as the maximum past read value in a history file, the current read voltage is compared only to those voltage readings in the history with a similar depth (e.g., no further than 1cm away from the current reading).

[0048] Third, a coarse spatial grid may be established and for each pixel in that grid, the maximum read value in the corresponding area is set as the local maximum read value maxV. These latter embodiments may be with the field simulation by constraining the simulation with actual readings.

[0049] In one implementation, a tool tracker (70) comprises hardware, software, firmware and/or circuitry for executing a tracking technique to track a position of an interventional tool (30) comprising at least one ultrasound transducer (31) disposed on a distal tip of the interventional tool (30) with an ultrasound probe (20), relative to an acoustic image plane (11) corresponding to an ultrasound image of an anatomical region generated by the ultrasound probe (20), based on a time of flight and an amplitude of ultrasound signals corresponding to each of a plurality of beams communicated from the ultrasound probe (20) to the at least one ultrasound transducer (31),

wherein the tool tracker (70) is configured to execute an algorithm that determines a projection of a 3D position of the at least one ultrasound transducer (31) including an X-azimuth, a Z-depth and a Y-elevation of the ultrasound transducer (31) relative to the ultrasound probe (20), onto a 2D position in the acoustic image plane (11) by performing the method steps of:

determining the Z-depth coordinate by measuring the time of flight of the ultrasound signals from the ultrasound probe (20) to the at least one ultrasound transducer (31);

determining the X-azimuth position by searching for a maximum received amplitude across beams from the ultrasound probe (20) received at the at least one ultrasound transducer (31);

estimating the Y elevation comprising the distance of the at least one ultrasound transducer (31) relative to the acoustic image plane (11) by recording the received amplitude of the ultrasound signals at the at least one ultrasound transducer (31) and comparing it to a past history of said ultrasound signals.

[0050] While various embodiments of the present invention have been illustrated and described, it will be understood by those skilled in the art that the embodiments of the present invention as described herein are illustrative, and various changes and modifications may be made and equivalents may be substituted for elements thereof without departing from the true scope of the present invention. In addition, many modifications may be made to adapt the teachings of the present invention without departing from its central scope. Therefore, it is intended that the present invention not be limited to the particular embodiments disclosed as the best mode contemplated for carrying out the present invention, but that the present invention includes all embodiments falling within the scope of the appended claims.

Claims

1. A tool navigation system, comprising:

an ultrasound probe (20) configured to generate an acoustic image plane for scanning an anatomical region; an ultrasound scanner (60) operatively connected to the ultrasound probe (20), the ultrasound scanner (60) being configured to generate an ultrasound image of the anatomical region;

an interventional tool (30) configured to be navigated within the anatomical region relative to the acoustic image plane; and wherein the interventional tool (30) has a distal tip;

at least one ultrasound transducer (31) connected to the interventional tool (30) to communicate at least one ultrasound tracking signal between the ultrasound probe (20) and the interventional tool (30) indicative of a distance of the interventional tool (30) relative to the acoustic image plane as the interventional tool (30) is navigated within the anatomical region; the at least one ultrasound transducer (31) being disposed on the distal tip of the interventional tool (30);

a tool tracker (70) operatively connected to the at least one ultrasound transducer (31) to track the distance of the interventional tool (30) relative to the acoustic image plane;

wherein the tool tracker (70) is configured to estimate the distance of the interventional tool (30) relative to the acoustic image plane as a function of an amplitude of the at least one ultrasound tracking signal; and

an image navigator (80) operatively connected to the ultrasound scanner (60) and the tool tracker (70) to display a graphical icon on the ultrasound image of the anatomical region as generated by the ultrasound scanner (60) for illustrating a tracking by the tool tracker (70) of the distance of the interventional tool (30) relative to the acoustic image plane,

wherein the image navigator (80) is configured to modulate at least one aspect of the graphical icon responsive

to the distance of the interventional tool (30) relative to the acoustic image plane as tracked by the tool tracker (70); wherein the at least one aspect of the graphical icon includes at least one of a size, a shape and a color of the graphical icon; and
 wherein the image navigator (80) is configured to monotonically modulate the at least one aspect of the graphical icon as a function of at least one of an amplitude and a signal-to-noise ratio of the at least one ultrasound tracking signal.

2. The tool navigation system of claim 1, wherein the tool tracker (70) is configured to measure a time of flight of the ultrasound tracking signals between the ultrasound probe (20) and the interventional tool (30).
3. The tool navigation system of claim 2, wherein the tool tracker (70) is further configured to determine a position of the at least one ultrasound transducer (31) within the anatomical region relative to the acoustic image plane as a function of the time of flight of the ultrasound tracking signals between the ultrasound probe (20) and the interventional tool (30).
4. The tool navigation system of claim 1, wherein the image navigator (80) is configured to monotonically modulate the at least one aspect of the graphical icon responsive to the distance of the interventional tool (30) relative to the acoustic image plane as tracked by the tool tracker (70).
5. The tool navigation system of claim 1, wherein the image navigator (80) is further configured to monotonically modulate the at least one aspect of the graphical icon between a fixed minimum amplitude and a fixed maximum amplitude of the at least one ultrasound tracking signal.
6. The tool navigation system of claim 1, wherein the image navigator (80) is further configured to monotonically modulate the at least one aspect of the graphical icon between a fixed minimum signal-to-noise ratio and a fixed maximum signal-to-noise ratio of the at least one ultrasound tracking signal.
7. The tool navigation system of claim 1, wherein the image navigator (80) is further configured to monotonically modulate the at least one aspect of the graphical icon between a fixed minimum signal-to-noise ratio and a variable maximum signal-to-noise ratio of the at least one ultrasound tracking signal.
8. The tool navigation system of claim 1, wherein the image navigator (80) is further configured to monotonically modulate the at least one aspect responsive to a minimal movement of the interventional tool (30) perpendicular to the acoustic image plane as tracked by the tool tracker (70).

Patentansprüche

1. Werkzeugnavigationssystem, umfassend:

eine Ultraschallsonde (20), die konfiguriert ist, eine akustische Bildebene für das Scannen einer anatomischen Region zu erzeugen;
 einen Ultraschall-Scanner (60), der mit der Ultraschallsonde (20) betriebsbereit verbunden ist, wobei der Ultraschall-Scanner (60) konfiguriert ist, ein Ultraschallbild der anatomischen Region zu erzeugen;
 ein interventionelles Werkzeug (30), das konfiguriert ist, innerhalb der anatomischen Region relativ zu der akustischen Bildebene navigiert zu werden; und wobei das interventionelle Werkzeug (30) eine distale Spitze aufweist;
 mindestens einen Ultraschallwandler (31) der mit dem interventionellen Werkzeug (30) verbunden ist, um mindestens ein Ultraschallabweichsignal zwischen der Ultraschallsonde (20) und dem interventionellen Werkzeug (30) zu kommunizieren, das für eine Entfernung des interventionellen Werkzeugs (30) relativ zu der akustischen Bildebene indikativ ist, wenn das interventionelle Werkzeug (30) innerhalb der anatomischen Region navigiert wird; wobei sich mindestens ein Ultraschallwandler (31) an der distalen Spitze des interventionellen Werkzeugs (30) befindet;
 einen Werkzeugverfolger (70), der mit dem mindestens einen Ultraschallwandler (31) betriebsbereit verbunden ist, um die Entfernung des interventionellen Werkzeugs(30) relativ zu der akustischen Bildebene zu verfolgen; wobei der Werkzeugverfolger (70) konfiguriert ist, die Entfernung des interventionellen Werkzeugs (30) relativ zu der akustischen Bildebene als Funktion einer Amplitude des mindestens einen Ultraschallabweichsignals zu schätzen; und

einen Bildnavigator (80), der mit dem Ultraschall-Scanner (60) und dem Werkzeugverfolger (70) betriebsbereit verbunden ist, um ein grafisches Symbol auf dem Ultraschallbild der anatomischen Region, wie von dem Ultraschall-Scanner (60) erzeugt, anzuzeigen, um ein Verfolgen der Entfernung des interventionellen Werkzeugs (30) relativ zu der akustischen Bildebene durch den Werkzeugverfolger (70) zu veranschaulichen, wobei der Bildnavigator (80) konfiguriert ist, mindestens einen Aspekt des grafischen Symbols als Reaktion auf die Entfernung des interventionellen Werkzeugs (30) relativ zu der akustischen Bildebene, wie von dem Werkzeugverfolger (70) verfolgt, zu modulieren; wobei der mindestens eine Aspekt des grafischen Symbols mindestens einen von einer Größe, einer Form und einer Farbe des grafischen Symbols einschließt; und wobei der Bildnavigator (80) konfiguriert ist, den mindestens einen Aspekt des grafischen Symbols als Funktion von mindestens einem von einer Amplitude und einem Signal-Rauschen-Verhältnis des mindestens einen Ultraschallabweichsignals monoton zu modulieren.

2. Werkzeugnavigationssystem nach Anspruch 1, wobei der Werkzeugverfolger (70) konfiguriert ist, eine Flugzeit der Ultraschallabweichsignale zwischen der Ultraschallsonde (20) und dem interventionellen Werkzeug (30) zu messen.
3. Werkzeugnavigationssystem nach Anspruch 2, wobei der Werkzeugverfolger (70) weiter konfiguriert ist, eine Position des mindestens einen Ultraschallwandlers (31) innerhalb der anatomischen Region relativ zu der akustischen Bildebene als Funktion der Flugzeit der Ultraschallabweichsignale zwischen der Ultraschallsonde (20) und dem interventionellen Werkzeug (30) zu bestimmen.
4. Werkzeugnavigationssystem nach Anspruch 1, wobei der Bildnavigator (80) konfiguriert ist, den mindestens einen Aspekt des grafischen Symbols als Reaktion auf die Entfernung des interventionellen Werkzeugs (30) relativ zu der akustischen Bildebene, wie von dem Werkzeugverfolger (70) verfolgt, monoton zu modulieren.
5. Werkzeugnavigationssystem nach Anspruch 1, wobei der Bildnavigator (80) weiter konfiguriert ist, den mindestens einen Aspekt des grafischen Symbols zwischen einer festen minimalen Amplitude und einer festen maximalen Amplitude des mindestens einen Ultraschallabweichsignals monoton zu modulieren.
6. Werkzeugnavigationssystem nach Anspruch 1, wobei der Bildnavigator (80) weiter konfiguriert ist, den mindestens einen Aspekt des grafischen Symbols zwischen einem festen minimalen Signal-Rauschen-Verhältnis und einem festen maximalen Signal-Rauschen-Verhältnis des mindestens einen Ultraschallabweichsignals monoton zu modulieren.
7. Werkzeugnavigationssystem nach Anspruch 1, wobei der Bildnavigator (80) weiter konfiguriert ist, den mindestens einen Aspekt des grafischen Symbols zwischen einem festen minimalen Signal-Rauschen-Verhältnis und einem variablen maximalen Signal-Rauschen-Verhältnis des mindestens einen Ultraschallabweichsignals monoton zu modulieren.
8. Werkzeugnavigationssystem nach Anspruch 1, wobei der Bildnavigator (80) weiter konfiguriert ist, den mindestens einen Aspekt als Reaktion auf eine minimale Bewegung des interventionellen Werkzeugs (30) senkrecht zu der akustischen Bildebene, wie durch den Werkzeugverfolger (70) verfolgt, monoton zu modulieren.

Revendications

1. Système de navigation d'outil, comprenant :

une sonde ultrasonore (20) configurée pour générer un plan image acoustique pour balayer une région anatomique ;
 un ultrasonographe (60) connecté fonctionnellement à la sonde ultrasonore (20), l'ultrasonographe (60) étant configuré pour générer une image ultrasonore de la région anatomique ;
 un outil interventionnel (30) configuré pour faire l'objet d'une navigation au sein de la région anatomique par rapport au plan image acoustique ; et dans lequel l'outil interventionnel (30) a un embout distal ;
 au moins un transducteur ultrasonore (31) connecté à l'outil interventionnel (30) pour communiquer au moins un signal de suivi ultrasonore entre la sonde ultrasonore (20) et l'outil interventionnel (30) indicatif d'une distance de l'outil interventionnel (30) par rapport au plan image acoustique lorsque l'outil interventionnel (30) fait l'objet d'une navigation au sein de la région anatomique ; le au moins un transducteur ultrasonore (31) étant disposé

sur le bout distal de l'outil interventionnel (30) ;
un organe suiveur d'outil (70) connecté fonctionnellement à l'au moins un transducteur ultrasonore (31) pour
suivre la distance de l'outil interventionnel (30) par rapport au plan image acoustique ;
dans lequel l'organe suiveur d'outil (70) est configuré pour estimer la distance de l'outil interventionnel (30) par
rapport au plan image acoustique en fonction d'une amplitude de l'au moins un signal de suivi ultrasonore ; et
un navigateur d'image (80) connecté fonctionnellement à l'ultrasonographe (60) et à l'organe suiveur d'outil
(70) pour afficher une icône graphique sur l'image ultrasonore de la région anatomique telle que générée par
l'ultrasonographe (60) pour illustrer un suivi par l'organe suiveur d'outil (70) de la distance de l'outil interventionnel
(30) par rapport au plan image acoustique,
dans lequel le navigateur d'image (80) est configuré pour moduler au moins un aspect de l'icône graphique en
réaction à la distance de l'outil interventionnel (30) par rapport au plan image acoustique tel que suivi par
l'organe suiveur d'outil (70) ;
dans lequel le au moins un aspect de l'icône graphique inclut au moins l'une parmi une taille, une forme et une
couleur de l'icône graphique ; et
dans lequel le navigateur d'image (80) est configuré pour moduler de façon monotone le au moins un aspect
de l'icône graphique comme une fonction d'au moins l'un(e) d'une amplitude et d'un rapport signal sur bruit de
l'au moins un signal de suivi ultrasonore.

2. Système de navigation d'outil selon la revendication 1, dans lequel l'organe suiveur d'outil (70) est configuré pour mesurer un temps de vol des signaux de suivi ultrasonores entre la sonde ultrasonore (20) et l'outil interventionnel (30).
3. Système de navigation d'outil selon la revendication 2, dans lequel l'organe suiveur d'outil (70) est en outre configuré pour déterminer une position de l'au moins un transducteur ultrasonore (31) au sein de la région anatomique par rapport au plan image acoustique comme une fonction du temps de vol des signaux de suivi ultrasonores entre la sonde ultrasonore (20) et l'outil interventionnel (30).
4. Système de navigation d'outil selon la revendication 1, dans lequel le navigateur d'image (80) est configuré pour moduler de façon monotone l'au moins un aspect de l'icône graphique en réaction à la distance de l'outil interventionnel (30) par rapport au plan image acoustique tel que suivi par l'organe suiveur d'outil (70).
5. Système de navigation d'outil selon la revendication 1, dans lequel le navigateur d'image (80) est en outre configuré pour moduler de façon monotone l'au moins un aspect de l'icône graphique entre une amplitude minimale fixe et une amplitude maximale fixe de l'au moins un signal de suivi ultrasonore.
6. Système de navigation d'outil selon la revendication 1, dans lequel le navigateur d'image (80) est en outre configuré pour moduler de façon monotone l'au moins un aspect de l'icône graphique entre un rapport signal sur bruit minimal fixe et un rapport signal sur bruit maximal fixe de l'au moins un signal de suivi ultrasonore.
7. Système de navigation d'outil selon la revendication 1, dans lequel le navigateur d'image (80) est en outre configuré pour moduler de façon monotone l'au moins un aspect de l'icône graphique entre un rapport signal sur bruit minimal fixe et un rapport signal sur bruit maximal variable de l'au moins un signal de suivi ultrasonore.
8. Système de navigation d'outil selon la revendication 1, dans lequel le navigateur d'image (80) est en outre configuré pour moduler de façon monotone l'au moins un aspect en réponse à un mouvement minimal de l'outil interventionnel (30) perpendiculaire au plan image acoustique tel que suivi par l'organe suiveur d'outil (70).

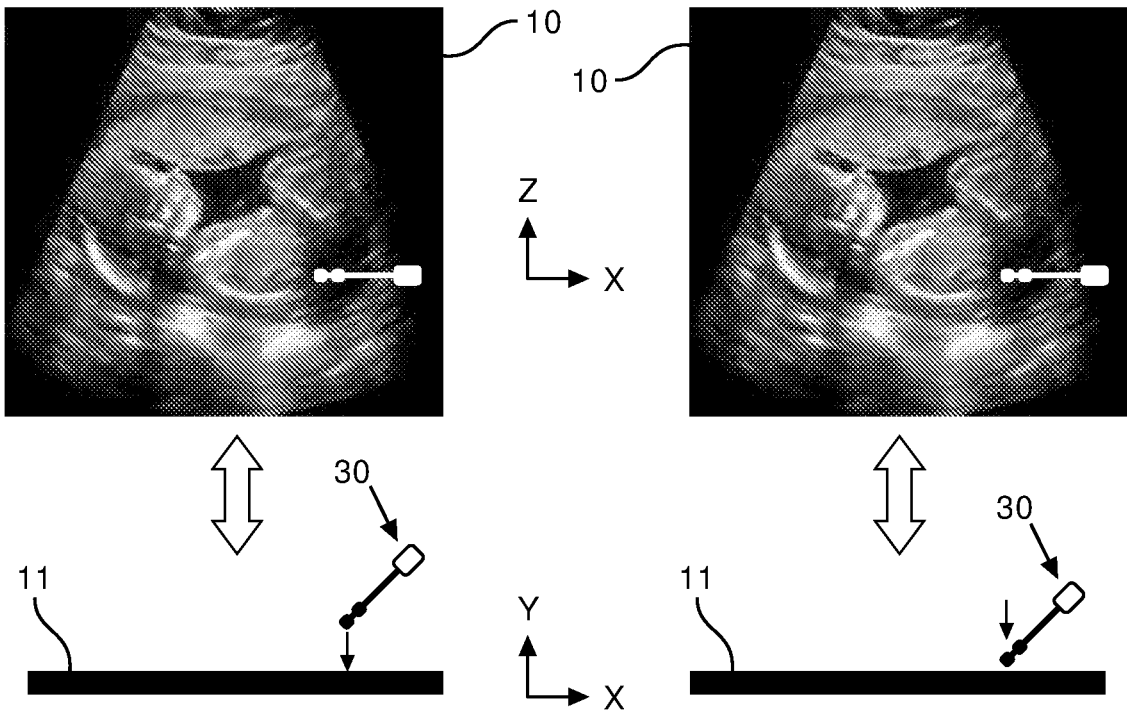


FIG. 1A
(Prior art)

FIG. 1B
(Prior art)

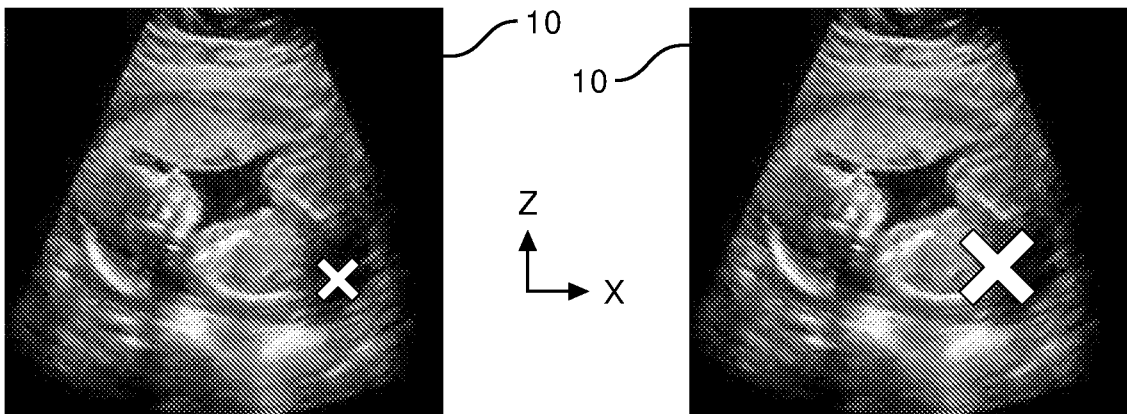


FIG. 2A

FIG. 2B

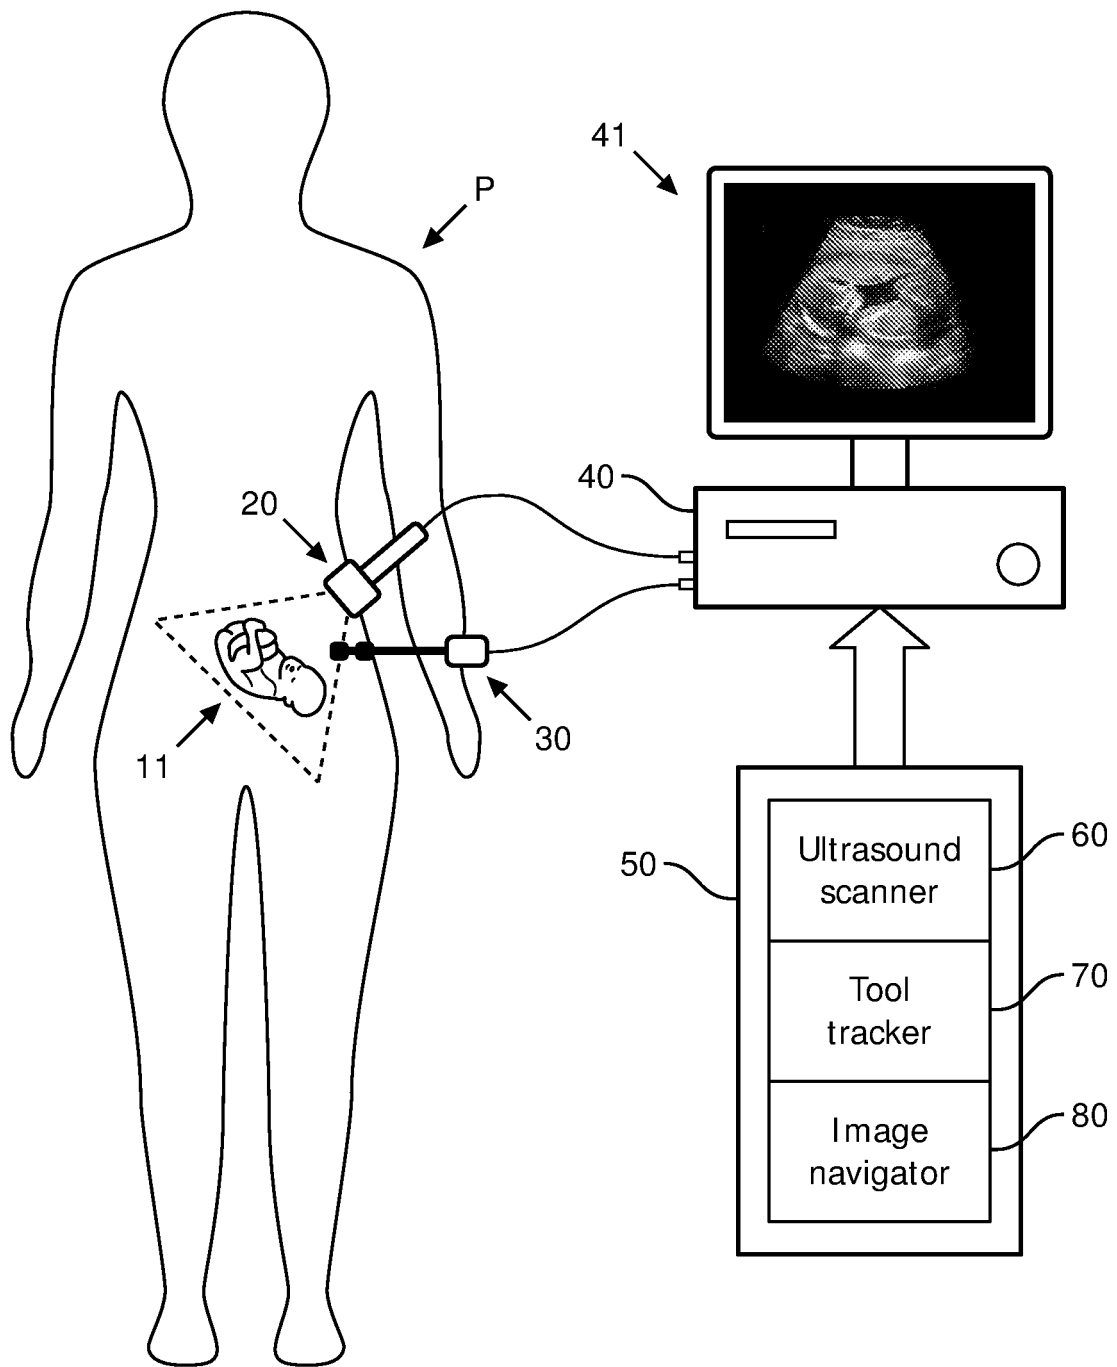


FIG. 3

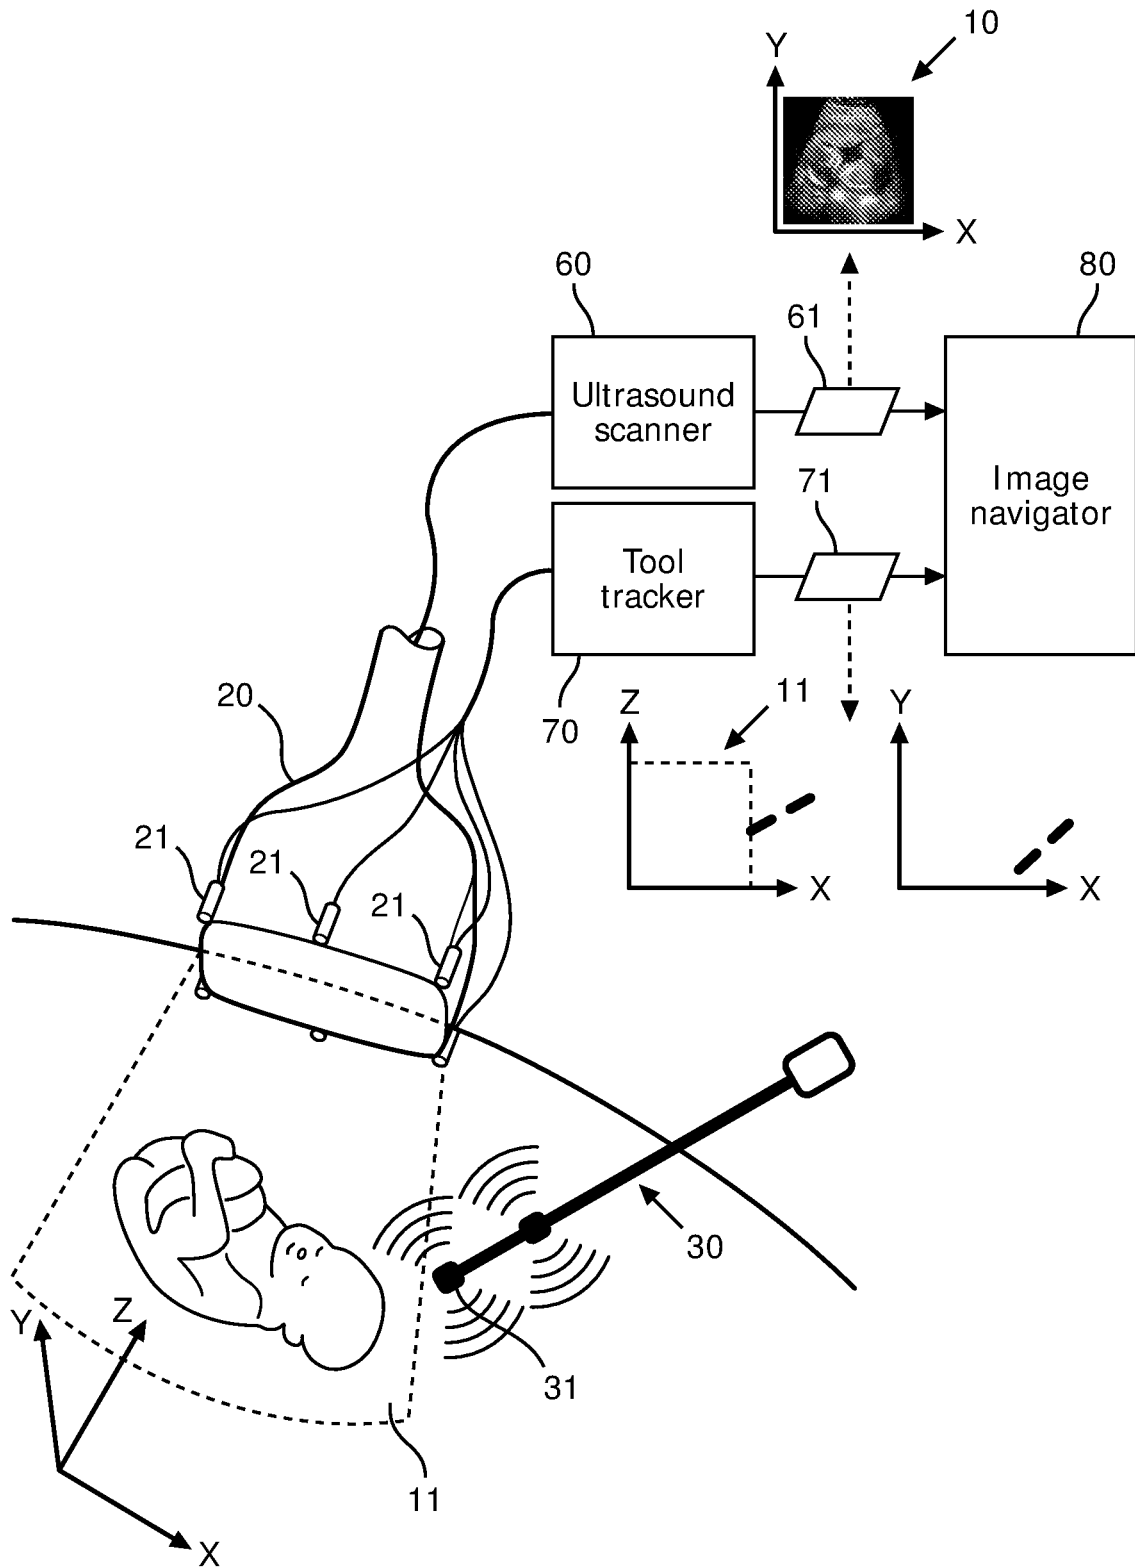


FIG. 4

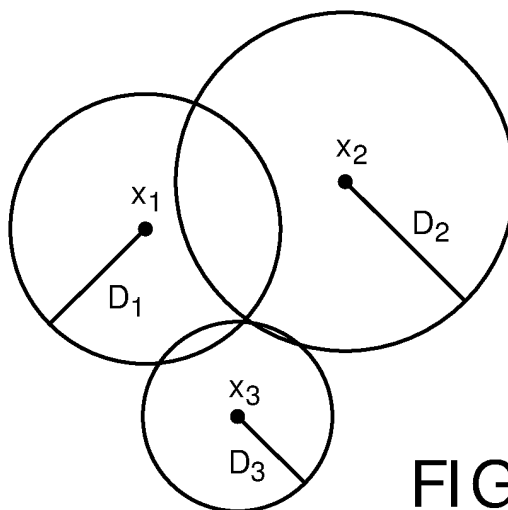


FIG. 5

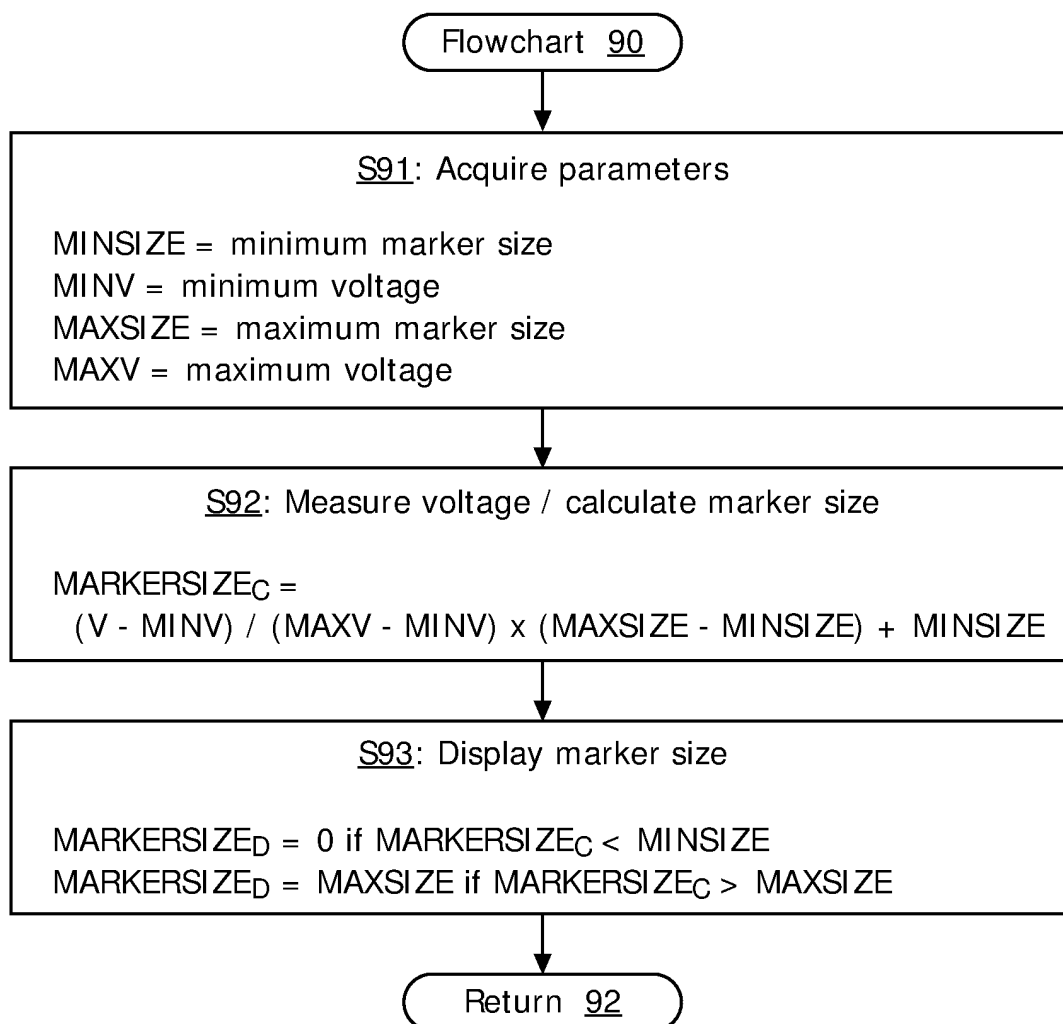


FIG. 6

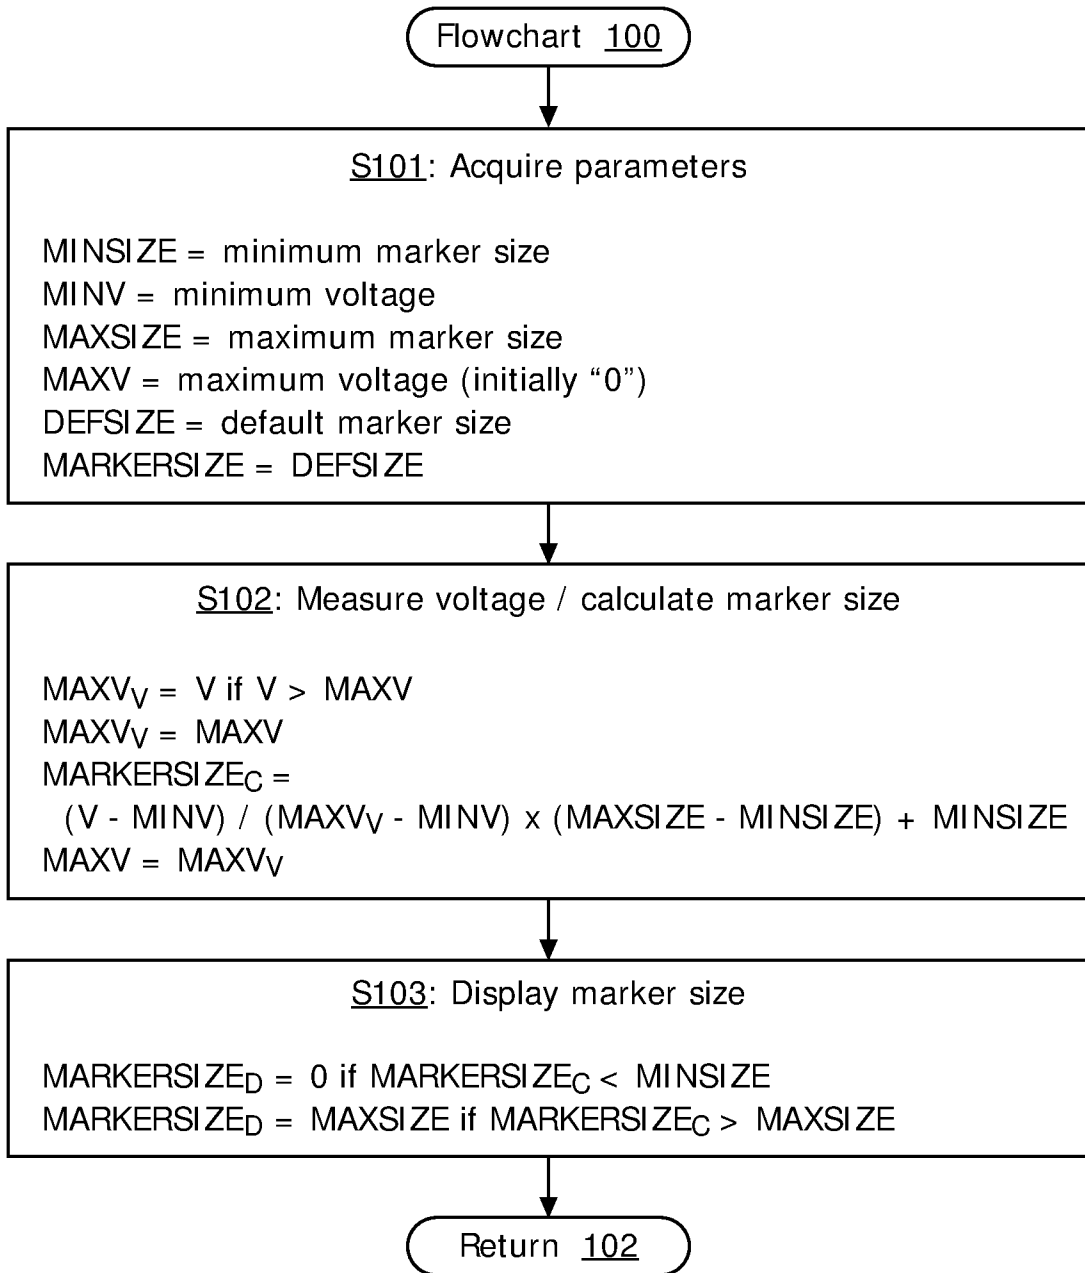


FIG. 7

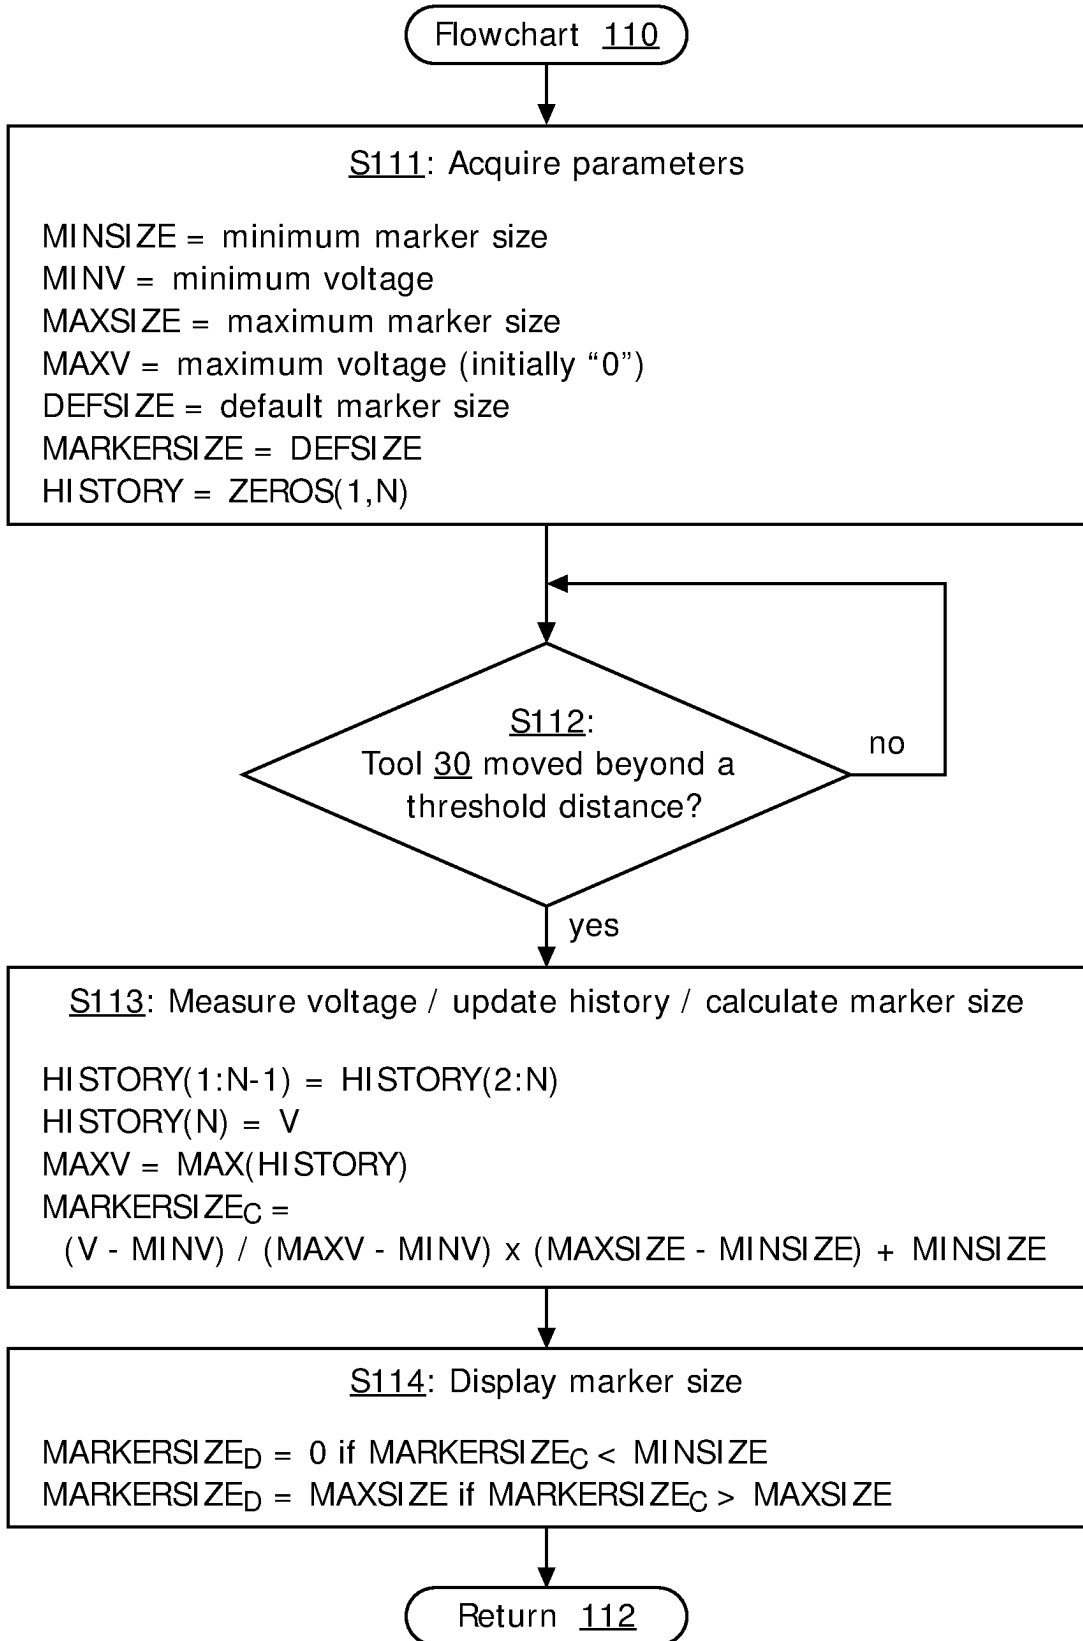


FIG. 8

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20110245659 A1 [0006]
- US 20130041252 A1 [0007]
- US 20130211243 A1 [0008]
- US 20100298704 A1 [0009]

专利名称(译)	仪器对准和超声成像平面跟踪		
公开(公告)号	EP3089671B1	公开(公告)日	2019-05-22
申请号	EP2015704590	申请日	2015-01-02
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	VIGNON FRANCOIS GUY GERARD MARIE JAIN AMEET KUMAR		
发明人	VIGNON, FRANCOIS GUY GERARD MARIE JAIN, AMEET KUMAR		
IPC分类号	A61B8/12 A61B34/20 A61B8/08 A61B8/00 A61B17/34 A61B90/00		
代理机构(译)	飞利浦知识产权及标准		
优先权	61/922882 2014-01-02 US		
其他公开文献	EP3089671A1		
外部链接	Espacenet		

摘要(译)

一种工具导航系统，其采用超声探头（20），超声扫描仪（60），介入工具（30）（例如，针或导管），多个超声换能器（21,31），工具跟踪器（70）和图像导航器。在操作中，超声探头（20）生成用于扫描解剖区域的声学图像平面，并且超声扫描仪（60）从解剖区域的扫描生成解剖区域的超声图像。在扫描期间，介入工具（30）在解剖区域内相对于声像平面导航，并且超声换能器（21,31）通过工具跟踪器（70）促进介入工具的位置的轨迹（30）相对于声像平面。图像导航器在由超声扫描仪（60）生成的解剖区域的超声图像内显示图形图标，用于示出工具跟踪器（70）跟踪介入工具（30）相对于声像的距离。平面。当介入工具（30）在解剖区域内导航时，响应于介入工具（30）相对于声像平面的跟踪距离，图像导航器调制图形图标的一个或多个方面。

