

(19)



(11)

EP 2 808 865 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
26.04.2017 Bulletin 2017/17

(51) Int Cl.:
G10K 11/30 (2006.01) A61B 8/00 (2006.01)

(21) Application number: **14151364.8**

(22) Date of filing: **16.01.2014**

(54) **Ultrasound probe and manufacturing method thereof**

Ultraschallsonde und Herstellungsverfahren dafür

Sonde à ultrasons et son procédé de fabrication

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **30.05.2013 KR 20130061410**

(43) Date of publication of application:
03.12.2014 Bulletin 2014/49

(73) Proprietor: **Samsung Medison Co., Ltd.
Gangwon-do 250-870 (KR)**

(72) Inventor: **Yoo, Beom Keun
Incheon (KR)**

(74) Representative: **Schmid, Wolfgang
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft mbB
Alte Ulmer Strasse 2
89522 Heidenheim (DE)**

(56) References cited:
**EP-A1- 1 816 492 EP-A1- 2 405 671
WO-A1-2008/084455 WO-A2-2007/125500**

EP 2 808 865 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND

1. Field

[0001] Embodiments of the present invention relate to an ultrasound probe which generates images of the inside of an object using ultrasonic waves and a manufacturing method thereof.

2. Description of the Related Art

[0002] In general, an ultrasound diagnostic apparatus radiates an ultrasound signal to a target region of the inside of an object from the surface of the object, and non-invasively acquires tomographic images or images regarding a blood current of soft tissues using information of ultrasound signals (ultrasound echo signals) reflected by the target region.

[0003] As compared to other image diagnostic apparatuses, such as an X-ray diagnostic apparatus, a computed tomography (CT) scanner, a magnetic resonance imaging (MRI) apparatus, and a nuclear medicine diagnostic apparatus, the ultrasonic diagnostic apparatus is small and inexpensive, displays images in real time, and has high safety without X-ray exposure. Due to these advantages, the ultrasonic diagnostic apparatus is used for diagnosis of the heart, the abdomen, the renal system, and in obstetrics and gynecology.

[0004] The ultrasound diagnostic apparatus includes an ultrasound probe transmitting an ultrasound signal to an object and receiving ultrasound echo signals reflected by the object so as to acquire ultrasound images of the object.

[0005] The ultrasound probe includes a transducer in which a piezoelectric material vibrates and converts electrical signals and acoustic signals into each other, a matching layer reducing an acoustic impedance difference between the transducer and the object so as to maximally transmit ultrasonic waves generated from the transducer to the object, an acoustic lens focusing ultrasonic waves progressing in the forward direction of the transducer at a specific point, and a sound-absorbing layer blocking ultrasonic waves progressing in the backward direction of the transducer to prevent image distortion.

[0006] The EP 2 405 671 A1 discloses an ultrasonic transducer, an ultrasonic probe, and an ultrasonic diagnostic device which enable an ultrasonic beam in the depth direction of diagnosis to be narrowly focused in a wide region, thereby obtaining a high-resolution diagnostic image. An ultrasonic transducer is provided with an ultrasonic vibrator, a shape change layer which is provided on the subject side of the ultrasonic vibrator and the shape of which is changed by an electrical signal, electrodes which are respectively disposed on both surfaces of the shape change layer, and a variable power

source which applies the electrical signal between the electrodes, wherein the variable power source varies the focus or diffusion of the ultrasonic beam by changing the shape of the shape change layer; by controlling the electrical signal to be applied between the electrodes.

[0007] The EP 1 816 492 A1 discloses an optical device comprising: a liquid container that contains water-based liquid and oil-based liquid that are different in refractive index from each other and immiscible with each other to have respective optical-transmission properties so that light can transmit in a predetermined optical-axis direction; a coat film that covers at least part of an inner surface of the liquid container and has a hydrophilic/hydrophobic property changing with temperature; and a temperature regulator that regulates temperature of the coat film.

[0008] In the WO 2007/125500 A2 an acoustic probe includes an acoustic transducer including a plurality of acoustic transducer elements arranged in a one-dimensional array; and a variably-refracting acoustic lens coupled to the acoustic transducer. The variably-refracting acoustic lens has at least a pair of electrodes adapted to adjust the focus of the variably-refracting acoustic lens in response to a selected voltage applied across the electrodes. In one embodiment, the variably-refracting acoustic lens includes a cavity, first and second fluid media disposed within the cavity, and the pair of electrodes. The speed of sound of an acoustic wave in the first fluid medium is different than the speed of sound of the acoustic wave in the second fluid medium. The first and second fluid media are immiscible with respect to each other, and the first fluid medium has a substantially different electrical conductivity than the second fluid medium.

SUMMARY

[0009] Therefore, it is an aspect of the present invention to provide an ultrasound probe which may adjust curvature of an acoustic lens using a shape memory alloy and a manufacturing method thereof.

[0010] Additional aspects of the invention will be set forth in part in the description which follows and, in part, will be obvious from the description, or may be learned by practice of the invention.

[0011] In accordance with one aspect of the present invention, an ultrasonic probe includes an acoustic lens, a focus adjusting unit installed on the acoustic lens and deforming the shape of the acoustic lens to adjust the focus of ultrasonic waves radiated through the acoustic lens, and a current applying unit applying current to the focus adjusting unit to contract or expand the focus adjusting unit.

[0012] The focus adjusting unit may include at least one wire formed of a shape memory alloy that is deformed according to supply of current.

[0013] The at least one wire may be attached to or inserted into the acoustic lens in the azimuthal direction.

[0014] The at least one wire may be attached to or inserted into the acoustic lens along the boundary of the

acoustic lens.

[0015] The current applying unit may apply current to the at least one wire to contract or expand the at least one wire.

[0016] The focus adjusting unit may deform the shape of the acoustic lens to change curvature of the acoustic lens.

[0017] When current is applied to the focus adjusting unit from the current applying unit, the focus adjusting unit may contract and increase curvature of the acoustic lens.

[0018] The ultrasound probe may further include a current adjusting unit allowing a user to adjust current applied to the focus adjusting unit through the current applying unit.

[0019] In accordance with another aspect of the present invention, a manufacturing method of an ultrasound probe includes installing a focus adjusting unit, deforming the shape of an acoustic lens to adjust the focus of ultrasonic waves radiated through the acoustic lens, on the acoustic lens, installing a current applying unit applying current to the focus adjusting unit to contract or expand the focus adjusting unit, and installing the acoustic lens provided with the focus adjusting unit on the front surface of a matching layer.

[0020] The focus adjusting unit may include at least one wire formed of a shape memory alloy that is deformed according to supply of current.

[0021] The installation of the focus adjusting unit may include attaching or inserting the at least one wire to or into the acoustic lens in the azimuthal direction.

[0022] The installation of the focus adjusting unit may include attaching or inserting the at least one wire to or into the acoustic lens along the boundary of the acoustic lens.

[0023] In accordance with yet another aspect of the present invention, a control method of an ultrasound probe according to claim 1 includes receiving a signal output from a current adjusting unit of the ultrasound probe corresponding to user operation, outputting a current applying signal corresponding to the signal output from the current adjusting unit to the current applying unit of the ultrasound probe, and causing the current applying unit to apply current to the focus adjusting unit of the ultrasound probe according to the current applying signal.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] These and/or other aspects of the invention will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings of which:

FIG. 1 is a view illustrating the structure of an ultrasound probe in accordance with one embodiment of the present invention;

FIGS. 2(a) to 2(c) are views illustrating various ex-

amples of a focus adjusting unit installed on an acoustic lens in accordance with the embodiment of the present invention;

FIG. 3 is a block diagram illustrating a configuration to control curvature of the acoustic lens in accordance with the embodiment of the present invention; FIGS. 4(a) to 4(c) are views illustrating various examples of a current adjusting unit of the ultrasound probe in accordance with the embodiment of the present invention; and

FIG. 5 is a flowchart illustrating a manufacturing method of an ultrasound probe in accordance with one embodiment of the present invention.

15 DETAILED DESCRIPTION

[0025] Reference will now be made in detail to the embodiments of the present invention, examples of which are illustrated in the accompanying drawings, wherein like reference numerals refer to like elements throughout.

[0026] FIG. 1 is a view illustrating the structure of an ultrasound probe in accordance with one embodiment of the present invention.

[0027] With reference to FIG. 1, the ultrasound probe in accordance with this embodiment includes a sound-absorbing layer 10, a transducer 20 installed on the front surface of the sound-absorbing layer 10, a matching layer 30 installed on the front surface of the transducer 20, and an acoustic lens 40 installed on the front surface of the matching layer 30.

[0028] For example, as the transducer 20, a magnetostrictive ultrasound transducer using the magnetostrictive effect of a magnetic material, a capacitive micromachined ultrasound transducer transmitting and receiving ultrasonic waves using vibration of hundreds or thousands of micromachined films, or a piezoelectric ultrasound transducer using the piezoelectric effect of a piezoelectric material may be used. Hereinafter, a piezoelectric ultrasound transducer used as the transducer 20 will be exemplarily described.

[0029] When mechanical pressure is applied to a designated material, voltage is generated, and when voltage is applied, mechanical deformation of the material occurs. Such an effect is referred to as the piezoelectric effect or the inverse piezoelectric effect, and a material having such an effect is referred to as a piezoelectric material.

[0030] That is, a piezoelectric material is a material converting electrical energy into mechanical vibration energy or converting mechanical vibration energy into electrical energy.

[0031] The ultrasound probe in accordance with this embodiment of the present invention includes the transducer 20 formed of a piezoelectric material that, when an electrical signal is applied to the transducer 20, converts the electrical signal into mechanical vibration and thus generates ultrasonic waves.

[0032] The piezoelectric material of the transducer 20

may include ceramic of lead zirconate titanate (PZT), a PZMT single crystal formed of a solid solution of lead magnesium niobate and lead titanate, a PZNT single crystal formed of a solid solution of lead zinc niobate and lead titanate, PMN-PT, or a single crystal basically doped with PMN-PT.

[0033] Further, the transducer 20 may be arranged in a single layered structure or a multi-layered stack structure.

[0034] In general, the transducer 20 of a stack structure may more easily adjust impedance and voltage and thus acquire high sensitivity, high energy conversion efficiency, and a soft spectrum.

[0035] Further, electrodes to which electrical signals may be applied may be formed on the front and rear surfaces of the transducer 20. If electrodes are formed on the front and rear surfaces of the transducer 20, one of the electrodes formed on the front and rear surfaces of the transducer 20 may be a ground electrode and the other may be a signal electrode.

[0036] The matching layer 30 may be installed on the front surface of the transducer 20. The matching layer 20 reduces an acoustic impedance difference between the transducer 30 and an object and thus matches the acoustic impedances of the transducer 30 and the object, thereby effectively transmitting ultrasonic waves generated from the transducer 20 to the object.

[0037] For this purpose, the matching layer 30 may be provided so as to have a median value between the acoustic impedance of the transducer 20 and the acoustic impedance of the object.

[0038] The matching layer 30 may be formed of carbon, glass, or a resin.

[0039] Further, the matching layer 30 may include a plurality of matching layers 30 so that acoustic impedance may be changed in stages from the transducer 20 to the object, and the plural matching layers 30 may be formed of different materials.

[0040] The transducer 20 and the matching layer 30 may be processed to a matrix-type 2D array through a dicing process, or be processed to a 1 D array.

[0041] Although shown in the drawings, a protective layer may be installed on the front surface of the matching layer 30, and the acoustic lens 40 may be installed on the front surface of the protective layer. The protective layer may include an RF shield to prevent a high frequency component which may be generated from the transducer 20 from leaking to the outside and to block introduction of high frequency signals from the outside. Further, the protective layer may include a chemical shield formed by coating or depositing a conductive material on the surface of a moisture and chemical resistant film to protect inner part from water or chemicals used for disinfection.

[0042] In order to focus ultrasonic waves, the acoustic lens 40 may be formed in a convex shape in the radiation direction of the ultrasonic waves, or be formed in a concave shape if sound velocity is lower than in a human

body. The acoustic lens 40 in accordance with this embodiment may be formed of an elastic material which is changeable in shape, scarcely cause fatigue due to deformation, and returns to its original shape prior to deformation.

[0043] The acoustic lens 40 of the ultrasound probe in accordance with this embodiment of the present invention includes a focus adjusting unit 43 changing the shape of the acoustic lens 40 to change the focus of ultrasonic waves radiated through the acoustic lens 40. FIGS. 2(a) to 2(c) are views illustrating various examples of the focus adjusting unit 43 installed on the acoustic lens 40 in accordance with the embodiment of the present invention.

[0044] As exemplarily shown in FIGS. 2(a) to 2(c), the focus adjusting unit 43 may be attached to or inserted into the boundary of the acoustic lens 40. The focus adjusting unit 43 shown in FIGS. 2(a) or 2(b) may be installed on the acoustic lens 40 having the same shape as the acoustic lens 40 exemplarily shown in FIG. 1. That is, the focus adjusting unit 43 may be installed along the boundary of the acoustic lens 40.

[0045] If the acoustic lens 40 has the shape shown in FIG. 2(c), the focus adjusting unit 43 may be installed at the boundary of the acoustic lens 40 in the azimuthal direction.

[0046] Further, the focus adjusting unit 43 may be formed in the type of a wire, a coil, or a frame formed of a shape memory alloy. For example, as exemplarily shown in FIGS. 2(a) to 2(c), the focus adjusting unit 43 may be formed as a wire which may be easily processed.

[0047] Since the focus adjusting unit 43 is formed of a shape memory alloy, when current is applied to the focus adjusting unit 43, the focus adjusting unit 43 contracts. Since the focus adjusting unit 43 is installed on the acoustic lens 40, when the focus adjusting unit 43 contracts, the convex portion of the lens 40 contracts and curvature of the acoustic lens 40 is increased, and when curvature of the acoustic lens 40 is increased, a focusing distance of the ultrasound probe with respect to ultrasonic waves is shortened.

[0048] When the curvature of the acoustic lens 40 is changed, as describe above, a space may be formed between the acoustic lens 40 and the matching layer 30 or an existing space may be expanded. In the ultrasound probe in accordance with the embodiment of the present invention, the space between the acoustic lens 40 and the matching layer 30 varying according to change of the curvature of the acoustic lens 40 may be filled with a liquid. By filling the vacant space with a liquid, radiation of ultrasonic waves may be more effectively carried out.

[0049] Change of the curvature of the acoustic lens 40 may be adjusted by adjusting the intensity of current applied to the focus adjusting unit 43, and therethrough, the focusing distance of the ultrasound probe with respect to ultrasonic waves may be adjusted.

[0050] By changing the curvature of the acoustic lens 40 using the focus adjusting unit 43 formed of a shape memory alloy, as described above, the focusing distance

may be variously changed using only one ultrasound probe without replacement of the ultrasonic probe.

[0051] FIG. 3 is a block diagram illustrating a configuration to control curvature of the acoustic lens 40, and FIGS. 4(a) to 4(c) are views illustrating various examples of a current adjusting unit 41 of FIG. 3.

[0052] The ultrasound probe in accordance with the embodiment of the present invention further includes a current applying unit 42 applying current to the above-described focus adjusting unit 43, and a current adjusting unit 41 allowing a user to apply current to the focus adjusting unit 43 to adjust the focusing distance of the ultrasound probe.

[0053] The current adjusting unit 41 is provided on the ultrasound probe so that the user may adjust the focusing distance of the ultrasound probe with respect to ultrasonic waves radiated through the acoustic lens 40.

[0054] A button-type current adjusting unit 41 may be provided on the outer surface of the ultrasound probe, as exemplarily shown in FIG. 4(a), or a dial-type toggle switch serving as the current adjusting unit 41 may be provided on a panel of a rear end apparatus to control the overall operation of the ultrasonic probe, as exemplarily shown in FIG. 4(b). Otherwise, a pedal-type current adjusting unit 41 may be provided, as exemplarily shown in FIG. 4(c). The current adjusting units 41 exemplarily shown in FIGS. 4(a) to 4(c) are just examples, and the embodiments of the present invention are not limited thereto. When a user operates the current adjusting unit 41, the focusing distance of the ultrasound probe which varies according to user operation may be displayed through a display of a rear end apparatus.

[0055] In order to change the focusing distance as desired by the user, the user may operate one of the current adjusting units 41, as exemplarily shown in FIGS. 4(a) to 4(c). When the user operates the current adjusting unit 41, the current adjusting unit 41 generates a current applying signal corresponding to user operation and outputs the current applying signal to the current applying unit 42.

[0056] The current applying unit 42 receives the current applying signal output from the current adjusting unit 41 and applies current corresponding to the current applying signal to the focus adjusting unit 43. The current applying unit 42 may include a power source generating electricity corresponding to the current applying signal applied from the current adjusting unit 41.

[0057] When current is supplied from the current applying unit 42 to the focus adjusting unit 43 formed of a shape memory alloy, the shape of the focus adjusting unit 43 is changed and thus the curvature of the acoustic lens 40 is changed. When current is applied from the current applying unit 42 to the focus adjusting unit 43 and thus the focus adjusting unit 43 contracts, the curvature of the acoustic lens 40 is increased and the focusing distance of the ultrasound probe with respect to ultrasonic waves is shortened.

[0058] FIG. 5 is a flowchart illustrating a manufacturing method of an ultrasound probe in accordance with one

embodiment of the present invention.

[0059] With reference to FIG. 5, the focus adjusting unit 43 is installed on the acoustic lens 40 (Operation 500).

5 **[0060]** The acoustic lens 40 of the ultrasound probe in accordance with the embodiment of the present invention includes the focus adjusting unit 43 changing the shape of the acoustic lens 40 to change the focus of ultrasonic waves radiated through the acoustic lens 40. FIGS. 2(a) to 2(c) illustrate various examples of the focus adjusting unit 43 installed on the acoustic lens 40 in accordance with the embodiment of the present invention.

10 **[0061]** As exemplarily shown in FIGS. 2(a) to 2(c), the focus adjusting unit 43 may be attached to or inserted into the boundary of the acoustic lens 40. The focus adjusting unit 43 shown in FIGS. 2(a) or 2(b) may be installed on the acoustic lens 40 having the same shape as the shape exemplarily shown in FIG. 1. That is, the focus adjusting unit 43 may be installed along the boundary of the acoustic lens 40. If the acoustic lens 40 has the shape shown in FIG. 2(c), the focus adjusting unit 43 may be installed at the boundary of the acoustic lens 40 in the azimuthal direction.

15 **[0062]** Further, the focus adjusting unit 43 may be formed in the type of a wire, a coil, or a frame formed of a shape memory alloy. For example, as exemplarily shown in FIGS. 2(a) to 2(c), the focus adjusting unit 43 may be formed as a wire which may be easily processed.

20 **[0063]** Since the focus adjusting unit 43 is formed of a shape memory alloy, when current is applied to the focus adjusting unit 43, the focus adjusting unit 43 contracts. Since the focus adjusting unit 43 is installed on the acoustic lens 40, when the focus adjusting unit 43 contracts, the convex portion of the lens 40 contracts and curvature of the acoustic lens 40 is increased, and when curvature of the acoustic lens 40 is increased, a focusing distance of the ultrasound probe with respect to ultrasonic waves is shortened.

25 **[0064]** Change of the curvature of the acoustic lens 40 may be adjusted by adjusting the intensity of current applied to the focus adjusting unit 43, and therethrough, the focusing distance of the ultrasound probe with respect to ultrasonic waves may be adjusted.

30 **[0065]** When the focus adjusting unit 43 is installed on the acoustic lens 40, the acoustic lens 40 provided with the focus adjusting unit 43 is installed on the front surface of the matching layer 30 (Operation 510).

35 **[0066]** The matching layer 30 may be installed on the front surface of the transducer 20, and the acoustic lens 40 provided with the focus adjusting unit 43 may be installed on the front surface of the matching layer 30. Otherwise, the protective layer may be installed on the front surface of the matching layer 30, and the acoustic lens 40 may be installed on the front surface of the protective layer.

40 **[0067]** As is apparent from the above description, in an ultrasound probe and a manufacturing method thereof in accordance with one embodiment of the present in-

vention, curvature of an acoustic lens may be adjusted.

[0068] Further, the focusing distance of the ultrasound probe may be changed by adjusting the curvature of the acoustic lens and, thus, accurate information of an object may be confirmed using only one ultrasonic probe.

[0069] Although a few embodiments of the present invention have been shown and described, it would be appreciated by those skilled in the art that changes may be made in these embodiments without departing from the invention, the scope of which is defined in the claims and their equivalents.

Claims

1. An ultrasound probe comprising:

an acoustic lens (40);
a focus adjusting unit (43) installed on the acoustic lens (40) and deforming the shape of the acoustic lens (40) to adjust the focus of ultrasonic waves radiated through the acoustic lens (40); and
a current applying unit (42) applying current to the focus adjusting unit (43) to contract or expand the focus adjusting unit (43).

2. The ultrasound probe according to claim 1, wherein the focus adjusting unit (43) includes at least one wire formed of a shape memory alloy that is deformed according to supply of current.

3. The ultrasound probe according to claim 2, wherein the at least one wire is attached to or inserted into the acoustic lens (40) in the azimuthal direction.

4. The ultrasound probe according to claim 2, wherein the at least one wire is attached to or inserted into the acoustic lens (40) along the boundary of the acoustic lens (40).

5. The ultrasound probe according to claim 2, wherein the current applying unit (42) applies current to the at least one wire to contract or expand the at least one wire.

6. The ultrasound probe according to claim 1, wherein the focus adjusting unit (43) deforms the shape of the acoustic lens (40) to change curvature of the acoustic lens (40).

7. The ultrasound probe according to claim 1, wherein, when current is applied to the focus adjusting unit (43) from the current applying unit (42), the focus adjusting unit (43) contracts and increases curvature of the acoustic lens (40).

8. The ultrasound probe according to claim 1, further

comprising a current adjusting unit (41) allowing a user to adjust current applied to the focus adjusting unit (43) through the current applying unit (42).

9. A manufacturing method of an ultrasound probe comprising:

installing a focus adjusting unit (43), deforming the shape of an acoustic lens (40) to adjust the focus of ultrasonic waves radiated through the acoustic lens (40), on the acoustic lens (40);
installing a current applying unit (42) applying current to the focus adjusting unit (43) to contract or expand the focus adjusting unit (43); and
installing the acoustic lens (40) provided with the focus adjusting unit (43) on the front surface of a matching layer.

10. The manufacturing method according to claim 9, wherein the focus adjusting unit (43) includes at least one wire formed of a shape memory alloy that is deformed according to supply of current.

11. The manufacturing method according to claim 10, wherein the installation of the focus adjusting unit (43) includes attaching or inserting the at least one wire to or into the acoustic lens (40) in the azimuthal direction.

12. The manufacturing method according to claim 10, wherein the installation of the focus adjusting unit (43) includes attaching or inserting the at least one wire to or into the acoustic lens (40) along the boundary of the acoustic lens (40).

13. A control method of an ultrasound probe according to claim 1 comprising:

receiving a signal output from a current adjusting unit (41) of the ultrasound probe corresponding to user operation;
outputting a current applying signal corresponding to the signal output from the current adjusting unit (41) to the current applying unit (42) of the ultrasound probe; and
causing the current applying unit (42) to apply current to the focus adjusting unit (43) of the ultrasound probe according to the current applying signal.

Patentansprüche

1. Ultraschallsonde, welche folgendes aufweist:

eine akustische Linse (40);
eine Fokuseinstelleinheit (43), die auf der akustischen Linse (40) angeordnet ist und die Form

- der akustischen Linse (40) deformiert, um den Fokus von durch die akustische Linse (40) hindurch gestrahlten Ultraschallwellen einzustellen; und
eine Stromaufbringungseinheit (42), welche Strom auf die Fokuseinstelleinheit (43) aufbringt, um die Fokuseinstelleinheit (43) zu kontrahieren oder zu expandieren.
2. Ultraschallsonde nach Anspruch 1, wobei die Fokuseinstelleinheit (43) wenigstens einen Draht aufweist, der aus einer Formgedächtnislegierung gebildet ist, die entsprechend der Zuführung von Strom deformiert wird.
 3. Ultraschallsonde nach Anspruch 2, wobei der wenigstens eine Draht in der azimuthalen Richtung an der akustischen Linse (40) angebracht oder in dieselbe eingeführt ist.
 4. Ultraschallsonde nach Anspruch 2, wobei der wenigstens eine Draht entlang des Rands der akustischen Linse (40) an der akustischen Linse (40) angebracht oder in dieselbe eingeführt ist.
 5. Ultraschallsonde nach Anspruch 2, wobei die Stromaufbringungseinheit (42) Strom auf den wenigstens einen Draht aufbringt, um den wenigstens einen Draht zu kontrahieren oder zu expandieren.
 6. Ultraschallsonde nach Anspruch 1, wobei die Fokuseinstelleinheit (43) die Form der akustischen Linse (40) deformiert, um die Krümmung der akustischen Linse (40) zu verändern.
 7. Ultraschallsonde nach Anspruch 1, wobei, wenn von der Stromaufbringungseinheit (42) Strom auf die Fokuseinstelleinheit (43) aufgebracht wird, die Fokuseinstelleinheit (43) die Krümmung der akustischen Linse (40) kontrahiert und vergrößert.
 8. Ultraschallsonde nach Anspruch 1, welche des Weiteren eine Stromeinstelleinheit (41) aufweist, welche es einem Benutzer erlaubt, den auf die Fokuseinstelleinheit (43) durch die Stromaufbringungseinheit (42) aufgebrachten Strom einzustellen.
 9. Verfahren zur Herstellung einer Ultraschallsonde, welches folgendes aufweist:
Installieren einer Fokuseinstelleinheit (43), welche die Form einer akustischen Linse (40) deformiert, um den Fokus von durch die akustische Linse (40) gestrahlten Ultraschallwellen auf die akustische Linse (40) einzustellen;
Installieren einer Stromaufbringungseinheit (42), welche Strom auf die Fokuseinstelleinheit (43) aufbringt, um die Fokuseinstelleinheit (43) zu kontrahieren oder expandieren; und
Installieren der akustischen Linse (40), die von der Fokuseinstelleinheit (43) zur Verfügung gestellt wird, auf der vorderen Fläche einer passenden Schicht.
 10. Herstellungsverfahren nach Anspruch 9, wobei die Fokuseinstelleinheit (43) wenigstens einen Draht aufweist, der aus einer Formgedächtnislegierung gebildet ist, die entsprechend der Zuführung von Strom deformiert wird.
 11. Herstellungsverfahren nach Anspruch 10, wobei die Installation der Fokuseinstelleinheit (43) das Anbringen oder Einführen des wenigstens einen Drahts in der azimuthalen Richtung an oder in die akustische Linse (40) beinhaltet.
 12. Herstellungsverfahren nach Anspruch 10, wobei die Installation der Fokuseinstelleinheit (43) das Anbringen oder Einführen des wenigstens einen Drahts entlang des Rands der akustischen Linse (40) an oder in die akustische Linse (40) beinhaltet.
 13. Verfahren zur Steuerung einer Ultraschallsonde nach Anspruch 1, welches folgendes aufweist:
Empfangen eines Signalausgangs von einer Stromeinstelleinheit (41) der Ultraschallsonde entsprechend der Eingabe eines Benutzers;
Ausgeben eines Stromaufbringungssignals entsprechend der Signalausgabe von der Stromeinstelleinheit (41) auf die Stromaufbringungseinheit (42) der Ultraschallsonde; und
Bewirken, dass die Stromaufbringungseinheit (42) Strom auf die Fokuseinstelleinheit (43) der Ultraschallsonde entsprechend dem Stromaufbringungssignal aufbringt.

Revendications

1. Sonde ultrasonique comportant :

une lentille acoustique (40);
une unité d'ajustage du foyer (43) installée sur la lentille acoustique (40) et déformant la forme de la lentille acoustique (40) pour ajuster le foyer des ondes ultrasoniques rayonnant à travers la lentille acoustique (40) ; et
une unité d'application de courant (42) appliquant un courant sur l'unité d'ajustage du foyer (43) pour contracter ou provoquer l'expansion de l'unité d'ajustage du foyer (43).

2. Sonde ultrasonique selon la revendication 1, dans laquelle l'unité d'ajustage du foyer (43) comporte au moins un câble réalisé en un alliage à mémoire de

forme qui est déformé selon le courant appliqué.

3. Sonde ultrasonique selon la revendication 2, dans laquelle ledit au moins un câble est lié à ou inséré dans la lentille acoustique (40) dans la direction azimutale. 5
4. Sonde ultrasonique selon la revendication 2, dans laquelle ledit au moins un câble est lié à ou inséré dans la lentille acoustique (40) le long du bord de la lentille acoustique (40). 10
5. Sonde ultrasonique selon la revendication 2, dans laquelle l'unité d'application de courant (42) délivre un courant audit au moins un câble pour contracter ou provoquer l'expansion dudit au moins un câble. 15
6. Sonde ultrasonique selon la revendication 1, dans laquelle l'unité d'ajustage du foyer (43) déforme la forme de la lentille d'ajustage (40) pour modifier la courbure de la lentille acoustique (40). 20
7. Sonde ultrasonique selon la revendication 1, dans laquelle, lorsque le courant est appliqué à l'unité d'ajustage du foyer (43) par l'unité d'application d'un courant (42), l'unité d'ajustage du foyer (43) contracte et augmente la courbure de la lentille d'ajustage (40). 25
8. Sonde ultrasonique selon la revendication 1, comprenant en outre une unité d'ajustage de courant (41) permettant à un utilisateur d'ajuster le courant appliqué à l'unité d'ajustage du foyer (43) au moyen de l'unité d'application d'un courant (42). 30
9. Procédé de fabrication d'une sonde ultrasonique comprenant : 35
 - l'installation d'une unité d'ajustage du foyer (43), modifiant la forme de la lentille acoustique (40) pour ajuster le foyer des ondes ultrasoniques rayonnant à travers la lentille acoustique (40), sur la lentille acoustique (40) ; 40
 - l'installation d'une unité d'application de courant (42) appliquant un courant sur l'unité d'ajustage du foyer (43) pour contracter ou provoquer l'expansion de l'unité d'ajustage du foyer (43) ; et 45
 - l'installation d'une lentille acoustique (40) équipée de l'unité d'ajustage du foyer (43) sur la surface frontale d'une couche d'ajustage. 50
10. Procédé de fabrication selon la revendication 9, dans lequel l'unité d'ajustage du foyer (43) comporte au moins un câble réalisé en un alliage à mémoire de forme qui est déformé selon le courant appliqué. 55
11. Procédé de fabrication selon la revendication 10, dans lequel l'installation de l'unité d'ajustage du

foyer (43) comporte la liaison ou l'insertion dudit au moins un câble à la ou dans la lentille acoustique (40) dans la direction azimutale.

12. Procédé de fabrication selon la revendication 10, dans lequel l'installation de l'unité d'ajustage du foyer (43) comporte la liaison ou l'insertion dudit au moins un câble à la ou dans la lentille acoustique (40) le long du bord de la lentille acoustique (40).

13. Procédé de commande d'une sonde ultrasonique, selon la revendication 1, comportant :

la réception d'un signal émis par une unité d'ajustage de courant (41) de la sonde ultrasonique correspondant à une opération d'un utilisateur ;

l'émission d'un signal d'application d'un courant correspondant au signal émis par l'unité d'ajustage de courant (41) à l'unité d'application d'un courant (42) de la sonde ultrasonique ;

et

la cause de l'application d'un courant par l'unité d'application d'un courant (42) sur l'unité d'ajustage du foyer (43) de la sonde ultrasonique en fonction du signal d'application de courant.

FIG. 1




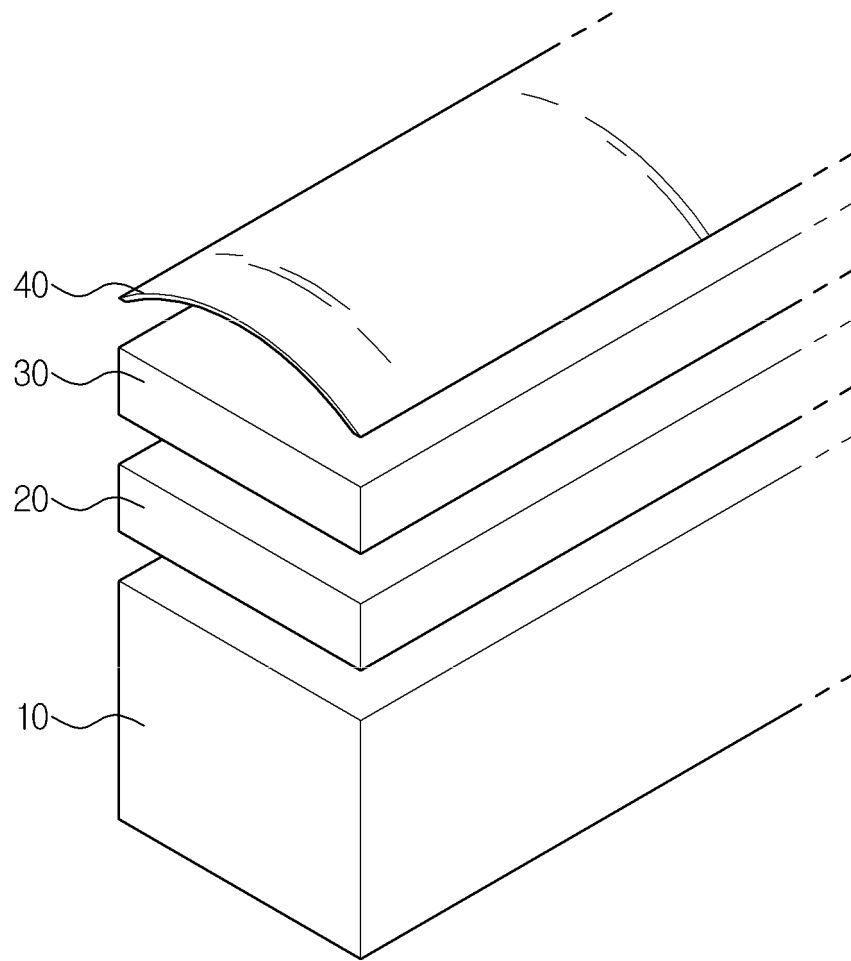


FIG. 2

(a)

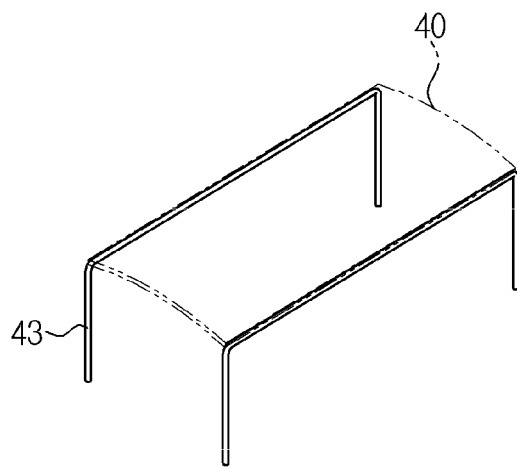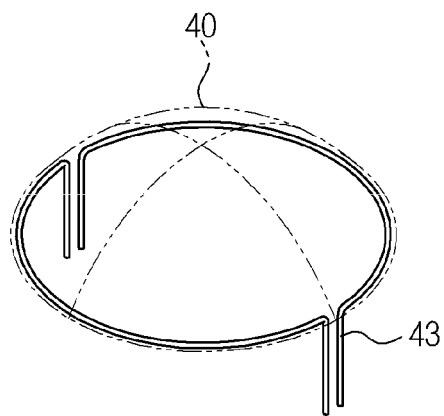

(b)

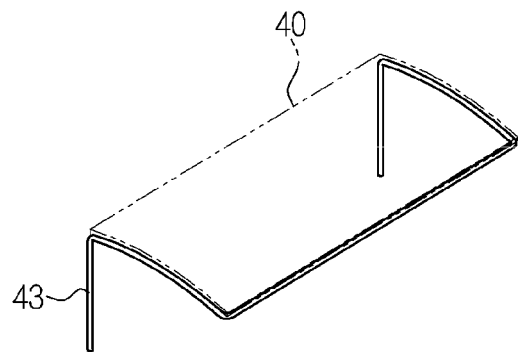

(c)

FIG. 3

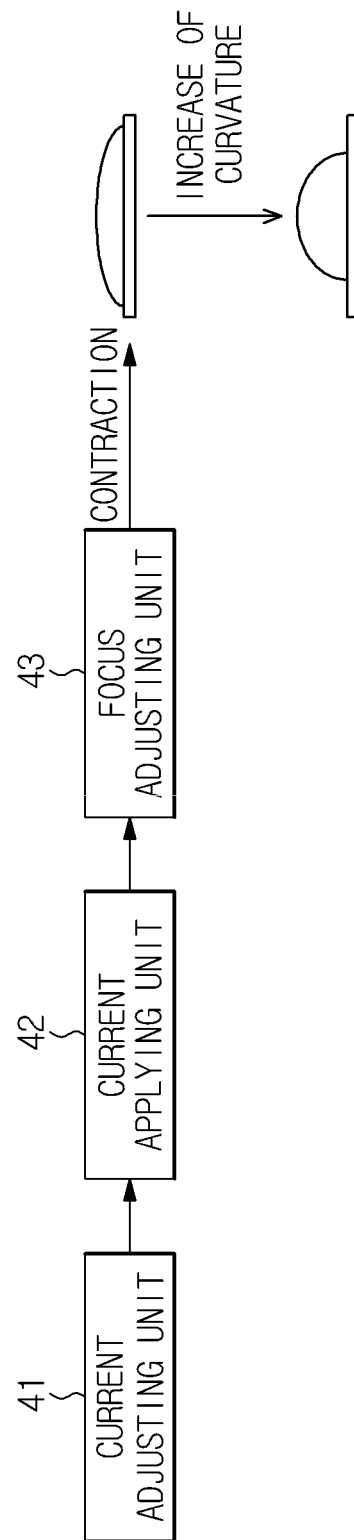


FIG. 4


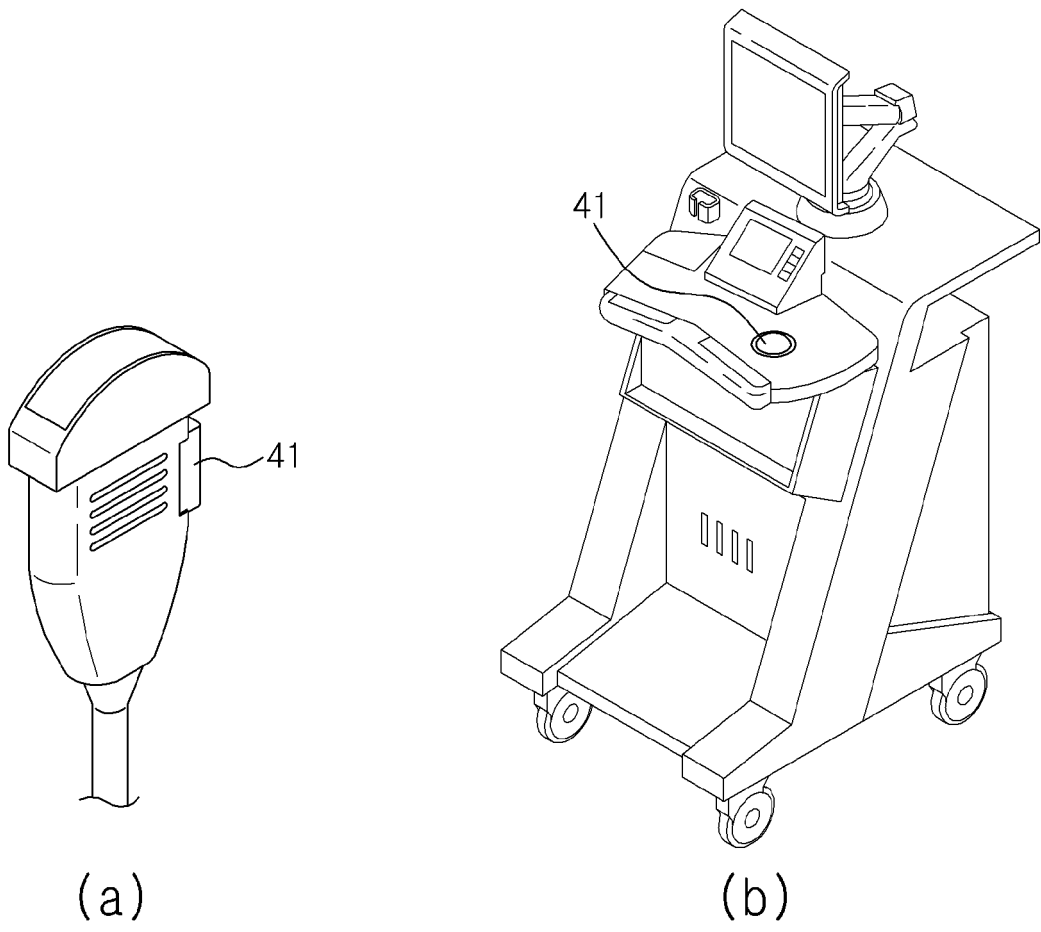


FIG. 5

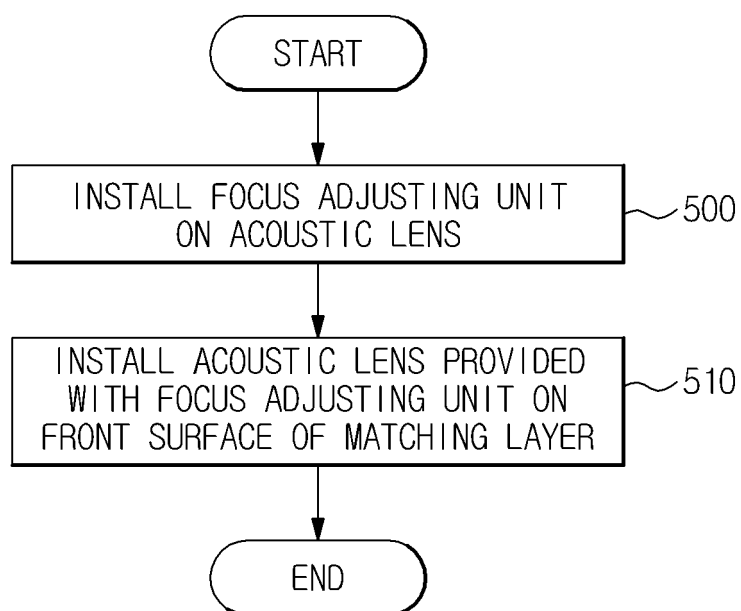

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- EP 2405671 A1 [0006]
- EP 1816492 A1 [0007]
- WO 2007125500 A2 [0008]

专利名称(译)	超声探头及其制造方法		
公开(公告)号	EP2808865B1	公开(公告)日	2017-04-26
申请号	EP2014151364	申请日	2014-01-16
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	YOO BEOM KEUN		
发明人	YOO, BEOM KEUN		
IPC分类号	G10K11/30 A61B8/00		
CPC分类号	A61B8/4444 G10K11/30 Y10T29/49826 A61B8/4281 A61B8/54		
代理机构(译)	SCHMID , WOLFGANG		
优先权	1020130061410 2013-05-30 KR		
其他公开文献	EP2808865A1		
外部链接	Espacenet		

摘要(译)

本文公开了一种超声探头，其可以使用形状记忆合金来调节声透镜的曲率。超声探头包括声透镜，安装在声透镜上的焦点调节单元和使声透镜的形状变形以调节通过声透镜辐射的超声波的焦点，以及电流施加单元向焦点调节单元施加电流收缩或扩大焦点调整单位。

FIG. 1

