

(19)



(11)

EP 3 322 344 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

20.05.2020 Bulletin 2020/21

(51) Int Cl.:

A61B 8/00 (2006.01)

(86) International application number:

PCT/IB2016/053998

(21) Application number: **16738226.6**

(22) Date of filing: **04.07.2016**

(87) International publication number:

WO 2017/009735 (19.01.2017 Gazette 2017/03)

(54) **WIRELESS ULTRASOUND PROBE PAIRING WITH A MOBILE ULTRASOUND SYSTEM**

DRAHTLOSE ULTRASCHALLSONDENPAARUNG MIT EINEM MOBILEN ULTRASCHALLSYSTEM

APPARIEMENT DE SONDE À ULTRASON SANS FIL AVEC SYSTÈME À ULTRASON MOBILE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(72) Inventors:

- **BELL, Kristy**
5656 AE Eindhoven (NL)
- **POLAND, McKee Dunn**
5656 AE Eindhoven (NL)
- **HUNT, Alexander**
5656 AE Eindhoven (NL)

(30) Priority: **16.07.2015 US 201562193210 P**

(43) Date of publication of application:

23.05.2018 Bulletin 2018/21

(74) Representative: **Mumbrú Forn, José**

Société Civile SPID
33, rue de Verdun
92150 Suresnes (FR)

(60) Divisional application:

20150926.2

(73) Proprietor: **Koninklijke Philips N.V.**

5656 AG Eindhoven (NL)

(56) References cited:

US-A1- 2008 114 241 US-A1- 2008 242 220
US-A1- 2013 245 451 US-A1- 2014 180 110

EP 3 322 344 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] This invention relates to medical diagnostic ultrasound systems and, in particular, to the pairing of a wireless ultrasound probe with the desired ultrasound system.

[0002] An ultrasound probe transmits ultrasound waves and receives ultrasonic echo signals with piezo-electric transducer elements that mechanically deflect when driven by a high voltage signal and convert vibrations due to received echo signals into electrical signals. Historically, ultrasound probes have been detachably connected to an ultrasound system by multiconductor cables which couple power and signals between the ultrasound system mainframe, which processes the echo signals into images, and the probe. To afford great latitude in positioning the ultrasound system, patient, and sonographer, these probe cables can be lengthy, extending upwards of three meters in length. But numerous sonographers do not like the inconvenience of the probe cable, which can be heavy, become tangled, and drag on the floor and get run over by the wheels when the ultrasound cart is moved or repositioned. The solution to this dilemma is a wireless ultrasound probe whereby communication with the system mainframe is done by r.f. communication and the probe is battery-powered. While wireless probes were first invented in 1998 as shown in US Pat. 6,142,946 (Hwang et al.), their development and integration into mainstream diagnostic ultrasound has been slow. But aided by improved r.f. spectra availability, transceivers with greater bandwidth and performance, and smaller and lighter batteries, the prospects for wireless probes are brighter than ever before.

[0003] Before a wireless probe can be used to scan a patient, it must first be put into reliable two-way communication with the ultrasound system mainframe. A patent which has considered this step is US Pat. 8,656,783 (Randall et al.), where this process is termed "linkup" as described in conjunction with Fig. 9 of the patent. This patent proposes to establish a communication link between a probe and an ultrasound system based upon the proximity of the two with each other and/or with other devices. For instance, if the probe and system are in proximity such that they are within r.f. range of each other, the communication link would be established. If there are multiple probes and/or systems within range, linkup would occur between the probe and system within closest proximity. The patent also proposes that the user may participate in the linkup by pressing a button to communicate a particular data sequence or character between the system and the probe to establish the linkup. The user may also select a desired probe type from a list of different types of probes, causing the system to send a linkup request to probes of the selected type. The patent goes on to say that the system and the probe may identify each other by their proximity (e.g., the linked probe is the one nearest the system), strength of signal communicated by the system (e.g., the probe links to the system

sending the strongest signal), communication of a predetermined identifier, or the absence of any other probes. Once a communication link is established, it will endure for at least one operating session or over some predetermined period of time.

[0004] The list of linkup factors and possibilities proposed by Randall et al., however, does not fully consider the unlimited portability of wireless probes in a hospital or clinic, and the interactions between sonographers in a setting with many systems and probes, as is common in many clinical practices today. Simply linking the probe in closest proximity to a system becomes ambiguous when sonographer A, with a probe in the pocket of her lab coat, comes over to speak with sonographer B at sonographer B's ultrasound system. When sonographer B puts down her probe to have a dialog with sonographer A, the system will link with the now nearer probe in sonographer A's pocket, disrupting sonographer B's exam and leading to confusion. Linking with a probe that come into range, or even with the probe in closest proximity, is undesirable. If the sonographer takes a lunch break before a defined operating session has concluded, should the probe and system try to maintain the linkup? If a sonographer walks by with another mobile ultrasound system during the break, the linkup of one or both systems to the probe can change. If the predetermined time period expires before the sonographer has finished the exam, should the probe and system end their communication? These dilemmas, unaddressed by the Randall et al. patent, will be posed repeatedly in the large diagnostic labs in common practice today, and must be addressed and resolved so that the proper probe is quickly paired with the proper ultrasound system and remains in communication with it without interruption at all times during the diagnostic exam.

[0005] US 2013/245451 discloses an ultrasonic diagnostic apparatus having multiple ultrasonic probes and an apparatus body. The probes are connected to the apparatus body and an interface unit controls switching between the multiple probes. Lights on the probes are controlled in dependence upon a connection state.

[0006] US 2014/180110 discloses a system for pairing a wireless ultrasound probe and an ultrasound scanner via near field communication (NFC) connection.

[0007] US 2008/114241, similar to the aforementioned US Pat. 8,656,783, discloses a method for establishing linkup between a probe and a main unit based on proximity between the two.

[0008] In some aspects, the present invention provides methods for pairing a wireless ultrasound probe with a mobile ultrasound system. The methods can include locating a wireless ultrasound probe with a radio within a predetermined range of a mobile ultrasound system with a radio, determining, at the mobile ultrasound system, that the wireless ultrasound probe present is within the predetermined range, and pairing the wireless ultrasound probe and mobile ultrasound system to be in communication with each other when the wireless ultrasound

probe is determined to be present in the predetermined range and when the mobile ultrasound system is determined not to be in communication with another wireless ultrasound probe.

[0009] In certain aspects, the predetermined range is one meter, or the predetermined range is a distance of one meter from an antenna of the mobile ultrasound system radio. In some aspects, the ultrasound system radio and the wireless probe radio are both ultra wideband transceivers, such as WiFi (802.11) standard transceivers.

[0010] In some aspects, the determining step of the methods can further include receiving with the ultrasound system radio a radio signal from the wireless probe and producing a signal indicating the strength of the received signal. The determining step can further include comparing the signal indicating the strength of the received signal to a threshold voltage. The producing step can further include producing an RSSI signal by the ultrasound system radio. In certain aspects, the threshold voltage is equal to a signal indicating the strength of the received signal when the wireless probe is at the predetermined distance from the ultrasound system.

[0011] In certain aspects, the methods can further include maintaining a communication link established by the pairing until the user affirmatively ends it; or the wireless ultrasound probe is turned off; or the wireless ultrasound probe has been out of range of the mobile ultrasound system for a long period of time; or the communication of new data over the link has been idle for a preset period of time.

[0012] In some aspects, the methods can further include conducting an ultrasound exam with the paired wireless ultrasound probe and mobile ultrasound system; suspending the ultrasound exam; and actuating a user control of the mobile ultrasound system to maintain the paired communication during suspension of the ultrasound exam.

[0013] In certain aspects, the present invention can include a method for pairing one of a plurality of wireless ultrasound probes that are within radio range of a mobile ultrasound system with the mobile ultrasound system that includes locating a plurality of wireless ultrasound probes, each having a radio, within radio range of a mobile ultrasound system having a radio; receiving, with the radio of the mobile ultrasound system, a unique identifier signal from each of the wireless ultrasound probes; displaying on a display of the mobile ultrasound system the identities of the wireless ultrasound probes in correspondence with the unique identifier signals; and pairing a particular wireless ultrasound probe and the mobile ultrasound system by selecting the displayed identity of the particular wireless ultrasound probe.

[0014] In some aspects, the displaying step can include displaying the identities of the wireless ultrasound probes in order of the strength of signals received from the probes, and/or the displaying can include displaying the identity of a wireless ultrasound probe only if it is

within a predetermined distance of the mobile ultrasound system; and wherein pairing further comprises selecting the displayed wireless ultrasound probe for pairing.

[0015] In certain aspects, the methods can include maintaining a communication link established by the pairing until the user affirmatively ends it; or the particular wireless ultrasound probe is turned off; or the particular wireless ultrasound probe has been out of range of the mobile ultrasound system for a long period of time; or the communication of new data over the link has been idle for a preset period of time.

[0016] In the drawings:

FIGURE 1 illustrates an ultrasound lab with several wireless probes and four mobile ultrasound systems capable of communicating with the wireless probes. FIGURE 2 illustrates the functional components of a wireless 2D array probe.

FIGURE 3 illustrates in block diagram form the major electronic subsystems between the microbeam-former and antenna of the wireless probe of FIGURE 2.

FIGURE 4a illustrates in block diagram form the major components of a radio module for a mobile ultrasound system constructed in accordance with the principles of the present invention which is capable of communicating with the probe of FIGURE 2.

FIGURE 4b illustrates the packaging of the radio module of FIGURE 4a, which is configured as a USB stick.

FIGURE 5 illustrates in block diagram form the components of the pairing circuit of FIGURE 4a and their interface with other components of the USB stick.

FIGURE 6 illustrates a display screen of a mobile ultrasound system showing a variety of wireless probes which can be paired with the ultrasound system.

[0017] In accordance with the principles of the present invention, a wireless probe is paired to be in r.f. communication with a mobile ultrasound system when the probe is brought within a predetermined distance of the ultrasound system, as indicated by the received signal strength indication (RSSI) at the ultrasound system's radio. The radio type used by the probe and the ultrasound system can be ultra wideband (UWB) transceivers, WiFi (IEEE 802.11) transceivers, or transceivers of some other standard. The probe transmits an identifier which uniquely identifies that probe. The signal transmitted by the probe is calibrated to the predetermined distance so that, when the probe is at or closer than the predetermined distance with the ultrasound system, the RSSI received and measured at the system will be at or above a predetermined threshold. When this condition occurs, the system automatically selects the probe's unique transmitted identifier as the one with which to establish communication for an ultrasound procedure. The pairing process can be set to occur automatically when a wire-

less probe is brought within the predetermined range and the system is not currently in communication with another probe, or can be initiated by the user pressing a button on the system when a probe is within the predetermined range. The communication link is maintained until the user affirmatively ends it, or until the wireless probe is turned off, or until the wireless probe has been out of range of the ultrasound system for a long period of time, or for as long as data is being communicated over the link, or until after the communication of new data over the link has been idle for a preset period of time, i.e., the idle link times out.

[0018] In accordance with a further aspect of the present invention, the user can select a wireless probe with which to pair from a list of probes on the display of the ultrasound system. The displayed list is a list of the probes currently found to be within r.f. communication range of the ultrasound system, and is preferably displayed on the screen in signal strength order, that is, the probe nearest to the system is at the top of the list. The user then selects a probe to pair to the system and, if the probe is not presently linked to be in communication with another system, the communication link to that probe is established.

[0019] FIGURE 1 depicts an ultrasound lab with four mobile ultrasound systems in it, a premium Epiq system 20, a midrange ClearVue system 30, a tablet style Visiq system 40, and a laptop style CX50 system 50, all made by Philips Healthcare of Andover, MA, USA. In this example, all of the ultrasound systems have wireless capability and so are able to work with wireless ultrasound probes. Also in the lab are three wireless probes, including probe 10a which is being used with the laptop system 50 and probe 10b which is being used with the tablet system 40. The third probe 10c is in the process of being carried through the lab to be used with the premium system 20. As it does so in this example, it passes into close proximity with the laptop system 50. If the pairing protocol used by these systems and probes would pair a probe and system which are in closest proximity, the in-transit probe 10c could pair with the laptop system 50 as it passes close to the antenna 54 of the laptop system's radio. This undesired pairing would disrupt the intended use of probe 10a with the laptop system 50, and illustrates a problem with proximity pairing which must be addressed.

[0020] FIGURE 1 also illustrates a dashed circle 60 which in this example is marking the outer boundary of a spherical one meter distance from the radio antenna 54 of the laptop system 50. The problem just described is prevented in accordance with the present invention by bringing a probe 10a within one meter or less of the antenna 54 in order to pair the probe 10a with ultrasound system 50. Once the probe 10a is within this distance from the antenna, pairing can proceed either automatically or with user assistance such as by touching or clicking a "Pair" button on the display screen 56 or control panel 58 of the ultrasound system 50. The probe 10c remains paired with the ultrasound system 50 until the

user affirmatively de-associates the probe from the system as by touching or clicking an "End Exam" button on the system; or turns off the probe; or the probe goes out of range of the radio of system 50 for an extended period of time, a length of time which can be determined by the user during system setup. A pairing and de-association procedure such as this will prevent the foregoing problem from happening. If someone passes by carrying a powered-on wireless probe 10c that is within radio range of system 50, pairing will not occur because the transported probe is not within the one meter distance required for pairing. And even if the transported probe passes within the one meter distance and even is in closer proximity to antenna 54 than is probe 10a, no pairing will occur because probe 10a has been previously paired with the system and is in use with (within radio range of) the system.

[0021] The pairing procedure of the present invention may be implemented with a wireless ultrasound probe such as that shown in FIGURE 2. In order to scan a two dimensional image plane the probe 10 uses a one-dimensional (1D) transducer array located at the distal end 12 of the probe at the acoustic window of the probe. For both two dimensional and three dimensional electronic scan imaging, the probe uses a 2D matrix array transducer 80 as shown in this example. The transducer array is formed of ceramic piezoelectric transducer elements, a piezoelectric polymer (PVDF), or may be a semiconductor-based micromachined ultrasound transducer (MUT) such as a PMUT (piezoelectric MUT) or a CMUT (capacitive MUT) array of elements. The array transducer 80 is driven by, and echoes are processed by, one or more microbeamformer ASICs 82. The microbeamformer 82 receives echo signals from the elements of the transducer array 80 and delays and combines the per-element echo signals into a small number of partially beamformed signals. For instance the microbeamformer 82 can receive echo signals from a row of 128 transducer elements of the array and combine these signals to form eight partially beamformed signals, thereby reducing the number of signal paths from 128 to eight. The microbeamformer 82 can also be implemented to produce fully beamformed signals from all of the elements of the active aperture as described in US Pat. 6,142,946 (Hwang et al.) In a preferred embodiment fully beamformed and detected signals are produced by the probe for wireless transmission to the host ultrasound system so as to reduce the data rate to one which accommodates acceptable real time imaging frame rates. Microbeamformer technology suitable for use in beamformer 82 is described in US Pats. 5,229,933 (Larson III); 6,375,617 (Fraser); and 5,997,479 (Savord et al.) The beamformed echo signals are coupled to a probe controller and transceiver subsystem 74 which transmits the beamformed signals to a host system, the mainframe ultrasound system such as ultrasound system 20, 30, 40 or 50, where the partially beamformed signals undergo further beamforming and then image processing and display. The

probe controller and transceiver subsystem 74 also receives control signals from the host system when the probe is controlled from the host, and couples corresponding control signals to the microbeamformer 82 to, for example, steer and focus beams at a desired depth or transmit and receive signals of a desired mode (Doppler, B mode) to and from a desired location of an image region. Not shown in this illustration are the power subsystem and battery to power the probe, which are described below.

[0022] The transceiver of the probe controller and transceiver subsystem 74 transmits and receives r.f. signals 16 by means of an internal or stub antenna 76, similar to that of a cellphone. The stub antenna provides one of the same benefits as it does on a cellphone, which is that its small profile makes it convenient to hold and carry and reduces the possibility of damage. However in this embodiment of a wireless probe, the stub antenna 76 serves an additional purpose. When a sonographer holds a conventional cabled probe, the probe is grasped from the side as if holding a thick pencil. A wireless probe such as that of FIGURE 2 can be held in the same manner, however, since the probe has no cable, it can also be held by grasping the proximal end of the probe. This cannot be done with a conventional cabled probe due to the presence of the cable. A wireless probe user may want to hold the wireless probe by the proximal end in order to exert a large amount of force against the body for good acoustic contact. However, wrapping the hand around the proximal end of the probe, when the antenna is inside the proximal end of the probe, will at least partially shield the antenna from signal transmission and reception and may cause unreliable communication. It has been found that using an antenna which projects from the proximal end of the probe not only extends the antenna field well outside the probe case 8, but also discourages the user from holding the probe by the proximal end due to the discomfort of pressing against the stub antenna. Instead, the user is more likely to grasp the probe from the side in the conventional manner, leaving the antenna field exposed for good signal transmission and reception. For good reception the antenna configuration of the base station host can introduce some diversity against polarization and orientation effects by producing two complementary beam patterns with different polarizations. Alternatively, the antenna can be a single high performance dipole antenna with a good single polarization beam pattern. With the antenna at the proximal end of the probe, the probe beam pattern can extend radially with respect to the longitudinal axis of the probe, and readily intersect the beam pattern of the base station host. Such a probe beam pattern can be effective with antennas of the base station host located at the ceiling, as may be done in a surgical suite. Reception has also been found to be effective with this probe beam pattern from reflections by room walls and other surfaces, which are often close to the site of the ultrasound procedure, such as a diagnostic imaging exam. Typically a ten meter range is sufficient for

most exams, as the probe and base station host are in close proximity to each other. Communication frequencies employed can be in the 4GHz range, and suitable polymers for the probe case 8 such as ABS are relatively transparent to r.f. signals at these frequencies. R.f. communication can be improved at the base station host, where multiple antennae can be employed for improved diversity in embodiments where multiple antennae are not cumbersome as they would be for the wireless probe. See, for example, International Patent Publication WO 2004/051882, entitled "Delay Diversity In A Wireless Communications System." The multiple antennae can utilize different polarizations and locations to provide reliable communications even with the varying linear and angular orientations assumed by the probe during the typical ultrasound exam. The typical probe manipulation can roll the probe throughout a 360° range of rotation and tilt angles through approximately a hemispherical range of angles centered on vertical. Hence, a dipole radiation pattern centered on the center longitudinal axis of the probe will be optimal for a single antenna and a location at the proximal end has been found to be most desirable. The antenna pattern can be aligned exactly with this center axis, or offset but still in approximate parallel alignment with this center axis.

[0023] A typical probe controller and transceiver subsystem for a wireless probe is shown in FIGURE 3. A battery 92 powers the wireless probe and is coupled to a power supply and conditioning circuit 90. The power supply and conditioning circuit translates the battery voltage into a number of voltages required by the components of the wireless probe including the transducer array. A typical constructed probe may require nine different voltages, for example. The power supply and conditioning circuit also provides charge control during the recharging of the battery 92. In a constructed embodiment the battery is a lithium polymer battery which is prismatic and can be formed in a suitable shape for the available battery space inside the probe case.

[0024] An acquisition module 94 provides communication between the microbeamformer and the transceiver. The acquisition module provides timing and control signals to the microbeamformer, directing the transmission of ultrasound waves and receiving at least partially beamformed echo signals from the microbeamformer, which are demodulated and detected (and optionally scan converted) and communicated to the transceiver 96 for transmission to the base station host. In this example the acquisition module communicates with the transceiver over a parallel or a USB bus so that the probe can be used with a USB cable when desired. If a USB or other bus is employed, it can provide an alternative wired connection to the base station host over a cable, thus bypassing the transceiver portion 96 and becoming a wired probe.

[0025] Also coupled to the acquisition module 94 and powered by the power supply and conditioning circuit 90 is a loudspeaker 102, driven by an amplifier 104, which produces audible tones or sounds. In a preferred embod-

iment the loudspeaker 102 is a piezoelectric loudspeaker located inside the case 8 and which may be behind a membrane or the wall of the case for good acoustics and sealing. The loudspeaker can be used to produce a variety of sounds or tones or even voice messages. The loudspeaker has a variety of uses. If the wireless probe is moved too far away from the host so that there is unreliable reception or even a complete loss of signal by the host or the probe, the loudspeaker can beep to alert the user. The loudspeaker can also emit a unique tone when the probe is within the one meter pairing distance. The loudspeaker can beep when the battery charge is low. The loudspeaker can emit a tone when the user presses a button or control on the probe, providing audible feedback of control activation. The loudspeaker can provide haptic feedback based upon the ultrasound examination. The loudspeaker can emit a sound when a paging control is activated to locate the probe. The loudspeaker can produce audio Doppler sounds during a Doppler exam, or heart sounds when the probe is used as an audio stethoscope.

[0026] The transceiver in this example is an ultra wideband chip set 96, although it can also be a WiFi (802.11 standard) radio or other standard radio. An ultra wideband transceiver was found to have a data communication rate which provides acceptable real time imaging frame rates as well as acceptable range for an acceptable level of battery power consumption. Ultra wideband chip sets are available from a variety of sources such as Starix of Irvine, California and Alereon of Austin, Texas. WiFi radio adapters such as the Netgear N300 wireless-N USB adapter are also suitable for wireless WiFi communication.

[0027] FIGURE 4a illustrates the wireless probe signal path at the base station host, here shown in the laptop system configuration 50. The antenna 54 is coupled to an identical or compatible ultra wideband chip set 96 which performs transception at the host. In a preferred embodiment for the laptop configuration, the antenna 54 and ultra wideband chip set are configured as a USB-connectible "dongle" 110 as shown in FIGURE 4b, which plugs into and is powered by a USB port of the host system 50. The optional USB link between probe and the host laptop allows charging of the battery in the probe, via the power connection, or wired data transfer when preferred over wireless operation. Further details of the wireless probe and mobile ultrasound system shown in FIGURES 2-4b may be found in US pat. pub. no. 2010/0168576 (Poland et al.)

[0028] In accordance with the principles of the present invention, the USB radio module 110 also includes a pairing circuit 98. While the pairing circuit 98 in this example is shown located in the radio module 110, it could also be implemented in the ultrasound system. The pairing circuit responds to a pairing request from a wireless probe, such as the presence of a wireless probe within the one meter pairing distance, verifies that the probe is within the pairing distance and, if so, commands the ul-

trasound system 50 to proceed with the pairing protocol.

[0029] One implementation of a pairing circuit 98 is shown in FIGURE 5. Radios such as the UWB chip set commonly produce a signal indicating the strength of received signals known as the received signal strength indicator (RSSI). An equivalent signal can be produced by envelope-detecting a received probe radio signal, which also indicates the strength (amplitude) of the received signal. The RSSI signal from the UWB chip set is coupled to one input of a comparator 32, which compares the RSSI with a threshold voltage V_{TH} . This threshold voltage is preset and is approximately equal to the RSSI produced in response to signals from a wireless probe when the probe is one meter from the radio antenna. Thus, a wireless probe which is one meter from the mobile system 50 or closer will transmit signals to the system radio which produce an RSSI which equals or exceeds V_{TH} . When that happens, the comparator 32 produces a PAIR signal which is coupled to a low power USB microcontroller 34 along with the data received from the wireless probe by the UWB chip set. The received data includes the unique identifier of the wireless probe. The USB microcontroller couples the PAIR signal to the USB connector of the radio module 110 so that the mobile ultrasound system 50 receives the PAIR signal in USB format. The ultrasound system is thereby notified that a wireless probe has been identified in pairing range and the system responds by reading the probe's unique identifier on the USB data bus 36 and selecting this identifier as the one with which to pair. The ultrasound system and probe then exchange pairing protocol data as is known in the art and the communication between the wireless probe and ultrasound system is established. This exclusive communication connection remains in place unless the user affirmatively ends it as by pressing a control button; or turns off the wireless probe; or does not use the communication link or is out of radio range for a predetermined extended period of time, whereupon the connection times out and is ended by the system or probe.

[0030] To aid the user in reliably pairing with a specific wireless probe, the mobile ultrasound system can produce a display of the wireless probes within radio range as shown in FIGURE 6. In this example the display screen 56 is showing a list of wireless probes identified to be within radio range, as indicated by their transmitted unique identifier signals. The identified probes are preferably listed on the screen in received signal strength order so that the probe nearest to the ultrasound system will be at the top of the list. The ultrasound system uses the RSSI to order the list of probes, each of which is displayed on a screen button 42, 44, or 46. In this example each probe also has a unique number, which is printed on a label on each probe. In this example the user at the ultrasound system is holding a P5-3 wireless probe with the number "#0767" on it. The user can thus look at the number on the physical probe and the number of the identified wireless probe at the top of the list and know that a selection of the top probe on the screen list will

pair the probe she is holding. The user clicks on button 42 on the screen and the ultrasound system proceeds to execute the protocol necessary to pair with the correct probe.

[0031] In this example the mobile ultrasound system also displays a "Pause" user control button 48 in the lower right corner of the screen, which is available while a wireless probe is paired with the system. When the user wants to temporarily suspend an exam for another activity, such as taking a phone call or having a discussion with a colleague, the user clicks on the Pause button 48. This action informs the ultrasound system that, even though the wireless probe is currently not being used to scan a patient, the system is to remain paired with the wireless probe and not break the communication. The system and probe will thus remain in communication, awaiting continuance of the exam until overridden by another action such as the communication link being affirmatively ended by the user, the probe or system being turned off, the two being out of radio range for an extended time, or depletion of the battery charge of the wireless probe.

Claims

1. A method for pairing a wireless ultrasound probe (10) with a mobile ultrasound system (50) having a radio comprising:

locating a wireless ultrasound probe (10) with a radio within a predetermined range of a mobile ultrasound system (50) with a radio;
determining, at the mobile ultrasound system, that the wireless ultrasound probe present is within the predetermined range; and
pairing the wireless ultrasound probe and mobile ultrasound system to be in communication with each other when the wireless ultrasound probe is determined to be present in the predetermined range and when the mobile ultrasound system is determined not to be in communication with another wireless ultrasound probe.

2. The method of Claim 1, wherein the predetermined range comprises one meter.
3. The method of Claim 2, wherein the predetermined range is a distance of one meter from an antenna (54) of the mobile ultrasound system radio.
4. The method of Claim 1, wherein the ultrasound system radio and the wireless probe radio are both ultra wideband transceivers.
5. The method of Claim 1, wherein the ultrasound system radio and the wireless probe radio are both WiFi (802.11) standard transceivers.

6. The method of Claim 1, wherein the determining whether the wireless ultrasound probe (10) is present within the predetermined range further comprises receiving with the ultrasound system radio a radio signal from the wireless probe and producing a signal indicating a strength of the received signal.

7. The method of Claim 6, wherein the producing a signal comprises producing a received signal strength indicator signal by the ultrasound system radio.

8. The method of Claim 6, wherein the determining whether the wireless ultrasound probe (10) is present within the predetermined range further comprises comparing the signal indicating the strength of the received signal to a threshold voltage.

9. The method of Claim 8, wherein the threshold voltage is configured to be equal to the signal indicating the strength of the received signal when the wireless probe (10) is at the predetermined range from the ultrasound system (50).

10. The method of Claim 1, further comprising maintaining a communication link established by the pairing until:

the user affirmatively ends it; or
the wireless ultrasound probe (10) is turned off; or
the wireless ultrasound probe has been out of range of the mobile ultrasound system for a certain period of time; or
the communication of new data over the link has been idle for a preset period of time.

11. The method of Claim 1, further comprising:

conducting an ultrasound exam with the paired wireless ultrasound probe (10) and mobile ultrasound system (50);
suspending the ultrasound exam; and
actuating a user control of the mobile ultrasound system to maintain the paired communication during suspension of the ultrasound exam.

12. The method of Claim 1, wherein the wireless ultrasound probe (10) is one of a plurality of wireless ultrasound probes, each having a radio, wherein the locating comprises locating the plurality of wireless ultrasound probes (10) within the predetermined range of the mobile ultrasound system (50); wherein the determining comprises determining, at the mobile ultrasound system, that each of the wireless ultrasound probes present is within the predetermined range; wherein the method further comprises the steps of:

receiving, with the radio of the mobile ultrasound system, a unique identifier signal from each of the wireless ultrasound probes; and displaying on a display of the mobile ultrasound system the identities of the wireless ultrasound probes in correspondence with the unique identifier signals; and wherein the pairing of a particular wireless ultrasound probe and the mobile ultrasound system comprises selecting the displayed identity of the particular wireless ultrasound probe.

13. The method of Claim 12, wherein the displaying further comprises displaying the identities of the wireless ultrasound probes (10) in order of the strength of signals received from the probes.

14. The method of Claim 12, wherein the displaying further comprises displaying the identity of a wireless ultrasound probe (10) only if it is within a predetermined distance of the mobile ultrasound system (50); and wherein pairing further comprises selecting the displayed wireless ultrasound probe for pairing.

15. The method of Claim 12, further comprising maintaining a communication link established by the pairing until:

the user affirmatively ends it; or
the particular wireless ultrasound probe is turned off; or
the particular wireless ultrasound probe (10) has been out of range of the mobile ultrasound system (50) for a long period of time; or
the communication of new data over the link has been idle for a preset period of time.

Patentansprüche

1. Verfahren zum Paaren einer drahtlosen Ultraschallsonde (10) mit einem mobilen Ultraschallsystem (50), das einem Funkgerät aufweist, umfassend:

Lokalisieren einer drahtlosen Ultraschallsonde (10) mit einem Funkgerät innerhalb einer vorbestimmten Reichweite eines mobilen Ultraschallsystems (50) mit einem Funkgerät;
Bestimmen bei dem mobilen Ultraschallsystem, dass die drahtlose Ultraschallsonde innerhalb der vorbestimmten Reichweite vorhanden ist; und
Paaren der drahtlosen Ultraschallsonde und des mobilen Ultraschallsystems, um miteinander in Verbindung zu stehen, wenn festgestellt wird, dass die drahtlose Ultraschallsonde in der vorbestimmten Reichweite vorhanden ist, und

wenn festgestellt wird, dass das mobile Ultraschallsystem nicht mit einer anderen drahtlosen Ultraschallsonde in Verbindung steht.

2. Verfahren nach Anspruch 1, wobei die vorbestimmte Reichweite einen Meter umfasst.

3. Verfahren nach Anspruch 2, wobei die vorbestimmte Reichweite eine Entfernung von einem Meter von einer Antenne (54) des mobilen Ultraschallsystem-Funkgeräts ist.

4. Verfahren nach Anspruch 1, wobei das Ultraschallsystem-Funkgerät und das drahtlose Sonde-Funkgerät beide Ultra-Breitband-Transceiver sind.

5. Verfahren nach Anspruch 1, wobei das Ultraschallsystem-Funkgerät und das drahtlose Sonden-Funkgerät beide WiFi (802.11) Standard-Transceiver sind.

6. Verfahren nach Anspruch 1, wobei das Bestimmen, ob die drahtlose Ultraschallsonde (10) innerhalb der vorbestimmten Reichweite vorhanden ist, ferner umfasst das Empfangen eines Funksignals von der drahtlosen Sonde mit dem Ultraschallsystems-Funkgerät und das Erzeugen eines Signals, das eine Stärke des empfangenen Signal anzeigt.

7. Verfahren nach Anspruch 6, wobei das Erzeugen eines Signals das Erzeugen eines empfangenen Signalstärke-Indikatorsignals durch das Ultraschallsystems-Funkgerät umfasst.

8. Verfahren nach Anspruch 6, wobei das Bestimmen, ob die drahtlose Ultraschallsonde (10) innerhalb der vorbestimmten Reichweite vorhanden ist, ferner das Vergleichen des Signals, das die Stärke des empfangenen Signals anzeigt, mit einer Schwellenspannung umfasst.

9. Verfahren nach Anspruch 8, wobei die Schwellenspannung so konfiguriert ist, dass sie gleich dem Signal ist, das die Stärke des empfangenen Signals anzeigt, wenn sich die drahtlose Sonde (10) in der vorbestimmten Reichweite von dem Ultraschallsystem (50) befindet.

10. Verfahren nach Anspruch 1, ferner umfassend das Aufrechterhalten einer durch die Paarung hergestellten Kommunikationsverbindung, bis:

der Benutzer sie bejahend beendet; oder
die drahtlose Ultraschallsonde (10) ausgeschaltet ist; oder
die drahtlose Ultraschallsonde für einen bestimmten Zeitraum außerhalb der Reichweite des mobilen Ultraschallsystems war; oder

die Kommunikation neuer Daten über die Verbindung für einen voreingestellten Zeitraum inaktiv war.

11. Verfahren nach Anspruch 1, ferner umfassend:

Durchführen einer Ultraschalluntersuchung mit der gepaarten drahtlosen Ultraschallsonde (10) und dem mobilen Ultraschallsystem (50);
Aussetzen der Ultraschalluntersuchung; und
Betätigen einer Benutzersteuerung des mobilen Ultraschallsystems, um die gepaarte Kommunikation während der Aussetzung der Ultraschalluntersuchung aufrechtzuerhalten.

12. Verfahren nach Anspruch 1, wobei die drahtlose Ultraschallsonde (10) eine von mehreren drahtlosen Ultraschallsonden ist, die jeweils ein Funkgerät aufweisen,
wobei das Lokalisieren das Lokalisieren der mehreren drahtlosen Ultraschallsonden (10) innerhalb der vorbestimmten Reichweite des mobilen Ultraschallsystems (50) umfasst;
wobei das Bestimmen das Bestimmen bei dem mobilen Ultraschallsystem umfasst, dass jede der drahtlosen Ultraschallsonden innerhalb der vorbestimmten Reichweite vorhanden ist;
wobei das Verfahren ferner die folgenden Schritte umfasst:

Empfangen eines eindeutigen Identifikationssignals von jeder der drahtlosen Ultraschallsonden mit dem Funkgerät des mobilen Ultraschallsystems; und
Anzeigen der Identitäten der drahtlosen Ultraschallsonden in Übereinstimmung mit den eindeutigen Identifikationssignalen auf einer Anzeige des mobilen Ultraschallsystems; und
wobei das Paaren einer bestimmten drahtlosen Ultraschallsonde und des mobilen Ultraschallsystems das Auswählen der angezeigten Identität der bestimmten drahtlosen Ultraschallsonde umfasst.

13. Verfahren nach Anspruch 12, wobei das Anzeigen ferner das Anzeigen der Identitäten der drahtlosen Ultraschallsonden (10) in der Reihenfolge der Stärke der von den Sonden empfangenen Signale umfasst.

14. Verfahren nach Anspruch 12, wobei das Anzeigen ferner das Anzeigen der Identität einer drahtlosen Ultraschallsonde (10) nur dann umfasst, wenn sie sich innerhalb eines vorbestimmten Abstands von dem mobilen Ultraschallsystem (50) befindet; und wobei das Paaren ferner das Auswählen der angezeigten drahtlosen Ultraschallsonde zur Paarung umfasst.

15. Verfahren nach Anspruch 12, ferner umfassend das Aufrechterhalten einer durch die Paarung hergestellten Kommunikationsverbindung, bis:

der Benutzer sie bejahend beendet; oder
die bestimmte drahtlose Ultraschallsonde ausgeschaltet ist; oder
die bestimmte drahtlose Ultraschallsonde (10) über einen langen Zeitraum außerhalb der Reichweite des mobilen Ultraschallsystems (50) war; oder
die Kommunikation neuer Daten über die Verbindung für einen voreingestellten Zeitraum inaktiv war.

Revendications

1. Procédé pour coupler une sonde à ultrasons sans fil (10) à un système à ultrasons mobile (50) ayant une radio comprenant:

localiser une sonde à ultrasons sans fil (10) avec une radio dans une portée prédéterminée d'un système à ultrasons mobile (50) avec une radio; déterminer, dans le système à ultrasons mobile, que la sonde à ultrasons sans fil est présente dans la portée prédéterminée; et coupler la sonde à ultrasons sans fil et le système à ultrasons mobile pour être en communication l'un avec l'autre lorsqu'il est déterminé que la sonde à ultrasons sans fil est présente dans la portée prédéterminée et lorsqu'il est déterminé que le système à ultrasons mobile n'est pas en communication avec une autre sonde à ultrasons sans fil.

2. Procédé selon la revendication 1, dans lequel la portée prédéterminée comprend un mètre.

3. Procédé selon la revendication 2, dans lequel la portée prédéterminée est une distance d'un mètre d'une antenne (54) de la radio du système à ultrasons mobile.

4. Procédé selon la revendication 1, dans lequel la radio du système à ultrasons et la radio de la sonde sans fil sont toutes deux des émetteurs-récepteurs à bande ultra large.

5. Procédé selon la revendication 1, dans lequel la radio du système à ultrasons et la radio de la sonde sans fil sont toutes deux des émetteurs-récepteurs standard WiFi (802.11).

6. Procédé selon la revendication 1, dans lequel déterminer si la sonde à ultrasons sans fil (10) est présente dans la portée prédéterminée comprend en

autre la réception avec la radio du système à ultrasons d'un signal radio provenant de la sonde sans fil et la production d'un signal indiquant la force du signal reçu.

7. Procédé selon la revendication 6, dans lequel la production d'un signal comprend la production d'un signal indicateur de force du signal reçu par la radio du système à ultrasons.

8. Procédé selon la revendication 6, dans lequel déterminer si la sonde à ultrasons sans fil (10) est présente dans la portée prédéterminée comprend en outre la comparaison du signal indiquant la force du signal reçu à une tension de seuil.

9. Procédé selon la revendication 8, dans lequel la tension de seuil est configurée pour être égale au signal indiquant la force du signal reçu lorsque la sonde sans fil (10) est dans la portée prédéterminée du système à ultrasons (50).

10. Procédé selon la revendication 1, comprenant en outre le maintien d'une liaison de communication établie par l'appariement jusqu'à ce que:

l'utilisateur y mette fin de manière affirmative; ou la sonde à ultrasons sans fil (10) est éteinte; ou la sonde à ultrasons sans fil a été hors de portée du système à ultrasons mobile pendant un certain période de temps; ou la communication de nouvelles données sur la liaison a été inactive pendant une période de temps prédéfinie.

11. Procédé selon la revendication 1, comprenant en outre:

réaliser un examen par ultrasons avec la sonde à ultrasons sans fil appariée (10) et le système à ultrasons mobile (50); suspendre l'examen par ultrasons; et actionner une commande utilisateur du système à ultrasons mobile pour maintenir la communication appariée pendant la suspension de l'examen à ultrasons.

12. Procédé selon la revendication 1, dans lequel la sonde à ultrasons sans fil (10) est l'une d'une pluralité de sondes à ultrasons sans fil, chacune ayant une radio, dans lequel la localisation comprend le positionnement de la pluralité de sondes à ultrasons sans fil (10) dans la portée prédéterminée du système à ultrasons mobile (50); dans lequel la détermination comprend déterminer, dans le système à ultrasons mobile, que chacune des sondes à ultrasons sans fil est présente dans la

portée prédéterminée;

dans lequel le procédé comprend en outre les étapes de:

5 recevoir, avec la radio du système à ultrasons mobile, un signal d'identification unique provenant de chacune des sondes à ultrasons sans fil; et

10 afficher sur un afficheur du système à ultrasons mobile les identités des sondes à ultrasons sans fil en correspondance avec les signaux d'identification uniques; et

15 dans lequel l'appariement d'une sonde à ultrasons sans fil particulière et du système à ultrasons mobile comprend la sélection de l'identité affichée de la sonde à ultrasons sans fil particulière.

20 13. Procédé selon la revendication 12, dans lequel l'affichage comprend en outre l'affichage des identités des sondes à ultrasons sans fil (10) dans l'ordre de la force des signaux reçus des sondes.

25 14. Procédé selon la revendication 12, dans lequel l'affichage comprend en outre l'affichage de l'identité d'une sonde à ultrasons sans fil (10) uniquement si elle se trouve à une distance prédéterminée du système à ultrasons mobile (50); et dans lequel l'appariement comprend en outre la sélection de la sonde à ultrasons sans fil affichée pour l'appariement.

35 15. Procédé selon la revendication 12, comprenant en outre le maintien d'une liaison de communication établie par l'appariement jusqu'à ce que:

l'utilisateur y mette fin de manière affirmative; ou la sonde à ultrasons sans fil particulière est éteinte; ou la sonde à ultrasons sans fil particulière (10) a été hors de portée du système à ultrasons mobile (50) pendant une longue période de temps; ou la communication de nouvelles données sur la liaison a été inactive pendant une période de temps prédéfinie.

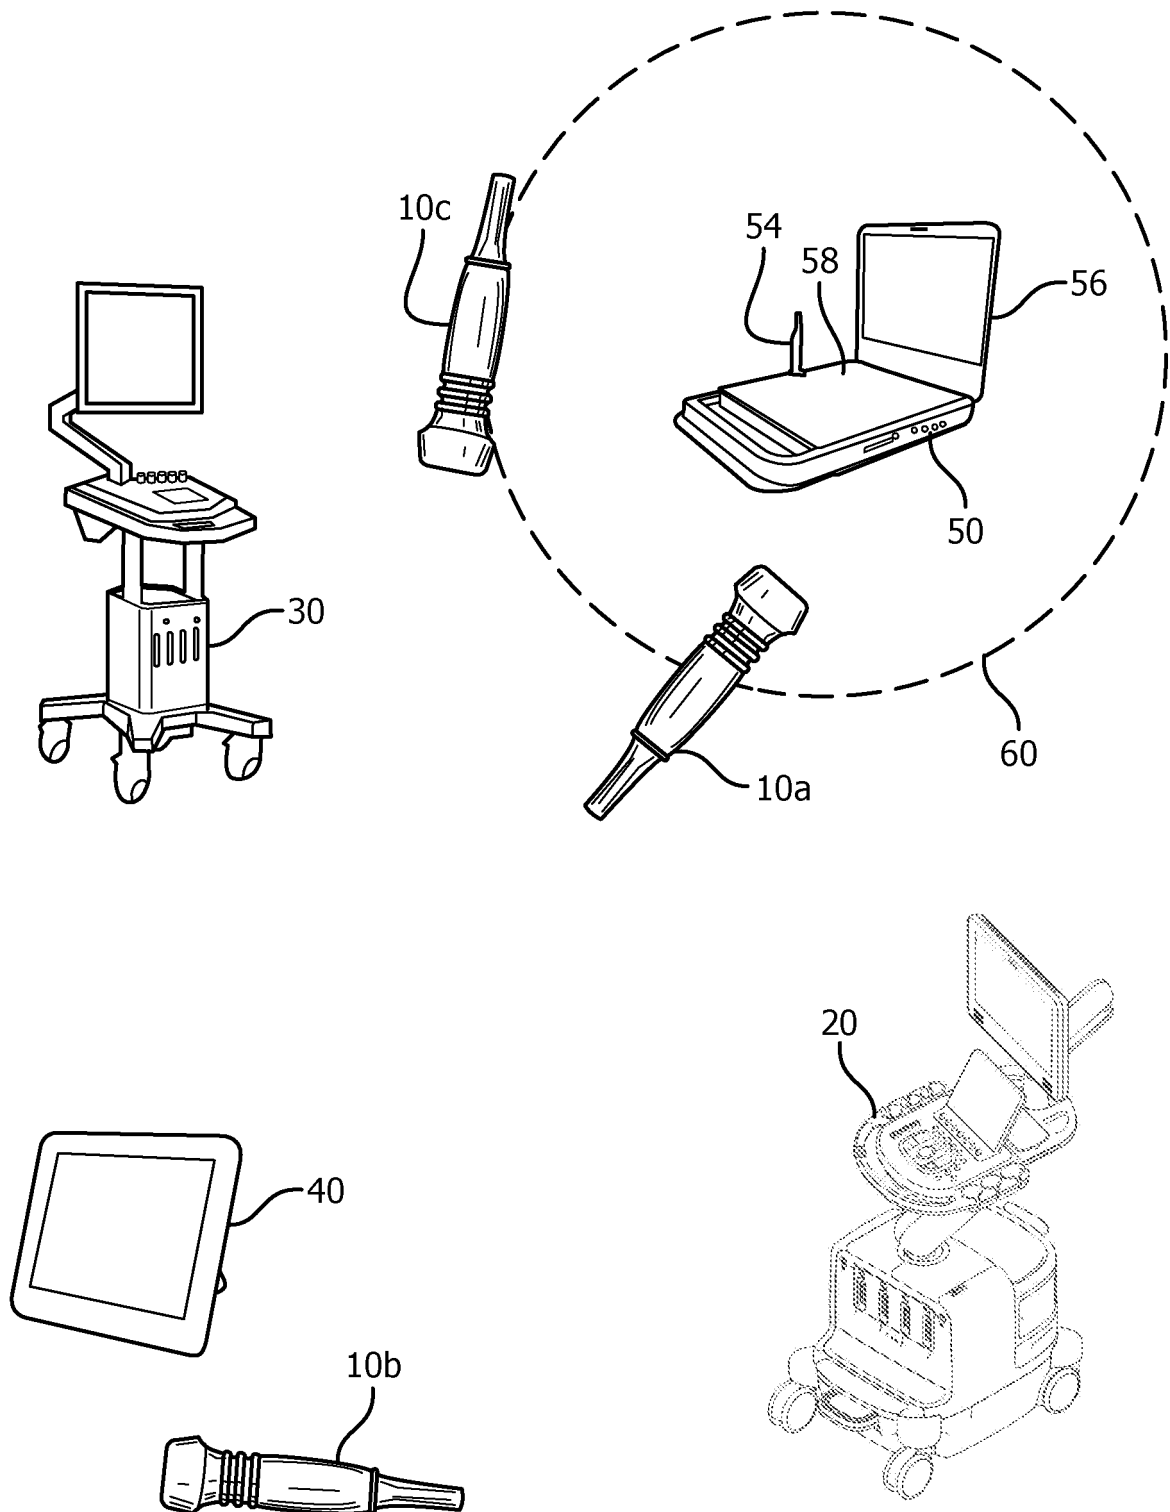


FIG. 1

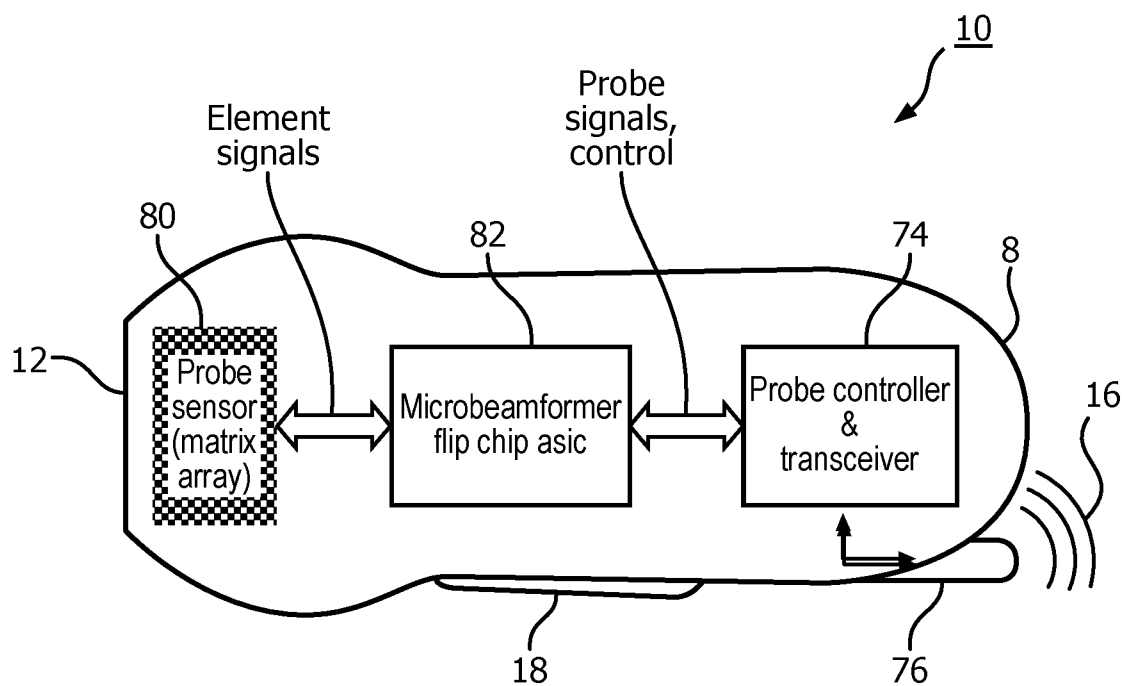


FIG. 2

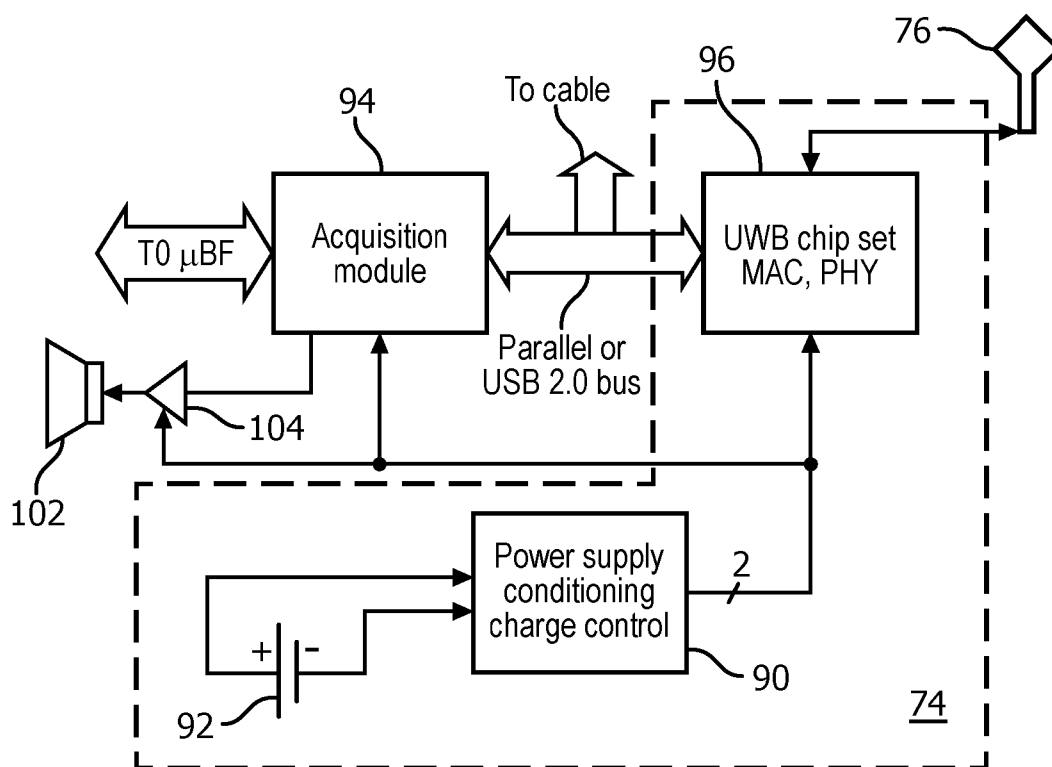


FIG. 3

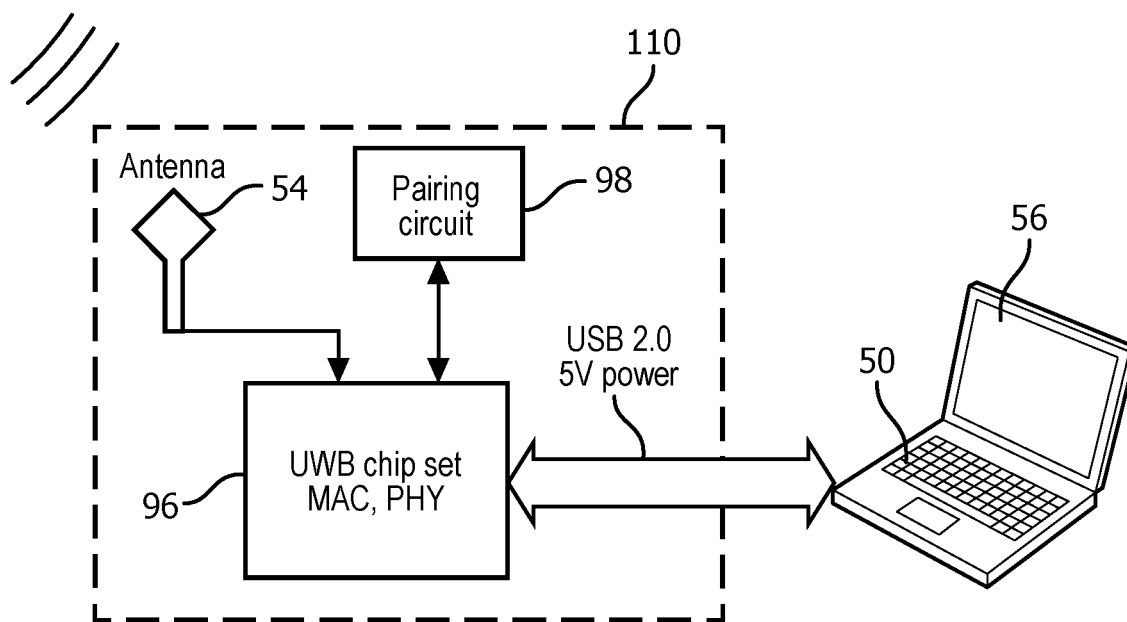


FIG. 4a

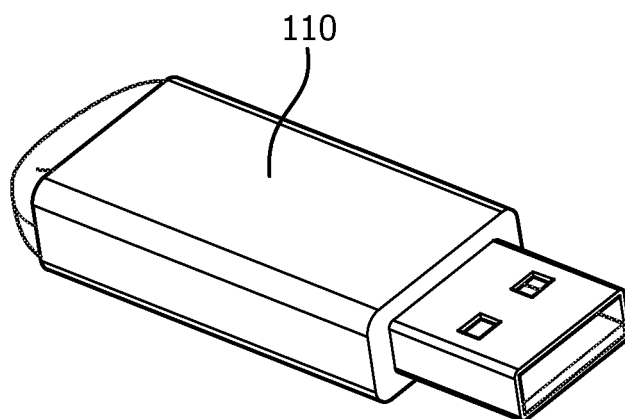


FIG. 4b

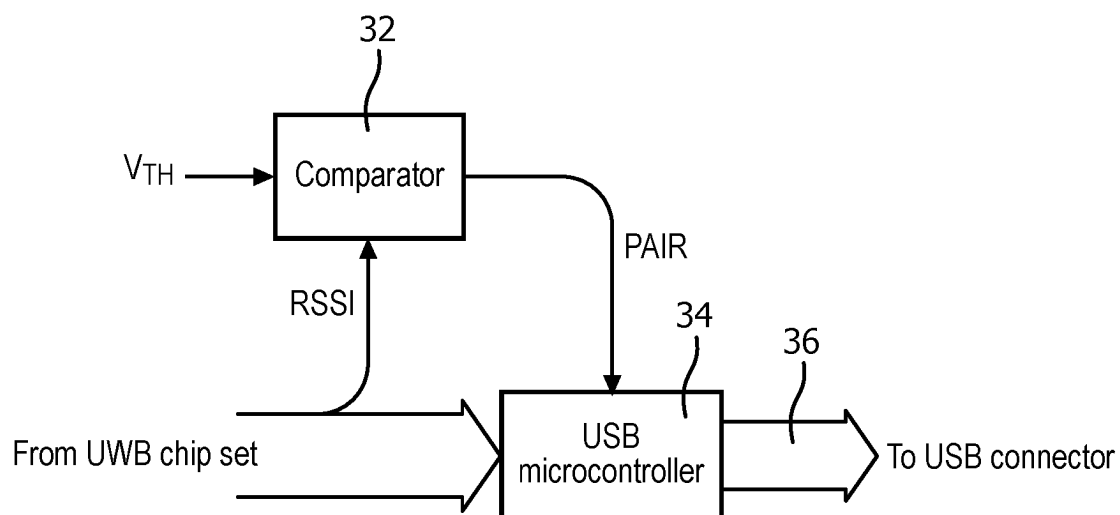


FIG. 5

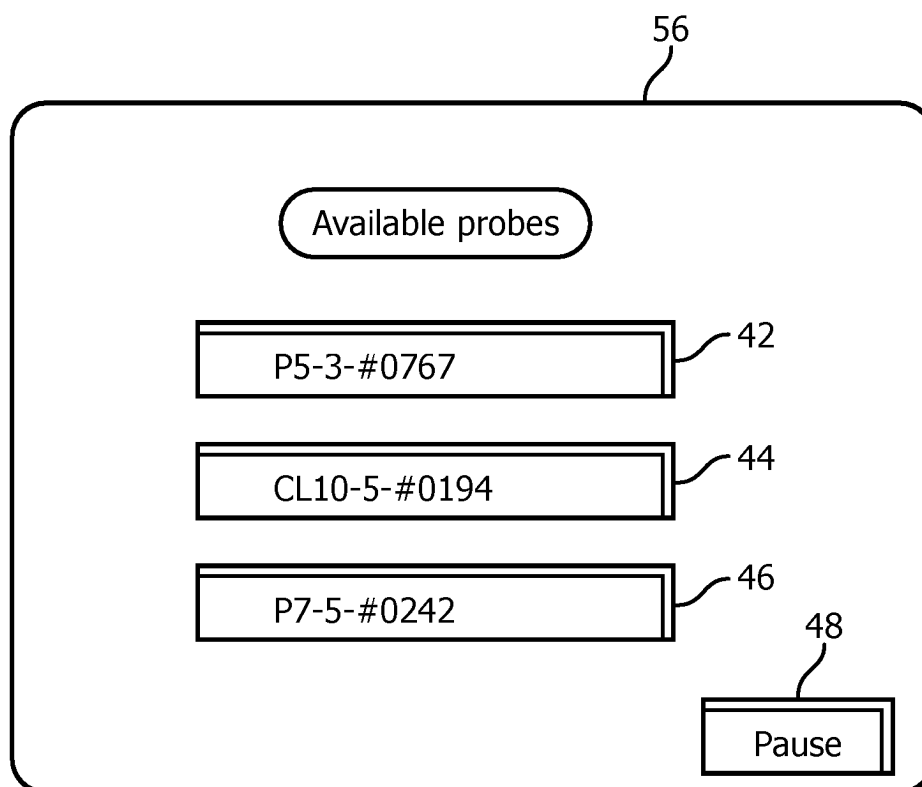


FIG. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6142946 A, Hwang [0002] [0021]
- US 8656783 B, Randall [0003] [0007]
- US 2013245451 A [0005]
- US 2014180110 A [0006]
- US 2008114241 A [0007]
- US 5229933 A, Larson III [0021]
- US 6375617 B, Fraser [0021]
- US 5997479 A, Savord [0021]
- WO 2004051882 A [0022]
- US 20100168576 A, Poland [0027]

专利名称(译)	移动超声系统的无线超声探头配对		
公开(公告)号	EP3322344B1	公开(公告)日	2020-05-20
申请号	EP2016738226	申请日	2016-07-04
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	BELL KRISTY POLAND MCKEE DUNN HUNT ALEXANDER		
发明人	BELL, KRISTY POLAND, MCKEE DUNN HUNT, ALEXANDER		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4411 A61B8/4427 A61B8/4472 G01S7/003 G01S7/52		
优先权	62/193210 2015-07-16 US		
其他公开文献	EP3322344A1		
外部链接	Espacenet		

摘要(译)

当将无线探头置于移动超声系统的预定距离内时，移动超声系统将无线超声探头配对，以便在两者之间进行排他性通信以进行超声检查。超声系统确定无线探针与系统从无线探针接收的信号的范围在预定距离内。当无线探头在预定距离内时，或者在用户启动控件以启动配对后，配对会自动进行。超声系统可以在系统的显示器上显示范围内的探针的标识，以供用户选择，从而用户将确信将与期望的无线探针进行配对。

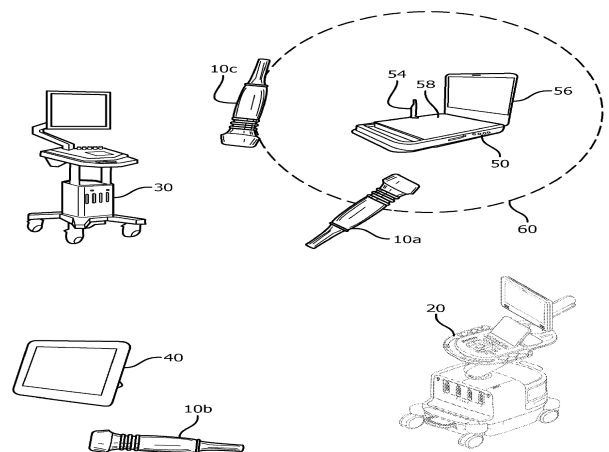


FIG. 1