



(11) **EP 1 627 602 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
25.04.2012 Bulletin 2012/17

(51) Int Cl.:
A61B 8/06 ^(2006.01) **G01S 7/52** ^(2006.01)
G01S 15/89 ^(2006.01)

(21) Application number: **04735519.3**

(86) International application number:
PCT/JP2004/007852

(22) Date of filing: **31.05.2004**

(87) International publication number:
WO 2004/105614 (09.12.2004 Gazette 2004/50)

(54) **ULTRASONOGRAPHIC DEVICE AND ULTRASONOGRAPHIC DEVICE DATA PROCESSING METHOD**

ULTRASCHALLGERÄT UND VERFAHREN ZUM VERARBEITEN VON DATEN DES
ULTRASCHALLGERÄTS

DISPOSITIF ULTRASONOGRAPHIQUE ET PROCEDE DE TRAITEMENT DE DONNEES DUDIT
DISPOSITIF ULTRASONOGRAPHIQUE

(84) Designated Contracting States:
DE FR GB

(30) Priority: **29.05.2003 JP 2003152958**

(43) Date of publication of application:
22.02.2006 Bulletin 2006/08

(73) Proprietor: **Olympus Corporation**
Tokyo 151-0072 (JP)

(72) Inventor: **MIYAKI, Hironaka,**
Olympus Corporation
Tokyo 151-0072 (JP)

(74) Representative: **von Hellfeld, Axel**
Wuesthoff & Wuesthoff
Patent- und Rechtsanwälte
Schweigerstrasse 2
81541 München (DE)

(56) References cited:
EP-A1- 0 312 059 JP-A- 5 212 032
JP-A- 11 056 847 JP-A- 2001 137 242
JP-A- 2001 276 076 US-A- 4 799 490

- "Signal Processing for Colour Flow Imaging" In: Evans D: "Doppler Ultrasound: Physics, Instrumentation and Signal Processing", 2000, John Wiley & Sons, Ltd., Chichester, XP007916986, ISBN: 978-0-471-97001-9 pages 245-263, * page 245, right-hand column, line 33 - page 246, left-hand column, line 8 * * page 255, left-hand column, line 19 - line 37 *
- KASAI C ET AL: "REAL-TIME TWO-DIMENSIONAL BLOOD FLOW IMAGING USING ULTRASOUND DOPPLER", JAPANESE JOURNAL OF APPLIED PHYSICS, JAPAN SOCIETY OF APPLIED PHYSICS, JP, vol. 26, no. SUPPL. 26-1, 1 January 1987 (1987-01-01), pages 9-13, XP000037227, ISSN: 0021-4922, DOI: DOI: 10.1143/JJAP.26.671

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 627 602 B1

Description

Technical Field

[0001] The present invention relates to a data processing method for an ultrasonic diagnostic apparatus, for obtaining tomograms inside a living body by transmitting/receiving ultrasonic waves to/from a living body tissue, and to the ultrasonic diagnostic apparatus.

Background Art

[0002] Hitherto, various ultrasonic diagnostic apparatuses for obtaining tomograms of a living body tissue by transmitting/receiving ultrasonic waves between an ultrasonic transducer and the living body tissue, have been put into actual use.

[0003] Regarding this type of ultrasonic diagnostic apparatuses, the power Doppler processing has been known as one of the methods for sensitively displaying the presence/absence of a blood flow in the living body tissue using ultrasonic waves. As an example of ultrasonic diagnostic apparatus performing this power Doppler processing, an ultrasonic diagnostic apparatus is known to apply quadrature detection to received reflected echo signals, and that, after having passing the detection signals through moving target indicator (MTI) filters, determines a blood flow power by obtaining a squared sum of an I signal and a Q signal, thereby displaying it as an two-dimensional image (for example, see Japanese Unexamined Patent Application Publication No. 61-257631 (pp. 2 to 4, and Figs. 1 to 5)).

[0004] The above-described MTI filters each operates on the principle of the moving target indicator (MTI) radar, and chiefly uses a low-order indefinite impulse response (IIR).

[0005] US 4,799,490 discloses to transmit two ultrasonic waves having different repetition periods in the same direction into an object of observation at different times, and to calculate a sum or a difference between a first velocity signal obtained from a first of the two ultrasonic transmission waves and a second velocity signal obtained from a second of the two ultrasonic transmission waves, the second transmission wave being transmitted after the first transmission wave. In another embodiment, two ultrasonic waves having different repetition periods are transmitted into an observation site. Received signals are mixed with complex reference signals which are 90 degrees out of phase, resulting in two signals having a frequency equal to the sum of the frequencies of the received signal and another having a frequency equal to a difference between the two frequencies. The signal is filtered to pass only the difference frequency component. Then, a difference between a first resulting signal and a second resulting signal having one time period delay between them is calculated, in order to remove the influence of a detected object moving at a low speed and to eliminate clutter. A difference value from a first period is multiplied by a complex conjugate of a difference value from a second period, and the resulting signal is averaged to eliminate noise components.

[0006] "Signal Processing for Colour Flow Imaging", Evans D: "Doppler Ultrasound: Physics, Instrumentation and Signal Processing", 2000, John Wiley & Sons., Ltd., Chichester, XP 007916986, ISBN; 978-0-471-97001-9, pages 245-263, discloses converting ultrasonic response data to a color coded display according to the amplitude of the signal, and threshold processing which assigns grey pixels to data above or below a corresponding threshold value related to solid tissue and noise from data.

[0007] The object of the present invention is to provide a data processing method for an ultrasonic diagnostic apparatus and the ultrasonic diagnostic apparatus, capable of performing blood flow visualization as well as improving the effectiveness for inhibiting the noise.

Disclosure of Invention

[0008] A data processing method for an ultrasonic diagnostic apparatus, according to independent claim 1 is provided.

[0009] An ultrasonic diagnostic apparatus according to independent claim 6 is provided.

Brief Description of the Drawings

[0010]

Fig. 1 is a block diagram of the overall construction of an ultrasonic diagnostic apparatus according to a first embodiment of the present invention.

Fig. 2 is a flowchart showing a data processing method for the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 3 is a timing chart showing operations of a first autocorrelation calculating section in the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 4 is a timing chart showing operations of a second autocorrelation calculating section in the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 5 is a representation of the relationship between the autocorrelation amplitude value and the white noise in the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 6 is a flowchart more specifically showing a data processing method for an ultrasonic diagnostic apparatus, in the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 7 is a flowchart showing in detail a step S15 in Fig. 6, in the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 8 is a flowchart showing in detail a step S16 in Fig. 6, in the ultrasonic diagnostic apparatus according to the first embodiment.

Fig. 9 is a block diagram of the overall construction of an ultrasonic diagnostic apparatus according to a second embodiment of the present invention.

Fig. 10 is a flowchart showing a data processing method for the ultrasonic diagnostic apparatus according to the second embodiment.

Fig. 11 is a flowchart more specifically showing the data processing method for the ultrasonic diagnostic apparatus according to the second embodiment.

Fig. 12 is a block diagram of the overall construction of an ultrasonic diagnostic apparatus according to a third embodiment.

Fig. 13 is a flowchart specifically showing a data processing method for the ultrasonic diagnostic apparatus according to the third embodiment.

Best Mode for Carrying Out the Invention

[0011] Hereinafter, embodiments according to the present invention will be described with reference to the drawings.

First Embodiment

[Construction]

[0012] Figs. 1 to 8 show an ultrasonic diagnostic apparatus according to a first embodiment of the present invention.

[0013] As shown in Fig. 1, the ultrasonic diagnostic apparatus 1 comprises an ultrasonic probe 11; an ultrasonic transmission/reception section 12; an analog/digital converter (hereinafter referred to as "A/D converter") 13; an orthogonal transformer 14; a delay device 15; MTI filters 16 and 17; first and second autocorrelation calculating sections 18 and 19; a multiplier 20; a B-mode image calculation section 21; a digital scan converter (hereinafter referred to as "DSC") 22; and a monitor 23.

[0014] The ultrasonic probe 11 is connected to the ultrasonic transmission/reception section 12, and performs the transmission/reception of ultrasonic waves.

[0015] Here, the ultrasonic probe 11 may include an array transducer for performing electric scanning, and a single plate or array transducer for performing mechanical scanning.

[0016] The ultrasonic transmission/reception section 12 supplies pulse signals to the ultrasonic probe 11. Upon receipt of the pulse signals from the ultrasonic transmission/reception section 12, the ultrasonic probe 11 transmits ultrasonic pulses, and receives echoes reflected from the living body.

[0017] Here, when the array transducer is used as the ultrasonic probe 11, the ultrasonic transmission/reception section 12 performs beam forming processing to generate sound ray data.

[0018] When attempting to acquire blood flow information, the ultrasonic transmission/reception section 12 operates in a manner such as to perform a plurality of transmitting/receiving operations in the same sound ray direction and at predetermined time intervals. In the first embodiment according to the present invention, the number of times that transmitting/receiving operations are performed in the same sound ray direction is on the order of six. In each of the sound rays, pieces of data corresponding to the same predetermined depth are acquired by the number of times of the transmitting/receiving operations are performed on the same sound ray.

[0019] The sound ray data generated in the ultrasonic transmission/reception section 12 is inputted into the A/D converter 13, and converted into digital data at a predetermined sampling frequency. Between the ultrasonic transmission/reception section 12 and the A/D converter 13, there is provided an anti-aliasing filter (not shown), which performs the function of preventing aliasing when the sound ray data is subjected to A/D conversion.

[0020] Here, the term "aliasing" refers to the phenomenon in which, when an analog signal is subjected to A/D conversion, a pseudo signal at a different frequency from the original signal occurs. Specifically, the aliasing occurs when a signal at a frequency exceeding a half a sampling frequency of the A/D converter is inputted into the A/D converter. For example, in the A/D converter at a frequency of 4 MHz, the inputting of a signal at a frequency higher than 2 MHz

causes aliasing. With this being the situation, in this first embodiment, an anti-aliasing filter (low-pass filter) for cutting off frequency components exceeding a half the sampling frequency, is provided at the pre-stage of the A/D converter 13.

[0021] The orthogonal transformer 14 is connected to the A/D converter 13. This orthogonal transformer 14 is a section for perform an orthogonal transform, and comprises a Hilbert transform filter. The orthogonal transformer 14 has the function of delaying the phase of an inputted signal by 90 degrees. The Hilbert transform filter can be made by a digital FIR filter having a predetermined filter coefficient.

[0022] The delay device 15 has the function of providing a delay equivalent to data delay amount generated in the orthogonal transformer 14. Output data from the orthogonal transformer 14 and delay device 15 constitute paired signals having a phase difference of 90 degrees with each other.

[0023] The MTI filters 16 and 17 are each a high-pass filter for removing, from the orthogonal transformer 14 and delay device 15, slow Doppler signals from a tissue except for blood flows, and are each constituted of a digital IIR filter. The filter coefficient of this digital IIR filter can be arbitrarily set from an external input section (not shown).

[0024] The first and second autocorrelation calculating sections 18 and 19 are each a section for performing data processing, which characterizes the present invention. With respect to outputs from the MTI filters 16 and 17, respectively, the first and second autocorrelation calculating sections 18 and 19 acquire respective autocorrelation amplitude values of delay times different from each other, and thereby perform calculation processing for calculating blood flow information data, to output the calculated results to the multiplier 20.

[0025] The multiplier 20 multiplies a first blood flow information data by a second blood flow information data outputted from the first and second autocorrelation calculating sections 18 and 19, respectively, and then outputs the multiplied blood flow information data.

[0026] The B-mode image calculation section 21 is a section for generating B-mode image data based on output data from the orthogonal transformer 14 and delay device 15. The output data from the orthogonal transformer 14 and delay device 15 are in an orthogonal relationship with respect to each other. Calculating the square root of squared sum of the output data from the orthogonal transformer 14 and delay device 15 allows amplitude information on reflected echoes to be obtained. The obtained amplitude information is subjected to processing such as logarithmic compression, gain adjustment, and contrast adjustment, resulting in B-mode image data.

[0027] Based on the multiplied blood flow information data calculated in the multiplier 20, and the B-mode image data calculated in the B-mode image calculation section 21, the DSC 22 performs a coordinate conversion and interpolation processing in conformance with the scan form of the ultrasonic probe 11, and thereby generates ultrasonic image data formed by synthesizing the multiplied blood flow information data and the B-mode image data.

[0028] Here, for example, when a convex probe with a curvature of 6 mm and an angle of view of 180 degrees, is used as the ultrasonic probe 11, two-dimensional sound ray data arranged in a radial shape from the center of a semicircle is obtained. The two-dimensional sound ray data is data in the form of polar coordinates (r, θ), which are defined by the distance from the center of a circle and the angle of a sound ray. In this case, as processing for a coordinate conversion, the DSC 22 converts data on polar coordinates into Cartesian coordinates (x, y coordinates), which is suitable for monitor display. Specifically, using the following relational expressions (1) and (2), the conversion between the polar coordinates (r, θ) and Cartesian coordinates (x, y) is performed.

$$x = r \times \cos \theta \dots (1)$$

$$y = r \times \sin \theta \dots (2)$$

[0029] At this time, if the density of sound rays is low, gaps occur between pieces of data, and hence the DSC 22 derives data from surrounding data by interpolation processing. For example, the DSC 22 performs four-point interpolation, in which surrounding four points are utilized for interpolation.

[0030] The monitor 23 image displays ultrasonic image data generated by the DSC 22.

[Operation]

[0031] Hereinafter, operations of the ultrasonic diagnostic apparatus according to the first embodiment will be explained with reference to Figs. 2 to 5. Here, these operations are described as observation operations by the ultrasonic diagnostic apparatus.

[0032] First, in step S1 shown in Fig. 2, the ultrasonic probe 11 and ultrasonic transmission/reception section 12 perform a plurality of times of ultrasonic transmitting/receiving operations in the same sound ray direction and at prede-

terminated time periods, and obtains a plurality of pieces of ultrasonic data. Thereby, in each sound ray, pieces of data corresponding to the same predetermined depth are acquired by the number of times that the transmitting/receiving operations are performed.

[0033] Next, in step S2 shown in Fig. 2, the ultrasonic transmission/reception section 12 extracts data corresponding to the same predetermined depth, out of the plurality of pieces of ultrasonic data obtained in step S1.

[0034] In such processes in steps S1 and S2, for example, when six times of transmitting/receiving operations are repeated in the same sound ray direction, the same predetermined pieces of data are obtained by six.

[0035] Then, in step S3 shown in Fig. 2, the ultrasonic diagnostic apparatus 1 outputs data to MTI filters 16 and 17 through the orthogonal transformer 14 and delay device 15. Thereby, the MTI filters 16 and 17 output echo data.

[0036] Hereinafter, descriptions are made of the calculation inside the first autocorrelation calculating section 18 in step S4 shown in Fig. 2, and that inside the second autocorrelation calculating section 19 in step S5 shown in Fig. 2.

[0037] As described above, in each sound ray, pieces of data corresponding to the same predetermined depth are acquired by the number of times that the transmitting/receiving operations are performed. For example, when six times of transmitting/receiving operations are repeated in the same sound ray direction, pieces of data corresponding to the same predetermined depth are obtained by six, like the original data $Z(i)$ shown in Fig. 3B. The data "a" to the data "f" are complex data obtained by combining data from the MTI filter 16 as an imaginary part, and data from the MTI filter 17 as a real part. In general, the original data $Z(i)$ when N times of transmitting/receiving operations are repeated in the same sound ray direction, is represented by the following expression (3):

$$Z(i) = X(i) + jY(i) \dots (3)$$

where, i = an integer from 1 to N.

[0038] In the first autocorrelation calculating section 18, the original data $Z(i)$ is delayed by M clocks of the clock signal CLK shown in Fig. 3A, and this delayed data is assumed to be delayed data $Z_M(i)$ shown in Fig. 3C. Here, M is an arbitrary integer from 1 to (N-1). However, if M is too large, the number of data from which vector shift data can be taken decreases, and therefore, M = about 1 to 2 is desirable.

[0039] Here, as shown in Fig. 3D, it is possible to calculate vector shift data $R_M(i)$ at each time. In general, $R_M(i)$ can be represented by the expression (4):

$$R_M(i) = Z_M(i)^* \times Z(i) \dots (4)$$

where, $*$ denotes a conjugate complex number.

[0040] In Fig. 3E, the gate pulse is a pulse having a time width equivalent to the time period during which effective data is outputted from the vector shift data $R_M(i)$.

[0041] Only for the time period during which the gate pulse is "High", the vector shift data $R_M(i)$ is integrated in an integrator (not shown) inside the first autocorrelation calculating section 18, and thereby the first autocorrelation value is calculated.

[0042] The gate pulse shown in Fig. 3E is "High" only for the time period during which the original data shown in Fig. 3B and the delayed data shown in Fig. 3C superimpose on each other, so that the vector shift data $R_M(i)$ is integrated in the integrator (not shown) only for the above-described time period. Next, the integrated value is reset to 0 before the gate pulse becomes "High".

[0043] Considering based on data examples shown in Figs. 3A to 3E, the first autocorrelation value R_M corresponding to the first autocorrelation data shown in Fig. 3D is represented by the following expression (5):

$$R_M = ca^* + db^* + ec^* + fd^* \dots (5)$$

[0044] Ultimately, data having the amplitude value of the first autocorrelation value R_M , which is a complex number, is assumed to be first blood flow information data.

[0045] Likewise, in the second autocorrelation calculating section 19, the original data $Z(i)$ shown in Fig. 4B is delayed by K clocks of the clock signal CLK shown in Fig. 4A, and this delayed data is assumed to be a delayed data $Z_K(i)$ shown in Fig. 4C. Here, K is an arbitrary integer from 1 to (N-1), and may take the same value as K. For the value of K, K = 1 to 2 is desirable, as well.

[0046] Here, as in Fig. 4D, the vector shift data $R_K(i)$ is generally represented by the expression (6):

$$R_K(i) = Z_K(i)^* \times Z(i) \dots (6)$$

[0047] In Fig. 4E, the gate pulse is a pulse having a time width equivalent to the time period during which effective data is outputted from the vector shift data $R_K(i)$.

[0048] In the second autocorrelation calculating section 19, an autocorrelation value is calculated in the same manner as in the first autocorrelation calculating section 18. Considering based on data examples shown in Figs. 4A to 4E, the second autocorrelation value R_K corresponding to the second autocorrelation data (shown in Fig. 4D) in the second autocorrelation calculating section 19, is represented by the following expression (7):

$$R_K = ba^* + cb^* + dc^* + ed^* + fe^* \dots (7)$$

[0049] Ultimately, data having the amplitude value of the second autocorrelation value R_K , which is a complex number, is assumed to be second blood flow information data.

[0050] Regarding white noise, commonly to the first blood flow information data and second blood flow information data, each piece of vector shift data has a random phase, so that the autocorrelation amplitude value obtained by adding all pieces of the data approaches 0.

[0051] On the other hand, regarding the echo from a blood flow, each piece of vector shift data has substantially the same phase, so that the autocorrelation amplitude value to be obtained by adding all pieces of the data, is added in the direction of a specified phase, resulting in a larger amplitude than that of white noise. Regarding the echo from a living body tissue, each piece of vector shift data has substantially the same phase, and in addition, the amplitude of each piece of vector shift data is large, so that the autocorrelation amplitude value takes a large value.

[0052] Therefore, as shown in Fig. 5, for each of the first blood flow information data and the second blood flow information data, the region in which the autocorrelation amplitude value is small represents white noise, the region in which the autocorrelation amplitude value is large represents the echo from a living body tissue, and the region in which autocorrelation amplitude value is intermediate represents the echo from a blood flow.

[0053] In step S6 shown in Fig. 2, the first blood flow information data is multiplied by the second blood flow information data using the multiplier 20, and thereby multiplied blood flow information data is generated. By performing the multiplication by the multiplier 20, out of the multiplied blood flow information, the value taken by the white noise becomes smaller, while the value taken by the echo from a living body tissue becomes larger. As a result, mutual ratios among the white noise, echo from the blood flow, and echo from the living body tissue become larger. This facilitates the mutual discrimination among the white noise, echo from the blood flow, and echo from the living body tissue.

[0054] Consequently, DSC 22 extracts multiplied blood flow information data having a specified magnitude, and screen displays it on the monitor 23, whereby the echo from the blood flow can be exclusively displayed. For example, a threshold value B1 defining the boundary between the white noise and blood flow echo, and a threshold value B2 defining the boundary between the echo from a living body tissue and the echo from a blood flow are provided, and the DSC 22 screen displays, on the monitor 23, only data having values not less than the threshold B1 nor more than the threshold value B2, whereby the echo from the blood flow can be exclusively displayed.

[0055] The threshold values B1 and B2 are constants uniquely determined by the transmission voltage of the ultrasonic transmission/reception section 12, and the amplification factor of a reception circuit in the ultrasonic transmission/reception section 12. After having determined the actually used transmission voltage and reception circuit, the threshold values B1 and B2 are set to the respective most effective value by determining them in an experimental manner.

[0056] With respect to the multiplied blood flow information data, the DSC 22 displays the amplitude value by relating it to the luminance of a predetermined hue, or alternatively, color displays the amplitude value by relating it to the predetermined hue.

[0057] By these operations, step S1 shown in Fig. 2 constitutes an ultrasonic data acquisition step for acquiring a plurality of pieces of ultrasonic data by performing the plurality of times of ultrasonic transmitting/receiving operations in the same sound ray direction and at predetermined time intervals.

[0058] Step S2 shown in Fig. 2 constitutes a data extraction step for acquiring data corresponding to the same predetermined depth, out of the plurality of ultrasonic data acquired in the above-described step S1.

[0059] Step S3 shown in Fig. 2 constitutes a filtering step for inputting the data corresponding to the same predetermined depth, acquired in the above-described step S2, into filter means having predetermined characteristics, and extracting echo data from a moving part in a body.

[0060] Step S4 shown in Fig. 2 constitutes a first amplitude value acquisition step for acquiring the first autocorrelation amplitude value when the echo data from the moving part in the body, acquired in the above-described step S3, is delayed by a first predetermined time period.

[0061] Step S5 shown in Fig. 2 constitutes a second amplitude value acquisition step for acquiring the second autocorrelation amplitude value when the echo data from the moving part in the body, acquired in the above-described step S3, is delayed by a second predetermined time period.

[0062] Step S6 shown in Fig. 2 constitutes a colorization step for relating the multiplied value acquired by multiplying the first autocorrelation amplitude value by the second autocorrelation amplitude value, to the luminance of a predetermined hue.

[0063] Using Fig. 6, a data processing method for an ultrasonic diagnostic apparatus shown in Fig. 2 will be described as specific processing operations.

[0064] First, in step S11 shown in Fig. 6, the ultrasonic probe 11 and ultrasonic transmission/reception section 12 acquire a plurality of pieces of ultrasonic data.

[0065] Next, in step S12 shown in Fig. 6, the orthogonal transform of the plurality of pieces of ultrasonic data are performed by the orthogonal transformer 14.

[0066] Then, in step S13 shown in Fig. 6, the ultrasonic transmission/reception section 12 extracts data corresponding to the same predetermined depth, out of the plurality of pieces of ultrasonic data obtained in step S11 shown in Fig. 6.

[0067] By the processes of such steps S11, S12, and S13, pieces of data corresponding to the same predetermined depth are obtained by six, as shown in Figs. 3A to 3E and Figs. 4A to 4E.

[0068] Next, in step S14 shown in Fig. 6, the MTI filters 16 and 17 perform MTI filter calculation with respect to the data corresponding to the same predetermined depth, the data being obtained through the orthogonal transformer 14 and delay device 15, and then output echo data.

[0069] Then, in step S15 shown in Fig. 6, the first autocorrelation calculating section 18 performs first blood flow information data calculation with respect to the echo data from the MTI filters 16 and 17.

[0070] Thereafter, in step S16 shown in Fig. 6, the second autocorrelation calculating section 19 performs second blood flow information data calculation with respect to the echo data from the MTI filters 16 and 17.

[0071] Next, in step S17 shown in Fig. 6, the multiplier 20 multiplies the first blood flow information data by the second blood flow information data, thereby generating multiplied blood flow information data.

[0072] Then, in step S18 shown in Fig. 6, the DSC 22 extracts data having values not less than the threshold B1 nor more than the threshold value B2, from the multiplied blood flow information data obtained by the multiplier 20. After this, in step S19 shown in Fig. 6, the DSC 22 performs the determination as to whether all calculation object data has been completed. If the calculation has not been completed, the process returns to step S13, and if the calculation has been completed, the process transfers to step S20.

[0073] In step S20 shown in Fig. 6, the DSC 22 allocates hue and luminance to the multiplied blood flow information data extracted in step S18. Then, in step S21 shown in Fig. 6, the DSC 22 generates ultrasonic image data formed by synthesizing B-mode image data calculated in the B-mode image calculation section 21 and the above-described multiplied blood flow information data, and displays it on the monitor 23. After this, the process returns to step S11 shown in Fig. 6.

[0074] Hereinafter, the processing of step S15 will be described with reference to Fig. 7.

[0075] Steps S31 to S34 shown in Fig. 7 constitute step S15 shown in Fig. 6.

[0076] First, in step S31 shown in Fig. 7, the first autocorrelation calculating section 18 delays the original data $Z(i)$ shown in Fig. 3B by M clocks of clock signal CLK shown in Fig. 3A, thereby generating delayed data $Z_M(i)$ shown in Fig. 3C.

[0077] Next, in step S32 shown in Fig. 7, the first autocorrelation calculating section 18 performs the calculation shown in the above-described expression (4), thereby generating the vector shift data $R_M(i)$.

[0078] Then, in step S33 shown in Fig. 7, the first autocorrelation calculating section 18 integrates the vector shift data $R_M(i)$, thereby generating the first autocorrelation value R_M .

[0079] Thereafter, in step S34 shown in Fig. 7, the first autocorrelation calculating section 18 calculates the amplitude value of the first autocorrelation value R_M , thereby generating the first blood flow information data.

[0080] Hereinafter, the processing of step S16 will be described with reference to Fig. 8.

[0081] Steps S41 to S44 shown in Fig. 8 constitute step S16 shown in Fig. 6.

[0082] First, in step S41 shown in Fig. 8, the second autocorrelation calculating section 19 delays the original data $Z(i)$ shown in Fig. 4B by K clocks of the clock signal CLK shown in Fig. 4A, thereby generating delayed data $Z_K(i)$ shown in Fig. 4C.

[0083] Next, in step S42 shown in Fig. 8, the second autocorrelation calculating section 19 performs the calculation shown in the above-described expression (6), thereby generating the vector shift data $R_K(i)$.

[0084] Then, in step S43 shown in Fig. 8, the second autocorrelation calculating section 19 integrates the vector shift data $R_K(i)$, thereby generating the second autocorrelation value R_K .

[0085] Thereafter, in step S44 shown in Fig. 8, the second autocorrelation calculating section 19 calculates the am-

plitude value of the second autocorrelation value R_K , thereby generating the second blood flow information data.

[Advantages]

[0086] When the blood information data is simply taken as a power value, the white noise also exhibits a certain level of value, whereas the white noise in the multiplied blood flow information data outputted by the multiplier 20 approaches 0. As a result, as compared with the conventional method for displaying blood flow power, the data processing method for the ultrasonic diagnostic apparatus according to the first embodiment increases the ratio between the blood flow signal and white noise. In other words, the data processing method for the ultrasonic diagnostic apparatus according to this embodiment is superior in the effect of inhibiting white noise.

[0087] Thereby, the ultrasonic diagnostic apparatus according to the first embodiment is capable of implementing blood flow visualization and improving the effectiveness for inhibiting the noise, thereby enabling more correct detection of blood flow information.

Second Embodiment

[0088] Figs. 9 to 11 show an ultrasonic diagnostic apparatus according to a second embodiment of the present invention.

[0089] In Figs. 9 to 11, same components are denoted by the same symbols as those in the ultrasonic diagnostic apparatus of the above-described first embodiment shown in Figs. 1 to 8, and detailed descriptions of these components will be omitted here.

[Construction]

[0090] As shown in Fig. 9, the ultrasonic diagnostic apparatus 2 according to the second embodiment of the present invention has an averaging processor 30 instead of the multiplier 20 in the above-described ultrasonic diagnostic apparatus according to the first embodiment.

[0091] This averaging processor 30 outputs average blood flow information data obtained by averaging amplitude values of the first blood flow information data and second blood flow information data, outputted by the first and second autocorrelation calculating sections 18 and 19, respectively.

[0092] Based on the average blood flow information data calculated in the averaging processor and the B-mode image data calculated in the B-mode image calculation section 21, the DSC 22 performs a coordinate conversion and interpolation processing in conformance with the scan form of the ultrasonic probe 11, and thereby generates ultrasonic image data by synthesizing the average blood flow information data and B-mode image data.

[Operation]

[0093] As shown in Fig. 10, instead of the processing of step S6 in the first embodiment, the ultrasonic diagnostic apparatus 2 according to the second embodiment uses a colorization step shown in step S56 for relating the average value obtained by averaging the first and second autocorrelation amplitude values, to the luminance of a predetermined hue.

[0094] Also, as shown in Fig. 11, the ultrasonic diagnostic apparatus 2 according to the second embodiment performs processing shown in step 67, instead of step 17 in the first embodiment.

[0095] In step 67, the averaging processor 30 outputs average blood flow information data by calculating the average between the first blood flow information data and second blood flow information data generated in steps 15 and 16, respectively.

[0096] As described above on the ultrasonic diagnostic apparatus according to the first embodiment, in the first blood flow information data outputted by the first autocorrelation calculating section 18, and the second blood flow information data outputted by the second autocorrelation calculating section 19, the white noise, echo from a blood flow, and echo from a living body tissue have a magnitude relationship with respect to one another, as shown in Fig. 5.

[0097] Therefore, also in the average blood flow information data obtained by averaging the first blood flow information data and second blood flow information data using the averaging processor 30, the echo from a blood flow and echo from a living body tissue mutually have substantially the same magnitude relationship as that in Fig. 5. However, regarding the white noise, the averaging produces the effectiveness for inhibiting sudden occurrences of large values thereof, so that the white noise comes to take a lower value in a stable manner.

[0098] Hence, in step S56 (corresponding to step S67 in Fig. 11), extracting and displaying average blood flow information data with a specified magnitude allows the echo from a blood flow to be exclusively displayed. For example, by providing the threshold value B1 defining the boundary between the white noise and blood flow echo, the threshold value

B2 defining the boundary between the echo from a living body tissue and the echo from a blood flow, and by displaying on screen only data having values not less than the threshold B1 nor more than the threshold value B2, it is possible to exclusively display the echo from the blood flow.

[0099] The DSC 22 displays the average blood flow information data by relating the amplitude value thereof to the luminance of a predetermined hue, or alternatively, color displays the average blood flow information data by relating the amplitude value thereof to the predetermined hue.

[Advantages]

[0100] When the blood information data is simply taken as a power value, the white noise also exhibits a certain level of value, whereas the white noise in the average blood flow information data from the averaging processor 30 approaches 0. As a result, as in the case of the ultrasonic diagnostic apparatus according to the first embodiment, the ultrasonic diagnostic apparatus according to the second embodiment is capable of visualizing blood flow as well as enhancing the effectiveness for inhibiting the noise, thereby allowing more correct detection of blood flow information.

[0101] Also, regarding the white noise, the ultrasonic diagnostic apparatus according to the second embodiment has the effectiveness for inhibiting sudden occurrences of large values thereof, thereby enabling more stable detection of blood flow information.

Third Embodiment

[0102] Figs. 12 and 13 show an ultrasonic diagnostic apparatus according to a third embodiment of the present invention.

[0103] In Figs. 12 and 13, same components are denoted by the same symbols as those in the ultrasonic diagnostic apparatus of the above-described first embodiment shown in Figs. 1 to 8, and second embodiment shown in Figs. 9 to 11, and detailed descriptions of these components will be omitted here.

[Construction]

[0104] As shown in Fig. 12, as compared with the above-described ultrasonic diagnostic apparatus according to the second embodiment, the ultrasonic diagnostic apparatus according to the third embodiment of the present invention further has a blood flow image calculation section 40 provided at the post-stage of the averaging processor 30.

[0105] This blood flow image calculation section 40 inputs the first autocorrelation value R_M calculated in the first autocorrelation calculating section 18, and the average blood flow information data calculated in the averaging processor 30, and outputs blood flow image data after having been subjected to a predetermined calculation.

[0106] This blood flow image data becomes either the blood flow velocity data or average blood flow information data that has been processed, depending upon an operation mode selected by an operator using an operation panel (not shown).

[0107] Also, in this embodiment, based on the blood flow image data calculated in the blood flow image calculation section 40 and the B-mode image data calculated in the B-mode image calculation section 21, the digital scan converter 22 performs a coordinate conversion and interpolation processing in conformance with the scan form of the ultrasonic probe 11, and thereby generates ultrasonic image data by synthesizing the blood flow image data and B-mode image data.

[Operation]

[0108] As shown in Fig. 13, the ultrasonic diagnostic apparatus 3 has a threshold value processing step shown in step S101, instead of step S18 in the above-described second embodiment, and further has a velocity value calculation step shown in step S100.

[0109] First, step S100 will be described below.

[0110] The velocity v of a blood flow is calculated in the blood flow image calculation section 40 by the following expression:

$$v = \{c / (4\pi f_0 T M)\} \tan^{-1}(R_{My} / R_{Mx})$$

c : velocity of sound

f_0 : center frequency of transmitted/received ultrasonic pulses

T : time interval during which transmitting/receiving operations are repeated in the same sound ray direction

M: integer defining the delay described in the above-described first embodiment

R_{Mx} : real part of autocorrelation value R_M

R_{My} : imaginary part of autocorrelation value R_M

[0111] Next, step S101 will be described.

[0112] First, the blood flow image calculation section 40 calculates blood flow velocity data by performing the following threshold value processing. The average blood flow information data is compared with the threshold values B1 and B2, and if the average blood flow information data is not less than the threshold value B1 nor more than the threshold value B2, it can be determined that this average blood flow information data corresponds to the echo from a blood flow, and hence, the blood flow information data is assumed to be the value itself of the velocity v .

[0113] If the average blood flow information data is less than the threshold value B1, or more than the threshold value B2, it is determined that this average blood flow information data does not correspond to the echo from a blood flow, and the blood flow information data is replaced with zero. Generally, when the blood flow information data is zero, no color display is performed, and therefore, it is possible to exclusively display in color the velocity value of the echo from the blood flow.

[0114] The blood flow image calculation section 40 determines the average blood flow information data that has been processed, using the following procedures:

[0115] The absolute value of the velocity v of a blood flow is compared with a predetermined threshold value v_0 , and if the absolute value of the velocity v of the blood flow is larger than the threshold value v_0 , it is determined that this average blood flow information data corresponds to the echo from the blood flow, and the average blood flow information data that has been processed is assumed to be the average blood flow information data itself. If the absolute value of the velocity v of blood flow is smaller than the threshold value v_0 , it is determined that the average blood flow information data corresponds to the echo from a living body tissue, and zero is outputted as average blood flow information data that has been processed.

[0116] Generally, when the average blood flow information data that has been processed is zero, no color display is performed, and therefore it is possible to exclusively display in color average blood flow information data on the echo from a blood flow.

[0117] The blood flow image calculation section 40 outputs, as blood flow image data, either the blood flow velocity data or the average blood flow information data that has been processed, depending upon an operation mode selected by the operator using an operation panel (not shown).

[0118] The velocity value calculation step in step S100 has been described regarding the case where the first autocorrelation value R_M calculated in the first autocorrelation calculating section 18 is used. However, the second autocorrelation value R_K calculated in the second autocorrelation calculating section 19, instead of the first autocorrelation calculating section 18, may also be employed.

[0119] Also, from the above-described descriptions of the first and second embodiments, it is evident that, in the third embodiment, the multiplier 20 may be used instead of the averaging processor 30.

[0120] Furthermore, processing in the averaging processor 30 is not necessarily limited to simple averaging processing. The processing in the averaging processor 30 may include an average that has been multiplied by a predetermined weight, or addition.

[0121] Moreover, each of the MTI filters in the present invention is not limited to a digital IIR filter. Each of the MTI filters in the present invention may be constituted of a digital FIR filter.

[Advantages]

[0122] When the blood flow image data is to be color displayed, by performing threshold value processing using the average blood flow information data outputted from the averaging processor 30 and the velocity value calculated in the blood flow image calculation section 40, it is possible to inhibit the color display of the white noise and echo from a living body tissue, and realize an ultrasonic diagnostic apparatus which is capable of detecting velocity information on a blood flow more correctly.

[0123] Embodiments constructed by partially combining the above-described embodiments are also subsumed under the present invention.

[0124] Furthermore, it is believed obviously that the present invention is not limited to the above-described embodiments, and that various modifications and adaptations are possible.

Industrial Applicability

[0125] As describe above, according to the present invention, it is possible to visualize blood flow and improve the effectiveness for inhibiting the noise, thereby enabling the implementation of an ultrasonic diagnostic apparatus capable of more correctly detecting blood flow information.

Cross-Reference to Related Applications

[0126] This application is based upon and claims priority from Japanese Patent Application No. 2003-152958, filed on May 29, 2003.

Claims

1. A data processing method for an ultrasonic diagnostic apparatus (1), the method comprising:

a data extraction step for acquiring a plurality of pieces of data corresponding to a same predetermined depth, out of a plurality of pieces of ultrasonic data acquired by ultrasonic transmission/reception means (12) for acquiring the plurality of pieces of ultrasonic data by performing ultrasonic transmitting/receiving operations a plurality of times in a same sound ray direction and at predetermined time intervals;

a filtering step for inputting the data corresponding to the same predetermined depth, acquired in the data extraction step, into filters (16, 17) each having a predetermined characteristic, and extracting echo data from a moving part in a body;

characterized by further comprising:

a first amplitude value acquisition step for acquiring a first autocorrelation amplitude value from the echo data from the moving part in the body, acquired in the filtering step, by multiplying the echo data from a first time period by the complex conjugate of the echo data delayed by a first predetermined time period;

a second amplitude value acquisition step for acquiring a second autocorrelation amplitude value from the echo data from the moving part in the body, acquired in the filtering step, by multiplying the echo data from the first time period by the complex conjugate of the echo data delayed by a second predetermined time period, wherein the first and second predetermined time periods are integer multiples of a common clock signal that are different from one another; and

a colorization step for relating a value to a luminance of a predetermined hue, wherein the value is one of:

a multiplied value obtained by multiplying the first autocorrelation amplitude value by the second autocorrelation amplitude value; and

an average value obtained by averaging the first and second autocorrelation amplitude values.

2. The data processing method for an ultrasonic diagnostic apparatus according to claim 1, the method further comprising an ultrasonic data acquisition step for acquiring the plurality of pieces of ultrasonic data by performing the ultrasonic transmitting/receiving operations the plurality of times in the same sound ray direction and at predetermined time intervals, wherein the moving part of the body is a moving reflector including a blood flow.

3. The data processing method for an ultrasonic diagnostic apparatus according to Claim 2, wherein the ultrasonic transmitting/receiving operations in the data acquisition step are performed using an ultrasonic probe (11).

4. The data processing method for an ultrasonic diagnostic apparatus according to Claim 2, wherein the filters are MTI filters (16, 17).

5. The data processing method for an ultrasonic diagnostic apparatus according to one of claims 1 to 4, wherein:

the value is the average value obtained by averaging the first and second autocorrelation amplitude values; and the colorization step for relating the average value obtained by averaging the first and second autocorrelation amplitude values, to the luminance of a predetermined hue comprises:

a step of acquiring a velocity value from the real part and the imaginary part of the first autocorrelation amplitude value;

a threshold value processing step for subjecting the velocity value to threshold value processing, using the average value, generating a processed velocity value; and

a colorization step for relating the processed velocity value to the luminance of the predetermined hue.

6. An ultrasonic diagnostic apparatus comprising:

ultrasonic data acquisition means (12) for acquiring a plurality of pieces of ultrasonic data by performing ultrasonic transmitting/receiving operations by an ultrasonic transducer (11) a plurality of times in a same sound ray direction and at predetermined time intervals;

data extraction means for acquiring a plurality of pieces of data corresponding to a same predetermined depth, out of a plurality of pieces of ultrasonic data acquired by the ultrasonic data acquisition means (12);

filters (16, 17) each of which has a predetermined filter characteristic, with input data corresponding to the same predetermined depth, acquired by the data extraction means, which extract echo data from a moving part in a body;

characterized by further comprising:

first amplitude value acquisition means (18) for acquiring a first autocorrelation amplitude value from the echo data from the moving part in the body, acquired by the filters (16, 17), by multiplying the echo data from a first time period by the complex conjugate of the echo data delayed by a first predetermined time period;

second amplitude value acquisition means (19) for acquiring a second autocorrelation amplitude value from the echo data from the moving part in the body, acquired by the filters (16, 17), by multiplying the echo data from the first time period by the complex conjugate of the echo data delayed by a second predetermined time period, wherein the first and second predetermined time periods are integer multiples of a common clock signal that are different from one another; and

colorization means (22) for relating a multiplied value obtained by multiplying the first autocorrelation amplitude value by the second autocorrelation amplitude value, to a luminance of a predetermined hue.

7. The ultrasonic diagnostic apparatus according to Claim 6, wherein the filters are MTI filters (16, 17).

Patentansprüche

1. Datenverarbeitungsverfahren für eine Ultraschall Diagnosevorrichtung (1), wobei das Verfahren aufweist:

einen Datenextraktionsschritt zum Erlangen einer Mehrzahl von Datenteilen, die einer selben vorbestimmten Tiefe entsprechen, aus einer Mehrzahl von Ultraschall datenteilen, die von Ultraschallsende-/empfangsmitteln (12) zum Erlangen der Mehrzahl von Ultraschall datenteilen durch mehrmaliges Ausführen von Ultraschallsende-/empfangsoperationen in einer gleichen Schallstrahlrichtung und zu vorbestimmten Zeitintervallen erlangt wurden;

einen Filterschritt zum Eingeben der Daten, die derselben vorbestimmten Tiefe entsprechen und in dem Datenextraktionsschritt erlangt wurden, in Filter (16, 17), von denen jeder eine vorbestimmte Charakteristik aufweist, und Extrahieren von Echodaten von einem sich in einem Körper bewegenden Teil;

dadurch gekennzeichnet, dass es ferner aufweist:

einen ersten Amplitudenwerterlangungsschritt zum Erlangen eines ersten Autokorrelationsamplitudenwerts aus den Echodaten von dem sich in dem Körper bewegenden Teil, die in dem Filterschritt erlangt wurde, durch Multiplizieren der Echodaten einer ersten Zeitperiode mit dem komplexen Konjugat der Echodaten verzögert um eine erste vorbestimmte Zeitperiode;

einen zweiten Amplitudenwerterlangungsschritt zum Erlangen eines zweiten Autokorrelationsamplitudenwerts aus den Echodaten von dem sich in dem Körper bewegenden Teil, die in dem Filterschritt erlangt wurden, durch Multiplizieren der Echodaten der ersten Zeitperiode mit dem komplexen Konjugat der Echodaten verzögert um eine zweite vorbestimmte Zeitperiode, wobei die ersten und zweiten vorbestimmten Zeitperioden ganzzahlige Vielfache eines gemeinsamen Taktsignals und verschieden voneinander sind; und

einen Farbgebungsschritt zum Miteinanderinverbindungbringen eines Wertes mit einer Helligkeit eines vorbestimmten Farbtönen, wobei der Wert einer ist von:

einem multiplizierten Wert, der durch Multiplikation des ersten Autokorrelationsamplitudenwerts mit dem zweiten Autokorrelationsamplitudenwert erlangt wurde; und

einem Mittelwert, der durch Mittelwertbildung der ersten und zweiten Autokorrelationsamplitudenwerte erlangt wurde.

2. Datenverarbeitungsverfahren für eine Ultraschall Diagnosevorrichtung nach Anspruch 1, wobei das Verfahren ferner

aufweist einen Ultraschalldatenerlangungsschritt zum Erlangen der Mehrzahl von Ultraschalldatenteilen durch das mehrmalige Ausführen der Ultraschallsende-/empfangsoperationen in der gleichen Schallstrahlrichtung und bei vorbestimmten Zeitintervallen,
wobei das sich in dem Körper bewegende Teil ein sich bewegendes Reflektor enthaltend ein Blutfluss ist.

3. Datenverarbeitungsvorrichtung für eine Ultraschalldiagnosevorrichtung nach Anspruch 2, bei der die Ultraschallsende-/empfangsoperationen in dem Datenerlangungsschritt unter Verwendung einer Ultraschallsonde (11) ausgeführt werden.

4. Datenverarbeitungsverfahren für eine Ultraschalldiagnosevorrichtung nach Anspruch 2, bei der die Filter MTI-Filter (16, 17) sind.

5. Datenverarbeitungsverfahren für eine Ultraschalldiagnosevorrichtung nach einem der Ansprüche 1 bis 4, bei dem:

der Wert der Mittelwert ist, der durch Mittelwertbildung der ersten und zweiten Autokorrelationsamplitudenwerte erlangt wurde; und
der Farbgebungsschritt zum Miteinanderinverbindungbringen des Mittelwerts, der durch Mittelwertbildung der ersten und zweiten Autokorrelationsamplitudenwerte erlangt wurde, mit der Helligkeit eines vorbestimmten Farbtons aufweist:

einen Schritt eines Erlangens eines Geschwindigkeitswerts von dem Realteil und dem Imaginärteil des ersten Autokorrelationsamplitudenwerts;
einen Schwellwertverarbeitungsschritt zum Unterziehen des Geschwindigkeitswerts einer Schwellwertverarbeitung, unter Verwendung des Mittelwerts, der einen verarbeiteten Geschwindigkeitswert erzeugt; und
einen Farbgebungsschritt zum Miteinanderinverbindungbringen des verarbeiteten Geschwindigkeitswerts mit der Helligkeit des vorbestimmten Farbtons.

6. Ultraschalldiagnosevorrichtung aufweisend:

Ultraschalldatenerlangungsmittel (12) zum Erlangen einer Mehrzahl von Ultraschalldatenteilen durch mehrmaliges Ausführen von Ultraschallsende/- empfangsoperationen durch einen Ultraschallwandler (11) in einer gleichen Schallstrahlrichtung und bei vorbestimmten Zeitintervallen;
Datenextraktionsmittel zum Erlangen einer Mehrzahl von Datenteilen, die einer selben vorbestimmten Tiefe entsprechen, aus einer Mehrzahl von Ultraschalldatenteilen, die durch die Ultraschalldatenerlangungsmittel (12) erlangt wurden;
Filter (16, 17), von denen jeder einer vorbestimmte Filtercharakteristik aufweist, mit Eingangsdaten, die derselben vorbestimmten Tiefe entsprechen und durch die Datenextraktionsmittel erlangt wurden, welche die Echodaten von einem sich in einem Körper bewegenden Teil extrahieren;
charakterisiert durch ferner aufweisend:

erste Amplitudenwerterlangungsmittel (18) zum Erlangen eines ersten Autokorrelationsamplitudenwerts aus den Echodaten von dem sich in dem Körper bewegenden Teil, erlangt durch die Filter (16, 17), durch Multiplizieren der Echodaten einer ersten Zeitperiode mit dem komplexen Konjugat der Echodaten verzögert um eine erste vorbestimmte Zeitperiode;
zweite Amplitudenwerterlangungsmittel (19) zum Erlangen eines zweiten Autokorrelationsamplitudenwerts aus den Echodaten von dem sich in dem Körper bewegenden Teil, erlangt durch die Filter (16, 17), durch Multiplizieren der Echodaten der ersten Zeitperiode mit dem komplexen Konjugat der Echodaten verzögert um eine zweite vorbestimmte Zeitperiode, wobei die ersten und zweite vorbestimmten Zeitperioden ganzzahlige Vielfache eines gemeinsamen Taktsignals und verschieden voneinander sind; und
Farbgebungsmittel (22) zum Miteinanderinverbindungbringen eines multiplizierten Wertes, der durch Multiplikation des ersten Autokorrelationsamplitudenwerts mit dem zweiten Autokorrelationsamplitudenwert erlangt wurde, mit einer Helligkeit eines vorbestimmten Farbtons.

7. Ultraschalldiagnosevorrichtung nach Anspruch 6, bei der die Filter MTI-Filter (16, 17) sind.

Revendications

1. Procédé de traitement de données pour un appareil de diagnostic à ultrasons (1), le procédé comprenant :

5 une étape d'extraction de données destinée à acquérir une pluralité de morceaux de données correspondant à une même profondeur prédéterminée, en dehors d'une pluralité de morceaux de données ultrasonores obtenus par un moyen d'émission/réception à ultrasons (12) destiné à obtenir la pluralité de morceaux de données ultrasonores en exécutant des opérations d'émission/réception par ultrasons une pluralité de fois dans une même direction de rayon sonore et à des intervalles de temps prédéterminés ;
 10 une étape de filtrage destinée à délivrer en entrée les données correspondant à la même profondeur prédéterminée, obtenues à l'étape d'extraction de données, dans des filtres (16, 17) possédant chacun une caractéristique prédéterminée, et extraire des données d'écho à partir d'une partie mobile dans un corps ;
caractérisé en ce qu'il comprend en outre :

15 une étape d'acquisition de première valeur d'amplitude destinée à acquérir une première valeur d'amplitude d'autocorrélation à partir des données d'écho provenant de la partie mobile dans le corps, obtenues à l'étape de filtrage, en multipliant les données d'écho d'une première période de temps par le nombre complexe conjugué des données d'écho retardées par une deuxième période de temps prédéterminée, dans laquelle les première et deuxième périodes de temps prédéterminées sont des multiples entiers d'un signal d'horloge commun qui sont différents l'un de l'autre ; et
 20 une étape de colorisation destinée à rapporter une valeur à une luminance d'une teinte prédéterminée, dans laquelle la valeur est l'une parmi :

25 une valeur multipliée obtenue en multipliant la première valeur d'amplitude d'autocorrélation par la deuxième valeur d'amplitude d'autocorrélation ; et
 une valeur moyenne obtenue en pondérant les première et deuxième valeurs d'amplitude d'autocorrélation.

30 **2.** Procédé de traitement de données pour un appareil de diagnostic à ultrasons selon la revendication 1, le procédé comprenant en outre une étape d'acquisition de données ultrasonores destinée à acquérir la pluralité de morceaux de données ultrasonores en exécutant des opérations d'émission/réception par ultrasons une pluralité de fois dans une même direction de rayon sonore et à des intervalles de temps prédéterminés, dans lequel la partie mobile du corps est un réflecteur mobile incluant un débit sanguin.

35 **3.** Procédé de traitement de données pour un appareil de diagnostic à ultrasons selon la revendication 2, dans lequel les opérations d'émission/réception par ultrasons à l'étape d'acquisition de données sont exécutées en utilisant une sonde ultrasonore (11).

40 **4.** Procédé de traitement de données pour un appareil de diagnostic à ultrasons selon la revendication 2, dans lequel les filtres sont des filtres éliminateurs d'échos fixes (16, 17).

5. Procédé de traitement de données pour un appareil de diagnostic à ultrasons selon l'une quelconque des revendications 1 à 4, dans lequel :

45 la valeur est la valeur moyenne obtenue en pondérant les première et deuxième valeurs d'amplitude d'autocorrélation ; et
 l'étape de colorisation destinée à rapporter la valeur moyenne obtenue en pondérant les première et deuxième valeurs d'amplitude d'autocorrélation à la luminance d'une teinte prédéterminée comprend :

50 une étape consistant à acquérir une valeur de vitesse à partir de la partie réelle et de la partie imaginaire de la première valeur d'amplitude d'autocorrélation ;
 une étape de traitement de valeur de seuil destinée à soumettre la valeur de vitesse au traitement de la valeur de seuil, en utilisant la valeur moyenne, générant une valeur de vitesse traitée ; et
 55 une étape de colorisation destinée à rapporter la valeur de vitesse traitée à la luminance de la teinte prédéterminée.

6. Appareil de diagnostic à ultrasons comprenant :

un moyen d'acquisition de données ultrasonores (12) destiné à acquérir une pluralité de morceaux de données ultrasonores en exécutant des opérations d'émission/réception par ultrasons par un transducteur ultrasonore (11) une pluralité de fois dans une même direction de rayon sonore et à des intervalles de temps prédéterminés ;
 un moyen d'extraction de données destiné à acquérir une pluralité de morceaux de données correspondant à une même profondeur prédéterminée, en dehors d'une pluralité de morceaux de données ultrasonores obtenus par le moyen d'acquisition de données ultrasonores (12) ;
 des filtres (16, 17) dont chacun possède une caractéristique de filtre prédéterminée, avec des données d'entrée correspondant à la même profondeur prédéterminée, obtenues par le moyen d'extraction de données, qui extrait des données d'écho à partir d'une partie mobile dans un corps ;
caractérisé en ce qu'il comprend en outre :

un moyen d'acquisition de première valeur d'amplitude (18) destiné à acquérir une première valeur d'amplitude d'autocorrélation à partir des données d'écho provenant de la partie mobile dans le corps, obtenues par les filtres (16, 17), en multipliant les données d'écho d'une première période de temps par le nombre complexe conjugué des données d'écho retardées par une première période de temps ;
 un moyen d'acquisition de deuxième valeur d'amplitude (19) destiné à acquérir une deuxième valeur d'amplitude d'autocorrélation à partir des données d'écho provenant de la partie mobile dans le corps, obtenues par les filtres (16, 17), en multipliant les données d'écho de la première période de temps par le nombre complexe conjugué des données d'écho retardées par une première période de temps, dans lequel les première et deuxième périodes de temps prédéterminées sont des multiples entiers d'un signal d'horloge commun qui sont différents l'un de l'autre ; et
 un moyen de colorisation (22) destiné à rapporter une valeur multipliée obtenue en multipliant la première valeur d'amplitude d'autocorrélation par la deuxième valeur d'amplitude d'autocorrélation, à une luminance d'une teinte prédéterminée.

7. Appareils de diagnostic à ultrasons selon la revendication 6, dans lequel les filtres sont des filtres éliminateurs d'échos fixes (16, 17).

FIG.1

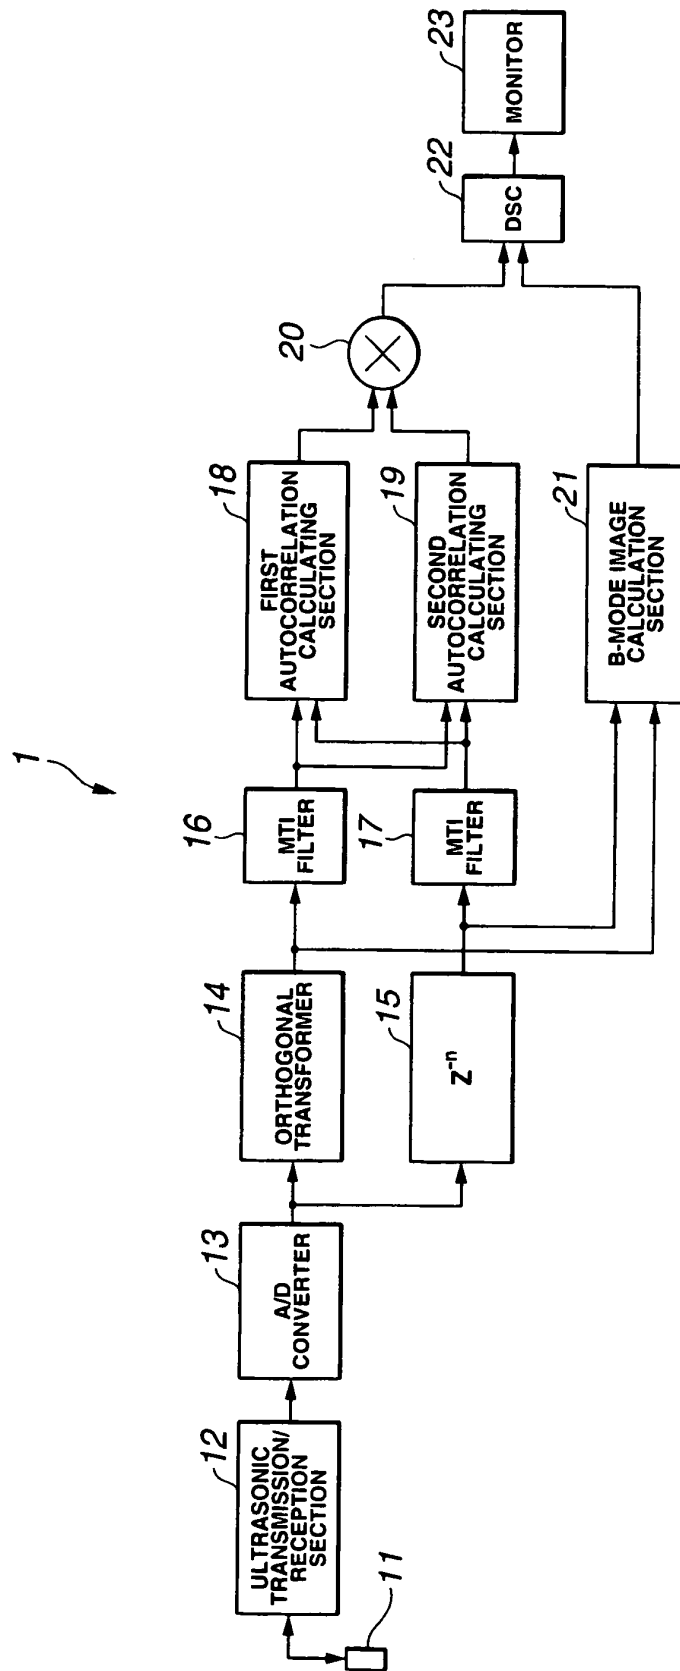


FIG.2

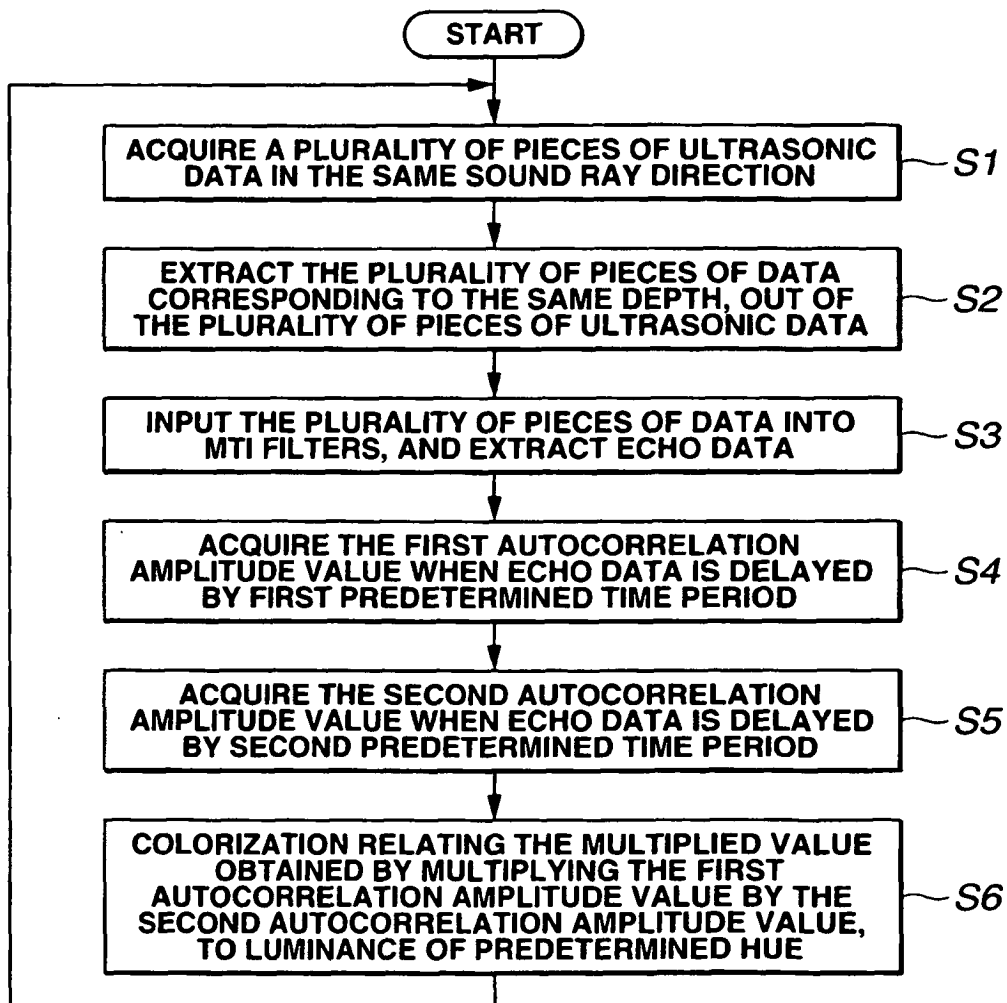


FIG.3

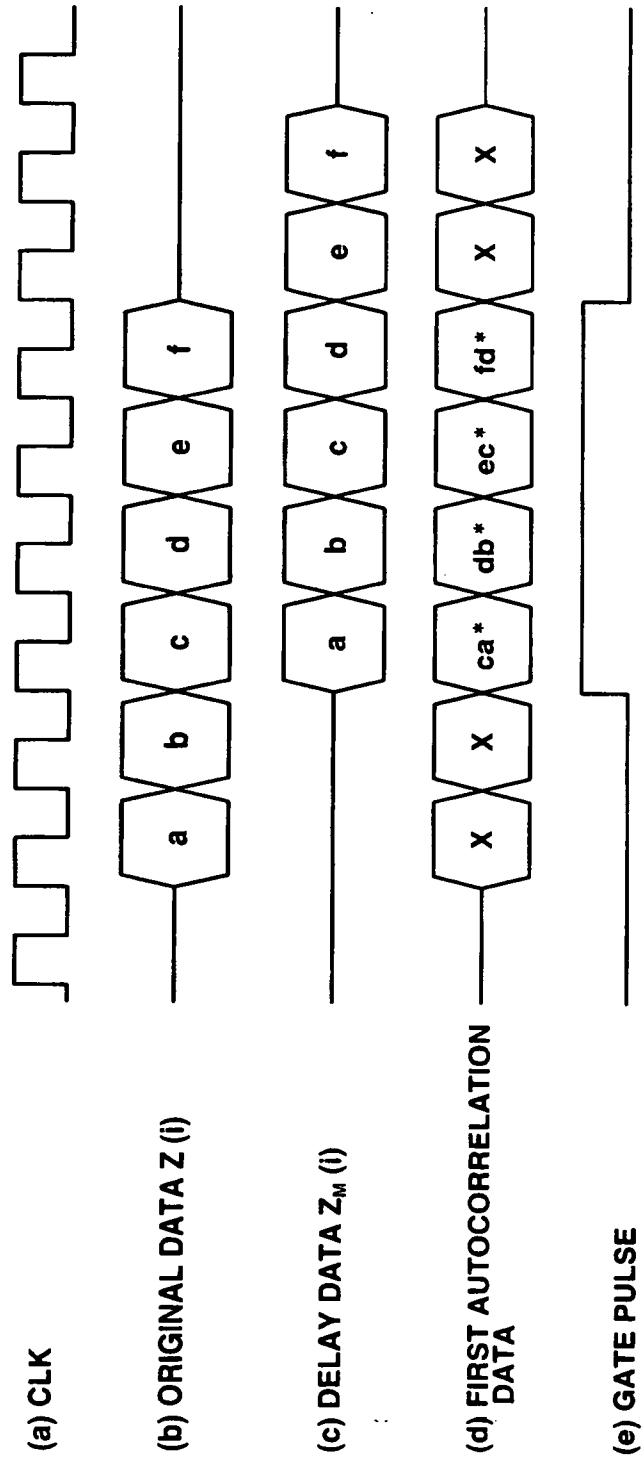


FIG.4

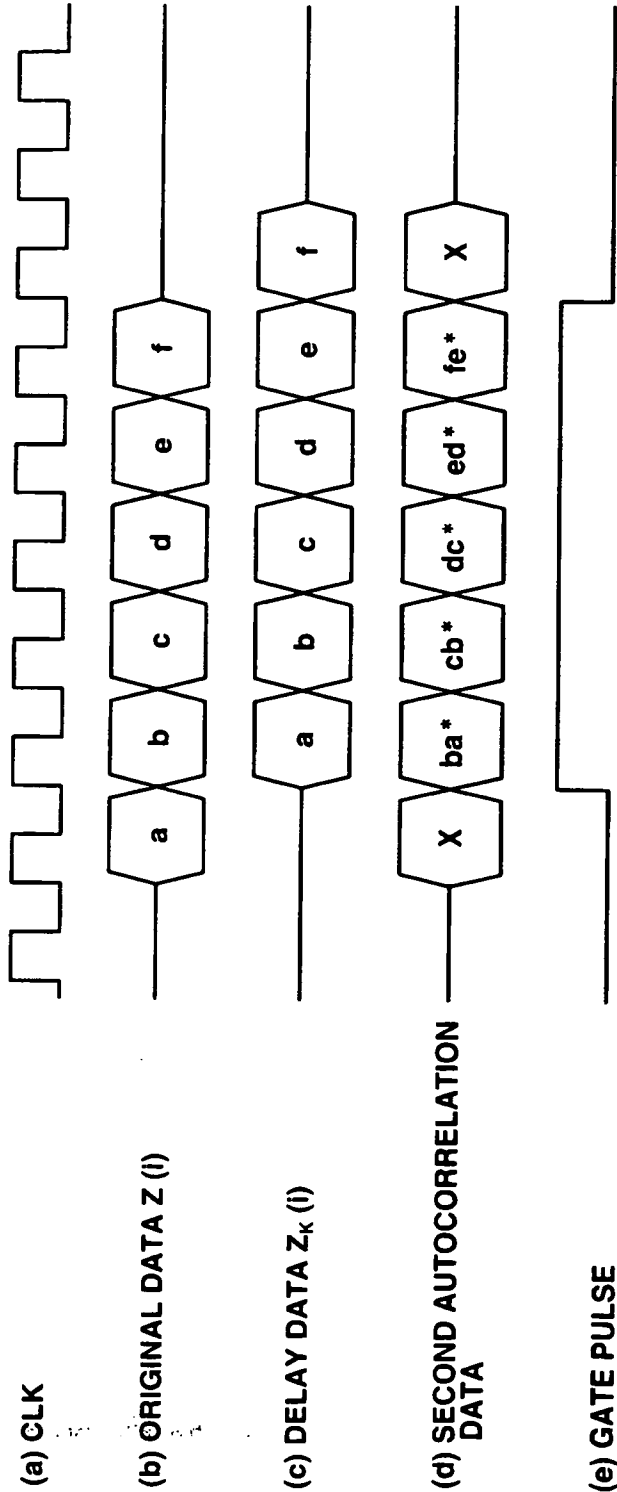


FIG.5

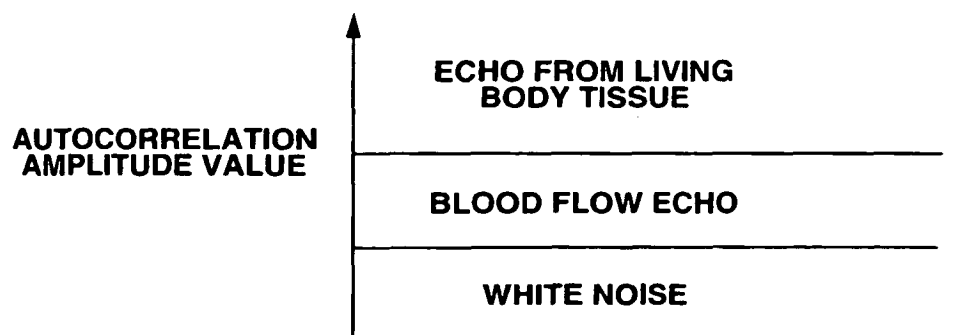


FIG.6

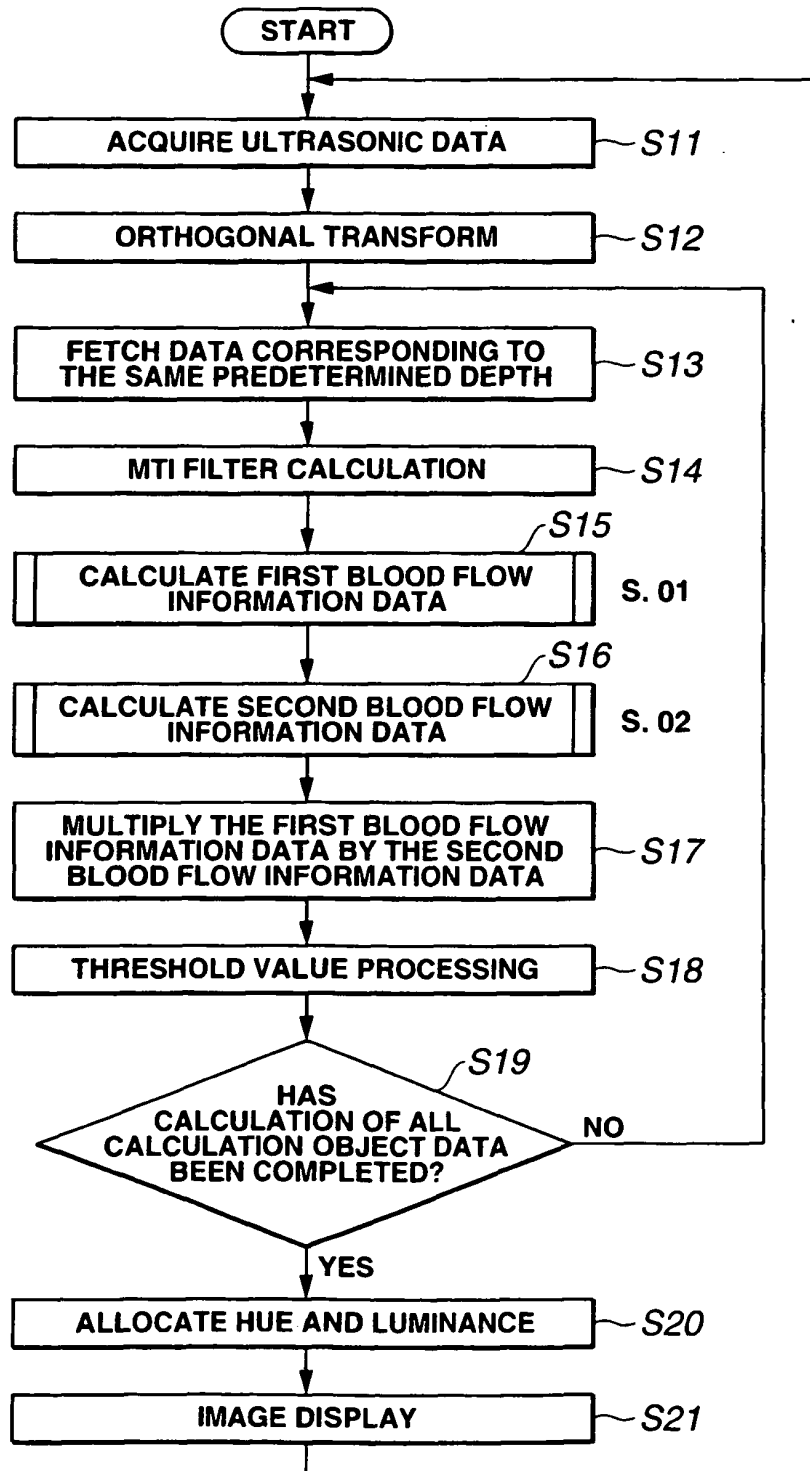


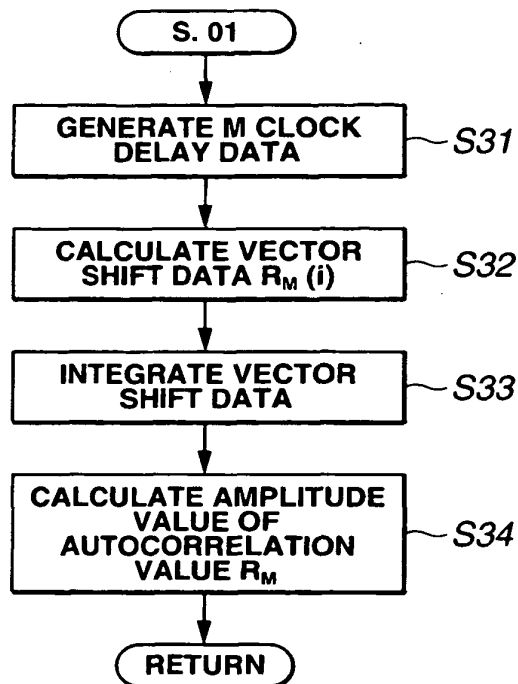
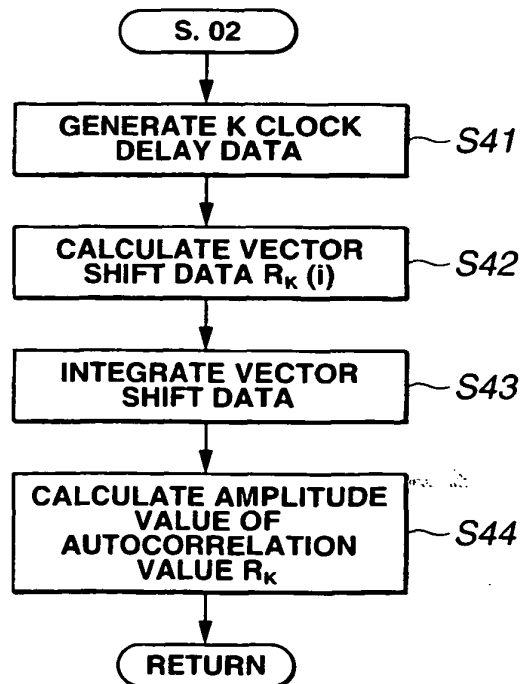
FIG.7**FIG.8**

FIG.9

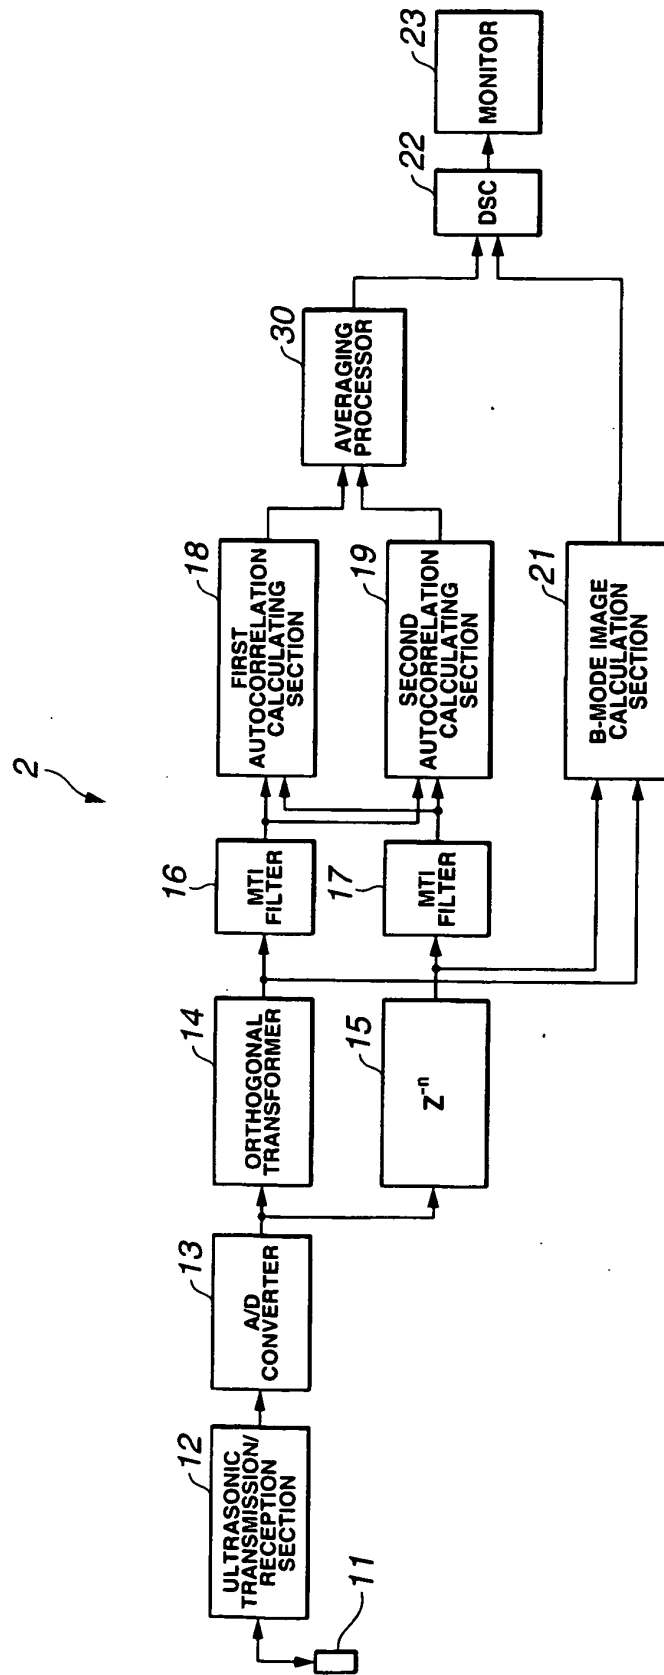


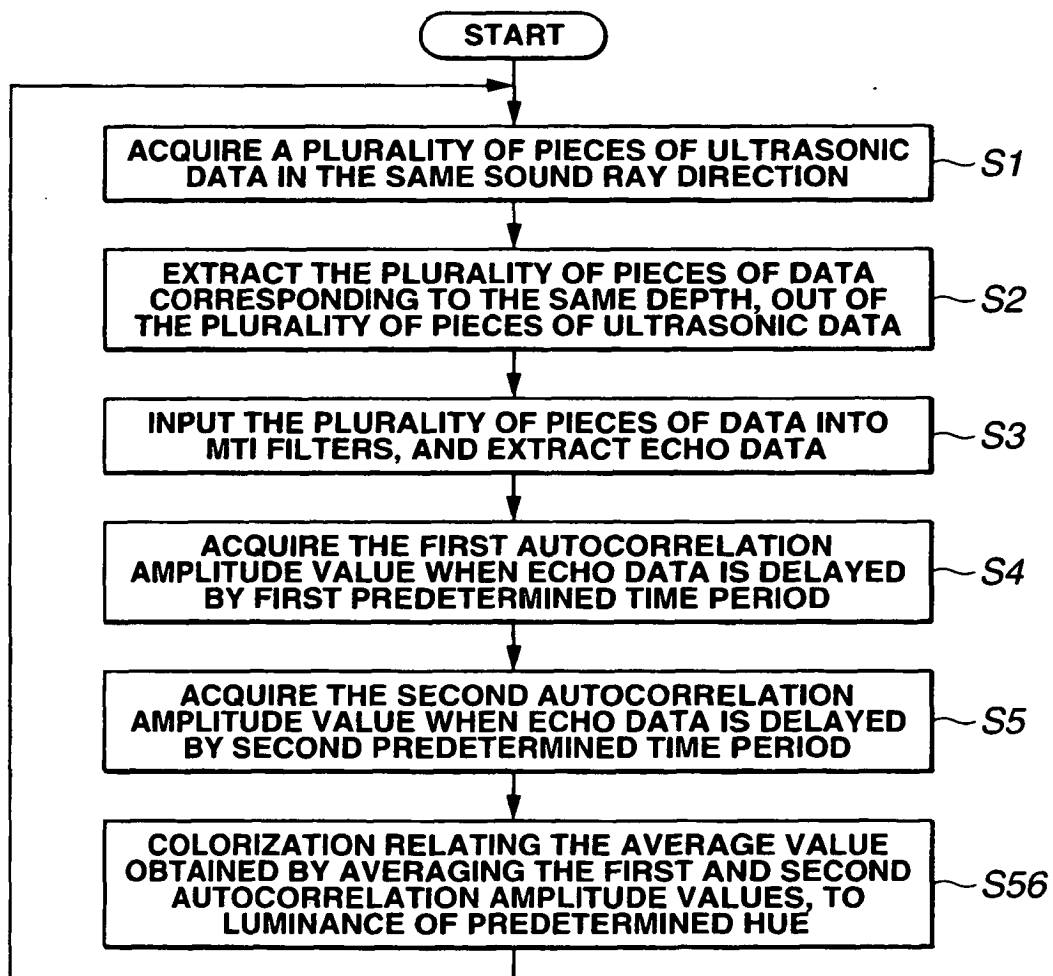
FIG.10

FIG.11

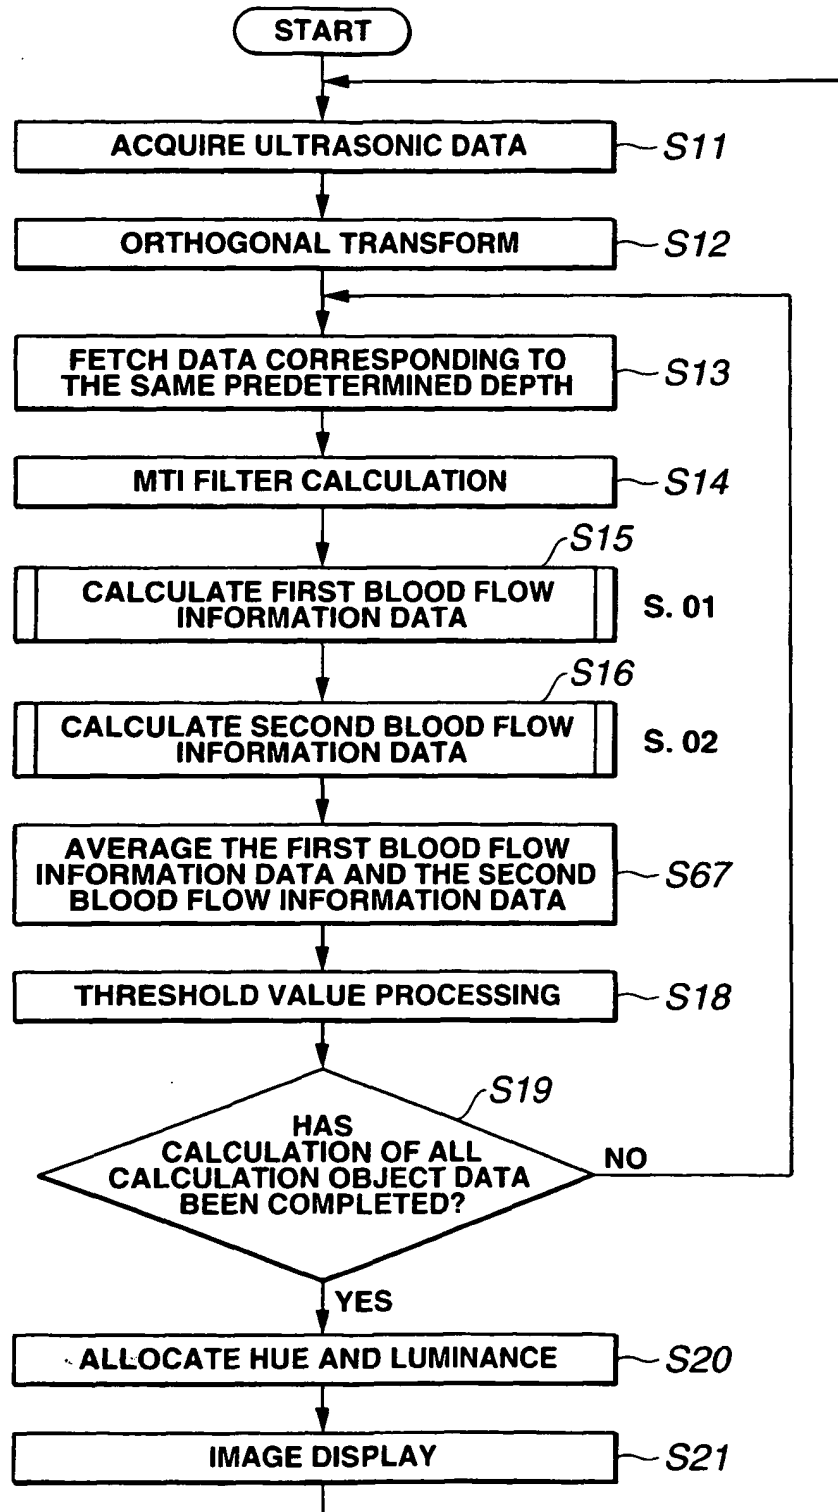


FIG.12

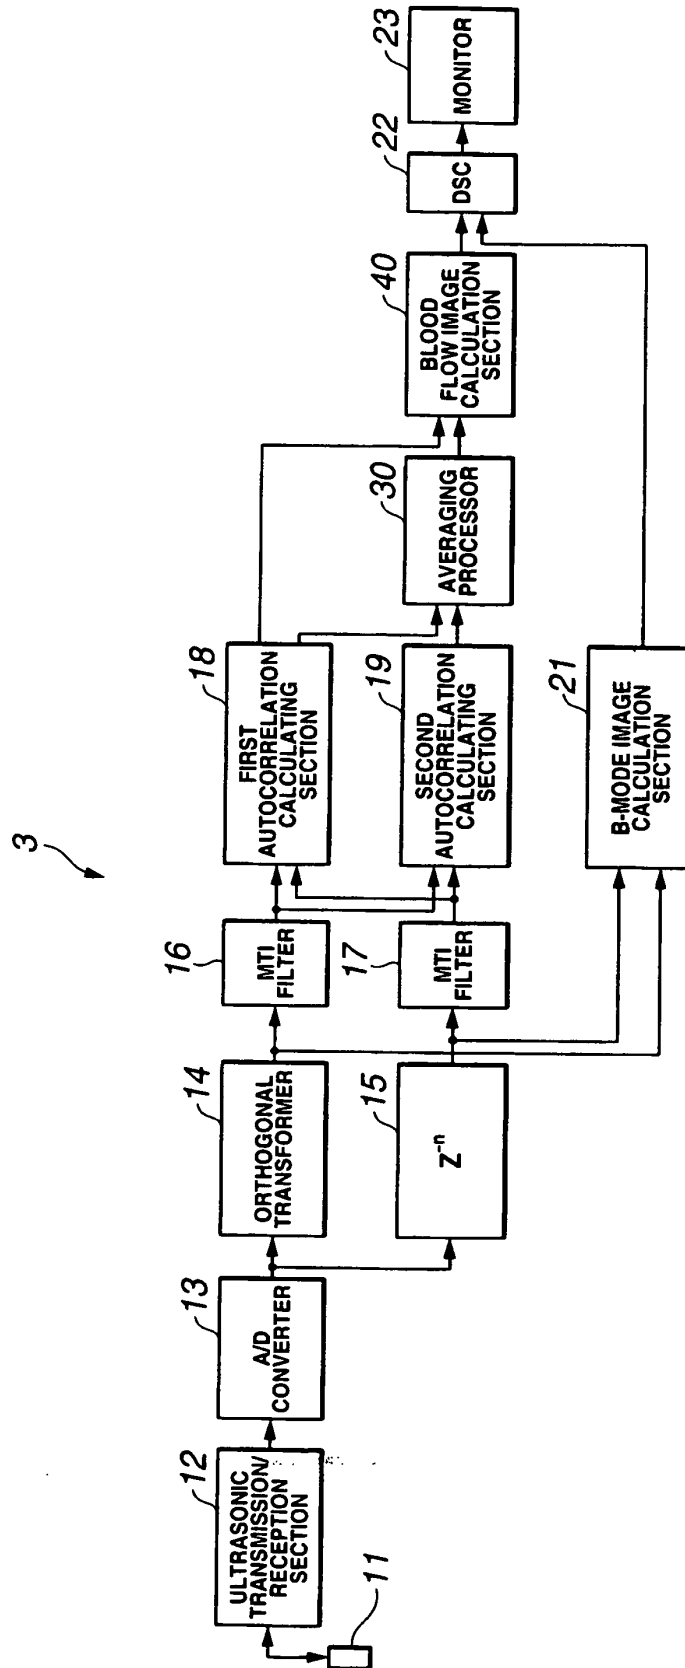
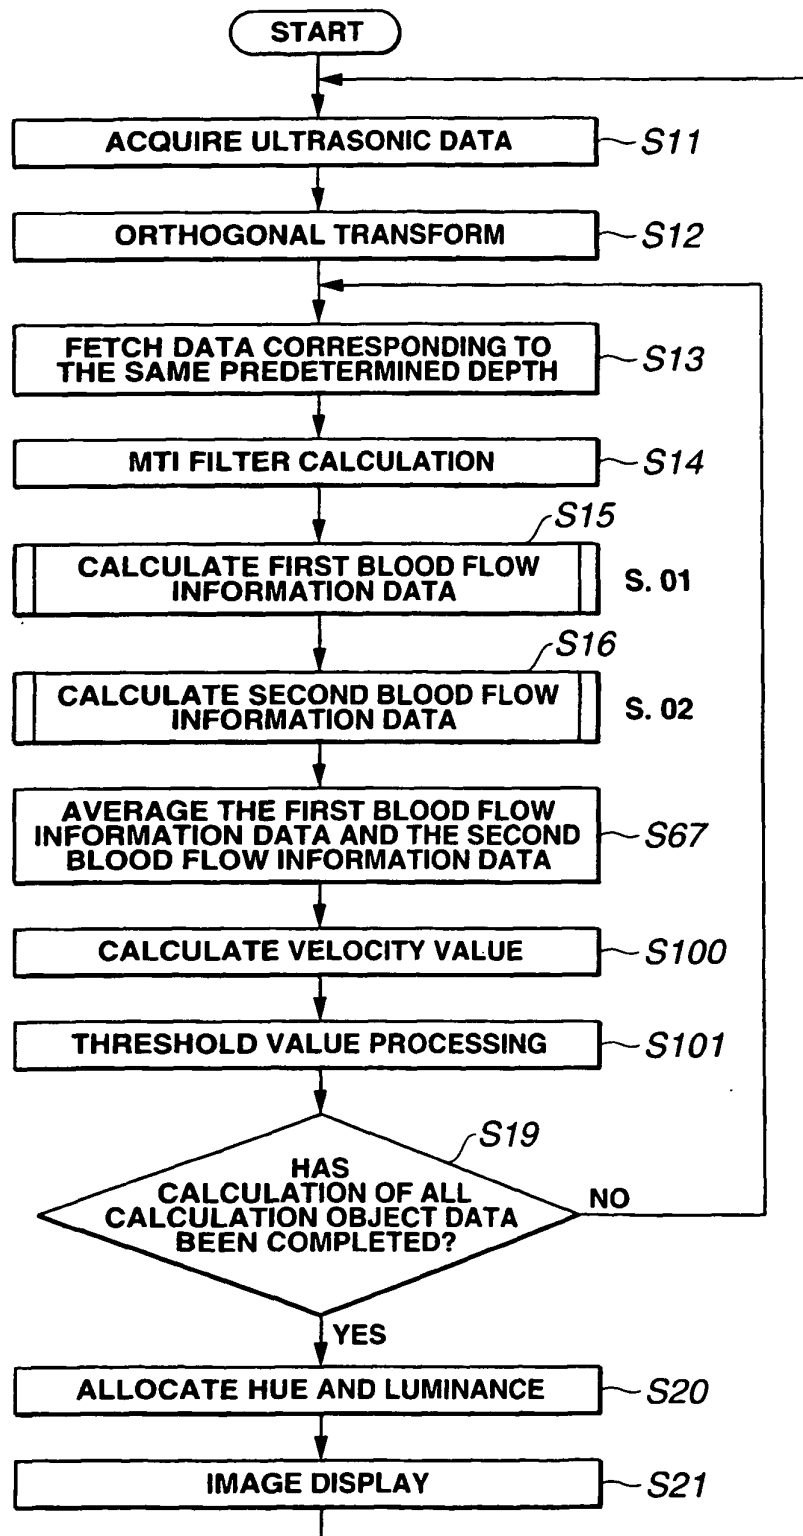


FIG.13



REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 61257631 A [0003]
- US 4799490 A [0005]
- JP 2003152958 A [0126]

Non-patent literature cited in the description

- Signal Processing for Colour Flow Imaging. **Evans D.** Doppler Ultrasound: Physics, Instrumentation and Signal Processing. John Wiley & Sons., Ltd, 2000, 245-263 [0006]

专利名称(译)	超声波装置和超声波装置数据处理方法		
公开(公告)号	EP1627602B1	公开(公告)日	2012-04-25
申请号	EP2004735519	申请日	2004-05-31
[标]申请(专利权)人(译)	奥林巴斯株式会社		
申请(专利权)人(译)	OLYMPUS CORPORATION		
当前申请(专利权)人(译)	OLYMPUS CORPORATION		
发明人	MIYAKI, HIRONAKA, OLYMPUS CORPORATION		
IPC分类号	A61B8/06 G01S7/52 G01S15/89		
CPC分类号	G01S15/8981 A61B8/06 G01S7/52071		
优先权	2003152958 2003-05-29 JP		
其他公开文献	EP1627602A1 EP1627602A4		
外部链接	Espacenet		

摘要(译)

根据本发明的超声诊断设备的数据处理方法包括：从通过执行多次超声波发送/接收操作获得的多个超声波数据中获取对应于相同预定深度的数据。相同的声线方向和预定的时间间隔;过滤对应于相同预定深度的采集数据，并从体内运动部分提取回波数据;当该回波数据被延迟第一预定时间段时，获取第一自相关幅度值;当上述回波数据被延迟第二预定时间段时，获取第二自相关幅度值;并且进一步将通过将第一自相关幅度值乘以第二自相关幅度值而获得的相乘值与预定色调的亮度相关联。

$$X = I \times \cos \theta \dots (1)$$