



(11) **EP 1 813 195 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
11.08.2010 Bulletin 2010/32

(21) Application number: **05790499.7**

(22) Date of filing: **04.10.2005**

(51) Int Cl.:
A61B 8/12 (2006.01)

(86) International application number:
PCT/JP2005/018317

(87) International publication number:
WO 2006/051659 (18.05.2006 Gazette 2006/20)

(54) **ULTRASONIC ENDOSCOPE**
ULTRASCHALL-ENDOSKOP
ENDOSCOPE A ULTRASONS

(84) Designated Contracting States:
DE FR GB

(30) Priority: **09.11.2004 JP 2004325248**

(43) Date of publication of application:
01.08.2007 Bulletin 2007/31

(73) Proprietor: **Olympus Corporation**
Tokyo 151-0072 (JP)

(72) Inventors:
• **IMAHASHI, Takuya**
Olympus Medical Systems Corp.
Tokyo 151-0072 (JP)
• **MIZUNUMA, Akiko**
Olympus Medical Systems Corp.
Tokyo 1510072 (JP)
• **SAWADA, Yukihiro**
Olympus Medical Systems Corp.
Tokyo 151-0072 (JP)

• **WAKABAYASHI, Katsuhiko**
Olympus Medical Systems Corp.
Tokyo 151-0072 (JP)
• **SATO, Sunao**
Olympus Medical Systems Corp.
Tokyo 1510072 (JP)

(74) Representative: **von Hellfeld, Axel**
Wuesthoff & Wuesthoff
Patent- und Rechtsanwälte
Schweigerstrasse 2
81541 München (DE)

(56) References cited:
EP-A- 1 795 132 JP-A- 2 116 358
JP-A- 10 192 281 JP-A- 2003 033 353
JP-A- 2004 298 240 JP-A- 2004 298 240
US-A- 5 685 311 US-A- 5 810 009

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Technical Field

[0001] The present invention relates to an electronic radial scanning ultrasonic endoscope, and particularly to a method of connecting coaxial cables for transmitting signals and an ultrasonic transducer in which a plurality of transducer elements are arranged in such a manner that the arranged transducer elements to the cylindrical shape along the periphery of the ultrasonic transducer.

Background Art

[0002] There are two conventional methods of radial scanning ultrasonic endoscopes, the electronic scanning method that performs electronic scans and the mechanical scanning method that performs mechanical scans. In the ultrasonic endoscopes of the electronic scanning method, the configuration is generally employed in which the ultrasonic transducer formed in a cylindrical shape for performing the radial scan and the endoscopic observation and endo-therapy units for performing endoscopic image observation are arranged in very close proximity to each other and are fixed as one piece, and a plurality of flexible printed circuit (FPC) boards are used as cables for transmitting electric signals to and from the ultrasonic transducer.

[0003] In addition, a plurality of FPC boards connected to the transducer elements are arranged in such a manner that an arch is formed by the plurality of FPC boards in order to avoid being close to the endoscopic observation and endo-therapy units such as its instrument channel port and the like, and thereafter the plurality of FPC boards are connected to signal cables (coaxial cables) at a spot closer to the proximal end than the bending section of the endoscope (on the side of the control section of the ultrasonic endoscope body) (see Patent Document 1, for example).

[0004] In the ultrasonic endoscopes of the mechanical scanning method, a scan is performed by turning one ultrasonic transducer in the insertion axis direction using an electric motor or the like provided at the proximal end. Accordingly, the ultrasonic transducer is attached by means of a shaft bearing structure such as ball bearings provided in the vicinity of the ultrasonic transducer (see Patent Document 2, for example).

Patent Document 1 Japanese Patent Application Publication No. 2001-314406

Patent Document 2 Japanese Patent Application Publication No. 2-116358

[0005] EP 1 795 132 discloses the preamble of claim 1

[0006] US 5,685,311 discloses an ultrasonic probe with an electronic radial transducer. A plurality of piezoelectric elements with electrodes on both surfaces thereof are arranged on a backing member. On an end surface

over the piezoelectric elements there is arranged a doughnut-shaped substrate. Flexible substrates are used to connect the doughnut-shaped substrate with cables providing transmission of signals and power.

[0007] US 5,810,009 also discloses an ultrasonic probe with a plurality of ultrasonic transducers set in an array. There are provided electrodes at the front or side surfaces of the piezoelectric elements which are connected to cables at the proximal ends.

[0008] JP 2004-298240 shows an ultrasonic endoscope having an ultrasonic block with two or more oscillators and an endoscope block. The oscillators are contacted on the inside by signal cables.

Disclosure of the Invention

[0009] The ultrasonic endoscope of the electronic scanning method has the problem that when the FPC boards and the coaxial cables are connected and the components for the cables are inserted into the insertion tube, tensile force applied in the direction of the control section tends to break the connection between the ultrasonic transducer and the FPC boards, which results in disconnection.

[0010] Also, because the FPC boards, which are naturally flat shaped, are curved to form an arch, the residual stress of the FPC boards varies with thermal variations and variations in atmospheric pressure during sterilization and disinfection, and the FPC boards tend to change their shape, causing an increased likelihood of disconnection between the ultrasonic transducer and the connection portions in the FPC boards and between the cables and the connection portions in the FPC boards, which is problematic.

[0011] Also, the cross section of the FPC board is rectangular while the cross section of the ultrasonic endoscope is circular; accordingly, there is the problem that spatial losses result, requiring larger diameter of the ultrasonic endoscope even when the FPC boards are packed together into the insertion tube.

[0012] Also, there is the problem that, because the connection portions are at a place that is closer to the control section than to the bending section, it is difficult to repair when a disconnection is caused in this configuration.

[0013] Also, in the ultrasonic endoscope of the mechanical scanning method, the interval between the axis of an endoscopic image and the acoustic axis emitted from the ultrasonic transducer is determined by the dimension (diameter) of the ultrasonic transducer and the structure of the shaft bearing in the vicinity of the ultrasonic transducer. The diameter of the ultrasonic transducer influences the penetration, which in turn influences ultrasonic images; thus, the diameter of the ultrasonic transducer is required to be at least approximately 10 mm. Additionally, the structure is conventionally required to be the bearing structure; accordingly, the interval between the endoscopic image and the acoustic axis is ap-

proximately 10 mm. Thus, it is difficult to make images of surfaces of the body cavities that are in endoscopic images correspond to ultrasonic images (cross section images) of inside portions of the corresponding area on the endoscopic surfaces of the body cavities, which is problematic.

[0014] The present invention is achieved in view of the above problems, and it is an object of the present invention to provide an ultrasonic endoscope having an ultrasonic transducer in which the ultrasonic transducer and coaxial cables will not become disconnected even under thermal or mechanical loads.

[0015] In addition, it is another object of the present invention to provide an ultrasonic endoscope in which the length of the rigid portion required as a space for wiring is shortened as much as possible.

[0016] The present invention employs the configurations as described below in order to solve the above problems.

[0017] According to one aspect of the present invention, an ultrasonic endoscope according to the present invention is an ultrasonic endoscope according to claim 1 comprising: an ultrasonic transducer in a cylindrical shape including a plurality of piezoelectric devices, an acoustic matching layer stacked on a principal plane on a sound emitting plane side, an acoustic lens on a plane of the acoustic matching layer opposite to a plane facing the piezoelectric devices, and a backing material stacked on another principal planes of the piezoelectric devices; an endoscopic observation and endo-therapy units provided, for performing endoscopic image observation, at the proximal end side of the ultrasonic transducer; a cable ass'y (a bundle of cable) including a plurality of cables for transmitting signals to and from the ultrasonic transducer, in which: the cable ass'y is arranged in such a manner that the cable ass'y passes through an inside portion of the ultrasonic transducer and is connected to the ultrasonic transducer at the distal end side of the ultrasonic transducer.

[0018] Also, it is desirable in an ultrasonic endoscope according to the present invention that the ultrasonic transducer includes a ring-shaped frame member in an inside portion of the distal end side for forming the cylindrical shape; the ultrasonic endoscope further includes a ring-shaped circuit board having an outer diameter that is greater than the inner diameter of the frame member and that is smaller than the inner diameter of the ultrasonic transducer, the ring-shaped circuit board being for connecting respective cables included in the cable ass'y to the ultrasonic transducer; and the circuit board be locked in the frame member at the distal end side of the ultrasonic transducer.

[0019] Also, it is desirable in an ultrasonic endoscope according to the present invention that the ultrasonic transducer includes a ring-shaped frame member in an inside portion of the distal end side for forming the cylindrical shape; and the ultrasonic endoscope further comprises: a ring-shaped circuit board having an outer diam-

eter that is smaller than the inner diameter of the frame member, the ring-shaped circuit board being for connecting respective cables included in the cable ass'y to the ultrasonic transducer; and a locking member for locking the circuit board in the frame member at the distal end side of the ultrasonic transducer.

[0020] Also, it is desirable in an ultrasonic endoscope according to the present invention that, for the ultrasonic endoscope according to claim 1, the ultrasonic endoscope further comprises a balloon unit for covering the ultrasonic transducer; and the balloon unit or the acoustic lens be arranged in such a manner that the acoustic axis of ultrasound emitted from the acoustic lens and the balloon unit are not orthogonal to each other.

Brief Description of the Drawings

[0021]

Fig. 1 shows a configuration of the entire ultrasonic endoscope;

Fig. 2 shows a configuration of the rigid tip portion; Fig. 3 shows a configuration of the ultrasonic transducer;

Fig. 4 shows an internal configuration of the ultrasonic transducer;

Fig. 5 is a first view showing processes of manufacturing the ultrasonic transducer;

Fig. 6 is a second view showing processes of manufacturing the ultrasonic transducer;

Fig. 7 is a first view showing processes of manufacturing the ultrasonic transducer in an example of a variation;

Fig. 8 shows locking members in an example of a variation of the ultrasonic transducer;

Fig. 9 is a second view showing processes of manufacturing the ultrasonic transducer in an example of a variation;

Fig. 10 shows a positional relationship between the objective lens and the acoustic axis; and

Fig. 11 shows a positional relationship between a balloon unit and the acoustic axis.

Best Modes for Carrying Out the Invention

[0022] Hereinafter, embodiments of the present invention will be described by referring to the drawings.

[0023] Fig. 1 shows a configuration of an entire ultrasonic endoscope.

[0024] In Fig. 1, an ultrasonic endoscope 1 comprises an insertion section 11 that is to be inserted into body cavities, a control section 12 connected to a proximal end side of the insertion section 11, and a universal code 13 that extends from a side surface of the control section 12.

[0025] A scope connector 14 that is connected to a light source unit (not shown) for providing illumination light is connected to the proximal end of the universal code 13. An ultrasonic code 15 has an ultrasonic con-

nector 16 that is electrically connected to a diagnostic ultrasound system (not shown) and that is for driving an ultrasonic transducer and creating ultrasonic diagnosis images by performing various signal processes on received signals. The ultrasonic code 15 extends from the scope connector 14.

[0026] The insertion section 11 comprises, in the order starting from the distal end side thereof and in a connected state, a rigid tip portion 17 made of a stiff material, a bending section 18 that is at the proximal end side of the rigid tip portion 17 and that can arbitrarily bend, and an insertion tube 19 that is at the proximal end side of the bending section 18, is connected to the distal end side of the control section 12, and is elongate and flexible.

[0027] Fig. 2 shows a configuration of the rigid tip portion.

[0028] In Fig. 2, the rigid tip portion 17 comprises an endoscopic observation and endo-therapy unit 22 for directly performing endoscopic image observation of surfaces of tissues of diseased area, and an ultrasonic transducer 21 for emitting ultrasound in order to receive the ultrasound that have been reflected from the acoustic impedance boundary in the tissues of diseased area that are the observation area.

[0029] The endoscopic observation and endo-therapy unit 22 comprises an illumination lens 23 for guiding the illumination light to the surfaces of the tissues of diseased area, an objective lens 24 for condensing the light reflected from the surfaces of the tissues of diseased area, an nozzle 25 for feeding gas or liquid to body cavities, and an instrument channel outlet 26 for suction the gas or liquid in the body cavities and accepting an instrument.

[0030] Fig. 3 shows a configuration of the ultrasonic transducer.

[0031] In Fig. 3, the ultrasonic transducer 21 comprises circuit boards 32 connected to a cable ass'y 31 that includes a plurality of cables for the transmission of electric signals to and from an ultrasonic endoscope body via the bending section 18 and the insertion tube 19, boards 33 connected to the circuit boards 32 and linked to a cylindrical piezoelectric device for emitting ultrasound (see Fig. 4), an acoustic matching layer 34 formed on the outer surfaces of the piezoelectric devices for protecting the piezoelectric devices and for performing acoustic matching with an external environment, an acoustic lens 35 formed on the outer surface of the acoustic matching layer 34 for condensing the ultrasound transmitted from the piezoelectric devices, and a backing material (see Fig. 4) on the inner surfaces of the piezoelectric devices. The ultrasonic transducer 21 is cylindrical.

[0032] Fig. 4 shows an internal configuration of the ultrasonic transducer.

[0033] In Fig. 4, the ultrasonic transducer 21 comprises the circuit boards 32 connected to the cable ass'y 31, the boards 33, piezoelectric devices 36, the acoustic matching layer 34 stacked on the outer surface of the piezoelectric devices 36, the acoustic lens 35 stacked on the outer surface of the acoustic matching layer 34, and a

backing material 38 on the inner surfaces of the piezoelectric devices 36.

[0034] The cable ass'y 31 and the circuit boards 32 are connected to each other via cables 43, and the connection spots between them are covered by a potting material 44. The circuit boards 32 and the boards 33 are connected to each other via wires 45 at soldered portions 46, and the boards 33 are connected to the piezoelectric devices 36 via connection units 37. Thereby, electric signals are transmitted to the piezoelectric devices 36.

[0035] A cylindrical nose piece 42 surrounding the cable ass'y 31 is provided to the circuit boards 32, and the circuit boards 32 are partially grounded via a ground line 47 in the cylindrical nose piece 42. The circuit boards 32 are locked in ring-shaped frame members 41 in such a way that the piezoelectric devices 36, the boards 33, the acoustic matching layer 34, the acoustic lens 35, and the backing material 38 form a cylindrical shape.

[0036] Next, processes of manufacturing the ultrasonic transducer 21 are explained.

[0037] First, as shown in Fig. 5, the cable ass'y 31 and the circuit boards 32 are connected to each other, and the portion of the cable ass'y 31 closer to the circuit boards 32 is surrounded by the nose piece 42. The portion of the cable ass'y 31 closer to the ultrasonic endoscope body is inserted, from the distal end side of the ultrasonic endoscope, into a cylinder made by stacking the backing material 38, the boards 33, the piezoelectric devices 36, the acoustic matching layer 34, and the acoustic lens 35.

[0038] Then, as shown in Fig. 6, the circuit boards 32 are fixed to the frame member 41 that is closer to the distal end of the ultrasonic endoscope. In this configuration, the outer diameter of the entire set of circuit boards 32 arranged in a ring shape is greater than the inner diameter of the frame members 41, and is smaller than the inner diameter of the ultrasonic transducer 21.

[0039] Next, variations in the ultrasonic transducer and its manufacturing processes will be explained.

[0040] In this present variation example, the circuit boards 32 are not locked in the ring-shaped frame member 41, but are locked by using the members that are used for locking the circuit boards 32. This contrasts with the above embodiment.

[0041] First, as shown in Fig. 7, the cable ass'y 31 and a circuit board 73 are connected to each other, and the portion of the cable ass'y 31 closer to the circuit board 73 is surrounded by a nose piece 72. This nose piece 72 has a trench 71. Next, in a similar manner to the above embodiment, the portion of the cable ass'y 31 closer to the ultrasonic endoscope body is inserted, from the distal end side of the ultrasonic endoscope, into a cylinder made by stacking the backing material 38, the boards 33, the piezoelectric devices 36, the acoustic matching layer 34, and the acoustic lens 35.

[0042] Then, as shown in Fig. 8, locking members 81 are fitted into the trench 71, and the circuit board 73 is fixed to the frame member 41 that is closer to the distal

end of the ultrasonic endoscope by using the locking members 81 as shown in Fig. 9. In this configuration, the outer diameter of the circuit board 73, which has a ring shape, is smaller than the inner diameter of the above ultrasonic transducer 21, and is smaller than the inner diameter of the frame members 41. However, the circuit board 73 is fixed to the ring-shaped frame members 41 by the locking members 81 that are fitted into the trench 71.

[0043] As described above, the cable ass'y 31 is formed by grouping a plurality of cables for the transmission of electric signals via the bending section 18 and the insertion tube 19; accordingly, the sectional area of the cable ass' y 31 can be minimized. Further, the cable ass'y 31 is inserted, from the distal end side of the ultrasonic endoscope, into the inside portion of the backing material 38 that is one of the materials stacked in a cylindrical shape, and is connected to the circuit boards 32 at the distal end side of the ultrasonic endoscope. Accordingly, the cable ass' y 31 can be thinner on the portion closer to the control section 12 than on the portion closer to the distal end of the ultrasonic endoscope. In addition, there will not be an unnecessary load on the connection point between the cable ass'y 31 and the circuit boards 32 when manufacturing the ultrasonic transducer 21.

[0044] Because the cable ass'y 31 is connected to the circuit boards 32 at a position closer to the distal end of the ultrasonic endoscope and inside the backing material 38, which is one of the materials stacked in a cylindrical shape so that bearing members can be dispensed with, the interval 102 between an acoustic axis 101 representing the direction in which the ultrasound emitted from the ultrasonic transducer 21 travel and the objective lens 24 can be shortened. Further, it is also possible to shorten rigid length of the rigid tip portion 17 that is inserted into body cavities.

[0045] Also, the cable ass' y 31 is connected to the circuit board 32 inside the backing material 38, which is one of the materials stacked in a cylindrical shape, and at the distal end side of the ultrasonic endoscope when a balloon unit 111 for covering the ultrasonic transducer 21 is attached to balloon attachment grooves 112a and 112b; accordingly, it is possible, as shown in Fig. 11, to prevent an acoustic axis 101 from being at the midpoint of the interval 113 between the balloon attachment grooves 112a and 112b, and to prevent the acoustic axis 101 from being orthogonal to the wall of the balloon unit 111 when the balloon unit 111 is in an inflated state. This configuration contributes to the reduction of multiple echoes.

[0046] According to the present invention, a bearing structure is dispensed with, and the ultrasonic transducer and the coaxial cables are connected at the tip portion of the insertion tube of the ultrasonic endoscope. Accordingly, it is also possible to shorten the length of the rigid portion of the ultrasonic endoscope's tip portion, which is inserted into body cavities, thus realizing an ultrasonic endoscope that causes less discomfort in patients.

[0047] In addition, according to the present invention, the ultrasonic transducer and the coaxial cables are connected to each other at the tip portion of the insertion tube of the ultrasonic endoscope; accordingly, an acoustic lens for converting ultrasound can be arranged on the control section side of the tip portion of the ultrasonic endoscope, and thus it is possible to prevent the directions of the ultrasound transmitted and received from and by the acoustic lens from being orthogonal to the balloon unit. Thereby, multiple reflection caused by the balloon unit can be reduced.

Claims

1. An ultrasonic endoscope (1), comprising:

an ultrasonic transducer (21) in a cylindrical shape including a plurality of piezoelectric devices (36), an acoustic matching layer (34) stacked on a principal plane on a sound emitting plane side, an acoustic lens (35) on a plane of the acoustic matching layer (34) opposite to a plane facing the piezoelectric devices (36), and a backing material stacked on another principal planes of the piezoelectric devices (36);

an endoscopic observation and endo-therapy unit (22) provided, for performing endoscopic image observation, at a proximal end side of the ultrasonic transducer (21);

a cable assembly (31) including a plurality of cables for transmitting signals to and from the ultrasonic transducer (21), wherein:

the cable assembly (31) is arranged in such a manner that the cable ass'y passes through an inside portion of the ultrasonic transducer (21) and is connected to the ultrasonic transducer (21) at a distal end side of the ultrasonic transducer (21) and the ultrasonic transducer (21) includes a ring-shaped frame member (41) in an inside portion of the distal end side for forming the cylindrical shape; and

the ultrasonic endoscope (1) further comprises:

a ring-shaped circuit board (73) having an outer diameter that is smaller than an inner diameter of the frame member (41), for connecting respective cables included in the cable assembly (31) to the ultrasonic transducer (21), **characterized in that** the portion of the cable assembly (31) closer to the circuit board (73) is surrounded by a nose piece (72) with a trench (71), and a locking member (81) for locking the circuit board (73) in the frame member (41) at the distal end side of the ultrasonic transducer (21) is fitted into the trench (71).

2. The ultrasonic endoscope (1) according to claim 1, wherein:

the ultrasonic endoscope (1) further comprises a balloon unit for covering the ultrasonic transducer; and
the balloon unit (111) or the acoustic lens is arranged in such a manner that the acoustic axis of ultrasound emitted from the acoustic lens and the balloon unit (111) are not orthogonal to each other.

Patentansprüche

1. Ultraschallendoskop (1), umfassend:

einen Ultraschallwandler (21) in einer zylindrischen Form enthaltend eine Vielzahl von piezoelektrischen Geräten (36), eine akustische Anpassungsschicht (34), die auf einer Hauptebene auf einer schallabstrahlenden Ebene gestapelt ist, eine akustische Linse (35) auf einer Ebene der akustischen Anpassungsschicht (34) gegenüber einer den piezoelektrischen Geräten (36) zugewandten Ebene, und ein Trägermaterial, das auf einer anderen Hauptebene der piezoelektrischen Geräte (36) gestapelt ist;
eine endoskopische Beobachtungs- und Endotherapie-Einheit (22), die zum Durchführen endoskopischer Bildbeobachtung an einer proximalen Endseite des Ultraschallwandlers (21) vorgesehen ist;
eine Kabelanordnung (31) enthaltend eine Vielzahl von Kabeln zum Übertragen von Signalen zu und von dem Ultraschallwandler (21), wobei:

die Kabelanordnung (31) in solch einer Weise angeordnet ist, dass die Kabelanordnung sich durch einen Innenabschnitt des Ultraschallwandlers (21) erstreckt und mit dem Ultraschallwandler (21) an einer distalen Endseite des Ultraschallwandlers (21) verbunden ist und der Ultraschallwandler (21) ein ringförmiges Rahmenelement (41) in einem Innenabschnitt der distalen Endseite zum Bilden der zylindrischen Form enthält; und
das Ultraschallendoskop (1) weiter umfasst:

eine ringförmige Leiterplatte (73) mit einem Außendurchmesser, der kleiner ist als ein Innendurchmesser des Rahmenelements (41), zum Verbinden entsprechender in der Kabelanordnung (31) enthaltener Kabel mit dem Ultraschallwandler (21), **dadurch gekenn-**

zeichnet, dass der Abschnitt der Kabelanordnung (31), der näher an der Leiterplatte (73) ist, von einem Nasenstück (72) mit einer Furche (71) umgeben ist, und
ein Blockierelement (81) zum Blockieren der Leiterplatte (73) in dem Rahmenelement (71) an der distalen Endseite des Ultraschallwandlers (21) in der Furche (71) eingebracht ist.

2. Ultraschallendoskop (1) nach Anspruch 1, wobei:

das Ultraschallendoskop (1) weiter eine Balloneinheit zum Abdecken des Ultraschallwandlers umfasst; und
die Balloneinheit (111) oder die akustische Linse in solch einer Weise angeordnet ist, dass die akustische Achse des von der akustischen Linse und der Balloneinheit (111) abgestrahlten Ultraschalls nicht orthogonal zueinander sind.

Revendications

1. Endoscope ultrasonique (1), comprenant :

un transducteur ultrasonique (21) sous une forme cylindrique incluant une pluralité de dispositifs piézoélectriques (36), une couche d'adaptation acoustique (34) empilée sur un plan principal sur un côté de plan d'émission sonore, une lentille acoustique (35) sur un plan de la couche d'adaptation acoustique (34) opposé à un plan faisant face aux dispositifs piézoélectriques (36), et un matériau de dos empilé sur un autre plan principal des dispositifs piézoélectriques (36) ;
une unité d'observation endoscopique et d'endothérapie (22) prévue pour effectuer une observation d'une image endoscopique, au niveau d'un côté d'extrémité proximale du transducteur ultrasonique (21) ;
un ensemble de câbles (31) incluant une pluralité de câbles pour transmettre des signaux vers le et du transducteur ultrasonique (21), dans lequel :

l'ensemble de câbles (31) est agencé de telle manière que l'ensemble de câbles passe à travers une partie intérieure du transducteur ultrasonique (21) et est connecté au transducteur ultrasonique (21) au niveau d'un côté d'extrémité distale du transducteur ultrasonique (21) et le transducteur ultrasonique (21) inclut un élément de cadre (41) en forme d'anneau dans une partie intérieure du côté d'extrémité distale pour for-

mer la forme cylindrique ; et
l'endoscope ultrasonique (1) comprend en
outre :

une carte de circuit imprimé (73) en forme d'anneau ayant un diamètre extérieur qui est plus petit qu'un diamètre intérieur de l'élément de cadre (41), pour la connexion de câbles respectifs inclus dans l'ensemble de câbles (31) au transducteur ultrasonique (21), **caractérisé en ce que** la partie de l'ensemble de câbles (31) plus proche de la carte de circuit imprimé (73) est entourée par un nez (72) avec une rainure (71), et
un élément de blocage (81) pour bloquer la carte de circuit imprimé (73) dans l'élément de cadre (41) au niveau du côté d'extrémité distale du transducteur ultrasonique (21) est inséré dans la rainure (71).

2. Endoscope ultrasonique (1) selon la revendication 1, dans lequel :

l'endoscope ultrasonique (1) comprend en outre une unité de ballonnet pour recouvrir le transducteur ultrasonique ; et
l'unité de ballonnet (111) ou la lentille acoustique est agencée de telle manière que l'axe acoustique de l'ultrason émis de la lentille acoustique et l'unité de ballonnet (lit) ne sont pas orthogonaux l'un à l'autre.

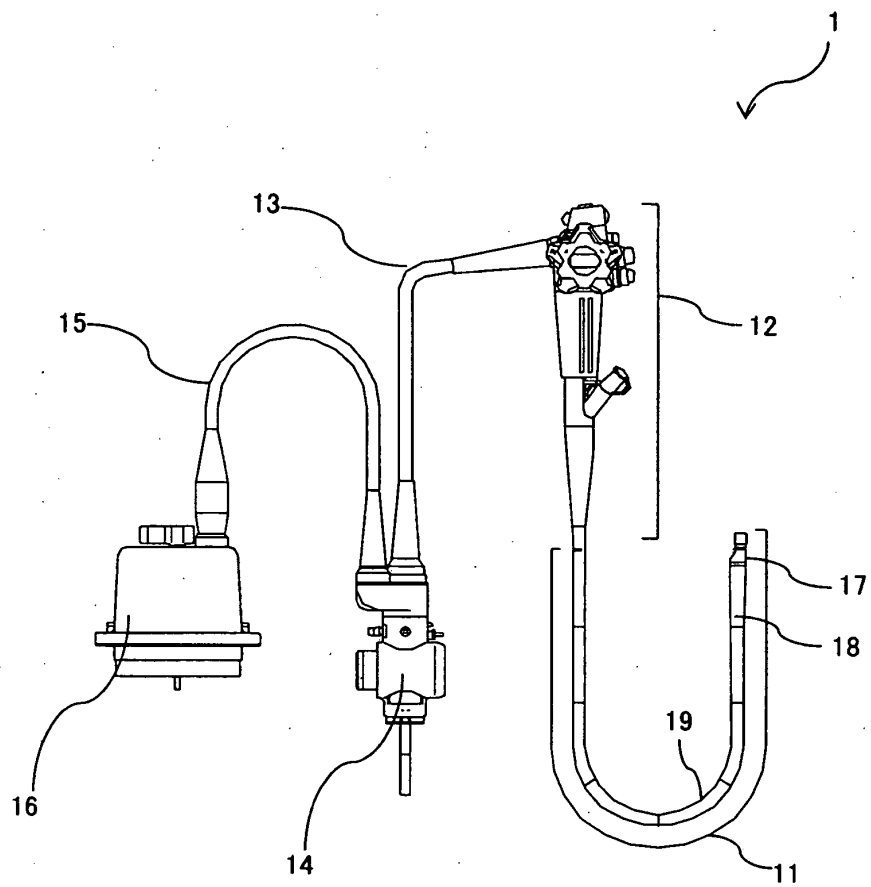


FIG. 1

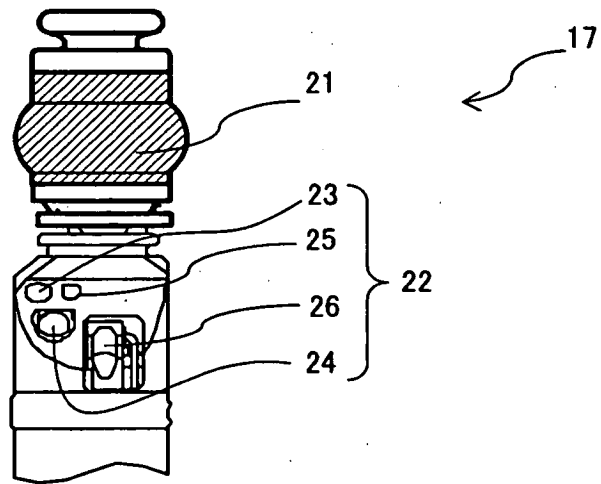


FIG. 2

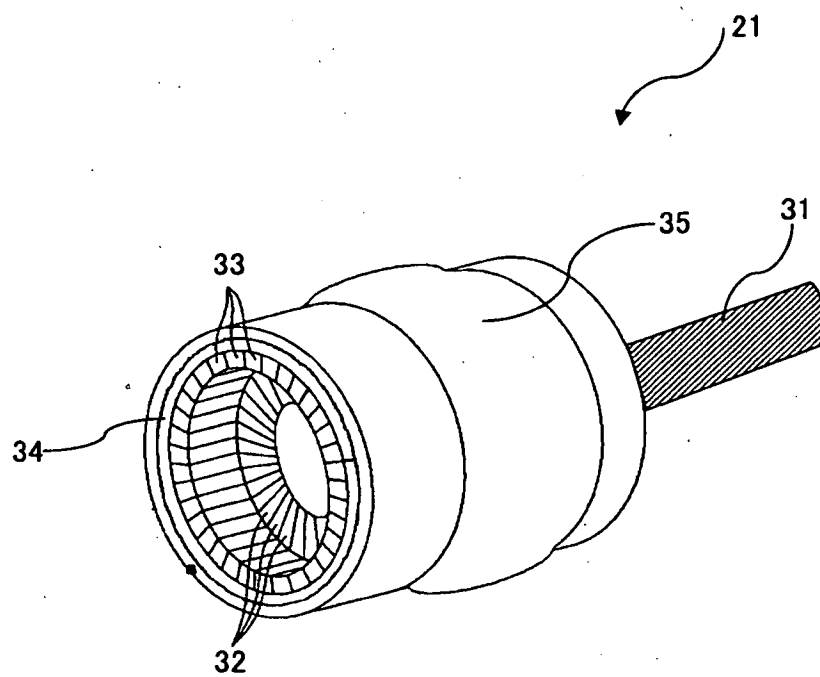


FIG. 3

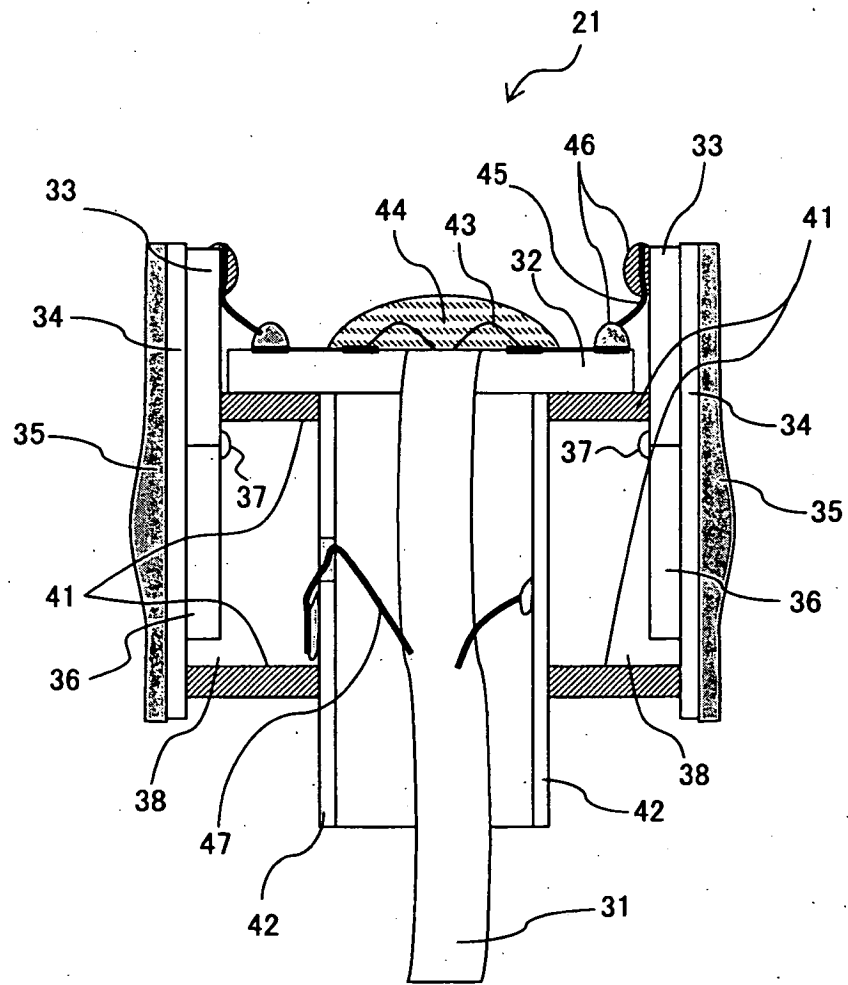


FIG. 4

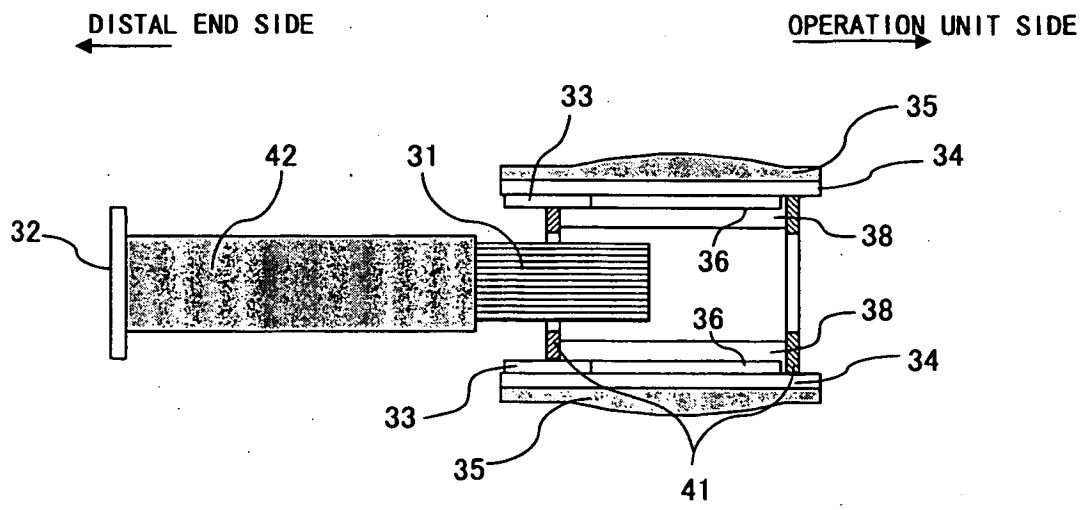


FIG. 5

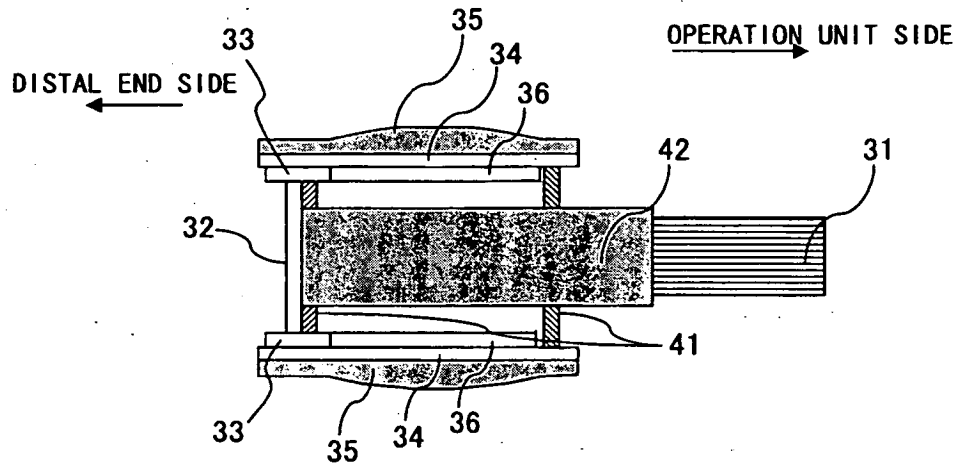


FIG. 6

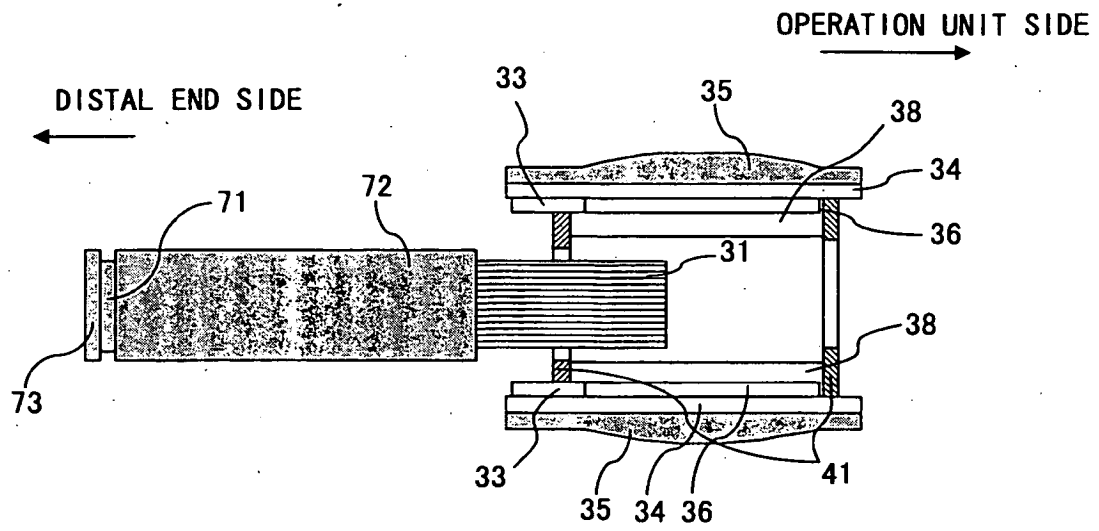


FIG. 7

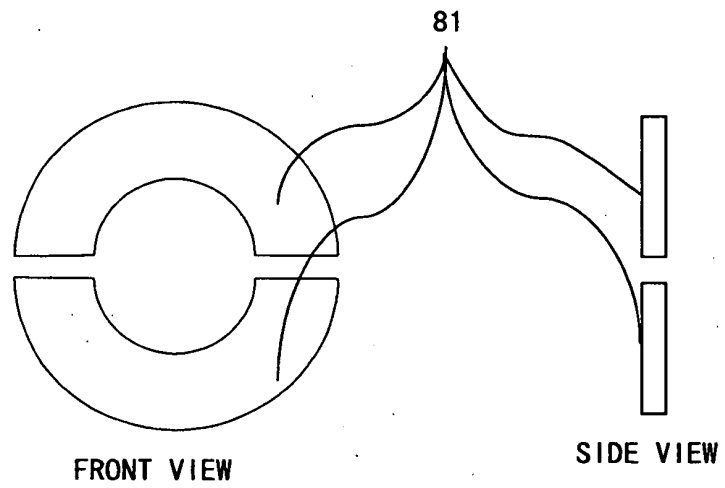


FIG. 8

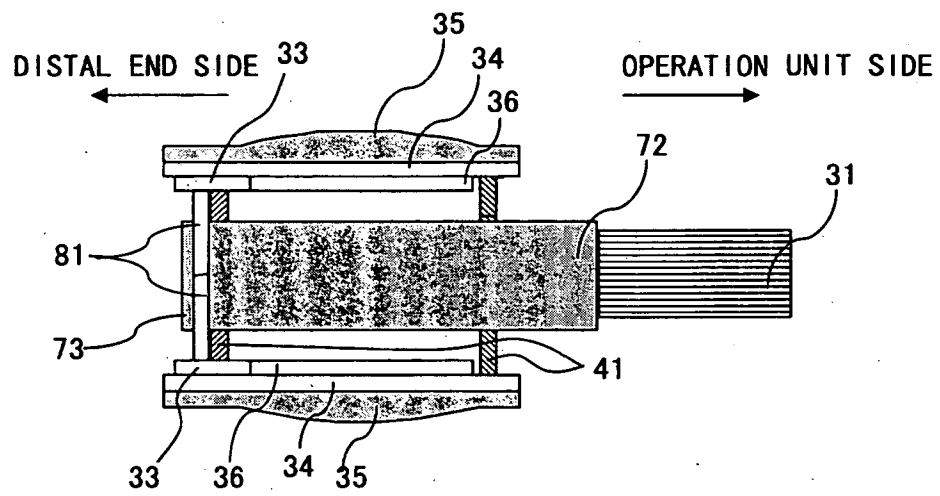


FIG. 9

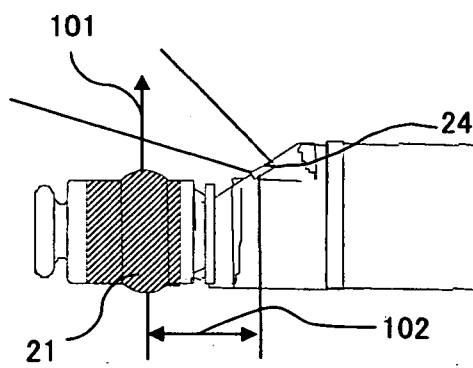


FIG. 10.

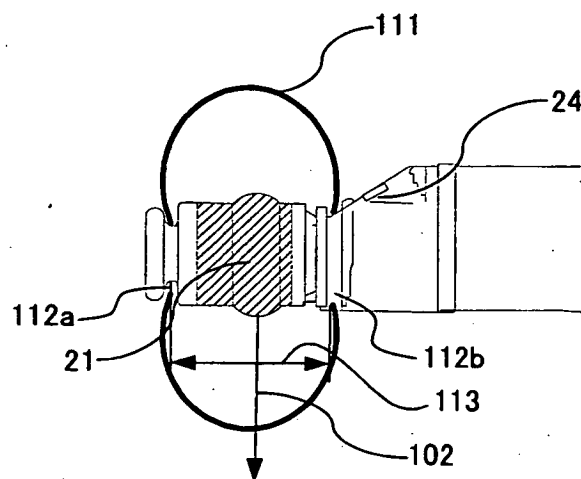


FIG. 11

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2001314406 A [0004]
- JP 2116358 A [0004]
- EP 1795132 A [0005]
- US 5685311 A [0006]
- US 5810009 A [0007]
- JP 2004298240 A [0008]

专利名称(译)	超声波内窥镜		
公开(公告)号	EP1813195A4	公开(公告)日	2008-03-19
申请号	EP2005790499	申请日	2005-10-04
[标]申请(专利权)人(译)	奥林巴斯株式会社		
申请(专利权)人(译)	OLYMPUS CORPORATION		
当前申请(专利权)人(译)	OLYMPUS CORPORATION		
发明人	IMAHASHI, TAKUYA OLYMPUS MEDICAL SYSTEMS CORP. MIZUNUMA, AKIKO OLYMPUS MEDICAL SYSTEMS CORP. SAWADA, YUKIHIKO OLYMPUS MEDICAL SYSTEMS CORP. WAKABAYASHI, KATSUHIRO OLYMPUS MEDICAL SYSTEMS CORP. SATO, SUNAO OLYMPUS MEDICAL SYSTEMS CORP.		
IPC分类号	A61B8/12		
CPC分类号	A61B8/12 A61B8/445 A61B8/4483 B06B1/0633		
优先权	2004325248 2004-11-09 JP		
其他公开文献	EP1813195B1 EP1813195A1		
外部链接	Espacenet		

摘要(译)

本发明提供一种超声波内窥镜，包括：包括多个压电装置的圆柱形超声波换能器，堆叠在发声平面侧的主平面上的声学匹配层，声学匹配平面上的声学透镜与面对压电器件的平面相对的层，和堆叠在压电器件的另一主面上的背衬材料；内窥镜观察和/或治疗单元，用于在超声换能器的近端侧进行内窥镜图像观察；电缆组件包括多个电缆，用于向超声换能器发送信号和从超声换能器发送信号。在上述结构中，电缆组件以电缆组件穿过超声波换能器的内部的方式布置，并且在超声波换能器的远端侧连接到超声波换能器。因此，提供了一种超声波内窥镜，其具有超声波换能器，其中超声波换能器和同轴电缆即使在热负荷或机械负荷下也不会断开。

