



(11) **EP 2 425 784 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
07.03.2012 Bulletin 2012/10

(51) Int Cl.:
A61B 8/00 (2006.01) G01S 7/52 (2006.01)

(21) Application number: **11176129.2**

(22) Date of filing: **01.08.2011**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(30) Priority: **02.09.2010 KR 20100085969**

(71) Applicant: **Samsung Medison Co., Ltd.**
Nam-myun,
Hongchun-gun
Kangwon do 250-870 (KR)

(72) Inventors:
• **Lee, Jae Keun**
135-851 Seoul (KR)
• **Lee, Hyeong Do**
135-851 Seoul (KR)
• **Lee, Yong Ho**
135-851 Seoul (KR)


(74) Representative: **Schmid, Wolfgang**
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft
Alte Ulmer Strasse 2
89522 Heidenheim (DE)

(54) **Providing a color Doppler mode image in an ultrasound system**

(57) Embodiments for providing a color Doppler mode image are disclosed. In one embodiment, by way of non-limiting example, an ultrasound system comprises: an ultrasound data acquisition unit configured to transmit and receive ultrasound signals to and from a living body to acquire first ultrasound data and second ultrasound data; a user input unit configured to receive input information corresponding to a region of interest and a balance threshold value having a predetermined

brightness value; and a processing unit configured to form a brightness mode image and a color Doppler mode image corresponding to the region of interest based on the first and second ultrasound data, respectively, form a balance mask for performing a balance process upon the color Doppler mode image based on the brightness mode image and the input information, and perform the balance process upon the color Doppler mode image based on the balance mask.

FIG. 1

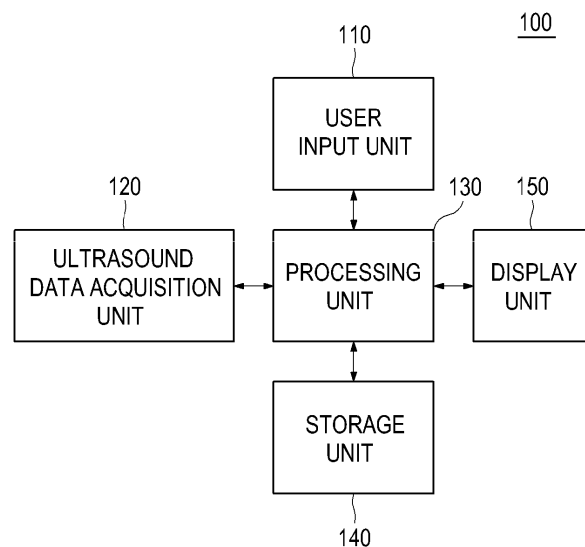

Description

CROSS-REFERENCE TO RELATED APPLICATION

- 5 **[0001]** The present application claims priority from Korean Patent Application No. 10-2010-0085969 filed on September 2, 2010.

TECHNICAL FIELD

- 10 **[0002]** The present disclosure generally relates to ultrasound systems, and more particularly to providing a color Doppler mode image in an ultrasound system.

BACKGROUND

- 15 **[0003]** An ultrasound system has become an important and popular diagnostic tool since it has a wide range of applications. Specifically, due to its non-invasive and non-destructive nature, the ultrasound system has been extensively used in the medical profession. Modern high-performance ultrasound systems and techniques are commonly used to produce two-dimensional or three-dimensional ultrasound images of internal features of an object (e.g., human organs).

- 20 **[0004]** The ultrasound system provides ultrasound images of various modes including a brightness mode (B mode) image representing reflection coefficients of the ultrasound signals reflected from a target object of a living body with a two-dimensional image, a Doppler mode image representing speed of a moving object with spectral Doppler by using a Doppler effect, a color Doppler mode image representing speed of a moving object with colors by using the Doppler effect, and an elastic mode image representing mechanical characteristics of tissues before and after applying a pressure thereto. Particularly, the ultrasound system transmits and receives ultrasound signals to and from the target object to thereby form Doppler signals corresponding to a region of interest (ROI), which is set on a B mode image. The ultrasound system further forms a color Doppler mode image that represents the speed of the moving object with colors based on the Doppler signals.

- 25 **[0005]** The ultrasound system performs a balance process to eliminate the color Doppler mode image corresponding to regions wherein a brightness value corresponding to a pixel of a brightness mode image is larger than a predetermined balance threshold value upon the color Doppler mode image. This is to remove color artifacts, which occurs by motion of regions such as blood-vessel walls, except interior spaces of the blood vessels, i.e., a lumen in which blood flows. However, this can be a problem since the conventional balance process cannot remove the color artifacts perfectly and decreases quality of the color Doppler mode image.

35 SUMMARY

- [0006]** Embodiments for providing a color Doppler mode image in an ultrasound system are disclosed herein. In one embodiment, by way of non-limiting example, an ultrasound system comprises: an ultrasound data acquisition unit configured to transmit and receive ultrasound signals to and from a living body to acquire first ultrasound data and second ultrasound data; a user input unit configured to receive input information corresponding to a region of interest and a balance threshold value having a predetermined brightness value; and a processing unit in communication with the ultrasound data acquisition unit and the user input unit, the processing unit being configured to form a brightness mode image and a color Doppler mode image corresponding to the region of interest based on the first and second ultrasound data, respectively, form a balance mask for performing a balance process upon the color Doppler mode image based on the brightness mode image and the input information, and perform the balance process upon the color Doppler mode image based on the balance mask.

- 40 **[0007]** In another embodiment, there is provided a method of providing a color Doppler mode image, comprising: a) forming a brightness mode image based on first ultrasound data for a living body; b) receiving input information corresponding to a region of interest and a balance threshold value having a predetermined brightness value from a user; c) forming a color Doppler mode image corresponding to the region of interest based on second ultrasound data for the living body; d) forming a balance mask for performing a balance process upon the color Doppler mode image based on the brightness mode image and the input information; and e) performing the balance process upon the color Doppler mode image based on the balance mask.

- 45 **[0008]** This summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This Summary is not intended to identify key or essential features of the claimed subject matter, nor is it intended to be used in determining the scope of the claimed subject matter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009]

- 5 FIG 1 is a block diagram showing an illustrative embodiment of an ultrasound system.
 FIG 2 is a schematic diagram showing an example of a brightness mode image and a region of interest.
 FIG 3 is a block diagram showing an illustrative embodiment of an ultrasound data acquisition unit.
 FIG 4 is a flow chart showing a process of performing a balance process upon a color Doppler mode image.
 FIG 5 is a flow chart showing a process of forming a balance mask.
 10 FIG 6 is a schematic diagram showing an example of an image parameter.
 FIG 7 is a schematic diagram showing another example of the image parameter.
 FIG 8 is a schematic diagram showing yet another example of the image parameter.
 FIG 9 is a schematic diagram showing still yet another example of the image parameter.

15 DETAILED DESCRIPTION

[0010] A detailed description may be provided with reference to the accompanying drawings. One of ordinary skill in the art may realize that the following description is illustrative only and is not in any way limiting.

20 **[0011]** Referring to FIG 1, an ultrasound system 100 in accordance with an illustrative embodiment is shown. As depicted therein, the ultrasound system 100 includes a user input unit 110. The user input unit 110 is configured to receive input information for a user. In one embodiment, the input information includes first input information for setting a region of interest (ROI) 220 on a brightness mode image 210 as shown in FIG 2. The ROI 220 includes a color box for obtaining a color Doppler mode image. The input information further includes second input information for setting a
 25 threshold value having a predetermined brightness value ("balance threshold value") for performing a balance processing upon the color Doppler mode image corresponding to the ROI 220. However, it should be noted herein that the input information may not be limited thereto. The user input unit 110 includes a control panel, a track ball, a mouse, a keyboard and the like.

[0012] The ultrasound system 100 further includes an ultrasound data acquisition unit 120. The ultrasound data acquisition unit 120 is configured to transmit and receive ultrasound signals to and from a living body and output ultrasound data. The living body includes a plurality of target objects (e.g., blood vessels, heart, etc.).
 30

[0013] FIG 3 is a block diagram showing an illustrative embodiment of the ultrasound data acquisition unit 120. Referring to FIG 3, the ultrasound data acquisition unit 120 includes an ultrasound probe 310. The ultrasound probe 310 includes a plurality of elements (not shown) for reciprocally converting between ultrasound signals and electrical signals. The ultrasound probe 310 is configured to transmit ultrasound signals to the living body. The ultrasound probe 310 is further
 35 configured to receive ultrasound signals (i.e., ultrasound echo signals) from the living body to output received signals. The received signals are analog signals. The ultrasound probe 310 includes a convex probe, a linear probe and the like.

[0014] The ultrasound data acquisition unit 120 further includes a transmit (Tx) signal generating section 320. The Tx signal generating section 320 is configured to control the transmission of the ultrasound signals. The Tx signal generating section 320 is further configured to generate electrical signals ("Tx signals") for obtaining at least one ultrasound image
 40 in consideration of the elements and focal points.

[0015] In one embodiment, the Tx signal generating section 320 is configured to generate first Tx signals for obtaining the brightness mode image. Thus, the ultrasound probe 310 is configured to convert the first Tx signals provided from the Tx signal generating section 320 into the ultrasound signals, transmit the ultrasound signals to the living body and receive the ultrasound echo signals from the living body to thereby output first received signals. The Tx signal generating
 45 section 320 is further configured to generate second Tx signals for obtaining the color Doppler mode image based on a predetermined ensemble number. The ensemble number represents the number of transmitting and receiving ultrasound signals in order to obtain Doppler signals corresponding to each of the scan-lines. Thus, the ultrasound probe 310 is configured to convert the second Tx signals provided from the Tx signal generating section 320 into the ultrasound signals, transmit the ultrasound signals to the living body and receive the ultrasound echo signals from the living body
 50 to thereby output second received signals.

[0016] The ultrasound data acquisition unit 120 further includes a beam former 330. The beam former 330 is configured to convert the received signals provided from the ultrasound probe 310 into digital signals. The beam former 330 is further configured to apply delays to the digital signals in consideration of the elements and the focal points to thereby output digital receive-focused signals.

55 **[0017]** In one embodiment, the beam former 330 is configured to convert the first received signals provided from the ultrasound probe 310 into first digital signals. The beam former 330 is further configured to apply delays to the first digital signals in consideration of the elements and the focal points to output first digital receive-focused signals. Also, the beam former 330 is configured to convert the second received signals provided from the ultrasound probe 310 into second

digital signals. The beam former 330 is further configured to apply delays to the second digital signals in consideration of the elements and the focal points to output second digital receive-focused signals.

[0018] The ultrasound data acquisition unit 120 further includes an ultrasound data forming section 340. The ultrasound data forming section 340 is configured to form ultrasound data based on the digital receive-focused signals provided from the beam former 330. The ultrasound data forming section 340 is further configured to perform signal processing (e.g., gain control, etc.) upon the digital receive-focused signals.

[0019] In one embodiment, the ultrasound data forming section 340 is configured to form first ultrasound data based on the first digital receive-focused signals provided from the beam former 330. The first ultrasound data includes radio frequency data. However, it should be noted herein that the first ultrasound data may not be limited thereto. The ultrasound data forming section 340 is further configured to form second ultrasound data based on the second digital receive-focused signals provided from the beam former 330. The second ultrasound data includes in-phase/quadrature (IQ) data. However, it should be noted herein that the second ultrasound data may not be limited thereto.

[0020] Although it is described above that the ultrasound data acquisition unit 120 is configured to acquire the ultrasound data by transmitting and receiving the ultrasound signals to and from the living body, the ultrasound data acquisition unit 120 is further configured to acquire the ultrasound data from an external or internal storage unit (not shown) connected to the ultrasound system 100.

[0021] Referring back to FIG 1, the ultrasound system 100 further includes a processing unit 130 in communication with the user input unit 110 and the ultrasound data acquisition unit 120. The processing unit 130 includes a central processing unit, a microprocessor or a graphic processing unit. However, it should be noted herein that the processing unit 130 may not be limited thereto.

[0022] FIG 4 is a flow chart showing a process of performing the balance process upon the color Doppler mode image. The processing unit 130 is configured to form the brightness mode image based on the first ultrasound data provided from the ultrasound data acquisition unit 120 at step S402 in FIG 4. The brightness mode image is displayed on a display unit 150. Thus, the user sets the ROI on the brightness mode image displayed on the display unit 150 by using the user input unit 110.

[0023] The processing unit 130 is configured to set the ROI on the brightness mode image based on the input information (i.e., first input information) provided from the user input unit 110 at step S404 in FIG 4. Thus, the ultrasound data acquisition unit 120 transmits and receives the ultrasound data to and from the living body to thereby acquire the second ultrasound data corresponding to the ROI.

[0024] The processing unit 130 is configured to form the color Doppler mode image based on the second ultrasound data provided from the ultrasound data acquisition unit 120 at step S406 in FIG 4. The methods of the color Doppler mode image are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0025] The processing unit 130 is configured to form a mask ("balance mask") for performing the balance process upon the color Doppler mode image based on the input information (i.e., second input information) provided from the user input unit 110 and the brightness mode image at step S408 in FIG 4.

[0026] FIG 5 is a flow chart showing a process of forming the balance mask. The processing unit 130 is configured to perform a preprocessing upon the brightness mode image to eliminate unnecessary image data at step S502 in FIG 5. The preprocessing includes a noise elimination process by using an average filter. However, it should be noted herein that the preprocessing may not be limited thereto.

[0027] The processing unit 130 is configured to set an image parameter based on the input information (i.e., second input information) provided from the user input unit 110 and the brightness mode image at step S504 in FIG 5. The image parameter is a parameter for forming the balance mask. That is, the image parameter is a parameter for securing connectivity of regions (e.g., blood vessels, tissues, etc.) except the inside space of the blood vessels, i.e., a lumen in which the blood flows.

[0028] In one embodiment, the processing unit 130 is configured to calculate a mean brightness value ("global mean brightness value") of pixels corresponding to the ROI of the brightness mode image based on brightness values corresponding to the pixels.

[0029] The processing unit 130 is further configured to calculate a pivot point value of a contrast stretching curve for controlling brightness levels based on the second input information (i.e., balance threshold value) provided from the user input unit 110 and the global mean brightness value. The processing unit 130 calculates the pivot point value using equation 1 provided below.

$$PPV = (V_{GM} + BTV)/2 \times V_{PPT} \quad (1)$$

[0030] In the equation, PPV represents the pivot point value, V_{GM} represents the global mean brightness value, BTV represents the balance threshold value and V_{PPT} represents a pivot point threshold value. The pivot point threshold value is a predetermined value in consideration of an application and type of the target object. For example, the pivot point threshold value is 0.8 to 1.2.

[0031] The processing unit 130 is configured to calculate a gradient ("curvature") of the contrast stretching curve based on the second input information (i.e., balance threshold value) and the global mean brightness value. For example, the processing unit 130 detects a maximum brightness value from the brightness mode image. The processing unit 130 further calculates a difference between a predetermined brightness value and the maximum brightness value. The processing unit 130 further sets the difference as the gradient of the contrast stretching curve. The methods of calculating the gradient are well known in the art. For example, the processing unit 130 calculates the gradient using equation 2 provided below.

$$w = \alpha \cdot x^d \quad (2)$$

[0032] In the equation, w represents the gradient, α represents a weight value, which is a predetermined value, x represents a constant value, and d represent a different value between the mean brightness value (i.e., global mean brightness value or local mean brightness value) and the balance threshold value.

[0033] As the difference between the global mean brightness value and the balance threshold value gets larger, the gradient becomes larger. As the difference between the global mean brightness value and the balance threshold value gets smaller, the gradient becomes smaller. However, it should be noted herein that the sign may not be limited thereto.

[0034] The processing unit 130 is configured to set a sign of the contrast stretching curve based on the second input information (i.e., balance threshold value) and the pivot point value. The sign includes "+" and "-." However, it should be noted herein that the sign may not be limited thereto. For example, the processing unit 130 compares the balance threshold value with the pivot point value. If the balance value is equal to or larger than the pivot point value, then the processing unit 130 sets the sign as "+." If the balance threshold value is smaller than the pivot point value, then the processing unit 130 sets the sign as "-."

[0035] The processing unit 130 is configured to set the image parameter based on the second input information, the global mean brightness value, the pivot point value, the gradient and the sign.

[0036] As one example, when the balance threshold value is 100, the global mean brightness value is 100 and the pivot point threshold value is 1.0, the processing unit 130 sets a first contrast stretching curve SC_1 based on the balance threshold value BTV as shown in FIG 6. The processing unit 130 further calculates the pivot point value ("100") by applying the balance threshold value, the global mean brightness value and the pivot threshold value to equation 1. The processing unit 130 further calculates a difference between the balance brightness value and the global mean brightness value. The processing unit 130 further calculates the gradient W of the first contrast stretching curve SC_1 based on the calculated difference. The processing unit 130 further compares the balance threshold value with the pivot point value, and determines that the balance threshold value is equal to the pivot point value. The processing unit 130 further sets the sign of the first contrast stretching curve SC_1 as "+" based on the determining result. The processing unit 130 further sets a second contrast stretching curve SC_2 for setting the brightness values of regions corresponding to pixels that the brightness value is equal to or larger than 100 as a predetermined value (e.g., 255) based on the balance threshold value, the global mean brightness value, the pivot point value, the gradient and the sign, as shown in FIG 6. The processing unit 130 further sets the second contrast stretching curve SC_2 as the image parameter for forming the balance mask. In FIG 6, the reference numeral PP represents a pivot point corresponding to the pivot point value. The image parameter shown in FIG 6 is used to form the second contrast stretching curve SC_2 , which controls the brightness values of the brightness mode image. That is, the image parameter is used to decrease the brightness values under the pivot point value and increase the brightness values above the pivot point value.

[0037] As another example, when the balance threshold value is 100, the global mean brightness value is 100 and the pivot point threshold value is 0.85, the processing unit 130 sets the first contrast stretching curve SC_1 based on the balance threshold value BTV as shown in FIG 7. The processing unit 130 further calculates the pivot point value (i.e., 85) by applying the balance threshold value (i.e., 100), the global mean brightness value (i.e., 100) and the pivot point threshold value (i.e., 0.85) to equation 1. The processing unit 130 further calculates a difference between the balance threshold value and the global mean brightness value. The processing unit 130 further calculates the gradient W of the first contrast stretching curve SC_1 based on the calculated difference as shown in FIG 7. The processing unit 130 further compares the balance threshold value with the pivot point value, and determines that the balance threshold value is larger than the pivot point value. The processing unit 130 further sets the sign of the first contrast stretching curve SC_1 as "+" based on the determining result. The processing unit 130 further sets the second contrast stretching curve SC_2

for setting the brightness values of regions corresponding to pixels that the brightness value is equal to or larger than 85 as a predetermined value (e.g., 255) based on the balance threshold value, the global mean brightness value, the pivot point value, the gradient and the sign, as shown in FIG 7. The processing unit 130 further sets the second contrast stretching curve SC₂ as the image parameter for forming the balance mask. In FIG 7, the reference numeral PP represents the pivot point corresponding to the pivot point value.

[0038] As yet another example, when the balance threshold value is 100, the global mean bright value is 50 and the pivot threshold value is 1.1, the processing unit 130 sets the first contrast stretching curve SC₁ based on the balance threshold value BTV as shown in FIG 8. The processing unit 130 further calculates the pivot point value (i.e., 82.5) by applying the balance threshold value (i.e., 100), the global mean brightness value (i.e., 50) and the pivot point threshold value (i.e., 1.1) to equation 1. The processing unit 130 further calculates a difference between the balance brightness value and the global mean brightness value. The processing unit 130 further calculates the gradient W of the first contrast stretching curve SC₁ based on the calculated difference as shown in FIG 8. Also, the processing unit 130 compares the balance threshold value with the pivot point value, and determines that the balance threshold value is larger than the pivot point value. The processing unit 130 further sets the sign of the first contrast stretching curve SC₁ as "+" based on the determining result. The processing unit 130 additionally sets the second contrast stretching curve SC₂ for setting the brightness values of regions corresponding to pixels wherein the brightness value is equal to or larger than 82.5 as a predetermined value (e.g., 255) based on the balance threshold value, the global mean brightness value, the pivot point value, the gradient and the sign, as shown in FIG 8. The processing unit 130 further sets the second contrast stretching curve SC₂ as the image parameter for forming the balance mask. In FIG 8, the reference numeral PP represents the pivot point corresponding to the pivot point value.

[0039] As yet another example, when the balance threshold value is 100, the global mean brightness value is 150 and the pivot point threshold value is 1.0, the processing unit 130 sets the first contrast stretching curve SC₁ based on the balance threshold value BTV as shown in FIG 9. The processing unit 130 further calculates the pivot point value (i.e., 125) by applying the balance threshold value (i.e. 100), the global mean brightness value (i.e., 150) and the pivot point threshold value (i.e., 1.0) to equation 1. Also, the processing unit 130 calculates a difference between the balance threshold value and the global mean brightness value. The processing unit 130 further calculates the gradient W of the first contrast stretching curve SC₁ based on the calculated difference as shown in FIG 9. The processing unit 130 further compares the balance threshold value with the pivot point value, and determines that the balance threshold value is smaller than the pivot point value. The processing unit 130 sets the sign of the first contrast stretching curve SC₁ as "-" based on the determining result. Also, the processing unit 130 sets the second contrast stretching curve SC₂ for setting the brightness values of regions corresponding to pixels wherein the brightness value is equal to or larger than 125 as a predetermined value (e.g., 255) based on the balance threshold value, the global mean brightness value, the pivot point value, the gradient and the sign, as shown in FIG 9. The processing unit 130 further sets the second contrast stretching curve SC₂ as the image parameter for forming the balance mask. In FIG 9, the reference numeral PP represents the pivot point corresponding to the pivot point value.

[0040] In another embodiment, the processing unit 130 is configured to calculate the global mean brightness value of pixels corresponding to the ROI of the brightness mode image based on the brightness values corresponding to the pixels. The processing unit 130 is further configured to divide the ROI into a plurality of regions. Each of the regions has at least one pixel. The processing unit 130 is further configured to calculate a mean brightness value ("local mean brightness value") of the at least one pixel corresponding to each of the regions. The processing unit 130 is further configured to calculate a mean brightness value of the global mean brightness value and the local mean brightness value. Also, the processing unit 130 is configured to set the image parameter based on the mean brightness value and the second input information provided from the user input unit 110, as mentioned above.

[0041] In yet another embodiment, the processing unit 130 is configured to divide the ROI into a plurality of regions. Each of the regions has at least one pixel. The processing unit 130 is further configured to calculate the local mean brightness value of the at least one pixel corresponding to each of the regions based on the brightness value of the at least one pixel. The processing unit 130 is further configured to calculate the pivot point value based on the local mean brightness value and the second input information (i.e., balance threshold value) provided from the user input unit 110. The processing unit 130 calculates the pivot point value as equation 3 provided below.

$$PPV = (V_{LM} + BTV)/2 \times V_{PPT} \quad (3)$$

[0042] In the equation, PPV represents the pivot point value, V_{LM} represents the local mean brightness value, BTV represents the balance threshold value and V_{PPT} represents the pivot point threshold value.

[0043] The processing unit 130 is configured to calculate the gradient of the contrast stretching curve based on the second input information (i.e., balance threshold value) and the local mean brightness value for each of the regions, as mentioned above. The processing unit 130 is further configured to set the sign of the contrast stretching curve based on the second input information (i.e., balance brightness value) and the pivot point value, as mentioned above. Also, the processing unit 130 is configured to set the image parameter based on the second input information, the local mean brightness value, the pivot point value, the gradient and the sign, as mentioned above.

[0044] Referring back to FIG 5, the processing unit 130 is configured to form the balance mask based on the image parameter at step S506 in FIG 5. In one embodiment, the processing unit 130 performs an image process upon the brightness mode image based on the image parameter for setting the brightness values of regions corresponding to pixels wherein the brightness value is equal to or larger than the pivot point value as a predetermined value (e.g., 255) to form the balance mask.

[0045] The processing unit 130 is configured to perform a morphological process for filling up empty space or enhancing connectivity upon the balance mask at step S508 in FIG 5. The morphological process is carried out by sequentially performing dilation and erosion. That is, the balance mask is removed as many as the predetermined number of pixels and then contracted (erosion).

[0046] Although it is described above that the processing unit 130 uses the dilation and erosion as the morphological process, the processing unit 130 uses opening and closing as the morphological process.

[0047] Referring back to FIG 4, the processing unit 130 is configured to perform the balance process upon the color Doppler mode image by using the balance mask at step S410 in FIG 4.

[0048] The processing unit 130 is configured to compound the brightness mode image and the balance-processed color Doppler mode image to form compound image at step S412 in FIG 4. The methods of compounding the brightness mode image and the color Doppler mode image are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0049] Referring back to FIG 1, the ultrasound system 100 includes a storage unit 140. The storage unit 140 stores the input information (i.e., first input information and second input information) received by the user input unit 110. The storage unit 140 further stores the ultrasound data (i.e., first ultrasound data and second ultrasound data) acquired by the ultrasound data acquisition unit 120. The storage unit 140 further stores the brightness mode image formed by the processing unit 130. The storage unit 140 further stores the color Doppler mode image formed by the processing unit 130.

[0050] The ultrasound system 100 includes the display unit 150. The display unit 150 displays the brightness mode image formed by the processing unit 130. The display unit 150 further displays the compound image formed by the processing unit 130. The display unit 150 further displays the color Doppler mode image formed by the processing unit 130.

[0051] Although embodiments have been described with reference to a number of illustrative embodiments thereof, it should be understood that numerous other modifications and embodiments can be devised by those skilled in the art that will fall within the scope of the principles of this disclosure. More particularly, numerous variations and modifications are possible in the component parts and/or arrangements of the subject combination arrangement within the scope of the disclosure, the drawings and the appended claims. In addition to variations and modifications in the component parts and/or arrangements, alternative uses will also be apparent to those skilled in the art.

Claims

1. An ultrasound system, comprising:

an ultrasound data acquisition unit configured to transmit and receive ultrasound signals to and from a living body to acquire first ultrasound data and second ultrasound data;
a user input unit configured to receive input information corresponding to a region of interest and a balance threshold value having a predetermined brightness value; and
a processing unit in communication with the ultrasound data acquisition unit and the user input unit, the processing unit being configured to form a brightness mode image and a color Doppler mode image corresponding to the region of interest based on the first and second ultrasound data, respectively, form a balance mask for performing a balance process upon the color Doppler mode image based on the brightness mode image and the input information, and perform the balance process upon the color Doppler mode image based on the balance mask.

2. The ultrasound system of Claim 1, wherein the processing unit is configured to:

form the brightness mode image based on the first ultrasound data;
set the region of interest on the brightness mode image based on the input information;

form the color Doppler mode image based on the second ultrasound data;
 set an image parameter for forming the balance mask based on the input information and the brightness mode image; and
 form the balance mask based on the image parameter.

3. The ultrasound system of Claim 2, wherein the processing unit is configured to:

calculate a mean brightness value of pixels corresponding to the region of interest of the brightness mode image;
 calculate a pivot point value of a contrast stretching curve and a gradient of the contrast stretching curve based on the mean brightness value and the balance threshold value, wherein the contrast stretching curve controls brightness levels of the brightness mode image;
 set a sign of the contrast stretching curve based on the balance threshold value and the pivot point value; and
 set the image parameter based on the mean brightness value, the balance threshold value, the pivot point value, the gradient and the sign.

4. The ultrasound system of Claim 3, wherein the processing unit is configured to calculate the pivot point value as a following equation:

$$PPV = (V_{GB} + BTV) / 2 \times V_{PPT}$$

wherein PPV is the pivot point value, V_{GB} is the mean brightness value, BTV is the balance threshold value, and V_{PPT} is a pivot point threshold value.

5. The ultrasound system of Claim 2, wherein the processing unit is configured to:

calculate a first mean brightness value of pixels corresponding to the region of interest of the brightness mode image;
 divide the region of interest into a plurality of regions having a predetermined size;
 calculate a second mean brightness value of pixels corresponding to each of the regions;
 calculate a mean brightness value of the first mean brightness value and the second mean brightness value for each of the regions;
 calculate a pivot point value of a contrast stretching curve and a gradient of the contrast stretching curve based on the mean brightness value and the balance threshold value, wherein the contrast stretching curve controls brightness levels of the brightness mode image;
 set a sign of the contrast stretching curve based on the balance threshold value and the pivot point value; and
 set the image parameter based on the mean brightness value, the balance threshold value, the pivot point value, the gradient and the sign.

6. The ultrasound system of Claim 2, wherein the processing unit is configured to:

divide the region of interest into a plurality of regions having a predetermined size;
 calculate a mean brightness value of pixels corresponding to each of the regions;
 calculate a pivot point value of a contrast stretching curve and a gradient of the contrast stretching curve based on the mean brightness value and the balance threshold value, wherein the contrast stretching curve controls brightness levels of the brightness mode image;
 set a sign of the contrast stretching curve based on the balance threshold value and the pivot point value; and
 set the image parameter based on the mean brightness value, the balance threshold value, the pivot point value, the gradient and the sign.

7. The ultrasound system of Claim 6, wherein the processing unit is configured to calculate the pivot point value as a following equation:

$$PPV = (V_{LM} + BTV) / 2 \times V_{PPT}$$

wherein PPV is the pivot point value, V_{LM} is the mean brightness value, BTV represents the balance threshold value and V_{PPT} represents the pivot point threshold value.

8. The ultrasound system of any of Claims 1 to 7, wherein the processing unit is further configured to:

perform a preprocessing upon the brightness mode image to eliminate unnecessary image data; and
perform a morphological process upon the balance mask to fill up empty space or enhance connectivity upon the balance mask.

9. A method of providing a color Doppler mode image, comprising:

- a) forming a brightness mode image based on first ultrasound data for a living body;
- b) receiving input information corresponding to a region of interest and a balance threshold value having a predetermined brightness value from a user;
- c) forming a color Doppler mode image corresponding to the region of interest based on second ultrasound data for the living body;
- d) forming a balance mask for performing a balance process upon the color Doppler mode image based on the brightness mode image and the input information; and
- e) performing the balance process upon the color Doppler mode image based on the balance mask.

10. The method of Claim 9, wherein the step d) includes:

calculating a mean brightness value of pixels corresponding to the region of interest of the brightness mode image;
calculating a pivot point value of a contrast stretching curve and a gradient of the contrast stretching curve based on the mean brightness value and the balance threshold value, wherein the contrast stretching curve controls brightness levels of the brightness mode image;
setting a sign of the contrast stretching curve based on the balance threshold value and the pivot point value;
setting an image parameter for forming the balance mask based on the mean brightness value, the balance threshold value, the pivot point value, the gradient and the sign; and
forming the balance mask based on the image parameter.

11. The method of Claim 10, wherein the pivot point value is calculated as a following equation:

$$PPV = (V_{GB} + BTV) / 2 \times V_{PPT}$$

wherein PPV is the pivot point value, V_{GB} is the mean brightness value, BTV is the balance threshold value, and V_{PPT} is a pivot point threshold value.

12. The method of Claim 10, wherein the step d) includes:

calculating a first mean brightness value of pixels corresponding to the region of interest of the brightness mode image;
dividing the region of interest into a plurality of regions having a predetermined size;
calculating a second mean brightness value of pixels corresponding to each of the regions;
calculating a mean brightness value of the first mean brightness value and the second mean brightness value for each of the region;
calculating a pivot point value of a contrast stretching curve and a gradient of the contrast stretching curve based on the mean brightness value and the balance threshold value, wherein the contrast stretching curve

controls brightness levels of the brightness mode image;
 setting a sign of the contrast stretching curve based on the balance threshold value and the pivot point value;
 setting an image parameter for forming the balance mask based on the mean brightness value, the balance
 threshold value, the pivot point value, the gradient and the sign; and
 forming the balance mask based on the image parameter.

13. The method of Claim 10, wherein the step d) includes:

dividing the region of interest into a plurality of regions having a predetermined size;
 calculating a mean brightness value of pixels corresponding to each of the regions;
 calculating a pivot point value of a contrast stretching curve and a gradient of the contrast stretching curve
 based on the mean brightness value and the balance threshold value, wherein the contrast stretching curve
 controls brightness levels of the brightness mode image;
 setting a sign of the contrast stretching curve based on the balance threshold value and the pivot point value;
 setting an image parameter for forming the balance mask based on the mean brightness value, the balance
 threshold value, the pivot point value, the gradient and the sign; and
 forming the balance mask based on the image parameter.

14. The method of the Claim 13, wherein the pivot point value is calculated as following equation:

$$PPV = (V_{LM} + BTV) / 2 \times V_{PPT}$$

wherein PPV is the pivot point value, V_{LM} is the mean brightness value, BTV represents the balance threshold value
 and V_{PPT} represents the pivot point threshold value.

15. The method of any of Claims 9 to 14, wherein the step d) further includes:

performing a preprocessing upon the brightness mode image to eliminate unnecessary image data; and
 performing a morphological process upon the balance mask to fill up empty space or
 enhance connectivity upon the balance mask.

FIG. 1

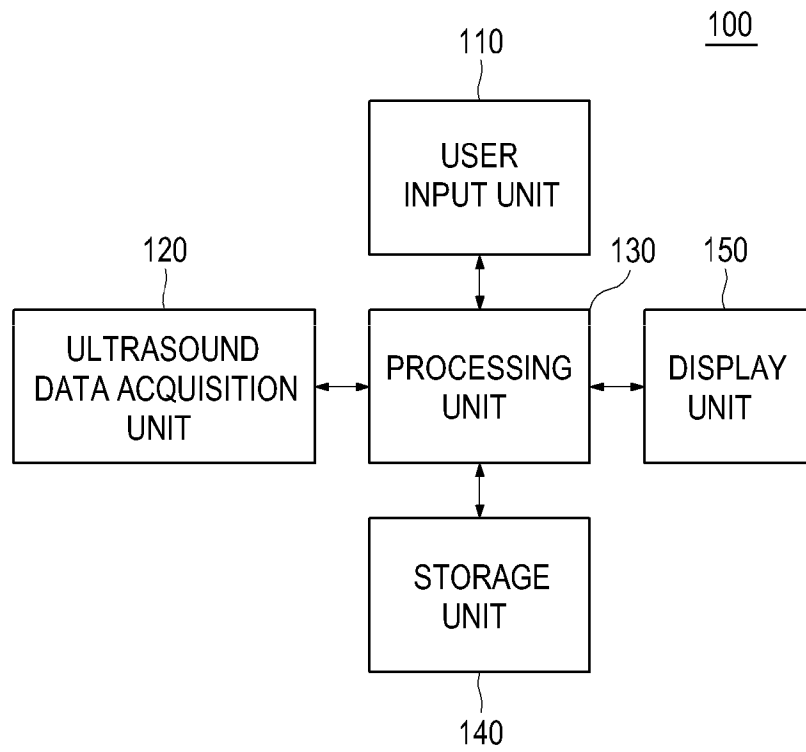


FIG. 2

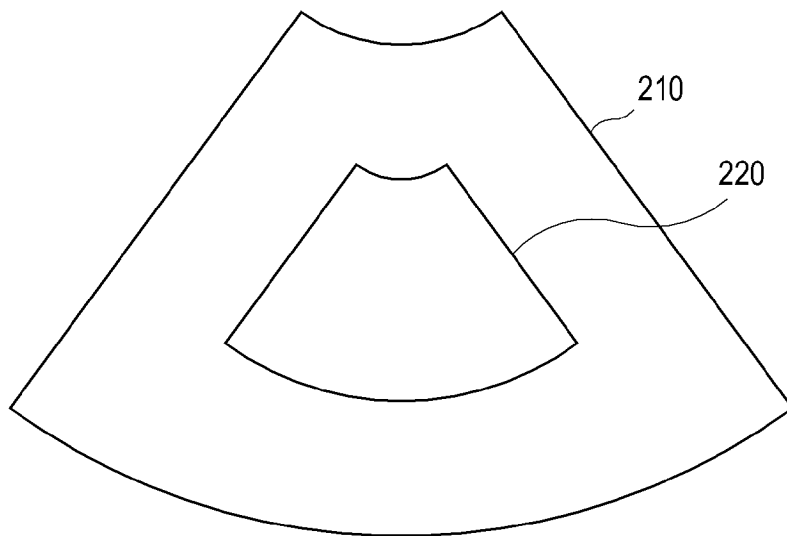


FIG. 3

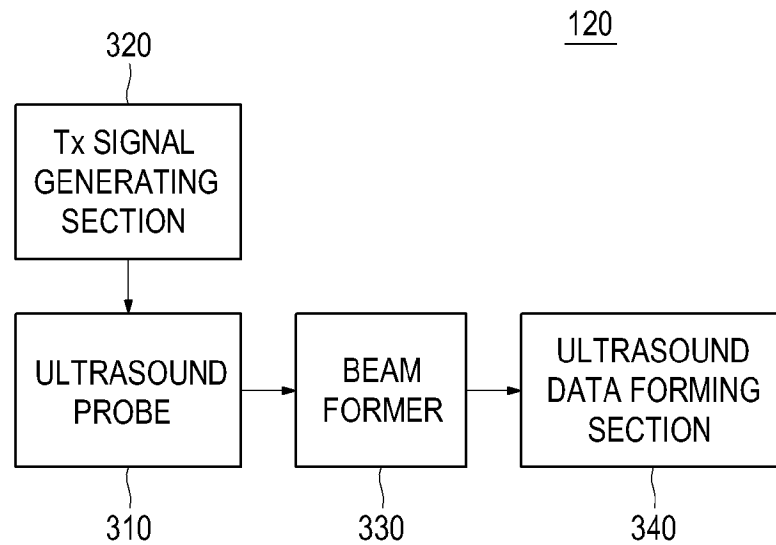


FIG. 4

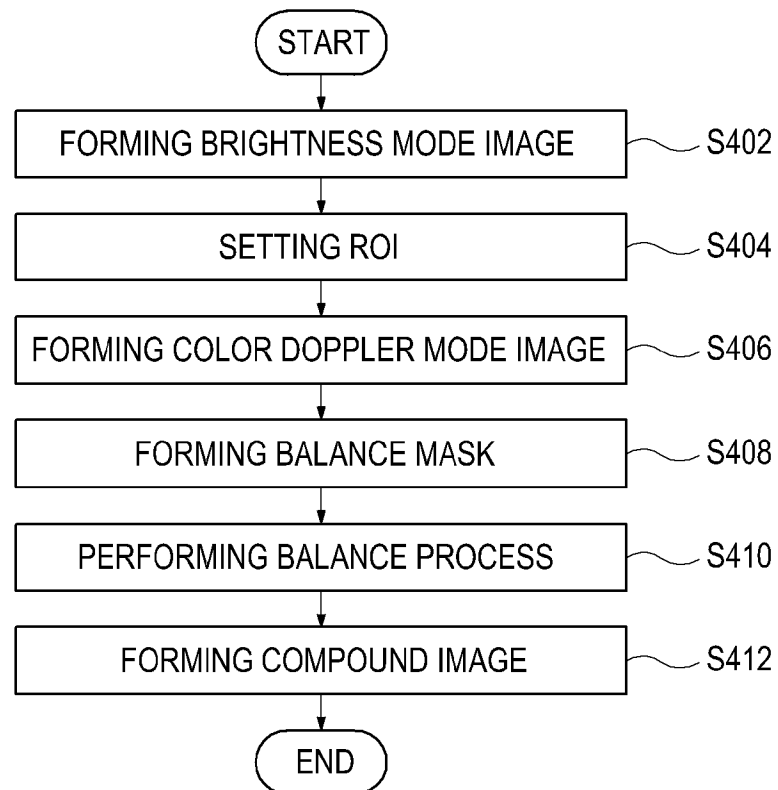


FIG. 5

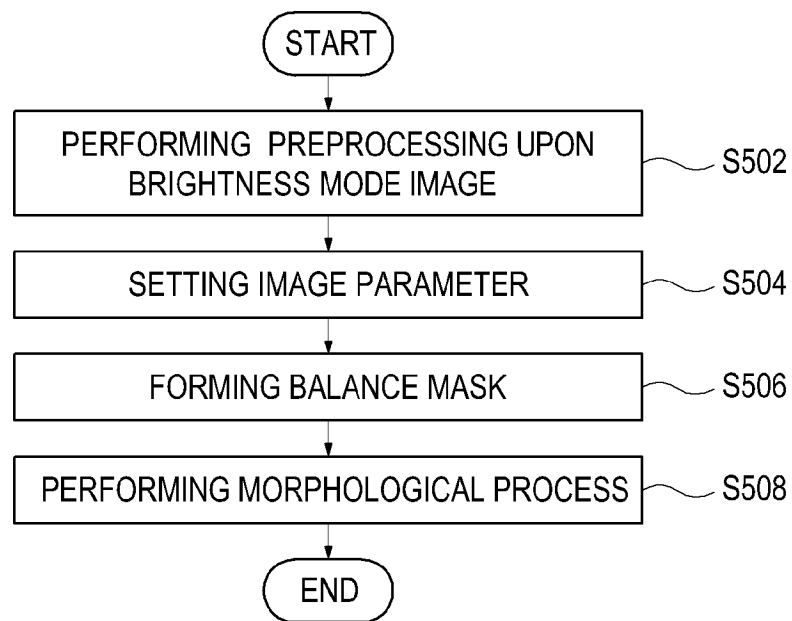


FIG. 6

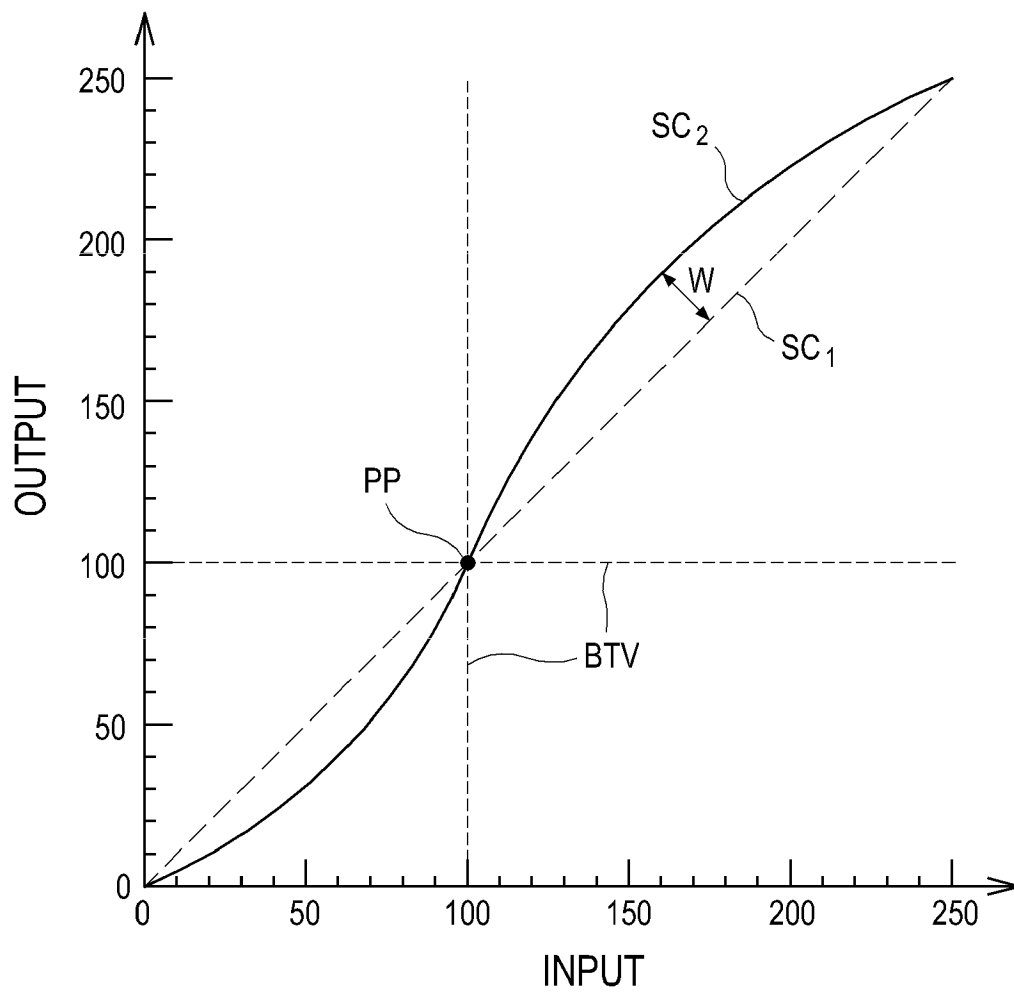


FIG. 7

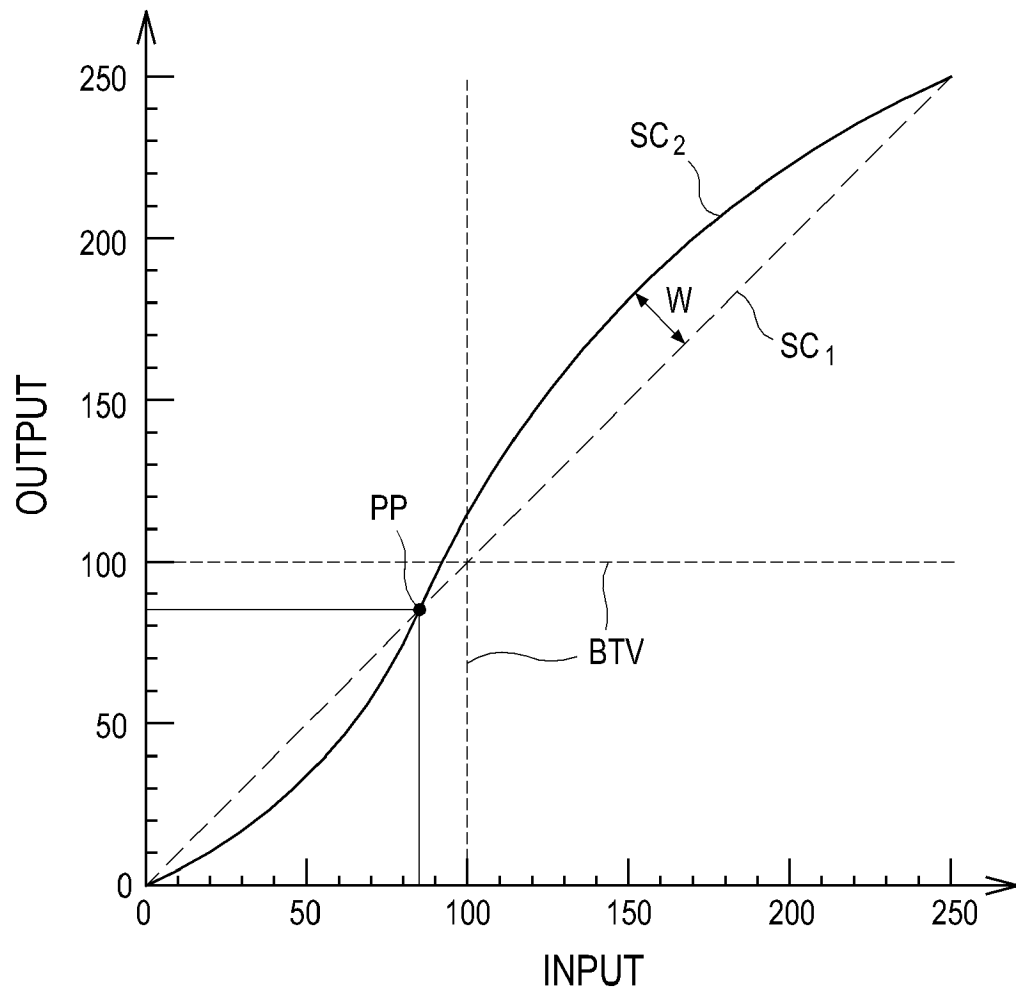


FIG. 8


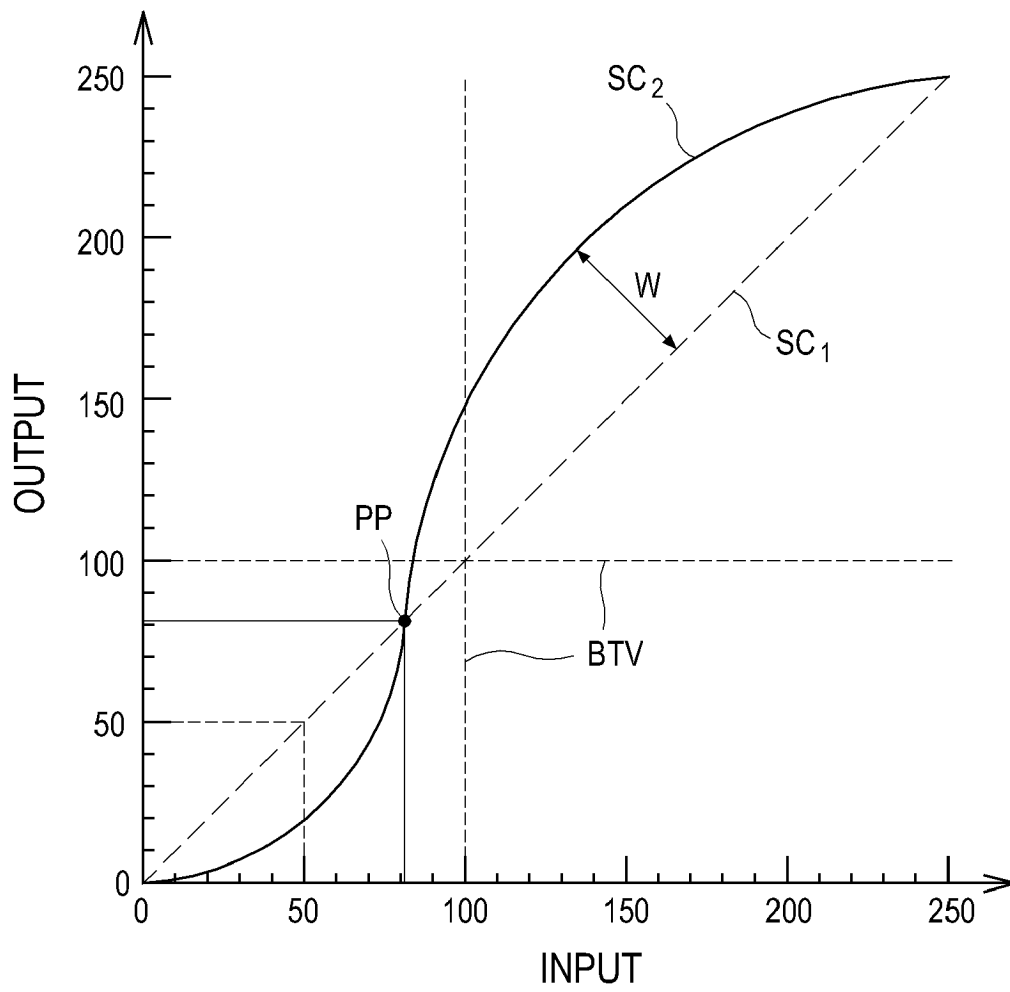


FIG. 9



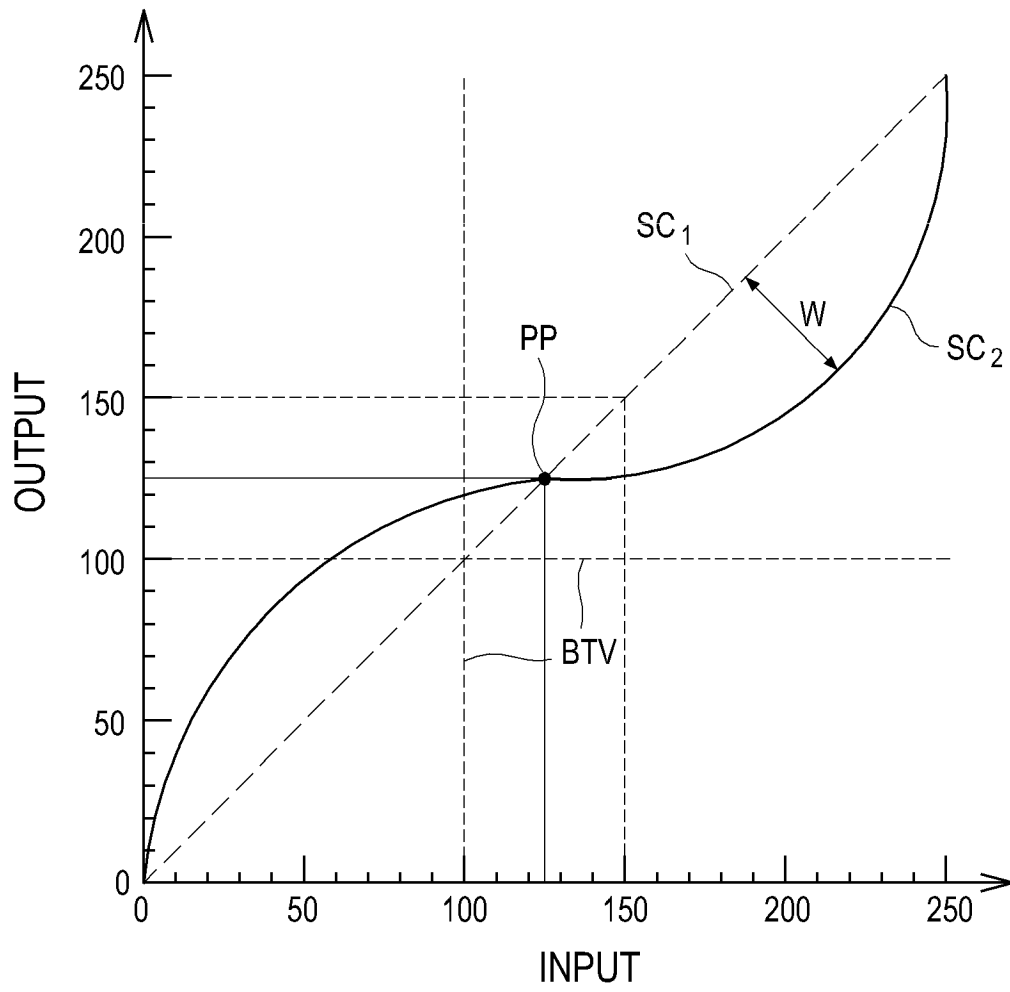

EUROPEAN SEARCH REPORT

Application Number
EP 11 17 6129

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
Y	JACINTA E BROWNE ET AL: "COLOUR DOPPLER SPATIAL RESOLUTION PERFORMANCE TESTING", ULTRASOUND, ROYAL SOCIETY OF MEDICINE PRESS, GB, vol. 15, 1 August 2007 (2007-08-01), pages 162-166, XP007919778, ISSN: 1742-271X, DOI: 10.1179/174313407X208677 * pages 3,8,9 * * page 11, lines 4-6 *	1-15	INV. A61B8/00 G01S7/52
Y	US 2005/059892 A1 (DUBOIS ELIZABETH [US] ET AL) 17 March 2005 (2005-03-17) * paragraphs [0009], [0050] - [0051]; figure 5 *	1-15	
A	US 2004/207760 A1 (FILLIMAN PAUL DEAN [US] ET AL) 21 October 2004 (2004-10-21) * figure 1 *	1-15	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61B G01S
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 14 December 2011	Examiner Metz, Carsten
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

1
EPO FORM 1503 03/82 (P04/C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 11 17 6129

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

14-12-2011

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2005059892 A1	17-03-2005	NONE	
US 2004207760 A1	21-10-2004	NONE	

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 1020100085969 [0001]

专利名称(译)	在超声系统中提供彩色多普勒模式图像		
公开(公告)号	EP2425784A1	公开(公告)日	2012-03-07
申请号	EP2011176129	申请日	2011-08-01
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	LEE JAE KEUN LEE HYEONG DO LEE YONG HO		
发明人	LEE, JAE KEUN LEE, HYEONG DO LEE, YONG HO		
IPC分类号	A61B8/00 G01S7/52 A61B8/08 G01S15/89 G06T7/00		
CPC分类号	G01S7/52071 A61B8/0891 A61B8/469 A61B8/5269 G01S15/8979 G06T7/11 G06T7/155 G06T7/194 G06T2207/10136		
代理机构(译)	SCHMID , WOLFGANG		
优先权	1020100085969 2010-09-02 KR		
其他公开文献	EP2425784B1		
外部链接	Espacenet		

摘要(译)

公开了用于提供彩色多普勒模式图像的实施例。在一个实施例中，作为非限制性示例，超声系统包括：超声数据获取单元，被配置为向活体发送超声信号和从活体接收超声信号以获取第一超声数据和第二超声数据；用户输入单元，被配置为接收与感兴趣区域相对应的输入信息和具有预定亮度值的平衡阈值；处理单元，被配置为分别基于第一和第二超声数据形成对应于感兴趣区域的亮度模式图像和彩色多普勒模式图像，形成用于基于彩色多普勒模式图像执行平衡处理的平衡掩模。关于亮度模式图像和输入信息，并基于平衡掩模对彩色多普勒模式图像执行平衡处理。

FIG. 1

