

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
1 May 2003 (01.05.2003)

PCT

(10) International Publication Number  
WO 03/034922 A1

(51) International Patent Classification<sup>7</sup>: A61B 8/00

(21) International Application Number: PCT/US02/34160

(22) International Filing Date: 24 October 2002 (24.10.2002)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
60/348,446 24 October 2001 (24.10.2001) US

(71) Applicant: CUTTING EDGE SURGICAL, INC.  
[US/US]; 2593 Willow Lane, Gilbertsville, PA 19525 (US).

(72) Inventor: GOODWIN, Mark, R.; 2593 Willow Lane, Gilbertsville, PA 19525 (US).

(74) Agents: PABST, Patrea, L. et al.; Holland & Knight LLP, One Atlantic Center, 1201 West Peachtree Street, N.E., Suite 2000, Atlanta, GA 30309-3400 (US).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,


CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Published:**  
— with international search report  
— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: INTRAOSTEAL ULTRASOUND DURING SURGICAL IMPLANTATION

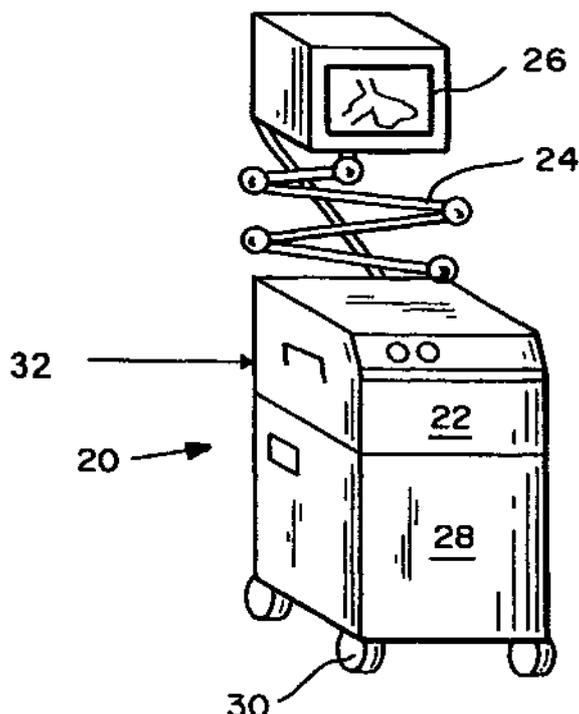

(57) Abstract: IntraOsteal UltraSound (IOUS) is the use of acoustical energy to facilitate "real-time" manipulation and navigation of a device for intraosseous placement of synthetic or biologic implants and to diagnose the condition of the tissue into which the implant is being placed. Representative applications include placement of synthetic or biologic implants, such as bone screws, through vertebral pedicles during spinal fusion surgery. Devices for use in the placement of the implants include a means for creating a lumen or channel into the bone at the desired site in combination with a probe (38) for providing real-time feedback of differences in density of the tissue, typically differences in acoustical impedance between cancellous and cortical bone. The devices will also typically include means for monitoring the feedback (26) such as a screen creating an image for the surgeon as he creates the channel, and/or an audible signal which different tissues are present. The system can also be used for diagnostic applications.



WO 03/034922 A1

## INTRAOSTEAL ULTRASOUND DURING SURGICAL IMPLANTATION

### Background of the Invention

The present invention is generally in the field of methods  
5 and devices for surgical placement of implants, especially into  
bone.

Surgical implantation of devices such as screws, pins, and  
other medical implants into bone is frequently the only means to  
safely immobilize the bone. Typically, this is done by passing a  
10 probe through the cortical bone, the dense, hard bone on the  
outside of bony structures, and into the cancellous bone, the soft,  
compliant spongy bone on the inside of the bone.

As shown in Figure 1, the relevant structures are the  
pedicles 12 and vertebral body 10. These structures are comprised  
15 of two types of bone: cortical 14 and cancellous 16. Cortical bone  
is the dense, hard bone covering the illustrated structures.  
Cancellous bone, commonly referred to as "spongy bone" is "soft"  
and compliant and provides the inner core for these structures.

Surgeons exploit the difference in these two bone types  
20 during pedicular cannulation. When passing a blunt, narrow  
"probe" through the pedicle, the instrument tip tends to follow the  
path of least resistance, the cancellous bone. The operator  
continues to direct this instrument, usually with x-ray assistance,  
until it has penetrated 50-80% of the anterior/posterior diameter of  
25 vertebral body. Successful cannulation is achieved when an intra-  
cancellous pilot channel is created without a breach of the cortical  
bone. A breach can injure critical structures in close proximity,  
such as spinal cord, nerve root, and vessels. The larger the  
cancellous inner core and the thicker the outer cortex, the easier  
30 the task. This is the case, for example, in the lumbar vertebrae,  
particularly the L3-S1 pedicles. However, in ascending the spine

from the lumbar to thoracic and cervical vertebrae, the complexity of the task increases substantially.

Since pedicular cannulation is essentially a "blind" technique, tactile feedback is critical to the operator during creation of the pilot channel. When the boundaries of the bone type are large and well defined, as they generally are in the lumbar pedicles, the relatively thick cortical wall and large core of cancellous bone facilitates intraosteal passage of a blunt tipped probe. The cortical/cancellous boundary is readily detected as the probe is advanced. In higher vertebrae, i.e., thoracic and cervical, the pedicle dimensions decrease markedly. As the overall cross-sectional diameter of the pedicle decreases, so does the cortical wall thickness. As the operator's tactile sensitivity to the cortical/cancellous boundary decreases, the risk for breach increases, even with adjunctive virtual image guidance.

A high complication rate associated with pedicle screw placement in lumbar vertebrae is well documented. As previously stated the risk is even higher in thoracic and cervical spine. Placement of pedicle screws in the cervical vertebrae, with the exception of perhaps C2 and C7, is virtually unheard of. Most posterior fixation procedures of the cervical spine, therefore, are through screw fixation in the lateral masses; not nearly as strong as pedicular fixation.

Since pedicular fixation in many cases provides for maximum construct stability and strength an alternative and improved method and mode of navigation is essential for routine cannulation of these upper vertebral pedicles.

Currently, there is no simple or reliable method to navigate cannulation of vertebral pedicles *in vivo* and in real time during placement of implants. This is a challenging task even in the hands of the most experienced spine surgeon, especially in the

upper thoracic and cervical vertebrae. Current modes of virtual guidance are all based on "historical" data and the images upon which the guidance is dependent do not necessarily present the actual anatomic position at any given instant in real time an  
5 instrument is engaging tissue.

It is therefore an object of the present invention to provide methods and devices to guide cannulation or other procedures within bone or similar types of materials in the body, which are reliable and realtime.

### 10 Summary of the Invention

As defined herein, IntraOsteal UltraSound (IOUS) is the use of acoustical energy, .e., ultrasound, to facilitate "real-time" manipulation and navigation of a device for intraosseous placement of synthetic or biologic implants. Representative  
15 applications include placement of synthetic or biologic implants, such as bone screws, through vertebral pedicles during spinal fusion surgery. Such implants are part of a larger "construct" designed to immobilize unstable vertebrae incorporated by it. The purpose of such a construct is to permit bony fusion of those  
20 unstable vertebrae that contribute to pain or impaired spine function. Devices for use in the placement of the implants include a means for creating a lumen or channel into the bone at the desired site in combination with a probe for providing realtime feedback of differences in density of the tissue, typically  
25 differences in density between cancellous and cortical bone. The devices also typically includes means for monitoring the feedback such as a screen creating an image for the surgeon as he creates the channel.

IOUS can also be used for measurement of bone thickness,  
30 identification and confirmation of pseudoarthrosis in failed spinal fusions, bone-to-avascular-necrosis interface, guidance of pedicle

screws across a vertebral body during anterior spinal deformity corrective surgery, and search for osteoid osteoma and vascular lesions such as aneurismal bone cysts, etc.

### **Brief Description of the Drawings**

5           Figure 1 is a diagram of a thoracic vertebra (T6) showing the pedicles, cortical bones, cancellous bone, and bone screw trajectory for spinal fusion.

          Figures 2a, 2b and 2c are diagrams of a device for use in IOUS, including a computer processor, acoustical generator,  
10           monitor, articulating arm, and transducer input ports. Figure 2a, perspective view; Figure 2b, side view; Figure 2c, top view.

          Figure 3 is a perspective view of a transducer.

          Figure 4 is a perspective view of input means from the transducer to the transducer input port.

15           Figures 5a and 5b are schematics of the process, wherein the computer processor processes the input and output from the acoustical generator and transducer in Figure 5a, to produce an image, shown in Figure 5b.

          Figures 6a-d are perspective views of the instruments used  
20           in the process. Figures 6a and 6b are drill bits of a type currently available modified to incorporate transducers that provide feedback to create an image as the drill bit creates a pilot hole. Figures 6c and 6d are perspective views of an instrument that is both a transducer and capable of creating a pilot hole.

### **Detailed Description of the Invention**

          An IntraOsteal UltraSound (IOUS) based system is used for  
the placement of implants, both initially and/or as the surgeon is  
operating, and for detection and characterization of bone to enable  
the surgeon to determine the precise location to begin surgery to  
30           place the implant, as well as to determine the condition of the  
tissues into which the implant is to be placed.

The system includes a device for sensing and alerting via an auditory or visual signal the absence of bone (cortical, cancerous, cartilaginous) i.e., as would be the case of a bony non-union (pseudoarthrosis), fracture, neoplasms, avascular necrosis, vascular lesions, etc. Such abnormalities will have acoustical properties with echogenicity widely disparate from all normal bone types. The IOUS provides a means to qualitatively recognize or delineate abnormal regions, to insure that any implant being guided and placed is done so in bone of a normal caliber (density, homogeneity, architecture, etc.). The frequency range of bone is such that any quantifiable signal falling outside of a particular range will produce an alert signal that is different than that of a signal produced with normal bone. This is important when navigating from one bony structure to another bony structure across a non-bony interface, i.e., as in joints, especially when implanting facet screws, hip pins, etc.

Effective deployment of IOUS can be predicated on a multiple number of factors or variables that are unique to bone, including:

1. Bone mineral density (BMD).
2. Histology of bone;
3. Bone disease or degeneration
4. Water content (blood, bone marrow, etc.).
5. Cartilage composition.

In its totality, bone, in all of its iterations, combinations and architecture, has a distinct "signature". Its echogenicity, modes of attenuation, scattering coefficients, and other characteristics will always be quite distinct from other soft tissues of the. The array of acoustical properties, i.e., frequency, bandwidth, attenuation characteristics, amplitude, scatter coefficients, will all be unique for each type of bone. Effective navigation involves not only

delineating cortical bone from cancellous bone but the integrity of those elements as well.

## **I. Implants**

5           A number of different types of implants can be placed using the devices described herein. In the simplest embodiment, the implant is a titanium screw or pin which is implanted into a channel created by channeling a probe through the cortical bone into the cancellous bone within the bone to be immobilized.

10           In the preferred embodiment, the bone is a vertebral body and channels are created within the pedicles of adjacent vertebral bodies which are then screwed together. Simply put, this spine construct is analogous to a splint or cast placed on or around long bone fractures until healing (fusion) occurs. Screws can be  
15 removed after the bone has healed.

Other implants that can be used include pedicle screws and hip pins. Implants may be formed of metal, ceramic, polymer, biological materials (including bone), and combinations thereof.

## **II. Devices that can be used to image the area**

20           Devices include at a minimum a probe for moving within the tissue to be imaged and means for applying and/or receiving ultrasound or acoustic energy, and means for transmitting data to an external monitoring means. Optionally, the devices also including means for placement of the implant, and signaling  
25 devices that generate a signal when the probe crosses from one type of tissue to another.

Ultrasound is a form of energy that is quantifiable, reliable, non-ionizing, and relatively inexpensive. The different acoustical properties of cortical and cancellous bone make it amenable to real  
30 time interrogation and delineation during instrument manipulation. There are two modes by which acoustical energy

that is emitted and received *in vivo* could be utilized for reliable guidance:

1. **Visual (Radar):** Though a small transducer mounted on or within a narrow instrument, emission of a predefined acoustical  
5 signal, can, upon reflection, be electronically processed to present the disparate signals, altered by the marked difference in echogenicity of cortical and cancellous bone, into a visual graphic image displaying the relationship of the instrument tip with respect to the cortical/cancellous tissue in both the axial and  
10 sagittal planes.
2. **Auditory (Sonar):** By a process similar to the above, the altered signal can be processed such that when a given threshold is met, e.g., when the instrument tip is in direct contact with cortical bone, an audible tone can be generated alerting the  
15 operator of an impending breach if he were to continue the manipulation at the present trajectory.
3. **Dual Visual/Auditory:** By blending the benefits of both, the operator has constant feedback that would enhance accuracy and efficiency of cannulation.

### 20 III. Methods for Detection and Characterization of Bone

The ultrasound is used to measure or provide analysis of one or more factors or variables, including

1. Bone mineral density (BMD);
2. Histology of bone, i.e., cancellous which is trabecular versus  
25 cortical which is lamellar;
3. disease such as osteoporosis, calcification, pseudoarthrosis or arthritis;
4. water content (blood, bone marrow, etc.);
5. cartilage composition;
- 30 6. lesions, vascular defects, neoplasms, or avascular necrosis.

This information assists in knowing the integrity (ex. normal BMD, low BMD) of where one is going as well as the location (ex. cortical to cancellous) one is going to.

Figures 2a-2c represent a system 20 for use as described  
5 herein. The system 20 includes a computer processing unit  
("CPU") 22, articulating arm 24 connecting a monitor 26 to the  
system 20, a monitor 26, an acoustical generator 28, and  
transducer input port 32. In a preferred embodiment, the system  
20 can be rolled on rollers 30 to the operating room. In another  
10 preferred embodiment, the articulating arm 24 allows for a  
complete 360 degree rotation and height adjustment by the  
surgeon.

The transducer 34 is shown in more detail in Figure 3. The  
transducer 34 includes input and output connections 36 and a  
15 probe 38, typically between about 2 and 4 mm in diameter. The  
transducer emits signals at a defined bandwidth and frequency  
which is conveyed to and from the input/output connections 36 to  
the system 20 via the input port 32.

The signals are processed by the CPU 22 to generate signals  
20 (Figure 5a) sent to the monitor 26, which then displays an image  
of the tissue the probe 38 is passing through. The image 40,  
shown in Figure 5b, indicates the cortical interface as a black area  
42, and the cancellous tissue as a white area 44. Both radial and  
sagittal scans can be used to image the tissue, and to provide  
25 measurements in real time of the tissue being imaged.

Two general types of instruments can be used to create the  
images and pilot holes for the surgeon. These consist of  
instruments such as the drill bits currently in use, modified to  
include a transducer, as shown in Figures 6a and 6b, and  
30 instruments wherein the transducer includes a means of creating  
the pilot hole, as shown in Figures 6c and 6d. The latter may be

made by modifying existing ultrasound probes to include a hard pointed end. Figure 6a shows a hollow drill bit 50, with a burr 52 for creating the hole, typically 4-5 mm in height and about 2-4 mm in diameter, a side scan port 54, a lumen 56, and end for  
5 connection to the input/output means 36. Figure 6b shows a hollow drill bit 60, through which the transducer 38 can be introduced through the hollow lumen 62, and visualize the area through side port 64 or forward slot 66.

Figure 6c shows a "joystick" type of instrument 70. The  
10 diameter 72 is between 4 and 8 mm, typically, with an interior lumen diameter 74 of between 2 and 4 mm. There is a side scan port 76 and forward view port 78. A handle 80 directs the drill 82 through the lumen to create the pilot hole in the bone.

Figure 6d shows a transducer 84 for use in scanning and  
15 drilling a pilot hole. The drill bit 86 is about 2-7 mm in diameter. The input/output means 88 connects to port 90.

IOUS can be used to determine the initial starting location that is optimal for introduction of an implant. For example, the transducer is placed on the lamina and used to detect and  
20 characterize the bone interface where the implant is to be positioned.

IOUS can be used to navigate through the bone as the surgeon prepares the site for implantation, detecting changes from cortical to cancellous to cartilaginous areas, detecting bone to bone  
25 unions, and more clearly defining the area in which the implant is to be placed. For example, IOUS can be used to guide the placement of screws during guidance of pedicle screws across a vertebral body during spinal fusion or during anterior spinal deformity corrective surgery.

30 Further, IOUS can be used as a diagnostic, for measurement of bone thickness, identification and confirmation of




pseudoarthrosis in failed spinal fusions, detection of bone-to-  
avascular-necrosis interface, detection of fractures, and search for  
neoplasms, osteoid osteoma and vascular lesions such as  
aneurismal bone cysts, etc. In general the same equipment and  
5 analytical techniques will be used as for surgical placement.

I claim:

1. A method for guiding and placing an implant within a region of tissues characterized by defined differences in acoustical impedance comprising  
introducing into the region a transducer and receiver for ultrasound or audio signals and  
monitoring differences in acoustical impedance as the transducer and receiver are moved through the region.
2. The method of claim 1 wherein the region is bone and the tissues are cortical bone and cancellous bone.
3. The method of claim 1 wherein the region is a joint and the tissues are soft tissues such as ligaments, tendons or cartilage and bone.
4. The method of claim 1 wherein the method further comprises locating an implant in the region.
5. The method of claim 4 wherein the implant is a metal, ceramic, biological or polymeric implant.
6. The method of claim 5 wherein the implant is screw or pin.
7. The method of claim 6 wherein the implant is placed into the spinal pedicles.
8. The method of claim 1 wherein the method is used to guide the placement of pedicle screws across a vertebral body during anterior spinal deformity corrective surgery.
9. The method of claim 1 wherein the ultrasound is used to measure or provide analysis of one or more factors or variables selected from the group consisting of Bone mineral density (BMD), Histology of bone, disease, water content, cartilage composition, lesions, vascular defects, neoplasms, and areas of avascular necrosis.

10. The method of claim 1 wherein the method is used to determine areas of bony non-union, fracture, or regions between bone.
11. A bone drill bit comprising a transducer and receiver.
12. The bone drill bit of claim 11 further comprising a means for producing a signal when the drill bit encounters regions having different acoustic impedance.
13. A system for use in guiding and placing an implant within a region of tissues characterized by defined differences in acoustical impedance comprising
  - a transducer and receiver for ultrasound or audio signals
  - and
  - means for monitoring differences in acoustical impedance as the transducer and receiver are moved through the region.
14. The system of claim 13 wherein the region is bone and the tissues are cortical bone and cancellous bone, and the system produces a signal when differences in density between the cortical bone and the cancellous bone are detected.
15. The system of claim 13 wherein the device further includes means for cutting tissue or bone.
16. The system of claim 13 further comprising a sensor that detects changes in acoustical impedance.
17. The system claim 16 wherein the sensor produces a detectable signal when there is a change in acoustical impedance.
18. A method of measuring bone characteristics in a region comprising
  - introducing into the region a transducer and receiver for ultrasound or audio signals and
  - monitoring differences in acoustical impedance as the transducer and receiver are moved through the region.

19. The method of claim 18 wherein the bone characteristic is thickness.
20. The method of claim 18 wherein the bone characteristic is identification and confirmation of pseudoarthrosis in failed spinal fusions.
21. The method of claim 18 wherein the bone characteristics is bone-to-avascular-necrosis interface.
22. The method of claim 18 wherein the bone characteristic is an osteoid osteoma or vascular lesion.
23. The method of claim 22 wherein the vascular lesion is a aneurismal bone cyst.

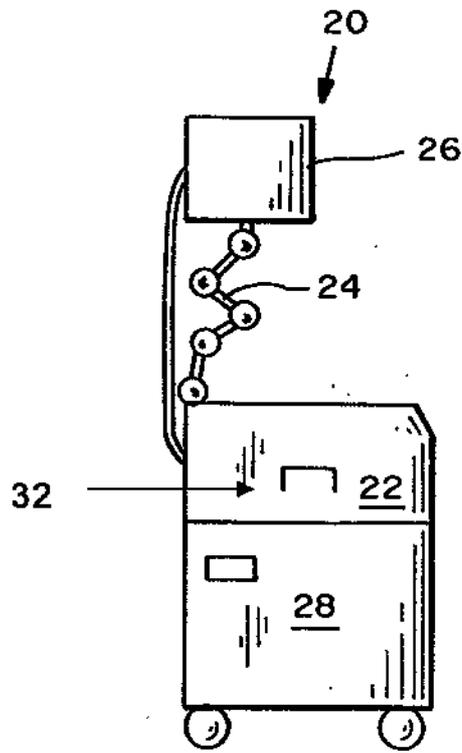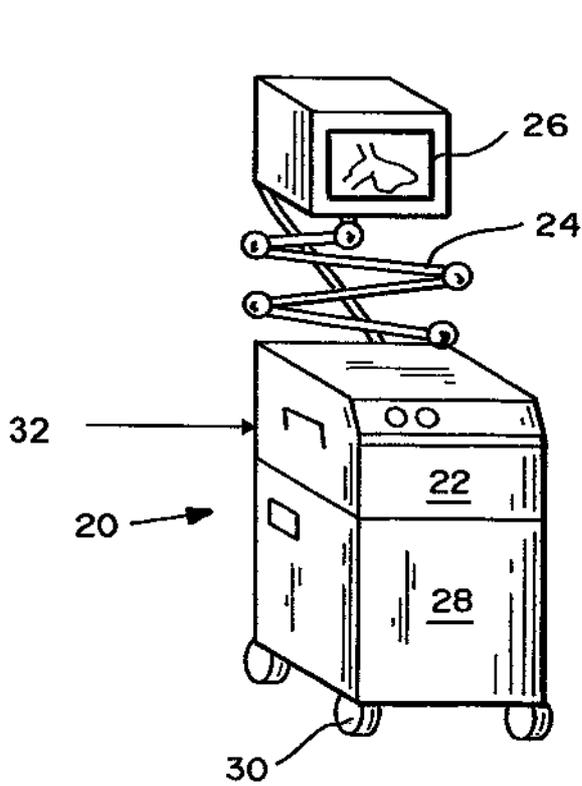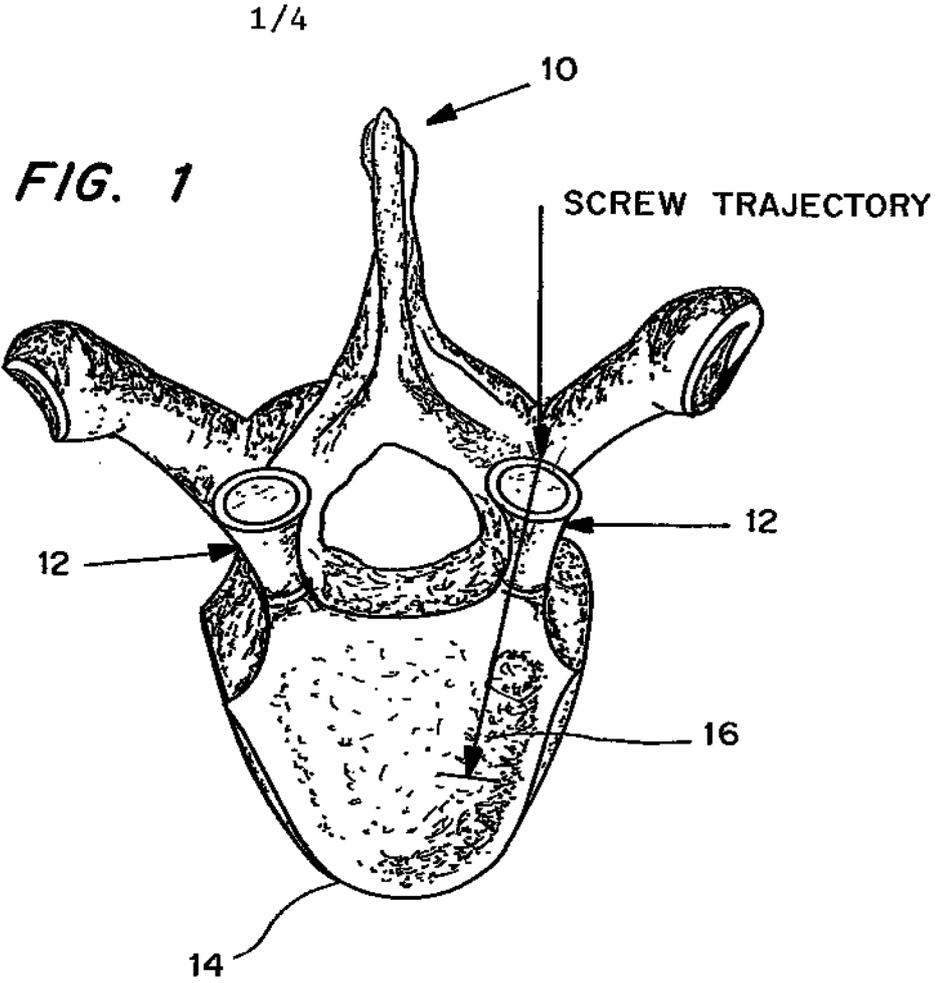

**FIG. 2A**

**FIG. 2B**

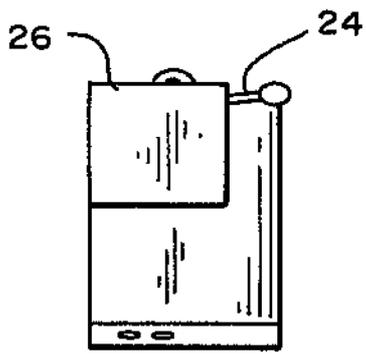


FIG. 2C

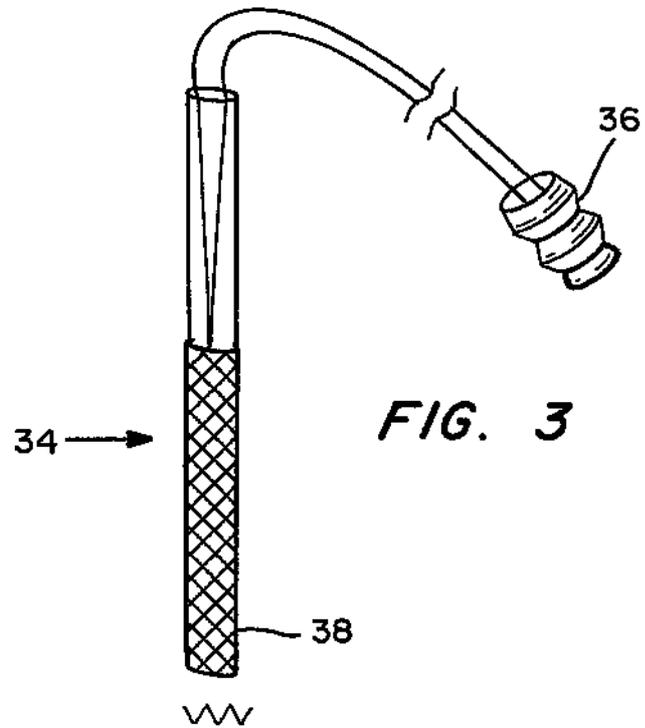


FIG. 3

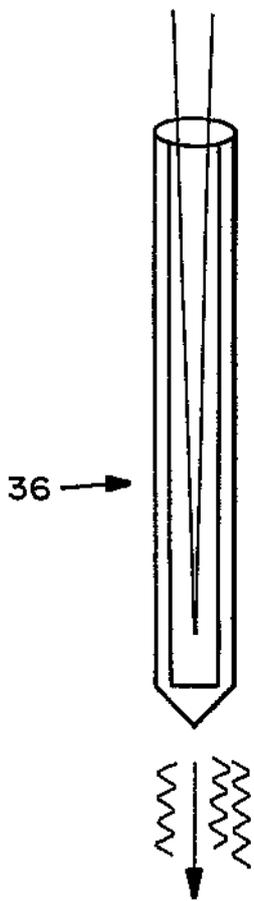


FIG. 4

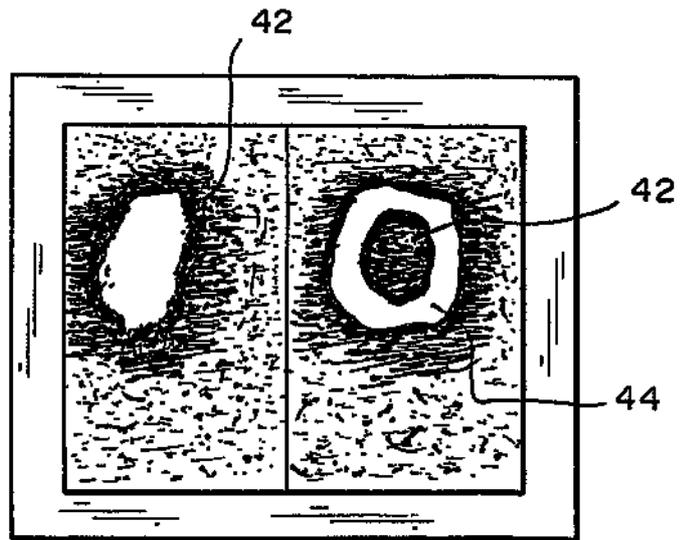


FIG. 5B

FIG. 5A

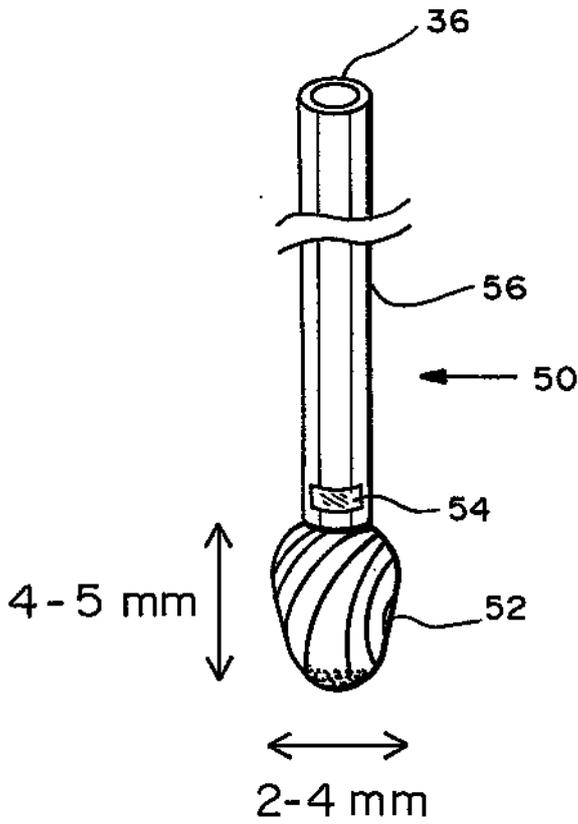
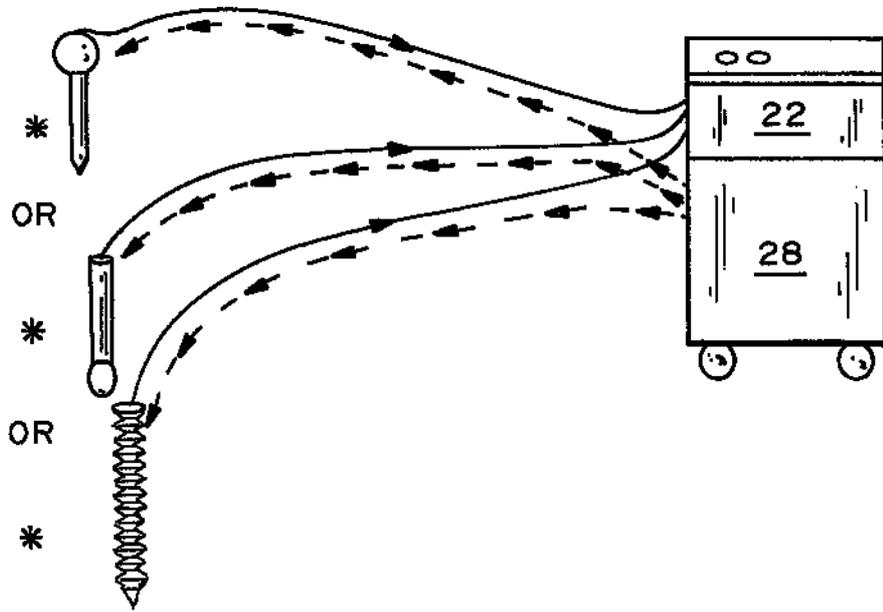


FIG. 6A



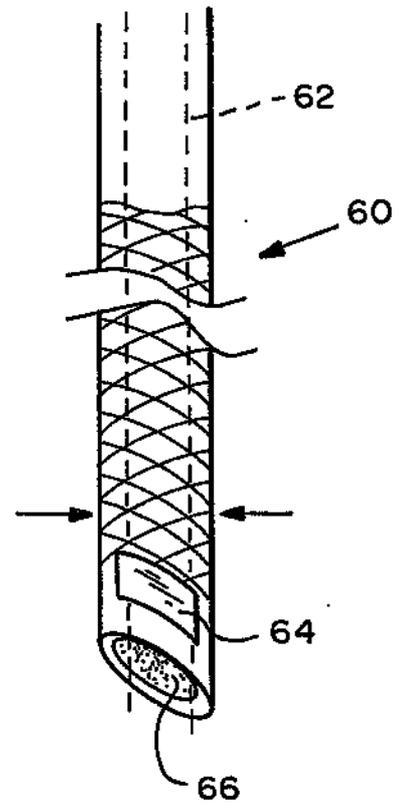


FIG. 6B

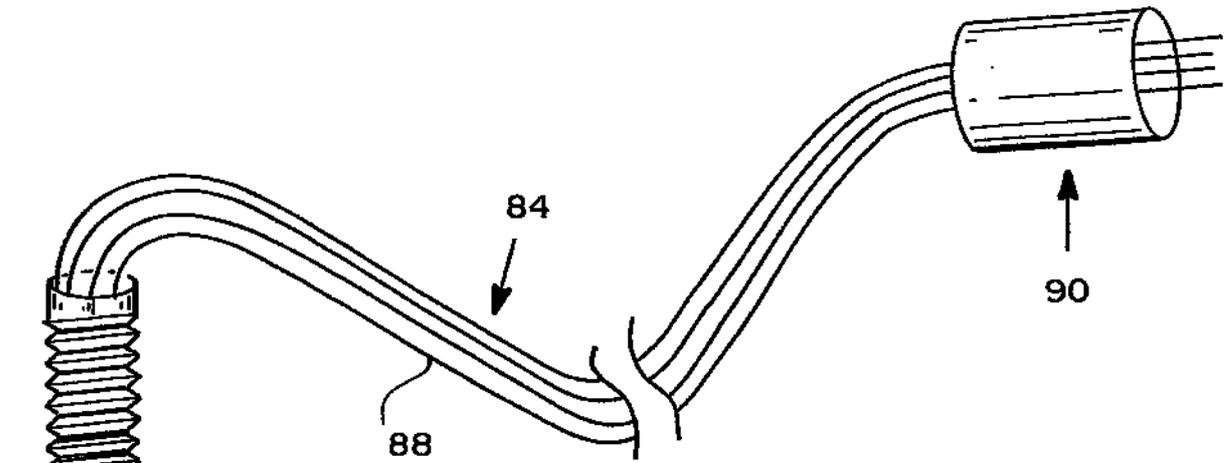

**FIG. 6D**

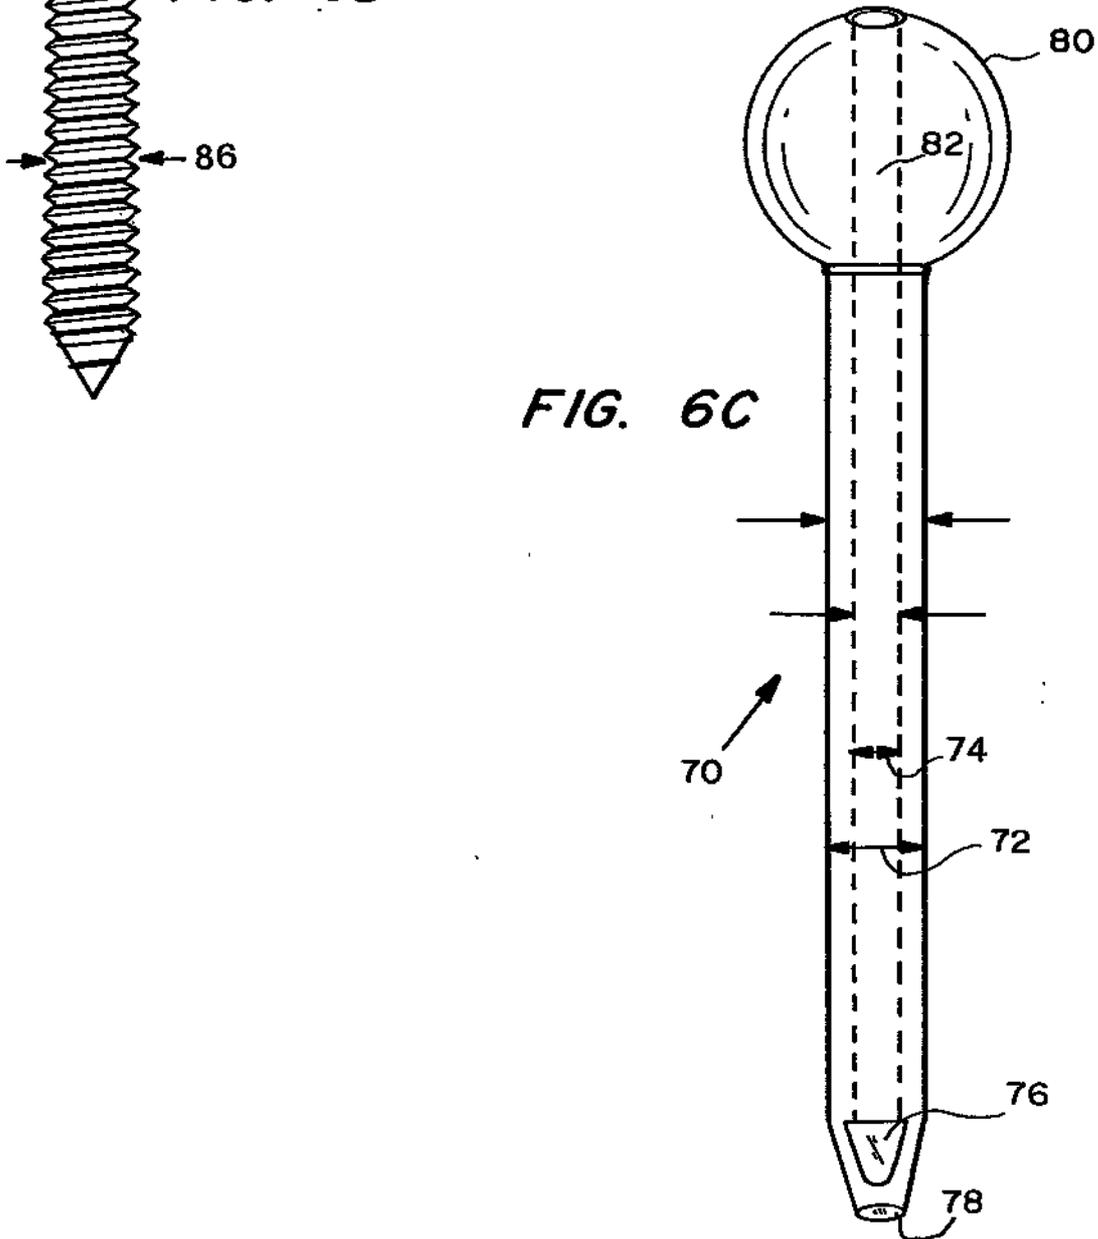

**FIG. 6C**

INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US02/84160

A. CLASSIFICATION OF SUBJECT MATTER

IPC(7) : A61B 8/00  
US CL : 600/489

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 600/437, 439, 443, 447, 459, 471, 594; 606/80-81, 72, 79-80, 96-98

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched  
NONE

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EAST  
search terms: (fuse\$1 or fusi\$2 or vertebra\$1 or pedicle\$1 or arthrodesis or spine or spinal) or implant, and ultraso\$7

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X ---	US 5,957,847 A (MINAKUCHI et al) 28 September 1999, col. 2 lines 29-58	1-2,4-6,10,13-19/3,7-8,20-23
Y	US 6,205,411 B1 (DIGIOIA, III et al) 20 March 2001, col. 6 lines 24-67, col. 12 lines 30-67.	3,7-8,20-23
Y	US 5,309,898 A (KAUFMAN et al) 10 May 1994, col. 1 lines 10-15.	9
Y	US 4,979,939 A (SHIBER) 25 December 1990, col. 5 lines 5 - 22	11-12
Y	US 4,809,689 A (ANAPLIOTIS) 07 March 1989, col. 3 lines 35-39	11-12

Further documents are listed in the continuation of Box C.  See patent family annex.

* Special categories of cited documents:	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"B" earlier document published on or after the international filing date	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Z"	document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means		
"P" document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search  
31 JANUARY 2003

Date of mailing of the international search report  
20 MAR 2003

Name and mailing address of the ISA/US  
Commissioner of Patents and Trademarks  
Box PCT  
Washington, D.C. 20231  
Facsimile No. (703) 805-8230

Authorized officer  
FRANCIS J JAWORSKI  
Telephone No. (703) -808-0858

专利名称(译)	手术植入期间的骨内超声		
公开(公告)号	<a href="#">EP1443859A1</a>	公开(公告)日	2004-08-11
申请号	EP2002773899	申请日	2002-10-24
[标]申请(专利权)人(译)	尖端手术		
[标]发明人	GOODWIN MARK R		
发明人	GOODWIN, MARK, R.		
IPC分类号	A61B8/08 A61B17/58 A61B8/12 A61B17/16 A61B17/17 A61B19/00 A61B8/00		
CPC分类号	A61B17/1626 A61B8/0833 A61B8/0841 A61B8/0858 A61B8/0875 A61B8/12 A61B8/4405 A61B8/463 A61B17/1671 A61B17/1757 A61B90/06		
优先权	60/348446 2001-10-24 US		
其他公开文献	EP1443859A4		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

骨内超声 ( 10US ) 是使用声能来促进用于骨内放置合成或生物植入物的装置的“实时”操纵和导航，并且诊断放置植入物的组织的状况。代表性应用包括在脊柱融合手术期间通过椎骨放置合成或生物植入物，例如骨螺钉。用于放置植入物的装置包括用于在用于提供组织密度差异的实时反馈的探针 ( 38 ) 的所需部位处产生进入骨中的腔或通道的装置，通常是声阻抗的差异松质骨和皮质骨之间。所述装置通常还将包括用于监测反馈 ( 26 ) 的装置，例如在创建通道时为外科医生创建图像的屏幕和/或存在不同组织的可听信号。该系统也可用于诊断应用。