



(11) **EP 2 455 753 A2**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
23.05.2012 Bulletin 2012/21

(51) Int Cl.:
G01N 29/024 ^(2006.01) **G01N 29/06** ^(2006.01)
A61B 8/00 ^(2006.01)

(21) Application number: **11189301.2**

(22) Date of filing: **16.11.2011**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(72) Inventors:
• **Lee, Hyeong Do**
135-851 Seoul (KR)
• **Lee, Jae Keun**
135-851 Seoul (KR)

(30) Priority: **23.11.2010 KR 20100116920**

(74) Representative: **Schmid, Wolfgang**
Lorenz & Kollegen
Patentanwlte Partnerschaftsgesellschaft
Alte Ulmer Strasse 2
89522 Heidenheim (DE)


(71) Applicant: **Samsung Medison Co., Ltd.**
Nam-myun
Hongchun-gun
Kangwon do 250-875 (KR)

(54) **Providing Color Doppler Image Based on Qualification Curve Information in Ultrasound System**

(57) There are provided embodiments for providing a color Doppler image based on qualification curve information. In one embodiment, an ultrasound system comprises: an ultrasound data acquisition unit configured to acquire ultrasound data corresponding to a living body including a moving target object; a storage unit for storing qualification curve information for determining blood flow signals of the target object, clutter signals and noise based on velocity and power components of Doppler sig-

nals; and a processing unit configured to form first Doppler signals based on the ultrasound data, perform a clutter filtering process upon the first Doppler signals to form second Doppler signals, calculate velocity and power components of the second Doppler signals, form a color Doppler image based on the calculated velocity and power components, and perform a blending process upon the color Doppler image based on the calculated velocity and power components and the qualification curve information.

FIG. 1

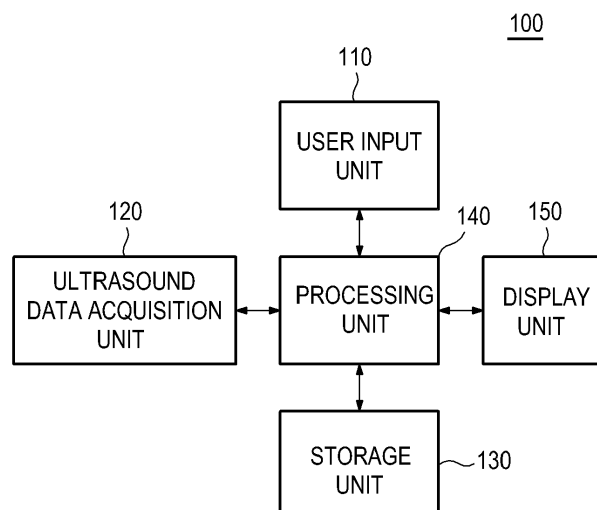

EP 2 455 753 A2

Description

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application claims priority from Korean Patent Application No. 10-2010-0116920 filed on November 23, 2010.

TECHNICAL FIELD

[0002] The present disclosure generally relates to ultrasound systems, and more particularly to providing a color Doppler image based on qualification curve information corresponding to characteristics of Doppler signals in an ultrasound system.

BACKGROUND

[0003] An ultrasound system has become an important and popular diagnostic tool since it has a wide range of applications. Specifically, due to its non-invasive and non-destructive nature, the ultrasound system has been extensively used in the medical profession. Modern high-performance ultrasound systems and techniques are commonly used to produce two-dimensional or three-dimensional ultrasound images of internal features of a target object (e.g., human organs).

[0004] The ultrasound system may provide ultrasound images of various modes including a brightness mode (B mode) image representing reflection coefficients of the ultrasound signals reflected from a target object of a living body with a 2D (two-dimensional) image, a Doppler mode (D mode) image representing speed of a moving target object with spectral Doppler by using a Doppler effect, a color Doppler mode (C mode) image representing speed of a moving target object with colors by using the Doppler effect, and an elastic mode (E mode) image representing mechanical characteristics of tissues object before and after applying a pressure thereto. Particularly, the ultrasound system may transmit and receive ultrasound signals to and from the living body to thereby form Doppler signals corresponding to a region of interest (ROI), which is set on a B mode image. The ultrasound system may further form a C mode image that represents the speed of the moving target object such as blood flow, heart, etc. with colors based on the Doppler signals.

[0005] The color Doppler image may be formed based on Doppler signals obtained by alternately transmitting and receiving ultrasound signals to and from a target object. The Doppler signals may include a low frequency signal (so-called clutter signals) due to the motion of a cardiac wall or valve of a heart. The clutter signals may have amplitude, which is over 100 times than that of the blood flow signals indicative of velocities of the blood flow. The clutter signals may be an obstacle for accurately detecting a velocity of the blood flow. Thus, it is required to remove the clutter signals from the Doppler signals for an accurate velocity detection of the blood flow.

[0006] The ultrasound system typically adopts a clutter filter that may be a high pass filter to remove the clutter signals from the Doppler signals. However, this presents a problem since the clutter filter cannot completely remove the clutter signals from the Doppler signals.

SUMMARY

[0007] There are provided embodiments for providing a color Doppler image based on qualification curve information corresponding to characteristics of Doppler signals in an ultrasound system.

[0008] In one embodiment, by way of non-limiting example, an ultrasound system comprises: an ultrasound data acquisition unit configured to acquire ultrasound data corresponding to a living body including a moving target object; a storage unit for storing qualification curve information for determining blood flow signals of the target object, clutter signals and noise based on velocity and power components of Doppler signals; and a processing unit configured to form first Doppler signals based on the ultrasound data, perform a clutter filtering process upon the first Doppler signals to form second Doppler signals, calculate velocity and power components of the second Doppler signals, form a color Doppler image based on the calculated velocity and power components, and perform a blending process upon the color Doppler image based on the calculated velocity and power components and the qualification curve information.

[0009] In another embodiment, there is a method of providing a color Doppler image, comprising: a) acquiring ultrasound data corresponding to a living body including a moving target object; b) forming first Doppler signals based on the ultrasound data; c) performing a clutter filtering process upon the first Doppler signals to form second Doppler signals; d) calculating velocity and power components of the second Doppler signals; e) forming a color Doppler image based on the calculated velocity and power components; and f) performing a blending process upon the color Doppler image based on the calculated velocity and power components and qualification curve information for determining blood flow signals of the target object, clutter signals and noise.

[0010] This summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This Summary is not intended to identify key or essential features of the claimed subject matter, nor is it intended to be used in determining the scope of the claimed subject matter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011]

FIG 1 is a block diagram showing an illustrative embodiment of an ultrasound system.

FIG 2 is a schematic diagram showing an example of a brightness mode image and a region of interest.

FIG 3 is a block diagram showing an illustrative embodiment of an ultrasound data acquisition unit.

FIG 4 is a schematic diagram showing an example of qualification curve information.

FIG 5 is a flow chart showing a process of forming a color Doppler image.

FIG 6 is a schematic diagram showing an example of transparency.

DETAILED DESCRIPTION

[0012] A detailed description may be provided with reference to the accompanying drawings. One of ordinary skill in the art may realize that the following description is illustrative only and is not in any way limiting.

[0013] Referring to FIG 1, an ultrasound system 100 in accordance with an illustrative embodiment is shown. As depicted therein, the ultrasound system 100 includes a user input unit 110.

[0014] The user input unit 110 is configured to receive input information from a user. In the embodiment, the input information includes information for setting a region of interest RI on a brightness mode image BI, as shown in FIG 2. However, it should be noted herein that the input information may not be limited thereto. The region of interest RI includes a color box for obtaining a color Doppler image. In FIG 2, reference numeral BV represents a blood vessel. The user input unit 110 includes a control panel, a trackball, a mouse, a keyboard and the like.

[0015] The ultrasound system 100 further includes an ultrasound data acquisition unit 120. The ultrasound data acquisition unit 120 is configured to transmit ultrasound signals to a living body and receive ultrasound signals (i.e., ultrasound echo signals) from the living body to acquire ultrasound data. The living body includes a periodically moving target object (e.g., blood flow, a heart, etc.).

[0016] FIG 3 is a block diagram showing an illustrative embodiment of the ultrasound data acquisition unit. Referring to FIG 3, the ultrasound data acquisition unit 120 includes an ultrasound probe 310.

[0017] The ultrasound probe 310 includes a plurality of elements (not shown) for reciprocally converting between ultrasound signals and electrical signals. The ultrasound probe 310 is configured to transmit the ultrasound signals to the living body. The ultrasound probe 310 is further configured to receive the ultrasound echo signals from the living body to output received signals. The received signals are analog signals. The ultrasound probe 310 includes a convex probe, a linear probe and the like.

[0018] The ultrasound data acquisition unit 120 further includes a transmitting section 320. The transmitting section 320 is configured to control the transmission of the ultrasound signals. The transmitting section 320 is further configured to generate electrical signals ("transmitting signals") for obtaining an ultrasound image in consideration of the elements and focusing points. Thus, the ultrasound probe 310 converts the transmitting signals into

the ultrasound signals, transmits the ultrasound signals to the living body and receives the ultrasound echo signals from the living body to thereby output the received signals. The transmitting section 320 includes a transmitting signal forming section (not shown), a transmitting delay time information memory (not shown), a transmitting beam former (not shown) and the like.

[0019] In the embodiment, the transmitting section 320 generates first transmitting signals for obtaining the brightness mode image BI. Thus, the ultrasound probe 310 converts the first transmitting signals into the ultrasound signals, transmits the ultrasound signals to the living body and receives the ultrasound echo signals from the living body to thereby output first received signals. The transmitting section 320 further generates second transmitting signals for obtaining the color Doppler image corresponding to the region of interest RI based on a predetermined ensemble number. Thus, the ultrasound probe 310 converts the second transmitting signals into the ultrasound signals, transmits the ultrasound signals to the living body and receives the ultrasound echo signals from the living body to thereby output second received signals. The ensemble number represents the number of transmitting and receiving the ultrasound signals needed to acquire Doppler signals corresponding to a scan-line.

[0020] The ultrasound data acquisition unit 120 further includes a receiving section 330. The receiving section 330 is configured to convert the received signals provided from the ultrasound probe 310 into digital signals. The receiving section 330 is further configured to apply delays to the digital signals in consideration of the elements and the focusing points to thereby output digital receive-focused signals. The receiving section 330 includes an analog-to-digital converter (not shown), a receiving delay time information memory (not shown), a receiving beam former (not shown) and the like.

[0021] In the embodiment, the receiving section 330 converts the first received signals provided from the ultrasound probe 310 into first digital signals. The receiving section 330 further applies delays to the first digital signals in consideration of the elements and the focusing points to thereby output first digital receive-focused signals. The receiving section 330 further converts the second received signals provided from the ultrasound probe 310 into second digital signals. The receiving section 330 further applies delays to the second digital signals in consideration of the elements and the focusing points to thereby output second digital receive-focused signals.

[0022] The ultrasound data acquisition unit 120 further includes an ultrasound data forming section 340. The ultrasound data forming section 340 is configured to form ultrasound data corresponding to the ultrasound image based on the digital receive-focused signals provided from the receiving section 330. The ultrasound data forming section 340 is further configured to perform a signal process (e.g., gain control, etc) upon the digital receive-focused signals.

[0023] In the embodiment, the ultrasound data forming section 340 forms first ultrasound data corresponding to the brightness mode image BI based on the first digital receive-focused signals provided from the receiving section 330. The first ultrasound data include radio frequency data. However, it should be noted herein that the first ultrasound data may not be limited thereto. The ultrasound data forming section 340 further forms second ultrasound data corresponding to the color Doppler image based on the second digital receive-focused signals provided from the receiving section 330. The second ultrasound data include the radio frequency data or in-phase/quadrature data. However, it should be noted herein that the second ultrasound data may not be limited thereto.

[0024] Referring back to FIG 1, the ultrasound system 100 further includes a storage unit 130. The storage unit 130 stores the ultrasound data (i.e., first ultrasound data and second ultrasound data) acquired by the ultrasound data acquisition unit 120. The storage unit 130 further stores qualification curve information corresponding to the characteristics of Doppler signals.

[0025] In the embodiment, the storage unit 130 stores the qualification curve information for determining Doppler signals (hereinafter, "blood flow signals") by the blood flow, clutter signals by a motion of a blood vessel wall, and a noise from the Doppler signals based on velocity and power components of the Doppler signals. For example, the qualification curve is a curve for determining a first region 410 corresponding to the blood flow signals, a second region 420 corresponding to the clutter signals, a third region 430 corresponding to the noise, a fourth region 440 that the blood flow signals and the clutter signals intermingle, and a fifth region 450 that the blood flow signals and the noise intermingle.

[0026] The ultrasound system 100 further includes a processing unit 140 in communication with the user input unit 110, the ultrasound data acquisition unit 120 and the storage unit 130. The processing unit 140 includes a central processing unit, a microprocessor, a graphic processing unit and the like.

[0027] FIG 5 is a flow chart showing a process of forming the color Doppler image. The processing unit 140 is configured to form the brightness mode image BI based on the first ultrasound data provided from the ultrasound data acquisition unit 120, at step S502 in FIG 5. The brightness mode image BI is displayed on a display unit 150. Thus, the user sets the region of interest RI on the brightness mode image BI by using the user input unit 110.

[0028] The processing unit 140 is configured to set the region of interest RI on the brightness mode image BI based on the input information provided from the user input unit 110, at step S504 in FIG 5. Thus, the ultrasound data acquisition unit 120 acquires the second ultrasound data corresponding to the region of interest RI.

[0029] The processing unit 140 is configured to form Doppler signals (hereinafter, "first Doppler signals") based on the second ultrasound data provided from the

ultrasound data acquisition unit 120, at step S506 in FIG 5. The first Doppler signals include the blood flow signals by the blood flow, the clutter signals by the motion of the blood vessel wall and the noise.

[0030] The processing unit 140 is configured to perform a clutter filtering process upon the first Doppler signals to form the clutter-filtered Doppler signals (hereinafter, "second Doppler signals"), at step S508 in FIG 5. The methods of performing the clutter filtering process are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0031] The processing unit 140 is configured to calculate velocity and power components of the second Doppler signals, at step S510 in FIG 5. The methods of calculating the velocity and power components are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0032] The processing unit 140 is configured to form the color Doppler image based on the calculated velocity and power components, at step S512 in FIG 5. The methods of forming the color Doppler image are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0033] The processing unit 140 is configured to analyze the calculated velocity and power components based on the qualification curve information stored in the storage unit 130 to form qualification analysis information, at step S514 in FIG 5. In the embodiment, the processing unit 140 detects a region corresponding to the calculated velocity and power components among the first to fifth regions 410 to 450 of the qualification curve information, and form the qualification analysis information including the detected region.

[0034] The processing unit 140 is configured to set transparency of the color Doppler image based on the qualification analysis information, at step S516 in FIG 5. For example, the processing unit 140 sets first transparency T_0 of the color Doppler image based on the qualification analysis information that detected region is the first region 410 of the qualification curve information, as shown in FIG 6. The first transparency T_0 is 0. However, it should be noted herein that the first transparency may not be limited thereto. The processing unit 140 further sets second transparency T_1 of the color Doppler image based on the qualification analysis information that the detected region is the second region 420 or the third region 430 of the qualification curve information, as shown in FIG 6. The second transparency T_1 is 1. However, it should be noted herein that the second transparency may be not limited thereto. The processing unit 140 further sets third transparency of the color Doppler image based on the qualification analysis information that the detected region is the fourth region 440 or the fifth region 450 of the qualification curve information, as shown in FIG 6. The third transparency is transparency between the first transparency T_0 and the second transparency T_1 (i.e., 0

< third transparency < 1). That is, the processing unit 140 sets the third transparency close to the first transparency. To as the calculated velocity and power components are closer to the first region 410, and set the third transparency close to the second transparency T_1 as the calculated velocity and power components are closer to the second region 420.

[0035] The processing unit 140 is configured to perform a blending process upon the color Doppler image based on the transparency, at step S518 in FIG 5. In the embodiment, the processing unit 110 performs a transparency process upon the color Doppler image based on the transparency. The processing unit 140 further compounds the transparency-processed color Doppler image on the region of interest RI set on the brightness mode image BI.

[0036] Referring back to FIG 1, the ultrasound system 100 further includes the display unit 150. The display unit 150 is configured to display the brightness mode image BI formed by the processing unit 140. The display unit 150 is further configured to display the color Doppler image formed by the processing unit 140.

[0037] Although embodiments have been described with reference to a number of illustrative embodiments thereof, it should be understood that numerous other modifications and embodiments can be devised by those skilled in the art that will fall within the scope of the principles of this disclosure. More particularly, numerous variations and modifications are possible in the component parts and/or arrangements of the subject combination arrangement within the scope of the disclosure, the drawings and the appended claims. In addition to variations and modifications in the component parts and/or arrangements, alternative uses will also be apparent to those skilled in the art.

Claims

1. An ultrasound system, comprising:

an ultrasound data acquisition unit configured to acquire ultrasound data corresponding to a living body including a moving target object;
a storage unit for storing qualification curve information for determining blood flow signals of the target object, clutter signals and noise based on velocity and power components of Doppler signals; and
a processing unit configured to form first Doppler signals based on the ultrasound data, perform a clutter filtering process upon the first Doppler signals to form second Doppler signals, calculate velocity and power components of the second Doppler signals, form a color Doppler image based on the calculated velocity and power components, and perform a blending process upon the color Doppler image based on the calculated

velocity and power components and the qualification curve information.

2. The ultrasound system of Claim 1, wherein the qualification curve information includes a qualification curve for determining a first region corresponding to the blood flow signals, a second region corresponding to the clutter signals, a third region corresponding to the noise, a fourth region that the blood flow signals and the clutter signals intermingle, and a fifth region that the blood flow signals and the noise intermingle.

3. The ultrasound system of Claim 2, wherein the processing unit is configured to:

detect a region corresponding to the calculated velocity and power components among the first to fifth regions of the qualification curve information;
form qualification analysis information including the detected region; and
perform the blending process based on the qualification analysis information.

4. The ultrasound system of Claim 3, wherein the processing unit is configured to:

set transparency of the color Doppler image based on the qualification analysis information; and
perform the blending process for performing a transparency process upon the color Doppler image based on the transparency.

5. The ultrasound system of Claim 4, wherein the processing unit is configured to:

set first transparency of the color Doppler image based on the qualification analysis information that the detected region is the first region;
set second transparency of the color Doppler image based on the qualification analysis information that the detected region is the second region or the third region; and
set third transparency of the color Doppler image based on the qualification analysis information that the detected region is the fourth region or the fifth region.

6. The ultrasound system of Claim 5, wherein the first transparency is 0, the second transparency is 1, and the third transparency is a transparency between the first transparency and the second transparency.

7. The ultrasound system of Claim 6, wherein the processing unit is configured to:

set the third transparency close to the first transparency as the calculated velocity and power components are closer to the first region, and set the third transparency close to the second transparency as the calculated velocity and power components are closer to the second region or the third region, based on the qualification analysis information that the detected region is the fourth or fifth region.

8. A method of providing a color Doppler image, comprising:

- a) acquiring ultrasound data corresponding to a living body including a moving target object;
- b) forming first Doppler signals based on the ultrasound data;
- c) performing a clutter filtering process upon the first Doppler signals to form second Doppler signals;
- d) calculating velocity and power components of the second Doppler signals;
- e) forming a color Doppler image based on the calculated velocity and power components; and
- f) performing a blending process upon the color Doppler image based on the calculated velocity and power components and qualification curve information for determining blood flow signals of the target object, clutter signals and noise.

9. The method of Claim 8, wherein the qualification curve information includes a qualification curve for determining a first region corresponding to the blood flow signals, a second region corresponding to the clutter signals, a third region corresponding to the noise, a fourth region that the blood flow signals and the clutter signals intermingle, and a fifth region that the blood flow signals and the noise intermingle.

10. The method of Claim 9, wherein the step f) comprises:

- f1) detect a region corresponding to the calculated velocity and power components among the first to fifth regions of the qualification curve information;
- f2) forming qualification analysis information including the detected region;
- and
- f3) performing the blending process based on the qualification analysis information.

11. The method of Claim 10, wherein the step f3) comprises:

- f31) setting transparency of the color Doppler image based on the qualification analysis information; and

f32) performing the blending process for performing a transparency process upon the color Doppler image based on the transparency.

12. The method of Claim 11, wherein the step f31) comprises:

- f311) setting first transparency of the color Doppler image based on the qualification analysis information that the detected region is the first region;
- f312) setting second transparency of the color Doppler image based on the qualification analysis information that the detected region is the second region or the third region; and
- f313) setting third transparency of the color Doppler image based on the qualification analysis information that the detected region is the fourth region or the fifth region.

13. The method of Claim 12, wherein the first transparency is 0, the second transparency is 1 and the third transparency is a transparency between the first transparency and the second transparency.

14. The method of Claim 12, wherein the step f313) comprises:

setting the third transparency close to the first transparency as the calculated velocity and power components are closer to the first region, and setting the third transparency close to the second transparency as the calculated velocity and power components are closer to the second region or the third region, based on the qualification analysis information that the detected region is the fourth or fifth region.

FIG. 1

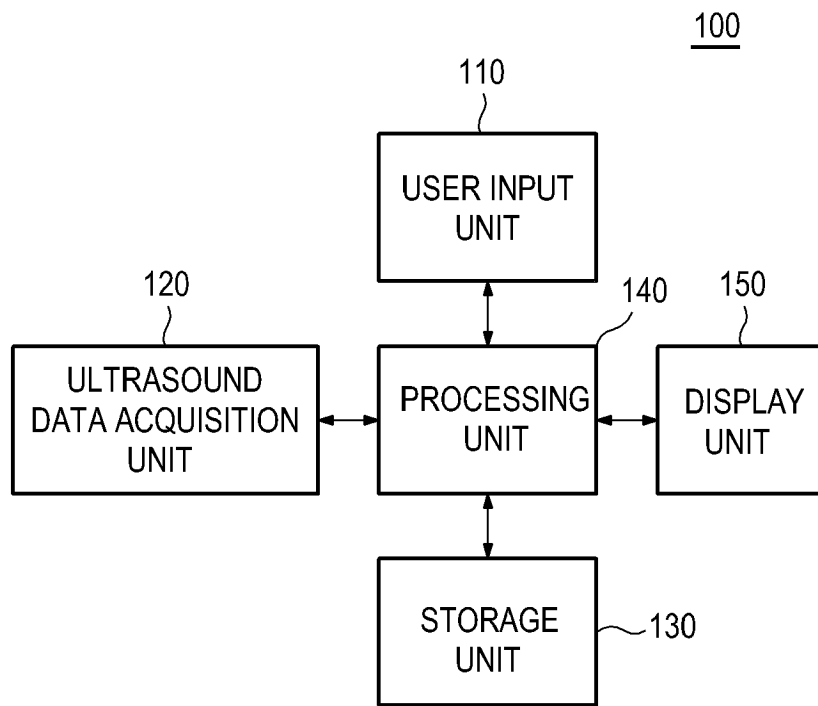


FIG. 2

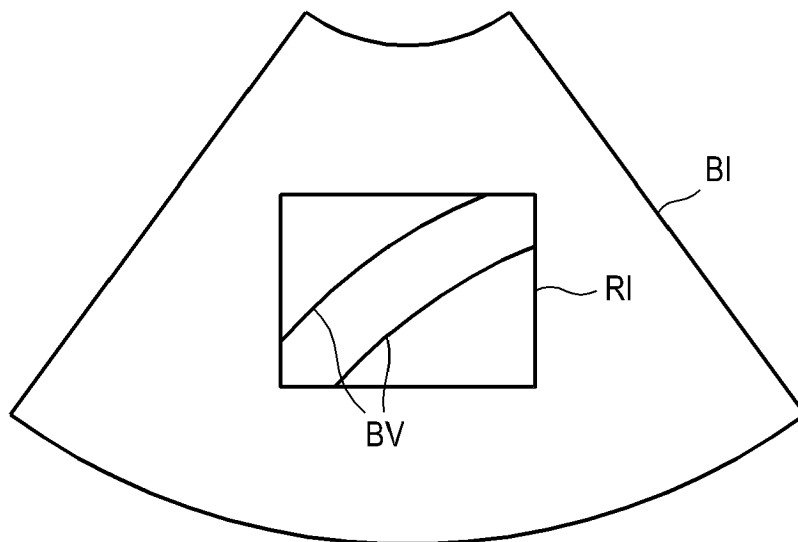


FIG. 3

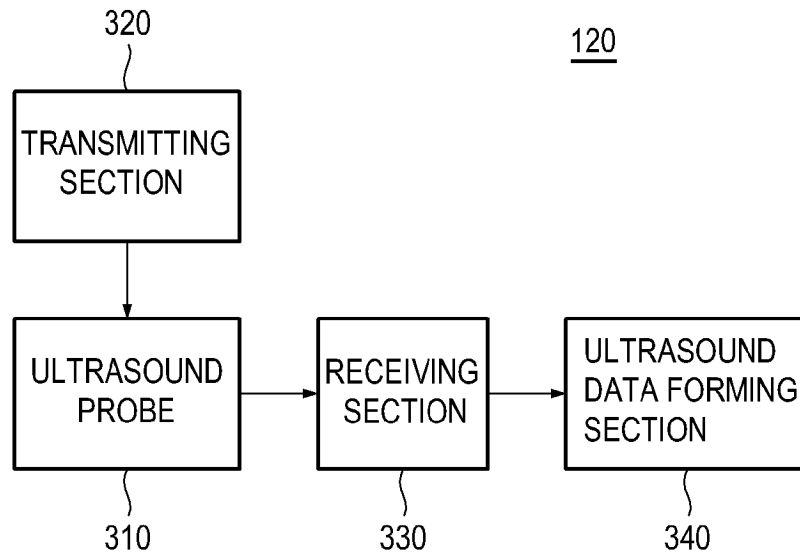


FIG. 4

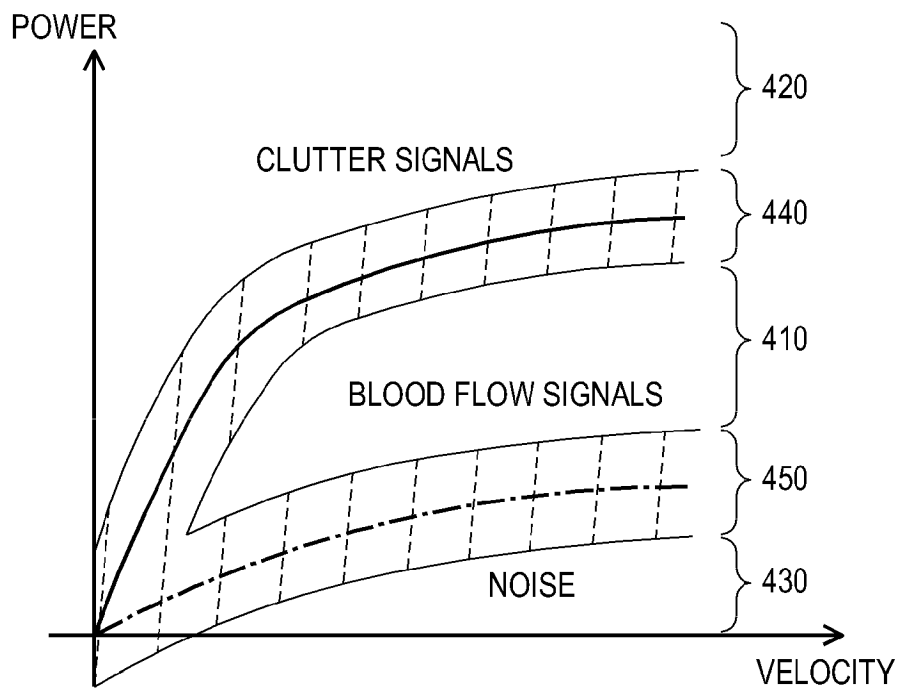


FIG. 5


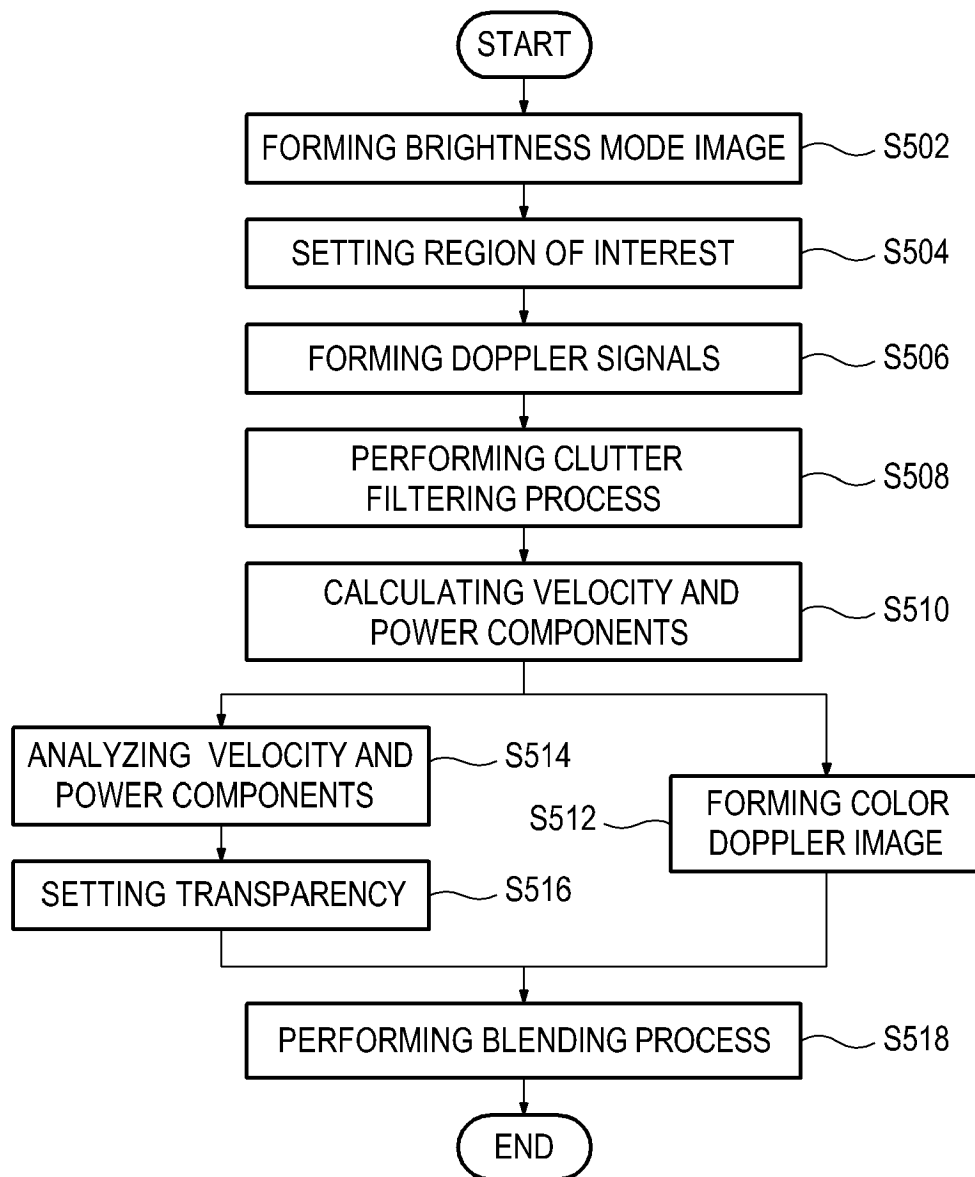


FIG. 6

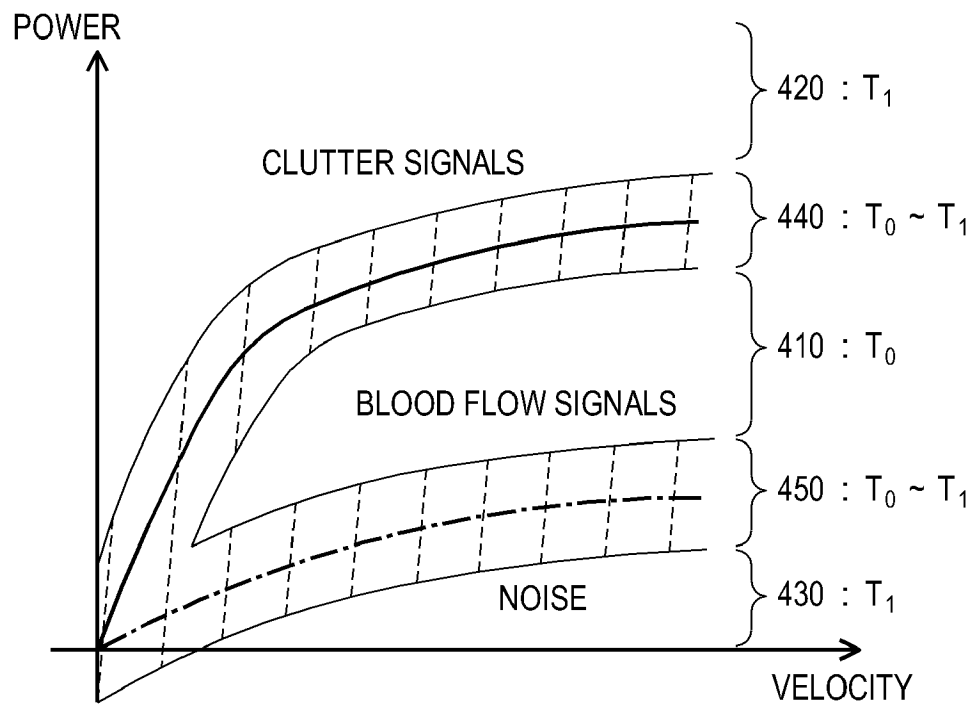

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 1020100116920 [0001]

专利名称(译)	基于资格曲线信息的超声系统彩色多普勒图像提供		
公开(公告)号	EP2455753A2	公开(公告)日	2012-05-23
申请号	EP2011189301	申请日	2011-11-16
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	LEE HYEONG DO LEE JAE KEUN		
发明人	LEE, HYEONG DO LEE, JAE KEUN		
IPC分类号	G01N29/024 G01N29/06 A61B8/00 A61B8/06 A61B8/08 G01S7/52 G01S15/89		
CPC分类号	A61B8/06 A61B8/488 G01N29/024 G01N29/0654 G01N2291/017 G01N2291/02466 G01S7/52071 G01S15/8981 G01S15/8988		
代理机构(译)	SCHMID , WOLFGANG		
优先权	1020100116920 2010-11-23 KR		
其他公开文献	EP2455753A3		
外部链接	Espacenet		

摘要(译)

提供了用于基于限定曲线信息提供彩色多普勒图像的实施例。在一个实施例中，超声系统包括：超声数据获取单元，被配置为获取与包括移动目标对象的活体相对应的超声数据；存储单元，用于存储用于基于多普勒信号的速度和功率分量确定目标对象的血流信号，杂波信号和噪声的鉴定曲线信息；以及处理单元，被配置为基于所述超声数据形成第一多普勒信号，对所述第一多普勒信号执行杂波滤波处理以形成第二多普勒信号，计算所述第二多普勒信号的速度和功率分量，基于计算的速度和功率分量，并且基于计算的速度和功率分量和资格曲线信息对彩色多普勒图像执行混合处理。

FIG. 1

