

(19)



(11)

EP 2 725 983 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

28.02.2018 Bulletin 2018/09

(51) Int Cl.:

A61B 8/06 (2006.01)

(86) International application number:

PCT/IB2012/053315

(21) Application number: **12751605.2**

(22) Date of filing: **29.06.2012**

(87) International publication number:

WO 2013/001503 (03.01.2013 Gazette 2013/01)

(54) **APPARATUS FOR AUTOMATED ULTRASONIC DOPPLER ANGLE AND FLOW VELOCITY ESTIMATION**

VORRICHTUNG FÜR AUTOMATISIERTE ULTRASCHALLDOPPLERWINKEL- UND
FLUSSGESCHWINDIGKEITSMESSUNG

APPAREIL POUR ESTIMATION ULTRASONORE AUTOMATISÉE D'ANGLE DOPPLER ET DE
VITESSE D'ÉCOULEMENT

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **30.06.2011 IN 2236CH2011**

(43) Date of publication of application:

07.05.2014 Bulletin 2014/19

(73) Proprietor: **Koninklijke Philips N.V.**

5656 AE Eindhoven (NL)

(72) Inventors:

- **GUPTA, Lalit**
5656 AE Eindhoven (NL)
- **ANAND, Ajay**
5656 AE Eindhoven (NL)

• **PETRUZZELLO, John**

5656 AE Eindhoven (NL)

• **VAJINEPALLI, Pallavi**

5656 AE Eindhoven (NL)

• **SISODIA, Rajendra Singh**

5656 AE Eindhoven (NL)

• **FIRTION, Celine**

5656 AE Eindhoven (NL)

• **RAMACHANDRAN, Ganesan**

5656 AE Eindhoven (NL)

(74) Representative: **Steffen, Thomas**

Philips Intellectual Property & Standards

High Tech Campus 5

5656 AE Eindhoven (NL)

(56) References cited:

EP-A1- 1 977 694 US-A- 5 555 886

US-A- 5 701 898 US-A1- 2009 306 513

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD OF THE INVENTION

[0001] This belongs to the field of ultrasound velocimetry.

BACKGROUND OF THE INVENTION

[0002] Monitoring a blood flow pattern in the blood vessels of a subject is an important means of assessing the health of the subject. Monitoring blood flow patterns is of importance in maternal and fetal vessels during routine antenatal consultation, carotid artery for stroke screening, lower extremities for Peripheral Arterial Disease (PAD) for example. Especially in the field of obstetrics, measurements of blood flow to the uterus and the fetus is an important means of assessing the adequacy of blood supply to the fetus and hence fetal health or distress.

In ultrasonic velocimetry the velocity of blood flow is measured by the use of Doppler shift experienced by pulsed ultrasound. For the measurement to be accurate, ideally, the beam of ultrasound must be parallel to the blood flow. For measuring the velocity with acceptable accuracy the angle between the direction of flow and the beam, called the Doppler angle, must be below a certain threshold. This threshold is normally 60° and it is not recommended to make measurements when the Doppler angle is greater than this value.

[0003] Even when the Doppler angle is less than 60°, the angle needs to be measured and the velocity estimated needs be corrected for the difference between the ideal, i.e. the beam being parallel to the flow, and the actual Doppler angle. When blood velocity is measured using an ultrasound imaging device, it is possible to ascertain that the Doppler angle is within 60° and measure the angle and correct for it.

However, ultrasound imaging devices with blood velocimetry are expensive and needs a trained radiologist to operate and interpret the results. Thus there has been a need for inexpensive systems, may be without imaging capabilities, but able to carry out ultrasound blood velocimetry.

[0004] US 5,555,886 A discloses an ultrasonic diagnostic system that automatically measures a volumetric flow rate of a vessel presented on a graphical display by estimating the vessel size and direction. The Doppler information signals received from an ultrasonic transducer include frequency components representing fluid flow through a region of interest. The operator selects a vessel represented graphically on the display in which a volumetric flow rate measurement is desired. The ultrasonic diagnostic system then performs a search in a plurality of directions that extend radially outward from a location within the vessel for an upper and a lower set of edge points that correspond to inner wall surfaces of the vessel. Once the upper and lower set of edge points are

identified, curves are fitted through the respective sets of edge points to define respective estimates of the inner wall surfaces. Next, an angular difference between the respective curves and a beam direction of the Doppler information signals is measured. Finally, a volumetric flow rate measurement of the selected vessel can be derived within a region defined by the respective curves and based on the measured angular difference.

10 SUMMARY OF THE INVENTION

[0005] One of the problems encountered in blood velocimetry without imaging is determining the Doppler angle.

15 **[0006]** This document discloses an ultrasound device for measuring blood flow velocity in the blood vessels of a subject according to claim 1. Such a device provides a means of carrying blood velocimetry in a subject where the device has no imaging function. This may provide the advantage that such a device is more economical than a device with imaging functionality. This may further provide the advantage that a user who is not a highly trained ultrasonologist may also carry out blood velocimetry.

25 **[0007]** Further, a non-claimed method of measuring blood flow velocity using Doppler ultrasound is disclosed. A method of determining a Doppler angle for Doppler blood velocimetry in a volume of a body part of a subject, the method comprising the steps of, a receiving step of receiving electrical signals from a two dimensional array of ultrasound transducers, the signals being representative of ultrasound energy reflected from the body part of the subject, the ultrasound energy having been radiated by the two dimensional array, a computation step of computing the Doppler power in a predetermined frequency band received from predetermined locations in the volume, a generating step of generating a first three dimensional array wherein each cell of the array contains the Doppler power value received from a location in the volume with a predefined relationship between the location and the position of the cell in the array, a mapping step of generating a second three dimensional array wherein each cell of the second array contains a binary bit representing whether a the value in the corresponding cell of the first three dimensional array is above a threshold or not, an identification step of identifying a group of adjoining cells that contain the binary bit representing values above the threshold, in each two dimensional array forming the second three dimensional array, a calculation step of calculating the three dimensional coordinates of the centroid of the area covered by each group in each of the two dimensional arrays and an angle calculation step of calculating the angle between a first line joining two centroids nearest to each other in the two adjacent two dimensional arrays and a second line passing through one of the two centroids, the line being parallel to the radiated ultrasound.

[0008] With this, the angle between the beam of ultra-

sound and the blood vessel is known and may be used to correct measured values of blood velocity in a known way. This enables a method of carrying out blood velocimetry without the need for a device with imaging capability. It is to be understood that the method may also be used in a device with imaging capability also to correct the measured values of blood flow velocity, using the Doppler angle calculated using the method.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] These and other aspects will be described in detail, by way of example, on the basis of the following embodiments and implementations, with reference to the accompanying drawings, wherein:

- Fig. 1 is a two dimensional array of Ultrasound transducer elements;
- Fig. 2 is an embodiment of the disclosed device;
- Fig. 3 is a representation of the disclosed method;
- Fig. 4 is a representation of an aspect of the disclosed method;
- Fig. 5 is a representation of another aspect of the disclosed method;
- Fig. 6a is a representation of an aspect of the disclosed method;
- Fig. 6b is a representation of an aspect of the disclosed method;
- Fig. 6c is a representation of an aspect of the disclosed method; and
- Fig. 6d is a representation of an aspect of the disclosed method;

in which, like reference numerals refer to like parts in the different figures.

DETAILED DESCRIPTION OF EMBODIMENTS

[0010] Fig. 1 shows an ultrasound transducer 100 that is used with the disclosed device and the arrangement of transducer elements therein. The transducer arrangement consists of a plurality of transducer elements arranged in a two dimensional array. The Fig. 1 shows a 32 element transducer arranged in six rows. The rows at the top and bottom of the array have four elements each and there are four rows of six elements each between them. However, this is only an exemplary arrangement and other arrangements may also be used. It is also possible that the size of the transducer elements and their shape may be different. A characteristic of the transducer array is that the individual transducer elements are activated independently of one another and are not driven to steer the beam with phase shifted signals. Such an array as the one in Fig. 1 may be driven to produce a collimated beam of ultrasound in a known way. During Doppler data acquisition, the elements may be driven either sequentially or in groups such that the acoustic signal from one transducer does not affect the others that

are driven at the same time.

[0011] Fig. 2 shows the disclosed device 200 schematically. The elements of the transducers are driven, as described before with reference to Fig. 1, by the driver 201. The transducers receive the reflected ultrasound energy and convert them to electrical signals. The signals provided by the individual transducer elements are analyzed by the analyzer 203 to compute the Doppler power at a known number of points in the sample volume and stores them in a three dimensional array .

An angle determining unit 207 uses this three dimensional array to determine the angle, at each point of the sample volume from which Doppler data has been acquired, between the ultrasound radiation at the point and the direction of the vessel at the point. The angles thus calculated are the Doppler angles at each point in the sample volume. A Doppler velocity calculator 209 uses the Doppler data and the determined angle to determine the velocity of blood flow at all points at which the Doppler angle is less than 60°.

[0012] The blood flow velocities, corrected for the Doppler angle are conveyed to the user suitably using the user interface 211. It is to be understood that the user interface itself need not be a part of the device and may be an external unit to which the calculated velocities are sent in a wired or wireless means for being conveyed suitably to the user. This could for instance be a printer or a general purpose computer or a mobile device. However, it may be more useful to have the user interface as a part of the device itself so that the device is a stand-alone unit that needs no interaction with other devices or systems.

[0013] It is possible that due to the anatomy of the vessels in an individual subject or the position of the transducer on the subject or both, none of the calculated Doppler angles are below 60° or that at very few points in the sample volume are the Doppler angles less than 60°. The device may be configured to convey to the user, in such cases, that the position of the transducer on the subject be changed for useful measurement to be made.

[0014] A method of determining the Doppler angle during Doppler blood velocimetry is also disclosed hereby. This describes the method of processing the reflected ultrasound energy pulses received and converted to electrical signals by a transducer. The transducer has a sparse array of transducer elements as described with reference to Fig. 1 and the disclosed device above.

The received signal is processed for Doppler power. The frequency range chosen for this is 300-2500 Hz, which is, typically, representative of blood flow. The Doppler data is acquired from points in the scan volume at step lengths of 2 mm, for example, from each element of the transducer, in a direction perpendicular to the surface of the transducer elements. Doppler data may be acquired at any chosen step lengths and 2 mm is normally deemed sufficient since, usually, no vessel of interest is smaller than 2 mm in diameter. Doppler data is acquired up to a distance of 10 cm from the transducer or the skin surface

of the subject or any other suitable starting and ending point. The analyzed data is used to generate a three dimensional representation of flow in the scan volume.

[0015] It is to be understood that the numerical values above are mentioned for the sake of explanation. However, it is possible to vary these values to suit a particular application. Or that the devices are built based on this disclosure, which have a varying values and ranges to make the device applicable in cases in which the values are different from those stated. For instance the frequency range may be wider to accommodate the measurement of a larger blood velocity caused by a stenosis. Or that the step lengths smaller than 2 mm - in case of infants which may have blood vessels of a much smaller cross sectional diameter, and so on. All such variations are deemed to be covered under the scope of this disclosure.

[0016] For the further description, it is assumed that the step length chosen is in fact 2 mm and that the transducer is a 32 element transducer as described before. Further, each transducer element face is assumed to be a square with the dimensions 10 mm by 10 mm. With this, the flow information that results may be arranged in a 3 dimensional array which has 6 rows, 6 columns and 50 layers, except for the top and bottom rows, which have only 4 transducer elements. Thus, the four corner cells of each layer will have no Doppler power information in them. Except for the said cells, each cell of this array contains information in terms of Doppler power measured. This data is used to create a second array that is a replica of the first array in structure but has a digital '1' in all those cells that have a Doppler power value greater than a predetermined threshold and a digital '0' in all those cells that have a Doppler power value less than or equal to that threshold. The threshold is chosen such that noise and spurious signals do not interfere with the delineation of the vessels.

[0017] This three dimensional array is visualized as the flow map in three dimensions from which the vessels in the sample volume are delineated. That means, the three dimensional array may be visualised as having dimensions in the real world matching the volume of the subject's body from which the reflected radiation is received and processed. Thus each cell of the array has the dimensions corresponding to the dimensions of the radiating surface of the transducer elements and the distance between layers is visualised to have the step lengths at which the Doppler power is received and processed. This visualisation of the array as having physical dimensions is key to the disclosure.

[0018] In each layer of the array all neighbouring cells containing a '1' are considered to belong to the same vessel. This group of cells containing adjoining 1's are deemed to represent the cross section of a vessel in a plane formed by each layer. Thus we get cross sections of the vessels separated by distances of 2 mm in the direction of the layers of the array.

[0019] Once the sections are determined, the centroid of each of them is determined in a known way. Starting

from any layer, the nearest centroids on the two adjacent layers are treated as belonging to the same vessel. Thus a line joining all such centroids is deemed to be the centre line of each of the vessels in the sample volume. Once these vessels are thus delineated, the vessel is treated as piecewise linear and the angle between each line joining two nearest centroids and a line at each centroid perpendicular to the section and in the direction of the transducer may be determined in a known way. Each of these angles so measured is the Doppler angle at that point.

[0020] The smallest angle determined, i.e., a point at the centre of the cross section of the vessel at which the ultrasound beam is closest to being parallel to the vessel is extracted and the Doppler power information from the first three dimensional array belonging to the cell closest to the centroid is used to calculate the velocity information using the formula:

$$v = \frac{Fs * c}{2 * Ft * \cos(th)}$$

wherein, v denotes the velocity of blood flow in an artery at a particular point, Fs represents the Doppler frequency shift, c represents speed of sound in the medium, th represents the angle between the probe and the vessel and Ft represents the frequency of the probe. This could be seen with reference to Fig. 4 as in step 427, the initial velocity is calculated and in step 429 the final or corrected velocity is calculated.

[0021] It is possible that due to the position of the transducer on the surface of the abdomen of the subject, and the path of the vessel relative to the transducer, none of the Doppler angles calculated as described above has a value less than 60°. In one variant of the method, an information that the position of the probe needs to be changed, since the current position is not suitable for velocimetry with sufficient accuracy, may be conveyed to the user, in such cases. This is shown in Fig 5. The number of locations where the calculated angle is less than the predetermined threshold is counted and in step 531, the number is compared with a predetermined number. If the counted number is less than the predetermined number the information may be conveyed to the user suitably to change the position of the transducer on the surface of the subject's body. It is to be understood that the word position here may mean the location on the subject, the angle or tilt and orientation and so on. Needless to say, the process may be repeated till reliable values of the velocity of blood flow are determined i.e., at least one Doppler angle value less than 60° is obtained.

[0022] In another variant of the method, the velocities of blood flow at different points on the vessel that meet the criteria, viz., where the Doppler angle is less than 60°, may be calculated and the attention of the user may be suitably drawn to any large difference between them. A large difference in velocities may be indicative of an obstruction in the vessel or a hemorrhage.

[0023] It is also conceivable that the Doppler data for all the cells adjacent to the centroid are used to calculate the velocities at each of those cells and the average of the velocities may be obtained to determine the blood flow velocity and then corrected for the Doppler angle. Alternatively, the average of values stored in all the cells adjacent to the centroid is first determined and using this average, the velocity is determined and then corrected for the Doppler angle.

[0024] The description hitherto is with the assumption that the sections are obtained and the flow mapped at the layers of the array as shown in Fig. 6a. The visualisation of the array, for purposes of understanding, is shown in 6b. It is to be understood that this is not the only way of delineating the vessels. It is equally possible to do it with the other two planes perpendicular to the one shown in 6a. These are indicated in Fig. 6b and in Fig 6c with suitable modifications in the calculations that follow. Knowing the normal anatomy of the vessels being considered for velocimetry and the position of the probe it may be advantageous to choose one of the three possibilities. In all the three figures, the arrow indicates the direction of insonation or radiation of the collimated beam of ultrasound. The description hitherto has assumed that the vessel structures are always distinct enough to delineate the vessels uniquely based on the method described. However in reality it is possible that the vessels are twisted or cross over each other such that the vessels when delineated based on the method described will at some point cross over. In other words the flow is mapped for one vessel for a certain distance (certain number of contiguous centroids) and then a centroid belonging to another vessel is treated as the next contiguous centroid. Thus once the centroids are determined and the flow is mapped, the Doppler data stored in the array are compared in a known way to determine if they actually belong to the same vessel or not. The comparison may be based on cross correlation or any other numerical comparison method. An alternative may be to use the Cross Teager-Ville distribution or cross Wigner-Ville distributions, for instance. The blood flow has characteristics that remain substantially the same along a given blood vessel. By comparing these characteristics at different points in the vessel it may be confirmed that the mapping of the vessels has been carried out correctly. In case this test shows that the mapping is incorrect, by repositioning the transducer better results could easily be obtained.

[0025] While the embodiments have been described in detail in the drawings and description, such drawings and description are to be considered exemplary and not restrictive; the invention is not limited to the disclosed embodiments.

[0026] For example, it is possible to practice the invention in an arrangement wherein there are more than one computer memory units to store the three dimensional arrays. Similarly, the steps of methods disclosed in different embodiments may be combined with advantage.

[0027] Other variations to the disclosed embodiments

can be understood and effected by those skilled in the art, in practicing the claimed invention, from a study of the drawings, the disclosure, and the appended claims. In the claims, the word "comprising" does not exclude elements or steps other than those mentioned, and the indefinite article "a" or "an" does not exclude a plurality. A single processor or other unit may fulfill the functions of several items recited in the claims. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage.

Claims

1. An ultrasound device (200) for measuring blood flow velocity in a blood vessel of a subject, the measurement depending on reflections from a volume of a subject's body part of a collimated beam of ultrasound energy radiated by an ultrasound transducer (100) along a beam direction into the volume of the subject's body part, the device comprising:

a signal input unit (203) for receiving electrical signals representative of the reflected ultrasound energy received by each transducer element (101) of the ultrasound transducer (100) including a two dimensional array of transducer elements;

an analyzer (205) for analyzing the signals for generating a representation of blood flow at a plurality of predetermined locations in the volume and calculating a first blood flow velocity at each of the locations;

a delineating unit (207) for delineating the blood flow in the blood vessel in the volume from the representation of blood flow;

an angle calculating unit (209) for calculating, at a plurality of points in the delineated blood flow, a Doppler angle between the beam direction of the radiated collimated beam of ultrasound energy and a direction of the blood flow, said direction of the blood flow depending on the delineation; and

a velocity calculator (211) for calculating a second blood flow velocity at the plurality of points based on the calculated first velocities at the plurality of locations and the calculated Doppler angle at the plurality of points for conveying the second blood velocity to a user.

2. The device of claim 1 wherein the second blood flow velocity at any point of the plurality of points is determined only if the Doppler angle at that point is less than a predetermined value.

3. The device of claim 1, wherein the angle calculating unit (209) is for conveying to the user an information

to change a position of the transducer on the subject when the number of the Doppler angles determined that are below the predefined value is less than a predefined number.

5

Patentansprüche

1. Ultraschallvorrichtung (200) zum Messen von Blutflussgeschwindigkeit in einem Blutgefäß eines Subjekts, wobei die Messung von Reflexionen, aus einem Volumen eines Körperteils eines Subjekts, eines kollimierten Ultraschallenergiestrahls abhängt, der von einem Ultraschallwandler (100) entlang einer Strahlrichtung in das Volumen des Körperteils des Subjekts ausgesendet wird, wobei die Vorrichtung umfasst:

10

eine Signaleingangseinheit (203) zum Empfangen von elektrischen Signalen, die für die von jedem Wandlerelement (101) des Ultraschallwandlers (100), der ein zweidimensionales Array aus Wandlerelementen einschließt, empfangene reflektierte Ultraschallenergie repräsentativ sind;

15

einen Analysator (205) zum Analysieren der Signale, um eine Darstellung des Blutflusses an einer Vielzahl von vorbestimmten Stellen im Volumen zu erzeugen und eine erste Blutflussgeschwindigkeit an jeder der Stellen zu berechnen;

20

eine Abgrenzungseinheit (207) zum Abgrenzen des Blutflusses im Blutgefäß in dem Volumen von der Blutflussdarstellung;

25

eine Winkelberechnungseinheit (209) zum Berechnen eines Dopplerwinkels zwischen der Strahlrichtung des abgestrahlten kollimierten Ultraschallenergiestrahls und einer Richtung des Blutflusses an einer Vielzahl von Punkten in dem abgegrenzten Blutfluss, wobei die Richtung des Blutflusses von der Abgrenzung abhängig ist; und

30

einen Geschwindigkeitsrechner (211) zum Berechnen einer zweiten Blutflussgeschwindigkeit an der Vielzahl von Punkten basierend auf den berechneten ersten Geschwindigkeiten an der Vielzahl von Stellen und dem berechneten Dopplerwinkel an der Vielzahl von Punkten, um die zweite Blutflussgeschwindigkeit an einen Benutzer zu übermitteln.

35

40

45

50

2. Vorrichtung nach Anspruch 1, wobei die zweite Blutflussgeschwindigkeit an einem beliebigen Punkt aus der Vielzahl von Punkten nur bestimmt wird, wenn der Dopplerwinkel an diesem Punkt kleiner als ein vorbestimmter Wert ist.

55

3. Vorrichtung nach Anspruch 1, wobei die Winkelbe-

rechnungseinheit (209) dazu dient, dem Benutzer eine Information zu übermitteln, eine Position des Wandlers auf dem Subjekt zu verändern, wenn die Anzahl der bestimmten Dopplerwinkel, die unter dem vordefinierten Wert liegen, kleiner als eine vordefinierte Anzahl ist.

Revendications

1. Dispositif ultrasonore (200) pour mesurer la vitesse d'écoulement sanguin dans un vaisseau sanguin d'un sujet, la mesure dépendant de réflexions à partir d'un volume d'une partie corporelle d'un sujet, d'un faisceau collimaté d'énergie ultrasonore émise par un transducteur ultrasonore (100) le long d'une direction de faisceau dans le volume de la partie corporelle du sujet, le dispositif comprenant :

une unité d'entrée de signal (203) pour recevoir des signaux électriques représentatifs de l'énergie ultrasonore réfléchie reçue par chaque élément de transducteur (101) du transducteur ultrasonore (100) incluant un réseau bidimensionnel d'éléments de transducteurs ;

un système d'analyse (205) pour analyser les signaux pour générer une représentation d'écoulement sanguin sur une pluralité d'emplacements prédéterminés dans le volume et pour calculer une première vitesse d'écoulement sanguin sur chacun des emplacements ;

une unité de délimitation (207) pour délimiter l'écoulement sanguin dans le vaisseau sanguin dans le volume à partir de la représentation de l'écoulement sanguin ;

une unité de calcul d'angle (209) pour calculer, sur une pluralité de points dans l'écoulement sanguin délimité, un angle Doppler entre la direction de faisceau du faisceau collimaté émis d'énergie ultrasonore et une direction de l'écoulement sanguin, ladite direction de l'écoulement sanguin dépendant de la délimitation ; et

un calculateur de vitesse (211) pour calculer une deuxième vitesse d'écoulement sanguin sur la pluralité de points basés sur les premières vitesses calculées sur la pluralité d'emplacements et l'angle Doppler calculé sur la pluralité de points pour transmettre la deuxième vitesse du sang à un utilisateur.

2. Dispositif selon la revendication 1, dans lequel la deuxième vitesse d'écoulement sanguin sur un point quelconque de la pluralité de points est déterminée uniquement si l'angle Doppler sur ce point est inférieur à une valeur prédéterminée.

3. Dispositif selon la revendication 1, dans lequel l'unité de calcul de l'angle (209) est destinée à transmettre

à l'utilisateur une information pour changer une position du transducteur sur le sujet lorsque le nombre d'angles Doppler déterminés qui sont inférieurs à la valeur prédéfinie est inférieur à un nombre prédéfini.

5

10

15

20

25

30

35

40

45

50

55

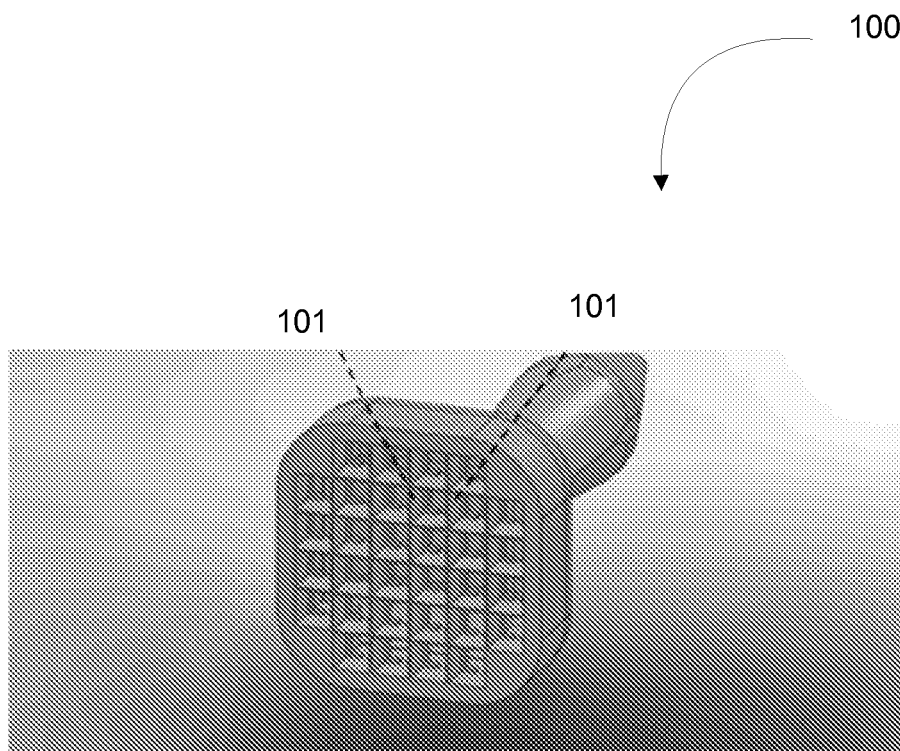


Fig. 1

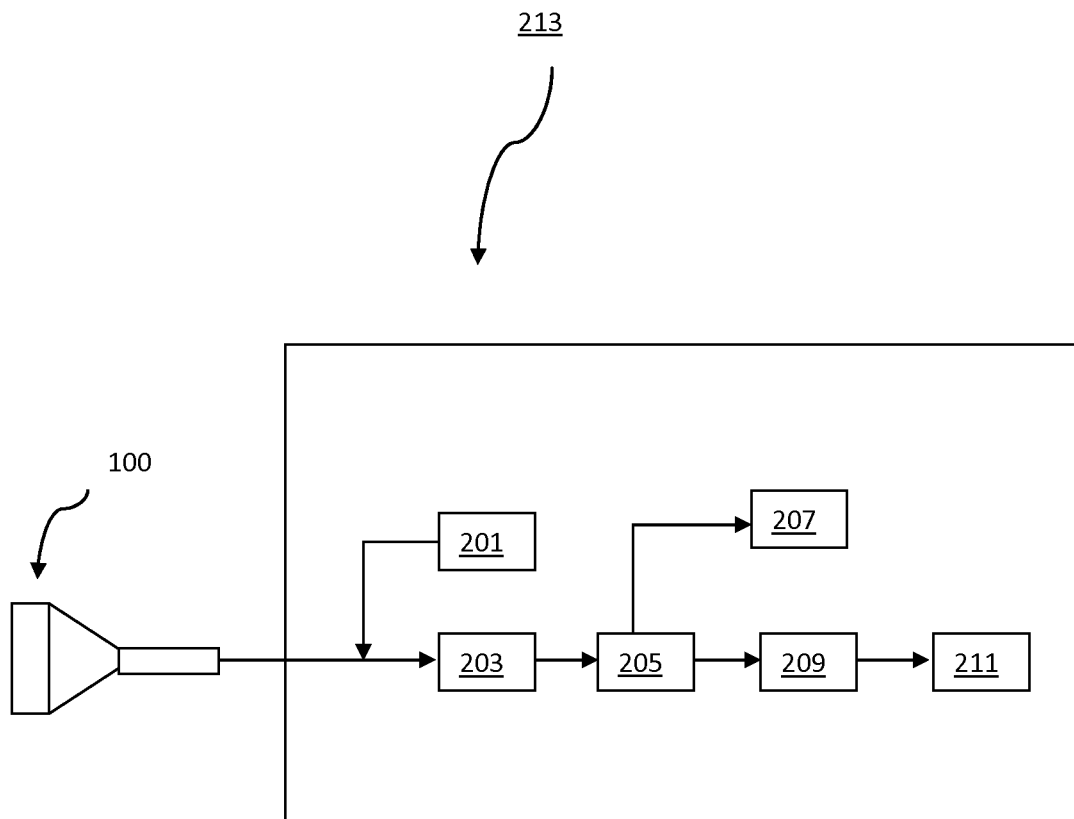


Fig. 2

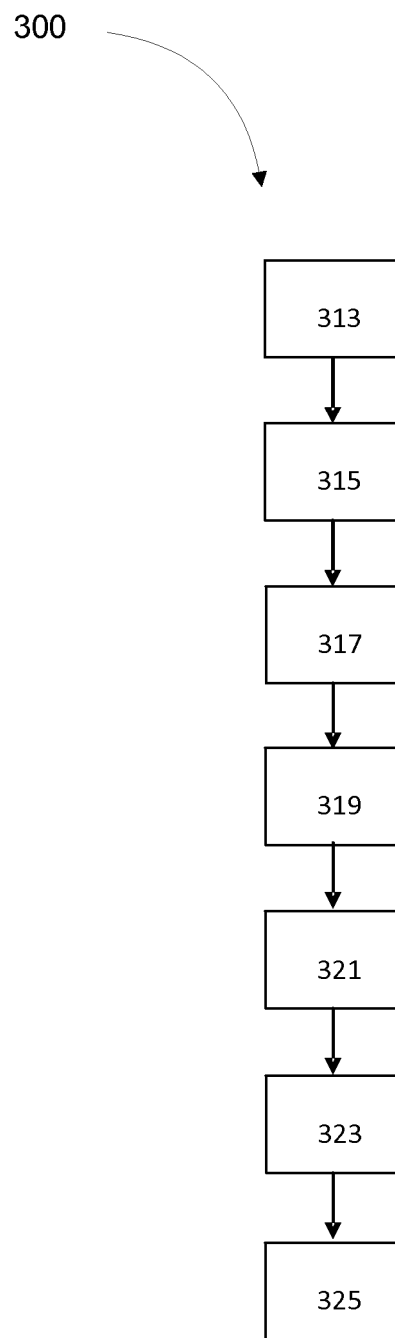


Fig. 3

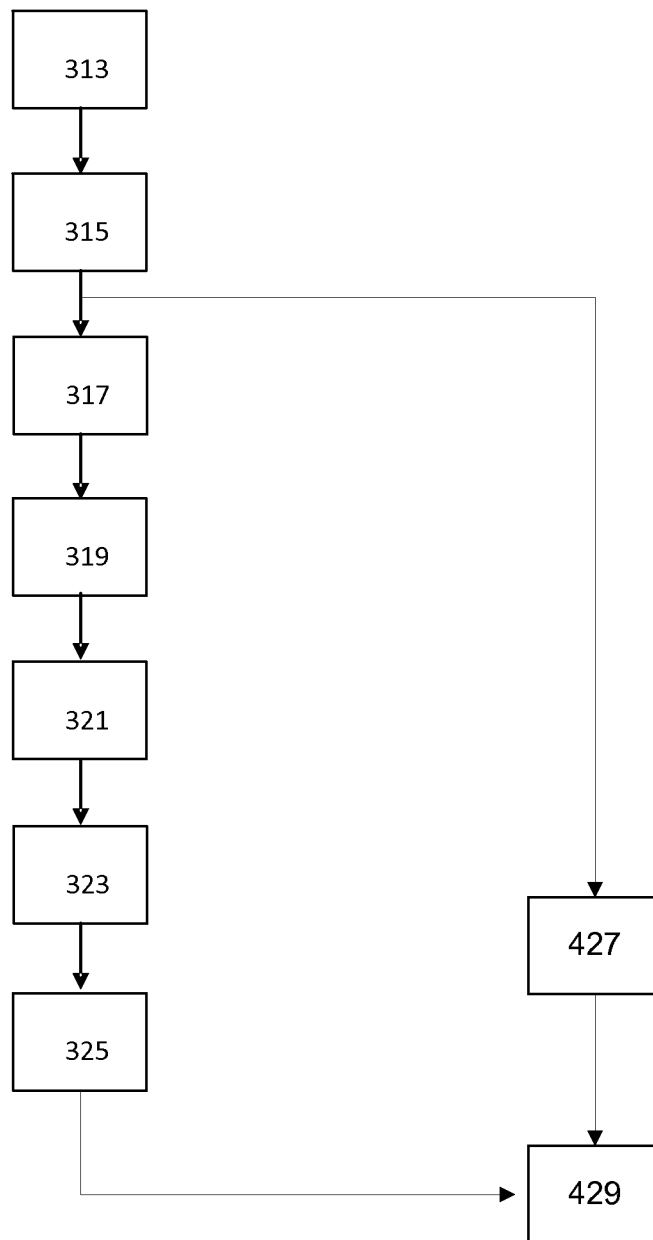


Fig. 4

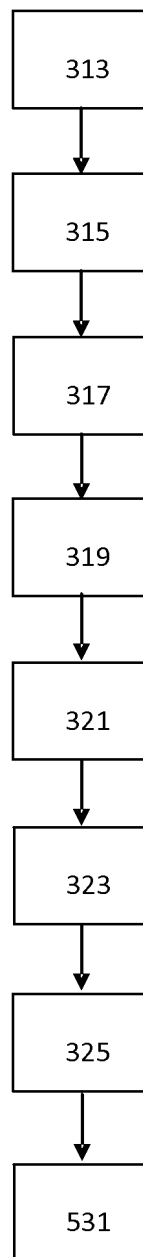


Fig. 5

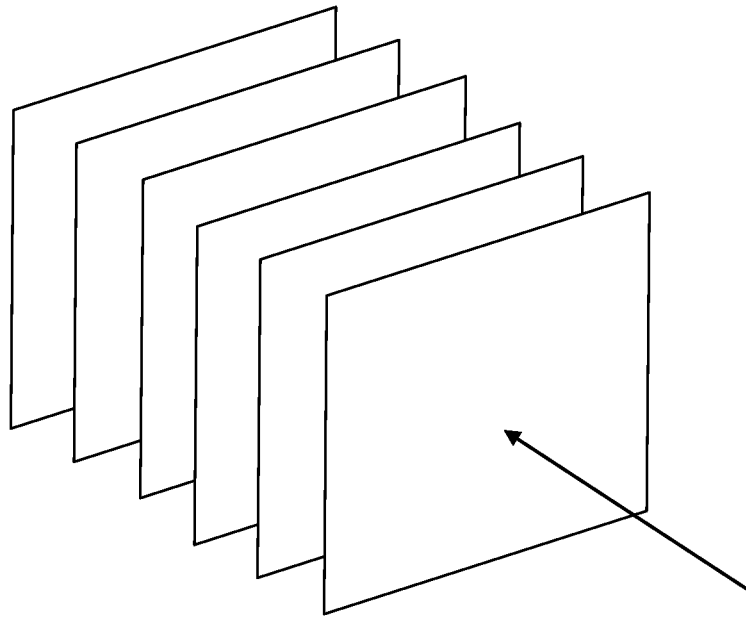


Fig. 6a

0					0
0					0

Fig. 6b

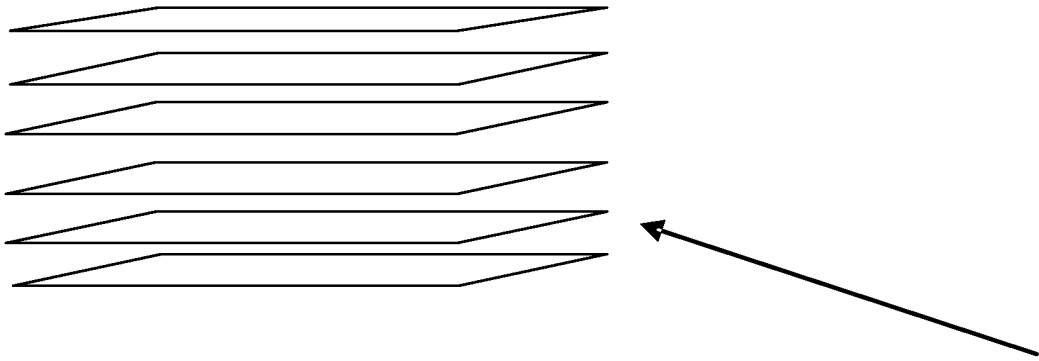


Fig. 6c

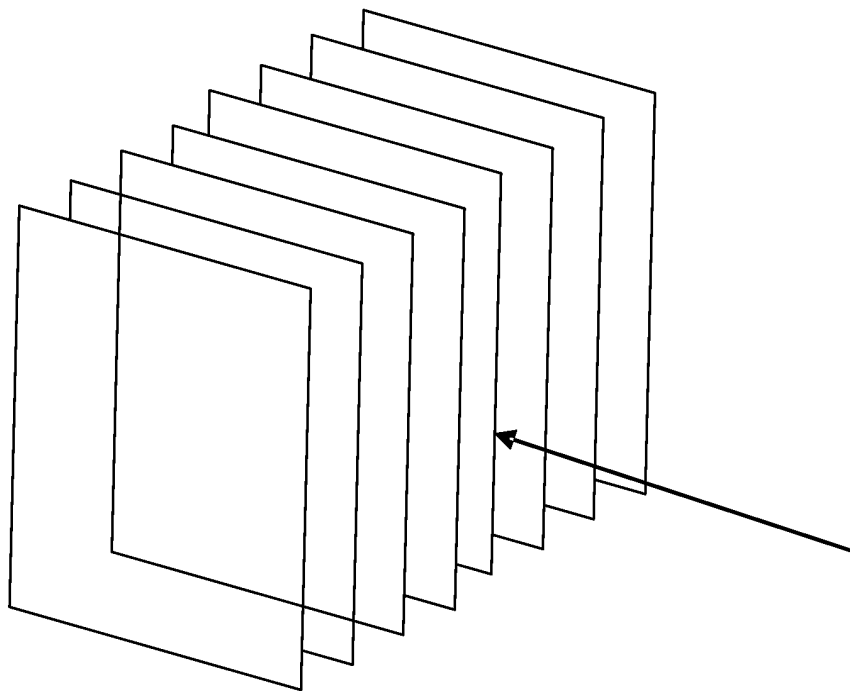


Fig. 6d

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5555886 A [0004]

专利名称(译)	用于自动超声波多普勒角度和流速估计的装置		
公开(公告)号	EP2725983B1	公开(公告)日	2018-02-28
申请号	EP2012751605	申请日	2012-06-29
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	GUPTA LALIT ANAND AJAY PETRUZZELLO JOHN VAJINEPALLI PALLAVI SISODIA RAJENDRA SINGH FIRTION CELINE RAMACHANDRAN GANESAN		
发明人	GUPTA, LALIT ANAND, AJAY PETRUZZELLO, JOHN VAJINEPALLI, PALLAVI SISODIA, RAJENDRA SINGH FIRTION, CELINE RAMACHANDRAN, GANESAN		
IPC分类号	A61B8/06		
CPC分类号	A61B8/06 A61B8/4494 A61B8/483 A61B8/488 A61B8/5223		
代理机构(译)	STEFFEN , THOMAS		
优先权	2236CHE2011 2011-06-30 IN		
其他公开文献	EP2725983A2		
外部链接	Espacenet		

摘要(译)

公开了一种用于测量受试者的血管中的血流速度的超声装置，其在装置中没有成像功能。测量取决于来自受试者身体部位的准直超声波束的反射。表示反射的超声能量的接收电信号用于在体积中的多个预定位置处生成血流的表示，并计算每个位置处的第一血流速度。流动表示用于描绘体积中血管中的血流。角度计算单元计算在每个点处描绘的血流中的辐射准直光束的方向之间的多普勒角。速度计算器基于计算的第一速度和该点处的计算角度计算多个点处的第二血流速度。

$$v = \frac{F_r \cdot c}{2 \cdot F_t \cdot \cos(\theta)}$$