

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
24 April 2003 (24.04.2003)

PCT

(10) International Publication Number
WO 03/032840 A2

- (51) International Patent Classification⁷: A61B 8/00
- (21) International Application Number: PCT/IB02/04724
- (22) International Filing Date: 18 October 2002 (18.10.2002)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
10/036,072 19 October 2001 (19.10.2001) US
- (63) Related by continuation (CON) or continuation-in-part (CIP) to earlier application:
US 10/036,072 (CIP)
Filed on 19 October 2001 (19.10.2001)

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZM, ZW.


(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

- (71) Applicants and
- (72) Inventors: **HOFF, Lars** [NO/NO]; Oygardvei 103, N-1357 Bekkestua (NO). **OYGARDEN, Kjell** [NO/NO]; Raknesv 1, 1473 Skarerer (NO).
- (74) Agent: **ONSAGERS SA**; P.O. Box 6963, St. Olavs plass, N-0130 Oslo (NO).

Published:
— without international search report and to be republished upon receipt of that report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: ULTRASOUND MEASUREMENT TECHNIQUES FOR BONE ANALYSIS

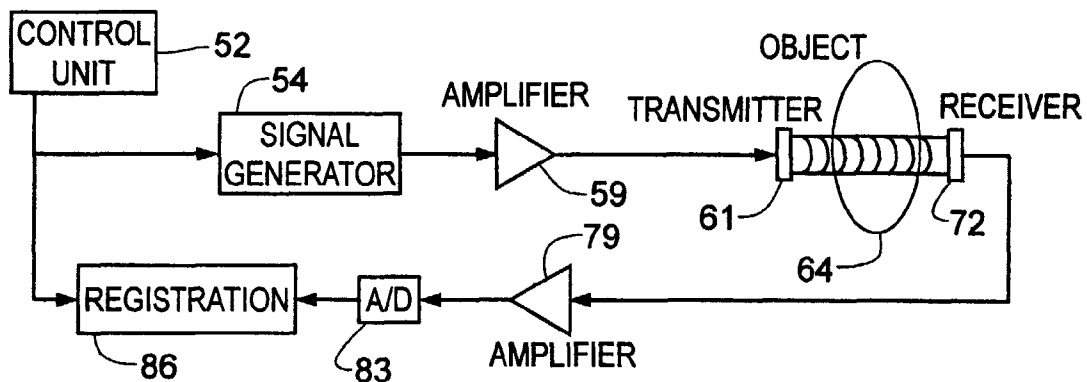

(57) Abstract: Ultrasound measurement of bone quality using nonlinear analysis in combination with or alternatively using shear waves provide improved information about human bone conditions. Surface waves also provide a novel method to estimate shear wave velocity.



WO 03/032840 A2

ULTRASOUND MEASUREMENT TECHNIQUES FOR BONE ANALYSIS

Field of the Invention

5 The invention relates to improved sensing and analysis of ultrasound measurement signals for use as a diagnostic tool in bone analysis.

Background of the Invention

10 The field of ultrasound imaging of mammalian physiology is well known and well established. However, the methodology is dominated by certain techniques which have known limitations that are susceptible to improvement or alteration. This technology is known to be used in the imaging of various sites, such as spinal, wrist, knee, cartilaginous areas, and other musculoskeletal locations in mammals, particularly humans. The use of ultrasound for these sites generally is referred to as Quantitative Ultrasound (QUS), and is
15 often in a competitive role with other imaging modalities.

 However, there has recently been some interest in using ultrasound in a predictive role for the disease known as osteoporosis. Osteoporosis is a disease of the skeleton in which the amount of calcium present in the bones slowly decreases to the point where the bones become brittle and prone to fracture. In other words, the bone loses density. It is estimated
20 that over 10 million people in the United States suffer from this disease, and 18 million more have low bone mass, placing them at increased risk for this disorder. Osteoporosis is no longer considered a solely age or gender-dependent, and when diagnosed early it can often be treated successfully.

 In summary, osteoporosis is a major public health problem characterized by
25 significant morbidity, mortality, and economic burden. Bone mass measurements, using ultrasound technologies, appears to be one of the best ways to make the diagnosis of osteoporosis. However, certain improvements are needed in this emerging area of medical technology to overcome reliability and availability of imaging systems.

Summary of the Invention

30 A system and method is disclosed for diagnosing osteoporosis comprising the components and software implemented steps of transmitting a signal sequence of ultrasound waves for impingement on a bone being measured; arranging a detection transducer configuration for receiving a portion of the transmitted signal sequence of ultrasound waves
35 after impingement on the bone being measured; and measuring the degree of acoustic

nonlinearity of the bone to estimate the material conditions of the bone indicative of the onset of osteoporosis.

There is also disclosed a system and method for measuring bone strength comprising components and software implemented steps of measuring the shear wave velocity (c_s);

5 estimating the Lamé coefficient shear modulus (μ) of the bone by use of the formula:

$$C_s = \sqrt{\frac{\mu}{\rho}}$$

and assigning a bone strength index of measure based on the estimate of shear modulus.

There is further disclosed a system and method for diagnosing osteoporosis comprising components and software implemented steps of measuring the pressure wave
10 velocity through a patient's bone; measuring the shear wave velocity through a patient's bone; calculating the ratio of shear wave velocity to the pressure wave velocity to determine whether the bone is degraded.

A still further disclosure includes a system for diagnosing osteoporosis comprising a transmitter configured for transmitting ultrasonic waves onto a predetermined area on the
15 surface of a patient's skin and through the tissue to the bone so as to create a surface wave at a bone-tissue interface region that is measurable by a receiver of the ultrasonic surface wave; at least one receiver of ultrasonic waves on an area on the surface of the patient's skin a known distance from the transmitter; and analysis circuitry for measuring the surface wave velocity and translating the measured velocity into an indicator of bone health status.

20

Description of the Drawings

Figure 1 is a schematic of ultrasound wave propagations in tissue and bone media.

Figure 2 is a graph of measured P waves in human samples.

Figure 3 is a graph of measured S waves in human samples.

25 Figure 4 is a graph of the ratio of measured S and P waves in human samples.

Figure 5 is a block diagram of a pulse propagation measuring setup.

Figure 6 is a block diagram of a backscatter or reflection measuring setup.

Figure 7 is a block diagram of a reflection at an angle measuring setup.

Figure 8 is a block diagram of an experimental non-linearity detection setup.

30 Figure 9 is a graph of the power spectra of a received signal in a human sample.

Figure 10 is a plot of the strength of the second harmonic received and the strength of the transmit frequency received as a function of transmit voltage.

Figure 11 is a plot of the relative strength of the second harmonic received to the transmit frequency received as a function of transmit voltage.

Figure 12 is a plot comparing non-linearity in healthy and osteoporotic humans.

5 Detailed Description of the Preferred Embodiment

Osteoporosis is also defined as a skeletal disorder characterized by compromised bone strength predisposing to an increased risk of fracture. Bone strength reflects the integration of two main features: bone density and bone quality. Bone density is expressed as grams of mineral per area or volume and in any given individual is determined by peak bone mass and
10 amount of bone loss. Bone quality refers to architecture, turnover, damage accumulation (e.g., microfractures) and mineralization. Osteoporosis is well established as a significant risk factor for fracture.

Osteoporosis can be further characterized as either primary or secondary. Primary osteoporosis can occur in both genders at all ages but often follows menopause in women and
15 occurs later in life in men. In contrast, secondary osteoporosis is a result of medications, other conditions, or diseases. Osteoporosis is diagnosed when bone density has decreased to the point where fractures will happen with mild stress, its so-called fracture threshold. This is defined by the World Health Organizations as bone mass density (BMD) that is a 2.5 standard deviation (SD) or more below the average BMD for young adults. (One standard
20 deviation below the norm in a measurement of hip bone density is equivalent to adding 14 years to a person's risk for fracture.) Measurements of between 1 and 2.5 SD below normal are defined as osteopenia.

The consequences of osteoporosis include the financial, physical, and psychosocial, which significantly affect the individual as well as the family and community. An
25 osteoporotic fracture is a tragic outcome of a traumatic event in the presence of compromised bone strength, and its incidence is increased by various other risk factors. Traumatic events can range from high-impact falls to normal lifting and bending. The incidence of fracture is high in individuals with osteoporosis and increases with age. Osteoporotic fractures, particularly vertebral fractures, can be associated with chronic disabling pain. Nearly one-
30 third of patients with hip fractures are discharged to nursing homes within the year following a fracture. Notably, one in five patients is no longer living 1 year after sustaining an osteoporotic hip fracture. Hip and vertebral fractures are a problem for women in their late 70s and 80s, wrist fractures are a problem in the late 50s to early 70s, and all other fractures (e.g., pelvic and rib) are a problem throughout postmenopausal years. Indeed, the National

Osteoporosis Foundation (United States) estimates that there are more than 1.5 million fractures reported each year.

By way of example, hip fracture alone has a profound impact on quality of life, as evidenced by findings that 80 percent of women older than 75 years preferred death to a bad hip fracture resulting in nursing home placement. However, little data exist on the relationship between fractures and psychological and social well-being. Other quality-of-life issues include adverse effects on physical health (impact of skeletal deformity) and financial resources. An osteoporotic fracture is associated with increased difficulty in activities of daily life, as only one-third of fracture patients regain pre-fracture level of function and one-third require nursing home placement. Fear, anxiety, and depression are frequently reported in women with established osteoporosis and such consequences are likely under-addressed when considering the overall impact of this condition. Direct financial expenditures for treatment of osteoporotic fracture are estimated at \$10 to \$15 billion annually. A majority of these estimated costs are due to in-patient care but do not include the costs of treatment for individuals without a history of fractures, nor do they include the indirect costs of lost wages or productivity of either the individual or the caregiver.

Currently, the most popular technique for determining bone density is dual-energy x-ray absorptiometry (DEXA), which measures bone density throughout the body within two to four minutes. The measurements are made by detecting the extent to which bones absorb photons that are generated by very low-level x-rays. Physicians use a formula based on the results of these procedures to determine if bone density has deteriorated to the fracture threshold.

Unfortunately, DEXA is not widely available and may be inappropriate for many patients. Other techniques that measure density may also result in accurate measures of overall bone loss and be less expensive and may not expose the patient to the radiation inherent to DEXA and its analogs. These are examples of the opportunities for ultrasound, subject to basic improvements in its accuracy, sensitivity, and overall predictive value.

Use of ultrasound in relation to monitoring of bone growth is also well documented. With respect to bone healing, one study reports that callus (i.e., the hard bonelike substance thrown out between and around the ends of a fractured bone) is easily visualized with ultrasound. Moreover, callus as seen on ultrasound predates its appearance on radiographs. It has also been suggested that fracture union on ultrasound precedes radiographic union. Thus, it is believed that ultrasound may provide important prognostic information concerning

fracture healing as well as valuable information of regenerate bone during the process of limb lengthening.

5 Ultrasound has been used for many years to investigate the mechanical properties of various engineering materials. It offers the theoretic advantage of measuring material properties other than density. As noted above, this technique is termed quantitative ultrasound (QUS). This offers the advantages of small size, relatively quick and simple measurements, and no radiation. QUS measurements are generally considered as much easier to perform at skeletal sites with minimal soft tissue covering. However, to date, most QUS devices measure the peripheral skeleton, including the heel, shin, knee cap, and fingers only, due to certain
10 limitations.

Regardless, several different QUS devices and methods have been shown to be predictive of hip fracture, independent of radiograph-based bone density measurements. QUS has enjoyed widespread use around the world and has recently been approved for clinical use in the United States. Indeed, certain changes in government reimbursement schemes may
15 even accelerate the introduction and use of QUS technologies in order to avail lower cost high quality methodologies to a greater population. Although apparently the QUS technologies are exciting, there are still concerns and room for improvements. For example, researchers are still not certain exactly which mechanical or structural parameters of the bone are being measured with QUS. It has been speculated that QUS may be related to trabecular
20 size, trabecular spacing, and parameters of bone mineralization such as crystal size and orientation.

In yet another analysis, it has been found that broadband ultrasound attenuation (BUA) also predicts the occurrence of fractures in older women and is a useful diagnostic test for osteoporosis. The strength of the association between BUA and fracture is similar to that
25 observed with bone mineral density. Broad-band acoustic attenuation and speed-of-sound have also been shown to display a quantitative relationship to mineralization. Further, in another study, measurements of the attenuation and velocity of ultrasound from 0.3 to 0.8 MHz have been performed on a number of bovine cancellous bone samples. The influence of bone mineral content was isolated by measuring the acoustic properties of the samples at
30 various stages of demineralization resulting from controlled nitric acid attack. The correlation coefficient r , between the attenuation at different frequencies and bone density was found to be in the range 0.68-0.97. Broadband ultrasonic attenuation (BUA) was also calculated and produced r values between 0.84 and 0.99. The velocity measurements indicated a correlation greater than 0.97 in all cases. Thus velocity appears to be the parameter most sensitive to

changes in bone mineral density alone. Attenuation and BUA are less well correlated presumably because of a sensitivity to minor structural change. Accordingly, further advances in research are required and encouraged.

Yet another study determined that each standard deviation decrease in calcaneal
5 broadband ultrasound attenuation was associated with a doubling of the risk for hip fractures after adjustment for age and clinic. The relationship was similar for bone mineral density of the calcaneus and femoral neck. Decreased broadband ultrasound attenuation was associated
10 with an increased risk for hip fracture. A low broadband ultrasound attenuation value was particularly strongly correlated with intertrochanteric fractures, i.e., fractures at the proximal femur. The conclusion reached was that decreased broadband ultrasound attenuation predicts the occurrence of fracture in elderly women and that this may also provide a useful diagnostic test for osteoporosis. Thus, the need to accurately account for attenuation and sound velocity profiles of bone in patients at various sites is quite important in this fight against osteoporosis.

15 In summary, osteoporosis is a major public health problem characterized by significant morbidity, mortality, and economic burden. Osteoporotic fractures in older women are related, for the most part, to the women's BMD. Ultrasound does not measure bone density but rather measures two parameters called speed of sound (SOS) and broadband
20 ultrasound attenuation (BUA) that are related to the structural properties of bone. Studies have shown that QUS measures have the ability to distinguish fracture patients from controls and to predict future fracture. The advantage for ultrasound devices is that they are small, portable, use no ionizing radiation, and may provide an attractive alternative to radiation-based densitometry. Bone mass measurement appears to be one of the best ways to make the diagnosis of osteoporosis. However, considerable improvements are needed in this emerging
25 area of medical technology.

The methods in use for the measurement of bone density by ultrasound are generally limited to measurement of direct transmission and scatter measurements, sending sound through a bone, and measuring acoustic transmission and speed of sound, including reflection. The velocity of sound in bone can be measured using a technique analogous to
30 that used in the field of refraction seismics, which involves investigations of the sea floor for various purposes. As applied to physiological testing, the method consists of a first transducer transmitting an ultrasonic wave from a point external of the tissue into an inner bone at a critical angle. This generates pressure, shear and/or surface waves that propagate along the interface between the bone and the soft tissue. The wave radiated from these waves

is then received by a second transducer, also positioned external to the tissue. The speed of sound in the bone is calculated from the first time of arrival of the sound pulse at the receiving transducer. This method requires the velocity of sound in bone to be greater than in the surrounding soft tissue, which is true for pressure waves, but may not be fulfilled for shear waves.

The method is illustrated in Figure 1, and is summarized as follows. An acoustic wave is emitted from the transmitter T into the body of the patient and received with the receiver R. T and R are placed on the skin of the patient at a distance x . The emitted wave may follow three paths from T to R:

(1) **Direct wave.** This wave follows a straight line parallel to the skin surface and is denoted by line 13.

(2) **Reflected wave.** This wave is reflected at the boundary between the soft tissue and the bone, and is denoted by line 15.

(3) **Refracted wave.** This wave, denoted by line 17, hits the bone at critical angle θ_c , propagates along the interface between soft tissue and bone, while radiating acoustic energy back to the tissue at critical angle θ_c . Some of the radiated sound is received by the receiver R. The critical angle θ_c is given by

$$\theta_c = \frac{v_o}{v_l} \tag{1}$$

where v_o is the speed of sound in the tissue and v_l is the speed of sound in the bone.

The time of flight from T to R for these three waves are t_1 , t_2 and t_3 . The arrival time t_3 of the refracted wave can be found from Figure 1 to be

$$t_3 = x/v_l + 2 d_o \frac{\sqrt{v_l^2 - v_o^2}}{v_o v_l} \tag{2}$$

where x is the distance between transmitter T and receiver R and d_o is the distance from the skin surface to the bone, as shown in Figure 1.

The wave velocity v_l of the bone is larger than the wave velocity v_o of the soft tissue. If, in addition, the distance x between T and R exceeds a minimum value x_{min} , the refracted wave 17 may arrive on R before the other waves 13, 15, that is

$$v_1 > v_0 \text{ and } x > x_{min} \Rightarrow t_3 < t_1, t_2$$

(3)

5 Hence, the time t_3 can be found from the first arrival of a signal at R after transmitting from T. When the time of first arrival t_3 is measured, the speed of sound in the bone v_1 is calculated from (Eq. 2). The speed of sound in the soft tissue v_0 and the distances x and d_0 must be measured independently. This may be done from ultrasound time-of-flight measurements. This technique allows accurate measurements of sound velocity independent
 10 of geometric dimensions. This technique may be combined by one or more of the principles below to increase the accuracy of the estimates of sound velocity.

United States Patent No. 5,197,475 illustrates ultrasound measurement setups using such basic principles of ultrasound pressure wave transmission and/or reflection, particularly as a function of angle. The reference provides very broad but useful description of
 15 measurement systems and techniques, and also briefly addresses the concept known as shear wave measurements. Elaborating on that latter concept, and other unknown combinations of techniques, is one of the goals of the present invention.

Shear waves do not propagate far in tissue, but will propagate in solid structures like bone. Moreover, the shear wave velocity is more sensitive to material structure than the
 20 pressure wave velocity, in that it differs more strongly between various materials. Hence, the shear wave velocity is a more sensitive parameter than pressure wave velocity for detecting the state of the measured bone.

The pressure c_p and shear c_s wave velocities of an elastic solid are given by the expressions

$$25 \quad C_p = \sqrt{\frac{\lambda + 2\mu}{\rho}} \quad \text{and} \quad C_s = \sqrt{\frac{\mu}{\rho}} \quad (4)$$

where ρ is the density and λ and μ are the Lamé coefficients of the material.

Measurement of the shear wave velocity includes an estimate for the second Lamé coefficient μ , which is the shear modulus of the material. Degradation of a material typically causes a reduction in its density ρ and a reduction in material rigidity, that is, lower values of
 30 λ and μ . Measurements of both c_p and c_s in (Eq. 4) gives more information about the underlying material properties than measurements of c_p alone.

If a material undergoes a transition from an elastic solid to a looser porous structure, this causes a larger reduction in the shear modulus μ than in the bulk modulus $K = \lambda + 2/3 \mu$. Hence, independent measurements of c_p and c_s , calculating e.g. the ratio c_s/c_p , will provide information about the relation between the shear and bulk moduli of the material. This gives information about whether the material is changed from an homogeneous solid into a looser porous structure.

Velocity dispersion is a characteristic property of heterogenous media, especially porous materials. If the bone undergoes a transition from homogeneous to porous, it can also change from non-dispersive to dispersive. Hence, sound velocity dispersion can be used as an indicator of altered tissue material structure. In addition, this technique can reduce the need for an accurate measurement of sound velocity, as it only requires relative measurement of phase velocity as function of frequency, and the technique does not depend on accurate measurements of geometric dimensions. In the case of a heterogenous medium, the phase velocity typically undergoes a change where the wavelength is of the same magnitude as the grain size. This transition may be used as an estimate for "grain size" in a porous material. Velocity dispersion measurements can be combined with measurement of frequency dependent attenuation, to further increase the accuracy of the estimates.

Another aspect of ultrasound imaging relates to nonlinearity. All sound propagation is nonlinear, and will generate harmonics at sufficiently high amplitudes over sufficiently long distances. Small voids or other inhomogeneities can act as nonlinear sources in solid materials, and increase the acoustic nonlinearity parameter. Hence, measurements of the degree of nonlinearity in a material can be used to estimate material conditions. Especially, it may be used to estimate whether the material is changing from a homogeneous to a more heterogenous structure.

There are several ways to measure the degree of nonlinearity. The most obvious is to transmit a sound pulse through the material and measure the harmonic distortion, i.e. the level at harmonics of the transmitted frequency. Here, the second harmonic is the most natural choice, but also higher harmonics, or combinations of harmonics can be used. Harmonic detection is summarized as

30	Transmit frequency	f_T	(5)
	Receive one or more of the harmonics	$2f_T, 3f_T, 4f_T, \dots$	

Nonlinear frequency mixing may be an even better method. Two frequencies are transmitted through the sample. This can be done either by two separate transducers, or by exciting one transducer with both frequencies. The transmitted or scattered signals from the material is picked up by another, or the same, transducer. Nonlinear mixing will cause sum- and difference frequencies in the received signals. The level at these sum and/or difference frequencies is an indicator of the condition of the material. Nonlinear frequency mixing is summarized as

10	Transmit frequencies	f_1 and f_2	
	Receive at sum and/or difference frequencies	$f_1 + f_2, f_1 - f_2$	(6)

The harmonic and nonlinear frequency mixing techniques may also be combined, i.e. receive at sum and difference frequencies of the harmonics. An example would be

15	Transmit frequencies	f_1 and f_2	
	Receive at sums and/or differences around harmonics, e.g.	$2f_1 - f_2, 2f_1 + f_2, 3f_1 + f_2$	(7)

The methods mentioned above may be combined in various measuring or display techniques to increase the quality of the outcomes. Further, these techniques may be combined with other measurement techniques, such as measurements of reflection, scatter, attenuation and speed of sound. They may also be combined with estimates for elastic properties, and with measurements of shape and geometrical dimensions.

In addition to the possible combinations noted above, the invention also includes a recognition of technical know how across diverse industries. For example, as is well known in the petroleum industry, porosity of materials is one of the parameters that influences acoustic velocity and attenuation. In the case of increasing porosity, a decrease in the acoustic velocities and an increase of the attenuation are expected. Moreover, it is now appreciated that compressional and shear waves can be affected differently from an increase in porosity. Past studies on acoustic P wave velocity measurements in bones were made primarily for porosity monitoring. A more efficient and suitable method for clinical use may be to measure the shear or S-wave velocity, and a combination of petroleum and medical

research knowledge may be useful in that regard, as well as certain breakthrough realizations of the inventor.

5 Preliminary acoustic velocity measurements on bovine bones were made in order to test the possibility of measuring P-wave velocity, S-wave velocity and attenuation in bones using the equipment available in the Formation Physics Laboratory at SINTEF Petroleum Research in Trondheim, Norway. A sample description and preparation of samples in a representative bone structure comprises a compact outer layer, a cancellous bone, and inner bone marrow. Pieces of the cow bones were obtained from a butcher's shop and were preserved in a supposed best condition, but which included partially frozen matter which later
10 caused some concern as to certain readings.

The bone to be examined is a structural bio composite of ca. 70% (by weight) inorganic calcium salts embedded in collagen fibres. Most of the inorganic phase consists of hydroxyapatite (calcium phosphate) but a large amount of carbonate, citrate and fluoride amines are also present. Long bones such as the femur or thigh bones are composed of a
15 harder, compact composite outer layer, which improves the stiffness and strength-to-weight indices for the material, surrounding a spongy interior (cancellous bone) and the marrow. Bones exhibit viscoelastic properties and are sensitive to rate of loading.

Suitable results of the testing on the bovine samples validate the equipment and methodology suitable for advancement to tests on human bone samples. Pulse wave
20 transmission (PWT) techniques and continuous wave techniques (CWT) were then used in order to measure compressional (Pw) and shear (Sw) wave velocities on the bovine samples TI 1-TI 5 and on the human samples TIU 1- TIU 6. The transducers used in the experiments were broadband P-wave and S-wave Panametric 500 kHz transducers for the PWT and 5 MHz for the CWT. Generally, two oppositely parallel, smooth sides were made on the
25 samples to allow for mounting of the acoustic transducers.

The PWT equipment consisted of a WAVETEK model 278 12MHz Programmable Synthesized Function Wave Generator, an ENI model 2100L RF 10kHz-12MHz amplifier, a YOKOGAWA model DL 1300A 4 Channels 100MHz digital oscilloscope, a Physical Acoustic Corporation model 220b 40-60 dB preamplifier and filter between 100 and 1200
30 kHz, a computer to control the system, and a sample holder mechanism.

The continuous wave equipment consisted of a Hewlett Packard 33120A 15 MHz Function Arbitrary Waveform wave generator, a wave detector (containing) an amplifier and a modulator, a computer to control the system, and a sample holder mechanism.

Measurements were made at 100, 250, 500, 750 kHz emitting frequencies, when possible. Measurements were made by CWT, both for P and S wave. The amplitude of the output signal was also recorded.

In the pulse wave techniques, the signal was sinusoidal and was generated at 230 mV and amplified by 50dB. Corrections were made for the system delay, and the velocities were calculated using the first break criterion. For each position, 5 measurements were taken and the average value of those measurements was calculated. Acoustic velocity, amplitude and wavelength were reported. The error in the measurements was estimated to +/- 2%.

10 **Sample TI 1**

P wave and S wave measurements were performed at three different positions on the bone by pulse wave technique and by using 500 kHz transducers at 100 kHz excitation frequencies. The P wave velocity was also measured at 250 kHz. It was not possible to record the output signal at 250 kHz for S-wave. Measurements were made on all three different bone structures. The measurements performed on the sample TI 1 were made in three different positions on the bone, in order to detect the velocities of the marrow, cancellous and hard zones as accurately as possible.

Table 1A

TI 1						
Material	Frequency (kHz)	P wave vel (km/s)	Typical P-wave length (m)	S wave vel (km/s)	Typical S-wave length (m)	Typical A Pw Sw (v)
Marrow	100	2.278	0.022	1.004	0.01	$4 \cdot 10^{-4}$ $5 \cdot 10^{-4}$
Cancellous zone	100	2.456	0.024	1.111	0.011	$1.5 \cdot 10^{-3}$ $3 \cdot 10^{-4}$
Hard zone	100	2.691	0.024			$5 \cdot 10^{-4}$

Table 1B

TI 1						
Material	Frequency (kHz)	P wave vel (m/s)	Typical P-wave length (m)	S wave vel (m/s)	Typical S-wave length (m)	Typical A (v) Pw
Marrow	250	2.446	0.009			$3 \cdot 10^{-4}$
Cancellous zone	250	2.529	0.010			$4.7 \cdot 10^{-4}$
Hard zone	250	2.618	0.010			

Sample TI 2

P wave and S wave measurements were performed by using the pulse wave technique with 500 kHz transducers at 100, 250, 500 and 750 kHz excitation frequencies. It was not possible to record the output signal at 100 kHz for S wave. Measurements were made on the cancellous zone.

Table 2

10

TI 2						
Material	Frequency (kHz)	P wave vel (km/s)	Typical P-wave length (m)	S wave vel (km/s)	Typical S-wave length (m)	Typical A (v) Pw Sw
Cancellous zone	100	2.291	0.022			2.5*10 ⁻³ --
Cancellous zone	250	2.395	0.009	1.552	0.006	2*10 ⁻³ 2*10 ⁻⁴
Cancellous zone	500	2.566	0.005	1.460	0.0029	1*10 ⁻³ 4*10 ⁻⁴
Cancellous zone	750	2.751	0.003	2.013	0.0026	5*10 ⁻⁴ --

Sample TI 3

P wave and S wave measurements were performed by using the pulse wave technique with 500 kHz transducers at an excitation frequency of 100 kHz. It was not possible to record output signals at higher frequencies. The measurements were made on the cancellous zone.

Table 3

20

TI 3						
Material	Frequency (kHz)	P wave vel (km/s)	Typical P-wave length (m)	S wave vel (km/s)	Typical S-wave length (m)	Typical A (v)
Cancellous zone	100	3.120	0.031	1.408 or (?) 1.722	0.015	

25

Sample TI 4

P wave and S wave velocity measurements were made by using the CWT technique on a small sample (millimeter or cutting dimension). In this case, 5 MHz transducers were used in a range of frequencies from 3 to 10 MHz. The results reported are average values of the velocities measured at all those frequencies. The measurements were made on a selected piece of the hard outer zone.

Table 4

TI 4			
Material	Frequency (MHz)	P wave vel (km/s)	S wave vel (km/s)
Cancellous hard zone	3-10	3.83± (0.05)	1.80± (0.04)

Since one of the objectives of the bovine study was to validate the measuring of P and S wave acoustic velocities on bone samples and to achieve some experience with this material, the experiments were considered to be successful and indicative. Also, acoustic velocity in this bone was validated as being frequency dependent, with the velocities increasing with frequency. Measurements on the human bone samples then occurred. The samples were already prepared at the arrival in the laboratory, and were in natural condition in plastic envelopes. Occasional grinding was necessary to enhance proper contact. A summary of the human bone sample sources is shown below in Table 5 below .

Table 5

Sample	Age	Gender
TIU 1	77	Female
TIU 2	91	Male*
TIU 3	91	Male*
TIU 4	95	Female**
TIU 5	95	Female**
TIU 6	76	Female

* from the same person

** from the same person

The human bone sample measurements were performed with only pulse wave techniques. Measurements were done systematically at 100, 250, 500, and 750 kHz both for P wave and S wave.

5 **Sample TIU 1**

The P wave and S wave measurements were performed by pulse wave technique and by using 500 kHz transducers at 100, 250, 500, and 750 kHz excitation frequencies. The P wave signal was clear at all frequencies even if the resolution at 750 was quite poor. The S wave signal was best defined at 250 kHz. At this frequency the two modes separated.

10

Table 6

TIU 1

Frequency (kHz)	P wave vel (km/s)	Typical P wave length (m)	S wave vel (km/s)	Typical S wave length (m)
100	3.18	0.03	1.45	0.014
250	3.28	0.01	1.52	0.006
500	3.40	0.006	1.57	0.003
750	3.43	0.004	-	-

15 **Sample TIU 2**

P wave and S wave measurements were performed by pulse wave technique and by using 500 kHz transducers at 100, 250, 500 and 750 kHz excitation frequencies. The P wave signal was clear at all frequencies. The S wave signal was well defined at frequencies higher than 250 kHz, and after that the sample was grounded.

20

Table 7

TIU 2

Frequency (kHz)	P wave vel (km/s)	Typical P wave length (m)	S wave vel (km/s)	Typical S wave length (m)
100	2.86	0.02	1.27	0.012
250	2.94	0.01	1.44	0.005
500	3.01	0.006	1.47	0.0029
750	3.16	0.004	1.53	.002

25 **Sample TIU 3**

P wave and S wave measurements were performed by pulse wave technique and by using 500 kHz transducers at 100, 250, 500 and 750 kHz excitation frequencies. The P wave

signal was clear at all frequencies even though the resolution at 750 kHz was poor. The S wave signal was readable only at 250 kHz and was recognized at 100 kHz.

Table 8

5

TIU 3

Frequency (kHz)	P wave vel (km/s)	Typical P wave length (m)	S wave vel (km/s)	Typical S wave length (m)
100	2.71	0.03	1.24	0.012
250	2.88	0.01	1.48	0.006
500	2.98	0.006	-	-
750	3.03	0.004	-	-

Sample TIU 4

10 P wave and S wave measurements were performed by pulse wave technique and by using 500 kHz transducers at 100, 250, 500 and 750 kHz excitation frequencies. The P wave signal was clear at all frequencies even though the resolution at 750 kHz was poor. The S wave signal was readable only at 250 kHz, but that result may be suspect.

Table 9

15

TIU 4

Frequency (kHz)	P wave vel (km/s)	Typical P wave length (m)	S wave vel (km/s)	Typical S wave length (m)
100	2.36	0.02	-	-
250	2.42	0.01	1.55	0.006
500	2.52	0.005	-	-
750	2.61	0.003	-	-

Sample TIU 5

20 P wave and S wave measurements were performed by pulse wave technique and by using 500 kHz transducers at 100, 250, 500 and 750 kHz excitation frequencies. The P wave signal was clear at all frequencies even though the resolution at 750 kHz was poor. The S wave signal was readable only at 250, 500, and 750 kHz, but the signal was poor.

25

Table 10

TIU 5

Frequency (kHz)	P wave vel (km/s)	Typical P wave length (m)	S wave vel (km/s)	Typical S wave length (m)
100	2.37	0.02	-	-
250	2.50	0.01	1.34	0.005
500	2.53	0.005	1.40	0.003
750	2.61	0.003	1.43	0.0019

5 **Sample TIU 6**

P wave and S wave measurements were performed by pulse wave technique and by using 500 kHz transducers at 100, 250, 500 and 750 kHz excitation frequencies. The P wave signal was clear at all frequencies even though the resolution at 750 kHz was poor. The S wave signal was readable only at 250 and 500 kHz.

10

Table 11

TIU 6

Frequency (kHz)	P wave vel (km/s)	Typical P wave length (m)	S wave vel (km/s)	Typical S wave length (m)
100	2.68	0.03	-	-
250	2.74	0.01	1.18	0.005
500	2.93	0.006	1.20	0.002
750	2.96	0.004	-	-

15

Figures 2-4 are plots of the recorded human sample P wave velocities (V_p), S wave velocities (V_s), and a ratio of the velocities (V_s/V_p). In these Figures, line 21 represents human sample TIU 1, line 22 represents human sample TIU 2, line 23 represents human sample TIU 3, line 24 represents human sample TIU 4, line 25 represents human sample TIU 5, and line 26 represents human sample TIU 6. Again, the main interest was in the trabecular part of the bone, as this is where the effect of osteoporosis is generally first seen.

20

These findings suggest that although S wave velocities were more difficult to measure than P wave velocities, the existence of a shear wave in human trabecular bone is verified. The shear wave in trabecular bone is heavily attenuated, i.e. more attenuated than the P wave. In these samples the shear wave velocity in the trabecular bone was measured at between about 1200 and 1600 m/s, depending on sample and frequency.

25

These results support the inventors' analysis that shear waves may be a useful measure of bone condition, including possible degradation. The shear wave velocity and/or

attenuation is believed to be a more sensitive indicator of bone condition than the P wave parameters widely used in present instruments, particularly for the trabecular bone in which a marked change in shear wave velocity may indicate that normal lattice bridges and connections are no longer competent. Improved means of determining shear wave, or S wave, velocity v_s , and possibly attenuation α_s , at one or more frequencies, or as a function of frequency, $v_s(f)$, $\alpha_s(f)$, are all viable techniques included herein. Surface waves at the bone-tissue interface is one very interesting method to estimate the shear wave velocity in the bone. Surface waves at a fluid-solid interface typically have a velocity of about 0.87 and 0.95 times the shear velocity. Hence, the surface wave velocity provides a method to estimate the shear wave velocity in the bone. This is somewhat analogous to methods used to estimate the shear wave velocity in the sea floor from surface waves propagating along the water-sea floor interface.

A different but very promising method to estimate bone condition, is the use of nonlinear acoustics. Such methods are expected to be particularly useful in estimating micro-cracks or micro-fractures in the human bone. These cracks may act as sources for nonlinear acoustic generation, and therefore the methods identified herein may be considered somewhat analogous to recently developed methods for detecting micro-cracks and other defects in nondestructive testing/evaluation of materials known generally as nonlinear acoustic nondestructive evaluation (NANDE) or nonlinear wave modulation spectroscopy. Measurement of acoustic nonlinearity can therefore be used as an indicator of bone condition.

Several of the disclosed measurement methods are considered part of this novel technique. The transmitted signal may either be a continuous wave, CW, or a pulsed wave, PW. The measurements can be accomplished as through-transmission (as shown in Figure 5), pulse-echo backscatter (as shown in Figure 6), or scatter at an angle (as shown in Figure 7). In Figure 5, there is shown representatively configured components of a control unit 52, signal generator 54, amplifier 59, transmitter 61, the object being measured 64, receiver 72, amplifier 79, analog to digital converter, and registration unit 86. The configuration of Figure 6 includes most of the similar components but also that of transmit/receive switch 60 and transmit/receive transducer 62. In Figure 7, the configuration is similar to that depicted in Figure 5 but with an angled reflection setup. The detection of nonlinearity can be done by any of the following methods:

1. Two frequency mixing by transmitting two frequencies f_1 and f_2 . Signals are then received at the difference and/or sum frequencies f_1-f_2 and f_1+f_2 ;

2. Amplitude modulated signal by transmitting a signal $p=(1+A\sin 2\pi f_m t) \sin 2\pi f_0 t$ and then receiving at the modulation frequency f_m and/or its harmonics, e.g., $2f_m$;

3. Transmit one high imaging frequency f_i and one low pumping frequency f_p and then receive at the sum and/or difference frequencies f_i-f_p and f_i+f_p ; and

5 4. Transmit at one frequency f_0 and receive at the harmonics of the transmit frequency, such as $2f_0, 3f_0, 4f_0, \dots$ or xf_0 .

The following experiment confirms the utility of using and measuring acoustic nonlinearity to measure differences in bone characteristics between osteoporotic patients and healthy persons.

10 The setup is shown in Figure 8. The two signal generators 54 (in this example a *Wavetek 185* and a *Wavetek 148A*) were configured to generate 30 cycles long sine wave bursts with center frequency 100 kHz, with pulse repetition frequency 1 kHz. The bursts were amplified 50 dB in the power amplifier 59 (in this example an *ENI 2100L*), and transferred to the transmitting transducer 61 (in this example a *Panametrics Videoscan V1011, 100kHz,*
15 $\varnothing 1.5''$).

The heel of the person to be investigated 64 was placed between the transmitting transducer 61 and receiving transducer 72 (in this example a *Panametrics Accuscan A301S, 500 kHz, \varnothing 1.0''*). Sound pulses from the transmitting transducer 61 traversed through the heel bone of the person 64, and were picked up by the receiving transducer 72. The received
20 signals were sampled by the digital oscilloscope 88 (in this example a *Tektronix TDS 210*), averaged over 64 traces, and transferred to a laptop computer 90 via RS232 interface 92. Data collection and processing was done using proprietary software written in *Matlab*. The transmit amplitude voltage was varied in at least 6 steps for each heel, spanning a range from 5 to 150 V.

25 Power spectra were calculated using Fast Fourier Transforms on the received pulses enveloped in a Hanning window. The received level at the transmit frequency and its harmonics were then found. An example of such a plot is shown in Figure 9 where the transmit frequency and its harmonics are easily recognized as peaks. The received level at the transmit frequency and the level of its second harmonic is shown in figure 10. The difference
30 between the two levels were plotted as function of transmit voltage in a scatter diagram in Figure 11. In figure 10 and 11, a logarithmic axis was used for the transmit voltage, while the received power was plotted in decibels. In these diagrams, the points lie on almost straight lines..

The strength of the second harmonic normalized for transmit voltage was calculated from the fitted straight lines in Figure 10 and 11. First order polynomials were fitted to the data by minimizing least square error. The resulting two coefficients represent slope and level of the straight lines. *Level* is received power in decibels, dB, normalized to driving voltage amplitude 1 Volt. *Slope* is measured as $\text{dB}/\log_{10}(V)$, where V is the driving voltage amplitude in Volts and \log_{10} is base-10 logarithm.

Five patients with confirmed osteoporosis and six healthy volunteers were investigated using this method. The left and right heels of the persons were measured. Regression coefficients from all these investigations were presented as scatter plots. Figure 12 indicates the level of the second harmonic relative to the level at the transmitted frequency. This data shows a significant difference between the healthy and the diseased individuals: The persons with confirmed osteoporosis give a higher relative second harmonic level and larger slope than the healthy volunteers.

We conclude that this experiment has shown that the generation of second harmonics is measurably stronger in patients with osteoporosis than in a healthy population. It is possible to use and measure nonlinear generation of second harmonics to diagnose osteoporosis.

It is further appreciated as an embodiment of this measurement technology that to effectively measure bone characteristics using acoustic nonlinearity, a transmitter which minimizes transmission of second harmonics is useful to reduce background signals in the measurement. In standard medical ultrasound imaging, the same transducer is used to transmit and receive. This requires both the transmit frequency and its second harmonic to lie within the transducer's useful frequency band. Contrary to this, transmission measurements like the above example use two different transducers, one to transmit and one to receive. There is no need for the transmitting transducer to be sensitive at the second harmonic. On the contrary, the transmitter should transmit as little second harmonic as possible. Creating a pure sine wave with second harmonic suppressed by 50 dB or more requires a linear power amplifiers of high quality. Such amplifiers are expensive, large, heavy and have high power consumption.

An efficient suppression of the transmitted second harmonic frequency can be obtained by using an inherit property of standard transducers operating in thickness mode. The transducers have resonance peaks also at odd harmonics of the center frequency: Let f_0 be the center frequency, and the transducer sensitivity has peaks near $3f_0$, $5f_0$, $7f_0$, etc. The

transducer has almost zero sensitivity near its even harmonics: $2f_0$, $4f_0$, $6f_0$, etc. This property is used to minimize the transmitted second harmonic.

The transducer is driven at a frequency at $f_d = \frac{1}{2}f_z$, where f_z is the first minimum in the transducer sensitivity, corresponding to approximately one whole wavelength across the transducer thickness. The frequency f_d will be close to the center frequency f_0 , but not necessarily equal to f_0 . The sensitivity minimum around f_z can be quite sharp. Hence, optimizing the transmit frequency to one half of the natural minimum sensitivity can suppress the transmitted second harmonic considerably compared to simply transmitting at the transducer's nominal center frequency.

A second solution to the issue of transmitted second harmonic is to drive the transducer by a square wave. A square wave with exactly 50% duty cycle contains only odd harmonics. The even harmonics, including the second, are suppressed. The crucial part to avoid transmitting a second harmonic, is to keep the duty cycle extremely accurately at 50%. We propose to drive the transmitting transducer with such a square wave, created by the following method. A simple oscillator generates a square wave with arbitrary duty cycle, but well stabilized frequency. This frequency is divided by two in a simple divider circuit. This will result in a square wave output with exactly 50% duty cycle, hence, containing no even harmonics. The accuracy may be improved further by dividing the frequency by a number higher than two. The number need not necessarily be a power of two, any integer can be used. This method allows a small, simple and inexpensive transmit signal generator and amplifier, with very low power dissipation, giving signals with very good performance for our purpose. This is a great improvement compared to using a conventional sine wave generator and a linear power amplifier.

The invention thus recognizes alternate methods and techniques to improve the quality and availability of ultrasound quantitative measurement modalities for various bone conditions. It is recognized that the various techniques may be combined with or substituted for known techniques and systems to achieve an overall improvement in this measurement capability.

What is claimed is:

1. A method of measuring bone condition using ultrasound waves, comprising the steps of:
 - 5 a) transmitting a signal sequence of ultrasound waves for impingement on a bone being measured;
 - b) arranging a detection transducer configuration for receiving a portion of the transmitted signal sequence of ultrasound waves after impingement on the bone being measured; and
 - 10 c) determining the degree of acoustic nonlinearity of the bone to estimate the material conditions of the bone.
2. The method of claim 1 used for detecting bone reduction and conditions related thereto.
- 15 3. The method of claim 1 used to estimate whether the bone is changing from a homogenous to a more heterogeneous structure.
4. The method of claim 1 wherein the nonlinearity of the bone is measured with harmonic frequency detection comprising the steps of:
 - 20 a) transmitting a sound pulse through the bone; and
 - b) measuring the harmonic distortion.
5. The method of claim 4 wherein the second harmonic is sensed.
- 25 6. The method of claim 4 wherein a harmonic higher than the second harmonic is sensed.
7. The method of claim 4 wherein combinations of harmonics are sensed.
- 30 8. The method of claim 1 wherein the nonlinearity of the bone is measured with nonlinear frequency mixing detection comprising the steps of:
 - a) transmitting two frequencies through the bone;
 - b) receiving the transmitted signals; and
 - c) measuring the sum and/or difference frequencies in the received signal.

9. The method of claim 8 wherein the two frequencies transmitted are transmitted by two separate transducers.
- 5 10. The method of claim 8 wherein the two frequencies are transmitted by exciting one transducer with both frequencies.
11. The method claim 9 wherein the transmitted signals are received by one of the transducers that transmitted a frequency.
- 10 12. The method of claim 9 wherein the transmitted signals are received by a third transducer.
13. The method of claim 10 wherein the transmitted signals are received by the transducer
15 that transmitted the frequencies.
14. The method of claim 10 wherein the transmitted signals are received by a second transducer.
- 20 15. The method of claim 1 wherein the nonlinearity of the bone is measured with a combination of harmonic detection and nonlinear frequency mixing detection.
16. The method of claim 15 further comprising the steps of:
- 25 a) transmitting a plurality of signals at different frequencies through the bone;
- b) receiving a portion of the transmitted signals;
- c) measuring the sum and/or difference frequencies of a first transmit frequency combined with the harmonics of a second transmit frequency.
- 30 17. The method of claim 15 further comprising the steps of:
- a) transmitting two frequencies through the bone;
- b) receiving the transmitted signals;
- c) measuring the sum and/or difference frequencies of the harmonics of the transmit frequencies.

18. The method of claim 1 used in conjunction with other measurement techniques.
19. The method of claim 18 where the other measurement technique measures at least one
5 of reflection of sound and scatter of sound.
20. The method of claim 18 where the other measurement technique measures attenuation
of sound.
- 10 21. The method of claim 18 where the other measurement technique measures speed of
sound.
22. The method of claim 1 used in conjunction with estimates for elastic properties.
- 15 23. The method of claim 1 used in conjunction with measurements of shape.
24. The method of claim 1 used in conjunction with measurements of geometrical
dimensions.
- 20 25. A method for diagnosing osteoporosis comprising the steps of:
a) transmitting a signal sequence of ultrasound waves for impingement on
a bone being measured;
b) arranging a detection transducer configuration for receiving a portion
of the transmitted signal sequence of ultrasound waves after impingement on the bone
being measured; and
25 c) measuring the degree of acoustic nonlinearity of the bone to estimate
the material conditions of the bone indicative of the onset of osteoporosis.
26. The method of claim 25 further comprising the step of assigning the measured bone
30 portion a bone strength index.
27. The method of claim 26 further comprising the step of repeatedly comparing
sequential time spaced measurements of the same bone structure to identify onset or
susceptibility to bone disease.

28. The method of claim 25 in which the step of measuring the degree of acoustic nonlinearity of the bone comprises:

- 5 a) transmission to achieve a two frequency mixing by transmitting two frequencies f_1 and f_2 ; and
- b) receipt of f_1 and f_2 at the difference and/or sum frequencies f_1-f_2 and f_1+f_2 .

29. The method of claim 25 in which the step of measuring the degree of acoustic nonlinearity of the bone comprises:

- 10 a) transmission of an amplitude modulated signal by transmitting a signal $p=(1+A\sin 2\pi f_m t) \sin 2\pi f_0 t$; and
- b) receiving the signal at a modulation frequency f_m and a selected second or higher harmonic of that frequency.

30. The method of claim 25 in which the step of measuring the degree of acoustic nonlinearity of the bone comprises:

- 15 a) transmission of signals comprising one high imaging frequency f_i and one low pumping frequency f_p ; and
- 20 b) receiving the signals at sum and/or difference frequencies f_i-f_p and f_i+f_p .

31. The method of claim 25 in which the step of measuring the degree of acoustic nonlinearity of the bone comprises:

- 25 a) transmission of a signal comprising one transmit frequency f_0 ; and
- b) receiving the signal at a harmonic of the transmit frequency.

32. A method of measuring bone strength comprising the steps of:

- 30 a) measuring the shear wave velocity (c_s);
- b) estimating the Lamé coefficient shear modulus (μ) of the bone by use of the formula:

$$C_s = \sqrt{\frac{\mu}{\rho}} \quad \text{and}$$

c) assigning a bone strength index of measure based on the estimate of shear modulus.

5

33. The method of claim 32 further comprising the additional step of measuring bone strength by measuring the degree of nonlinearity of the bone to estimate the material conditions of the bone.

10

34. The method of claim 32 used in conjunction with other measurement techniques.

35. The method of claim 34 where the other measurement technique measures reflection of sound.

15

36. The method of claim 34 where the other measurement technique measures scatter of sound.

37. The method of claim 34 where the other measurement technique measures attenuation of sound.

20

38. The method of claim 34 where the other measurement technique measures speed of sound.

39. The method of claim 34 used in conjunction with estimates for elastic properties.

25

40. The method of claim 34 used in conjunction with measurements of shape.

41. The method of claim 34 used in conjunction with measurements of geometrical dimensions.

30

42. A method for diagnosing osteoporosis comprising the steps of:

- a) measuring the pressure wave velocity through a patient's bone;
- b) measuring the shear wave velocity through a patient's bone;

c) calculating the ratio of shear wave velocity to the pressure wave velocity to determine whether the bone is degraded.

43. The method of claim 42 further including calculating the speed of sound in the bone
5 by transmitting ultrasonic waves using a transmitter placed on the surface of a patient's skin,
through the tissue to the bone at a predetermined angle, receiving ultrasonic waves refracted
from the bone at a receiver positioned on the surface of a patient's skin a known distance
from the transmitter, and measuring the time of the first arrival of refracted ultrasonic wave at
the receiver.

10

44. A device for measuring bone density comprising a means for measuring the shear
wave velocity through a patient's bone.

15

45. The device of claim 44 wherein a first transducer transmits a wave into the patient's
bone and a second transducer receives the wave.

46. The device of claim 45 wherein the first and second transducers are the same transducer.

20

47. The device of claim 44 further comprising a means for measuring the pressure wave
velocity through a patient's bone.

48. A system for measuring bone density by measuring the shear wave velocity through a
patient's bone.

25

49. A method of measuring bone density comprising the step of measuring the phase
velocity as a function of frequency.

50. The method of claim 49 further comprising the step of measuring the frequency
dependant attenuation.

30

51. The method of claim 49 further comprising the steps of

a) measuring the degree of nonlinearity of the bone to estimate the
material conditions of the bone; and

b) measuring the shear wave velocity and estimating the shear modulus (μ) of the bone.

52. The method of claim 49 used in conjunction with other measurement techniques.

5

53. The method of claim 52 where the other measurement technique measures reflection of sound.

54. The method of claim 52 where the other measurement technique measures scatter of sound.

10

55. The method of claim 52 where the other measurement technique measures attenuation of sound.

15

56. The method of claim 52 where the other measurement technique measures speed of sound.

57. The method of claim 49 used in conjunction with estimates for elastic properties.

20

58. The method of claim 49 used in conjunction with measurements of shape.

59. The method of claim 49 used in conjunction with measurements of geometrical dimensions.

25

60. A device for measuring bone density comprising a means for measuring the phase velocity as a function of frequency.

61. A system for measuring bone density comprising a means for measuring the phase velocity as a function of frequency.

30

62. A method for diagnosing osteoporosis comprising the steps of:

- 1) placing a transmitter of ultrasonic waves on a predetermined area on the surface of a patient's skin;
- 2) placing a receiver of ultrasonic waves on an area on the surface of the patient's skin a known distance from the transmitter;
- 5 3) transmitting ultrasonic waves through the tissue to the bone at a predetermined angle;
- 4) measuring the time of the arrival of the first ultrasonic wave by the receiver; and
- 10 5) calculating the speed of sound in the bone using the time of arrival of the first ultrasonic wave.

63. A system for diagnosing osteoporosis comprising:

- 1) a transmitter configured for transmitting ultrasonic waves onto a predetermined area on the surface of a patient's skin and through the tissue to the bone so as to create a surface wave at a bone-tissue interface region that is measurable by a receiver of the ultrasonic surface wave;
- 15 2) at least one receiver of ultrasonic waves on an area on the surface of the patient's skin a known distance from the transmitter; and
- 20 3) analysis circuitry for measuring the surface wave velocity and translating the measured velocity into an indicator of bone health status.

64. The system of claim 63 in which the transmitter is configured so that the tissue-bone interface is in the acoustic near field of the transmitter.

25 65. The system of claim 63 comprising means for selectively either vertically polarizing or horizontally polarizing the surface wave that is generated.

66. An ultrasound transmission process comprising the steps of;

- 30 1) determining a resonance frequency of a transducer's minimum sensitivity;
- 2) operating the transducer at one-half of the so determined frequency.

67. The ultrasound transmission process of claim 66, wherein the resonance frequency determined is the first resonance frequency of the transducer's minimum sensitivity.

68. An ultrasound transmission process comprising the steps of;
- 1) generating a square wave with a well-stabilized frequency;
 - 2) dividing the frequency by an integer in a divider circuit.

5

69. The ultrasound transmission process of claim 68, wherein the frequency is divided by two.

Fig. 1

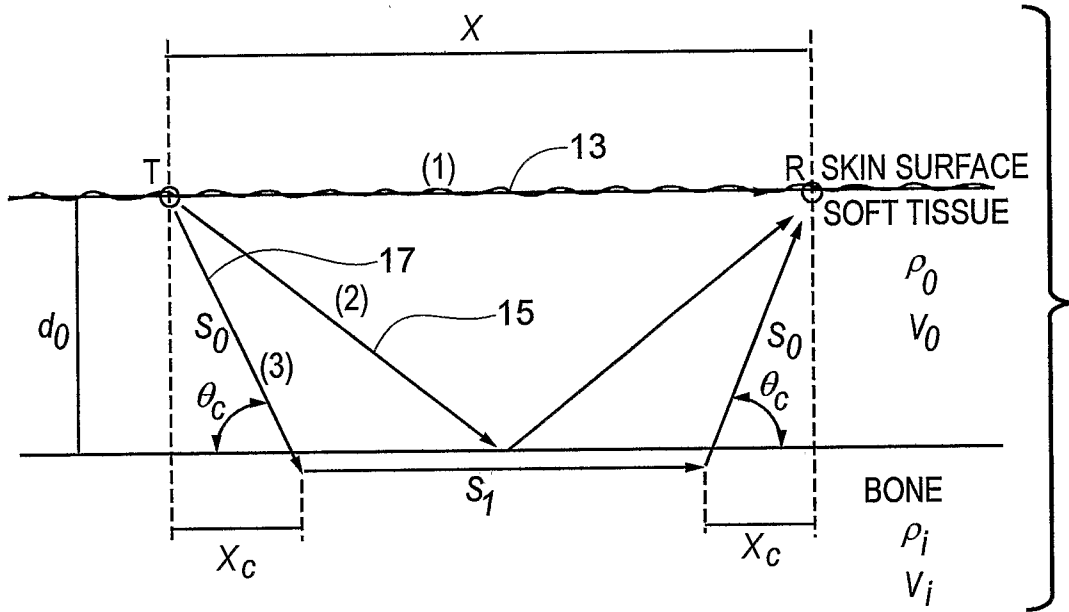


Fig. 2

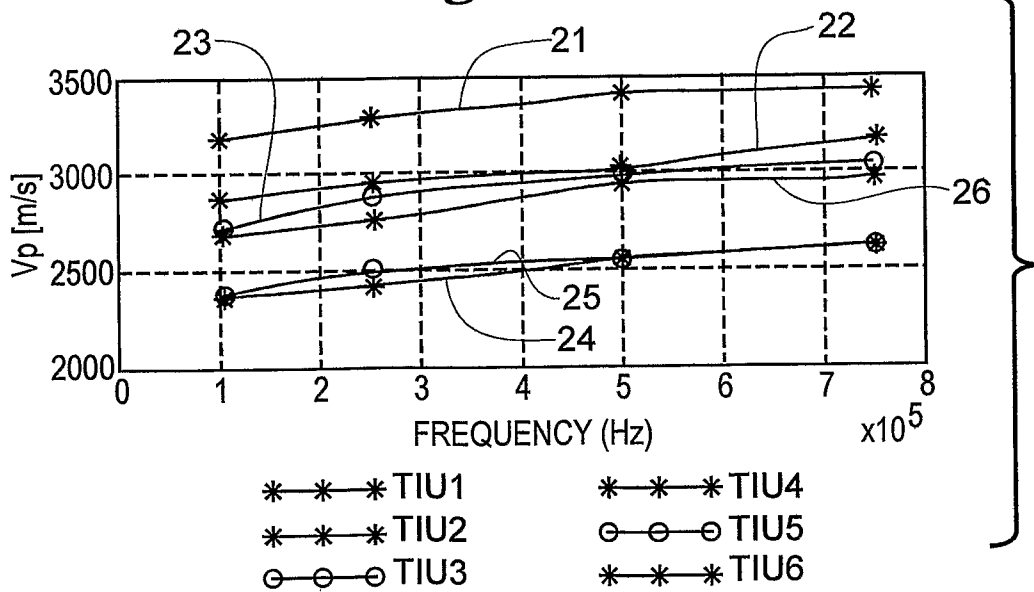


Fig. 3

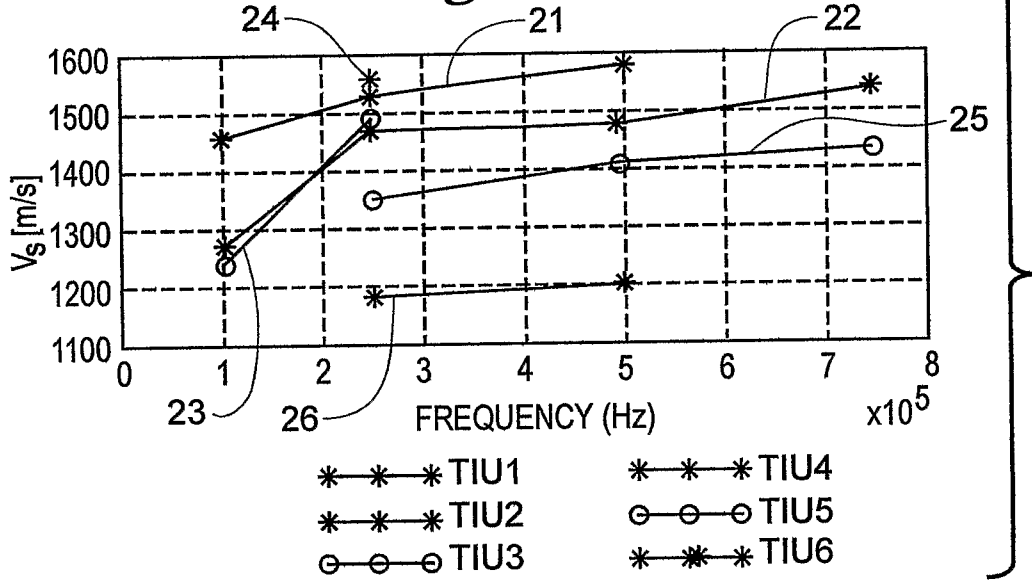


Fig. 4

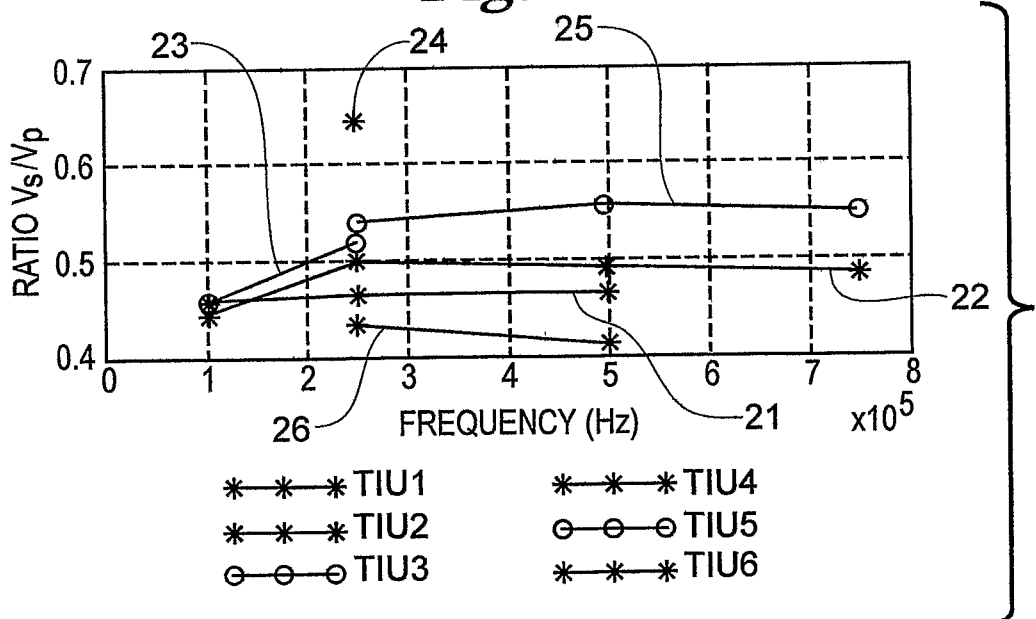


Fig. 5

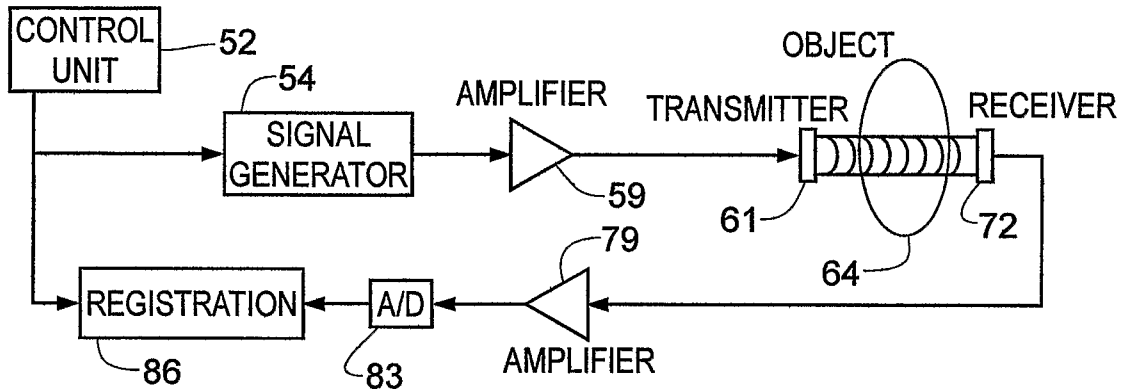


Fig. 6

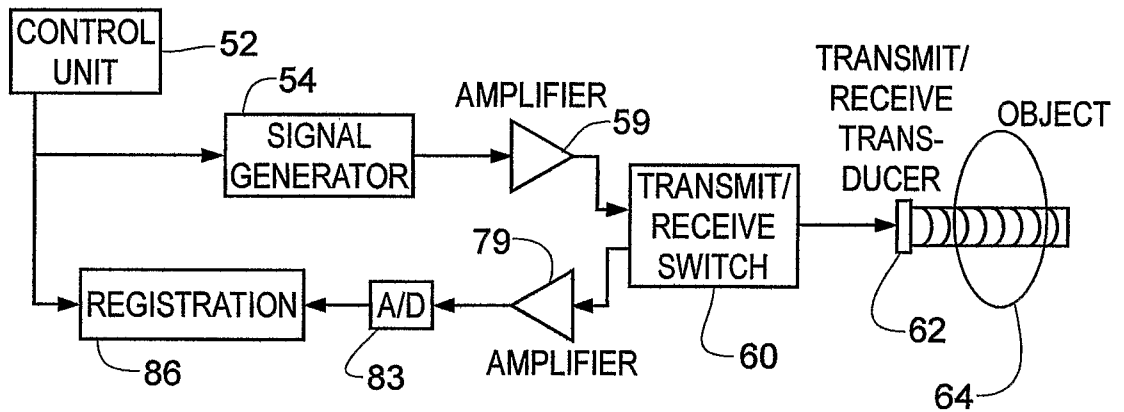


Fig. 7

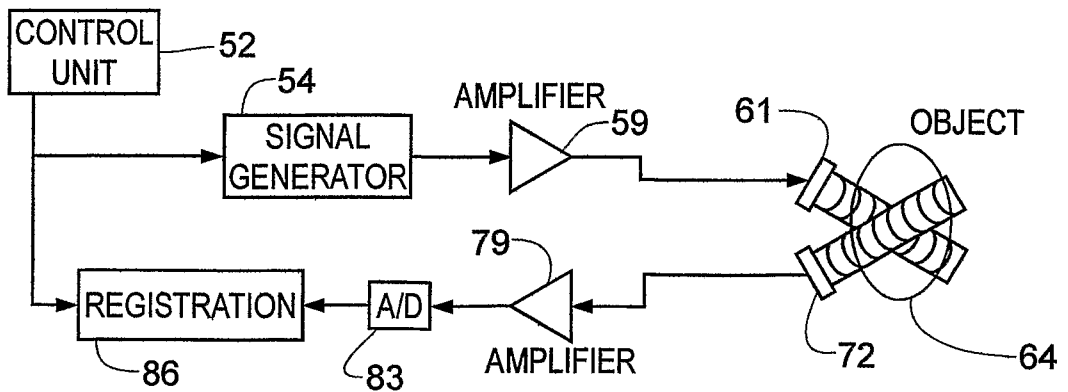


Fig. 8

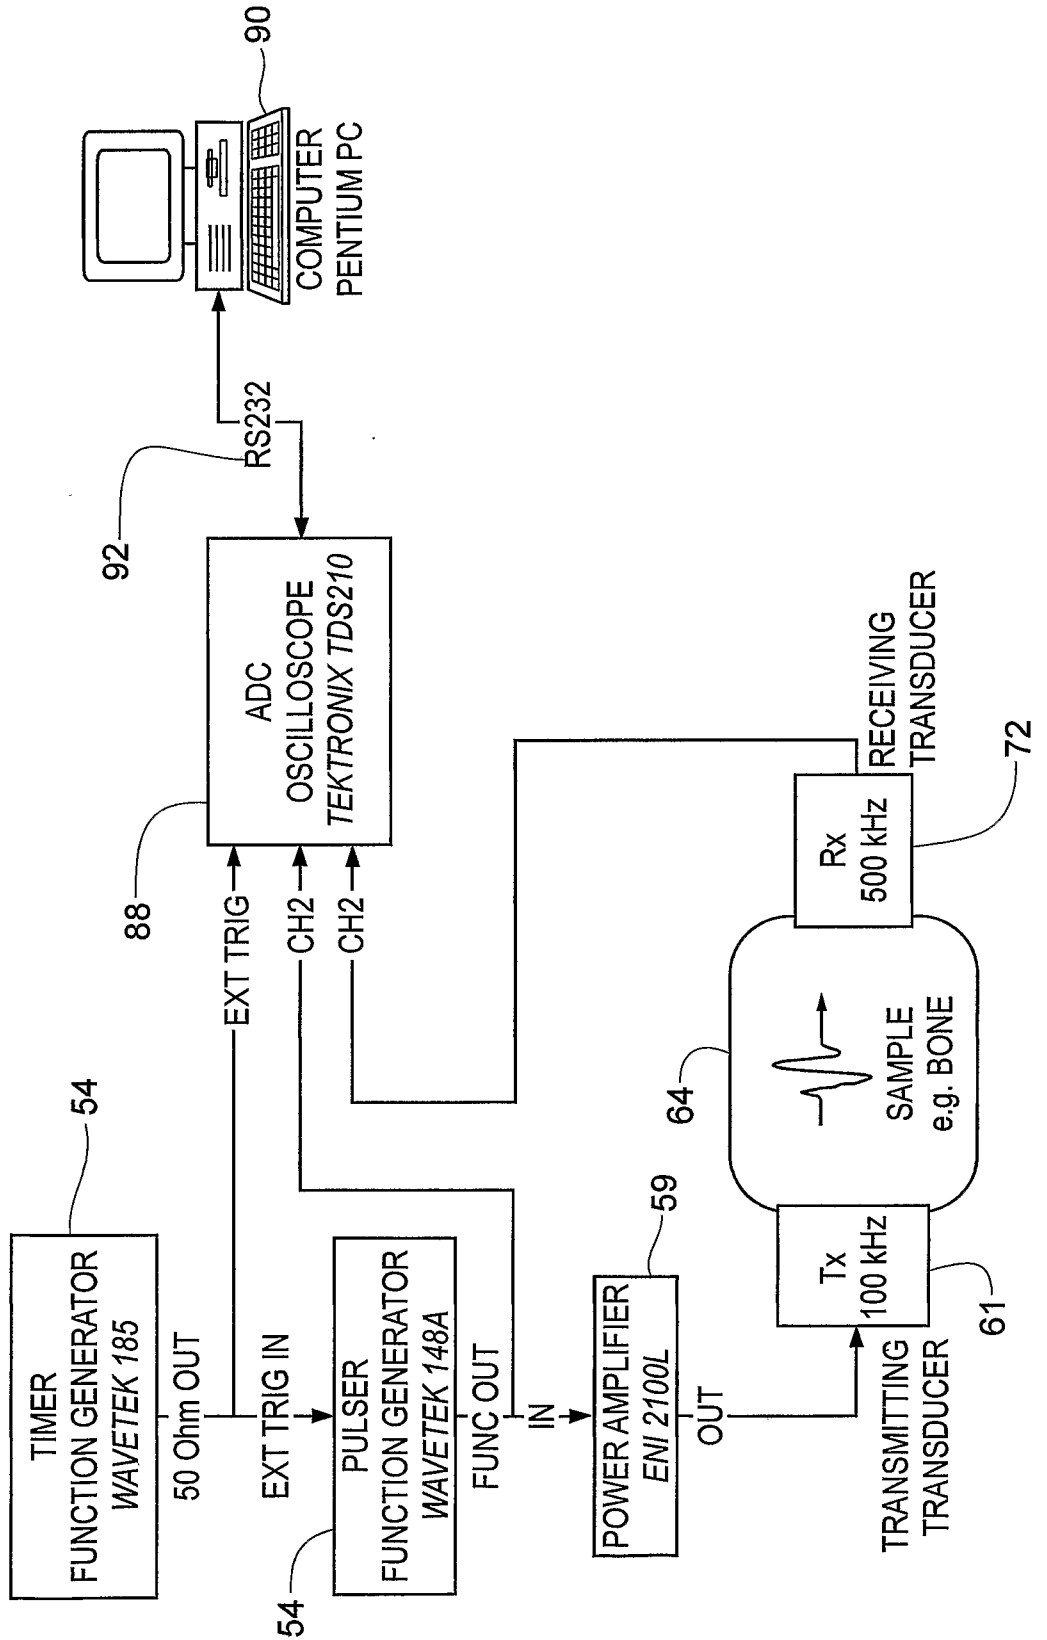


Fig. 9

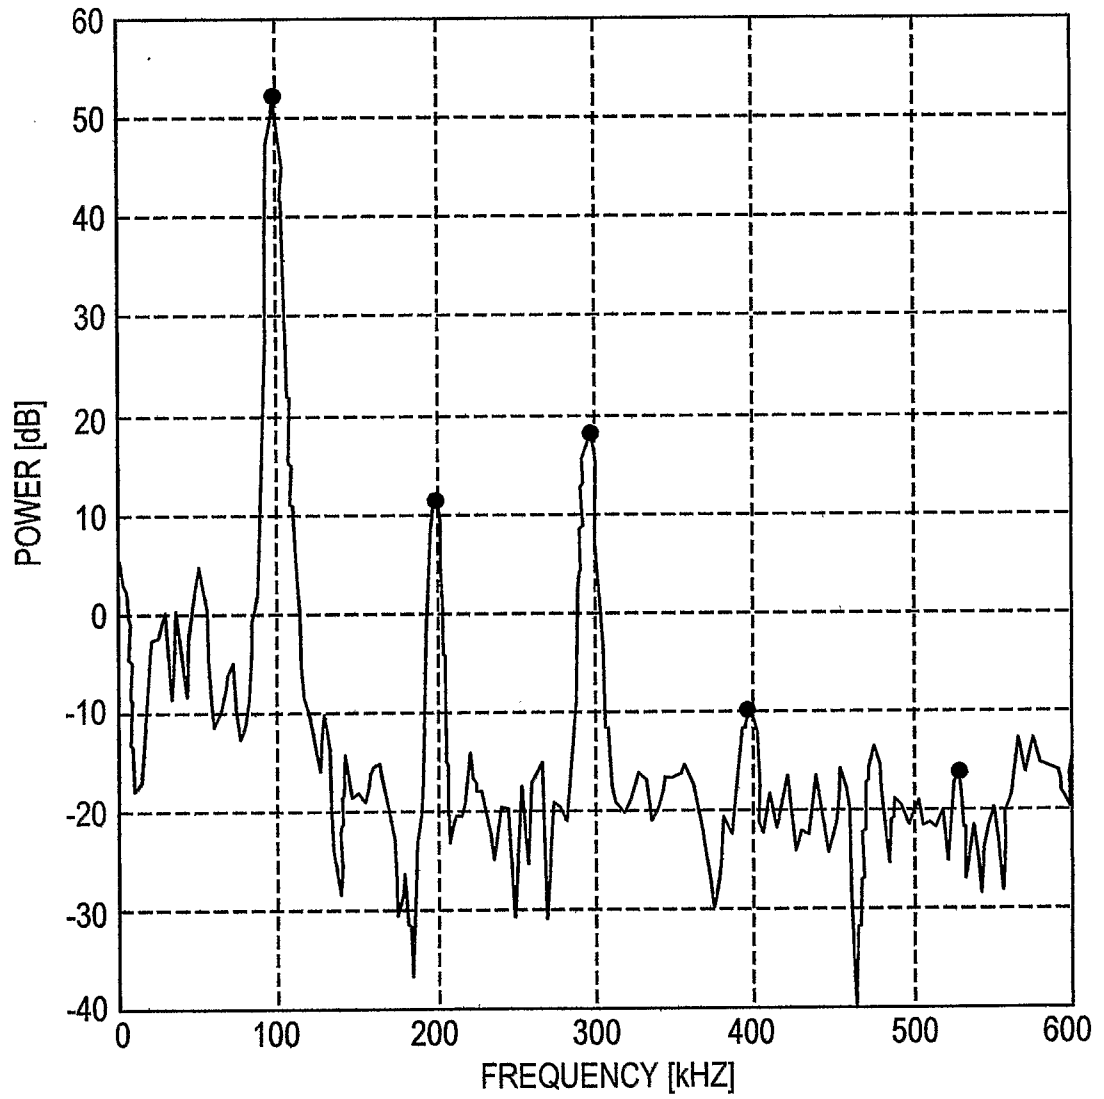


Fig. 10

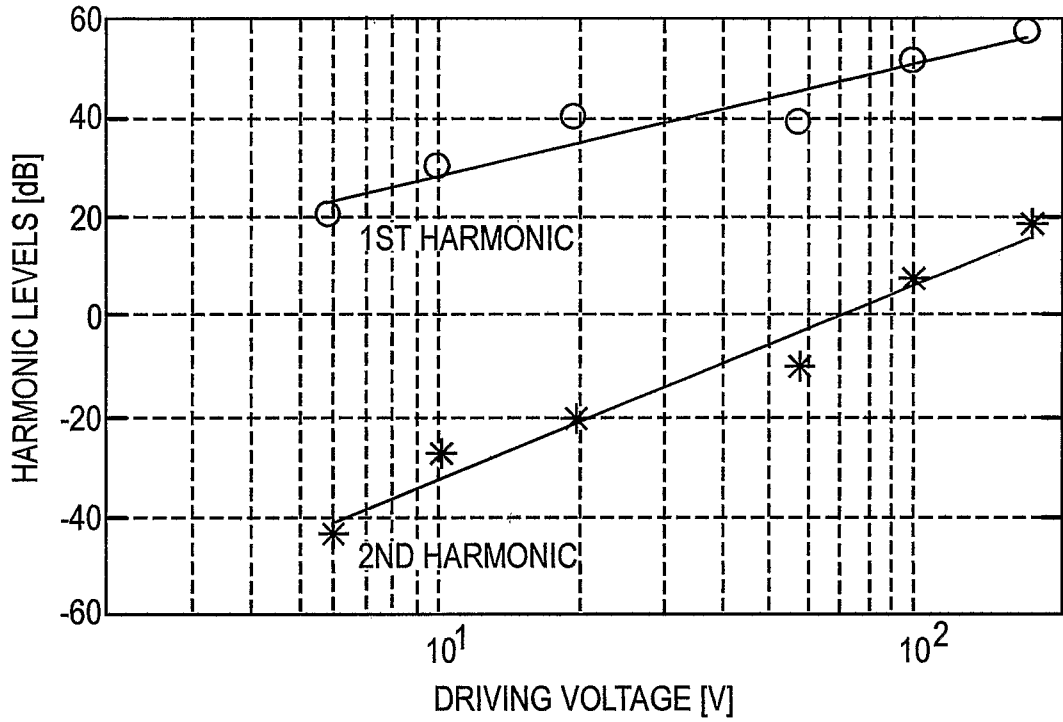


Fig. 11


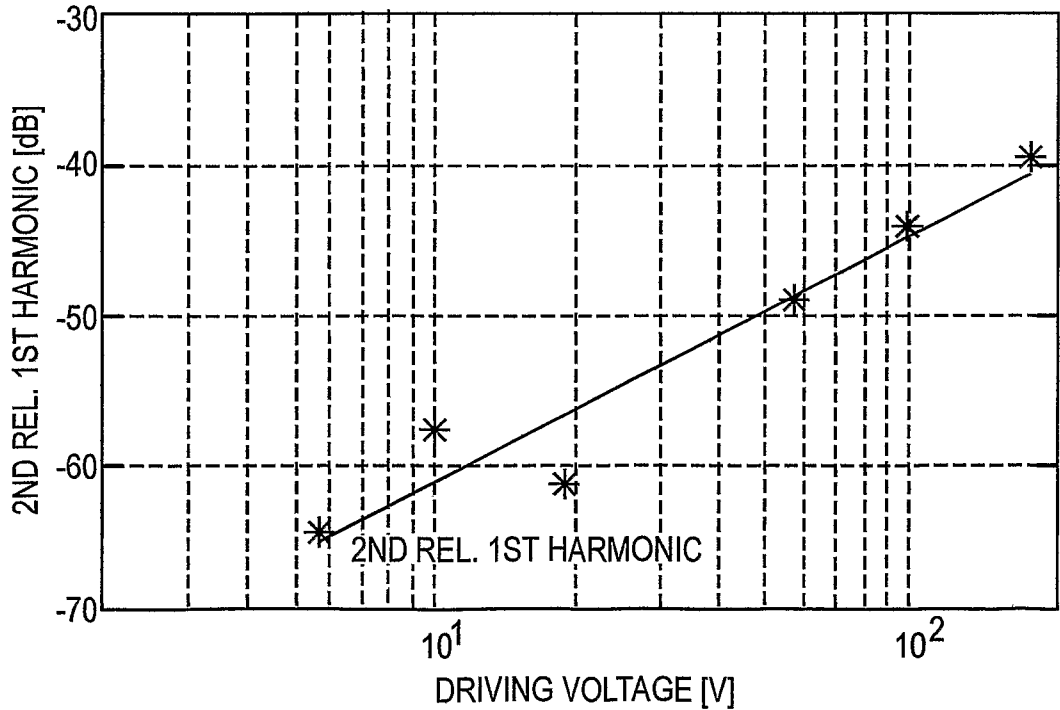


Fig. 12

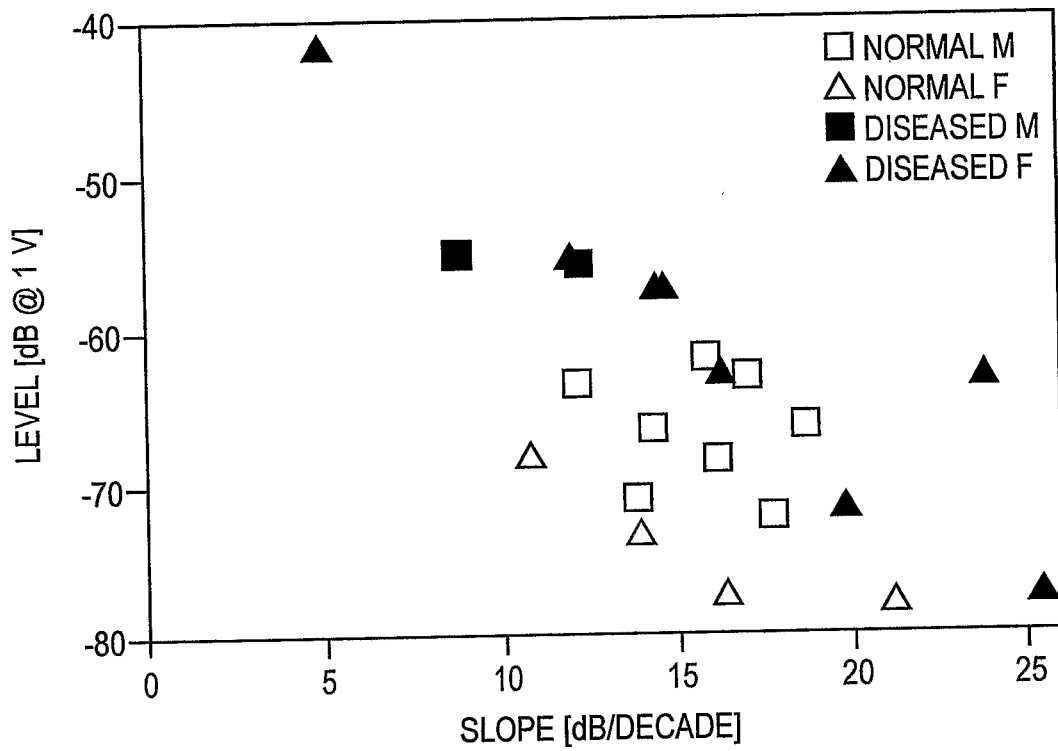

专利名称(译)	用于骨骼分析的超声测量技术		
公开(公告)号	EP1448100A2	公开(公告)日	2004-08-25
申请号	EP2002781493	申请日	2002-10-18
[标]申请(专利权)人(译)	HOFF LARS OYGARDEN KJELL		
申请(专利权)人(译)	霍夫LARS OYGARDEN谢尔		
当前申请(专利权)人(译)	霍夫LARS OYGARDEN谢尔		
[标]发明人	HOFF LARS OYGARDEN KJELL		
发明人	HOFF, LARS OYGARDEN, KJELL		
IPC分类号	A61B8/08 A61B8/00		
CPC分类号	A61B8/0875 A61B8/485		
外部链接	Espacenet		

摘要(译)

使用非线性分析结合或替代地使用剪切波进行超声波测量骨质量提供了关于人类骨骼状况的改进信息。表面波还提供了一种估算剪切波速的新方法。