

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
4 December 2003 (04.12.2003)

PCT

(10) International Publication Number
WO 03/099129 A1

(51) International Patent Classification⁷: **A61B 8/00**,
A47B 21/03, G01S 15/89, G06F 3/02

(21) International Application Number: PCT/IB03/02290

(22) International Filing Date: 21 May 2003 (21.05.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
10/154,733 23 May 2002 (23.05.2002) US

(71) Applicant: **KONINKLIJKE PHILIPS ELECTRONICS N.V. [NL/NL]**; Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).

(72) Inventors: **WILKINS, Jay**; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **MESAROS, Robert**; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **MATSUI, Yas**; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **LORD, Randall, D.**; c/o Prof. Holstlaan

6, NL-5656 AA Eindhoven (NL). **MURKOWSKI, John, R.**; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **HOLLMAN, William**; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **RANKERS, Ulrich**; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).


(74) Agent: **LOTTIN, Claudine**; Internationaal Octrooibureau B.V., c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: EXAMINATION ULTRASOUND SYSTEM CART WITH VARIABLE ELEVATION CONTROL PANEL

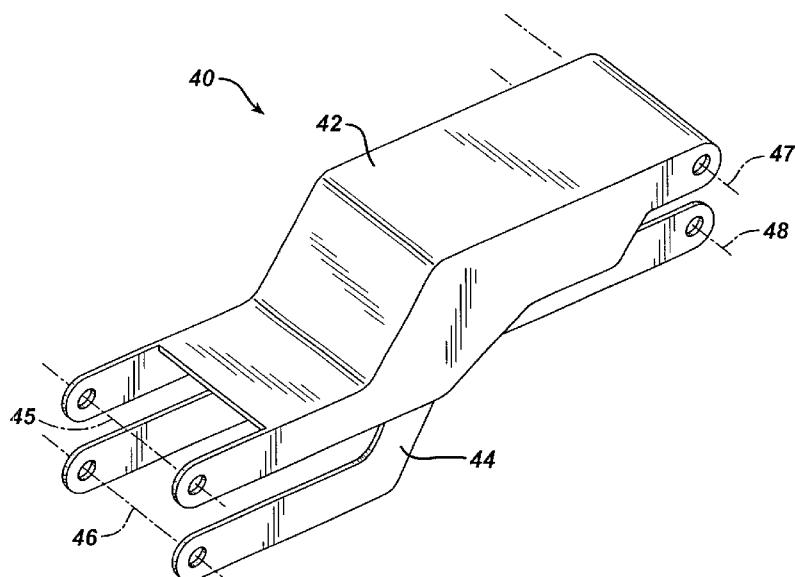

WO 03/099129 A1

(57) Abstract: A cart-borne ultrasound system is described which includes a portable cart holding the electronic circuitry of the ultrasound system, a control panel for controlling the ultrasound system, and a display. The control panel is supported by an articulating mechanism which enables the control panel to be raised and lowered to accommodate operators of different height, and enables the control panel to move toward and away from the user to accommodate users in the sitting or standing positions. In a preferred embodiment the articulating mechanism comprises a parallelogram-shaped linkage which also maintains a constant angle of inclination of the control panel as it is raised and lowered.

**Declaration under Rule 4.17:**

— *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii)) for the following designation CN*

— *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments*

Published:

— *with international search report*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Examination ultrasound system cart with variable elevation control panel

This invention relates to ultrasonic examination imaging systems and, in particular, to ultrasound systems with control panels that have an adjustable height.

Cart-borne ultrasound systems are intended to be operated by any examinationian with the requisite training. This means that the ultrasound system may be used by some who are short in stature and others who are very tall. The system should adapt to people of different height. Otherwise, the operator may need to stretch, bend over, or otherwise contort to an uncomfortable position. Over time such contortions can lead to muscular or skeletal discomfort. To relieve these problems some manufacturers have designed the ultrasound system cart so that the control panel can be adjusted vertically. One simple approach is to hinge the control panel so that it will swing up and down. As it does so, however, it will assume a different angle at each elevational height. It is desirable for the control panel to maintain a constant angle to the operator so that the control panel is comfortable to use regardless of its elevation.

One way to maintain a constant angle is to elevate the entire control and display portion of the ultrasound system. Such an approach should take into consideration the posture of users of the ultrasound system when the control panel and display are elevated to different heights. In particular, an elevation system should provide positions of comfort for both standing and sitting users. It is desirable to provide a control panel for an ultrasound system which maintains a comfortable user angle to the operator and is comfortable for both sitting and standing users.

In accordance with the principles of the present invention a variable elevation control panel is provided for a cart-borne ultrasound system. The control panel is supported by an articulating mechanism by which the height of the control panel can be adjusted. Preferably the control panel maintains a comfortable angle of inclination as its height is changed. As the control panel is articulated vertically it simultaneously extends toward the user when lowered to better accommodate a sitting user, and extends back toward the cart when raised to better accommodate a standing user. In one embodiment the articulation mechanism is configured as a parallelogram-shaped linkage. In another embodiment the

articulation mechanism raises and lowers the control panel at an acute angle to the vertical direction.

5

In the drawings:

Fig. 1 illustrates a cart-borne ultrasound system in perspective;

Fig. 2 illustrates the concept of a control panel lift mechanism of the present invention;

Fig. 3 shows the mechanism of Fig. 2 with a control panel in an end view;

10 Fig. 4 illustrates the control panel lift mechanism of a constructed embodiment of the present invention;

Fig. 5a illustrates a preferred lift mechanism in the raised position;

Fig. 5b illustrates a preferred lift mechanism in the lowered position;

15 Figs. 6a and 6b illustrate a further embodiment of the present invention in the lowered position; and

Figs. 7a and 7b illustrate the embodiment of Figs. 6a and 6b in the raised position.

20

Referring first to Fig. 1, a cart-borne ultrasound system 10 is shown in perspective. The cart includes an electronics bay 12 inside of which are located printed circuit boards for electronically processing received ultrasound signals. The ultrasound signals are processed to produce an image which is displayed on a display 16. The cart is mounted on wheels or casters 14 so that it can be rolled to a lab or a patient's bedside. In the front of the cart is a control panel 18, which contains a number of knobs, buttons, slide switches, and a trackball by which a user operates the ultrasound system. The control panel is mounted above a handle 20 which extends from the front of the ultrasound system. The handle 20 can be used to pull the cart to move it from one location to another. On the inside of the handle 20 is a lift release 22 which will be discussed below.

25

The concept of a lift mechanism of the present invention is shown in Fig. 2. A four bar linkage 30 is defined by four pivot points, A, B, A' and B'. Two of the bars are shown at 32 and 34, with the other two bars comprised by the pivot connections to the control panel 18 at A and B and the pivot connections to a base (not shown) at A' and B'. The linkage is shown in a raised position and a lowered position by the upper and lower locations

of the control panel 18. The control panel moves between these positions as indicated by the large arrow. As can be seen by the block representation of the control panel 18, the angle of the control panel 18 does not change as the control panel is raised and lowered. In this drawing it is seen that the horizontal and vertical sides of the control panel block remain in 5 this orientation in the raised and lowered and all intermediate positions.

Fig. 3 illustrates the four bar linkage 30 with the control panel 18 shown in a side view. As this drawing illustrates, the control panel is tilted at an angle which is comfortable for the user. Again it is seen that the angle of the control panel does not change between the raised and lowered positions by reason of the four bar linkage 30, which in the 10 preferred embodiment is a parallelogram-shaped mechanism providing this benefit. The bars 30 and 32 remain parallel as the linkage moves, as do the axes between pivot points A-B and A'-B'.

Fig. 4 illustrates another articulating linkage 40 for a control panel which is suitable for use with the ultrasound system cart shown in Fig. 1. This linkage comprises a lift top cover 42 and a lift bottom cover 44. Each lift cover has two pivot holes at the front which are aligned on horizontal axes 45,46 and two pivot holes at the back which are aligned on 15 horizontal axes 47,48. This lift cover assembly is partially visible behind the control panel 18 in Fig. 1. It is approximately 6 inches wide and 15 inches in length. The rear pivot holes at axes 47,48 are mounted to the ultrasound system cart and the control panel is mounted in the 20 vicinity of front pivot holes at axes 45,46 as shown in the following drawings. If desired, beard covers can be provided below the linkage 40 to prevent the development of pinch points below the linkage when the control panel is elevated, as shown in concurrently filed US patent [application serial number ATL-295] incorporated herein by reference.

Fig. 5a illustrates the linkage assembly 40 in a raised position when attached 25 to an ultrasound system cart. The two rear pivot points 47,48 of the assembly are connected to a lift base bracket 56, which is attached to the ultrasound system cart. The two forward pivot points are attached to a base for an ultrasound system control panel by attachment to an articulation base support 54 which supports the base. The base includes a bearing 50 on which is mounted a base slide 52. When the control panel is mounted on the base slide, it can 30 slide forward and backward (left-right in the drawing) to an extended or retracted position selected by the system operator. Below the base the handle 20 is seen in a cutaway view.

As this drawing illustrates, the control panel can be raised and lowered by grasping the handle 20 to move the handle and control panel up and down, as both the handle and control panel are mounted on the articulating linkage 40. The articulating linkage is seen

to be a four bar, parallelogram shaped linkage, as indicated by the lines w,x,y, and z drawn between the four pivot points 45,46,47,48 of the linkage.

Located beneath the lift top cover 42 is a positive lock, hydraulic piston 60 shown in phantom in Fig. 5a. The piston 60 supports the weight of the linkage, control panel and handle and is normally locked to maintain the positions of these elements. When the operator desires to raise or lower the control panel the handle 20 is grasped and the lift release 22 on the handle is depressed. The lift release could alternatively be operated by a foot pedal or located elsewhere on the cart. When the lift release 22 is depressed a valve is opened between two oil-filled compartments of the hydraulic piston. Oil then flows slowly from one compartment to the other, the direction of flow depending upon whether the control panel is being raised or lowered. The piston will extend or retract as the oil flows. When the control panel is at the desired height, the lift release is released by the operator, causing the valve of the piston to close, holding the piston and the control panel in its current elevation.

Fig. 5b shows the linkage 40 and piston 60 when the control panel is in a lowered position. It is seen that the piston is in a retracted position in comparison to Fig. 5a. It is also seen that the angle of the control panel has not changed.

When the control panel is elevated such that the parallelogram w,x,y,z of the linkage 40 forms a rectangle, the control panel is at its most forward position relative to the cart and the center of the cart, which is approximately the vertical plane of the display 16. The control panel can be rolled forward even further toward the operator by sliding the control panel on the base slide 52. In this lowered position the control panel can be positioned over the lap of a system operator who is in the sitting position. As the control panel is raised from this elevation the sides x,z of the parallelogram will draw closer together and the control panel will simultaneously pivot up and rearward toward the center of the cart. In this raised position the control panel is retracted back to be more comfortable for use by an operator who is standing for the ultrasonic exam. In a constructed embodiment the control panel has approximately a ten inch range of vertical adjustment.

Various modifications of the illustrated embodiments will be readily apparent to those skilled in the art. For instance, the four bar linkage can be modified to have more than four pivot points, permitting more complex ranges of control panel movement. Instead of being manually raised and lowered, the control panel could be raised and lowered by motor control. The hydraulic piston can be a gas shock or replaced by other supporting devices such as springs or counterweights, in which case the elevation locking mechanism may comprise a mechanical device such as a detent or locking pin.

Figs. 6a, 6b, 7a and 7b illustrate another embodiment of the present invention in which both the control panel and display are elevated and lowered by motor control. A cart-borne ultrasound system 70 includes a frame 72 mounted on wheels 14. The system display 16 and control panel 18 are supported on a yoke 74. The yoke 74 houses an articulation telescope bearing system which includes two shafts 78 which turn two threads 80. One shaft and thread is located on each side of the yoke 74. The shafts 78 are rotated by a $\frac{1}{4}$ hp DC motor 82, which is connected to one shaft 78 by a gearbox 83. Also connected to the gearbox is a pulley assembly 84, which is connected to a similar pulley assembly on the other side of the yoke by a belt 88. An idler 86 maintains the proper belt tension. Figs. 6a and 10 6b illustrate the ultrasound system 70 with the control panel and display in the lowered position. When the shafts 78 are rotated by the motor, gearbox, and pulley mechanism, the threads turn and cause the yoke to raise, lifting the control panel and display to a greater height, as shown in Figs. 7a and 7b. When the shafts are rotated in the opposite direction the control panel and display are lowered.

15 In accordance with the principles of the present invention, the articulation assembly does not move in the vertical direction, but at an acute angle θ with respect to vertical. This angled motion will cause the control panel and display to move forward toward the front of the cart when lowered, and to move backward away from the front of the cart when raised. Consequently, the control panel and display will be retracted back to better 20 serve a standing user, and will move forward to extend over the lap of a sitting user. The angle of the control panel and display will not change as they are lowered, but will be maintained at the desired angle of comfort. In the illustrated embodiment the articulation mechanism is at approximately a 10° angle from vertical.

In a preferred embodiment the ultrasound system 70 includes a 12 volt battery 25 which will power the articulation system when the power supply of the cart is not plugged in or energized. This enables the elevation of the control panel and display to be changed for transport of the system, without the need to power up the system's DC power supply from an a.c. source. The embodiment of FIGURES 6a-7b has been tested by lifting 150 pounds, and can be controlled by a simple pushbutton or rocker switch on the cart.

CLAIMS:

1. A cart-borne ultrasound system (10) including a movable cart having a center; electronic circuitry located on the cart which processes ultrasound signals for the formation of ultrasound images, and a display (16) coupled to the circuitry for the display of ultrasound images, comprising:

- 5 - a control panel (18) coupled to the electronic circuitry for user control of the ultrasound system (10); and
- an articulation mechanism (30) mounted on the cart and coupled to the control panel (18) which enables the control panel (18) to be articulated vertically while maintaining a substantially constant angle of inclination, the articulation mechanism (30) further enabling
10 the control panel (18) to move closer to the center of the cart in the highest position and further from the center of the cart in the lowest position.

2. The cart-borne ultrasound system (10) of claim 1, wherein the articulation mechanism (30) enables the control panel (18) to be articulated independently of the display (16).

3. The cart-borne ultrasound system (10) of claim 1, wherein the articulation mechanism (30) comprises four pivot points (A, B, A', B') defining the corners of a parallelogram.

- 20 4. The cart-borne ultrasound system (10) of claim 3, wherein two of the pivot points (A, B) of the articulation mechanism (30) are coupled to the control panel (18) and two of the pivot points (A', B') of the articulation mechanism (30) are coupled to the cart.

- 25 5. The cart-borne ultrasound system (10) of claim 1, further comprising a counterbalance (40) coupled to the cart and to the control panel (18) to support at least some of the weight of the control panel (18) when the height of the control panel (18) is adjusted.

6. The cart-borne ultrasound system (10) of claim 1, wherein the articulation mechanism (30) comprises a lift mechanism (32, 34) which moves the control panel (18) in a direction which is at an acute angle with respect to vertical.

5 7. The cart-borne ultrasound system (10) of claim 6, wherein the lift mechanism (32, 34) raises and lowers the control panel (18) in a straight line direction.


8. The cart-borne ultrasound system (70) of claim 6, wherein the lift mechanism (74) is motor driven.

10 9. The cart-borne ultrasound system (70) of claim 8, wherein the ultrasound system further comprises a battery which powers the motor driven lift mechanism (74).



15 10. A cart-borne ultrasound system (10) including a movable cart having a center, ultrasound electronics located on the cart which processes ultrasound signal to form ultrasound image signals, and a display device (16) located on the cart and coupled to the ultrasound electronics for the display of ultrasound images, comprising:

- a control panel (18) which provides user controls for the control of operation of the ultrasound system; and
- 20 - an articulating linkage (30) coupled to the control panel (18) for enabling the control panel (18) to move vertically independently of the display device (16) while maintaining the inclination of the control panel (18).


1/9

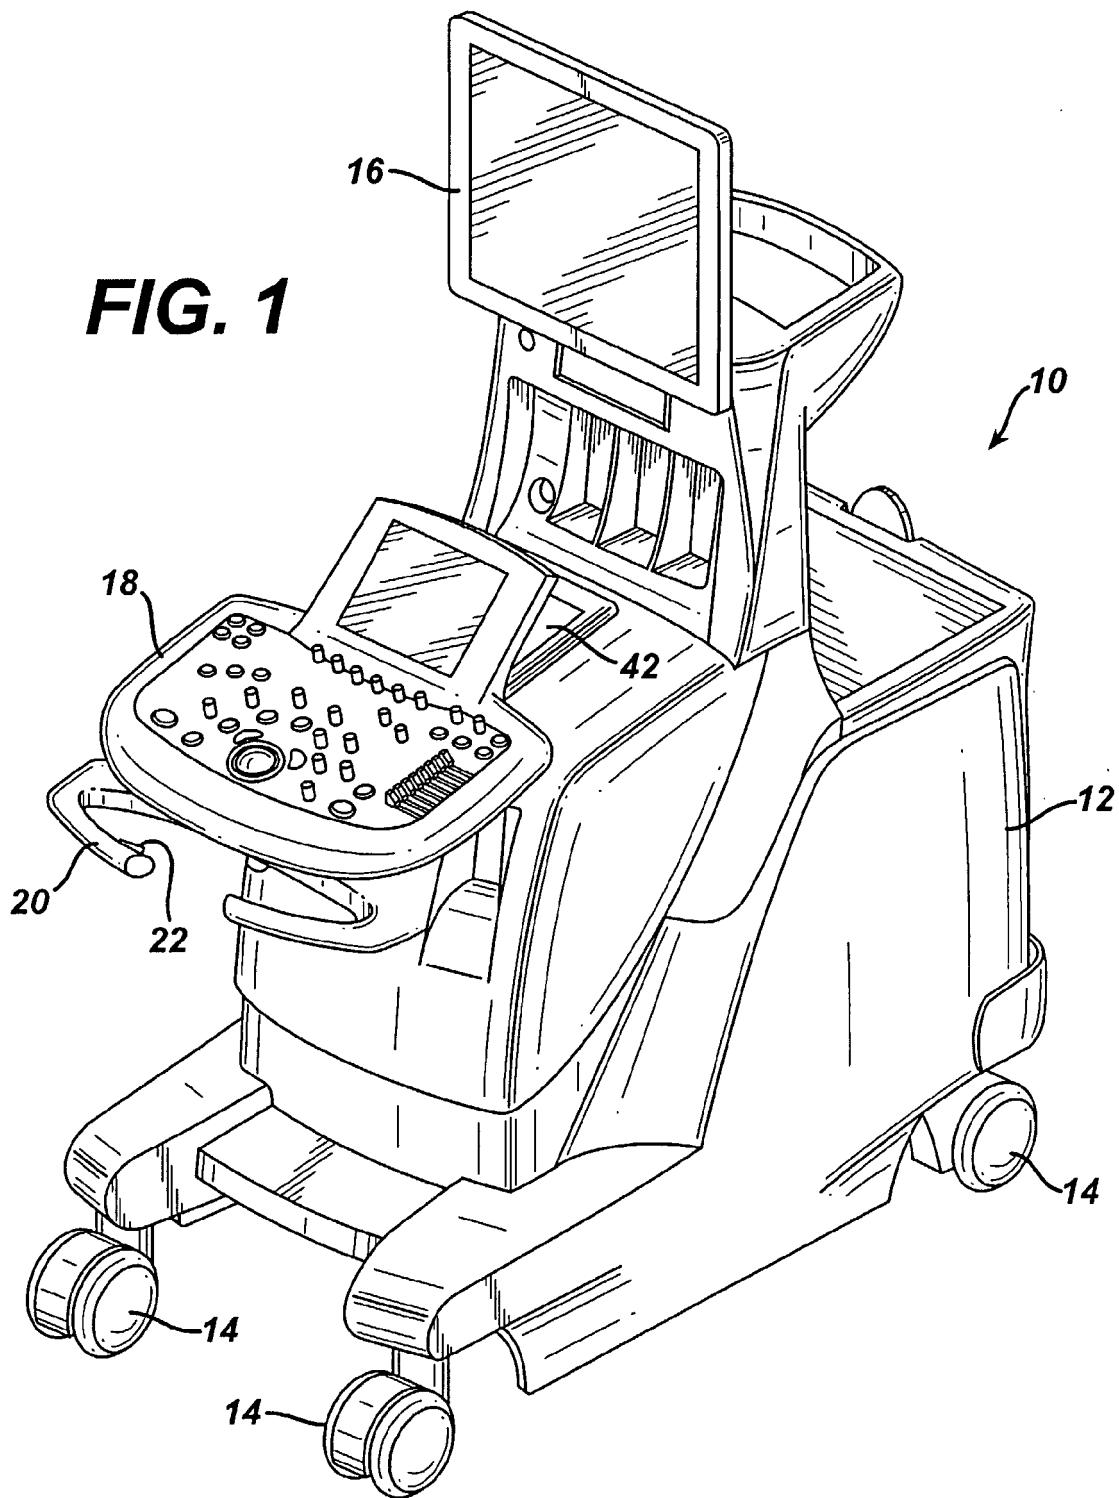FIG. 1

2/9

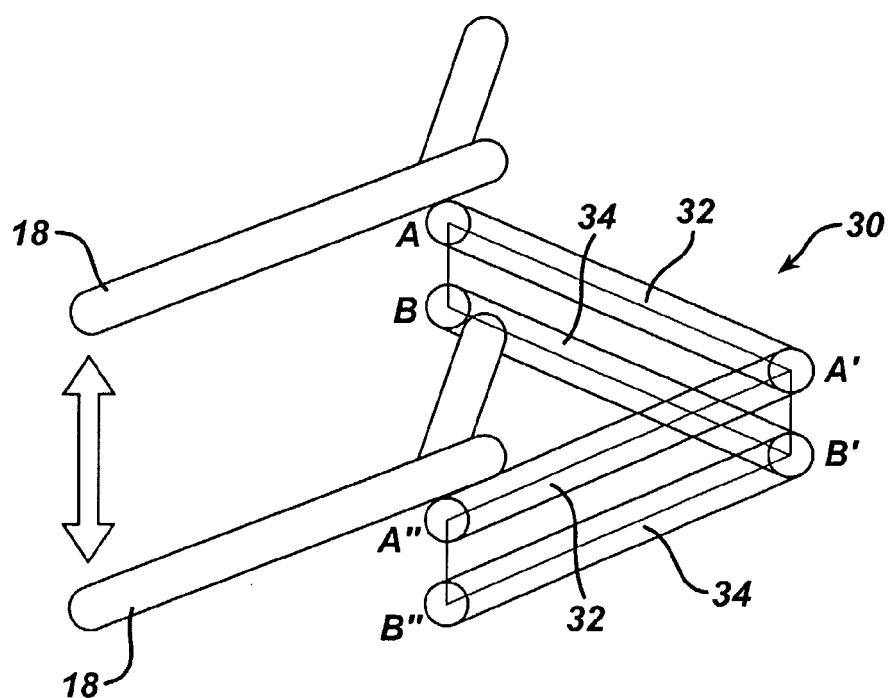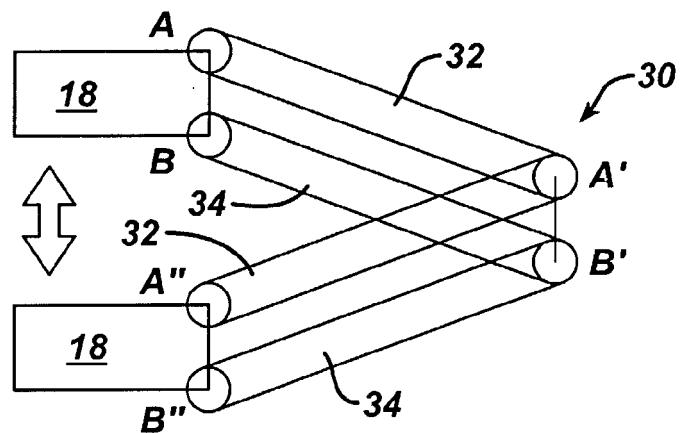FIG. 2**FIG. 3**

3/9

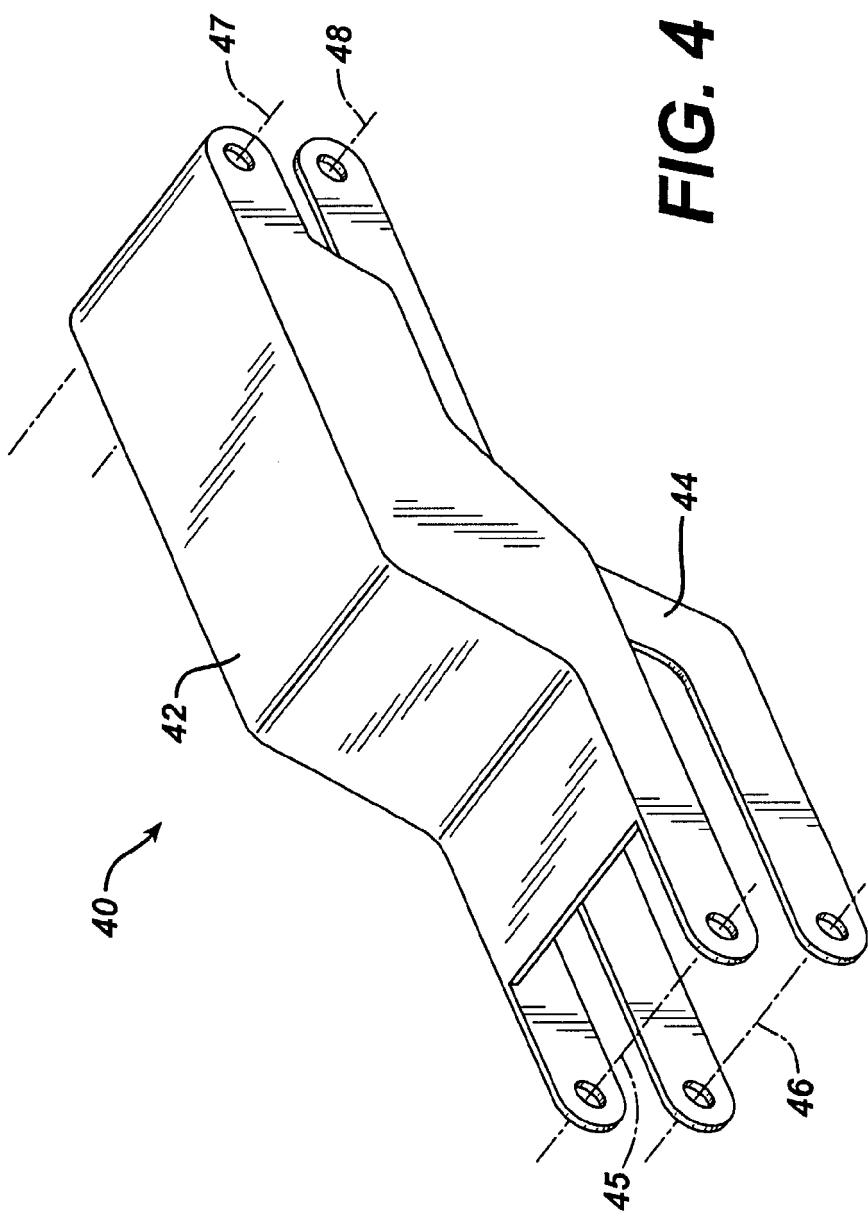FIG. 4

4/9

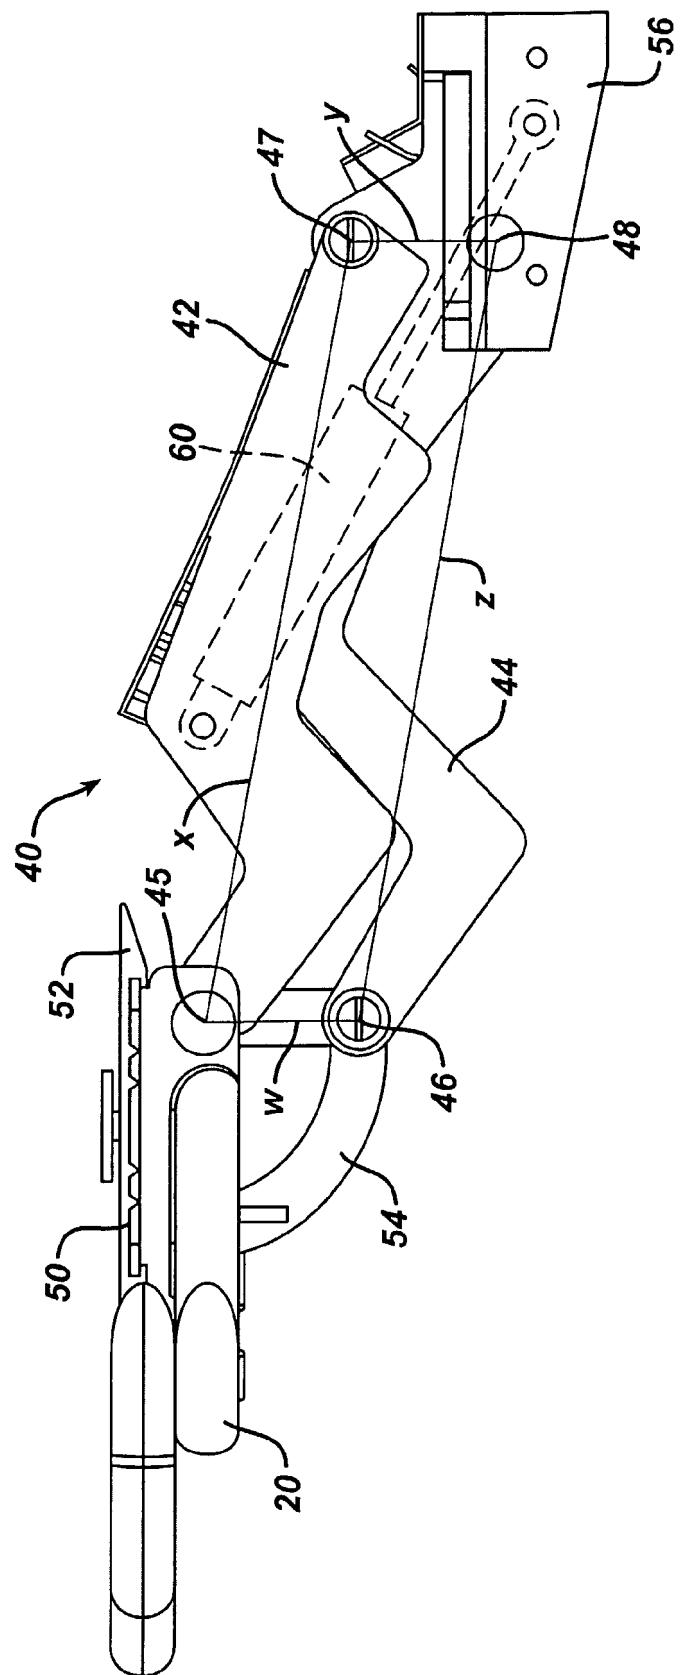


FIG. 5a

5/9

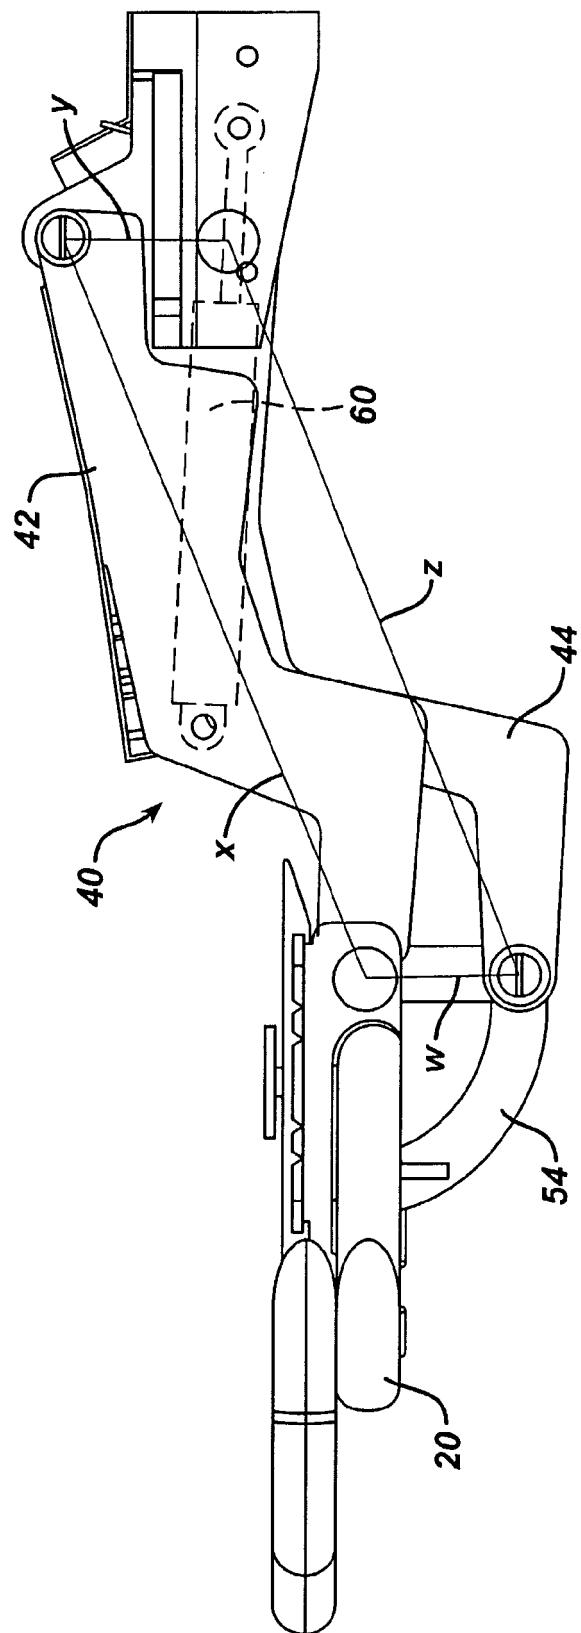
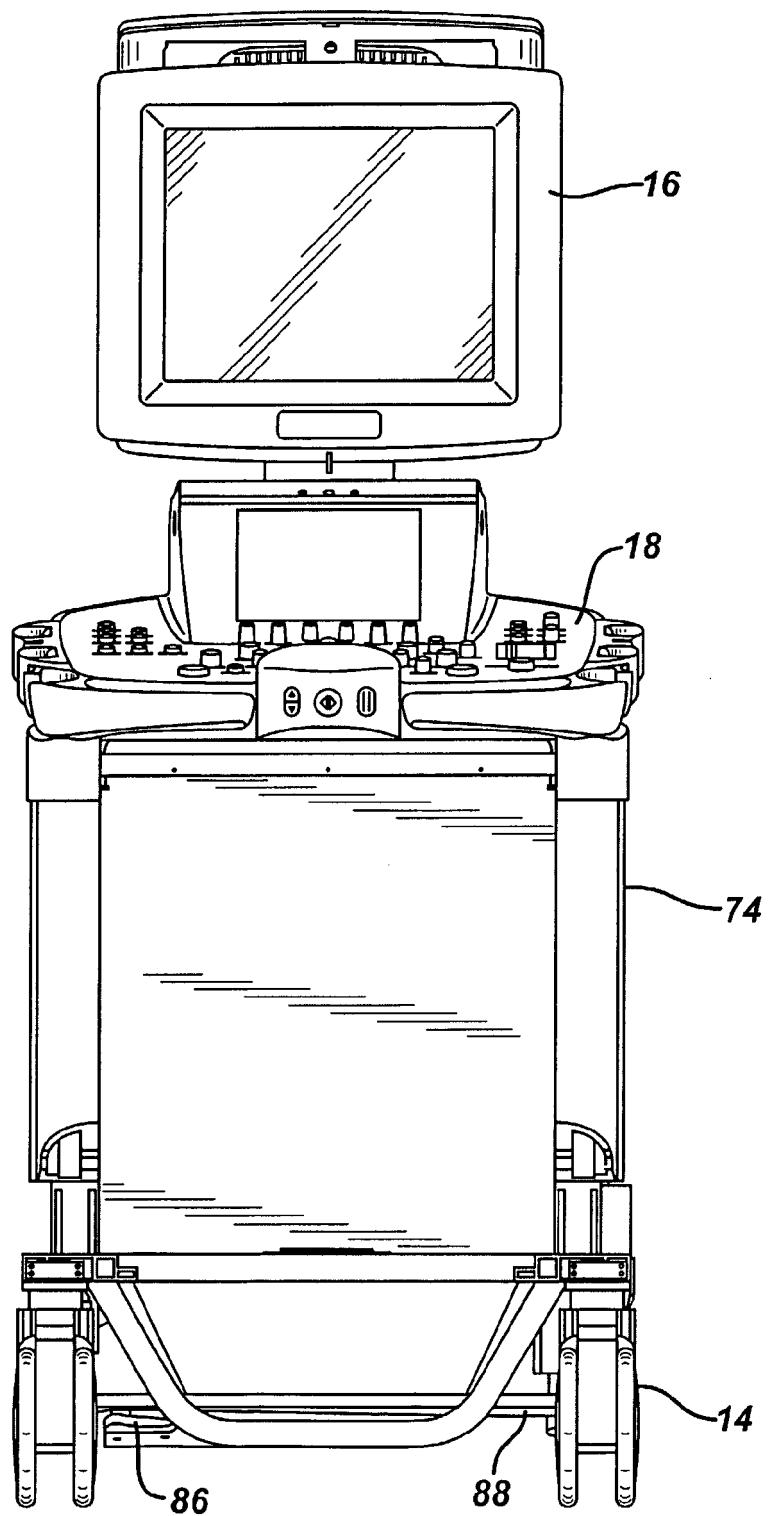
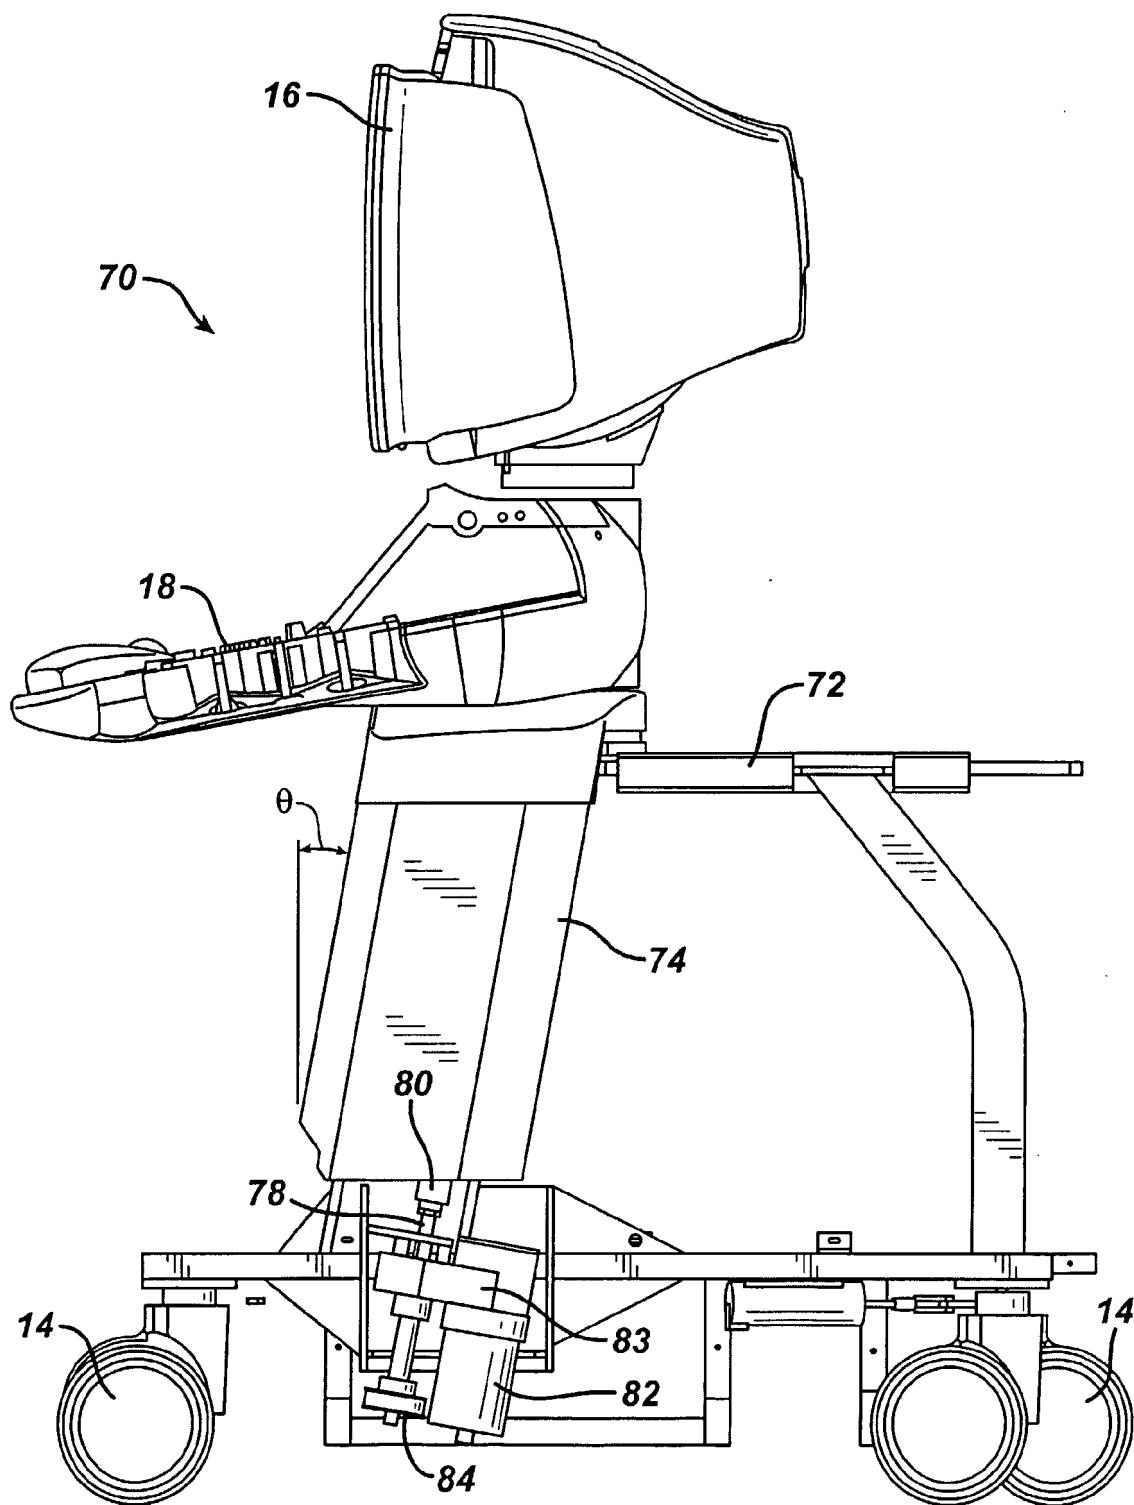


FIG. 5b

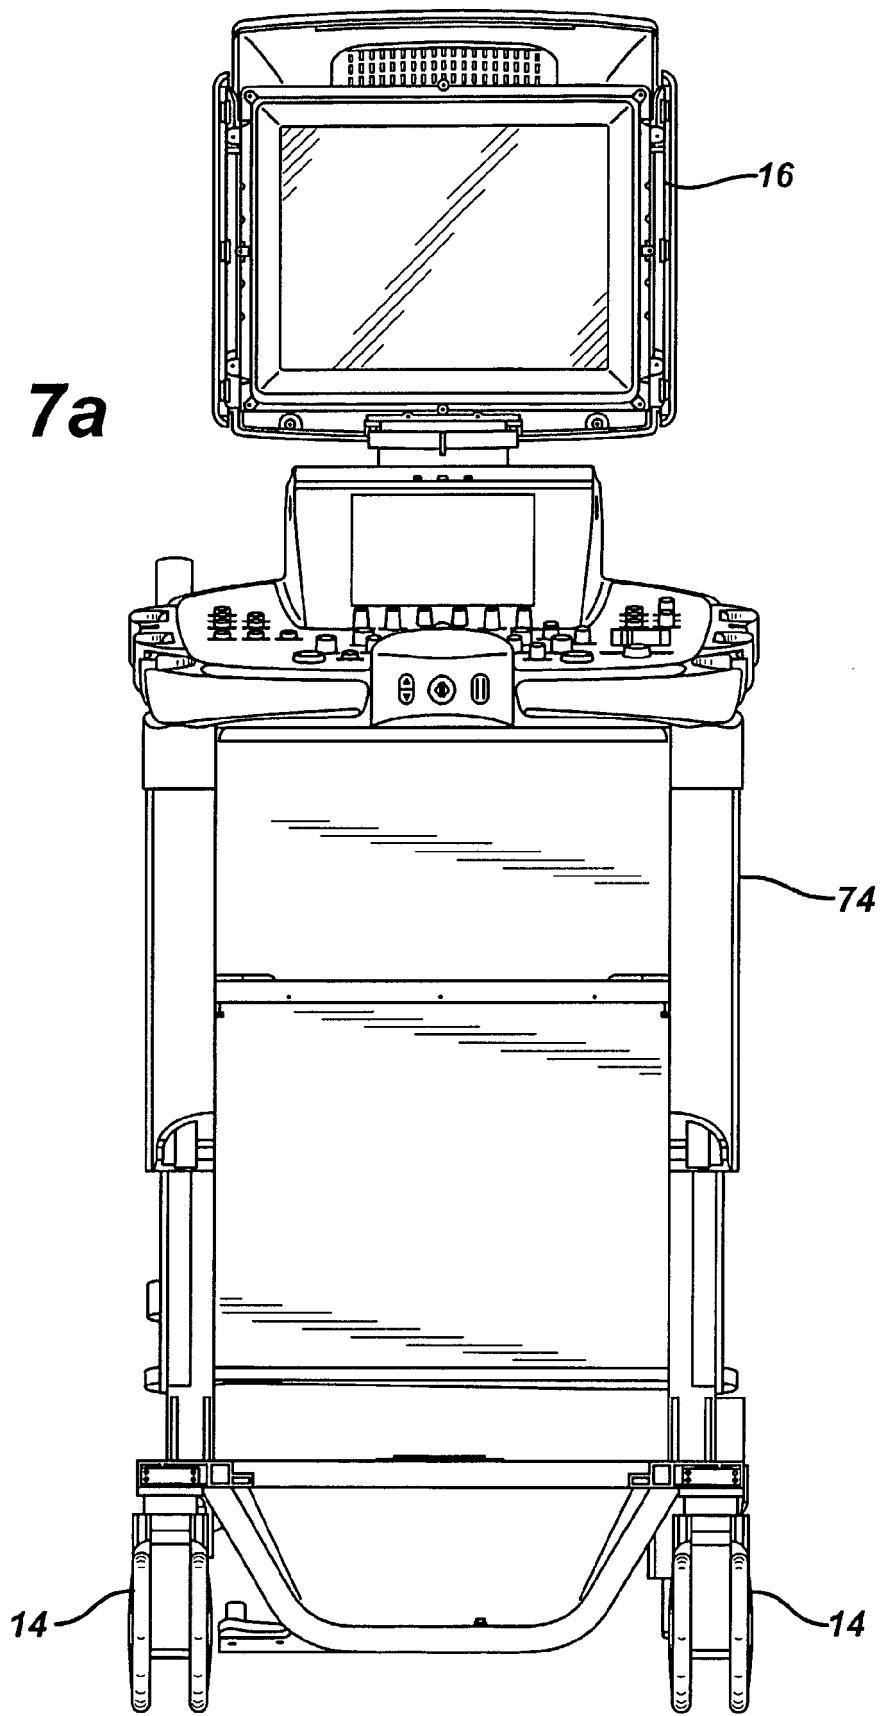
6/9

FIG. 6a


7/9

FIG. 6b

8/9

FIG. 7a

9/9

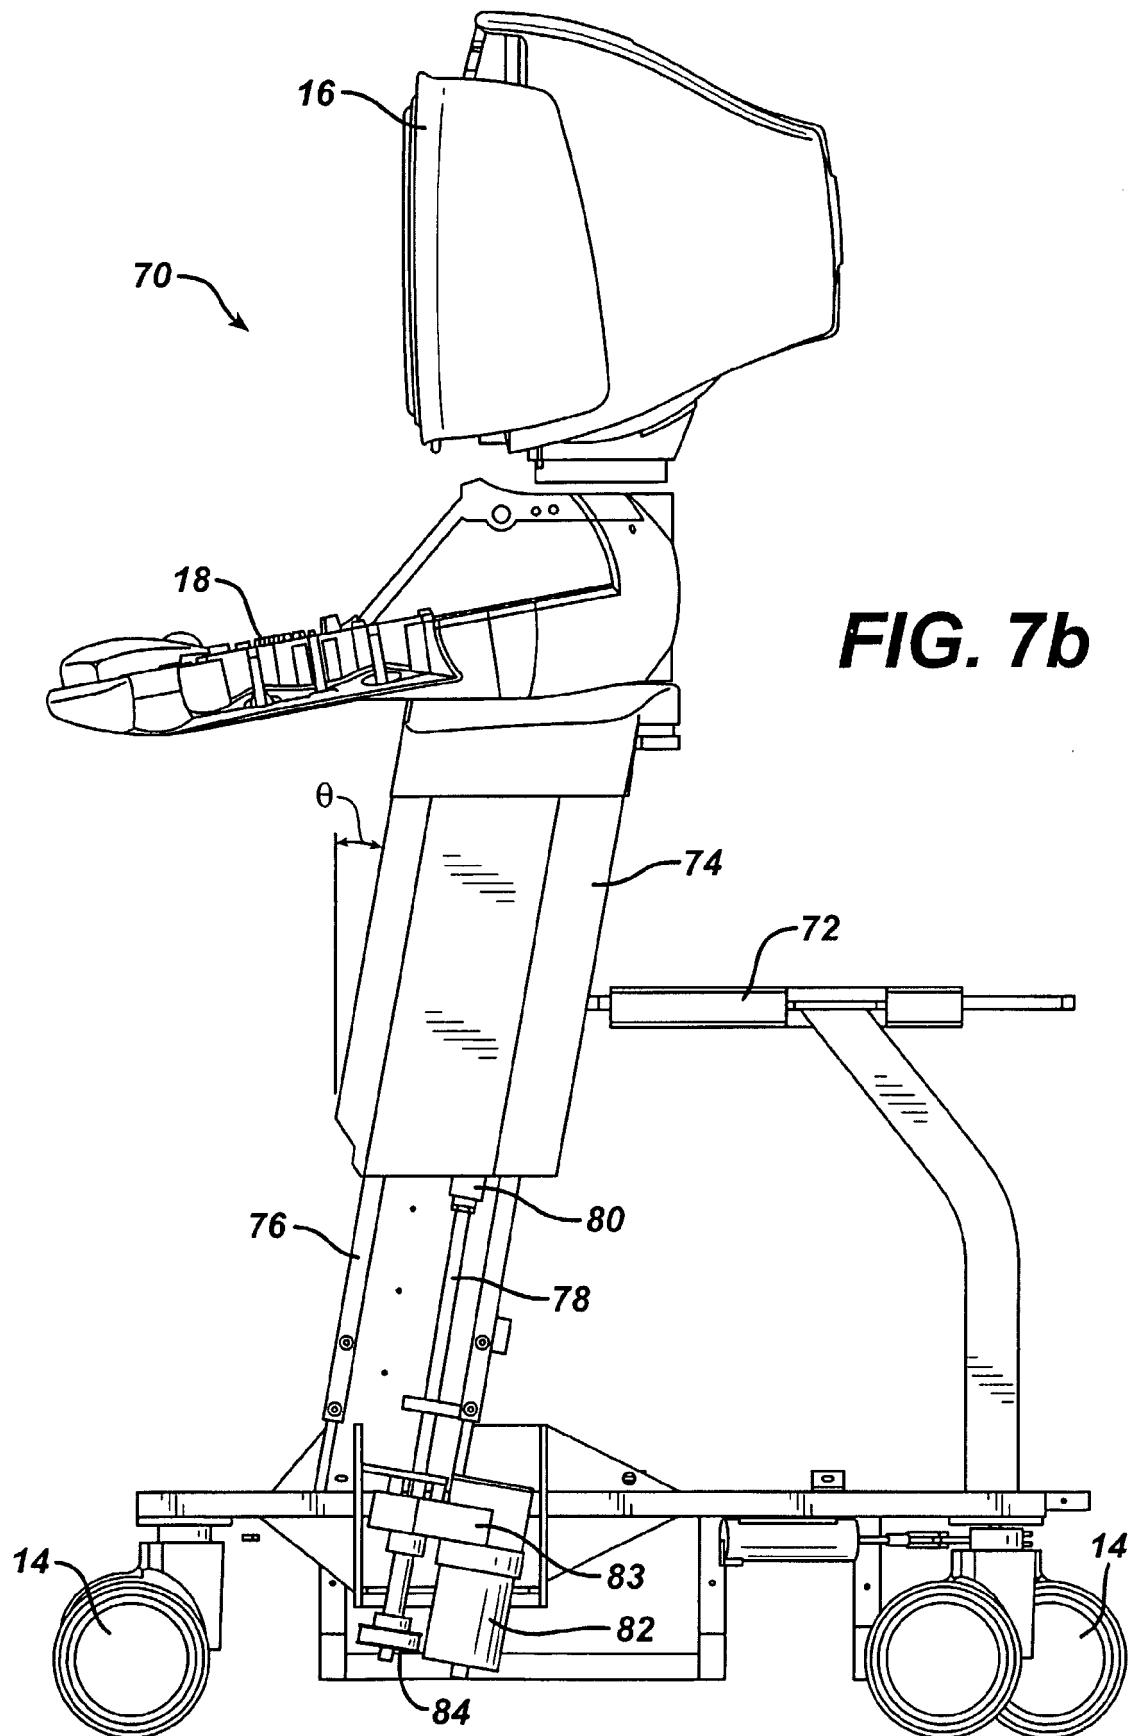

INTERNATIONAL SEARCH REPORT

Inte...onal Application No

PCT/IB 03/02290

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B8/00 A47B21/03 G01S15/89 G06F3/02

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B A47B G01S G06F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6 098 935 A (KAPLAN JONATHAN IRA ET AL) 8 August 2000 (2000-08-08) abstract; figure 5 ---	1,10
A	GB 2 176 996 A (RISOM & MARBLE FURNITURE LIMIT) 14 January 1987 (1987-01-14) abstract ---	1
A	US 6 135 405 A (JONES DAVID K ET AL) 24 October 2000 (2000-10-24) abstract ---	1
A	US 6 257 531 B1 (PENNER PHILLIP R) 10 July 2001 (2001-07-10) abstract ---	1 -/-

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *&* document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
19 September 2003	25/09/2003
Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Authorized officer Papone, F

INTERNATIONAL SEARCH REPORT

International Application No

PCT/IB 03/02290

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 02 24028 A (3M INNOVATIVE PROPERTIES CO) 28 March 2002 (2002-03-28) abstract -----	1

INTERNATIONAL SEARCH REPORT

Inte
ional Application No

PCT/IB 03/02290

Patent document cited in search report		Publication date		Patent family member(s)	Publication date
US 6098935	A	08-08-2000	US	5975474 A	02-11-1999
			US	5836560 A	17-11-1998
			DE	69627965 D1	12-06-2003
			EP	0775456 A2	28-05-1997
			US	6135405 A	24-10-2000
			US	6343775 B1	05-02-2002
GB 2176996	A	14-01-1987	NONE		
US 6135405	A	24-10-2000	US	5836560 A	17-11-1998
			US	6343775 B1	05-02-2002
			DE	69627965 D1	12-06-2003
			EP	0775456 A2	28-05-1997
			US	5975474 A	02-11-1999
			US	6098935 A	08-08-2000
US 6257531	B1	10-07-2001	WO	02100768 A1	19-12-2002
WO 0224028	A	28-03-2002	AU	3461801 A	02-04-2002
			EP	1318736 A1	18-06-2003
			WO	0224028 A1	28-03-2002

专利名称(译)	检查超声波系统推车带可变高度控制面板		
公开(公告)号	EP1509138A1	公开(公告)日	2005-03-02
申请号	EP2003727829	申请日	2003-05-21
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦电子N.V.		
[标]发明人	WILKINS JAY MESAROS ROBERT MATSUI YAS LORD RANDALL D MURKOWSKI JOHN R HOLLMAN WILLIAM RANKERS ULRICH		
发明人	WILKINS, JAY MESAROS, ROBERT MATSUI, YAS LORD, RANDALL, D. MURKOWSKI, JOHN, R. HOLLMAN, WILLIAM RANKERS, ULRICH		
IPC分类号	A61B8/00 G01S7/521 G01S15/89 A47B21/03 G06F3/02		
CPC分类号	A61B8/4405 A61B8/00 F16M11/046 F16M11/048 F16M11/18 F16M11/2092 F16M11/24 F16M11/42 F16M2200/021 F16M2200/044 F16M2200/063 G01S7/52079 G01S15/899		
优先权	10/154733 2002-05-23 US		
其他公开文献	EP1509138B1		
外部链接	Espacenet		

摘要(译)

描述了一种车载超声系统，其包括保持超声系统的电子电路的便携式推车，用于控制超声系统的控制面板和显示器。控制面板由铰接机构支撑，该铰接机构使得控制面板能够升高和降低以适应不同高度的操作者，并且使控制面板能够朝向和远离用户移动以适应坐着或站立位置的用户。在一个优选实施例中，铰接机构包括平行四边形形状的连杆，当控制板升高和降低时，该连杆也保持控制板的恒定倾斜角度。