

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
2 October 2008 (02.10.2008)

PCT

(10) International Publication Number
WO 2008/118917 A2

- (51) **International Patent Classification:**
A61N 7/00 (2006.01)
- (21) **International Application Number:**
PCT/US2008/058156
- (22) **International Filing Date:** 25 March 2008 (25.03.2008)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
60/908,074 26 March 2007 (26.03.2007) US
60/976,867 2 October 2007 (02.10.2007) US
- (71) **Applicant (for all designated States except US):** LI-
POSONIX, INC. [US/US]; 11818 North Creek Parkway
North, Bothell, Washington 98011 (US).
- (72) **Inventor; and**
- (75) **Inventor/Applicant (for US only):** CRUNKILTON, Jef-
frey, Robert [US/US]; 2331 Oakes Avenue, Everett, Wash-
ington 98201 (US).
- (74) **Agents:** HESLIN, James, M. et al.; Townsend And
Townsend And Crew Llp, Two Embarcadero Center, 8th
Floor, San Francisco, California 94111-3834 (US).
- (81) **Designated States (unless otherwise indicated, for every
kind of national protection available):** AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA,
CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE,
EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID,
IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC,
LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN,
MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH,
PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV,
SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN,
ZA, ZM, ZW.
- (84) **Designated States (unless otherwise indicated, for every
kind of regional protection available):** ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL,
NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG,
CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
— without international search report and to be republished
upon receipt of that report

(54) **Title:** INTERCHANGEABLE HIGH INTENSITY FOCUSED ULTRASOUND TRANSDUCER

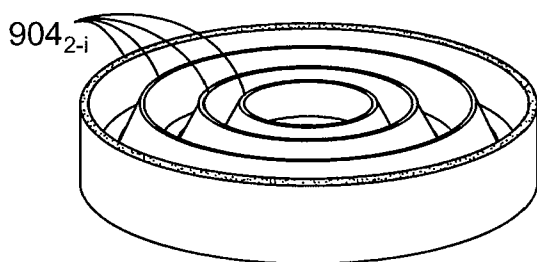


FIG. 9D

(57) **Abstract:** An interchangeable transducer for use with an ultrasound medical system having a keyless adaptor and capable of operating in a wet environment. The interchangeable transducer has an adaptor for engaging a medical system, an ultrasound transducer and additional electronics to provide a self-contained insert for easy replacement and usage in a variety of medical applications. A slip ring spacer is also disclosed, the slip ring spacer for use with a pancake slip ring having a base and flange configuration to form one or more channels around each contact ring of the pancake slip ring. The channels provide fluid isolation around each connector to help reduce electronic cross talk and contact corrosion between the connector pads of the slip ring while the slip ring is immersed in a wet environment.

WO 2008/118917 A2

INTERCHANGEABLE HIGH INTENSITY FOCUSED ULTRASOUND TRANSDUCER

BACKGROUND OF THE INVENTION

5 [0001] The present invention relates to a sealing adaptor for use with a interchangeable transducer for use within a wet environment transducer housing.

[0002] Some high intensity focused ultrasound (HIFU) transducers have limited life span because of the high power levels that may tax their physical construction. These transducers degrade and fail for a variety of reasons much faster than transducers used in other medical fields (like diagnostic ultrasound, or other low power applications). Transducers designed for
10 therapeutic ultrasound applications delivering therapeutic power levels may suffer delamination of their metallization layers, pitting or physical destruction of the transducer caused by cavitation or thermal effects from exposure to very high temperatures.

[0003] To combat some of these side effects of HIFU operation, system designs may use HIFU transducers below the threshold where damage may occur to the transducer itself.
15 Other systems use water baths with degassed circulating water, or design their therapy regimens with long intervals between therapy pulses. These extended pauses between pulses produce a low pulse repetition frequency (PRF) allowing the transducer to cool, and negative effects in tissue to dissipate.

[0004] Unfortunately, some therapy regimen require HIFU with a higher PRF, or
20 continuous operation of the transducer for certain lengths of time that preclude low PRF operation. These higher PRF and/or continuous wave (CW) style regimen are desirable when the treatment is designed to maximize the amount of tissue destruction to be achieved in a certain period of time. In these types of operations, transducer degradation necessitates a frequent replacement of the HIFU transducer. Replacement is made difficult in that the
25 transducers are generally expensive and delicate components, so handling the transducers is usually kept to a minimum. Further more, transducers in therapeutic medical systems are often imbedded into large bulk chambers filled with water, or attached in a manner that precludes easy removal and replacement of the transducer. The transducer environment may contain water, which should not be permitted to mix with the system electronics. The
30 presence of water during a transducer exchange can make the replacing of a transducer messy

and difficult. Once the transducer is replaced, water may linger between the electrical connectors between the system and the new transducer. System performance may be degraded due to electrode corrosion or signal cross-talk among the conduction paths caused by the presence of water or other fluids.

5 [0005] Thus it would be desirable to provide a transducer connector, or connecting means, that provides an easier method of removing and connecting transducers to a medical ultrasound device that is compatible with the demands of a wet environment, and capable of handling all system requirements without degradation in performance.

[0006] Thus it is an objective of the present invention to provide a connectorized transducer
10 that can be connected to a therapy head or medical system with as few steps as practical, while preserving the environmental conditions of the connection.

[0007] Another objective is a connection that has a high reliability and ease of use, to promote a user friendly procedure for removing and/or installing transducers in the medical system.

15 [0008] Yet another objective is to provide a transducer that provides various features and operation parameters to expand or broaden the type of transducers a user may connect with the medical system.

[0009] Still another objective is a transducer that possesses the necessary driving electronics particular to their designed features, so as to reduce the required programming and
20 electronics of the main system.

[0010] Still another objective is to provide a simple disposal path for used components.

[0011] Still another objective is a sealing device for electrical signal isolation or electrical connector isolation in a wet environment.

BRIEF SUMMARY OF THE INVENTION

25 [0012] These and other objectives are achieved through an interchangeable transducer adapted for use with a high intensity focused ultrasound (HIFU) medical system. The interchangeable transducer has a housing that is generally rigid and hollow. The housing has two open ends, one adapted for fitting a HIFU transducer, and the other end having an isolation layer and electrical connection for electrical signal and power communication with
30 the HIFU medical system. The interchangeable transducer is adapted to fit into a socket style

receptacle on the medical system. The transducer is ideally replaced by the user, so the portion of the transducer which fits into the socket is designed for easy insertion and extraction. Easy insertion is achieved through an orientation free, low engagement force connection between the transducer and the medical system which allows easy user access to the transducer.

[0013] A slip ring spacer is also described herein for use with a wet electrical connection having a pancake style slip ring. The slip ring spacer has a base formed from a non-conductive material. Multiple apertures extend through the base. The apertures are designed to sheath electrical connectors which extend through the base. There are one or more flanges extending from the base. The flanges are arranged so as to isolate the apertures into cells.

[0014] Additional embodiments and methods of making and using the interchangeable transducer are also herein described.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] Fig. 1 shows an exterior view of an interchangeable transducer.

[0016] Fig. 2 is a cut away view of an interchangeable transducer.

[0017] Fig. 3 shows a system for use with an interchangeable transducer.

[0018] Figs. 4A-4E illustrate a method of swapping a transducer.

[0019] Fig. 5A shows an exploded view of one embodiment of the interchangeable transducer.

[0020] Fig. 5B provides an alternative embodiment of a PCB for use inside the insert.

[0021] Figs. 6A-6C show the interchangeable transducer connection to the system socket.

[0022] Figs. 6D-6E show the transducer insert using an alternative PCB.

[0023] Figs. 6F-6I illustrate a progression of possible adaptor shapes.

[0024] Figs. 7 and 8 show alternative PCB positions for the interchangeable transducer.

[0025] Figs. 9A-9E show a slip ring seal and a slip ring.

[0026] Figs. 10-15C show alternative embodiments of the slip ring seal.

DETAILED DESCRIPTION OF THE INVENTION

[0027] Described herein are various forms of replaceable transducers for use with high intensity focused ultrasound (HIFU) medical systems. The basic design of the interchangeable transducer incorporates a housing which is hollow and generally rigid. The housing holds within it a transducer, such as one compatible with HIFU medical systems, electrical pathways (electronics) for connecting the transducer to a medical system so the transducer can be properly controlled, and a connector that allows the interchangeable transducer to be removed and/or inserted into a receptacle on the medical system. The transducer housing has a shape and electrical connection assembly that allows the housing to be inserted in any radial orientation relative to the system receptacle axis. The axial symmetry may allow for two or more orientations, and desirably an unlimited number of orientations. For visualization purposes only, one may imagine the ease of inserting a mini-plug for headphones into a portable music player. The radial orientation of the plug to the receptacle does not matter, and during use if the plug is rotated within the socket, there is no interruption of the power and signal sent to the head phones. This concept is analogous to the type of adaptor and socket used in the interchangeable transducer connection described herein.

[0028] In the following paragraphs, various aspects and embodiments of the apparatus will be described. Specific details will be set forth in order to provide a thorough understanding of the described embodiments of the present invention. However, it will be apparent to those skilled in the art that the described embodiments may be practiced with only some or all of the described aspects, and with or without some of the specific details. In some instances, descriptions of well-known features may be omitted or simplified so as not to obscure the various aspects and embodiments of the present invention.

[0029] Parts of the description will be presented using terminology commonly employed by those skilled in the art to convey the substance of their work to others skilled in the art, including terms of operations performed by or components routinely used in ultrasound systems, medical ultrasound systems and HIFU systems. As well understood by those skilled in the art, the operations typically involve producing and controlling the wave form of the transducer through a transmitter signal which generally uses well understood electronics components and controllers. Signal control, depends primarily on the desired objective for using HIFU. Novel variations from prior art devices will be presented here in a straight forward and simple manner so as to highlight the elements necessary to practice the present

invention, but not to be prolix in description for those details which are well understood in the art. The term system includes general purpose as well as special purpose arrangements of these components that are stand alone, adjunct or embedded.

5 [0030] Various operations may be described as multiple discrete steps performed in turn in a manner that is most helpful in understanding the present invention. However, the order of description should not be construed as to imply that these operations are necessarily performed in the order they are presented, or even order dependent.

10 [0031] Reference throughout this specification to “one embodiment” or “an embodiment” means that a particular feature, structure, or characteristic described in connection with the embodiment is included in at least one embodiment of the present invention. Thus, appearances of the phrases “in one embodiment” or “in an embodiment” in various places throughout this specification are not necessarily all referring to the same embodiment.

15 [0032] The present invention relates to an interchangeable transducer apparatus and methods of making the same, for use with medical ultrasound systems, particularly those considered HIFU medical systems.

20 [0033] The transducer described herein incorporates both novel physical components and design, combined with existing materials in a novel fashion to produce a transducer insert meeting one or more of the objectives of the invention. The combinations of various novel elements in one embodiment will meet some objectives, while a different combination of novel elements will meet different objectives. The collective whole of novel developments and arrangements of existing parts contributes to a design that satisfies the most objectives, though not necessarily all objectives in a single design. Different objective requirements will call for different combinations of the inventive concepts herein described.

25 [0034] The transducer insert may be suitable for any number of medical devices or medical systems desiring to use an easily replaceable transducer. In pending United States Patent application 11/027,912 “Ultrasound Therapy Head with Movement Control,” filed 29 December 2004 (commonly assigned and herein incorporated by reference), a therapeutic ultrasound system is described having a therapy head. The therapy head contains a first chamber, being wet, in which a transducer is positioned. There is a second chamber, which
30 may be wet or dry, that contains a motor drive system. The motor drive system uses one of several possible means to move the transducer in the first chamber. Means described include use of actuators that extend from the motor side chamber to the transducer side chamber, a

slide positioned on the motor chamber with a magnetically connected transducer in the transducer chamber, or various mechanical translation components for converting the work produced from the motors into the movement of the transducer through a barrier between the two chambers.

5 [0035] The interchangeable transducer, (also referred to herein as a connectorized transducer or transducer insert), of the present design is well suited for use in a therapy head of the previous description. The interchangeable transducer or transducer insert is formed from a housing having an adaptor end and an acoustic end. There is a communication port at the adaptor end. The adaptor end is designed to fit into a corresponding receptacle on or in
10 the medical ultrasound system. In one embodiment the transducer adaptor end has a plurality of orientations for removably engaging a receptacle in the medical ultrasound system. There is a transducer at the acoustic end, and a means for electrical communication between the communication port and the transducer.

[0036] The adaptor end may be a male or female type part, while the receptacle would be
15 the logical corresponding type part. While we describe primarily a male adaptor and a female receptacle, it should be understood that the adaptor end of the transducer insert can be the female component while the system side receptacle is the male component. The adaptor end and corresponding receptacle end are designed in a manner to provide a plurality of working orientations in which the transducer insert can be placed into the system. In one embodiment
20 the plurality of orientations may simply be a slotted design for the adaptor and receptacle. The electronics of the adaptor and receptacle are arranged in a manner as to allow a “key-less” type of connection. Regardless of which orientation the insert is placed into the receptacle, the insert will connect with the system and operate properly. The connection between the adaptor and receptacle may be any design having symmetry about an axis, so the
25 insert may be rotated about the axis so the insert can be fit into the receptacle in at least two directions (normal and flipped). If the connection is shaped like a triangle, three orientations would be possible. For a square four orientations would be possible. This dynamic continues to the logical and most desirable shape of having a circular shaped adaptor where absolute radial freedom is afforded. The insert may be placed into the system receptacle at any radial
30 orientation and proper electrical connection is guaranteed. Regular shapes are not required to make the adaptor connection. Irregular shapes may also be used so long as they are symmetrical. The symmetry of the connection provides the advantage to the user of not having to worry about the orientation of the transducer insert relative to the system socket

(receptacle). So long as the shape of the connector matches the receptacle the user knows the orientation will work.

[0037] Electrical communication is required from the ultrasound medical system and the transducer within the transducer insert. Electrical communication enters the transducer insert at the communication side. Electrical communication means providing any combination of power, signal or ground connections from the transducer to the ultrasound system through the communication port in the transducer insert. This communication can be achieved using wires, cables, connector pins, or other electron conveying instruments as known in the art. In one embodiment, the connection may be wires running directly from the communication port to the transducer in a “dumb” design, where no on board intelligence is provided in the insert. In another embodiment, intelligence may be incorporated into the insert by adding electrical components to an electrical circuit used to provide electrical communication from the communication port to the transducer. A variety of components may be used in an intelligent design. Electrical components may include a tuning transformer for optimizing the transducer, sensors for measuring various parameters about the environment within the transducer insert, sensors for monitoring the transducers performance and/or safety, components for recording measured or detected data, IC chips for running programmed applications or storing information within the insert, or any other operation desired.

[0038] In another embodiment of the present invention, the electrical communication between the communication port and the transducer may be provided by a two stage spring pin connection scheme. A first stage set of connection pins connects the communication port to an electrical circuit board. The circuit board may be a PCB/PCBA and may further be a pancake slip ring style PCB/PCBA. A second stage set of connection pins connects the electrical circuit to the transducer. Electrical communication enters the communication port from the ultrasound system. The Electrical communication then travels to the electronic circuit. The circuit board may provide the proper coordination and layout of the various electrical components, and assures proper handling of Electrical communication between the system and the transducer. From the electrical circuit, Electrical communication continues to the transducer. Any return Electrical communication from the transducer may follow a similar route back from the transducer to the circuit board, and then back to the system.

[0039] The insert may have various data recorders, sensors or programmable components within it. These elements may be on the circuit board. Various possible components that may

be incorporated into the insert include a chip for tracking the number of times the transducer has been used, sensors which determine the proper coupling between the transducer and the patient, sensors to determine if the transducer is properly installed into the ultrasound system, or sensors to determine the safe operation of the transducer while providing therapy output.

5 There may also be a tuner for a second transducer such as an “A” line transducer for providing simple imaging information to the user or to the system.

[0040] The transducer insert may also be constructed to operate with a component style ultrasound system such as those described in US Patent Application 11/027,919 entitled “COMPONENT ULTRASOUND SYSTEM” and filed on December 29, 2004 (commonly
10 assigned and herein incorporated by reference). In this embodiment, the insert has an adaptor for fitting to an ultrasound system having two or more identical sockets for receiving more than one type of insert, where one of the inserts may be a transducer insert as described herein. In a component ultrasound transducer, there are two or more sockets in the therapy head. The sockets are identical and the inserts used within the sockets may be plugged into
15 any one of the sockets, Each insert has a challenge and recognition component programmed in it, so when the insert is plugged in, the ultrasound medical system can identify each individual insert and know how to properly use it. The system can handle multiple kinds of inserts simultaneously. Each insert may have a different focal depth, performance parameter or use requirement, the system can determine and properly handle the proper operation of all
20 inserts. Desirably the transducer inserts would be properly utilized by the system automatically (without specialized user contribution or instruction to the system other than that used for a single receptacle ultrasound system using a transducer insert).

[0041] Use of modern materials and electronics greatly reduces the costs of manufacturing transducers for the medical ultrasound systems disclosed herein. This cost reduction and ease
25 of manufacturing allows replacement parts to be disposable when worn out or no longer desired.

[0042] In addition to the transducer insert described herein, a novel structure is now disclosed allowing an electrical connection to be made in a wet environment. The novel structure is a slip ring seal, designed for use with a pancake style slip ring PCB. The slip ring
30 seal has a base, two or more apertures extending through the base, and flanges extending from the base to isolated the apertures into cells. The flanges may define cells discretely

formed around each aperture, or around a select group of apertures, or a combination of the two.

[0043] The connection between the transducer insert and the system is generally a wet environment. Particularly during operation of the transducer the chamber in which the transducer is located is fluid filled. Various fluids are suitable for use in the transducer chamber where the transducer of the present description can be used, in general water is the most common fluid used due to ease of availability, cost and performance characteristics. Reference herein to fluids or water should be understood to incorporate which ever fluid is most suitable for the intended use and design of the transducer, since not all operations will prefer water when another compatible fluid may be superior for the particular application.

[0044] Now turning to the accompanying drawings, it should be understood the drawing figures are provided to enhance the description provided. Elements shown in the figures are not necessarily illustrated to scale with respect to other drawings, or other parts within the same drawing. The parts or figures should not be taken in any absolute sense of actual design elements other than as illustrations of embodiments for the purpose of understanding the disclosure herein.

[0045] A simplified exterior view of the interchangeable transducer 10 is shown in Fig. 1. The transducer 10 has a housing 16 represented as generally cylindrical. The housing 16 is desirably rigid and hollow. The housing 16 has a transducer end 20, and an electrical connector and sealed end 14. External electrical connectors 40 extend through the seal end 14 and are designed to connect to the appropriate electrical lines from the medical system. These may include a transmit/receiver line, ground and power. Additional lines may be provided depending on the need or application of the medical system. The interchangeable transducer need only have addition electrical connectors and support circuitry to enable those capabilities. An adaptor 32 is also provided to allow physical engagement of the transducer 10 to a HIFU medical system.

[0046] A simplified interior view of the interchangeable transducer 10 is now illustrated (Fig. 2). Once again the seal end 14 has external electrical connectors 40 for electrical connection to a medical system. The external electrical connectors 40 may extend through the seal end 14 to connect to a component within the housing 16, or there may be an intermediate connection through the seal end from the interior of the housing. Desirably the external connectors extend through the seal end to provide electrical contact between the socket of the

medical system, and the interior of the interchangeable transducer. The transducer 22 is shown at the bottom or lower section of the housing 16. The transducer 22 is electrically connected to the connectors 40 by wires 12. Electrical signals from the ultrasound system to the transducer 22 (or visa-versa) may include power, ground, transmit, receive, data or other signals and information as desired. The housing may also contain one or more electrical components as part of the transducer's control circuit.

[0047] The interchangeable transducer 10 has a connector or other adapter allowing it to engage into a receptor on a medical device system (Fig. 3). A medical system 300 that might use an interchangeable transducer as described herein, is shown having base 302, an articulating arm 304, with a display screen 306 and a therapy head 308. Within the therapy head 308, there is an adaptor for receiving an interchangeable transducer. A computer or other electronic intelligence (CPU) is also provided to operate the system 300 and the transducer 10.

[0048] The internal components of the therapy head 308 are generally described along with the method of changing out transducers (Figs. 4A-4E).

[0049] Any water or other fluids in the therapy head 308 are desirably drained from the therapy head so that water does not splash out of the therapy head when opened. Having water or other fluids in the therapy head is not an impediment to the removal and installation of transducers described herein, so it is not necessary to completely drain the therapy head. In one embodiment the therapy head 308 is inverted, so the main transducer chamber 310 is positioned on the bottom. The therapy head 308 has a removable cap 312 section, with a transmission window 316 (Fig. 4A).

[0050] The cap 312 is removed (Fig. 4B) exposing the interior of the therapy head transducer chamber 310. The interchangeable transducer 10 is connected to a receptor socket 38. A pair of water lines 320 are used to circulate water inside the transducer chamber when the cap 312 is sealed to the transducer housing 310. There are mating flanges 322 on the treatment cap 312 and bulkhead 324 that contain an O ring seal on the transducer housing 310 that when assembled create the water tight seal of the chamber (not shown). Under the receptor 38, the transducer chamber may have motors or motor cams 326 or drive shafts connected to a mechanical drive system for moving the receptor 38.

[0051] Once the cap 312 is removed, the interchangeable transducer 10 can be removed (Fig. 4C). Desirably the transducer can be lifted straight out of the receptor 38, or detached

from the receptor with a minimal amount of force (like twisting or rocking). The empty receptor 38 has a PCB slip ring which may get wet during this step, and the presence of water on the PCB is of no concern.

[0052] A new transducer 10' is now seated onto the receptor 38 in place of the old transducer 10 (Fig. 4D). Again the insertion force for placing the new transducer 10' is desirably fairly low, allowing any user to insert the new transducer 10' easily and quickly. The round shape of the transducer plug and the receptor 38 allow for any radial orientation when the new transducer 10' is seated into the receptor 38. The cap 312 is then repositioned over the transducer chamber 310 to re-form the therapy head 308 (Fig. 4E).

[0053] Once the new transducer is in place, it may be desirable to refill the water chamber, activate the medical system 300, and allow the system to communicate with the new transducer 10' to ensure the transducer is properly seated in the receptor 38, and that the transducer is responding normally. The system may use a 'challenge and answer' protocol to determine the nature of the transducer, and establish the appropriate therapy regimen to use with the particular transducer. The transducer 10 may have an integrated circuit (IC) 30 on board that can provide detailed information to the medical system once it is properly connected. Alternatively the IC may be used for other purposes (see below).

[0054] A connector or adaptor 32 is shown on the outside of the housing 16 (Fig. 1). The connector 32 allows the transducer housing 16 to mate with a socket or receptacle 38 of a medical system 300. The connector 32 desirably allows the housing 16 to be inserted into the socket or receptacle with a low insertion force to provide easy insertion or removal. The electrical connectors 40 are designed to operate in conjunction with the mechanism used to mate the transducer 10 to the receptor 38, so the electrical connectors 40 can establish and maintain contact with the appropriate system side electronic channels regardless of the radial orientation of the transducer when mated to the receptor. The connector 32 similarly can engage the socket 38 in any radial orientation. The receptor or socket 38 has a receiving element 36 for the connector 32. The connector 32 for engaging the socket may be mechanical, magnetic or electromagnetic in nature. As long as the connector can hold the transducer housing in its proper place in the socket and allow for any radial orientation for insertion and removal, the connector will be sufficient for the intended use.

[0055] The interchangeable transducer assembly is now described (Fig. 5A). In this embodiment, the housing 16 is made from two sections, a lower portion 16B for receiving the

transducer 22, and an upper portion 16A adapted for connection with the medical system socket 38. The transducer 22 is shown having a set of pin receptors 24r where the electrical pins 24 attach to the transducer. The electrical pins 24 extend from the interface 28 to the transducer and pass through the concentric liner 26. Desirably the liner has apertures for lining up the connection points on the interface and the transducer. An optional transformer 42 can be connected to the interface 28, and would sit within the aperture defined by the concentric liner 26.

[0056] The lower portion 16B may be assembled by first inserting the transducer 22 into the lower portion 16B. The transducer 22 may be secured using epoxy or resin along the transducer rim to seal the transducer to the aperture defined by the housing opening 20. The electrical connector pins 24 are inserted into the concentric liner 26, and then the connector pins 24 are oriented to match the transducer receiver placements 24r. The concentric liner 26 is then placed into the lower portion and secured. Electrical components such as the transformer 42, or the data IC (not shown) may be attached to the PCB 28, and then the PCB 28 is lined up to match the desired connector pin 24 layout. The PCB 28 has predefined lands on both its upper and lower surface. These lands correspond to the pin orientation for the electrical connector pins 24 of the lower portion, and for the electrical pins of the upper portion 40.

[0057] The upper portion 16A is similarly assembled. The upper portion is sealed across the top, and the electrical pins 40 that extend through the top of the upper portion 16A are sealed against fluid flow from the outside of the housing to the inside. The electrical pins 40 may be soldered in place, or fixed with an epoxy or other agent to provide the fluid seal between the upper portion 16A and the apertures needed for the pins. The upper connector pins 40 are inserted through the isolation layer 34 in a predefined arrangement matching the upper lands of the PCB 28. The connector pins may be any type of electrical pins suitable for use in an interchangeable design. Spring pins, pogo-pins, spring clips and other tensioned electrical connectors are desirable in one embodiment due to their expansive nature. Spring loaded connectors allow a greater margin of safety in physical distance between the transducer and PCB. Once the connection pins 40 are in place, the isolation layer 34 is lowered into the upper housing 16A. The isolation layer 34 is desirably attached to the upper portion so that the upper housing 16A and isolation layer 34 can be moved as a single unit. The isolation layer 34 may be attached using an adhesive compound between the isolation layer and the top of the upper housing. Alternatively the isolation layer 34 may be

constructed so there is an interference fit between the isolation layer and the upper section of the housing. Desirably the adhesive or interference fit would prevent water from pooling underneath the isolation layer and the housing. The upper housing is then lowered onto the lower housing assembly so the connector pins 40 match the PCB land layout (Fig. 5A). The entire transducer housing may be filled with an inert gas to promote stability and operational life span of the internal components.

[0058] In an alternative embodiment, the transducer insert 10 replaces the standard PCB 28 with a slip ring PCB 29 (Fig. 5B). In this embodiment there are discrete lands LD or traces for direct attachment to particular components (transformer, IC chips, etc...) as well as traces made into slip rings 102a-i for connection to various connectors. In this embodiment the transducer insert realizes an advantage in assembly by having electrical communication with portions of the transducer insert not directly attached to the PCB 29 in that those non attached components are free from discrete orientation relative to the PCB 29. Parts desirably directly connected to the PCB 29 would connect to discrete lands sites LD, while pin connections 24, 40 could connect to the land rings. The transducer 22 may also have a land ring instead of discrete connection points 24r. By utilizing land rings in the various components within the transducer, freedom from particular orientations are achieved, and thus provide advantages in manufacturing/assembly of the parts and sub components.

[0059] Although the medical system socket 38 is illustrated (Fig. 5A), this component is not a part of the interchangeable transducer 10, and is merely illustrated here to show the alignment of all the parts described. Desirably the socket utilizes a pancake style slip ring to improve contact regardless or radial orientation.

[0060] The transducer used in the interchangeable transducer design may have a single fixed zone, or be designed having two or more focal zones. The transducer may have an imperfect focal zone achieved through a mechanical distortion formed in the transducer, such as those described in US patent application 10/816197 entitled "VORTEX TRANSDUCER" and filed on March 31, 2004, and US patent application 11/439706 entitled "Medical Ultrasound Transducer Having Non-Ideal Focal Region" filed May 23, 2006. (both applications commonly assigned and herein incorporated by reference). The vortex transducer and the non-ideal focal region transducers allow for a focal region in a circular or donut shaped pattern wherein the pattern is produced by a mechanical offset in the bowl of the transducer. The isolation layer 34 is primarily used to prevent electrical cross talk and

contact corrosion among and between the electrical contacts 40. The shape and size of the focal region can be mathematically calculated and an appropriate mechanical shape to a transducer can be manufactured. This allows the transducer to focus ultrasound waves in particular desired shapes and patterns without requiring the complexity and cost of an electronically steered transducer. The transducer may also be an electronically focused device, such as a 2D array or a phased array transducer.

[0061] Internal details of the transducer-socket connection are now described (Fig. 6A). In one embodiment, there is a housing 16 having a substantially cylindrical shape. The housing 16 has a neck down region located near the isolation layer 34, and a larger diameter near the transducer 22. The transducer side 20 is open, or has a window so ultrasound energy may be broadcast out of the housing 16 unimpeded. The transducer 22 is secured near the open end 20, and connects to an interface 28 via a set of connection pins 24. The connection pins 24 are held in place with a concentric liner 26 inside the housing 16. The interface 28 may be a set of connecting wires as previously described, or may include a circuit, PCB, PC(B)A or other hardware component. The interface may also have additional electronics, such as a transformer 42 for tuning the transducer 22, a data chip or integrated circuit (IC) 30 to help identify the interchangeable transducer 10 to the medical system 300. Additional components are described below.

[0062] Opposite the transducer 22, there is a seal 14 for preventing water or atmosphere from entering the internal compartment of the transducer 10. Working in conjunction with the seal 14 is an isolation layer 34 for reducing pin corrosion and/or cross talk between the external electrical connectors 40. Note the transducer side 20 is also sealed against the outside environment. While the transducer side 20 may be sealed with the transducer 22 itself and various compounds which can be used to prevent leakage, the seal 14 has one or more apertures 50 for the protrusion of the external electrical connectors 40. The apertures 50 are desirably large enough to allow the passage of the electrical connectors 40. The apertures may rely on an interference fit to prevent seepage of fluid between the apertures and the pins, or the use of a sealing agent, or both. The apertures 50 may be sealed once the external electrical connectors 40 are placed using solder, epoxy, resin, adhesive or other suitable sealing agents. A connector 32 is located on the housing and designed for engagement of a corresponding connection on the medical system socket 38. The receiving element 36 and connector 32 form a transducer-system connection. This connection is desirably one having high endurance. Repetitive reliability is desirable, but not required for the transducer

connector 32, as it is not envisioned that any one particular transducer will be removed and inserted a large number of times.

[0063] The design of the transducer connector 32 and the system side connection (receptor) 36 allow for individual transducers to be interchanged with the medical system 300 on demand. This allows a single medical system to have a great deal of variety in its operational scope. Each new transducer can provide added capability as well as replacement for worn or out dated parts. Desirably the mating of the transducer 10 to the system 300 can be accomplished with a low insertion force connector 32 and receptor 36 combination. Though the insertion force is low, the connection is robust so the transducer 10 will be stable while mounted in socket 38. The socket 38 is desirably connected to a motor assembly through a set of cams 326. Electrical communication between the system 300 and the transducer 10 is maintained regardless of how the socket 38 might be moved..

[0064] The electrical pin 40 layout as they extend through the seal 34 are designed to make contact with additional lands built into the socket 38 (Fig. 6B). The socket lands 102a-c form concentric structures within the socket. There are isolation rings 104 between the electrical connection lands. The electrical pins 40, now identified individually 40a, 40b, 40c (Fig. 6B) each carry a separate electrical signal from the medical system 100 to the interchangeable transducer 10. The individual connectors may carry power, transmit/receiver signal information, IC chip detection, ground or other signals as desired. The corresponding lands in the socket PCB form concentric rings for connection with each pin separately. This is achieved by arranging the electrical pins 40a-d at a discrete radius from the center of the transducer connector end. Then the transducer housing engages the socket, the pins of the transducer housing match up to the appropriate concentric lands of the slip ring. In this fashion, even if the transducer is rotated within the socket, the proper electrical pin 40a-c always remains in contact with the corresponding land ring forming corresponding pin-land connections 102a-40a, 102b-40b, 102c-40c. There is no limit to the lands 102x and connector pins 40x and as many pairings as are desired may be incorporated into the design. When the transducer is mated with the system, the electrical pins and PCB lands match up, and provide a secure electrical connection (Fig. 6C). The pressure used to hold the removable transducer 10 in place with the system side socket 38 desirably provides sufficient force exerted on the isolation layer 34 to prevent fluid from seeping into the region between the isolation layer 34 and the recess of the housing 16A where the isolation layer is placed. The isolation layer may also be manufactured with flanges on the bottom (not shown) so that isolation layer forms

discrete channels or chambers for each electrical connector, or groups of connectors, as the flange or ridge configuration on the top side of the isolation layer.

[0065] The pin layout and slip ring described herein and shown in the figures represents one embodiment, however this embodiment is not meant to be limiting of the connector layout. The number of electrical pins in the “plug” end of the transducer may be as many as 5 desired or needed to perform the necessary tasks of providing electrical connection, or even stabilizing plugs for structural integrity. The lands of the slip ring like wise may be as many as desired and it does not necessarily follow that each land will have a corresponding electrical connector. A land may be used as a cross-talk sensor by having no physical pin 10 designed to make contact with it, yet still monitor electrical signal when the connection is made. The land itself can be used as an electrical sensor to monitor the safety and stability of the electrical connection and/or the isolation between lands.

[0066] An alternative embodiment using the pancake slip ring PCB 29 in the insert is now described. The transducer insert resembles the assembly previously described. Individual 15 components such as a transformer 42 are still directly connected to the modified PCB 29 (Fig. 6D). The electrical pins 24, 40 are no longer connected to discrete traces on the PCB 29. The electrical pins 24, 40 are now pressed against the trace rings 102a-c on the PCB 29. This allows the top section 16A and bottom section 16B to be press fit together without regard to the orientation of the parts relative to each other. No matter what orientation the top 16A has 20 to the bottom 16B, the electrical pins 24, 40 will still match up with the traces to provide proper electrical communication from the communication port to the transducer.

[0067] In another embodiment using either the standard PCB 28 or the slip ring PCB 29, the transducer 22 may have a trace ring 24LR around the circumference of the transducer so the transducer may also be assembled to the bottom 16B section without concern for 25 orientation and placement of the electrical pins 24 to the transducer 22.

[0068] A close up of the electrical pin connections 40 to the top of the slip ring PCB 29 is now shown (Fig. 6E). Here the discrete connections for the transformer 42 are shown in the form of a series of discrete lands LD or trace positions.

[0069] The adaptor for the transducer insert 10 need not be circular, though the circular 30 design is desirable. Various other shapes allowing for multiple orientation of the transducer insert are shown in Figs. 6G-6I. To simplify the process of replacing the transducer insert 10 for a user, the transducer adaptor has a “keyless” orientation to the “socket” on the system

side. So the adaptor may be oblong for two orientations, triangular for three orientations, progressing to a circular insert and socket (Fig. 6I). There is also no restriction on the shape of the adaptor as being a regular shape, so long as the adaptor shape is symmetrical about one axis so the adaptor can still mate with the ultrasound system when it is oriented in another symmetric alignment. Regardless of the physical shape of the insert connector and socket, the socket has electrical contacts in the form of slip rings (dotted lines in Figs. 6F-6I), with electrical contact pins set at the desired radius to make physical contact with the corresponding land so the appropriate pins 40a-x communicates with the corresponding lands 102a-x.

10 [0070] The orientation of the interface 28 as shown in Figs. 5, 6A-6C need not be perpendicular to the axis of the transducer housing. The interface 28, along with any additional components may be at any orientation desired. In one embodiment, the interface 28 is a PCB or PCA aligned with the axis of the housing 16 (Fig. 7) and has connection wires 12 from the external electronic connectors 40 to a PCB style interface 28 having a transformer 42 and a data IC 30 along with other electronics as may be desired.

15 [0071] In another embodiment, the interface may be a PCB with a data IC having additional embedded information. The data IC 30 may include data related to the number of uses the transducer is allowed to be activated, or it may record use data which can be used to help improve future interchangeable transducer designs (such as measuring attenuation, feedback, decoupling, thermal information or the like). While this collected data may be stored in the data IC, additional sensors 4021-i could be added to the interface 28 to record the desired data (Fig. 8).

20 [0072] The isolation layer 34 used with the interchangeable transducer may be a washer or disk of electrical isolation material. While the isolation layer may be a solid or otherwise uniform component, an independently novel design for an electrical isolation layer is desirable.

25 [0073] An isolation layer well suited for providing isolation between individual contacts in a wet environment is realized in the form of a slip ring seal (spacer). The slip ring spacer is provided at the docking end of the connectorized transducer. The slip ring spacer may have any one of a variety of forms consistent with the general description and requirements described herein, or similar or equivalent to any of the enumerated embodiments described. The slip ring spacer provides a bumper between the connectorized transducer and the socket

of the medical system. Furthermore, the seal provides apertures or other means of allowing electrical communication through the seal, between the connectorized transducer and the socket. In addition, the seal allows for simultaneous electrical communication between multiple isolated electrical connectors in a wet environment. The seal provides isolation of each separate electrical connector type, reducing cross talk between different kinds of signal and/or power connectors. The slip ring seal is desirably made from or has properties incorporated into it, that provide water and electrical resistance. If the material is slightly conductive, it is possible for a short to occur between the electrical pins even in the presence of a partial or complete fluid seal.

10 [0074] A slip ring spacer is now described as shown in Figs. 9A-9E. The slip ring spacer 900 has a base 902 and one or more flanges or ridges 9041-i rising from the base. The ridges or flanges are adapted to press against a slip ring SR and form one or more concentric channels 9061-i so that each electrical connection ring of the slip ring SR is separated from the other electrical connection rings by the ridges 9041-i. When the slip ring seal 900 is pressed against a slip ring SR, channels 9061-i are formed by the ridges or flanges of the slip ring. The ridges are pressed against the slip ring SR, forming a seal against fluid flow between the discrete channels 9061-i. The slip ring forms one barrier to fluid movement while the slip ring seal forms the sides and bottom of the channels. In this way, electrically conductive fluid is restricted from flowing between the channels, and exposure to the electrical pins is reduced. This minimizes corrosion and cross-talk among and between the electrical pins. The base desirably has apertures for electrical pins or connectors for making contact with the electrical connection rings on the slip ring. In operation, the slip ring spacer 900 allows each connector to communicate with a corresponding slip ring pad without producing cross talk between other channels, even if the environment is wet.

25 [0075] The pin connectors may be organized into groups so that multiple pins may be intended to make contact with a slip ring land. In this case the pins may be organized into groups, similar to the two pins 40b, 40i sharing a single circular channel (Fig. 9A). This illustration is an example of more than one pin designed to make contact with a single land, and there is no limit to the number of pins that can be grouped into a single channel or group, or the number of groups that can be used in the interconnection arrangement between the transducer and the socket.

[0076] Alternatively the slip ring spacer may have flanges or ridges on the underside of the base (not shown) in a pattern similar to the flange or ridge pattern on the top surface of the spacer. The presence of flanges or ridges on the bottom of the spacer can help isolate the electrical contact pins from one another in the event fluid seeps below the slip ring seal
5 during operation.

[0077] The slip ring spacer 900 may utilize numerous alternative embodiments. The slip ring spacer 900 has individually isolated electrical pin zones (Fig. 10). In this embodiment each aperture 40 of the slip ring spacer 900 has one or more rising ridges 904 surrounding each aperture. The outer rim of the base 902 is also encircled with a flange or ridge 904R to
10 minimize water or fluid flow from the outside of the connector to the inside components. The individual electrical pins that would protrude through the apertures are individually insulated to reduce the risk of electrode corrosion and/or cross talk.

[0078] A single spiral channel can be formed with a spiral shaped ridge (Fig. 11) with periodic partitions placed in the spiral pattern. The spacer may use various arrangements of
15 ridges or flanges extending from the base. The ridges may be tapered, block shaped, or arranged in a series of thin partitions operating as a group (Figs. 12A-12C). Desirably the spacer is made from material that has high water and electrical resistance (like rubber, RTV (Room Temperature Vulcanization) silicone rubber, polymers, etc...). The material desirably has a durometer low enough to allow the flanges or ridges to deform when they are pressed
20 against a slip ring so the flanges will deform slightly to seal against the slip ring. Designs that are more structurally robust desirably have a lower durometer material with a wider area of contact (Figs. 12A, 12B) while configurations of the seal having a more rigid construction may use material that is a higher durometer material, but a reduced area of contact (Fig. 12C).

[0079] In another embodiment the spacer has a top portion that can compress directly on to
25 the slip ring, and pressure pressure forces any fluid out of the surface area of the slip ring itself so the electrical connection can be made relatively free of any fluid. In another embodiment, temporary channels 1301 may join the apertures for the electrical pins, to the outer circumference of the slip ring seal so water may escape or be forced away from the electrical pin outs (Figs. 13A-13B). As the seal is pressed against the slip ring, the channels
30 are compressed against the slip ring surface, and thus reducing the flow of fluid among the electrical connections to a level where cross talk between the slip ring lands is acceptable.

[0080] In yet another embodiment of the spacer, the spacer may comprise a water and electrically resistant material having a web like structure (Fig. 14A-14C). Gap spaces between the webbing serve as apertures for the electrical pins to protrude from the transducer and the medical system socket. Optionally the webbing may have additional material between the web strands to further restrict water flow between the web strands when the slip ring seal is compressed into position between the interchangeable transducer and the system socket. As the spacer is pressed against the slip ring while the connectorized transducer is pushed into the socket of the medical system, the webbing with or without additional material in the webbing) collapses and presses fluid out of the cells and away from the electrical connectors. The collapsed webbing forms a barrier to fluid flow between the web strands. The webbing may be organized (Figs. 14A-14C) or randomly distributed in the formation of the seal (Figs. 15A-15C).

[0081] In operation, a transducer as described herein can be removed from a socket, and then a new one inserted without regard to the radial orientation of the transducer relative to the socket. If the environment containing the socket is wet, the seal on the transducer allows the transducer housing to make good connection on the electrical lands on the socket side, while ensuring solid connection with the transducer and internal workings of the interchangeable transducer. Seams or assembly joints may be sealed with resin or epoxy if needed. Seams and assembly joints may also be sealed with solder, ultrasound welding or similar techniques.

[0082] In addition to the embodiments described above, alternative interconnect schemes suitable for use with the present invention are now described. Alternative transducer signal connections include using direct electrical connection via pin and socket, direct electrical connection via soldered spring contact and PCB trace, direct electrical connection via PCB trace to floating spring contact (e.g. in carrier) to PCB trace, direct electrical contact via a post and socket with multiple connections (e.g. stereo headphone jack), as well as wireless types of interconnects, such as inductive coupling, and capacitive coupling.

[0083] The transducer can be secured within the housing by gluing it or mechanically affixing it to the housing. The transducer may be sandwiched between a preformed lip in the housing and the electrical connection pins 24. In another embodiment the transducer may be attached using a soluble adhesive allowing for the transducer ceramic to be replaced when the interchangeable transducer fails.

[0084] Structurally the physical connector between the transducer housing and the socket may be combined with the electrical connectors. One may visualize a series of stacked electrical connector rings designed to match up to corresponding pin connectors within the socket. Alternatively the relationship of socket and insert may be reversed so the transducer
5 has a socket for receiving a male end adaptor from the medical system.

[0085] In other embodiments, the physical connection between the transducer housing and the socket can be achieved through any low force insertion mechanism suitable for the medical system and medical procedures desired. These may include a bearing ring, a snap ring, or simply frictional engagement. Rotational capability of the transducer housing within
10 the socket is not critical, so long as the transducer electronically connects to the medical system electronics through the unaligned electrical connections.

[0086] Additional alternative embodiments of the present invention will be readily apparent to those skilled in the art upon review of the present disclosure. The lack of description or the embodiments described herein should not be considered as the sole or only method and
15 apparatus of providing for an interchangeable transducer. The scope of the present invention should not be taken as limited by the present disclosure except as defined in the appended claims.

WHAT IS CLAIMED IS:

- 1 1. An insert for use with a medical ultrasound system, the insert
2 comprising:
3 a housing having an adaptor end and an acoustic end;
4 a communication port at said adaptor end, the adapter end having two or more
5 orientations for engagement to a receptacle in a medical ultrasound system;
6 a transducer at said acoustic end, said transducer forming a fluid tight seal
7 with said housing; and
8 a means for electrical communication between said communication port and
9 said transducer.
- 1 2. The insert as described in claim 1, wherein said connection port further
2 comprises an isolation layer.
- 1 3. The insert of claim 2, wherein the isolation layer is a slip ring spacer.
- 1 4. The insert as described in claim 1, wherein the adapter end has radial
2 freedom to engage a receptacle in any radial orientation.
- 1 5. The insert as described in claim 1, wherein said electrical contacts are
2 spring loaded contract pins.
- 1 6. The insert as described in claim 1, wherein the transducer has two or
2 more discrete focal zones.
- 1 7. The insert as described in claim 1, wherein the transducer has an
2 imperfect focal region.
- 1 8. The insert as described in claim 1, wherein the adaptor end is slidably
2 engaged into said medical ultrasound system.
- 1 9. The insert as described in claim 1, wherein said electrical connector
2 comprises one or more electrical components.
- 1 10. The insert as described in claim 1, wherein the electrical connector are
2 a first set of spring pins frictionally engaged between said communication port and a PCB,
3 and a second set of spring pins frictionally engaged between the PCB and the transducer.

- 1 11. The insert as described in claim 1, wherein the insert is disposable.
- 1 12. An interchangeable transducer apparatus adapted for use with a high
2 intensity focused ultrasound (HIFU) medical system, the apparatus comprising:
3 a substantially rigid and hollow housing having an axial alignment and having
4 a first end and a second end;
5 a transducer positioned within the first end of the housing, the transducer
6 being electrically connected to an interface disposed within the housing and forming a fluid
7 tight seal with the housing;
8 an isolation layer positioned within the second end of the housing, the
9 isolation layer having a plurality of apertures for receiving a plurality of electrical connectors
10 extending from the interface;
11 a connector positioned on the exterior surface of the housing, the connector
12 allowing for the removable engagement of the housing with an ultrasound medical system;
13 wherein the connector and electrical connectors provide releasable mechanical
14 and electrical engagement (respectively) to a receptacle in the medical system in two or more
15 axial alignments between the housing and the ultrasound medical system.
- 1 13. The apparatus of claim 12, wherein said ultrasound medical system is a
2 high intensity focused ultrasound (HIFU) medical system.
- 1 14. The apparatus of claim 12, wherein the isolation layer is a slip ring
2 spacer.
- 1 15. The apparatus of claim 14, wherein the slip ring spacer has a plurality
2 of concentric rings adapted to isolate the electrical connectors from one another.
- 1 16. The ultrasound medical system of claim 12, wherein the receptacle is a
2 wet environment.
- 1 17. The apparatus of claim 12, wherein the interface is a circuit.
- 1 18. The circuit of claim 17, further comprising at least one electronic
2 control component for controlling the transducer.

1 19. The apparatus of claim 12, wherein the interface is a printed circuit
2 board or assembly (PCB or PCBA).

1 20. The apparatus of claim 12, wherein the electrical connectors are spring
2 loaded contact pins.

1 21. The apparatus of claim 12, wherein the transducer has two or more
2 discrete focal zones.

1 22. The apparatus of claim 12, wherein the transducer has an imperfect
2 focal region.

1 23. The apparatus of claim 12, wherein the apparatus is disposable.

1 24. The apparatus of claim 12, wherein the electrical connectors are
2 arranged at a specific radius from the center of the seal so as to match a corresponding set of
3 connection rings in a socket of a medical system.

1 25. The apparatus of claim 12, further comprising an inert gas filled
2 interior.

1 26. A slip ring spacer comprising:
2 a base formed from a non-conductive and fluid resistant material;
3 a plurality of apertures extending through said base, said apertures capable of
4 slidably engaging a plurality of electrical connectors;
5 one or more flanges (ridges) extending from said base, said flanges arranged
6 so as to isolate said plurality of apertures into a plurality of cells.

1 27. The spacer of claim 26, wherein said flanges form an enclosed space
2 when pressed against a slip ring, said enclosed space being substantially sealed against fluid
3 flow.

1 28. The spacer of claim 26, wherein said flanges are arranged to form
2 concentric rings.

1 29. A slip ring spacer comprising:

2 a base made from a substantially electrically insulating and fluid resistant
3 material;

4 a plurality of concentric circular ridges rising from said base, said ridges
5 forming a center ring and one or more concentric channels; and

6 a plurality of apertures extending there through said base into said center ring
7 and at least one concentric channel.

1 30. The spacer of claim 29, wherein said plurality of concentric circular
2 ridges are of varying heights extending from said base.

1 31. The spacer of claim 29, wherein said plurality of concentric circular
2 ridges are of varying thicknesses.

1 32. The spacer of claim 29, wherein at least one of said plurality of
2 concentric circular ridges has a gap space to allow connection between two or more
3 concentric channels.

1 33. The spacer of claim 29, wherein the ridges rising from the base are
2 compressible.

1 34. A compressible slip ring spacer made of an electrical insulating
2 material comprising:

3 a web like structure, the web being sufficiently dense to prevent fluid flow
4 through the web strands; and

5 a sponge like structure, the sponge structure being sufficiently porous to allow
6 fluid flow through the sponge like structure when said sponge like structure is compressed;
7 and

8 at least one aperture extending there through said sponge like structure,
9 wherein said web like structure has strands which isolate each aperture so as to prevent fluid
10 flow between apertures when said spacer is compressed, but allowing fluid flow through the
11 apertures as the spacer is compressed.

1 35. An apparatus for electrical communication in a wet environment, the
2 apparatus comprising:

3 a removable electrical appliance having a docking plug, the docking plug

4 having one or more electrical contacts extending from said appliance to a medical system, the

5 docking plug having a slip ring spacer composed of an electronically insulating material and
6 having one or more apertures for the electrical contacts to extend through the slip ring spacer;
7 a receptacle on a medical system, said receptacle adapted for removably
8 receiving the docking plug, the receptacle having a pancake slip ring to provide electrical
9 signals to the removable electrical appliance;
10 wherein the electrical contacts match the radial positions of the slip ring lands,
11 and the slip ring spacer mates to the slip ring to form a substantially wet seal between the
12 docking plug and receptacle.

1 36. A method for assembling a slip ring structure, said method comprising:
2 disposing a slip ring spacer as in claim 1 adjacent to a plurality of electrical
3 contacts, wherein the contacts extend through said apertures in the base;
4 engaging a slip ring against the slip ring spacer such that the slip ring spacer
5 mates to the slip ring to form an assembly having a wet seal; and
6 exposing the assembly to a wet environment.

+

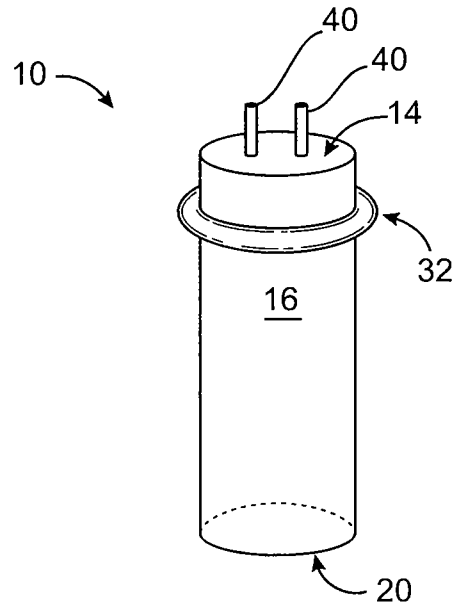


FIG. 1

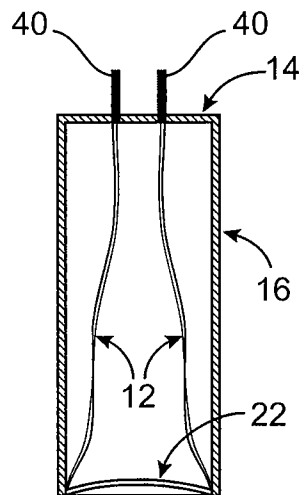


FIG. 2

+

+

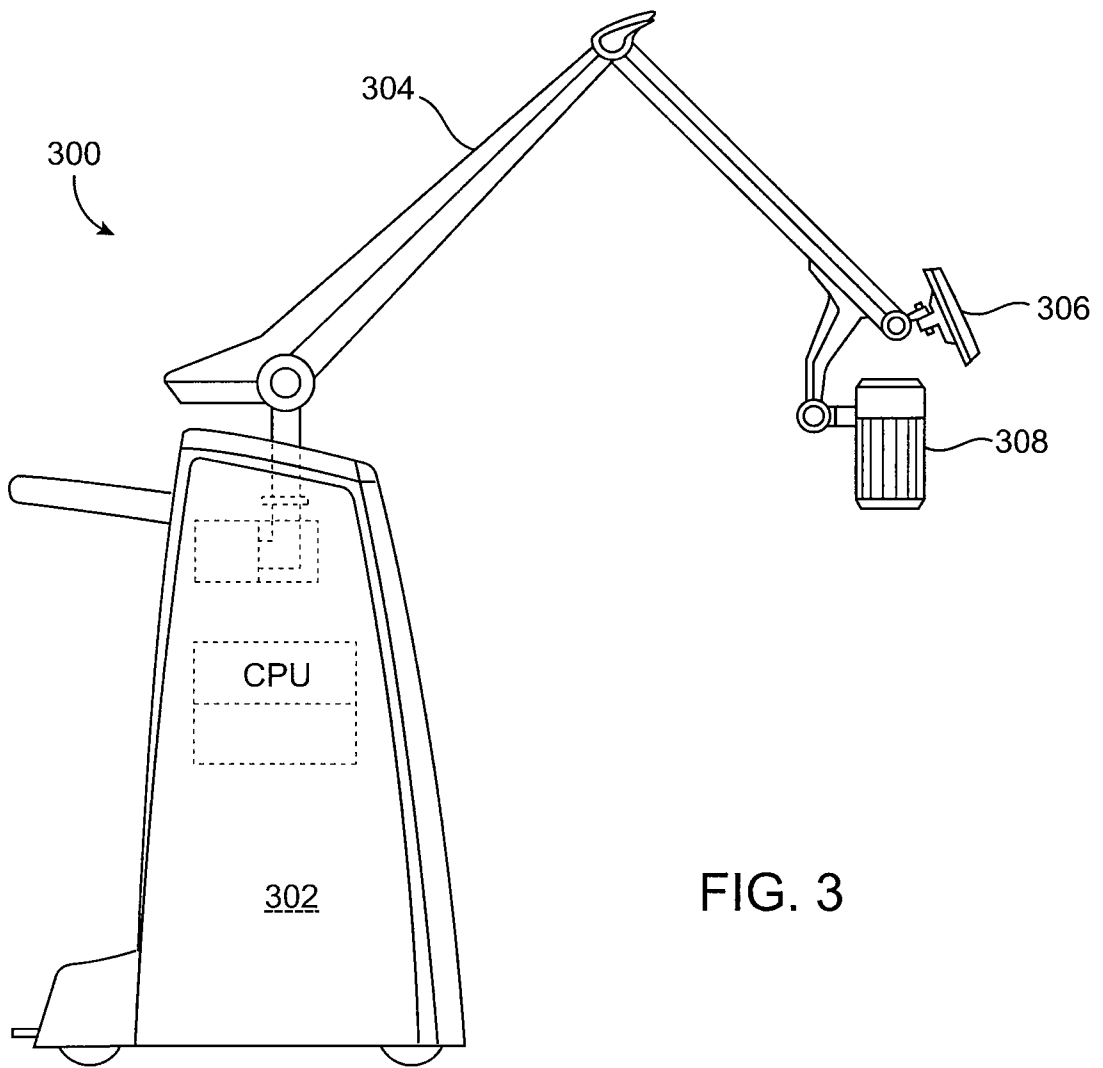


FIG. 3

+

+

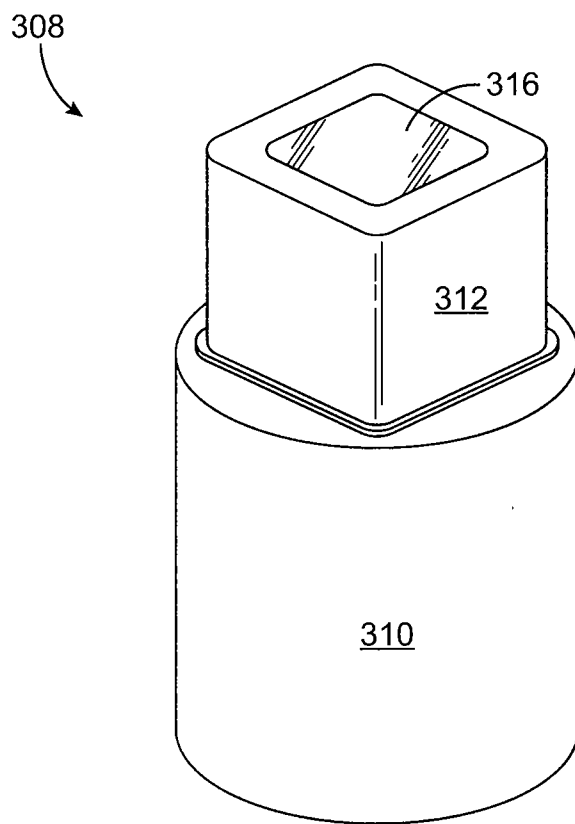


FIG. 4A

+

4/21

+

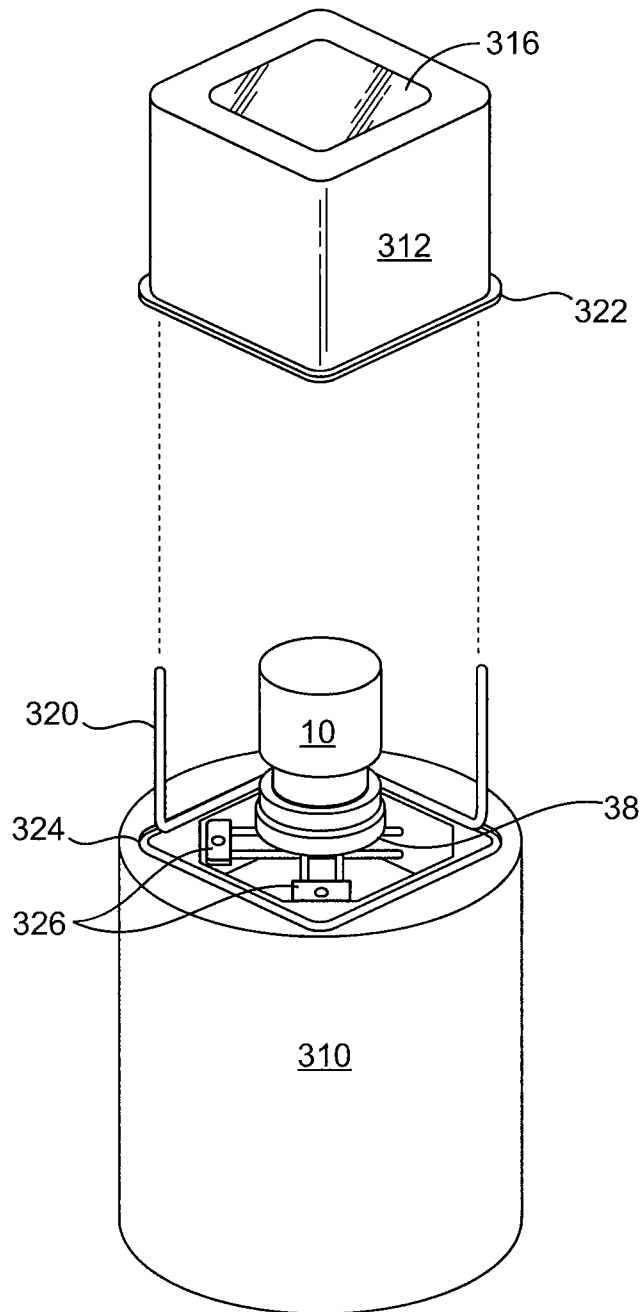


FIG. 4B

+

5/21

+

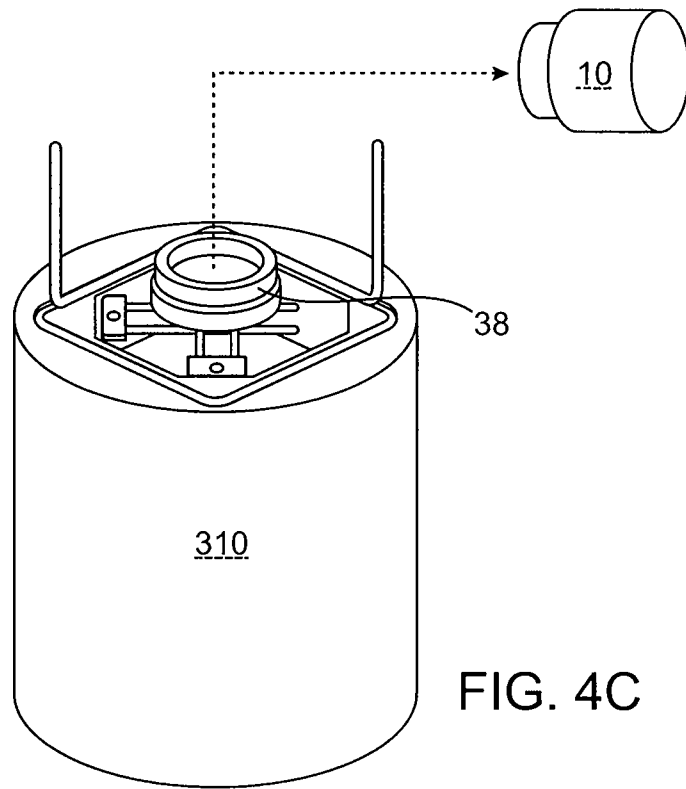


FIG. 4C

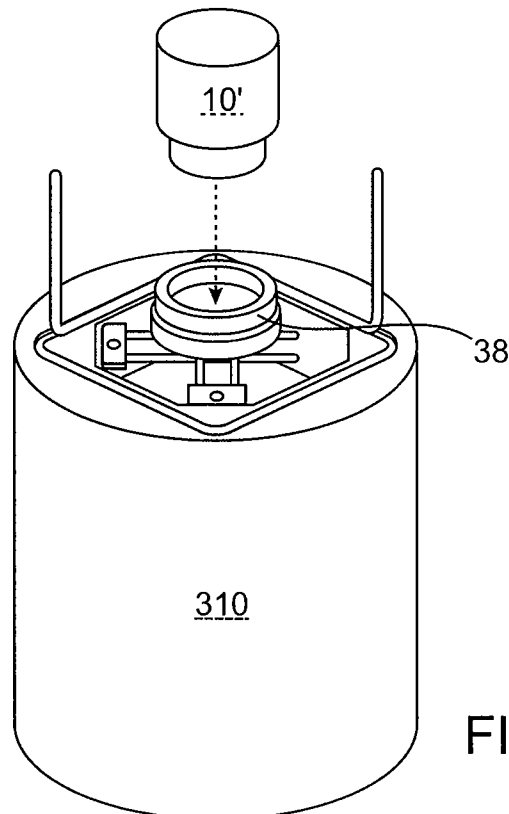


FIG. 4D

+

6/21

+

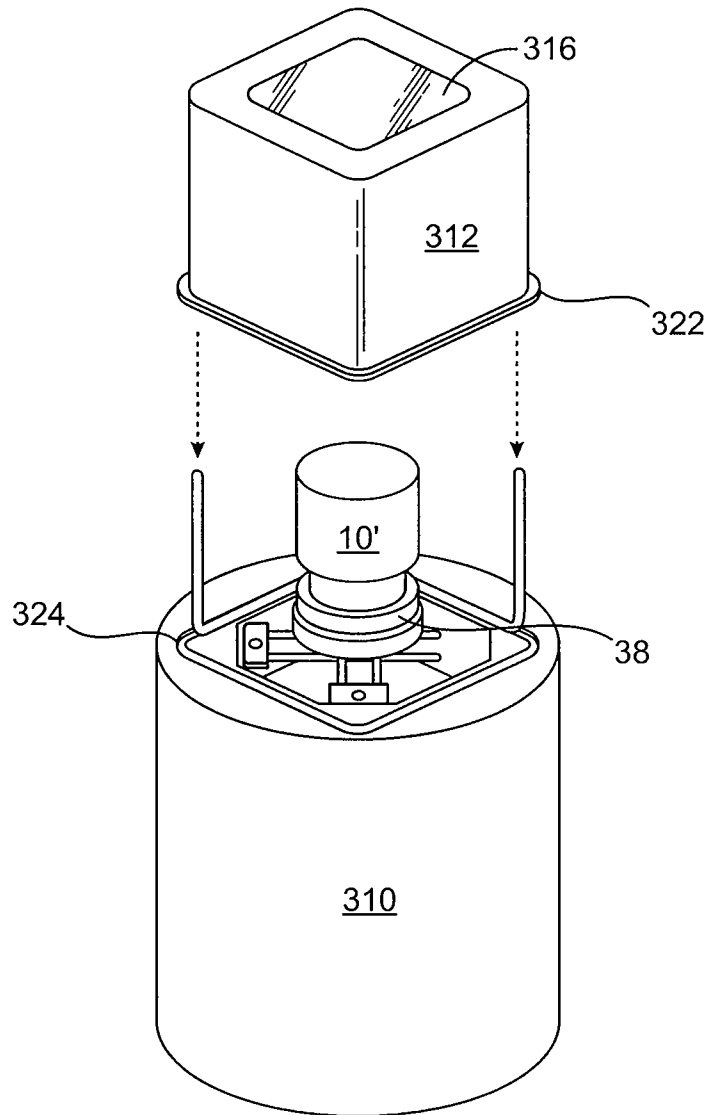


FIG. 4E

+

7/21

+

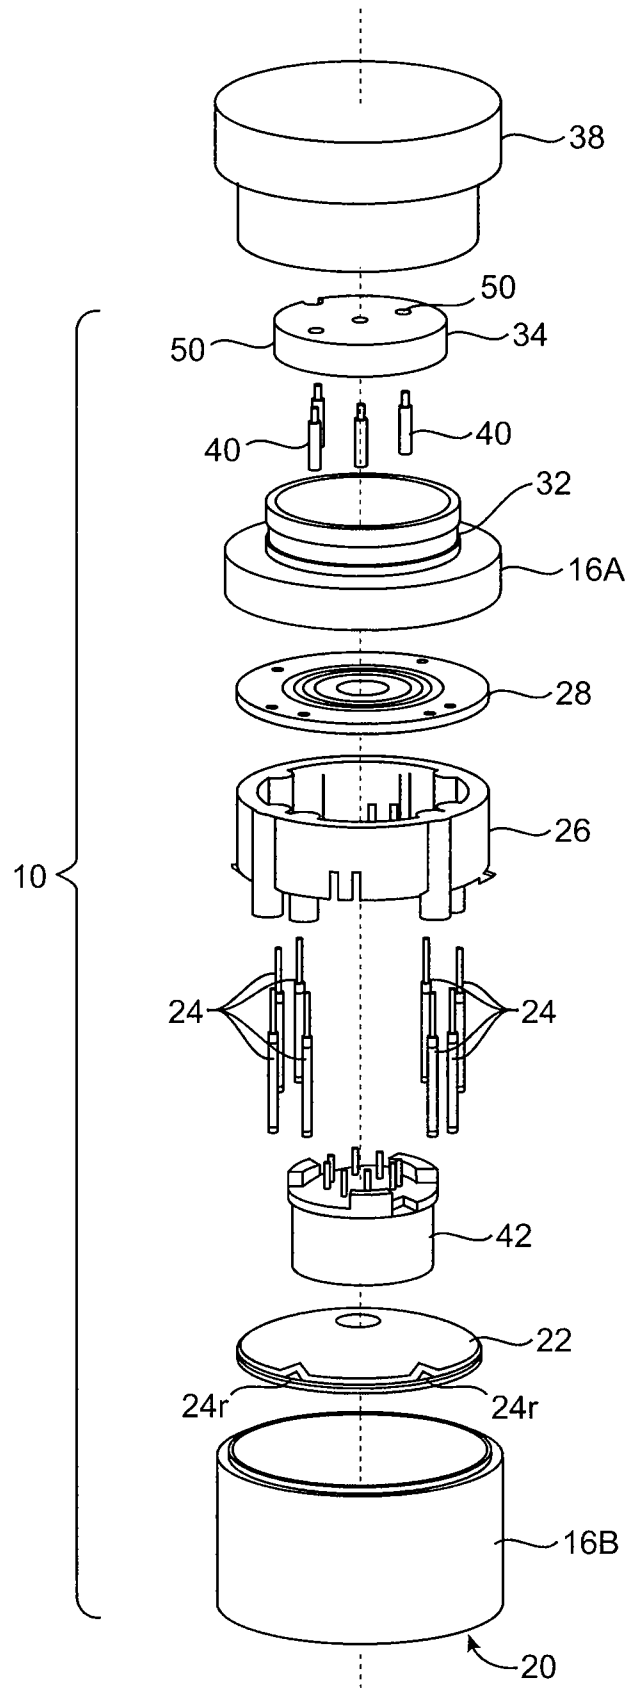


FIG. 5A

+

+

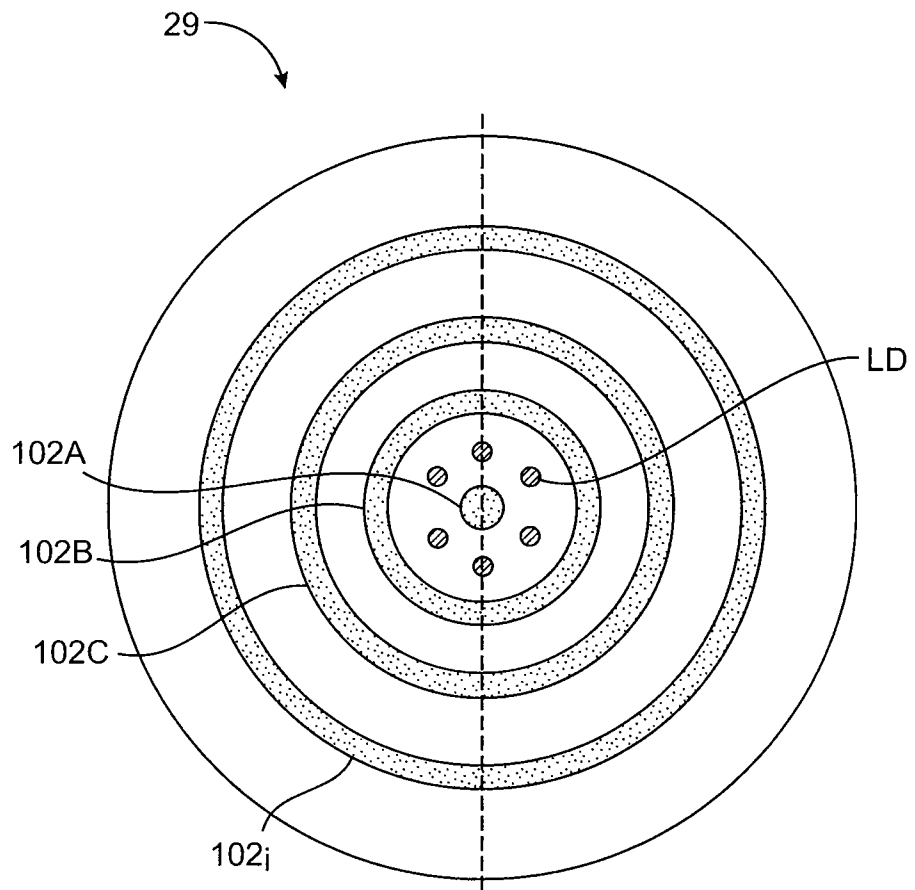


FIG. 5B

+

+

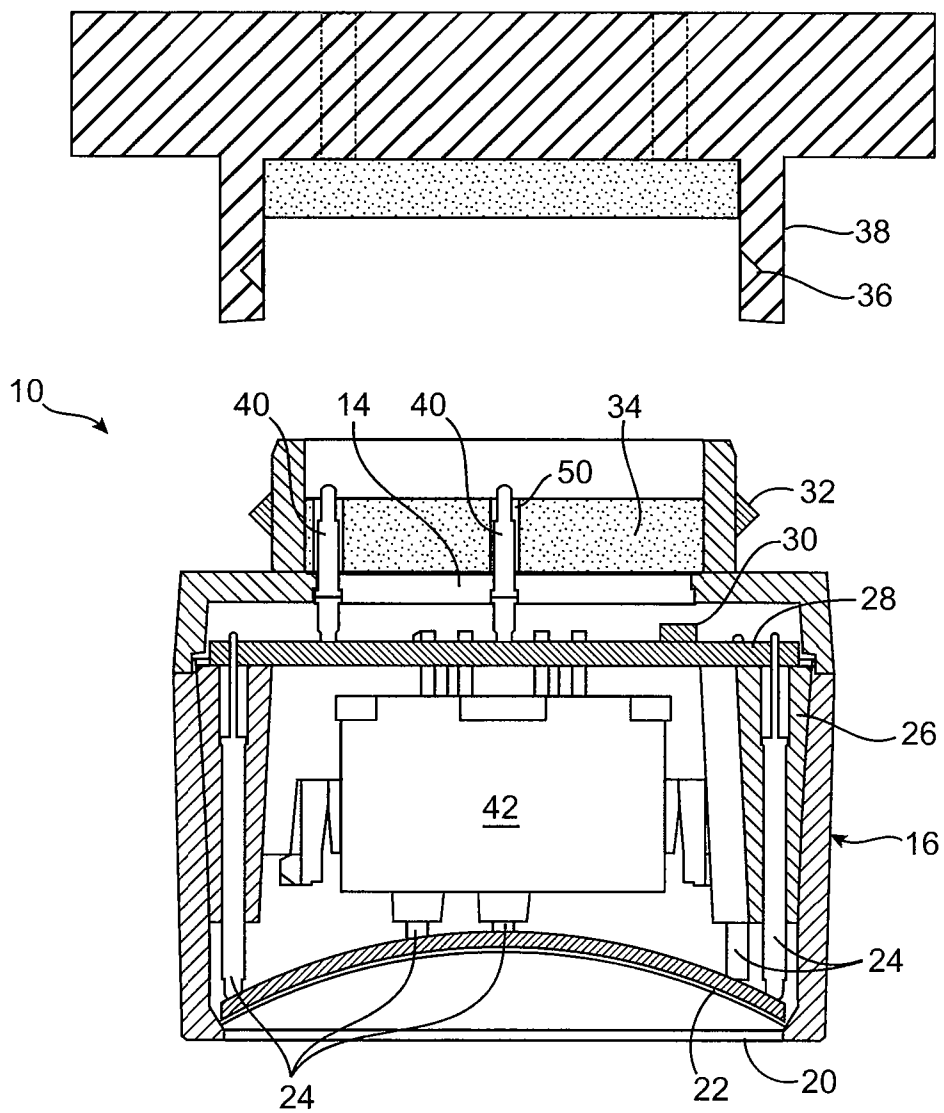


FIG. 6A

+

10/21

+

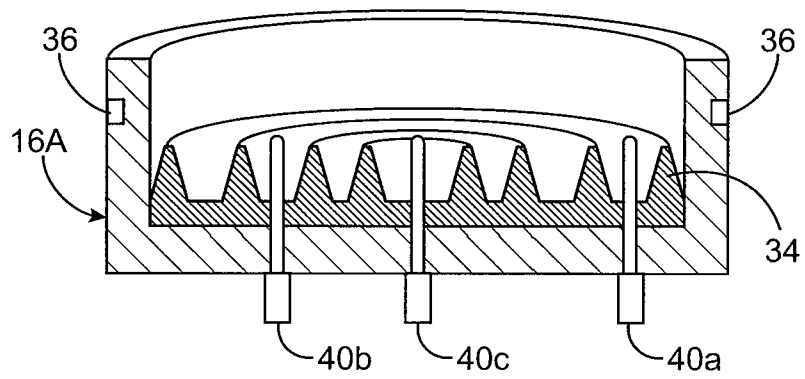
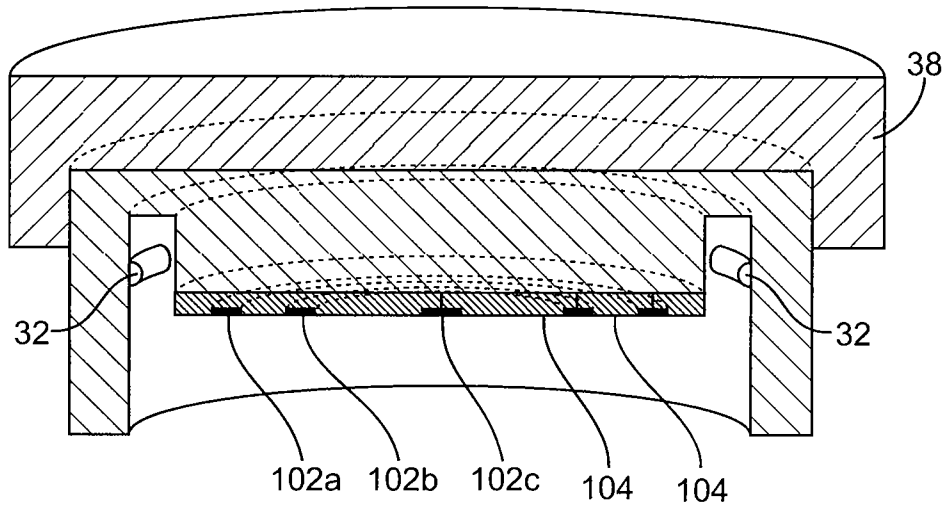


FIG. 6B

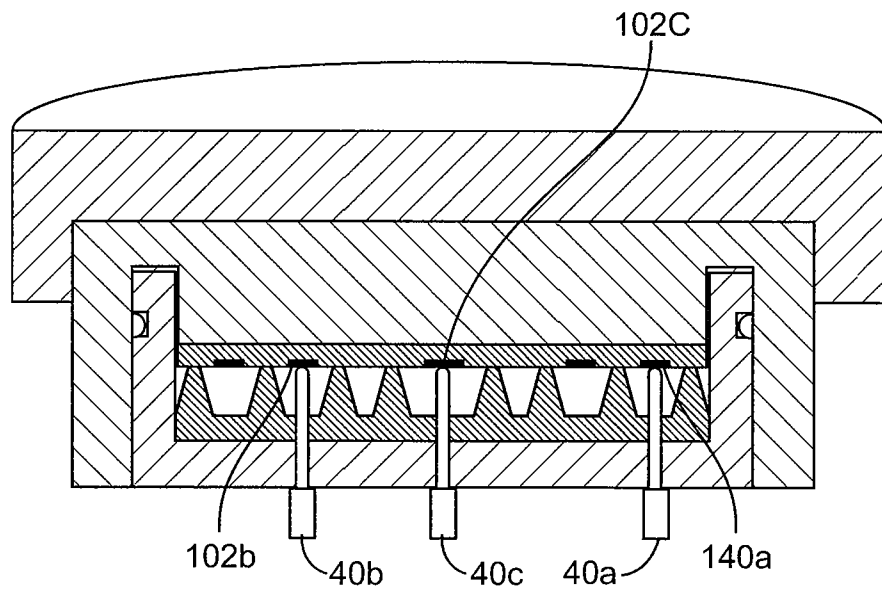


FIG. 6C

+

+

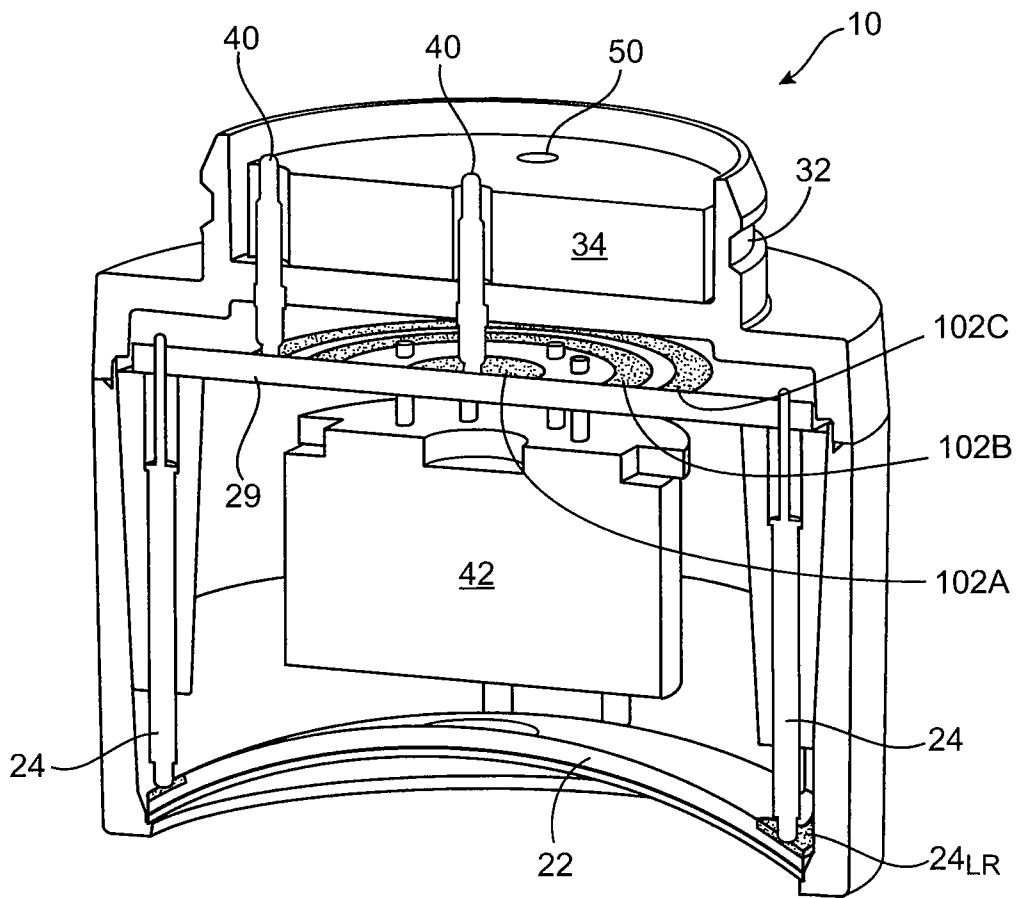


FIG. 6D

+

+

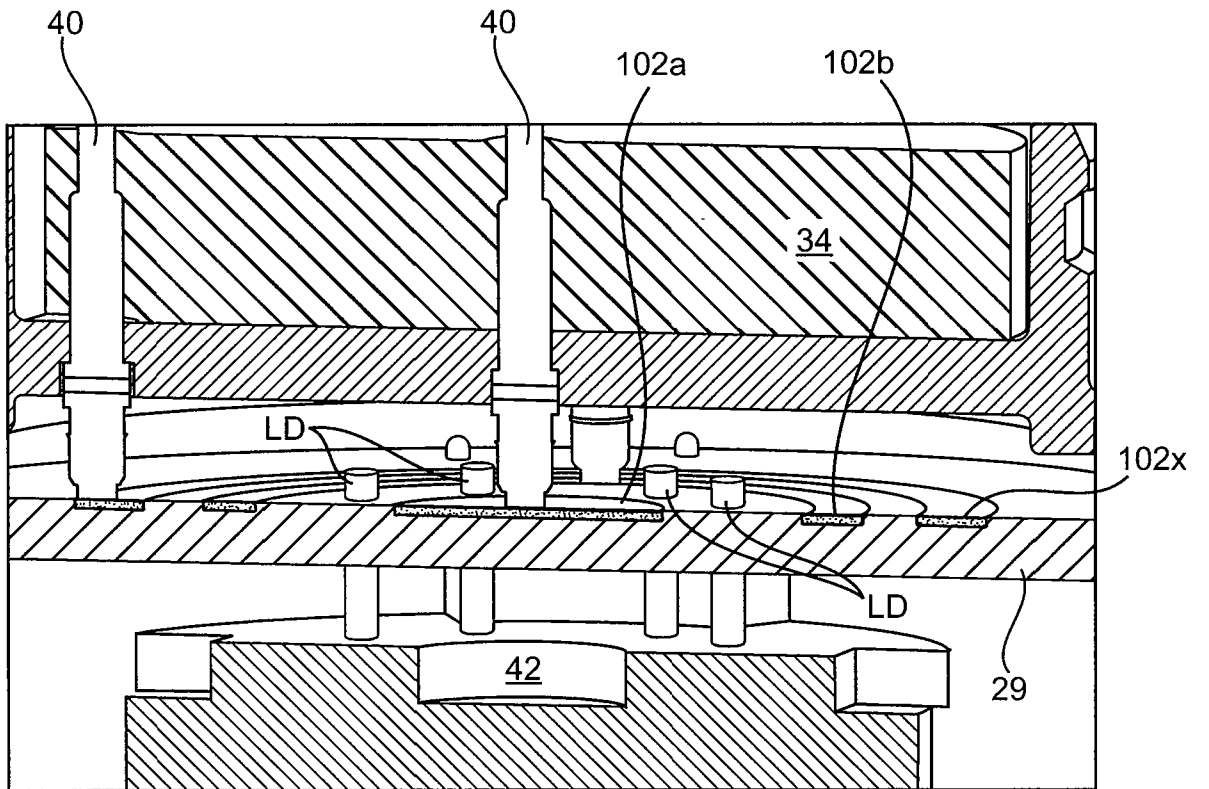


FIG. 6E

+

13/21

+

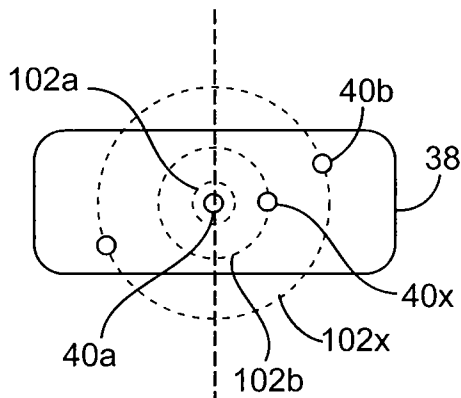


FIG. 6F

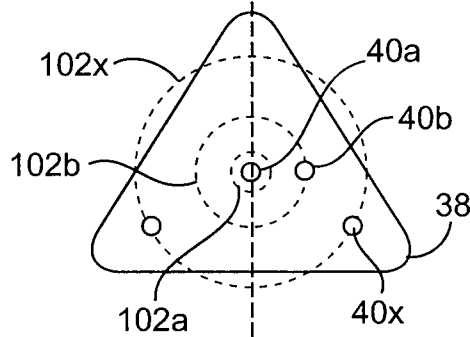


FIG. 6G

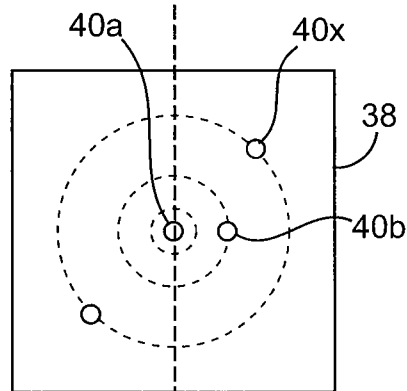


FIG. 6H

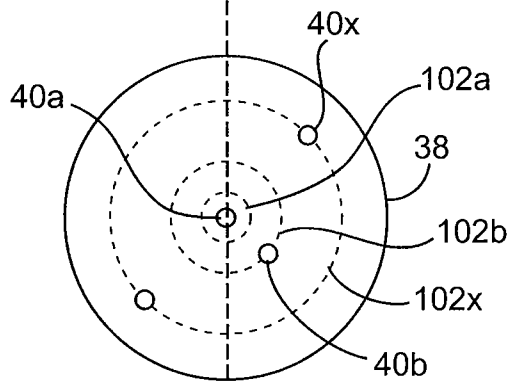


FIG. 6I

+

+

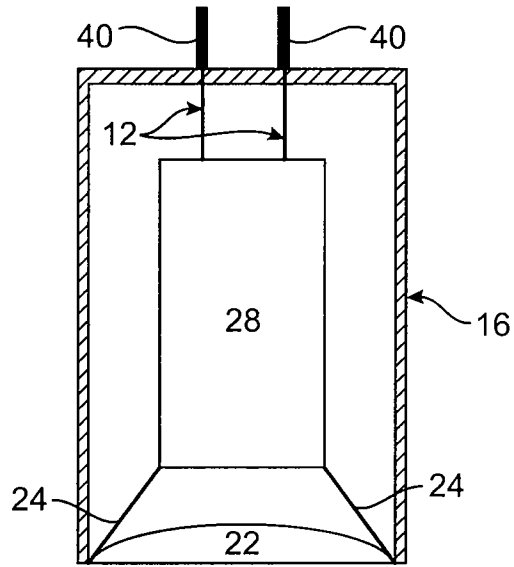


FIG. 7




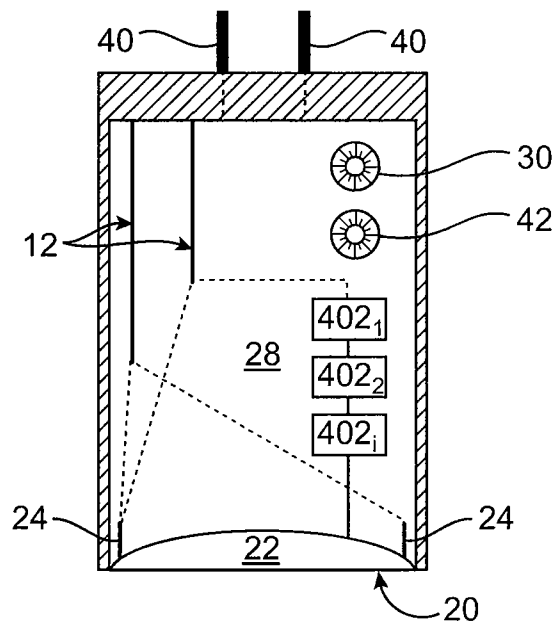


FIG. 8

+

+

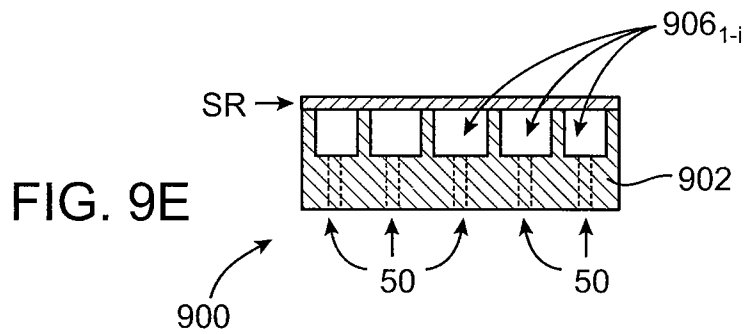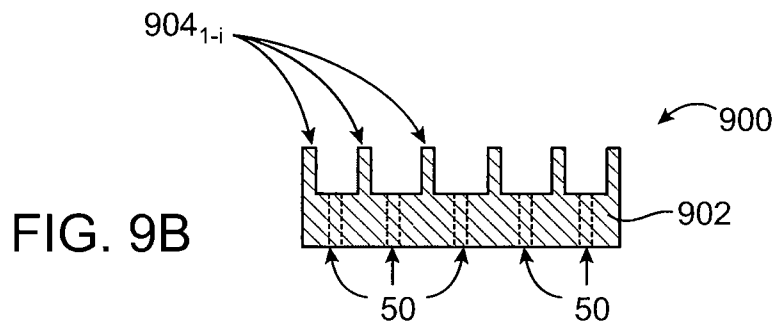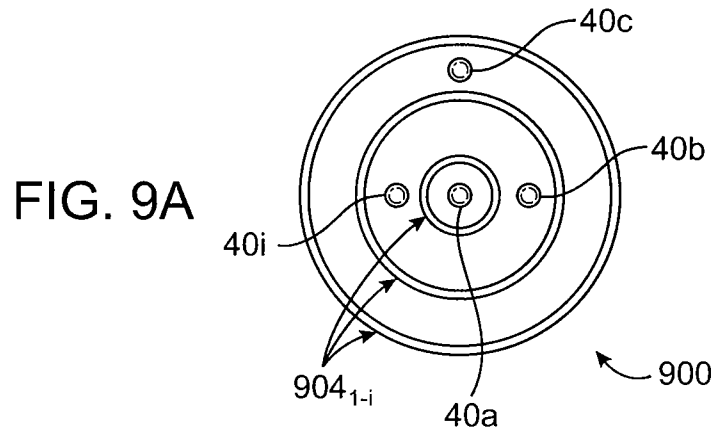

+

+

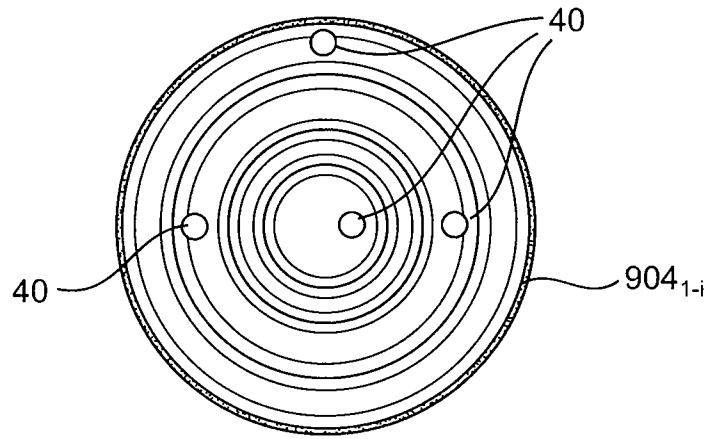


FIG. 9C

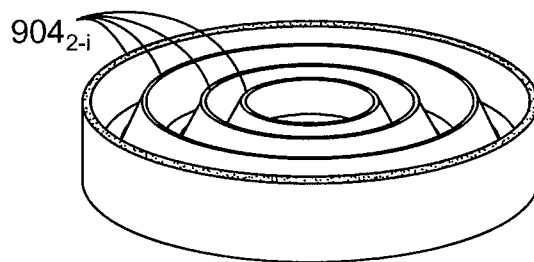


FIG. 9D

+

+

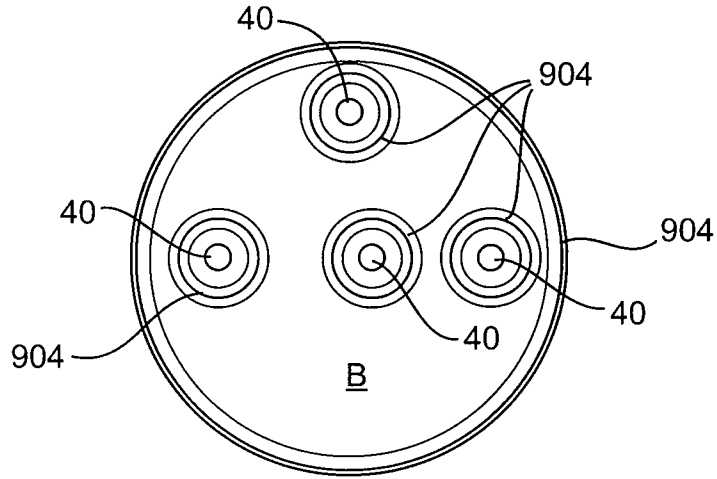


FIG. 10

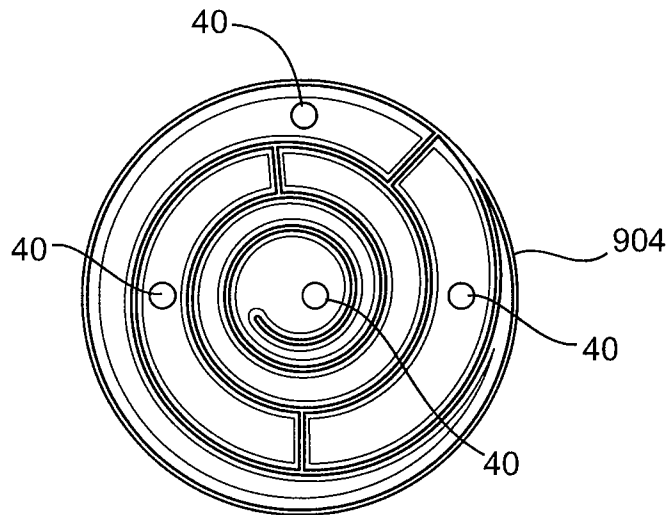


FIG. 11

+

+

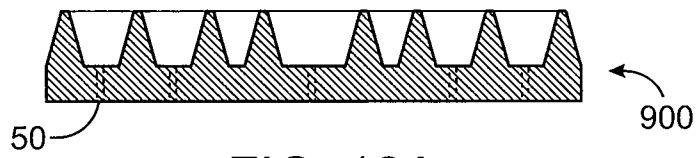


FIG. 12A

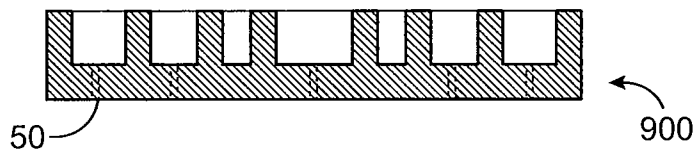


FIG. 12B

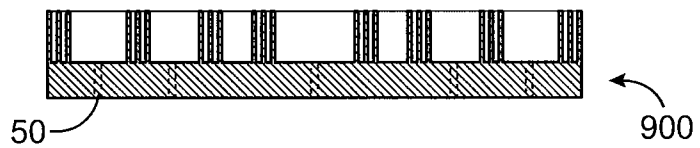


FIG. 12C

+

+

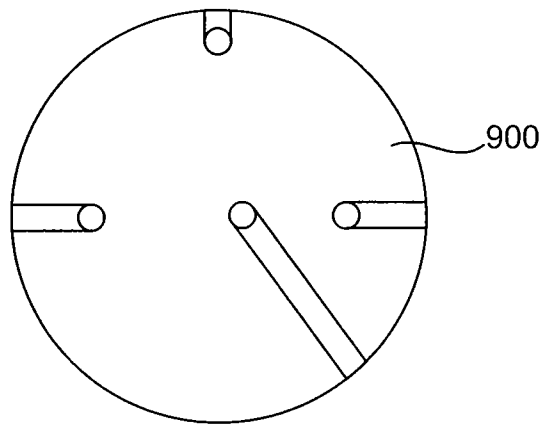


FIG. 13A

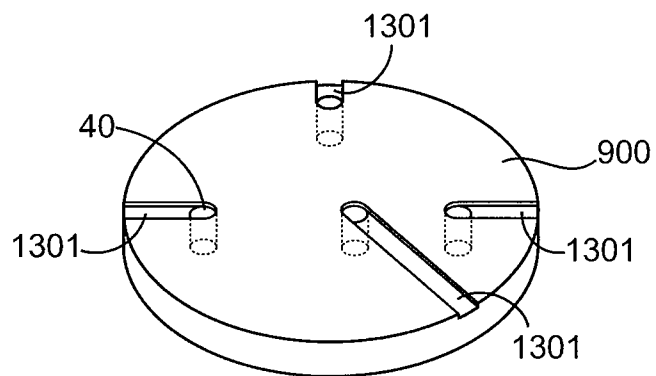


FIG. 13B

+

+

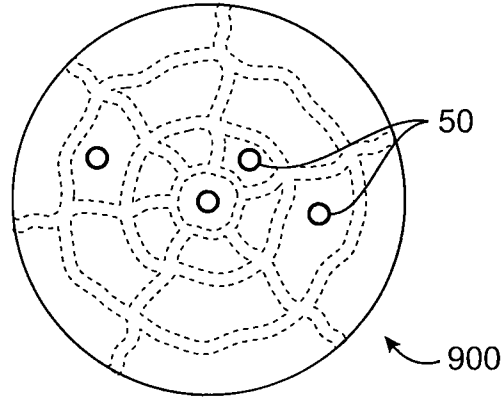


FIG. 14A

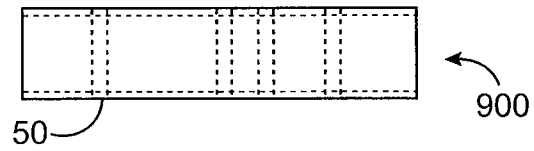


FIG. 14B

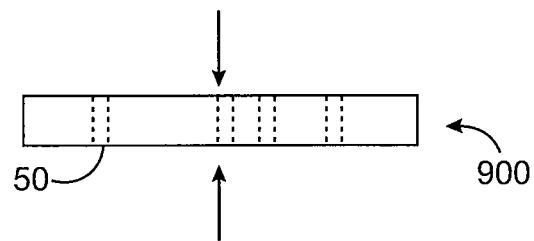


FIG. 14C

+

+

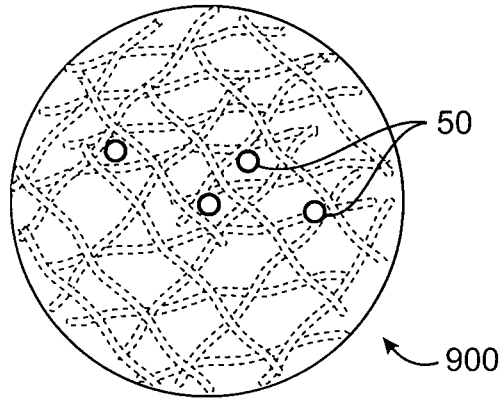


FIG. 15A



FIG. 15B

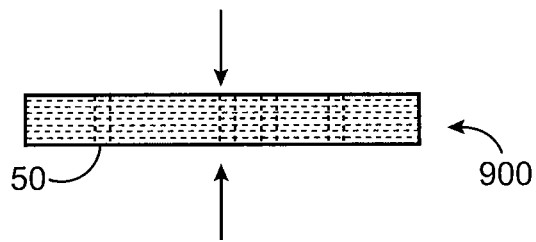


FIG. 15C

+

专利名称(译)	可互换的高强度聚焦超声换能器		
公开(公告)号	EP2131744A2	公开(公告)日	2009-12-16
申请号	EP2008744340	申请日	2008-03-25
申请(专利权)人(译)	MEDICIS科技股份有限公司		
当前申请(专利权)人(译)	LIPOSONIX INC.		
[标]发明人	CRUNKILTON JEFFREY ROBERT		
发明人	CRUNKILTON, JEFFREY, ROBERT		
IPC分类号	A61B8/14 A61N7/02 A61B17/00		
CPC分类号	A61N7/02 A61B2017/0046 A61B2017/00477		
优先权	60/976867 2007-10-02 US 60/908074 2007-03-26 US		
其他公开文献	EP2131744A4		
外部链接	Espacenet		

摘要(译)

一种可互换的换能器，用于具有无键适配器并且能够在潮湿环境中操作的超声医疗系统。可互换换能器具有用于接合医疗系统的适配器，超声换能器和附加电子器件，以提供独立的插入件，以便于在各种医疗应用中更换和使用。还公开了一种滑环间隔件，该滑环间隔件与薄饼滑环一起使用，该薄饼滑动环具有基部和凸缘构造，以在薄饼滑动环的每个接触环周围形成一个或多个通道。这些通道在每个连接器周围提供流体隔离，以帮助减少滑环的连接器垫之间的电子串扰和接触腐蚀，同时滑环浸没在潮湿环境中。