


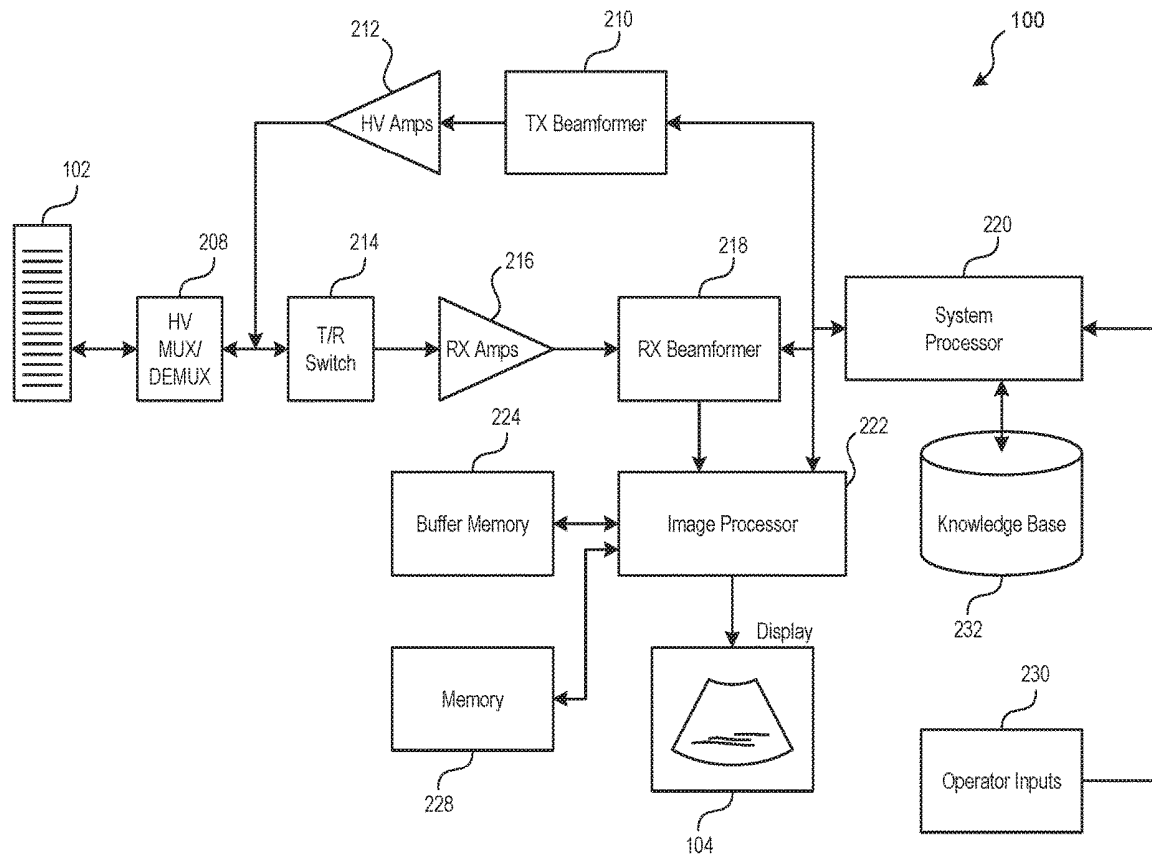

US 20190380676A1

(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2019/0380676 A1**
(43) **Pub. Date: Dec. 19, 2019**(54) **ULTRASOUND IMAGING SYSTEM WITH
AUTOMATIC IMAGE SAVING**(71) Applicant: **FUJIFILM SonoSite, Inc.**, Bothell,
WA (US)(72) Inventors: **Wendy Swan**, Lake Forest Park, WA
(US); **Daniel Shelton**, Prosper, TX
(US); **Somnath Banik**, Bothell, WA
(US)(21) Appl. No.: **16/012,627**(22) Filed: **Jun. 19, 2018****Publication Classification**(51) **Int. Cl.**
A61B 8/08 (2006.01)
G01S 15/89 (2006.01)
G01S 7/52 (2006.01)
A61B 8/00 (2006.01)
G16H 30/20 (2006.01)
G06N 99/00 (2006.01)(52) **U.S. Cl.**
CPC **A61B 8/0841** (2013.01); **G01S 15/8911**
(2013.01); **G01S 7/52085** (2013.01); **G01S**
7/52053 (2013.01); **G06T 7/0016** (2013.01);
A61B 8/5276 (2013.01); **A61B 8/463**
(2013.01); **G16H 30/20** (2018.01); **G06N**
99/005 (2013.01); **G01S 7/5202** (2013.01)(57) **ABSTRACT**

Ultrasound imaging systems for automatically identifying and saving ultrasound images relevant to a needle injection procedure, and associated systems and methods, are described herein. For example, an ultrasound imaging system includes a transducer for transmitting/receiving ultrasound signals during a needle injection procedure, and receive circuitry configured to convert the received ultrasound signals into ultrasound image data. The image data can be stored in a buffer memory. A processor can analyze the image data stored in the buffer memory to identify image data that depicts a specified injection event of the needle injection procedure, and the identified image data can be stored in a memory for archival purposes.



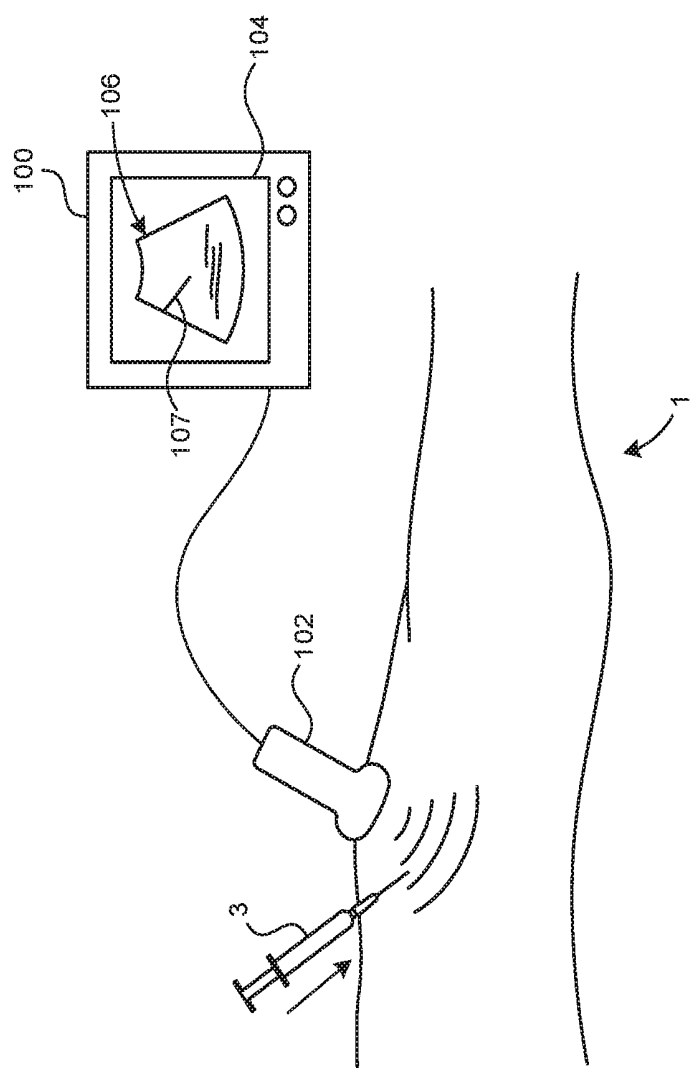


FIG. 1

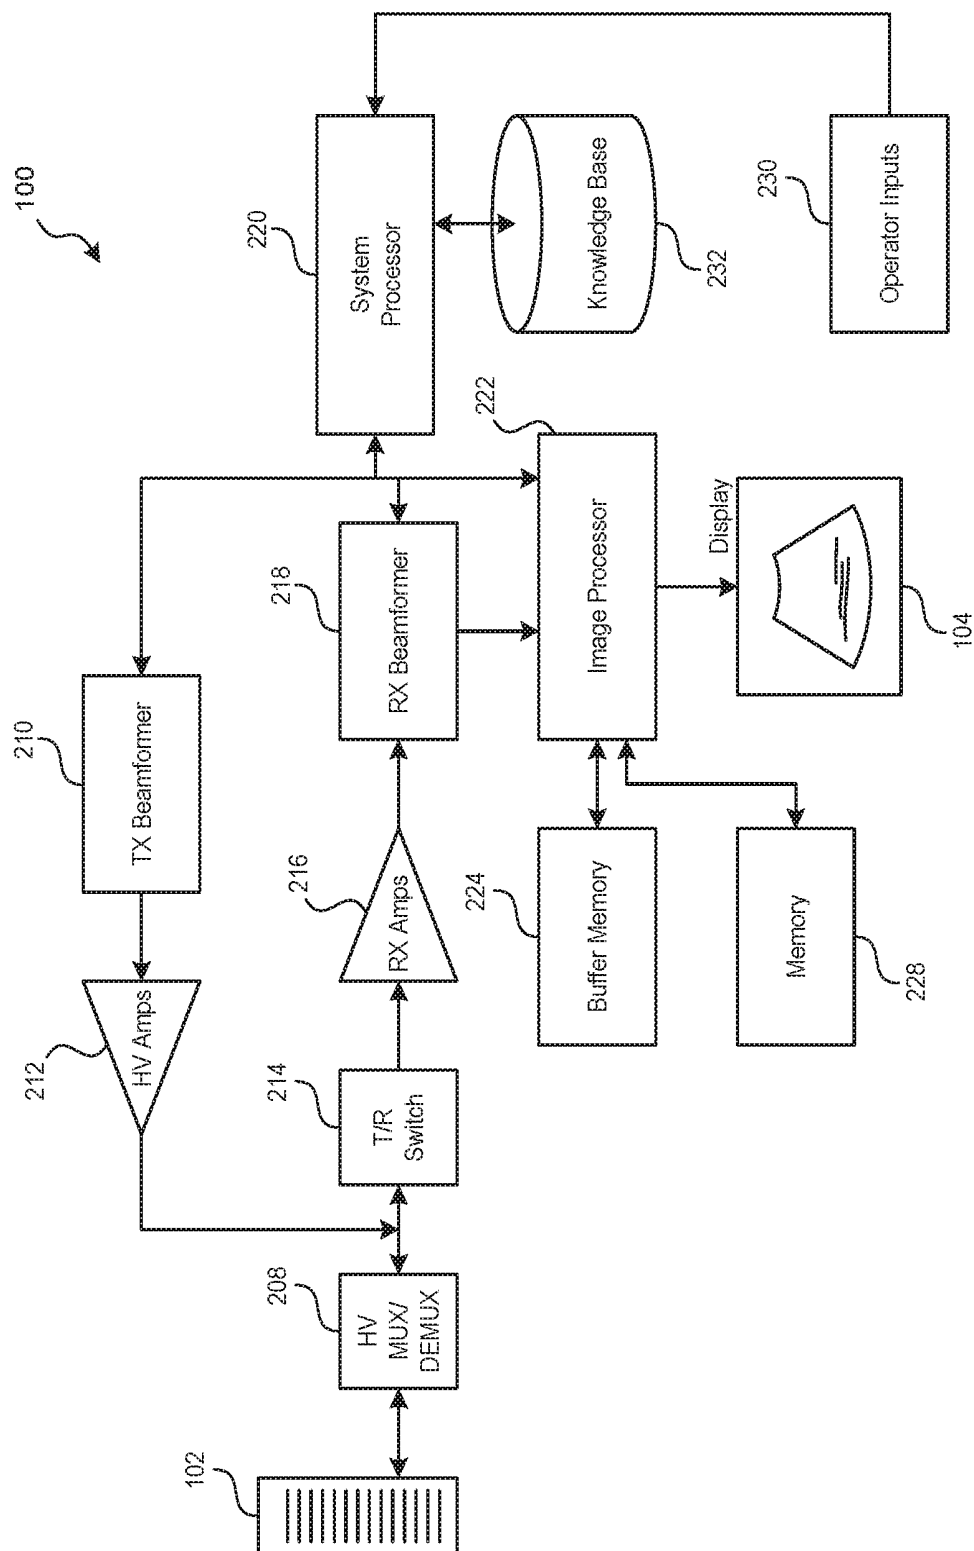
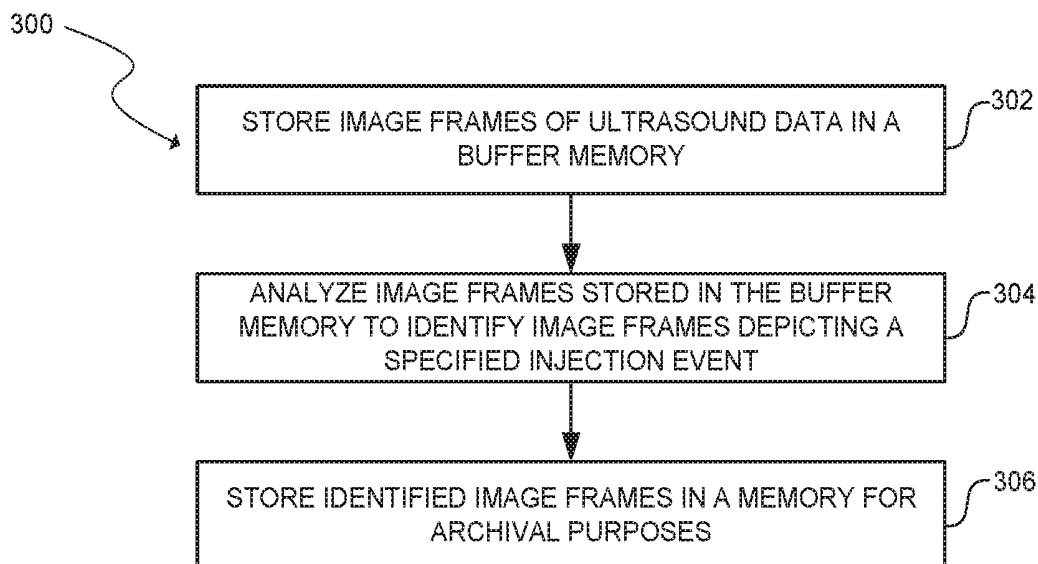
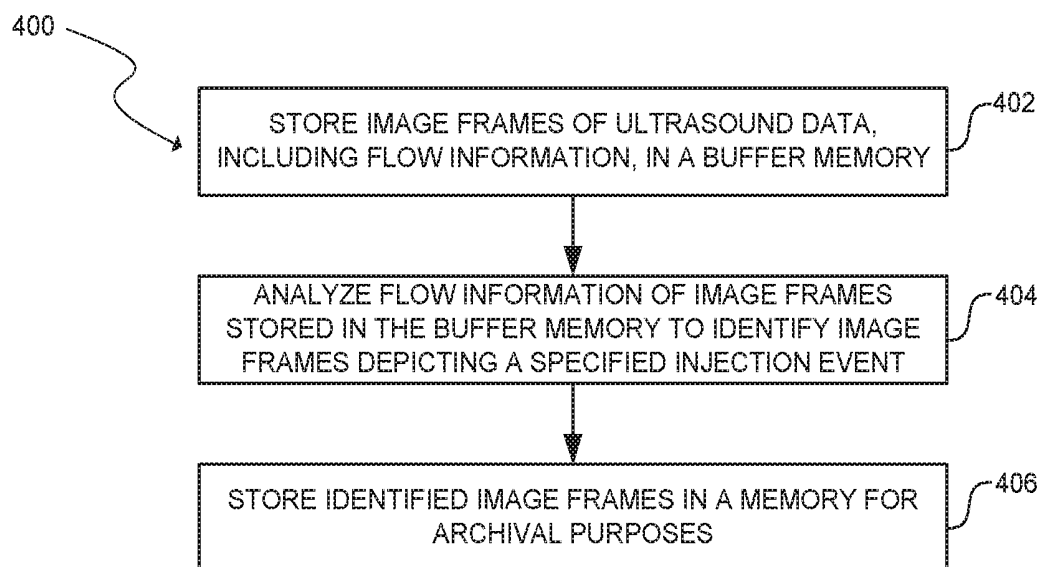


FIG. 2

**FIG. 3****FIG. 4**

ULTRASOUND IMAGING SYSTEM WITH AUTOMATIC IMAGE SAVING

TECHNICAL FIELD

[0001] The disclosed technology relates to ultrasound imaging systems, and in particular to systems for improving workflow within clinical settings using ultrasound imaging systems.

BACKGROUND

[0002] In ultrasound imaging, an operator of a system uses a transducer probe to obtain ultrasound images of a patient during an examination. The images captured by the system may be viewed, printed, and/or included in a patient report for diagnosis and record keeping. In addition, select images may be included in a written and/or electronic report that is used to bill the patient or their insurance for the services rendered. Depending on the examination procedure being performed, the number and subject of the images required in a report of the examination may be standardized or defined. For example, a needle injection procedure, such as an ultrasound-guided regional anesthesia injection, may require an image of the needle at a target location, an image of the needle during the injection, etc.

[0003] In a typical single operator examination, a physician or an ultrasound technician uses the imaging system to obtain all the images needed to complete the examination. However, during some needle procedures, where the care provider cannot stop mid procedure or has no free hands to control the system, a second person may assist in controlling the system settings and collecting the needed images during the procedure. The obtained images are typically stored in a buffer memory and must be reviewed after the examination is complete to mark or otherwise identify images to be used in creating a record of the examination. Often, clinicians collect a loop of images (“clip”) and review the loop after the examination is complete to select images to be used in creating a record of the examination. This additional step requires extra time. If single images are collected instead of a loop, it can be difficult for the operator to know at the time of the procedure whether the required images of the examination have been captured.

BRIEF DESCRIPTION OF THE DRAWINGS

[0004] FIG. 1 is a simplified illustration of an ultrasound imaging system in accordance with an embodiment of the present technology.

[0005] FIG. 2 is a block diagram of the ultrasound imaging system shown in FIG. 1 in accordance with an embodiment of the present technology.

[0006] FIG. 3 is a flow diagram of a method or process of identifying image frames stored in a buffer memory that depict an injection event in accordance with an embodiment of the present technology.

[0007] FIG. 4 is a flow diagram of a method or process of identifying image frames stored in a buffer memory that depict an injection event in accordance with another embodiment of the present technology.

DETAILED DESCRIPTION

[0008] Specific details of several embodiments of ultrasound systems for automatically saving ultrasound images generated during an ultrasound imaging procedure using an

interventional device, and associated devices and methods, are described below reference to FIGS. 1-4. In some embodiments, for example, an ultrasound imaging system includes a transducer configured to transmit ultrasound signals to and receive ultrasound signals from a region of interest during an ultrasound-guided needle injection procedure. The ultrasound imaging system further includes receive circuitry configured to convert the received ultrasound signals into image frames of ultrasound data, and a buffer memory in which the image frames are stored. The ultrasound imaging system also includes a processor configured to analyze the image frames stored in the buffer memory and identify and mark one or more of the image frames that depict an event of the needle injection procedure—for example, the delivery of a fluid from the needle used during the procedure. In some embodiments, the processor can further be configured to save the image frames depicting the injection event in a memory—other than the buffer memory—for archival purposes.

[0009] Although many of the embodiments described below are described with respect to devices, systems, and methods for automatically saving an ultrasound image during a needle injection procedure in which a needle is used to deliver anesthesia or other drugs to a desired location, other applications and other embodiments in addition to those described herein are within the scope of the present technology. For example, at least some embodiments of the present technology may be useful for procedures employing other invasive medical instruments. It should be noted that other embodiments in addition to those disclosed herein are within the scope of the present technology.

[0010] Further, embodiments of the present technology can have different configurations, components, and/or procedures than those shown or described herein. Moreover, a person of ordinary skill in the art will understand that embodiments of the present technology can have configurations, components, and/or procedures in addition to those shown or described herein and that these and other embodiments can be without several of the configurations, components, and/or procedures shown or described herein without deviating from the present technology. The phrases “in some embodiments,” “according to some embodiments,” “in certain embodiments,” “in the illustrated embodiment,” “in other embodiments,” and the like generally mean the particular feature, structure, or characteristic following the phrase is included in at least one implementation of the present technology, and may be included in more than one implementation. In addition, such phrases do not necessarily refer to the same embodiments or different embodiments.

[0011] The terminology used below is to be interpreted in its broadest reasonable manner, even though it is being used in conjunction with a detailed description of certain examples of embodiments of the technology. Indeed, certain terms may even be emphasized below; however, any terminology intended to be interpreted in any restricted manner will be overtly and specifically defined as such in this Detailed Description section.

[0012] FIG. 1 shows a representative ultrasound imaging system 100 (“system 100”) that implements the present technology for imaging the tissue of a subject or patient 1. In one embodiment, the system 100 can be a hand-held, portable or cart-based system that uses a transducer probe 102 to transmit ultrasound signals into a region of interest and to receive the corresponding echo signals in order to

produce an image of the tissue being scanned. The transducer probe **102** can be a one or two dimensional linear or curved transducer, a phased array transducer, or another type of ultrasound transducer as is well known in the art. The system **100** converts characteristics of the received echo signals (e.g., their amplitude, phase, power, frequency shift, etc.) into data that is quantified and displayed for the user as an image on a video monitor, screen, or other display **104** (“display **104**”). As described in detail below, the images created may also be stored electronically for digital record keeping or transmitted via a wired or wireless communication link to another device or location.

[0013] In some embodiments, the system **100** can be used during a needle injection procedure in which an operator of the system **100** guides an interventional instrument such as a needle **3** into the patient **1** with one hand while holding the transducer probe **102** with the other hand. In certain embodiments, the operator can view a composite image **106** of the tissue and a representation **107** of where the needle **3** is located in the tissue. The composite image **106** can be updated on the display **104** while the needle **3** is guided to a target location within the patient **1**. The target location may be a particular nerve site (e.g., when the needle injection procedure is a regional anesthesia procedure) or other area of interest such as a vessel or a particular organ (e.g., uterus, prostate, tumor, heart vessel etc.). In some embodiments, both the needle **3** and an injectate (e.g., a drug) delivered via the needle **3** can be seen in the composite image **106**. For example, if the injection is made in a place with low resistance (e.g., appearing dark in the composite image **106**), the injectate can fill the space such that characteristic fluid motion is visible in the composite image **106**. In some embodiments, a material removed by the needle **3** (e.g., during a biopsy procedure) can be seen in the composite image **106**.

[0014] FIG. 2 is a simplified block diagram of the system **100** configured in accordance with an embodiment of the present technology. As will be appreciated by those skilled in the art, the system **100** may be constructed with components that are different than those shown in FIG. 2. In addition, the system **100** can include components that are not discussed (e.g., a power supply, etc.) and that are not necessary for the understanding of how to make and use the present technology.

[0015] In the illustrated embodiment, the transducer probe **102** is connected to a high voltage multiplexer/de-multiplexer (HV mux/demux) **208** that is used select individual or groups of transducer elements in the transducer probe **102**. Signals to be transmitted by the transducer probe **102** are generated by a transmit (TX) beamformer **210** that adjusts the timing of the signals in order to direct the signals in a particular direction and to focus the signals at a particular depth in the tissue. Alternatively, unfocused (plane) waves can be transmitted by the transducer probe **102**. Signals from the TX beamformer **210** are amplified by one or more high-voltage amplifiers (HV amps) **212** before being applied to the HV mux/demux **208** and the transducer probe **102**. In other embodiments, however, signals from the TX beamformer **210** can be passed to the transducer probe **102** directly without an intervening multiplexer/demultiplexer.

[0016] A transmit/receive (T/R) switch **214** operates to disconnect the receive electronics of the system **100** from the transducer probe **102** when the higher powered transmit pulses are being transmitted. The T/R switch **214** is closed

when the system **100** is to detect the returning echo signals. Signals received by the T/R switch **214** are amplified by low-noise receive amplifiers (RX amps) **216** that implement a gain function that typically varies according to the depth from which the echo signals originate. Where the system **100** is a directional ultrasound system, the outputs of the RX amps **216** feed a receive (RX) beamformer **218** that delays and sums the amplified received echo signals. In some embodiments, the analog received signals are converted to corresponding digital signals, after amplification, with a number of analog to digital converters (not shown) that are positioned in the signal path between the RX amps **216** and the RX beamformer **218**.

[0017] In some embodiments, a system processor **220**, which can be implemented as one or more programmed microprocessors, is configured to execute program instructions that are stored in an internal or external computer readable memory (not shown) to control the operation of the system **100**. As further illustrated in FIG. 2, beamformed ultrasound signals produced by the RX beamformer **218** are delivered to an image processor **222**. The image processor **222**, which may include one or more general purpose microprocessors (including the system processor **220**), one or more digital signal processors (DSP), one or more graphics processor units (GPU), application-specific integrated circuits (ASIC) or the like, converts the raw, beamformed signals into a two-dimensional image frame of pixel data that can be stored in memory and shown to the operator on the display **104**.

[0018] The image frames produced by the image processor **222** are stored in a buffer memory **224** (also known as a cine buffer), which in one embodiment is operated as a circular buffer of memory elements that stores a select number of image frames as they are produced during an ultrasound imaging procedure using the system **100**. The image frames can be captured using either a retrospective or prospective capture mode, as is known in the art. In one embodiment, the buffer memory **224** can store 2-5 minutes of data or 3600-9000 image frames of ultrasound data or more. In one embodiment, once the buffer memory **224** is full, the oldest image frame stored in the buffer memory **224** is overwritten with a new image frame in a circular fashion. In the illustrated embodiment, a memory **228** is used to store the image frames for archival purposes. The contents of the memory **228** may be transferred to a remote patient records keeping system after an imaging procedure is complete. In some embodiments, at least some of the image frames that are stored in the memory **228** are compressed to save space and therefore may lack some detail compared with the image frames that are stored in the buffer memory **224**. In some embodiments, image data other than image frames (e.g., raw image data, pre-conversion image data, etc.) can be stored in the buffer memory **224**.

[0019] In the illustrated embodiment, the system **100** includes a number of operator inputs **230** such as keys, buttons, knobs, a microphone to receive voice commands, a camera to capture gestures, or software-configured controls, such as touch screen controls or the like. The operator inputs **230** allow an operator to change the operating characteristics of the system **100** and to input commands to the system processor **220**.

[0020] In some embodiments, the operator begins an ultrasound imaging procedure (e.g., an examination) by using the operator inputs **230** to select a procedure type from a number

of pre-defined procedure types that are shown on the display **104** or that may have a dedicated control on a keyboard or other input device of the system **100**. For example, the imaging procedure could be a regional anesthesia injection or other ultrasound-guided needle injection procedure. Each procedure type may be associated with particular views and/or measurements that are to be captured by the operator during the specific procedure. For example, some needle injection procedures may require an image of the needle at the target region with the patient, an image of the needle during injection of a drug or other injectate, etc. For example, a nerve block procedure may require that three or more different image frames be recorded including views of (i) a needle approaching a target nerve, (ii) the needle at the position of the target nerve, and (iii) anesthetic being delivered around the target nerve. Such views may be required to be stored (e.g., archived) by the medical facility or operator for insurance billing purposes. In the illustrated embodiment, the views and/or measurements required by the various procedure types are stored in a knowledge base **232** (e.g., a memory, database, etc.) that is accessible to the system processor **220**. In some embodiments, the knowledge base **232** can further store one or more parameters, image frames, or other data from previous examinations that can be, for example, compared to the image frames stored in the buffer memory **224** as described in detail below.

[0021] After selecting a particular imaging procedure, the operator can use one or more of the operator inputs **230** (e.g., an on-screen button, footswitch, control on an imaging probe, etc.) to begin capturing ultrasound image frames using the system **100**. These image frames are produced and stored in the buffer memory **224** until the operator uses one or more of the operator inputs **230** to halt the image capture process. In some embodiments, the image capture process can be halted based on other criteria such as, for example, a timer, an electrocardiogram signal, etc. As will be appreciated, the buffer memory **224** can be constructed to store several thousand image frames of ultrasound data.

[0022] In the past, using conventional ultrasound systems, the operator was required to take the time to review/search through all of the stored image frames to select which frames would be included in a patient's record and/or submitted for billing purposes. Moreover, the review/search for relevant images was conducted after the imaging procedure concluded—meaning it was not possible for the operator to know with certainty during a needle injection procedure whether they captured the required views (e.g., for billing purposes). In some other conventional ultrasound systems, the operator could press a button on an ultrasound probe or use a voice control during a procedure to print or save particular images—for example, those taken at approximately the time of an injection. While such systems may reduce the amount of review required by the operator to identify relevant image frames, buttons may be pressed accidentally, and voice controls may be accidentally activated in noisy environments. Furthermore, it is often cumbersome for the operator to conduct a needle injection procedure while simultaneously triggering an ultrasound system to save certain images during the procedure.

[0023] In contrast to conventional systems, the system **100** of the present technology is configured to automatically identify (e.g., select, determine, etc.) and save image frames that are relevant to, or required, by a needle injection procedure—for example, those image frames depicting a

particular event, trigger, or aspect of the needle injection procedure (referred to herein as an “injection event”). For example, the system **100** can be configured to automatically identify image frames that depict a specified injection event such as a needle being positioned at or approaching a target location, an injection taking place, etc. Specifically, the system processor **220**, the image processor **222**, and/or another suitable processor such as a DSP or a GPU can execute a number of programmed instructions to analyze the image frames that are stored in the buffer memory **224** and identify one or more of the image frames that likely depict the specified injection event. In other embodiments, image data other than image frames (e.g., pre-conversion image data) can be analyzed to identify portions of the image data that depict or relate to the specified injection event.

[0024] The identified image frames can be saved to the memory **228** for archival or other purposes. In some embodiments, the identified image frames are stored in the memory **228** with lossless compression or with little or no compression compared to the unselected image frames generated during the examination in order to retain more image detail. In certain embodiments, the identified image frames are marked for inclusion in, or automatically entered into, a patient report of an examination. In some embodiments, the system **100** can generate an indication (e.g., a sound, display, etc.) to provide real-time or near-real-time feedback to the operator that image frames showing the specified injection event were successfully captured.

[0025] The system processor **220** (or another processor) can automatically identify image frames stored in the buffer memory **224** that likely depict a specified injection event in a number of different manners. FIG. 3, for example, is a flow diagram of a process or method **300** performed by one or more of the processors in the system **100** for identifying image frames that depict an injection event using frame-to-frame comparison in accordance with embodiments of the present technology. Beginning at block **302**, the method **300** includes generating ultrasound signals and receiving the corresponding echo signals for a needle injection procedure and storing image frames of ultrasound data about the procedure in the buffer memory **224**, as described in detail above. At block **304**, the method includes comparing and/or analyzing image frames stored in the buffer memory **224** to identify the image frames that depict the specified injection event. In some embodiments, for example, the system processor **220** correlates and/or compares the image frames stored in the buffer memory **224** to detect changes between the image frames such as those caused by motion of a needle and/or the fluid injected from the needle.

[0026] For example, the system processor **220** can use well-known image processing methods to estimate and characterize the point correspondence from one image frame to the next in the vicinity of the needle. For example, the system processor **220** can estimate the correspondence (or motion) of each point of interest by maximizing a figure of merit for the match between a patch of one image frame centered about the point in question with a sliding window in the next image frame for each image frame stored in the buffer memory **224**. That is, the system processor **220** can estimate flow vectors for each or a subset of pixels between two or more image frames. Potential figures of merit include 2D correlation, mutual information, or structural similarity. In some embodiments, regularization or pre-processing may be applied to assist in (e.g., lower the processing costs of)

estimating the correspondence of each point of interest. In other embodiments, optical flow methods such as the Lucas—Kanade or Horn-Schunck may be employed to establish the point correspondences (e.g., flow vectors). In either case, the flow vector properties can be classified to indicate the needle and/or injectate.

[0027] Regardless of the specific image processing method(s) employed, the system processor **220** can identify that certain image frames stored in the buffer memory **224** likely depict the specified injection event based on the estimated optical flow/motion between the image frames. In some embodiments, for example, the system processor **220** can determine that the needle is stationary or generally stationary in certain image frames and thus that the needle is positioned at the target location and/or that an injection is occurring in those image frames. Similarly, a detection of fluid motion around the needle tip in certain image frames can indicate that the injection is depicted in those frames.

[0028] In other embodiments, the system processor **220** may execute instructions that implement a trained neural network or a machine learning algorithm to analyze/compare image frames stored in the buffer memory **224** in order to identify the image frames that depict the specified injection event. The machine learning algorithm can be an artificial neural network or deep learning algorithm that is trained to recognize motion indicative of the injection event in the image frames (e.g., the swirl or expansion of the fluid of the injection around the tip of the needle). In some embodiments, for example, a neural network can be used to detect the injection event based on the differences between image frames in the buffer memory **224** (e.g., based on a time series of image frames). In some embodiments, the machine learning algorithm can be trained based one or more image frames that were generated and saved in one or more previous examinations and that are similar to the image frames required to be saved in the current examination. These previous images can be stored in, for example, the knowledge base **232**. Based on the previous images, the machine learning algorithm can determine the image frames in the buffer memory **224** that, for example, bear the closest resemblance to the previous images and thus likely depict the injection event. In this manner, the system processor **220** can identify the image frames that likely depict the injection event based on the historical data/examples from previous examinations.

[0029] In certain embodiments, the system processor **220** can further mark or identify a particular region (e.g., a sub-region) in one or more of the image frames that likely depicts the injection. For example, the system processor **220** could automatically determine a bounding box around the likely region of injection based on classification of flow vectors calculated or determined for the image frame(s).

[0030] In some embodiments, the system processor **220** can be configured to analyze only a portion (e.g., a specific region) of the image frames and/or a subset of the total number of image frames in order to detect the specified injection event. For example, the system processor **220** can be configured to analyze only a portion (e.g., a region) of the image frames that is proximate to a determined location of the needle. Likewise, the system processor **220** could employ different levels or types of imaging processing methods on different subsets of the image frames stored in the buffer memory **224**. For example, the system processor could analyze the image frames stored in the buffer memory

224 until detecting that the needle has stopped moving, and then analyze subsequently generated/stored image frames to detect those image frames that depict the fluid from the injection around the needle. Such embodiments can advantageously reduce the processing burden of the system **100** by localizing some of the imaging processing steps to a subset of the image frames stored in the buffer memory **224**.

[0031] At block **306**, the method **300** includes automatically storing the image frames identified as depicting the injection event in a memory for archival purposes (e.g., for inclusion in a patient report, billing record, or other report). For example, the image frames can be stored in the memory **228** and/or in a different memory accessible to the system processor **220**. In some embodiments, the identified image frames can be marked or flagged in the buffer memory **224** in addition to or instead of being stored in a memory for archival purposes.

[0032] In some embodiments, the system processor **220** can automatically identify image frames stored in the buffer memory **224** in other manners (e.g., other than by a frame-to-frame comparison). FIG. **4**, for example, is a flow diagram of a process or method **400** performed by one or more of the processors in the system **100** for identifying image frames that depict an injection event based on flow information in the image frames, in accordance with embodiments of the present technology. Beginning at block **402**, the method **400** includes generating ultrasound signals and receiving the corresponding echo signals for a needle injection procedure and storing image frames of ultrasound data about the procedure in the buffer memory **224**, as described in detail above. More specifically, in some embodiments, the system **100** can be operated in a Doppler Mode or another color flow imaging mode that generally correlates multiple ultrasound signal pulses into a single image frame that contains motion or flow information (often displayed in color), as is known in the art. In some embodiments, the color flow imaging need not employ the entire color flow processing chain—instead segmentation and classification of a subset of the signals (e.g., lag-0 correlations, lag-1 correlations, etc.) can be used to produce the flow information. At block **304**, the system processor **220** can proceed to analyze the flow information of the image frames stored in the buffer memory **224** to identify those image frames depicting the specified injection event.

[0033] In some embodiments, the method **400** requires a relatively greater amount of front-end processing by the processor(s) than the method **300** illustrated in FIG. **3**, because multiple ultrasound signals pulses are used to generate each image frame. Accordingly, the frame rate of the system **100** can be slower when performing the method **400** as compared to the method **300**. In certain embodiments, to improve the frame rate of the system **100** while performing the method **400**, the system **100** can be configured to capture flow information (e.g., to generate, detect, and correlate multiple ultrasound signal pulses) for only a portion or region of each image frame. In some embodiments, for example, the system **100** can determine a bounding box (e.g., a virtual color box) or other region in which to search for the specified injection event that is smaller than the entire image frame. For example, the system processor **220** can execute instructions that implement an image classification algorithm (e.g., a detection, trained neural network, or machine learning algorithm) to detect the location of the needle (e.g., by detecting a bright reflector, either

stationary or moving) and/or the location of the needle tip (e.g., by detecting a transition from a bright reflector). The system processor **200** can then specify a small region around the needle in which to search for an injection of fluid from the needle by generating flow information for the small region. In some embodiments, the detected location of the needle in one image frame can be used to expedite the search for the needle in another image frame (e.g., a subsequent image frame). That is, once the needle is detected in one image frame, the entirety of each subsequent image frame does not need to be classified from there forward in time. Finally, at block **406**, the method **400** includes automatically storing the image frames identified as depicting the injection event in a memory for archival purposes, or otherwise marking or flagging the image frames in the buffer memory **224**.

[0034] In general, the system **100** can automatically identify image frames stored in the buffer memory **224** that likely depict the specified injection event using any of frame-to-frame image processing, image processing using trained neural networks or machine learning algorithms, optical flow (e.g., classification of flow vectors that indicate the cessation of movement of a needle structure and/or the swirling or expanding of a flow pattern of injectate), color flow imaging, or combinations thereof. For example, simple frame-to-frame comparison methods could be used to detect motion of the needle between image frames, and specifically to detect that motion of the needle has stopped. A trained neural network or machine learning algorithm could then be employed to detect the needle tip in subsequently generated image frames. Finally, a region around the identified needle tip could be interrogated using color flow imaging to detect the injection of fluid from the needle tip. In this manner, the system **100** can automatically accurately identify image frames depicting the specified injection event while reducing the processing requirements of the system **100** compared to, for example, generating flow information for each full image frame produced during a procedure.

[0035] In some embodiments, the system **100** is configured to analyze the image frames stored in the buffer memory **224** in real-time or near-real-time as they are generated and added to the buffer memory **224**. In such embodiments, after identifying that one or more of the image frames depicts the specified injection event, the system **100** can be configured to generate a notification or indication that at least one of the image frames depicts the injection event. In some embodiments, for example, the system processor **220** can cause a notification to be displayed on the display **226** or a sound to be played via a speaker of the system **100**. Accordingly, the system **100** can advantageously provide feedback alerting the operator of the system **100**—during the examination—that the necessary image frames were captured. In other embodiments, image frames from an entire ultrasound procedure can be accessed and analyzed after the procedure is concluded to automatically determine and save image frames depicting the specified injection event.

[0036] In some embodiments, the image frames are associated with meta-data (e.g., narrative information) about the image frame. The meta-data may include the type of tissue being imaged and one or more parameters of the system **100** used to obtain the image. Such parameters can include the operating mode of the ultrasound machine (B-mode, Doppler Mode, Power mode, etc.) as well as power settings, pulse repetition rate, focal depth, probe used, likelihood of

needle presence/motion, etc. In some embodiments, the system processor **220** can insert one or more of the identified image frames into a patient record (e.g., PACS system, knowledge repository, etc.), patient chart, or other record, while also inserting (e.g., pre-populating) the corresponding operating parameters of the ultrasound machine that were used to obtain the image frame and/or other meta-data so that the operator does not have to enter them manually.

[0037] Embodiments of the subject matter and the operations described in this specification can be implemented in digital electronic circuitry, or in computer software, firmware, or hardware, including the structures disclosed in this specification and their structural equivalents, or in combinations of one or more of them. Embodiments of the subject matter described in this specification can be implemented as one or more computer programs, i.e., one or more modules of computer program instructions, encoded on computer storage medium for execution by, or to control the operation of, data processing apparatus.

[0038] A computer storage medium can be, or can be included in, a computer-readable storage device, a computer-readable storage substrate, a random or serial access memory array or device, or a combination of one or more of them. Moreover, while a computer storage medium is not a propagated signal, a computer storage medium can be a source or destination of computer program instructions encoded in an artificially-generated propagated signal. The computer storage medium also can be, or can be included in, one or more separate physical components or media (e.g., multiple CDs, disks, or other storage devices). The operations described in this specification can be implemented as operations performed by a data processing apparatus on data stored on one or more computer-readable storage devices or received from other sources.

[0039] The term “processor” encompasses all kinds of apparatus, devices, and machines for processing data, including by way of example a programmable processor, a computer, a system on a chip, or multiple ones, or combinations, of the foregoing. The apparatus can include special purpose logic circuitry, e.g., an FPGA (field programmable gate array) or an ASIC (application-specific integrated circuit). The apparatus also can include, in addition to hardware, code that creates an execution environment for the computer program in question, e.g., code that constitutes processor firmware, a protocol stack, a database management system, an operating system, a cross-platform runtime environment, a virtual machine, or a combination of one or more of them. The apparatus and execution environment can realize various different computing model infrastructures, such as web services, distributed computing and grid computing infrastructures.

[0040] A computer program (also known as a program, software, software application, script, or code) can be written in any form of programming language, including compiled or interpreted languages, declarative or procedural languages, and it can be deployed in any form, including as a stand-alone program or as a module, component, subroutine, object, or other unit suitable for use in a computing environment. A computer program may, but need not, correspond to a file in a file system. A program can be stored in a portion of a file that holds other programs or data (e.g., one or more scripts stored in a markup language document), in a single file dedicated to the program in question, or in multiple coordinated files (e.g., files that store one or more

modules, sub-programs, or portions of code). A computer program can be deployed to be executed on one computer or on multiple computers that are located at one site or distributed across multiple sites and interconnected by a communication network.

[0041] The processes and logic flows described in this specification can be performed by one or more programmable processors executing one or more computer programs to perform actions by operating on input data and generating output. The processes and logic flows can also be performed by, and apparatus can also be implemented as, special purpose logic circuitry, e.g., an FPGA (field programmable gate array) or an ASIC (application-specific integrated circuit).

[0042] Processors suitable for the execution of a computer program include, by way of example, both general and special purpose microprocessors, and any one or more processors of any kind of digital computer. Generally, a processor will receive instructions and data from a read-only memory or a random access memory or both. The essential elements of a computer are a processor for performing actions in accordance with instructions and one or more memory devices for storing instructions and data. Generally, a computer will also include, or be operatively coupled to receive data from or transfer data to, or both, one or more mass storage devices for storing data, e.g., magnetic, magneto-optical disks, or optical disks. Devices suitable for storing computer program instructions and data include all forms of non-volatile memory, media and memory devices, including by way of example semiconductor memory devices, e.g., EPROM, EEPROM, and flash memory devices; magnetic disks, e.g., internal hard disks or removable disks; magneto-optical disks; and CD-ROM and DVD-ROM disks. The processor and the memory can be supplemented by, or incorporated in, special purpose logic circuitry.

[0043] To provide for interaction with a user, embodiments of the subject matter described in this specification can be implemented on an imaging system having a display device, e.g., an LCD (liquid crystal display), LED (light emitting diode), or OLED (organic light emitting diode) monitor, for displaying information to the operator and a keyboard and a pointing device, e.g., a mouse or a trackball, by which the operator can provide input to the computer. In some implementations, a touch screen can be used to display information and to receive input from a user. Other kinds of devices can be used to provide for interaction with an operator as well; for example, feedback provided to the operator can be any form of sensory feedback, e.g., visual feedback, auditory feedback, or tactile feedback; and input from the operator can be received in any form, including acoustic, speech, or tactile input. In addition, a computer can interact with an operator by sending documents to and receiving documents from a device that is used by the user; for example, by sending web pages to a web browser on a user's client device in response to requests received from the web browser.

[0044] From the foregoing, it will be appreciated that specific embodiments of the technology have been described herein for purposes of illustration, but that various modifications may be made without deviating from the disclosure. Accordingly, the invention is not limited except as by the appended claims. Furthermore, certain aspects of the new technology described in the context of particular embodi-

ments may also be combined or eliminated in other embodiments. Moreover, although advantages associated with certain embodiments of the new technology have been described in the context of those embodiments, other embodiments may also exhibit such advantages and not all embodiments need necessarily exhibit such advantages to fall within the scope of the technology. Accordingly, the disclosure and associated technology can encompass other embodiments not expressly shown or described herein.

I/We claim:

1. An ultrasound imaging system, comprising:
 - a transducer configured to transmit ultrasound signals to and receive ultrasound signals from a region of interest during a needle injection procedure;
 - receive circuitry configured to convert the received ultrasound signals into ultrasound image data;
 - a buffer memory in which the image data is stored; and
 - a processor configured to identify image data that depicts a specified injection event of the needle injection procedure.
2. The ultrasound imaging system of claim 1, further comprising a memory, wherein the processor is configured to save the image data that depicts the specified injection event in the memory.
3. The ultrasound imaging system of claim 1, further comprising a display for displaying the image data as image frames, wherein the processor is configured to produce a notification on the display that at least one of the image frames depicts the specified injection event.
4. The ultrasound imaging system of claim 1 wherein the processor is configured to include the image data that depicts the specified injection event in a patient record.
5. The ultrasound imaging system of claim 1 wherein the processor is configured to identify the image data that depicts the specified injection event by analyzing the image data in the buffer memory using a machine learning algorithm to detect motion of at least one of a needle, a fluid delivered by the needle, and a material removed by the needle.
6. The ultrasound imaging system of claim 1 wherein the specified injection event is at least one of a needle being positioned at a target location within the region of interest and the needle approaching the target location within the region of interest, and wherein the processor is configured to identify the image data that depicts the specified injection event by analyzing the image data stored in the buffer memory to detect motion of the needle.
7. The ultrasound imaging system of claim 1 further comprising a display for displaying the image data as image frames, wherein the processor is configured to identify and mark a region of at least one of the image frames that likely depicts the specified injection event.
8. The ultrasound imaging system of claim 1 wherein the specified injection event is an injection taking place within the region of interest.
9. The ultrasound imaging system of claim 8 wherein the processor is configured to identify the image data that depicts the injection taking place by analyzing the image data stored in the buffer memory to detect motion of an injectate.
10. The ultrasound imaging system of claim 1 wherein—
 - the transducer is configured to transmit the ultrasound signals in two or more pulses,

the receive circuitry is configured to correlate the received ultrasound signals into image data including flow information, and

the processor is configured to analyze the flow information to identify the image data that depicts the specified injection event.

11. An ultrasound system for imaging a region of interest of a subject during a needle injection into the region of interest, comprising:

a transducer configured to transmit ultrasound signals to and receive ultrasound signals from the region of interest;

receive circuitry configured to convert the received ultrasound signals into image frames of ultrasound data;

a buffer configured to store the image frames; and

a processor configured to execute instructions to cause the processor to—

identify at least one image frame from the plurality of image frames stored in the cine buffer that depicts a needle injection; and

store the at least one identified image frame that depicts the needle injection in a memory for archival purposes.

12. The ultrasound system of claim **11** wherein the processor is configured to execute the instructions to identify the at least one image frame that depicts the needle injection by analyzing the image frames stored in the buffer to detect that a needle used for the needle injection is generally stationary.

13. The ultrasound system of claim **11** wherein the processor is configured to execute the instructions to identify the at least one image frame that depicts the needle injection by analyzing the image frames stored in the buffer to detect a fluid around a needle used for the needle injection.

14. The ultrasound system of claim **11** wherein the processor is configured to execute the instructions to identify

the at least one image frame that depicts the needle injection by comparing the image frames stored in the buffer to detect motion of at least one of a needle used for the needle injection and a fluid from the needle.

15. The ultrasound system of claim **11** wherein the processor is configured to execute the instructions to identify the at least one image frame depicting the needle injection by analyzing flow information associated with the image frames stored in the buffer.

16. A method performed by a processor in an ultrasound system, the method comprising:

receiving ultrasound signals from a region of interest during a needle injection procedure;

converting the received ultrasound signals into image frames of ultrasound data;

storing the image frames in a buffer memory;

identifying one or more of the image frames that depict an injection event of the needle injection procedure; and

saving the image frames that depict the injection event.

17. The method of claim **16**, further comprising inserting at least one of the image frames that depict the injection event into a patient chart.

18. The method of claim **16** wherein identifying the image frames that depict the injection event includes using a machine learning to compare the image frames stored in the buffer memory to detect a change between two or more of the image frames.

19. The method of claim **16** wherein the injection event is the delivery of an injectate to the region of interest, and wherein identifying the image frames that depict the delivery of the injectate includes analyzing flow information in the image frames to detect motion of the injectate.

20. The method of claim **16**, further comprising providing an indication to an operator that at least one of the image frames depicts the injection event.

* * * * *

专利名称(译)	具有自动图像保存功能的超声成像系统		
公开(公告)号	US20190380676A1	公开(公告)日	2019-12-19
申请号	US16/012627	申请日	2018-06-19
[标]申请(专利权)人(译)	富士胶片索诺声公司		
申请(专利权)人(译)	FUJIFILM SONOSITE , INC.		
当前申请(专利权)人(译)	FUJIFILM SONOSITE , INC.		
[标]发明人	SWAN WENDY SHELTON DANIEL BANIK SOMNATH		
发明人	SWAN, WENDY SHELTON, DANIEL BANIK, SOMNATH		
IPC分类号	A61B8/08 G01S15/89 G01S7/52 A61B8/00 G16H30/20 G06N99/00		
CPC分类号	G16H30/20 G06T2207/10132 A61B8/463 A61B8/0841 G01S15/8911 G01S7/52053 G06N20/00 A61B2560/0475 G06T7/0016 G01S7/52085 G06T2207/20081 G06T7/20 A61B8/5276 G01S7/5202 A61B8/488 A61B8/5292 G01S7/52036 G06N3/08 G06T7/246 G06T2207/20084 G06T2207/30004 G16H10/60 G16H20/40 G16H30/40 G16H50/20		
外部链接	Espacenet USPTO		

摘要(译)

本文描述了用于自动识别和保存与针头注射过程有关的超声图像的超声成像系统以及相关的系统和方法。例如，超声成像系统包括：换能器，用于在针头注射过程期间发送/接收超声信号；以及接收电路，被配置为将接收到的超声信号转换成超声图像数据。图像数据可以存储在缓冲存储器中。处理器可以分析存储在缓冲存储器中的图像数据，以识别描述针头注射过程的指定注射事件的图像数据，并且可以将所识别的图像数据存储在存储器中以用于存档。

