


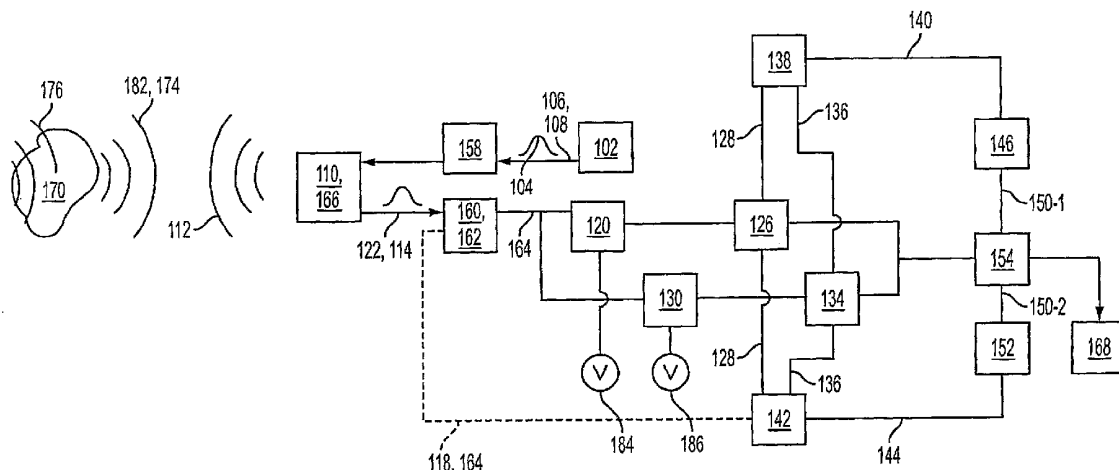

US 20120053460A1

(19) **United States**(12) **Patent Application Publication**  
**Blalock et al.**(10) **Pub. No.: US 2012/0053460 A1**  
(43) **Pub. Date: Mar. 1, 2012**(54) **ULTRASOUND IMAGING BEAM-FORMER  
APPARATUS AND METHOD**filed on Jan. 14, 2003, provisional application No.  
60/440,262, filed on Jan. 15, 2003.(75) Inventors: **Travis N. Blalock**, Charlottesville,  
VA (US); **William F. Walker**,  
Barboursville, VA (US); **John A.**  
**Hossack**, Charlottesville, VA (US)**Publication Classification**(51) **Int. Cl.**  
**A61B 8/14** (2006.01)  
(52) **U.S. Cl.** ..... **600/440; 600/472; 600/443**(73) Assignee: **The University of Virginia Patent  
Foundation**, Charlottesville, VA  
(US)(57) **ABSTRACT**(21) Appl. No.: **13/210,890**(22) Filed: **Aug. 16, 2011****Related U.S. Application Data**(63) Continuation of application No. 11/160,915, filed on  
Jul. 14, 2005, now abandoned, which is a continuation  
of application No. PCT/US04/00887, filed on Jan. 14,  
2004.(60) Provisional application No. 60/440,020, filed on Jan.  
14, 2003, provisional application No. 60/439,990,

In some illustrative embodiments, an incoming signal from a transducer in an ultrasound imaging beam-former apparatus is applied to an in-phase sample-and-hold and a quadrature sample-and-hold. The quadrature sample-and-hold may be clocked a quarter period behind the in-phase sample-and-hold. The output of the sample-and-holds are applied to in-phase and quadrature analog-to-digital converters. A magnitude calculator receives the in-phase and quadrature digital values, and outputs a magnitude. A phase calculator receives the in-phase and quadrature digital values, and outputs a phase. An apodizer applies a difference between an amplitude of the outgoing signal and the magnitude and applies a first illumination to a image point in substantial proportion to the difference, and a phase rotator applies a second illumination to the image point in substantial proportion to the phase.



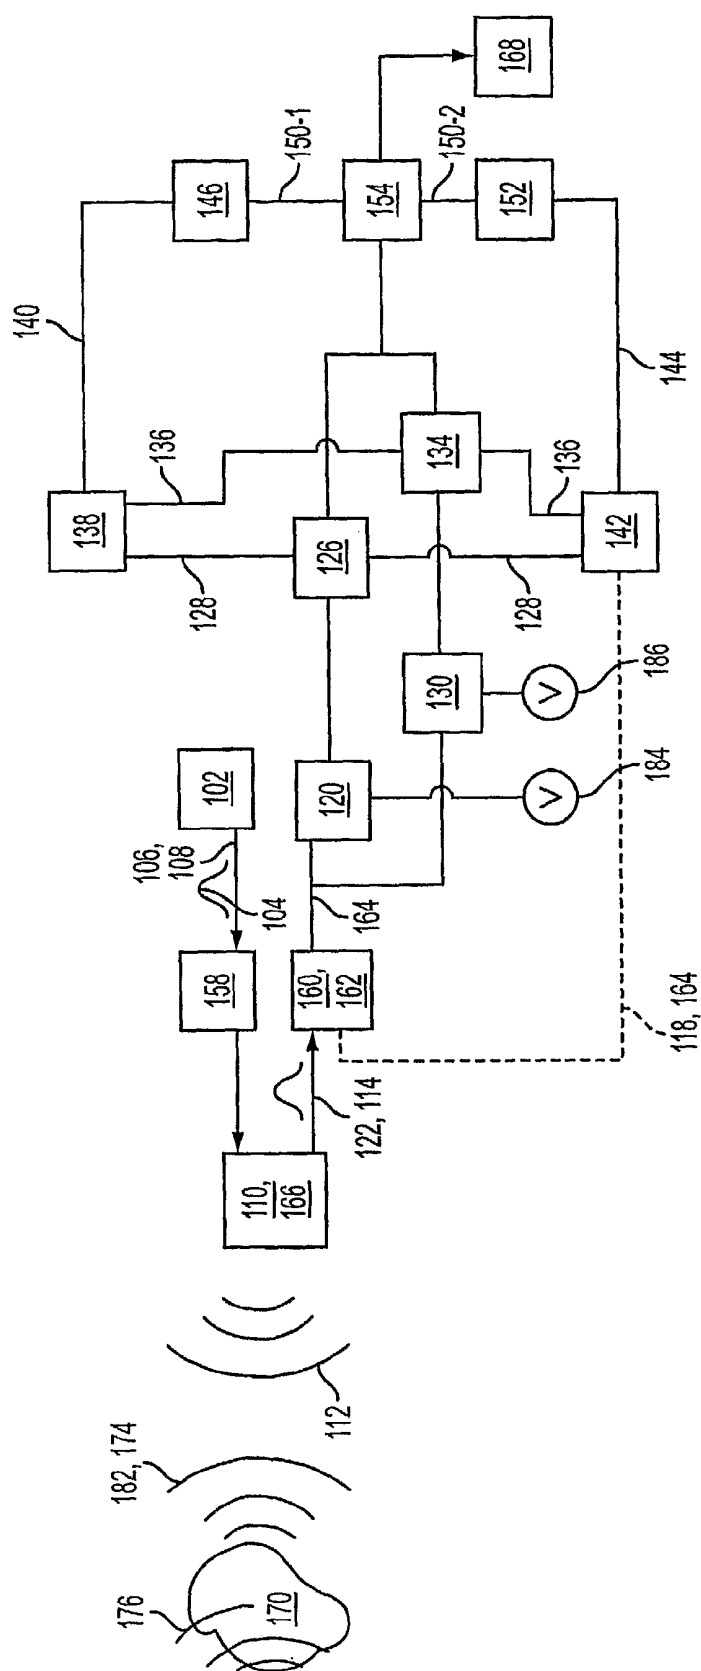


FIG. 1

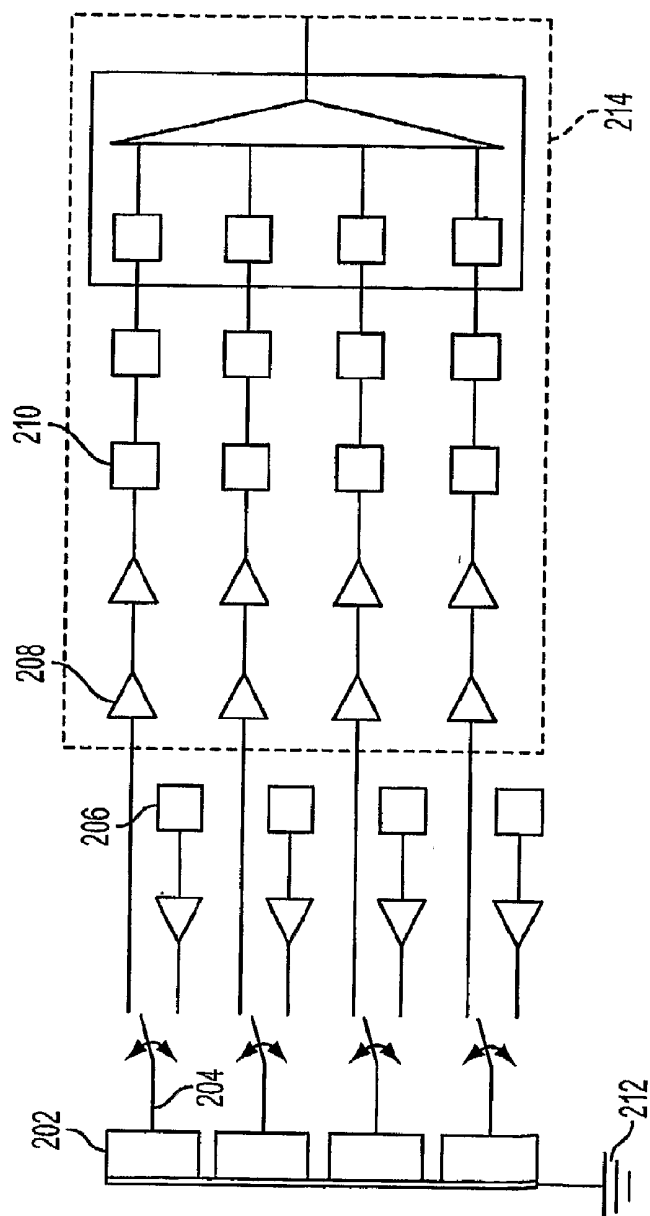


FIG. 2

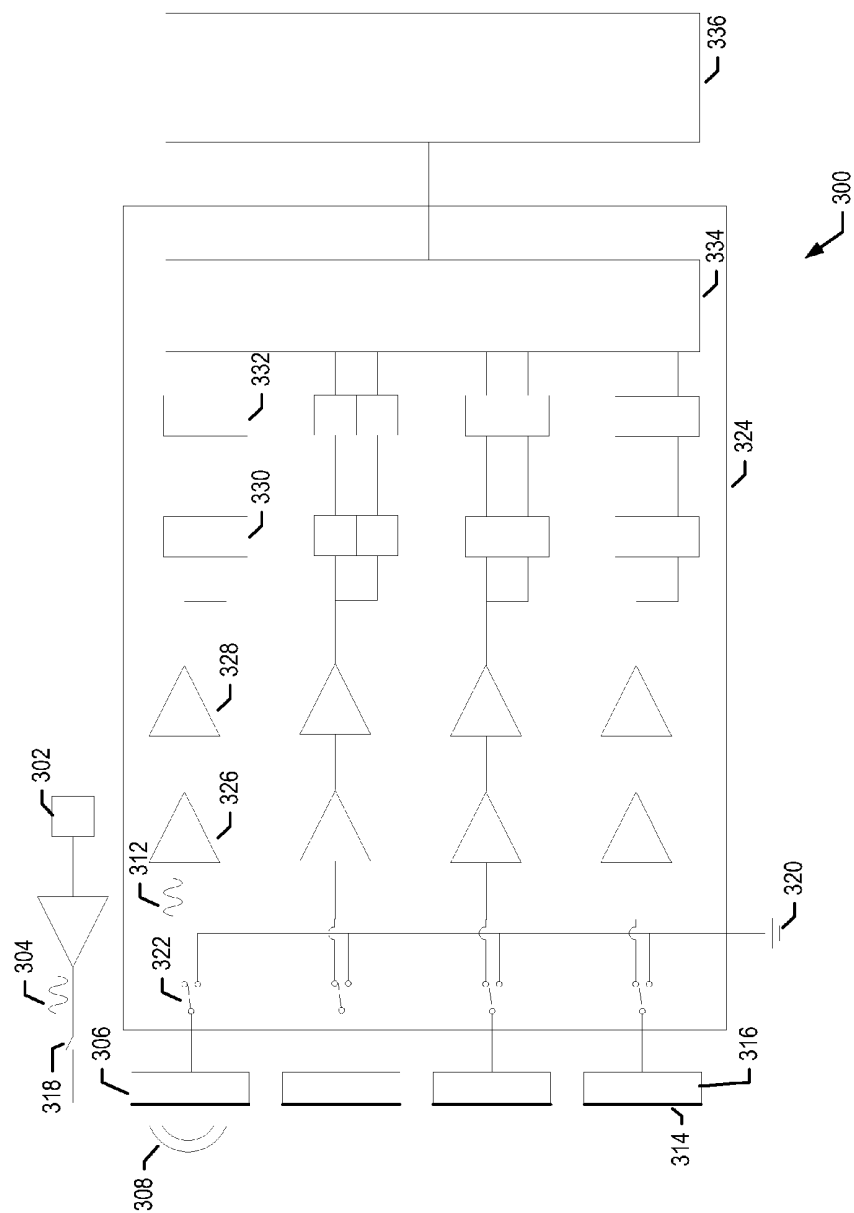


FIG. 3



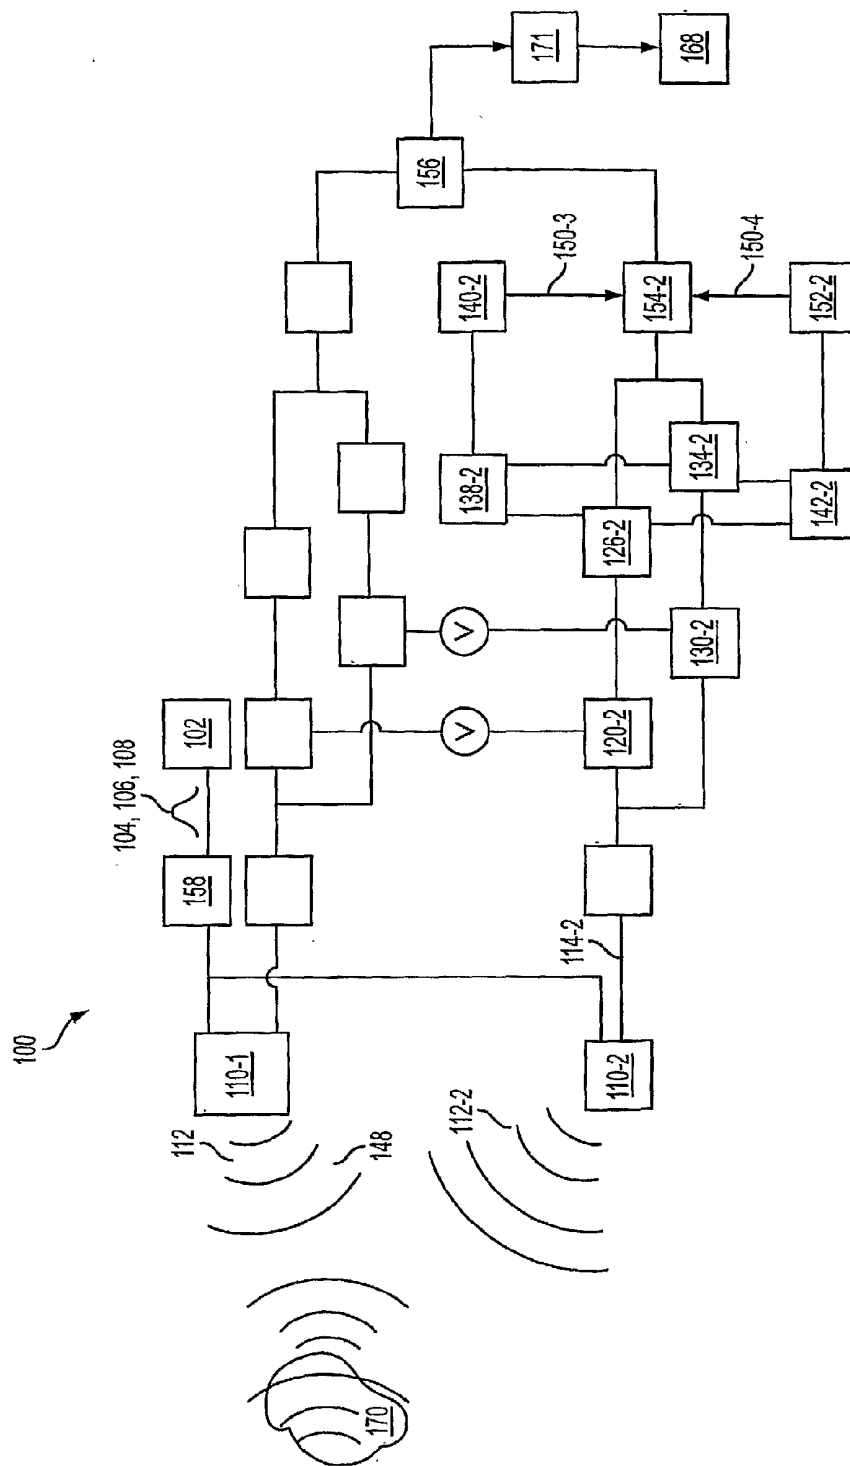


FIG. 4

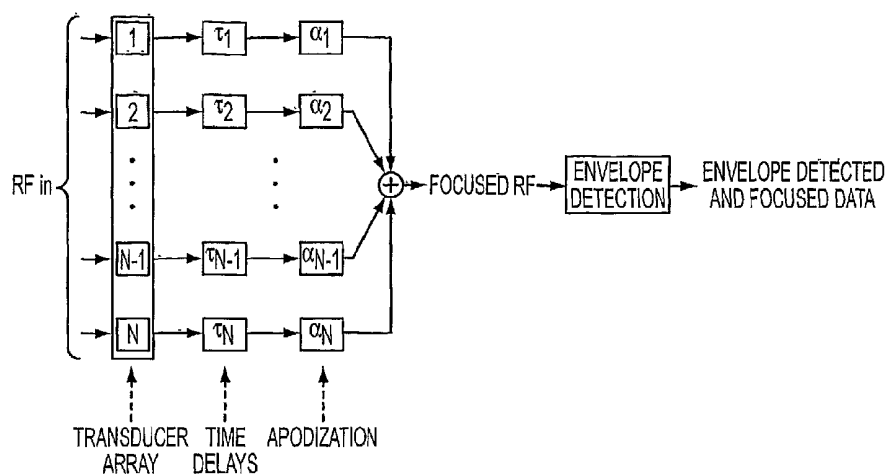

CONVENTIONAL ART  
FIG. 5A

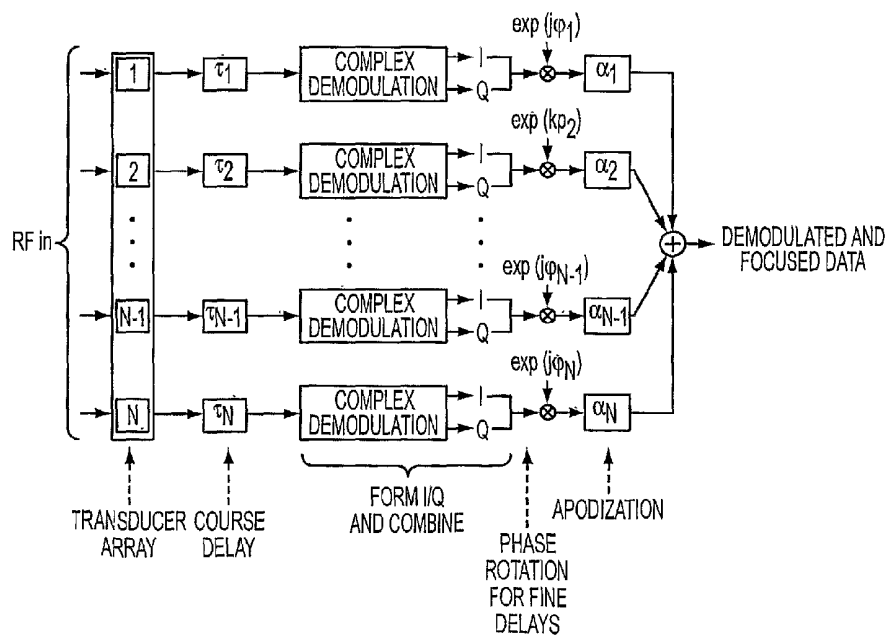

CONVENTIONAL ART  
FIG. 5B

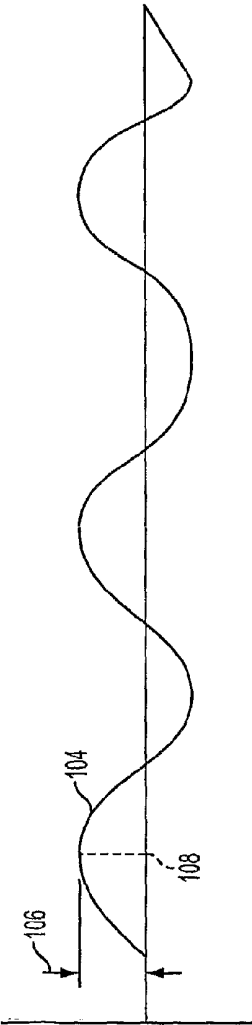


FIG. 6A

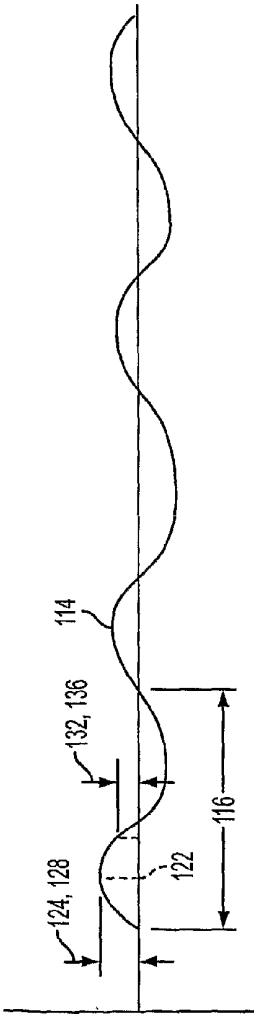


FIG. 6B

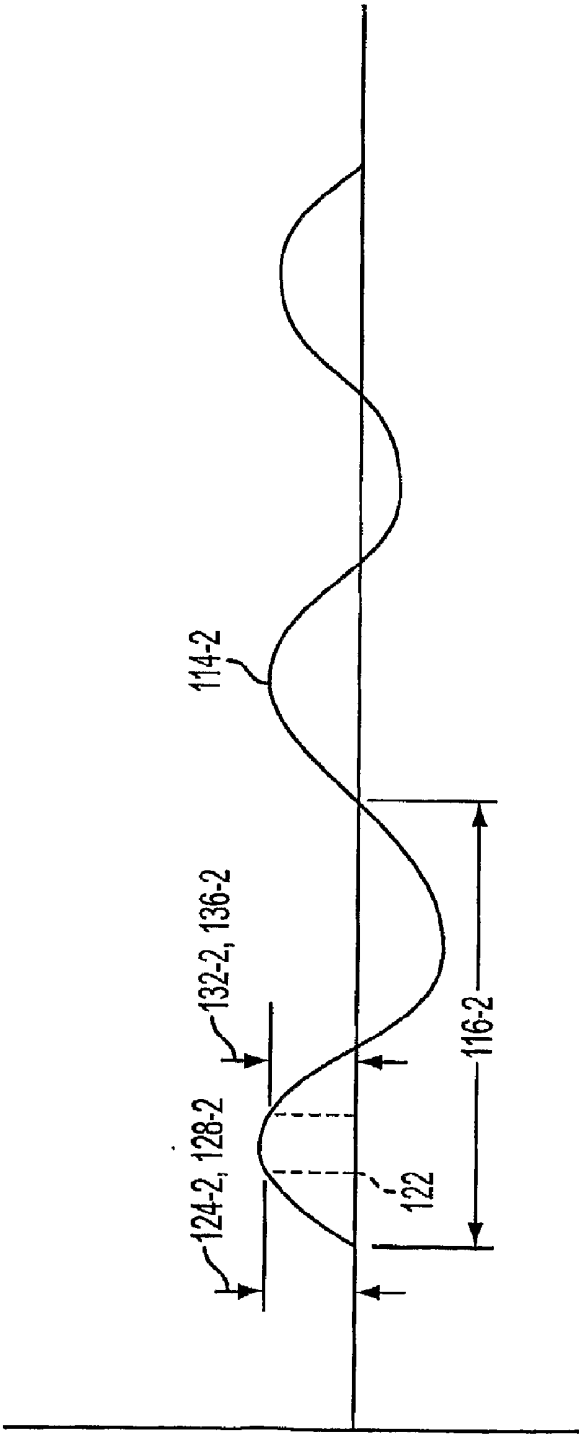


FIG. 6C



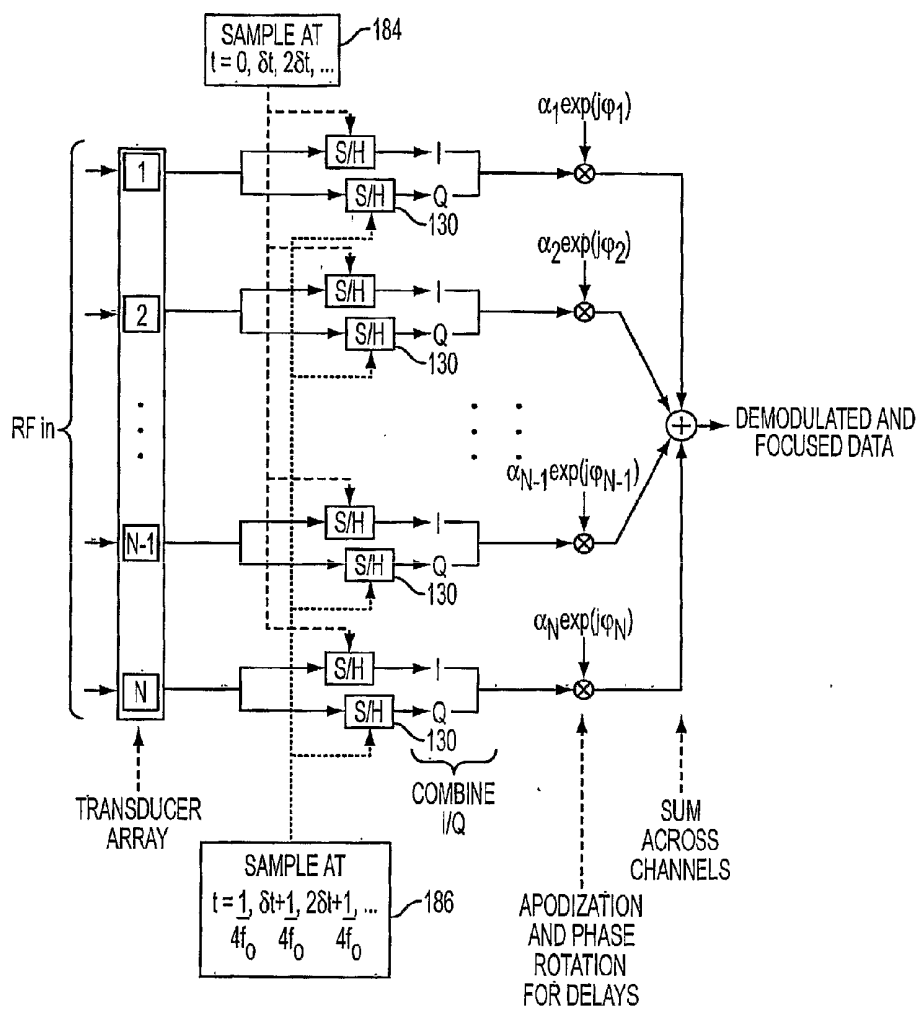


FIG. 7

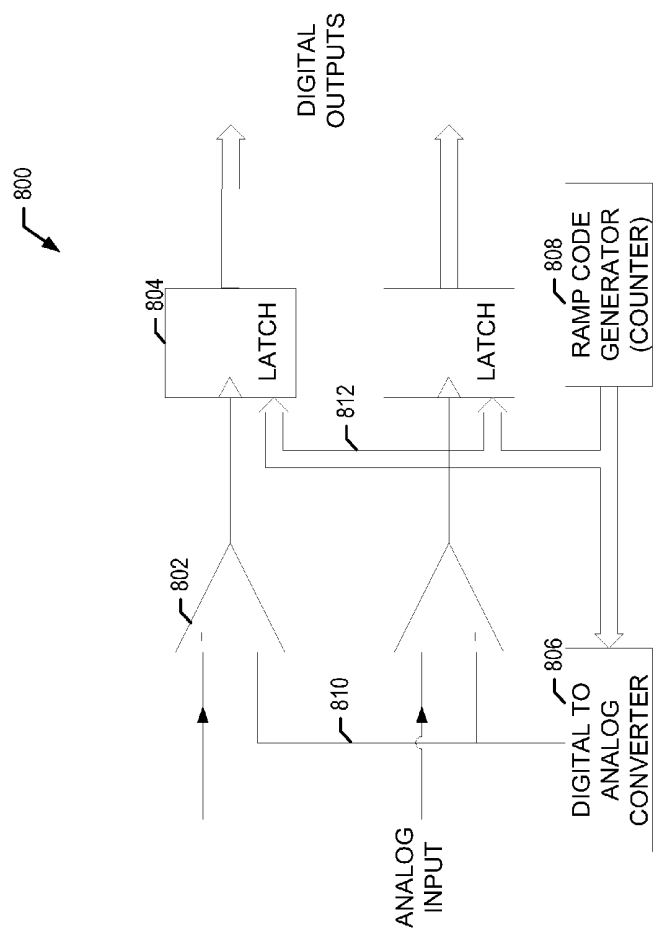


FIG. 8

## ULTRASOUND IMAGING BEAM-FORMER APPARATUS AND METHOD

### CROSS-REFERENCE TO RELATED APPLICATIONS

**[0001]** The present application is National Stage filing under 35 U.S.C. 371 of International Applications No. PCT/US2004/000887 which claims priority to U.S. Provisional Application Ser. Nos. 60/440,020 filed on Jan. 14, 2003, 60/439,990 filed on Jan. 14, 2003, and 60/440,262 filed on Jan. 15, 2003 the entire disclosures of which are incorporated herein by reference.

### BACKGROUND

**[0002]** 1. Field of the Invention

**[0003]** The present invention relates to ultrasonic diagnostic imaging systems and methods. More specifically, the preferred embodiments relate to a device and method for ultrasound imaging beam-forming that may be incorporated in a substantially integrated hand-held ultrasonic diagnostic imaging instrument.

**[0004]** 2. Introduction

**[0005]** Medical imaging is a field dominated by high cost systems that may be so complex as to require specialized technicians for operation and the services of experienced medical doctors and nurses for image interpretation. Medical ultrasound, which is considered a low cost modality, utilizes imaging systems costing as much as \$250K. These systems may be operated by technicians with two years of training or specialized physicians. This high-tech, high-cost approach works very well for critical diagnostic procedures. However it makes ultrasound impractical for many of the routine tasks for which it would be clinically useful.

**[0006]** A number of companies have attempted to develop low cost, easy to use systems for more routine use. The most notable effort is that by Sonosite. Their system produces very high quality images at a system cost of approximately \$20,000. While far less expensive than high-end systems, these systems are still very sophisticated and require a well-trained operator. Furthermore, at this price few new applications may be opened.

**[0007]** Many ultrasonic imaging systems utilize an array transducer that is connected to beamformer circuitry through a cable, and a display that is usually connected directly to or integrated with the beam-former. This approach is attractive because it allows the beamformer electronics to be as large as is needed to produce an economical system. In addition, the display may be of a very high quality.

**[0008]** Some conventional system architectures have been improved upon through reductions in beam-former size. One of the most notable efforts has been undertaken by Advanced Technologies Laboratories and then continued by a spin-off company, Sonosite. U.S. Pat. No. 6,135,961 to Pflugrath et al., entitled "Ultrasonic Signal Processor for a Hand Held Ultrasonic Diagnostic Instrument," hereby incorporated by reference herein in its entirety, describes some of the signal processing employed to produce a highly portable ultrasonic imaging system. The Pflugrath '961 patent makes reference to an earlier patent, U.S. Pat. No. 5,817,024 to Ogle et al., entitled, "Hand Held Ultrasonic Diagnostic instrument with Digital Beamformer," hereby incorporated by reference herein in its entirety. In U.S. Pat. No. 6,203,498 to Bunce et al., entitled "Ultrasonic Imaging Device with Integral Dis-

play," hereby incorporated by reference herein in its entirety, however, the transducer, beamformer, and display may be all integrated to produce a very small and convenient imaging system.

**[0009]** Other references of peripheral interest are U.S. Pat. No. 6,669,641 to Poland, et al., entitled "Method of and system for ultrasound imaging," which describes an ultrasonic apparatus and method in which a volumetric region of the body is imaged by biplane images. One biplane image has a fixed planar orientation to the transducer, and the plane of the other biplane image can be varied in relation to the fixed reference image.

**[0010]** U.S. Pat. No. 6,491,634 to Leavitt, et al., entitled "Sub-beam-forming apparatus and method for a portable ultrasound imaging," describes a sub-beam-forming method and apparatus that is applied to a portable, one-dimensional ultrasonic imaging system. The sub-beam-forming circuitry may be included in the probes assembly housing the ultrasonic transducer, thus minimizing the number of signals that are communicated between the probe assembly and the portable processor included in the imaging system.

**[0011]** U.S. Pat. No. 6,380,766 to Savord, entitled "Integrated circuitry for use with transducer elements in an imaging system," describes integrated circuitry for use with an ultrasound transducer of an ultrasound imaging system.

**[0012]** U.S. Pat. No. 6,013,032 to Savord, entitled "Beam-forming methods and apparatus for three-dimensional ultrasound imaging using two-dimensional transducer array," describes an ultrasound imaging system including a two-dimensional array of ultrasound transducer elements that define multiple sub-arrays, a transmitter for transmitting ultrasound energy into a region of interest with transmit elements of the array, a sub-array processor and a phase shift network associated with each of the sub-arrays, a primary beam-former and an image generating circuit.

**[0013]** U.S. Pat. No. 6,126,602 to Savord, et al., entitled "Phased array acoustic systems with intra-group processors," describes an ultrasound imaging apparatus and method that uses a transducer array with a very large number of transducer elements or a transducer array with many more transducer elements than beam-former channels.

**[0014]** U.S. Pat. No. 5,997,479 to Savord, et al., entitled "Phased array acoustic systems with intra-group processors," describes an ultrasound imaging apparatus and method that uses a transducer array with a very large number of transducer elements or a transducer array with many more transducer elements than beam-former channels.

**[0015]** U.S. Pat. No. 6,582,372 to Poland, entitled "Ultrasound system for the production of 3-D images," describes an ultrasound system that utilizes a probe in conjunction with little or no specialized 3-D software/hardware to produce images having depth cues.

**[0016]** U.S. Pat. No. 6,179,780 to Hossack, et al., entitled "Method and apparatus for medical diagnostic ultrasound real-time 3-D transmitting and imaging," describes a medical diagnostic ultrasound real-time 3-D transmitting and imaging system that generates multiple transmit beam sets using a 2-D transducer array.

**[0017]** U.S. Pat. No. 6,641,534 to Smith, et al., entitled "Methods and devices for ultrasound scanning by moving sub-apertures of cylindrical ultrasound transducer arrays in two dimensions," describes methods of scanning using a two dimensional (2-D) ultrasound transducer array.

[0018] U.S. Pat. No. 4,949,310 to Smith, et al., entitled "Maltese cross processor: a high speed compound acoustic imaging system," describes an electronic signal processing device which forms a compound image for any pulse-echo ultrasound imaging system using a two-dimensional array transducer.

[0019] U.S. Pat. No. 6,276,211 to Smith, entitled "Methods and systems for selective processing of transmit ultrasound beams to display views of selected slices of a volume," describes the selection of a configuration of slices of a volume, such as B slices, I slices, and/or C slices.

[0020] Commercial ultrasound systems have been limited to one-dimensional (1-D) or linear transducer arrays until fairly recently. A typical number of transducers in such an array may be 128. Providing separate multiplex and receive circuitry is manageable with this many transducers, albeit with significant use of expensive high-voltage switches. Newer arrays, however, may be likely to be two-dimensional (2-D) or square arrays. The number of transducers in a two-dimensional array may range up to  $128 \times 128$  or 16,384, and is often in the thousands. Maintaining separate receive, transmit, and multiplex partitioning for the transducers in such an array creates a tremendous burden in terms of cost, space, and complexity. The power consumption and heat dissipation of thousands high-voltage multiplexers is enough to discourage the use of two-dimensional arrays in portable ultrasound imaging systems.

[0021] Current beam-forming strategies can be broadly classified into the two approaches depicted in FIG. 5. One approach is to use digital time delays to focus the data, as illustrated in 5 (a). Geometric delays are calculated and applied to the digitized data on each channel. In such beam-formers, the data needs to either be sampled at a very high sampling rate or interpolated. Implementation of time delays requires sufficient memory to hold a few hundred samples per channel to implement an adequate delay envelope, constraining system complexity.

[0022] In the second approach, systems combine time delays with complex phase rotation, as depicted in 5 (b). Coarse focusing is implemented by delaying the digitized data on each channel. Fine focusing is accomplished by phase rotation of data that has undergone complex demodulation at the center frequency. Such systems require circuitry to perform complex demodulation on every channel. Time delay beam-forming requires significant fast memory to implement a reasonable delay envelope.

[0023] Conventional approaches to generating I/Q data may also include analog/digital baseband demodulation, or use a Hilbert transform. Using a demodulation based approach to generate I/Q data may necessitate significant extra circuitry on each channel, while use of the Hilbert transform may require a significant amount of memory to hold the raw RF data.

[0024] Accordingly, existing ultrasound systems with thousands of separate transmit and receive switches may be too expensive for many applications. While a variety of systems and methods may be known, there remains a need for improved systems and methods.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0025] The preferred embodiments of the present invention are shown by a way of example, and not limitation, in the accompanying figures, in which:

[0026] FIG. 1 is a schematic diagram of an ultrasound imaging beam-forming apparatus according to a first embodiment of the invention;

[0027] FIG. 2 is a schematic diagram of a protection circuit for use with an embodiment of the invention;

[0028] FIG. 3 is a schematic diagram of a protection circuit for use with an embodiment of the invention;

[0029] FIG. 4 is a schematic diagram of an ultrasound imaging beam-forming apparatus according to a second embodiment of the invention;

[0030] FIG. 5 is a schematic diagram of a conventional ultrasound imaging beam-forming apparatus;

[0031] FIG. 6 are graphs of signals for use with an embodiment of the invention; and

[0032] FIG. 7 is a schematic diagram of a signal receiver for use with an embodiment of the invention.

#### SUMMARY OF THE INVENTION

[0033] The present invention ultrasound imaging beam-former may be incorporated in an ultrasonic imaging system convenient enough to be a common component of nearly every medical examination and procedure. The present invention ultrasound imaging beam-former provides the potential to have a broad and significant impact in healthcare. The instant document identifies various clinical applications of the present invention ultrasound imaging beam-forming apparatus, but should not be limited thereto, and other applications will become attained as clinicians gain access to the system and method.

[0034] The preferred embodiments of the present invention may improve significantly upon existing methods and/or apparatuses. In particular, the present invention comprises an ultrasound imaging beam-former that may be used in a hand held ultrasonic instrument such as one provided in a portable unit which performs B-mode or C-Mode imaging and/or collects three dimensional (3-D) image data.

[0035] According to some embodiments, an ultrasound imaging beam-former is provided that includes, in a first aspect of the invention, an ultrasound imaging beam-former apparatus includes a signal generator for producing an outgoing signal, a transducer for converting the outgoing signal to outgoing ultrasound and for converting at least a portion of the outgoing ultrasound that is reflected to an incoming signal, the incoming signal having a period, and a signal receiver for processing the incoming signal, the signal receiver including, an in-phase sample-and-hold connected receiveably to the transducer for sampling the incoming signal at an incoming time and outputting an in-phase amplitude of the incoming signal at substantially the incoming time, a quadrature sample-and-hold connected receiveably to the transducer for sampling the incoming signal at substantially one-quarter of the period after the incoming time, the quadrature sample-and-hold outputting a quadrature amplitude of the incoming signal at substantially one-quarter of the period after the incoming time, a phase calculator connected receiveably to the in-phase sample-and-hold and the quadrature sample-and-hold for receiving the incoming time, the in-phase amplitude, and the quadrature amplitude and outputting a phase, and a phase rotator for applying an illumination to the image point in substantial proportion to the phase.

[0036] In a second aspect, a method of beam-forming for ultrasound imaging includes generating an outgoing signal, transducing the outgoing signal to outgoing ultrasound, receiving at least a portion of reflected outgoing ultrasound,

transducing the reflected ultrasound to an incoming signal having a period, sampling the incoming signal at an incoming time to produce an in-phase amplitude of the incoming signal, sampling the incoming signal at substantially one-quarter of the period after the incoming time to produce a quadrature amplitude of the incoming signal, calculating a phase at the incoming time based on the in-phase amplitude and the quadrature amplitude, and applying an illumination to the image point in substantial proportion to the phase.

**[0037]** In a third aspect, a system for beam-forming for ultrasound imaging includes means for generating an outgoing signal, means for transducing the outgoing signal to outgoing ultrasound, means for transducing at least a portion of reflected outgoing ultrasound to an incoming signal having a period, means for sampling the incoming signal at an incoming time and outputting an in-phase amplitude of the incoming signal, means for sampling the incoming signal at substantially one-quarter of the period after the incoming time and outputting a quadrature amplitude of the incoming signal, means for calculating a phase at the incoming time, based on the in-phase amplitude and the quadrature amplitude and outputting the phase, means for measuring a difference between the outgoing amplitude and the magnitude, means for applying a first illumination to a image point in substantial proportion to the difference, and means for applying a second illumination to the image point in substantial proportion to the phase.

**[0038]** The above and/or other aspects, features and/or advantages of various embodiments will be further appreciated in view of the following description in conjunction with the accompanying figures. Various embodiments can include and/or exclude different aspects, features and/or advantages where applicable. In addition, various embodiments can combine one or more aspect or feature of other embodiments where applicable. The descriptions of aspects, features and/or advantages of particular embodiments should not be construed as limiting other embodiments or the claims.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

**[0039]** The device and method for ultrasound imaging beam-forming may be utilized with various products and services as discussed below, but is not limited thereto. Technicians may attempt to insert needles into a vein based on the surface visibility of the vein coupled with their knowledge of anatomy. While this approach works quite well in thin, healthy individuals, it can prove extremely difficult in patients who may be ill or obese. It may be desirable to have a relatively small, inexpensive, and portable ultrasound imaging system for guiding the insertion of intravenous (IV) devices like needles and catheters into veins, or for drawing blood.

**[0040]** Sleep apnea (obstruction of the air passage in the of the throat) may affect more than eighteen million Americans. Obstructive sleep apnea may be among the most common variants of sleep apnea. Obstructive sleep apnea may represent a significant risk to the patient. It is difficult and expensive to diagnose obstructive sleep apnea. Typical diagnostic methods require an overnight hospital stay in an instrumented laboratory. Many at-risk patients refuse this inconvenient testing regime and thus go undiagnosed. It may be desirable to have a relatively small, inexpensive, and portable ultrasound imaging system to aid in the diagnosis of obstructive sleep apnea in a minimally obtrusive manner.

**[0041]** Manual palpation is an exceedingly common diagnostic procedure. Clinicians use their sense of touch to feel for subcutaneous lumps or even to estimate the size of lymph nodes or other masses. While palpation undoubtedly yields valuable qualitative information, numerous studies have shown it to have extremely poor sensitivity and that quantitative size estimates may be completely unreliable. It may be desirable to have a relatively small, inexpensive, and portable ultrasound imaging system to aid in observing subcutaneous tissues.

**[0042]** It may be desirable to place an image display at a transducer. It may be desirable to have a relatively small, inexpensive, and portable ultrasound imaging system to aid in placing the image display at the transducer.

**[0043]** Ultrasound may be used to search for internal defects in metallic or ceramic parts in a broad variety of industrial applications. Current systems may be cost effective, but may be unwieldy and acquire limited data, making it difficult to ensure that a thorough search has been performed. It may be desirable to have a relatively small, inexpensive, and portable ultrasound imaging system to aid in non-destructive evaluation.

**[0044]** Furthermore, new users may expect ultrasound images to produce representations parallel to the skin's surface, i. e. C-Scan images. It would be desirable for a low cost, system to be capable of producing C-Scan images. It may further be desirable to display data in the intuitive C-scan format to allow clinicians with little or no training in reviewing ultrasound images to make use of the device.

**[0045]** Ultrasound imaging devices may be too expensive for some applications. It may be desirable for an ultrasound imaging device to rely primarily or exclusively on receive side beam-forming to reduce or eliminate transmit-side circuitry, enabling the beam-former to be implemented using large scale integration or as software, and enabling system to be produced at a lower cost.

**[0046]** It may further be desirable for an ultrasound imaging device to rely primarily or exclusively on phase rotation for focusing, enabling the beam-former to be implemented using large scale integration or as software, and enabling system to be produced at a lower cost.

**[0047]** Ultrasound imaging devices may be insufficiently portable for some applications. It may be desirable for an ultrasonic imaging device to be of a small size to make it easy to carry the device in a pocket or on a belt attachment. This may make the device as convenient as a stethoscope and will thus open new applications. It may be desirable for an ultrasound imaging device to rely primarily or exclusively on receive side beam-forming to reduce or eliminate transmit-side circuitry, enabling the beam-former to be implemented using large scale integration or as software, and enabling the system to be made portable. It may further be desirable for an ultrasound imaging device to rely primarily or exclusively on phase rotation for focusing to reduce or eliminate transmit-side circuitry, enabling the beam-former to be implemented using large scale integration or as software, and enabling the system to be made portable.

**[0048]** Since it would be desirable for a beam-former to be simple, small, and low cost, it would be further desirable for the size and speed requirements of digital memory in such a beam-former to be minimized. It would be further desirable for focusing to be performed solely by phase rotation of I/Q data, thus eliminating the need for some circuitry, and allowing some of the remaining circuitry to be implemented as an

integrated circuit. This may also allow the use of slower memory and reduce the computational complexity of the beam-former.

**[0049]** It would be further desirable for I/Q data to be generated by sampling an RF signal directly. In one embodiment, an analytic signal (I/Q data) is generated by sampling the received RF signal directly, in a manner analogous to the Hilbert transform. In one embodiment, focusing is implemented via phase rotation of this I/Q data.

**[0050]** In FIG. 1 is shown an ultrasound imaging beam-former apparatus **100** according to a first embodiment of the invention. Ultrasound imaging beam-former apparatus **100** may include a signal generator **102** for producing an outgoing signal **104** having an outgoing amplitude **106** at an outgoing time **108**, as shown in FIG. 6A. In several embodiments, outgoing signal **104** may be an electrical signal, an electro-magnetic signal, or an optical signal.

**[0051]** If outgoing signal **104** is an optical signal, cross-talk between the circuits of ultrasound imaging beam-former apparatus **100** may be reduced or eliminated, since optical signals do not, in general, interfere with one another. This may allow ultrasound imaging beam-former apparatus **100** to be made smaller than an equivalent electronic device by increasing the density of the circuits. In one case, outgoing signal **104** may be processed as an optical signal and converted to an electrical signal to drive a transducer. An integrated circuit comprising ultrasound imaging beam-forming apparatus **100** may be implemented out of gallium-arsenide (GaAs) so that the both the optical circuits and the electrical circuits can be implemented on the same device. In another case, a transducer utilizing sono-luminescence to convert light directly into sound may be used, dispensing entirely with any need for an electrical-optical interface.

**[0052]** In several embodiments, signal generator **102** may be a storage device, such as a read-only memory (ROM), an oscillator such as a crystal oscillator, a resonant circuit such as a resistor-inductor-capacitor (RLC) or tank circuit, a resonant cavity such as a ruby laser or a laser diode or a tapped delay line.

**[0053]** In the event that signal generator **102** is a storage device, outgoing signal **104** may have been stored previously, to be read out when needed. In this embodiment, several versions of outgoing signal **104** may be stored for use with various objects **170** to be imaged. Ultrasound imaging beam-forming apparatus **100** may thus be set to produce a signal appropriate for a particular object **170** to be imaged by choosing one of the stored versions of outgoing signal **104**.

**[0054]** In the event that signal generator **102** is an oscillator, outgoing signal **104** may be a sinusoid of varying frequencies. In this case, outgoing signal **104** may be generated at an arbitrarily high clock speed and still be forced through filters of arbitrarily small bandwidth. This may be advantageous, for example, if a wide band signal is inconvenient. A resonant circuit or a resonant cavity may work in a similar manner. Furthermore, an oscillator may be used to produce a range of frequencies, from which a frequency that generates an optimum response may be selected.

**[0055]** In the event that signal generator **102** is tapped delay line, outgoing signal **104** could be generated in a manner similar to a spreading code in a code division multiple access (CDMA) format cell phone system. In this case outgoing signal **104** would not need to be a pure sinusoid, but may be a code with a fixed repetition length, such as a Walsh or a Gold code. This may, for example, allow an autocorrelation length

of outgoing signal **104** to be adjusted to enhance or suppress coded excitation of an incoming signal.

**[0056]** If signal generator **102** is a tapped delay line it may be followed by an equalizer to bias or pre-emphasize a range of frequencies in outgoing signal **104**. In one embodiment, the equalizer may be an adaptive equalizer that operates on an incoming signal analogous to the sound reflected by the imaged object **170**. In this case, the incoming signal could be measured and the result applied to the adaptive equalizer to compensate for frequency attenuation of the sound by amplifying one or more frequencies of the incoming signal or outgoing signal **104** as necessary. This may be useful if, for example, object **170** attenuates or absorbs sound to the point that no return signal is available for imaging. In one embodiment, the adaptive equalizer could be placed in parallel with signal generator **102** and in series with the incoming signal.

**[0057]** In one embodiment, an equalizer could be placed in series with signal generator **102**. In this case the equalizer could emphasize a particular frequency or frequencies in outgoing signal **104**. The equalizer may, for example, place a bias or pre-emphasis toward lower frequencies on outgoing signal **104**. This embodiment may be appropriate if, for example, object **170** to be imaged is expected to have features that attenuate lower frequencies significantly more than higher frequencies to the extent that imaging may be difficult. The converse may be true as well, in that the equalizer may have a bias or pre-emphasis toward higher frequencies.

**[0058]** In one embodiment, outgoing signal **104** may be amplified. In one embodiment, signal generator **102** may include a generator amplifier **158** for amplifying outgoing signal **104**. Generator amplifier **158** may pre-emphasize certain frequencies of outgoing signal **104** to suit the attenuation characteristics of object **170** to be imaged as well. Signal generator **102** may also include an oscillator to produce an appropriate modulation frequency, such as a radio frequency (RF) signal, with which to modulate outgoing signal **104**.

**[0059]** A transducer **110** may convert outgoing signal **104** to outgoing ultrasound **112**. In several embodiments, transducer **110** may be a piezoelectric element, a voice coil, a crystal oscillator or a Hall effect transducer **110**. In one embodiment, reversals of outgoing signal **104** produce vibration of a surface of transducer **110** at substantially the frequency of outgoing signal **104**. In another embodiment, reversals of outgoing signal **104** produce vibrations of a surface of transducer **110** at frequencies that are significantly higher or lower than the frequency of outgoing signal **104**, such as harmonics of outgoing signal **104**. This vibration may, in turn, produce successive compressions and rarefactions of an atmosphere surrounding the surface of transducer **110**, also at substantially the frequency of outgoing signal **104**. If the frequency of outgoing signal **104** is substantially higher than a frequency at which sound may be heard, the successive compressions and rarefactions of the atmosphere may be termed ultrasound.

**[0060]** In one embodiment, transducer **110** may include a plurality of transducers **110**. In one embodiment, plurality of transducers **110** may be arranged in an array **166**. In several embodiments, array **166** may be a linear array, a phased array, a curvilinear array, an unequally sampled 2-D array, a 1.5-D array, an equally sampled 2D array, a sparse 2D array, or a fully sampled 2D array.

**[0061]** If outgoing ultrasound **112** is reflected by object **170**, some of outgoing ultrasound **112** may return to ultrasound imaging system **100** as reflected ultrasound **182**.

Reflected ultrasound **182** may be converted to an incoming signal **114** having a period **116**, as shown in FIG. 6B. In several embodiments, incoming signal **114** may be an electromagnetic signal, an electrical signal or an optical signal. In several embodiments, incoming signal **114** may be amplified, pre-amplified, or stored.

[0062] In one embodiment, outgoing ultrasound **112** may be delayed or attenuated partially by object **170**. A first portion **174** of outgoing ultrasound **112**, for example, may be reflected immediately upon encountering a nearer surface **178** of object **170** while a second portion **176** of outgoing ultrasound **112** is not reflected until it encounters a further surface **180** of object **170**. A round trip of second portion **176** will thus be longer than a round trip of first portion **174**, resulting in a delay of second portion **176** relative to first portion **174**, as well as delays of both first and second portions **174,176** relative to outgoing ultrasound **112**. Furthermore, second portion **176** may be damped or attenuated by a material of object **170**. The delays may be measured for disparate points of object **170**, producing an image **168** of object **170**.

[0063] Apparatus **100** may include a signal receiver **118** for processing incoming signal **114**. In one embodiment, signal receiver **118** may be implemented as a digital signal processor **164**. In one embodiment, signal receiver **118** may be implemented as an integrated circuit.

[0064] Ultrasonic transducers associated with ultrasound imaging systems may be driven from a single terminal with the second terminal grounded. A transducer may be used to transmit ultrasound signals as well as receive reflected ultrasound. A signal received at a transducer may typically be several orders of magnitude smaller than the signal that was transmitted due to, inter alia, signal attenuation by the target tissue. Some of the signal may be lost due to transducer inefficiencies as well. It may be thus necessary to couple the transducer to a high-voltage transmit signal while the ultrasound is being transmitted, and then to a sensitive low-noise pre-amplifier while the reflected ultrasound is being received.

[0065] A switch that couples the transducer to the transmit and receive signals must be capable of withstanding high peak transmit voltages (typically 50-200 volts) while isolating the pre-amplifier input from those voltage levels, since they would otherwise destroy the pre-amplifier. If a receiver for the signals from the transducers is implemented as a high-density, low-voltage integrated circuit (IC), the switches themselves may need to be implemented off-chip in a separate package from materials and devices that can withstand the high voltage transmit pulses.

[0066] In one embodiment, ultrasound imaging system **100** may include a protection circuit **172** to allow both transmit and receive operations, as shown in FIG. 2. A piezoelectric transducer array **202**, shown on the left, acts as an interface to a signal processor by converting electrical signals to acoustic pulses and vice versa. Images may be formed by transmitting a series of acoustic pulses from the transducer array **202** and displaying signals representative of the magnitude of the echoes received from these pulses. A beam-former **214** applies delays to the electrical signals to steer and focus the acoustic pulses and echoes.

[0067] Image formation begins when a state of a transmit/receive switch (TX/RX switch) **204** is altered to connect the transducer elements **202** to individual transmit circuits. Next, transmit generators **206** output time varying waveforms with delay and amplitude variations selected to produce a desired acoustic beam. Voltages of up to 200 Volts may be applied to

the transducer elements **202**. Once transmission is complete, the state of the TX/RX switch **204** is altered again to connect the transducer elements **202** to individual receive circuitry associated with each element.

[0068] Signals representative of incoming echoes may be amplified by pre-amplifiers **208** and time gain control (TGC) **210** circuits to compensate for signal losses due to diffraction and attenuation. Note that the transducer array **202** shown in FIG. 2 has one common electrode **212**, and the non-common electrodes may be multiplexed between high-voltage transmit and low-voltage receive signals. This conventional TX/RX switch **204** is the source of considerable expense and bulk in typical ultrasound systems.

[0069] In FIG. 3 is shown an alternative ultrasound imaging beam-forming apparatus **300** with a protection circuit for use with an embodiment of the invention. Ultrasound imaging beam-forming apparatus **300** may include a signal generator **302** for producing an outgoing signal **304**.

[0070] Ultrasound imaging beam-forming apparatus **300** may also include a transducer **306** for converting outgoing signal **304** to outgoing ultrasound **308** at a frequency of outgoing signal **304**. In one embodiment, transducer **306** may have a transmit side **314** forming an interface with outgoing signal **304**.

[0071] In one embodiment, transmit side **314** may be connected operably to a transmit switch **318**. In several embodiments, transmit switch **318** may be an electronic switch, an optical switch, a micro-mechanical switch, a transistor, a field-effect transistor (FET), a bi-polar transistor, a metal-oxide-semiconductor (MOS) transistor, a complementary metal-oxide-semiconductor (CMOS) transistor, or a metal-oxide-semiconductor field-effect transistor (MOSFET). Transmit switch **318** may be connected switchably to signal generator **302** and a ground **320**.

[0072] In one embodiment, transducer **306** may convert at least a portion of reflected ultrasound **310** to an incoming signal **312**. In several embodiments, incoming signal **312** may be an electro-magnetic signal, an electrical signal, or an optical signal. In one embodiment, transducer **306** may have a receive side **316** forming an interface with incoming signal **312**.

[0073] In one embodiment, receive side **316** may be connected operably to a receive switch **322**. In several embodiments, receive switch **322** may be an electronic switch, an optical switch, a micro-mechanical switch, a transistor, a field-effect transistor, a bi-polar transistor, a MOS transistor, a CMOS transistor, or a MOSFET transistor. Receive switch **322** may be connected switchably to a signal receiver **324** and ground **320**.

[0074] In one embodiment, transmit switch **318** may connect transmit side **314** to signal generator **302** for a first predetermined period of time while signal generator **302** generates outgoing signal **304**. In this embodiment, receive switch **322** may connect receive side **316** to signal receiver **324** for a second predetermined period of time while signal receiver **324** receives incoming signal **312**. Transmit switch **318** may connect transmit side **314** to ground **320** during substantially second predetermined period of time while signal receiver **324** receives incoming signal **312**, and receive switch **322** may connect receive side **316** to ground **320** during substantially first predetermined period of time while signal generator **302** generates outgoing signal **304**. In one embodiment, transmit side **314** and receive side **316** are on separate transducers **306**.

[0075] In one embodiment, signal receiver 118 may include a receiver amplifier 160 for amplifying incoming signal 114. In one embodiment, signal receiver 118 may include a receiver pre-amplifier 162 for amplifying incoming signal 114. In one embodiment, signal receiver 118 may include a band-pass filter 164 for filtering incoming signal 114.

[0076] In one embodiment, signal receiver 118 may include an in-phase sample-and-hold 120 connected receiveably to transducer 110 for sampling incoming signal 114 at an incoming time 122 and outputting an in-phase amplitude 124 of incoming signal 114 at substantially incoming time 122. In one embodiment, signal receiver 118 may include an in-phase analog-to-digital converter 126 connected receiveably to in-phase sample-and-hold 120 for assigning an in-phase digital value 128 to in-phase amplitude 124 and outputting in-phase digital value 128.

[0077] In one embodiment, signal receiver 118 may include a quadrature sample-and-hold 130 connected receiveably to transducer 110 for sampling incoming signal 114 at substantially one-quarter of period 116 after incoming time 122, quadrature sample-and-hold 130 outputting a quadrature amplitude 132 of incoming signal 114 at substantially one-quarter of period 116 after incoming time 122. One-quarter of period 116 is merely exemplary. Incoming signal 114 may be sampled at any appropriate interval or fraction of period 116. In one embodiment, signal receiver 118 may include a quadrature analog-to-digital converter 134 connected receiveably to quadrature sample-and-hold 130 for assigning a quadrature digital value 136 to quadrature amplitude 132 and outputting quadrature digital value 136.

[0078] In one embodiment, signal receiver 118 may include a magnitude calculator 138 connected receiveably to in-phase analog-to-digital converter 126 and quadrature analog-to-digital converter 134 for receiving incoming time 122, in-phase digital value 128, and quadrature digital value 136 and outputting a magnitude 140. In one embodiment, signal receiver 118 may include a phase calculator 142 connected receiveably to in-phase analog-to-digital converter 126 and quadrature analog-to-digital converter 134 for receiving incoming time 122, in-phase digital value 128, and quadrature digital value 136 and outputting a phase 144.

[0079] In one embodiment, incoming signal 114 may be band-pass filtered by band-pass filter 164 and diverted to in-phase sample-and-hold 120 and quadrature sample-and-hold 130. An in-phase clock signal 184 driving in-phase sample-and-hold 120 may be of the same frequency as a quadrature clock signal 186 driving quadrature sample-and-hold 130. Quadrature clock signal 186 may, however, be offset by a quarter of period 116 with respect to in-phase clock signal 184 at an assumed center frequency of incoming signal 114. An output of in-phase sample-and-hold 120 may be digitized by in-phase analog-to-digital converter 126 while an output of quadrature sample-and-hold 130 is digitized in quadrature analog-to-digital converter 134, forming I and Q channel data.

[0080] Reflected ultrasound 182 may be considered to be real part of an amplitude and phase modulated complex exponential signal, or analytic signal. The modulating signal may be expressed mathematically as:

[0081] [text missing or illegible when filed]  $A(t)e^{j\phi(t)}$  with instantaneous amplitude  $A(t)$  and phase  $\phi(t)$ . This is superimposed on a carrier signal  $e^{-j\omega_0 t}$ , where  $\omega_0 = 2\pi f_0$  and  $f_0$  is the frequency of the signal. Therefore the analytic signal  $S(t)$  can be written as,

$$\begin{aligned} S(t) &= A(t)e^{-j(\omega_0 t - \phi(t))} \\ &= A(t)\cos(\omega_0 t - \phi(t)) - jA(t)\sin(\omega_0 t - \phi(t)) \end{aligned} \quad (1)$$

[0082] Only the real part of  $S(t)$ , which is equivalent to reflected ultrasound 182, is able to be acquired experimentally.

$$I(t) = \text{Re}\{S(t)\} = A(t)\cos(\omega_0 t - \phi(t)) \quad (2)$$

[0083] The output of in-phase analog-to-digital converter 126 is the signal in equation 2 after sampling, or

$$\hat{I}(nT) = I(nT) = A(nT)\cos(\omega_0 nT - \phi(nT)), n=0, 1, 2, 3 \dots \quad (3)$$

[0084] where  $T$  is the sample interval. However, we also require the imaginary component of  $S(t)$ , shown below in equation 4, to perform beam-forming.

$$Q(t) = \text{Im}\{S(t)\} = -A(t)\sin(\omega_0 t - \phi(t)) \quad (4)$$

[0085] Quadrature clock signal 186 has a time lag of a quarter period at the assumed center frequency relative to the in-phase clock signal 184, as shown 1 schematically in FIG. 7. Therefore the relative time lag is:

$$\frac{1}{4f_0}, \text{ or } \frac{\pi}{2\omega_0}.$$

[0086] The output of quadrature sample-and-hold 130 is,

$$\begin{aligned} \hat{Q}(nT) &= I\left\{nT + \frac{\pi}{2\omega_0}\right\} \\ &= A\left(nT + \frac{\pi}{2\omega_0}\right)\cos\left(\omega_0\left(nT + \frac{\pi}{2\omega_0}\right) - \phi\left(nT + \frac{\pi}{2\omega_0}\right)\right) \end{aligned} \quad (5)$$

[0087] We assume that the modulating signal  $A(t)e^{j\phi(t)}$  varies slowly with time and approximate,

$$A\left(nT + \frac{\pi}{2\omega_0}\right) \approx A(nT) \quad (6)$$

and

$$\phi\left(nT + \frac{\pi}{2\omega_0}\right) \approx \phi(nT) \quad (7)$$

[0088] Equation 5 can now be rewritten as follows.

$$\begin{aligned} \hat{Q}(nT) &\approx A(nT)\cos\left(\omega_0\left(nT + \frac{\pi}{2\omega_0}\right) - \phi(nT)\right), \\ n &= 0, 1, 2, 3 \dots \\ &\approx -A(nT)\sin(\omega_0 nT - \phi(nT)) \\ &\approx Q(nT) \end{aligned} \quad (8)$$

[0089] We therefore approximate the imaginary component of  $S(t)$ , or  $Q(t)$  in equation 4, by estimating it to be the output of quadrature sample-and-hold 130.

[0090] Geometric time delays may be calculated and converted to phase delays at the assumed center frequency. Com-



plex weights that implement apodization and focus with the calculated phase delays may be applied to the I/Q data. In one embodiment, signal receiver 118 may include an apodizer 146 for applying a difference 148 between outgoing amplitude 106 and magnitude 140 and applying a first illumination 150-1 to an image point 154 in substantial proportion to difference 148. In one embodiment, signal receiver 118 may include a phase rotator 152 for applying a second illumination 150-2 to image point 154 in substantial proportion to phase 144.

[0091] In a second embodiment of the invention, shown in FIG. 4, apparatus 100 may include a second transducer 110-2 for converting outgoing signal 104 to second outgoing ultrasound 112-2. Some of second outgoing ultrasound 112-2 may return to second transducer 110-2 if it is reflected by object 170 as well. Second transducer 110-2 may convert at least a portion of outgoing ultrasound 112 and second outgoing ultrasound 112-2 to a second incoming signal 114-2 having a second period 116-2, as shown in FIG. 6C.

[0092] In one embodiment, signal receiver 118 may include a second in-phase sample-and-hold 120-2 connected receiveably to second transducer 110-2 for sampling second incoming signal 114-2 at incoming time 122 and outputting a second in-phase amplitude 124-2 of second incoming signal 114-2 at substantially incoming time 122. In one embodiment, signal receiver 118 may include a second in-phase analog-to-digital converter 126-2 connected receiveably to second in-phase sample-and-hold 120-2 for assigning a second in-phase digital value 128-2 to second in-phase amplitude 124-2 and outputting second in-phase digital value 128-2.

[0093] In one embodiment, signal receiver 118 may include a second quadrature sample-and-hold 130-2 connected receiveably to second transducer 110-2 for sampling second incoming signal 114-2 at substantially one-quarter of second period 116-2 after incoming time 122, second quadrature sample-and-hold 130-2 outputting a second quadrature amplitude 132-2 of second incoming signal 114-2 at substantially one-quarter of second period 116-2 after incoming time 122. In one embodiment, signal receiver 118 may include a second quadrature analog-to-digital converter 134-2 connected receiveably to second quadrature sample-and-hold 130-2 for assigning a second quadrature digital value 136-2 to second quadrature amplitude 132-2 and outputting second quadrature digital value 136-2. [0085] In one embodiment, signal receiver 118 may include a second magnitude calculator 138-2 connected receiveably to second in-phase analog-to-digital converter 126-2 and second quadrature analog-to-digital converter 134-2 for receiving incoming time 122, second in-phase digital value 128-2, and second quadrature digital value 136-2 and outputting a second magnitude 140-2. In one embodiment, signal receiver 118 may include a second phase calculator 142-2 connected receiveably to second in-phase analog-to-digital converter 126-2 and second quadrature analog-to-digital converter 134-2 for receiving incoming time 122, second in-phase digital value 128-2, and second quadrature digital value 136-2 and outputting a second phase 144-2.

[0094] In one embodiment, signal receiver 118 may include a second apodizer 146-2 for applying a second difference 148-2 between outgoing amplitude 106 and second magnitude 140-2 and applying a third illumination 150-3 to an image point 154 in substantial proportion to second difference 148-2. In one embodiment, signal receiver 118 may include a second phase rotator 152-2 for applying a fourth

illumination 150-4 to image point 154 in substantial proportion to second phase 144-2. In one embodiment, signal receiver 118 may include a summer 156 for combining difference 148, second difference 148-2, phase 144, and second phase 144-2 before first, second, third, and fourth illuminations 150-1-150-4 are applied to image point 154.

[0095] In a third embodiment, a method of beam-forming for ultrasound imaging may include the steps of generating an outgoing signal 104 having an outgoing amplitude 106 at an outgoing time 108, transducing outgoing signal 104 to outgoing ultrasound 112, receiving at least a portion of reflected outgoing ultrasound 112, transducing reflected ultrasound to an incoming signal 114 having a period 116, sampling incoming signal 114 at an incoming time 122 to produce an in-phase amplitude 124 of incoming signal 114, assigning an in-phase digital value 128 to in-phase amplitude 124 sampling incoming signal 114 at substantially one-quarter of period 116 after incoming time 122 to produce a quadrature amplitude 132 of incoming signal 114, assigning a quadrature digital value 136 to quadrature amplitude 132, calculating a magnitude 140 at incoming time 122 based on in-phase digital value 128 and quadrature digital value 136, calculating a phase 144 at incoming time 122 based on in-phase digital value 128 and quadrature digital value 136, measuring a difference 148 between outgoing amplitude 106 and magnitude 140, applying a first illumination 150-1 to an image point 154 in substantial proportion to difference 148, and applying a second illumination 150-2 to image point 154 in substantial proportion to phase 144.

[0096] In one embodiment, the method of beam-forming for ultrasound imaging may further include the steps of transducing outgoing signal 104 to second outgoing ultrasound 112-2, receiving at least a portion of reflected outgoing ultrasound 112 and second outgoing ultrasound 112-2, transducing reflected outgoing ultrasound 112 and second outgoing ultrasound 112-2 to a second incoming signal 114-2 having a second period 116-2, sampling second incoming signal 114-2 at incoming time 122 to produce a second in-phase amplitude 124-2 of second incoming signal 114-2, assigning a second in-phase digital value 128-2 to second in-phase amplitude 124-2, sampling second incoming signal 114-2 at substantially one-quarter of second period 116-2 after incoming time 122 to produce a second quadrature amplitude 122-2 of second incoming signal 114-2, assigning a second quadrature digital value 136-2 to second quadrature amplitude 122-2, calculating a second magnitude 140-2 at incoming time 122 based on second in-phase digital value 128-2 and second quadrature digital value 136-2, calculating a second phase 144-2 at incoming time 122 based on second in-phase digital value 128-2 and second quadrature digital value 136-2, measuring a second difference 148-2 between outgoing amplitude 106 and second magnitude 140-2, summing difference 148, second difference 148-2, phase 144, and second phase 144-2, applying a third illumination 150-3 to image point 154 in substantial proportion to second difference 148-2, and applying a fourth illumination 150-4 to image point 154 in substantial proportion to second phase 144-2.

[0097] In one embodiment, the method of beam-forming may be repeated to produce a plurality of image points 154 forming an image 168. In several embodiments, image 168 may be viewed, used to guide insertion of a needle, used to guide insertion of a catheter, used to guide insertion of an endoscope, used to estimate blood flow, or used to estimate tissue motion. In one embodiment, plurality of image points

**154** may be focused. In one embodiment, focusing may be repeated on reflected outgoing ultrasound **112** at plurality of image points **154**.

**[0098]** In one embodiment, plurality of image points **154** may be along a line at a range of interest. In one embodiment, a line may be formed at a plurality of ranges to form a planar image. In one embodiment, the planar image may be a B-mode image. In one embodiment, plurality of image points **154** may lie within a plane at a range of interest. In one embodiment, plurality of image points **154** may form a C-scan. In one embodiment, the plane may be formed at multiple ranges. In one embodiment, several planes may form a complex 1-D image.

**[0099]** In one embodiment, an envelope of magnitude **140** may be displayed. In one embodiment, phase **144** may be used to compensate for a path difference **148** between various transducers and object **170**. In one embodiment, a main lobe resolution and a side lobe level may be balanced based on magnitude **140**. In one embodiment, a sum squared error between a desired system response and a true system response may be minimized.

**[0100]** One skilled in the art would appreciate that a variety of tissue information may be obtained through judicious pulse transmission and signal processing of received echoes with the current invention. Such information could be displayed in conjunction with or instead of the aforementioned echo information.

**[0101]** One such type of information is referred to as color flow Doppler as described in U.S. Pat. No. 4,573,477 to Namekawa et al., entitled "Ultrasonic Diagnostic Apparatus," hereby incorporated by reference herein in its entirety. Another useful type of information is harmonic image data as described in U.S. Pat. No. 6,251,074 to Averkiou et al., entitled "Ultrasonic Tissue Harmonic Imaging" and U.S. Pat. No. 5,632,277 to Chapman et al., entitled "Ultrasound Imaging System Employing Phase Inversion Subtraction to Enhance the Image," both of which are hereby incorporated by reference herein in their entirety. Yet another type of information that may be obtained and displayed is known as Power Doppler as described in U.S. Pat. No. 5,471,990 to Thirsk, entitled "Ultrasonic Doppler Power Measurement and Display System," hereby incorporated by reference herein in its entirety.

**[0102]** Angular scatter information might also be acquired using a method described in a co-pending U.S. patent application Ser. No. 10/030,958, entitled "Angular Scatter Imaging System Using Translating Apertures Algorithm and Method Thereof," filed Jun. 3, 2002, of which is hereby incorporated by reference herein in its entirety. Speckle is a common feature of ultrasound images. While it is fundamental to the imaging process, many users find its appearance confusing and it has been shown to limit target detectability. A variety of so called compounding techniques have been described which could be valuable for reducing the appearance of speckle in ultrasound transducer drive images. These techniques include spatial compounding and frequency compounding, both of which are well described in the literature.

**[0103]** One skilled in the art would appreciate that the common practice of frequency compounding could be readily applied to the current invention. By transmitting a plurality of pulses at different frequencies and forming separate detected images using the pulses one may obtain multiple unique speckle patterns from the same target. These patterns may then be averaged to reduce the overall appearance of speckle.

**[0104]** The well known techniques of spatial compounding may also be applied to the current invention. The most conventional form of spatial compounding, which we call two-way or transmit-receive spatial compounding, entails the acquisition of multiple images with the active transmit and receive apertures shifted spatially between image acquisitions. This shifting operation causes the speckle patterns obtained to differ from one image to the next, enabling image averaging to reduce the speckle pattern.

**[0105]** In another technique, which we term one-way or receive-only spatial compounding, the transmit aperture is held constant between image acquisitions while the receive aperture is shifted between image acquisitions. As with two-way spatial compounding, this technique reduces the appearance of speckle in the final image.

**[0106]** In many ultrasound applications the received echoes from tissue have very small amplitude, resulting in an image with poor signal to noise ratio. This problem may be addressed through the use of a technique known as coded excitation. In this method the transmitted pulse is long in time and designed so that it has a very short auto-correlation length. In this manner the pulse is transmitted and received signals are correlated with the transmitted pulse to yield a resultant signal with good signal to noise ratio, but high axial resolution (short correlation length). This method could be readily applied in the present invention ultrasound transducer drive device and method to improve the effective signal to noise ratio. The coded excitation technique is described in U.S. Pat. No. 5,014,712 to O'Donnell, entitled "Coded Excitation for Transmission Dynamic Focusing of Vibratory Energy Beam," hereby incorporated by reference herein in its entirety.

**[0107]** An aspect in fabricating a system like the present invention ultrasound imaging beam-forming apparatus is in construction of the transducer array. Both cost and complexity could be reduced by incorporating a transducer implemented using photolithographic techniques, i. e. the transducer is formed using micro electro mechanical systems (MEMS). One particularly attractive approach has been described in U.S. Pat. No. 6,262,946 to Khuri-Yakub et al., entitled "Capacitive Micromachined Ultrasonic Transducer Arrays with Reduced Cross-Coupling," hereby incorporated by reference herein in its entirety.

**[0108]** While the present invention may be embodied in many different forms, a number of illustrative embodiments are described herein with the understanding that the present disclosure is to be considered as providing examples of the principles of the invention and such examples are not intended to limit the invention to preferred embodiments described herein and/or illustrated herein.

#### Broad Scope of the Invention:

**[0109]** While illustrative embodiments of the invention have been described herein, the present invention is not limited to the various preferred embodiments described herein, but includes any and all embodiments having equivalent elements, modifications, omissions, combinations (e. g. , of aspects across various embodiments), adaptations and/or alterations as would be appreciated by those in the art based on the present disclosure. The limitations in the claims are to be interpreted broadly based on the language employed in the claims and not limited to examples described in the present specification or during the prosecution of the application, which examples are to be construed as non-exclusive. For

example, in the present disclosure, the term “preferably” is non-exclusive and means “preferably, but not limited to.” In this disclosure and during the prosecution of this application, means-plus-function or step-plus-function limitations will only be employed where for a specific claim limitation all of the following conditions are present in that limitation: a) “means for” or “step for” is expressly recited; b) a corresponding function is expressly recited; and c) structure, material or acts that support that structure are not recited. In this disclosure and during the prosecution of this application, the terminology “present invention” or “invention” may be used as a reference to one or more aspect within the present disclosure. The language present invention or invention should not be improperly interpreted as an identification of criticality, should not be improperly interpreted as applying across all aspects or embodiments (i. e. , it should be understood that the present invention has a number of aspects and embodiments), and should not be improperly interpreted as limiting the scope of the application or claims. In this disclosure and during the prosecution of this application, the terminology “embodiment” can be used to describe any aspect, feature, process or step, any combination thereof, and/or any portion thereof, etc. In some examples, various embodiments may include overlapping features. In this disclosure, the following abbreviated terminology may be employed : “e.g.” which means “for example;” and “NB” which means “note well.”

1-72. (canceled)

73. An apparatus, comprising:

a transducer array, comprising a plurality of transducers, each configured to convert reflected ultrasound to at least one incoming signal, wherein each of the at least one incoming signal has a period and an amplitude;

a signal receiver configured to:

obtain at least two samples of the each of the at least one incoming signal spaced apart by a predetermined fraction of the period; and

create at least one pair of signals representing an in-phase digital value and a quadrature digital value, for each of the at least two samples;

a focusing apparatus configured to combine the at least one pair of signals and to generate at least one image point.

74. The apparatus of claim 73 wherein only a subset of the plurality of transducers are used to convert reflected ultrasound.

75. The apparatus of claim 73 further comprising a transmit array having a first subset of transducer elements and the receive array comprises a second subset of elements, and the first subset and second subsets are not identical.

76. The apparatus of claim 75 wherein the second subset of elements is chosen to minimize speckle distortion.

77. The apparatus of claim 73 further comprising a transmit array having a first subset of transducer elements and the receive array comprises a second subset of elements, and the first subset and second subsets are identical.

78. The apparatus of claim 73 wherein the receiver comprises each of the plurality of transducers connected to an in-phase sample-and-hold configured to output an in-phase amplitude and a quadrature sample-and-hold configured to output a quadrature amplitude.

79. The apparatus of claim 78 wherein the quadrature sample-and-hold is triggered one-quarter of the period after the in-phase sample-and-hold is triggered.

80. The apparatus of claim 78 comprising:

an in-phase analog-to-digital converter connected to the in-phase sample-and-hold for receiving the in-phase amplitude and outputting the in-phase digital value representative of the in-phase amplitude;

a quadrature analog-to-digital converter connected to the quadrature sample-and-hold for receiving the quadrature amplitude and outputting the quadrature digital value representative of the quadrature amplitude.

81. The apparatus of claim 78 comprising at least one analog-to-digital converter configured to receive the in-phase amplitude and outputs the in-phase digital value representative of the in-phase amplitude and receive the quadrature amplitude and outputs the quadrature digital value representative of the quadrature amplitude.

82. The apparatus of claim 73 comprising:

a magnitude calculator configured to receive the pair of signals and responsively generate a magnitude;

a phase calculator configured to receive the pair of signals and responsively generate a phase.

83. The apparatus of claim 73 wherein a protection circuit switches between a transmit mode and a receive mode, allowing the transducer to both transmit and receive ultrasound.

84. A method, comprising:

using a plurality of transducers to receive reflected ultrasound signals, each transducer generating a respective incoming signal having a period and an amplitude;

generating a plurality of signal pairs using a plurality of analog-to-digital converters to sample each of the respective incoming signals at least twice, wherein the samples are separated in time by a fraction of the period, and responsively generating a respective signal pair from each transducer, each respective signal pair comprising an in-phase sample and a quadrature sample; processing the plurality of signal pairs to obtain at least one focused image point.

85. The method of claim 84 wherein the fraction of the period is one quarter of the period.

86. The method of claim 84 wherein the plurality of analog-to-digital converters obtains an inphase amplitude sample and a quadrature amplitude sample and assigns an in-phase digital value to the in-phase amplitude sample, and assigns a quadrature digital value to the quadrature amplitude sample.

87. The method of claim 84 wherein processing the plurality of signal pairs comprises applying complex weights to the plurality of signal pairs to focus the image point.

88. The method of claim 84 wherein processing the signal pairs comprises:

calculating a magnitude based on the in-phase digital value and the quadrature digital value; and

calculating a phase based on the in-phase digital value and the quadrature digital value.

89. The method of claim 84 wherein the least one focused image point forms an image having a format selected from the group consisting of:

a planar image;

B-mode image;

C-scan image;

and a complex 1-D image.

90. The method of claim 88 further comprising displaying an envelope of the magnitude.

91. The method of claim 88 further comprising applying an illumination to an image point substantially in proportion to the phase.

**92.** The method of claim **91** further comprising compensating for a path difference with the phase.

**93.** The method of claim **88** further comprising balancing a main lobe resolution and a side lobe level based on the magnitude.

**94.** The method of claim **84** wherein processing the plurality of signal pairs to obtain at least one focused image point comprises applying calculated phase delays to the plurality of signal pairs.

**95.** The method of claim **84** wherein sampling is performed a plurality of times for one outgoing ultrasound transmit event to increase in image formation rate by sampling multiple ranges.

**96.** An apparatus, comprising:

- a transducer array comprising multiple transducer elements, wherein each transducer element is configured to convert ultrasound to a respective incoming signal, the incoming signal having a period and an amplitude;
- a sampling clock configured to generate trigger signals to initiate sampling;
- a plurality of analog-to-digital converters configured to generate a plurality of signal pairs, each signal pair corresponding to a respective transducer element, by converting the respective incoming signal to a digital signal pair having an in-phase digital value and a quadrature digital value, wherein the in-phase digital value is representative of an instantaneous amplitude upon the occurrence of one of at least two trigger signals, and the quadrature digital value is representative of an instantaneous amplitude upon the occurrence of another one of at least two trigger signals; and

a focusing apparatus configured to generate a plurality of image points based on the plurality of signal pairs.

**97.** The apparatus of claim **96** wherein the transducer array comprises a transmit array and a receive array, wherein the transmit array comprises a first subset of elements and the receive array comprises a second subset of elements, and the first and second subsets are not identical.

**98.** The apparatus of claim **97** wherein the second subset of elements is chosen to minimize speckle distortion.

**99.** The apparatus of claim **96** wherein the transducer array comprises a transmit array and a receive array, wherein the transmit array comprises a first subset of elements and the receive array comprises a second subset of elements, and the first and second subsets are identical.

**100.** The apparatus of claim **96** wherein the at least two trigger signals are separated in time by one-quarter of the period.

**101.** The apparatus of claim **96** comprising:

- a magnitude calculator configured to receive the in-phase digital value and the quadrature digital value outputting and output a magnitude;
- a phase calculator configured to receive the in-phase digital value and the quadrature digital value outputting and output a phase.

**102.** The apparatus of claim **99** further comprising a protection circuit configured to switch between a transmit mode and a receive mode, thereby allowing the array to both transmit and receive ultrasound.

\* \* \* \* \*

专利名称(译)	超声成像光束成形装置和方法		
公开(公告)号	<a href="#">US20120053460A1</a>	公开(公告)日	2012-03-01
申请号	US13/210890	申请日	2011-08-16
[标]申请(专利权)人(译)	弗吉尼亚大学专利基金会		
申请(专利权)人(译)	VIRGINIA专利大学基金会		
当前申请(专利权)人(译)	VIRGINIA专利大学基金会		
[标]发明人	BLALOCK TRAVIS N WALKER WILLIAM F HOSSACK JOHN A		
发明人	BLALOCK, TRAVIS N. WALKER, WILLIAM F. HOSSACK, JOHN A.		
IPC分类号	A61B8/14 A61B A61B8/00 G01S15/89 G10K11/34		
CPC分类号	A61B8/00 G01S7/52028 G01S7/52034 G01S15/8915 G01S15/8959 G01S15/8995 G10K11/346 G01S7/5208 A61B8/4494 A61B8/145 A61B8/4483 A61B8/4488 A61B8/461 A61B8/5207 G01S7/52085		
优先权	60/440262 2003-01-15 US 60/440020 2003-01-14 US 60/439990 2003-01-14 US		
其他公开文献	US9275630		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

在一些说明性实施例中，来自超声成像波束形成装置中的换能器的输入信号被应用于同相采样保持和正交采样保持。正交采样和保持可以在同相采样保持之后的四分之一周期内计时。采样保持的输出被施加到同相和正交模数转换器。幅度计算器接收同相和正交数字值，并输出幅度。相位计算器接收同相和正交数字值，并输出相位。变迹器应用输出信号的幅度和幅度之间的差值，并且对该差值基本成比例的像点施加第一照明，并且相位旋转器对该相位基本成比例的像点施加第二照明。

