



(19) **United States**

(12) **Patent Application Publication**
Jin et al.

(10) **Pub. No.: US 2019/0247025 A1**

(43) **Pub. Date: Aug. 15, 2019**

(54) **ULTRASOUND IMAGING APPARATUS,
METHOD OF CONTROLLING THE SAME,
AND COMPUTER PROGRAM PRODUCT**

Publication Classification

(51) **Int. Cl.**
A61B 8/00 (2006.01)
A61B 8/14 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 8/565* (2013.01); *A61B 8/463*
(2013.01); *A61B 8/145* (2013.01); *A61B 8/54*
(2013.01)

(71) Applicant: **SAMSUNG MEDISON CO., LTD.,**
Hongcheon-gun (KR)
(72) Inventors: **Gil-ju Jin**, Seongnam-si (KR);
Young-seok Kang, Seongnam-si (KR);
Mi-jeoung Ahn, Seongnam-si (KR);
Dae-hwan Kim, Seongnam-si (KR)

(73) Assignee: **SAMSUNG MEDISON CO., LTD.,**
Hongcheon-gun (KR)

(21) Appl. No.: **16/131,562**

(22) Filed: **Sep. 14, 2018**

(30) **Foreign Application Priority Data**

Feb. 13, 2018 (KR) 10-2018-0018064

(57) **ABSTRACT**
Provided are an ultrasound imaging apparatus and a method of controlling the same. The ultrasound imaging apparatus includes: a probe including a transducer array; an ultrasound signal receiver including a first time gain compensation (TGC) channel and a second TGC channel that each perform TGC on an ultrasound signal received from the probe; a communicator configured to communicate with a first client apparatus; and one or more processors configured to change a second TGC parameter of the second TGC channel, based on a control signal received from the first client apparatus, generate a second ultrasound image based on a second ultrasound signal produced via the second TGC channel, and transmit the second ultrasound image to the first client apparatus via the communicator.

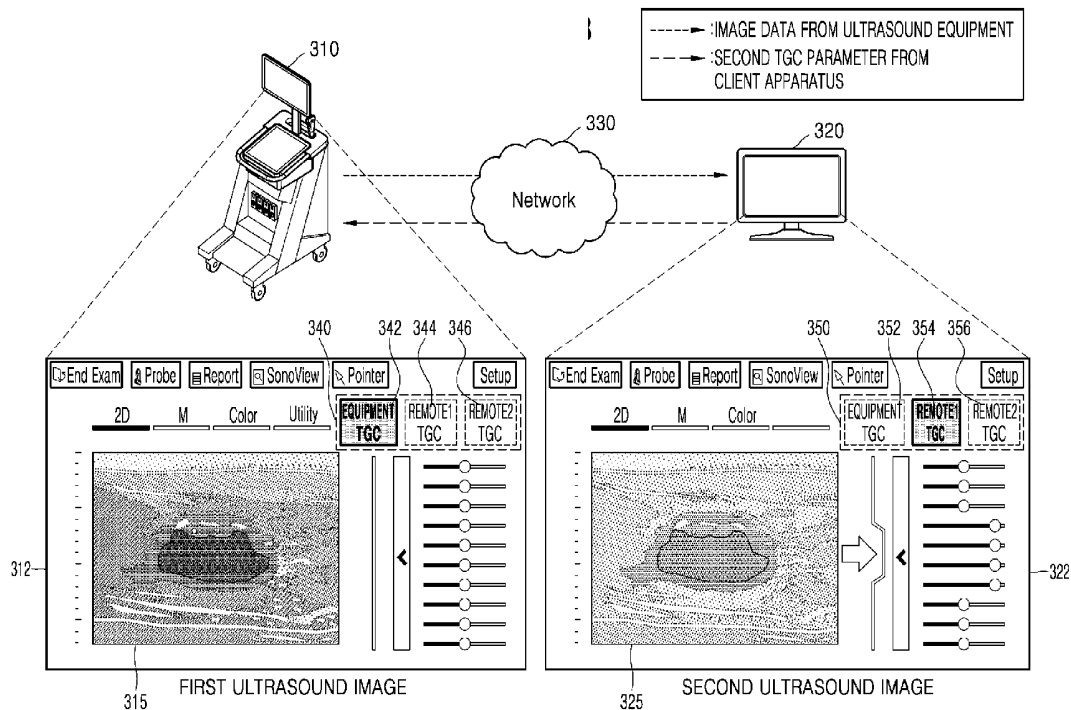


FIG. 1

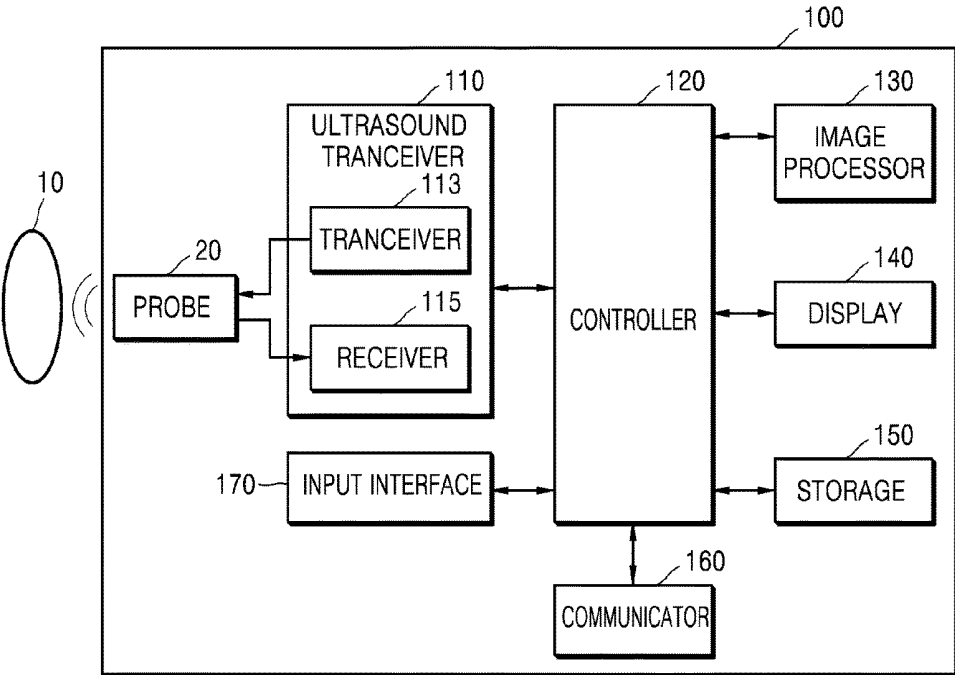


FIG. 2C

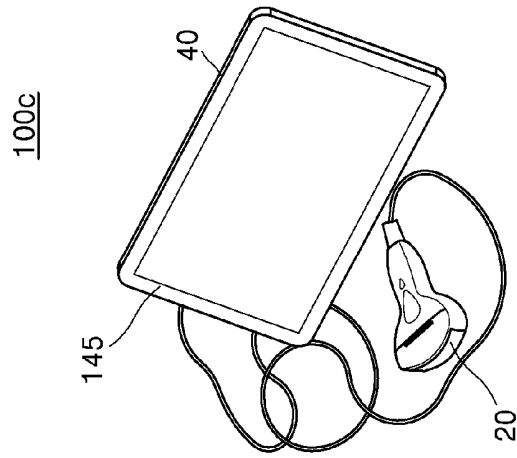


FIG. 2B

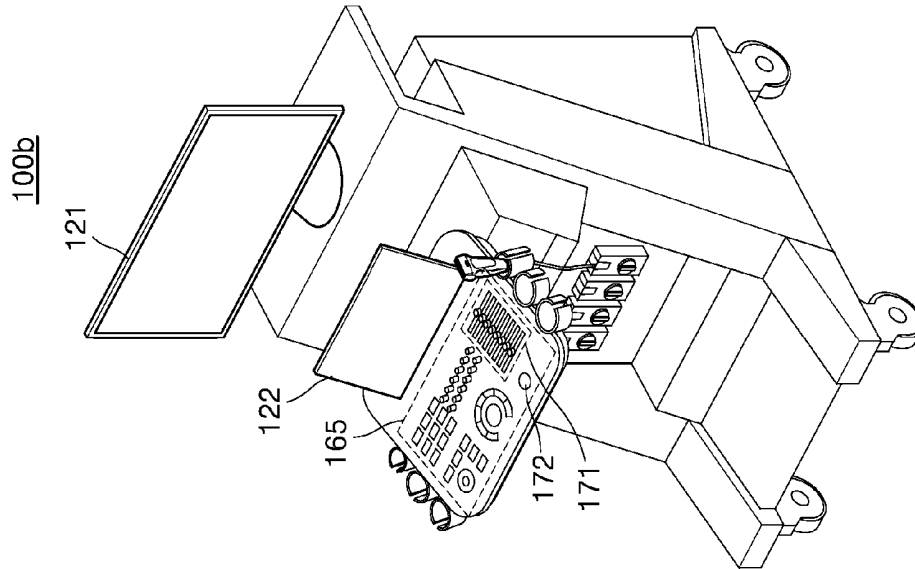
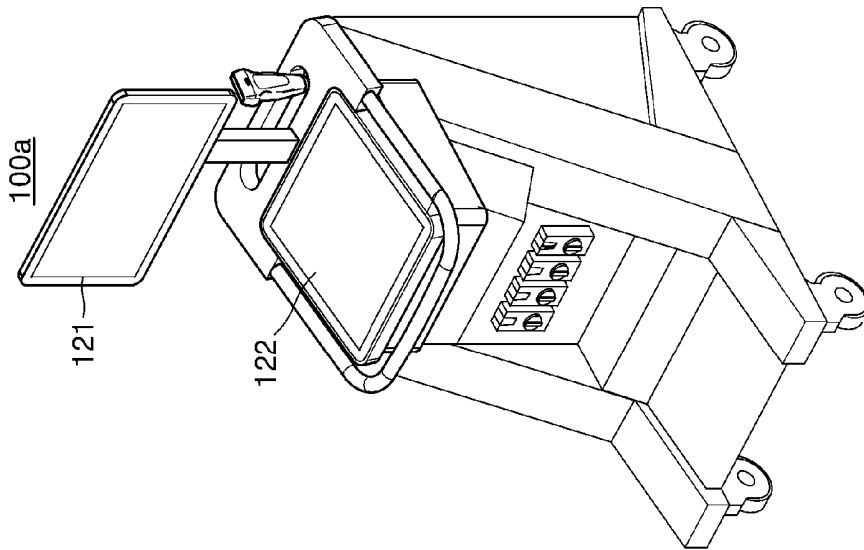


FIG. 2A



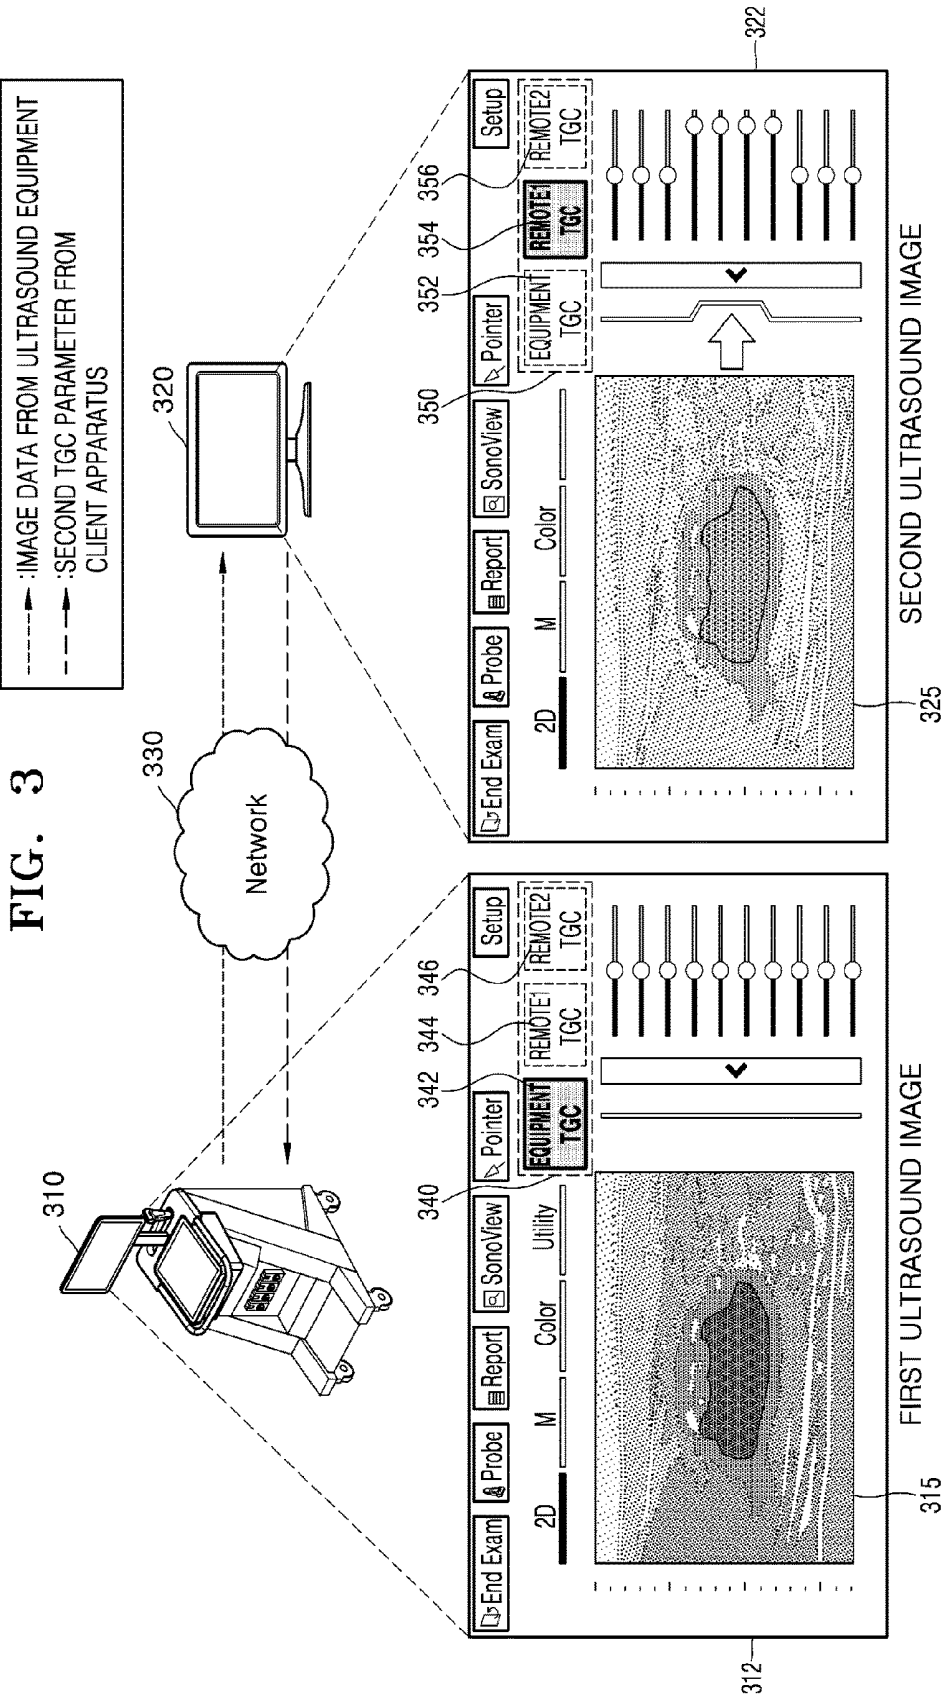


FIG. 4

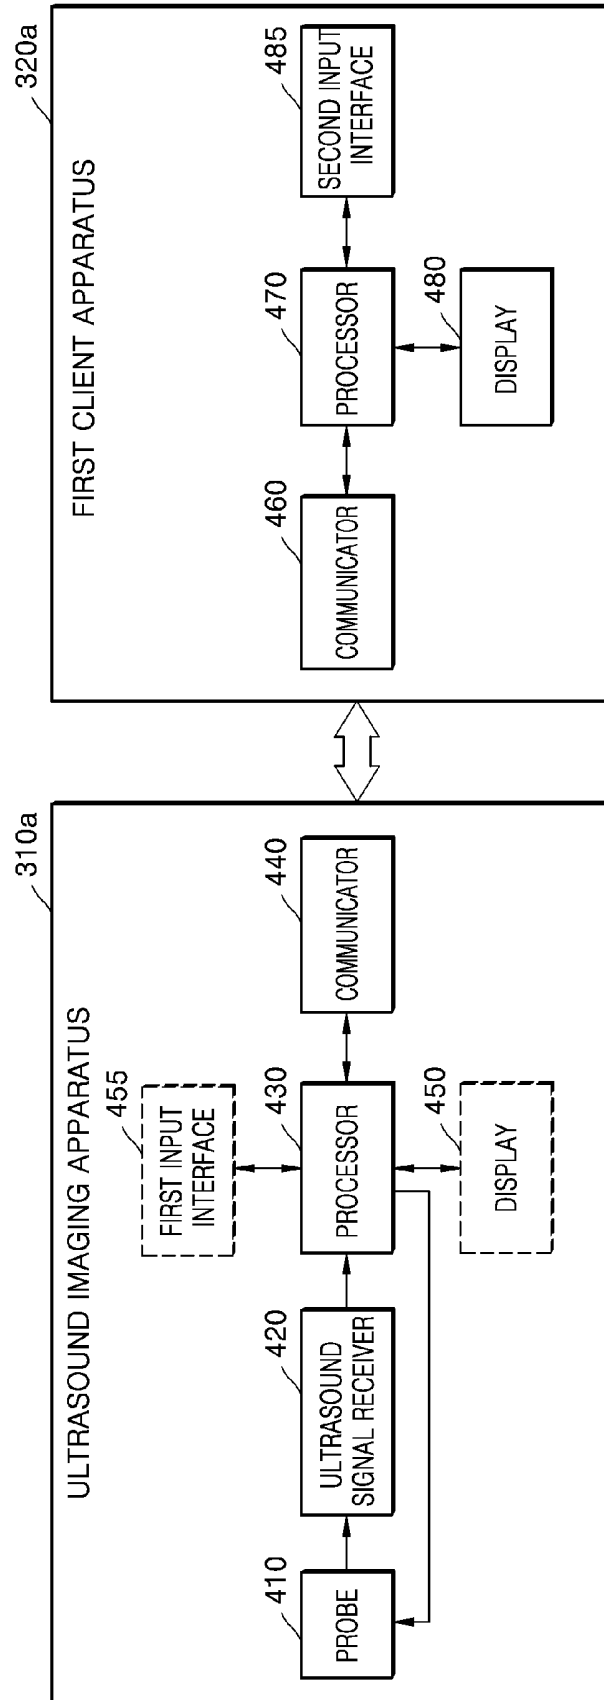


FIG. 5

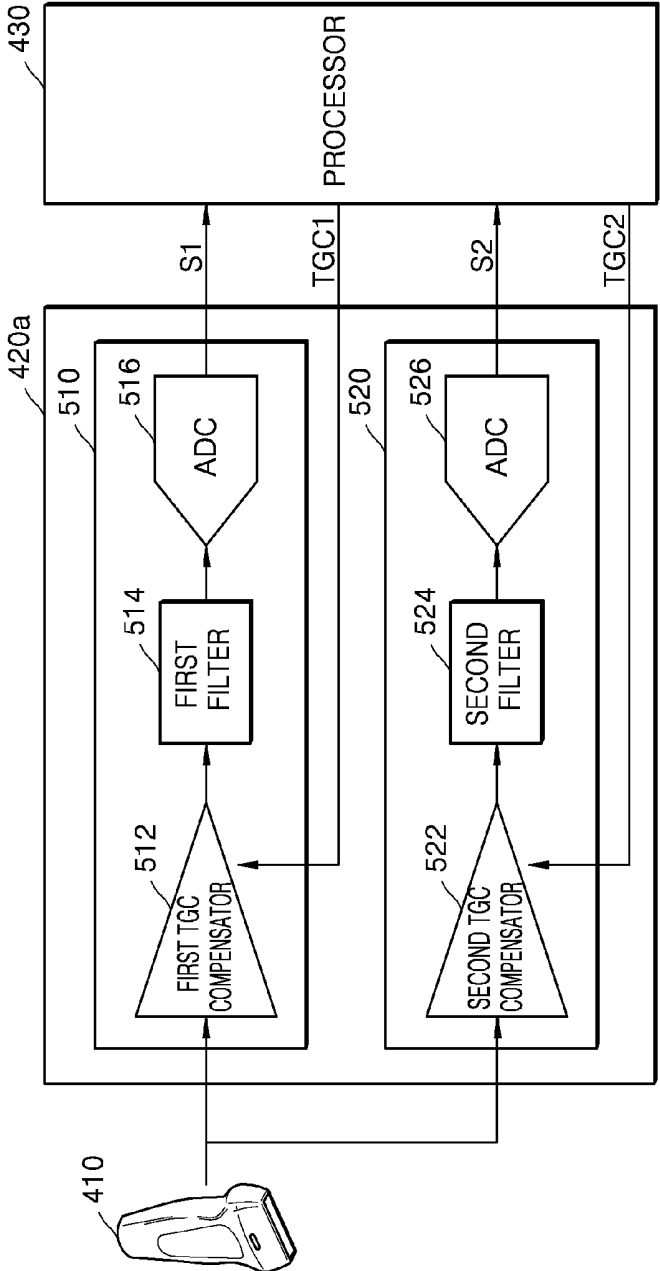


FIG. 6

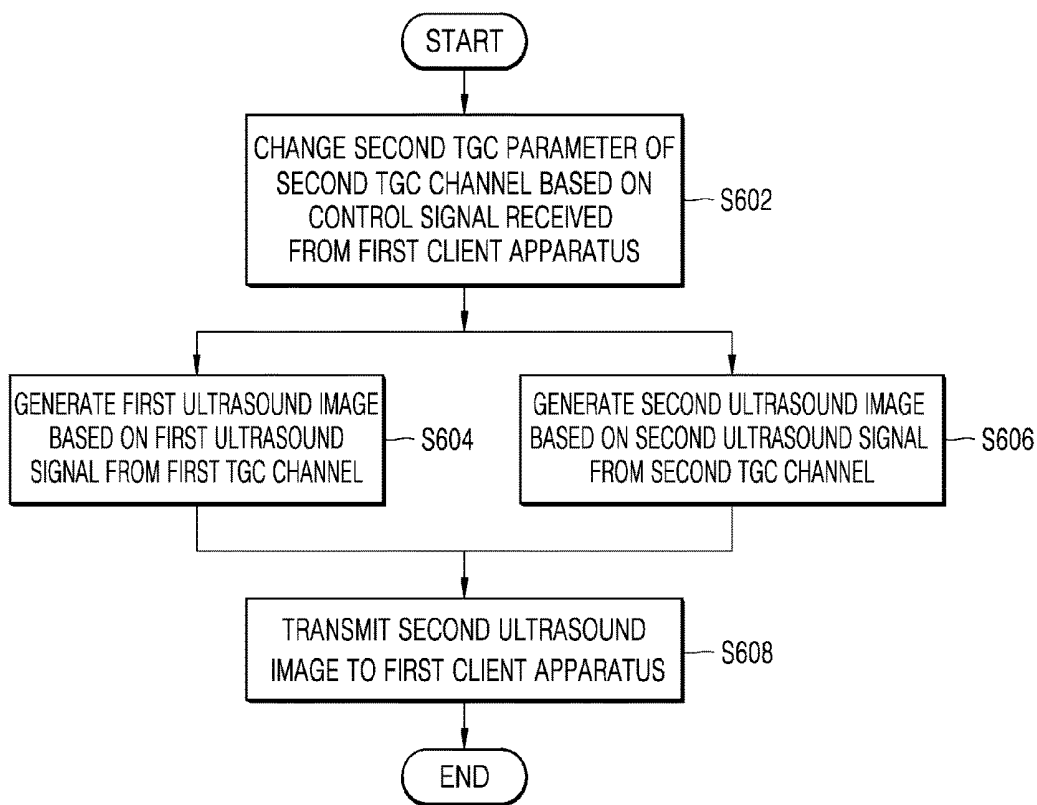


FIG. 7

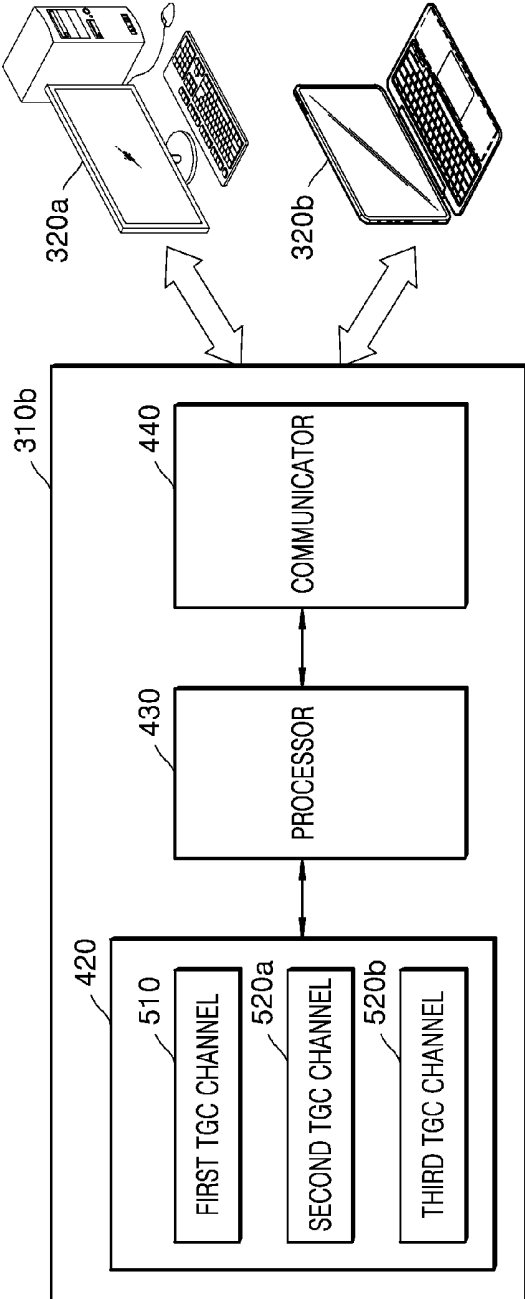


FIG. 8

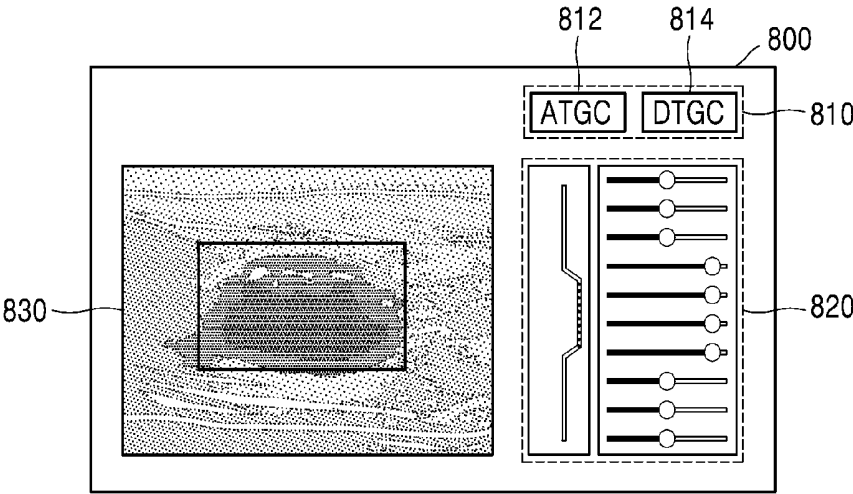


FIG. 9

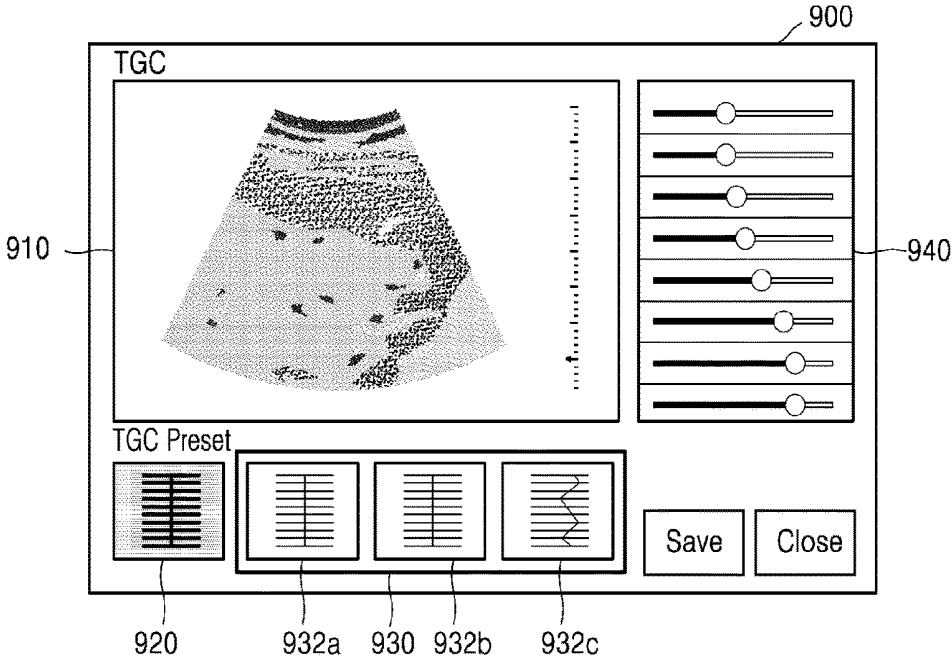


FIG. 10

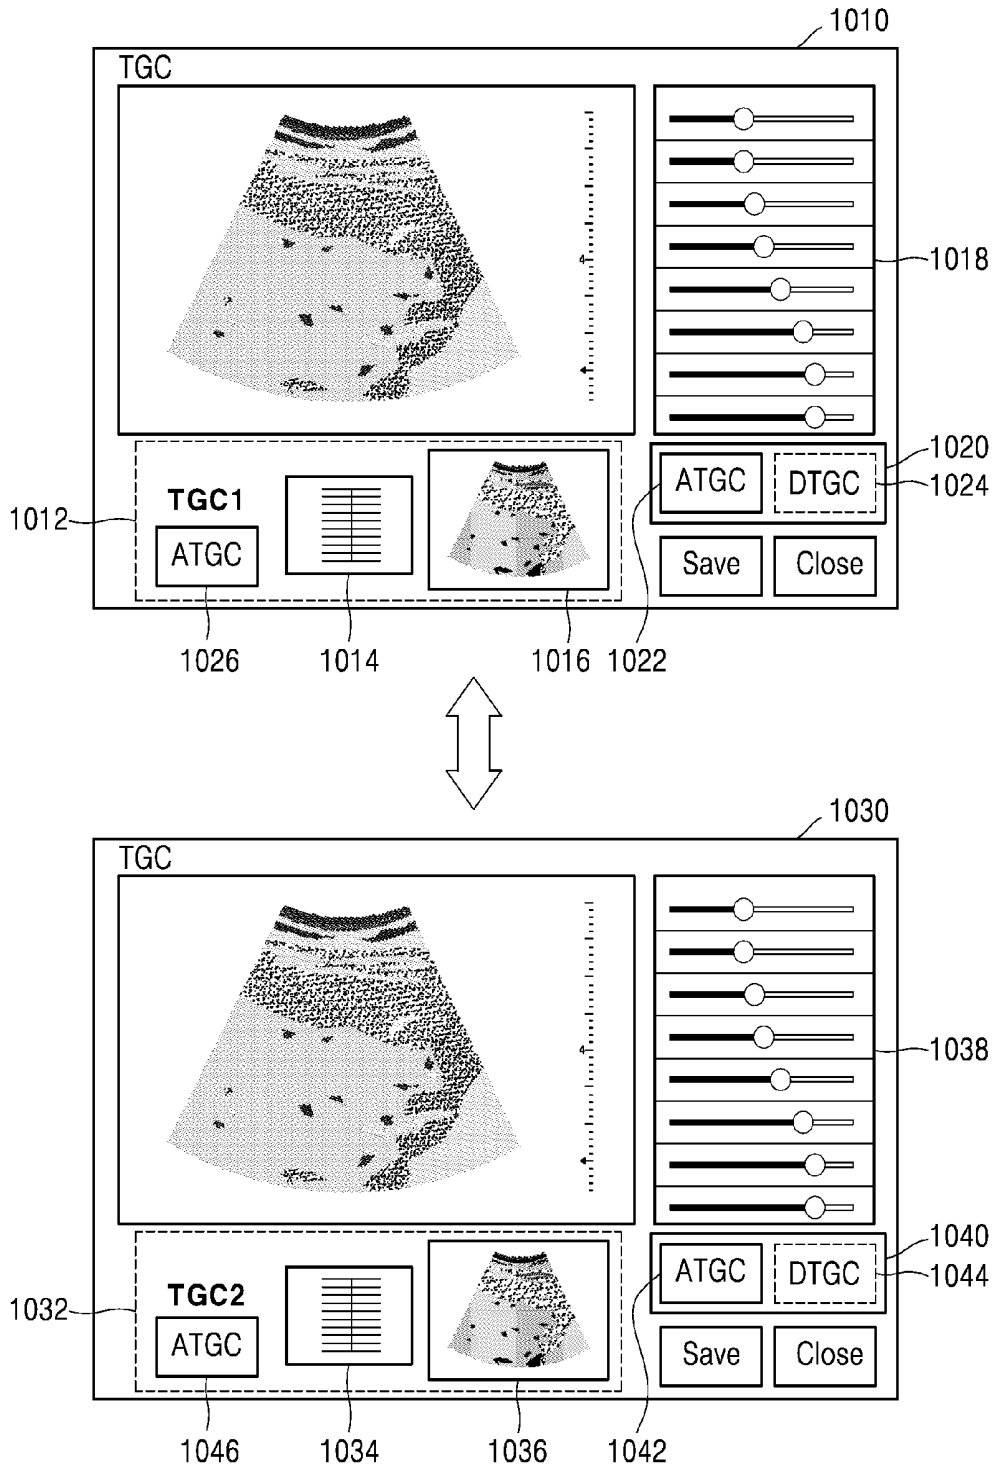


FIG. 11

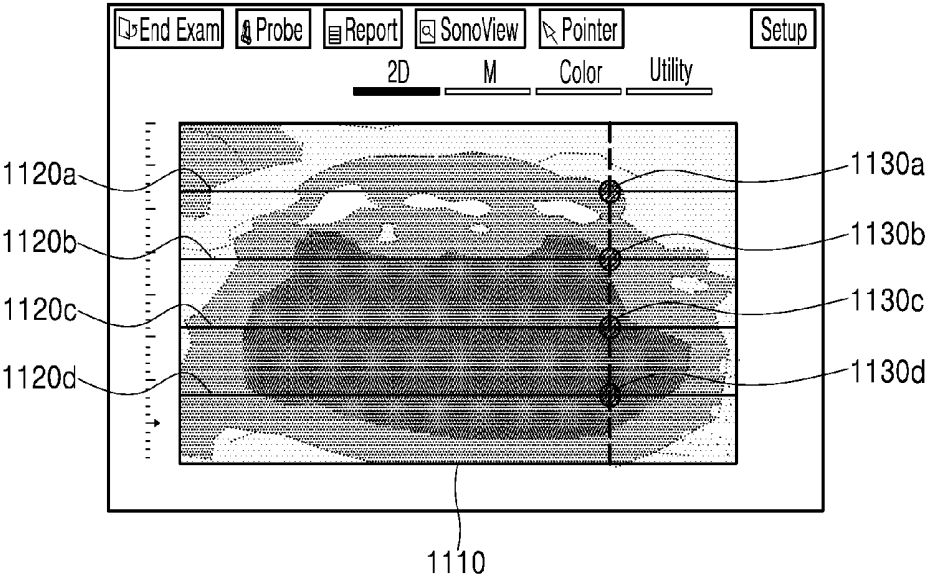


FIG. 12

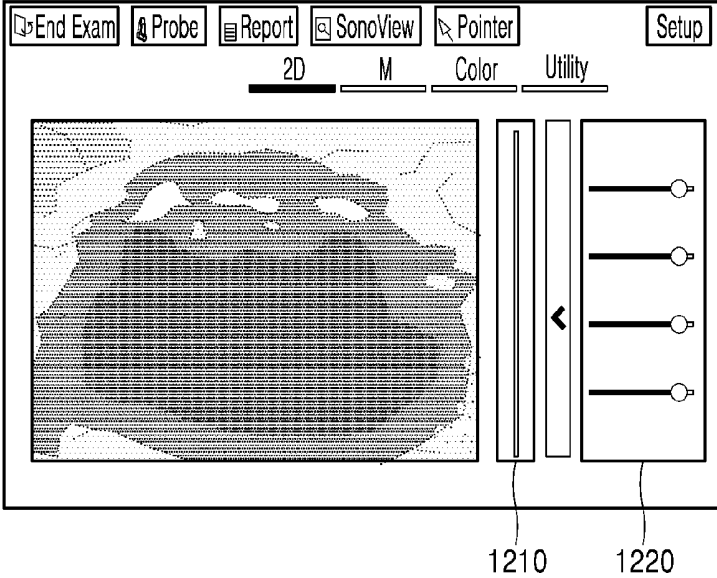


FIG. 13


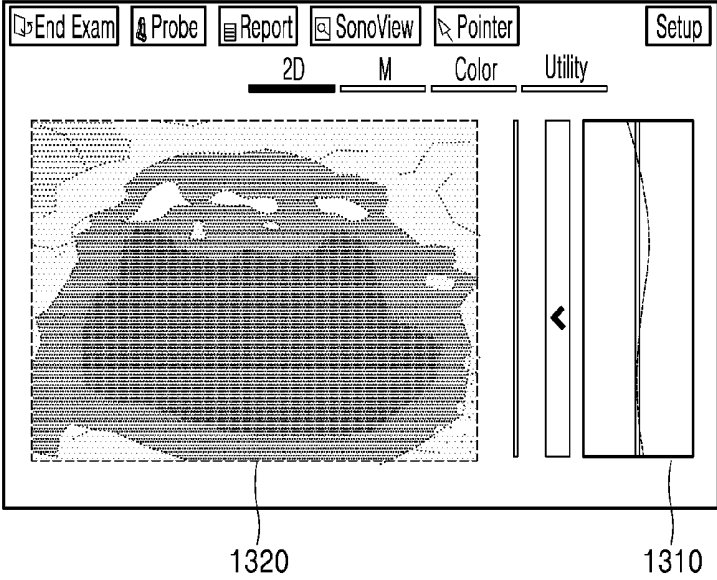


FIG. 14

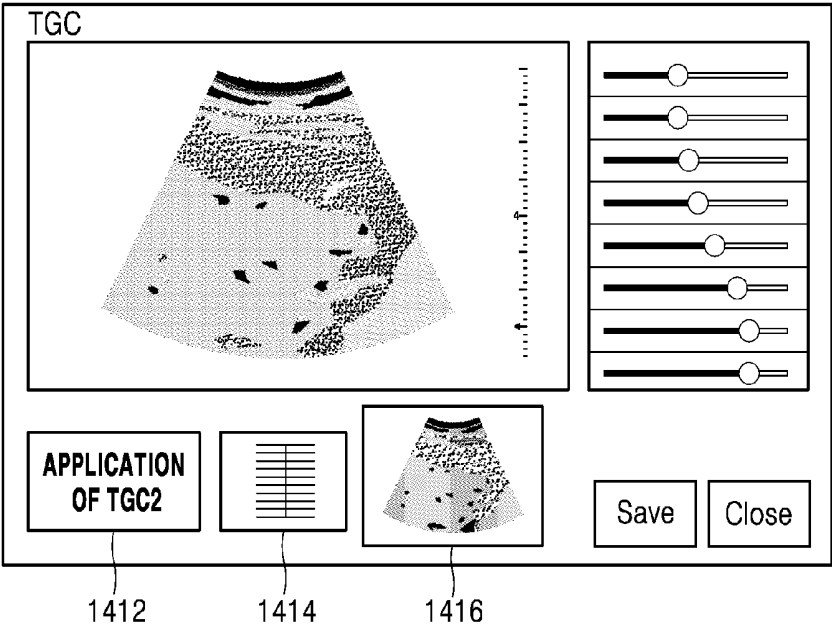

**ULTRASOUND IMAGING APPARATUS,
METHOD OF CONTROLLING THE SAME,
AND COMPUTER PROGRAM PRODUCT**

CROSS-REFERENCE TO RELATED
APPLICATION(S)

[0001] This application is based on and claims priority under 35 U.S.C. § 119 to Korean Patent Application No. 10-2018-0018064, filed on Feb. 13, 2018, in the Korean Intellectual Property Office, the disclosure of which is incorporated by reference herein in its entirety.

BACKGROUND

1. Field

[0002] The disclosure relates to ultrasound imaging apparatuses, methods of controlling the same, and a computer program product.

2. Description of Related Art

[0003] Ultrasound diagnosis apparatuses transmit ultrasound signals generated by transducers of a probe to an object and receive information of signals reflected from the object, thereby obtaining at least one image of an internal part (e.g., soft tissues or blood flow) of the object.

SUMMARY

[0004] Provided are methods and apparatuses that allow a client apparatus to control a time gain compensation (TGC) parameter of an ultrasound imaging apparatus.

[0005] Provided are methods and apparatuses that allow a client apparatus to adjust an analog TGC parameter and separately generate and provide an image to an ultrasound imaging apparatus and an image to the client apparatus.

[0006] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0007] In accordance with an aspect of the disclosure, an ultrasound imaging apparatus includes: a probe including a transducer array; an ultrasound signal receiver including a first TGC channel and a second TGC channel that each perform TGC on an ultrasound signal received from the probe; a communicator configured to communicate with a first client apparatus; and one or more processors configured to change a second TGC parameter of the second TGC channel, based on a control signal received from the first client apparatus, generate a second ultrasound image based on a second ultrasound signal produced via the second TGC channel, and transmit the second ultrasound image to the first client apparatus via the communicator.

[0008] The one or more processors may be further configured to generate a first ultrasound image based on a first ultrasound signal produced via the first TGC channel and display the first ultrasound image on a display.

[0009] The first TGC channel may include a first TGC compensator configured to compensate for an echo signal received from the probe by applying a first TGC set that is a set of gain values at reception depths,

[0010] The second TGC channel may include a second TGC compensator configured to compensate for an echo signal received from the probe by applying a second TGC set that is a set of gain values at reception depths. The first

TGC set may be determined based on a control signal received from the ultrasound imaging apparatus, and the second TGC set may be determined based on a control signal received from the first client apparatus.

[0011] The one or more processors may be further configured to generate a live streaming signal from the second ultrasound image and transmit the live streaming signal to the first client apparatus via the communicator.

[0012] The ultrasound signal receiver may further include a third TGC channel, and the one or more processors may be further configured to change a TGC parameter of the third TGC channel, based on a control signal received from a second client apparatus, generate a third ultrasound image based on a third ultrasound signal produced via the third TGC channel, and transmit the third ultrasound image to the second client apparatus via the communicator.

[0013] The first client apparatus may be configured to receive a selection signal for selecting one of analog TGC and digital TGC, and the one or more processors may be further configured to change, based on reception of the selection signal for selecting the analog TGC by the first client apparatus, the second TGC parameter of the second TGC channel, based on the control signal from the first client apparatus.

[0014] The one or more processors may be further configured to perform, based on reception of the selection signal for selecting the digital TGC by the first client apparatus, the digital TGC on the second ultrasound image based on a TGC parameter included in the control signal from the first client apparatus and transmit the second ultrasound image that has undergone the digital TGC to the first client apparatus via the communicator.

[0015] The one or more processors may be further configured to provide via a display at least one or a combination of information about a first TGC parameter of the first TGC channel, information about the second TGC parameter of the second TGC channel, and information about which TGC parameter is used to generate a displayed ultrasound image.

[0016] The one or more processors may be further configured to change a first TGC parameter based on the second TGC parameter in response to one of a control signal received from the ultrasound imaging apparatus and the control signal received from the first client apparatus.

[0017] The ultrasound imaging apparatus may further include a storage storing information about the second TGC parameter according to a user of the first client apparatus, and the one or more processors may be further configured to set, based on information about the user of the first client apparatus, the second TGC parameter of the second TGC channel to be the second TGC parameter according to the user of the first client apparatus.

[0018] In accordance with another aspect of the disclosure, a method of controlling an ultrasound imaging apparatus including a first TGC channel and a second TGC channel that each perform TGC on an ultrasound signal received via a probe includes: changing a second TGC parameter of the second TGC channel, based on a control signal received from the first client apparatus; generating a second ultrasound image based on a second ultrasound signal produced via the second TGC channel; and transmitting the second ultrasound image to the first client apparatus.

[0019] In accordance with another aspect of the disclosure, a computer program product includes a non-transitory computer-readable recording medium having stored therein

a computer program code for performing a method of controlling an ultrasound imaging apparatus.

BRIEF DESCRIPTION OF THE DRAWINGS

[0020] The above and other aspects, features, and advantages of certain embodiments of the present disclosure will be more apparent from the following description taken in conjunction with the accompanying drawings, in which:

[0021] FIG. 1 is a block diagram of a configuration of an ultrasound diagnosis apparatus according to an embodiment;

[0022] FIGS. 2A through 2C respectively illustrate ultrasound diagnosis apparatuses according to embodiments;

[0023] FIG. 3 illustrates an ultrasound imaging apparatus and a client apparatus according to an embodiment;

[0024] FIG. 4 illustrates a structure of an ultrasound imaging apparatus and a first client apparatus, according to an embodiment;

[0025] FIG. 5 illustrates a structure of an ultrasound signal receiver according to an embodiment;

[0026] FIG. 6 is a flowchart of a method of controlling an ultrasound imaging apparatus, according to an embodiment;

[0027] FIG. 7 illustrates an ultrasound imaging apparatus and a plurality of client apparatuses according to an embodiment;

[0028] FIG. 8 illustrates a graphical user interface (GUI) view provided by a client apparatus, according to an embodiment;

[0029] FIG. 9 illustrates a GUI view for time gain compensation (TGC) control of an ultrasound imaging apparatus or a client apparatus, according to an embodiment;

[0030] FIG. 10 illustrates GUI views for TGC control of an ultrasound imaging apparatus and a client apparatus, according to an embodiment;

[0031] FIG. 11 illustrates a GUI view for TGC control of an ultrasound imaging apparatus or a client apparatus, according to an embodiment;

[0032] FIG. 12 illustrates a GUI view for TGC control of an ultrasound imaging apparatus or a client apparatus, according to an embodiment;

[0033] FIG. 13 illustrates a GUI view for TGC control of an ultrasound imaging apparatus or a client apparatus, according to an embodiment; and

[0034] FIG. 14 illustrates a GUI view for TGC control of an ultrasound imaging apparatus, according to an embodiment.

DETAILED DESCRIPTION

[0035] Embodiments are described in greater detail below with reference to the accompanying drawings.

[0036] In the following description, the same drawing reference numerals are used for the same elements even in different drawings. The matters defined in the description, such as detailed construction and elements, are provided to assist in a comprehensive understanding of exemplary embodiments. Thus, it is apparent that exemplary embodiments can be carried out without those specifically defined matters. Also, well-known functions or constructions are not described in detail since they would obscure embodiments with unnecessary detail.

[0037] Terms such as “part” and “portion” used herein denote those that may be embodied by software or hardware. According to embodiments, a plurality of parts or portions

may be embodied by a single unit or element, or a single part or portion may include a plurality of elements.

[0038] In embodiments, an image may include any medical image acquired by various medical imaging apparatuses such as a magnetic resonance imaging (MRI) apparatus, a computed tomography (CT) apparatus, an ultrasound imaging apparatus, or an X-ray apparatus.

[0039] Also, in the present specification, an “object”, which is a thing to be imaged, may include a human, an animal, or a part thereof. For example, an object may include a part of a human, that is, an organ or a tissue, or a phantom.

[0040] Throughout the specification, an ultrasound image refers to an image of an object processed based on ultrasound signals transmitted to the object and reflected therefrom.

[0041] FIG. 1 is a block diagram illustrating a configuration of an ultrasound diagnosis apparatus 100, i.e., a diagnostic apparatus, according to an embodiment.

[0042] Referring to FIG. 1, the ultrasound diagnosis apparatus 100 may include a probe 20, an ultrasound transceiver 110, a controller 120, an image processor 130, one or more displays 140, a storage 150, e.g., a memory, a communicator 160, i.e., a communication device or an interface, and an input interface 170.

[0043] The ultrasound diagnosis apparatus 100 may be of a cart-type or a portable-type ultrasound diagnosis apparatus which is portable, moveable, mobile, or hand-held. Examples of the portable-type ultrasound diagnosis apparatus may include a smart phone, a laptop computer, a personal digital assistant (PDA), and a tablet personal computer (PC), each of which may include a probe and a software application, but embodiments are not limited thereto.

[0044] The probe 20 may include a plurality of transducers. The plurality of transducers may transmit ultrasound signals to an object 10 in response to transmitting signals received by the probe 20, from a transmitter 113. The plurality of transducers may receive ultrasound signals reflected from the object 10 to generate reception signals. In addition, the probe 20 and the ultrasound diagnosis apparatus 100 may be formed in one body (e.g., disposed in a single housing), or the probe 20 and the ultrasound diagnosis apparatus 100 may be formed separately (e.g., disposed separately in separate housings) but linked wirelessly or via wires. In addition, the ultrasound diagnosis apparatus 100 may include one or more probes 20 according to embodiments.

[0045] The controller 120 may control the transmitter 113 for the transmitter 113 to generate transmitting signals to be applied to each of the plurality of transducers based on a position and a focal point of the plurality of transducers included in the probe 20.

[0046] The controller 120 may control the receiver 115 to generate ultrasound data by converting reception signals received from the probe 20 from analogue to digital signals and summing the reception signals converted into digital form, based on a position and a focal point of the plurality of transducers.

[0047] The image processor 130 may generate an ultrasound image by using ultrasound data generated from the receiver 115.

[0048] The display 140 may display a generated ultrasound image and various pieces of information processed by the ultrasound diagnosis apparatus 100. The ultrasound diagnosis apparatus 100 may include two or more displays

140 according to the present embodiment. The display **140** may include a touch screen in combination with a touch panel.

[0049] The controller **120** may control the operations of the ultrasound diagnosis apparatus **100** and flow of signals between the internal elements of the ultrasound diagnosis apparatus **100**. The controller **120** may include a memory for storing a program or data to perform functions of the ultrasound diagnosis apparatus **100** and a processor and/or a microprocessor (not shown) for processing the program or data. For example, the controller **120** may control the operation of the ultrasound diagnosis apparatus **100** by receiving a control signal from the input interface **170** or an external apparatus.

[0050] The ultrasound diagnosis apparatus **100** may include the communicator **160** and may be connected to external apparatuses, for example, servers, medical apparatuses, and portable devices such as smart phones, tablet personal computers (PCs), wearable devices, etc., via the communicator **160**.

[0051] The communicator **160** may include at least one element capable of communicating with the external apparatuses. For example, the communicator **160** may include at least one among a short-range communication module, a wired communication module, and a wireless communication module.

[0052] The communicator **160** may receive a control signal and data from an external apparatus and transmit the received control signal to the controller **120** so that the controller **120** may control the ultrasound diagnosis apparatus **100** in response to the received control signal.

[0053] The controller **120** may transmit a control signal to the external apparatus via the communicator **160** so that the external apparatus may be controlled in response to the control signal of the controller **120**.

[0054] For example, the external apparatus connected to the ultrasound diagnosis apparatus **100** may process the data of the external apparatus in response to the control signal of the controller **120** received via the communicator **160**.

[0055] A program for controlling the ultrasound diagnosis apparatus **100** may be installed in the external apparatus. The program may include command languages to perform part of operation of the controller **120** or the entire operation of the controller **120**.

[0056] The program may be pre-installed in the external apparatus or may be installed by a user of the external apparatus by downloading the program from a server that provides applications. The server that provides applications may include a recording medium where the program is stored.

[0057] The storage **150** may store various data or programs for driving and controlling the ultrasound diagnosis apparatus **100**, input and/or output ultrasound data, ultrasound images, applications, etc.

[0058] The input interface **170** may receive a user's input to control the ultrasound diagnosis apparatus **100** and may include a keyboard, button, keypad, mouse, trackball, jog switch, knob, a touchpad, a touch screen, a microphone, a motion input means, a biometrics input means, etc. For example, the user's input may include inputs for manipulating buttons, keypads, mice, trackballs, jog switches, or knobs, inputs for touching a touchpad or a touch screen, a voice input, a motion input, and a bioinformation input, for

example, iris recognition or fingerprint recognition, but an embodiment is not limited thereto.

[0059] An example of the ultrasound diagnosis apparatus **100** according to the present embodiment is described below with reference to FIGS. 2A, 2B, and 2C.

[0060] FIGS. 2A, 2B, and 2C are diagrams illustrating ultrasound diagnosis apparatuses according to embodiments.

[0061] Referring to FIGS. 2A and 2B, an ultrasound diagnosis apparatus **100a** or **100b** may include a main display **121** and a sub-display **122**. At least one among the main display **121** and the sub-display **122** may include a touch screen. The main display **121** and the sub-display **122** may display ultrasound images and/or various information processed by the ultrasound diagnosis apparatus **100a** or **100b**. The main display **121** and the sub-display **122** may provide graphical user interfaces (GUI), thereby receiving user's inputs of data to control the ultrasound diagnosis apparatus **100a** or **100b**. For example, the main display **121** may display an ultrasound image and the sub-display **122** may display a control panel to control display of the ultrasound image as a GUI. The sub-display **122** may receive an input of data to control the display of an image through the control panel displayed as a GUI. The ultrasound diagnosis apparatus **100a** or **100b** may control the display of the ultrasound image on the main display **121** by using the input control data.

[0062] Referring to FIG. 2B, the ultrasound diagnosis apparatus **100b** may include a control panel **165**. The control panel **165** may include buttons, trackballs, jog switches, or knobs, and may receive data to control the ultrasound diagnosis apparatus **100b** from the user. For example, the control panel **165** may include a time gain compensation (TGC) button **171** and a freeze button **172**. The TGC button **171** is to set a TGC value for each depth of an ultrasound image. Also, when an input of the freeze button **172** is detected during scanning an ultrasound image, the ultrasound diagnosis apparatus **100b** may keep displaying a frame image at that time point.

[0063] The buttons, trackballs, jog switches, and knobs included in the control panel **165** may be provided as a GUI to the main display **121** or the sub-display **122**.

[0064] Referring to FIG. 2C, the ultrasound diagnosis apparatus **100c** may be implemented as a portable ultrasound diagnosis apparatus. An example of the portable ultrasound diagnosis apparatus may include, for example, smart phones including probes and applications, laptop computers, personal digital assistants (PDAs), or tablet PCs, but an embodiment is not limited thereto.

[0065] The ultrasound diagnosis apparatus **100c** may include the probe **20** and a main body **40**. The probe **20** may be connected to one side of the main body **40** by wire or wirelessly. The main body **40** may include a touch screen **145**. The touch screen **145** may display an ultrasound image, various pieces of information processed by the ultrasound diagnosis apparatus **100c**, and a GUI.

[0066] FIG. 3 illustrates an ultrasound imaging apparatus and a client apparatus according to an embodiment.

[0067] Referring to FIG. 3, an ultrasound imaging apparatus **310** transmits ultrasound signals generated by transducers of a probe to an affected area of a patient and receives information regarding ultrasound signals reflected from the patient to thereby reconstruct an image of a part or organ of the patient. When an ultrasound signal is transmitted to an

affected area via a probe, the intensity of the ultrasound signal decreases with depth in the human body due to characteristics of ultrasound waves. TGC is used to compensate for the decreased intensity of the ultrasound signal. TGC is a method that uses preset values to vary the degree of compensation according to the time elapsed from the start of transmission of an ultrasound signal. The ultrasound signal, attenuation of which is compensated by the TGC, may then be converted into digital data by an analog-to-digital converter (ADC), and an image of an internal body part of a patient may be obtained based on the digital data.

[0068] The obtained image may be displayed on a display, be stored in the ultrasound imaging apparatus 310, or be transmitted to a server or a client apparatus 320. The client apparatus 320 may be used by a user, such as a medical doctor, to receive and view an ultrasound image.

[0069] The ultrasound imaging apparatus 310 has a live streaming function and may transmit an ultrasound image over a network 330 to provide the ultrasound image in real-time to the client apparatus 320 at a remote location. A live streaming technology may be used to provide various types of multimedia digital information such as video, audio, etc. to users who use external devices connected to a network such as the Internet. The users of the external devices may use live streaming functions to play back files such as video, audio, and the like in real-time on the Internet without downloading the files onto a hard disk drive.

[0070] Regarding the ultrasound imaging apparatus 310, a live streaming technology is used to transmit in real-time an ultrasound image being captured by the ultrasound imaging apparatus 310 to the client apparatus 320 at the remote location. By using the live streaming function provided by the ultrasound imaging apparatus 310, a user of the client apparatus 320 (e.g., a medical doctor) may view in real-time a video including ultrasound images of the internal body part of the patient that are being captured even when the user is not in an examination room where the patient is having an ultrasound scan. In detail, the user who uses the client apparatus 320 may quickly diagnose a disease of the patient based on the live streaming video including the ultrasound images provided via the client apparatus 320 and give feedback with respect to an imaged part or whether another scan of the patient is necessary.

[0071] During live streaming of an ultrasound image, when a TGC setting needs to be changed due to a failure of an operator of the ultrasound imaging apparatus 310 to properly use the ultrasound imaging apparatus, the user of the client apparatus 320 may induce a user of the ultrasound imaging apparatus 310 to change the TGC setting by using a voice call, etc. However, when the user of the client apparatus 320 instructs the user of the ultrasound imaging apparatus 310 to change a TGC setting in this way, the intention of the user of the client apparatus 320 may not be properly delivered to the user of the ultrasound imaging apparatus 310, and changing the TGC setting indirectly via the user of the ultrasound imaging apparatus 310 may be inconvenient. Another inconvenience may arise from a difference between TGC settings respectively desired by the user of the ultrasound imaging apparatus 310 and the user of the client apparatus 320. According to an embodiment, the ultrasound imaging apparatus 310 may allow the user of the client apparatus 320 to directly change the TGC setting of the ultrasound imaging apparatus 310. Furthermore, according to embodiments, the ultrasound imaging apparatus 310

may provide a first ultrasound image 315 generated by applying a first TGC set while the client apparatus 320 may provide a second ultrasound image generated by applying a second TGC set.

[0072] In an embodiment, TGC settings are settings with respect to parameters related to a TGC function and include settings for gain values at reception depths. Furthermore, TGC parameters are parameters related to the TGC function and include gain values at the reception depths. A TGC set is a set of TGC parameters and includes a set of gain values at reception depths.

[0073] Embodiments may be applied to both TGC control and lateral gain compensation (LGC) control. LGC is a technique of varying the degree of compensation according to a lateral position. Analog LGC may be performed by applying, depending on a position of a transducer element, different gains to signals respectively detected by individual transducer elements or to sums of signals respectively detected by a predetermined number of transducer element arrays. Digital LGC may be performed by applying different gains according to a lateral position in an ultrasound image. The descriptions presented with respect to TGC may be also valid with respect to LGC. In an embodiment, the ultrasound imaging apparatus 310 may receive a control signal for setting an LGC parameter from the client apparatus 320 and perform an analog LGC operation based on LGC parameters received from the client apparatus 320.

[0074] According to an embodiment, the ultrasound imaging apparatus 310 may be connected to the client apparatus 320 via the network 330. The ultrasound imaging apparatus 310 may exchange data and a control signal with the client apparatus 320 via the network 330.

[0075] The network 330 may use various types of wired or wireless communication techniques. The ultrasound imaging apparatus 310 and the client apparatus 320 may be in the same room or be located in different rooms or buildings. Furthermore, the ultrasound imaging apparatus 310 may be connected to the client apparatus 320 directly or via a server.

[0076] According to an embodiment, the client apparatus 320 may adjust a TGC parameter of the ultrasound imaging apparatus 310. The client apparatus 320 may set the TGC parameter of the ultrasound imaging apparatus 310 via a UI for a TGC setting of the client apparatus 320. The ultrasound imaging apparatus 310 adjusts the TGC parameter based on a TGC setting control signal received from the client apparatus 320. According to an embodiment, the ultrasound imaging apparatus 310 may control an analog TGC parameter based on a control signal received from the client apparatus 320.

[0077] The ultrasound imaging apparatus 310 may generate the first ultrasound image 315 by using a first TGC parameter set in the ultrasound imaging apparatus 310 and display the first ultrasound image 315 via the ultrasound imaging apparatus 310. The ultrasound imaging apparatus 310 may generate a second ultrasound image 325 by using a second TGC parameter and transmit the second ultrasound image 325 to the client apparatus 320.

[0078] According to an embodiment, the ultrasound imaging apparatus 310 may provide information indicating an apparatus that has a setting used to generate an image currently being displayed on a UI view 312. The UI view 312 of the ultrasound imaging apparatus 310 may include a first region 340 that provides information indicating an apparatus that has a setting used to generate an ultrasound

image. In an embodiment, the first region 340 may include an icon 342 corresponding to the ultrasound imaging apparatus 310 and icons 344 and 346 respectively corresponding to at least one client apparatus 320. The ultrasound imaging apparatus 310 may display an ultrasound image generated based on a setting of an apparatus corresponding to the icon 342, 344, or 346 that is selected in response to a control signal for selecting one of the icons 342, 344, and 346. In an embodiment, when the user selects the icon 342, the ultrasound imaging apparatus 310 may display the first ultrasound image 315 based on its TGC setting. When the user selects the icon 344, the ultrasound imaging apparatus 310 may display a second ultrasound image based on a TGC setting of a first client apparatus. When the user selects the icon 346, the ultrasound imaging apparatus 310 may display a third ultrasound image based on a TGC setting of a second client apparatus.

[0079] According to an embodiment, the client apparatus 320 may provide information indicating an apparatus having a setting that is used to generate an image currently being displayed on a UI view 322. The UI view 322 of the client apparatus 320 may include a second region 350 that provides information indicating an apparatus having a setting that is used to generate an ultrasound image. In an embodiment, the second region 350 may include an icon 354 corresponding to the client apparatus 320, an icon 352 corresponding to the ultrasound imaging apparatus 310, and an icon 356 corresponding to another client apparatus. The client apparatus 320 may display an ultrasound image generated based on a setting of an apparatus corresponding to the icon 352, 354, or 356 that is selected in response to a control signal for selecting one of the icons 352, 354, and 356. In an embodiment, when the user selects the icon 352, the client apparatus 320 may display a first ultrasound image 315 based on a TGC setting of the ultrasound imaging apparatus 310. When the user selects the icon 354, the client apparatus 320 may display a second ultrasound image 325 based on its TGC setting. When the user selects the icon 356, the client apparatus 320 may display a third ultrasound image based on a TGC setting of the other client apparatus.

[0080] FIG. 4 illustrates a structure of an ultrasound imaging apparatus and a first client apparatus, according to an embodiment.

[0081] Referring to FIG. 4, an ultrasound imaging apparatus 310a may include a probe 410, an ultrasound signal receiver 420, a processor 430, and a communicator 440. According to an embodiment, the ultrasound imaging apparatus 310a may further include a display 450.

[0082] The probe 410 includes a plurality of transducers and transmits ultrasound signals to an object and detects echo signals reflected from the object. The probe 410 may correspond to the probe 20 described with reference to FIG. 1.

[0083] The ultrasound signal receiver 420 receives ultrasound signals generated by the probe 410 to perform operations such as compensation, filtering, and analog-to-digital conversion on the ultrasound signals, and converts the ultrasound signals into digital signals to output the digital signals to the processor 430. The ultrasound signals are electrical signals generated and output by the probe 410. The ultrasound signal receiver 420 may correspond to the receiver 115 described with reference to FIG. 1. According to an embodiment, the ultrasound signal receiver 420 may include a plurality of TGC channels. In an embodiment, the

ultrasound signal receiver 420 may include first and second TGC channels. The first TGC channel may generate a first ultrasound signal by applying a first TGC parameter to a signal received from the probe 410. The second TGC channel may generate a second ultrasound signal by applying a second TGC parameter to a signal received from the probe 410. The ultrasound signal receiver 420 may output the first and second ultrasound signals to the processor 430.

[0084] The processor 430 controls all operations of the ultrasound imaging apparatus 310a. The processor 430 may be implemented as one or more processors.

[0085] The processor 430 receives an ultrasound signal from the ultrasound signal receiver 420 to reconstruct an ultrasound image. According to an embodiment, the processor 430 may respectively generate first and second ultrasound images based on the first and second ultrasound signals received from the ultrasound signal receiver 420.

[0086] Furthermore, the processor 430 controls a TGC parameter of the first TGC channel based on a TGC control signal received from the ultrasound imaging apparatus 310a, and a TGC parameter of the second TGC channel based on a control signal received from a first client apparatus 320a.

[0087] The processor 430 sets a TGC parameter of the first TGC channel based on a control signal received from the ultrasound imaging apparatus 310a. In an embodiment, the ultrasound imaging apparatus 310a may include an input interface and set a TGC parameter of the first TGC channel based on a control signal received via the input interface. Furthermore, the processor 430 may provide a UI for setting a TGC parameter in the ultrasound imaging apparatus 310a and set the TGC parameter of the first TGC channel based on a control signal input via the UI. The processor 430 may perform analog TGC based on a TGC control signal received from the first client apparatus 320a by separately controlling TGC parameters of the first and second TGC channels.

[0088] The processor 430 may determine a gain value at each reception depth based on a TGC control signal received from the ultrasound imaging apparatus 310a and adjust a compensation value from a compensator, which corresponds to each reception depth for the first TGC channel, to control the first TGC parameter. Furthermore, the processor 430 may determine a gain value at each reception depth based on a TGC control signal received from the first client apparatus 320a and adjust a compensation value from a compensator, which corresponds to each reception depth for the second TGC channel, to control the second TGC parameter.

[0089] Furthermore, the processor 430 may provide a UI for TGC control in the ultrasound imaging apparatus 310a. The processor 430 may provide a GUI for TGC control via the display 450 of the ultrasound imaging apparatus 310a. According to an embodiment, the ultrasound imaging apparatus 310a is equipped with a touch screen, and the processor 430 may provide a GUI for TGC control via the touch screen and receive a TGC control signal via the touch screen.

[0090] According to an embodiment, the processor 430 may provide and control a part of or all of a GUI for TGC control of the first client apparatus 320a. In an embodiment, the processor 430 may provide data, a control signal, a program code, a link address, etc. for constructing the GUI for TGC control to the first client apparatus 320a.

[0091] The communicator 440 communicates with the first client apparatus 320a. The communicator 440 may transmit or receive control signals and data to or from the first client apparatus 320a. The communicator 440 may

transmit a second ultrasound image to the first client apparatus **320a** and receive a TGC control signal from the first client apparatus **320a**. Furthermore, the communicator **440** may transmit a live streaming image to the first client apparatus **320a** as an ultrasound image.

[0092] The communicator **440** may perform local area communication and use communication technologies such as Bluetooth, Bluetooth low energy (BLE), near field communication (NFC), wireless LAN (WLAN), Wi-Fi, ZigBee, infrared data association (IrDA) communication, Wi-Fi Direct (WFD), ultra wideband (UWB), and Ant+. As another example, the communicator **440** may use a mobile communication method to transmit or receive wireless signals to or from at least one of a base station, an external terminal, and a server on a mobile communication network.

[0093] According to an embodiment, the ultrasound imaging apparatus **310a** may further include a first input interface **455**. The first input interface **455** may receive a control signal from the outside (e.g., a user). For example, the first input interface **455** may include at least one or a combination of a touch screen, a touch pad, a trackball, a knob, a dial, a keyboard, and a mouse. The first input interface **455** may correspond to the input interface described with reference to FIG. 1. The first input interface **455** may receive a TGC control signal for selecting a TGC parameter. The TGC control signal may be received in various forms, such as a control signal for selecting a TGC value according to a reception depth, a control signal for drawing a TGC curve, etc. An LGC control signal may be received in various forms, such as a control signal for selecting an LGC value according to a lateral position, a control signal for drawing an LGC curve, etc.

[0094] The first client apparatus **320a** includes a communicator **460**, a processor **470**, and a display **480**. For example, the first client apparatus **320a** may be formed as a smartphone, a tablet PC, a communication terminal, a PC, a kiosk, or the like.

[0095] The communicator **460** communicates with the ultrasound imaging apparatus **310a**. The communicator **460** may receive a second ultrasound image from the ultrasound imaging apparatus **310a** and transmit a control signal for setting a second TGC parameter to the ultrasound imaging apparatus **310a**. Furthermore, the communicator **460** may receive a live streaming signal with respect to the second ultrasound image from the ultrasound imaging apparatus **310a**. The communicator **460** may communicate with the ultrasound imaging apparatus **310a** wirelessly or by wire by using a communication method such as local area communication, mobile communication, etc.

[0096] The processor **470** controls all operations of the first client apparatus **320a**. The processor **470** may be implemented as one or more processors. The processor **470** may provide the second ultrasound image and a UI for TGC control via the display **480** of the client apparatus **320a**. For example, the display **480** may be formed as a touch screen, and the processor **470** may receive a user input for setting a second TGC parameter based on a touch input.

[0097] FIG. 5 illustrates a structure of an ultrasound signal receiver according to an embodiment.

[0098] According to an embodiment, an ultrasound signal receiver **420a** may include a plurality of TGC channels such as a first TGC channel **510** and a second TGC channel **520**. Each of the plurality of TGC channels performs TGC on an ultrasound signal received from the probe **410**. In detail, a

TGC channel may perform TGC by applying a different gain value to an ultrasound signal at each reception depth via a compensator. The TGC channel may perform analog TGC by compensating for an analog ultrasound signal. According to embodiments, the ultrasound signal receiver **420a** has the plurality of TGC channels that each perform analog TGC based on a control signal received from the first client apparatus (**320a** of FIG. 4) to thereby obtain a second ultrasound image that is different from a first ultrasound image for the ultrasound imaging apparatus (**310a** of FIG. 4).

[0099] The first TGC channel **510** may include a first TGC compensator **512**, a first filter **514**, and a first ADC **516**. The first TGC compensator **512** may perform an analog TGC operation by applying different gain values to an ultrasound signal received from the probe **410** according to a reception depth to thereby compensate for attenuation of the ultrasound signal. The first TGC compensator **512** may receive a first TGC parameter TGC1 from a processor **430** to perform the analog TGC operation based on the first TGC parameter TGC1. The first filter **514** performs an operation such as noise filtering with respect to a first ultrasound signal output from the first TGC compensator **512**. The first ADC **516** then performs analog-to-digital conversion with respect to a first ultrasound signal output from the first filter **514**. The first TGC channel **510** outputs first ultrasound signal S1 to the processor **430**.

[0100] The second TGC channel **520** may include a second TGC compensator **522**, a second filter **524**, and a second ADC **526**. The second TGC compensator **522** performs an analog TGC operation by applying different gain values to an ultrasound signal received from the probe **410** according to a reception depth to thereby compensate for attenuation of the ultrasound signal. The second TGC compensator **522** may receive a second TGC parameter TGC2 from the processor **430** to perform the analog TGC operation based on the second TGC parameter TGC2. The second filter **524** performs an operation such as noise filtering with respect to a second ultrasound signal output from the second TGC compensator **522**. The second ADC **526** then performs analog-to-digital conversion with respect to a second ultrasound signal output from the second filter **524**. The second TGC channel **520** outputs second ultrasound signal S2 to the processor **430**.

[0101] The ultrasound signal receiver **420a** may include three or more TGC channels according to an embodiment, and each TGC channel may correspond to a different apparatus.

[0102] When the present embodiment is applied to LGC, first and second LGC channels may be provided in the ultrasound signal receiver (**420** of FIG. 4). The first LGC channel may perform analog LGC based on a first LGC parameter set in the ultrasound imaging apparatus (**310** of FIG. 3), and the second LGC channel performs analog LGC based on a second LGC parameter received from the client apparatus (**320** of FIG. 3). Furthermore, the processor **430** may generate a first ultrasound image based on a first ultrasound signal that passed through the first TGC channel **510** and the first LGC channel, and a second ultrasound image based on a second ultrasound signal (that passed through the second TGC channel **520** and the second LGC channel).

[0103] FIG. 6 is a flowchart of a method of controlling an ultrasound imaging apparatus, according to an embodiment.

[0104] Operations of the method of FIG. 6 may be performed by an ultrasound imaging apparatus including a plurality of TGC channels and having a communication function that enables communication with a client apparatus. The specification mainly describes an embodiment in which an ultrasound imaging apparatus 310 (310 is hereinafter used as a reference numeral collectively denoting ultrasound imaging apparatuses disclosed herein) according to embodiments performs a method of controlling the ultrasound imaging apparatus. Thus, embodiments described with respect to the ultrasound imaging apparatus 310 may be applied to a method of controlling the ultrasound imaging apparatus 310, and embodiments described with respect to the method may be applied to the embodiments described with respect to the ultrasound imaging apparatus 310. A method of controlling the ultrasound imaging apparatus 310 according to embodiments is performed by the ultrasound imaging apparatus 310 described herein, but embodiments are not limited thereto. The method may be performed by various types of ultrasound imaging apparatuses.

[0105] The ultrasound imaging apparatus 310 receives a control signal for setting a second TGC parameter from the first client apparatus (320a of FIG. 4) and changes a TGC parameter of a second TGC channel based on the control signal received from the first client apparatus 320a (S602).

[0106] The ultrasound imaging apparatus 300 produces a first ultrasound signal via a first TGC channel by performing analog TGC based on a first TGC parameter set in the ultrasound imaging apparatus 310 and generates a first ultrasound image based on the first ultrasound signal (S604). The ultrasound imaging apparatus 310 may display the first ultrasound image on the display (450 of FIG. 4) of the ultrasound imaging apparatus 310.

[0107] The ultrasound imaging apparatus 310 produces a second ultrasound signal via a second TGC channel by performing analog TGC based on a second TGC parameter received from the first client apparatus 320a and generates a second ultrasound image based on the second ultrasound signal (S606).

[0108] The ultrasound imaging apparatus 310 transmits the second ultrasound image to the first client apparatus 320a (S608).

[0109] FIG. 7 illustrates an ultrasound imaging apparatus and a plurality of client apparatuses according to an embodiment.

[0110] According to an embodiment, an ultrasound imaging apparatus 310b may respectively transmit ultrasound images to and receive TGC parameters from a plurality of client apparatuses 320a and 320b. An ultrasound signal receiver 420 of the ultrasound imaging apparatus 310b may include three or more TGC channels. The ultrasound signal receiver 420 may include a plurality of TGC channels, i.e., first through third TGC channels 510, 520a, and 520b, and support a function of remotely performing analog TGC with respect to a number of client apparatuses. The number of client apparatus is one (1) less than the number of TGC channels. In an embodiment, when the ultrasound signal receiver 420 includes four (4) TGC channels that provide remote analog TGC functions with respect to three (3) client apparatuses. According to the embodiment of FIG. 7, the first TGC channel 510 may perform analog TGC based on a TGC parameter received from the ultrasound imaging apparatus 310b, and the second and third TGC channels 520a and 520b may respectively perform analog TGCs

based on TGC parameters received from the plurality of client apparatuses 320a and 320b.

[0111] A processor 430 may respectively assign the second and third TGC channels 520a and 520b to the plurality of client apparatuses 320a and 320b and transmit the TGC parameters respectively received from the plurality of client apparatuses 320a and 320b to the assigned second and third TGC channels 520a and 520b. Furthermore, when the client apparatus 320a or 320b is connected to the ultrasound imaging apparatus 310b, the processor 430 may assign a corresponding TGC channel 520a or 520b to the connected client apparatus 320a or 320b. On the other hand, when the client apparatus 320a or 320b is disconnected from the ultrasound imaging apparatus 310b, the processor 430 may cancel assignment of a corresponding TGC channel 520a or 520b to the disconnected client apparatus 320a or 320b. The processor 430 may respectively generate ultrasound images based on ultrasound signals produced via the second and third TGC channels 520a and 520b and transmit the ultrasound images to the plurality of client apparatuses 320a and 320b to which the second and third TGC channels 520a and 520b are respectively assigned. For example, the processor 430 may transmit to the client apparatus 320a a second ultrasound image generated based on a second ultrasound signal produced via the second TGC channel 520a. The processor 430 may also transmit to the client apparatus 320b a third ultrasound image generated based on a third ultrasound signal produced via the third TGC channel 520b.

[0112] A communicator 440 may communicate with the plurality of client apparatuses 320a and 320b and respectively transmit corresponding ultrasound images thereto. Furthermore, the communicator 440 may respectively receive TGC parameters from the plurality of client apparatuses 320a and 320b.

[0113] FIG. 8 illustrates a GUI view 800 provided by the client apparatus (320 of FIG. 3), according to an embodiment.

[0114] According to an embodiment, the client apparatus 320 may receive a user input of selecting analog TGC or digital TGC to perform a TGC operation selected by the user. For example, the client apparatus 320 may receive a user's selection by providing a TGC method selection menu 810 via a display.

[0115] The GUI view 800 may include the TGC method selection menu 810, a TGC parameter input portion 820, and a second ultrasound image 830. The TGC method selection menu 810 may include an analog TGC selection icon 812 and a digital TGC selection icon 814 and be provided to receive a user input of selecting a TGC method. The TGC parameter input portion 820 may be used to receive a user input of setting a second TGC parameter. The second ultrasound image may be provided as a streaming image via the display.

[0116] When analog TGC is selected in the client apparatus 320, the client apparatus 320 may transmit the set second TGC parameter to the ultrasound imaging apparatus 310. According to an embodiment, the client apparatus 320 may transmit information about the selected analog TGC together during transmission of the second TGC parameter. According to an embodiment, the ultrasound imaging apparatus 310 may assign a TGC channel to the client apparatus 320 based on selection of the analog TGC in the client apparatus 320.

[0117] According to an embodiment, when digital TGC is selected in the client apparatus 320, the client apparatus 320 may perform the digital TGC with respect to the second ultrasound image 830 based on the second TGC parameter.

[0118] According to another embodiment, when digital TGC is selected in the client apparatus 320, the client apparatus 320 may transmit the second TGC parameter and information indicating selection of the digital TGC to the ultrasound imaging apparatus 310, and the ultrasound imaging apparatus 310 may perform the digital TGC on the second ultrasound image based on the second TGC parameter and then transmit the second ultrasound image that has undergone the digital TGC to the client apparatus 320.

[0119] FIG. 9 illustrates a GUI view 900 for TGC control of the ultrasound imaging apparatus 310 or the client apparatus 320, according to an embodiment.

[0120] According to an embodiment, the ultrasound imaging apparatus 310 or the client apparatus 320 may provide a plurality of predefined TGC curve options 932a, 932b, and 932c and set a TGC parameter based on a user input of selecting one of the plurality of predefined TGC curve options 932a, 932b, and 932c. According to an embodiment, the GUI view 900 for TGC control may include an ultrasound image 910, currently set TGC curve information 920, a TGC curve option selection menu 930, and a TGC parameter setting unit 940. The TGC curve option selection menu 930 may include the plurality of predefined TGC curve options 932a, 932b, and 932c. A TGC parameter setting method used by the TGC parameter setting unit 940 of FIG. 9 is merely an example and may vary according to circumstances.

[0121] FIG. 10 illustrates GUI views 1010 and 1030 for TGC control of the client apparatus 320 and the ultrasound imaging apparatus 310, according to an embodiment.

[0122] According to an embodiment, the client apparatus 320 may provide information 1012 about a TGC setting of the ultrasound imaging apparatus 310 via the GUI view 1010. The information 1012 about the TGC setting of the ultrasound imaging apparatus 310 may include a TGC curve 1014 and a first ultrasound image 1016. Furthermore, the ultrasound imaging apparatus 310 may provide information 1032 about a TGC setting of the client apparatus 320 via the GUI view 1030. The information 1032 about the TGC setting of the client apparatus 320 may include a TGC curve 1034 and a first ultrasound image 1036.

[0123] According to an embodiment, the client apparatus 320 may provide information 1020 about a TGC method. For example, when the client apparatus 320 performs analog TGC, an icon 1022 corresponding to the analog TGC may be highlighted. On the other hand, when the client apparatus 320 performs digital TGC, an icon 1024 corresponding to the digital TGC may be highlighted. A user may select the analog TGC or digital TGC by using the corresponding icons 1022 or 1024. Furthermore, according to an embodiment, the client apparatus 320 may provide information 1026 indicating whether the TGC method performed by the ultrasound imaging apparatus 310 is analog TGC or digital TGC while providing the information 1012 about the TGC setting of the ultrasound imaging apparatus 310.

[0124] According to an embodiment, the ultrasound imaging apparatus 310 may provide information 1040 about a TGC method. For example, when the ultrasound imaging apparatus 310 performs analog TGC, an icon 1042 corresponding to the analog TGC may be highlighted. On the

other hand, when the ultrasound imaging apparatus 310 performs digital TGC, an icon 1044 corresponding to the digital TGC may be highlighted. The user may select the analog TGC or digital TGC by using the corresponding icons 1042 or 1044. Furthermore, according to an embodiment, the ultrasound imaging apparatus 310 may provide information 1046 indicating whether the TGC method performed by the client apparatus 320 is analog TGC or digital TGC while providing the information 1032 about the TGC setting of the client apparatus 320.

[0125] FIG. 11 illustrates a GUI view for TGC control of the ultrasound imaging apparatus 310 or the client apparatus 320, according to an embodiment.

[0126] According to an embodiment, the GUI view for TGC control may include a plurality of lines 1120a, 1120b, 1120c, and 1120d respectively corresponding to reception depths and icons 1130a, 1130b, 1130c, and 1130d respectively corresponding thereto. A user may adjust each TGC gain value corresponding to each of the reception depths by moving each of the icons 1130a, 1130b, 1130c, and 1130d corresponding to each of the reception depths to the left or right side of an ultrasound image 1110. In an embodiment, the user may decrease a TGC gain value by moving each of the icons 1130a, 1130b, 1130c, and 1130d respectively corresponding to the reception depths to the left side of the ultrasound image 1110 and increase the TGC gain value by moving each of the icons 1130a, 1130b, 1130c, and 1130d to the right side thereof. The user may move the icons 1130a, 1130b, 1130c, and 1130d via a touch screen, a mouse, a keyboard, a knob, etc.

[0127] Furthermore, according to an embodiment, the plurality of lines 1120a, 1120b, 1120c, and 1120d and the icons 1130a, 1130b, 1130c, and 1130d respectively corresponding to the reception depths may be arranged on the ultrasound image 1110. In this case, each of the plurality of lines 1120a, 1120b, 1120c, and 1120d may be located at a position on the ultrasound image 1110, which corresponds to a reception depth of the line.

[0128] FIG. 12 illustrates a GUI view for TGC control of the ultrasound imaging apparatus 310 or the client apparatus 320, according to an embodiment.

[0129] According to an embodiment, the GUI view for TGC control may provide a TGC curve representing a currently set TGC parameter. According to an embodiment, the GUI view may include a first region 1220 composed of a plurality of lines and icons respectively corresponding to reception depths and a TGC curve region 1210 corresponding to a set TGC parameter.

[0130] FIG. 13 illustrates a GUI view for TGC control of the ultrasound imaging apparatus 310 or the client apparatus 320, according to an embodiment.

[0131] According to an embodiment, the GUI view for TGC control may be used to receive a user input of drawing a TGC curve in a second region 1310 and display the TGC curve corresponding to the received user input in the second region 1310. According to an embodiment, an ultrasound image 1320 and the second region 1310 may be arranged parallel to each other, and a reception depth in the ultrasound image 1320 and a corresponding reception depth in the TGC curve may be shown by a horizontal line.

[0132] FIG. 14 illustrates a GUI view for TGC control of the ultrasound imaging apparatus 310, according to an embodiment.

[0133] According to an embodiment, the ultrasound imaging apparatus 310 may apply a second TGC parameter for the client apparatus 320 to the ultrasound imaging apparatus 310 itself. The GUI view for TGC control of the ultrasound imaging apparatus 310, may include a first icon 1412 for selecting application of the second TGC parameter to the ultrasound imaging apparatus 310. In addition, the GUI view of the ultrasound imaging apparatus 310 may include information 1414 about the second TGC parameter and a second ultrasound image 1416. When the user selects the first icon 1412, the second TGC parameter may be applied to a first TGC channel.

[0134] According to embodiments, a client apparatus is capable of controlling a TGC parameter of an ultrasound imaging apparatus.

[0135] Furthermore, according to the embodiments, the client apparatus may adjust an analog TGC parameter and separately generate and provide an image to an ultrasound imaging apparatus and an image to a client apparatus.

[0136] Embodiments may be implemented through non-transitory computer-readable recording media having recorded thereon computer-executable instructions and data. The instructions may be stored in the form of program codes, and when executed by a processor, generate a pre-determined program module to perform a specific operation. Furthermore, when being executed by the processor, the instructions may perform specific operations according to the embodiments.

What is claimed is:

1. An ultrasound imaging apparatus comprising:
 - a probe including a transducer array;
 - an ultrasound signal receiver including a first time gain compensation (TGC) channel and a second TGC channel that each perform TGC on an ultrasound signal received from the probe;
 - a communicator configured to communicate with a first client apparatus; and
 - one or more processors configured to change a second TGC parameter of the second TGC channel, based on a control signal received from the first client apparatus, generate a second ultrasound image based on a second ultrasound signal produced via the second TGC channel, and transmit the second ultrasound image to the first client apparatus via the communicator.
2. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to generate a first ultrasound image based on a first ultrasound signal produced via the first TGC channel and display the first ultrasound image on a display.
3. The ultrasound imaging apparatus of claim 1, wherein the first TGC channel comprises a first TGC compensator configured to compensate for an echo signal received from the probe by applying a first TGC set that is a set of gain values at reception depths,
 - wherein the second TGC channel comprises a second TGC compensator configured to compensate for an echo signal received from the probe by applying a second TGC set that is a set of gain values at reception depths,
 - wherein the first TGC set is determined based on a control signal received from the ultrasound imaging apparatus, and
 - wherein the second TGC set is determined based on a control signal received from the first client apparatus.

4. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to generate a live streaming signal from the second ultrasound image and transmit the live streaming signal to the first client apparatus via the communicator.

5. The ultrasound imaging apparatus of claim 1, wherein the ultrasound signal receiver further comprises a third TGC channel, and

wherein the one or more processors are further configured to change a TGC parameter of the third TGC channel, based on a control signal received from a second client apparatus, generate a third ultrasound image based on a third ultrasound signal produced via the third TGC channel, and transmit the third ultrasound image to the second client apparatus via the communicator.

6. The ultrasound imaging apparatus of claim 1, wherein the first client apparatus is configured to receive a selection signal for selecting one of analog TGC and digital TGC, and

wherein the one or more processors are further configured to change, based on reception of the selection signal for selecting the analog TGC by the first client apparatus, the second TGC parameter of the second TGC channel, based on the control signal from the first client apparatus.

7. The ultrasound imaging apparatus of claim 6, wherein the one or more processors are further configured to perform, based on reception of the selection signal for selecting the digital TGC by the first client apparatus, the digital TGC on the second ultrasound image based on a TGC parameter included in the control signal from the first client apparatus and transmit the second ultrasound image that has undergone the digital TGC to the first client apparatus via the communicator.

8. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to provide via a display at least one or a combination of information about a first TGC parameter of the first TGC channel, information about the second TGC parameter of the second TGC channel, and information about which TGC parameter is used to generate a displayed ultrasound image.

9. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to change a first TGC parameter based on the second TGC parameter in response to one of a control signal received from the ultrasound imaging apparatus and the control signal received from the first client apparatus.

10. The ultrasound imaging apparatus of claim 1, further comprising a storage storing information about the second TGC parameter according to a user of the first client apparatus,

wherein the one or more processors are further configured to set, based on information about the user of the first client apparatus, the second TGC parameter of the second TGC channel to be the second TGC parameter according to the user of the first client apparatus.

11. A method of controlling an ultrasound imaging apparatus including a first time gain compensation (TGC) channel and a second TGC channel that each perform TGC on an ultrasound signal received via a probe, the method comprising:

changing a second TGC parameter of the second TGC channel, based on a control signal received from the first client apparatus;

generating a second ultrasound image based on a second ultrasound signal produced via the second TGC channel; and
transmitting the second ultrasound image to the first client apparatus.

12. The method of claim **11**, further comprising:
generating a first ultrasound image based on a first ultrasound signal produced via the first TGC channel; and
displaying the first ultrasound image on a display of the ultrasound imaging apparatus.

13. The method of claim **11**, further comprising:
determining a first TGC set that is a set of gain values at reception depths, based on a control signal received from the ultrasound imaging apparatus;
determining a second TGC set that is a set of gain values at reception depths, based on the control signal received from the first client apparatus;
compensating for an echo signal received from the probe by applying the first TGC set by using a first TGC compensator of the first TGC channel; and
compensating for an echo signal received from the probe by applying the second TGC set by using a second TGC compensator of the second TGC channel.

14. The method of claim **11**, further comprising transmitting a live streaming signal generated from the second ultrasound image to the first client apparatus.

15. The method of claim **11**, wherein the ultrasound imaging apparatus further comprises a third TGC channel, the method further comprising:
changing a TGC parameter of the third TGC channel, based on a control signal received from a second client apparatus;
generating a third ultrasound image based on a third ultrasound signal produced via the third TGC channel, and
transmitting the third ultrasound image to the second client apparatus.

16. The method of claim **11**, wherein the first client apparatus receives a selection signal for selecting one of analog TGC and digital TGC, and

wherein the changing of the second TGC parameter of the second TGC channel comprises changing, based on reception of the selection signal for selecting the analog TGC by the first client apparatus, the second TGC parameter of the second TGC channel based on the control signal from the first client apparatus.

17. The ultrasound imaging apparatus of claim **6**, further comprising:

performing, based on reception of the selection signal for selecting the digital TGC by the first client apparatus, the digital TGC on the second ultrasound image, based on a TGC parameter included in the control signal from the first client apparatus; and

transmitting the second ultrasound image that has undergone the digital TGC to the first client apparatus.

18. The method of claim **11**, further comprising:

providing at least one or a combination of information about a first TGC parameter of the first TGC channel, information about the second TGC parameter of the second TGC channel, and information about which TGC parameter is used to generate a displayed ultrasound image.

19. The method of claim **11**, further comprising:

changing a first TGC parameter based on the second TGC parameter in response to one of a control signal received from the ultrasound imaging apparatus and the control signal received from the first client apparatus.

20. A computer program product comprising a non-transitory computer-readable recording medium having stored therein a computer program code for performing the method of claim **11**.

* * * * *

专利名称(译)	超声成像设备，其控制方法和计算机程序产品		
公开(公告)号	US20190247025A1	公开(公告)日	2019-08-15
申请号	US16/131562	申请日	2018-09-14
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO., LTD.		
当前申请(专利权)人(译)	三星MEDISON CO., LTD.		
[标]发明人	JIN GIL JU KANG YOUNG SEOK AHN MI JEOUNG KIM DAE HWAN		
发明人	JIN, GIL-JU KANG, YOUNG-SEOK AHN, MI-JEOUNG KIM, DAE-HWAN		
IPC分类号	A61B8/00 A61B8/14		
CPC分类号	A61B8/565 A61B8/54 A61B8/145 A61B8/463		
优先权	1020180018064 2018-02-13 KR		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种超声成像设备及其控制方法。超声成像设备包括：探头，包括换能器阵列；超声信号接收器，包括第一时间增益补偿（TGC）通道和第二TGC通道，每个通道对从探针接收的超声信号执行TGC；通信器，被配置为与第一客户端装置通信；一个或多个处理器，被配置为基于从第一客户端装置接收的控制信号改变第二TGC通道的第二TGC参数，基于经由第二TGC通道产生的第二超声信号生成第二超声图像，并且发送第二超声图像通过通信器到第一客户端装置。

