




US 20160199023A1

(19) **United States**(12) **Patent Application Publication**  
**Pelissier et al.**(10) **Pub. No.: US 2016/0199023 A1**(43) **Pub. Date: Jul. 14, 2016**(54) **ULTRASOUND IMAGING INSTRUMENT  
VISUALIZATION****Publication Classification**(71) Applicant: **ULTRASONIX MEDICAL  
CORPORATION**, Richmond (CA)(51) **Int. Cl.**  
*A61B 8/08* (2006.01)  
*A61B 8/00* (2006.01)  
(52) **U.S. Cl.**  
CPC ..... *A61B 8/0841* (2013.01); *A61B 8/463*  
(2013.01); *A61B 8/5215* (2013.01)(72) Inventors: **Laurent Pelissier**, North Vancouver  
(CA); **Kris Dickie**, Vancouver (CA); **Bo  
Zhuang**, New Westminster (CA)(73) Assignee: **Ultrasonix Medical Corporation**,  
Richmond, BC (CA)(21) Appl. No.: **14/912,620**(22) PCT Filed: **Aug. 19, 2013**(86) PCT No.: **PCT/IB2013/001790**

§ 371 (c)(1),

(2) Date: **Feb. 18, 2016**(57) **ABSTRACT**

A method includes transitioning, via a micro-processor, an ultrasound imaging system (100) running in a first mode (128), in which a first location and a first orientation of an elongate needle (106) of an instrument (102) at a surface (111) of an object (110) is determined based on a first signal from a tracking device (112) at least on the instrument, to a second different mode, in which a second location and a second orientation of the needle within the object is determined based on an ultrasound image representing the object, in response to determining the needle penetrated the surface of the object, wherein a beam steering angle with which the ultrasound image is acquired is determined based on the first location and the first orientation of the needle, and displaying the ultrasound image.

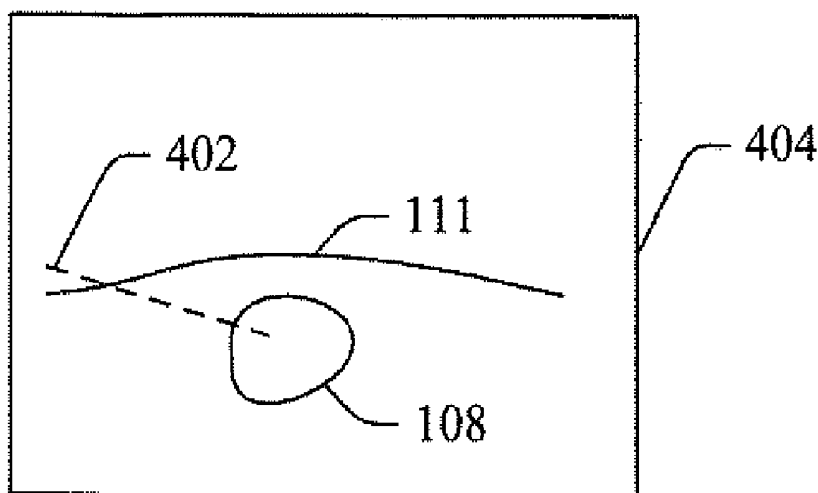

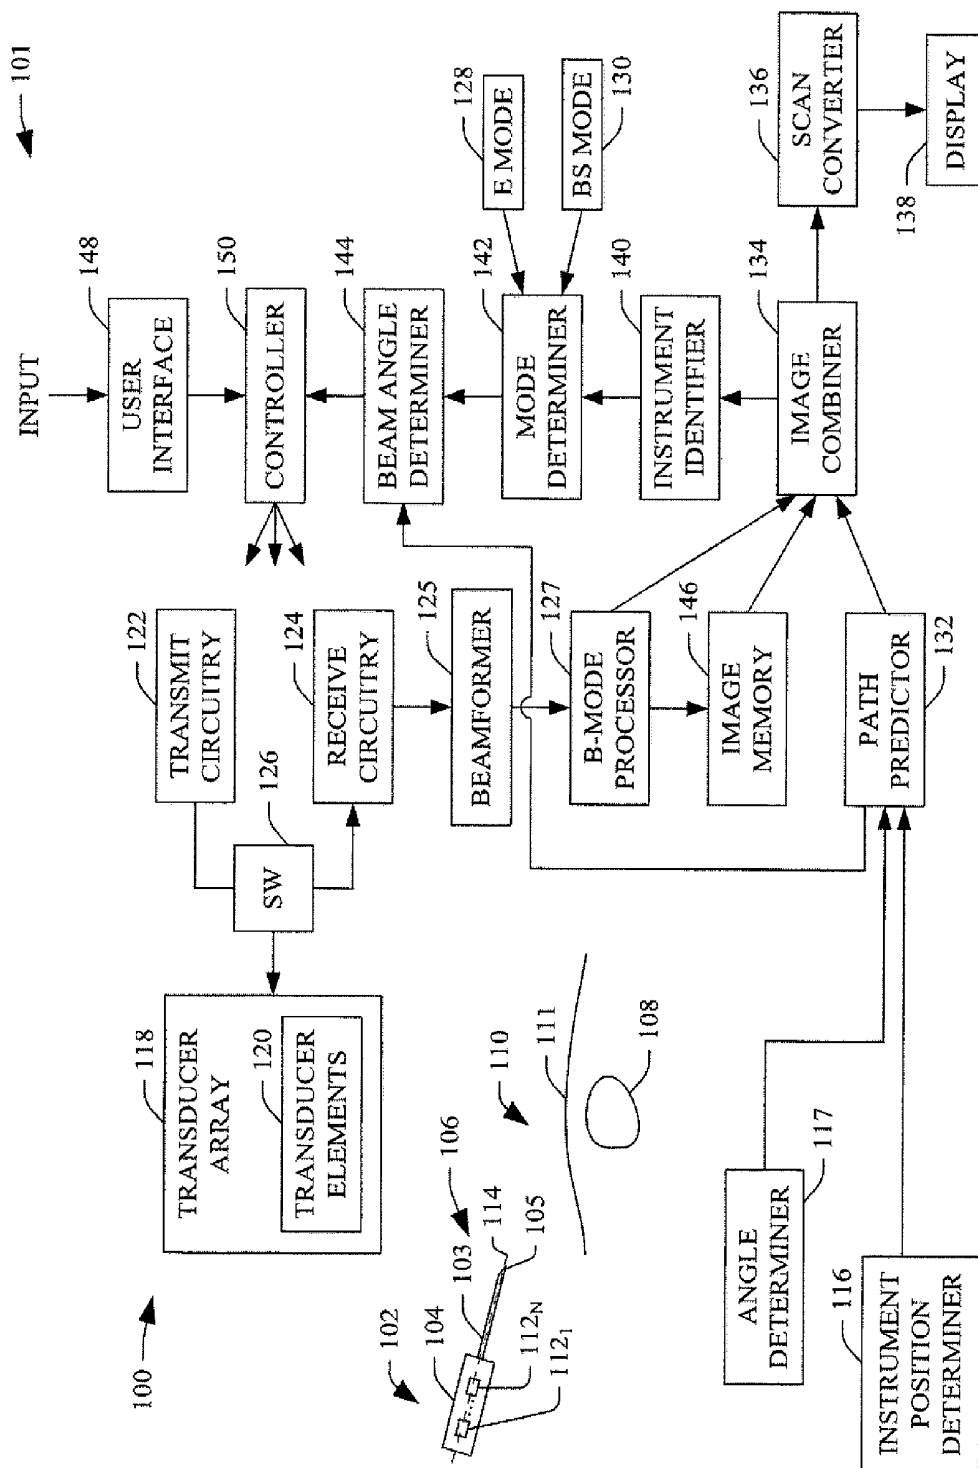


FIGURE 1

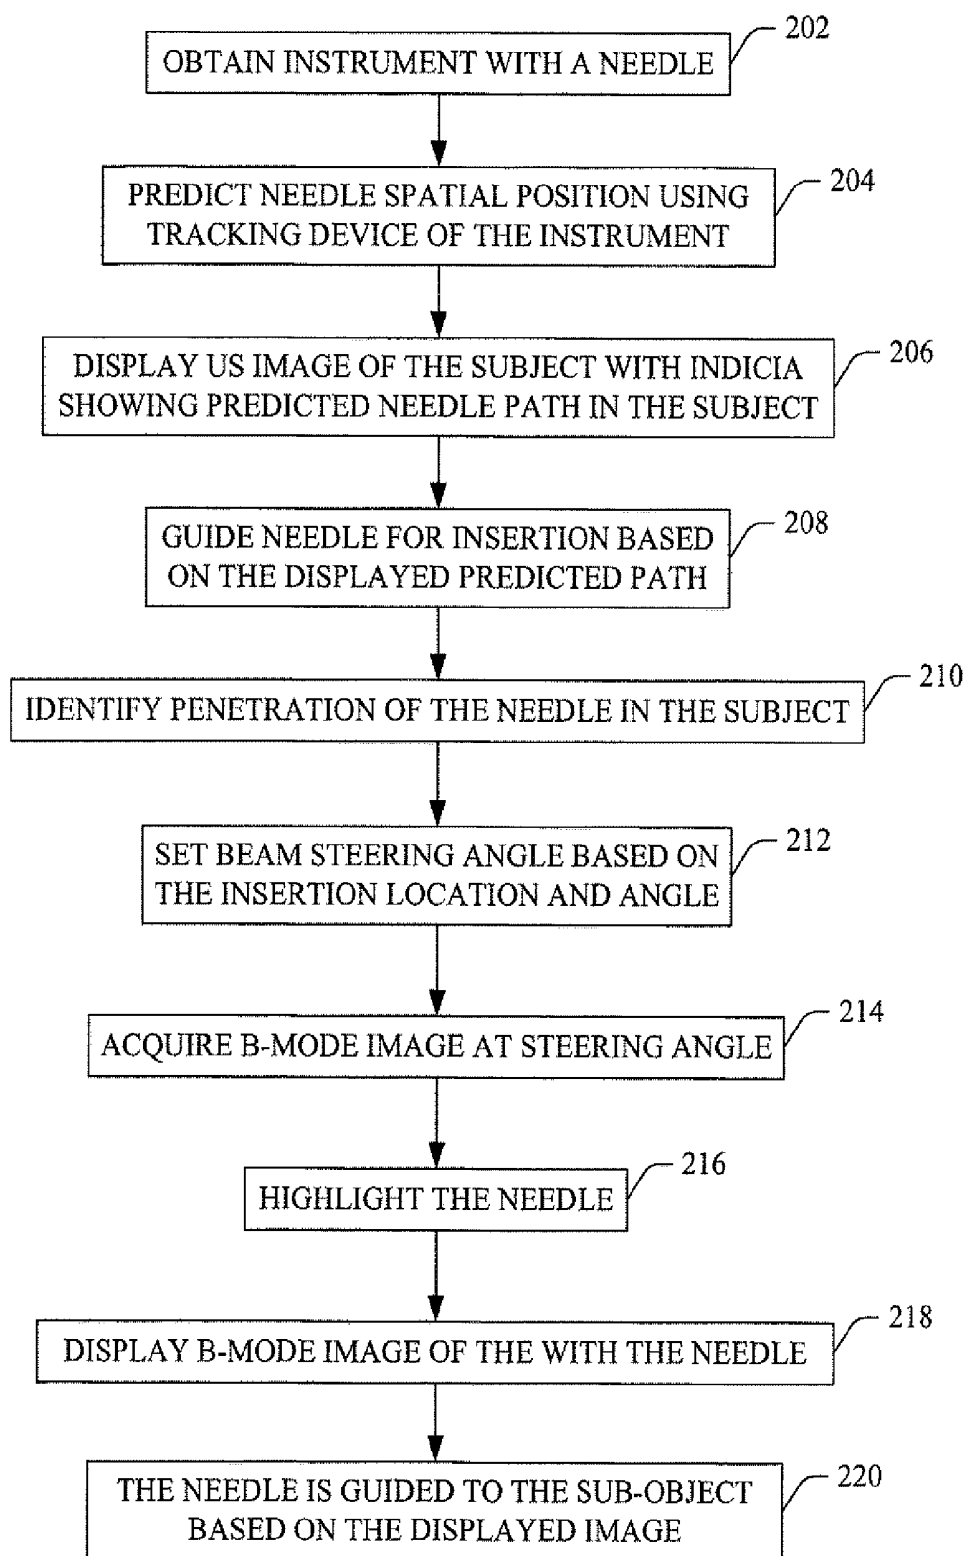


FIGURE 2

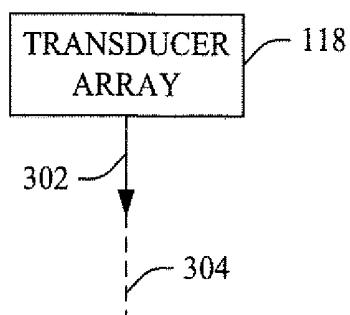


FIGURE 3A

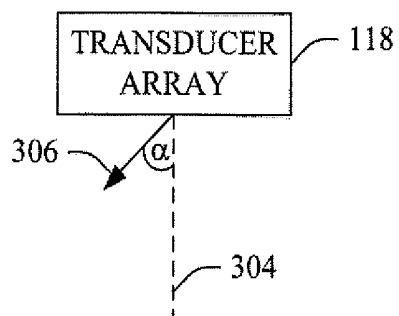


FIGURE 3B

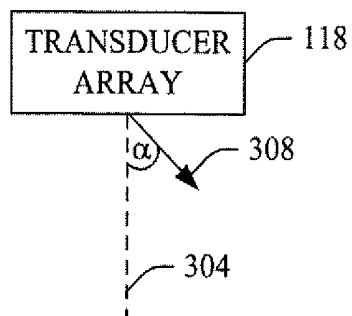


FIGURE 3C

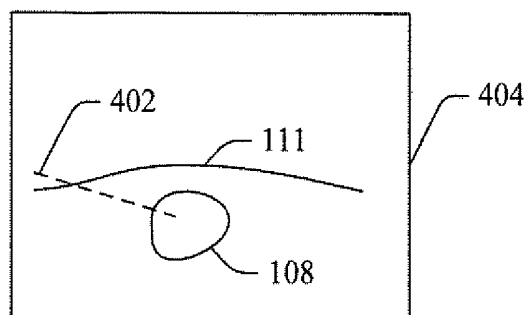


FIGURE 4

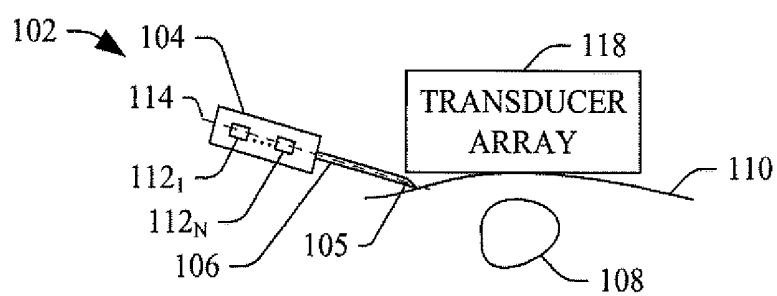


FIGURE 5

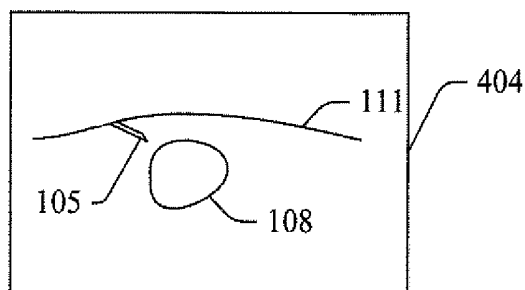


FIGURE 6

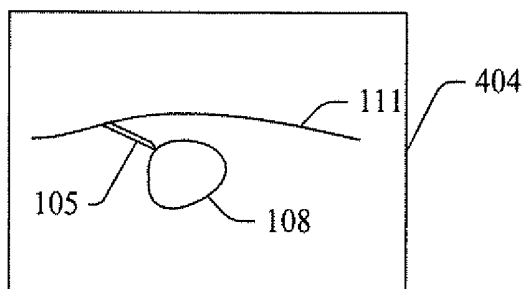


FIGURE 7

## ULTRASOUND IMAGING INSTRUMENT VISUALIZATION

TECHNICAL FIELD The following generally relates to ultrasound imaging and more particularly to ultrasound imaging instrument visualization.

### BACKGROUND

[0001] An ultrasound imaging apparatus has included a transducer array that transmits an ultrasound beam into an examination field of view. As the beam traverses structure (e.g., of a sub-portion of an object or subject) in the field of view, sub-portions of the beam are attenuated, scattered, and/or reflected off the structure, with some of the reflections (echoes) traversing back towards the transducer array. The transducer array receives and processes the echoes, and generates one or more images of a sub-portion of the subject or object. The one or more images are visually displayed.

[0002] Ultrasound imaging has also been used to visualize an instrument disposed in or being disposed in the object or subject. For example, ultrasound imaging has been used to produce images of a needle being positioned in a subject and to verify positioning of the needle tip for a medical procedure. Unfortunately, the image quality of the needle in the images tends to be low, e.g., due to the low signal to noise ratio of the ultrasound images and speckle. Approaches to improve visualization of a needle have included beam steering and needle shaft tracking with a tracking device on the instrument.

[0003] Beam steering has included steering the beam so that the direction of the beam is perpendicular to the instrument being visualized (e.g., the shaft of a needle), which improves image quality of the instrument. However, since the position and angle of insertion of the instrument is unknown, the ultrasound beam is steered over a wide range of angles to cover multiple possible scenarios in an attempt to find a suitable angle. Unfortunately, steering the beam to cover a wide range of angles may introduce artifacts into the images, such as false enhancement on strong tissue interfaces.

[0004] With needle shaft tracking, an electro-magnetic device(s) has been affixed to a handle of the instrument or the needle tip, and the device is calibrated so that signal received by the device(s) indicates the location/angle of the device and can be used to predict the location and orientation of the needle. With the device affixed to the handle, any bending of the needle shaft introduces error between the predicted location and the actual location of the needle tip. Having the device affixed to the needle tip mitigates this error. Unfortunately, it also requires a custom-made needle, which adds cost and limits which needles can be used.

### SUMMARY

[0005] Aspects of the application address the above matters, and others.

[0006] In one aspect, a method includes transitioning, via a micro-processor, an ultrasound imaging system running in a first mode, in which a first location and a first orientation of an elongate needle of an instrument at a surface of an object relative to the ultrasound imaging device is determined based on a first signal from a tracking device at least on the instrument, to a second different mode, in which a second location and a second orientation of the needle within the object is determined based on an ultrasound image representing the object, in response to determining the needle penetrated the

surface of the object, wherein a beam steering angle with which the ultrasound image is acquired is determined based on the first location and the first orientation of the needle, and displaying the ultrasound image.

[0007] In another aspect, a system includes a device with a handle that supports a needle, the handle including at least one position information emitter. The system further includes an instrument position determiner that identifies a spatial position of a shaft of the needle, relative to an object, based on an output of the at least one position emitter and generates a signal indicative thereof. The system further includes an ultrasound imaging system with a transducer array and a controller that activates acquisition of an image of the object with the transducer array using a beam steering angle based on the orientation and position information of the needle which results in activation of an ultrasound beam that traverses a direction approximately perpendicular to shaft.

[0008] In another aspect, a computer readable storage medium is encoded with computer readable instructions. The computer readable instructions, when executed by a processor, causes the processor to: automatically turn on a beam steering mode of an ultrasound imaging system based on a penetration depth of a needle in an object obtained from a signal from a tracking element of an instrument carrying the needle.

[0009] Those skilled in the art will recognize still other aspects of the present application upon reading and understanding the attached description.

### BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The application is illustrated by way of example and not limited by the figures of the accompanying drawings, in which like references indicate similar elements and in which:

[0011] FIG. 1 schematically illustrates an imaging apparatus in connection with an instrument;

[0012] FIG. 2 illustrates an example method for guiding a needle being inserted into a subject or object;

[0013] FIG. 3A illustrates a beam steering angle of zero;

[0014] FIG. 3B illustrates a beam steering angle +20 degrees (or -20 degrees);

[0015] FIG. 3C illustrates a beam steering angle -20 degrees (or +20 degrees);

[0016] FIG. 4 illustrates an image with a predicted path of a needle of an instrument, predicted based on an emitter(s) of the instrument, superimposed over an image of a subject or object;

[0017] FIG. 5 illustrates placement of the needle with respect to the subject or object based on FIG. 4;

[0018] FIG. 6 illustrates an image of the needle, using beam steering angle to enhance visibility of the needle, superimposed over an image of a subject or object, acquired with a beam steering angle for the subject or object; and

[0019] FIG. 7 illustrates an example of guiding the needle to a region of interest based on the image of FIG. 6.

### DETAILED DESCRIPTION

[0020] The following relates to visualizing an instrument disposed in or being disposed in an object or subject. In one instance, this includes determining an insertion location and angle based on position information from a tracking device affixed to the instrument and inserting the instrument in accordance therewith. Ultrasound imaging is used to track the

instrument in the object or subject using a beam steering angle automatically determined based on the insertion location and the angle.

**[0021]** FIG. 1 schematically illustrates a system **101** including an imaging apparatus, such as an ultrasound (US) imaging apparatus **100**, in connection with an instrument **102**.

**[0022]** In the illustrated embodiment, the instrument **102** includes a handle or support **104** and an elongate needle **106** with a shaft **103** (e.g., biopsy, surgical, etc. needle), which is removably attachable to the support **104**. At least a tip **105** of the needle **106**, in the illustrated embodiment, is to be positioned in a sub-object **108** (e.g., a vessel, a tissue mass, etc.) of a subject or object **110** having a surface **111**. In other embodiments, the instrument **102** may include another device (e.g., a guide wire, a lumen, etc.).

**[0023]** The support **104** includes N emitters,  $112_1, \dots, 112_N$  (collectively referred to herein as emitters **112**), where N is a positive integer equal to or greater than one (1). The emitters **112** can be affixed to the support **104**, as shown in FIG. 1, integrated as part of the support **104**, and/or affixed to and/or integrated in the needle **106**. In the illustrated example, the emitters **112** are positioned along a long axis **114** of the needle **106** and emit signals indicative of their location in three dimensional (3D) space. The signals can be processed to determine a spatial location and orientation of the emitters **112**.

**[0024]** The determined spatial location and orientation of the emitters **112** can then be used to predict the spatial location and orientation of the needle **106**. In a variation, the emitters **112** are not positioned along the long axis **114**. However, the relative position of the emitters **112** to the long axis **114** is known and allows for predicting the location and orientation of the needle **106**. The emitters **112** can include an electro-magnetic device (e.g. with 5, 6, etc. degrees of freedom), a coil, an optical device, and/or other emitter. In an alternative embodiment, a transmitter, a passive sensor, a combination of an emitter, a transmitter and/or a passive sensor, and/or other tracking device can be affixed to the instrument **102**, e.g., at the support **104** and/or the needle **106**, and used to determine the spatial location and the orientation of the particular tracking device(s).

**[0025]** An instrument position determiner **116** detects the signals from the emitters **112** and determines the location and orientation of the emitters in 3D space based thereon. For example, where the emitters **112** include magnets, the instrument position determiner **116** can include a sensor(s) that measures a magnetic field strength of the magnets. The magnetic field strength seen at the sensor(s) depends on a distance and direction of the magnets to the sensor(s) and thus the strength and direction can be used to determine location and orientation of the emitters (and hence the needle **106**). Other approaches are also contemplated herein.

**[0026]** Examples of suitable position determiner systems are also described in U.S. patent application Ser. No. 12/703,706, filed Feb. 10, 2010, and entitled "Ultrasound Systems Incorporating Position Sensors and Associated Method," which is incorporated herein by reference in its entirety, and U.S. patent application Ser. No. 12/775,403, filed May 6, 2010, and entitled "Freehand Ultrasound Imaging Systems and Methods for Guiding Elongate Instruments," which is incorporated herein by reference in its entirety. Other approaches are also contemplated herein. As disclosed at least in these references, an emitter, a sensor, and/or a transmitter

additionally can be affixed to an ultrasound imaging system, which is described in greater detail below.

**[0027]** In a variation, the instrument is supported by mechanical guide, which can have a triangular or other shape configuration. The needle is fixed on one side of the triangle with a track. A sensor/emitter is attached to the needle to determine the movement of needle along the track (needs a determiner too). The angle relative to the skin surface can be determined by affixing the other side of the triangle on the skin surface. Then the angle between these two sides can be determined (either fixed or through an angle determiner). An optional angle determiner **117** would determine the angle. A distance between the needle **106** and the subject or object **110** can be fixed and pre-measured or determined. Other guides and approaches are also contemplated herein.

**[0028]** The ultrasound imaging system **100** includes a transducer array **118** with a one or two-dimensional array of transducer elements **120**. The transducer elements **120** convert electrical signals to an ultrasound pressured field and vice versa respectively to transmit ultrasound signals into a field of view and receive echo signals, generated in response to interaction with structure in the field of view, from the field of view. The transducer array **118** can be square, rectangular and otherwise shape, linear and/or curved, fully populated or sparse, etc.

**[0029]** Transmit circuitry **122** generates a set of pulses (or a pulsed signal) that are conveyed, via hardwire (e.g., through a cable) and/or wirelessly, to the transducer array **118**. The set of pulses excites a set (i.e., a sub-set or all) of the transducer elements **120** to transmit ultrasound signals. This includes exciting the transducer array **118** to transmit signals in connection with B-mode, Doppler, and/or other imaging modes. In one instance, this includes exciting the transducer elements **120** to steer the beam based on a predetermined beam steering angle.

**[0030]** As utilized herein, and shown in FIG. 3A, a beam steering angle of zero (0) corresponds to an ultrasound beam **302** traversing in a direction along an axis **304** perpendicular to the transducer array **118**. As utilized herein, and shown in FIG. 3B, a beam steering angle ( $\alpha$ ) of +20 degrees corresponds to a beam **306** traversing in a direction at an angle of 20 degrees to one side of the axis **304**. As utilized herein, and shown in FIG. 3C, a beam steering angle ( $\alpha$ ) of -20 degrees corresponds to a beam **308** traversing at an angle of 20 degrees to the other side of the axis **304**.

**[0031]** Returning to FIG. 1, receive circuitry **124** receives a set of echoes (or echo signals) generated in response to a transmitted ultrasound signal interacting with structure in the field of view. The receive circuitry **124** is configured to receive echoes corresponding at least to B-mode, Doppler, and/or other imaging. A switch (SW) **126** controls whether the transmit circuitry **122** or the receive circuitry **124** is in electrical communication with the transducer elements **120** to transmit ultrasound signals or receive echoes.

**[0032]** A beamformer **125** processes the received echoes by applying time delays to echoes, weighting echoes, summing delayed and weighted echoes, and/or otherwise beamforming received echoes, creating beamformed data. The beamformer **125** and/or other processing circuitry may also perform other processing such as, but not limited to, one or more of echo-cancellation, wall-filtering, basebanding, averaging and decimating, envelope detection, log-compression, and/or other processing.

[0033] A B-mode processor 127 processes the beamformed data and generates B-mode images, which, generally, include a sequence of focused, coherent echo samples along focused scanlines of a scanplane. The B-mode images may be based on acquisitions with a beam steering angle of zero or non-zero. The B-mode processor 127 may also be configured to process the scanlines to lower speckle and/or improve specular reflector delineation via spatial compounding, and/or perform other processing such as FIR filtering, IIR filtering, edge enhancement, etc.

[0034] A path predictor 132 receives a signal from the instrument position determiner 116 and the angle determiner 117. As discussed above, the signals include the location and orientation of the emitters 112 in 3D space and the angle of the needle 106 with respect to the surface 111 of the subject or object 110. The path predictor 132, based on a mapping to the ultrasound image space, predicts a path of the needle 106 in the field of view of the transducer array 118. For example, with a straight (non-curved) needle, the predicted path may be a linear extrapolation of the line segment between the emitters 112, which, in the illustrated embodiment, is along the long axis 114 of the needle 106.

[0035] An image combiner 134 superimposes or otherwise combines indicia (e.g., a dashed line, color, etc.) representing the predicted path over the B-mode image. The image combiner 134 can also combined multiple B-mode images, as discusses herein, e.g., a B-mode image (or a sub-portion thereof) acquired with a non-zero beam steering angle with a different B-mode image (or a sub-portion thereof) acquired with a zero or different non-zero beam steering angle. The image combiner 134 can also behave as a pass through for a B-mode image.

[0036] A scan converter 136 scan converts the output of the image combiner 134 to generate data for display, e.g., by converting the data to the coordinate system of a display 138. In the illustrated embodiment, this includes scan converts a B-mode image. The scan converter 136 can be configured to employ analog and/or digital scan converting techniques. The display 138 can be a light emitting diode (LED), liquid crystal display (LCD), and/or type of display, which is part of the ultrasound imaging system 100 or in electrical communication therewith via a cable.

[0037] An instrument identifier 140 identifies the instrument 102 in the combined image that includes the predicated path superimposed over the B-mode image. This includes identifying a location of the instrument 102 with respect to the subject or object 110. For example, the instrument identifier 140 can identify whether the needle 106 is outside of, against or has penetrated the surface 111 of the subject or object 108. The instrument identifier 140 evaluates relative spatial position of the instrument 102 in conjunction with pre-calibrated data based on the needle 106 and the relative spatial position of transducer elements 120 to determine penetration of the surface 111.

[0038] A mode determiner 142 determines an operational mode of the system 100 based on the location of the needle 106 with respect to the subject or object 110. In the illustrated embodiment, the system 100 can operate in a first (emitter, or E) mode 128 in which the signal from the emitters 112 is used to track the needle 106, a second (beam steering, or BS) mode 130 in which ultrasound images are used track the needle 106, or, an optional combined mode which combines the modes 128 and 130. The latter may include a smooth transition from the mode 128 to the mode 130.

[0039] Note that as used herein the terms “first,” “second,” etc. in connection with mode and/or other terms in the application are used as an order of introduction of the terms herein and are not part of the naming nomenclature. As such, a term introduced as “third,” for example, a “third” signal, may or may not have been generated before the “first” or “second” signal. Furthermore, even where the “third” signal is generated before the “first” or “second” signal, it still may be introduced and discussed after the “first” or “second” signal.

[0040] A beam angle determiner 144 determines a beam steering angle for the transmitted beam based on the mode. For example, when operating in the E mode 128, the beam steering angle is set to zero, with respect the axis 304, which is perpendicular to transducer array 118, or other, non-zero, beam steering angle determined based on the subject or object 110. However, when operating in the BS mode 130, the beam steering angle is determined based on the predicted location and orientation of the needle 106 with respect to the transducer array 118.

[0041] For example, in the latter instance, the beam steering angle can be set so that the beam is perpendicular or approximately perpendicular to the long axis 114 of the needle 106 and hence the needle shaft 103. Generally, the needle 106 reflects an ultrasound beam traversing at an angle closer to 90 degrees to the shaft in a manner in which the needle 106 is clearer in the generated image relative to angle less than 90 degrees. However, angles of less than 90 degrees, but around 90 degrees, are contemplated herein and may facilitate mitigating reverberation noise.

[0042] By using both, the E mode 128 and the BS mode 130, the needle 106 can be accurately tracked outside of the subject or object 110 and positioned for insertion and then accurately tracked inside the subject or object 110 through automatically setting the beam steering angle to optimize imaging the needle 106 based on the insertion location and angle and then superimposing the image of the needle 106 over an image with a beam steering angle set to optimize visualization of the subject or object 110.

[0043] The transition from the E mode 128 to the BS mode 130 may include, once the needle 106 penetrates the subject or object 110, fading away of the superimposed predicted path and visually presenting the beam steered image. The fading away can be based on a depth of the needle 106 in the object or subject 110 to mitigate error, e.g., due to bending of the needle 106. The beam steered image can be displayed alone or in combination with a previous acquired B-mode image acquired with a different beam steering angle (e.g., of zero), which can be stored in image memory 146.

[0044] A user interface (UI) 148 includes an input device(s) (e.g., a physical button, a touch screen, etc.) and/or an output device(s) (e.g., a touch screen, a display, etc.), which allow for interaction between a user and the ultrasound imaging apparatus 100. Such interaction may include activating the system 100 to use both the E mode 128 to the BS mode 130 as described herein. A controller 150 controls one or more of the components 122-148 of the system 100. Such control includes controlling one or more of these components to perform the functions described herein and/or other functions.

[0045] The US ultrasound imaging apparatus 100 can be part of a hand-held ultrasound imaging apparatus. An example of such an apparatus is described in U.S. Pat. No. 7,699,776 B2, entitled “Intuitive Ultrasonic Imaging System and Related Method thereof,” filed Mar. 6, 2003, which is



incorporated herein in its entirety by reference. Alternatively, the transducer array **118** is housed in a probe and the remaining components are part of a separate single computing system with an integrated and/or separate display. In this configuration, the probe and console have complementary interfaces and communicate with each other via the interfaces.

[0046] The ultrasound imaging system **100** components **128**, **130**, **132**, **134**, **136**, **140**, **142**, and/or **144** can be implemented via one or more computer processors (e.g., a central processing unit (CPU), a microprocessor, a controller, etc.) executing one or more computer executable instructions embedded or encoded on computer readable storage medium, which excludes transitory medium, such as physical memory. However, at least one of the computer executable instructions can alternatively be carried by a carrier wave, signal, and other transitory medium and implemented via the one or more computer processors.

[0047] FIG. 2 illustrates an example method for guiding a needle being inserted into a subject or object.

[0048] It is to be understood that the following acts are provided for explanatory purposes and are not limiting. As such, one or more of the acts may be omitted, one or more acts may be added, one or more acts may occur in a different order (including simultaneously with another act), etc.

[0049] At **202**, the instrument **102** with the support **104** and needle **106** is obtained. Where the emitters **112** are not already attached to the instrument **102**, the emitters **112** are attached to the instrument **102** and the needle position and angle are calibrated. The calibration can be done on-the-fly after the emitter **112** attachment, before-hand based on the needle type and length, and/or otherwise.

[0050] At **204**, the system **100** is operated in the E mode **128** in which the signal from the emitters **112** is utilized to predict a path of the needle **106** with respect to the subject or object **110**.

[0051] At **206**, indicia representing the predicted path is superimposed over and displayed with a B-mode image showing the subject or object **110**.

[0052] An example of this is shown in FIG. 4. In FIG. 4, a line **402** visually presented in a display **404** represents indicia representing a predicted path in the subject or object **110**, based on a location and spatial orientation of the emitters **112** outside of the subject or object **110** and the angle of the needle **106** with respect to the surface **111** of the subject or object **110**.

[0053] At **208**, the predicted path is used to guide the placement (e.g., position and angle) of the needle for insertion.

[0054] An example of this is shown in FIG. 5. In FIG. 5, the instrument **102** is positioned such that the tip **105** of the needle **106** is at a location and angle with respect to the subject or object **110**. Furthermore, the transducer array **118** is shown against the subject or object **110**.

[0055] At **210**, penetration of the needle **106** with respect to the subject or object **110** is identified. This is achieved by evaluating the combined image.

[0056] At **212**, in response thereto, the beam steering angle is automatically set based on the position and angle of the needle **106**. As described herein, the beam steering angle is set to be near or approximately at **90** degrees with respect to the shaft of the needle **106**.

[0057] At **214**, B-mode images are acquired using the set of the beam steering angle.

[0058] At **216**, the B-mode images are processed so the needle **106** is highlighted and isolated (e.g., segmented, visually enhanced, etc.) from the steered image.

[0059] At **218**, the image of the needle **106** is then superimposed over a B-mode image acquired with a steering angle of zero or other steering angle based on the subject or object **110**.

[0060] An example of this is shown in FIG. 6. In FIG. 6, the needle **106** is visualized in the subject or object **110** therewith.

[0061] At **220**, the needle **106** is guided to the sub-object **108** using the displayed image. The displayed image is periodically updated or refreshed with a combined beam steered image and non-beam steered image, showing the current location of the needle **106**.

[0062] An example of this is shown in FIG. 7. In FIG. 7, the needle **106** is guided to the sub-object **108** based on the visualization of FIG. 6.

[0063] As described here, the transition from determining the needle location and orientation can be based on penetration depth, which may reduce the artifact, simplify the operating process, avoid unnecessary frame rate loss, without user interaction.

[0064] With the above method, the needle **106** location can be accurately predicted, via the emitters **112**, outside of the subject or object **110**. Once the needle **106** penetrates the subject or object **110** and the accuracy of the prediction becomes susceptible to error, e.g., due to bending of the tip **105** of the needle **106**, beam steering based on the position and angle of the needle at insertion is automatically invoked so that the needle **106** can be accurately guided within the subject or object **110**.

[0065] As such, no custom-made needle with an emitter disposed at the tip is needed. In fact, all types of needle (i.e., both rigid and non-rigid) can be used with minimal to no sacrifice of artifact and/or frame rate. However, the needle path can be accurately predicted. Furthermore, the user does not have to acquire multiple images using different beam steering angles in an attempt to figure out which beam steering angle is "best" to use, via trial and error, to visualize the needle **106** within the subject or object **110**. Instead, the beam steering angle is automatically set based on the emitter information.

[0066] The methods described herein may be implemented via one or more processors executing one or more computer readable instructions encoded or embodied on computer readable storage medium which causes the one or more processors to carry out the various acts and/or other functions and/or acts. Additionally or alternatively, the one or more processors can execute instructions carried by transitory medium such as a signal or carrier wave.

[0067] The application has been described with reference to various embodiments. Modifications and alterations will occur to others upon reading the application. It is intended that the invention be construed as including all such modifications and alterations, including insofar as they come within the scope of the appended claims and the equivalents thereof.

#### 1. A method, comprising:

transitioning, via a micro-processor, an ultrasound imaging system running in a first mode, in which a first location and a first orientation of an elongate needle of an instrument at a surface of an object is determined based on a first signal from a tracking device at least on the instrument, to a second different mode, in which a second location and a second orientation of the needle

within the object is determined based on an ultrasound image representing the object, in response to determining the needle penetrated the surface of the object, wherein a beam steering angle with which the ultrasound image is acquired is determined based on the first location and the first orientation of the needle; and displaying the ultrasound image.

2. The method of claim 1, further comprising: determining the beam steering angle is an angle at which a transmitted ultrasound beam of the ultrasound imaging system traverses a direction approximately perpendicular to a shaft of the needle.

3. The method of claim 2, further comprising: segmenting a sub-region of the ultrasound including pixels representing the needle; superimposing the segmented sub-region over a second ultrasound image, generating a combined image; and displaying the combined image.

4. The method of claim 3, wherein the beam steering angle of the transmitted ultrasound beam is not perpendicular to the shaft.

5. The method of claim 4, wherein the beam steering angle of the transmitted ultrasound beam is approximately zero with respect to a transducer array of the ultrasound imaging system.

6. The method of claim 1, prior to the needle penetrating the surface, further comprising:

predicting a path of the needle through the object based on the first location and the first orientation of the needle; and

displaying a graphical representation of the predicted path superimposed over a third ultrasound image of the object, acquired before the first and second ultrasound images.

7. The method of claim 1, transitioning from the first mode to the second mode further based on a depth of the needle in the object, wherein the transition gradually occurs as a depth of the needle tip in the object increases.

8. The method of claim 1, further comprising: updating the display with an updated ultrasound image as the needle moves through the object.

9. The method of claim 1, further comprising: detecting when the needle penetrates the surface; generating a signal the indicates the needle penetrated the surface; and transitioning from the first mode to the second mode based on the signal.

10. The method of claim 1, wherein the updated display shows the needle at a location at which the needle tip is at a tissue of interest.

11. A system, comprising:

an instrument with a handle that supports a needle, the handle including at least one position information emitter;

an instrument position determiner that identifies a spatial position of a shaft of the needle, relative to an object,

based on an output of the at least one position emitter and generates a signal indicative thereof;

an ultrasound imaging system, including:

a transducer array; and

a controller that activates acquisition of an image of the object with the transducer array using a beam steering angle based on the orientation and position information of the needle which results in activation of an ultrasound beam that traverses a direction approximately perpendicular to shaft.

12. The system of claim 11, wherein the controller, prior to the signal, activates acquisition of a second image of the object using a second beam steering angle which results in a second transmitted ultrasound beam that is approximately perpendicular the transducer array.

13. The system of claim 12, further comprising:

a path predictor that predicts a path of the needle through the object based on the spatial position in response to the needle being outside of the object.

14. The system of claim 13, further comprising:

an image combiner that combines a representation of the predicted path with the second image; and

a display which visually presents the combined representation and second image.

15. The system of claim 14, further comprising:

an instrument identifier that identifies whether the needle is inside or outside of the object based on the combined representation and second image.

16. The system of claim 15, further comprising:

a mode determiner that determines whether the needle is to be tracked using spatial position or the image.

17. The system of claim 13, further comprising:

an image combiner that combines the image, which includes data that represents the needle with a second image acquired with a different beam steering angle, and:

a display which visually presents the combined image and second image.

18. The system of claim 17, wherein the image combiner segments the needle from the image and combine segmented image and the second image.

19. A computer readable storage medium encoded with computer readable instructions, which, when executed by a processor, causes the processor to:

automatically turn on a beam steering mode of an ultrasound imaging system based on a penetration depth of a needle in an object obtained from a signal from a tracking element at least of an instrument carrying the needle.

20. The computer readable storage medium of claim 19, wherein the computer readable instructions, which, when executed by the processor, further causes the processor to:

automatically set a beam steering angle so that an ultrasound beam transmitted by the ultrasound imaging system traverses a direction approximately perpendicular to a direct of a shaft of a needle, which is determined based on the signal.

\* \* \* \* \*

|                |                                                                                                                                                                                                                                                                                                                               |         |            |
|----------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 超声成像仪器可视化                                                                                                                                                                                                                                                                                                                     |         |            |
| 公开(公告)号        | <a href="#">US20160199023A1</a>                                                                                                                                                                                                                                                                                               | 公开(公告)日 | 2016-07-14 |
| 申请号            | US14/912620                                                                                                                                                                                                                                                                                                                   | 申请日     | 2013-08-19 |
| [标]申请(专利权)人(译) | 优胜医疗有限公司                                                                                                                                                                                                                                                                                                                      |         |            |
| 申请(专利权)人(译)    | ULTRASONIX医疗法人                                                                                                                                                                                                                                                                                                                |         |            |
| 当前申请(专利权)人(译)  | ULTRASONIX医疗法人                                                                                                                                                                                                                                                                                                                |         |            |
| [标]发明人         | PELISSIER LAURENT<br>DICKIE KRIS<br>ZHUANG BO                                                                                                                                                                                                                                                                                 |         |            |
| 发明人            | PELISSIER, LAURENT<br>DICKIE, KRIS<br>ZHUANG, BO                                                                                                                                                                                                                                                                              |         |            |
| IPC分类号         | A61B8/08 A61B8/00                                                                                                                                                                                                                                                                                                             |         |            |
| CPC分类号         | A61B8/0841 A61B8/5215 A61B8/463 A61B8/4245 A61B8/4254 A61B8/4427 A61B8/461 A61B8/467<br>A61B8/5207 A61B8/5246 A61B8/5269 A61B8/54 A61B10/02 A61B10/0233 G01S7/52073 G01S15/899<br>G16H50/20 A61B5/061 A61B5/066 A61B8/0833 A61B8/0891 A61B8/52 A61B8/5238 A61B17/3403<br>A61B34/20 G01S7/52074 G06T7/0012 G06T7/0016 G06T7/10 |         |            |
| 其他公开文献         | US10674995                                                                                                                                                                                                                                                                                                                    |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>                                                                                                                                                                                                                                                                               |         |            |

#### 摘要(译)

一种方法包括经由微处理器转换以第一模式 ( 128 ) 运行的超声成像系统 ( 100 ) , 其中第一位置和第一方向在物体的表面 ( 111 ) 处的仪器 ( 102 ) 的细长针 ( 106 ) ( 110 ) b> ) 基于来自跟踪设备 ( 112 ) 的至少在仪器上的第一信号到第二不同模式确定, 其中针的第二位置和第二方向在基于表示对象的超声图像确定对象, 响应于确定针穿透对象的表面, 其中基于第一位置 and 第一方向确定获取超声图像的光束转向角。针, 并显示超声图像。

