



US 20140046185A1

(19) **United States**

(12) **Patent Application Publication**
Mo et al.

(10) **Pub. No.: US 2014/0046185 A1**

(43) **Pub. Date: Feb. 13, 2014**

(54) **APPARATUSES AND METHODS FOR USER INTERACTIONS DURING ULTRASOUND IMAGING**

(52) **U.S. CL.**
USPC 600/443

(76) Inventors: **Ruoli Mo**, Wuxi (CN); **Danhua Zhao**, Wuxi (CN); **Mingchang Zhao**, Wuxi (CN)

(57) **ABSTRACT**


An ultrasound imaging apparatus configured with a touch screen display and computer aided measurement and/or diagnosis capability. In response to a touch input, image parameters for the computer aided measurement and/or diagnosis are determined from an analysis of the ultrasound image. A touch screen user interface allows the user to further adjust the parameters and/or other system parameters for the computer aided measurement and/or diagnosis in an interactive way. The computer aided measurement can be used directly for the computer aided diagnosis for improved accuracy and user experience.

(21) Appl. No.: **13/572,562**

(22) Filed: **Aug. 10, 2012**

Publication Classification

(51) **Int. Cl.**
A61B 8/14 (2006.01)

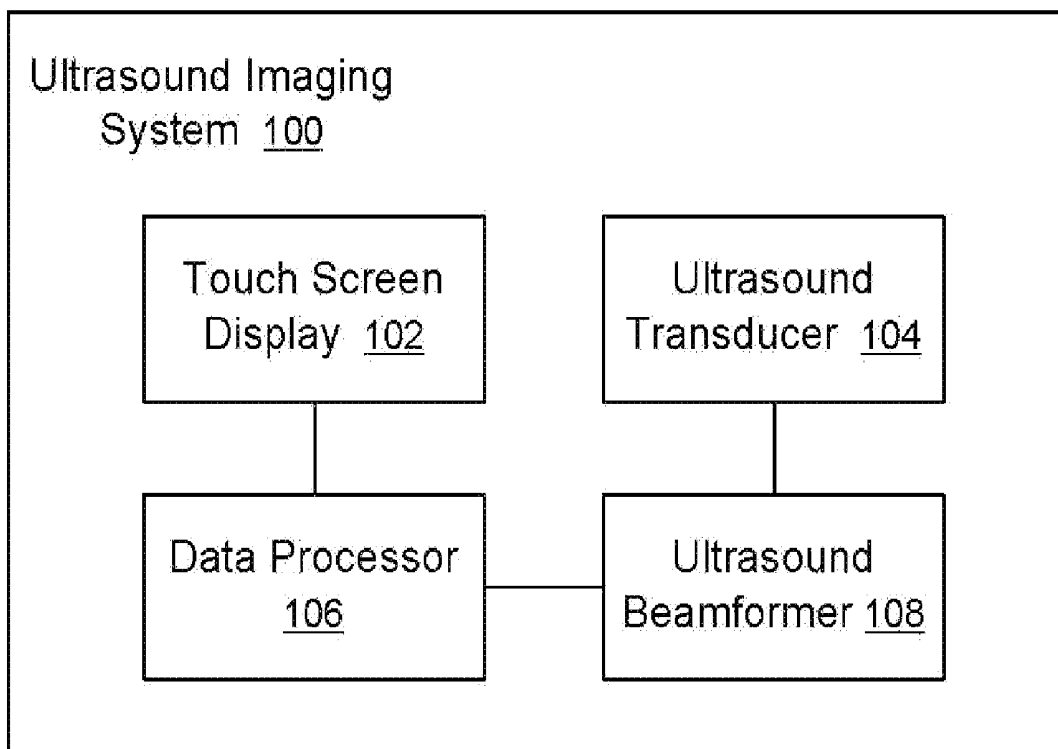

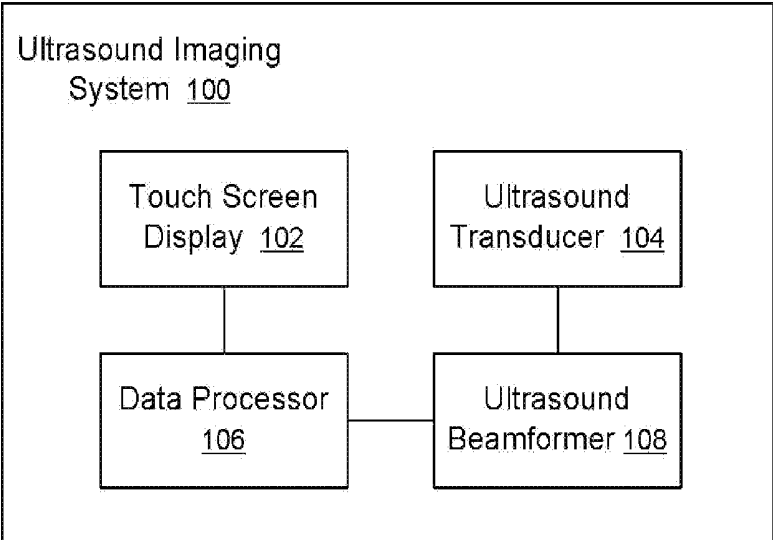


Figure 1

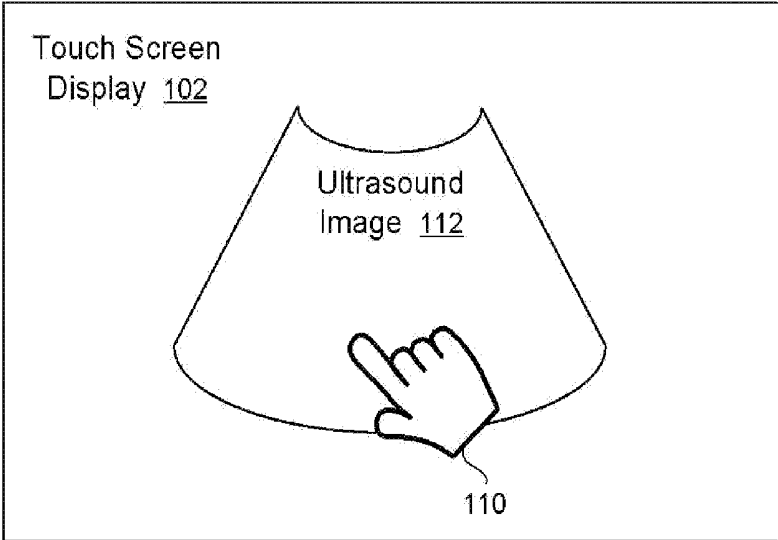


Figure 2

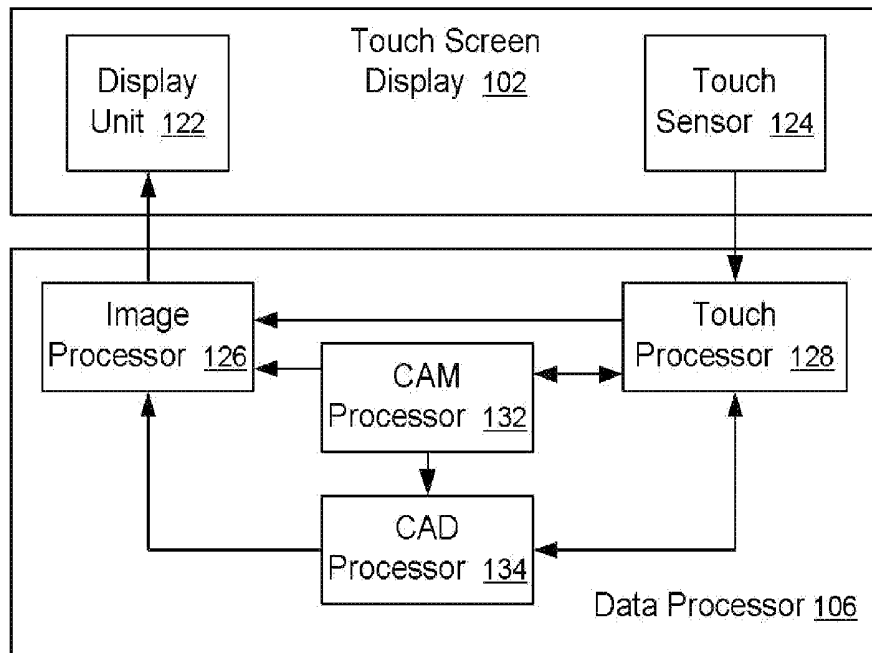


Figure 3

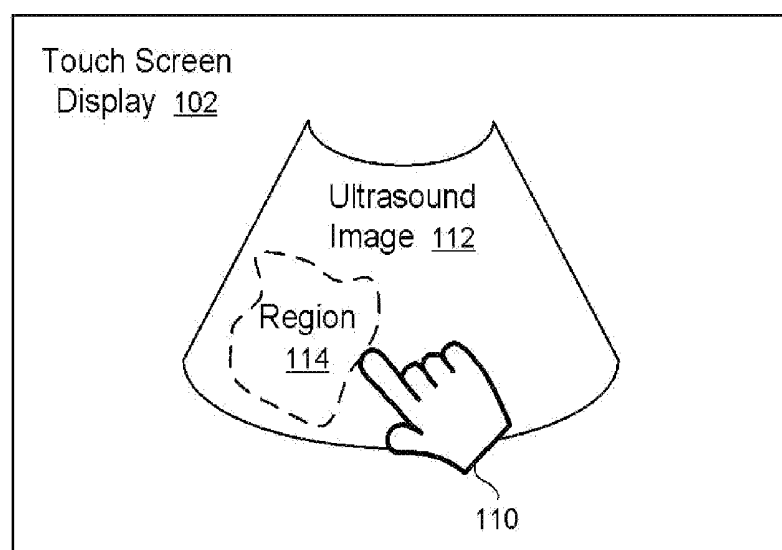


Figure 4

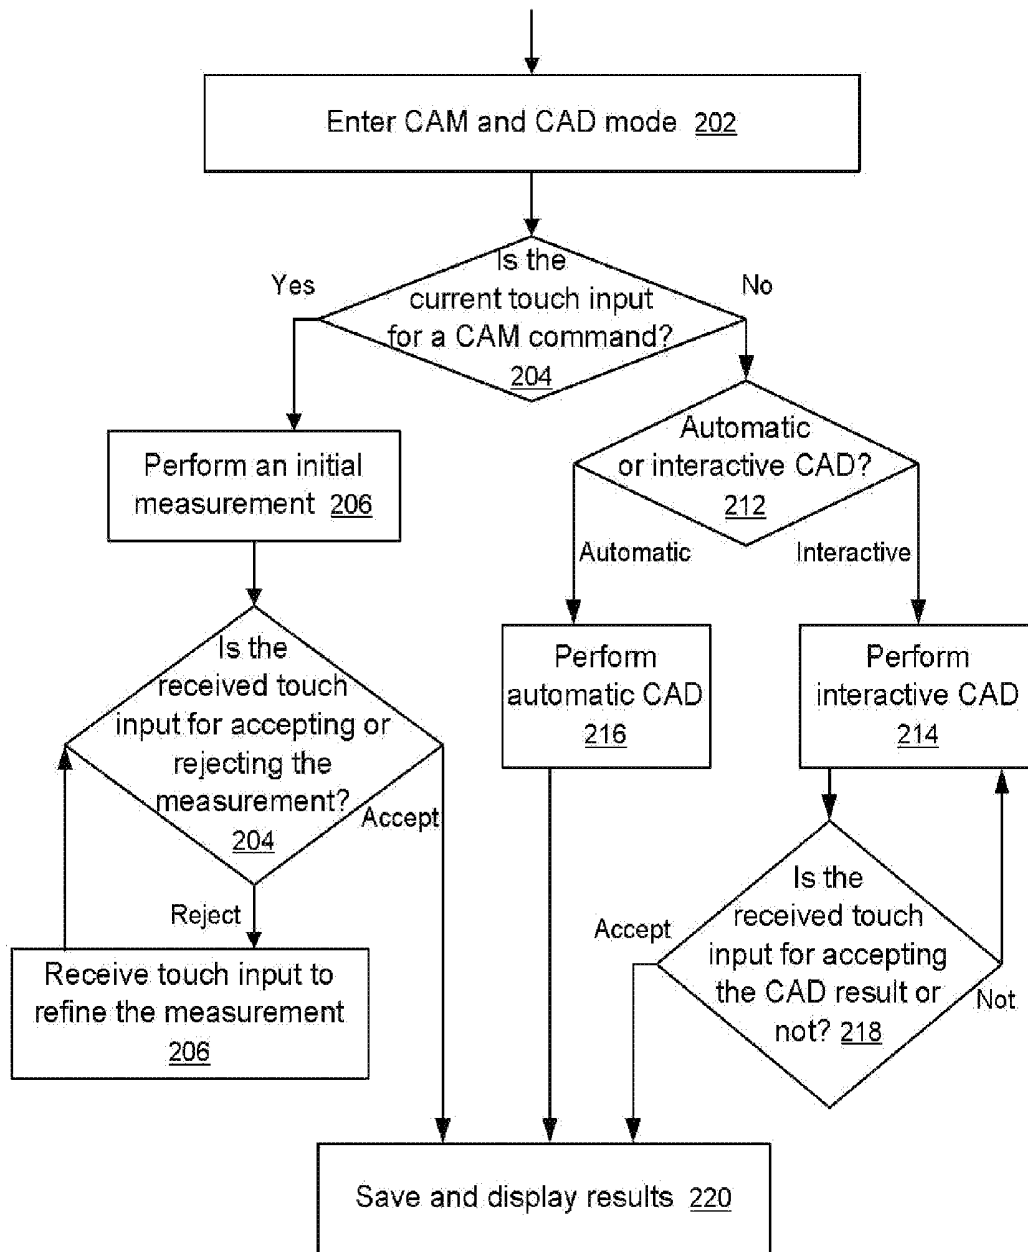


Figure 5

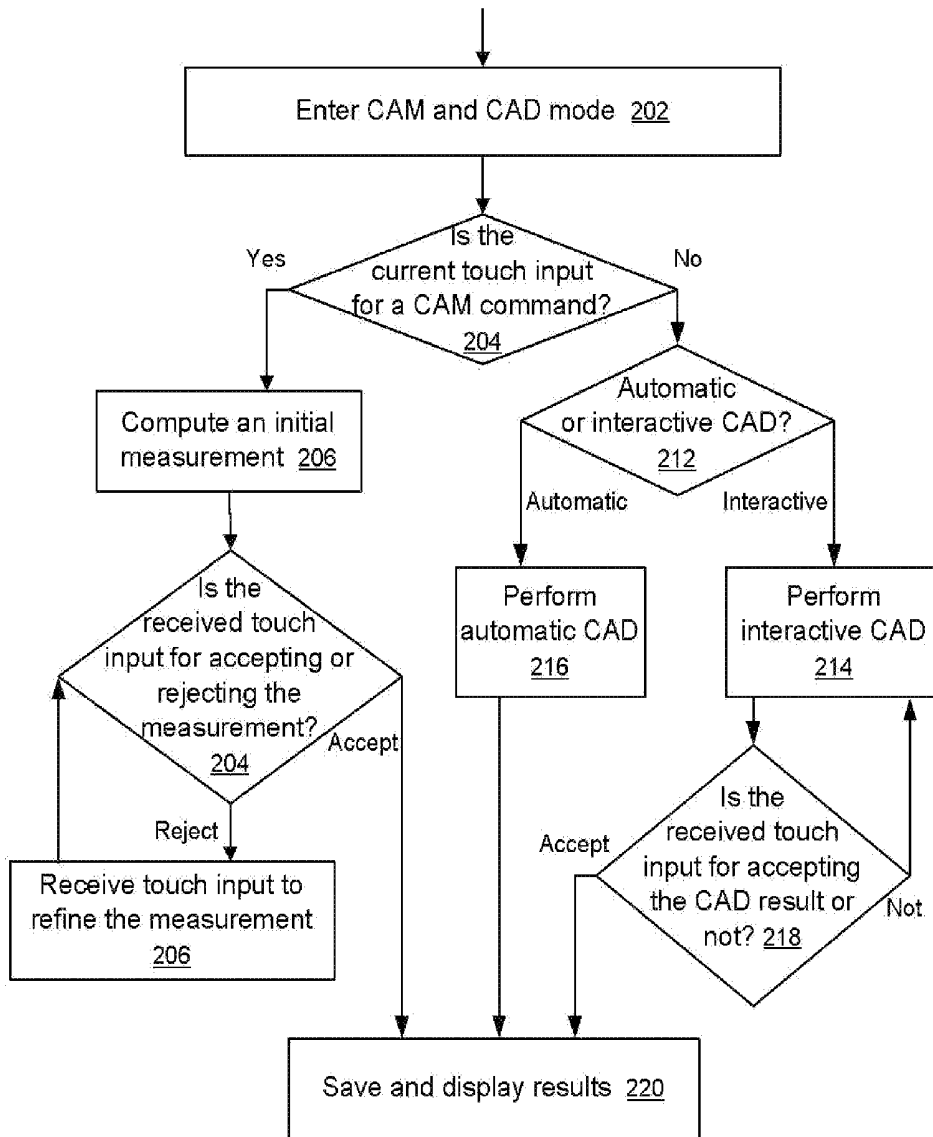


Figure 5

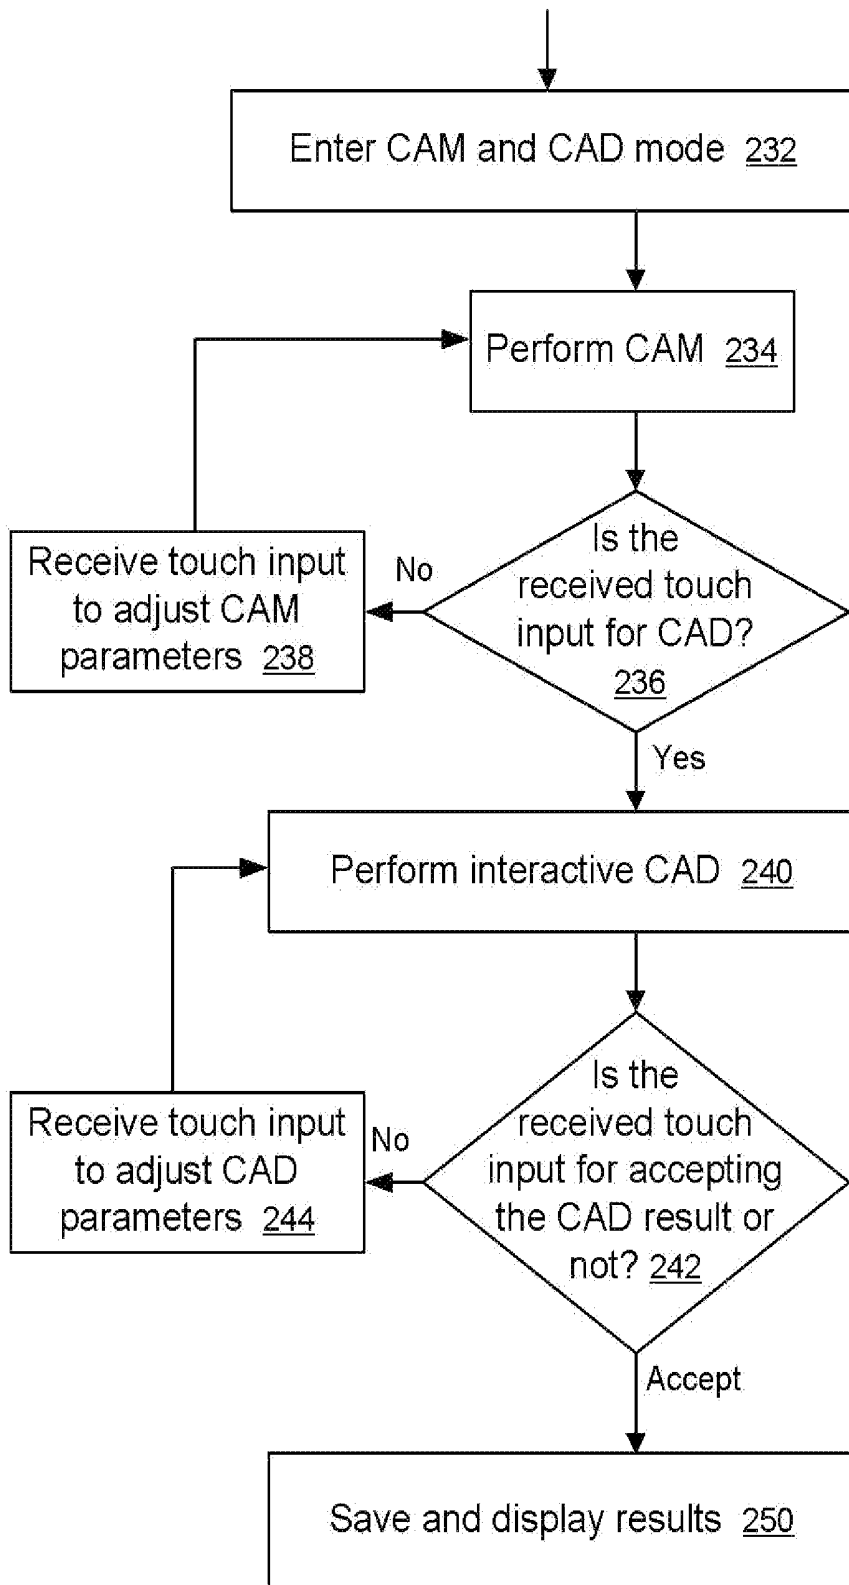


Figure 6

APPARATUSES AND METHODS FOR USER INTERACTIONS DURING ULTRASOUND IMAGING

FIELD OF TECHNOLOGY

[0001] The disclosure of the present application relates to, but not limited to, ultrasound imaging and user input processing for ultrasound imaging.

BACKGROUND

[0002] The conventional computer aided measurement (CAM) and computer aided diagnosis (CAD) technologies used in medical ultrasound imaging systems have a number of problems and limitations.

[0003] In a typical system, measurements are performed based on input generated using a touchpad or trackball and a number of buttons on the keyboard. Such a measurement system is slow, unintuitive, cumbersome, and inaccurate.

[0004] Conventional CAD technologies use predefined image processing algorithms and existing knowledge database to help doctors make diagnosis based on medical imaging, such as ultrasound imaging.

[0005] At least some embodiments of the present invention overcome some of the limitations of the current measurement technologies and diagnosis technologies by at least utilizing a touch screen based user interface.

BRIEF DESCRIPTION OF THE DRAWINGS

[0006] The embodiments disclosed in the presented application are illustrated by way of example and not limitation in the figures of the accompanying drawings in which like references indicate similar elements.

[0007] FIG. 1 shows an ultrasound imaging system according to one embodiment.

[0008] FIG. 2 shows a user interface for an ultrasound imaging system according to one embodiment.

[0009] FIG. 3 shows a portion of an ultrasound imaging system configured to process touch input for computer aided measurement and/or computer aided diagnosis according to one embodiment.

[0010] FIG. 4 illustrates an example of selecting a region for computer aided measurement and/or diagnosis according to one embodiment.

[0011] FIG. 5 shows a method to perform computer aided measurement or diagnosis according to one embodiment.

[0012] FIG. 6 shows a method to perform computer aided measurement and diagnosis according to one embodiment.

SUMMARY OF THE DESCRIPTION

[0013] In one embodiment, an ultrasound imaging apparatus is configured with a touch screen display and computer aided measurement and/or diagnosis capability. In response to a touch input, geometric parameters for the computer aided measurement and/or diagnosis are determined from an analysis of the ultrasound image. A touch screen user interface allows the user to further adjust the geometric parameters and/or other parameters for the computer aided measurement and/or diagnosis in an interactive way. The computer aided measurement can be used directly for the computer aided diagnosis for improved accuracy and user experience.

[0014] In one aspect, an ultrasound imaging apparatus, includes: an ultrasound transducer; a beamformer configured to control the ultrasound transducer; an image processor

coupled with the ultrasound transducer to generate an ultrasound image; a touch screen display coupled with the image processor to display the ultrasound image; a touch processor coupled with the touch screen display to receive and process touch input from the entire touch screen display including the portion where the ultrasound image is currently being displayed; a computer aided measurement processor coupled with the touch processor to provide measurement results; and a computer aided diagnosis processor coupled with the touch processor to provide diagnosis results.

[0015] In one embodiment, at least one of the touch processor, the image processor, the computer aided measurement processor and the computer aided diagnosis processor includes one of: an application-specific integrated circuit and a field programmable circuit.

[0016] In one embodiment, the computer aided diagnosis processor is further coupled to the computer aided measurement processor to receive measurement results for producing the diagnosis results. In one embodiment, the computer aided diagnosis processor operates based on a knowledge base.

[0017] In one embodiment, when the touch processor determines that a current touch input received on the touch screen display is for accepting a measurement result from the computer aided measurement processor, the touch processor instructs the computer aided diagnosis processor to perform a diagnosis in an interactive mode.

[0018] In one embodiment, when in the interactive mode, the computer aided diagnosis processor is configured to receive at least one input from the touch processor between starting of the diagnosis and presentation of a result for the diagnosis.

[0019] In one embodiment, the computer aided measurement processor is coupled with the image processor to present one or more geometric parameters used for producing the measurement results. In one embodiment, the one or more geometric parameters are overlaid on the ultrasound image to allow the user to visually inspect the degree of agreement between the geometric parameters used in the computation and the features in the ultrasound image. In one embodiment, the touch processor is configured to determine whether a currently received touch input is for adjusting the one or more geometric parameters, or for accepting the measurement results.

[0020] In one embodiment, the computer aided diagnosis processor is coupled with the image processor to present one or more geometric parameters used for producing the diagnosis results. In one embodiment, the one or more geometric parameters are overlaid on the ultrasound image to allow the user to visually inspect the degree of agreement between the geometric parameters used in the computation and the features in the ultrasound image. In one embodiment, the touch processor is configured to determine whether a currently received touch input is for adjusting the one or more geometric parameters, or for accepting the diagnosis results.

[0021] In another aspect, an ultrasound imaging apparatus, includes: an ultrasound transducer; a beamformer configured to control the ultrasound transducer; an image processor coupled with the ultrasound transducer to generate an ultrasound image; a touch screen display coupled with the image processor to display the ultrasound image; a touch processor coupled with the touch screen display to receive and process touch input from the entire touch screen display including the portion where the ultrasound image is currently being displayed, a computer aided processor coupled with the touch

processor to determine one or more geometric parameters based on input from the touch processor.

[0022] In one embodiment, the computer aided processor includes a computer aided measurement processor to determine at least one of: distance, perimeter, angle, ratio, area, volume, velocity, peak, and heart rate.

[0023] In one embodiment, the computer aided processor includes a computer aided diagnosis processor configured to generate diagnosis results based on a knowledge base.

[0024] In one embodiment, the computer aided processor is coupled with the image processor and the touch processor to allow interactive adjustment of the one or more geometric parameters via touching the touch screen display.

[0025] In one embodiment, the touch processor dynamically adjusts sensitivity and scale of the adjustment of the one or more geometric parameters.

[0026] In one embodiment, the one or more geometric parameters are determined based on an initial touch input identifying a location or an area and based on an analysis of the ultrasound image.

[0027] In a further aspect, a computer storage medium storing instructions configured to instruct one or more microprocessors of an ultrasound imaging apparatus having an ultrasound transducer, a beamformer and a touch screen display to at least: generate an ultrasound image based on signals from the ultrasound transducer; display the ultrasound image on the touch screen display; receive and process touch input from the entire touch screen display including the portion where the ultrasound image is currently being displayed; determine one or more geometric parameters based on input from the touch processor; provide a user interface allowing interactive adjustment of the one or more geometric parameters via touching the touch screen display; and generate a computer aided measurement or diagnosis result based on the one or more geometric parameters.

[0028] The disclosure includes methods and apparatuses which perform these methods, including data processing systems which perform these methods, and computer readable media containing instructions which when executed on data processing systems cause the systems to perform these methods.

[0029] Other features will be apparent from the accompanying drawings and from the detailed description which follows.

DETAILED DESCRIPTION

[0030] The following description and drawings are illustrative and are not to be construed as limiting. Numerous specific details are described to provide a thorough understanding. However, in certain instances, well known or conventional details are not described in order to avoid obscuring the description.

[0031] References to one or an embodiment in the present disclosure are not necessarily references to the same embodiment; and, such references mean at least one. One or more features described in reference to one or an embodiment can be viewed as optional, except in instances where it is apparent from the present description that the presence of other features explicitly requires, or excludes, the presence of such one or more features. Thus, the present disclosure includes all combinations of various features discussed in connection with different references to one or an embodiment, except certain combinations are excluded by ways of explicit discussion or obvious incompatibility.

[0032] The present disclosure includes a touch screen based computer aided measurement and/or diagnosis method and system. In at least some embodiments, the measurement process is simplified and made more intuitive and accurate by at least using a touch screen user interface. In at least some embodiments, the CAD is augmented with real time adjustments made using a touch screen user interface to improve the system diagnostic performance. Further details are provided below.

[0033] In one embodiment, an ultrasound imaging system is provided with a touch screen based user interface, which is configured to allow users to provide input based at least in part on touching a portion of a touch screen display, on which portion an ultrasound image is currently being displayed while the touching input is received. Allowing a user to provide touch input on the portion of the touch screen display where the ultrasound image is currently being displayed provides a large touch surface for input operations and allow the system to interpret touch input in a context sensitive manner to provide improved user experience.

[0034] In one embodiment, the touch screen based user interface allows the user to select, via touching the displayed image, a sub-region to cause the imaging system to perform, change, modify and/or adjust image processing tasks on the displayed image based on the region selected by the user.

[0035] In one embodiment, instead of utilizing only the user touch input to select a command that corresponding to the touch input, the touch screen based user interface identifies a command and/or parameters for the execution of the command, based on not only the touch input but also the underlying image that is being touched. In one embodiment, the underlying image is analyzed for the touch screen based user interface; and the analysis result is combined, by the touch screen based user interface, with the touch input to generate intelligently a command appropriate for the processing of the underlying image and corresponding to the touch input.

[0036] In one embodiment, the underlying image is a live ultrasound image, which updates periodically according to the most recent signals from the ultrasound transducer. In one embodiment, the underlying image is a frozen ultrasound image, which is based on the signals from the ultrasound transducer during a particular time period and not further updated according to recent signals from the ultrasound transducer.

[0037] Systems and methods of a touch screen based user interface in medical ultrasound imaging systems according to some embodiments are described in further details below.

[0038] FIG. 1 shows an ultrasound imaging system according to one embodiment. In FIG. 1, the ultrasound imaging system 100 includes an ultrasound transducer 104, an ultrasound beamformer 108 controlling the ultrasound transducer 104, a touch screen display 102 and a data processor 106 coupled with the ultrasound transducer 104 to generate ultrasound image and coupled with the touch screen display 102 to display the ultrasound image and receive user touch input.

[0039] In one embodiment, the data processor 106 is coupled with the ultrasound beamformer 108 to control the ultrasound transducer 104.

[0040] FIG. 2 shows a user interface for an ultrasound imaging system according to one embodiment. In FIG. 2, the ultrasound image 112 generated based on the signals from the ultrasound transducer 104 is displayed in at least portion of the touch screen 102.

[0041] In one embodiment, while the ultrasound image **112** is displayed on a portion of the touch screen **102**, one or more user interface elements can be displayed concurrently on a different portion of the touch screen **102**. Examples of such one or more user interfaces elements include icon image representations of function buttons, which can be selected via touch to activate the execution of pre determined image functions or to invoke other user interfaces to replace the currently displayed user interface elements and/or the ultrasound image **112**.

[0042] In one embodiment, the ultrasound image **112** is displayed on a portion of the touch screen **102** without concurrently displaying other conventional graphical user interface elements, such as icon buttons, menu buttons, text fields for receiving text input, etc. Some conventional graphical user interface elements may be overlaid on the ultrasound image **112** in response to the user touch input on the ultrasound image **112**.

[0043] In one embodiment, the user interface is configured to allow the user to touch the ultrasound image **112** displayed on the touch screen **102** to provide the touch input. The touch input is received while the ultrasound image **112** is displayed on the corresponding portion of the touch screen **102** being touched, without the display of a conventional graphical user interface element on the corresponding portion of the touch screen **102**.

[0044] In one embodiment, the touch input on the ultrasound image **112** is interpreted to generate an image processing command to process the ultrasound image **112** and provide an updated display of the ultrasound image **112**.

[0045] In one embodiment, different touch inputs are interpreted by the user interface as different touch gestures; and different touch gestures are pre-associated with different, pre-defined user interface functions (e.g., open a predefined user interface, open a pre-identified document or form) and/or image processing functions (e.g., zooming in or zooming out, edge enhancing the image, adjusting the brightness or contrast of the image).

[0046] In one embodiment, a touch input represents a user request to improve the image; and the image is analyzed to select an image processing function to improve the image. In one embodiment, the improvement is based on the analysis of a local region touched by the user; and the image processing function may be applied to the same local region, or the entire ultrasound image. In one embodiment, the improvement is applied on a local region touched by the user, based on the image analysis of the location region or the entire ultrasound image. [This seems belong to the first patent application.]

[0047] In one embodiment, the touch gestures are mapped to predefined user interface operations without relying upon the image properties of the ultrasound image **112** being touched. Thus, the same touch gesture applied on different ultrasound images **112** causes the system to apply the same user interface function or image processing function that is pre-associated with the touch gesture.

[0048] In one embodiment, a touch gesture includes a sequence of touching operations that identify one or more locations or regions in the ultrasound image **112** and a desired operation based on the identified one or more locations or regions. In one embodiment, the identified one or more locations or regions are used for the desired operation in processing the ultrasound image **112**.

[0049] In one embodiment, the ultrasound image **112** as displayed is considered a graphical user interface element,

which may have a set of user interface/image processing functions pre-associated with the graphical user interface element, regardless of the content of the ultrasound image **112**.

[0050] In one embodiment, the ultrasound image **112** as displayed is considered a graphical user interface element, which may have a set of user interface/image processing functions associated with the graphical user interface element based on the certain properties of the ultrasound image **112**. The properties of the ultrasound image **112** may be based on a statistical analysis of the ultrasound image **112** (e.g., brightness, contrast) or based on a pattern recognition analysis of ultrasound image **112** (e.g., predefined tissue features captured in the ultrasound image **112**). Different portions of the ultrasound image **112** that have different image characteristics and/or captured features or image patterns may be assigned dynamically with different graphical user interface functions.

[0051] In one embodiment, the properties of the ultrasound image **112** are determined in response to touch input and used to determine the graphical user interface functions to be invoked in response to the touch input. The properties are determined based on the entire ultrasound image **112** as displayed in one embodiment or alternatively, based on a portion of the ultrasound image **112** as identified via the touch gesture.

[0052] For example, in one embodiment, when a portion of the ultrasound image **112** as identified via the touch gesture has a contrast level below a threshold, the touch gesture is interpreted as a request to improve the contrast level, and when the contrast level is with a predetermined range, the touch gesture is interpreted as a request to perform edge enhancement on the ultrasound image **112**, if there are detected edge in the area touched by the hand **110** of the user (or a stylus).

[0053] In one embodiment, the ultrasound image **112** is analyzed to generate a scale of operation; and the touch gesture is interpreted based on the scale of operation to generate parameters for an image processing operation that is performed as a response to the touch gesture.

[0054] When the touch input/gesture is interpreted based on the context provided by the image properties and/or features captured in the ultrasound image **112**, the user interface can process the touch input more intelligently.

[0055] FIG. 3 shows a portion of an ultrasound imaging system configured to process touch input for computer aided measurement and/or computer aided diagnosis according to one embodiment. In FIG. 3, the touch screen display **102** includes a display unit **122** configured to display images and a touch sensor **124** configured to detect touch input on the display unit **122**.

[0056] In one embodiment, the touch sensor **124** is configured for the measurement of the locations over the display unit touched by one or more human fingers, or any pointing objects. In one embodiment, the touch sensor **124** is also configured for the measurement of the pressure of the touch. Various touch sensing technologies, currently known in the field and developed in the future, can be used in various embodiments of the touch sensor **124**. The disclosure is not limited to a particular type of touch sensing technique.

[0057] In FIG. 3, the data processor **106** includes an image processor **126** configured to generate images for display on the display unit **122** (e.g., based on the signal input from the ultrasound transducer **104**). The data processor **106** further

includes a touch processor **128** configured to process the touch input generated by the touch sensor **124**. The touch sensor **124** is configured to generate processing commands in response to the touch input received from the touch sensor **124**.

[0058] In one embodiment, the touch processor **128** is configured to generate commands based on not only the touch input received from the touch sensor **124**, but also the image information received from the image processor **126**.

[0059] In one embodiment, the ultrasound image **112** displayed on the display unit **122** is analyzed to provide an image context; and the touch sensor **124** is configured to interpret the touch input based on the image context to identify, select, or generate a context sensitive processing command for the image processor.

[0060] In one embodiment, the image context is determined based on a portion of the touch input. For example, a touch input may specify one or more locations or a region; and the touch processor **128** is configured to request the image processor to obtain the image context based on the one or more locations or a region in the ultrasound image **112**; and the image context is further used to interpret the remaining portion of the touch input to transform the ultrasound image **112**.

[0061] Examples of the image context include the brightness level of the ultrasound image **112**, the contrast level of the ultrasound image **112**, a pattern recognized as being corresponding to a feature (e.g., a bone, an organ, and a tumor), the location and/or size of the recognized feature, etc.

[0062] For example, in one embodiment, a touch input at a location corresponding to a recognized feature may be interpreted as a request to adjust the zoom level and the center point to present the recognized feature using the available display area on the display unit **122**, when the recognized feature is currently displayed in a small area of the display unit.

[0063] For example, in one embodiment, when a touch input is at an ultrasound image having a contrast level lower than a predetermined threshold but not at a location on a recognized feature, the touch input is interpreted as a request to adjust the contrast level of the ultrasound image **112**.

[0064] Thus, in one embodiment, the touch processor **128** takes the user inputs originated from the touch sensor **124** of the touch screen display **102** and image information derived by the image processor from the ultrasound image **112** currently being displayed to on the display unit **122** of the touch screen display **102** to intelligently generate commands or instructions to operate the image processor **126** and/or the ultrasound imaging system **100**.

[0065] In one embodiment, the user inputs originated from the touch sensor **124** and combined with the image information for the determination of the commands or instructions include the inputs from the area currently used to display the ultrasound image **112** and/or the inputs from the area configured to display graphical user interface elements, such as icon buttons, menu buttons, sliders, etc.

[0066] In one embodiment, in response to the user touch input, the data processor **126** is configured to generate one or more conventional graphical user interface elements, such as buttons, sliders, text input boxes, etc., which are temporarily displayed over the ultrasound image **112** to further collect user inputs. In one embodiment, the displayed conventional graphical user interface elements overlaid on the ultrasound image **112** is translucent, allowing the user to partially see ultrasound image **112** through the displayed conventional

graphical user interface elements. The translucent graphical user interface elements provide hints to assist the user in providing input.

[0067] For example, when there are ambiguities regarding to the intent of the user, a plurality of choices can be presented to allow the user to select one from a plurality of possible processing options.

[0068] For example, when there are multiple processing options of similar priorities, the options can be displayed for an explicit selection by the user.

[0069] For example, the graphical user interface elements may be presented in one embodiment to receive user specified parameters for an operation selected based on the image context and the previous touch input.

[0070] Various types of image information can be derived from either a local region of the ultrasound image **112** touched by the user or the entire ultrasound image **112**. The derived image information, which is typically different from the ultrasound image **112** itself, can be used by the touch processor **128** to deduce optimal commands for controlling the image processor **126** and/or the ultrasound imaging system **100**. In one embodiment, the deduced commands may cause the image processor **126** to perform a local image processing operation within the local region identified via user touching or a global image processing operation for the entire ultrasound image **112**.

[0071] Examples of the image processing operations include imaging parameter adjustment, zooming, translation, measurement, editing, deletion, copying, and combinations of such image processing operations. The imaging parameter adjustment can be applied to a local region touched by the user or the global ultrasound image **112**. Examples of the imaging parameters that may be adjusted via such touch inputs include spatial resolution, temporal resolution, contrast, dynamic range, focal point, display depth, gain, time gain control (TGC), pulse repetition frequency (PRF), etc.

[0072] In one embodiment, the touch processor **128** is configured to determine the touch direction, speed, position, pressure, order of multiple touch operations, and combinations of multiple touch operations to determine an image processing operation intended by the user.

[0073] Examples of image information and properties that can be used as the image context for the determination of the image processing operation intended by the user include statistics data, such as mean brightness, noise level, different tissue texture, tissue motion, boundary, etc.

[0074] In one embodiment, the touch processor **128** is configured to detect one or more input signals from the touch sensor **124** of the touch screen display **102**; and in response, the touch processor **128** analyzes the input signals to recognize one or more predefined touch gestures. The touch processor **128** optionally instructs the image processor **126** to process and analyze the currently displayed ultrasound image **112** to obtain image analysis results. Based on the image analysis results and the recognized touch gestures, the touch processor **128** is configured to generate one or more commands instructing the image processor **126** to transform the ultrasound image **112** or adjust the mode or parameters to generate the ultrasound image **112**.

[0075] In one embodiment, the touch processor **128** provides the recognized touch gesture to the image processor **126**; and the image processor **126** is configured to use the image analysis results and the recognized touch gesture to determine the one or more commands for transforming the

ultrasound image **112**, or adjusting the mode or parameters to generate the ultrasound image **112**.

[0076] Examples of image analyses to obtain image context for the determination of the one or more commands include, but not limited to, filtering, statistical analyses, feature extraction, edge detection, and pattern recognition. For instance, local image mean brightness can be computed for image based dynamic gain control (DGC) adjustment.

[0077] Examples of the determined command include, but not limited to, image optimization, edge enhancement, restoration, segmentation, and imaging parameter adjustment.

[0078] In FIG. 3, the data processor **106** further includes a computer aided measurement (CAM) processor **132** and a computer aided diagnosis (CAD) processor **134**, each coupled with the touch processor **128** to receive data and/or commands generated based on the touch input detected by the touch sensor **124**.

[0079] Although FIG. 3 illustrates an embodiment that includes both the CAM processor **132** and the CAD processor **134**, the data processor **106** of FIG. 1 in some embodiments has the CAM processor **132** but not the CAD processor **134**; and in other embodiments, the data processor **106** of FIG. 1 in some embodiments has the CAD processor **134** but not the CAM processor **132**.

[0080] In FIG. 3, the CAD processor **134** receives input from the CAM processor **132** for improved performance and user experience.

[0081] In one embodiment, the CAM processor **132** is implemented as specialized software and/or firmware running on one or more general purpose or special purpose microprocessors. The CAM processor **132** can also be implemented as a special purpose digital circuit without software and/or firmware instruction. The CAM processor **132** is configured to assist the user to perform various measurements based on the touch input result processed by the touch processor **128**. The CAM processor **132** may provide feedback to the touch processor **128** to adjust the way the touch processor **128** processes the touch inputs.

[0082] For example, the touch processor **128** may interpret certain touch inputs as user identification of geometric input relative to the ultrasound image **112** presented on the touch screen. The geometric input may include one or more points, one or more line/curve segments, and one or more regions. The CAM processor **132** is configured to determine one or more measurement based on the geometric input, provided by the touch processor **128** according to the signals for the touch sensors.

[0083] In one embodiment, the CAM processor **132** is capable of measuring, based on the user touch input, parameters such as distance, perimeter, angle, ratio, area, volume, velocity, peak, heart rate, and auto trace, etc.

[0084] In one embodiment, the touch processor **128** is configured to interpret a predetermined touch gesture as a request to perform a measurement, and one or more subsequent touch inputs as geometric parameters for the measurement. The CAM processor **132** is configured to determine the measurement and instruct the image processor **126** to generate, on the display unit **122**, a visual feedback of the geometric parameters used in the calculation. Based on the visual feedback, the user may determine whether the measurement as specified via the previous touch input is of sufficient accuracy. If the user determines that the visual feedback indicates inaccuracy in the geometric parameters specified via the previous touch input, the user may provide further touch input to adjust to

geometric parameters. For example, in one embodiment, the visual feedback represents new user interface elements that can be selected to fine tune the parameters. The user interface dynamically adjusts the sensitivity and/or the scale for the fine tuning of the parameters. Thus, the user can easily provide accurate geometric parameters through a few iterations of touch inputs at different scale and sensitivity.

[0085] In one embodiment, the CAD processor **134** is implemented as specialized software and/or firmware running on one or more general purpose or special purpose microprocessors. The CAD processor **134** can also be implemented as a special purpose digital circuit without software and/or firmware instruction.

[0086] In one embodiment, the CAD processor **134** has two operating modes: interactive mode and automatic mode. In the interactive mode, the CAD processor **134** allows the user to influence the calculation performed by the CAD processor **134** using the touch screen inputs. In the automatic mode, the CAD processor **134** completes the diagnosis without considering any touch input received from the touch screen display **102**.

[0087] In one embodiment, the CAD processor **134** performs a diagnosis through the operations of image preprocessing, image segmentation, image structure analysis, and structure classification.

[0088] In one embodiment, the image analysis is performed for a local region within the ultrasound image **112** to obtain the image context for the determination of the one or more commands. For example, a user may draw an arbitrary shape via touching, using a hand **110** (or a stylus), to define a region of interest (ROI) **114** as illustrated in FIG. 4. After the region **114** is defined via touching, the user may further tap a point inside the region **114** to request the region **114** to be processed.

[0089] In one embodiment, the image processor **126** analyzes the region **114** of the ultrasound image **112** but not the region outside the region **114** to determine a local image context, based on which a processing command is determined for the tap at the point side the region **114**.

[0090] In one embodiment, the image processor **126** analyzes the ultrasound image **114**, including both the region **114** and the region outside the region **114**, to determine a global image context, based on which a processing command is determined for the tap at the point side the region **114**.

[0091] In one embodiment, the processing command, determined based on the local image content or the global image context, is applied to transform the region **114** within the ultrasound image **112**, but not the region outside the region **114**. Alternatively, the processing command can be applied globally to the entire ultrasound image **112**.

[0092] In one embodiment, the region of interest (ROI) **114** has an arbitrary shape, determined according to the path of touch made via the hand **110** of the user. In one embodiment, the path of touch is converted into a regular shape, such as a box, an oval, a circle, etc., to simplify processing.

[0093] In one embodiment, the image analysis for the image context and/or the processing command to transform is applied to the live ultrasound images that are periodically updated according to the input from the ultrasound transducer **104**. Alternatively, the image analysis and/or the processing command can be applied to a frozen image that is based on a particular set of input obtained from the ultrasound trans-

ducer **104** within a particular time period, where the input from the ultrasound transducer **104** is not updated with the passage of time.

[0094] In one embodiment, a dynamic ROI **114** is generated according to the location and motion of a user finger or a pointing device, such as a stylus. Image analysis performed within the ROI **114** to obtain the image context may be the operation of filtering, statistical analyses, feature extraction, edge detection, and pattern recognition, etc to obtain local image context. Such local image analysis can be applied to the live ultrasound image **112** or a frozen ultrasound image **112**.

[0095] In one embodiment, after a dynamic ROI **114** is identified, an adaptive image optimization process is applied to the local image inside the ROI **114** as a response to a tap on a point inside the region **114**. For instance, in response to the tap on the point inside the region **114**, edge enhancement is applied if the ROI **114** contains boundaries; or a smoothing filter is applied if the ROI **114** has a speckle noise level above a threshold. Thus, the results of the boundary detection and speckle noise level evaluation performed on the ROI **114** provide the image context for the selection of the edge enhancement operation and/or the smoothing filter operation, as a response to the touch input on the ROI **114** from the user.

[0096] In one embodiment, after the touch sensor **124** detects one or more touch inputs, the touch processor **128** analyzes the touch inputs to identify one or more instructions represented by the touch input. The CAM processor **132** performs initial measurement based on the output of the touch processor **128** and then instructs the image processor **126** to display the measurement results and the geometric parameters used for the computation of the measurement results. If based on the visual feedback of the geometric parameters and the measurement results, the user determines that the measurement is acceptable, the user may provide a touch input to accept the measurement. In some embodiments, the measurement is accepted if the user does not provide a touch input to reject the measurement. If the user observes inaccuracy in the visual feedback, the user may refine the measurement process with additional touch screen based instructions. The refinement can be local or global. For example, if the user wants to modify one corner of a border, the user interface allows the user to readjust the border line with a touch of the touch screen display **102** with one finger or any stylus type tool. For example, the user interface allows the user to use two fingers to touch the touch screen display **102** and reduce or increase the distance between the touch points of the two fingers to reduce or increase the size of a closed border. For example, the user interface allows the user to touch a border representation displayed on the touch screen display **102** and move the touch point to adjust the border of a fetal head.

[0097] In one embodiment, after the touch sensor **124** generates touch signals in response to user touch on the touch screen display **102**, the touch processor **128** analyzes the touch signals to identify one or more input instructions corresponding to the touch signals. The CAM processor **132** performs an automatic measurement based on the one or more input instructions and then instructs the image processor **126** to display the result of the automatic measurement. For example, if it is detected that the user touches a place inside an object shown in the ultrasound area **112** of the touch screen display, the CAM processor **132** analyzes the ultrasound image **112** to automatically detect the border of the object as shown in the ultrasound image **112** and measures the

diameter, perimeter, and/or area of the object defined by the border. The object can be a heart chamber, a fetal head, bladder, gall bladder, or other organs and lesions. The detected border is drawn on over the ultrasound image **112** to provide a visual feedback of the detected border that is used as a geometric parameter for the computation of the measurements. Based on the visual inspection of the alignment between the visual feedback of the border used in the calculation and the underline object as in the ultrasound image, the user may decide to accept the measurement or reject the measurement. The user may indicate the decision to accept or reject the measurement result using a touch gesture performed on the touch screen. The user interface may allow the user to touch the visual feedback of the border and move the touch point to adjust the border. The user interface may allow the user to draw a region of interest (ROI) **114** to limit the border detection operation with the region of interest **114**, or suggest an initial estimate of the border; and the CAM processor **132** performs the measurement of the desired parameters based on the region of interest **114** drawn by the user via the touch of the touch screen display **102**. For instance, intima-media thickness (IMT) measurement can be done in such a way.

[0098] In one embodiment, after the touch sensor **124** generates touch signals in response to user touch on the touch screen display **102**, the touch processor **128** analyzes the touch signals to identify one or more input instructions corresponding to the touch signals. In response to the one or more input instructions, the CAD processor **134** performs an automatic diagnosis and then displays the results. For example, the CAD processor **134** detects a lesion in an organ and displays diagnostic information about the lesion based on the properties of the lesion and the disease knowledge database on the system. The properties may include size, shape, orientation, border smoothness, contrast ratio, and acoustic shadow. The diagnostic information may display that the detected lesion is a tumor with a specific level of confidence. The CAD processor **134** may instruct the image processor **126** to draw geometric elements illustrating the properties, such as size, shape, orientation, etc., that are used in the diagnosis for visual confirmation by the user.

[0099] In one embodiment, after the touch sensor **124** generates touch signals in response to user touch on the touch screen display **102**, the touch processor **128** analyzes the touch signals to identify one or more input instructions corresponding to the touch signals. In response to the one or more input instructions, the CAD processor **134** performs diagnoses with input from the user in an interactive way. For instance, the CAD processor **134** may show a segmented lesion and display some diagnostic data and information on the screen for the user to determine whether the results are satisfactory. If not, the user can adjust the CAD algorithm, input new instructions using the touch screen, and then rerun the diagnosis. For example, the visual feedback of the geometric parameters used in the diagnosis can be overlaid on the ultrasound image **112**; and the user may determine whether the diagnosis identified by the CAD processor **134** is acceptable based on the alignment in position, shape, orientation, size, etc, between the visual feedback of the geometric parameters used in the diagnosis and the underline ultrasound image **112** displayed on the touch screen display **102**. If misalignment is visually detected by the user, the user inter-

face allows the user to provide touch input to adjust the geometric parameters to assist the CAP processor 134 to make an improved diagnosis.

[0100] In one embodiment, after the touch sensor 124 generates touch signals in response to user touch on the touch screen display 102, the touch processor 128 analyzes the touch signals to identify one or more input instructions corresponding to the touch signals. In response to the one or more input instructions, the CAM processor 132 performs an initial measurement and instructs the image processor 126 to display the measurement results, together with visual feedback of the geometric parameters used in the measuring operation. The visual feedback is overlaid on the ultrasound image to allow the user to inspect the quality of the geometric parameters used in the measuring operation. If the user decides not to accept the measurement result, the user may refine the measurement process by providing touch inputs to adjust the geometric parameters, and if the user decides to accept the measurement result, as indicated via a touch input on the touch screen display 102, the CAD processor 134 proceeds to make a diagnosis. Based on the touch input made to accept the measurement generated by the CAM processor 132, the CAD processor 134 may operate in an automated way, or in an interactive way. When running in an interactive mode, the CAD processor 134 makes diagnoses using the measurement results from the CAM processor 132 and the touch input provided by the user using the touch screen display 102.

[0101] Through at least some of the arrangements discussed above, the measurement can be performed on the ultrasound imaging system 100 more intuitively, due to the combination of touch screen user interface and CAM processor. Further, the use of a CAD processor in an interactive mode overcomes the limitation of both pure CAD and manual diagnostic processes. The combination of the CAD processor and the CAM processor improves the accuracy of diagnosis and provides an intuitive user experience.

[0102] FIG. 5 shows a method to perform computer aided measurement or diagnosis according to one embodiment. In FIG. 5, after the ultrasound imaging system 100 enters the CAM and CAD mode (e.g., via the selection of a menu option, or via a touch gesture performed over the ultrasound image 112 on the touch screen display 102), the touch processor 128 determines 204 whether the current touch input is for a CAM command.

[0103] If it is determined 204 that the current touch input is for a CAM command, the CAM processor 132 computes 206 an initial measurement. The result of the initial measurement and the geometric parameters, such as points, lines, curves, areas, etc., that are used in the computation of the initial measurements are displayed over the ultrasound image 112 by the image processor 126.

[0104] If it is determined that the user rejects, or does not accept, the measurement results, the touch processor 128 is configured to receive 206 and process touch inputs to refine the measurement 206; otherwise, the ultrasound imaging system 100 saves 220 and displays the measurement results accepted by the user.

[0105] If it is determined 204 that the current touch input is for a CAD command, the touch processor 128 further determines 212 whether the CAD processor 134 is instructed to run in an automatic mode, or in an interactive mode.

[0106] If it is determined 212 that the CAD processor 134 is instructed by the user to run in an automatic mode, the CAD

processor 134 performs automatic computed aided diagnosis and instructs the image processor 126 to display 220 the results, without considering touch input between the starting point of the automatic computed aided diagnosis and the display of the diagnosis result.

[0107] If it is determined 212 that the CAD processor 134 is instructed by the user to run in an interactive mode, the CAD processor 134 performs interactive computer aided diagnosis, in which the CAD processor 134 is to receive at least one input from the touch processor 128, responsive to at least one user touch, between the starting point of the automatic computer aided diagnosis and the display of the diagnosis result. The result of the initial diagnosis and the geometric parameters, such as points, lines, curves, areas, etc., that are used in the computation of the initial diagnosis are displayed over the ultrasound image 112 by the image processor 126. The touch processor 134 is configured to determine whether the received touch input is for accepting the CAD result. If it is determined 218 that the received touch input is not for accepting the CAD result, the touch processor 128 processes further touch inputs to adjust parameters for the CAD processor 134 to refine diagnosis result.

[0108] If it is determined 218 that the received touch input is for accepting the CAD result, the diagnosis result is saved 220.

[0109] FIG. 6 shows a method to perform computer aided measurement and diagnosis according to one embodiment. In FIG. 6, after the ultrasound imaging system 100 enters the CAM and CAD mode (e.g., via the selection of a menu option, or via a touch gesture performed over the ultrasound image 112 on the touch screen display 102), the touch processor 128 instructs the CAM processor 132 to perform one or more measurement 234. The touch processor 128 then determines whether the currently received touch input is for CAD; and if not, the touch processor 128 is configured to receive 238 and process touch input to adjust CAM parameters for the CAM processor 132 to perform one or more measurement 234.

[0110] If it is determined 236 that the currently received touch input is for CAD, the CAD processor 134 is instructed to perform interactive CAD 240. After a diagnosis is reached using a set of geometric parameters, the touch processor 128 determines 242 whether the currently received touch input for accepting the CAD result or not; and if not, the touch processor 128 is configured to receive 244 and process touch input to adjust CAD parameters for the CAD processor 134 to perform 240 interactive CAD.

[0111] In one embodiment, one or more other input devices, such as a mouse, a keyboard, a switch, a voice recognition system, etc., can be used in combination with the touch screen display 102 to receive input signals corresponding to at least some of the input parameters discussed in the present disclosure. For example, the determination of whether 204 the measurement is to be accepted or rejected can be based on a touch input, an input signal from a switch, keyboard, mouse, or a voice recognition system. For example, the determination of whether 218 to accept the CAD result can be based on a touch input, an input signal from a switch, keyboard, mouse, or a voice recognition system. For example, the determination of whether 204 the current command is for a CAM command can be based on a touch input, an input signal from a switch, keyboard, mouse, and/or a voice recognition system. For example, the determination of whether 212 the current command is for an automatic or

interactive CAD command can be based on a touch input, an input signal from a switch, keyboard, mouse, and/or a voice recognition system. For example, the determination of whether **236** the current input is for CAD can be based on a touch input, an input signal from a switch, keyboard, mouse, and/or a voice recognition system. For example, the determination of whether **242** the received input is for accepting the CAD result or not can be based on a touch input, an input signal from a switch, keyboard, mouse, and/or a voice recognition system. In one embodiment, a combination of the input from two or more input devices is used to indicate a signal to invoke a command or represent an input parameter. Some of the input commands or parameters discussed in the present disclosure can be detected or determined based on a predetermined pattern of input signals from one or more input devices, which may include some of the devices, such as the touch screen display **102**, a mouse, a keyboard, a switch, a voice recognition system, a trackball, a touch pad, a joystick, etc. In one embodiment, at least some of the touch inputs discussed above is in connection with input signals from one or more other devices. In one embodiment, at least some of the touch inputs discussed above can be replaced with inputs from input devices other than the touch screen display **102**. In one embodiment, the ultrasound imaging system **100** includes one or more such input devices, but not others. Some of the commands and/or input parameters can be based on one or input devices without using the touch screen display **102**. Thus, the disclosure is not limited to receiving input solely from the touch screen display **102**.

[0112] In one embodiment, at least a portion of the touch input discussed above in connection with the operation of the CAM processor **132** and the CAD processor **134** is received from an area of the display unit **122** of the touch screen display **102**, on which area the ultrasound image **112** is displayed.

[0113] In one embodiment, at least a portion of the touch input is received from an area that is outside the ultrasound image **112** and that displays graphical representation of user interface elements that are separate from the ultrasound image **112**.

[0114] In one embodiment, at least a portion of the touch input is received from a graphical representation of one or more user interface elements overlaid in a partially transparent manner over the ultrasound image **112**.

[0115] In one embodiment, at least a portion of the touch input identifies a region **114** of interest within the ultrasound image **112**.

[0116] In one embodiment, the image processor **126**, the touch processor **128**, and the CAD processor **134** are implemented using separate hardware. For example, the image processor **126**, the touch processor **128**, the CAM processor **132**, and/or the CAD processor **134** can be implemented using application-specific integrated circuit (ASIC) or field-programmable gate array (FPGA). Alternatively, the image processor **126**, the touch processor **128**, the CAM processor **132**, and/or the CAD processor **134** can be implemented using general purpose microprocessor controlled by firmware and/or software. In one embodiment, the image processor **126**, the touch processor **128**, the CAM processor **132**, and the CAD processor **134** are configured to share one or more microprocessors.

[0117] Thus, at least one embodiment of the disclosure provides an ultrasound imaging system configured with a touch screen based user interface, which addresses at least

one of the limitations and/or problems in the conventional medical ultrasound imaging system equipped with touch screens.

[0118] An ultrasound imaging system according to one embodiment of the disclosure includes an ultrasound transducer **104**, a touch screen display **102**, a beamformer **108**, a data processing unit (e.g., data processor **106**) and an electronic circuit interconnecting the components.

[0119] In one embodiment, the data processing unit is configured to perform signal processing, image processing, and input/output handling.

[0120] In one embodiment, the input/output handling includes receiving touch input from the image area displayed on the touch screen display and using image information derived from the ultrasound image **112** currently being displayed on the touch screen display **102** to generate intelligently proper commands or instructions corresponding to the touch input.

[0121] In one embodiment, in response to the touch input received from the image area, the touch input is processed and analyzed to determine the intended instructions by the user. According to the determined instructions by the user, an image analysis is performed to derive image information from either a local region of the image presented on the image area of the touch screen display **102**, or the entire ultrasound image **112**. Based on the derived image information, one or more commands are then generated to perform imaging tasks for the processing the live or frozen ultrasound image **112**.

[0122] In one embodiment, the commands determined in accordance with the touch input and the derived image information are executed for local image processing within a location region **114** identified by the user touch input. Alternatively or in combination, the commands may be executed for global image processing of the entire ultrasound image **112**.

[0123] In one embodiment, a local region is predefined or preselected. In one embodiment, a local region **114** is defined or selected by the user via touch input. In one embodiment, the local region is where the user is touching (e.g., via simultaneously touching multiple points using multiple fingers, via sequentially touching a set of discrete points using one finger, or via sliding one or more fingers on the touch screen); and the image in the local region is a portion of the ultrasound image **112** displayed on the touch screen display **102**.

[0124] Limiting the processing of the image to a local region reduces the processing load on the data processing unit and can improve the response time. Thus, the result of the image processing can be provided in real time as the user providing input via touch input. For example, when the global image has 500×600 pixels and the local image has 20×30 pixels, the time used for the processing of the local image can be much shorter than that for the global image.

[0125] In one embodiment, the image processing operations associated with the determined instructions include imaging parameter adjustment, zooming, translation, measurement, editing, deletion, and copying. The imaging parameter adjustment can be either local or global.

[0126] In one embodiment, a local image processing operation is applied to the portion of image that is displayed within a predefined region (e.g., the image area of the touch screen, or a portion of the image area of the touch screen); and a global image processing operation is applied to the entire ultrasound image which may have a portion that is outside the predefined region.

[0127] In one embodiment, the imaging parameters that can be adjusted via the determined instructions include spatial resolution, temporal resolution, contrast, dynamic range, focal point, display depth, gain, time gain control (TGC), pulse repetition frequency (PRF), etc.

[0128] In one embodiment, the data processing unit is configured to detect direction, speed, position, pressure, and order of user operations, and combinations of multiple user touch inputs. The detected direction, speed, position, pressure, and order of user operations, and combinations of multiple user touch inputs are used to determine the intended instructions of the user.

[0129] In one embodiment, the image information and properties that can be displayed in accordance with the intended instructions of the user include statistics such as mean brightness, noise level, different tissue texture, tissue motion, boundary, etc.

[0130] In one embodiment, the data processing unit is configured to detect input signal from the touch screen, analyze the input signal to determine the intended instruction of the user, process and analyze the displayed ultrasound image in accordance with the determined instruction of the user, and provide an output on the touch screen display based on the input instruction and the result of the image analysis.

[0131] In one embodiment, the touch input of the user can be generated not only from the control area of the touch screen, but also the image area of the touch screen.

[0132] In one embodiment, the properties of ultrasound image are processed and analyzed, and then combined with the user input instructions from the touch screen to generate proper commands, such as an optimal command that will be carried out to perform certain tasks, such as image enhancement. For example, the local image brightness is determined and used in one embodiment to generate gain adjustment commands for processing a local region of the ultrasound image in accordance with a touch input received in the image region of the touch screen display.

[0133] In one embodiment, local image processing and optimization are performed in response to the determined user instruction and based on local image properties.

[0134] In one embodiment, the touch screen operations are reconfigurable. The user can change or redefine some or all of predefined touch screen operations. For instance, a left-to-right move can be redefined as brightness increase instead of the default meaning: forward replay.

[0135] In one embodiment, after a touch input requesting reconfiguration is received from the touch screen display 102, the touch processor 128 analyzes and recognizes touch inputs that are provided by the user as the training inputs. The training inputs are used to determine parameters for recognizing subsequent touch inputs that are intended to signal the user request corresponding to the instruction or command that is being reconfigured. Thus, the touch recognition for the instruction or command, corresponding to a touch gesture is reconfigured based on the training results.

[0136] In one embodiment, for instance, in the default setting, pressing a point on an image with a finger tip for a certain amount of time like 2 seconds brings transmitting focus to the nearest location of the finger tip; the same operation can be reconfigured to perform a different task like drawing a box of a predetermined size corresponding to a region 114 of interest.

[0137] In the above discussion, examples of touch screen input processing are presented in connection with ultrasound

imaging systems. However, the touch screen image processing techniques can also be applied to other types of imaging systems and systems configured for displaying images, such as computed axial tomography (CAT or CT) systems, magnetic resonance imaging (MRI) systems, photoacoustic imaging systems, etc.

[0138] In the foregoing specification, the disclosure has been described with reference to specific exemplary embodiments thereof. It will be evident that various modifications may be made thereto without departing from the broader spirit and scope as set forth in the following claims. The specification and drawings are, accordingly, to be regarded in an illustrative sense rather than a restrictive sense.

What is claimed is:

1. An ultrasound imaging apparatus, comprising:
 - an ultrasound transducer;
 - a beamformer coupled with the ultrasound transducer to transmit and receive beams;
 - an image processor coupled with the beamformer to generate an ultrasound image;
 - a touch screen display coupled with the image processor to display the ultrasound image;
 - a touch processor coupled with the touch screen display to receive and process touch input from a portion of the touch screen display on which portion the ultrasound image is currently being displayed;
 - a computer aided measurement processor coupled with the touch processor to provide measurement results; and
 - a computer aided diagnosis processor coupled with the touch processor to provide diagnosis results.
2. The ultrasound imaging apparatus of claim 1, wherein at least one of the touch processor, the image processor, the computer aided measurement processor and the computer aided diagnosis processor includes one of: an application-specific integrated circuit and a field programmable circuit.
3. The ultrasound imaging apparatus of claim 2, wherein the computer aided diagnosis processor is further coupled to the computer aided measurement processor to receive measurement results for producing the diagnosis results.
4. The ultrasound imaging apparatus of claim 3, wherein the computer aided diagnosis processor operates based on a knowledge base.
5. The ultrasound imaging apparatus of claim 4, wherein when the touch processor determines that a current touch input received on the touch screen display is for accepting a measurement result from the computer aided measurement processor, the touch processor instructs the computer aided diagnosis processor to perform a diagnosis in an interactive mode.
6. The ultrasound imaging apparatus of claim 5, wherein when in the interactive mode, the computer aided diagnosis processor is configured to receive at least one input from the touch processor between starting of the diagnosis and presentation of a result for the diagnosis.
7. The ultrasound imaging apparatus of claim 1, wherein the computer aided measurement processor is coupled with the image processor to present one or more parameters used for producing the measurement results.
8. The ultrasound imaging apparatus of claim 7, wherein the one or more parameters are overlaid on the ultrasound image.
9. The ultrasound imaging apparatus of claim 8, wherein the touch processor is configured to determine whether a

currently received touch input is for adjusting the one or more parameters, or for accepting the measurement results.

10. The ultrasound imaging apparatus of claim **1**, wherein the computer aided diagnosis processor is coupled with the image processor to present one or more parameters used for producing the diagnosis results.

11. The ultrasound imaging apparatus of claim **10**, wherein the one or more parameters are overlaid on the ultrasound image.

12. The ultrasound imaging apparatus of claim **11**, wherein the touch processor is configured to determine whether a currently received touch input is for adjusting the one or more parameters, or for accepting the diagnosis results.

13. An ultrasound imaging apparatus, comprising:

an ultrasound transducer;

a beamformer coupled with the ultrasound transducer to transmit and receive beams;

an image processor coupled with the beamformer to generate an ultrasound image;

a touch screen display coupled with the image processor to display the ultrasound image;

a touch processor coupled with the touch screen display to receive and process touch input from a portion of the touch screen display on which portion the ultrasound image is currently being displayed;

a computer aided processor coupled with the touch processor to provide determine one or more geometric parameters based on input from the touch processor.

14. The ultrasound imaging apparatus of claim **13**, wherein the computer aided processor includes a computer aided measurement processor to determine at least one of: distance, perimeter, angle, ratio, area, volume, velocity, peak, and heart rate.

15. The ultrasound imaging apparatus of claim **14**, wherein the computer aided processor further includes a computer

aided diagnosis processor configured to generate diagnosis results based on a knowledge base.

16. The ultrasound imaging apparatus of claim **13**, wherein the computer aided processor further includes a computer aided diagnosis processor configured to generate diagnosis results based on a knowledge base.

17. The ultrasound imaging apparatus of claim **11**, wherein the computer aided processor is coupled with the image processor and the touch processor to allow interactive adjustment of the one or more parameters via touching the touch screen display.

18. The ultrasound imaging apparatus of claim **17**, wherein the touch processor dynamically adjusts sensitivity and scale of the adjustment of the one or more parameters.

19. The ultrasound imaging apparatus of claim **18**, wherein the one or more parameters are determined based on an initial touch input identifying a location or an area and based on an analysis of the ultrasound image.

20. A computer storage medium storing instructions configured to instruct one or more microprocessors of an ultrasound imaging apparatus having an ultrasound transducer, a beamformer and a touch screen display to at least:

generate an ultrasound image based on signals from the ultrasound transducer;

display the ultrasound image on the touch screen display;

receive and process touch input from a portion of the touch screen display on which portion the ultrasound image is currently being displayed;

determine one or more parameters based on input from the touch processor;

provide a user interface allowing interactive adjustment of the one or more parameters via touching the touch screen display; and

generate a computer aided measurement or diagnosis result based on the one or more parameters.

* * * * *

专利名称(译)	用于超声成像期间的用户交互的设备和方法		
公开(公告)号	US20140046185A1	公开(公告)日	2014-02-13
申请号	US13/572562	申请日	2012-08-10
[标]申请(专利权)人(译)	MO RUOLI 赵蛋花 赵明昌		
申请(专利权)人(译)	MO, RUOLI 赵, 蛋花 赵, 明昌		
当前申请(专利权)人(译)	MO, RUOLI 赵, 蛋花 赵, 明昌		
[标]发明人	MO RUOLI ZHAO DANHUA ZHAO MINGCHANG		
发明人	MO, RUOLI ZHAO, DANHUA ZHAO, MINGCHANG		
IPC分类号	A61B8/14		
其他公开文献	US8951200		
外部链接	Espacenet USPTO		

摘要(译)

一种超声成像设备，配置有触摸屏显示器和计算机辅助测量和/或诊断能力。响应于触摸输入，从超声图像的分析确定用于计算机辅助测量和/或诊断的图像参数。触摸屏用户界面允许用户以交互方式进一步调整用于计算机辅助测量和/或诊断的参数和/或其他系统参数。计算机辅助测量可以直接用于计算机辅助诊断，以提高准确性和用户体验。

