


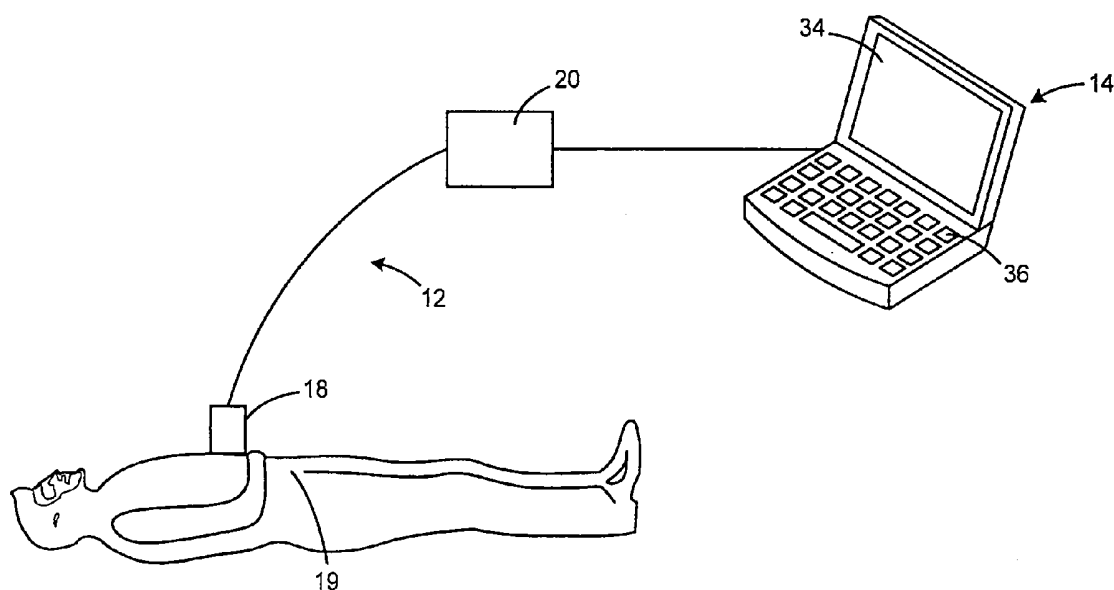

US 20160262728A1

(19) **United States**(12) **Patent Application Publication**  
**Barthe et al.**(10) **Pub. No.: US 2016/0262728 A1**(43) **Pub. Date: Sep. 15, 2016**(54) **ULTRASOUND SYSTEM AND METHOD FOR  
IMAGING AND/OR MEASURING  
DISPLACEMENT OF MOVING TISSUE AND  
FLUID**(71) Applicant: **Ardent Sound Inc.**, Mesa, AZ (US)(72) Inventors: **Peter G. Barthe**, Pheonix, AZ (US);  
**Michael H. Slayton**, Tempe, AZ (US);  
**Paul Jaeger**, Mesa, AZ (US)(21) Appl. No.: **14/966,377**(22) Filed: **Dec. 11, 2015****Related U.S. Application Data**(63) Continuation of application No. 11/538,794, filed on  
Oct. 4, 2006, now Pat. No. 9,241,683.**Publication Classification**(51) **Int. Cl.**  
**A61B 8/08** (2006.01)  
**A61B 8/06** (2006.01)**A61B 8/14** (2006.01)**A61B 8/00** (2006.01)(52) **U.S. Cl.**CPC ..... **A61B 8/5207** (2013.01); **A61B 8/461**  
(2013.01); **A61B 8/4411** (2013.01); **A61B**  
**8/488** (2013.01); **A61B 8/06** (2013.01); **A61B**  
**8/14** (2013.01); **A61B 8/4483** (2013.01)(57) **ABSTRACT**

A system and method for improved imaging is disclosed. An exemplary system provides a peripheral ultrasound system connected to a host computer with a plug-and-play interface such as a USB. An exemplary system utilizes a dedicated graphics processing unit such as a graphics card to analyze data obtained from a region of interest to produce an image on one or more output units for the user's viewing. Based on the image displayed on the output units, the user can determine the velocity of the moving tissue and fluid. The system of the present invention can be used to produce a Doppler color flow map or for power Doppler imaging.



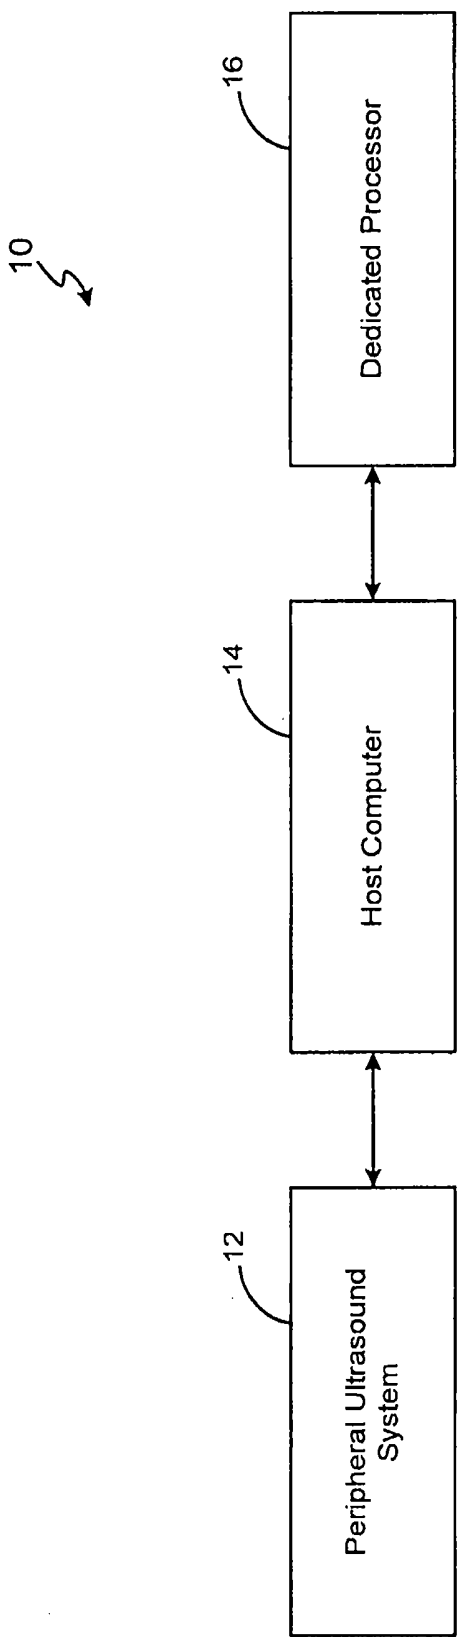


FIG. 1

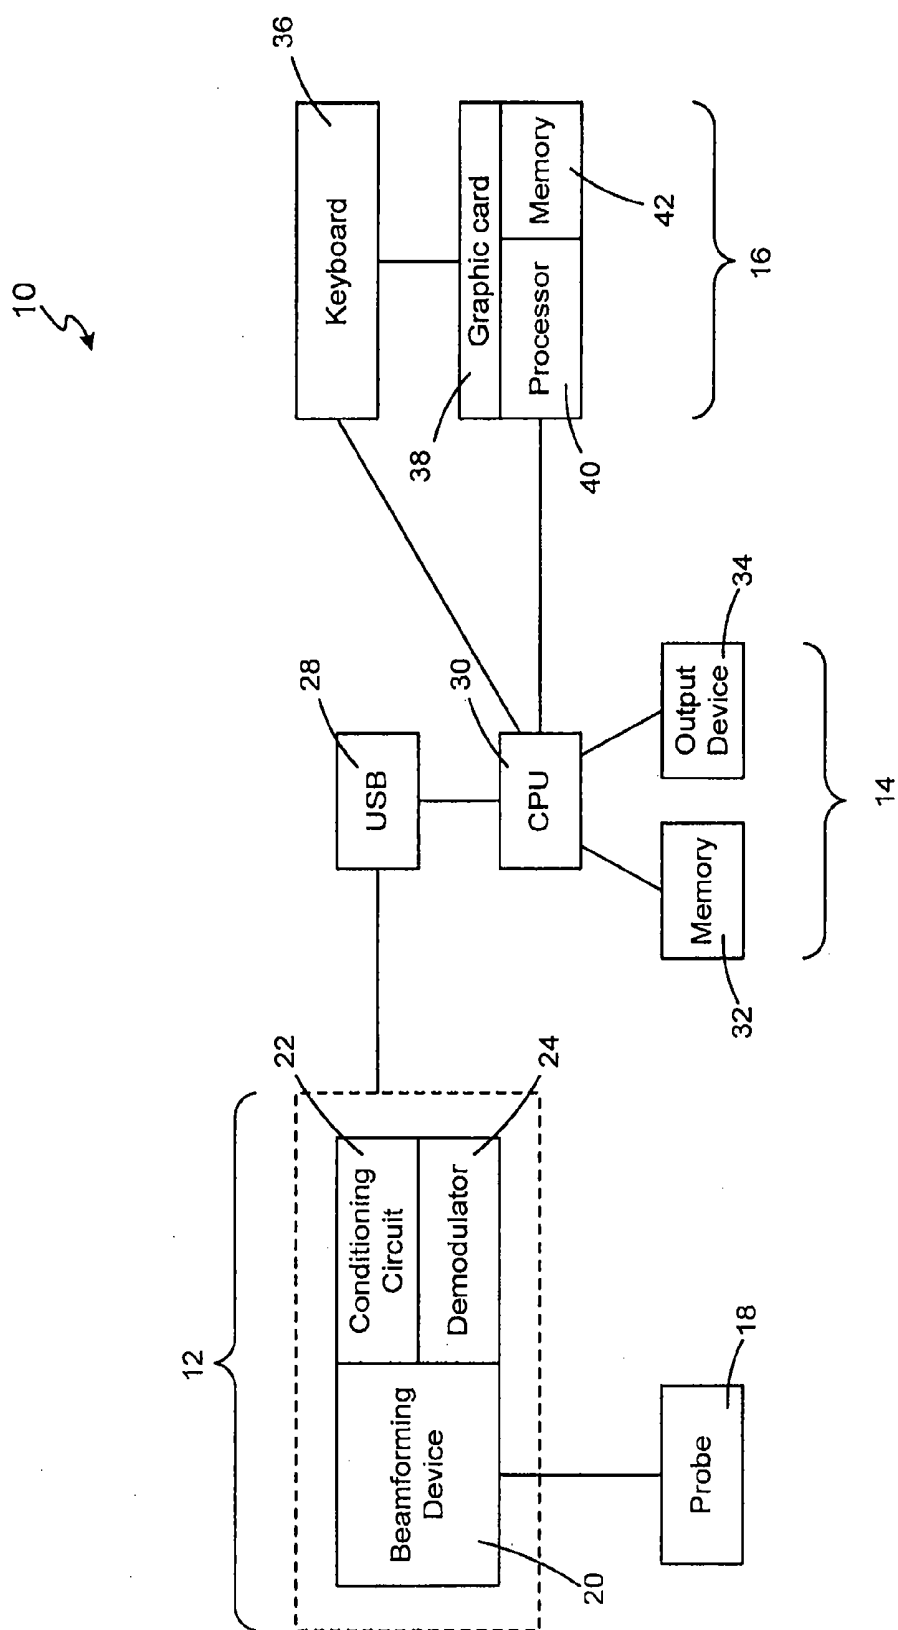


FIG. 2

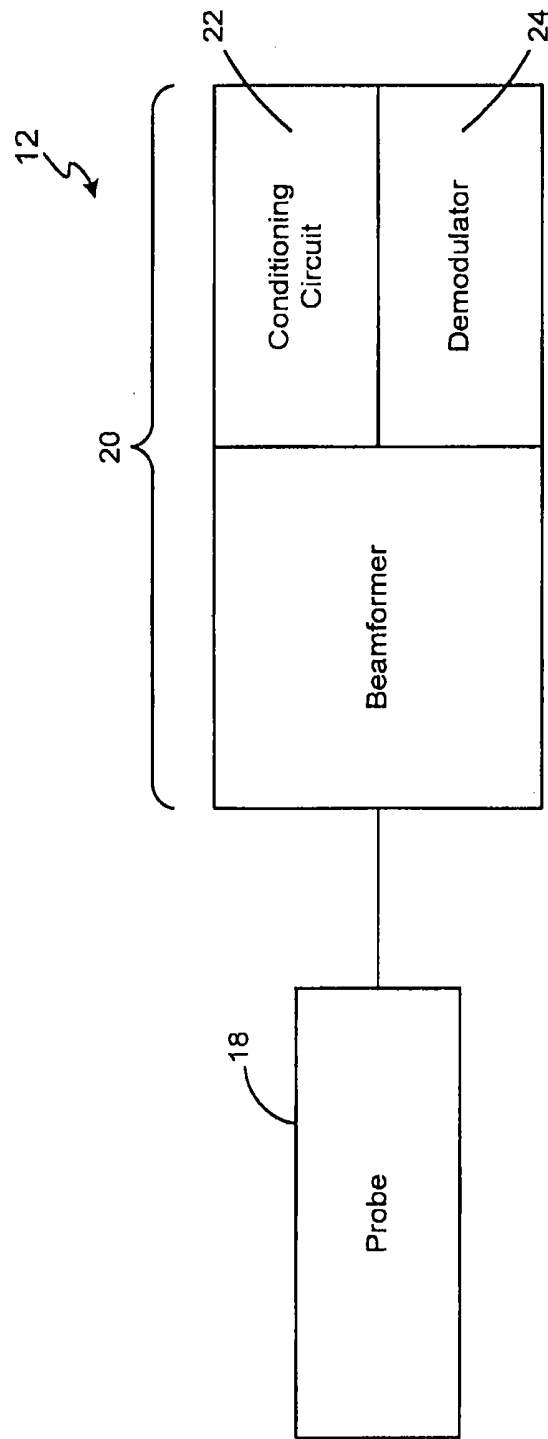
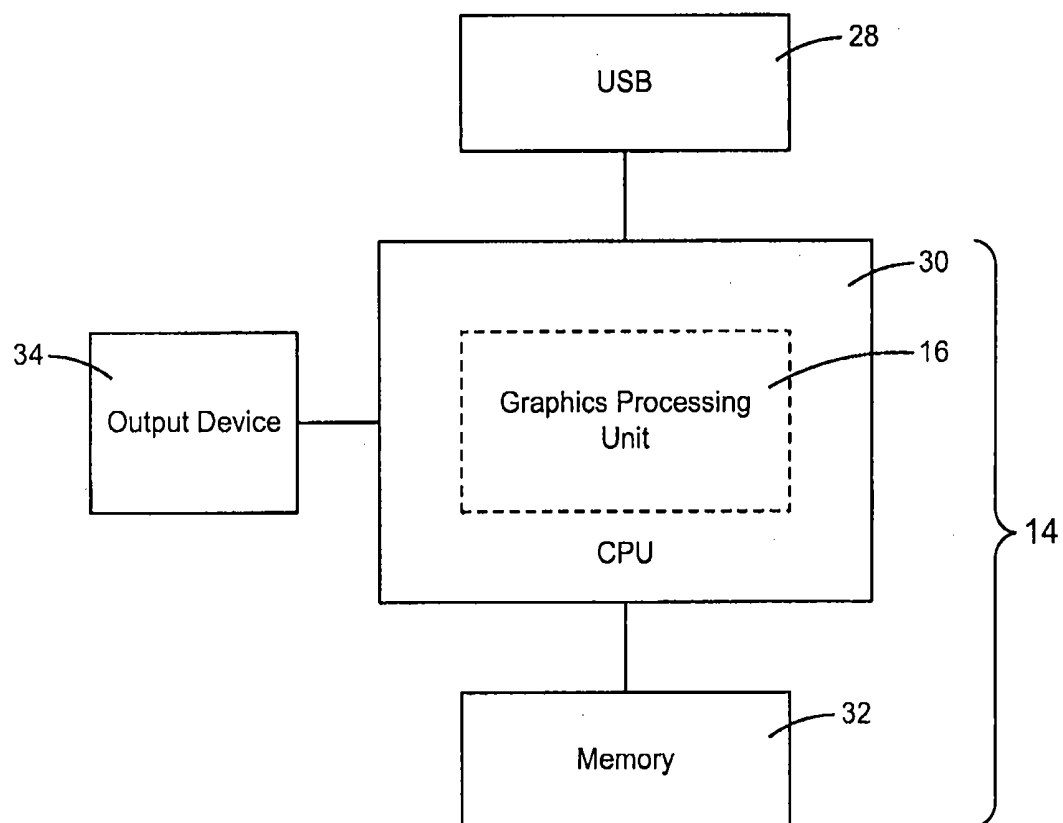


FIG. 3



**FIG. 4**

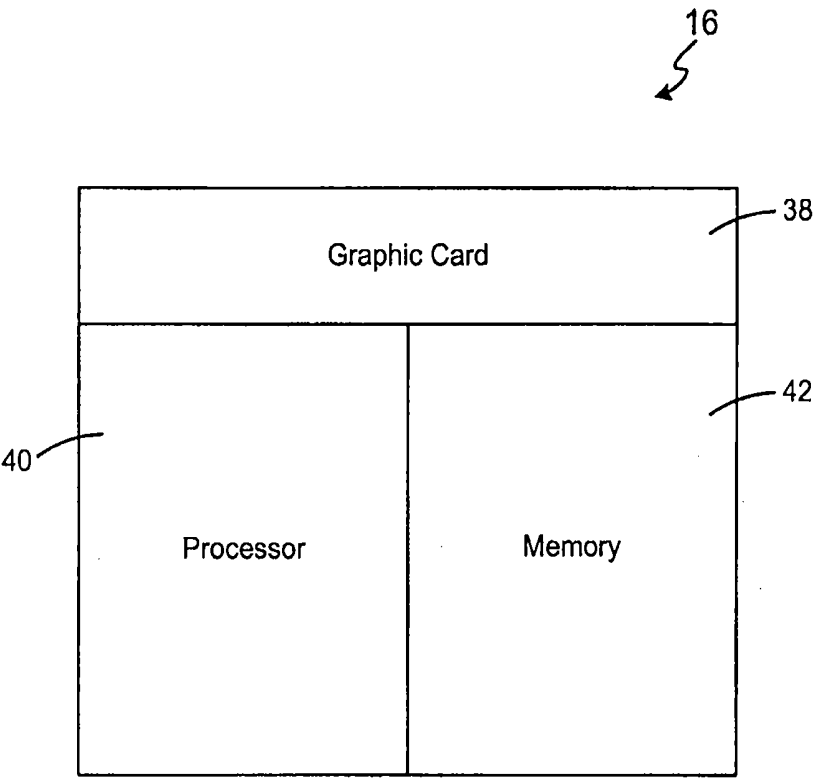


FIG. 5

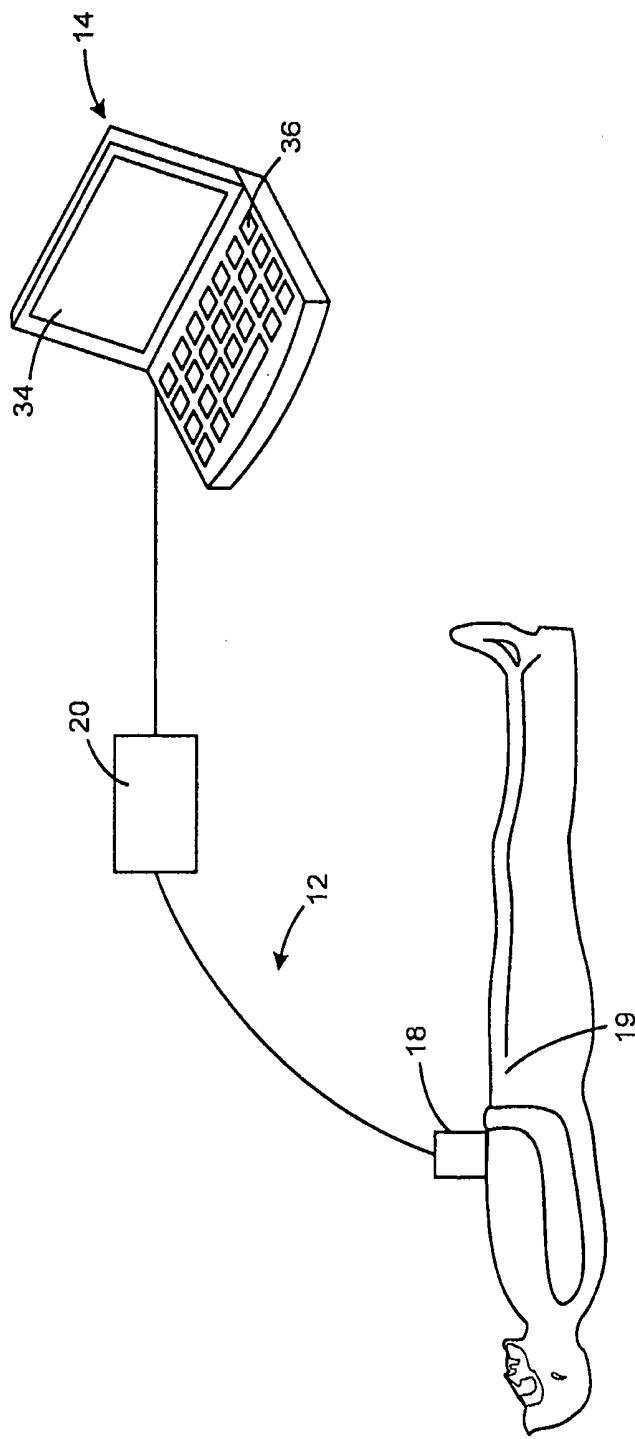


FIG. 6

# ULTRASOUND SYSTEM AND METHOD FOR IMAGING AND/OR MEASURING DISPLACEMENT OF MOVING TISSUE AND FLUID

## FIELD OF INVENTION

[0001] The present invention relates to imaging and treatment systems, and in particular to an improved ultrasound system for imaging and/or measuring the displacement of moving tissue and fluid.

## BACKGROUND OF THE INVENTION

[0002] Ultrasound technology is an efficient and accurate way to examine and measure internal body structures and detect bodily abnormalities. Ultrasound technology works by emitting high frequency sound waves into a region of interest. The sound waves are emitted from a probe, strike the region of interest, and then reflect back to the probe. For example, certain sound waves strike tissues or fluid in the region of interest before other sound waves do and are thus reflected back to the probe sooner than other sound waves. The ultrasound machine measures the difference in time for various ultrasonic waves to be emitted and reflected back to the transducer probe and produces a picture of the region of interest based on those time differences.

[0003] Besides producing an image of the region of interest, ultrasound is capable of determining the velocity of moving tissue and fluids. For example, an ultrasound user can observe a patient's blood as it flows through the heart, determine the speed or flow rate of the blood's movement, and whether the blood is moving towards or away from the heart.

[0004] One method of measuring velocity of moving tissue and fluid is the use of Doppler ultrasound with color mapping. Doppler ultrasound is based upon the Doppler effect. When the object reflecting the sound waves is moving, it changes the frequency of the echoes that are reflected back to the probe. A Doppler ultrasound machine measures the change in frequency of the sound wave echoes and calculates how fast a particular object is moving within the region of interest. Doppler color flow mapping utilizes color to depict the directional movement of tissue and fluid (such as blood) within the region of interest. Color flow mapping produces a two-dimensional image in color with flow towards the probe shown in one color and flow away from the probe shown in another color.

[0005] Another method for measuring the displacement of moving tissue and fluid is power Doppler imaging. Power Doppler imaging is similar to color flow mapping in that it can produce an image that shows the presence or absence of blood flow and the directional movement of the flow. Power Doppler is advantageous because it is up to five times more sensitive in detecting blood flow and other forms of tissue and fluid movement than color mapping. But, power Doppler imaging is not used to determine the velocity of the moving tissue and fluid.

[0006] Ultrasound equipment used for ultrasound imaging and treatment can be divided into three main components. First, there is a peripheral ultrasound system that comprises a probe with a transducer array or a single element for emitting ultrasound waves and equipment that produces and conditions the ultrasound waves for emission from the probe. Second, a host computer system connected to the peripheral ultrasound system serves as to interface with the ultrasound

user. Specifically, the host computer comprises a keyboard or other equipment to help control the ultrasound equipment and a monitor to display the image to the user. Finally, known ultrasound equipment comprises a microprocessor within, or connected to, the host computer.

[0007] The microprocessor is the "brain" of an ultrasound system because it performs all the computing tasks to convert the data collected at the peripheral ultrasound system into the images shown on the monitor to the user. In a Doppler ultrasound system with color flow mapping, the microprocessor will process all the data and generate the velocities of the moving tissues and fluid as well as associated colors to show the directional movement of the tissues and fluid.

[0008] To properly process this data, the microprocessor comprises memory and software. The software utilizes known algorithms to measure the velocity and to chart the color of the tissue and fluid to depict the directional movement of the tissue and fluid.

[0009] Unfortunately, known Doppler ultrasound systems have numerous disadvantages. Microprocessors are not capable of quickly processing the vast information obtained during a Doppler ultrasound. Color flow mapping complicates the problem because producing color images requires a large memory and the processing capabilities that are not appropriate for processing by known microprocessors. Another drawback with Doppler ultrasound systems is despite their accuracy, they are relatively slow in producing images.

[0010] Another problem with known ultrasound equipment is the interface between the peripheral ultrasound equipment and the host computer. Specifically, known ultrasound machines utilize an uncommon type of interface which requires the user to modify his personal computer to use it as a host computer.

## SUMMARY OF THE INVENTION

[0011] A system and method for ultrasound imaging and/or measurement of displacement of tissue and fluid movement is disclosed. An exemplary embodiment of a system for diagnostic imaging and measurement of displacement of living tissue utilizes a dedicated graphics processing unit to process data obtained by a peripheral ultrasound system. Additionally, the system provides a common interface for connecting the peripheral ultrasound system to the host computer.

[0012] In accordance with an exemplary embodiment, the dedicated graphics processing unit comprises a dedicated graphics card with an associated video memory and graphics processor configured to process the data obtained by the peripheral ultrasound system. The graphics card further comprises software that utilizes various algorithms to process the data, examples of which include a Doppler shift algorithm and/or a CFM algorithm and the like.

[0013] In accordance with an exemplary embodiment, the peripheral ultrasound system comprises a transducer probe with a single element or an array to emit ultrasound waves. Further, the peripheral ultrasound system can comprise a beamforming system that focuses the ultrasound beam prior to emission from the transducer probe. In this exemplary embodiment, the beamforming system also conditions the ultrasound energy prior to emission from the probe by incorporating a conditioning circuit. The peripheral ultrasound system can also comprise a processing device such as a demodulator to process ultrasound waves that have been reflected back to the probe into computer readable data.



[0014] In accordance with an exemplary embodiment, the peripheral ultrasound system combines Doppler imaging with B-Flow imaging. This combination increases the speed of image production, yet it does not diminish the quality of images produced by the system.

[0015] In accordance with an exemplary embodiment, a common interface between the host computer and peripheral ultrasound system is provided. The common interface can be any type of interface used on personal computers that enables a personal computer to be connected to the peripheral ultrasound system. In one exemplary embodiment, a plug-and-play style interface is used, such as a Universal Serial Bus (USB) interface.

[0016] In accordance with an exemplary embodiment, ultrasound energy is conditioned within the beamforming device, transmitting from the transducer probe to the region of interest, reflected back to the transducer probe, demodulated by the demodulator into data readable by the host computer, delivered to the host computer through a USB interface as computer readable data, and processed by the dedicated graphics processing unit to determine the velocity of the moving tissue and fluid.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0017] The subject matter of the invention is particularly pointed out in the concluding portion of the specification. The invention, however, both as to organization and method of operation, may be best understood by reference to the following description taken in conjunction with the accompanying drawing figures, in which like parts may be referred to by like numerals.

[0018] FIG. 1 illustrates a block diagram of an ultrasound system in accordance with an exemplary embodiment of the present invention;

[0019] FIG. 2 illustrates a block diagram of the peripheral ultrasound system, the host computer, and the graphics processing unit in accordance with an exemplary embodiment of the present invention;

[0020] FIG. 3 illustrates a block diagram of the peripheral ultrasound system in accordance with an exemplary embodiment of the present invention;

[0021] FIG. 4 illustrates a block diagram of the host computer in accordance with an exemplary embodiment of the present invention;

[0022] FIG. 5 illustrates a block diagram of the graphics processing unit in accordance with an exemplary embodiment of the present invention; and

[0023] FIG. 6 illustrates the ultrasound system in use in an exemplary embodiment of the present invention.

#### DETAILED DESCRIPTION

[0024] The present invention may be described herein in terms of various functional components and processing steps. It should be appreciated that such components and steps may be realized by any number of hardware components configured to perform the specified functions. For example, the present invention may employ various visual imaging and display devices used for medical treatment which may carry out a variety of functions under the control of one or more control systems or other control devices. In addition, the present invention may be practiced in any number of imaging and medical contexts and that the exemplary embodiments relating to an ultrasound system and method as described

herein are merely indicative of exemplary applications for the invention. For example, the principles, features and methods discussed may be applied to any imaging or medical application. Further, various aspects of the present invention may be suitably applied to other applications that utilize imaging technology.

[0025] An exemplary system for ultrasonic imaging and/or measurement of displacement of moving tissue and fluid denoted throughout as system 10 is provided. The system of the present invention can be used in traditional gray-scale ultrasound imaging or for color-mapping imaging. In an exemplary embodiment, system 10 is an ultrasound treatment system and comprises a peripheral ultrasound system 12 for emitting and receiving energy that is connected to and in operative communication with a host computer 14. System 10 further comprises a graphics processing unit 16 that is dedicated to process data obtained by peripheral ultrasound system 12.

[0026] With reference to FIG. 3, peripheral ultrasound system 12 comprises a probe 18 that transmits and receives energy. While a peripheral ultrasound system is specifically mentioned herein, any peripheral system that emits energy can be used and fall within the scope of the present invention. An exemplary energy transmitted and received by probe 18 is ultrasound energy which can be either focused or unfocused. Additionally, an exemplary probe 18 is a transducer probe that contacts a region of interest 19 on a patient or other subject that the user wishes to scan. Peripheral ultrasound system 12 also comprises beamforming device 20 for focusing the ultrasound energy before it is emitted from probe 18.

[0027] Examples of exemplary ultrasound systems are disclosed in U.S. Pat. No. 6,440,071 entitled "Peripheral Ultrasound Imaging System", U.S. patent application assigned Ser. No. 10/944,499 entitled "Method and System For Ultrasound Treatment With A Multi-Directional Transducer", U.S. application assigned Ser. No. 10/944,500 entitled "System and Method For Variable Depth Ultrasound Treatment", and U.S. application assigned Ser. No. 11/163,148 entitled "Method and System For Controlled Thermal Injury of Human Superficial Tissue." All four of these patents and patent applications are hereby incorporated by reference.

[0028] In an exemplary embodiment, a conditioning circuit 22 or other similar conditioning device and a demodulator 24 are part of beamforming device 20. Demodulator 24 demodulates ultrasound energy received by probe 18 into data that is readable by host computer 14 and processed by graphics processing unit 16. Therefore, the ultrasound energy's conditioning and demodulation occurs within beamforming device 20.

[0029] An exemplary probe 18 can be configured in various manners and comprise a number of reusable or disposable components and parts in various embodiments to facilitate its operation. For example, probe 18 can be configured within any type of probe housing or arrangement for facilitating the contact of probe 18 to the patient's skin at region of interest 19, with such housing comprising various shapes, contours and configurations. Probe 18 may also comprise cables and connectors; motion mechanisms, motion sensors and encoders; thermal monitoring sensors; or user control and status related switches, and indicators such as LEDs.

[0030] In an exemplary embodiment, probe 18 includes a single transduction element mounted within probe 18. The transduction element can comprise a piezoelectrically active material, such as lead zirconate titanate (PZT), or any other

piezoelectrically active material, such as a piezoelectric ceramic, crystal, plastic, or composite materials, as well as lithium niobate, lead titanate, barium titanate, or lead metaniobate. In addition to, or instead of, a piezoelectrically active material, probe 18 can comprise other materials configured for generating radiation or acoustical energy. In other exemplary embodiments, probe 18 includes a transducer array.

[0031] Lenses can also be used in the emission of ultrasound waves from probe 18. Lenses or other transduction elements can be configured to be concave, convex, or planar. For example, in one exemplary embodiment, the transduction element is configured to be concave in order to provide focused energy for treatment of region of interest 19. Additional embodiments are disclosed in U.S. patent application Ser. No. 10/944,500, entitled “Variable Depth Transducer System and Method”, which is herein incorporated by reference.

[0032] An exemplary peripheral ultrasound system 12 is depicted in FIG. 3 and shows probe 18 as a separate element from beamforming device 20 and its related components. While probe 18 can be a separate element as shown, it should be noted that beamforming device 20 and its related components can be placed within probe 18 in other exemplary embodiments. Moreover, any type of transducer probe or similar device can be used and fall within the scope of the present invention.

[0033] Peripheral ultrasound system 12 is connected to host computer 14 by an interface 28 that is described in more detail below and depicted in. Host computer 14 enables the user of system 10 to view images obtained at region of interest 19, provide estimations of moving tissue and fluid displacement within region of interest 19, and to control and adjust system 10. Host computer 14 can be any type of computer system suitable for imaging applications. Exemplary computers include personal computers and laptop computers.

[0034] With additional reference to FIG. 2, host computer 14 comprises a central processing unit (CPU) 30 and a memory 32. While any type memory 32 can be used, an exemplary memory is a cine memory. Host computer 14 further comprises at least one output device 34 to provide the user of system 10 with an image of region of interest 19. In addition to displaying an image to the user, output device 34 enables the user to view the directional movement or obtain the velocity of the moving tissue and fluid such as blood within region of interest 19. An exemplary output device 34 is a color computer monitor that is capable of visually displaying a color flow map of region of interest 19 as described below. Further, in certain exemplary embodiments, multiple output devices 34 can be attached to CPU 30.

[0035] As shown in FIG. 4, host computer 14 further comprises control devices to enable the user to control system 10. Exemplary control devices include a keyboard 36 and a computer mouse. Other exemplary control devices include joysticks and other similar control devices and systems.

[0036] As noted above, host computer 14 is connected to peripheral ultrasound system 12 by interface 28. While any type of wired or wireless interface 28 can be used, a plug-and-play interface 28 is used in an exemplary embodiment. A plug-and-play interface 28 enables the user to quickly connect and disconnect peripheral ultrasound system 12 to host computer 14. An exemplary plug-and-play interface 28 is known as a “hot-plug capable” interface 28 in that it can enable the user of system 10 to plug peripheral ultrasound system 12 into host computer 14 without having to shut down and reboot host computer 14. These types of interfaces 28

include a Universal Serial Bus (USB) interface 28. Exemplary USB interfaces include an A type and B type USB interface.

[0037] Unlike traditional ultrasound systems that rely on a microprocessor to process the data obtained by peripheral ultrasound system 12, system 10 utilizes a dedicated graphics processing unit 16 to process the data. This enables system 10 to have a dedicated processing device for processing the large amount of data collected at peripheral ultrasound system 12 and more efficiently displaying an image on output device 34 than a microprocessor. In an exemplary embodiment, graphics processing unit 16 is dedicated solely to the function of processing data obtained by peripheral ultrasound system 12. It should be noted that while the term “graphics processing unit” can comprise any dedicated processing device or combinations of devices that process data. An exemplary dedicated processing device is depicted in FIG. 5.

[0038] In one exemplary embodiment, graphics processing unit 16 comprises graphics card 38. In another exemplary embodiment, graphics processing unit 16 comprises a physics processing unit (PPU).

[0039] In another exemplary embodiment, graphics processing unit 16 could be a combination of a graphics card 38 and a PPU. A PPU performs nearly identical functions as graphics processing unit 16 except that a PPU is capable of processing physics code and removing the load that calculating physics puts on the graphics processing unit 16 and allocate it to the PPU. Therefore, in an exemplary embodiment, graphics processing unit 16 would comprise two devices, one being the graphics card 38 and the other a PPU. Graphics card 38 in combination with the PPU increases the efficiency and accuracy of system 10.

[0040] Other exemplary processing devices include systems that are dedicated to process the graphics data obtained by ultrasound system 12. For example, a system of a card and processor chip could be an exemplary graphics processing unit 16. Alternatively, any other dedicated chip, processor, or combination thereof can be utilized as graphics processing unit 16.

[0041] In accordance with an exemplary embodiment, graphics processing unit 16 can comprise a graphics card 38 with a processor 40 and a memory 42. For example, exemplary graphics cards 38 can comprise those produced by the NVIDIA Corporation of Santa Clara, Calif. and/or ATI Technologies, Inc. of Ontario, Canada. In an exemplary embodiment, multiple graphics cards 38 can be used to process data. In one embodiment, the image is split into two portions and a single graphics card 38 is used to process each portion.

[0042] In an exemplary embodiment, graphics processing unit 16 processes the data obtained by peripheral ultrasound system 12 by utilizing software with algorithms that are programmed within memory 42. One exemplary algorithm is the Doppler shift algorithm; however, various other algorithms can also be used.

[0043] System 10 can utilize certain imaging techniques in addition to or instead of Doppler imaging. Certain exemplary techniques include various decorrelation of frames techniques. One exemplary technique is B-flow imaging. B-flow imaging can be used by itself by system 10 or it can be combined with other techniques such as Doppler imaging. In an exemplary embodiment, system 10 combines various Doppler techniques with B-flow techniques to increase the speed and accuracy of images produced by system 10. One

advantage of this increase in speed and accuracy is the ability to use a single transduction element within probe 18.

[0044] Turning now to FIG. 6, system 10 is used to obtain images of region of interest 19. In exemplary embodiments, ultrasound images can be obtained and an estimation of displacement of moving tissue including fluid is obtained by use of system 10.

[0045] When system 10 is used for Doppler color flow mapping, the user can determine the velocity of the moving tissue and fluid as well as obtain an image of region of interest 19. Specifically, graphics processing unit 16 processes the data obtained by peripheral ultrasound system 12 and produces an image displayed on output device 34 that includes the speed of the moving tissue and fluid. In certain exemplary embodiments, the image is shown in traditional gray-scale imaging.

[0046] In other exemplary embodiments, ultrasound system 12 produces a color map to show the direction of fluid and tissue movement. The directional movement either towards or away from probe is shown on output device 34 in contrasting colors. In an exemplary embodiment, tissue and fluid moving towards the probe could be shown in shades of blue and tissue and fluid moving away from probe 18 could be shown in shades of red.

[0047] If system 10 is used to generate an image and obtain and estimation of tissue displacement using power Doppler imaging an image detailing the presence or absence of blood flow is displayed on output device 34. By viewing that image, the user can determine the directional movement of the blood flow or other moving tissue using the power Doppler imaging technique. In an exemplary embodiment, B-Flow imaging is combined with power Doppler imaging to increase speed and efficiency.

[0048] An exemplary process of obtaining an image and measuring displacement of tissue movement begins with a user connecting peripheral ultrasound system 12 to host computer 14 with interface 28. In an exemplary embodiment, the user simply plugs one end of a USB connector provided on peripheral ultrasound system 12 into the corresponding USB connector located on host computer 14.

[0049] Probe 18 is placed on the patient's skin and the transduction element produces ultrasound energy which is conditioned by conditioning circuit 22 and focused by beamforming device 20 before being emitted from probe 18. The ultrasound energy waves enter region of interest 19 and are reflected and echoed back to probe 18. These reflected ultrasound waves are demodulated into computer readable data by demodulator 24 and sent to host computer 14 via interface 28.

[0050] Once the computer data has arrived at host computer 14, it is processed by graphics processing unit 16. Specifically, graphics processing unit 16 uses an algorithm to generate an image and measure displacement of the tissue or fluid movement, e.g., by producing a color flow map or gray-scale image and/or implementing a power Doppler technique. The image is displayed on output device 34 for the user's viewing. If multiple output devices 34 are used, the image is displayed on all of them. The user can then view the image and obtain an estimate of the moving tissue's displacement.

[0051] The present invention may be described herein in terms of various functional components and processing steps. It should be appreciated that such components and steps may be realized by any number of hardware components configured to perform the specified functions. For example, the present invention may employ various medical treatment

devices, visual imaging and display devices, input terminals and the like, which may carry out a variety of functions under the control of one or more control systems or other control devices. In addition, the present invention may be practiced in any number of medical contexts and that the exemplary embodiments relating to a system as described herein are merely indicative of exemplary applications for the invention. For example, the principles, features and methods discussed may be applied to any medical application. Further, various aspects of the present invention may be suitably applied to other applications, such as other medical or industrial applications.

1. A system for diagnostic imaging and estimation of displacement of moving tissue and fluid comprising:

a probe that transmits and receives energy; and  
a dedicated graphics processing unit comprising a memory and configured with algorithms to estimate tissue and fluid movement from energy received by the probe.

2. The system according to claim 1, further comprising a demodulator for processing energy received by the probe.

3. The system according to claim 1 further comprising a beamforming device for focusing and conditioning the energy emitted from the probe.

4. The system according to claim 3 wherein the beamforming device further comprises a conditioning circuit.

5. The system according to claim 3 further comprising a host computer connected to the beamforming device and in communication with the dedicated graphics processing unit for displaying an image and displacement of moving tissue to a user.

6. The system according to claim 5 wherein the host computer is connected to the beamforming device by a plug-and-play interface.

7. The system according to claim 6 wherein the plug-and-play interface is a USB.

8. The system according to claim 1 wherein the probe comprises a single element to deliver energy to a region of interest.

9. The system according to claim 1 wherein the dedicated graphics processing unit comprises a physics processing unit.

10. The system according to claim 1 wherein the dedicated graphics processing unit is a graphics card.

11. A system for diagnostic imaging and estimation of displacement of moving tissue and fluid comprising:

a peripheral ultrasound system for obtaining data from a region of interest comprising,

a probe that transmits and receives ultrasound energy,  
a demodulator processing the ultrasound energy received by the probe,

a beamforming device for focusing and conditioning the ultrasound energy before it is emitted from the probe;

a graphics processing unit for processing the data obtained at the region of interest comprising a memory, a processor, and software configured with algorithms to estimate tissue displacement; and

a host computer in operative communication with the peripheral ultrasound system and the graphics processing unit for providing data processed by the graphics processing unit to the user and enabling the user to control the system.

12. The system according to claim 11 further comprising a plug-and-play interface to connect the host computer to the peripheral ultrasound system.

**13.** The system according to claim **12** wherein the plug-and-play interface is a USB.

**14.** The system according to claim **11** wherein the graphics processing unit utilizes an algorithm to determine a directional movement of tissue.

**15.** The system according to claim **11** wherein the graphics processing unit utilizes an algorithm to determine velocity of tissue displacement.

**16.** The system according to claim **11** wherein the graphics processing unit utilizes a Doppler shift algorithm to estimate tissue displacement.

**17.** The system according to claim **11** wherein the system utilizes a B-flow imaging technique to estimate tissue displacement.

**18.** The system according to claim **11** wherein the system combines a B-flow imaging technique with a Doppler shift algorithm to estimate tissue displacement.

**19.** The system according to claim **11** wherein the host computer further comprises at least two output devices to relay information about the region of interest to a user.

**20.** The system according to claim **19** wherein the at least two output devices are monitors that display an image.

**21-39.** (canceled)

\* \* \* \* \*

专利名称(译)	用于成像和/或测量移动组织和流体的位移的超声系统和方法		
公开(公告)号	<a href="#">US20160262728A1</a>	公开(公告)日	2016-09-15
申请号	US14/966377	申请日	2015-12-11
[标]申请(专利权)人(译)	ARDENT SOUND		
申请(专利权)人(译)	ARDENT SOUND INC.		
当前申请(专利权)人(译)	ARDENT SOUND INC.		
[标]发明人	BARTHE PETER G SLAYTON MICHAEL H JAEGER PAUL		
发明人	BARTHE, PETER G. SLAYTON, MICHAEL H. JAEGER, PAUL		
IPC分类号	A61B8/08 A61B8/06 A61B8/14 A61B8/00		
CPC分类号	A61B8/5207 A61B8/461 A61B8/4411 A61B8/4483 A61B8/06 A61B8/14 A61B8/488 A61B8/08 A61B8/13		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

系统和改进的成像方法被披露。示例性系统提供了连接到一个主计算机带有一个插头和播放接口的外围超声波系统例如USB。示例性系统利用专用的图形处理单元，例如图形卡，以分析来自感兴趣区域获得的一个或多个输出单元为用户的观看产生的图像数据。基于所述输出单元显示的图像上，用户可以决定移动组织和流体的速度。本发明的系统可用于产生多普勒彩色流映射或用于功率多普勒成像。

