



US 20070167811A1

(19) **United States**(12) **Patent Application Publication****Lemmerhirt et al.**(10) **Pub. No.: US 2007/0167811 A1**(43) **Pub. Date:****Jul. 19, 2007**(54) **CAPACITIVE MICROMACHINED
ULTRASONIC TRANSDUCER****Publication Classification**(76) Inventors: **David F. Lemmerhirt**, Ann Arbor, MI
(US); **Collin A. Rich**, Ypsilanti, MI
(US)(51) **Int. Cl.****A61B 8/14** (2006.01)(52) **U.S. Cl.** **600/459**


(57)

ABSTRACT

Correspondence Address:

SCHOX PLC**209 N. MAIN STREET #200****ANN ARBOR, MI 48104 (US)**(21) Appl. No.: **11/612,656**(22) Filed: **Dec. 19, 2006****Related U.S. Application Data**(63) Continuation-in-part of application No. 11/229,197,
filed on Sep. 15, 2005.(60) Provisional application No. 60/610,320, filed on Sep.
15, 2004. Provisional application No. 60/610,319,
filed on Sep. 15, 2004. Provisional application No.
60/610,337, filed on Sep. 15, 2004.

The first integrated circuit/transducer device **36** of the hand-held probe includes CMOS circuits **110** and cMUT elements **112**. The cMUT elements **112** function to generate an ultrasonic beam, detect an ultrasonic echo, and output electrical signals, while the CMOS circuits **110** function to perform analog or digital operations on the electrical signals generated through operation of the cMUT elements **112**. The manufacturing method for the first integrated circuit/transducer device **36** of the preferred embodiment includes the steps of depositing the lower electrode **S102**; depositing a sacrificial layer **S104**; depositing a dielectric layer **S106**; depositing the upper electrode **S108**; depositing a protective layer on the upper electrode **S110**; and removing the sacrificial layer **S112**. In the preferred embodiment, the manufacturing method also includes the step of depositing a sealant layer to seal a cavity between the lower electrode and the upper electrode **S114**.

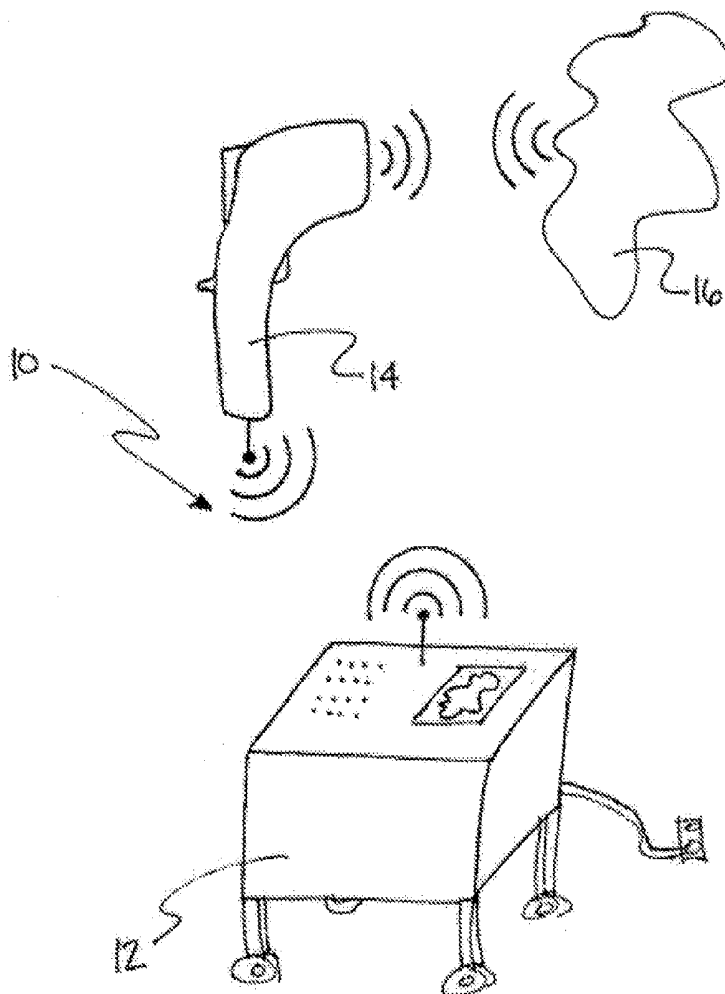

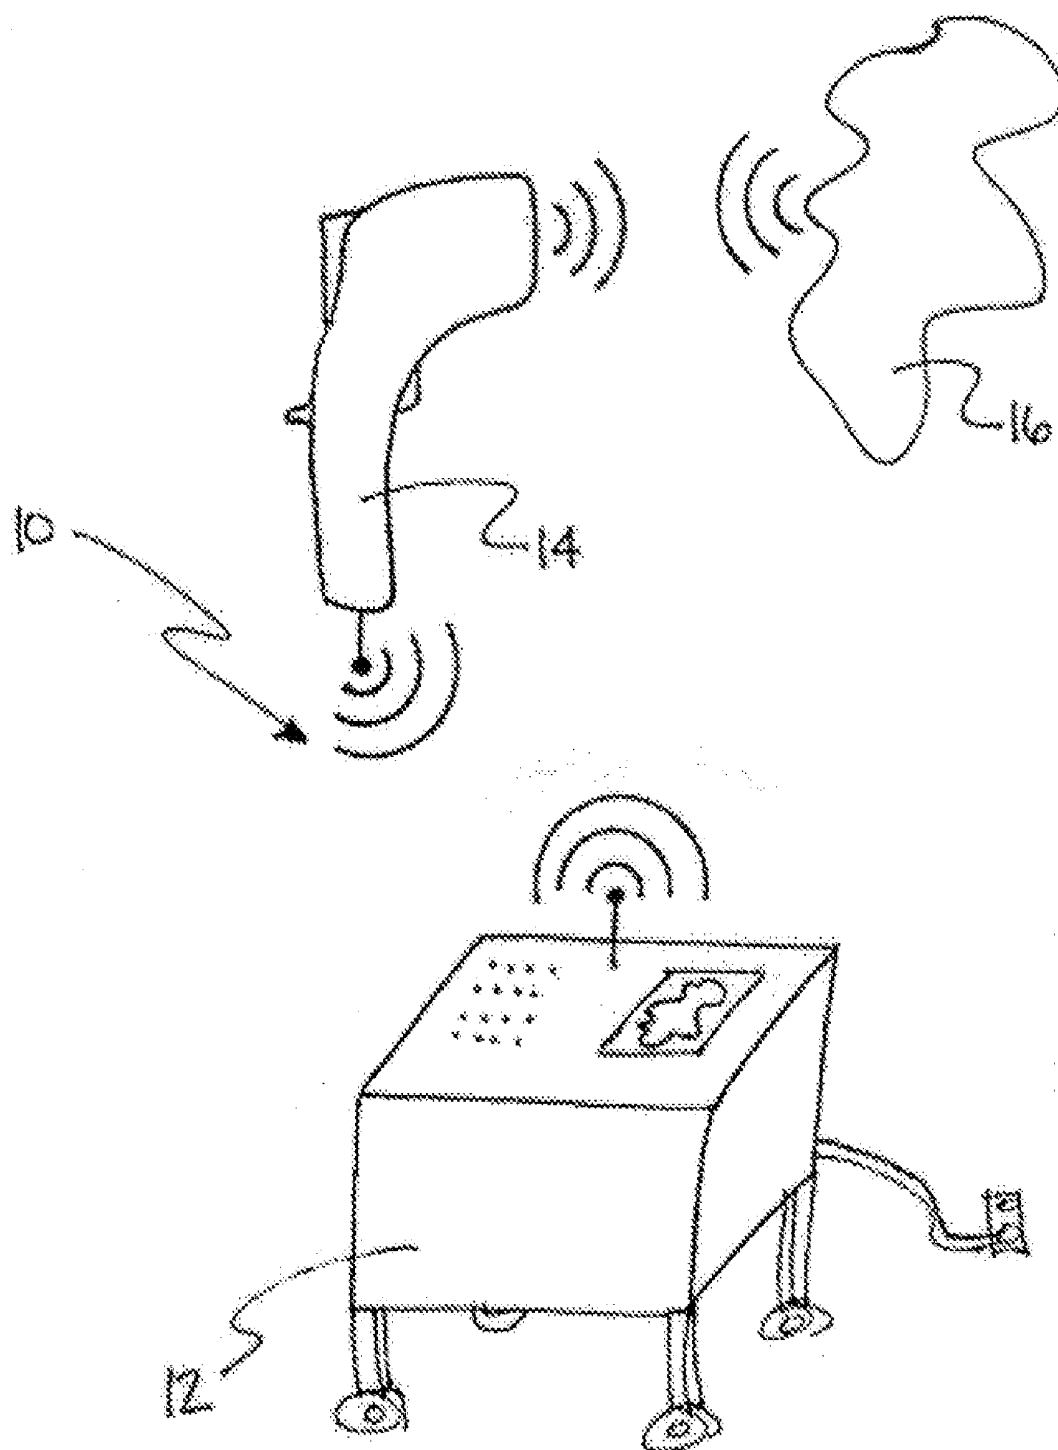


FIGURE 1

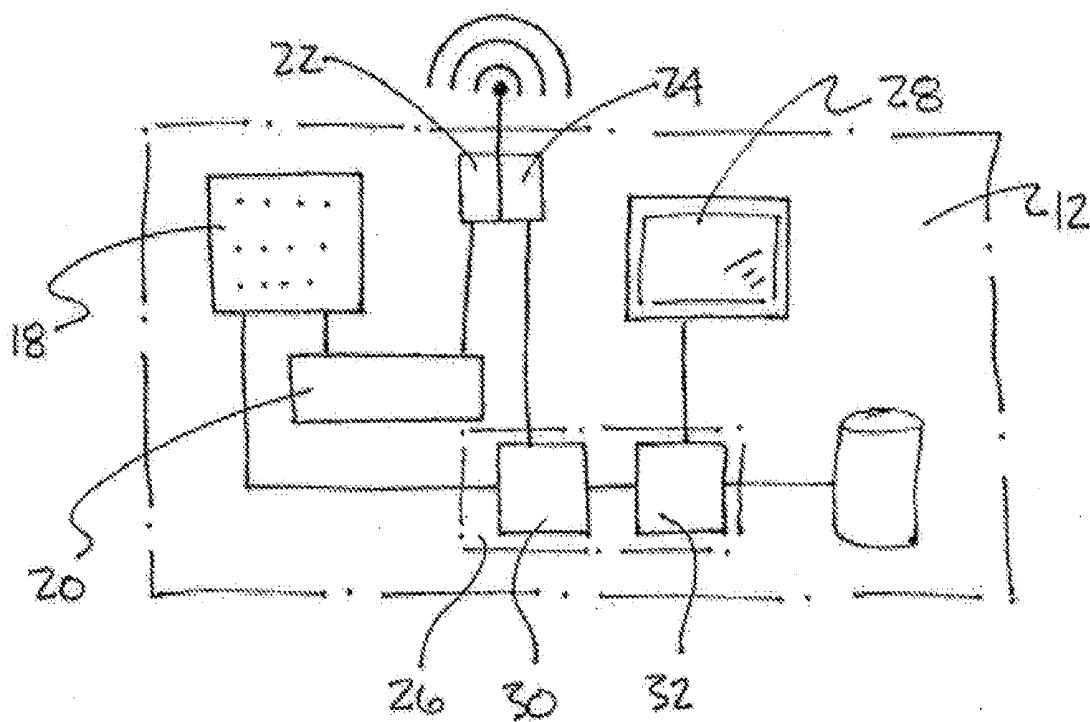


FIGURE 2

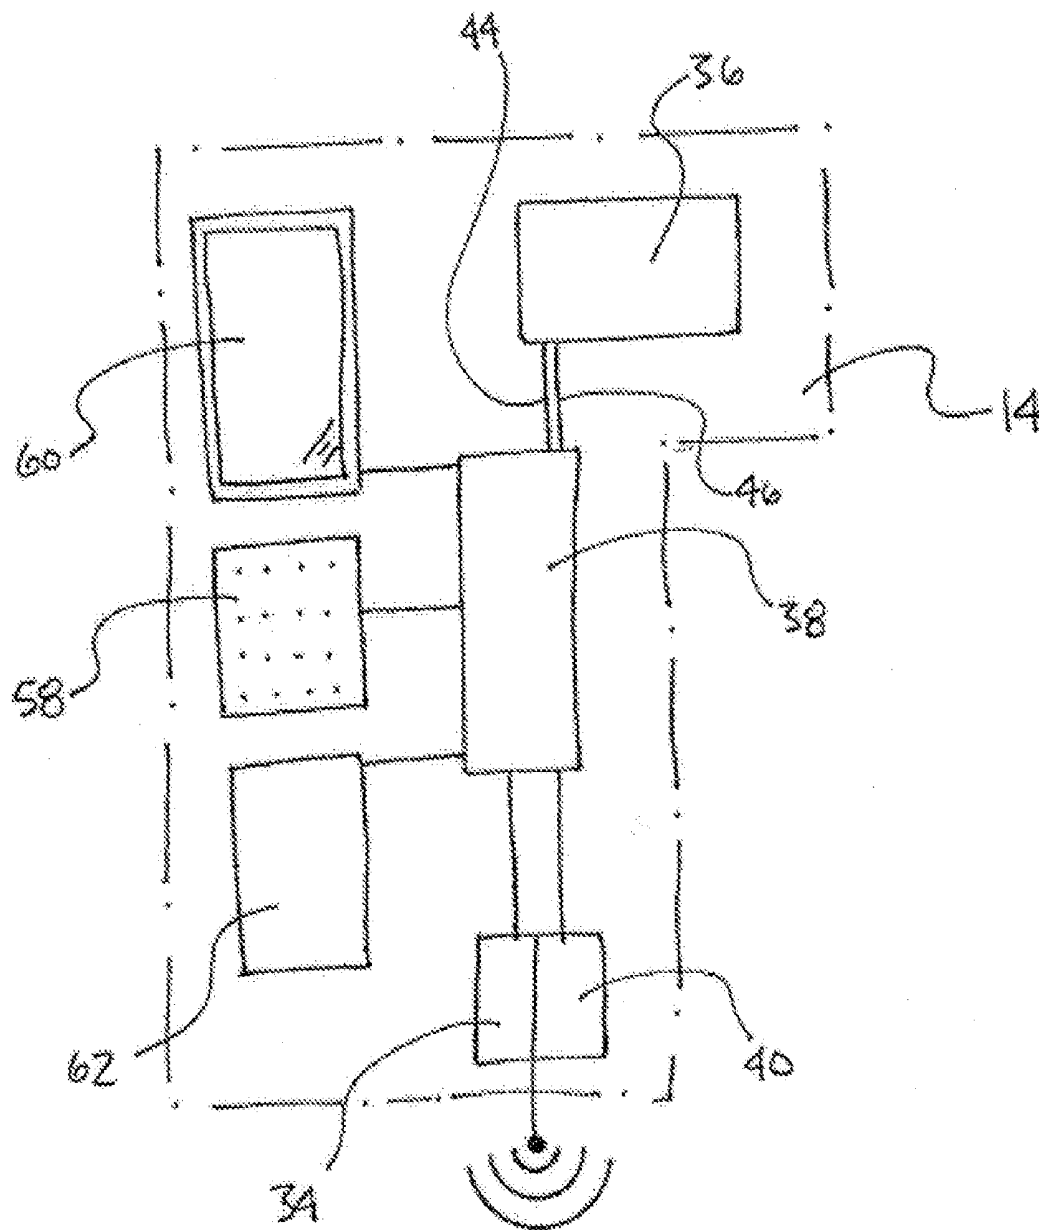


FIGURE 3

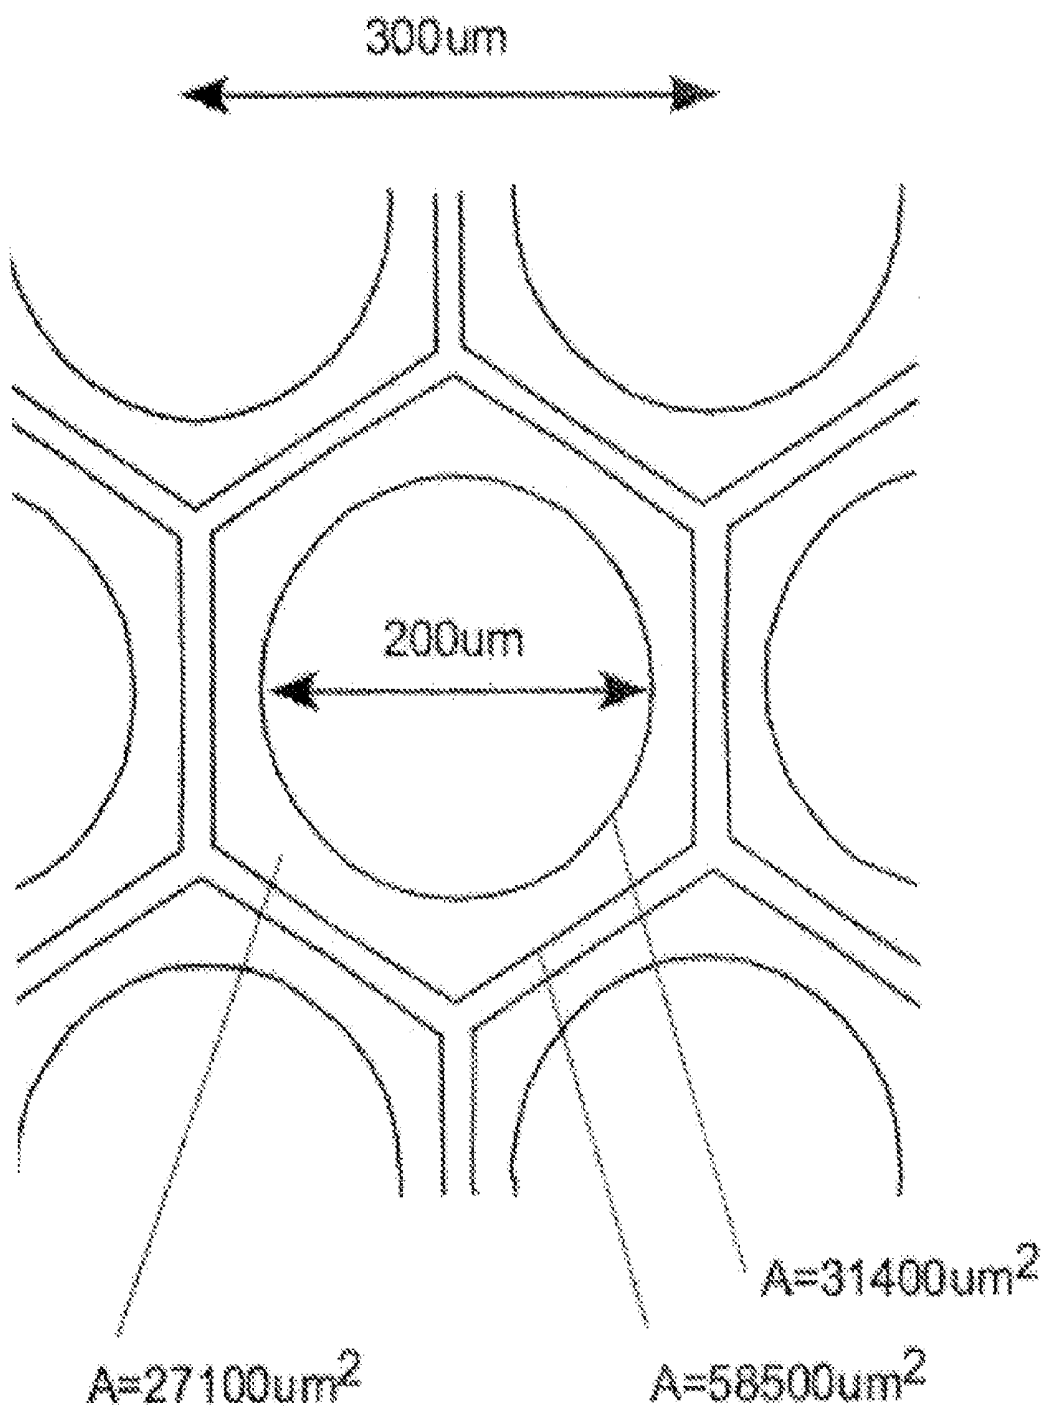


FIGURE 5

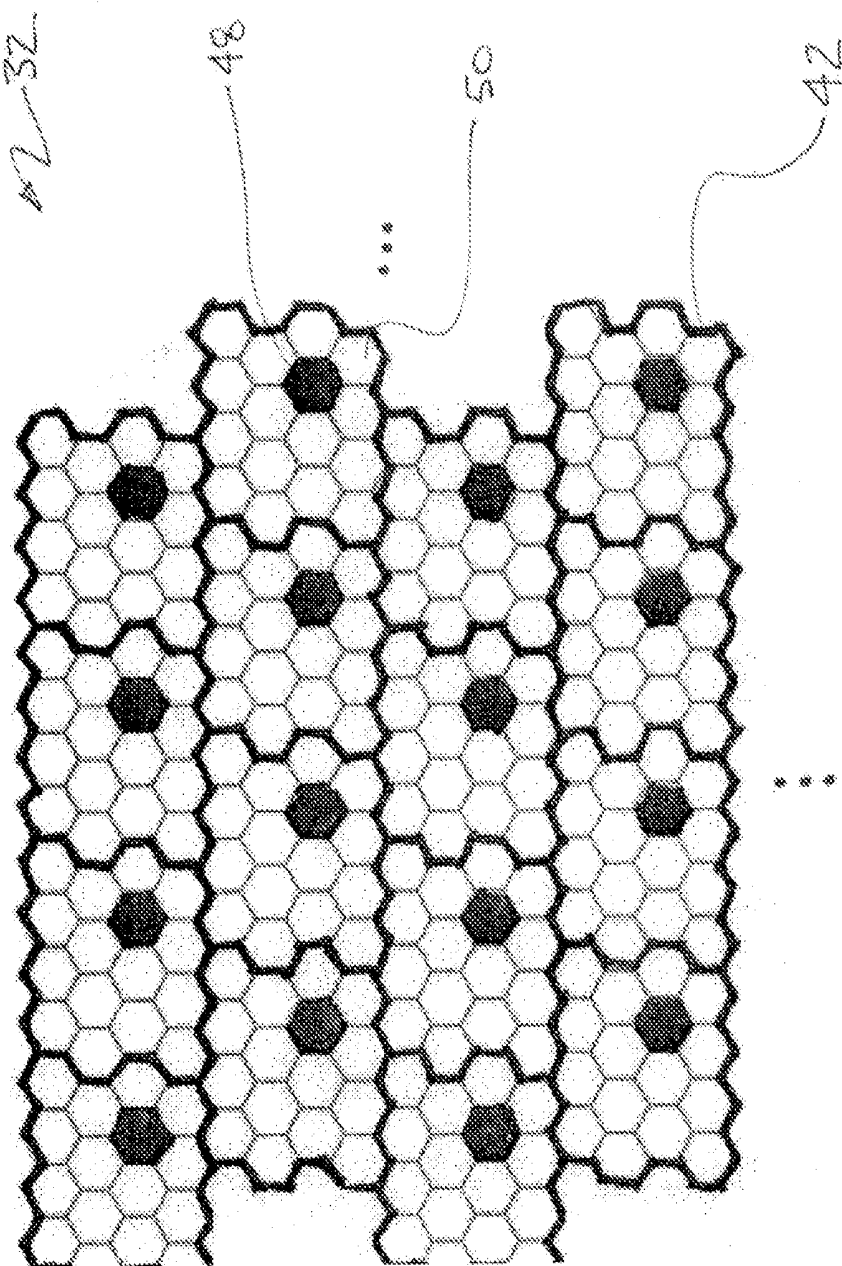


FIGURE 6

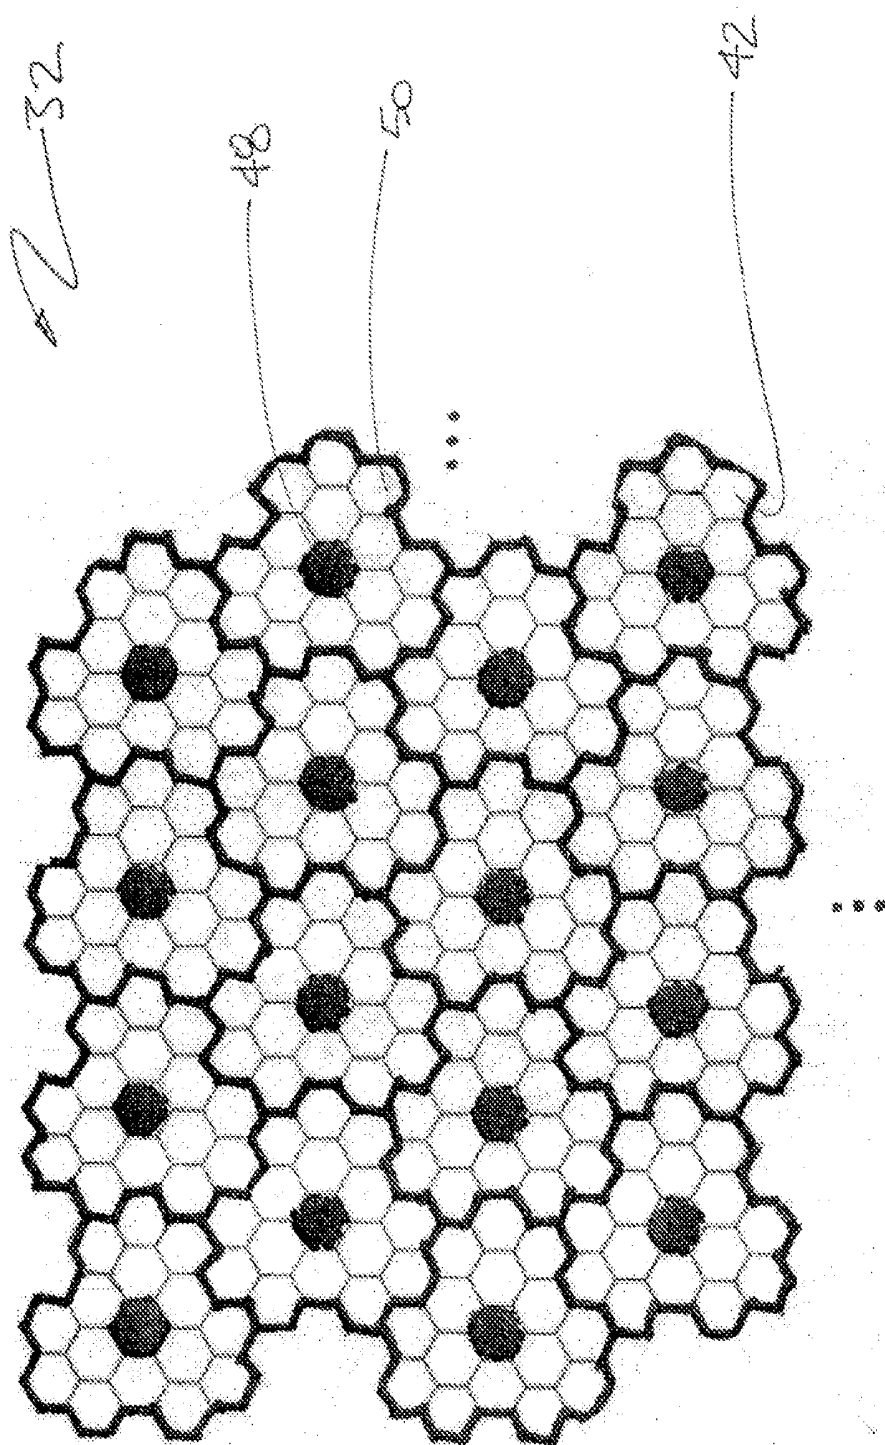


FIGURE 7

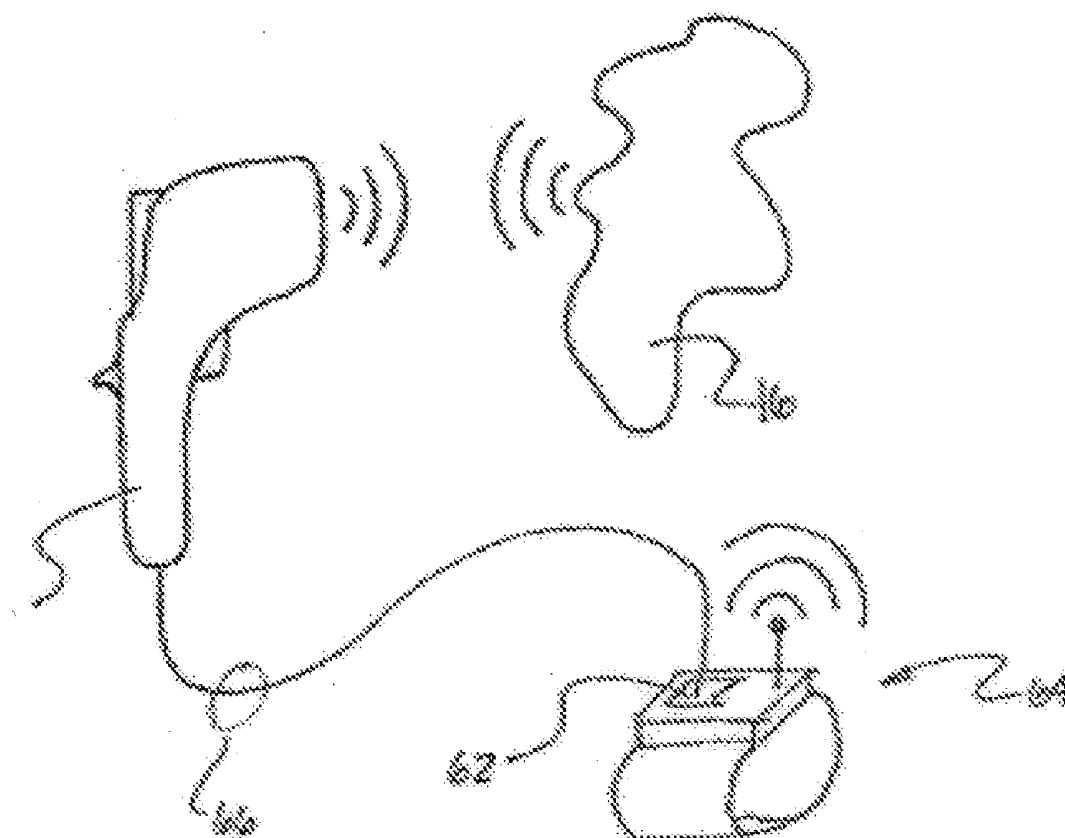


FIGURE 8

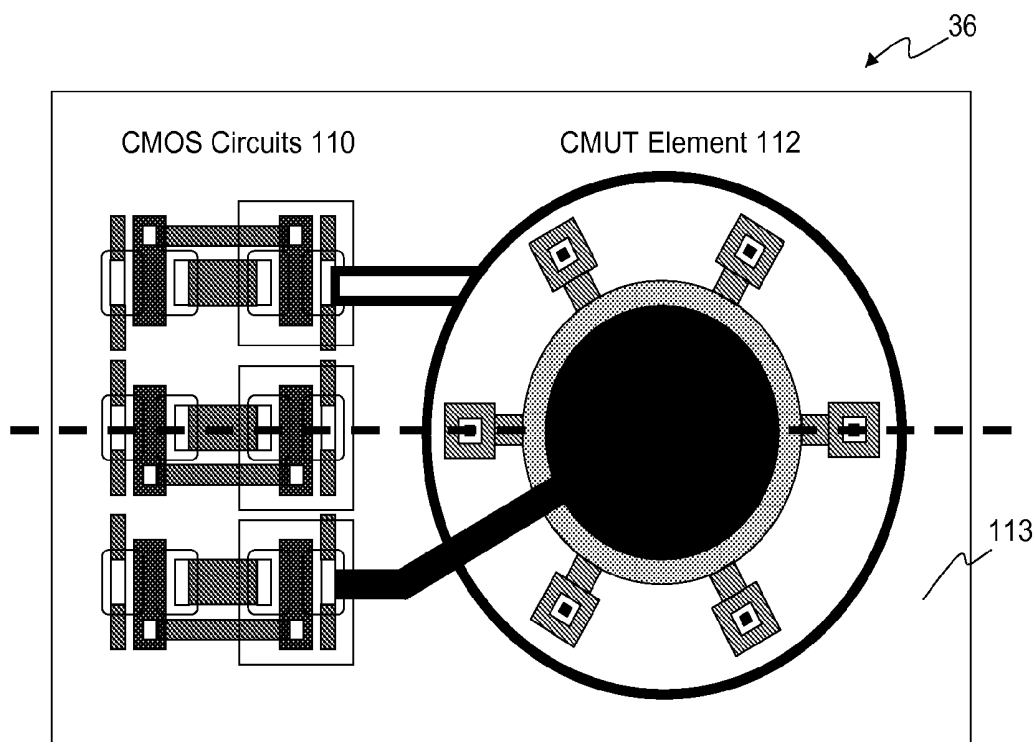


Figure 9

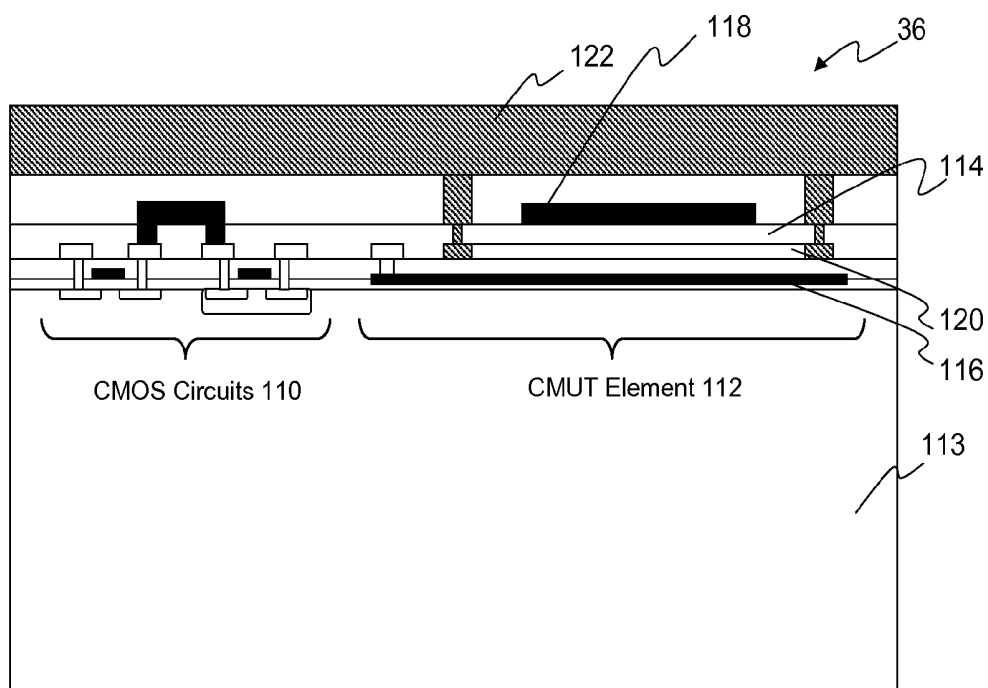


Figure 10

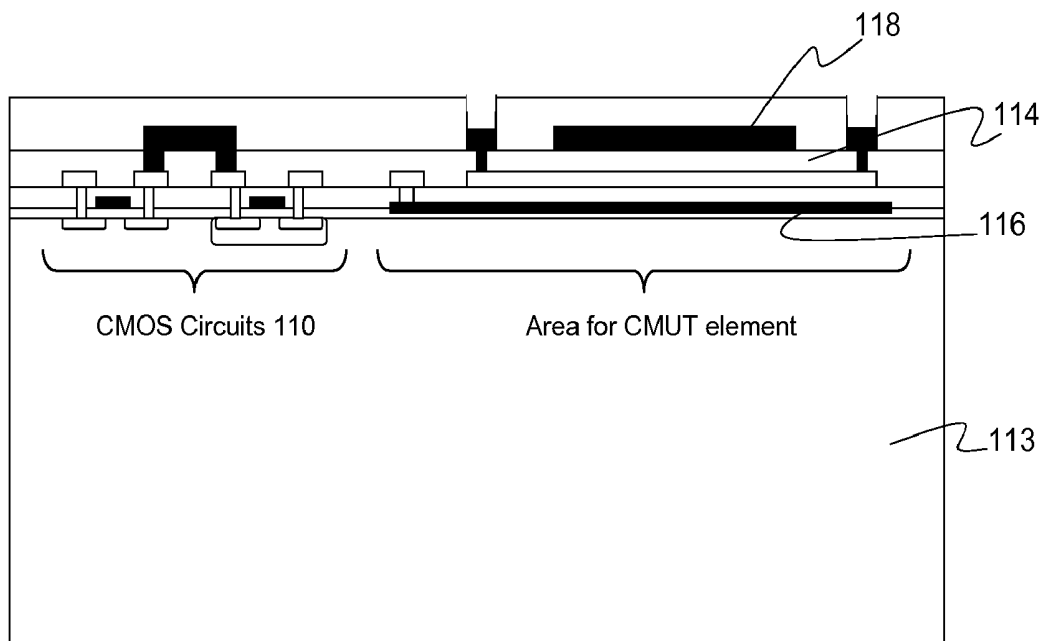


Figure 11

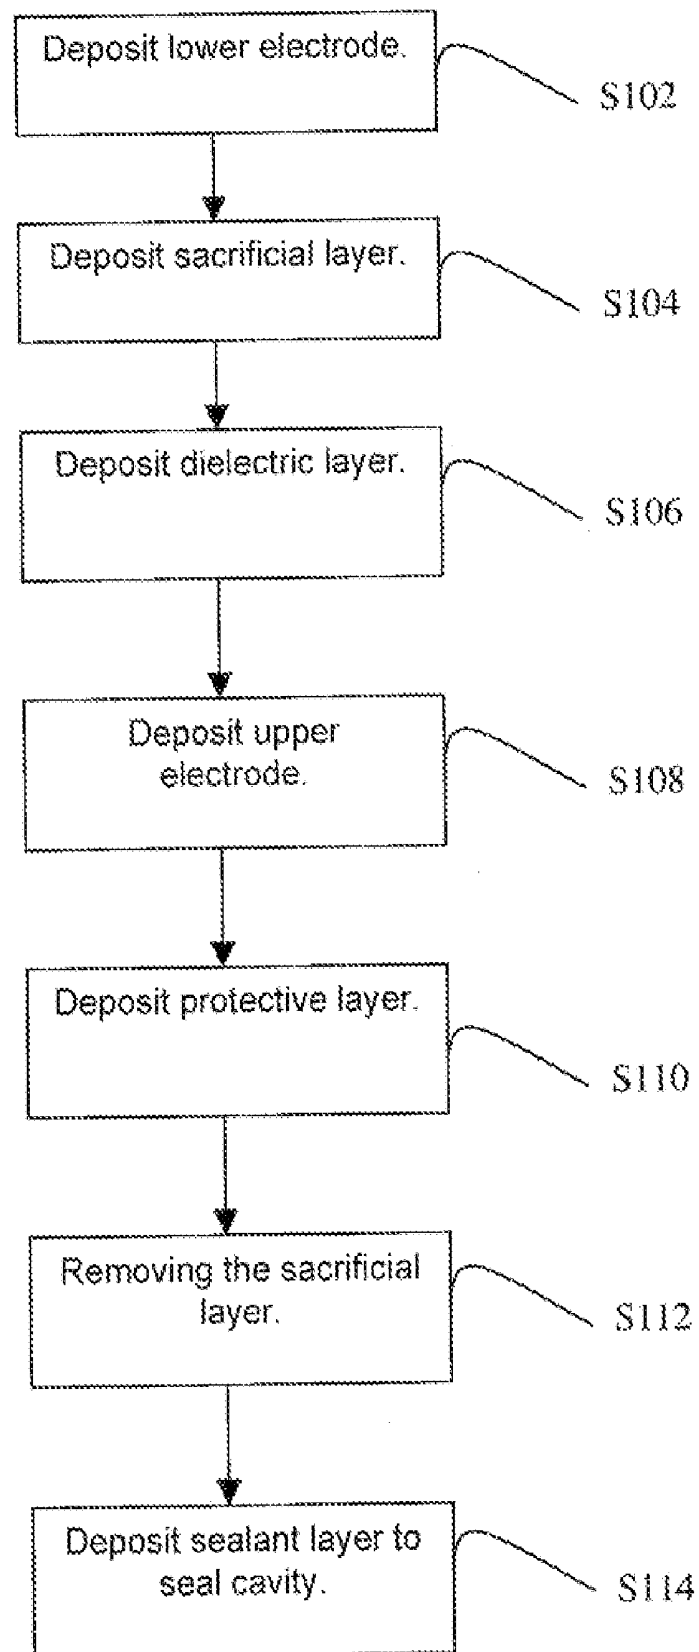


FIGURE 12

CAPACITIVE MICROMACHINED ULTRASONIC TRANSDUCER

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present invention claims priority as a continuation-in-part of U.S. Serial Number 11,229,197 filed on 15 Nov. 2005 and titled "Integrated Circuit for an Ultrasound System", which claims priority to the following three provisional applications: U.S. Provisional Patent Application No. 60/610,320 filed 15 Sep. 2004 and titled "Beamforming", U.S. Provisional Patent Application No. 60/610,319 filed 15 Sep. 2004 and titled "Transducer", and U.S. Provisional Patent Application No. 60/610,337 filed 15 Sep. 2004 and titled "Electronics". Each of the four applications (the one application and the three provisional applications) are incorporated in their entirety by this reference.

[0002] The present invention is related to U.S. Ser. No. _____, filed on the same date with the same title as this invention, which is incorporated in its entirety by this reference.

TECHNICAL FIELD

[0003] The present invention relates generally to the field of semiconductor design and manufacture, and more particularly to the field of capacitive micromachined ultrasonic transducers.

BACKGROUND

[0004] Historically, transducer elements of ultrasonic imaging devices have employed piezoelectric transducers to receive and transmit acoustic signals at ultrasonic frequencies. The performance of piezoelectric transducers is limited by their narrow bandwidth and acoustic impedance mismatch to air, water, and tissue. In an attempt to overcome these limitations, current research and development has focused on the production of capacitive micromachined ultrasonic transducer (cMUT) elements. cMUT elements generally include at least a pair of electrodes separated by a uniform air or vacuum gap, with the upper electrode suspended on a flexible membrane. Impinging acoustic signals cause the membrane to deflect, resulting in capacitive changes between the electrodes, which produce electronic signals usable for ultrasonic imaging.

[0005] The nature of the signals produced by cMUT elements demands that they are located as close as possible to the electronic readout circuits, ideally on the same physical substrate. While there have been efforts to make cMUT elements compatible with complementary metal-oxide (CMOS) integrated circuits, the conventional approaches have relied on depositing and patterning layers to form cMUT structures after the CMOS process steps are complete. These approaches raise substantial financial and technical barriers due to the high cost of adding patterned layers to a finely-tuned CMOS process and due to the high process temperatures needed to deposit the high quality structural layers needed for micromachined devices. The production of a cMUT element using this approach may require temperatures higher than 500 degrees Celsius, at which point the metallization layers within the CMOS circuit elements may begin to form hillocks or to alloy with adjacent layers. These phenomena may render the integrated circuit non-functional

or, at best, will severely reduce production yield. In short, the existing approaches have failed to viably integrate the ultrasonic functions of a cMUT into an integrated circuit.

[0006] Thus, there is a need in the art of ultrasonic imaging devices for a new and improved capacitive micromachined ultrasonic transducer. This invention provides a design and manufacturing method for such transducer device.

BRIEF DESCRIPTION OF THE FIGURES

[0007] FIG. 1 is a representation of an ultrasound system of the preferred embodiment.

[0008] FIG. 2 is a schematic representation of the central console of the ultrasound system.

[0009] FIG. 3 is a schematic representation of a handheld probe for the ultrasound system.

[0010] FIG. 4 is a schematic representation of a first example of an integrated circuit for the handheld probe.

[0011] FIG. 5 is a representation of the relative size and proportion of the elements of the integrated circuit.

[0012] FIGS. 6 and 7 are schematic representations of two variations of a second example of an integrated circuit for the handheld probe.

[0013] FIG. 8 is a representation of an alternative handheld probe for the ultrasound system.

[0014] FIGS. 9 and 10 are top and side views, respectively, of the first integrated circuit/transducer device of the preferred embodiment.

[0015] FIG. 11 is a side view of the first integrated circuit/transducer device of the preferred embodiment, shown in the first stage of the preferred manufacturing method.

[0016] FIG. 12 is a flowchart depicting a manufacturing method of a capacitive micromachined ultrasonic transducer in accordance with the preferred manufacturing method.

DESCRIPTION OF THE PREFERRED EMBODIMENT

[0017] The following description of the preferred embodiment of the invention is not intended to limit the invention to this preferred embodiment, but rather to enable any person skilled in the art of medical devices to make and use this invention.

[0018] The ultrasound system 10 of the preferred embodiment, as shown in FIG. 1, includes a central console 12 and a handheld probe 14 with an integrated circuit/transducer device. The handheld probe 14 is adapted to receive a wireless beam signal from the central console 12, generate an ultrasonic beam, detect an ultrasonic echo at multiple locations, combine the ultrasonic echoes into a single multiplexed echo signal, and transmit a multiplexed echo signal to the central console 12. The ultrasound system 10 provides an improved ultrasound system that collects enough echo data for 3D imaging and that transmits the echo data by a wireless link to overcome the limitations and drawbacks of typical ultrasound systems.

[0019] The ultrasound system 10 has been specifically designed to allow medical specialists to view the anatomy and pathologic conditions of a patient. The ultrasound system 10 may, however, be used to view any subject 16 that at least partially reflects ultrasound beams. Such non-medical uses may include ultrasonic microscopy, non-destructive testing, and other situations that would benefit from a volumetric imaging of the subject 16.

1. Central Console

[0020] The central console 12 of the preferred embodiment functions to: provide interaction with the operator of the ultrasound system 10; wirelessly communicate with the handheld probe 14; control the ultrasonic beams of the handheld probe 14; process the 3D images from the multiplexed echo signals of the handheld probe 14; and display a 3D image. The central console 12 may further provide other functions, such as providing data storage, data compression, image printouts, format conversions, communication links to a network, or any other appropriate function. To accomplish the five main functions, the central console 12 is conceptually separated into console controls 18, a beam controller 20, a console transmitter 22 and console receiver 24, an image processor 26, and a console display 28, as shown in FIG. 2. The central console 12 is preferably designed as a mobile unit (such as a wheeled cart or a laptop computer), but may alternatively be designed as a fixed unit (such as a cabinet structure).

[0021] The console controls 18 of the central console 12 provide interaction with the operator of the ultrasound system 10. The console controls 18 preferably allow the operator to configure the ultrasound system 10, to switch between imaging modes, and to capture frame/cine. The console controls 18 may alternatively provide other appropriate functions. Input from the operator is collected, parsed, and sent to the image processor 26 and/or the beam controller 20 as appropriate. The console controls 18 may include knobs, dials, switches, buttons, touch pads, fingertip sensors, sliders, joysticks, keys, or any other appropriate device to provide interaction with the operator.

[0022] The beam controller 20 of the central console 12 controls the ultrasonic beams of the handheld probe 14. The operator of the ultrasound system 10, through the console controls 18 described above, may select a particular imaging mode (e.g., 3D, 2D slice, or local image zoom) for a subject 16. To comply with this selection, the beam controller 20 preferably creates a beam signal that adjusts or modulates the frequency, sampling rate, filtering, phasing scheme, amplifier gains, transducer bias voltages, and/or multiplexer switching of the handheld probe 14. Alternatively, the beam controller 20 may create two or more signals that adjust or modulate these parameters. Further, the beam controller 20 may create a beam signal that adjusts or modulates other appropriate parameters of the handheld probe 14.

[0023] The console transmitter 22 and the console receiver 24 of the central console 12 function to provide a wireless communication link with the handheld probe 14. Specifically, the console transmitter 22 functions to transmit beam signals to the handheld probe 14, while the console receiver 24 functions to receive echo signals from the handheld probe 14. In the preferred embodiment, the console transmitter 22 and the console receiver 24 use radiofrequency (RF) communication and an appropriate protocol with a high data

throughput. In an alternative embodiment, however, the console transmitter 22 and the console receiver 24 may use infrared or other high-speed optical communication instead of, or in addition to, RF communication. The console transmitter 22 and the console receiver 24 may incorporate frequency hopping, spread-spectrum, dual-band, encryption, and/or other specialized transmission techniques known in the art to ensure data security and/or integrity in noisy environments. In the preferred embodiment, the console transmitter 22 and the console receiver 24 are located within different housings and are operated at different frequencies. In an alternative embodiment, the console transmitter 22 and the console receiver 24 may be combined (as a console transceiver) and/or may operate within the same channel or frequency.

[0024] The image processor 26 of the central console 12, which functions to construct 3D images from the multiplexed echo signals of the handheld probe 14, is preferably composed of a frame compiler 30 and an image engine 32. The frame compiler 30 of the image processor 26 functions to assemble a single 3D image (or 3D frame) from the multiplexed echo signals of the handheld probe 14. The echo signals, which are a series of pulses with specific time, amplitude, and phasing information, are correlated, summed, and transformed into voxels for the 3D image. Noise reduction, phase deaberration, contrast enhancement, orthogonal compounding, and other operations are also performed at this stage. In the preferred embodiment, as much as possible, these operations are performed in parallel fashion with dedicated algorithms, thus allowing the frame compiler 30 to be optimized for maximum speed. The frame compiler 30 preferably consists of a massively parallel set of lower-cost, medium-performance DSP cores, but may alternatively include other appropriate devices.

[0025] The image engine 32 of the image processor 26 receives complete frames from the frame compiler 30 and provides all higher-level processing (such as image segmentation) of the 3D frames. In the preferred embodiment, the image engine 32 also serves as a collection point for all echo data in the ultrasound system 10. The image engine 32 preferably consists of a high-performance, highly programmable DSP core, but may alternatively include other appropriate devices. In an alternative embodiment, the image processor 26 may include other appropriate devices to construct 3D images from the multiplexed echo signals of the handheld probe 14.

[0026] The console display 28 functions to present an image of the subject 16 to the operator in a form that facilitates easy and intuitive manipulation, navigation, measurement, and quantification. Examples of display modes include 3D, semi-transparent rendering, and 2D slices through the 3D structure. The console display 28 preferably includes a conventional LCD screen, but may alternatively include any appropriate device (such as a holographic or stereoscopic device) to present the scanned images.

2. Handheld Probe

[0027] The handheld probe 14 of the preferred embodiment functions to: wirelessly receive beam signals from the central console 12; generate an ultrasonic beam and detect an ultrasonic echo at multiple locations; combine the ultrasonic echoes into a single multiplexed echo signal; and wirelessly transmit the echo signals to the central console

12. The handheld probe 14 may further provide other functions, such as providing data storage, data compression, or any other appropriate function. To accomplish the four main functions, the central console 12 is conceptually separated into a probe receiver 34, a first integrated circuit/transducer device 36, a second integrated circuit 38, and a probe transmitter 40, as shown in FIG. 3.

[0028] The probe receiver 34 and the probe transmitter 40 of the handheld probe 14 function to provide a wireless communication link with the central console 12. Specifically, the probe receiver 34 functions to receive beam signals from the central console 12, while the probe transmitter 40 functions to transmit a multiplexed echo signal to the central console 12. The probe receiver 34 and the probe transmitter 40 use the same communication method and protocol as the console transmitter 22 and the console receiver 24. In the preferred embodiment, the probe receiver 34 and the probe transmitter 40 are located within different housings. In an alternative embodiment, the probe receiver 34 and the probe transmitter 40 may be combined (as a probe transceiver).

[0029] The first integrated circuit/transducer device 36 of the handheld probe 14 functions to generate an ultrasonic beam, detect an ultrasonic echo at multiple locations, and to combine the ultrasonic echoes into multiplexed echo signals. The first integrated circuit/transducer device 36 preferably accomplishes these functions with the use of a 2D array of transducer cells 42, a series of beam-signal leads 44 that are adapted to carry the beam signals to the transducer cells 42, and a series of echo-signal leads 46 that are adapted to carry the multiplexed echo signals from the transducer cells 42, as shown in FIG. 4. The first integrated circuit/transducer device 36 may alternatively accomplish these functions with other suitable devices.

[0030] Each transducer cell 42 of the first integrated circuit/transducer device 36, which functions as a 2D phased subarray to scan one sector of the entire viewing field, preferably includes at least one ultrasonic beam generator 48, at least four (and preferably fifteen or sixteen) ultrasonic echo detectors 50, and at least one first multiplexer 52. The ultrasonic beam generator 48 and the ultrasonic echo detectors 50 of the transducer cell 42 function to generate an ultrasonic beam and to detect an ultrasonic echo at multiple locations, respectively. Preferably, the ultrasonic beam generator 48 and the ultrasonic echo detectors 50 are separate elements, which simplifies the front-end electronics for the first integrated circuit/transducer device 36 and allows the ultrasonic beam generator 48 and the ultrasonic echo detectors 50 to be separately optimized for their individual function. For example, the ultrasonic beam generator 48 may be optimized for high output (with increased ruggedness), while the ultrasonic echo detector 50 may be optimized for high sensitivity. This separate optimization may reduce edge wave effects (since a single point source can be fired instead of a complete subaperture). Although separate elements, the ultrasonic beam generator 48 and the ultrasonic echo detector 50 preferably share a basic shape and construction and preferably differ only by the diaphragm diameter, thickness, tensile stress, gap spacing, control electronics, and/or electrode configuration. Alternatively, the ultrasonic beam generator 48 and the ultrasonic echo detectors 50 may be formed as the same component (i.e., dual-function transducers). If the first integrated circuit/transducer device 36 is operating at 3 MHz, the ultrasonic beam

generator 48 and the ultrasonic echo detectors 50 have a preferred diameter of 100-200 μm and a preferred pitch of approximately $250 \pm 50 \mu\text{m}$, as shown in FIG. 5. The ultrasonic beam generator 48 and the ultrasonic echo detectors 50 may, however, have any suitable diameter and pitch.

[0031] The first multiplexer 52 of the transducer cell 42 functions to combine the ultrasonic echoes from the ultrasonic echo detectors 50 into a multiplexed echo signal. To collect enough echo data for 3D imaging, the first integrated circuit/transducer device 36 preferably includes at least 4,096 ultrasonic echo detectors 50, more preferably includes at least 15,360 ultrasonic echo detectors 50, and most preferably includes at least 16,384 ultrasonic echo detectors 50. From a manufacturing standpoint, the number of echo-signal leads 46 between the first integrated circuit/transducer device 36 and the second integrated circuit 38 is preferably equal to or less than 1024 connections, and more preferably equal to or less than 512 connections. Thus, the first multiplexer 52 preferably combines the echo signals at least in a 4:1 ratio. The first multiplexer 52 may use time division multiplexing (TDM), quadrature multiplexing, frequency division multiplexing (FDM), or any other suitable multiplexing scheme. Further, the first multiplexer 52 may actually be two multiplexers (indicated in FIG. 4 as a first portion 54 and a second portion 56) combined that either use the same or different multiplexing schemes.

[0032] In a first example of the preferred embodiment, as shown in FIG. 4, the transducer cell 42 is square shaped and the first integrated circuit/transducer device 36 includes 1,024 transducer cells 42 (preferably arranged in a square pattern with thirty-two transducer cells 42 along one dimension and thirty-two transducer cells 42 along another dimension). Preferably, each transducer cell 42 includes: sixteen ultrasound echo detectors 50 (plus one ultrasound beam generator 48 and one first multiplexer 52) in a transducer cell, and 1,024 transducer cells 42 in the first integrated circuit/transducer device 36. This arrangement provides a manageable level of echo-signal leads 46 to the second integrated circuit 38 (1,024 echo-signal leads), while providing enough echo data (16,384 ultrasonic echo detectors 50) for 3D image rendering. The first multiplexer 52, in this arrangement, combines sixteen echo signals into one multiplexed echo signal using a 16:1 TDM device. In a variation of this example, the first multiplexer 52 combines only four echo signals into one multiplexed echo signal using a 4:1 TDM device. Since there are four multiplexed echo signals and only one echo-signal lead, the first integrated circuit of this example performs four passes, each pass with a new beam signal and each pass with only $\frac{1}{4}$ th of the ultrasonic echo detectors 50 contributing to the echo signal. In this manner, the first multiplexer 52 is only combining a portion of the echo signals into a multiplexed signal.

[0033] In a second example of the preferred embodiment, as shown in FIG. 6, the transducer cell 42 is roughly rectangular shaped and the first integrated circuit/transducer device 36 includes 1,024 transducer cells 42 (preferably arranged in a square pattern with thirty-two transducer cells 42 along one dimension and thirty-two transducer cells 42 along another dimension). Preferably, each roughly rectangular transducer cell 42 includes: one ultrasound beam generator 48 near the center, fifteen ultrasound echo detectors 50, and one first multiplexer (not shown). The ultrasound beam generators 48 are preferably arranged in a

regular hexagonal tessellation, but may alternatively be arranged in any suitable pattern. This arrangement provides a manageable level of echo-signal leads to the second integrated circuit (1,024 echo-signal leads), while providing enough echo data (15,360 ultrasonic echo detectors so) for 3D image rendering. The first multiplexer, in this arrangement, combines fifteen echo signals into one multiplexed echo signal using a 15:1 TDM device (potentially implemented as a 16:1 device, or as two 4:1 devices, with one repeated or null signal). In a variation of this second example, as shown in FIG. 7, the transducer cell 42 is roughly snowflake shaped. Preferably, each roughly snow-flaked shaped transducer cell 42 includes: one ultrasound beam generator 48 in the center, fifteen ultrasound echo detectors 50 (arranged as six "interior" ultrasound echo detectors 50 and nine "exterior" ultrasound echo detectors so), and one first multiplexer (not shown).

[0034] Since the first integrated circuit/transducer device 36 is preferably limited to electronics that are essential to getting signals on- and off-chip, the first integrated circuit/transducer device 36 is preferably manufactured by a standard low-cost CMOS process at an existing foundry (e.g. AMI Semiconductor, 1.5 μ m). The ultrasonic beam generator 48 and the ultrasonic echo detectors 50 are preferably microfabricated on the first integrated circuit/transducer device 36 as capacitive micro-machined ultrasonic transducers (cMUT), similar in structure and function to devices disclosed by U.S. Pat. No. 6,246,158 (which is incorporated in its entirety by this reference), but differing significantly in structural materials and manufacturing method as described in sections three and four below.

[0035] The second integrated circuit 38, as shown in FIG. 3, of the handheld probe 14 functions to receive and transmit the beam signals from the probe receiver 34 to the beam-signal leads 44 of the first integrated circuit/transducer device 36, and to receive and transmit the multiplexed echo signals from the echo-signal leads 46 to the probe transmitter 40. Preferably, the second integrated circuit 38 further conditions the multiplexed echo signals to facilitate wireless communication to the central console 12. The conditioning may include converting the analog echo signals to adequately sampled (e.g. above Nyquist) digital signals, amplifying the analog echo signals, compressing the digital echo signals, and performing an error-correction process on the echo signals. The conditioning may further include additional multiplexing of the multiplexed echo signals into one channel (or simply less channels). Any number of multiplexing schemes may be used, including time-division multiplexing, code-division multiplexing, frequency-division multiplexing, packet-based transmission, or any other suitable multiplexing scheme. The second integrated circuit 38 preferably uses conventional devices and manufacturing methods, but may alternatively use any suitable device and any suitable manufacturing method.

[0036] In the preferred embodiment, the handheld probe 14 further provides time gain compensation of the echo signals, which corrects for attenuation and allows objects at a greater depth to be clearly depicted with objects of lesser depth. This function may be integrated onto the first integrated circuit/transducer device 36, the second integrated circuit 38, or any other suitable locations within the handheld probe 14. In alternative embodiments, the problem of

attenuation may be solved with other suitable devices, either within the handheld probe 14, the central console 12, or any other suitable location.

[0037] In the preferred embodiment, the central console 12 transmits multiple beam signals as a single multiplexed beam signal. For this reason, the central console 12 preferably includes a multiplexer (not shown) and the handheld probe 14 includes a de-multiplexer (not shown). In alternative embodiments, the beam signals are sent using multiple channels or using another suitable scheme.

[0038] In the preferred embodiment, the handheld probe 14 further includes probe controls 58, which function to provide additional interaction with the operator of the ultrasound system 10. Like the console controls 18, the probe controls 58 preferably allow the operator to configure the ultrasound system 10, to switch between imaging modes, and to capture frame/cine. Because of the proximity to the subject 16, however, the probe controls 58 may further include additional features, such as flag image, add caption or notation, add voice notation, and take measurement from image. The probe controls 58 may alternatively provide other appropriate functions. Input from the operator is collected, wirelessly transmitted to the central console 12, and routed to the image processor 26 and/or the beam controller 20 as appropriate. The probe controls 58 may include knobs, dials, switches, buttons, touch pads, fingertip sensors, sliders, joysticks, keys, or any other appropriate device(s) to provide interaction with the operator. The handheld probe 14 with the probe controls 58 of the preferred embodiment satisfies the need to allow operation of an ultrasound system 10 during a patient examination without requiring physical proximity to the central console 12.

[0039] In the preferred embodiment, the handheld probe 14 further includes a probe display 60. In a first variation of the preferred embodiment, the console transmitter 22 and the probe receiver 34 are further adapted to communicate information about the system configuration (such as imaging modes). With this variation, the probe display 60 is preferably adapted to display the system configuration. In a second variation of the preferred embodiment, the console transmitter 22 and the probe receiver 34 are further adapted to communicate a processed image of the subject 16 (e.g., 3D, semi-transparent rendering, and 2D slices through the 3D structure). With this variation, the probe display 60 is preferably adapted to display the processed image. In a third variation, the console transmitter 22 and the probe receiver 34 are adapted to communicate both the information about the system configuration and the processed images. With this variation, the handheld probe 14 may include an additional probe display 60, or may include a switch between the two sources. The probe display 60 preferably includes a conventional LCD screen, but may alternatively include any appropriate device such as individual lights, digital displays, alphanumeric displays, or other suitable indicators. With the probe controls 58 and the probe display 60, the handheld probe 14 of the preferred embodiment further exceeds the need to allow operation of an ultrasound system 10 during a patient examination without requiring physical proximity to the central console 12.

[0040] In the preferred embodiment, the handheld probe 14 further includes a power source 62, which functions to power the components of the handheld probe 14. The power

source 62 is preferably a conventional rechargeable battery, but may alternatively be a capacitor, a fuel cell, or any other suitable power source 62. Considering the state of battery technology, however, it is possible that the addition of a power source 62 would make the handheld probe 14 unacceptably heavy or bulky. Thus, in a variation of the preferred embodiment shown in FIG. 8, the power source 62 is located in a remote portion 64 of the handheld probe 14, which is connected to the handheld probe 14 with a lightweight cord 66. The remote portion 64 may be designed to be strapped to the operator's body (e.g., wrist, arm, or shoulder) or clipped to the operator's belt, with the cable routed such that it is kept conveniently out of the way (e.g., along the arm). Although this variation still requires a cable connected to the handheld probe 14, the cable moves with the operator and thus provides a degree of freedom that is still greater than a transducer head tethered to the central console. Further, in the variation of the preferred embodiment, other elements of the handheld probe 14 may be located in the remote portion 64. For example, the probe receiver, the probe transmitter, the probe controls, and/or the probe display may be located in the remote portion 64 of the handheld probe 14.

3. Structure of the First Integrated Circuit/Transducer Device

[0041] As shown in FIGS. 9 and 10, the first integrated circuit/transducer device 36 of the handheld probe includes both CMOS circuits 110 and cMUT elements 112. The cMUT elements 112 function to generate an ultrasonic beam, detect an ultrasonic echo, and output electrical signals, while the CMOS circuits 110 function to perform analog or digital operations on the electrical signals generated through operation of the cMUT elements 112. The first integrated circuit/transducer device 36 may be configured in any suitable size and shape, and may include any suitable number of CMOS circuits 110 and cMUT elements 112. Both the CMOS circuits 110 and cMUT elements 112 are preferably fabricated on a suitable substrate 113.

[0042] The CMOS circuits 110 function to perform analog or digital operations, such as multiplexing or amplification, on the electrical signals generated through operation of the cMUT elements 112. The CMOS circuits 110 preferably include any suitable number of p-type, n-type, and insulating dielectric layers, arranged into active and/or passivation layers, as well as electrical leads for receiving input signals, receiving electrical power, and transmitting output signals. The CMOS circuits 110 may, however, include any suitable layer, element, or object in a conventional complementary-metal-oxide-semiconductor process.

[0043] The cMUT elements 112 function to generate an ultrasonic beam, detect an ultrasonic echo, and output electrical signals. The cMUT elements 112 include at least one dielectric layer 114, lower electrode 116, an upper electrode 118, and a cavity 120.

[0044] The dielectric layer 114 of the preferred embodiment functions to electrically and chemically isolate the lower electrode 116 and the upper electrode 118, and is accordingly preferably located between the lower electrode 116 and the upper electrode 118. The dielectric layer 114 preferably includes silicon dioxide or silicon nitride, but may alternatively include other suitable dielectric material usable in forming CMOS or MOS structures. The thickness

of the dielectric layer can range between 0.5 microns and 1.5 microns, depending upon the functionality desired for the cMUT element 112.

[0045] The lower electrode 116 of the preferred embodiment functions to maintain a first electrical potential. To maintain a first electrical potential, the lower electrode is preferably connected to a power source that provides the necessary voltage. The lower electrode 116 preferably forms a layer within the CMOS circuits 110, and as such can function as a transistor gate, capacitor plate, metallization, or other layer. The lower electrode 116 further functions to provide one portion of a capacitor within the structure of the cMUT elements 112. The lower electrode 116 may be composed of any suitable material, including both metals and semiconductors, that is capable of maintaining a predetermined voltage level. In one variation, as shown in FIG. 9, the lower electrode 116 is doped polysilicon. In another variation, the lower electrode 116 is a metal. In both variations, the lower electrode 116 is preferably deposited by conventional methods, but may be deposited by any other suitable method.

[0046] The upper electrode 118 of the preferred embodiment functions to maintain a second electrical potential. To maintain a second electrical potential, the upper electrode 118 may be connected to a power source that provides the necessary voltage. The upper electrode 118 preferably forms a layer within the CMOS circuits 110, and as such can function as a transistor gate, capacitor plate, metallization, or other layer. The upper electrode 118 further functions to provide one portion of a capacitor within the structure of the cMUT elements 112. The upper electrode 118 may be composed of any suitable material, including both metals and semiconductors, that is capable of maintaining a predetermined voltage level. The upper electrode 118 is preferably deposited by conventional methods, but may be deposited by any other suitable method.

[0047] The cavity 120 of the preferred embodiment, which is formed between the lower electrode 116 and the upper electrode 118, functions to facilitate relative displacement of the lower electrode 116 and the upper electrode 118, which thereby allow the cMUT elements 112 to receive and transmit acoustic waves, preferably at ultrasonic frequencies. The cavity 120 further functions to provide an air or vacuum gap capacitor formed by its position relative to the lower electrode 116 and the upper electrode 118. As acoustic waves are directed towards the cavity 120, the transmission of those waves will cause relative displacement of the upper electrode 118 and the lower electrode 116, which in turn will cause a change in the capacitance between the upper electrode 118 and the lower electrode 116. The cavity 120 may be of any suitable dimension for use in the acoustic detection arts, depending upon the application and the frequencies of the transmitted and received waves. The cavity 120 preferably has a depth of 0.1 microns to 1.5 microns and lateral dimensions of 10 microns to 1 millimeter, depending upon the application for which the first integrated circuit/transducer device 36 is designed.

[0048] The first integrated circuit/transducer 36 of the preferred embodiment also includes a sealant layer 122 disposed on the cMUT elements 112. The sealant layer 122 functions to prevent fluid, air, or debris from entering the cavity 120 and impeding relative displacement of the lower

electrode **116** and the upper electrode **118** during acoustic transmission or reception. The sealant layer **122** may be any suitable material used in the art of semiconductor manufacturing and micromachining, including for example silicon dioxide, silicon nitride, or a mixture of the two (referred to as "oxynitride"). The sealant layer **122** may alternatively be a vacuum-deposited polymer such as parylene, or it may be a thin flexible membrane material applied as a sheet adhered to the dielectric layer **114** by chemical or thermal activation. The sealant layer **122** is preferably impermeable to air and water or similar fluids. The sealant layer **122** is also preferably mechanically flexible so as to minimally impede displacement of the relative displacement of the lower electrode **116** and the upper electrode **118** during acoustic transmission or reception.

4. Method of Manufacturing the First Integrated Circuit/Transducer Device

[0049] The mechanical structure of the first integrated circuit/transducer device **36** is preferably formed by layers deposited and patterned as part the foundry CMOS process itself (and preferably not augmented with additional steps for depositing material and aligning/patterning layers). The steps performed on the first integrated circuit/transducer device **36** after the foundry fabrication preferably include only blanket etch and deposition steps, which require no alignment procedure or only rough alignment (with tolerances greater than 400 μm).

[0050] As described above, the first integrated circuit/transducer device **36** consists of a lower electrode, a dielectric layer, and an upper electrode, with all layers integral to the CMOS process flow. In summary, a capacitive gap with a thickness of 0.1 microns to 1.5 microns is preferably formed by selectively etching a sacrificial metal layer (also integral to the CMOS process) that has been patterned to be exposed when the chip is immersed in a metal etch solution after completion of the foundry CMOS process. A vacuum-sealed cavity is preferably formed between the membrane and the lower electrode by sealing access ports to the gap using a low-temperature blanket dielectric deposition under vacuum (by PECVD and/or sputtering). More details of the process appear below.

[0051] As shown in FIGS. **11** and **12**, the manufacturing method for the first integrated circuit/transducer device **36** of the preferred embodiment includes the steps of depositing the lower electrode **S102**; depositing a sacrificial layer **S104**; depositing a dielectric layer **S106**; depositing the upper electrode **S108**; depositing a protective layer on the upper electrode **S110**; and removing the sacrificial layer **S112**. In the preferred embodiment, the manufacturing method also includes the step of depositing a sealant layer to seal a cavity between the lower electrode and the upper electrode **S114**.

[0052] Step **S104** of the preferred method recites depositing a sacrificial layer. The sacrificial layer, which is deposited over the lower electrode, is removed at a later step in the preferred method. The sacrificial layer functions to create a volume of space between the lower electrode and the upper electrode, which is subsequently evacuated to form the cavity. The sacrificial layer may be deposited directly on the lower electrode, or may be deposited on the dielectric layer, which is deposited directly on the lower electrode. As described above, the cavity may be of any suitable dimension for use in the acoustic detection arts, depending upon

the application and the frequencies of the transmitted and received waves. Accordingly, the sacrificial layer deposited over the lower electrode preferably has a thickness that is substantially identical to the depth sought for the cavity, such as a thickness of approximately 0.1 microns to approximately 1.5 microns. The sacrificial layer may be any suitable material that is distinct from the dielectric layer, such that the sacrificial layer—and not the dielectric material—is removed during the process of removing the sacrificial layer.

[0053] Step **S110** of the preferred method recites depositing a protective layer over the upper electrode. The protective layer preferably includes any suitable material that is electrically distinct from the upper electrode, including both dielectric materials and sealant layers. The protective layer functions to electrically isolate the upper electrode and to protect the upper electrode from unwanted debris and environmental interference with the operation of the cMUT device.

[0054] Step **S112** of the preferred method recites removing the sacrificial layer. As noted above, step **S112** is preferably performed subsequent to steps **S102** through **S110**. Removal of the sacrificial layer results in the formation of the cavity, with an air or vacuum gap, between the upper electrode and the lower electrode. The removal of the sacrificial layer is preferably accomplished with any known or suitable process for removing materials used in semiconductor manufacturing. The selected removing mechanism depends largely upon the type of sacrificial material used, and can be readily selected by those skilled in the art of semiconductor manufacturing. For example, if the sacrificial material is aluminum, then the step of removing the sacrificial layer can include etching in a phosphoric/nitric/acetic acid solution such as Aluminum Etch A, from Transene, Inc.

[0055] In an alternative embodiment, Steps **S104** and **S112** may be altered to use other suitable materials. For example, Steps **S104** may include depositing a polysilicon layer (also integral to the CMOS process flow) as the sacrificial layer. Access ports to the polysilicon layer are preferably opened by immersing the chip in a metal etch solution to expose metal-polysilicon contact holes. The polysilicon sacrificial layer is preferably etched with a wet or dry isotropic etchant such as xenon difluoride gas using an apparatus such as that described in U.S. Pat. No. 6,887,337, which is hereby incorporated in its entirety by this reference. A vacuum-sealed cavity is then formed between the membrane and the lower electrode by sealing access ports to the gap using a low-temperature blanket dielectric deposition under vacuum (by PECVD, sputtering, parylene deposition, or any other suitable method).

[0056] In addition to the foregoing steps, a variation of the preferred method includes the additional step of thinning the sealant layer. The step of thinning the sealant layer functions to reduce the overall vertical dimension of the cMUT device. Additionally, a thinned sealant layer might possibly increase the bandwidth of the device while lowering the resonant frequency and operating voltage of the device. The step of thinning the sealant layer can include any known or suitable process for removing and/or etching materials used in semiconductor manufacturing. The selected thinning mechanism depends largely upon the type of sealant layer used, and can be readily selected by those skilled in the art of semiconductor manufacturing. For example, if the sealant layer is

silicon oxynitride, then the step of thinning the sealant layer can include exposing the sealant layer to a reactive ion etching (RIE) process

[0057] As a person skilled in the art of ultrasound systems will recognize from the previous detailed description and from the figures and claims, modifications and changes can be made to the preferred embodiment of the invention without departing from the scope of this invention defined in the following claims.

We claim:

1. An integrated circuit/transducer device, comprising:
 - a substrate;
 - a complementary-metal-oxide-semiconductor (CMOS) circuit fabricated on the substrate; and
 - a capacitive micromachined ultrasonic transducer (cMUT) element fabricated on the substrate and connected to the CMOS circuit, wherein the cMUT element includes a lower electrode adapted to maintain a first electrical potential, an upper electrode adapted to maintain a second electrical potential, and a cavity the lower electrode and the upper electrode.
2. The device of claim 1, further comprising at least 256 transducer cells, wherein each transducer cell is adapted to receive a beam signal, generate an ultrasonic beam, detect an ultrasonic echo at multiple locations, and combine the ultrasonic echoes into a single multiplexed echo signal, wherein each transducer cell includes at least one cMUT element adapted to generate ultrasonic beams and at least four cMUT elements adapted to detect ultrasonic echoes.
3. The device of claim 2, wherein the cMUT element adapted to generate ultrasonic beams and the cMUT elements adapted to detect ultrasonic echoes differ by at least one characteristic from a group consisting of diaphragm diameter, thickness, tensile stress, gap spacing, control electronics, and electrode configuration.
4. The device of claim 2, wherein the cMUT elements adapted to generate ultrasonic beams are arranged in a substantially regular hexagonal tessellation.

5. The device of claim 4, wherein each cMUT element adapted to generate an ultrasonic beam is arranged in the center of the transducer cell.

6. The device of claim 1 wherein the lower electrode is metal.

7. The device of claim 1 wherein the lower electrode is polysilicon.

8. The device of claim 1, wherein the upper electrode is disposed within the dielectric layer.

9. The device of claim 8, wherein the upper electrode is disposed on the dielectric layer and adjacent the cavity.

10. The device of claim 1 further comprising a sealant layer disposed on the dielectric layer.

11. The device of claim 10 wherein the sealant layer seals the cavity.

12. The device of claim 10 wherein the sealant is oxynitride.

13. A method of producing an integrated circuit/transducer device, the method comprising the steps of:

providing a substrate;

fabricating a complementary-metal-oxide-semiconductor (CMOS) circuit on the substrate;

fabricating a capacitive micromachined ultrasonic transducer (cMUT) element on the substrate and connecting the cMUT element to the CMOS circuit, wherein the cMUT element includes the following components that consist of layers corresponding to layers within the CMOS circuit: a lower electrode, an upper electrode, and a sacrificial layer located between the lower electrode and the upper electrode;

removing the sacrificial layer thereby defining a cavity between the lower electrode and the upper electrode; and

depositing a sealant layer thereby sealing the cavity.

14. The method of claim 13, further comprising thinning the sealant layer.

* * * * *

专利名称(译)	电容微机械超声换能器		
公开(公告)号	US20070167811A1	公开(公告)日	2007-07-19
申请号	US11/612656	申请日	2006-12-19
[标]申请(专利权)人(译)	LEMMERHIRT DAVID F RICH COLLIN A		
申请(专利权)人(译)	LEMMERHIRT DAVID F RICH COLLIN A		
当前申请(专利权)人(译)	SONETICS超声波, INC.		
[标]发明人	LEMMERHIRT DAVID F RICH COLLIN A		
发明人	LEMMERHIRT, DAVID F. RICH, COLLIN A.		
IPC分类号	A61B8/14		
CPC分类号	A61B8/00 B06B1/0292 A61B8/4472		
优先权	60/610337 2004-09-15 US 60/610319 2004-09-15 US 60/610320 2004-09-15 US		
其他公开文献	US8309428		
外部链接	Espacenet USPTO		

摘要(译)

手持式探头的第一集成电路/换能器设备36包括CMOS电路110和cMUT元件112。cMUT元件112用于产生超声波束，检测超声回波，并输出电信号，而CMOS电路110用于执行对通过cMUT元件112的操作产生的电信号进行模拟或数字操作。优选实施例的第一集成电路/换能器装置36的制造方法包括沉积下电极S102的步骤；沉积牺牲层S104；沉积介电层S106；沉积上电极S108；在上电极S110上沉积保护层；并去除牺牲层S112。在优选实施例中，制造方法还包括沉积密封剂层以密封下电极和上电极S114之间的空腔的步骤。

